


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040725\
Data File : BM049832.D
Acq On : 07 Apr 2025 10:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 14:55:34 2025

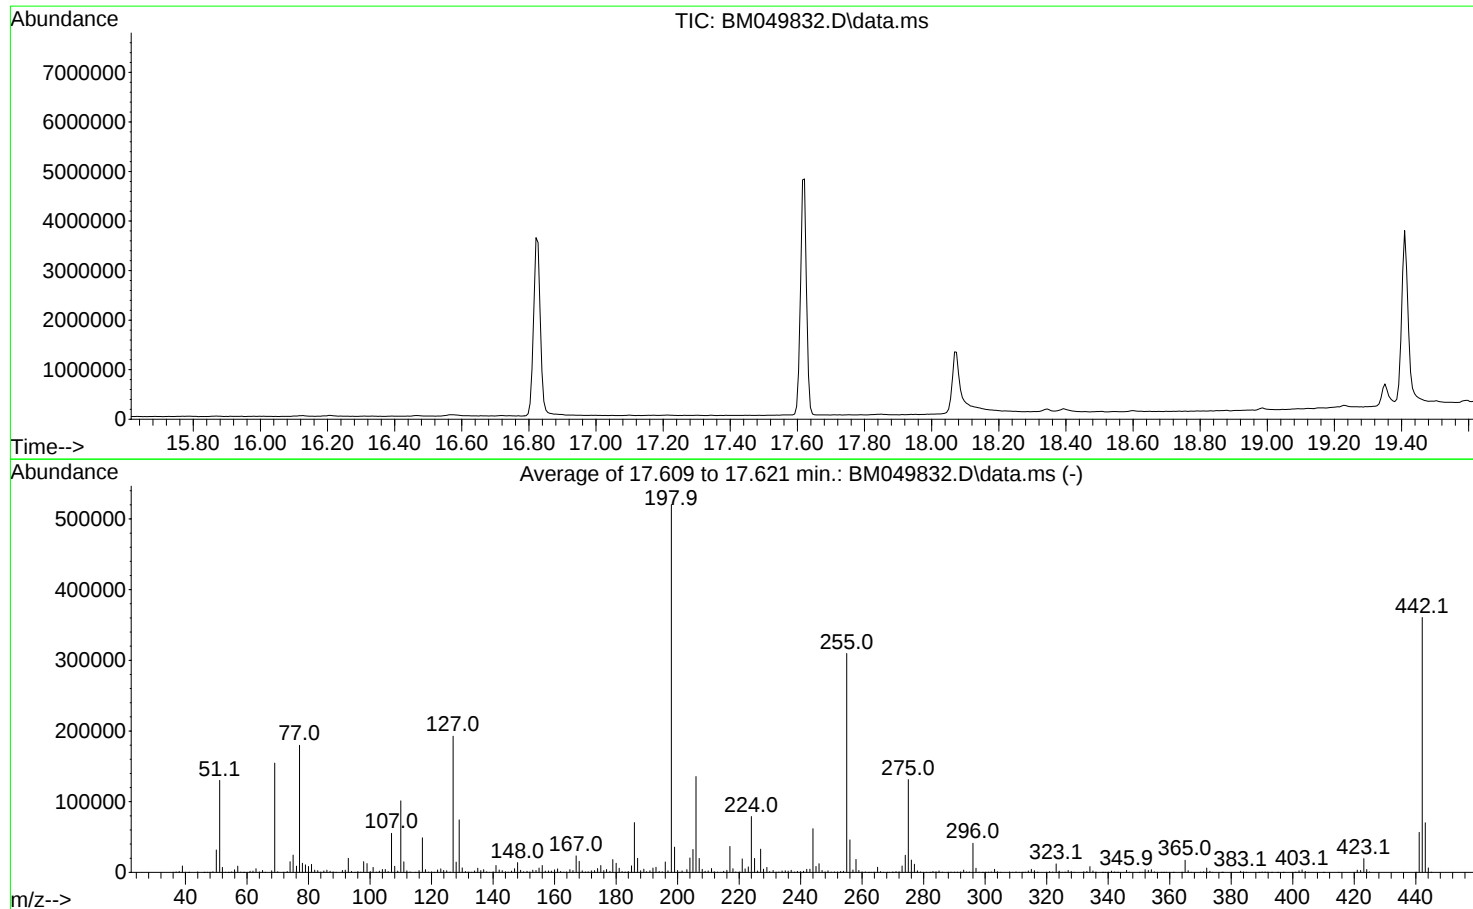

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	130102	PASS
68	69	0.00	2	1.4	2212	PASS
69	198	0.00	100	29.7	154617	PASS
70	69	0.00	2	0.5	813	PASS
127	198	10	80	37.0	192677	PASS
197	198	0.00	2	0.4	2189	PASS
198	198	100	100	100.0	520448	PASS
199	198	5	9	6.9	35763	PASS
275	198	10	60	25.2	131323	PASS
365	198	1	100	3.3	17327	PASS
441	198	0.01	100	10.9	56533	PASS
442	442	50	100	100.0	360597	PASS
443	442	15	24	19.5	70301	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/7/2025	BNA_M	<u>BM049832.D</u>
Compound Name	Response	Retention Time
DDT	1617502	20.65
DDD	42454	20.209
DDE	1581	19.703
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44035	1661537	2.65

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040725\
Data File : BM049832.D
Acq On : 07 Apr 2025 10:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 07 11:52:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

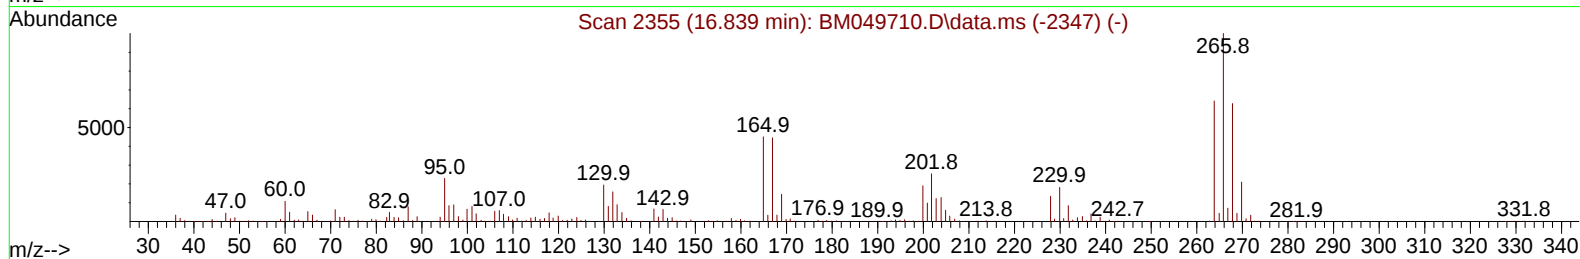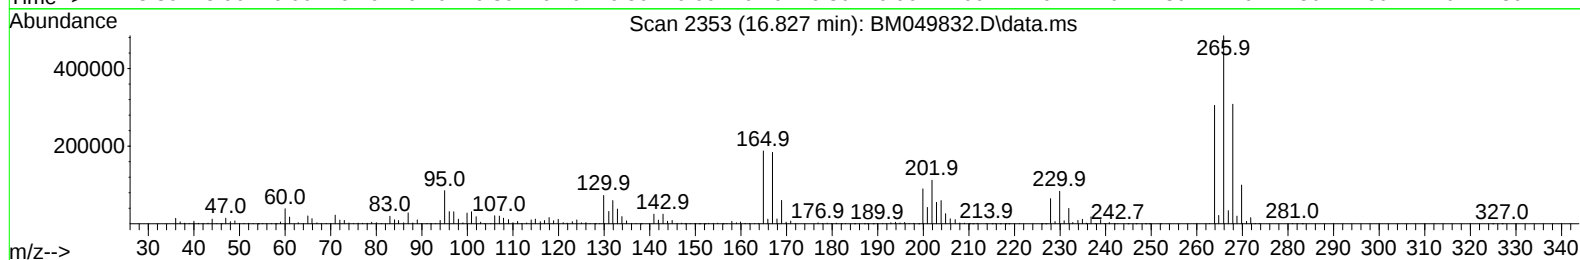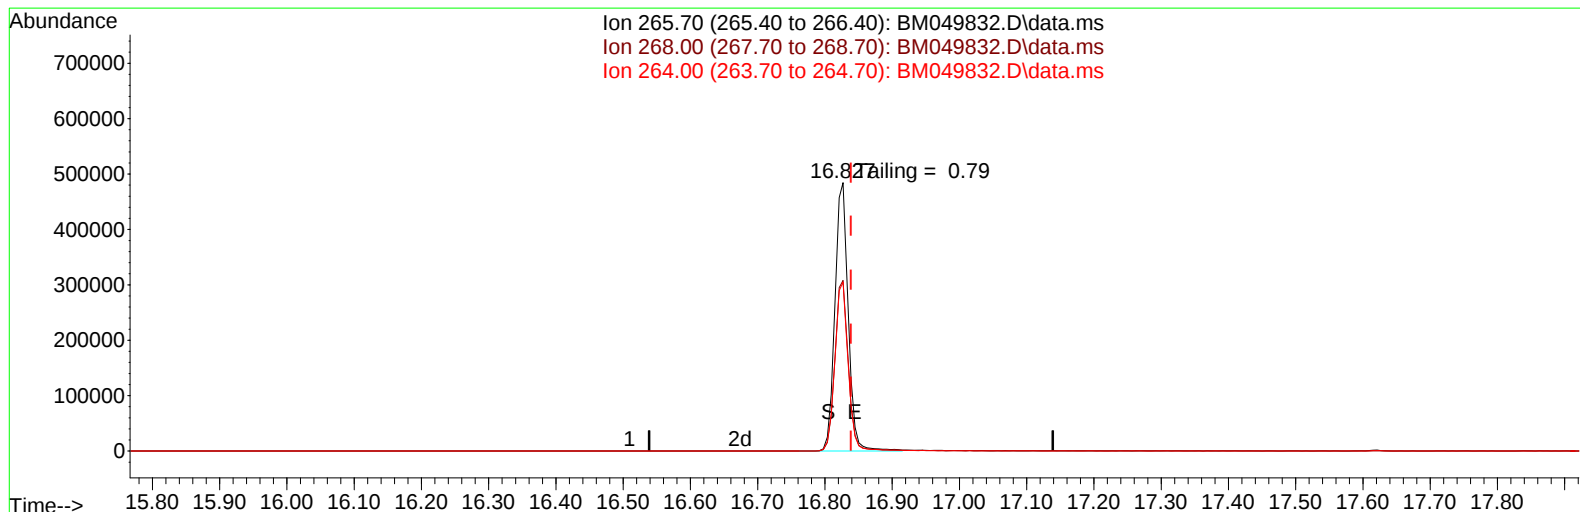

TIC: BM049832.D\data.ms

(70) Pentachlorophenol (C)




16.827min (-0.012) 198903.16 ng m

response 666998

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.57
264.00	64.10	62.98
0.00	0.00	0.00

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 07 11:52:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

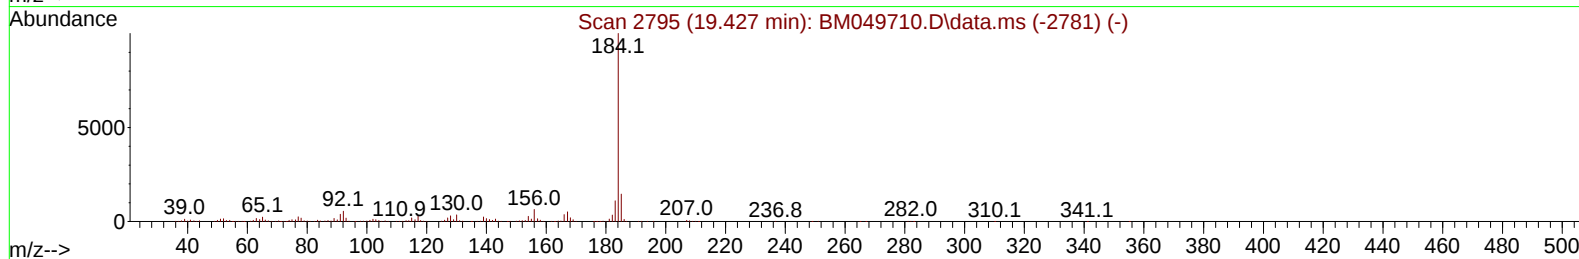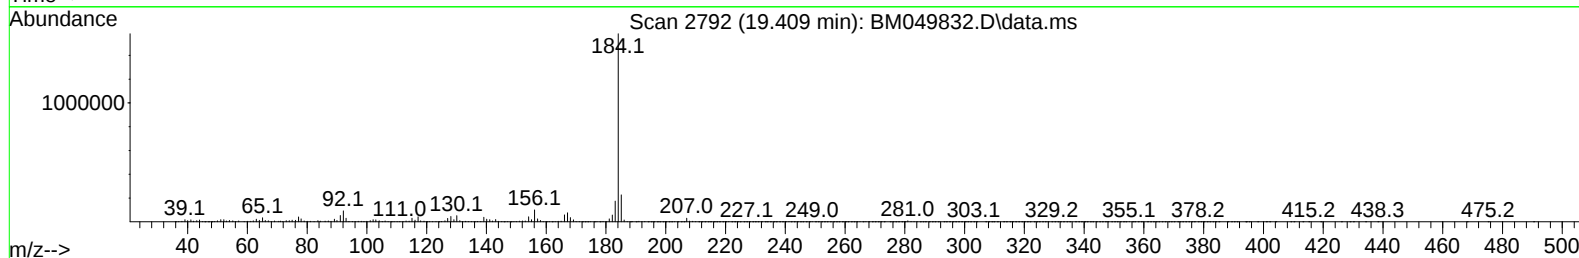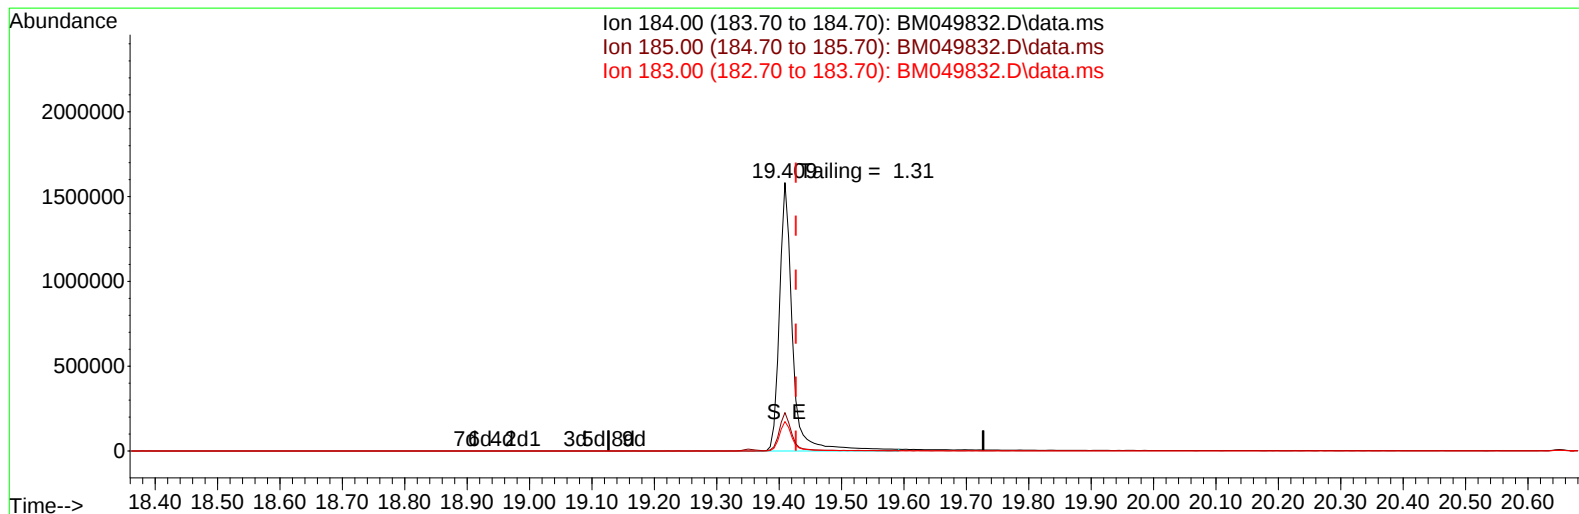

TIC: BM049832.D\data.ms

(77) Benzidine

19.409min (-0.018) 1046979.26 ng m

response **2352162**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.32
183.00	11.00	10.99
0.00	0.00	0.00