


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040325\
Data File : BM049799.D
Acq On : 03 Apr 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 14:55:34 2025

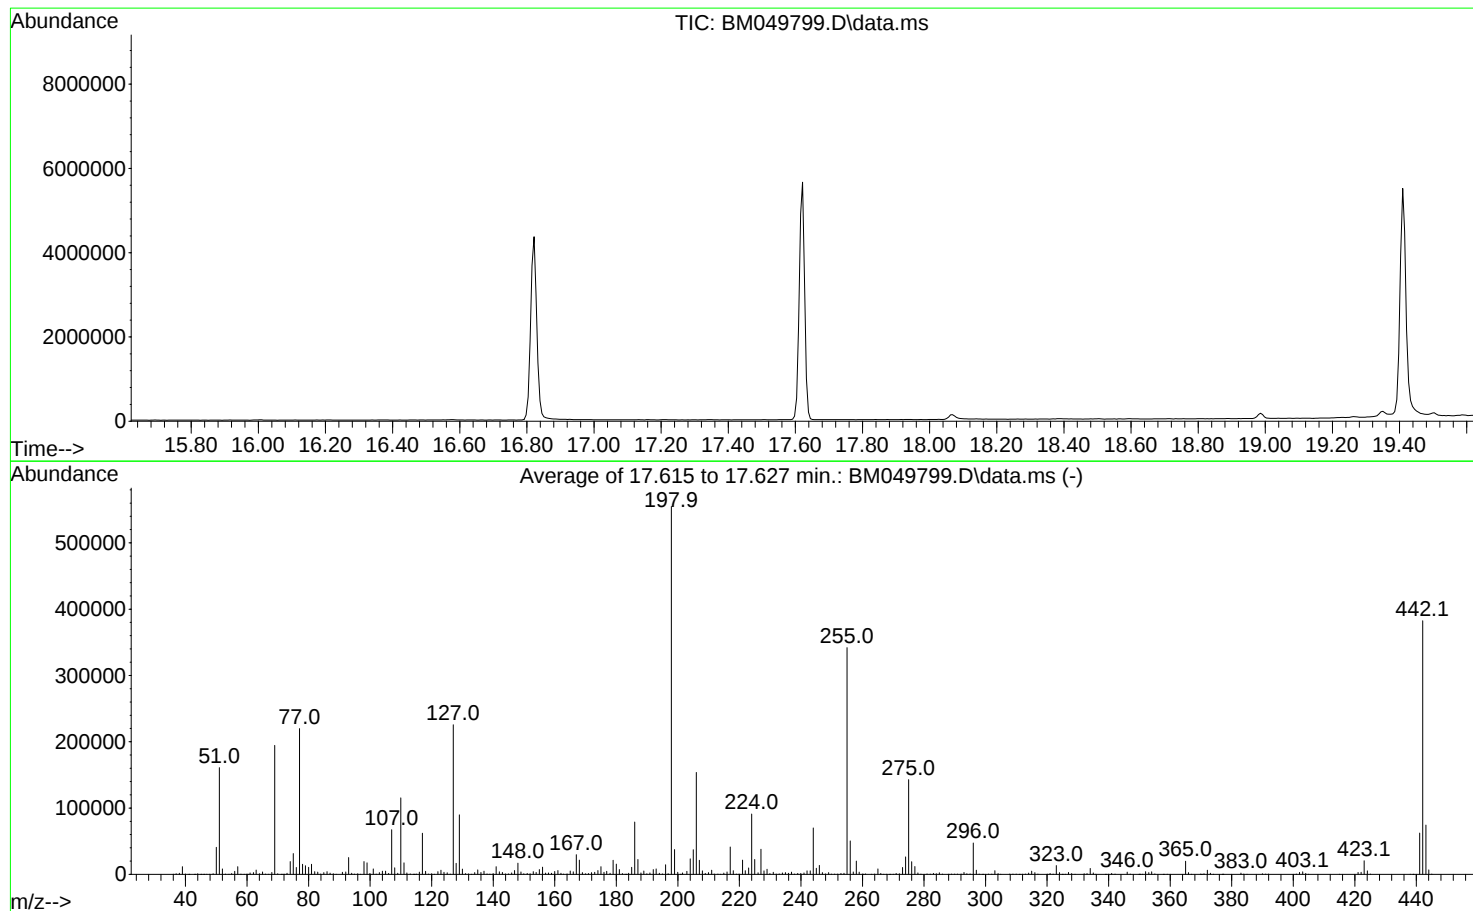

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	160892	PASS
68	69	0.00	2	1.5	2851	PASS
69	198	0.00	100	35.1	194648	PASS
70	69	0.00	2	0.5	1037	PASS
127	198	10	80	40.7	225728	PASS
197	198	0.00	2	0.1	825	PASS
198	198	100	100	100.0	554837	PASS
199	198	5	9	6.7	37451	PASS
275	198	10	60	25.7	142861	PASS
365	198	1	100	3.6	19811	PASS
441	198	0.01	100	11.2	62291	PASS
442	442	50	100	100.0	382421	PASS
443	442	15	24	19.4	74349	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/3/2025	BNA_M	<u>BM049799.D</u>
Compound Name	Response	Retention Time
DDT	1824130	20.65
DDD	16326	20.262
DDE	358	19.709
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16684	1840814	0.91

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040325\
Data File : BM049799.D
Acq On : 03 Apr 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 03 11:39:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

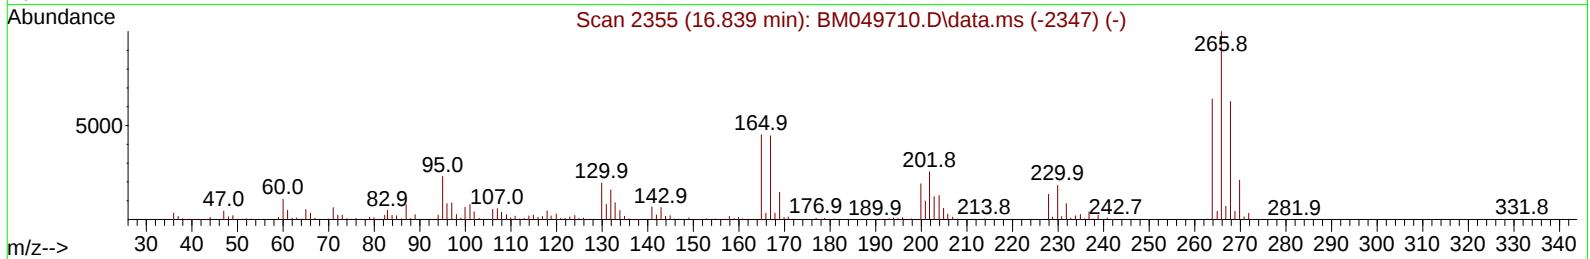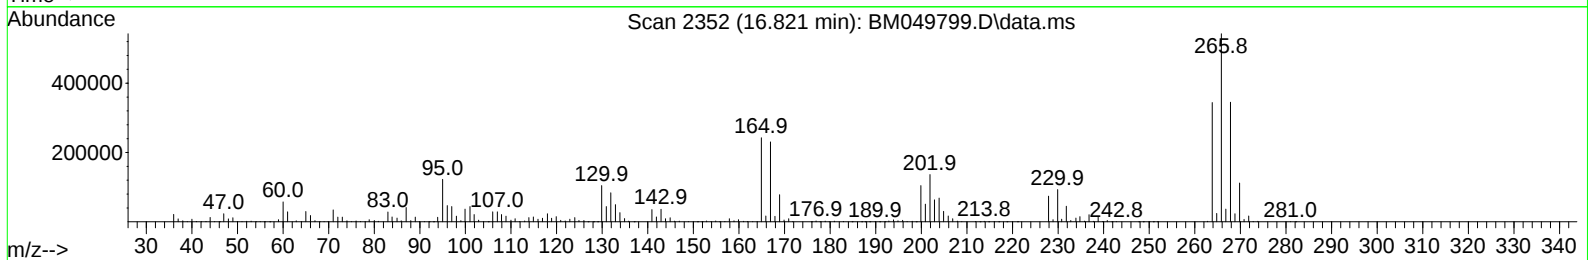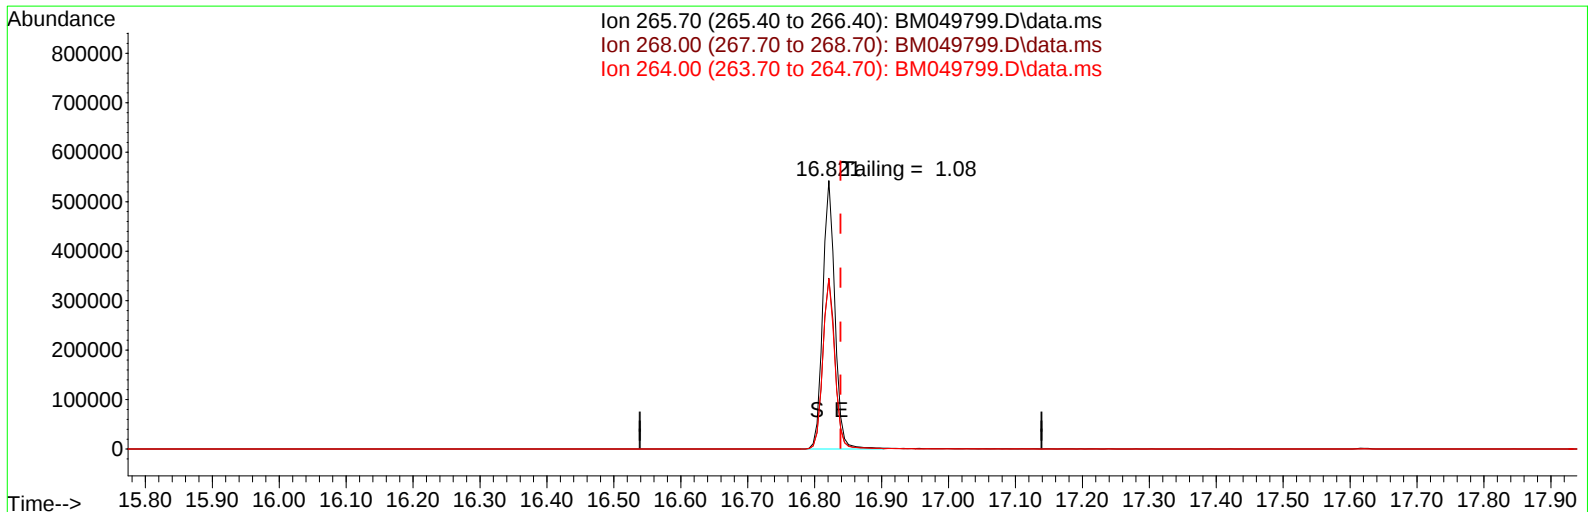

TIC: BM049799.D\data.ms

(70) Pentachlorophenol (C)

16.821min (-0.018) 57528.84 ng




response 685298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.60
264.00	64.10	63.40
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040325\  
Data File : BM049799.D  
Acq On    : 03 Apr 2025  10:38  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 03 11:39:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

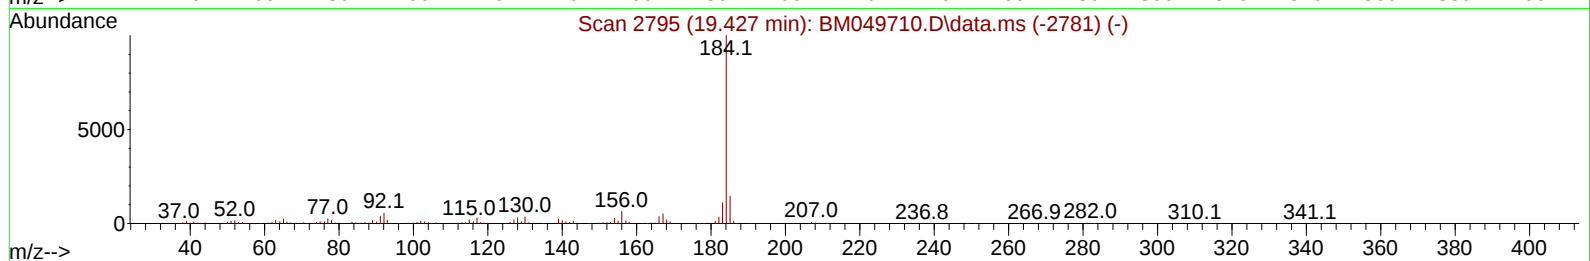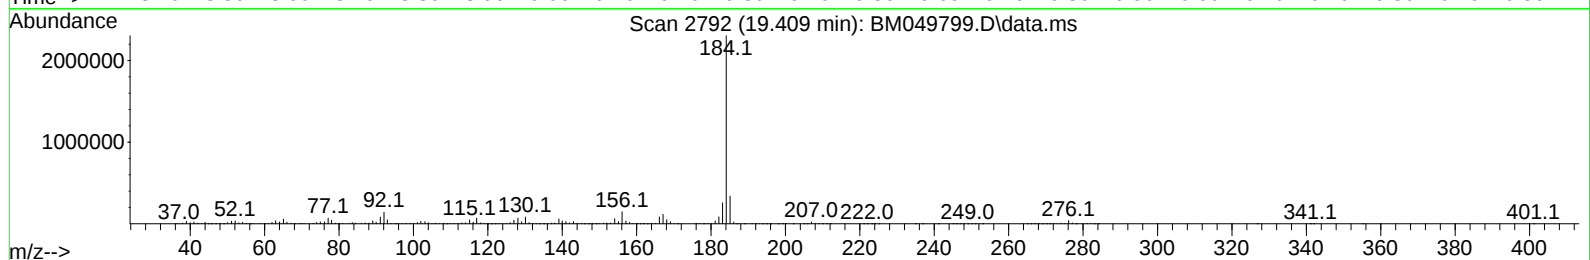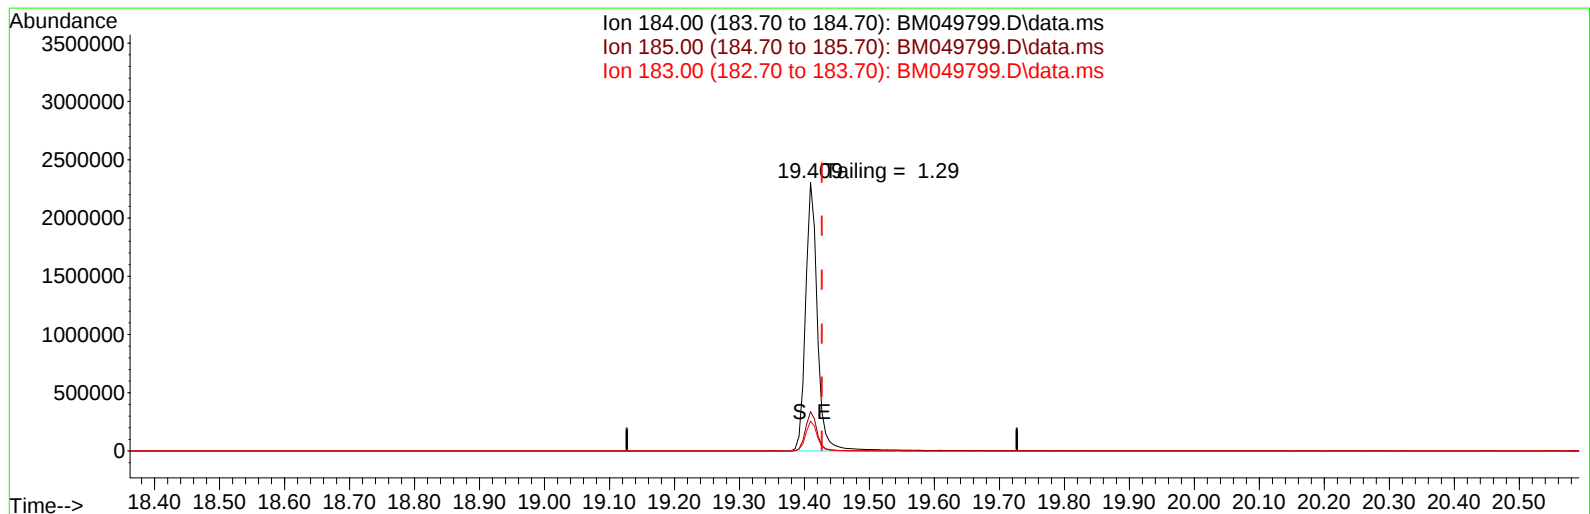

TIC: BM049799.D\data.ms

(77) Benzidine

19.409min (-0.018) 112742.95 ng

response 2947378

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.70
183.00	11.00	11.18
0.00	0.00	0.00