


Ident	Instrument IC-1				Analyst: NF		Method: 300.0 / 9056A		Initial Analyst		
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4				
STD1	0	0	0	0	0	0	0	0	IC1-032125	3/21/2025 10:45	10 NF/IZ
STD2	0.421	0.619	0.631	2.075	0.523	1.052	3.247	IC1-032125	3/21/2025 11:07	10 NF/IZ	
STD3	0.795	1.199	1.203	3.994	1.001	1.993	5.998	IC1-032125	3/21/2025 11:28	10 NF/IZ	
STD4	0.977	1.475	1.468	4.904	1.226	2.407	7.216	IC1-032125	3/21/2025 11:50	10 NF/IZ	
STD5	1.993	3.009	2.995	10.03	2.493	4.968	14.842	IC1-032125	3/21/2025 12:11	10 NF/IZ	
STD6	4.034	5.988	5.986	19.975	5.011	10.256	30.502	IC1-032125	3/21/2025 12:32	10 NF/IZ	
STD7	4.979	7.51	7.517	25.022	6.247	12.323	36.695	IC1-032125	3/21/2025 12:54	10 NF/IZ	
ICV	2.031	3.038	3.08	10.364	2.568	5.199	15.269	IC1-032125	3/21/2025 13:37	10 NF/IZ	
ICB	0	0.122	0.08	0	0	0	0	IC1-032125	3/21/2025 13:58	10 NF/IZ	
CCV	2.034	3.119	3.093	10.383	2.559	5.188	15.179	IC1-032125	4/3/2025 9:38	10 NF/IZ	
CCB	0	0	0	0	0	0	0	IC1-032125	4/3/2025 9:59	10 NF/IZ	
LB135296BSW	2.028	3.121	3.103	10.387	2.561	5.226	15.185	IC1-032125	4/3/2025 10:43	10 NF/IZ	
LB135296BLW	0	0	0	0	0	0	0	IC1-032125	4/3/2025 11:04	10 NF/IZ	
Q1711-01	0.332	26.59	0	0.215	0	2.108	10.666	IC1-032125	4/3/2025 12:29	10 NF/IZ	
Q1711-02MS	2.301	28.881	3.076	10.43	2.571	2.367	24.892	IC1-032125	4/3/2025 12:50	10 NF/IZ	
Q1711-03MSD	2.172	28.857	2.983	10.101	2.479	1.573	24.485	IC1-032125	4/3/2025 13:12	10 NF/IZ	
Q1711-04	0.275	20.1	0	0.221	0	0	4.529	IC1-032125	4/3/2025 13:55	10 NF/IZ	
Q1711-08	0	0.047	0	0	0	0	0	IC1-032125	4/3/2025 14:16	10 NF/IZ	
Q1716-01	0.433	427.687	0	0.63	0.296	0	54.697	IC1-032125	4/3/2025 14:38	10 NF/IZ	
Q1711-01DLX10	0.054	2.364	0	0	0	0	1.413	IC1-032125	4/3/2025 14:59	10 NF/IZ	
Q1711-04DLX5	0.071	3.687	0	0	0	0	1.238	IC1-032125	4/3/2025 15:21	10 NF/IZ	
CCV	2.072	3.107	3.112	10.418	2.589	5.237	15.386	IC1-032125	4/3/2025 15:43	10 NF/IZ	
CCB	0	0	0	0	0	0	0	IC1-032125	4/3/2025 17:16	10 NF/IZ	

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0	0	0	0	0	0	0	0 IC1-032125	3/21/2025 10:45	10	NF/IZ
STD2	0.421	0.619	0.631	2.075	0.523	1.052	3.247	IC1-032125	3/21/2025 11:07	10	NF/IZ
STD3	0.795	1.199	1.203	3.994	1.001	1.993	5.998	IC1-032125	3/21/2025 11:28	10	NF/IZ
STD4	0.977	1.475	1.468	4.904	1.226	2.407	7.216	IC1-032125	3/21/2025 11:50	10	NF/IZ
STD5	1.993	3.009	2.995	10.03	2.493	4.968	14.842	IC1-032125	3/21/2025 12:11	10	NF/IZ
STD6	4.034	5.988	5.986	19.975	5.011	10.256	30.502	IC1-032125	3/21/2025 12:32	10	NF/IZ
STD7	4.979	7.51	7.517	25.022	6.247	12.323	36.695	IC1-032125	3/21/2025 12:54	10	NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1											
STD2	5.2500	3.1667	5.1667	3.7500	4.6000	5.2000	8.2333				
STD3	-0.6250	-0.0833	0.2500	-0.1500	0.1000	-0.3500	-0.0333				
STD4	-2.3000	-1.6667	-2.1333	-1.9200	-1.9200	-3.7200	-3.7867				
STD5	-0.3500	0.3000	-0.1667	0.3000	-0.2800	-0.6400	-1.0533				
STD6	0.8500	-0.2000	-0.2333	-0.1250	0.2200	2.5600	1.6733				
STD7	-0.4200	0.1333	0.2267	0.0880	-0.0480	-1.4160	-0.8243				

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

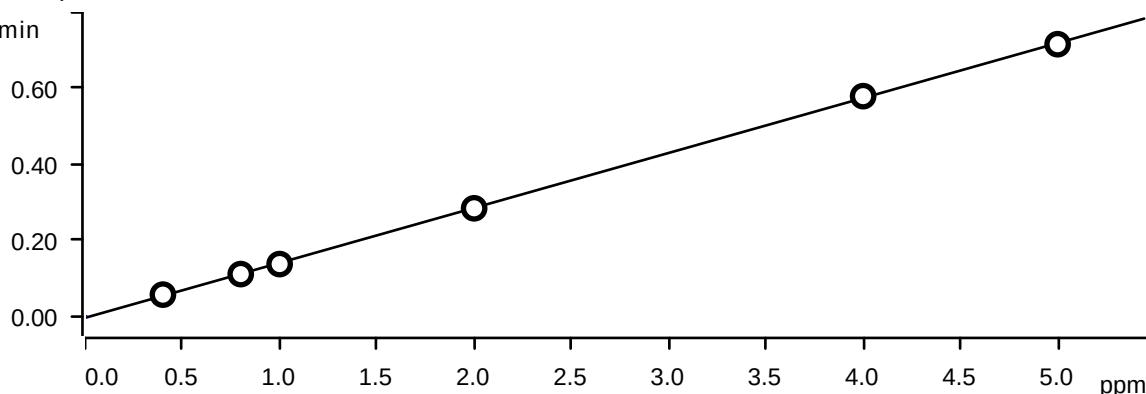

Function: $A = -4.00269E-3 + 0.0144679 \times Q$


Relative standard deviation: 1.180947 %

Correlation coefficient: 0.999926

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.137	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.284	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.580	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.716	STD7	2025-03-21 12:54:24 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

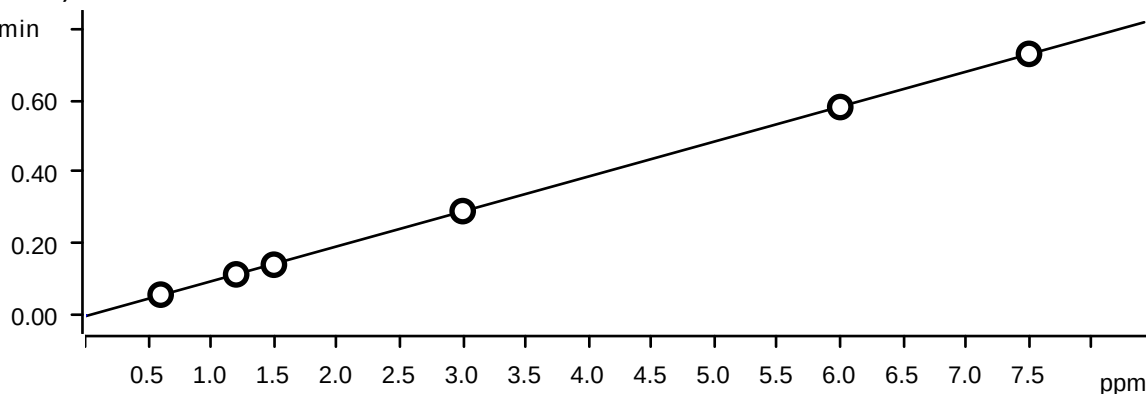

Function: $A = -2.25189E-3 + 9.74103E-3 \times Q$


Relative standard deviation 0.547466 %

Correlation coefficient 0.999984

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.058	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.115	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.291	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.581	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.729	STD7	2025-03-21 12:54:24 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

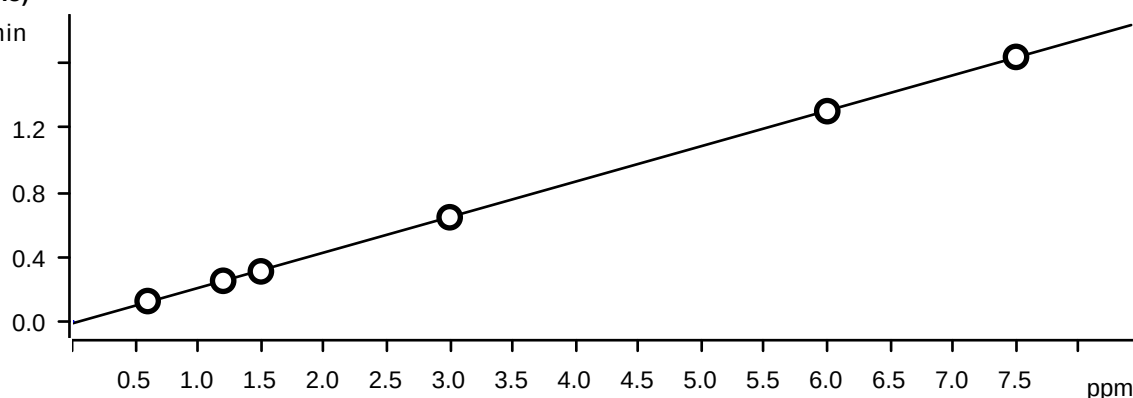Function: $A = -0.0127504 + 0.0219707 \times Q$


Relative standard deviation 0.767970 %

Correlation coefficient 0.999969

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.252	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.310	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.645	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.302	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.639	STD7	2025-03-21 12:54:24 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

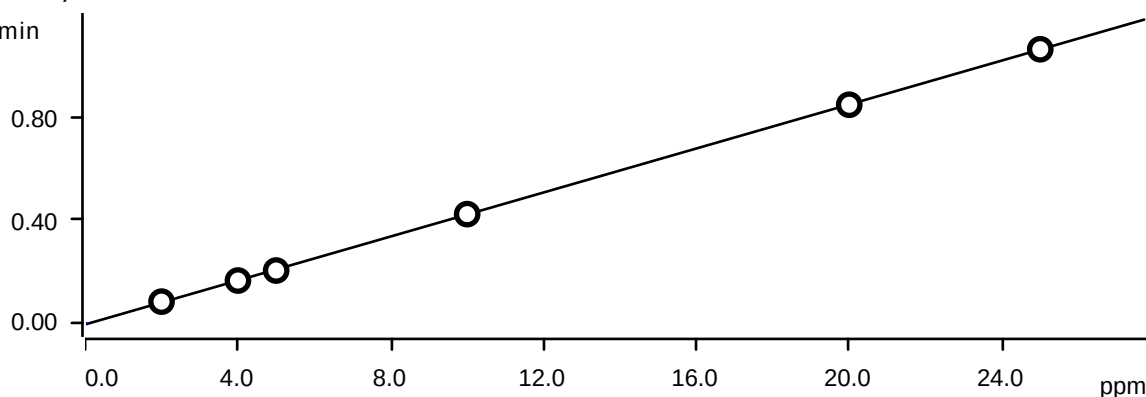

Function: $A = -4.26620E-3 + 4.25885E-3 \times Q$


Relative standard deviation: 0.597348 %

Correlation coefficient: 0.999981

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.166	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.205	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.423	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.846	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.061	STD7	2025-03-21 12:54:24 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

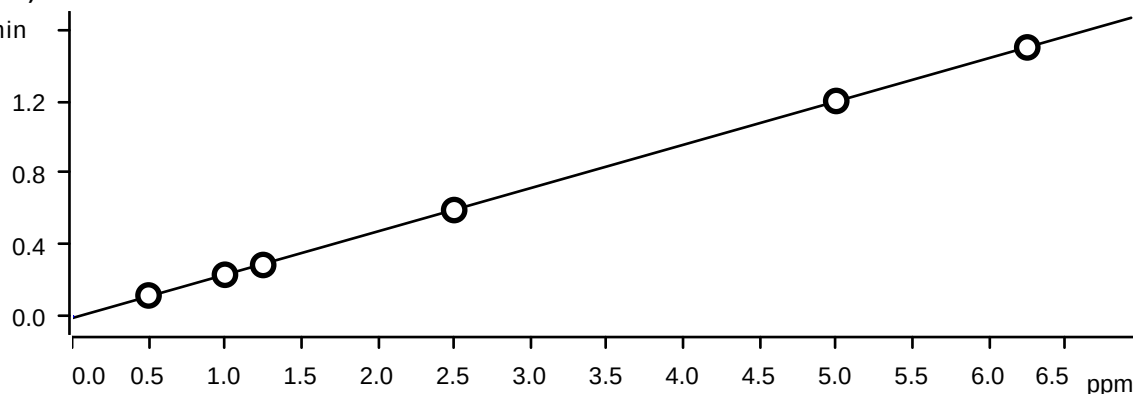


Function: $A = -9.20754E-3 + 0.0241631 \times Q$

Relative standard deviation: 0.659338 %

Correlation coefficient 0.999977

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.117	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.233	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.287	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.593	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.202	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.500	STD7	2025-03-21 12:54:24 UTC-4	used

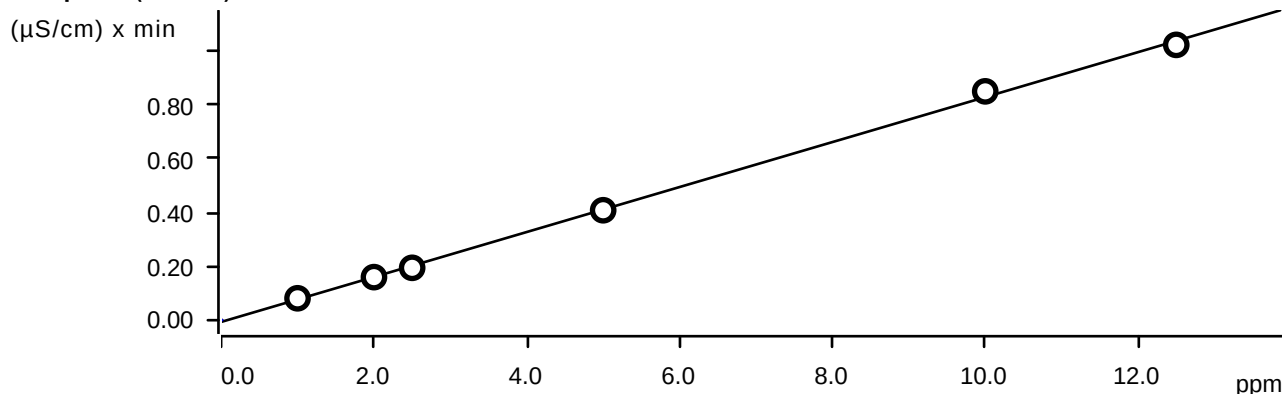
Phosphate (Anions)Function: $A = -6.92112E-3 + 8.35786E-3 \times Q$

Relative standard deviation 3.051728 %

Correlation coefficient 0.999508

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.081	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.160	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.194	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.408	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.850	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.023	STD7	2025-03-21 12:54:24 UTC-4	used

Sulfate (Anions)

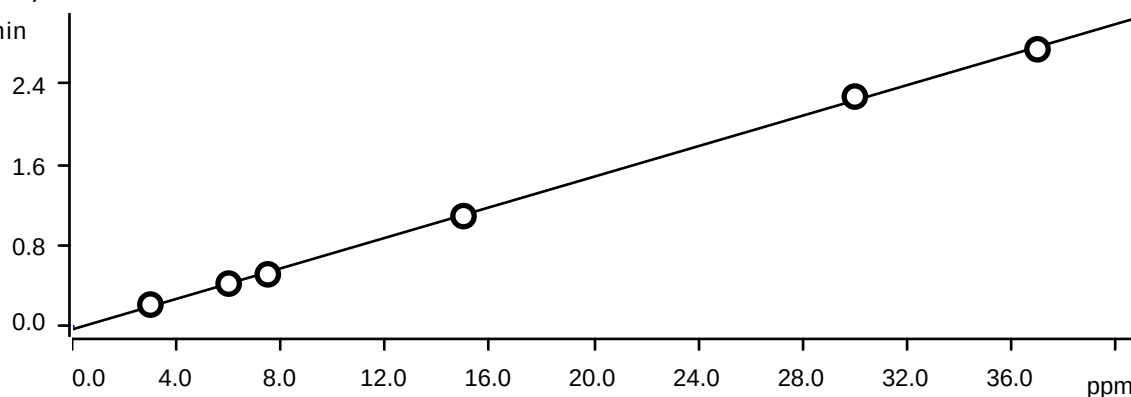 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0318458 + 7.56676E-3 \times Q$

Relative standard deviation 2.235653 %

Correlation coefficient 0.999739


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.214	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.422	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.514	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.091	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.276	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.745	STD7	2025-03-21 12:54:24 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-03-21 10:45:52 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

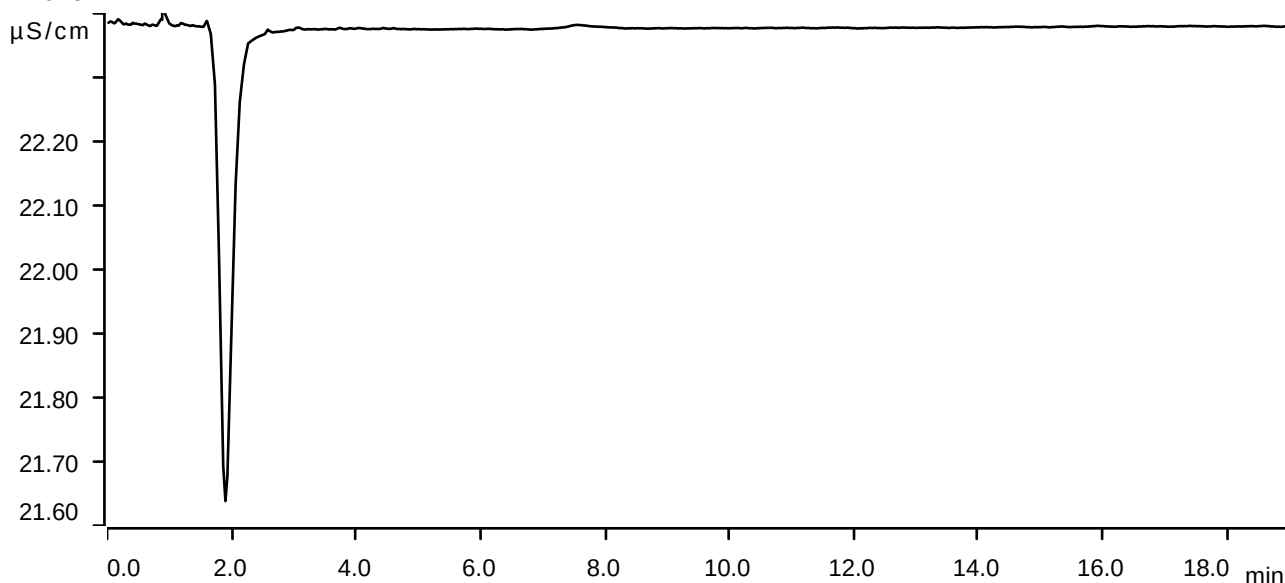Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-03-21 11:07:15 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

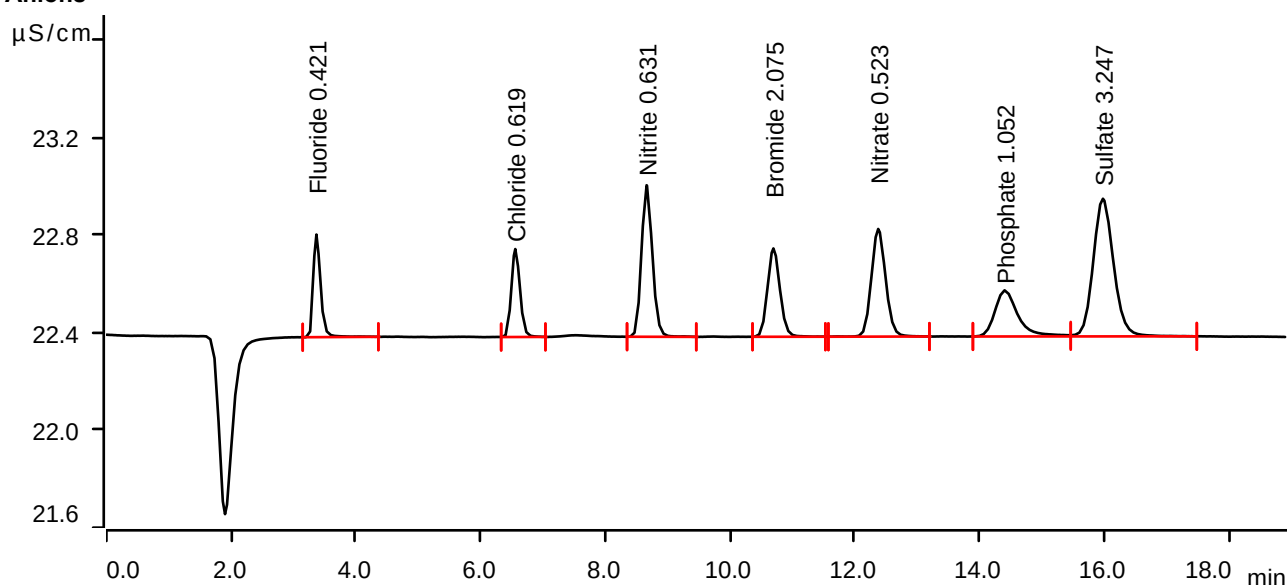

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.368	0.0570	0.420	0.421	Fluoride
2	6.557	0.0580	0.361	0.619	Chloride
3	8.662	0.1260	0.621	0.631	Nitrite
4	10.695	0.0841	0.362	2.075	Bromide
5	12.375	0.1171	0.441	0.523	Nitrate
6	14.403	0.0810	0.189	1.052	Phosphate
7	15.978	0.2139	0.564	3.247	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-03-21 11:28:39 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

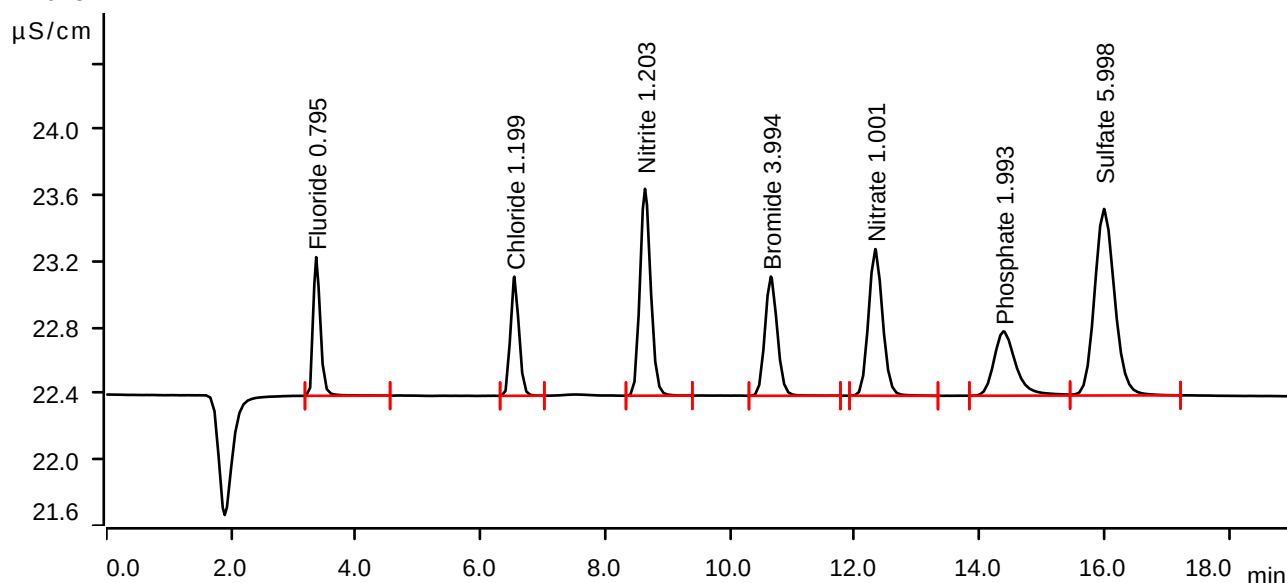

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.365	0.1110	0.839	0.795	Fluoride
2	6.542	0.1146	0.721	1.199	Chloride
3	8.637	0.2515	1.252	1.203	Nitrite
4	10.653	0.1658	0.722	3.994	Bromide
5	12.328	0.2325	0.888	1.001	Nitrate
6	14.383	0.1597	0.389	1.993	Phosphate
7	15.995	0.4220	1.129	5.998	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-03-21 11:50:04 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

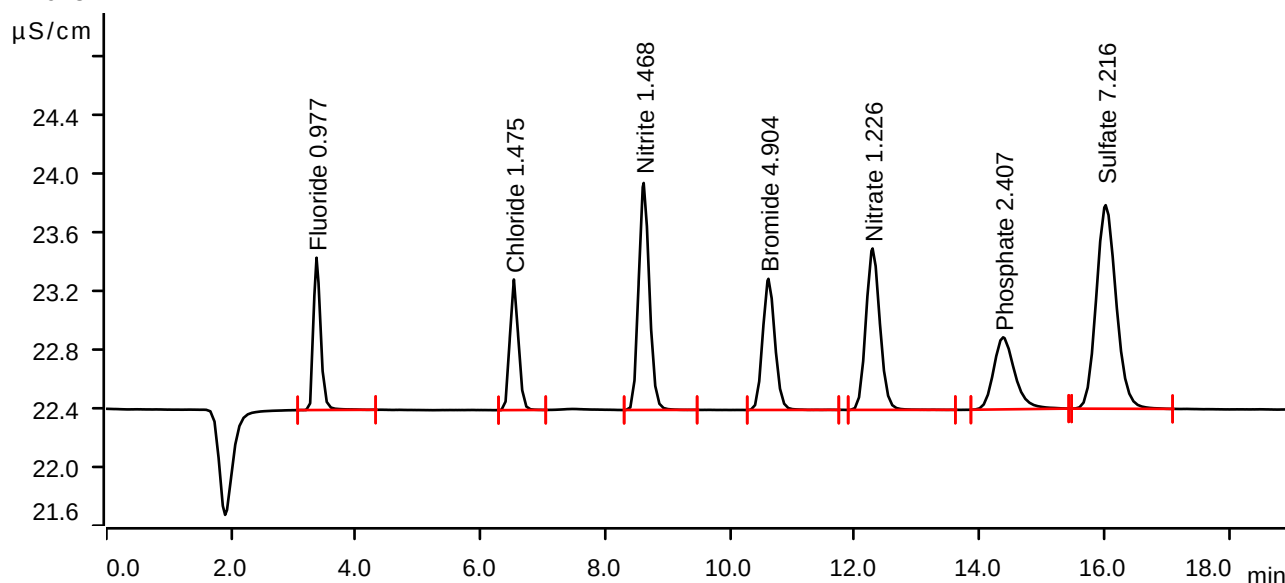

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.370	0.1374	1.040	0.977	Fluoride
2	6.533	0.1415	0.892	1.475	Chloride
3	8.615	0.3099	1.551	1.468	Nitrite
4	10.615	0.2046	0.896	4.904	Bromide
5	12.285	0.2869	1.103	1.226	Nitrate
6	14.378	0.1943	0.492	2.407	Phosphate
7	16.022	0.5142	1.391	7.216	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-03-21 12:11:30 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.20 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

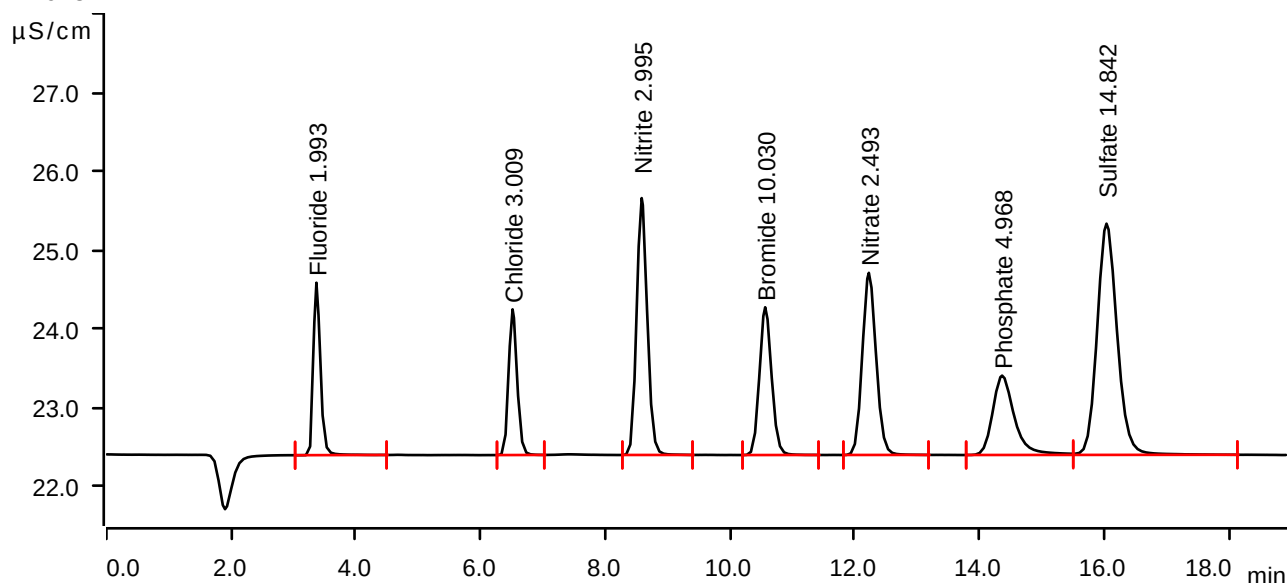

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.368	0.2843	2.188	1.993	Fluoride
2	6.513	0.2909	1.849	3.009	Chloride
3	8.583	0.6452	3.260	2.995	Nitrite
4	10.563	0.4229	1.875	10.030	Bromide
5	12.225	0.5933	2.311	2.493	Nitrate
6	14.362	0.4083	1.007	4.968	Phosphate
7	16.035	1.0913	2.934	14.842	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-03-21 12:32:57 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

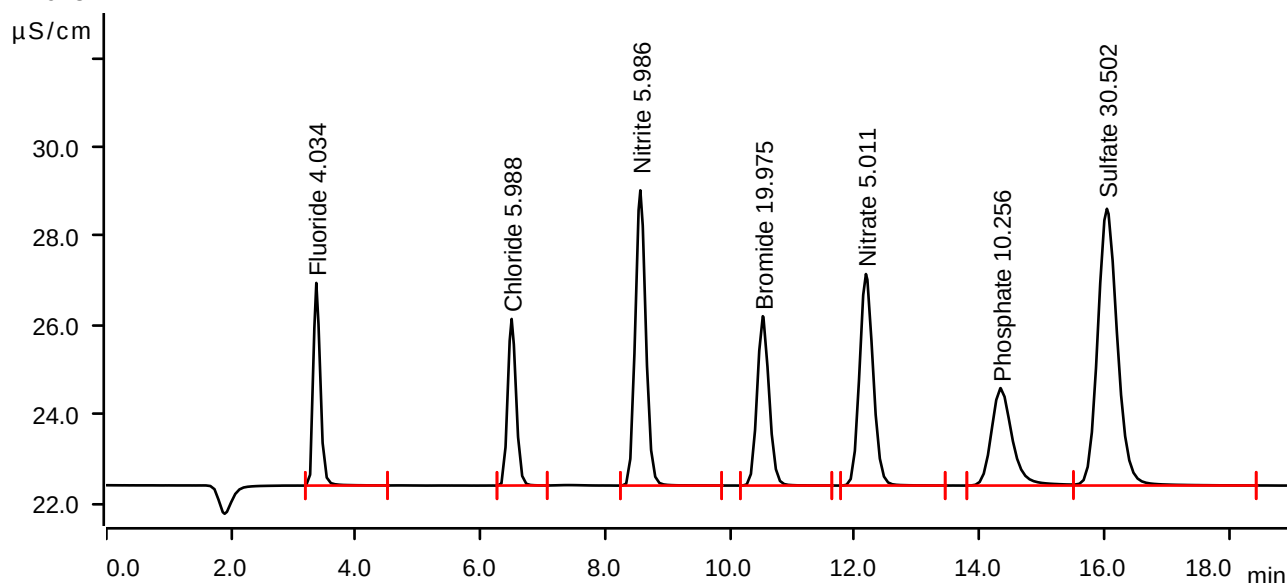

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.367	0.5796	4.549	4.034	Fluoride
2	6.498	0.5810	3.740	5.988	Chloride
3	8.562	1.3025	6.628	5.986	Nitrite
4	10.525	0.8465	3.803	19.975	Bromide
5	12.178	1.2015	4.749	5.011	Nitrate
6	14.338	0.8503	2.187	10.256	Phosphate
7	16.042	2.2762	6.214	30.502	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-03-21 12:54:24 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

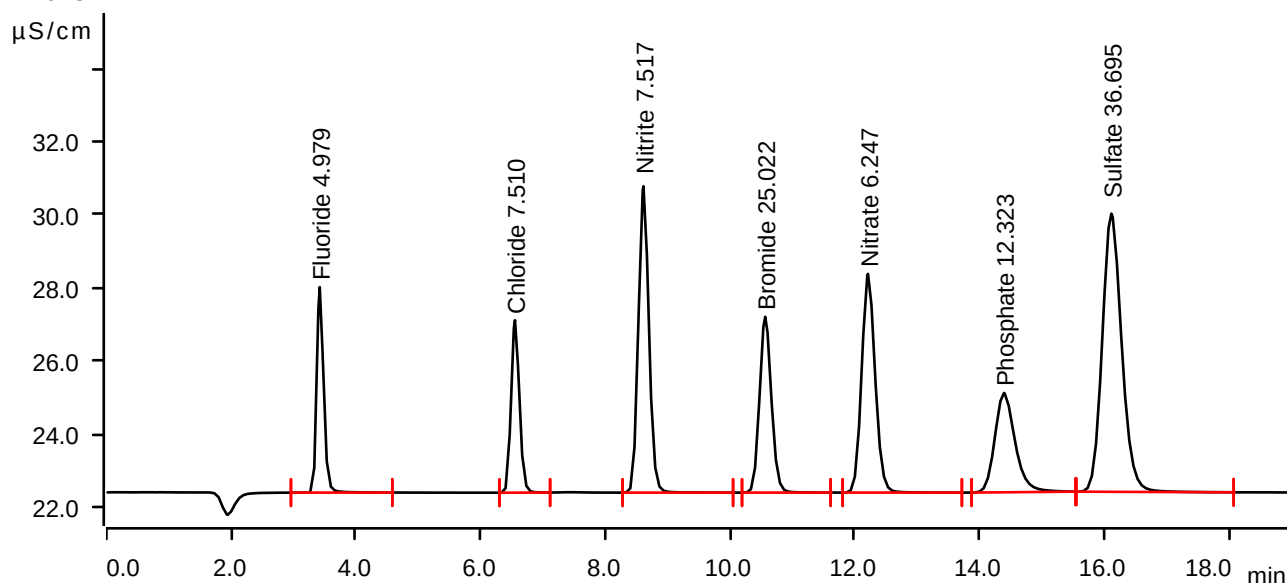

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.422	0.7164	5.617	4.979	Fluoride
2	6.552	0.7293	4.712	7.510	Chloride
3	8.612	1.6387	8.371	7.517	Nitrite
4	10.563	1.0614	4.806	25.022	Bromide
5	12.212	1.5003	5.978	6.247	Nitrate
6	14.392	1.0231	2.714	12.323	Phosphate
7	16.113	2.7448	7.604	36.695	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-04-03 09:38:28 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

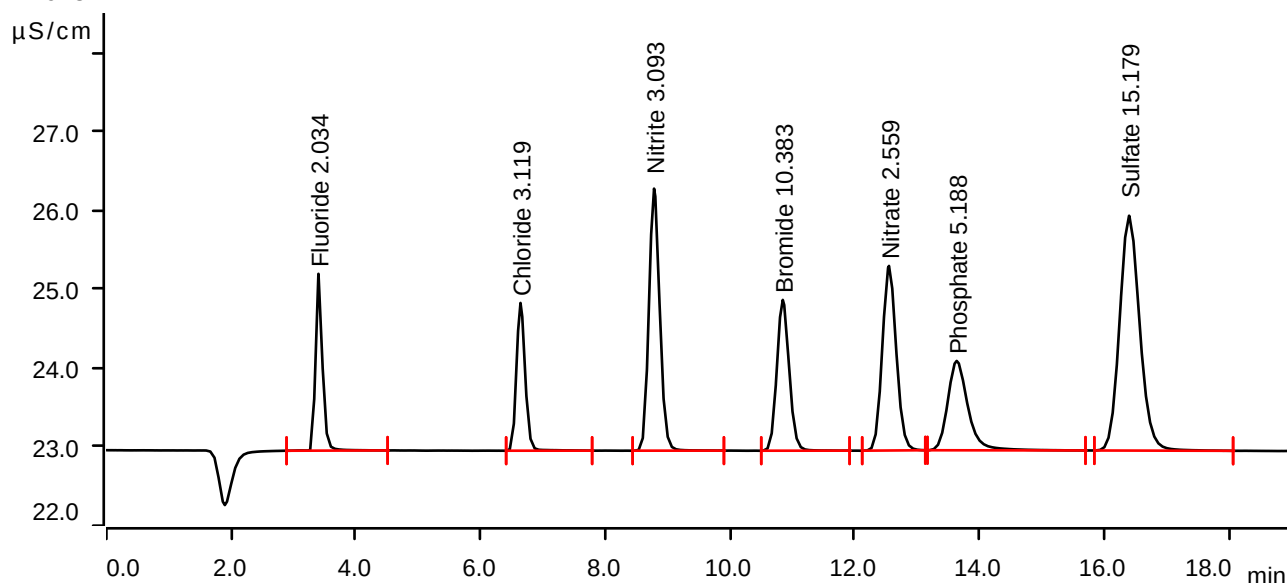


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.402	0.2903	2.243	2.034	Fluoride
2	6.640	0.3016	1.875	3.119	Chloride
3	8.782	0.6668	3.325	3.093	Nitrite
4	10.845	0.4379	1.914	10.383	Bromide
5	12.548	0.6091	2.343	2.559	Nitrate
6	13.633	0.4267	1.134	5.188	Phosphate
7	16.397	1.1167	2.980	15.179	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-04-03 09:59:58 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

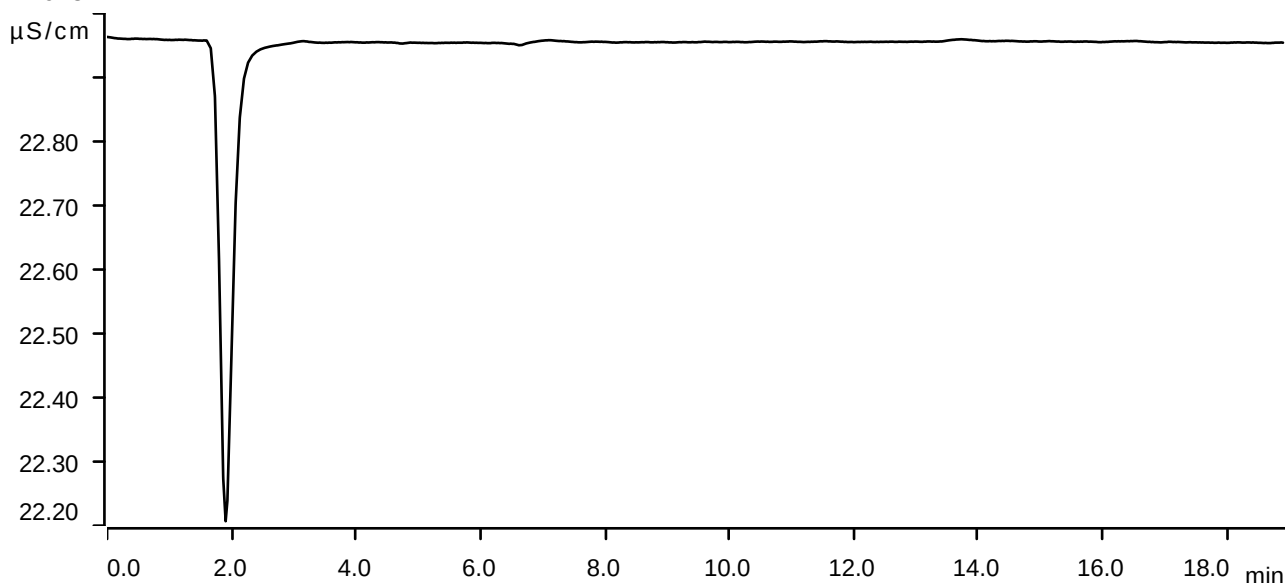Anions


Sample data

Ident LB135296BSW
Sample type Check standard 1
Determination start 2025-04-03 10:43:00 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

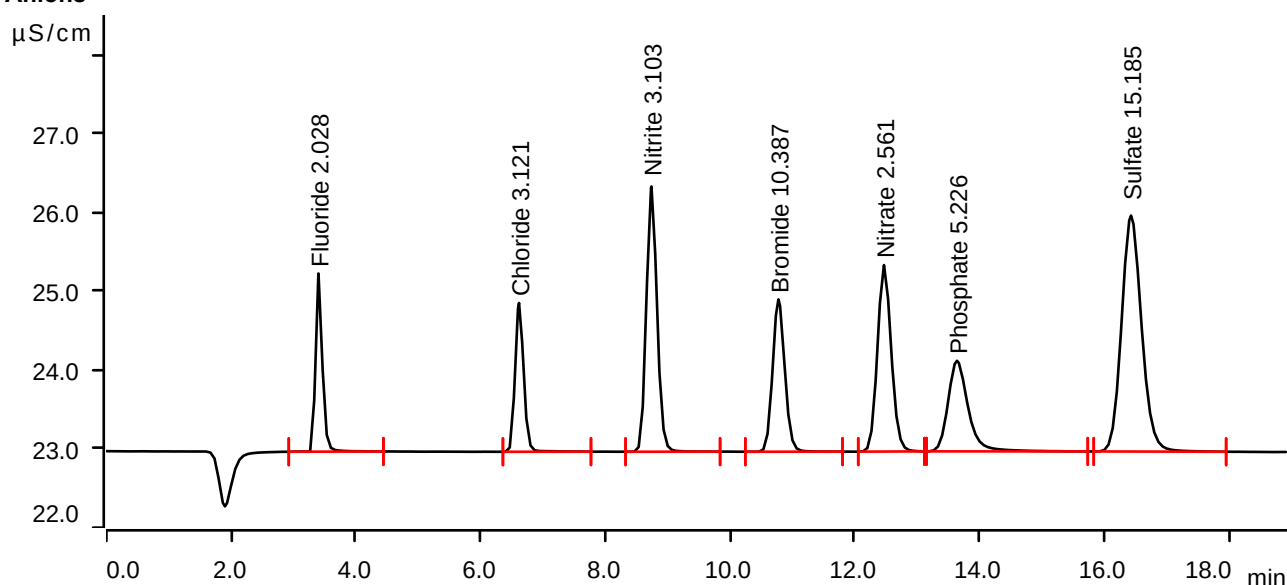


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.402	0.2894	2.260	2.028	Fluoride
2	6.617	0.3018	1.888	3.121	Chloride
3	8.740	0.6691	3.365	3.103	Nitrite
4	10.775	0.4381	1.933	10.387	Bromide
5	12.468	0.6096	2.366	2.561	Nitrate
6	13.638	0.4298	1.150	5.226	Phosphate
7	16.428	1.1172	2.994	15.185	Sulfate

Sample data

Ident LB135296BLW
Sample type Sample
Determination start 2025-04-03 11:04:32 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

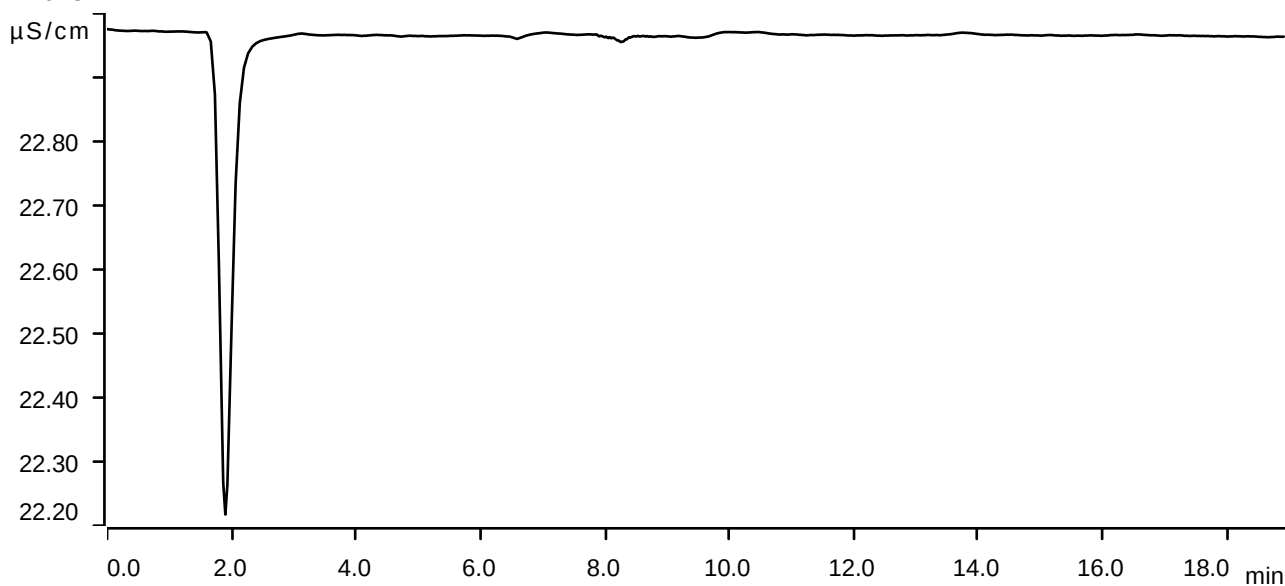Anions


Sample data

Ident Q1711-01
Sample type Sample
Determination start 2025-04-03 12:29:01 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

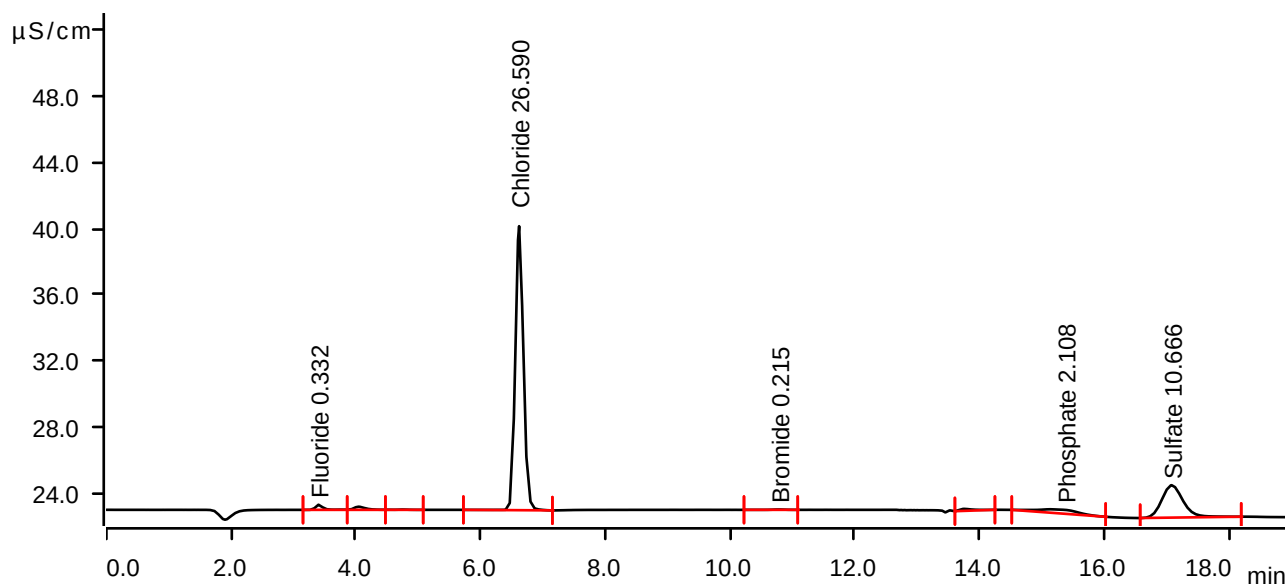

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.402	0.0440	0.309	0.332	Fluoride
2	4.043	0.0410	0.190	invalid	
3	4.747	0.0043	0.018	invalid	
4	6.618	2.5879	17.186	26.590	Chloride
5	10.788	0.0049	0.020	0.215	Bromide
6	13.753	0.0307	0.121	invalid	
7	15.130	0.1693	0.206	2.108	Phosphate
8	17.080	0.7752	1.961	10.666	Sulfate


Sample data

Ident Q1711-02MS
Sample type Sample
Determination start 2025-04-03 12:50:34 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

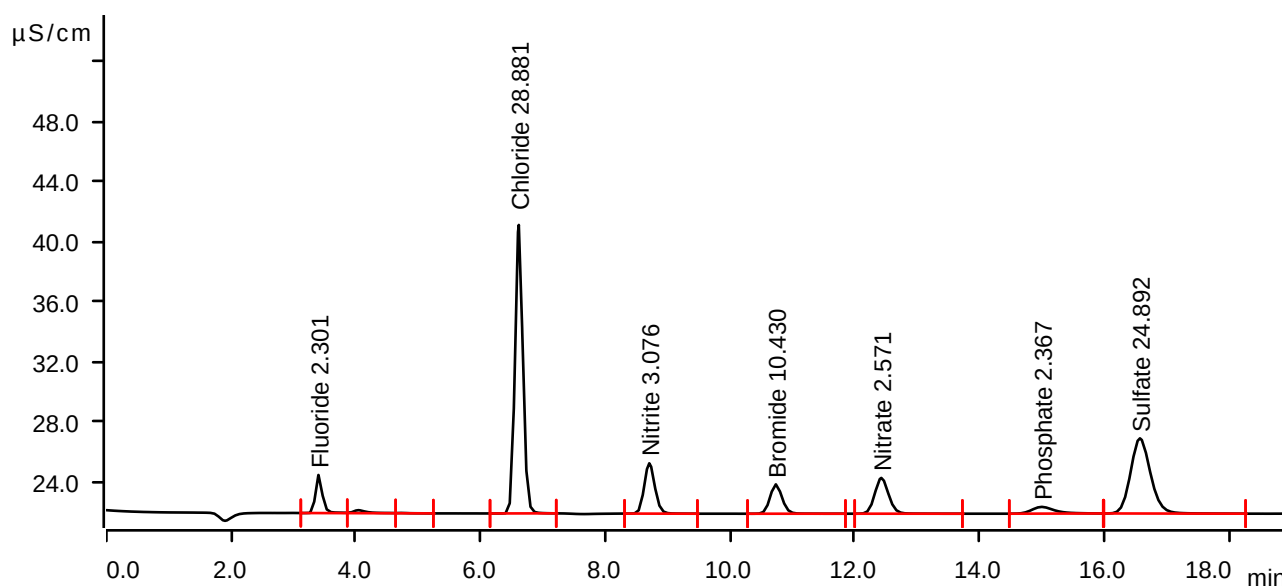

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.400	0.3289	2.526	2.301	Fluoride
2	4.042	0.0521	0.199	invalid	
3	4.730	0.0049	0.024	invalid	
4	6.613	2.8111	19.147	28.881	Chloride
5	8.705	0.6631	3.341	3.076	Nitrite
6	10.733	0.4399	1.947	10.430	Bromide
7	12.425	0.6120	2.375	2.571	Nitrate
8	14.997	0.1909	0.447	2.367	Phosphate
9	16.572	1.8517	4.990	24.892	Sulfate


Sample data

Ident Q1711-03MSD
Sample type Sample
Determination start 2025-04-03 13:12:08 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

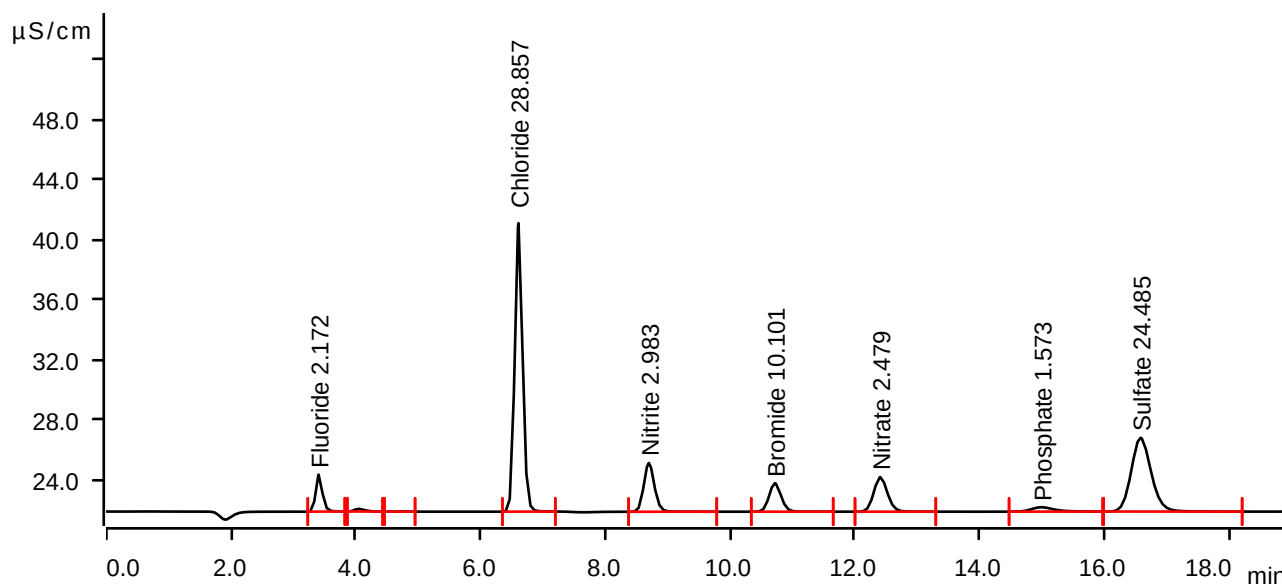

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.403	0.3102	2.455	2.172	Fluoride
2	4.045	0.0340	0.173	invalid	
3	4.737	0.0024	0.014	invalid	
4	6.608	2.8087	19.146	28.857	Chloride
5	8.698	0.6426	3.237	2.983	Nitrite
6	10.718	0.4259	1.891	10.101	Bromide
7	12.408	0.5899	2.298	2.479	Nitrate
8	14.993	0.1246	0.294	1.573	Phosphate
9	16.582	1.8209	4.901	24.485	Sulfate


Sample data

Ident Q1711-04
Sample type Sample
Determination start 2025-04-03 13:55:13 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

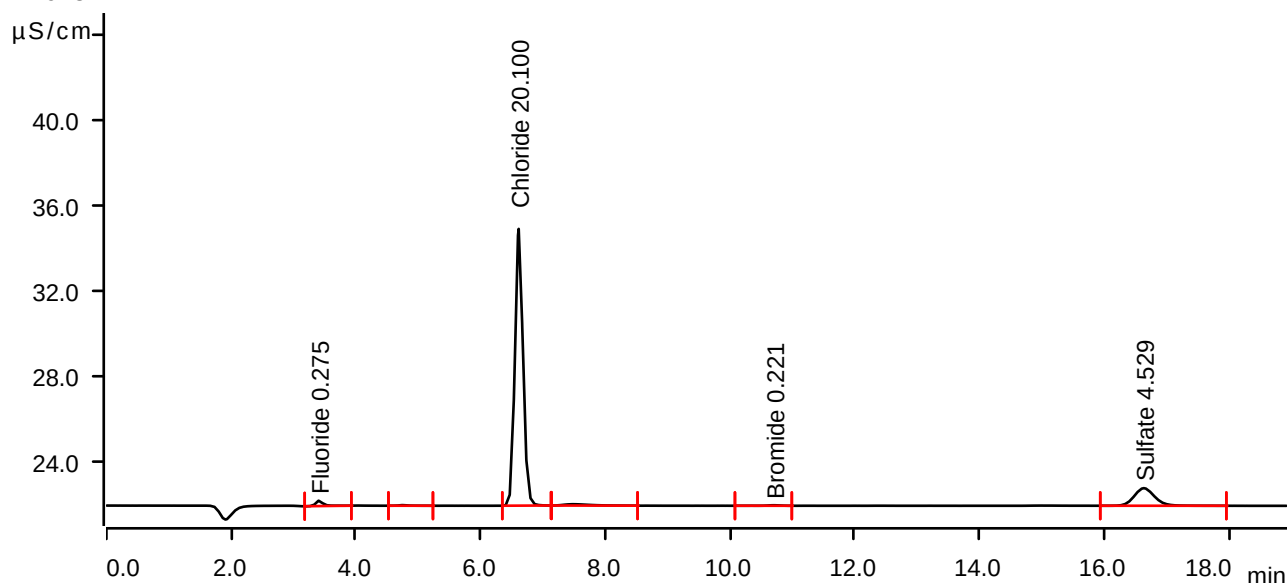

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.405	0.0358	0.250	0.275	Fluoride
2	4.750	0.0047	0.028	invalid	
3	6.612	1.9557	12.967	20.100	Chloride
4	7.478	0.0300	0.062	invalid	
5	10.705	0.0052	0.023	0.221	Bromide
6	16.633	0.3108	0.824	4.529	Sulfate


Sample data

Ident Q1711-08
Sample type Sample
Determination start 2025-04-03 14:16:48 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.20 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

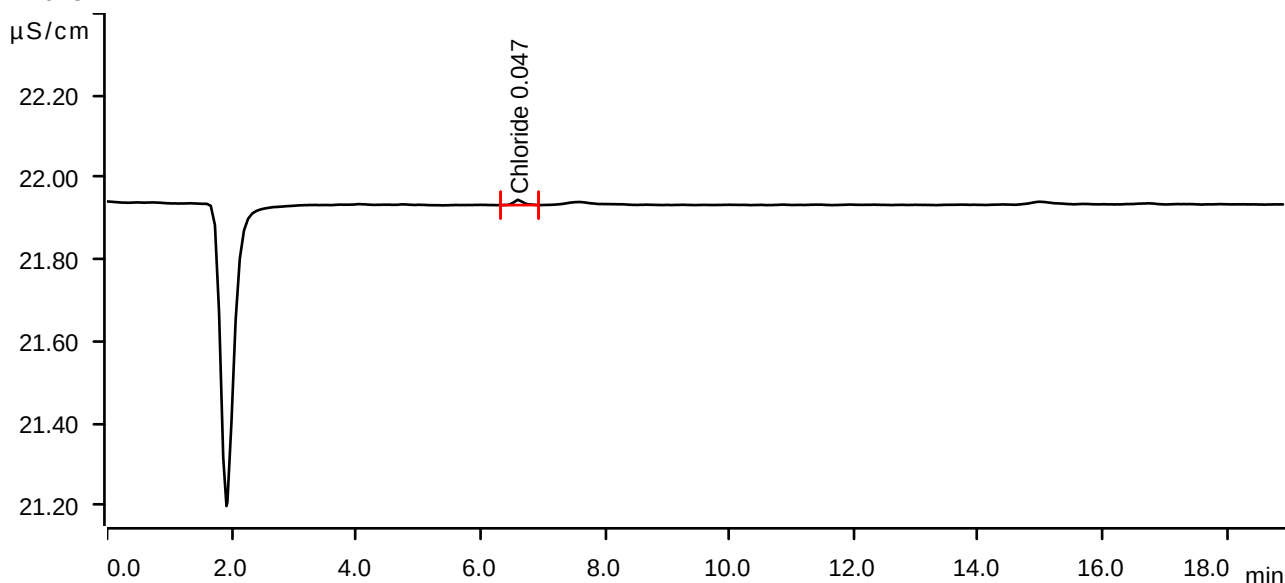

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.602	0.0023	0.013	0.047	Chloride


Sample data

Ident Q1716-01
Sample type Sample
Determination start 2025-04-03 14:38:22 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.96 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

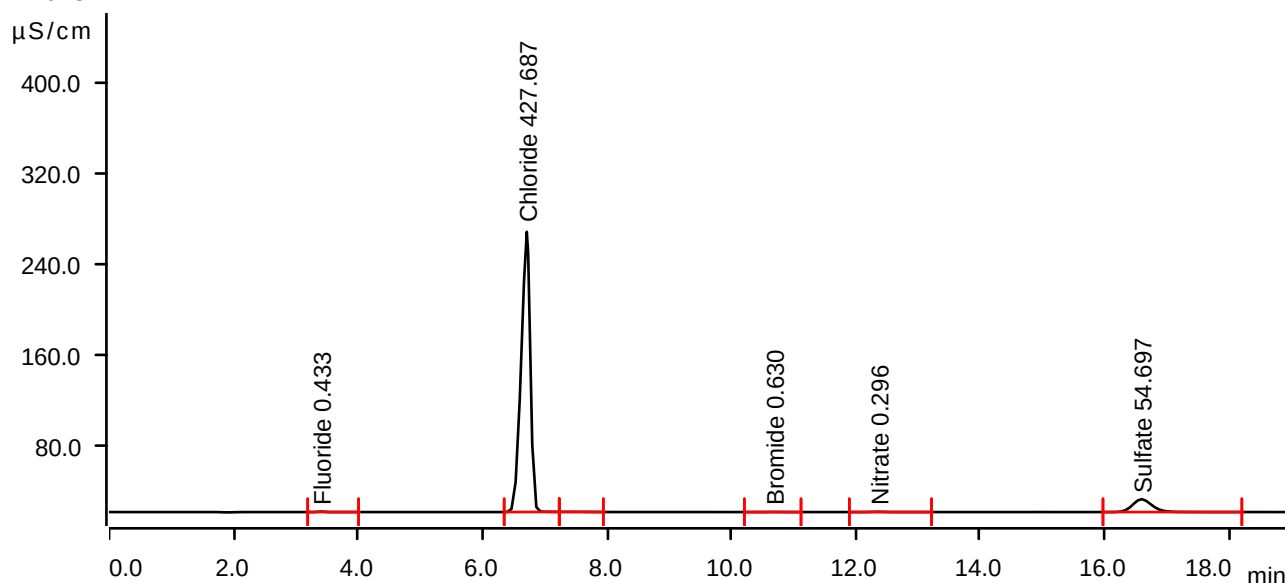

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.403	0.0586	0.445	0.433	Fluoride
2	6.713	41.6589	246.092	427.687	Chloride
3	7.423	0.0196	0.056	invalid	
4	10.682	0.0226	0.101	0.630	Bromide
5	12.363	0.0622	0.243	0.296	Nitrate
6	16.592	4.1070	11.278	54.697	Sulfate


Sample data

Ident Q1711-01DLX10
Sample type Sample
Determination start 2025-04-03 14:59:56 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

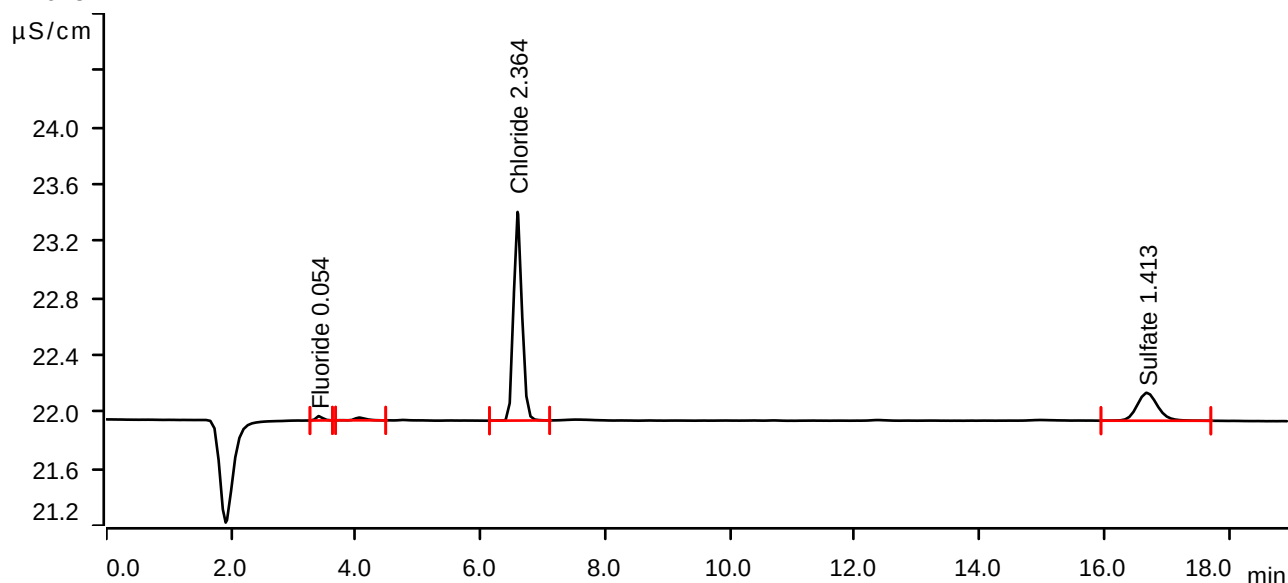

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.407	0.0039	0.030	0.054	Fluoride
2	4.052	0.0041	0.019	invalid	
3	6.593	0.2280	1.466	2.364	Chloride
4	16.682	0.0751	0.196	1.413	Sulfate


Sample data

Ident Q1711-04DLX5
Sample type Sample
Determination start 2025-04-03 15:21:28 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

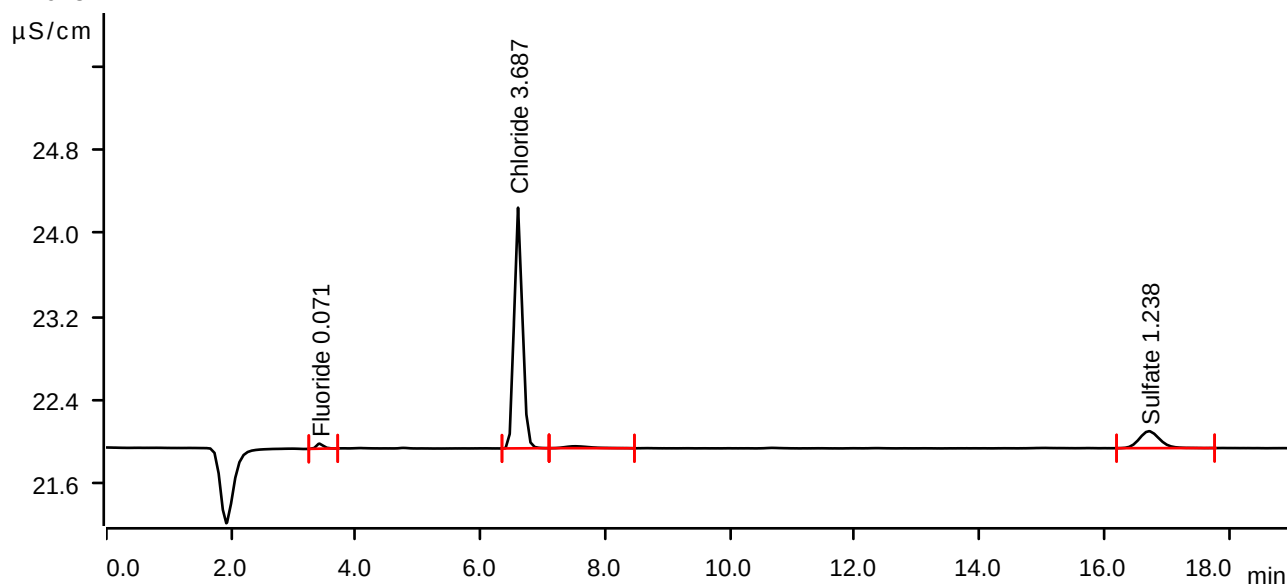

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.418	0.0063	0.048	0.071	Fluoride
2	6.600	0.3569	2.302	3.687	Chloride
3	7.522	0.0089	0.018	invalid	
4	16.717	0.0618	0.162	1.238	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-04-03 15:43:00 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.92 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

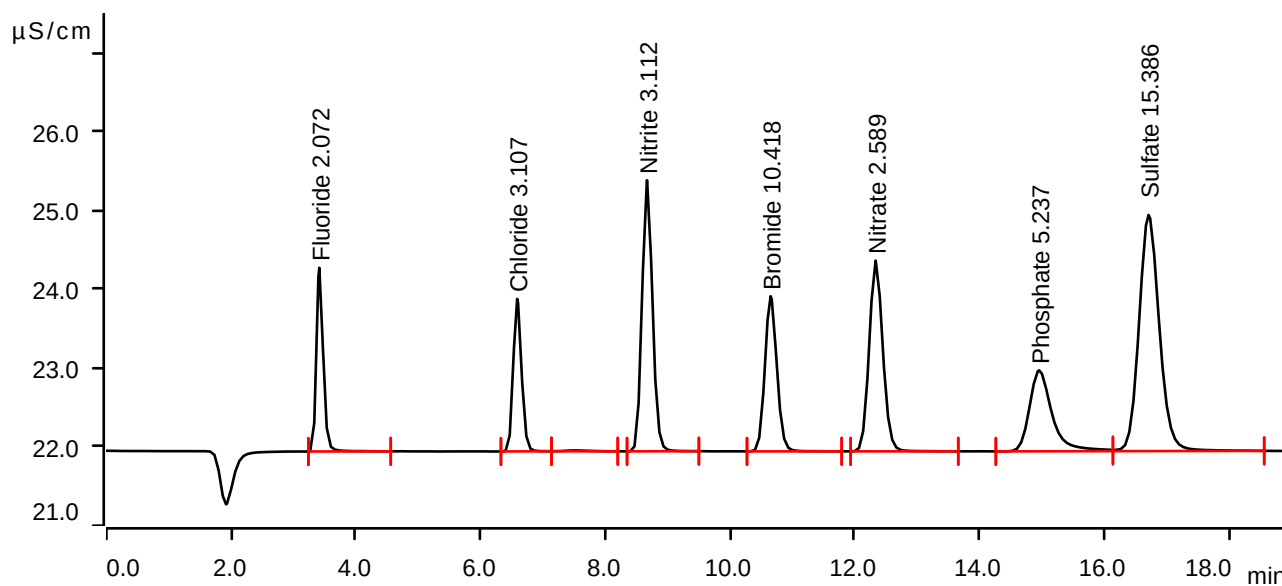


Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.415	0.2957	2.330	2.072	Fluoride
2	6.587	0.3004	1.936	3.107	Chloride
3	7.513	0.0045	0.011	invalid	
4	8.670	0.6709	3.439	3.112	Nitrite
5	10.650	0.4394	1.969	10.418	Bromide
6	12.335	0.6163	2.420	2.589	Nitrate
7	14.955	0.4308	1.027	5.237	Phosphate
8	16.710	1.1324	2.996	15.386	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-04-03 17:16:13 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.81 MPa
Maximum pressure monitored yes
Temperature ---- °C

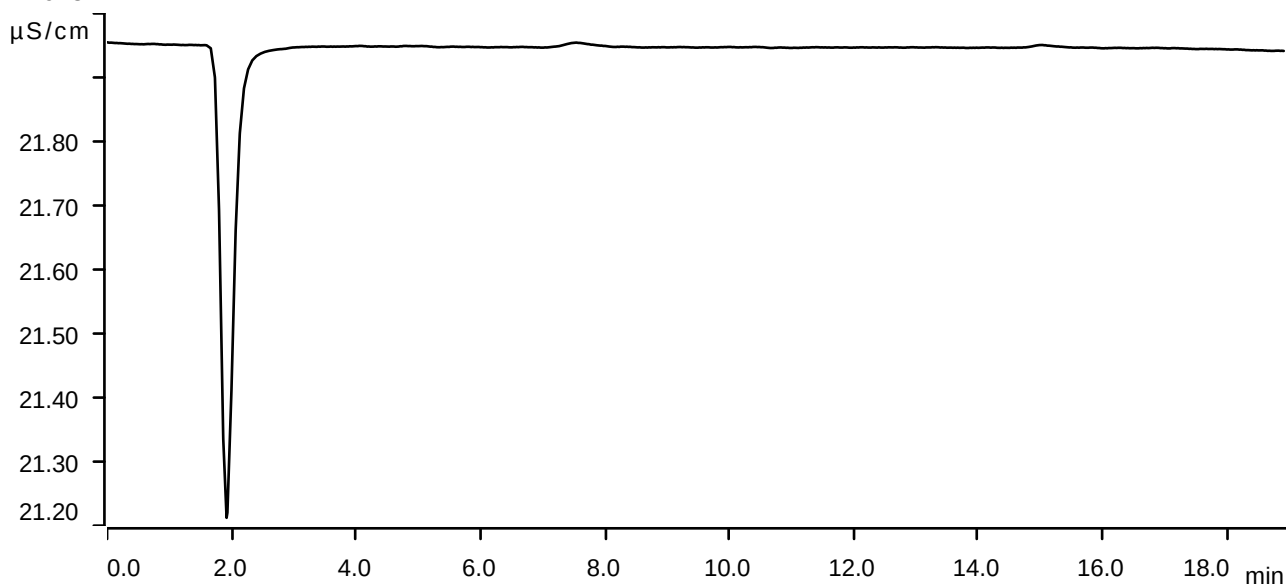Anions

WORKLIST(Hardcopy Internal Chain)

LB135296

WorkList Name : ANIONS-04032025

WorkList ID : 188704

Department : Wet-Chemistry

Date : 04-03-2025 11:03:28

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1711-01	MW-18B-56-040225	Water	Anions Group1	Cool 4 deg C	JACO05	I41	04/02/2025	9056A
Q1711-02	Q1711-01MS	Water	Anions Group1	Cool 4 deg C	JACO05	I41	04/02/2025	9056A
Q1711-03	Q1711-01MSD	Water	Anions Group1	Cool 4 deg C	JACO05	I41	04/02/2025	9056A
Q1711-04	MW-17B-55-040225	Water	Anions Group1	Cool 4 deg C	JACO05	I41	04/02/2025	9056A
Q1711-08	EB01-040225	Water	Anions Group1	Cool 4 deg C	JACO05	I41	04/02/2025	9056A

Date/Time 04.03.2025, 11:15
 Raw Sample Received by: NF(WC)
 Raw Sample Relinquished by: [Signature]

Date/Time 04.03.2025, 16:00
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: NF(WC)

LB135296

WORKLIST(Hardcopy Internal Chain)

WorkList Name : ANIONS -04032025

WorkList ID : 188735

Department : Wet-Chemistry

Date : 04-03-2025 13:41:37

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1716-01	MOD-FOR-LRSA	Water	Anions Group1	Cool 4 deg C	PSEG04	I31	04/03/2025	9056A

Date/Time 04.03.2025, 13:45
Raw Sample Received by: NF(WC)
Raw Sample Relinquished by: TD WCC

Date/Time 04.03.2025, 16:00
Raw Sample Received by: TD WCC
Raw Sample Relinquished by: NF(WC)