
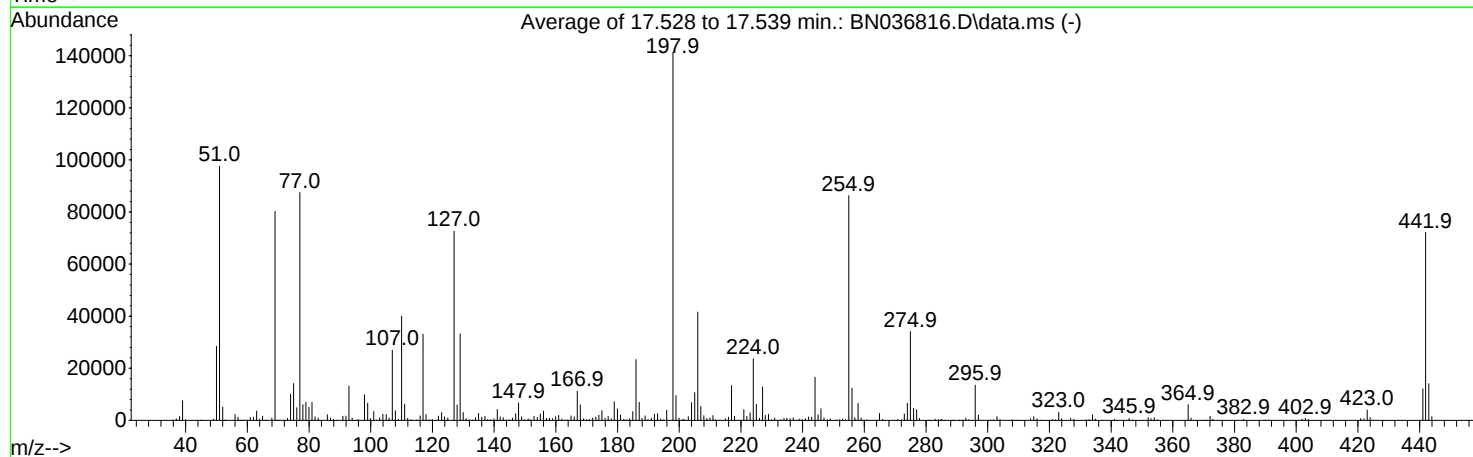


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040325\
Data File : BN036816.D
Acq On : 03 Apr 2025 11:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 04 03:26:58 2025

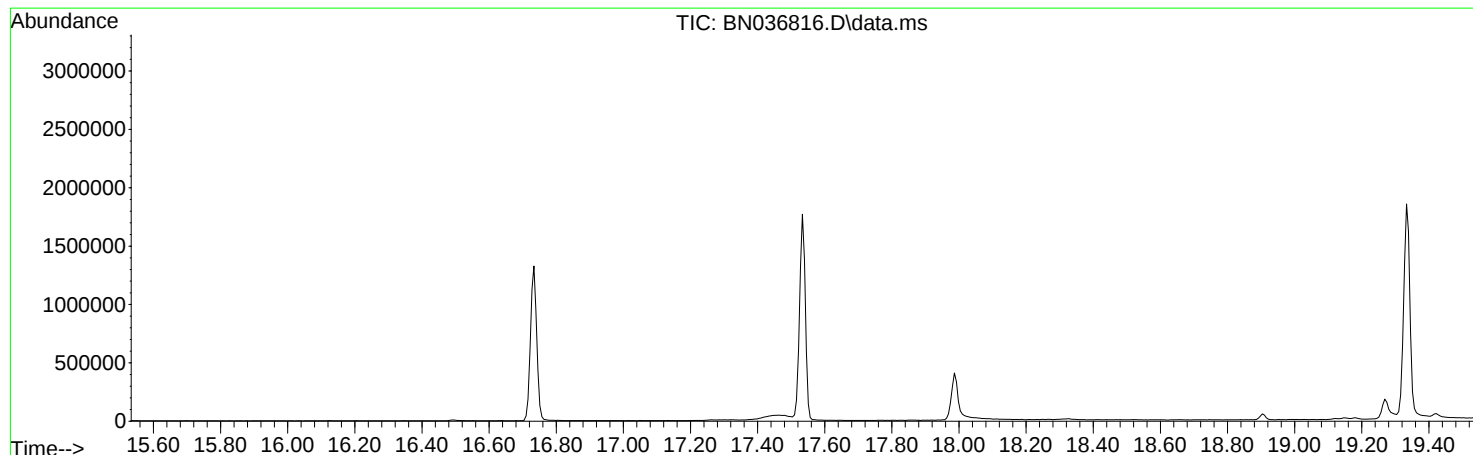

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.1	97555	PASS
68	69	0.00	2	1.1	870	PASS
69	198	0.00	100	56.8	80233	PASS
70	69	0.00	2	0.2	177	PASS
127	198	10	80	51.4	72618	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	141227	PASS
199	198	5	9	6.8	9559	PASS
275	198	10	60	24.2	34109	PASS
365	198	1	100	4.3	6027	PASS
441	198	0.01	100	8.6	12097	PASS
442	442	50	100	100.0	72160	PASS
443	442	15	24	19.5	14074	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/3/2025	BNA_N	<u>BN036816.D</u>
Compound Name	Response	Retention Time
DDT	569032	20.574
DDD	7825	20.186
DDE	69	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7894	576926	1.37

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040325\
Data File : BN036816.D
Acq On : 03 Apr 2025 11:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 03 14:18:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 03 14:16:27 2025
Response via : Initial Calibration

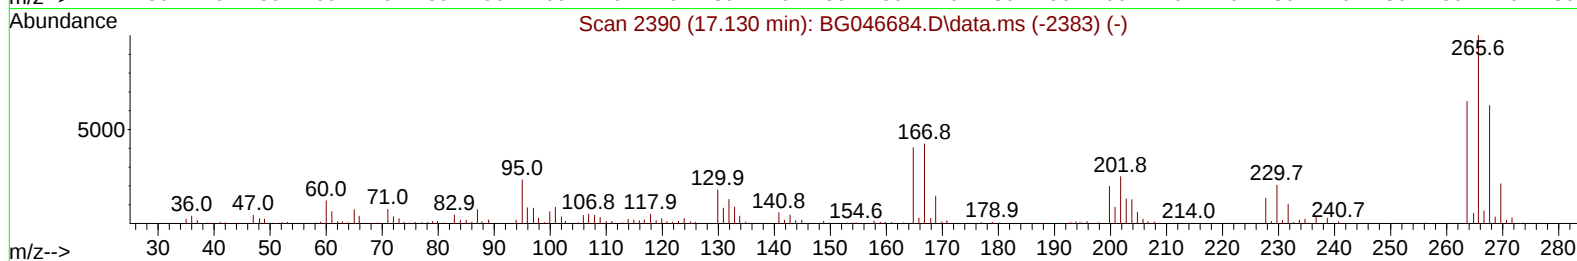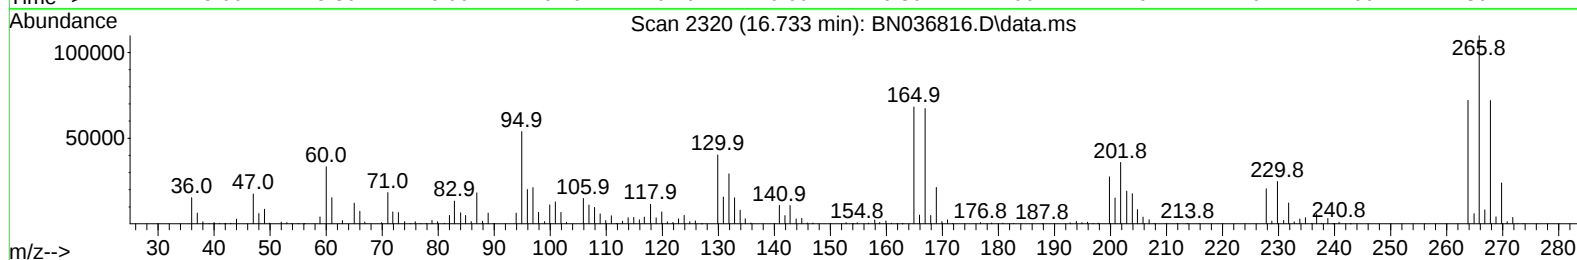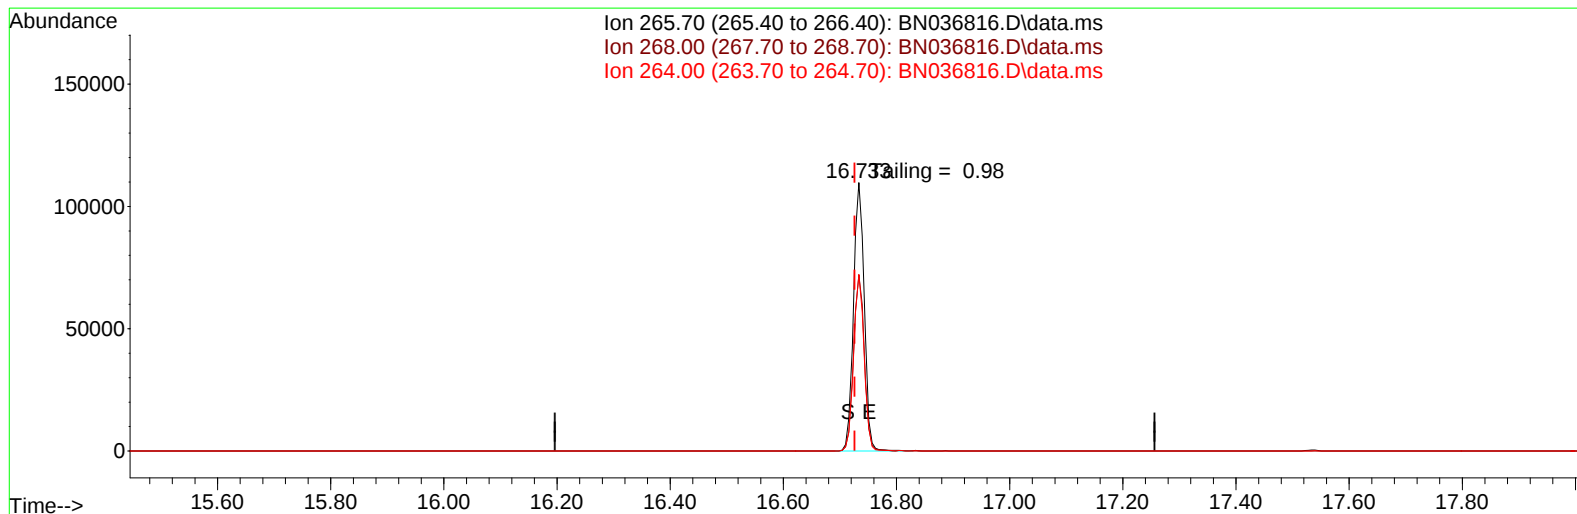

TIC: BN036816.D\data.ms

(70) Pentachlorophenol (C)

16.733min (+ 0.007) 15766.87 ng




response 145132

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.56
264.00	61.60	65.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040325\
Data File : BN036816.D
Acq On : 03 Apr 2025 11:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 03 14:25:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 03 14:16:27 2025
Response via : Initial Calibration

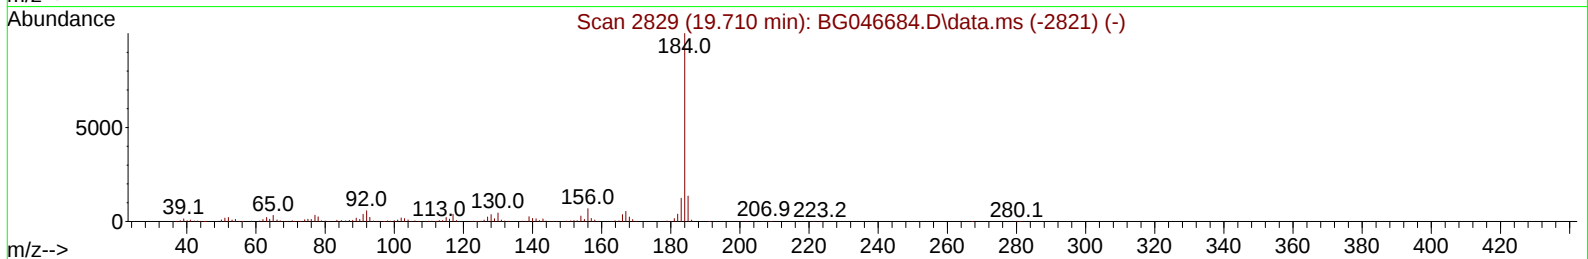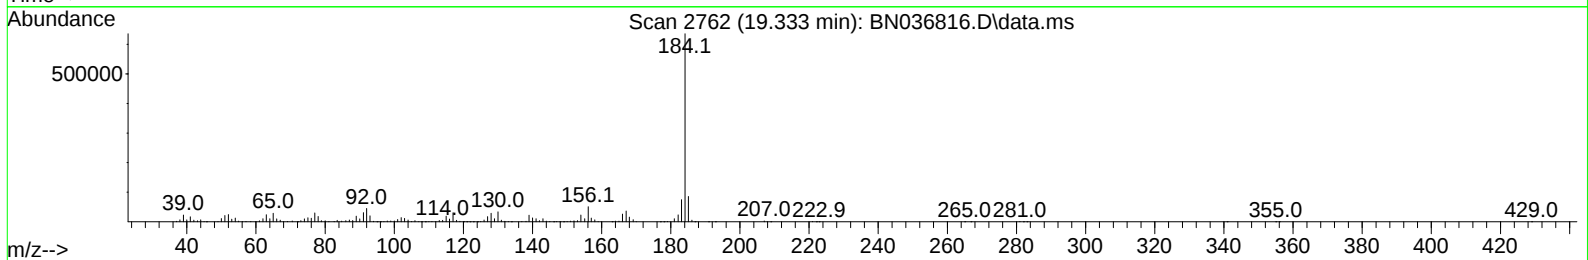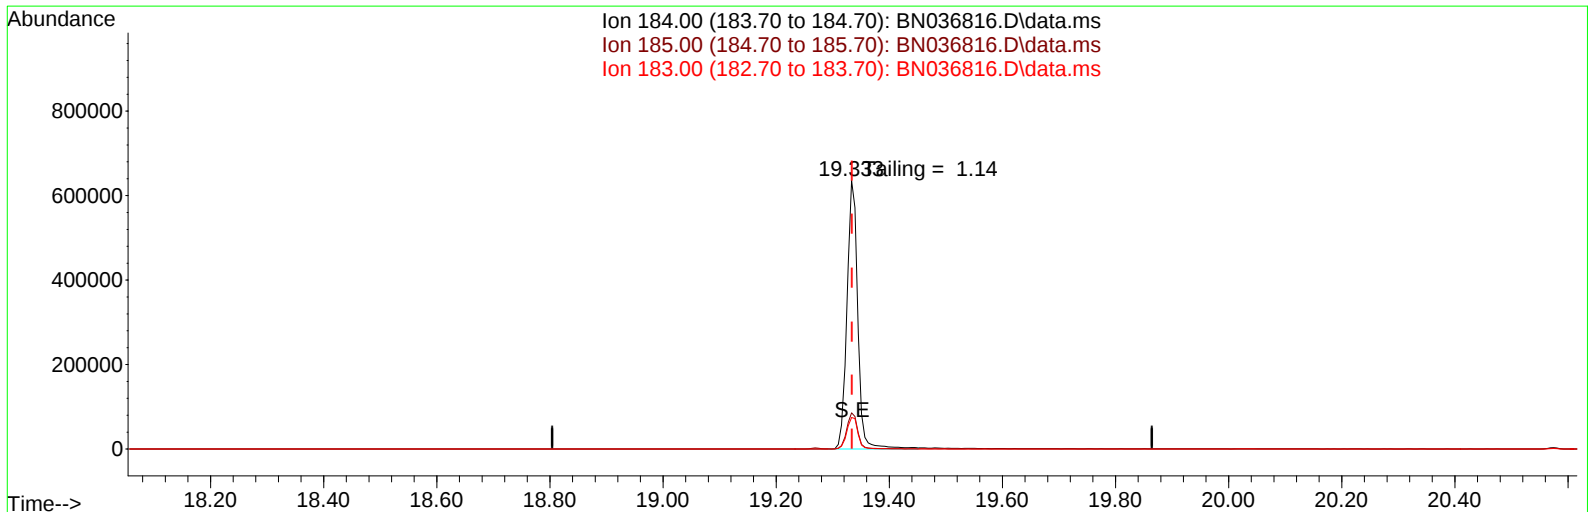

TIC: BN036816.D\data.ms

(77) Benzidine

19.333min (-0.001) 0.00 ng

response 839528

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.48
183.00	13.20	11.75
0.00	0.00	0.00