
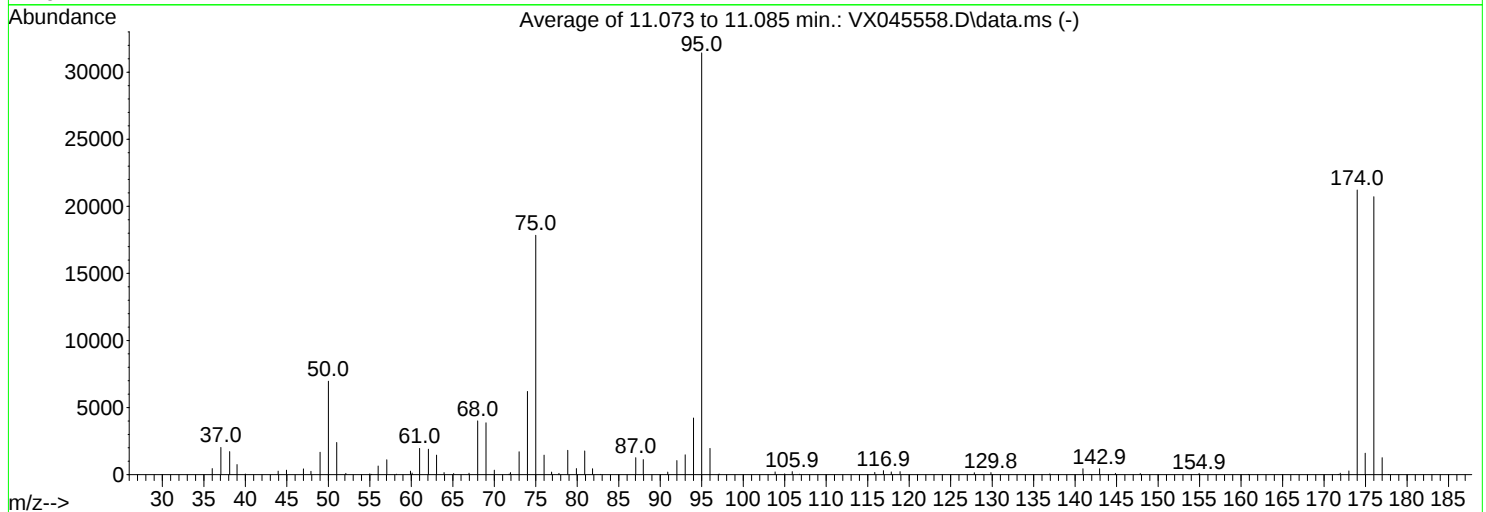


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040325\
Data File : VX045558.D
Acq On : 03 Apr 2025 10:01
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Title : SW846 8260
Last Update : Wed Apr 02 03:11:43 2025

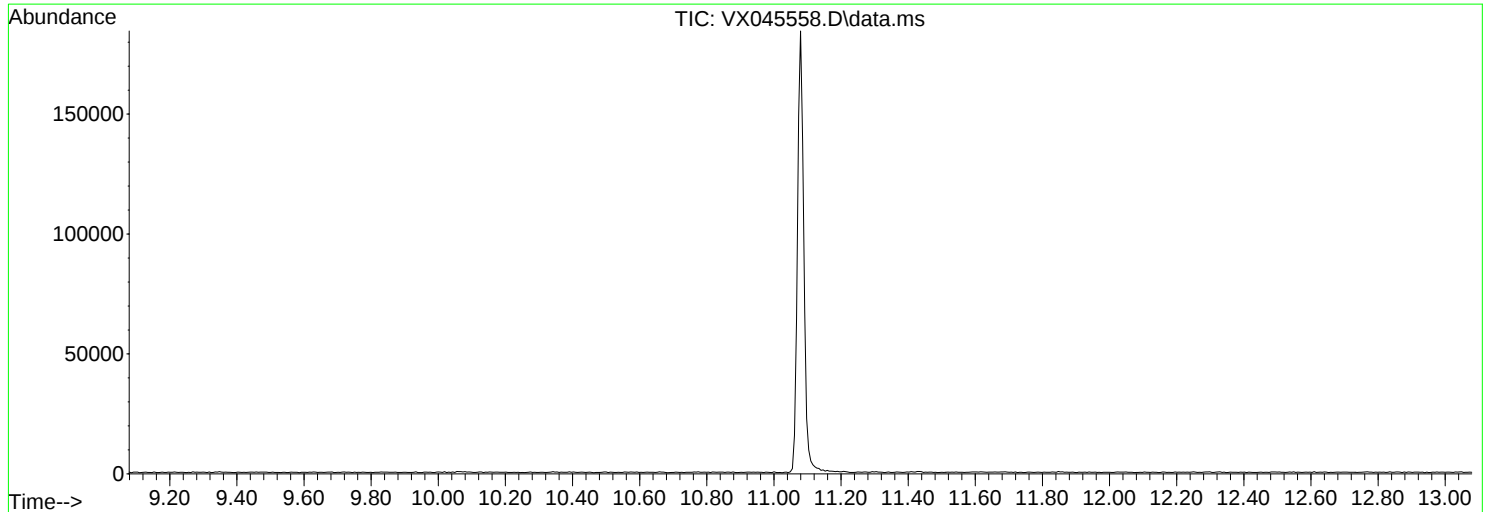

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.2	6965	PASS
75	95	30	60	56.7	17840	PASS
95	95	100	100	100.0	31443	PASS
96	95	5	9	6.2	1961	PASS
173	174	0.00	2	1.3	271	PASS
174	95	50	100	67.5	21221	PASS
175	174	5	9	7.5	1598	PASS
176	174	95	101	97.6	20720	PASS
177	176	5	9	6.1	1260	PASS