

## **DATA PACKAGE VOLATILE ORGANICS**

**PROJECT NAME : FORMER SCHLUMBERGER STC PTC SITE D3868221**

**JACOBS ENGINEERING GROUP, INC.**

**412 Mt. Kemble Ave**

**Downtown Building**

**Morristown, NJ - 07960**

**Phone No: 9732670555**

**ORDER ID : Q1711**

**ATTENTION : John Ynfante**



**Laboratory Certification ID # 20012**

<b>1) VOLATILES DATA</b>	<b>2</b>
<b>2) Signature Page</b>	<b>4</b>
<b>3) Case Narrative</b>	<b>5</b>
<b>4) Qualifier Page</b>	<b>7</b>
<b>5) Conformance/Non Conformance</b>	<b>8</b>
<b>6) QA Checklist</b>	<b>10</b>
<b>7) Chronicle</b>	<b>11</b>
<b>8) Hit Summary</b>	<b>12</b>
<b>9) QC Data Summary For VOCMS Group3</b>	<b>13</b>
<b>9.1) Deuterated Monitoring Compound Summary</b>	<b>14</b>
<b>9.2) MS/MSD Summary</b>	<b>15</b>
<b>9.3) LCS/LCSD Summary</b>	<b>17</b>
<b>9.4) Method Blank Summary</b>	<b>19</b>
<b>9.5) GS/MS Tune Summary</b>	<b>21</b>
<b>9.6) Internal Standard Area and RT Summary</b>	<b>24</b>
<b>10) Sample Data</b>	<b>28</b>
<b>10.1) MW-18B-56-040225</b>	<b>29</b>
<b>10.2) MW-17B-55-040225</b>	<b>39</b>
<b>10.3) RMW-05B-89-040225</b>	<b>48</b>
<b>10.4) EB01-040225</b>	<b>57</b>
<b>10.5) TB01-040225</b>	<b>65</b>
<b>11) Calibration Data Summary</b>	<b>72</b>
<b>11.1) Initial Calibration Data</b>	<b>73</b>
<b>11.1.1) VX040225</b>	<b>73</b>
<b>11.2) Continued Calibration Data</b>	<b>442</b>
<b>11.2.1) VX045559.D</b>	<b>442</b>
<b>11.2.2) VX045586.D</b>	<b>501</b>
<b>12) QC Sample Data</b>	<b>560</b>
<b>12.1) Tune Raw Data</b>	<b>561</b>
<b>12.2) Method Blank Data</b>	<b>564</b>
<b>12.3) LCS Data</b>	<b>578</b>
<b>12.4) MS Data</b>	<b>684</b>
<b>12.5) MSD Data</b>	<b>737</b>
<b>13) Manual Integration</b>	<b>790</b>
<b>14) Analytical Runlogs</b>	<b>794</b>

## Table Of Contents for Q1711

<b>15) Standard Prep Logs</b>	<b>806</b>	
<b>16) Shipping Document</b>	<b>908</b>	
<b>16.1) Chain Of Custody</b>	<b>909</b>	
<b>16.2) ROC</b>	<b>911</b>	
<b>16.3) Lab Certificate</b>	<b>914</b>	
<b>16.4) Internal COC</b>	<b>915</b>	
	6	
	7	
	8	
	9	
	10	
	11	
	12	
	13	
	14	
	15	
	16	

## Cover Page

**Order ID :** Q1711

**Project ID :** Former Schlumberger STC PTC Site D3868221

**Client :** JACOBS Engineering Group, Inc.

### Lab Sample Number

Q1711-01  
Q1711-02  
Q1711-03  
Q1711-04  
Q1711-07  
Q1711-08  
Q1711-10  
Q1711-12  
Q1711-13  
Q1711-14  
Q1711-15  
Q1711-16

### Client Sample Number

MW-18B-56-040225  
MW-18B-56-040225MS  
MW-18B-56-040225MSD  
MW-17B-55-040225  
RMW-05B-89-040225  
EB01-040225  
TB01-040225  
MW-17B-55-040225  
EB01-040225  
MW-18B-56-040225  
MW-18B-56-040225MS  
MW-18B-56-040225MSD

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : \_\_\_\_\_

Date: 4/10/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

## CASE NARRATIVE

**JACOBS Engineering Group, Inc.**

**Project Name:** Former Schlumberger STC PTC Site D3868221

**Project # N/A**

**Chemtech Project # Q1711**

**Test Name:** VOCMS Group3

### **A. Number of Samples and Date of Receipt:**

12 Water samples were received on 04/02/2025.

### **B. Parameters**

According to the Chain of Custody document, the following analyses were requested: Alkalinity, Anions Group1, Dissolved ICP-Group2, Dissolved Metals Group3, Metals Group4, SVOC-SIMGroup1, TDS, VOC-TRACE-SFAM and VOCMS Group3. This data package contains results for VOCMS Group3.

### **C. Analytical Techniques:**

The analysis performed on instrument MSVOA\_X were done using GC column DB-624UI 20m 0.18mm 1.0 um. Cat#121-1324UIThe analysis of VOCMS Group3 was based on method 8260D.

### **D. QA/ QC Samples:**

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria.

The Internal Standards Areas met the acceptable requirements.

The Retention Times were acceptable for all samples.

The MS {Q1711-02MS} with File ID: VX045591.D recoveries met the requirements for all compounds except for cis-1,2-Dichloroethene[30%] this compound did not meet the NJDKQP criteria and in-house criteria due to matrix interference.

The MSD {Q1711-03MSD} with File ID: VX045577.D recoveries met the acceptable requirements except for cis-1,2-Dichloroethene[50%] this compound did not meet the NJDKQP criteria and in-house criteria due to matrix interference.

The RPD for {Q1711-03MSD} with File ID: VX045577.D met criteria except for cis-1,2-Dichloroethene[50%] this compound did not meet the NJDKQP criteria and in-house criteria due to difference in results of MS and MSD.

The Blank Spike met requirements for all samples.

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements.

The Continuous Calibration met the requirements.

The Tuning criteria met requirements.



284 Sheffield Street, Mountainside, NJ 07092  
Phone: 908 789 8900 Fax: 908 789 8922

Samples MW-18B-56-040225, MW-17B-55-040225 was diluted due to high concentrations of compound Trichloroethene.

**E. Additional Comments:**

Trip Blank was not provided with this set of samples.

For Sample #01 & 04 at the time of fax Sequence Processed with wrong method after further review it is corrected in Hardcopy therefore fax and Hardcopy data will not match.

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

**F. Manual Integration Comments:**

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

---

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature\_\_\_\_\_

**DATA REPORTING QUALIFIERS- ORGANIC**

For reporting results, the following "Results Qualifiers" are used:

- Value** If the result is a value greater than or equal to the detection limit, report the value
- U** Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
- ND** Indicates the analyte was analyzed for, but not detected
- J** Indicates an estimated value. This flag is used:  
(1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.)  
(2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
- B** Indicates the analyte was found in the blank as well as the sample report as "12 B".
- E** Indicates the analyte's concentration exceeds the calibrated range of the instrument for that specific analysis.
- D** This flag identifies all compounds identified in an analysis at a secondary dilution factor.
- P** This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
- N** This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
- A** This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
- Q** Indicates the LCS did not meet the control limits requirements

# **ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092**

NEW JERSEY LAB ID#: 20012: NEW YORK LAB ID#: 11376

## **GC/MS VOA CONFORMANCE/NON-CONFORMANCE SUMMARY**

CHEMTECH PROJECT NUMBER: Q1711

MATRIX: Water

METHOD: 8260D

	NA	NO	YES
1. Chromatograms Labeled/Compounds Identified. (Field samples and Method Blanks)			✓
2. GC/MS Tuning Specifications BFB Meet Criteria (NOTE THAT THERE ARE DIFFERENT CRITERIA FOR NY ASP CLP, CLP AND NJ)			✓
3. GC/MS Tuning Frequency - Performed every 24 hours for 600 series and 12 hours for 8000 Series.			✓
4. GC/MS Calibration - Initial Calibration performed before sample analysis and continuing calibration performed within 24 hours of sample analysis for 600 series and 12 hours for 8000 series.			✓
5. GC/MS Calibration Requirements. The Initial Calibration met the requirements. The Continuous Calibration met the requirements.			✓
6. Blank Contamination - If yes, list compounds and concentrations in each blank:			✓
7. Surrogate Recoveries Meet Criteria  If not met, list those compounds and their recoveries which fall outside the acceptable ranges.			✓
8. Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria  If not met, list those compounds and their recoveries which fall outside the acceptable range.  The MS {Q1711-02MS} with File ID: VX045591.D recoveries met the requirements for all compounds except for cis-1,2-Dichloroethene[30%] this compound did not meet the NJDKQP criteria and in-house criteria, due to matrix interference. The MSD {Q1711-03MSD} with File ID: VX045577.D recoveries met the acceptable requirements except for cis-1,2-Dichloroethene[50%] this compound did not meet the NJDQP criteria and in-house criteria, due to matrix interference. The RPD for {Q1711-03MSD} with File ID: VX045577.D met criteria except for cis- 1,2-Dichloroethene[50%] this compound did not meet the NJDKQP criteria and in- house criteria due, to difference in results of MS and MSD.			✓
9. Internal Standard Area/Retention Time Shift Meet Criteria			✓

Comments:

# **ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092**

NEW JERSEY LAB ID#: 20012: NEW YORK LAB ID#: 11376

## **GC/MS VOA CONFORMANCE/NON-CONFORMANCE SUMMARY (CONTINUED)**

NA      NO      YES

10. Analysis Holding Time Met

If not met, list number of days exceeded for each sample:

### **ADDITIONAL COMMENTS:**

Samples MW-18B-56-040225, MW-17B-55-040225 was diluted due to high concentrations of compound Trichloroethene.

Trip Blank was not provided with this set of samples.

For Sample #01 & 04 at the time of fax Sequence Processed with wrong method after further review it is corrected in Hardcopy therefore fax and Hardcopy data will not match.

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

---

QA REVIEW

---

Date

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

## APPENDIX A

### QA REVIEW GENERAL DOCUMENTATION

Project #: Q1711

Completed

For thorough review, the report must have the following:

#### GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page) ✓

Check chain-of-custody for proper relinquish/return of samples ✓

Is the chain of custody signed and complete ✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts ✓

Collect information for each project id from server. Were all requirements followed ✓

#### COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page ✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody ✓

#### CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results ✓

Do requested analyses on Chain of Custody agree with the log-in page ✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody ✓

Were the samples received within hold time ✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle ✓

#### ANALYTICAL:

Was method requirement followed? ✓

Was client requirement followed? ✓

Does the case narrative summarize all QC failure? ✓

All runlogs and manual integration are reviewed for requirements ✓

All manual calculations and /or hand notations verified ✓

QA Review Signature: SOHIL JODHANI

Date: 04/10/2025

## LAB CHRONICLE

<b>OrderID:</b>	Q1711	<b>OrderDate:</b>	4/3/2025 10:00:00 AM
<b>Client:</b>	JACOBS Engineering Group, Inc.	<b>Project:</b>	Former Schlumberger STC PTC Site D3868221
<b>Contact:</b>	John Ynfante	<b>Location:</b>	I41,L21,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1711-01	<b>MW-18B-56-040225</b>	<b>Water</b>	VOCMS Group3	8260-Low	<b>04/02/25</b>		04/03/25	<b>04/02/25</b>
Q1711-04	<b>MW-17B-55-040225</b>	<b>Water</b>	VOCMS Group3	8260-Low	<b>04/02/25</b>		04/03/25	<b>04/02/25</b>
Q1711-07	<b>RMW-05B-89-040225</b>	<b>Water</b>	VOCMS Group3	8260-Low	<b>04/02/25</b>		04/03/25	<b>04/02/25</b>
Q1711-08	<b>EB01-040225</b>	<b>Water</b>	VOCMS Group3	8260-Low	<b>04/02/25</b>		04/03/25	<b>04/02/25</b>
Q1711-10	<b>TB01-040225</b>	<b>Water</b>	VOCMS Group3	8260-Low	<b>04/02/25</b>		04/03/25	<b>04/02/25</b>

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

### Hit Summary Sheet SW-846

**SDG No.:** Q1711  
**Client:** JACOBS Engineering Group, Inc.

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
<b>Client ID:</b>	<b>MW-18B-56-040225</b>							
Q1711-01	MW-18B-56-04022 Water		Vinyl Chloride	47.7	2.60		10.0	ug/L
Q1711-01	MW-18B-56-04022 Water		1,1-Dichloroethene	13.0	2.30		10.0	ug/L
Q1711-01	MW-18B-56-04022 Water		cis-1,2-Dichloroethene	850	1.90		10.0	ug/L
Q1711-01	MW-18B-56-04022 Water		Trichloroethene	370	0.93		10.0	ug/L
			<b>Total Voc :</b>	1280				
			<b>Total Concentration:</b>	1280				
<b>Client ID:</b>	<b>MW-17B-55-040225</b>							
Q1711-04	MW-17B-55-04022 Water		cis-1,2-Dichloroethene	2200	19.0		100	ug/L
Q1711-04	MW-17B-55-04022 Water		Trichloroethene	11400	9.30		100	ug/L
Q1711-04	MW-17B-55-04022 Water		Tetrachloroethene	110	23.0		100	ug/L
			<b>Total Voc :</b>	13700				
			<b>Total Concentration:</b>	13700				
<b>Client ID:</b>	<b>RMW-05B-89-040225</b>							
Q1711-07	RMW-05B-89-0402 Water		1,1-Dichloroethane	1.60	0.23		1.00	ug/L
Q1711-07	RMW-05B-89-0402 Water		cis-1,2-Dichloroethene	4.00	0.19		1.00	ug/L
			<b>Total Voc :</b>	5.60				
			<b>Total Concentration:</b>	5.60				



# QC SUMMARY

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

### Surrogate Summary

**SDG No.:** Q1711

**Client:** JACOBS Engineering Group, Inc.

**Analytical Method:** SW8260-Low

Lab Sample ID	Client ID	Parameter	Spike	Result	RecoveryQual	Limits	
						Low	High
Q1711-01	MW-18B-56-040225	1,2-Dichloroethane-d4	50	53.4	107	70 (74)	130 (125)
		Dibromofluoromethane	50	51.5	103	70 (75)	130 (124)
		Toluene-d8	50	51.2	102	70 (86)	130 (113)
		4-Bromofluorobenzene	50	49.1	98	70 (77)	130 (121)
Q1711-02MS	MW-18B-56-040225MS	1,2-Dichloroethane-d4	50	53.2	106	70 (74)	130 (125)
		Dibromofluoromethane	50	50.8	102	70 (75)	130 (124)
		Toluene-d8	50	50.8	102	70 (86)	130 (113)
		4-Bromofluorobenzene	50	53.1	106	70 (77)	130 (121)
Q1711-03MSD	MW-18B-56-040225MSD	1,2-Dichloroethane-d4	50	46.9	94	70 (74)	130 (125)
		Dibromofluoromethane	50	44.8	90	70 (75)	130 (124)
		Toluene-d8	50	44.8	90	70 (86)	130 (113)
		4-Bromofluorobenzene	50	46.0	92	70 (77)	130 (121)
Q1711-04	MW-17B-55-040225	1,2-Dichloroethane-d4	50	54.8	110	70 (74)	130 (125)
		Dibromofluoromethane	50	52.2	104	70 (75)	130 (124)
		Toluene-d8	50	50.7	101	70 (86)	130 (113)
		4-Bromofluorobenzene	50	46.9	94	70 (77)	130 (121)
Q1711-07	RMW-05B-89-040225	1,2-Dichloroethane-d4	50	55.2	110	70 (74)	130 (125)
		Dibromofluoromethane	50	52.0	104	70 (75)	130 (124)
		Toluene-d8	50	50.6	101	70 (86)	130 (113)
		4-Bromofluorobenzene	50	50.6	101	70 (77)	130 (121)
Q1711-08	EB01-040225	1,2-Dichloroethane-d4	50	53.4	107	70 (74)	130 (125)
		Dibromofluoromethane	50	51.0	102	70 (75)	130 (124)
		Toluene-d8	50	50.9	102	70 (86)	130 (113)
		4-Bromofluorobenzene	50	49.8	100	70 (77)	130 (121)
Q1711-10	TB01-040225	1,2-Dichloroethane-d4	50	53.9	108	70 (74)	130 (125)
		Dibromofluoromethane	50	52.0	104	70 (75)	130 (124)
		Toluene-d8	50	51.0	102	70 (86)	130 (113)
		4-Bromofluorobenzene	50	51.0	102	70 (77)	130 (121)
VX0403WBL01	VX0403WBL01	1,2-Dichloroethane-d4	50	53.2	106	70 (74)	130 (125)
		Dibromofluoromethane	50	52.6	105	70 (75)	130 (124)
		Toluene-d8	50	50.9	102	70 (86)	130 (113)
		4-Bromofluorobenzene	50	51.1	102	70 (77)	130 (121)
VX0403WBS01	VX0403WBS01	1,2-Dichloroethane-d4	50	48.8	98	70 (74)	130 (125)
		Dibromofluoromethane	50	48.5	97	70 (75)	130 (124)
		Toluene-d8	50	48.5	97	70 (86)	130 (113)
		4-Bromofluorobenzene	50	49.0	98	70 (77)	130 (121)
VX0404WBL01	VX0404WBL01	1,2-Dichloroethane-d4	50	54.8	110	70 (74)	130 (125)
		Dibromofluoromethane	50	52.0	104	70 (75)	130 (124)
		Toluene-d8	50	50.8	102	70 (86)	130 (113)
		4-Bromofluorobenzene	50	49.5	99	70 (77)	130 (121)
VX0404WBS01	VX0404WBS01	1,2-Dichloroethane-d4	50	52.9	106	70 (74)	130 (125)
		Dibromofluoromethane	50	53.3	107	70 (75)	130 (124)
		Toluene-d8	50	53.2	106	70 (86)	130 (113)
		4-Bromofluorobenzene	50	53.2	106	70 (77)	130 (121)

( ) = LABORATORY INHOUSE LIMIT

### Matrix Spike/Matrix Spike Duplicate Summary

**SW-846**

**SDG No.:** Q1711

**Client:** JACOBS Engineering Group, Inc.

**Analytical Method:** SW8260-Low

Parameter	Spike	Sample Result	Result	Units	Rec		RPD Qual	Limits		RPD
					Rec	Qual		Low	High	
<b>Lab Sample ID :</b>	<b>Q1711-02MS</b>	<b>Client Sample ID :</b>	<b>MW-18B-56-040225MS</b>		<b>Datafile :</b>		<b>VX045591.D</b>			
Vinyl chloride	500	47.7	530	ug/L	96			70 (69)	130 (125)	
1,1-Dichloroethene	500	13.0	500	ug/L	97			70 (53)	130 (162)	
1,1-Dichloroethane	500	0	510	ug/L	102			70 (78)	130 (122)	
cis-1,2-Dichloroethene	500	850	1000	ug/L	30	*		70 (82)	130 (124)	
1,1,1-Trichloroethane	500	0	510	ug/L	102			70 (83)	130 (117)	
Benzene	500	0	500	ug/L	100			70 (81)	130 (128)	
1,2-Dichloroethane	500	0	510	ug/L	102			70 (76)	130 (120)	
Trichloroethene	500	370	740	ug/L	74			70 (28)	130 (175)	
1,1,2-Trichloroethane	500	0	510	ug/L	102			70 (27)	130 (175)	
Tetrachloroethene	500	0	460	ug/L	92			70 (48)	130 (153)	

( ) = LABORATORY INHOUSE LIMIT

### Matrix Spike/Matrix Spike Duplicate Summary

**SW-846**

**SDG No.:** Q1711

**Client:** JACOBS Engineering Group, Inc.

**Analytical Method:** SW8260-Low

Parameter	Spike	Sample Result	Result	Units	Rec		RPD Qual	Limits			RPD
					Rec	Qual		Low	High		
<b>Lab Sample ID :</b>	<b>Q1711-03MSD</b>	<b>Client Sample ID :</b>	<b>MW-18B-56-040225MSD</b>					<b>Datafile :</b>	<b>VX045577.D</b>		
Vinyl chloride	500	47.7	480	ug/L	86		11	70 (69)	130 (125)	20 (20)	
1,1-Dichloroethene	500	13.0	430	ug/L	83		16	70 (53)	130 (162)	20 (20)	
1,1-Dichloroethane	500	0	420	ug/L	84		19	70 (78)	130 (122)	20 (20)	
cis-1,2-Dichloroethene	500	850	1100	ug/L	50	*	50	70 (82)	130 (124)	20 (20)	
1,1,1-Trichloroethane	500	0	420	ug/L	84		19	70 (83)	130 (117)	20 (20)	
Benzene	500	0	420	ug/L	84		17	70 (81)	130 (128)	20 (20)	
1,2-Dichloroethane	500	0	430	ug/L	86		17	70 (76)	130 (120)	20 (20)	
Trichloroethene	500	370	740	ug/L	74		0	70 (28)	130 (175)	20 (20)	
1,1,2-Trichloroethane	500	0	430	ug/L	86		17	70 (27)	130 (175)	20 (20)	
Tetrachloroethene	500	0	400	ug/L	80		14	70 (48)	130 (153)	20 (20)	

( ) = LABORATORY INHOUSE LIMIT

**Laboratory Control Sample/Laboratory Control Sample Duplicate Summary**

**SW-846**

**SDG No.:** Q1711

**Client:** JACOBS Engineering Group, Inc.

**Analytical Method:** SW8260-Low

**Datafile :** VX045563.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		RPD
								Low	High	
VX0403WBS01	Vinyl chloride	20	18.9	ug/L	95			70 (65)	130 (117)	
	1,1-Dichloroethene	20	18.8	ug/L	94			70 (74)	130 (110)	
	1,1-Dichloroethane	20	18.7	ug/L	94			70 (78)	130 (112)	
	cis-1,2-Dichloroethene	20	18.2	ug/L	91			70 (77)	130 (110)	
	1,1,1-Trichloroethane	20	18.4	ug/L	92			70 (80)	130 (108)	
	Benzene	20	18.7	ug/L	94			70 (82)	130 (109)	
	1,2-Dichloroethane	20	19.6	ug/L	98			70 (80)	130 (115)	
	Trichloroethene	20	18.5	ug/L	93			70 (77)	130 (113)	
	1,1,2-Trichloroethane	20	19.1	ug/L	96			70 (83)	130 (112)	
	Tetrachloroethene	20	18.4	ug/L	92			70 (67)	130 (123)	

( ) = LABORATORY INHOUSE LIMIT

**Laboratory Control Sample/Laboratory Control Sample Duplicate Summary**

**SW-846**

**SDG No.:** Q1711

**Client:** JACOBS Engineering Group, Inc.

**Analytical Method:** SW8260-Low

**Datafile :** VX045589.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		RPD
								Low	High	
VX0404WBS01	Vinyl chloride	20	19.6	ug/L	98			70 (65)	130 (117)	
	1,1-Dichloroethene	20	19.4	ug/L	97			70 (74)	130 (110)	
	1,1-Dichloroethane	20	19.5	ug/L	98			70 (78)	130 (112)	
	cis-1,2-Dichloroethene	20	19.2	ug/L	96			70 (77)	130 (110)	
	1,1,1-Trichloroethane	20	19.7	ug/L	99			70 (80)	130 (108)	
	Benzene	20	19.9	ug/L	100			70 (82)	130 (109)	
	1,2-Dichloroethane	20	20.4	ug/L	102			70 (80)	130 (115)	
	Trichloroethene	20	19.2	ug/L	96			70 (77)	130 (113)	
	1,1,2-Trichloroethane	20	20.5	ug/L	103			70 (83)	130 (112)	
	Tetrachloroethene	20	19.6	ug/L	98			70 (67)	130 (123)	

( ) = LABORATORY INHOUSE LIMIT

VOLATILE METHOD BLANK SUMMARY

EPA SAMPLE NO.

**VX0403WBL01**

Lab Name: CHEMTECH

Contract: JACO05

Lab Code: CHEM Case No.: Q1711

SAS No.: Q1711 SDG NO.: Q1711

Lab File ID: VX045561.D

Lab Sample ID: VX0403WBL01

Date Analyzed: 04/03/2025

Time Analyzed: 11:21

GC Column: DB-624UI ID: 0.18 (mm)

Heated Purge: (Y/N) N

Instrument ID: MSVOA\_X

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VX0403WBS01	VX0403WBS01	VX045563.D	04/03/2025
RMW-05B-89-040225	Q1711-07	VX045568.D	04/03/2025
MW-17B-55-040225	Q1711-04	VX045569.D	04/03/2025
TB01-040225	Q1711-10	VX045571.D	04/03/2025
EB01-040225	Q1711-08	VX045572.D	04/03/2025
MW-18B-56-040225	Q1711-01	VX045575.D	04/03/2025
MW-18B-56-040225MSD	Q1711-03MSD	VX045577.D	04/03/2025

COMMENTS:

---

## VOLATILE METHOD BLANK SUMMARY

EPA SAMPLE NO.

VX0404WBL01

Lab Name: CHEMTECHContract: JACO05Lab Code: CHEM Case No.: Q1711SAS No.: Q1711 SDG NO.: Q1711Lab File ID: VX045588.DLab Sample ID: VX0404WBL01Date Analyzed: 04/04/2025Time Analyzed: 10:51GC Column: DB-624UI ID: 0.18 (mm)Heated Purge: (Y/N) NInstrument ID: MSVOA\_X

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VX0404WBS01	VX0404WBS01	VX045589.D	04/04/2025
MW-18B-56-040225MS	Q1711-02MS	VX045591.D	04/04/2025

COMMENTS:

---

---



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
BROMOFLUOROBENZENE (BFB)

Lab Name:	CHEMTECH	Contract:	JAC005
Lab Code:	CHEM	Case No.:	Q1711
Lab File ID:	VX045524.D	SAS No.:	Q1711
Instrument ID:	MSVOA_X	BFB Injection Date:	04/01/2025
GC Column:	DB-624UI ID: 0.18 (mm)	BFB Injection Time:	16:15
		Heated Purge:	Y/N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	23.6
75	30.0 - 60.0% of mass 95	58.2
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.3
173	Less than 2.0% of mass 174	0.8 ( 1.2 ) 1
174	50.0 - 100.0% of mass 95	66.8
175	5.0 - 9.0% of mass 174	5.2 ( 7.8 ) 1
176	95.0 - 101.0% of mass 174	65.3 ( 97.8 ) 1
177	5.0 - 9.0% of mass 176	4.4 ( 6.8 ) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDICC001	VSTDICC001	VX045525.D	04/01/2025	17:06
VSTDICC005	VSTDICC005	VX045526.D	04/01/2025	17:29
VSTDICC020	VSTDICC020	VX045527.D	04/01/2025	17:52
VSTDICCC050	VSTDICCC050	VX045528.D	04/01/2025	18:15
VSTDICC100	VSTDICC100	VX045529.D	04/01/2025	18:38
VSTDICC150	VSTDICC150	VX045530.D	04/01/2025	19:02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
BROMOFLUOROBENZENE (BFB)

Lab Name:	CHEMTECH	Contract:	JAC005
Lab Code:	CHEM	Case No.:	Q1711
Lab File ID:	VX045558.D	SAS No.:	Q1711
Instrument ID:	MSVOA_X	BFB Injection Date:	04/03/2025
GC Column:	DB-624UI ID: 0.18 (mm)	BFB Injection Time:	10:01
		Heated Purge:	Y/N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	22.2
75	30.0 - 60.0% of mass 95	56.7
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.2
173	Less than 2.0% of mass 174	0.9 ( 1.3 ) 1
174	50.0 - 100.0% of mass 95	67.5
175	5.0 - 9.0% of mass 174	5.1 ( 7.5 ) 1
176	95.0 - 101.0% of mass 174	65.9 ( 97.6 ) 1
177	5.0 - 9.0% of mass 176	4 ( 6.1 ) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC050	VSTDCCC050	VX045559.D	04/03/2025	10:30
VX0403WBL01	VX0403WBL01	VX045561.D	04/03/2025	11:21
VX0403WBS01	VX0403WBS01	VX045563.D	04/03/2025	12:08
RMW-05B-89-040225	Q1711-07	VX045568.D	04/03/2025	14:04
MW-17B-55-040225	Q1711-04	VX045569.D	04/03/2025	14:27
TB01-040225	Q1711-10	VX045571.D	04/03/2025	15:14
EB01-040225	Q1711-08	VX045572.D	04/03/2025	15:37
MW-18B-56-040225	Q1711-01	VX045575.D	04/03/2025	16:47
MW-18B-56-040225MSD	Q1711-03MSD	VX045577.D	04/03/2025	17:33



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
BROMOFLUOROBENZENE (BFB)

Lab Name:	CHEMTECH	Contract:	JAC005
Lab Code:	CHEM	Case No.:	Q1711
Lab File ID:	VX045585.D	SAS No.:	Q1711
Instrument ID:	MSVOA_X	BFB Injection Date:	04/04/2025
GC Column:	DB-624UI ID: 0.18 (mm)	BFB Injection Time:	09:31
		Heated Purge:	Y/N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	25
75	30.0 - 60.0% of mass 95	57.7
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	7.2
173	Less than 2.0% of mass 174	0.9 ( 1.4 ) 1
174	50.0 - 100.0% of mass 95	68.1
175	5.0 - 9.0% of mass 174	5.7 ( 8.3 ) 1
176	95.0 - 101.0% of mass 174	65.8 ( 96.6 ) 1
177	5.0 - 9.0% of mass 176	4.9 ( 7.5 ) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC050	VSTDCCC050	VX045586.D	04/04/2025	10:00
VX0404WBL01	VX0404WBL01	VX045588.D	04/04/2025	10:51
VX0404WBS01	VX0404WBS01	VX045589.D	04/04/2025	11:14
MW-18B-56-040225MS	Q1711-02MS	VX045591.D	04/04/2025	12:04

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: JAC005  
 Lab Code: CHEM Case No.: Q1711 SAS No.: Q1711 SDG NO.: Q1711  
 Lab File ID: VX045559.D Date Analyzed: 04/03/2025  
 Instrument ID: MSVOA\_X Time Analyzed: 10:30  
 GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	95221	5.54	162684	6.76	143783	10.05
	190442	6.044	325368	7.257	287566	10.549
	47610.5	5.044	81342	6.257	71891.5	9.549
EPA SAMPLE NO.						
MW-18B-56-040225	64116	5.55	121192	6.76	112037	10.06
MW-18B-56-040225MSD	69182	5.55	124452	6.76	109108	10.06
MW-17B-55-040225	63215	5.55	122949	6.76	111016	10.06
RMW-05B-89-040225	63845	5.55	125144	6.76	116415	10.05
EB01-040225	63287	5.54	123377	6.76	114226	10.05
TB01-040225	66937	5.54	129076	6.76	121728	10.05
VX0403WBL01	66309	5.55	126206	6.76	118586	10.05
VX0403WBS01	95034	5.54	168178	6.76	149052	10.05

IS1 = Pentafluorobenzene

IS2 = 1,4-Difluorobenzene

IS3 = Chlorobenzene-d5

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name:	CHEMTECH	Contract:	JACO05
Lab Code:	CHEM	SAS No.:	Q1711
Case No.:	Q1711	SDG NO.:	Q1711
Lab File ID:	VX045559.D	Date Analyzed:	04/03/2025
Instrument ID:	MSVOA_X	Time Analyzed:	10:30
GC Column:	DB-624UI	ID:	0.18 (mm)
		Heated Purge:	(Y/N) <u>N</u>

	IS4 AREA #	RT #				
12 HOUR STD	66270	12.018				
	132540	12.518				
	33135	11.518				
EPA SAMPLE NO.						
MW-18B-56-040225	43792	12.02				
MW-18B-56-040225MSD	51026	12.02				
MW-17B-55-040225	41790	12.02				
RMW-05B-89-040225	47044	12.02				
EB01-040225	46598	12.02				
TB01-040225	49430	12.02				
VX0403WBL01	50130	12.02				
VX0403WBS01	68919	12.02				

IS4 = 1,4-Dichlorobenzene-d4

AREA UPPER LIMIT = +100% of internal standard area  
 AREA LOWER LIMIT = -50% of internal standard area  
 RT UPPER LIMIT = +0.50 minutes of internal standard RT  
 RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: JAC005  
 Lab Code: CHEM Case No.: Q1711 SAS No.: Q1711 SDG NO.: Q1711  
 Lab File ID: VX045586.D Date Analyzed: 04/04/2025  
 Instrument ID: MSVOA\_X Time Analyzed: 10:00  
 GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	96707	5.54	163287	6.75	142048	10.05
UPPER LIMIT	193414	6.038	326574	7.251	284096	10.549
LOWER LIMIT	48353.5	5.038	81643.5	6.251	71024	9.549
EPA SAMPLE NO.						
MW-18B-56-040225MS	84872	5.55	154383	6.76	136696	10.05
VX0404WBL01	66301	5.54	128686	6.76	118182	10.06
VX0404WBS01	95127	5.55	168453	6.76	151744	10.05

IS1 = Pentafluorobenzene

IS2 = 1,4-Difluorobenzene

IS3 = Chlorobenzene-d5

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name:	CHEMTECH	Contract:	JACO05		
Lab Code:	<u>CHEM</u>	SAS No.:	<u>Q1711</u>	SDG NO.:	<u>Q1711</u>
Lab File ID:	<u>VX045586.D</u>	Date Analyzed:	<u>04/04/2025</u>		
Instrument ID:	<u>MSVOA_X</u>	Time Analyzed:	<u>10:00</u>		
GC Column:	<u>DB-624UI</u>	ID:	<u>0.18</u> (mm)	Heated Purge:	(Y/N) <u>N</u>

	IS4 AREA #	RT #				
12 HOUR STD	67379	12.018				
UPPER LIMIT	134758	12.518				
LOWER LIMIT	33689.5	11.518				
EPA SAMPLE NO.						
MW-18B-56-040225MS	64924	12.02				
VX0404WBL01	46025	12.02				
VX0404WBS01	66584	12.02				

IS4 = 1,4-Dichlorobenzene-d4

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.



# SAMPLE

# DATA

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	04/02/25
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	04/02/25
Client Sample ID:	MW-18B-56-040225			SDG No.:	Q1711
Lab Sample ID:	Q1711-01			Matrix:	Water
Analytical Method:	SW8260			% Solid:	0
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045575.D	10		04/03/25 16:47	VX040325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	47.7		2.60	10.0	ug/L
75-35-4	1,1-Dichloroethene	13.0		2.30	10.0	ug/L
75-34-3	1,1-Dichloroethane	2.30	U	2.30	10.0	ug/L
156-59-2	cis-1,2-Dichloroethene	850		1.90	10.0	ug/L
71-55-6	1,1,1-Trichloroethane	2.00	U	2.00	10.0	ug/L
71-43-2	Benzene	1.50	U	1.50	10.0	ug/L
107-06-2	1,2-Dichloroethane	2.20	U	2.20	10.0	ug/L
79-01-6	Trichloroethene	370		0.93	10.0	ug/L
79-00-5	1,1,2-Trichloroethane	2.10	U	2.10	10.0	ug/L
127-18-4	Tetrachloroethene	2.30	U	2.30	10.0	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	53.4		70 (74) - 130 (125)	107%	SPK: 50
1868-53-7	Dibromofluoromethane	51.5		70 (75) - 130 (124)	103%	SPK: 50
2037-26-5	Toluene-d8	51.2		70 (86) - 130 (113)	102%	SPK: 50
460-00-4	4-Bromofluorobenzene	49.1		70 (77) - 130 (121)	98%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	64100	5.55			
540-36-3	1,4-Difluorobenzene	121000	6.757			
3114-55-4	Chlorobenzene-d5	112000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	43800	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045575.D  
 Acq On : 03 Apr 2025 16:47  
 Operator : JC/MD  
 Sample : Q1711-01 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-18B-56-040225

Quant Time: Apr 04 01:25:19 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	64116	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	121192	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	112037	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	43792	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	62586	53.378	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	106.760%	
35) Dibromofluoromethane	5.379	113	44291	51.510	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	103.020%	
50) Toluene-d8	8.647	98	153765	51.234	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	102.460%	
62) 4-Bromofluorobenzene	11.079	95	53724	49.144	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	98.280%	
<b>Target Compounds</b>						
				Qvalue		
4) Vinyl Chloride	1.374	62	4299	4.769	ug/l	96
12) 1,1-Dichloroethene	2.312	96	997	1.295	ug/l	88
16) Acetone	2.379	43	5722	11.885	ug/l	95
27) cis-1,2-Dichloroethene	4.483	96	81070	84.620	ug/l	90
29) Tetrahydrofuran	5.019	42	5635	12.332	ug/l	96
44) Trichloroethene	7.122	130	30963	36.740	ug/l	95




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045575.D  
 Acq On : 03 Apr 2025 16:47  
 Operator : JC/MD  
 Sample : Q1711-01 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-18B-56-040225





Quant Time: Apr 04 01:25:19 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

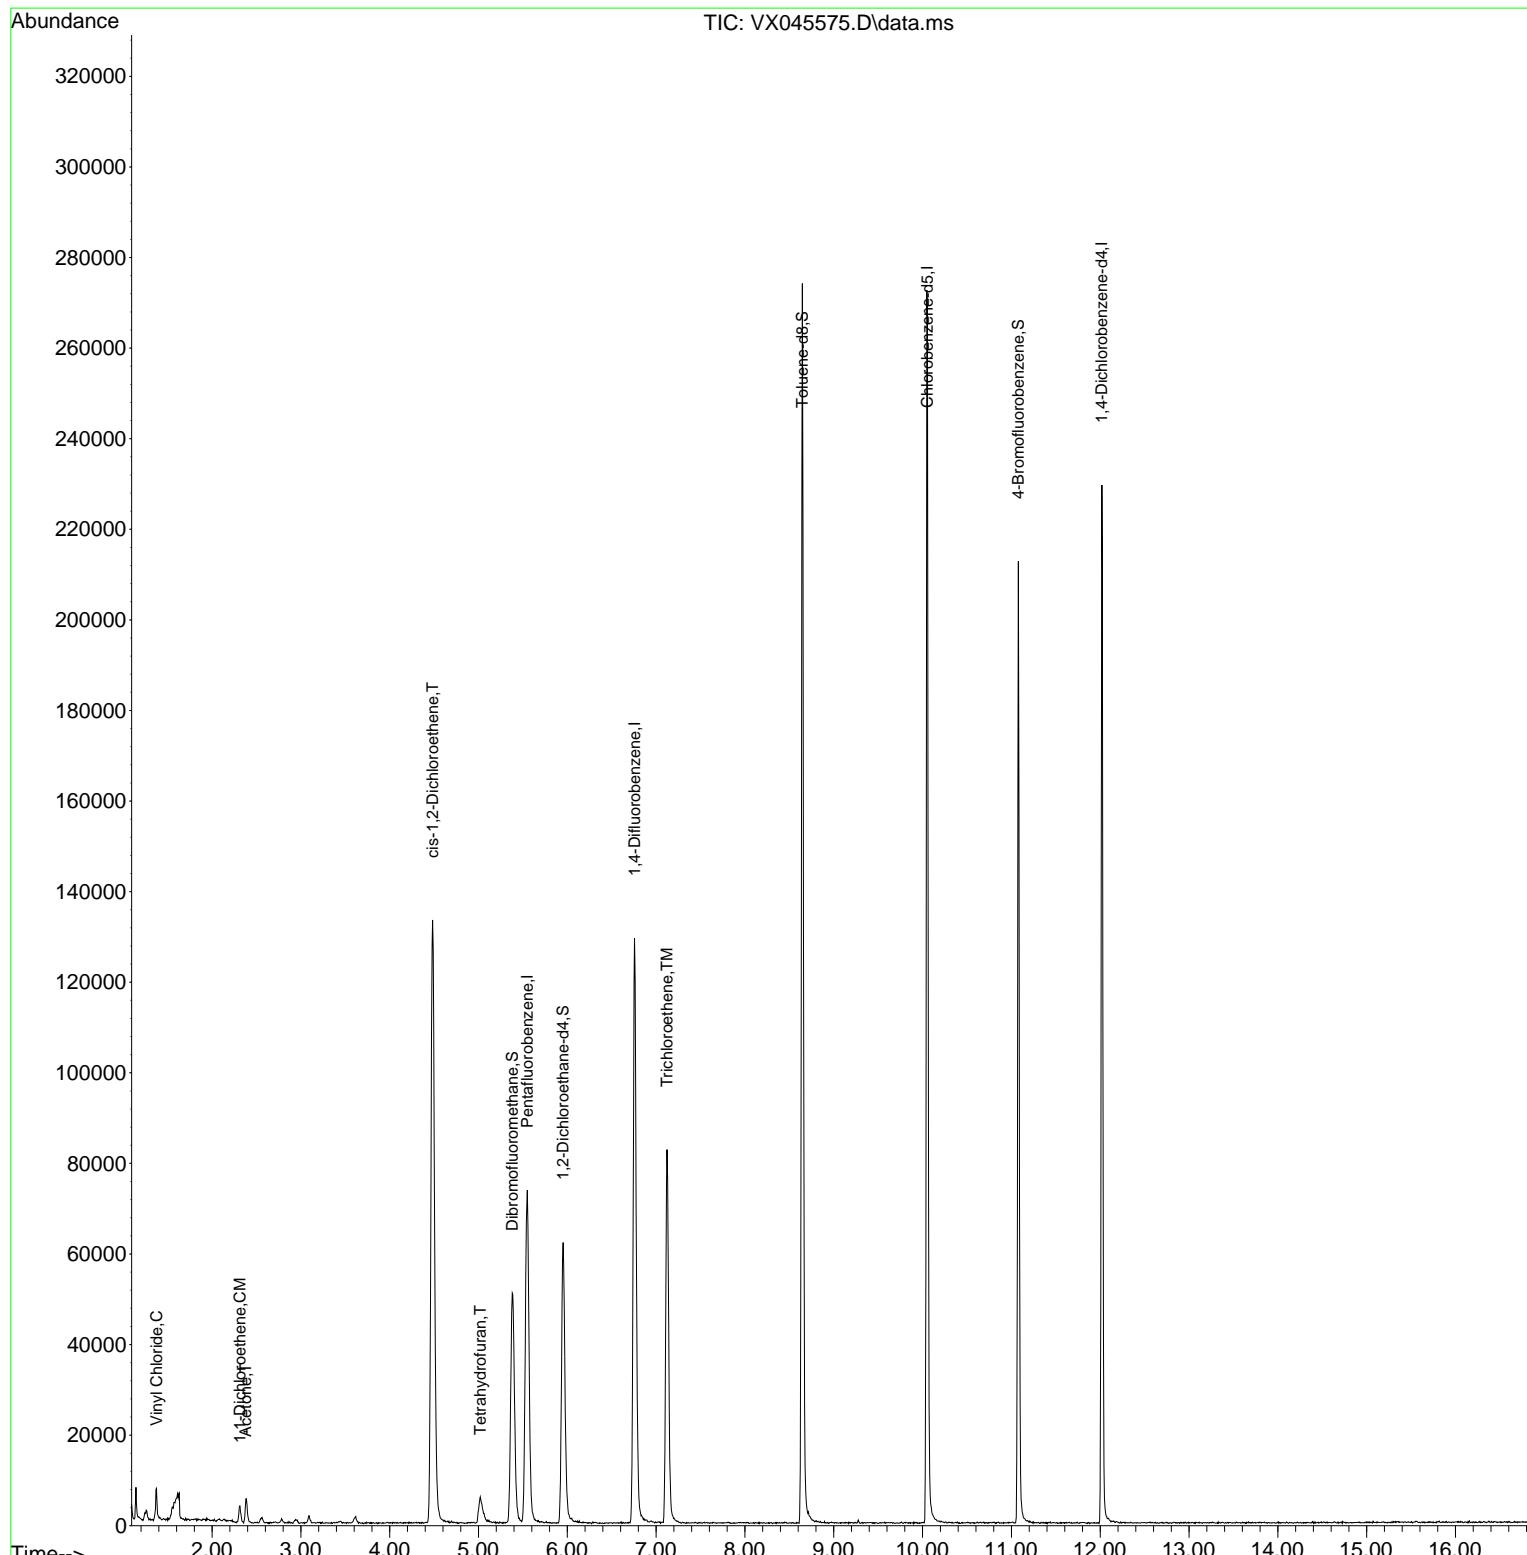

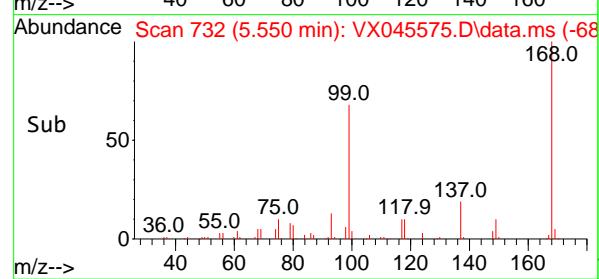


#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Instrument: MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX045575.D  
ClientSampleId :  
Acq: 03 Apr 2025 16:47 MW-18B-56-040225




Tgt Ion:168 Resp: 64116  
Ion Ratio Lower Upper  
168 100  
99 68.4 52.3 78.5

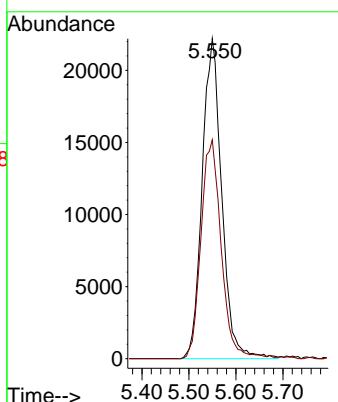

#4  
Vinyl Chloride  
Concen: 4.769 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. -0.000 min  
Lab File: VX045575.D  
Acq: 03 Apr 2025 16:47

Tgt Ion: 62 Resp: 4299  
Ion Ratio Lower Upper  
62 100  
64 29.4 25.5 38.3

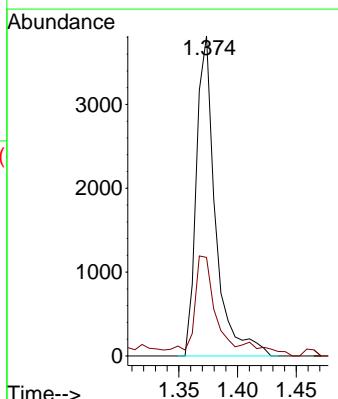



#12

1,1-Dichloroethene

Concen: 1.295 ug/l

RT: 2.312 min Scan# 2

Instrument:

Delta R.T. -0.000 min

MSVOA\_X

Lab File: VX045575.D

ClientSampleId :

Acq: 03 Apr 2025 16:47

MW-18B-56-040225





Tgt Ion: 96 Resp: 997

Ion Ratio Lower Upper

96 100

61 204.6 145.7 218.5

98 62.2 51.6 77.4



#16

Acetone

Concen: 11.885 ug/l

RT: 2.379 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX045575.D


Acq: 03 Apr 2025 16:47




Tgt Ion: 43 Resp: 5722

Ion Ratio Lower Upper

43 100

58 25.1 22.3 33.5




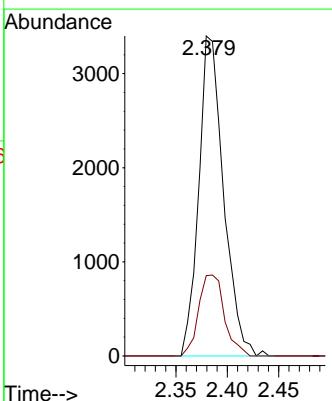




#27  
cis-1,2-Dichloroethene  
Concen: 84.620 ug/l  
RT: 4.483 min Scan# 5  
Delta R.T. -0.000 min  
Lab File: VX045575.D  
Acq: 03 Apr 2025 16:47


Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225




Tgt Ion: 96 Resp: 81070  
Ion Ratio Lower Upper  
96 100  
61 139.0 0.0 313.2  
98 63.5 0.0 126.4

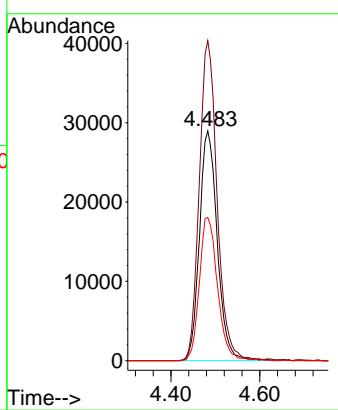

#29  
Tetrahydrofuran  
Concen: 12.332 ug/l  
RT: 5.019 min Scan# 645  
Delta R.T. 0.018 min  
Lab File: VX045575.D  
Acq: 03 Apr 2025 16:47

Tgt Ion: 42 Resp: 5635  
Ion Ratio Lower Upper  
42 100  
72 39.4 33.4 50.0  
71 36.8 31.4 47.0

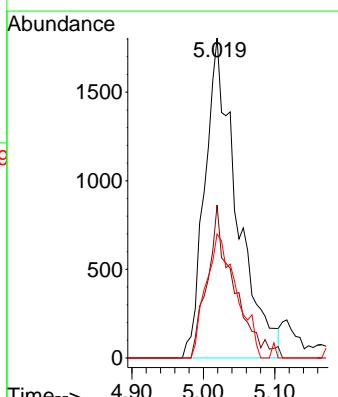



#33

1,2-Dichloroethane-d4

Concen: 53.378 ug/l

RT: 5.952 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX045575.D

Acq: 03 Apr 2025 16:47

Instrument:

MSVOA\_X

ClientSampleId :





MW-18B-56-040225

Tgt Ion: 65 Resp: 62586

Ion Ratio Lower Upper

65 100

67 48.6 0.0 99.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX045575.D

Acq: 03 Apr 2025 16:47


Tgt Ion: 114 Resp: 121192




Ion Ratio Lower Upper

114 100

63 24.4 0.0 46.8

88 17.0 0.0 35.4

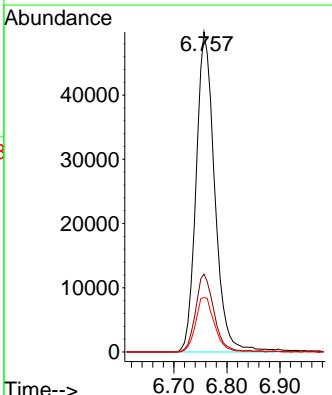



#35

Dibromofluoromethane

Concen: 51.510 ug/l

RT: 5.379 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX045575.D

Acq: 03 Apr 2025 16:47

Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225





Tgt Ion:113 Resp: 44291

Ion Ratio Lower Upper

113 100

111 103.8 81.8 122.6

192 16.6 13.8 20.6

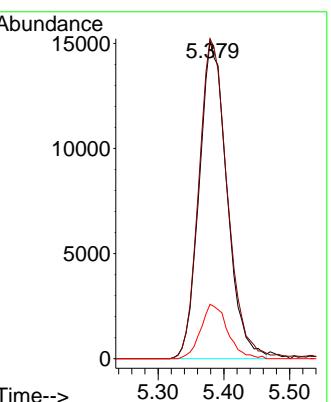

#44

Trichloroethene

Concen: 36.740 ug/l

RT: 7.122 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX045575.D


Acq: 03 Apr 2025 16:47


Tgt Ion:130 Resp: 30963

Ion Ratio Lower Upper


130 100

95 105.8 0.0 202.0

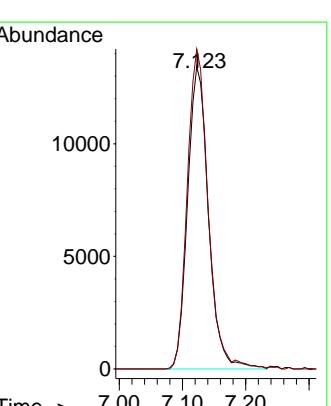




Abundance Scan 1240 (8.647 min): VX045575.D\data.ms

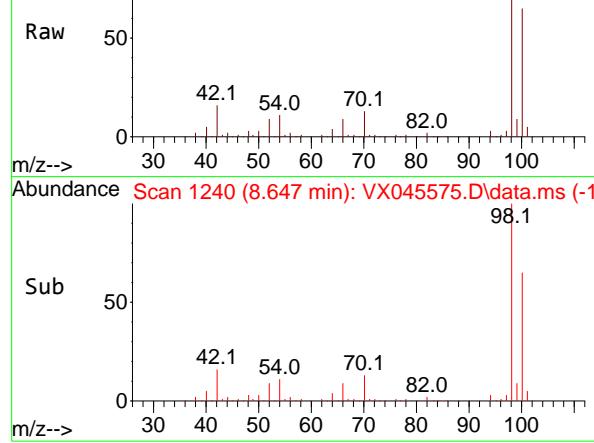

Abundance Scan 1240 (8.647 min): VX045575.D\data.ms (-1)

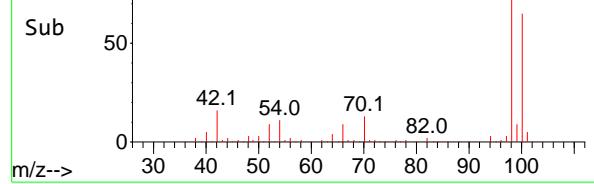

#50  
Toluene-d8  
Concen: 51.234 ug/l  
RT: 8.647 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045575.D  
Acq: 03 Apr 2025 16:47



Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225

Tgt Ion: 98 Resp: 153765


Ion Ratio Lower Upper

98 100


100 64.9 52.2 78.4

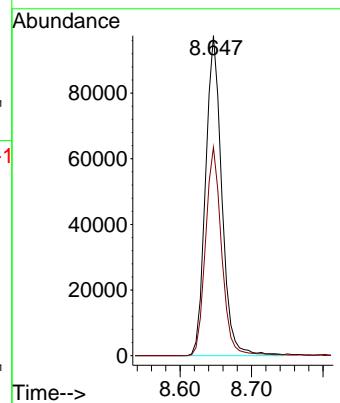

Abundance Scan 1639 (11.079 min): VX045575.D\data.ms

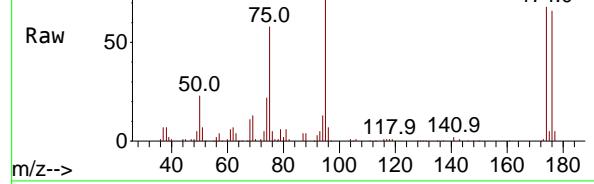

Abundance Scan 1639 (11.079 min): VX045575.D\data.ms (-1)

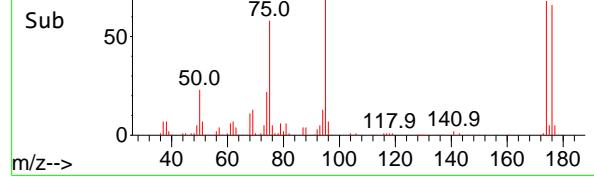

#62  
4-Bromofluorobenzene  
Concen: 49.144 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX045575.D  
Acq: 03 Apr 2025 16:47


Tgt Ion: 95 Resp: 53724


Ion Ratio Lower Upper

95 100

174 68.8 0.0 135.8



176 65.5 0.0 131.4

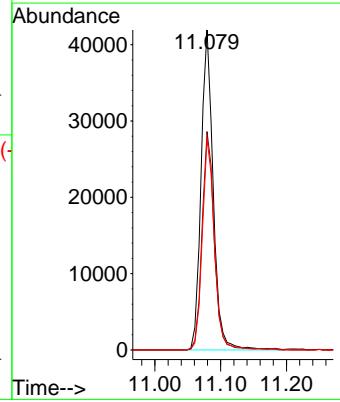

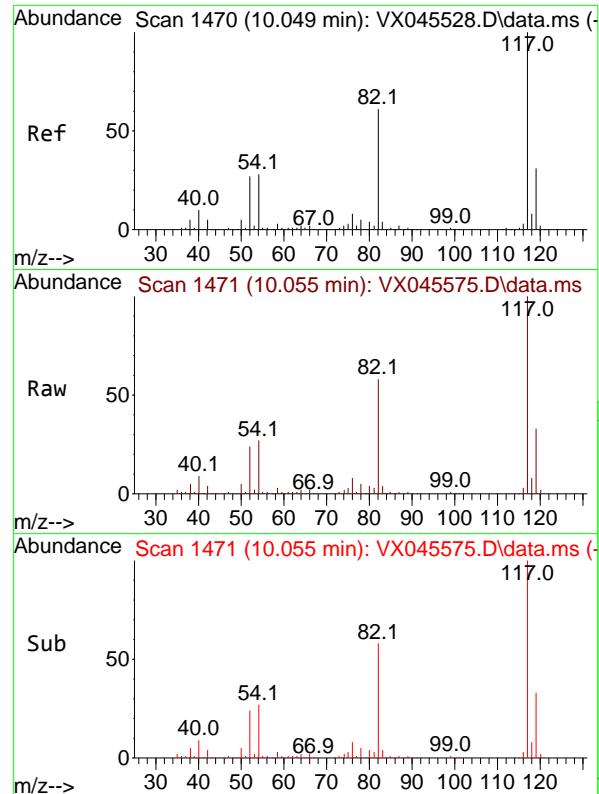


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX045575.D  
ClientSampleId : MW-18B-56-040225  
Acq: 03 Apr 2025 16:47

Tgt Ion:117 Resp: 112037  
Ion Ratio Lower Upper  
117 100  
82 58.3 49.2 73.8  
119 32.6 25.1 37.7

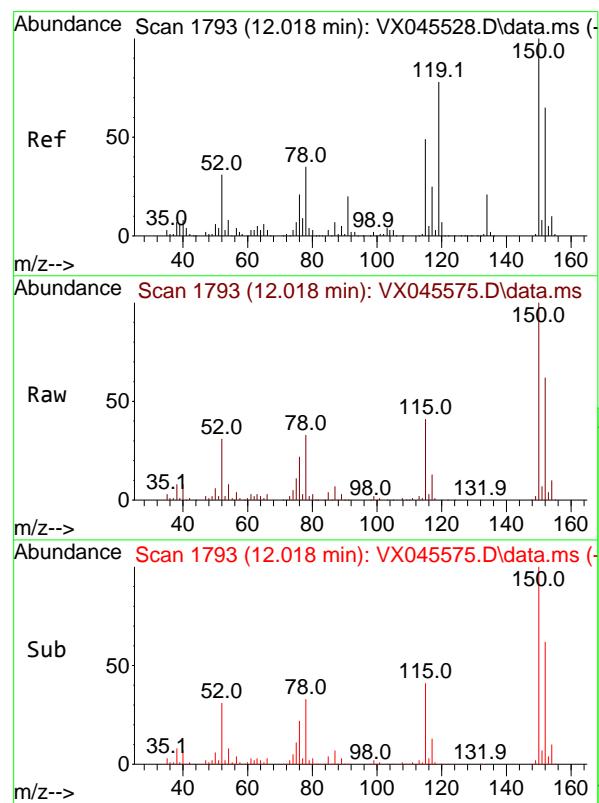

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. -0.000 min  
Lab File: VX045575.D  
Acq: 03 Apr 2025 16:47

Tgt Ion:152 Resp: 43792  
Ion Ratio Lower Upper  
152 100  
115 65.5 46.9 140.7  
150 158.9 0.0 349.4





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	04/02/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	04/02/25	
Client Sample ID:	MW-17B-55-040225			SDG No.:	Q1711	
Lab Sample ID:	Q1711-04			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045569.D	100		04/03/25 14:27	VX040325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	26.0	U	26.0	100	ug/L
75-35-4	1,1-Dichloroethene	23.0	U	23.0	100	ug/L
75-34-3	1,1-Dichloroethane	23.0	U	23.0	100	ug/L
156-59-2	cis-1,2-Dichloroethene	2200		19.0	100	ug/L
71-55-6	1,1,1-Trichloroethane	20.0	U	20.0	100	ug/L
71-43-2	Benzene	15.0	U	15.0	100	ug/L
107-06-2	1,2-Dichloroethane	22.0	U	22.0	100	ug/L
79-01-6	Trichloroethene	11400		9.30	100	ug/L
79-00-5	1,1,2-Trichloroethane	21.0	U	21.0	100	ug/L
127-18-4	Tetrachloroethene	110		23.0	100	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	54.8		70 (74) - 130 (125)	110%	SPK: 50
1868-53-7	Dibromofluoromethane	52.2		70 (75) - 130 (124)	104%	SPK: 50
2037-26-5	Toluene-d8	50.7		70 (86) - 130 (113)	101%	SPK: 50
460-00-4	4-Bromofluorobenzene	46.9		70 (77) - 130 (121)	94%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	63200	5.55			
540-36-3	1,4-Difluorobenzene	123000	6.757			
3114-55-4	Chlorobenzene-d5	111000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	41800	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045569.D  
 Acq On : 03 Apr 2025 14:27  
 Operator : JC/MD  
 Sample : Q1711-04 100X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**MW-17B-55-040225**

Quant Time: Apr 04 01:22:53 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	63215	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	122949	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	111016	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	41790	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	63364	54.811	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	109.620%	
35) Dibromofluoromethane	5.379	113	45550	52.217	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	104.440%	
50) Toluene-d8	8.647	98	154375	50.702	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	101.400%	
62) 4-Bromofluorobenzene	11.079	95	51995	46.882	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	93.760%	
<b>Target Compounds</b>						
				Qvalue		
9) 1,1,2-Trichlorotrifluo...	2.325	101	1122	1.445	ug/l	# 83
27) cis-1,2-Dichloroethene	4.483	96	21152	22.393	ug/l	90
44) Trichloroethene	7.123	130	97815	114.405	ug/l	95
64) Tetrachloroethene	9.275	164	887	1.132	ug/l	# 87




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045569.D  
 Acq On : 03 Apr 2025 14:27  
 Operator : JC/MD  
 Sample : Q1711-04 100X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-17B-55-040225




Quant Time: Apr 04 01:22:53 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

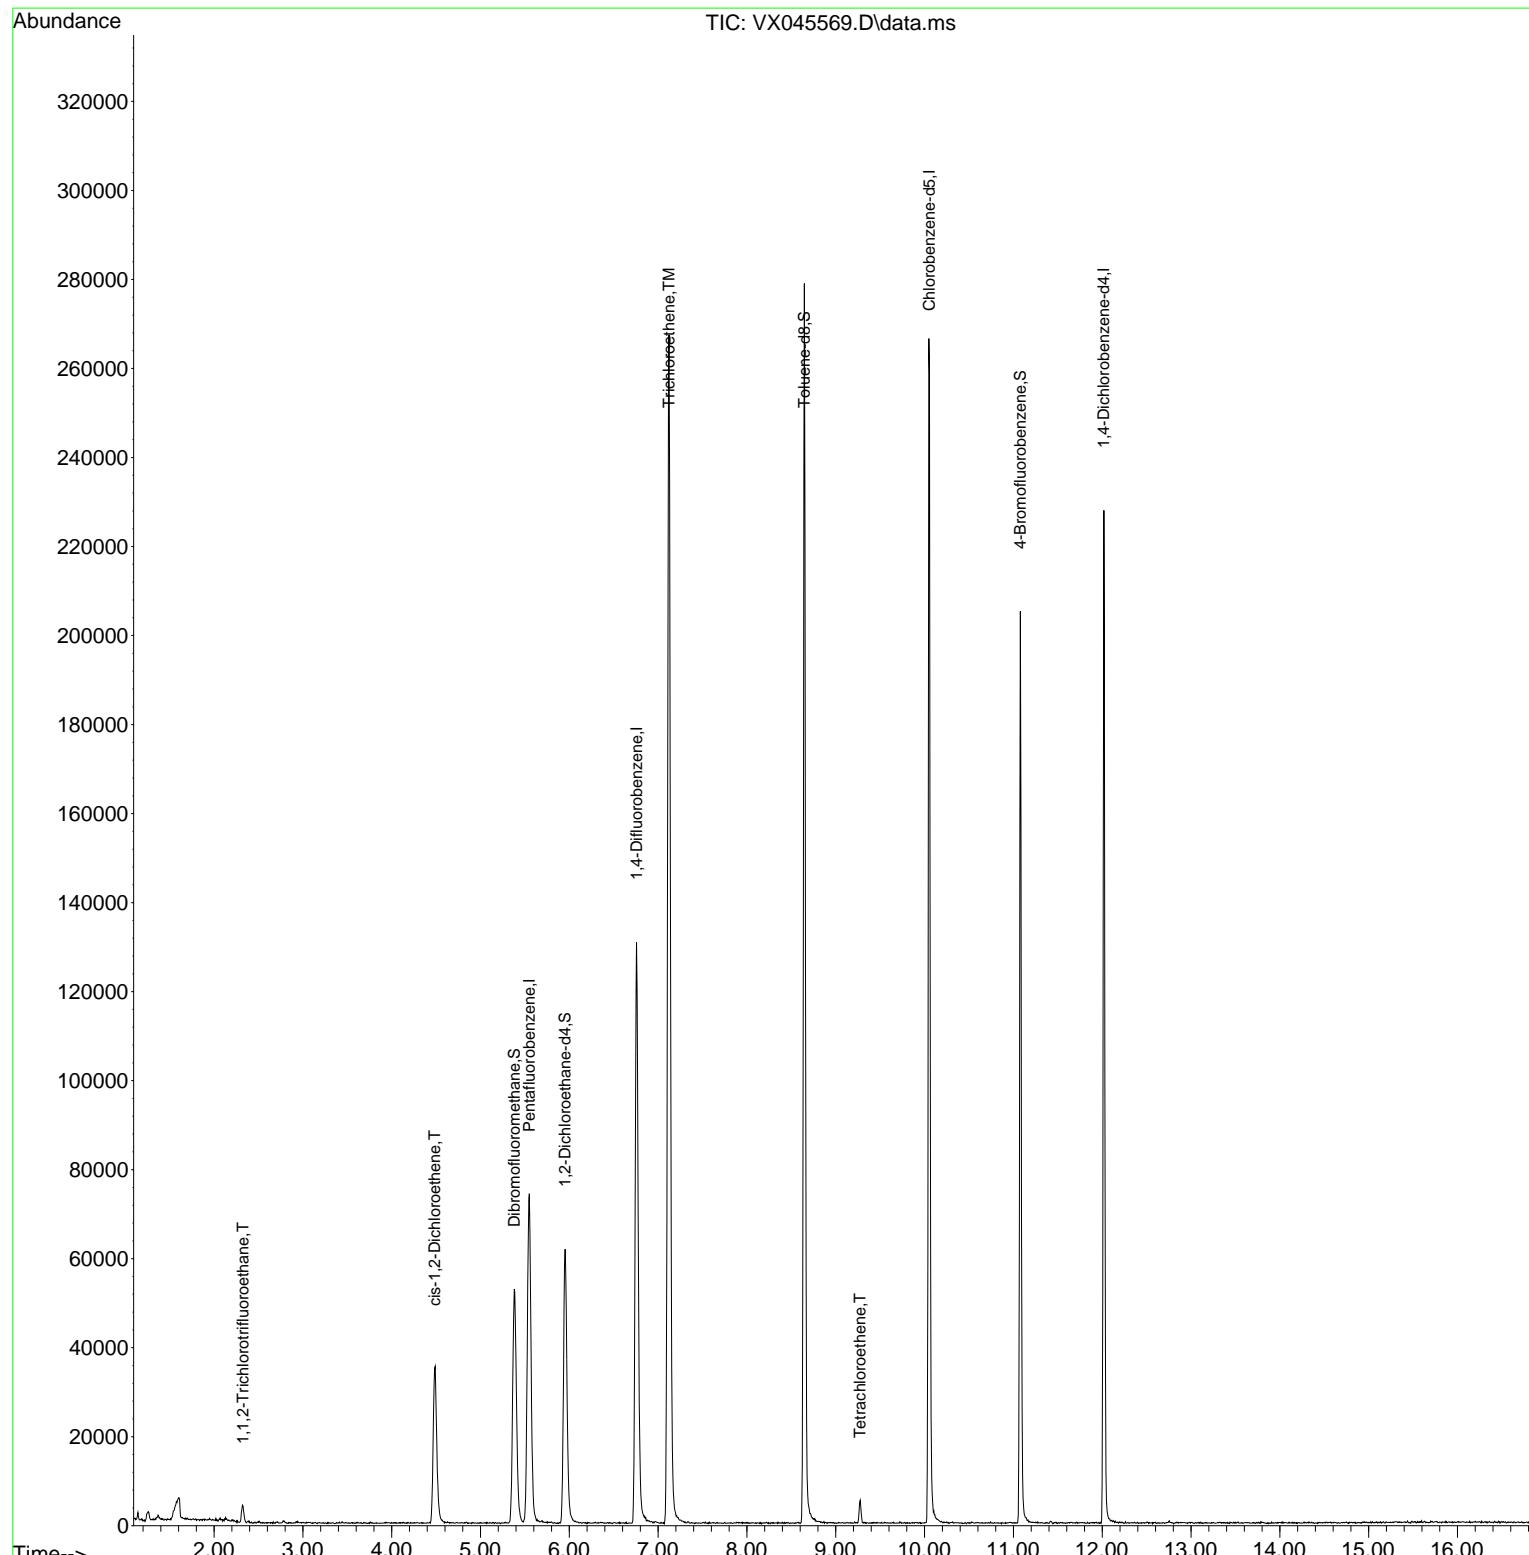





#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Instrument: MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX045569.D  
Acq: 03 Apr 2025 14:27  
ClientSampleId : MW-17B-55-040225


Tgt Ion:168 Resp: 63215  
Ion Ratio Lower Upper  
168 100  
99 72.0 52.3 78.5



#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 1.445 ug/l  
RT: 2.325 min Scan# 203  
Delta R.T. 0.000 min  
Lab File: VX045569.D  
Acq: 03 Apr 2025 14:27

Tgt Ion:101 Resp: 1122  
Ion Ratio Lower Upper  
101 100  
85 52.9 38.9 58.3  
151 92.4 57.5 86.3#


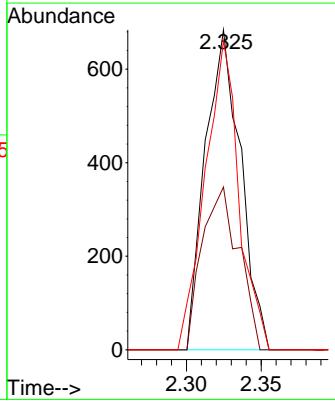


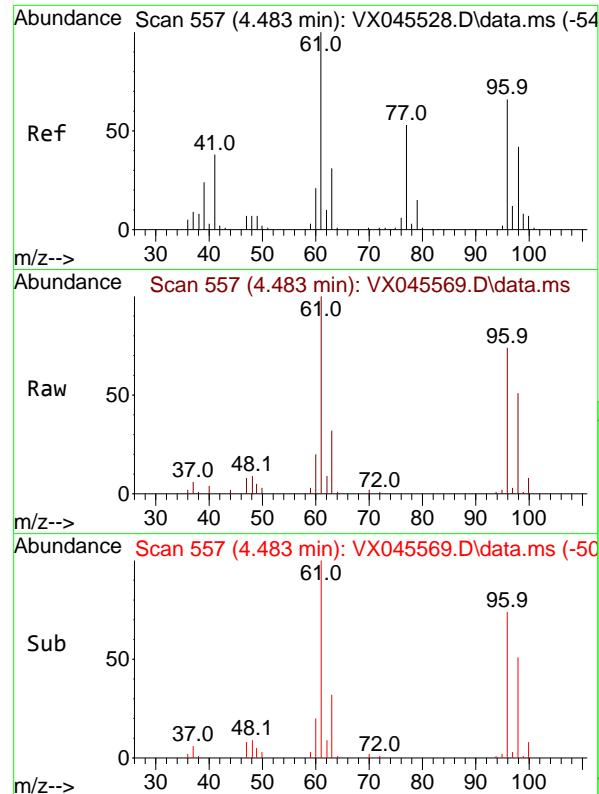

#27  
cis-1,2-Dichloroethene  
Concen: 22.393 ug/l  
RT: 4.483 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX045569.D  
Acq: 03 Apr 2025 14:27


Instrument : MSVOA\_X  
ClientSampleId : MW-17B-55-040225


Tgt Ion: 96 Resp: 21152  
Ion Ratio Lower Upper  
96 100  
61 138.2 0.0 313.2  
98 64.1 0.0 126.4

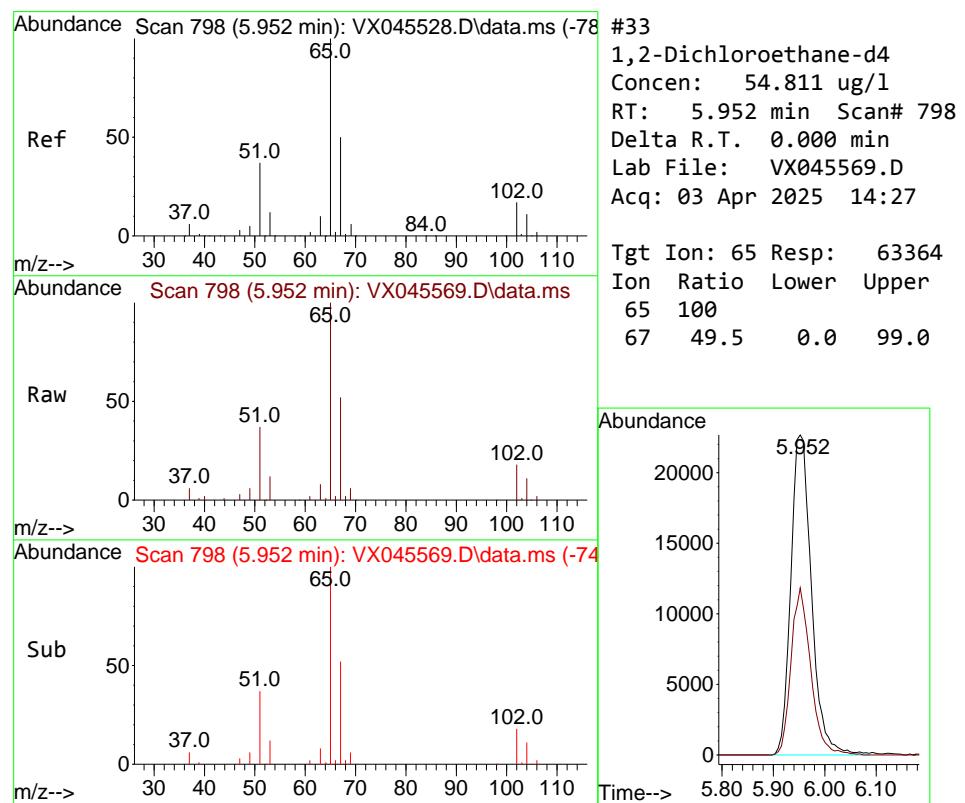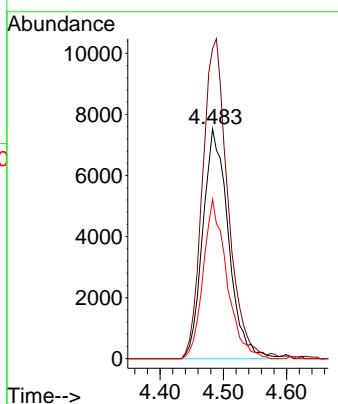

#33  
1,2-Dichloroethane-d4  
Concen: 54.811 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. 0.000 min  
Lab File: VX045569.D  
Acq: 03 Apr 2025 14:27

Tgt Ion: 65 Resp: 63364  
Ion Ratio Lower Upper  
65 100  
67 49.5 0.0 99.0

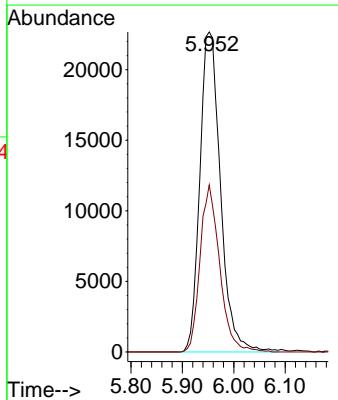

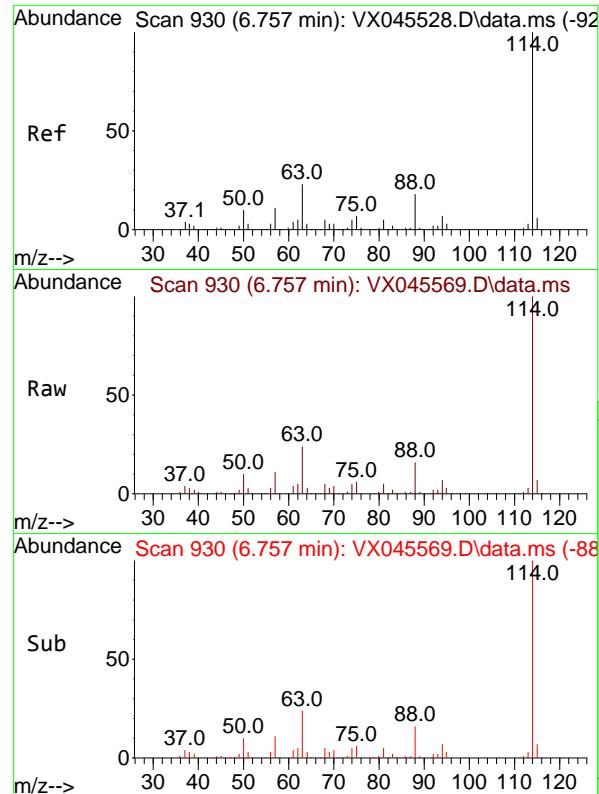

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 9

Delta R.T. 0.000 min

Lab File: VX045569.D


Acq: 03 Apr 2025 14:27

Instrument:

MSVOA\_X

ClientSampleId :

MW-17B-55-040225

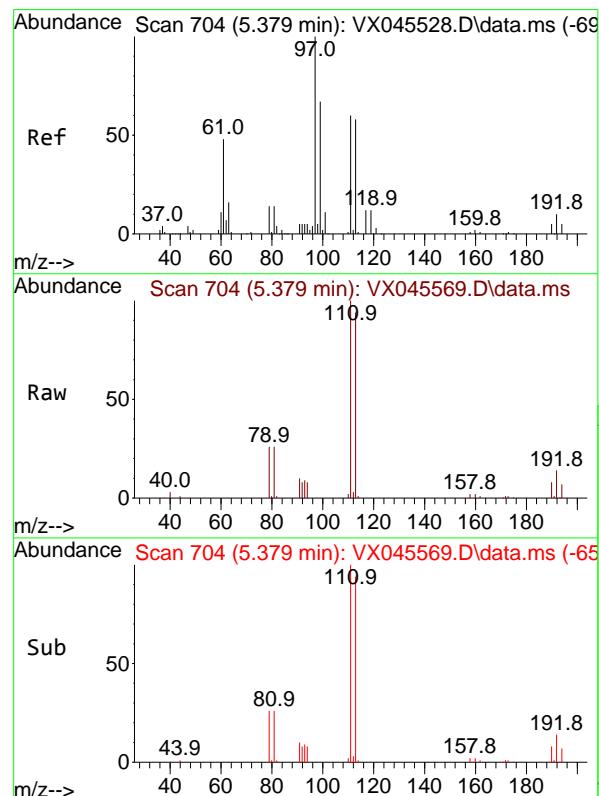

#35

Dibromofluoromethane

Concen: 52.217 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX045569.D

Acq: 03 Apr 2025 14:27


Tgt Ion:113 Resp: 45550




Ion Ratio Lower Upper

113 100

111 104.5 81.8 122.6

192 16.3 13.8 20.6

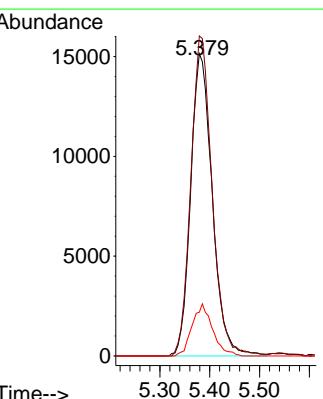

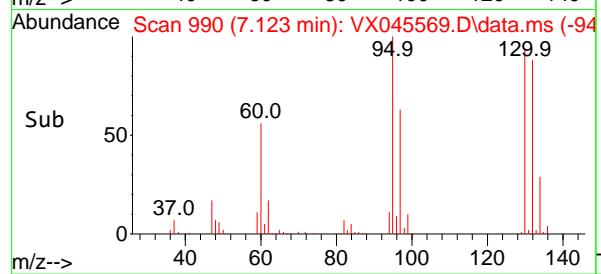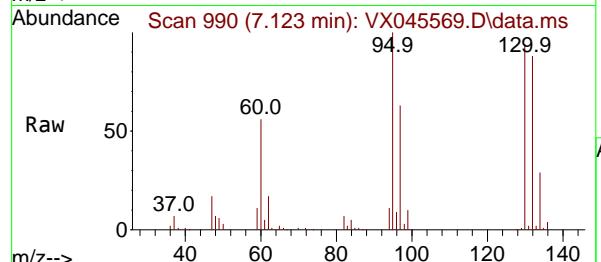

#44

Trichloroethene

Concen: 114.405 ug/l

RT: 7.123 min Scan# 9

Delta R.T. 0.000 min

Lab File: VX045569.D

Acq: 03 Apr 2025 14:27

Instrument:

MSVOA\_X

ClientSampleId :





MW-17B-55-040225

Tgt Ion:130 Resp: 97815

Ion Ratio Lower Upper

130 100

95 106.1 0.0 202.0

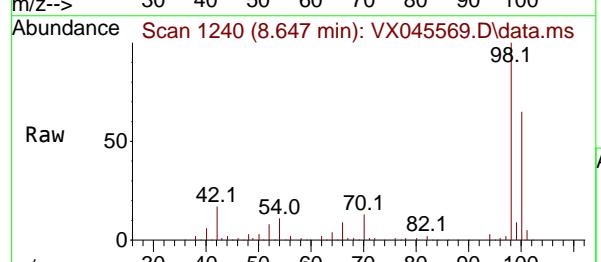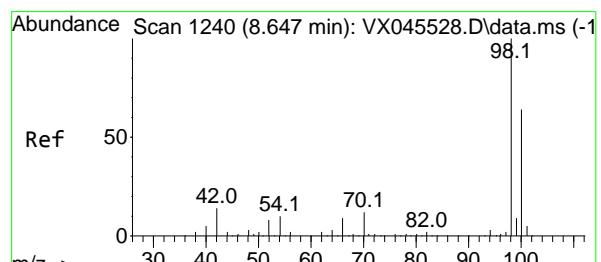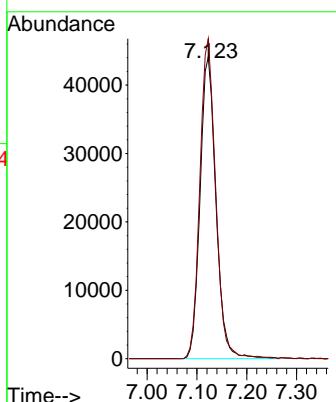

#50

Toluene-d8

Concen: 50.702 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX045569.D


Acq: 03 Apr 2025 14:27


Tgt Ion: 98 Resp: 154375

Ion Ratio Lower Upper

98 100



100 65.1 52.2 78.4

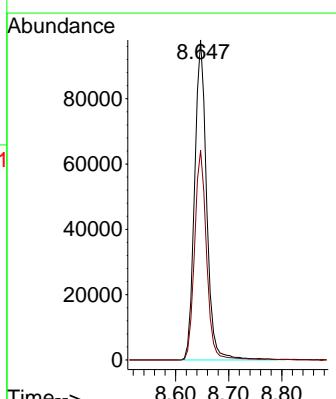

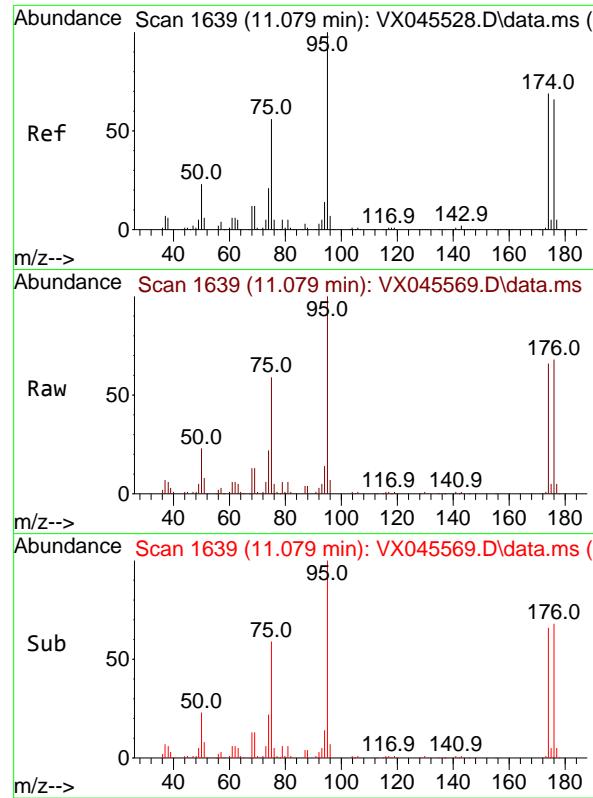


#62  
4-Bromofluorobenzene  
Concen: 46.882 ug/l  
RT: 11.079 min Scan# 1  
Instrument: MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045569.D  
ClientSampleId : MW-17B-55-040225  
Acq: 03 Apr 2025 14:27




Tgt Ion: 95 Resp: 51995  
Ion Ratio Lower Upper  
95 100  
174 69.3 0.0 135.8  
176 68.1 0.0 131.4

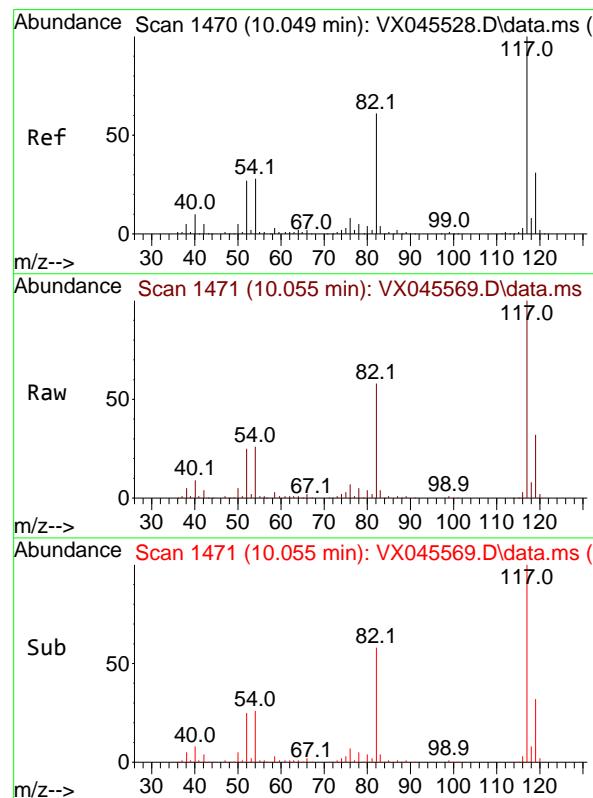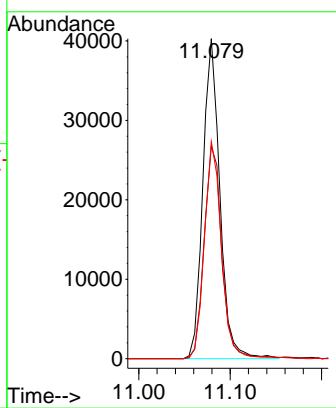

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.006 min  
Lab File: VX045569.D  
Acq: 03 Apr 2025 14:27

Tgt Ion:117 Resp: 111016  
Ion Ratio Lower Upper  
117 100  
82 58.2 49.2 73.8  
119 31.6 25.1 37.7

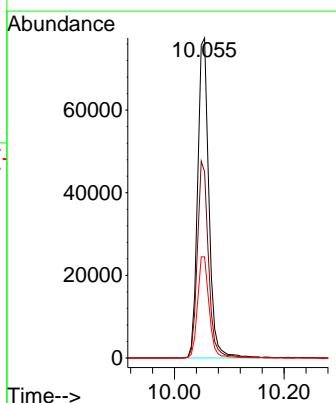



#64

Tetrachloroethene

Concen: 1.132 ug/l

RT: 9.275 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045569.D

Acq: 03 Apr 2025 14:27

Instrument:

MSVOA\_X

ClientSampleId :

MW-17B-55-040225

Tgt Ion:164 Resp: 887

Ion Ratio Lower Upper

164 100




166 134.3 103.8 155.8

129 115.8 84.3 126.5

131 73.5 80.9 121.3#

Abundance

Time--&gt;



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX045569.D

Acq: 03 Apr 2025 14:27

Tgt Ion:152 Resp: 41790

Ion Ratio Lower Upper


152 100

115 65.3 46.9 140.7

150 159.4 0.0 349.4

Abundance

Time--&gt;

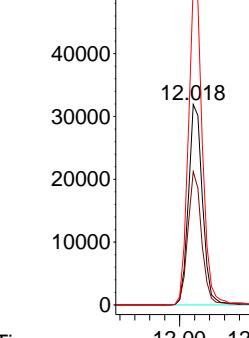



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	04/02/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	04/02/25	
Client Sample ID:	RMW-05B-89-040225			SDG No.:	Q1711	
Lab Sample ID:	Q1711-07			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045568.D	1		04/03/25 14:04	VX040325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	1.60		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	4.00		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	55.2		70 (74) - 130 (125)	110%	SPK: 50
1868-53-7	Dibromofluoromethane	52.0		70 (75) - 130 (124)	104%	SPK: 50
2037-26-5	Toluene-d8	50.6		70 (86) - 130 (113)	101%	SPK: 50
460-00-4	4-Bromofluorobenzene	50.6		70 (77) - 130 (121)	101%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	63800	5.55			
540-36-3	1,4-Difluorobenzene	125000	6.757			
3114-55-4	Chlorobenzene-d5	116000	10.049			
3855-82-1	1,4-Dichlorobenzene-d4	47000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045568.D  
 Acq On : 03 Apr 2025 14:04  
 Operator : JC/MD  
 Sample : Q1711-07  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**RMW-05B-89-040225**

Quant Time: Apr 04 01:22:25 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	63845	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	125144	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	116415	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	47044	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	64496	55.240	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	110.480%	
35) Dibromofluoromethane	5.385	113	46192	52.024	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	104.040%	
50) Toluene-d8	8.647	98	156862	50.615	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	101.240%	
62) 4-Bromofluorobenzene	11.079	95	57168	50.643	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	101.280%	
<b>Target Compounds</b>						
				Qvalue		
16) Acetone	2.379	43	1776	3.704	ug/l	97
17) Carbon Disulfide	2.507	76	819	0.433	ug/l	# 90
24) 1,1-Dichloroethane	3.605	63	2586	1.596	ug/l	# 91
27) cis-1,2-Dichloroethene	4.489	96	3859	4.045	ug/l	91




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045568.D  
 Acq On : 03 Apr 2025 14:04  
 Operator : JC/MD  
 Sample : Q1711-07  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RMW-05B-89-040225




Quant Time: Apr 04 01:22:25 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

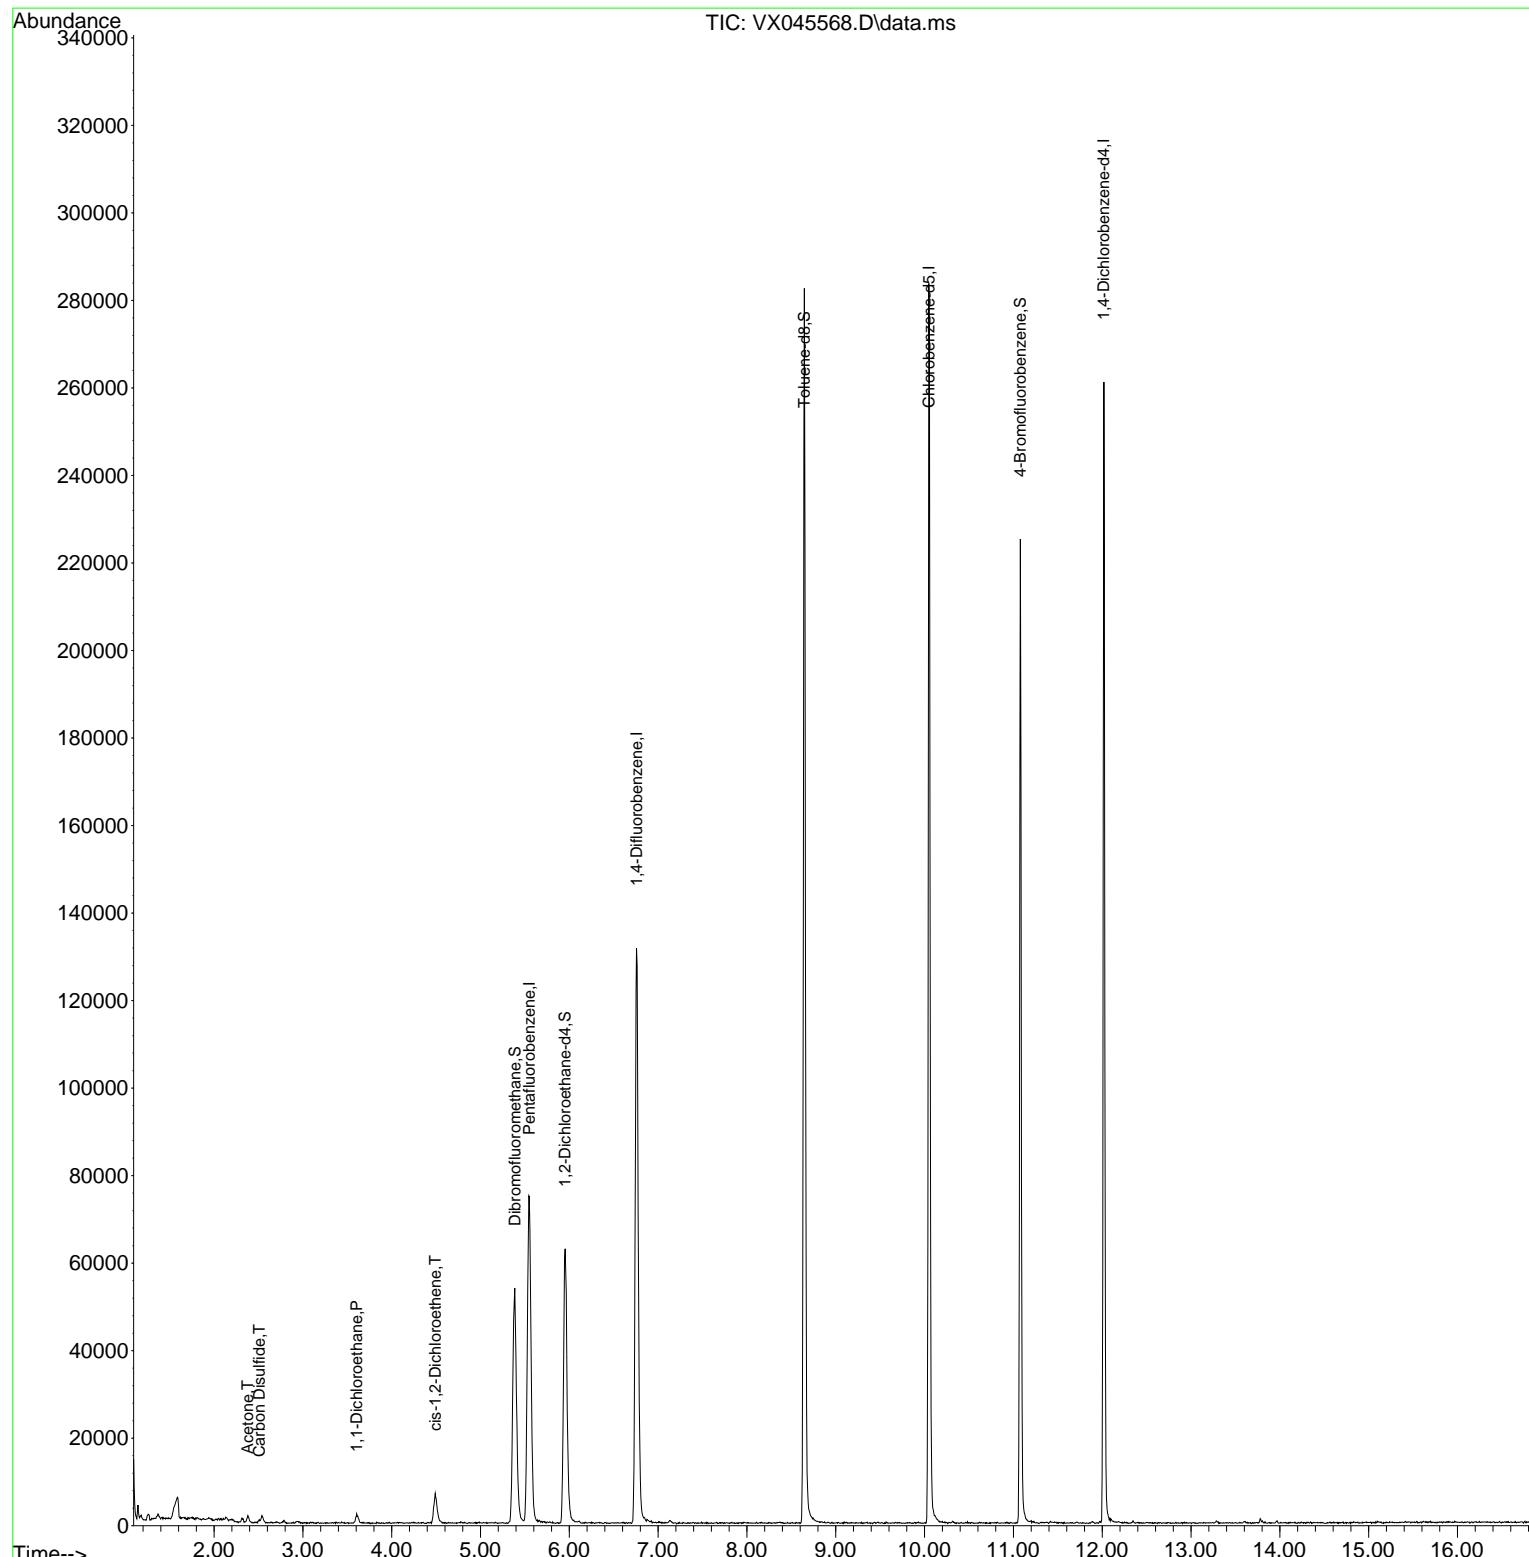





#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Instrument: MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX045568.D  
Acq: 03 Apr 2025 14:04  
ClientSampleId : RMW-05B-89-040225







Tgt Ion:168 Resp: 63845  
Ion Ratio Lower Upper  
168 100  
99 69.6 52.3 78.5

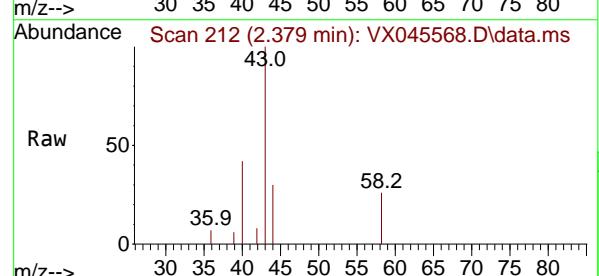

#16  
Acetone  
Concen: 3.704 ug/l  
RT: 2.379 min Scan# 212  
Delta R.T. -0.006 min  
Lab File: VX045568.D  
Acq: 03 Apr 2025 14:04

Tgt Ion: 43 Resp: 1776  
Ion Ratio Lower Upper  
43 100  
58 26.5 22.3 33.5

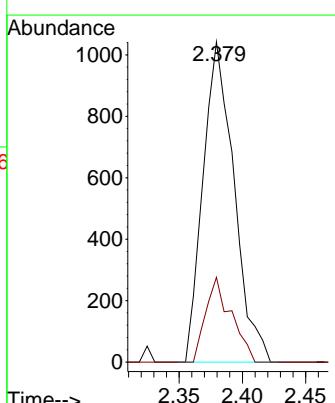



#17

Carbon Disulfide

Concen: 0.433 ug/l

RT: 2.507 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX045568.D

Acq: 03 Apr 2025 14:04

Instrument:

MSVOA\_X

ClientSampleId :


RMW-05B-89-040225

Tgt Ion: 76 Resp: 819

Ion Ratio Lower Upper

76 100

78 12.4 7.0 10.6#

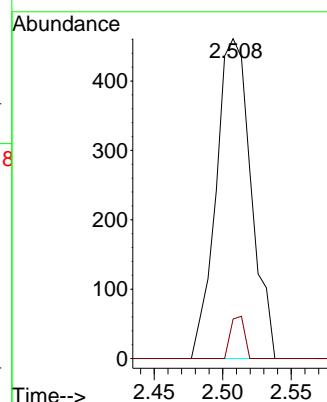

#24

1,1-Dichloroethane

Concen: 1.596 ug/l

RT: 3.605 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX045568.D

Acq: 03 Apr 2025 14:04


Tgt Ion: 63 Resp: 2586




Ion Ratio Lower Upper

63 100

98 8.9 3.4 10.1

100 0.0 2.2 6.6#




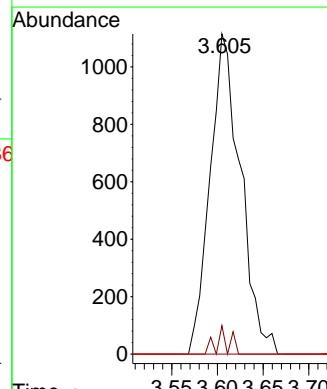




#27  
cis-1,2-Dichloroethene  
Concen: 4.045 ug/l  
RT: 4.489 min Scan# 5  
Delta R.T. 0.006 min  
Lab File: VX045568.D  
Acq: 03 Apr 2025 14:04


Instrument : MSVOA\_X  
ClientSampleId : RMW-05B-89-040225


Tgt Ion: 96 Resp: 3859  
Ion Ratio Lower Upper  
96 100  
61 142.5 0.0 313.2  
98 66.6 0.0 126.4



#33  
1,2-Dichloroethane-d4  
Concen: 55.240 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. -0.000 min  
Lab File: VX045568.D  
Acq: 03 Apr 2025 14:04

Tgt Ion: 65 Resp: 64496  
Ion Ratio Lower Upper  
65 100  
67 49.1 0.0 99.0

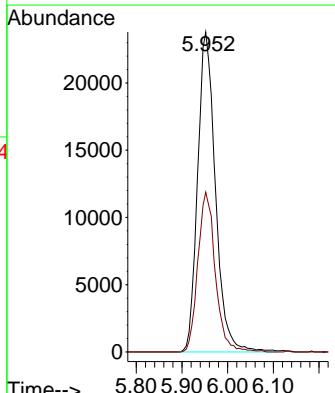

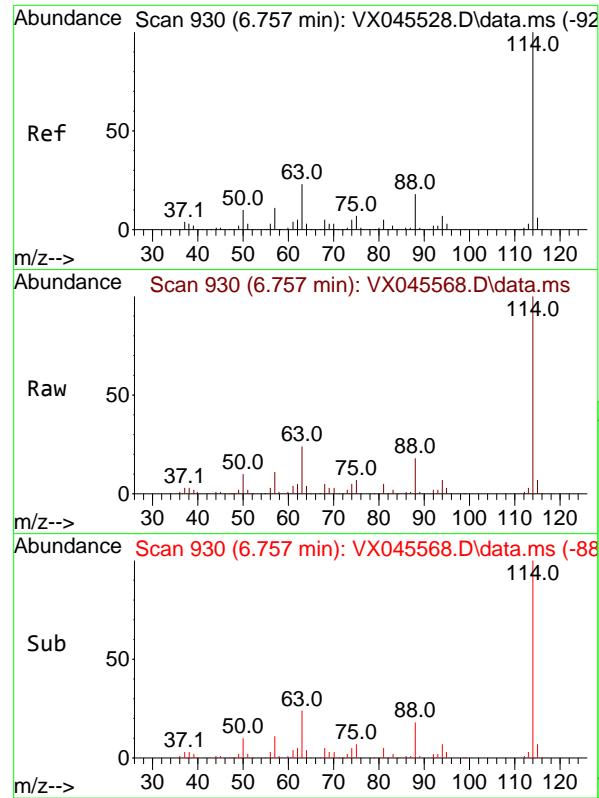

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 9

Instrument:

MSVOA\_X

Delta R.T. -0.000 min

Lab File: VX045568.D ClientSampleId :

Acq: 03 Apr 2025 14:04 RMW-05B-89-040225



Tgt Ion:114 Resp: 125144

Ion Ratio Lower Upper

114 100

63 24.1 0.0 46.8

88 18.2 0.0 35.4

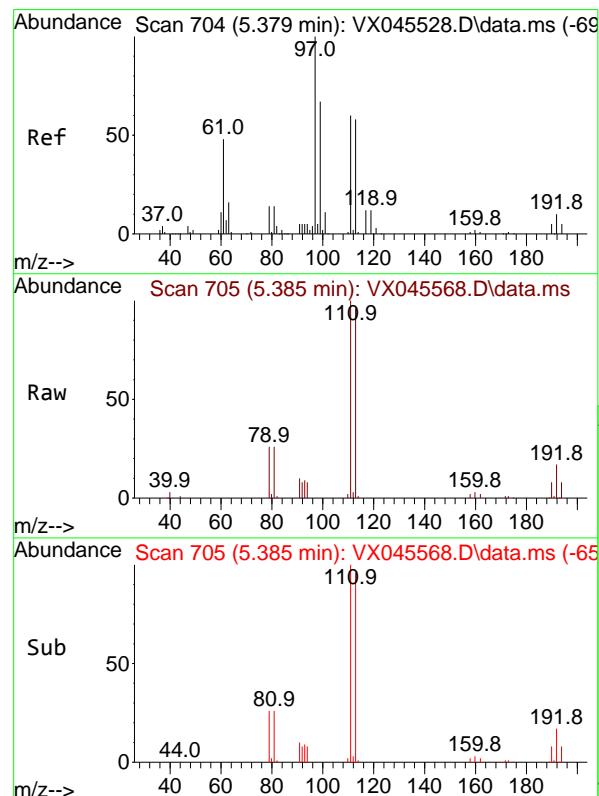

#35  
Dibromofluoromethane  
Concen: 52.024 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.006 min  
Lab File: VX045568.D  
Acq: 03 Apr 2025 14:04


Tgt Ion:113 Resp: 46192




Ion Ratio Lower Upper

113 100

111 102.0 81.8 122.6

192 17.0 13.8 20.6







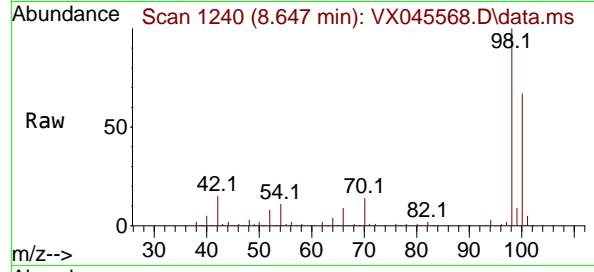

#50  
Toluene-d8  
Concen: 50.615 ug/l  
RT: 8.647 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045568.D  
Acq: 03 Apr 2025 14:04


Instrument : MSVOA\_X  
ClientSampleId : RMW-05B-89-040225


Tgt Ion: 98 Resp: 156862  
Ion Ratio Lower Upper  
98 100  
100 64.9 52.2 78.4

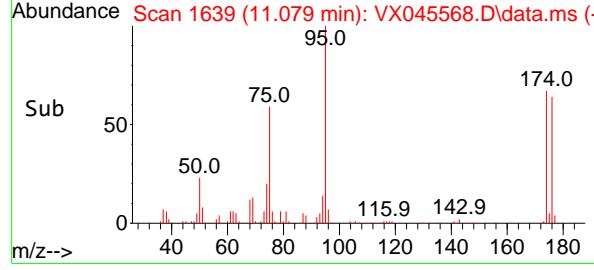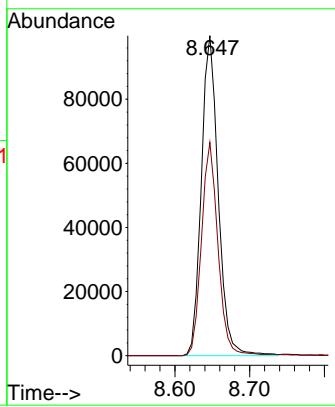

#62  
4-Bromofluorobenzene  
Concen: 50.643 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX045568.D  
Acq: 03 Apr 2025 14:04



Tgt Ion: 95 Resp: 57168  
Ion Ratio Lower Upper  
95 100  
174 68.6 0.0 135.8  
176 65.9 0.0 131.4

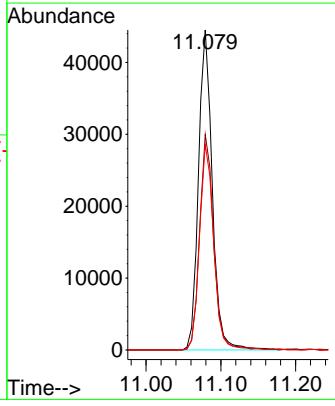

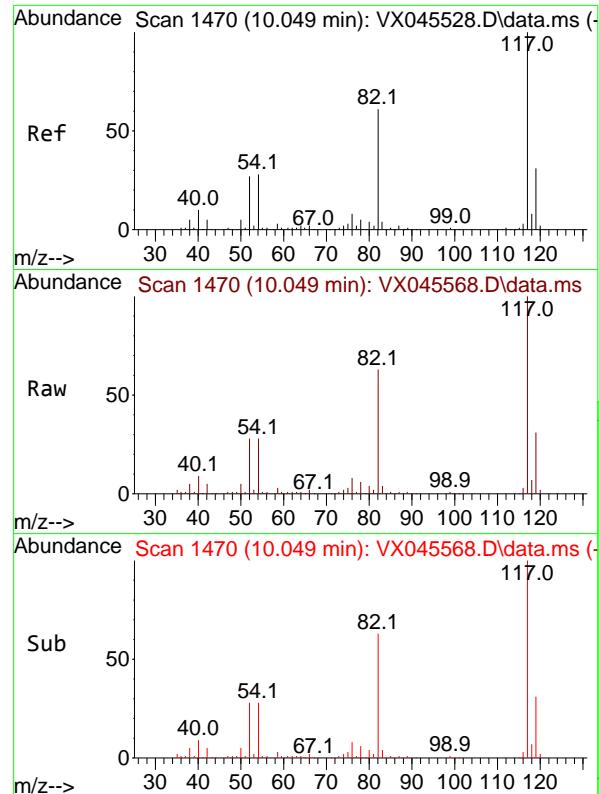


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX045568.D  
ClientSampleId : RMW-05B-89-040225  
Acq: 03 Apr 2025 14:04

Tgt Ion:117 Resp: 116415  
Ion Ratio Lower Upper  
117 100  
82 62.6 49.2 73.8  
119 31.4 25.1 37.7

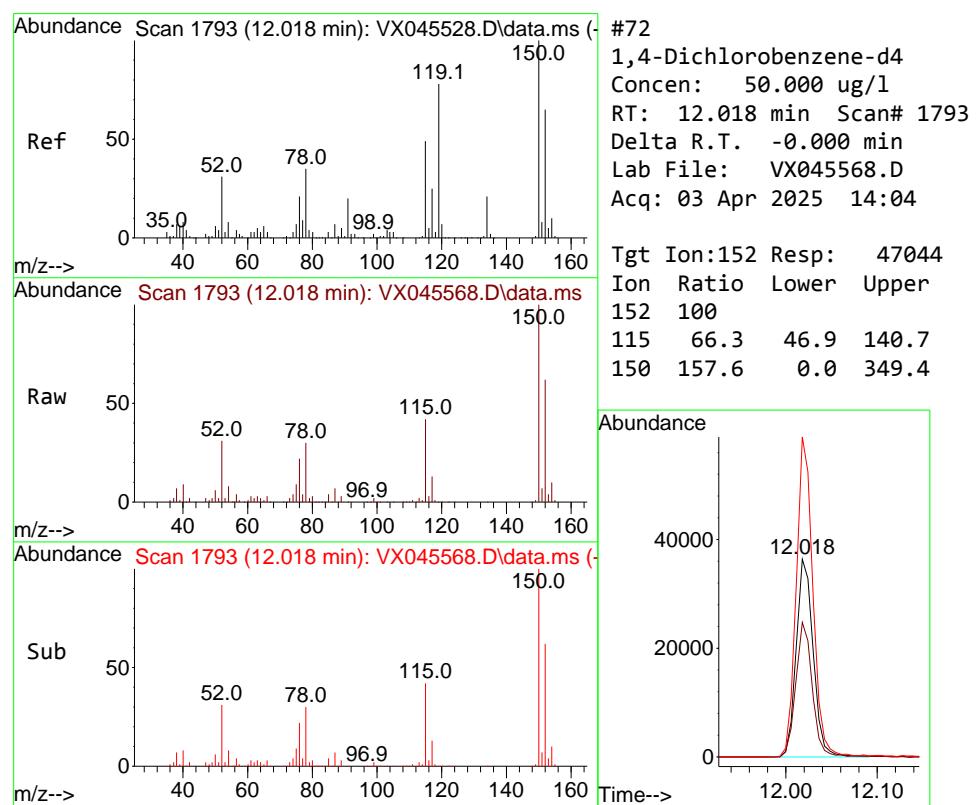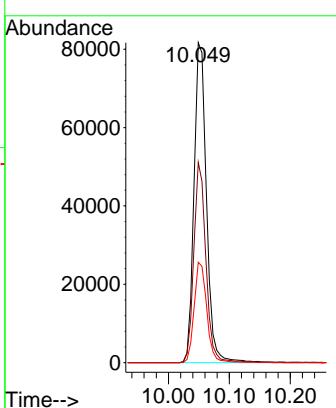

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. -0.000 min  
Lab File: VX045568.D  
Acq: 03 Apr 2025 14:04

Tgt Ion:152 Resp: 47044  
Ion Ratio Lower Upper  
152 100  
115 66.3 46.9 140.7  
150 157.6 0.0 349.4

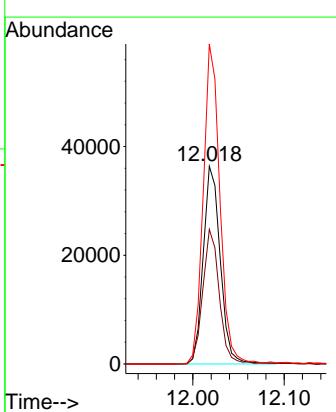



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	04/02/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	04/02/25	
Client Sample ID:	EB01-040225			SDG No.:	Q1711	
Lab Sample ID:	Q1711-08			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045572.D	1		04/03/25 15:37	VX040325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	53.4		70 (74) - 130 (125)	107%	SPK: 50
1868-53-7	Dibromofluoromethane	51.0		70 (75) - 130 (124)	102%	SPK: 50
2037-26-5	Toluene-d8	50.9		70 (86) - 130 (113)	102%	SPK: 50
460-00-4	4-Bromofluorobenzene	49.8		70 (77) - 130 (121)	100%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	63300	5.543			
540-36-3	1,4-Difluorobenzene	123000	6.757			
3114-55-4	Chlorobenzene-d5	114000	10.049			
3855-82-1	1,4-Dichlorobenzene-d4	46600	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045572.D  
 Acq On : 03 Apr 2025 15:37  
 Operator : JC/MD  
 Sample : Q1711-08  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 15 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
EB01-040225

Quant Time: Apr 04 01:24:01 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.543	168	63287	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	123377	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	114226	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	46598	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	61834	53.427	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	106.860%	
35) Dibromofluoromethane	5.379	113	44624	50.978	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	101.960%	
50) Toluene-d8	8.646	98	155462	50.882	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	101.760%	
62) 4-Bromofluorobenzene	11.079	95	55448	49.822	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	99.640%	
<b>Target Compounds</b>						
				Qvalue		
16) Acetone	2.385	43	15475	32.562	ug/l	99
20) Methylene Chloride	2.782	84	895	1.006	ug/l	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045572.D  
 Acq On : 03 Apr 2025 15:37  
 Operator : JC/MD  
 Sample : Q1711-08  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EB01-040225




Quant Time: Apr 04 01:24:01 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

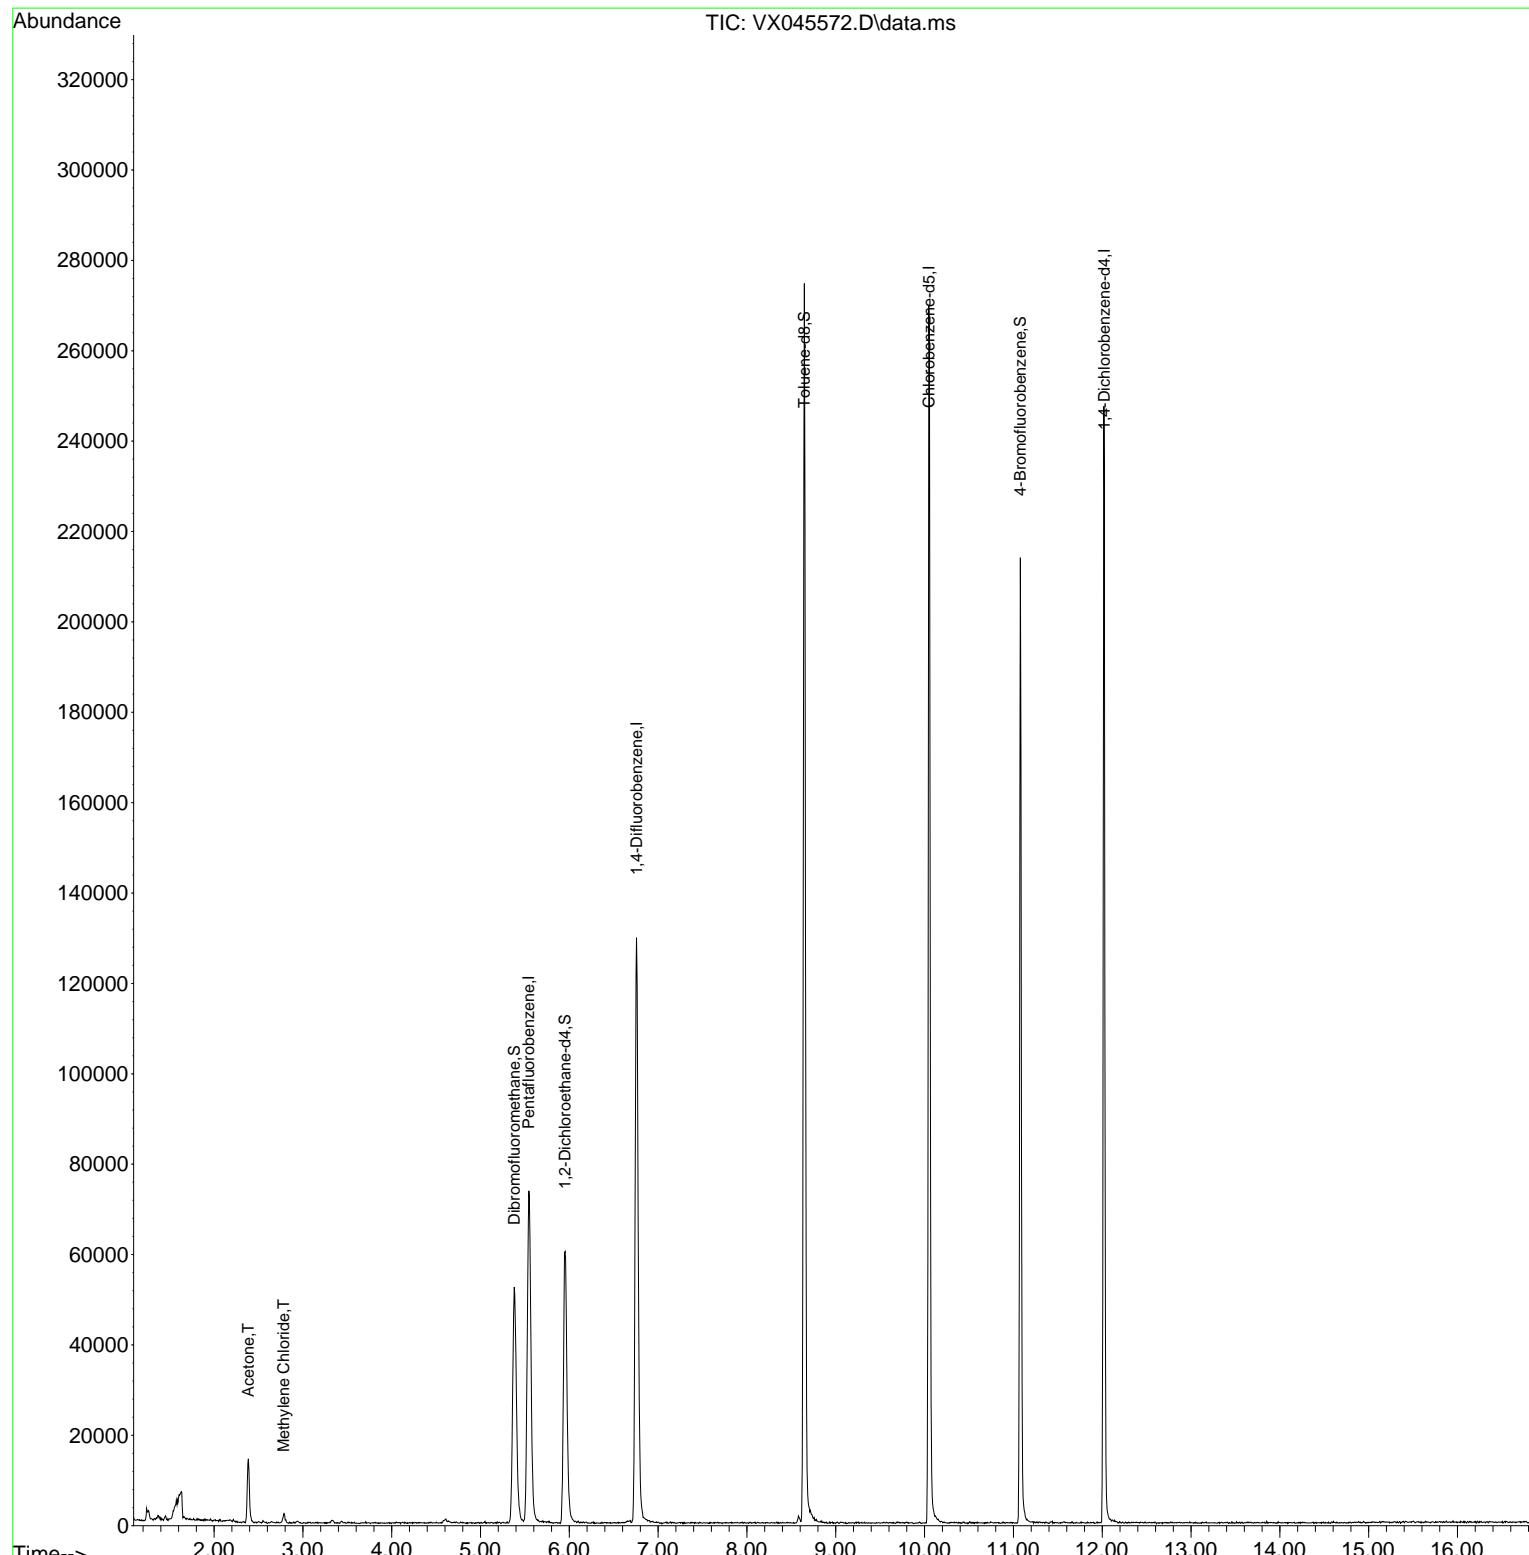

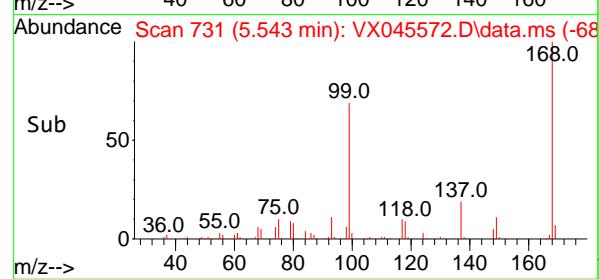



#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.543 min Scan# 7  
Instrument : MSVOA\_X  
Delta R.T. -0.007 min  
Lab File: VX045572.D  
Acq: 03 Apr 2025 15:37  
ClientSampleId : EB01-040225




Tgt Ion:168 Resp: 63287  
Ion Ratio Lower Upper  
168 100  
99 68.9 52.3 78.5

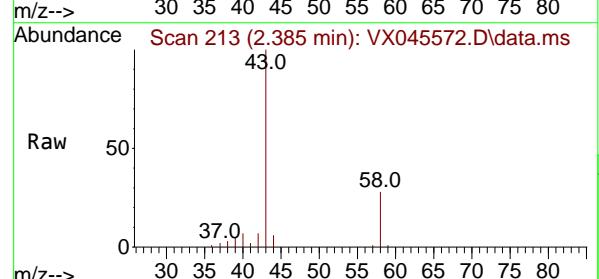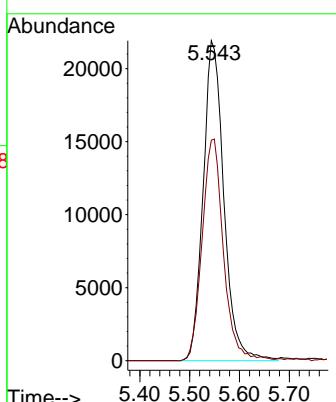

#16  
Acetone  
Concen: 32.562 ug/l  
RT: 2.385 min Scan# 213  
Delta R.T. -0.000 min  
Lab File: VX045572.D  
Acq: 03 Apr 2025 15:37

Tgt Ion: 43 Resp: 15475  
Ion Ratio Lower Upper  
43 100  
58 27.6 22.3 33.5

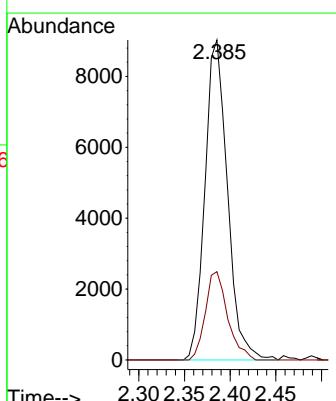



#20

Methylene Chloride

Concen: 1.006 ug/l

RT: 2.782 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX045572.D

Acq: 03 Apr 2025 15:37

Instrument:

MSVOA\_X

ClientSampleId :

EB01-040225

Tgt Ion: 84 Resp: 895

Ion Ratio Lower Upper





84 100

49 128.1 107.5 161.3

51 42.0 33.0 49.6

86 59.1 50.1 75.1

Abundance

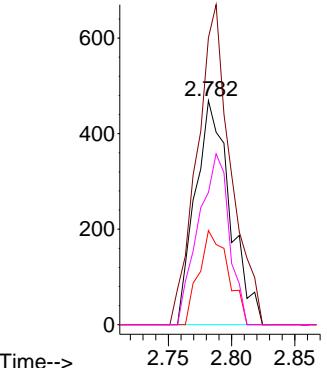

#33

1,2-Dichloroethane-d4

Concen: 53.427 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX045572.D

Acq: 03 Apr 2025 15:37


Tgt Ion: 65 Resp: 61834


Ion Ratio Lower Upper

65 100

67 50.1 0.0 99.0

Abundance

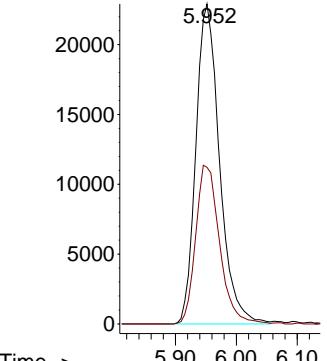

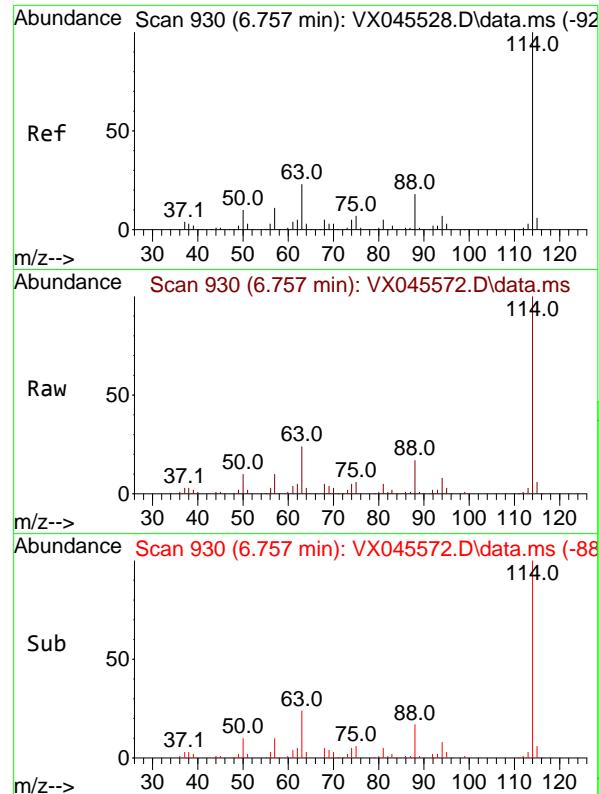

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 9

Delta R.T. -0.000 min

Lab File: VX045572.D

Acq: 03 Apr 2025 15:37

Instrument:

MSVOA\_X

ClientSampleId :

EB01-040225



Tgt Ion:114 Resp: 123377

Ion Ratio Lower Upper

114 100

63 24.4 0.0 46.8

88 17.4 0.0 35.4

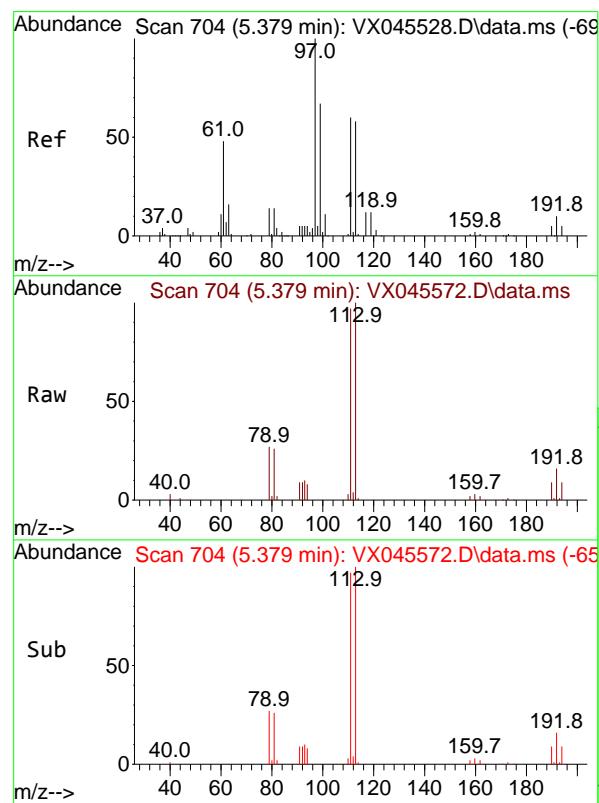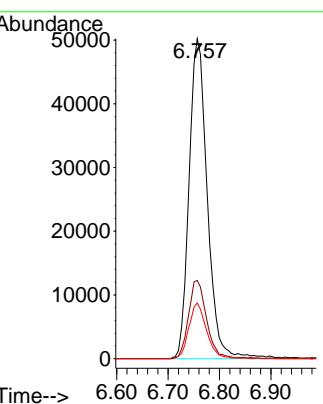

#35

Dibromofluoromethane

Concen: 50.978 ug/l

RT: 5.379 min Scan# 704

Delta R.T. -0.000 min

Lab File: VX045572.D

Acq: 03 Apr 2025 15:37


Tgt Ion:113 Resp: 44624


Ion Ratio Lower Upper

113 100


111 102.8 81.8 122.6

192 17.0 13.8 20.6

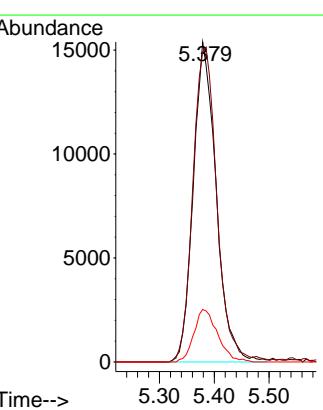




Abundance Scan 1240 (8.646 min): VX045572.D\data.ms

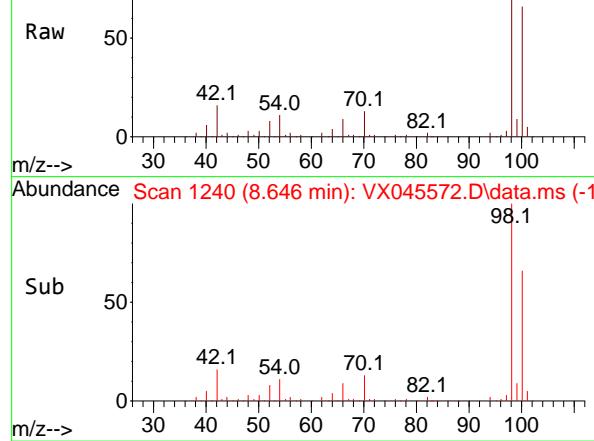

Abundance Scan 1240 (8.646 min): VX045572.D\data.ms (-1)

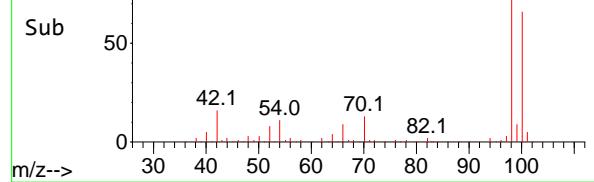

#50  
Toluene-d8  
Concen: 50.882 ug/l  
RT: 8.646 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045572.D  
Acq: 03 Apr 2025 15:37



Instrument: MSVOA\_X  
ClientSampleId : EB01-040225

Tgt Ion: 98 Resp: 155462


Ion Ratio Lower Upper

98 100


100 65.6 52.2 78.4



Abundance Scan 1639 (11.079 min): VX045572.D\data.ms

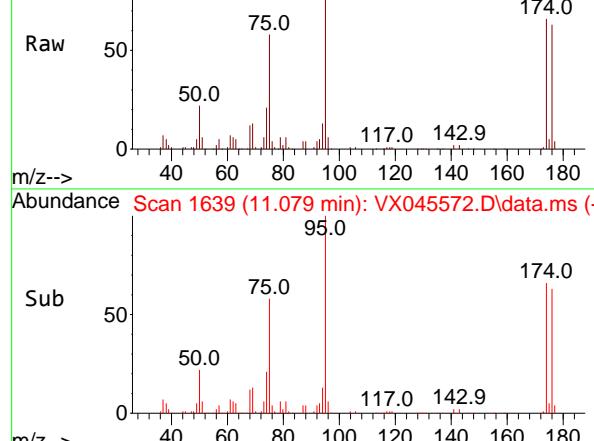

Abundance Scan 1639 (11.079 min): VX045572.D\data.ms (-1)

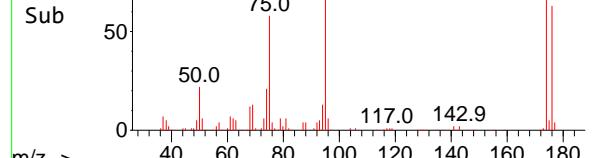

#62  
4-Bromofluorobenzene  
Concen: 49.822 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX045572.D  
Acq: 03 Apr 2025 15:37


Tgt Ion: 95 Resp: 55448


Ion Ratio Lower Upper

95 100

174 67.8 0.0 135.8



176 65.8 0.0 131.4

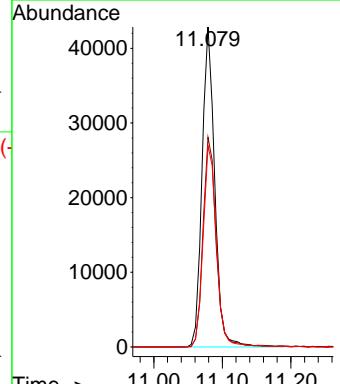

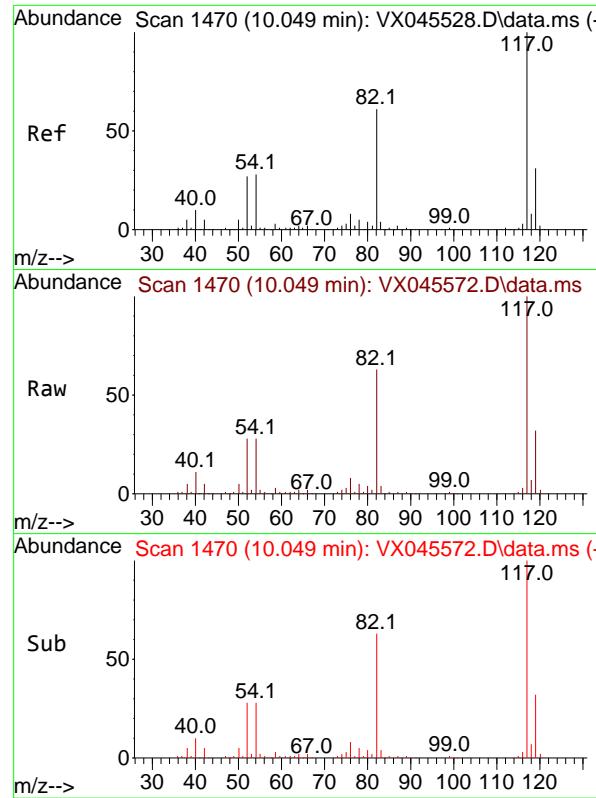


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX045572.D  
ClientSampleId : EB01-040225  
Acq: 03 Apr 2025 15:37

Tgt Ion:117 Resp: 114226  
Ion Ratio Lower Upper  
117 100  
82 63.1 49.2 73.8  
119 32.2 25.1 37.7

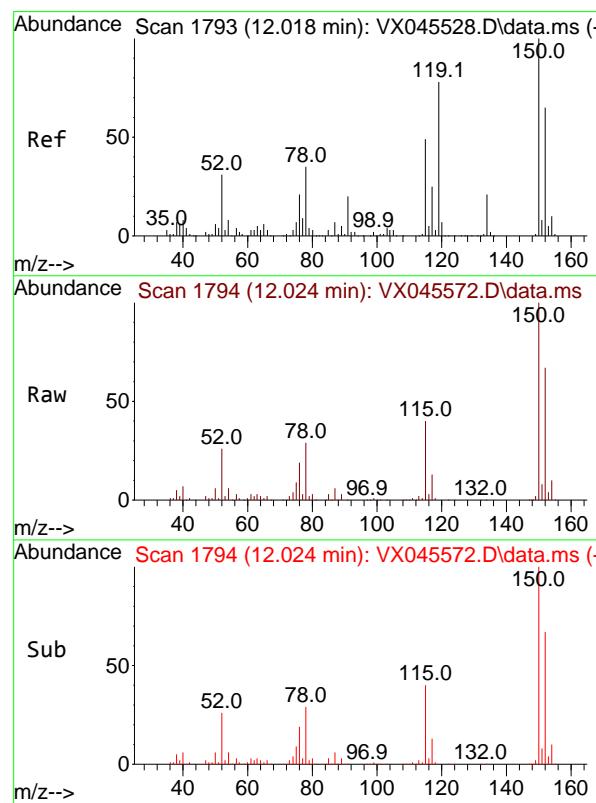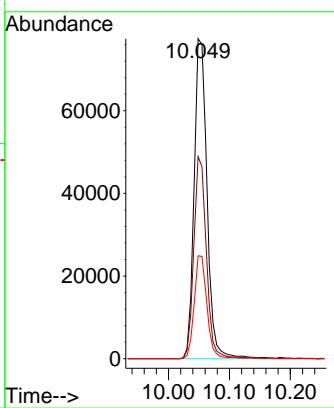

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. 0.006 min  
Lab File: VX045572.D  
Acq: 03 Apr 2025 15:37

Tgt Ion:152 Resp: 46598  
Ion Ratio Lower Upper  
152 100  
115 64.1 46.9 140.7  
150 156.0 0.0 349.4

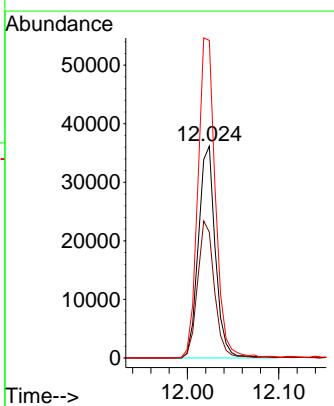



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	04/02/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	04/02/25	
Client Sample ID:	TB01-040225			SDG No.:	Q1711	
Lab Sample ID:	Q1711-10			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045571.D	1		04/03/25 15:14	VX040325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	53.9		70 (74) - 130 (125)	108%	SPK: 50
1868-53-7	Dibromofluoromethane	52.0		70 (75) - 130 (124)	104%	SPK: 50
2037-26-5	Toluene-d8	51.0		70 (86) - 130 (113)	102%	SPK: 50
460-00-4	4-Bromofluorobenzene	51.0		70 (77) - 130 (121)	102%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	66900	5.544			
540-36-3	1,4-Difluorobenzene	129000	6.757			
3114-55-4	Chlorobenzene-d5	122000	10.049			
3855-82-1	1,4-Dichlorobenzene-d4	49400	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045571.D  
 Acq On : 03 Apr 2025 15:14  
 Operator : JC/MD  
 Sample : Q1711-10  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 14 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
TB01-040225

Quant Time: Apr 04 01:23:40 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	66937	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	129076	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	121728	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	49430	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	65957	53.882	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 107.760%			
35) Dibromofluoromethane	5.385	113	47665	52.048	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 104.100%			
50) Toluene-d8	8.647	98	162893	50.960	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 101.920%			
62) 4-Bromofluorobenzene	11.079	95	59432	51.044	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 102.080%			




Target Compounds	Qvalue
(#)= qualifier out of range (m)= manual integration (+)= signals summed	

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
Data File : VX045571.D  
Acq On : 03 Apr 2025 15:14  
Operator : JC/MD  
Sample : Q1711-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB01-040225




Quant Time: Apr 04 01:23:40 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

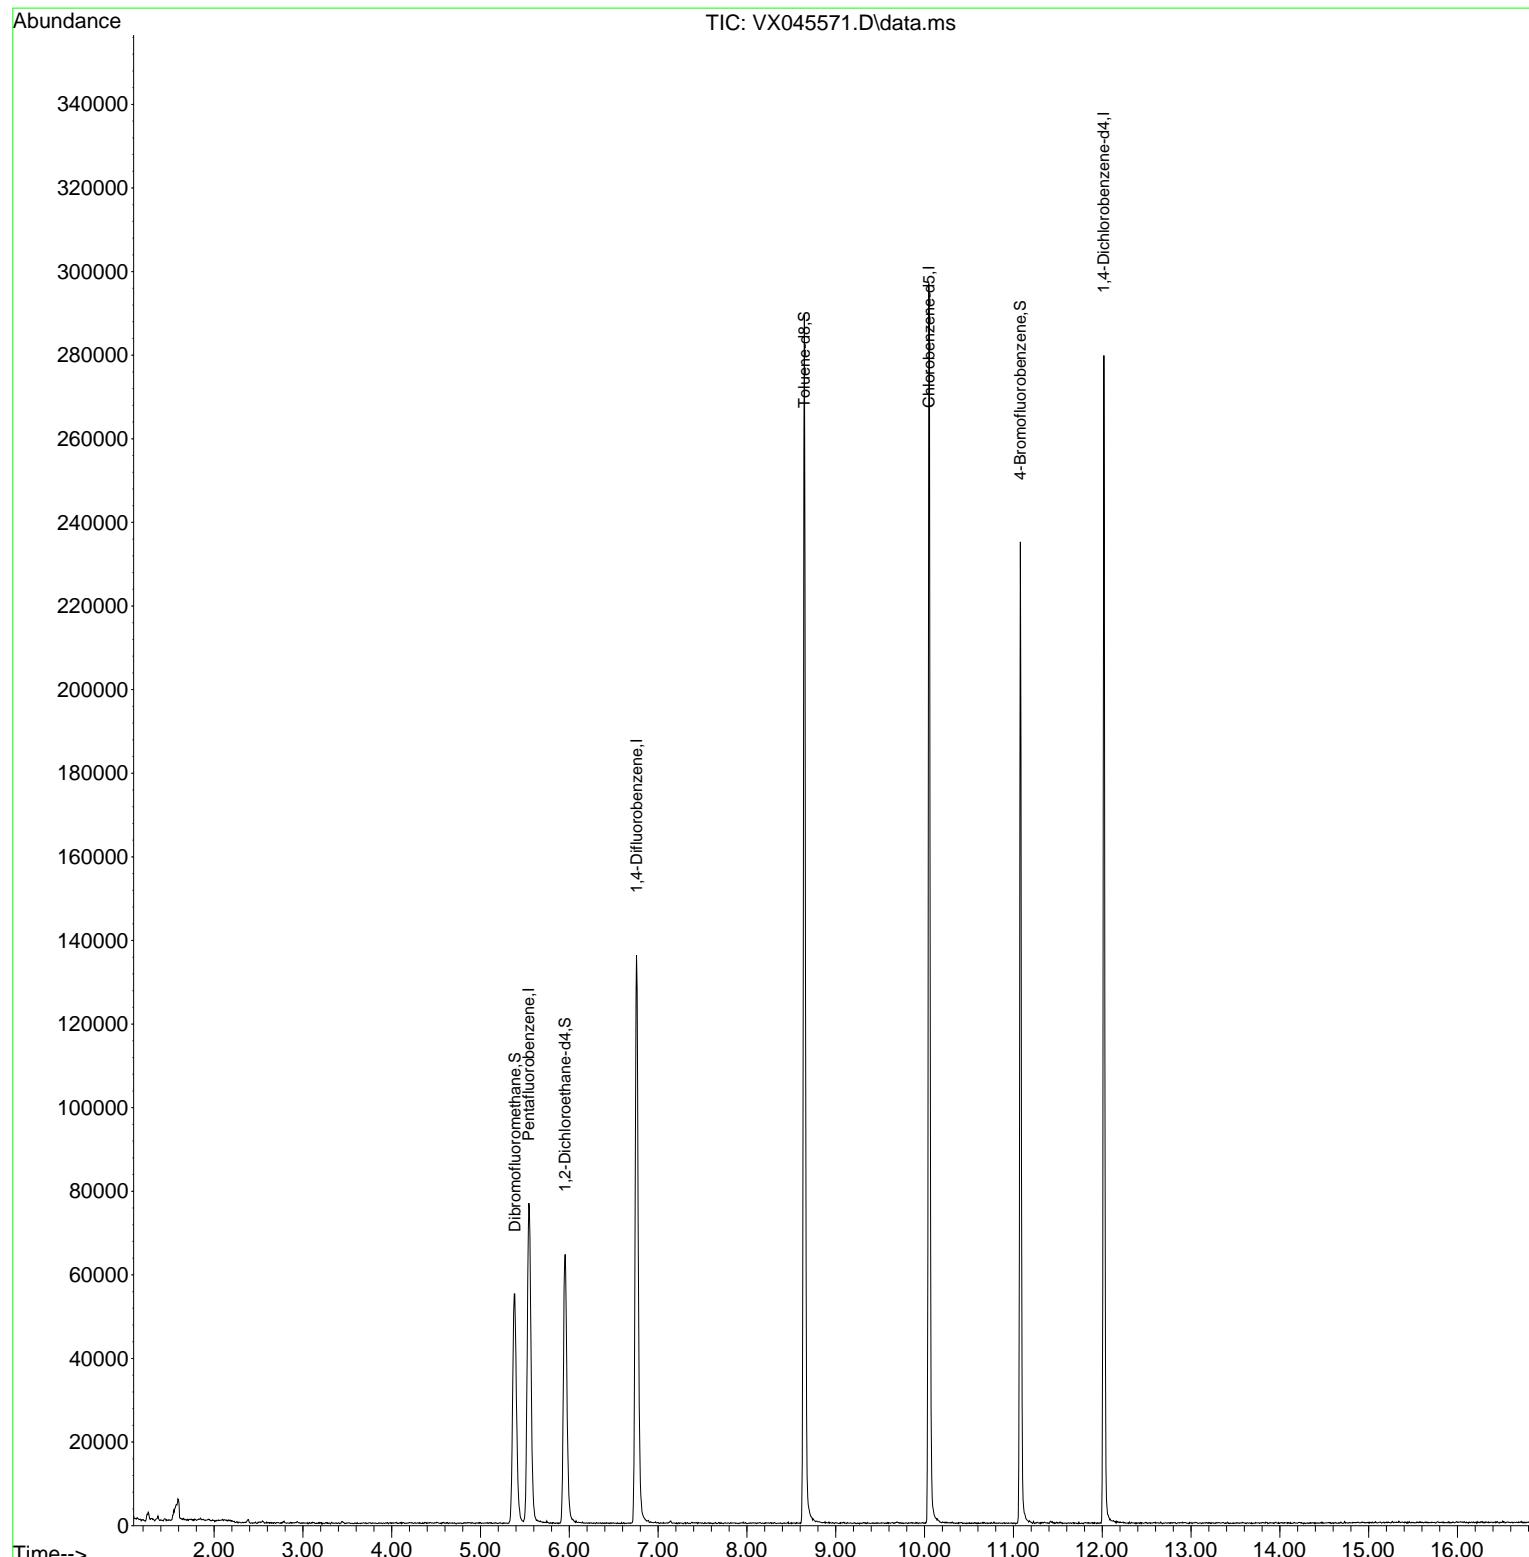





#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.544 min Scan# 7  
Instrument: MSVOA\_X  
Delta R.T. -0.006 min  
Lab File: VX045571.D  
Acq: 03 Apr 2025 15:14  
ClientSampleId : TB01-040225


Tgt Ion:168 Resp: 66937  
Ion Ratio Lower Upper  
168 100  
99 69.5 52.3 78.5

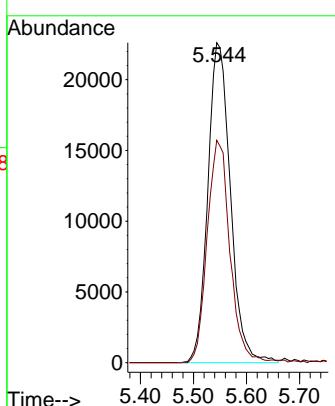

#33  
1,2-Dichloroethane-d4  
Concen: 53.882 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. 0.000 min  
Lab File: VX045571.D  
Acq: 03 Apr 2025 15:14

Tgt Ion: 65 Resp: 65957  
Ion Ratio Lower Upper  
65 100  
67 50.1 0.0 99.0

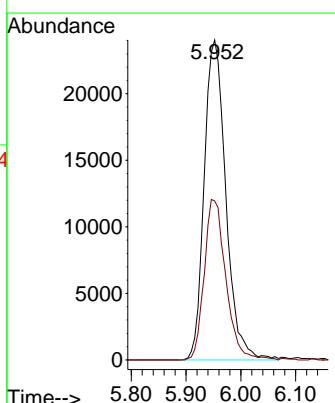

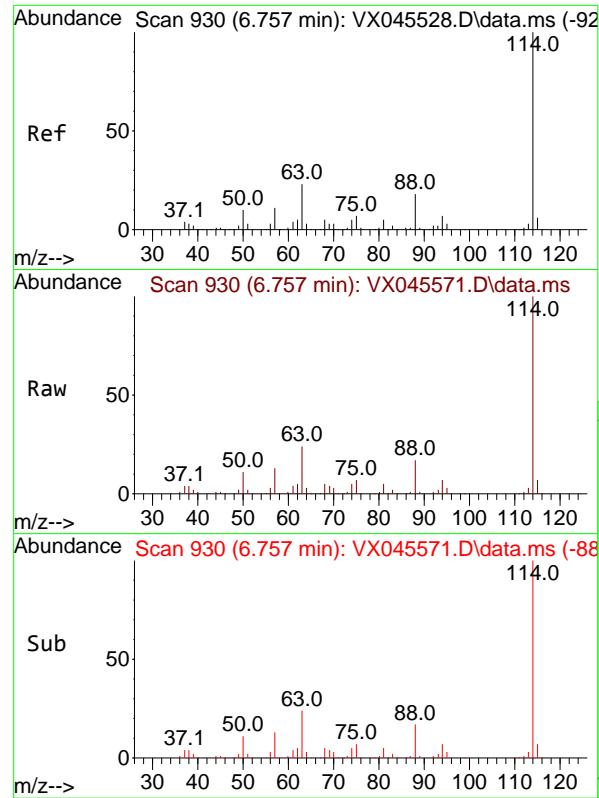

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 9

Delta R.T. 0.000 min

Lab File: VX045571.D

Acq: 03 Apr 2025 15:14

Instrument:

MSVOA\_X

ClientSampleId :

TB01-040225

Tgt Ion:114 Resp: 129076

Ion Ratio Lower Upper

114 100

63 24.4 0.0 46.8

88 17.0 0.0 35.4

Abundance

50000

40000



30000

20000

10000

0

Time--&gt;

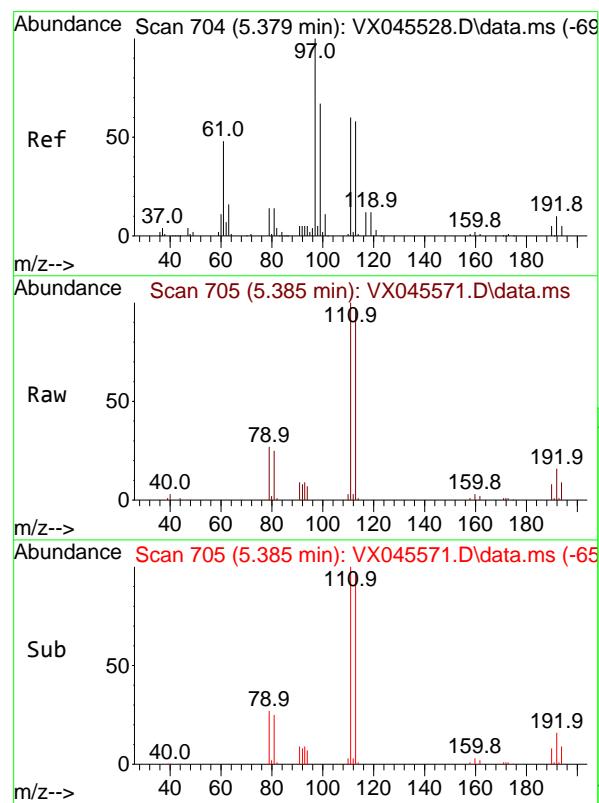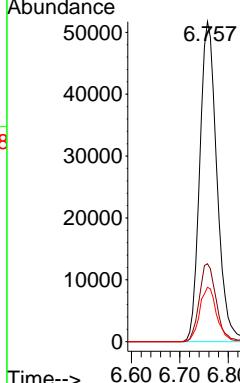

#35

Dibromofluoromethane

Concen: 52.048 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX045571.D

Acq: 03 Apr 2025 15:14

Tgt Ion:113 Resp: 47665

Ion Ratio Lower Upper

113 100

111 104.5 81.8 122.6

192 16.6 13.8 20.6

Abundance


15000




10000

5000

0

Time--&gt;




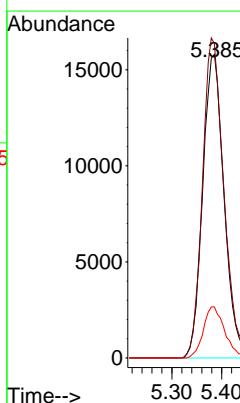


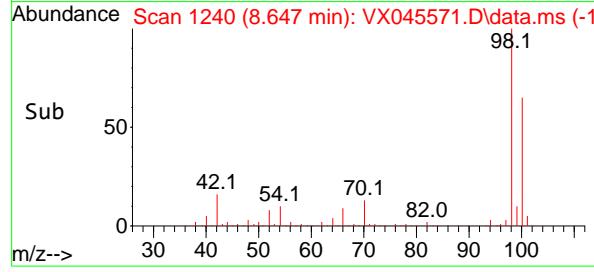

#50  
Toluene-d8  
Concen: 50.960 ug/l  
RT: 8.647 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045571.D  
Acq: 03 Apr 2025 15:14


Instrument : MSVOA\_X  
ClientSampleId : TB01-040225


Tgt Ion: 98 Resp: 162893  
Ion Ratio Lower Upper  
98 100  
100 64.5 52.2 78.4

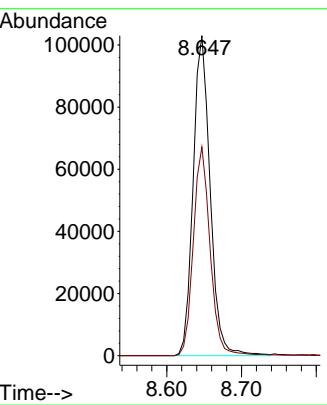

#62  
4-Bromofluorobenzene  
Concen: 51.044 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.000 min  
Lab File: VX045571.D  
Acq: 03 Apr 2025 15:14



Tgt Ion: 95 Resp: 59432  
Ion Ratio Lower Upper  
95 100  
174 68.6 0.0 135.8  
176 66.0 0.0 131.4

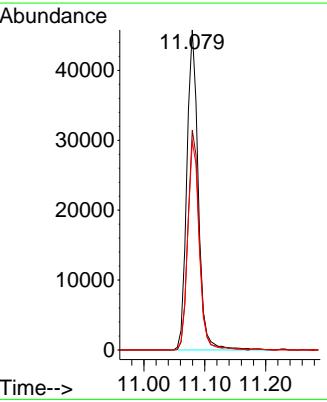

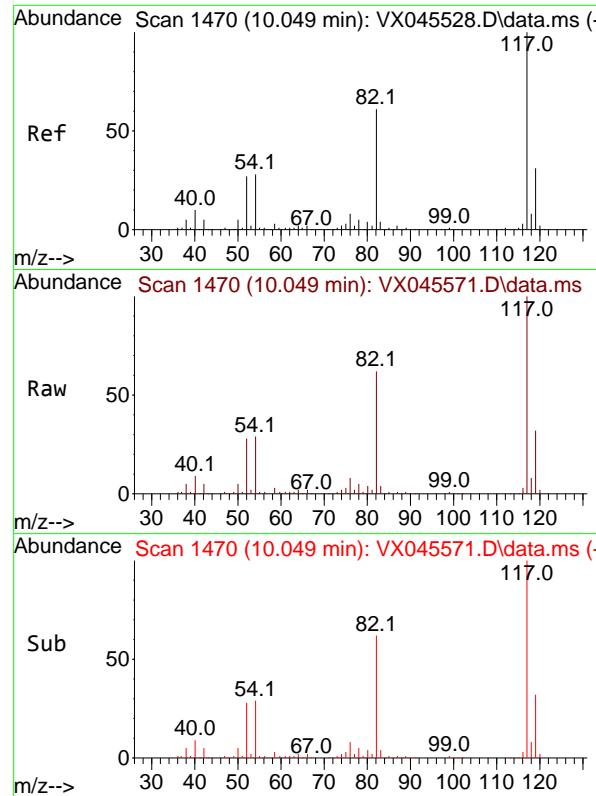


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045571.D ClientSampleId :  
Acq: 03 Apr 2025 15:14 TB01-040225

Tgt Ion:117 Resp: 121728  
Ion Ratio Lower Upper  
117 100  
82 61.7 49.2 73.8  
119 31.7 25.1 37.7

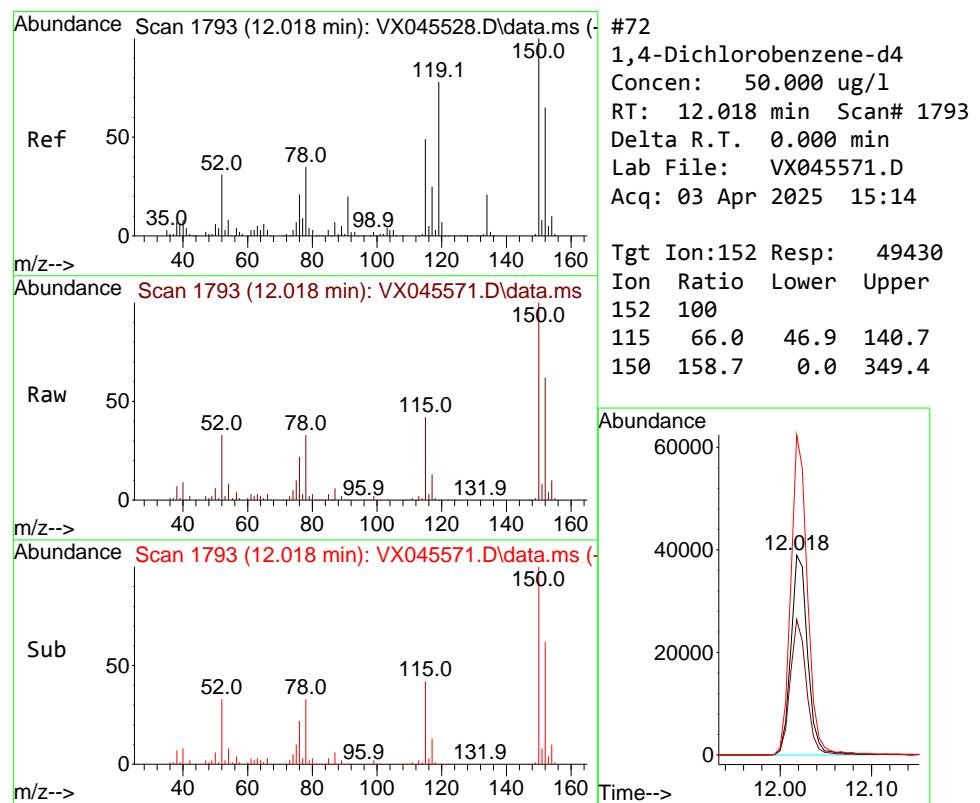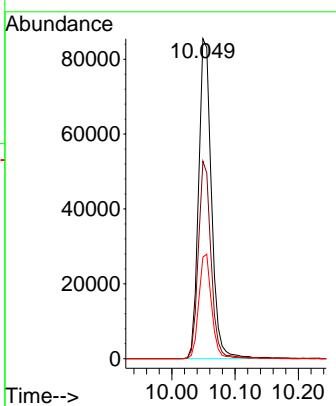

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. 0.000 min  
Lab File: VX045571.D  
Acq: 03 Apr 2025 15:14

Tgt Ion:152 Resp: 49430  
Ion Ratio Lower Upper  
152 100  
115 66.0 46.9 140.7  
150 158.7 0.0 349.4

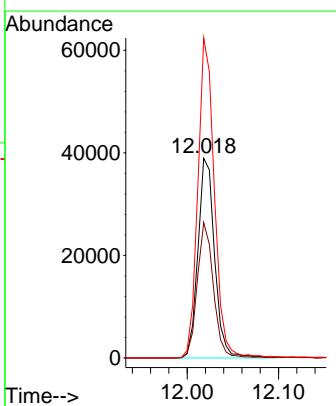



# CALIBRATION

# SUMMARY

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: CHEMTECH  
 Lab Code: CHEM Case No.: Q1711  
 Instrument ID: MSVOA\_X  
 Heated Purge: (Y/N) N  
 GC Column: DB-624UI ID: 0.18 (mm)

Contract: JAC005  
 SAS No.: Q1711 SDG No.: Q1711  
 Calibration Date(s): 04/01/2025 04/01/2025  
 Calibration Time(s): 17:06 19:02

LAB FILE ID:	RRF001 = VX045525.D	RRF005 = VX045526.D	RRF020 = VX045527.D					
COMPOUND	RRF001	RRF005	RRF020	RRF050	RRF100	RRF150	RRF	% RSD
Vinyl Chloride	0.671	0.662	0.701	0.716	0.738	0.730	0.703	4.4
1,1-Dichloroethene	0.563	0.588	0.612	0.604	0.618	0.616	0.600	3.5
1,1-Dichloroethane	1.211	1.240	1.318	1.269	1.283	1.292	1.269	3
cis-1,2-Dichloroethene	0.762	0.696	0.760	0.751	0.754	0.760	0.747	3.4
1,1,1-Trichloroethane	1.028	1.052	1.120	1.109	1.153	1.167	1.105	5
Benzene	1.414	1.416	1.519	1.481	1.483	1.465	1.463	2.8
1,2-Dichloroethane	0.533	0.585	0.649	0.622	0.620	0.617	0.604	6.7
Trichloroethene	0.349	0.322	0.356	0.351	0.351	0.356	0.348	3.7
1,1,2-Trichloroethane	0.337	0.346	0.376	0.359	0.358	0.340	0.353	4.1
Tetrachloroethene	0.346	0.373	0.371	0.347	0.333	0.347	0.353	4.5
1,2-Dichloroethane-d4		0.962	0.900	0.868	0.904	0.937	0.914	3.9
Dibromofluoromethane		0.372	0.342	0.345	0.353	0.362	0.355	3.5
Toluene-d8		1.257	1.233	1.214	1.230	1.257	1.238	1.5
4-Bromofluorobenzene		0.413	0.448	0.453	0.481	0.460	0.451	5.5

\* Compounds with required minimum RRF and maximum %RSD values.

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.

Method Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\

Method File : 82X040225W.M

Title : SW846 8260

Last Update : Wed Apr 02 03:11:43 2025

Response Via : Initial Calibration

## Calibration Files

1 =VX045525.D 5 =VX045526.D 20 =VX045527.D 50 =VX045528.D 100 =VX045529.D 150 =VX045530.D

	Compound	1	5	20	50	100	150	Avg	%RSD
<hr/>									
1) I	Pentafluorobenzene	-----	-----	ISTD-----					
2) T	Dichlorodifluo...	0.615	0.695	0.700	0.820	0.837	0.820	0.748	12.13
3) P	Chloromethane	0.764	0.734	0.777	0.784	0.815	0.734	0.768	4.05
4) C	Vinyl Chloride	0.671	0.662	0.701	0.716	0.738	0.730	0.703	4.43#
5) T	Bromomethane	0.342	0.327	0.330	0.341	0.327	0.333		2.20
6) T	Chloroethane	0.378	0.397	0.390	0.398	0.355	0.319	0.373	8.27
7) T	Trichlorofluor...	1.051	0.999	1.075	1.086	1.089	0.989	1.048	4.22
8) T	Diethyl Ether	0.345	0.340	0.356	0.355	0.358	0.357	0.352	2.11
9) T	1,1,2-Trichlor...	0.575	0.599	0.635	0.621	0.621	0.634	0.614	3.74
10) T	Methyl Iodide	0.705	0.789	0.799	0.788	0.750	0.766		5.08
11) T	Tert butyl alc...	0.111	0.124	0.127	0.128	0.124	0.123		5.44
12) CM	1,1-Dichloroet...	0.563	0.588	0.612	0.604	0.618	0.616	0.600	3.51#
13) T	Acrolein	0.176	0.161	0.167	0.170	0.172	0.169		3.41
14) T	Allyl chloride	1.092	1.068	1.142	1.172	1.199	1.160	1.139	4.36
15) T	Acrylonitrile	0.356	0.382	0.413	0.407	0.394	0.376	0.388	5.38
16) T	Acetone	0.400	0.369	0.387	0.378	0.365	0.355	0.375	4.28
17) T	Carbon Disulfide	1.334	1.327	1.434	1.553	1.604	1.642	1.483	9.24
18) T	Methyl Acetate	0.901	0.863	0.864	0.857	0.855	0.846	0.864	2.22
19) T	Methyl tert-bu...	1.915	1.964	2.169	2.118	2.217	2.216	2.100	6.20
20) T	Methylene Chlo...	0.692	0.695	0.726	0.709	0.705	0.690	0.703	1.96
21) T	trans-1,2-Dich...	0.574	0.594	0.636	0.624	0.621	0.630	0.613	3.94
22) T	Diisopropyl ether	2.003	2.120	2.329	2.293	2.359	2.357	2.243	6.59
23) T	Vinyl Acetate	1.542	1.693	2.005	2.087	2.147	2.156	1.938	13.34
24) P	1,1-Dichloroet...	1.211	1.240	1.318	1.269	1.283	1.292	1.269	3.01
25) T	2-Butanone	0.474	0.537	0.582	0.586	0.571	0.548	0.550	7.55
26) T	2,2-Dichloropr...	0.676	0.757	0.802	0.847	0.903	0.933	0.820	11.67
27) T	cis-1,2-Dichlo...	0.762	0.696	0.760	0.751	0.754	0.760	0.747	3.43
28) T	Bromochloromet...	0.671	0.608	0.617	0.596	0.610	0.576	0.613	5.18
29) T	Tetrahydrofuran	0.339	0.341	0.371	0.371	0.364	0.352	0.356	4.05
30) C	Chloroform	1.244	1.309	1.348	1.315	1.309	1.309	1.306	2.60#
31) T	Cyclohexane	1.044	1.148	1.123	1.145	1.149	1.122		4.00
32) T	1,1,1-Trichlor...	1.028	1.052	1.120	1.109	1.153	1.167	1.105	4.96
33) S	1,2-Dichloroet...	0.962	0.900	0.868	0.904	0.937	0.914		3.94
34) I	1,4-Difluorobenzene	-----	-----	ISTD-----					
35) S	Dibromofluorom...	0.372	0.342	0.345	0.353	0.362	0.355		3.48
36) T	1,1-Dichloropr...	0.477	0.443	0.474	0.485	0.496	0.499	0.479	4.26
37) T	Ethyl Acetate	0.582	0.565	0.609	0.623	0.629	0.614	0.604	4.15
38) T	Carbon Tetrach...	0.450	0.497	0.521	0.536	0.545	0.556	0.518	7.49
39) T	Methylcyclohexane	0.519	0.527	0.596	0.622	0.628	0.632	0.587	8.76
40) TM	Benzene	1.414	1.416	1.519	1.481	1.483	1.465	1.463	2.81
41) T	Methacrylonitrile	0.252	0.276	0.338	0.351	0.350	0.343	0.318	13.52
42) TM	1,2-Dichloroet...	0.533	0.585	0.649	0.622	0.620	0.617	0.604	6.72
43) T	Isopropyl Acetate	0.735	0.831	0.952	0.978	1.002	0.991	0.915	11.77
44) TM	Trichloroethene	0.349	0.322	0.356	0.351	0.351	0.356	0.348	3.67
45) C	1,2-Dichloropr...	0.309	0.365	0.388	0.376	0.379	0.374	0.365	7.83#
46) T	Dibromomethane	0.237	0.287	0.297	0.292	0.286	0.282	0.280	7.76
47) T	Bromodichlorom...	0.521	0.519	0.576	0.571	0.587	0.583	0.560	5.56
48) T	Methyl methacr...	0.405	0.416	0.486	0.508	0.518	0.502	0.472	10.44
49) T	1,4-Dioxane	0.007	0.010	0.009	0.009	0.009	0.008	0.009	13.93
50) S	Toluene-d8	1.257	1.233	1.214	1.230	1.257	1.238		1.50
51) T	4-Methyl-2-Pen...	0.499	0.578	0.661	0.663	0.647	0.589	0.606	10.57
52) CM	Toluene	0.817	0.866	0.939	0.910	0.905	0.875	0.885	4.79#
53) T	t-1,3-Dichloro...	0.316	0.400	0.465	0.508	0.555	0.558	0.467	20.27
54) T	cis-1,3-Dichlo...	0.371	0.474	0.546	0.568	0.597	0.600	0.526	16.88
55) T	1,1,2-Trichlor...	0.337	0.346	0.376	0.359	0.358	0.340	0.353	4.11
56) T	Ethyl methacry...	0.407	0.482	0.562	0.600	0.629	0.595	0.546	15.54

		Method Path : Z:\voasrv\HPCHEM1\MSVOA_X\Method\ Method File : 82X040225W.M										
57)	T	1,3-Dichloropr...	0.555	0.614	0.652	0.633	0.630	0.601	0.614	5.49		
58)	T	2-Chloroethyl ...	0.221	0.257	0.286	0.298	0.301	0.293	0.276	11.26	1	
59)	T	2-Hexanone	0.363	0.429	0.488	0.492	0.484	0.439	0.449	11.14	2	
60)	T	Dibromochlorom...	0.313	0.352	0.404	0.412	0.421	0.405	0.385	11.06	3	
61)	T	1,2-Dibromoethane	0.294	0.351	0.380	0.373	0.380	0.364	0.357	9.12	4	
62)	S	4-Bromofluorob...	0.413	0.448	0.453	0.481	0.460	0.451	5.45	5		
63)	I	Chlorobenzene-d5	-----ISTD-----									
64)	T	Tetrachloroethene	0.346	0.373	0.371	0.347	0.333	0.347	0.353	4.47	6	
65)	PM	Chlorobenzene	0.951	1.054	1.123	1.084	1.086	1.112	1.068	5.83	7	
66)	T	1,1,1,2-Tetra...	0.368	0.344	0.372	0.373	0.379	0.390	0.371	4.18	8	
67)	C	Ethyl Benzene	1.608	1.819	2.002	2.007	1.993	2.053	1.914	8.89#	9	
68)	T	m/p-Xylenes	0.594	0.669	0.732	0.728	0.723	0.729	0.696	7.92	10	
69)	T	o-Xylene	0.562	0.676	0.725	0.719	0.716	0.714	0.686	9.17	11	
70)	T	Styrene	0.897	1.043	1.202	1.216	1.230	1.202	1.132	11.82	12	
71)	P	Bromoform	0.220	0.252	0.272	0.296	0.307	0.315	0.277	13.07	13	
72)	I	1,4-Dichlorobenzen...	-----ISTD-----									
73)	T	Isopropylbenzene	3.581	3.850	4.224	4.181	4.043	4.151	4.005	6.17	14	
74)	T	N-amyl acetate	1.442	1.682	1.960	2.058	2.132	2.221	1.916	15.51	15	
75)	P	1,1,2,2-Tetra...	1.457	1.428	1.461	1.384	1.354	1.358	1.407	3.43	16	
76)	T	1,2,3-Trichlor...	1.221	1.257	1.251	1.225	1.192	1.171	1.220	2.71	17	
77)	T	Bromobenzene	0.877	0.927	0.953	0.938	0.925	0.932	0.925	2.77	18	
78)	T	n-propylbenzene	3.734	4.346	5.012	4.896	4.819	4.872	4.613	10.59	19	
79)	T	2-Chlorotoluene	2.894	2.873	3.130	2.966	2.915	2.918	2.949	3.19	20	
80)	T	1,3,5-Trimethyl...	2.931	3.119	3.571	3.511	3.367	3.371	3.312	7.35	21	
81)	T	trans-1,4-Dich...	0.274	0.323	0.371	0.401	0.428	0.359		17.16	22	
82)	T	4-Chlorotoluene	2.961	3.156	3.470	3.449	3.350	3.343	3.288	5.93	23	
83)	T	tert-Butylbenzene	2.894	3.124	3.437	3.427	3.387	3.405	3.279	6.78	24	
84)	T	1,2,4-Trimethyl...	2.906	3.129	3.529	3.523	3.438	3.420	3.324	7.57	25	
85)	T	sec-Butylbenzene	3.195	3.828	4.316	4.300	4.232	4.292	4.027	11.12	26	
86)	T	p-Isopropyltol...	2.734	3.157	3.515	3.524	3.506	3.484	3.320	9.63	27	
87)	T	1,3-Dichlorobe...	1.658	1.605	1.726	1.699	1.714	1.706	1.684	2.70	28	
88)	T	1,4-Dichlorobe...	1.671	1.724	1.768	1.703	1.674	1.706	1.708	2.09	29	
89)	T	n-Butylbenzene	2.117	2.486	2.974	3.160	3.256	3.283	2.879	16.50	30	
90)	T	Hexachloroethane	0.493	0.493	0.556	0.597	0.623	0.661	0.571	12.14	31	
91)	T	1,2-Dichlorobe...	1.644	1.645	1.750	1.678	1.665	1.667	1.675	2.34	32	
92)	T	1,2-Dibromo-3...	0.196	0.260	0.312	0.316	0.333	0.349	0.294	19.37	33	
93)	T	1,2,4-Trichlor...	0.727	0.844	0.948	0.947	1.045	1.083	0.932	14.07	34	
94)	T	Hexachlorobuta...	0.379	0.389	0.401	0.404	0.415	0.422	0.402	4.03	35	
95)	T	Naphthalene	2.544	3.070	3.630	3.722	3.867	3.982	3.469	15.93	36	
96)	T	1,2,3-Trichlor...	0.782	0.916	0.999	1.000	1.063	1.097	0.976	11.63	37	

(#= Out of Range)

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045525.D  
 Acq On : 01 Apr 2025 17:06  
 Operator : JC/MD  
 Sample : VSTDICC001  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC001

Quant Time: Apr 02 02:50:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	96737	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	175266	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	153312	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	61114	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	0.000	65	0d	0.000	ug/l	
Spiked Amount 50.000	Range 74 - 125		Recovery	=	0.000%#	
35) Dibromofluoromethane	0.000	113	0d	0.000	ug/l	
Spiked Amount 50.000	Range 75 - 124		Recovery	=	0.000%#	
50) Toluene-d8	0.000	98	0d	0.000	ug/l	
Spiked Amount 50.000	Range 86 - 113		Recovery	=	0.000%#	
62) 4-Bromofluorobenzene	0.000	95	0d	0.000	ug/l	
Spiked Amount 50.000	Range 77 - 121		Recovery	=	0.000%#	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.167	85	1189	0.822	ug/l	94
3) Chloromethane	1.307	50	1479	0.995	ug/l #	86
4) Vinyl Chloride	1.374	62	1299	0.955	ug/l	98
6) Chloroethane	1.673	64	732	1.014	ug/l #	67
7) Trichlorofluoromethane	1.880	101	2034	1.003	ug/l	93
8) Diethyl Ether	2.130	74	668	0.981	ug/l	83
9) 1,1,2-Trichlorotrifluo...	2.325	101	1113	0.936	ug/l	94
12) 1,1-Dichloroethene	2.313	96	1090	0.939	ug/l	95
14) Allyl chloride	2.660	41	2113	0.959	ug/l	93
15) Acrylonitrile	3.075	53	3446	4.592	ug/l	95
16) Acetone	2.380	43	3867	5.323	ug/l	98
17) Carbon Disulfide	2.508	76	2580	0.899	ug/l #	95
18) Methyl Acetate	2.703	43	1744	1.043	ug/l	91
19) Methyl tert-butyl Ether	3.117	73	3705	0.912	ug/l	92
20) Methylene Chloride	2.782	84	1338	0.984	ug/l	91
21) trans-1,2-Dichloroethene	3.087	96	1111	0.936	ug/l #	93
22) Diisopropyl ether	3.758	45	3875	0.893	ug/l #	59
23) Vinyl Acetate	3.727	43	14921	3.979	ug/l	95
24) 1,1-Dichloroethane	3.611	63	2343	0.954	ug/l #	90
25) 2-Butanone	4.581	43	4590	4.317	ug/l	92
26) 2,2-Dichloropropane	4.471	77	1307	0.824	ug/l	85
27) cis-1,2-Dichloroethene	4.495	96	1475	1.020	ug/l	80
28) Bromochloromethane	4.891	49	1298	1.094	ug/l #	97
29) Tetrahydrofuran	5.032	42	3276	4.752	ug/l	97
30) Chloroform	5.093	83	2406	0.953	ug/l	84
32) 1,1,1-Trichloroethane	5.385	97	1989	0.931	ug/l #	53
36) 1,1-Dichloropropene	5.696	75	1671	0.995	ug/l #	89
37) Ethyl Acetate	4.751	43	2040	0.964	ug/l #	76
38) Carbon Tetrachloride	5.672	117	1578	0.870	ug/l #	91
39) Methylcyclohexane	7.379	83	1818	0.883	ug/l #	89
40) Benzene	6.038	78	4957	0.967	ug/l	97
41) Methacrylonitrile	4.952	41	883m	0.784	ug/l	
42) 1,2-Dichloroethane	6.092	62	1867	0.882	ug/l	86
43) Isopropyl Acetate	6.361	43	2578	0.804	ug/l #	86
44) Trichloroethene	7.123	130	1224	1.004	ug/l	87
45) 1,2-Dichloropropane	7.434	63	1082	0.846	ug/l	90

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045525.D  
 Acq On : 01 Apr 2025 17:06  
 Operator : JC/MD  
 Sample : VSTDICC001  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC001

Quant Time: Apr 02 02:50:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) Dibromomethane	7.592	93	831	0.846	ug/1	90
47) Bromodichloromethane	7.824	83	1827	0.931	ug/1 #	77
48) Methyl methacrylate	7.720	41	1419	0.857	ug/1	92
49) 1,4-Dioxane	7.671	88	458m	15.288	ug/1	
51) 4-Methyl-2-Pentanone	8.574	43	8746	4.114	ug/1	100
52) Toluene	8.720	92	2863	0.923	ug/1	96
53) t-1,3-Dichloropropene	8.988	75	1109	2.850	ug/1	93
54) cis-1,3-Dichloropropene	8.379	75	1300	0.705	ug/1	90
55) 1,1,2-Trichloroethane	9.159	97	1183	0.957	ug/1 #	76
56) Ethyl methacrylate	9.129	69	1425m	0.745	ug/1	
57) 1,3-Dichloropropane	9.311	76	1946	0.904	ug/1	91
58) 2-Chloroethyl Vinyl ether	8.245	63	3880	4.008	ug/1	93
59) 2-Hexanone	9.439	43	6360	4.040	ug/1	85
60) Dibromochloromethane	9.519	129	1097	0.814	ug/1	99
61) 1,2-Dibromoethane	9.610	107	1032	0.825	ug/1	96
64) Tetrachloroethene	9.269	164	1062	0.981	ug/1	92
65) Chlorobenzene	10.080	112	2916	0.890	ug/1	95
66) 1,1,1,2-Tetrachloroethane	10.159	131	1128	0.992	ug/1 #	64
67) Ethyl Benzene	10.195	91	4930	0.840	ug/1	90
68) m/p-Xylenes	10.305	106	3645	1.708	ug/1	97
69) o-Xylene	10.640	106	1724	0.820	ug/1	83
70) Styrene	10.659	104	2750	0.793	ug/1	94
71) Bromoform	10.805	173	675	0.795	ug/1 #	94
73) Isopropylbenzene	10.964	105	4377	0.894	ug/1	95
74) N-amyl acetate	10.854	43	1762	0.752	ug/1 #	93
75) 1,1,2,2-Tetrachloroethane	11.214	83	1781	1.036	ug/1	94
76) 1,2,3-Trichloropropane	11.244	75	1493m	1.002	ug/1	
77) Bromobenzene	11.201	156	1072	0.948	ug/1	95
78) n-propylbenzene	11.305	91	4564	0.809	ug/1	97
79) 2-Chlorotoluene	11.366	91	3537	0.981	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	3582	0.885	ug/1	100
82) 4-Chlorotoluene	11.457	91	3619	0.900	ug/1	96
83) tert-Butylbenzene	11.713	119	3537	0.883	ug/1	94
84) 1,2,4-Trimethylbenzene	11.750	105	3552	0.874	ug/1	99
85) sec-Butylbenzene	11.890	105	3905	0.793	ug/1	98
86) p-Isopropyltoluene	12.012	119	3342	0.824	ug/1	94
87) 1,3-Dichlorobenzene	11.969	146	2026	0.984	ug/1	97
88) 1,4-Dichlorobenzene	12.043	146	2042m	0.978	ug/1	
89) n-Butylbenzene	12.335	91	2587	0.735	ug/1	99
90) Hexachloroethane	12.543	117	602	0.863	ug/1	95
91) 1,2-Dichlorobenzene	12.335	146	2009	0.981	ug/1	93
92) 1,2-Dibromo-3-Chloropr...	12.945	75	239	0.665	ug/1 #	73
93) 1,2,4-Trichlorobenzene	13.591	180	888	0.779	ug/1	94
94) Hexachlorobutadiene	13.725	225	463	0.943	ug/1	90
95) Naphthalene	13.780	128	3109	0.733	ug/1	99
96) 1,2,3-Trichlorobenzene	13.969	180	956	0.801	ug/1	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045525.D  
 Acq On : 01 Apr 2025 17:06  
 Operator : JC/MD  
 Sample : VSTDICC001  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 3 Sample Multiplier: 1







Quant Time: Apr 02 02:50:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDICC001**

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

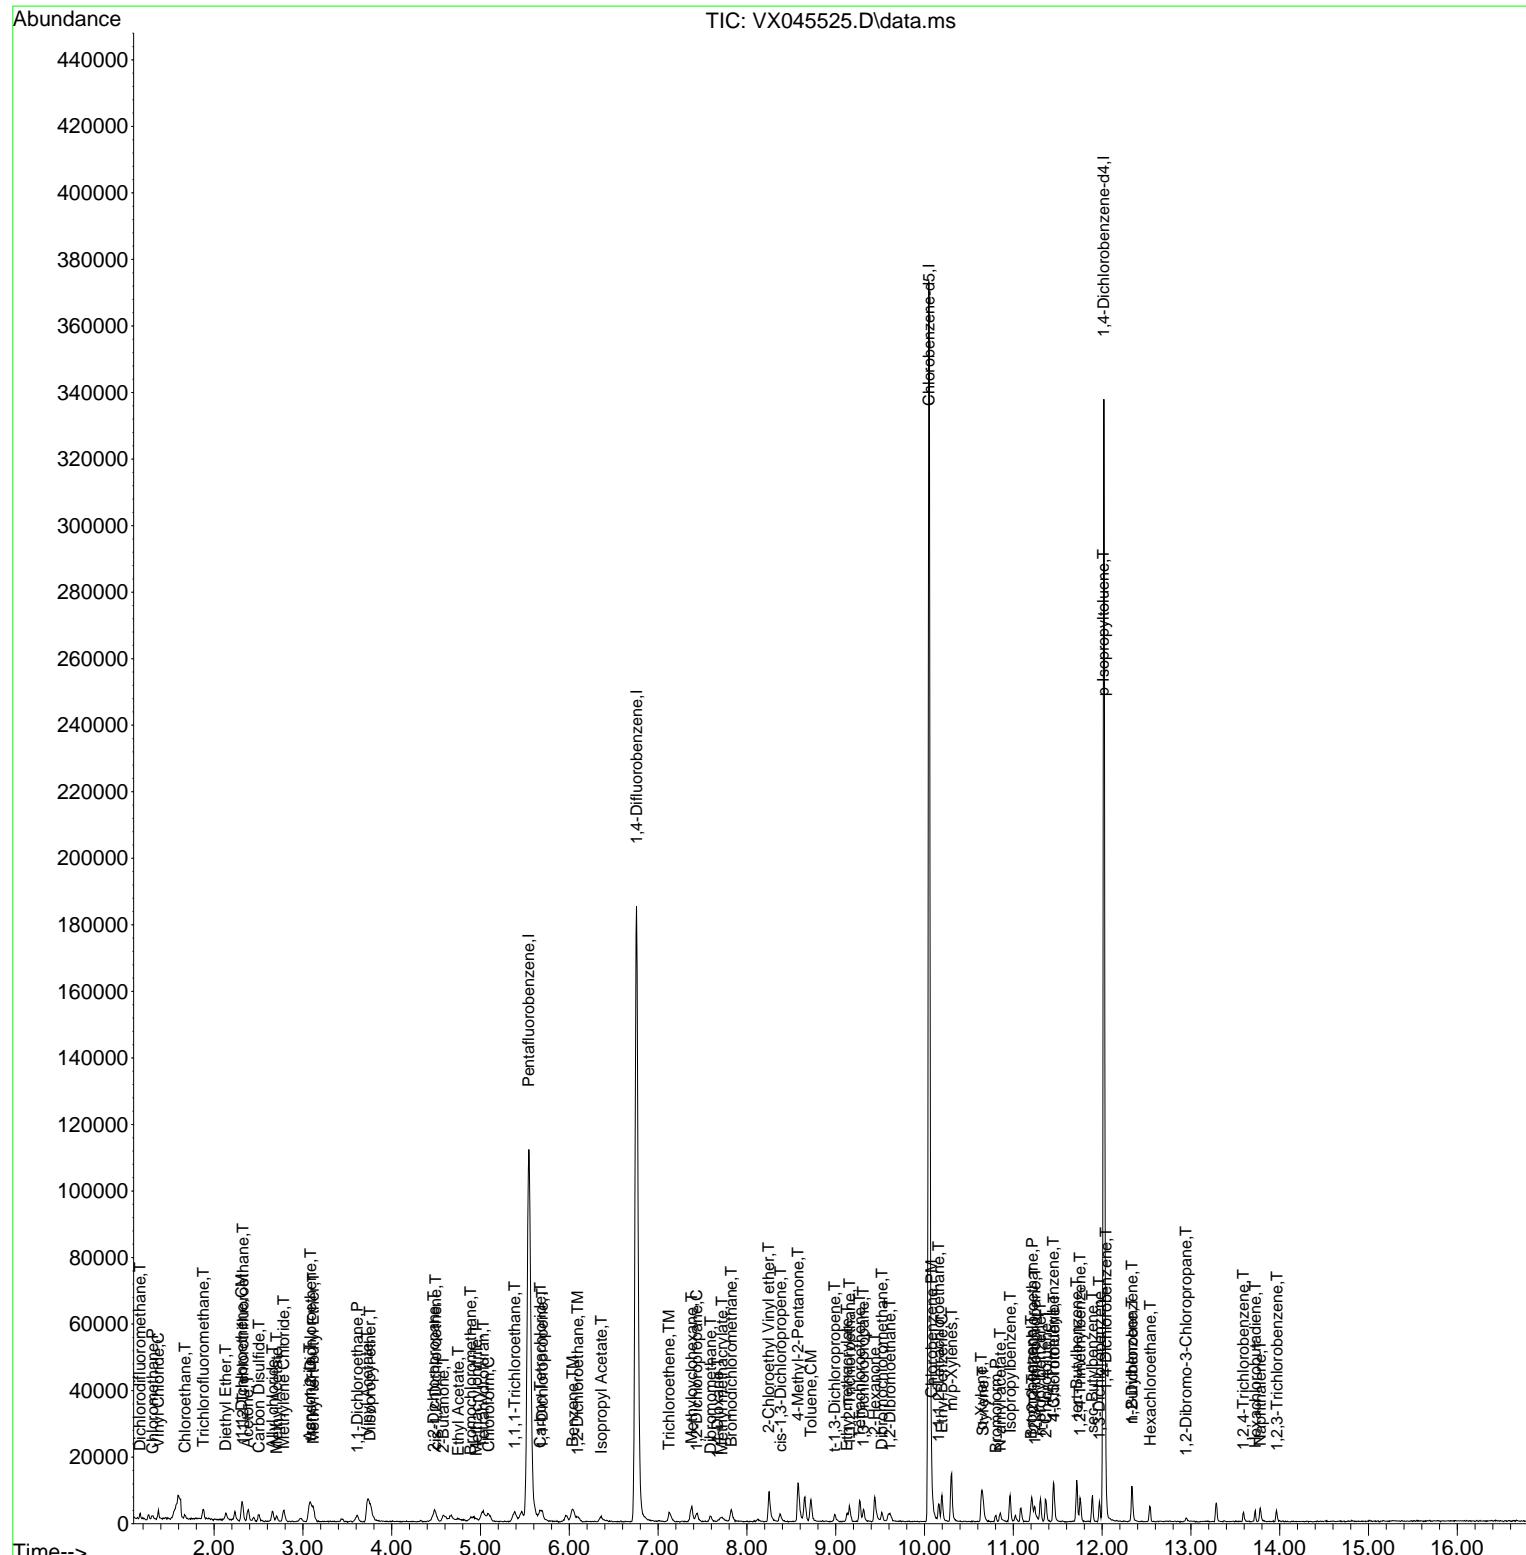

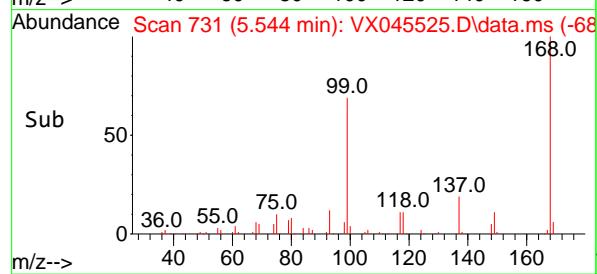

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.544 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#2

Dichlorodifluoromethane

Concen: 0.822 ug/l

RT: 1.167 min Scan# 13

Delta R.T. 0.000 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06


Tgt Ion: 85 Resp: 1189

Ion Ratio Lower Upper


85 100

87 35.5 16.1 48.2

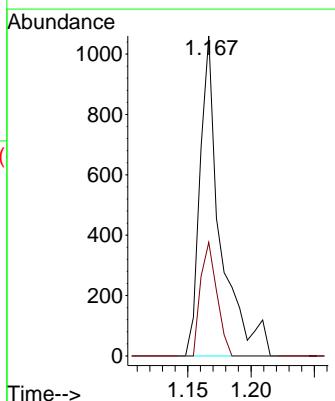



Abundance Scan 36 (1.307 min): VX045525.D\data.ms

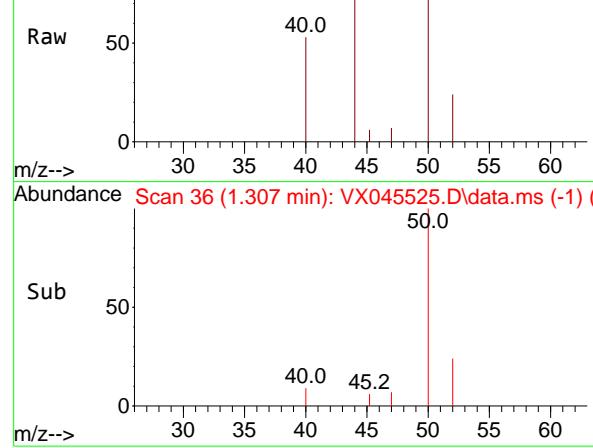

#3

Chloromethane

Concen: 0.995 ug/l

RT: 1.307 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC001


**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



Abundance Scan 47 (1.374 min): VX045525.D\data.ms

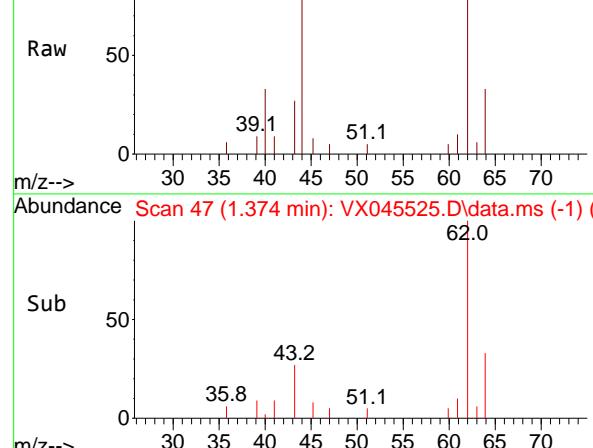

#4

Vinyl Chloride

Concen: 0.955 ug/l


RT: 1.374 min Scan# 47







Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt Ion: 62 Resp: 1299  
 Ion Ratio Lower Upper  
 62 100  
 64 32.9 25.5 38.3

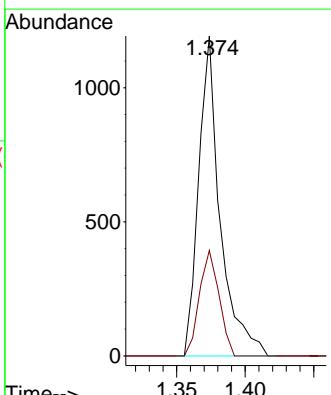

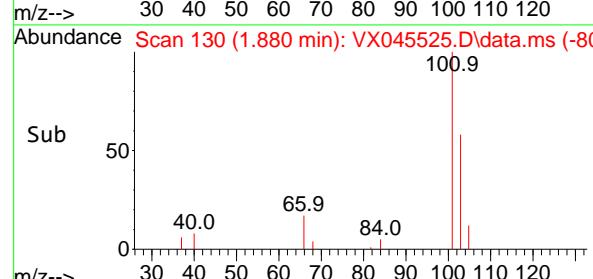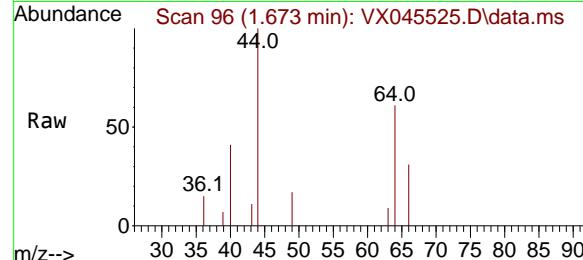

#6

Chloroethane

Concen: 1.014 ug/l

RT: 1.673 min Scan# 9

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

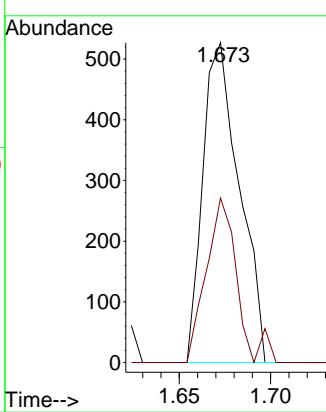

#7

Trichlorofluoromethane

Concen: 1.003 ug/l


RT: 1.880 min Scan# 130


Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt Ion:101 Resp: 2034  
 Ion Ratio Lower Upper  
 101 100  
 103 58.3 51.1 76.7

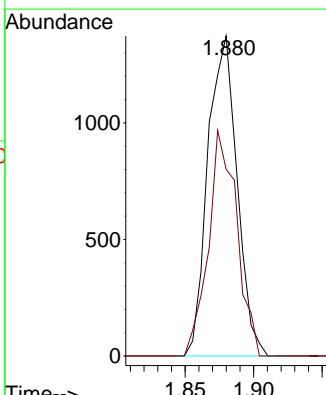


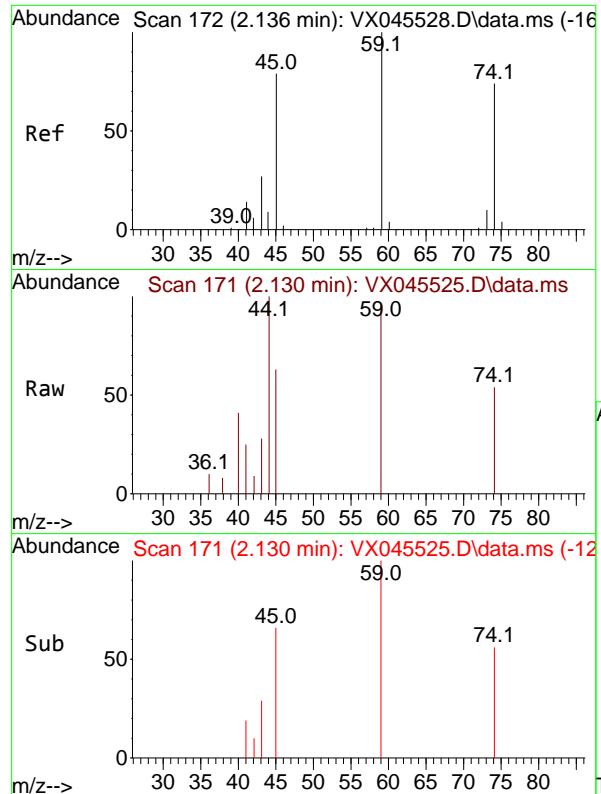


#8  
 Diethyl Ether  
 Concen: 0.981 ug/l  
 RT: 2.130 min Scan# 1  
 Delta R.T. -0.006 min  
 Lab File: VX045525.D  
 Acq: 01 Apr 2025 17:06

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

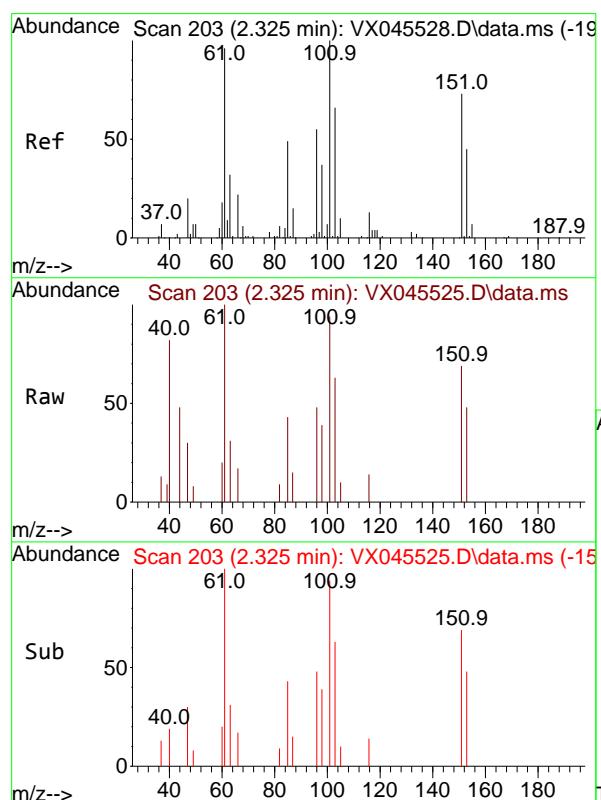

#9  
 1,1,2-Trichlorotrifluoroethane  
 Concen: 0.936 ug/l  
 RT: 2.325 min Scan# 203  
 Delta R.T. 0.000 min  
 Lab File: VX045525.D  
 Acq: 01 Apr 2025 17:06

Tgt Ion:101 Resp: 1113  
 Ion Ratio Lower Upper  
 101 100  
 85 48.7 38.9 58.3  
 151 80.3 57.5 86.3

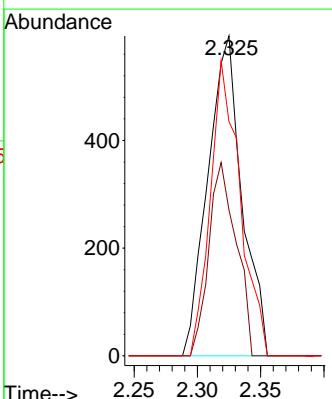

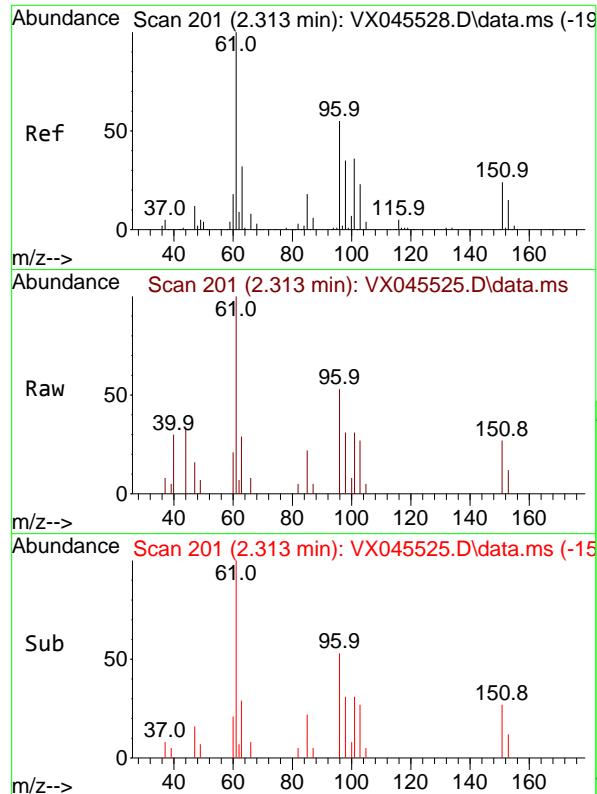

#12

1,1-Dichloroethene

Concen: 0.939 ug/l

RT: 2.313 min Scan# 201

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

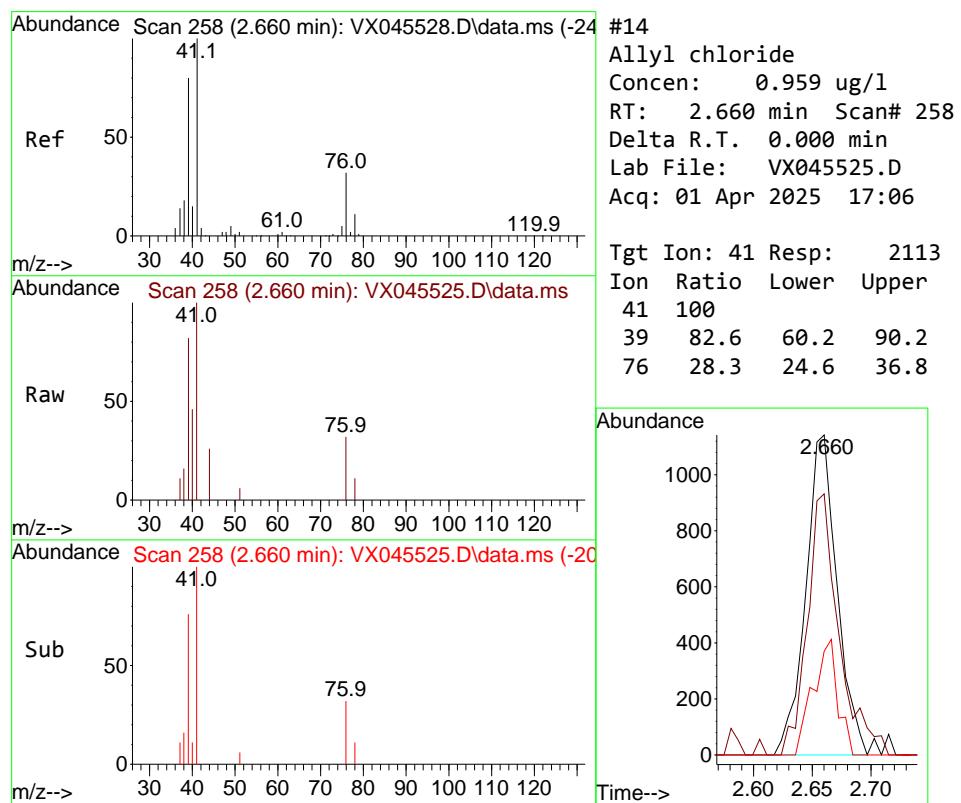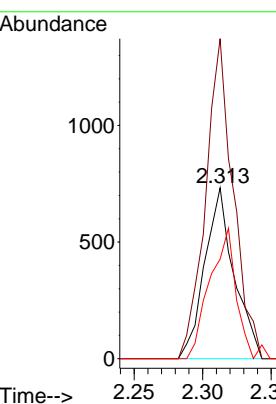

#14

Allyl chloride

Concen: 0.959 ug/l

RT: 2.660 min Scan# 258


Delta R.T. 0.000 min







Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt Ion: 41 Resp: 2113

Ion	Ratio	Lower	Upper
41	100		
39	82.6	60.2	90.2
76	28.3	24.6	36.8

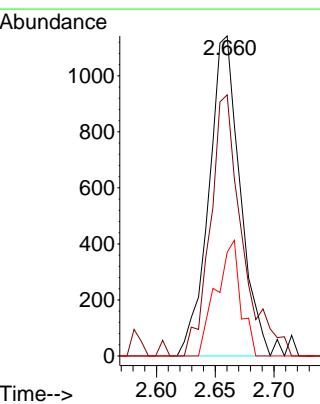



#15

**Acrylonitrile**

Concen: 4.592 ug/l

RT: 3.075 min Scan# 3

Delta R.T. 0.012 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC001

Tgt Ion: 53 Resp: 3440

Ion Ratio Lower Upper

53 100


52 89.4 67.4 101.2

51 40.1 29.9 44.9

**Manual Integrations****APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#16

**Acetone**

Concen: 5.323 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06




Tgt Ion: 43 Resp: 3867

Ion Ratio Lower Upper

43 100

58 29.2 22.3 33.5

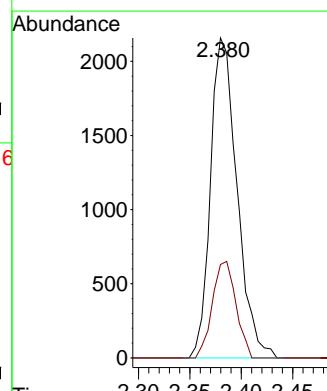



#17

Carbon Disulfide

Concen: 0.899 ug/l

RT: 2.508 min Scan# 233

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

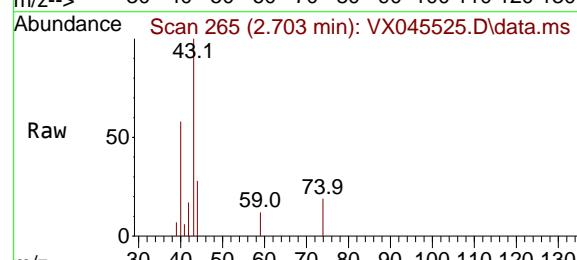

#18

Methyl Acetate

Concen: 1.043 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt Ion: 43 Resp: 1744

Ion Ratio Lower Upper

43 100

74 17.8 17.5 26.3



#19

Acetone

Concen: 0.999 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06


Tgt Ion: 57 Resp: 1744

Ion Ratio Lower Upper

57 100

74 17.8 17.5 26.3



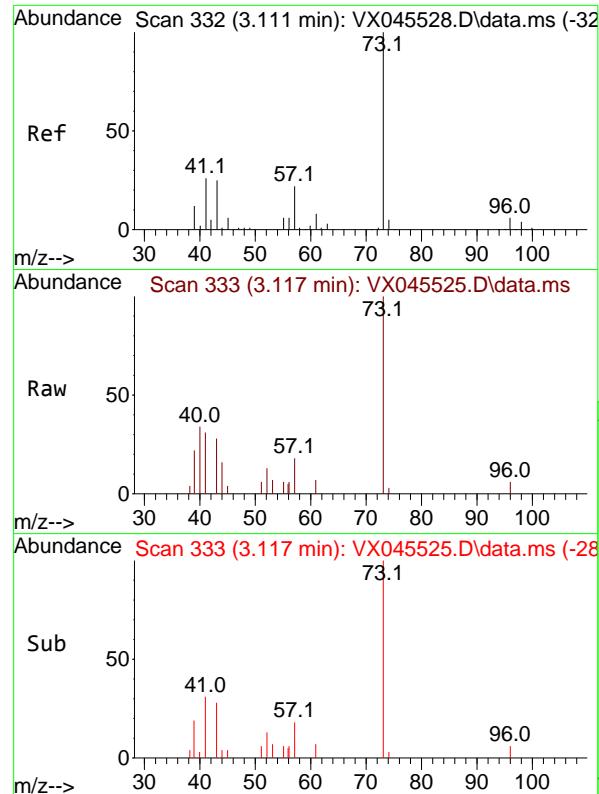



#19

Methyl tert-butyl Ether  
Concen: 0.912 ug/l  
RT: 3.117 min Scan# 3  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025


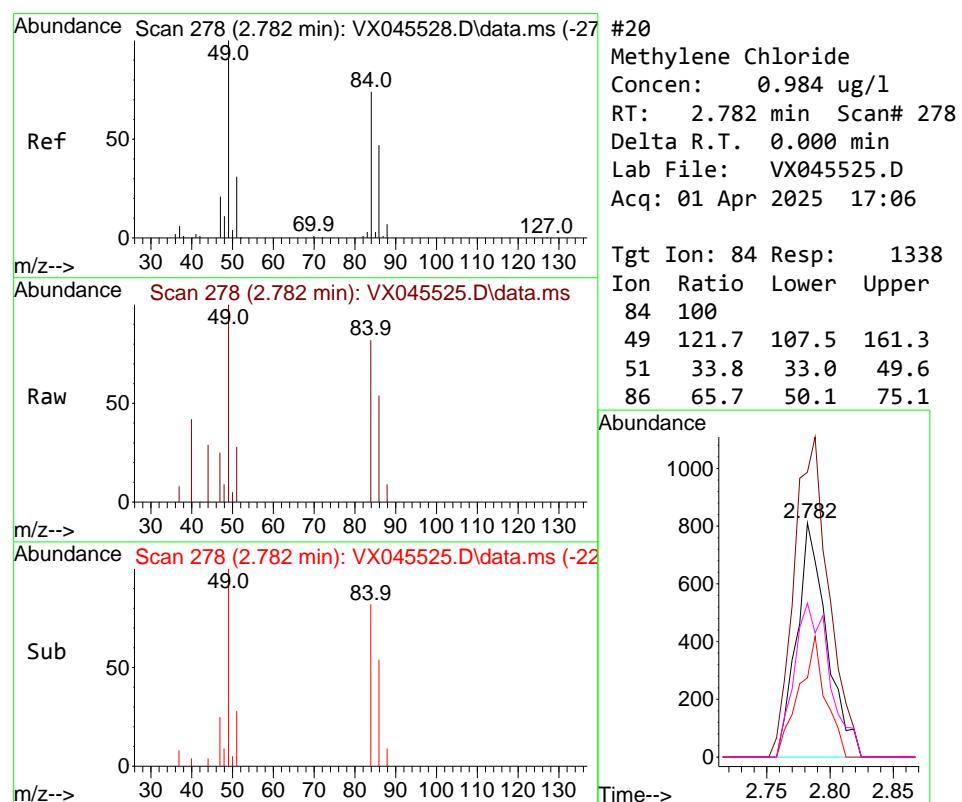



#20

Methylene Chloride  
Concen: 0.984 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion: 84 Resp: 1338  
Ion Ratio Lower Upper  
84 100  
49 121.7 107.5 161.3  
51 33.8 33.0 49.6  
86 65.7 50.1 75.1









#21  
trans-1,2-Dichloroethene  
Concen: 0.936 ug/l  
RT: 3.087 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025



#22  
Diisopropyl ether  
Concen: 0.893 ug/l  
RT: 3.758 min Scan# 438  
Delta R.T. -0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion: 45 Resp: 3875  
Ion Ratio Lower Upper  
45 100  
43 123.5 59.3 88.9#  
87 28.2 20.4 30.6  
59 8.0 9.0 13.6#

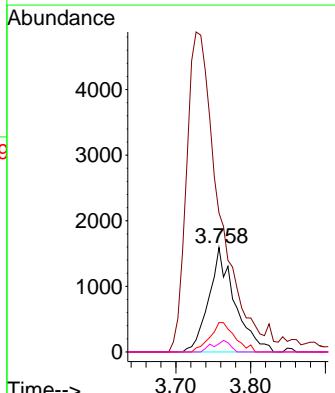



#23

## Vinyl Acetate



Concen: 3.979 ug/l

RT: 3.727 min Scan# 414

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

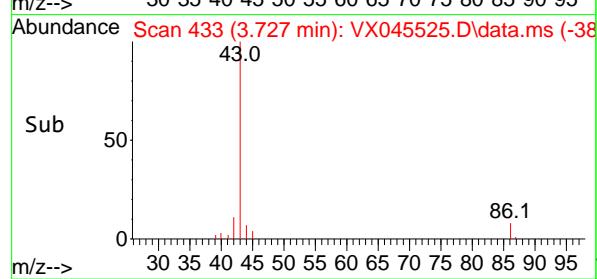

Tgt Ion: 43 Resp: 1492

Ion Ratio Lower Upper

43 100



86 7.7 7.5 11.3

## Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

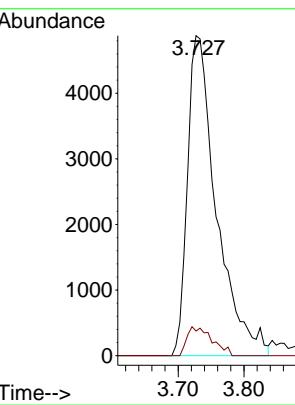

#24

## 1,1-Dichloroethane


Concen: 0.954 ug/l

RT: 3.611 min Scan# 414

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

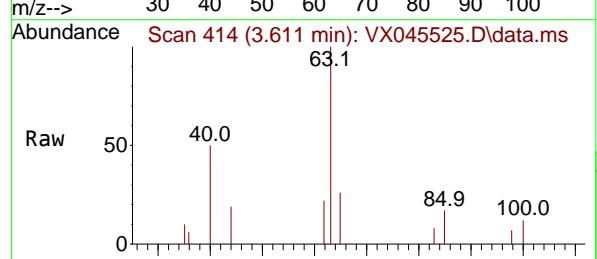



Tgt Ion: 63 Resp: 2343


Ion Ratio Lower Upper

63 100

98 7.4 3.4 10.1


100 11.6 2.2 6.6#

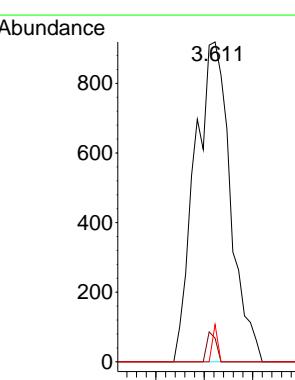



#25  
2-Butanone  
Concen: 4.317 ug/l  
RT: 4.581 min Scan# 51  
Delta R.T. 0.025 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001

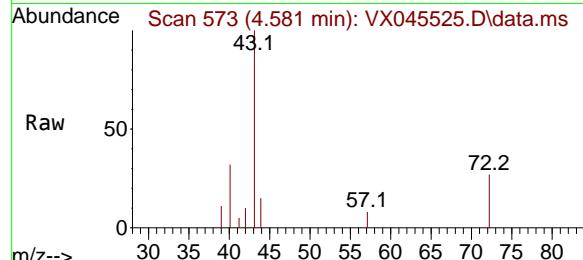


Tgt Ion: 43 Resp: 4590  
Ion Ratio Lower Upper  
43 100  
72 27.2 18.6 28.0

Manual Integrations  
APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

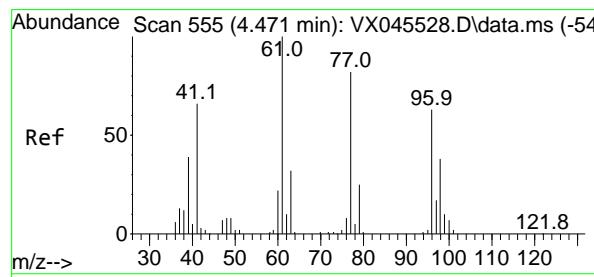
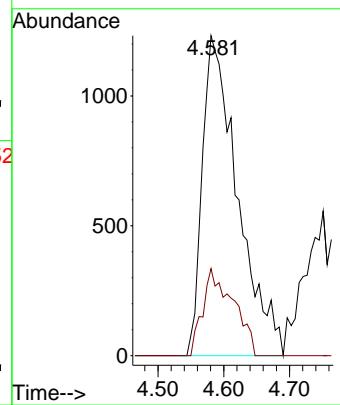
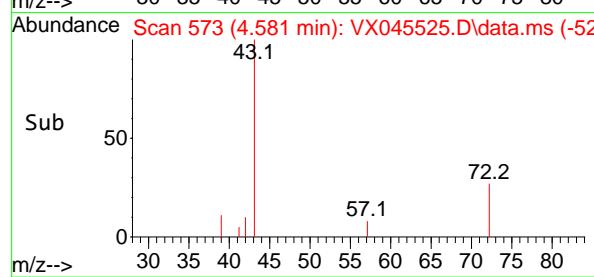


#26  
2,2-Dichloropropane  
Concen: 0.824 ug/l  
RT: 4.471 min Scan# 555  
Delta R.T. 0.000 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

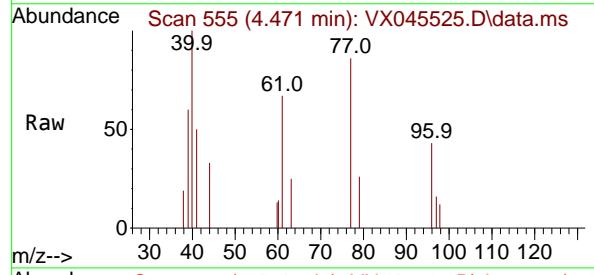

Tgt Ion: 77 Resp: 1307  
Ion Ratio Lower Upper  
77 100  
97 13.9 10.6 31.8

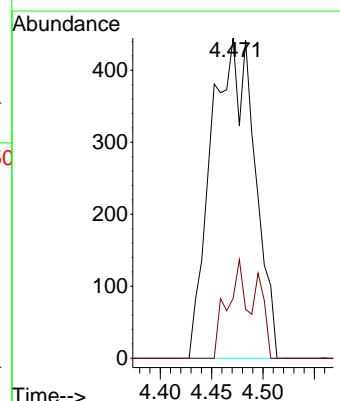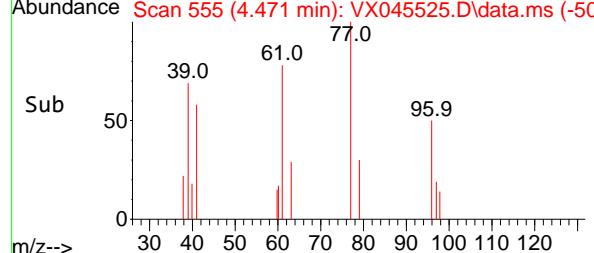



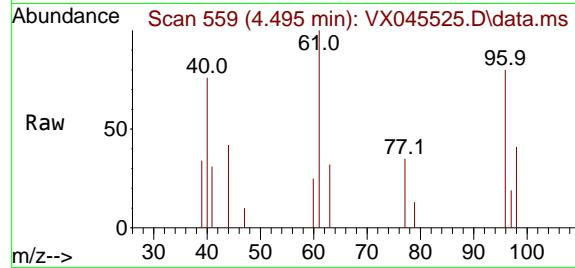



#27  
cis-1,2-Dichloroethene  
Concen: 1.020 ug/l  
RT: 4.495 min Scan# 51  
Delta R.T. 0.012 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025



#28  
Bromochloromethane  
Concen: 1.094 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion: 49 Resp: 1298  
Ion Ratio Lower Upper  
49 100  
129 0.0 0.0 3.8  
130 66.0 54.6 81.8

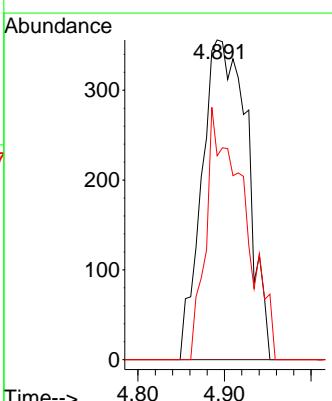

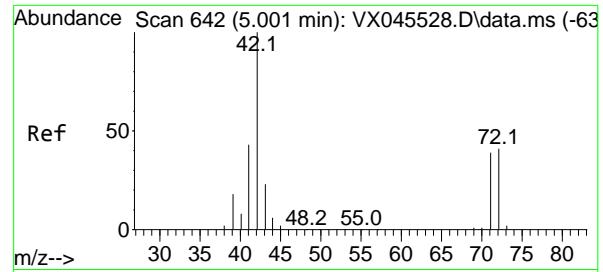

#29

Tetrahydrofuran

Concen: 4.752 ug/l

RT: 5.032 min Scan# 6

Delta R.T. 0.031 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC001

Tgt Ion: 42 Resp: 3270

Ion Ratio Lower Upper

42 100

72 42.3 33.4 50.0





71 36.0 31.4 47.0

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#30

Chloroform

Concen: 0.953 ug/l

RT: 5.093 min Scan# 657

Delta R.T. 0.006 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06


Tgt Ion: 83 Resp: 2406

Ion Ratio Lower Upper

83 100

85 53.7 52.8 79.2

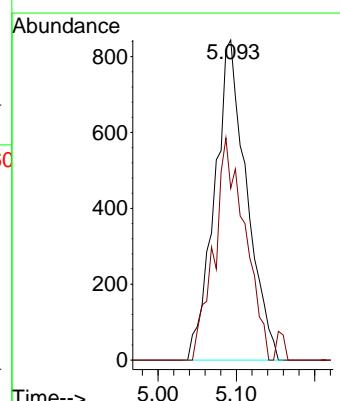

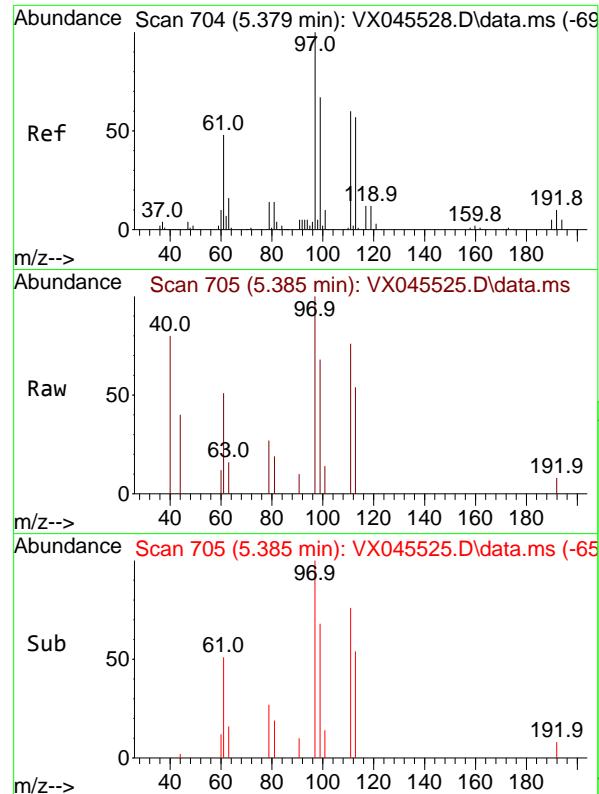

#32

1,1,1-Trichloroethane

Concen: 0.931 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

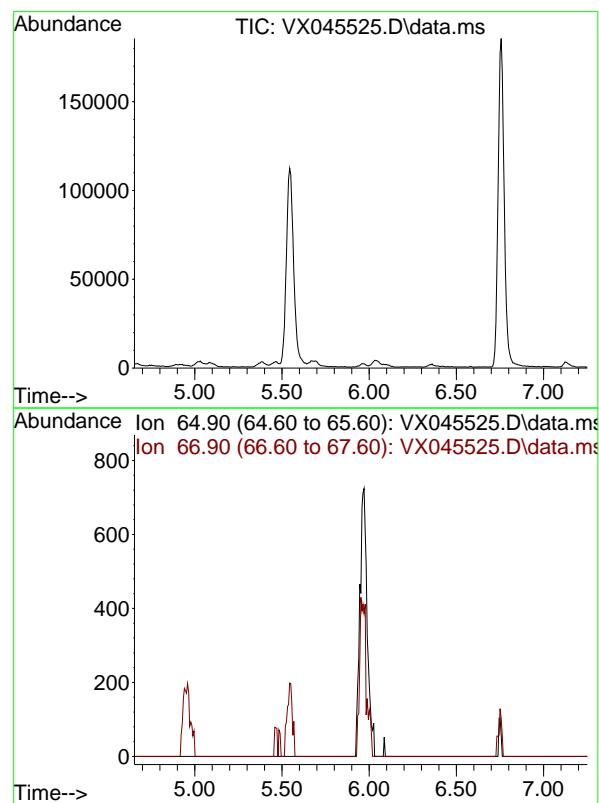

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 5.95 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt Ion: 65

Sig Exp Ratio

65 100

67 49.5


1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12

13

14

15

16

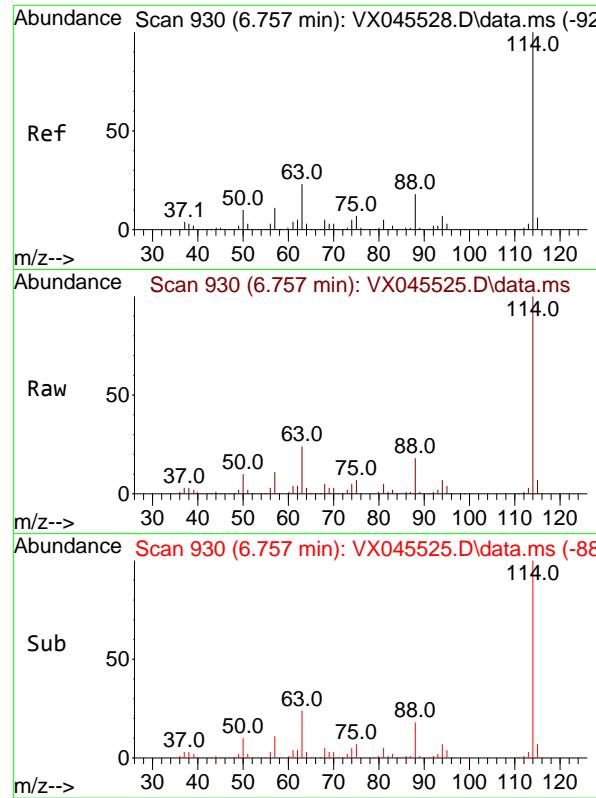

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 9

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

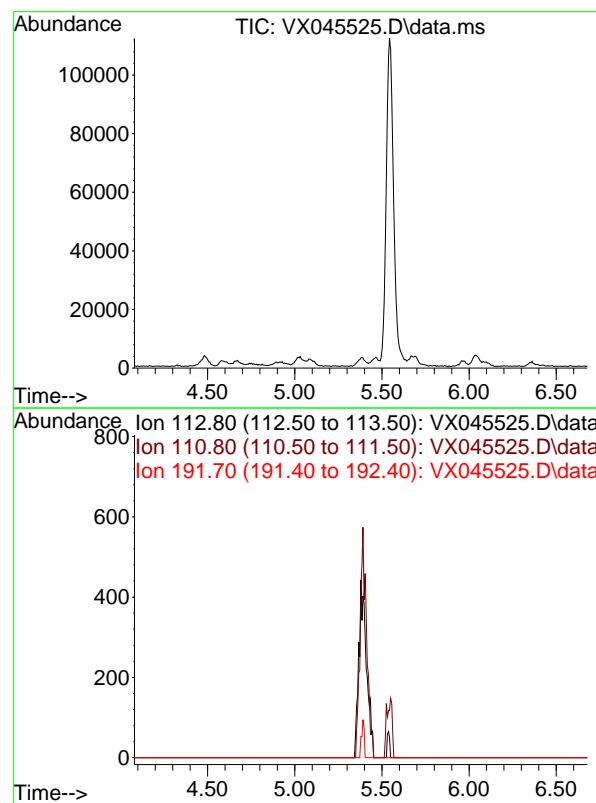

#35

Dibromofluoromethane

Concen: 0.000 ug/l

Expected RT: 5.38 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06


Tgt Ion: 113

Sig Exp Ratio

113 100

111 102.2


192 17.2



#36

1,1-Dichloropropene  
Concen: 0.995 ug/l  
RT: 5.696 min Scan# 7  
Delta R.T. 0.012 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001

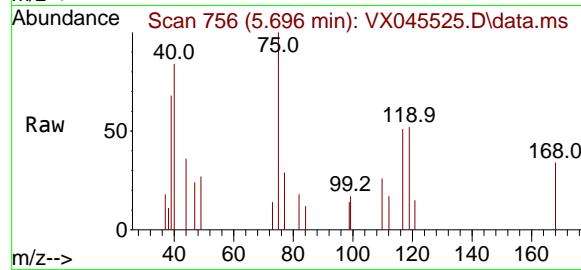


Tgt Ion: 75 Resp: 167:  
Ion Ratio Lower Upper  
75 100  
110 27.6 16.9 50.6  
77 25.0 25.0 37.4

Manual Integrations  
APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025


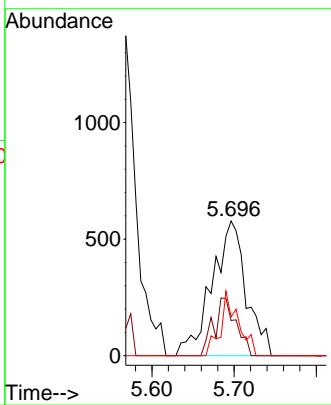



#37  
Ethyl Acetate  
Concen: 0.964 ug/l  
RT: 4.751 min Scan# 601  
Delta R.T. 0.037 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06



Tgt Ion: 43 Resp: 2040  
Ion Ratio Lower Upper  
43 100  
61 3.3 9.9 14.9#  
70 0.0 7.5 11.3#

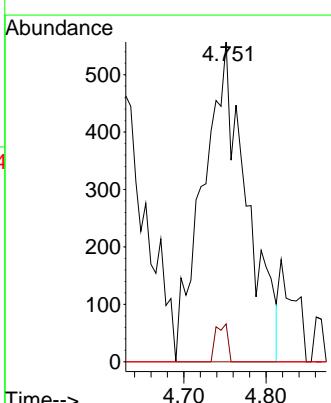



#38

Carbon Tetrachloride

Concen: 0.870 ug/l

RT: 5.672 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025




Tgt Ion:117 Resp: 1573

Ion Ratio Lower Upper

117 100

119 102.7 76.9 115.3

121 39.6 24.2 36.2

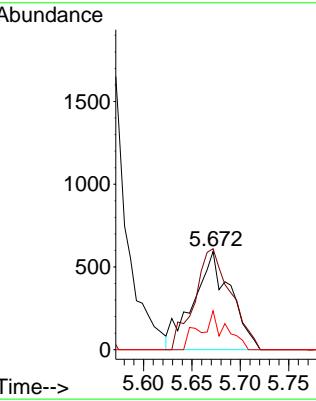

#39

Methylcyclohexane

Concen: 0.883 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06


Tgt Ion: 83 Resp: 1818




Ion Ratio Lower Upper

83 100

55 77.0 64.9 97.3

98 62.1 37.4 56.0#

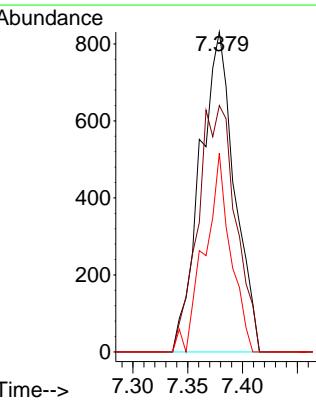

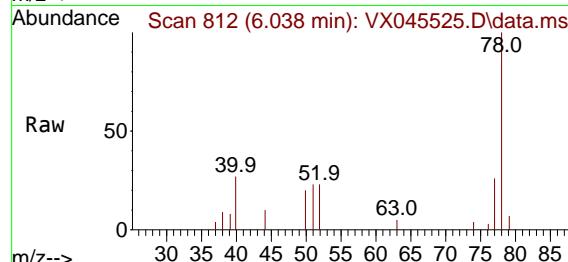

#40

Benzene

Concen: 0.967 ug/l

RT: 6.038 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC001

Tgt Ion: 78 Resp: 495

Ion Ratio Lower Upper

78 100

77 25.5




19.0

28.6

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

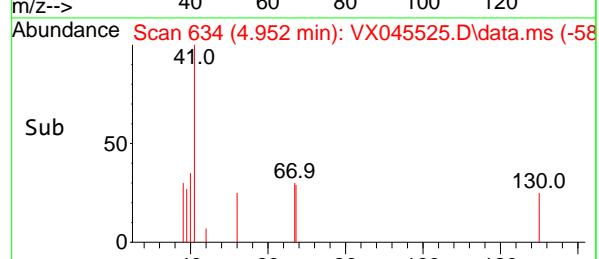

#41

Methacrylonitrile

Concen: 0.784 ug/l m

RT: 4.952 min Scan# 634

Delta R.T. 0.031 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt Ion: 41 Resp: 883

Ion Ratio Lower Upper

41 100

39 0.0

47.0

70.6#

67 0.0


53.2




79.8#

52 0.0

25.0

37.6#

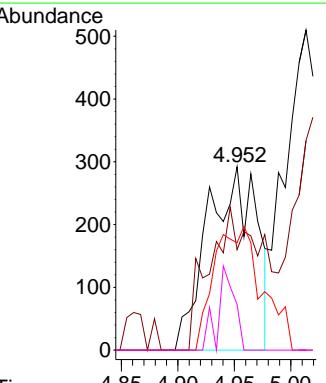



#42

1,2-Dichloroethane

Concen: 0.882 ug/l

RT: 6.092 min Scan# 8

Delta R.T. 0.012 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#43

Isopropyl Acetate

Concen: 0.804 ug/l

RT: 6.361 min Scan# 865

Delta R.T. 0.025 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06


Tgt Ion: 43 Resp: 2578


Ion Ratio Lower Upper

43 100

61 10.6 14.1 21.1#

87 6.9 9.2 13.8#

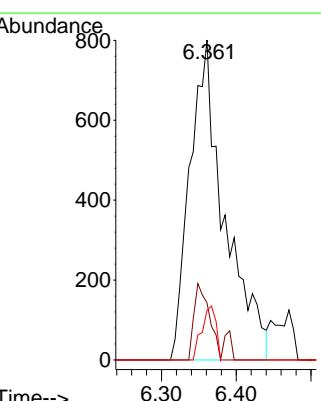

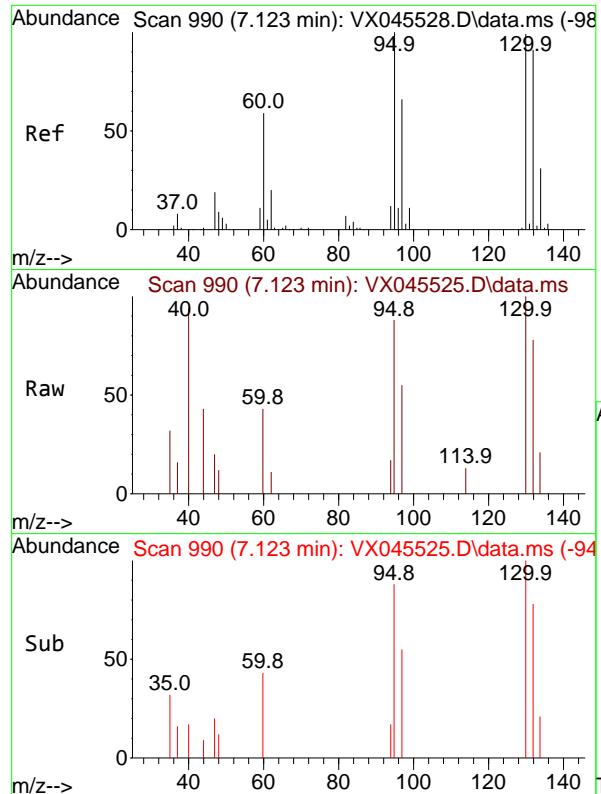

#44

Trichloroethene

Concen: 1.004 ug/l

RT: 7.123 min Scan# 990

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC001

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

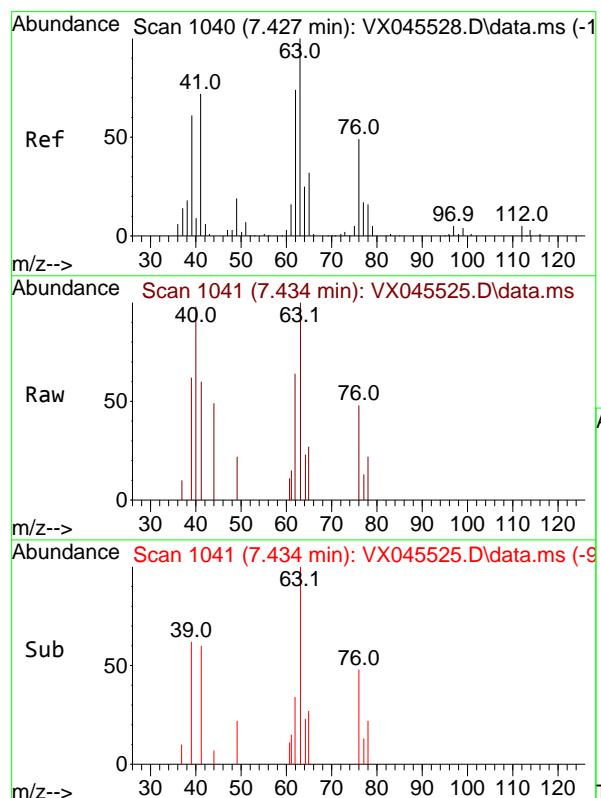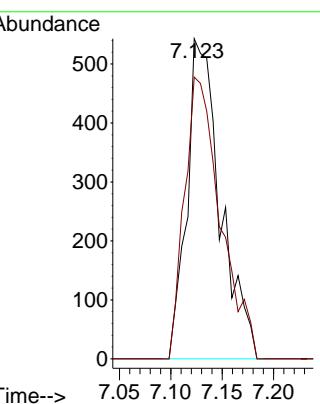

#45

1,2-Dichloropropane

Concen: 0.846 ug/l

RT: 7.434 min Scan# 1041


Delta R.T. 0.006 min







Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt Ion: 63 Resp: 1082

Ion	Ratio	Lower	Upper
63	100		
65	26.6	25.8	38.6

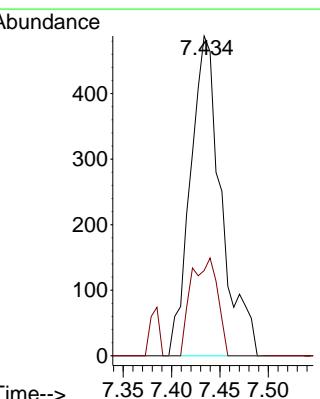

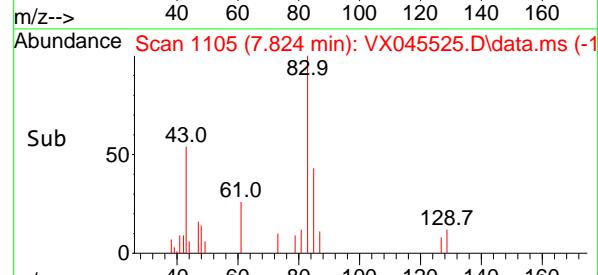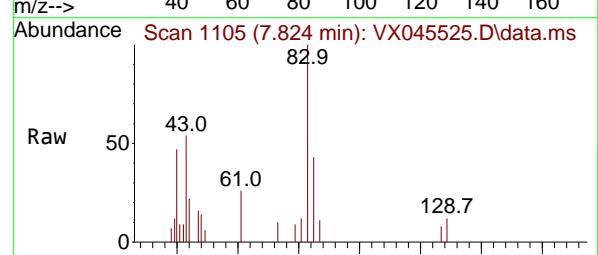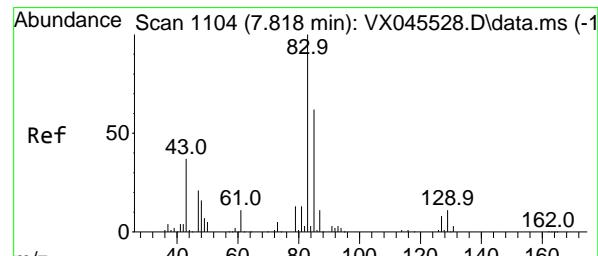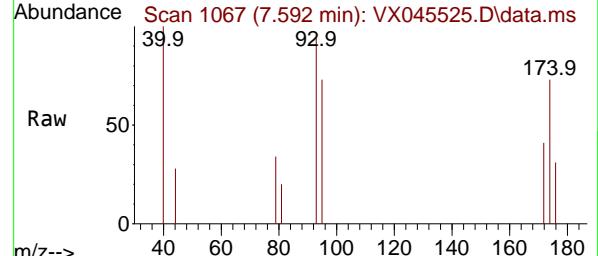

#46

Dibromomethane

Concen: 0.846 ug/l

RT: 7.592 min Scan# 1

Delta R.T. 0.018 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X



ClientSampleId :




VSTDICC001

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

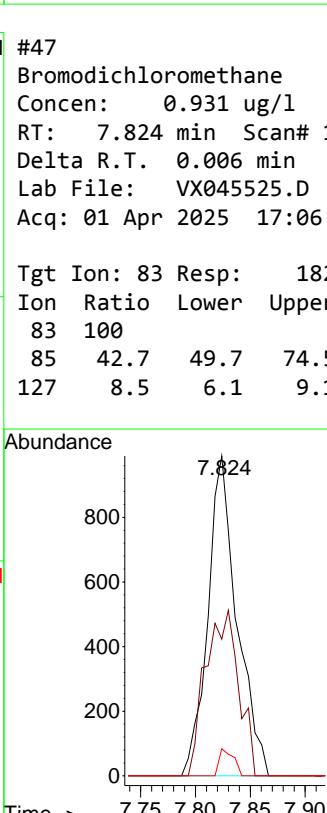

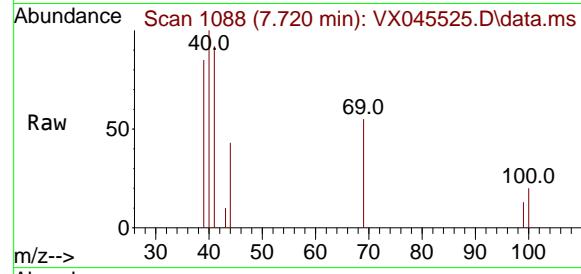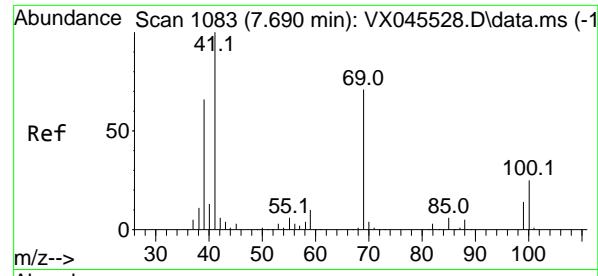

#48

Methyl methacrylate

Concen: 0.857 ug/l

RT: 7.720 min Scan# 1088

Delta R.T. 0.031 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC001

Tgt Ion: 41 Resp: 1419

Ion Ratio Lower Upper

41 100

69 64.7 58.2 87.2





39 72.7 53.6 80.4

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

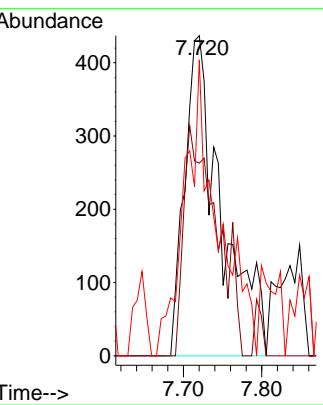

#49

1,4-Dioxane

Concen: 15.288 ug/l

RT: 7.671 min Scan# 1080

Delta R.T. 0.012 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06


Tgt Ion: 88 Resp: 458






Ion Ratio Lower Upper

88 100

43 30.3 32.2 48.4#

58 72.3 58.6 88.0

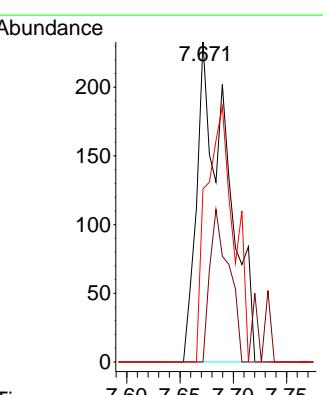

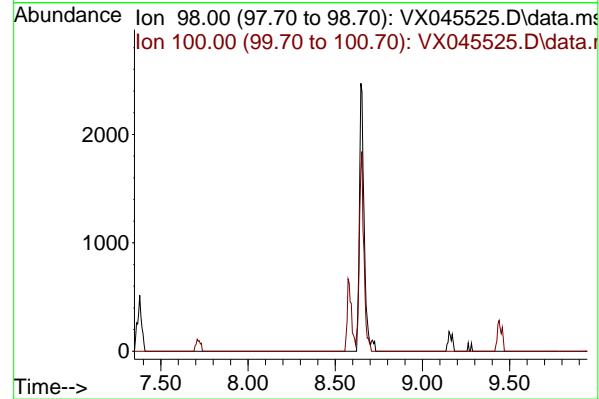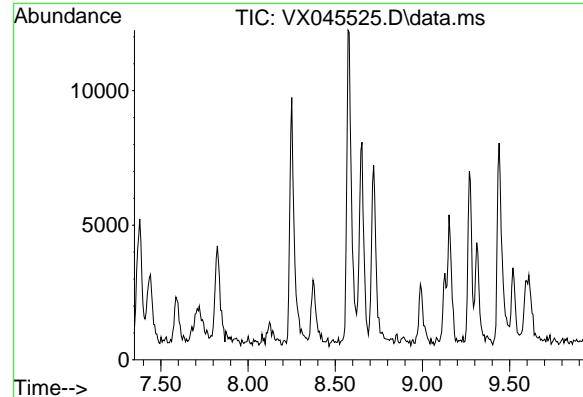

#50  
Toluene-d8  
Concen: 0.000 ug/l  
Expected RT: 8.65 min

Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion: 98  
Sig Exp Ratio  
98 100  
100 65.3


Instrument :  
MSVOA\_X  
ClientSampleId :  
VSTDICC001


Manual Integrations  
APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

#51  
4-Methyl-2-Pentanone  
Concen: 4.114 ug/l  
RT: 8.574 min Scan# 1228  
Delta R.T. 0.000 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06


Tgt Ion: 43 Resp: 8746  
Ion Ratio Lower Upper  
43 100  
58 35.5 28.5 42.7





#52  
Toluene  
Concen: 0.923 ug/l  
RT: 8.720 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001




Tgt Ion: 92 Resp: 2863  
Ion Ratio Lower Upper  
92 100  
91 167.2 138.7 208.1

Manual Integrations  
APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025





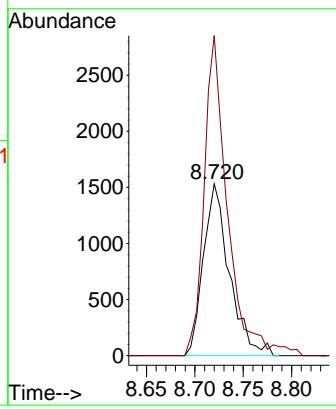
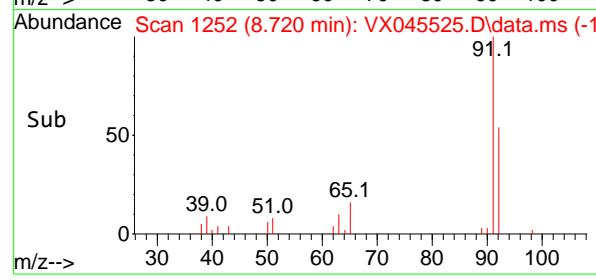


#53  
t-1,3-Dichloropropene  
Concen: 2.850 ug/l  
RT: 8.988 min Scan# 1296  
Delta R.T. 0.012 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06



Tgt Ion: 75 Resp: 1109  
Ion Ratio Lower Upper  
75 100  
77 35.6 25.4 38.0

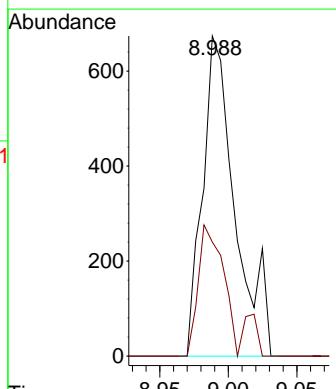



#54

cis-1,3-Dichloropropene

Concen: 0.705 ug/l

RT: 8.379 min Scan# 1

Delta R.T. 0.013 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#55

1,1,2-Trichloroethane

Concen: 0.957 ug/l

RT: 9.159 min Scan# 1324

Delta R.T. 0.012 min


Lab File: VX045525.D


Acq: 01 Apr 2025 17:06

Tgt Ion: 97 Resp: 1183

Ion Ratio Lower Upper

97	100		
83	53.9	71.8	107.8#
85	48.5	47.0	70.6
99	51.7	48.6	73.0



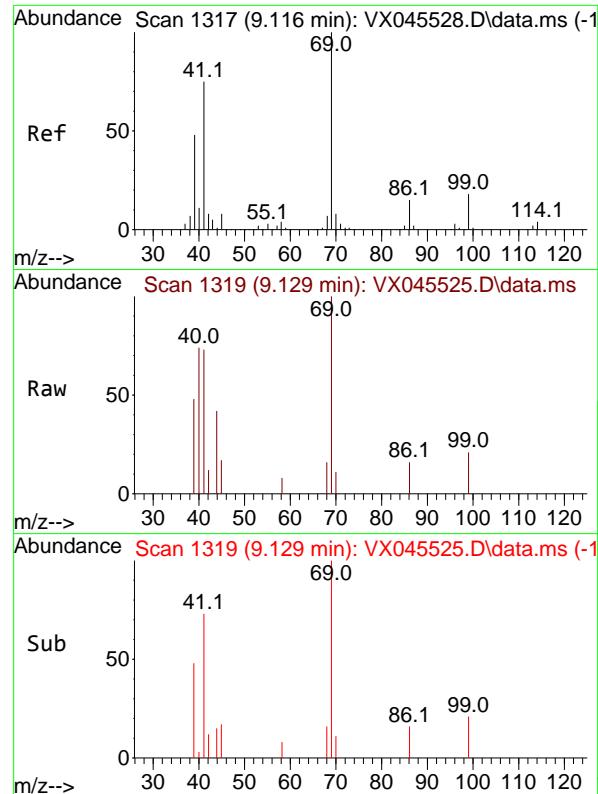

#56

Ethyl methacrylate

Concen: 0.745 ug/l m

RT: 9.129 min Scan# 1

Delta R.T. 0.013 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC001

Tgt Ion: 69 Resp: 1425

Ion Ratio Lower Upper

69 100

41 77.3 61.3 91.9



39 56.9 40.2 60.2

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

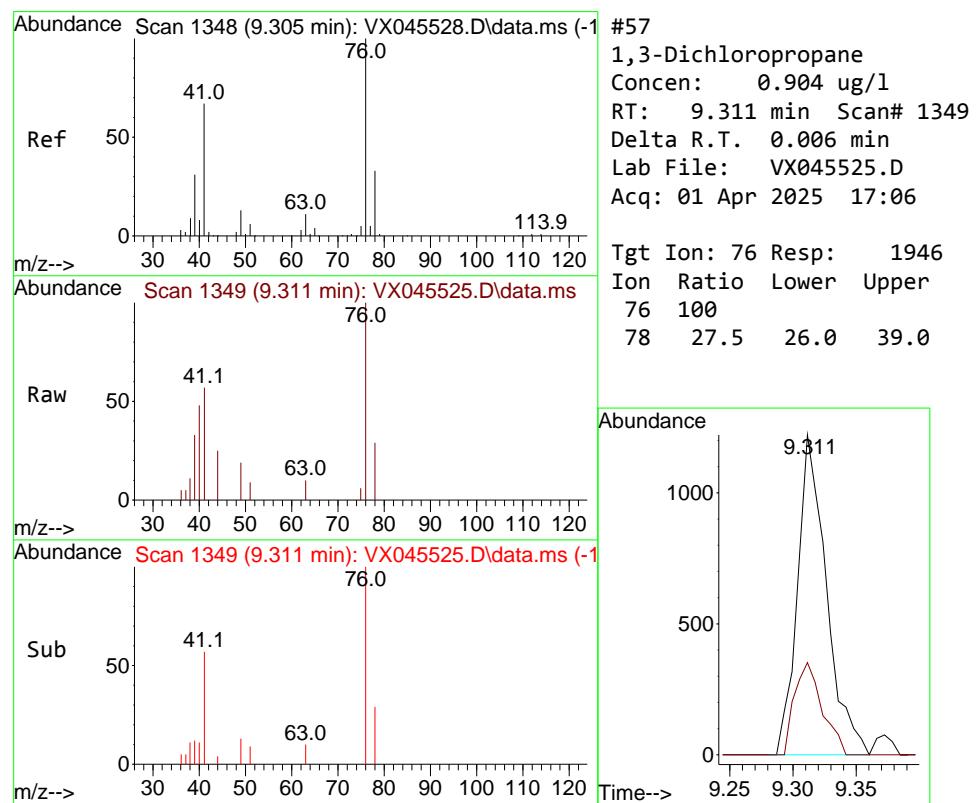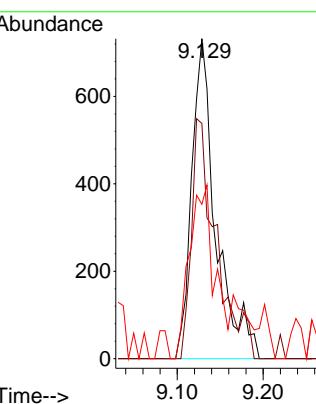

#57

1,3-Dichloropropane

Concen: 0.904 ug/l

RT: 9.311 min Scan# 1349

Delta R.T. 0.006 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06




Tgt Ion: 76 Resp: 1946

Ion Ratio Lower Upper

76 100

78 27.5 26.0 39.0

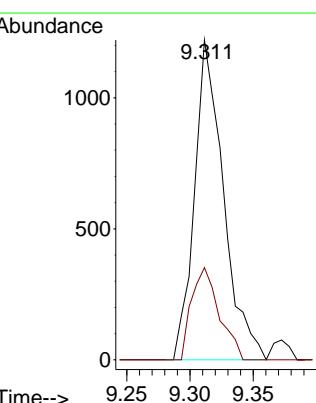

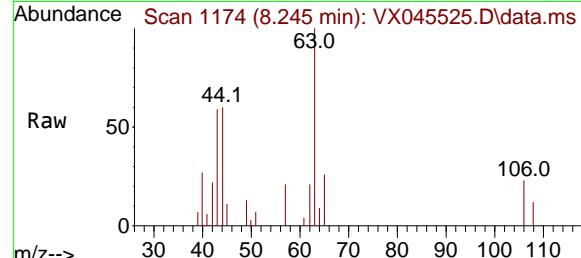

#58

2-Chloroethyl Vinyl ether

Concen: 4.008 ug/l

RT: 8.245 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

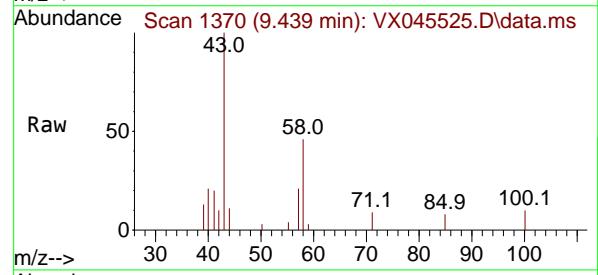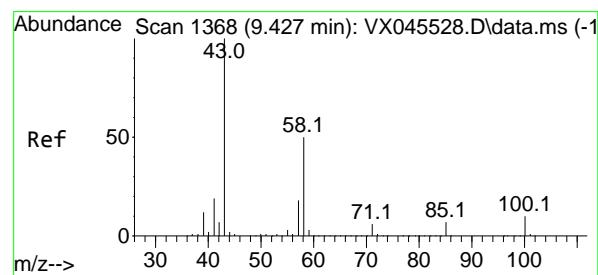

#59

2-Hexanone

Concen: 4.040 ug/l

RT: 9.439 min Scan# 1370

Delta R.T. 0.012 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06




Tgt Ion: 43 Resp: 6360

Ion Ratio Lower Upper

43 100

58 39.5 24.9 74.6

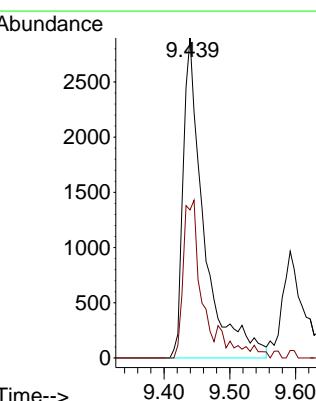

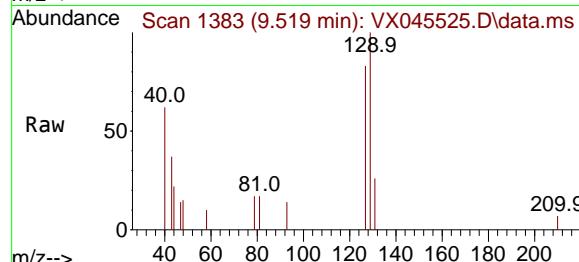

#60

Dibromochloromethane

Concen: 0.814 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#61

1,2-Dibromoethane

Concen: 0.825 ug/l

RT: 9.610 min Scan# 1398

Delta R.T. 0.006 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06


Tgt Ion:107 Resp: 1032

Ion Ratio Lower Upper

107 100

109 98.1 75.7 113.5

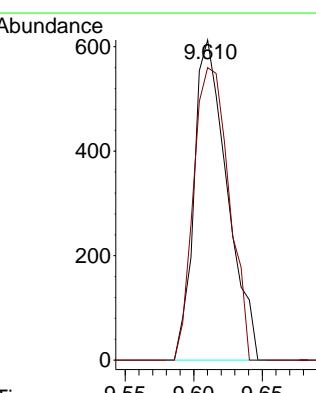


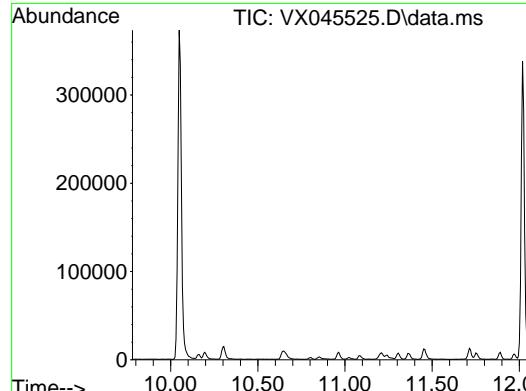


#62  
4-Bromofluorobenzene  
Concen: 0.000 ug/l  
Expected RT: 11.08 min  
  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06  
  
Tgt Ion: 95  
Sig Exp Ratio  
95 100  
174 67.9  
176 65.7


Instrument :  
MSVOA\_X  
ClientSampleId :  
VSTDICC001

**Manual Integrations**  
**APPROVED**



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

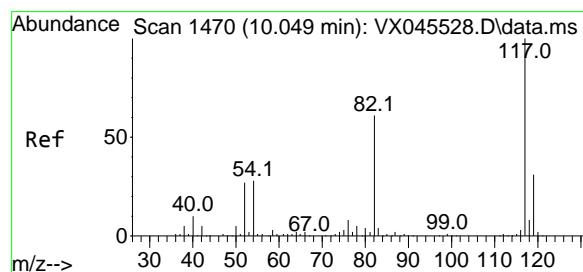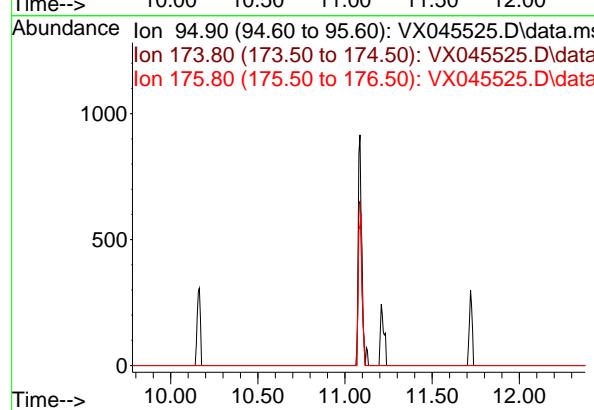


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1470  
Delta R.T. 0.000 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

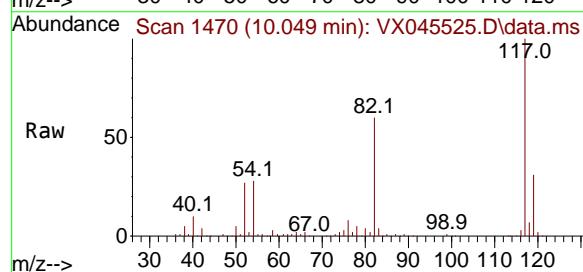

Tgt Ion:117 Resp: 153312  
Ion Ratio Lower Upper  
117 100  
82 60.5 49.2 73.8  
119 31.0 25.1 37.7

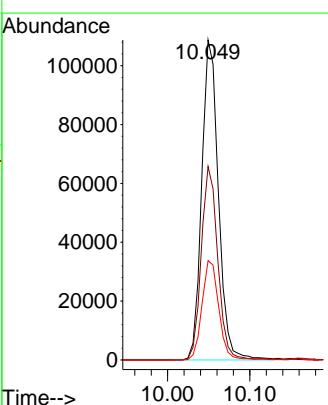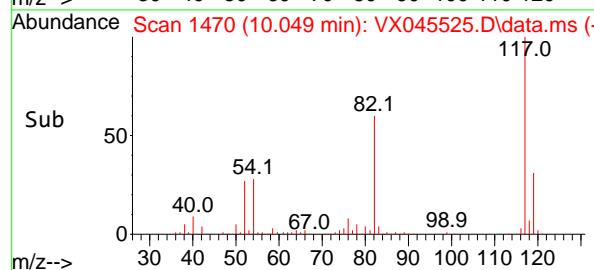

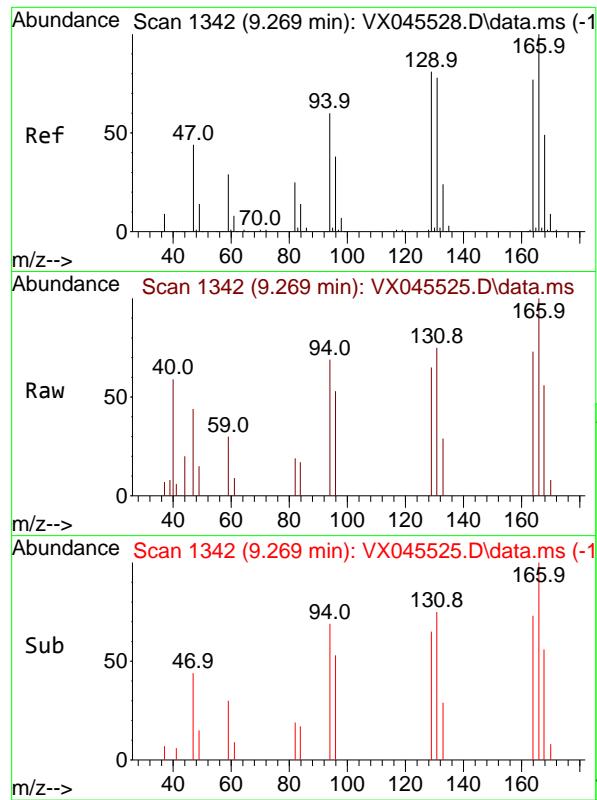

#64

Tetrachloroethene

Concen: 0.981 ug/l

RT: 9.269 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

Tgt Ion:164 Resp: 1063

Ion Ratio Lower Upper



164 100

166 137.7 103.8 155.8

129 90.1 84.3 126.5

131 103.7 80.9 121.3

Abundance

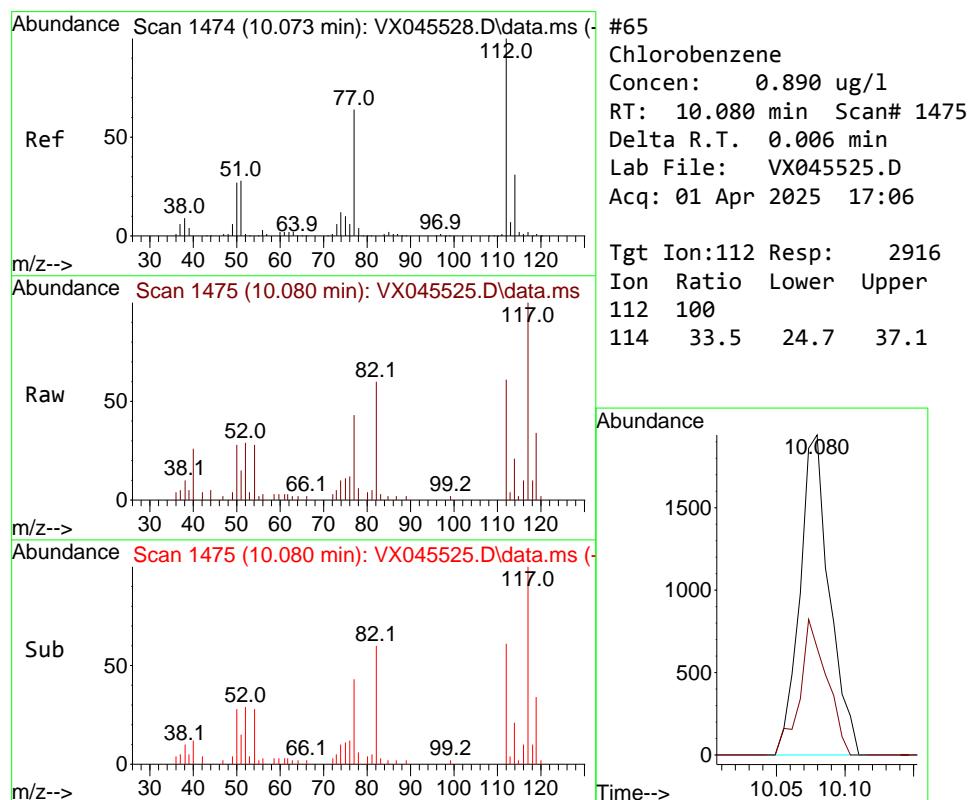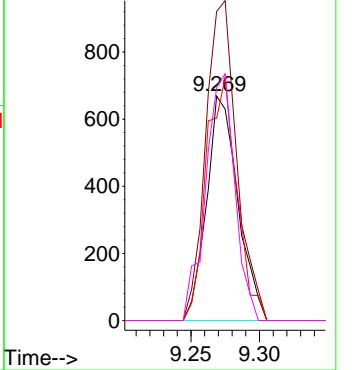

#65

Chlorobenzene

Concen: 0.890 ug/l

RT: 10.080 min Scan# 1475

Delta R.T. 0.006 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06




Tgt Ion:112 Resp: 2916

Ion Ratio Lower Upper

112 100

114 33.5 24.7 37.1

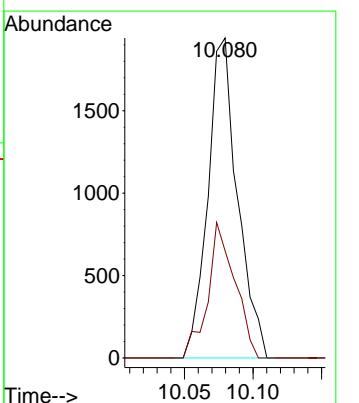

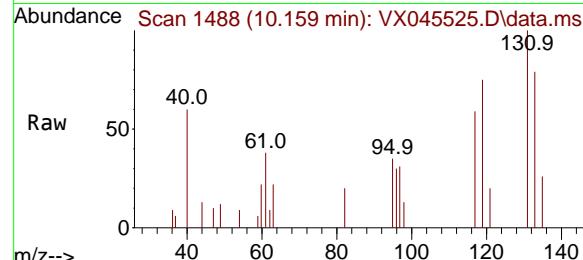

#66

1,1,1,2-Tetrachloroethane

Concen: 0.992 ug/l

RT: 10.159 min Scan# 1488

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06




Instrument : MSVOA\_X

ClientSampleId : VSTDICC001

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

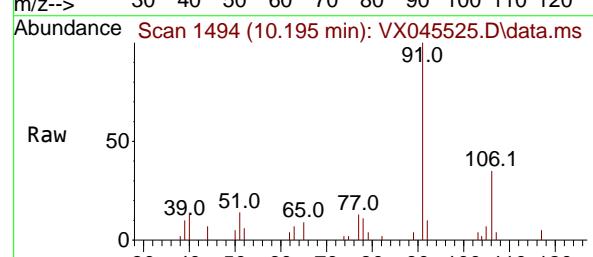

#67

Ethyl Benzene

Concen: 0.840 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.006 min


Lab File: VX045525.D




Acq: 01 Apr 2025 17:06

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
91	100		4930		
106	35.2	23.7	35.5		

Time--&gt; 10.10 10.15 10.20

Abundance

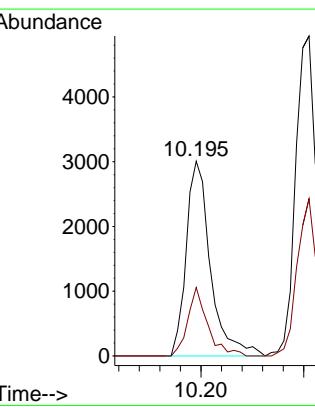







#68  
m/p-Xylenes  
Concen: 1.708 ug/l  
RT: 10.305 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06  
ClientSampleId : VSTDICC001

Tgt Ion:106 Resp: 3645  
Ion Ratio Lower Upper  
106 100  
91 221.2 172.6 258.8


### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

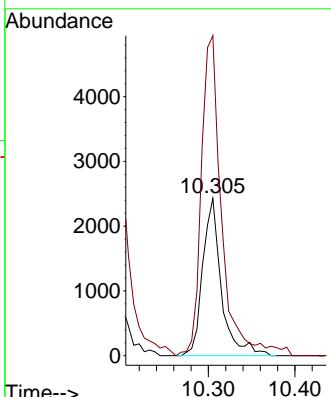

#69  
o-Xylene  
Concen: 0.820 ug/l  
RT: 10.640 min Scan# 1567  
Delta R.T. 0.000 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion:106 Resp: 1724  
Ion Ratio Lower Upper  
106 100  
91 254.4 113.6 340.6

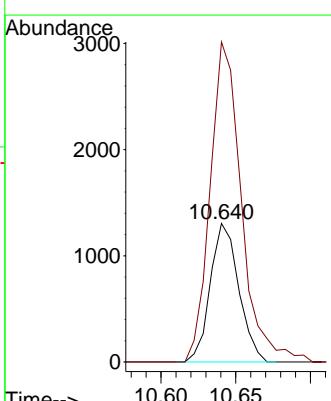


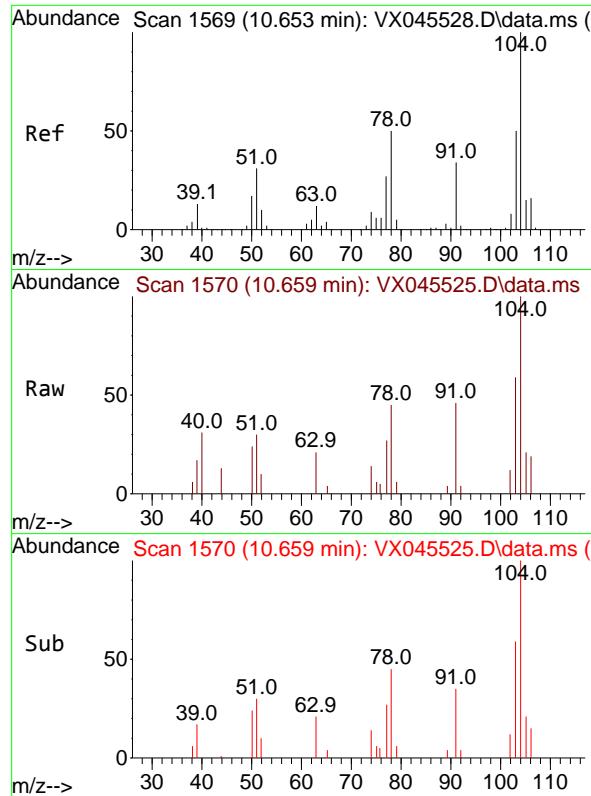


#70  
Styrene  
Concen: 0.793 ug/l  
RT: 10.659 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

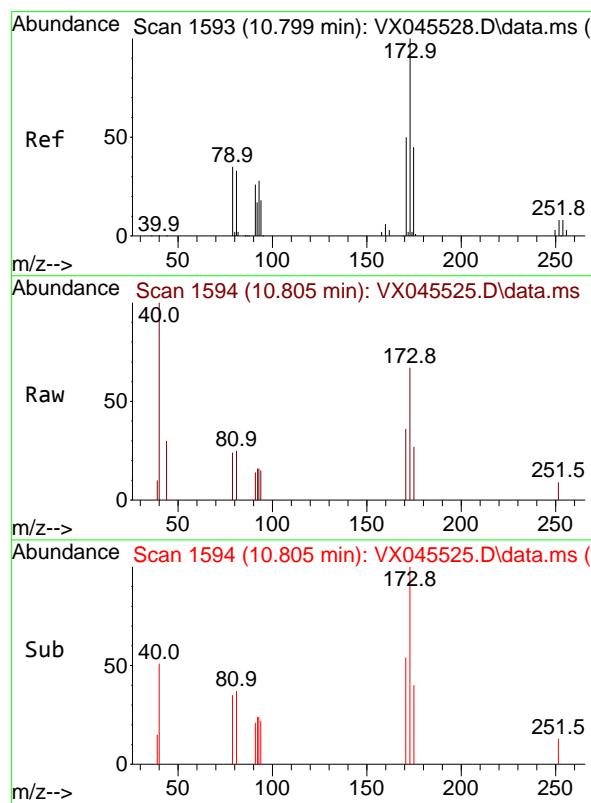

#71  
Bromoform  
Concen: 0.795 ug/l  
RT: 10.805 min Scan# 1594  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion:173 Resp: 675  
Ion Ratio Lower Upper  
173 100  
175 42.7 23.4 70.2  
254 0.0 0.0 0.0




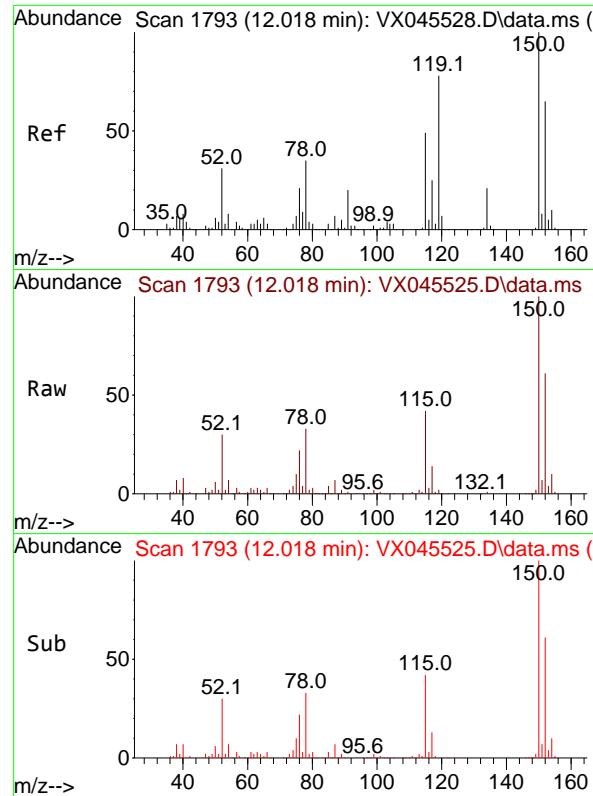


#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

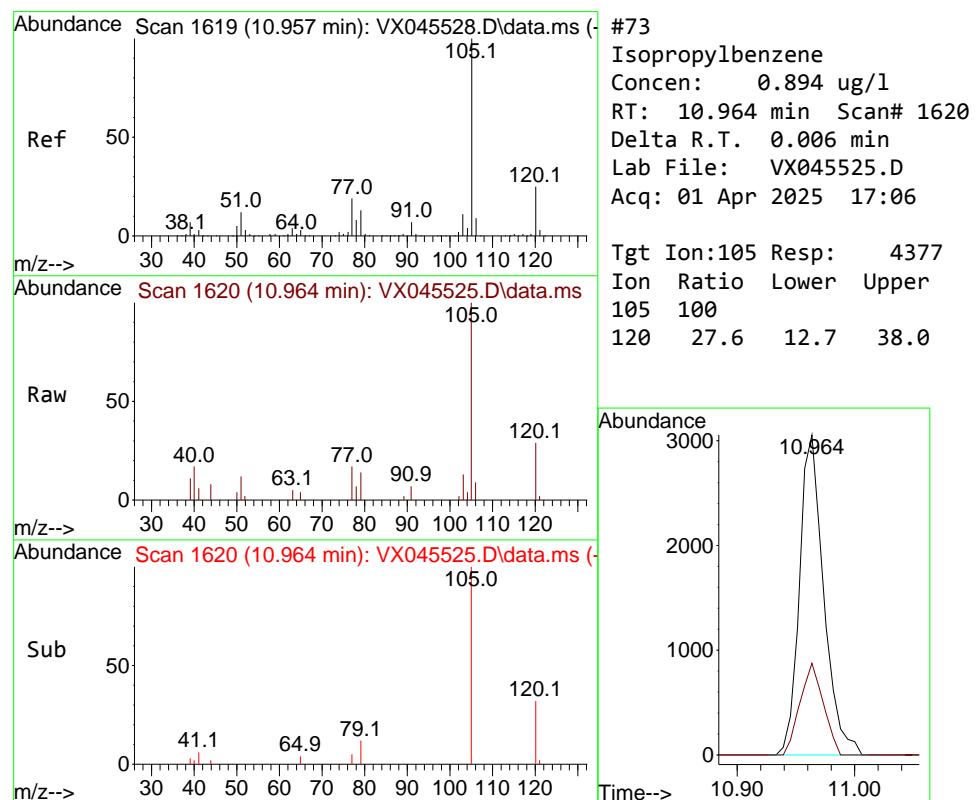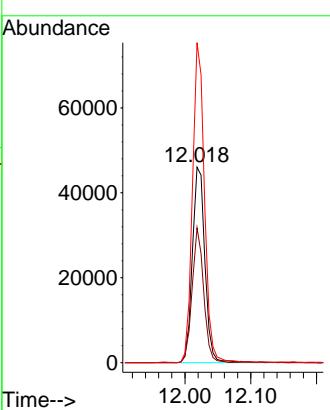

#73  
Isopropylbenzene  
Concen: 0.894 ug/l  
RT: 10.964 min Scan# 1620  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion:105 Resp: 4377  
Ion Ratio Lower Upper  
105 100  
120 27.6 12.7 38.0

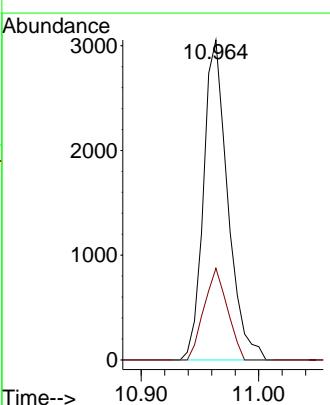

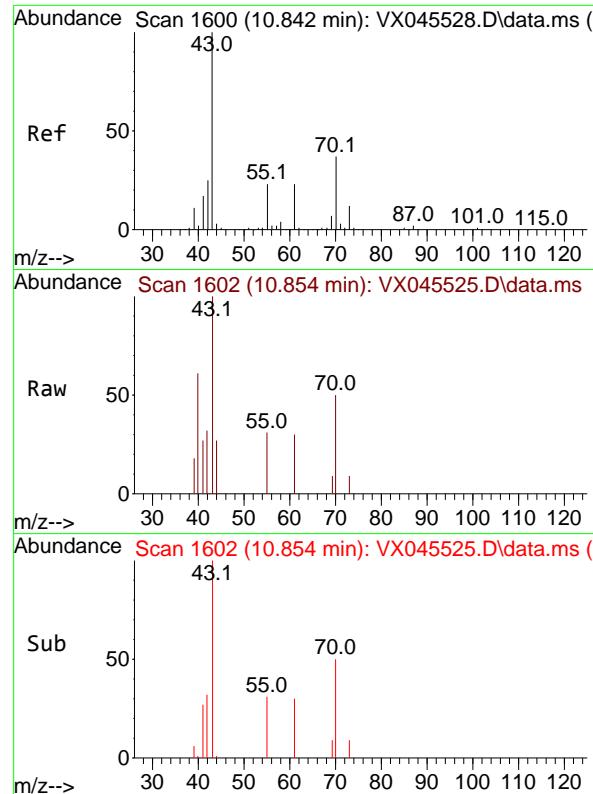

#74

N-amyl acetate

Concen: 0.752 ug/l

RT: 10.854 min Scan# 1602

Delta R.T. 0.012 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**



Reviewed By :Amit Patel 04/02/2025


Supervised By :Mahesh Dadoda 04/02/2025




#75  
1,1,2,2-Tetrachloroethane  
Concen: 1.036 ug/l  
RT: 11.214 min Scan# 1661  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion: 83 Resp: 1781  
Ion Ratio Lower Upper  
83 100  
131 5.3 4.7 14.1  
85 61.1 32.4 97.2

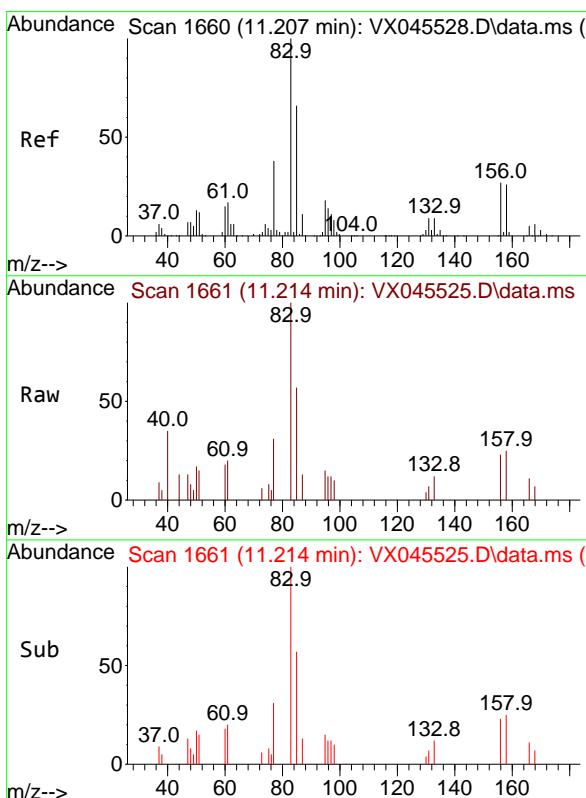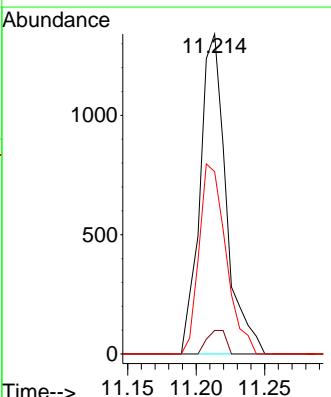




Abundance Scan 1666 (11.244 min): VX045525.D\data.ms

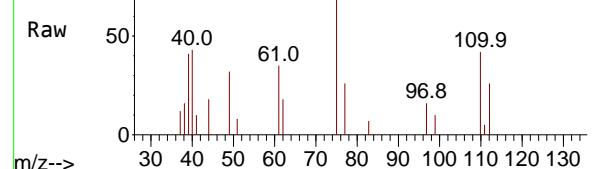

Abundance Scan 1666 (11.244 min): VX045525.D\data.ms (-)

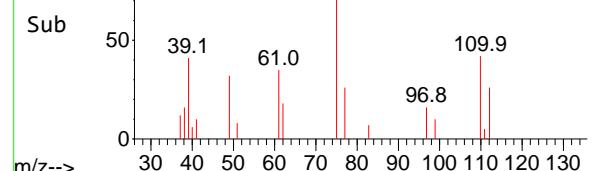

#76

1,2,3-Trichloropropane

Concen: 1.002 ug/l m

RT: 11.244 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001


**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025


Supervised By :Mahesh Dadoda 04/02/2025

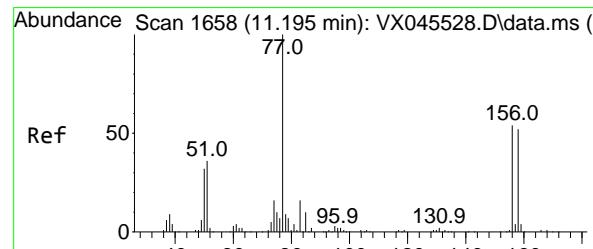

Abundance Scan 1659 (11.201 min): VX045525.D\data.ms

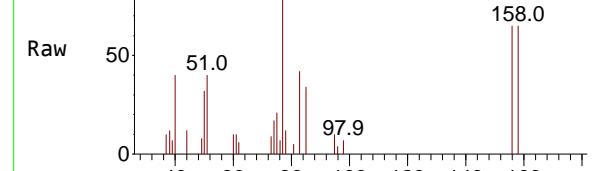

Abundance Scan 1659 (11.201 min): VX045525.D\data.ms (-)

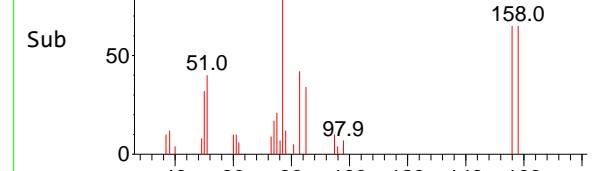

#77

Bromobenzene

Concen: 0.948 ug/l

RT: 11.201 min Scan# 1659

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06



Tgt Ion:156 Resp: 1072


Ion Ratio Lower Upper

156 100


77 176.5 92.6 277.8

158 98.4 48.1 144.4

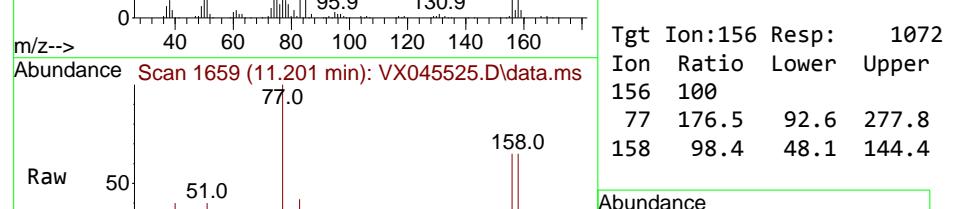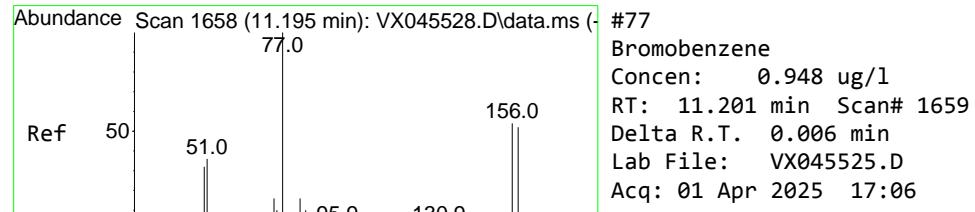



Abundance Scan 1676 (11.305 min): VX045525.D\data.ms (-)

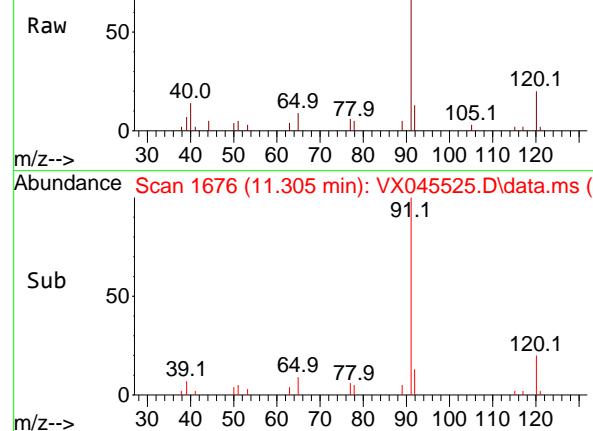

#78

n-propylbenzene

Concen: 0.809 ug/l

RT: 11.305 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001


**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



Abundance Scan 1686 (11.366 min): VX045525.D\data.ms (-)

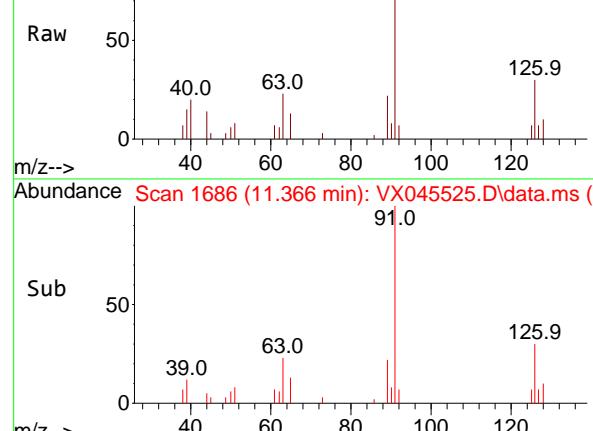

#79

2-Chlorotoluene

Concen: 0.981 ug/l

RT: 11.366 min Scan# 1686

Delta R.T. 0.006 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06




Tgt Ion: 91 Resp: 3537

Ion Ratio Lower Upper

91 100

126 31.8 15.8 47.4

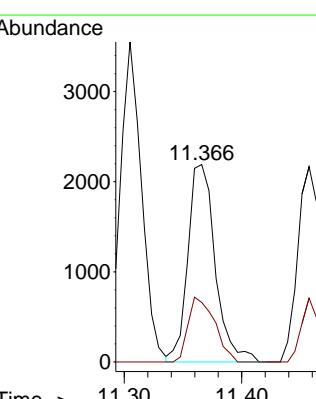

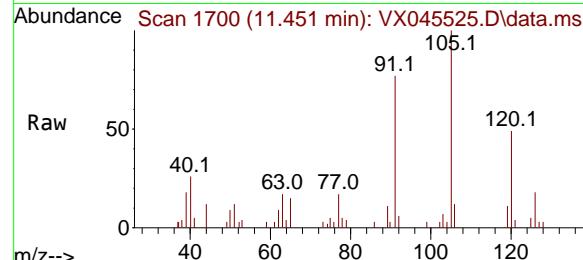

#80

1,3,5-Trimethylbenzene

Concen: 0.885 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

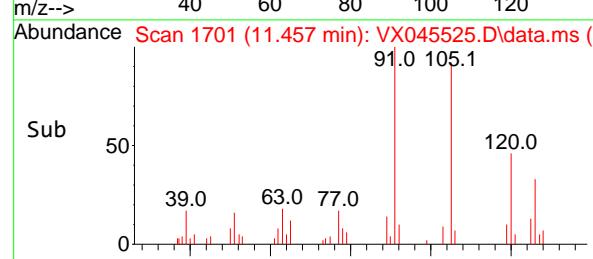

#82

4-Chlorotoluene

Concen: 0.900 ug/l


RT: 11.457 min Scan# 1701




Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt	Ion:	91	Resp:	3619
Ion	Ratio	Lower	Upper	
91	100			
126	24.7	13.3	39.9	





#83

tert-Butylbenzene

Concen: 0.883 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#84

1,2,4-Trimethylbenzene

Concen: 0.874 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045525.D


Acq: 01 Apr 2025 17:06




Tgt Ion:105 Resp: 3552

Ion Ratio Lower Upper

105 100

120 42.0 21.4 64.3

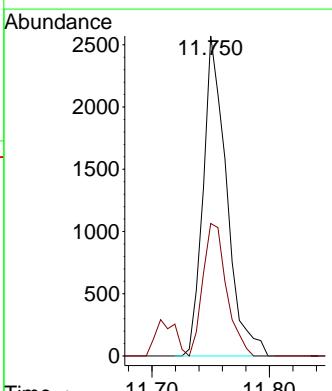



#85

sec-Butylbenzene

Concen: 0.793 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

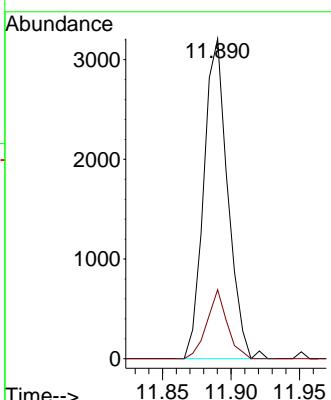

#86

p-Isopropyltoluene

Concen: 0.824 ug/l


RT: 12.012 min Scan# 1792

Delta R.T. 0.006 min


Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt	Ion:119	Resp:	3342
Ion	Ratio	Lower	Upper
119	100		
134	26.6	12.6	37.8
91	31.9	13.7	41.1

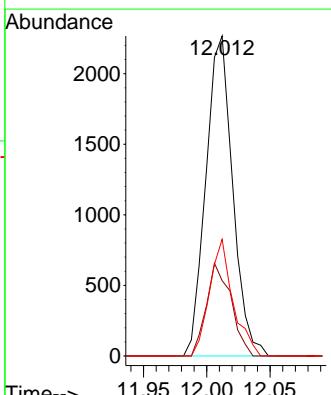

Q1711-VOCMS Group3

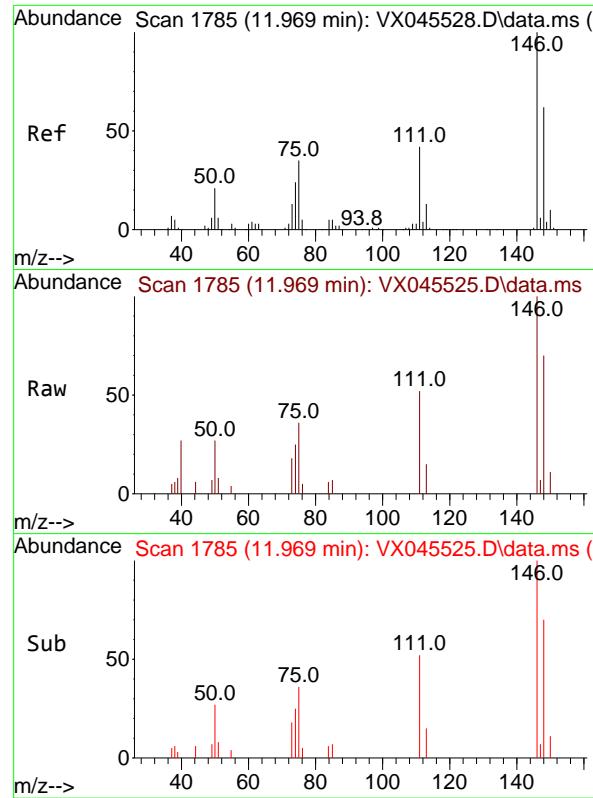

#87

1,3-Dichlorobenzene

Concen: 0.984 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC001

Tgt

Ion:146 Resp: 2020

Ion Ratio Lower Upper

146 100

111 42.2 22.2 66.6

148 61.2 31.9 95.7

Manual Integrations


APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

Abundance

11.969

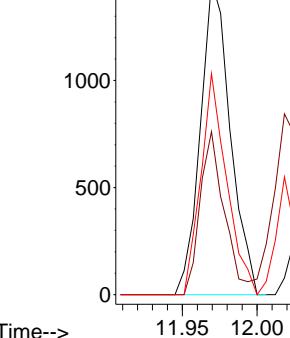

#88

1,4-Dichlorobenzene

Concen: 0.978 ug/l

RT: 12.043 min Scan# 1797

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt

Ion:146 Resp: 2042

Ion Ratio Lower Upper



146 100


111 41.8 20.9 62.8

148 60.7 31.5 94.5

Abundance

12.043

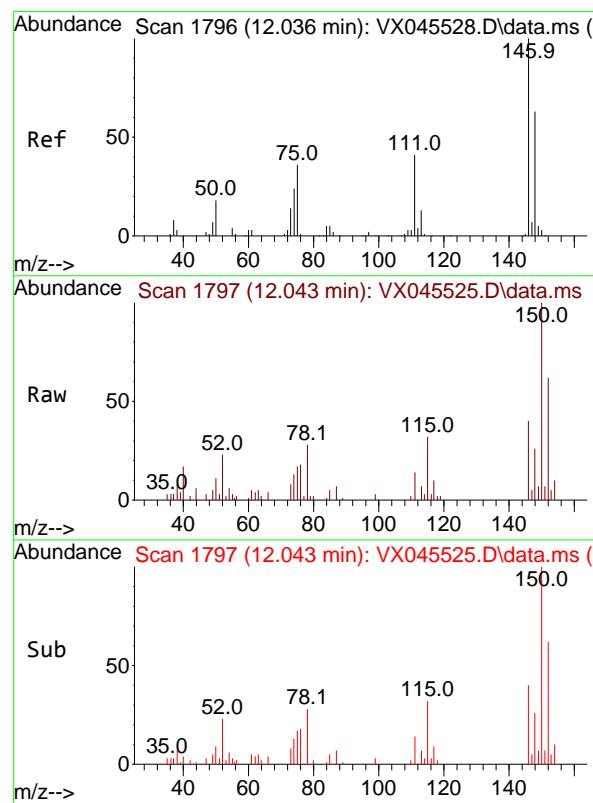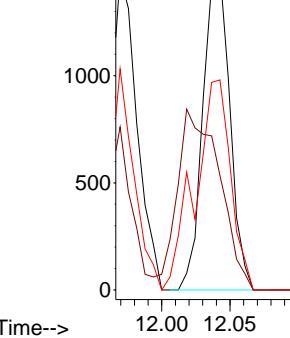

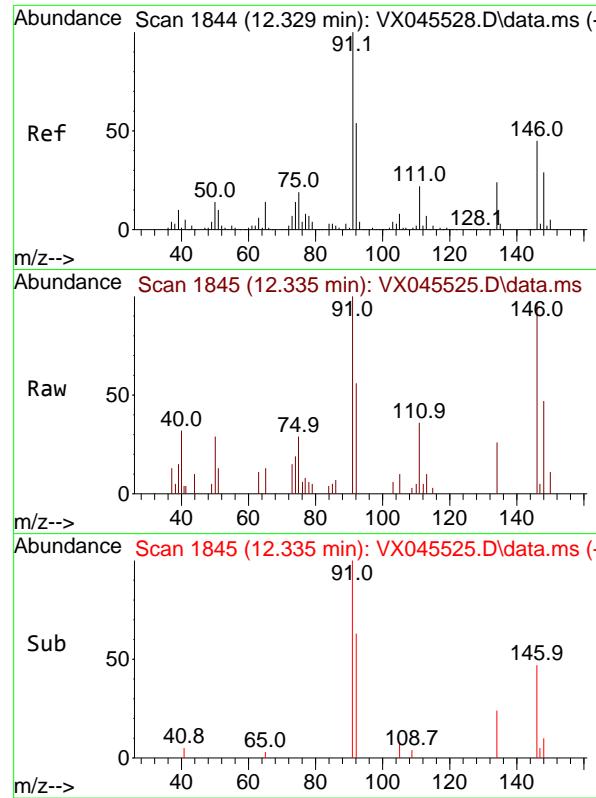

#89

n-Butylbenzene

Concen: 0.735 ug/l

RT: 12.335 min Scan# 1844

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06



Instrument : MSVOA\_X

ClientSampleId : VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

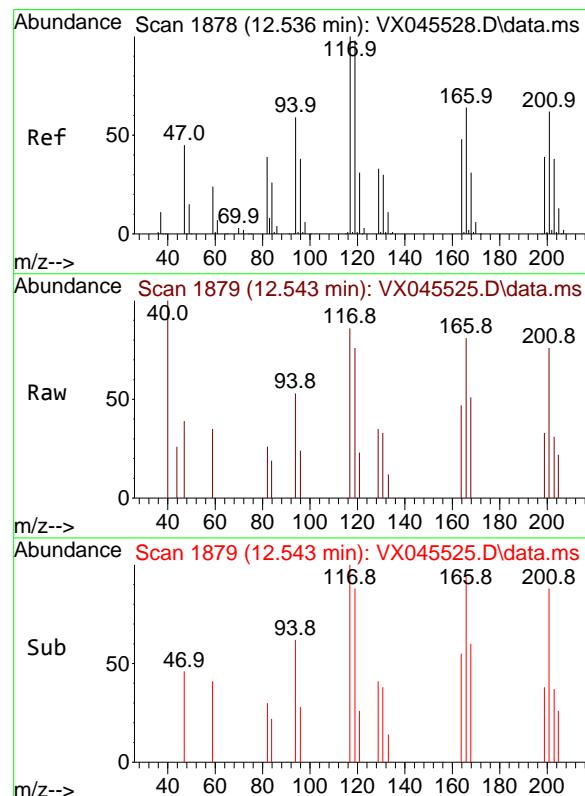

#90

Hexachloroethane

Concen: 0.863 ug/l


RT: 12.543 min Scan# 1879







Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt	Ion:	117	Resp:	602
Ion	Ratio	Lower	Upper	
117	100			
201	66.3	31.2	93.6	

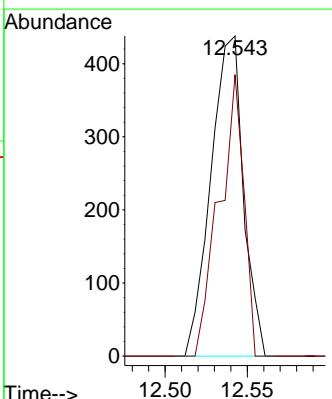



#91

1,2-Dichlorobenzene

Concen: 0.981 ug/l

RT: 12.335 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

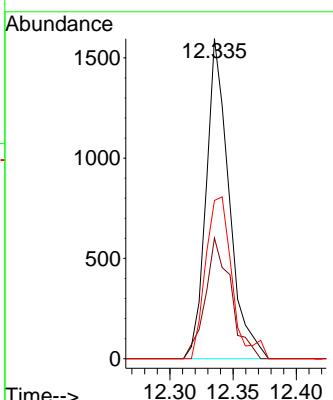

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.665 ug/l

RT: 12.945 min Scan# 1945

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06


Tgt Ion: 75 Resp: 239


Ion Ratio Lower Upper

75 100

155 105.4 34.9 104.7#

157 103.8 44.9 134.7

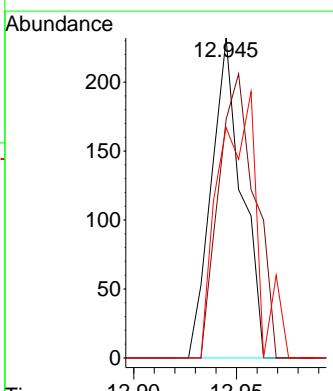


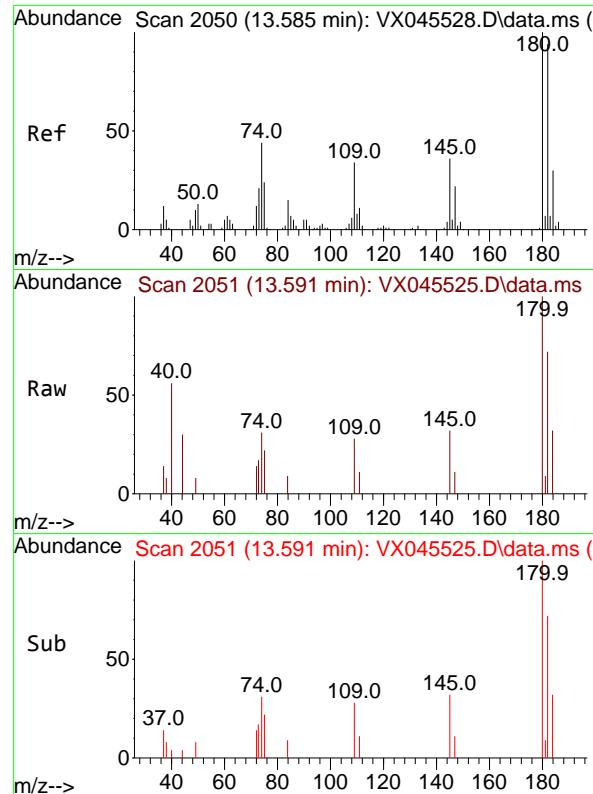


#93  
1,2,4-Trichlorobenzene  
Concen: 0.779 ug/l  
RT: 13.591 min Scan# 2051  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**







Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

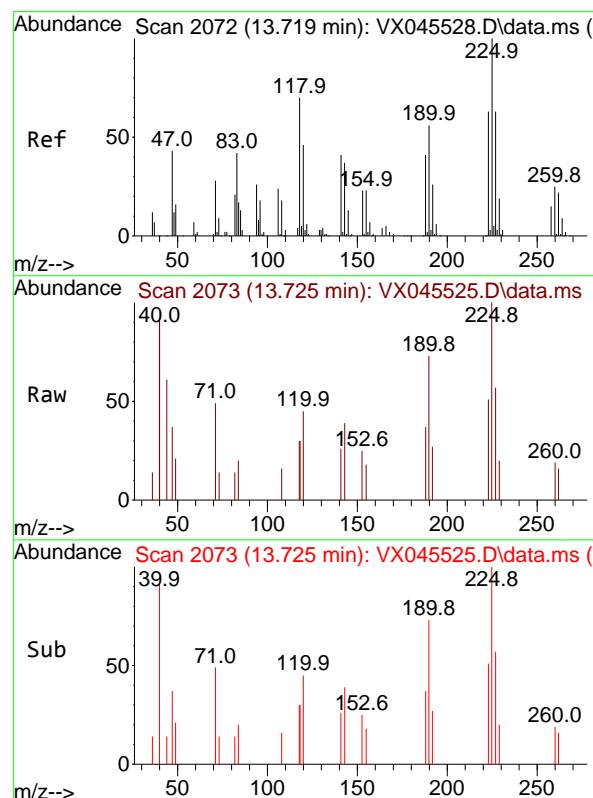

#94  
Hexachlorobutadiene  
Concen: 0.943 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. 0.006 min  
Lab File: VX045525.D  
Acq: 01 Apr 2025 17:06

Tgt Ion:225 Resp: 463  
Ion Ratio Lower Upper  
225 100  
223 54.9 31.1 93.3  
227 56.4 32.2 96.6



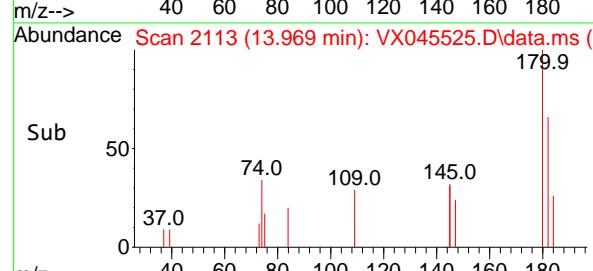

#95

Naphthalene

Concen: 0.733 ug/l

RT: 13.780 min Scan# 2

Delta R.T. 0.006 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

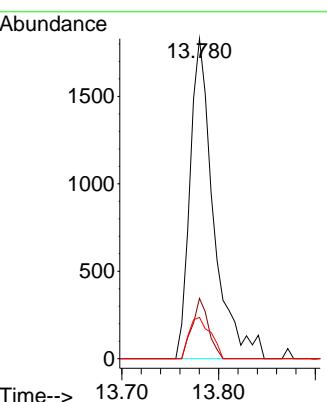

#96

1,2,3-Trichlorobenzene

Concen: 0.801 ug/l


RT: 13.969 min Scan# 2113

Delta R.T. 0.012 min

Lab File: VX045525.D

Acq: 01 Apr 2025 17:06

Tgt	Ion:180	Resp:	956
Ion	Ratio	Lower	Upper
180	100		
182	80.5	47.3	141.8
145	40.4	18.2	54.6

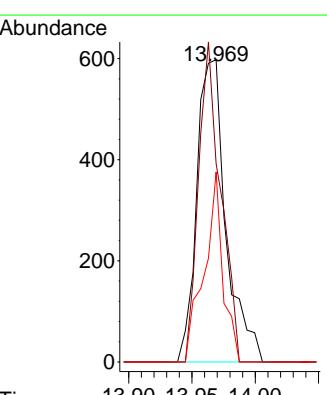

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045526.D  
 Acq On : 01 Apr 2025 17:29  
 Operator : JC/MD  
 Sample : VSTDICC005  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC005

Quant Time: Apr 02 02:51:06 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	93234	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	166137	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	143937	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	63909	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.958	65	8969	5.260	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	10.520%	#
35) Dibromofluoromethane	5.391	113	6181	5.244	ug/l	0.01
Spiked Amount 50.000	Range 75 - 124		Recovery	=	10.480%	#
50) Toluene-d8	8.647	98	20890	5.077	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	10.160%	#
62) 4-Bromofluorobenzene	11.079	95	6867	4.582	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	9.160%	#
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	6482	4.649	ug/l	91
3) Chloromethane	1.307	50	6846	4.779	ug/l	99
4) Vinyl Chloride	1.374	62	6169	4.706	ug/l	100
5) Bromomethane	1.593	94	3185	5.124	ug/l	90
6) Chloroethane	1.666	64	3703	5.324	ug/l	96
7) Trichlorofluoromethane	1.874	101	9316	4.766	ug/l	94
8) Diethyl Ether	2.136	74	3171	4.832	ug/l	96
9) 1,1,2-Trichlorotrifluo...	2.325	101	5589	4.879	ug/l	99
10) Methyl Iodide	2.447	142	6574	4.601	ug/l	97
11) Tert butyl alcohol	2.983	59	5186	22.633	ug/l	99
12) 1,1-Dichloroethene	2.313	96	5485	4.901	ug/l	90
13) Acrolein	2.239	56	8202	25.993	ug/l	97
14) Allyl chloride	2.654	41	9960	4.690	ug/l	95
15) Acrylonitrile	3.069	53	17811	24.624	ug/l	97
16) Acetone	2.386	43	17188	24.550	ug/l	99
17) Carbon Disulfide	2.502	76	12376	4.477	ug/l	# 93
18) Methyl Acetate	2.703	43	8042	4.989	ug/l	96
19) Methyl tert-butyl Ether	3.111	73	18314	4.677	ug/l	100
20) Methylene Chloride	2.782	84	6481	4.945	ug/l	96
21) trans-1,2-Dichloroethene	3.087	96	5534	4.840	ug/l	95
22) Diisopropyl ether	3.764	45	19765	4.725	ug/l	# 82
23) Vinyl Acetate	3.721	43	78907	21.831	ug/l	98
24) 1,1-Dichloroethane	3.605	63	11562	4.887	ug/l	98
25) 2-Butanone	4.574	43	25026	24.419	ug/l	99
26) 2,2-Dichloropropane	4.477	77	7054	4.615	ug/l	95
27) cis-1,2-Dichloroethene	4.483	96	6485	4.655	ug/l	95
28) Bromochloromethane	4.898	49	5666	4.956	ug/l	95
29) Tetrahydrofuran	5.013	42	15913	23.950	ug/l	100
30) Chloroform	5.087	83	12200	5.012	ug/l	99
31) Cyclohexane	5.465	56	9731	4.653	ug/l	97
32) 1,1,1-Trichloroethane	5.379	97	9811	4.763	ug/l	99
36) 1,1-Dichloropropene	5.690	75	7354	4.621	ug/l	98
37) Ethyl Acetate	4.721	43	9384	4.679	ug/l	# 91
38) Carbon Tetrachloride	5.666	117	8264	4.804	ug/l	99
39) Methylcyclohexane	7.379	83	8757	4.489	ug/l	95
40) Benzene	6.038	78	23522	4.839	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045526.D  
 Acq On : 01 Apr 2025 17:29  
 Operator : JC/MD  
 Sample : VSTDICC005  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC005

Quant Time: Apr 02 02:51:06 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	4593	4.302	ug/1	92
42) 1,2-Dichloroethane	6.092	62	9713	4.838	ug/1	100
43) Isopropyl Acetate	6.348	43	13803	4.541	ug/1	97
44) Trichloroethene	7.129	130	5355	4.635	ug/1	99
45) 1,2-Dichloropropane	7.434	63	6060	4.997	ug/1	99
46) Dibromomethane	7.580	93	4767	5.120	ug/1	99
47) Bromodichloromethane	7.818	83	8619	4.636	ug/1 #	97
48) Methyl methacrylate	7.696	41	6908	4.401	ug/1	98
49) 1,4-Dioxane	7.665	88	3205	112.864	ug/1	95
51) 4-Methyl-2-Pentanone	8.574	43	48050	23.844	ug/1	97
52) Toluene	8.714	92	14391	4.893	ug/1	100
53) t-1,3-Dichloropropene	8.982	75	6643	5.834	ug/1	97
54) cis-1,3-Dichloropropene	8.366	75	7873	4.506	ug/1	95
55) 1,1,2-Trichloroethane	9.153	97	5741	4.898	ug/1	90
56) Ethyl methacrylate	9.116	69	8012	4.417	ug/1	95
57) 1,3-Dichloropropane	9.305	76	10208	5.002	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.244	63	21382	23.302	ug/1	99
59) 2-Hexanone	9.433	43	35628	23.875	ug/1	99
60) Dibromochloromethane	9.519	129	5855	4.582	ug/1	99
61) 1,2-Dibromoethane	9.610	107	5837	4.920	ug/1	98
64) Tetrachloroethene	9.275	164	5373	5.287	ug/1	93
65) Chlorobenzene	10.073	112	15178	4.935	ug/1	96
66) 1,1,1,2-Tetrachloroethane	10.159	131	4945	4.631	ug/1	97
67) Ethyl Benzene	10.195	91	26180	4.753	ug/1	97
68) m/p-Xylenes	10.299	106	19268	9.617	ug/1	99
69) o-Xylene	10.640	106	9735	4.932	ug/1	99
70) Styrene	10.653	104	15017	4.610	ug/1	96
71) Bromoform	10.799	173	3634	4.558	ug/1 #	95
73) Isopropylbenzene	10.964	105	24604	4.806	ug/1	100
74) N-amyl acetate	10.848	43	10750	4.390	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	9127	5.075	ug/1	98
76) 1,2,3-Trichloropropane	11.238	75	8032m	5.152	ug/1	
77) Bromobenzene	11.195	156	5927	5.011	ug/1	97
78) n-propylbenzene	11.305	91	27777	4.711	ug/1	98
79) 2-Chlorotoluene	11.360	91	18358	4.870	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	19936	4.710	ug/1	98
81) trans-1,4-Dichloro-2-b...	11.018	75	1752	3.814	ug/1	85
82) 4-Chlorotoluene	11.457	91	20171	4.799	ug/1	99
83) tert-Butylbenzene	11.713	119	19962	4.763	ug/1	98
84) 1,2,4-Trimethylbenzene	11.750	105	19998	4.707	ug/1	99
85) sec-Butylbenzene	11.890	105	24465	4.753	ug/1	100
86) p-Isopropyltoluene	12.006	119	20178	4.755	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	10255	4.763	ug/1	98
88) 1,4-Dichlorobenzene	12.036	146	11016	5.047	ug/1	93
89) n-Butylbenzene	12.329	91	15887	4.317	ug/1	98
90) Hexachloroethane	12.536	117	3151	4.320	ug/1	98
91) 1,2-Dichlorobenzene	12.335	146	10510	4.910	ug/1	98
92) 1,2-Dibromo-3-Chloropr...	12.945	75	1661	4.417	ug/1	92
93) 1,2,4-Trichlorobenzene	13.591	180	5391	4.524	ug/1	95
94) Hexachlorobutadiene	13.719	225	2483	4.836	ug/1	98
95) Naphthalene	13.774	128	19618	4.424	ug/1	97
96) 1,2,3-Trichlorobenzene	13.957	180	5854	4.692	ug/1	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045526.D  
 Acq On : 01 Apr 2025 17:29  
 Operator : JC/MD  
 Sample : VSTDICC005  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC005

Quant Time: Apr 02 02:51:06 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045526.D  
 Acq On : 01 Apr 2025 17:29  
 Operator : JC/MD  
 Sample : VSTDICC005  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1




Quant Time: Apr 02 02:51:06 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC005

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

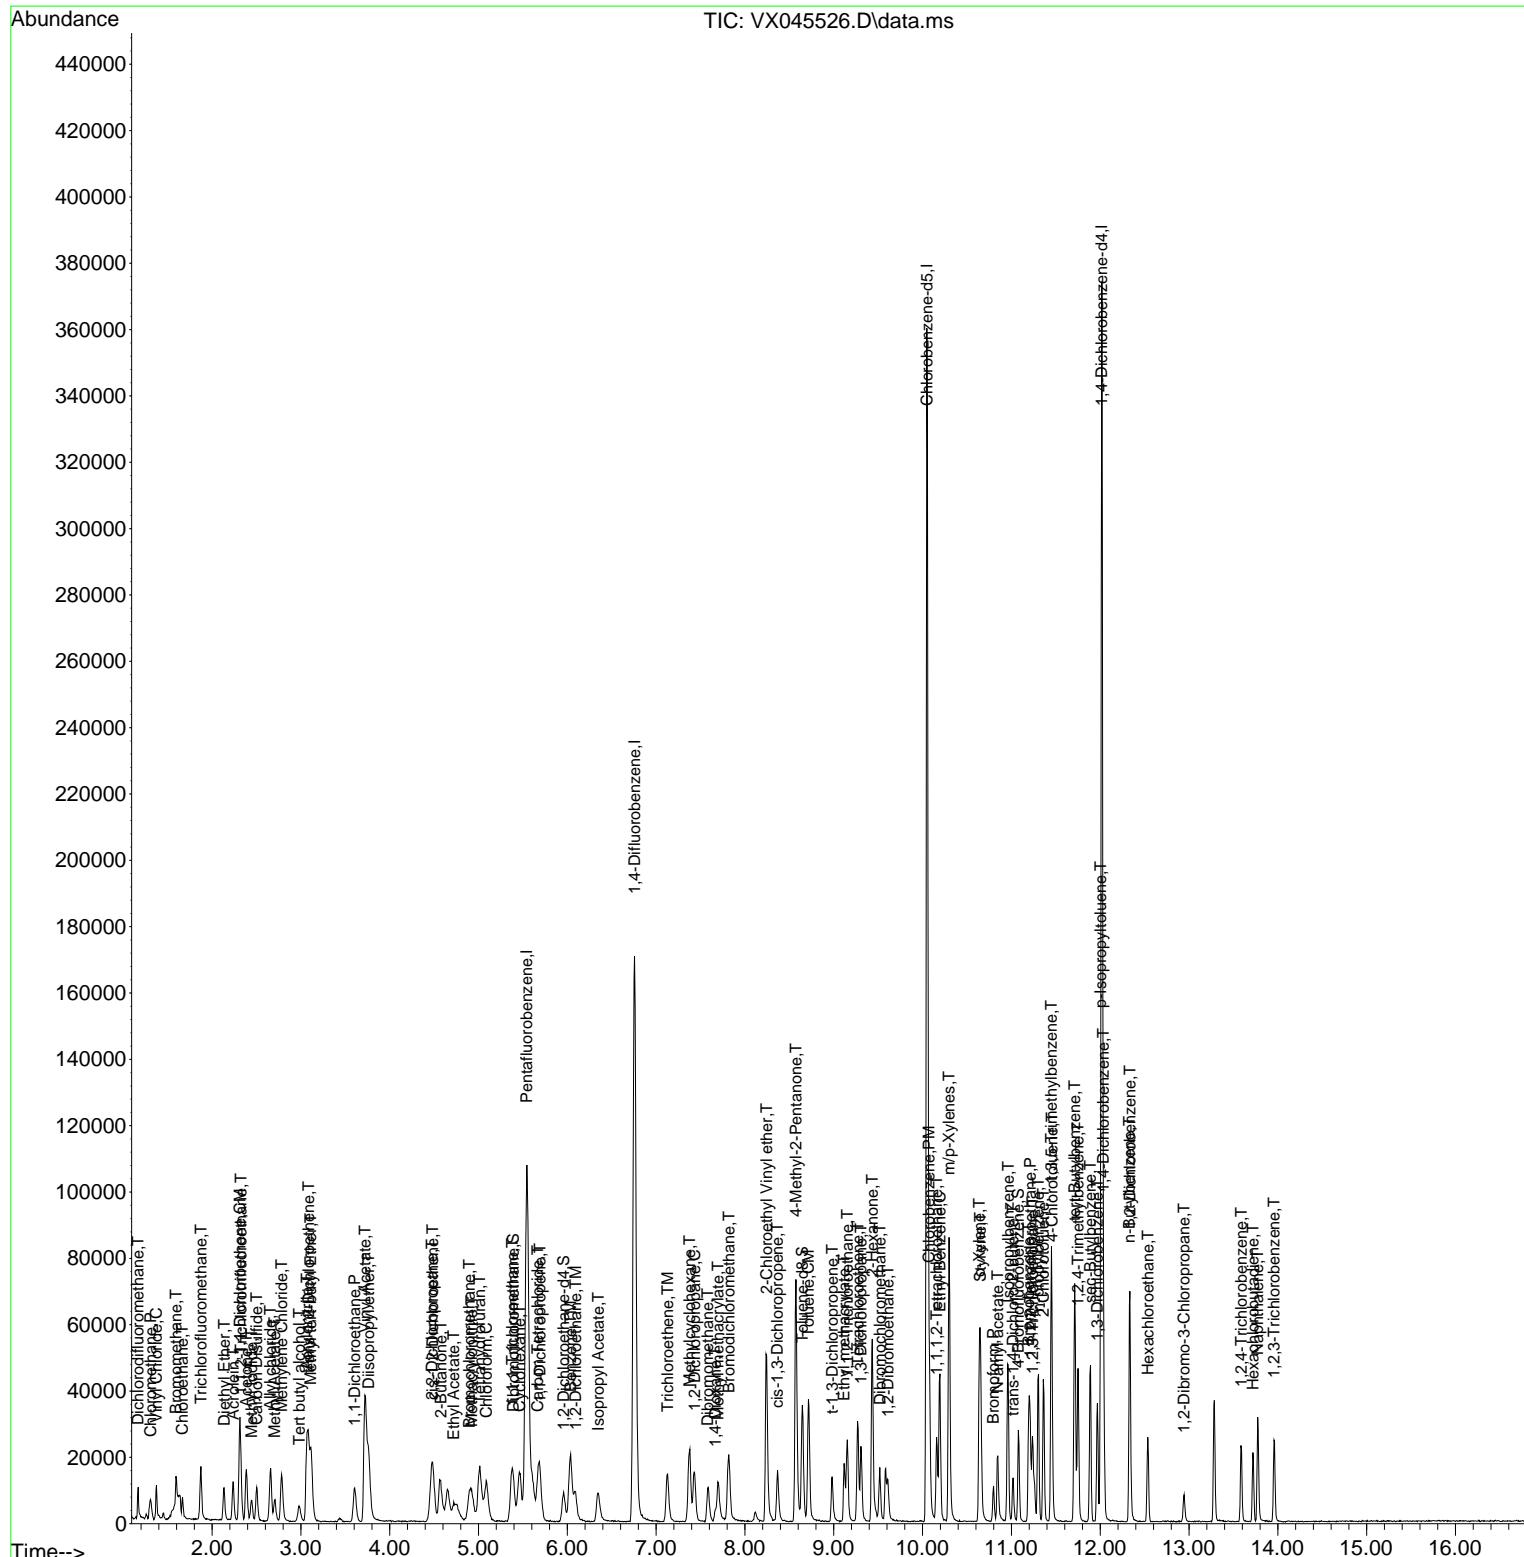

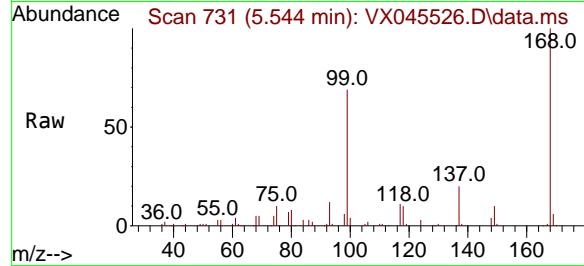

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.544 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#2

Dichlorodifluoromethane

Concen: 4.649 ug/l


RT: 1.166 min Scan# 13




Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion: 85 Resp: 6482  
 Ion Ratio Lower Upper  
 85 100  
 87 27.3 16.1 48.2

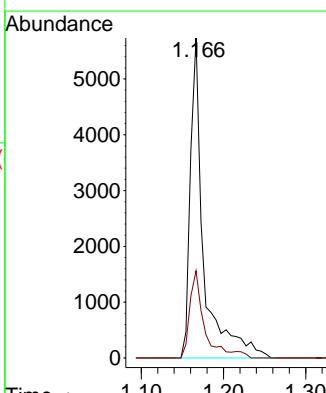



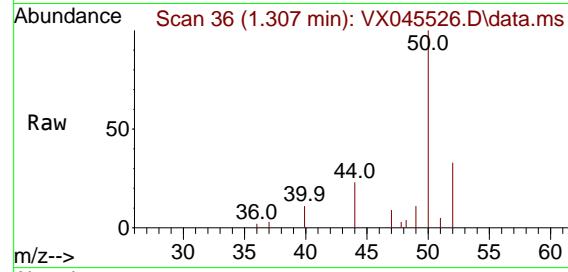



#3  
Chloromethane  
Concen: 4.779 ug/l  
RT: 1.307 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

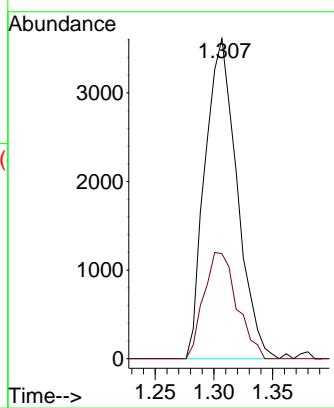

#4  
Vinyl Chloride  
Concen: 4.706 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion: 62 Resp: 6169  
Ion Ratio Lower Upper  
62 100  
64 31.9 25.5 38.3

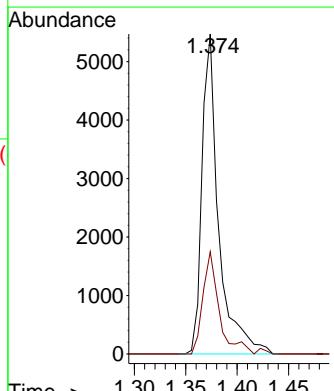







#5  
 Bromomethane  
 Concen: 5.124 ug/l  
 RT: 1.593 min Scan# 8  
 Delta R.T. 0.000 min  
 Lab File: VX045526.D  
 Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

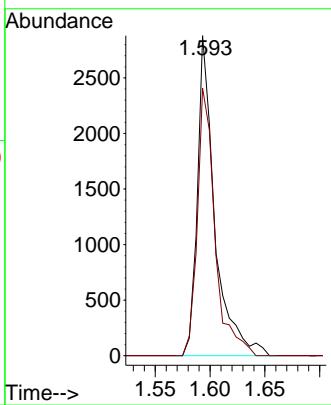

#6  
 Chloroethane  
 Concen: 5.324 ug/l  
 RT: 1.666 min Scan# 95  
 Delta R.T. 0.000 min  
 Lab File: VX045526.D  
 Acq: 01 Apr 2025 17:29

Tgt Ion: 64 Resp: 3703  
 Ion Ratio Lower Upper  
 64 100  
 66 30.9 26.3 39.5

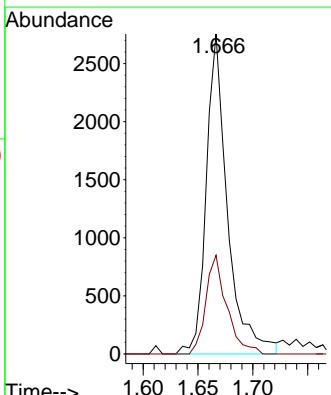


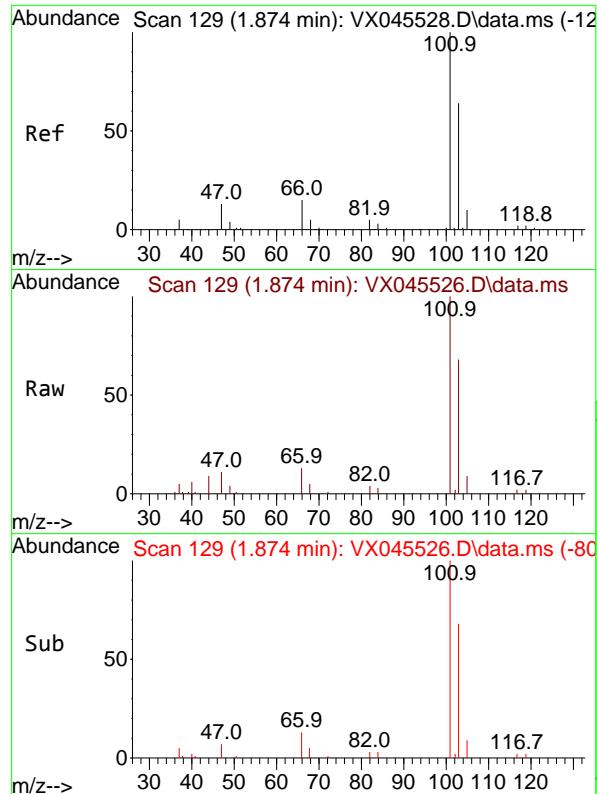


#7  
Trichlorofluoromethane  
Concen: 4.766 ug/l  
RT: 1.874 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

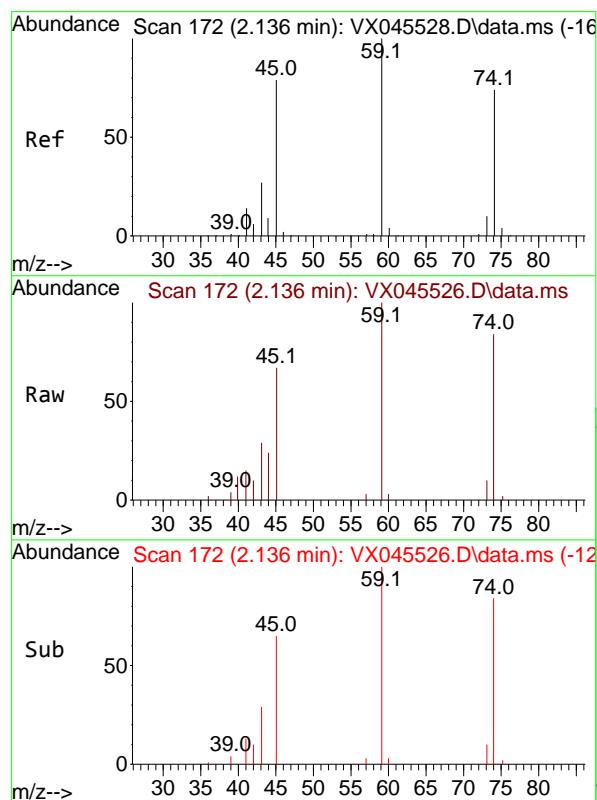

#8  
Diethyl Ether  
Concen: 4.832 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29


Tgt Ion: 74 Resp: 3171  
Ion Ratio Lower Upper  
74 100  
45 110.2 53.0 159.1

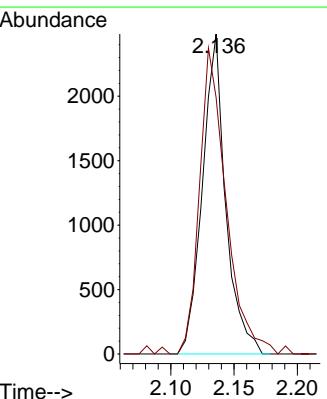



#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 4.879 ug/l  
RT: 2.325 min Scan# 21  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29



Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005

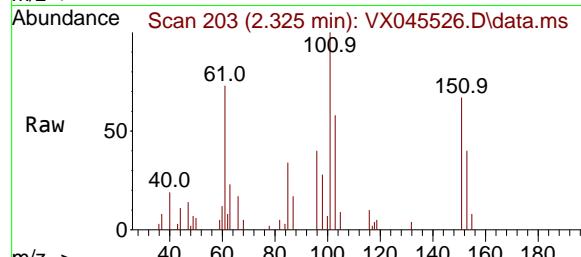


Tgt	Ion:101	Ion Ratio	Resp:	5589
	100		Lower	Upper
101	100			
85	47.8	38.9	58.3	
151	72.4	57.5	86.3	

Manual Integrations  
APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

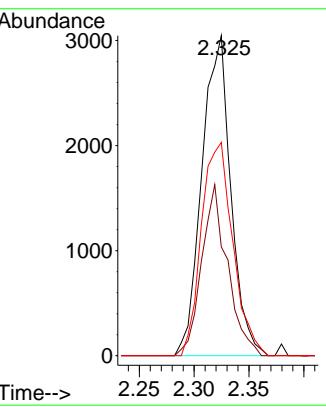


#10  
Methyl Iodide  
Concen: 4.601 ug/l  
RT: 2.447 min Scan# 223  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29



Tgt	Ion:142	Ion Ratio	Resp:	6574
	100		Lower	Upper
142	100			
127	48.4	40.2	60.4	
141	13.7	11.7	17.5	

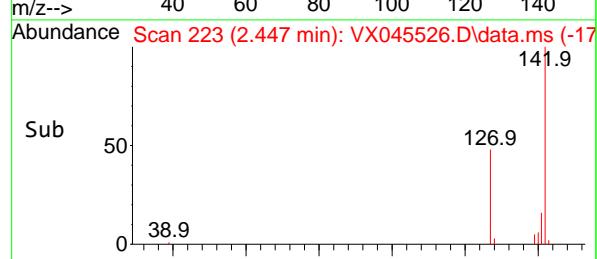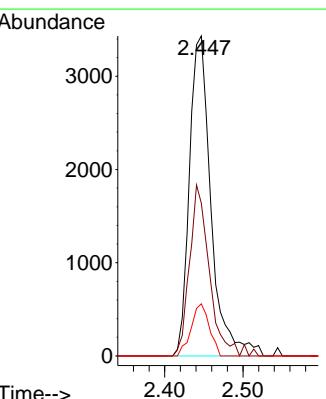



Ref 50

0

50.0 55.0 60.0 65.0 70.0

30 35 40 45 50 55 60 65 70

m/z-->

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1

50.0

41.1

35.9

59.1


50.0

41.1

35.9

59.1





50.0




#13

Acrolein  
Concen: 25.993 ug/l  
RT: 2.239 min Scan# 189  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29



Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005









#14  
Allyl chloride  
Concen: 4.690 ug/l  
RT: 2.654 min Scan# 257  
Delta R.T. -0.006 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29



Tgt Ion: 41 Resp: 9960  
Ion Ratio Lower Upper  
41 100  
39 79.8 60.2 90.2  
76 28.8 24.6 36.8

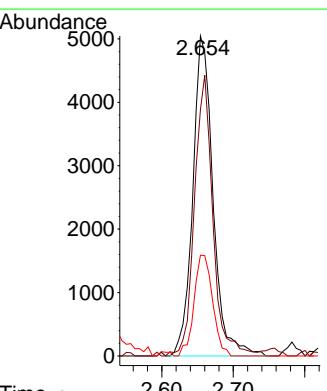

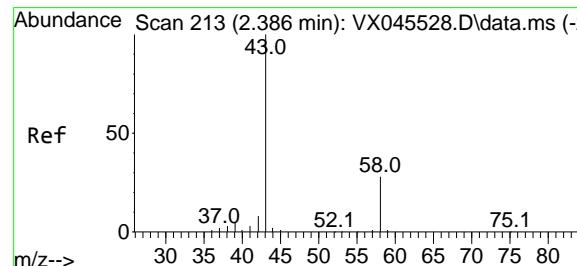

#15

Acrylonitrile

Concen: 24.624 ug/l

RT: 3.069 min Scan# 3

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

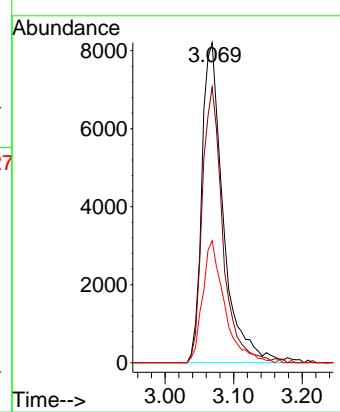

#16

Acetone

Concen: 24.550 ug/l

RT: 2.386 min Scan# 213

Delta R.T. 0.000 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29


Tgt Ion: 43 Resp: 17188

Ion Ratio Lower Upper


43 100

58 28.4 22.3 33.5

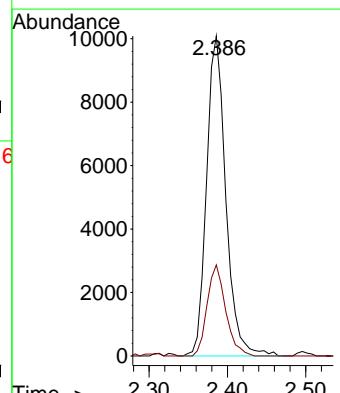





Abundance Scan 232 (2.502 min): VX045526.D\data.ms

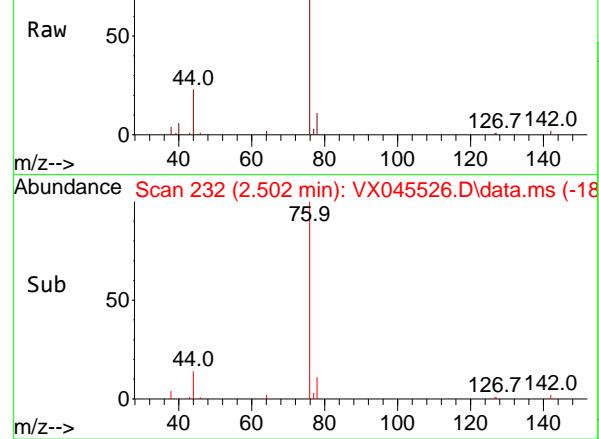


Abundance Scan 232 (2.502 min): VX045526.D\data.ms (-18)

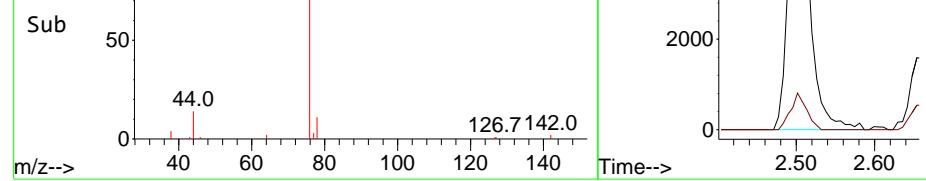


Abundance Scan 265 (2.703 min): VX045528.D\data.ms (-25)

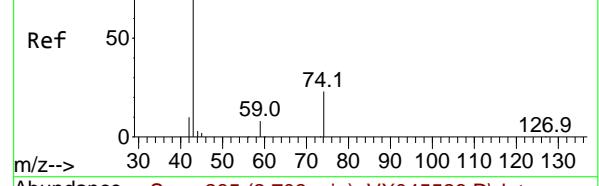

Abundance Scan 265 (2.703 min): VX045526.D\data.ms

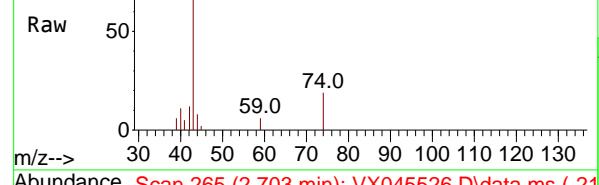

Abundance Scan 265 (2.703 min): VX045526.D\data.ms (-21)

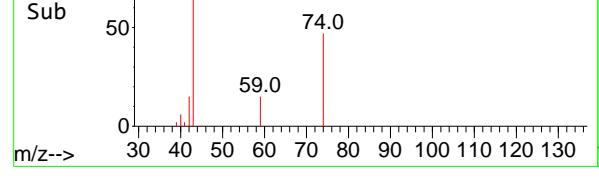

#17

Carbon Disulfide

Concen: 4.477 ug/l

RT: 2.502 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#18

Methyl Acetate

Concen: 4.989 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29


Tgt Ion: 43 Resp: 8042

Ion Ratio Lower Upper

43 100

74 20.2 17.5 26.3



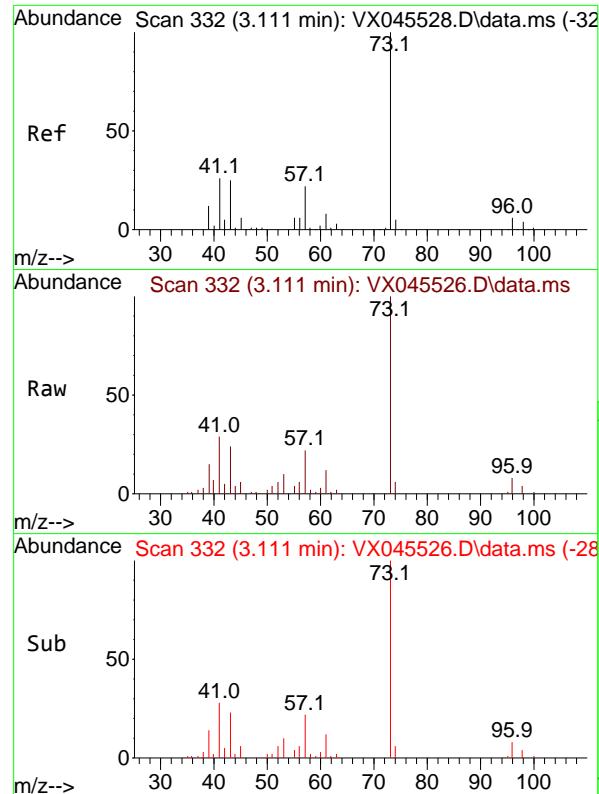



#19

Methyl tert-butyl Ether  
Concen: 4.677 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025


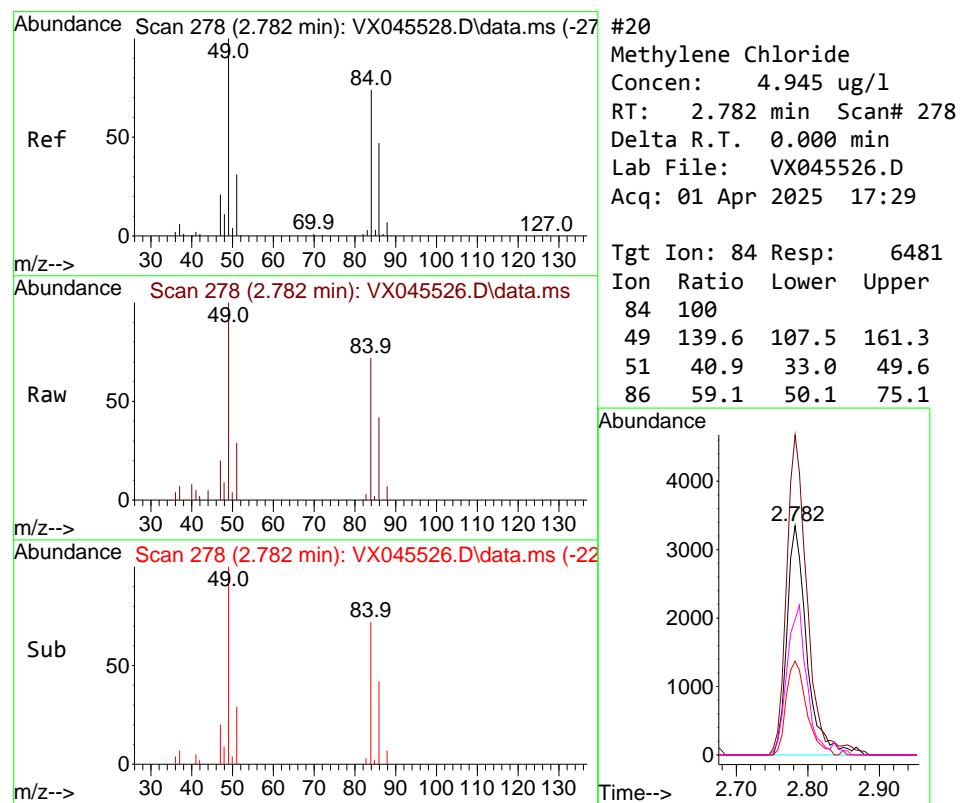
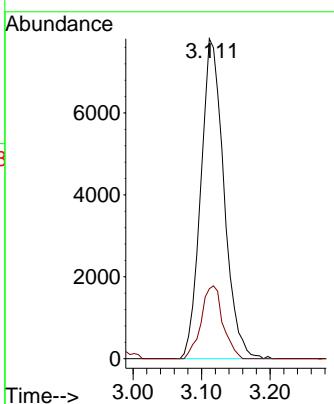


#20

Methylene Chloride  
Concen: 4.945 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion: 84 Resp: 6481  
Ion Ratio Lower Upper  
84 100  
49 139.6 107.5 161.3  
51 40.9 33.0 49.6  
86 59.1 50.1 75.1

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16







#21  
trans-1,2-Dichloroethene  
Concen: 4.840 ug/l  
RT: 3.087 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


### Manual Integrations APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

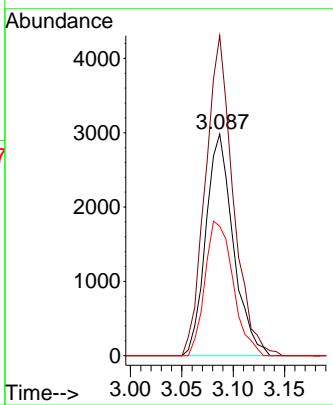

#22  
Diisopropyl ether  
Concen: 4.725 ug/l  
RT: 3.764 min Scan# 439  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion: 45 Resp: 19765  
Ion Ratio Lower Upper  
45 100  
43 94.7 59.3 88.9#  
87 27.8 20.4 30.6  
59 10.3 9.0 13.6



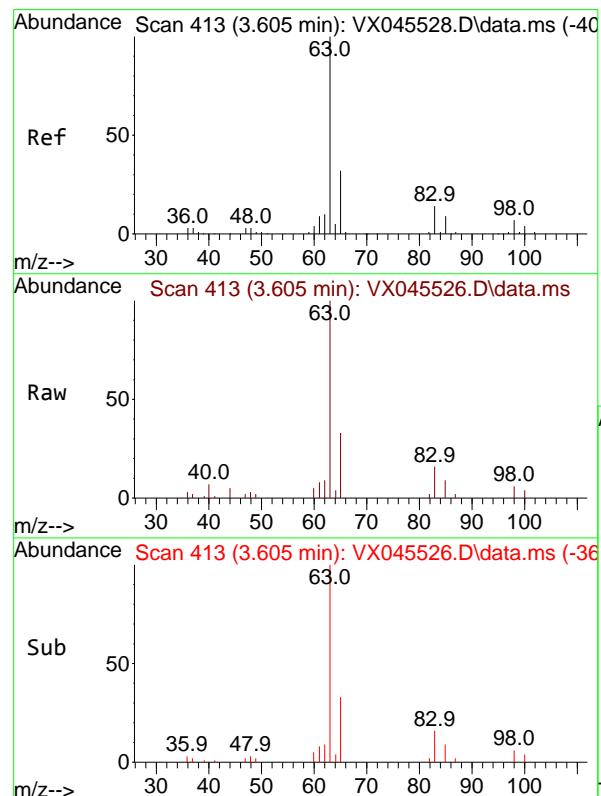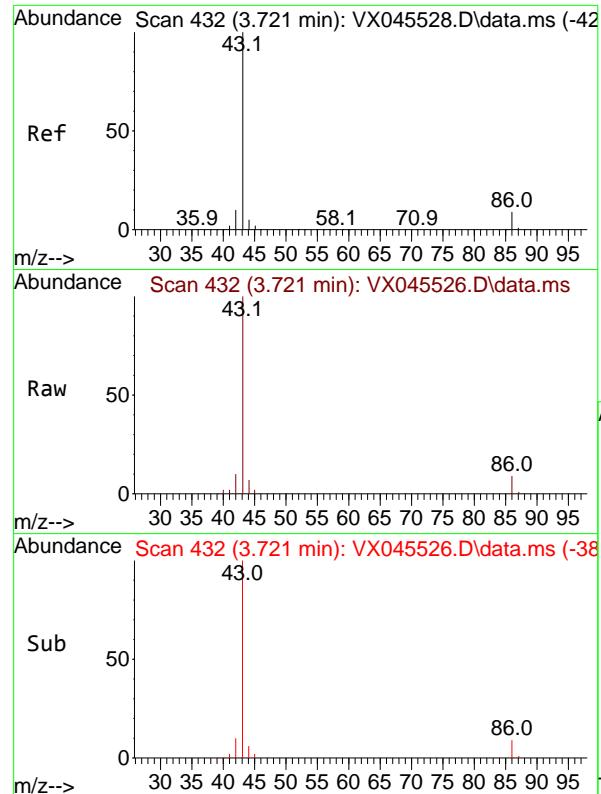

#23

**Vinyl Acetate**

Concen: 21.831 ug/l

RT: 3.721 min Scan# 4

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#24

**1,1-Dichloroethane**

Concen: 4.887 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29


Tgt Ion: 63 Resp: 11562


Ion Ratio Lower Upper

63 100

98 6.3 3.4 10.1


100 3.6 2.2 6.6

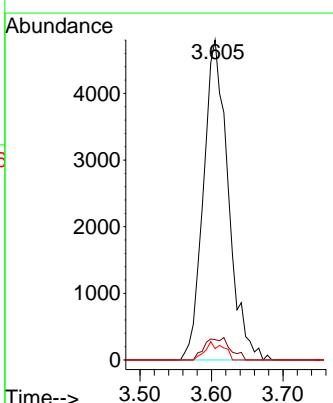



#25  
2-Butanone  
Concen: 24.419 ug/l  
RT: 4.574 min Scan# 51  
Delta R.T. 0.018 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005

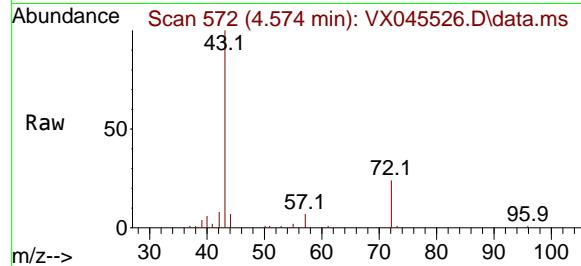


Tgt Ion: 43 Resp: 25020  
Ion Ratio Lower Upper  
43 100  
72 23.8 18.6 28.0

### Manual Integrations APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025


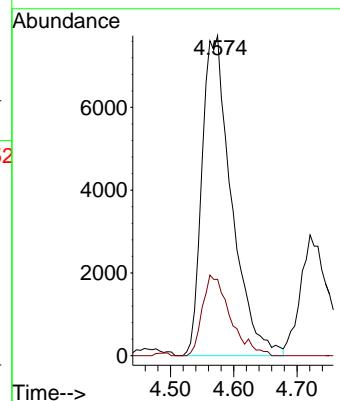



#26  
2,2-Dichloropropane  
Concen: 4.615 ug/l  
RT: 4.477 min Scan# 556  
Delta R.T. 0.006 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29



Tgt Ion: 77 Resp: 7054  
Ion Ratio Lower Upper  
77 100  
97 23.4 10.6 31.8

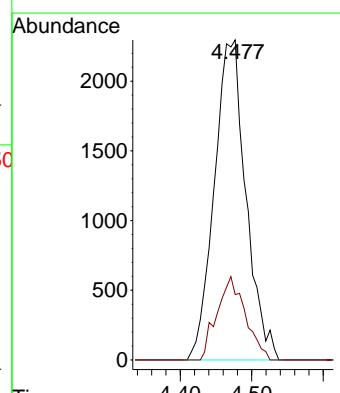


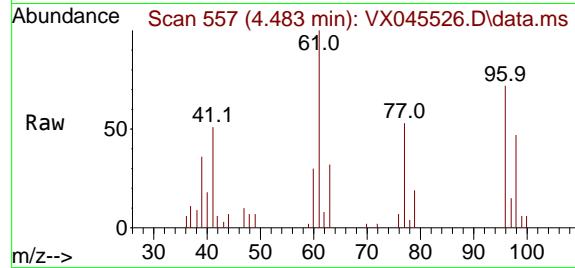
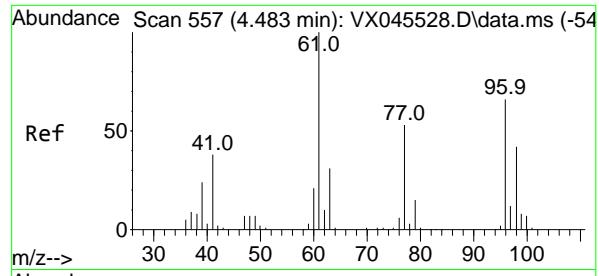


#27  
cis-1,2-Dichloroethene  
Concen: 4.655 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005



### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025



#28  
Bromochloromethane  
Concen: 4.956 ug/l  
RT: 4.898 min Scan# 625  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion: 49 Resp: 5666  
Ion Ratio Lower Upper  
49 100  
129 1.2 0.0 3.8  
130 72.2 54.6 81.8

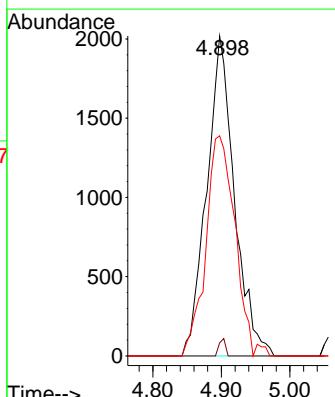

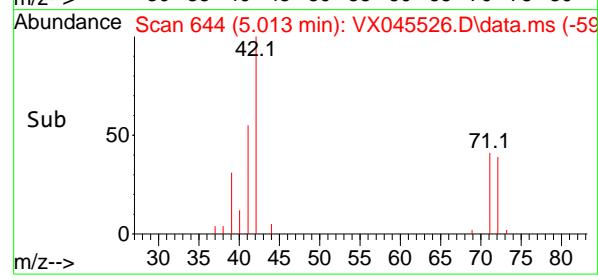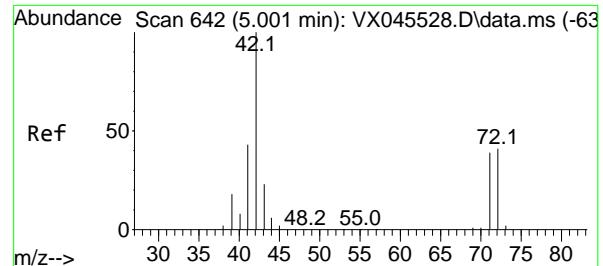

#29

Tetrahydrofuran

Concen: 23.950 ug/l

RT: 5.013 min Scan# 6

Delta R.T. 0.012 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

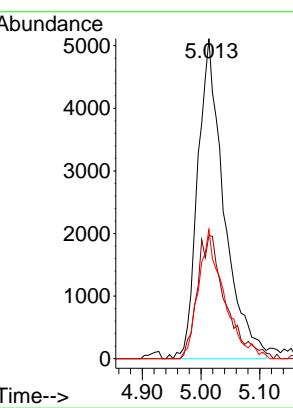

#30

Chloroform

Concen: 5.012 ug/l

RT: 5.087 min Scan# 656


Delta R.T. 0.000 min




Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion: 83 Resp: 12200

Ion	Ratio	Lower	Upper
83	100		
85	65.0	52.8	79.2

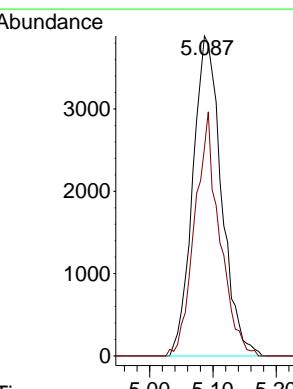

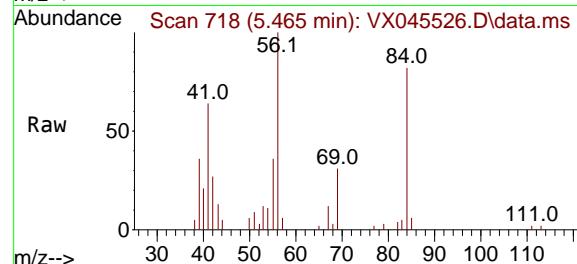

#31

Cyclohexane

Concen: 4.653 ug/l

RT: 5.465 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#32

1,1,1-Trichloroethane

Concen: 4.763 ug/l

RT: 5.379 min Scan# 704


Delta R.T. 0.000 min


Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion: 97 Resp: 9811

Ion	Ratio	Lower	Upper
97	100		
99	63.2	51.7	77.5
61	52.0	41.0	61.4



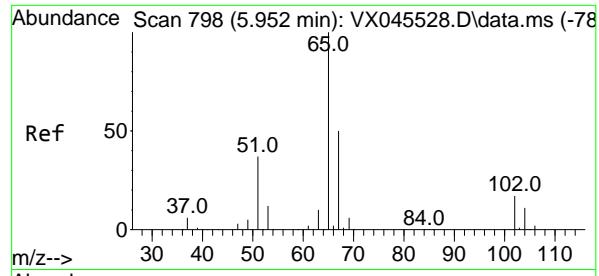

#33

1,2-Dichloroethane-d4

Concen: 5.260 ug/l

RT: 5.958 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29


Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC005

Abundance Scan 799 (5.958 min): VX045526.D\data.ms

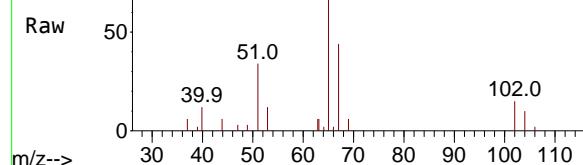

Abundance Scan 799 (5.958 min): VX045526.D\data.ms (-74)

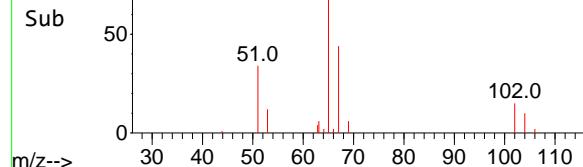

Tgt Ion: 65 Resp: 8969

Ion Ratio Lower Upper

65 100


67 46.7 0.0 99.0

Manual Integrations


APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

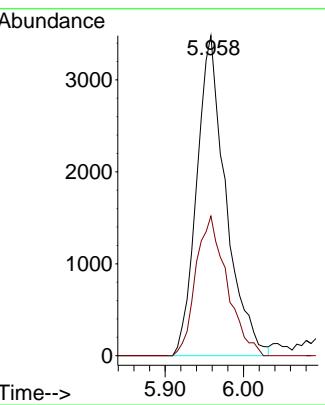

Abundance Scan 930 (6.757 min): VX045528.D\data.ms (-92)

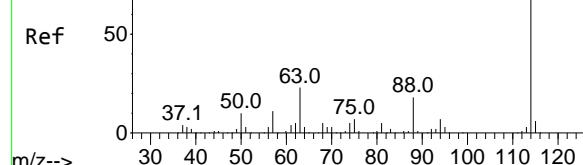

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29


Tgt Ion:114 Resp: 166137

Ion Ratio Lower Upper


114 100

63 24.4 0.0 46.8


88 16.1 0.0 35.4



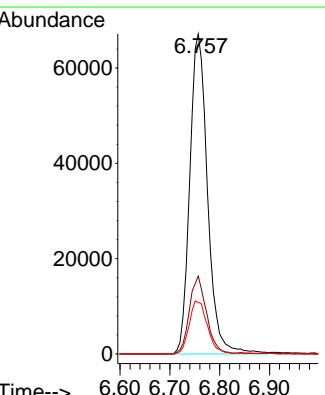


Abundance Scan 930 (6.757 min): VX045526.D\data.ms (-88)

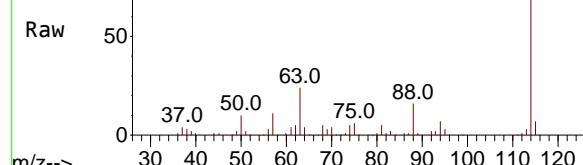

Abundance Scan 930 (6.757 min): VX045526.D\data.ms (-88)

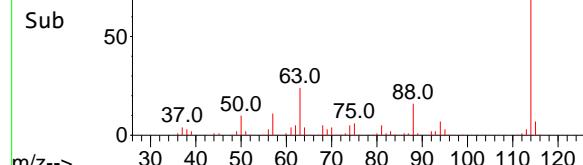

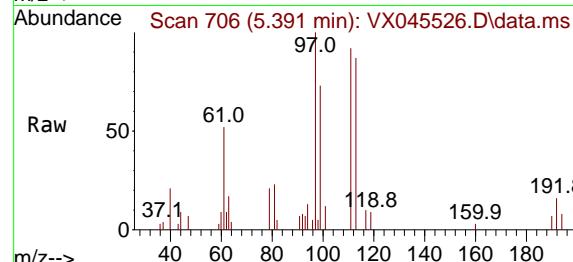

#35

Dibromofluoromethane

Concen: 5.244 ug/l

RT: 5.391 min Scan# 7

Delta R.T. 0.012 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

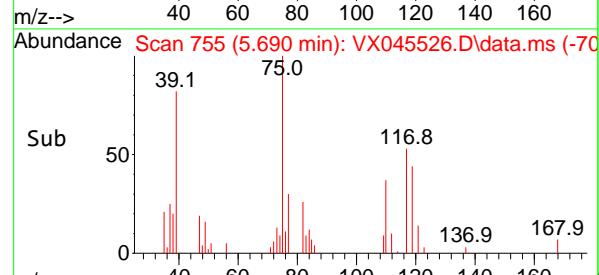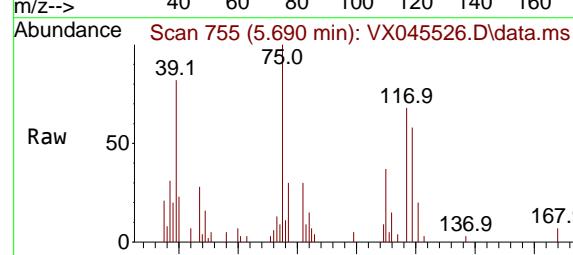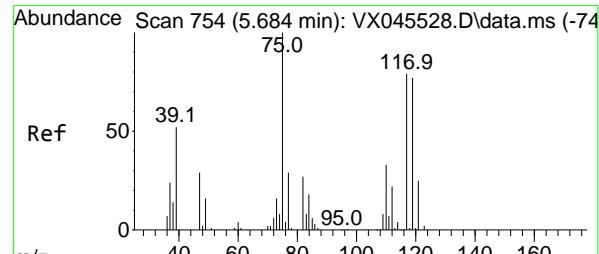

#36

1,1-Dichloropropene

Concen: 4.621 ug/l

RT: 5.690 min Scan# 755

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion: 75 Resp: 7354

Ion Ratio Lower Upper

75 100

110 33.3 16.9 50.6



77 29.8 25.0 37.4


1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16

Abundance

Time--&gt; 5.30 5.40 5.50

5.391

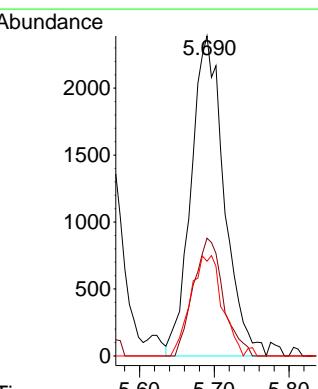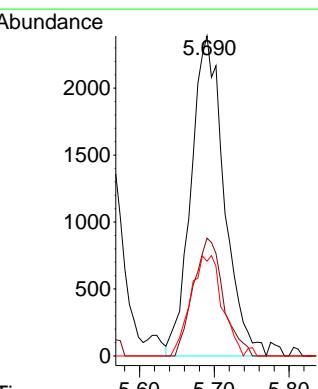

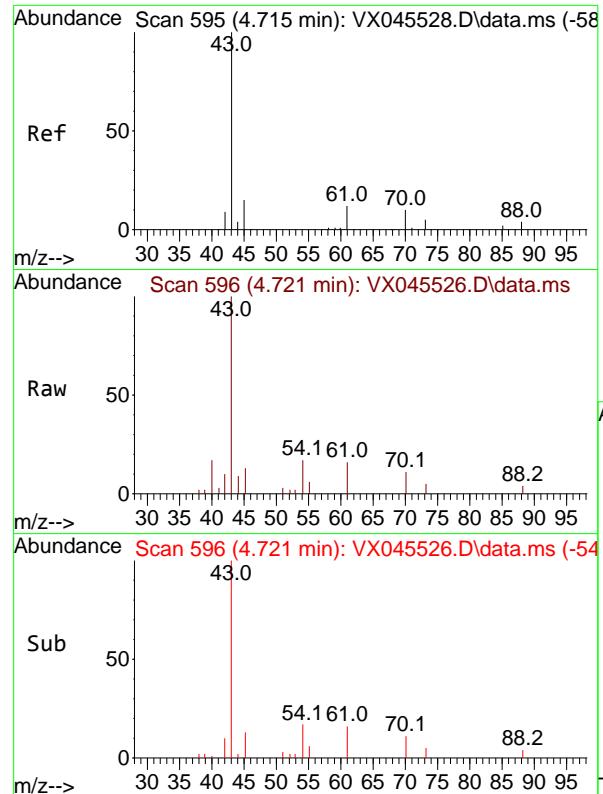

#37

Ethyl Acetate

Concen: 4.679 ug/l

RT: 4.721 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

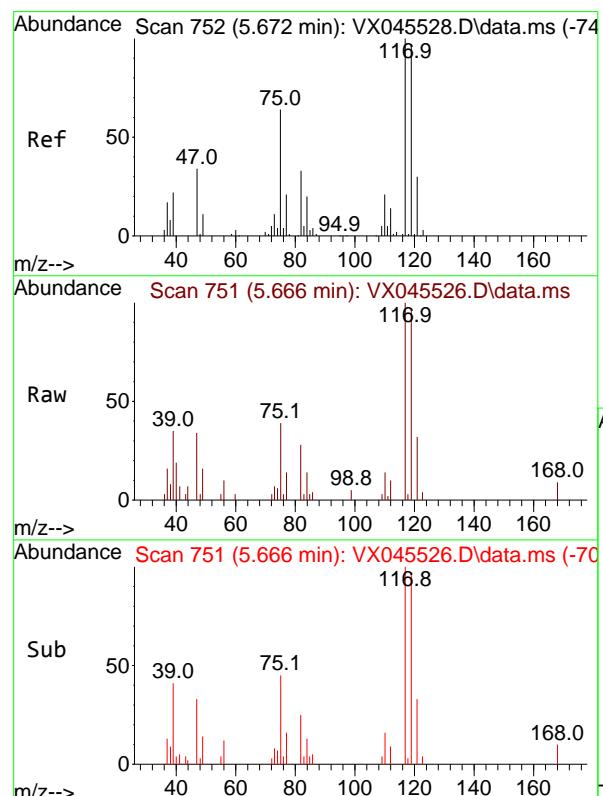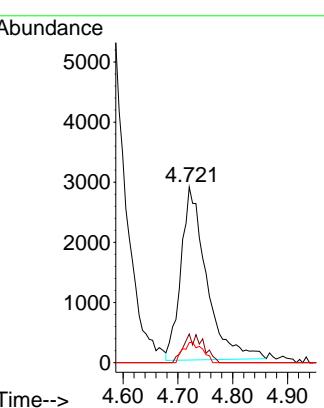

#38

Carbon Tetrachloride

Concen: 4.804 ug/l


RT: 5.666 min Scan# 751


Delta R.T. -0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt	Ion:	117	Resp:	8264
Ion	Ratio	Lower	Upper	
117	100			
119	96.4	76.9	115.3	
121	31.7	24.2	36.2	

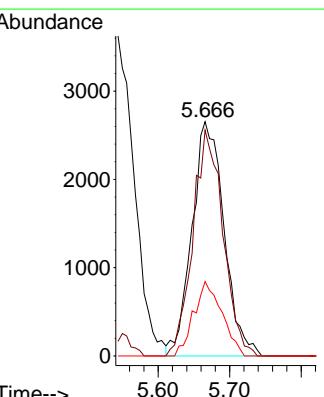

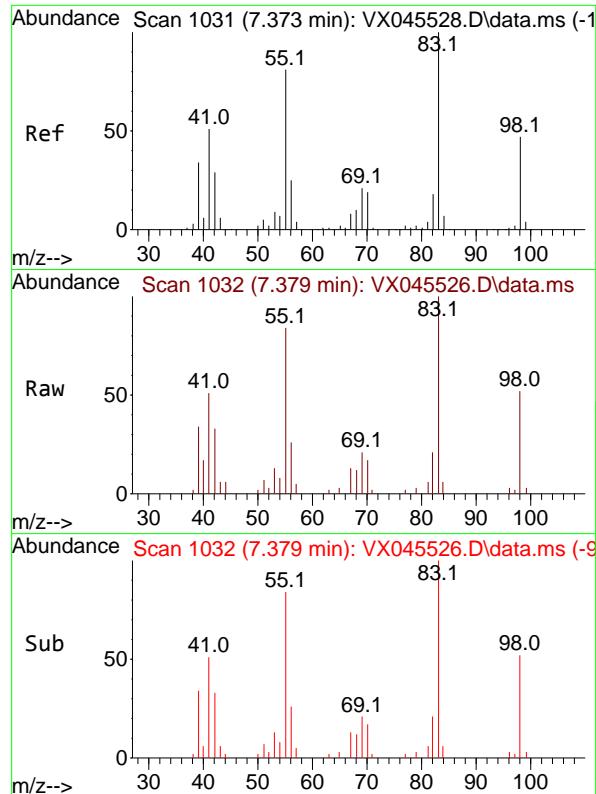

#39

Methylcyclohexane

Concen: 4.489 ug/l

RT: 7.379 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

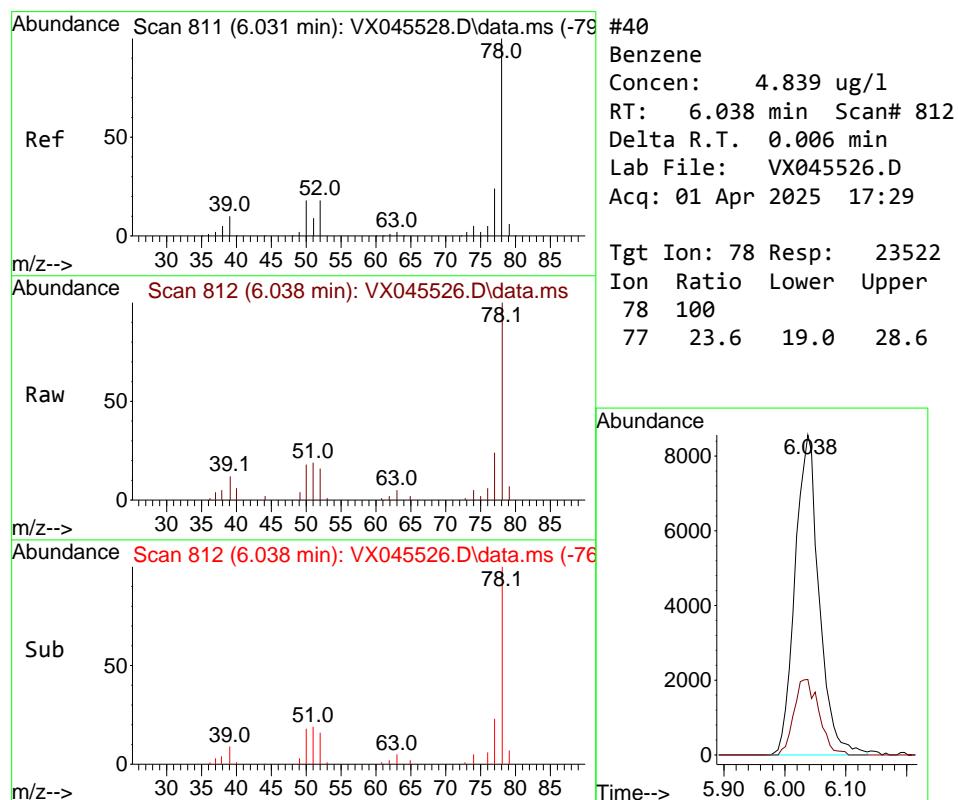

#40

Benzene

Concen: 4.839 ug/l

RT: 6.038 min Scan# 812


Delta R.T. 0.006 min







Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion: 78 Resp: 23522

Ion	Ratio	Lower	Upper
78	100		
77	23.6	19.0	28.6





#41

Methacrylonitrile

Concen: 4.302 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29


Instrument : MSVOA\_X

ClientSampleId : VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

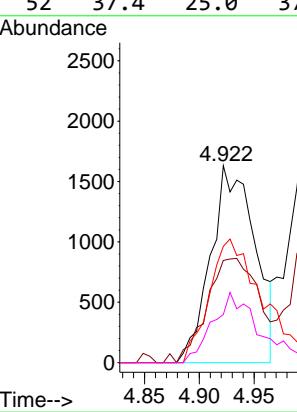

#42

1,2-Dichloroethane

Concen: 4.838 ug/l


RT: 6.092 min Scan# 821


Delta R.T. 0.012 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29





Tgt Ion: 62 Resp: 9713  
 Ion Ratio Lower Upper  
 62 100  
 98 7.7 0.0 15.2

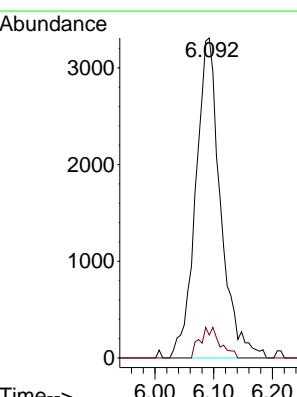

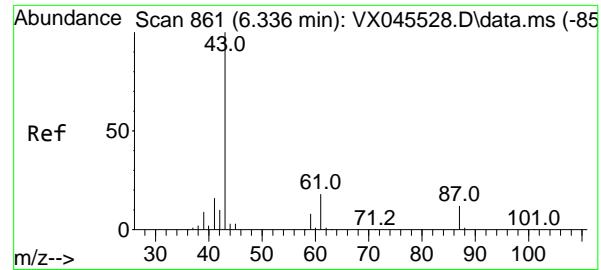

Ref 50  
0

Abundance Scan 863 (6.348 min): VX045526.D\data.ms

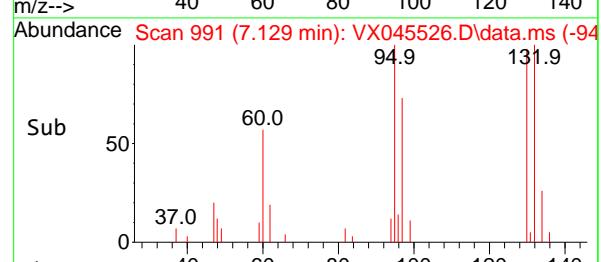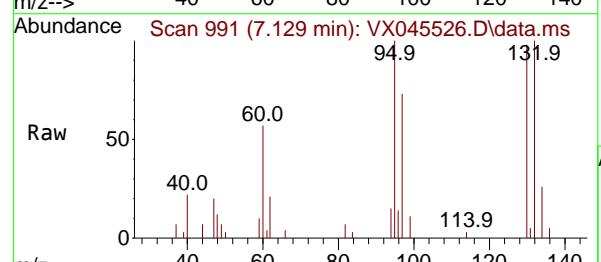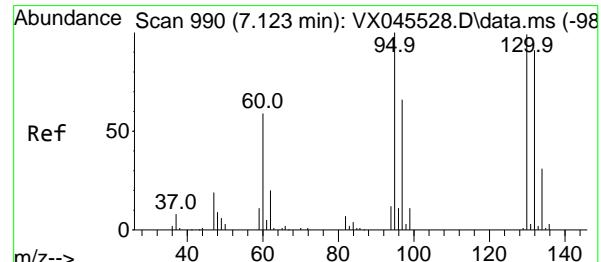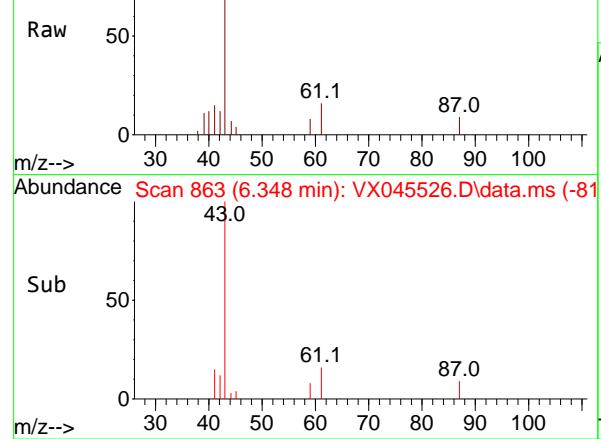

#43

Isopropyl Acetate

Concen: 4.541 ug/l

RT: 6.348 min Scan# 8

Delta R.T. 0.012 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

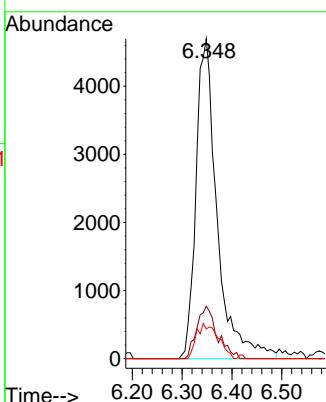

#44

Trichloroethene

Concen: 4.635 ug/l


RT: 7.129 min Scan# 991




Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion:130 Resp: 5355  
 Ion Ratio Lower Upper  
 130 100  
 95 102.2 0.0 202.0

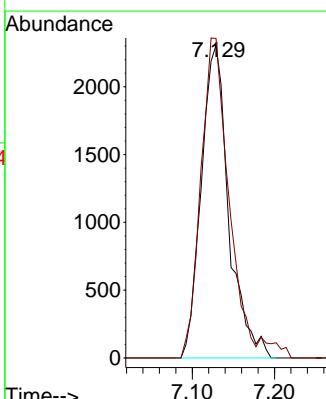



#45

1,2-Dichloropropane

Concen: 4.997 ug/l

RT: 7.434 min Scan# 1040

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

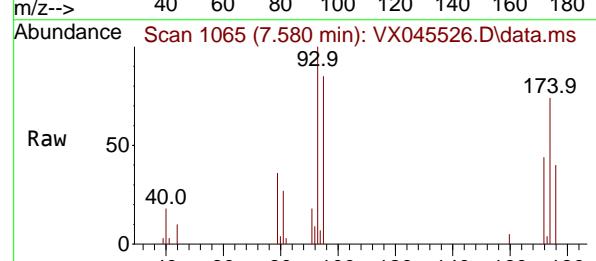

#46

Dibromomethane

Concen: 5.120 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29


Tgt Ion: 93 Resp: 4767


Ion Ratio Lower Upper

93 100

95 81.0 64.8 97.2

174 83.1 65.4 98.0

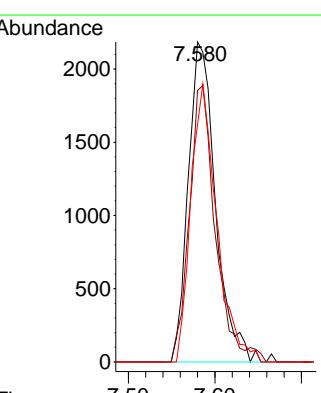


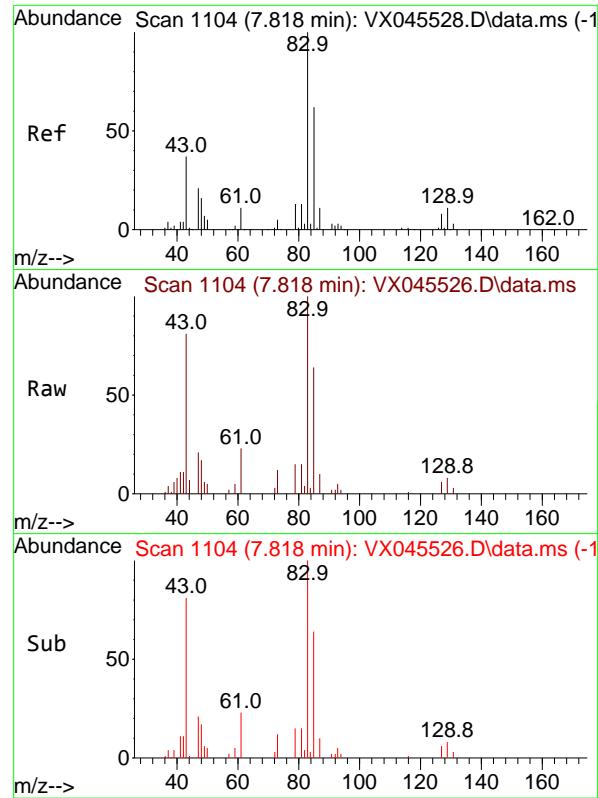


#47  
 Bromodichloromethane  
 Concen: 4.636 ug/l  
 RT: 7.818 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: VX045526.D  
 Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

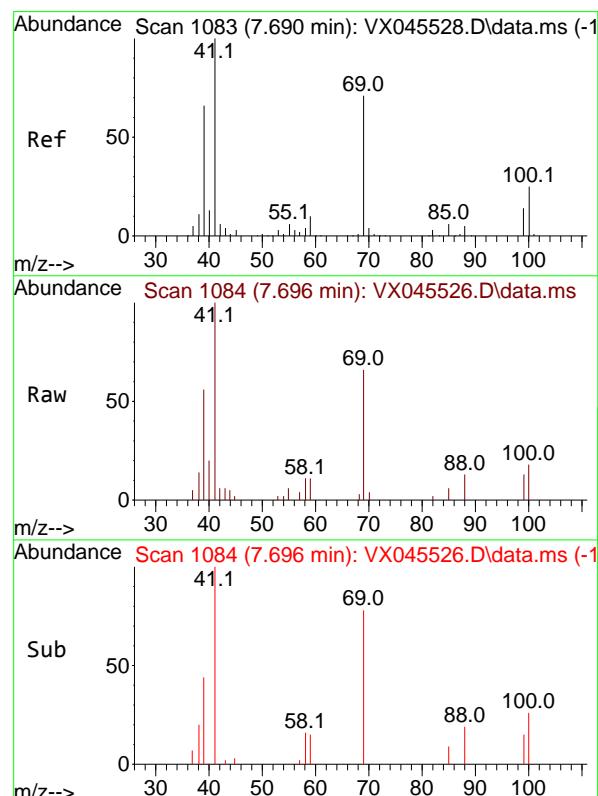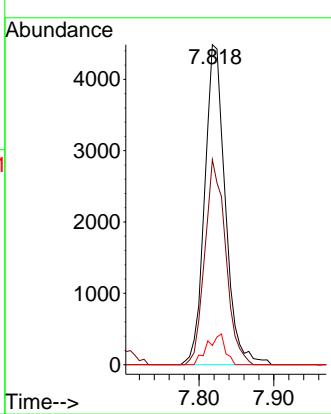

#48  
 Methyl methacrylate  
 Concen: 4.401 ug/l  
 RT: 7.696 min Scan# 1084  
 Delta R.T. 0.006 min  
 Lab File: VX045526.D  
 Acq: 01 Apr 2025 17:29

Tgt Ion: 41 Resp: 6908  
 Ion Ratio Lower Upper  
 41 100  
 69 74.6 58.2 87.2  
 39 68.3 53.6 80.4

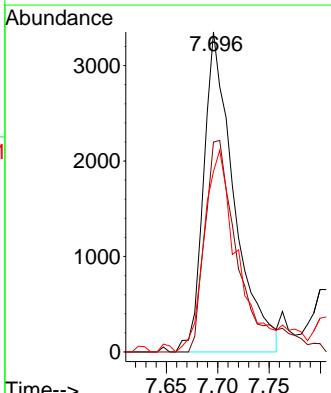

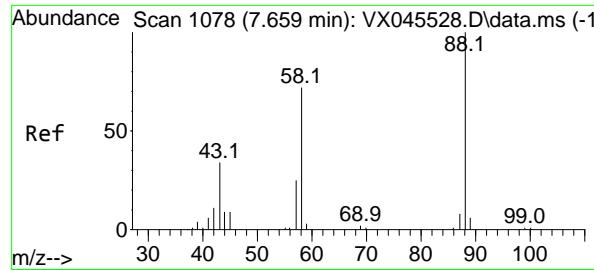

#49

1,4-Dioxane

Concen: 112.864 ug/l

RT: 7.665 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC005

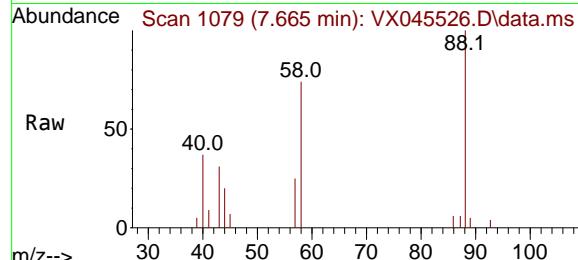

Tgt Ion: 88 Resp: 3205

Ion Ratio Lower Upper

88 100







43 32.4 32.2 48.4



58 72.7 58.6 88.0

**Manual Integrations****APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025
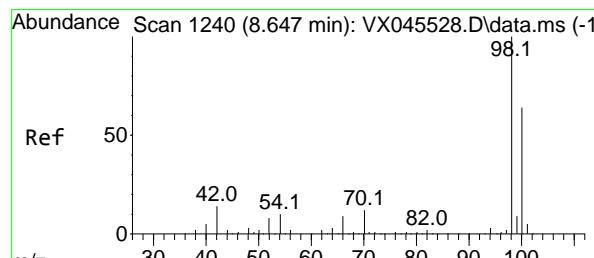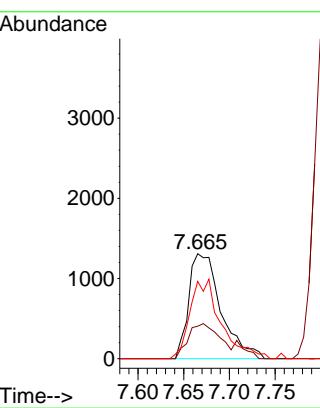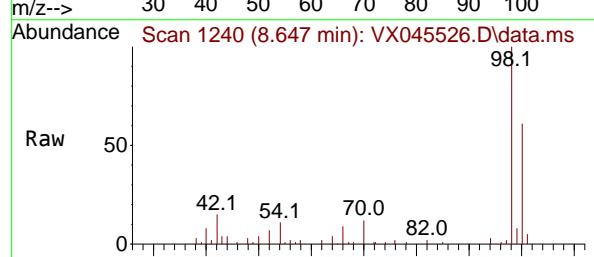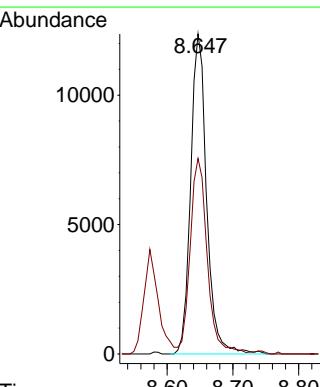
#50  
Toluene-d8  
Concen: 5.077 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29Tgt Ion: 98 Resp: 20890  
Ion Ratio Lower Upper  
98 100  
100 63.5 52.2 78.4

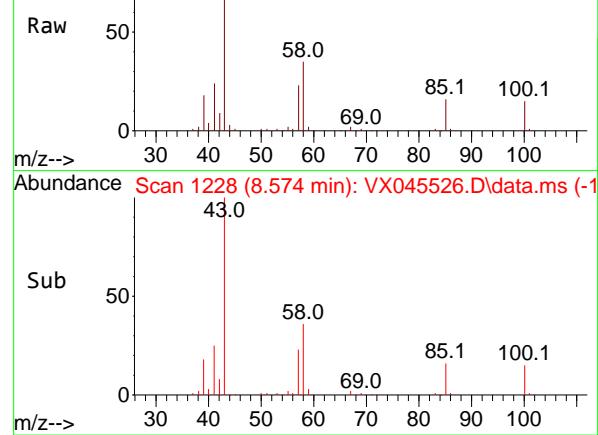

#51

4-Methyl-2-Pentanone

Concen: 23.844 ug/l

RT: 8.574 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#52

Toluene

Concen: 4.893 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29




Tgt Ion: 92 Resp: 14391

Ion Ratio Lower Upper

92 100

91 173.1 138.7 208.1

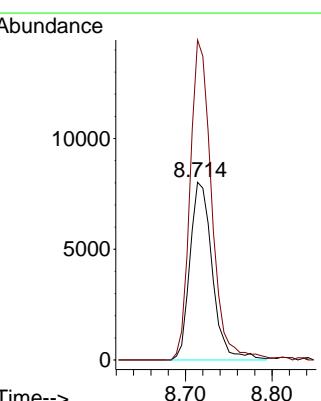







#53

t-1,3-Dichloropropene  
Concen: 5.834 ug/l  
RT: 8.982 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025






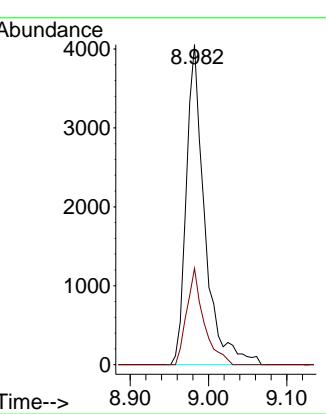


#54

cis-1,3-Dichloropropene  
Concen: 4.506 ug/l  
RT: 8.366 min Scan# 1194  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion: 75 Resp: 7873  
Ion Ratio Lower Upper  
75 100  
77 28.6 24.6 36.8  
39 64.4 48.4 72.6

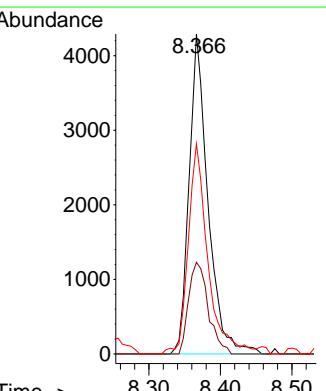




#55

1,1,2-Trichloroethane  
Concen: 4.898 ug/l  
RT: 9.153 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

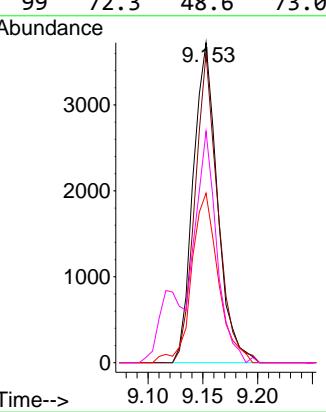

#56  
Ethyl methacrylate  
Concen: 4.417 ug/l  
RT: 9.116 min Scan# 1317  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion: 69 Resp: 8012  
Ion Ratio Lower Upper  
69 100  
41 75.8 61.3 91.9  
39 58.5 40.2 60.2

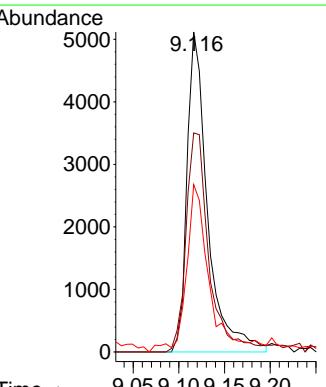



#57

1,3-Dichloropropane

Concen: 5.002 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#58

2-Chloroethyl Vinyl ether

Concen: 23.302 ug/l

RT: 8.244 min Scan# 1174

Delta R.T. 0.006 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29


Tgt Ion: 63 Resp: 21382

Ion Ratio Lower Upper


63	100
106	25.8

21.0 31.6


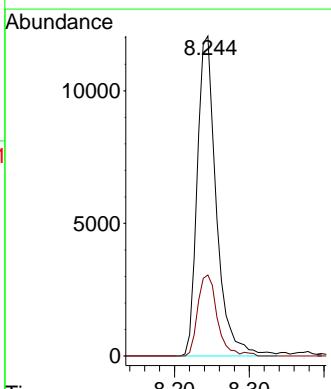





Abundance Scan 1369 (9.433 min): VX045526.D\data.ms

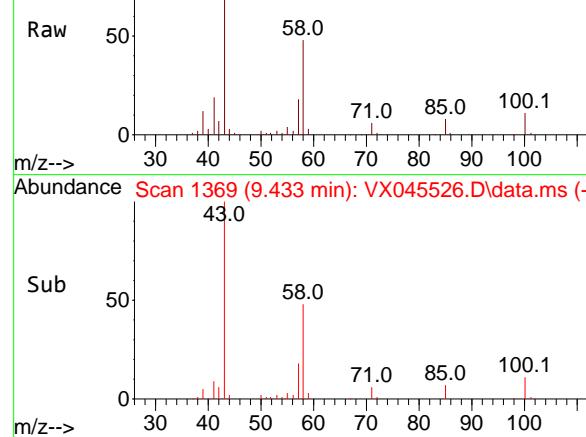


Abundance Scan 1369 (9.433 min): VX045526.D\data.ms (-1)

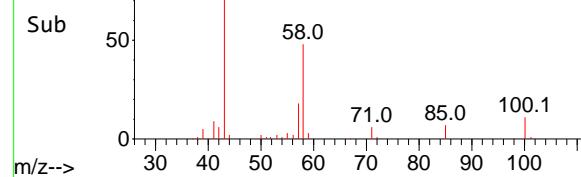

Abundance Scan 1383 (9.519 min): VX045526.D\data.ms

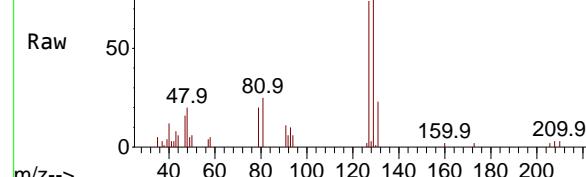

Abundance Scan 1383 (9.519 min): VX045526.D\data.ms (-1)

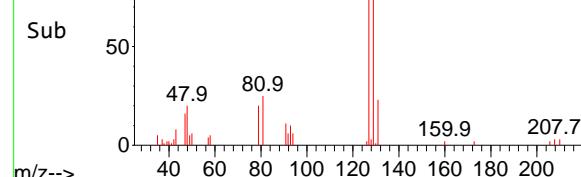

#59

2-Hexanone

Concen: 23.875 ug/l

RT: 9.433 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC005

Tgt Ion: 43 Resp: 3562

Ion Ratio Lower Upper

43 100


58 48.7 24.9 74.6

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

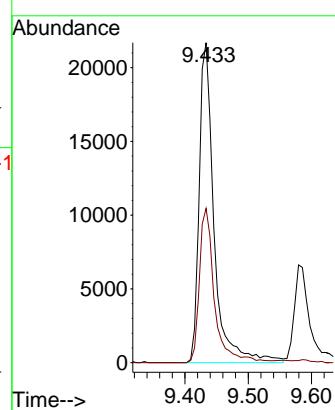

#60

Dibromochloromethane

Concen: 4.582 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29




Tgt Ion:129 Resp: 5855

Ion Ratio Lower Upper

129 100

127 77.5 39.4 118.2

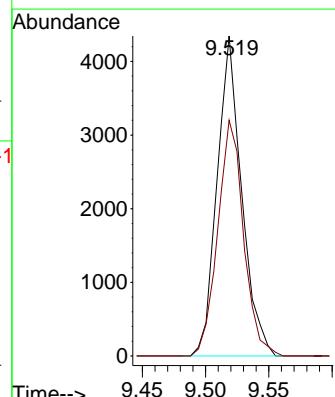

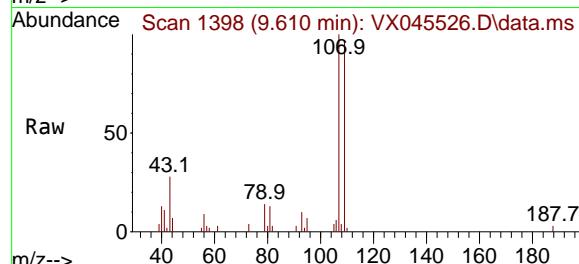

#61

1,2-Dibromoethane

Concen: 4.920 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#62

4-Bromofluorobenzene

Concen: 4.582 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29


Tgt Ion: 95 Resp: 6867


Ion Ratio Lower Upper

95 100

174 73.1 0.0 135.8

176 73.3 0.0 131.4

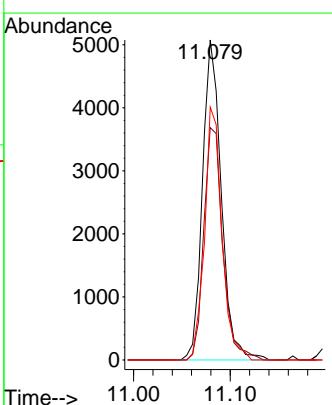


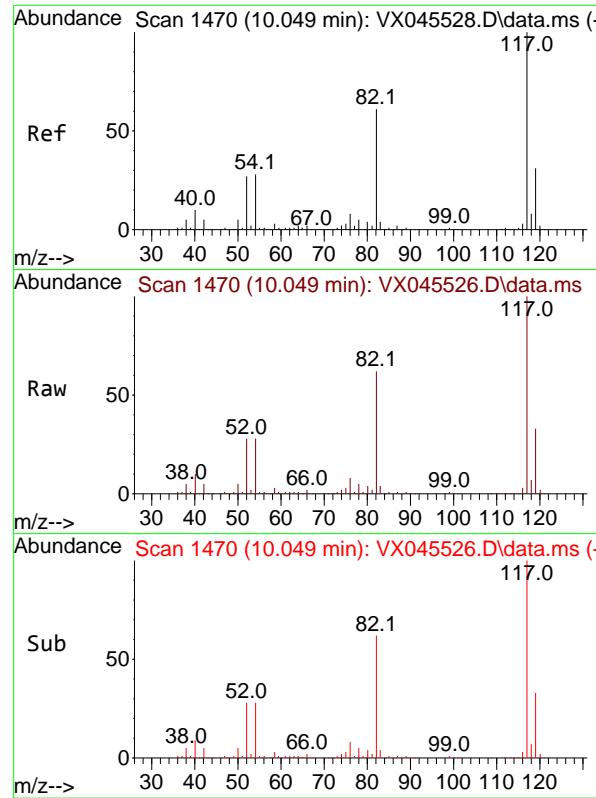


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 14393  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

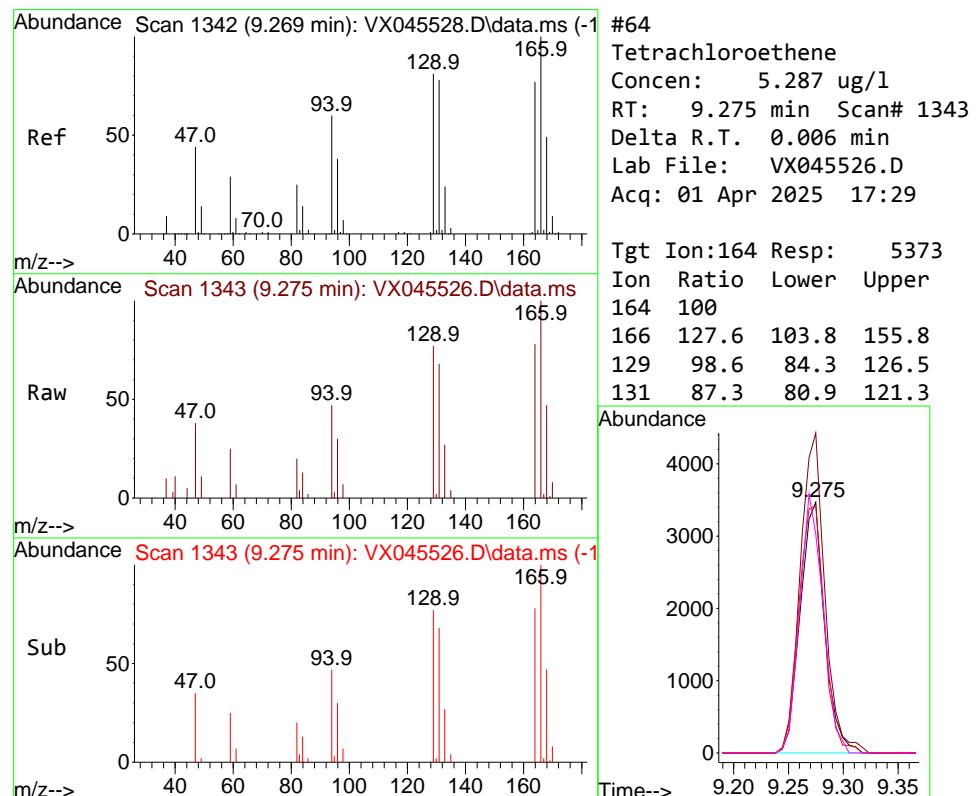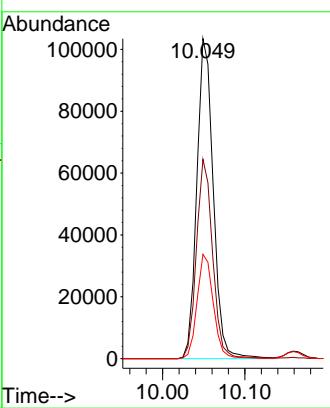

#64  
Tetrachloroethene  
Concen: 5.287 ug/l  
RT: 9.275 min Scan# 1343  
Delta R.T. 0.006 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion:164 Resp: 5373  
Ion Ratio Lower Upper  
164 100  
166 127.6 103.8 155.8  
129 98.6 84.3 126.5  
131 87.3 80.9 121.3

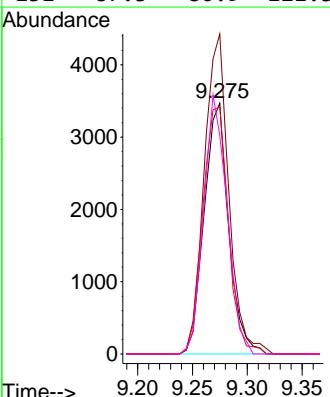



#65

Chlorobenzene

Concen: 4.935 ug/l

RT: 10.073 min Scan# 1474

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#66

1,1,1,2-Tetrachloroethane

Concen: 4.631 ug/l



RT: 10.159 min Scan# 1488


Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion:131 Resp: 4945  
 Ion Ratio Lower Upper  
 131 100  
 133 95.6 47.5 142.5  
 119 70.0 32.9 98.6

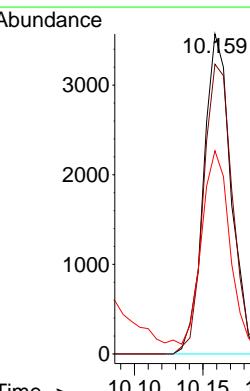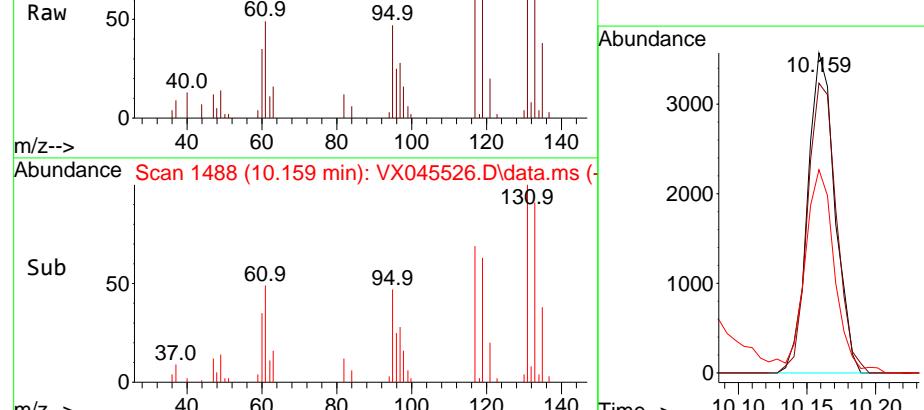

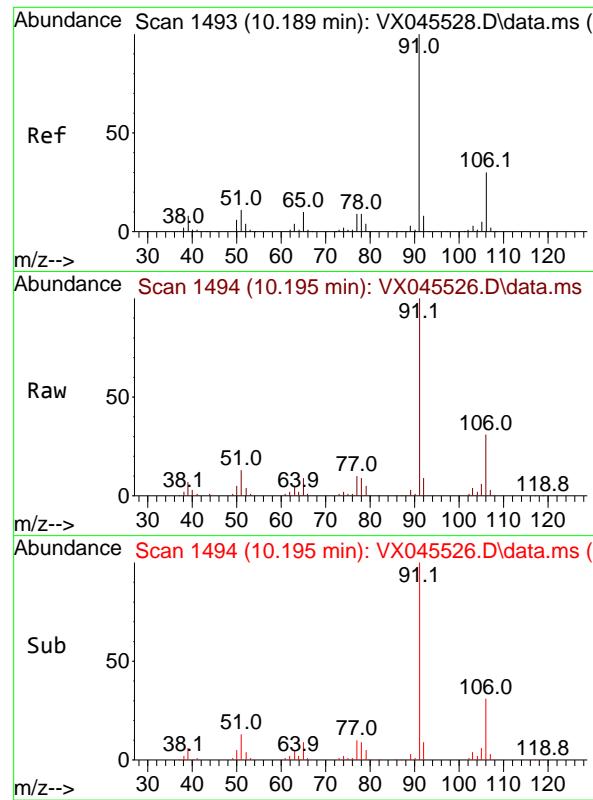

#67

Ethyl Benzene

Concen: 4.753 ug/l

RT: 10.195 min Scan# 1493

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

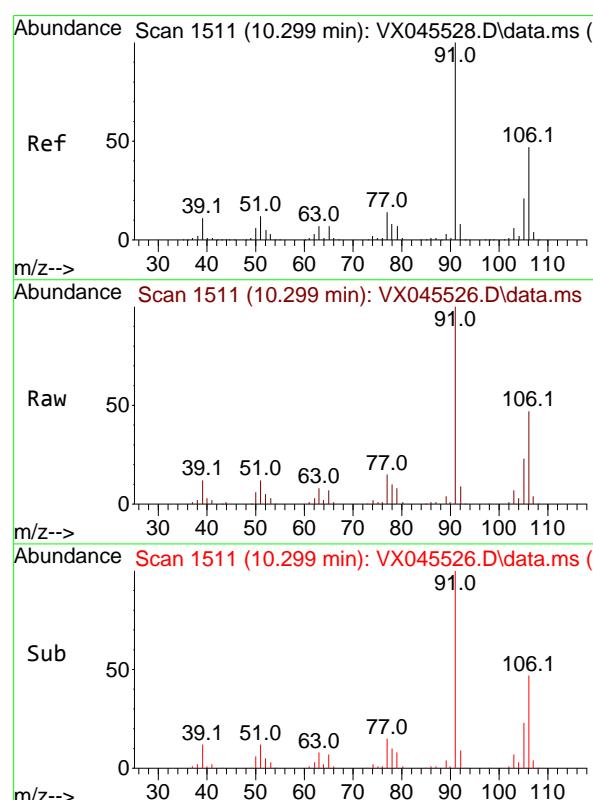

#68

m/p-Xylenes

Concen: 9.617 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29


Tgt Ion:106 Resp: 19268

Ion Ratio Lower Upper

106 100

91 213.6 172.6 258.8

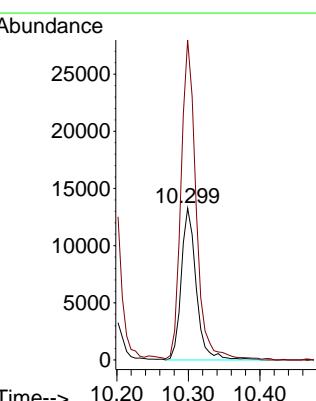


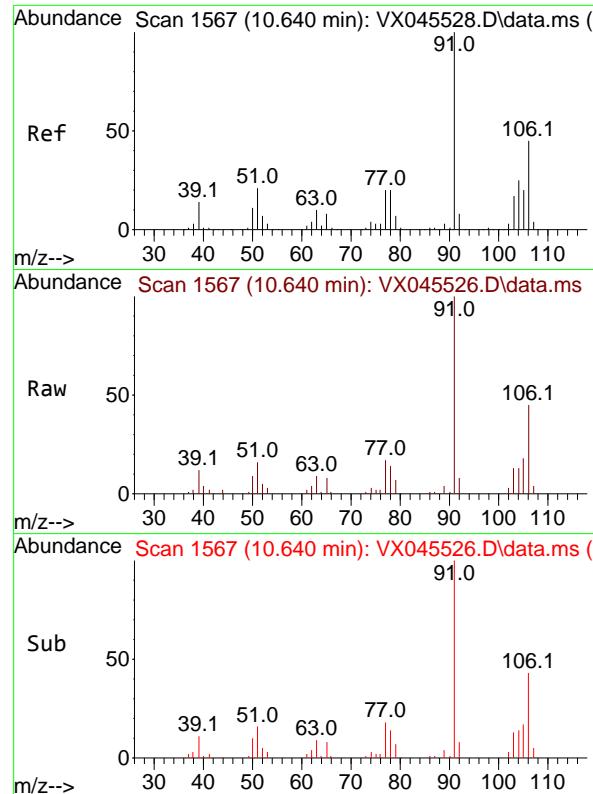


#69  
o-Xylene  
Concen: 4.932 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29  
ClientSampleId : VSTDICC005

Tgt Ion:106 Resp: 9739  
Ion Ratio Lower Upper  
106 100  
91 225.8 113.6 340.6


### Manual Integrations APPROVED







Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

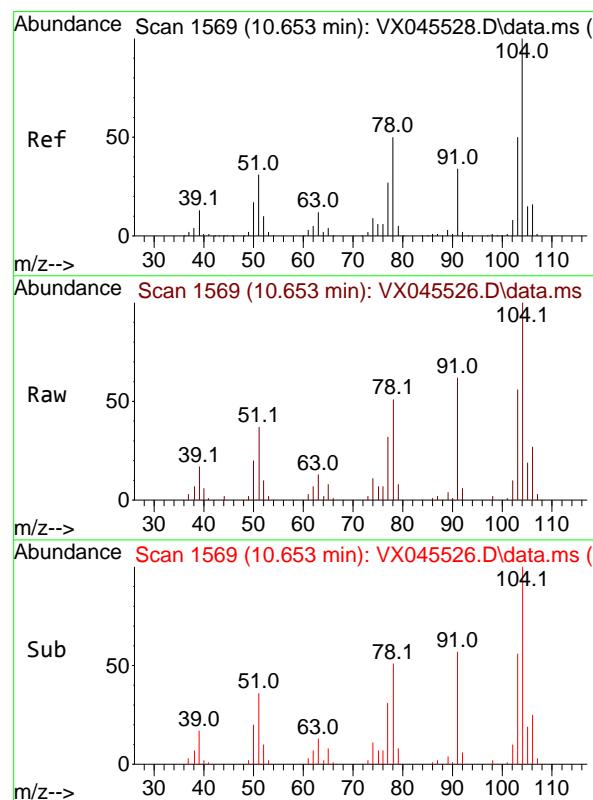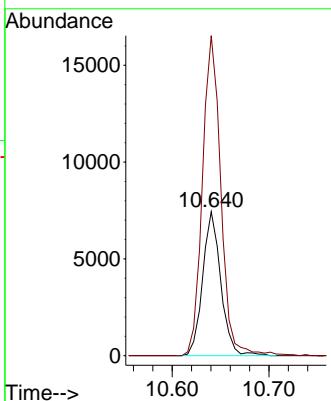


#70  
Styrene  
Concen: 4.610 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion:104 Resp: 15017  
Ion Ratio Lower Upper  
104 100  
78 59.8 45.4 68.2  
103 57.1 43.8 65.8

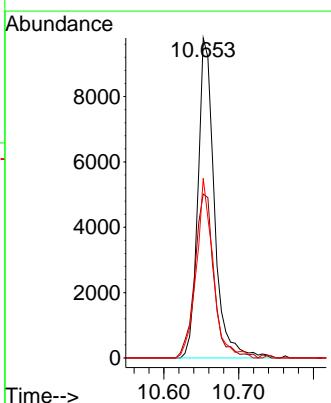





#71

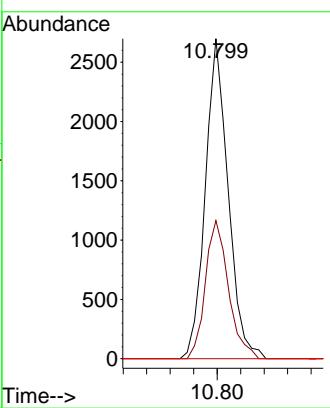Bromoform  
Concen: 4.558 ug/lRT: 10.799 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29Instrument :  
MSVOA\_X  
ClientSampleId :  
VSTDICC005**Manual Integrations  
APPROVED**Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

#72

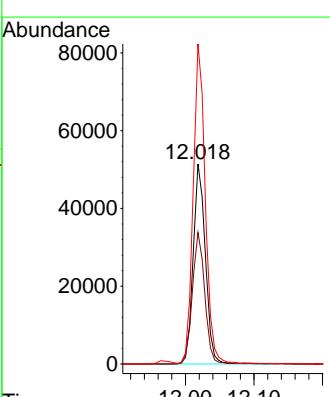1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29Tgt Ion:152 Resp: 63909  
Ion Ratio Lower Upper  
152 100  
115 66.5 46.9 140.7  
150 157.5 0.0 349.4

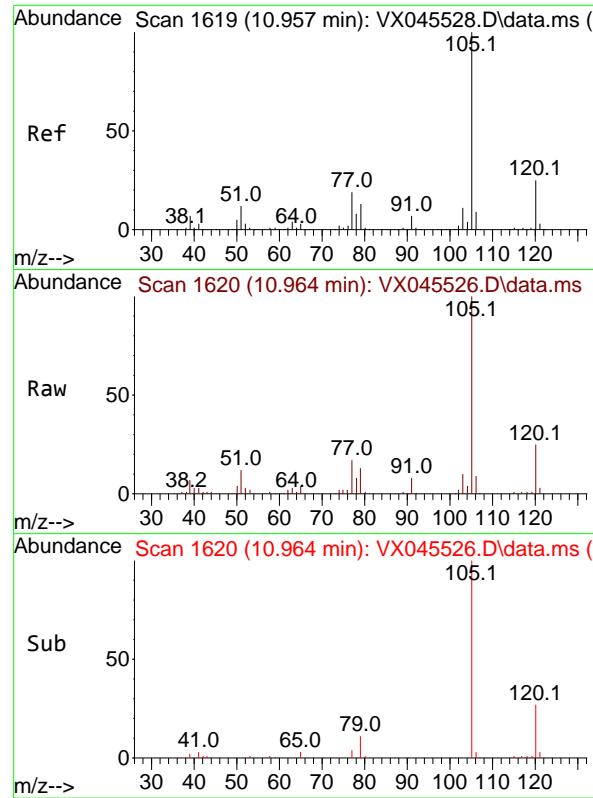

#73

Isopropylbenzene

Concen: 4.806 ug/l

RT: 10.964 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

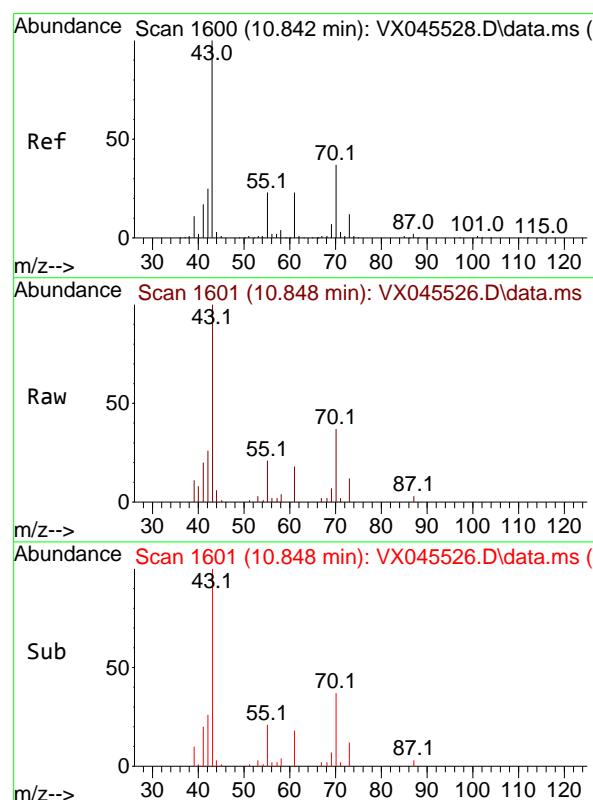

#74

N-amyl acetate

Concen: 4.390 ug/l

RT: 10.848 min Scan# 1601

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion: 43 Resp: 10750


Ion Ratio Lower Upper


43 100

70 37.8 30.1 45.1

55 23.0 18.3 27.5

61 20.1 17.5 26.3

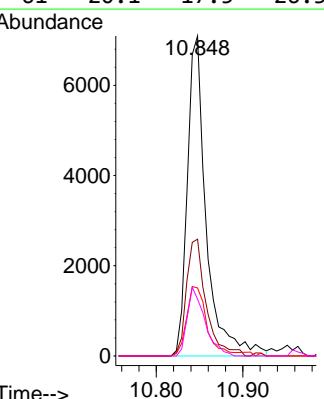


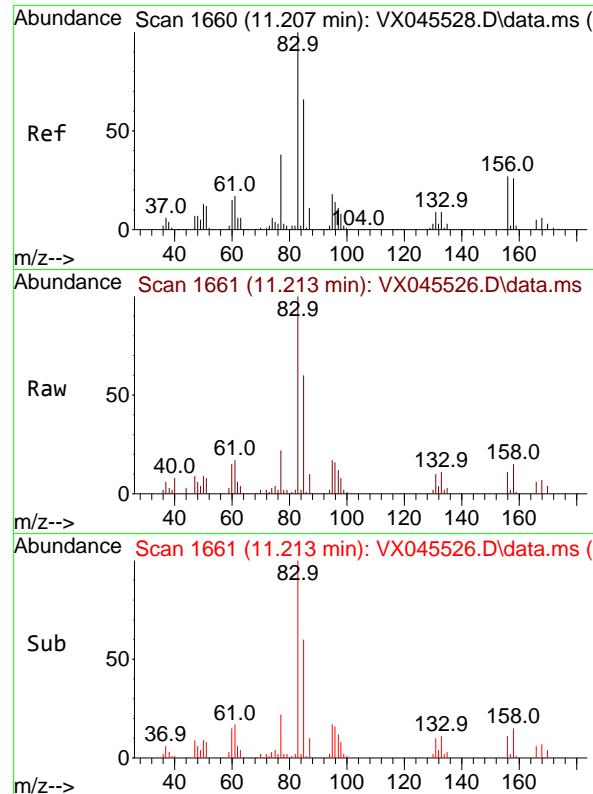


#75  
1,1,2,2-Tetrachloroethane  
Concen: 5.075 ug/l  
RT: 11.213 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

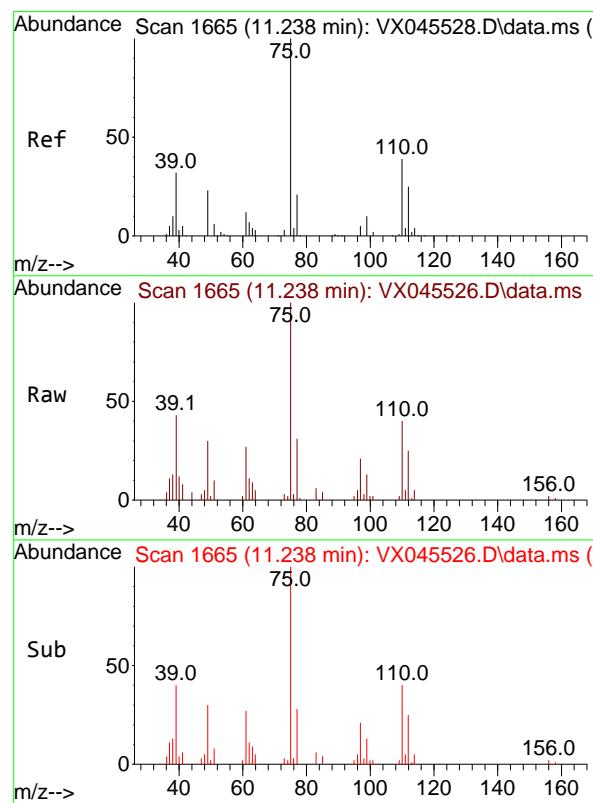

#76  
1,2,3-Trichloropropane  
Concen: 5.152 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion: 75 Resp: 8032  
Ion Ratio Lower Upper  
75 100  
77 40.2 20.0 59.9





#77

Bromobenzene

Concen: 5.011 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

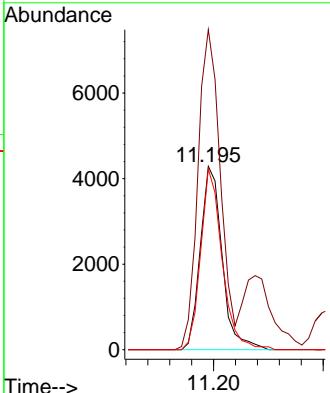

#78

n-propylbenzene

Concen: 4.711 ug/l


RT: 11.305 min Scan# 1676


Delta R.T. 0.006 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29

Tgt	Ion	91	Resp:	27777
Ion	Ratio	Lower	Upper	
	100			
91	100			
120	20.6	10.8	32.3	

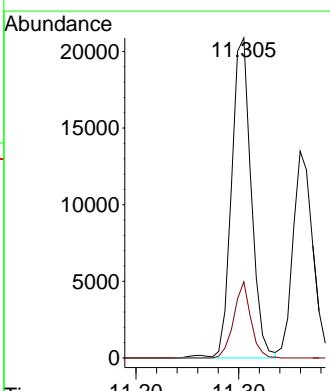




Abundance Scan 1685 (11.360 min): VX045526.D\data.ms (-)

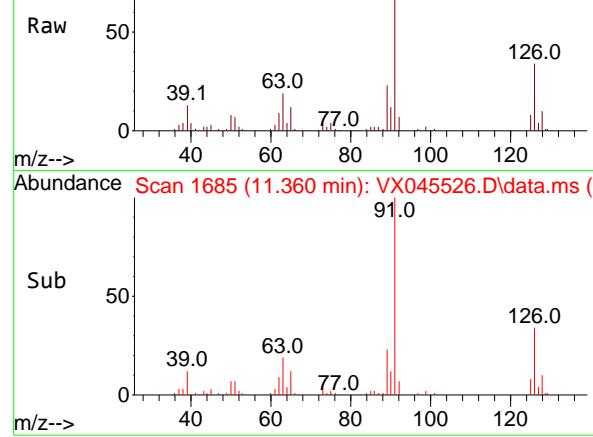

Abundance Scan 1685 (11.360 min): VX045526.D\data.ms (-)

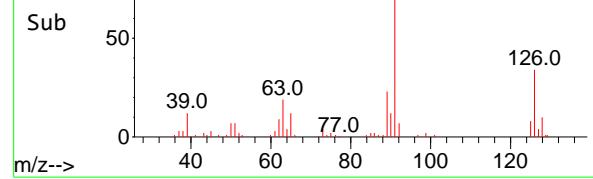

#79

2-Chlorotoluene

Concen: 4.870 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005


**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025


Supervised By :Mahesh Dadoda 04/02/2025

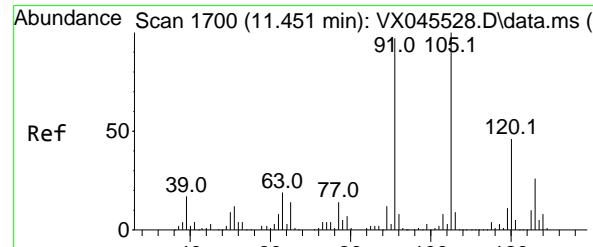

Abundance Scan 1700 (11.451 min): VX045526.D\data.ms (-)

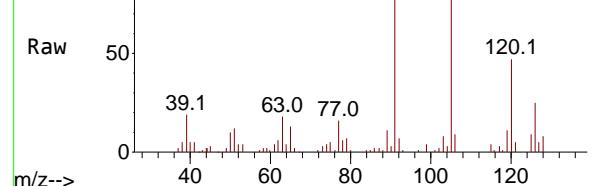

Abundance Scan 1700 (11.451 min): VX045526.D\data.ms (-)

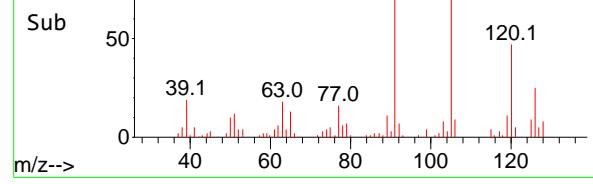

#80

1,3,5-Trimethylbenzene

Concen: 4.710 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt Ion:105 Resp: 19936

Ion Ratio Lower Upper


105 100

120 47.1 23.0 69.0

Abundance Scan 1700 (11.451 min): VX045526.D\data.ms (-)

Abundance Scan 1700 (11.451 min): VX045526.D\data.ms (-)

Abundance Scan 1700 (11.451 min): VX045526.D\data.ms (-)

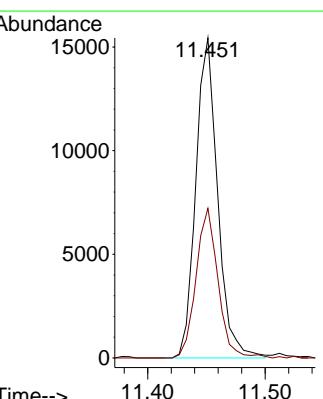


#13

#14

#15

#16


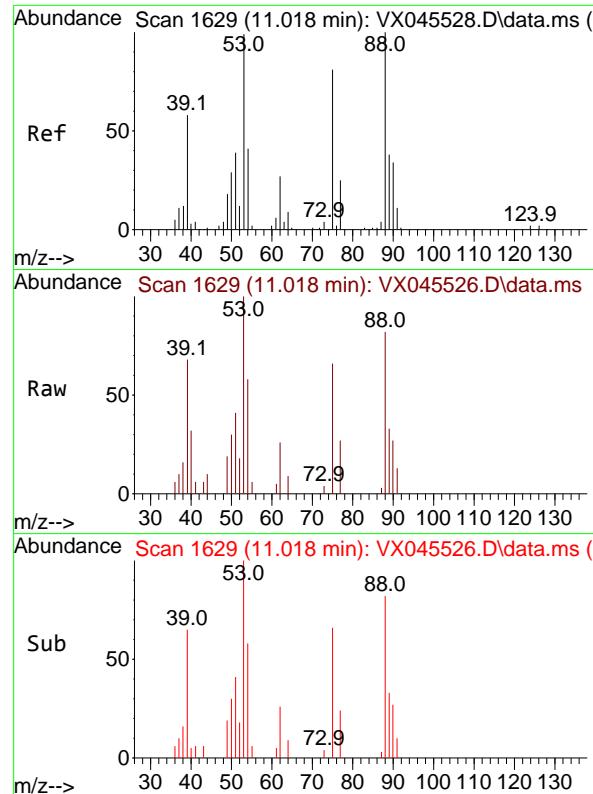


#81  
trans-1,4-Dichloro-2-butene  
Concen: 3.814 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

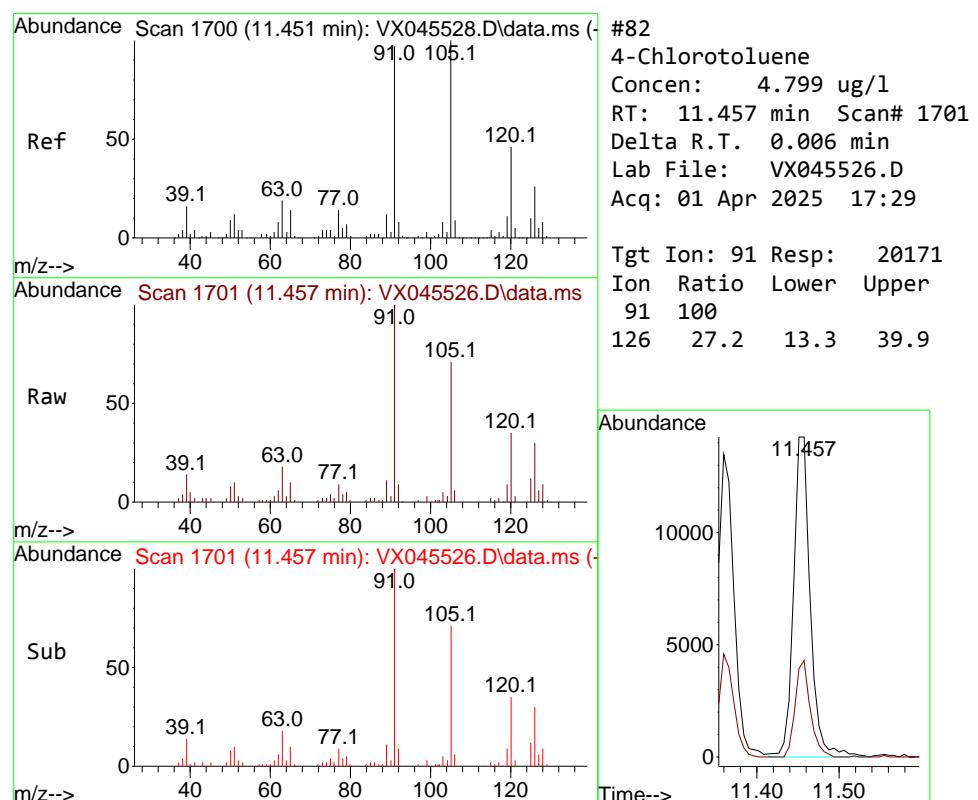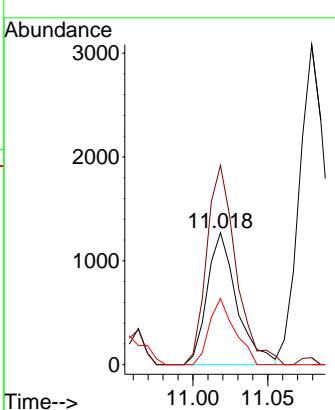

#82  
4-Chlorotoluene  
Concen: 4.799 ug/l  
RT: 11.457 min Scan# 1701  
Delta R.T. 0.006 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion: 91 Resp: 20171  
Ion Ratio Lower Upper  
91 100  
126 27.2 13.3 39.9

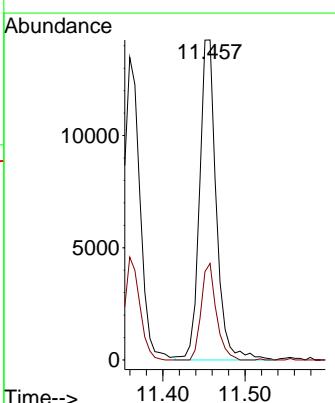



#83

tert-Butylbenzene

Concen: 4.763 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

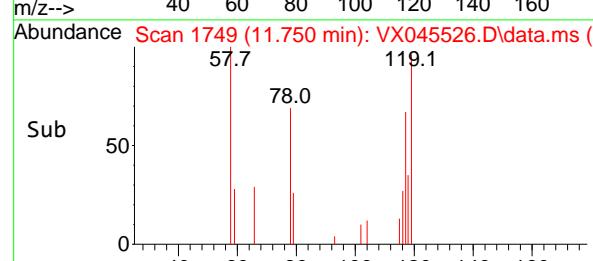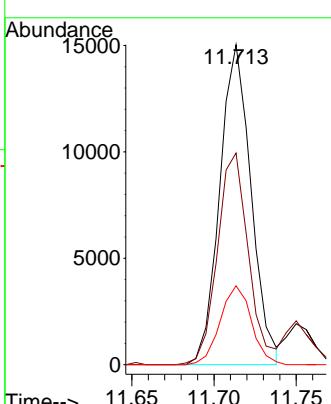

#84

1,2,4-Trimethylbenzene

Concen: 4.707 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045526.D


Acq: 01 Apr 2025 17:29



Tgt Ion:105 Resp: 19998

Ion Ratio Lower Upper

105 100

120 43.5 21.4 64.3

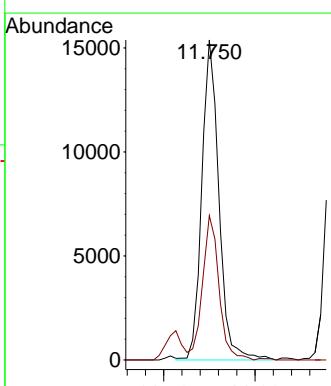



#85

sec-Butylbenzene

Concen: 4.753 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

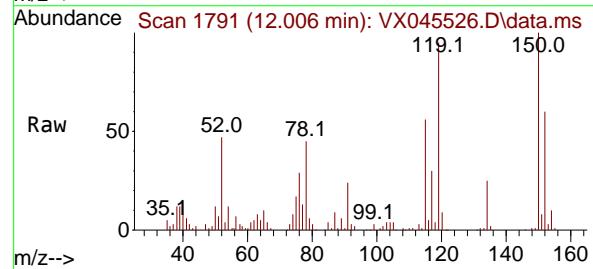

#86

p-Isopropyltoluene

Concen: 4.755 ug/l


RT: 12.006 min Scan# 1791


Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt	Ion:119	Resp:	20178
Ion	Ratio	Lower	Upper
119	100		
134	25.1	12.6	37.8
91	26.4	13.7	41.1



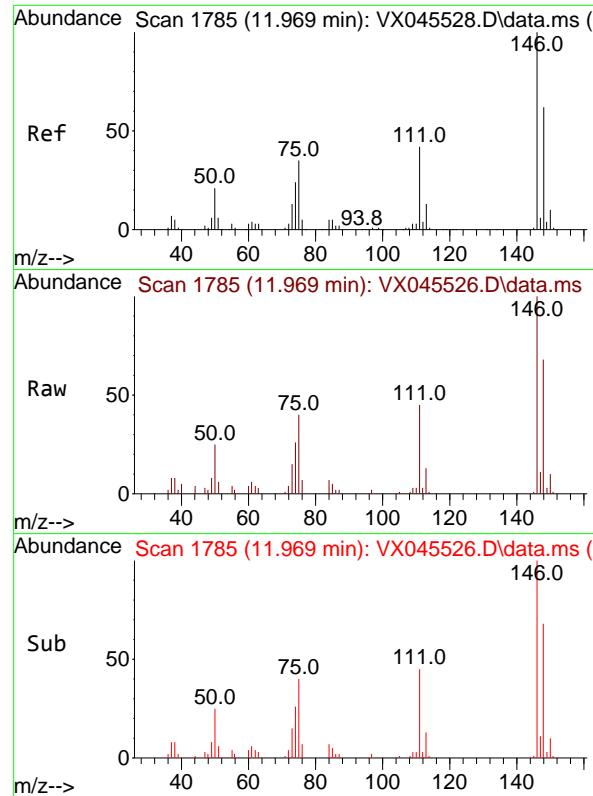

#87

1,3-Dichlorobenzene

Concen: 4.763 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

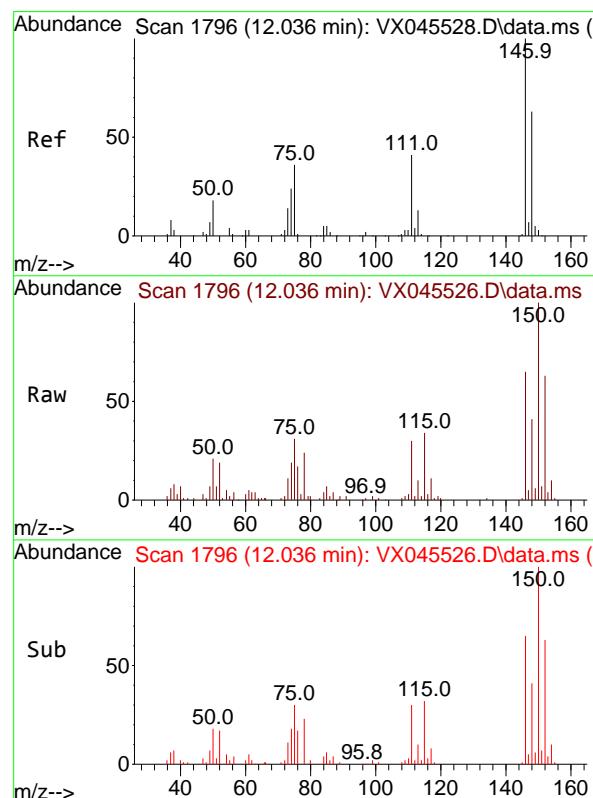

#88

1,4-Dichlorobenzene

Concen: 5.047 ug/l


RT: 12.036 min Scan# 1796

Delta R.T. 0.000 min







Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Tgt	Ion:146	Resp:	11016
Ion	Ratio	Lower	Upper
146	100		
111	51.4	20.9	62.8
148	64.2	31.5	94.5

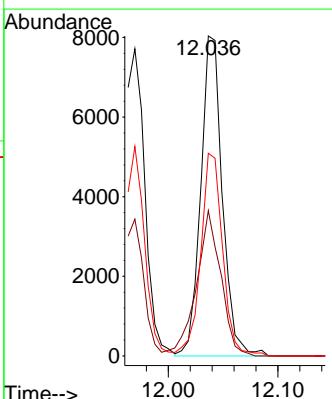





#91

1,2-Dichlorobenzene

Concen: 4.910 ug/l

RT: 12.335 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#92

1,2-Dibromo-3-Chloropropane

Concen: 4.417 ug/l

RT: 12.945 min Scan# 1945

Delta R.T. 0.006 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29


Tgt Ion: 75 Resp: 1661


Ion Ratio Lower Upper

75 100

155 67.3 34.9 104.7

157 100.4 44.9 134.7




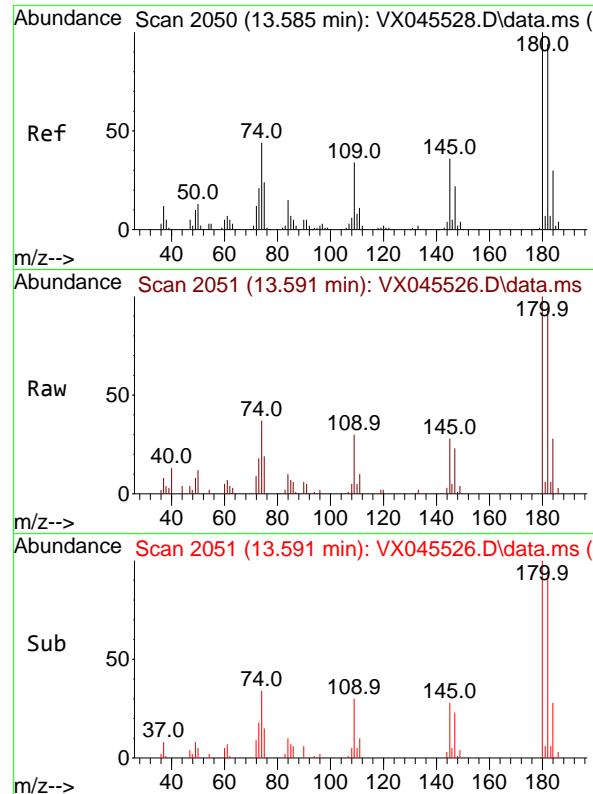


#93  
1,2,4-Trichlorobenzene  
Concen: 4.524 ug/l  
RT: 13.591 min Scan# 2051  
Delta R.T. 0.006 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

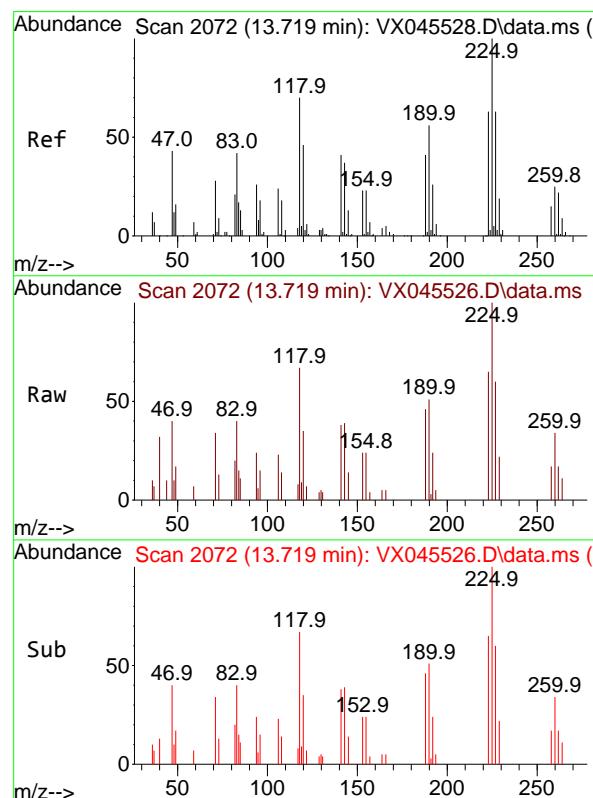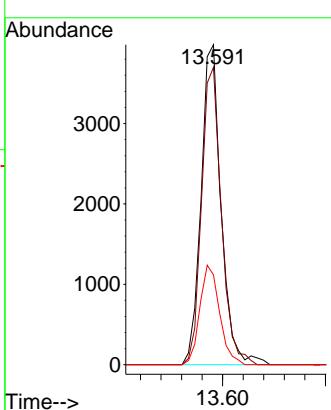

#94  
Hexachlorobutadiene  
Concen: 4.836 ug/l  
RT: 13.719 min Scan# 2072  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion:225 Resp: 2483  
Ion Ratio Lower Upper  
225 100  
223 64.4 31.1 93.3  
227 62.8 32.2 96.6

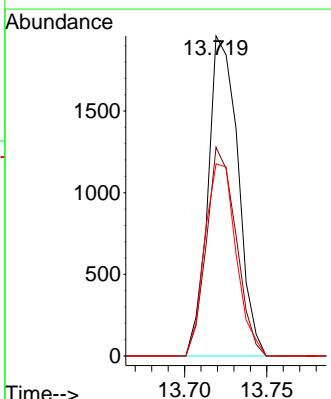

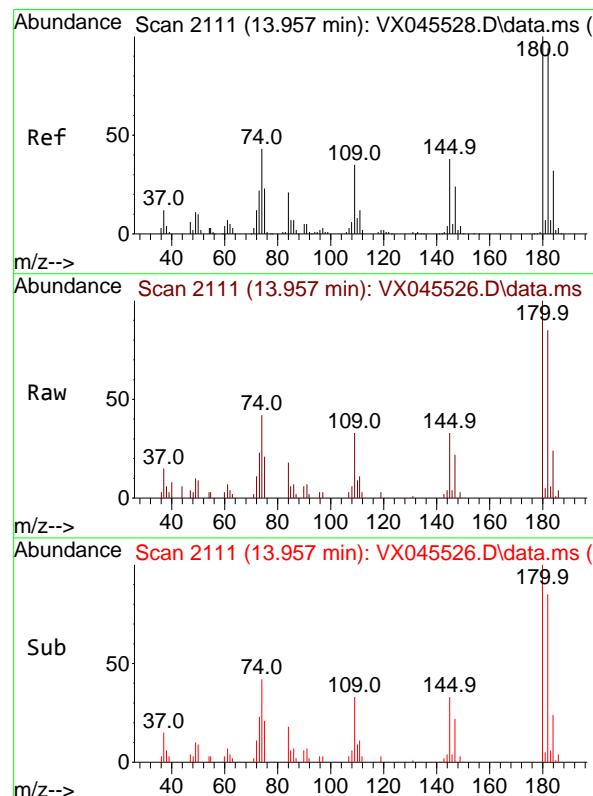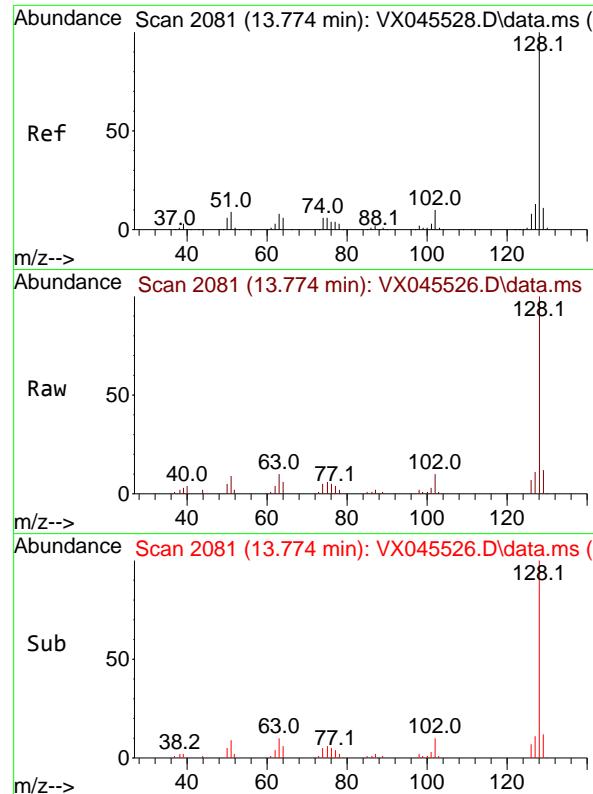

#95

Naphthalene

Concen: 4.424 ug/l

RT: 13.774 min Scan# 2

Delta R.T. 0.000 min

Lab File: VX045526.D

Acq: 01 Apr 2025 17:29

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**


Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#96  
1,2,3-Trichlorobenzene  
Concen: 4.692 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045526.D  
Acq: 01 Apr 2025 17:29

Tgt Ion:180 Resp: 5854  
Ion Ratio Lower Upper  
180 100  
182 90.7 47.3 141.8  
145 35.2 18.2 54.6

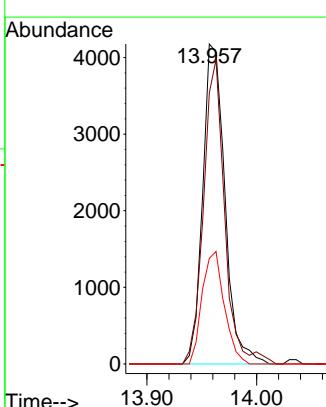

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045527.D  
 Acq On : 01 Apr 2025 17:52  
 Operator : JC/MD  
 Sample : VSTDICC020  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDICC020**

Quant Time: Apr 02 02:52:02 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	90228	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	160754	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	144087	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	65341	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	32500	19.697	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 39.400%#			
35) Dibromofluoromethane	5.385	113	21963	19.256	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 38.520%#			
50) Toluene-d8	8.647	98	79303	19.921	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 39.840%#			
62) 4-Bromofluorobenzene	11.079	95	28795	19.858	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 39.720%#			
<b>Target Compounds</b>						
				<b>Qvalue</b>		
2) Dichlorodifluoromethane	1.166	85	25265	18.724	ug/l	97
3) Chloromethane	1.301	50	28034	20.223	ug/l	98
4) Vinyl Chloride	1.374	62	25285	19.931	ug/l	97
5) Bromomethane	1.593	94	11815	19.642	ug/l	99
6) Chloroethane	1.666	64	14071	20.905	ug/l	98
7) Trichlorofluoromethane	1.874	101	38815	20.518	ug/l	98
8) Diethyl Ether	2.136	74	12852	20.235	ug/l	99
9) 1,1,2-Trichlorotrifluo...	2.319	101	22917	20.673	ug/l	95
10) Methyl Iodide	2.441	142	28478	20.596	ug/l	99
11) Tert butyl alcohol	2.983	59	22453	101.253	ug/l	100
12) 1,1-Dichloroethene	2.306	96	22103	20.406	ug/l	96
13) Acrolein	2.239	56	28991	94.938	ug/l	99
14) Allyl chloride	2.660	41	41233	20.063	ug/l	99
15) Acrylonitrile	3.062	53	74487	106.412	ug/l	98
16) Acetone	2.386	43	69788	103.000	ug/l	99
17) Carbon Disulfide	2.502	76	51771	19.352	ug/l	98
18) Methyl Acetate	2.703	43	31190	19.994	ug/l	99
19) Methyl tert-butyl Ether	3.117	73	78284	20.660	ug/l	96
20) Methylene Chloride	2.782	84	26212	20.664	ug/l	96
21) trans-1,2-Dichloroethene	3.087	96	22968	20.755	ug/l	92
22) Diisopropyl ether	3.757	45	84046	20.760	ug/l #	81
23) Vinyl Acetate	3.721	43	361881	103.458	ug/l	99
24) 1,1-Dichloroethane	3.605	63	47560	20.772	ug/l	99
25) 2-Butanone	4.556	43	105062	105.931	ug/l	99
26) 2,2-Dichloropropane	4.471	77	28956	19.574	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	27425	20.342	ug/l	98
28) Bromochloromethane	4.897	49	22285	20.141	ug/l	100
29) Tetrahydrofuran	5.007	42	66994	104.187	ug/l	99
30) Chloroform	5.093	83	48639	20.646	ug/l	100
31) Cyclohexane	5.458	56	41450	20.478	ug/l	99
32) 1,1,1-Trichloroethane	5.373	97	40407	20.270	ug/l	99
36) 1,1-Dichloropropene	5.684	75	30504	19.808	ug/l	98
37) Ethyl Acetate	4.715	43	39163	20.180	ug/l	98
38) Carbon Tetrachloride	5.672	117	33533	20.148	ug/l	94
39) Methylcyclohexane	7.373	83	38303	20.291	ug/l	97
40) Benzene	6.031	78	97667	20.766	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045527.D  
 Acq On : 01 Apr 2025 17:52  
 Operator : JC/MD  
 Sample : VSTDICC020  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC020

Quant Time: Apr 02 02:52:02 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	21740	21.046	ug/l	97
42) 1,2-Dichloroethane	6.086	62	41733	21.484	ug/l	100
43) Isopropyl Acetate	6.342	43	61222	20.814	ug/l	99
44) Trichloroethene	7.123	130	22918	20.501	ug/l	97
45) 1,2-Dichloropropane	7.428	63	24926	21.241	ug/l	90
46) Dibromomethane	7.580	93	19104	21.207	ug/l	99
47) Bromodichloromethane	7.818	83	37036	20.587	ug/l	99
48) Methyl methacrylate	7.696	41	31247	20.575	ug/l	99
49) 1,4-Dioxane	7.659	88	12104	440.515	ug/l	96
51) 4-Methyl-2-Pentanone	8.574	43	212645	109.055	ug/l	99
52) Toluene	8.714	92	60357	21.208	ug/l	99
53) t-1,3-Dichloropropene	8.976	75	29870	18.764	ug/l	96
54) cis-1,3-Dichloropropene	8.366	75	35099	20.762	ug/l	95
55) 1,1,2-Trichloroethane	9.147	97	24191	21.331	ug/l	96
56) Ethyl methacrylate	9.116	69	36155	20.600	ug/l	99
57) 1,3-Dichloropropane	9.305	76	41900	21.217	ug/l	100
58) 2-Chloroethyl Vinyl ether	8.238	63	91923	103.534	ug/l	100
59) 2-Hexanone	9.427	43	156999	108.730	ug/l	99
60) Dibromochloromethane	9.519	129	25992	21.023	ug/l	98
61) 1,2-Dibromoethane	9.604	107	24456	21.303	ug/l	99
64) Tetrachloroethene	9.269	164	21379	21.015	ug/l	98
65) Chlorobenzene	10.079	112	64727	21.023	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	21447	20.064	ug/l	98
67) Ethyl Benzene	10.189	91	115368	20.921	ug/l	99
68) m/p-Xylenes	10.299	106	84420	42.092	ug/l	99
69) o-Xylene	10.640	106	41803	21.158	ug/l	100
70) Styrene	10.653	104	69290	21.249	ug/l	99
71) Bromoform	10.799	173	15659	19.619	ug/l #	99
73) Isopropylbenzene	10.957	105	110396	21.093	ug/l	100
74) N-amyl acetate	10.842	43	51238	20.466	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	38177	20.764	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	32690m	20.510	ug/l	
77) Bromobenzene	11.195	156	24902	20.592	ug/l	100
78) n-propylbenzene	11.299	91	130994	21.729	ug/l	98
79) 2-Chlorotoluene	11.360	91	81817	21.229	ug/l	99
80) 1,3,5-Trimethylbenzene	11.451	105	93328	21.564	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	8435	17.961	ug/l	88
82) 4-Chlorotoluene	11.451	91	90704	21.108	ug/l	99
83) tert-Butylbenzene	11.713	119	89828	20.964	ug/l	98
84) 1,2,4-Trimethylbenzene	11.750	105	92242	21.235	ug/l	100
85) sec-Butylbenzene	11.890	105	112800	21.433	ug/l	100
86) p-Isopropyltoluene	12.006	119	91866	21.173	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	45105	20.490	ug/l	100
88) 1,4-Dichlorobenzene	12.036	146	46208	20.706	ug/l	99
89) n-Butylbenzene	12.329	91	77739	20.662	ug/l	100
90) Hexachloroethane	12.536	117	14544	19.505	ug/l	100
91) 1,2-Dichlorobenzene	12.335	146	45732	20.896	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	8153	21.203	ug/l	100
93) 1,2,4-Trichlorobenzene	13.585	180	24787	20.347	ug/l	98
94) Hexachlorobutadiene	13.725	225	10488	19.979	ug/l	97
95) Naphthalene	13.774	128	94875	20.928	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	26113	20.471	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045527.D  
 Acq On : 01 Apr 2025 17:52  
 Operator : JC/MD  
 Sample : VSTDICC020  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC020

Quant Time: Apr 02 02:52:02 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
Data File : VX045527.D  
Acq On : 01 Apr 2025 17:52  
Operator : JC/MD  
Sample : VSTDICC020  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC020

## Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

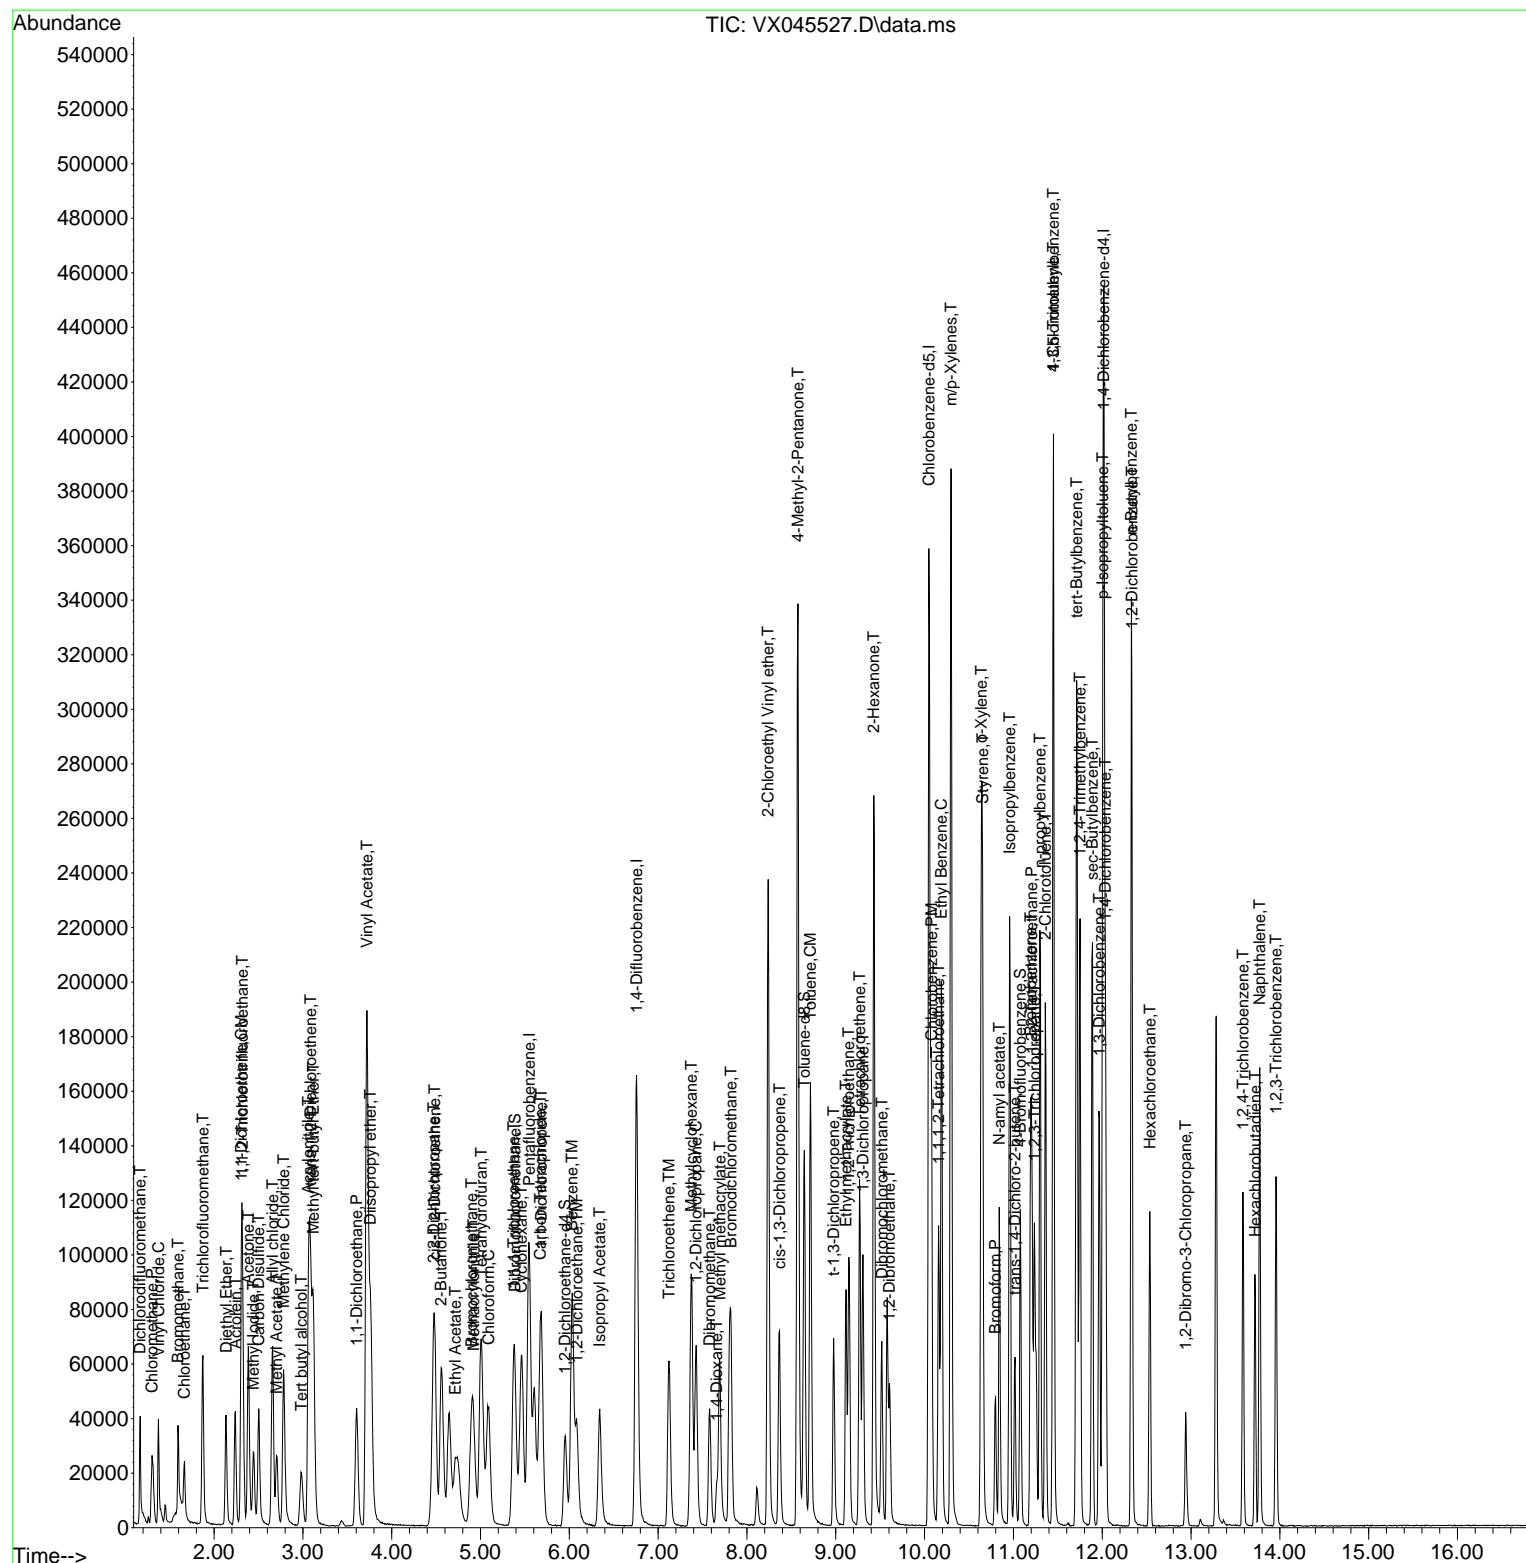



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#2

Dichlorodifluoromethane

Concen: 18.724 ug/l



RT: 1.166 min Scan# 13

Delta R.T. 0.000 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52


Tgt Ion: 85 Resp: 25265  
 Ion Ratio Lower Upper  
 85 100  
 87 33.7 16.1 48.2

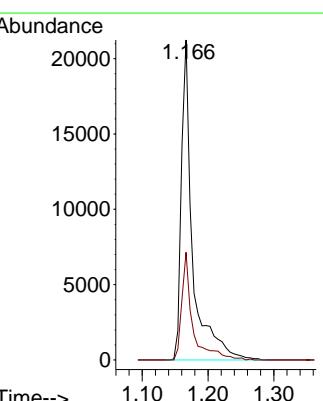



#3

Scan 13 (1.166 min): VX045527.D\data.ms (-1)

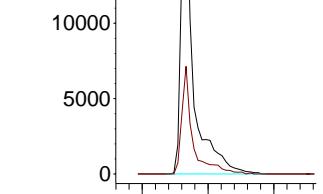


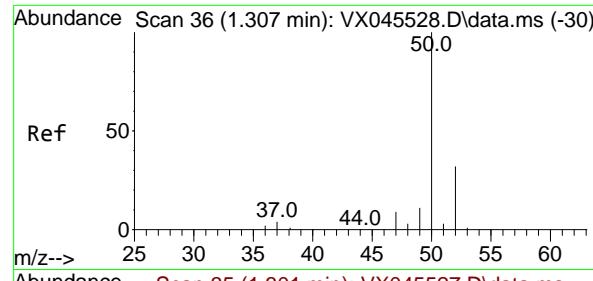

Abundance Scan 35 (1.301 min): VX045527.D\data.ms

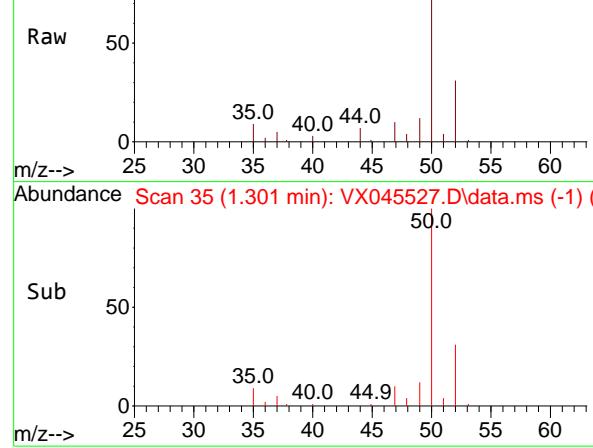

Abundance Scan 47 (1.374 min): VX045527.D\data.ms

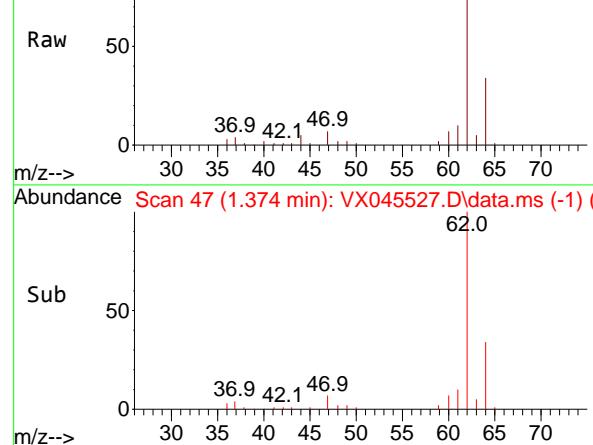

Abundance Scan 47 (1.374 min): VX045527.D\data.ms (-1)

#3

Chloromethane

Concen: 20.223 ug/l

RT: 1.301 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#4

Vinyl Chloride

Concen: 19.931 ug/l

RT: 1.374 min Scan# 47


Delta R.T. 0.000 min


Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 62 Resp: 25285

Ion	Ratio	Lower	Upper
62	100		
64	33.5	25.5	38.3



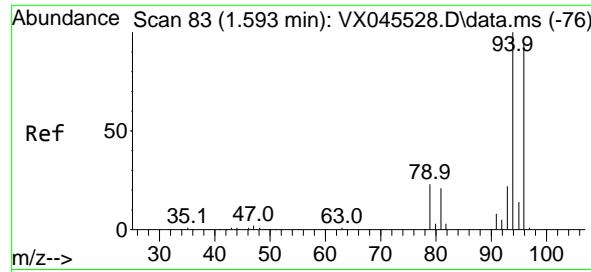




#5  
Bromomethane  
Concen: 19.642 ug/l  
RT: 1.593 min Scan# 8  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52  
ClientSampleId : VSTDICC020




Tgt Ion: 94 Resp: 1181  
Ion Ratio Lower Upper  
94 100  
96 92.7 74.8 112.2

### Manual Integrations APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

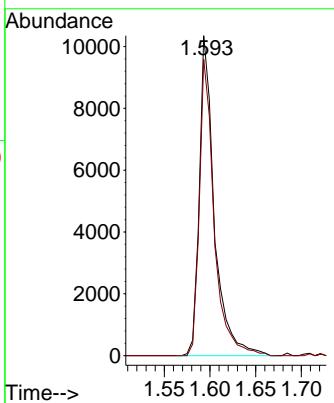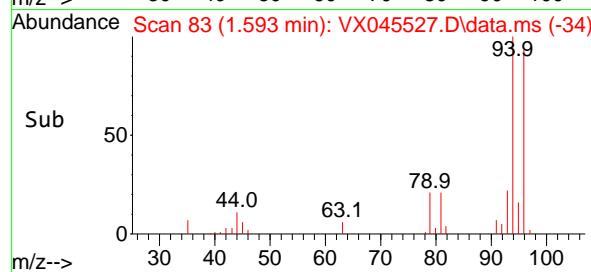


#6  
Chloroethane  
Concen: 20.905 ug/l  
RT: 1.666 min Scan# 95  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52



Tgt Ion: 64 Resp: 14071  
Ion Ratio Lower Upper  
64 100  
66 31.9 26.3 39.5

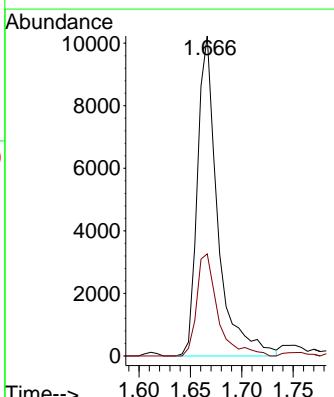


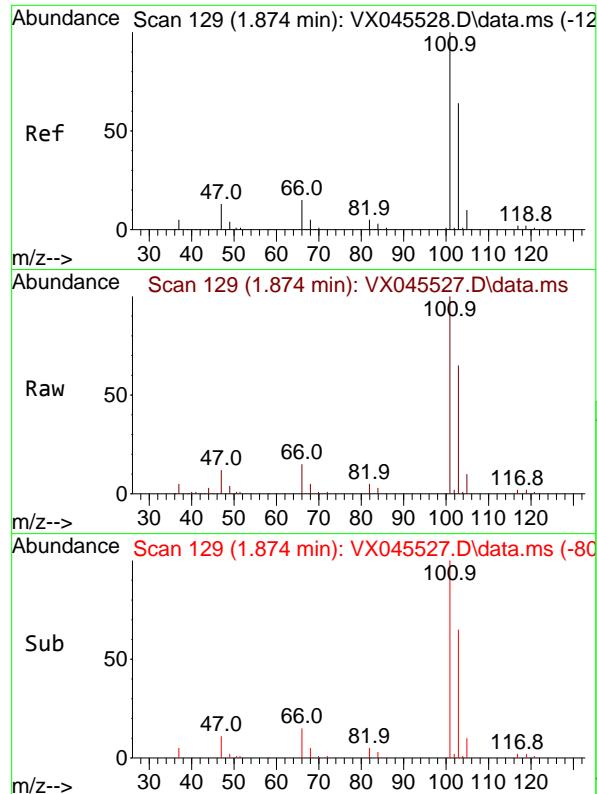


#7  
Trichlorofluoromethane  
Concen: 20.518 ug/l  
RT: 1.874 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

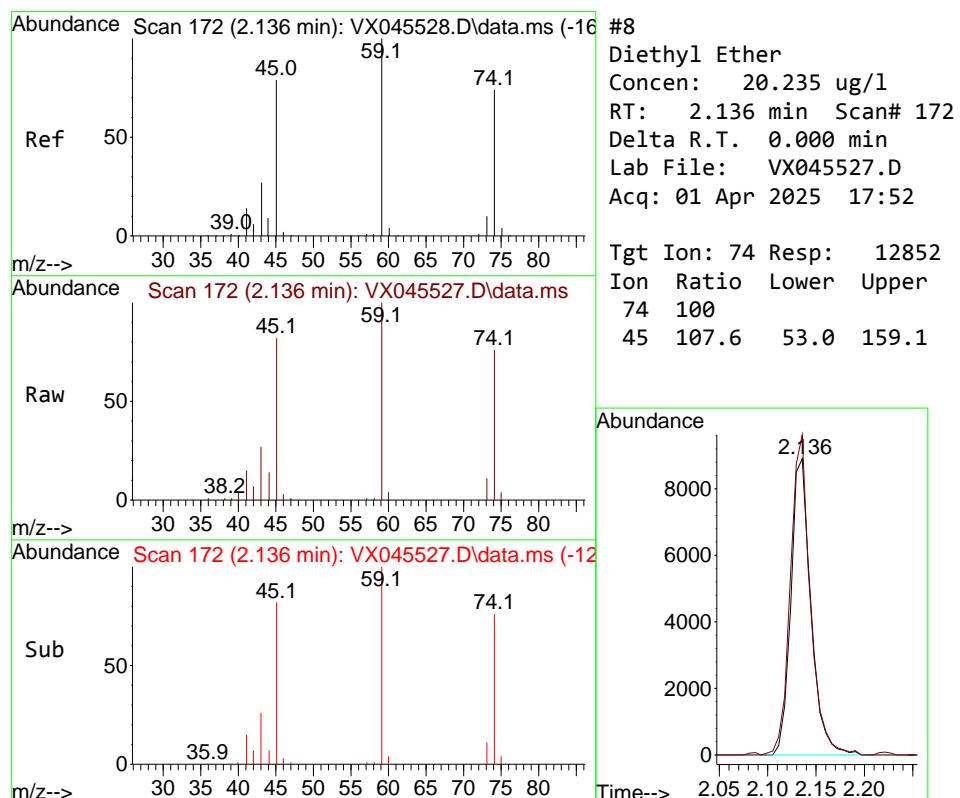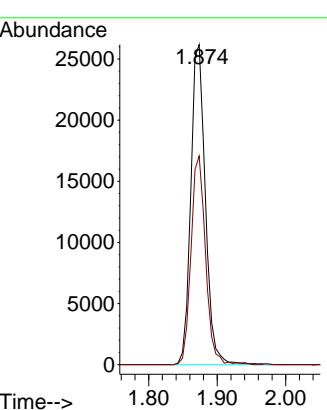

#8  
Diethyl Ether  
Concen: 20.235 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52


Tgt Ion: 74 Resp: 12852  
Ion Ratio Lower Upper  
74 100  
45 107.6 53.0 159.1





#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 20.673 ug/l  
RT: 2.319 min Scan# 2  
Delta R.T. -0.006 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020




Tgt Ion:101 Resp: 2291  
Ion Ratio Lower Upper  
101 100  
85 46.2 38.9 58.3  
151 66.8 57.5 86.3

### Manual Integrations APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

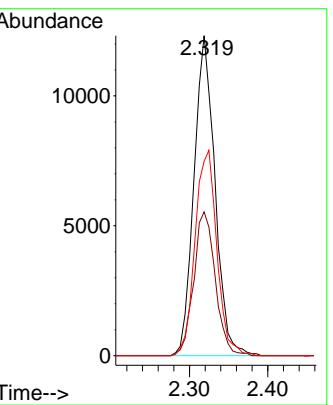


#10  
Methyl Iodide  
Concen: 20.596 ug/l  
RT: 2.441 min Scan# 222  
Delta R.T. -0.006 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52




Tgt Ion:142 Resp: 28478  
Ion Ratio Lower Upper  
142 100  
127 51.5 40.2 60.4  
141 14.8 11.7 17.5





Abundance Scan 311 (2.983 min): VX045527.D\data.ms

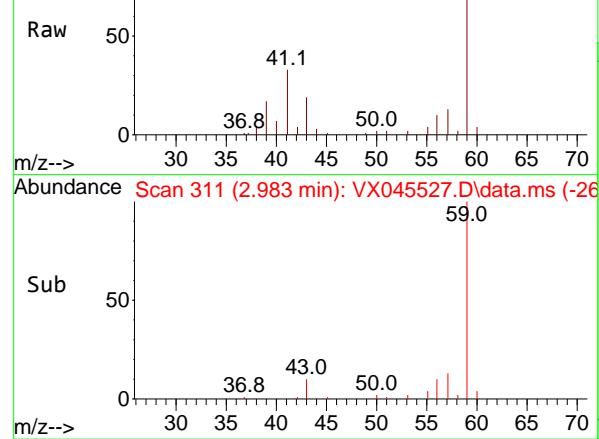

#11

Tert butyl alcohol

Concen: 101.253 ug/l

RT: 2.983 min Scan# 3

Delta R.T. 0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020


**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



Abundance Scan 200 (2.306 min): VX045527.D\data.ms

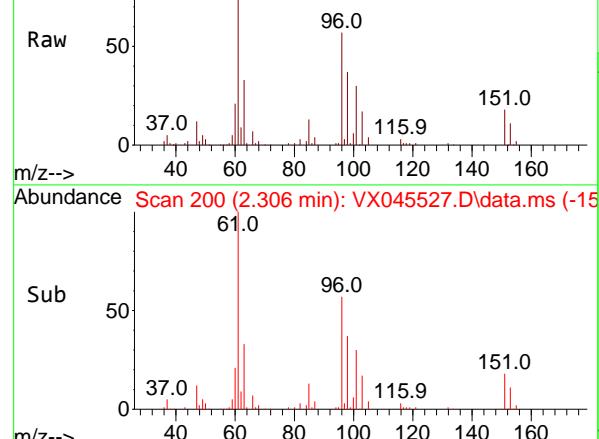

#12

1,1-Dichloroethene

Concen: 20.406 ug/l

RT: 2.306 min Scan# 200

Delta R.T. -0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 96 Resp: 22103


Ion Ratio Lower Upper

96 100

61 175.0 145.7 218.5

98 64.2 51.6 77.4




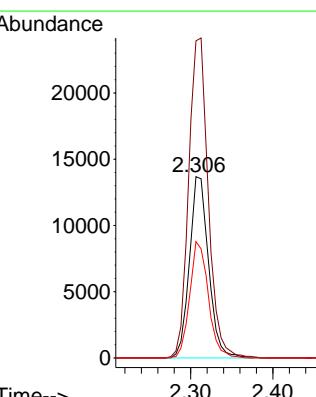





#13

Acrolein  
Concen: 94.938 ug/l  
RT: 2.239 min Scan# 189  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52



Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020









#14  
Allyl chloride  
Concen: 20.063 ug/l  
RT: 2.660 min Scan# 258  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52



Tgt Ion: 41 Resp: 41233  
Ion Ratio Lower Upper  
41 100  
39 74.2 60.2 90.2  
76 31.0 24.6 36.8

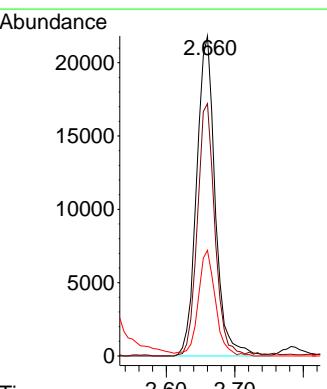

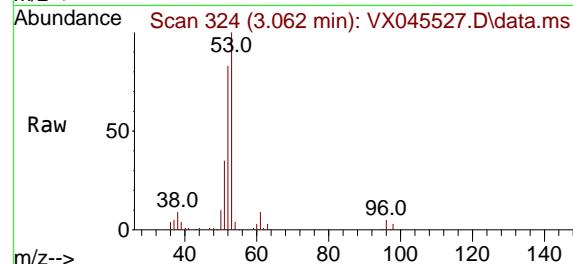

#15

Acrylonitrile

Concen: 106.412 ug/l

RT: 3.062 min Scan# 3

Instrument:

Delta R.T. 0.000 min

MSVOA\_X

Lab File: VX045527.D

ClientSampleId :

Acq: 01 Apr 2025 17:52

VSTDICC020

Tgt Ion: 53 Resp: 7448

Ion Ratio Lower Upper

53 100

52 81.8 67.4 101.2


51 37.6 29.9 44.9

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

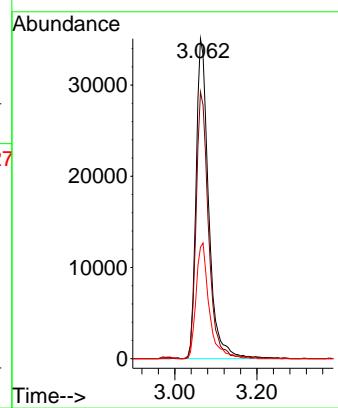

#16

Acetone

Concen: 103.000 ug/l

RT: 2.386 min Scan# 213

Delta R.T. 0.000 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52







Tgt Ion: 43 Resp: 69788

Ion Ratio Lower Upper

43 100

58 28.6 22.3 33.5

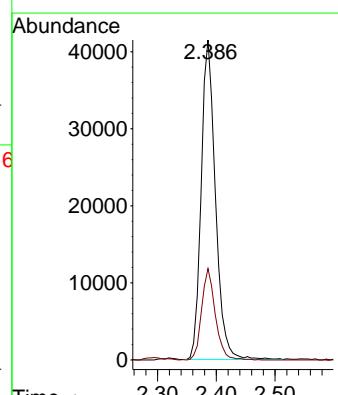

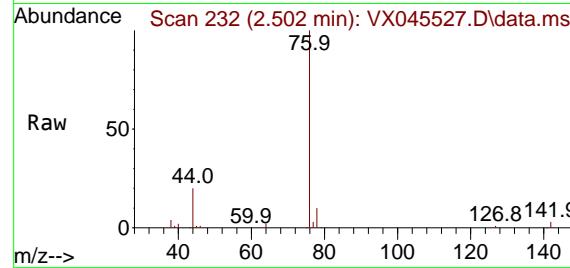

#17

Carbon Disulfide

Concen: 19.352 ug/l

RT: 2.502 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#18

Methyl Acetate

Concen: 19.994 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min


Lab File: VX045527.D







Acq: 01 Apr 2025 17:52

Tgt Ion: 43 Resp: 31190

Ion Ratio Lower Upper

43	100
74	21.3
17.5	26.3

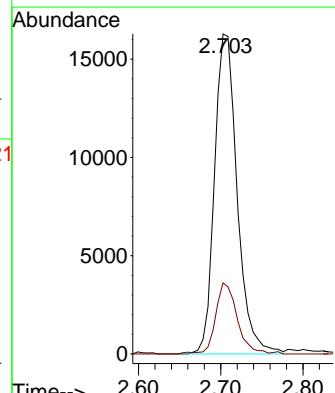



#19

Methyl tert-butyl Ether

Concen: 20.660 ug/l

RT: 3.117 min Scan# 3

Delta R.T. 0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#20

Methylene Chloride

Concen: 20.664 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt Ion: 84 Resp: 26212


Ion Ratio Lower Upper


84 100

49 139.9 107.5 161.3

51 43.0 33.0 49.6

86 61.1 50.1 75.1

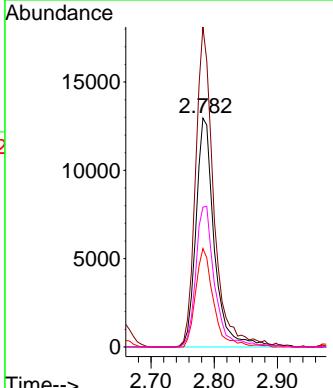

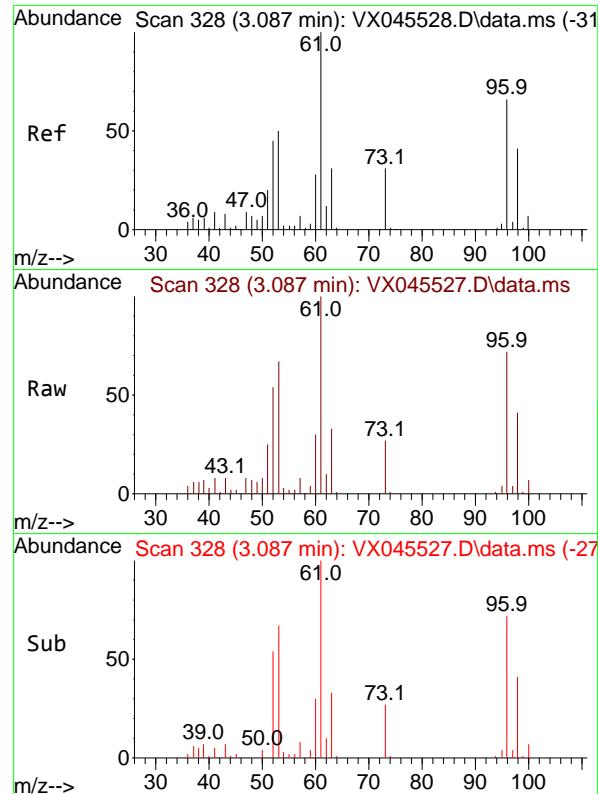


#21  
trans-1,2-Dichloroethene  
Concen: 20.755 ug/l  
RT: 3.087 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

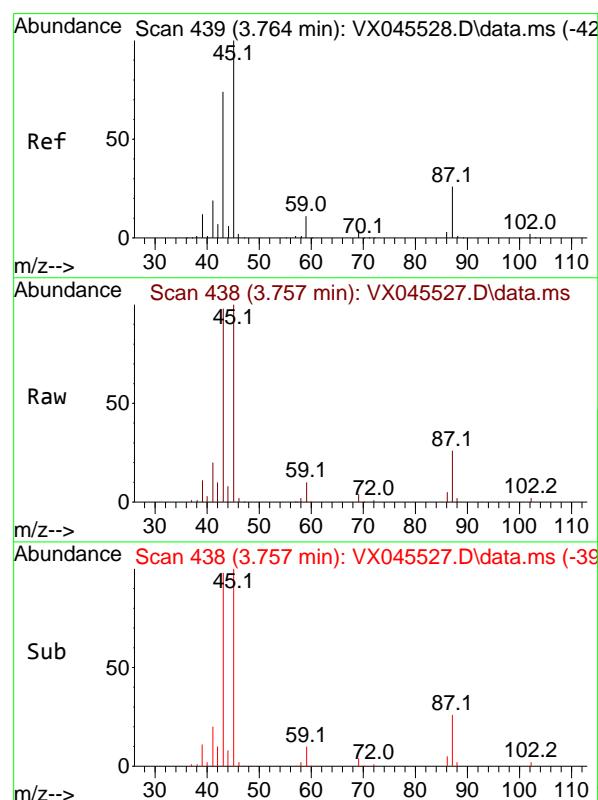

#22  
Diisopropyl ether  
Concen: 20.760 ug/l  
RT: 3.757 min Scan# 438  
Delta R.T. -0.006 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Tgt Ion: 45 Resp: 84046  
Ion Ratio Lower Upper  
45 100  
43 98.0 59.3 88.9#  
87 25.9 20.4 30.6  
59 10.3 9.0 13.6

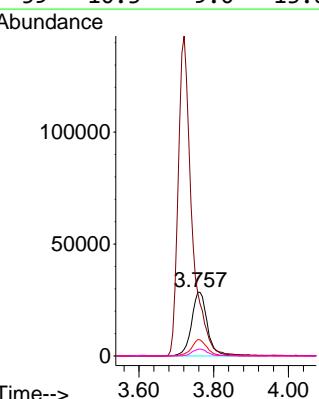

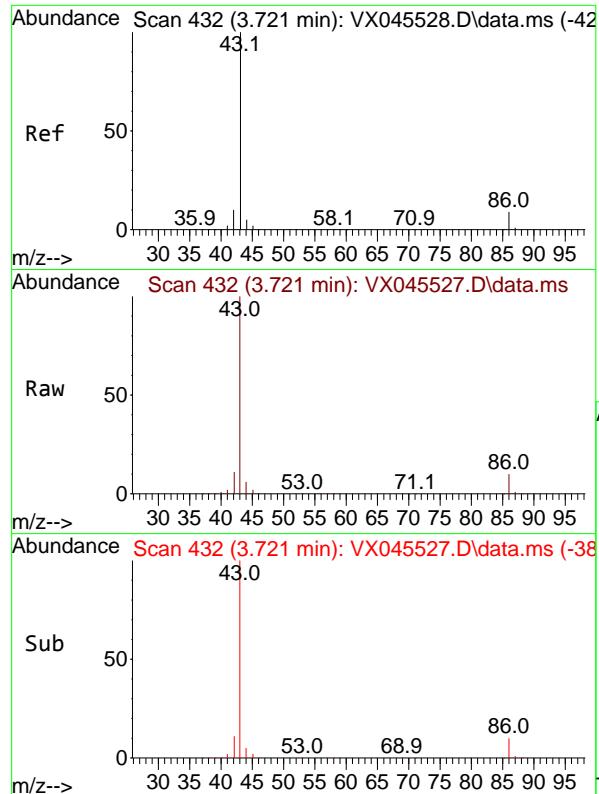

#23

Vinyl Acetate

Concen: 103.458 ug/l

RT: 3.721 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC020

Tgt Ion: 43 Resp: 36188

Ion Ratio Lower Upper

43 100



86 9.6 7.5 11.3

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

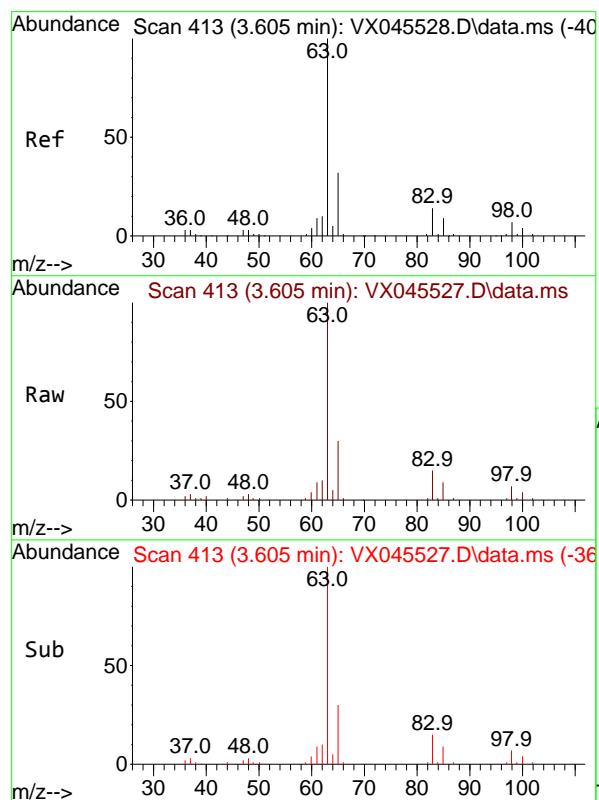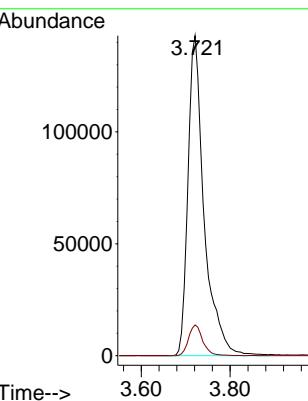

#24

1,1-Dichloroethane

Concen: 20.772 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 63 Resp: 47560


Ion Ratio Lower Upper

63 100

98 6.5 3.4 10.1


100 3.8 2.2 6.6

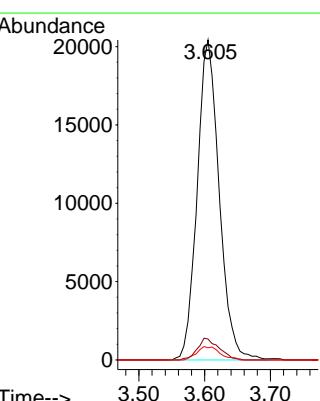



#25  
2-Butanone  
Concen: 105.931 ug/l  
RT: 4.556 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020




Tgt Ion: 43 Resp: 10506  
Ion Ratio Lower Upper  
43 100  
72 22.9 18.6 28.0

Manual Integrations  
APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025


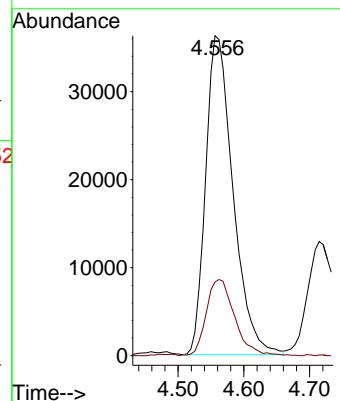



#26  
2,2-Dichloropropane  
Concen: 19.574 ug/l  
RT: 4.471 min Scan# 555  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52



Tgt Ion: 77 Resp: 28956  
Ion Ratio Lower Upper  
77 100  
97 21.8 10.6 31.8

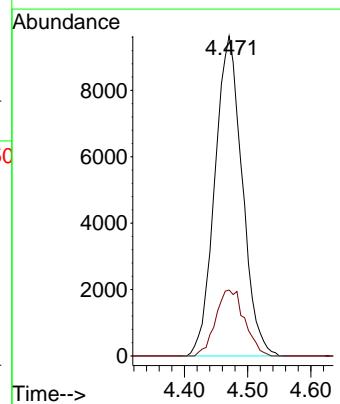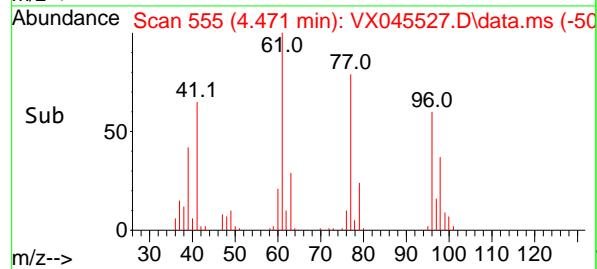


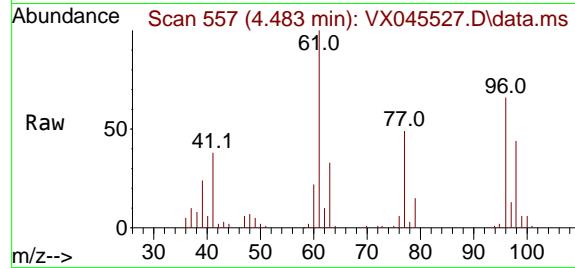



#27  
*cis*-1,2-Dichloroethene  
 Concen: 20.342 ug/l  
 RT: 4.483 min Scan# 5  
 Delta R.T. 0.000 min  
 Lab File: VX045527.D  
 Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC020



### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025



#28  
 Bromochloromethane  
 Concen: 20.141 ug/l  
 RT: 4.897 min Scan# 625  
 Delta R.T. 0.000 min  
 Lab File: VX045527.D  
 Acq: 01 Apr 2025 17:52

Tgt Ion: 49 Resp: 22285  
 Ion Ratio Lower Upper  
 49 100  
 129 1.8 0.0 3.8  
 130 68.0 54.6 81.8



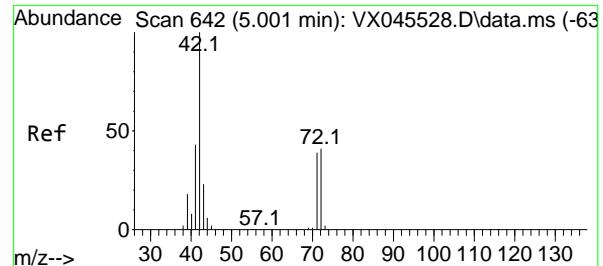

#29

Tetrahydrofuran

Concen: 104.187 ug/l

RT: 5.007 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC020

Tgt Ion: 42 Resp: 6699

Ion Ratio Lower Upper

42 100





72 42.1 33.4 50.0

71 38.2 31.4 47.0

**Manual Integrations****APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

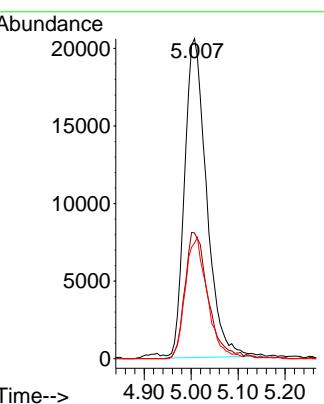

#30

Chloroform

Concen: 20.646 ug/l

RT: 5.093 min Scan# 657

Delta R.T. 0.006 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52


Tgt Ion: 83 Resp: 48639

Ion Ratio Lower Upper


83 100

85 65.8 52.8 79.2


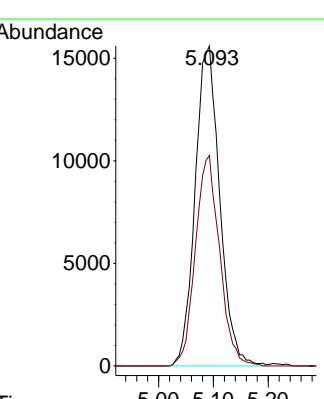





Abundance Scan 717 (5.458 min): VX045527.D\data.ms

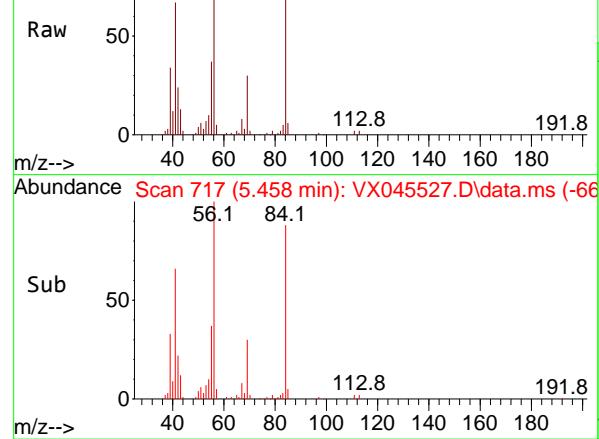


Abundance Scan 717 (5.458 min): VX045527.D\data.ms (-66)

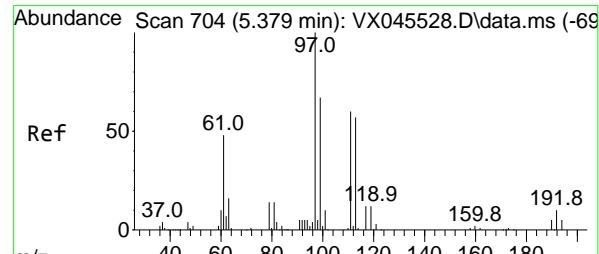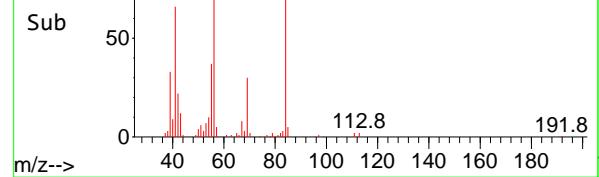

Abundance Scan 703 (5.373 min): VX045527.D\data.ms

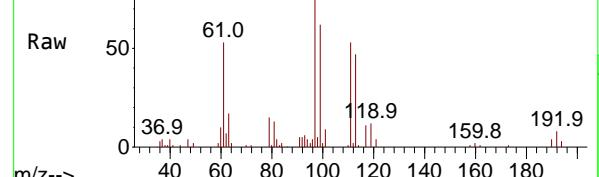

Abundance Scan 703 (5.373 min): VX045527.D\data.ms (-65)

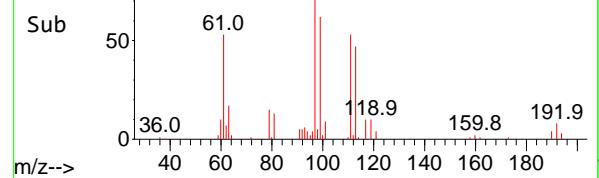

#31

Cyclohexane

Concen: 20.478 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020


### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025


Supervised By :Mahesh Dadoda 04/02/2025

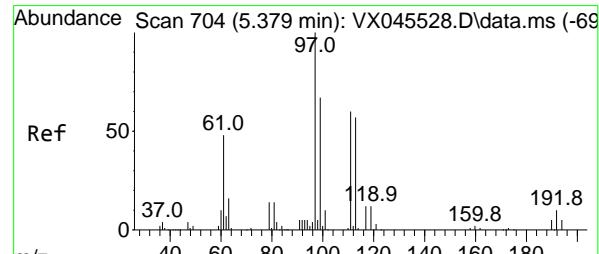

Abundance Scan 703 (5.373 min): VX045527.D\data.ms

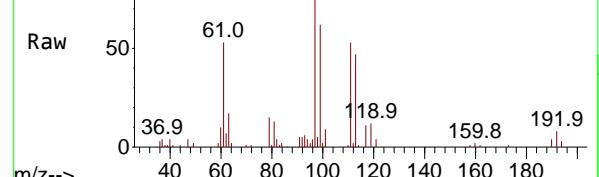

Abundance Scan 703 (5.373 min): VX045527.D\data.ms (-65)

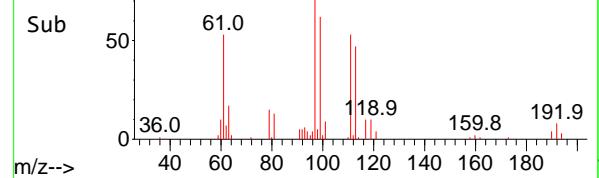

#32

1,1,1-Trichloroethane

Concen: 20.270 ug/l

RT: 5.373 min Scan# 703

Delta R.T. -0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 97 Resp: 40407


Ion Ratio Lower Upper

97 100

99 63.3 51.7 77.5

61 51.3 41.0 61.4





#33

1,2-Dichloroethane-d4




Concen: 19.697 ug/l

RT: 5.952 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

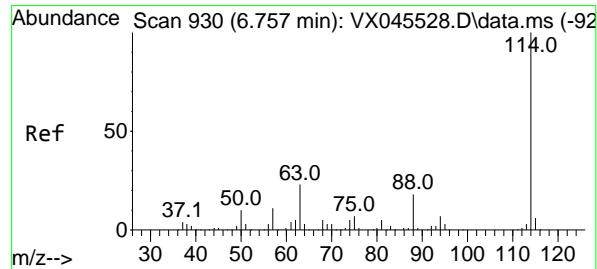

#34

1,4-Difluorobenzene



Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

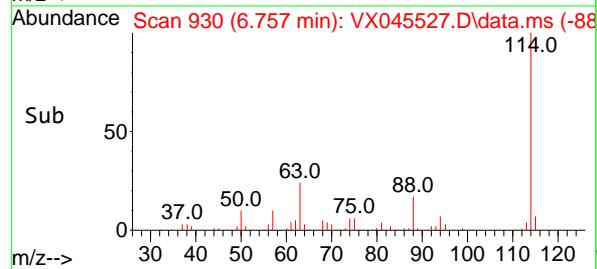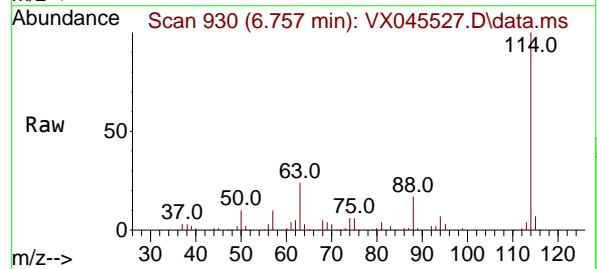

Time--&gt;

Tgt Ion: 65 Resp: 32500

Ion Ratio Lower Upper

65 100

67 51.5 0.0 99.0

Instrument :

MSVOA\_X

ClientSampleId :


VSTDICC020

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

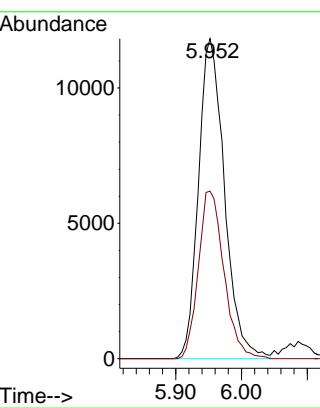

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 114 Resp: 160754







Ion Ratio Lower Upper

114 100

63 24.2 0.0 46.8

88 16.7 0.0 35.4

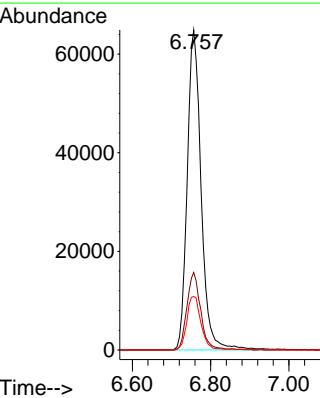

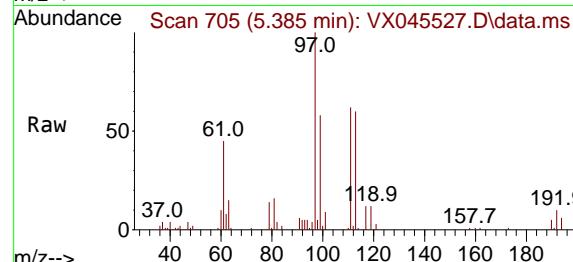

#35

Dibromofluoromethane

Concen: 19.256 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#36

1,1-Dichloropropene

Concen: 19.808 ug/l

RT: 5.684 min Scan# 754

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 75 Resp: 30504




Ion Ratio Lower Upper

75 100

110 34.0 16.9 50.6

77 32.7 25.0 37.4



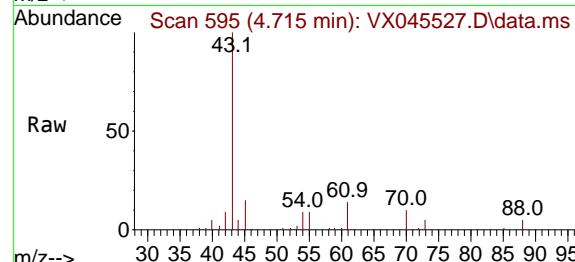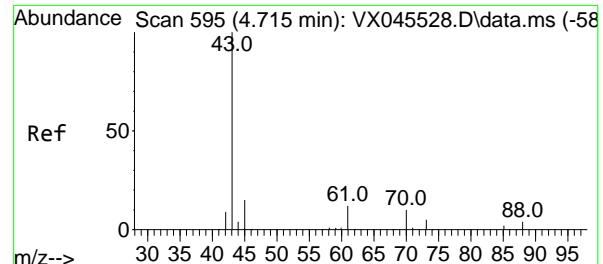

#37

## Ethyl Acetate

Concen: 20.180 ug/l

RT: 4.715 min Scan# 595

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#38

## Carbon Tetrachloride

Concen: 20.148 ug/l


RT: 5.672 min Scan# 752


Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt	Ion:117	Resp:	33533
Ion	Ratio	Lower	Upper
117	100		
119	88.5	76.9	115.3
121	30.3	24.2	36.2

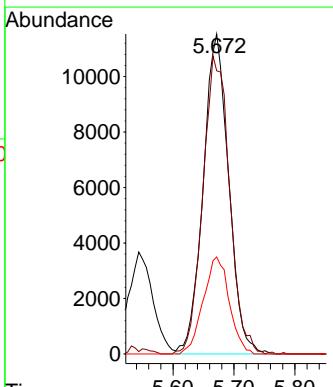

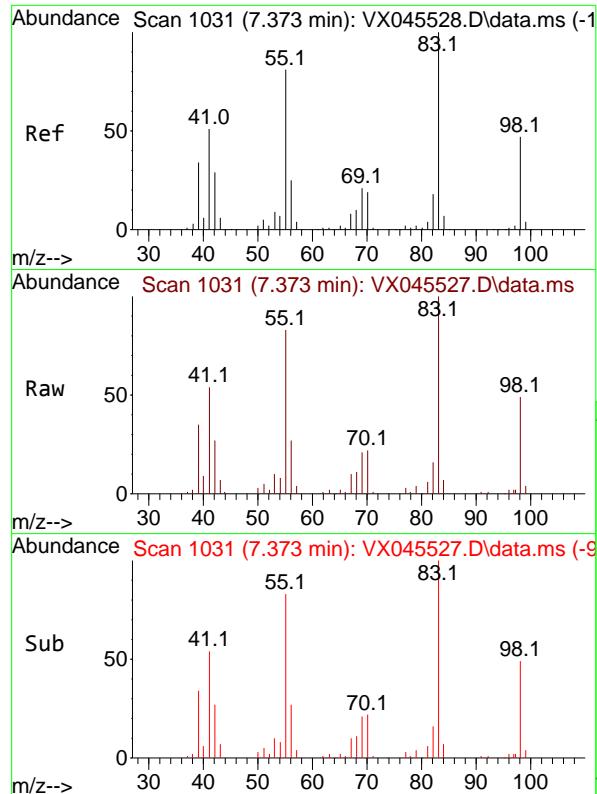

#39

Methylcyclohexane

Concen: 20.291 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

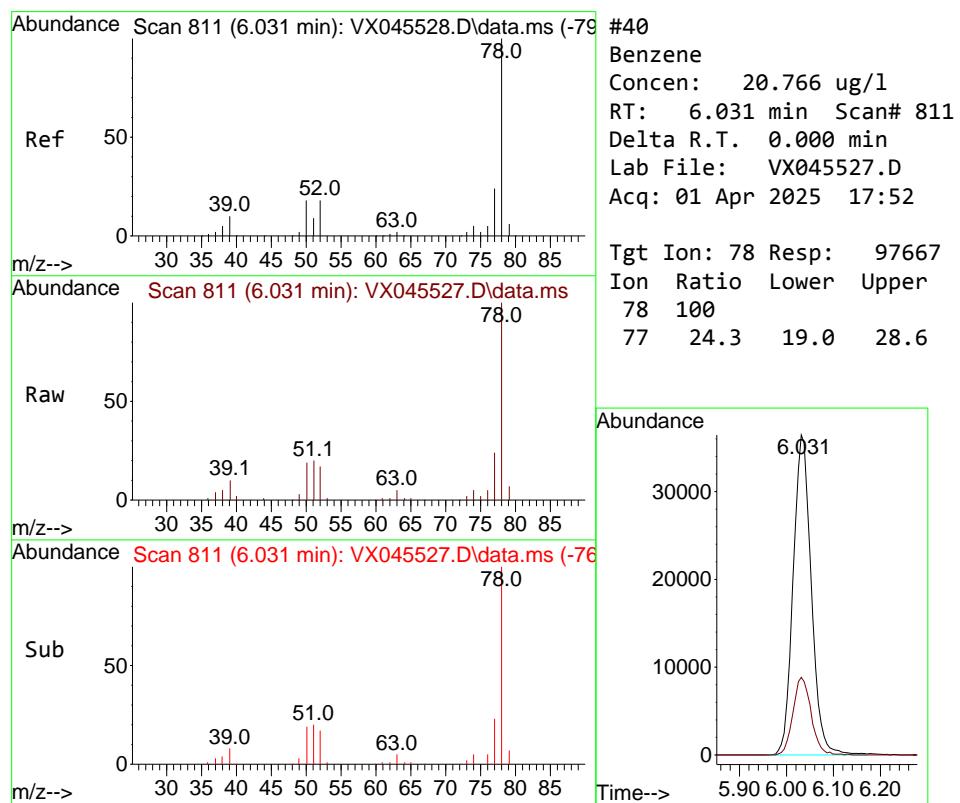

#40

Benzene

Concen: 20.766 ug/l

RT: 6.031 min Scan# 811


Delta R.T. 0.000 min







Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt Ion: 78 Resp: 97667

Ion	Ratio	Lower	Upper
78	100		
77	24.3	19.0	28.6



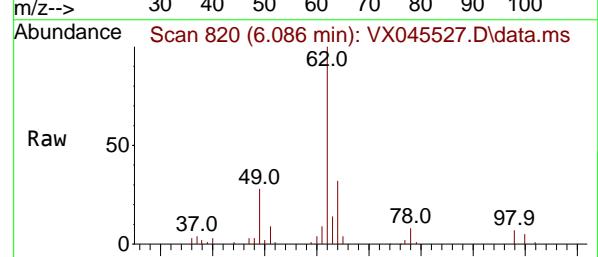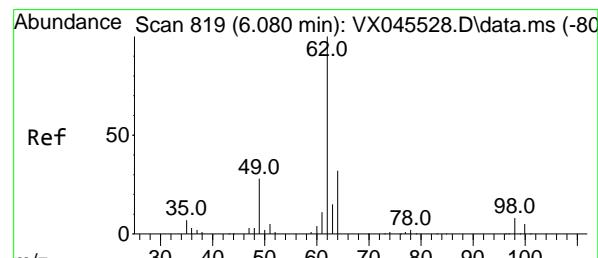

#41

Methacrylonitrile

Concen: 21.046 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X


ClientSampleId : VSTDICC020

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

Abundance

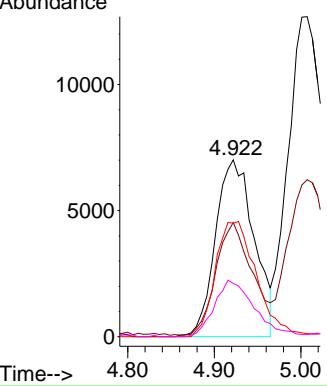

#42

1,2-Dichloroethane

Concen: 21.484 ug/l

RT: 6.086 min Scan# 820

Delta R.T. 0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 62 Resp: 41733







Ion Ratio Lower Upper

62 100

98 7.7 0.0 15.2

Abundance

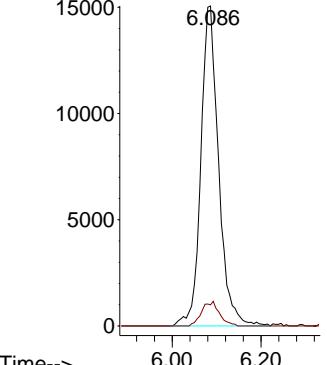

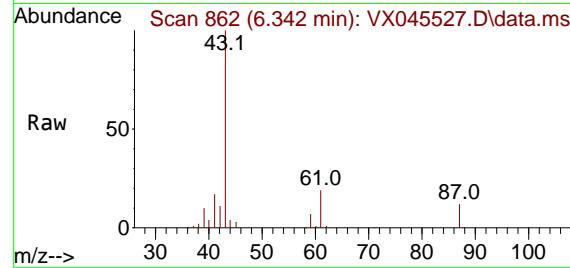

#43

Isopropyl Acetate

Concen: 20.814 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

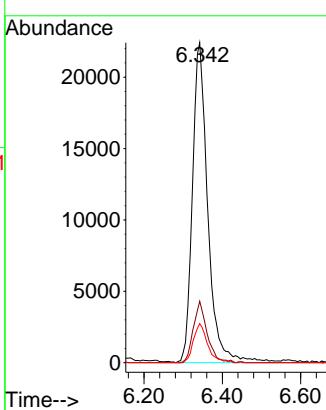

#44

Trichloroethene

Concen: 20.501 ug/l

RT: 7.123 min Scan# 990

Delta R.T. 0.000 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52




Tgt Ion:130 Resp: 22918

Ion Ratio Lower Upper

130 100

95 104.4 0.0 202.0

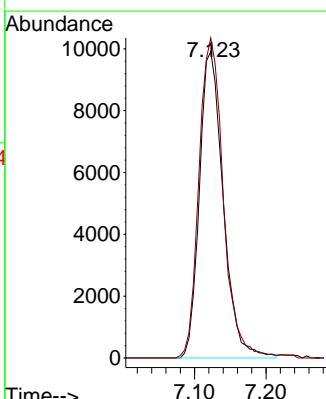



#45

1,2-Dichloropropane

Concen: 21.241 ug/l

RT: 7.428 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

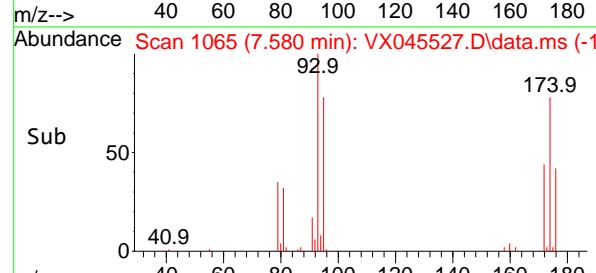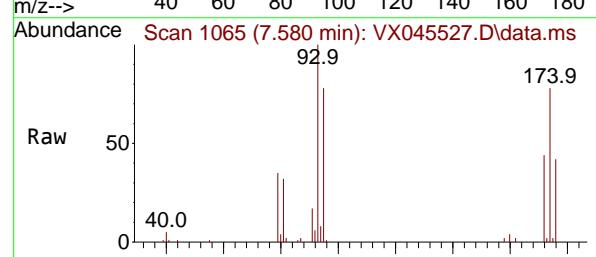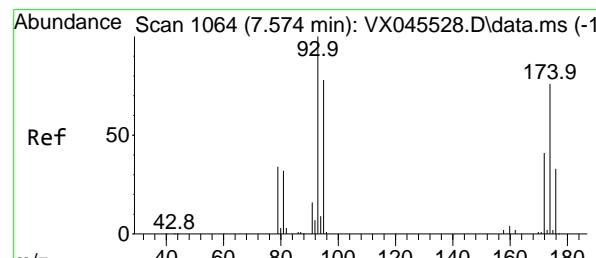

#46

Dibromomethane

Concen: 21.207 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 93 Resp: 19104


Ion Ratio Lower Upper

93 100

95 79.2 64.8 97.2

174 81.1 65.4 98.0



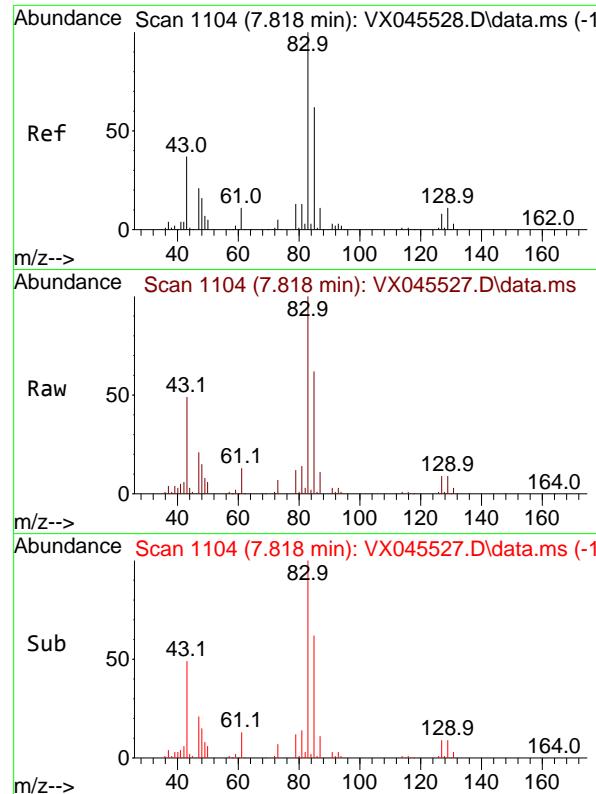

#47

Bromodichloromethane

Concen: 20.587 ug/l

RT: 7.818 min Scan# 1104

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

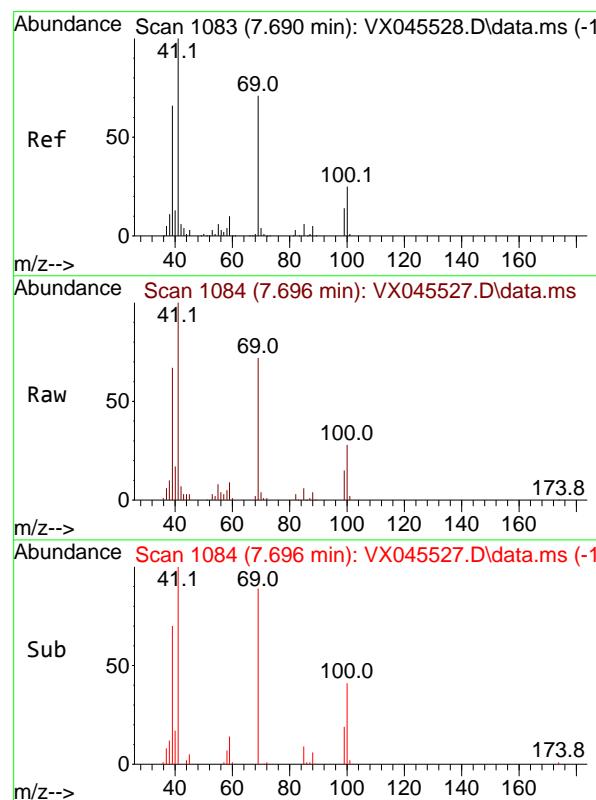

#48

Methyl methacrylate

Concen: 20.575 ug/l

RT: 7.696 min Scan# 1084


Delta R.T. 0.006 min


Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt Ion: 41 Resp: 31247

Ion	Ratio	Lower	Upper
41	100		
69	73.4	58.2	87.2
39	68.7	53.6	80.4

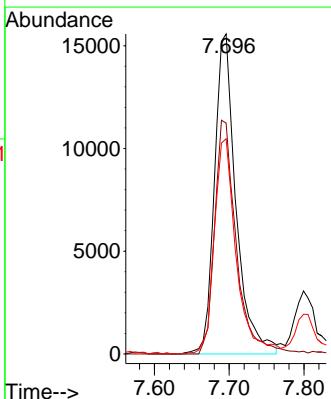



#49

1,4-Dioxane

Concen: 440.515 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC020

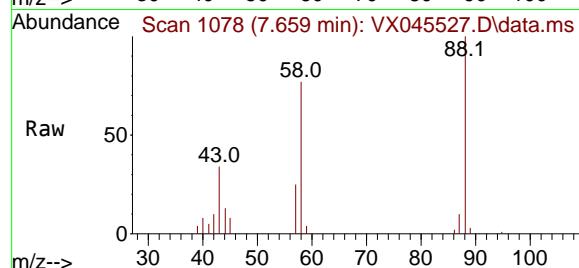

Tgt Ion: 88 Resp: 12104

Ion Ratio Lower Upper

88 100

43 43.5 32.2 48.4







58 76.4 58.6 88.0


Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025
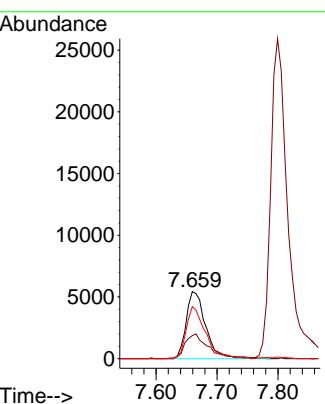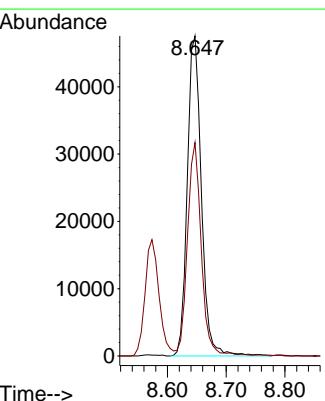
#50  
Toluene-d8  
Concen: 19.921 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52Tgt Ion: 98 Resp: 79303  
Ion Ratio Lower Upper  
98 100  
100 64.7 52.2 78.4




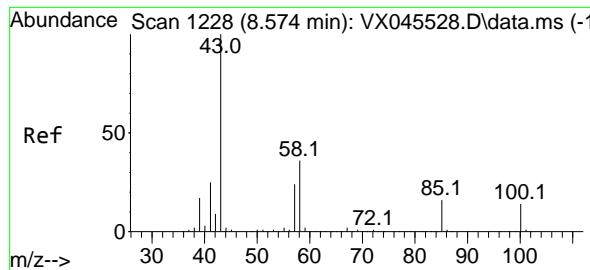


#51  
4-Methyl-2-Pentanone  
Concen: 109.055 ug/l  
RT: 8.574 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

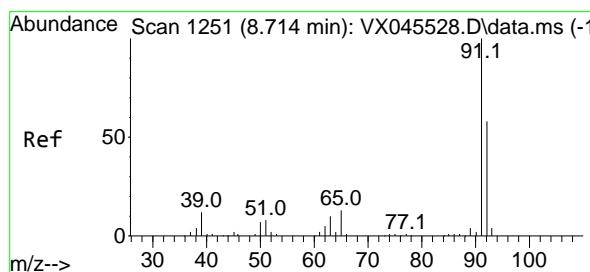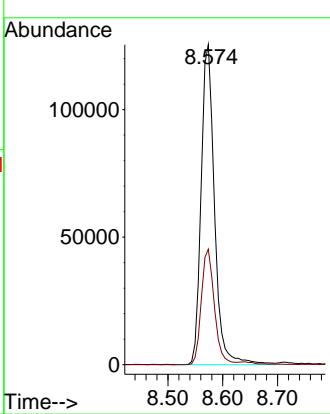
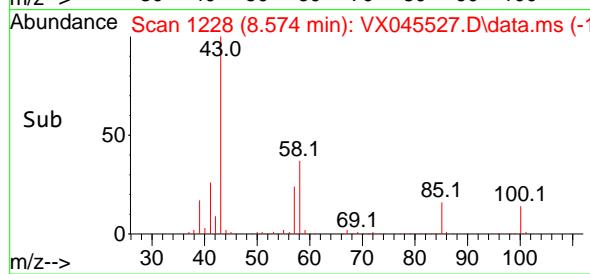
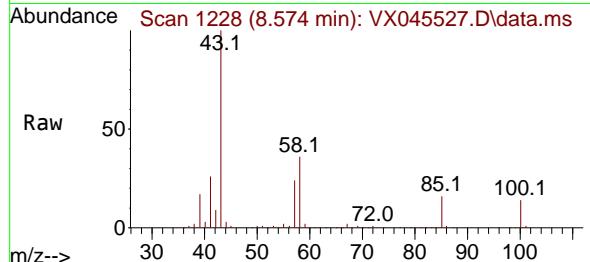





#52  
Toluene  
Concen: 21.208 ug/l  
RT: 8.714 min Scan# 1251  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

```

Tgt Ion: 92 Resp: 60357
Ion Ratio Lower Upper
 92 100
 91 171.6 138.7 208.1

```

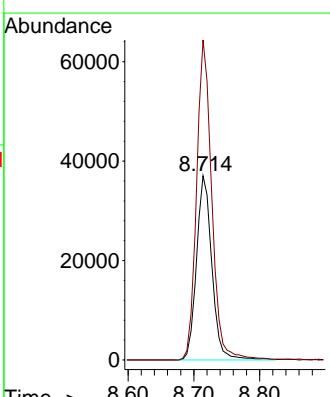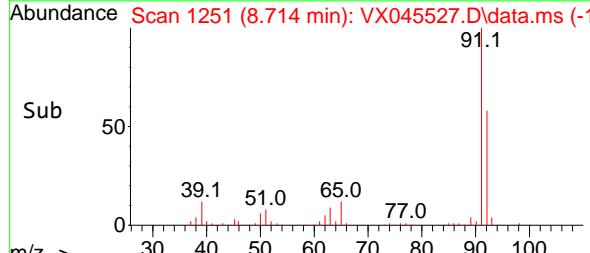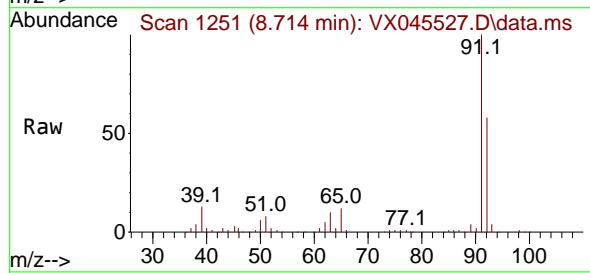



#53

t-1,3-Dichloropropene

Concen: 18.764 ug/l

RT: 8.976 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

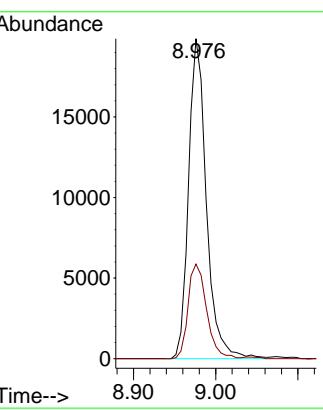

#54

cis-1,3-Dichloropropene

Concen: 20.762 ug/l


RT: 8.366 min Scan# 1194







Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt	Ion: 75	Resp:	35099
Ion	Ratio	Lower	Upper
75	100		
77	32.1	24.6	36.8
39	65.0	48.4	72.6

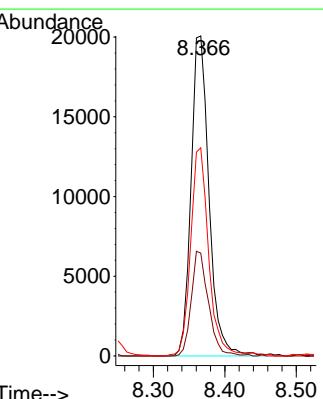



#55

1,1,2-Trichloroethane

Concen: 21.331 ug/l

RT: 9.147 min Scan# 1322

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC020

**Manual Integrations****APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

Tgt Ion: 97 Resp: 2419


Ion Ratio Lower Upper

97 100

83 93.4 71.8 107.8

85 55.9 47.0 70.6

99 64.9 48.6 73.0

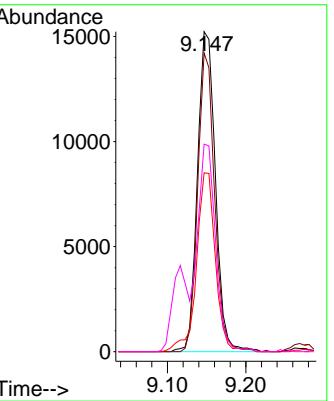

#56

Ethyl methacrylate

Concen: 20.600 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 69 Resp: 36155


Ion Ratio Lower Upper

69 100

41 77.4 61.3 91.9

39 51.5 40.2 60.2

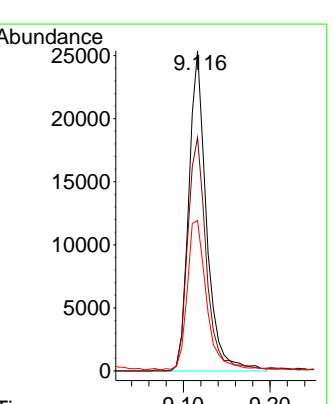


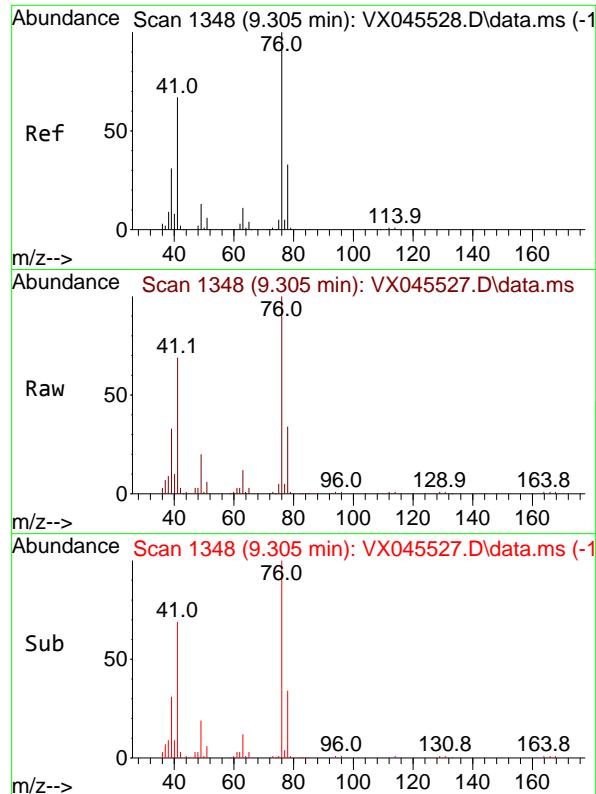


#57  
1,3-Dichloropropane  
Concen: 21.217 ug/l  
RT: 9.305 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

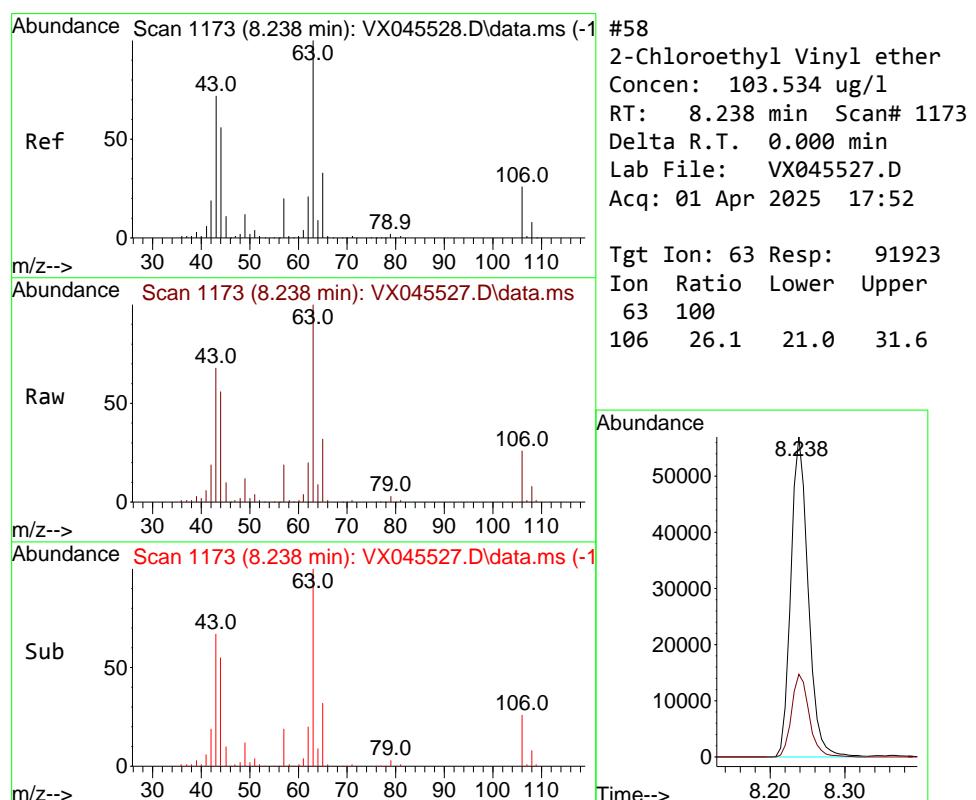


#58  
2-Chloroethyl Vinyl ether  
Concen: 103.534 ug/l  
RT: 8.238 min Scan# 1173  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Tgt Ion: 63 Resp: 91923  
Ion Ratio Lower Upper  
63 100  
106 26.1 21.0 31.6







Abundance Scan 1368 (9.427 min): VX045527.D\data.ms

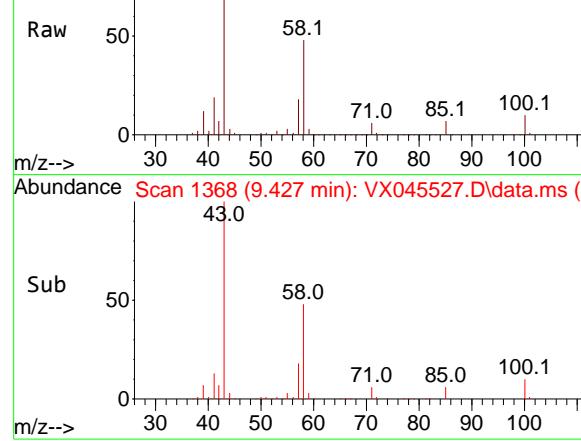


Abundance Scan 1368 (9.427 min): VX045527.D\data.ms (-1)

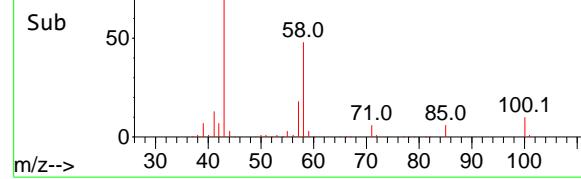


Abundance Scan 1383 (9.519 min): VX045528.D\data.ms (-1)

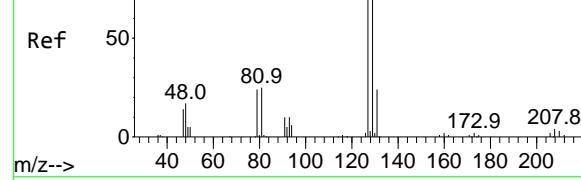

Abundance Scan 1383 (9.519 min): VX045527.D\data.ms

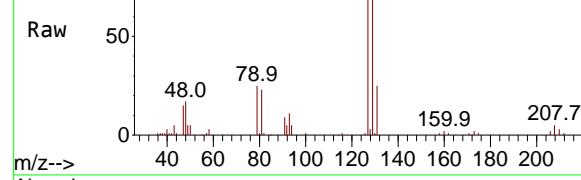

Abundance Scan 1383 (9.519 min): VX045527.D\data.ms (-1)

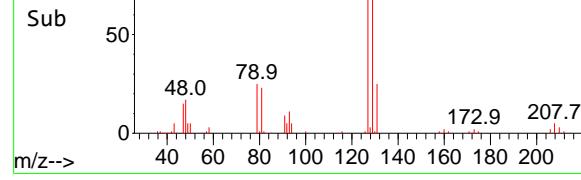

#59

2-Hexanone

Concen: 108.730 ug/l

RT: 9.427 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC020

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

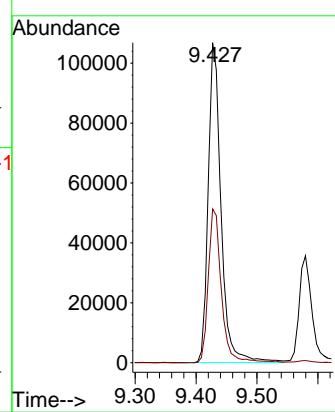

#60

Dibromochloromethane

Concen: 21.023 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52




Tgt Ion:129 Resp: 25992

Ion Ratio Lower Upper

129 100

127 77.3 39.4 118.2

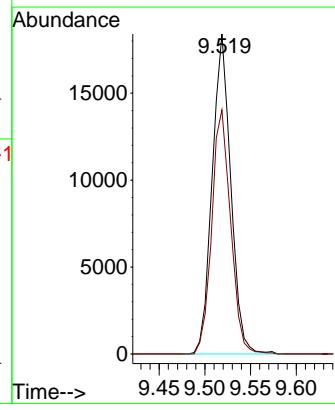

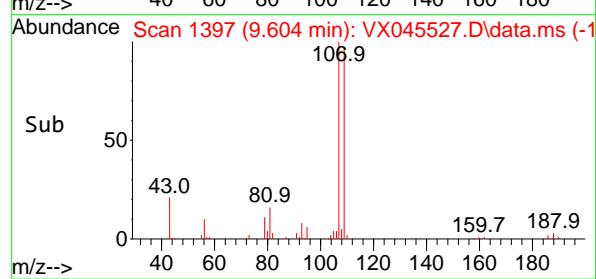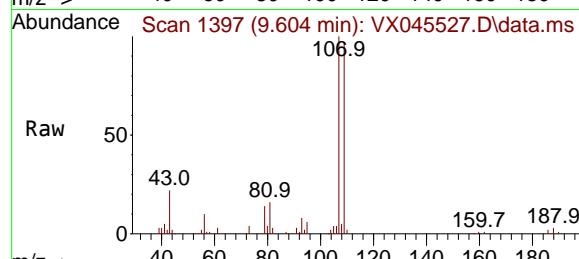

#61

1,2-Dibromoethane

Concen: 21.303 ug/l

RT: 9.604 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

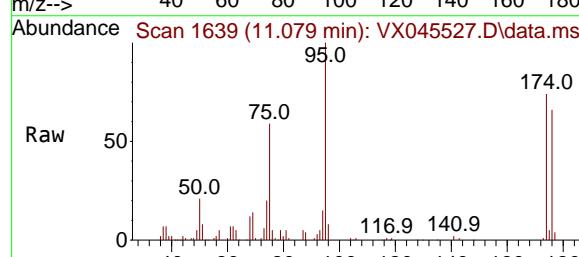

#62

4-Bromofluorobenzene

Concen: 19.858 ug/l


RT: 11.079 min Scan# 1639


Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt	Ion:	95	Resp:	28795
Ion	Ratio	Lower	Upper	
95	100			
174	71.1	0.0	135.8	
176	65.8	0.0	131.4	




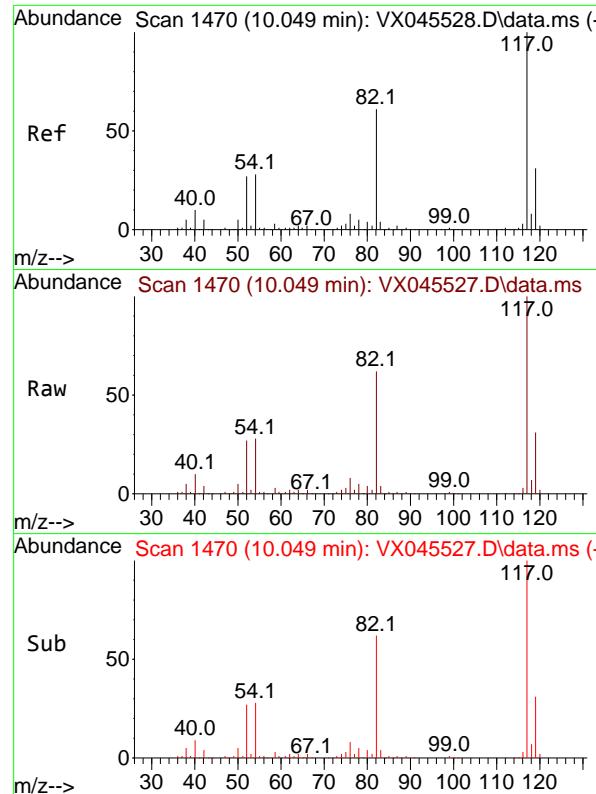


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1470  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

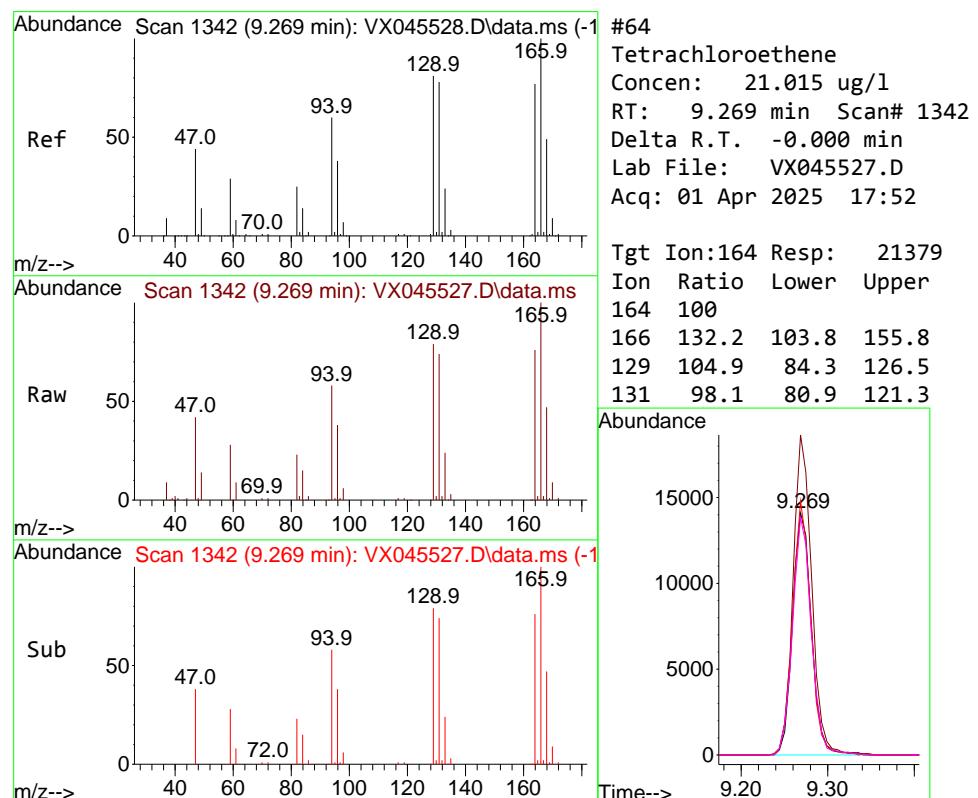

#64  
Tetrachloroethene  
Concen: 21.015 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Tgt Ion:164 Resp: 21379  
Ion Ratio Lower Upper  
164 100  
166 132.2 103.8 155.8  
129 104.9 84.3 126.5  
131 98.1 80.9 121.3

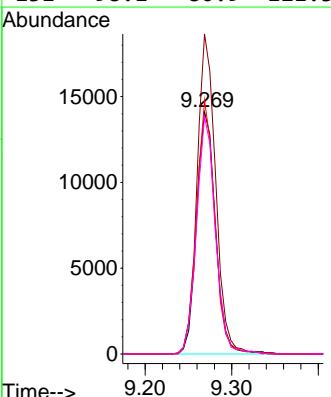

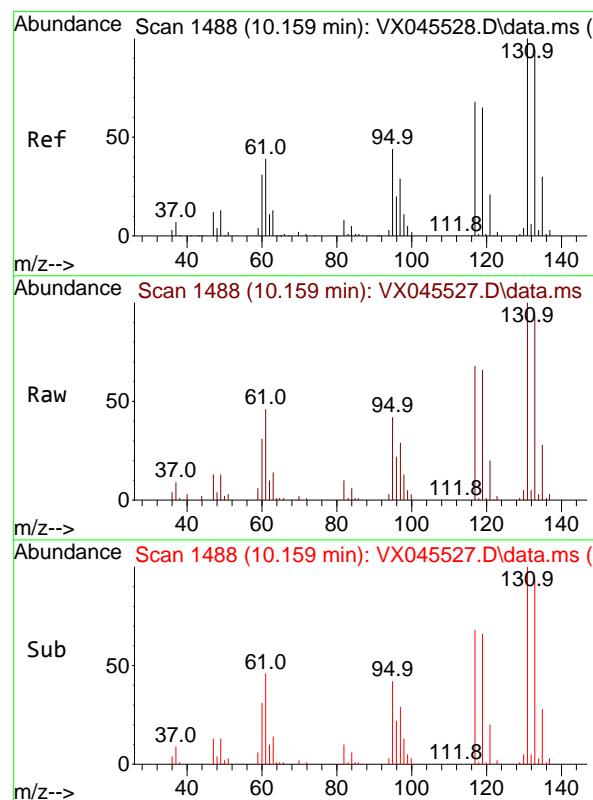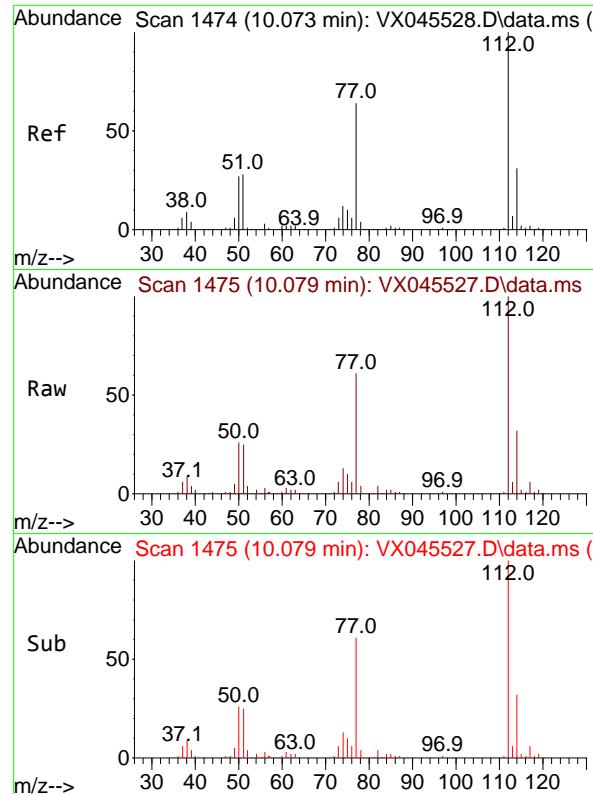

#65

Chlorobenzene

Concen: 21.023 ug/l

RT: 10.079 min Scan# 1475

Delta R.T. 0.006 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#66

1,1,1,2-Tetrachloroethane

Concen: 20.064 ug/l

RT: 10.159 min Scan# 1488

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion:131 Resp: 21447




Ion Ratio Lower Upper

131 100

133 92.8 47.5 142.5

119 66.3 32.9 98.6

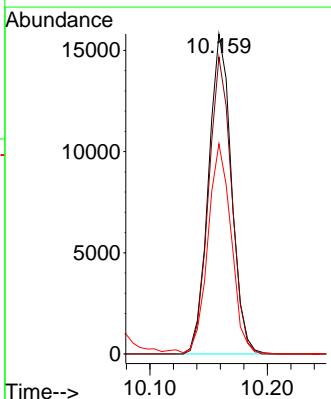



#67

Ethyl Benzene

Concen: 20.921 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#68

m/p-Xylenes

Concen: 42.092 ug/l


RT: 10.299 min Scan# 1511


Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt Ion:106 Resp: 84420  
 Ion Ratio Lower Upper  
 106 100  
 91 214.4 172.6 258.8

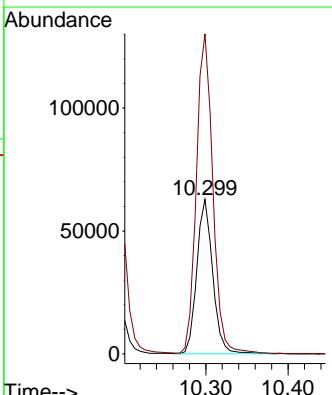

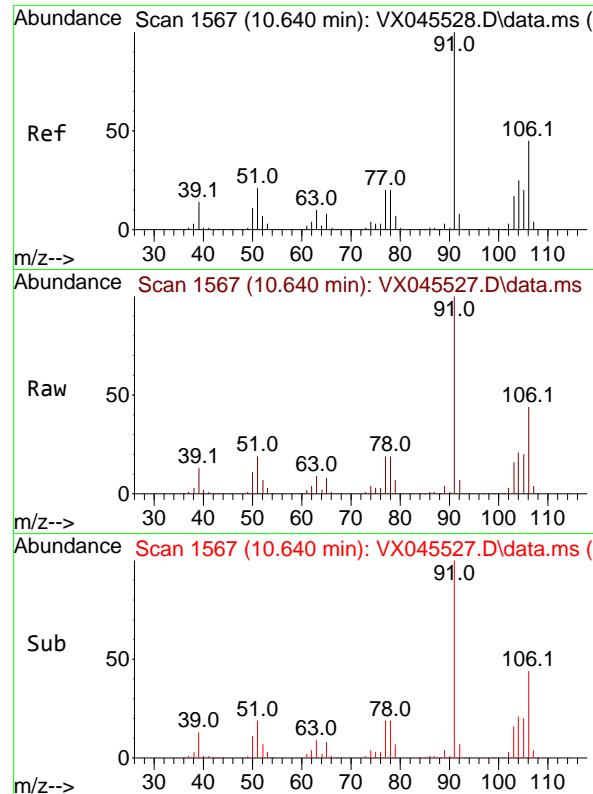


#69  
o-Xylene  
Concen: 21.158 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52  
ClientSampleId : VSTDICC020

**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025




Supervised By :Mahesh Dadoda 04/02/2025

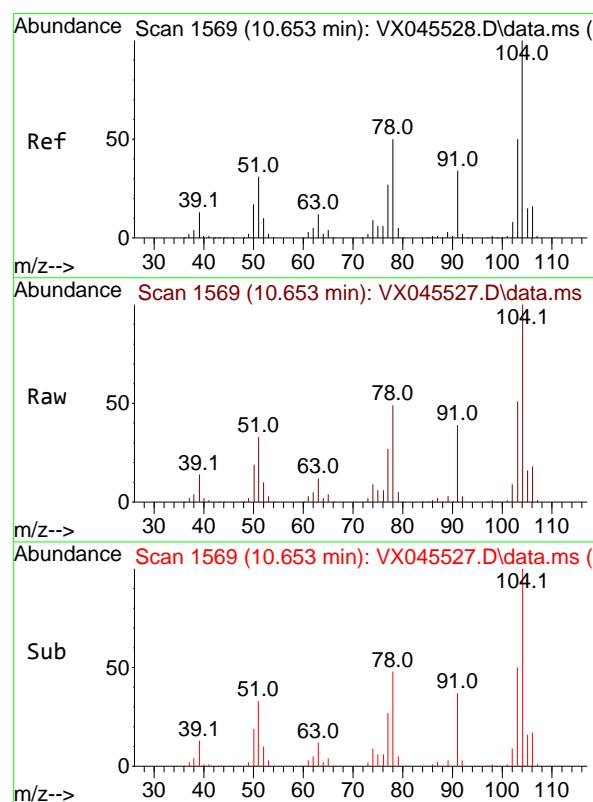

#70  
Styrene  
Concen: 21.249 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Tgt Ion:104 Resp: 69290  
Ion Ratio Lower Upper  
104 100  
78 57.0 45.4 68.2  
103 56.5 43.8 65.8

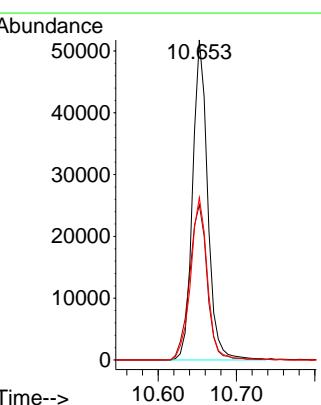

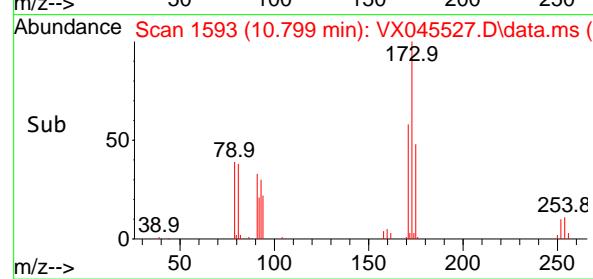

#71

Bromoform

Concen: 19.619 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

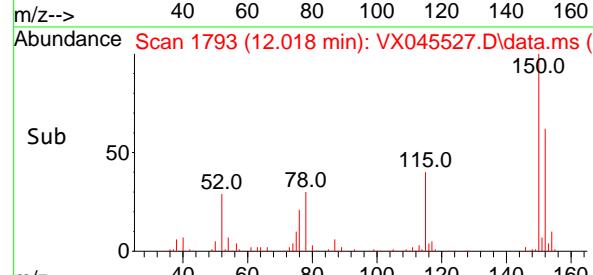

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion:152 Resp: 65341


Ion Ratio Lower Upper

152 100

115 76.8 46.9 140.7

150 166.0 0.0 349.4

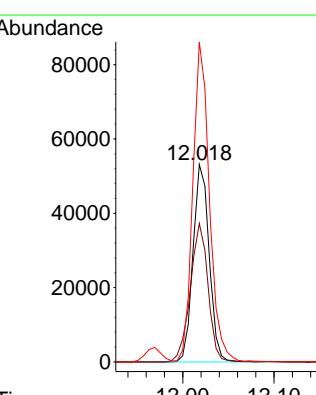

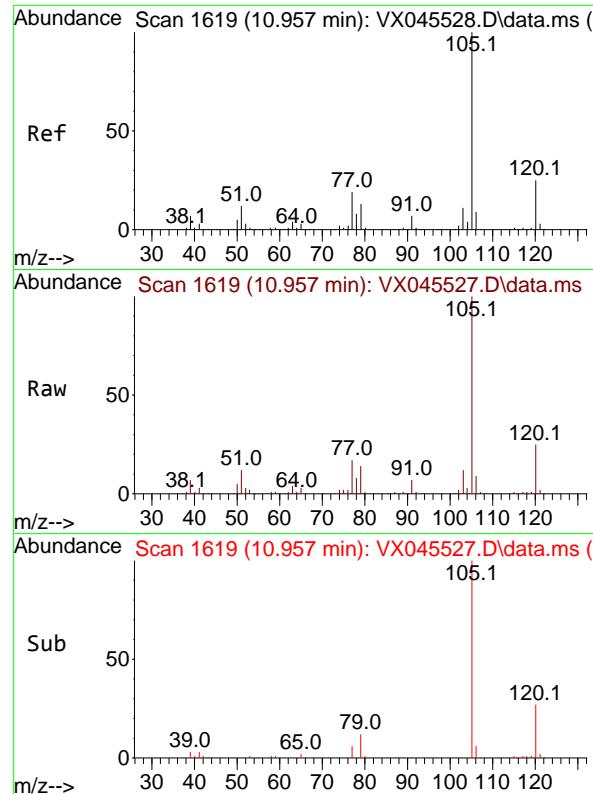

#73

Isopropylbenzene

Concen: 21.093 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

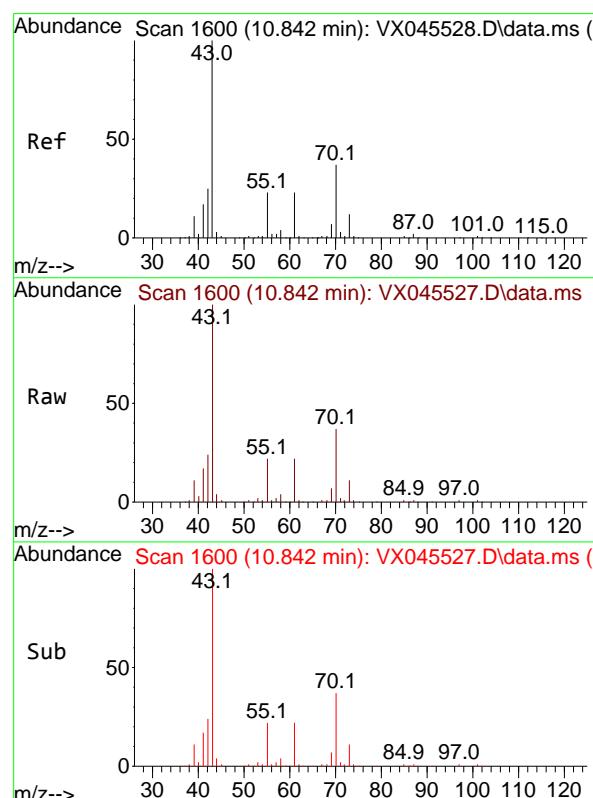

#74

N-amyl acetate

Concen: 20.466 ug/l

RT: 10.842 min Scan# 1600

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt Ion: 43 Resp: 51238


Ion Ratio Lower Upper



43 100

70 38.1 30.1 45.1

55 22.5 18.3 27.5

61 22.1 17.5 26.3

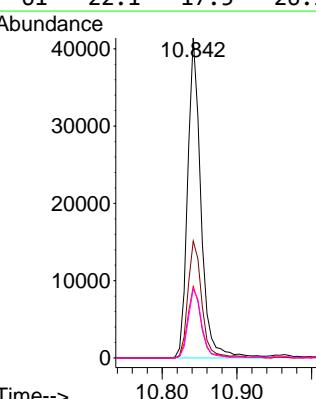

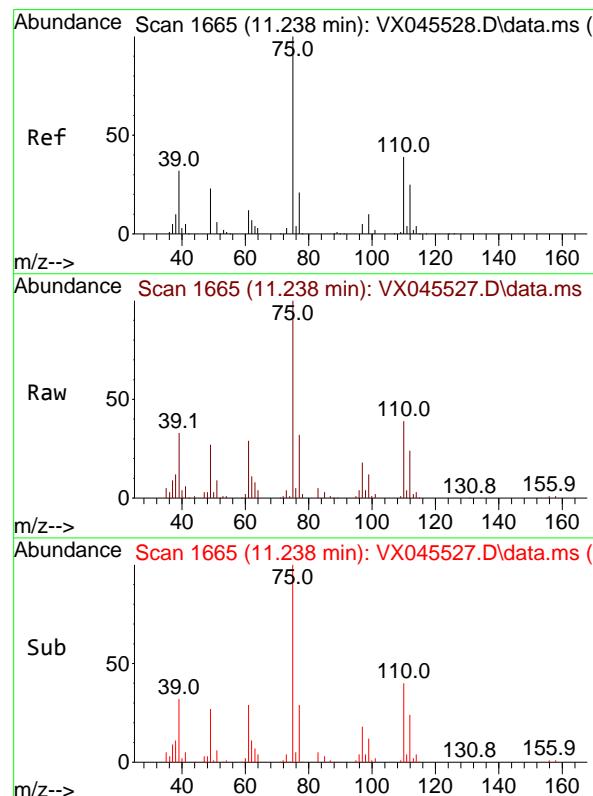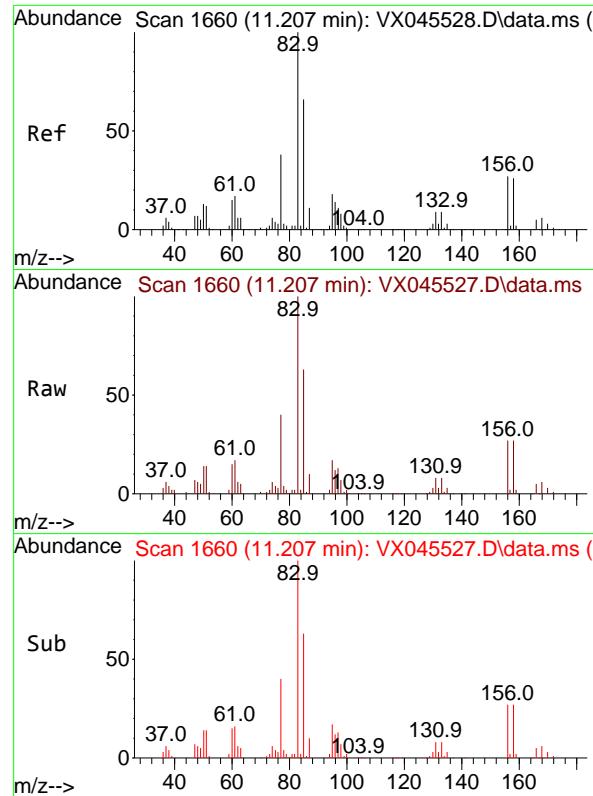


#75  
1,1,2,2-Tetrachloroethane  
Concen: 20.764 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

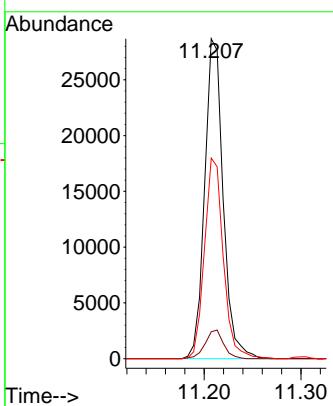

#76  
1,2,3-Trichloropropane  
Concen: 20.510 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Tgt Ion: 75 Resp: 32690  
Ion Ratio Lower Upper  
75 100  
77 41.2 20.0 59.9



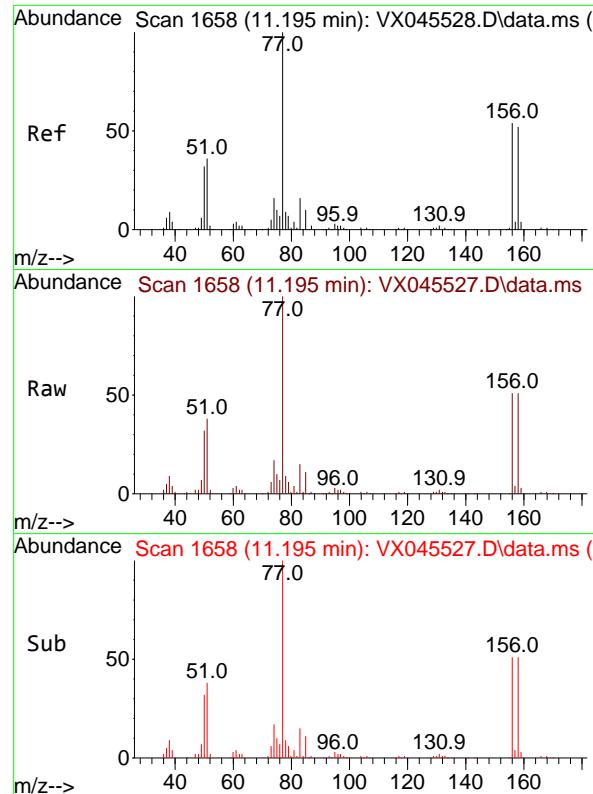

#77

Bromobenzene

Concen: 20.592 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

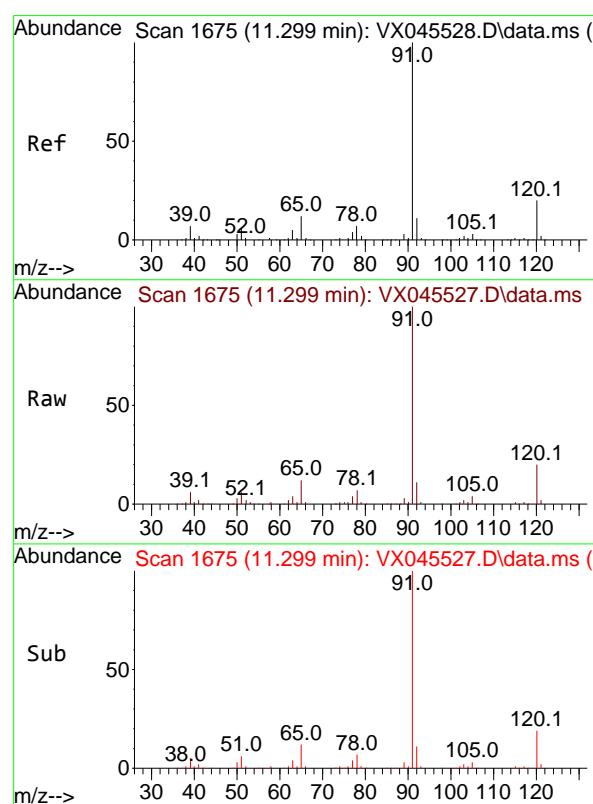

#78

n-propylbenzene

Concen: 21.729 ug/l

RT: 11.299 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52


Tgt Ion: 91 Resp: 130994

Ion Ratio Lower Upper



91 100

120 20.5 10.8 32.3

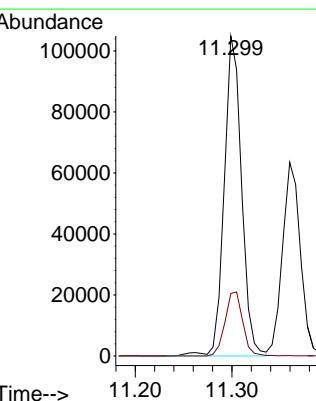




Abundance Scan 1685 (11.360 min): VX045527.D\data.ms (-)

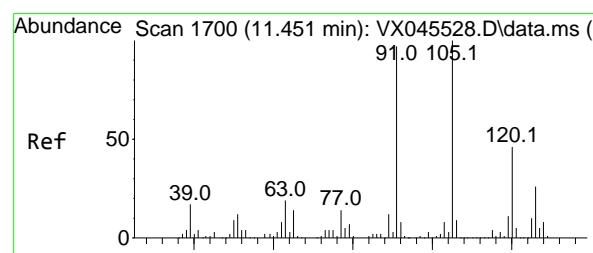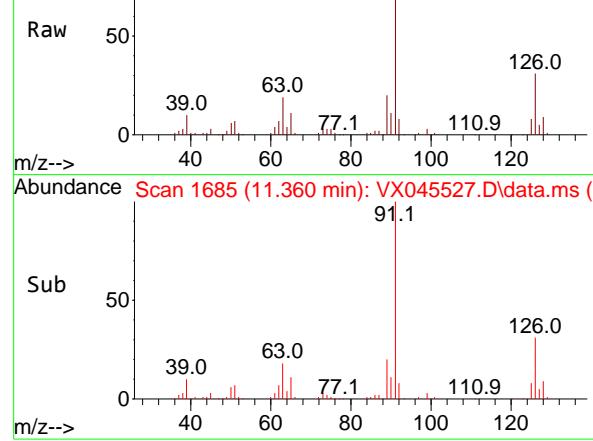

Abundance Scan 1700 (11.451 min): VX045527.D\data.ms (-)

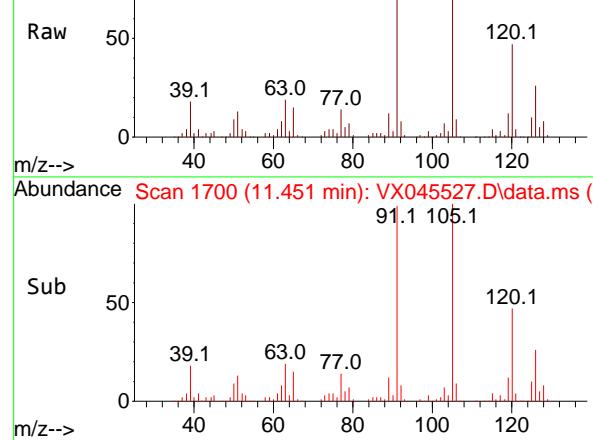

Abundance Scan 1700 (11.451 min): VX045527.D\data.ms (-)

#79

2-Chlorotoluene

Concen: 21.229 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC020

Tgt Ion: 91 Resp: 8181

Ion Ratio Lower Upper

91 100


126 30.9 15.8 47.4

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#80

1,3,5-Trimethylbenzene

Concen: 21.564 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52


Tgt Ion:105 Resp: 93328

Ion Ratio Lower Upper

105 100

120 46.5 23.0 69.0

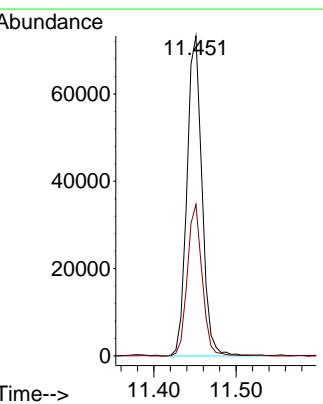


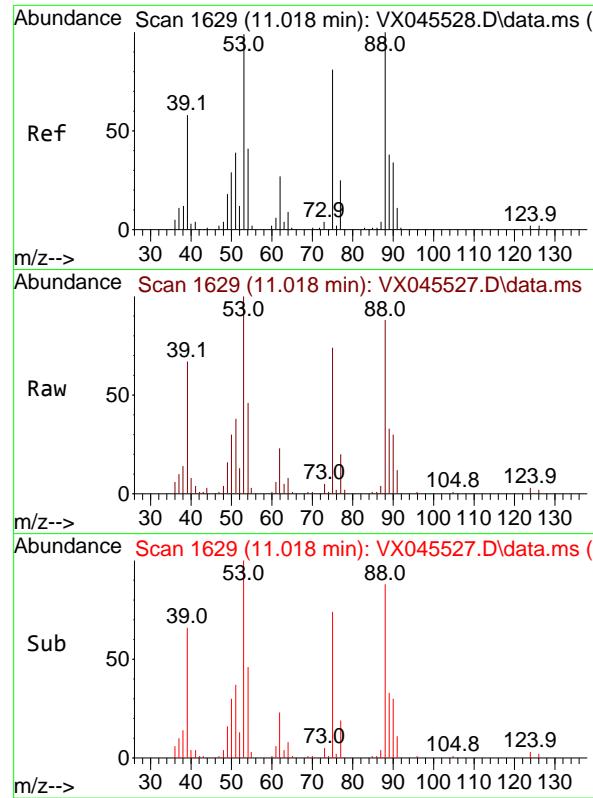


#81  
trans-1,4-Dichloro-2-butene  
Concen: 17.961 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

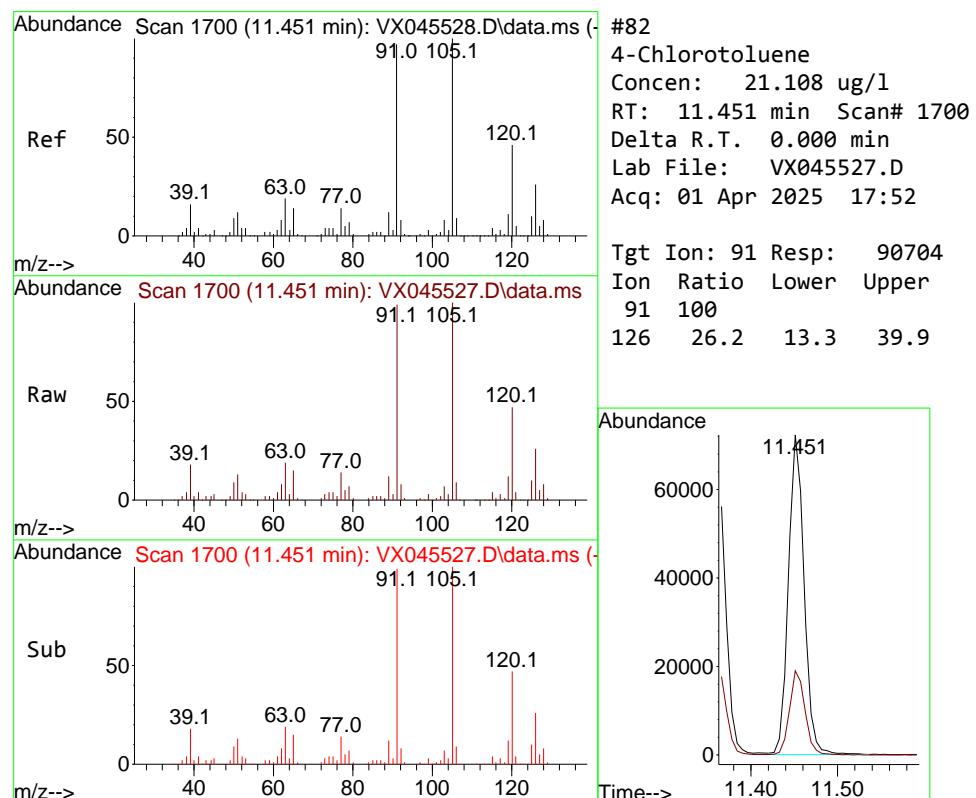

#82  
4-Chlorotoluene  
Concen: 21.108 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Tgt Ion: 91 Resp: 90704  
Ion Ratio Lower Upper  
91 100  
126 26.2 13.3 39.9





#83

tert-Butylbenzene

Concen: 20.964 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

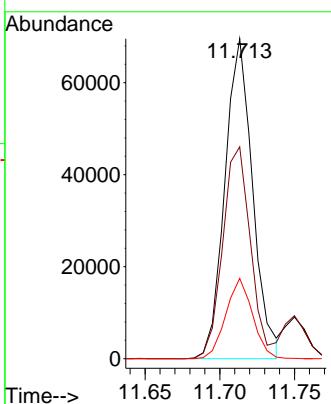

#84

1,2,4-Trimethylbenzene

Concen: 21.235 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045527.D


Acq: 01 Apr 2025 17:52




Tgt Ion:105 Resp: 92242

Ion Ratio Lower Upper

105 100

120 43.1 21.4 64.3

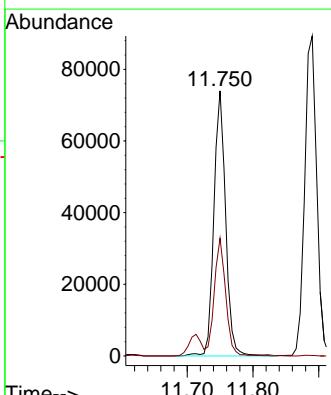



#85

sec-Butylbenzene

Concen: 21.433 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

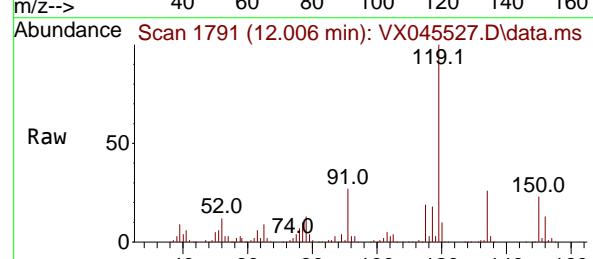

#86

p-Isopropyltoluene

Concen: 21.173 ug/l



RT: 12.006 min Scan# 1791


Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt	Ion:119	Resp:	91866
Ion	Ratio	Lower	Upper
119	100		
134	25.7	12.6	37.8
91	27.1	13.7	41.1

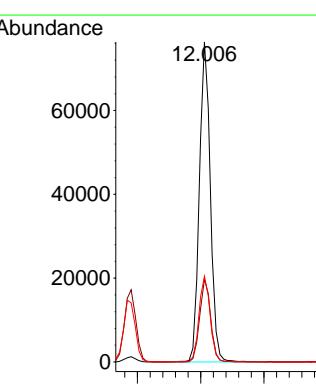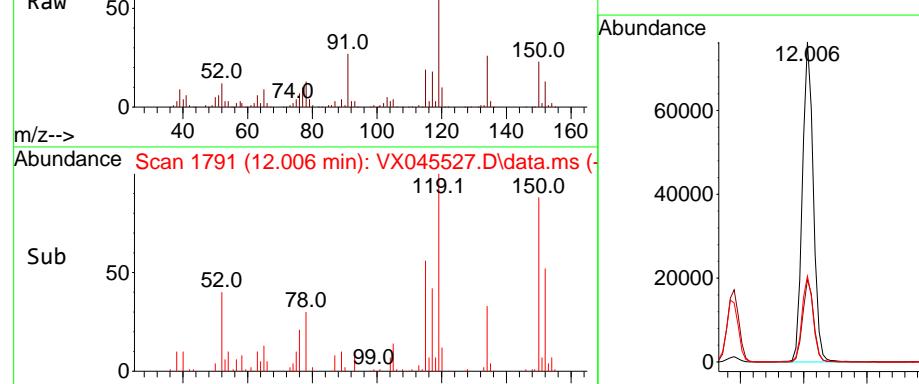

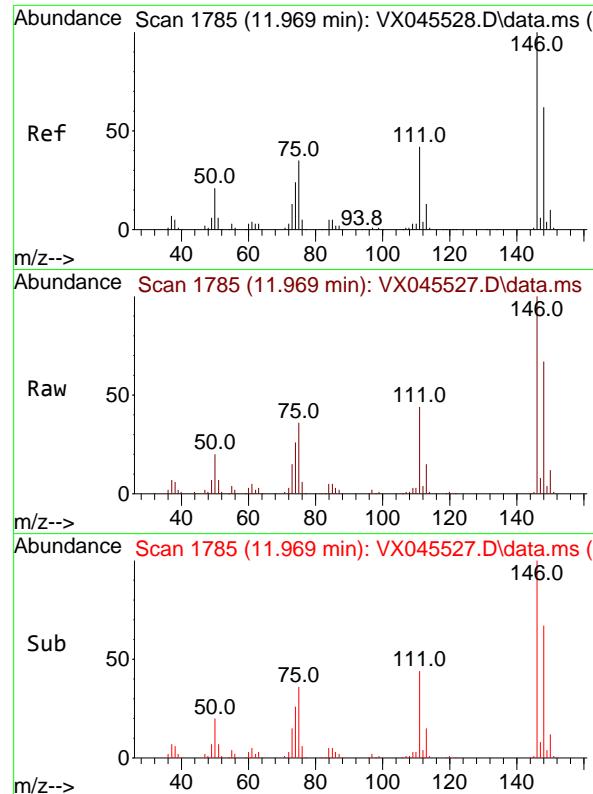

#87

1,3-Dichlorobenzene

Concen: 20.490 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

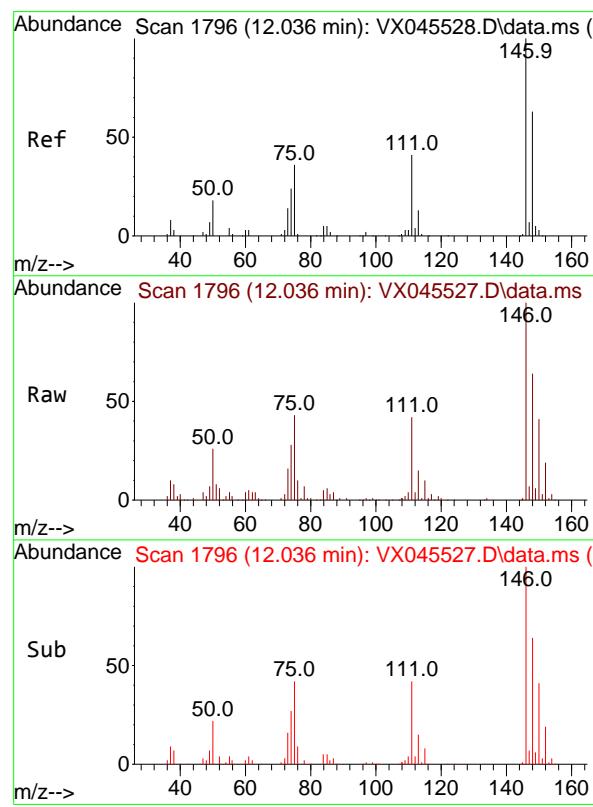

#88

1,4-Dichlorobenzene

Concen: 20.706 ug/l


RT: 12.036 min Scan# 1796




Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt	Ion:146	Resp:	46208
Ion	Ratio	Lower	Upper
146	100		
111	43.6	20.9	62.8
148	62.6	31.5	94.5





#89

n-Butylbenzene

Concen: 20.662 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52





Instrument : MSVOA\_X

ClientSampleId : VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

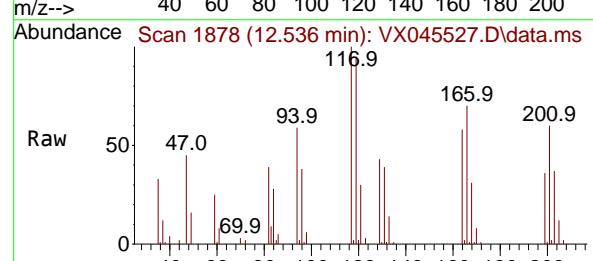

#90

Hexachloroethane

Concen: 19.505 ug/l


RT: 12.536 min Scan# 1878







Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Tgt	Ion:117	Resp:	14544
Ion	Ratio	Lower	Upper
117	100		
201	62.2	31.2	93.6

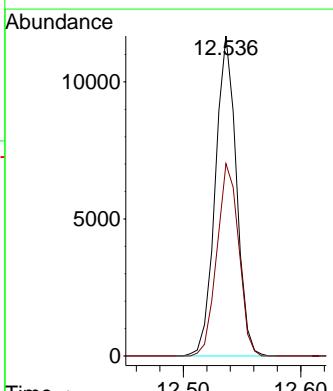



#91

1,2-Dichlorobenzene

Concen: 20.896 ug/l

RT: 12.335 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

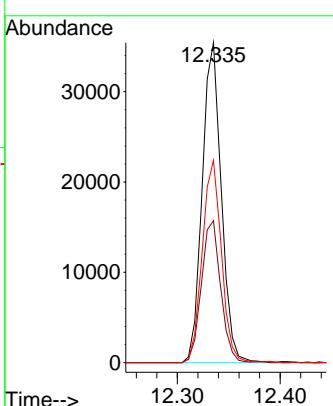

#92

1,2-Dibromo-3-Chloropropane

Concen: 21.203 ug/l

RT: 12.939 min Scan# 1944

Delta R.T. 0.000 min

Lab File: VX045527.D

Acq: 01 Apr 2025 17:52


Tgt Ion: 75 Resp: 8153


Ion Ratio Lower Upper

75 100

155 70.0 34.9 104.7

157 89.1 44.9 134.7




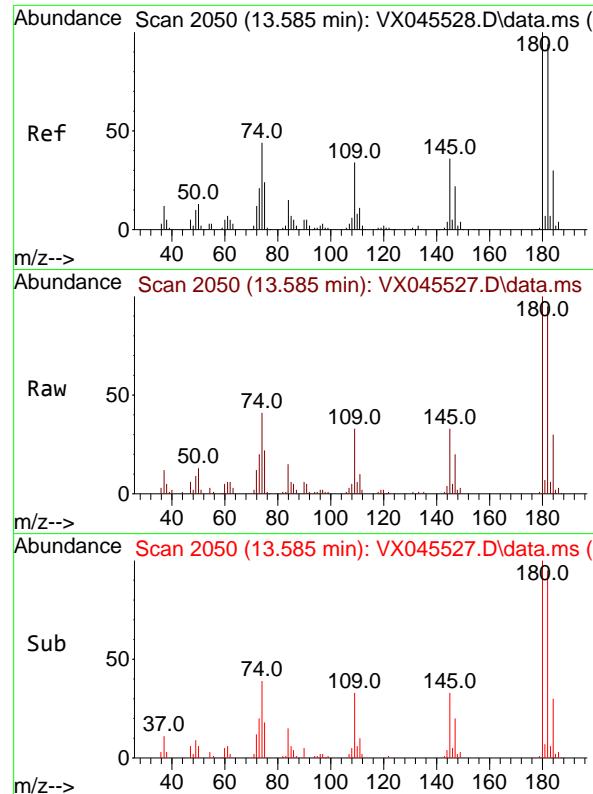


#93  
1,2,4-Trichlorobenzene  
Concen: 20.347 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

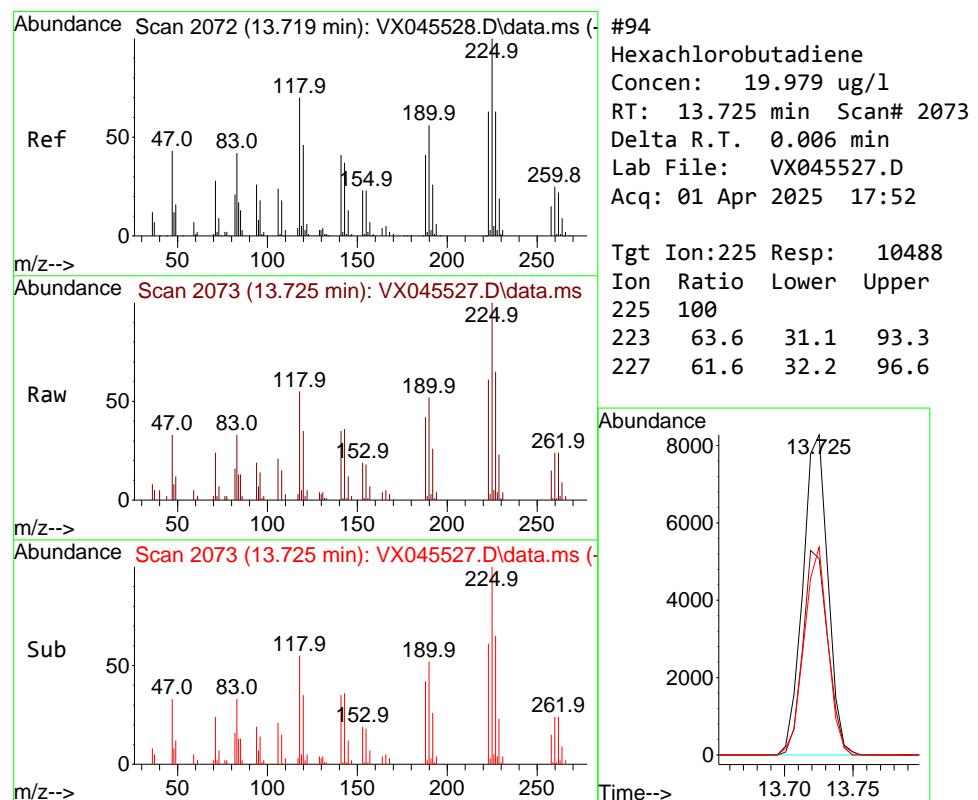

#94  
Hexachlorobutadiene  
Concen: 19.979 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. 0.006 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Tgt Ion:225 Resp: 10488  
Ion Ratio Lower Upper  
225 100  
223 63.6 31.1 93.3  
227 61.6 32.2 96.6

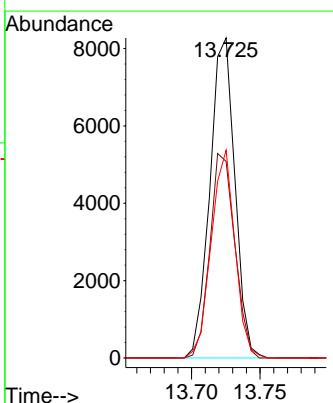


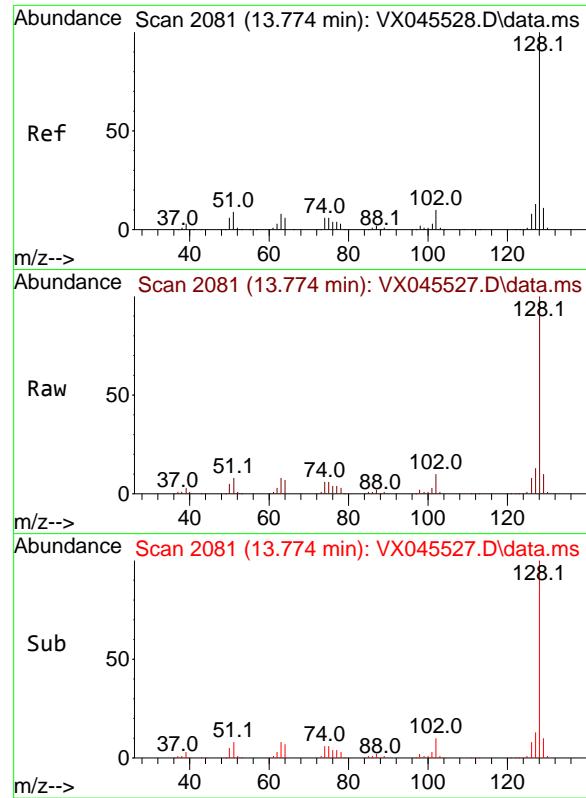


#95  
Naphthalene  
Concen: 20.928 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

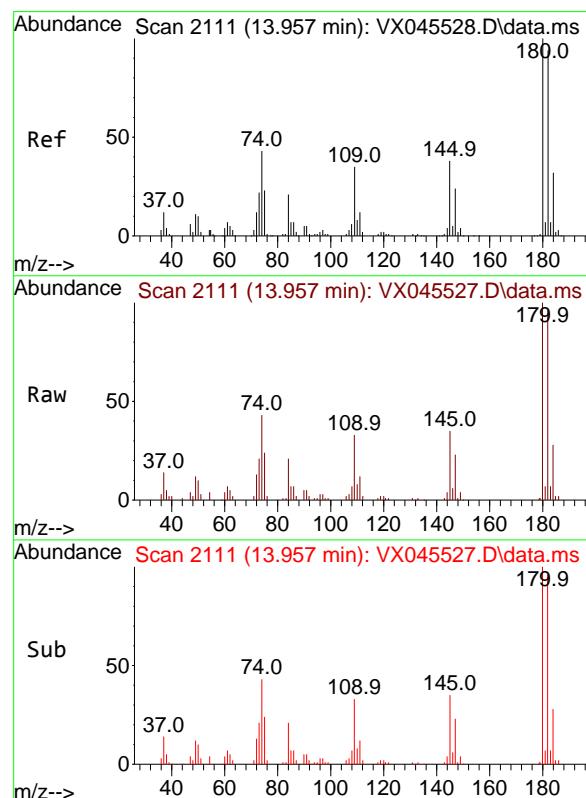

#96  
1,2,3-Trichlorobenzene  
Concen: 20.471 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045527.D  
Acq: 01 Apr 2025 17:52

Tgt Ion:180 Resp: 26113  
Ion Ratio Lower Upper  
180 100  
182 97.4 47.3 141.8  
145 36.7 18.2 54.6

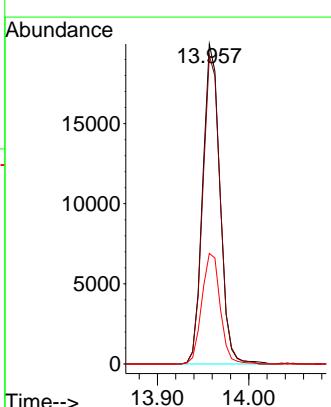

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045528.D  
 Acq On : 01 Apr 2025 18:15  
 Operator : JC/MD  
 Sample : VSTDICCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICCC050

Quant Time: Apr 02 02:53:01 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	95658	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	168287	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	150201	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	68786	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	83054	47.477	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	94.960%		
35) Dibromofluoromethane	5.379	113	58108	48.667	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.340%		
50) Toluene-d8	8.647	98	204338	49.031	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	98.060%		
62) 4-Bromofluorobenzene	11.079	95	76190	50.190	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	100.380%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	78444	54.834	ug/l	100
3) Chloromethane	1.307	50	75032	51.054	ug/l	100
4) Vinyl Chloride	1.374	62	68516	50.942	ug/l	100
5) Bromomethane	1.593	94	31584	49.526	ug/l	100
6) Chloroethane	1.666	64	38112	53.409	ug/l	100
7) Trichlorofluoromethane	1.874	101	103888	51.798	ug/l	100
8) Diethyl Ether	2.136	74	33953	50.424	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.325	101	59431	50.569	ug/l	100
10) Methyl Iodide	2.447	142	76404	52.121	ug/l	100
11) Tert butyl alcohol	2.977	59	60610	257.809	ug/l	100
12) 1,1-Dichloroethene	2.313	96	57738	50.278	ug/l	100
13) Acrolein	2.239	56	79989	247.074	ug/l	100
14) Allyl chloride	2.660	41	112085	51.441	ug/l	100
15) Acrylonitrile	3.062	53	194445	262.015	ug/l	100
16) Acetone	2.386	43	180563	251.366	ug/l	100
17) Carbon Disulfide	2.508	76	148601	52.393	ug/l	100
18) Methyl Acetate	2.703	43	82000	49.581	ug/l	100
19) Methyl tert-butyl Ether	3.111	73	202582	50.429	ug/l	100
20) Methylene Chloride	2.782	84	67855	50.457	ug/l	100
21) trans-1,2-Dichloroethene	3.087	96	59696	50.882	ug/l	100
22) Diisopropyl ether	3.764	45	219374	51.111	ug/l	100
23) Vinyl Acetate	3.721	43	998064	269.139	ug/l	100
24) 1,1-Dichloroethane	3.605	63	121348	49.992	ug/l	100
25) 2-Butanone	4.556	43	280076	266.363	ug/l	100
26) 2,2-Dichloropropane	4.471	77	81054	51.683	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	71871	50.282	ug/l	100
28) Bromochloromethane	4.897	49	57046	48.632	ug/l	100
29) Tetrahydrofuran	5.001	42	177402	260.230	ug/l	100
30) Chloroform	5.086	83	125797	50.366	ug/l	100
31) Cyclohexane	5.464	56	107407	50.052	ug/l	100
32) 1,1,1-Trichloroethane	5.379	97	106062	50.184	ug/l	100
36) 1,1-Dichloropropene	5.684	75	81607	50.620	ug/l	100
37) Ethyl Acetate	4.715	43	104896	51.632	ug/l	100
38) Carbon Tetrachloride	5.672	117	90247	51.797	ug/l	100
39) Methylcyclohexane	7.373	83	104678	52.970	ug/l	100
40) Benzene	6.031	78	249161	50.605	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045528.D  
 Acq On : 01 Apr 2025 18:15  
 Operator : JC/MD  
 Sample : VSTDICCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICCC050

Quant Time: Apr 02 02:53:01 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	59068	54.623	ug/1	100
42) 1,2-Dichloroethane	6.080	62	104601	51.437	ug/1	100
43) Isopropyl Acetate	6.336	43	164588	53.452	ug/1	100
44) Trichloroethene	7.123	130	59042	50.452	ug/1	100
45) 1,2-Dichloropropane	7.427	63	63316	51.540	ug/1	100
46) Dibromomethane	7.574	93	49125	52.092	ug/1	100
47) Bromodichloromethane	7.818	83	96176	51.068	ug/1	100
48) Methyl methacrylate	7.690	41	85483	53.768	ug/1	100
49) 1,4-Dioxane	7.659	88	31199	1084.635	ug/1	100
51) 4-Methyl-2-Pentanone	8.574	43	558029	273.375	ug/1	100
52) Toluene	8.714	92	153143	51.402	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	85462	47.317	ug/1	100
54) cis-1,3-Dichloropropene	8.366	75	95524	53.975	ug/1	100
55) 1,1,2-Trichloroethane	9.147	97	60452	50.919	ug/1	100
56) Ethyl methacrylate	9.116	69	100998	54.970	ug/1	100
57) 1,3-Dichloropropane	9.305	76	106580	51.554	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	250428	269.434	ug/1	100
59) 2-Hexanone	9.427	43	413824	273.765	ug/1	100
60) Dibromochloromethane	9.519	129	69258	53.511	ug/1	100
61) 1,2-Dibromoethane	9.604	107	62812	52.264	ug/1	100
64) Tetrachloroethene	9.269	164	52155	49.181	ug/1	100
65) Chlorobenzene	10.073	112	162829	50.733	ug/1	100
66) 1,1,1,2-Tetrachloroethane	10.159	131	55974	50.233	ug/1	100
67) Ethyl Benzene	10.189	91	301481	52.447	ug/1	100
68) m/p-Xylenes	10.299	106	218702	104.606	ug/1	100
69) o-Xylene	10.640	106	108028	52.452	ug/1	100
70) Styrene	10.653	104	182620	53.723	ug/1	100
71) Bromoform	10.799	173	44397	53.361	ug/1 #	100
73) Isopropylbenzene	10.957	105	287628	52.203	ug/1	100
74) N-amyl acetate	10.842	43	141589	53.721	ug/1	100
75) 1,1,2,2-Tetrachloroethane	11.207	83	95200	49.185	ug/1	100
76) 1,2,3-Trichloropropane	11.238	75	84279m	50.230	ug/1	
77) Bromobenzene	11.195	156	64527	50.686	ug/1	100
78) n-propylbenzene	11.299	91	336796	53.069	ug/1	100
79) 2-Chlorotoluene	11.360	91	203994	50.279	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	241536	53.013	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	25488	51.556	ug/1	100
82) 4-Chlorotoluene	11.451	91	237213	52.439	ug/1	100
83) tert-Butylbenzene	11.713	119	235715	52.256	ug/1	100
84) 1,2,4-Trimethylbenzene	11.750	105	242301	52.986	ug/1	100
85) sec-Butylbenzene	11.890	105	295799	53.391	ug/1	100
86) p-Isopropyltoluene	12.006	119	242416	53.073	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	116890	50.441	ug/1	100
88) 1,4-Dichlorobenzene	12.036	146	117164	49.871	ug/1	100
89) n-Butylbenzene	12.329	91	217345	54.874	ug/1	100
90) Hexachloroethane	12.536	117	41095	52.352	ug/1	100
91) 1,2-Dichlorobenzene	12.335	146	115426	50.099	ug/1	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	21712	53.638	ug/1	100
93) 1,2,4-Trichlorobenzene	13.585	180	65145	50.797	ug/1	100
94) Hexachlorobutadiene	13.719	225	27795	50.296	ug/1	100
95) Naphthalene	13.774	128	256009	53.643	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	68781	51.219	ug/1	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045528.D  
 Acq On : 01 Apr 2025 18:15  
 Operator : JC/MD  
 Sample : VSTDICCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDICCC050**

Quant Time: Apr 02 02:53:01 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045528.D  
 Acq On : 01 Apr 2025 18:15  
 Operator : JC/MD  
 Sample : VSTDICCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1




Quant Time: Apr 02 02:53:01 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

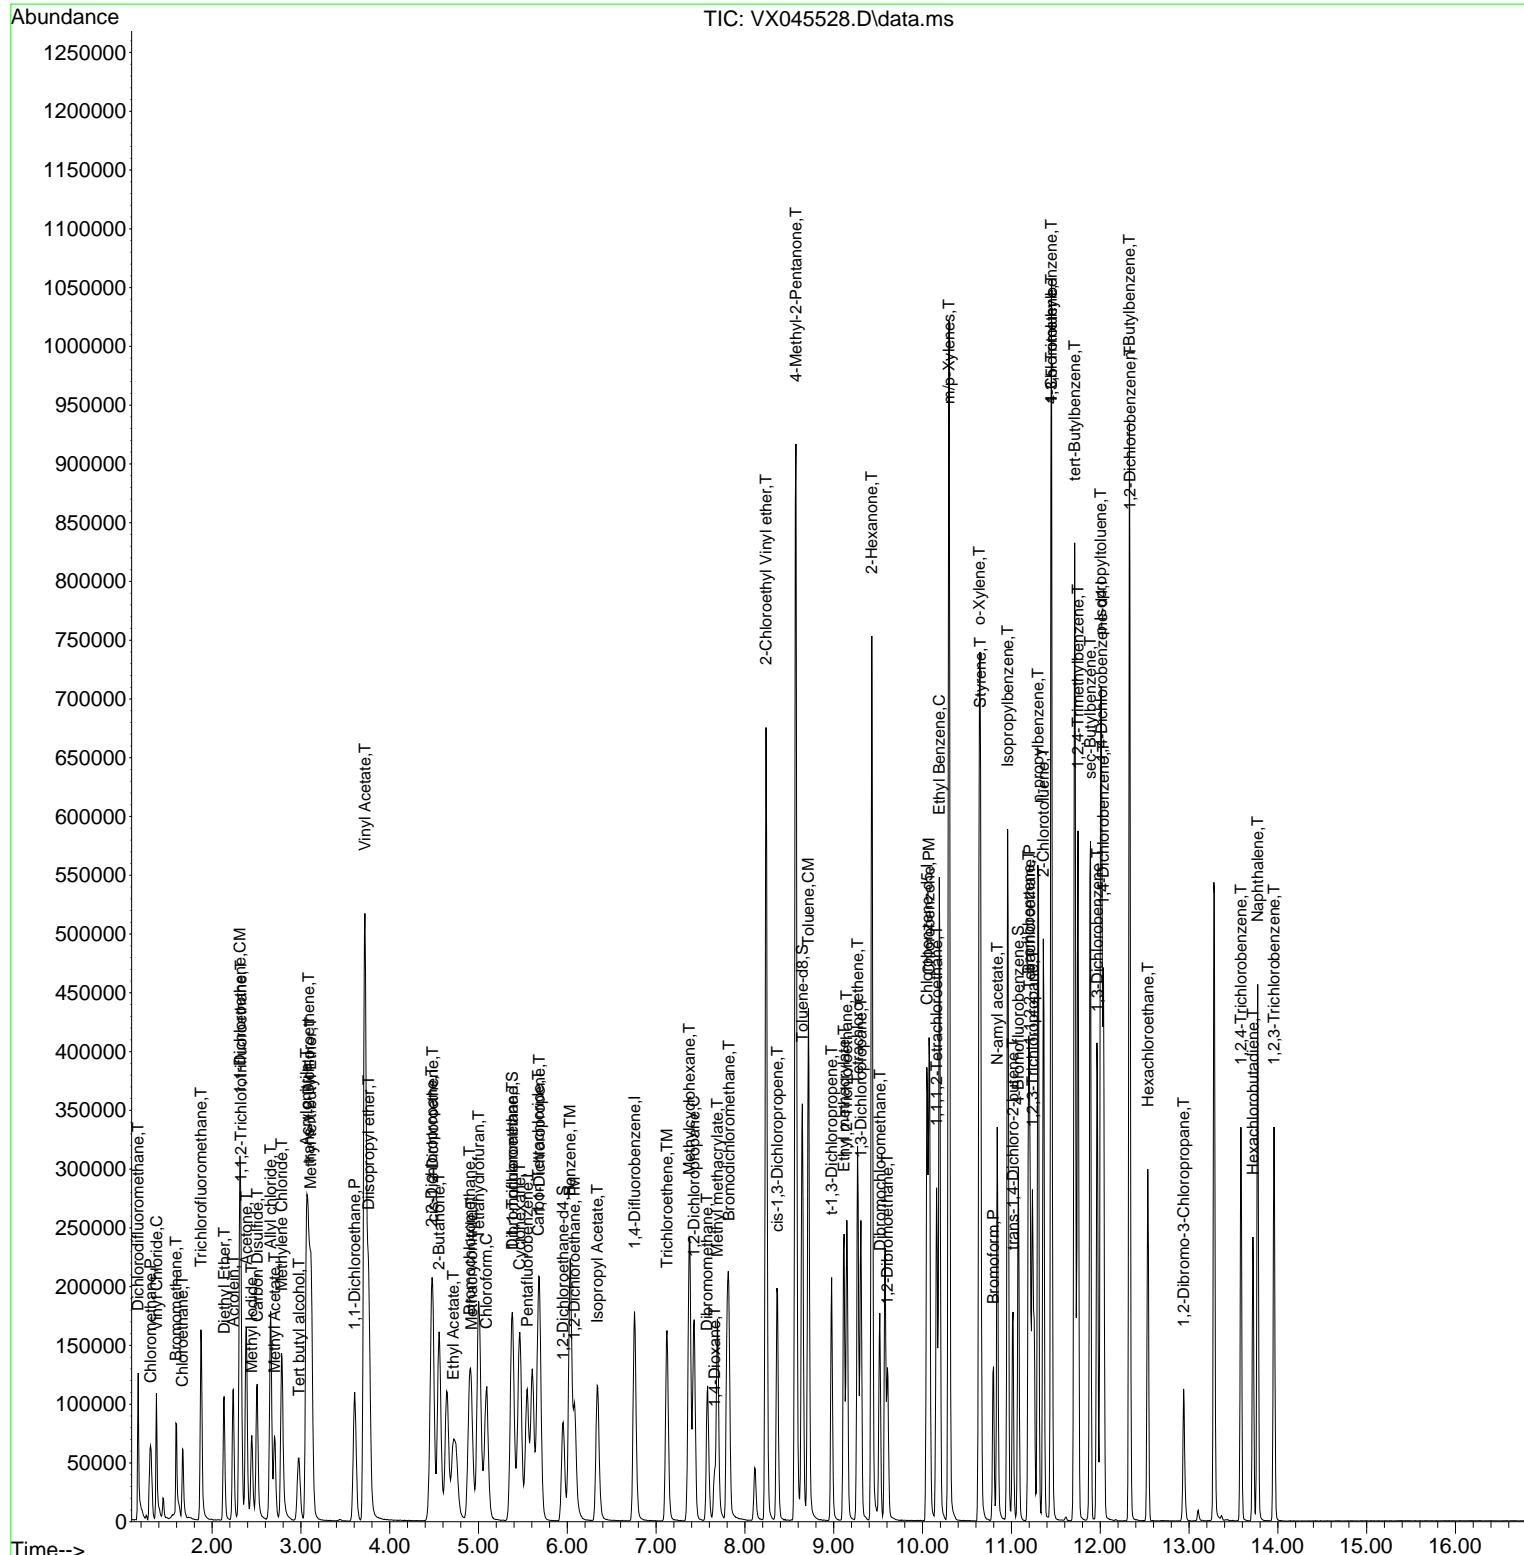



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#2

Dichlorodifluoromethane

Concen: 54.834 ug/l




RT: 1.166 min Scan# 13


Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15

Tgt Ion: 85 Resp: 78444  
 Ion Ratio Lower Upper  
 85 100  
 87 32.1 16.1 48.2

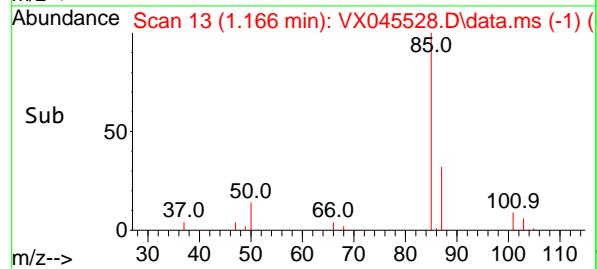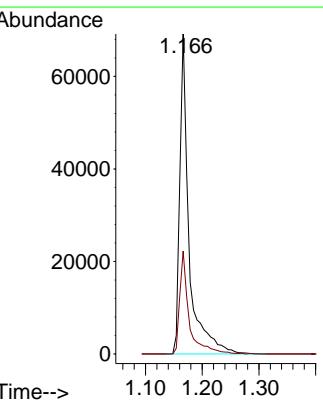



Ref Scan 36 (1.307 min): VX045528.D\data.ms

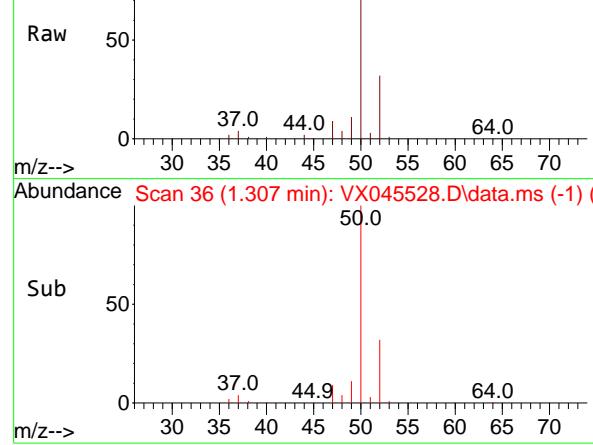

Raw Scan 36 (1.307 min): VX045528.D\data.ms

Sub Scan 36 (1.307 min): VX045528.D\data.ms (-1)

#3

Chloromethane

Concen: 51.054 ug/l

RT: 1.307 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

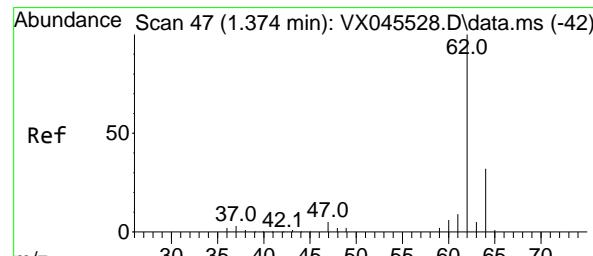

Ref Scan 47 (1.374 min): VX045528.D\data.ms

Raw Scan 47 (1.374 min): VX045528.D\data.ms

Sub Scan 47 (1.374 min): VX045528.D\data.ms (-1)

#4

Vinyl Chloride

Concen: 50.942 ug/l

RT: 1.374 min Scan# 47

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15


Tgt Ion: 62 Resp: 68516

Ion Ratio Lower Upper

62 100

64 31.9 25.5 38.3

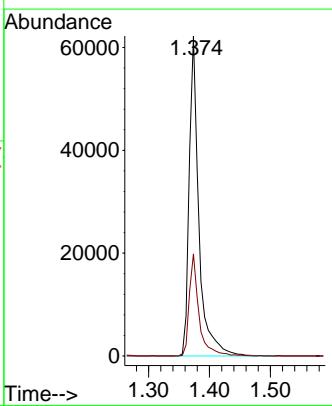


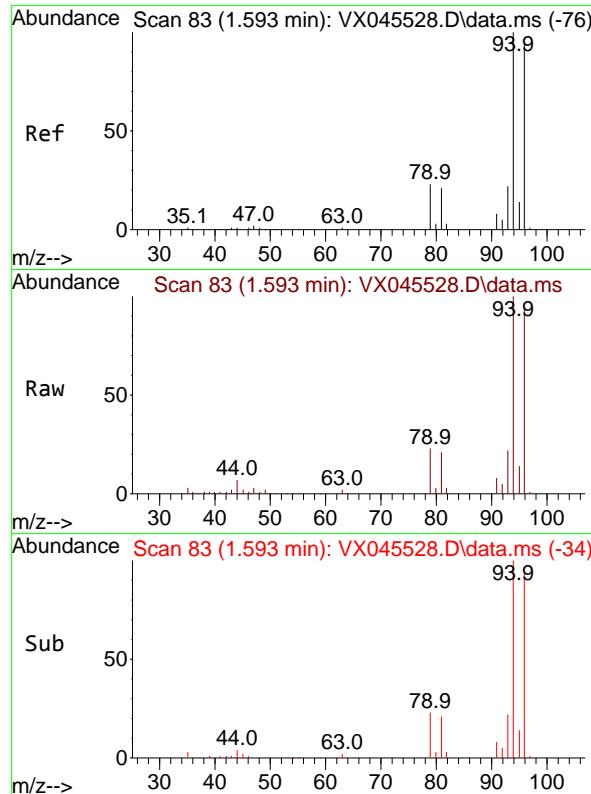


#5  
 Bromomethane  
 Concen: 49.526 ug/l  
 RT: 1.593 min Scan# 8  
 Delta R.T. 0.000 min  
 Lab File: VX045528.D  
 Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

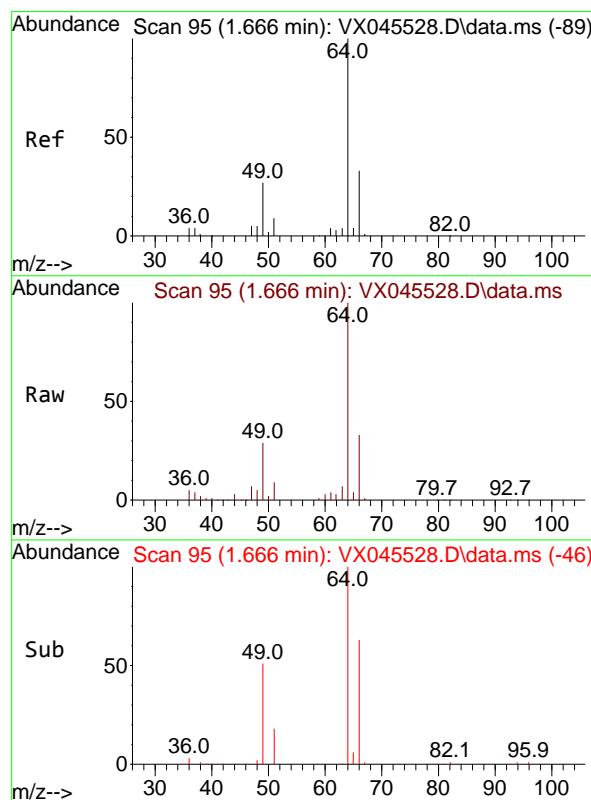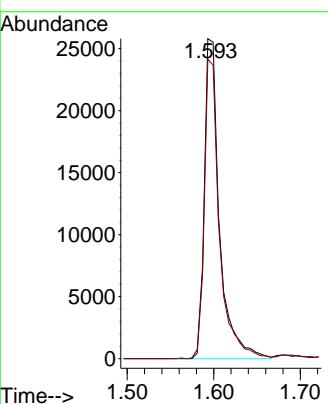

#6  
 Chloroethane  
 Concen: 53.409 ug/l  
 RT: 1.666 min Scan# 95  
 Delta R.T. 0.000 min  
 Lab File: VX045528.D  
 Acq: 01 Apr 2025 18:15

Tgt Ion: 64 Resp: 38112  
 Ion Ratio Lower Upper  
 64 100  
 66 32.9 26.3 39.5

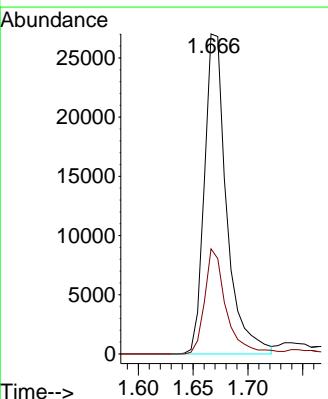


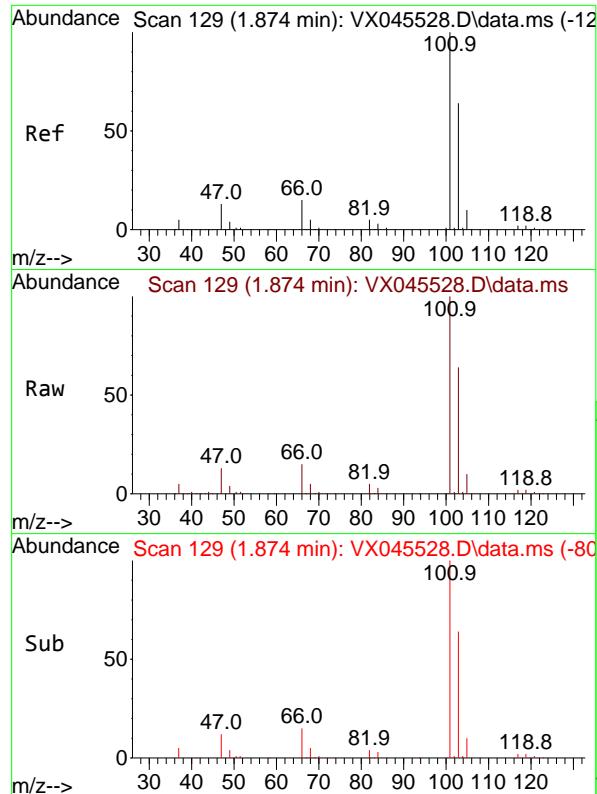


#7  
Trichlorofluoromethane  
Concen: 51.798 ug/l  
RT: 1.874 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

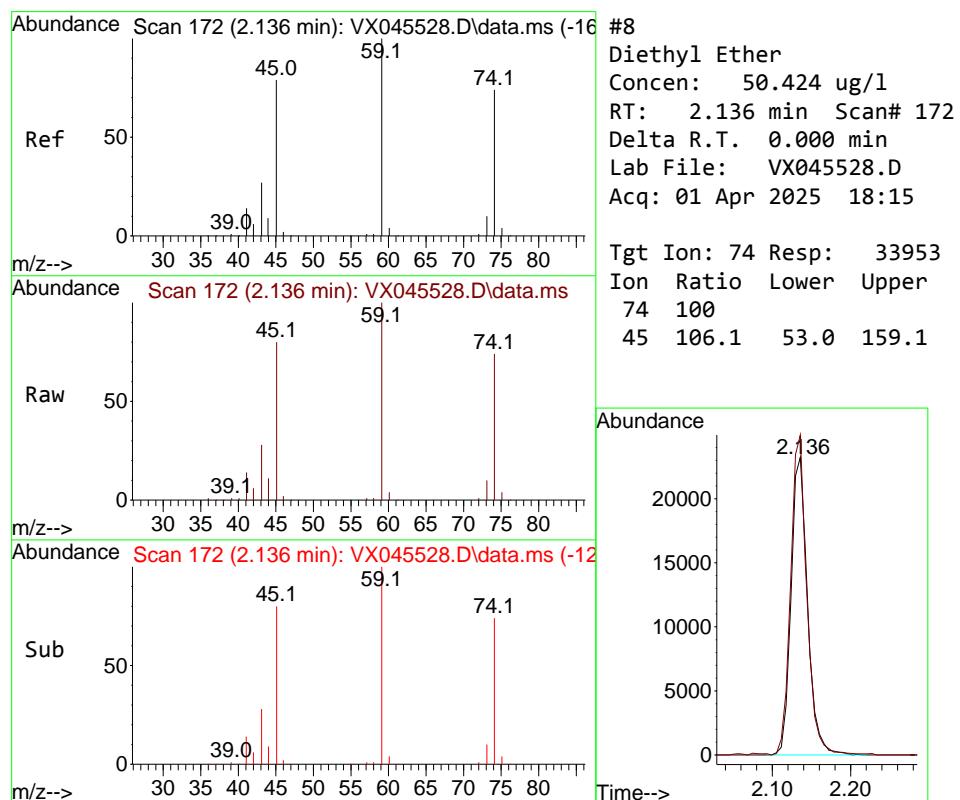

#8  
Diethyl Ether  
Concen: 50.424 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion: 74 Resp: 33953  
Ion Ratio Lower Upper  
74 100  
45 106.1 53.0 159.1

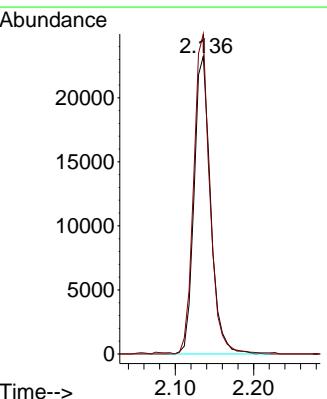

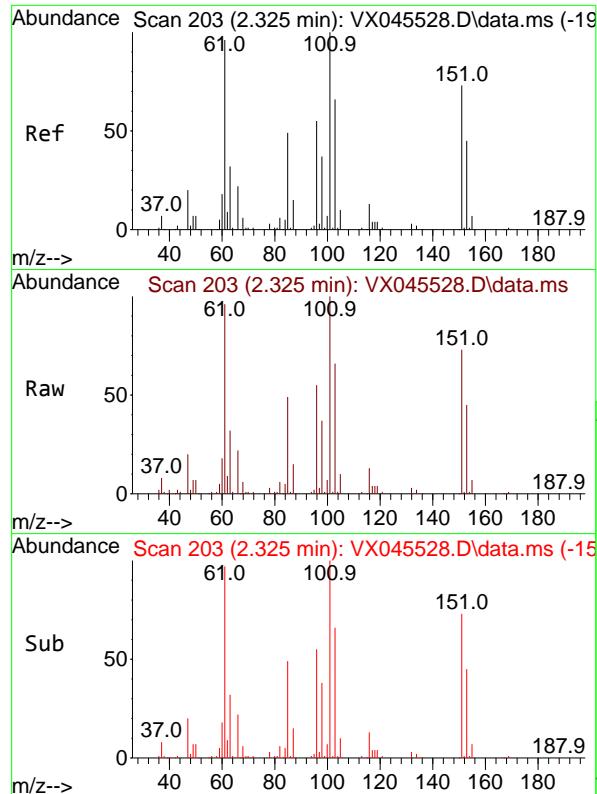


#9  
 1,1,2-Trichlorotrifluoroethane  
 Concen: 50.569 ug/l  
 RT: 2.325 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: VX045528.D  
 Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**




Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

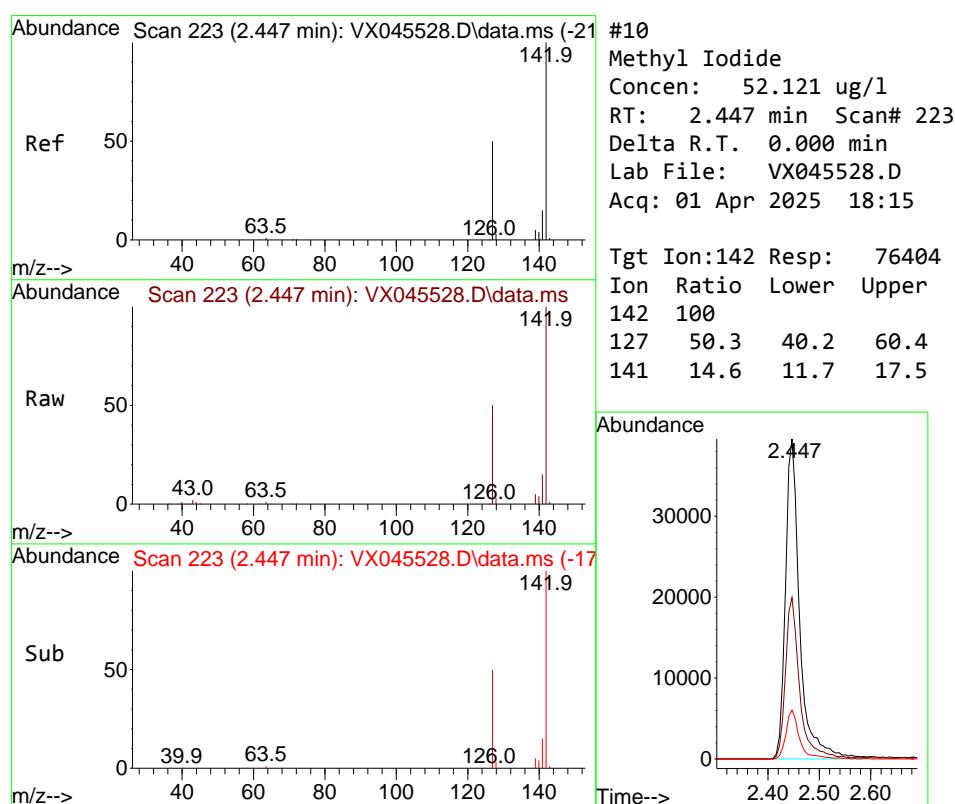

#10  
 Methyl Iodide  
 Concen: 52.121 ug/l  
 RT: 2.447 min Scan# 223  
 Delta R.T. 0.000 min  
 Lab File: VX045528.D  
 Acq: 01 Apr 2025 18:15

Tgt Ion:142 Resp: 76404  
 Ion Ratio Lower Upper  
 142 100  
 127 50.3 40.2 60.4  
 141 14.6 11.7 17.5

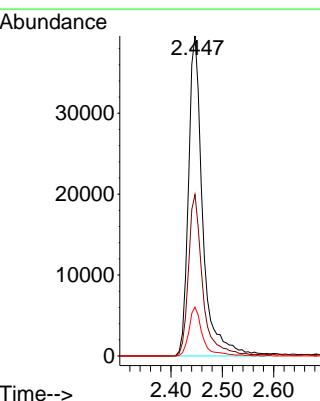



#11

Tert butyl alcohol

Concen: 257.809 ug/l

RT: 2.977 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

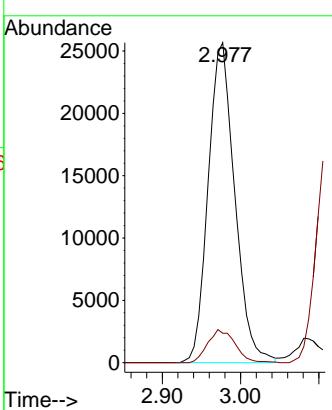

#12

1,1-Dichloroethene

Concen: 50.278 ug/l

RT: 2.313 min Scan# 201


Delta R.T. 0.000 min


Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion: 96 Resp: 57738

Ion	Ratio	Lower	Upper
96	100		
61	182.1	145.7	218.5
98	64.5	51.6	77.4

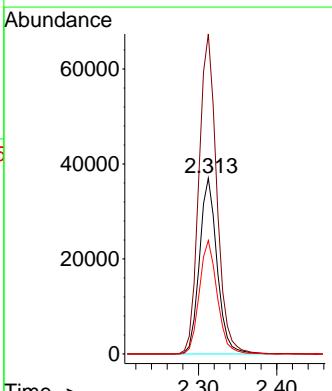



#13

Acrolein

Concen: 247.074 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15


Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050

Abundance Scan 189 (2.239 min): VX045528.D\data.ms

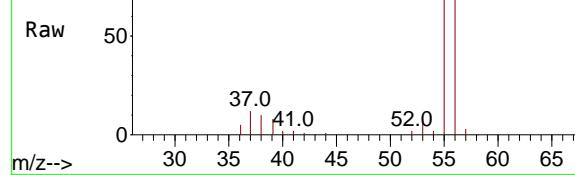

Abundance Scan 189 (2.239 min): VX045528.D\data.ms (-14)

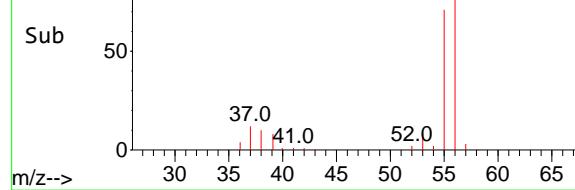

Tgt Ion: 56 Resp: 79989

Ion Ratio Lower Upper


56 100

55 70.2 56.2 84.2


**Manual Integrations****APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

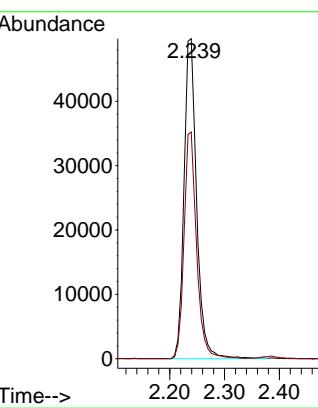

Abundance Scan 258 (2.660 min): VX045528.D\data.ms (-24)

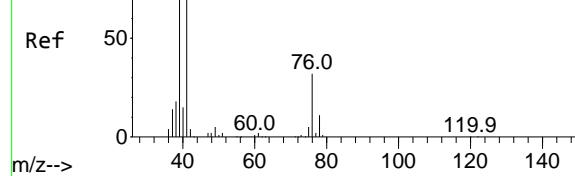

#14

Allyl chloride

Concen: 51.441 ug/l

RT: 2.660 min Scan# 258

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion: 41 Resp: 112085


Ion Ratio Lower Upper

41 100


39 75.2 60.2 90.2

76 30.7 24.6 36.8


Abundance Scan 258 (2.660 min): VX045528.D\data.ms



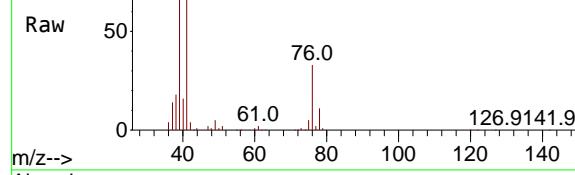


Abundance

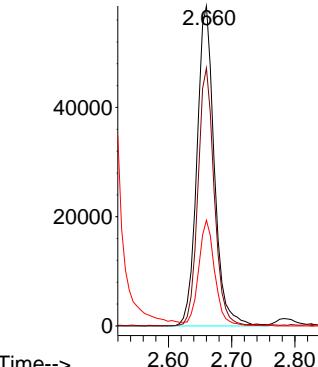

Abundance Scan 258 (2.660 min): VX045528.D\data.ms (-20)

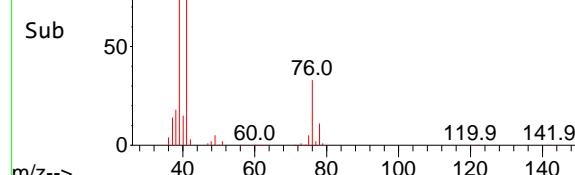



#15

Acrylonitrile

Concen: 262.015 ug/l

RT: 3.062 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

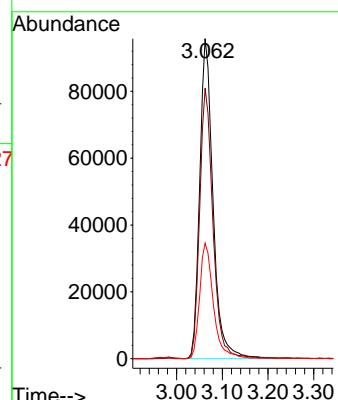

#16

Acetone

Concen: 251.366 ug/l


RT: 2.386 min Scan# 213




Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt	Ion	Resp:	
Ion	Ratio	Lower	Upper
43	100		
58	27.9	22.3	33.5

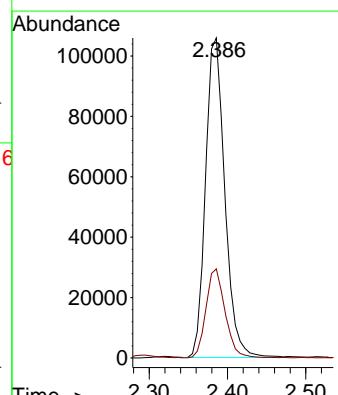



#17

Carbon Disulfide

Concen: 52.393 ug/l

RT: 2.508 min Scan# 233

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

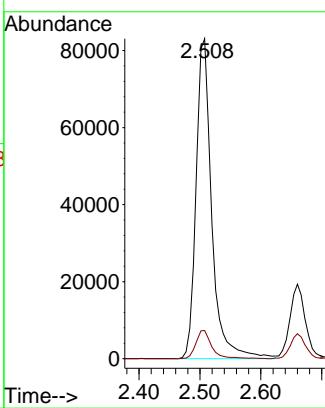

#18

Methyl Acetate

Concen: 49.581 ug/l


RT: 2.703 min Scan# 265







Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion: 43 Resp: 82000  
 Ion Ratio Lower Upper  
 43 100  
 74 21.9 17.5 26.3

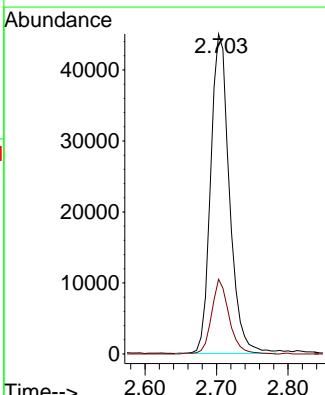

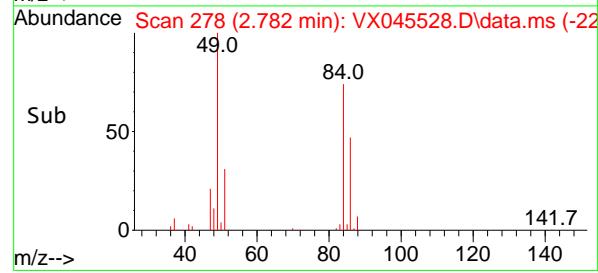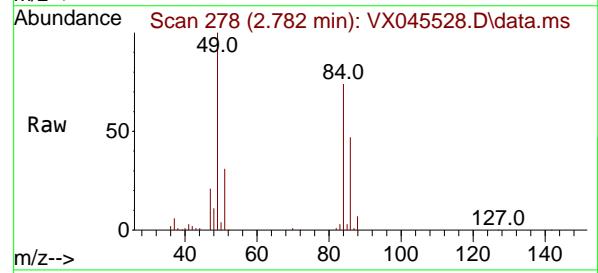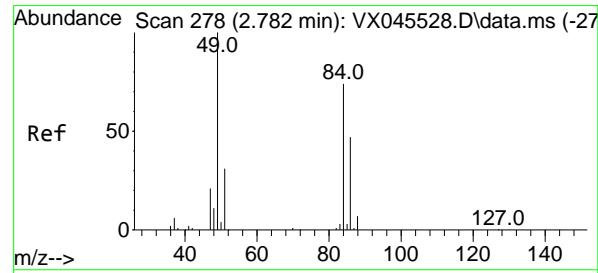


#19

Methyl tert-butyl Ether  
Concen: 50.429 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025




#20



Methylene Chloride  
Concen: 50.457 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt	Ion:	84	Resp:	67855
Ion	Ratio	Lower	Upper	
84	100			
49	134.4	107.5	161.3	
51	41.3	33.0	49.6	
86	62.6	50.1	75.1	


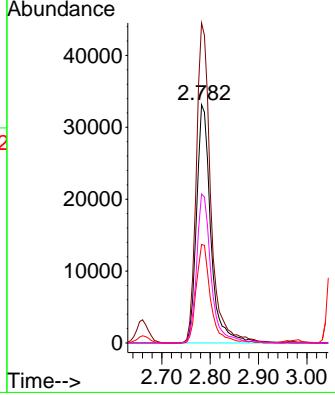


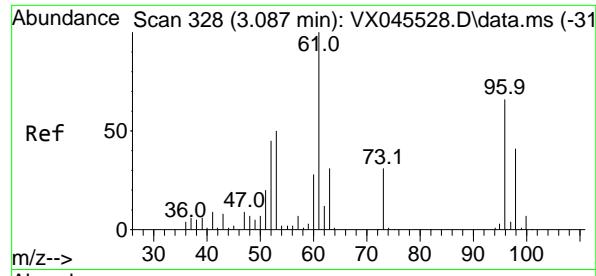

Abundance Scan 328 (3.087 min): VX045528.D\data.ms

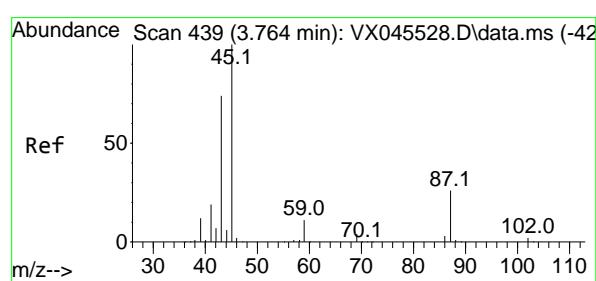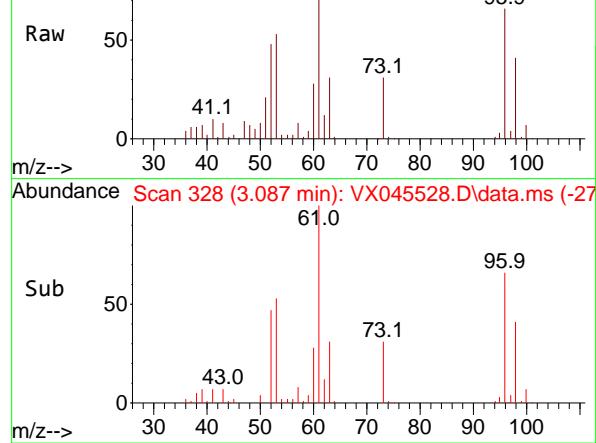

Abundance Scan 439 (3.764 min): VX045528.D\data.ms

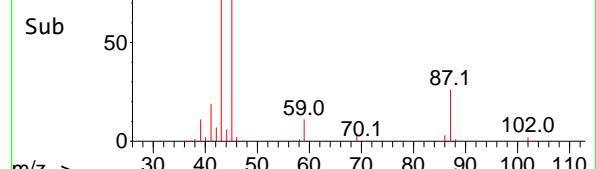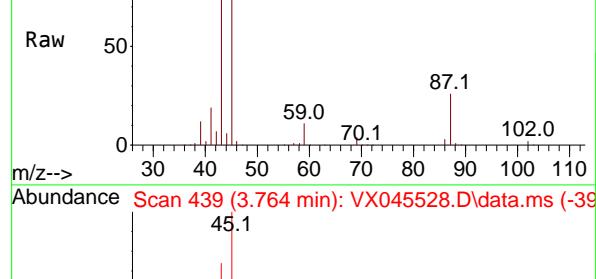

#21

trans-1,2-Dichloroethene

Concen: 50.882 ug/l

RT: 3.087 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#22

Diisopropyl ether

Concen: 51.111 ug/l

RT: 3.764 min Scan# 439

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion: 45 Resp: 219374


Ion Ratio Lower Upper


45 100

43 74.1 59.3 88.9

87 25.5 20.4 30.6

59 11.3 9.0 13.6

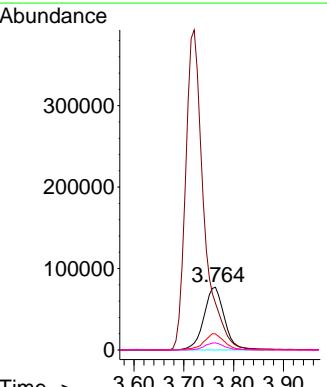

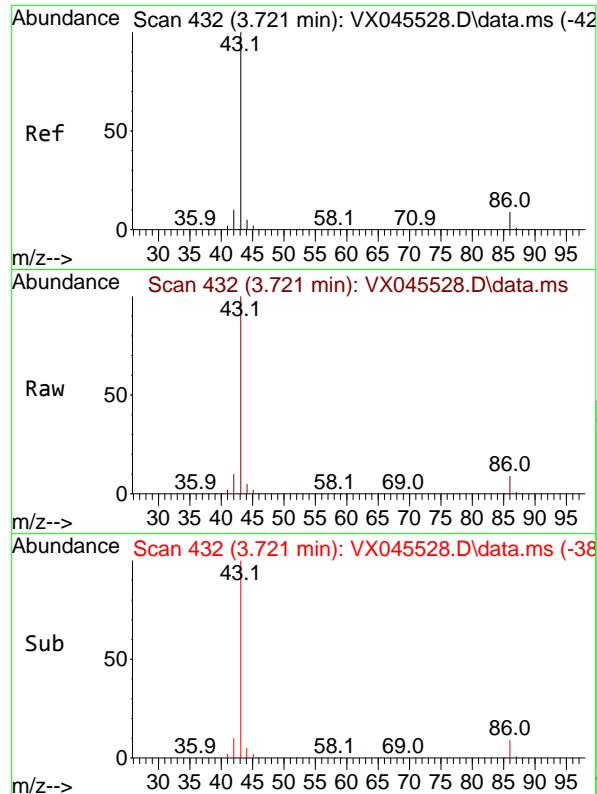

#23

Vinyl Acetate

Concen: 269.139 ug/l

RT: 3.721 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

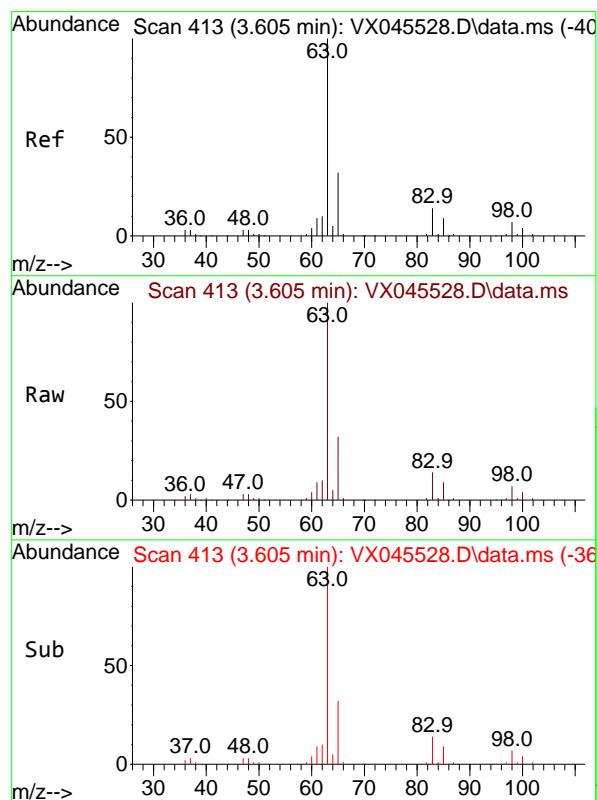

#24

1,1-Dichloroethane

Concen: 49.992 ug/l


RT: 3.605 min Scan# 413


Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15

Tgt Ion: 63 Resp: 121348  
 Ion Ratio Lower Upper  
 63 100  
 98 6.7 3.4 10.1  
 100 4.4 2.2 6.6

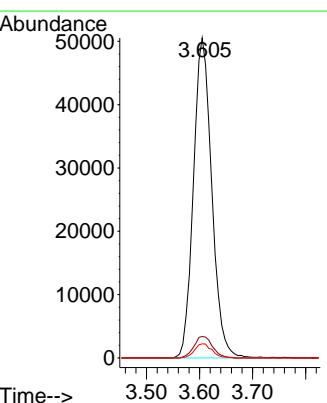




Abundance Scan 569 (4.556 min): VX045528.D\data.ms

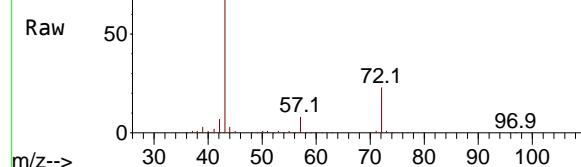

Abundance Scan 569 (4.556 min): VX045528.D\data.ms (-52)

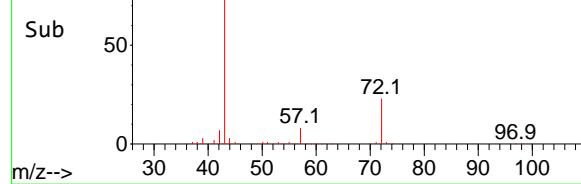

#25

2-Butanone

Concen: 266.363 ug/l

RT: 4.556 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICCC050


**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025


Supervised By :Mahesh Dadoda 04/02/2025

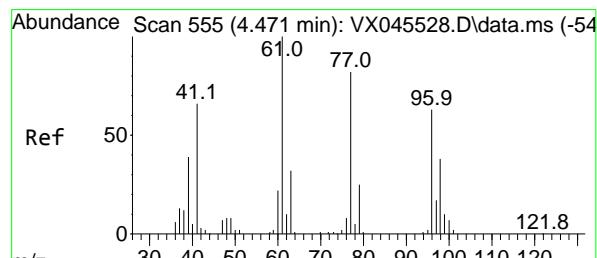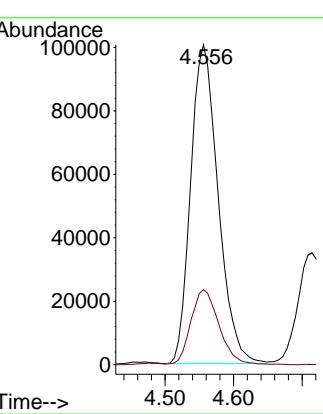

Abundance Scan 555 (4.471 min): VX045528.D\data.ms

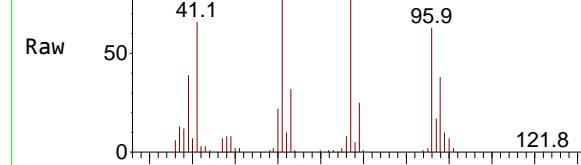

Abundance Scan 555 (4.471 min): VX045528.D\data.ms (-50)

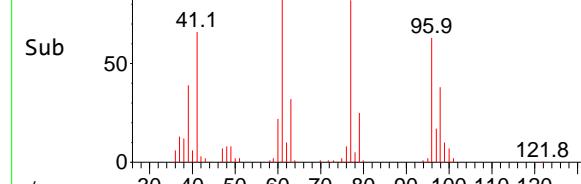

#26

2,2-Dichloropropane

Concen: 51.683 ug/l


RT: 4.471 min Scan# 555




Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion: 77 Resp: 81054  
Ion Ratio Lower Upper  
77 100  
97 21.2 10.6 31.8

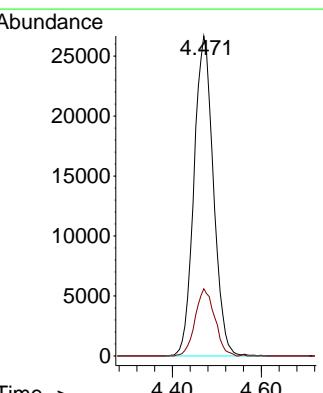


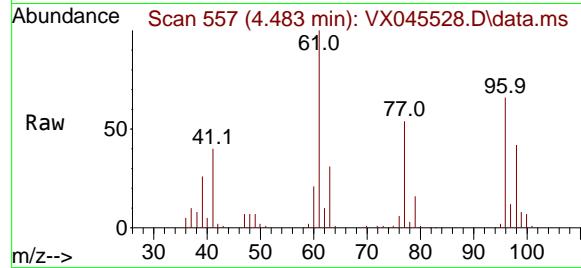



#27  
cis-1,2-Dichloroethene  
Concen: 50.282 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050



### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

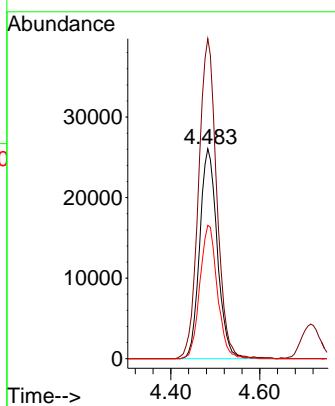

#28  
Bromochloromethane  
Concen: 48.632 ug/l  
RT: 4.897 min Scan# 625  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion: 49 Resp: 57046  
Ion Ratio Lower Upper  
49 100  
129 1.9 0.0 3.8  
130 68.2 54.6 81.8

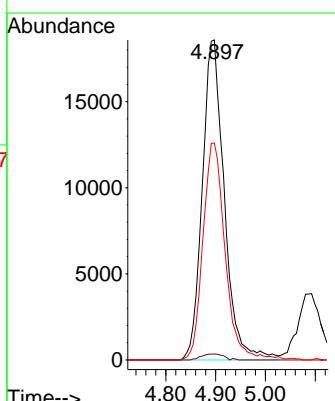

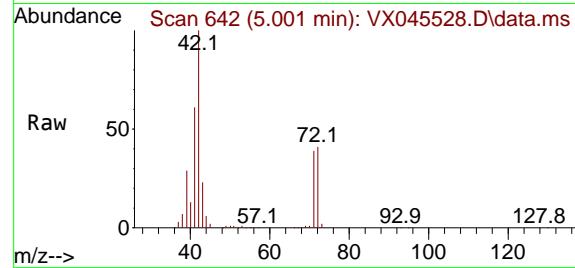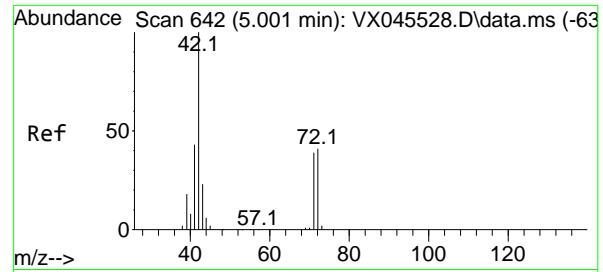

#29

Tetrahydrofuran

Concen: 260.230 ug/l

RT: 5.001 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

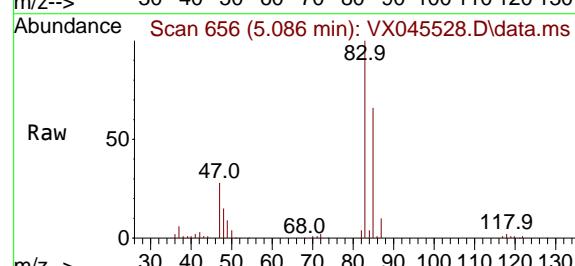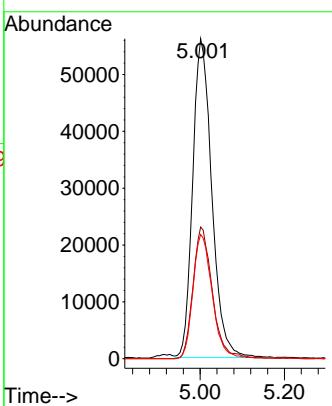

#30

Chloroform

Concen: 50.366 ug/l


RT: 5.086 min Scan# 656


Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15

Tgt Ion: 83 Resp: 125797  
 Ion Ratio Lower Upper  
 83 100  
 85 66.0 52.8 79.2

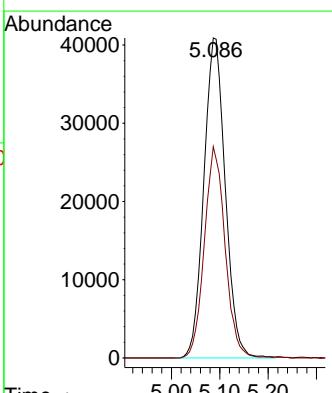



Abundance Scan 718 (5.464 min): VX045528.D\data.ms

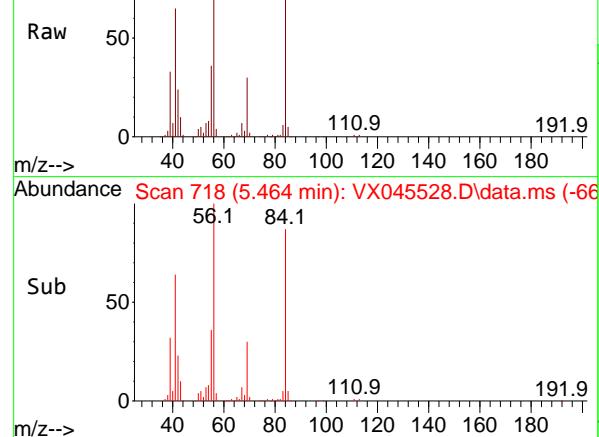

Abundance Scan 718 (5.464 min): VX045528.D\data.ms (-66)

#31

Cyclohexane

Concen: 50.052 ug/l

RT: 5.464 min Scan# 718

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050


**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

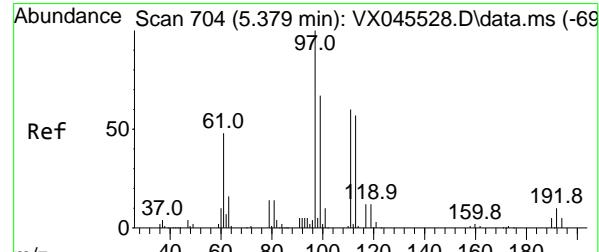

Abundance Scan 704 (5.379 min): VX045528.D\data.ms

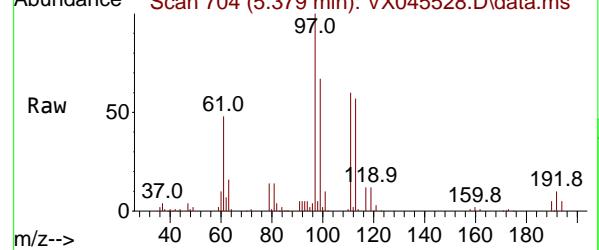

Abundance Scan 704 (5.379 min): VX045528.D\data.ms (-65)

#32

1,1,1-Trichloroethane

Concen: 50.184 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15


Tgt Ion: 97 Resp: 106062







Ion Ratio Lower Upper

97 100

99 64.6 51.7 77.5

61 51.2 41.0 61.4

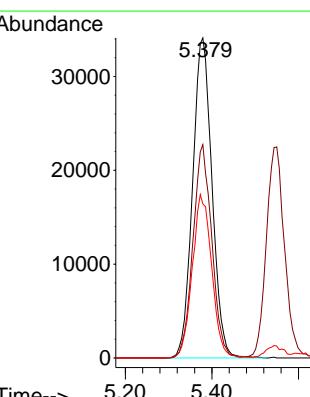

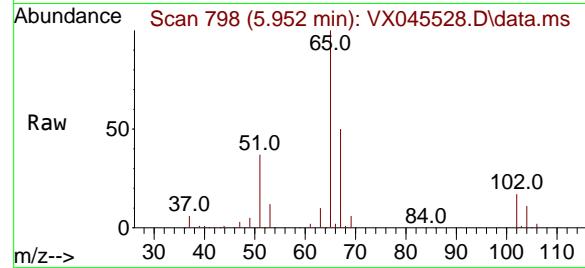

#33

1,2-Dichloroethane-d4

Concen: 47.477 ug/l

RT: 5.952 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICCC050

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025




Supervised By :Mahesh Dadoda 04/02/2025



#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 930  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion:114 Resp: 168287  
Ion Ratio Lower Upper  
114 100  
63 23.4 0.0 46.8  
88 17.7 0.0 35.4

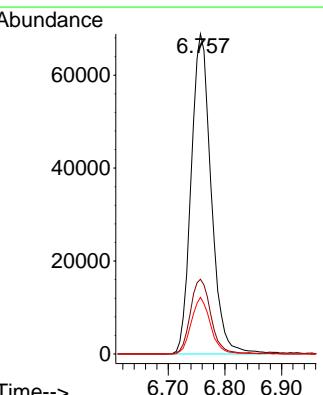

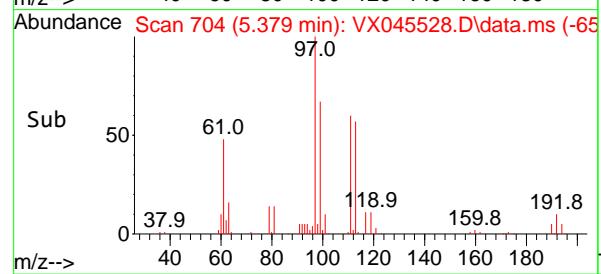

#35

Dibromofluoromethane

Concen: 48.667 ug/l

RT: 5.379 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

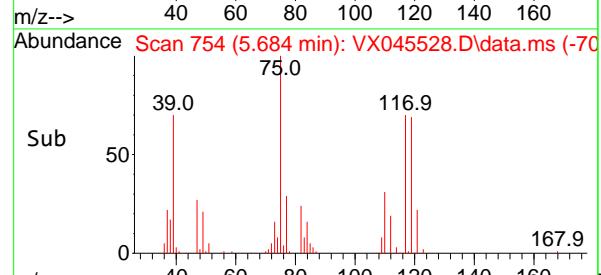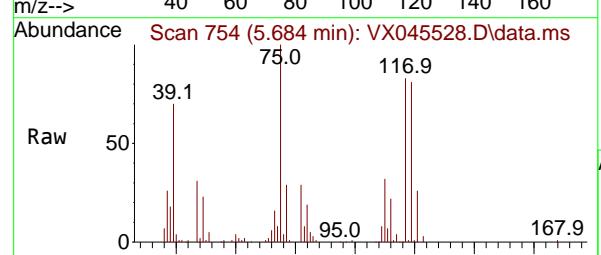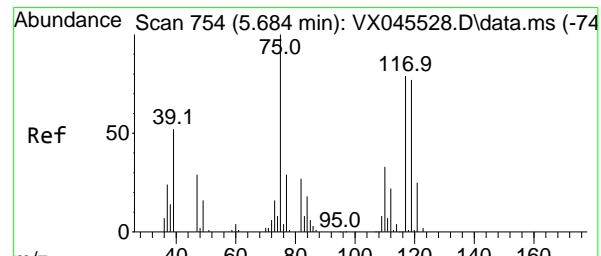

#36

1,1-Dichloropropene

Concen: 50.620 ug/l

RT: 5.684 min Scan# 754

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15



Tgt Ion: 75 Resp: 81607




Ion Ratio Lower Upper

75 100

110 33.7 16.9 50.6

77 31.2 25.0 37.4

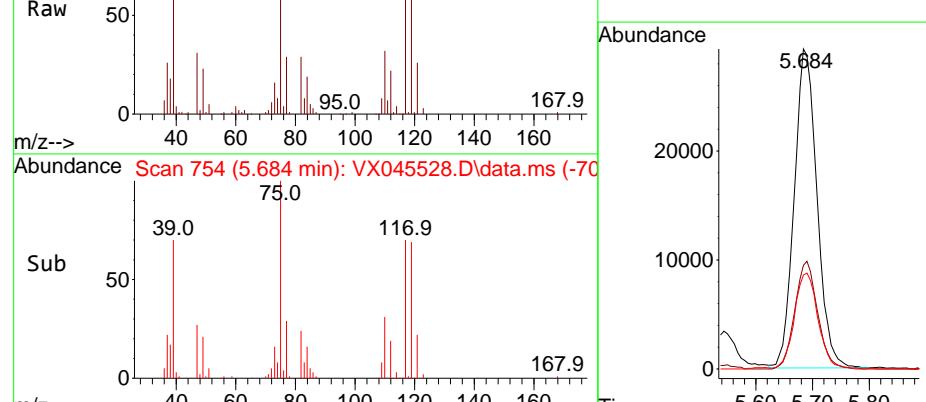

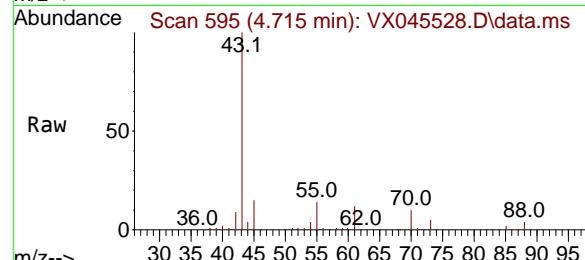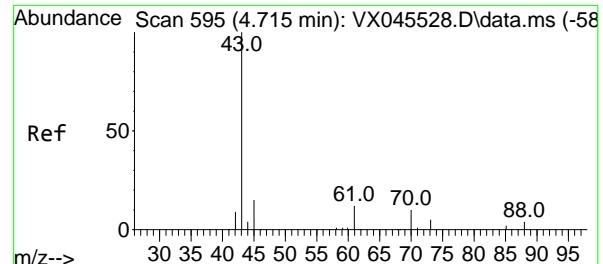

#37

**Ethyl Acetate**

Concen: 51.632 ug/l

RT: 4.715 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

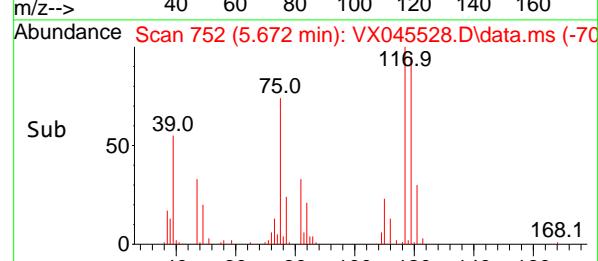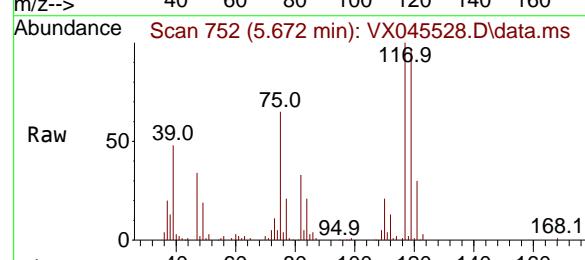

#38

**Carbon Tetrachloride**

Concen: 51.797 ug/l


RT: 5.672 min Scan# 752


Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion:117 Resp: 90247  
 Ion Ratio Lower Upper  
 117 100  
 119 96.1 76.9 115.3  
 121 30.2 24.2 36.2

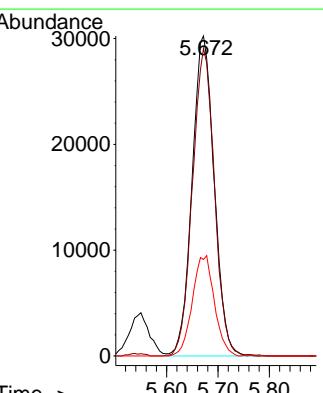

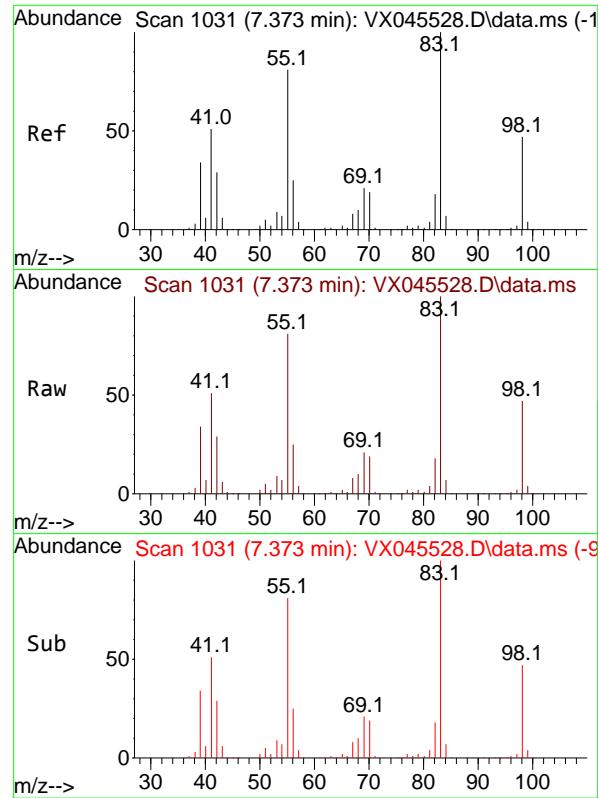

#39

Methylcyclohexane

Concen: 52.970 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICCC050

Tgt Ion: 83 Resp: 104673

Ion Ratio Lower Upper

83 100

55 81.1 64.9 97.3



98 46.7 37.4 56.0




Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

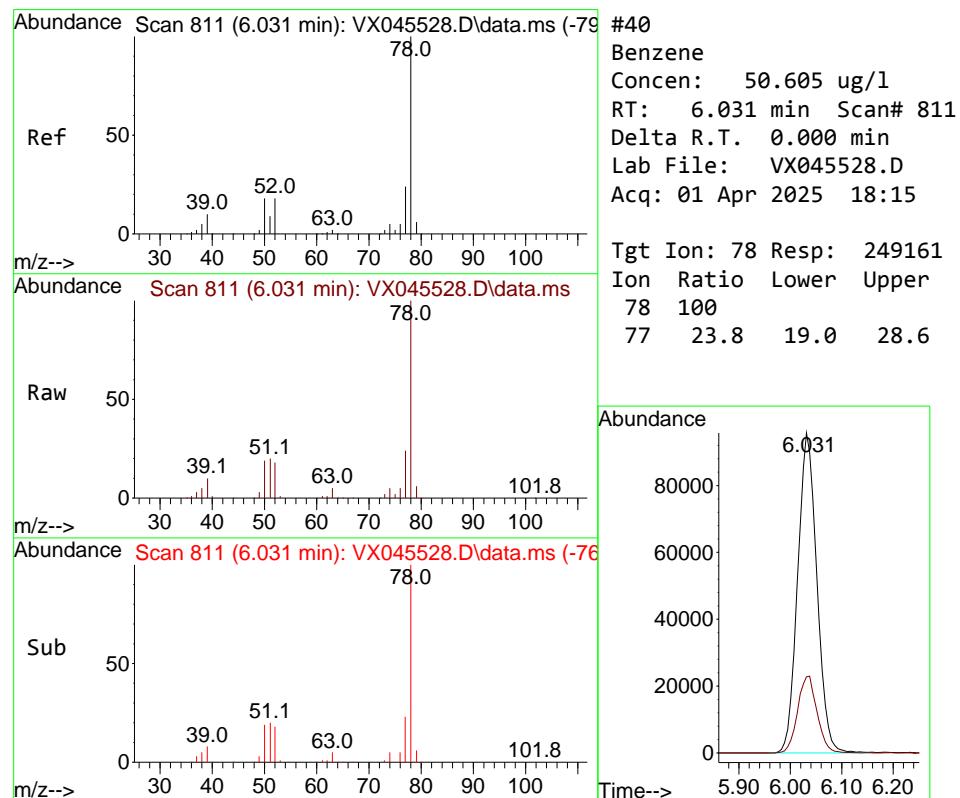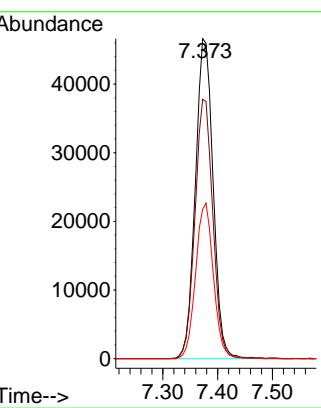



#41

Methacrylonitrile

Concen: 54.623 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15




Instrument : MSVOA\_X

ClientSampleId : VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#42

1,2-Dichloroethane

Concen: 51.437 ug/l

RT: 6.080 min Scan# 819

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15




Tgt Ion: 62 Resp: 104601

Ion Ratio Lower Upper

62 100

98 7.6 0.0 15.2

Abundance

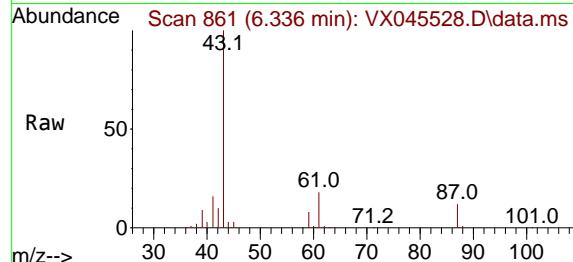

#43

Isopropyl Acetate

Concen: 53.452 ug/l

RT: 6.336 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

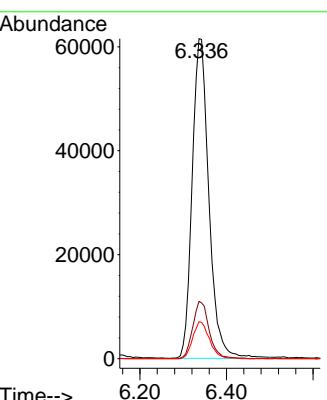

#44

Trichloroethene


Concen: 50.452 ug/l

RT: 7.123 min Scan# 990

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15











Tgt Ion:130 Resp: 59042

Ion Ratio Lower Upper

130 100

95 101.0 0.0 202.0





#45

1,2-Dichloropropane

Concen: 51.540 ug/l

RT: 7.427 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#46

Dibromomethane

Concen: 52.092 ug/l


RT: 7.574 min Scan# 1064




Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion: 93 Resp: 49125  
 Ion Ratio Lower Upper  
 93 100  
 95 81.0 64.8 97.2  
 174 81.7 65.4 98.0

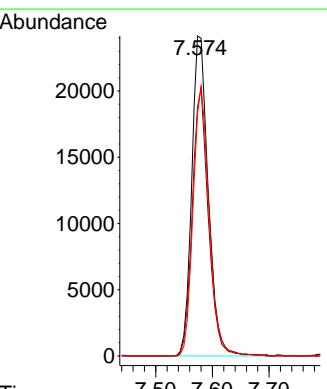

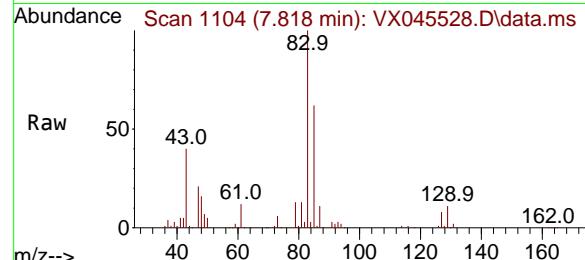





#47

Bromodichloromethane  
Concen: 51.068 ug/l  
RT: 7.818 min Scan# 1083  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025




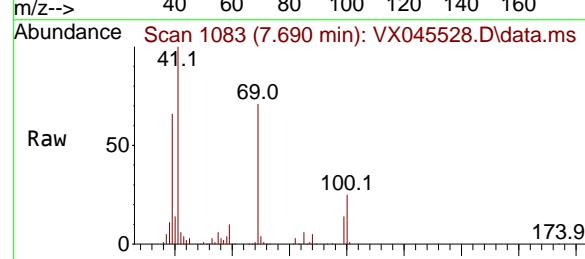




#48

Methyl methacrylate  
Concen: 53.768 ug/l  
RT: 7.690 min Scan# 1083  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion: 41 Resp: 85483  
Ion Ratio Lower Upper  
41 100  
69 72.7 58.2 87.2  
39 67.0 53.6 80.4



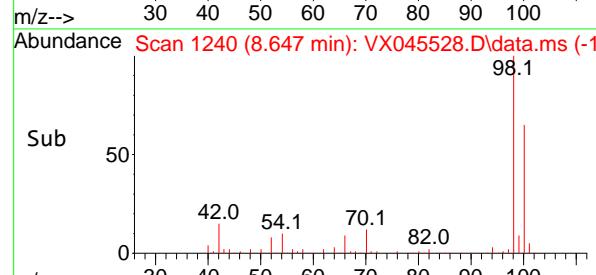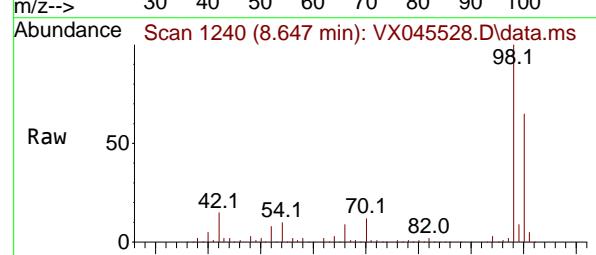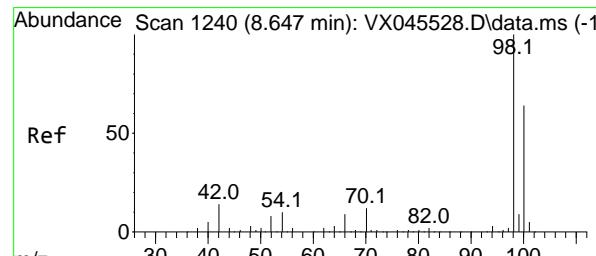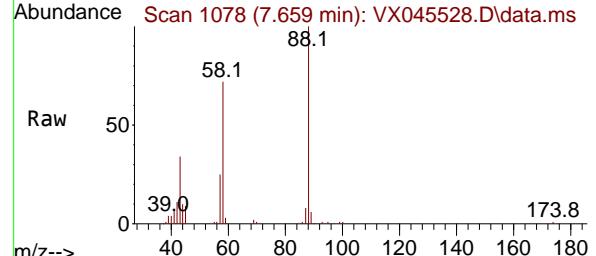

#49

1,4-Dioxane

Concen: 1084.635 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#50

Toluene-d8

Concen: 49.031 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15



Tgt Ion: 98 Resp: 204338

Ion Ratio Lower Upper

98 100

100 65.3 52.2 78.4

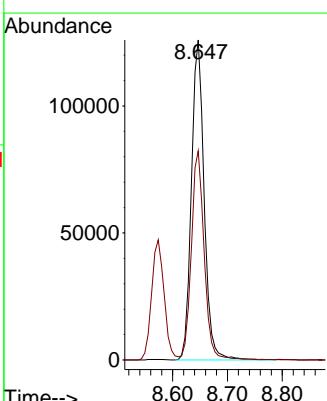

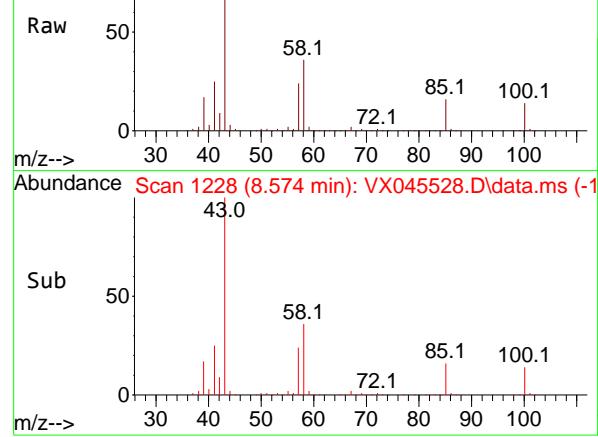

#51

4-Methyl-2-Pentanone

Concen: 273.375 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15



Instrument : MSVOA\_X

ClientSampleId : VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#52

Toluene

Concen: 51.402 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15




Tgt Ion: 92 Resp: 153143

Ion Ratio Lower Upper

92 100

91 173.4 138.7 208.1

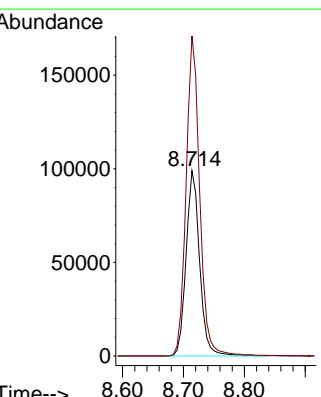



#53

t-1,3-Dichloropropene

Concen: 47.317 ug/l

RT: 8.976 min Scan# 1194

Delta R.T. -0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

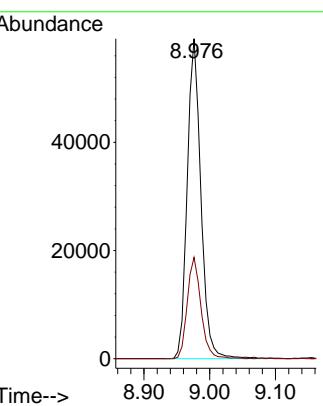

#54

cis-1,3-Dichloropropene

Concen: 53.975 ug/l

RT: 8.366 min Scan# 1194

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15


Tgt Ion: 75 Resp: 95524




Ion Ratio Lower Upper

75 100

77 30.7 24.6 36.8

39 60.5 48.4 72.6

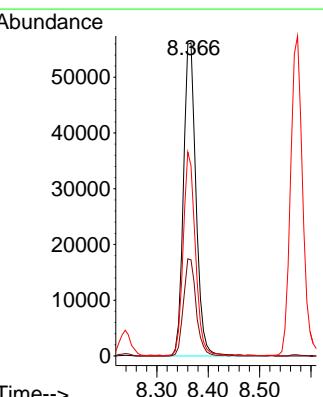



#55

1,1,2-Trichloroethane

Concen: 50.919 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#56

Ethyl methacrylate

Concen: 54.970 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15


Tgt Ion: 69 Resp: 100998


Ion Ratio Lower Upper

69 100

41 76.6 61.3 91.9

39 50.2 40.2 60.2

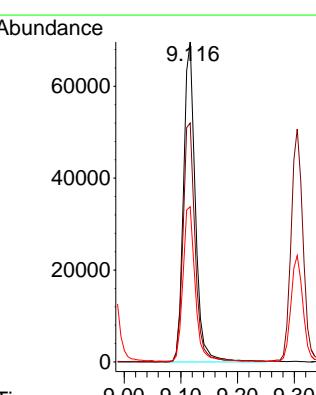


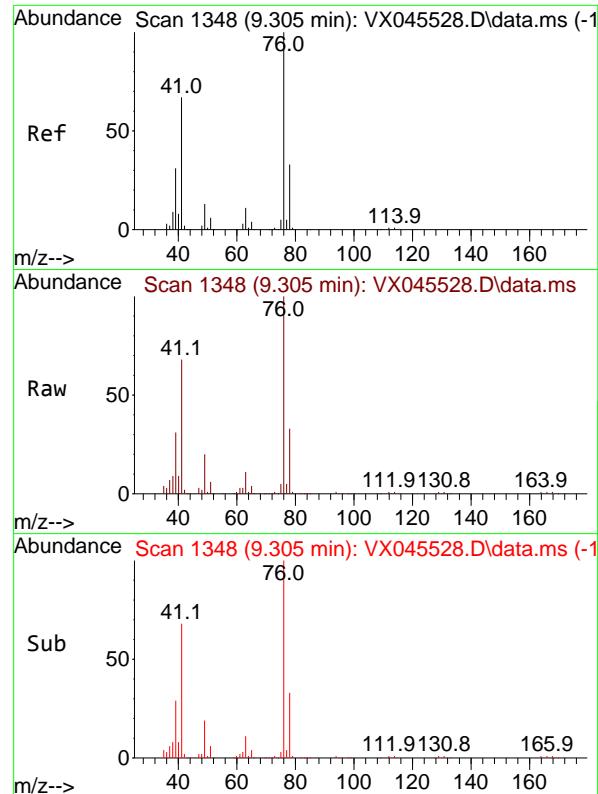


#57  
1,3-Dichloropropane  
Concen: 51.554 ug/l  
RT: 9.305 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

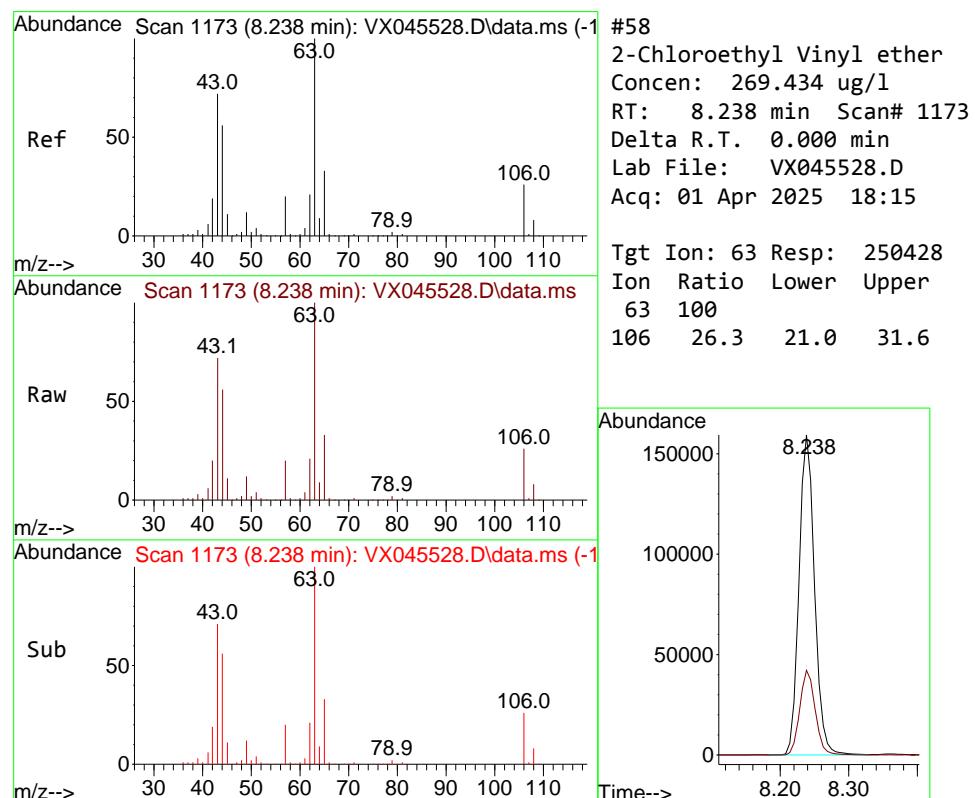



#58  
2-Chloroethyl Vinyl ether  
Concen: 269.434 ug/l  
RT: 8.238 min Scan# 1173  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion: 63 Resp: 250428  
Ion Ratio Lower Upper  
63 100  
106 26.3 21.0 31.6






Abundance Scan 1368 (9.427 min): VX045528.D\data.ms

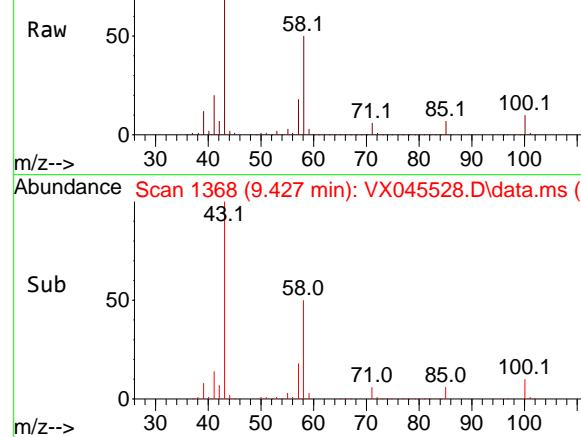

Abundance Scan 1383 (9.519 min): VX045528.D\data.ms

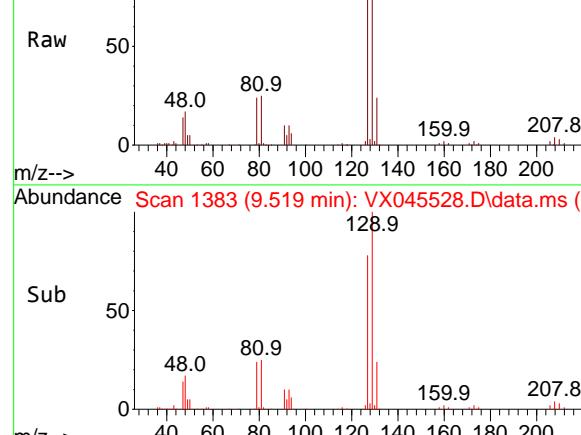

Abundance Scan 1383 (9.519 min): VX045528.D\data.ms (-1)

#59

2-Hexanone

Concen: 273.765 ug/l

RT: 9.427 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

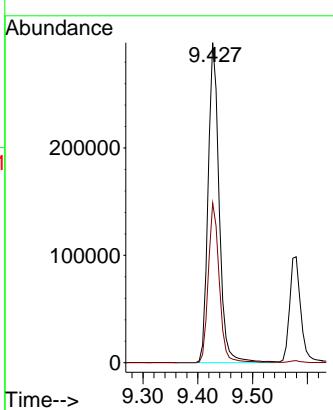

#60

Dibromochloromethane

Concen: 53.511 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15




Tgt Ion:129 Resp: 69258

Ion Ratio Lower Upper

129 100

127 78.8 39.4 118.2

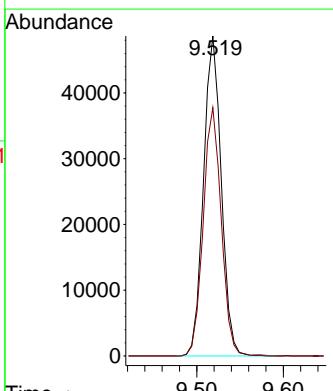

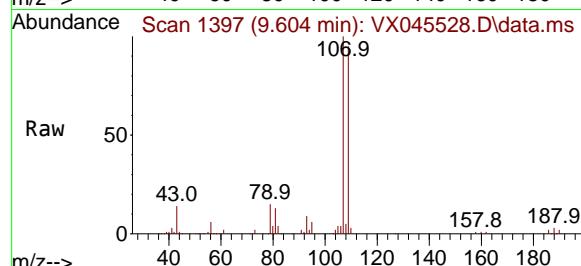

#61

1,2-Dibromoethane

Concen: 52.264 ug/l

RT: 9.604 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

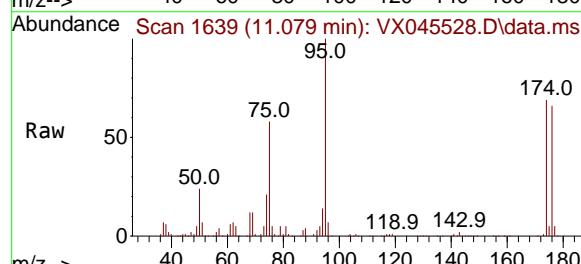

#62

4-Bromofluorobenzene

Concen: 50.190 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion: 95 Resp: 76190



Ion Ratio Lower Upper

95 100

174 67.9 0.0 135.8

176 65.7 0.0 131.4



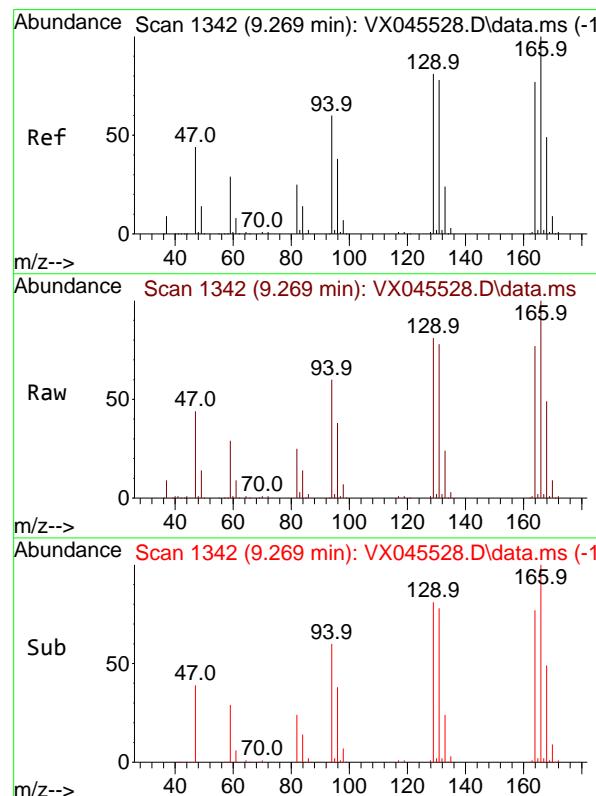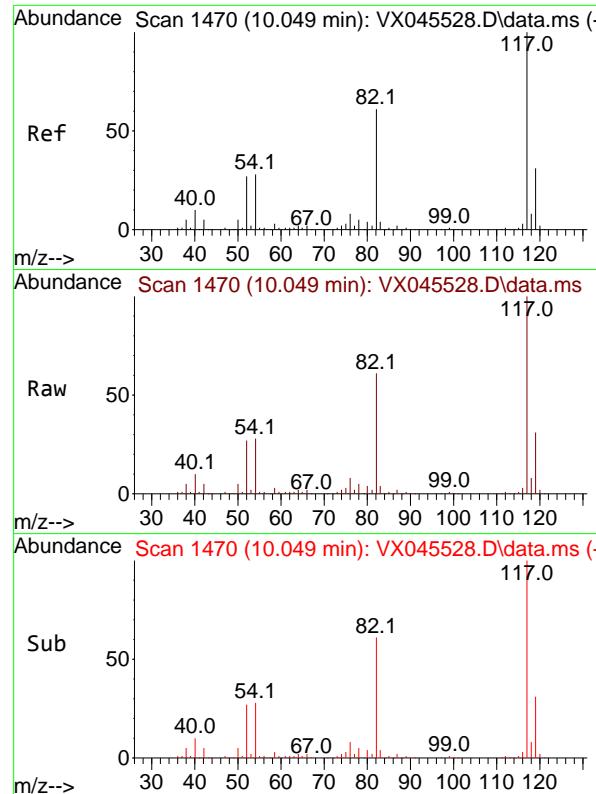


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1470  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025



#64  
Tetrachloroethene  
Concen: 49.181 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion:164 Resp: 52155  
Ion Ratio Lower Upper  
164 100  
166 129.8 103.8 155.8  
129 105.4 84.3 126.5  
131 101.1 80.9 121.3

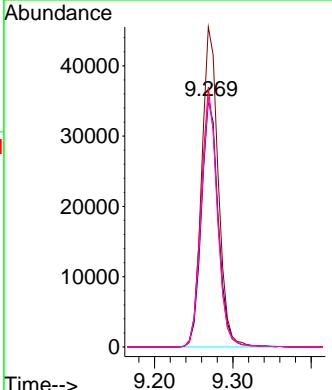


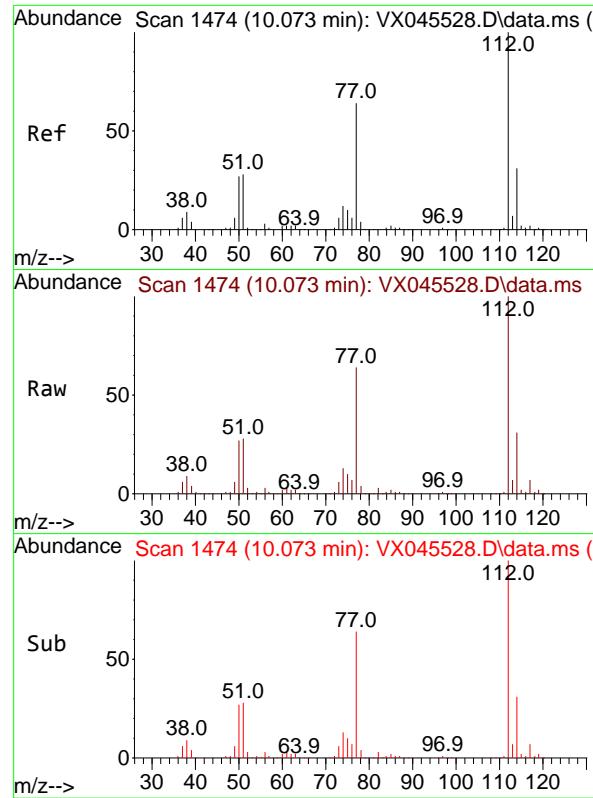


#65  
Chlorobenzene  
Concen: 50.733 ug/l  
RT: 10.073 min Scan# 1474  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**







Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

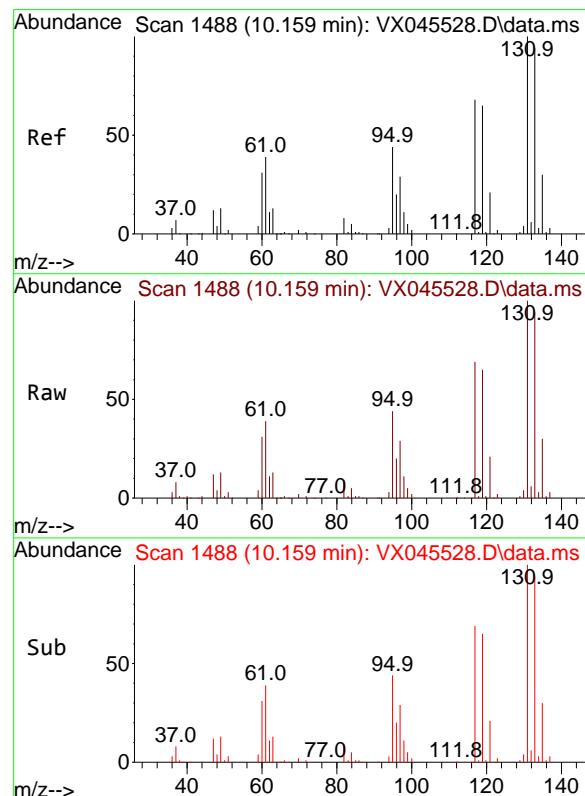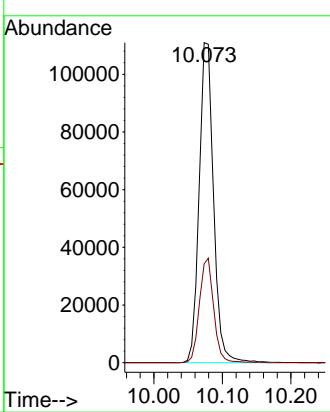

#66  
1,1,1,2-Tetrachloroethane  
Concen: 50.233 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion:131 Resp: 55974  
Ion Ratio Lower Upper  
131 100  
133 95.0 47.5 142.5  
119 65.7 32.9 98.6

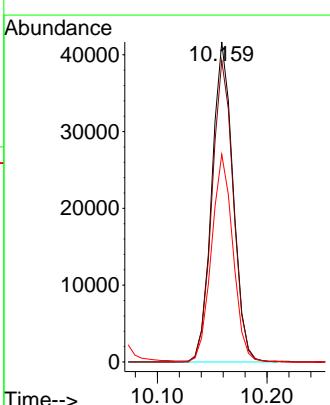

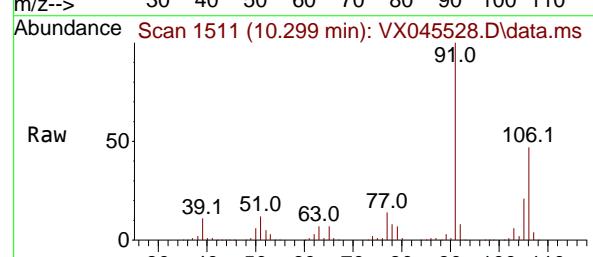

#67

Ethyl Benzene

Concen: 52.447 ug/l

RT: 10.189 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICCC050

1 Manual Integrations  
2 APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

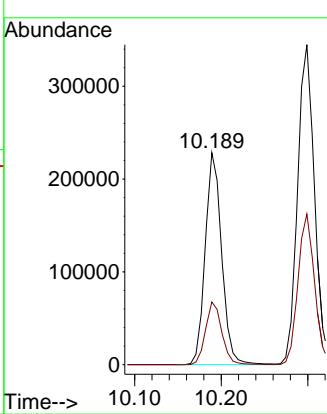

#68

m/p-Xylenes

Concen: 104.606 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15


Tgt Ion:106 Resp: 218702

Ion Ratio Lower Upper

106 100

91 215.7 172.6 258.8

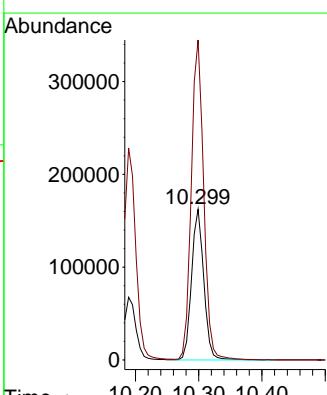

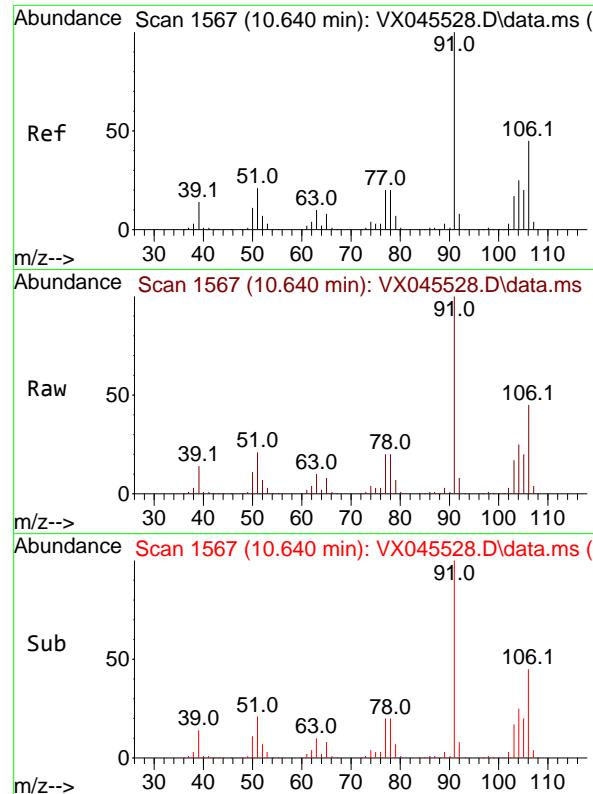



#69  
o-Xylene  
Concen: 52.452 ug/l  
RT: 10.640 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050

**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025


Supervised By :Mahesh Dadoda 04/02/2025

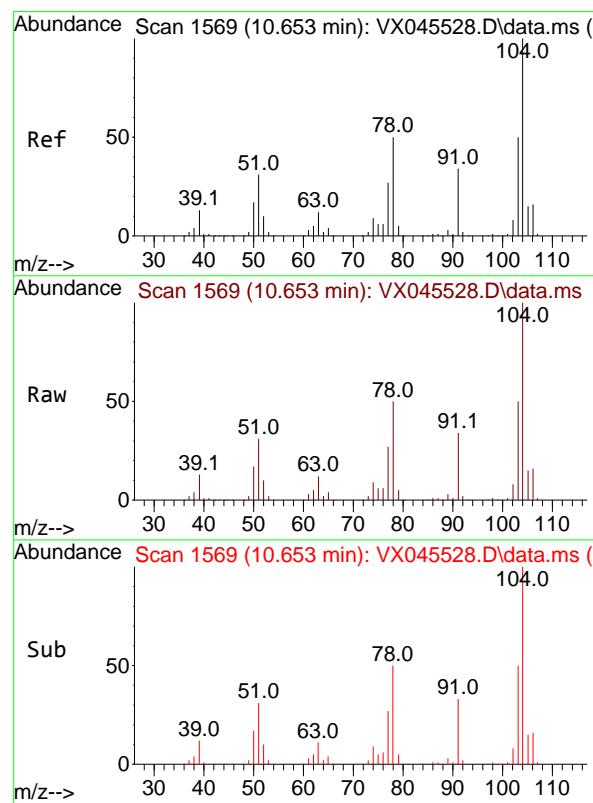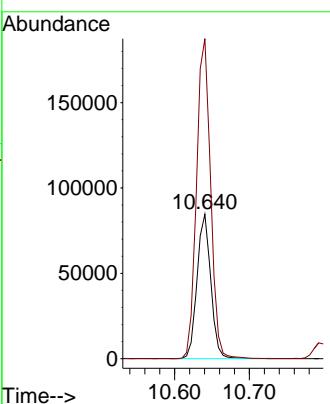


#70  
Styrene  
Concen: 53.723 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion:104 Resp: 182620  
Ion Ratio Lower Upper  
104 100  
78 56.8 45.4 68.2  
103 54.8 43.8 65.8

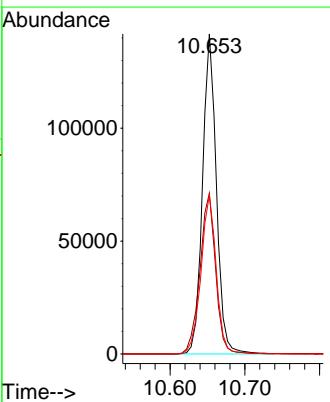



Abundance Scan 1593 (10.799 min): VX045528.D\data.ms (-)

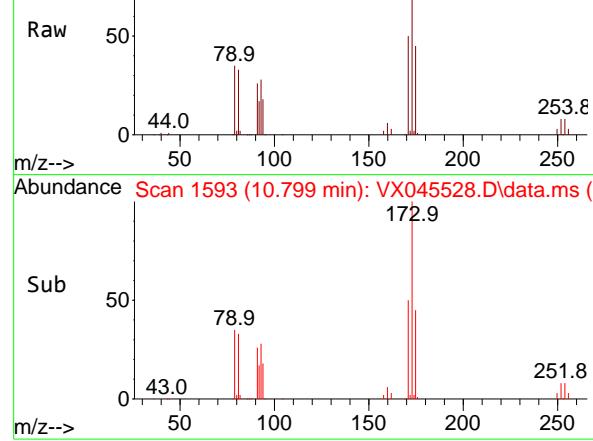



Abundance Scan 1593 (10.799 min): VX045528.D\data.ms (-)

#71  
Bromoform  
Concen: 53.361 ug/l  
RT: 10.799 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15


Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

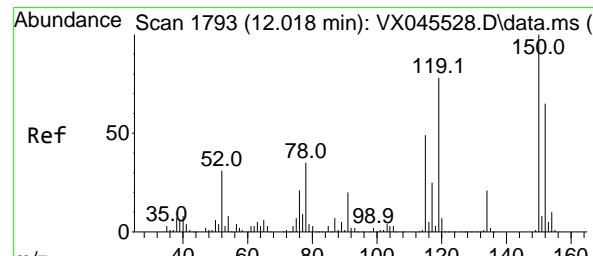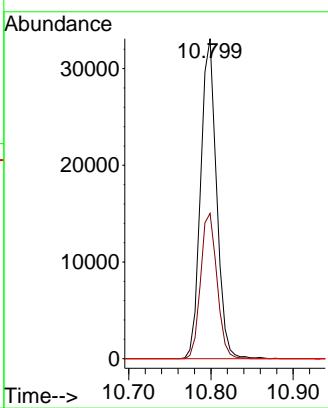


Abundance Scan 1793 (12.018 min): VX045528.D\data.ms (-)

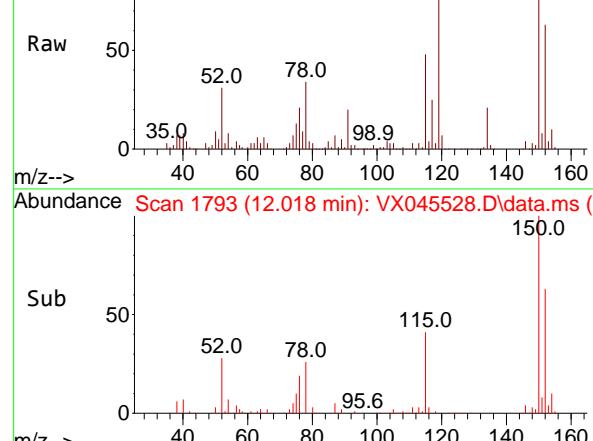


Abundance Scan 1793 (12.018 min): VX045528.D\data.ms (-)

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion:152 Resp: 68786  
Ion Ratio Lower Upper  
152 100  
115 93.8 46.9 140.7  
150 174.7 0.0 349.4

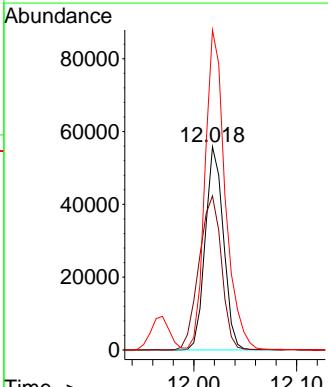

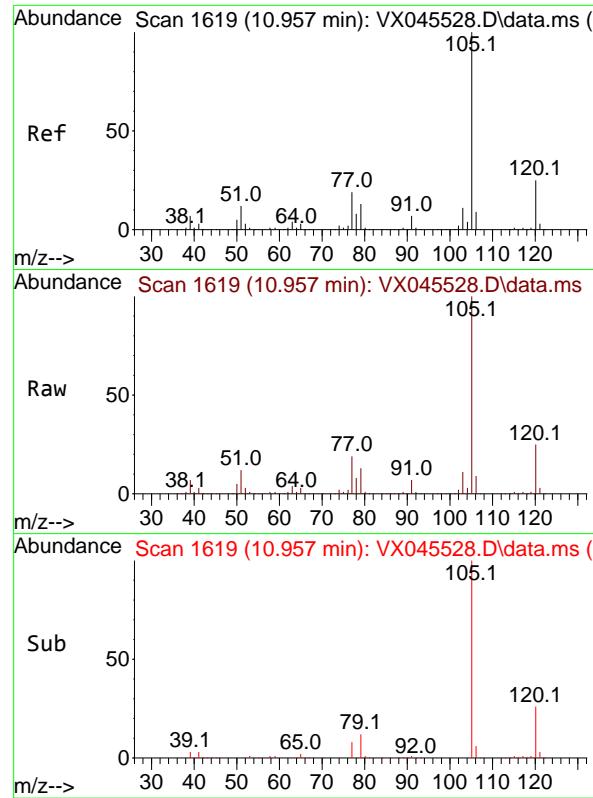

#73

Isopropylbenzene

Concen: 52.203 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

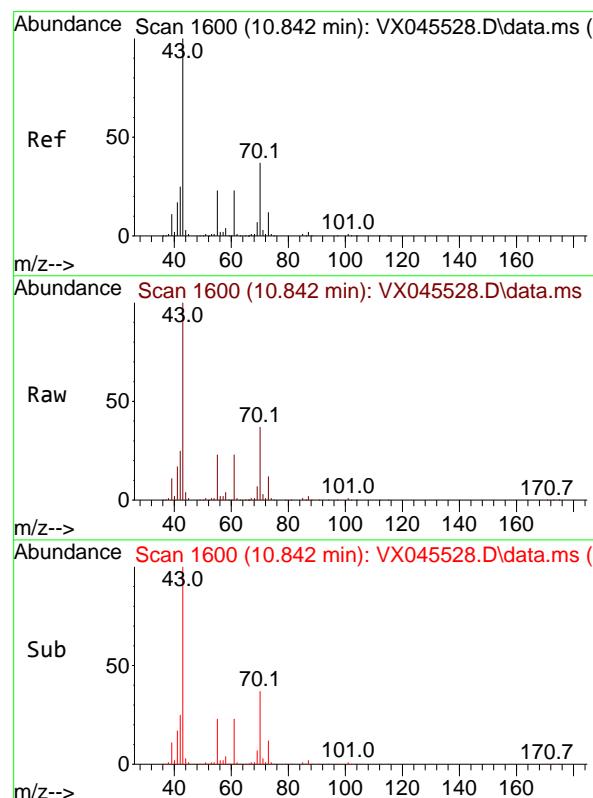

#74

N-amyl acetate

Concen: 53.721 ug/l

RT: 10.842 min Scan# 1600

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt Ion: 43 Resp: 141589


Ion Ratio Lower Upper




43 100

70 37.6 30.1 45.1

55 22.9 18.3 27.5

61 21.9 17.5 26.3

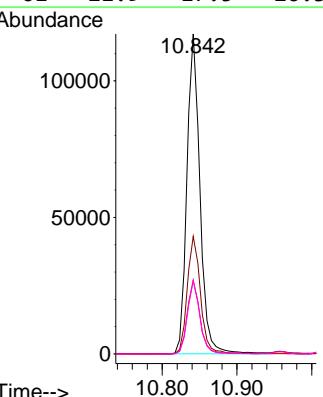

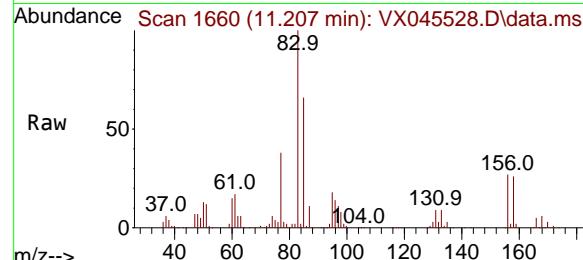

#75

1,1,2,2-Tetrachloroethane

Concen: 49.185 ug/l

RT: 11.207 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

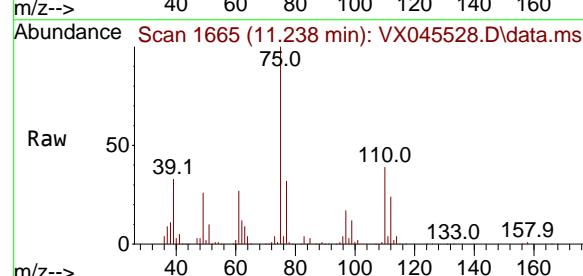

#76

1,2,3-Trichloropropane

Concen: 50.230 ug/l

RT: 11.238 min Scan# 1665

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15




Tgt Ion: 75 Resp: 84279

Ion Ratio Lower Upper

75 100

77 39.9 20.0 59.9





#77

Bromobenzene

Concen: 50.686 ug/l

RT: 11.195 min Scan# 1658

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

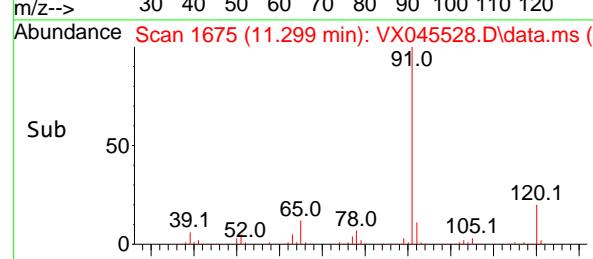

#78

n-propylbenzene

Concen: 53.069 ug/l

RT: 11.299 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15


Tgt Ion: 91 Resp: 336796

Ion Ratio Lower Upper



91 100

120 21.5 10.8 32.3

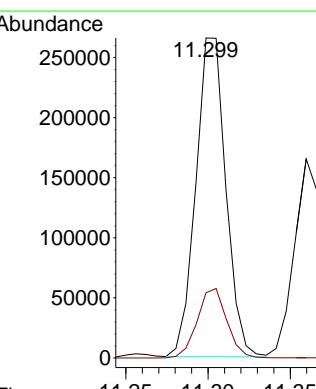





Abundance Scan 1685 (11.360 min): VX045528.D\data.ms (-)

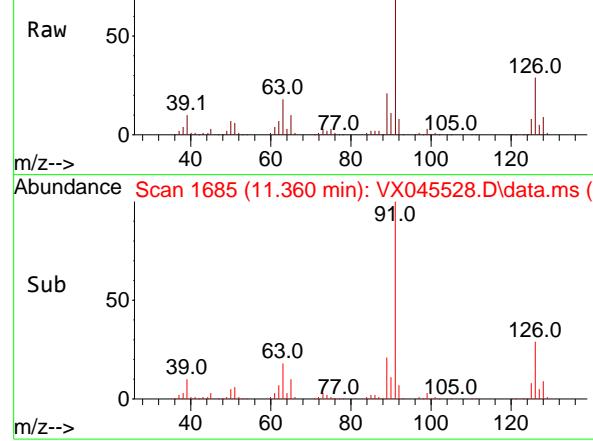

Abundance Scan 1700 (11.451 min): VX045528.D\data.ms (-)

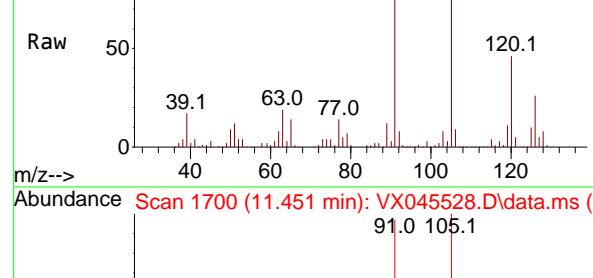

Abundance Scan 1700 (11.451 min): VX045528.D\data.ms (-)

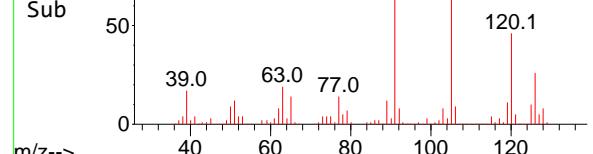

#79

2-Chlorotoluene

Concen: 50.279 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#80

1,3,5-Trimethylbenzene

Concen: 53.013 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15


Tgt Ion:105 Resp: 241536

Ion Ratio Lower Upper

105 100

120 46.0 23.0 69.0

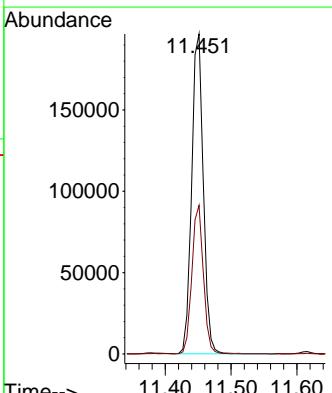


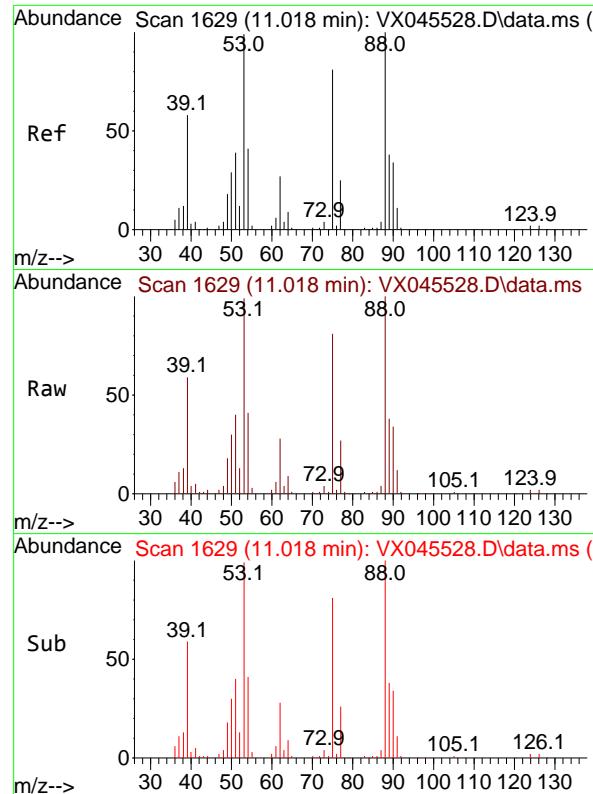


#81  
trans-1,4-Dichloro-2-butene  
Concen: 51.556 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

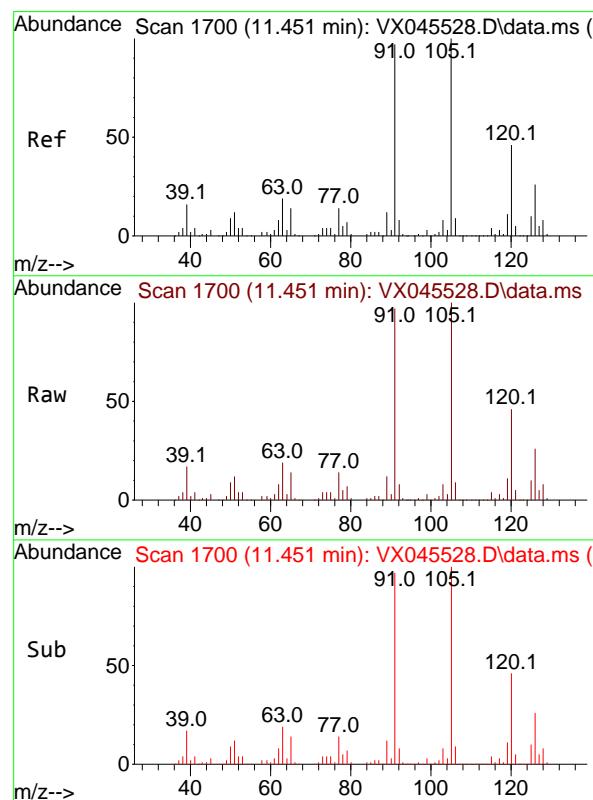

#82  
4-Chlorotoluene  
Concen: 52.439 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion: 91 Resp: 237213  
Ion Ratio Lower Upper  
91 100  
126 26.6 13.3 39.9



#83

tert-Butylbenzene

Concen: 52.256 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D




Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICCC050

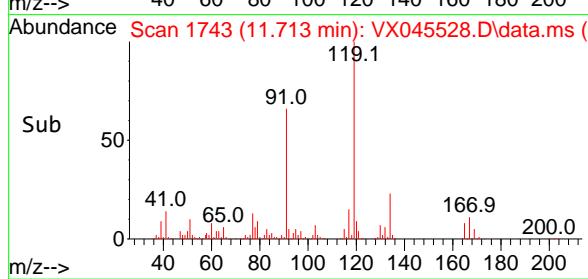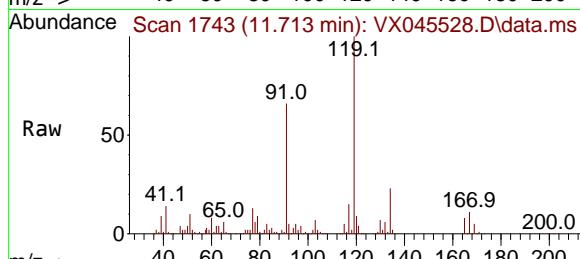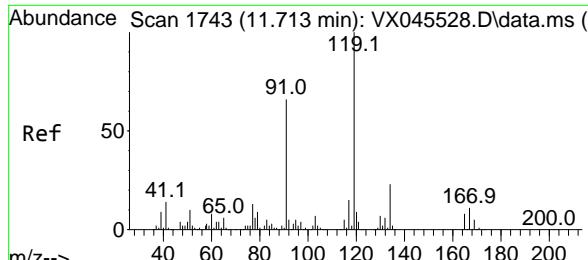

Tgt Ion:119 Resp: 23571

Ion Ratio Lower Upper

119 100





91 64.8 32.4 97.2

134 23.0 11.5 34.5

**Manual Integrations****APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

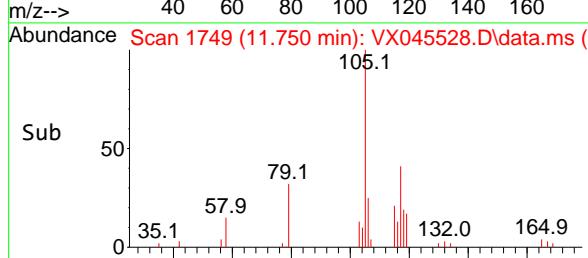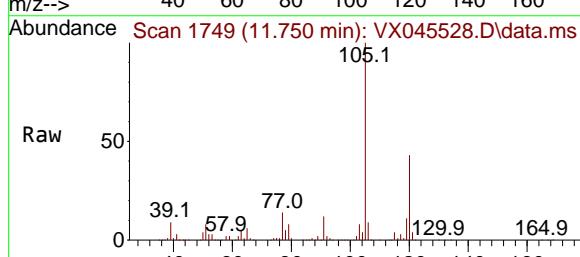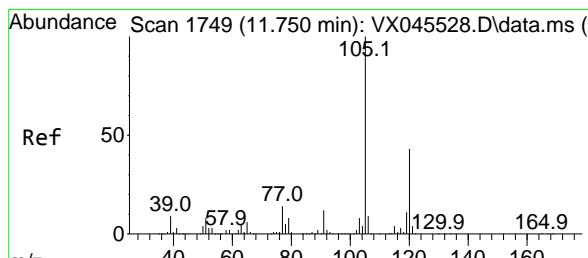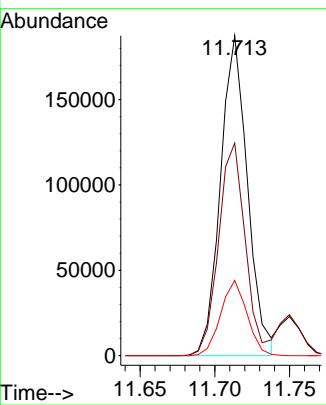

#84

1,2,4-Trimethylbenzene

Concen: 52.986 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045528.D


Acq: 01 Apr 2025 18:15


Tgt Ion:105 Resp: 242301

Ion Ratio Lower Upper


105 100

120 42.9 21.4 64.3

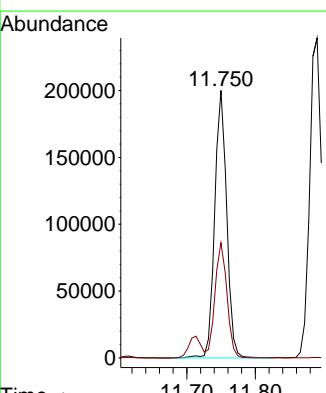



Abundance Scan 1772 (11.890 min): VX045528.D\data.ms (-)

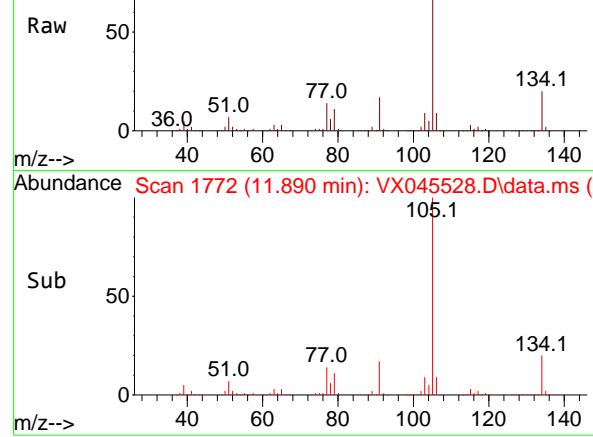


Abundance Scan 1772 (11.890 min): VX045528.D\data.ms (-)

#85  
sec-Butylbenzene  
Concen: 53.391 ug/l  
RT: 11.890 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15


Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

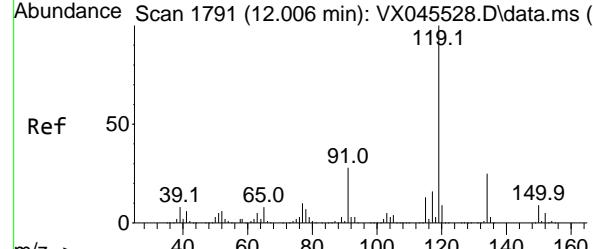


Abundance Scan 1791 (12.006 min): VX045528.D\data.ms (-)

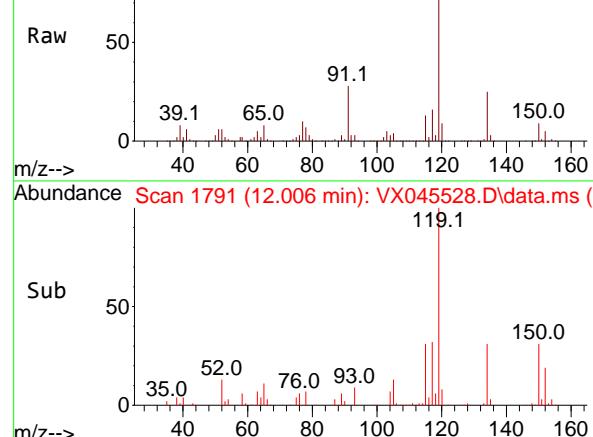


Abundance Scan 1791 (12.006 min): VX045528.D\data.ms (-)

#86  
p-Isopropyltoluene  
Concen: 53.073 ug/l  
RT: 12.006 min Scan# 1791  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion:119 Resp: 242416  
Ion Ratio Lower Upper  
119 100  
134 25.2 12.6 37.8  
91 27.4 13.7 41.1

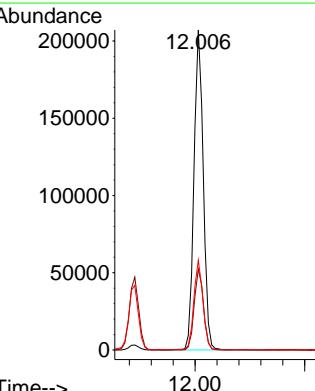

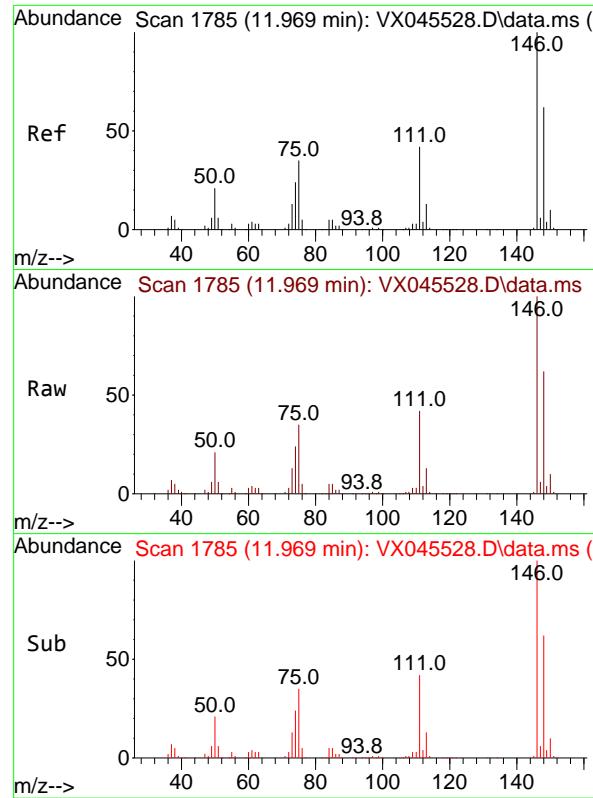

#87

1,3-Dichlorobenzene

Concen: 50.441 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

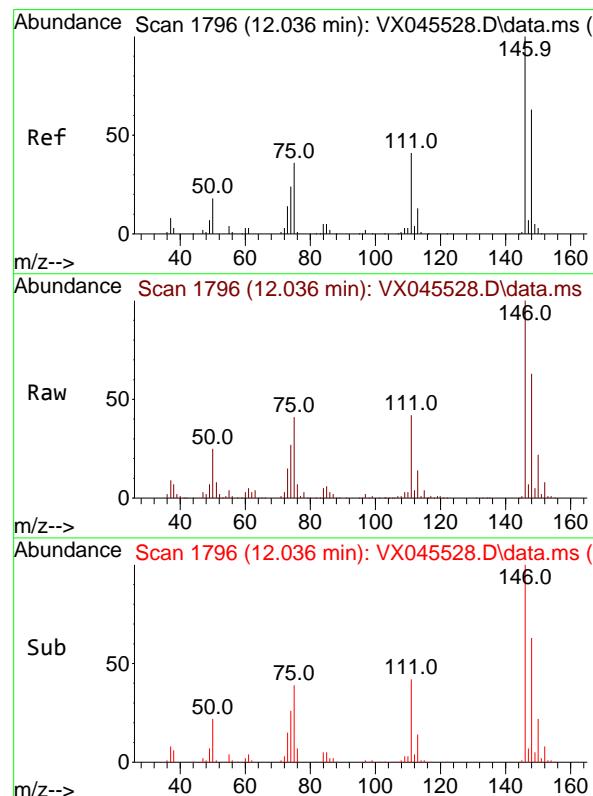

#88

1,4-Dichlorobenzene

Concen: 49.871 ug/l


RT: 12.036 min Scan# 1796




Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt	Ion:146	Resp:	117164
Ion	Ratio	Lower	Upper
146	100		
111	41.9	20.9	62.8
148	63.0	31.5	94.5

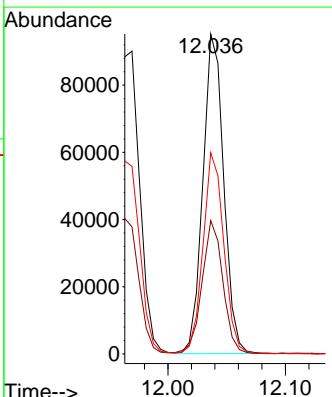

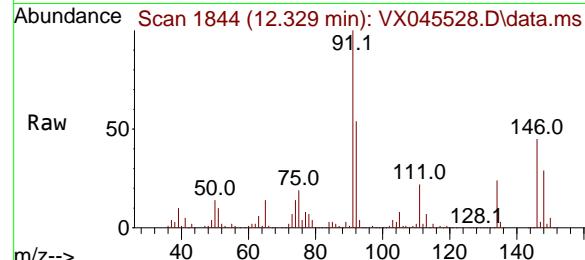

#89

n-Butylbenzene

Concen: 54.874 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

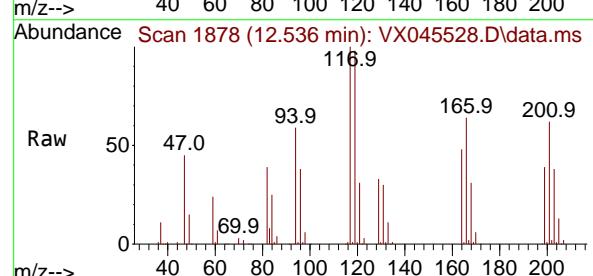

#90

Hexachloroethane

Concen: 52.352 ug/l


RT: 12.536 min Scan# 1878




Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt	Ion:117	Resp:	41095
Ion	Ratio	Lower	Upper
117	100		
201	62.4	31.2	93.6





#91

1,2-Dichlorobenzene

Concen: 50.099 ug/l

RT: 12.335 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

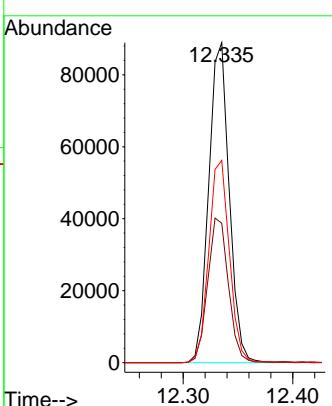

#92

1,2-Dibromo-3-Chloropropane

Concen: 53.638 ug/l



RT: 12.939 min Scan# 1944


Delta R.T. 0.000 min

Lab File: VX045528.D

Acq: 01 Apr 2025 18:15

Tgt	Ion:	75	Resp:	21712
Ion	Ratio	Lower	Upper	
	75	100		
	155	69.8	34.9	104.7
	157	89.8	44.9	134.7

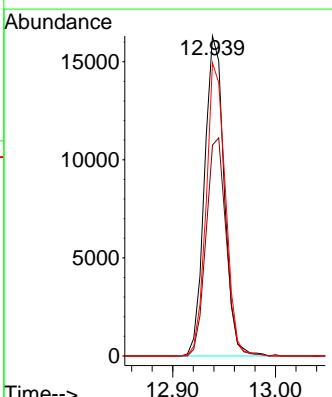


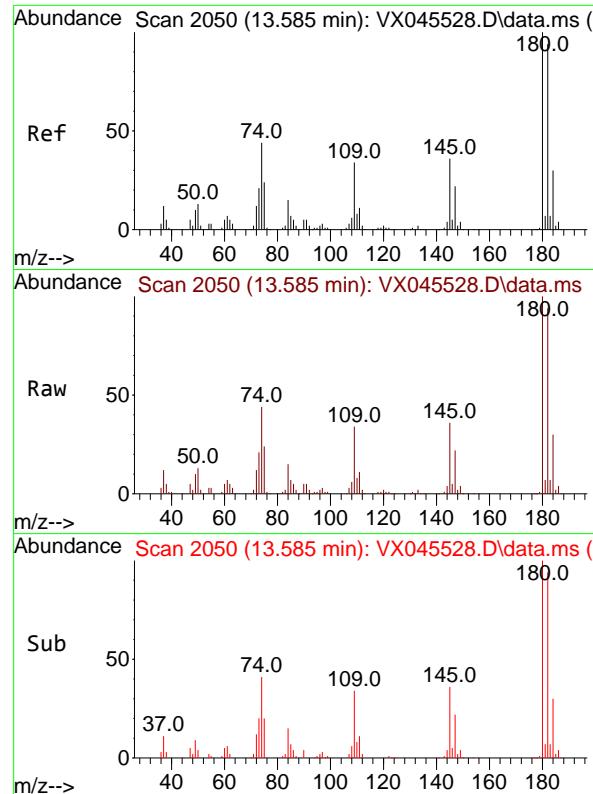


#93  
1,2,4-Trichlorobenzene  
Concen: 50.797 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

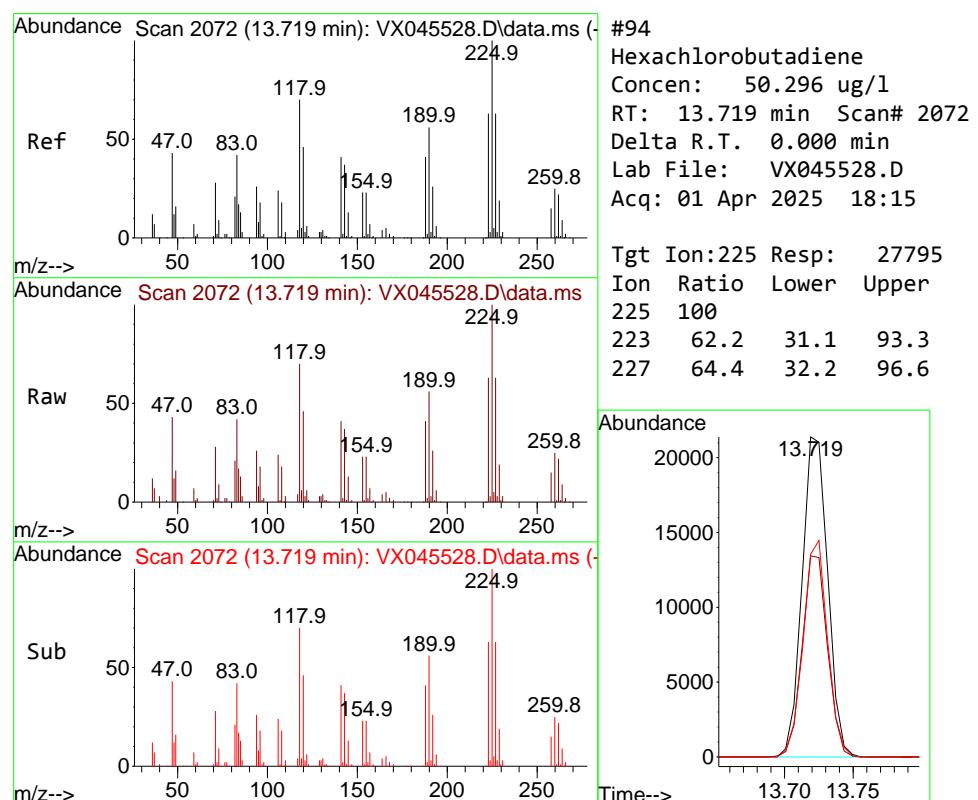

#94  
Hexachlorobutadiene  
Concen: 50.296 ug/l  
RT: 13.719 min Scan# 2072  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion:225 Resp: 27795  
Ion Ratio Lower Upper  
225 100  
223 62.2 31.1 93.3  
227 64.4 32.2 96.6

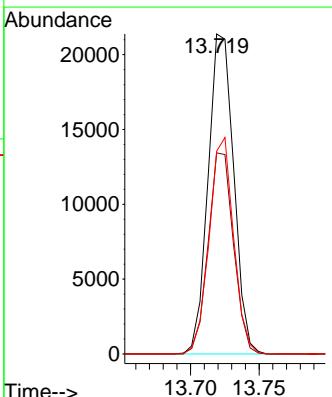


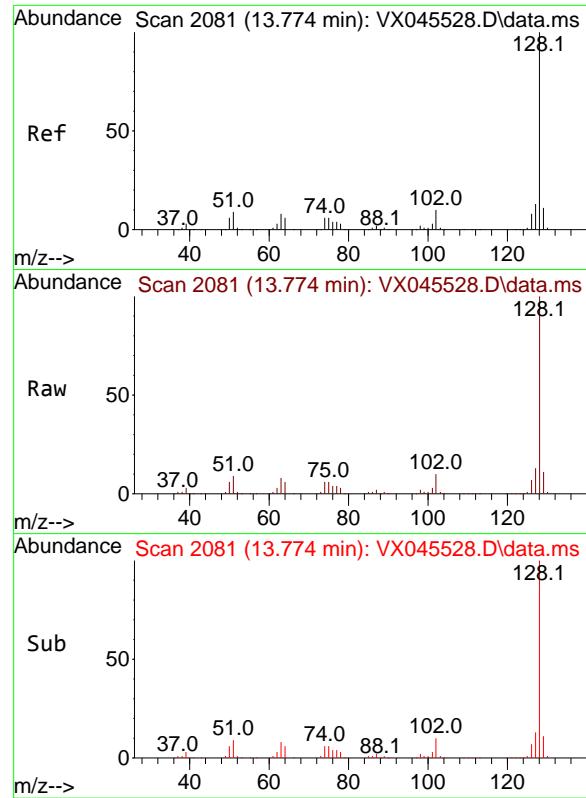


#95  
Naphthalene  
Concen: 53.643 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

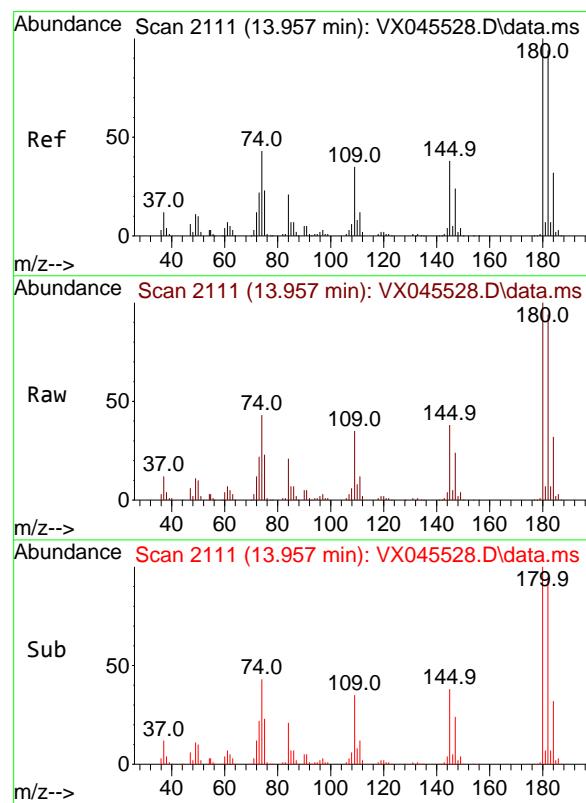

#96  
1, 2, 3-Trichlorobenzene  
Concen: 51.219 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045528.D  
Acq: 01 Apr 2025 18:15

Tgt Ion:180 Resp: 68781  
Ion Ratio Lower Upper  
180 100  
182 94.5 47.3 141.8  
145 36.4 18.2 54.6



Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045529.D  
 Acq On : 01 Apr 2025 18:38  
 Operator : JC/MD  
 Sample : VSTDICC100  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC100

Quant Time: Apr 02 02:54:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	86107	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	152724	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	136369	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	64612	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.946	65	155757	98.914	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 197.820%	#	
35) Dibromofluoromethane	5.379	113	107908	99.585	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 199.160%	#	
50) Toluene-d8	8.647	98	375599	99.309	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 198.620%	#	
62) 4-Bromofluorobenzene	11.079	95	146944	106.664	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 213.320%	#	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	144108	111.909	ug/l	99
3) Chloromethane	1.307	50	140360	106.098	ug/l	100
4) Vinyl Chloride	1.374	62	127174	105.042	ug/l	99
5) Bromomethane	1.593	94	58706	102.266	ug/l	98
6) Chloroethane	1.660	64	61099	95.120	ug/l	98
7) Trichlorofluoromethane	1.867	101	187555	103.887	ug/l	98
8) Diethyl Ether	2.136	74	61683	101.767	ug/l	99
9) 1,1,2-Trichlorotrifluo...	2.319	101	106989	101.133	ug/l	97
10) Methyl Iodide	2.441	142	135732	102.863	ug/l	100
11) Tert butyl alcohol	2.989	59	110044	519.999	ug/l	99
12) 1,1-Dichloroethene	2.306	96	106404	102.934	ug/l	99
13) Acrolein	2.233	56	146268	501.914	ug/l	99
14) Allyl chloride	2.654	41	206484	105.276	ug/l	99
15) Acrylonitrile	3.062	53	338970	507.426	ug/l	99
16) Acetone	2.386	43	314285	486.054	ug/l	100
17) Carbon Disulfide	2.502	76	276285	108.215	ug/l	100
18) Methyl Acetate	2.703	43	147272	98.925	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	381719	105.561	ug/l	99
20) Methylene Chloride	2.782	84	121435	100.316	ug/l	98
21) trans-1,2-Dichloroethene	3.081	96	106896	101.220	ug/l	98
22) Diisopropyl ether	3.757	45	406185	105.132	ug/l	95
23) Vinyl Acetate	3.721	43	1848817	553.853	ug/l	99
24) 1,1-Dichloroethane	3.605	63	220934	101.114	ug/l	100
25) 2-Butanone	4.556	43	491249	519.018	ug/l	100
26) 2,2-Dichloropropane	4.465	77	155592	110.215	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	129785	100.871	ug/l	98
28) Bromochloromethane	4.891	49	105093	99.530	ug/l	100
29) Tetrahydrofuran	5.001	42	313121	510.264	ug/l	99
30) Chloroform	5.086	83	225402	100.255	ug/l	99
31) Cyclohexane	5.458	56	197136	102.056	ug/l	98
32) 1,1,1-Trichloroethane	5.379	97	198511	104.346	ug/l	99
36) 1,1-Dichloropropene	5.684	75	151448	103.515	ug/l	99
37) Ethyl Acetate	4.715	43	192130	104.207	ug/l	99
38) Carbon Tetrachloride	5.672	117	166465	105.278	ug/l	99
39) Methylcyclohexane	7.373	83	191752	106.921	ug/l	99
40) Benzene	6.031	78	452946	101.369	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045529.D  
 Acq On : 01 Apr 2025 18:38  
 Operator : JC/MD  
 Sample : VSTDICC100  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDICC100**

Quant Time: Apr 02 02:54:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	107037	109.068	ug/l	99
42) 1,2-Dichloroethane	6.080	62	189528	102.696	ug/l	100
43) Isopropyl Acetate	6.336	43	305974	109.494	ug/l	100
44) Trichloroethene	7.123	130	107332	101.062	ug/l	97
45) 1,2-Dichloropropane	7.421	63	115731	103.806	ug/l	98
46) Dibromomethane	7.574	93	87381	102.101	ug/l	97
47) Bromodichloromethane	7.818	83	179265	104.886	ug/l	98
48) Methyl methacrylate	7.690	41	158241	109.675	ug/l	99
49) 1,4-Dioxane	7.665	88	52624	2015.906	ug/l	97
51) 4-Methyl-2-Pentanone	8.574	43	988881	533.814	ug/l	99
52) Toluene	8.714	92	276323	102.199	ug/l	99
53) t-1,3-Dichloropropene	8.976	75	169413	100.645	ug/l	100
54) cis-1,3-Dichloropropene	8.366	75	182328	113.521	ug/l	99
55) 1,1,2-Trichloroethane	9.147	97	109208	101.361	ug/l	98
56) Ethyl methacrylate	9.116	69	192034	115.168	ug/l	99
57) 1,3-Dichloropropane	9.305	76	192473	102.588	ug/l	100
58) 2-Chloroethyl Vinyl ether	8.238	63	460297	545.696	ug/l	100
59) 2-Hexanone	9.427	43	738772	538.538	ug/l	99
60) Dibromochloromethane	9.519	129	128700	109.570	ug/l	98
61) 1,2-Dibromoethane	9.604	107	115919	106.282	ug/l	99
64) Tetrachloroethene	9.269	164	90817	94.325	ug/l	99
65) Chlorobenzene	10.073	112	296300	101.682	ug/l	98
66) 1,1,1,2-Tetrachloroethane	10.159	131	103437	102.243	ug/l	99
67) Ethyl Benzene	10.189	91	543568	104.152	ug/l	99
68) m/p-Xylenes	10.299	106	394241	207.694	ug/l	100
69) o-Xylene	10.640	106	195381	104.487	ug/l	99
70) Styrene	10.653	104	335333	108.654	ug/l	100
71) Bromoform	10.799	173	83632	110.714	ug/l #	97
73) Isopropylbenzene	10.957	105	522436	100.944	ug/l	100
74) N-amyl acetate	10.842	43	275462	111.267	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	174977	96.243	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	154048m	97.744	ug/l	
77) Bromobenzene	11.195	156	119561	99.983	ug/l	99
78) n-propylbenzene	11.299	91	622679	104.454	ug/l	100
79) 2-Chlorotoluene	11.360	91	376682	98.840	ug/l	99
80) 1,3,5-Trimethylbenzene	11.451	105	435137	101.675	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.018	75	51873	111.704	ug/l	95
82) 4-Chlorotoluene	11.451	91	432884	101.877	ug/l	99
83) tert-Butylbenzene	11.713	119	437649	103.292	ug/l	99
84) 1,2,4-Trimethylbenzene	11.750	105	444211	103.414	ug/l	99
85) sec-Butylbenzene	11.890	105	546857	105.082	ug/l	100
86) p-Isopropyltoluene	12.006	119	453109	105.609	ug/l	100
87) 1,3-Dichlorobenzene	11.969	146	221481	101.749	ug/l	99
88) 1,4-Dichlorobenzene	12.036	146	216367	98.047	ug/l	98
89) n-Butylbenzene	12.329	91	420694	113.075	ug/l	99
90) Hexachloroethane	12.536	117	80489	109.160	ug/l	100
91) 1,2-Dichlorobenzene	12.335	146	215157	99.419	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	43047	113.214	ug/l	99
93) 1,2,4-Trichlorobenzene	13.585	180	135046	112.106	ug/l	99
94) Hexachlorobutadiene	13.725	225	53636	103.326	ug/l	98
95) Naphthalene	13.774	128	499719	111.473	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	137328	108.869	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045529.D  
 Acq On : 01 Apr 2025 18:38  
 Operator : JC/MD  
 Sample : VSTDICC100  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDICC100**

Quant Time: Apr 02 02:54:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045529.D  
 Acq On : 01 Apr 2025 18:38  
 Operator : JC/MD  
 Sample : VSTDICC100  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1




Quant Time: Apr 02 02:54:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC100

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

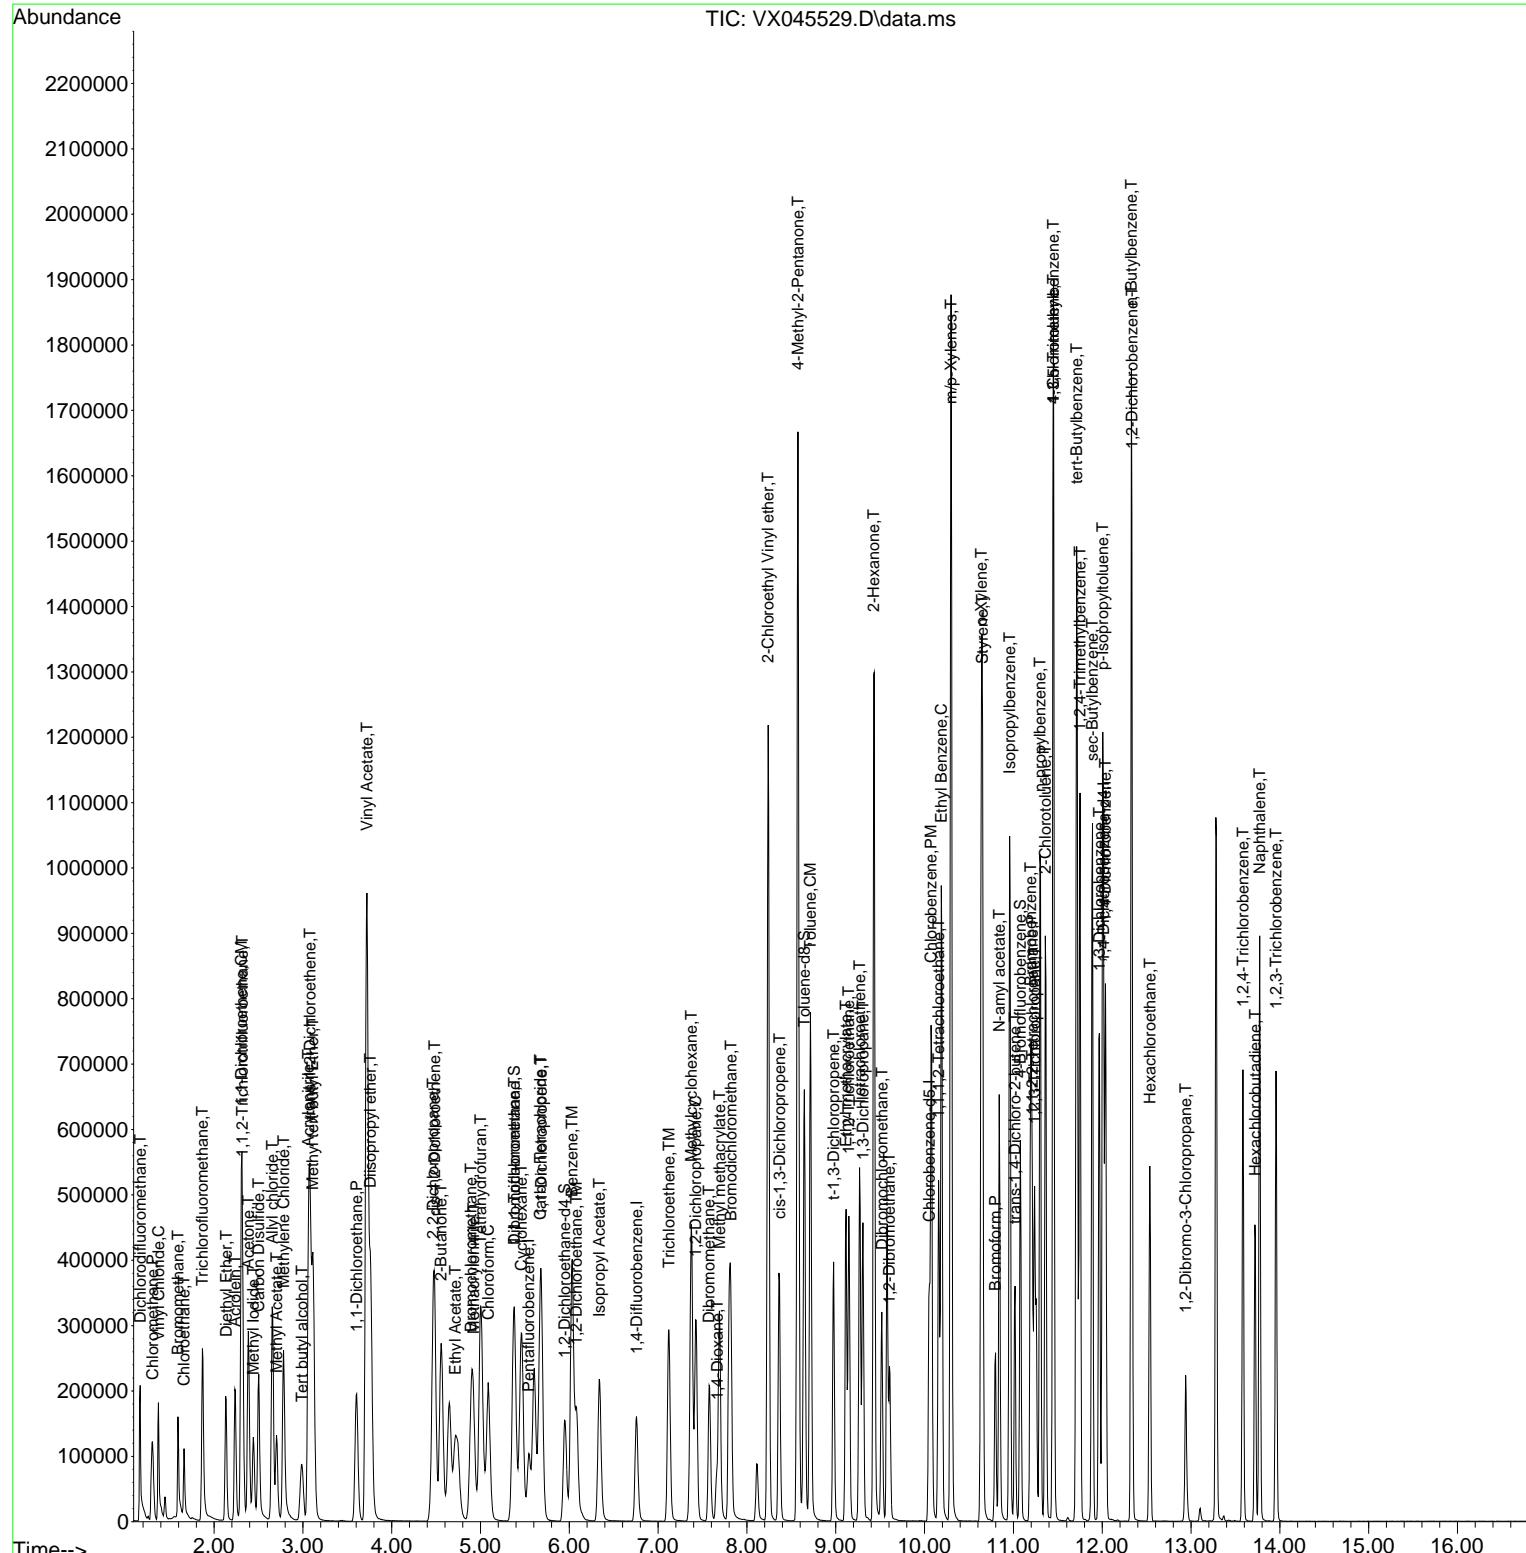

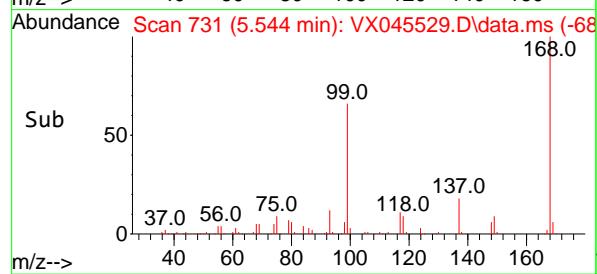




#1  
 Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.544 min Scan# 7  
 Delta R.T. -0.006 min  
 Lab File: VX045529.D  
 Acq: 01 Apr 2025 18:38

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC100



### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

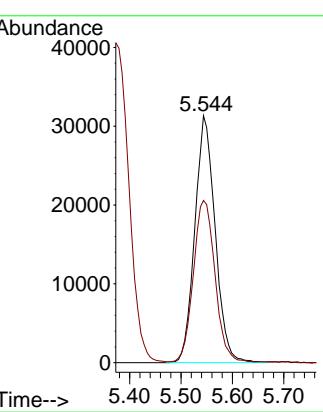

#2  
 Dichlorodifluoromethane  
 Concen: 111.909 ug/l  
 RT: 1.166 min Scan# 13  
 Delta R.T. 0.000 min  
 Lab File: VX045529.D  
 Acq: 01 Apr 2025 18:38

Tgt Ion: 85 Resp: 144108  
 Ion Ratio Lower Upper  
 85 100  
 87 32.4 16.1 48.2

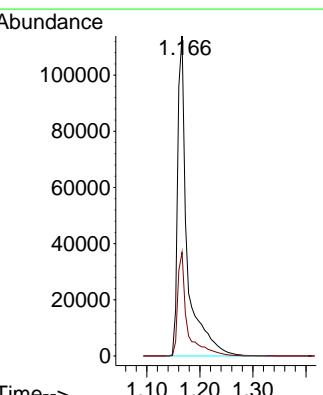



#3

Chloromethane

Concen: 106.098 ug/l

RT: 1.307 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

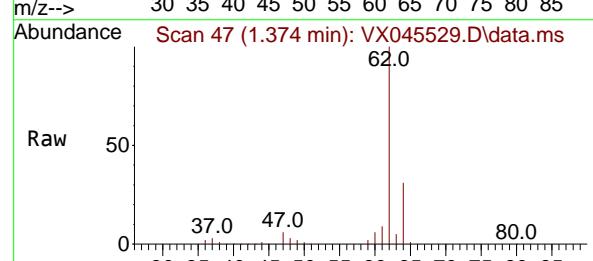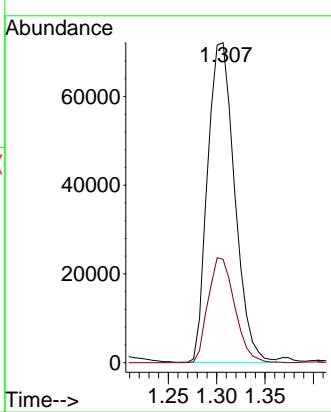

#4

Vinyl Chloride

Concen: 105.042 ug/l


RT: 1.374 min Scan# 47




Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt Ion: 62 Resp: 127174  
 Ion Ratio Lower Upper  
 62 100  
 64 31.2 25.5 38.3

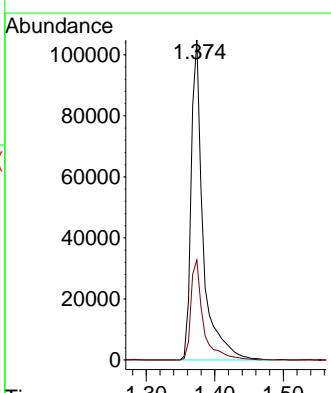



#5

Bromomethane

Concen: 102.266 ug/l

RT: 1.593 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#6

Chloroethane

Concen: 95.120 ug/l


RT: 1.660 min Scan# 94


Delta R.T. -0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt Ion: 64 Resp: 61099  
 Ion Ratio Lower Upper  
 64 100  
 66 31.7 26.3 39.5

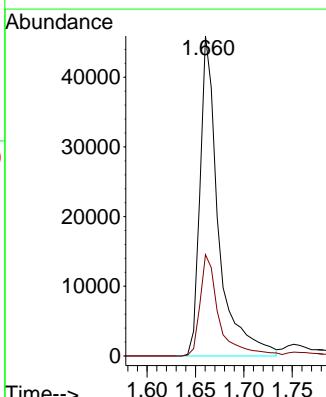


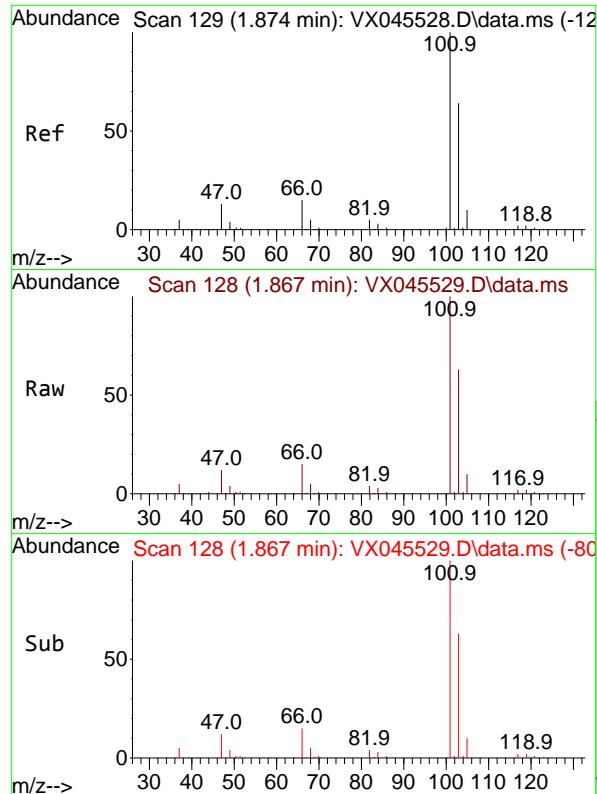


#7  
Trichlorofluoromethane  
Concen: 103.887 ug/l  
RT: 1.867 min Scan# 1  
Delta R.T. -0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

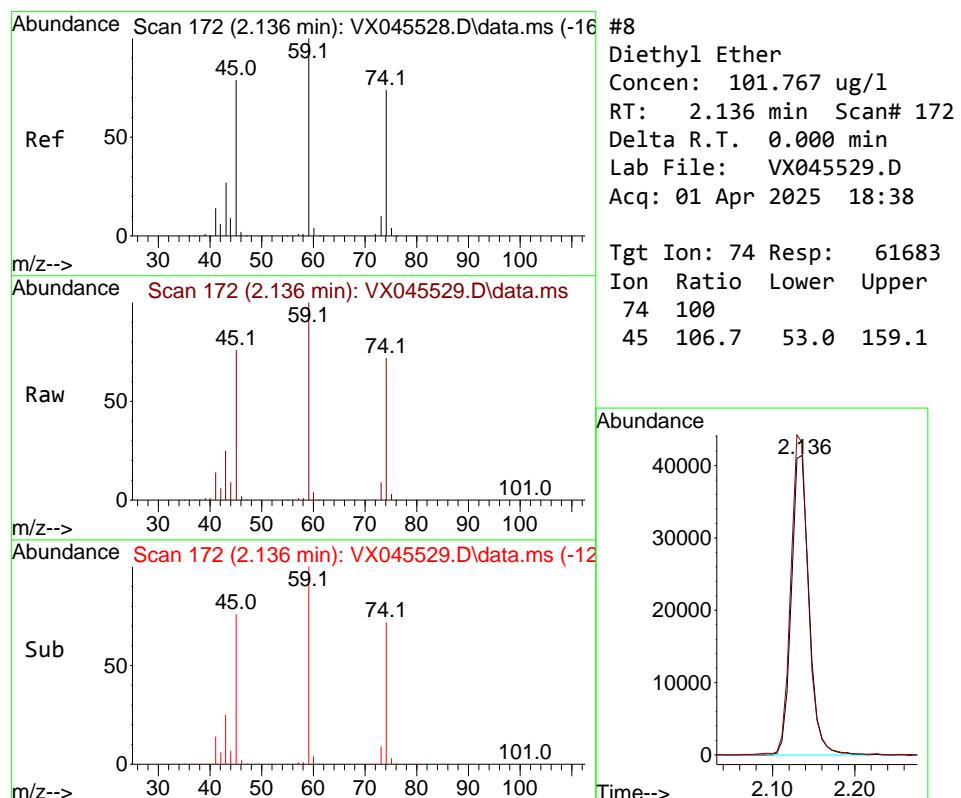



#8  
Diethyl Ether  
Concen: 101.767 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 74 Resp: 61683  
Ion Ratio Lower Upper  
74 100  
45 106.7 53.0 159.1







#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 101.133 ug/l  
RT: 2.319 min Scan# 2  
Delta R.T. -0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38




Tgt Ion:101 Resp: 106989  
Ion Ratio Lower Upper  
101 100  
85 47.3 38.9 58.3  
151 69.0 57.5 86.3

### Manual Integrations APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

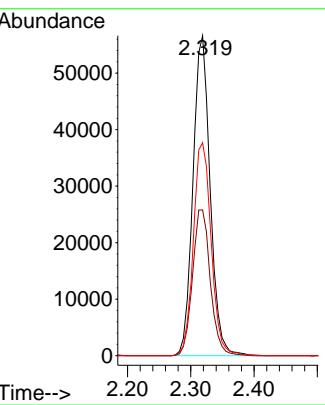


#10  
Methyl Iodide  
Concen: 102.863 ug/l  
RT: 2.441 min Scan# 222  
Delta R.T. -0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38



Tgt Ion:142 Resp: 135732  
Ion Ratio Lower Upper  
142 100  
127 50.6 40.2 60.4  
141 14.5 11.7 17.5

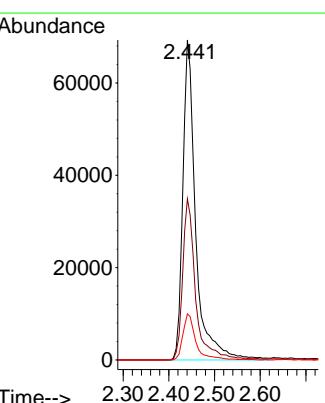

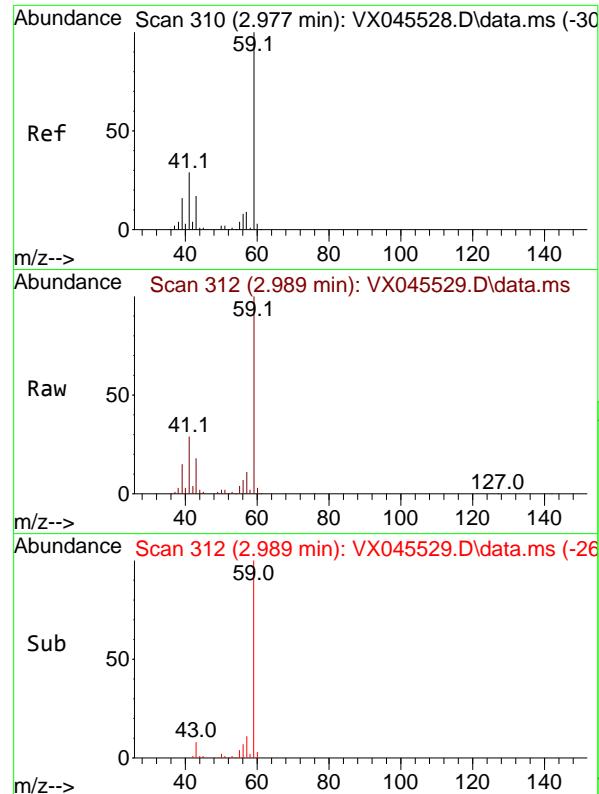



#11

Tert butyl alcohol  
Concen: 519.999 ug/l  
RT: 2.989 min Scan# 3  
Delta R.T. 0.012 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

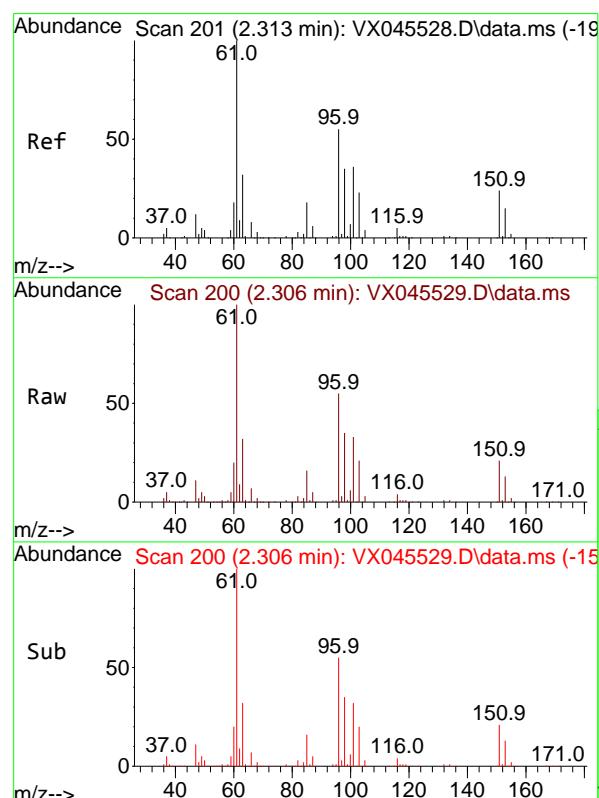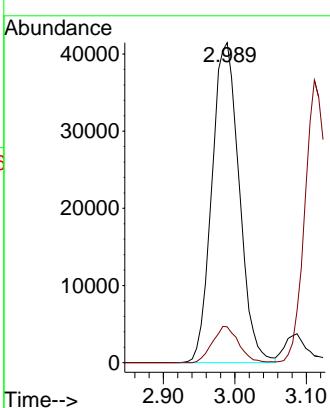


#12

1,1-Dichloroethene  
Concen: 102.934 ug/l  
RT: 2.306 min Scan# 200  
Delta R.T. -0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 96 Resp: 106404  
Ion Ratio Lower Upper  
96 100  
61 183.3 145.7 218.5  
98 63.3 51.6 77.4



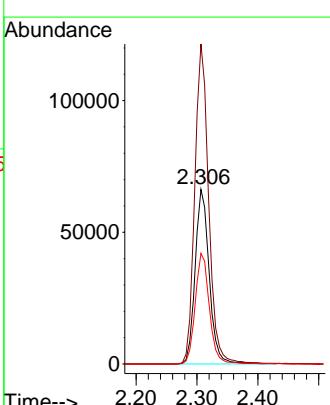




#13

Acrolein  
Concen: 501.914 ug/l  
RT: 2.233 min Scan# 189  
Delta R.T. -0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38


Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100





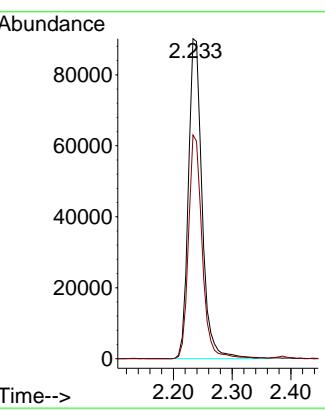



#14  
Allyl chloride  
Concen: 105.276 ug/l  
RT: 2.654 min Scan# 257  
Delta R.T. -0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38



Tgt Ion: 41 Resp: 206484  
Ion Ratio Lower Upper  
41 100  
39 75.8 60.2 90.2  
76 31.3 24.6 36.8

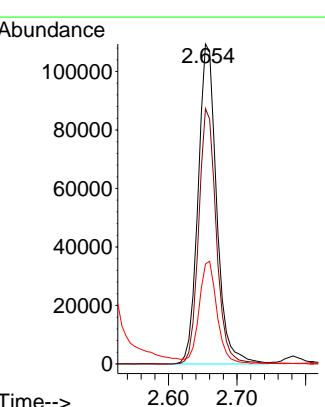



#15

Acrylonitrile

Concen: 507.426 ug/l

RT: 3.062 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

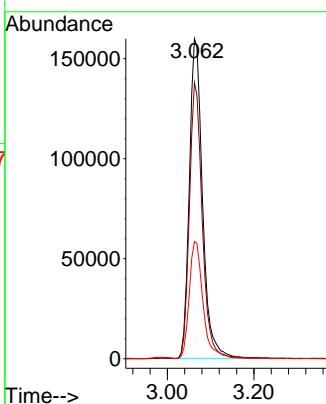

#16

Acetone

Concen: 486.054 ug/l


RT: 2.386 min Scan# 213







Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt Ion: 43 Resp: 314285  
Ion Ratio Lower Upper  
43 100  
58 27.8 22.3 33.5

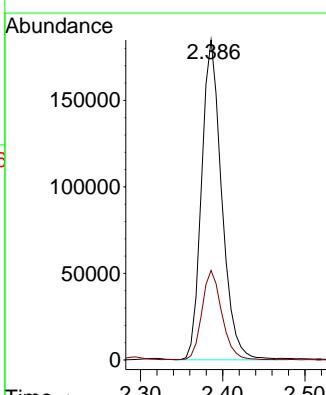

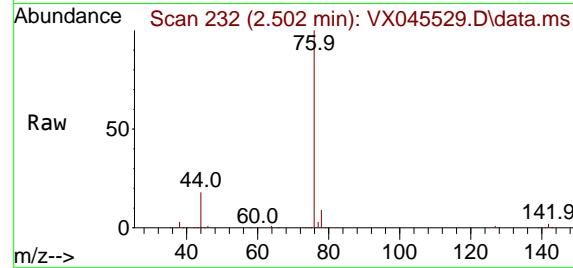

#17

Carbon Disulfide

Concen: 108.215 ug/l

RT: 2.502 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#18

Methyl Acetate

Concen: 98.925 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min


Lab File: VX045529.D




Acq: 01 Apr 2025 18:38

Tgt Ion: 43 Resp: 147272

Ion Ratio Lower Upper

43	100
74	22.2 17.5 26.3









#19

Methyl tert-butyl Ether  
Concen: 105.561 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025









#20

Methylene Chloride  
Concen: 100.316 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 84 Resp: 121435  
Ion Ratio Lower Upper  
84 100  
49 137.2 107.5 161.3  
51 42.1 33.0 49.6  
86 63.5 50.1 75.1

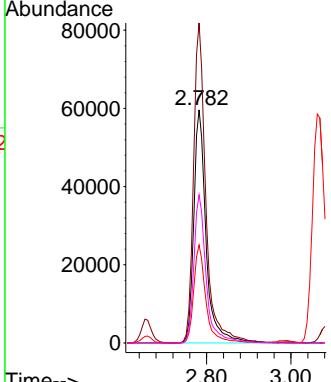

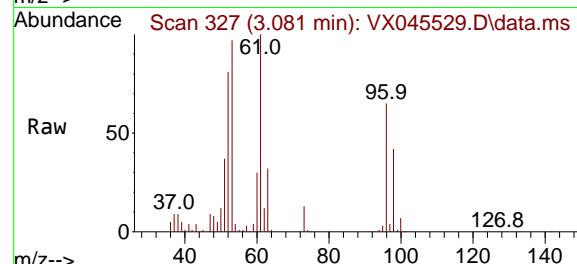

#21

trans-1,2-Dichloroethene

Concen: 101.220 ug/l

RT: 3.081 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

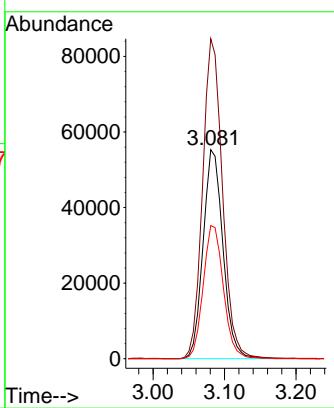

#22

Diisopropyl ether

Concen: 105.132 ug/l

RT: 3.757 min Scan# 438

Delta R.T. -0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt Ion: 45 Resp: 406185


Ion Ratio Lower Upper







45 100

43 80.1 59.3 88.9

87 24.7 20.4 30.6

59 10.6 9.0 13.6

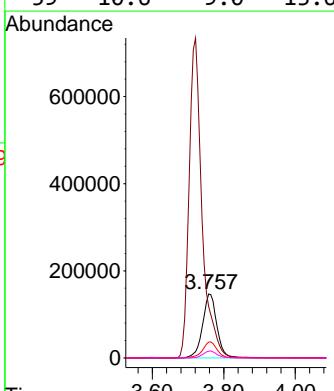

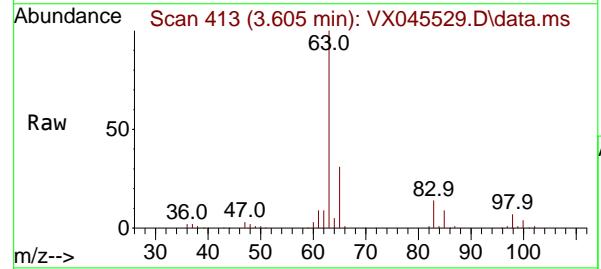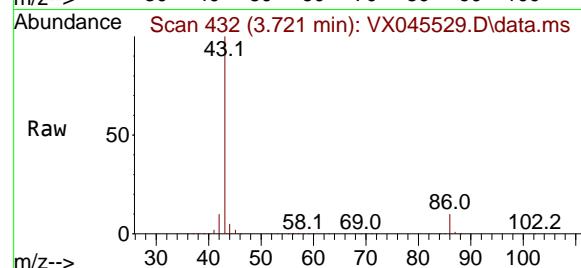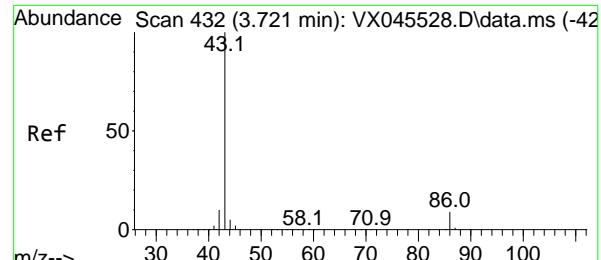

#23

**Vinyl Acetate**

Concen: 553.853 ug/l

RT: 3.721 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

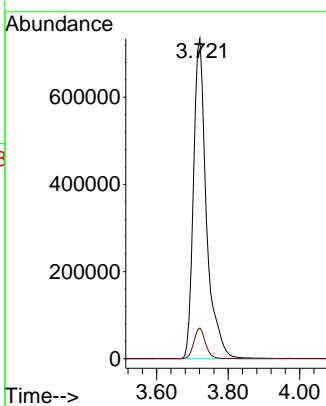

#24

**1,1-Dichloroethane**

Concen: 101.114 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion: 63 Resp: 220934


Ion Ratio Lower Upper

63 100

98 6.6 3.4 10.1


100 4.2 2.2 6.6



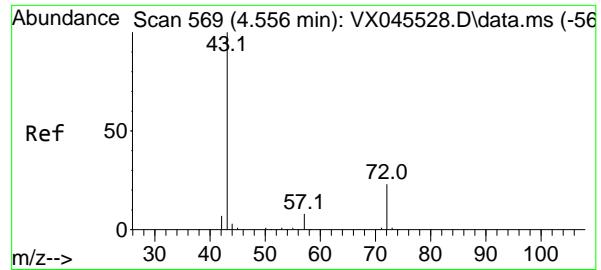

#25  
2-Butanone  
Concen: 519.018 ug/l  
RT: 4.556 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38



Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100




Tgt Ion: 43 Resp: 491249  
Ion Ratio Lower Upper  
43 100  
72 23.5 18.6 28.0

Manual Integrations  
APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025



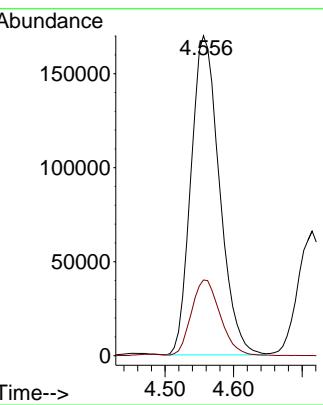


#26  
2,2-Dichloropropane  
Concen: 110.215 ug/l  
RT: 4.465 min Scan# 554  
Delta R.T. -0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

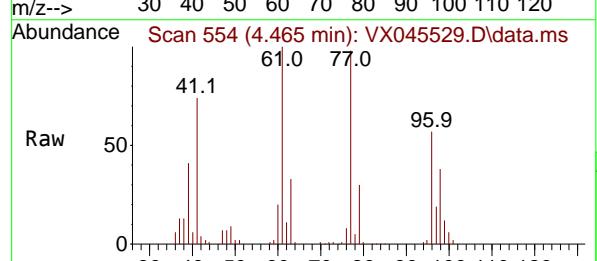

Tgt Ion: 77 Resp: 155592  
Ion Ratio Lower Upper  
77 100  
97 21.2 10.6 31.8

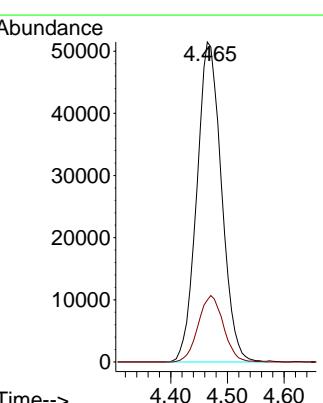

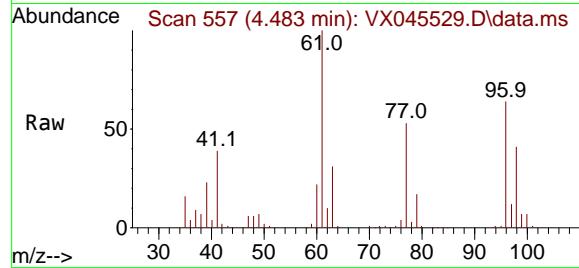

#27

cis-1,2-Dichloroethene

Concen: 100.871 ug/l

RT: 4.483 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#28

Bromochloromethane

Concen: 99.530 ug/l

RT: 4.891 min Scan# 624

Delta R.T. -0.006 min


Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion: 49 Resp: 105093

Ion Ratio Lower Upper


49	100		
129	1.8	0.0	3.8
130	68.4	54.6	81.8

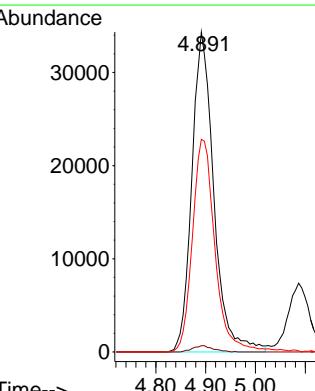


Abundance Scan 642 (5.001 min): VX045528.D\data.ms (-63)

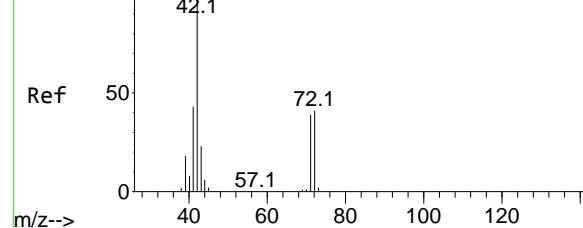

Abundance Scan 642 (5.001 min): VX045529.D\data.ms

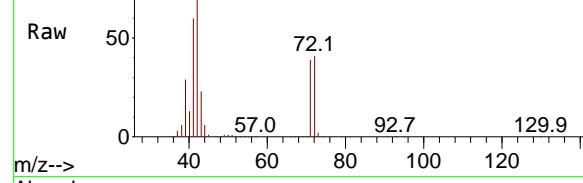

Abundance Scan 642 (5.001 min): VX045529.D\data.ms (-59)

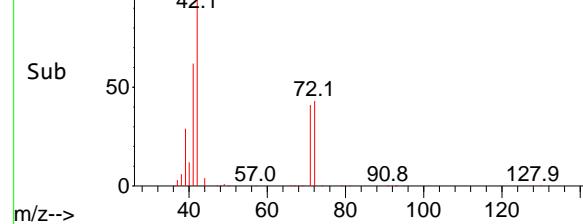

#29

Tetrahydrofuran

Concen: 510.264 ug/l

RT: 5.001 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC100

Tgt Ion: 42 Resp: 31312

Ion Ratio Lower Upper

42 100

72 42.3 33.4 50.0


71 39.1 31.4 47.0

**Manual Integrations****APPROVED**


Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025


Abundance Scan 656 (5.086 min): VX045528.D\data.ms (-64)

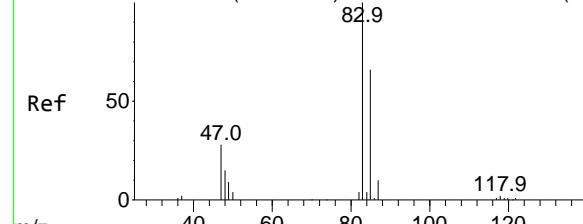

Abundance Scan 656 (5.086 min): VX045529.D\data.ms

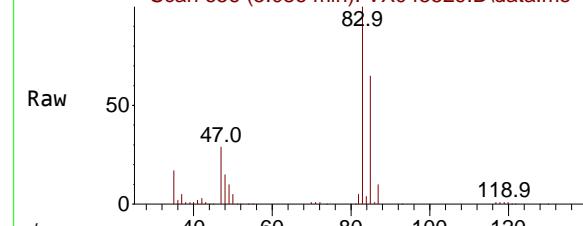

Abundance Scan 656 (5.086 min): VX045529.D\data.ms (-60)

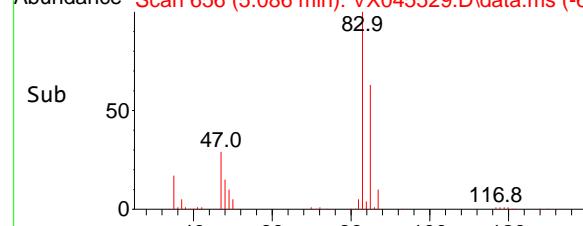

#30

Chloroform

Concen: 100.255 ug/l

RT: 5.086 min Scan# 656

Delta R.T. 0.000 min

Lab File: VX045529.D


Acq: 01 Apr 2025 18:38




Tgt Ion: 83 Resp: 225402

Ion Ratio Lower Upper

83 100

85 65.1 52.8 79.2

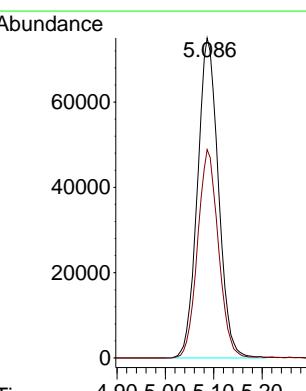



#31

Cyclohexane

Concen: 102.056 ug/l

RT: 5.458 min Scan# 718

Delta R.T. -0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

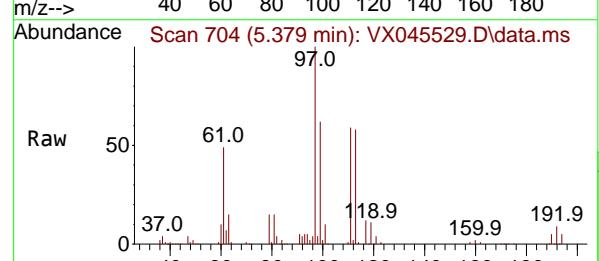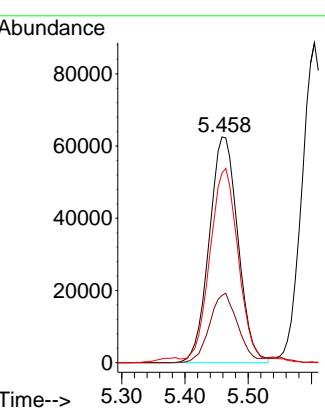

#32

1,1,1-Trichloroethane

Concen: 104.346 ug/l


RT: 5.379 min Scan# 704







Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt	Ion	Resp:	198511
Ion	Ratio	Lower	Upper
97	100		
99	64.1	51.7	77.5
61	50.2	41.0	61.4

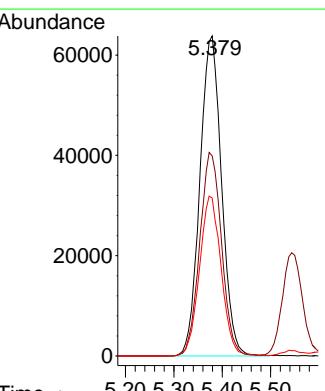

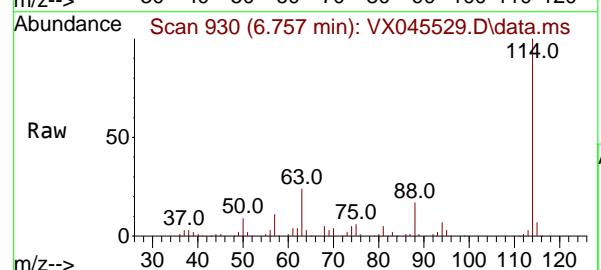

#33

1,2-Dichloroethane-d4

Concen: 98.914 ug/l

RT: 5.946 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**


Reviewed By :Amit Patel 04/02/2025







Supervised By :Mahesh Dadoda 04/02/2025

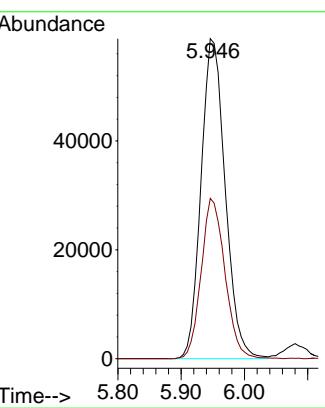

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 930  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion:114 Resp: 152724  
Ion Ratio Lower Upper  
114 100  
63 24.4 0.0 46.8  
88 16.6 0.0 35.4

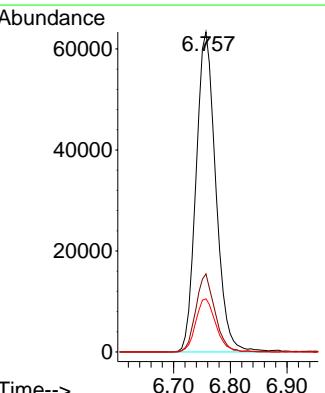



#35

Dibromofluoromethane

Concen: 99.585 ug/l

RT: 5.379 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#36

1,1-Dichloropropene

Concen: 103.515 ug/l

RT: 5.684 min Scan# 754

Delta R.T. 0.000 min


Lab File: VX045529.D







Acq: 01 Apr 2025 18:38

Tgt Ion: 75 Resp: 151448

Ion Ratio Lower Upper

75	100		
110	32.8	16.9	50.6
77	30.4	25.0	37.4

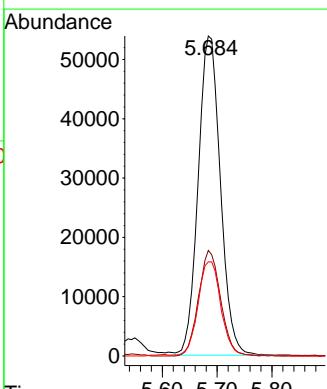

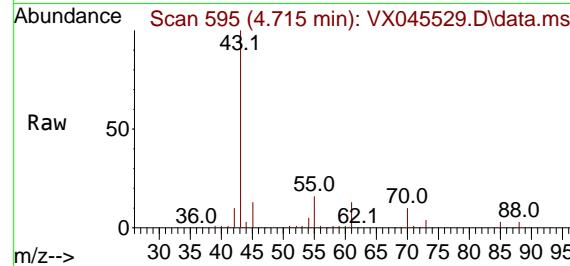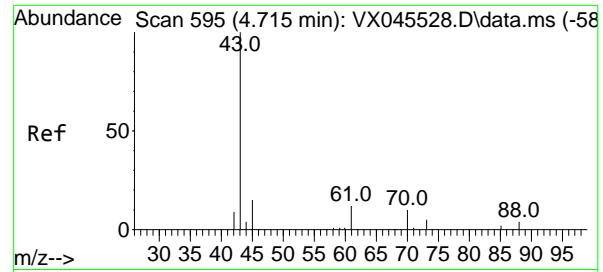

#37

**Ethyl Acetate**

Concen: 104.207 ug/l

RT: 4.715 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations****APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#38

**Carbon Tetrachloride**

Concen: 105.278 ug/l

RT: 5.672 min Scan# 752

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion:117 Resp: 166465




Ion Ratio Lower Upper

117 100

119 95.5 76.9 115.3

121 30.9 24.2 36.2



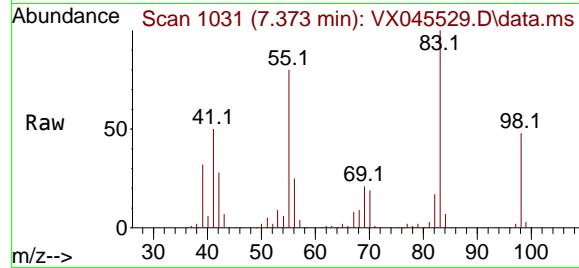

#39

Methylcyclohexane

Concen: 106.921 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**



Reviewed By :Amit Patel 04/02/2025







Supervised By :Mahesh Dadoda 04/02/2025



#40  
Benzene  
Concen: 101.369 ug/l  
RT: 6.031 min Scan# 811  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 78 Resp: 452946  
Ion Ratio Lower Upper  
78 100  
77 23.9 19.0 28.6





#41

Methacrylonitrile

Concen: 109.068 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Instrument : MSVOA\_X

ClientSampleId : VSTDICC100

**Manual Integrations  
APPROVED**


Reviewed By :Amit Patel 04/02/2025







Supervised By :Mahesh Dadoda 04/02/2025

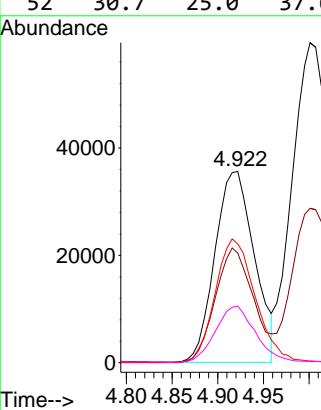

#42  
1,2-Dichloroethane  
Concen: 102.696 ug/l  
RT: 6.080 min Scan# 819  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 62 Resp: 189528  
Ion Ratio Lower Upper  
62 100  
98 7.4 0.0 15.2

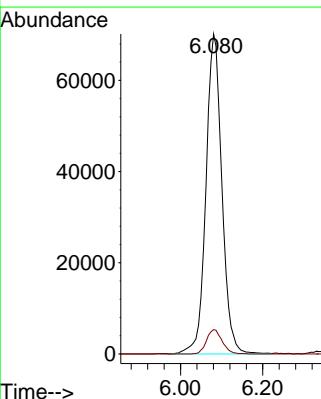

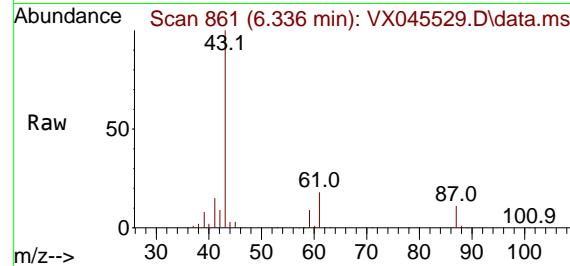

#43

Isopropyl Acetate

Concen: 109.494 ug/l

RT: 6.336 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#44

Trichloroethene

Concen: 101.062 ug/l

RT: 7.123 min Scan# 990

Delta R.T. 0.000 min

Lab File: VX045529.D


Acq: 01 Apr 2025 18:38




Tgt Ion:130 Resp: 107332

Ion Ratio Lower Upper

130 100

95 104.4 0.0 202.0

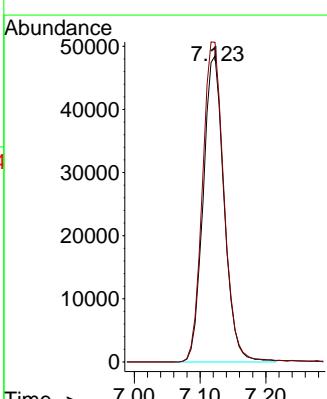



#45

1,2-Dichloropropane

Concen: 103.806 ug/l

RT: 7.421 min Scan# 1040

Delta R.T. -0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

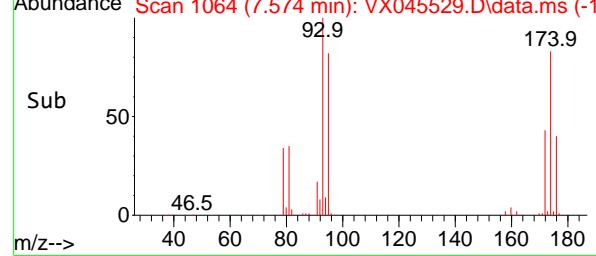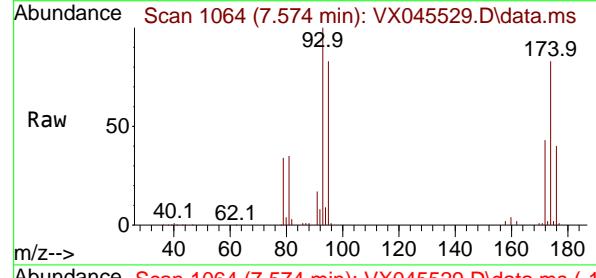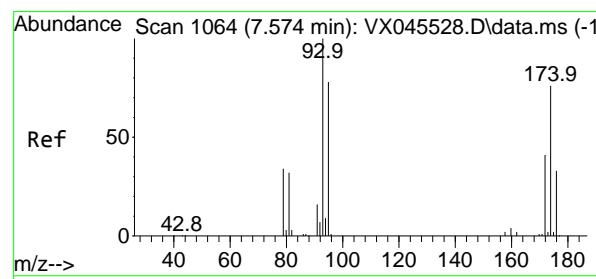

#46

Dibromomethane

Concen: 102.101 ug/l

RT: 7.574 min Scan# 1064

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion: 93 Resp: 87381



Ion Ratio Lower Upper

93 100

95 83.4 64.8 97.2

174 84.4 65.4 98.0

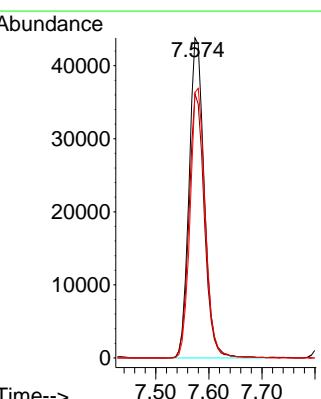

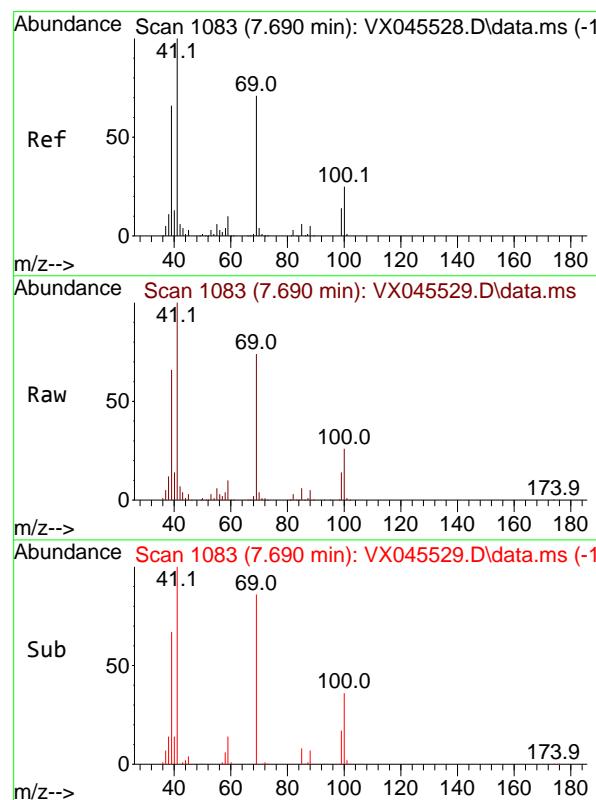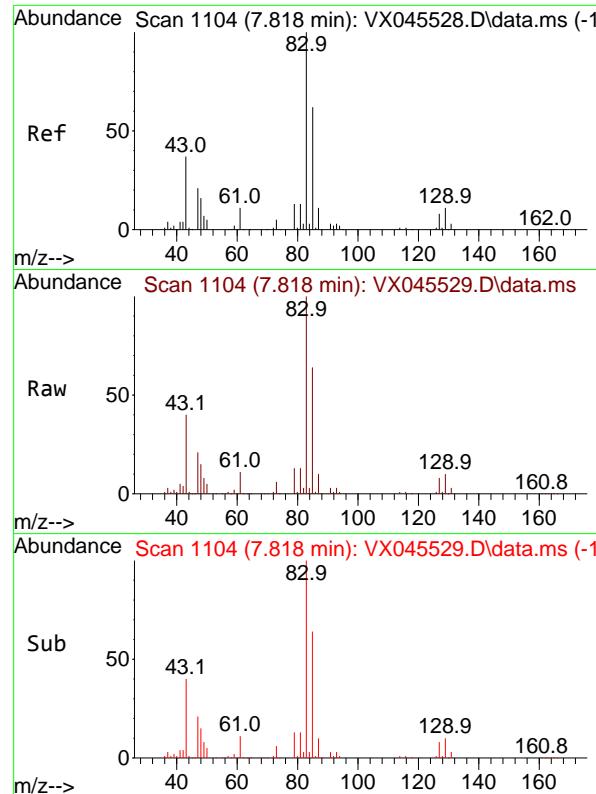

#47

Bromodichloromethane

Concen: 104.886 ug/l

RT: 7.818 min Scan# 1104

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100

Tgt Ion: 83 Resp: 179265

Ion Ratio Lower Upper

83 100

85 63.8 49.7 74.5


127 8.2 6.1 9.1

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

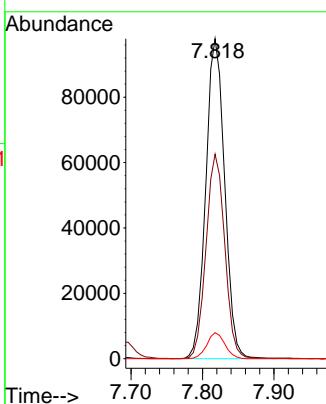

#48

Methyl methacrylate

Concen: 109.675 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion: 41 Resp: 158241







Ion Ratio Lower Upper

41 100

69 73.5 58.2 87.2

39 65.9 53.6 80.4

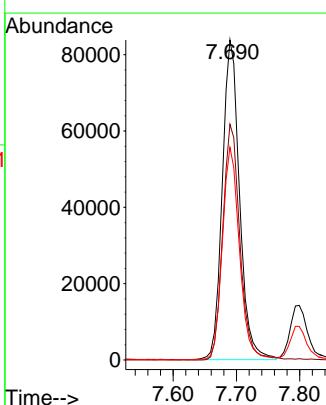

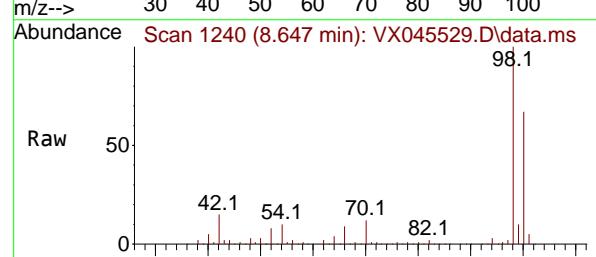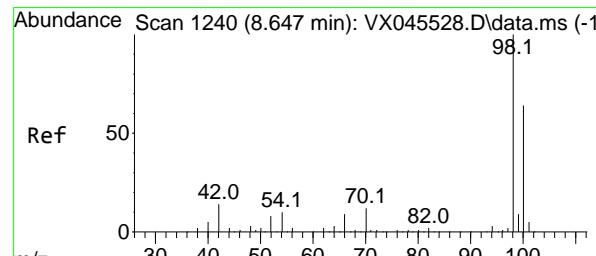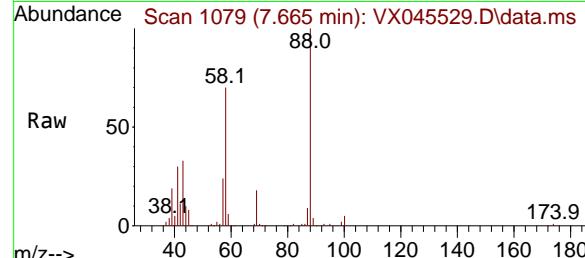

#49

1,4-Dioxane

Concen: 2015.906 ug/l

RT: 7.665 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#50

Toluene-d8

Concen: 99.309 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX045529.D


Acq: 01 Apr 2025 18:38







Tgt Ion: 98 Resp: 375599

Ion Ratio Lower Upper

98 100

100 65.7 52.2 78.4

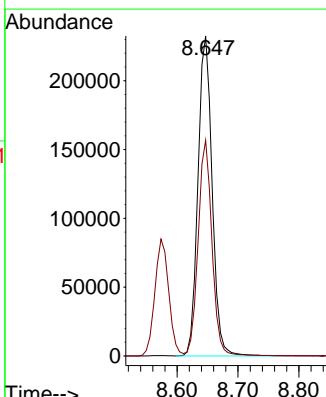

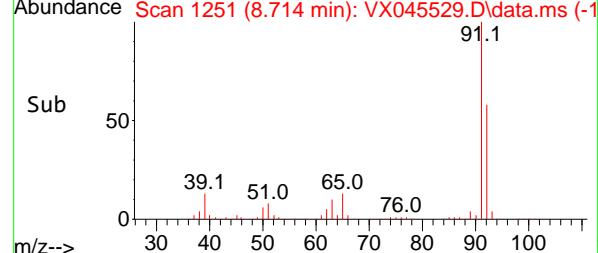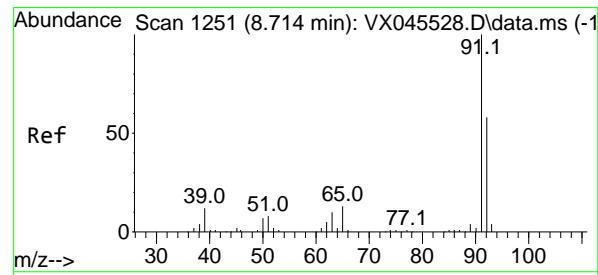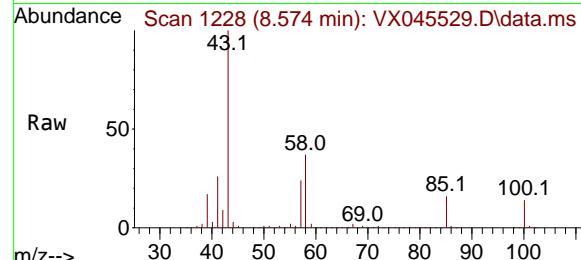

#51

4-Methyl-2-Pentanone

Concen: 533.814 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

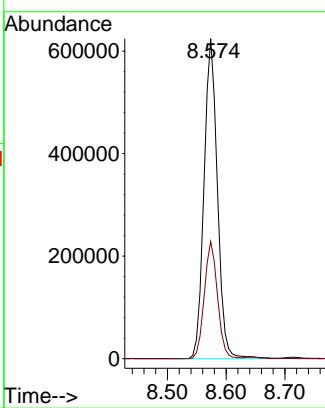

#52

Toluene

Concen: 102.199 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX045529.D


Acq: 01 Apr 2025 18:38




Tgt Ion: 92 Resp: 276323

Ion Ratio Lower Upper

92 100

91 172.5 138.7 208.1

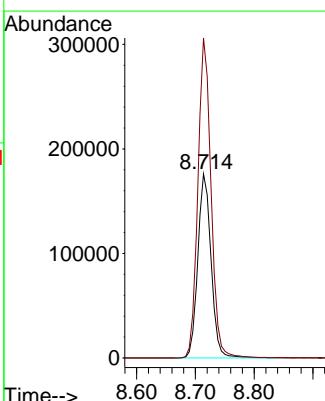



#53

t-1,3-Dichloropropene

Concen: 100.645 ug/l

RT: 8.976 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

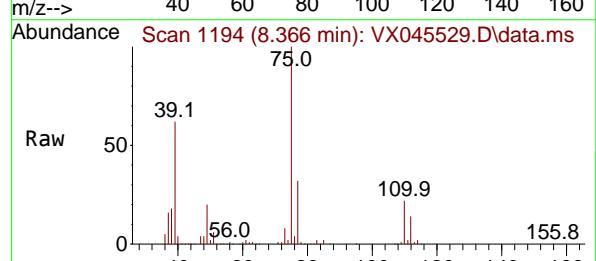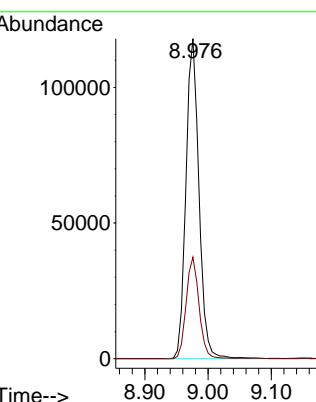

#54

cis-1,3-Dichloropropene

Concen: 113.521 ug/l

RT: 8.366 min Scan# 1194


Delta R.T. 0.000 min




Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt Ion: 75 Resp: 182328

Ion	Ratio	Lower	Upper
75	100		
77	31.6	24.6	36.8
39	61.4	48.4	72.6

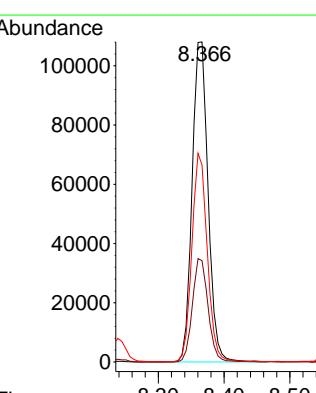






#55

1,1,2-Trichloroethane  
Concen: 101.361 ug/l  
RT: 9.147 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100

### Manual Integrations APPROVED



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025





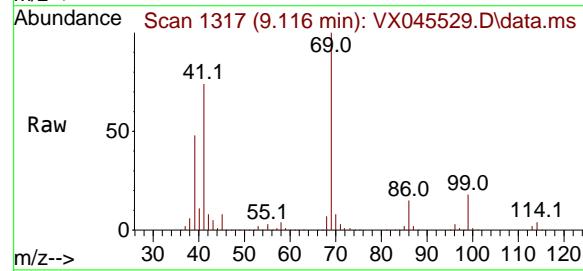



#56

Ethyl methacrylate  
Concen: 115.168 ug/l  
RT: 9.116 min Scan# 1317  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 69 Resp: 192034  
Ion Ratio Lower Upper  
69 100  
41 76.5 61.3 91.9  
39 49.0 40.2 60.2



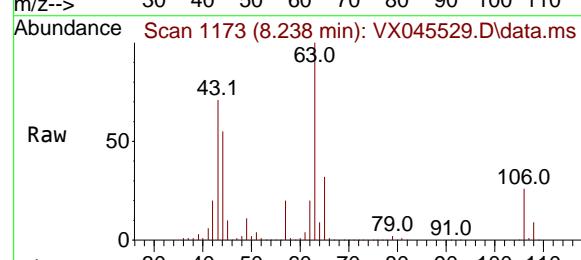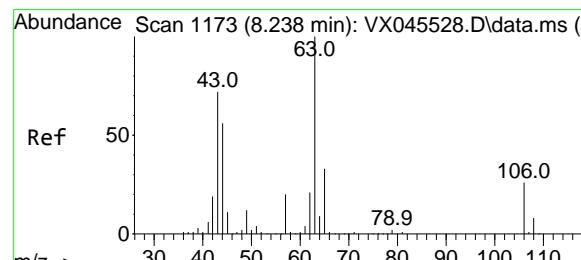

#57

1,3-Dichloropropane

Concen: 102.588 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

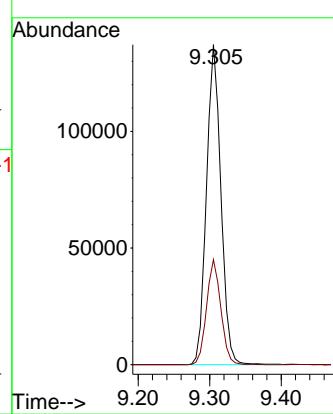

#58

2-Chloroethyl Vinyl ether

Concen: 545.696 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. 0.000 min

Lab File: VX045529.D


Acq: 01 Apr 2025 18:38







Tgt Ion: 63 Resp: 460297

Ion Ratio Lower Upper

63 100

106 26.4 21.0 31.6



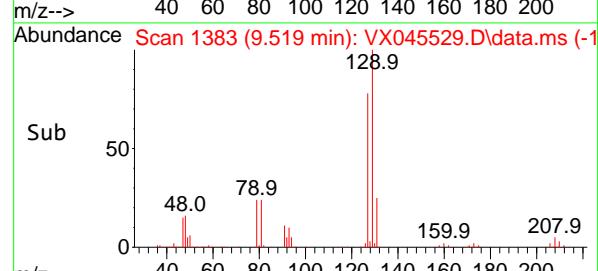

#59

2-Hexanone

Concen: 538.538 ug/l

RT: 9.427 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

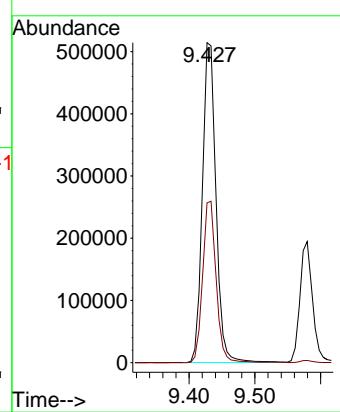

#60

Dibromochloromethane

Concen: 109.570 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045529.D


Acq: 01 Apr 2025 18:38




Tgt Ion:129 Resp: 128700

Ion Ratio Lower Upper

129 100

127 76.8 39.4 118.2

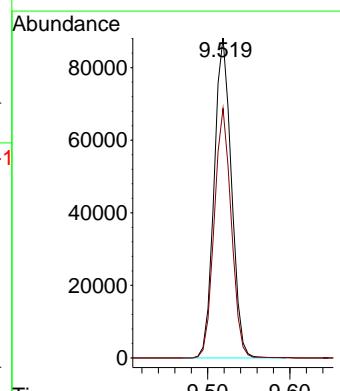

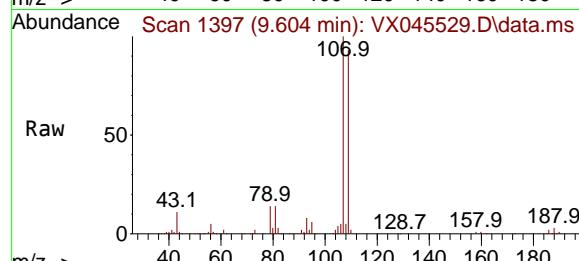

#61

1,2-Dibromoethane

Concen: 106.282 ug/l

RT: 9.604 min Scan# 1397

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

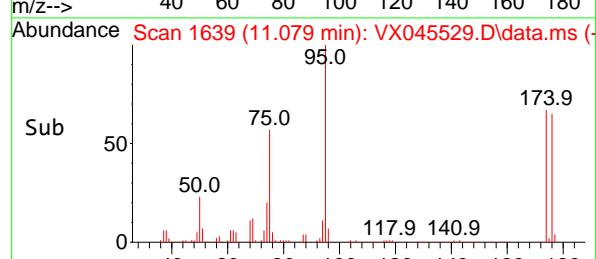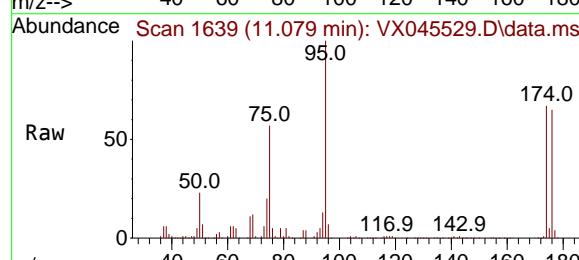

#62

4-Bromofluorobenzene

Concen: 106.664 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion: 95 Resp: 146944


Ion Ratio Lower Upper

95 100

174 67.8 0.0 135.8

176 64.7 0.0 131.4




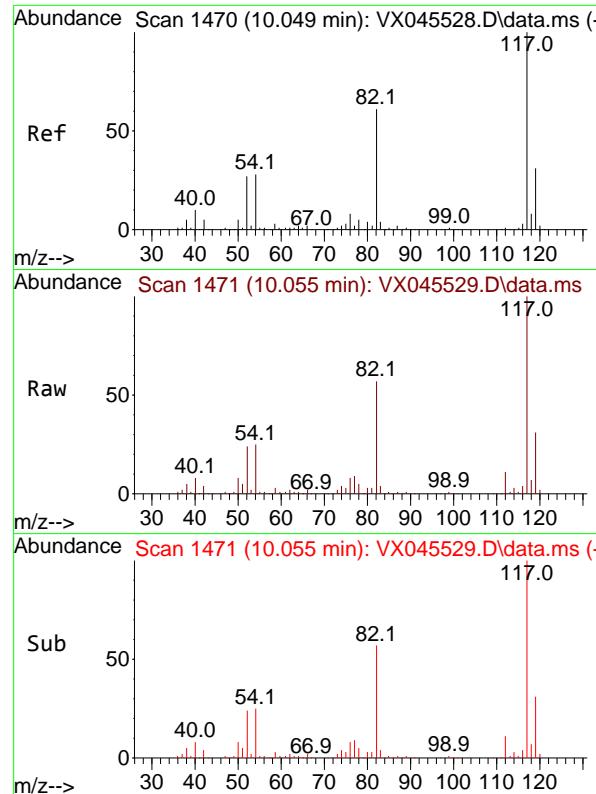


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1470  
Delta R.T. 0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

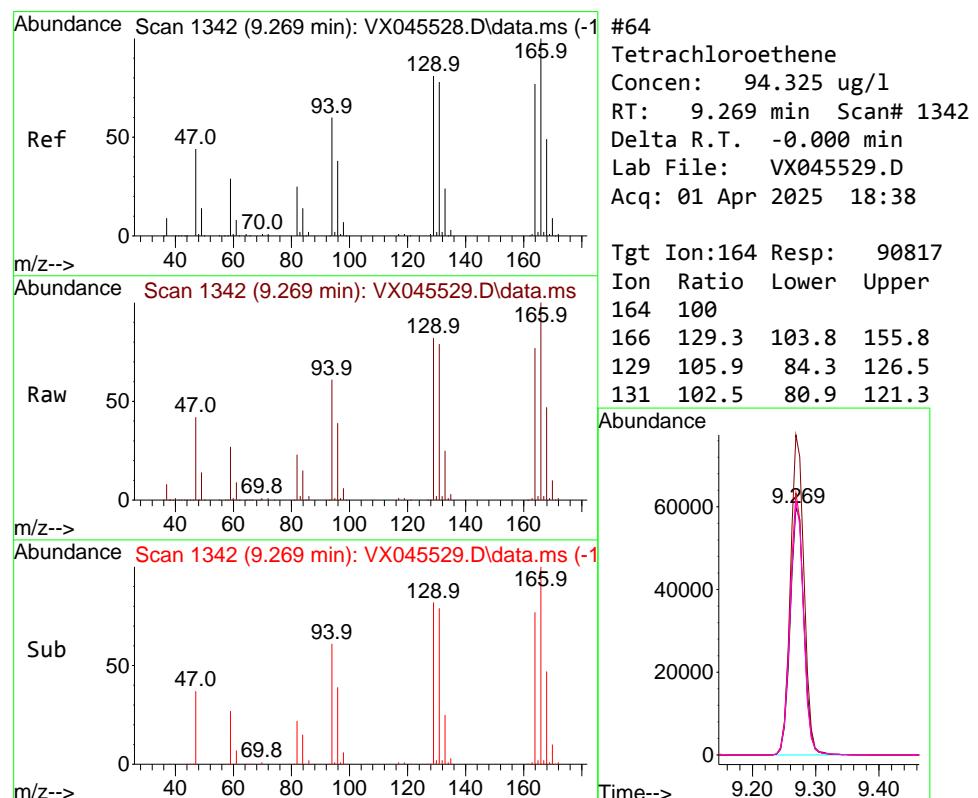

#64  
Tetrachloroethene  
Concen: 94.325 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion:164 Resp: 90817  
Ion Ratio Lower Upper  
164 100  
166 129.3 103.8 155.8  
129 105.9 84.3 126.5  
131 102.5 80.9 121.3

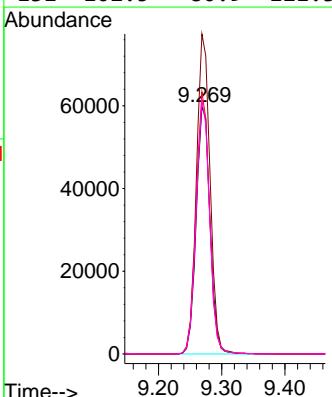

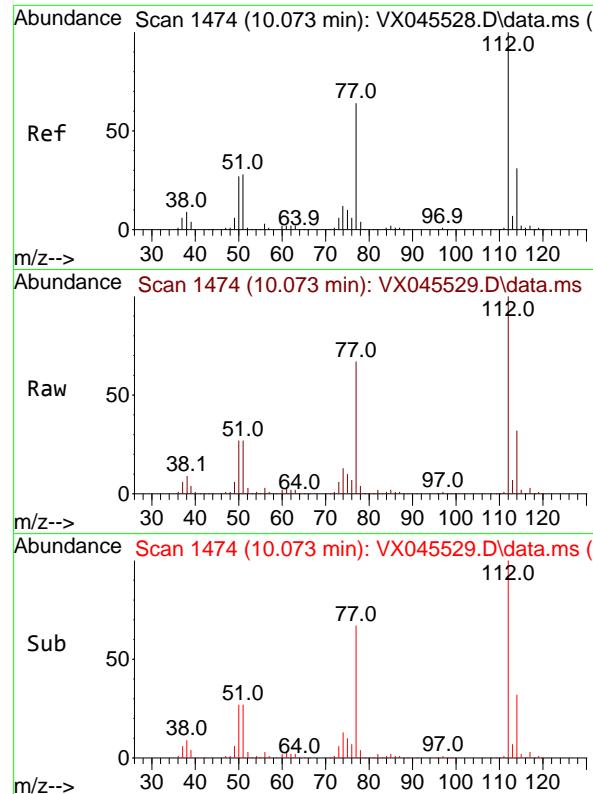

#65

Chlorobenzene

Concen: 101.682 ug/l

RT: 10.073 min Scan# 1474

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100

Tgt Ion:112 Resp: 296300

Ion Ratio Lower Upper

112 100



114 31.9 24.7 37.1

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

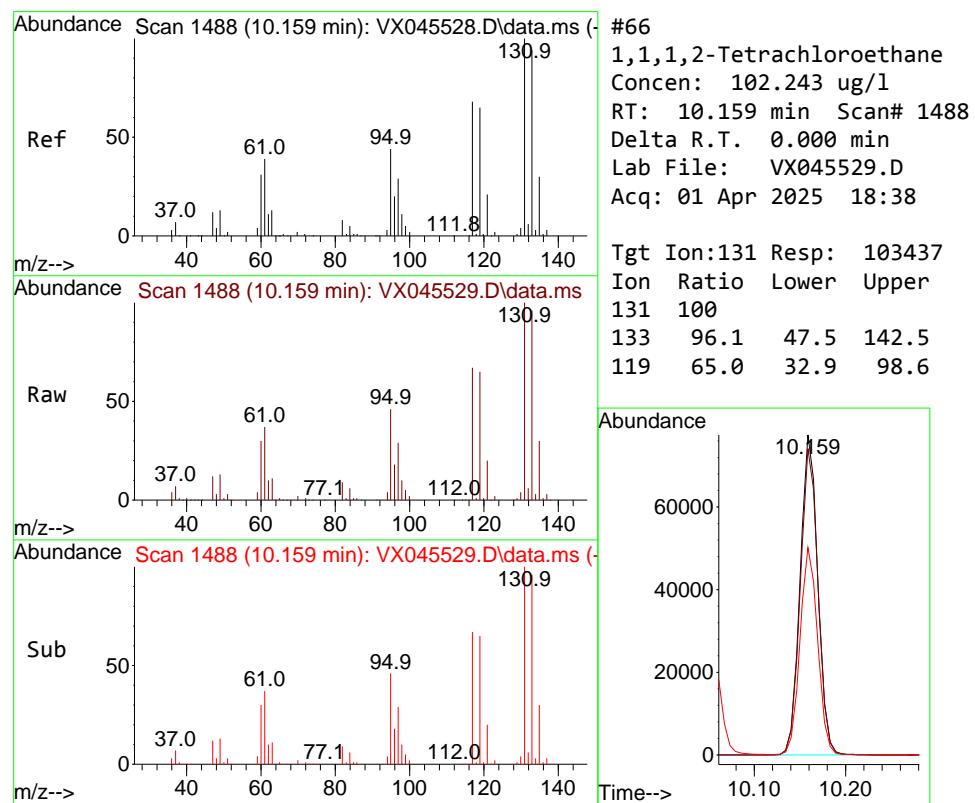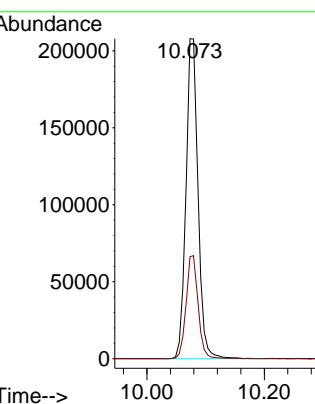

#66

1,1,1,2-Tetrachloroethane

Concen: 102.243 ug/l

RT: 10.159 min Scan# 1488

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion:131 Resp: 103437




Ion Ratio Lower Upper

131 100

133 96.1 47.5 142.5

119 65.0 32.9 98.6

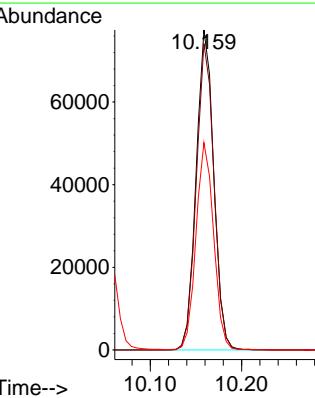

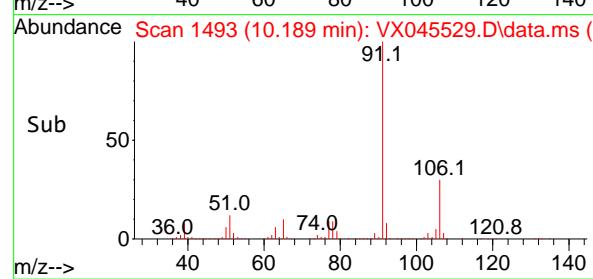

#67

Ethyl Benzene

Concen: 104.152 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#68

m/p-Xylenes

Concen: 207.694 ug/l


RT: 10.299 min Scan# 1511


Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt Ion: 106 Resp: 394241  
 Ion Ratio Lower Upper  
 106 100  
 91 216.1 172.6 258.8

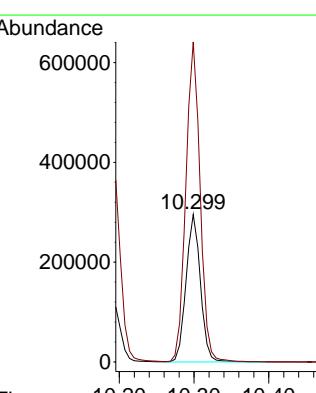

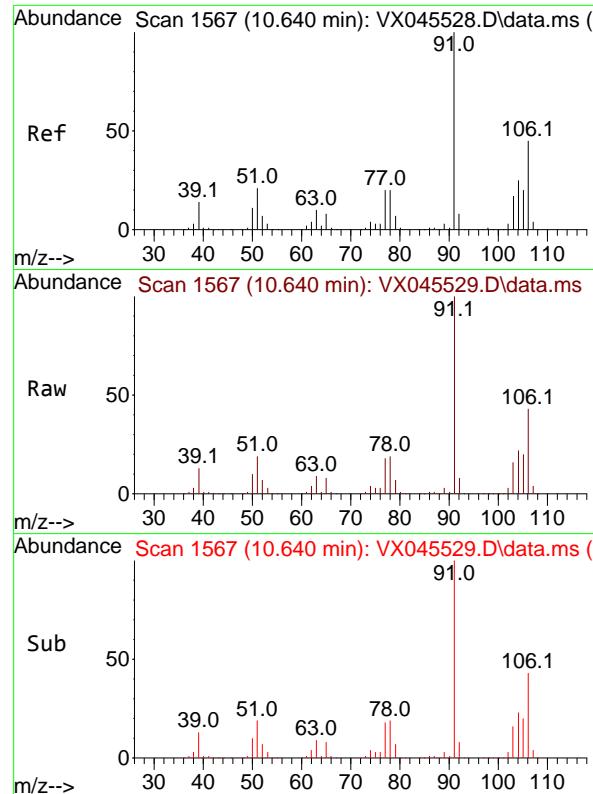


#69  
o-Xylene  
Concen: 104.487 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38  
ClientSampleId : VSTDICC100

Tgt Ion:106 Resp: 19538  
Ion Ratio Lower Upper  
106 100  
91 228.0 113.6 340.6


**Manual Integrations**  
**APPROVED**




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

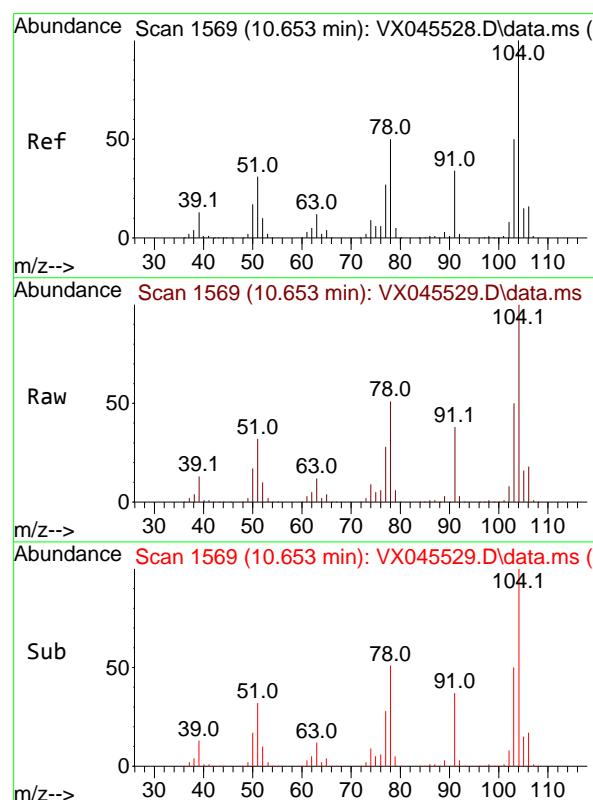

#70  
Styrene  
Concen: 108.654 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion:104 Resp: 335333  
Ion Ratio Lower Upper  
104 100  
78 57.0 45.4 68.2  
103 54.7 43.8 65.8

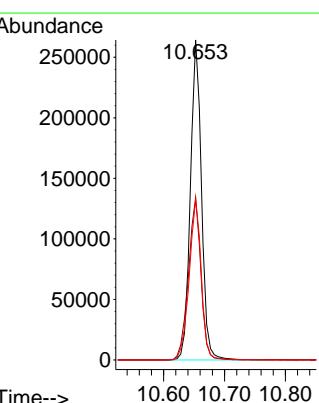

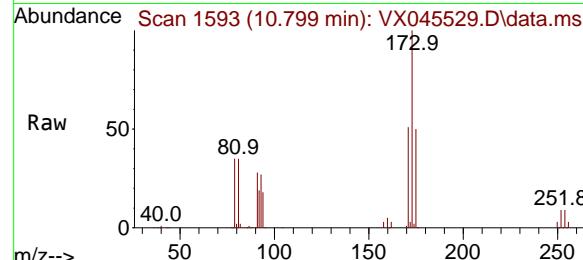

#71

Bromoform

Concen: 110.714 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

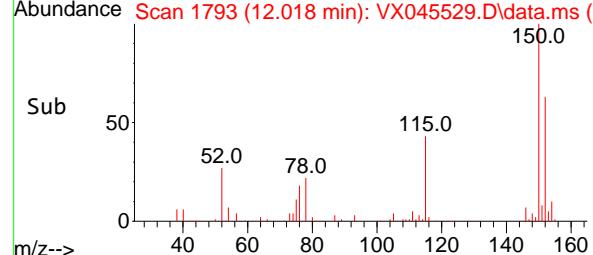

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion:152 Resp: 64612


Ion Ratio Lower Upper

152 100

115 121.0 46.9 140.7

150 188.4 0.0 349.4

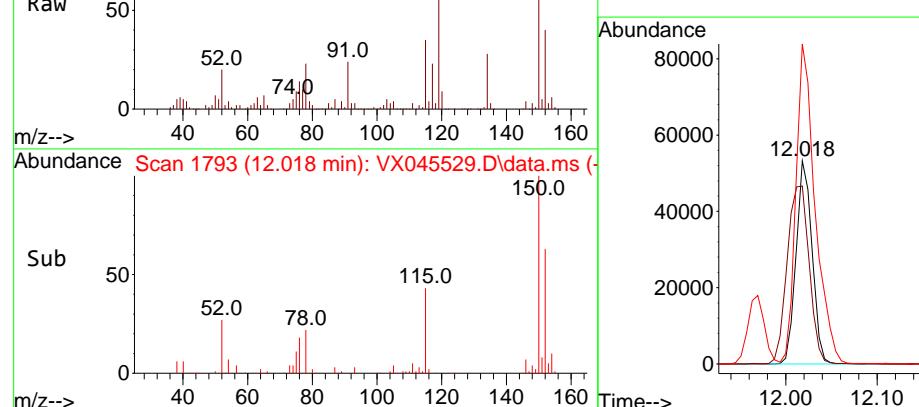

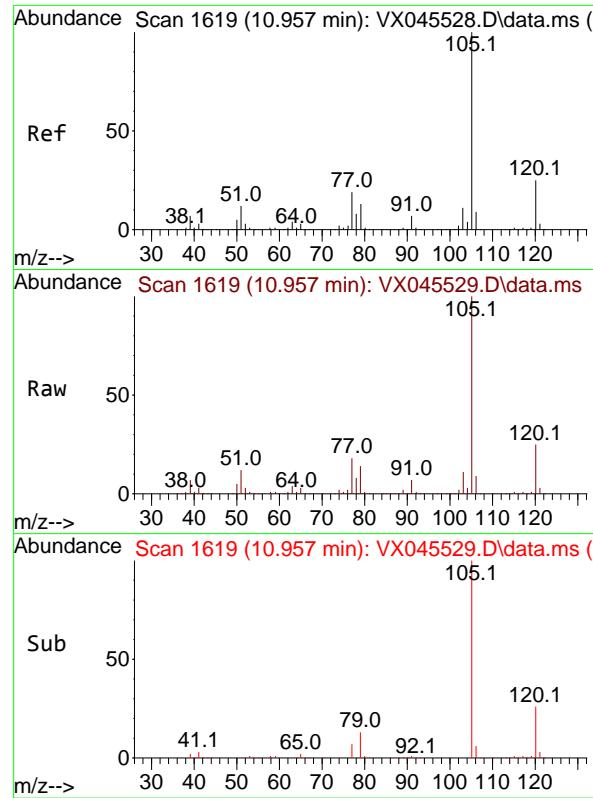

#73

Isopropylbenzene

Concen: 100.944 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

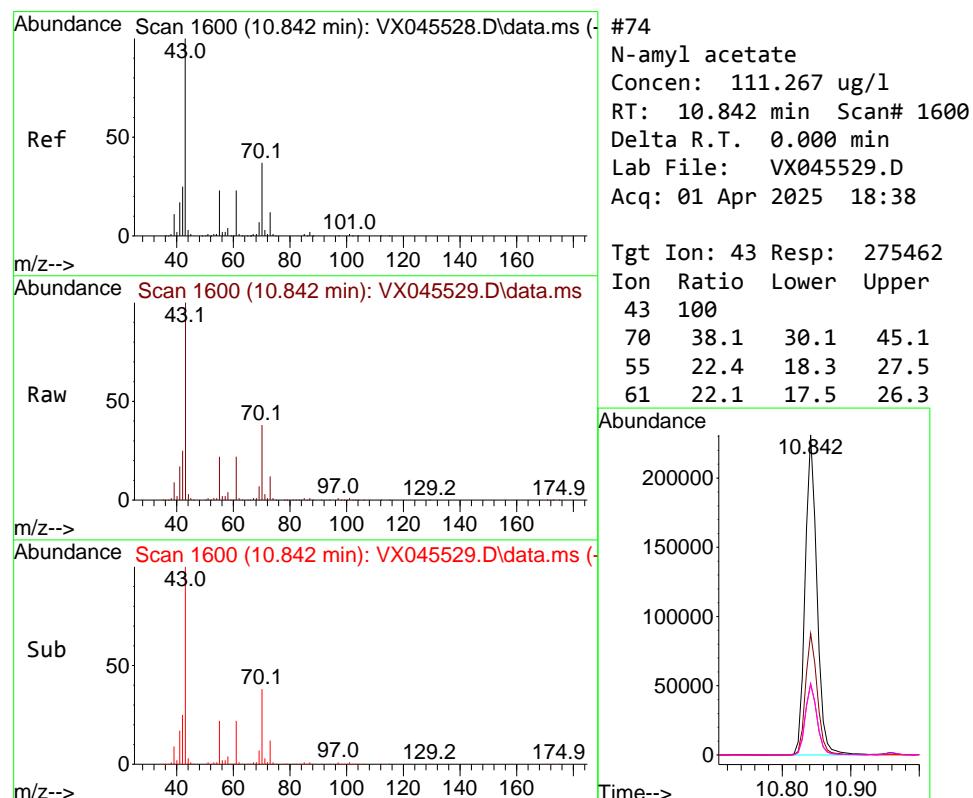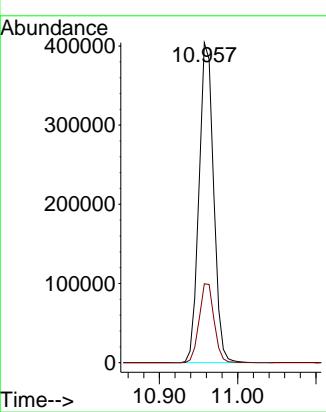

#74

N-amyl acetate

Concen: 111.267 ug/l


RT: 10.842 min Scan# 1600


Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt	Ion:	Resp:	
	43	275462	
	100		
43	100		
70	38.1	30.1	45.1
55	22.4	18.3	27.5
61	22.1	17.5	26.3

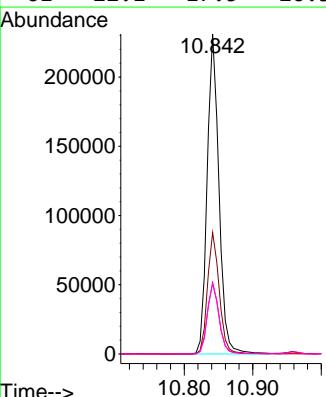


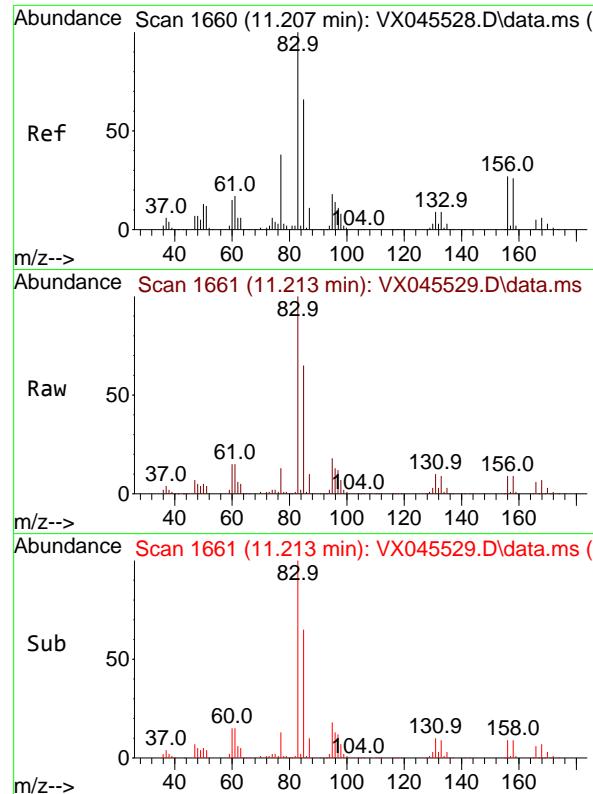


#75  
1,1,2,2-Tetrachloroethane  
Concen: 96.243 ug/l  
RT: 11.213 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

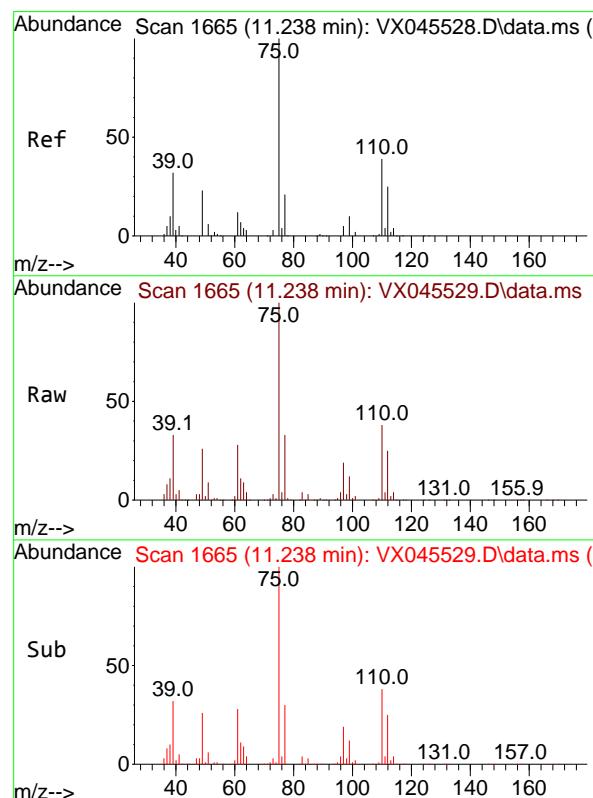

#76  
1,2,3-Trichloropropane  
Concen: 97.744 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 75 Resp: 154048  
Ion Ratio Lower Upper  
75 100  
77 41.8 20.0 59.9





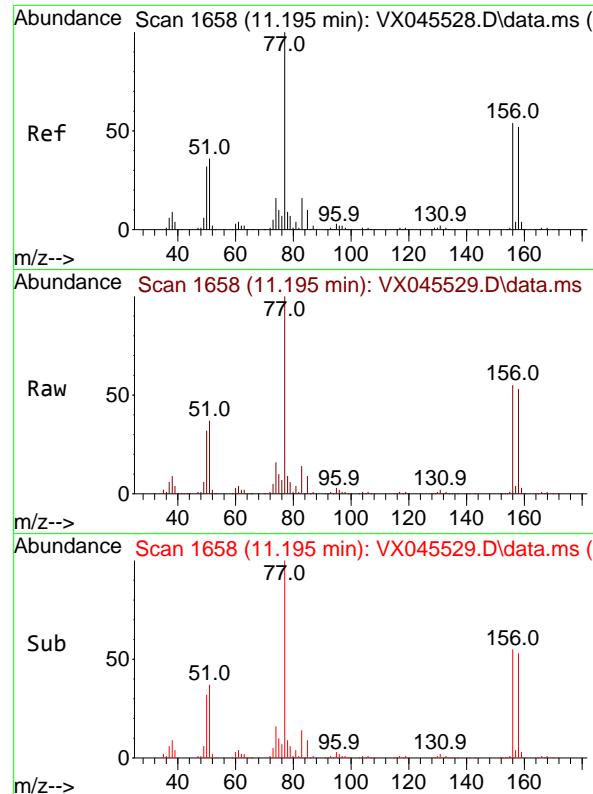

#77  
Bromobenzene  
Concen: 99.983 ug/l  
RT: 11.195 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
ClientSampleId : VSTDICC100  
Acq: 01 Apr 2025 18:38


**Manual Integrations**  
**APPROVED**




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

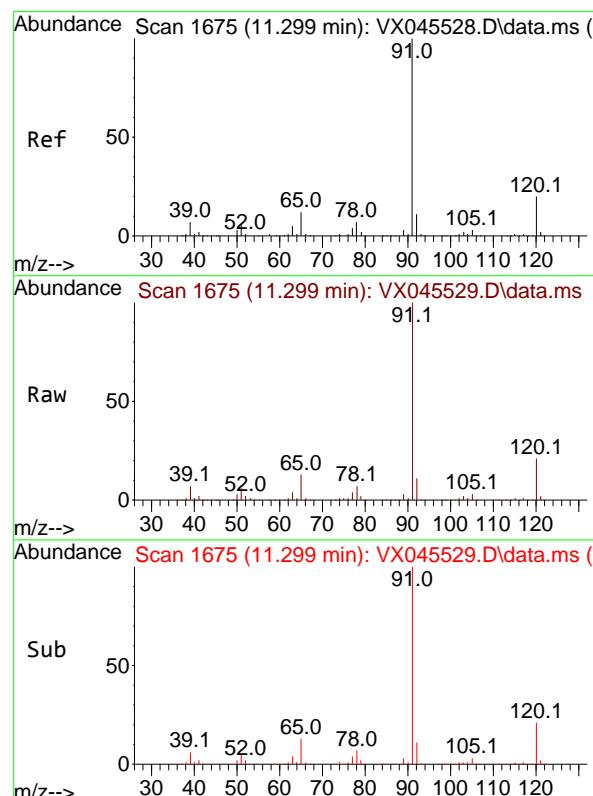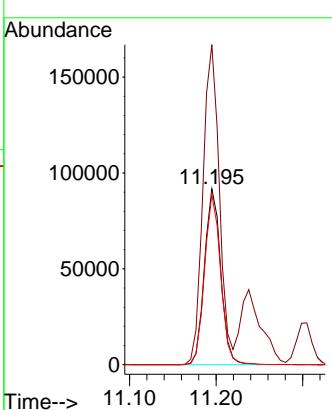

#78  
n-propylbenzene  
Concen: 104.454 ug/l  
RT: 11.299 min Scan# 1675  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 91 Resp: 622679  
Ion Ratio Lower Upper  
91 100  
120 21.5 10.8 32.3

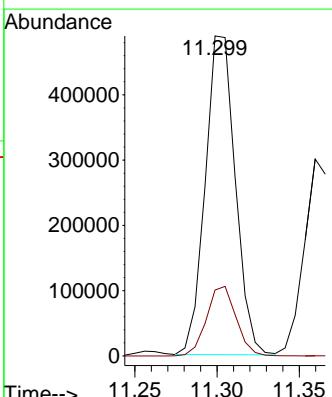



#79

2-Chlorotoluene

Concen: 98.840 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

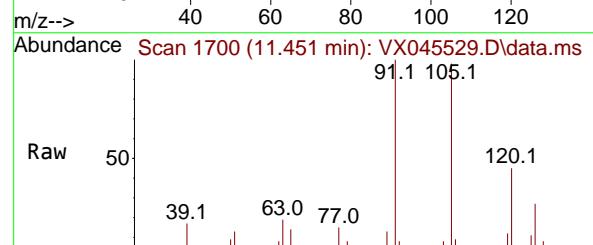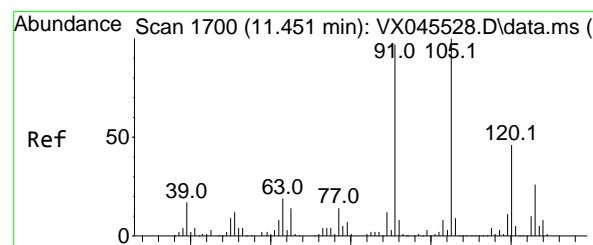

#80

1,3,5-Trimethylbenzene

Concen: 101.675 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045529.D


Acq: 01 Apr 2025 18:38


Tgt Ion:105 Resp: 435137

Ion Ratio Lower Upper

105 100

120 45.9 23.0 69.0

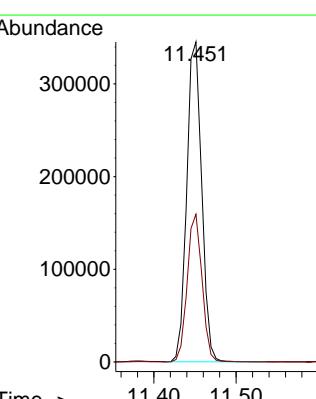

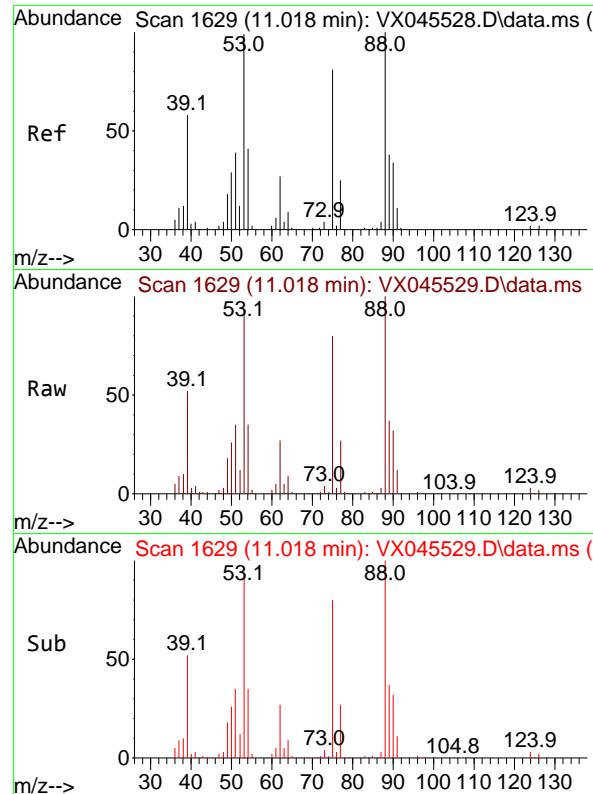


#81  
trans-1,4-Dichloro-2-butene  
Concen: 111.704 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

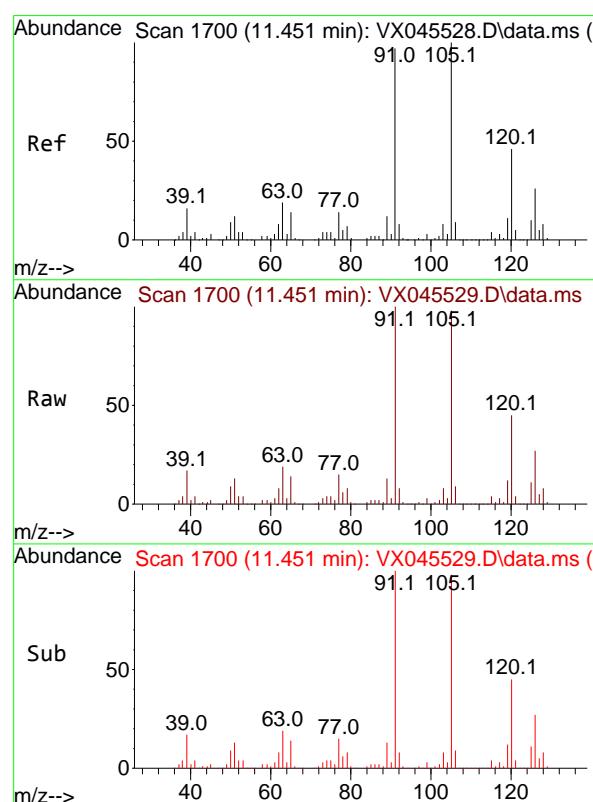

#82  
4-Chlorotoluene  
Concen: 101.877 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX045529.D  
Acq: 01 Apr 2025 18:38

Tgt Ion: 91 Resp: 432884  
Ion Ratio Lower Upper  
91 100  
126 26.9 13.3 39.9

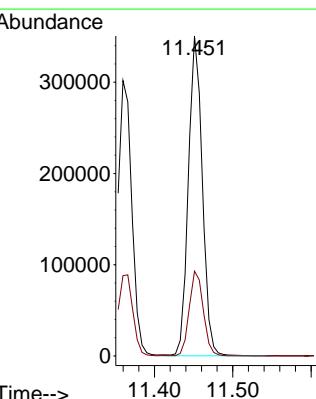

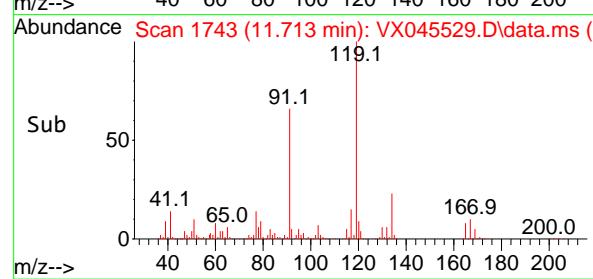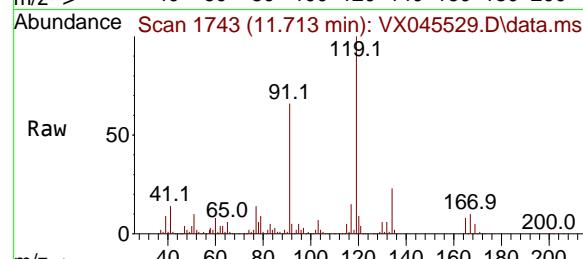

#83

tert-Butylbenzene

Concen: 103.292 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

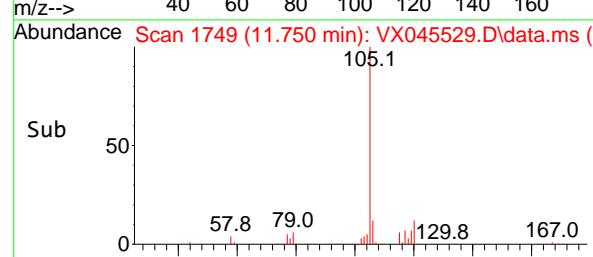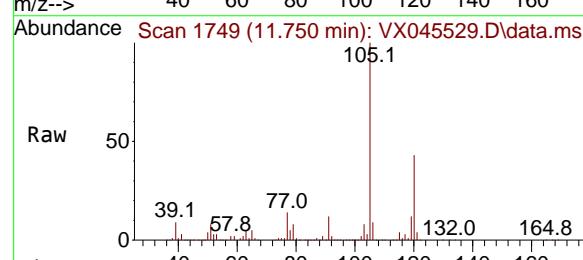

#84

1,2,4-Trimethylbenzene

Concen: 103.414 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045529.D


Acq: 01 Apr 2025 18:38




Tgt Ion:105 Resp: 444211

Ion Ratio Lower Upper

105 100

120 42.4 21.4 64.3

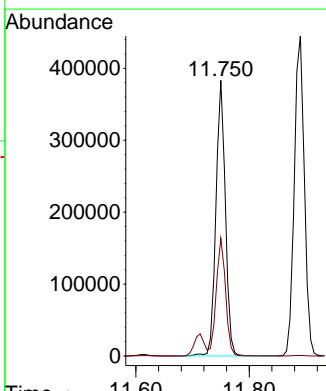



#85

sec-Butylbenzene

Concen: 105.082 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#86

p-Isopropyltoluene

Concen: 105.609 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion:119 Resp: 453109

Ion Ratio Lower Upper

119 100

134 25.1 12.6 37.8

91 27.4 13.7 41.1

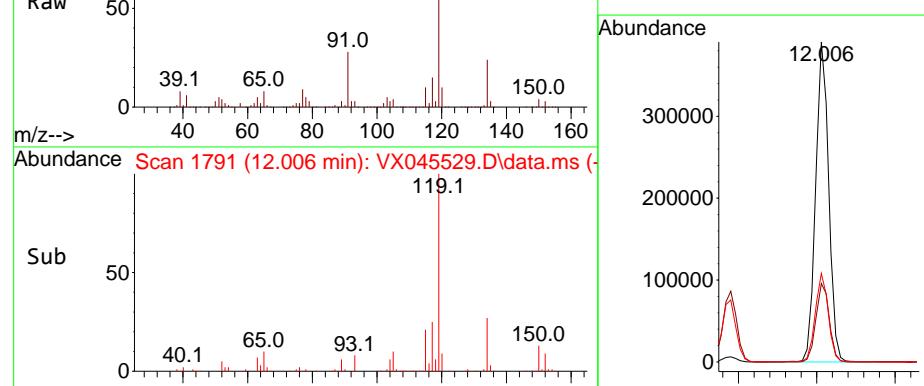

Abundance

12.006


300000

200000

100000

0

11.90 12.00 12.10

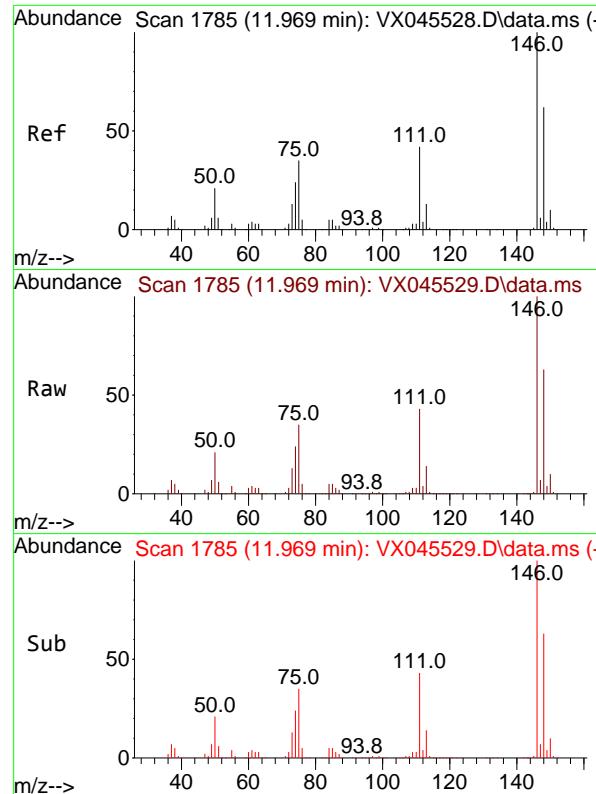

#87

1,3-Dichlorobenzene

Concen: 101.749 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

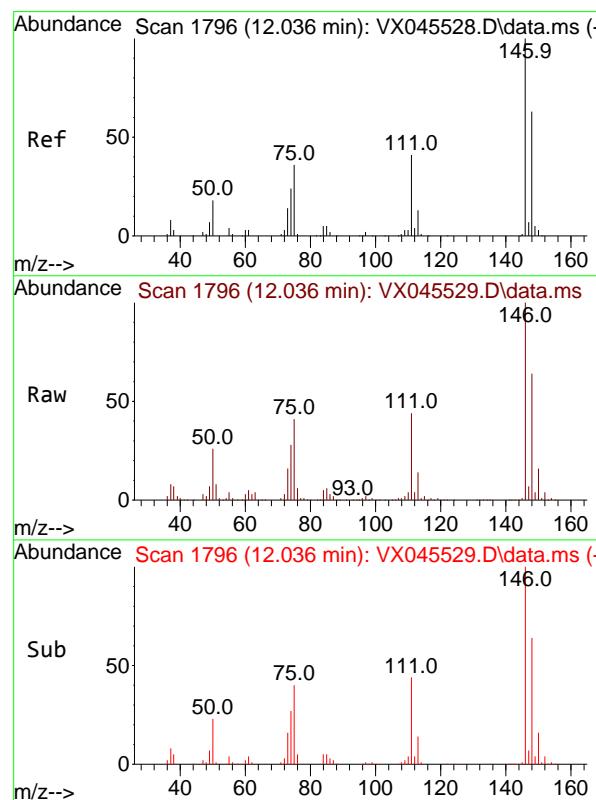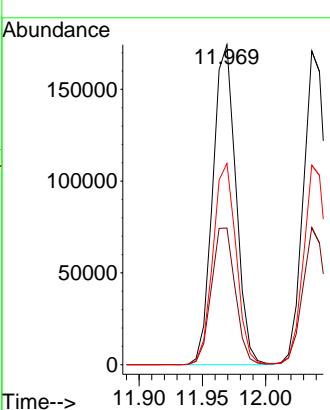

#88

1,4-Dichlorobenzene

Concen: 98.047 ug/l


RT: 12.036 min Scan# 1796




Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt	Ion:146	Resp:	216367
Ion	Ratio	Lower	Upper
146	100		
111	43.2	20.9	62.8
148	64.0	31.5	94.5

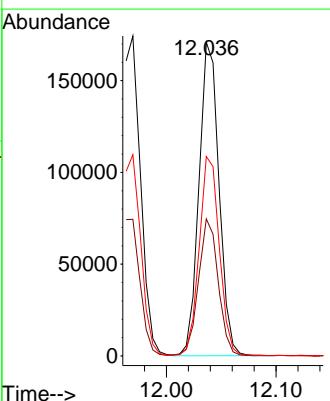



#89

n-Butylbenzene

Concen: 113.075 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

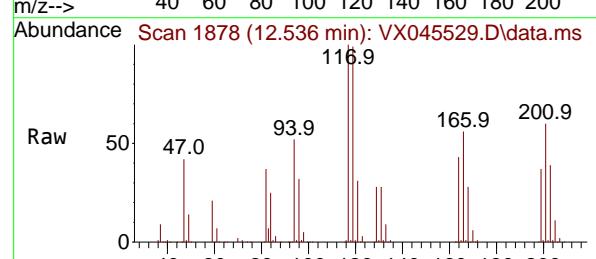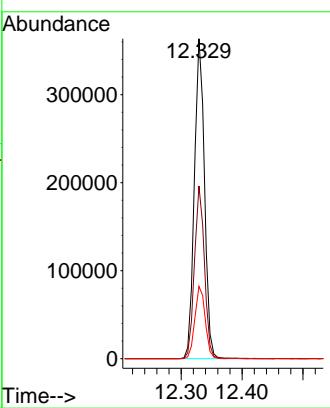

#90

Hexachloroethane

Concen: 109.160 ug/l


RT: 12.536 min Scan# 1878

Delta R.T. 0.000 min


Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
	117	100			
	201	62.1	80489	31.2	93.6

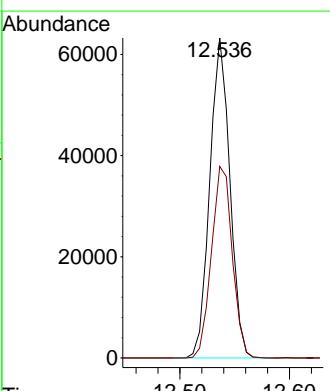



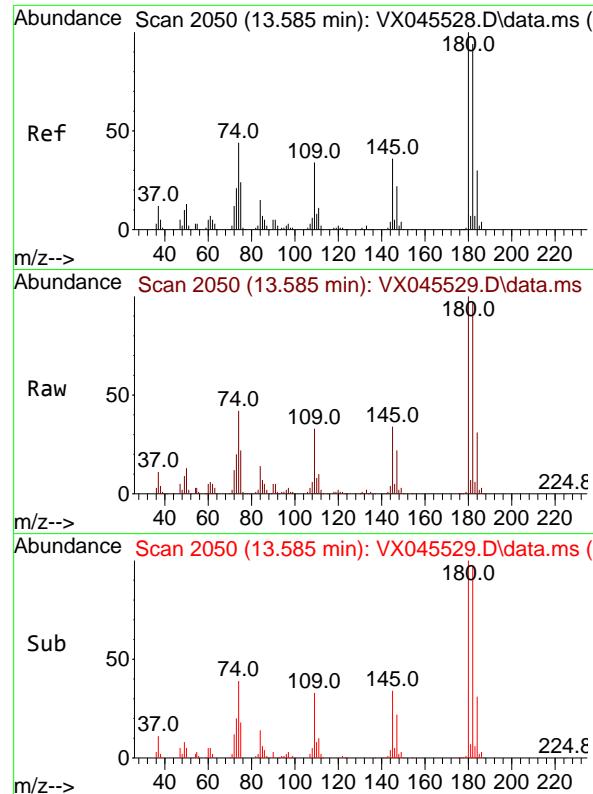

#93

1,2,4-Trichlorobenzene

Concen: 112.106 ug/l

RT: 13.585 min Scan# 2050

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

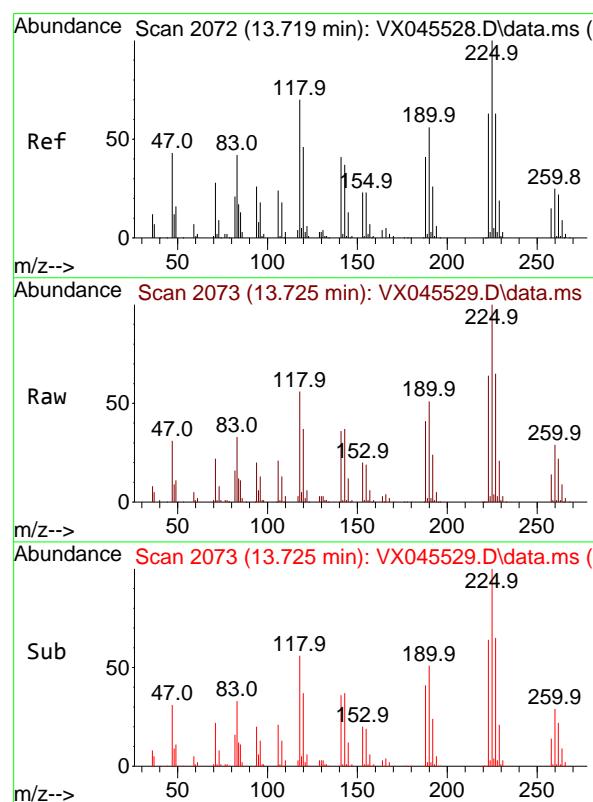

#94

Hexachlorobutadiene

Concen: 103.326 ug/l


RT: 13.725 min Scan# 2073




Delta R.T. 0.006 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Tgt	Ion:225	Resp:	53636
Ion	Ratio	Lower	Upper
225	100		
223	64.2	31.1	93.3
227	62.9	32.2	96.6

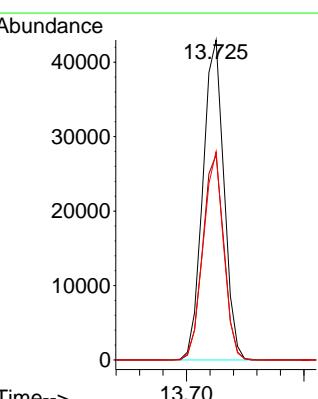

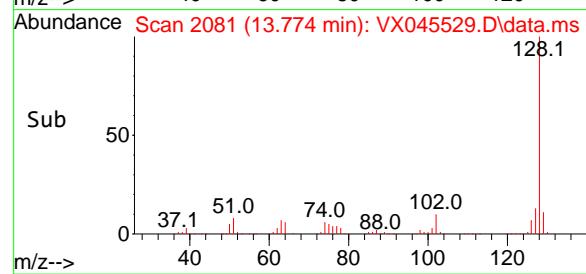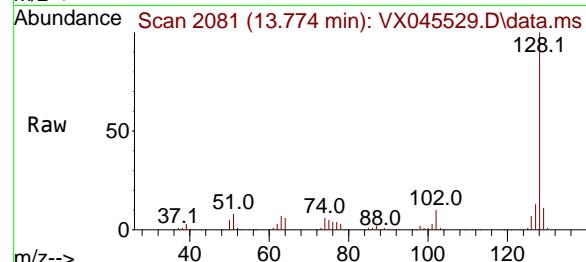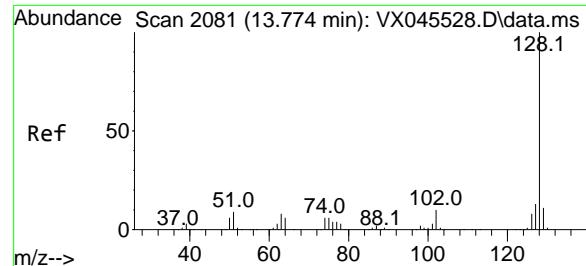

#95

Naphthalene

Concen: 111.473 ug/l

RT: 13.774 min Scan# 2111

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

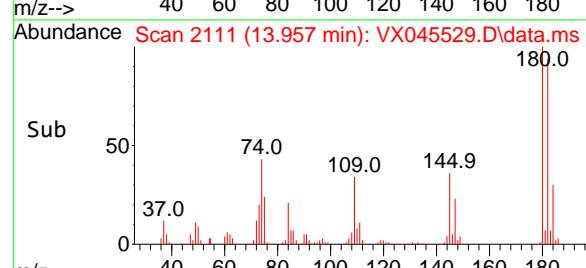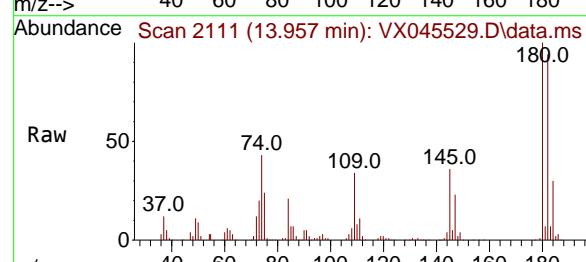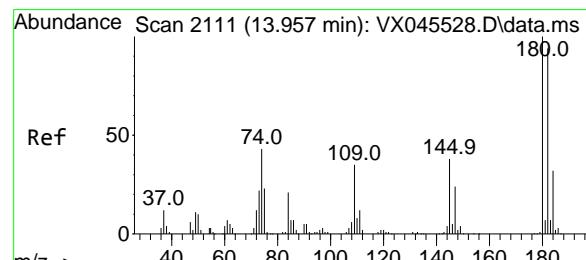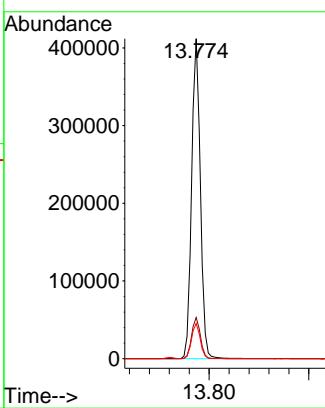

#96

1,2,3-Trichlorobenzene

Concen: 108.869 ug/l

RT: 13.957 min Scan# 2111

Delta R.T. 0.000 min

Lab File: VX045529.D

Acq: 01 Apr 2025 18:38


Tgt Ion:180 Resp: 137328

Ion Ratio Lower Upper

180 100

182 94.5 47.3 141.8

145 36.0 18.2 54.6

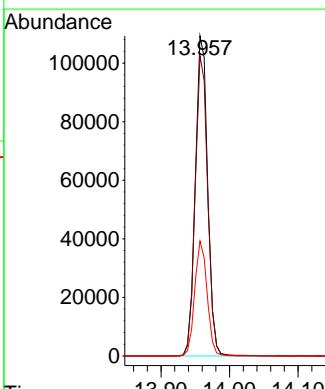

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045530.D  
 Acq On : 01 Apr 2025 19:02  
 Operator : JC/MD  
 Sample : VSTDICC150  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC150

Quant Time: Apr 02 02:54:59 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	90033	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	160037	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	133342	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	61380	50.000	ug/l	# 0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	252998	153.661	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 307.320%	#	
35) Dibromofluoromethane	5.379	113	173598	152.887	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 305.780%	#	
50) Toluene-d8	8.647	98	603264	152.216	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 304.440%	#	
62) 4-Bromofluorobenzene	11.079	95	220921	153.035	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 306.060%	#	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.167	85	221436	164.460	ug/l	100
3) Chloromethane	1.307	50	198321	143.373	ug/l	98
4) Vinyl Chloride	1.374	62	197096	155.697	ug/l	100
5) Bromomethane	1.593	94	88225	146.986	ug/l	97
6) Chloroethane	1.660	64	86251	128.421	ug/l	97
7) Trichlorofluoromethane	1.868	101	267098	141.495	ug/l	100
8) Diethyl Ether	2.136	74	96467	152.215	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.319	101	171118	154.698	ug/l	97
10) Methyl Iodide	2.441	142	202594	146.838	ug/l	99
11) Tert butyl alcohol	2.989	59	167769	758.202	ug/l	100
12) 1,1-Dichloroethene	2.307	96	166365	153.921	ug/l	97
13) Acrolein	2.239	56	232818	764.070	ug/l	100
14) Allyl chloride	2.654	41	313268	152.755	ug/l	99
15) Acrylonitrile	3.069	53	507965	727.247	ug/l	100
16) Acetone	2.386	43	479564	709.323	ug/l	99
17) Carbon Disulfide	2.502	76	443495	166.133	ug/l	99
18) Methyl Acetate	2.703	43	228558	146.832	ug/l	99
19) Methyl tert-butyl Ether	3.117	73	598532	158.301	ug/l	99
20) Methylene Chloride	2.782	84	186382	147.254	ug/l	99
21) trans-1,2-Dichloroethene	3.081	96	170283	154.210	ug/l	98
22) Diisopropyl ether	3.764	45	636728	157.617	ug/l	94
23) Vinyl Acetate	3.721	43	2911326	834.120	ug/l	100
24) 1,1-Dichloroethane	3.605	63	349040	152.778	ug/l	99
25) 2-Butanone	4.556	43	740096	747.834	ug/l	99
26) 2,2-Dichloropropane	4.465	77	252063	170.765	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	205254	152.571	ug/l	98
28) Bromochloromethane	4.891	49	155600	140.938	ug/l	97
29) Tetrahydrofuran	5.001	42	475589	741.226	ug/l	100
30) Chloroform	5.087	83	353681	150.451	ug/l	98
31) Cyclohexane	5.458	56	310219	153.595	ug/l	97
32) 1,1,1-Trichloroethane	5.373	97	315136	158.426	ug/l	98
36) 1,1-Dichloropropene	5.684	75	239776	156.399	ug/l	98
37) Ethyl Acetate	4.715	43	294559	152.461	ug/l	99
38) Carbon Tetrachloride	5.672	117	266770	161.005	ug/l	99
39) Methylcyclohexane	7.373	83	303251	161.366	ug/l	96
40) Benzene	6.031	78	703311	150.208	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045530.D  
 Acq On : 01 Apr 2025 19:02  
 Operator : JC/MD  
 Sample : VSTDICC150  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC150

Quant Time: Apr 02 02:54:59 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	164699	160.155	ug/1	98
42) 1,2-Dichloroethane	6.080	62	296168	153.146	ug/1	100
43) Isopropyl Acetate	6.336	43	475823	162.494	ug/1	99
44) Trichloroethene	7.117	130	170940	153.599	ug/1	95
45) 1,2-Dichloropropane	7.428	63	179457	153.610	ug/1	98
46) Dibromomethane	7.574	93	135415	150.996	ug/1	98
47) Bromodichloromethane	7.818	83	279881	156.272	ug/1	98
48) Methyl methacrylate	7.690	41	240818	159.281	ug/1	99
49) 1,4-Dioxane	7.659	88	74929	2739.196	ug/1	99
51) 4-Methyl-2-Pentanone	8.574	43	1414771	728.817	ug/1	99
52) Toluene	8.714	92	420015	148.245	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	267671	150.589	ug/1	98
54) cis-1,3-Dichloropropene	8.360	75	287973	171.104	ug/1	98
55) 1,1,2-Trichloroethane	9.147	97	163426	144.752	ug/1	98
56) Ethyl methacrylate	9.116	69	285895	163.624	ug/1	98
57) 1,3-Dichloropropane	9.305	76	288430	146.708	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	703881	796.340	ug/1	99
59) 2-Hexanone	9.433	43	1053971	733.198	ug/1	100
60) Dibromochloromethane	9.519	129	194342	157.895	ug/1	98
61) 1,2-Dibromoethane	9.610	107	174571	152.745	ug/1	99
64) Tetrachloroethene	9.269	164	138926	147.568	ug/1	98
65) Chlorobenzene	10.080	112	444631	156.049	ug/1	98
66) 1,1,1,2-Tetrachloroethane	10.159	131	156069	157.769	ug/1	99
67) Ethyl Benzene	10.189	91	821130	160.907	ug/1	99
68) m/p-Xylenes	10.299	106	583228	314.231	ug/1	99
69) o-Xylene	10.640	106	285670	156.241	ug/1	100
70) Styrene	10.653	104	480722	159.299	ug/1	99
71) Bromoform	10.799	173	126115	170.743	ug/1 #	98
73) Isopropylbenzene	10.957	105	764406	155.475	ug/1	100
74) N-amyl acetate	10.842	43	408934	173.877	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	249980	144.737	ug/1	100
76) 1,2,3-Trichloropropane	11.238	75	215694m	144.064	ug/1	
77) Bromobenzene	11.195	156	171573	151.033	ug/1	99
78) n-propylbenzene	11.305	91	897084	158.408	ug/1	100
79) 2-Chlorotoluene	11.360	91	537263	148.399	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	620819	152.700	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	78805	178.636	ug/1	93
82) 4-Chlorotoluene	11.451	91	615594	152.505	ug/1	99
83) tert-Butylbenzene	11.713	119	627039	155.783	ug/1	100
84) 1,2,4-Trimethylbenzene	11.750	105	629704	154.317	ug/1	100
85) sec-Butylbenzene	11.890	105	790355	159.869	ug/1	100
86) p-Isopropyltoluene	12.006	119	641521	157.397	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	314077	151.885	ug/1	100
88) 1,4-Dichlorobenzene	12.037	146	314197	149.876	ug/1	99
89) n-Butylbenzene	12.329	91	604445	171.019	ug/1	100
90) Hexachloroethane	12.536	117	121761	173.829	ug/1	99
91) 1,2-Dichlorobenzene	12.335	146	307031	149.342	ug/1	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	64317	178.062	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	199365	174.213	ug/1	99
94) Hexachlorobutadiene	13.725	225	77792	157.752	ug/1	99
95) Naphthalene	13.774	128	733300	172.191	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	201989	168.562	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045530.D  
 Acq On : 01 Apr 2025 19:02  
 Operator : JC/MD  
 Sample : VSTDICC150  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC150

Quant Time: Apr 02 02:54:59 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 02:44:48 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
Data File : VX045530.D  
Acq On : 01 Apr 2025 19:02  
Operator : JC/MD  
Sample : VSTDIICC150  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 8 Sample Multiplier: 1




Quant Time: Apr 02 02:54:59 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 02:44:48 2025  
Response via : Initial Calibration

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC150

## Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

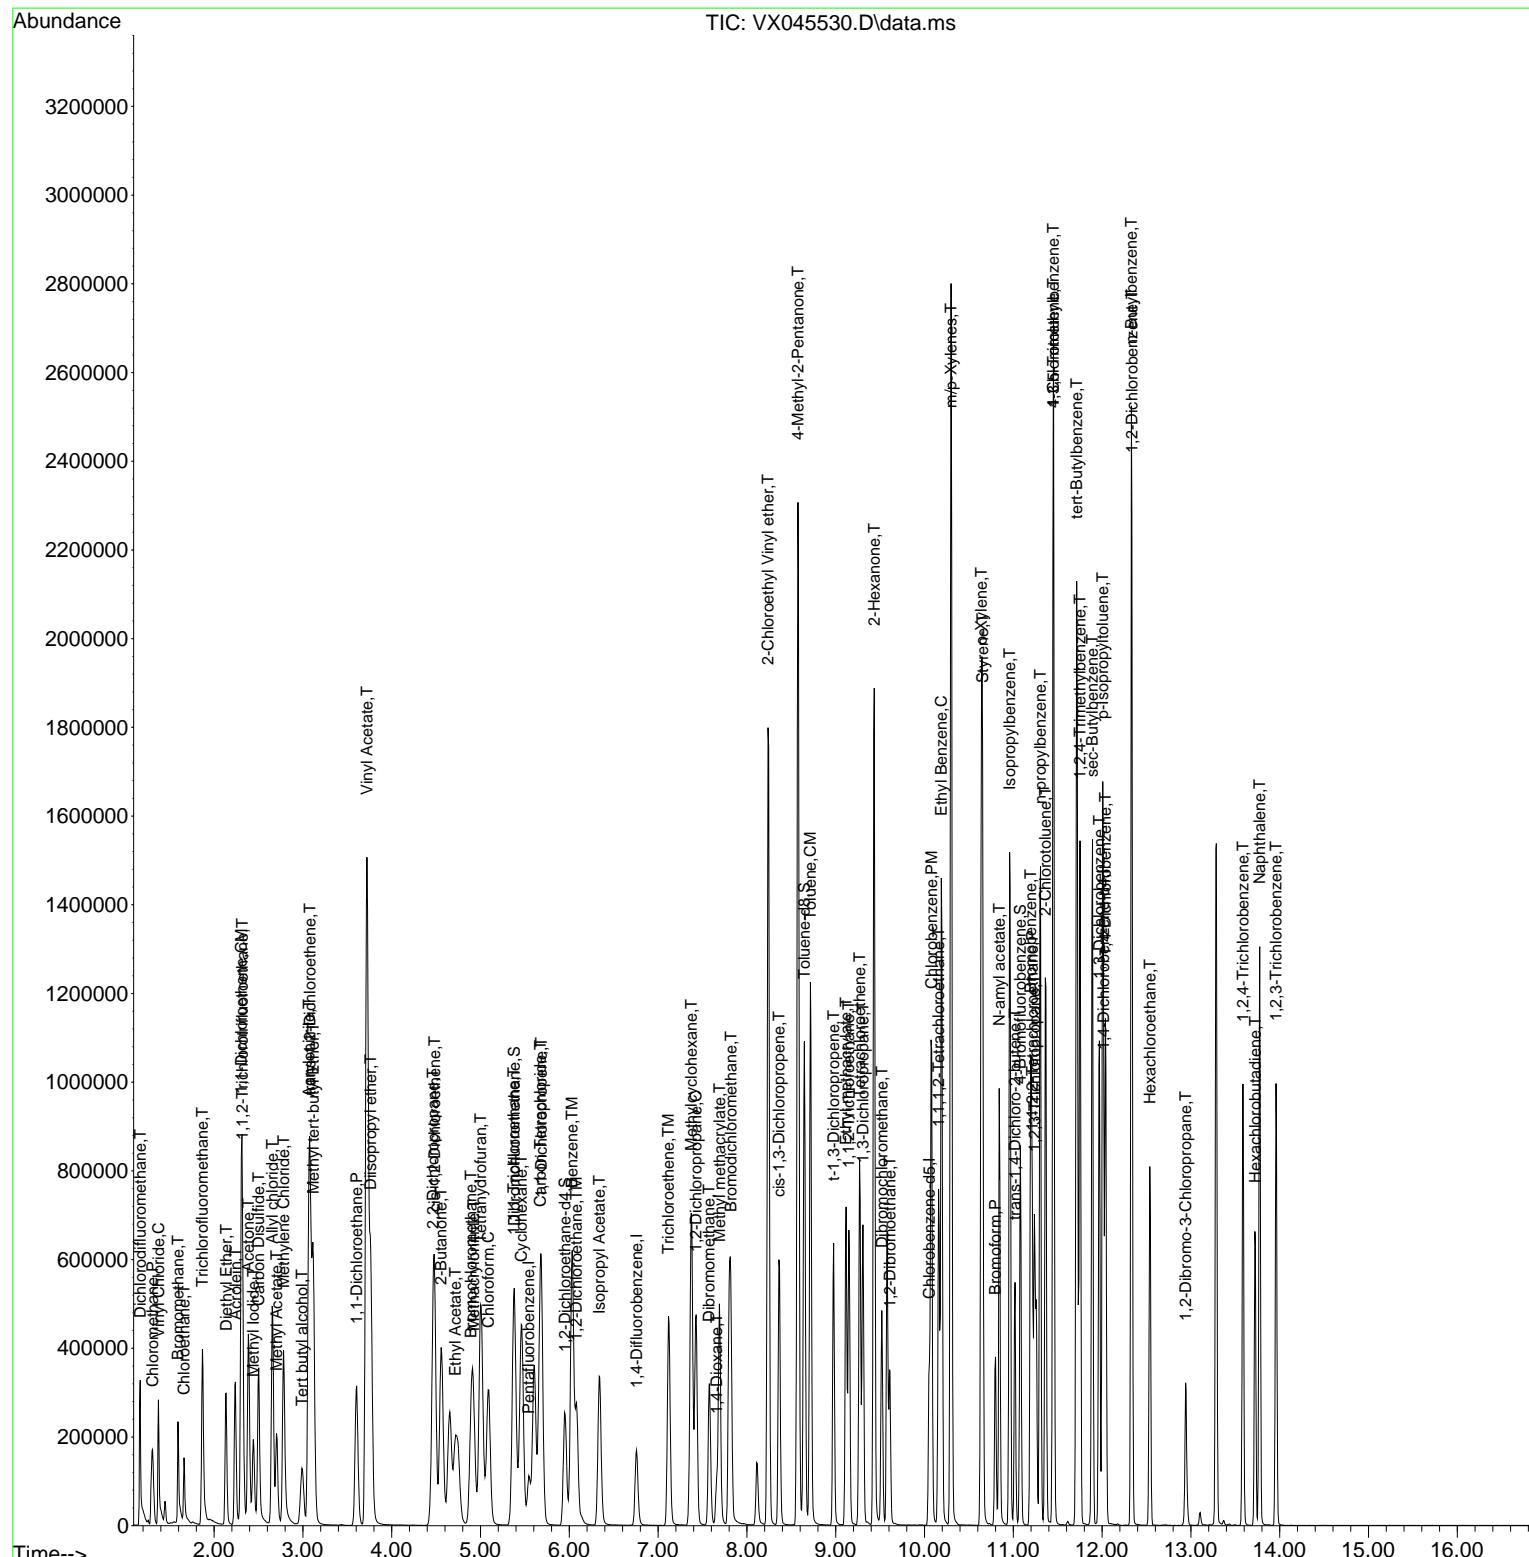

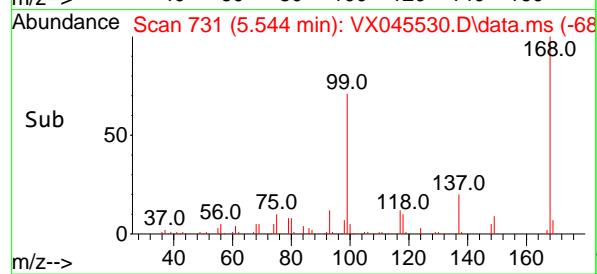

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.544 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

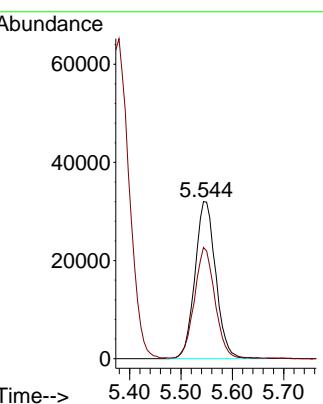

#2

Dichlorodifluoromethane

Concen: 164.460 ug/l



RT: 1.167 min Scan# 13




Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt	Ion:	Resp:	
Ion	Ratio	Lower	Upper
85	100		
87	32.0	16.1	48.2

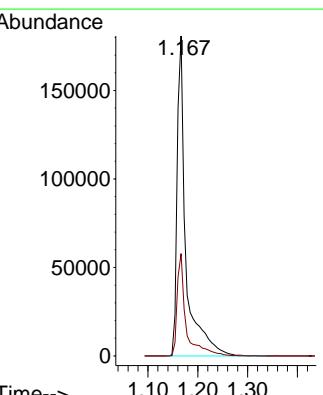



#3

Chloromethane

Concen: 143.373 ug/l

RT: 1.307 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

1 Manual Integrations  
2 APPROVED



3 Reviewed By :Amit Patel 04/02/2025




4 Supervised By :Mahesh Dadoda 04/02/2025

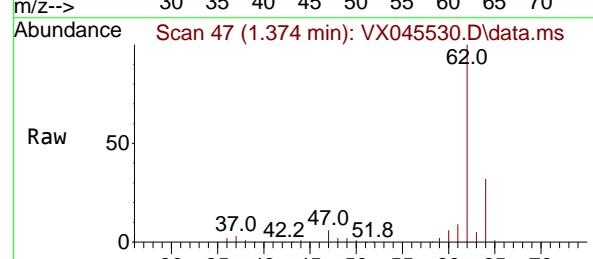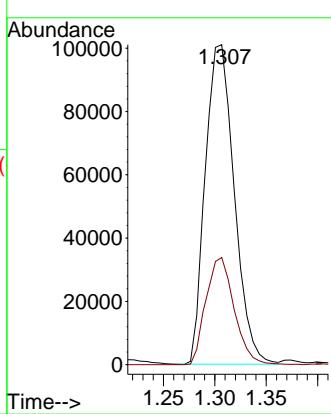

#4  
Vinyl Chloride  
Concen: 155.697 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Tgt Ion: 62 Resp: 197096  
Ion Ratio Lower Upper  
62 100  
64 32.1 25.5 38.3

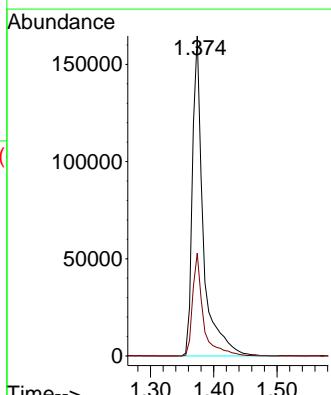

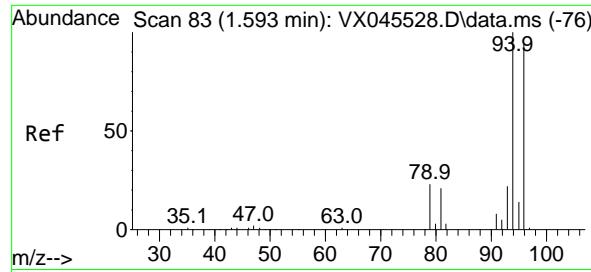

#5

Bromomethane

Concen: 146.986 ug/l

RT: 1.593 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#6

Chloroethane

Concen: 128.421 ug/l


RT: 1.660 min Scan# 94


Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt Ion: 64 Resp: 86251  
 Ion Ratio Lower Upper  
 64 100  
 66 31.4 26.3 39.5

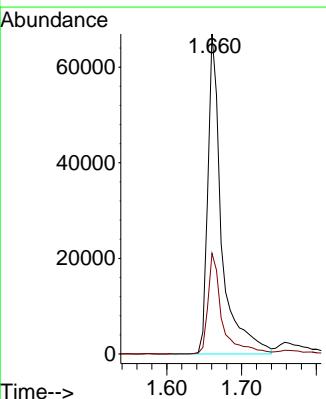


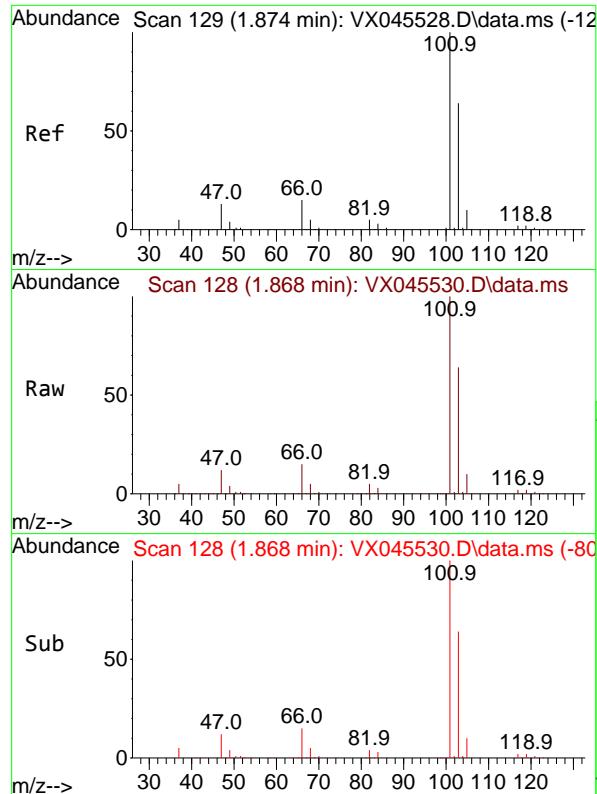


#7  
Trichlorofluoromethane  
Concen: 141.495 ug/l  
RT: 1.868 min Scan# 1  
Delta R.T. -0.006 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

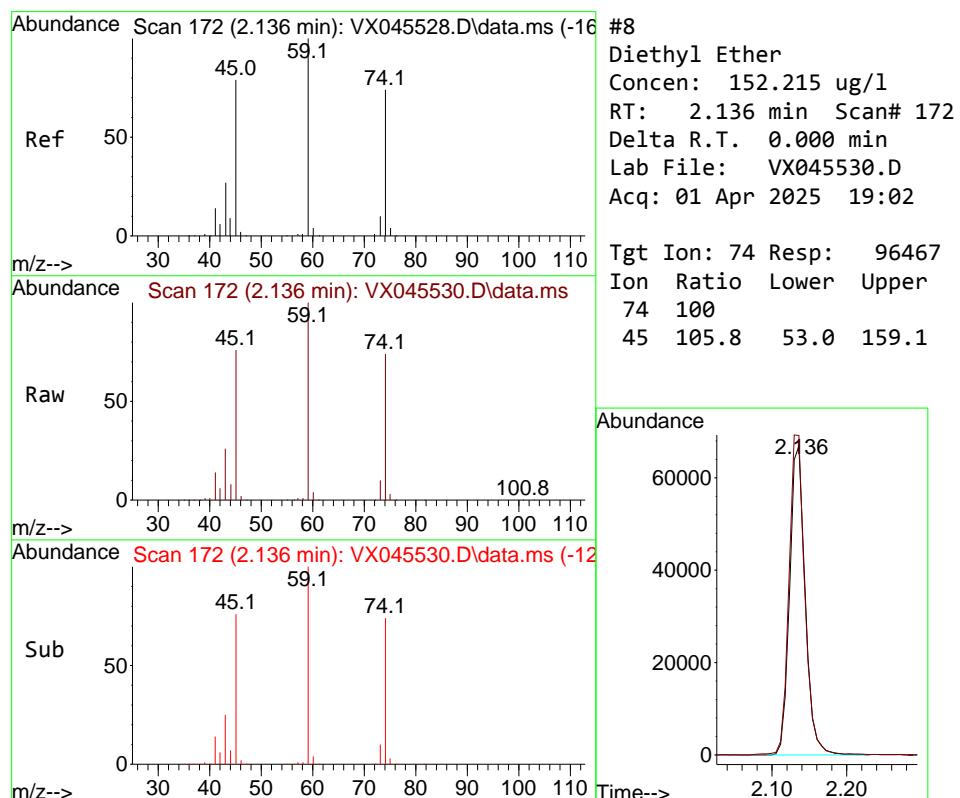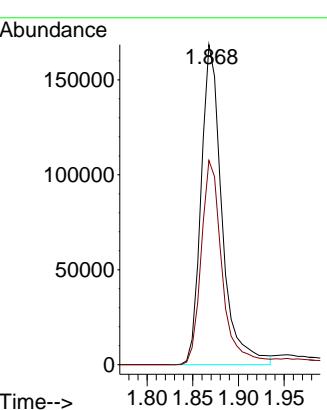

#8  
Diethyl Ether  
Concen: 152.215 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Tgt Ion: 74 Resp: 96467  
Ion Ratio Lower Upper  
74 100  
45 105.8 53.0 159.1




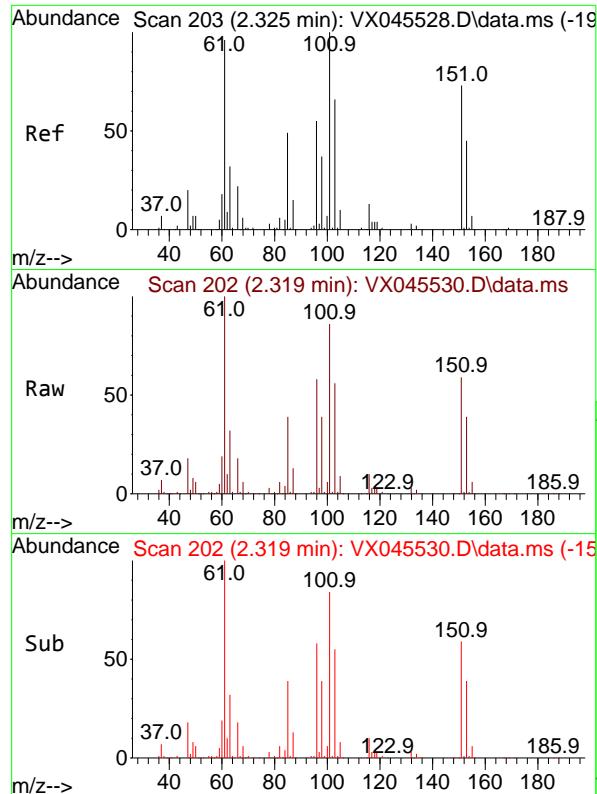


#9  
 1,1,2-Trichlorotrifluoroethane  
 Concen: 154.698 ug/l  
 RT: 2.319 min Scan# 2  
 Delta R.T. -0.006 min  
 Lab File: VX045530.D  
 Acq: 01 Apr 2025 19:02

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

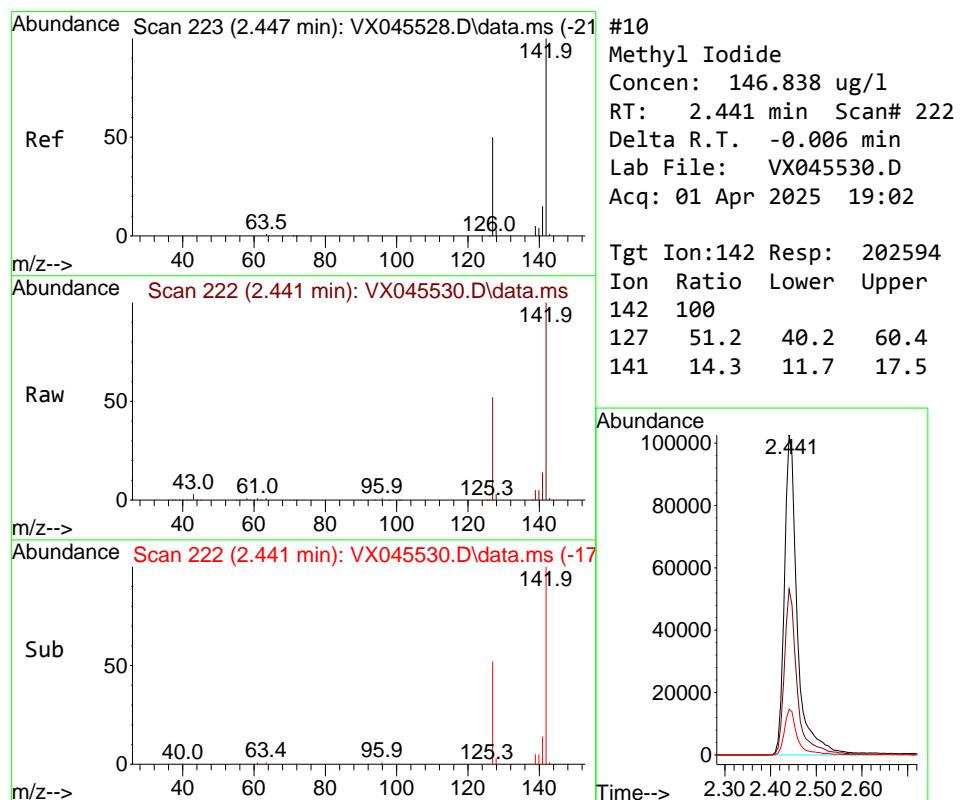

#10  
 Methyl Iodide  
 Concen: 146.838 ug/l  
 RT: 2.441 min Scan# 222  
 Delta R.T. -0.006 min  
 Lab File: VX045530.D  
 Acq: 01 Apr 2025 19:02

Tgt Ion:142 Resp: 202594  
 Ion Ratio Lower Upper  
 142 100  
 127 51.2 40.2 60.4  
 141 14.3 11.7 17.5

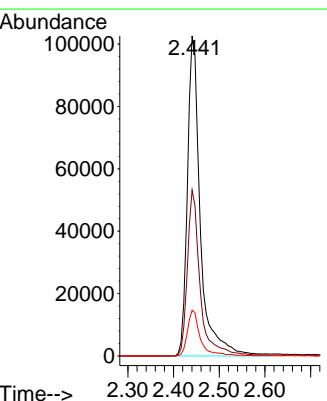

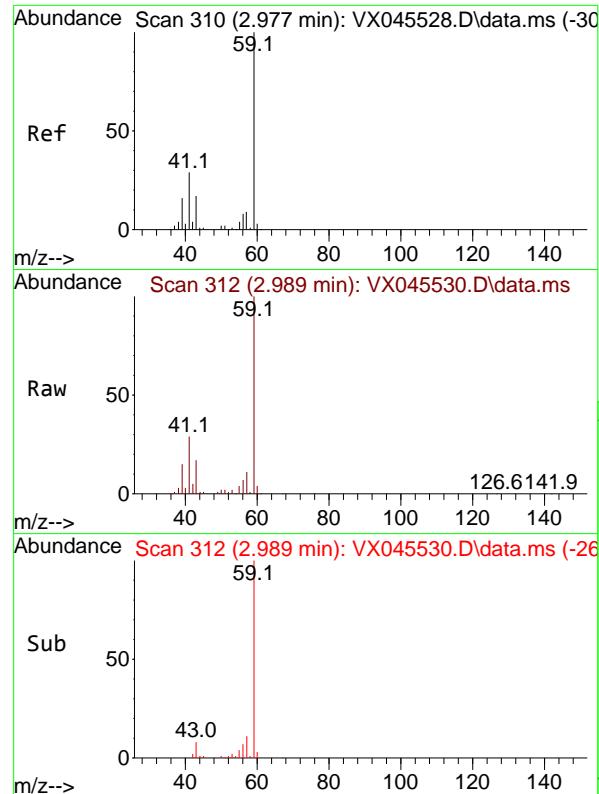

#11

Tert butyl alcohol

Concen: 758.202 ug/l

RT: 2.989 min Scan# 3

Delta R.T. 0.012 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

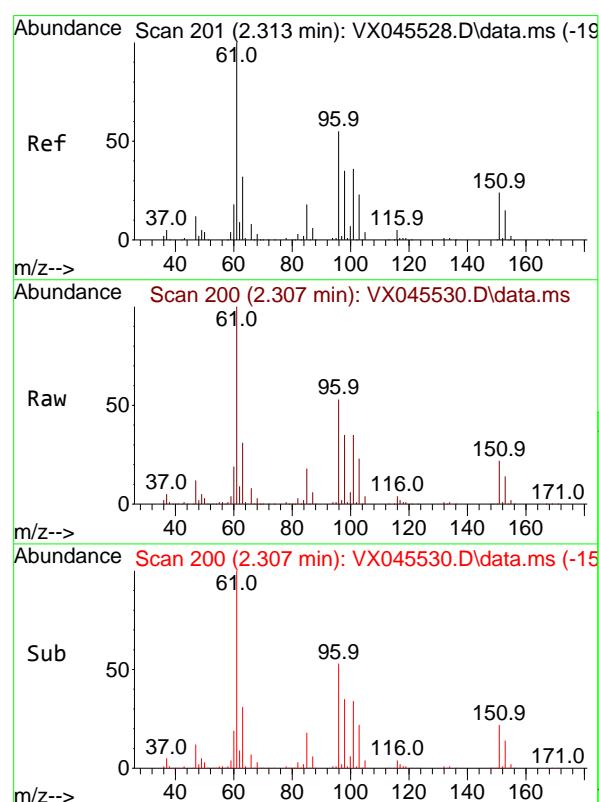

#12

1,1-Dichloroethene

Concen: 153.921 ug/l

RT: 2.307 min Scan# 200

Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 96 Resp: 166365


Ion Ratio Lower Upper

96 100

61 187.0 145.7 218.5

98 65.0 51.6 77.4

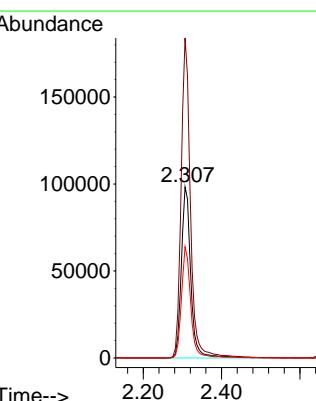



#13

Acrolein

Concen: 764.070 ug/l

RT: 2.239 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

Abundance Scan 189 (2.239 min): VX045530.D\data.ms

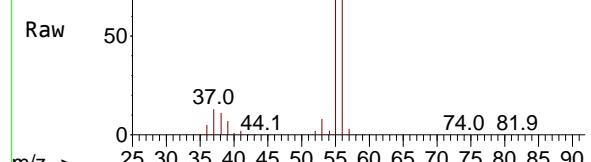

Abundance Scan 189 (2.239 min): VX045530.D\data.ms (-14)

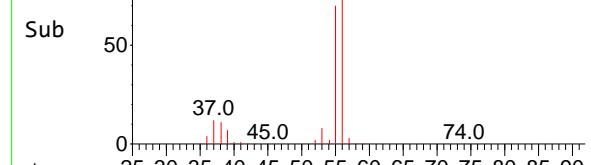

Tgt Ion: 56 Resp: 23281

Ion Ratio Lower Upper

56 100


55 70.2 56.2 84.2

Manual Integrations


APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

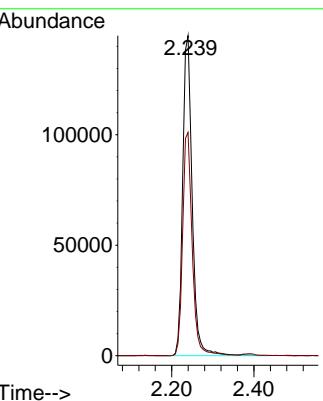

Abundance Scan 258 (2.660 min): VX045528.D\data.ms (-24)

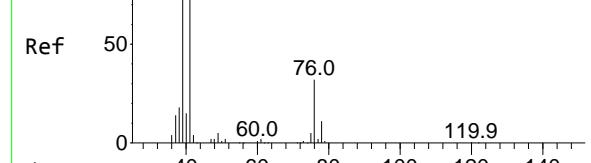

#14

Allyl chloride

Concen: 152.755 ug/l


RT: 2.654 min Scan# 257

Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Abundance Scan 257 (2.654 min): VX045530.D\data.ms

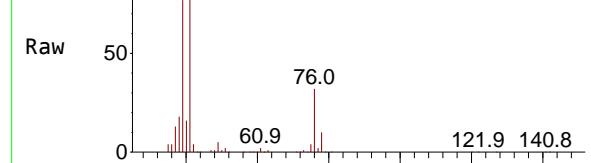


Tgt Ion: 41 Resp: 313268

Ion Ratio Lower Upper


41 100

39 75.0 60.2 90.2

76 32.2 24.6 36.8

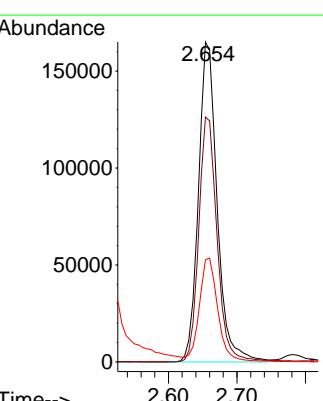

Abundance Scan 257 (2.654 min): VX045530.D\data.ms (-20)






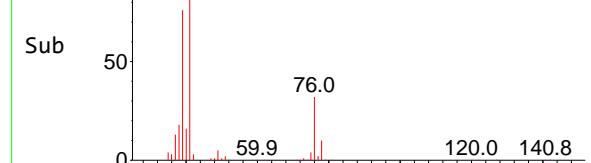


Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150



#15

Acrylonitrile

Concen: 727.247 ug/l

RT: 3.069 min Scan# 3

Delta R.T. 0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

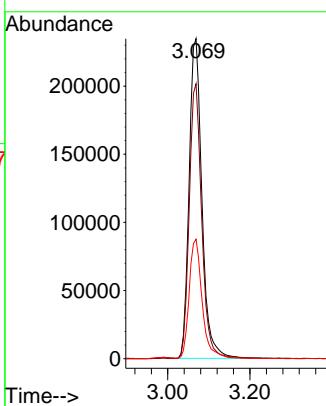

#16

Acetone

Concen: 709.323 ug/l


RT: 2.386 min Scan# 213


Delta R.T. 0.000 min

Lab File: VX045530.D



Acq: 01 Apr 2025 19:02

Tgt Ion: 43 Resp: 479564  
 Ion Ratio Lower Upper  
 43 100  
 58 27.2 22.3 33.5

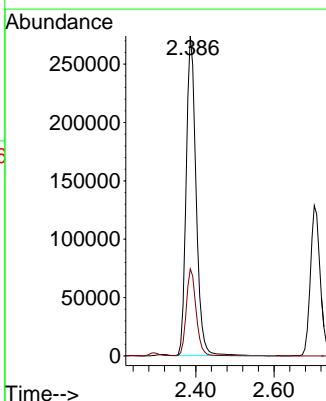




Abundance Scan 232 (2.502 min): VX045530.D\data.ms

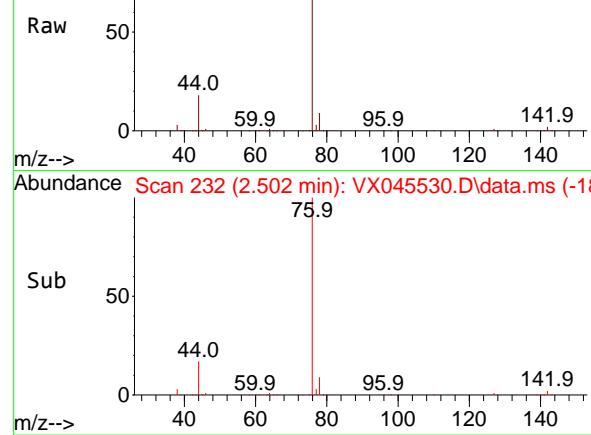

Abundance Scan 265 (2.703 min): VX045530.D\data.ms

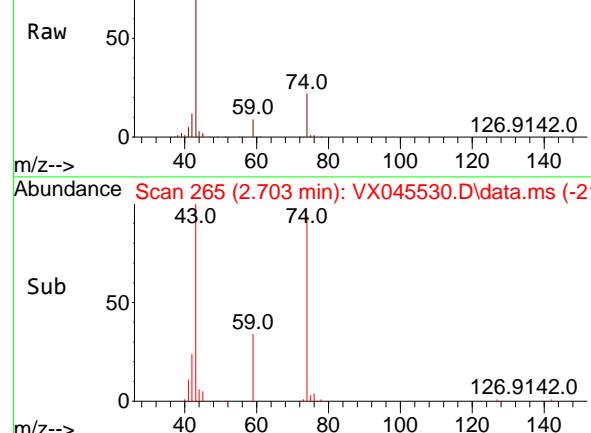

#17

Carbon Disulfide

Concen: 166.133 ug/l

RT: 2.502 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

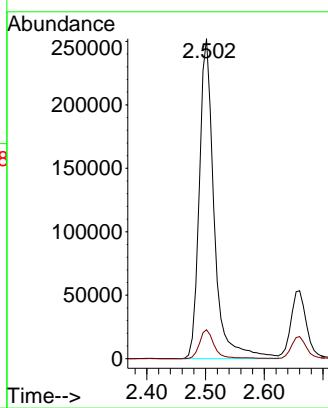

#18

Methyl Acetate

Concen: 146.832 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02







Tgt Ion: 43 Resp: 228558

Ion Ratio Lower Upper

43 100

74 22.4 17.5 26.3

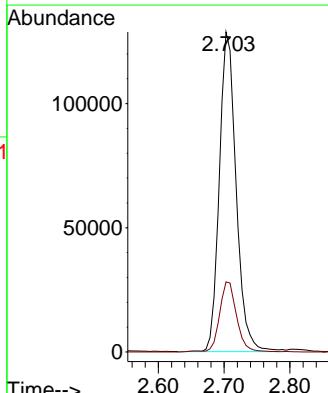

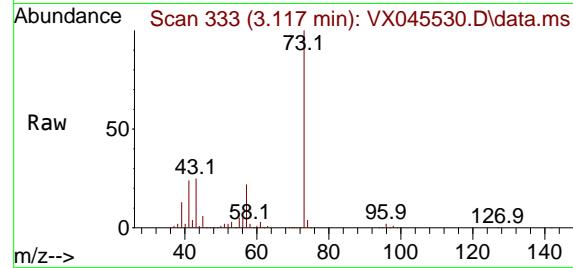

#19

Methyl tert-butyl Ether

Concen: 158.301 ug/l

RT: 3.117 min Scan# 3

Instrument: MSVOA\_X

Delta R.T. 0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

ClientSampleId : VSTDICC150

Tgt Ion: 73 Resp: 59853

Ion Ratio Lower Upper


73 100

57 21.7 17.6 26.4

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#20

Methylene Chloride

Concen: 147.254 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt Ion: 84 Resp: 186382


Ion Ratio Lower Upper







84 100

49 135.1 107.5 161.3

51 40.8 33.0 49.6

86 63.4 50.1 75.1



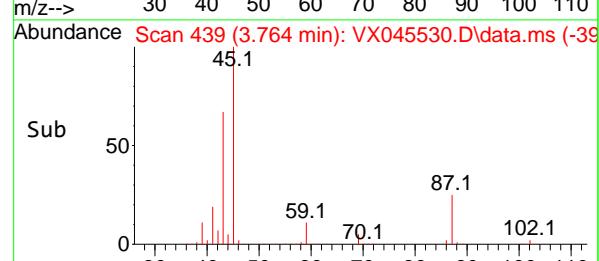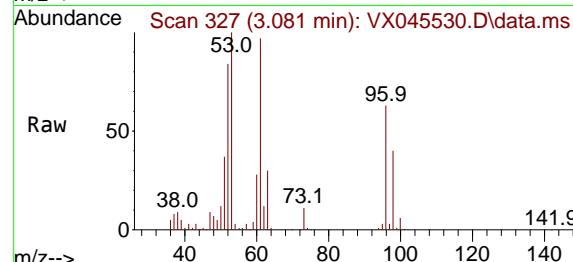

#21

trans-1,2-Dichloroethene

Concen: 154.210 ug/l

RT: 3.081 min Scan# 327

Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

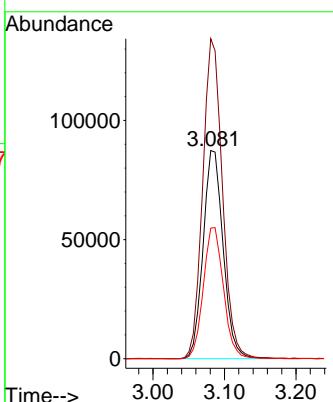

#22

Diisopropyl ether

Concen: 157.617 ug/l

RT: 3.764 min Scan# 439

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt Ion: 45 Resp: 636728


Ion Ratio Lower Upper


45 100

43 67.0 59.3 88.9



87 25.5 20.4 30.6

59 10.6 9.0 13.6






Abundance Scan 432 (3.721 min): VX045530.D\data.ms

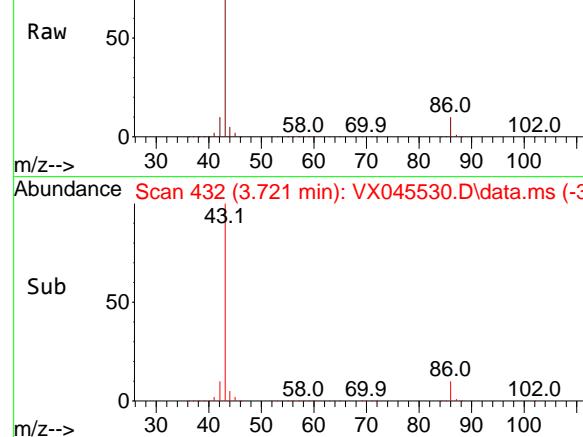

Abundance Scan 413 (3.605 min): VX045530.D\data.ms

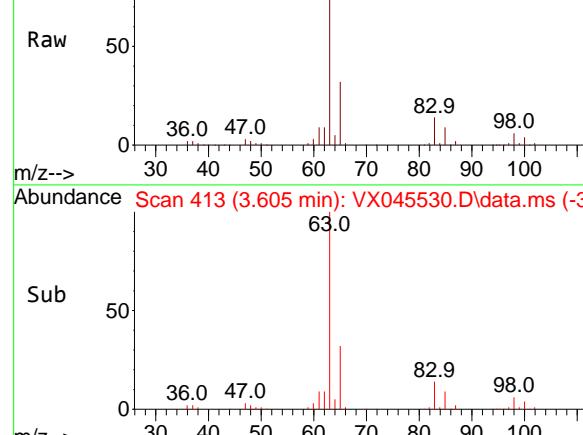

#23

**Vinyl Acetate**

Concen: 834.120 ug/l

RT: 3.721 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

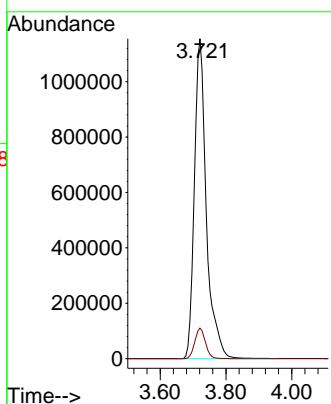

#24

**1,1-Dichloroethane**

Concen: 152.778 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 63 Resp: 349040


Ion Ratio Lower Upper

63 100

98 6.4 3.4 10.1


100 3.9 2.2 6.6

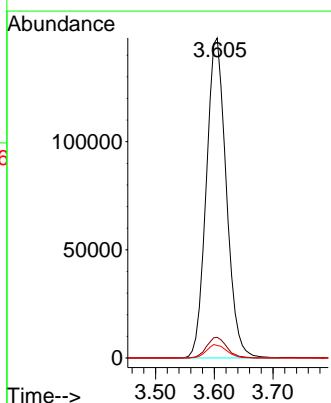



#25  
2-Butanone  
Concen: 747.834 ug/l  
RT: 4.556 min Scan# 569  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150

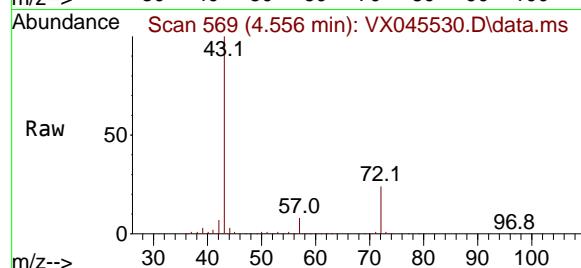


Tgt Ion: 43 Resp: 740090  
Ion Ratio Lower Upper  
43 100  
72 23.6 18.6 28.0

Manual Integrations  
**APPROVED**



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025



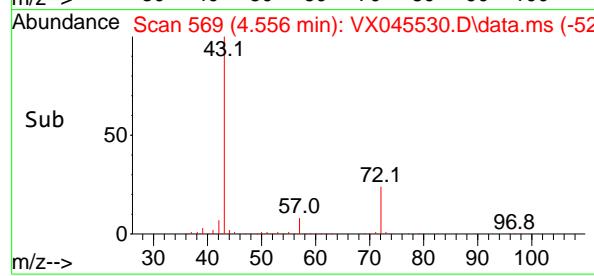


#26  
2,2-Dichloropropane  
Concen: 170.765 ug/l  
RT: 4.465 min Scan# 554  
Delta R.T. -0.006 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02



Tgt Ion: 77 Resp: 252063  
Ion Ratio Lower Upper  
77 100  
97 21.2 10.6 31.8

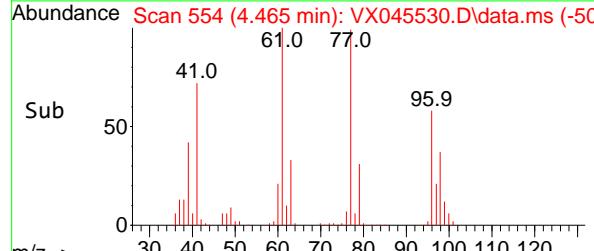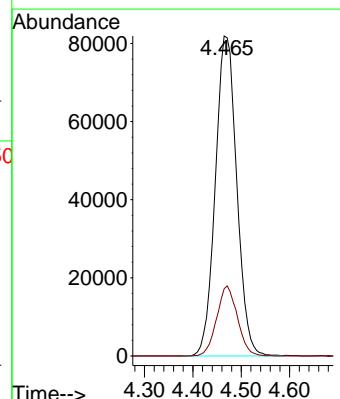

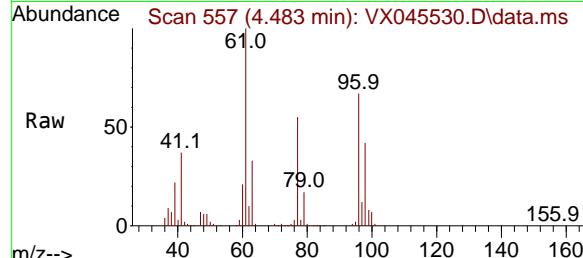





#27

cis-1,2-Dichloroethene  
Concen: 152.571 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

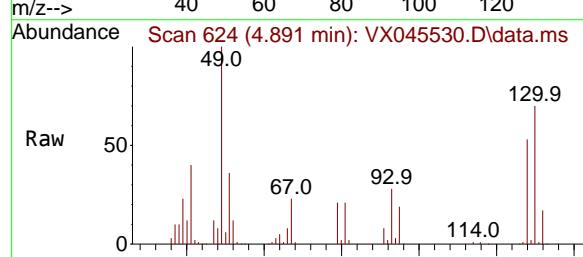




#28

Bromochloromethane  
Concen: 140.938 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Tgt Ion: 49 Resp: 155600  
Ion Ratio Lower Upper  
49 100  
129 1.8 0.0 3.8  
130 70.7 54.6 81.8



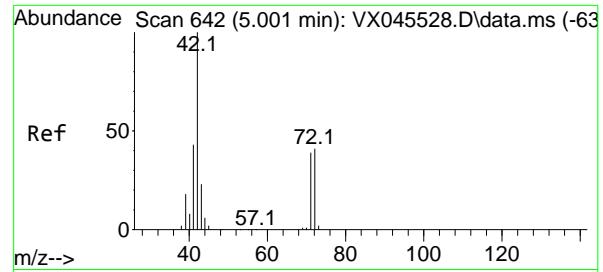

#29

Tetrahydrofuran

Concen: 741.226 ug/l

RT: 5.001 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150

Tgt Ion: 42 Resp: 475589

Ion Ratio Lower Upper

42 100

72 42.3 33.4 50.0




71 39.2 31.4 47.0

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#30

Chloroform

Concen: 150.451 ug/l

RT: 5.087 min Scan# 656

Delta R.T. 0.000 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02


Tgt Ion: 83 Resp: 353681

Ion Ratio Lower Upper


83 100

85 64.2 52.8 79.2


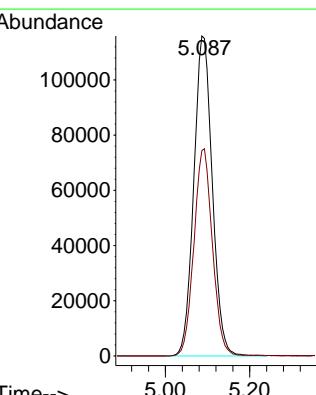





Abundance Scan 717 (5.458 min): VX045530.D\data.ms

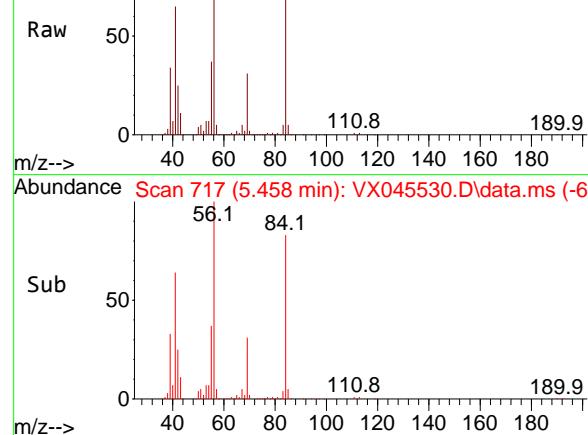


Abundance Scan 717 (5.458 min): VX045530.D\data.ms (-66)

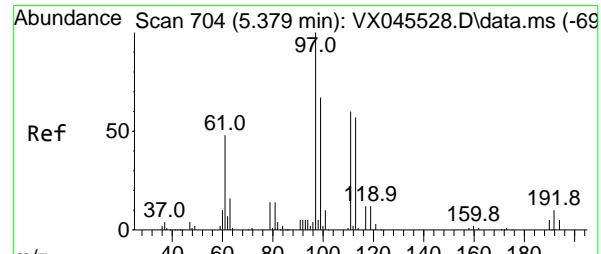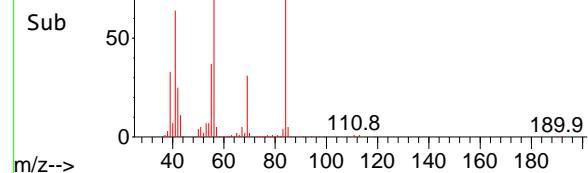

Abundance Scan 703 (5.373 min): VX045530.D\data.ms

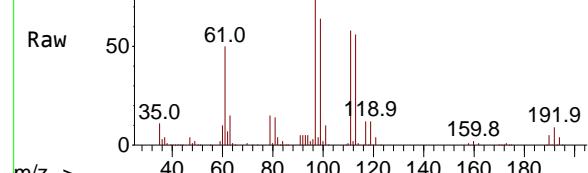

Abundance Scan 703 (5.373 min): VX045530.D\data.ms (-65)

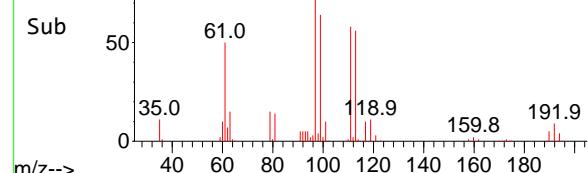

#31

Cyclohexane

Concen: 153.595 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#32

1,1,1-Trichloroethane

Concen: 158.426 ug/l

RT: 5.373 min Scan# 703

Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 97 Resp: 315136


Ion Ratio Lower Upper

97 100

99 63.7 51.7 77.5

61 49.1 41.0 61.4

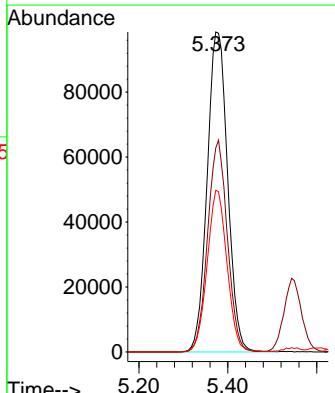



#33

1,2-Dichloroethane-d4




Concen: 153.661 ug/l

RT: 5.952 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

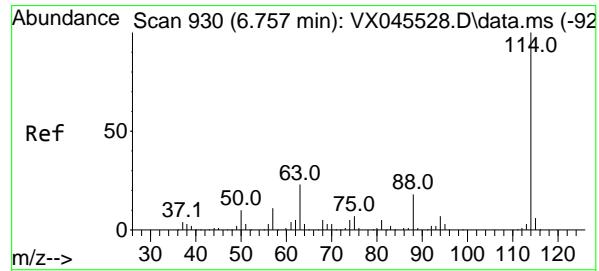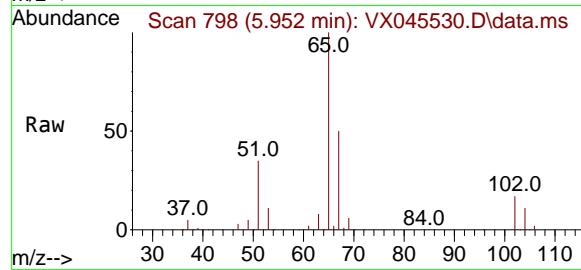

#34

1,4-Difluorobenzene



Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02

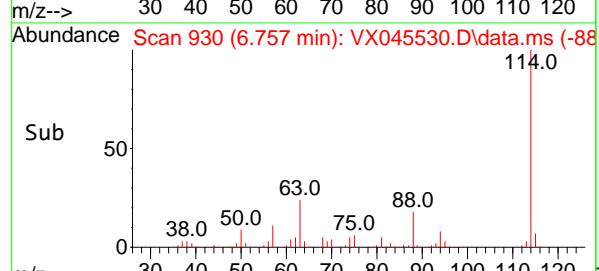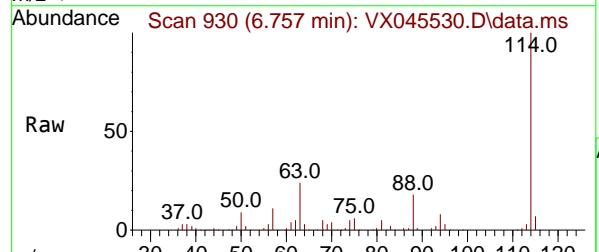


Instrument :  
MSVOA\_X  
ClientSampleId :  
VSTDICC150




Manual Integrations  
APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

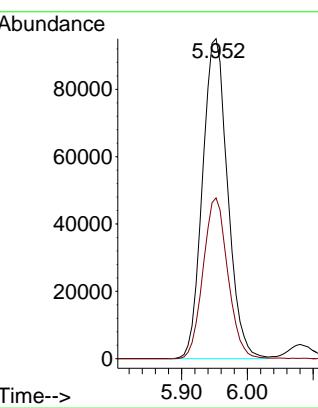

Tgt Ion:114 Resp: 160037  
Ion Ratio Lower Upper  
114 100  
63 24.3 0.0 46.8  
88 17.6 0.0 35.4

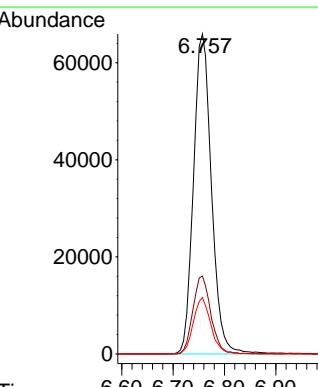

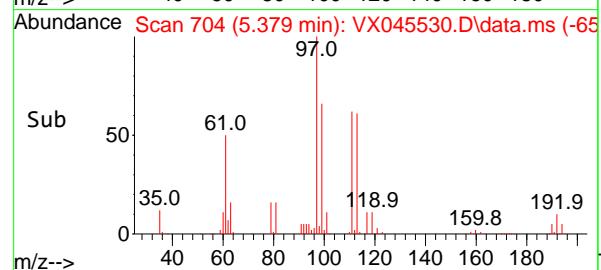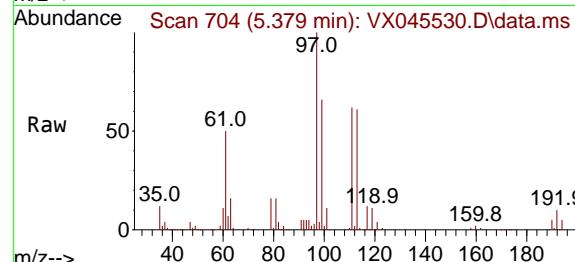

#35

Dibromofluoromethane

Concen: 152.887 ug/l

RT: 5.379 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#36

1,1-Dichloropropene

Concen: 156.399 ug/l

RT: 5.684 min Scan# 754

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 75 Resp: 239776




Ion Ratio Lower Upper

75 100

110 32.4 16.9 50.6

77 30.6 25.0 37.4

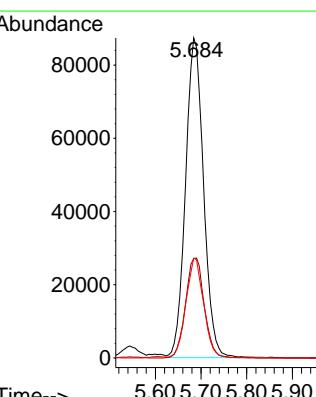

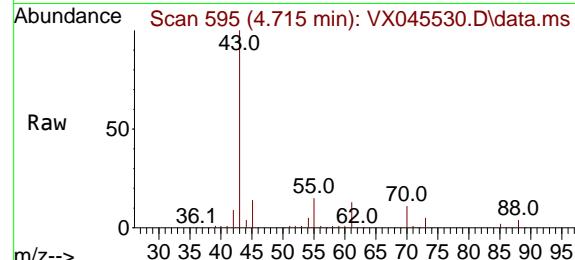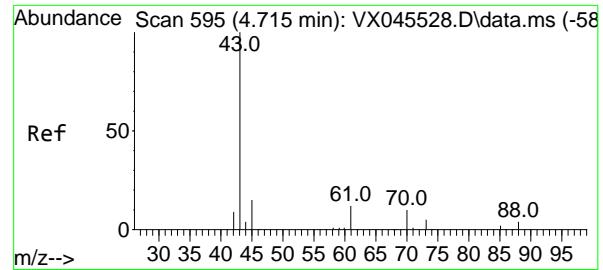

#37

Ethyl Acetate

Concen: 152.461 ug/l

RT: 4.715 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

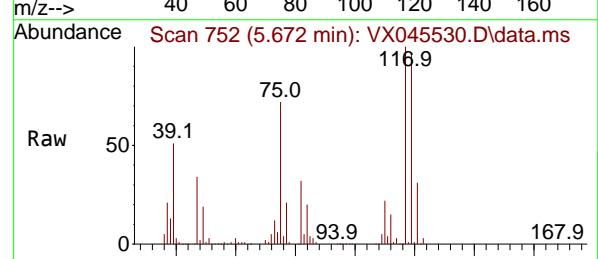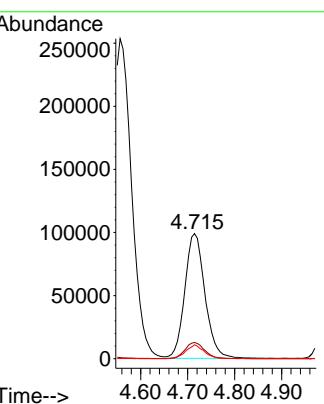

#38

Carbon Tetrachloride


Concen: 161.005 ug/l




RT: 5.672 min Scan# 752

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

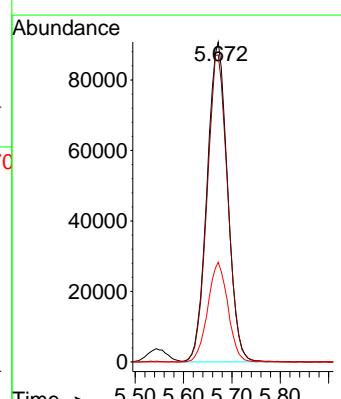 Tgt Ion:117 Resp: 266770  
 Ion Ratio Lower Upper  
 117 100  
 119 95.9 76.9 115.3  
 121 31.2 24.2 36.2
 

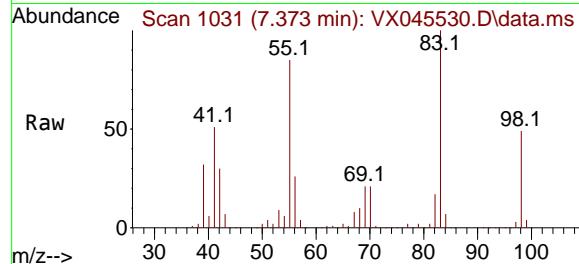

#39

Methylcyclohexane

Concen: 161.366 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02





Instrument : MSVOA\_X

ClientSampleId : VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

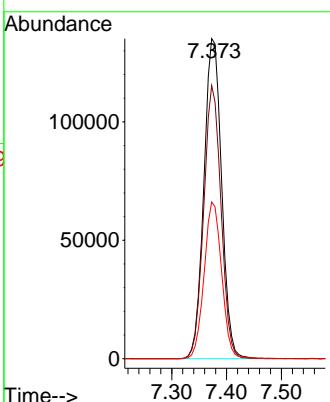

#40

Benzene

Concen: 150.208 ug/l


RT: 6.031 min Scan# 811







Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt	Ion	Resp:	703311
Ion	Ratio	Lower	Upper
78	100		
77	24.0	19.0	28.6

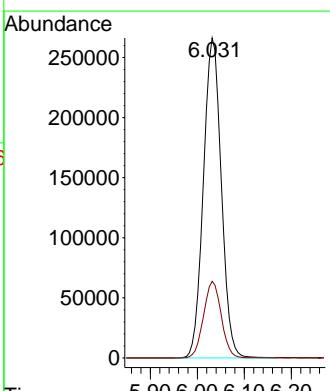



#41

Methacrylonitrile

Concen: 160.155 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument :

MSVOA\_X

ClientSampleId :


VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

Abundance

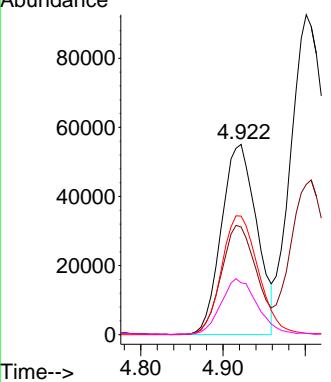

#42

1,2-Dichloroethane

Concen: 153.146 ug/l

RT: 6.080 min Scan# 819

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 62 Resp: 296168


Ion Ratio Lower Upper

62 100

98 7.6 0.0 15.2

Abundance

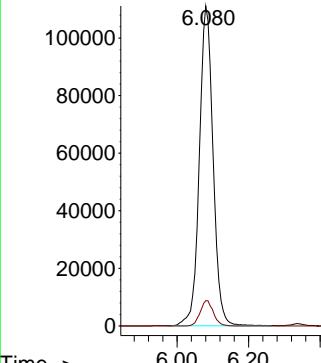

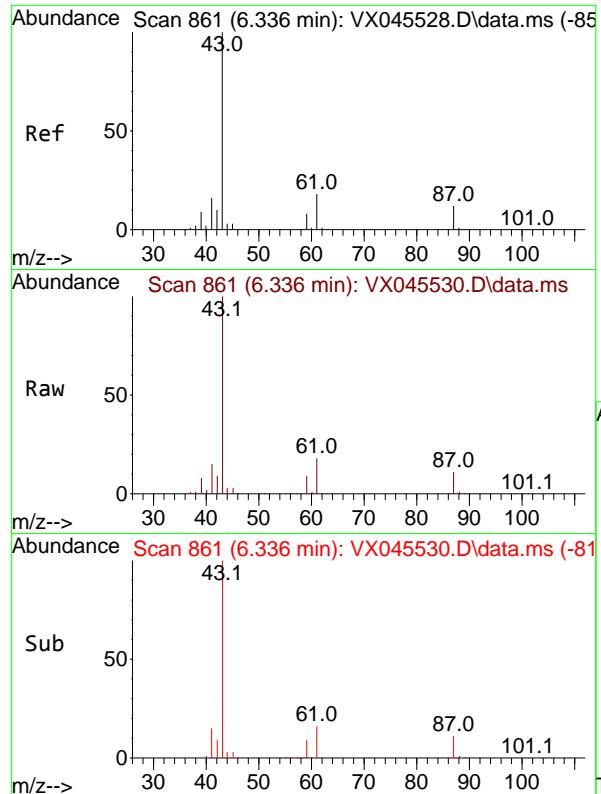

#43

Isopropyl Acetate

Concen: 162.494 ug/l

RT: 6.336 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC150

Tgt Ion: 43 Resp: 47582

Ion Ratio Lower Upper

43 100

61 18.1 14.1 21.1



87 11.8 9.2 13.8

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

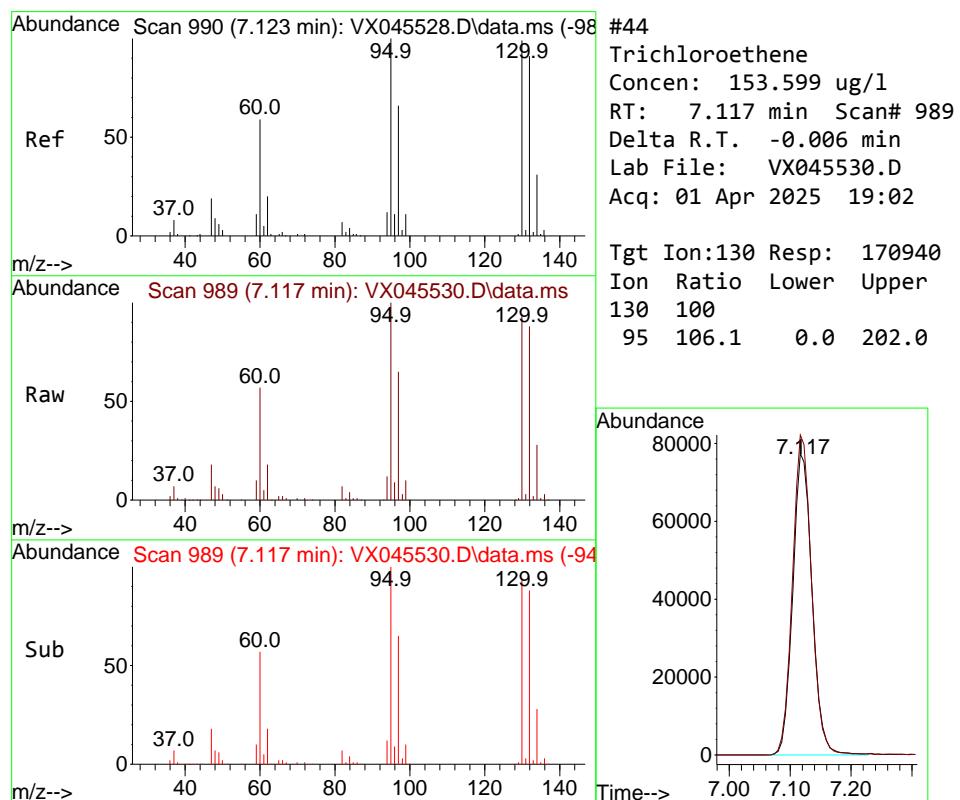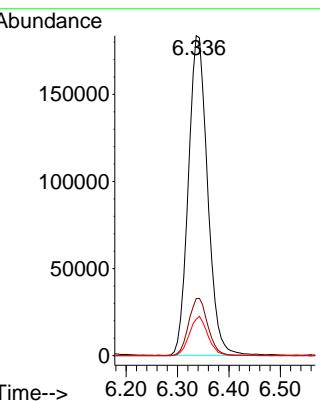

#44

Trichloroethene

Concen: 153.599 ug/l

RT: 7.117 min Scan# 989

Delta R.T. -0.006 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02




Tgt Ion:130 Resp: 170940

Ion Ratio Lower Upper

130 100

95 106.1 0.0 202.0

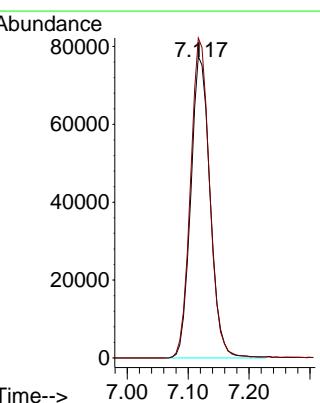

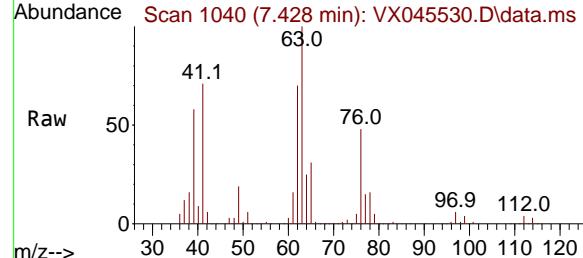

#45

1,2-Dichloropropane

Concen: 153.610 ug/l

RT: 7.428 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

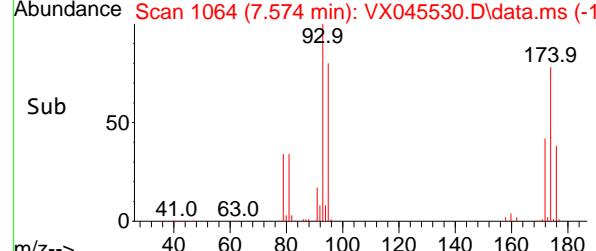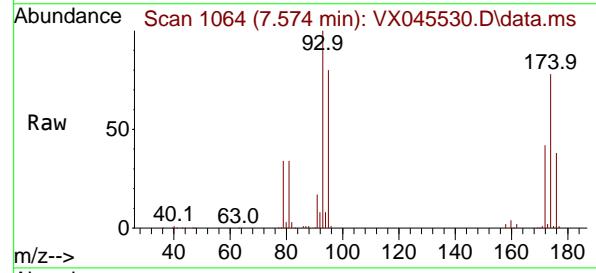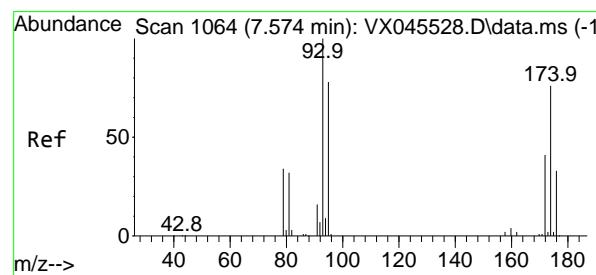

#46

Dibromomethane

Concen: 150.996 ug/l

RT: 7.574 min Scan# 1064

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 93 Resp: 135415




Ion Ratio Lower Upper

93 100

95 82.4 64.8 97.2

174 84.1 65.4 98.0

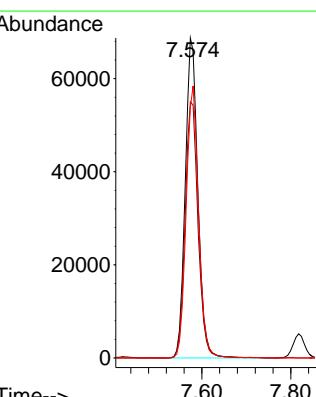



#47

Bromodichloromethane

Concen: 156.272 ug/l

RT: 7.818 min Scan# 1104

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

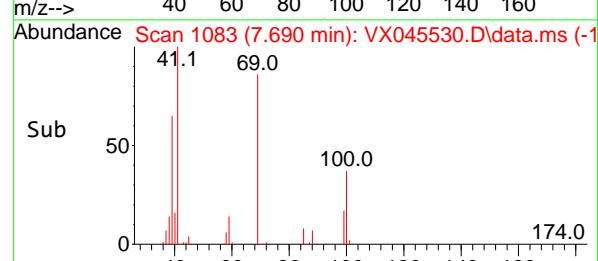

#48

Methyl methacrylate

Concen: 159.281 ug/l

RT: 7.690 min Scan# 1083


Delta R.T. 0.000 min


Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 41 Resp: 240818

Ion	Ratio	Lower	Upper
41	100		
69	73.0	58.2	87.2
39	64.9	53.6	80.4

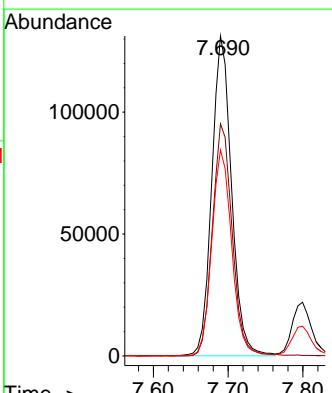





Abundance Scan 1078 (7.659 min): VX045530.D\data.ms

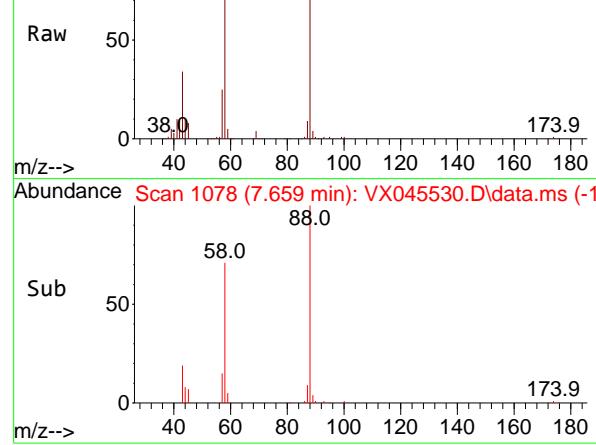


Abundance Scan 1078 (7.659 min): VX045530.D\data.ms (-1)

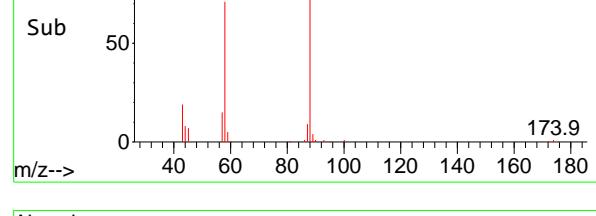

Abundance Scan 1078 (7.659 min): VX045530.D\data.ms (-1)

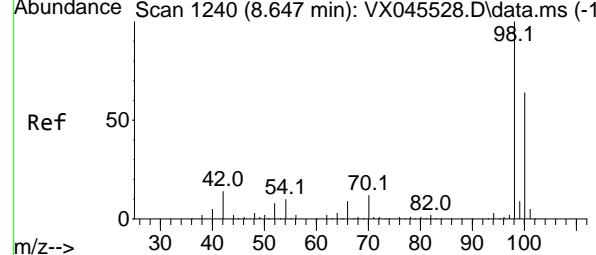

Abundance Scan 1240 (8.647 min): VX045530.D\data.ms

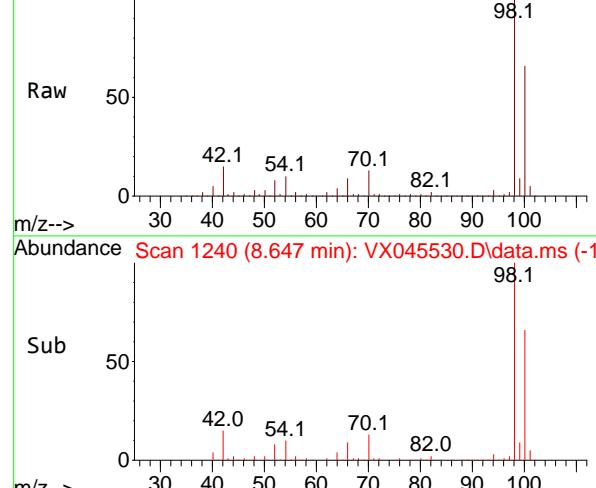

Abundance Scan 1240 (8.647 min): VX045530.D\data.ms (-1)



Abundance Scan 1240 (8.647 min): VX045530.D\data.ms (-1)

#49

1,4-Dioxane

Concen: 2739.196 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC150


**Manual Integrations****APPROVED**

Reviewed By :Amit Patel 04/02/2025


Supervised By :Mahesh Dadoda 04/02/2025

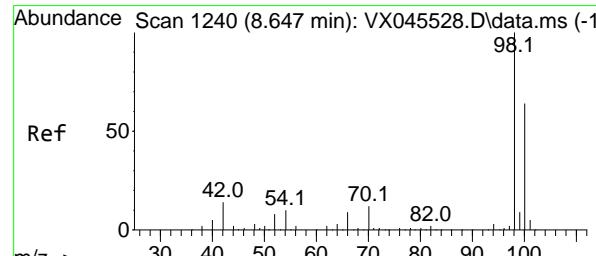

Abundance Scan 1240 (8.647 min): VX045530.D\data.ms

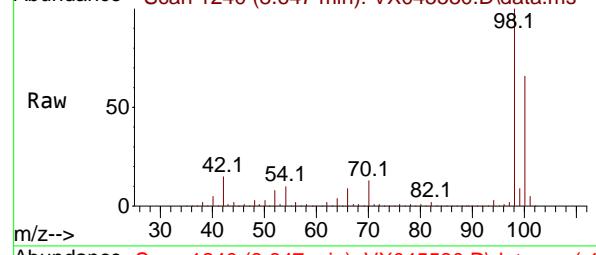


Abundance Scan 1240 (8.647 min): VX045530.D\data.ms (-1)


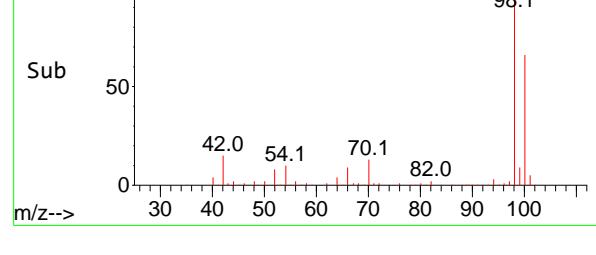


Abundance Scan 1240 (8.647 min): VX045530.D\data.ms (-1)

#50  
Toluene-d8  
Concen: 152.216 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Tgt Ion: 98 Resp: 603264  
Ion Ratio Lower Upper  
98 100  
100 65.5 52.2 78.4

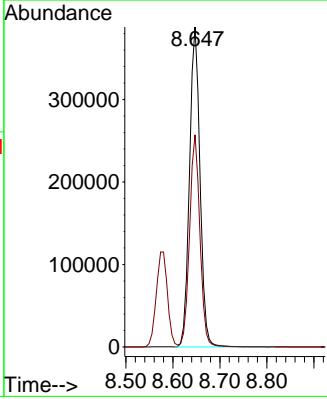

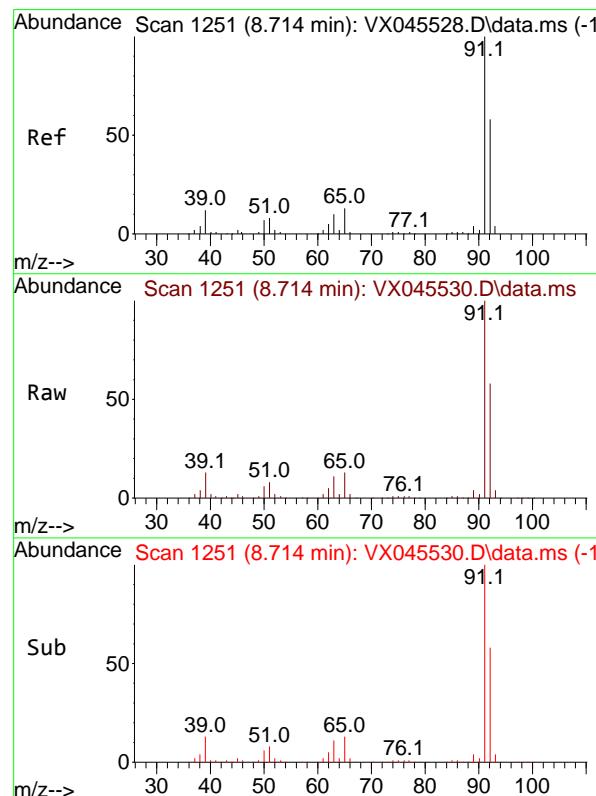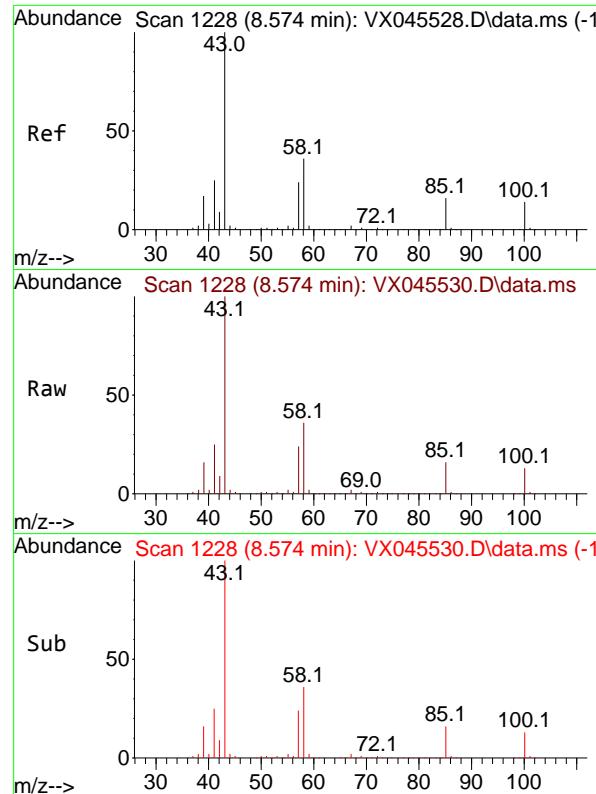

#51

4-Methyl-2-Pentanone

Concen: 728.817 ug/l

RT: 8.574 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#52

Toluene

Concen: 148.245 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02




Tgt Ion: 92 Resp: 420015

Ion Ratio Lower Upper

92 100

91 173.3 138.7 208.1



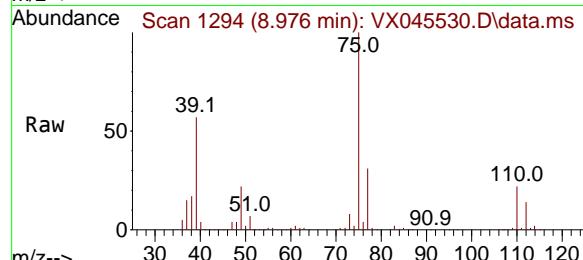

#53

t-1,3-Dichloropropene

Concen: 150.589 ug/l

RT: 8.976 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150




**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

Abundance

8.976

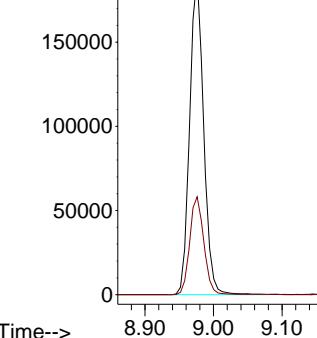

#54

cis-1,3-Dichloropropene

Concen: 171.104 ug/l

RT: 8.360 min Scan# 1193

Delta R.T. -0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt Ion: 75 Resp: 287973



Ion Ratio Lower Upper




75 100

77 30.6 24.6 36.8

39 62.9 48.4 72.6

Abundance

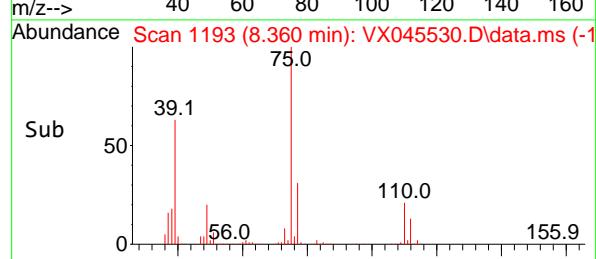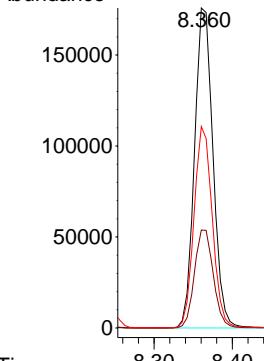



#55

1,1,2-Trichloroethane

Concen: 144.752 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#56

Ethyl methacrylate

Concen: 163.624 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 69 Resp: 285895


Ion Ratio Lower Upper

69 100

41 76.2 61.3 91.9

39 48.0 40.2 60.2

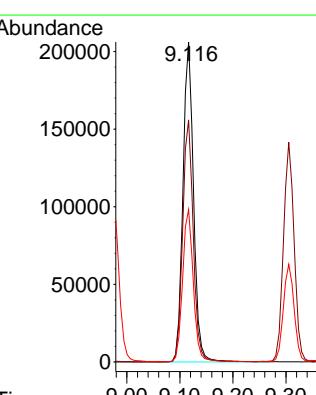

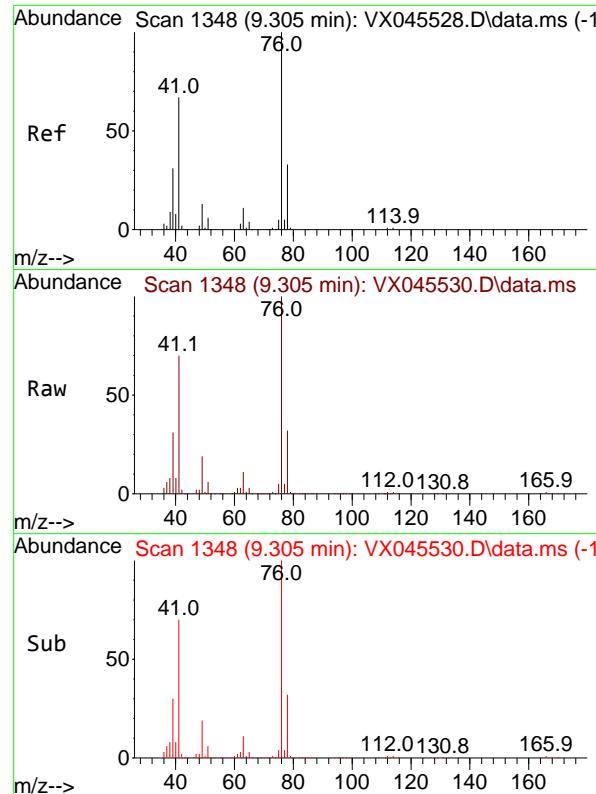

#57

1,3-Dichloropropane

Concen: 146.708 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150

Tgt Ion: 76 Resp: 288430

Ion Ratio Lower Upper

76 100


78 32.2 26.0 39.0

Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

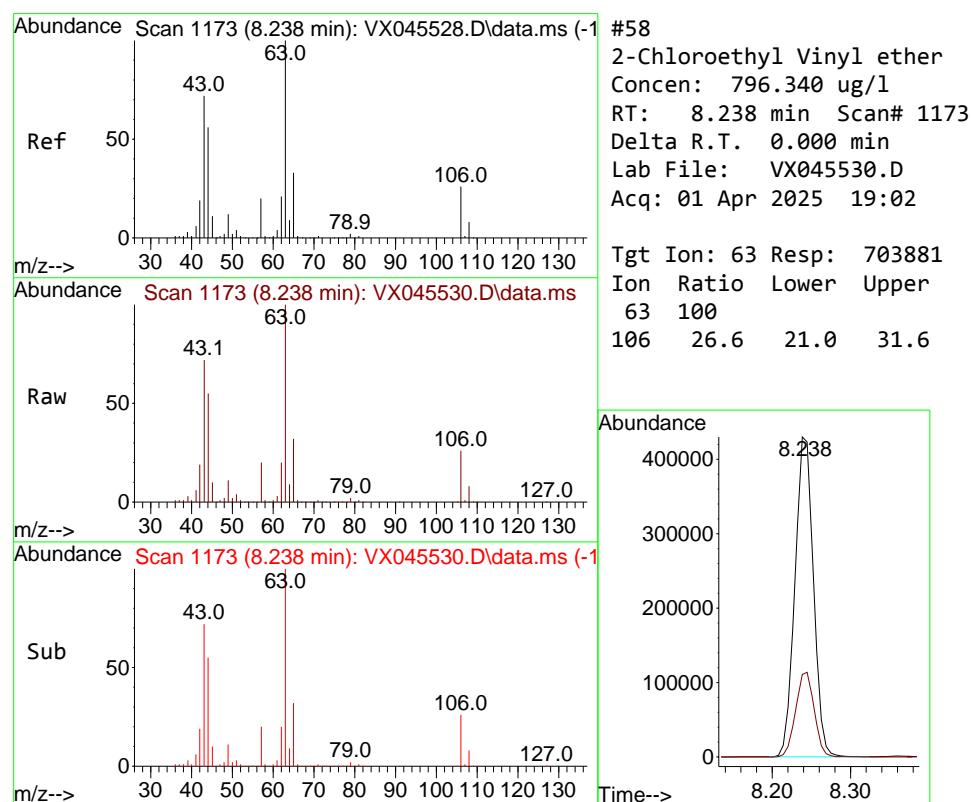

#58

2-Chloroethyl Vinyl ether

Concen: 796.340 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. 0.000 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02


Tgt Ion: 63 Resp: 703881

Ion Ratio Lower Upper


63 100

106 26.6 21.0 31.6

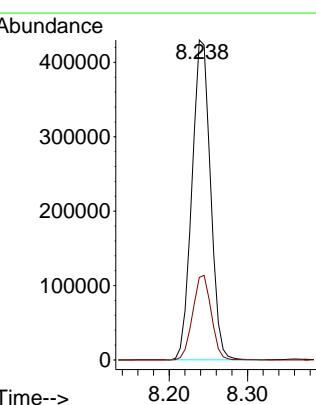





Abundance Scan 1369 (9.433 min): VX045530.D\data.ms

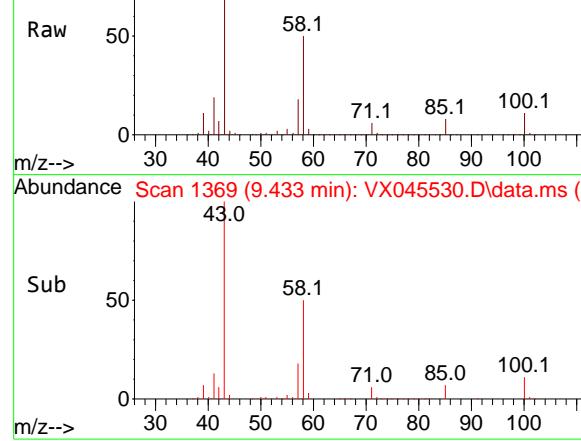


Abundance Scan 1369 (9.433 min): VX045530.D\data.ms (-1)

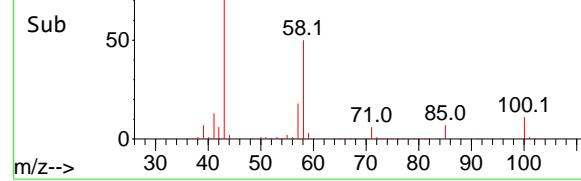


Abundance Scan 1383 (9.519 min): VX045528.D\data.ms (-1)

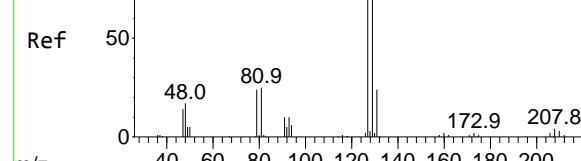

Abundance Scan 1383 (9.519 min): VX045530.D\data.ms

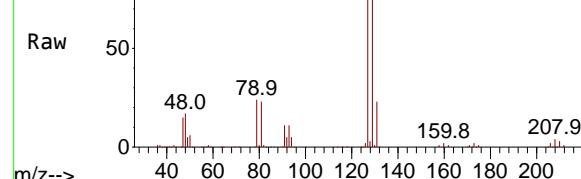

Abundance Scan 1383 (9.519 min): VX045530.D\data.ms (-1)

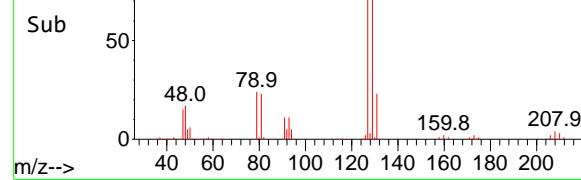

#59

2-Hexanone

Concen: 733.198 ug/l

RT: 9.433 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#60

Dibromochloromethane

Concen: 157.895 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02




Tgt Ion:129 Resp: 194342

Ion Ratio Lower Upper

129 100

127 77.4 39.4 118.2

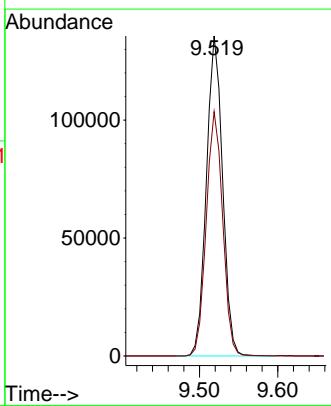

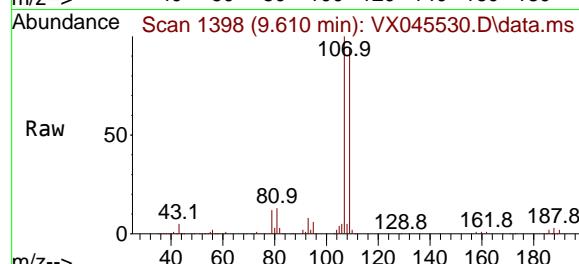

#61

1,2-Dibromoethane

Concen: 152.745 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

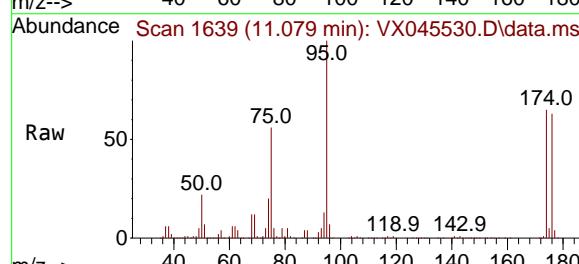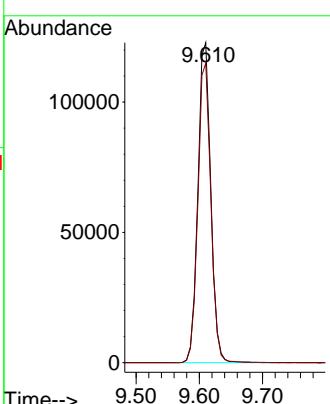

#62

4-Bromofluorobenzene

Concen: 153.035 ug/l


RT: 11.079 min Scan# 1639


Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt	Ion	95	100	Resp:	220921
Ion	Ratio	Lower	Upper		
95	100				
174	66.9	0.0	135.8		
176	64.3	0.0	131.4		

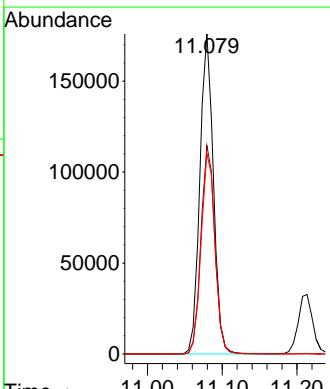

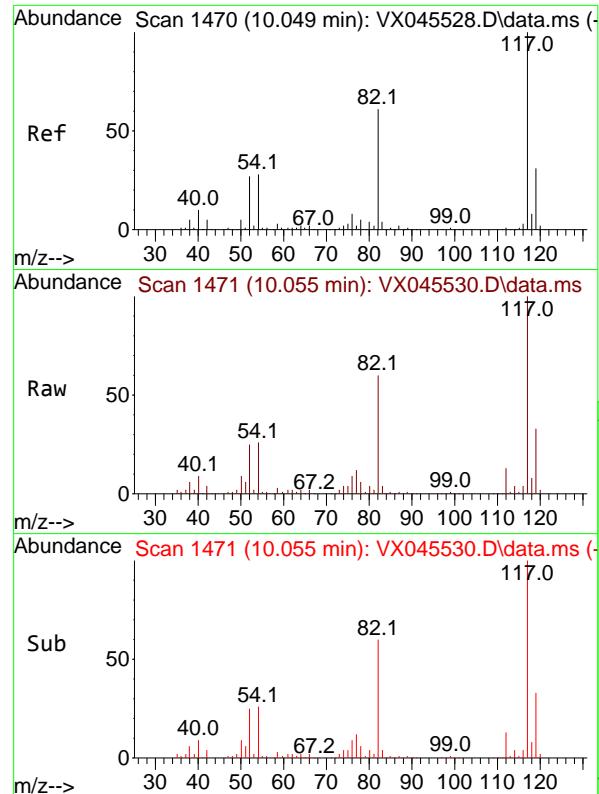

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1470

Delta R.T. 0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

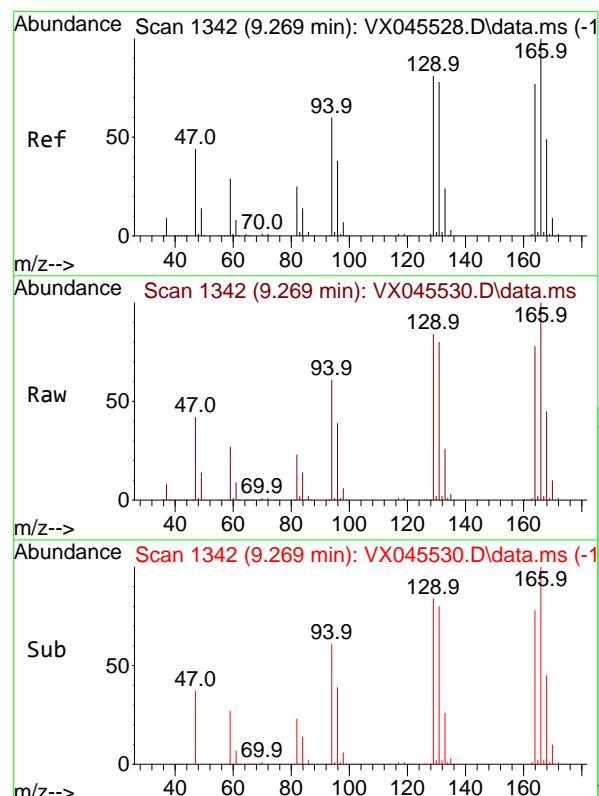

#64

Tetrachloroethene


Concen: 147.568 ug/l



RT: 9.269 min Scan# 1342

Delta R.T. -0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

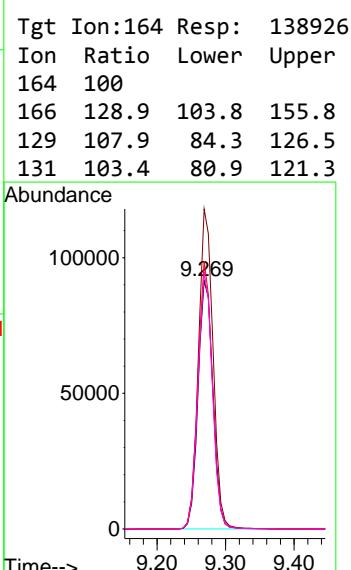

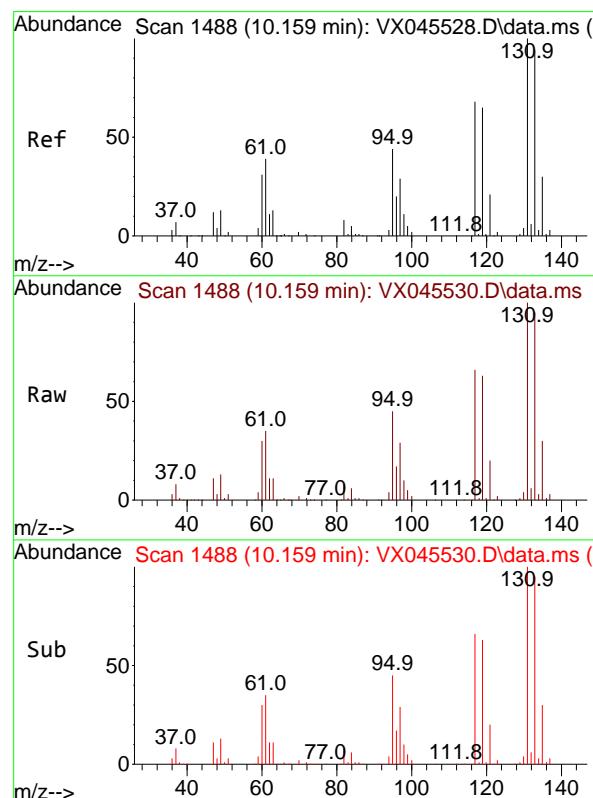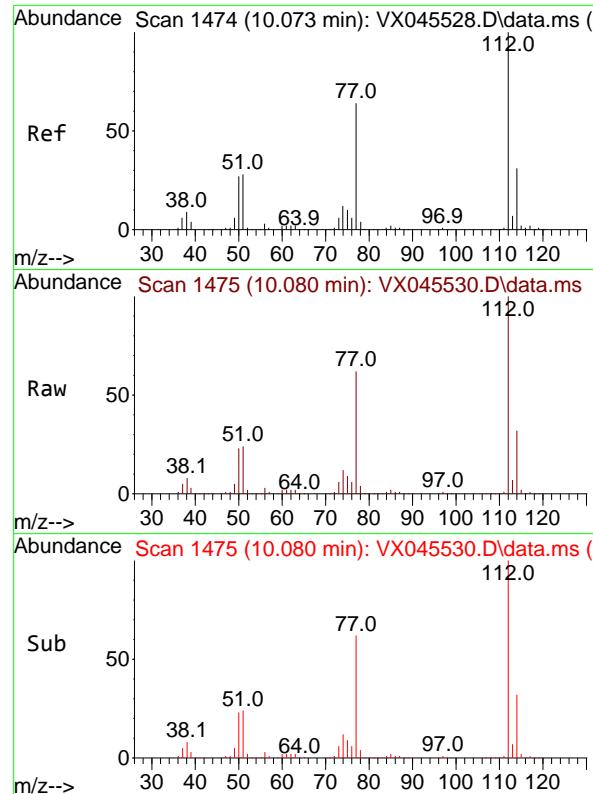

#65

Chlorobenzene

Concen: 156.049 ug/l

RT: 10.080 min Scan# 1475

Delta R.T. 0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC150

Tgt Ion:112 Resp: 44463

Ion Ratio Lower Upper


112 100

114 31.7 24.7 37.1

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#66

1,1,1,2-Tetrachloroethane

Concen: 157.769 ug/l

RT: 10.159 min Scan# 1488

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion:131 Resp: 156069




Ion Ratio Lower Upper

131 100

133 94.6 47.5 142.5

119 64.4 32.9 98.6

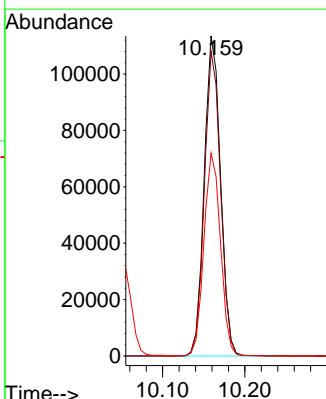



#67

Ethyl Benzene

Concen: 160.907 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

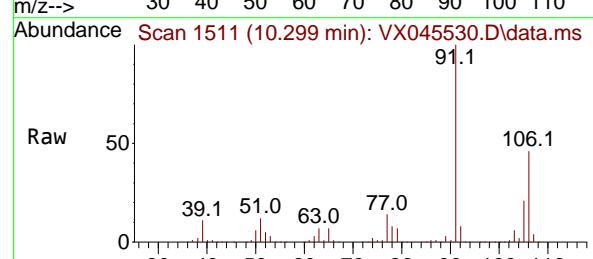

#68

m/p-Xylenes

Concen: 314.231 ug/l


RT: 10.299 min Scan# 1511


Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt Ion:106 Resp: 583228  
 Ion Ratio Lower Upper  
 106 100  
 91 216.7 172.6 258.8

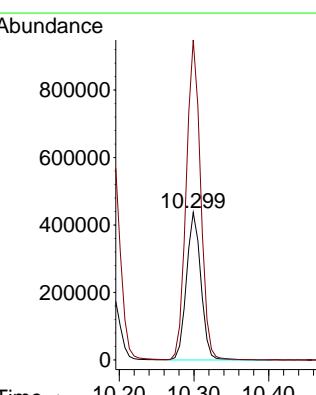


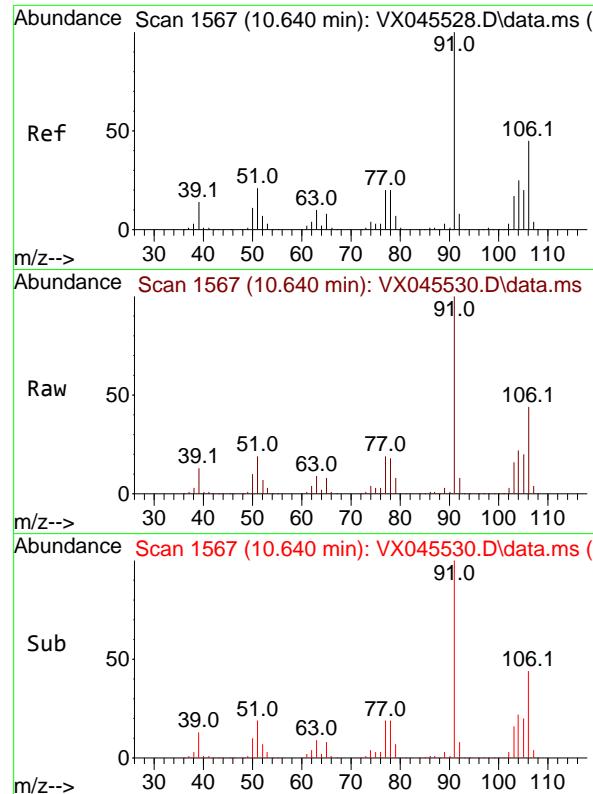


#69  
o-Xylene  
Concen: 156.241 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02  
ClientSampleId : VSTDICC150

Tgt Ion:106 Resp: 285670  
Ion Ratio Lower Upper  
106 100  
91 227.6 113.6 340.6


### Manual Integrations APPROVED







Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

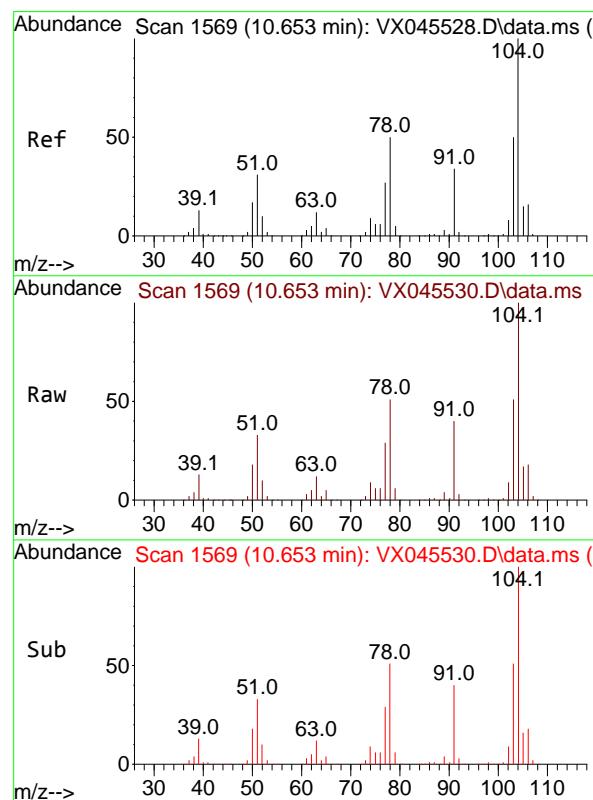

#70  
Styrene  
Concen: 159.299 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Tgt Ion:104 Resp: 480722  
Ion Ratio Lower Upper  
104 100  
78 57.9 45.4 68.2  
103 55.4 43.8 65.8

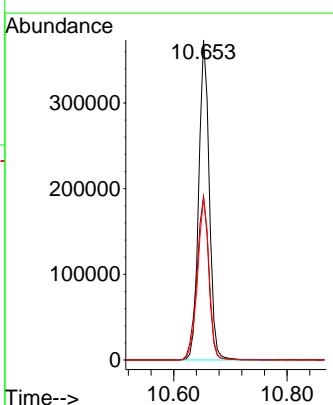

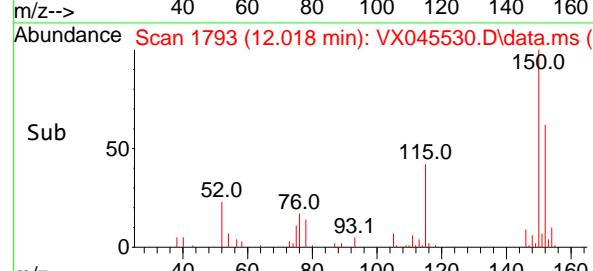

#71

Bromoform

Concen: 170.743 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC150

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l


RT: 12.018 min Scan# 1793


Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt	Ion:	Resp:	
	Ratio	Lower	Upper
152	100		
115	151.4	46.9	140.7
150	208.6	0.0	349.4



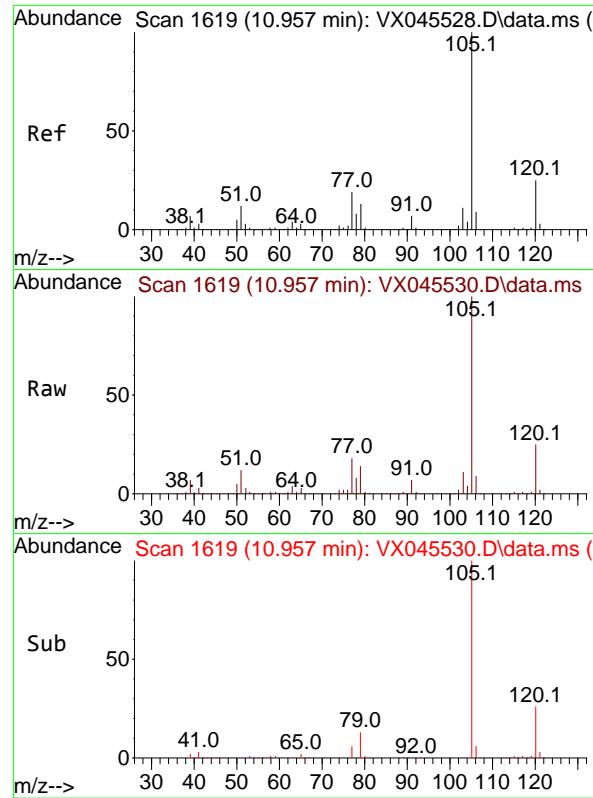

#73

Isopropylbenzene

Concen: 155.475 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

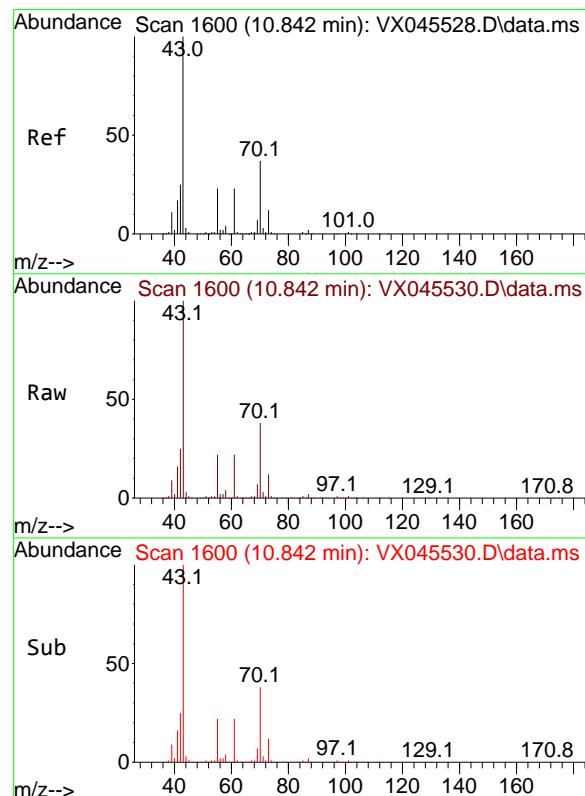

#74

N-amyl acetate

Concen: 173.877 ug/l


RT: 10.842 min Scan# 1600


Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt	Ion:	43	Resp:	408934
Ion	Ratio	Lower	Upper	
43	100			
70	38.3	30.1	45.1	
55	22.0	18.3	27.5	
61	22.3	17.5	26.3	

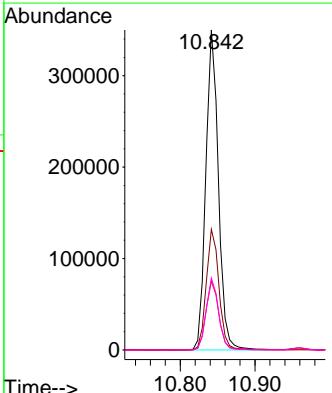


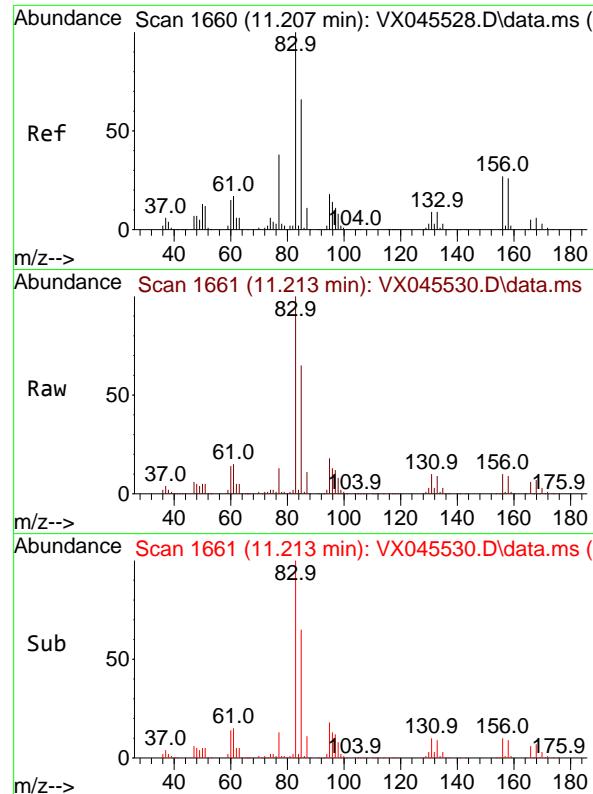


#75  
1,1,2,2-Tetrachloroethane  
Concen: 144.737 ug/l  
RT: 11.213 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

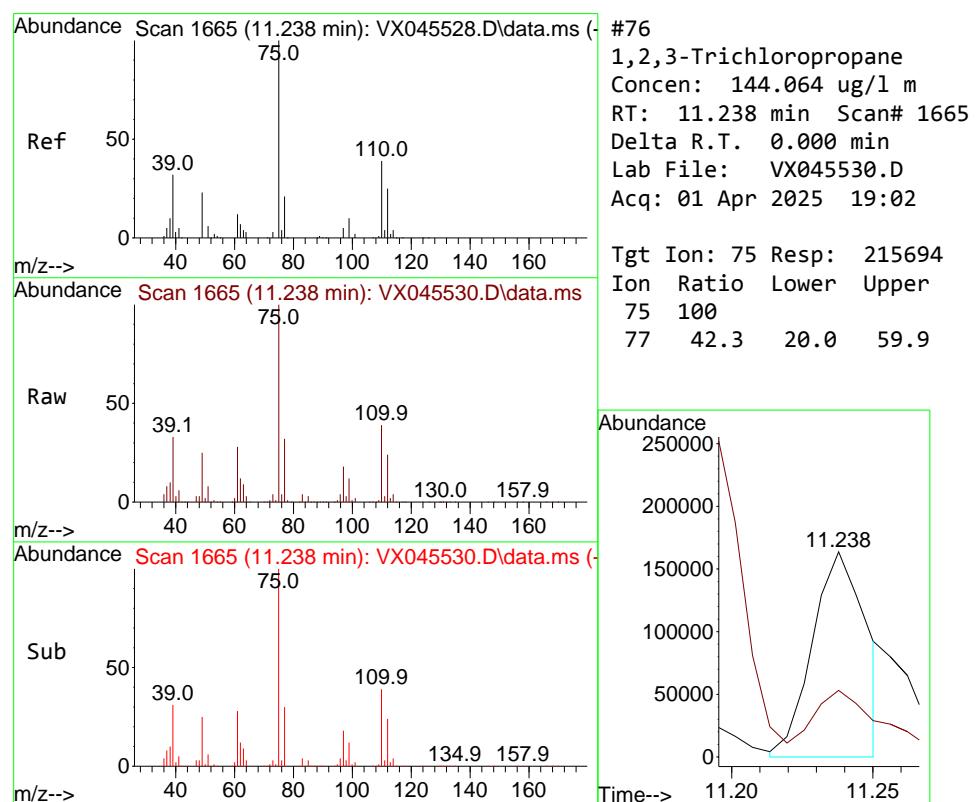

#76  
1,2,3-Trichloropropane  
Concen: 144.064 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Tgt Ion: 75 Resp: 215694  
Ion Ratio Lower Upper  
75 100  
77 42.3 20.0 59.9

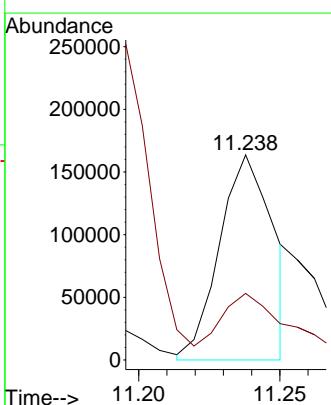

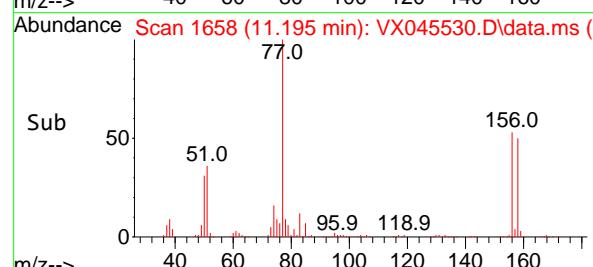

#77

Bromobenzene

Concen: 151.033 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#78

n-propylbenzene

Concen: 158.408 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.006 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02




Tgt Ion: 91 Resp: 897084

Ion Ratio Lower Upper

91 100

120 21.5 10.8 32.3

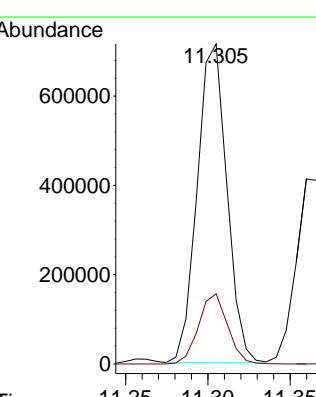



#79

2-Chlorotoluene

Concen: 148.399 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#80

1,3,5-Trimethylbenzene

Concen: 152.700 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045530.D



Acq: 01 Apr 2025 19:02

Tgt Ion:105 Resp: 620819

Ion Ratio Lower Upper

105 100

120 46.1 23.0 69.0

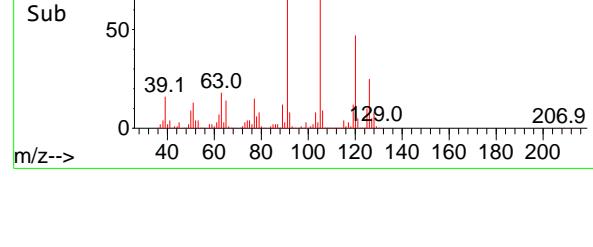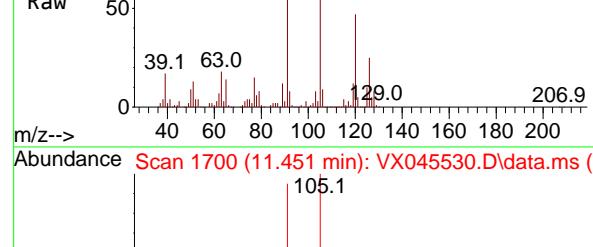

Abundance

500000 11.451

400000


300000

200000

100000

0

Time--&gt; 11.40 11.45 11.50


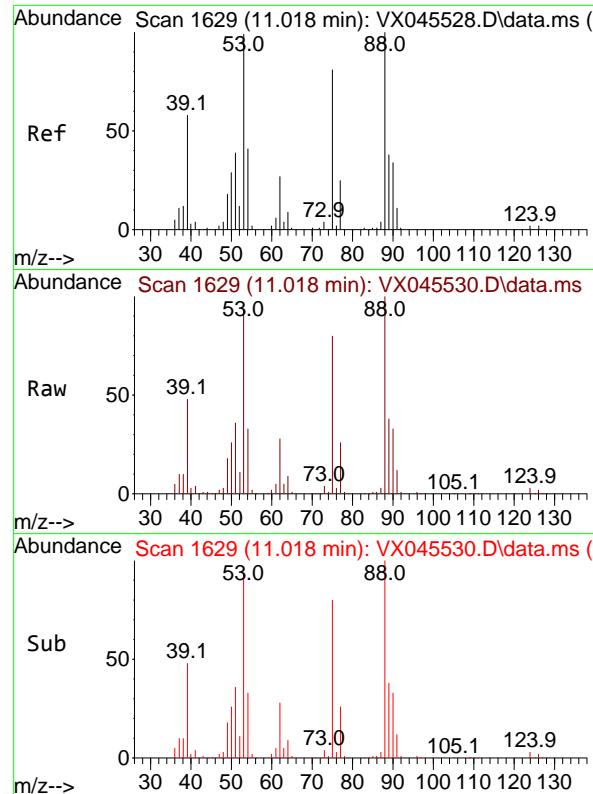


#81  
trans-1,4-Dichloro-2-butene  
Concen: 178.636 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

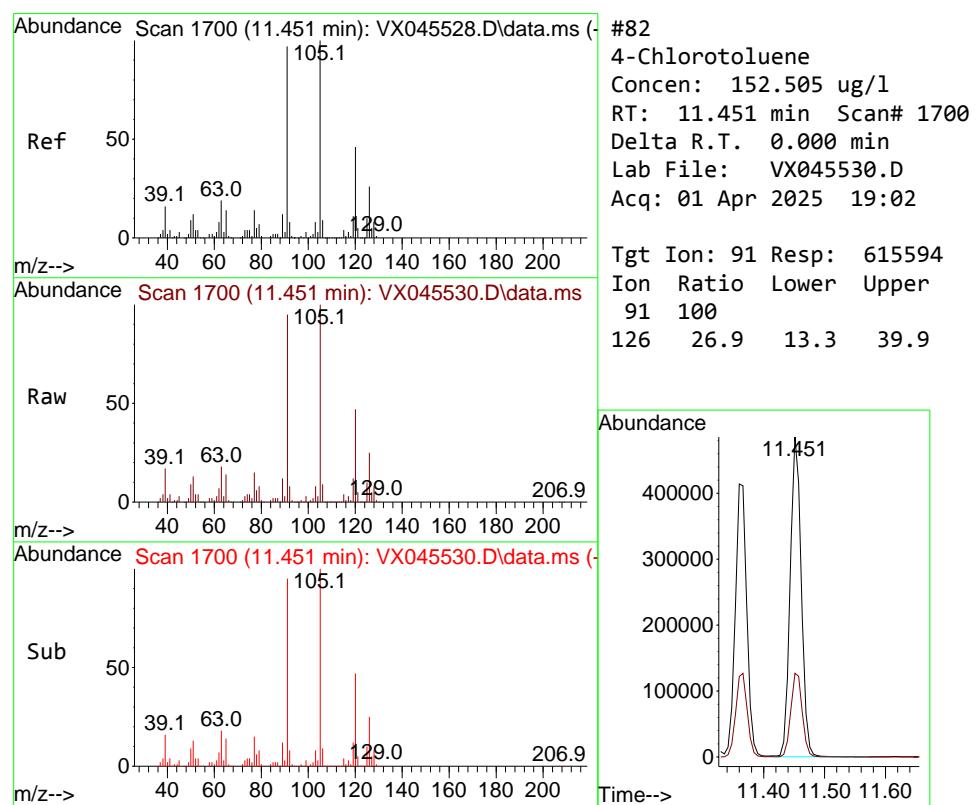

#82  
4-Chlorotoluene  
Concen: 152.505 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Tgt Ion: 91 Resp: 615594  
Ion Ratio Lower Upper  
91 100  
126 26.9 13.3 39.9

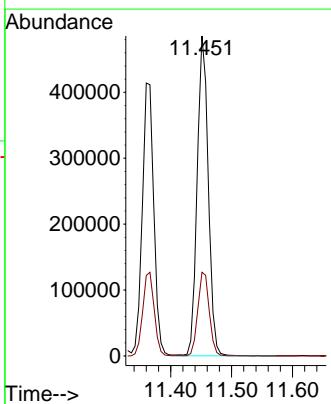

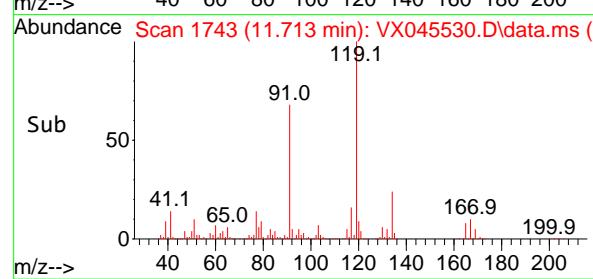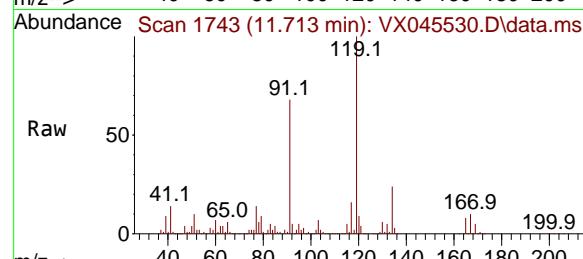

#83

tert-Butylbenzene

Concen: 155.783 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

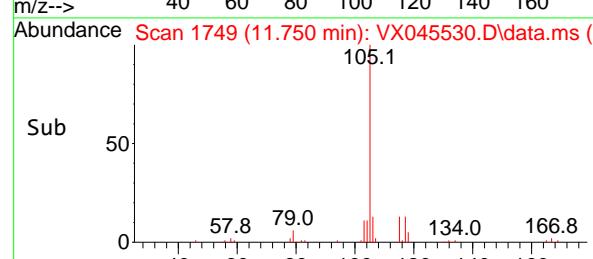

#84

1,2,4-Trimethylbenzene

Concen: 154.317 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045530.D


Acq: 01 Apr 2025 19:02



Tgt Ion:105 Resp: 629704

Ion Ratio Lower Upper

105 100

120 42.7 21.4 64.3

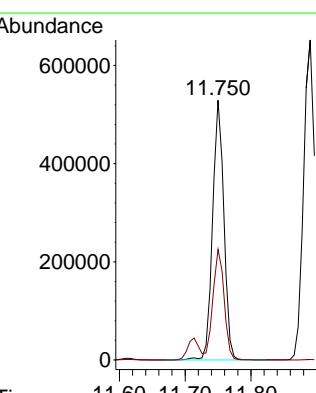



#85

sec-Butylbenzene

Concen: 159.869 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

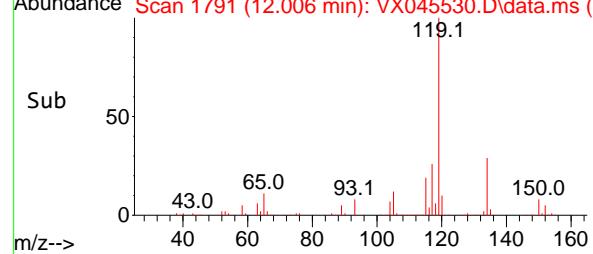

#86

p-Isopropyltoluene

Concen: 157.397 ug/l


RT: 12.006 min Scan# 1791


Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt	Ion:119	Resp:	641521
Ion	Ratio	Lower	Upper
119	100		
134	25.3	12.6	37.8
91	27.6	13.7	41.1

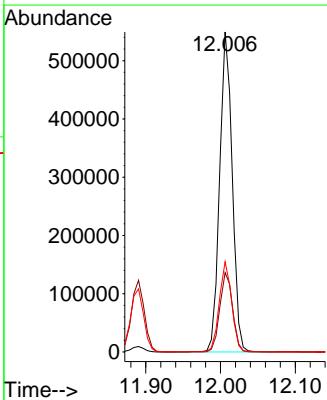

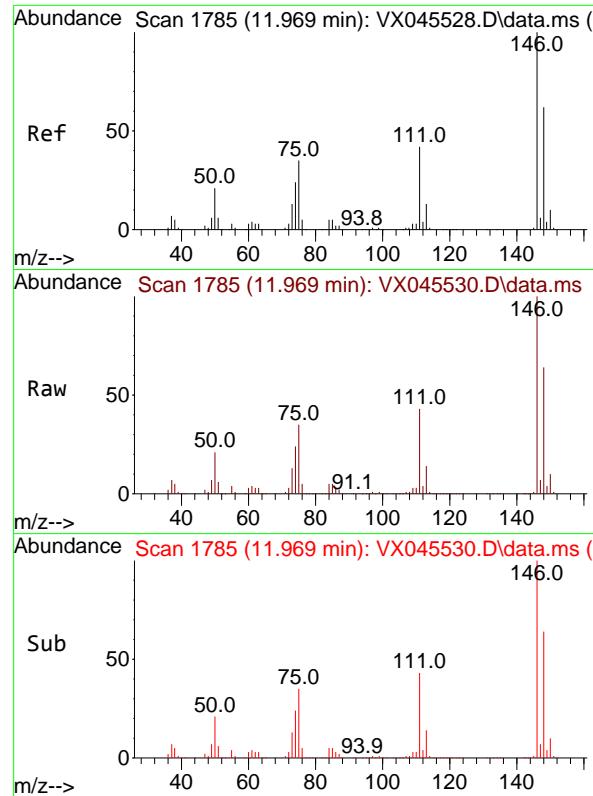

#87

1,3-Dichlorobenzene

Concen: 151.885 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

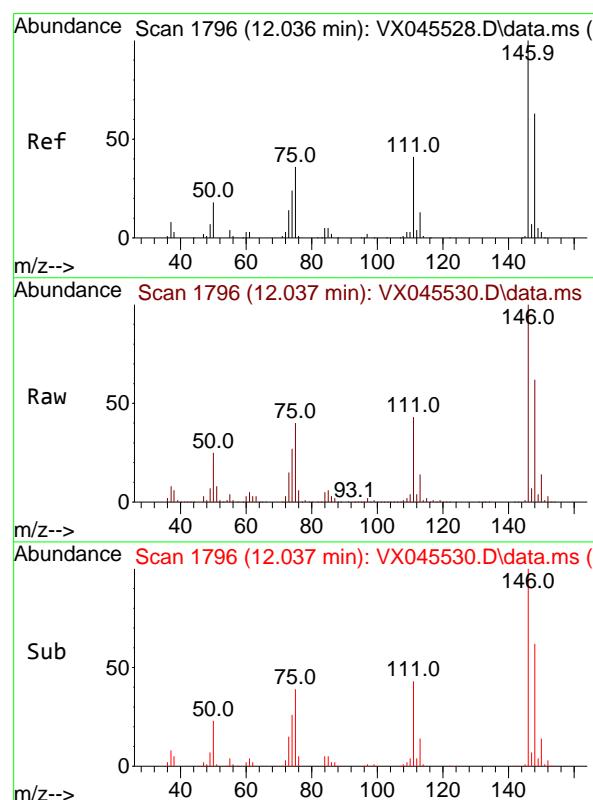

#88

1,4-Dichlorobenzene

Concen: 149.876 ug/l

RT: 12.037 min Scan# 1796

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt

Ion

Ratio

Lower

Upper

146

100

111

42.3

20.9


62.8


148

63.5

31.5

94.5

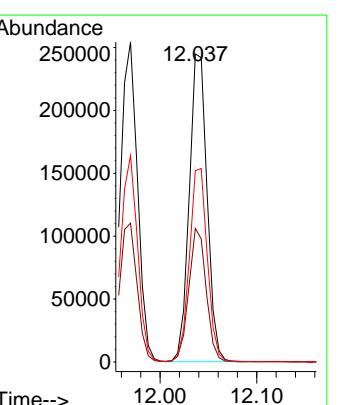

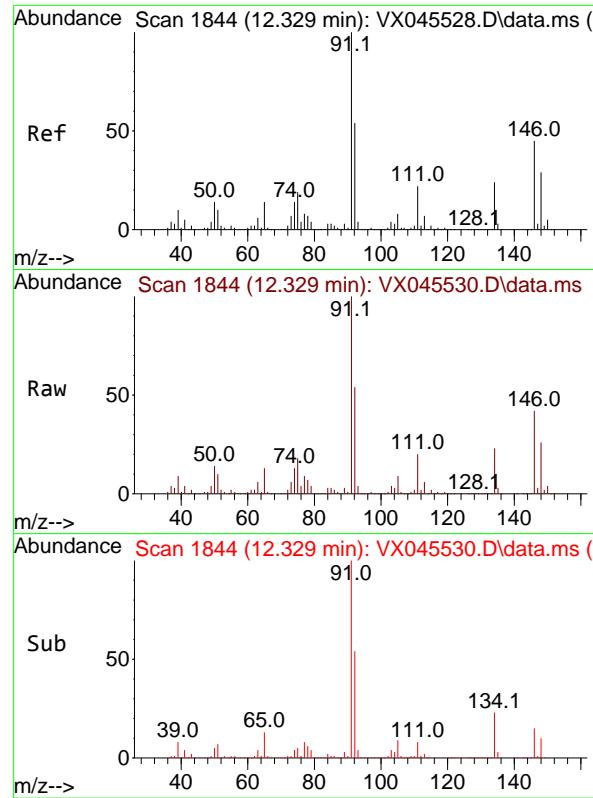

#89

n-Butylbenzene

Concen: 171.019 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

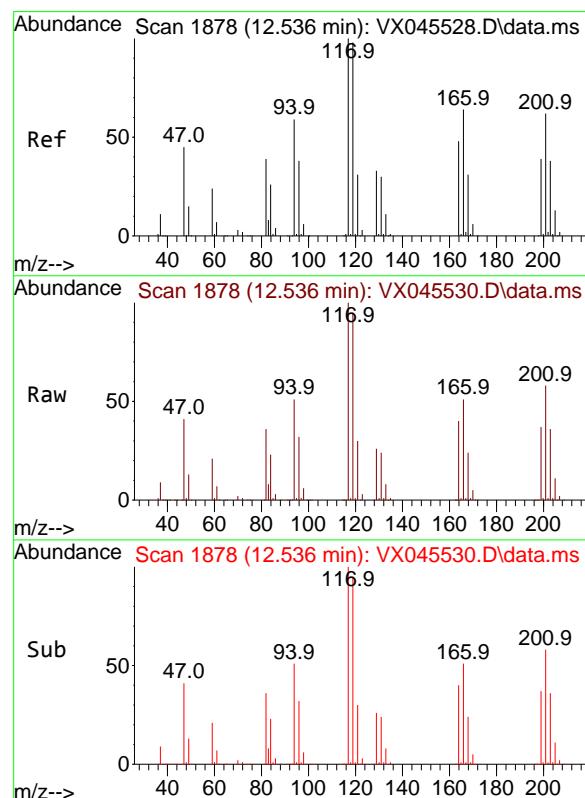

#90

Hexachloroethane

Concen: 173.829 ug/l

RT: 12.536 min Scan# 1878


Delta R.T. 0.000 min




Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Tgt Ion:117 Resp: 121761

Ion	Ratio	Lower	Upper
117	100		
201	61.9	31.2	93.6

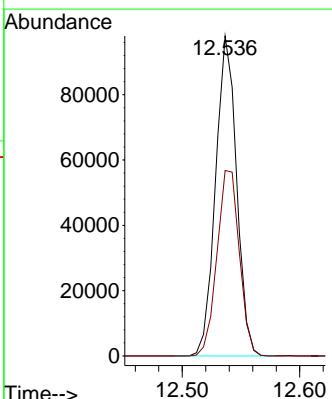



#91

1,2-Dichlorobenzene

Concen: 149.342 ug/l

RT: 12.335 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#92

1,2-Dibromo-3-Chloropropane

Concen: 178.062 ug/l

RT: 12.939 min Scan# 1944

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02


Tgt Ion: 75 Resp: 64317




Ion Ratio Lower Upper

75 100

155 69.7 34.9 104.7

157 91.3 44.9 134.7

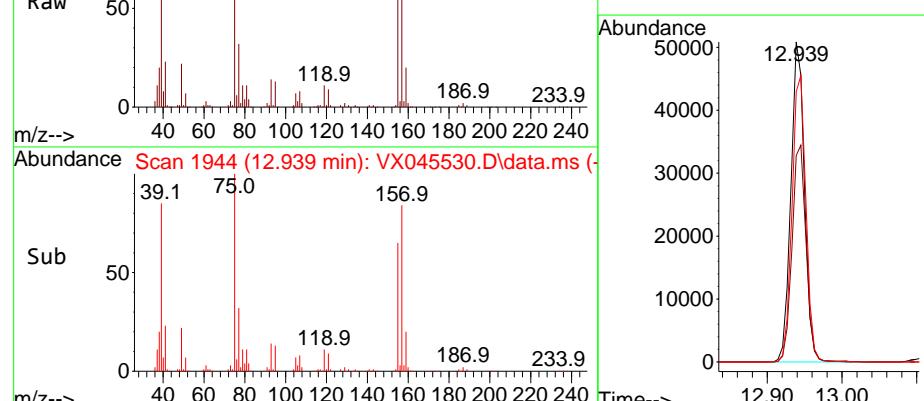



#93

1,2,4-Trichlorobenzene

Concen: 174.213 ug/l

RT: 13.585 min Scan# 2050

Delta R.T. 0.000 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#94

Hexachlorobutadiene

Concen: 157.752 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. 0.006 min

Lab File: VX045530.D

Acq: 01 Apr 2025 19:02































Tgt Ion:225 Resp: 77792


Ion Ratio Lower Upper

225 100

223 63.4 31.1 93.3

227 63.8 32.2 96.6

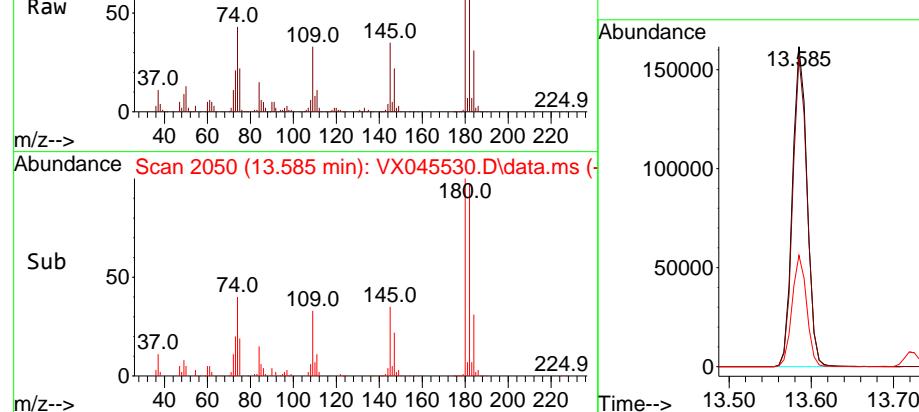


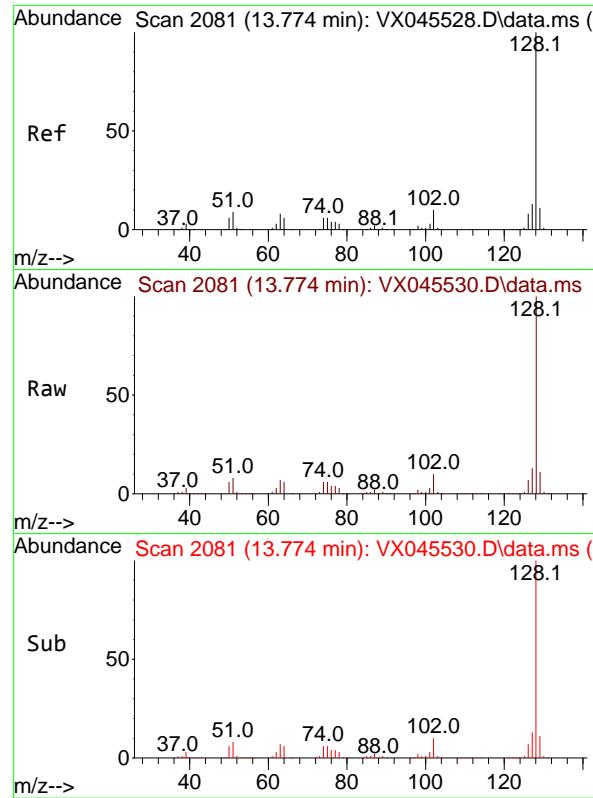


#95  
Naphthalene  
Concen: 172.191 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

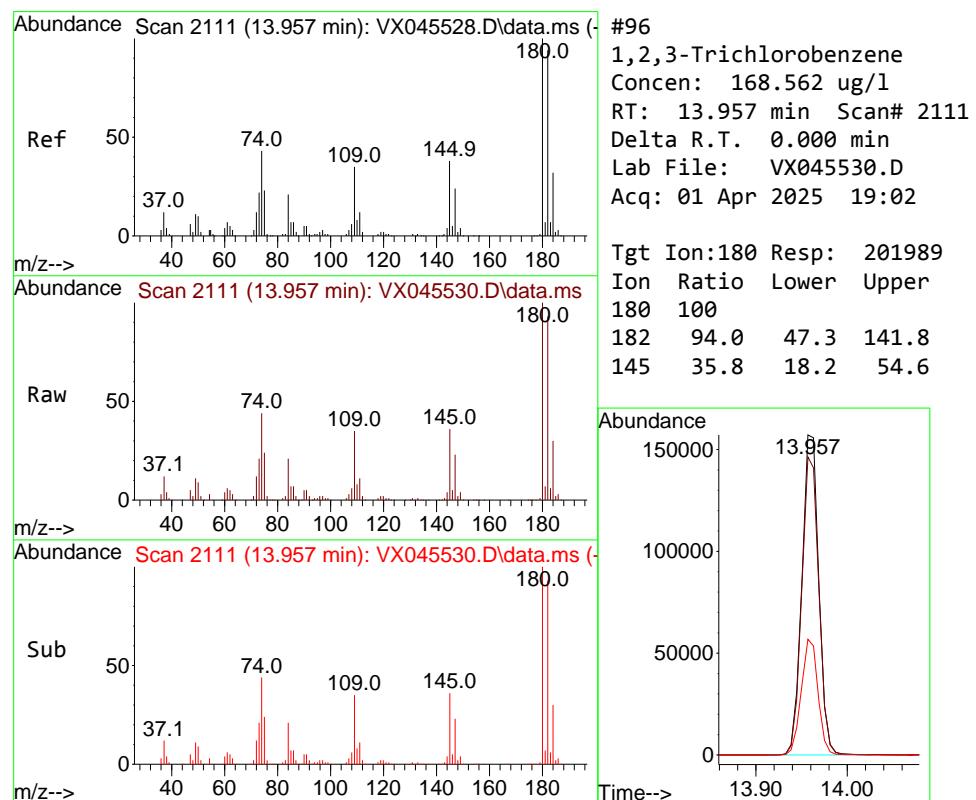

#96  
1,2,3-Trichlorobenzene  
Concen: 168.562 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045530.D  
Acq: 01 Apr 2025 19:02

Tgt Ion:180 Resp: 201989  
Ion Ratio Lower Upper  
180 100  
182 94.0 47.3 141.8  
145 35.8 18.2 54.6

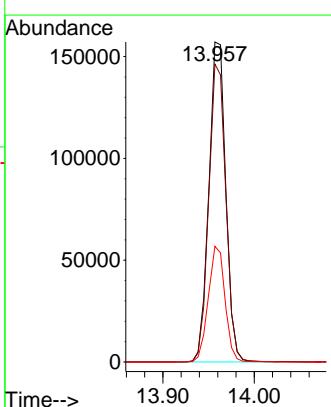

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045532.D  
 Acq On : 01 Apr 2025 19:48  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX040225**

Quant Time: Apr 02 03:14:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	96972	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	174855	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	152417	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	67633	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	89251	50.329	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125			Recovery =	100.660%	
35) Dibromofluoromethane	5.379	113	61107	49.256	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124			Recovery =	98.520%	
50) Toluene-d8	8.647	98	217200	50.160	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113			Recovery =	100.320%	
62) 4-Bromofluorobenzene	11.079	95	80376	50.959	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121			Recovery =	101.920%	
<b>Target Compounds</b>						
				<b>Qvalue</b>		
2) Dichlorodifluoromethane	1.166	85	76070	52.454	ug/l	97
3) Chloromethane	1.301	50	72033	48.349	ug/l	99
4) Vinyl Chloride	1.374	62	66559	48.816	ug/l	99
5) Bromomethane	1.593	94	30379	46.991	ug/l	99
6) Chloroethane	1.672	64	37317	51.586	ug/l	100
7) Trichlorofluoromethane	1.880	101	102379	50.354	ug/l	96
8) Diethyl Ether	2.130	74	33603	49.228	ug/l	99
9) 1,1,2-Trichlorotrifluo...	2.325	101	59007	49.528	ug/l	98
10) Methyl Iodide	2.447	142	72261	48.626	ug/l	99
11) Tert butyl alcohol	2.971	59	58774	246.612	ug/l	99
12) 1,1-Dichloroethene	2.313	96	57888	49.726	ug/l	99
13) Acrolein	2.233	56	78156	238.141	ug/l	99
14) Allyl chloride	2.660	41	111636	50.541	ug/l	99
15) Acrylonitrile	3.062	53	186837	248.351	ug/l	100
16) Acetone	2.380	43	176153	241.904	ug/l	99
17) Carbon Disulfide	2.508	76	149677	52.057	ug/l	100
18) Methyl Acetate	2.703	43	81720	48.742	ug/l	100
19) Methyl tert-butyl Ether	3.111	73	207487	50.950	ug/l	100
20) Methylene Chloride	2.782	84	66875	49.055	ug/l	99
21) trans-1,2-Dichloroethene	3.087	96	59229	49.800	ug/l	98
22) Diisopropyl ether	3.757	45	221449	50.895	ug/l	92
23) Vinyl Acetate	3.715	43	1005423	267.449	ug/l	99
24) 1,1-Dichloroethane	3.605	63	122240	49.677	ug/l	99
25) 2-Butanone	4.550	43	271686	254.882	ug/l	97
26) 2,2-Dichloropropane	4.471	77	82704	52.020	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	71072	49.049	ug/l	98
28) Bromochloromethane	4.891	49	57557	48.403	ug/l	99
29) Tetrahydrofuran	5.001	42	172405	249.473	ug/l	100
30) Chloroform	5.086	83	125621	49.614	ug/l	98
31) Cyclohexane	5.458	56	107862	49.583	ug/l	97
32) 1,1,1-Trichloroethane	5.379	97	107830	50.330	ug/l	99
36) 1,1-Dichloropropene	5.684	75	83901	50.088	ug/l	99
37) Ethyl Acetate	4.708	43	105095	49.787	ug/l	98
38) Carbon Tetrachloride	5.672	117	91723	50.667	ug/l	100
39) Methylcyclohexane	7.373	83	102919	50.124	ug/l	99
40) Benzene	6.031	78	251758	49.212	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045532.D  
 Acq On : 01 Apr 2025 19:48  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX040225**

Quant Time: Apr 02 03:14:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.916	41	59140	53.098	ug/l	99
42) 1,2-Dichloroethane	6.080	62	103270	48.875	ug/l	100
43) Isopropyl Acetate	6.336	43	164894	51.539	ug/l	100
44) Trichloroethene	7.123	130	57931	47.643	ug/l	92
45) 1,2-Dichloropropane	7.421	63	63210	49.521	ug/l	95
46) Dibromomethane	7.574	93	47564	48.542	ug/l	97
47) Bromodichloromethane	7.818	83	96418	49.273	ug/l	96
48) Methyl methacrylate	7.690	41	85084	51.507	ug/l	99
49) 1,4-Dioxane	7.659	88	28552	955.327	ug/l	99
51) 4-Methyl-2-Pentanone	8.568	43	540822	254.994	ug/l	100
52) Toluene	8.714	92	151664	48.994	ug/l	100
53) t-1,3-Dichloropropene	8.976	75	87744	46.783	ug/l	98
54) cis-1,3-Dichloropropene	8.360	75	99074	53.878	ug/l	98
55) 1,1,2-Trichloroethane	9.147	97	60452	49.007	ug/l	97
56) Ethyl methacrylate	9.116	69	102525	53.705	ug/l	100
57) 1,3-Dichloropropane	9.305	76	107121	49.869	ug/l	100
58) 2-Chloroethyl Vinyl ether	8.238	63	251285	260.201	ug/l	99
59) 2-Hexanone	9.427	43	395336	251.710	ug/l	100
60) Dibromochloromethane	9.519	129	68562	50.983	ug/l	99
61) 1,2-Dibromoethane	9.604	107	63301	50.693	ug/l	100
64) Tetrachloroethene	9.269	164	50834	47.239	ug/l	99
65) Chlorobenzene	10.073	112	163518	50.207	ug/l	98
66) 1,1,1,2-Tetrachloroethane	10.159	131	57096	50.495	ug/l	99
67) Ethyl Benzene	10.189	91	300747	51.558	ug/l	100
68) m/p-Xylenes	10.299	106	217943	102.728	ug/l	99
69) o-Xylene	10.640	106	107947	51.650	ug/l	100
70) Styrene	10.653	104	181524	52.624	ug/l	100
71) Bromoform	10.799	173	44489	52.694	ug/l #	98
73) Isopropylbenzene	10.957	105	286010	52.794	ug/l	100
74) N-amyl acetate	10.842	43	140941	54.387	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	92505	48.608	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	82060m	49.741	ug/l	
77) Bromobenzene	11.195	156	63244	50.525	ug/l	98
78) n-propylbenzene	11.299	91	336753	53.967	ug/l	100
79) 2-Chlorotoluene	11.360	91	203677	51.057	ug/l	99
80) 1,3,5-Trimethylbenzene	11.445	105	239822	53.534	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.018	75	25511	52.482	ug/l	98
82) 4-Chlorotoluene	11.451	91	233159	52.422	ug/l	100
83) tert-Butylbenzene	11.713	119	236276	53.274	ug/l	100
84) 1,2,4-Trimethylbenzene	11.750	105	238257	52.990	ug/l	100
85) sec-Butylbenzene	11.890	105	293633	53.903	ug/l	100
86) p-Isopropyltoluene	12.006	119	244031	54.337	ug/l	99
87) 1,3-Dichlorobenzene	11.963	146	115113	50.521	ug/l	100
88) 1,4-Dichlorobenzene	12.036	146	113458	49.117	ug/l	97
89) n-Butylbenzene	12.329	91	214931	55.189	ug/l	99
90) Hexachloroethane	12.536	117	41729	54.066	ug/l	98
91) 1,2-Dichlorobenzene	12.329	146	113126	49.938	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	21184	53.226	ug/l	100
93) 1,2,4-Trichlorobenzene	13.585	180	65488	51.935	ug/l	98
94) Hexachlorobutadiene	13.725	225	27147	49.961	ug/l	99
95) Naphthalene	13.774	128	247600	52.765	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	66542	50.396	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045532.D  
 Acq On : 01 Apr 2025 19:48  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
ICVVX040225

Quant Time: Apr 02 03:14:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045532.D  
 Acq On : 01 Apr 2025 19:48  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1




Quant Time: Apr 02 03:14:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025

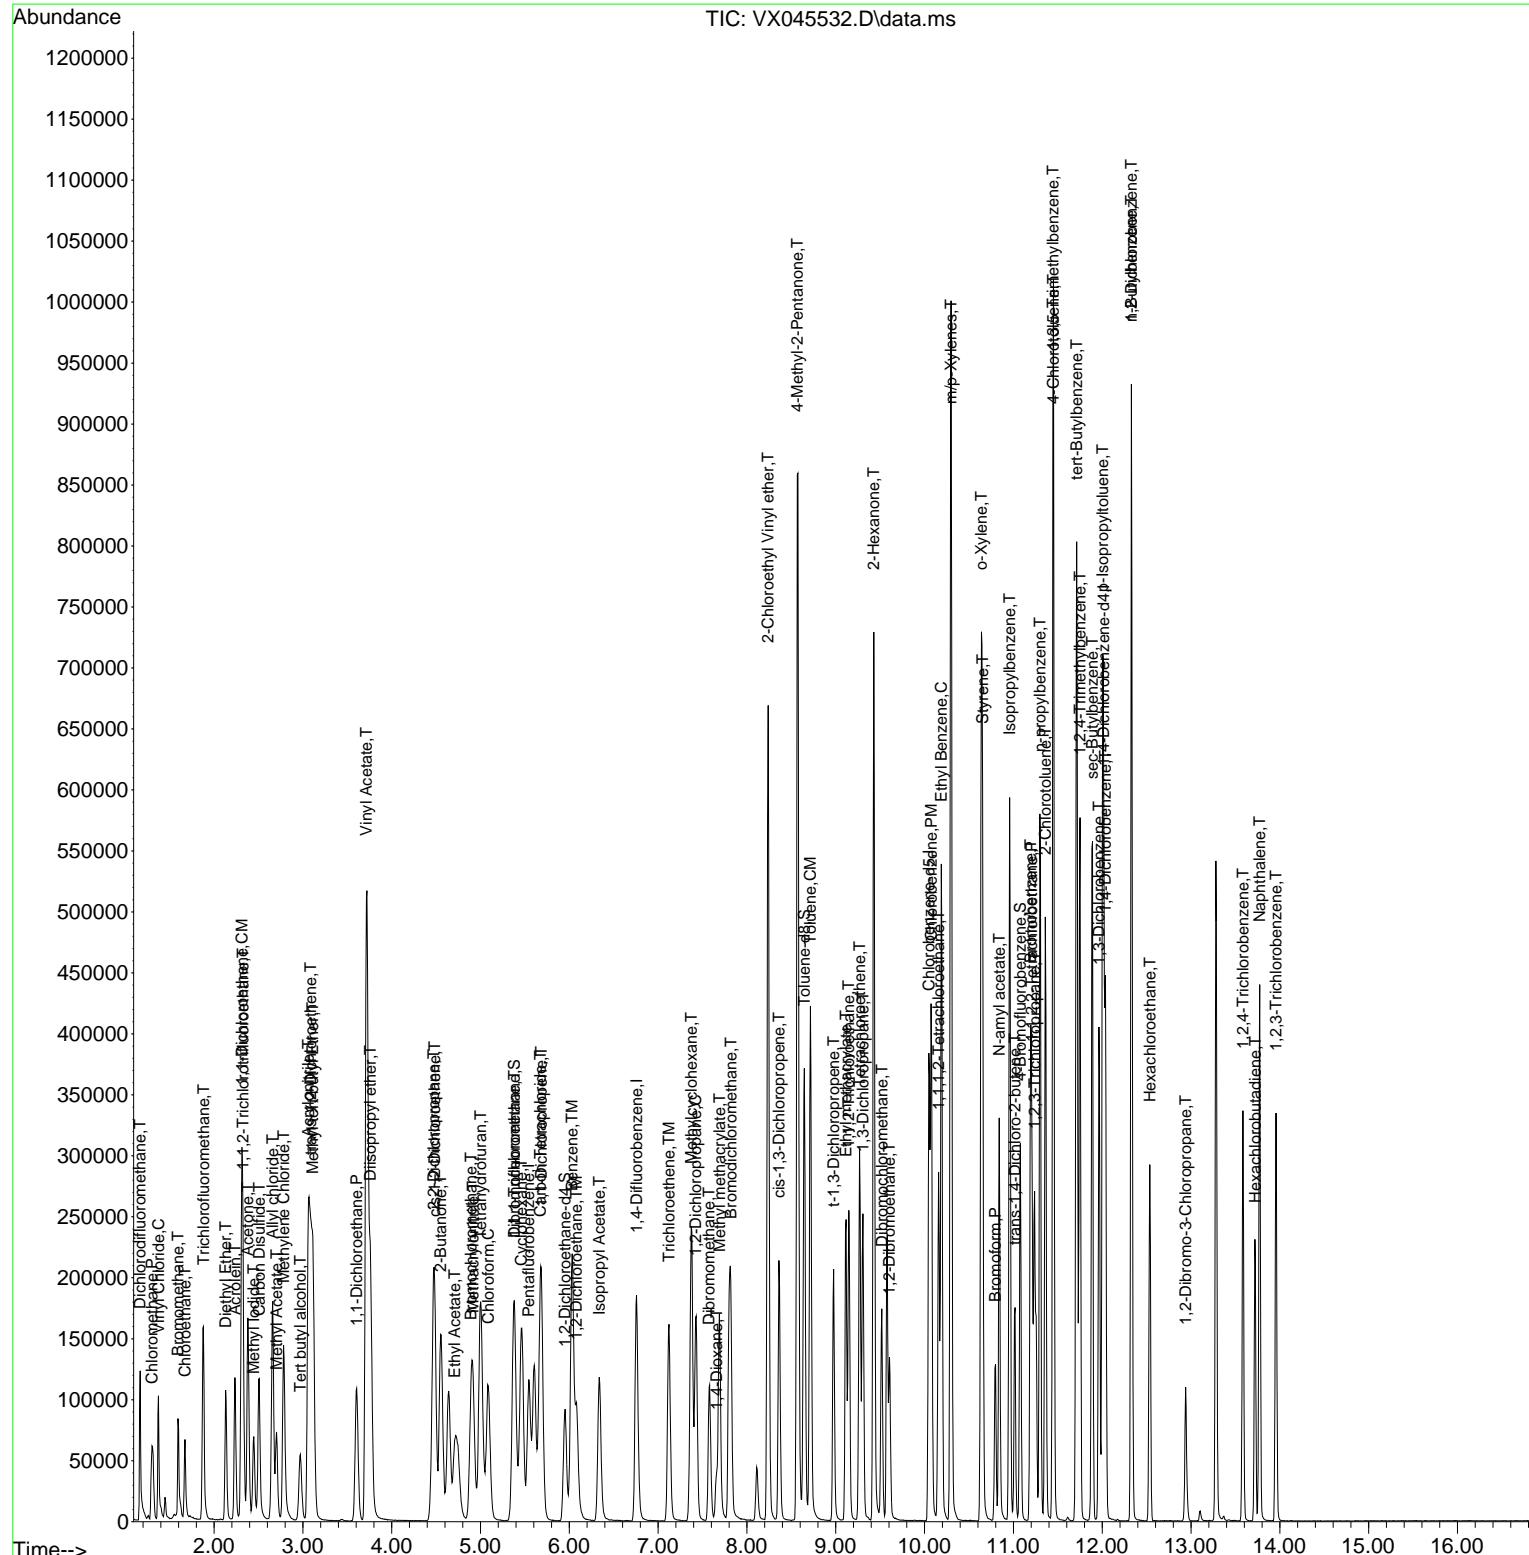







#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.544 min Scan# 7  
Instrument : MSVOA\_X  
Delta R.T. -0.006 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

ClientSampleId : ICVVX040225


### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

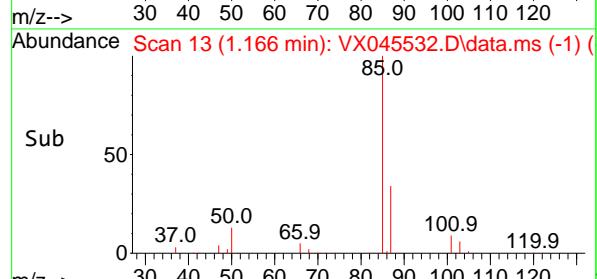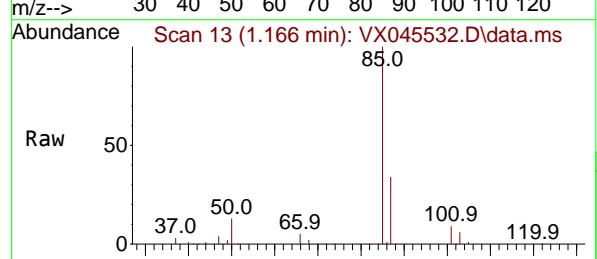


#2  
Dichlorodifluoromethane  
Concen: 52.454 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion: 85 Resp: 76070  
Ion Ratio Lower Upper  
85 100  
87 33.6 16.1 48.2


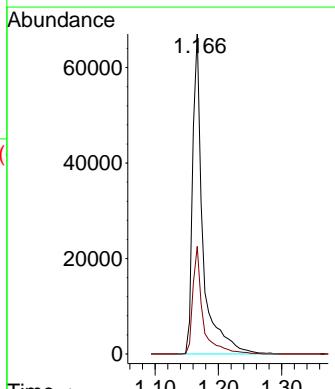





Abundance Scan 35 (1.301 min): VX045532.D\data.ms

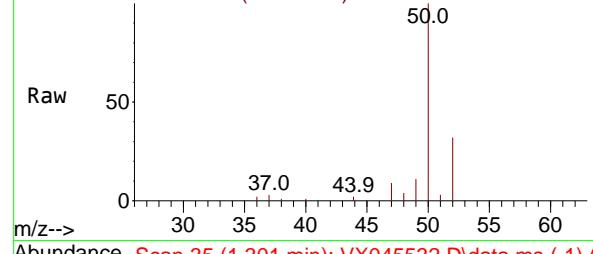


Abundance Scan 35 (1.301 min): VX045532.D\data.ms (-1)

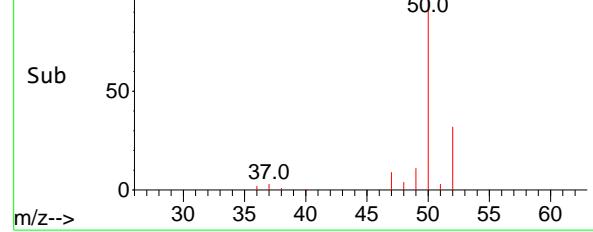

Abundance Scan 47 (1.374 min): VX045532.D\data.ms

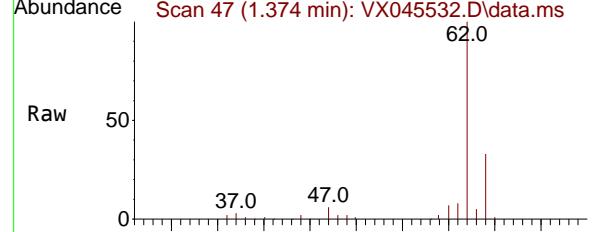

Abundance Scan 47 (1.374 min): VX045532.D\data.ms (-1)

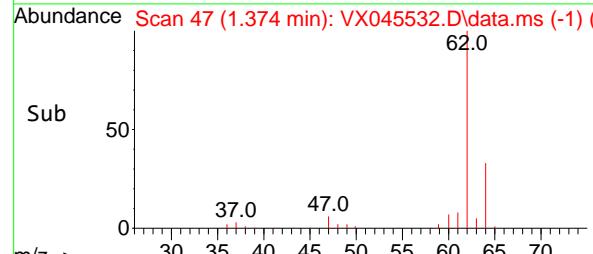

#3

Chloromethane

Concen: 48.349 ug/l

RT: 1.301 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#4

Vinyl Chloride

Concen: 48.816 ug/l


RT: 1.374 min Scan# 47




Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt Ion: 62 Resp: 66559  
Ion Ratio Lower Upper  
62 100  
64 32.5 25.5 38.3

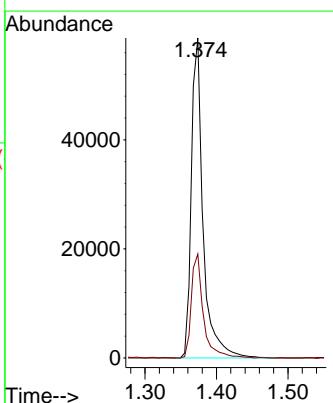






#5  
 Bromomethane  
 Concen: 46.991 ug/l  
 RT: 1.593 min Scan# 8  
 Delta R.T. 0.000 min  
 Lab File: VX045532.D  
 Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
 ClientSampleId : ICVVX040225



Manual Integrations  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
 Supervised By :Mahesh Dadoda 04/02/2025



#6  
 Chloroethane  
 Concen: 51.586 ug/l  
 RT: 1.672 min Scan# 96  
 Delta R.T. 0.006 min  
 Lab File: VX045532.D  
 Acq: 01 Apr 2025 19:48


Tgt Ion: 64 Resp: 37317  
 Ion Ratio Lower Upper  
 64 100  
 66 33.0 26.3 39.5





#7  
Trichlorofluoromethane  
Concen: 50.354 ug/l  
RT: 1.880 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48




Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225






Tgt Ion:101 Resp: 102379  
Ion Ratio Lower Upper  
101 100  
103 67.2 51.1 76.7




Manual Integrations  
APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

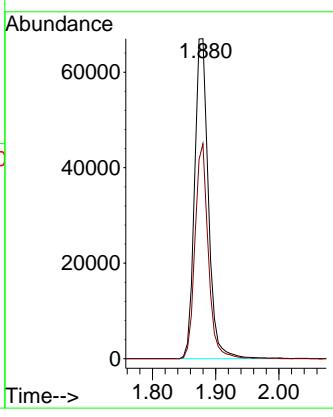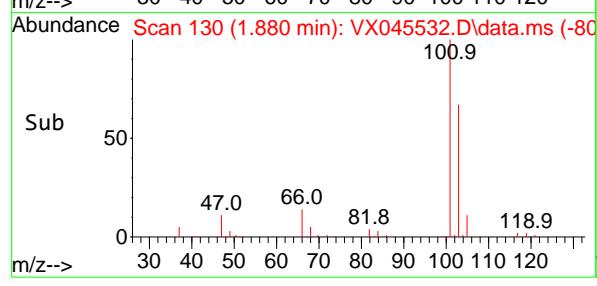

#8  
Diethyl Ether  
Concen: 49.228 ug/l  
RT: 2.130 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48



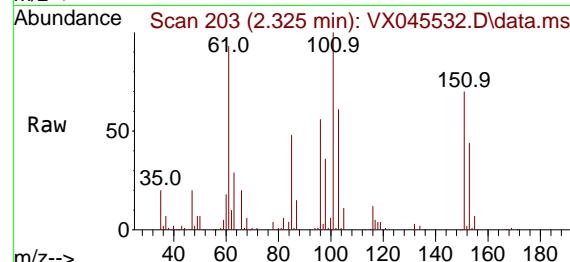

#9

1,1,2-Trichlorotrifluoroethane

Concen: 49.528 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

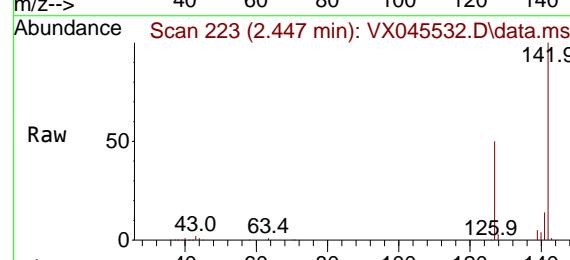

#10

Methyl Iodide

Concen: 48.626 ug/l

RT: 2.447 min Scan# 223

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt Ion:142 Resp: 72261

Ion Ratio Lower Upper

142 100


127 50.6 40.2 60.4

141 14.1 11.7 17.5

Abundance

2.447

Time--&gt; 2.40 2.50 2.60

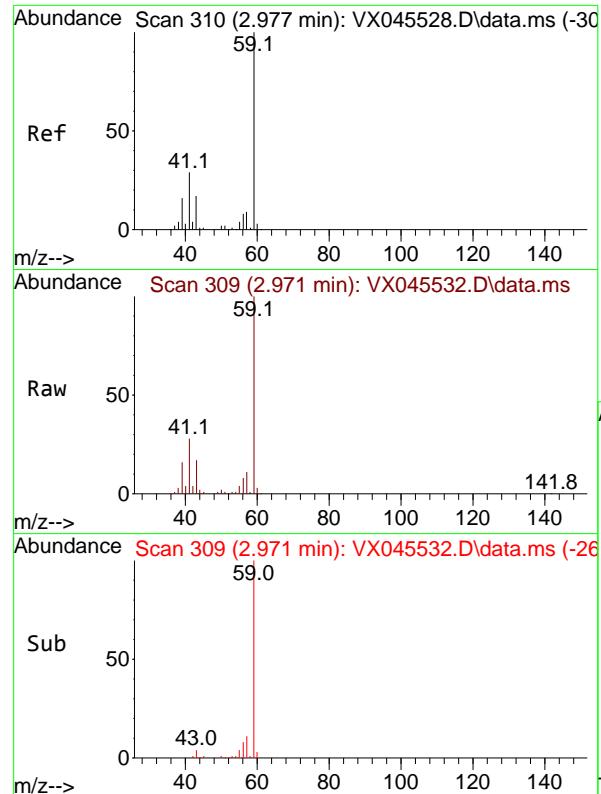



#11

Tert butyl alcohol  
Concen: 246.612 ug/l  
RT: 2.971 min Scan# 3  
Delta R.T. -0.006 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225

### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

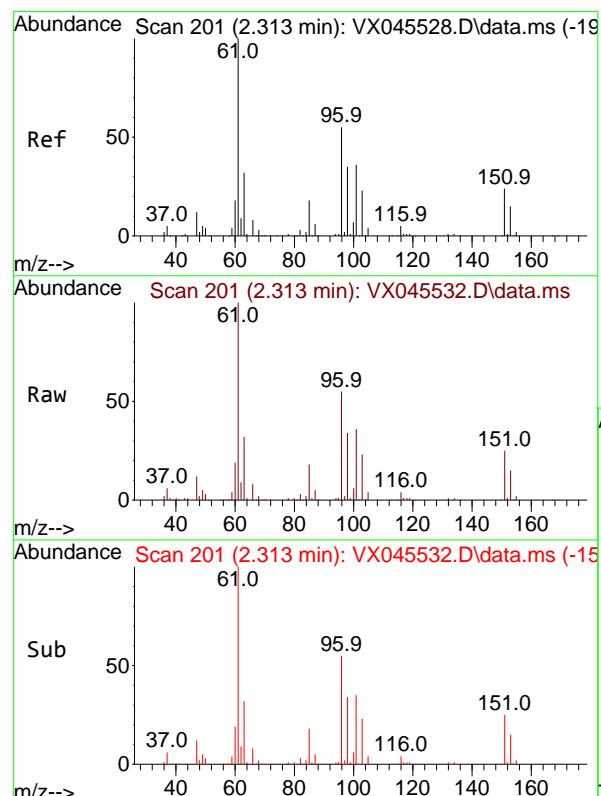


#12


1,1-Dichloroethene  
Concen: 49.726 ug/l  
RT: 2.313 min Scan# 201  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion: 96 Resp: 57888  
Ion Ratio Lower Upper  
96 100  
61 182.3 145.7 218.5  
98 62.8 51.6 77.4

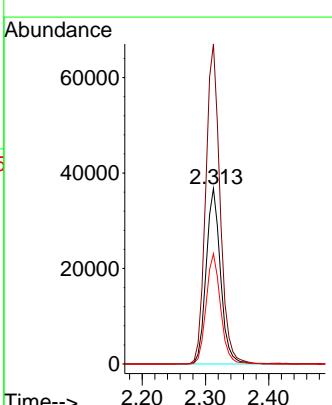



Abundance Scan 188 (2.233 min): VX045532.D\data.ms

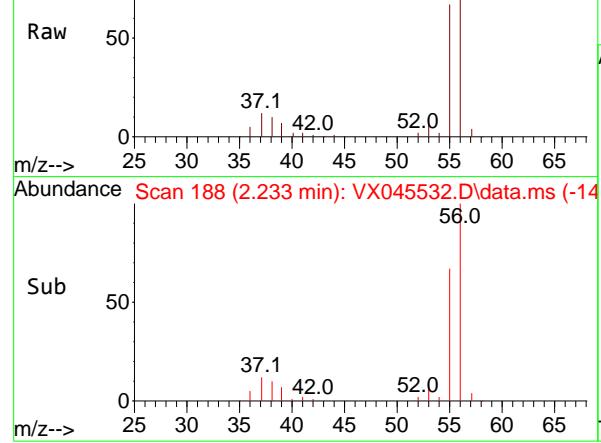

#13

Acrolein

Concen: 238.141 ug/l

RT: 2.233 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225


**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

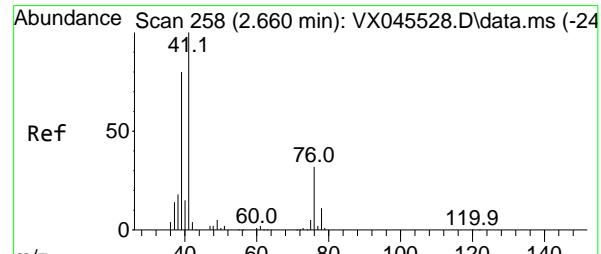

Abundance Scan 258 (2.660 min): VX045532.D\data.ms

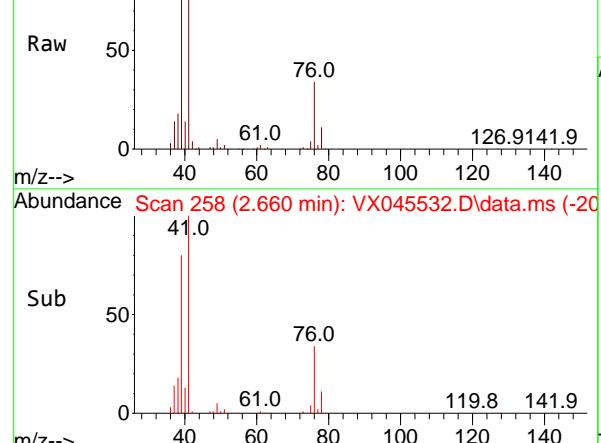

#14

Allyl chloride

Concen: 50.541 ug/l

RT: 2.660 min Scan# 258

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48


Tgt Ion: 41 Resp: 111636




Ion Ratio Lower Upper

41 100

39 76.2 60.2 90.2

76 31.6 24.6 36.8

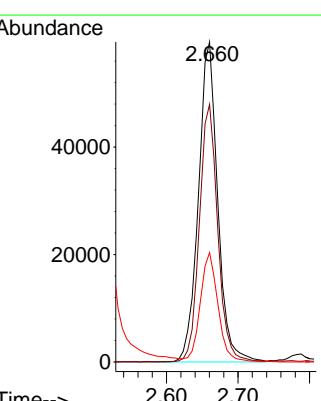

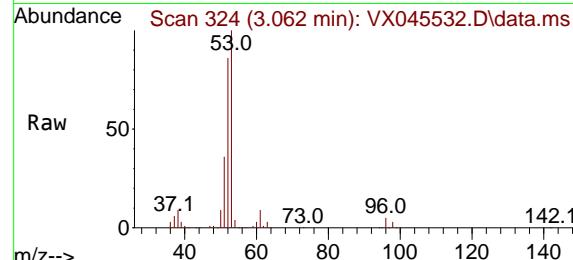

#15

Acrylonitrile

Concen: 248.351 ug/l

RT: 3.062 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument :

MSVOA\_X





ClientSampleId :

ICVVX040225

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

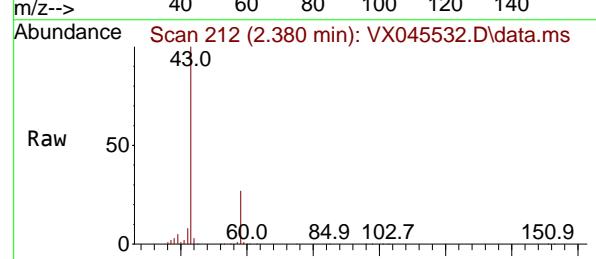

#16

Acetone

Concen: 241.904 ug/l


RT: 2.380 min Scan# 212


Delta R.T. -0.006 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48

Tgt Ion: 43 Resp: 176153  
 Ion Ratio Lower Upper  
 43 100  
 58 27.2 22.3 33.5

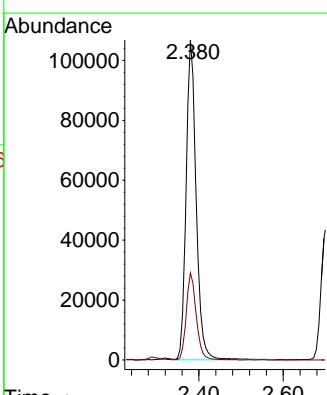



Abundance Scan 233 (2.508 min): VX045532.D\data.ms

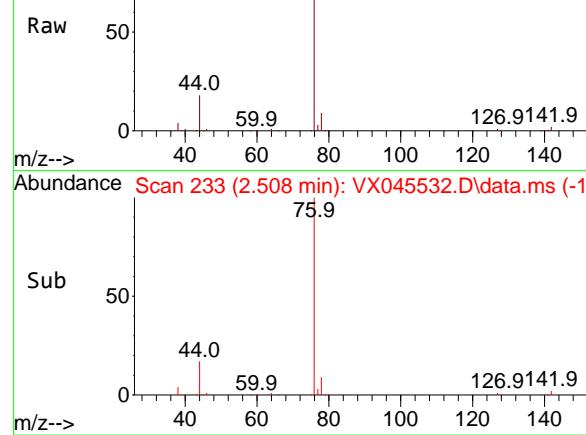

#17

Carbon Disulfide

Concen: 52.057 ug/l

RT: 2.508 min Scan# 2

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225


**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



Abundance Scan 265 (2.703 min): VX045532.D\data.ms

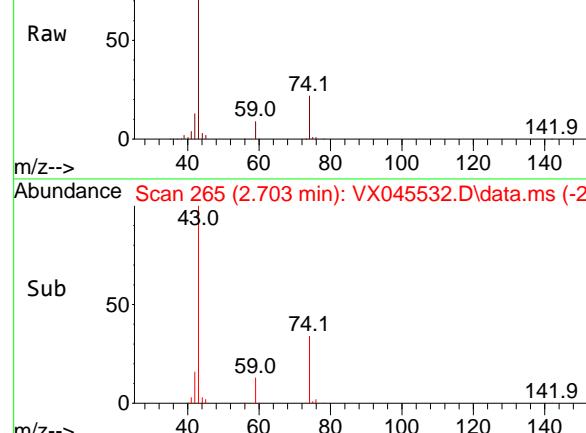

#18

Methyl Acetate

Concen: 48.742 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48







Tgt Ion: 43 Resp: 81720

Ion Ratio Lower Upper

43 100

74 21.8 17.5 26.3

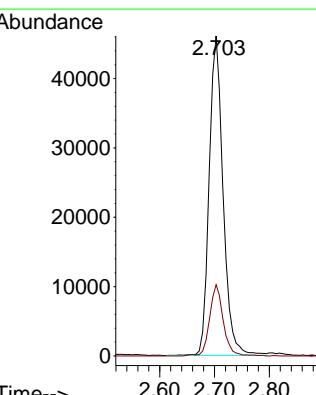



#19

Methyl tert-butyl Ether

Concen: 50.950 ug/l

RT: 3.111 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#20

Methylene Chloride

Concen: 49.055 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt Ion: 84 Resp: 66875


Ion Ratio Lower Upper







84 100

49 135.9 107.5 161.3

51 39.9 33.0 49.6

86 62.1 50.1 75.1

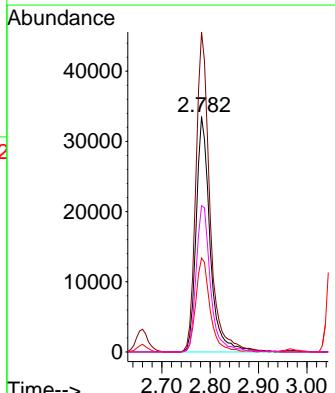

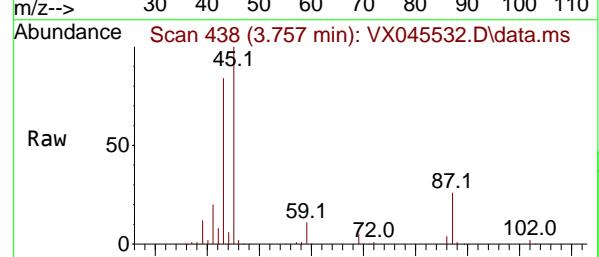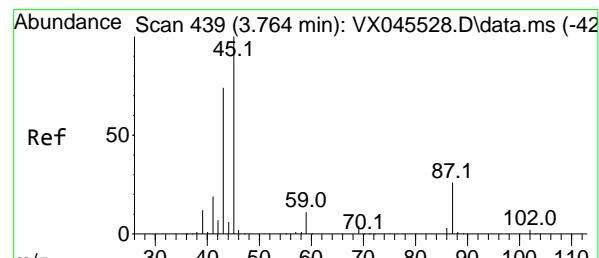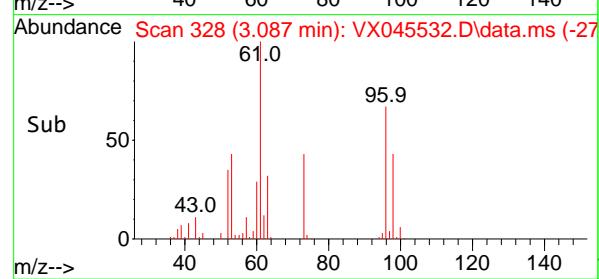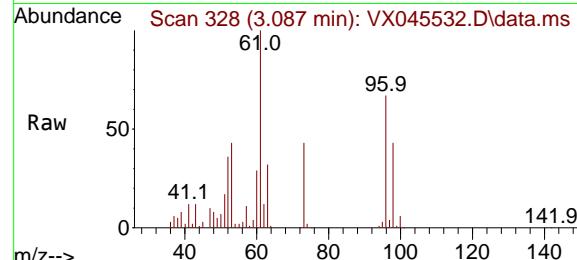

#21

trans-1,2-Dichloroethene

Concen: 49.800 ug/l

RT: 3.087 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument :

MSVOA\_X


ClientSampleId :

ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#22

Diisopropyl ether

Concen: 50.895 ug/l

RT: 3.757 min Scan# 438

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt Ion: 45 Resp: 221449


Ion Ratio Lower Upper


45 100

43 83.3 59.3 88.9

87 26.0 20.4 30.6

59 11.4 9.0 13.6

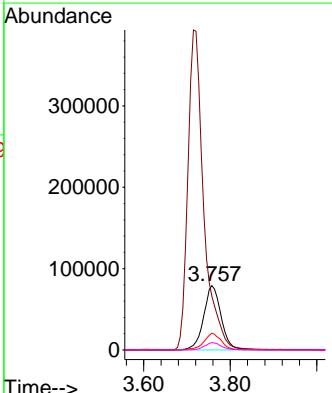



#23

## Vinyl Acetate

Concen: 267.449 ug/l

RT: 3.715 min Scan# 413

Delta R.T. -0.006 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X

ClientSampleId :

ICVVX040225

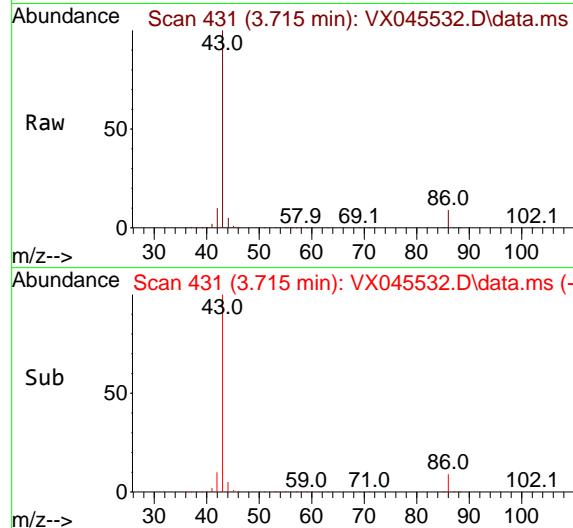

Tgt Ion: 43 Resp: 100542

Ion Ratio Lower Upper

43 100

86 9.1

Lower

7.5

Upper



11.3

## Manual Integrations

APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025
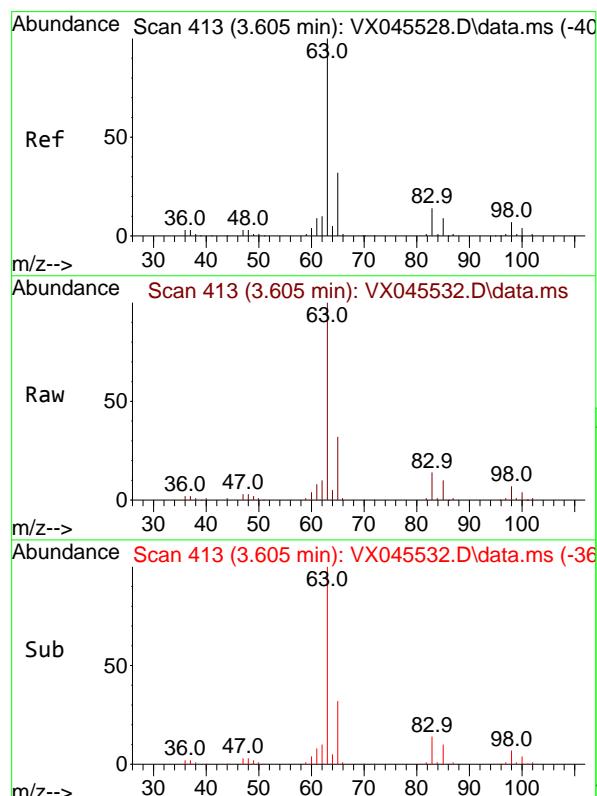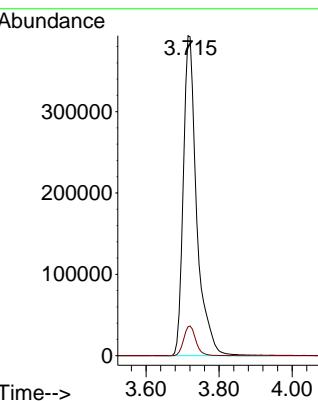
#24  
1,1-Dichloroethane  
Concen: 49.677 ug/l  
RT: 3.605 min Scan# 413  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion: 63 Resp: 122240

Ion Ratio Lower Upper

63 100

98 7.3

Lower

3.4



Upper




10.1

100 4.2

2.2

6.6

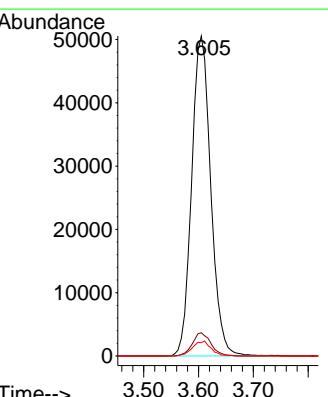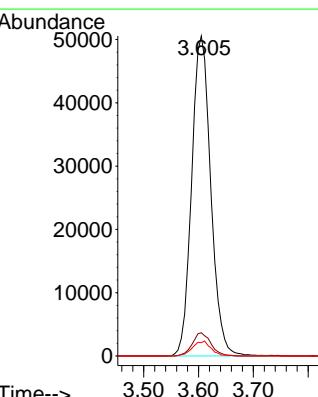

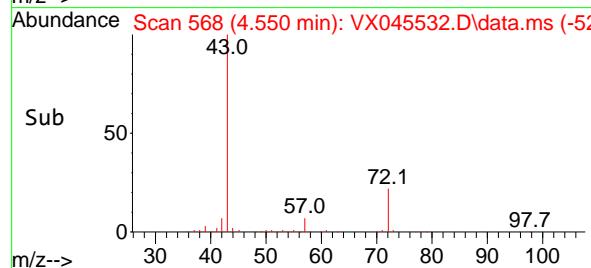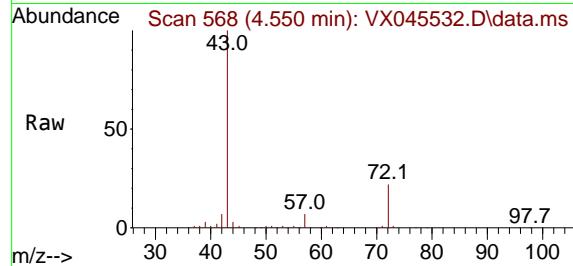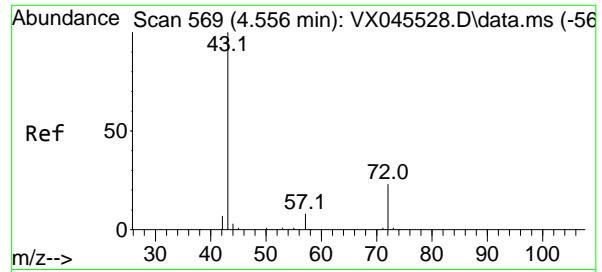

#25

2-Butanone

Concen: 254.882 ug/l

RT: 4.550 min Scan# 5

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

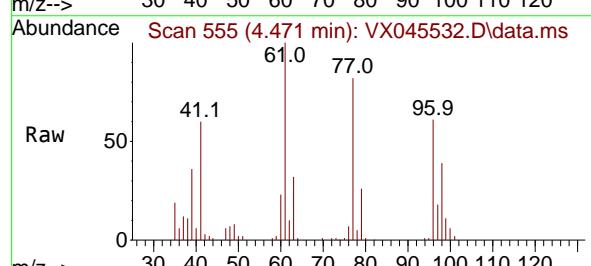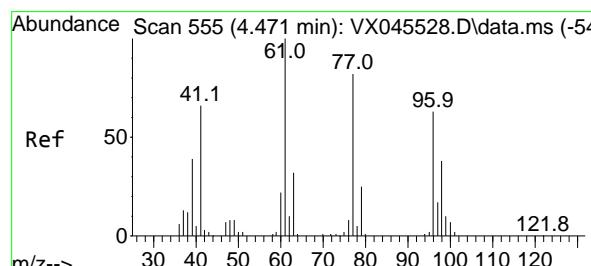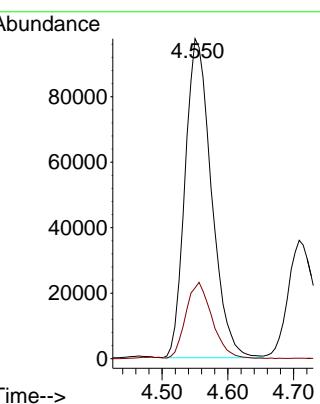

#26

2,2-Dichloropropane

Concen: 52.020 ug/l


RT: 4.471 min Scan# 555




Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt	Ion	Resp:	
Ion	Ratio	Lower	Upper
77	100		
97	21.2	10.6	31.8

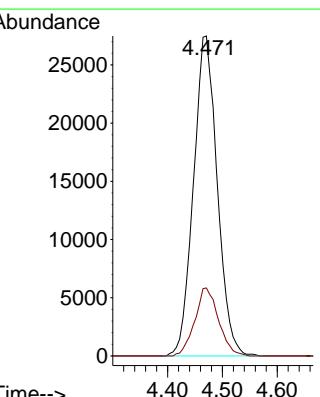






#27  
cis-1,2-Dichloroethene  
Concen: 49.049 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225



**Manual Integrations**  
**APPROVED**




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025



#28  
Bromochloromethane  
Concen: 48.403 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion: 49 Resp: 57557  
Ion Ratio Lower Upper  
49 100  
129 1.8 0.0 3.8  
130 69.3 54.6 81.8



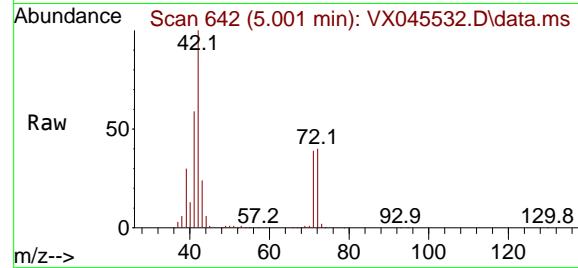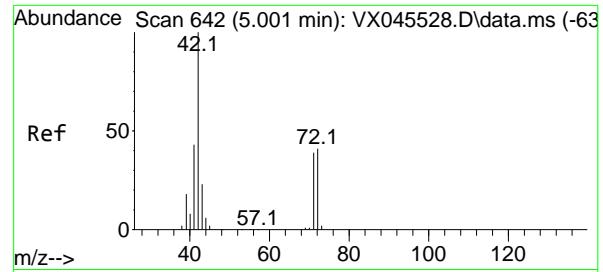

#29

Tetrahydrofuran

Concen: 249.473 ug/l

RT: 5.001 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument :

MSVOA\_X





ClientSampleId :

ICVVX040225

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

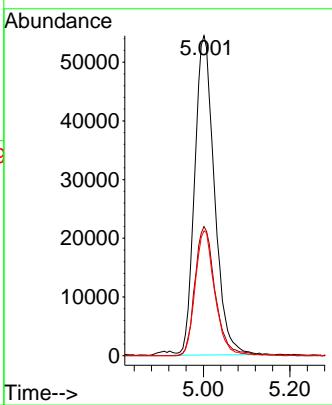

#30

Chloroform

Concen: 49.614 ug/l

RT: 5.086 min Scan# 656

Delta R.T. 0.000 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48


Tgt Ion: 83 Resp: 125621

Ion Ratio Lower Upper

83 100


85 64.2 52.8 79.2

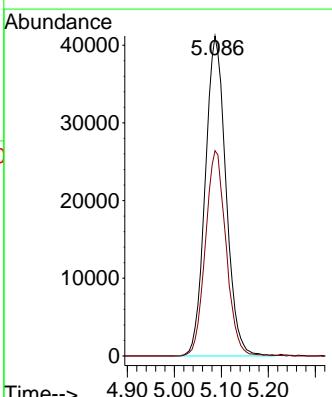




Ref 50  
0

Scan 717 (5.458 min): VX045532.D\data.ms

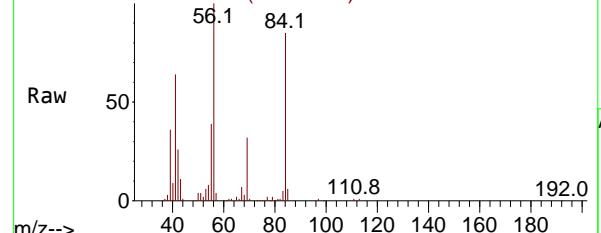


Raw 50  
0

Scan 717 (5.458 min): VX045532.D\data.ms (-66)

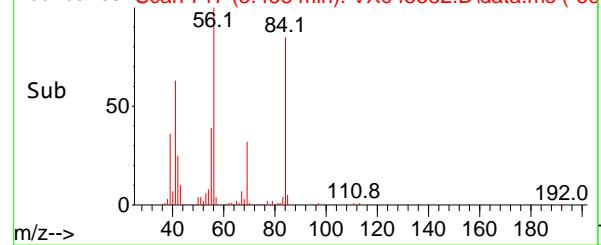


Sub 50  
0

Scan 704 (5.379 min): VX045528.D\data.ms (-69)

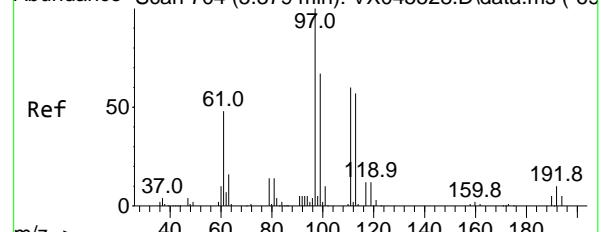


Ref 50  
0

Scan 704 (5.379 min): VX045532.D\data.ms

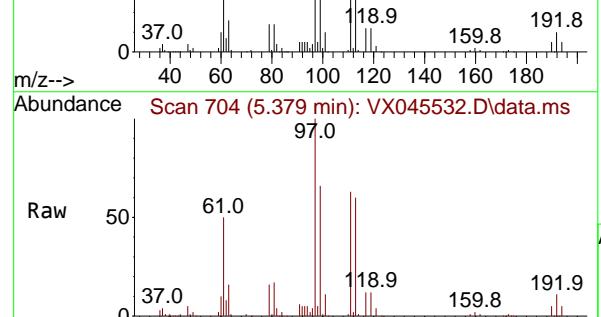

Raw 50  
0

Scan 704 (5.379 min): VX045532.D\data.ms (-65)

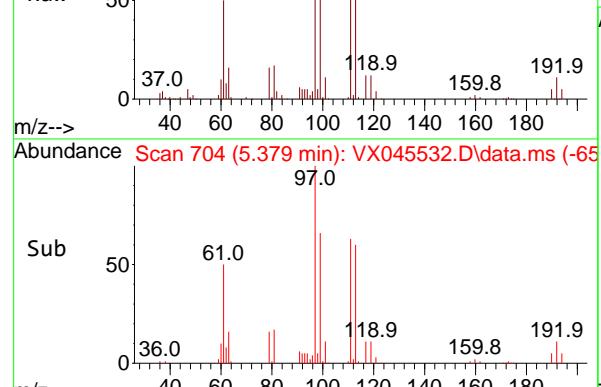

Sub 50  
0

#31

Cyclohexane

Concen: 49.583 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument :

MSVOA\_X


ClientSampleId :

ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#32

1,1,1-Trichloroethane

Concen: 50.330 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48


Tgt Ion: 97 Resp: 107830







Ion Ratio Lower Upper

97 100

99 64.9 51.7 77.5

61 50.5 41.0 61.4



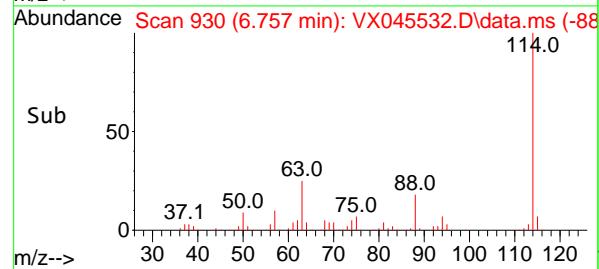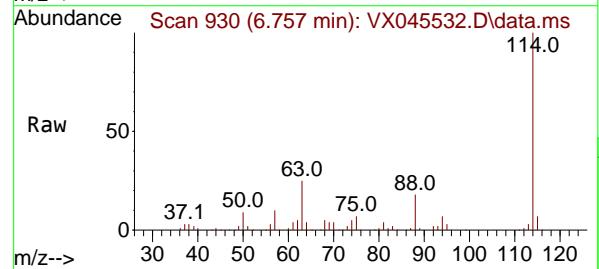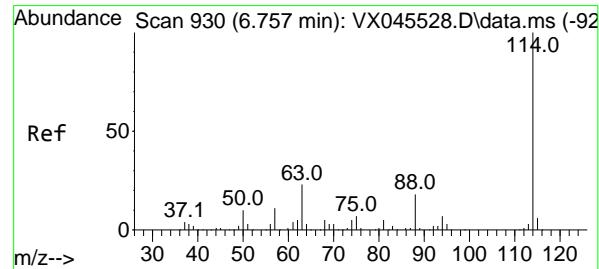


#33

1,2-Dichloroethane-d4  
Concen: 50.329 ug/l  
RT: 5.952 min Scan# 7  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

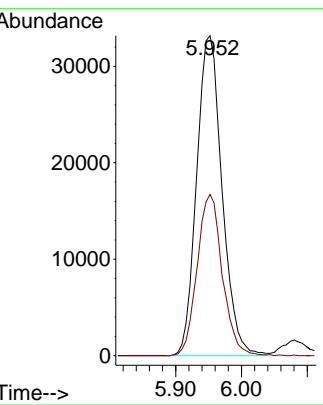





#34

1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 930  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion:114 Resp: 174855  
Ion Ratio Lower Upper

Ion	Ratio	Lower	Upper
114	100		
63	24.5	0.0	46.8
88	18.1	0.0	35.4

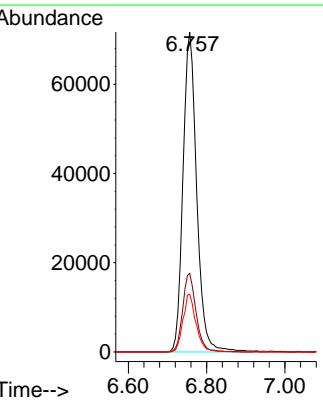

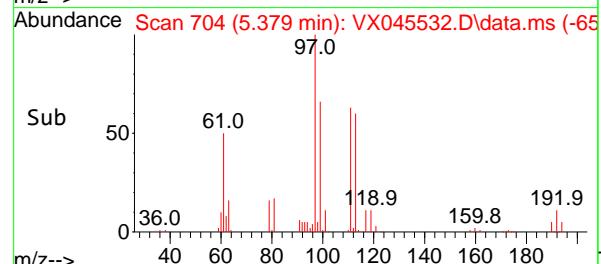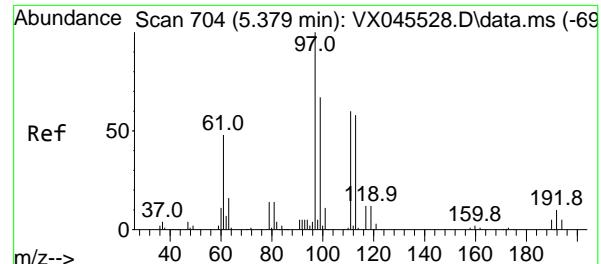

#35

Dibromofluoromethane

Concen: 49.256 ug/l

RT: 5.379 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

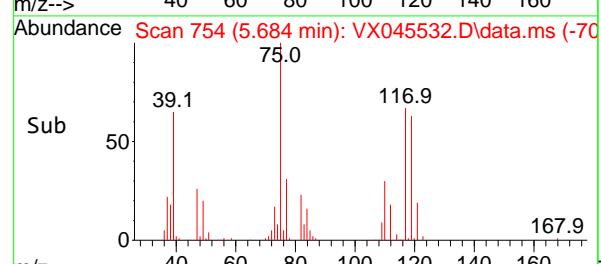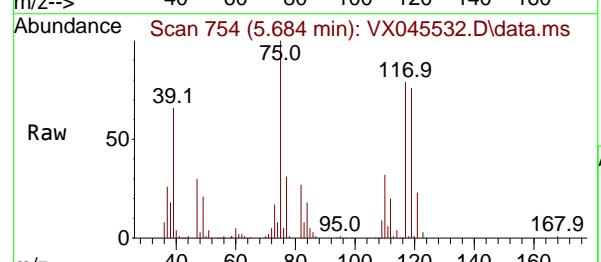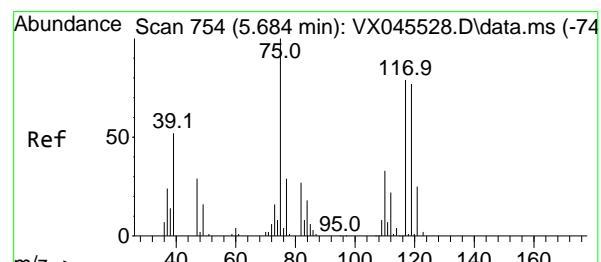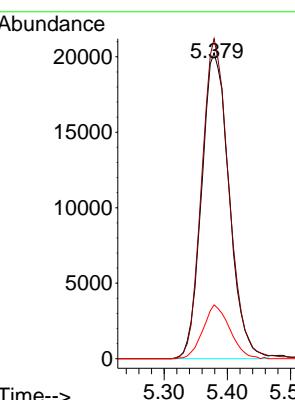

#36

1,1-Dichloropropene

Concen: 50.088 ug/l


RT: 5.684 min Scan# 754


Delta R.T. 0.000 min

Lab File: VX045532.D



Acq: 01 Apr 2025 19:48

Tgt	Ion: 75	Resp: 83901	
Ion	Ratio	Lower	Upper
75	100		
110	32.5	16.9	50.6
77	31.1	25.0	37.4

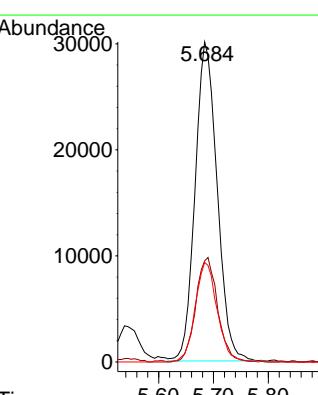


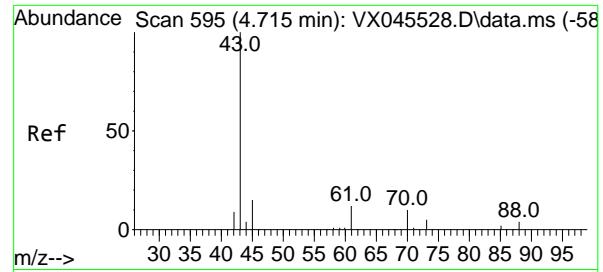

Abundance Scan 594 (4.708 min): VX045532.D\data.ms

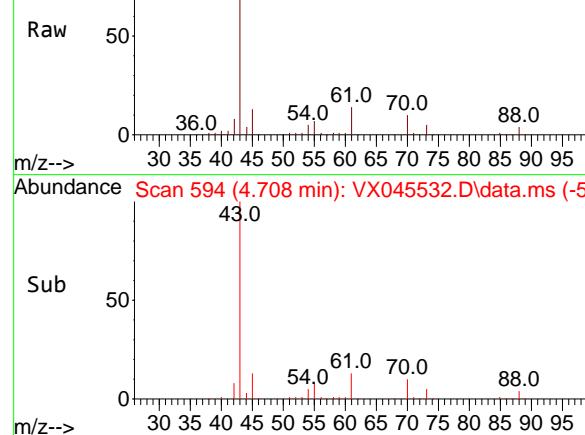

Abundance Scan 752 (5.672 min): VX045532.D\data.ms

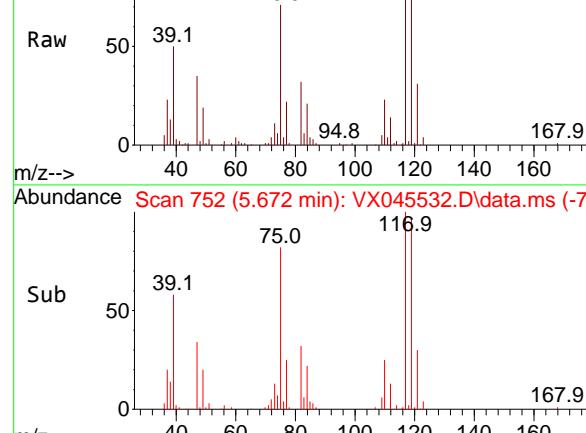

Abundance Scan 752 (5.672 min): VX045532.D\data.ms (-70)



#37

**Ethyl Acetate**

Concen: 49.787 ug/l

RT: 4.708 min Scan# 5

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X



ClientSampleId :

ICVVX040225


**Manual Integrations****APPROVED**




Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

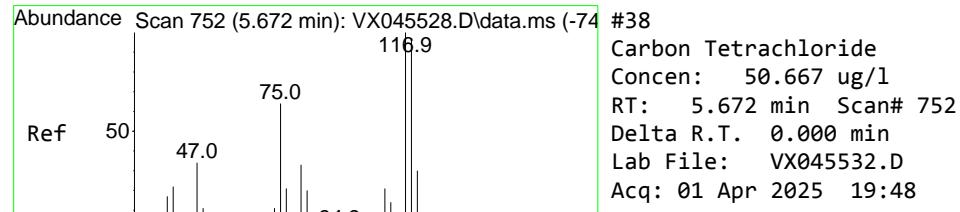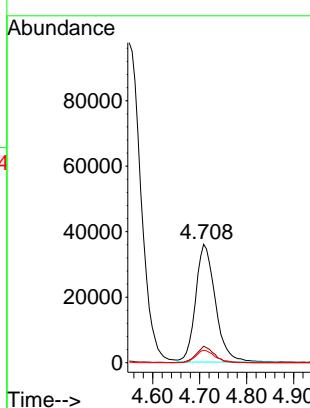

Tgt	Ion:117	Resp:	91723
Ion	Ratio	Lower	Upper
117	100		
119	95.9	76.9	115.3
121	30.6	24.2	36.2

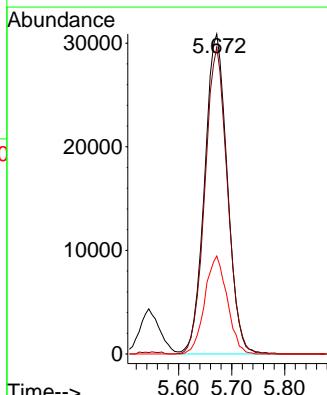

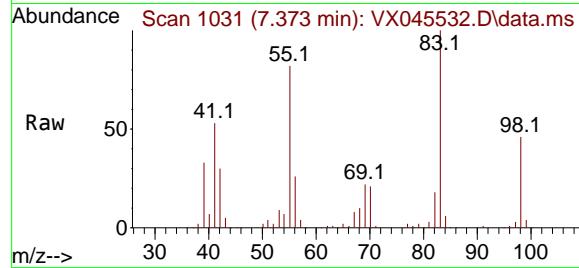

#39

Methylcyclohexane

Concen: 50.124 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48




Instrument : MSVOA\_X

ClientSampleId : ICVVX040225

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#40

Benzene

Concen: 49.212 ug/l

RT: 6.031 min Scan# 811



Delta R.T. 0.000 min







Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt Ion: 78 Resp: 251758

Ion	Ratio	Lower	Upper
78	100		
77	24.0	19.0	28.6

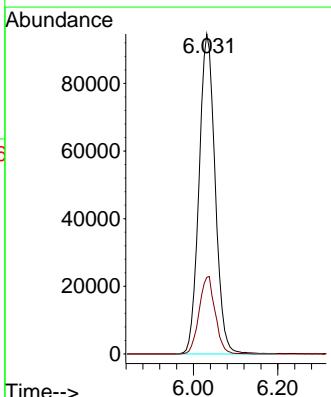

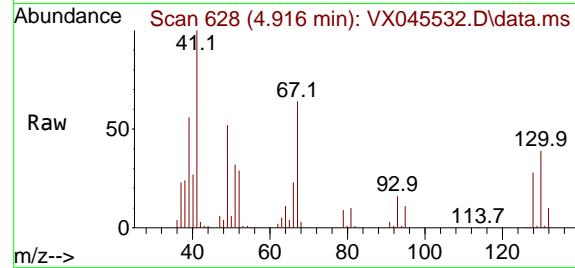

#41

Methacrylonitrile

Concen: 53.098 ug/l

RT: 4.916 min Scan# 6

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X

ClientSampleId :


ICVVX040225




**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

Abundance

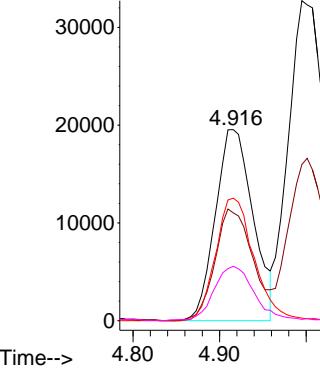

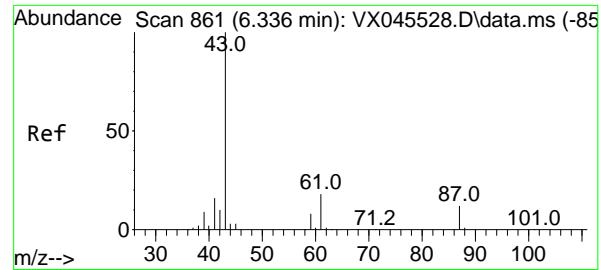

#43

Isopropyl Acetate

Concen: 51.539 ug/l

RT: 6.336 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument :

MSVOA\_X





ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

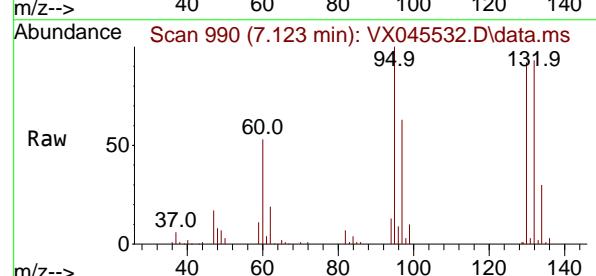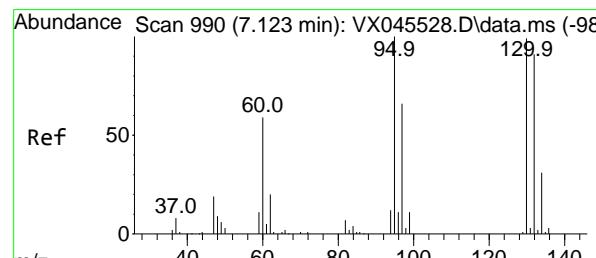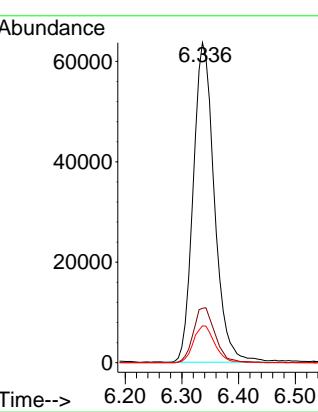

#44

Trichloroethene

Concen: 47.643 ug/l


RT: 7.123 min Scan# 990




Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt Ion:130 Resp: 57931  
 Ion Ratio Lower Upper  
 130 100  
 95 108.6 0.0 202.0

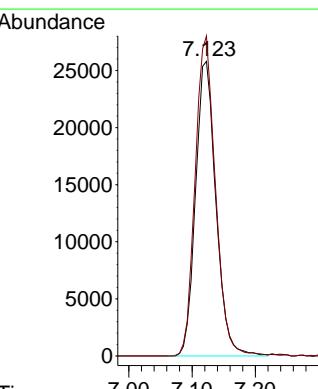



#45

1,2-Dichloropropane

Concen: 49.521 ug/l

RT: 7.421 min Scan# 1040

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48





Instrument: MSVOA\_X

ClientSampleId: ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

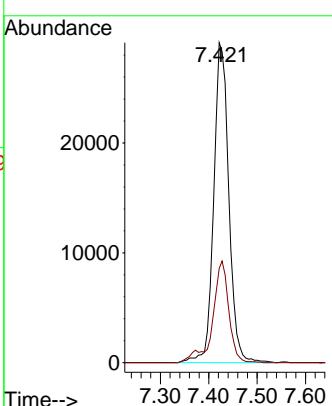

#46

Dibromomethane

Concen: 48.542 ug/l

RT: 7.574 min Scan# 1064

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48


Tgt Ion: 93 Resp: 47564


Ion Ratio Lower Upper

93 100

95 83.6 64.8 97.2

174 84.5 65.4 98.0

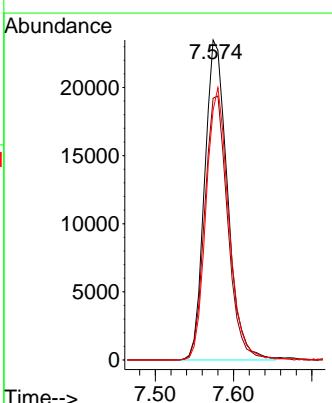

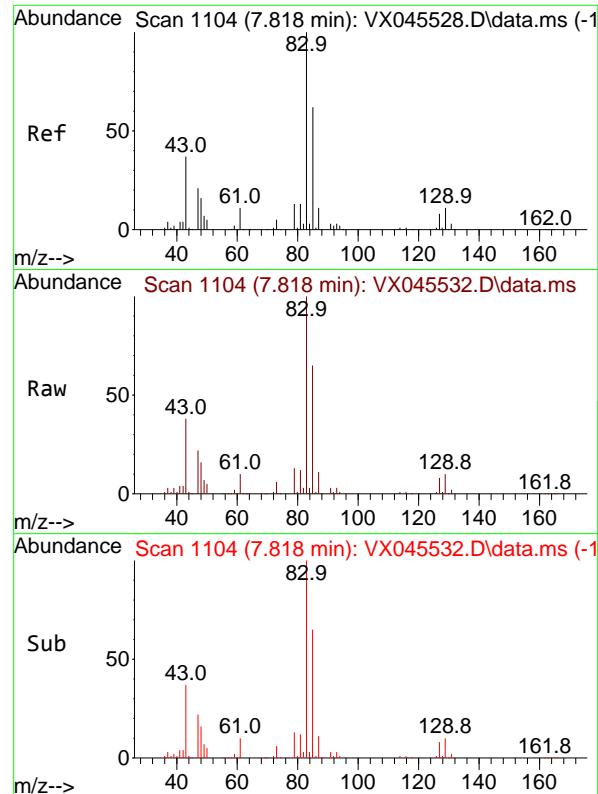

#47

Bromodichloromethane

Concen: 49.273 ug/l

RT: 7.818 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

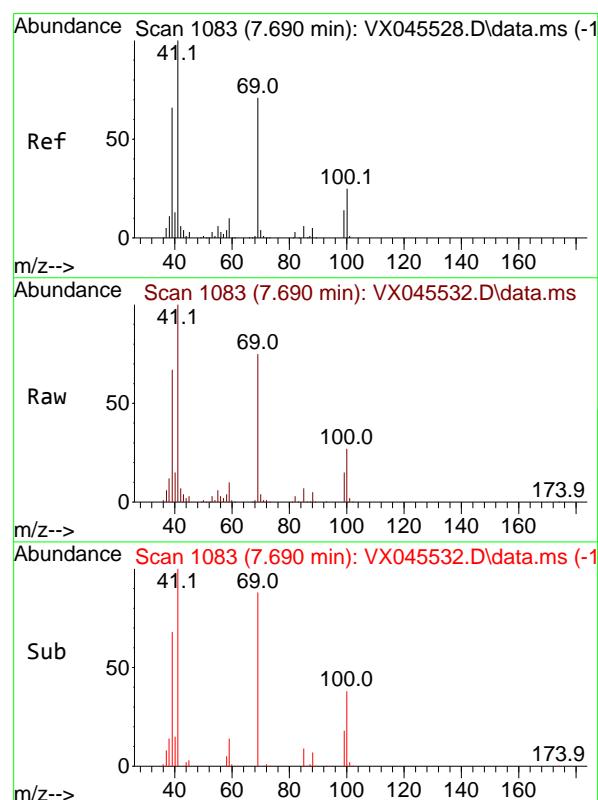

#48

Methyl methacrylate

Concen: 51.507 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48


Tgt Ion: 41 Resp: 85084







Ion Ratio Lower Upper

41 100

69 74.5 58.2 87.2

39 67.3 53.6 80.4

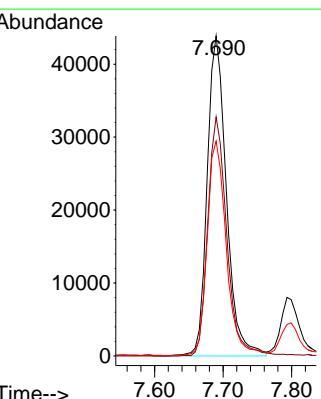

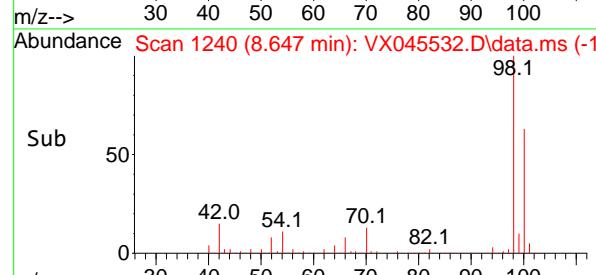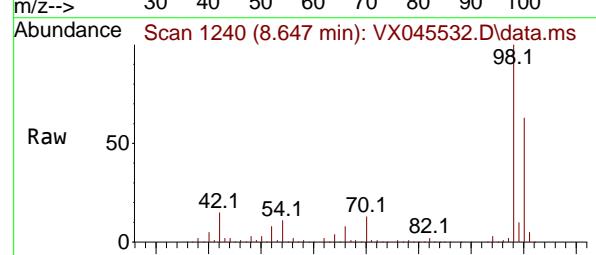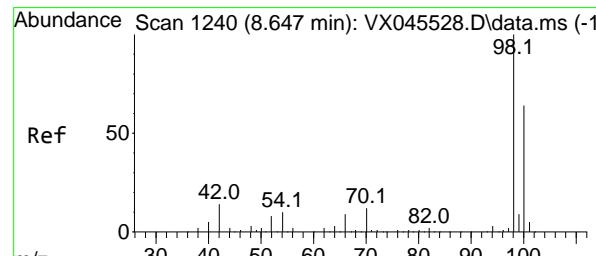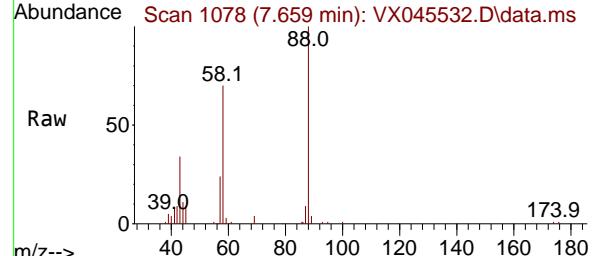

#49

1,4-Dioxane

Concen: 955.327 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument :

MSVOA\_X


ClientSampleId :

ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#50

Toluene-d8

Concen: 50.160 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48


Tgt Ion: 98 Resp: 217200

Ion Ratio Lower Upper


98 100

100 64.9 52.2 78.4


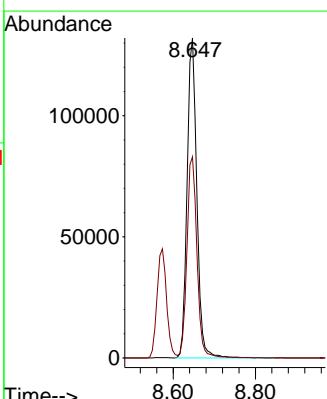





Abundance Scan 1227 (8.568 min): VX045532.D\data.ms

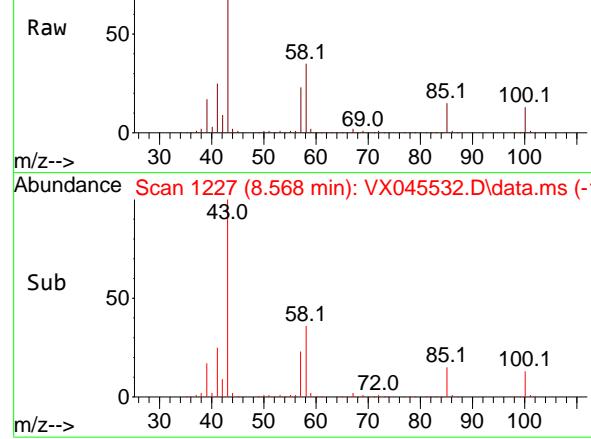


Abundance Scan 1227 (8.568 min): VX045532.D\data.ms (-1)

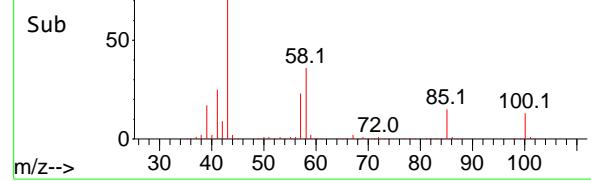

Abundance Scan 1251 (8.714 min): VX045532.D\data.ms

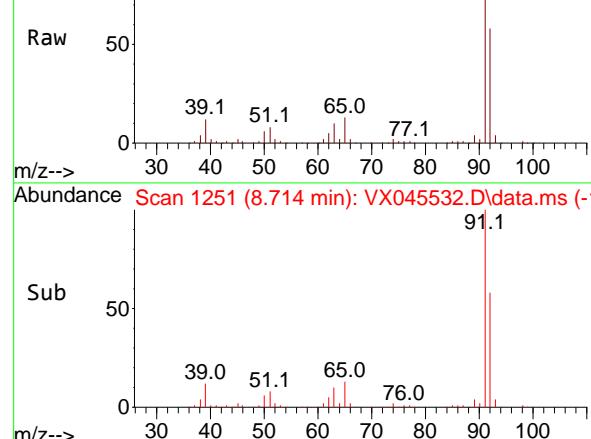

Abundance Scan 1251 (8.714 min): VX045532.D\data.ms (-1)

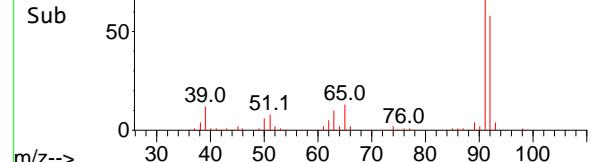

#51

4-Methyl-2-Pentanone

Concen: 254.994 ug/l

RT: 8.568 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument :

MSVOA\_X


ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

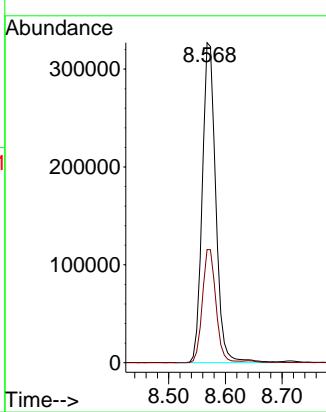

#52

Toluene

Concen: 48.994 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48




Tgt Ion: 92 Resp: 151664

Ion Ratio Lower Upper

92 100

91 174.0 138.7 208.1

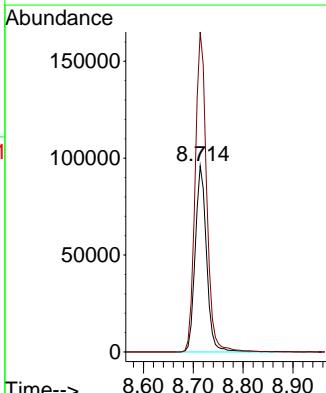

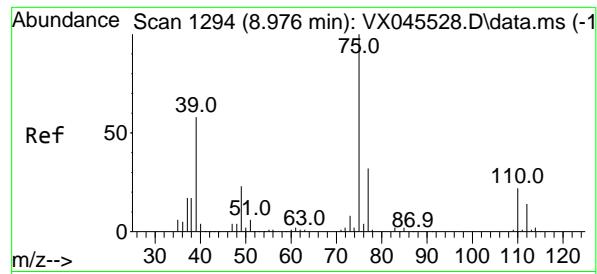

#53

t-1,3-Dichloropropene

Concen: 46.783 ug/l

RT: 8.976 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

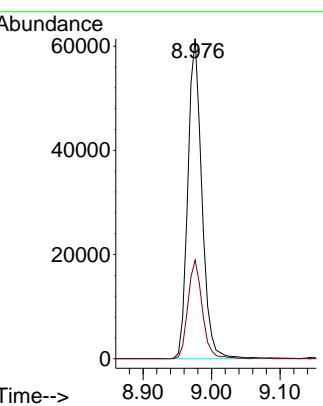

#54

cis-1,3-Dichloropropene

Concen: 53.878 ug/l

RT: 8.360 min Scan# 1193

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48


Tgt Ion: 75 Resp: 99074







Ion Ratio Lower Upper

75 100

77 31.3 24.6 36.8

39 62.0 48.4 72.6

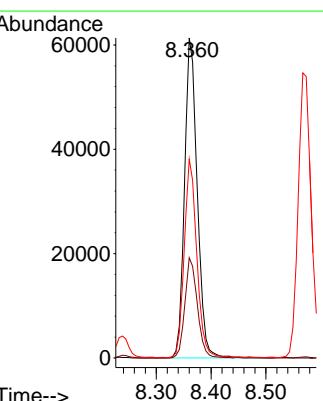

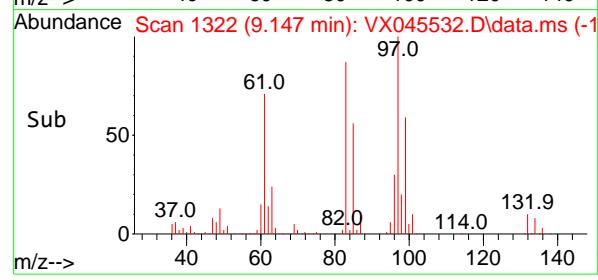


#55

1,1,2-Trichloroethane  
Concen: 49.007 ug/l  
RT: 9.147 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225


### Manual Integrations APPROVED


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

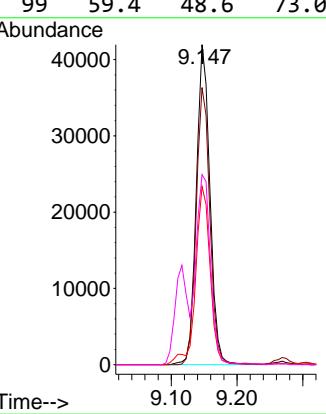

#56  
Ethyl methacrylate  
Concen: 53.705 ug/l  
RT: 9.116 min Scan# 1317  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion: 69 Resp: 102525  
Ion Ratio Lower Upper  
69 100  
41 76.7 61.3 91.9  
39 50.7 40.2 60.2

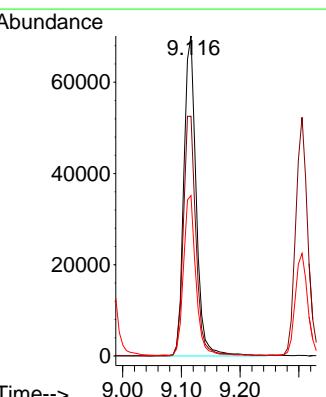

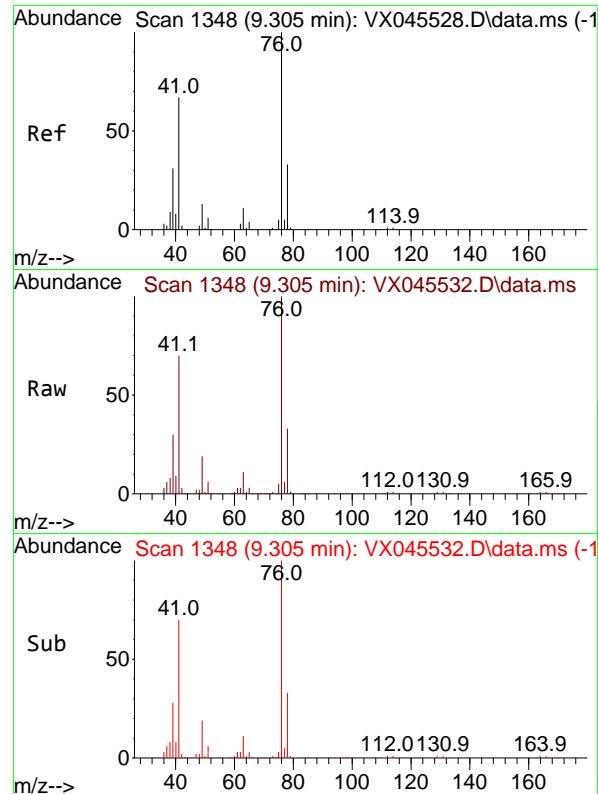

#57

1,3-Dichloropropane

Concen: 49.869 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

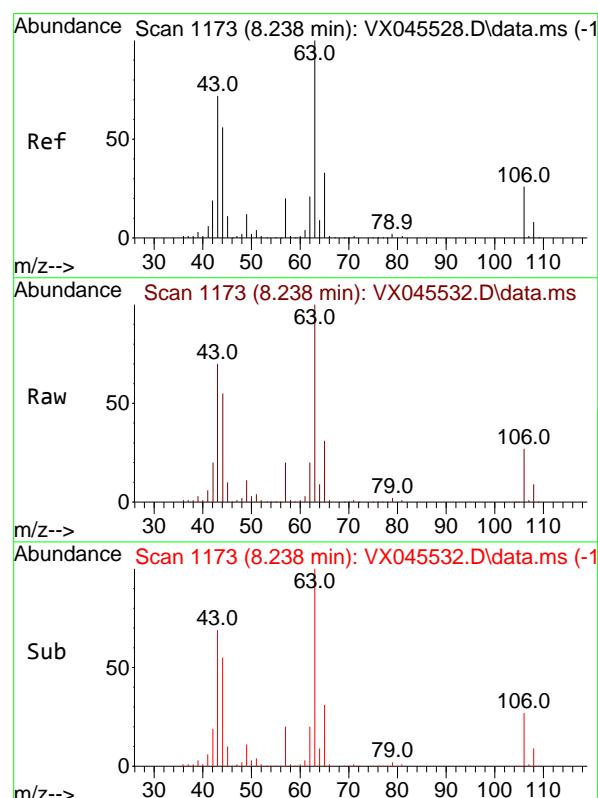

#58

2-Chloroethyl Vinyl ether

Concen: 260.201 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. 0.000 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48


Tgt Ion: 63 Resp: 251285

Ion Ratio Lower Upper


63 100

106 26.6 21.0 31.6


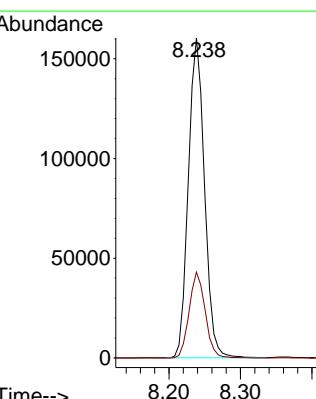





Abundance Scan 1368 (9.427 min): VX045532.D\data.ms

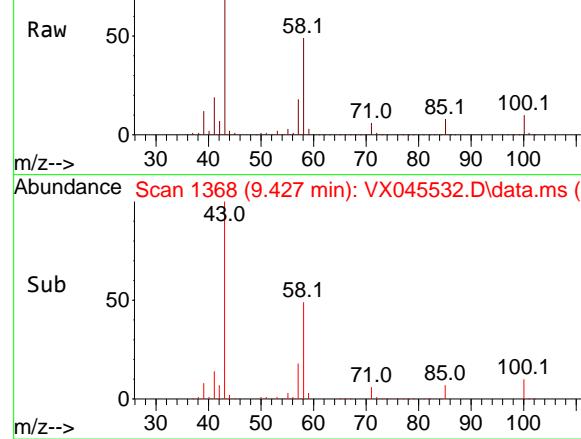


Abundance Scan 1368 (9.427 min): VX045532.D\data.ms (-1)

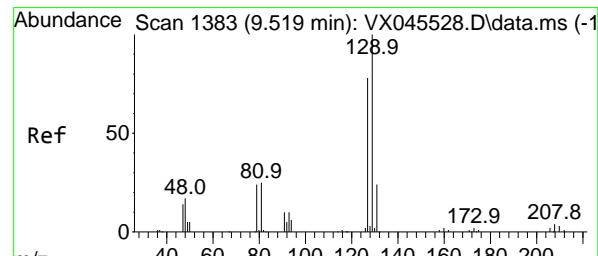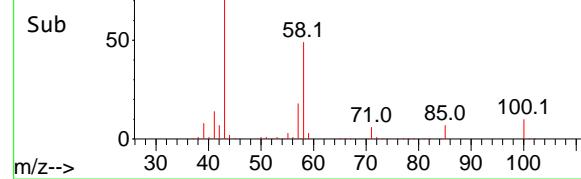

Abundance Scan 1383 (9.519 min): VX045532.D\data.ms

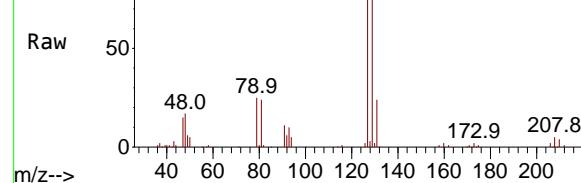

Abundance Scan 1383 (9.519 min): VX045532.D\data.ms (-1)

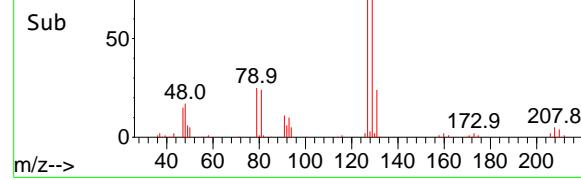

#59

2-Hexanone

Concen: 251.710 ug/l

RT: 9.427 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument :

MSVOA\_X


ClientSampleId :

ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

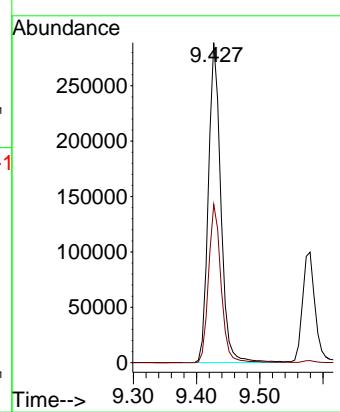

#60

Dibromochloromethane

Concen: 50.983 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48




Tgt Ion:129 Resp: 68562

Ion Ratio Lower Upper

129 100

127 78.2 39.4 118.2

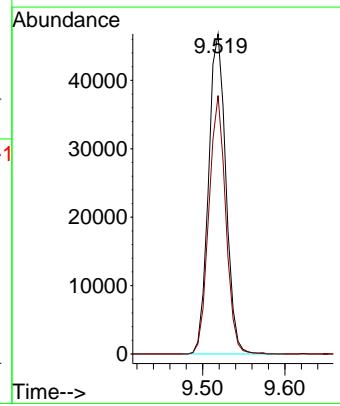

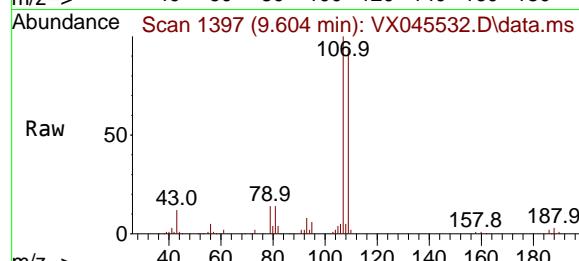

#61

1,2-Dibromoethane

Concen: 50.693 ug/l

RT: 9.604 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

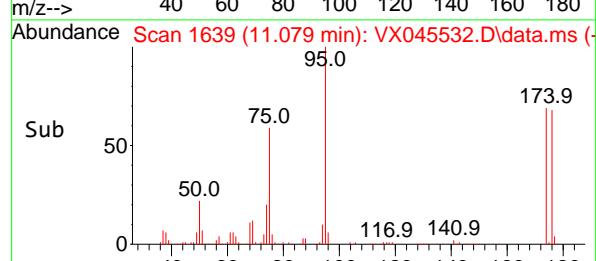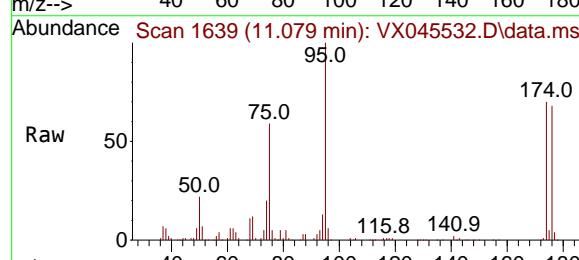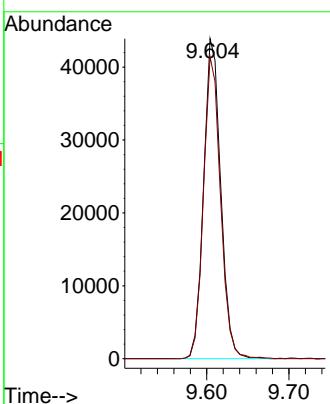

#62

4-Bromofluorobenzene

Concen: 50.959 ug/l


RT: 11.079 min Scan# 1639


Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt	Ion:	95	Resp:	80376
Ion	Ratio	Lower	Upper	
95	100			
174	66.4	0.0	135.8	
176	65.2	0.0	131.4	

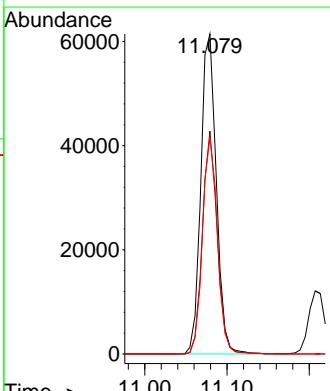

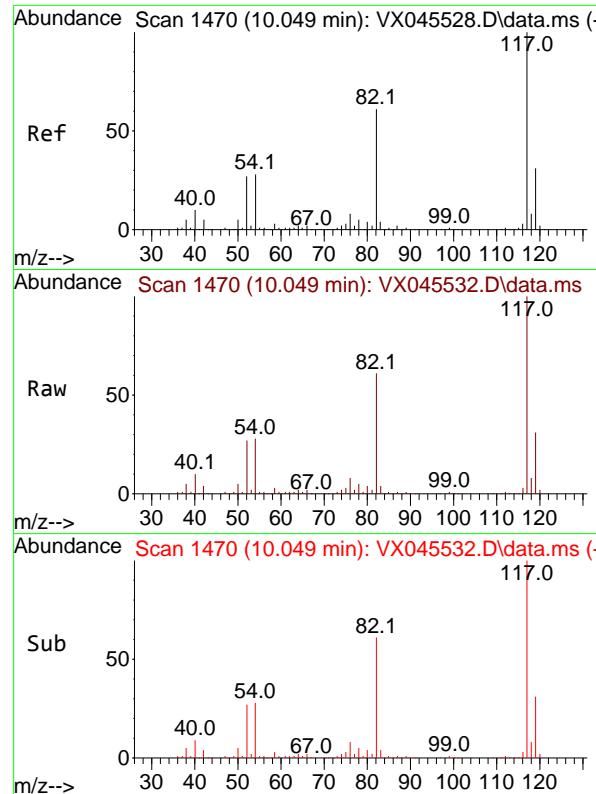

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

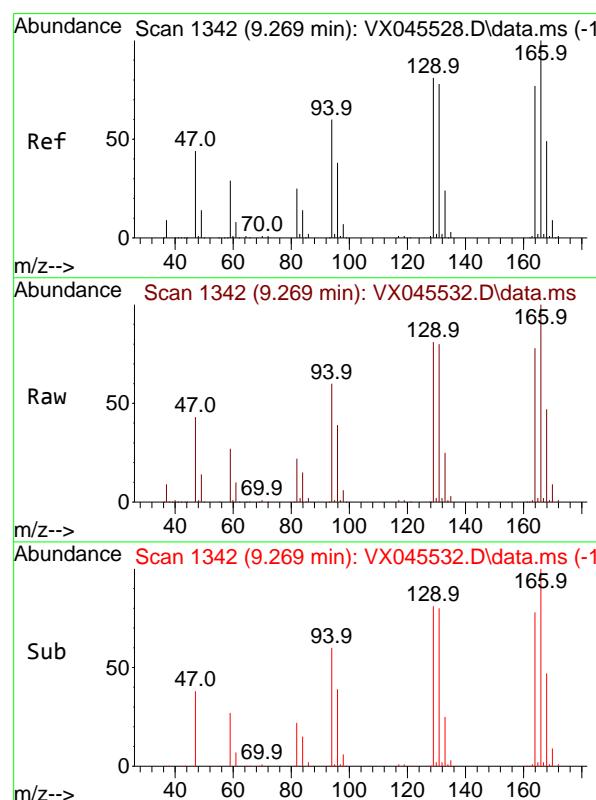

#64

Tetrachloroethene

Concen: 47.239 ug/l


RT: 9.269 min Scan# 1342


Delta R.T. -0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt	Ion:164	Resp:	50834
Ion	Ratio	Lower	Upper
164	100		
166	128.0	103.8	155.8
129	104.3	84.3	126.5
131	102.6	80.9	121.3

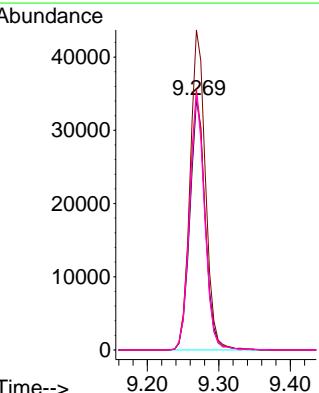


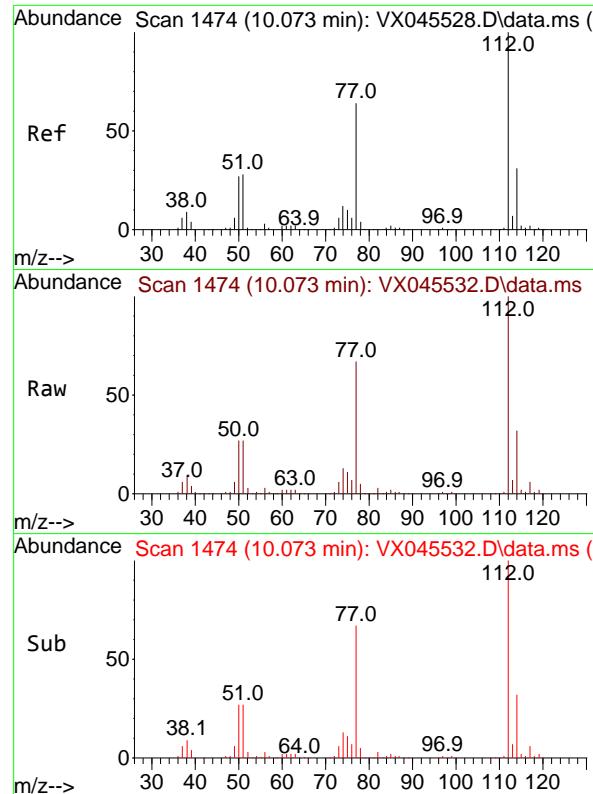


#65  
Chlorobenzene  
Concen: 50.207 ug/l  
RT: 10.073 min Scan# 1474  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225


**Manual Integrations**  
**APPROVED**







Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

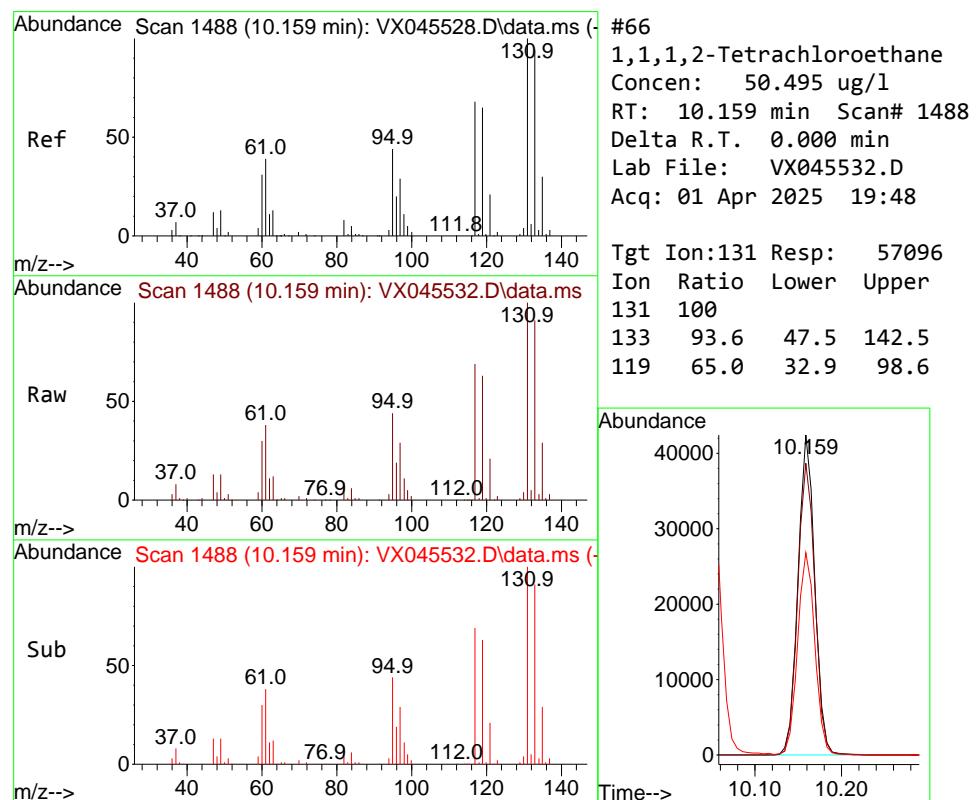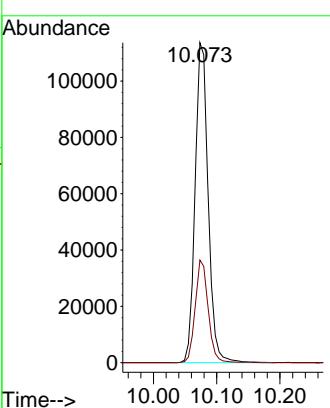

#66  
1,1,1,2-Tetrachloroethane  
Concen: 50.495 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion:131 Resp: 57096  
Ion Ratio Lower Upper  
131 100  
133 93.6 47.5 142.5  
119 65.0 32.9 98.6

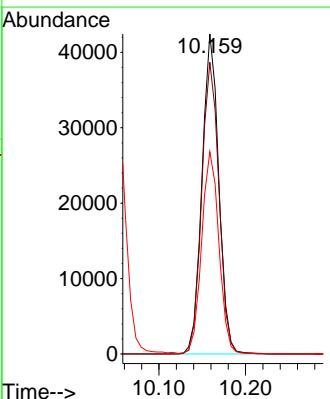



#67

Ethyl Benzene

Concen: 51.558 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

### Manual Integrations APPROVED

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

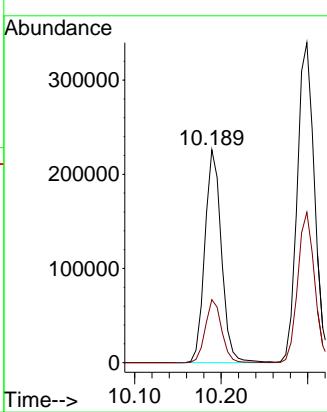

#68

m/p-Xylenes

Concen: 102.728 ug/l


RT: 10.299 min Scan# 1511




Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt Ion:106 Resp: 217943  
Ion Ratio Lower Upper  
106 100  
91 217.6 172.6 258.8









#69  
o-Xylene  
Concen: 51.650 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48  
ClientSampleId : ICVVX040225

Tgt Ion:106 Resp: 107941  
Ion Ratio Lower Upper  
106 100  
91 226.8 113.6 340.6


### Manual Integrations APPROVED







Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025



#70  
Styrene  
Concen: 52.624 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion:104 Resp: 181524  
Ion Ratio Lower Upper  
104 100  
78 57.0 45.4 68.2  
103 55.2 43.8 65.8





#71

Bromoform

Concen: 52.694 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l


RT: 12.018 min Scan# 1793


Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt	Ion:152	Resp:	67633
Ion	Ratio	Lower	Upper
152	100		
115	94.2	46.9	140.7
150	175.4	0.0	349.4

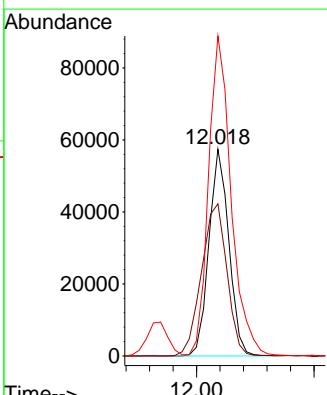

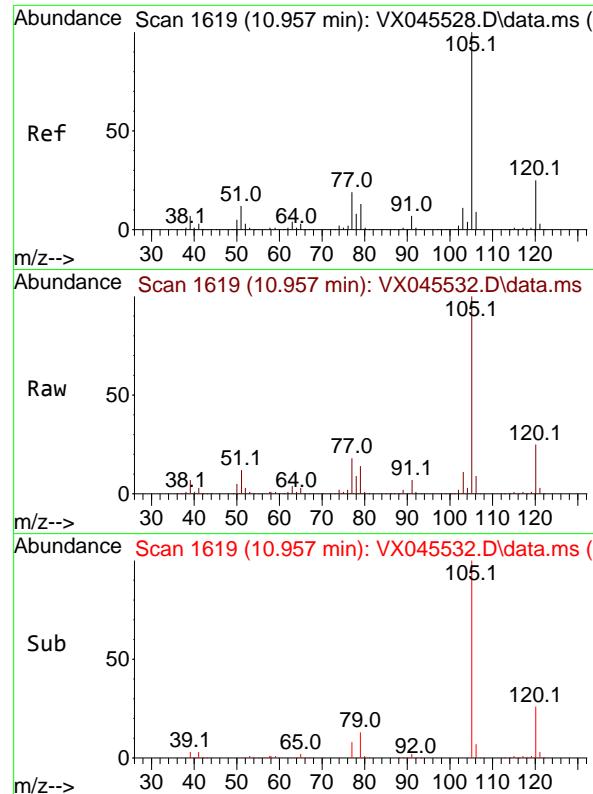

#73

Isopropylbenzene

Concen: 52.794 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

**Manual Integrations**  
**APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

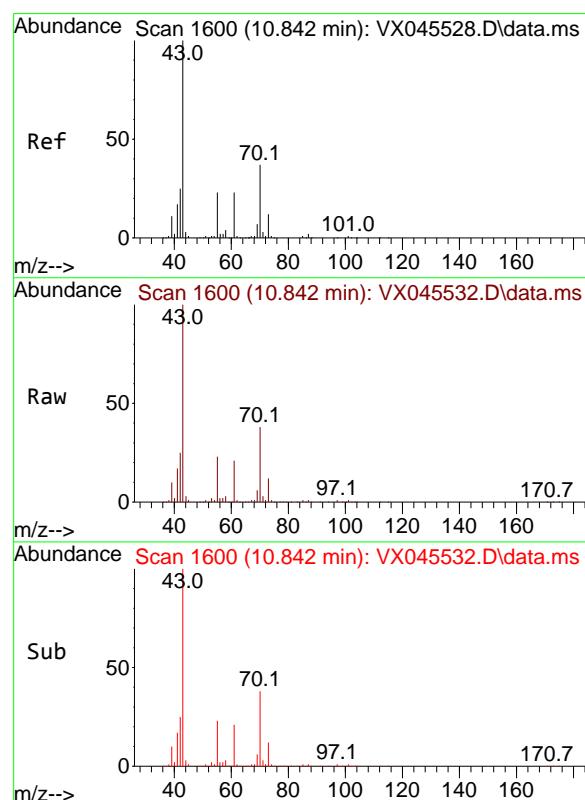

#74

N-amyl acetate

Concen: 54.387 ug/l


RT: 10.842 min Scan# 1600


Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt	Ion:	43	Resp:	140941
Ion	Ratio	Lower	Upper	
43	100			
70	38.2	30.1	45.1	
55	23.3	18.3	27.5	
61	21.7	17.5	26.3	

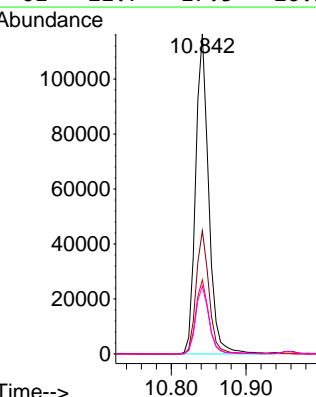


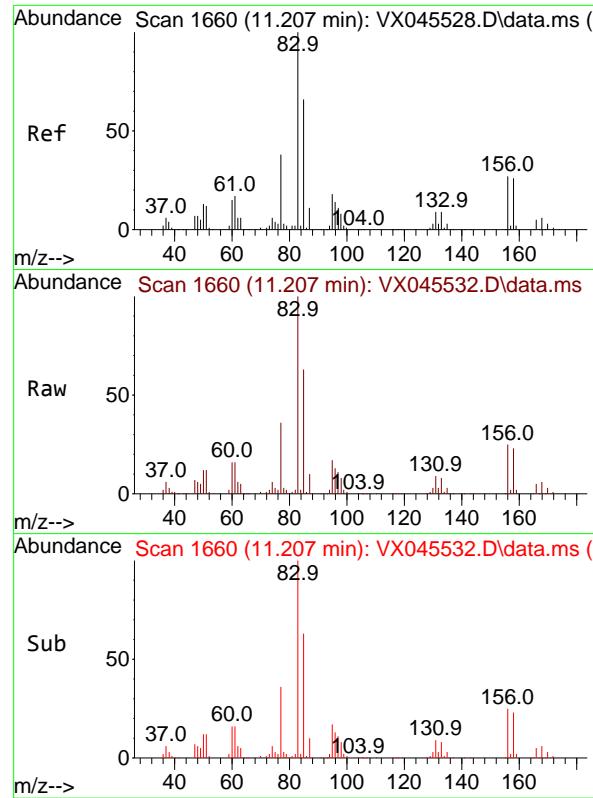


#75  
1,1,2,2-Tetrachloroethane  
Concen: 48.608 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

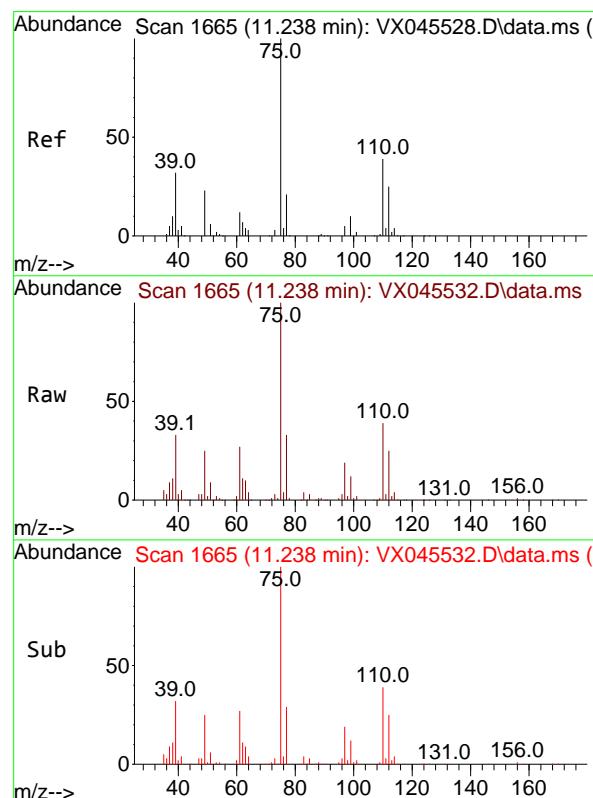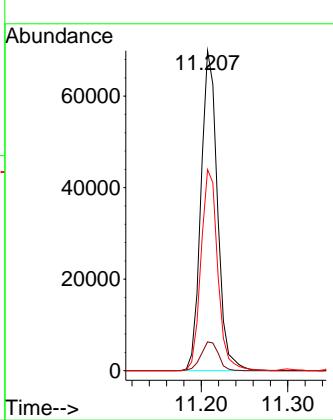

#76  
1,2,3-Trichloropropane  
Concen: 49.741 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion: 75 Resp: 82060  
Ion Ratio Lower Upper  
75 100  
77 40.0 20.0 59.9



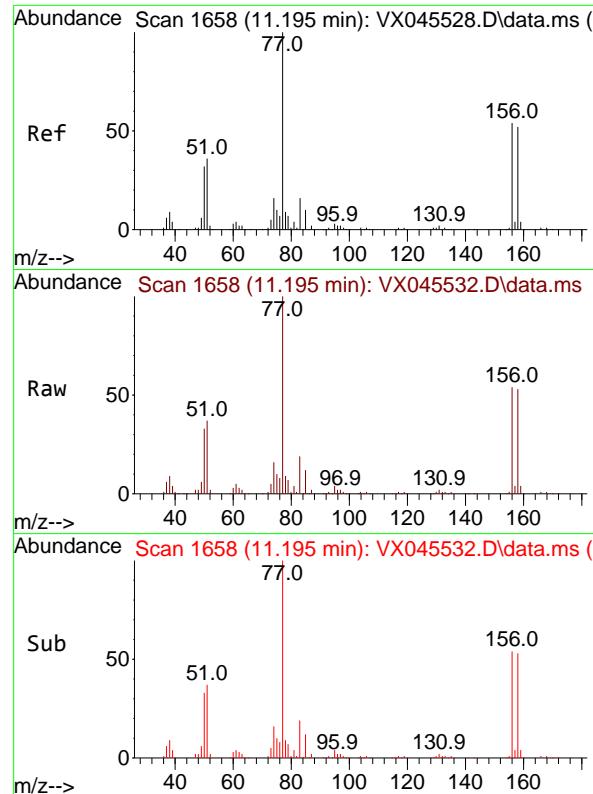

#77

Bromobenzene

Concen: 50.525 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X



ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

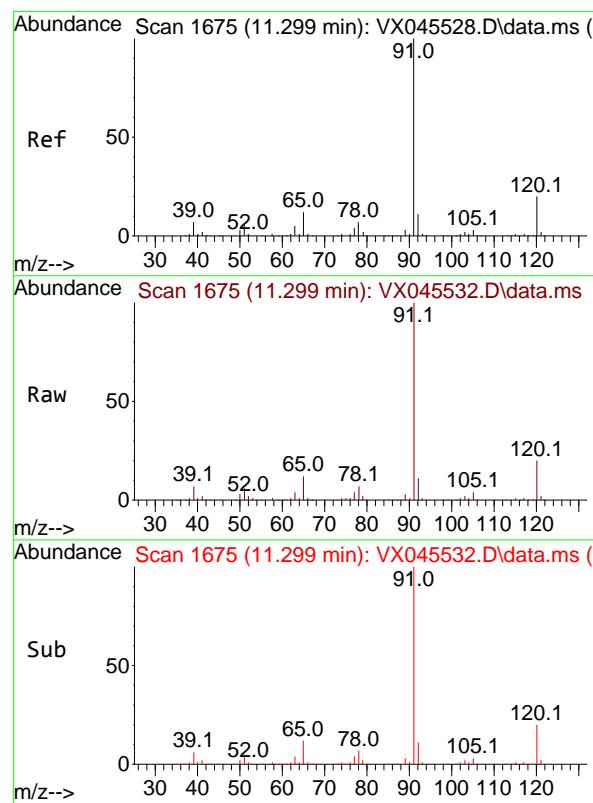

#78

n-propylbenzene

Concen: 53.967 ug/l

RT: 11.299 min Scan# 1675


Delta R.T. 0.000 min

Lab File: VX045532.D


Acq: 01 Apr 2025 19:48

Tgt Ion: 91 Resp: 336753

Ion	Ratio	Lower	Upper
91	100		
120	21.4	10.8	32.3






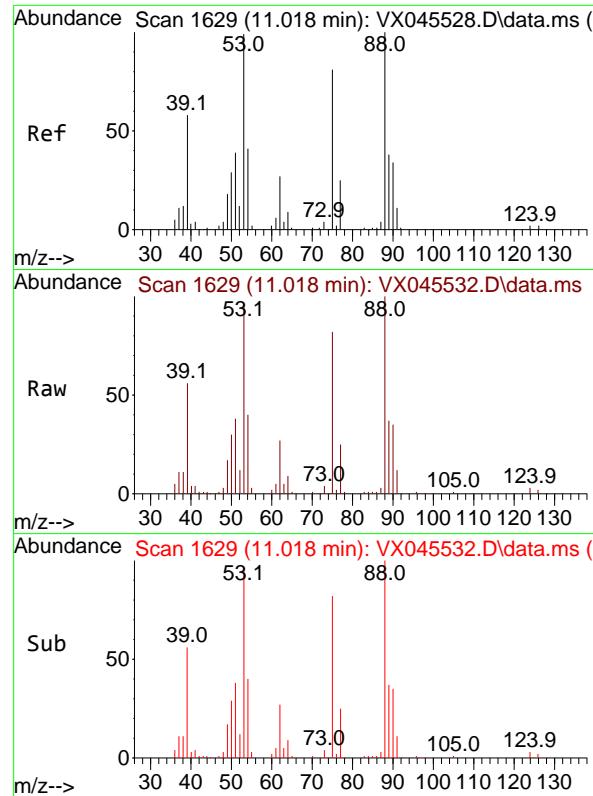


#81  
trans-1,4-Dichloro-2-butene  
Concen: 52.482 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225


### Manual Integrations APPROVED




Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

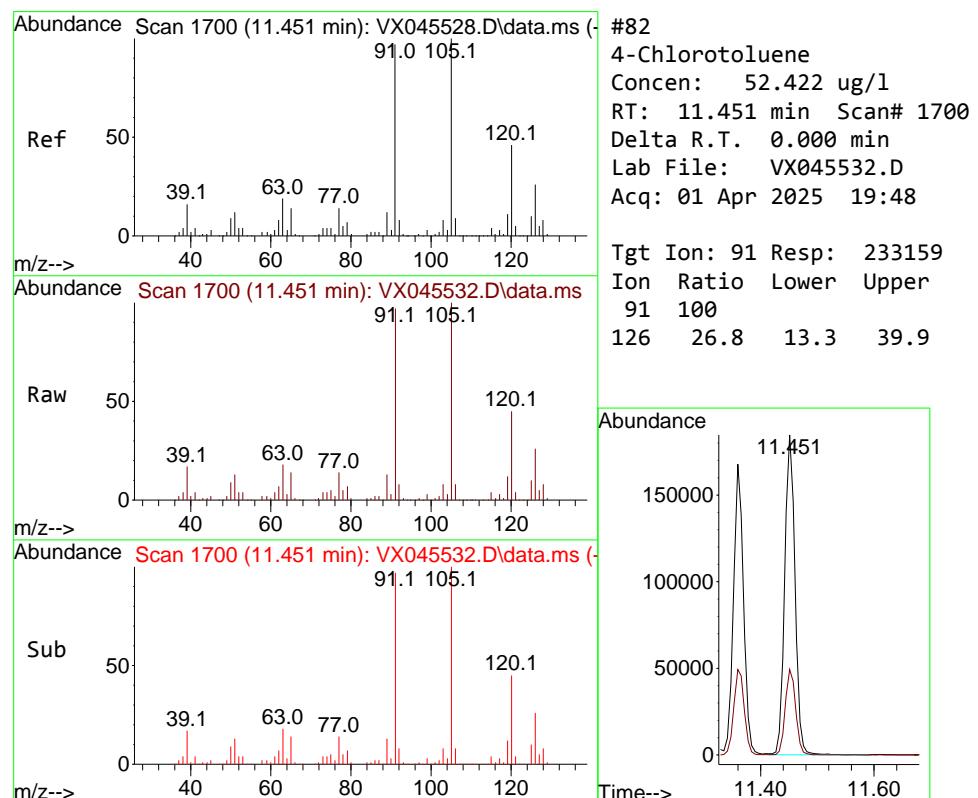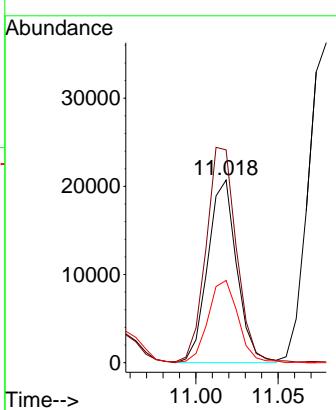

#82  
4-Chlorotoluene  
Concen: 52.422 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion: 91 Resp: 233159  
Ion Ratio Lower Upper  
91 100  
126 26.8 13.3 39.9

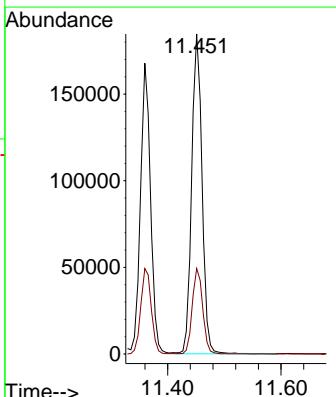



#83

tert-Butylbenzene

Concen: 53.274 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025



#84

1,2,4-Trimethylbenzene

Concen: 52.990 ug/l



RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min


Lab File: VX045532.D




Acq: 01 Apr 2025 19:48

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
105	100		238257		
120	42.8	21.4		64.3	

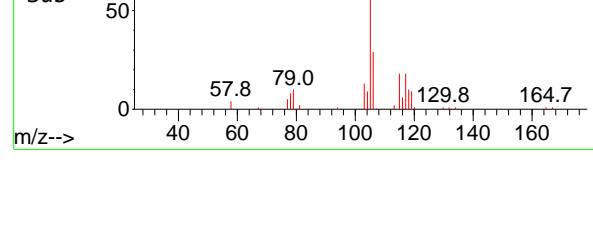

Abundance

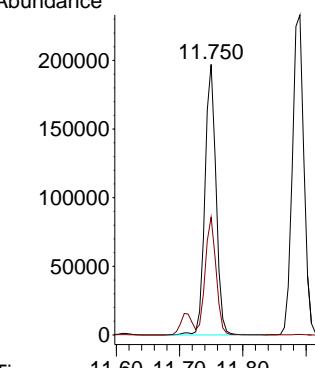



#85

sec-Butylbenzene

Concen: 53.903 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

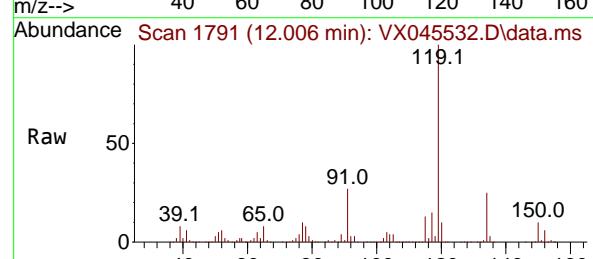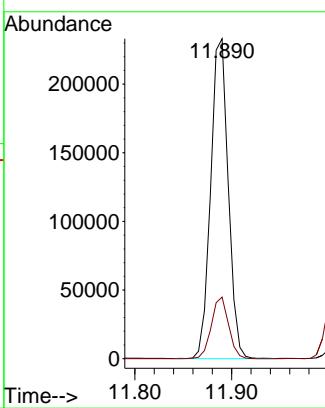

#86

p-Isopropyltoluene

Concen: 54.337 ug/l


RT: 12.006 min Scan# 1791



Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt	Ion:119	Resp:	244031
Ion	Ratio	Lower	Upper
119	100		
134	24.8	12.6	37.8
91	27.0	13.7	41.1

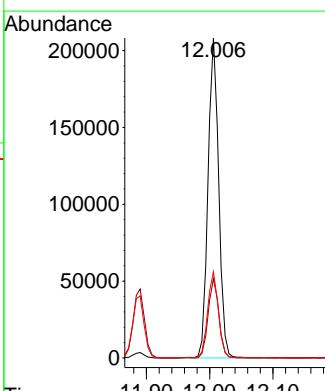

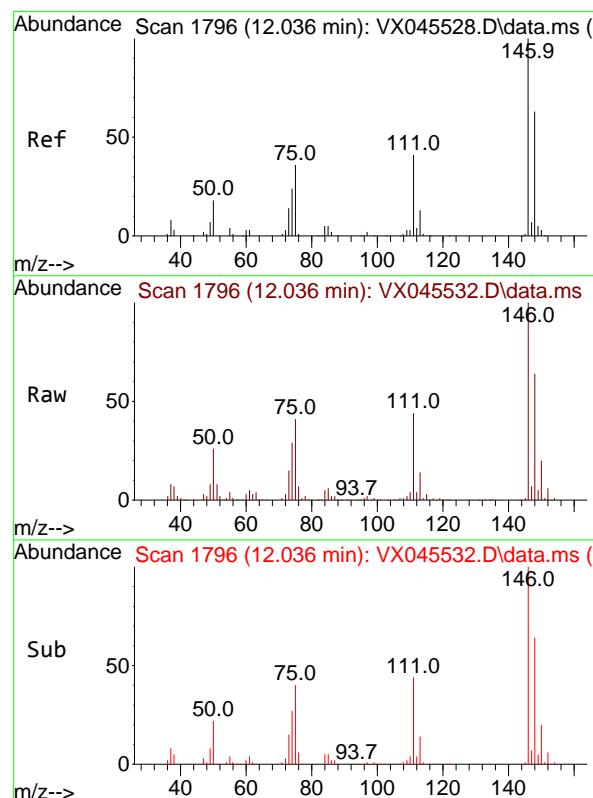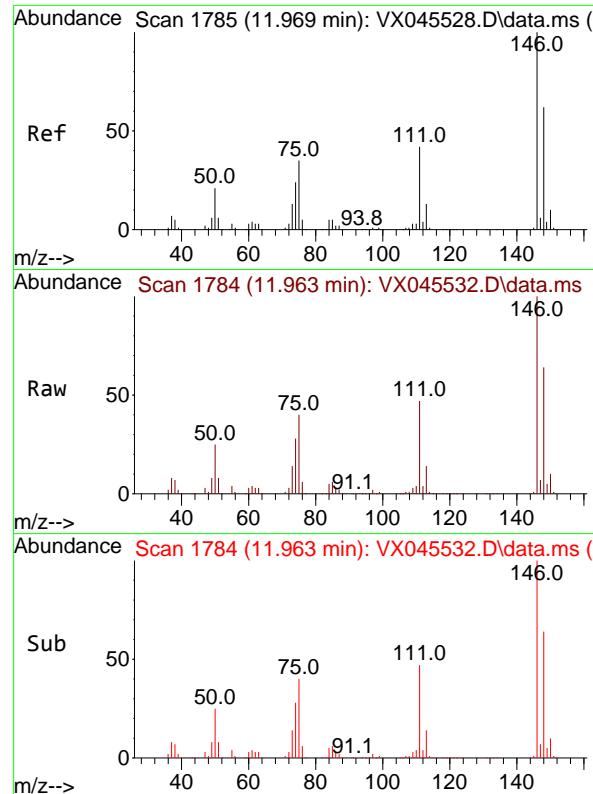

#87

1,3-Dichlorobenzene

Concen: 50.521 ug/l

RT: 11.963 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

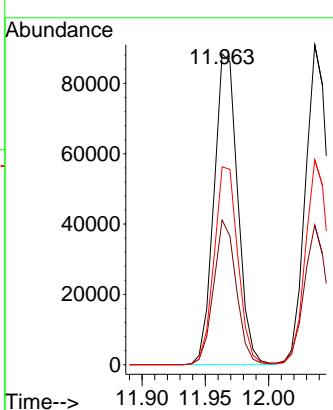

#88

1,4-Dichlorobenzene

Concen: 49.117 ug/l


RT: 12.036 min Scan# 1796




Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt	Ion:146	Resp:	113458
Ion	Ratio	Lower	Upper
146	100		
111	44.1	20.9	62.8
148	64.5	31.5	94.5





#89

n-Butylbenzene

Concen: 55.189 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48





Instrument : MSVOA\_X

ClientSampleId : ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

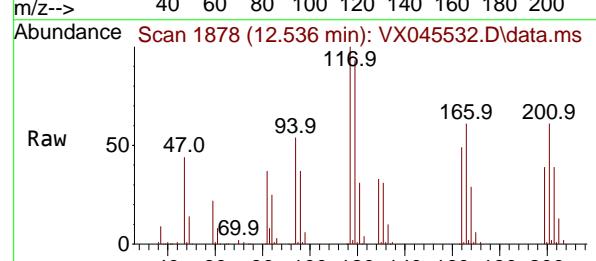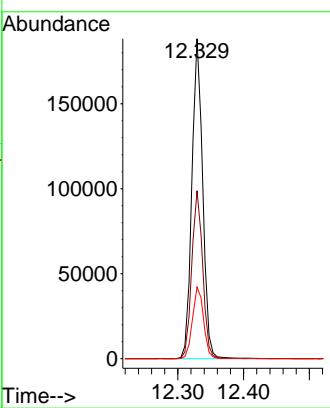

#90

Hexachloroethane

Concen: 54.066 ug/l


RT: 12.536 min Scan# 1878


Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt Ion:117 Resp: 41729  
 Ion Ratio Lower Upper  
 117 100  
 201 61.0 31.2 93.6

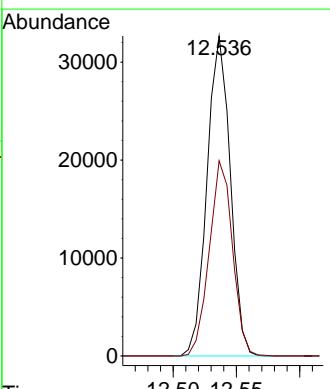

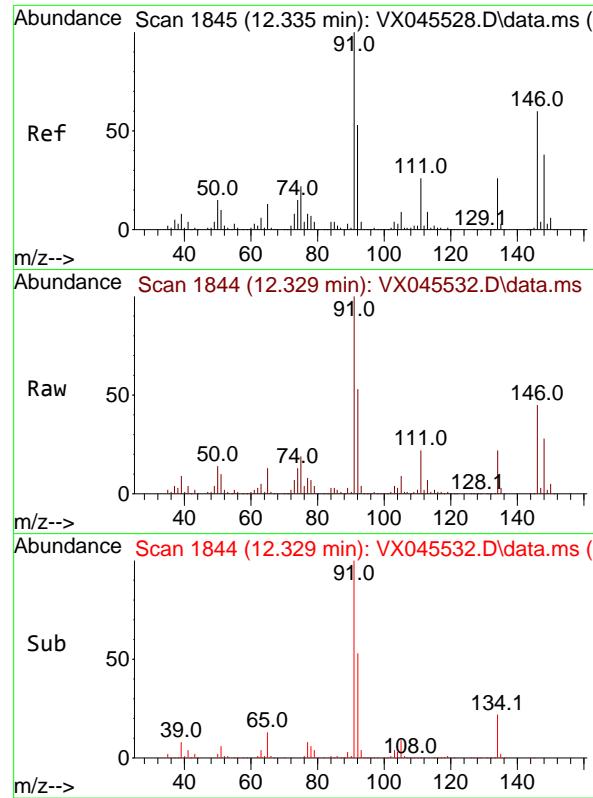


#91  
1,2-Dichlorobenzene  
Concen: 49.938 ug/l  
RT: 12.329 min Scan# 1  
Delta R.T. -0.006 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225


**Manual Integrations**  
**APPROVED**


Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

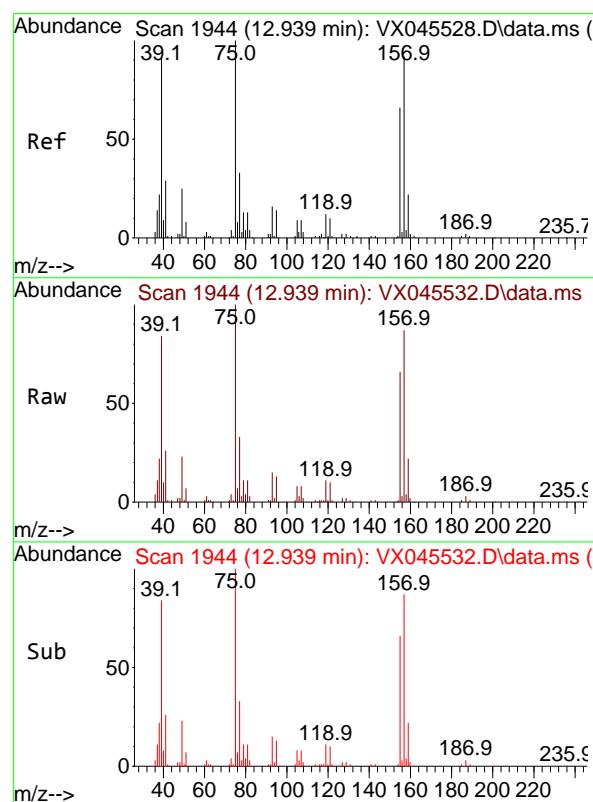

#92  
1,2-Dibromo-3-Chloropropane  
Concen: 53.226 ug/l  
RT: 12.939 min Scan# 1944  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion: 75 Resp: 21184  
Ion Ratio Lower Upper  
75 100  
155 69.4 34.9 104.7  
157 90.2 44.9 134.7

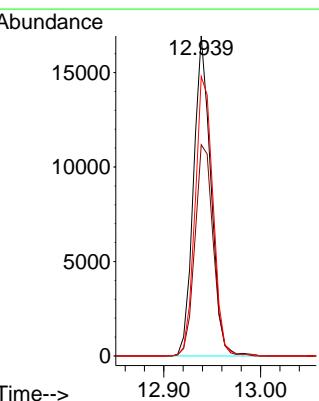


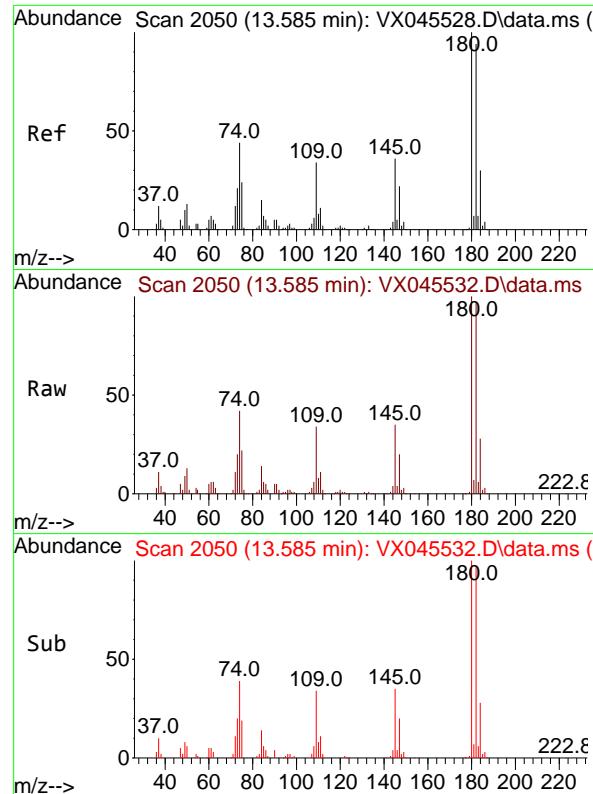


#93  
1,2,4-Trichlorobenzene  
Concen: 51.935 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Instrument : MSVOA\_X  
ClientSampleId : ICVVX040225


**Manual Integrations**  
**APPROVED**



Reviewed By :Amit Patel 04/02/2025  
Supervised By :Mahesh Dadoda 04/02/2025

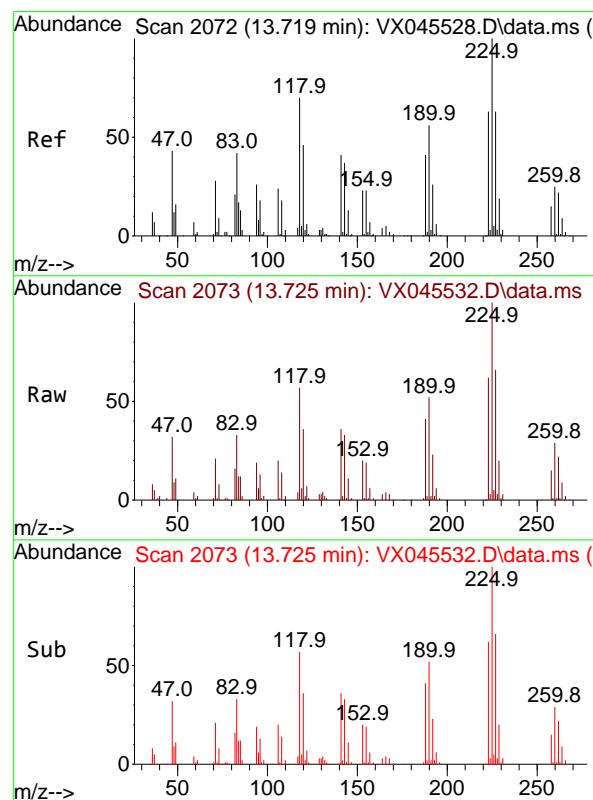

#94  
Hexachlorobutadiene  
Concen: 49.961 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. 0.006 min  
Lab File: VX045532.D  
Acq: 01 Apr 2025 19:48

Tgt Ion:225 Resp: 27147  
Ion Ratio Lower Upper  
225 100  
223 62.9 31.1 93.3  
227 63.0 32.2 96.6

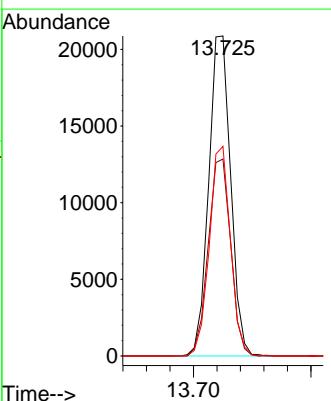

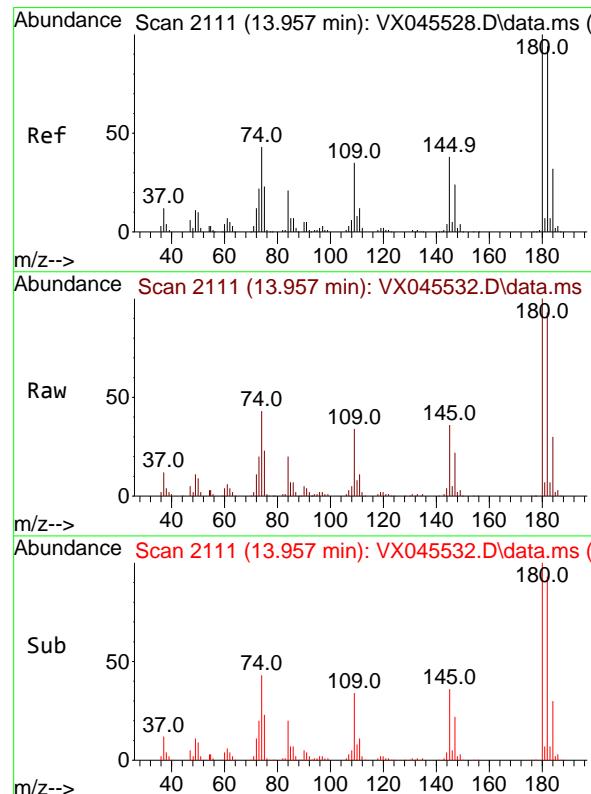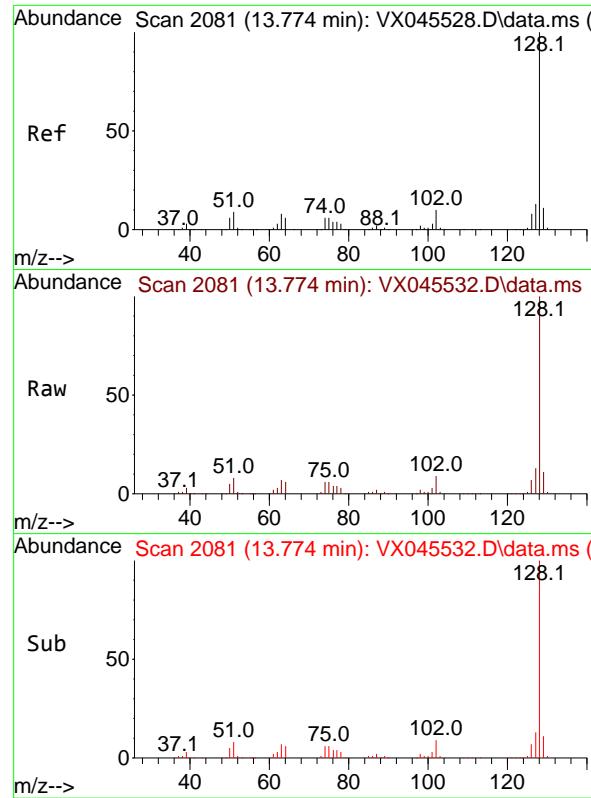

#95

Naphthalene

Concen: 52.765 ug/l

RT: 13.774 min Scan# 2111

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX040225

**Manual Integrations  
APPROVED**

Reviewed By :Amit Patel 04/02/2025

Supervised By :Mahesh Dadoda 04/02/2025

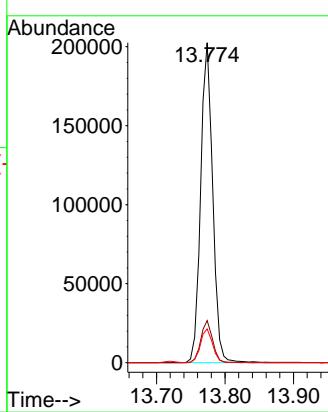

#96

1,2,3-Trichlorobenzene

Concen: 50.396 ug/l


RT: 13.957 min Scan# 2111

Delta R.T. 0.000 min

Lab File: VX045532.D

Acq: 01 Apr 2025 19:48

Tgt	Ion:180	Resp:	66542
Ion	Ratio	Lower	Upper
180	100		
182	94.8	47.3	141.8
145	36.4	18.2	54.6

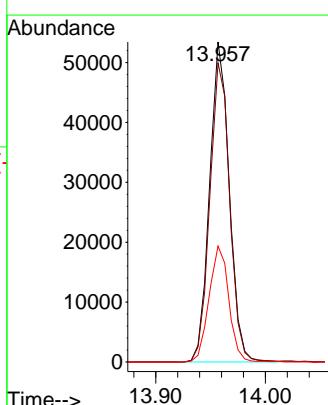

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045532.D  
 Acq On : 01 Apr 2025 19:48  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX040225**

Quant Time: Apr 02 03:14:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	101	0.00
2 T	Dichlorodifluoromethane	0.748	0.784	-4.8	97	0.00
3 P	Chloromethane	0.768	0.743	3.3	96	0.00
4 C	Vinyl Chloride	0.703	0.686	2.4#	97	0.00
5 T	Bromomethane	0.333	0.313	6.0	96	0.00
6 T	Chloroethane	0.373	0.385	-3.2	98	0.00
7 T	Trichlorofluoromethane	1.048	1.056	-0.8	99	0.00
8 T	Diethyl Ether	0.352	0.347	1.4	99	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.614	0.608	1.0	99	0.00
10 T	Methyl Iodide	0.766	0.745	2.7	95	0.00
11 T	Tert butyl alcohol	0.123	0.121	1.6	97	0.00
12 CM	1,1-Dichloroethene	0.600	0.597	0.5#	100	0.00
13 T	Acrolein	0.169	0.161	4.7	98	0.00
14 T	Allyl chloride	1.139	1.151	-1.1	100	0.00
15 T	Acrylonitrile	0.388	0.385	0.8	96	0.00
16 T	Acetone	0.375	0.363	3.2	98	0.00
17 T	Carbon Disulfide	1.483	1.544	-4.1	101	0.00
18 T	Methyl Acetate	0.864	0.843	2.4	100	0.00
19 T	Methyl tert-butyl Ether	2.100	2.140	-1.9	102	0.00
20 T	Methylene Chloride	0.703	0.690	1.8	99	0.00
21 T	trans-1,2-Dichloroethene	0.613	0.611	0.3	99	0.00
22 T	Diisopropyl ether	2.243	2.284	-1.8	101	0.00
23 T	Vinyl Acetate	1.938	2.074	-7.0	101	0.00
24 P	1,1-Dichloroethane	1.269	1.261	0.6	101	0.00
25 T	2-Butanone	0.550	0.560	-1.8	97	0.00
26 T	2,2-Dichloropropane	0.820	0.853	-4.0	102	0.00
27 T	cis-1,2-Dichloroethene	0.747	0.733	1.9	99	0.00
28 T	Bromochloromethane	0.613	0.594	3.1	101	0.00
29 T	Tetrahydrofuran	0.356	0.356	0.0	97	0.00
30 C	Chloroform	1.306	1.295	0.8#	100	0.00
31 T	Cyclohexane	1.122	1.112	0.9	100	0.00
32 T	1,1,1-Trichloroethane	1.105	1.112	-0.6	102	0.00
33 S	1,2-Dichloroethane-d4	0.914	0.920	-0.7	107	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	104	0.00
35 S	Dibromofluoromethane	0.355	0.349	1.7	105	0.00
36 T	1,1-Dichloropropene	0.479	0.480	-0.2	103	0.00
37 T	Ethyl Acetate	0.604	0.601	0.5	100	0.00
38 T	Carbon Tetrachloride	0.518	0.525	-1.4	102	0.00
39 T	Methylcyclohexane	0.587	0.589	-0.3	98	0.00
40 TM	Benzene	1.463	1.440	1.6	101	0.00
41 T	Methacrylonitrile	0.318	0.338	-6.3	100	0.00
42 TM	1,2-Dichloroethane	0.604	0.591	2.2	99	0.00
43 T	Isopropyl Acetate	0.915	0.943	-3.1	100	0.00
44 TM	Trichloroethene	0.348	0.331	4.9	98	0.00
45 C	1,2-Dichloropropane	0.365	0.361	1.1#	100	0.00
46 T	Dibromomethane	0.280	0.272	2.9	97	0.00
47 T	Bromodichloromethane	0.560	0.551	1.6	100	0.00
48 T	Methyl methacrylate	0.472	0.487	-3.2	100	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045532.D  
 Acq On : 01 Apr 2025 19:48  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX040225**

Quant Time: Apr 02 03:14:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.009	0.008	11.1	92	0.00
50 S	Toluene-d8	1.238	1.242	-0.3	106	0.00
51 T	4-Methyl-2-Pentanone	0.606	0.619	-2.1	97	0.00
52 CM	Toluene	0.885	0.867	2.0#	99	0.00
53 T	t-1,3-Dichloropropene	0.467	0.502	-7.5	103	0.00
54 T	cis-1,3-Dichloropropene	0.526	0.567	-7.8	104	0.00
55 T	1,1,2-Trichloroethane	0.353	0.346	2.0	100	0.00
56 T	Ethyl methacrylate	0.546	0.586	-7.3	102	0.00
57 T	1,3-Dichloropropane	0.614	0.613	0.2	101	0.00
58 T	2-Chloroethyl Vinyl ether	0.276	0.287	-4.0	100	0.00
59 T	2-Hexanone	0.449	0.452	-0.7	96	0.00
60 T	Dibromochloromethane	0.385	0.392	-1.8	99	0.00
61 T	1,2-Dibromoethane	0.357	0.362	-1.4	101	0.00
62 S	4-Bromofluorobenzene	0.451	0.460	-2.0	105	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	101	0.00
64 T	Tetrachloroethene	0.353	0.334	5.4	97	0.00
65 PM	Chlorobenzene	1.068	1.073	-0.5	100	0.00
66 T	1,1,1,2-Tetrachloroethane	0.371	0.375	-1.1	102	0.00
67 C	Ethyl Benzene	1.914	1.973	-3.1#	100	0.00
68 T	m/p-Xylenes	0.696	0.715	-2.7	100	0.00
69 T	o-Xylene	0.686	0.708	-3.2	100	0.00
70 T	Styrene	1.132	1.191	-5.2	99	0.00
71 P	Bromoform	0.277	0.292	-5.4	100	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	98	0.00
73 T	Isopropylbenzene	4.005	4.229	-5.6	99	0.00
74 T	N-amyl acetate	1.916	2.084	-8.8	100	0.00
75 P	1,1,2,2-Tetrachloroethane	1.407	1.368	2.8	97	0.00
76 T	1,2,3-Trichloropropane	1.220	1.213	0.6	97	0.00
77 T	Bromobenzene	0.925	0.935	-1.1	98	0.00
78 T	n-propylbenzene	4.613	4.979	-7.9	100	0.00
79 T	2-Chlorotoluene	2.949	3.012	-2.1	100	0.00
80 T	1,3,5-Trimethylbenzene	3.312	3.546	-7.1	99	0.00
81 T	trans-1,4-Dichloro-2-butene	0.359	0.377	-5.0	100	0.00
82 T	4-Chlorotoluene	3.288	3.447	-4.8	98	0.00
83 T	tert-Butylbenzene	3.279	3.494	-6.6	100	0.00
84 T	1,2,4-Trimethylbenzene	3.324	3.523	-6.0	98	0.00
85 T	sec-Butylbenzene	4.027	4.342	-7.8	99	0.00
86 T	p-Isopropyltoluene	3.320	3.608	-8.7	101	0.00
87 T	1,3-Dichlorobenzene	1.684	1.702	-1.1	98	0.00
88 T	1,4-Dichlorobenzene	1.708	1.678	1.8	97	0.00
89 T	n-Butylbenzene	2.879	3.178	-10.4	99	0.00
90 T	Hexachloroethane	0.571	0.617	-8.1	102	0.00
91 T	1,2-Dichlorobenzene	1.675	1.673	0.1	98	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.294	0.313	-6.5	98	0.00
93 T	1,2,4-Trichlorobenzene	0.932	0.968	-3.9	101	0.00
94 T	Hexachlorobutadiene	0.402	0.401	0.2	98	0.00
95 T	Naphthalene	3.469	3.661	-5.5	97	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
Data File : VX045532.D  
Acq On : 01 Apr 2025 19:48  
Operator : JC/MD  
Sample : VSTDICV050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
ICVVX040225

Quant Time: Apr 02 03:14:42 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	0.976	0.984	-0.8	97	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045532.D  
 Acq On : 01 Apr 2025 19:48  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX040225**

Quant Time: Apr 02 03:14:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	101	0.00
2 T	Dichlorodifluoromethane	50.000	52.454	-4.9	97	0.00
3 P	Chloromethane	50.000	48.349	3.3	96	0.00
4 C	Vinyl Chloride	50.000	48.816	2.4#	97	0.00
5 T	Bromomethane	50.000	46.991	6.0	96	0.00
6 T	Chloroethane	50.000	51.586	-3.2	98	0.00
7 T	Trichlorofluoromethane	50.000	50.354	-0.7	99	0.00
8 T	Diethyl Ether	50.000	49.228	1.5	99	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	49.528	0.9	99	0.00
10 T	Methyl Iodide	50.000	48.626	2.7	95	0.00
11 T	Tert butyl alcohol	250.000	246.612	1.4	97	0.00
12 CM	1,1-Dichloroethene	50.000	49.726	0.5#	100	0.00
13 T	Acrolein	250.000	238.141	4.7	98	0.00
14 T	Allyl chloride	50.000	50.541	-1.1	100	0.00
15 T	Acrylonitrile	250.000	248.351	0.7	96	0.00
16 T	Acetone	250.000	241.904	3.2	98	0.00
17 T	Carbon Disulfide	50.000	52.057	-4.1	101	0.00
18 T	Methyl Acetate	50.000	48.742	2.5	100	0.00
19 T	Methyl tert-butyl Ether	50.000	50.950	-1.9	102	0.00
20 T	Methylene Chloride	50.000	49.055	1.9	99	0.00
21 T	trans-1,2-Dichloroethene	50.000	49.800	0.4	99	0.00
22 T	Diisopropyl ether	50.000	50.895	-1.8	101	0.00
23 T	Vinyl Acetate	250.000	267.449	-7.0	101	0.00
24 P	1,1-Dichloroethane	50.000	49.677	0.6	101	0.00
25 T	2-Butanone	250.000	254.882	-2.0	97	0.00
26 T	2,2-Dichloropropane	50.000	52.020	-4.0	102	0.00
27 T	cis-1,2-Dichloroethene	50.000	49.049	1.9	99	0.00
28 T	Bromochloromethane	50.000	48.403	3.2	101	0.00
29 T	Tetrahydrofuran	250.000	249.473	0.2	97	0.00
30 C	Chloroform	50.000	49.614	0.8#	100	0.00
31 T	Cyclohexane	50.000	49.583	0.8	100	0.00
32 T	1,1,1-Trichloroethane	50.000	50.330	-0.7	102	0.00
33 S	1,2-Dichloroethane-d4	50.000	50.329	-0.7	107	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	104	0.00
35 S	Dibromofluoromethane	50.000	49.256	1.5	105	0.00
36 T	1,1-Dichloropropene	50.000	50.088	-0.2	103	0.00
37 T	Ethyl Acetate	50.000	49.787	0.4	100	0.00
38 T	Carbon Tetrachloride	50.000	50.667	-1.3	102	0.00
39 T	Methylcyclohexane	50.000	50.124	-0.2	98	0.00
40 TM	Benzene	50.000	49.212	1.6	101	0.00
41 T	Methacrylonitrile	50.000	53.098	-6.2	100	0.00
42 TM	1,2-Dichloroethane	50.000	48.875	2.3	99	0.00
43 T	Isopropyl Acetate	50.000	51.539	-3.1	100	0.00
44 TM	Trichloroethene	50.000	47.643	4.7	98	0.00
45 C	1,2-Dichloropropane	50.000	49.521	1.0#	100	0.00
46 T	Dibromomethane	50.000	48.542	2.9	97	0.00
47 T	Bromodichloromethane	50.000	49.273	1.5	100	0.00
48 T	Methyl methacrylate	50.000	51.507	-3.0	100	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045532.D  
 Acq On : 01 Apr 2025 19:48  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX040225**

Quant Time: Apr 02 03:14:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	955.327	4.5	92	0.00
50 S	Toluene-d8	50.000	50.160	-0.3	106	0.00
51 T	4-Methyl-2-Pentanone	250.000	254.994	-2.0	97	0.00
52 CM	Toluene	50.000	48.994	2.0#	99	0.00
53 T	t-1,3-Dichloropropene	50.000	46.783	6.4	103	0.00
54 T	cis-1,3-Dichloropropene	50.000	53.878	-7.8	104	0.00
55 T	1,1,2-Trichloroethane	50.000	49.007	2.0	100	0.00
56 T	Ethyl methacrylate	50.000	53.705	-7.4	102	0.00
57 T	1,3-Dichloropropane	50.000	49.869	0.3	101	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	260.201	-4.1	100	0.00
59 T	2-Hexanone	250.000	251.710	-0.7	96	0.00
60 T	Dibromochloromethane	50.000	50.983	-2.0	99	0.00
61 T	1,2-Dibromoethane	50.000	50.693	-1.4	101	0.00
62 S	4-Bromofluorobenzene	50.000	50.959	-1.9	105	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	101	0.00
64 T	Tetrachloroethene	50.000	47.239	5.5	97	0.00
65 PM	Chlorobenzene	50.000	50.207	-0.4	100	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	50.495	-1.0	102	0.00
67 C	Ethyl Benzene	50.000	51.558	-3.1#	100	0.00
68 T	m/p-Xylenes	100.000	102.728	-2.7	100	0.00
69 T	o-Xylene	50.000	51.650	-3.3	100	0.00
70 T	Styrene	50.000	52.624	-5.2	99	0.00
71 P	Bromoform	50.000	52.694	-5.4	100	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	98	0.00
73 T	Isopropylbenzene	50.000	52.794	-5.6	99	0.00
74 T	N-amyl acetate	50.000	54.387	-8.8	100	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	48.608	2.8	97	0.00
76 T	1,2,3-Trichloropropane	50.000	49.741	0.5	97	0.00
77 T	Bromobenzene	50.000	50.525	-1.0	98	0.00
78 T	n-propylbenzene	50.000	53.967	-7.9	100	0.00
79 T	2-Chlorotoluene	50.000	51.057	-2.1	100	0.00
80 T	1,3,5-Trimethylbenzene	50.000	53.534	-7.1	99	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	52.482	-5.0	100	0.00
82 T	4-Chlorotoluene	50.000	52.422	-4.8	98	0.00
83 T	tert-Butylbenzene	50.000	53.274	-6.5	100	0.00
84 T	1,2,4-Trimethylbenzene	50.000	52.990	-6.0	98	0.00
85 T	sec-Butylbenzene	50.000	53.903	-7.8	99	0.00
86 T	p-Isopropyltoluene	50.000	54.337	-8.7	101	0.00
87 T	1,3-Dichlorobenzene	50.000	50.521	-1.0	98	0.00
88 T	1,4-Dichlorobenzene	50.000	49.117	1.8	97	0.00
89 T	n-Butylbenzene	50.000	55.189	-10.4	99	0.00
90 T	Hexachloroethane	50.000	54.066	-8.1	102	0.00
91 T	1,2-Dichlorobenzene	50.000	49.938	0.1	98	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	53.226	-6.5	98	0.00
93 T	1,2,4-Trichlorobenzene	50.000	51.935	-3.9	101	0.00
94 T	Hexachlorobutadiene	50.000	49.961	0.1	98	0.00
95 T	Naphthalene	50.000	52.765	-5.5	97	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
Data File : VX045532.D  
Acq On : 01 Apr 2025 19:48  
Operator : JC/MD  
Sample : VSTDICV050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
ICVVX040225

Quant Time: Apr 02 03:14:42 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	50.000	50.396	-0.8	97	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	CHEMTECH	Contract:	JAC005				
Lab Code:	CHEM	Case No.:	Q1711	SAS No.:	Q1711	SDG No.:	Q1711
Instrument ID:	MSVOA_X	Calibration Date/Time:			04/03/2025	10:30	
Lab File ID:	VX045559.D	Init. Calib. Date(s):			04/01/2025	04/01/2025	
Heated Purge:	(Y/N) N	Init. Calib. Time(s):			17:06	19:02	
GC Column:	DB-624UI	ID:	0.18	(mm)			

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Vinyl Chloride	0.703	0.734		4.41	20
1,1-Dichloroethene	0.600	0.611		1.83	20
1,1-Dichloroethane	1.269	1.249	0.1	-1.58	20
cis-1,2-Dichloroethene	0.747	0.736		-1.47	20
1,1,1-Trichloroethane	1.105	1.105		0	20
Benzene	1.463	1.502		2.67	20
1,2-Dichloroethane	0.604	0.634		4.97	20
Trichloroethene	0.348	0.350		0.57	20
1,1,2-Trichloroethane	0.353	0.367		3.97	20
Tetrachloroethene	0.353	0.354		0.28	20
1,2-Dichloroethane-d4	0.914	0.886		-3.06	20
Dibromofluoromethane	0.355	0.358		0.85	20
Toluene-d8	1.238	1.248		0.81	20
4-Bromofluorobenzene	0.451	0.460		2	20

All other compounds must meet a minimum RRF of 0.010.  
RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045559.D  
 Acq On : 03 Apr 2025 10:30  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDCCC050

Quant Time: Apr 04 01:17:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	95221	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	162684	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	143783	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	66270	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.946	65	84371	48.452	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	96.900%	
35) Dibromofluoromethane	5.379	113	58174	50.400	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	100.800%	
50) Toluene-d8	8.647	98	203099	50.412	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	100.820%	
62) 4-Bromofluorobenzene	11.079	95	74900	51.040	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	102.080%	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.167	85	82166	57.700	ug/l	100
3) Chloromethane	1.307	50	74478	50.909	ug/l	98
4) Vinyl Chloride	1.374	62	69881	52.195	ug/l	99
5) Bromomethane	1.593	94	30702	48.364	ug/l	97
6) Chloroethane	1.666	64	38584	54.319	ug/l	99
7) Trichlorofluoromethane	1.874	101	105263	52.725	ug/l	98
8) Diethyl Ether	2.130	74	33034	49.284	ug/l	98
9) 1,1,2-Trichlorotrifluo...	2.319	101	62683	53.581	ug/l	98
10) Methyl Iodide	2.441	142	74575	51.106	ug/l	99
11) Tert butyl alcohol	2.977	59	57958	247.660	ug/l	99
12) 1,1-Dichloroethene	2.307	96	58158	50.876	ug/l	98
13) Acrolein	2.233	56	93576	290.369	ug/l	99
14) Allyl chloride	2.654	41	110918	51.139	ug/l	98
15) Acrylonitrile	3.063	53	185693	251.370	ug/l	98
16) Acetone	2.380	43	175069	244.836	ug/l	97
17) Carbon Disulfide	2.502	76	146189	51.779	ug/l	99
18) Methyl Acetate	2.703	43	81783	49.677	ug/l	100
19) Methyl tert-butyl Ether	3.111	73	197731	49.447	ug/l	100
20) Methylene Chloride	2.782	84	65985	49.292	ug/l	98
21) trans-1,2-Dichloroethene	3.081	96	58555	50.139	ug/l	99
22) Diisopropyl ether	3.757	45	216234	50.611	ug/l	96
23) Vinyl Acetate	3.715	43	963835	261.101	ug/l	100
24) 1,1-Dichloroethane	3.605	63	118946	49.227	ug/l	100
25) 2-Butanone	4.550	43	269054	257.055	ug/l	100
26) 2,2-Dichloropropane	4.465	77	86074	55.135	ug/l	99
27) cis-1,2-Dichloroethene	4.477	96	70036	49.223	ug/l	99
28) Bromochloromethane	4.891	49	56952	48.775	ug/l	99
29) Tetrahydrofuran	5.001	42	169709	250.088	ug/l	99
30) Chloroform	5.087	83	122855	49.413	ug/l	97
31) Cyclohexane	5.458	56	108125	50.618	ug/l	98
32) 1,1,1-Trichloroethane	5.373	97	105194	50.002	ug/l	99
36) 1,1-Dichloropropene	5.684	75	80867	51.889	ug/l	100
37) Ethyl Acetate	4.709	43	100010	50.922	ug/l	99
38) Carbon Tetrachloride	5.666	117	91247	54.175	ug/l	98
39) Methylcyclohexane	7.373	83	106620	55.811	ug/l	98
40) Benzene	6.025	78	244336	51.334	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045559.D  
 Acq On : 03 Apr 2025 10:30  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDCCC050

Quant Time: Apr 04 01:17:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.910	41	55849	53.895	ug/1	98
42) 1,2-Dichloroethane	6.080	62	103151	52.471	ug/1	99
43) Isopropyl Acetate	6.336	43	158368	53.203	ug/1	100
44) Trichloroethene	7.117	130	57018	50.400	ug/1	91
45) 1,2-Dichloropropane	7.421	63	61965	52.177	ug/1	99
46) Dibromomethane	7.574	93	47799	52.432	ug/1	99
47) Bromodichloromethane	7.818	83	97004	53.281	ug/1	98
48) Methyl methacrylate	7.690	41	82864	53.916	ug/1	99
49) 1,4-Dioxane	7.653	88	29748	1069.810	ug/1	98
51) 4-Methyl-2-Pentanone	8.568	43	535504	271.376	ug/1	99
52) Toluene	8.714	92	146995	51.038	ug/1	98
53) t-1,3-Dichloropropene	8.976	75	84356	48.265	ug/1	99
54) cis-1,3-Dichloropropene	8.360	75	95044	55.553	ug/1	96
55) 1,1,2-Trichloroethane	9.147	97	59666	51.988	ug/1	98
56) Ethyl methacrylate	9.116	69	97540	54.916	ug/1	100
57) 1,3-Dichloropropane	9.305	76	102855	51.465	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	250203	278.463	ug/1	100
59) 2-Hexanone	9.427	43	388703	266.003	ug/1	100
60) Dibromochloromethane	9.519	129	68554	54.791	ug/1	98
61) 1,2-Dibromoethane	9.604	107	61554	52.982	ug/1	99
64) Tetrachloroethene	9.269	164	50963	50.202	ug/1	97
65) Chlorobenzene	10.073	112	161334	52.511	ug/1	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	55208	51.757	ug/1	99
67) Ethyl Benzene	10.189	91	292313	53.122	ug/1	100
68) m/p-Xylenes	10.299	106	213521	106.687	ug/1	98
69) o-Xylene	10.640	106	104675	53.092	ug/1	99
70) Styrene	10.653	104	178474	54.847	ug/1	100
71) Bromoform	10.799	173	43615	54.761	ug/1 #	97
73) Isopropylbenzene	10.957	105	280025	52.752	ug/1	99
74) N-amyl acetate	10.842	43	131921	51.953	ug/1	100
75) 1,1,2,2-Tetrachloroethane	11.207	83	90162	48.351	ug/1	99
76) 1,2,3-Trichloropropane	11.238	75	80395m	49.735	ug/1	
77) Bromobenzene	11.195	156	62977	51.347	ug/1	99
78) n-propylbenzene	11.299	91	330313	54.023	ug/1	100
79) 2-Chlorotoluene	11.360	91	201387	51.521	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	237889	54.195	ug/1	99
81) trans-1,4-Dichloro-2-b...	11.018	75	25059	52.613	ug/1	99
82) 4-Chlorotoluene	11.451	91	231669	53.158	ug/1	99
83) tert-Butylbenzene	11.713	119	232038	53.394	ug/1	100
84) 1,2,4-Trimethylbenzene	11.750	105	238183	54.063	ug/1	100
85) sec-Butylbenzene	11.890	105	292834	54.862	ug/1	100
86) p-Isopropyltoluene	12.006	119	241650	54.914	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	114280	51.187	ug/1	100
88) 1,4-Dichlorobenzene	12.037	146	113108	49.973	ug/1	99
89) n-Butylbenzene	12.329	91	218225	57.188	ug/1	99
90) Hexachloroethane	12.536	117	42042	55.591	ug/1	100
91) 1,2-Dichlorobenzene	12.335	146	111954	50.437	ug/1	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	21298	54.613	ug/1	97
93) 1,2,4-Trichlorobenzene	13.585	180	66008	53.424	ug/1	97
94) Hexachlorobutadiene	13.725	225	28337	53.224	ug/1	98
95) Naphthalene	13.774	128	236621	51.463	ug/1	99
96) 1,2,3-Trichlorobenzene	13.957	180	66605	51.481	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045559.D  
 Acq On : 03 Apr 2025 10:30  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDCCC050**

Quant Time: Apr 04 01:17:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045559.D  
 Acq On : 03 Apr 2025 10:30  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1




Quant Time: Apr 04 01:17:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDCCC050

### Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

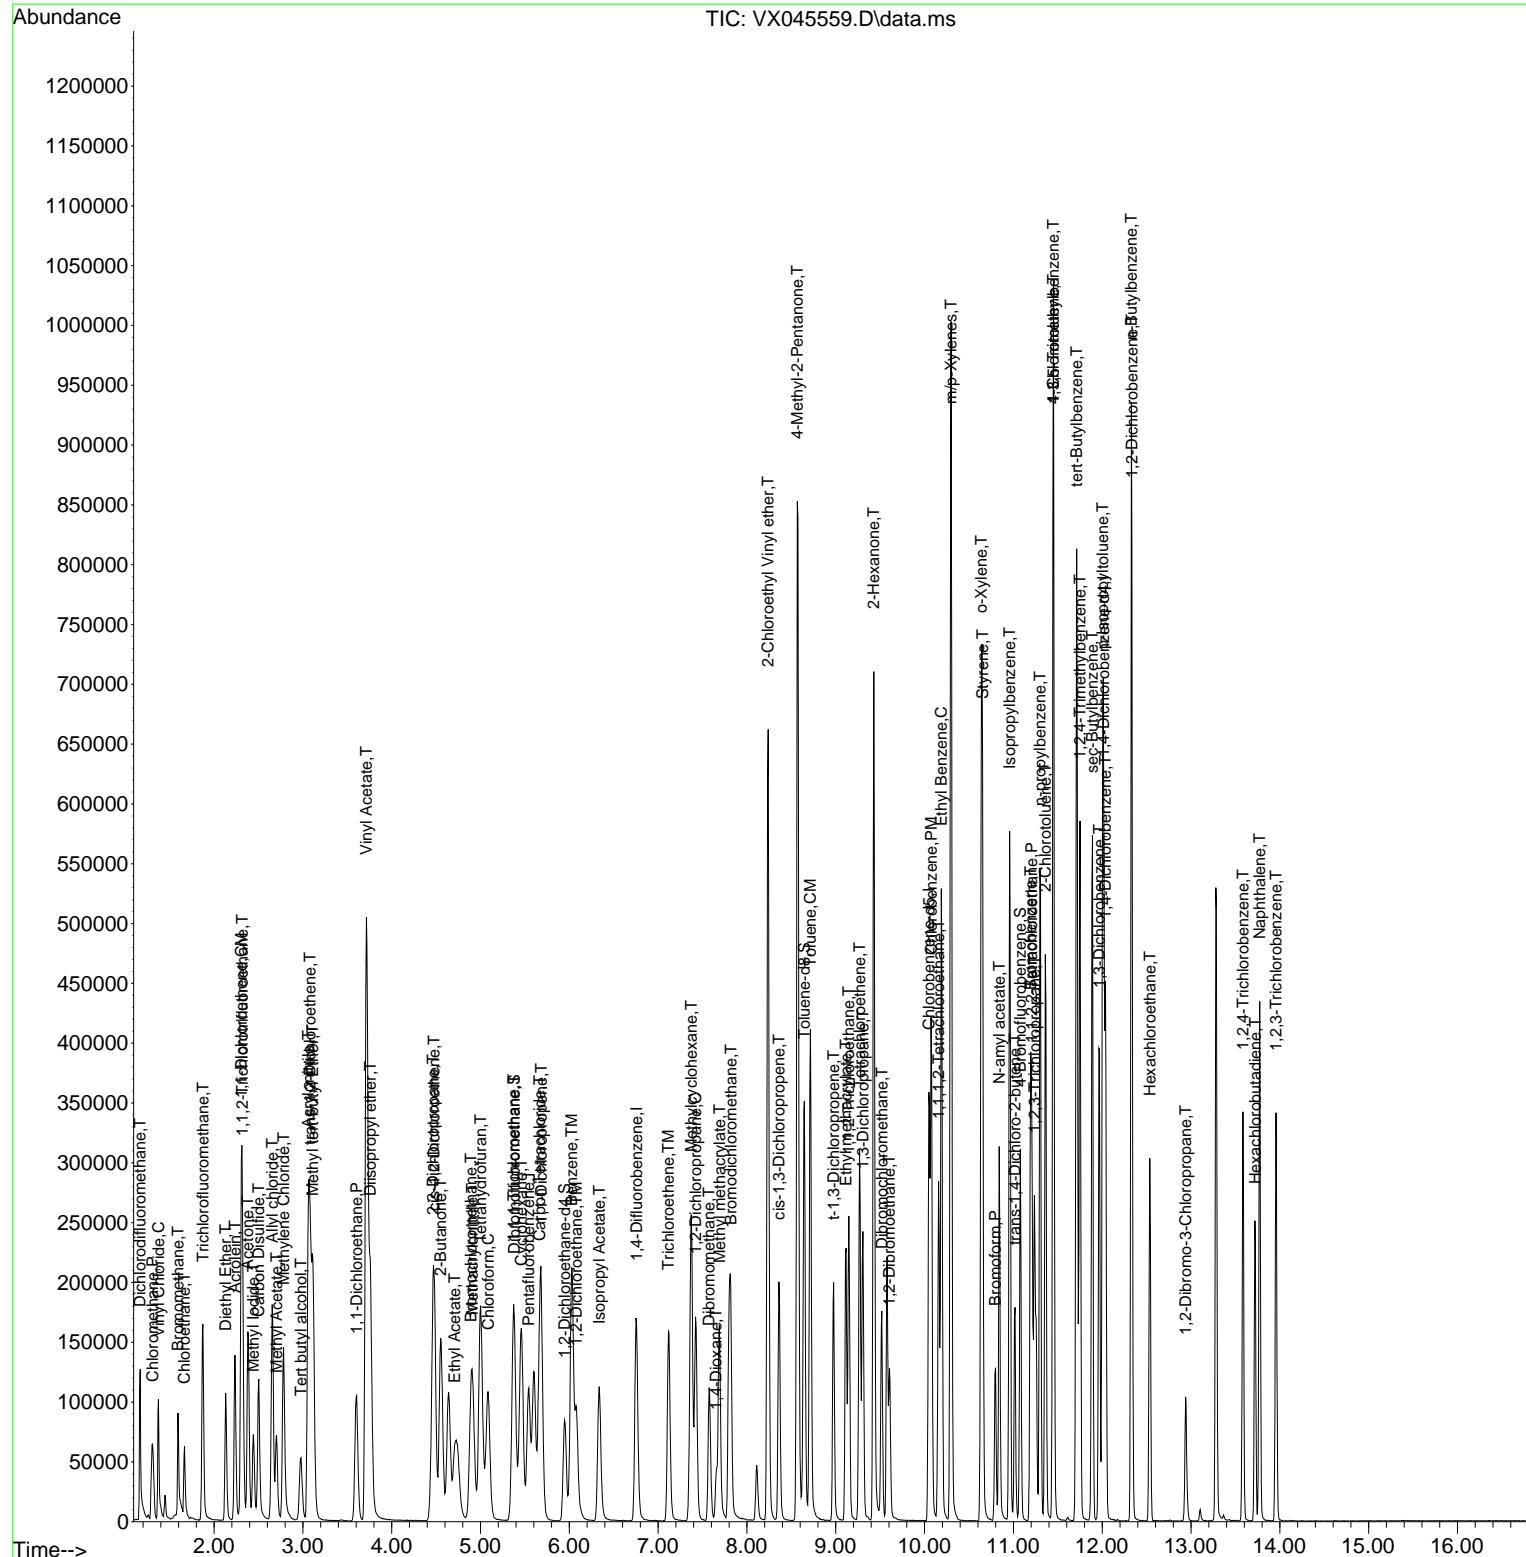





#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.544 min Scan# 7  
Delta R.T. -0.006 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30


Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

### Manual Integrations APPROVED



Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



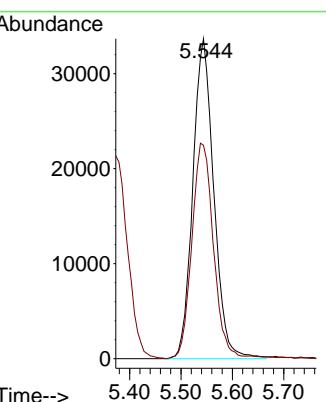


#2  
Dichlorodifluoromethane  
Concen: 57.700 ug/l  
RT: 1.167 min Scan# 13  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30



Tgt Ion: 85 Resp: 82166  
Ion Ratio Lower Upper  
85 100  
87 31.9 16.1 48.2

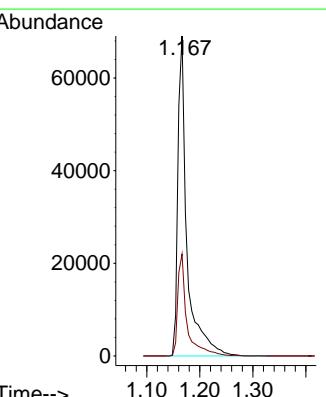



#3

Chloromethane

Concen: 50.909 ug/l

RT: 1.307 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30





Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

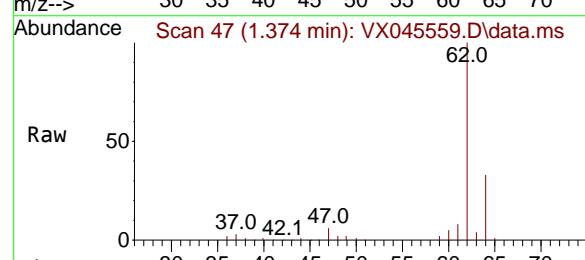 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#4

Vinyl Chloride


Concen: 52.195 ug/l




RT: 1.374 min Scan# 47

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

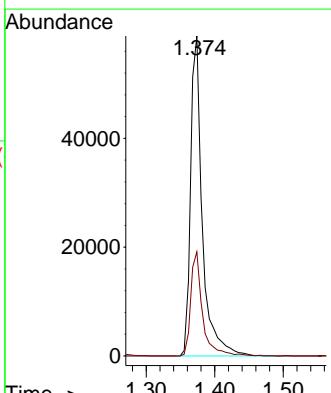 Tgt Ion: 62 Resp: 69881  
 Ion Ratio Lower Upper  
 62 100  
 64 32.5 25.5 38.3








#5  
Bromomethane  
Concen: 48.364 ug/l  
RT: 1.593 min Scan# 8  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025



#6  
Chloroethane  
Concen: 54.319 ug/l  
RT: 1.666 min Scan# 95  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30


Tgt Ion: 64 Resp: 38584  
Ion Ratio Lower Upper  
64 100  
66 32.6 26.3 39.5





#7  
Trichlorofluoromethane  
Concen: 52.725 ug/l  
RT: 1.874 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30




Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050




Tgt Ion:101 Resp: 10526  
Ion Ratio Lower Upper  
101 100  
103 65.4 51.1 76.7

### Manual Integrations APPROVED



Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

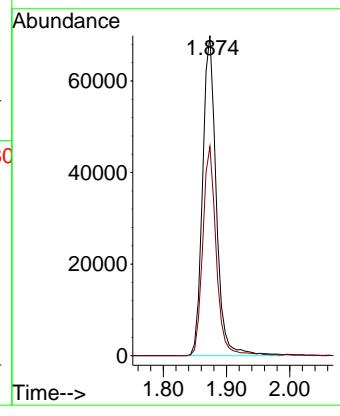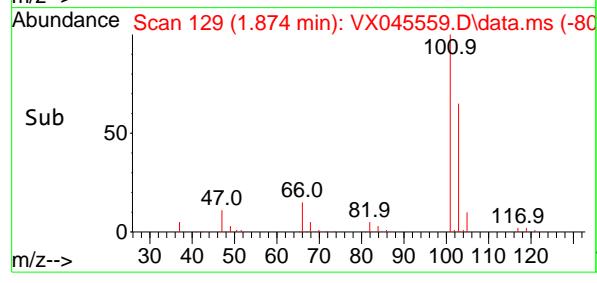


#8  
Diethyl Ether  
Concen: 49.284 ug/l  
RT: 2.130 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30





Tgt Ion: 74 Resp: 33034  
Ion Ratio Lower Upper  
74 100  
45 108.1 53.0 159.1

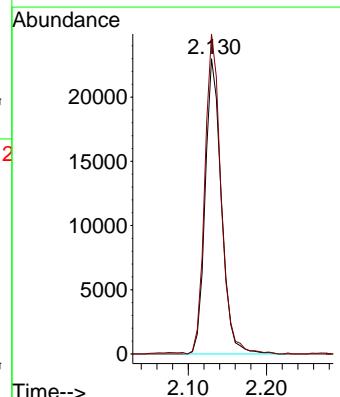





#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 53.581 ug/l  
RT: 2.319 min Scan# 2  
Delta R.T. -0.006 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30




Tgt Ion:101 Resp: 6268  
Ion Ratio Lower Upper  
101 100  
85 47.3 38.9 58.3  
151 70.2 57.5 86.3

### Manual Integrations APPROVED



Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

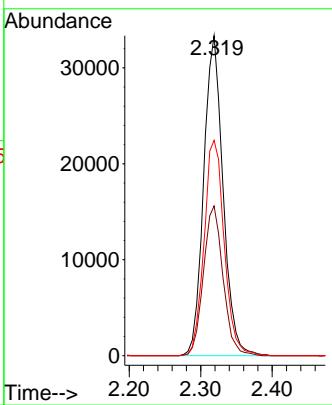


#10  
Methyl Iodide  
Concen: 51.106 ug/l  
RT: 2.441 min Scan# 222  
Delta R.T. -0.006 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30





Tgt Ion:142 Resp: 74575  
Ion Ratio Lower Upper  
142 100  
127 50.7 40.2 60.4  
141 14.2 11.7 17.5


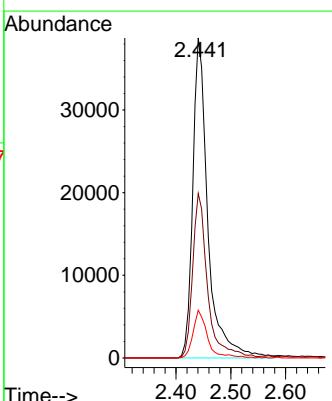




Abundance Scan 310 (2.977 min): VX045559.D\data.ms

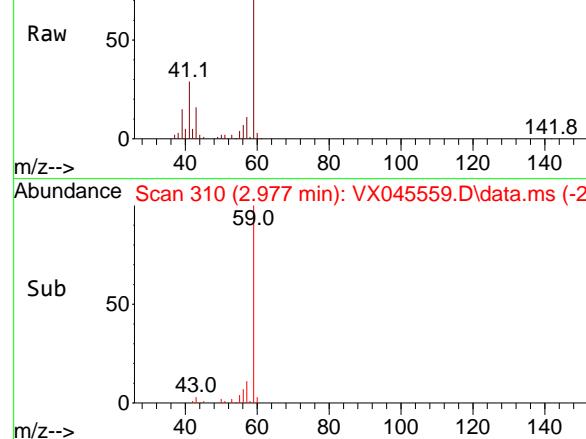

Abundance Scan 200 (2.307 min): VX045559.D\data.ms

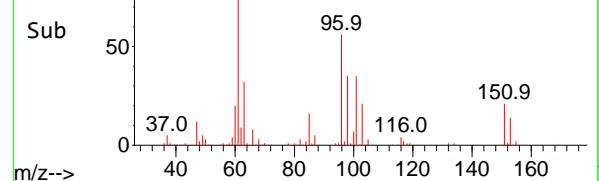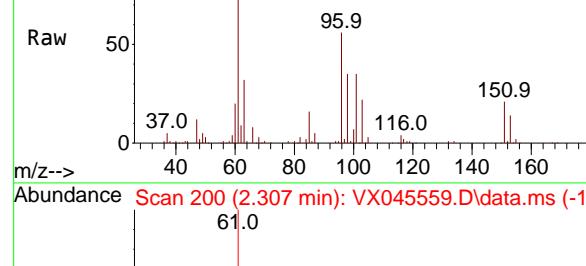

#11


Tert butyl alcohol  
Concen: 247.660 ug/l  
RT: 2.977 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCCC050

### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025







Tgt Ion: 59 Resp: 57958  
Ion Ratio Lower Upper  
59 100  
57 10.3 8.6 12.8

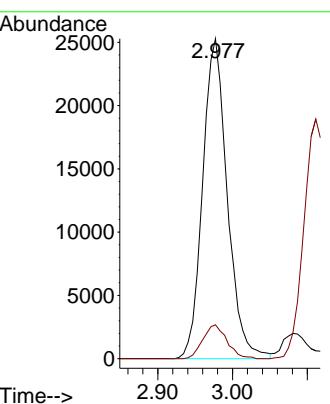

#12  
1,1-Dichloroethene  
Concen: 50.876 ug/l  
RT: 2.307 min Scan# 200  
Delta R.T. -0.006 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion: 96 Resp: 58158  
Ion Ratio Lower Upper  
96 100  
61 179.1 145.7 218.5  
98 63.0 51.6 77.4

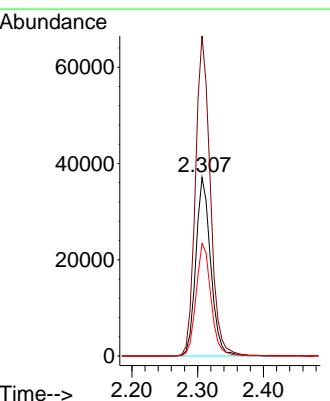

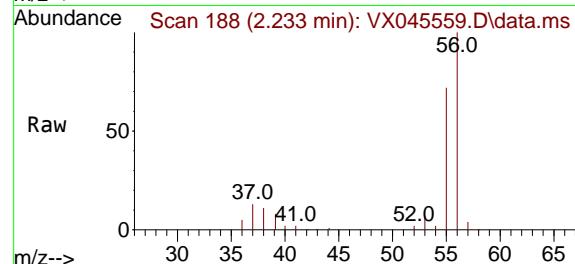

#13

Acrolein

Concen: 290.369 ug/l

RT: 2.233 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:


MSVOA\_X

ClientSampleId :

VSTDCCCC050

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#14

Allyl chloride

Concen: 51.139 ug/l

RT: 2.654 min Scan# 257

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion: 41 Resp: 110918







Ion Ratio Lower Upper

41 100

39 77.2 60.2 90.2

76 30.8 24.6 36.8

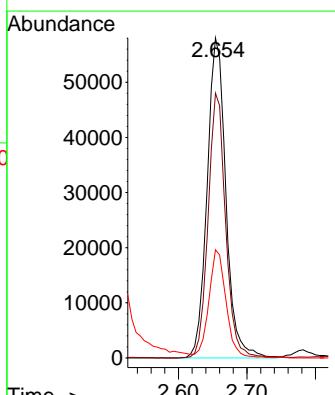

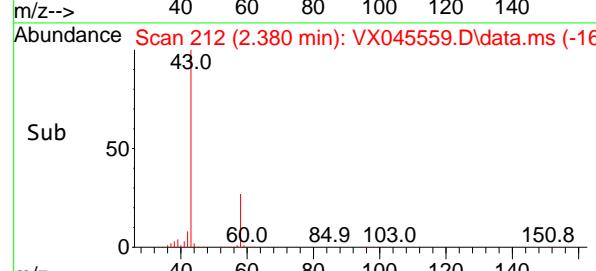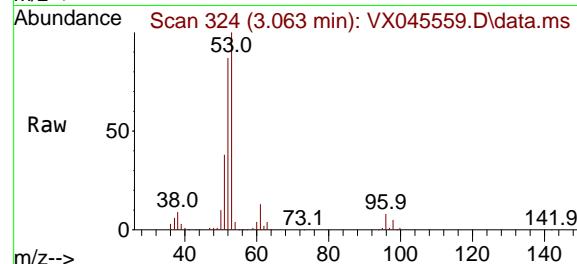

#15

Acrylonitrile

Concen: 251.370 ug/l

RT: 3.063 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

Tgt Ion: 53 Resp: 18569

Ion Ratio Lower Upper

53 100

52 85.8 67.4 101.2


51 38.5 29.9 44.9

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025

Supervised By :Mahesh Dadoda 04/04/2025



#16

Acetone

Concen: 244.836 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30







Tgt Ion: 43 Resp: 175069

Ion Ratio Lower Upper

43 100

58 26.4 22.3 33.5



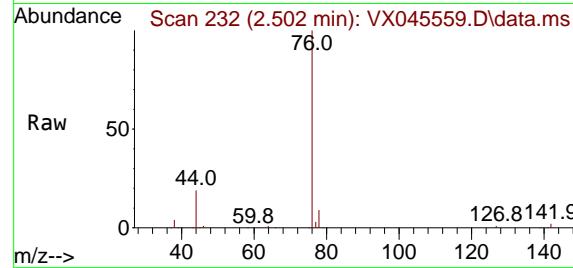

#17

Carbon Disulfide

Concen: 51.779 ug/l

RT: 2.502 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30





Instrument:







MSVOA\_X

ClientSampleId :

VSTDCCCC050

**Manual Integrations  
APPROVED**

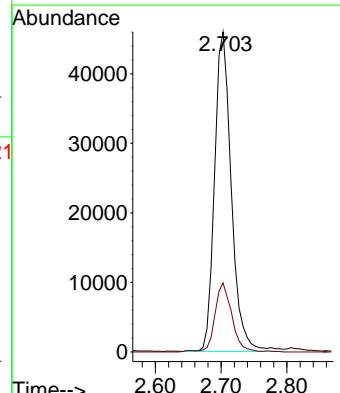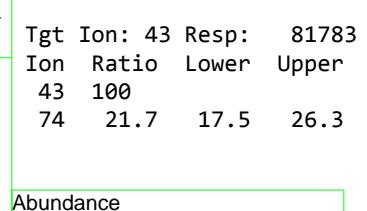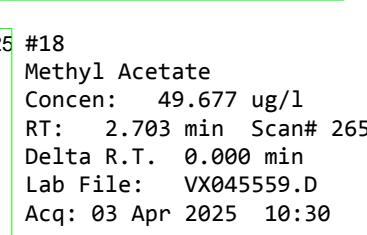 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025




#19

Methyl tert-butyl Ether

Concen: 49.447 ug/l

RT: 3.111 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:


MSVOA\_X

ClientSampleId :

VSTDCCC050

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

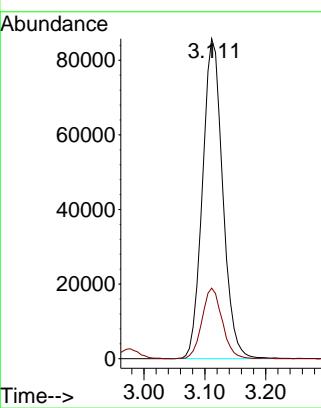

#20

Methylene Chloride

Concen: 49.292 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Tgt Ion: 84 Resp: 65985


Ion Ratio Lower Upper


84 100

49 136.3 107.5 161.3



51 42.2 33.0 49.6

86 65.2 50.1 75.1

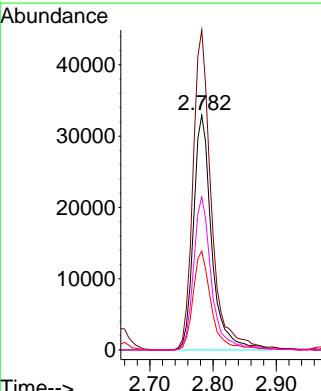




Abundance Scan 327 (3.081 min): VX045559.D\data.ms

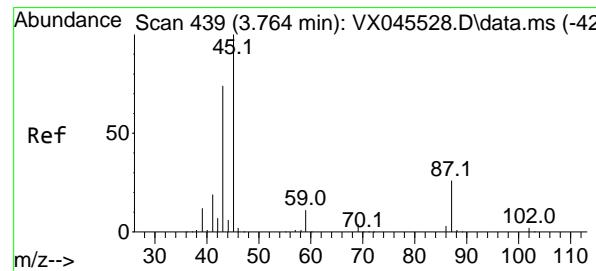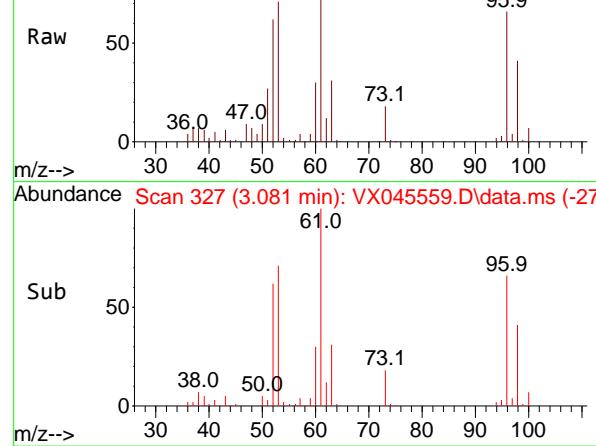

Abundance Scan 438 (3.757 min): VX045559.D\data.ms

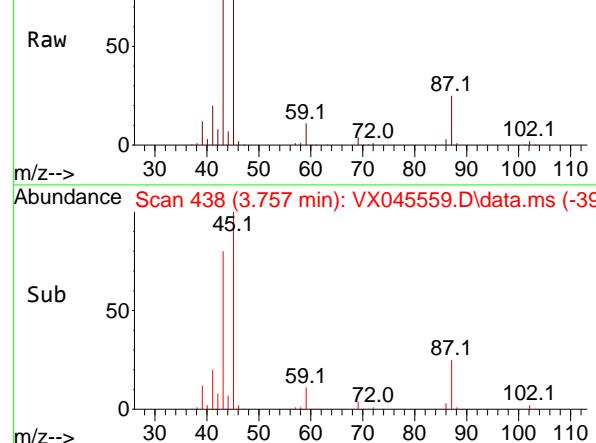

Abundance Scan 438 (3.757 min): VX045559.D\data.ms (-39)

Sub

50

0

45.1

87.1

102.1

72.0

59.1

40

110

#21

trans-1,2-Dichloroethene

Concen: 50.139 ug/l

RT: 3.081 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:


MSVOA\_X

ClientSampleId :

VSTDCCCC050

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#22

Diisopropyl ether

Concen: 50.611 ug/l

RT: 3.757 min Scan# 438

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Tgt Ion: 45 Resp: 216234


Ion Ratio Lower Upper




45 100

43 78.8 59.3 88.9

87 25.1 20.4 30.6

59 11.3 9.0 13.6

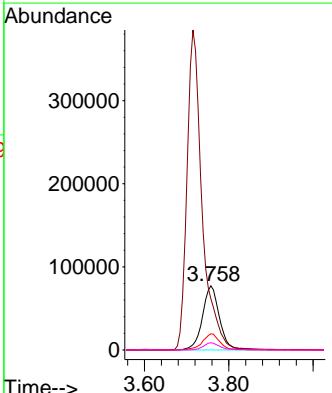

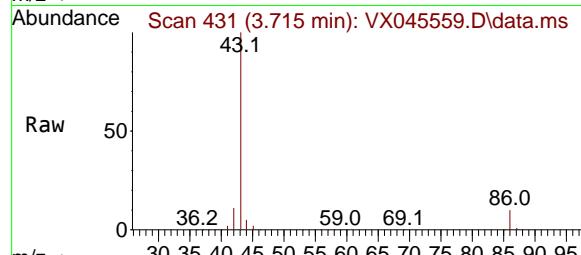

#23

**Vinyl Acetate**

Concen: 261.101 ug/l

RT: 3.715 min Scan# 413

Delta R.T. -0.006 min

Lab File: VX045559.D





Acq: 03 Apr 2025 10:30

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

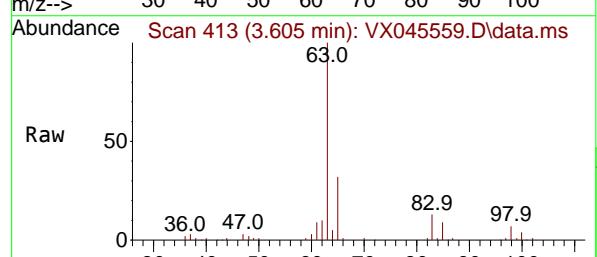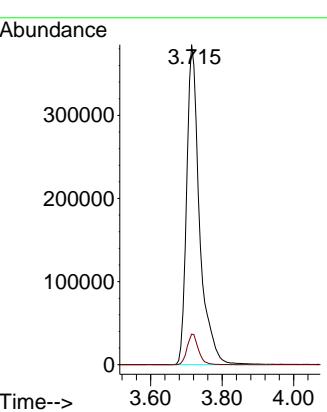**Manual Integrations  
APPROVED**Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

#24

**1,1-Dichloroethane**


Concen: 49.227 ug/l


RT: 3.605 min Scan# 413

Delta R.T. 0.000 min



Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

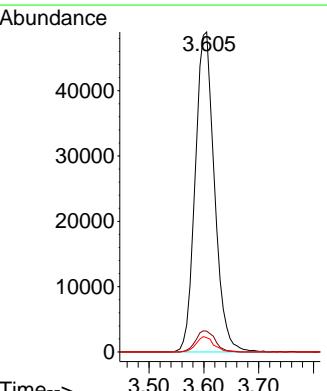
Tgt Ion: 63 Resp: 118946  
Ion Ratio Lower Upper  
63 100  
98 6.5 3.4 10.1  
100 4.5 2.2 6.6

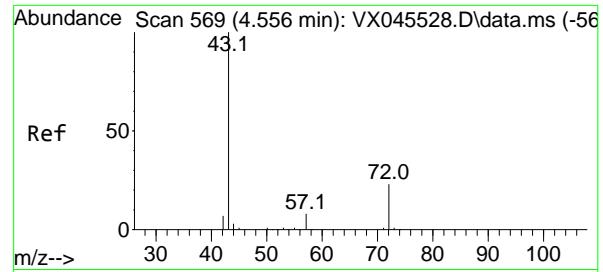

Abundance Scan 568 (4.550 min): VX045559.D\data.ms

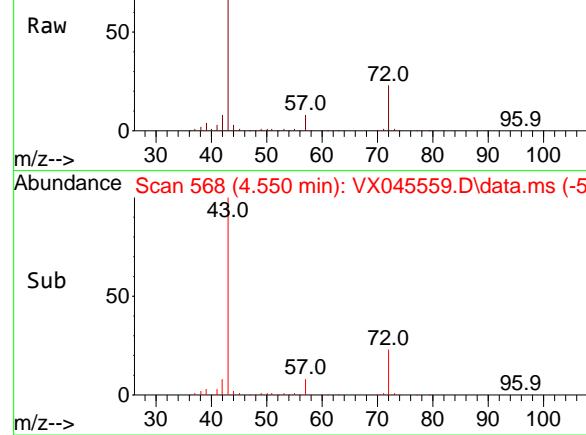

Abundance Scan 554 (4.465 min): VX045559.D\data.ms

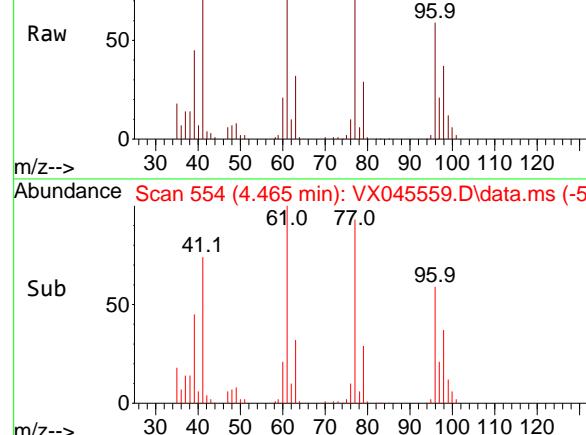

#25

2-Butanone

Concen: 257.055 ug/l

RT: 4.550 min Scan# 5

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#26

2,2-Dichloropropane

Concen: 55.135 ug/l

RT: 4.465 min Scan# 554

Delta R.T. -0.006 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30







Tgt Ion: 77 Resp: 86074

Ion Ratio Lower Upper

77 100

97 21.5 10.6 31.8

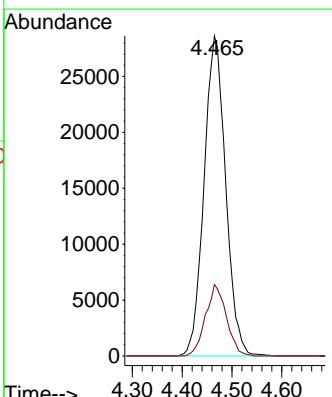




#27  
cis-1,2-Dichloroethene  
Concen: 49.223 ug/l  
RT: 4.477 min Scan# 51  
Delta R.T. -0.006 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025



#28  
Bromochloromethane  
Concen: 48.775 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion: 49 Resp: 56952  
Ion Ratio Lower Upper  
49 100  
129 1.6 0.0 3.8  
130 67.4 54.6 81.8





#29

Tetrahydrofuran

Concen: 250.088 ug/l

RT: 5.001 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

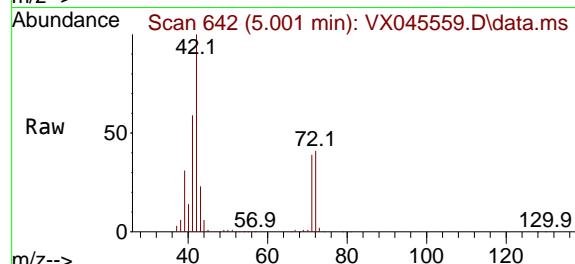

Tgt Ion: 42 Resp: 169709

Ion Ratio Lower Upper

42 100




72 41.8 33.4 50.0

71 38.6 31.4 47.0

**Manual Integrations****APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025

Supervised By :Mahesh Dadoda 04/04/2025



#30

Chloroform




Concen: 49.413 ug/l


RT: 5.087 min Scan# 656

Delta R.T. 0.000 min



Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

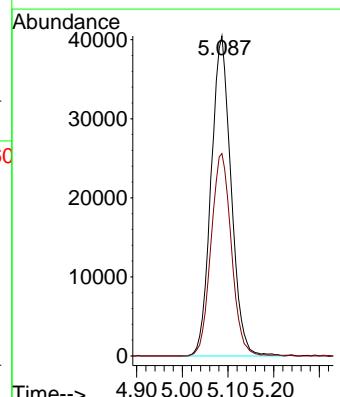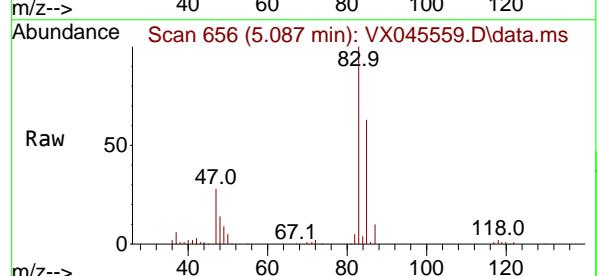



Abundance Scan 717 (5.458 min): VX045559.D\data.ms

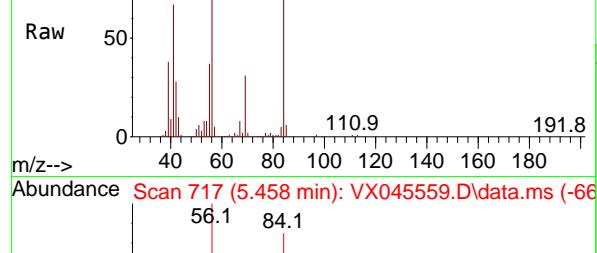

#31

Cyclohexane

Concen: 50.618 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30



Instrument:

MSVOA\_X



ClientSampleId :

VSTDCCCC050

**Manual Integrations  
APPROVED**

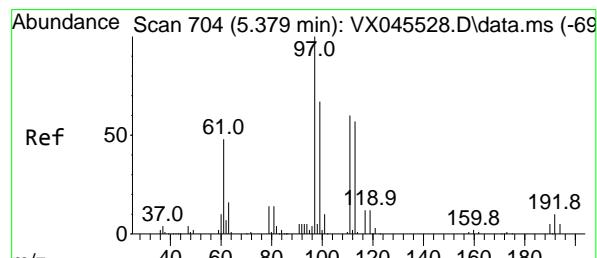 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


Abundance Scan 703 (5.373 min): VX045559.D\data.ms

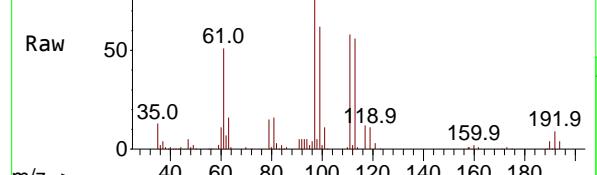

#32

1,1,1-Trichloroethane

Concen: 50.002 ug/l

RT: 5.373 min Scan# 703

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion: 97 Resp: 105194


Ion Ratio Lower Upper

97 100





99 64.1 51.7 77.5

61 52.9 41.0 61.4

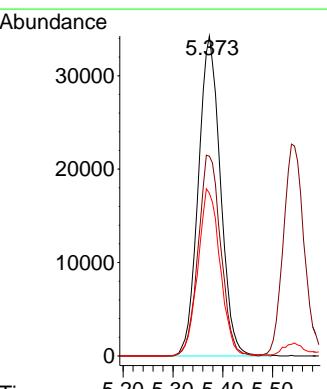



Abundance Scan 797 (5.946 min): VX045559.D\data.ms

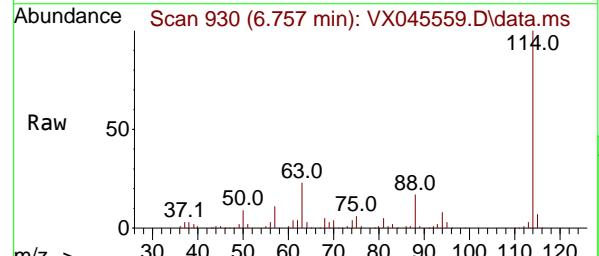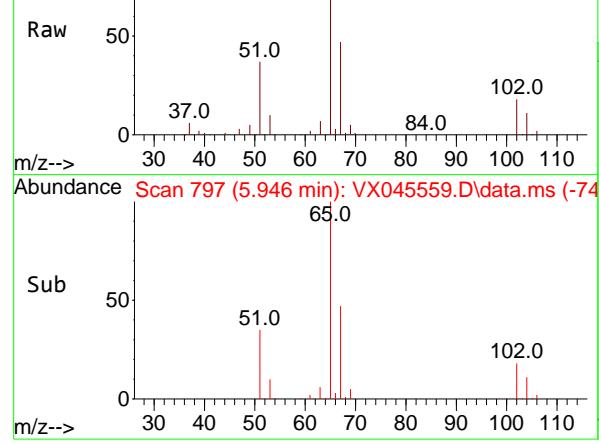

#33

1,2-Dichloroethane-d4

Concen: 48.452 ug/l

RT: 5.946 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:


MSVOA\_X

ClientSampleId :

VSTDCCCC050

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion:114 Resp: 162684







Ion Ratio Lower Upper

114 100

63 23.3 0.0 46.8

88 17.0 0.0 35.4

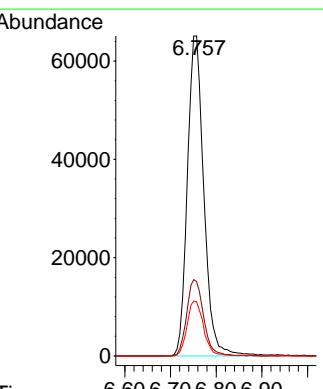



#35

Dibromofluoromethane

Concen: 50.400 ug/l

RT: 5.379 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:


MSVOA\_X

ClientSampleId :

VSTDCCCC050

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#36

1,1-Dichloropropene

Concen: 51.889 ug/l

RT: 5.684 min Scan# 754

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion: 75 Resp: 80867


Ion Ratio Lower Upper

75 100



110 33.3 16.9 50.6

77 31.4 25.0 37.4

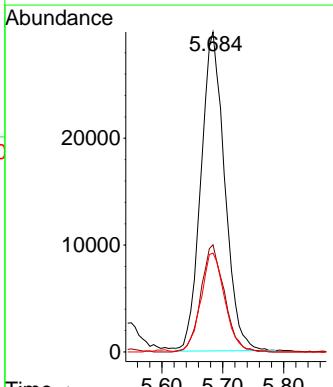




Abundance Scan 594 (4.709 min): VX045559.D\data.ms

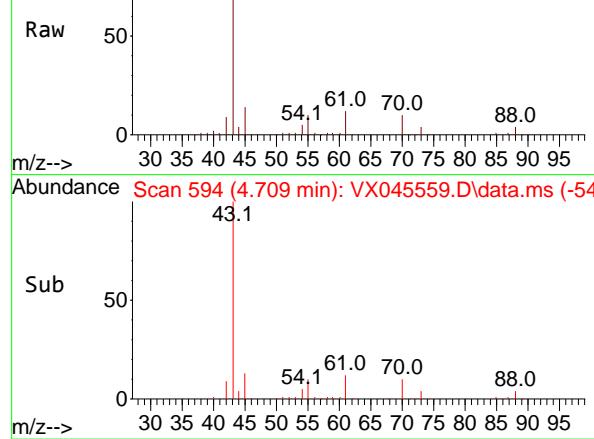

Abundance Scan 751 (5.666 min): VX045559.D\data.ms

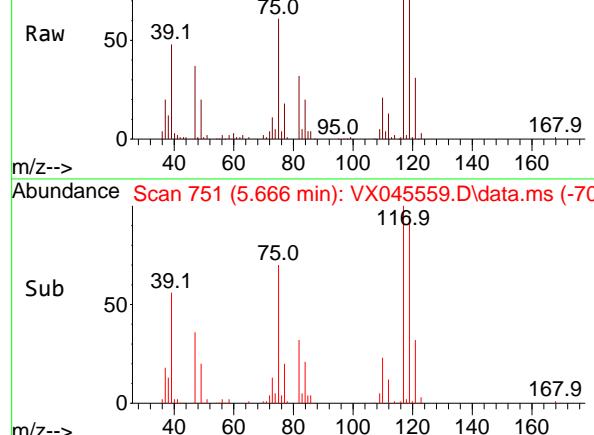

Abundance Scan 751 (5.666 min): VX045559.D\data.ms (-70)

Sub

m/z-->

#37

Ethyl Acetate

Concen: 50.922 ug/l

RT: 4.709 min Scan# 5

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#38

Carbon Tetrachloride

Concen: 54.175 ug/l

RT: 5.666 min Scan# 751

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion:117 Resp: 91247


Ion Ratio Lower Upper

117 100

119 93.8 76.9 115.3

121 31.2 24.2 36.2

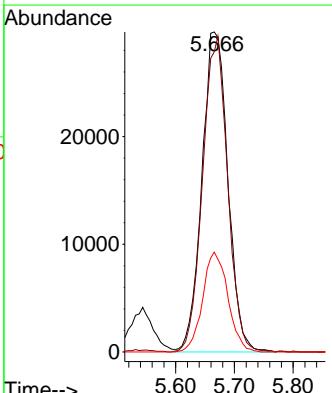

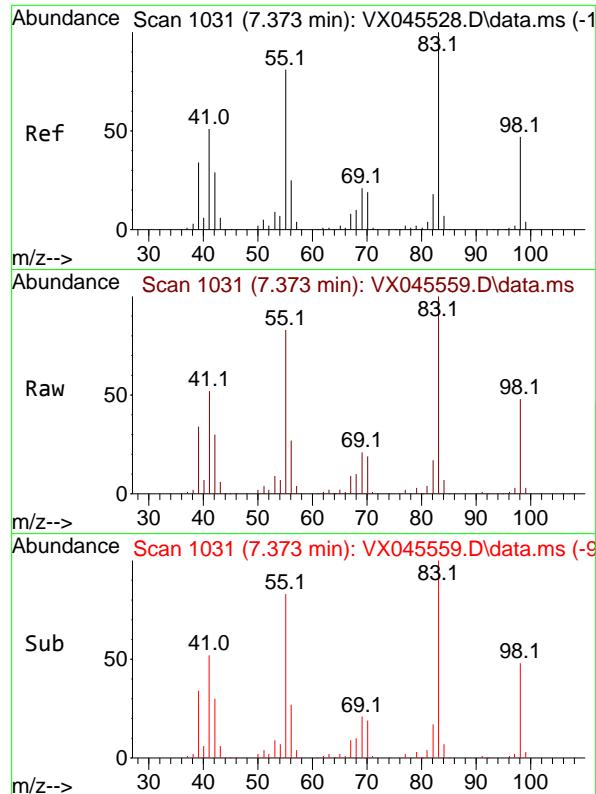

#39

Methylcyclohexane

Concen: 55.811 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

Tgt Ion: 83 Resp: 106620

Ion Ratio Lower Upper

83 100



55 82.7 64.9 97.3

98 48.4 37.4 56.0

**Manual Integrations  
APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025

Supervised By :Mahesh Dadoda 04/04/2025

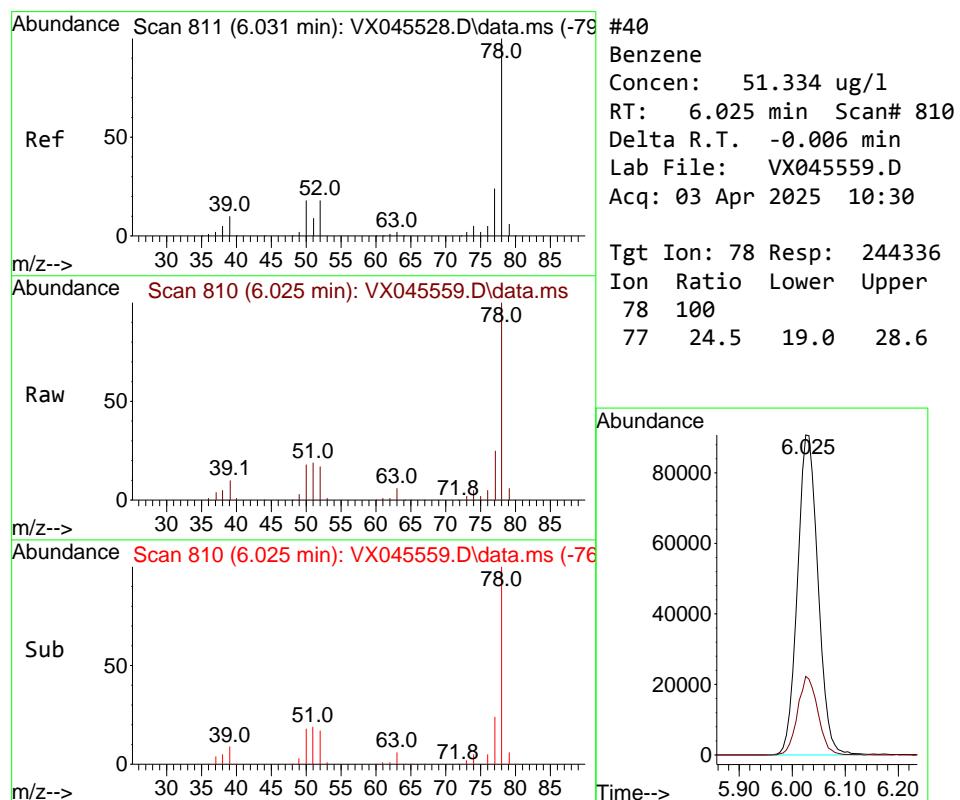

#40

Benzene

Concen: 51.334 ug/l

RT: 6.025 min Scan# 810

Delta R.T. -0.006 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30


Tgt Ion: 78 Resp: 244336

Ion Ratio Lower Upper





78 100

77 24.5 19.0 28.6

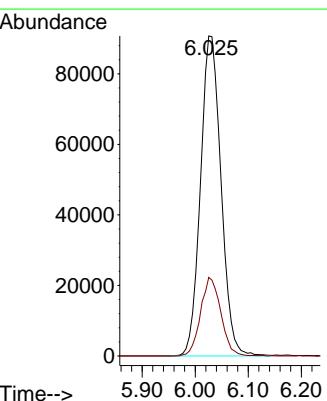



Abundance Scan 627 (4.910 min): VX045559.D\data.ms

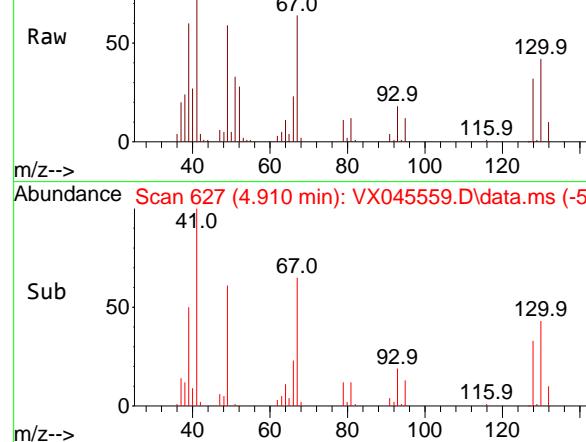

#41

Methacrylonitrile

Concen: 53.895 ug/l

RT: 4.910 min Scan# 6





Delta R.T. -0.012 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X

ClientSampleId : VSTDCCC050

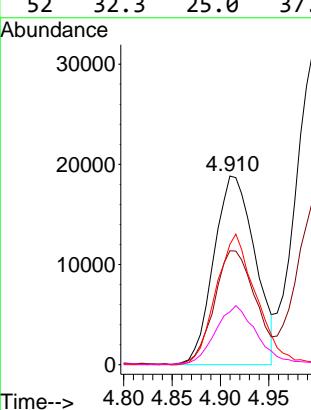**Manual Integrations  
APPROVED**
Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

#42

1,2-Dichloroethane


Concen: 52.471 ug/l


RT: 6.080 min Scan# 819

Delta R.T. 0.000 min



Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

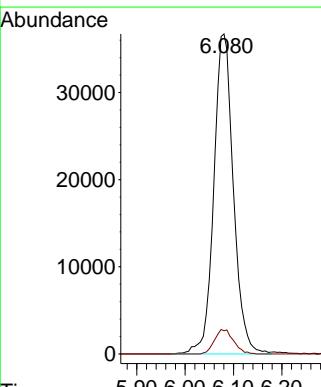
Tgt Ion: 62 Resp: 103151  
Ion Ratio Lower Upper  
62 100  
98 7.4 0.0 15.2



Abundance Scan 861 (6.336 min): VX045559.D\data.ms

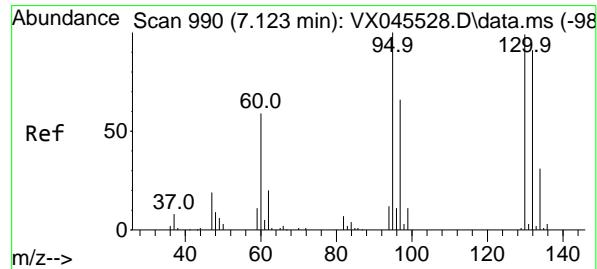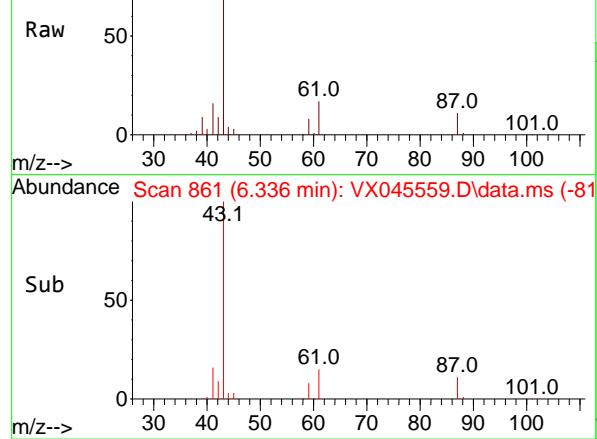

Abundance Scan 989 (7.117 min): VX045559.D\data.ms

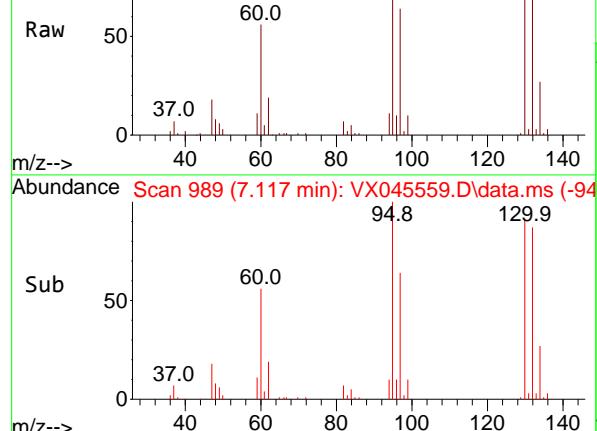

#43

Isopropyl Acetate

Concen: 53.203 ug/l

RT: 6.336 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#44

Trichloroethene

Concen: 50.400 ug/l

RT: 7.117 min Scan# 989

Delta R.T. -0.006 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30




Tgt Ion:130 Resp: 57018

Ion Ratio Lower Upper

130 100

95 109.9 0.0 202.0

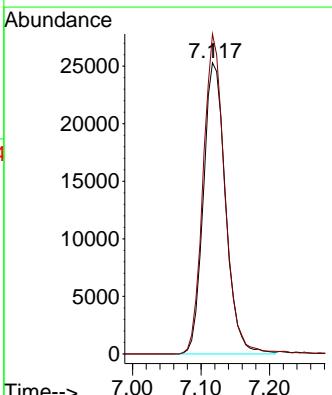



#45

1,2-Dichloropropane

Concen: 52.177 ug/l

RT: 7.421 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30





Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

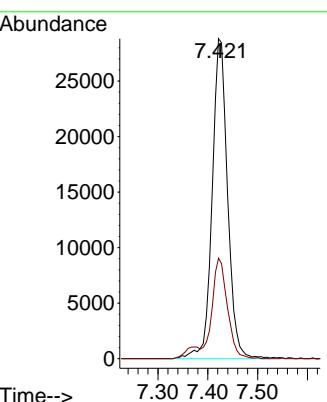 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#46

Dibromomethane


Concen: 52.432 ug/l




RT: 7.574 min Scan# 1064

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

 Tgt Ion: 93 Resp: 47799  
 Ion Ratio Lower Upper  
 93 100  
 95 81.2 64.8 97.2  
 174 82.5 65.4 98.0




#47

Bromodichloromethane

Concen: 53.281 ug/l

RT: 7.818 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30




Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#48

Methyl methacrylate

Concen: 53.916 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion: 41 Resp: 82864


Ion Ratio Lower Upper

41 100



69 72.4 58.2 87.2

39 64.9 53.6 80.4

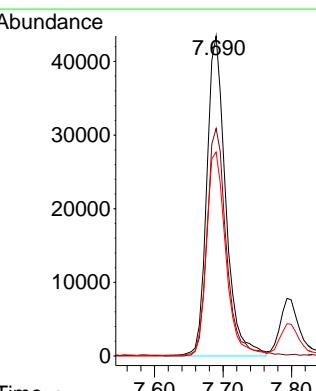




Abundance Scan 1077 (7.653 min): VX045559.D\data.ms

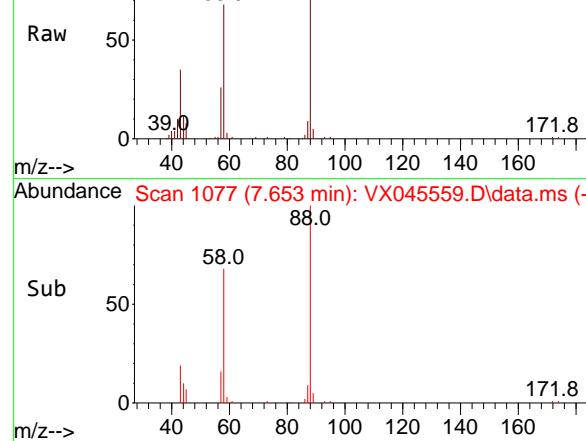

Abundance Scan 1240 (8.647 min): VX045559.D\data.ms

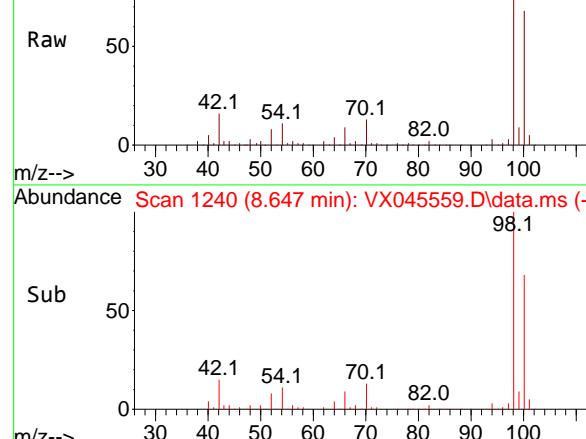

#49

1,4-Dioxane

Concen: 1069.810 ug/l

RT: 7.653 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:


MSVOA\_X

ClientSampleId :

VSTDCCCC050

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

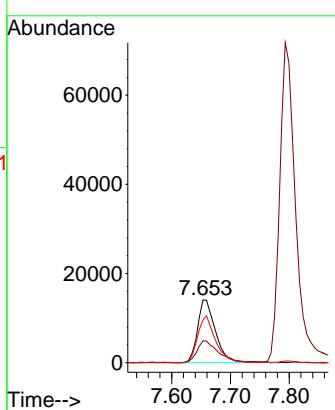

#50

Toluene-d8

Concen: 50.412 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30


Tgt Ion: 98 Resp: 203099

Ion Ratio Lower Upper


98 100

100 66.4 52.2 78.4

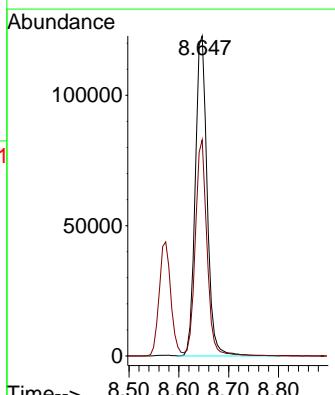




Abundance Scan 1227 (8.568 min): VX045559.D\data.ms

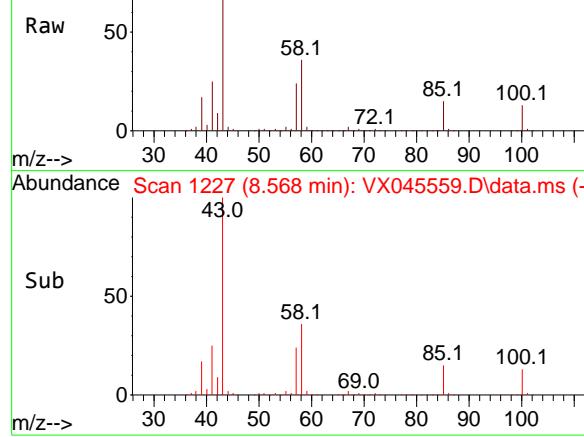

Abundance Scan 1227 (8.568 min): VX045559.D\data.ms (-1)

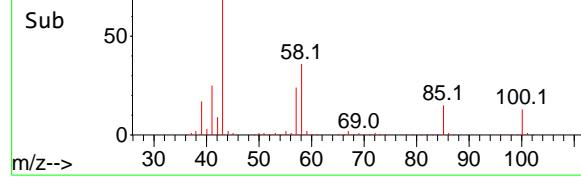

#51

4-Methyl-2-Pentanone

Concen: 271.376 ug/l

RT: 8.568 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:

MSVOA\_X

ClientSampleId :



VSTDCCC050

Tgt Ion: 43 Resp: 535504


Ion Ratio Lower Upper

43 100


58 35.2 28.5 42.7

**Manual Integrations  
APPROVED**Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

Abundance Scan 1251 (8.714 min): VX045559.D\data.ms

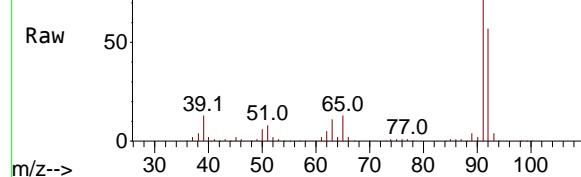

Abundance Scan 1251 (8.714 min): VX045559.D\data.ms (-1)

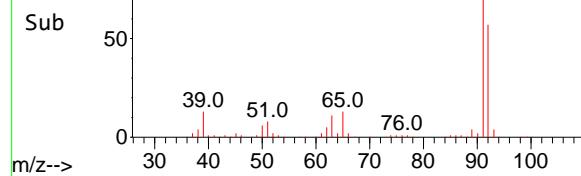

#52

Toluene

Concen: 51.038 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30




Tgt Ion: 92 Resp: 146995

Ion Ratio Lower Upper

92 100

91 176.0 138.7 208.1





#53

t-1,3-Dichloropropene

Concen: 48.265 ug/l

RT: 8.976 min Scan# 1294

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30




Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

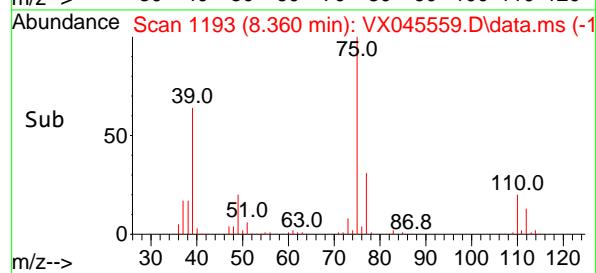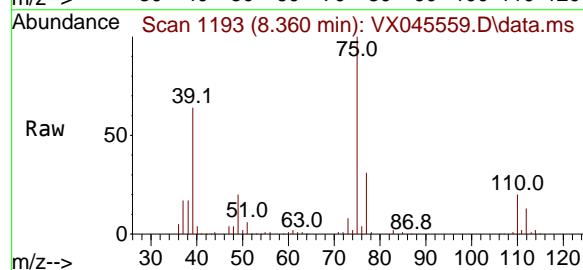 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#54

cis-1,3-Dichloropropene

Concen: 55.553 ug/l

RT: 8.360 min Scan# 1193

Delta R.T. -0.006 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion: 75 Resp: 95044




Ion Ratio Lower Upper

75 100

77 31.3 24.6 36.8

39 64.2 48.4 72.6

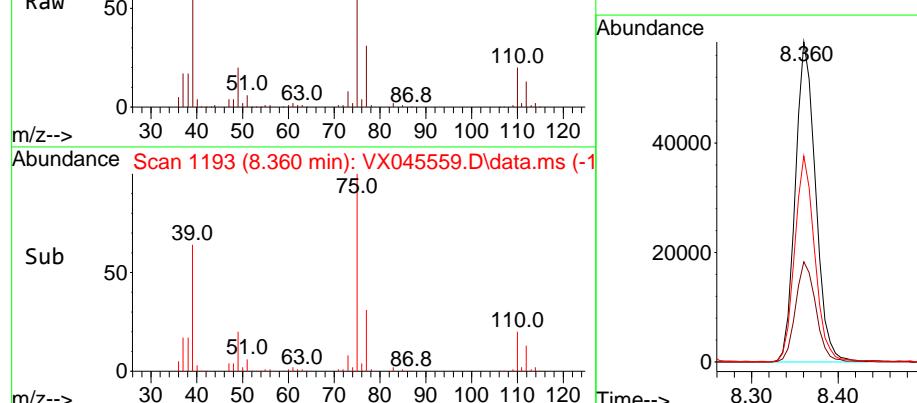

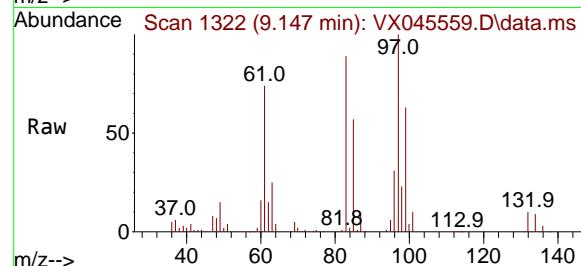

#55

1,1,2-Trichloroethane

Concen: 51.988 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30




Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

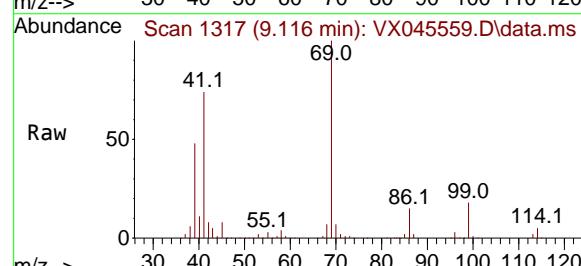 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#56

Ethyl methacrylate

Concen: 54.916 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion: 69 Resp: 97540




Ion Ratio Lower Upper

69 100

41 76.6 61.3 91.9

39 50.3 40.2 60.2

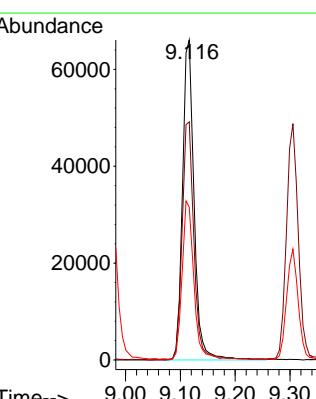



#57

1,3-Dichloropropane

Concen: 51.465 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30





Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

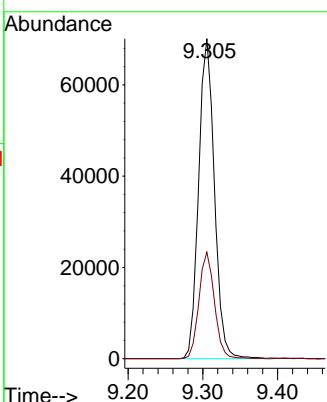 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#58

2-Chloroethyl Vinyl ether

Concen: 278.463 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. 0.000 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30


Tgt Ion: 63 Resp: 250203

Ion Ratio Lower Upper

63 100


106 26.5 21.0 31.6

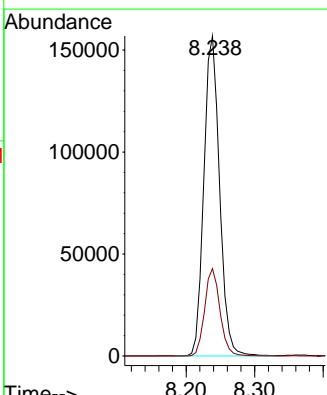



#59  
2-Hexanone  
Concen: 266.003 ug/l  
RT: 9.427 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30




Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050




Tgt Ion: 43 Resp: 38870  
Ion Ratio Lower Upper  
43 100  
58 49.6 24.9 74.6

### Manual Integrations APPROVED



Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025


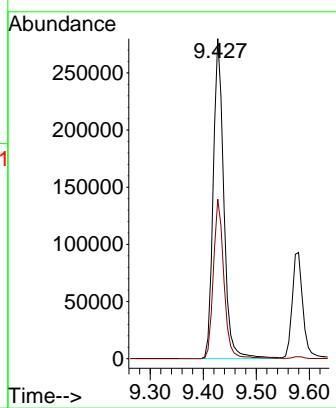
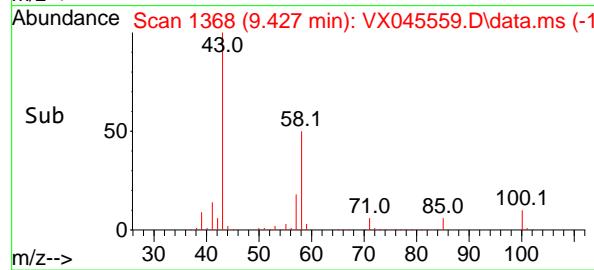


#60  
Dibromochloromethane  
Concen: 54.791 ug/l  
RT: 9.519 min Scan# 1383  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30



Tgt Ion:129 Resp: 68554  
Ion Ratio Lower Upper  
129 100  
127 76.9 39.4 118.2

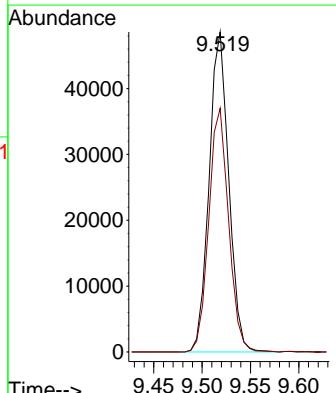



#61

1,2-Dibromoethane

Concen: 52.982 ug/l

RT: 9.604 min Scan# 1397

Delta R.T. 0.000 min





Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument: MSVOA\_X

ClientSampleId: VSTDCCC050

**Manual Integrations  
APPROVED**

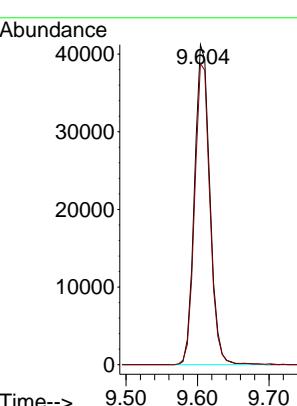 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#62

4-Bromofluorobenzene


Concen: 51.040 ug/l


RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

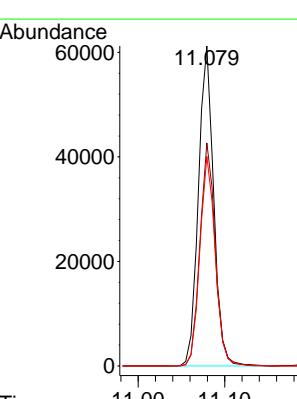 Tgt Ion: 95 Resp: 74900  
 Ion Ratio Lower Upper  
 95 100  
 174 69.5 0.0 135.8  
 176 66.0 0.0 131.4

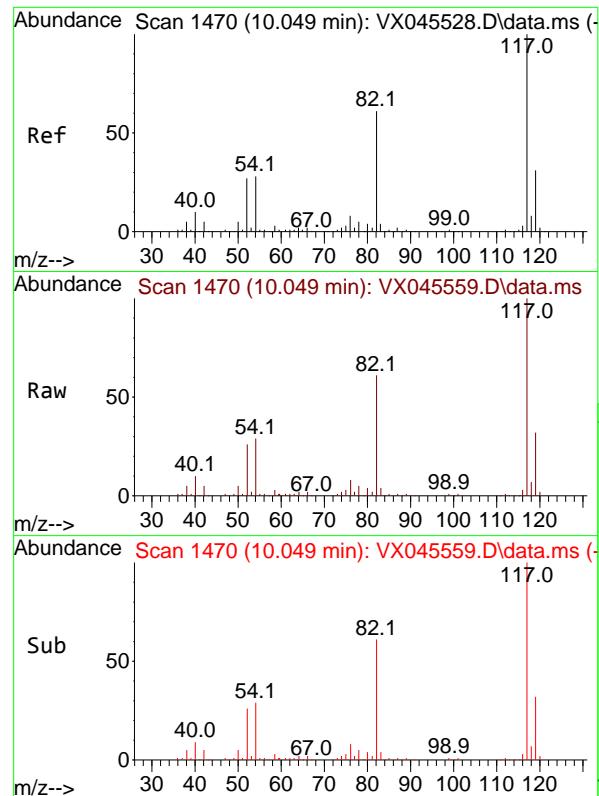
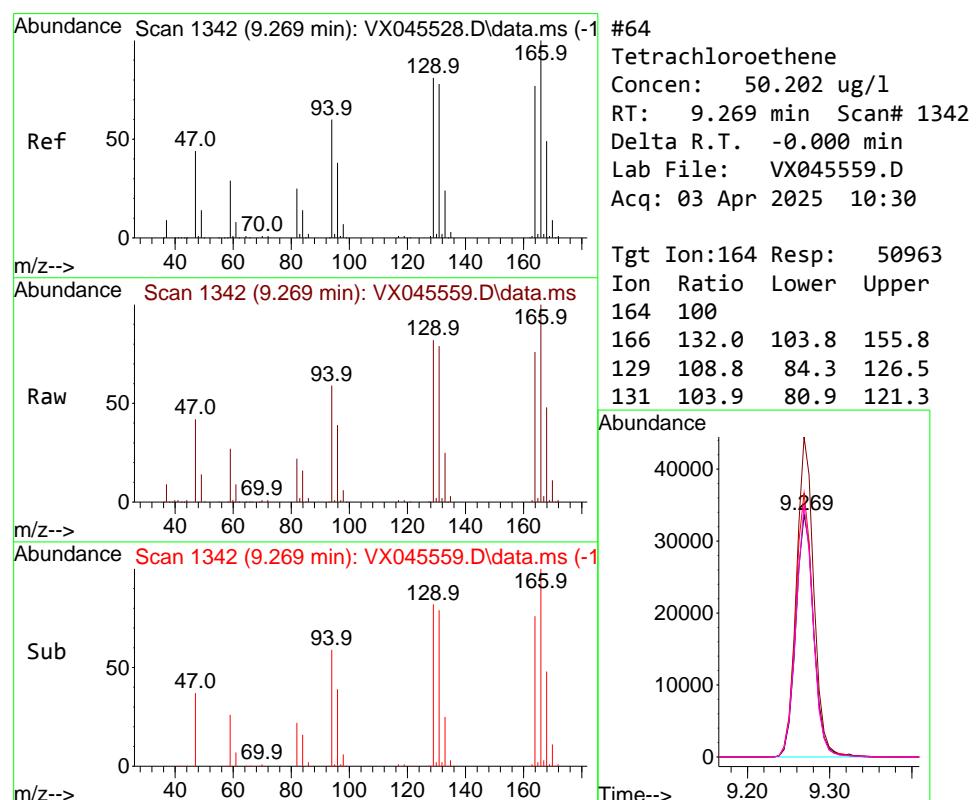



#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1470  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025



#64  
Tetrachloroethene  
Concen: 50.202 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion:164 Resp: 50963  
Ion Ratio Lower Upper  
164 100  
166 132.0 103.8 155.8  
129 108.8 84.3 126.5  
131 103.9 80.9 121.3

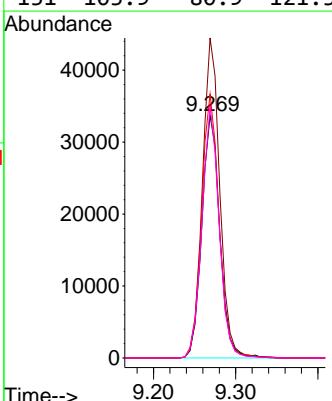


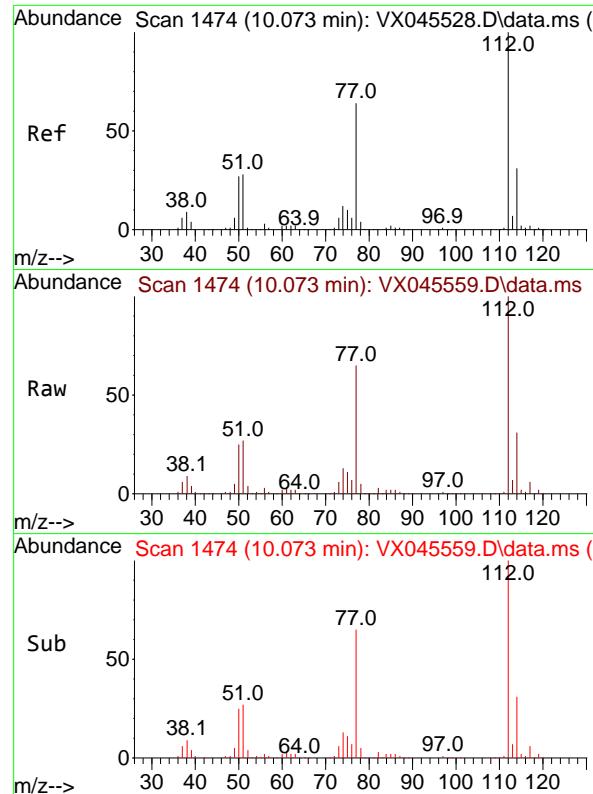


#65  
Chlorobenzene  
Concen: 52.511 ug/l  
RT: 10.073 min Scan# 1474  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


**Manual Integrations APPROVED**







Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

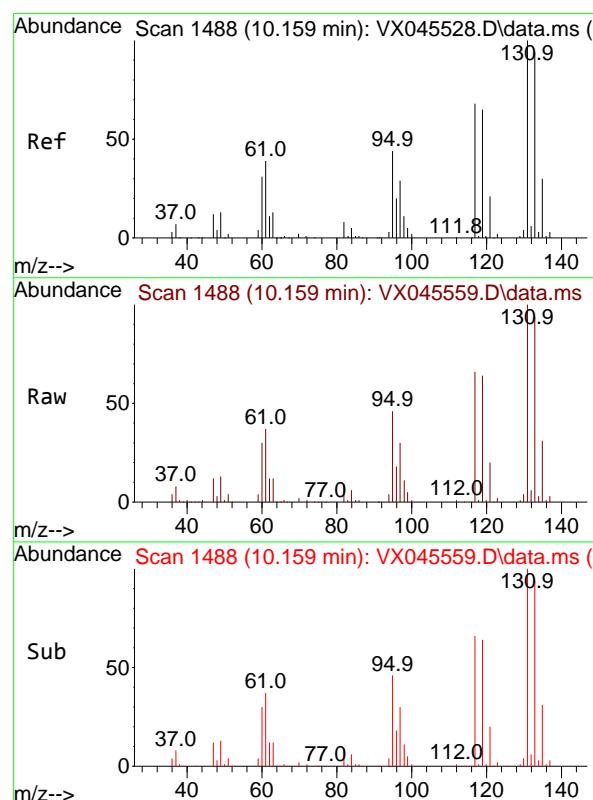

#66  
1,1,1,2-Tetrachloroethane  
Concen: 51.757 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion:131 Resp: 55208  
Ion Ratio Lower Upper  
131 100  
133 95.3 47.5 142.5  
119 64.8 32.9 98.6

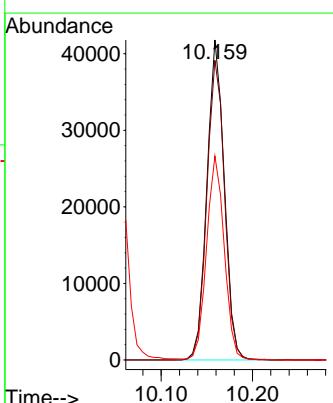



#67

Ethyl Benzene

Concen: 53.122 ug/l

RT: 10.189 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:


MSVOA\_X

ClientSampleId :

VSTDCCCC050

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#68

m/p-Xylenes

Concen: 106.687 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30




Tgt Ion:106 Resp: 213521

Ion Ratio Lower Upper

106 100

91 218.5 172.6 258.8









#69  
o-Xylene  
Concen: 53.092 ug/l  
RT: 10.640 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


Manual Integrations  
**APPROVED**







Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

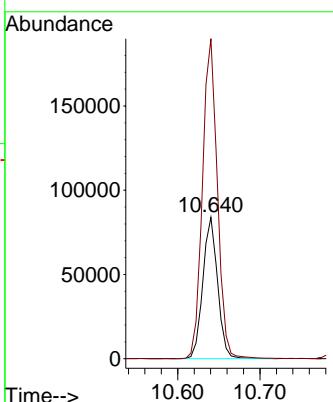

#70  
Styrene  
Concen: 54.847 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion:104 Resp: 178474  
Ion Ratio Lower Upper  
104 100  
78 57.4 45.4 68.2  
103 54.8 43.8 65.8





#71

Bromoform

Concen: 54.761 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument:


MSVOA\_X

ClientSampleId :

VSTDCCC050

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

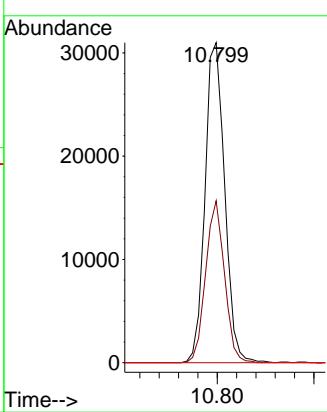

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion:152 Resp: 66270


Ion Ratio Lower Upper

152 100

115 96.4 46.9 140.7

150 174.6 0.0 349.4



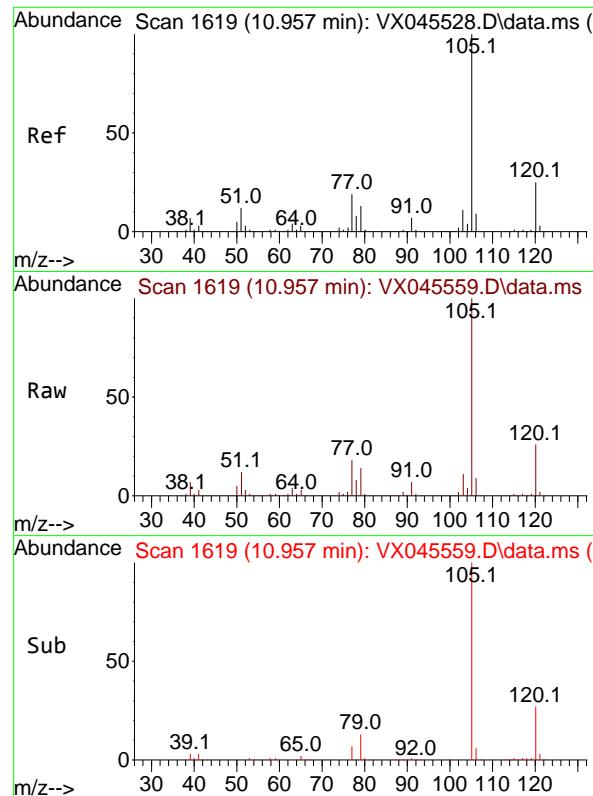

#73

Isopropylbenzene

Concen: 52.752 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

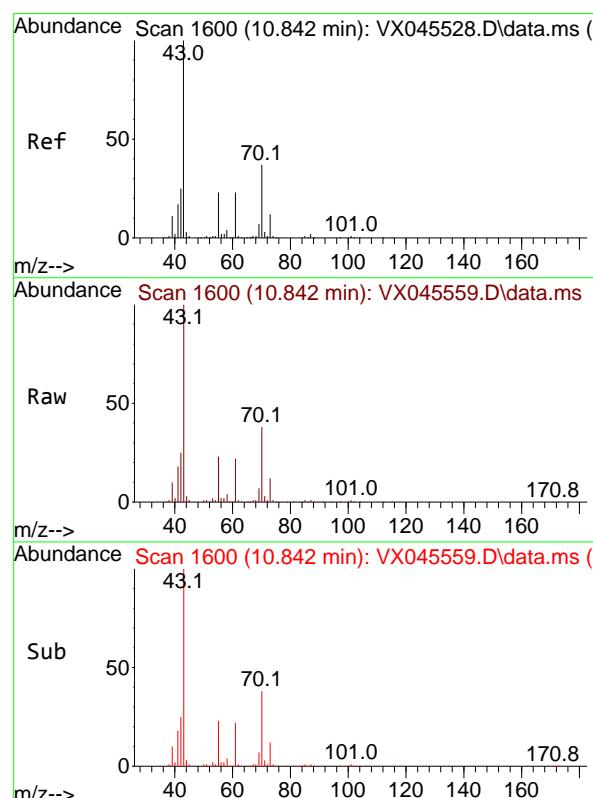 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#74

N-amyl acetate

Concen: 51.953 ug/l

RT: 10.842 min Scan# 1600

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Tgt Ion: 43 Resp: 131921


Ion Ratio Lower Upper


43 100

70 37.5 30.1 45.1

55 23.2 18.3 27.5

61 21.7 17.5 26.3

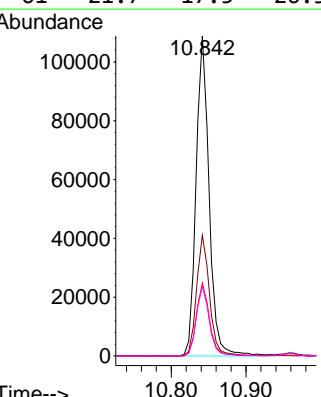

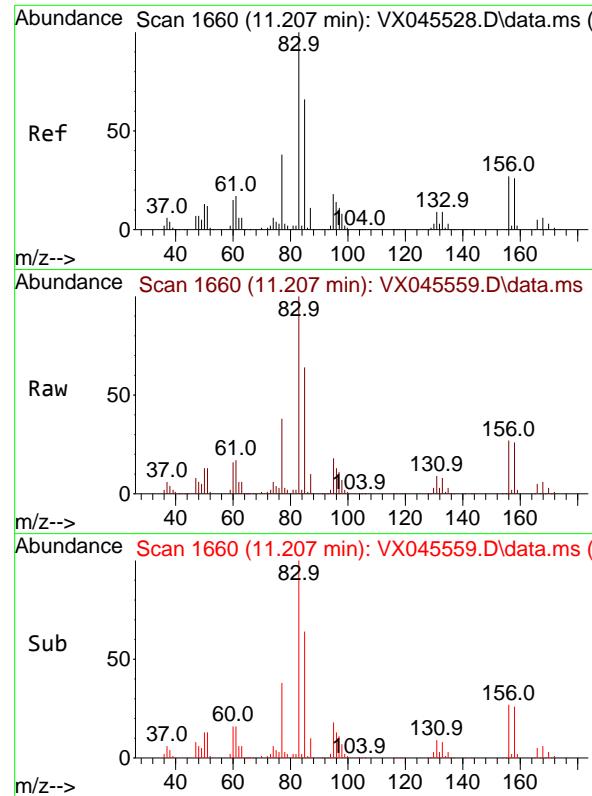


#75  
1,1,2,2-Tetrachloroethane  
Concen: 48.351 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


**Manual Integrations**  
**APPROVED**




Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

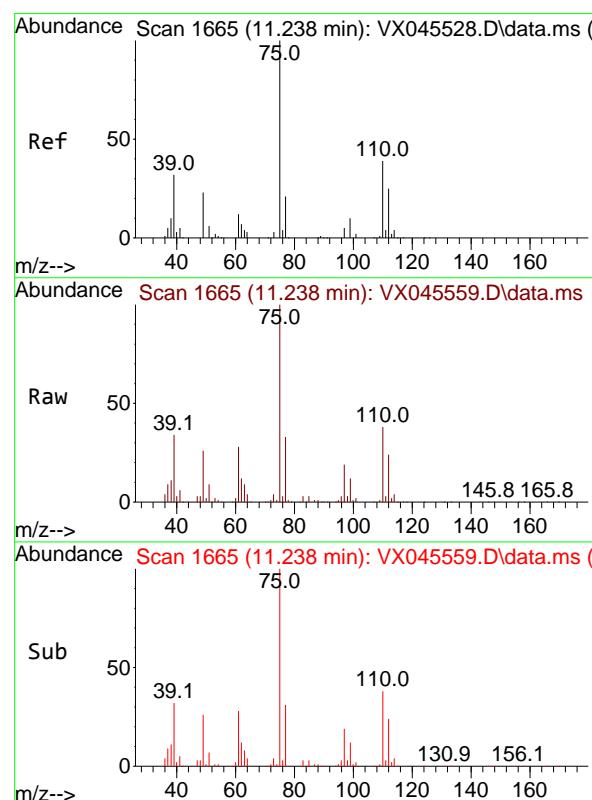

#76  
1,2,3-Trichloropropane  
Concen: 49.735 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion: 75 Resp: 80395  
Ion Ratio Lower Upper  
75 100  
77 40.6 20.0 59.9

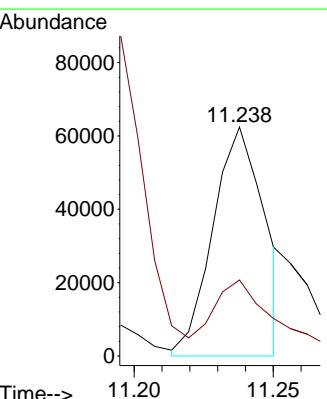

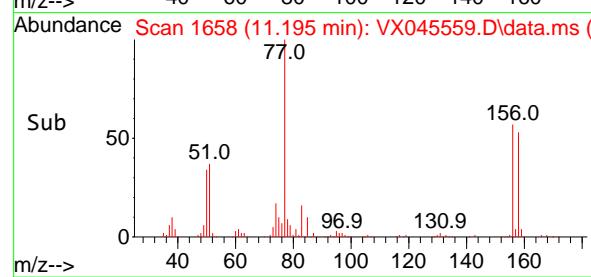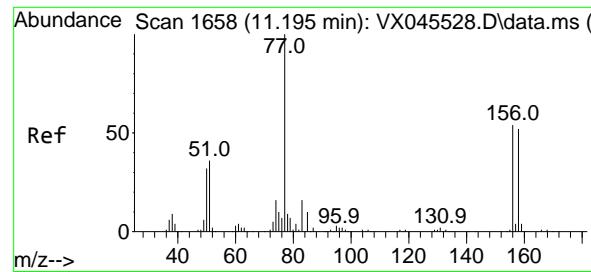

#77

Bromobenzene

Concen: 51.347 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30





Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations**  
**APPROVED**

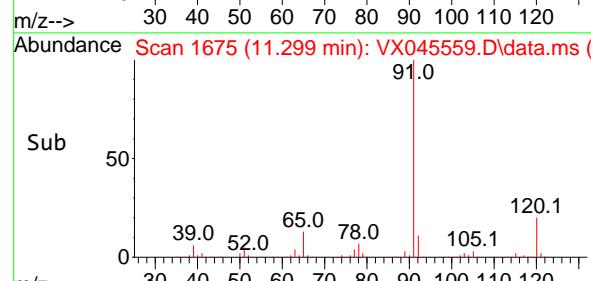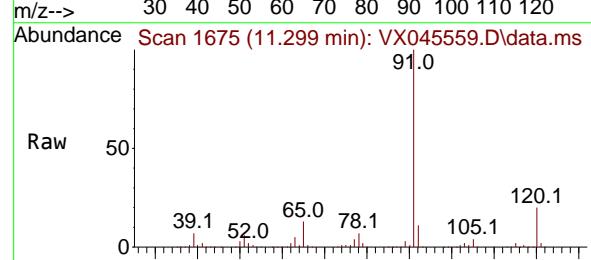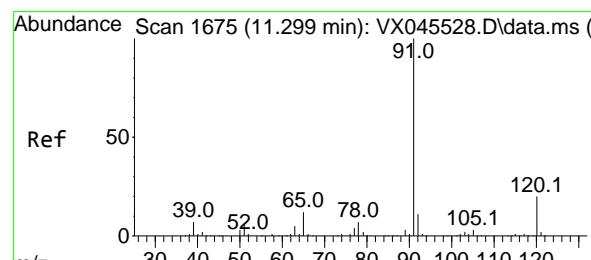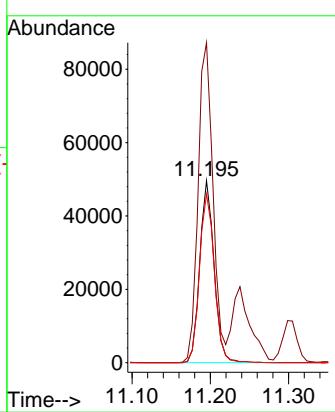 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#78

n-propylbenzene


Concen: 54.023 ug/l




RT: 11.299 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

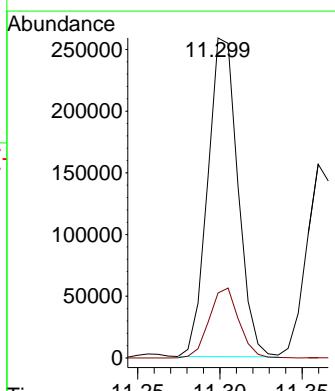 Tgt Ion: 91 Resp: 330313  
 Ion Ratio Lower Upper  
 91 100  
 120 21.6 10.8 32.3




#79

2-Chlorotoluene

Concen: 51.521 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30




Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#80

1,3,5-Trimethylbenzene

Concen: 54.195 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30


Tgt Ion:105 Resp: 237889

Ion Ratio Lower Upper

105 100

120 45.6 23.0 69.0

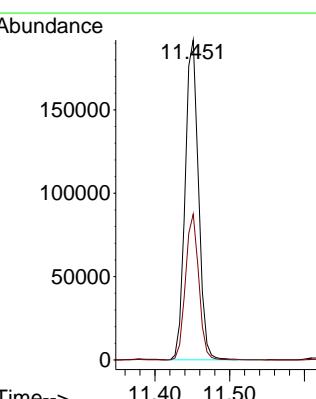


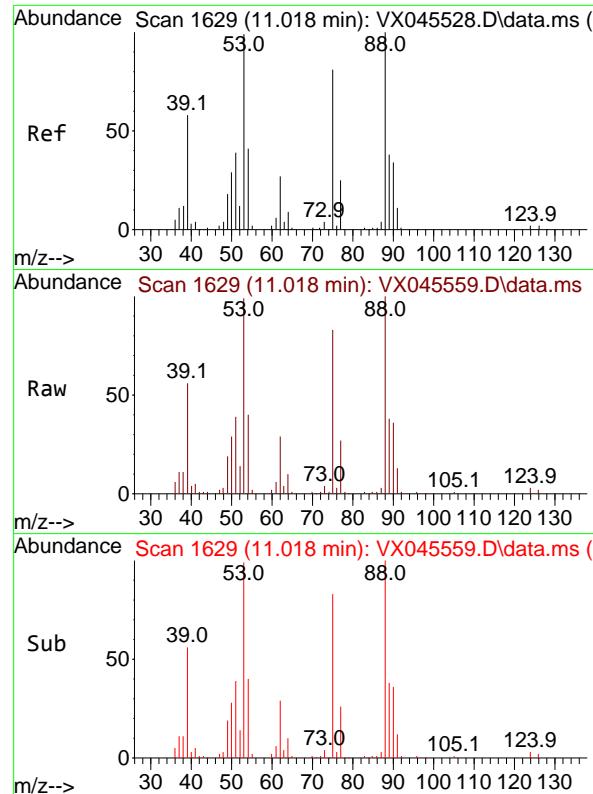


#81  
trans-1,4-Dichloro-2-butene  
Concen: 52.613 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED







Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

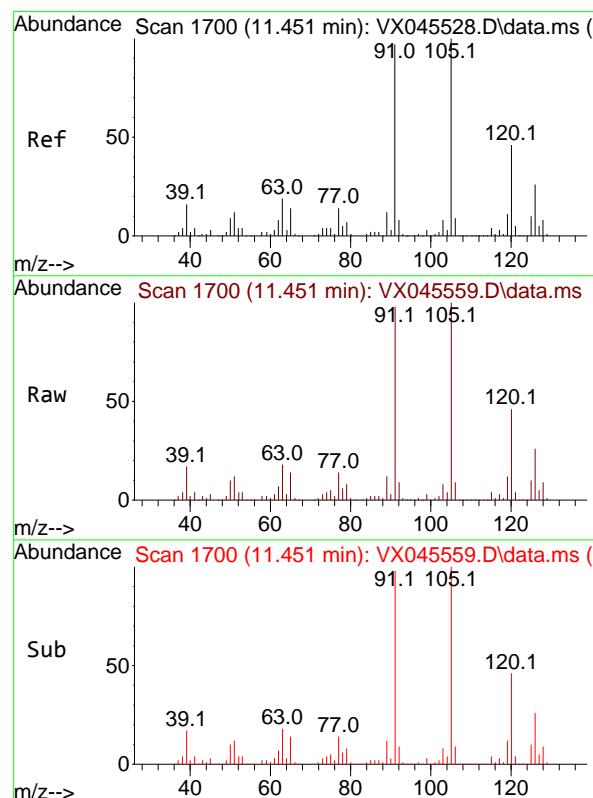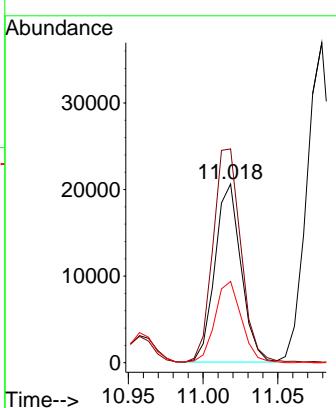

#82  
4-Chlorotoluene  
Concen: 53.158 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion: 91 Resp: 231669  
Ion Ratio Lower Upper  
91 100  
126 27.1 13.3 39.9

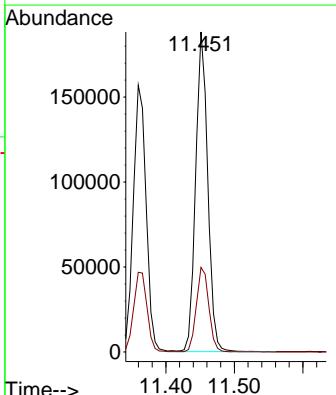



#83

tert-Butylbenzene

Concen: 53.394 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#84

1,2,4-Trimethylbenzene

Concen: 54.063 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045559.D


Acq: 03 Apr 2025 10:30




Tgt Ion:105 Resp: 238183

Ion Ratio Lower Upper

105 100

120 42.7 21.4 64.3

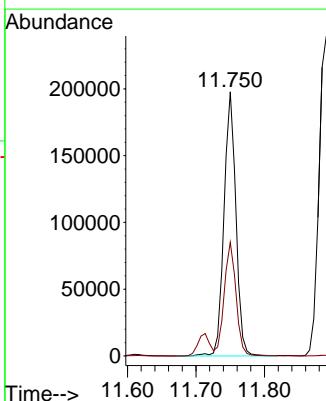



#85

sec-Butylbenzene

Concen: 54.862 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30




Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#86

p-Isopropyltoluene

Concen: 54.914 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30


Tgt Ion:119 Resp: 241650


Ion Ratio Lower Upper

119 100

134 25.1 12.6 37.8

91 27.4 13.7 41.1

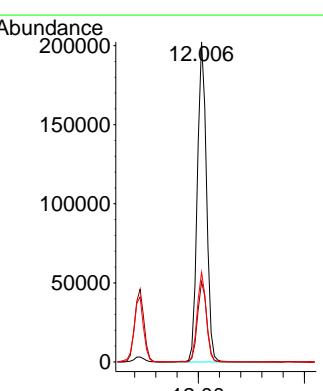


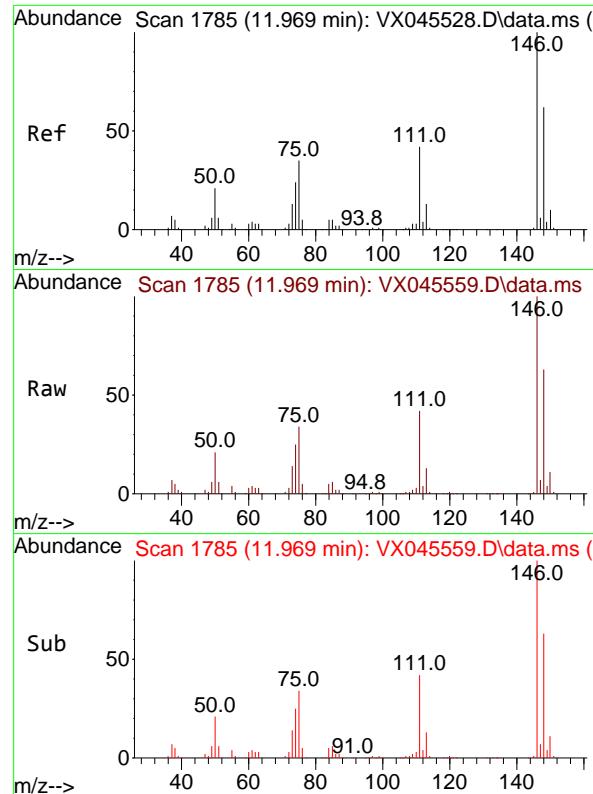


#87  
1,3-Dichlorobenzene  
Concen: 51.187 ug/l  
RT: 11.969 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED




Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

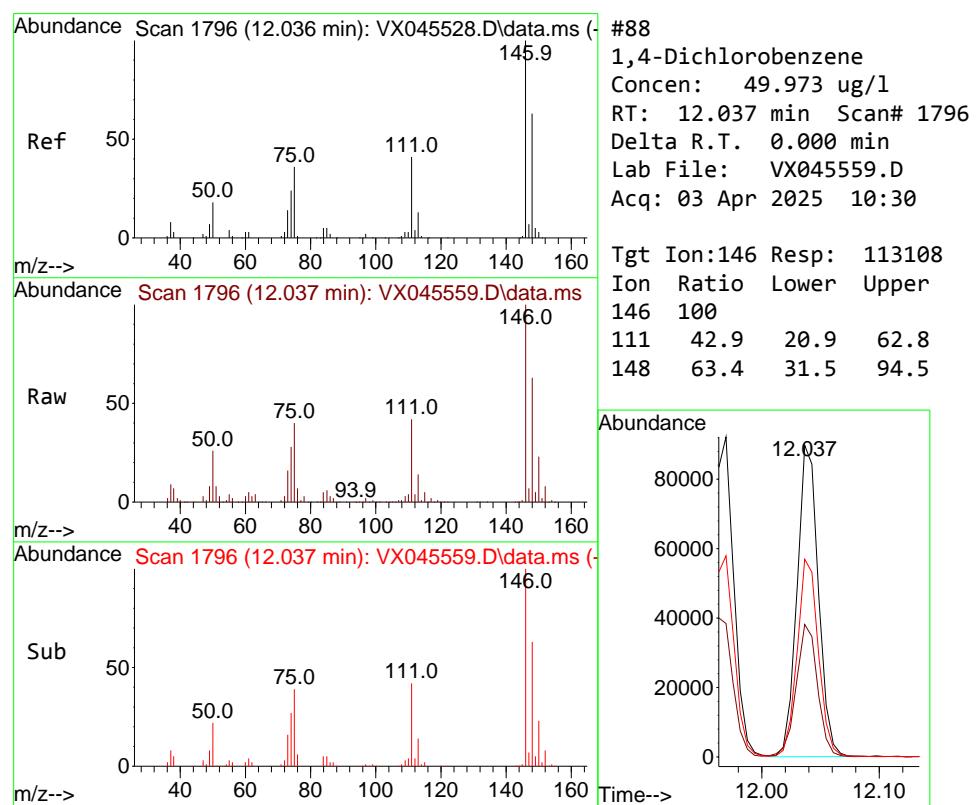

#88  
1,4-Dichlorobenzene  
Concen: 49.973 ug/l  
RT: 12.037 min Scan# 1796  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion:146 Resp: 113108  
Ion Ratio Lower Upper  
146 100  
111 42.9 20.9 62.8  
148 63.4 31.5 94.5





#89

n-Butylbenzene

Concen: 57.188 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30





Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#90

Hexachloroethane


Concen: 55.591 ug/l




RT: 12.536 min Scan# 1878

Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

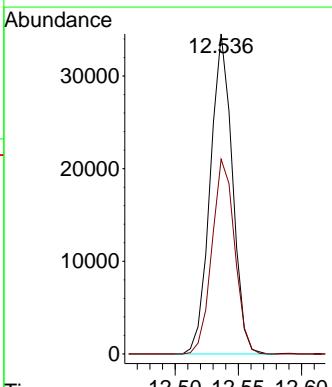 Tgt Ion:117 Resp: 42042  
 Ion Ratio Lower Upper  
 117 100  
 201 62.4 31.2 93.6




#91

1,2-Dichlorobenzene

Concen: 50.437 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min





Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X

ClientSampleId : VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#92

1,2-Dibromo-3-Chloropropane

Concen: 54.613 ug/l


RT: 12.939 min Scan# 1944


Delta R.T. 0.000 min

Lab File: VX045559.D

Acq: 03 Apr 2025 10:30

Tgt	Ion	Resp:	21298
Ion	Ratio	Lower	Upper
75	100		
155	66.9	34.9	104.7
157	87.1	44.9	134.7




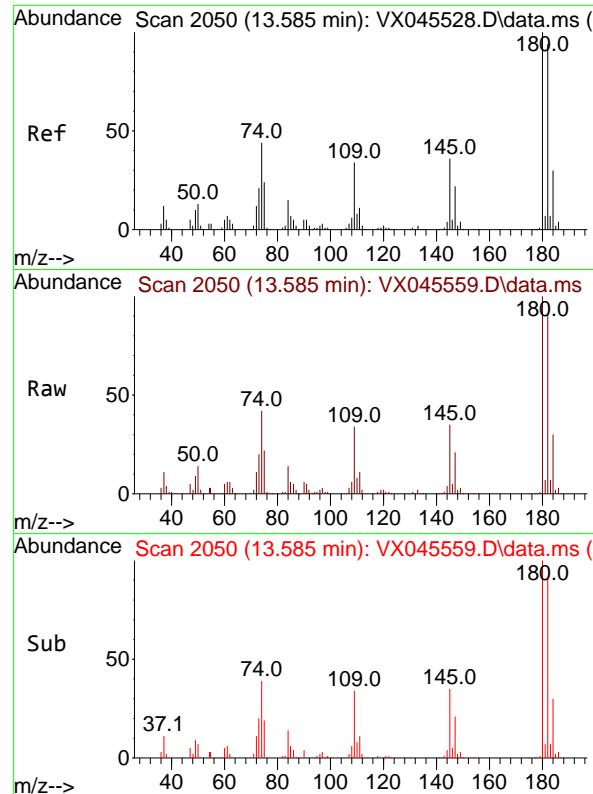


#93  
1,2,4-Trichlorobenzene  
Concen: 53.424 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED




Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

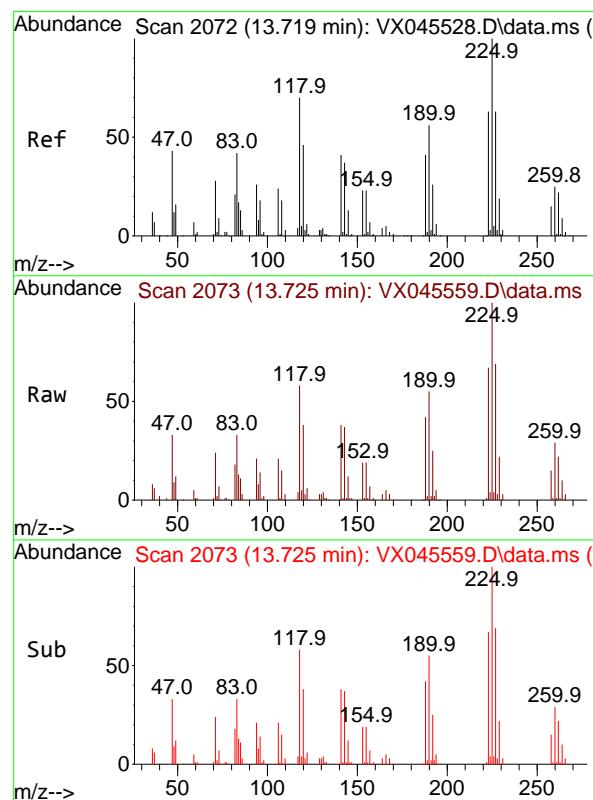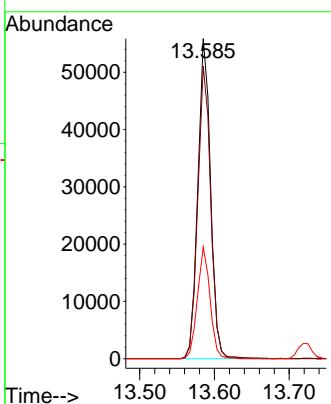

#94  
Hexachlorobutadiene  
Concen: 53.224 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. 0.006 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion:225 Resp: 28337  
Ion Ratio Lower Upper  
225 100  
223 64.6 31.1 93.3  
227 65.5 32.2 96.6

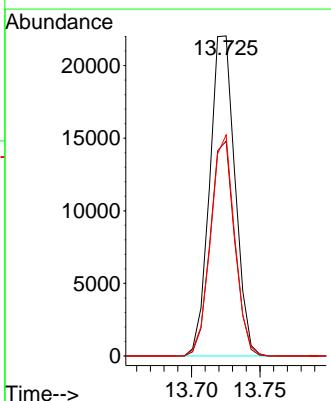


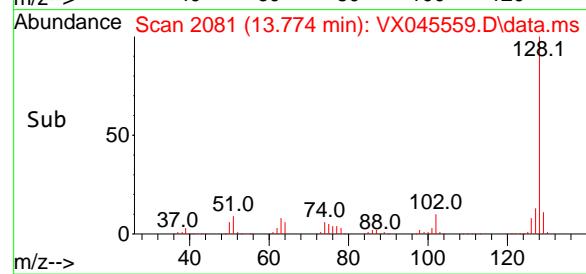
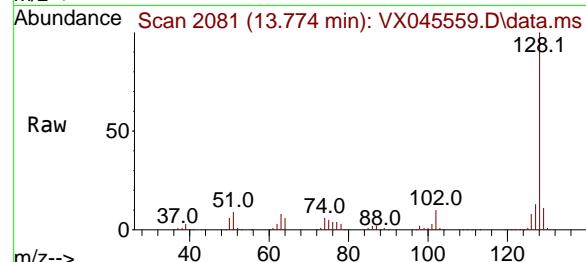
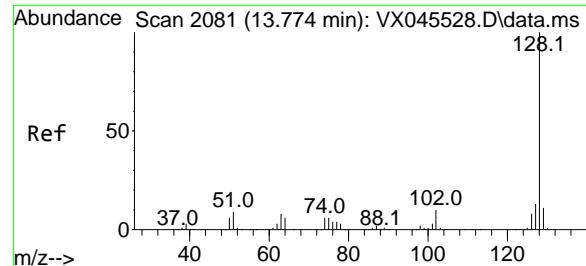


#95  
Naphthalene  
Concen: 51.463 ug/l  
RT: 13.774 min Scan# 2  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

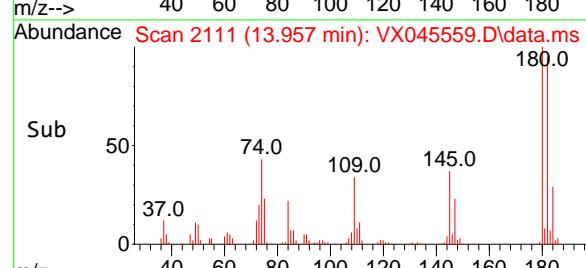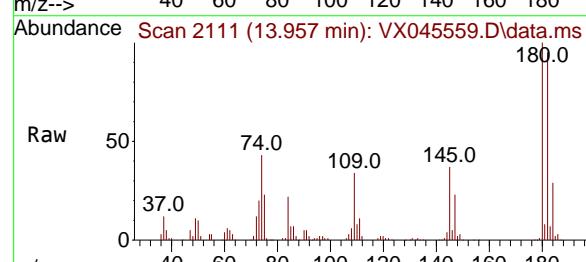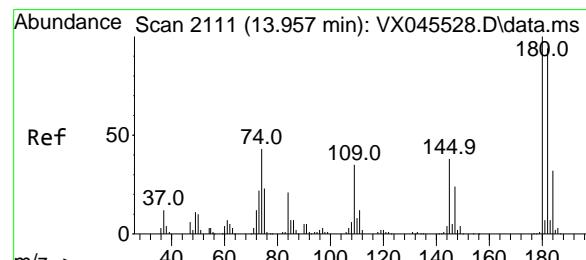

#96  
1,2,3-Trichlorobenzene  
Concen: 51.481 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045559.D  
Acq: 03 Apr 2025 10:30

Tgt Ion:180 Resp: 66605  
Ion Ratio Lower Upper  
180 100  
182 95.5 47.3 141.8  
145 36.6 18.2 54.6

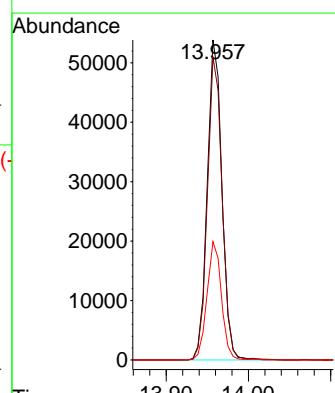

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045559.D  
 Acq On : 03 Apr 2025 10:30  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Apr 04 01:17:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	100	0.00
2 T	Dichlorodifluoromethane	0.748	0.863	-15.4	105	0.00
3 P	Chloromethane	0.768	0.782	-1.8	99	0.00
4 C	Vinyl Chloride	0.703	0.734	-4.4#	102	0.00
5 T	Bromomethane	0.333	0.322	3.3	97	0.00
6 T	Chloroethane	0.373	0.405	-8.6	101	0.00
7 T	Trichlorofluoromethane	1.048	1.105	-5.4	101	0.00
8 T	Diethyl Ether	0.352	0.347	1.4	97	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.614	0.658	-7.2	105	0.00
10 T	Methyl Iodide	0.766	0.783	-2.2	98	0.00
11 T	Tert butyl alcohol	0.123	0.122	0.8	96	0.00
12 CM	1,1-Dichloroethene	0.600	0.611	-1.8#	101	0.00
13 T	Acrolein	0.169	0.197	-16.6	117	0.00
14 T	Allyl chloride	1.139	1.165	-2.3	99	0.00
15 T	Acrylonitrile	0.388	0.390	-0.5	95	0.00
16 T	Acetone	0.375	0.368	1.9	97	0.00
17 T	Carbon Disulfide	1.483	1.535	-3.5	98	0.00
18 T	Methyl Acetate	0.864	0.859	0.6	100	0.00
19 T	Methyl tert-butyl Ether	2.100	2.077	1.1	98	0.00
20 T	Methylene Chloride	0.703	0.693	1.4	97	0.00
21 T	trans-1,2-Dichloroethene	0.613	0.615	-0.3	98	0.00
22 T	Diisopropyl ether	2.243	2.271	-1.2	99	0.00
23 T	Vinyl Acetate	1.938	2.024	-4.4	97	0.00
24 P	1,1-Dichloroethane	1.269	1.249	1.6	98	0.00
25 T	2-Butanone	0.550	0.565	-2.7	96	0.00
26 T	2,2-Dichloropropane	0.820	0.904	-10.2	106	0.00
27 T	cis-1,2-Dichloroethene	0.747	0.736	1.5	97	0.00
28 T	Bromochloromethane	0.613	0.598	2.4	100	0.00
29 T	Tetrahydrofuran	0.356	0.356	0.0	96	0.00
30 C	Chloroform	1.306	1.290	1.2#	98	0.00
31 T	Cyclohexane	1.122	1.136	-1.2	101	0.00
32 T	1,1,1-Trichloroethane	1.105	1.105	0.0	99	0.00
33 S	1,2-Dichloroethane-d4	0.914	0.886	3.1	102	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	97	0.00
35 S	Dibromofluoromethane	0.355	0.358	-0.8	100	0.00
36 T	1,1-Dichloropropene	0.479	0.497	-3.8	99	0.00
37 T	Ethyl Acetate	0.604	0.615	-1.8	95	0.00
38 T	Carbon Tetrachloride	0.518	0.561	-8.3	101	0.00
39 T	Methylcyclohexane	0.587	0.655	-11.6	102	0.00
40 TM	Benzene	1.463	1.502	-2.7	98	0.00
41 T	Methacrylonitrile	0.318	0.343	-7.9	95	-0.01
42 TM	1,2-Dichloroethane	0.604	0.634	-5.0	99	0.00
43 T	Isopropyl Acetate	0.915	0.973	-6.3	96	0.00
44 TM	Trichloroethene	0.348	0.350	-0.6	97	0.00
45 C	1,2-Dichloropropane	0.365	0.381	-4.4#	98	0.00
46 T	Dibromomethane	0.280	0.294	-5.0	97	0.00
47 T	Bromodichloromethane	0.560	0.596	-6.4	101	0.00
48 T	Methyl methacrylate	0.472	0.509	-7.8	97	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045559.D  
 Acq On : 03 Apr 2025 10:30  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Apr 04 01:17:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.009	0.009	0.0	95	0.00
50 S	Toluene-d8	1.238	1.248	-0.8	99	0.00
51 T	4-Methyl-2-Pentanone	0.606	0.658	-8.6	96	0.00
52 CM	Toluene	0.885	0.904	-2.1#	96	0.00
53 T	t-1,3-Dichloropropene	0.467	0.519	-11.1	99	0.00
54 T	cis-1,3-Dichloropropene	0.526	0.584	-11.0	99	0.00
55 T	1,1,2-Trichloroethane	0.353	0.367	-4.0	99	0.00
56 T	Ethyl methacrylate	0.546	0.600	-9.9	97	0.00
57 T	1,3-Dichloropropane	0.614	0.632	-2.9	97	0.00
58 T	2-Chloroethyl Vinyl ether	0.276	0.308	-11.6	100	0.00
59 T	2-Hexanone	0.449	0.478	-6.5	94	0.00
60 T	Dibromochloromethane	0.385	0.421	-9.4	99	0.00
61 T	1,2-Dibromoethane	0.357	0.378	-5.9	98	0.00
62 S	4-Bromofluorobenzene	0.451	0.460	-2.0	98	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	96	0.00
64 T	Tetrachloroethene	0.353	0.354	-0.3	98	0.00
65 PM	Chlorobenzene	1.068	1.122	-5.1	99	0.00
66 T	1,1,1,2-Tetrachloroethane	0.371	0.384	-3.5	99	0.00
67 C	Ethyl Benzene	1.914	2.033	-6.2#	97	0.00
68 T	m/p-Xylenes	0.696	0.743	-6.8	98	0.00
69 T	o-Xylene	0.686	0.728	-6.1	97	0.00
70 T	Styrene	1.132	1.241	-9.6	98	0.00
71 P	Bromoform	0.277	0.303	-9.4	98	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	96	0.00
73 T	Isopropylbenzene	4.005	4.226	-5.5	97	0.00
74 T	N-amyl acetate	1.916	1.991	-3.9	93	0.00
75 P	1,1,2,2-Tetrachloroethane	1.407	1.361	3.3	95	0.00
76 T	1,2,3-Trichloropropane	1.220	1.213	0.6	95	0.00
77 T	Bromobenzene	0.925	0.950	-2.7	98	0.00
78 T	n-propylbenzene	4.613	4.984	-8.0	98	0.00
79 T	2-Chlorotoluene	2.949	3.039	-3.1	99	0.00
80 T	1,3,5-Trimethylbenzene	3.312	3.590	-8.4	98	0.00
81 T	trans-1,4-Dichloro-2-butene	0.359	0.378	-5.3	98	0.00
82 T	4-Chlorotoluene	3.288	3.496	-6.3	98	0.00
83 T	tert-Butylbenzene	3.279	3.501	-6.8	98	0.00
84 T	1,2,4-Trimethylbenzene	3.324	3.594	-8.1	98	0.00
85 T	sec-Butylbenzene	4.027	4.419	-9.7	99	0.00
86 T	p-Isopropyltoluene	3.320	3.646	-9.8	100	0.00
87 T	1,3-Dichlorobenzene	1.684	1.724	-2.4	98	0.00
88 T	1,4-Dichlorobenzene	1.708	1.707	0.1	97	0.00
89 T	n-Butylbenzene	2.879	3.293	-14.4	100	0.00
90 T	Hexachloroethane	0.571	0.634	-11.0	102	0.00
91 T	1,2-Dichlorobenzene	1.675	1.689	-0.8	97	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.294	0.321	-9.2	98	0.00
93 T	1,2,4-Trichlorobenzene	0.932	0.996	-6.9	101	0.00
94 T	Hexachlorobutadiene	0.402	0.428	-6.5	102	0.00
95 T	Naphthalene	3.469	3.571	-2.9	92	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
Data File : VX045559.D  
Acq On : 03 Apr 2025 10:30  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
LabSampleId :  
VSTDCCC050

Quant Time: Apr 04 01:17:10 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	0.976	1.005	-3.0	97	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045559.D  
 Acq On : 03 Apr 2025 10:30  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Apr 04 01:17:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	100	0.00
2 T	Dichlorodifluoromethane	50.000	57.700	-15.4	105	0.00
3 P	Chloromethane	50.000	50.909	-1.8	99	0.00
4 C	Vinyl Chloride	50.000	52.195	-4.4#	102	0.00
5 T	Bromomethane	50.000	48.364	3.3	97	0.00
6 T	Chloroethane	50.000	54.319	-8.6	101	0.00
7 T	Trichlorofluoromethane	50.000	52.725	-5.5	101	0.00
8 T	Diethyl Ether	50.000	49.284	1.4	97	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	53.581	-7.2	105	0.00
10 T	Methyl Iodide	50.000	51.106	-2.2	98	0.00
11 T	Tert butyl alcohol	250.000	247.660	0.9	96	0.00
12 CM	1,1-Dichloroethene	50.000	50.876	-1.8#	101	0.00
13 T	Acrolein	250.000	290.369	-16.1	117	0.00
14 T	Allyl chloride	50.000	51.139	-2.3	99	0.00
15 T	Acrylonitrile	250.000	251.370	-0.5	95	0.00
16 T	Acetone	250.000	244.836	2.1	97	0.00
17 T	Carbon Disulfide	50.000	51.779	-3.6	98	0.00
18 T	Methyl Acetate	50.000	49.677	0.6	100	0.00
19 T	Methyl tert-butyl Ether	50.000	49.447	1.1	98	0.00
20 T	Methylene Chloride	50.000	49.292	1.4	97	0.00
21 T	trans-1,2-Dichloroethene	50.000	50.139	-0.3	98	0.00
22 T	Diisopropyl ether	50.000	50.611	-1.2	99	0.00
23 T	Vinyl Acetate	250.000	261.101	-4.4	97	0.00
24 P	1,1-Dichloroethane	50.000	49.227	1.5	98	0.00
25 T	2-Butanone	250.000	257.055	-2.8	96	0.00
26 T	2,2-Dichloropropane	50.000	55.135	-10.3	106	0.00
27 T	cis-1,2-Dichloroethene	50.000	49.223	1.6	97	0.00
28 T	Bromochloromethane	50.000	48.775	2.5	100	0.00
29 T	Tetrahydrofuran	250.000	250.088	-0.0	96	0.00
30 C	Chloroform	50.000	49.413	1.2#	98	0.00
31 T	Cyclohexane	50.000	50.618	-1.2	101	0.00
32 T	1,1,1-Trichloroethane	50.000	50.002	-0.0	99	0.00
33 S	1,2-Dichloroethane-d4	50.000	48.452	3.1	102	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	97	0.00
35 S	Dibromofluoromethane	50.000	50.400	-0.8	100	0.00
36 T	1,1-Dichloropropene	50.000	51.889	-3.8	99	0.00
37 T	Ethyl Acetate	50.000	50.922	-1.8	95	0.00
38 T	Carbon Tetrachloride	50.000	54.175	-8.3	101	0.00
39 T	Methylcyclohexane	50.000	55.811	-11.6	102	0.00
40 TM	Benzene	50.000	51.334	-2.7	98	0.00
41 T	Methacrylonitrile	50.000	53.895	-7.8	95	-0.01
42 TM	1,2-Dichloroethane	50.000	52.471	-4.9	99	0.00
43 T	Isopropyl Acetate	50.000	53.203	-6.4	96	0.00
44 TM	Trichloroethene	50.000	50.400	-0.8	97	0.00
45 C	1,2-Dichloropropane	50.000	52.177	-4.4#	98	0.00
46 T	Dibromomethane	50.000	52.432	-4.9	97	0.00
47 T	Bromodichloromethane	50.000	53.281	-6.6	101	0.00
48 T	Methyl methacrylate	50.000	53.916	-7.8	97	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045559.D  
 Acq On : 03 Apr 2025 10:30  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Apr 04 01:17:10 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	1069.810	-7.0	95	0.00
50 S	Toluene-d8	50.000	50.412	-0.8	99	0.00
51 T	4-Methyl-2-Pentanone	250.000	271.376	-8.6	96	0.00
52 CM	Toluene	50.000	51.038	-2.1#	96	0.00
53 T	t-1,3-Dichloropropene	50.000	48.265	3.5	99	0.00
54 T	cis-1,3-Dichloropropene	50.000	55.553	-11.1	99	0.00
55 T	1,1,2-Trichloroethane	50.000	51.988	-4.0	99	0.00
56 T	Ethyl methacrylate	50.000	54.916	-9.8	97	0.00
57 T	1,3-Dichloropropane	50.000	51.465	-2.9	97	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	278.463	-11.4	100	0.00
59 T	2-Hexanone	250.000	266.003	-6.4	94	0.00
60 T	Dibromochloromethane	50.000	54.791	-9.6	99	0.00
61 T	1,2-Dibromoethane	50.000	52.982	-6.0	98	0.00
62 S	4-Bromofluorobenzene	50.000	51.040	-2.1	98	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	96	0.00
64 T	Tetrachloroethene	50.000	50.202	-0.4	98	0.00
65 PM	Chlorobenzene	50.000	52.511	-5.0	99	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	51.757	-3.5	99	0.00
67 C	Ethyl Benzene	50.000	53.122	-6.2#	97	0.00
68 T	m/p-Xylenes	100.000	106.687	-6.7	98	0.00
69 T	o-Xylene	50.000	53.092	-6.2	97	0.00
70 T	Styrene	50.000	54.847	-9.7	98	0.00
71 P	Bromoform	50.000	54.761	-9.5	98	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	96	0.00
73 T	Isopropylbenzene	50.000	52.752	-5.5	97	0.00
74 T	N-amyl acetate	50.000	51.953	-3.9	93	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	48.351	3.3	95	0.00
76 T	1,2,3-Trichloropropane	50.000	49.735	0.5	95	0.00
77 T	Bromobenzene	50.000	51.347	-2.7	98	0.00
78 T	n-propylbenzene	50.000	54.023	-8.0	98	0.00
79 T	2-Chlorotoluene	50.000	51.521	-3.0	99	0.00
80 T	1,3,5-Trimethylbenzene	50.000	54.195	-8.4	98	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	52.613	-5.2	98	0.00
82 T	4-Chlorotoluene	50.000	53.158	-6.3	98	0.00
83 T	tert-Butylbenzene	50.000	53.394	-6.8	98	0.00
84 T	1,2,4-Trimethylbenzene	50.000	54.063	-8.1	98	0.00
85 T	sec-Butylbenzene	50.000	54.862	-9.7	99	0.00
86 T	p-Isopropyltoluene	50.000	54.914	-9.8	100	0.00
87 T	1,3-Dichlorobenzene	50.000	51.187	-2.4	98	0.00
88 T	1,4-Dichlorobenzene	50.000	49.973	0.1	97	0.00
89 T	n-Butylbenzene	50.000	57.188	-14.4	100	0.00
90 T	Hexachloroethane	50.000	55.591	-11.2	102	0.00
91 T	1,2-Dichlorobenzene	50.000	50.437	-0.9	97	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	54.613	-9.2	98	0.00
93 T	1,2,4-Trichlorobenzene	50.000	53.424	-6.8	101	0.00
94 T	Hexachlorobutadiene	50.000	53.224	-6.4	102	0.00
95 T	Naphthalene	50.000	51.463	-2.9	92	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
Data File : VX045559.D  
Acq On : 03 Apr 2025 10:30  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
LabSampleId :  
VSTDCCC050

Quant Time: Apr 04 01:17:10 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	Amount	Calc.	%Dev	Area	% Dev(min)
96 T 1,2,3-Trichlorobenzene	50.000	51.481	-3.0	97	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>CHEMTECH</u>		Contract:	<u>JAC005</u>	
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1711</u>	SAS No.:	<u>Q1711</u>
Instrument ID:	<u>MSVOA_X</u>		Calibration Date/Time:	<u>04/04/2025</u>	<u>10:00</u>
Lab File ID:	<u>VX045586.D</u>		Init. Calib. Date(s):	<u>04/01/2025</u>	<u>04/01/2025</u>
Heated Purge:	(Y/N)	N	Init. Calib. Time(s):	<u>17:06</u>	<u>19:02</u>
GC Column:	DB-624UI	ID: 0.18 (mm)			

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Vinyl Chloride	0.703	0.731		3.98	20
1,1-Dichloroethene	0.600	0.599		-0.17	20
1,1-Dichloroethane	1.269	1.270	0.1	0.08	20
cis-1,2-Dichloroethene	0.747	0.729		-2.41	20
1,1,1-Trichloroethane	1.105	1.107		0.18	20
Benzene	1.463	1.507		3.01	20
1,2-Dichloroethane	0.604	0.645		6.79	20
Trichloroethene	0.348	0.357		2.59	20
1,1,2-Trichloroethane	0.353	0.370		4.82	20
Tetrachloroethene	0.353	0.376		6.52	20
1,2-Dichloroethane-d4	0.914	0.776		-15.1	20
Dibromofluoromethane	0.355	0.311		-12.39	20
Toluene-d8	1.238	1.079		-12.84	20
4-Bromofluorobenzene	0.451	0.411		-8.87	20

All other compounds must meet a minimum RRF of 0.010.  
RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045586.D  
 Acq On : 04 Apr 2025 10:00  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDCCC050

Quant Time: Apr 04 23:10:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.538	168	96707	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.751	114	163287	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	142048	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	67379	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.946	65	75034	42.428	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	84.860%	
35) Dibromofluoromethane	5.379	113	50835	43.879	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	87.760%	
50) Toluene-d8	8.641	98	176247	43.586	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	87.180%	
62) 4-Bromofluorobenzene	11.079	95	67111	45.563	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	91.120%	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	81543	56.382	ug/l	98
3) Chloromethane	1.307	50	77087	51.883	ug/l	98
4) Vinyl Chloride	1.374	62	70654	51.962	ug/l	99
5) Bromomethane	1.593	94	31732	49.218	ug/l	99
6) Chloroethane	1.666	64	37965	52.626	ug/l	96
7) Trichlorofluoromethane	1.874	101	106831	52.688	ug/l	98
8) Diethyl Ether	2.130	74	33835	49.704	ug/l	96
9) 1,1,2-Trichlorotrifluo...	2.319	101	63673	53.591	ug/l	97
10) Methyl Iodide	2.441	142	74481	50.258	ug/l	99
11) Tert butyl alcohol	2.977	59	56849	239.188	ug/l	99
12) 1,1-Dichloroethene	2.306	96	57913	49.883	ug/l	97
13) Acrolein	2.233	56	96410	294.566	ug/l	100
14) Allyl chloride	2.654	41	113707	51.619	ug/l	98
15) Acrylonitrile	3.062	53	186427	248.485	ug/l	99
16) Acetone	2.380	43	178014	245.130	ug/l	97
17) Carbon Disulfide	2.502	76	145106	50.605	ug/l	100
18) Methyl Acetate	2.703	43	82725	49.477	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	203434	50.091	ug/l	97
20) Methylene Chloride	2.782	84	67127	49.375	ug/l	98
21) trans-1,2-Dichloroethene	3.081	96	58900	49.659	ug/l	96
22) Diisopropyl ether	3.757	45	220705	50.863	ug/l	97
23) Vinyl Acetate	3.715	43	975461	260.190	ug/l	100
24) 1,1-Dichloroethane	3.599	63	122843	50.059	ug/l	99
25) 2-Butanone	4.550	43	265772	250.017	ug/l	98
26) 2,2-Dichloropropane	4.465	77	91259	57.558	ug/l	99
27) cis-1,2-Dichloroethene	4.477	96	70467	48.765	ug/l	98
28) Bromochloromethane	4.885	49	58888	49.658	ug/l	99
29) Tetrahydrofuran	5.001	42	168431	244.391	ug/l	100
30) Chloroform	5.080	83	127207	50.378	ug/l	96
31) Cyclohexane	5.458	56	109881	50.650	ug/l	97
32) 1,1,1-Trichloroethane	5.373	97	107072	50.113	ug/l	99
36) 1,1-Dichloropropene	5.684	75	81866	52.336	ug/l	100
37) Ethyl Acetate	4.708	43	101136	51.305	ug/l	99
38) Carbon Tetrachloride	5.666	117	93252	55.161	ug/l	99
39) Methylcyclohexane	7.373	83	107689	56.163	ug/l	100
40) Benzene	6.025	78	246115	51.517	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045586.D  
 Acq On : 04 Apr 2025 10:00  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDCCC050

Quant Time: Apr 04 23:10:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.910	41	58687	56.425	ug/1	97
42) 1,2-Dichloroethane	6.074	62	105249	53.340	ug/1	100
43) Isopropyl Acetate	6.330	43	157563	52.737	ug/1	99
44) Trichloroethene	7.117	130	58260	51.308	ug/1	94
45) 1,2-Dichloropropane	7.421	63	62596	52.514	ug/1	98
46) Dibromomethane	7.574	93	47591	52.011	ug/1	98
47) Bromodichloromethane	7.818	83	97528	53.371	ug/1	100
48) Methyl methacrylate	7.690	41	83087	53.861	ug/1	99
49) 1,4-Dioxane	7.659	88	27137	972.308	ug/1	96
51) 4-Methyl-2-Pentanone	8.568	43	531642	268.424	ug/1	99
52) Toluene	8.714	92	151389	52.369	ug/1	99
53) t-1,3-Dichloropropene	8.976	75	86126	49.056	ug/1	100
54) cis-1,3-Dichloropropene	8.360	75	96025	55.919	ug/1	98
55) 1,1,2-Trichloroethane	9.147	97	60484	52.506	ug/1	96
56) Ethyl methacrylate	9.116	69	95283	53.447	ug/1	99
57) 1,3-Dichloropropane	9.305	76	105500	52.594	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.238	63	231389	256.573	ug/1	100
59) 2-Hexanone	9.427	43	391210	266.730	ug/1	99
60) Dibromochloromethane	9.519	129	69085	55.012	ug/1	97
61) 1,2-Dibromoethane	9.604	107	62072	53.230	ug/1	99
64) Tetrachloroethene	9.269	164	53413	53.258	ug/1	97
65) Chlorobenzene	10.073	112	160997	53.041	ug/1	97
66) 1,1,1,2-Tetrachloroethane	10.159	131	55317	52.492	ug/1	99
67) Ethyl Benzene	10.189	91	297368	54.700	ug/1	100
68) m/p-Xylenes	10.299	106	216775	109.636	ug/1	98
69) o-Xylene	10.640	106	105932	54.386	ug/1	99
70) Styrene	10.653	104	179659	55.886	ug/1	99
71) Bromoform	10.799	173	43659	55.486	ug/1 #	98
73) Isopropylbenzene	10.957	105	288495	53.453	ug/1	100
74) N-amyl acetate	10.842	43	134287	52.015	ug/1	100
75) 1,1,2,2-Tetrachloroethane	11.207	83	91045	48.021	ug/1	99
76) 1,2,3-Trichloropropane	11.238	75	81348m	49.496	ug/1	
77) Bromobenzene	11.195	156	63908	51.248	ug/1	100
78) n-propylbenzene	11.299	91	337878	54.351	ug/1	100
79) 2-Chlorotoluene	11.360	91	203932	51.314	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	239716	53.712	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	25247	52.135	ug/1	99
82) 4-Chlorotoluene	11.451	91	235414	53.128	ug/1	100
83) tert-Butylbenzene	11.713	119	234285	53.024	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	241455	53.903	ug/1	99
85) sec-Butylbenzene	11.890	105	298315	54.969	ug/1	100
86) p-Isopropyltoluene	12.006	119	246346	55.060	ug/1	99
87) 1,3-Dichlorobenzene	11.963	146	116982	51.535	ug/1	100
88) 1,4-Dichlorobenzene	12.036	146	116831	50.768	ug/1	99
89) n-Butylbenzene	12.329	91	223310	57.557	ug/1	99
90) Hexachloroethane	12.536	117	42554	55.342	ug/1	99
91) 1,2-Dichlorobenzene	12.335	146	115345	51.109	ug/1	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	21298	53.714	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	68119	54.225	ug/1	99
94) Hexachlorobutadiene	13.725	225	29467	54.435	ug/1	97
95) Naphthalene	13.774	128	241025	51.558	ug/1	99
96) 1,2,3-Trichlorobenzene	13.957	180	68237	51.875	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045586.D  
 Acq On : 04 Apr 2025 10:00  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDCCC050**

Quant Time: Apr 04 23:10:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
(#)						

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
Data File : VX045586.D  
Acq On : 04 Apr 2025 10:00  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 2 Sample Multiplier: 1




Quant Time: Apr 04 23:10:00 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

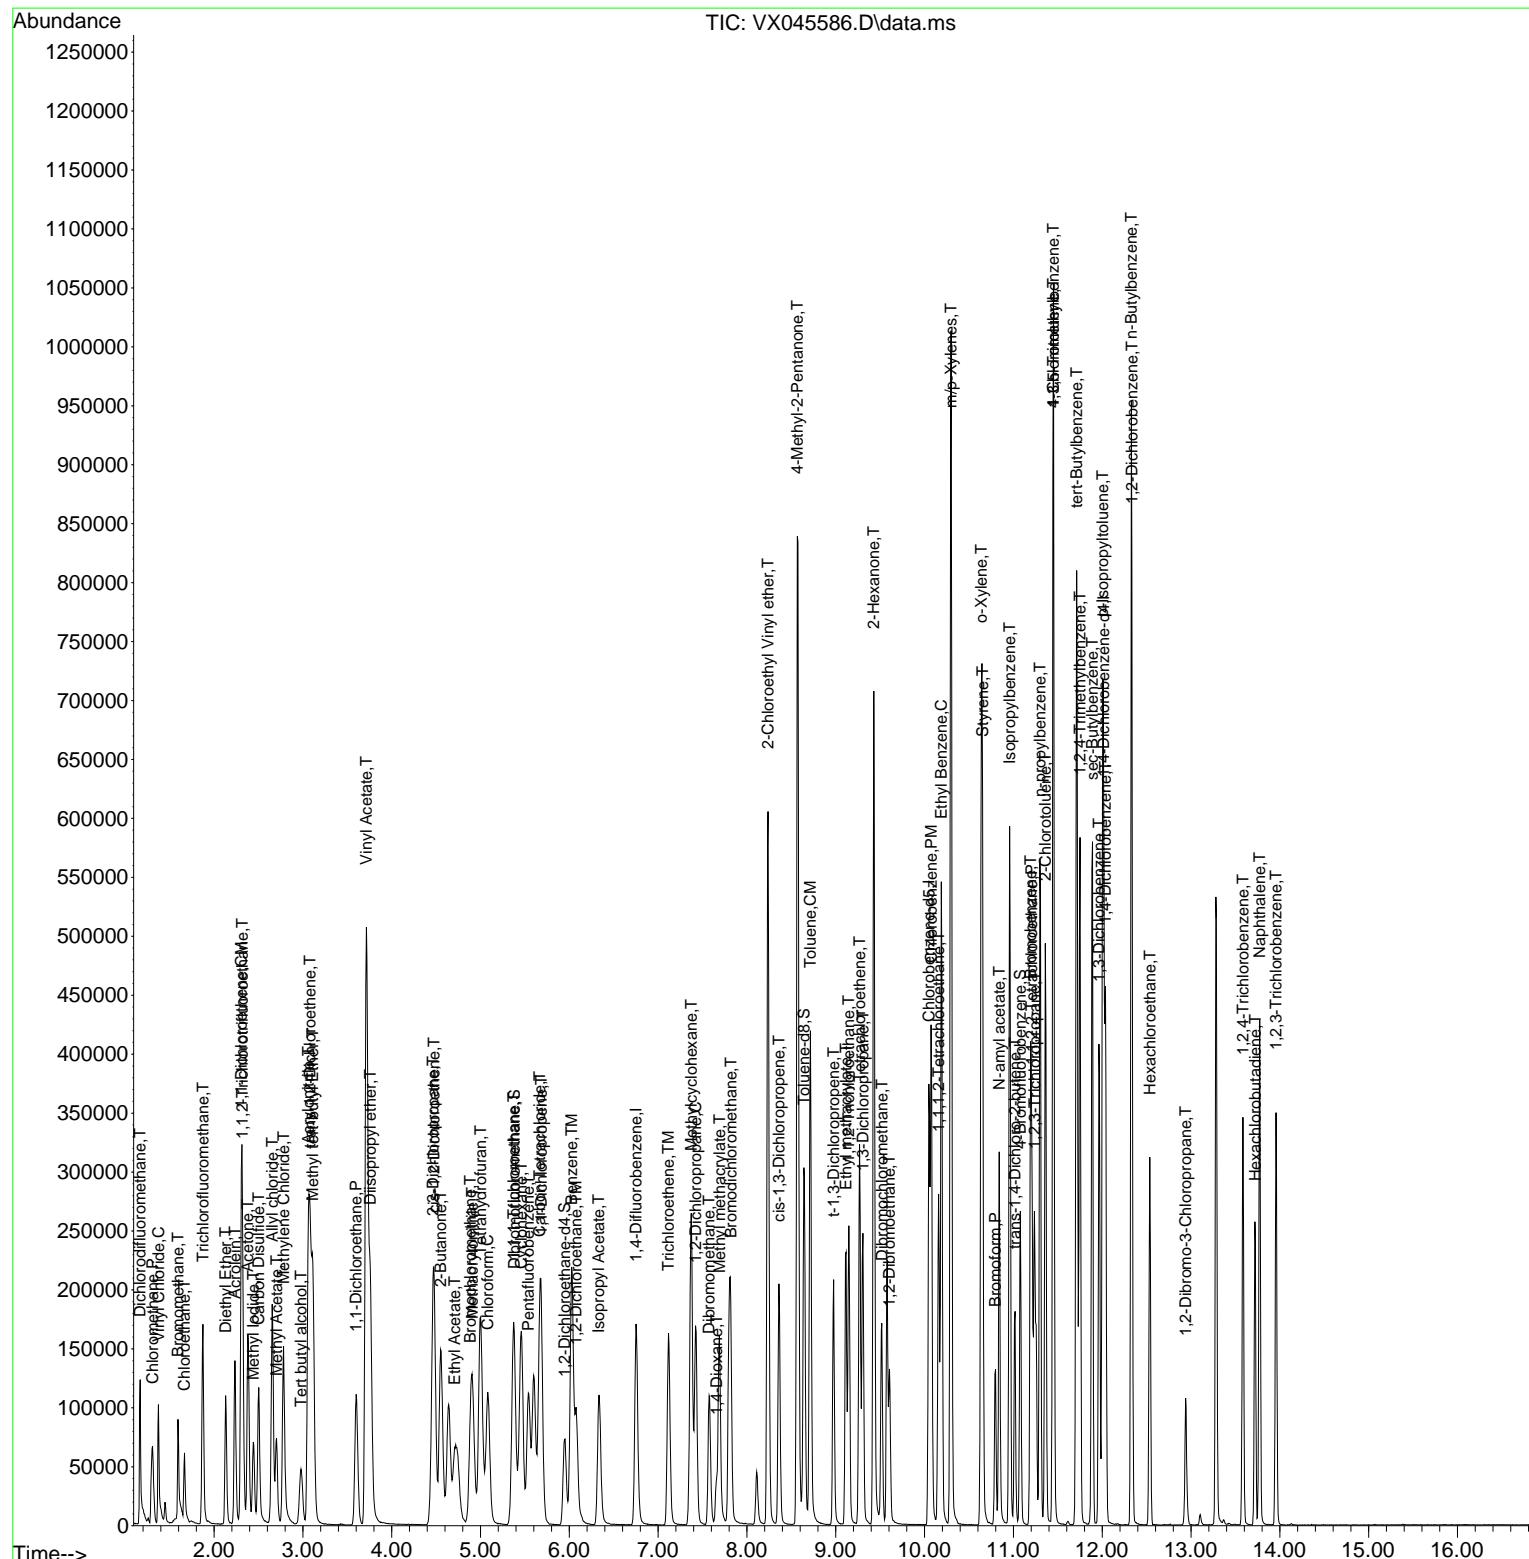

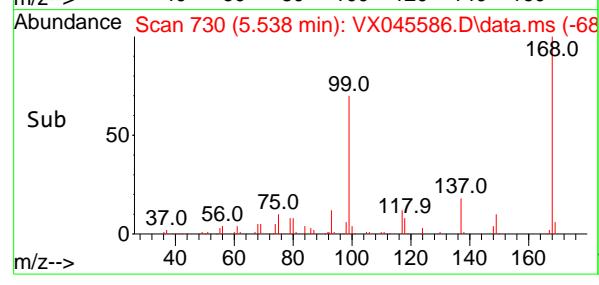

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.538 min Scan# 7

Delta R.T. -0.012 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X




ClientSampleId :

VSTDCCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#2

Dichlorodifluoromethane

Concen: 56.382 ug/l

RT: 1.166 min Scan# 13

Delta R.T. 0.000 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00


Tgt Ion: 85 Resp: 81543

Ion Ratio Lower Upper



85 100

87 33.0 16.1 48.2

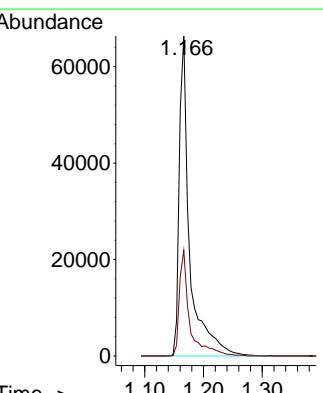




Abundance Scan 36 (1.307 min): VX045586.D\data.ms

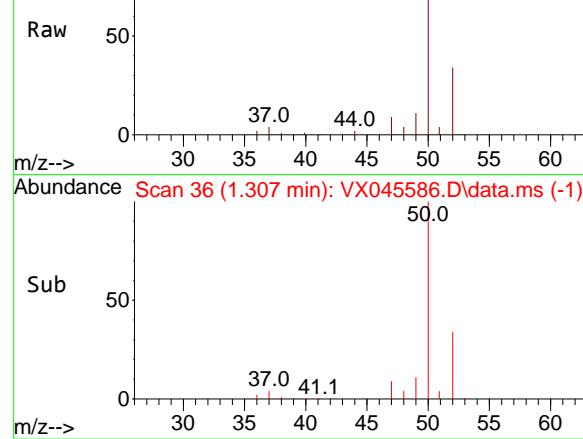

Abundance Scan 47 (1.374 min): VX045586.D\data.ms

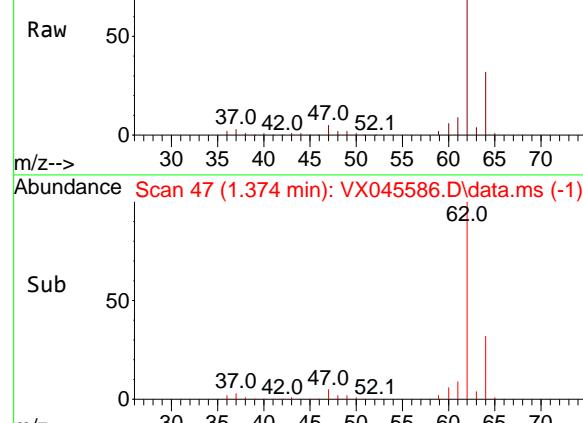

Abundance Scan 47 (1.374 min): VX045586.D\data.ms (-1)

#3

Chloromethane

Concen: 51.883 ug/l

RT: 1.307 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#4

Vinyl Chloride

Concen: 51.962 ug/l


RT: 1.374 min Scan# 47




Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt Ion: 62 Resp: 70654  
 Ion Ratio Lower Upper  
 62 100  
 64 32.2 25.5 38.3









#5  
Bromomethane  
Concen: 49.218 ug/l  
RT: 1.593 min Scan# 8  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

Tgt Ion: 94 Resp: 3173  
Ion Ratio Lower Upper  
94 100  
96 92.6 74.8 112.2


### Manual Integrations APPROVED




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

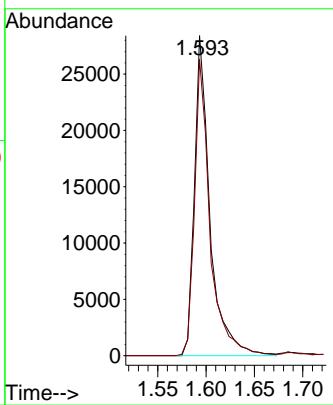

#6  
Chloroethane  
Concen: 52.626 ug/l  
RT: 1.666 min Scan# 95  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion: 64 Resp: 37965  
Ion Ratio Lower Upper  
64 100  
66 30.4 26.3 39.5



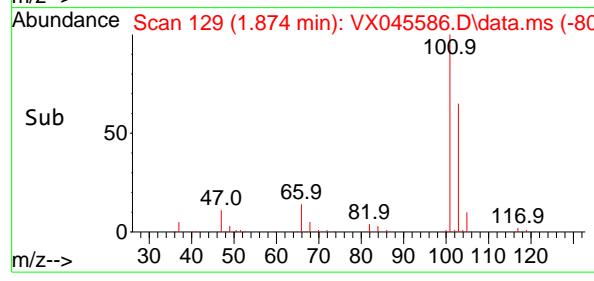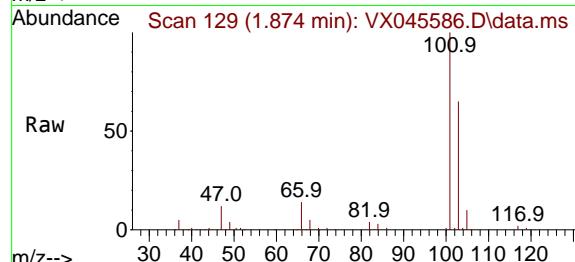



#7  
Trichlorofluoromethane  
Concen: 52.688 ug/l  
RT: 1.874 min Scan# 129  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050




### Manual Integrations APPROVED







Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

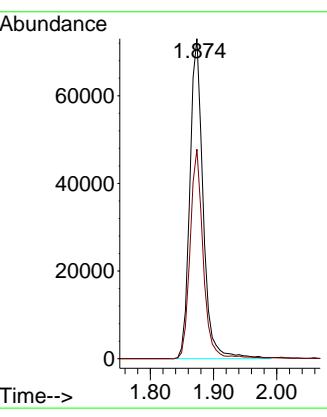

#8  
Diethyl Ether  
Concen: 49.704 ug/l  
RT: 2.130 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion: 74 Resp: 33835  
Ion Ratio Lower Upper  
74 100  
45 109.8 53.0 159.1



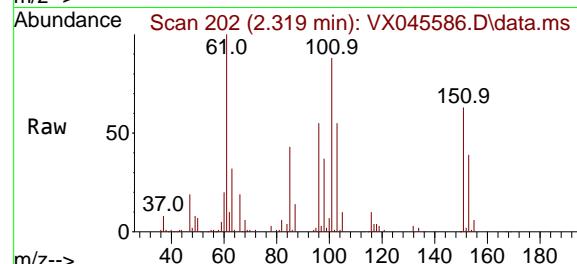

#9

1,1,2-Trichlorotrifluoroethane

Concen: 53.591 ug/l

RT: 2.319 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00


Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025


#10

Methyl Iodide

Concen: 50.258 ug/l

RT: 2.441 min Scan# 222

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00


Tgt Ion:142 Resp: 74481


Ion Ratio Lower Upper

142 100



127 50.8 40.2 60.4

141 14.7 11.7 17.5


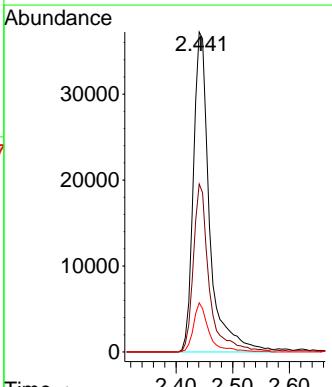




Abundance Scan 310 (2.977 min): VX045586.D\data.ms

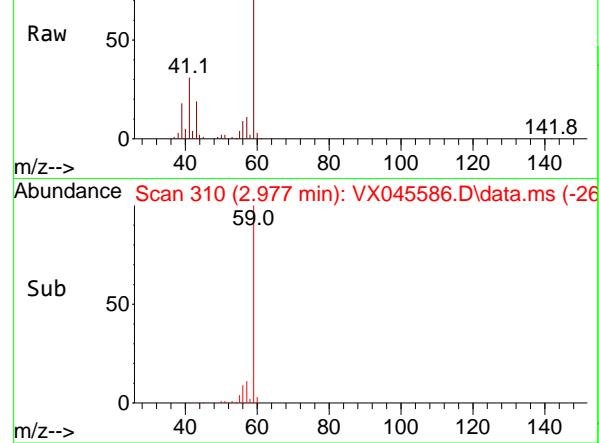

Abundance Scan 200 (2.306 min): VX045586.D\data.ms

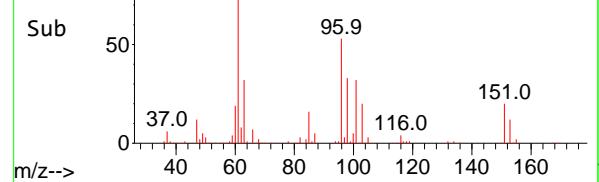


#11

Tert butyl alcohol  
Concen: 239.188 ug/l  
RT: 2.977 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCCC050

### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025




#12

1,1-Dichloroethene  
Concen: 49.883 ug/l  
RT: 2.306 min Scan# 200  
Delta R.T. -0.006 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion: 96 Resp: 57913  
Ion Ratio Lower Upper  
96 100  
61 187.1 145.7 218.5  
98 62.1 51.6 77.4

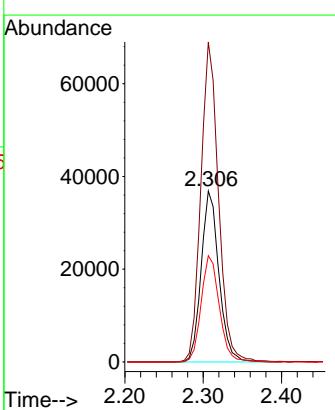




#13

Acrolein  
Concen: 294.566 ug/l  
RT: 2.233 min Scan# 189  
Delta R.T. -0.006 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050



Abundance

Time--&gt;


2.233

60000

40000

20000

0



#14

Allyl chloride  
Concen: 51.619 ug/l  
RT: 2.654 min Scan# 257  
Delta R.T. -0.006 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00



Tgt Ion: 41 Resp: 113707

Ion Ratio Lower Upper  
41 100  
39 77.6 60.2 90.2  
76 31.1 24.6 36.8

Abundance

Time--&gt;

2.654

60000







40000

20000

0



Time--&gt;

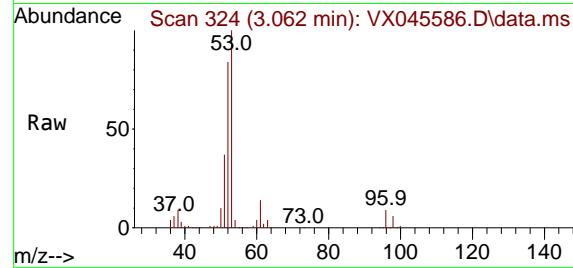

#15

Acrylonitrile

Concen: 248.485 ug/l

RT: 3.062 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

Tgt Ion: 53 Resp: 18642

Ion Ratio Lower Upper

53 100

52 83.1 67.4 101.2


51 37.6 29.9 44.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

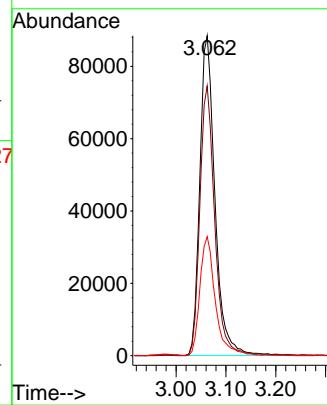

#16

Acetone

Concen: 245.130 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00


Tgt Ion: 43 Resp: 178014

Ion Ratio Lower Upper



43 100

58 26.3 22.3 33.5






Abundance Scan 232 (2.502 min): VX045586.D\data.ms

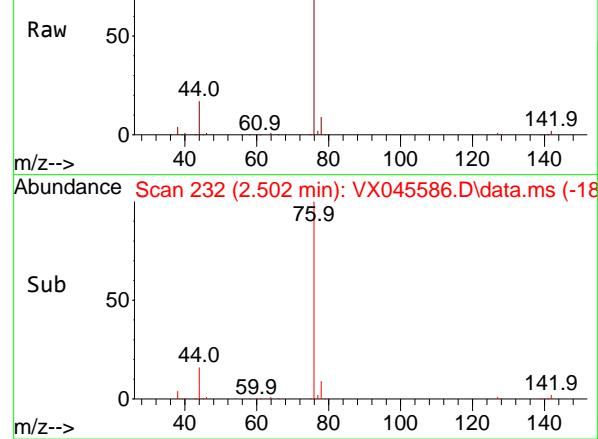

Abundance Scan 265 (2.703 min): VX045586.D\data.ms

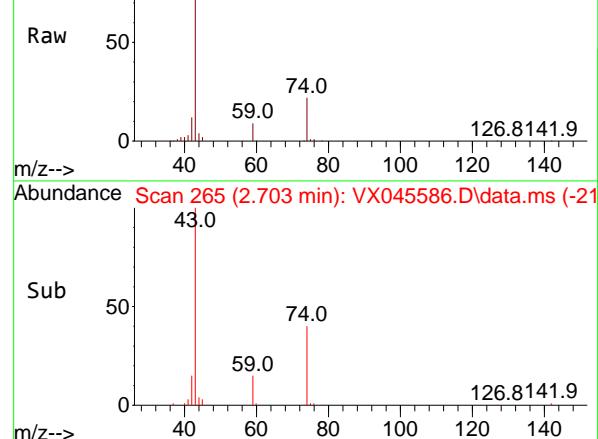

Abundance Scan 265 (2.703 min): VX045586.D\data.ms (-21)

#17

Carbon Disulfide

Concen: 50.605 ug/l

RT: 2.502 min Scan# 21

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#18

Methyl Acetate

Concen: 49.477 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00







Tgt Ion: 43 Resp: 82725

Ion Ratio Lower Upper

43 100

74 22.3 17.5 26.3






#19

Methyl tert-butyl Ether  
Concen: 50.091 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument :  
MSVOA\_X  
ClientSampleId :  
VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025









#20

Methylene Chloride  
Concen: 49.375 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion: 84 Resp: 67127  
Ion Ratio Lower Upper  
84 100  
49 138.8 107.5 161.3  
51 41.6 33.0 49.6  
86 63.0 50.1 75.1

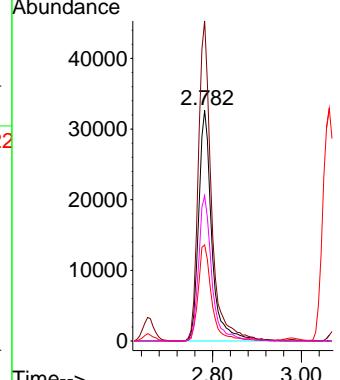

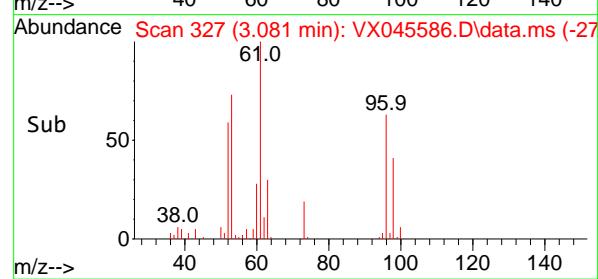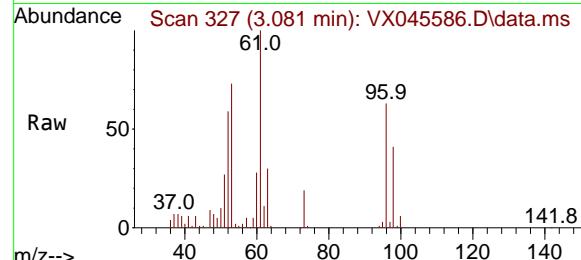

#21

trans-1,2-Dichloroethene

Concen: 49.659 ug/l

RT: 3.081 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

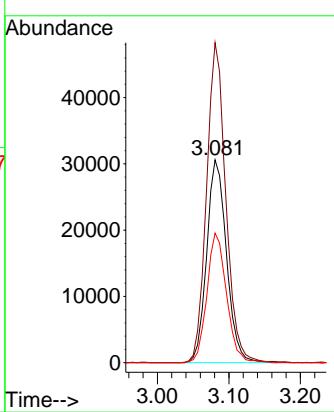

#22

Diisopropyl ether

Concen: 50.863 ug/l

RT: 3.757 min Scan# 438

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt Ion: 45 Resp: 220705


Ion Ratio Lower Upper


45 100

43 76.4 59.3 88.9

87 24.0 20.4 30.6

59 11.1 9.0 13.6

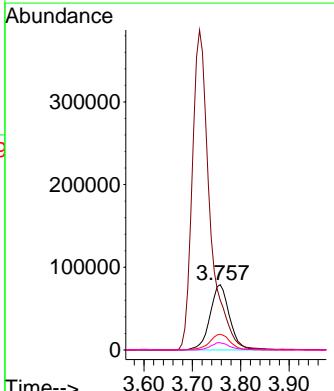



#23

**Vinyl Acetate**


Concen: 260.190 ug/l

RT: 3.715 min Scan# 412

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

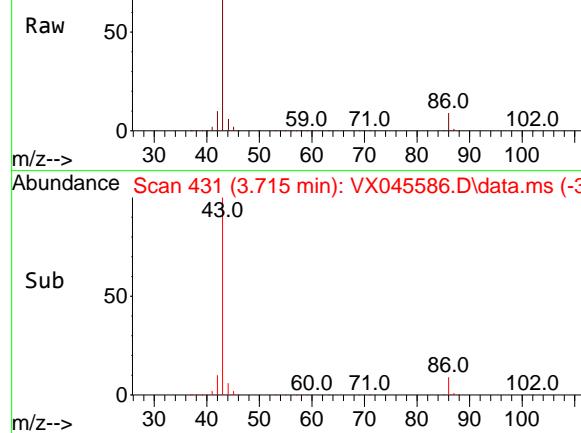

Tgt Ion: 43 Resp: 97546

Ion Ratio Lower Upper

43 100

86 9.3 7.5 11.3

Instrument:

MSVOA\_X



ClientSampleId :

VSTDCCC050

**Manual Integrations****APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

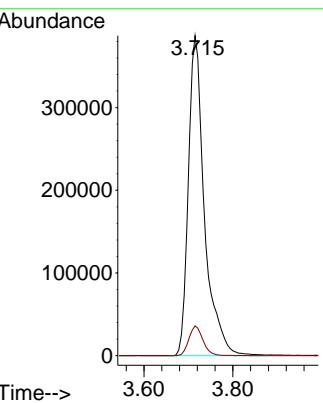

#24

**1,1-Dichloroethane**


Concen: 50.059 ug/l

RT: 3.599 min Scan# 412

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

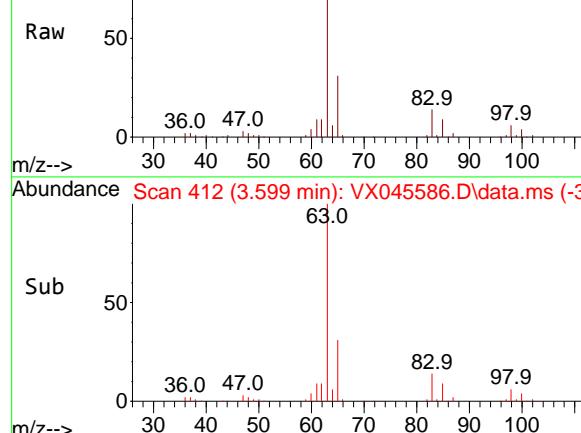


Tgt Ion: 63 Resp: 122843


Ion Ratio Lower Upper

63 100


98 6.2 3.4 10.1

100 4.1 2.2 6.6

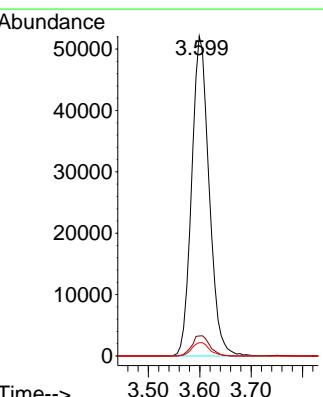


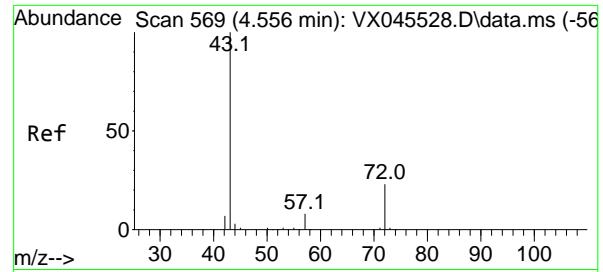

Abundance Scan 568 (4.550 min): VX045586.D\data.ms

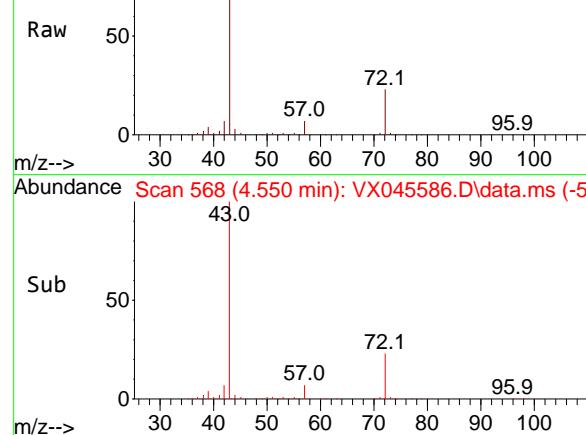

Abundance Scan 568 (4.550 min): VX045586.D\data.ms (-52)

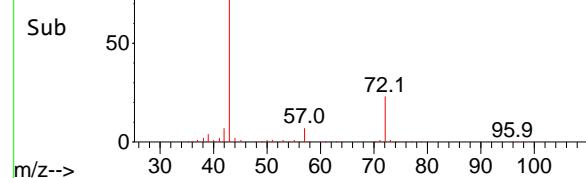

#25

2-Butanone

Concen: 250.017 ug/l

RT: 4.550 min Scan# 5

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050


**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025


Supervised By :Mahesh Dadoda 04/07/2025



Abundance Scan 554 (4.465 min): VX045586.D\data.ms

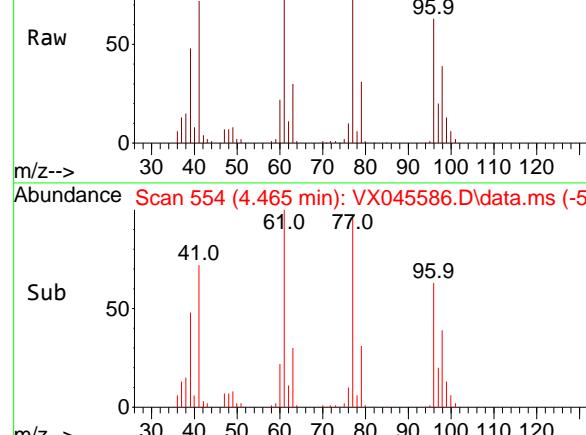

Abundance Scan 554 (4.465 min): VX045586.D\data.ms (-50)

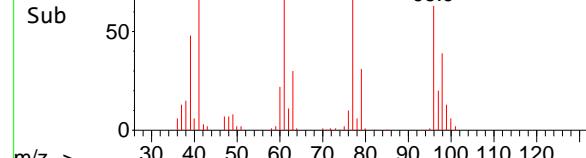

#26

2,2-Dichloropropane

Concen: 57.558 ug/l

RT: 4.465 min Scan# 554

Delta R.T. -0.006 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00







Tgt Ion: 77 Resp: 91259

Ion Ratio Lower Upper

77 100

97 20.8 10.6 31.8

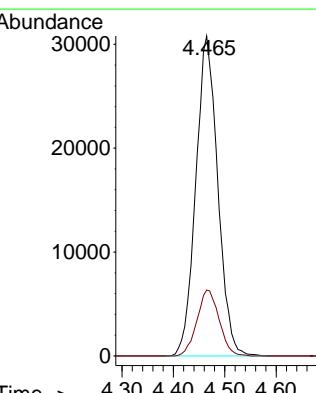

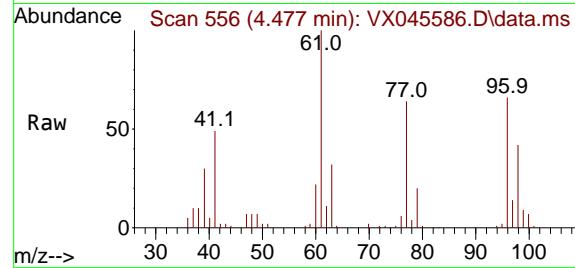


#27  
cis-1,2-Dichloroethene  
Concen: 48.765 ug/l  
RT: 4.477 min Scan# 51  
Delta R.T. -0.006 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED


Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025



#28  
Bromochloromethane  
Concen: 49.658 ug/l  
RT: 4.885 min Scan# 623  
Delta R.T. -0.012 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion: 49 Resp: 58888  
Ion Ratio Lower Upper  
49 100  
129 1.8 0.0 3.8  
130 67.2 54.6 81.8

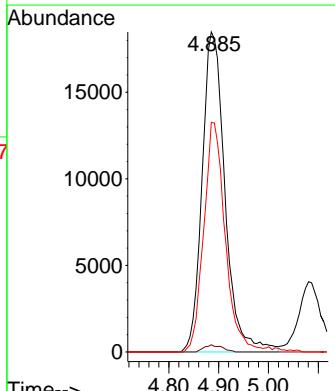



#29

Tetrahydrofuran

Concen: 244.391 ug/l

RT: 5.001 min Scan# 6


Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X

ClientSampleId : VSTDCCC050



Tgt Ion: 42 Resp: 16843

Ion Ratio Lower Upper

42 100




72 41.9 33.4 50.0

71 38.8 31.4 47.0

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

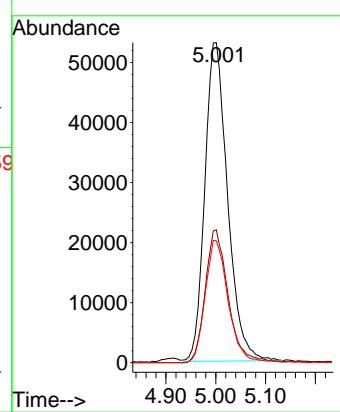

#30

Chloroform




Concen: 50.378 ug/l







RT: 5.080 min Scan# 655

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

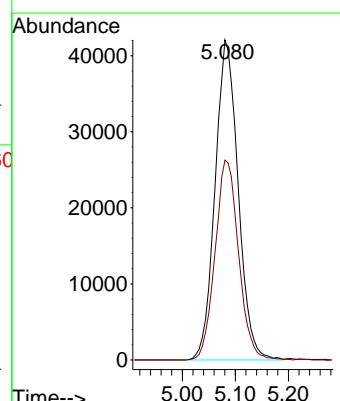



#31

Cyclohexane

Concen: 50.650 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X





ClientSampleId :


VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

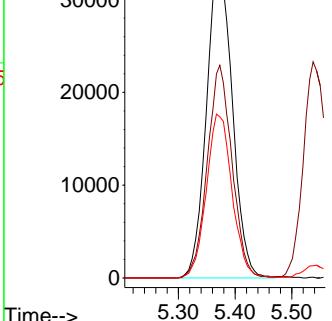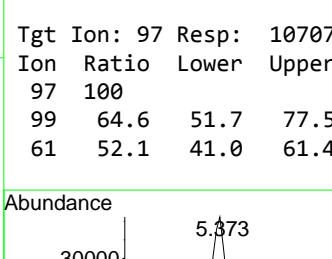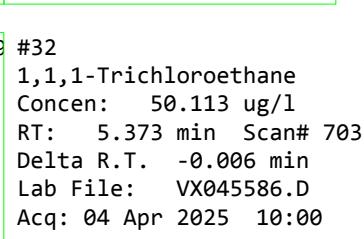

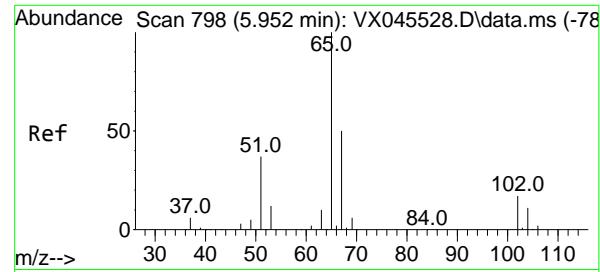





#33  
1,2-Dichloroethane-d4  
Concen: 42.428 ug/l  
RT: 5.946 min Scan# 7  
Delta R.T. -0.006 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

Tgt Ion: 65 Resp: 75034  
Ion Ratio Lower Upper  
65 100  
67 48.9 0.0 99.0




### Manual Integrations APPROVED







Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

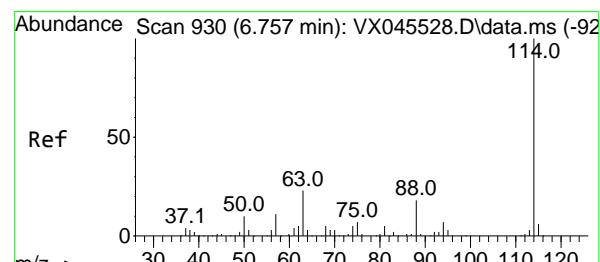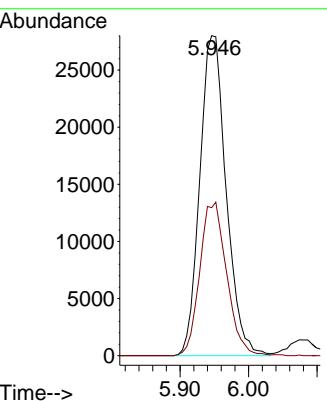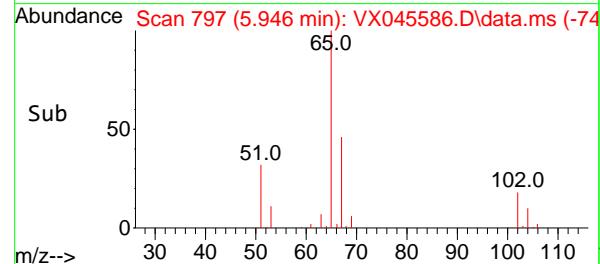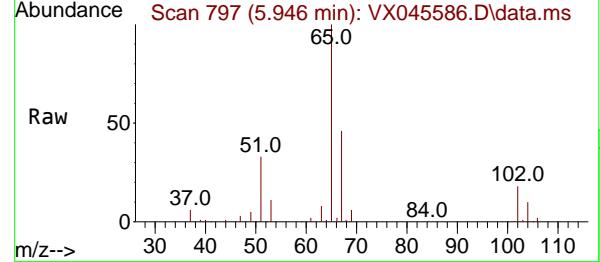

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.751 min Scan# 929  
Delta R.T. -0.006 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion:114 Resp: 163287  
Ion Ratio Lower Upper  
114 100  
63 23.3 0.0 46.8  
88 16.9 0.0 35.4

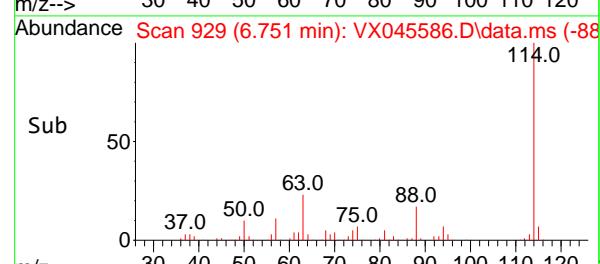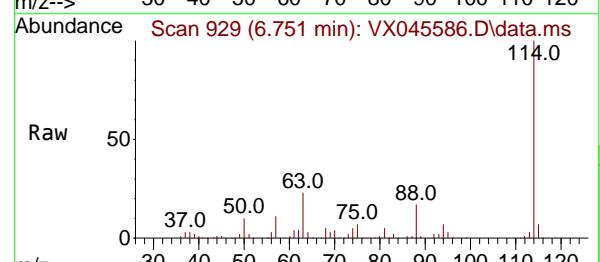



#35

Dibromofluoromethane

Concen: 43.879 ug/l

RT: 5.379 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCCC050

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#36

1,1-Dichloropropene

Concen: 52.336 ug/l


RT: 5.684 min Scan# 754


Delta R.T. 0.000 min

Lab File: VX045586.D





Acq: 04 Apr 2025 10:00

Tgt	Ion:	Resp:	81866
Ion	Ratio	Lower	Upper
75	100		
110	33.3	16.9	50.6
77	31.0	25.0	37.4

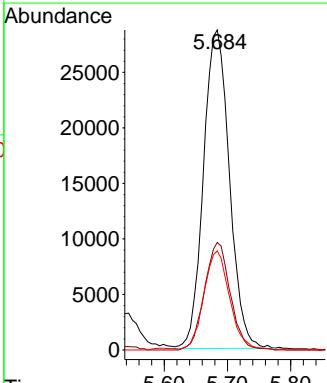

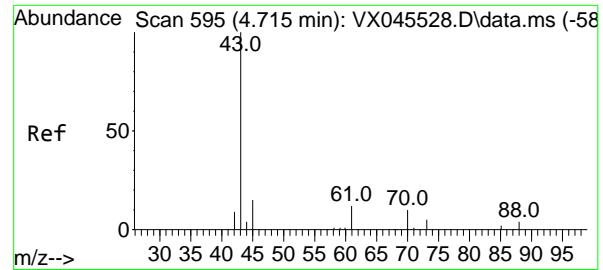

Abundance Scan 594 (4.708 min): VX045586.D\data.ms

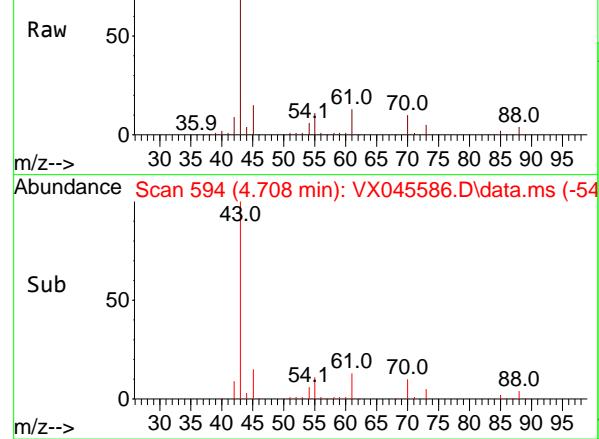

#37

**Ethyl Acetate**

Concen: 51.305 ug/l

RT: 4.708 min Scan# 5

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#38

**Carbon Tetrachloride**

Concen: 55.161 ug/l


RT: 5.666 min Scan# 751







Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt	Ion:117	Resp:	93252
Ion	Ratio	Lower	Upper
117	100		
119	94.6	76.9	115.3
121	30.3	24.2	36.2





#39

Methylcyclohexane

Concen: 56.163 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#40

Benzene

Concen: 51.517 ug/l

RT: 6.025 min Scan# 810

Delta R.T. -0.006 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00







Tgt Ion: 78 Resp: 246115

Ion Ratio Lower Upper

78 100

77 24.1 19.0 28.6



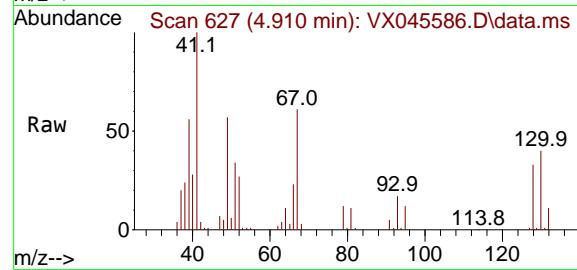

#41

Methacrylonitrile

Concen: 56.425 ug/l

RT: 4.910 min Scan# 6

Delta R.T. -0.012 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X


ClientSampleId : VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

Abundance

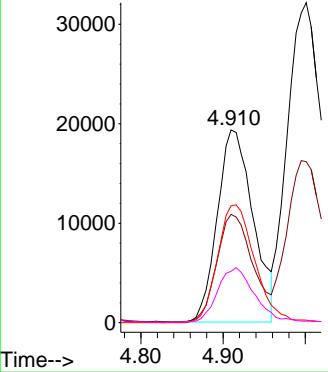

#42

1,2-Dichloroethane

Concen: 53.340 ug/l

RT: 6.074 min Scan# 818

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00


Tgt Ion: 62 Resp: 105249




Ion Ratio Lower Upper

62 100

98 7.6 0.0 15.2

Abundance

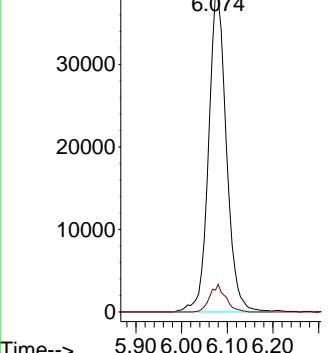

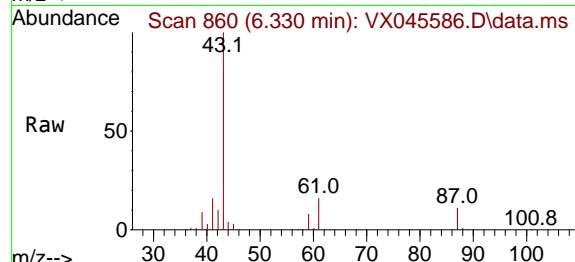

#43

Isopropyl Acetate

Concen: 52.737 ug/l

RT: 6.330 min Scan# 8

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

 Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Abundance

6.330

40000

20000

0

Time--&gt;

#44

Trichloroethene

Concen: 51.308 ug/l

RT: 7.117 min Scan# 989

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt Ion:130 Resp: 58260

Ion Ratio Lower Upper

130 100

95 107.1 0.0 202.0

Abundance

7.117

25000

20000




15000







10000

5000

0

Time--&gt;

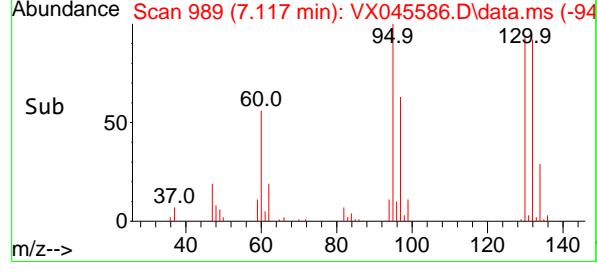



#45

1,2-Dichloropropane

Concen: 52.514 ug/l

RT: 7.421 min Scan# 1040

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

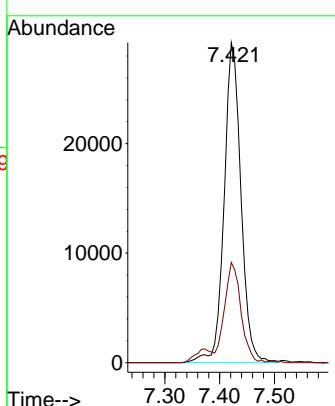

#46

Dibromomethane

Concen: 52.011 ug/l

RT: 7.574 min Scan# 1064

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00


Tgt Ion: 93 Resp: 47591




Ion Ratio Lower Upper

93 100

95 82.8 64.8 97.2

174 83.4 65.4 98.0

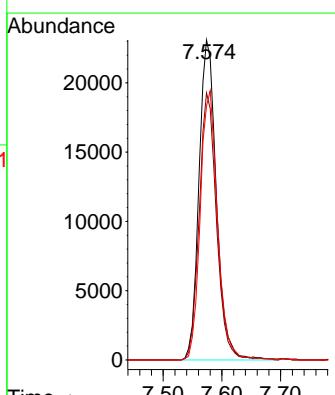







#47

Bromodichloromethane  
Concen: 53.371 ug/l  
RT: 7.818 min Scan# 1083  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument: MSVOA\_X  
ClientSampleId: VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025



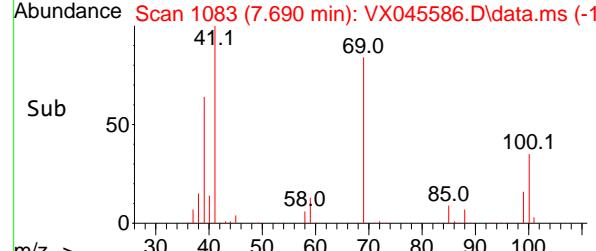
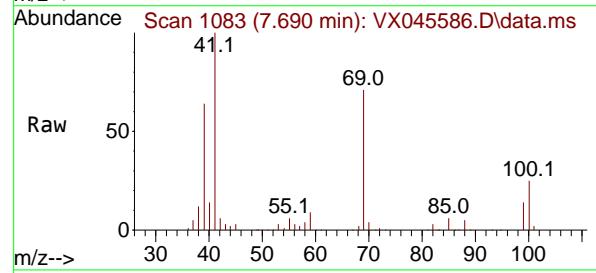




#48

Methyl methacrylate  
Concen: 53.861 ug/l  
RT: 7.690 min Scan# 1083  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion: 41 Resp: 83087  
Ion Ratio Lower Upper  
41 100  
69 72.1 58.2 87.2  
39 65.7 53.6 80.4





#49

1,4-Dioxane

Concen: 972.308 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

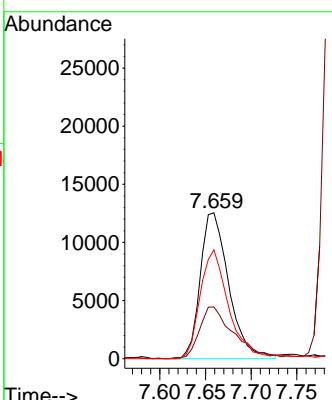

#50

Toluene-d8

Concen: 43.586 ug/l

RT: 8.641 min Scan# 1239

Delta R.T. -0.006 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00


Tgt Ion: 98 Resp: 176247

Ion Ratio Lower Upper


98 100

100 65.0 52.2 78.4

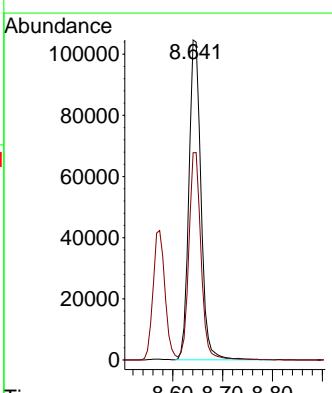




Abundance Scan 1227 (8.568 min): VX045586.D\data.ms

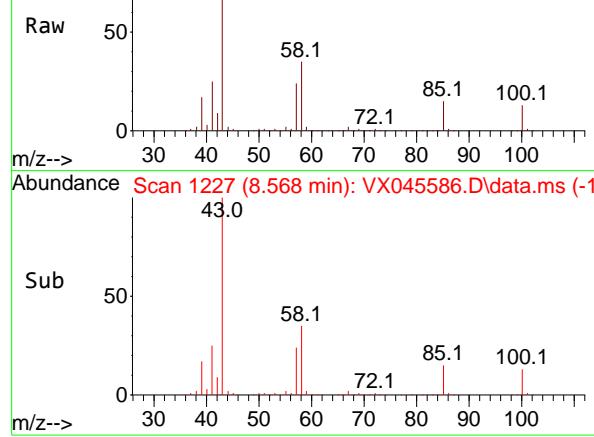

Abundance Scan 1227 (8.568 min): VX045586.D\data.ms (-1)

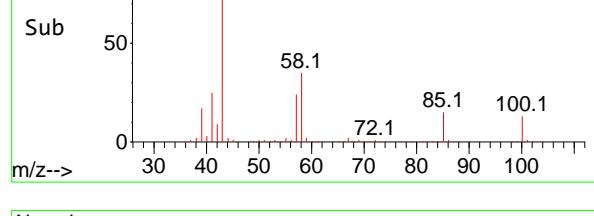

#51

4-Methyl-2-Pentanone

Concen: 268.424 ug/l

RT: 8.568 min Scan# 1228

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

Tgt Ion: 43 Resp: 53164

Ion Ratio Lower Upper



43 100

58 35.2 28.5 42.7


Manual Integrations  
APPROVED

Reviewed By :John Carlone 04/07/2025


Supervised By :Mahesh Dadoda 04/07/2025



Abundance Scan 1251 (8.714 min): VX045586.D\data.ms

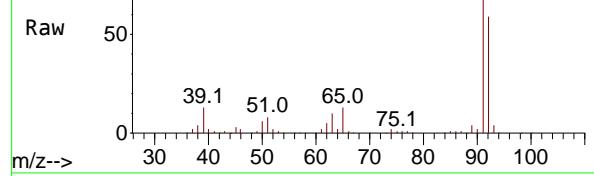

Abundance Scan 1251 (8.714 min): VX045586.D\data.ms (-1)

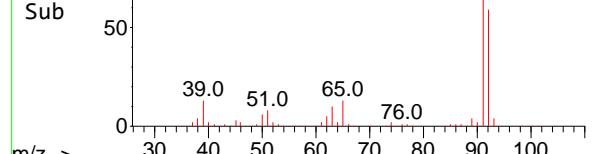

#52

Toluene

Concen: 52.369 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00




Tgt Ion: 92 Resp: 151389

Ion Ratio Lower Upper

92 100

91 172.1 138.7 208.1

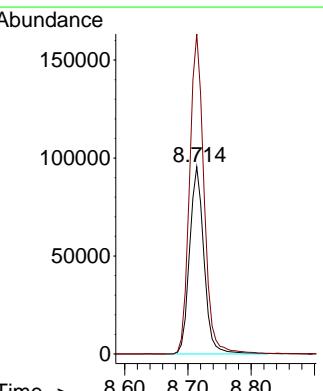



#53

t-1,3-Dichloropropene

Concen: 49.056 ug/l

RT: 8.976 min Scan# 1294

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

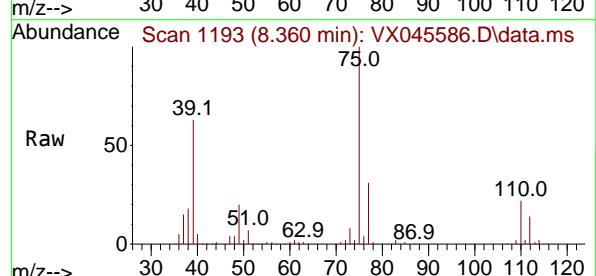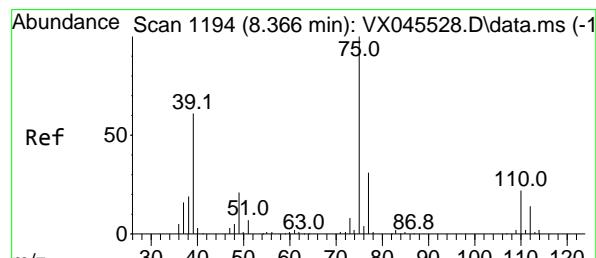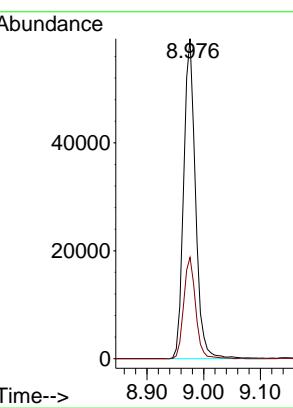

#54

cis-1,3-Dichloropropene

Concen: 55.919 ug/l


RT: 8.360 min Scan# 1193







Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt Ion: 75 Resp: 96025  
 Ion Ratio Lower Upper  
 75 100  
 77 30.9 24.6 36.8  
 39 63.2 48.4 72.6

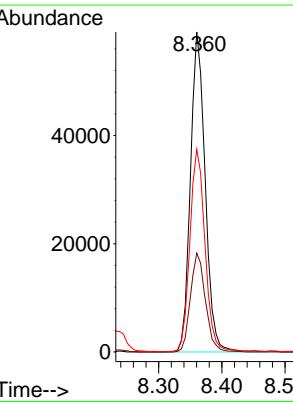



#55

1,1,2-Trichloroethane

Concen: 52.506 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCCC050

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

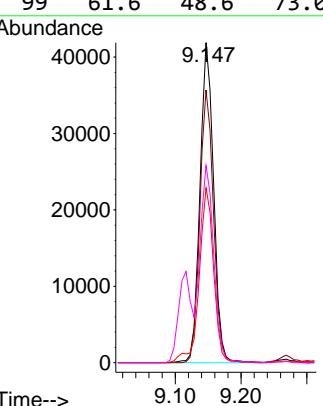

#56

Ethyl methacrylate

Concen: 53.447 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00


Tgt Ion: 69 Resp: 95283


Ion Ratio Lower Upper

69 100

41 77.7 61.3 91.9


39 50.0 40.2 60.2

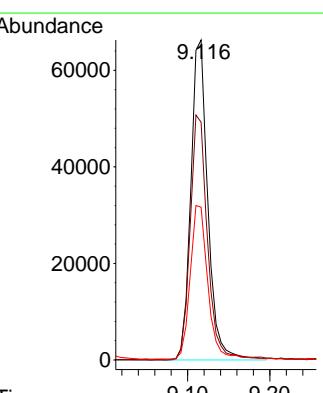

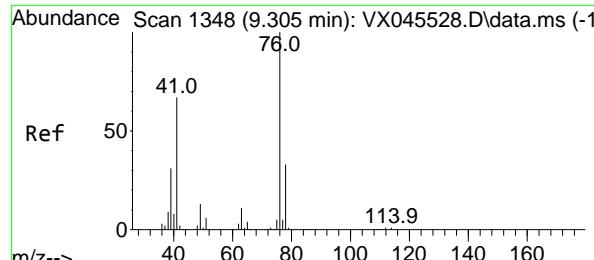

#57  
1,3-Dichloropropane  
Concen: 52.594 ug/l  
RT: 9.305 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00




Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

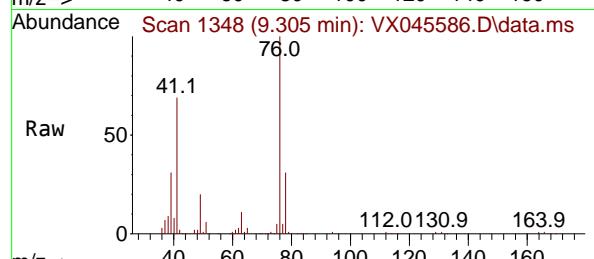


Tgt Ion: 76 Resp: 105500  
Ion Ratio Lower Upper  
76 100  
78 31.7 26.0 39.0

Manual Integrations  
APPROVED



Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

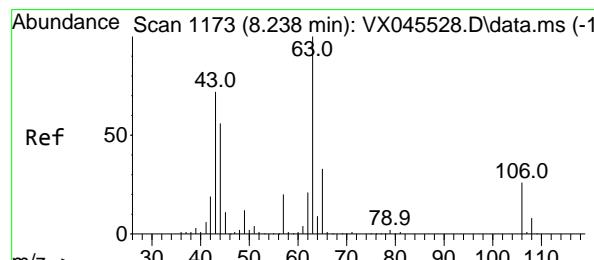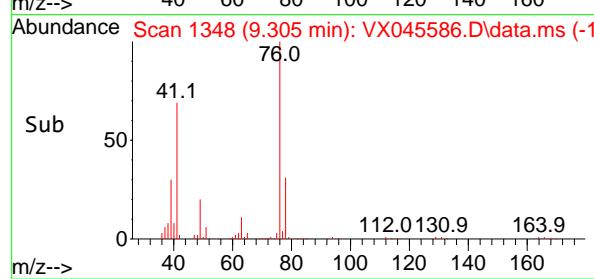


#58  
2-Chloroethyl Vinyl ether  
Concen: 256.573 ug/l  
RT: 8.238 min Scan# 1173  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

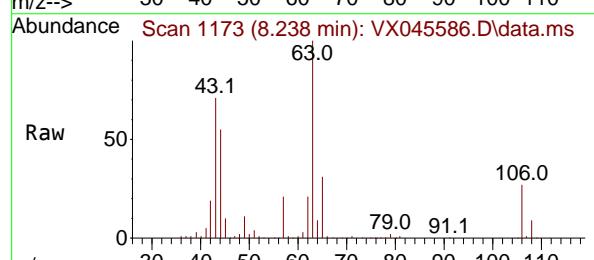



Tgt Ion: 63 Resp: 231389  
Ion Ratio Lower Upper  
63 100  
106 26.5 21.0 31.6

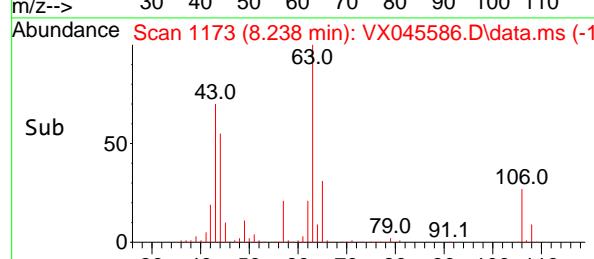



#59  
2-Hexanone  
Concen: 266.730 ug/l  
RT: 9.427 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00



Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

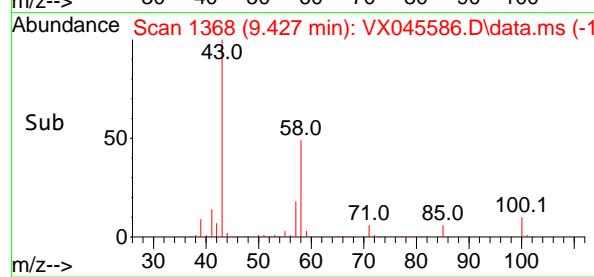


Tgt Ion: 43 Resp: 391210  
Ion Ratio Lower Upper  
43 100  
58 49.0 24.9 74.6

### Manual Integrations APPROVED



Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025


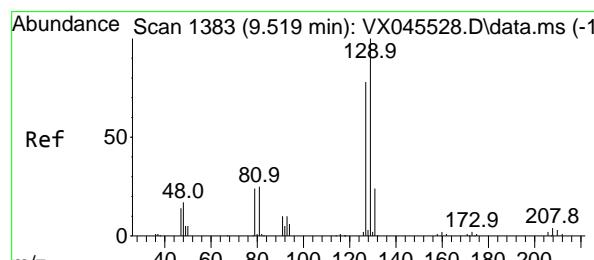
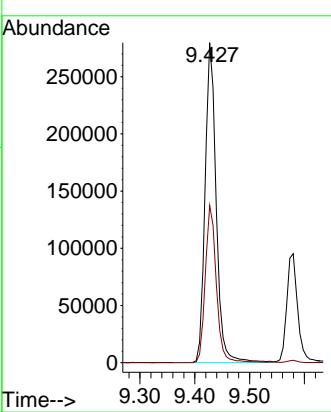


#60  
Dibromochloromethane  
Concen: 55.012 ug/l  
RT: 9.519 min Scan# 1383  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

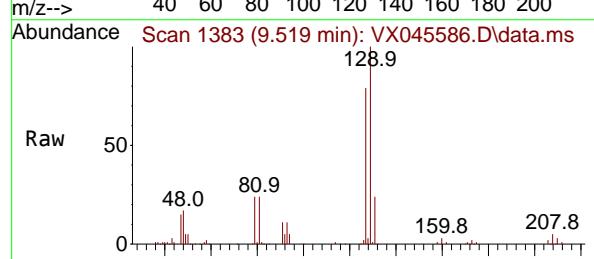

Tgt Ion:129 Resp: 69085  
Ion Ratio Lower Upper  
129 100  
127 76.1 39.4 118.2

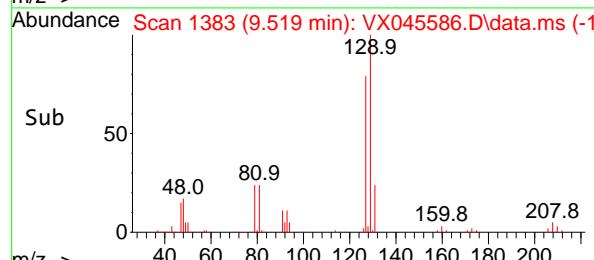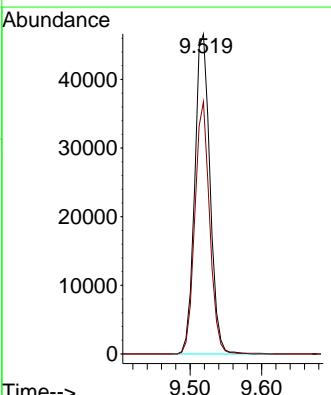

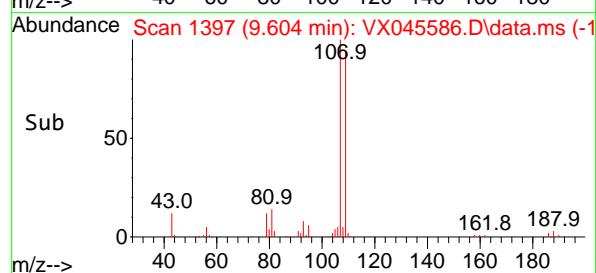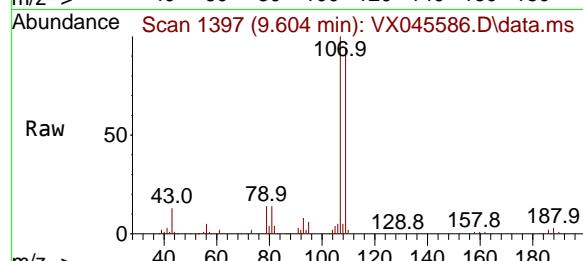

#61

1,2-Dibromoethane

Concen: 53.230 ug/l

RT: 9.604 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#62

4-Bromofluorobenzene

Concen: 45.563 ug/l


RT: 11.079 min Scan# 1639


Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt	Ion	Resp:	67111
Ion	Ratio	Lower	Upper
95	100		
174	66.8	0.0	135.8
176	64.5	0.0	131.4




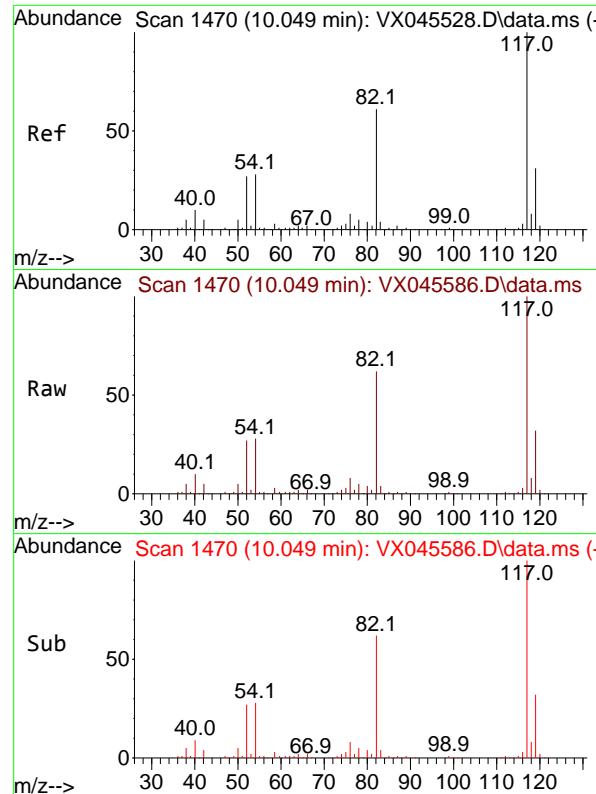


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1470  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


1 Manual Integrations  
2 APPROVED


3 Reviewed By :John Carlone 04/07/2025  
4 Supervised By :Mahesh Dadoda 04/07/2025

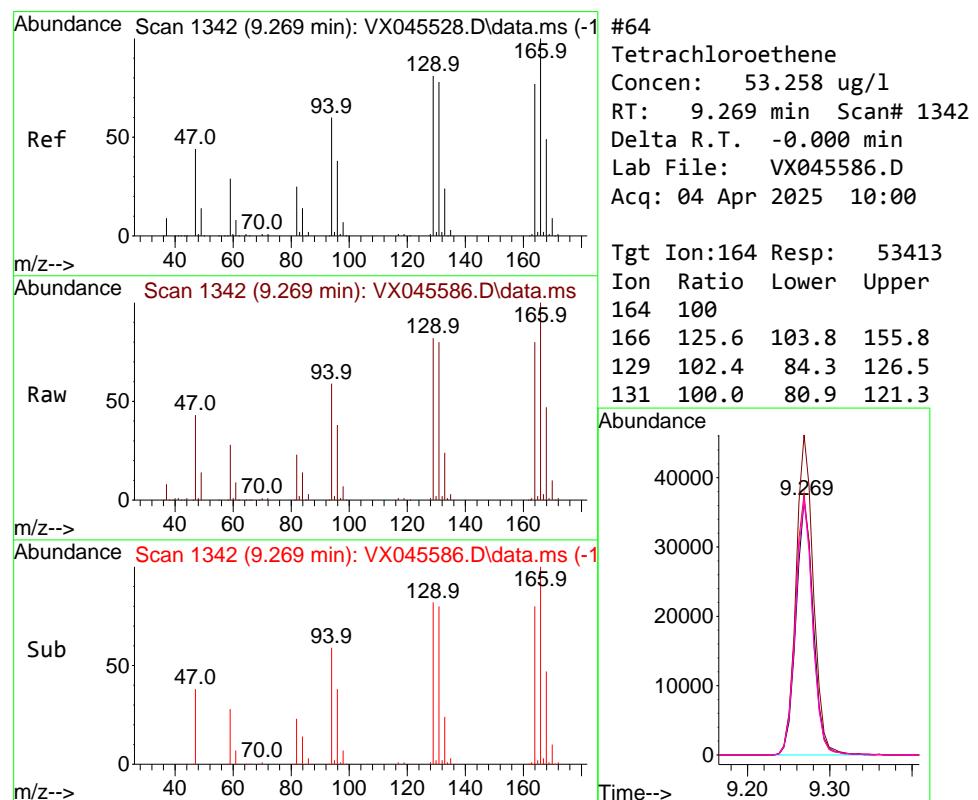

#64  
Tetrachloroethene  
Concen: 53.258 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion:164 Resp: 53413  
Ion Ratio Lower Upper  
164 100  
166 125.6 103.8 155.8  
129 102.4 84.3 126.5  
131 100.0 80.9 121.3




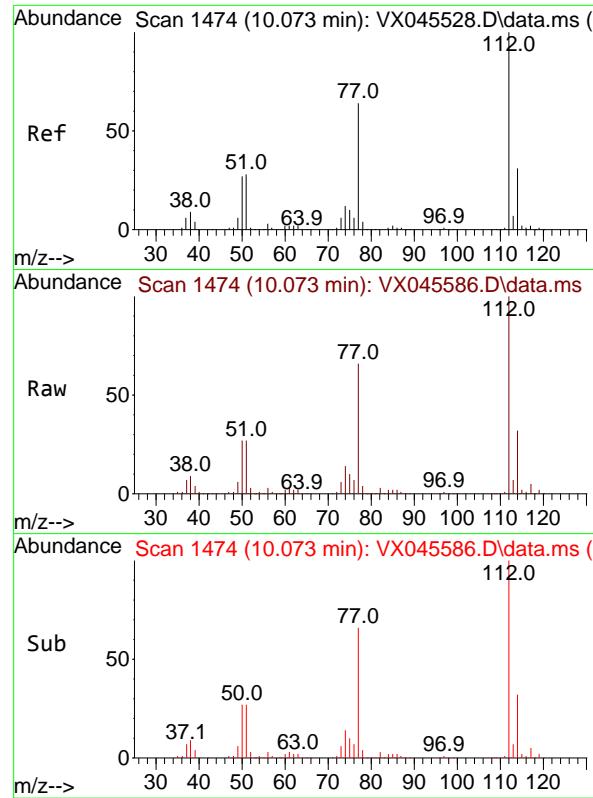


#65  
Chlorobenzene  
Concen: 53.041 ug/l  
RT: 10.073 min Scan# 1474  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

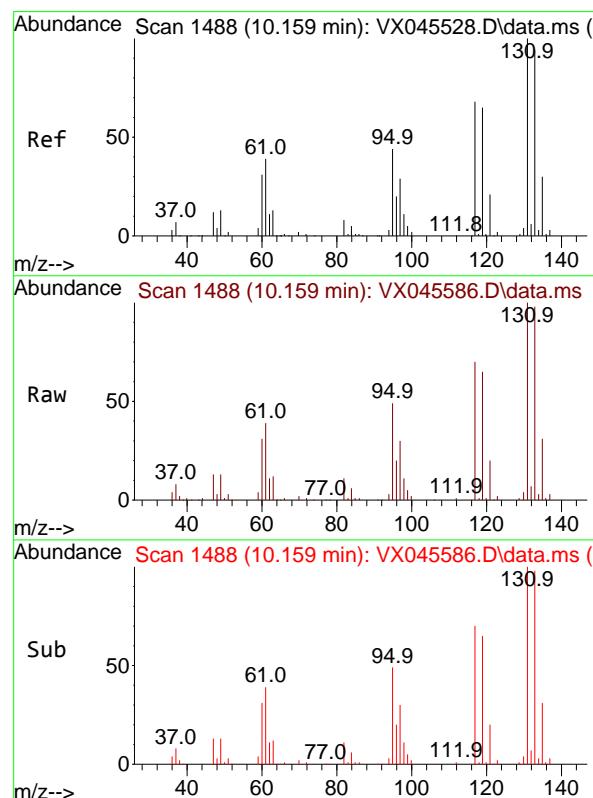

#66  
1,1,1,2-Tetrachloroethane  
Concen: 52.492 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion:131 Resp: 55317  
Ion Ratio Lower Upper  
131 100  
133 96.5 47.5 142.5  
119 64.9 32.9 98.6

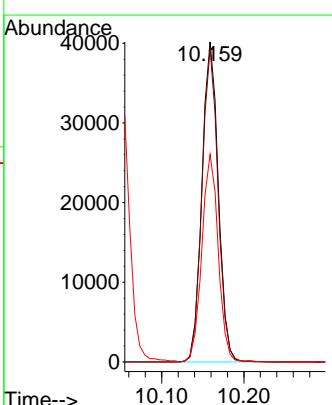



#67

Ethyl Benzene

Concen: 54.700 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X




ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#68

m/p-Xylenes

Concen: 109.636 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00




Tgt Ion:106 Resp: 216775

Ion Ratio Lower Upper

106 100

91 218.4 172.6 258.8

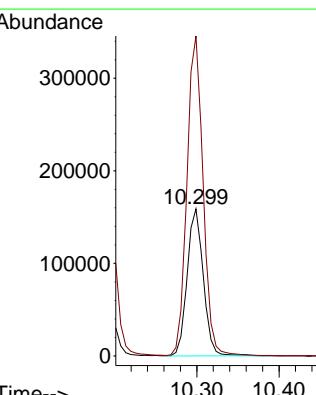




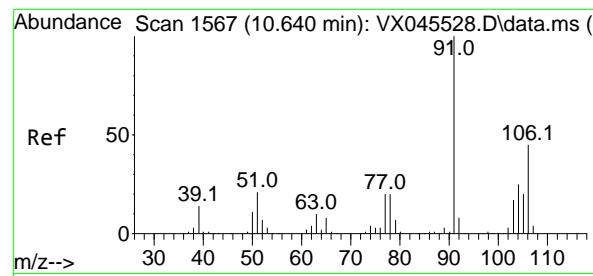


#69  
o-Xylene  
Concen: 54.386 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

ClientSampleId : VSTDCCC050


Manual Integrations  
**APPROVED**




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

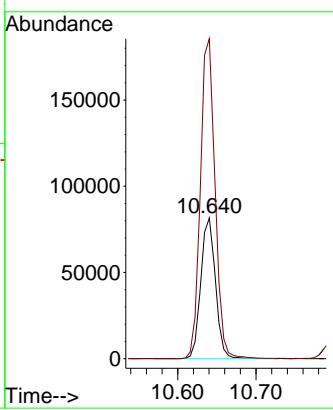

#70  
Styrene  
Concen: 55.886 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion:104 Resp: 179659  
Ion Ratio Lower Upper  
104 100  
78 57.9 45.4 68.2  
103 54.6 43.8 65.8





#71

Bromoform

Concen: 55.486 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00


Tgt Ion:152 Resp: 67379


Ion Ratio Lower Upper

152 100

115 95.7 46.9 140.7

150 173.4 0.0 349.4



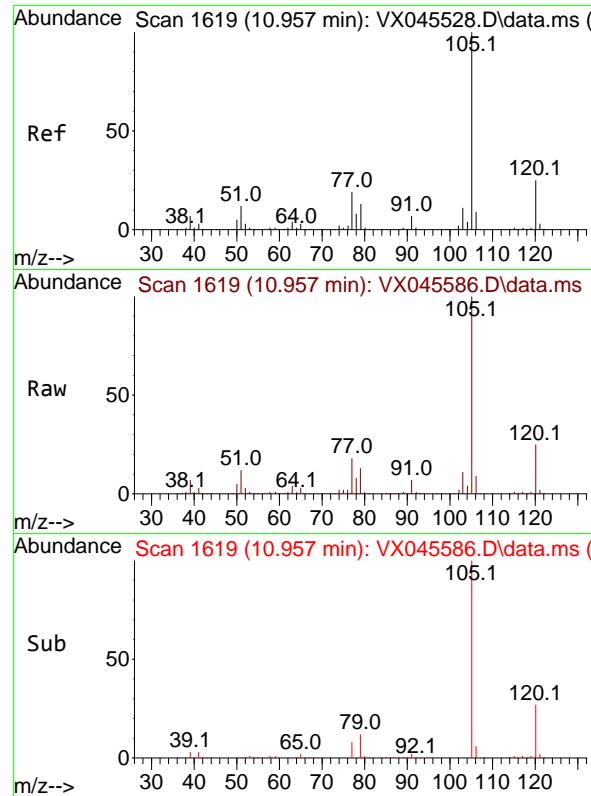

#73

Isopropylbenzene

Concen: 53.453 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

Abundance

105.1

120.1

100

120 25.4 12.7 38.0

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper


105 100

120 25.4 12.7 38.0

Ion:105 Resp: 28849

Tgt Ion:105 Resp: 28849

Ion Ratio Lower Upper

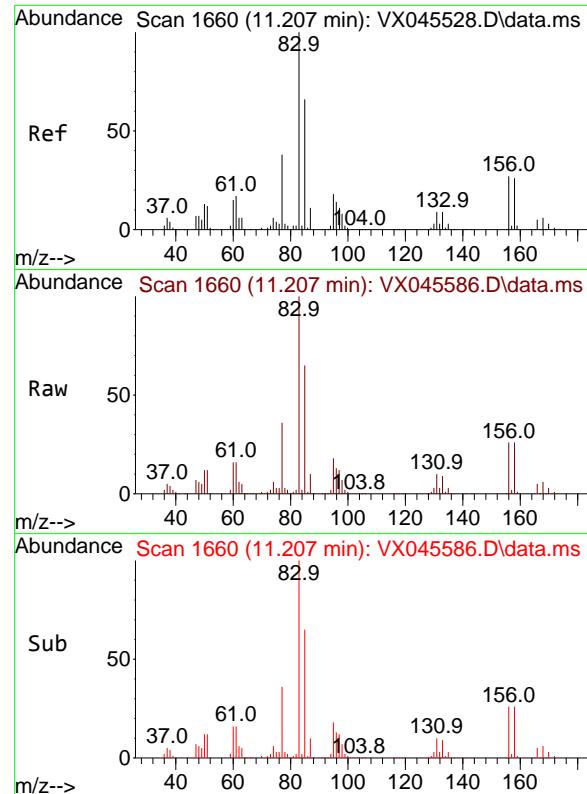


#75  
1,1,2,2-Tetrachloroethane  
Concen: 48.021 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument: MSVOA\_X  
ClientSampleId: VSTDCCC050


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

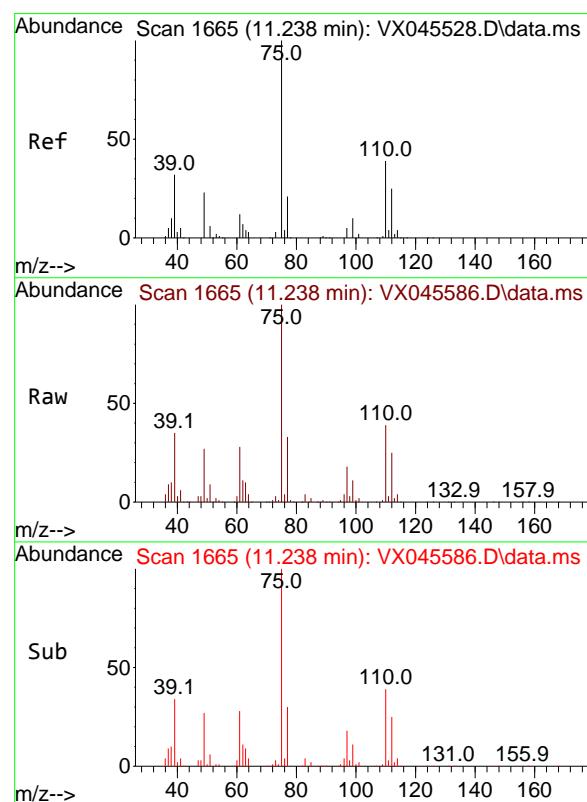

#76  
1,2,3-Trichloropropane  
Concen: 49.496 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion: 75 Resp: 81348  
Ion Ratio Lower Upper  
75 100  
77 39.7 20.0 59.9

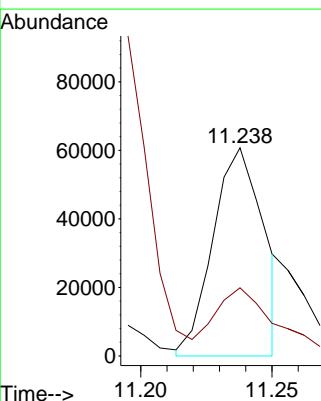

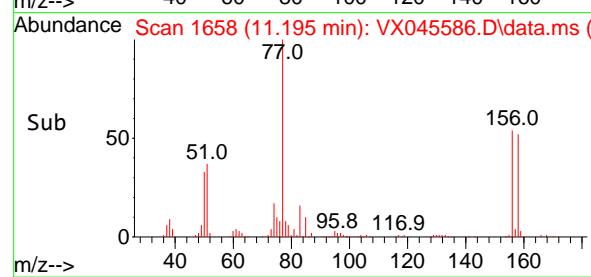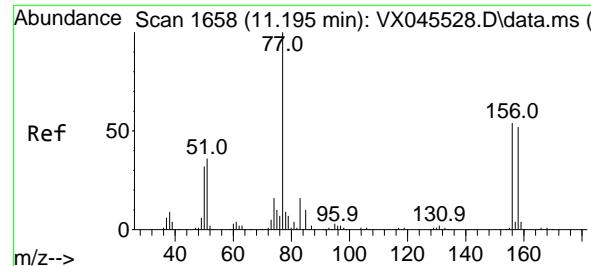

#77

Bromobenzene

Concen: 51.248 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

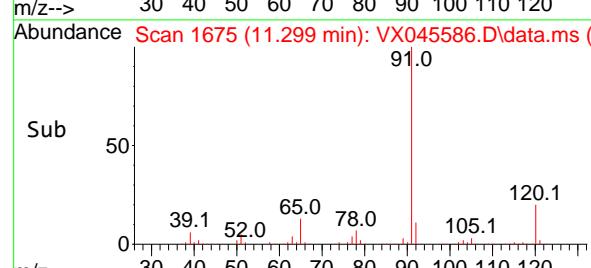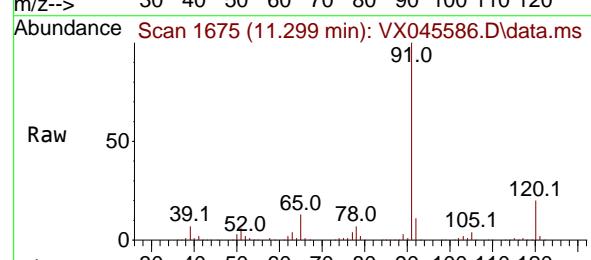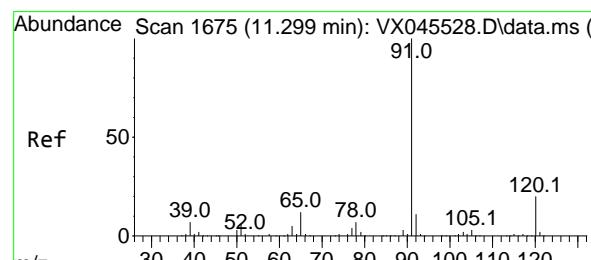

#78

n-propylbenzene

Concen: 54.351 ug/l

RT: 11.299 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00




Tgt Ion: 91 Resp: 337878

Ion Ratio Lower Upper

91 100

120 21.3 10.8 32.3

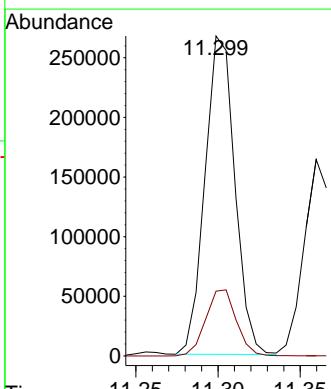



#79

2-Chlorotoluene

Concen: 51.314 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X




ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#80

1,3,5-Trimethylbenzene

Concen: 53.712 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045586.D


Acq: 04 Apr 2025 10:00


Tgt Ion:105 Resp: 239716

Ion Ratio Lower Upper

105 100

120 46.2 23.0 69.0

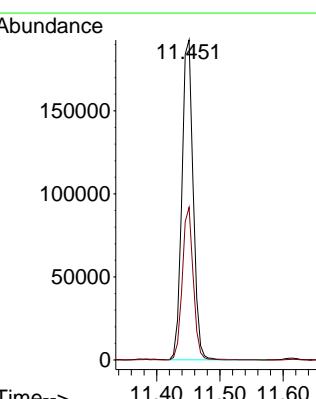


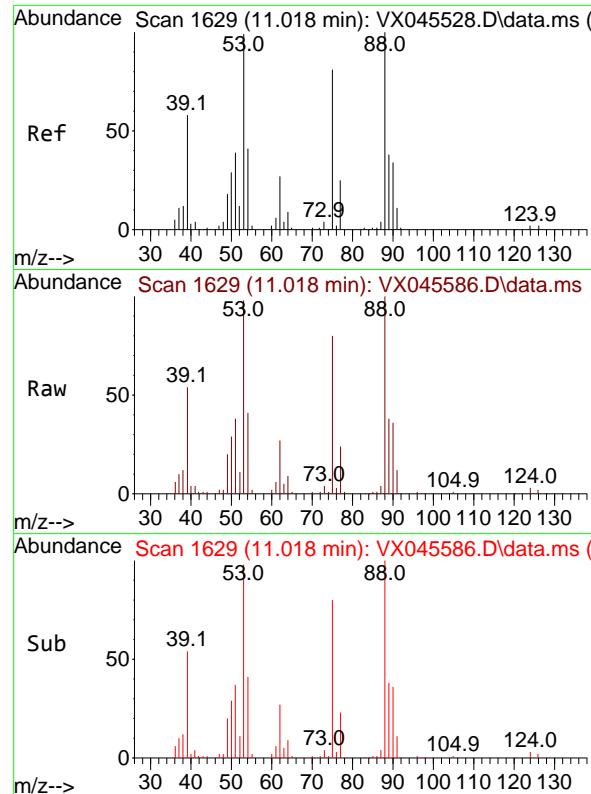


#81  
trans-1,4-Dichloro-2-butene  
Concen: 52.135 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


**Manual Integrations**  
**APPROVED**







Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

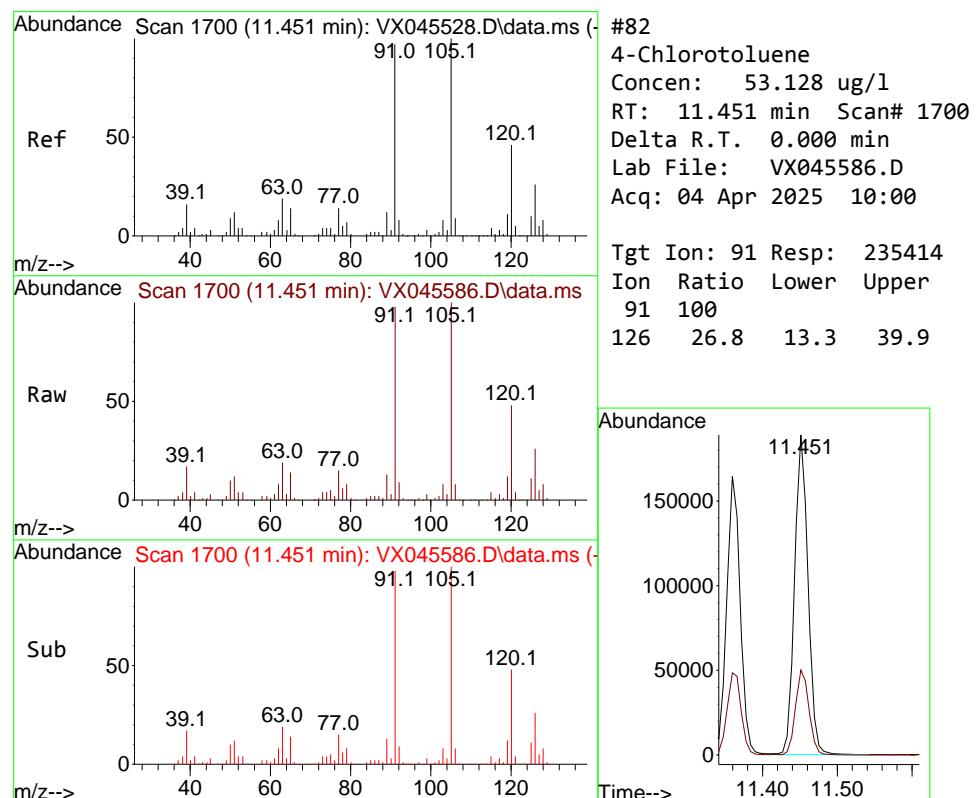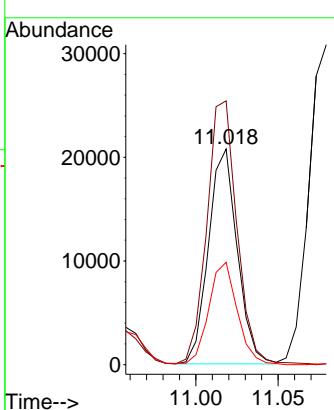

#82  
4-Chlorotoluene  
Concen: 53.128 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion: 91 Resp: 235414  
Ion Ratio Lower Upper  
91 100  
126 26.8 13.3 39.9

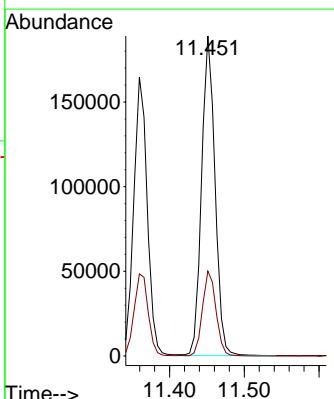



#83

tert-Butylbenzene

Concen: 53.024 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

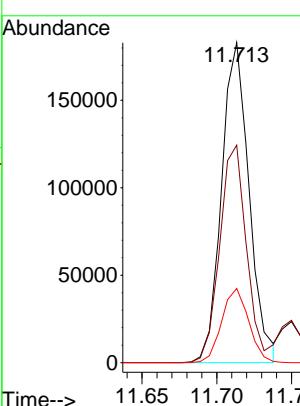

#84

1,2,4-Trimethylbenzene

Concen: 53.903 ug/l


RT: 11.750 min Scan# 1749


Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt	Ion:105	Resp:	241455
Ion	Ratio	Lower	Upper
105	100		
120	42.2	21.4	64.3

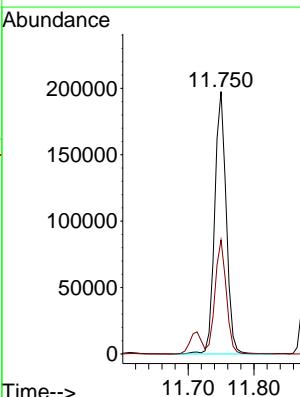

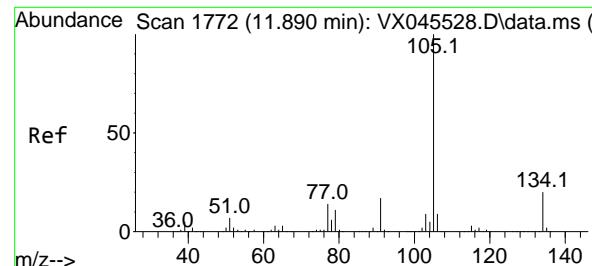





#85  
sec-Butylbenzene  
Concen: 54.969 ug/l  
RT: 11.890 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

Tgt Ion:105 Resp: 29831  
Ion Ratio Lower Upper  
105 100  
134 18.9 9.6 28.6




Manual Integrations  
**APPROVED**


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

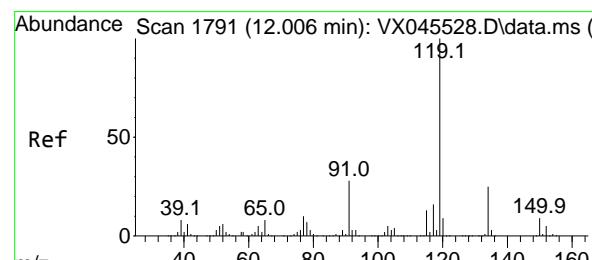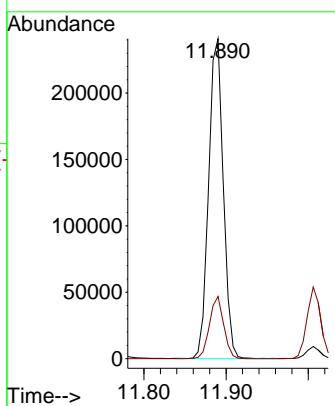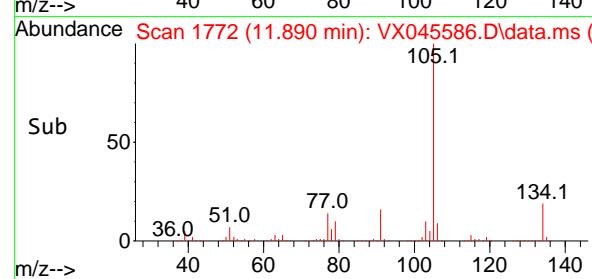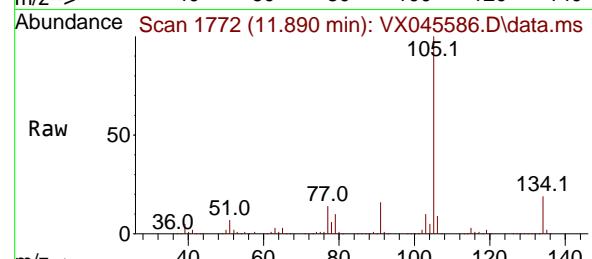

#86  
p-Isopropyltoluene  
Concen: 55.060 ug/l  
RT: 12.006 min Scan# 1791  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion:119 Resp: 246346  
Ion Ratio Lower Upper  
119 100  
134 25.4 12.6 37.8  
91 27.9 13.7 41.1

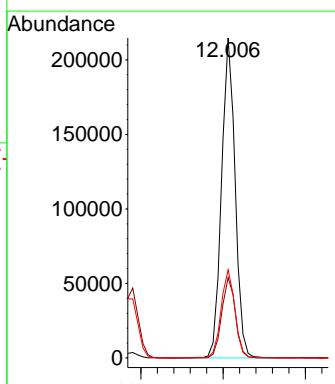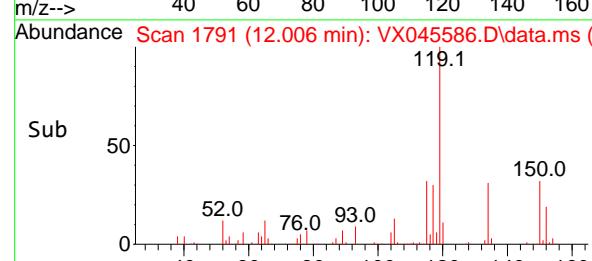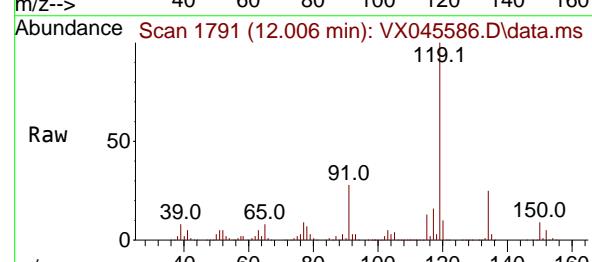

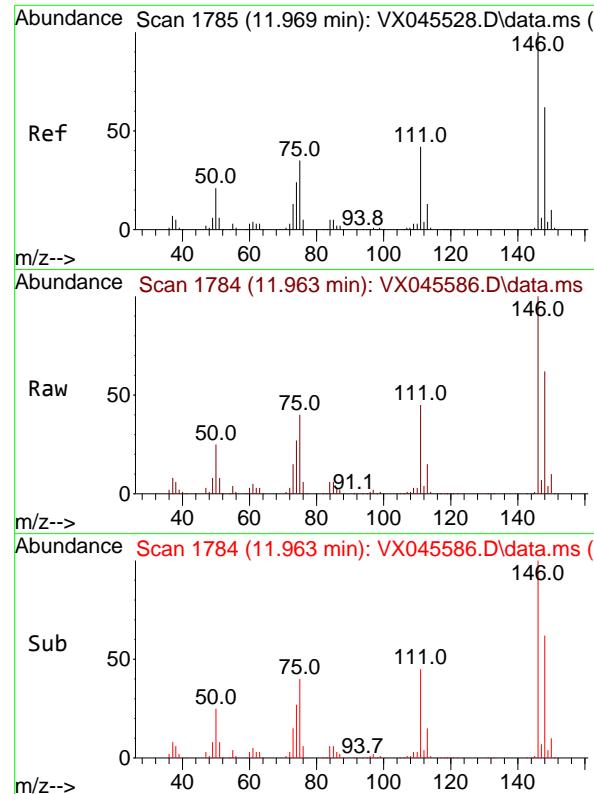

#87

1,3-Dichlorobenzene

Concen: 51.535 ug/l

RT: 11.963 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

Tgt Ion:146 Resp: 11698

Ion Ratio Lower Upper

146 100

111 44.3 22.2 66.6


148 63.6 31.9 95.7

Manual Integrations

APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#88

1,4-Dichlorobenzene

Concen: 50.768 ug/l

RT: 12.036 min Scan# 1796

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00



Tgt Ion:146 Resp: 116831




Ion Ratio Lower Upper

146 100

111 42.3 20.9 62.8

148 64.5 31.5 94.5

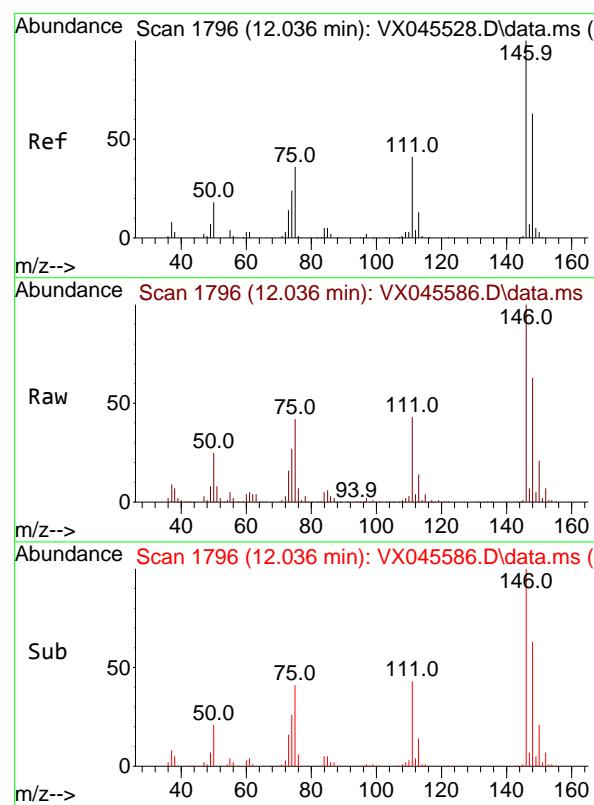



#89

n-Butylbenzene

Concen: 57.557 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

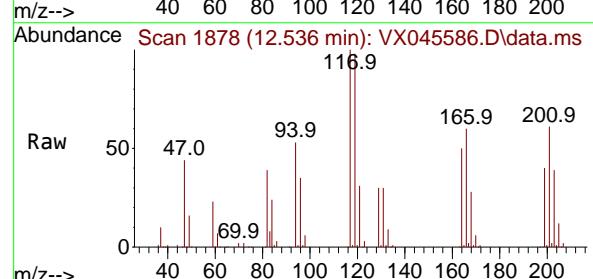

#90

Hexachloroethane

Concen: 55.342 ug/l


RT: 12.536 min Scan# 1878


Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
117	100		42554		
201	63.1	31.2	93.6		

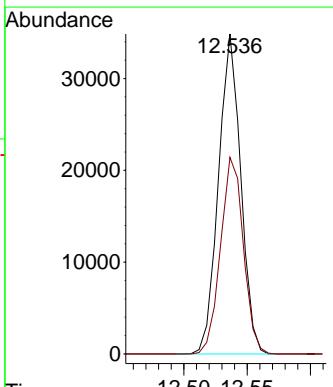

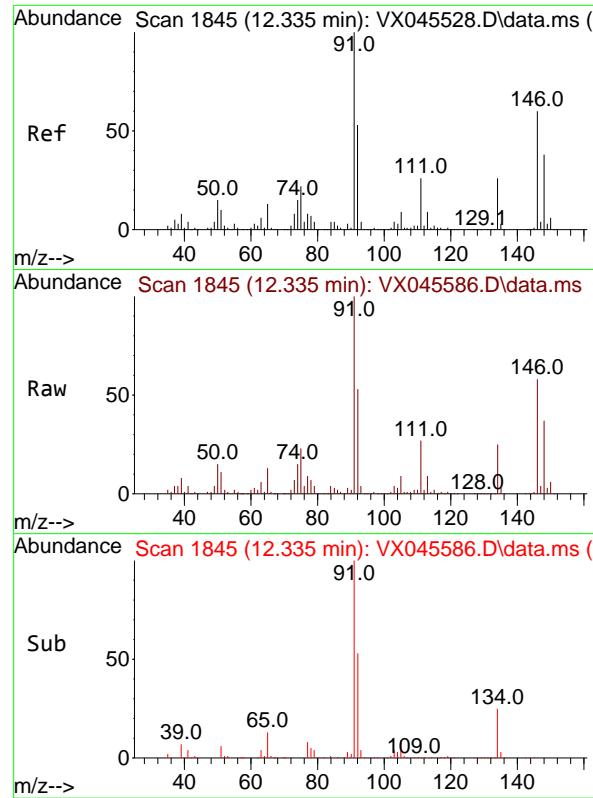

#91

1,2-Dichlorobenzene

Concen: 51.109 ug/l

RT: 12.335 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Instrument:

MSVOA\_X



ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

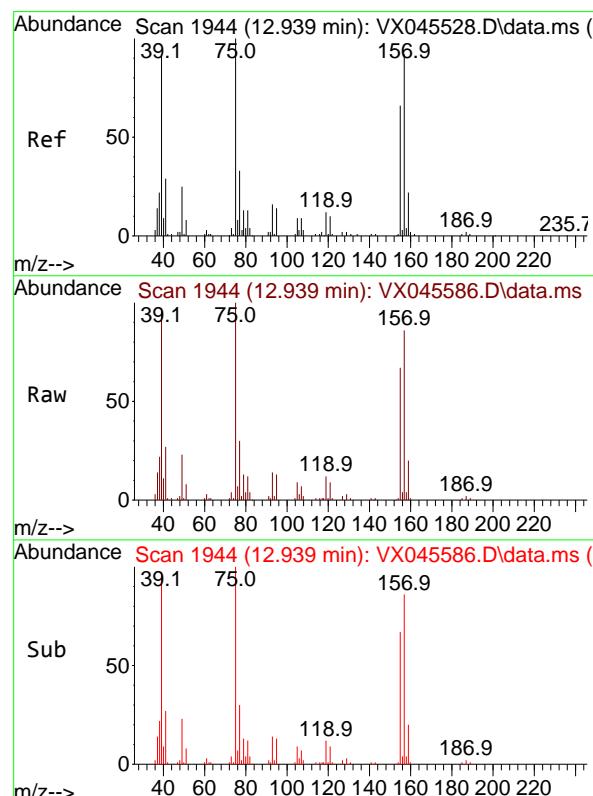

#92

1,2-Dibromo-3-Chloropropane

Concen: 53.714 ug/l


RT: 12.939 min Scan# 1944


Delta R.T. 0.000 min

Lab File: VX045586.D

Acq: 04 Apr 2025 10:00

Tgt	Ion:	75	Resp:	21298
Ion	Ratio	Lower	Upper	
	75	100		
155	69.8	34.9	104.7	
157	87.7	44.9	134.7	




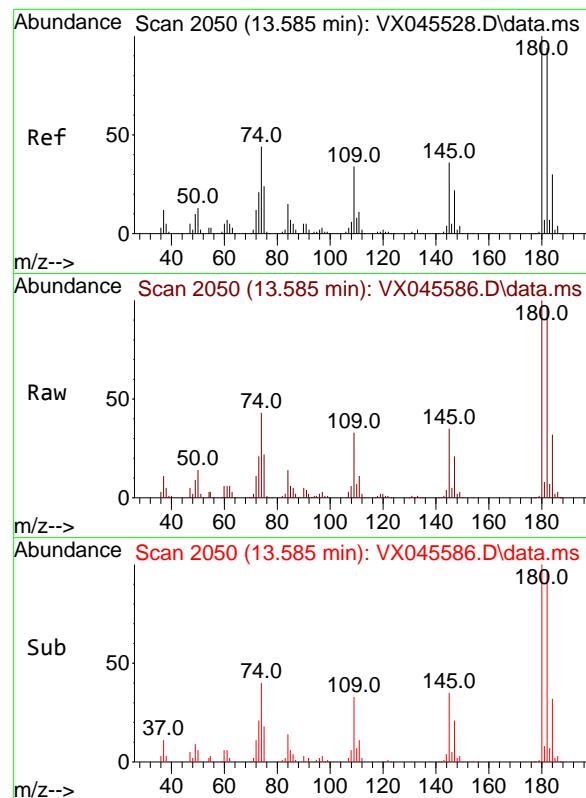


#93  
1,2,4-Trichlorobenzene  
Concen: 54.225 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

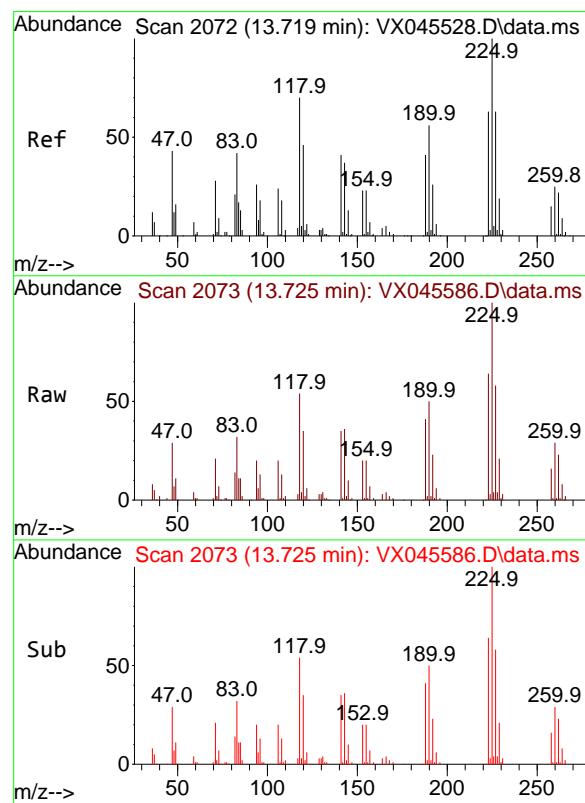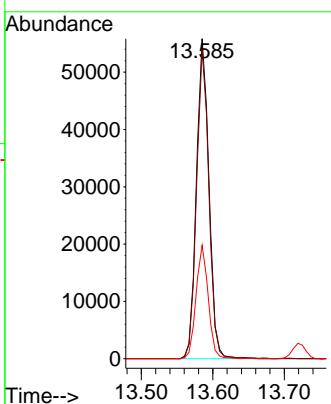

#94  
Hexachlorobutadiene  
Concen: 54.435 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. 0.006 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion:225 Resp: 29467  
Ion Ratio Lower Upper  
225 100  
223 64.2 31.1 93.3  
227 61.2 32.2 96.6

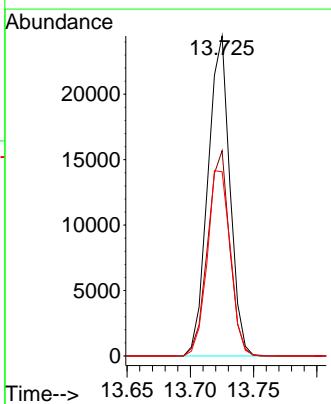


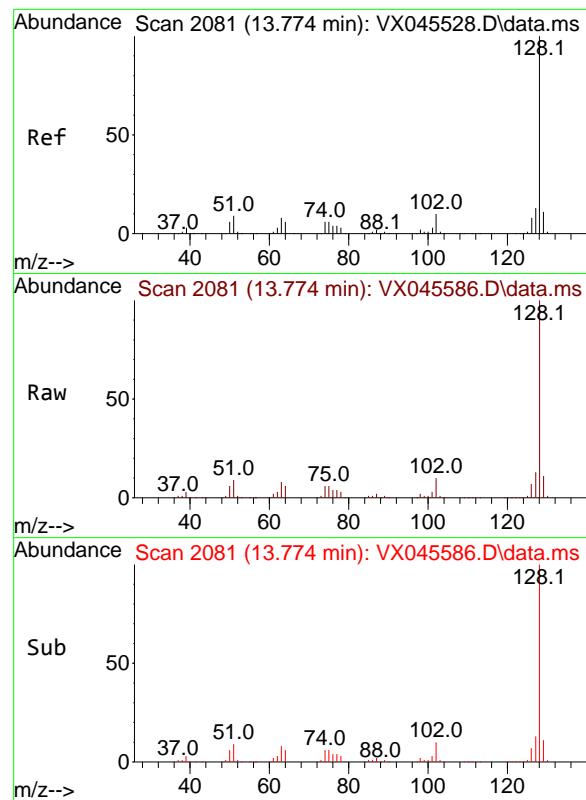


#95  
Naphthalene  
Concen: 51.558 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

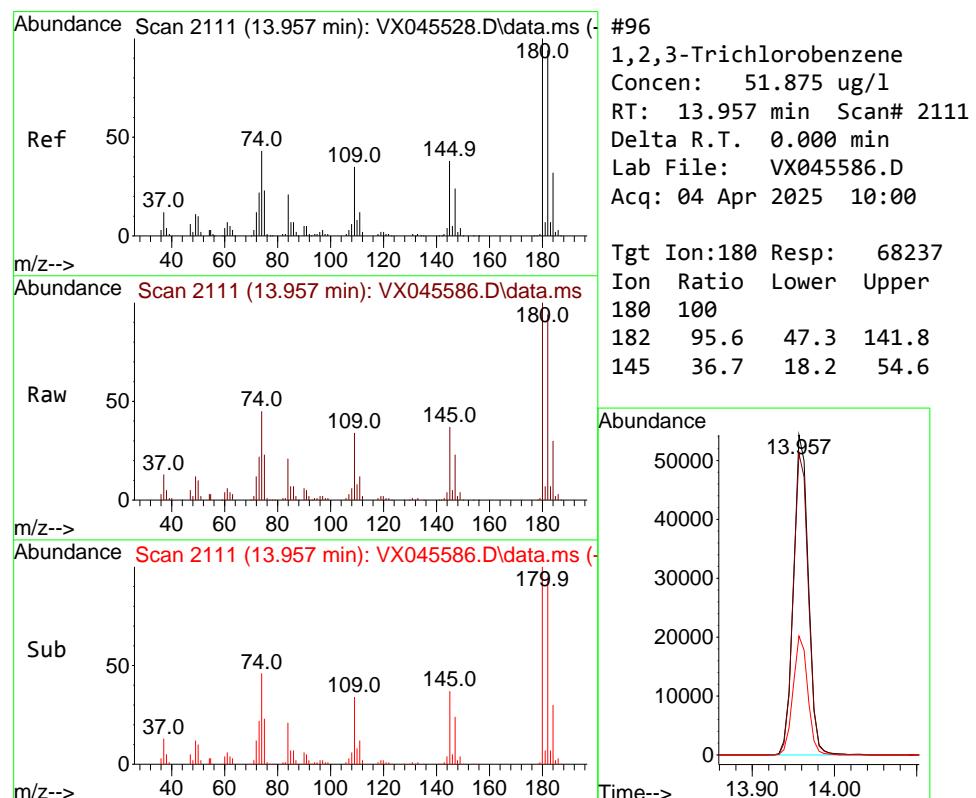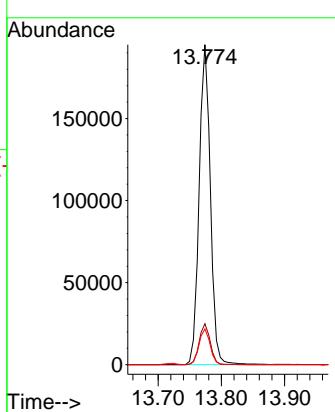

#96  
1,2,3-Trichlorobenzene  
Concen: 51.875 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX045586.D  
Acq: 04 Apr 2025 10:00

Tgt Ion:180 Resp: 68237  
Ion Ratio Lower Upper  
180 100  
182 95.6 47.3 141.8  
145 36.7 18.2 54.6

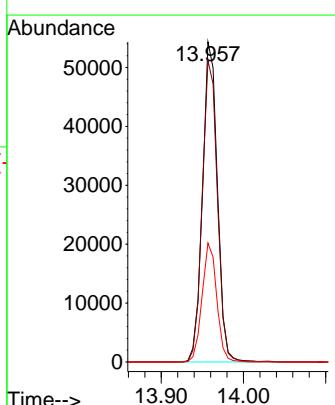

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045586.D  
 Acq On : 04 Apr 2025 10:00  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Apr 04 23:10:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	101	-0.01
2 T	Dichlorodifluoromethane	0.748	0.843	-12.7	104	0.00
3 P	Chloromethane	0.768	0.797	-3.8	103	0.00
4 C	Vinyl Chloride	0.703	0.731	-4.0#	103	0.00
5 T	Bromomethane	0.333	0.328	1.5	100	0.00
6 T	Chloroethane	0.373	0.393	-5.4	100	0.00
7 T	Trichlorofluoromethane	1.048	1.105	-5.4	103	0.00
8 T	Diethyl Ether	0.352	0.350	0.6	100	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.614	0.658	-7.2	107	0.00
10 T	Methyl Iodide	0.766	0.770	-0.5	97	0.00
11 T	Tert butyl alcohol	0.123	0.118	4.1	94	0.00
12 CM	1,1-Dichloroethene	0.600	0.599	0.2#	100	0.00
13 T	Acrolein	0.169	0.199	-17.8	121	0.00
14 T	Allyl chloride	1.139	1.176	-3.2	101	0.00
15 T	Acrylonitrile	0.388	0.386	0.5	96	0.00
16 T	Acetone	0.375	0.368	1.9	99	0.00
17 T	Carbon Disulfide	1.483	1.500	-1.1	98	0.00
18 T	Methyl Acetate	0.864	0.855	1.0	101	0.00
19 T	Methyl tert-butyl Ether	2.100	2.104	-0.2	100	0.00
20 T	Methylene Chloride	0.703	0.694	1.3	99	0.00
21 T	trans-1,2-Dichloroethene	0.613	0.609	0.7	99	0.00
22 T	Diisopropyl ether	2.243	2.282	-1.7	101	0.00
23 T	Vinyl Acetate	1.938	2.017	-4.1	98	0.00
24 P	1,1-Dichloroethane	1.269	1.270	-0.1	101	0.00
25 T	2-Butanone	0.550	0.550	0.0	95	0.00
26 T	2,2-Dichloropropane	0.820	0.944	-15.1	113	0.00
27 T	cis-1,2-Dichloroethene	0.747	0.729	2.4	98	0.00
28 T	Bromochloromethane	0.613	0.609	0.7	103	-0.01
29 T	Tetrahydrofuran	0.356	0.348	2.2	95	0.00
30 C	Chloroform	1.306	1.315	-0.7#	101	0.00
31 T	Cyclohexane	1.122	1.136	-1.2	102	0.00
32 T	1,1,1-Trichloroethane	1.105	1.107	-0.2	101	0.00
33 S	1,2-Dichloroethane-d4	0.914	0.776	15.1	90	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	97	0.00
35 S	Dibromofluoromethane	0.355	0.311	12.4	87	0.00
36 T	1,1-Dichloropropene	0.479	0.501	-4.6	100	0.00
37 T	Ethyl Acetate	0.604	0.619	-2.5	96	0.00
38 T	Carbon Tetrachloride	0.518	0.571	-10.2	103	0.00
39 T	Methylcyclohexane	0.587	0.660	-12.4	103	0.00
40 TM	Benzene	1.463	1.507	-3.0	99	0.00
41 T	Methacrylonitrile	0.318	0.359	-12.9	99	-0.01
42 TM	1,2-Dichloroethane	0.604	0.645	-6.8	101	0.00
43 T	Isopropyl Acetate	0.915	0.965	-5.5	96	0.00
44 TM	Trichloroethene	0.348	0.357	-2.6	99	0.00
45 C	1,2-Dichloropropane	0.365	0.383	-4.9#	99	0.00
46 T	Dibromomethane	0.280	0.291	-3.9	97	0.00
47 T	Bromodichloromethane	0.560	0.597	-6.6	101	0.00
48 T	Methyl methacrylate	0.472	0.509	-7.8	97	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045586.D  
 Acq On : 04 Apr 2025 10:00  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Apr 04 23:10:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.009	0.008	11.1	87	0.00
50 S	Toluene-d8	1.238	1.079	12.8	86	0.00
51 T	4-Methyl-2-Pentanone	0.606	0.651	-7.4	95	0.00
52 CM	Toluene	0.885	0.927	-4.7#	99	0.00
53 T	t-1,3-Dichloropropene	0.467	0.527	-12.8	101	0.00
54 T	cis-1,3-Dichloropropene	0.526	0.588	-11.8	101	0.00
55 T	1,1,2-Trichloroethane	0.353	0.370	-4.8	100	0.00
56 T	Ethyl methacrylate	0.546	0.584	-7.0	94	0.00
57 T	1,3-Dichloropropane	0.614	0.646	-5.2	99	0.00
58 T	2-Chloroethyl Vinyl ether	0.276	0.283	-2.5	92	0.00
59 T	2-Hexanone	0.449	0.479	-6.7	95	0.00
60 T	Dibromochloromethane	0.385	0.423	-9.9	100	0.00
61 T	1,2-Dibromoethane	0.357	0.380	-6.4	99	0.00
62 S	4-Bromofluorobenzene	0.451	0.411	8.9	88	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	95	0.00
64 T	Tetrachloroethene	0.353	0.376	-6.5	102	0.00
65 PM	Chlorobenzene	1.068	1.133	-6.1	99	0.00
66 T	1,1,1,2-Tetrachloroethane	0.371	0.389	-4.9	99	0.00
67 C	Ethyl Benzene	1.914	2.093	-9.4#	99	0.00
68 T	m/p-Xylenes	0.696	0.763	-9.6	99	0.00
69 T	o-Xylene	0.686	0.746	-8.7	98	0.00
70 T	Styrene	1.132	1.265	-11.7	98	0.00
71 P	Bromoform	0.277	0.307	-10.8	98	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	98	0.00
73 T	Isopropylbenzene	4.005	4.282	-6.9	100	0.00
74 T	N-amyl acetate	1.916	1.993	-4.0	95	0.00
75 P	1,1,2,2-Tetrachloroethane	1.407	1.351	4.0	96	0.00
76 T	1,2,3-Trichloropropane	1.220	1.207	1.1	97	0.00
77 T	Bromobenzene	0.925	0.948	-2.5	99	0.00
78 T	n-propylbenzene	4.613	5.015	-8.7	100	0.00
79 T	2-Chlorotoluene	2.949	3.027	-2.6	100	0.00
80 T	1,3,5-Trimethylbenzene	3.312	3.558	-7.4	99	0.00
81 T	trans-1,4-Dichloro-2-butene	0.359	0.375	-4.5	99	0.00
82 T	4-Chlorotoluene	3.288	3.494	-6.3	99	0.00
83 T	tert-Butylbenzene	3.279	3.477	-6.0	99	0.00
84 T	1,2,4-Trimethylbenzene	3.324	3.584	-7.8	100	0.00
85 T	sec-Butylbenzene	4.027	4.427	-9.9	101	0.00
86 T	p-Isopropyltoluene	3.320	3.656	-10.1	102	0.00
87 T	1,3-Dichlorobenzene	1.684	1.736	-3.1	100	0.00
88 T	1,4-Dichlorobenzene	1.708	1.734	-1.5	100	0.00
89 T	n-Butylbenzene	2.879	3.314	-15.1	103	0.00
90 T	Hexachloroethane	0.571	0.632	-10.7	104	0.00
91 T	1,2-Dichlorobenzene	1.675	1.712	-2.2	100	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.294	0.316	-7.5	98	0.00
93 T	1,2,4-Trichlorobenzene	0.932	1.011	-8.5	105	0.00
94 T	Hexachlorobutadiene	0.402	0.437	-8.7	106	0.00
95 T	Naphthalene	3.469	3.577	-3.1	94	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
Data File : VX045586.D  
Acq On : 04 Apr 2025 10:00  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
LabSampleId :  
VSTDCCC050

Quant Time: Apr 04 23:10:00 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	0.976	1.013	-3.8	99	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045586.D  
 Acq On : 04 Apr 2025 10:00  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Apr 04 23:10:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	101	-0.01
2 T	Dichlorodifluoromethane	50.000	56.382	-12.8	104	0.00
3 P	Chloromethane	50.000	51.883	-3.8	103	0.00
4 C	Vinyl Chloride	50.000	51.962	-3.9#	103	0.00
5 T	Bromomethane	50.000	49.218	1.6	100	0.00
6 T	Chloroethane	50.000	52.626	-5.3	100	0.00
7 T	Trichlorofluoromethane	50.000	52.688	-5.4	103	0.00
8 T	Diethyl Ether	50.000	49.704	0.6	100	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	53.591	-7.2	107	0.00
10 T	Methyl Iodide	50.000	50.258	-0.5	97	0.00
11 T	Tert butyl alcohol	250.000	239.188	4.3	94	0.00
12 CM	1,1-Dichloroethene	50.000	49.883	0.2#	100	0.00
13 T	Acrolein	250.000	294.566	-17.8	121	0.00
14 T	Allyl chloride	50.000	51.619	-3.2	101	0.00
15 T	Acrylonitrile	250.000	248.485	0.6	96	0.00
16 T	Acetone	250.000	245.130	1.9	99	0.00
17 T	Carbon Disulfide	50.000	50.605	-1.2	98	0.00
18 T	Methyl Acetate	50.000	49.477	1.0	101	0.00
19 T	Methyl tert-butyl Ether	50.000	50.091	-0.2	100	0.00
20 T	Methylene Chloride	50.000	49.375	1.3	99	0.00
21 T	trans-1,2-Dichloroethene	50.000	49.659	0.7	99	0.00
22 T	Diisopropyl ether	50.000	50.863	-1.7	101	0.00
23 T	Vinyl Acetate	250.000	260.190	-4.1	98	0.00
24 P	1,1-Dichloroethane	50.000	50.059	-0.1	101	0.00
25 T	2-Butanone	250.000	250.017	-0.0	95	0.00
26 T	2,2-Dichloropropane	50.000	57.558	-15.1	113	0.00
27 T	cis-1,2-Dichloroethene	50.000	48.765	2.5	98	0.00
28 T	Bromochloromethane	50.000	49.658	0.7	103	-0.01
29 T	Tetrahydrofuran	250.000	244.391	2.2	95	0.00
30 C	Chloroform	50.000	50.378	-0.8#	101	0.00
31 T	Cyclohexane	50.000	50.650	-1.3	102	0.00
32 T	1,1,1-Trichloroethane	50.000	50.113	-0.2	101	0.00
33 S	1,2-Dichloroethane-d4	50.000	42.428	15.1	90	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	97	0.00
35 S	Dibromofluoromethane	50.000	43.879	12.2	87	0.00
36 T	1,1-Dichloropropene	50.000	52.336	-4.7	100	0.00
37 T	Ethyl Acetate	50.000	51.305	-2.6	96	0.00
38 T	Carbon Tetrachloride	50.000	55.161	-10.3	103	0.00
39 T	Methylcyclohexane	50.000	56.163	-12.3	103	0.00
40 TM	Benzene	50.000	51.517	-3.0	99	0.00
41 T	Methacrylonitrile	50.000	56.425	-12.8	99	-0.01
42 TM	1,2-Dichloroethane	50.000	53.340	-6.7	101	0.00
43 T	Isopropyl Acetate	50.000	52.737	-5.5	96	0.00
44 TM	Trichloroethene	50.000	51.308	-2.6	99	0.00
45 C	1,2-Dichloropropane	50.000	52.514	-5.0#	99	0.00
46 T	Dibromomethane	50.000	52.011	-4.0	97	0.00
47 T	Bromodichloromethane	50.000	53.371	-6.7	101	0.00
48 T	Methyl methacrylate	50.000	53.861	-7.7	97	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045586.D  
 Acq On : 04 Apr 2025 10:00  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Apr 04 23:10:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	972.308	2.8	87	0.00
50 S	Toluene-d8	50.000	43.586	12.8	86	0.00
51 T	4-Methyl-2-Pentanone	250.000	268.424	-7.4	95	0.00
52 CM	Toluene	50.000	52.369	-4.7#	99	0.00
53 T	t-1,3-Dichloropropene	50.000	49.056	1.9	101	0.00
54 T	cis-1,3-Dichloropropene	50.000	55.919	-11.8	101	0.00
55 T	1,1,2-Trichloroethane	50.000	52.506	-5.0	100	0.00
56 T	Ethyl methacrylate	50.000	53.447	-6.9	94	0.00
57 T	1,3-Dichloropropane	50.000	52.594	-5.2	99	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	256.573	-2.6	92	0.00
59 T	2-Hexanone	250.000	266.730	-6.7	95	0.00
60 T	Dibromochloromethane	50.000	55.012	-10.0	100	0.00
61 T	1,2-Dibromoethane	50.000	53.230	-6.5	99	0.00
62 S	4-Bromofluorobenzene	50.000	45.563	8.9	88	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	95	0.00
64 T	Tetrachloroethene	50.000	53.258	-6.5	102	0.00
65 PM	Chlorobenzene	50.000	53.041	-6.1	99	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	52.492	-5.0	99	0.00
67 C	Ethyl Benzene	50.000	54.700	-9.4#	99	0.00
68 T	m/p-Xylenes	100.000	109.636	-9.6	99	0.00
69 T	o-Xylene	50.000	54.386	-8.8	98	0.00
70 T	Styrene	50.000	55.886	-11.8	98	0.00
71 P	Bromoform	50.000	55.486	-11.0	98	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	98	0.00
73 T	Isopropylbenzene	50.000	53.453	-6.9	100	0.00
74 T	N-amyl acetate	50.000	52.015	-4.0	95	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	48.021	4.0	96	0.00
76 T	1,2,3-Trichloropropane	50.000	49.496	1.0	97	0.00
77 T	Bromobenzene	50.000	51.248	-2.5	99	0.00
78 T	n-propylbenzene	50.000	54.351	-8.7	100	0.00
79 T	2-Chlorotoluene	50.000	51.314	-2.6	100	0.00
80 T	1,3,5-Trimethylbenzene	50.000	53.712	-7.4	99	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	52.135	-4.3	99	0.00
82 T	4-Chlorotoluene	50.000	53.128	-6.3	99	0.00
83 T	tert-Butylbenzene	50.000	53.024	-6.0	99	0.00
84 T	1,2,4-Trimethylbenzene	50.000	53.903	-7.8	100	0.00
85 T	sec-Butylbenzene	50.000	54.969	-9.9	101	0.00
86 T	p-Isopropyltoluene	50.000	55.060	-10.1	102	0.00
87 T	1,3-Dichlorobenzene	50.000	51.535	-3.1	100	0.00
88 T	1,4-Dichlorobenzene	50.000	50.768	-1.5	100	0.00
89 T	n-Butylbenzene	50.000	57.557	-15.1	103	0.00
90 T	Hexachloroethane	50.000	55.342	-10.7	104	0.00
91 T	1,2-Dichlorobenzene	50.000	51.109	-2.2	100	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	53.714	-7.4	98	0.00
93 T	1,2,4-Trichlorobenzene	50.000	54.225	-8.5	105	0.00
94 T	Hexachlorobutadiene	50.000	54.435	-8.9	106	0.00
95 T	Naphthalene	50.000	51.558	-3.1	94	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
Data File : VX045586.D  
Acq On : 04 Apr 2025 10:00  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
LabSampleId :  
VSTDCCC050

Quant Time: Apr 04 23:10:00 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	Amount	Calc.	%Dev	Area	% Dev(min)
96 T 1,2,3-Trichlorobenzene	50.000	51.875	-3.8	99	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6



# QC SAMPLE


# DATA

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040225\  
 Data File : VX045524.D  
 Acq On : 01 Apr 2025 16:15  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Title : SW846 8260  
 Last Update : Wed Apr 02 03:11:43 2025

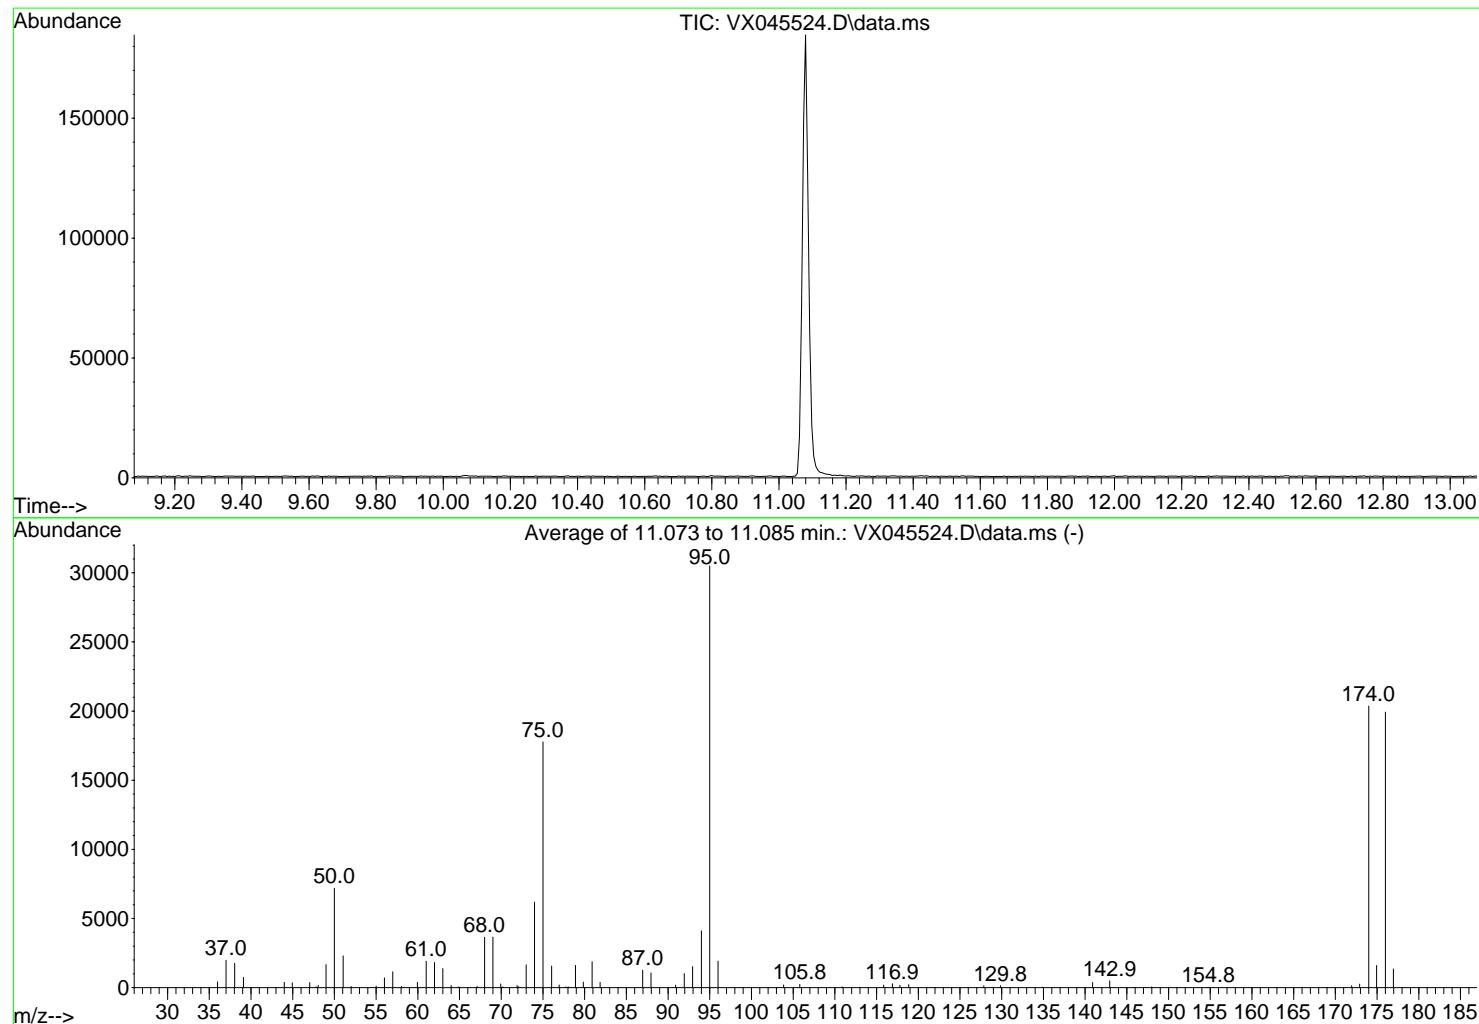

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632


Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	7184	PASS
75	95	30	60	58.2	17768	PASS
95	95	100	100	100.0	30504	PASS
96	95	5	9	6.3	1916	PASS
173	174	0.00	2	1.2	253	PASS
174	95	50	100	66.8	20365	PASS
175	174	5	9	7.8	1596	PASS
176	174	95	101	97.8	19923	PASS
177	176	5	9	6.8	1352	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045558.D  
 Acq On : 03 Apr 2025 10:01  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Title : SW846 8260  
 Last Update : Wed Apr 02 03:11:43 2025

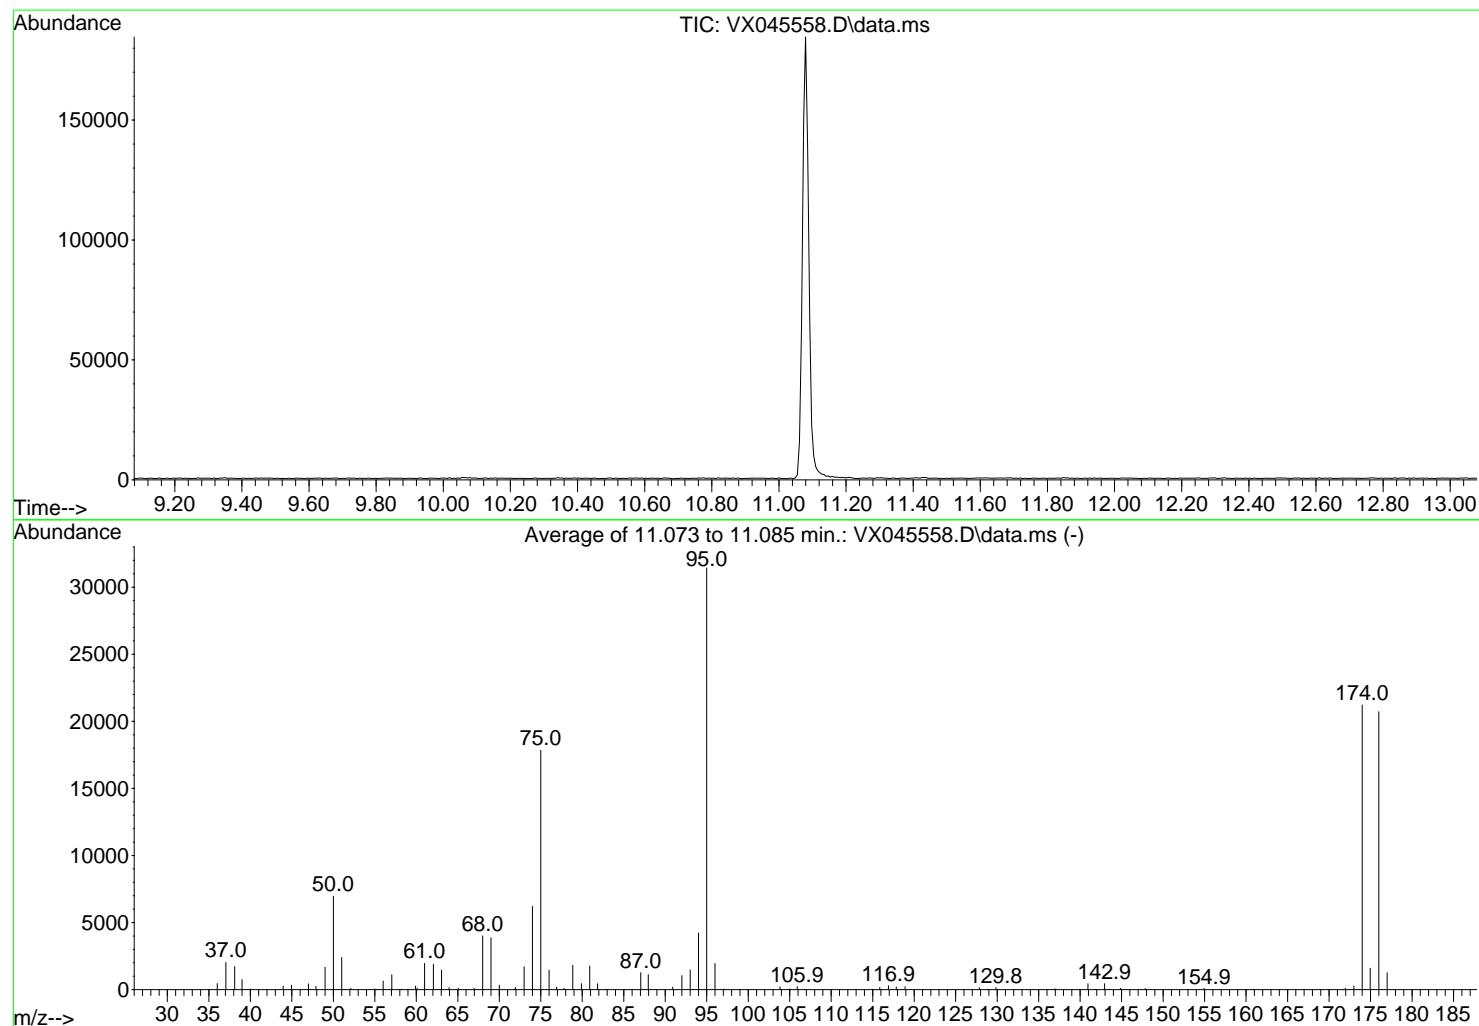

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632


Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	6965	PASS
75	95	30	60	56.7	17840	PASS
95	95	100	100	100.0	31443	PASS
96	95	5	9	6.2	1961	PASS
173	174	0.00	2	1.3	271	PASS
174	95	50	100	67.5	21221	PASS
175	174	5	9	7.5	1598	PASS
176	174	95	101	97.6	20720	PASS
177	176	5	9	6.1	1260	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045585.D  
 Acq On : 04 Apr 2025 09:31  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Title : SW846 8260  
 Last Update : Wed Apr 02 03:11:43 2025

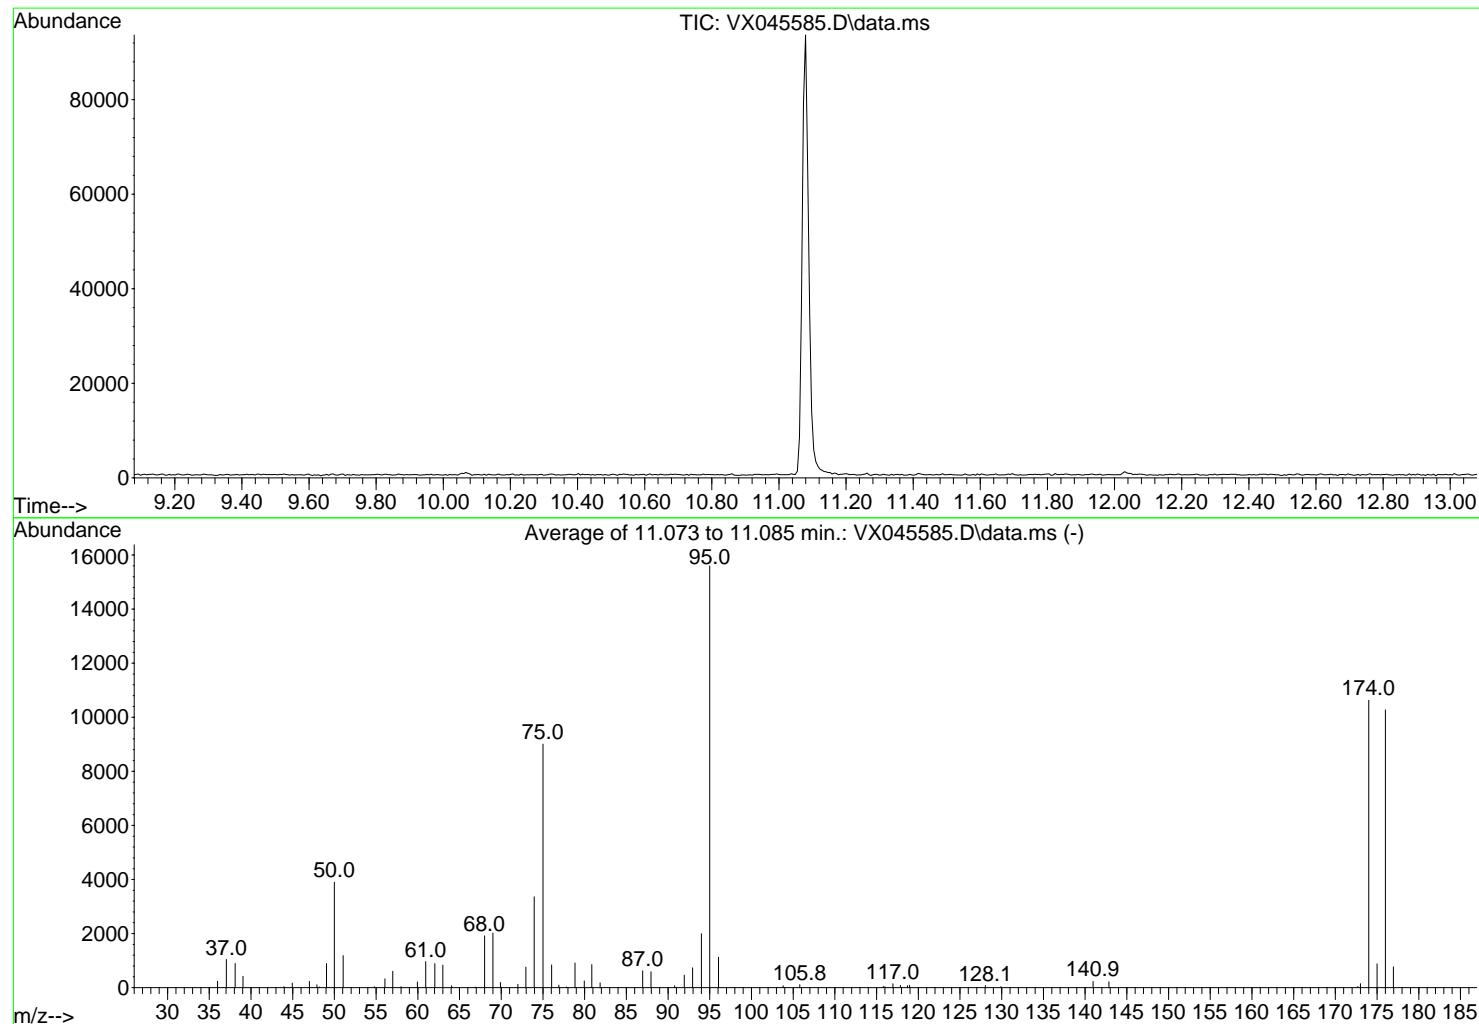

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	3902	PASS
75	95	30	60	57.7	9007	PASS
95	95	100	100	100.0	15601	PASS
96	95	5	9	7.2	1124	PASS
173	174	0.00	2	1.4	148	PASS
174	95	50	100	68.1	10629	PASS
175	174	5	9	8.3	882	PASS
176	174	95	101	96.6	10272	PASS
177	176	5	9	7.5	768	PASS



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	
Client Sample ID:	VX0403WBL01			SDG No.:	Q1711
Lab Sample ID:	VX0403WBL01			Matrix:	Water
Analytical Method:	SW8260			% Solid:	0
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000 uL
Soil Aliquot Vol:			uL	Test:	VOCMS Group3
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045561.D	1		04/03/25 11:21	VX040325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	53.2		70 (74) - 130 (125)	106%	SPK: 50
1868-53-7	Dibromofluoromethane	52.6		70 (75) - 130 (124)	105%	SPK: 50
2037-26-5	Toluene-d8	50.9		70 (86) - 130 (113)	102%	SPK: 50
460-00-4	4-Bromofluorobenzene	51.1		70 (77) - 130 (121)	102%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	66300	5.55			
540-36-3	1,4-Difluorobenzene	126000	6.757			
3114-55-4	Chlorobenzene-d5	119000	10.049			
3855-82-1	1,4-Dichlorobenzene-d4	50100	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045561.D  
 Acq On : 03 Apr 2025 11:21  
 Operator : JC/MD  
 Sample : VX0403WBL01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0403WBL01

Quant Time: Apr 04 01:18:45 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	66309	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	126206	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	118586	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	50130	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	64511	53.200	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	106.400%	
35) Dibromofluoromethane	5.379	113	47062	52.558	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	105.120%	
50) Toluene-d8	8.647	98	159136	50.917	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	101.840%	
62) 4-Bromofluorobenzene	11.079	95	58224	51.144	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	102.280%	




Target Compounds	Qvalue
(#= qualifier out of range (m) = manual integration (+) = signals summed	

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045561.D  
 Acq On : 03 Apr 2025 11:21  
 Operator : JC/MD  
 Sample : VX0403WBL01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0403WBL01





Quant Time: Apr 04 01:18:45 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

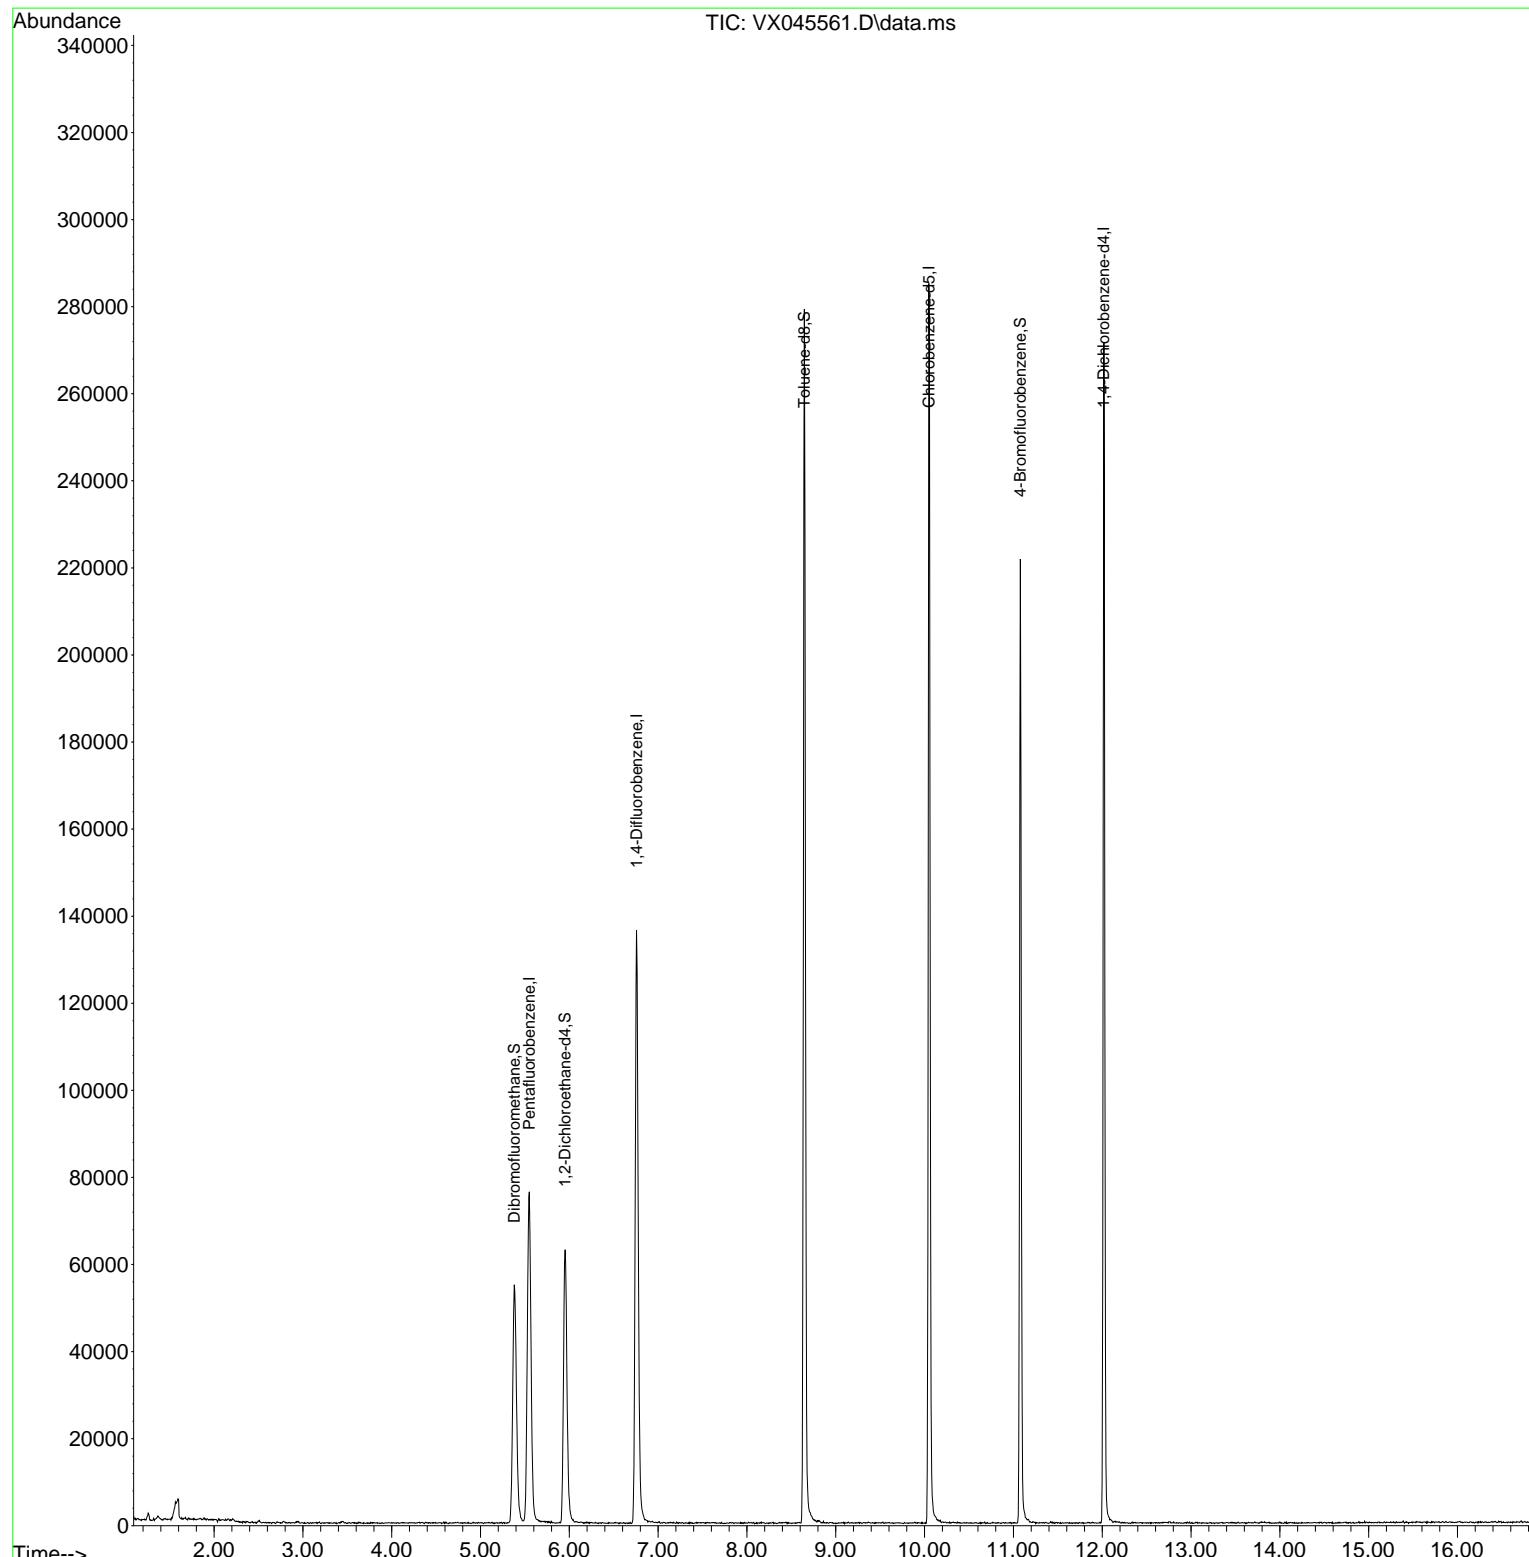




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX045561.D  
ClientSampleId : VX0403WBL01  
Acq: 03 Apr 2025 11:21




Tgt Ion:168 Resp: 66309  
Ion Ratio Lower Upper  
168 100  
99 66.2 52.3 78.5

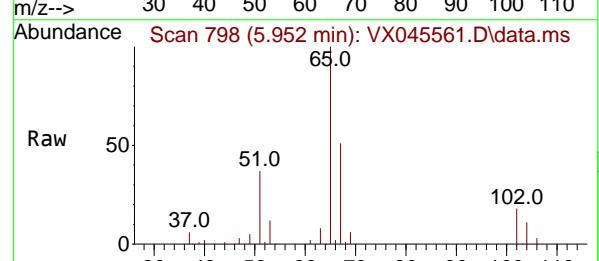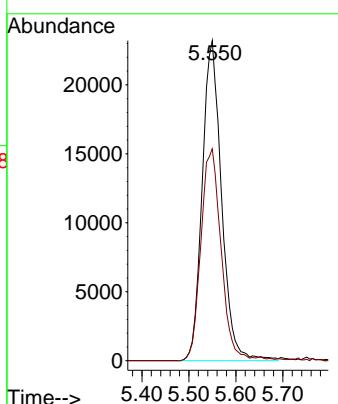

#33  
1,2-Dichloroethane-d4  
Concen: 53.200 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. -0.000 min  
Lab File: VX045561.D  
Acq: 03 Apr 2025 11:21

Tgt Ion: 65 Resp: 64511  
Ion Ratio Lower Upper  
65 100  
67 48.3 0.0 99.0

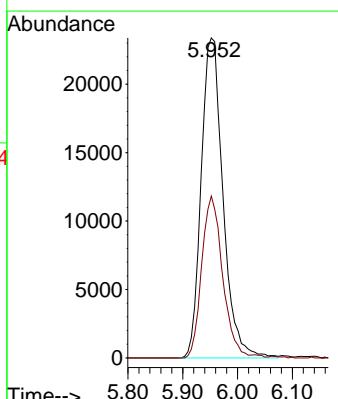



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 9

Instrument:

Delta R.T. -0.000 min

MSVOA\_X

Lab File: VX045561.D

ClientSampleId :

Acq: 03 Apr 2025 11:21

VX0403WBL01

Tgt Ion:114 Resp: 126206

Ion Ratio Lower Upper

114 100





63 22.3

0.0 46.8

88 16.7

0.0 35.4

Abundance

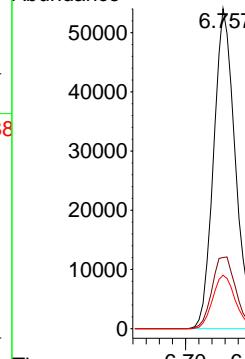

#35

Dibromofluoromethane

Concen: 52.558 ug/l

RT: 5.379 min Scan# 704

Delta R.T. -0.000 min

Lab File: VX045561.D

Acq: 03 Apr 2025 11:21

Tgt Ion:113 Resp: 47062

Ion Ratio Lower Upper

113 100


111 105.0


81.8 122.6

192 17.6


13.8 20.6

Abundance

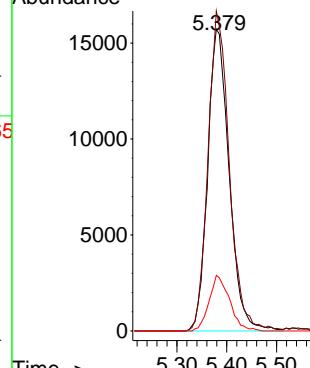




Abundance Scan 1240 (8.647 min): VX045561.D\data.ms

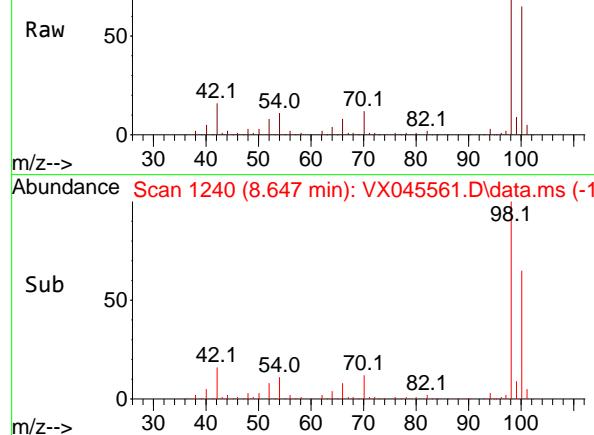

Abundance Scan 1240 (8.647 min): VX045561.D\data.ms (-1)

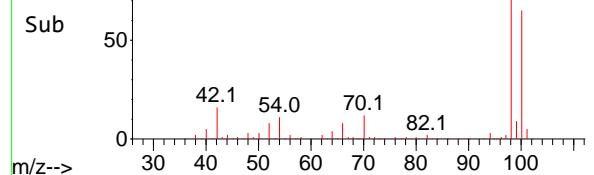

#50  
Toluene-d8  
Concen: 50.917 ug/l  
RT: 8.647 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045561.D  
Acq: 03 Apr 2025 11:21



Instrument : MSVOA\_X  
ClientSampleId : VX0403WBL01

Tgt Ion: 98 Resp: 159136


Ion Ratio Lower Upper

98 100


100 64.4 52.2 78.4

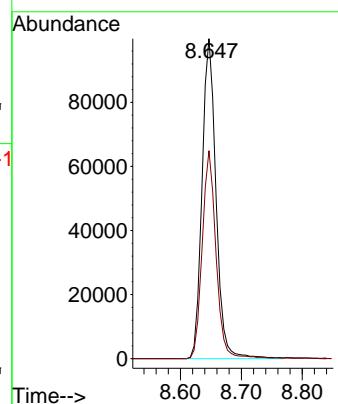

Abundance Scan 1639 (11.079 min): VX045561.D\data.ms

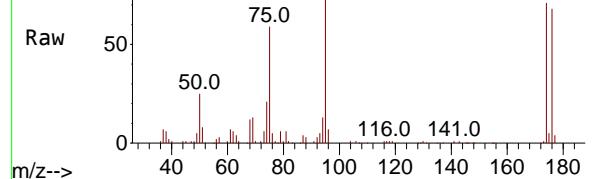

Abundance Scan 1639 (11.079 min): VX045561.D\data.ms (-1)

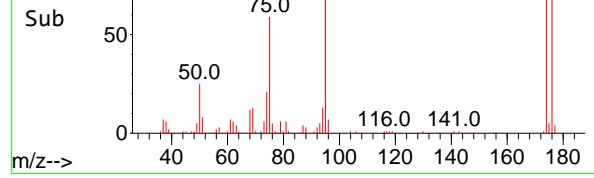

#62  
4-Bromofluorobenzene  
Concen: 51.144 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX045561.D  
Acq: 03 Apr 2025 11:21


Tgt Ion: 95 Resp: 58224


Ion Ratio Lower Upper

95 100

174 68.5 0.0 135.8



176 66.6 0.0 131.4

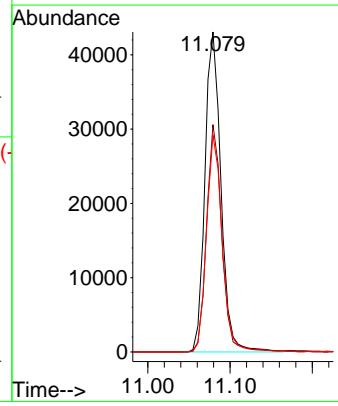

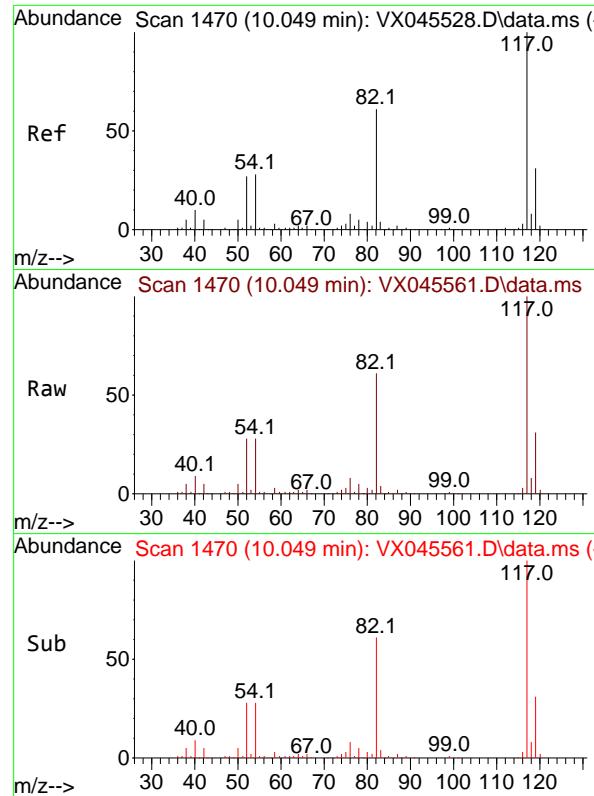


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX045561.D  
ClientSampleId : VX0403WBL01  
Acq: 03 Apr 2025 11:21

Tgt Ion:117 Resp: 118586  
Ion Ratio Lower Upper  
117 100  
82 60.7 49.2 73.8  
119 30.8 25.1 37.7

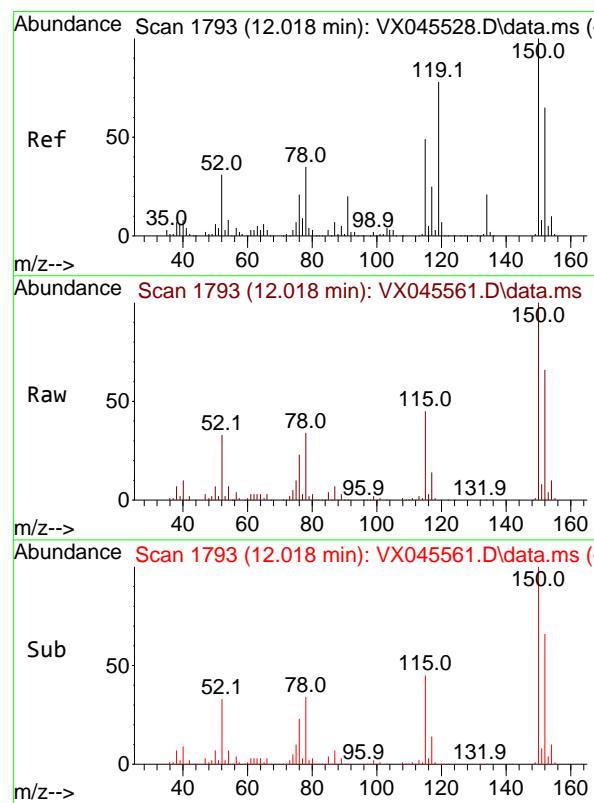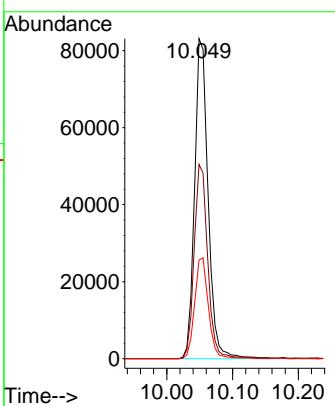

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. -0.000 min  
Lab File: VX045561.D  
Acq: 03 Apr 2025 11:21

Tgt Ion:152 Resp: 50130  
Ion Ratio Lower Upper  
152 100  
115 65.0 46.9 140.7  
150 155.1 0.0 349.4





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:
Client Sample ID:	VX0404WBL01		SDG No.:	Q1711
Lab Sample ID:	VX0404WBL01		Matrix:	Water
Analytical Method:	SW8260		% Solid:	0
Sample Wt/Vol:	5	Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group3
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045588.D	1		04/04/25 10:51	VX040425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	54.8		70 (74) - 130 (125)	110%	SPK: 50
1868-53-7	Dibromofluoromethane	52.0		70 (75) - 130 (124)	104%	SPK: 50
2037-26-5	Toluene-d8	50.8		70 (86) - 130 (113)	102%	SPK: 50
460-00-4	4-Bromofluorobenzene	49.5		70 (77) - 130 (121)	99%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	66300	5.543			
540-36-3	1,4-Difluorobenzene	129000	6.757			
3114-55-4	Chlorobenzene-d5	118000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	46000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045588.D  
 Acq On : 04 Apr 2025 10:51  
 Operator : JC/MD  
 Sample : VX0404WBL01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0404WBL01

Quant Time: Apr 04 23:10:30 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.543	168	66301	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	128686	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	118182	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	46025	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	66417	54.778	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	109.560%	
35) Dibromofluoromethane	5.379	113	47516	52.042	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	104.080%	
50) Toluene-d8	8.647	98	161989	50.831	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	101.660%	
62) 4-Bromofluorobenzene	11.079	95	57504	49.538	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	99.080%	




Target Compounds	Qvalue
(#= qualifier out of range (m) = manual integration (+) = signals summed	

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045588.D  
 Acq On : 04 Apr 2025 10:51  
 Operator : JC/MD  
 Sample : VX0404WBL01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0404WBL01

Quant Time: Apr 04 23:10:30 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration



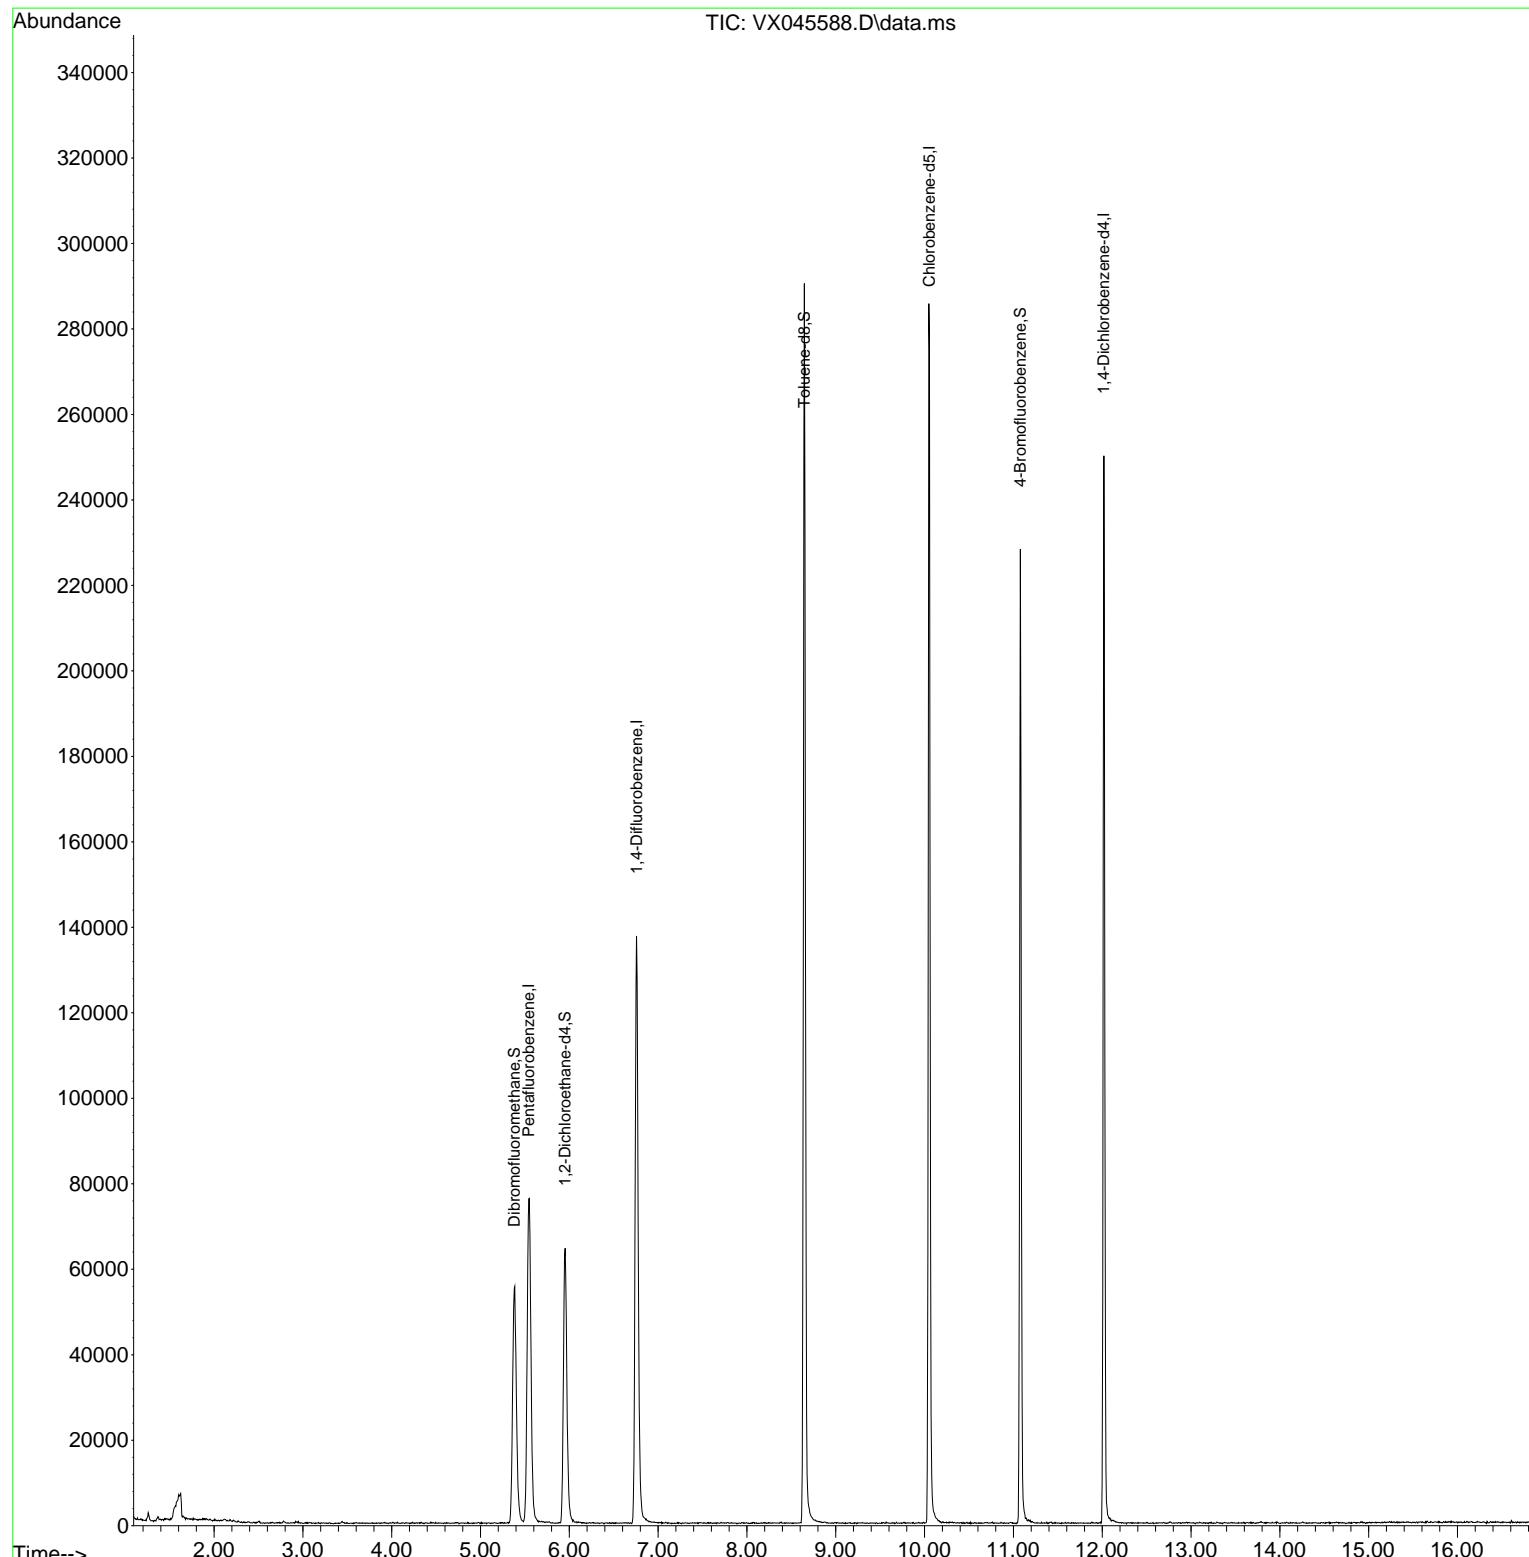




#1  
 Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.543 min Scan# 7  
 Delta R.T. -0.007 min  
 Lab File: VX045588.D  
 Acq: 04 Apr 2025 10:51



Instrument : MSVOA\_X  
 ClientSampleId : VX0404WBL01


Tgt Ion:168 Resp: 66301  
 Ion Ratio Lower Upper  
 168 100  
 99 67.3 52.3 78.5

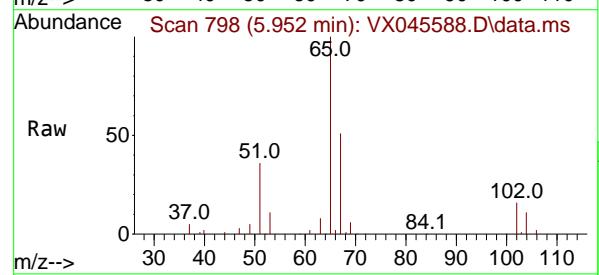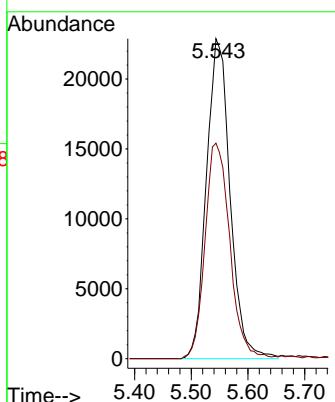

#33  
 1,2-Dichloroethane-d4  
 Concen: 54.778 ug/l  
 RT: 5.952 min Scan# 798  
 Delta R.T. -0.000 min  
 Lab File: VX045588.D  
 Acq: 04 Apr 2025 10:51



Tgt Ion: 65 Resp: 66417  
 Ion Ratio Lower Upper  
 65 100  
 67 48.8 0.0 99.0

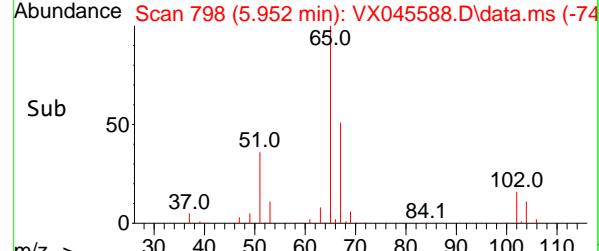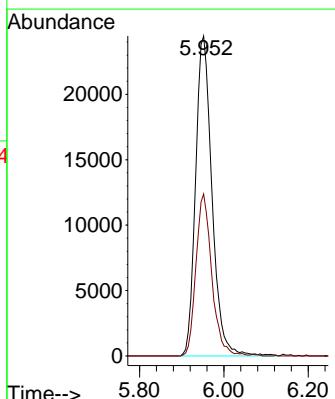

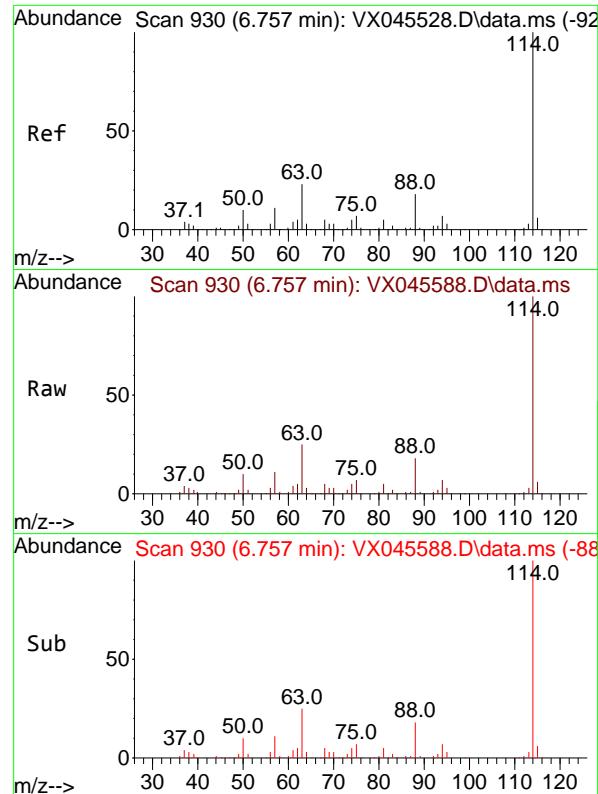


#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 9  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX045588.D  
Acq: 04 Apr 2025 10:51  
ClientSampleId : VX0404WBL01


Tgt Ion:114 Resp: 128686  
Ion Ratio Lower Upper  
114 100  
63 24.5 0.0 46.8  
88 17.7 0.0 35.4

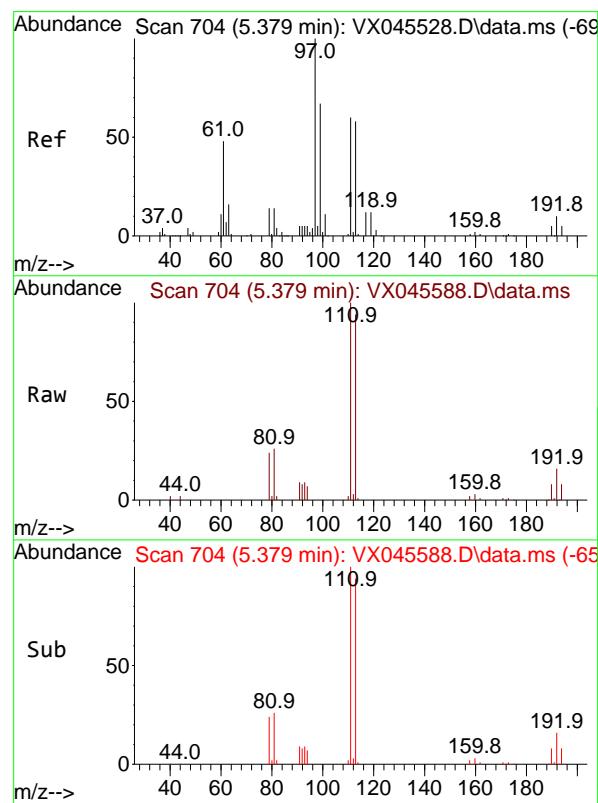

#35  
Dibromofluoromethane  
Concen: 52.042 ug/l  
RT: 5.379 min Scan# 704  
Delta R.T. -0.000 min  
Lab File: VX045588.D  
Acq: 04 Apr 2025 10:51


Tgt Ion:113 Resp: 47516  
Ion Ratio Lower Upper  
113 100  
111 103.9 81.8 122.6  
192 17.3 13.8 20.6

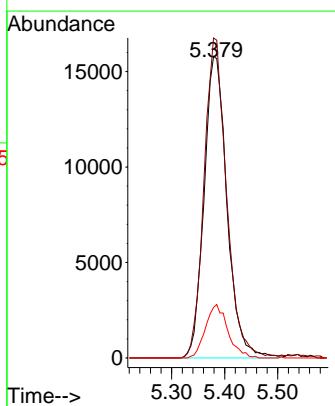



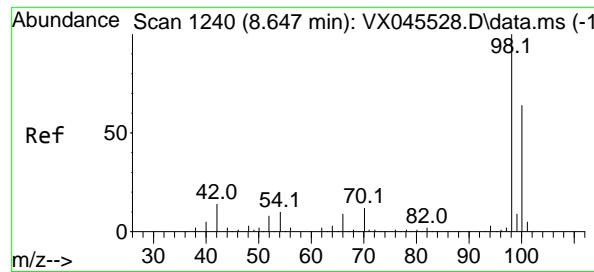


#50  
Toluene-d8  
Concen: 50.831 ug/l  
RT: 8.647 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045588.D  
Acq: 04 Apr 2025 10:51


Instrument : MSVOA\_X  
ClientSampleId : VX0404WBL01

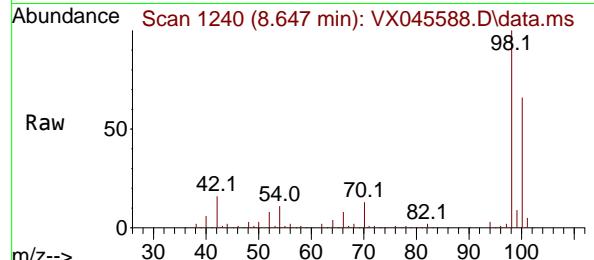



Tgt Ion: 98 Resp: 161989  
Ion Ratio Lower Upper  
98 100  
100 64.8 52.2 78.4

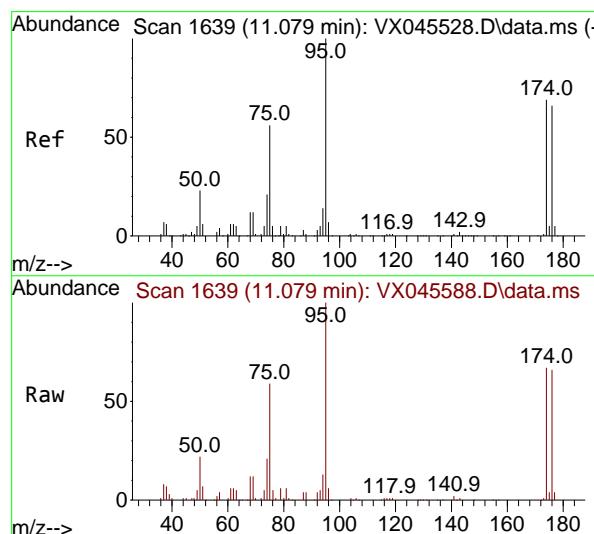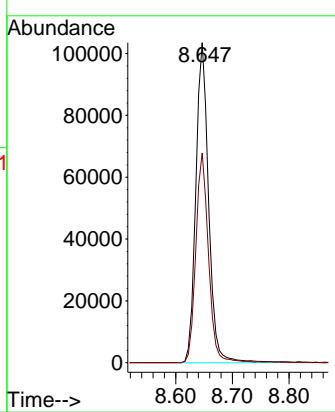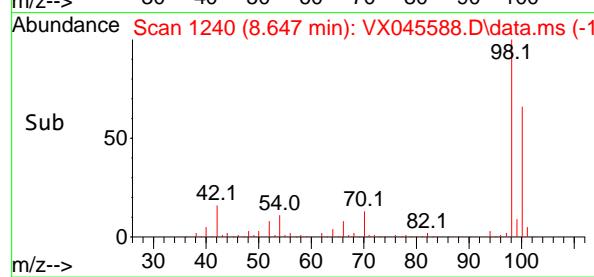


#62  
4-Bromofluorobenzene  
Concen: 49.538 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX045588.D  
Acq: 04 Apr 2025 10:51





Tgt Ion: 95 Resp: 57504  
Ion Ratio Lower Upper  
95 100  
174 68.9 0.0 135.8  
176 66.6 0.0 131.4

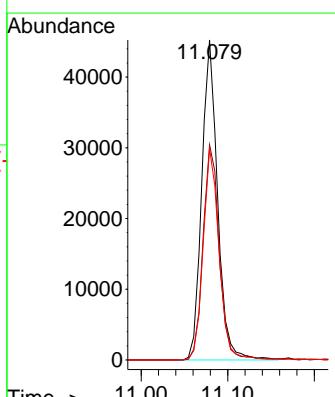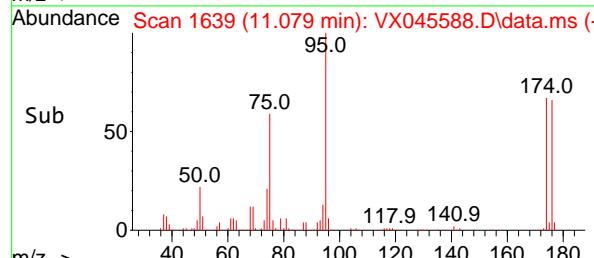

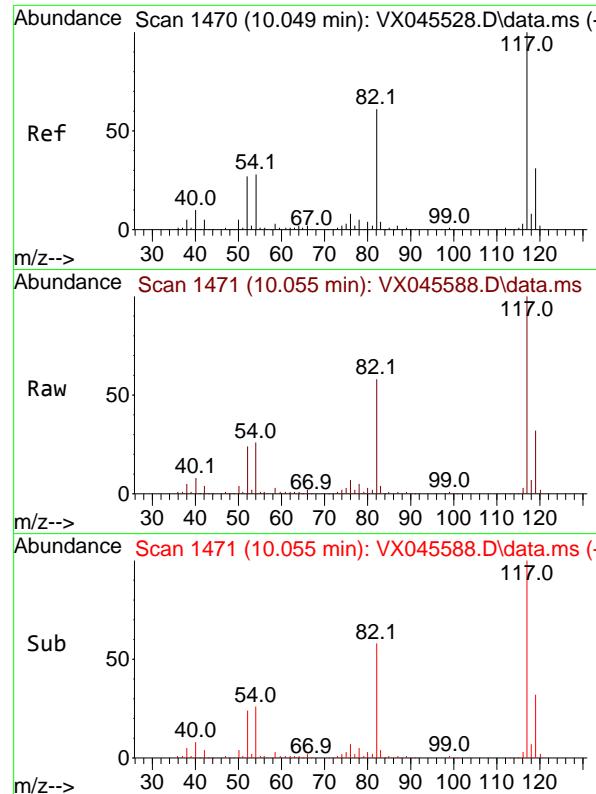


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX045588.D  
ClientSampleId : VX0404WBL01  
Acq: 04 Apr 2025 10:51

Tgt Ion:117 Resp: 118182  
Ion Ratio Lower Upper  
117 100  
82 58.3 49.2 73.8  
119 31.9 25.1 37.7

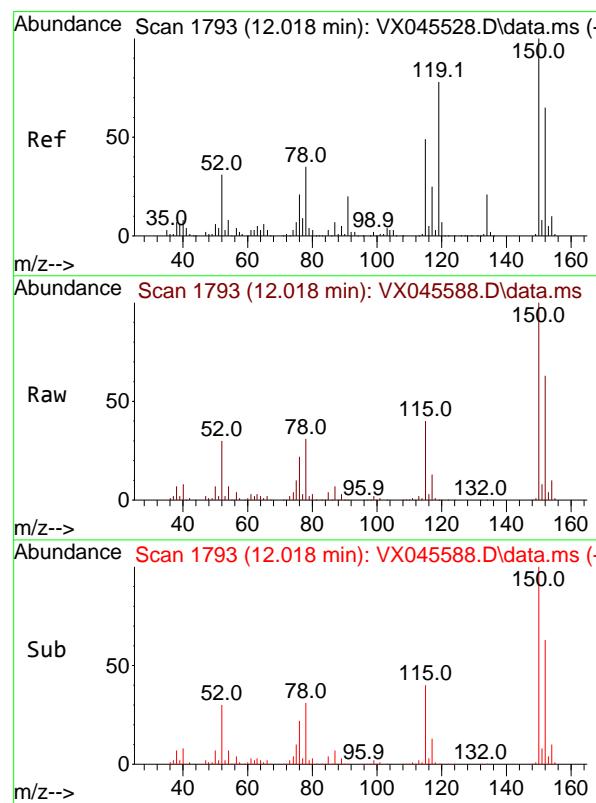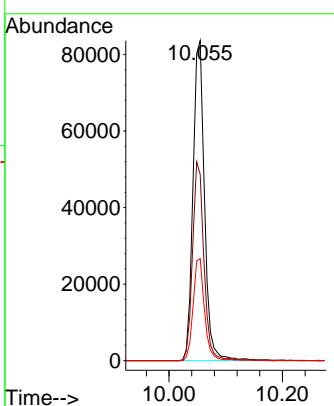

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. -0.000 min  
Lab File: VX045588.D  
Acq: 04 Apr 2025 10:51

Tgt Ion:152 Resp: 46025  
Ion Ratio Lower Upper  
152 100  
115 64.7 46.9 140.7  
150 155.8 0.0 349.4

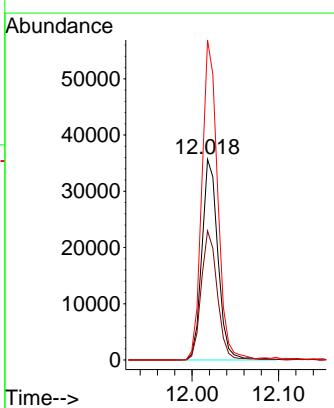



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	
Client Sample ID:	VX0403WBS01			SDG No.:	Q1711
Lab Sample ID:	VX0403WBS01			Matrix:	Water
Analytical Method:	SW8260			% Solid:	0
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000 uL
Soil Aliquot Vol:			uL	Test:	VOCMS Group3
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045563.D	1		04/03/25 12:08	VX040325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	18.9		0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	18.8		0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	18.7		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	18.2		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	18.4		0.20	1.00	ug/L
71-43-2	Benzene	18.7		0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	19.6		0.22	1.00	ug/L
79-01-6	Trichloroethene	18.5		0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	19.1		0.21	1.00	ug/L
127-18-4	Tetrachloroethene	18.4		0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	48.8		70 (74) - 130 (125)	98%	SPK: 50
1868-53-7	Dibromofluoromethane	48.5		70 (75) - 130 (124)	97%	SPK: 50
2037-26-5	Toluene-d8	48.5		70 (86) - 130 (113)	97%	SPK: 50
460-00-4	4-Bromofluorobenzene	49.0		70 (77) - 130 (121)	98%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	95000		5.544		
540-36-3	1,4-Difluorobenzene	168000		6.757		
3114-55-4	Chlorobenzene-d5	149000		10.049		
3855-82-1	1,4-Dichlorobenzene-d4	68900		12.018		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045563.D  
 Acq On : 03 Apr 2025 12:08  
 Operator : JC/MD  
 Sample : VX0403WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0403WBS01

Quant Time: Apr 04 01:19:08 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	95034	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	168178	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	149052	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	68919	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	84848	48.821	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	97.640%		
35) Dibromofluoromethane	5.385	113	57839	48.473	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.940%		
50) Toluene-d8	8.647	98	202186	48.546	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	97.100%		
62) 4-Bromofluorobenzene	11.079	95	74358	49.015	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	98.040%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	28474	20.035	ug/l	97
3) Chloromethane	1.307	50	27632	18.925	ug/l	98
4) Vinyl Chloride	1.374	62	25260	18.904	ug/l	99
5) Bromomethane	1.593	94	11759	18.560	ug/l	97
6) Chloroethane	1.672	64	14325	20.206	ug/l	97
7) Trichlorofluoromethane	1.880	101	38645	19.395	ug/l	100
8) Diethyl Ether	2.130	74	12406	18.545	ug/l	95
9) 1,1,2-Trichlorotrifluo...	2.319	101	22653	19.402	ug/l	97
10) Methyl Iodide	2.447	142	26828	18.421	ug/l	98
11) Tert butyl alcohol	2.971	59	23342	99.939	ug/l	99
12) 1,1-Dichloroethene	2.312	96	21405	18.762	ug/l	100
13) Acrolein	2.233	56	32619	101.417	ug/l	99
14) Allyl chloride	2.660	41	40847	18.870	ug/l	99
15) Acrylonitrile	3.062	53	71197	96.568	ug/l	99
16) Acetone	2.380	43	67462	94.532	ug/l	96
17) Carbon Disulfide	2.501	76	50650	17.975	ug/l	97
18) Methyl Acetate	2.703	43	31989	19.469	ug/l	100
19) Methyl tert-butyl Ether	3.117	73	72893	18.264	ug/l	97
20) Methylene Chloride	2.782	84	25254	18.902	ug/l	94
21) trans-1,2-Dichloroethene	3.087	96	21633	18.560	ug/l	97
22) Diisopropyl ether	3.757	45	79714	18.694	ug/l #	82
23) Vinyl Acetate	3.721	43	346163	93.960	ug/l	100
24) 1,1-Dichloroethane	3.605	63	45204	18.745	ug/l	98
25) 2-Butanone	4.556	43	101576	97.237	ug/l	98
26) 2,2-Dichloropropane	4.465	77	30795	19.765	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	25877	18.223	ug/l	97
28) Bromochloromethane	4.891	49	23399	20.079	ug/l	98
29) Tetrahydrofuran	5.001	42	64526	95.274	ug/l	99
30) Chloroform	5.086	83	47720	19.231	ug/l	99
31) Cyclohexane	5.458	56	40068	18.794	ug/l	96
32) 1,1,1-Trichloroethane	5.373	97	38732	18.447	ug/l	98
36) 1,1-Dichloropropene	5.690	75	31010	19.248	ug/l	97
37) Ethyl Acetate	4.714	43	37537	18.488	ug/l	98
38) Carbon Tetrachloride	5.672	117	32889	18.889	ug/l	98
39) Methylcyclohexane	7.379	83	38109	19.297	ug/l	97
40) Benzene	6.031	78	92131	18.724	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045563.D  
 Acq On : 03 Apr 2025 12:08  
 Operator : JC/MD  
 Sample : VX0403WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0403WBS01

Quant Time: Apr 04 01:19:08 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	20481	19.119	ug/1	97
42) 1,2-Dichloroethane	6.086	62	39817	19.592	ug/1	99
43) Isopropyl Acetate	6.342	43	57673	18.742	ug/1	100
44) Trichloroethene	7.123	130	21580	18.452	ug/1	99
45) 1,2-Dichloropropane	7.427	63	22690	18.482	ug/1	96
46) Dibromomethane	7.580	93	18338	19.458	ug/1	100
47) Bromodichloromethane	7.818	83	35669	18.952	ug/1	93
48) Methyl methacrylate	7.696	41	29793	18.752	ug/1	98
49) 1,4-Dioxane	7.659	88	11782	409.867	ug/1	98
51) 4-Methyl-2-Pentanone	8.574	43	204092	100.048	ug/1	98
52) Toluene	8.714	92	56597	19.009	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	29059	17.610	ug/1	99
54) cis-1,3-Dichloropropene	8.366	75	33695	19.051	ug/1	98
55) 1,1,2-Trichloroethane	9.147	97	22623	19.068	ug/1	97
56) Ethyl methacrylate	9.116	69	34400	18.735	ug/1	98
57) 1,3-Dichloropropane	9.305	76	39503	19.120	ug/1	98
58) 2-Chloroethyl Vinyl ether	8.238	63	84945	91.451	ug/1	100
59) 2-Hexanone	9.427	43	151035	99.982	ug/1	99
60) Dibromochloromethane	9.518	129	24684	19.084	ug/1	98
61) 1,2-Dibromoethane	9.610	107	23132	19.260	ug/1	97
64) Tetrachloroethene	9.269	164	19411	18.445	ug/1	97
65) Chlorobenzene	10.079	112	60989	19.149	ug/1	98
66) 1,1,1,2-Tetrachloroethane	10.159	131	20434	18.479	ug/1	98
67) Ethyl Benzene	10.189	91	108957	19.101	ug/1	99
68) m/p-Xylenes	10.299	106	79412	38.276	ug/1	97
69) o-Xylene	10.640	106	38939	19.052	ug/1	98
70) Styrene	10.652	104	66139	19.607	ug/1	100
71) Bromoform	10.799	173	15475	18.743	ug/1 #	100
73) Isopropylbenzene	10.957	105	103012	18.660	ug/1	99
74) N-amyl acetate	10.841	43	48409	18.332	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	36109	18.620	ug/1	100
76) 1,2,3-Trichloropropane	11.238	75	31309m	18.624	ug/1	
77) Bromobenzene	11.195	156	23469	18.399	ug/1	99
78) n-propylbenzene	11.299	91	119014	18.717	ug/1	99
79) 2-Chlorotoluene	11.360	91	75745	18.633	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	87968	19.270	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	8340	16.837	ug/1	92
82) 4-Chlorotoluene	11.451	91	84800	18.710	ug/1	99
83) tert-Butylbenzene	11.713	119	86089	19.049	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	87951	19.196	ug/1	100
85) sec-Butylbenzene	11.890	105	107693	19.401	ug/1	98
86) p-Isopropyltoluene	12.006	119	87307	19.078	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	41875	18.035	ug/1	100
88) 1,4-Dichlorobenzene	12.036	146	42877	18.215	ug/1	98
89) n-Butylbenzene	12.329	91	72973	18.388	ug/1	98
90) Hexachloroethane	12.536	117	15145	19.256	ug/1	97
91) 1,2-Dichlorobenzene	12.335	146	42284	18.317	ug/1	98
92) 1,2-Dibromo-3-Chloropr...	12.945	75	7578	18.685	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	22581	17.574	ug/1	97
94) Hexachlorobutadiene	13.719	225	10095	18.232	ug/1	99
95) Naphthalene	13.774	128	82961	17.350	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	23220	17.258	ug/1	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045563.D  
 Acq On : 03 Apr 2025 12:08  
 Operator : JC/MD  
 Sample : VX0403WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0403WBS01

**Manual Integrations**  
**APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

Quant Time: Apr 04 01:19:08 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed







Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
Data File : VX045563.D  
Acq On : 03 Apr 2025 12:08  
Operator : JC/MD  
Sample : VX0403WBS01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VX0403WBS01

## Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

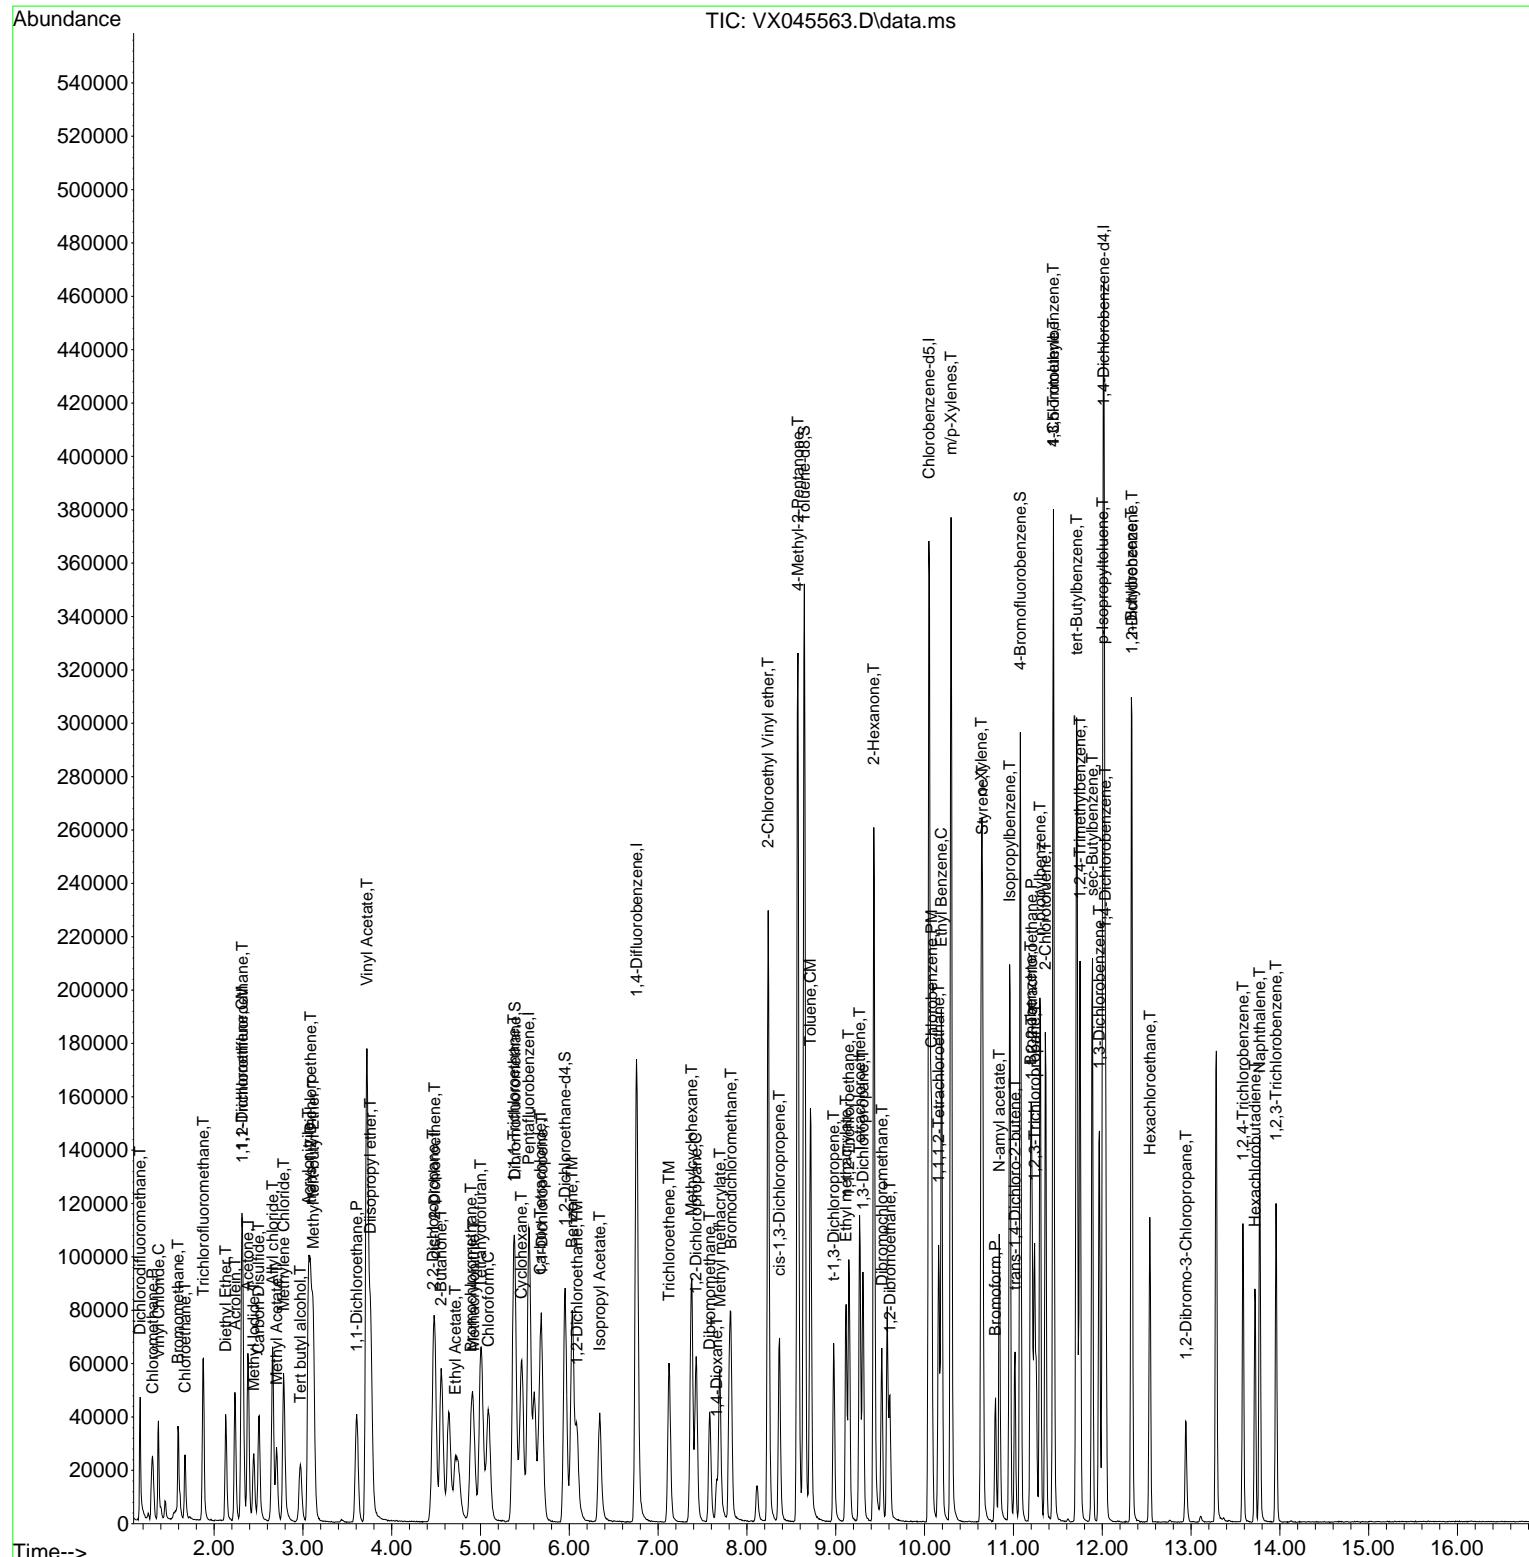

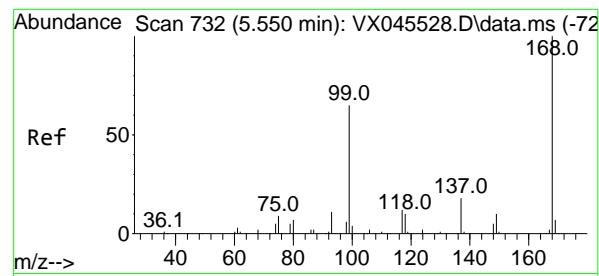


#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.544 min Scan# 7  
Delta R.T. -0.006 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

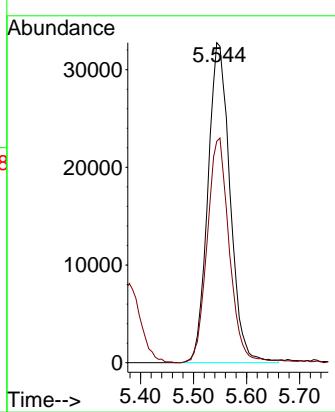



#2  
Dichlorodifluoromethane  
Concen: 20.035 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 85 Resp: 28474  
Ion Ratio Lower Upper  
85 100  
87 34.0 16.1 48.2






Abundance Scan 36 (1.307 min): VX045563.D\data.ms

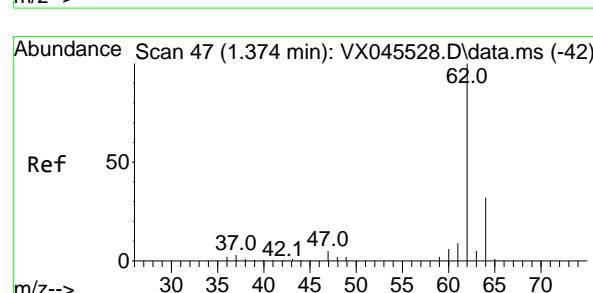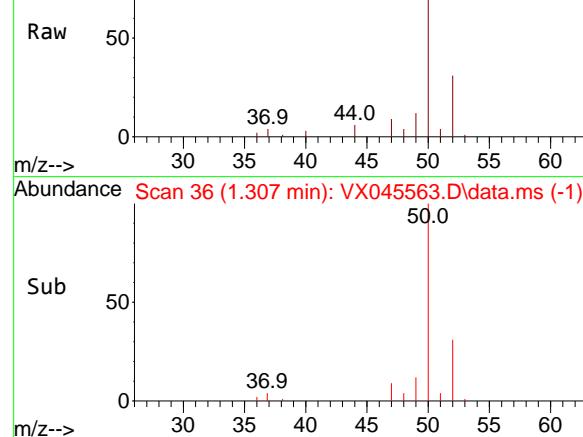

Abundance Scan 47 (1.374 min): VX045563.D\data.ms

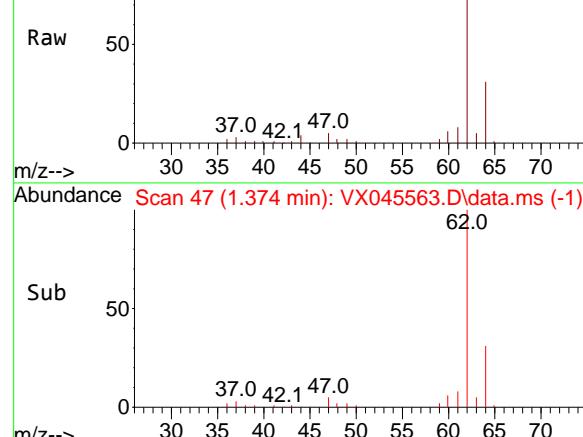

#3

Chloromethane

Concen: 18.925 ug/l

RT: 1.307 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

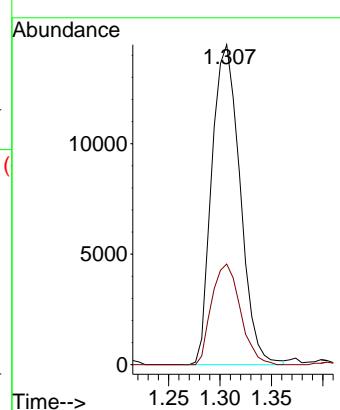 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#4

Vinyl Chloride


Concen: 18.904 ug/l




RT: 1.374 min Scan# 47

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

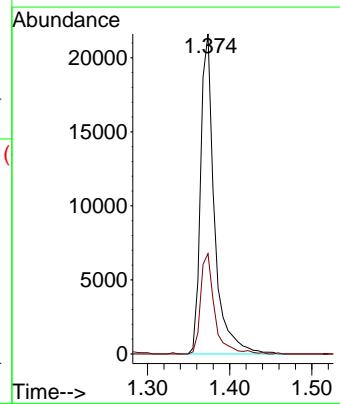 Tgt Ion: 62 Resp: 25260  
 Ion Ratio Lower Upper  
 62 100  
 64 31.3 25.5 38.3





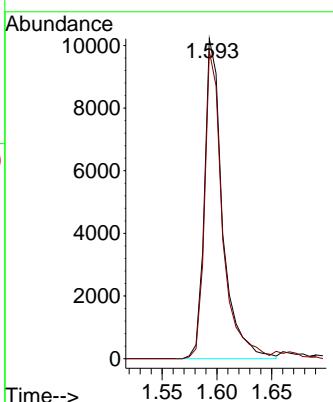


#5  
 Bromomethane  
 Concen: 18.560 ug/l  
 RT: 1.593 min Scan# 8  
 Delta R.T. -0.000 min  
 Lab File: VX045563.D  
 Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
 ClientSampleId : VX0403WBS01


**Manual Integrations**  
**APPROVED**


Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025



#6  
 Chloroethane  
 Concen: 20.206 ug/l  
 RT: 1.672 min Scan# 96  
 Delta R.T. 0.006 min  
 Lab File: VX045563.D  
 Acq: 03 Apr 2025 12:08


Tgt Ion: 64 Resp: 14325  
 Ion Ratio Lower Upper  
 64 100  
 66 31.2 26.3 39.5

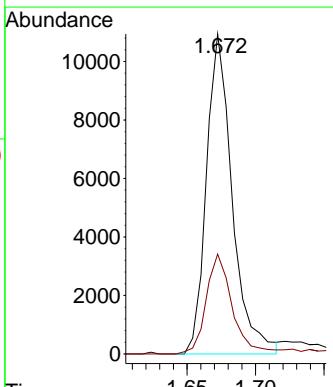



#7  
Trichlorofluoromethane  
Concen: 19.395 ug/l  
RT: 1.880 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08




Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01

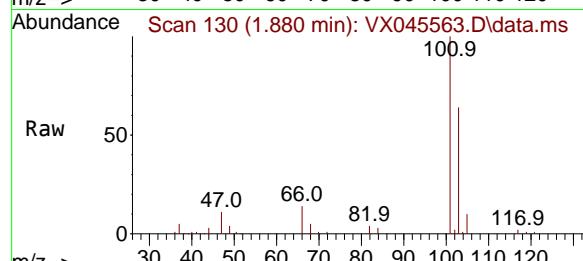


Tgt Ion:101 Resp: 3864  
Ion Ratio Lower Upper  
101 100  
103 63.8 51.1 76.7

Manual Integrations  
APPROVED



Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025






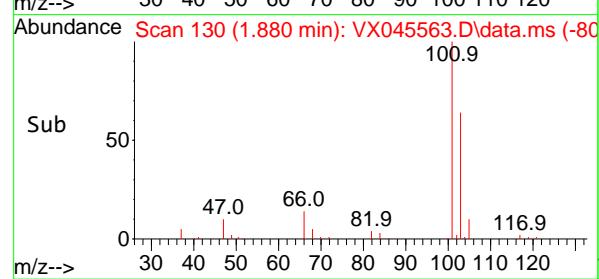


#8  
Diethyl Ether  
Concen: 18.545 ug/l  
RT: 2.130 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08



Tgt Ion: 74 Resp: 12406  
Ion Ratio Lower Upper  
74 100  
45 111.6 53.0 159.1

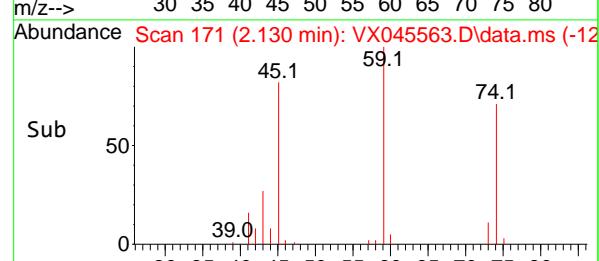

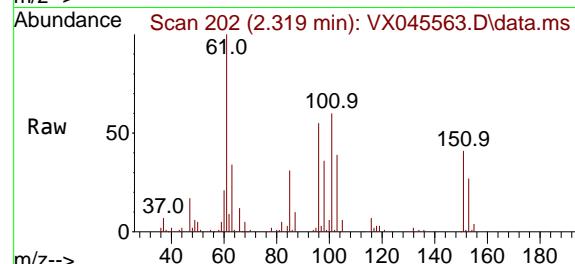

#9

1,1,2-Trichlorotrifluoroethane

Concen: 19.402 ug/l

RT: 2.319 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

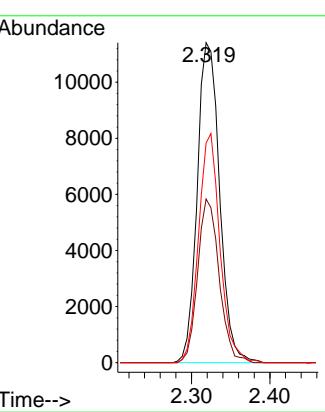 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#10

Methyl Iodide

Concen: 18.421 ug/l


RT: 2.447 min Scan# 223


Delta R.T. -0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08

Tgt	Ion:142	Resp:	26828
Ion	Ratio	Lower	Upper
142	100		
127	51.5	40.2	60.4
141	14.0	11.7	17.5


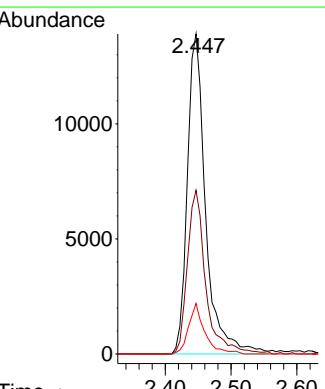





Abundance Scan 309 (2.971 min): VX045563.D\data.ms

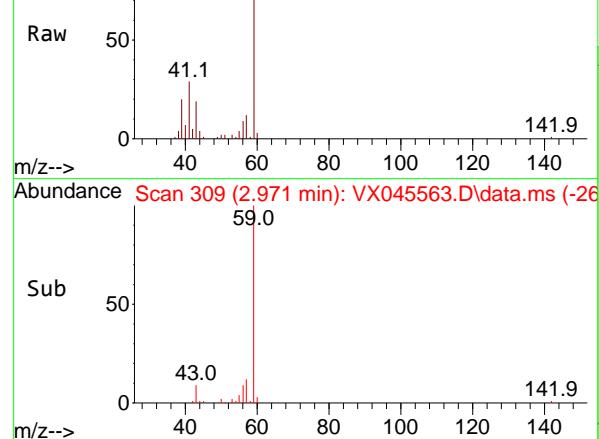


Abundance Scan 309 (2.971 min): VX045563.D\data.ms (-26)

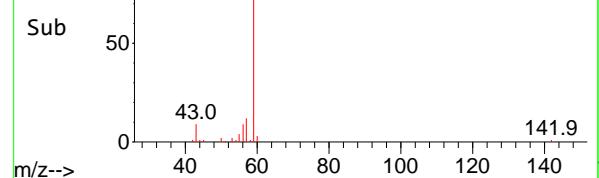

Abundance Scan 201 (2.312 min): VX045563.D\data.ms

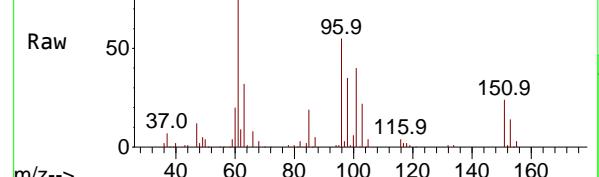

Abundance Scan 201 (2.312 min): VX045563.D\data.ms (-15)

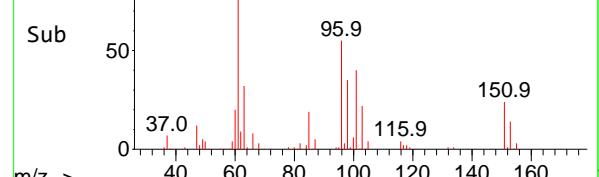


#11

Tert butyl alcohol  
Concen: 99.939 ug/l  
RT: 2.971 min Scan# 3  
Delta R.T. -0.006 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01

### Manual Integrations APPROVED


Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025




#12



1,1-Dichloroethene  
Concen: 18.762 ug/l  
RT: 2.312 min Scan# 201  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 96 Resp: 21405  
Ion Ratio Lower Upper  
96 100  
61 182.4 145.7 218.5  
98 64.6 51.6 77.4

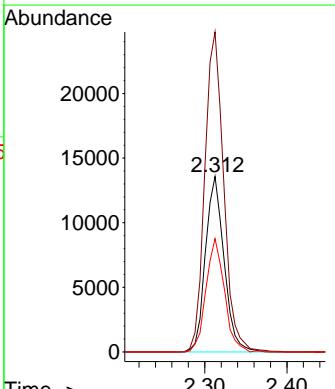




Ref Scan 188 (2.233 min): VX045563.D\data.ms

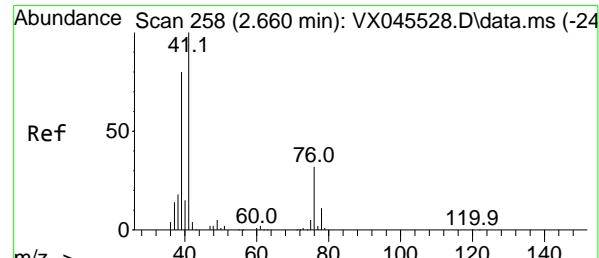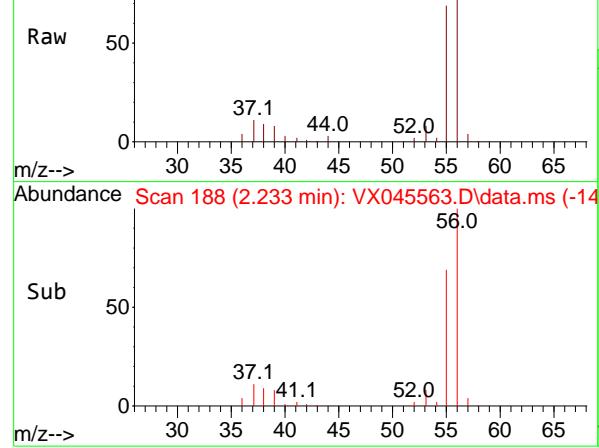

Ref Scan 258 (2.660 min): VX045563.D\data.ms

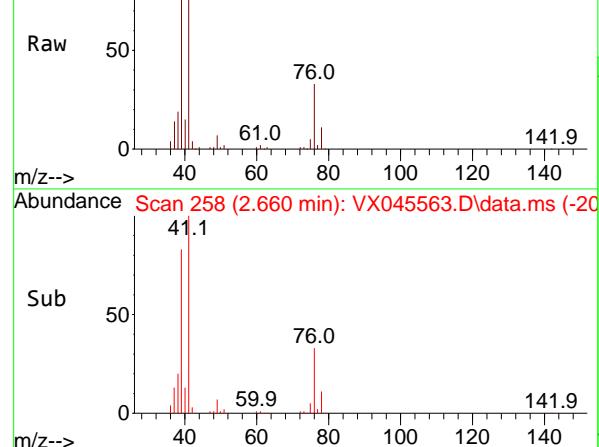

#13

Acrolein

Concen: 101.417 ug/l

RT: 2.233 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

Tgt Ion: 56 Resp: 32619

Ion Ratio Lower Upper

56 100


55 70.8 56.2 84.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025

Supervised By :Mahesh Dadoda 04/04/2025



#14

Allyl chloride

Concen: 18.870 ug/l

RT: 2.660 min Scan# 258

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Tgt Ion: 41 Resp: 40847







Ion Ratio Lower Upper

41 100

39 76.5 60.2 90.2

76 30.1 24.6 36.8

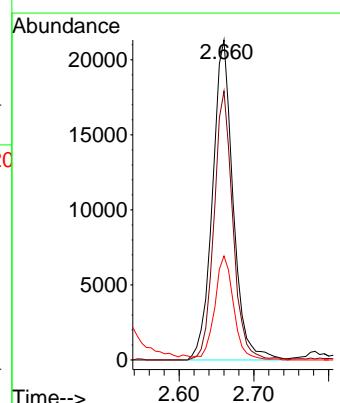

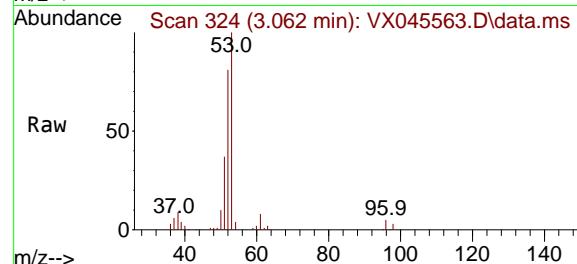

#15

Acrylonitrile

Concen: 96.568 ug/l

RT: 3.062 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument:


MSVOA\_X

ClientSampleId :

VX0403WBS01

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#16

Acetone

Concen: 94.532 ug/l


RT: 2.380 min Scan# 212


Delta R.T. -0.006 min

Lab File: VX045563.D





Acq: 03 Apr 2025 12:08

Tgt Ion: 43 Resp: 67462  
Ion Ratio Lower Upper  
43 100  
58 25.8 22.3 33.5

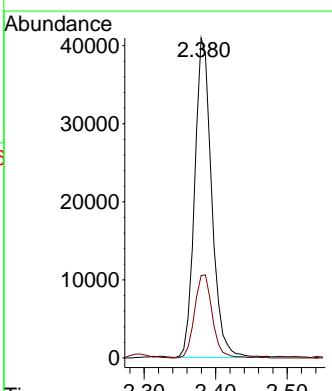



Abundance Scan 232 (2.501 min): VX045563.D\data.ms

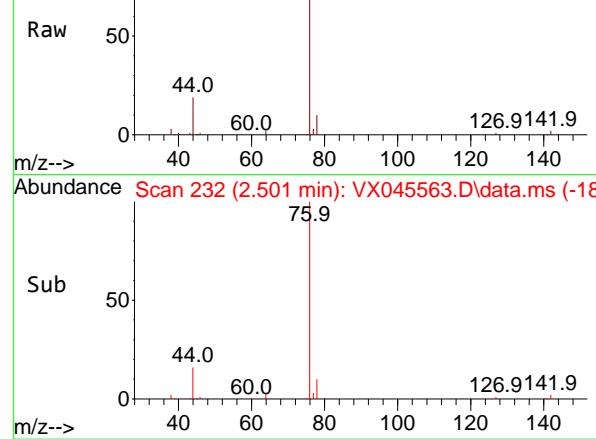

#17

Carbon Disulfide

Concen: 17.975 ug/l

RT: 2.501 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08

Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**
Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

#18

Methyl Acetate


Concen: 19.469 ug/l







RT: 2.703 min Scan# 265

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Tgt Ion: 43 Resp: 31989  
Ion Ratio Lower Upper  
43 100  
74 22.0 17.5 26.3

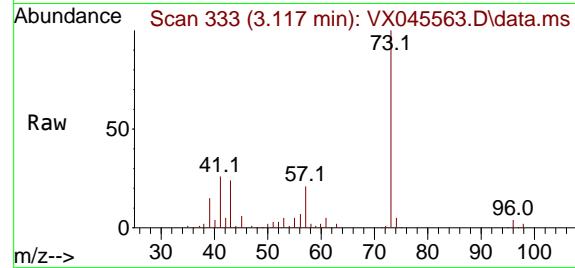


#19

Methyl tert-butyl Ether  
Concen: 18.264 ug/l  
RT: 3.117 min Scan# 3  
Delta R.T. 0.006 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01

### Manual Integrations APPROVED


Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025









#20

Methylene Chloride  
Concen: 18.902 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 84 Resp: 25254  
Ion Ratio Lower Upper  
84 100  
49 145.7 107.5 161.3  
51 41.7 33.0 49.6  
86 65.2 50.1 75.1

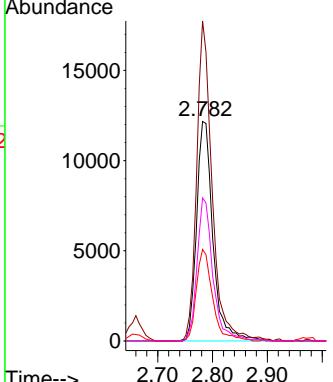




#21  
trans-1,2-Dichloroethene  
Concen: 18.560 ug/l  
RT: 3.087 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


### Manual Integrations APPROVED




Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025



#22  
Diisopropyl ether  
Concen: 18.694 ug/l  
RT: 3.757 min Scan# 438  
Delta R.T. -0.006 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 45 Resp: 79714  
Ion Ratio Lower Upper  
45 100  
43 96.4 59.3 88.9#  
87 25.1 20.4 30.6  
59 12.2 9.0 13.6



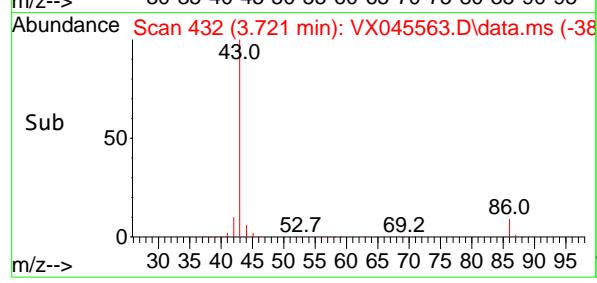

#23

**Vinyl Acetate**

Concen: 93.960 ug/l

RT: 3.721 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01





Tgt Ion: 43 Resp: 34616

Ion Ratio Lower Upper

43 100  
86 9.3 7.5 11.3**Manual Integrations****APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025

Supervised By :Mahesh Dadoda 04/04/2025



#24

**1,1-Dichloroethane**

Concen: 18.745 ug/l

RT: 3.605 min Scan# 413


Delta R.T. -0.000 min


Lab File: VX045563.D

Acq: 03 Apr 2025 12:08



Tgt Ion: 63 Resp: 45204

Ion Ratio Lower Upper


63 100  
98 7.0 3.4 10.1  
100 3.5 2.2 6.6



Abundance Scan 569 (4.556 min): VX045563.D\data.ms

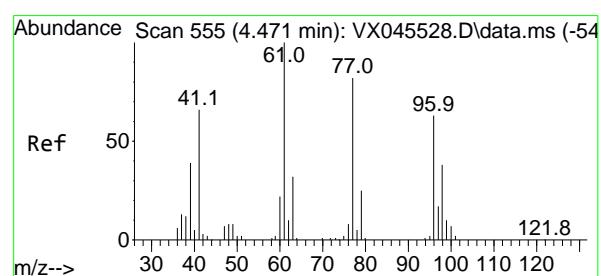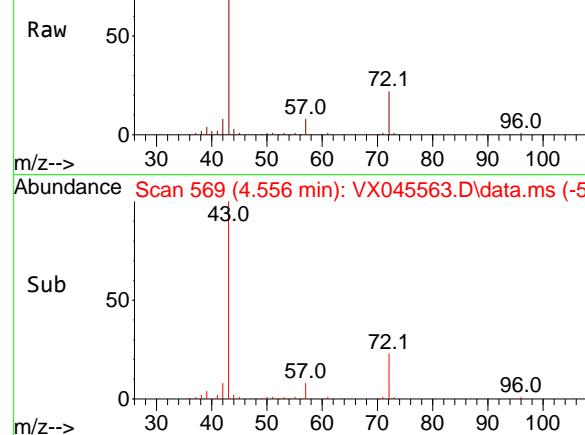

Abundance Scan 554 (4.465 min): VX045563.D\data.ms

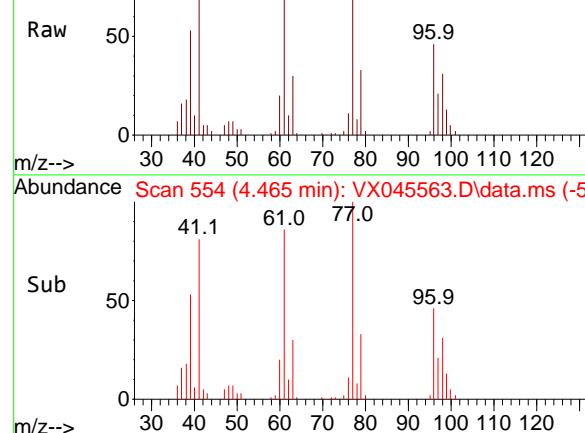

Abundance Scan 554 (4.465 min): VX045563.D\data.ms (-50)

#25

2-Butanone

Concen: 97.237 ug/l

RT: 4.556 min Scan# 5

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument:


MSVOA\_X

ClientSampleId :

VX0403WBS01

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#26

2,2-Dichloropropane

Concen: 19.765 ug/l

RT: 4.465 min Scan# 554

Delta R.T. -0.006 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08




Tgt Ion: 77 Resp: 30795

Ion Ratio Lower Upper

77 100

97 21.1 10.6 31.8

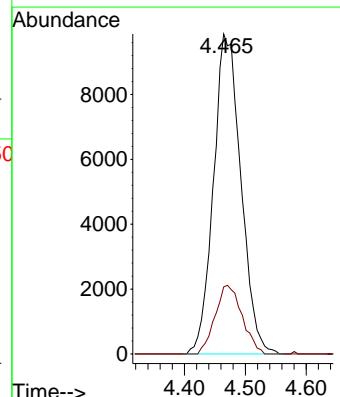


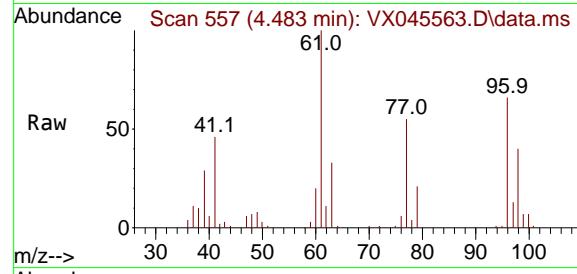



#27  
cis-1,2-Dichloroethene  
Concen: 18.223 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


### Manual Integrations APPROVED




Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

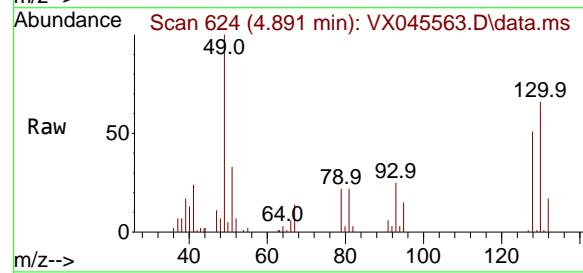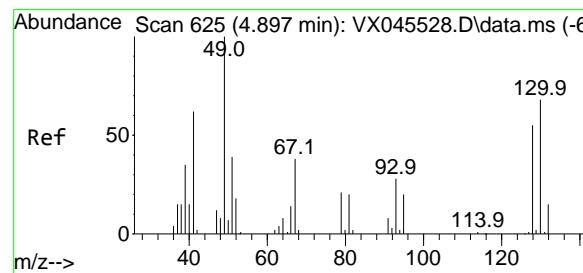

#28  
Bromochloromethane  
Concen: 20.079 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 49 Resp: 23399  
Ion Ratio Lower Upper  
49 100  
129 1.4 0.0 3.8  
130 66.7 54.6 81.8

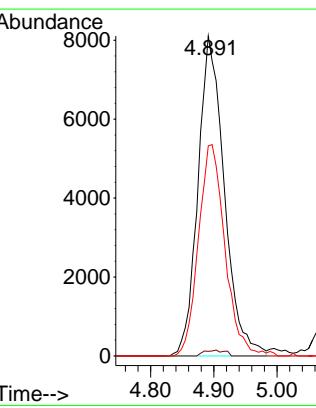

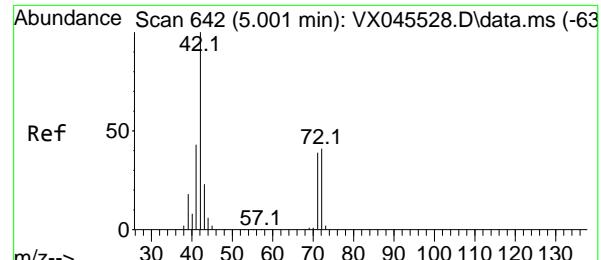

#29

Tetrahydrofuran

Concen: 95.274 ug/l

RT: 5.001 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08




Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations**  
**APPROVED**

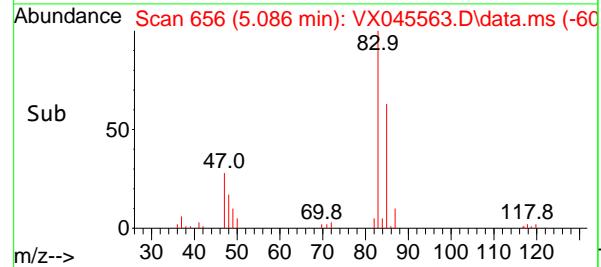 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#30

Chloroform

Concen: 19.231 ug/l

RT: 5.086 min Scan# 656

Delta R.T. -0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08







Tgt Ion: 83 Resp: 47720

Ion Ratio Lower Upper

83 100

85 65.3 52.8 79.2

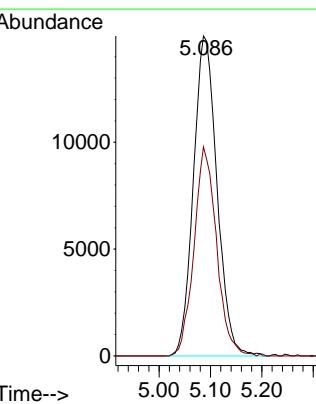

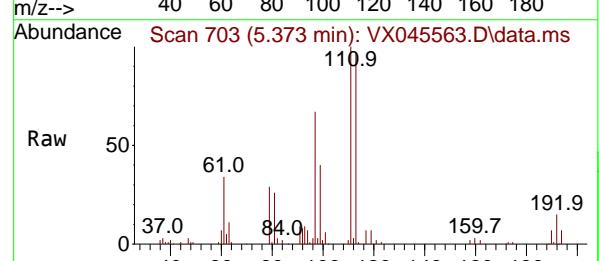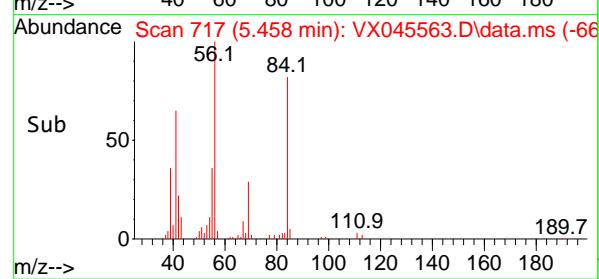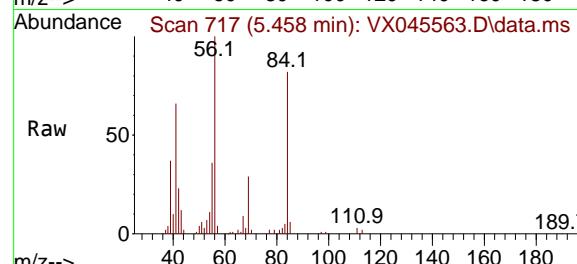

#31

Cyclohexane

Concen: 18.794 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

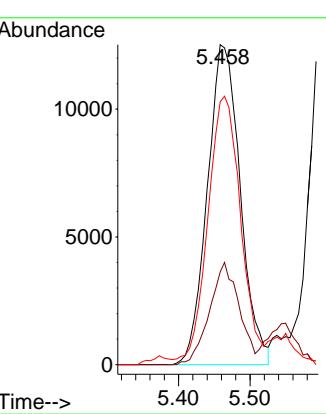 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#32

1,1,1-Trichloroethane

Concen: 18.447 ug/l


RT: 5.373 min Scan# 703


Delta R.T. -0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Tgt	Ion	Resp:	
Ion	Ratio	Lower	Upper
	97	100	
97	100	51.7	77.5
61	53.4	41.0	61.4

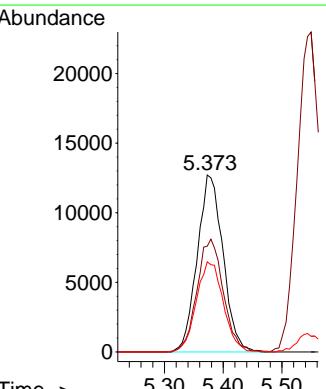

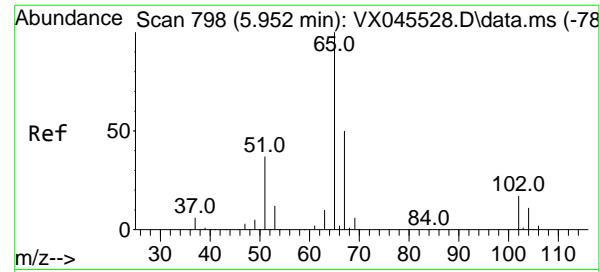

#33


1,2-Dichloroethane-d4  
Concen: 48.821 ug/l  
RT: 5.952 min Scan# 7  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0403WBS01


Tgt Ion: 65 Resp: 84848  
Ion Ratio Lower Upper  
65 100  
67 50.1 0.0 99.0

Manual Integrations  
APPROVED


Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025




Time--&gt;

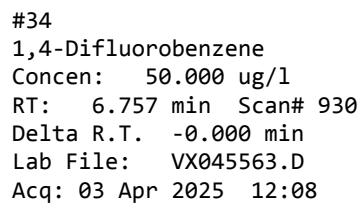


Time--&gt;

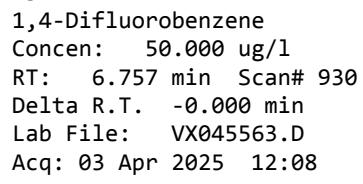


Tgt Ion:114 Resp: 168178  
Ion Ratio Lower Upper  
114 100  
63 24.2 0.0 46.8  
88 16.6 0.0 35.4



Time--&gt;



Time--&gt;

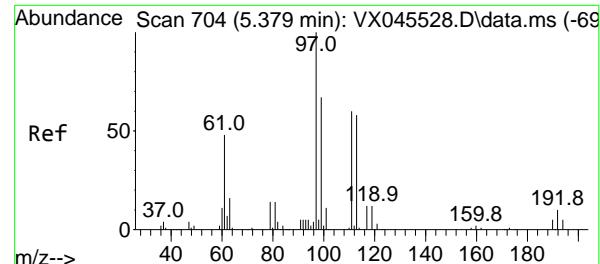

#35

Dibromofluoromethane




Concen: 48.473 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

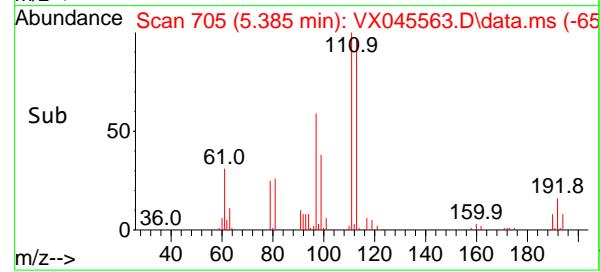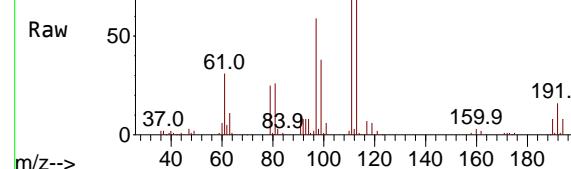

#36

1,1-Dichloropropene



Concen: 19.248 ug/l

RT: 5.690 min Scan# 755

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

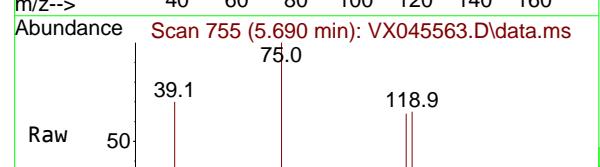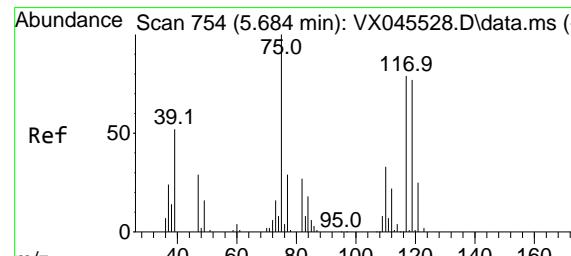

#36

1,1-Dichloropropene


Concen: 19.248 ug/l

RT: 5.690 min Scan# 755

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

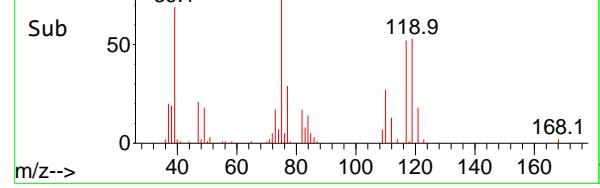

#36

1,1-Dichloropropene

Concen: 19.248 ug/l

RT: 5.690 min Scan# 755

Delta R.T. 0.006 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08

Instrument: MSVOA\_X


Client SampleId: VX0403WBS01

### Manual Integrations APPROVED




Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

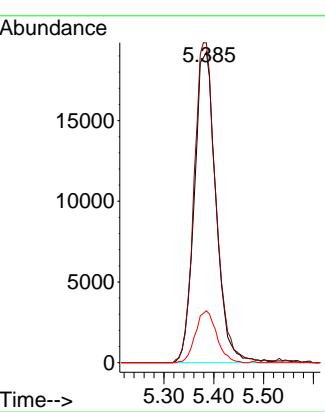

5.30 5.40 5.50

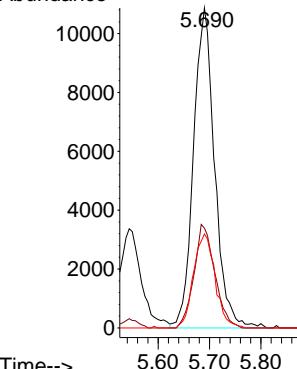

5.60 5.70 5.80

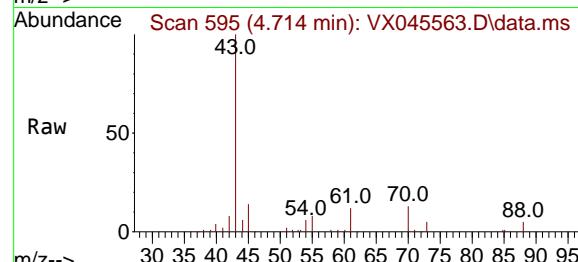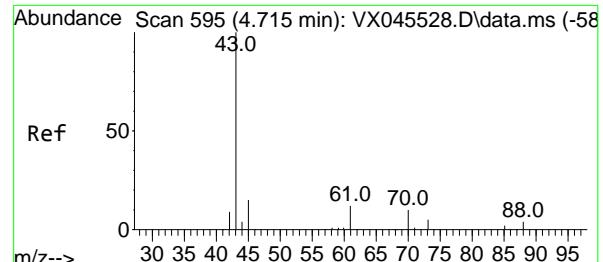

#37

**Ethyl Acetate**

Concen: 18.488 ug/l

RT: 4.714 min Scan# 5

Delta R.T. -0.000 min

Lab File: VX045563.D




Acq: 03 Apr 2025 12:08

Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

#38

**Carbon Tetrachloride**

Concen: 18.889 ug/l

RT: 5.672 min Scan# 752

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Tgt Ion:117 Resp: 32889







Ion Ratio Lower Upper

117 100

119 93.3 76.9 115.3

121 30.7 24.2 36.2

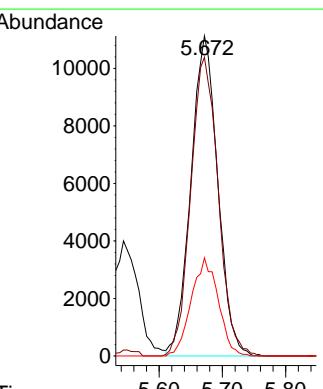



#39

Methylcyclohexane

Concen: 19.297 ug/l

RT: 7.379 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument :


MSVOA\_X

ClientSampleId :

VX0403WBS01

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#40

Benzene

Concen: 18.724 ug/l

RT: 6.031 min Scan# 811

Delta R.T. -0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08







Tgt Ion: 78 Resp: 92131

Ion Ratio Lower Upper

78 100

77 23.7 19.0 28.6





#41

Methacrylonitrile

Concen: 19.119 ug/l

RT: 4.922 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument :

MSVOA\_X


ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

Abundance

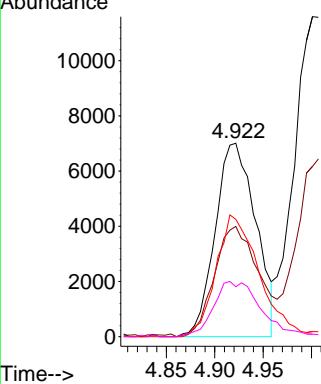

#42

1,2-Dichloroethane

Concen: 19.592 ug/l

RT: 6.086 min Scan# 820

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Tgt Ion: 62 Resp: 39817


Ion Ratio Lower Upper

62 100


98 7.4 0.0 15.2

Abundance

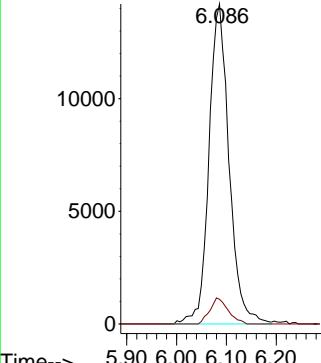




Abundance Scan 862 (6.342 min): VX045563.D\data.ms

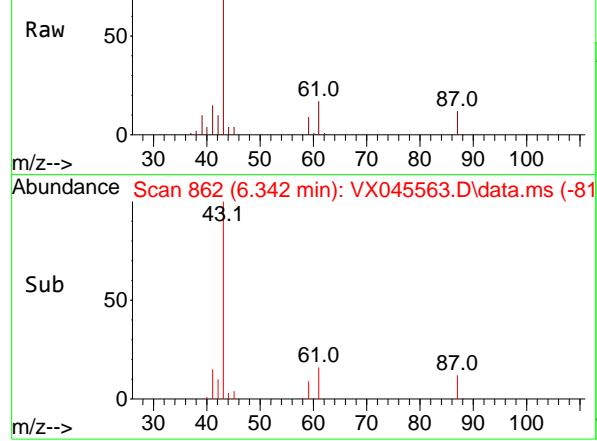

Abundance Scan 862 (6.342 min): VX045563.D\data.ms (-81)

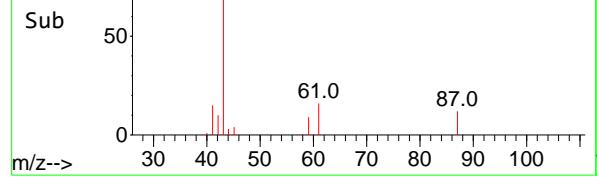

#43

Isopropyl Acetate

Concen: 18.742 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

Tgt Ion: 43 Resp: 5767

Ion Ratio Lower Upper

43 100

61 17.6 14.1 21.1



87 11.5 9.2 13.8

Manual Integrations


APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025


Supervised By :Mahesh Dadoda 04/04/2025

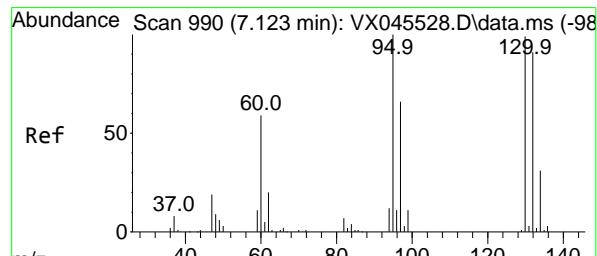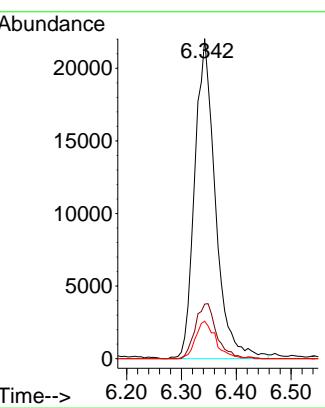

Abundance Scan 990 (7.123 min): VX045563.D\data.ms

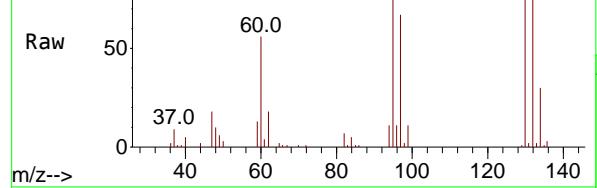

Abundance Scan 990 (7.123 min): VX045563.D\data.ms (-94)

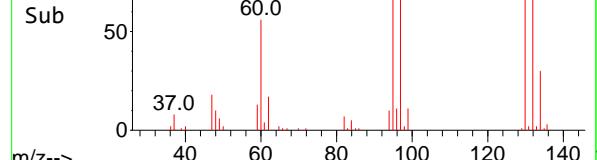

#44

Trichloroethene

Concen: 18.452 ug/l

RT: 7.123 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08




Tgt Ion: 130 Resp: 21580

Ion Ratio Lower Upper

130 100

95 99.7 0.0 202.0

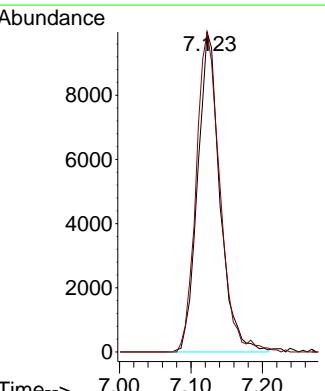



#45

1,2-Dichloropropane

Concen: 18.482 ug/l

RT: 7.427 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08




Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#46

Dibromomethane

Concen: 19.458 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Tgt Ion: 93 Resp: 18338


Ion Ratio Lower Upper

93 100

95 80.8 64.8 97.2

174 81.4 65.4 98.0

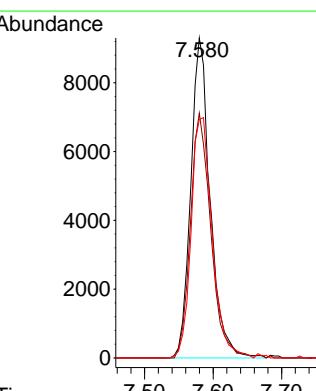

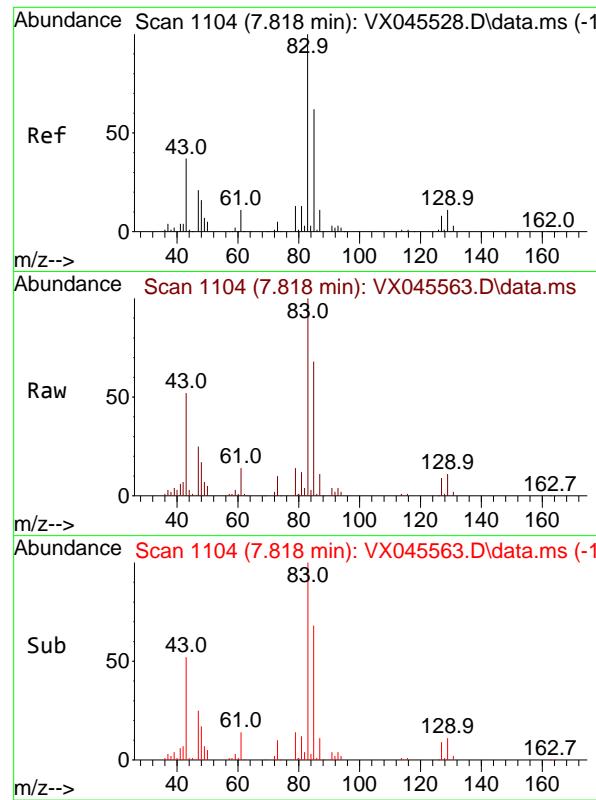

#47

Bromodichloromethane

Concen: 18.952 ug/l

RT: 7.818 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

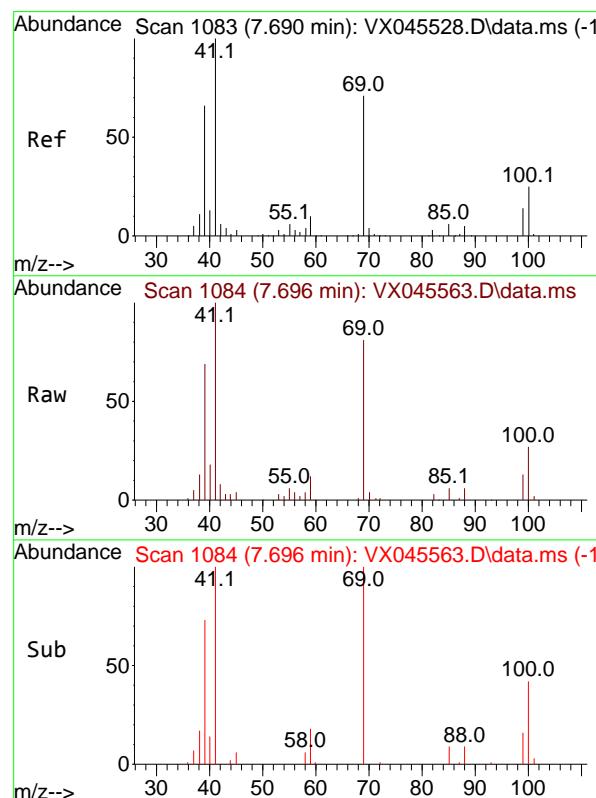 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#48

Methyl methacrylate

Concen: 18.752 ug/l

RT: 7.696 min Scan# 1084

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Tgt Ion: 41 Resp: 29793


Ion Ratio Lower Upper

41 100

69 73.8 58.2 87.2


39 68.7 53.6 80.4

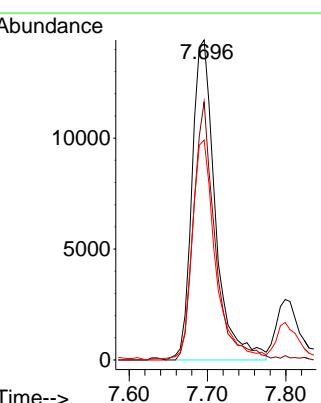

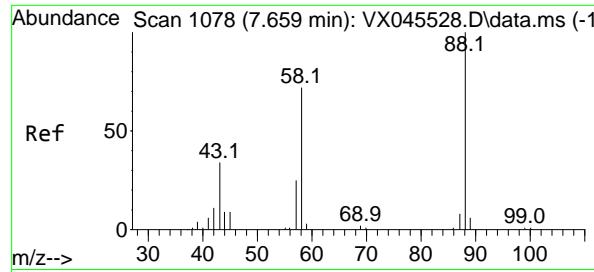

#49  
1,4-Dioxane  
Concen: 409.867 ug/l  
RT: 7.659 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08




Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01




Tgt Ion: 88 Resp: 11783  
Ion Ratio Lower Upper  
88 100  
43 41.6 32.2 48.4  
58 71.8 58.6 88.0

### Manual Integrations APPROVED



Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

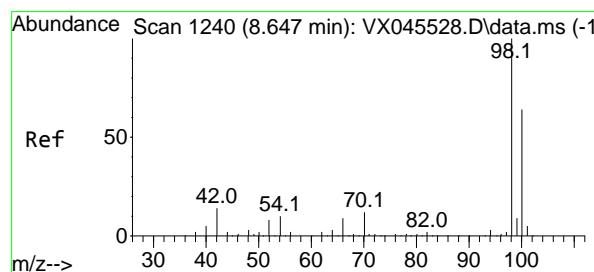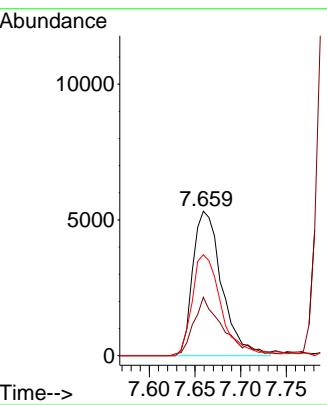


#50  
Toluene-d8  
Concen: 48.546 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08




Tgt Ion: 98 Resp: 202186  
Ion Ratio Lower Upper  
98 100  
100 64.9 52.2 78.4

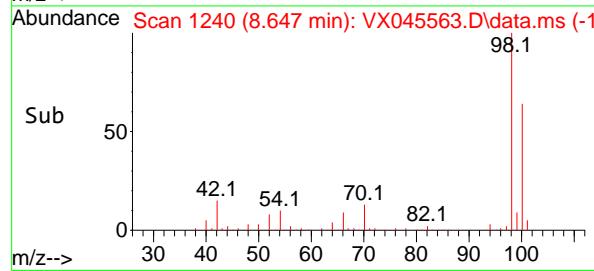




Abundance Scan 1228 (8.574 min): VX045563.D\data.ms

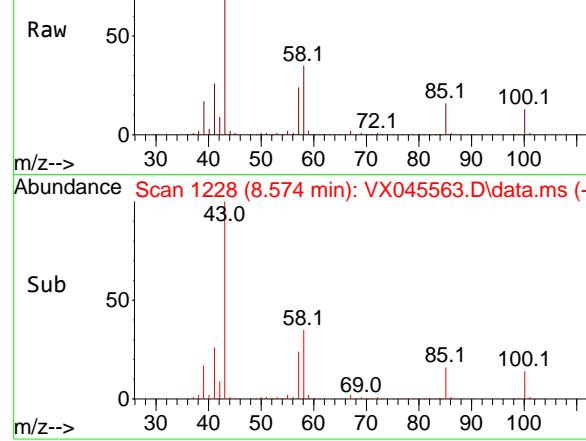

Abundance Scan 1228 (8.574 min): VX045563.D\data.ms (-1)

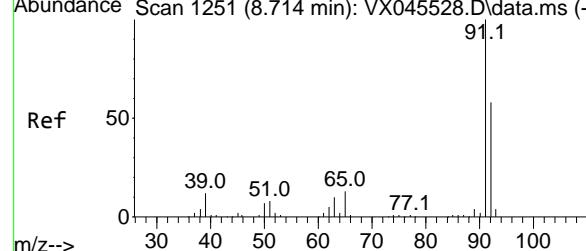

Abundance Scan 1228 (8.574 min): VX045563.D\data.ms

#51

4-Methyl-2-Pentanone

Concen: 100.048 ug/l

RT: 8.574 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D



Acq: 03 Apr 2025 12:08

Instrument:


MSVOA\_X

ClientSampleId :


VX0403WBS01

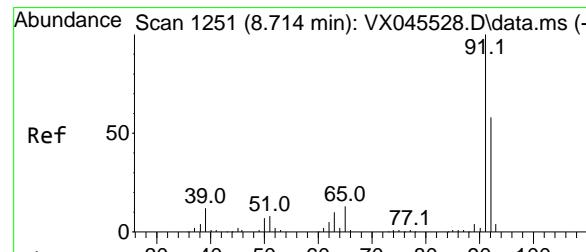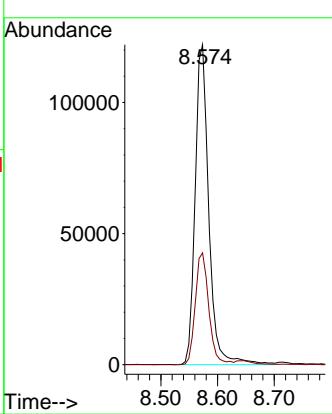**Manual Integrations  
APPROVED**Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

Abundance Scan 1251 (8.714 min): VX045563.D\data.ms

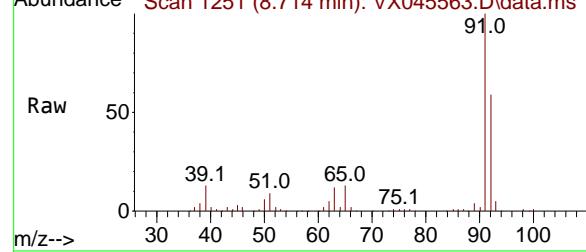

Abundance Scan 1251 (8.714 min): VX045563.D\data.ms

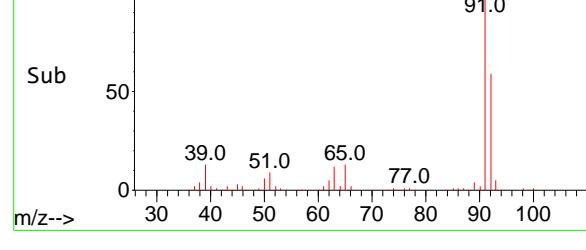

#52

Toluene

Concen: 19.009 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. -0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08







Tgt Ion: 92 Resp: 56597

Ion Ratio Lower Upper

92 100

91 173.1 138.7 208.1

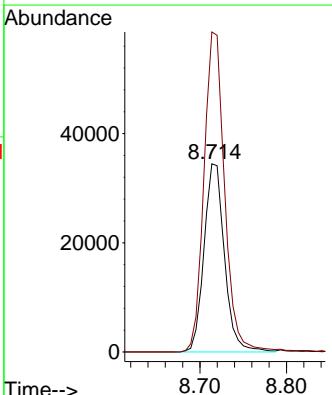

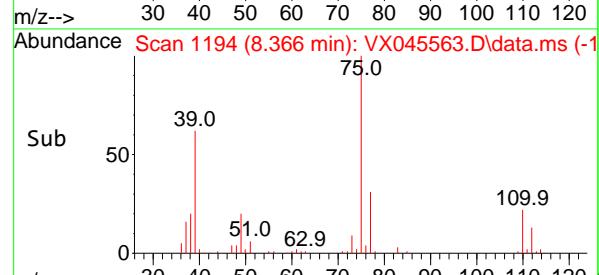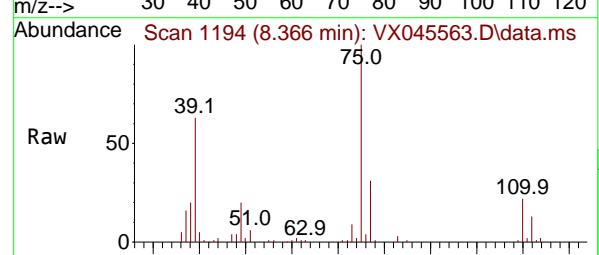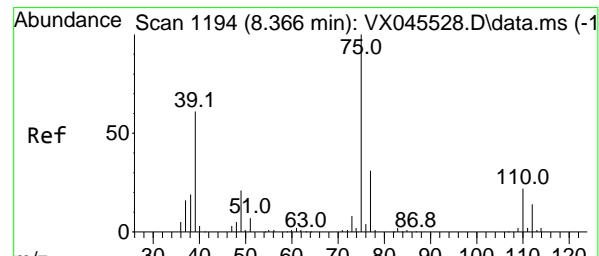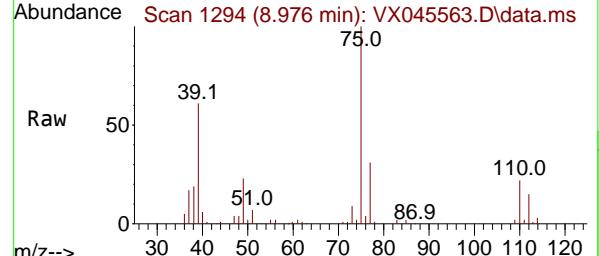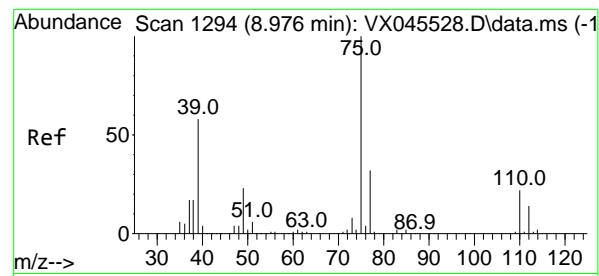


#53

t-1,3-Dichloropropene  
Concen: 17.610 ug/l  
RT: 8.976 min Scan# 1194  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


### Manual Integrations APPROVED




Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

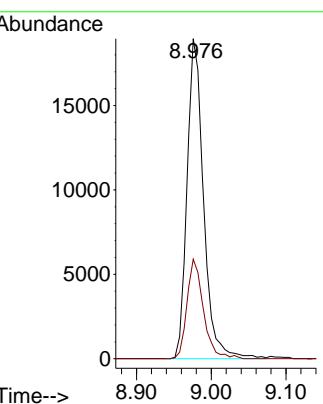

#54  
cis-1,3-Dichloropropene  
Concen: 19.051 ug/l  
RT: 8.366 min Scan# 1194  
Delta R.T. 0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 75 Resp: 33695  
Ion Ratio Lower Upper  
75 100  
77 30.7 24.6 36.8  
39 62.6 48.4 72.6

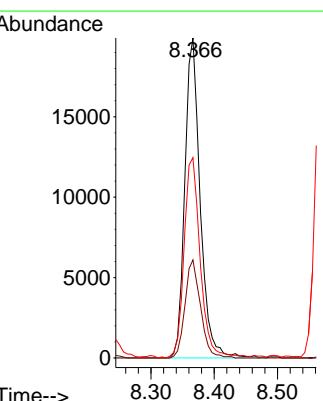



#55

1,1,2-Trichloroethane

Concen: 19.068 ug/l

RT: 9.147 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument:




MSVOA\_X

ClientSampleId :

VX0403WBS01

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#56

Ethyl methacrylate

Concen: 18.735 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min


Lab File: VX045563.D



Acq: 03 Apr 2025 12:08

Tgt Ion: 69 Resp: 34400

Ion Ratio Lower Upper

69	100		
41	78.9	61.3	91.9
39	51.1	40.2	60.2

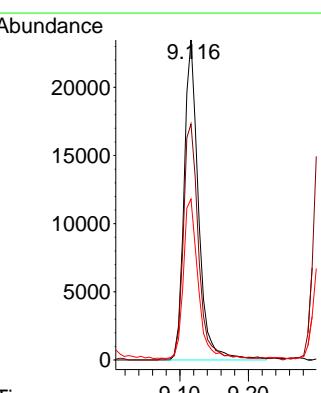

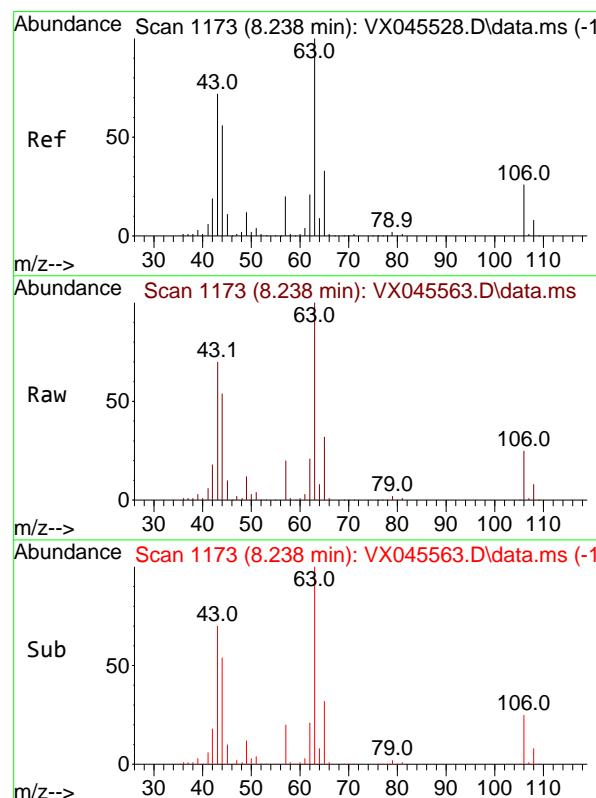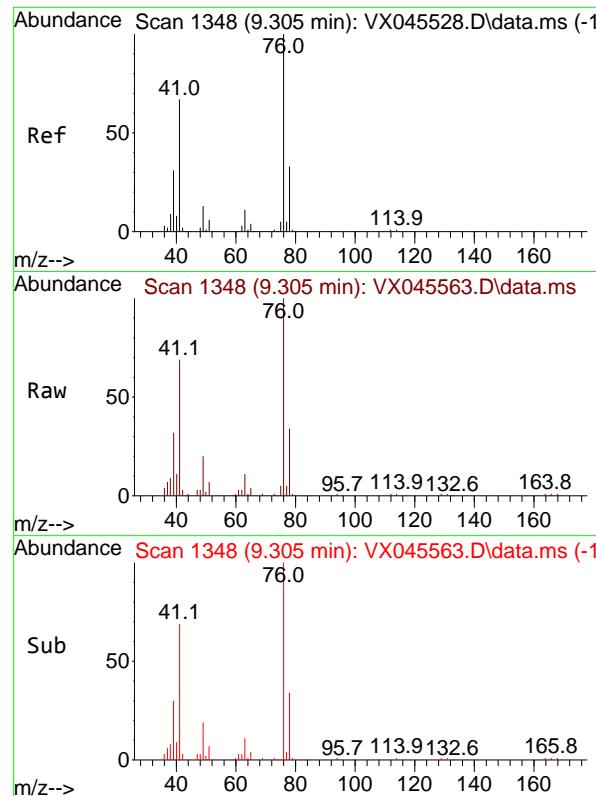

#57

1,3-Dichloropropane

Concen: 19.120 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08

Instrument :

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations**  
**APPROVED**
Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

#58

2-Chloroethyl Vinyl ether

Concen: 91.451 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. -0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08


Tgt Ion: 63 Resp: 84945

Ion Ratio Lower Upper


63 100

106 26.3 21.0 31.6

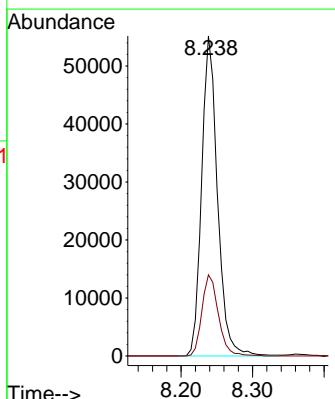





Abundance Scan 1368 (9.427 min): VX045563.D\data.ms

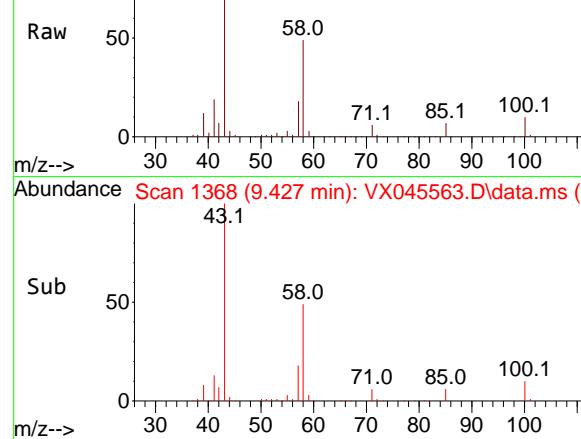


Abundance Scan 1368 (9.427 min): VX045563.D\data.ms (-1)

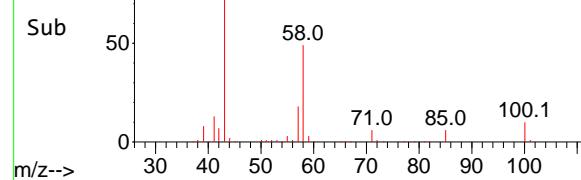


Abundance Scan 1383 (9.519 min): VX045528.D\data.ms (-1)

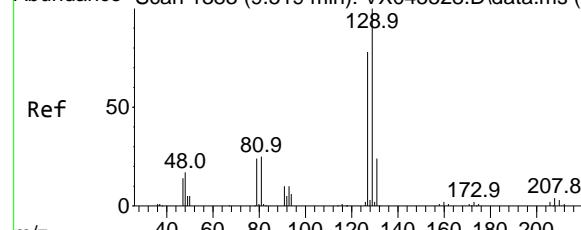

Abundance Scan 1383 (9.518 min): VX045563.D\data.ms

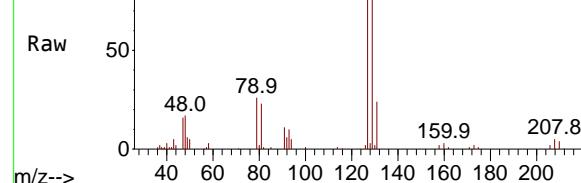

Abundance Scan 1383 (9.518 min): VX045563.D\data.ms (-1)

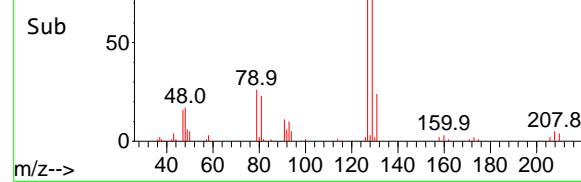

#59

2-Hexanone

Concen: 99.982 ug/l

RT: 9.427 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

Tgt Ion: 43 Resp: 15103

Ion Ratio Lower Upper

43 100


58 48.9 24.9 74.6

Manual Integrations


APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025


Supervised By :Mahesh Dadoda 04/04/2025

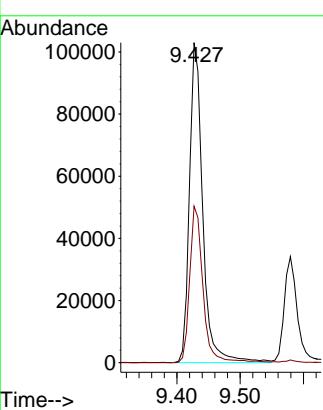


Abundance Scan 1383 (9.519 min): VX045528.D\data.ms (-1)

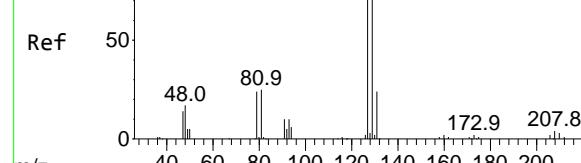

Abundance Scan 1383 (9.518 min): VX045563.D\data.ms

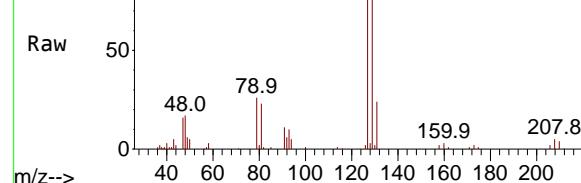

Abundance Scan 1383 (9.518 min): VX045563.D\data.ms (-1)

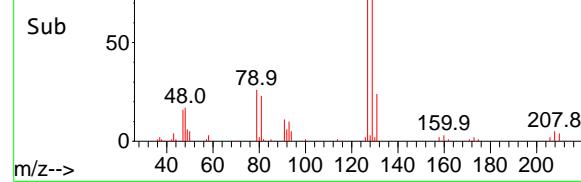

#60

Dibromochloromethane

Concen: 19.084 ug/l

RT: 9.518 min Scan# 1383

Delta R.T. -0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08




Tgt Ion:129 Resp: 24684

Ion Ratio Lower Upper

129 100

127 76.9 39.4 118.2

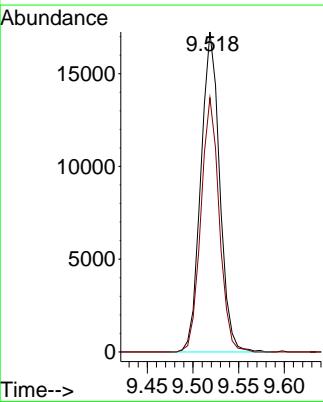



#61

1,2-Dibromoethane

Concen: 19.260 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08





Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

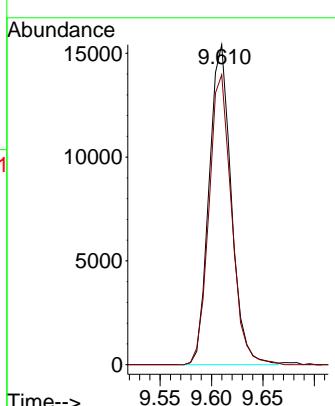 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#62

4-Bromofluorobenzene


Concen: 49.015 ug/l


RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

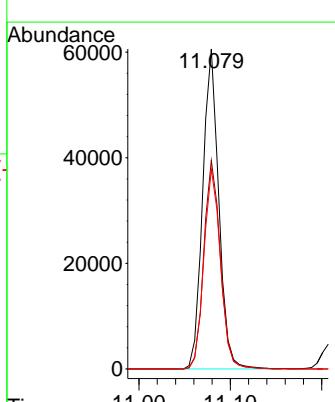 Tgt Ion: 95 Resp: 74358  
 Ion Ratio Lower Upper  
 95 100  
 174 67.0 0.0 135.8  
 176 64.3 0.0 131.4

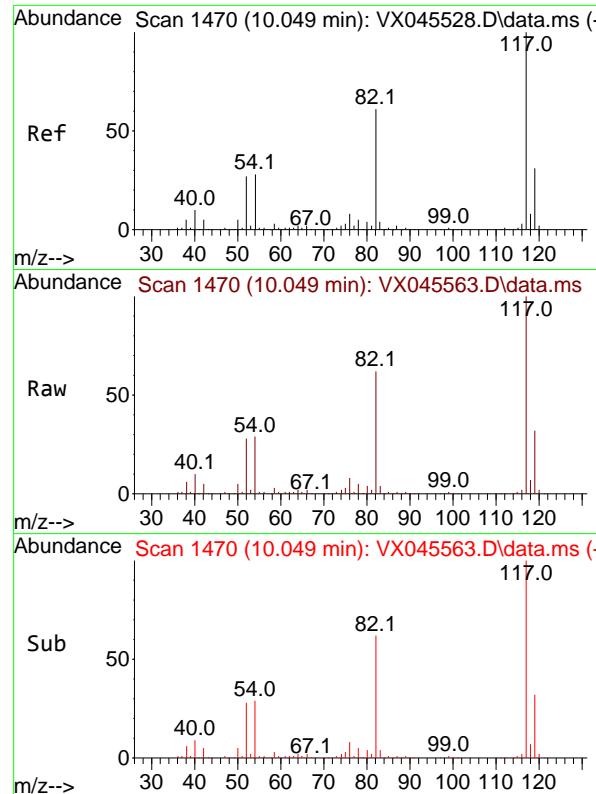


#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

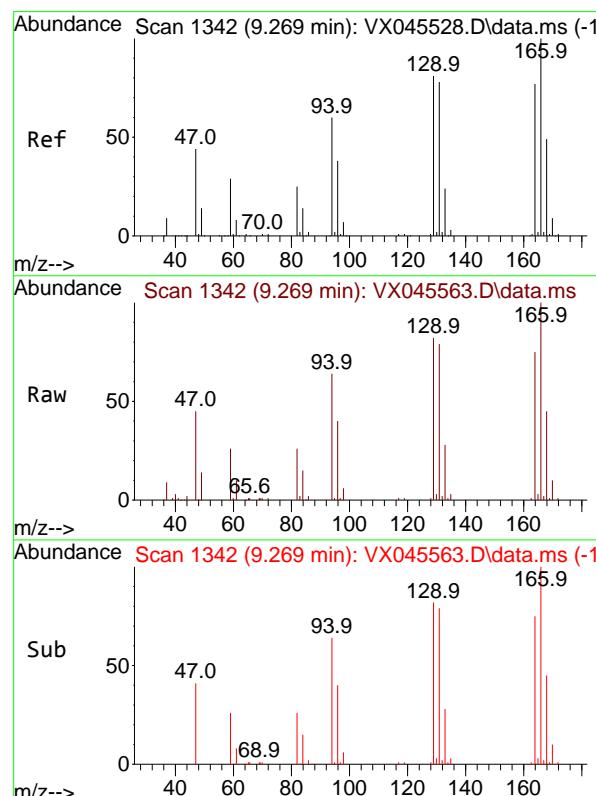 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#64

Tetrachloroethene

Concen: 18.445 ug/l


RT: 9.269 min Scan# 1342



Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Tgt	Ion:164	Resp:	19411
Ion	Ratio	Lower	Upper
164	100		
166	132.5	103.8	155.8
129	108.1	84.3	126.5
131	105.1	80.9	121.3

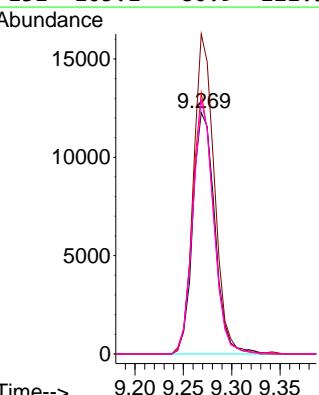

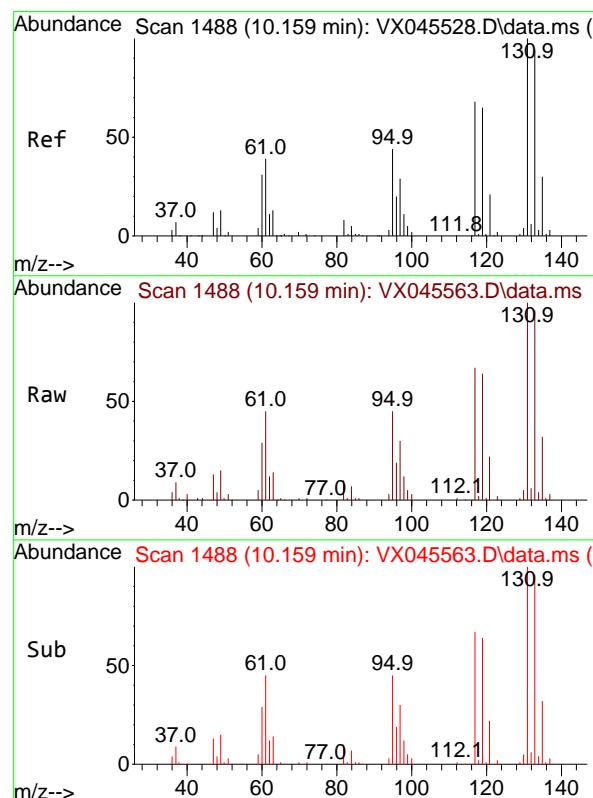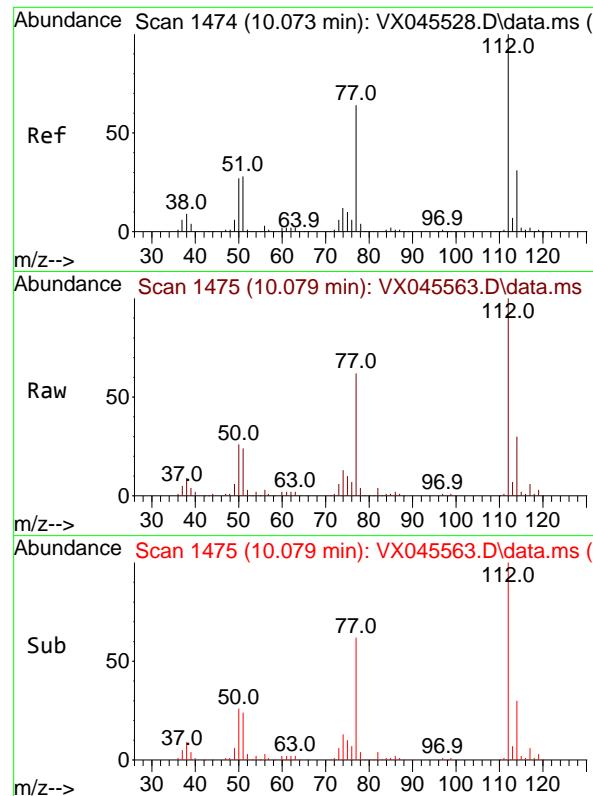

#65

Chlorobenzene

Concen: 19.149 ug/l

RT: 10.079 min Scan# 1475

Delta R.T. 0.006 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Instrument :

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#66

1,1,1,2-Tetrachloroethane


Concen: 18.479 ug/l




RT: 10.159 min Scan# 1488

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

 Tgt Ion:131 Resp: 20434  
 Ion Ratio Lower Upper  
 131 100  
 133 97.1 47.5 142.5  
 119 65.3 32.9 98.6

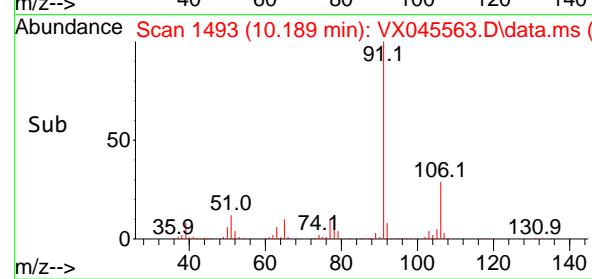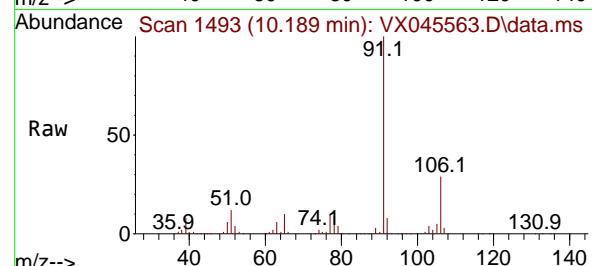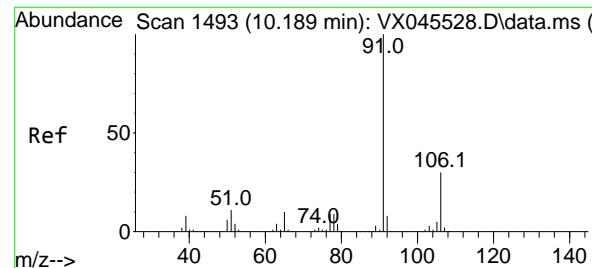


#67

Ethyl Benzene

Concen: 19.101 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08





Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

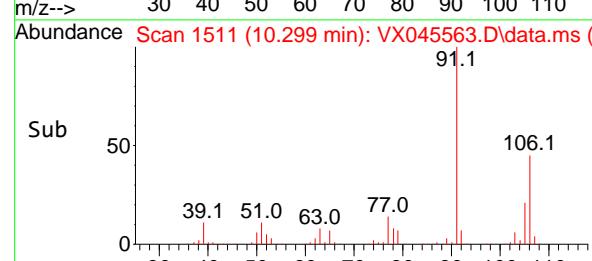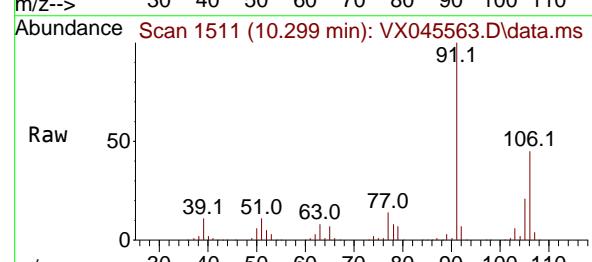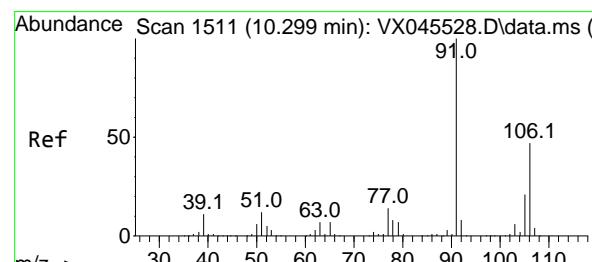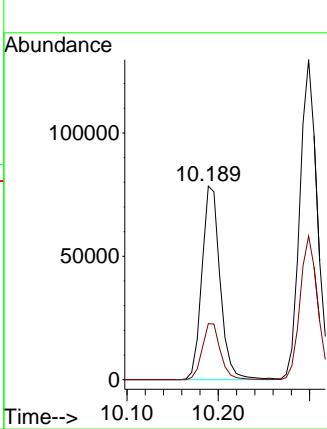 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#68

m/p-Xylenes


Concen: 38.276 ug/l


RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

 Tgt Ion:106 Resp: 79412  
 Ion Ratio Lower Upper  
 106 100  
 91 220.3 172.6 258.8

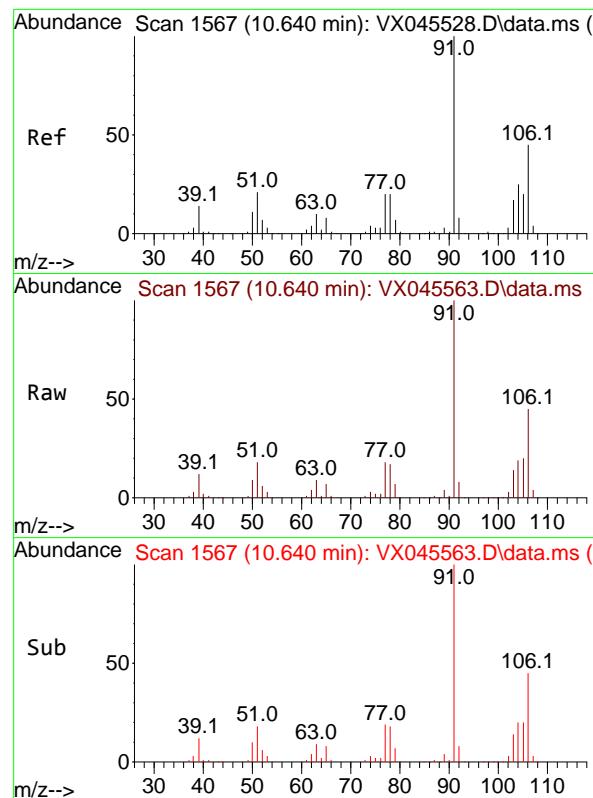
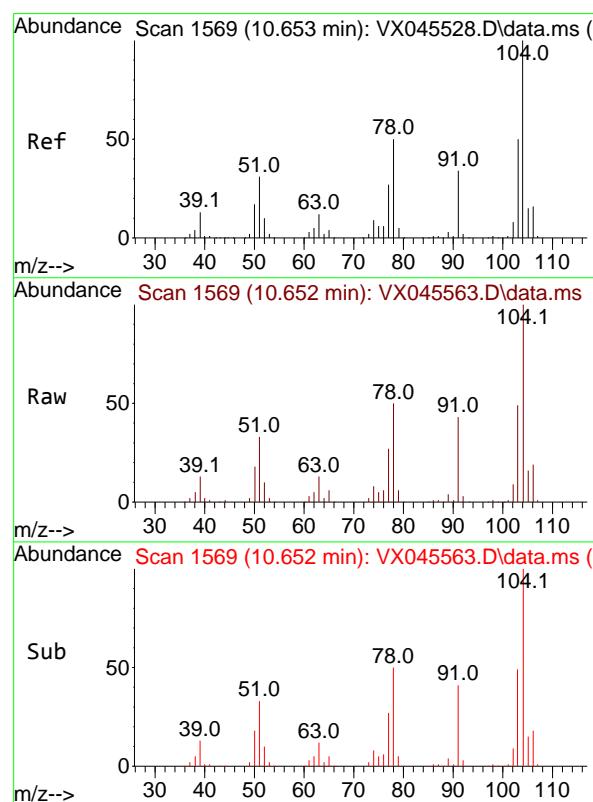



#69  
o-Xylene  
Concen: 19.052 ug/l  
RT: 10.640 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


**Manual Integrations**  
**APPROVED**




Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025



#70  
Styrene  
Concen: 19.607 ug/l  
RT: 10.652 min Scan# 1569  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion:104 Resp: 66139  
Ion Ratio Lower Upper  
104 100  
78 57.2 45.4 68.2  
103 55.0 43.8 65.8

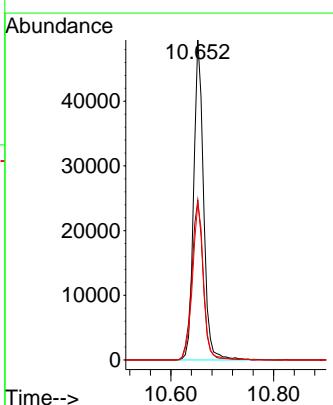



#71

Bromoform

Concen: 18.743 ug/l

RT: 10.799 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08





Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

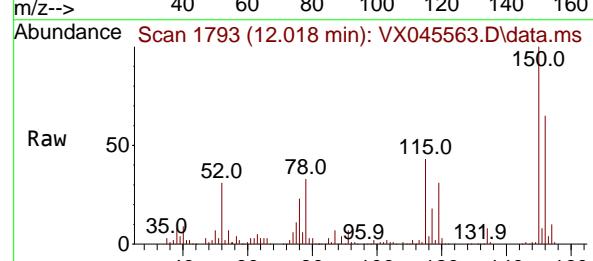 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l


RT: 12.018 min Scan# 1793


Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Tgt	Ion:152	Resp:	68919
Ion	Ratio	Lower	Upper
152	100		
115	74.1	46.9	140.7
150	160.0	0.0	349.4




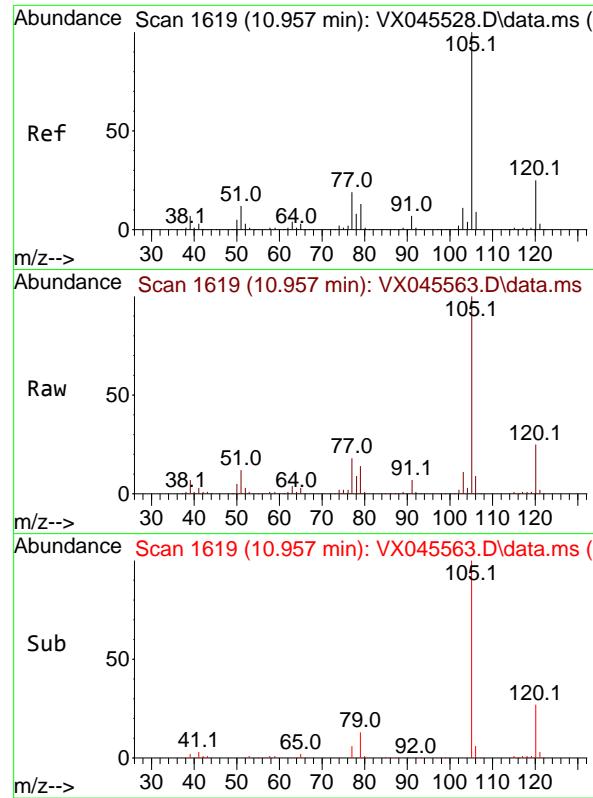


#73  
Isopropylbenzene  
Concen: 18.660 ug/l  
RT: 10.957 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


**Manual Integrations**  
**APPROVED**


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

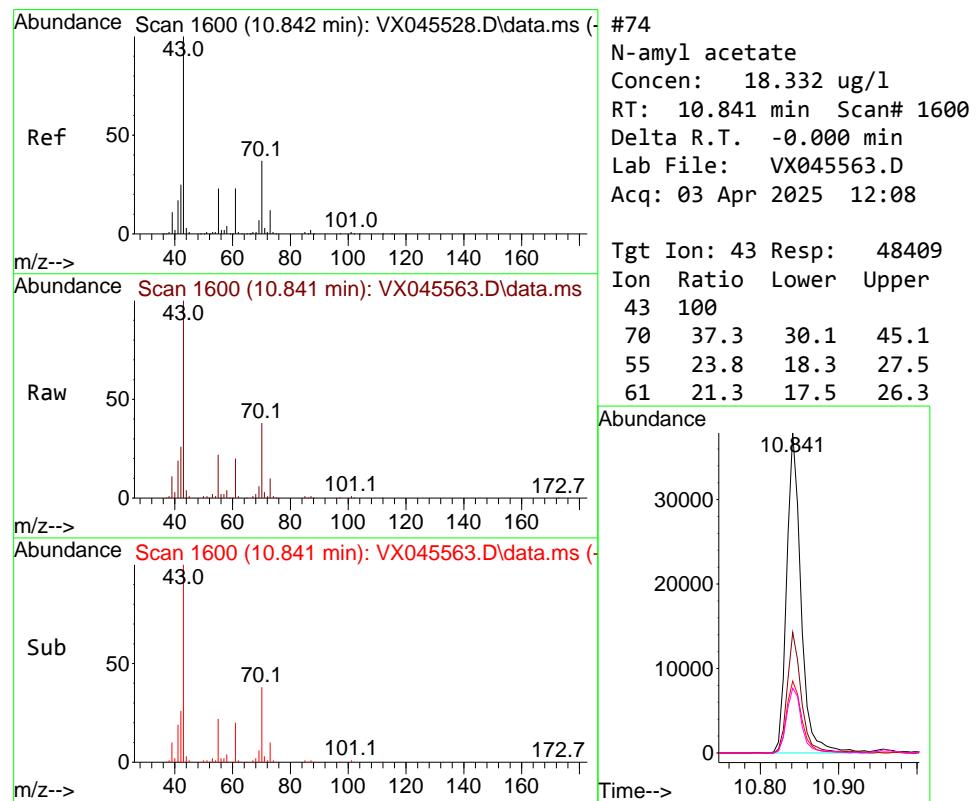

#74  
N-amyl acetate  
Concen: 18.332 ug/l  
RT: 10.841 min Scan# 1600  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 43 Resp: 48409  
Ion Ratio Lower Upper  
43 100  
70 37.3 30.1 45.1  
55 23.8 18.3 27.5  
61 21.3 17.5 26.3

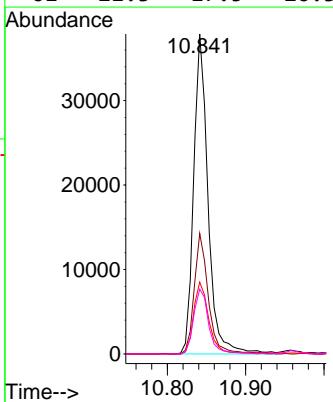

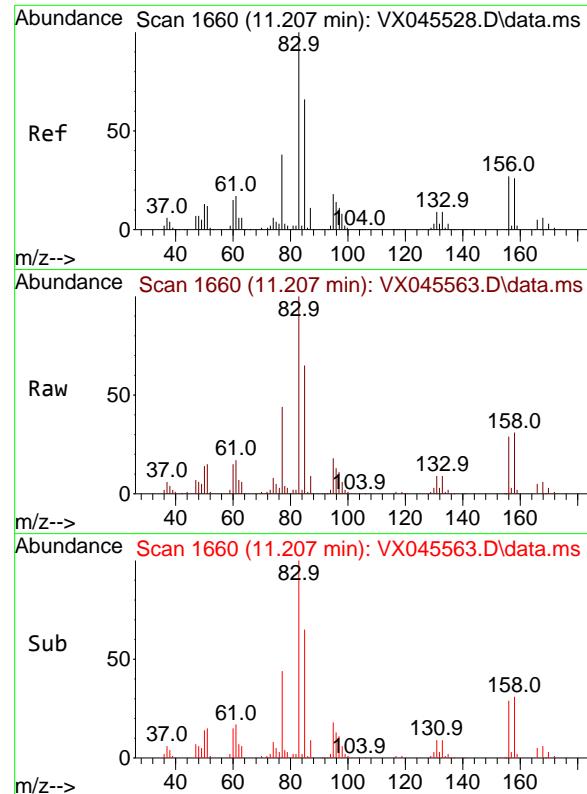


#75  
1,1,2,2-Tetrachloroethane  
Concen: 18.620 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


**Manual Integrations**  
**APPROVED**




Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

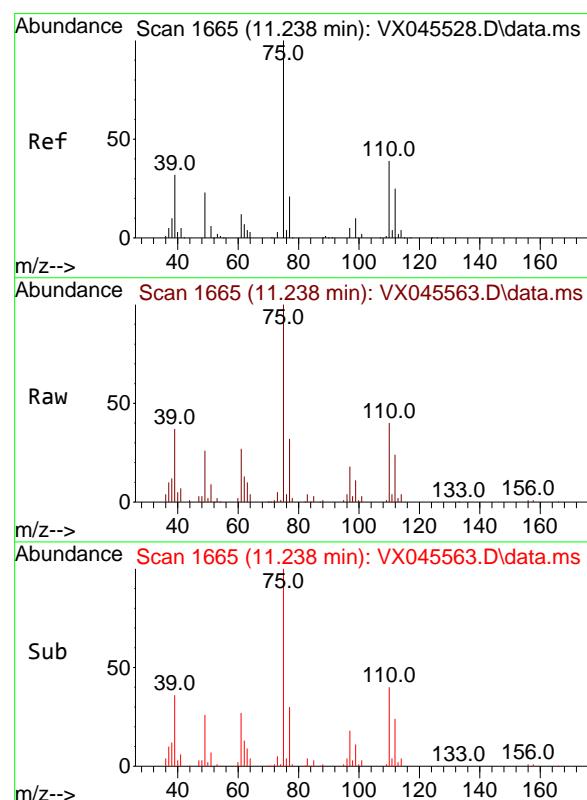

#76  
1,2,3-Trichloropropane  
Concen: 18.624 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 75 Resp: 31309  
Ion Ratio Lower Upper  
75 100  
77 39.3 20.0 59.9

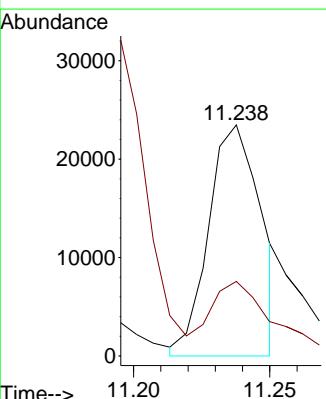



#77

Bromobenzene

Concen: 18.399 ug/l

RT: 11.195 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08





Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

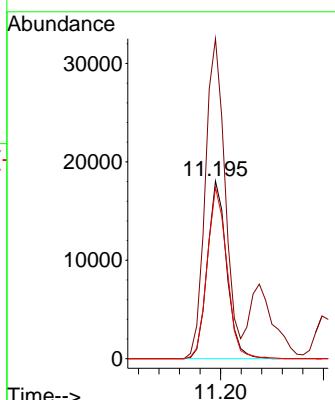 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#78

n-propylbenzene


Concen: 18.717 ug/l




RT: 11.299 min Scan# 1675

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

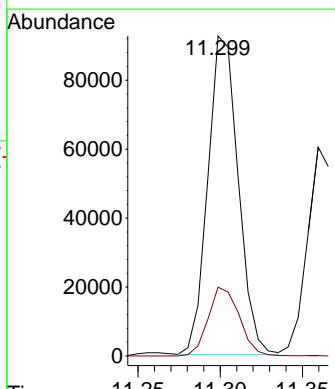 Tgt Ion: 91 Resp: 119014  
 Ion Ratio Lower Upper  
 91 100  
 120 22.1 10.8 32.3

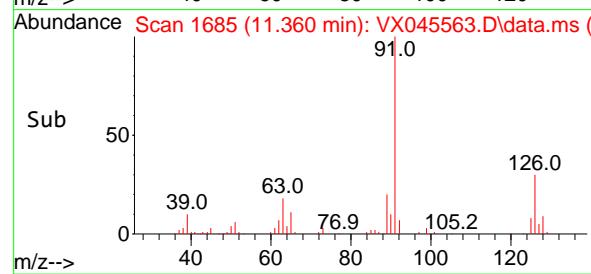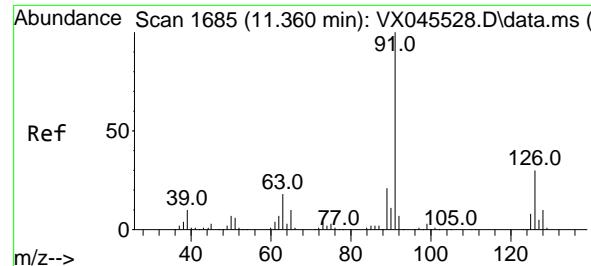


#79

2-Chlorotoluene

Concen: 18.633 ug/l

RT: 11.360 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08




Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

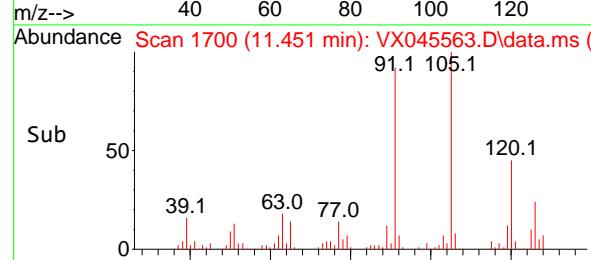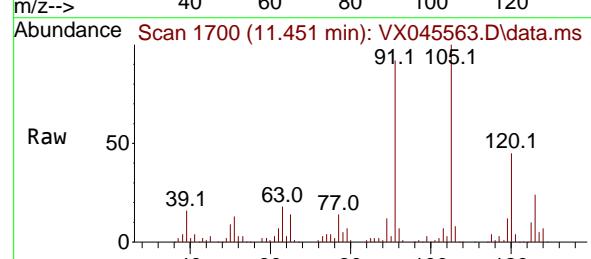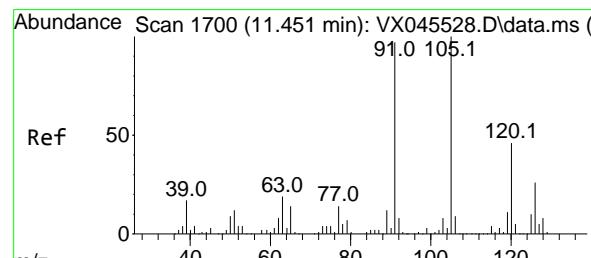 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#80

1,3,5-Trimethylbenzene

Concen: 19.270 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX045563.D


Acq: 03 Apr 2025 12:08


Tgt Ion:105 Resp: 87968

Ion Ratio Lower Upper

105 100

120 45.8 23.0 69.0

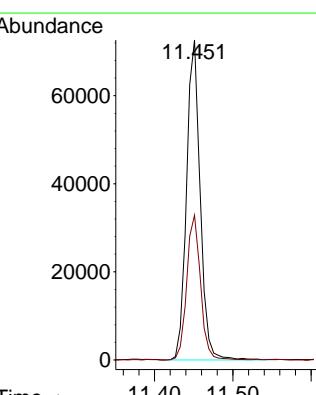


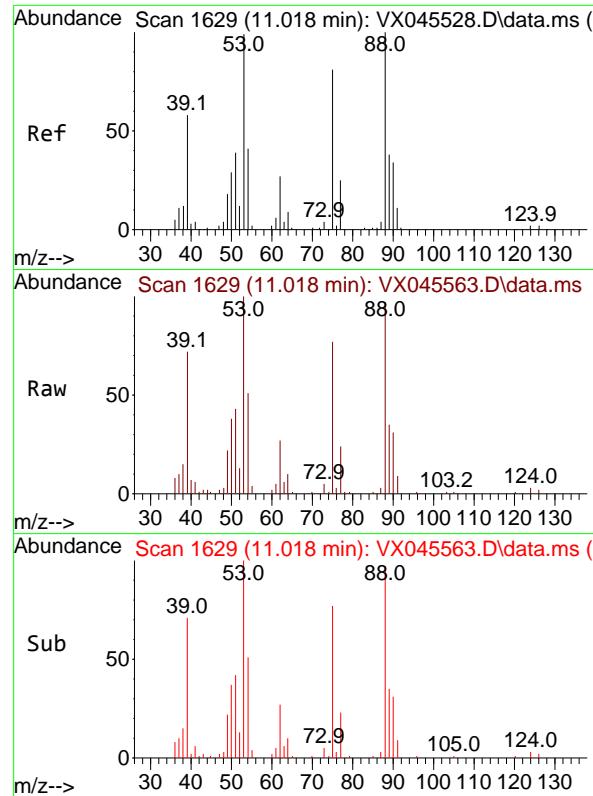


#81  
trans-1,4-Dichloro-2-butene  
Concen: 16.837 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


### Manual Integrations APPROVED




Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

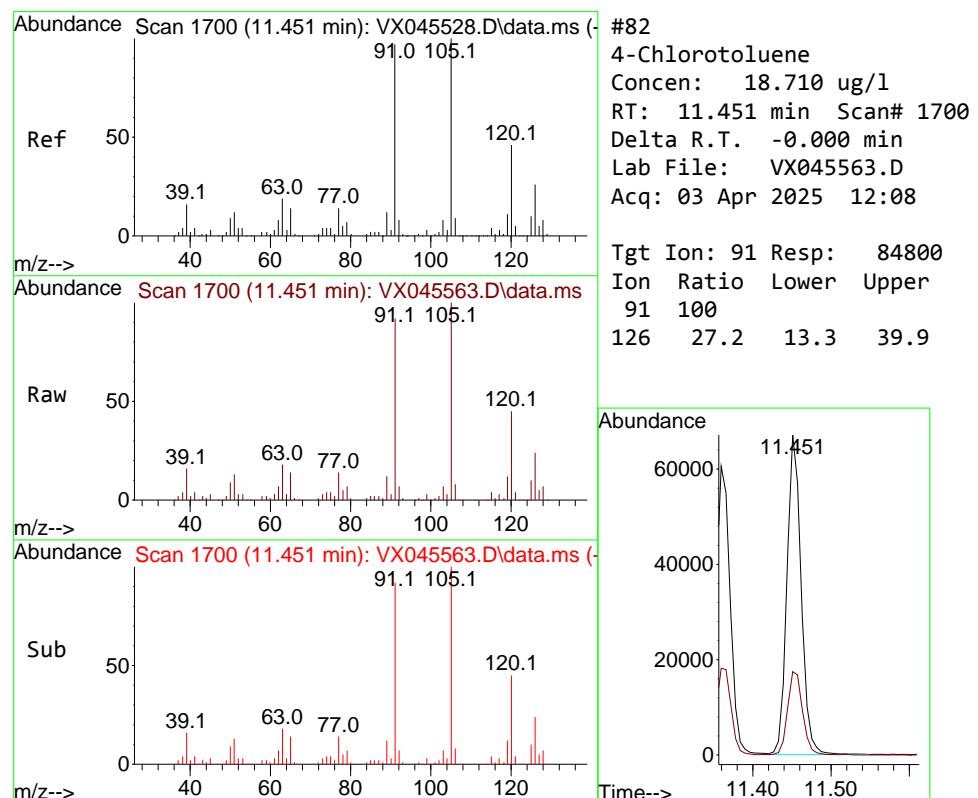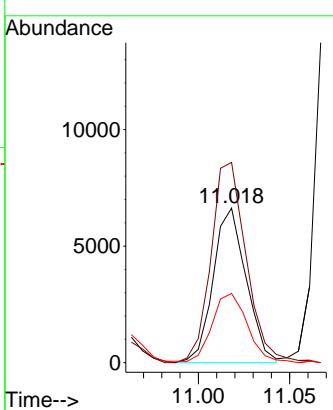

#82  
4-Chlorotoluene  
Concen: 18.710 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion: 91 Resp: 84800  
Ion Ratio Lower Upper  
91 100  
126 27.2 13.3 39.9





#83

tert-Butylbenzene

Concen: 19.049 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08




Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#84

1,2,4-Trimethylbenzene

Concen: 19.196 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min



Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Tgt Ion:105 Resp: 87951

Ion Ratio Lower Upper

Tgt Ion	Ratio	Lower	Upper
105	100		
120	43.2	21.4	64.3

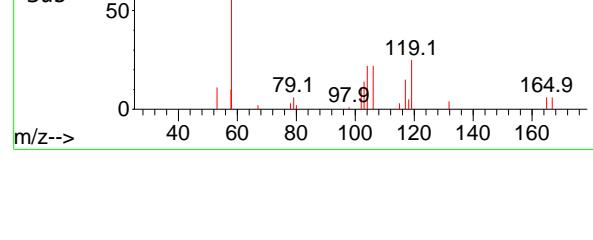

Abundance

Time--&gt;

11.65 11.70 11.75

11.713

60000 40000 20000 0




Time--&gt;

11.70 11.80

80000 60000 40000 20000 0

Time--&gt;

11.750



#85

sec-Butylbenzene

Concen: 19.401 ug/l

RT: 11.890 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08




Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#86

p-Isopropyltoluene

Concen: 19.078 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Tgt Ion:119 Resp: 87307




Ion Ratio Lower Upper

119 100

134 25.7 12.6 37.8

91 27.8 13.7 41.1

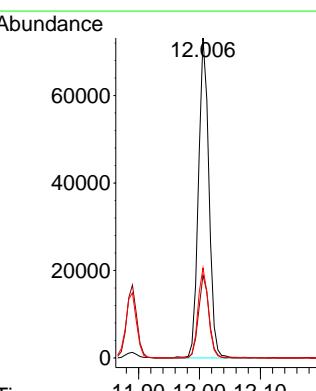



#87

1,3-Dichlorobenzene

Concen: 18.035 ug/l

RT: 11.969 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08





Instrument:

MSVOA\_X

ClientSampleId :

VX0403WBS01

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#88

1,4-Dichlorobenzene

Concen: 18.215 ug/l

RT: 12.036 min Scan# 1796

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08


Tgt Ion:146 Resp: 42877




Ion Ratio Lower Upper

146 100

111 44.2 20.9 62.8

148 64.3 31.5 94.5

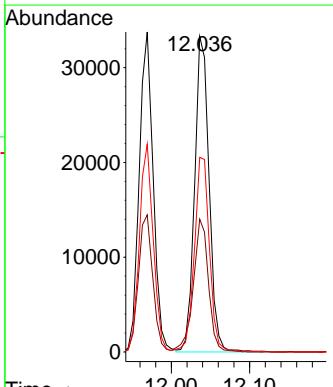



#89

n-Butylbenzene

Concen: 18.388 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min





Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X

ClientSampleId : VX0403WBS01

**Manual Integrations  
APPROVED**

 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#90

Hexachloroethane


Concen: 19.256 ug/l




RT: 12.536 min Scan# 1878

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08

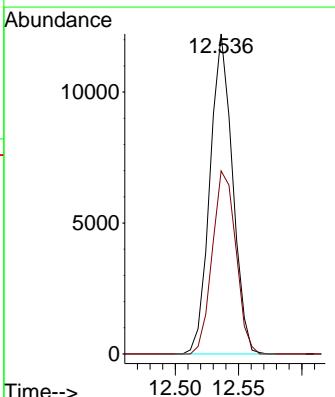 Tgt Ion: 117 Resp: 15145  
 Ion Ratio Lower Upper  
 117 100  
 201 59.8 31.2 93.6




#91

1,2-Dichlorobenzene

Concen: 18.317 ug/l

RT: 12.335 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045563.D

Acq: 03 Apr 2025 12:08




Instrument:

MSVOA\_X


ClientSampleId :


VX0403WBS01

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#92  
 1,2-Dibromo-3-Chloropropane  
 Concen: 18.685 ug/l  
 RT: 12.945 min Scan# 1945  
 Delta R.T. 0.006 min  
 Lab File: VX045563.D  
 Acq: 03 Apr 2025 12:08

 Tgt Ion: 75 Resp: 7578  
 Ion Ratio Lower Upper  
 75 100  
 155 71.2 34.9 104.7  
 157 90.8 44.9 134.7

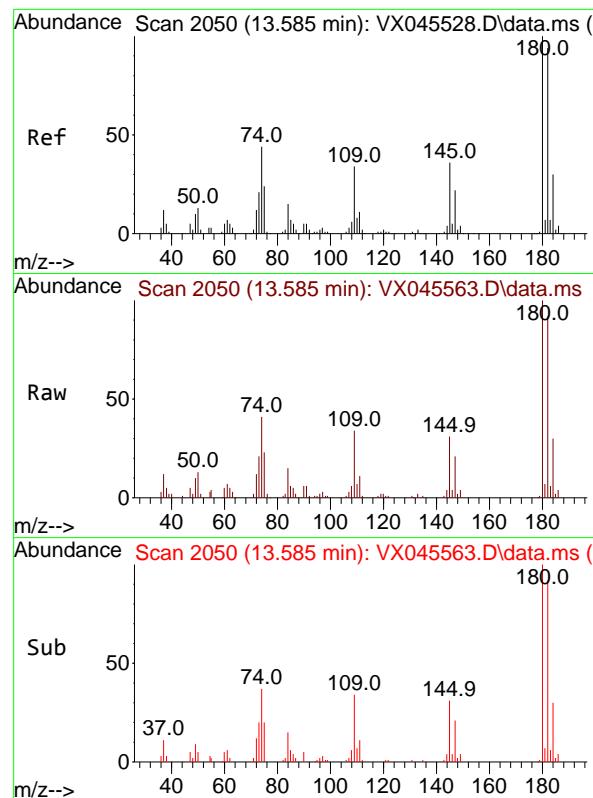
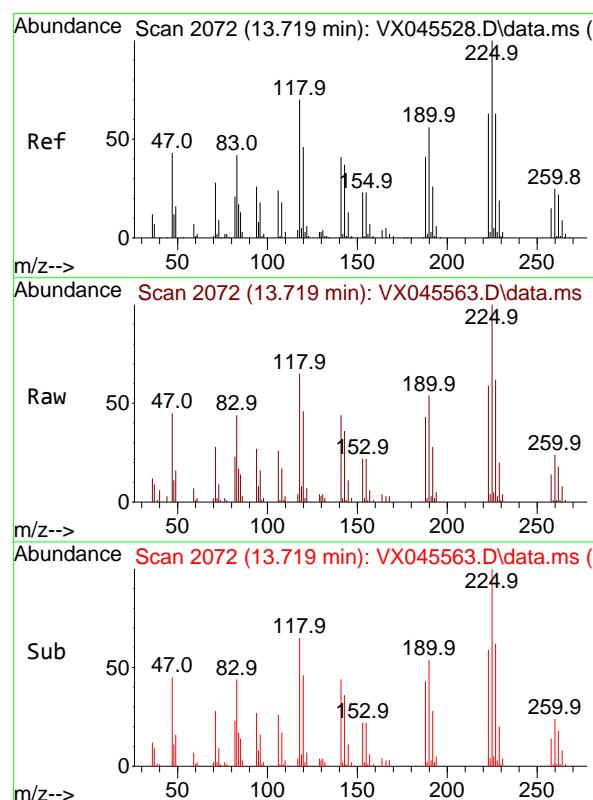



#93  
1,2,4-Trichlorobenzene  
Concen: 17.574 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025



#94  
Hexachlorobutadiene  
Concen: 18.232 ug/l  
RT: 13.719 min Scan# 2072  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion:225 Resp: 10095  
Ion Ratio Lower Upper  
225 100  
223 62.5 31.1 93.3  
227 62.8 32.2 96.6

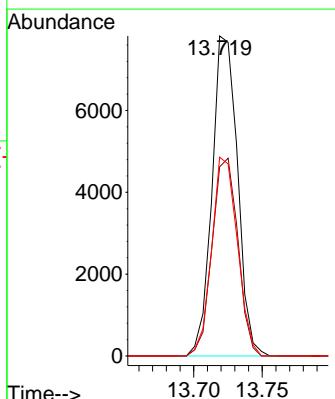


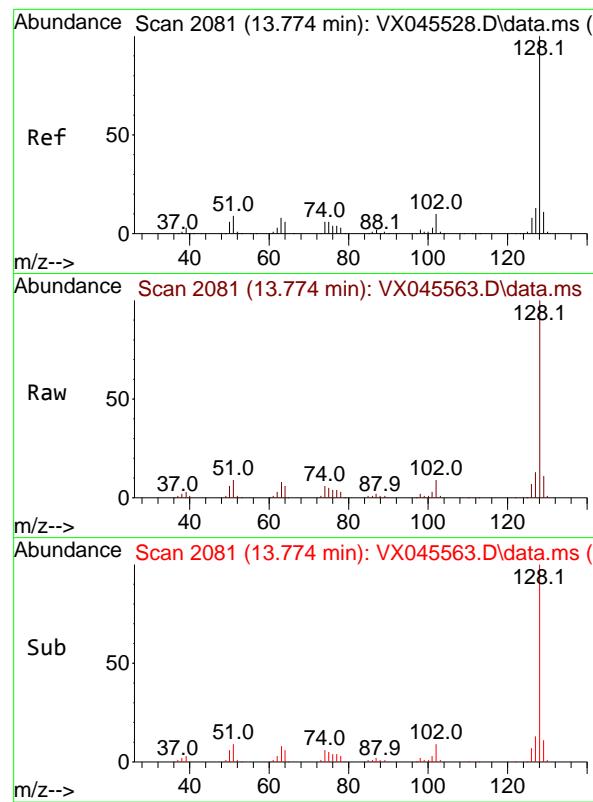


#95  
Naphthalene  
Concen: 17.350 ug/l  
RT: 13.774 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Instrument : MSVOA\_X  
ClientSampleId : VX0403WBS01


**Manual Integrations**  
**APPROVED**

Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

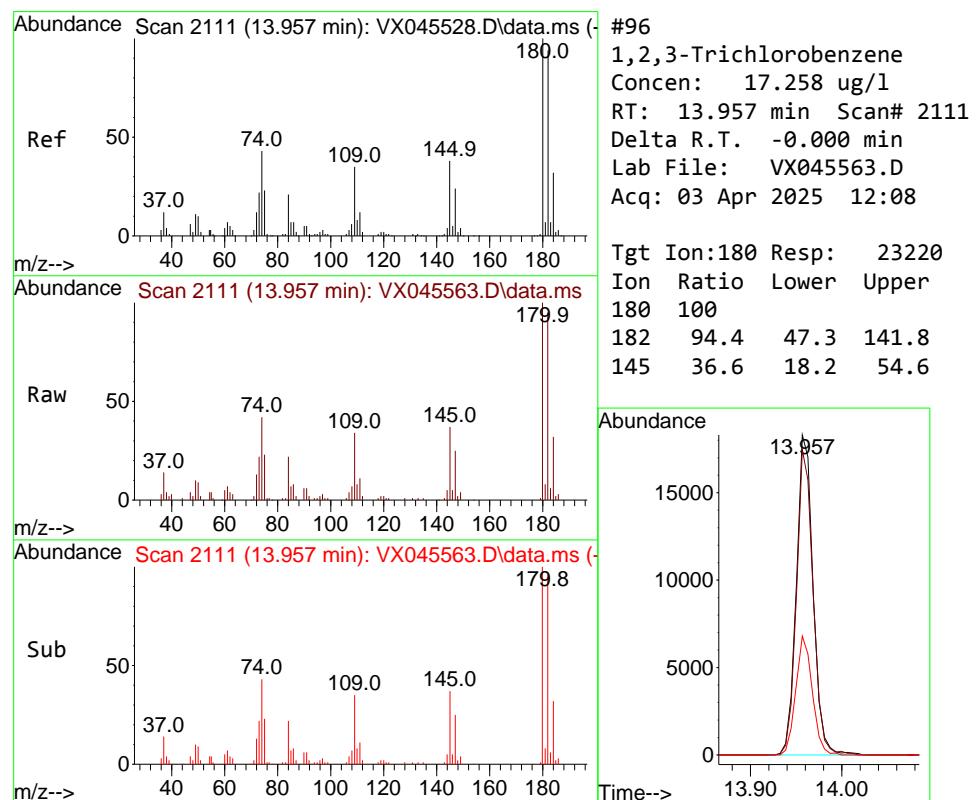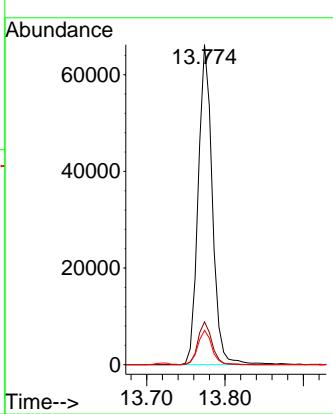

#96  
1,2,3-Trichlorobenzene  
Concen: 17.258 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX045563.D  
Acq: 03 Apr 2025 12:08

Tgt Ion:180 Resp: 23220  
Ion Ratio Lower Upper  
180 100  
182 94.4 47.3 141.8  
145 36.6 18.2 54.6

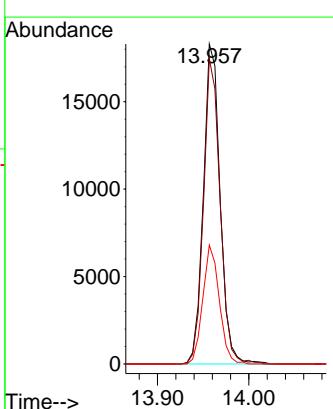



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	
Client Sample ID:	VX0404WBS01			SDG No.:	Q1711
Lab Sample ID:	VX0404WBS01			Matrix:	Water
Analytical Method:	SW8260			% Solid:	0
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000 uL
Soil Aliquot Vol:			uL	Test:	VOCMS Group3
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045589.D	1		04/04/25 11:14	VX040425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	19.6		0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	19.4		0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	19.5		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	19.2		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	19.7		0.20	1.00	ug/L
71-43-2	Benzene	19.9		0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	20.4		0.22	1.00	ug/L
79-01-6	Trichloroethene	19.2		0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	20.5		0.21	1.00	ug/L
127-18-4	Tetrachloroethene	19.6		0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	52.9		70 (74) - 130 (125)	106%	SPK: 50
1868-53-7	Dibromofluoromethane	53.3		70 (75) - 130 (124)	107%	SPK: 50
2037-26-5	Toluene-d8	53.2		70 (86) - 130 (113)	106%	SPK: 50
460-00-4	4-Bromofluorobenzene	53.2		70 (77) - 130 (121)	106%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	95100		5.549		
540-36-3	1,4-Difluorobenzene	168000		6.757		
3114-55-4	Chlorobenzene-d5	152000		10.049		
3855-82-1	1,4-Dichlorobenzene-d4	66600		12.018		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045589.D  
 Acq On : 04 Apr 2025 11:14  
 Operator : JC/MD  
 Sample : VX0404WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0404WBS01

Quant Time: Apr 04 23:10:41 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.549	168	95127	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	168453	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	151744	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	66584	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	91980	52.873	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 105.740%		
35) Dibromofluoromethane	5.385	113	63679	53.280	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 106.560%		
50) Toluene-d8	8.646	98	221910	53.195	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 106.400%		
62) 4-Bromofluorobenzene	11.079	95	80880	53.227	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 106.460%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	30356	21.338	ug/l	98
3) Chloromethane	1.306	50	28046	19.190	ug/l	97
4) Vinyl Chloride	1.373	62	26269	19.640	ug/l	99
5) Bromomethane	1.593	94	12147	19.154	ug/l	100
6) Chloroethane	1.666	64	14563	20.522	ug/l	98
7) Trichlorofluoromethane	1.873	101	40168	20.139	ug/l	95
8) Diethyl Ether	2.135	74	13256	19.796	ug/l	98
9) 1,1,2-Trichlorotrifluo...	2.318	101	23531	20.134	ug/l	98
10) Methyl Iodide	2.446	142	27472	18.845	ug/l	97
11) Tert butyl alcohol	2.971	59	22553	96.466	ug/l	99
12) 1,1-Dichloroethene	2.312	96	22114	19.364	ug/l	97
13) Acrolein	2.233	56	35297	109.636	ug/l	96
14) Allyl chloride	2.660	41	42970	19.831	ug/l	99
15) Acrylonitrile	3.062	53	73835	100.048	ug/l	99
16) Acetone	2.379	43	71844	100.574	ug/l	95
17) Carbon Disulfide	2.507	76	51789	18.361	ug/l	100
18) Methyl Acetate	2.702	43	33157	20.160	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	77491	19.397	ug/l	98
20) Methylene Chloride	2.782	84	26080	19.502	ug/l	98
21) trans-1,2-Dichloroethene	3.086	96	22921	19.646	ug/l	95
22) Diisopropyl ether	3.757	45	82229	19.265	ug/l #	85
23) Vinyl Acetate	3.721	43	363855	98.665	ug/l	99
24) 1,1-Dichloroethane	3.605	63	46953	19.451	ug/l	99
25) 2-Butanone	4.556	43	106093	101.462	ug/l	99
26) 2,2-Dichloropropane	4.464	77	32865	21.073	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	27229	19.156	ug/l	99
28) Bromochloromethane	4.891	49	23795	20.399	ug/l	97
29) Tetrahydrofuran	5.007	42	66295	97.791	ug/l	99
30) Chloroform	5.086	83	49173	19.797	ug/l	94
31) Cyclohexane	5.464	56	41598	19.493	ug/l	99
32) 1,1,1-Trichloroethane	5.379	97	41502	19.747	ug/l	98
36) 1,1-Dichloropropene	5.684	75	31963	19.807	ug/l	98
37) Ethyl Acetate	4.714	43	38551	18.957	ug/l	99
38) Carbon Tetrachloride	5.671	117	35237	20.204	ug/l	95
39) Methylcyclohexane	7.372	83	39542	19.990	ug/l	95
40) Benzene	6.031	78	97905	19.865	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045589.D  
 Acq On : 04 Apr 2025 11:14  
 Operator : JC/MD  
 Sample : VX0404WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0404WBS01

Quant Time: Apr 04 23:10:41 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	22088	20.585	ug/1	98
42) 1,2-Dichloroethane	6.086	62	41452	20.364	ug/1	100
43) Isopropyl Acetate	6.342	43	59314	19.244	ug/1	99
44) Trichloroethene	7.122	130	22535	19.237	ug/1	89
45) 1,2-Dichloropropane	7.427	63	24353	19.804	ug/1	92
46) Dibromomethane	7.580	93	19189	20.328	ug/1	98
47) Bromodichloromethane	7.817	83	37575	19.932	ug/1	96
48) Methyl methacrylate	7.689	41	31993	20.104	ug/1	99
49) 1,4-Dioxane	7.659	88	11949	414.998	ug/1	98
51) 4-Methyl-2-Pentanone	8.573	43	209485	102.524	ug/1	99
52) Toluene	8.714	92	58522	19.623	ug/1	98
53) t-1,3-Dichloropropene	8.976	75	30749	18.474	ug/1	99
54) cis-1,3-Dichloropropene	8.366	75	35158	19.846	ug/1	96
55) 1,1,2-Trichloroethane	9.152	97	24341	20.482	ug/1	95
56) Ethyl methacrylate	9.116	69	36657	19.931	ug/1	98
57) 1,3-Dichloropropane	9.305	76	42216	20.400	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.238	63	95516	102.664	ug/1	99
59) 2-Hexanone	9.427	43	152877	101.036	ug/1	98
60) Dibromochloromethane	9.518	129	25841	19.946	ug/1	99
61) 1,2-Dibromoethane	9.610	107	23976	19.930	ug/1	100
64) Tetrachloroethene	9.274	164	21048	19.646	ug/1	97
65) Chlorobenzene	10.079	112	63546	19.598	ug/1	98
66) 1,1,1,2-Tetrachloroethane	10.158	131	22150	19.676	ug/1	97
67) Ethyl Benzene	10.189	91	113903	19.613	ug/1	98
68) m/p-Xylenes	10.299	106	82893	39.245	ug/1	99
69) o-Xylene	10.640	106	41423	19.908	ug/1	99
70) Styrene	10.652	104	68156	19.846	ug/1	98
71) Bromoform	10.799	173	15776	18.768	ug/1 #	96
73) Isopropylbenzene	10.963	105	109126	20.461	ug/1	100
74) N-amyl acetate	10.841	43	49771	19.508	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	37577	20.056	ug/1	96
76) 1,2,3-Trichloropropane	11.237	75	31448m	19.363	ug/1	
77) Bromobenzene	11.195	156	25007	20.293	ug/1	98
78) n-propylbenzene	11.298	91	126822	20.644	ug/1	99
79) 2-Chlorotoluene	11.359	91	78774	20.058	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	91980	20.856	ug/1	99
81) trans-1,4-Dichloro-2-b...	11.018	75	8789	18.366	ug/1	95
82) 4-Chlorotoluene	11.451	91	90453	20.657	ug/1	100
83) tert-Butylbenzene	11.713	119	88794	20.336	ug/1	97
84) 1,2,4-Trimethylbenzene	11.750	105	91248	20.614	ug/1	99
85) sec-Butylbenzene	11.890	105	111812	20.849	ug/1	100
86) p-Isopropyltoluene	12.006	119	90695	20.513	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	44092	19.656	ug/1	99
88) 1,4-Dichlorobenzene	12.036	146	44331	19.494	ug/1	98
89) n-Butylbenzene	12.329	91	77639	20.250	ug/1	99
90) Hexachloroethane	12.536	117	15371	20.229	ug/1	99
91) 1,2-Dichlorobenzene	12.335	146	44325	19.875	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.938	75	7932	20.243	ug/1	97
93) 1,2,4-Trichlorobenzene	13.585	180	23660	19.059	ug/1	97
94) Hexachlorobutadiene	13.725	225	10408	19.457	ug/1	97
95) Naphthalene	13.774	128	87543	18.950	ug/1	100
96) 1,2,3-Trichlorobenzene	13.956	180	24870	19.132	ug/1	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045589.D  
 Acq On : 04 Apr 2025 11:14  
 Operator : JC/MD  
 Sample : VX0404WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0404WBS01

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Quant Time: Apr 04 23:10:41 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
Data File : VX045589.D  
Acq On : 04 Apr 2025 11:14  
Operator : JC/MD  
Sample : VX0404WBS01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VX0404WBS01

## Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

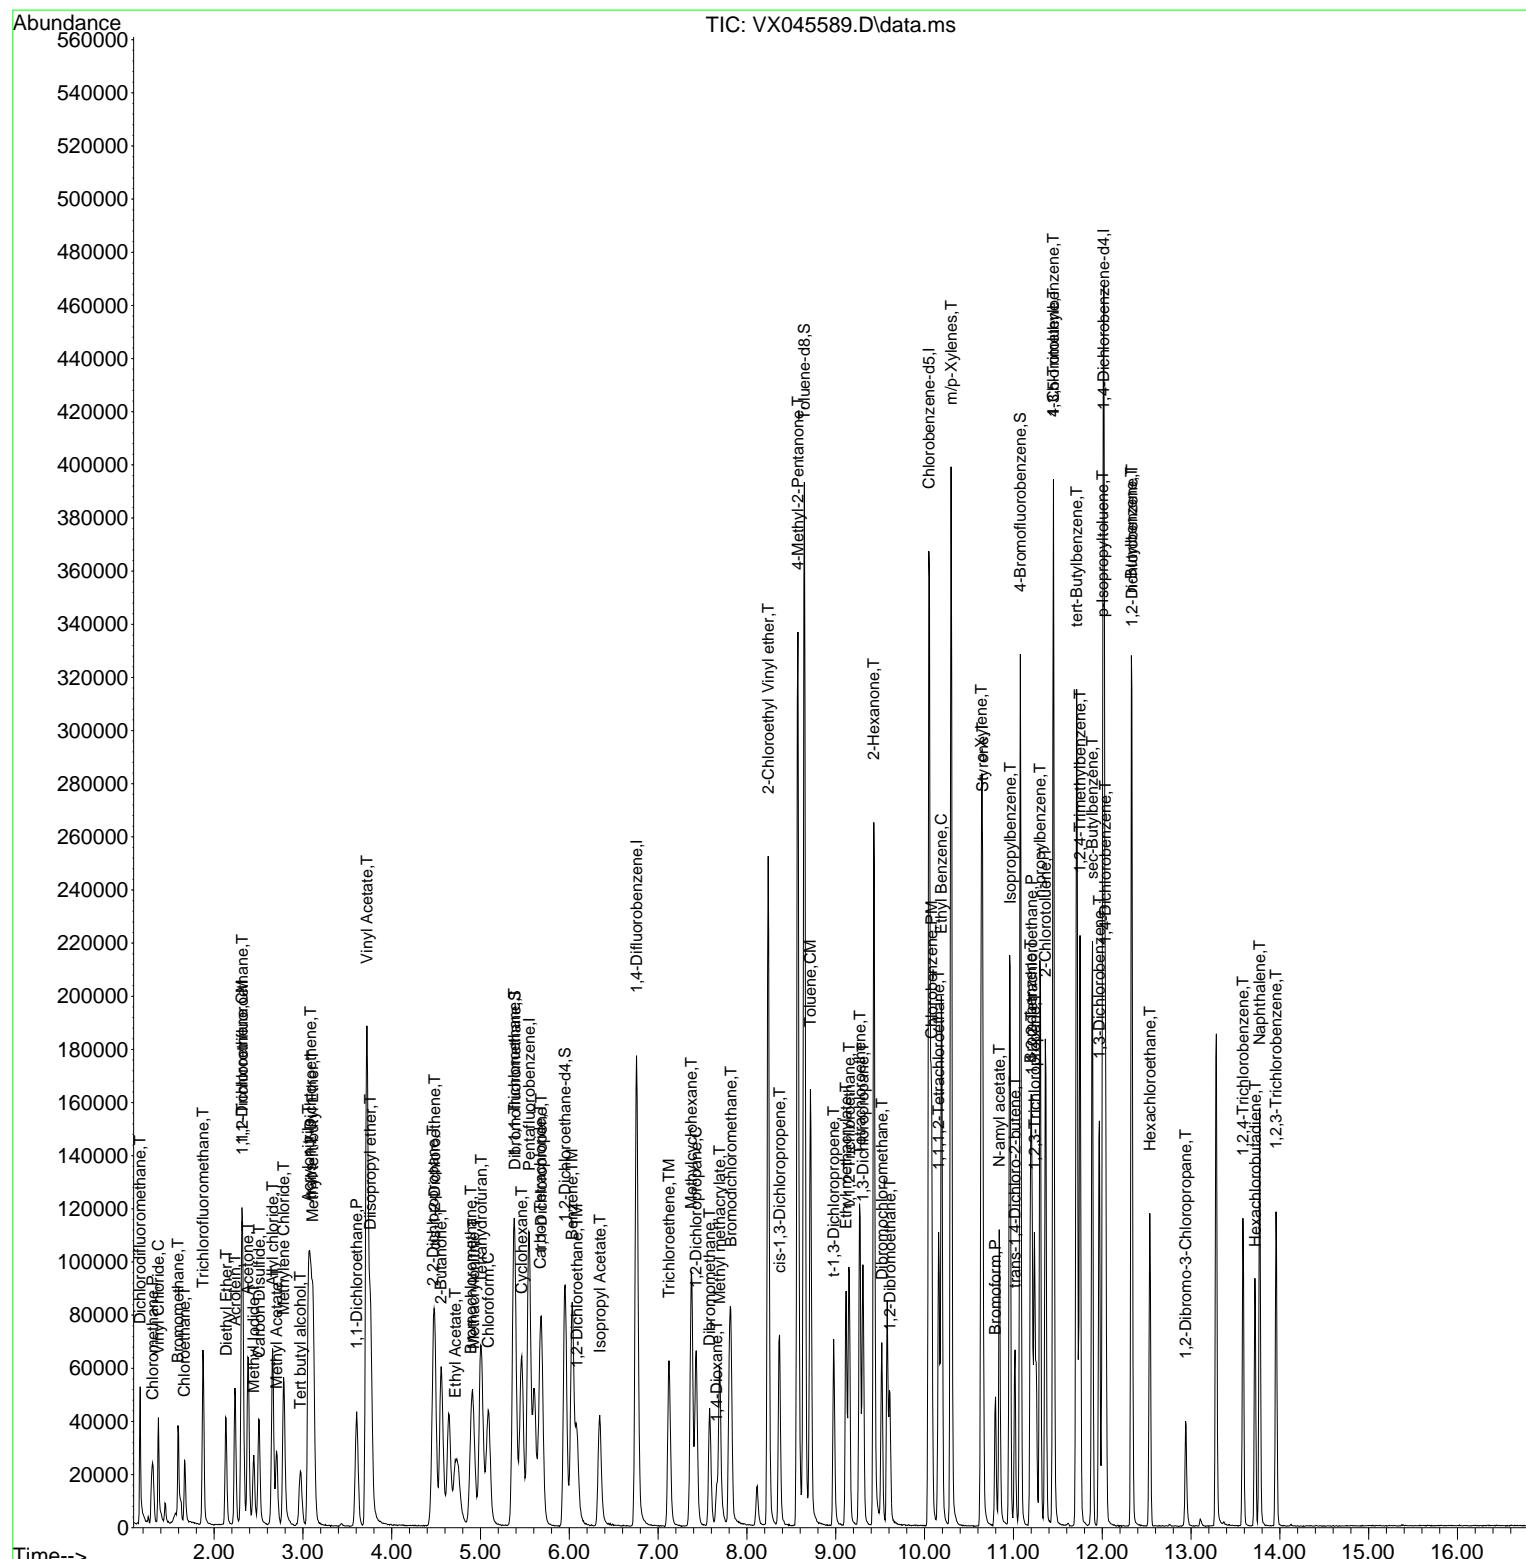







#1  
 Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.549 min Scan# 7  
 Delta R.T. -0.001 min  
 Lab File: VX045589.D  
 Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
 ClientSampleId : VX0404WBS01


### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

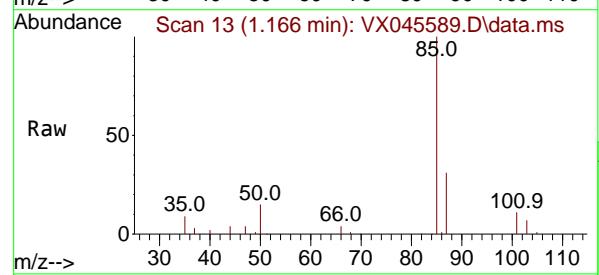





#2  
 Dichlorodifluoromethane  
 Concen: 21.338 ug/l  
 RT: 1.166 min Scan# 13  
 Delta R.T. -0.000 min  
 Lab File: VX045589.D  
 Acq: 04 Apr 2025 11:14

Tgt Ion: 85 Resp: 30356  
 Ion Ratio Lower Upper  
 85 100  
 87 30.9 16.1 48.2

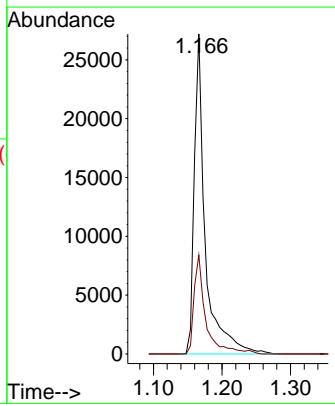



Abundance Scan 36 (1.306 min): VX045589.D\data.ms

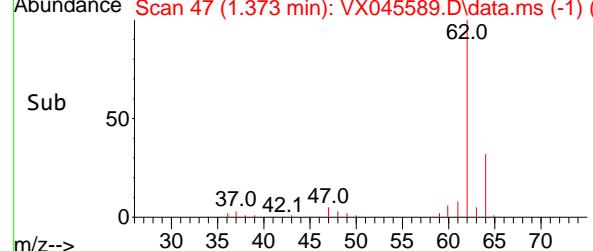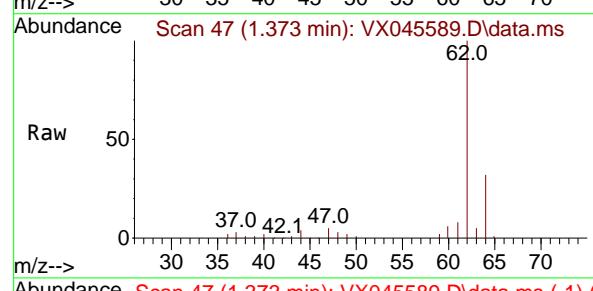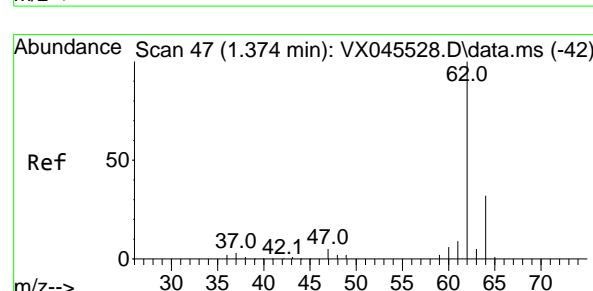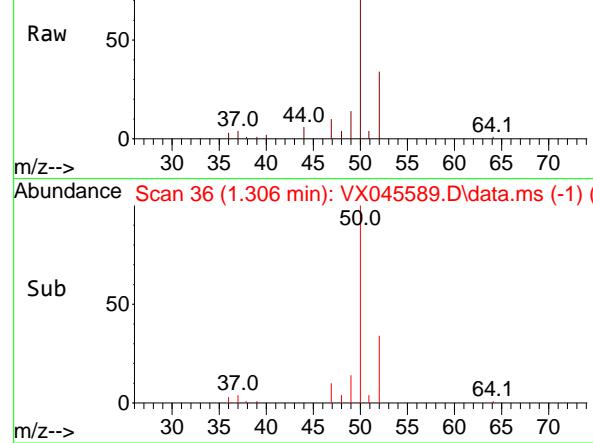

#3

Chloromethane

Concen: 19.190 ug/l

RT: 1.306 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X

ClientSampleId :

VX0404WBS01

Tgt Ion: 50 Resp: 28040

Ion Ratio Lower Upper

50 100


52 34.1 25.9 38.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#4

Vinyl Chloride

Concen: 19.640 ug/l

RT: 1.373 min Scan# 47

Delta R.T. -0.000 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14




Tgt Ion: 62 Resp: 26269

Ion Ratio Lower Upper

62 100

64 32.3 25.5 38.3









#5  
Bromomethane  
Concen: 19.154 ug/l  
RT: 1.593 min Scan# 8  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

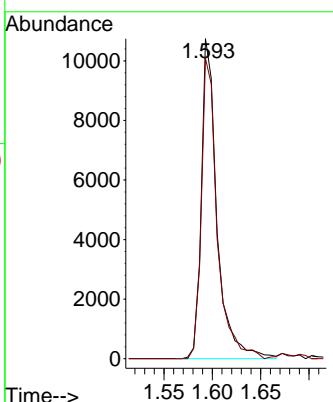

#6  
Chloroethane  
Concen: 20.522 ug/l  
RT: 1.666 min Scan# 95  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 64 Resp: 14563  
Ion Ratio Lower Upper  
64 100  
66 31.6 26.3 39.5

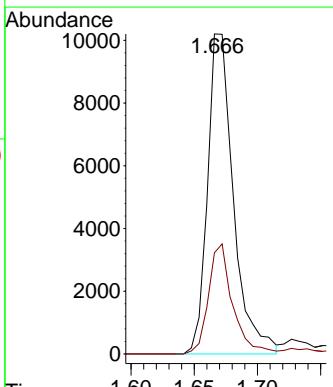


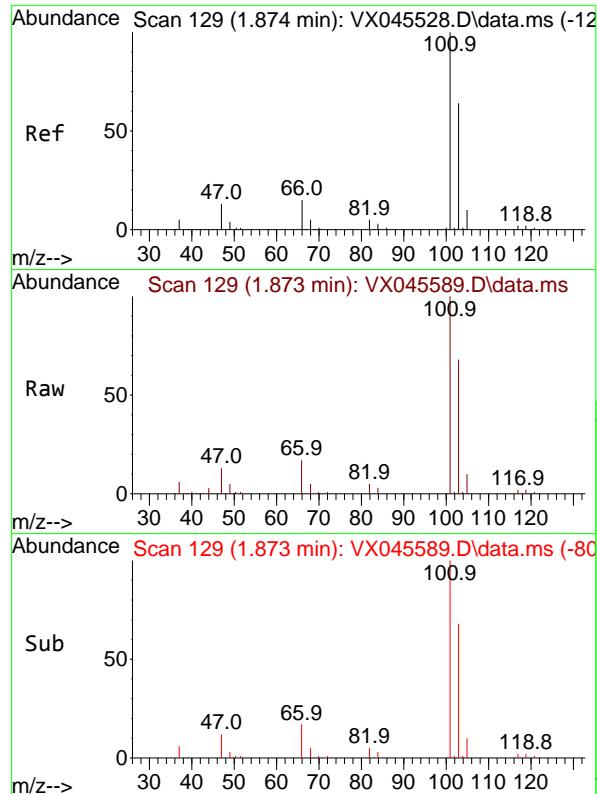


#7  
Trichlorofluoromethane  
Concen: 20.139 ug/l  
RT: 1.873 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01


### Manual Integrations APPROVED







Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

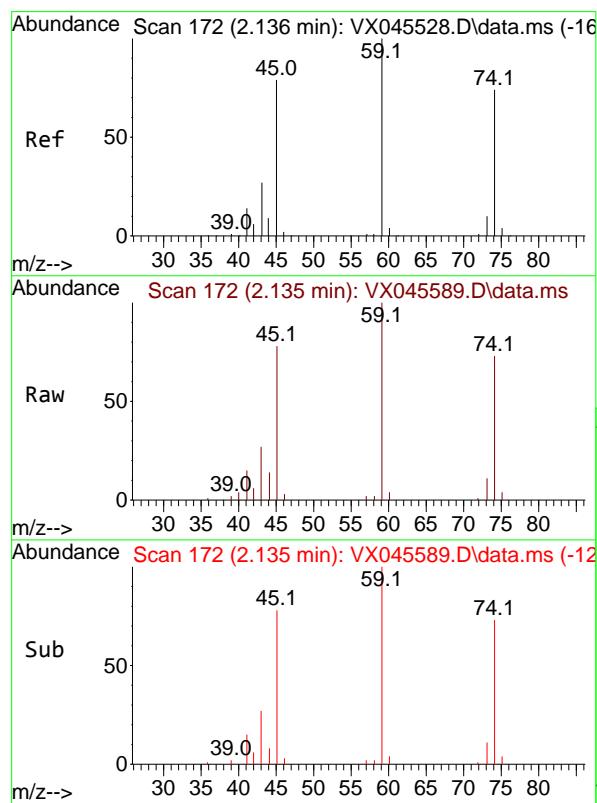

#8  
Diethyl Ether  
Concen: 19.796 ug/l  
RT: 2.135 min Scan# 172  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 74 Resp: 13256  
Ion Ratio Lower Upper  
74 100  
45 108.1 53.0 159.1

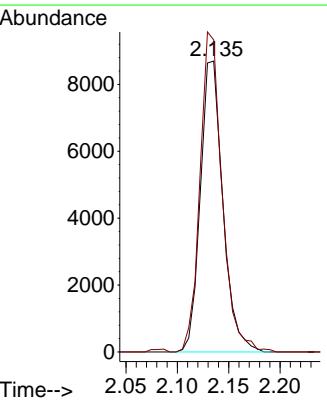

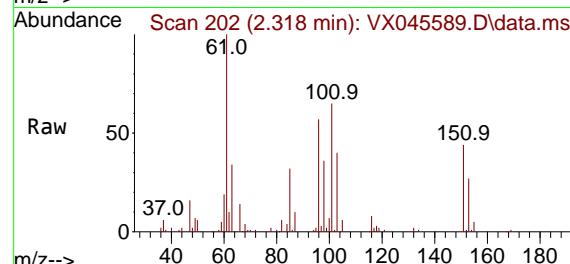

#9

1,1,2-Trichlorotrifluoroethane

Concen: 20.134 ug/l

RT: 2.318 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X


ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

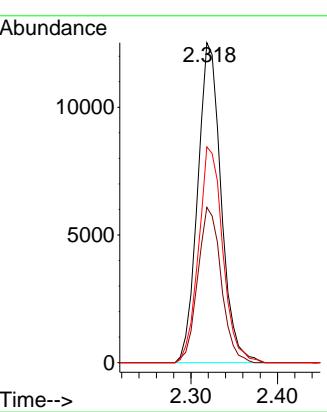

#10

Methyl Iodide

Concen: 18.845 ug/l


RT: 2.446 min Scan# 223


Delta R.T. -0.000 min

Lab File: VX045589.D





Acq: 04 Apr 2025 11:14

Tgt	Ion:142	Resp:	27472
Ion	Ratio	Lower	Upper
142	100		
127	53.0	40.2	60.4
141	14.4	11.7	17.5





Abundance Scan 309 (2.971 min): VX045589.D\data.ms

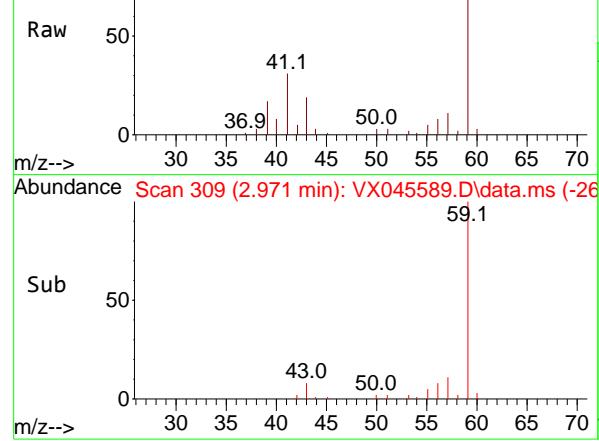

#11

Tert butyl alcohol

Concen: 96.466 ug/l

RT: 2.971 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X


ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#12

1,1-Dichloroethene

Concen: 19.364 ug/l

RT: 2.312 min Scan# 201

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion: 96 Resp: 22114


Ion Ratio Lower Upper

96 100

61 185.2 145.7 218.5

98 61.5 51.6 77.4

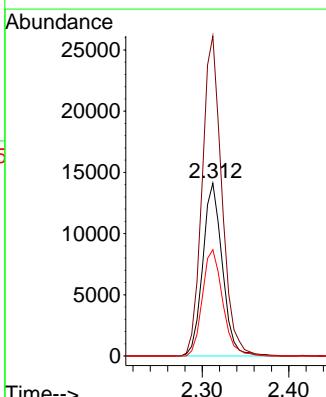

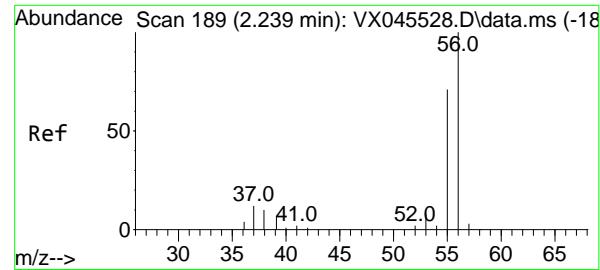

#13




Acrolein  
Concen: 109.636 ug/l  
RT: 2.233 min Scan# 189  
Delta R.T. -0.006 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01

Tgt Ion: 56 Resp: 35291  
Ion Ratio Lower Upper  
56 100  
55 73.5 56.2 84.2




Manual Integrations  
APPROVED




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

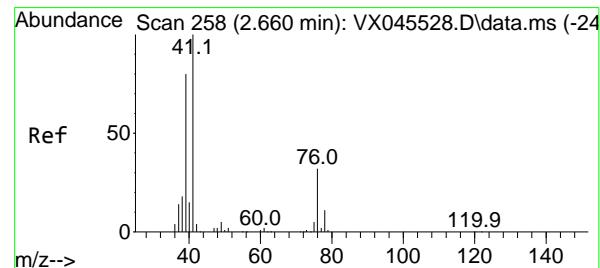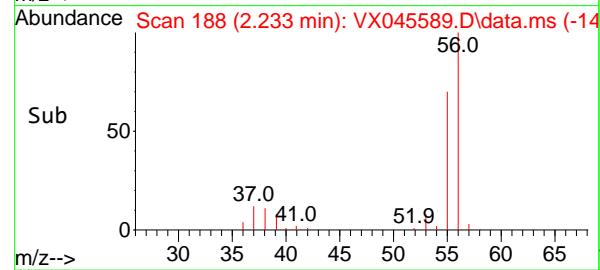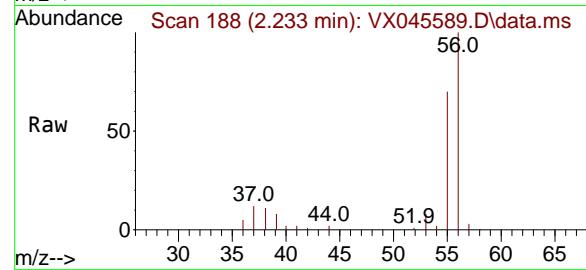

#14  
Allyl chloride  
Concen: 19.831 ug/l  
RT: 2.660 min Scan# 258  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 41 Resp: 42970  
Ion Ratio Lower Upper  
41 100  
39 74.3 60.2 90.2  
76 30.2 24.6 36.8

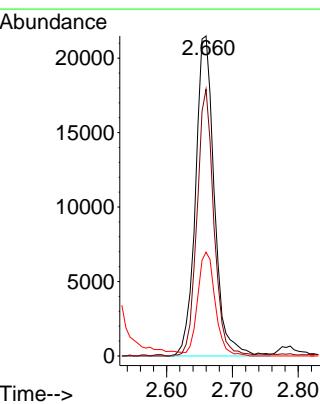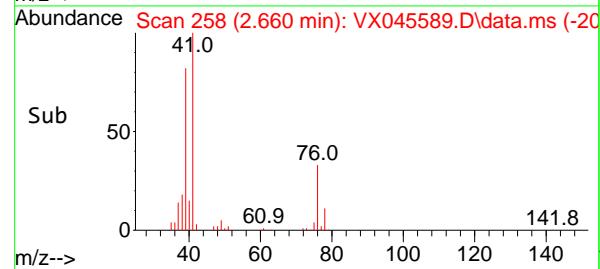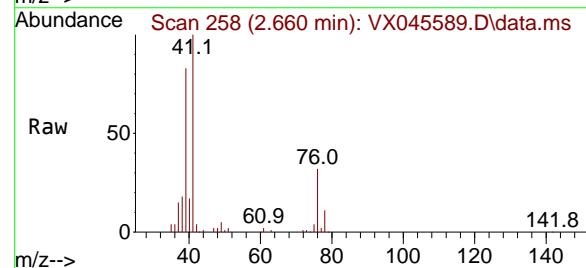

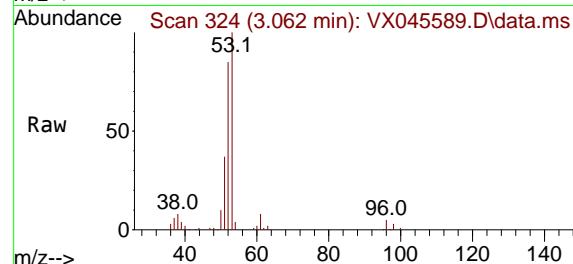

#15

Acrylonitrile

Concen: 100.048 ug/l

RT: 3.062 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X





ClientSampleId :

VX0404WBS01

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

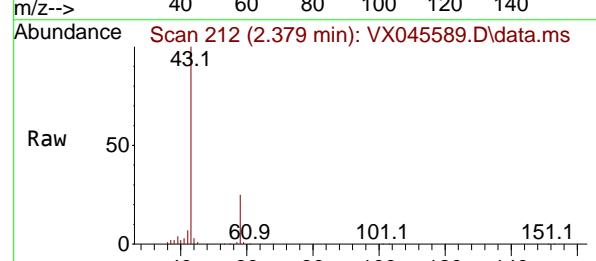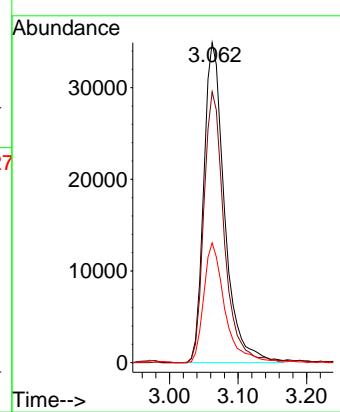

#16

Acetone

Concen: 100.574 ug/l

RT: 2.379 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14







Tgt Ion: 43 Resp: 71844

Ion Ratio Lower Upper

43 100

58 25.1 22.3 33.5

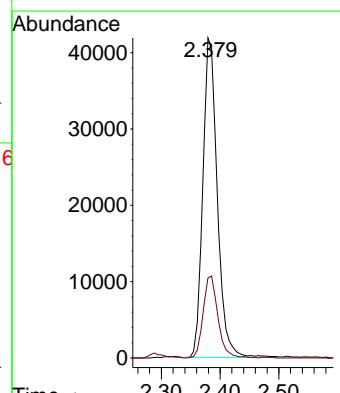



#17

Carbon Disulfide

Concen: 18.361 ug/l

RT: 2.507 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument :

MSVOA\_X


ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

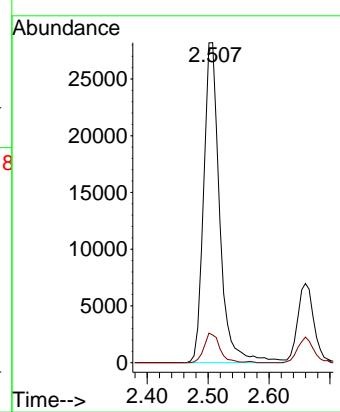

#18

Methyl Acetate

Concen: 20.160 ug/l

RT: 2.702 min Scan# 265

Delta R.T. -0.000 min


Lab File: VX045589.D







Acq: 04 Apr 2025 11:14

Tgt Ion: 43 Resp: 33157

Ion Ratio Lower Upper

43	100
74	21.4
	17.5
	26.3

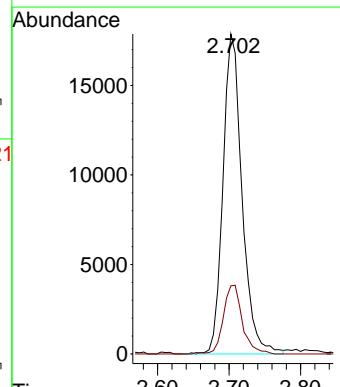




#19

Methyl tert-butyl Ether  
Concen: 19.397 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01

### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025




#20



Methylene Chloride  
Concen: 19.502 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 84 Resp: 26080  
Ion Ratio Lower Upper  
84 100  
49 136.8 107.5 161.3  
51 40.7 33.0 49.6  
86 64.6 50.1 75.1

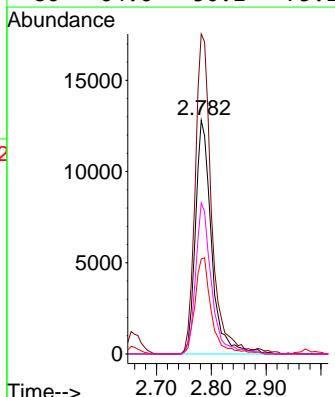




Abundance Scan 328 (3.086 min): VX045589.D\data.ms

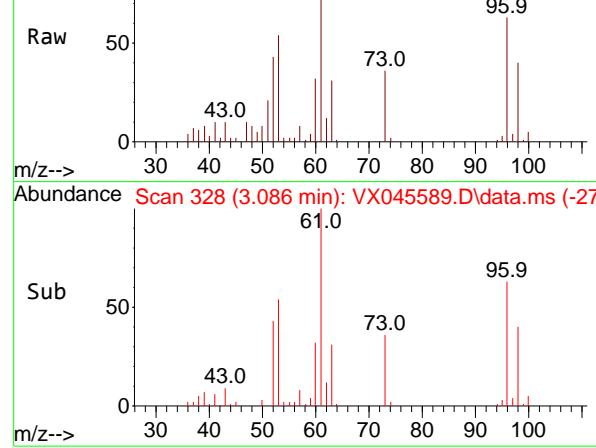


Abundance Scan 438 (3.757 min): VX045589.D\data.ms

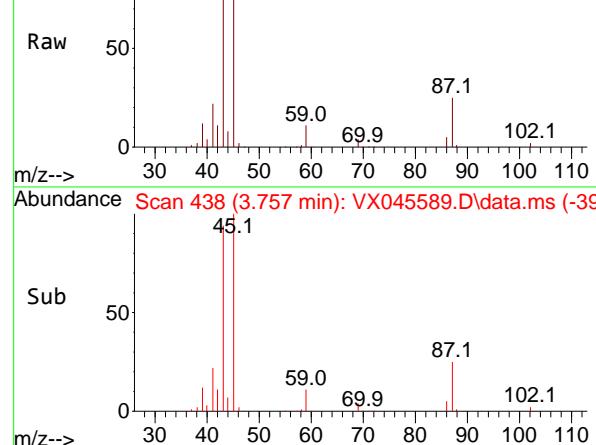

Abundance Scan 438 (3.757 min): VX045589.D\data.ms (-39)

Sub

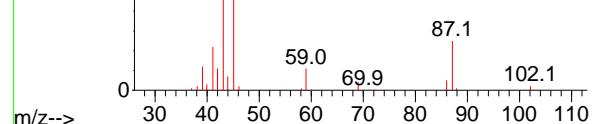

#21

trans-1,2-Dichloroethene

Concen: 19.646 ug/l

RT: 3.086 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X


ClientSampleId :

VX0404WBS01

### Manual Integrations APPROVED

Reviewed By :John Carbone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#22

Diisopropyl ether

Concen: 19.265 ug/l

RT: 3.757 min Scan# 438

Delta R.T. -0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Tgt Ion: 45 Resp: 82229


Ion Ratio Lower Upper


45 100

43 92.3 59.3 88.9#


87 24.6 20.4 30.6

59 11.1 9.0 13.6







Abundance Scan 432 (3.721 min): VX045589.D\data.ms

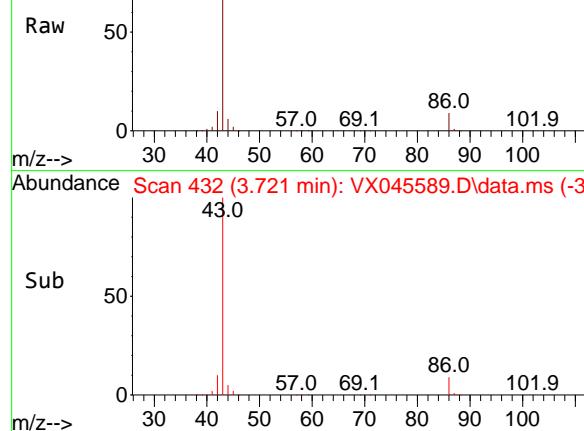

Abundance Scan 432 (3.721 min): VX045589.D\data.ms (-38)

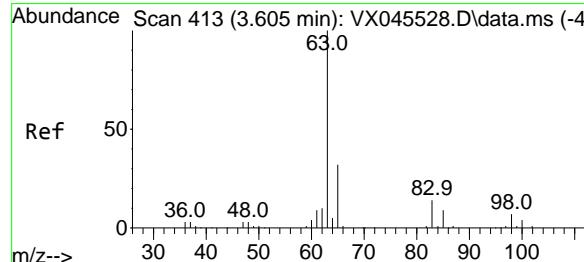

Abundance Scan 413 (3.605 min): VX045589.D\data.ms

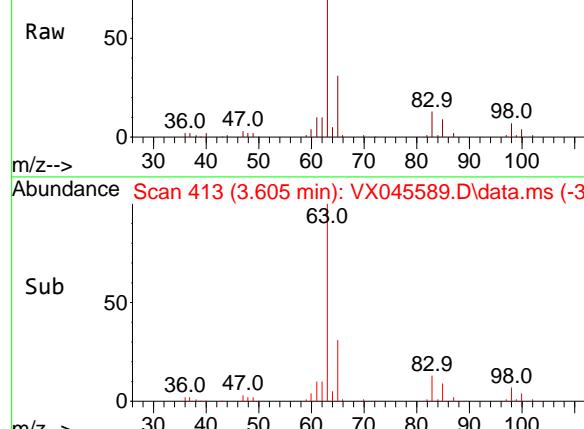

Abundance Scan 413 (3.605 min): VX045589.D\data.ms (-36)

#23

**Vinyl Acetate**

Concen: 98.665 ug/l

RT: 3.721 min Scan# 4

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X



ClientSampleId :

VX0404WBS01


**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



Abundance Scan 413 (3.605 min): VX045589.D\data.ms

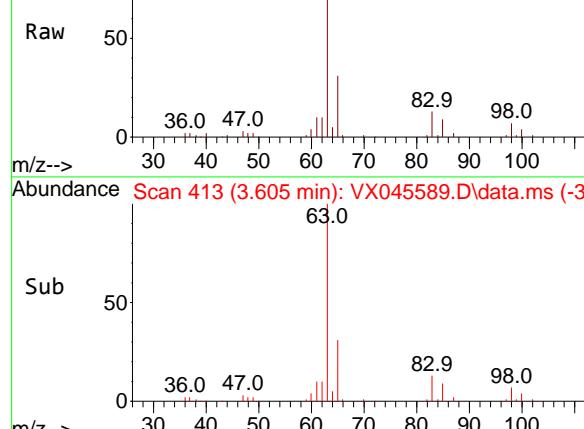

Abundance Scan 413 (3.605 min): VX045589.D\data.ms (-36)

#24

**1,1-Dichloroethane**

Concen: 19.451 ug/l

RT: 3.605 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion: 63 Resp: 46953


Ion Ratio Lower Upper

63 100



98 7.2 3.4 10.1

100 4.3 2.2 6.6

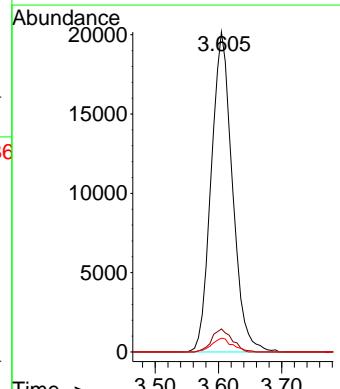


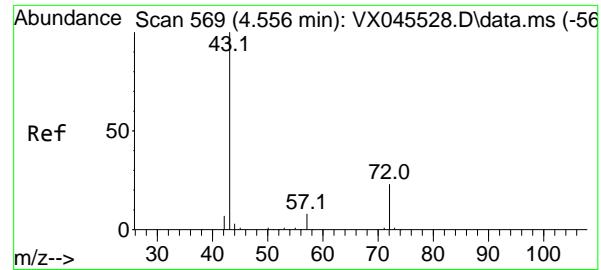

Abundance Scan 569 (4.556 min): VX045589.D\data.ms

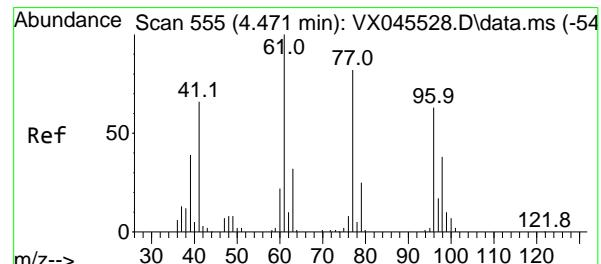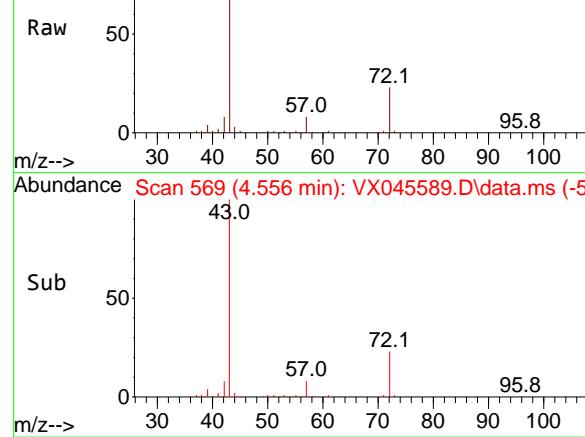

Abundance Scan 554 (4.464 min): VX045589.D\data.ms

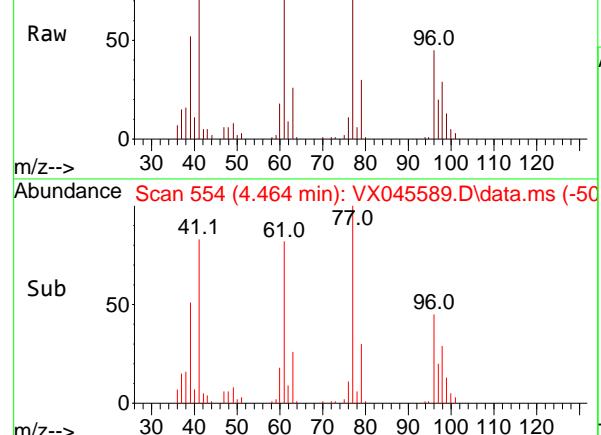

#25

2-Butanone

Concen: 101.462 ug/l

RT: 4.556 min Scan# 5

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X


ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

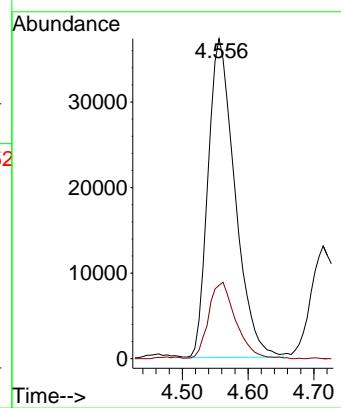

#26

2,2-Dichloropropane

Concen: 21.073 ug/l

RT: 4.464 min Scan# 554

Delta R.T. -0.006 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14




Tgt Ion: 77 Resp: 32865

Ion Ratio Lower Upper

77 100

97 21.8 10.6 31.8

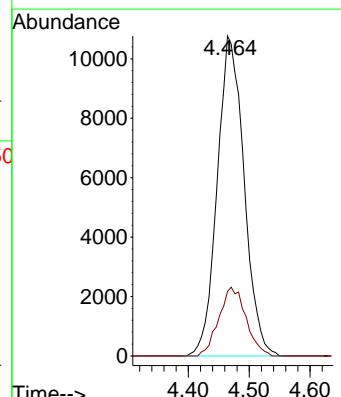






#27  
cis-1,2-Dichloroethene  
Concen: 19.156 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01



### Manual Integrations APPROVED




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025



#28  
Bromochloromethane  
Concen: 20.399 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 49 Resp: 23795  
Ion Ratio Lower Upper  
49 100  
129 0.8 0.0 3.8  
130 65.5 54.6 81.8

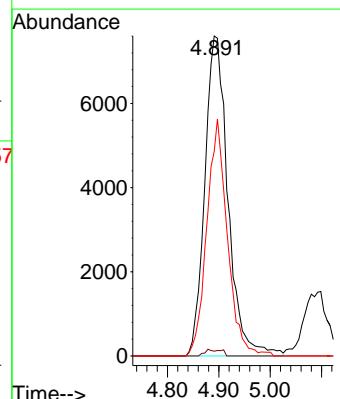



#29

Tetrahydrofuran

Concen: 97.791 ug/l

RT: 5.007 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X





ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

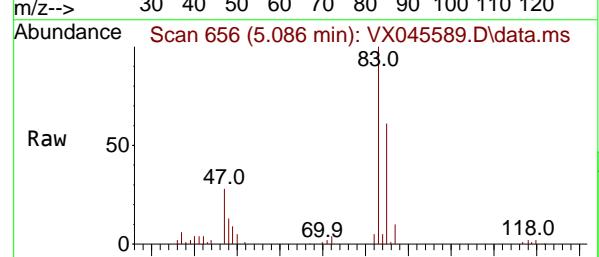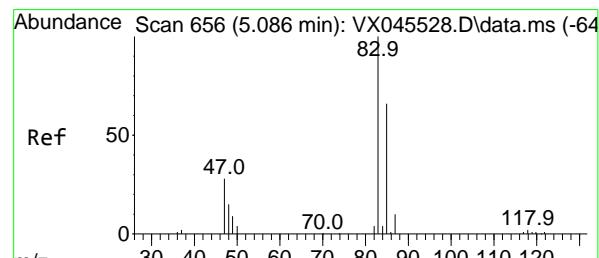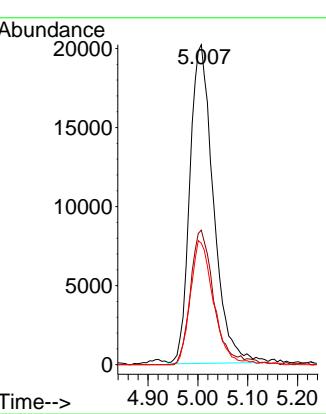

#30

Chloroform

Concen: 19.797 ug/l


RT: 5.086 min Scan# 656


Delta R.T. -0.000 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14

Tgt	Ion:	Resp:	
	83	49173	
	100		
	83		
	85	52.8	79.2

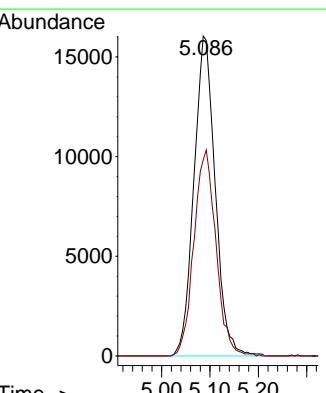



Abundance Scan 718 (5.464 min): VX045589.D\data.ms

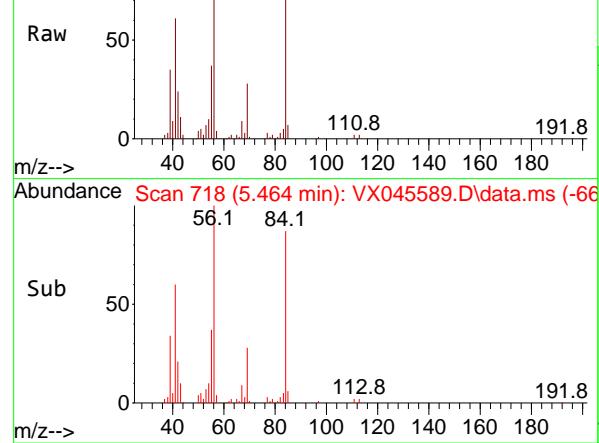

Abundance Scan 718 (5.464 min): VX045589.D\data.ms (-66)

#31

Cyclohexane

Concen: 19.493 ug/l

RT: 5.464 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X

ClientSampleId :

VX0404WBS01

Tgt Ion: 56 Resp: 41593

Ion Ratio Lower Upper

56 100

69 28.2 23.6 35.4



84 84.4 67.7 101.5

Manual Integrations



APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

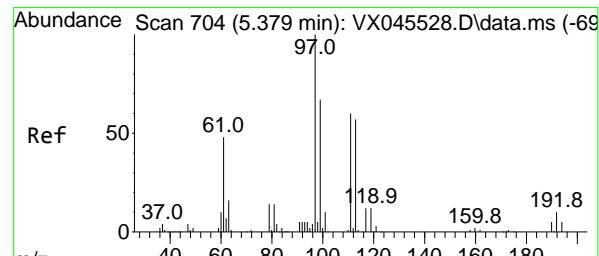

Abundance Scan 704 (5.379 min): VX045589.D\data.ms

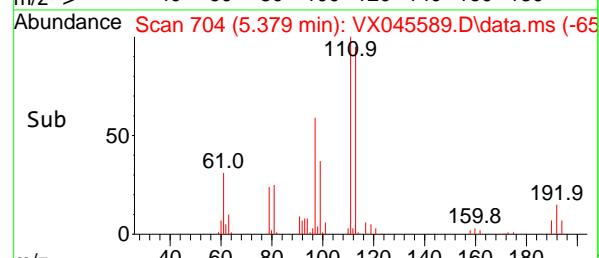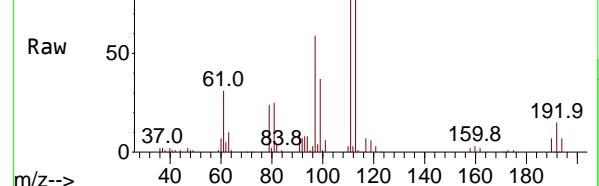

#32

1,1,1-Trichloroethane

Concen: 19.747 ug/l

RT: 5.379 min Scan# 704

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion: 97 Resp: 41502


Ion Ratio Lower Upper

97 100

99 63.4 51.7 77.5

61 52.7 41.0 61.4

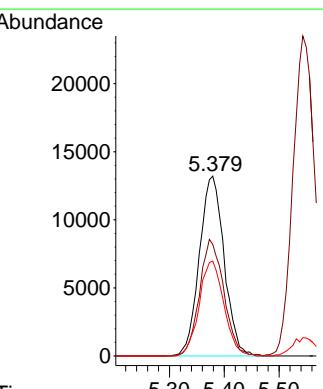

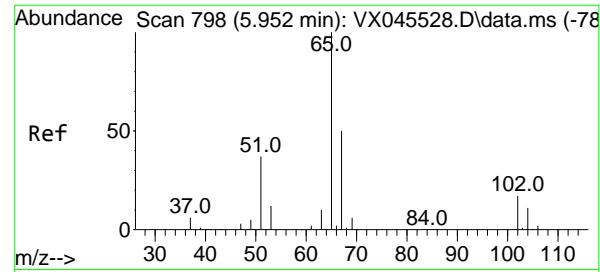


#33  
1,2-Dichloroethane-d4  
Concen: 52.873 ug/l  
RT: 5.952 min Scan# 7  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0404WBS01


Tgt Ion: 65 Resp: 91980  
Ion Ratio Lower Upper  
65 100  
67 49.8 0.0 99.0

### Manual Integrations APPROVED

Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025




Time--> 5.90 6.00 6.10

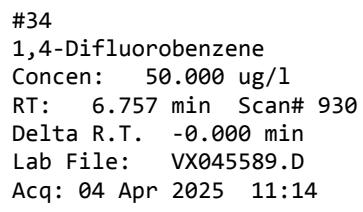


#34







1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 930  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion:114 Resp: 168453  
Ion Ratio Lower Upper  
114 100  
63 23.2 0.0 46.8  
88 16.5 0.0 35.4



Time--> 6.60 6.70 6.80 6.90

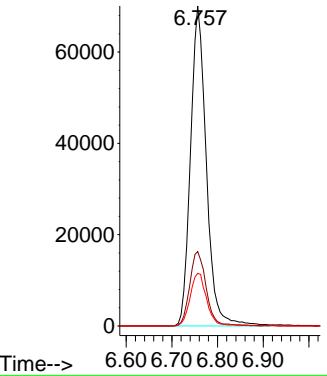

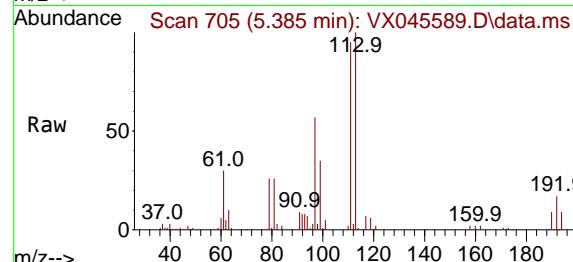

#35

Dibromofluoromethane

Concen: 53.280 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument :

MSVOA\_X


ClientSampleId :

VX0404WBS01

### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025




Supervised By :Mahesh Dadoda 04/07/2025

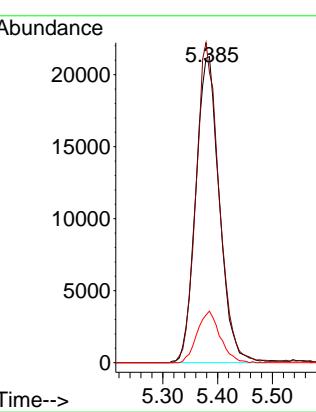

#36  
1,1-Dichloropropene  
Concen: 19.807 ug/l  
RT: 5.684 min Scan# 754  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 75 Resp: 31963  
Ion Ratio Lower Upper  
75 100  
110 32.8 16.9 50.6  
77 29.7 25.0 37.4

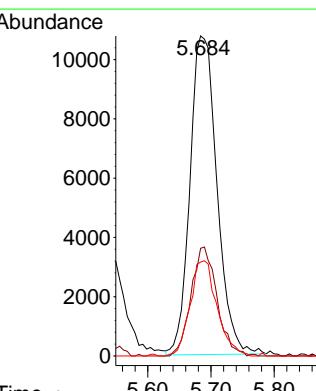

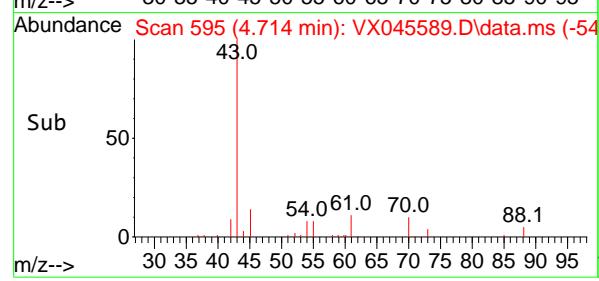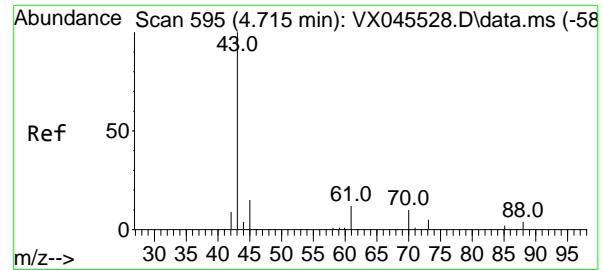

#37

**Ethyl Acetate**

Concen: 18.957 ug/l

RT: 4.714 min Scan# 5

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X




ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#38

**Carbon Tetrachloride**

Concen: 20.204 ug/l

RT: 5.671 min Scan# 752

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion:117 Resp: 35237




Ion Ratio Lower Upper

117 100

119 90.6 76.9 115.3

121 32.2 24.2 36.2

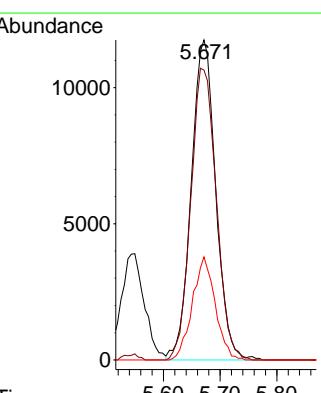

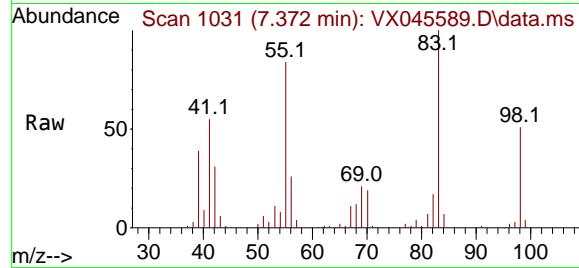

#39

Methylcyclohexane

Concen: 19.990 ug/l

RT: 7.372 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14





Instrument : MSVOA\_X

ClientSampleId : VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#40

Benzene

Concen: 19.865 ug/l


RT: 6.031 min Scan# 811




Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Tgt	Ion	Resp:	97905
Ion	Ratio	Lower	Upper
78	100		
77	24.0	19.0	28.6



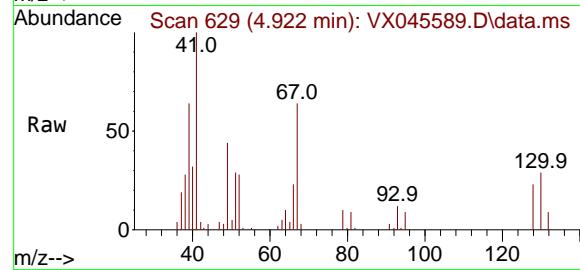

#41

Methacrylonitrile

Concen: 20.585 ug/l

RT: 4.922 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X





ClientSampleId : VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

Abundance

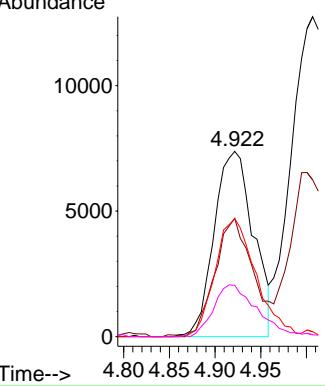

#42

1,2-Dichloroethane

Concen: 20.364 ug/l

RT: 6.086 min Scan# 820

Delta R.T. 0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion: 62 Resp: 41452


Ion Ratio Lower Upper

62 100


98 7.5 0.0 15.2

Abundance

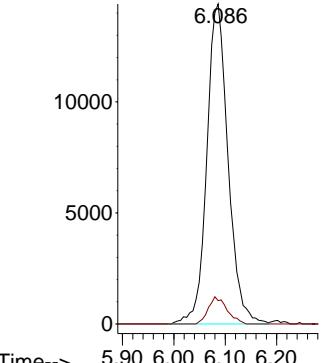




Abundance Scan 862 (6.342 min): VX045589.D\data.ms

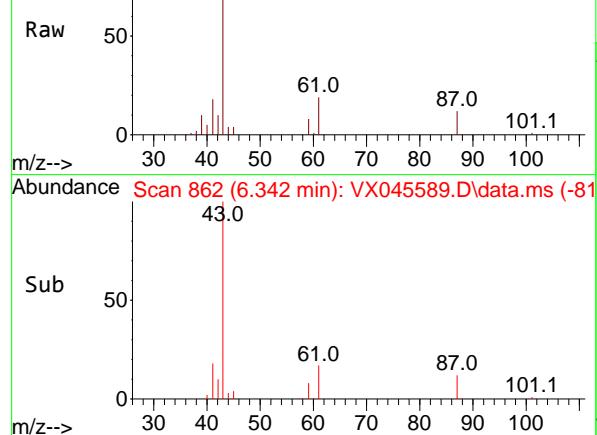

Abundance Scan 862 (6.342 min): VX045589.D\data.ms (-81)

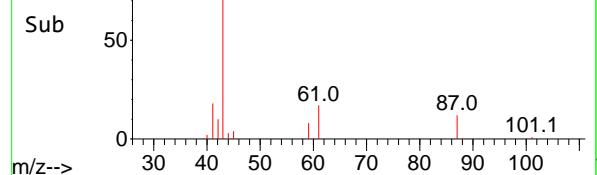

#43

Isopropyl Acetate

Concen: 19.244 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X

ClientSampleId :

VX0404WBS01

Tgt Ion: 43 Resp: 5931

Ion Ratio Lower Upper

43 100

61 18.1 14.1 21.1




87 11.3 9.2 13.8

Manual Integrations


APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

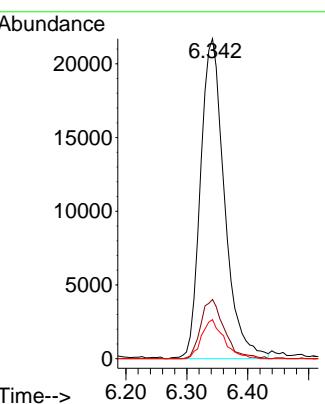

Abundance Scan 990 (7.122 min): VX045589.D\data.ms (-94)

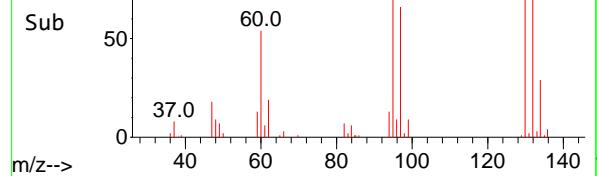

#44

Trichloroethene

Concen: 19.237 ug/l

RT: 7.122 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14




Tgt Ion: 130 Resp: 22535

Ion Ratio Lower Upper

130 100

95 111.8 0.0 202.0

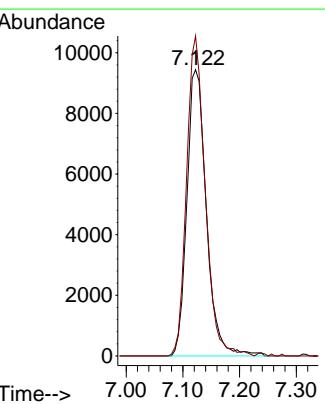



#45

1,2-Dichloropropane

Concen: 19.804 ug/l

RT: 7.427 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14





Instrument : MSVOA\_X

ClientSampleId : VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

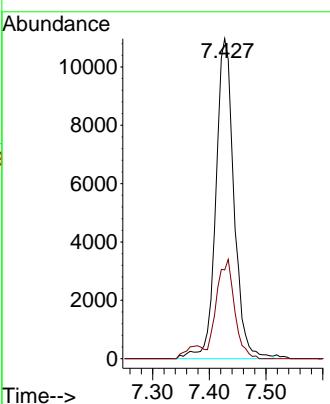

#46

Dibromomethane

Concen: 20.328 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion: 93 Resp: 19189







Ion Ratio Lower Upper

93 100


95 80.6 64.8 97.2

174 84.3 65.4 98.0

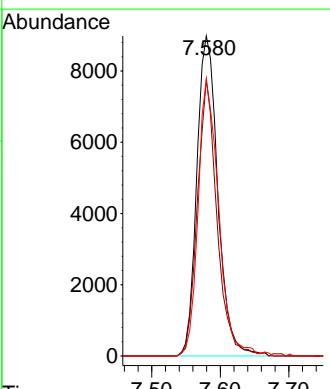










#47

Bromodichloromethane  
Concen: 19.932 ug/lRT: 7.817 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01**Manual Integrations  
APPROVED**Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

#48  
Methyl methacrylate  
Concen: 20.104 ug/l  
RT: 7.689 min Scan# 1083  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 41 Resp: 31993  
Ion Ratio Lower Upper  
41 100  
69 71.6 58.2 87.2  
39 65.8 53.6 80.4





#49

1,4-Dioxane

Concen: 414.998 ug/l

RT: 7.659 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X


ClientSampleId :

VX0404WBS01

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

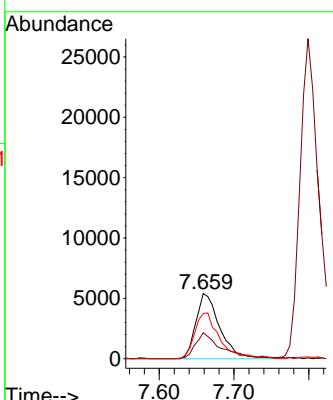

#50

Toluene-d8

Concen: 53.195 ug/l

RT: 8.646 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14


Tgt Ion: 98 Resp: 221910

Ion Ratio Lower Upper





98 100

100 63.8 52.2 78.4



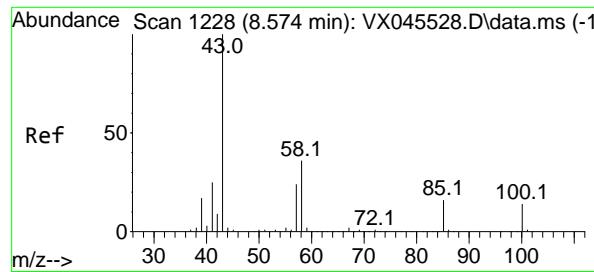

Abundance Scan 1228 (8.573 min): VX045589.D\data.ms

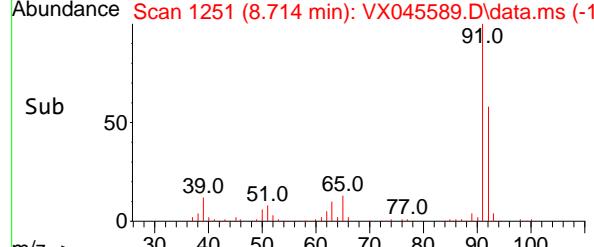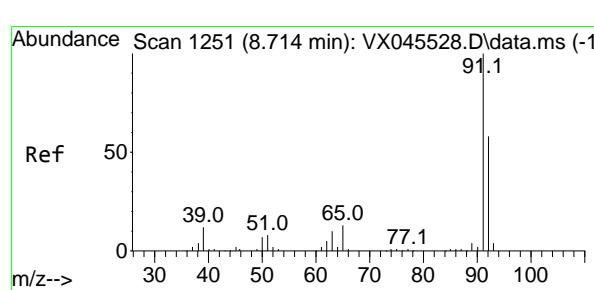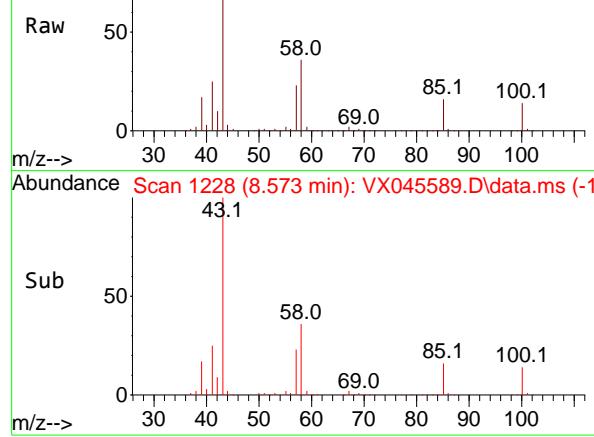

Abundance Scan 1251 (8.714 min): VX045589.D\data.ms (-1)

Sub

m/z--&gt;

#51

4-Methyl-2-Pentanone

Concen: 102.524 ug/l

RT: 8.573 min Scan# 1228

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X




ClientSampleId :

VX0404WBS01

**Manual Integrations**  
**APPROVED**


Reviewed By :John Carbone 04/07/2025




Supervised By :Mahesh Dadoda 04/07/2025

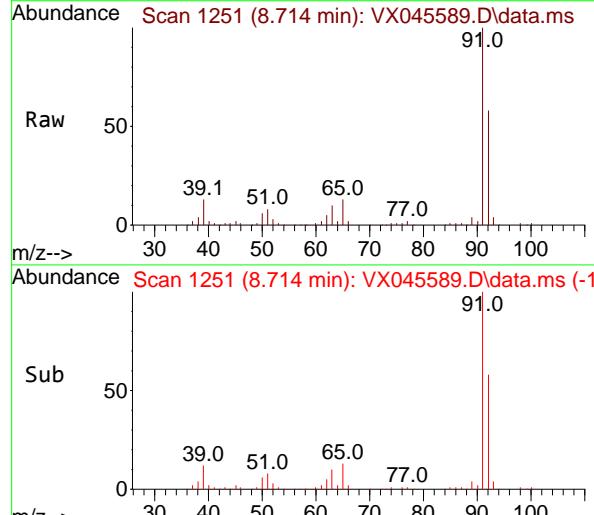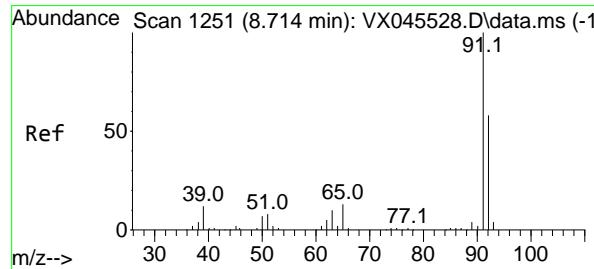

#52  
Toluene  
Concen: 19.623 ug/l  
RT: 8.714 min Scan# 1251  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 92 Resp: 58522  
Ion Ratio Lower Upper  
92 100  
91 176.2 138.7 208.1



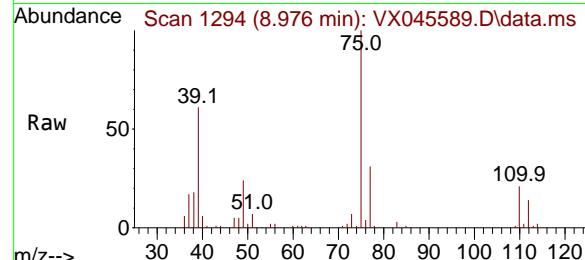

#53

t-1,3-Dichloropropene

Concen: 18.474 ug/l

RT: 8.976 min Scan# 1194

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X





ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

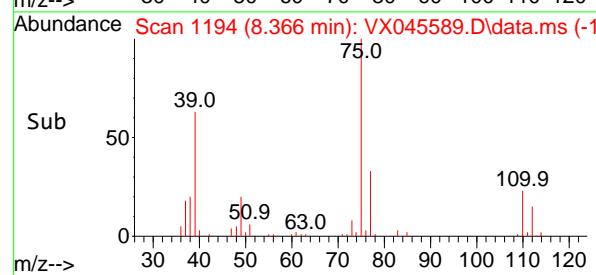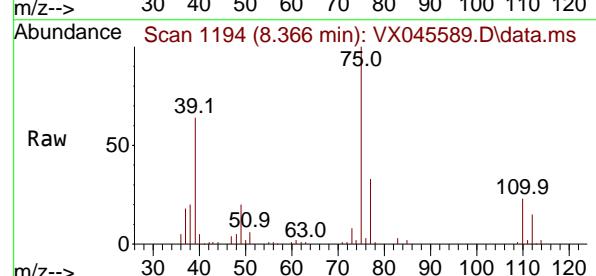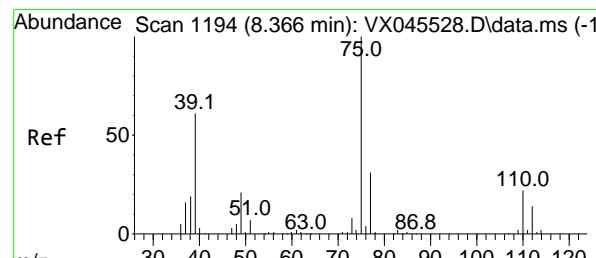

#54

cis-1,3-Dichloropropene

Concen: 19.846 ug/l

RT: 8.366 min Scan# 1194

Delta R.T. 0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion: 75 Resp: 35158







Ion Ratio Lower Upper

75 100

77 32.9 24.6 36.8

39 63.6 48.4 72.6



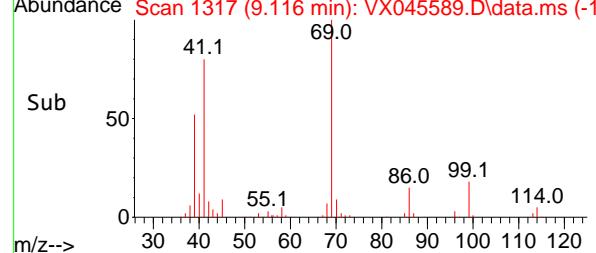

#55

1,1,2-Trichloroethane

Concen: 20.482 ug/l

RT: 9.152 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X


ClientSampleId :

VX0404WBS01

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

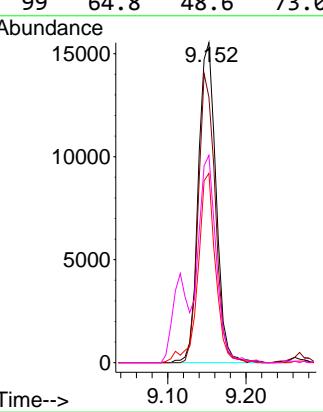

#56

Ethyl methacrylate

Concen: 19.931 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion: 69 Resp: 36657




Ion Ratio Lower Upper

69 100

41 78.8 61.3 91.9

39 50.6 40.2 60.2

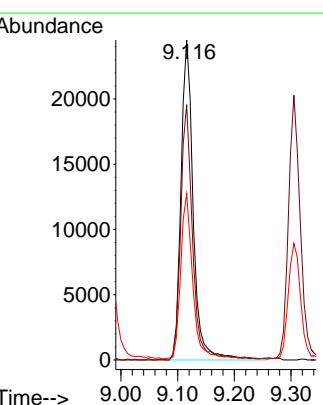



#57

1,3-Dichloropropane

Concen: 20.400 ug/l

RT: 9.305 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X





ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#58

2-Chloroethyl Vinyl ether

Concen: 102.664 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. -0.000 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14


Tgt Ion: 63 Resp: 95516

Ion Ratio Lower Upper


63 100

106 25.9 21.0 31.6

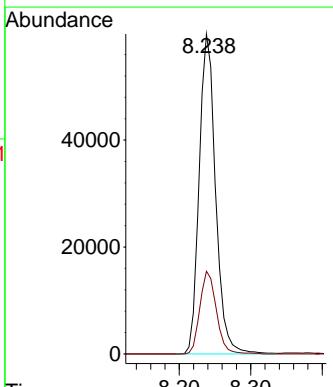





Abundance Scan 1368 (9.427 min): VX045589.D\data.ms

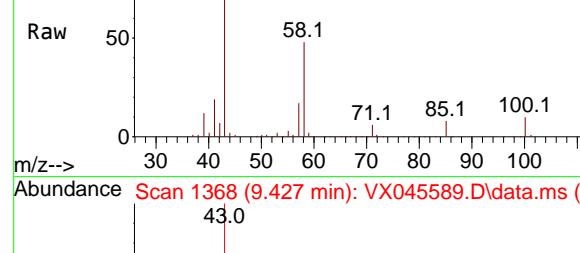


Abundance Scan 1368 (9.427 min): VX045589.D\data.ms (-1)

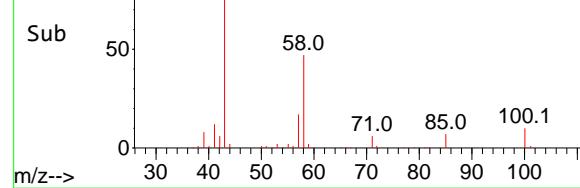


Abundance Scan 1383 (9.519 min): VX045528.D\data.ms (-1)

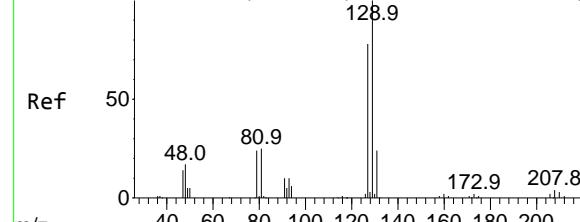

Abundance Scan 1383 (9.518 min): VX045589.D\data.ms

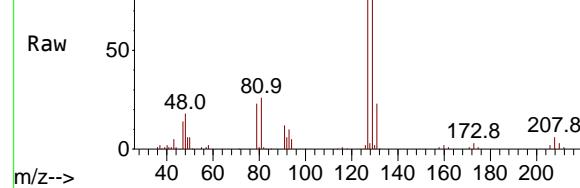

Abundance Scan 1383 (9.518 min): VX045589.D\data.ms (-1)

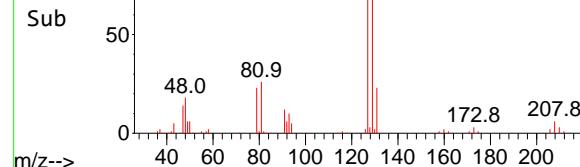

#59

2-Hexanone

Concen: 101.036 ug/l

RT: 9.427 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X

ClientSampleId :

VX0404WBS01

Tgt Ion: 43 Resp: 15287

Ion Ratio Lower Upper

43 100


58 48.7 24.9 74.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

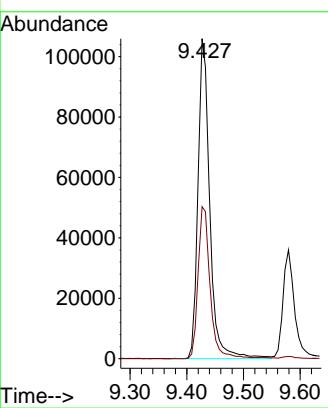

#60

Dibromochloromethane

Concen: 19.946 ug/l

RT: 9.518 min Scan# 1383

Delta R.T. -0.000 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14




Tgt Ion:129 Resp: 25841

Ion Ratio Lower Upper

129 100

127 79.5 39.4 118.2

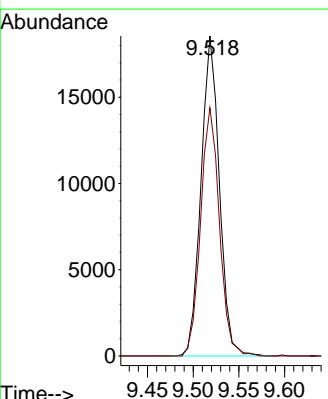



#61

1,2-Dibromoethane

Concen: 19.930 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X





ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

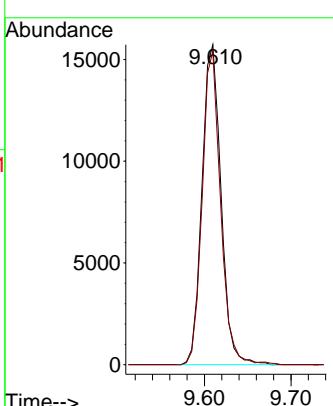

#62

4-Bromofluorobenzene

Concen: 53.227 ug/l


RT: 11.079 min Scan# 1639


Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Tgt	Ion:	95	Resp:	80880
Ion	Ratio	Lower	Upper	
95	100			
174	68.0	0.0	135.8	
176	65.0	0.0	131.4	

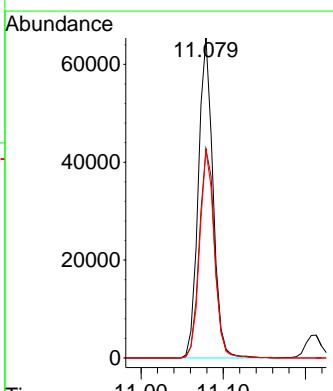


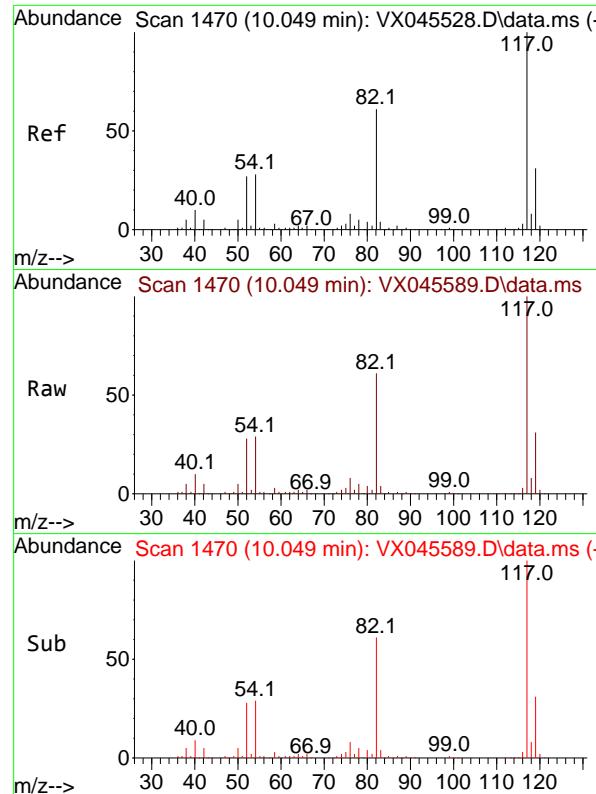


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01


### Manual Integrations APPROVED


Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

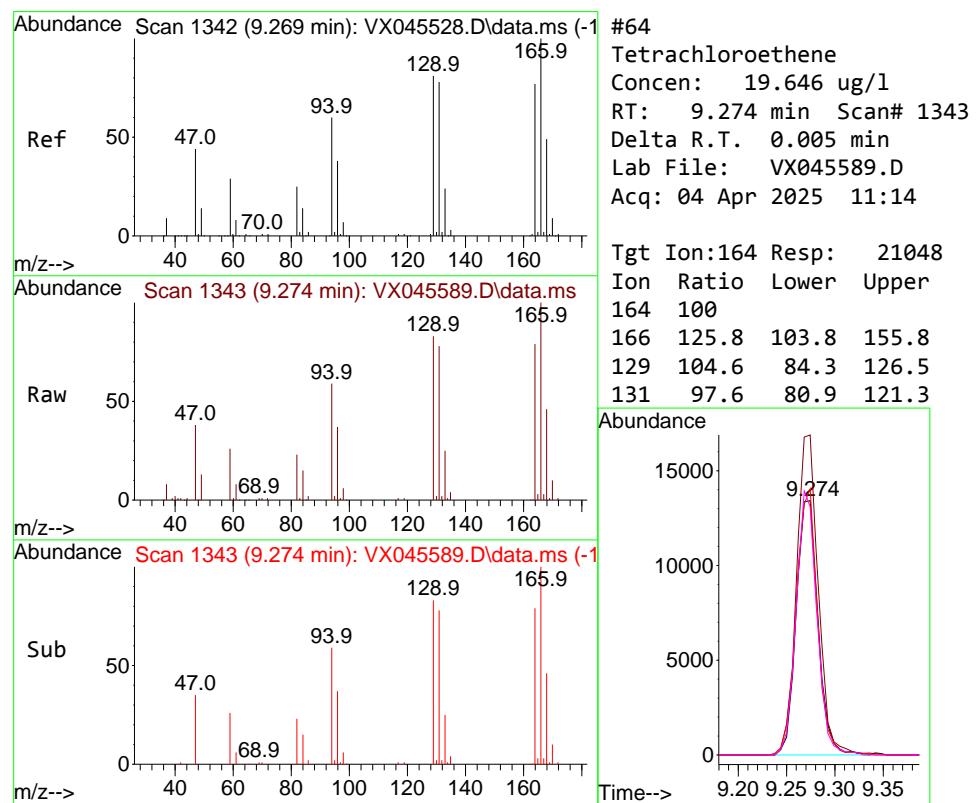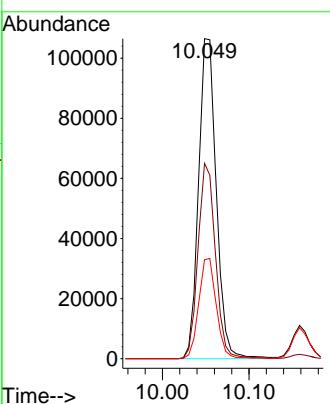

#64  
Tetrachloroethene  
Concen: 19.646 ug/l  
RT: 9.274 min Scan# 1343  
Delta R.T. 0.005 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion:164 Resp: 21048  
Ion Ratio Lower Upper  
164 100  
166 125.8 103.8 155.8  
129 104.6 84.3 126.5  
131 97.6 80.9 121.3

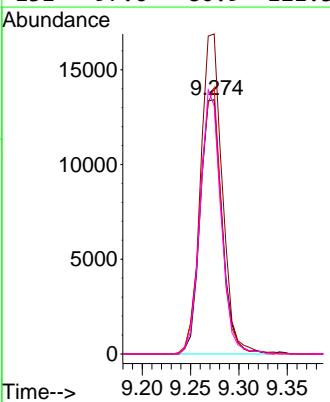


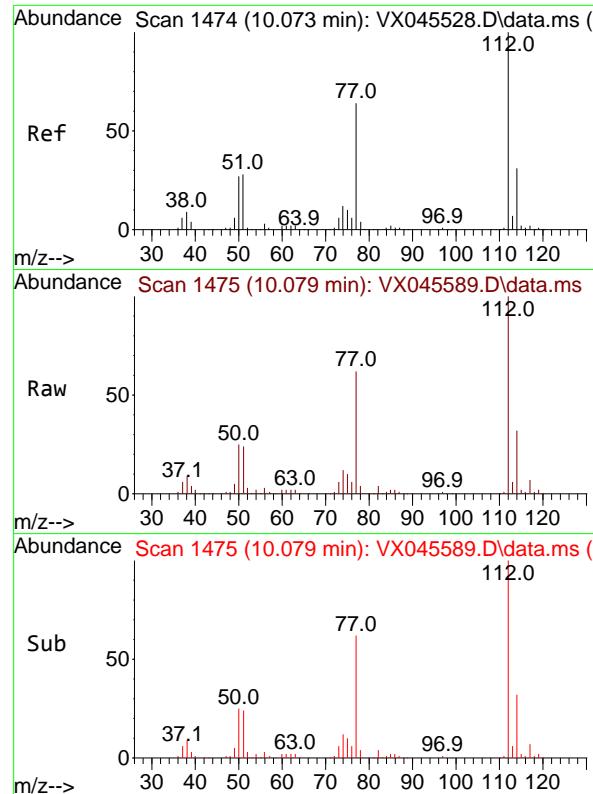


#65  
Chlorobenzene  
Concen: 19.598 ug/l  
RT: 10.079 min Scan# 1475  
Delta R.T. 0.006 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

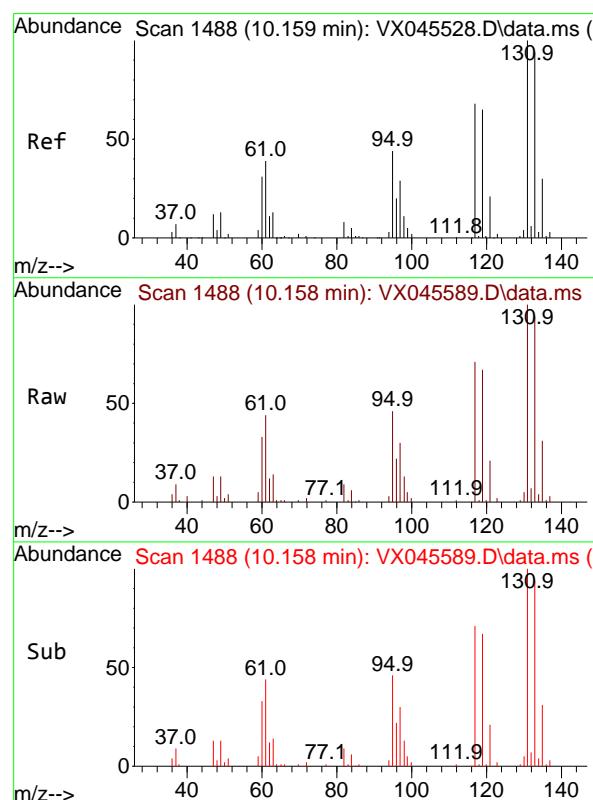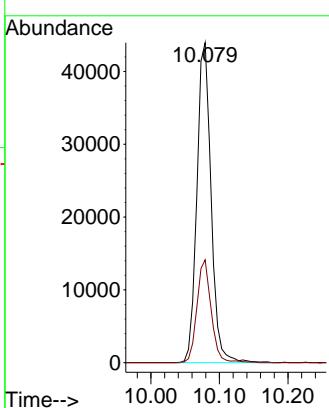

#66  
1,1,1,2-Tetrachloroethane  
Concen: 19.676 ug/l  
RT: 10.158 min Scan# 1488  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion:131 Resp: 22150  
Ion Ratio Lower Upper  
131 100  
133 92.3 47.5 142.5  
119 62.5 32.9 98.6

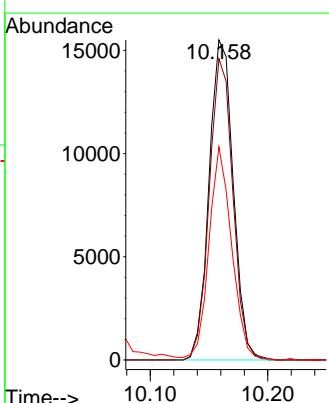

#67

Ethyl Benzene

Concen: 19.613 ug/l

RT: 10.189 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D




Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X

ClientSampleId :





VX0404WBS01

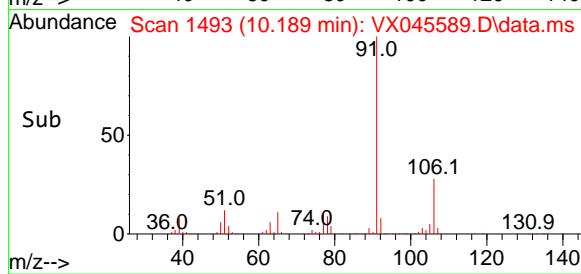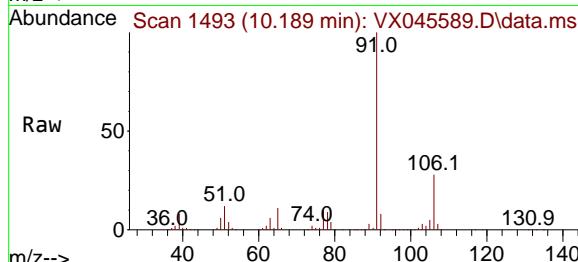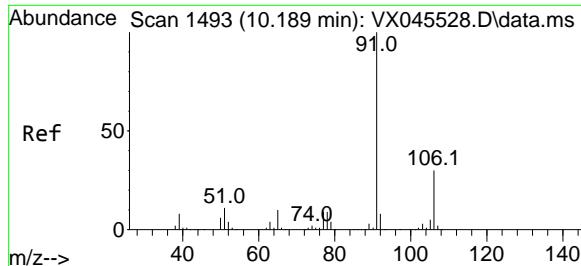

Tgt Ion: 91 Resp: 113901  
 Ion Ratio Lower Upper  
 91 100  
 106 28.4 23.7 35.5


### Manual Integrations APPROVED


Reviewed By :John Carbone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

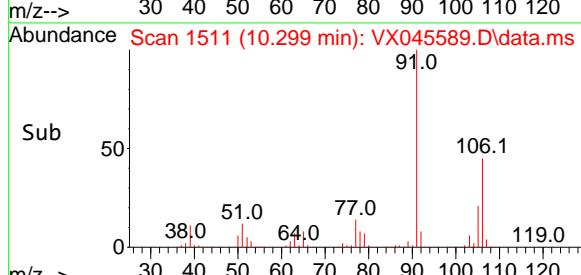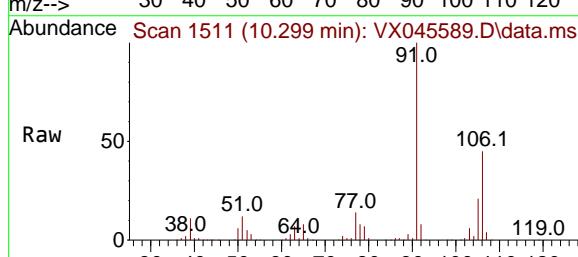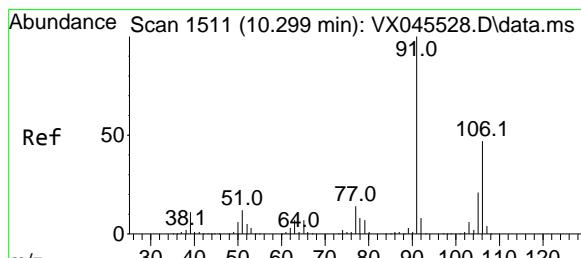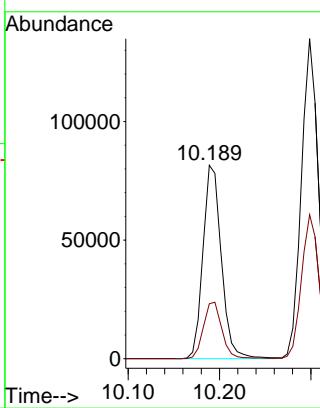

#68  
 m/p-Xylenes  
 Concen: 39.245 ug/l  
 RT: 10.299 min Scan# 1511  
 Delta R.T. -0.000 min  
 Lab File: VX045589.D  
 Acq: 04 Apr 2025 11:14

Tgt Ion:106 Resp: 82893  
 Ion Ratio Lower Upper  
 106 100  
 91 218.1 172.6 258.8

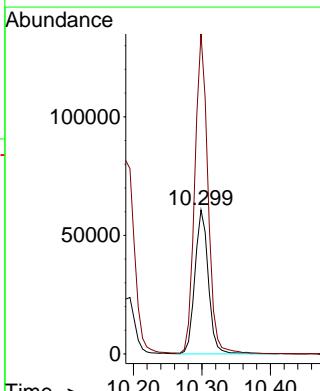


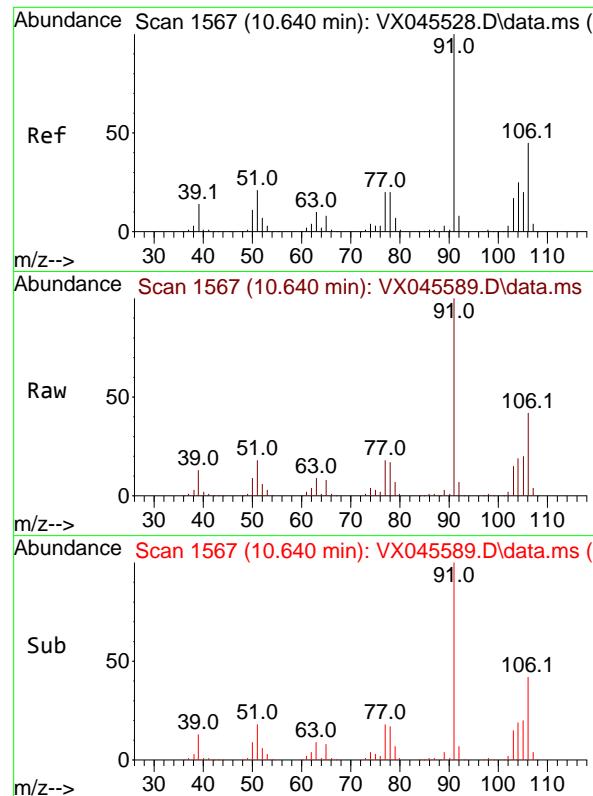


#69  
o-Xylene  
Concen: 19.908 ug/l  
RT: 10.640 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

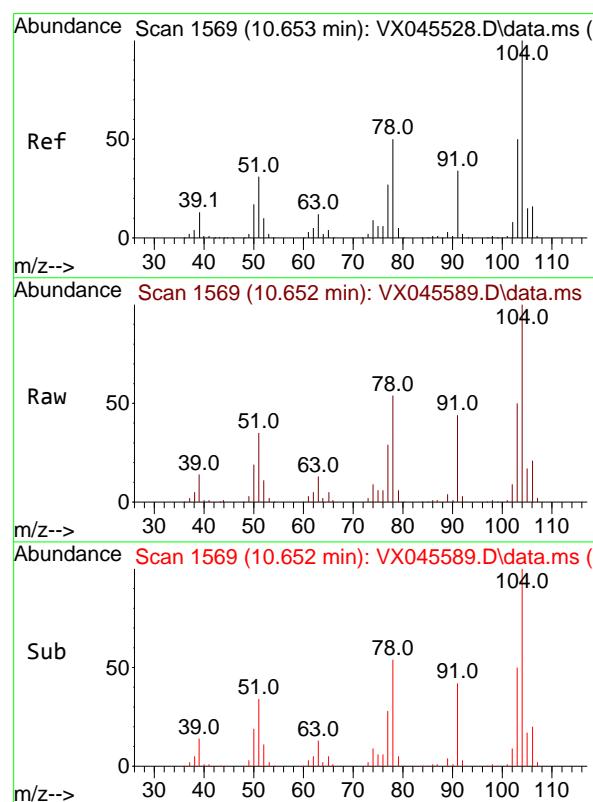

#70  
Styrene  
Concen: 19.846 ug/l  
RT: 10.652 min Scan# 1569  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion:104 Resp: 68156  
Ion Ratio Lower Upper  
104 100  
78 58.8 45.4 68.2  
103 55.7 43.8 65.8

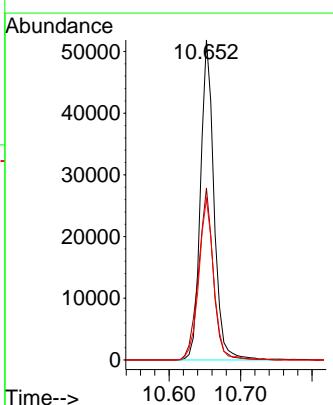



#71

Bromoform

Concen: 18.768 ug/l

RT: 10.799 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X





ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

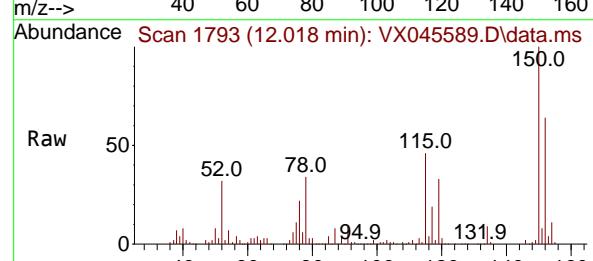

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l


RT: 12.018 min Scan# 1793


Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Tgt	Ion:152	Resp:	66584
Ion	Ratio	Lower	Upper
152	100		
115	77.8	46.9	140.7
150	162.7	0.0	349.4

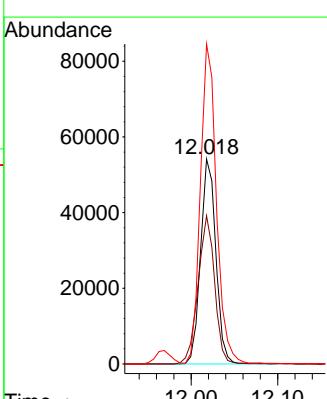


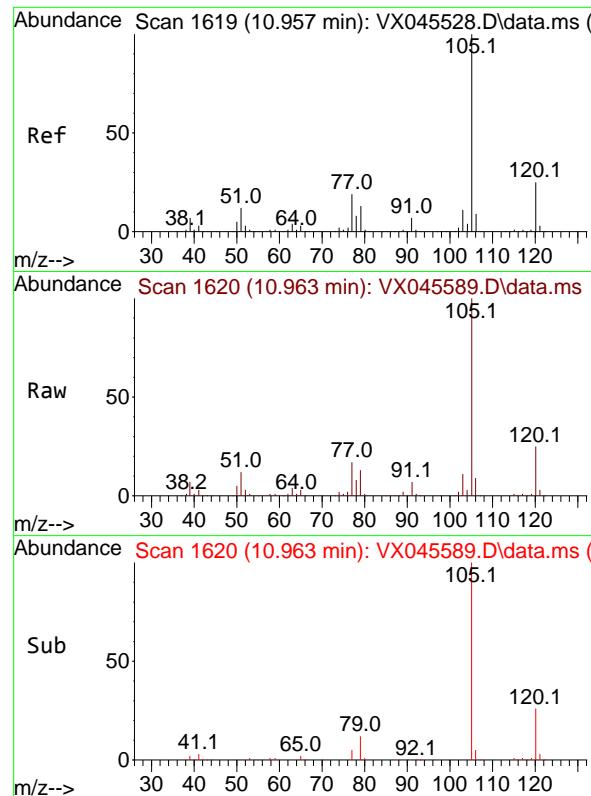


#73  
Isopropylbenzene  
Concen: 20.461 ug/l  
RT: 10.963 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14




Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01

Manual Integrations  
**APPROVED**

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

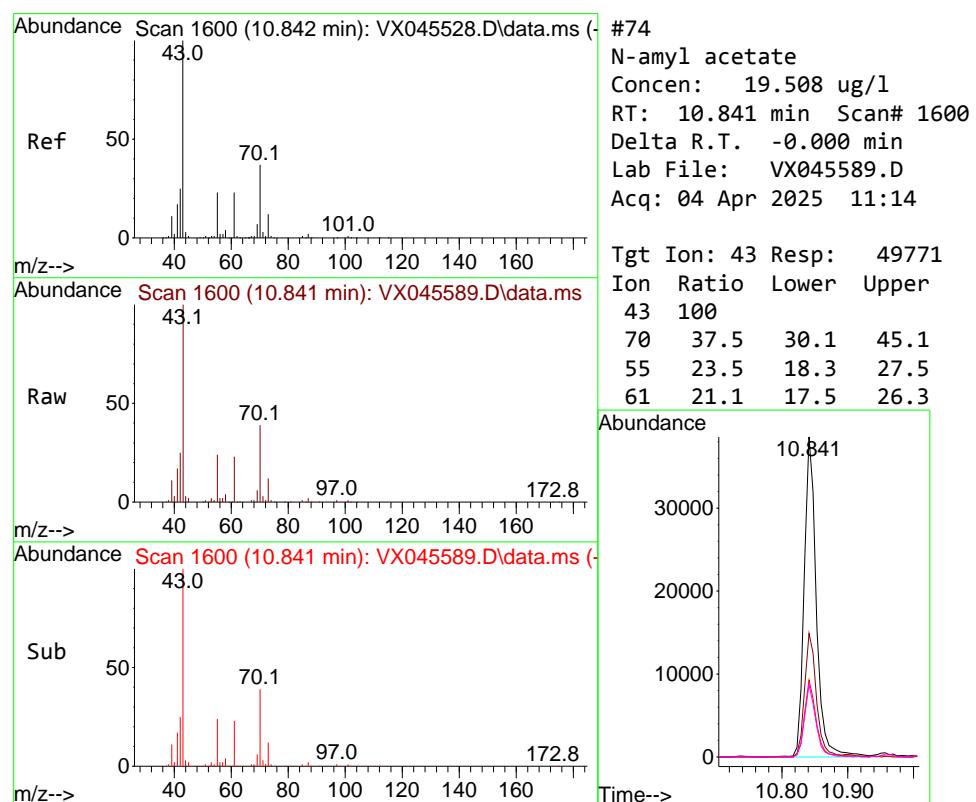

#74  
N-amyl acetate  
Concen: 19.508 ug/l  
RT: 10.841 min Scan# 1600  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

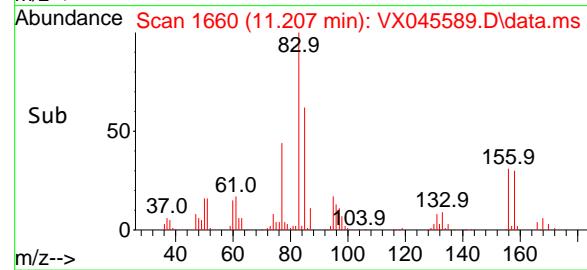
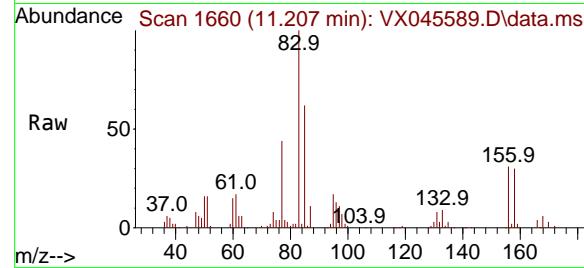
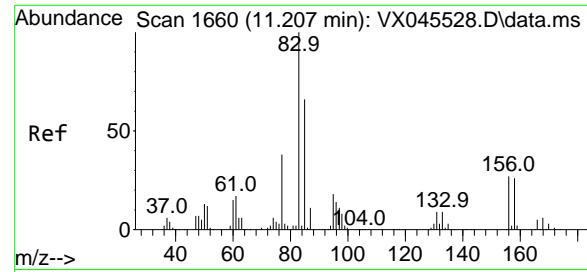


#75  
1,1,2,2-Tetrachloroethane  
Concen: 20.056 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01


### Manual Integrations APPROVED


Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

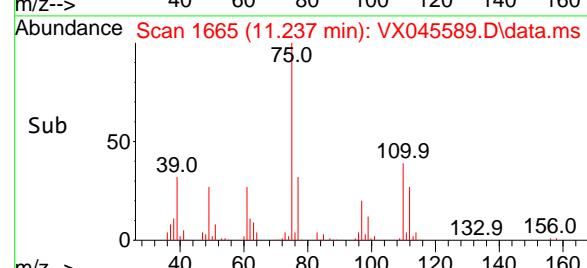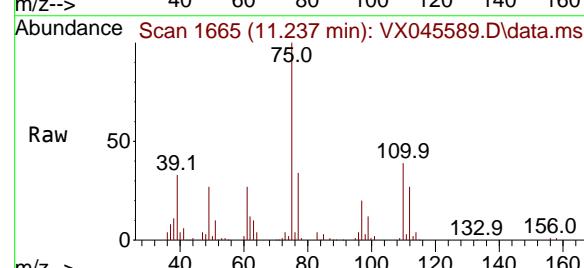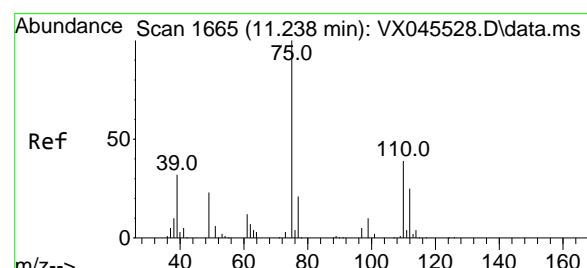

#76  
1,2,3-Trichloropropane  
Concen: 19.363 ug/l  
RT: 11.237 min Scan# 1665  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 75 Resp: 31448  
Ion Ratio Lower Upper  
75 100  
77 41.4 20.0 59.9

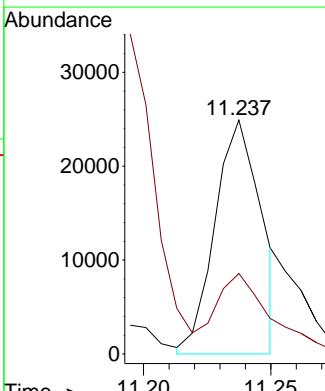

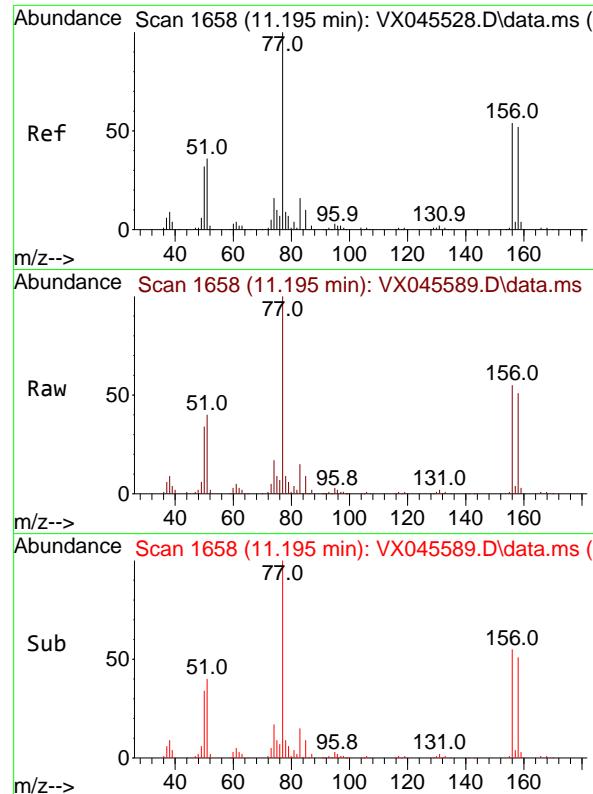

#77

Bromobenzene

Concen: 20.293 ug/l

RT: 11.195 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X



ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

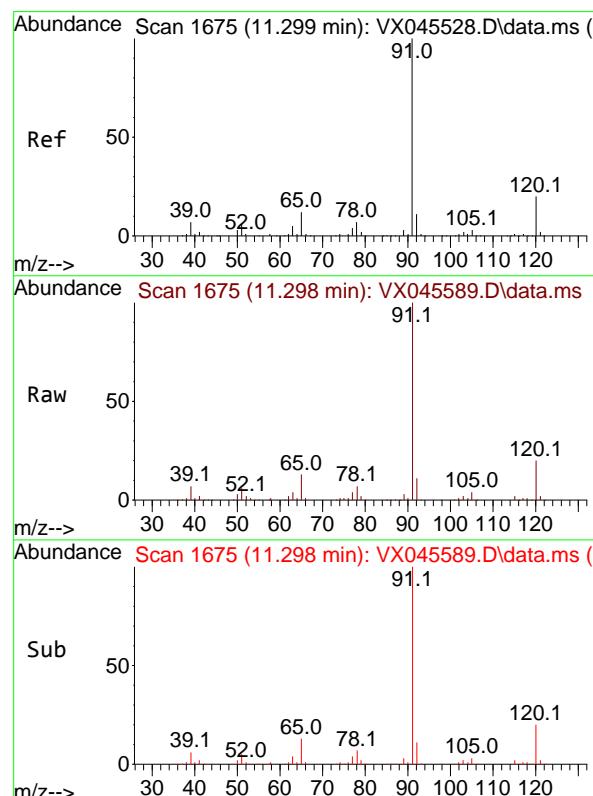

#78

n-propylbenzene

Concen: 20.644 ug/l

RT: 11.298 min Scan# 1675


Delta R.T. -0.000 min




Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Tgt Ion: 91 Resp: 126822

Ion	Ratio	Lower	Upper
91	100		
120	20.8	10.8	32.3



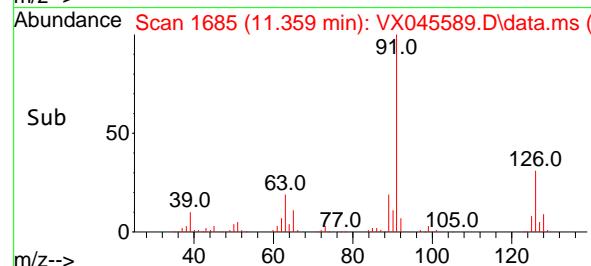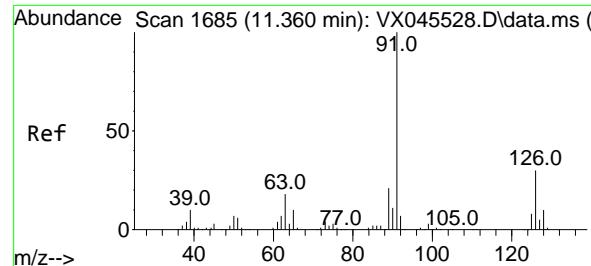

#79

2-Chlorotoluene

Concen: 20.058 ug/l

RT: 11.359 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X





ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

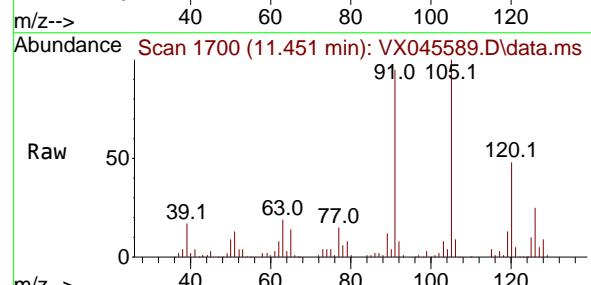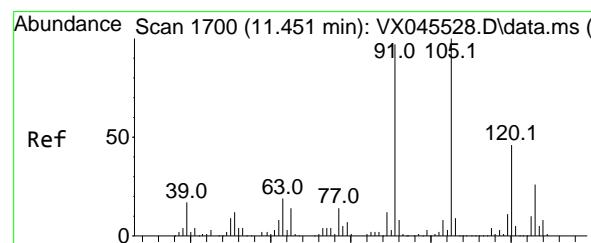

#80

1,3,5-Trimethylbenzene

Concen: 20.856 ug/l


RT: 11.451 min Scan# 1700


Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Tgt	Ion:105	Resp:	91980
Ion	Ratio	Lower	Upper
105	100		
120	45.5	23.0	69.0

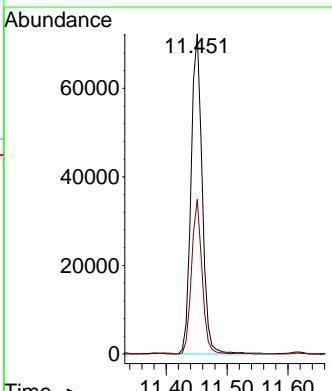


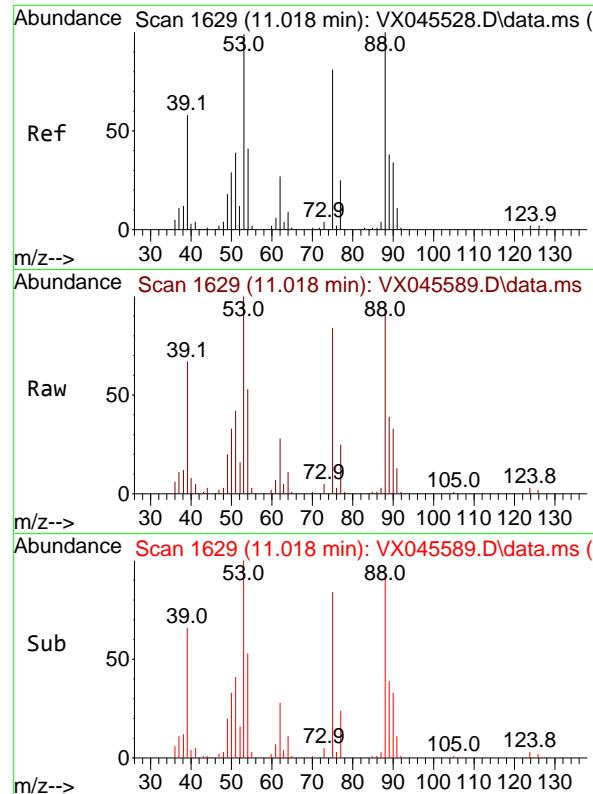


#81  
trans-1,4-Dichloro-2-butene  
Concen: 18.366 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

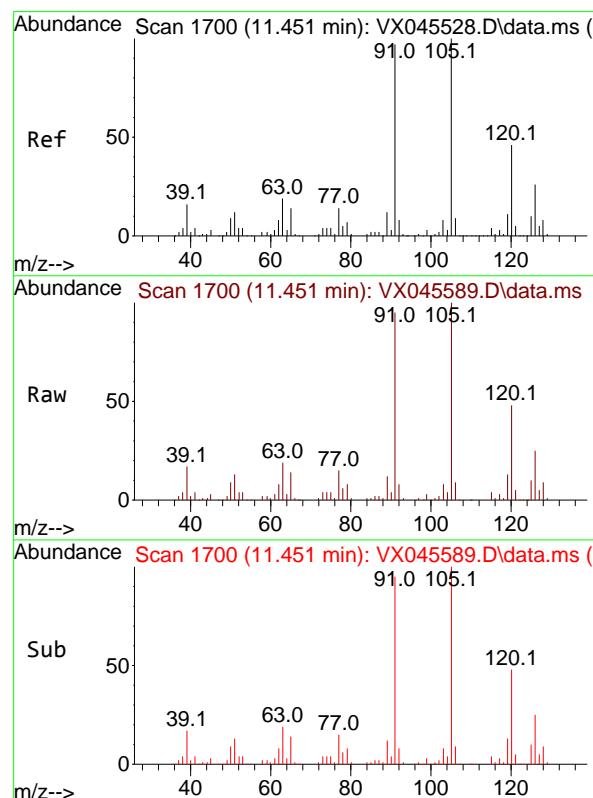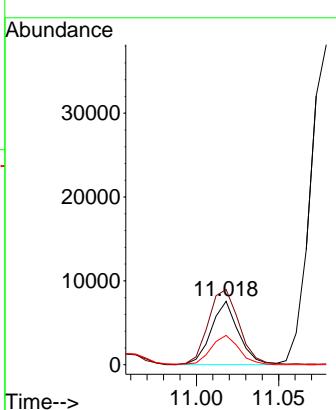

#82  
4-Chlorotoluene  
Concen: 20.657 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion: 91 Resp: 90453  
Ion Ratio Lower Upper  
91 100  
126 26.6 13.3 39.9

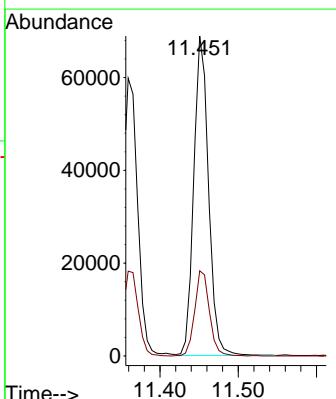

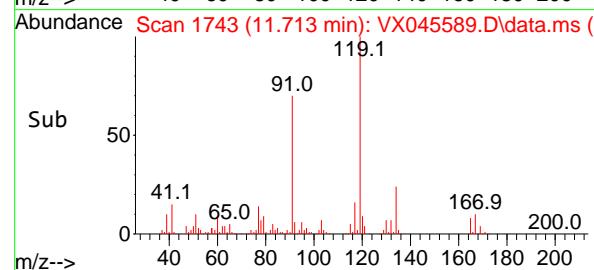

#83

tert-Butylbenzene

Concen: 20.336 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X





ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

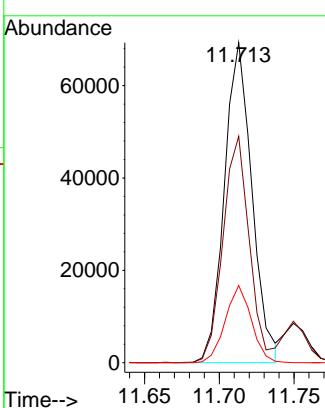

#84

1,2,4-Trimethylbenzene

Concen: 20.614 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14




Tgt Ion:105 Resp: 91248

Ion Ratio Lower Upper

105 100

120 42.1 21.4 64.3

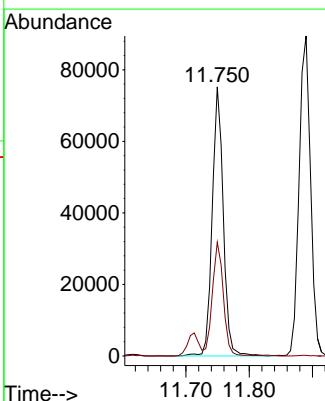



#85

sec-Butylbenzene

Concen: 20.849 ug/l

RT: 11.890 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X




ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#86

p-Isopropyltoluene

Concen: 20.513 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion:119 Resp: 90695


Ion Ratio Lower Upper

119 100

134 25.4 12.6 37.8

91 27.7 13.7 41.1

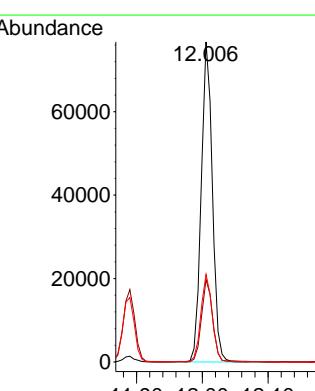

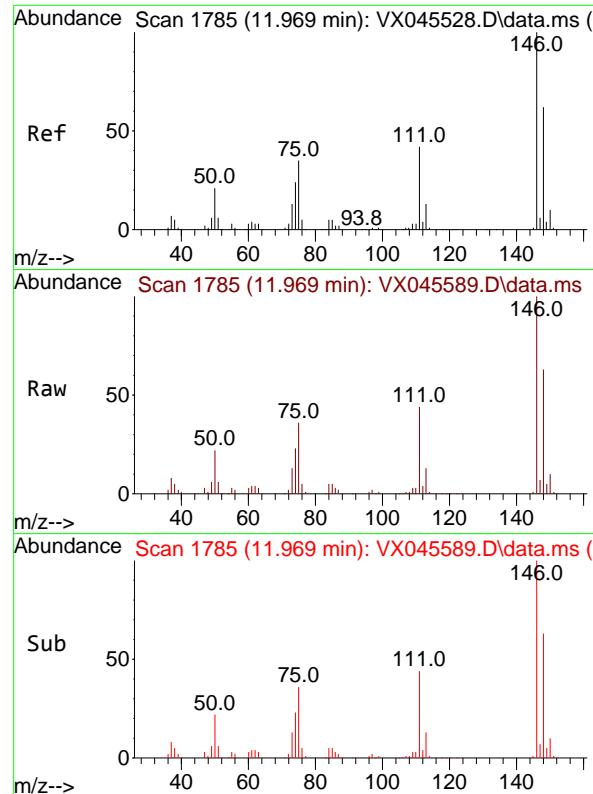

#87

1,3-Dichlorobenzene

Concen: 19.656 ug/l

RT: 11.969 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument:

MSVOA\_X



ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

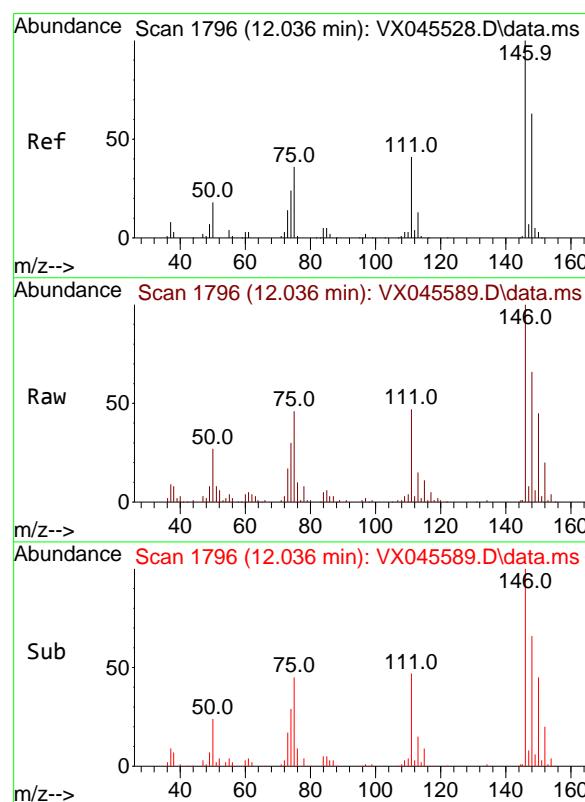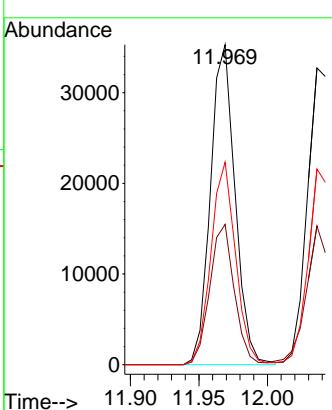

#88

1,4-Dichlorobenzene

Concen: 19.494 ug/l


RT: 12.036 min Scan# 1796




Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Tgt	Ion:146	Resp:	44331
Ion	Ratio	Lower	Upper
146	100		
111	43.7	20.9	62.8
148	63.9	31.5	94.5

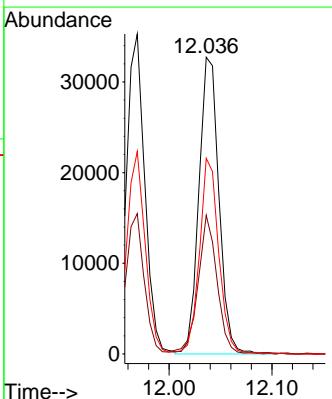



#89

n-Butylbenzene

Concen: 20.250 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X




ClientSampleId :

VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#90

Hexachloroethane

Concen: 20.229 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. -0.000 min

Lab File: VX045589.D


Acq: 04 Apr 2025 11:14







Tgt Ion:117 Resp: 15371

Ion Ratio Lower Upper

117 100

201 61.3 31.2 93.6

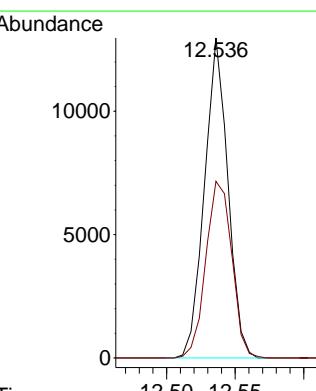



#91

1,2-Dichlorobenzene

Concen: 19.875 ug/l

RT: 12.335 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Instrument : MSVOA\_X

ClientSampleId : VX0404WBS01

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#92

1,2-Dibromo-3-Chloropropane

Concen: 20.243 ug/l

RT: 12.938 min Scan# 1944

Delta R.T. -0.000 min

Lab File: VX045589.D

Acq: 04 Apr 2025 11:14


Tgt Ion: 75 Resp: 7932




Ion Ratio Lower Upper

75 100

155 66.9 34.9 104.7

157 87.5 44.9 134.7








#93  
1,2,4-Trichlorobenzene  
Concen: 19.059 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01



### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

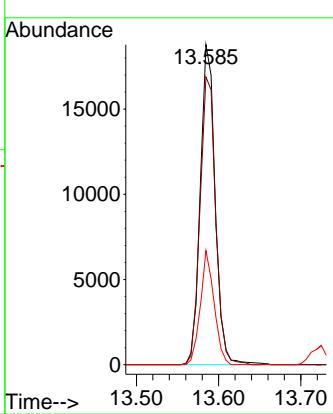

#94  
Hexachlorobutadiene  
Concen: 19.457 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. 0.006 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion:225 Resp: 10408  
Ion Ratio Lower Upper  
225 100  
223 64.9 31.1 93.3  
227 65.7 32.2 96.6




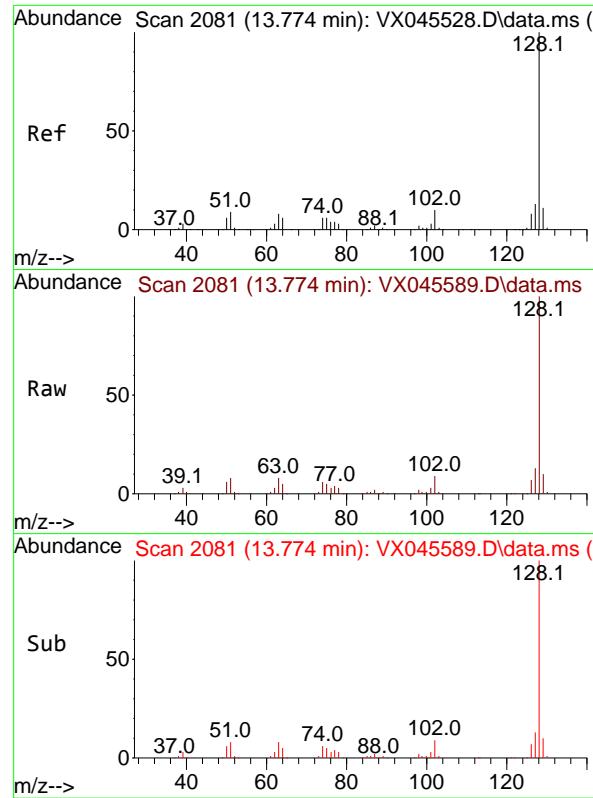


#95  
Naphthalene  
Concen: 18.950 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Instrument : MSVOA\_X  
ClientSampleId : VX0404WBS01


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

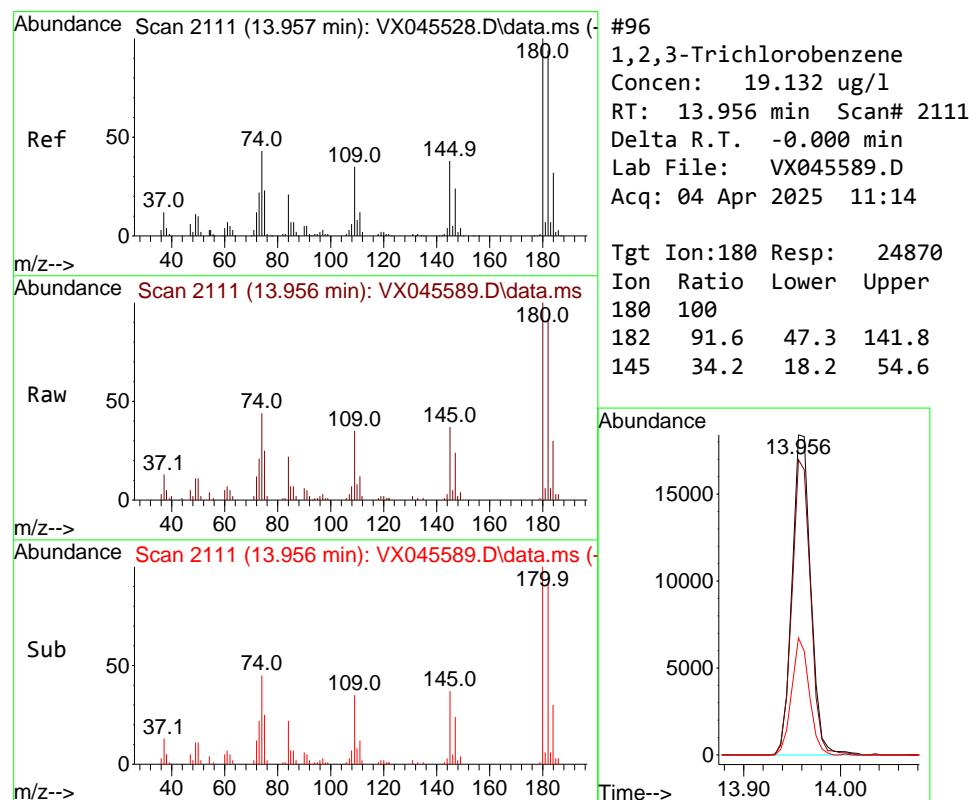

#96  
1,2,3-Trichlorobenzene  
Concen: 19.132 ug/l  
RT: 13.956 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX045589.D  
Acq: 04 Apr 2025 11:14

Tgt Ion:180 Resp: 24870  
Ion Ratio Lower Upper  
180 100  
182 91.6 47.3 141.8  
145 34.2 18.2 54.6

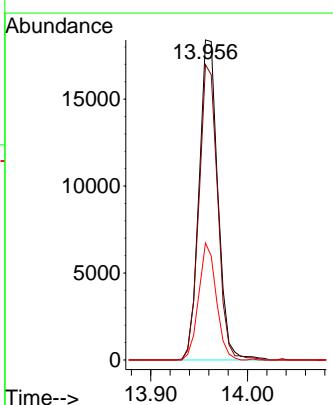



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	04/02/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	04/02/25	
Client Sample ID:	MW-18B-56-040225MS			SDG No.:	Q1711	
Lab Sample ID:	Q1711-02MS			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045591.D	10		04/04/25 12:04	VX040425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	530		2.60	10.0	ug/L
75-35-4	1,1-Dichloroethene	500		2.30	10.0	ug/L
75-34-3	1,1-Dichloroethane	510		2.30	10.0	ug/L
156-59-2	cis-1,2-Dichloroethene	1000		1.90	10.0	ug/L
71-55-6	1,1,1-Trichloroethane	510		2.00	10.0	ug/L
71-43-2	Benzene	500		1.50	10.0	ug/L
107-06-2	1,2-Dichloroethane	510		2.20	10.0	ug/L
79-01-6	Trichloroethene	740		0.93	10.0	ug/L
79-00-5	1,1,2-Trichloroethane	510		2.10	10.0	ug/L
127-18-4	Tetrachloroethene	460		2.30	10.0	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	53.2		70 (74) - 130 (125)	106%	SPK: 50
1868-53-7	Dibromofluoromethane	50.8		70 (75) - 130 (124)	102%	SPK: 50
2037-26-5	Toluene-d8	50.8		70 (86) - 130 (113)	102%	SPK: 50
460-00-4	4-Bromofluorobenzene	53.1		70 (77) - 130 (121)	106%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	84900	5.55			
540-36-3	1,4-Difluorobenzene	154000	6.757			
3114-55-4	Chlorobenzene-d5	137000	10.049			
3855-82-1	1,4-Dichlorobenzene-d4	64900	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045591.D  
 Acq On : 04 Apr 2025 12:04  
 Operator : JC/MD  
 Sample : Q1711-02MS 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-18B-56-040225MS

Quant Time: Apr 04 23:11:21 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	84872	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	154383	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	136696	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	64924	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	82614	53.228	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 106.460%		
35) Dibromofluoromethane	5.379	113	55683	50.836	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 101.680%		
50) Toluene-d8	8.647	98	194235	50.804	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 101.600%		
62) 4-Bromofluorobenzene	11.079	95	73975	53.120	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 106.240%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.167	85	67133	52.891	ug/l	98
3) Chloromethane	1.301	50	67765	51.969	ug/l	97
4) Vinyl Chloride	1.374	62	63807	53.470	ug/l	98
5) Bromomethane	1.593	94	28156	49.761	ug/l	99
6) Chloroethane	1.660	64	32023	50.579	ug/l	100
7) Trichlorofluoromethane	1.868	101	87557	49.204	ug/l	97
8) Diethyl Ether	2.130	74	30881	51.690	ug/l	99
9) 1,1,2-Trichlorotrifluo...	2.319	101	51983	49.853	ug/l	98
10) Methyl Iodide	2.441	142	65918	50.682	ug/l	98
11) Tert butyl alcohol	2.989	59	54825	262.838	ug/l	100
12) 1,1-Dichloroethene	2.307	96	51450	50.496	ug/l	99
13) Acrolein	2.233	56	86595	301.472	ug/l	99
14) Allyl chloride	2.654	41	101301	52.400	ug/l	99
15) Acrylonitrile	3.063	53	169829	257.927	ug/l	100
16) Acetone	2.386	43	165210	259.222	ug/l	99
17) Carbon Disulfide	2.502	76	123194	48.955	ug/l	99
18) Methyl Acetate	2.703	43	78724	53.650	ug/l	99
19) Methyl tert-butyl Ether	3.117	73	187482	52.601	ug/l	99
20) Methylene Chloride	2.782	84	60251	50.497	ug/l	97
21) trans-1,2-Dichloroethene	3.081	96	52111	50.062	ug/l	99
22) Diisopropyl ether	3.764	45	197510	51.865	ug/l	97
23) Vinyl Acetate	3.721	43	901097	273.871	ug/l	99
24) 1,1-Dichloroethane	3.605	63	110230	51.183	ug/l	100
25) 2-Butanone	4.556	43	246533	264.259	ug/l	99
26) 2,2-Dichloropropane	4.471	77	78555	56.455	ug/l	92
27) cis-1,2-Dichloroethene	4.483	96	133119	104.968	ug/l	96
28) Bromochloromethane	4.891	49	52993	50.918	ug/l	97
29) Tetrahydrofuran	5.001	42	162118	268.033	ug/l	99
30) Chloroform	5.087	83	113174	51.070	ug/l	97
31) Cyclohexane	5.465	56	93472	49.094	ug/l	97
32) 1,1,1-Trichloroethane	5.373	97	95681	51.026	ug/l	99
36) 1,1-Dichloropropene	5.684	75	73004	49.362	ug/l	98
37) Ethyl Acetate	4.715	43	92666	49.720	ug/l	99
38) Carbon Tetrachloride	5.666	117	80883	50.603	ug/l	95
39) Methylcyclohexane	7.379	83	88776	48.969	ug/l	97
40) Benzene	6.031	78	223833	49.555	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045591.D  
 Acq On : 04 Apr 2025 12:04  
 Operator : JC/MD  
 Sample : Q1711-02MS 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-18B-56-040225MS

Quant Time: Apr 04 23:11:21 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	52898	53.792	ug/1	99
42) 1,2-Dichloroethane	6.080	62	95516	51.199	ug/1	100
43) Isopropyl Acetate	6.342	43	147747	52.304	ug/1	99
44) Trichloroethene	7.117	130	79074	73.655	ug/1	97
45) 1,2-Dichloropropane	7.428	63	56617	50.237	ug/1	98
46) Dibromomethane	7.574	93	43998	50.857	ug/1	98
47) Bromodichloromethane	7.818	83	86485	50.058	ug/1	97
48) Methyl methacrylate	7.690	41	77910	53.418	ug/1	98
49) 1,4-Dioxane	7.659	88	27082	1026.301	ug/1	98
51) 4-Methyl-2-Pentanone	8.574	43	500710	267.387	ug/1	100
52) Toluene	8.714	92	134349	49.155	ug/1	99
53) t-1,3-Dichloropropene	8.976	75	78488	47.367	ug/1	99
54) cis-1,3-Dichloropropene	8.366	75	87327	53.787	ug/1	100
55) 1,1,2-Trichloroethane	9.147	97	55207	50.689	ug/1	96
56) Ethyl methacrylate	9.116	69	91670	54.386	ug/1	99
57) 1,3-Dichloropropane	9.305	76	96618	50.944	ug/1	98
58) 2-Chloroethyl Vinyl ether	8.238	63	39463	46.282	ug/1	100
59) 2-Hexanone	9.427	43	373976	269.685	ug/1	99
60) Dibromochloromethane	9.519	129	62616	52.736	ug/1	99
61) 1,2-Dibromoethane	9.610	107	57515	52.167	ug/1	97
64) Tetrachloroethene	9.269	164	44500	46.109	ug/1	97
65) Chlorobenzene	10.073	112	145232	49.720	ug/1	96
66) 1,1,1,2-Tetrachloroethane	10.159	131	50931	50.223	ug/1	100
67) Ethyl Benzene	10.189	91	264983	50.652	ug/1	100
68) m/p-Xylenes	10.299	106	193193	101.535	ug/1	100
69) o-Xylene	10.640	106	95904	51.166	ug/1	98
70) Styrene	10.653	104	163226	52.762	ug/1	99
71) Bromoform	10.799	173	40448	53.418	ug/1 #	97
73) Isopropylbenzene	10.957	105	251863	48.431	ug/1	100
74) N-amyl acetate	10.842	43	130118	52.306	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	89186	48.819	ug/1	99
76) 1,2,3-Trichloropropane	11.238	75	76754m	48.466	ug/1	
77) Bromobenzene	11.195	156	57978	48.251	ug/1	100
78) n-propylbenzene	11.305	91	295835	49.387	ug/1	100
79) 2-Chlorotoluene	11.360	91	185225	48.369	ug/1	98
80) 1,3,5-Trimethylbenzene	11.451	105	213377	49.619	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	22958	49.201	ug/1	96
82) 4-Chlorotoluene	11.451	91	212300	49.723	ug/1	100
83) tert-Butylbenzene	11.713	119	211417	49.658	ug/1	100
84) 1,2,4-Trimethylbenzene	11.750	105	214201	49.627	ug/1	99
85) sec-Butylbenzene	11.890	105	263221	50.337	ug/1	99
86) p-Isopropyltoluene	12.006	119	215878	50.074	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	105426	48.200	ug/1	99
88) 1,4-Dichlorobenzene	12.037	146	106695	48.117	ug/1	99
89) n-Butylbenzene	12.329	91	193978	51.887	ug/1	99
90) Hexachloroethane	12.536	117	37819	51.044	ug/1	99
91) 1,2-Dichlorobenzene	12.335	146	105351	48.446	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	20401	53.397	ug/1	98
93) 1,2,4-Trichlorobenzene	13.585	180	59595	49.234	ug/1	100
94) Hexachlorobutadiene	13.725	225	25397	48.691	ug/1	98
95) Naphthalene	13.774	128	228969	50.831	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	62422	49.248	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
 Data File : VX045591.D  
 Acq On : 04 Apr 2025 12:04  
 Operator : JC/MD  
 Sample : Q1711-02MS 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**MW-18B-56-040225MS**

Quant Time: Apr 04 23:11:21 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
(#)						

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040425\  
Data File : VX045591.D  
Acq On : 04 Apr 2025 12:04  
Operator : JC/MD  
Sample : Q1711-02MS 10X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1




Quant Time: Apr 04 23:11:21 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
MW-18B-56-040225MS

## Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

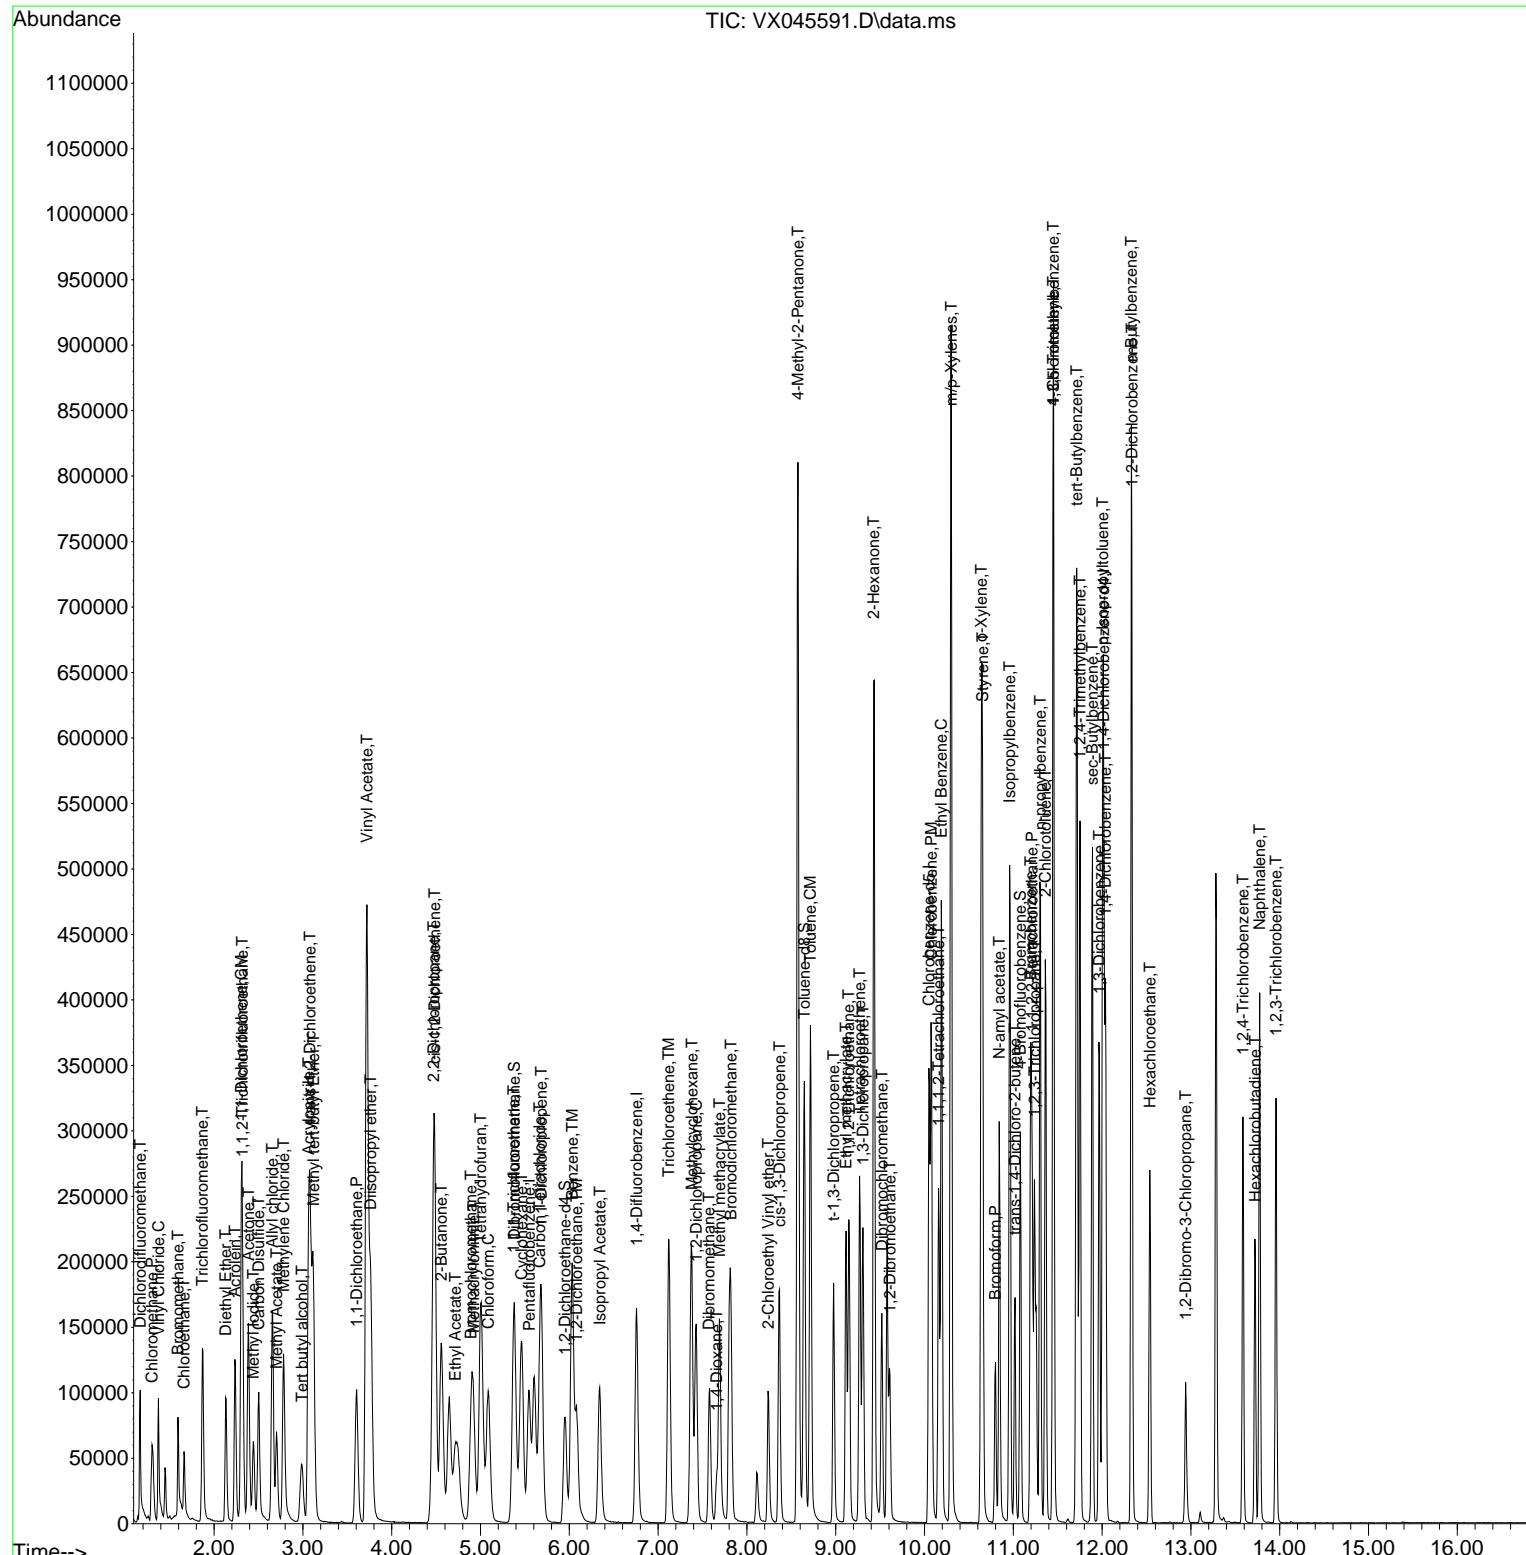



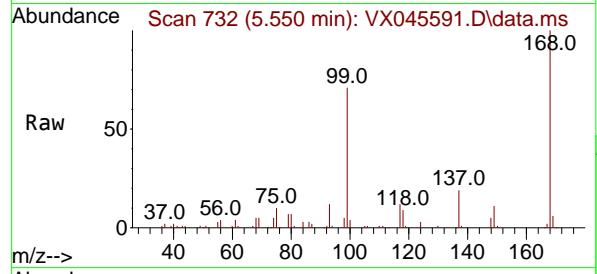
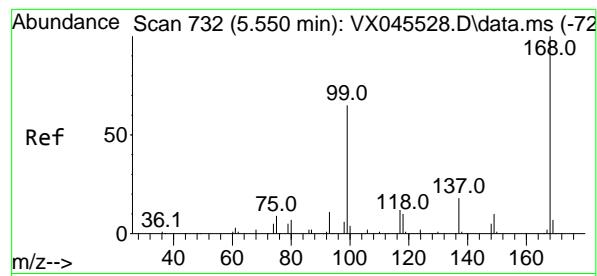


#1  
 Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.550 min Scan# 7  
 Delta R.T. -0.000 min  
 Lab File: VX045591.D  
 Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS


Manual Integrations  
APPROVED


Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025





#2  
 Dichlorodifluoromethane  
 Concen: 52.891 ug/l  
 RT: 1.167 min Scan# 13  
 Delta R.T. 0.000 min  
 Lab File: VX045591.D  
 Acq: 04 Apr 2025 12:04

Tgt Ion: 85 Resp: 67133  
 Ion Ratio Lower Upper  
 85 100  
 87 33.5 16.1 48.2

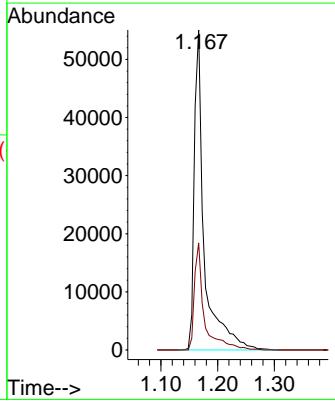




Abundance Scan 35 (1.301 min): VX045591.D\data.ms

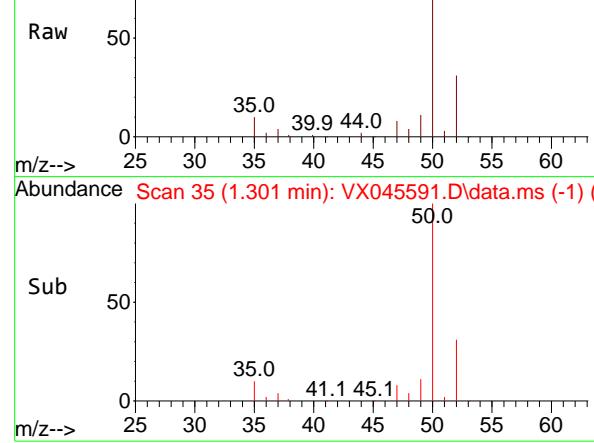

Abundance Scan 47 (1.374 min): VX045591.D\data.ms

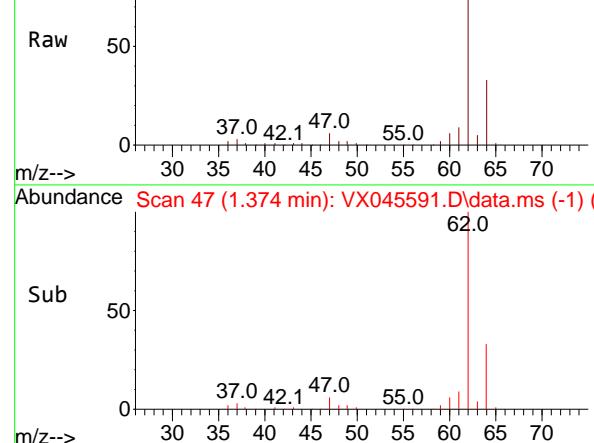

#3

Chloromethane

Concen: 51.969 ug/l

RT: 1.301 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MS

Tgt Ion: 50 Resp: 6776

Ion Ratio Lower Upper


50 100

52 30.8 25.9 38.9

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

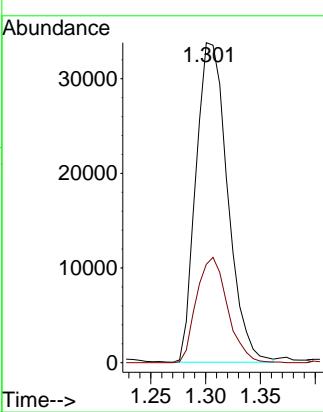

#4

Vinyl Chloride

Concen: 53.470 ug/l

RT: 1.374 min Scan# 47

Delta R.T. 0.000 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04




Tgt Ion: 62 Resp: 63807

Ion Ratio Lower Upper

62 100

64 33.0 25.5 38.3

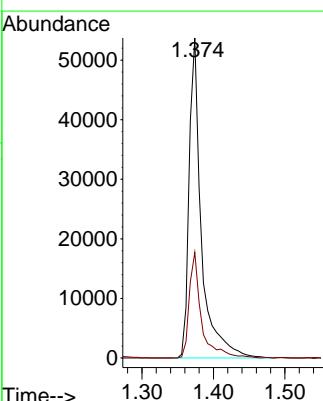



#5

Bromomethane

Concen: 49.761 ug/l

RT: 1.593 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument:

MSVOA\_X





ClientSampleId :

MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#6

Chloroethane

Concen: 50.579 ug/l


RT: 1.660 min Scan# 94


Delta R.T. -0.006 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04

Tgt Ion: 64 Resp: 32023  
 Ion Ratio Lower Upper  
 64 100  
 66 32.7 26.3 39.5

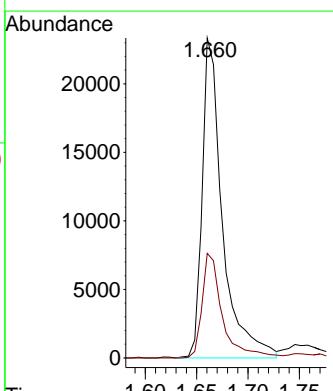




Abundance Scan 128 (1.868 min): VX045591.D\data.ms

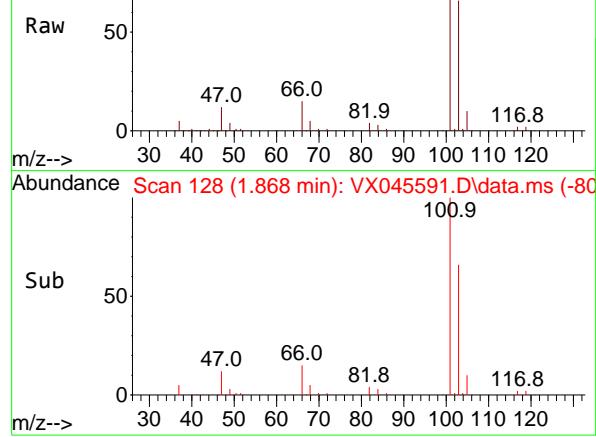

Abundance Scan 128 (1.868 min): VX045591.D\data.ms (-80)

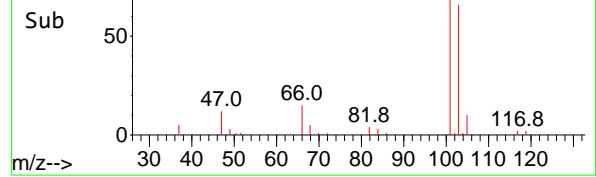



#7

Trichlorofluoromethane  
Concen: 49.204 ug/l  
RT: 1.868 min Scan# 1  
Delta R.T. -0.006 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04


Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS

### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025



Abundance Scan 171 (2.130 min): VX045591.D\data.ms

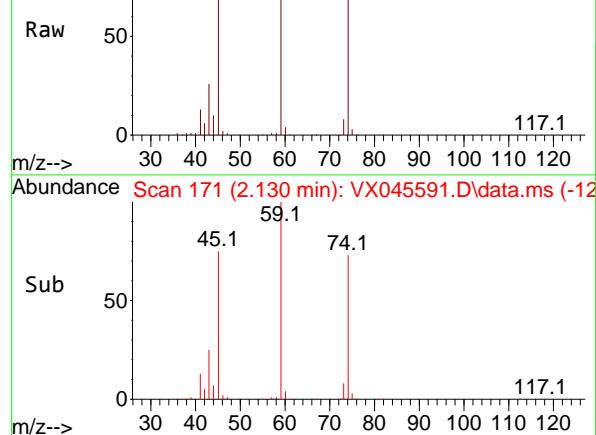


Abundance Scan 171 (2.130 min): VX045591.D\data.ms (-12)






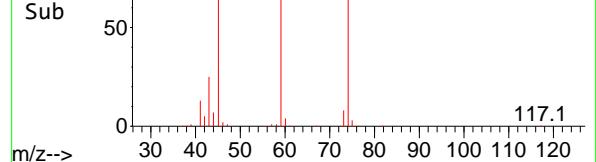


#8

Diethyl Ether  
Concen: 51.690 ug/l  
RT: 2.130 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion: 74 Resp: 30881  
Ion Ratio Lower Upper  
74 100  
45 107.4 53.0 159.1

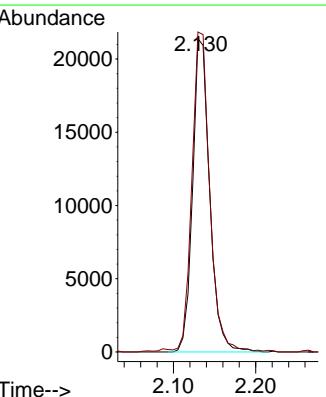

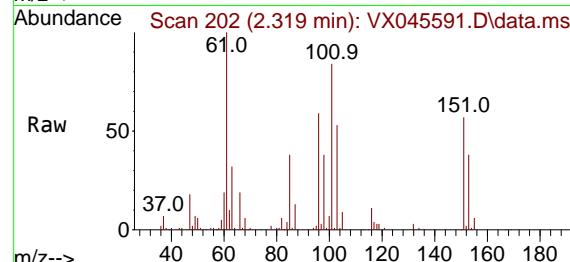

#9

1,1,2-Trichlorotrifluoroethane

Concen: 49.853 ug/l

RT: 2.319 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument:

MSVOA\_X


ClientSampleId :

MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#10

Methyl Iodide

Concen: 50.682 ug/l


RT: 2.441 min Scan# 222


Delta R.T. -0.006 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt	Ion:142	Resp:	65918
Ion	Ratio	Lower	Upper
142	100		
127	52.1	40.2	60.4
141	14.3	11.7	17.5



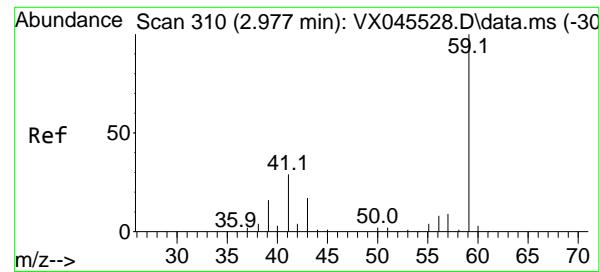

#11





Tert butyl alcohol  
Concen: 262.838 ug/l  
RT: 2.989 min Scan# 3  
Delta R.T. 0.012 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS

Tgt Ion: 59 Resp: 54825  
Ion Ratio Lower Upper  
59 100  
57 10.6 8.6 12.8




Manual Integrations  
APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

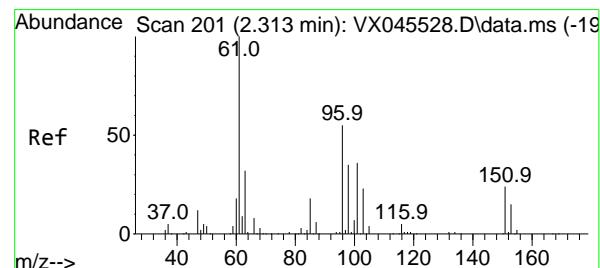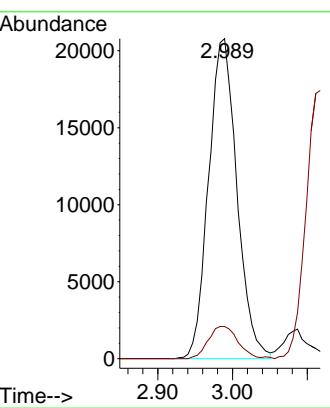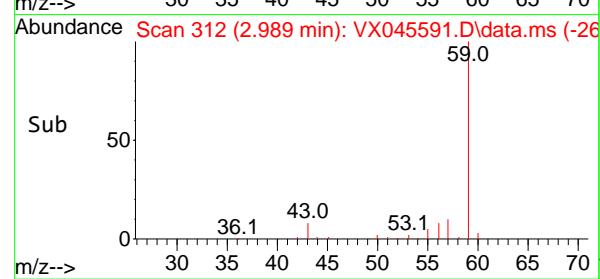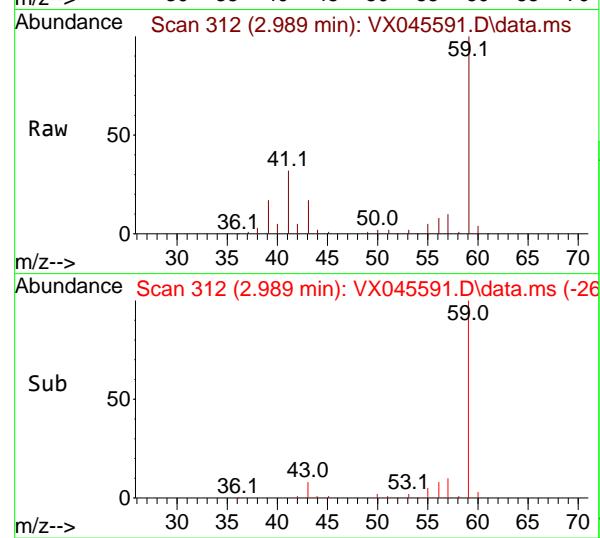



#12  
1,1-Dichloroethene  
Concen: 50.496 ug/l  
RT: 2.307 min Scan# 200  
Delta R.T. -0.006 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion: 96 Resp: 51450  
Ion Ratio Lower Upper  
96 100  
61 184.0 145.7 218.5  
98 63.7 51.6 77.4

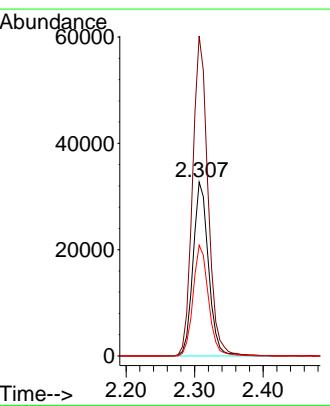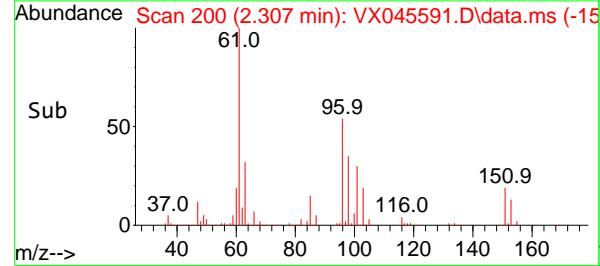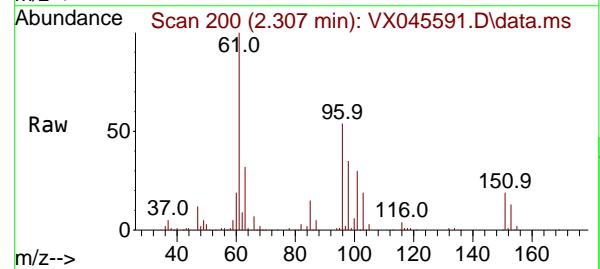




Ref Scan 188 (2.233 min): VX045591.D\data.ms

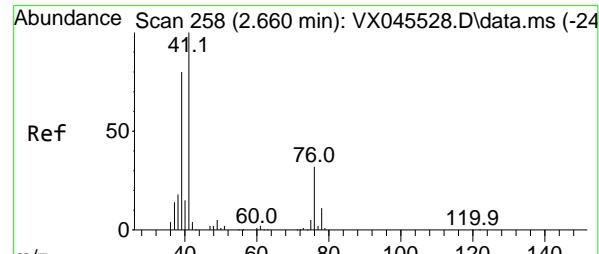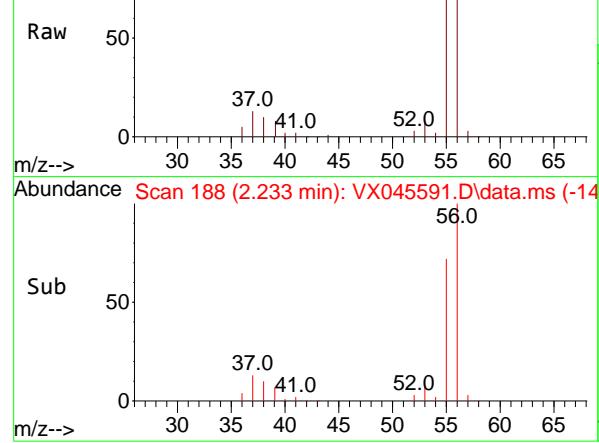

Ref Scan 257 (2.654 min): VX045591.D\data.ms

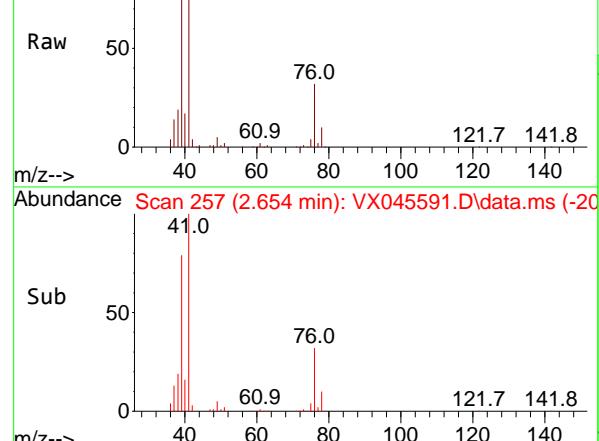

#13

Acrolein

Concen: 301.472 ug/l

RT: 2.233 min Scan# 1

Delta R.T. -0.006 min


Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument: MSVOA\_X  
ClientSampleId: MW-18B-56-040225MS

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025



#14

Allyl chloride

Concen: 52.400 ug/l

RT: 2.654 min Scan# 257


Delta R.T. -0.006 min







Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 41 Resp: 101301  
Ion Ratio Lower Upper

41	100		
39	76.7	60.2	90.2
76	30.9	24.6	36.8



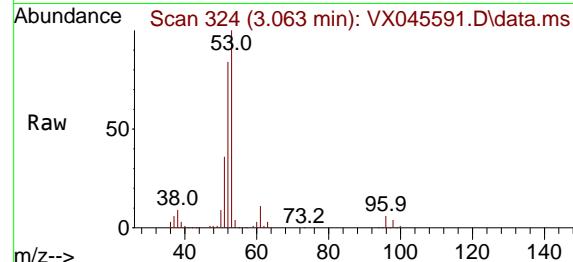

#15

Acrylonitrile

Concen: 257.927 ug/l

RT: 3.063 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument:

MSVOA\_X


ClientSampleId :







MW-18B-56-040225MS

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

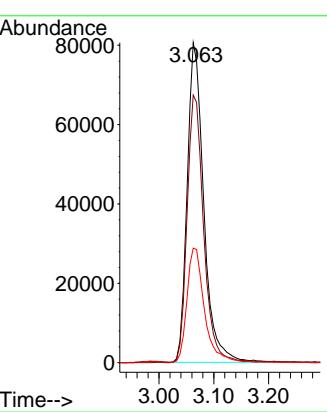

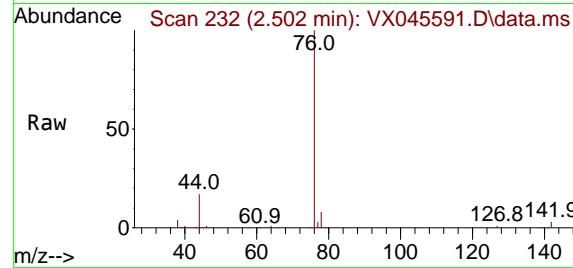

#17

Carbon Disulfide

Concen: 48.955 ug/l

RT: 2.502 min Scan# 2

Delta R.T. -0.006 min


Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument: MSVOA\_X  
ClientSampleId: MW-18B-56-040225MS

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025



#18

Methyl Acetate

Concen: 53.650 ug/l


RT: 2.703 min Scan# 265







Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 43 Resp: 78724  
Ion Ratio Lower Upper  
43 100  
74 21.2 17.5 26.3

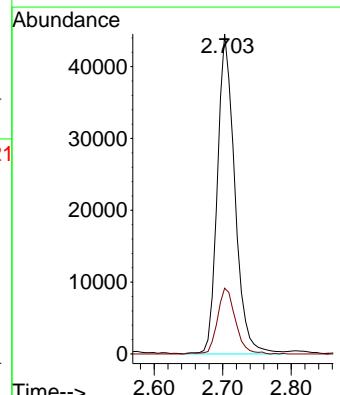

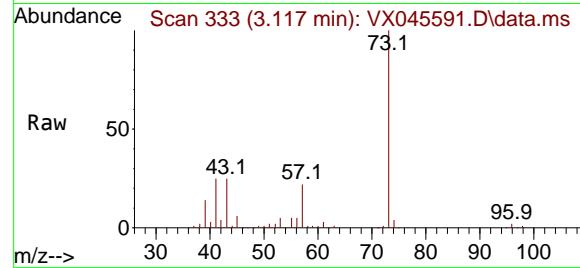


#19

Methyl tert-butyl Ether  
Concen: 52.601 ug/l  
RT: 3.117 min Scan# 3  
Delta R.T. 0.006 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS

### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025






#20

Methylene Chloride  
Concen: 50.497 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion: 84 Resp: 60251  
Ion Ratio Lower Upper  
84 100  
49 138.8 107.5 161.3  
51 41.6 33.0 49.6  
86 65.0 50.1 75.1

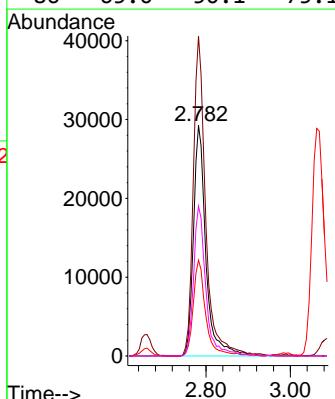






#21  
trans-1,2-Dichloroethene  
Concen: 50.062 ug/l  
RT: 3.081 min Scan# 327  
Delta R.T. -0.006 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument: MSVOA\_X  
Client SampleId: MW-18B-56-040225MS


### Manual Integrations APPROVED


Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025



#22  
Diisopropyl ether  
Concen: 51.865 ug/l  
RT: 3.764 min Scan# 439  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion: 45 Resp: 197510  
Ion Ratio Lower Upper  
45 100  
43 71.0 59.3 88.9  
87 25.5 20.4 30.6  
59 10.2 9.0 13.6

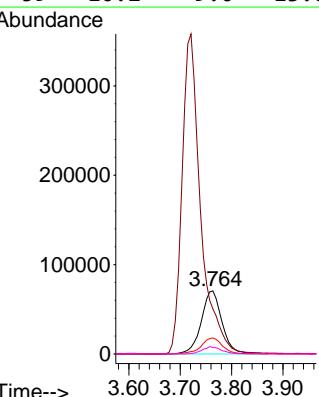



#23

**Vinyl Acetate**

Concen: 273.871 ug/l


RT: 3.721 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04



Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS

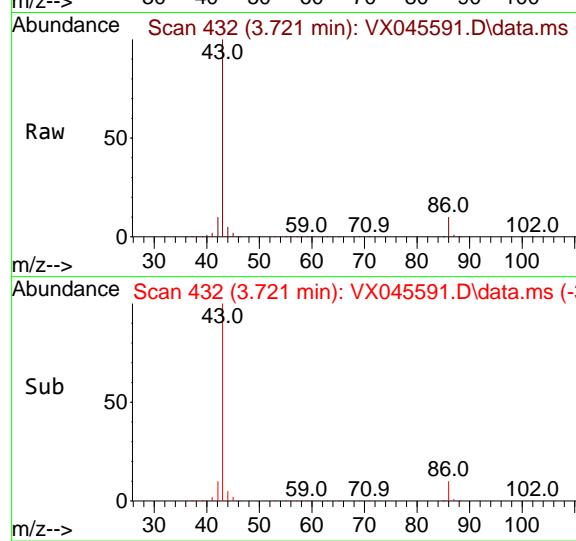

Tgt Ion: 43 Resp: 901091  
 Ion Ratio Lower Upper  
 43 100  
 86 9.6 7.5 11.3

Manual Integrations  
APPROVED

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

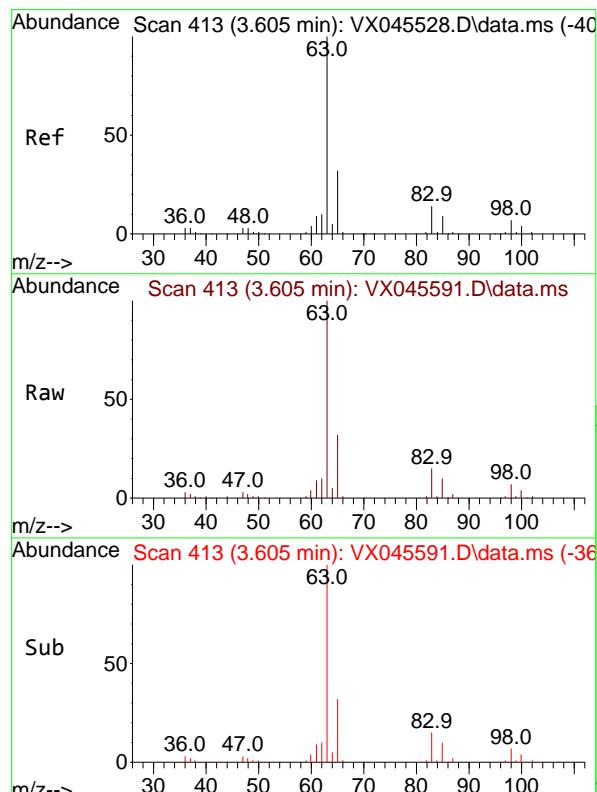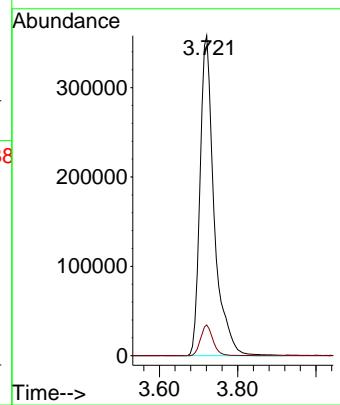

#24

**1,1-Dichloroethane**

Concen: 51.183 ug/l


RT: 3.605 min Scan# 413


Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04


Tgt Ion: 63 Resp: 110230  
 Ion Ratio Lower Upper  
 63 100  
 98 7.0 3.4 10.1  
 100 4.4 2.2 6.6

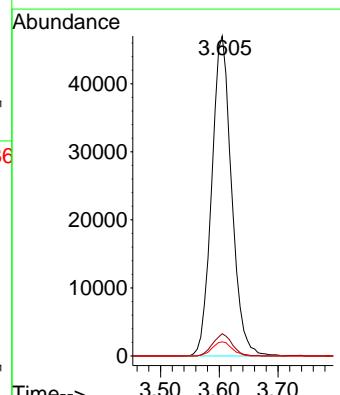



#25  
2-Butanone  
Concen: 264.259 ug/l  
RT: 4.556 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04




Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS

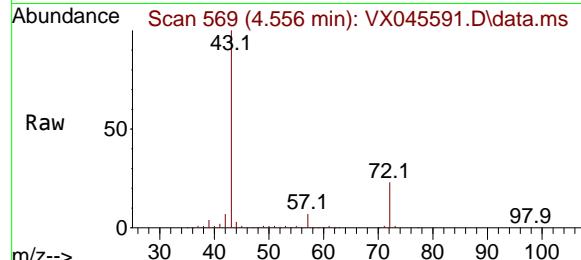


Tgt Ion: 43 Resp: 24653  
Ion Ratio Lower Upper  
43 100  
72 22.9 18.6 28.0

Manual Integrations  
**APPROVED**



Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025




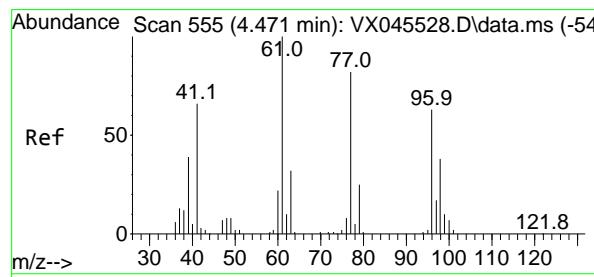
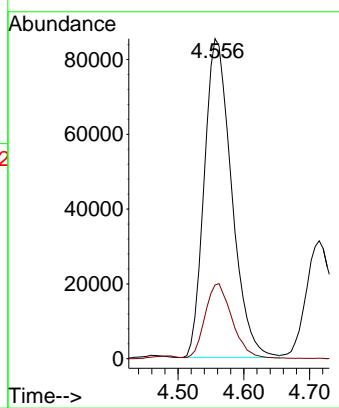
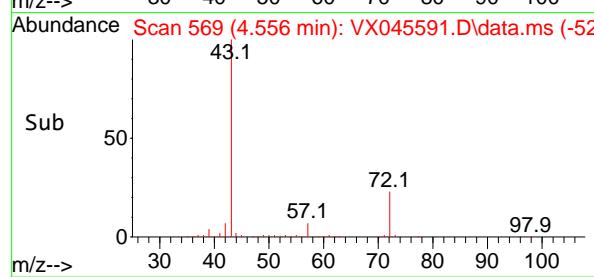


#26  
2,2-Dichloropropane  
Concen: 56.455 ug/l  
RT: 4.471 min Scan# 555  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

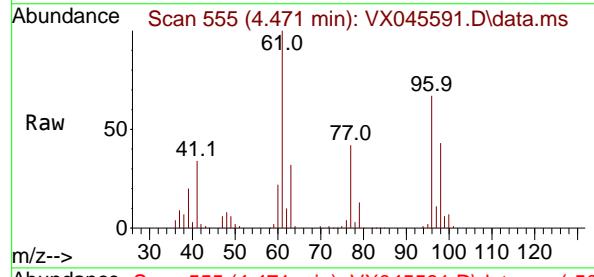

Tgt Ion: 77 Resp: 78555  
Ion Ratio Lower Upper  
77 100  
97 24.9 10.6 31.8

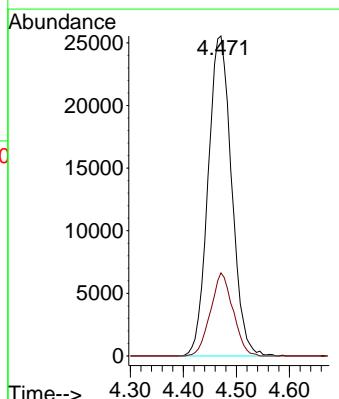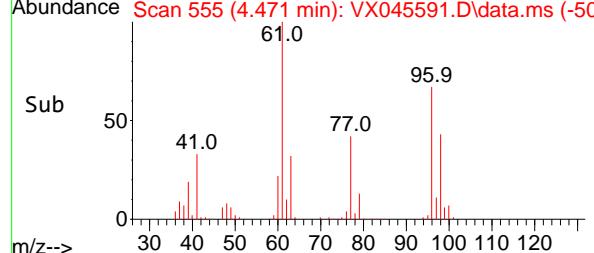




#27  
cis-1,2-Dichloroethene  
Concen: 104.968 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS


### Manual Integrations APPROVED


Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025




#28  
Bromochloromethane  
Concen: 50.918 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion: 49 Resp: 52993  
Ion Ratio Lower Upper  
49 100  
129 0.9 0.0 3.8  
130 66.1 54.6 81.8

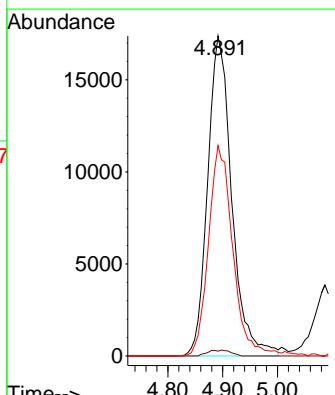



Abundance Scan 642 (5.001 min): VX045591.D\data.ms

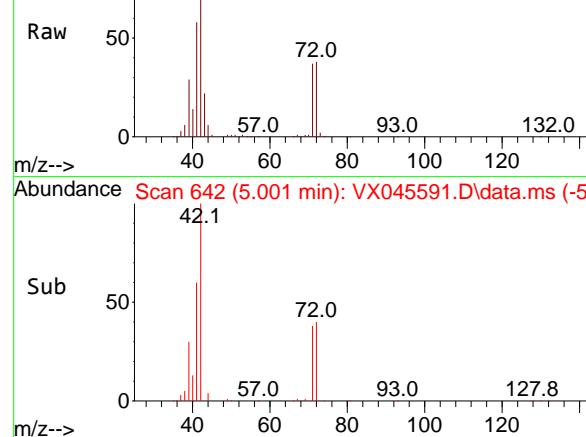

#29

Tetrahydrofuran

Concen: 268.033 ug/l

RT: 5.001 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument :

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MS

Tgt Ion: 42 Resp: 162113

Ion Ratio Lower Upper

42 100

72 42.2 33.4 50.0




71 38.7 31.4 47.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

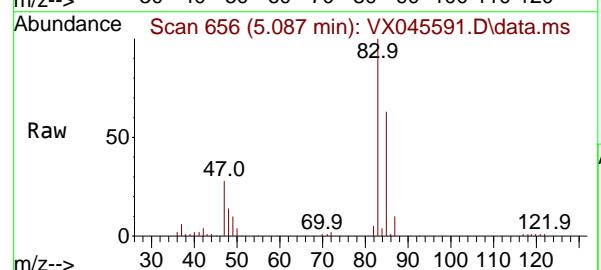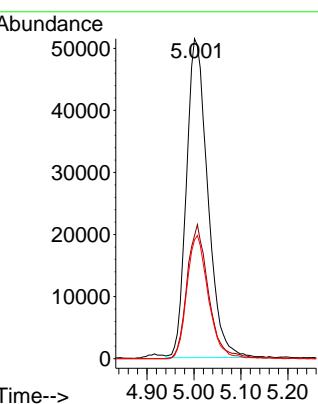

#30

Chloroform

Concen: 51.070 ug/l

RT: 5.087 min Scan# 656

Delta R.T. 0.000 min

Lab File: VX045591.D



Acq: 04 Apr 2025 12:04


Tgt Ion: 83 Resp: 113174

Ion Ratio Lower Upper

83 100

85 63.4 52.8 79.2

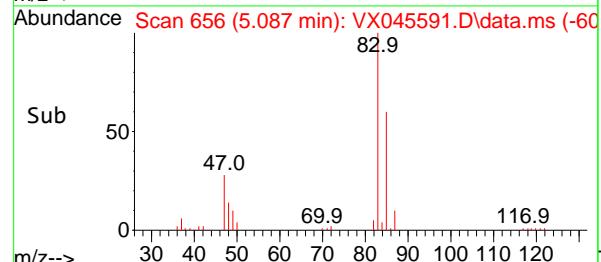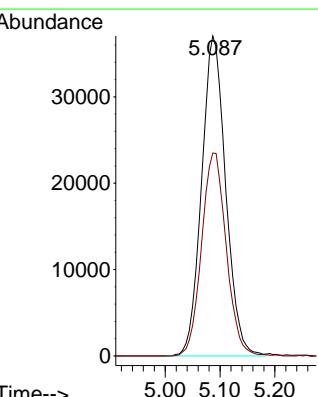



#31

Cyclohexane

Concen: 49.094 ug/l

RT: 5.465 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04

Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MS

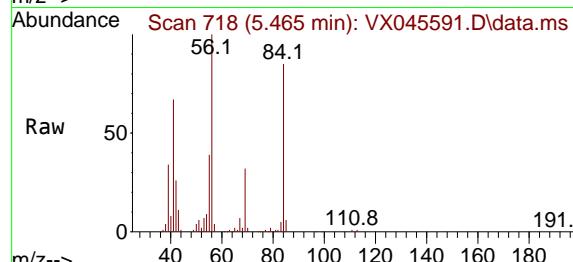

Tgt Ion: 56 Resp: 9347

Ion Ratio Lower Upper

56 100







69 32.2 23.6 35.4







84 82.4 67.7 101.5

**Manual Integrations****APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025
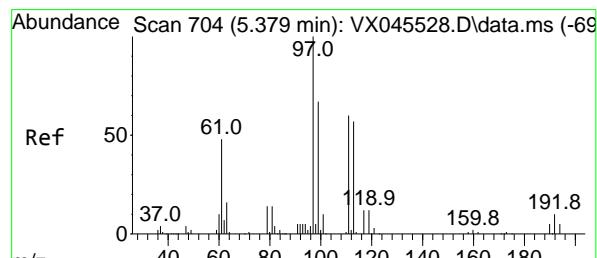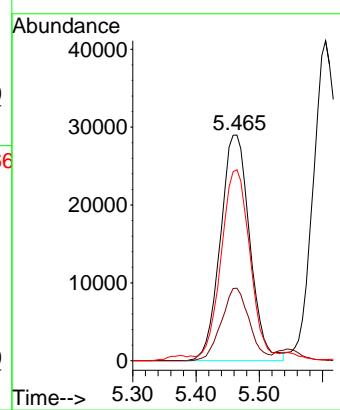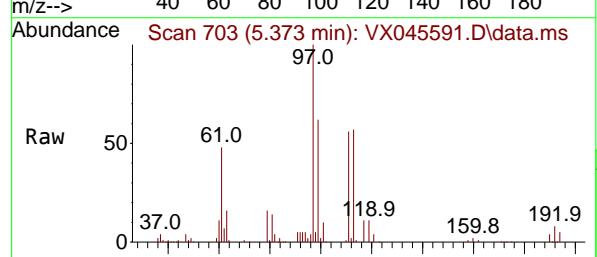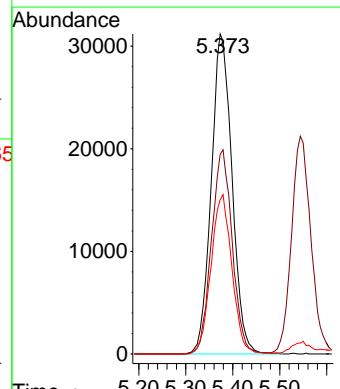
#32  
1,1,1-Trichloroethane  
Concen: 51.026 ug/l  
RT: 5.373 min Scan# 703  
Delta R.T. -0.006 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04Tgt Ion: 97 Resp: 95681  
Ion Ratio Lower Upper  
97 100  
99 63.8 51.7 77.5  
61 50.2 41.0 61.4

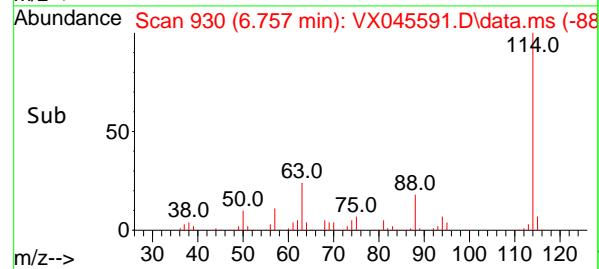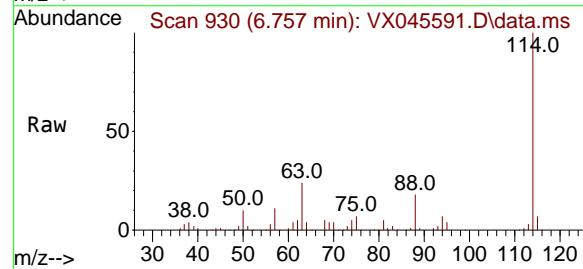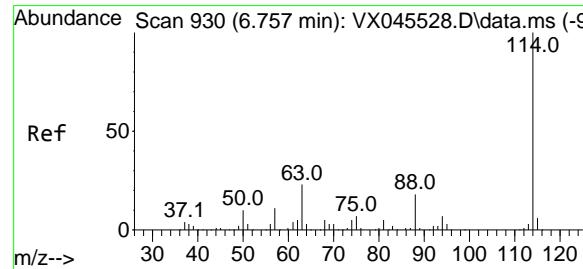

#33

1,2-Dichloroethane-d4

Concen: 53.228 ug/l

RT: 5.952 min Scan# 7

Delta R.T. 0.000 min


Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS

Manual Integrations  
APPROVED

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min


Lab File: VX045591.D




Acq: 04 Apr 2025 12:04

Tgt Ion:114 Resp: 154383

Ion Ratio Lower Upper

114	100		
63	23.8	0.0	46.8
88	17.8	0.0	35.4

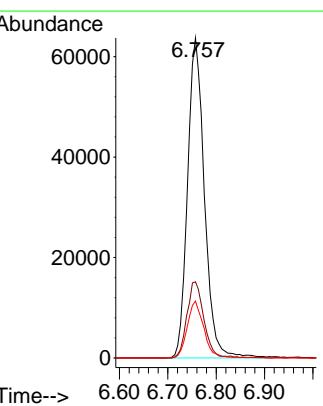



#35

Dibromofluoromethane

Concen: 50.836 ug/l

RT: 5.379 min Scan# 7

Delta R.T. 0.000 min




Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS  
 Acq Date : 04/04/2025 12:04:00  
 Acq Time : 12:04:00  
 Sample ID : VX045591.D

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025



#36

1,1-Dichloropropene

Concen: 49.362 ug/l

RT: 5.684 min Scan# 754


Delta R.T. 0.000 min







Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 75 Resp: 73004  
 Ion Ratio Lower Upper  
 75 100

Ion	Ratio	Lower	Upper
75	100		
110	31.7	16.9	50.6
77	30.7	25.0	37.4

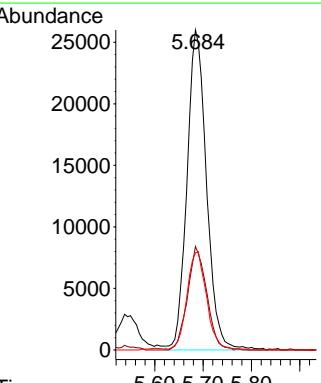

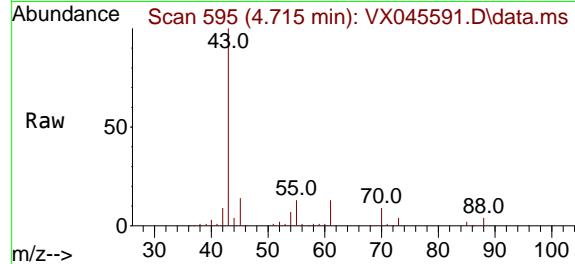

#37

**Ethyl Acetate**

Concen: 49.720 ug/l

RT: 4.715 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument:

MSVOA\_X


ClientSampleId :

MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#38

**Carbon Tetrachloride**

Concen: 50.603 ug/l


RT: 5.666 min Scan# 751







Delta R.T. -0.006 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt	Ion:117	Resp:	80883
Ion	Ratio	Lower	Upper
117	100		
119	90.2	76.9	115.3
121	28.8	24.2	36.2

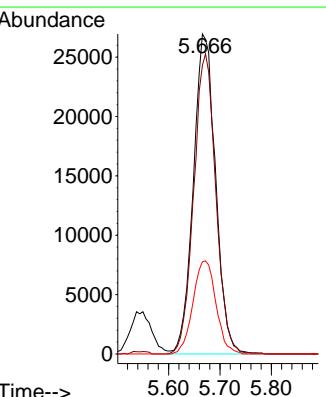

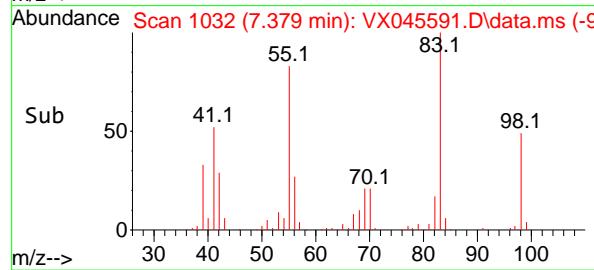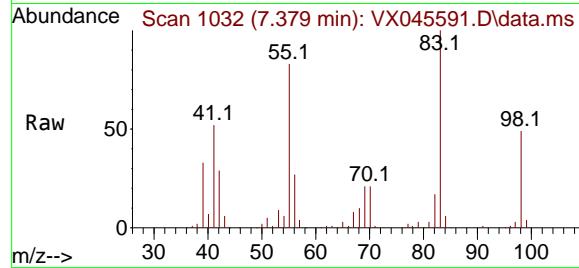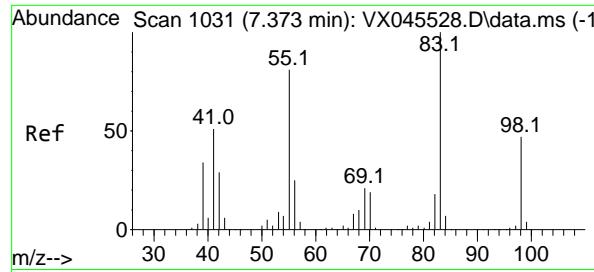

#39

Methylcyclohexane

Concen: 48.969 ug/l

RT: 7.379 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X


ClientSampleId :

MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#40

Benzene

Concen: 49.555 ug/l

RT: 6.031 min Scan# 811

Delta R.T. 0.000 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04







Tgt Ion: 78 Resp: 223833

Ion Ratio Lower Upper

78 100

77 24.0 19.0 28.6



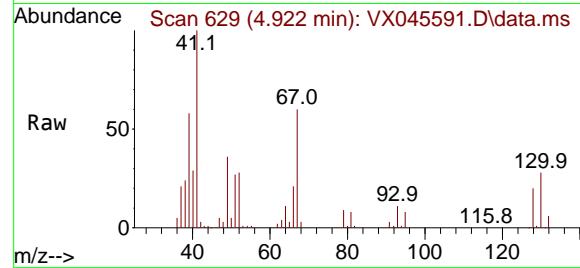

#41

Methacrylonitrile

Concen: 53.792 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument :

MSVOA\_X


ClientSampleId :

MW-18B-56-040225MS

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

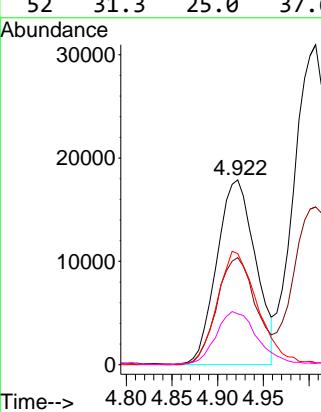

#42

1,2-Dichloroethane

Concen: 51.199 ug/l

RT: 6.080 min Scan# 819

Delta R.T. 0.000 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04


Tgt Ion: 62 Resp: 95516

Ion Ratio Lower Upper


62 100

98 7.5 0.0 15.2

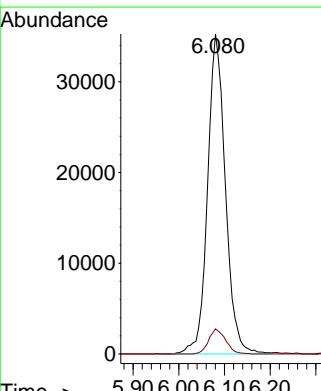




Abundance Scan 862 (6.342 min): VX045591.D\data.ms

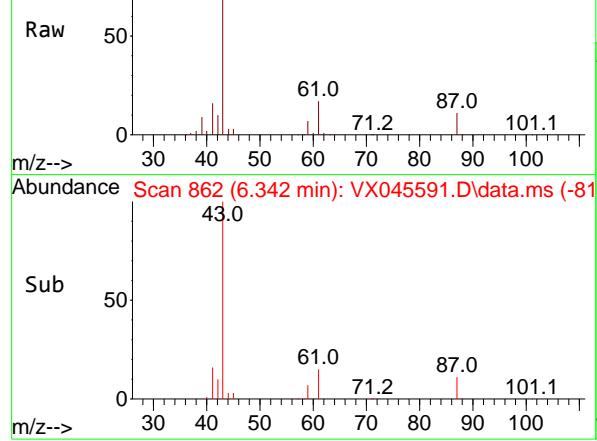

Abundance Scan 862 (6.342 min): VX045591.D\data.ms (-81)

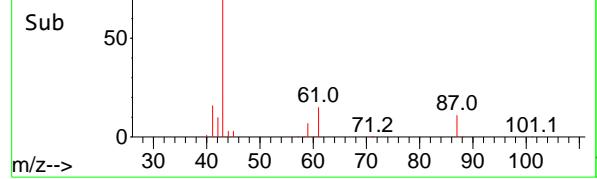

#43

Isopropyl Acetate

Concen: 52.304 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument :

MSVOA\_X

ClientSampleId :



MW-18B-56-040225MS

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025


Abundance

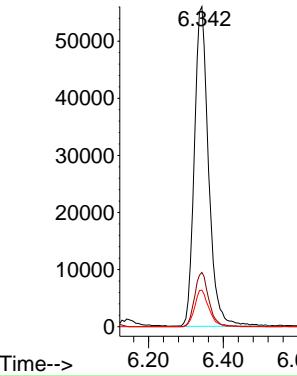

Abundance Scan 989 (7.117 min): VX045591.D\data.ms

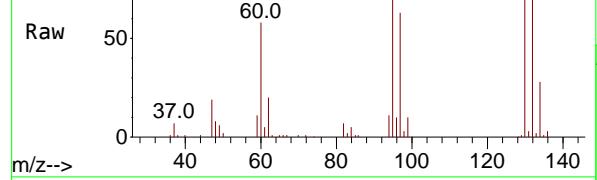

Abundance Scan 989 (7.117 min): VX045591.D\data.ms (-94)

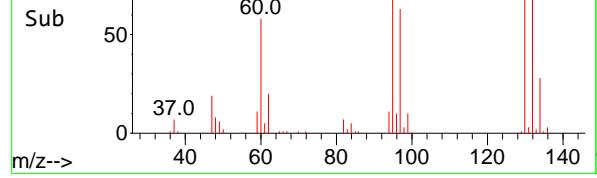

#44

Trichloroethene

Concen: 73.655 ug/l

RT: 7.117 min Scan# 989

Delta R.T. -0.006 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04


Tgt Ion:130 Resp: 79074




Ion Ratio Lower Upper

130 100

95 104.5 0.0 202.0

Abundance

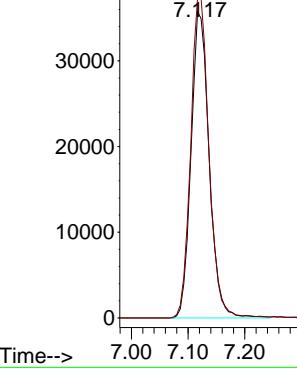



#45

1,2-Dichloropropane

Concen: 50.237 ug/l

RT: 7.428 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04





Instrument: MSVOA\_X

ClientSampleId : MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

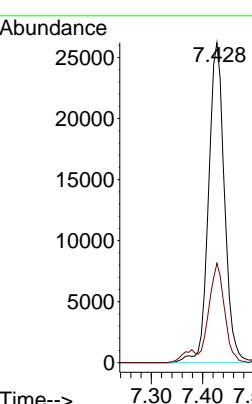

#46

Dibromomethane

Concen: 50.857 ug/l

RT: 7.574 min Scan# 1064


Delta R.T. 0.000 min




Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 93 Resp: 43998

Ion	Ratio	Lower	Upper
93	100		
95	83.0	64.8	97.2
174	84.0	65.4	98.0

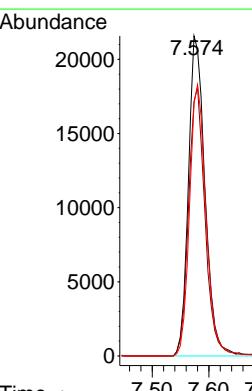



#47

Bromodichloromethane

Concen: 50.058 ug/l

RT: 7.818 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX045591.D





Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#48

Methyl methacrylate

Concen: 53.418 ug/l


RT: 7.690 min Scan# 1083







Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 41 Resp: 77910  
Ion Ratio Lower Upper  
41 100  
69 72.0 58.2 87.2  
39 65.3 53.6 80.4

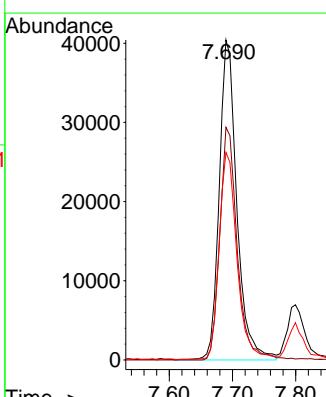

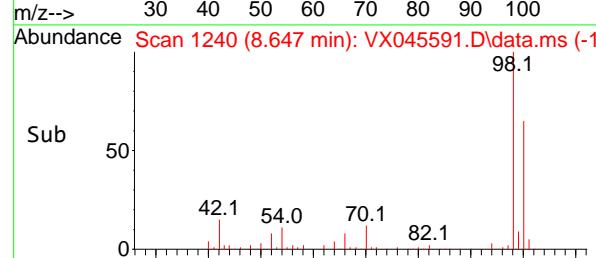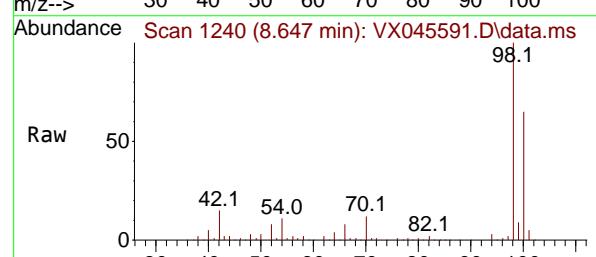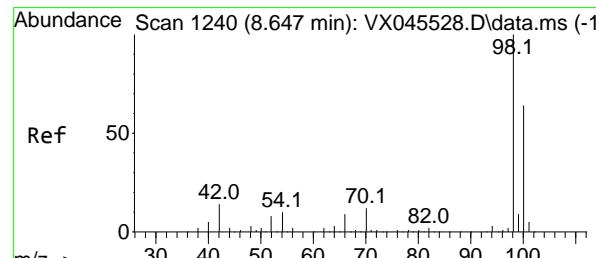

#49

1,4-Dioxane

Concen: 1026.301 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument :

MSVOA\_X


ClientSampleId :

MW-18B-56-040225MS

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

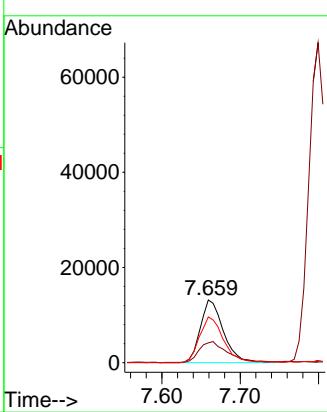

#50

Toluene-d8

Concen: 50.804 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04


Tgt Ion: 98 Resp: 194235

Ion Ratio Lower Upper


98 100

100 65.5 52.2 78.4

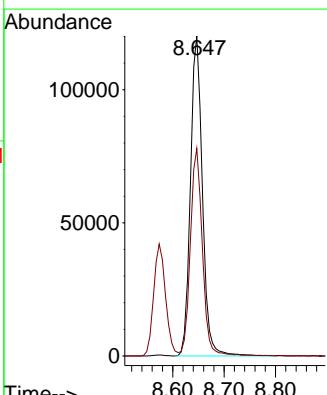




Abundance Scan 1228 (8.574 min): VX045591.D\data.ms

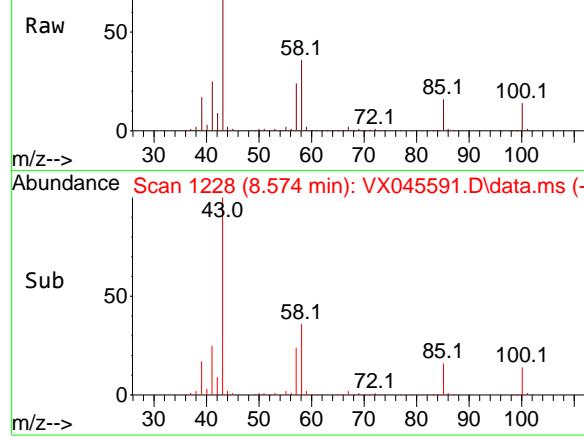

Abundance Scan 1228 (8.574 min): VX045591.D\data.ms (-1)

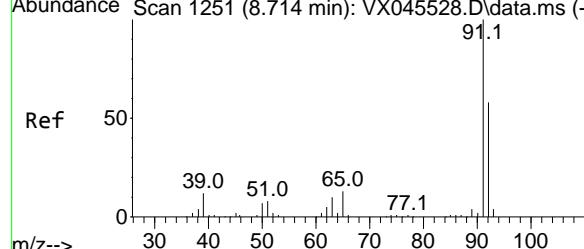

Abundance Scan 1228 (8.574 min): VX045591.D\data.ms

#51

4-Methyl-2-Pentanone

Concen: 267.387 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. 0.000 min



Lab File: VX045591.D

Acq: 04 Apr 2025 12:04


Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS

**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

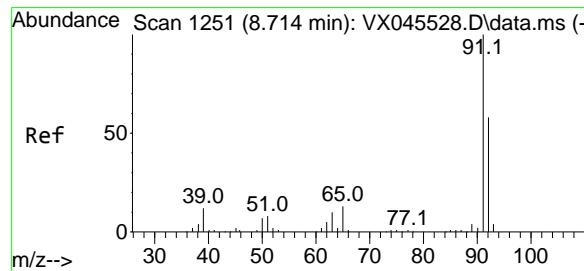

Abundance Scan 1251 (8.714 min): VX045591.D\data.ms

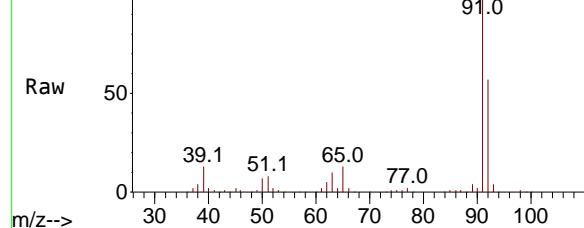

Abundance Scan 1251 (8.714 min): VX045591.D\data.ms

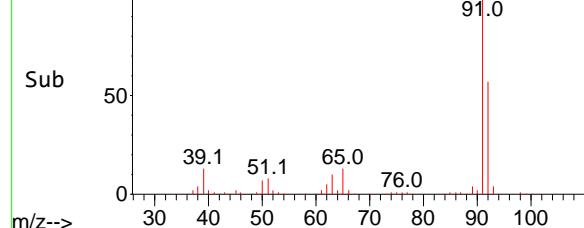

Abundance Scan 1251 (8.714 min): VX045591.D\data.ms

#52

Toluene

Concen: 49.155 ug/l


RT: 8.714 min Scan# 1251




Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 92 Resp: 134349  
 Ion Ratio Lower Upper  
 92 100  
 91 174.4 138.7 208.1

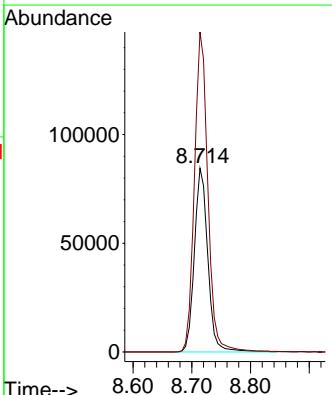



#53

t-1,3-Dichloropropene

Concen: 47.367 ug/l

RT: 8.976 min Scan# 1194

Delta R.T. 0.000 min





Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X

ClientSampleId : MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

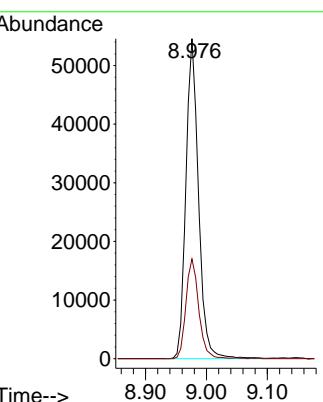 Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025


#54

cis-1,3-Dichloropropene


Concen: 53.787 ug/l




RT: 8.366 min Scan# 1194

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

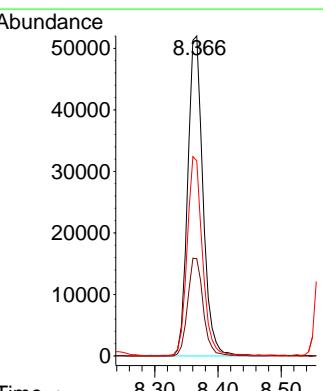 Tgt Ion: 75 Resp: 87327  
 Ion Ratio Lower Upper  
 75 100  
 77 30.4 24.6 36.8  
 39 60.8 48.4 72.6




#55

1,1,2-Trichloroethane

Concen: 50.689 ug/l

RT: 9.147 min Scan# 1322

Delta R.T. 0.000 min




Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025



#56

Ethyl methacrylate

Concen: 54.386 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min


Lab File: VX045591.D




Acq: 04 Apr 2025 12:04

Tgt Ion: 69 Resp: 91670

Ion Ratio Lower Upper

69	100		
41	76.6	61.3	91.9
39	49.0	40.2	60.2

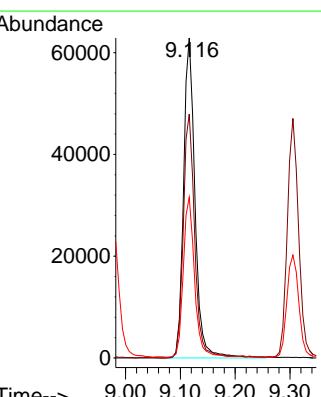

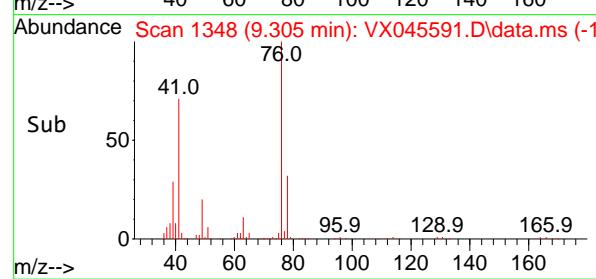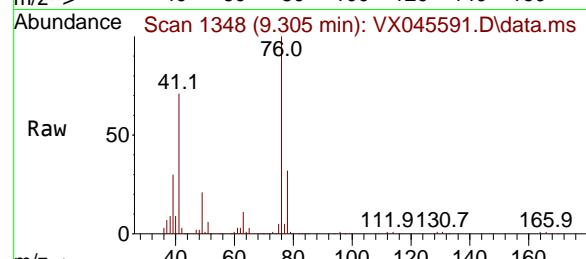

#57

1,3-Dichloropropane

Concen: 50.944 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04





Instrument : MSVOA\_X

ClientSampleId : MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

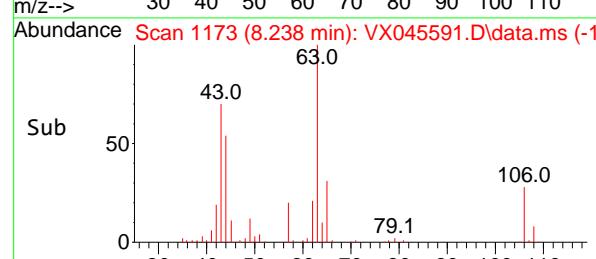

#58

2-Chloroethyl Vinyl ether


Concen: 46.282 ug/l


RT: 8.238 min Scan# 1173

Delta R.T. 0.000 min


Lab File: VX045591.D

Acq: 04 Apr 2025 12:04


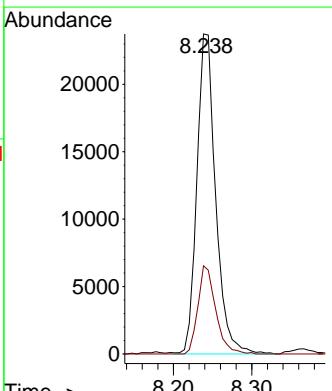
Tgt Ion: 63 Resp: 39463  
Ion Ratio Lower Upper  
63 100  
106 26.1 21.0 31.6




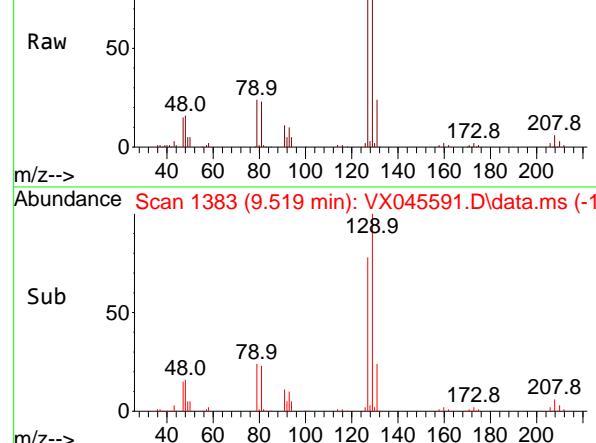
Abundance Scan 1368 (9.427 min): VX045591.D\data.ms

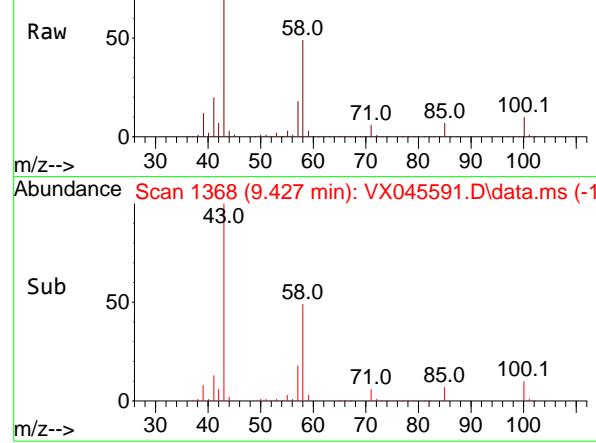


Abundance Scan 1368 (9.427 min): VX045591.D\data.ms (-1)

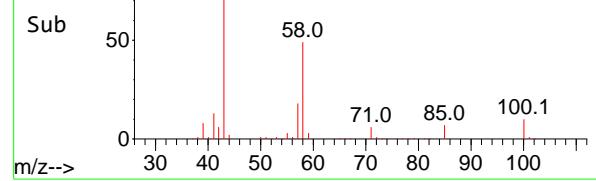

Abundance Scan 1383 (9.519 min): VX045591.D\data.ms



Abundance Scan 1383 (9.519 min): VX045591.D\data.ms (-1)

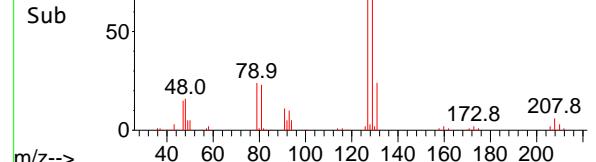

#59

2-Hexanone

Concen: 269.685 ug/l

RT: 9.427 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument:

MSVOA\_X


ClientSampleId :

MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

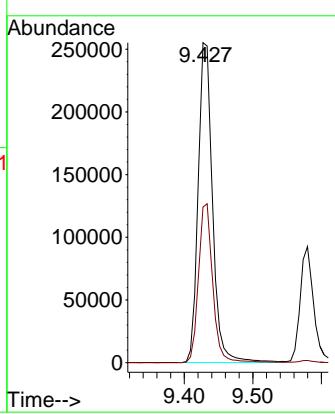

#60

Dibromochloromethane

Concen: 52.736 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04




Tgt Ion:129 Resp: 62616

Ion Ratio Lower Upper

129 100

127 78.1 39.4 118.2

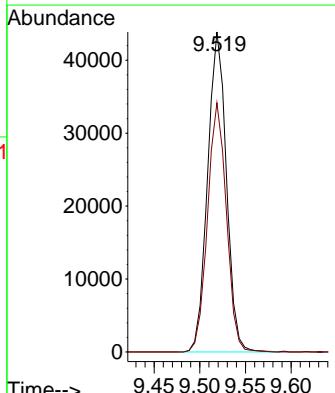

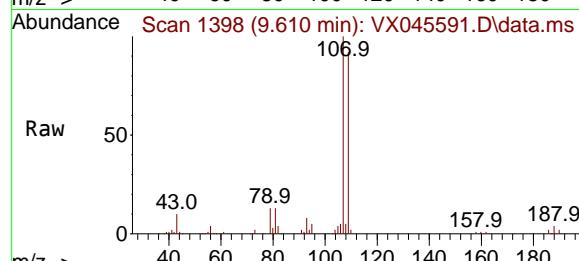

#61

1,2-Dibromoethane

Concen: 52.167 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045591.D





Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

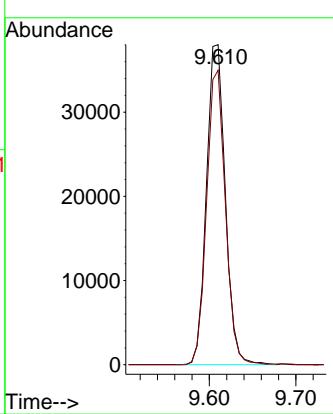

#62

4-Bromofluorobenzene

Concen: 53.120 ug/l


RT: 11.079 min Scan# 1639


Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 95 Resp: 73975  
 Ion Ratio Lower Upper  
 95 100  
 174 68.0 0.0 135.8  
 176 65.6 0.0 131.4




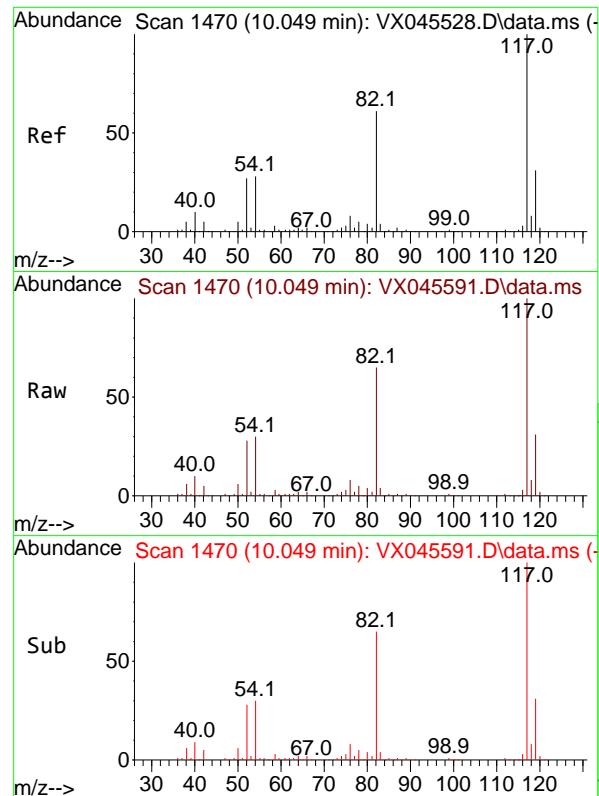


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1470  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04


Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS


### Manual Integrations APPROVED

Reviewed By :John Carbone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

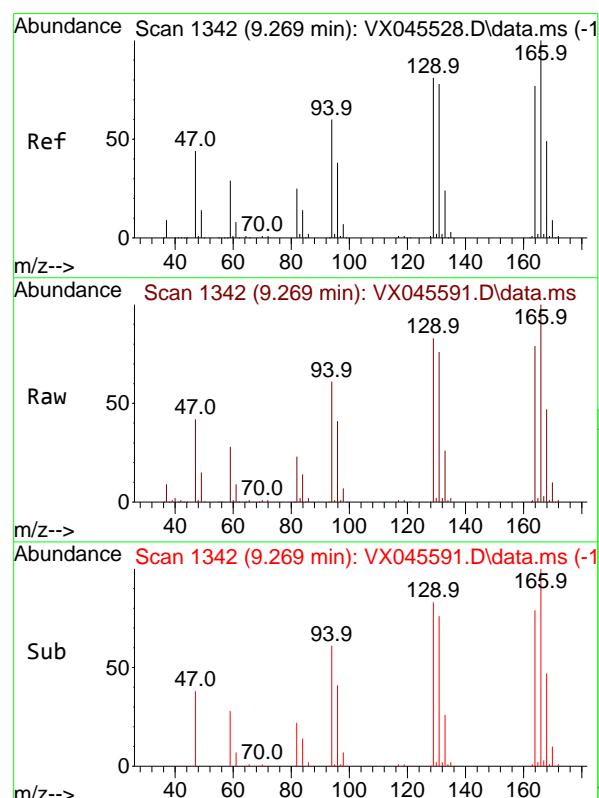

#64  
Tetrachloroethene  
Concen: 46.109 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

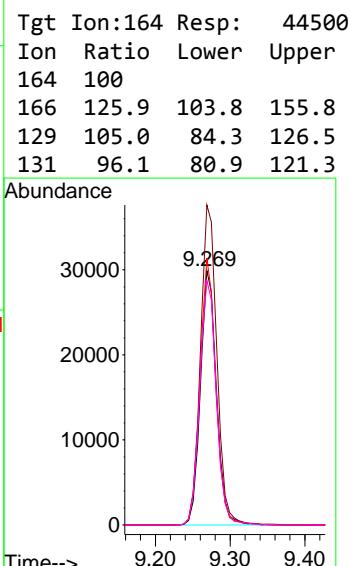


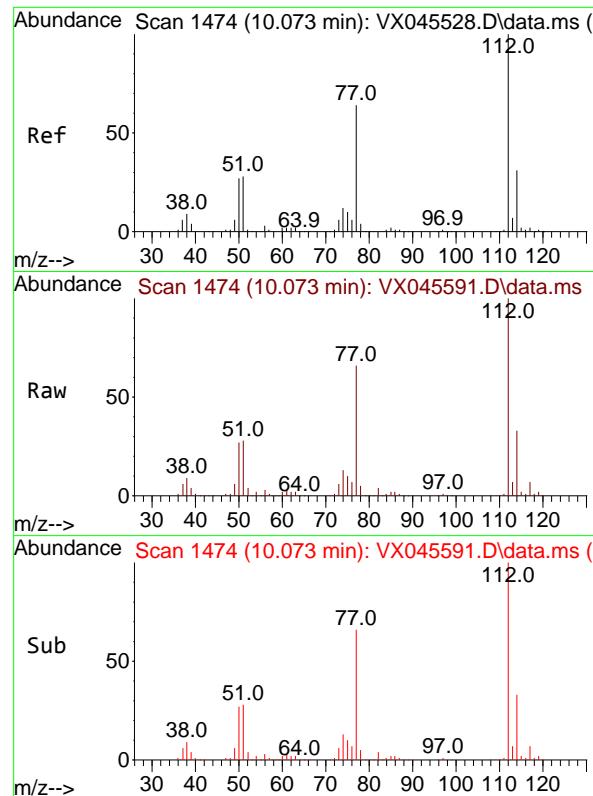


#65  
Chlorobenzene  
Concen: 49.720 ug/l  
RT: 10.073 min Scan# 1474  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS


### Manual Integrations APPROVED




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

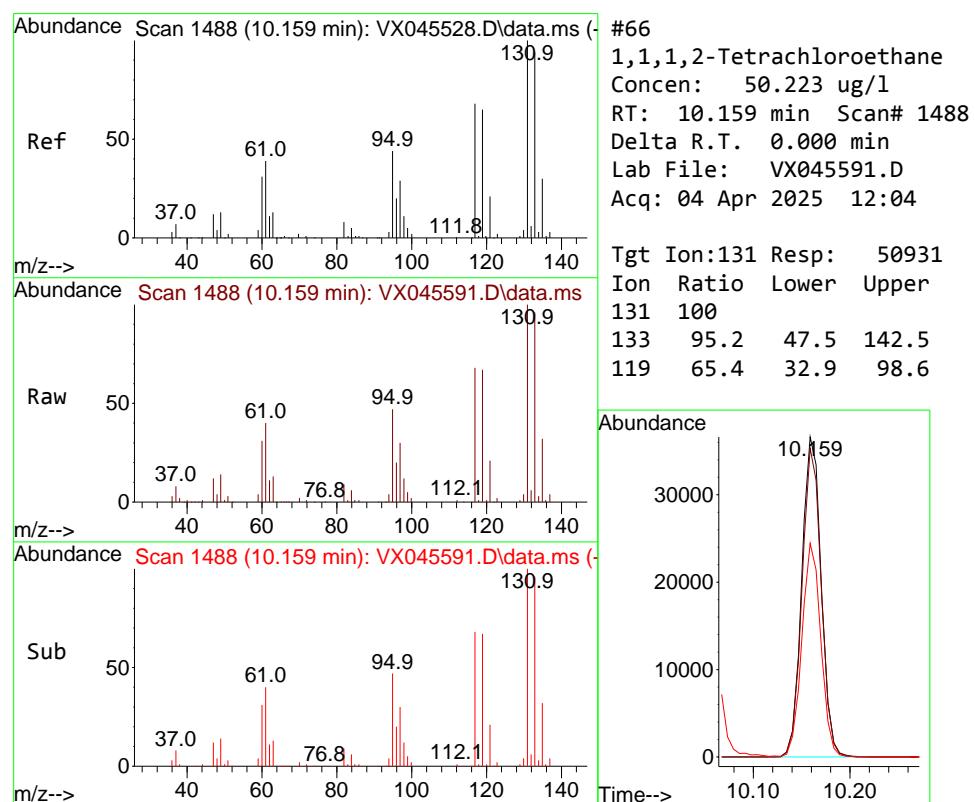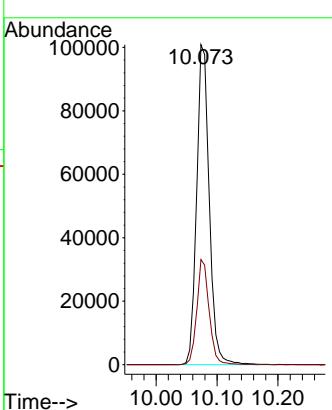

#66  
1,1,1,2-Tetrachloroethane  
Concen: 50.223 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion:131 Resp: 50931  
Ion Ratio Lower Upper  
131 100  
133 95.2 47.5 142.5  
119 65.4 32.9 98.6

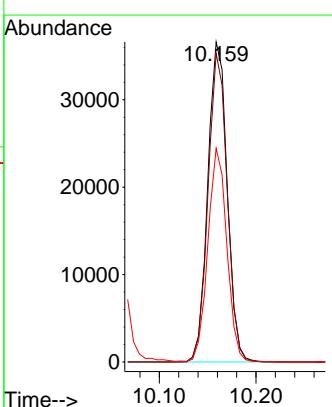



#67

Ethyl Benzene

Concen: 50.652 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min




Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS  
 Tgt Ion: 91 Resp: 264981  
 Ion Ratio Lower Upper  
 91 100  
 106 29.4 23.7 35.5

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025



#68

m/p-Xylenes

Concen: 101.535 ug/l


RT: 10.299 min Scan# 1511




Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 106 Resp: 193193  
 Ion Ratio Lower Upper  
 106 100  
 91 215.8 172.6 258.8

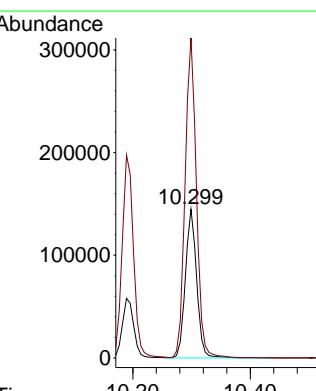




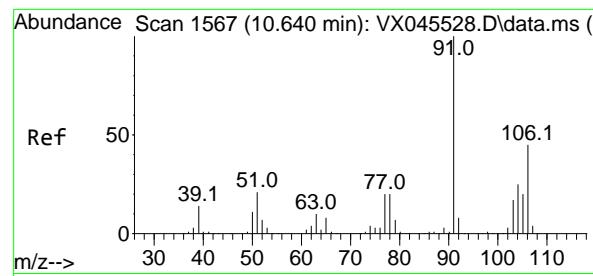


#69  
o-Xylene  
Concen: 51.166 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04  
ClientSampleId : MW-18B-56-040225MS

Tgt Ion:106 Resp: 9590  
Ion Ratio Lower Upper  
106 100  
91 230.0 113.6 340.6


### Manual Integrations APPROVED




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025



#70  
Styrene  
Concen: 52.762 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion:104 Resp: 163226  
Ion Ratio Lower Upper  
104 100  
78 57.1 45.4 68.2  
103 56.0 43.8 65.8





#71





Bromoform  
Concen: 53.418 ug/l

RT: 10.799 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument: MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS

### Manual Integrations APPROVED


Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

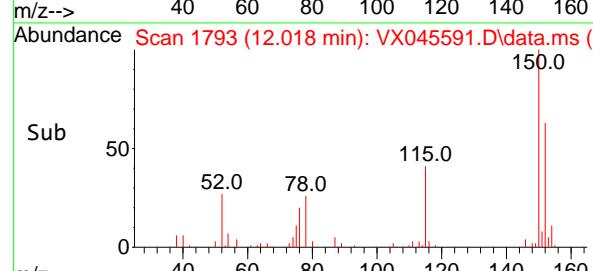


#72

1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion:152 Resp: 64924  
Ion Ratio Lower Upper  
152 100  
115 93.0 46.9 140.7  
150 174.8 0.0 349.4



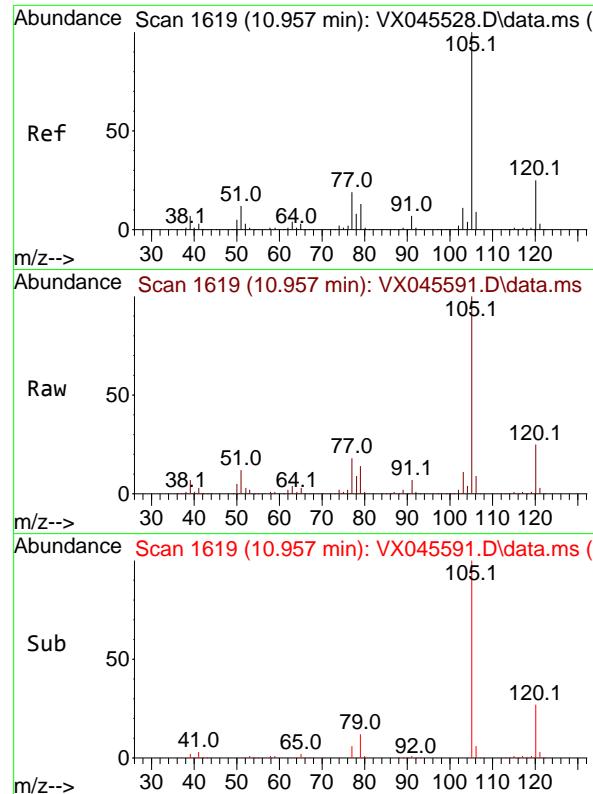

#73

Isopropylbenzene

Concen: 48.431 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min



Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

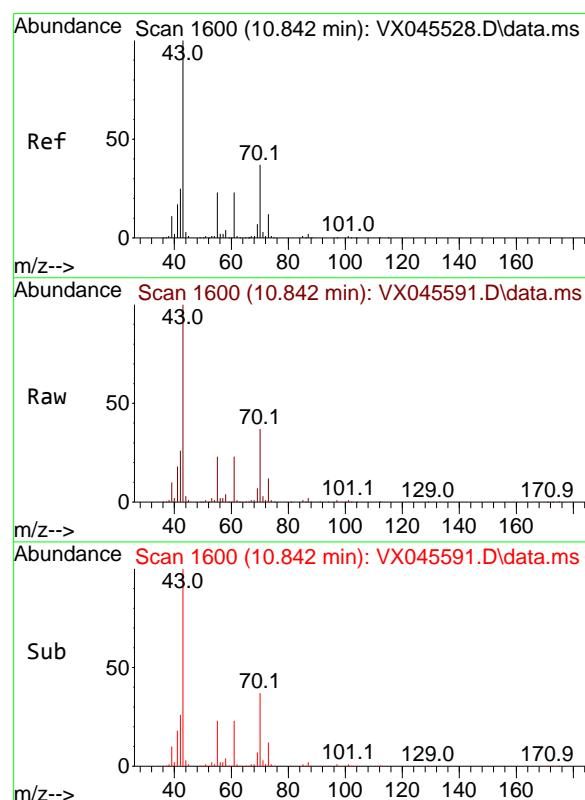

#74

N-amyl acetate

Concen: 52.306 ug/l


RT: 10.842 min Scan# 1600




Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion: 43 Resp: 130118  
Ion Ratio Lower Upper  
43 100  
70 37.3 30.1 45.1  
55 23.7 18.3 27.5  
61 21.7 17.5 26.3




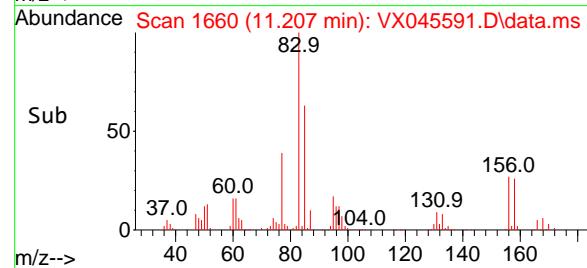
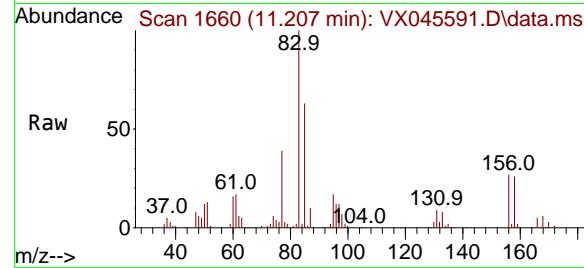
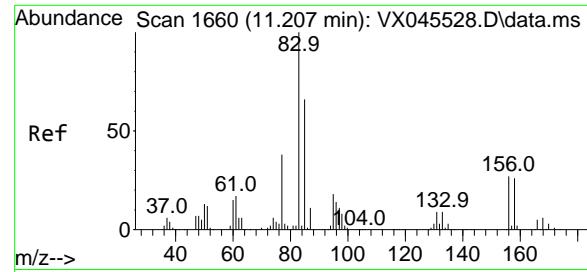


#75  
1,1,2,2-Tetrachloroethane  
Concen: 48.819 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

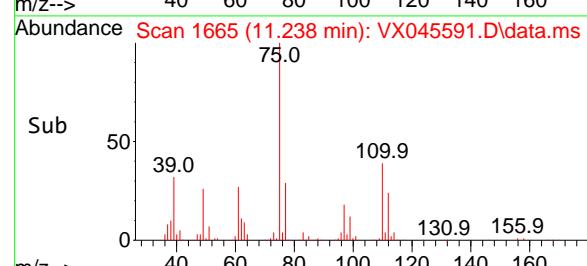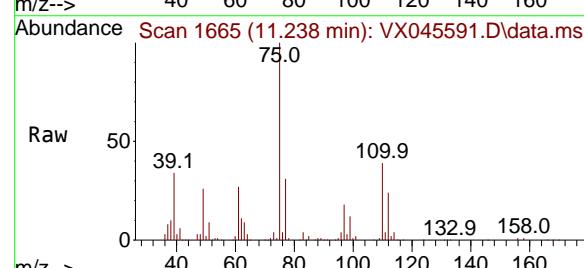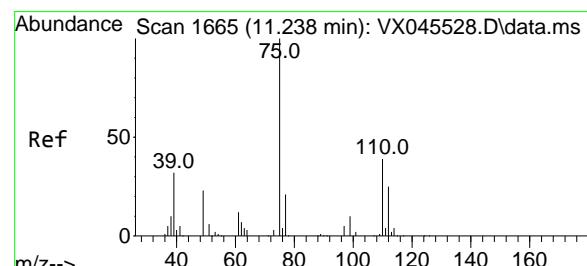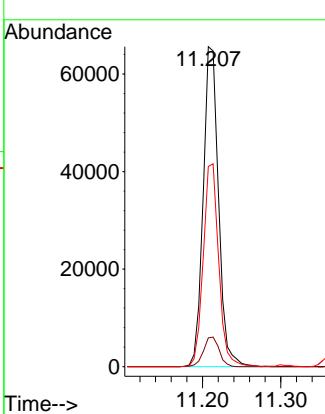

#76  
1,2,3-Trichloropropane  
Concen: 48.466 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion: 75 Resp: 76754  
Ion Ratio Lower Upper  
75 100  
77 40.0 20.0 59.9

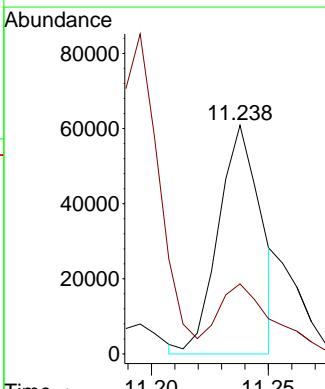



#77

Bromobenzene

Concen: 48.251 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X





ClientSampleId :

MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025



#78

n-propylbenzene

Concen: 49.387 ug/l


RT: 11.305 min Scan# 1676




Delta R.T. 0.006 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt	Ion:	91	Resp:	295835
Ion	Ratio	Lower	Upper	
91	100			
120	21.5	10.8	32.3	



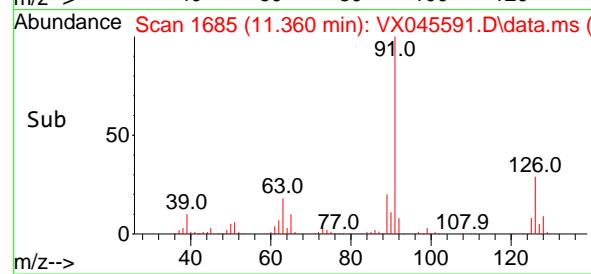

#79

2-Chlorotoluene

Concen: 48.369 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X




ClientSampleId :

MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 04/07/2025

Supervised By :Mahesh Dadoda 04/07/2025

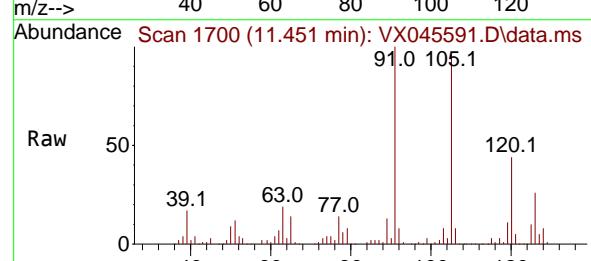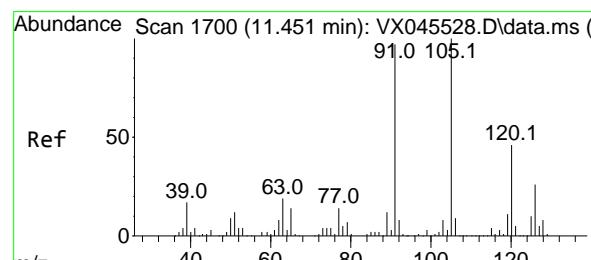

#80

1,3,5-Trimethylbenzene

Concen: 49.619 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04


Tgt Ion:105 Resp: 213377

Ion Ratio Lower Upper

105 100

120 46.0 23.0 69.0

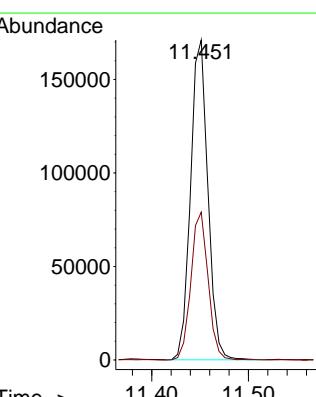


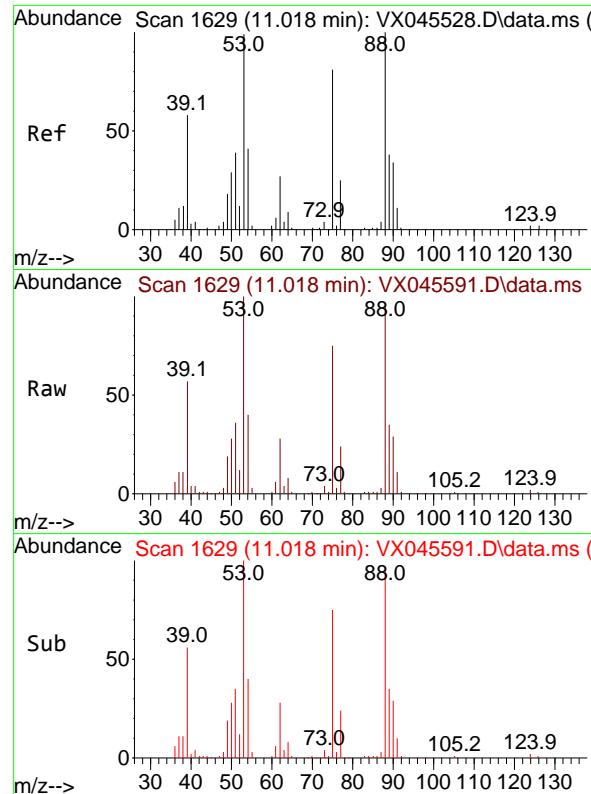


#81  
trans-1,4-Dichloro-2-butene  
Concen: 49.201 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS


### Manual Integrations APPROVED




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

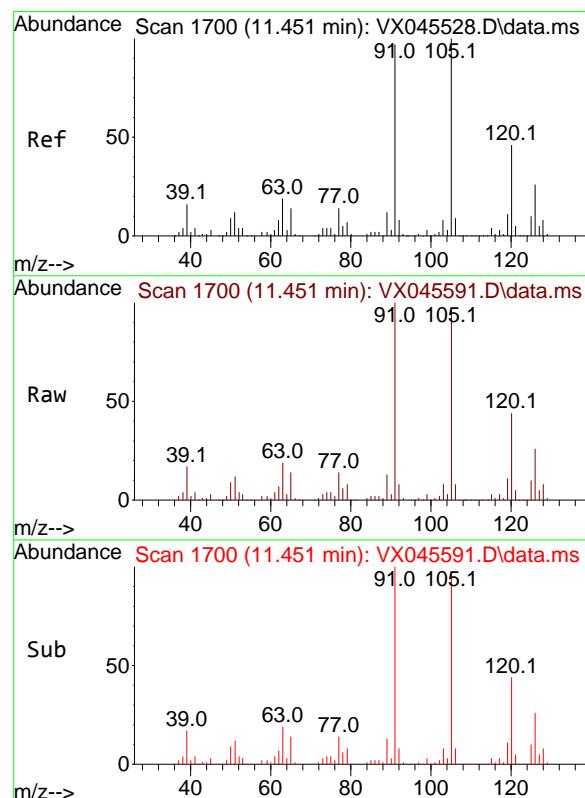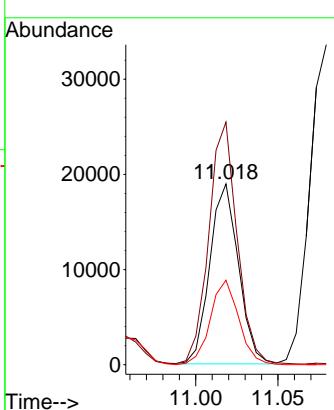

#82  
4-Chlorotoluene  
Concen: 49.723 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion: 91 Resp: 212300  
Ion Ratio Lower Upper  
91 100  
126 26.6 13.3 39.9

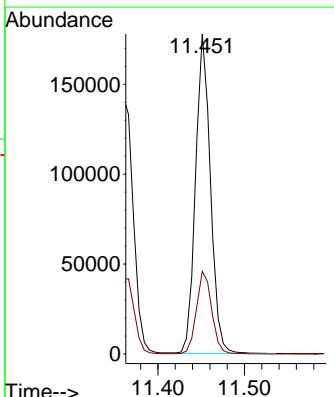



#83

tert-Butylbenzene

Concen: 49.658 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min




Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS  
 Acq Date : 04 Apr 2025 12:04  
 Acq Time : 11:04:00 AM  
 Scan Type : Full Scan  
 Scan Range : 40 - 200  
 Scan Step : 1.0000000000000002  
 Scan Width : 0.0000000000000002  
 Scan Speed : 1000000.0000000002  
 Scan Rate : 1000000.0000000002  
 Scan Mode : Normal  
 Scan Order : 1  
 Scan Number : 1  
 Scan Type : Full Scan  
 Scan Range : 40 - 200  
 Scan Step : 1.0000000000000002  
 Scan Width : 0.0000000000000002  
 Scan Speed : 1000000.0000000002  
 Scan Rate : 1000000.0000000002  
 Scan Mode : Normal  
 Scan Order : 1  
 Scan Number : 1

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025



#84

1,2,4-Trimethylbenzene

Concen: 49.627 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045591.D


Acq: 04 Apr 2025 12:04




Tgt Ion:105 Resp: 214201

Ion Ratio Lower Upper

105 100

120 43.4 21.4 64.3

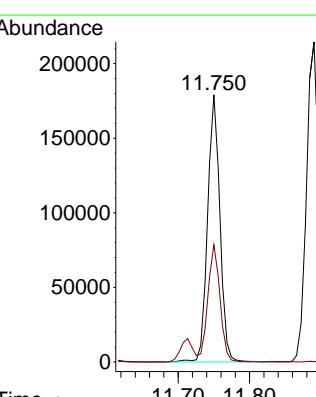



#85

sec-Butylbenzene

Concen: 50.337 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045591.D




Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X

ClientSampleId :

MW-18B-56-040225MS

**Manual Integrations  
APPROVED**

 Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025


#86

p-Isopropyltoluene

Concen: 50.074 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min


Lab File: VX045591.D


Acq: 04 Apr 2025 12:04

Tgt Ion:119 Resp: 215878

Ion Ratio Lower Upper

119	100		
134	25.0	12.6	37.8
91	27.5	13.7	41.1

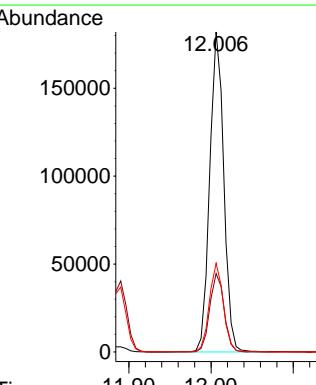

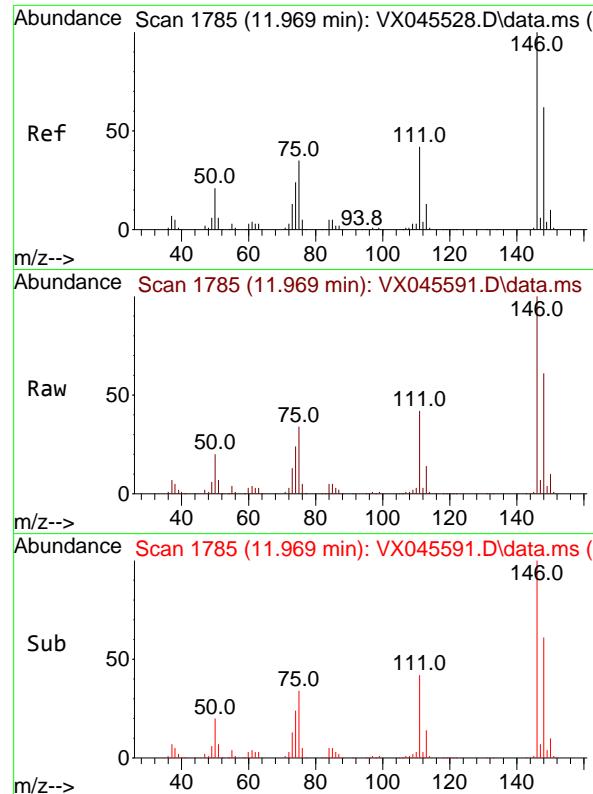

#87

1,3-Dichlorobenzene

Concen: 48.200 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min



Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

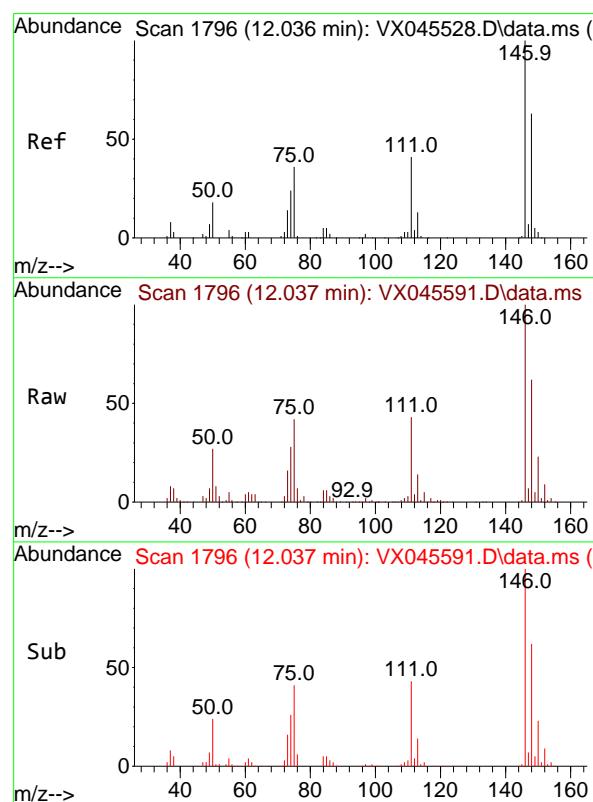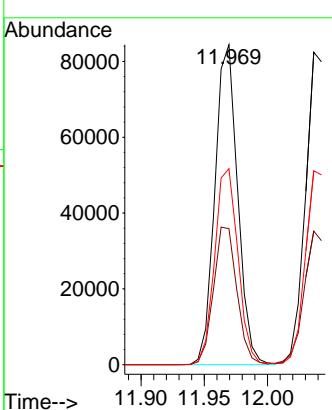

#88

1,4-Dichlorobenzene

Concen: 48.117 ug/l


RT: 12.037 min Scan# 1796




Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion:146 Resp: 106695  
 Ion Ratio Lower Upper  
 146 100  
 111 42.9 20.9 62.8  
 148 62.8 31.5 94.5

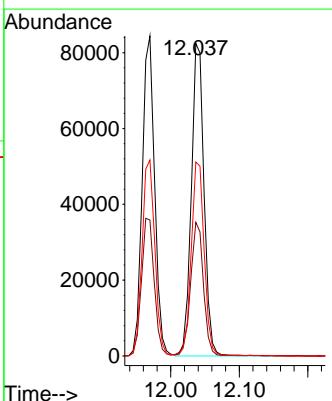



#89

n-Butylbenzene

Concen: 51.887 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min





Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS  
 Acq Date : 04/04/2025 12:04:00  
 Data File : VX045591.D

### Manual Integrations APPROVED

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

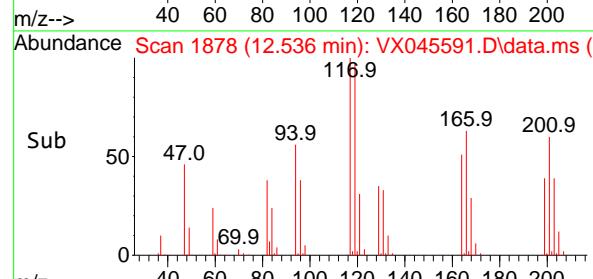

#90

Hexachloroethane

Concen: 51.044 ug/l


RT: 12.536 min Scan# 1878




Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion:117 Resp: 37819  
 Ion Ratio Lower Upper  
 117 100  
 201 61.8 31.2 93.6





#91

1,2-Dichlorobenzene

Concen: 48.446 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04




Instrument : MSVOA\_X

ClientSampleId : MW-18B-56-040225MS

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 04/07/2025


Supervised By :Mahesh Dadoda 04/07/2025



#92  
1,2-Dibromo-3-Chloropropane  
Concen: 53.397 ug/l  
RT: 12.939 min Scan# 1944  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion: 75 Resp: 20401  
Ion Ratio Lower Upper  
75 100  
155 69.1 34.9 104.7  
157 87.4 44.9 134.7




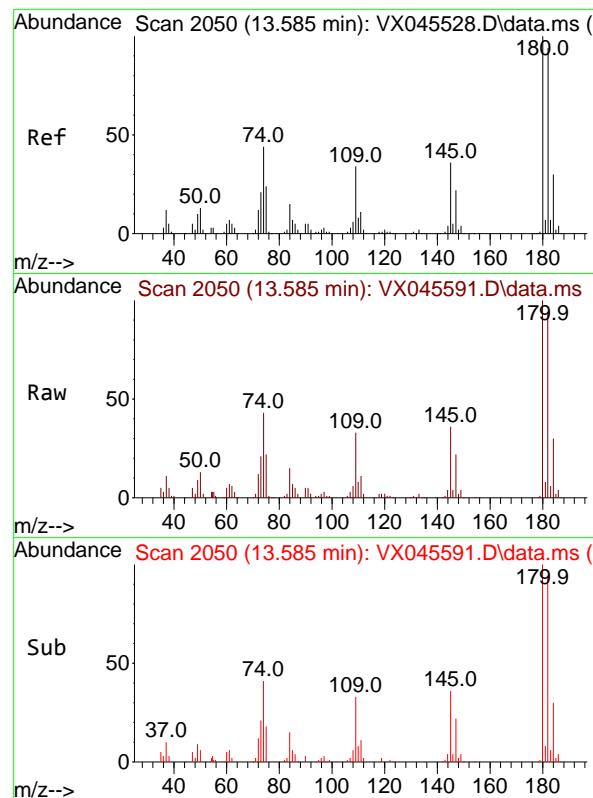


#93  
1,2,4-Trichlorobenzene  
Concen: 49.234 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MS


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 04/07/2025  
Supervised By :Mahesh Dadoda 04/07/2025

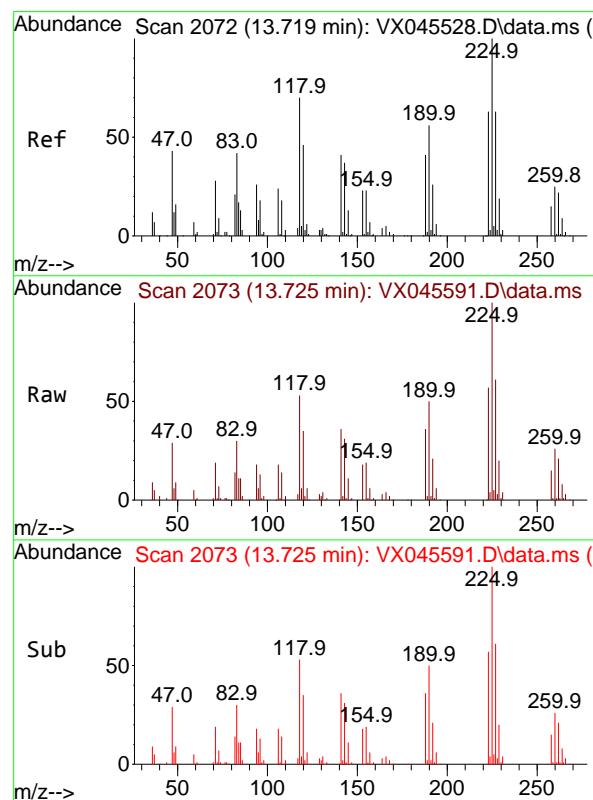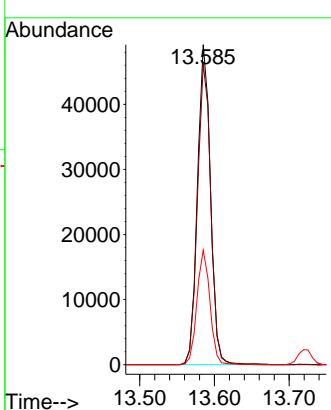

#94  
Hexachlorobutadiene  
Concen: 48.691 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. 0.006 min  
Lab File: VX045591.D  
Acq: 04 Apr 2025 12:04

Tgt Ion:225 Resp: 25397  
Ion Ratio Lower Upper  
225 100  
223 61.9 31.1 93.3  
227 61.3 32.2 96.6

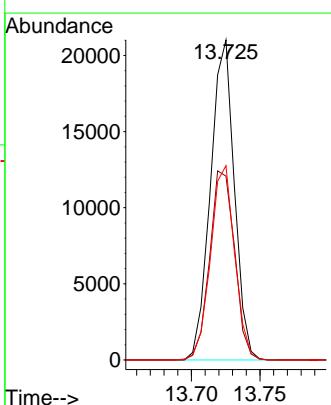

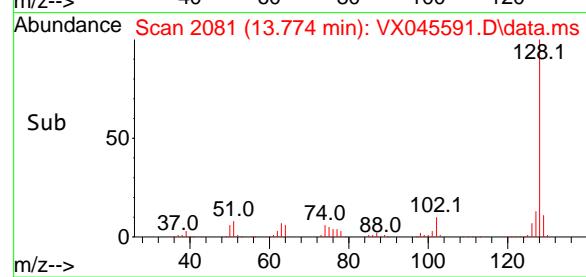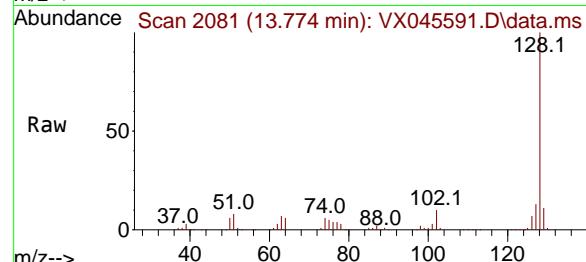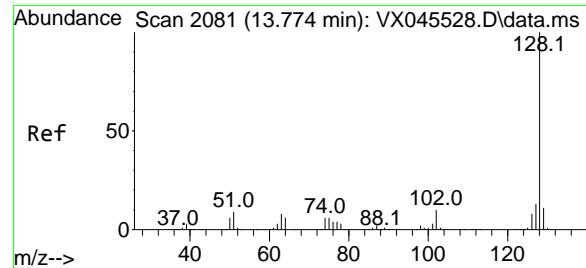

#95

Naphthalene

Concen: 50.831 ug/l

RT: 13.774 min Scan# 2081





Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MS  
 Manual Integrations  
**APPROVED**

Reviewed By :John Carlone 04/07/2025  
 Supervised By :Mahesh Dadoda 04/07/2025

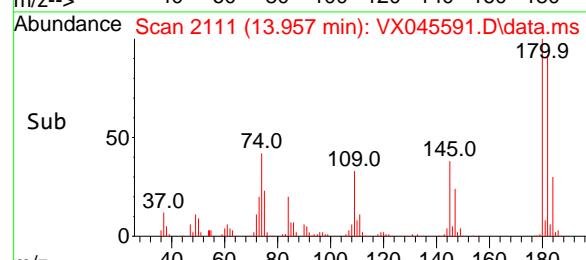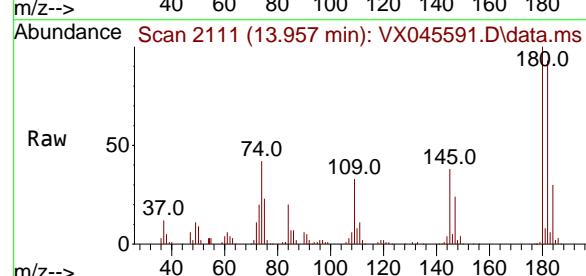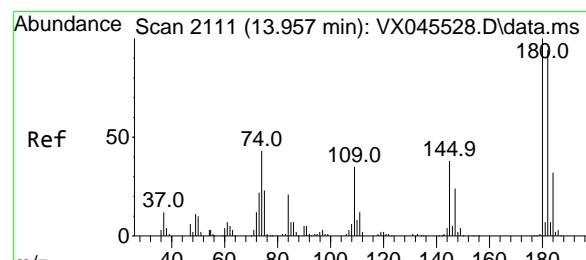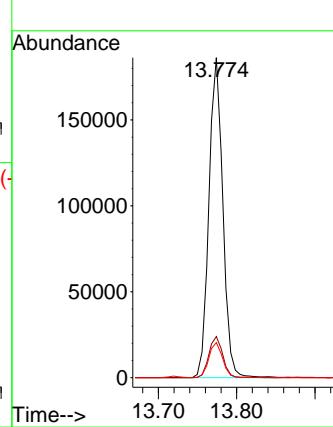

#96

1,2,3-Trichlorobenzene

Concen: 49.248 ug/l


RT: 13.957 min Scan# 2111

Delta R.T. 0.000 min

Lab File: VX045591.D

Acq: 04 Apr 2025 12:04

Tgt Ion:180 Resp: 62422  
 Ion Ratio Lower Upper  
 180 100  
 182 95.6 47.3 141.8  
 145 36.7 18.2 54.6

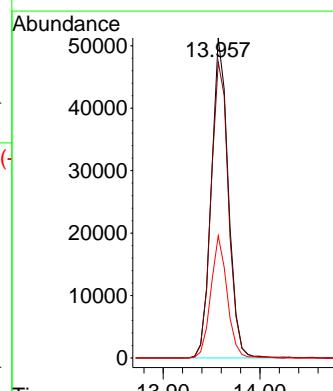



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	04/02/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	04/02/25	
Client Sample ID:	MW-18B-56-040225MSD			SDG No.:	Q1711	
Lab Sample ID:	Q1711-03MSD			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045577.D	10		04/03/25 17:33	VX040325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	480	2.60		10.0	ug/L
75-35-4	1,1-Dichloroethene	430	2.30		10.0	ug/L
75-34-3	1,1-Dichloroethane	420	2.30		10.0	ug/L
156-59-2	cis-1,2-Dichloroethene	1100	1.90		10.0	ug/L
71-55-6	1,1,1-Trichloroethane	420	2.00		10.0	ug/L
71-43-2	Benzene	420	1.50		10.0	ug/L
107-06-2	1,2-Dichloroethane	430	2.20		10.0	ug/L
79-01-6	Trichloroethene	740	0.93		10.0	ug/L
79-00-5	1,1,2-Trichloroethane	430	2.10		10.0	ug/L
127-18-4	Tetrachloroethene	400	2.30		10.0	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	46.9		70 (74) - 130 (125)	94%	SPK: 50
1868-53-7	Dibromofluoromethane	44.8		70 (75) - 130 (124)	90%	SPK: 50
2037-26-5	Toluene-d8	44.8		70 (86) - 130 (113)	90%	SPK: 50
460-00-4	4-Bromofluorobenzene	46.0		70 (77) - 130 (121)	92%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	69200	5.55			
540-36-3	1,4-Difluorobenzene	124000	6.757			
3114-55-4	Chlorobenzene-d5	109000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	51000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045577.D  
 Acq On : 03 Apr 2025 17:33  
 Operator : JC/MD  
 Sample : Q1711-03MSD 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-18B-56-040225MSD

Quant Time: Apr 04 01:26:51 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	69182	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	124452	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	109108	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	51026	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	59319	46.887	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	93.780%		
35) Dibromofluoromethane	5.385	113	39562	44.805	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.600%		
50) Toluene-d8	8.647	98	138195	44.840	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	89.680%		
62) 4-Bromofluorobenzene	11.079	95	51613	45.976	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	91.960%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	47385	45.800	ug/l	98
3) Chloromethane	1.307	50	48184	45.333	ug/l	99
4) Vinyl Chloride	1.374	62	46952	48.269	ug/l	99
5) Bromomethane	1.593	94	19170	41.564	ug/l	99
6) Chloroethane	1.660	64	22694	43.974	ug/l	100
7) Trichlorofluoromethane	1.874	101	62192	42.876	ug/l	98
8) Diethyl Ether	2.136	74	20167	41.412	ug/l	95
9) 1,1,2-Trichlorotrifluo...	2.319	101	36175	42.560	ug/l	97
10) Methyl Iodide	2.441	142	46035	43.422	ug/l	100
11) Tert butyl alcohol	2.989	59	33642	197.862	ug/l	100
12) 1,1-Dichloroethene	2.306	96	35734	43.026	ug/l	97
13) Acrolein	2.233	56	56800	242.590	ug/l	99
14) Allyl chloride	2.660	41	67571	42.879	ug/l	99
15) Acrylonitrile	3.062	53	118586	220.948	ug/l	99
16) Acetone	2.386	43	113493	218.462	ug/l	98
17) Carbon Disulfide	2.502	76	83677	40.793	ug/l	99
18) Methyl Acetate	2.703	43	51227	42.828	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	118298	40.718	ug/l	97
20) Methylene Chloride	2.782	84	41717	42.893	ug/l	96
21) trans-1,2-Dichloroethene	3.087	96	35999	42.427	ug/l	99
22) Diisopropyl ether	3.757	45	126501	40.752	ug/l #	83
23) Vinyl Acetate	3.721	43	579979	216.251	ug/l	100
24) 1,1-Dichloroethane	3.605	63	73743	42.006	ug/l	98
25) 2-Butanone	4.556	43	166641	219.133	ug/l	99
26) 2,2-Dichloropropane	4.465	77	47107	41.532	ug/l	87
27) cis-1,2-Dichloroethene	4.483	96	113129	109.437	ug/l	94
28) Bromochloromethane	4.891	49	44030	51.901	ug/l	100
29) Tetrahydrofuran	5.007	42	110855	224.845	ug/l	99
30) Chloroform	5.086	83	76188	42.177	ug/l	98
31) Cyclohexane	5.464	56	63718	41.056	ug/l	98
32) 1,1,1-Trichloroethane	5.373	97	63504	41.547	ug/l	99
36) 1,1-Dichloropropene	5.684	75	48513	40.692	ug/l	98
37) Ethyl Acetate	4.715	43	61701	41.067	ug/l	99
38) Carbon Tetrachloride	5.672	117	52678	40.884	ug/l	97
39) Methylcyclohexane	7.379	83	60427	41.348	ug/l	96
40) Benzene	6.031	78	151773	41.683	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045577.D  
 Acq On : 03 Apr 2025 17:33  
 Operator : JC/MD  
 Sample : Q1711-03MSD 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 04 01:26:51 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-18B-56-040225MSD

**Manual Integrations**  
**APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	35246	44.462	ug/l	99
42) 1,2-Dichloroethane	6.080	62	64394	42.819	ug/l	99
43) Isopropyl Acetate	6.342	43	93045	40.861	ug/l	100
44) Trichloroethene	7.123	130	64230	74.217	ug/l	98
45) 1,2-Dichloropropane	7.428	63	37608	41.396	ug/l	95
46) Dibromomethane	7.580	93	29576	42.409	ug/l	98
47) Bromodichloromethane	7.818	83	56518	40.580	ug/l	98
48) Methyl methacrylate	7.690	41	50434	42.896	ug/l	99
49) 1,4-Dioxane	7.659	88	18467	868.137	ug/l	96
51) 4-Methyl-2-Pentanone	8.574	43	327122	216.701	ug/l	99
52) Toluene	8.714	92	91494	41.527	ug/l	99
53) t-1,3-Dichloropropene	8.976	75	48435	36.797	ug/l	99
54) cis-1,3-Dichloropropene	8.366	75	53960	41.229	ug/l	99
55) 1,1,2-Trichloroethane	9.147	97	37650	42.883	ug/l	96
56) Ethyl methacrylate	9.116	69	57438	42.272	ug/l	99
57) 1,3-Dichloropropane	9.305	76	65336	42.735	ug/l	99
59) 2-Hexanone	9.427	43	244980	219.150	ug/l	100
60) Dibromochemicalmethane	9.519	129	40295	42.099	ug/l	99
61) 1,2-Dibromoethane	9.610	107	38304	43.098	ug/l	97
64) Tetrachloroethene	9.269	164	30936	40.159	ug/l	99
65) Chlorobenzene	10.079	112	97984	42.027	ug/l	98
66) 1,1,1,2-Tetrachloroethane	10.159	131	33130	40.930	ug/l	99
67) Ethyl Benzene	10.189	91	174928	41.892	ug/l	99
68) m/p-Xylenes	10.299	106	129635	85.358	ug/l	99
69) o-Xylene	10.640	106	62955	42.080	ug/l	97
70) Styrene	10.653	104	107687	43.611	ug/l	99
71) Bromoform	10.799	173	24522	40.574	ug/l #	95
73) Isopropylbenzene	10.957	105	167230	40.915	ug/l	100
74) N-amyl acetate	10.842	43	79786	40.809	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	58476	40.727	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	49248m	39.568	ug/l	
77) Bromobenzene	11.195	156	39023	41.322	ug/l	97
78) n-propylbenzene	11.305	91	194389	41.291	ug/l	100
79) 2-Chlorotoluene	11.360	91	122025	40.544	ug/l	100
80) 1,3,5-Trimethylbenzene	11.451	105	138429	40.958	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.018	75	13535	36.907	ug/l	90
82) 4-Chlorotoluene	11.451	91	140486	41.866	ug/l	99
83) tert-Butylbenzene	11.713	119	135774	40.577	ug/l	98
84) 1,2,4-Trimethylbenzene	11.750	105	140947	41.550	ug/l	99
85) sec-Butylbenzene	11.890	105	169765	41.307	ug/l	100
86) p-Isopropyltoluene	12.006	119	138266	40.807	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	68253	39.704	ug/l	99
88) 1,4-Dichlorobenzene	12.036	146	68792	39.473	ug/l	98
89) n-Butylbenzene	12.329	91	123161	41.918	ug/l	99
90) Hexachloroethane	12.536	117	23387	40.163	ug/l	98
91) 1,2-Dichlorobenzene	12.335	146	70002	40.959	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	12616	42.015	ug/l	98
93) 1,2,4-Trichlorobenzene	13.585	180	37705	39.634	ug/l	98
94) Hexachlorobutadiene	13.725	225	15843	38.647	ug/l	96
95) Naphthalene	13.774	128	144479	40.810	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	40388	40.543	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
 Data File : VX045577.D  
 Acq On : 03 Apr 2025 17:33  
 Operator : JC/MD  
 Sample : Q1711-03MSD 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 20 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**MW-18B-56-040225MSD**

**Manual Integrations**  
**APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

Quant Time: Apr 04 01:26:51 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Apr 02 03:11:43 2025  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
(#)	= qualifier out of range	(m)	= manual integration	(+)	= signals summed	


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040325\  
Data File : VX045577.D  
Acq On : 03 Apr 2025 17:33  
Operator : JC/MD  
Sample : Q1711-03MSD 10X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1




Quant Time: Apr 04 01:26:51 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260  
QLast Update : Wed Apr 02 03:11:43 2025  
Response via : Initial Calibration

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
MW-18B-56-040225MSD

## Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

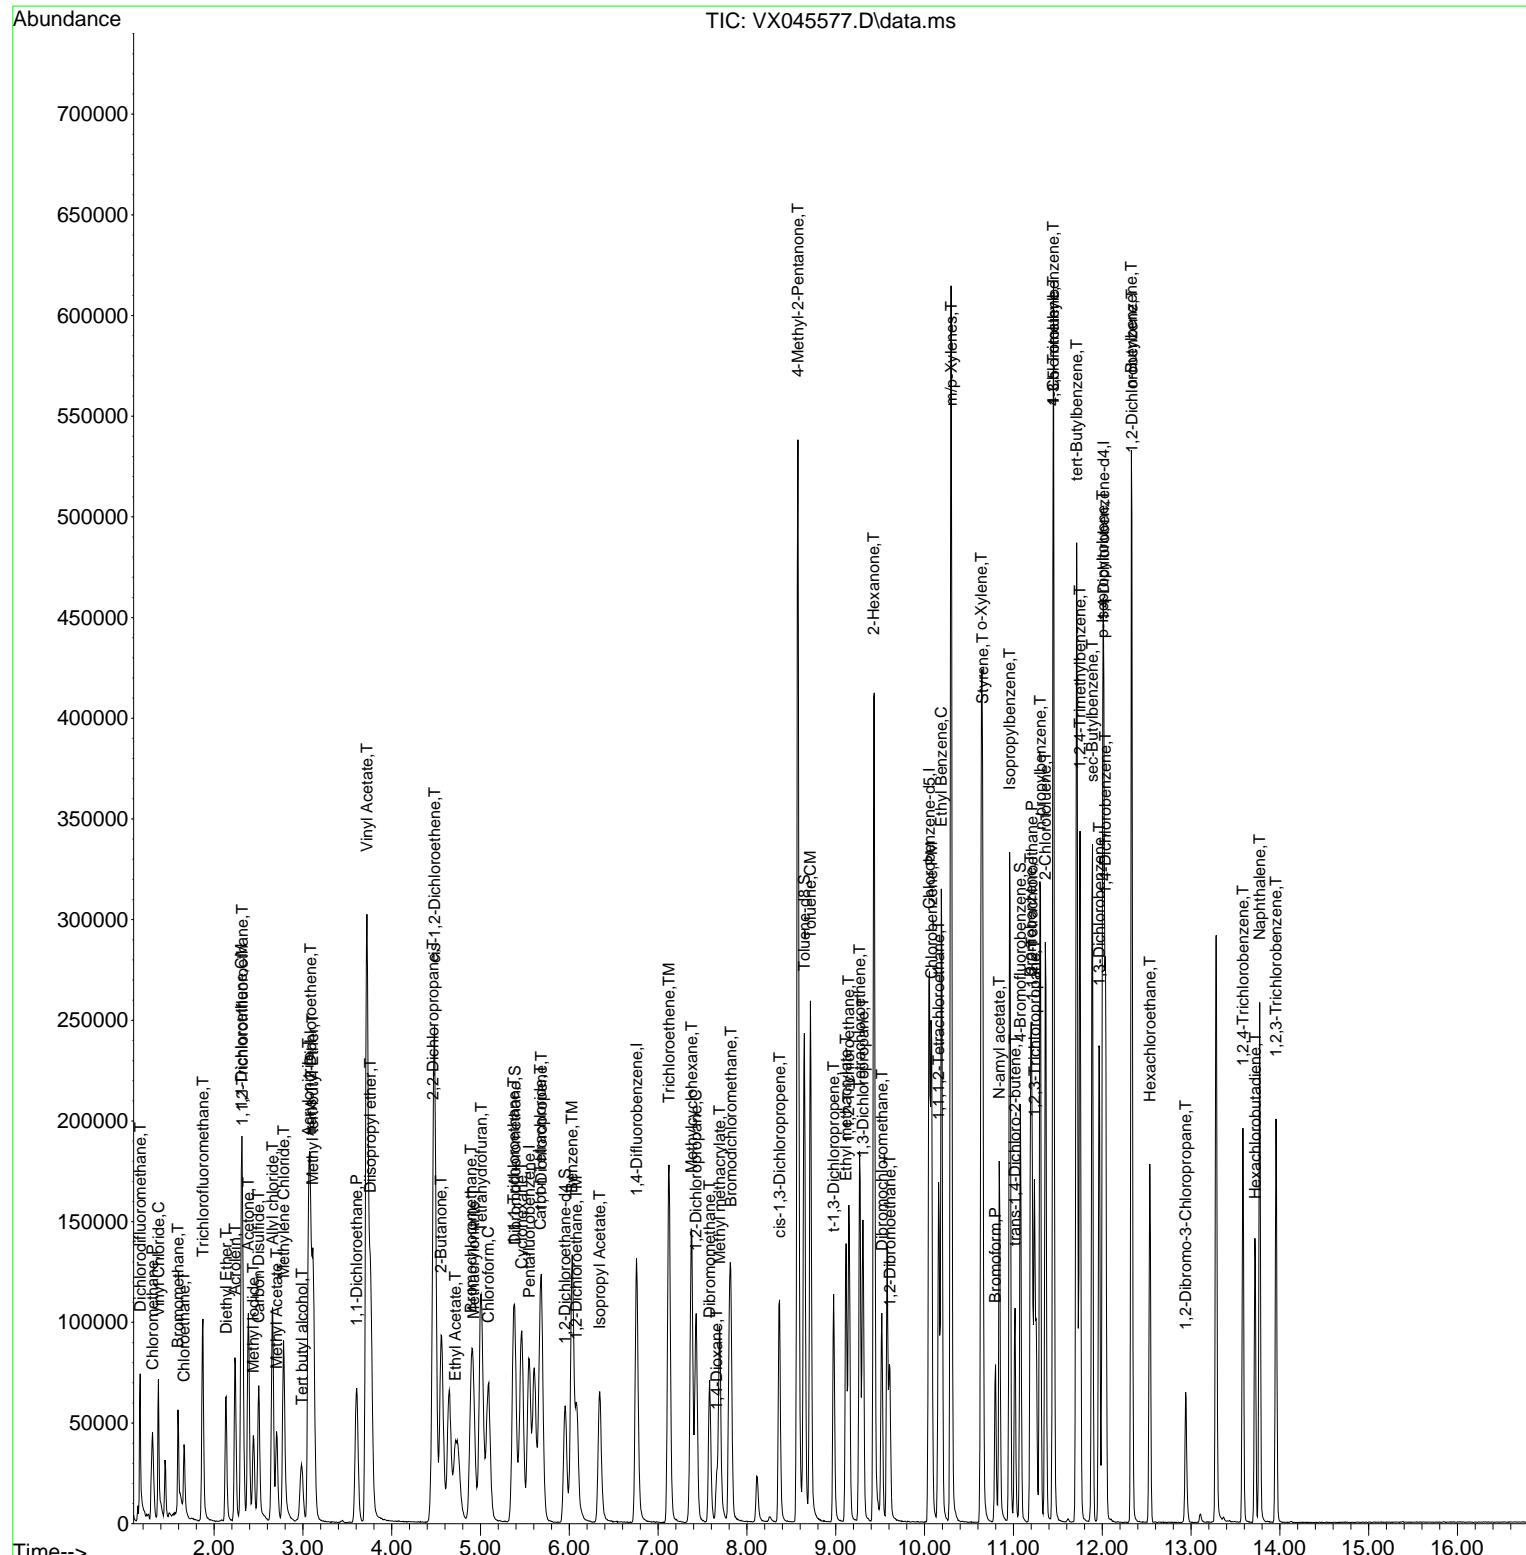







#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 72  
Delta R.T. -0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD


### Manual Integrations APPROVED


Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025




#2  
Dichlorodifluoromethane  
Concen: 45.800 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion: 85 Resp: 47385  
Ion Ratio Lower Upper  
85 100  
87 33.4 16.1 48.2

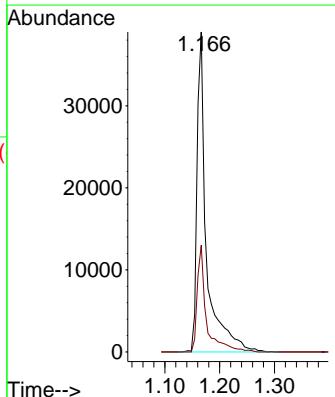

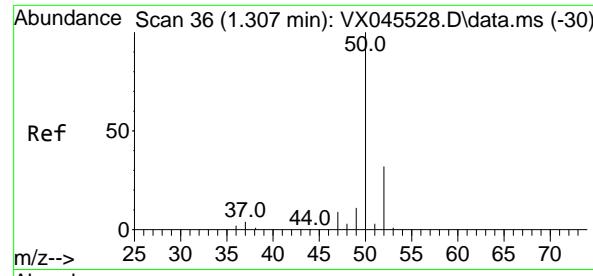

Abundance Scan 36 (1.307 min): VX045577.D\data.ms

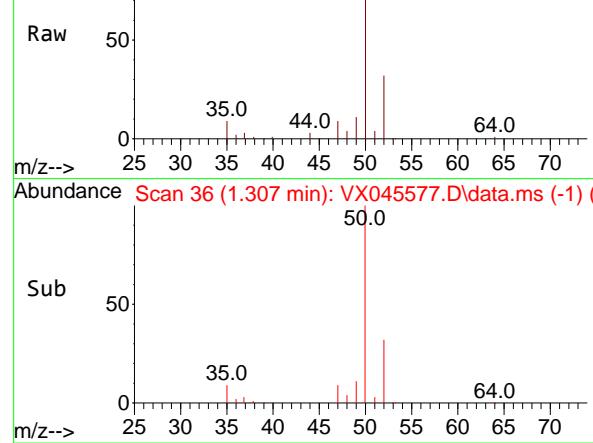

Abundance Scan 36 (1.307 min): VX045577.D\data.ms (-1) (



#3  
Chloromethane  
Concen: 45.333 ug/l  
RT: 1.307 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD


Tgt Ion: 50 Resp: 48184  
Ion Ratio Lower Upper  
50 100  
52 32.1 25.9 38.9

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

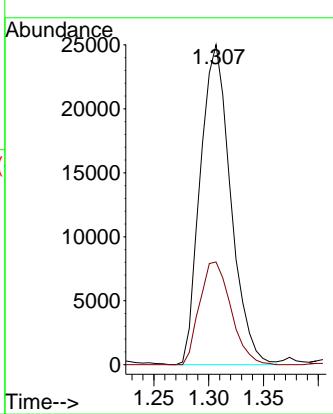


Abundance Scan 47 (1.374 min): VX045577.D\data.ms



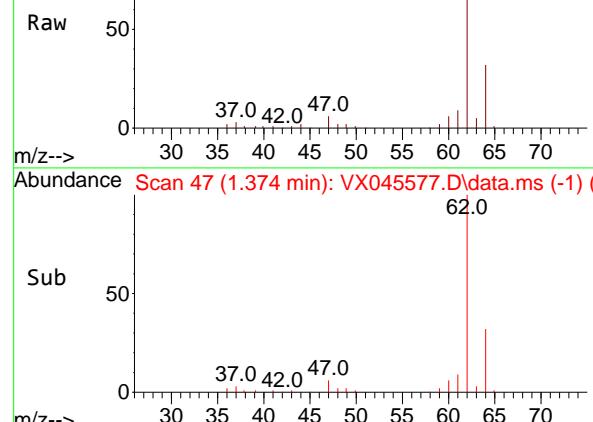


Abundance Scan 47 (1.374 min): VX045577.D\data.ms (-1) (

#4  
Vinyl Chloride  
Concen: 48.269 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion: 62 Resp: 46952  
Ion Ratio Lower Upper  
62 100  
64 32.3 25.5 38.3





#5

Bromomethane

Concen: 41.564 ug/l

RT: 1.593 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33





Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#6

Chloroethane


Concen: 43.974 ug/l


RT: 1.660 min Scan# 94

Delta R.T. -0.006 min


Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

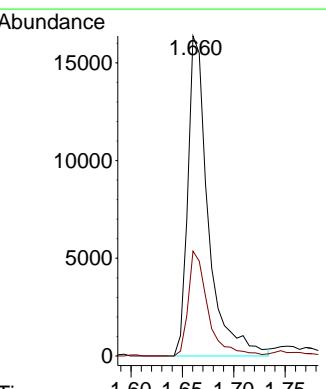 Tgt Ion: 64 Resp: 22694  
 Ion Ratio Lower Upper  
 64 100  
 66 32.8 26.3 39.5

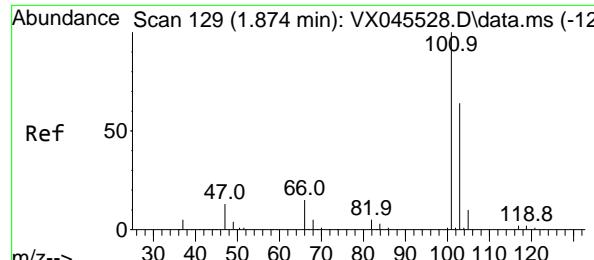



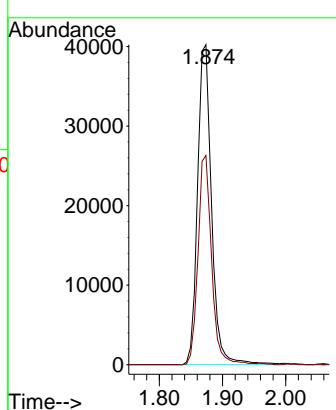
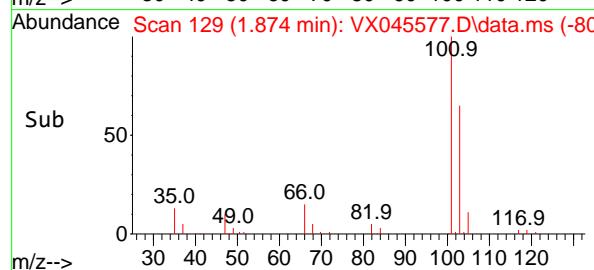
#7  
Trichlorofluoromethane  
Concen: 42.876 ug/l  
RT: 1.874 min Scan# 129  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33




Tgt Ion: 101 Resp: 62192  
Ion Ratio Lower Upper  
101 100  
103 65.3 51.1 76.7

### Manual Integrations APPROVED



Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025









#8  
Diethyl Ether  
Concen: 41.412 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33



Tgt Ion: 74 Resp: 20167  
Ion Ratio Lower Upper  
74 100  
45 101.3 53.0 159.1

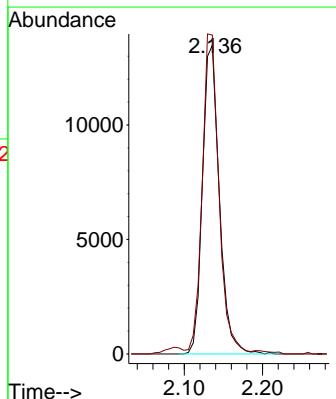

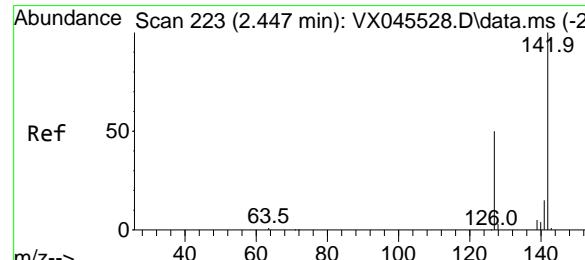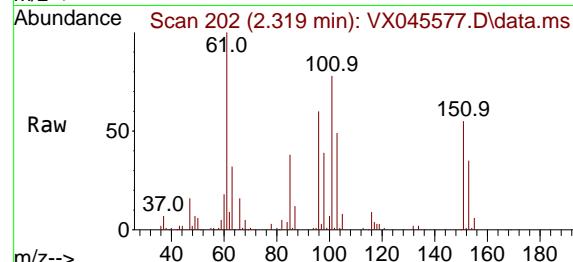

#9

1,1,2-Trichlorotrifluoroethane

Concen: 42.560 ug/l

RT: 2.319 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Instrument:

MSVOA\_X

ClientSampleId :


MW-18B-56-040225MSD


**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


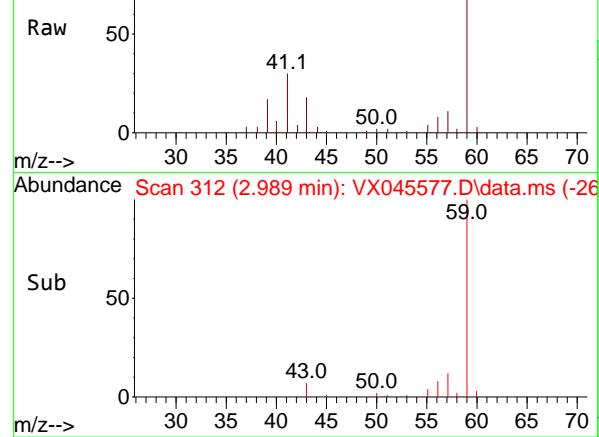
#10  
Methyl Iodide  
Concen: 43.422 ug/l  
RT: 2.441 min Scan# 222  
Delta R.T. -0.006 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion:142 Resp: 46035  
Ion Ratio Lower Upper  
142 100  
127 50.4 40.2 60.4  
141 14.1 11.7 17.5

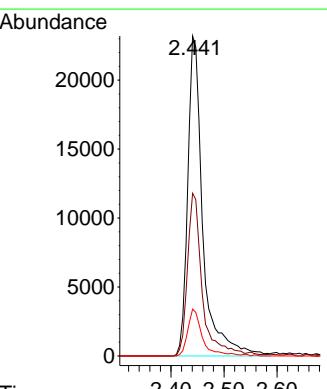




Abundance Scan 312 (2.989 min): VX045577.D\data.ms



Abundance Scan 312 (2.989 min): VX045577.D\data.ms (-26)

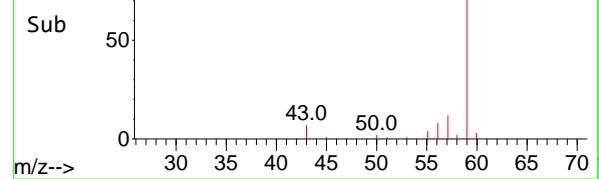

#11

Tert butyl alcohol

Concen: 197.862 ug/l

RT: 2.989 min Scan# 3

Delta R.T. 0.012 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33

Instrument:


MSVOA\_X

ClientSampleId :


MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**
Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

Abundance Scan 200 (2.306 min): VX045577.D\data.ms

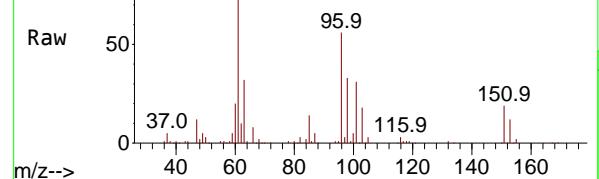

Abundance Scan 200 (2.306 min): VX045577.D\data.ms (-15)

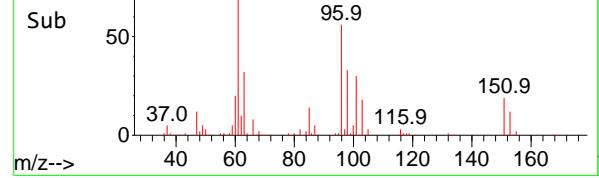

#12

1,1-Dichloroethene

Concen: 43.026 ug/l

RT: 2.306 min Scan# 200

Delta R.T. -0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Tgt Ion: 96 Resp: 35734


Ion Ratio Lower Upper

96 100

61 179.4 145.7 218.5

98 58.6 51.6 77.4

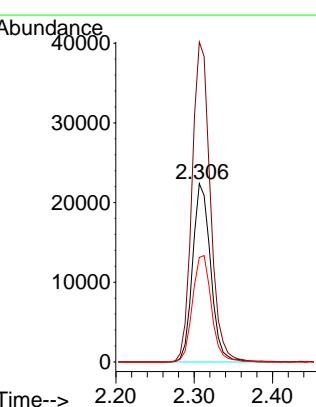

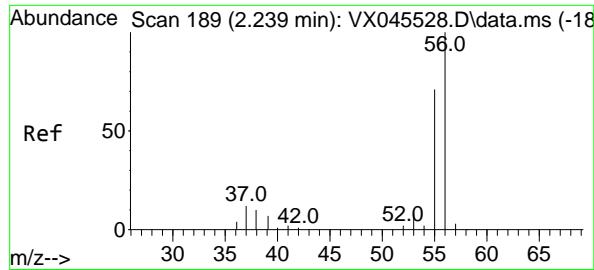

#13

Acrolein

Concen: 242.590 ug/l

RT: 2.233 min Scan# 1

Delta R.T. -0.006 min



Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument: MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

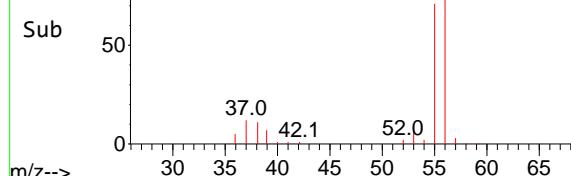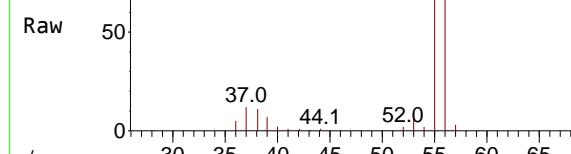

Tgt Ion: 56 Resp: 56800

Ion Ratio Lower Upper




56 100

55 71.4 56.2 84.2

**Manual Integrations****APPROVED**

Reviewed By :Semsettin Yesilyurt 04/04/2025

Supervised By :Mahesh Dadoda 04/04/2025

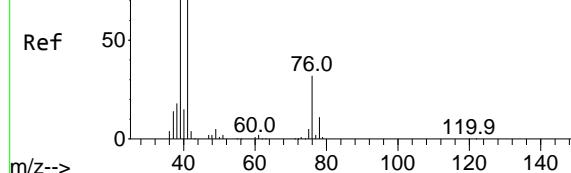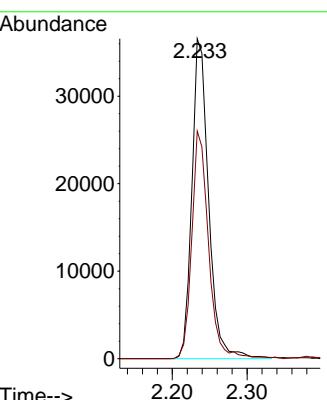

#14

Allyl chloride

Concen: 42.879 ug/l

RT: 2.660 min Scan# 258

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33




Tgt Ion: 41 Resp: 67571







Ion Ratio Lower Upper

41 100

39 74.7 60.2 90.2

76 30.2 24.6 36.8

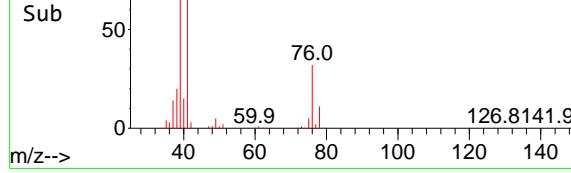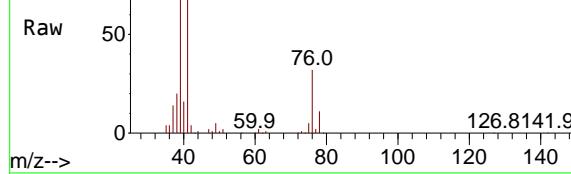

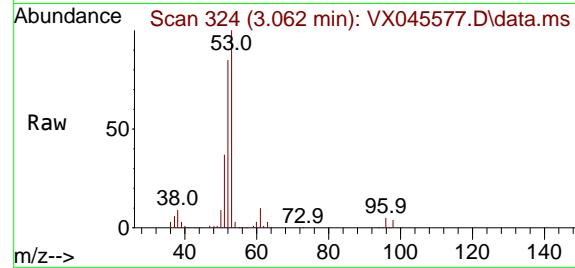

#15

Acrylonitrile

Concen: 220.948 ug/l

RT: 3.062 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument:


MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#16

Acetone

Concen: 218.462 ug/l


RT: 2.386 min Scan# 213


Delta R.T. 0.000 min

Lab File: VX045577.D



Acq: 03 Apr 2025 17:33

Tgt Ion: 43 Resp: 113493  
Ion Ratio Lower Upper  
43 100  
58 29.1 22.3 33.5


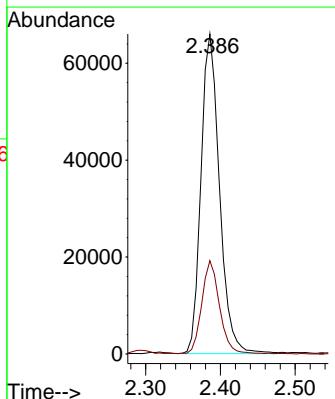




Abundance Scan 232 (2.502 min): VX045577.D\data.ms

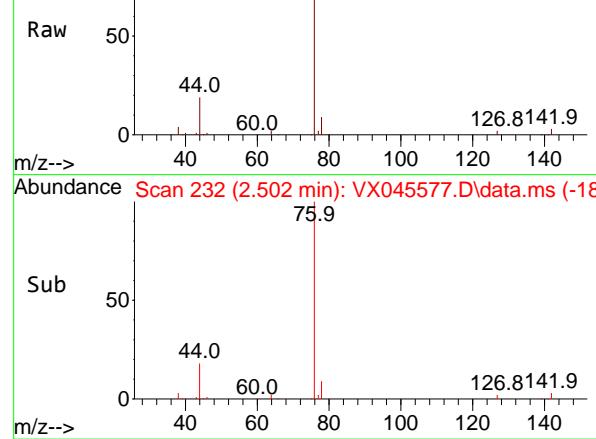

Abundance Scan 265 (2.703 min): VX045577.D\data.ms

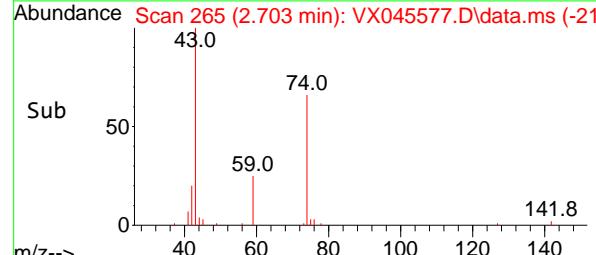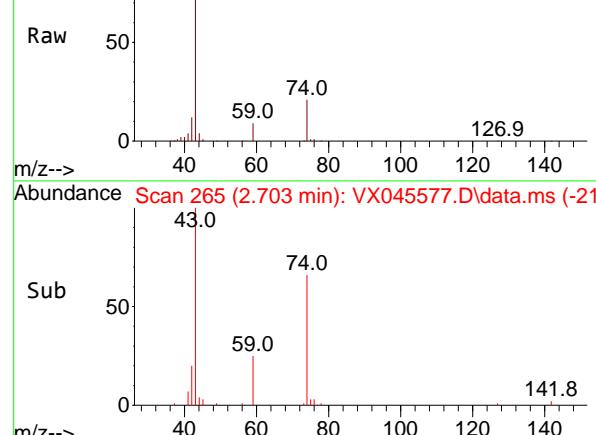

#17

Carbon Disulfide

Concen: 40.793 ug/l

RT: 2.502 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#18

Methyl Acetate

Concen: 42.828 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33







Tgt Ion: 43 Resp: 51227

Ion Ratio Lower Upper

43 100

74 21.5 17.5 26.3

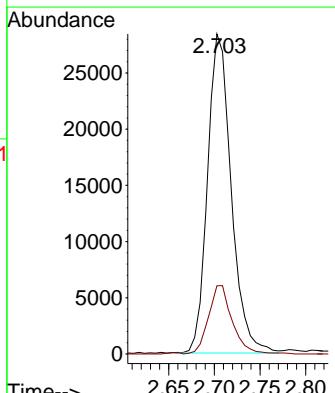



#19


Methyl tert-butyl Ether  
Concen: 40.718 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025


Tgt Ion: 73 Resp: 11829:  
Ion Ratio Lower Upper  
73 100  
57 23.6 17.6 26.4



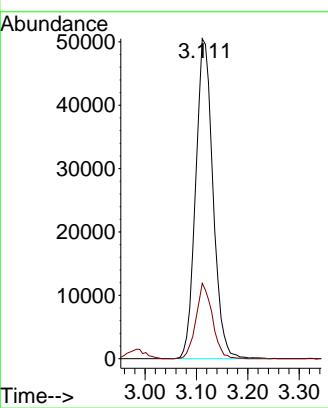


#20

Methylene Chloride  
Concen: 42.893 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion: 84 Resp: 41717:  
Ion Ratio Lower Upper  
84 100  
49 139.5 107.5 161.3  
51 44.0 33.0 49.6  
86 66.3 50.1 75.1

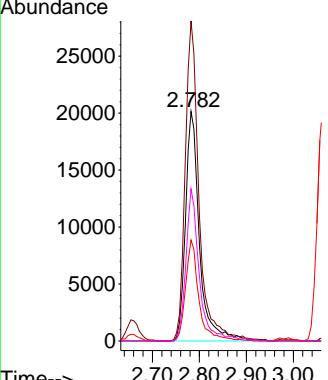



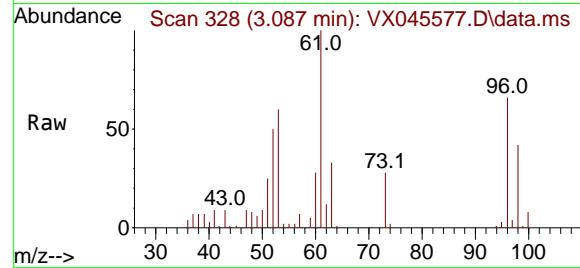



#21  
trans-1,2-Dichloroethene  
Concen: 42.427 ug/l  
RT: 3.087 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument: MSVOA\_X  
ClientSampleId: MW-18B-56-040225MSD


### Manual Integrations APPROVED


Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025




#22  
Diisopropyl ether  
Concen: 40.752 ug/l  
RT: 3.757 min Scan# 438  
Delta R.T. -0.006 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion: 45 Resp: 126501  
Ion Ratio Lower Upper  
45 100  
43 95.8 59.3 88.9#  
87 25.3 20.4 30.6  
59 10.3 9.0 13.6

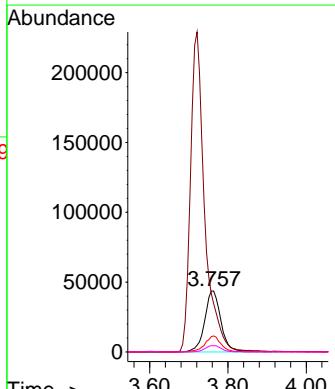




Abundance Scan 432 (3.721 min): VX045577.D\data.ms

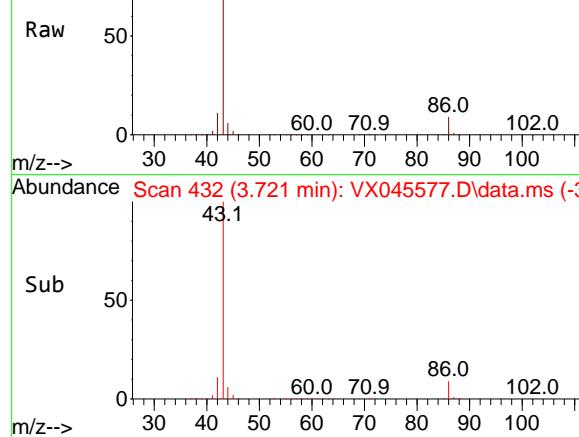

Abundance Scan 432 (3.721 min): VX045577.D\data.ms (-38)

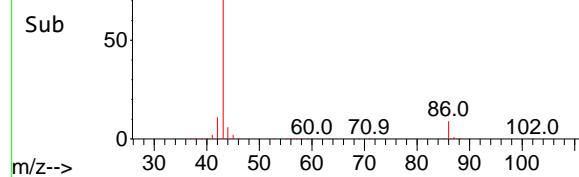

#23

Vinyl Acetate

Concen: 216.251 ug/l

RT: 3.721 min Scan# 4

Delta R.T. 0.000 min



Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED


Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

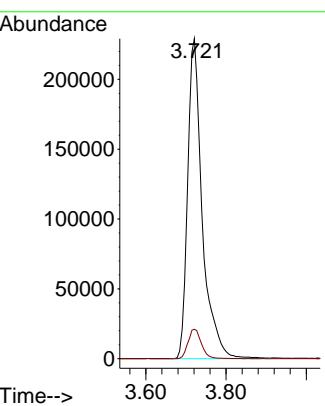

Abundance Scan 413 (3.605 min): VX045577.D\data.ms

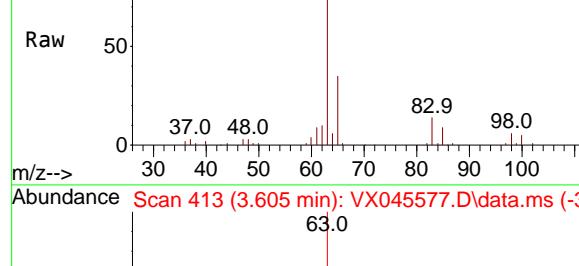

Abundance Scan 413 (3.605 min): VX045577.D\data.ms (-36)

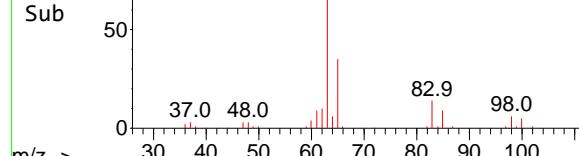

#24

1,1-Dichloroethane

Concen: 42.006 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Tgt Ion: 63 Resp: 73743


Ion Ratio Lower Upper

63 100

98 6.3 3.4 10.1


100 5.1 2.2 6.6

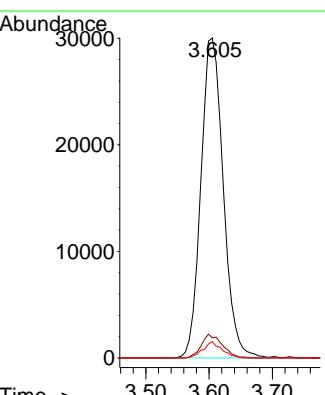



#25  
2-Butanone  
Concen: 219.133 ug/l  
RT: 4.556 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33




Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD




Tgt Ion: 43 Resp: 16664  
Ion Ratio Lower Upper  
43 100  
72 22.8 18.6 28.0

Manual Integrations  
**APPROVED**



Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

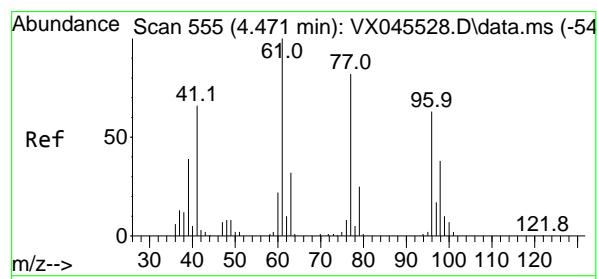




#26  
2,2-Dichloropropane  
Concen: 41.532 ug/l  
RT: 4.465 min Scan# 554  
Delta R.T. -0.006 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

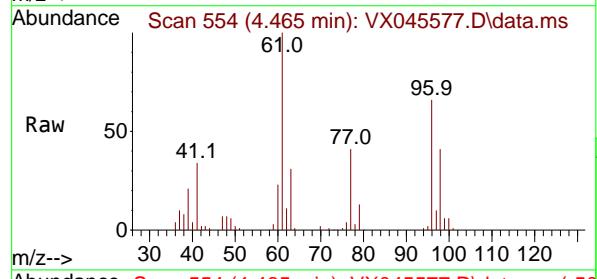

Tgt Ion: 77 Resp: 47107  
Ion Ratio Lower Upper  
77 100  
97 27.1 10.6 31.8

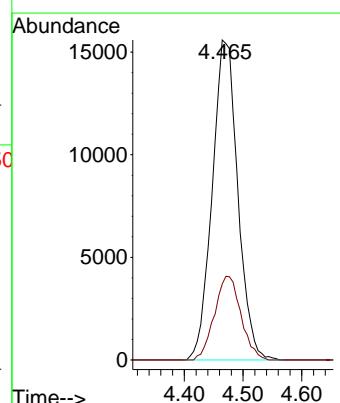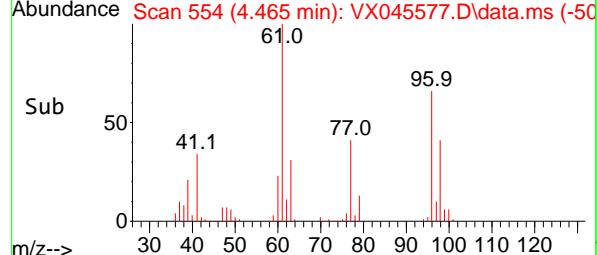


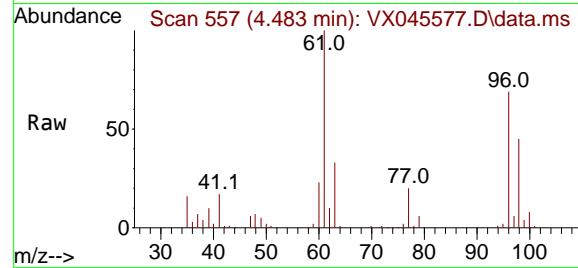



#27  
cis-1,2-Dichloroethene  
Concen: 109.437 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD



### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

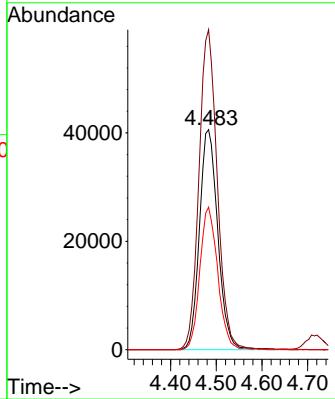



#28  
Bromochloromethane  
Concen: 51.901 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion: 49 Resp: 44030  
Ion Ratio Lower Upper  
49 100  
129 1.8 0.0 3.8  
130 68.4 54.6 81.8

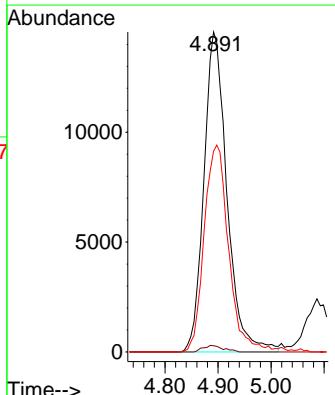





Abundance Scan 643 (5.007 min): VX045577.D\data.ms

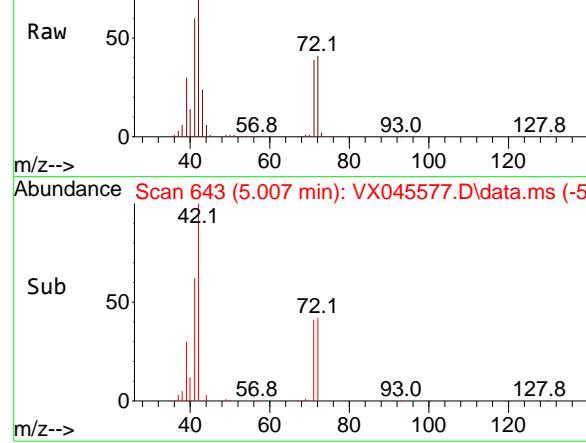

Abundance Scan 656 (5.086 min): VX045577.D\data.ms

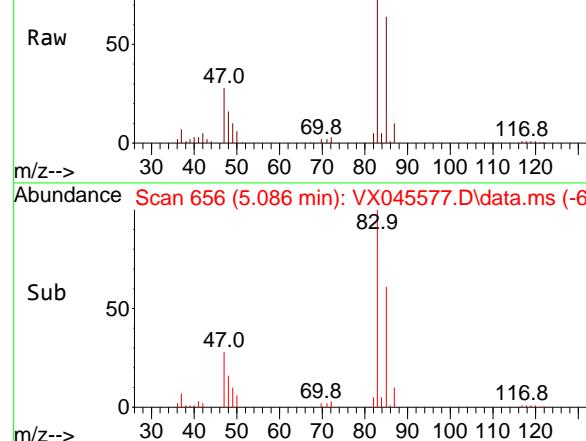

Abundance Scan 656 (5.086 min): VX045577.D\data.ms (-60)

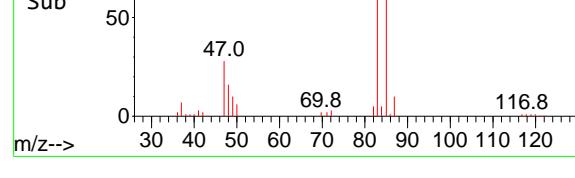

#29

Tetrahydrofuran

Concen: 224.845 ug/l

RT: 5.007 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument :

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

Tgt Ion: 42 Resp: 11085

Ion Ratio Lower Upper

42 100

72 42.3 33.4 50.0


71 39.0 31.4 47.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025

Supervised By :Mahesh Dadoda 04/04/2025

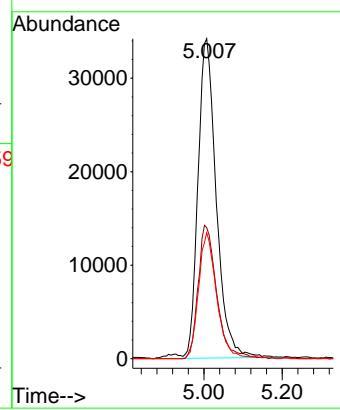

#30

Chloroform

Concen: 42.177 ug/l

RT: 5.086 min Scan# 656

Delta R.T. 0.000 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33


Tgt Ion: 83 Resp: 76188

Ion Ratio Lower Upper

83 100

85 64.5 52.8 79.2

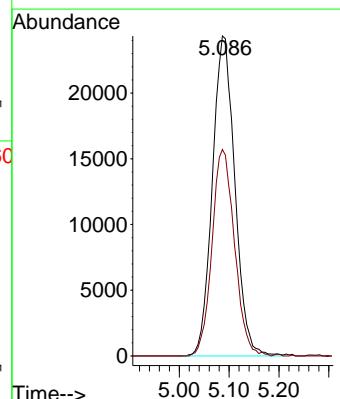



#31

Cyclohexane

Concen: 41.056 ug/l





RT: 5.464 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

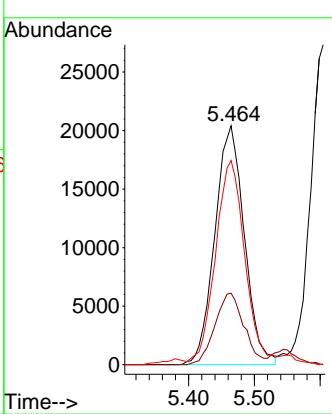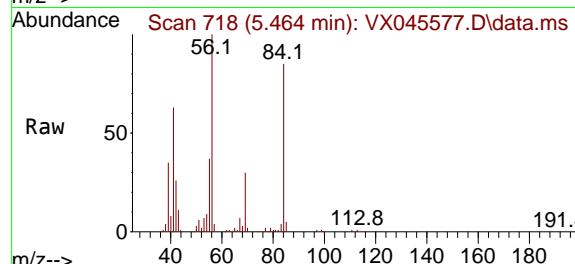

#32

1,1,1-Trichloroethane




Concen: 41.547 ug/l







RT: 5.373 min Scan# 703

Delta R.T. -0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

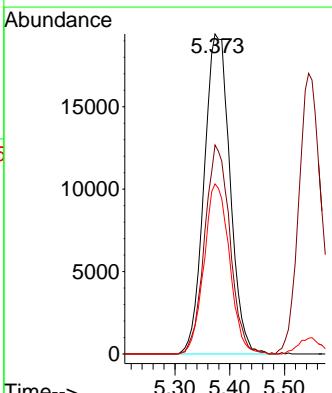

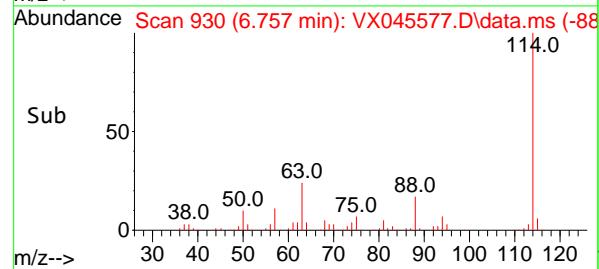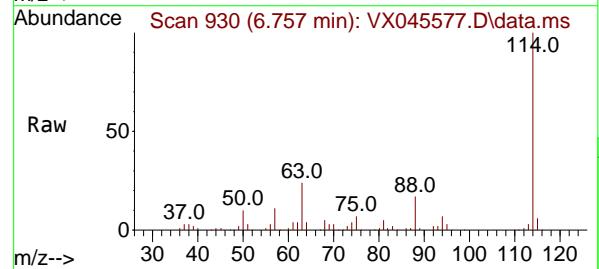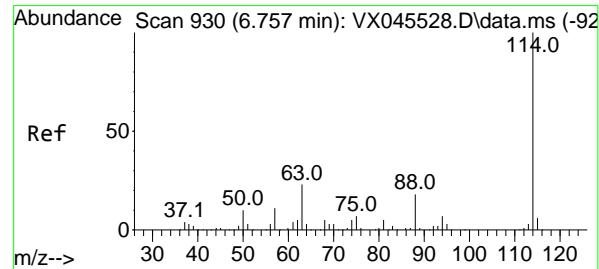

#33

1,2-Dichloroethane-d4

Concen: 46.887 ug/l

RT: 5.952 min Scan# 7

Delta R.T. 0.000 min


Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Tgt Ion:114 Resp: 124452







Ion Ratio Lower Upper

114 100

63 24.3 0.0 46.8

88 16.8 0.0 35.4





#35

Dibromofluoromethane

Concen: 44.805 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument :


MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD


### Manual Integrations APPROVED




Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025



#36  
1,1-Dichloropropene  
Concen: 40.692 ug/l  
RT: 5.684 min Scan# 754  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion: 75 Resp: 48513  
Ion Ratio Lower Upper  
75 100  
110 34.6 16.9 50.6  
77 32.2 25.0 37.4

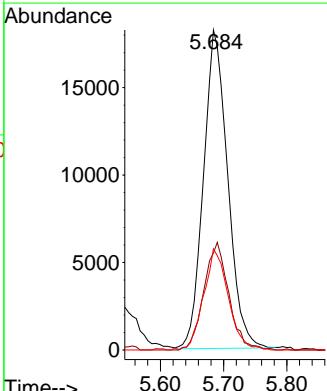

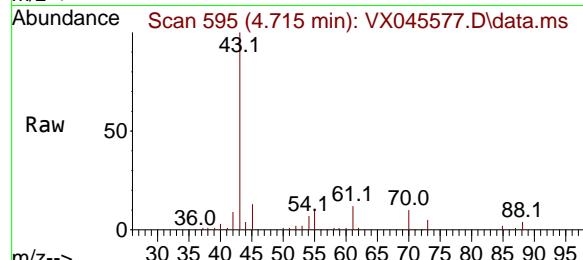

#37

**Ethyl Acetate**

Concen: 41.067 ug/l

RT: 4.715 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX045577.D





Acq: 03 Apr 2025 17:33

Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

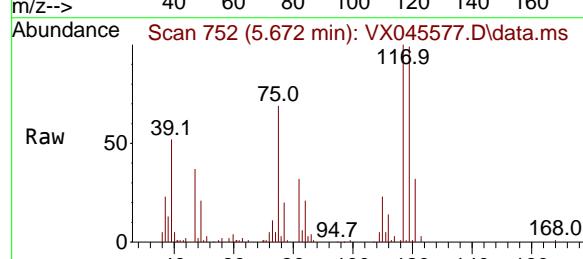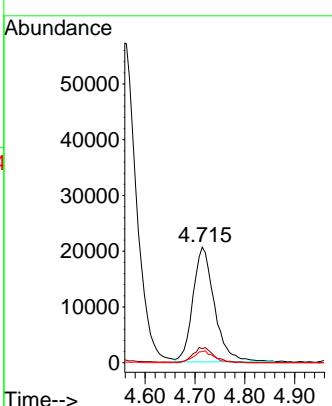**Manual Integrations  
APPROVED**Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

#38

**Carbon Tetrachloride**


Concen: 40.884 ug/l







RT: 5.672 min Scan# 752

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

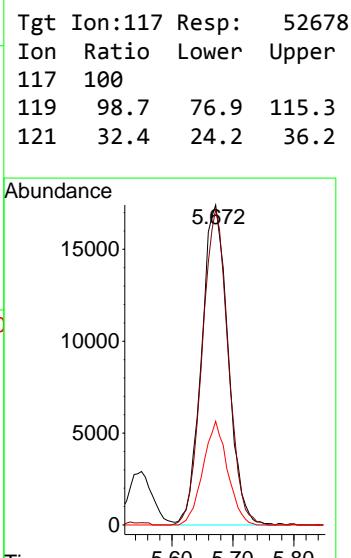



#39

Methylcyclohexane

Concen: 41.348 ug/l

RT: 7.379 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

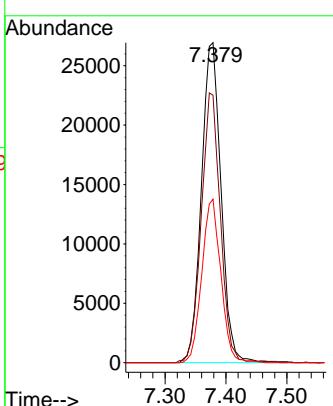 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#40

Benzene

Concen: 41.683 ug/l

RT: 6.031 min Scan# 811

Delta R.T. 0.000 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33







Tgt Ion: 78 Resp: 151773

Ion Ratio Lower Upper

78 100

77 22.6 19.0 28.6



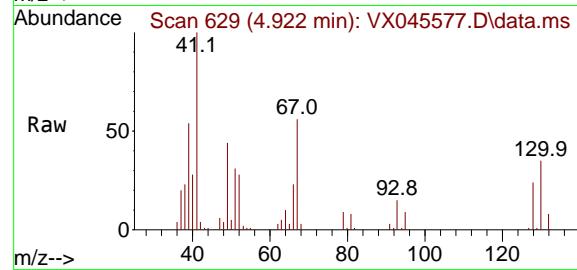

#41

Methacrylonitrile

Concen: 44.462 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.000 min


Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

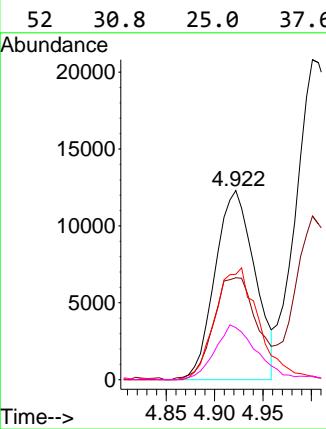

#42

1,2-Dichloroethane

Concen: 42.819 ug/l


RT: 6.080 min Scan# 819


Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt Ion: 62 Resp: 64394  
 Ion Ratio Lower Upper  
 62 100  
 98 8.0 0.0 15.2

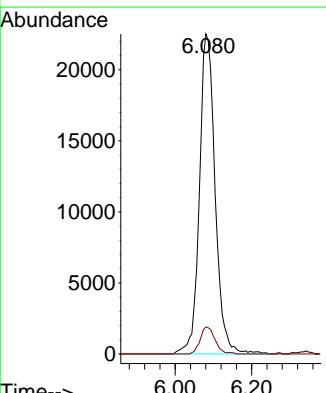



#43

Isopropyl Acetate

Concen: 40.861 ug/l



RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33



Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

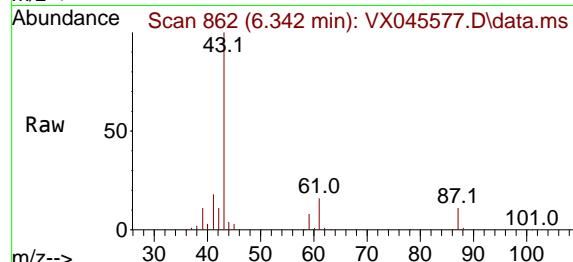


Tgt Ion: 43 Resp: 93045  
 Ion Ratio Lower Upper  
 43 100  
 61 17.4 14.1 21.1  
 87 11.4 9.2 13.8

### Manual Integrations APPROVED



Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


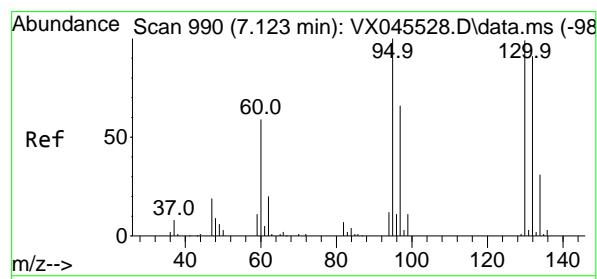



#44  
 Trichloroethene  
 Concen: 74.217 ug/l  
 RT: 7.123 min Scan# 990  
 Delta R.T. 0.000 min  
 Lab File: VX045577.D  
 Acq: 03 Apr 2025 17:33



Tgt Ion:130 Resp: 64230  
 Ion Ratio Lower Upper  
 130 100  
 95 103.0 0.0 202.0

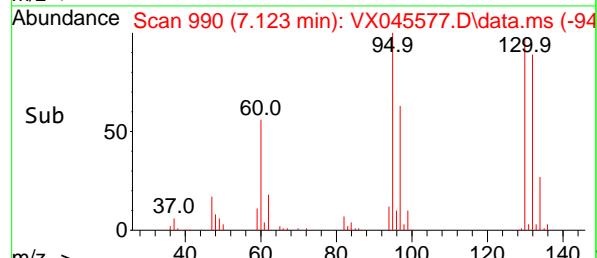

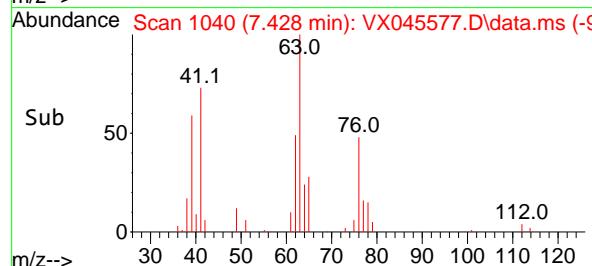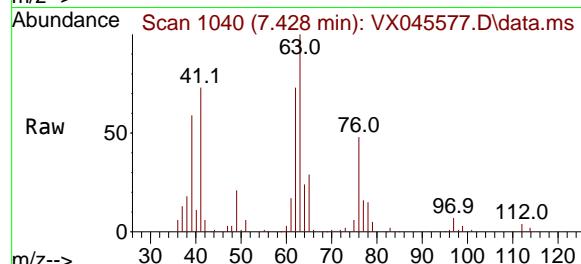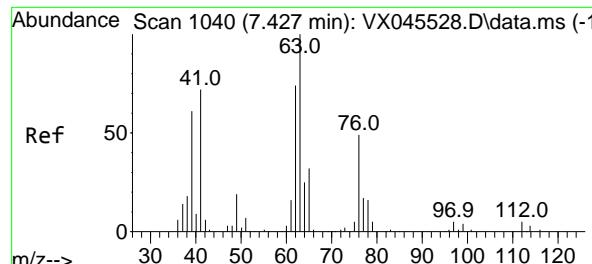

#45

1,2-Dichloropropane

Concen: 41.396 ug/l

RT: 7.428 min Scan# 1040

Delta R.T. 0.000 min



Lab File: VX045577.D

Acq: 03 Apr 2025 17:33



Instrument: MSVOA\_X

ClientSampleId: MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

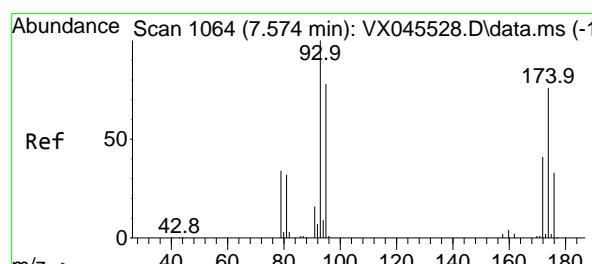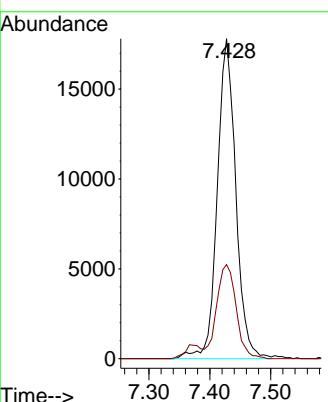 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

 #46  
 Dibromomethane  
 Concen: 42.409 ug/l  
 RT: 7.580 min Scan# 1065  
 Delta R.T. 0.006 min  
 Lab File: VX045577.D  
 Acq: 03 Apr 2025 17:33

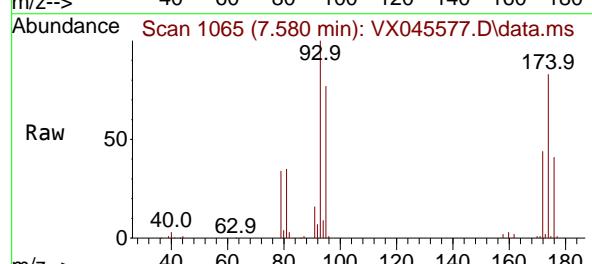
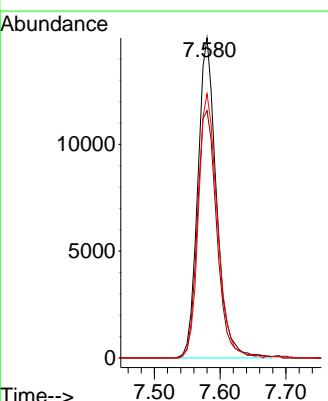
Tgt	Ion	Resp:	29576
Ion	Ratio	Lower	Upper
93	100		
95	80.5	64.8	97.2
174	84.0	65.4	98.0






Abundance Scan 1065 (7.580 min): VX045577.D\data.ms (-1)

 #46  
 Dibromomethane  
 Concen: 42.409 ug/l  
 RT: 7.580 min Scan# 1065  
 Delta R.T. 0.006 min  
 Lab File: VX045577.D  
 Acq: 03 Apr 2025 17:33

Tgt	Ion	Resp:	29576
Ion	Ratio	Lower	Upper
93	100		
95	80.5	64.8	97.2
174	84.0	65.4	98.0

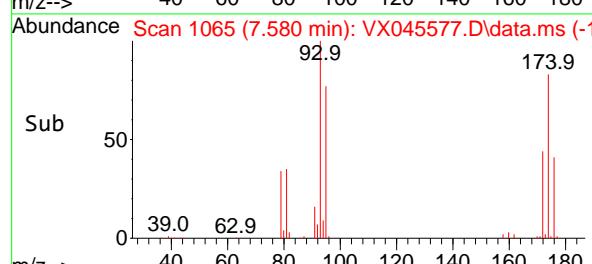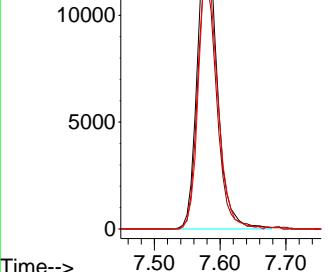



#47

Bromodichloromethane

Concen: 40.580 ug/l

RT: 7.818 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX045577.D





Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

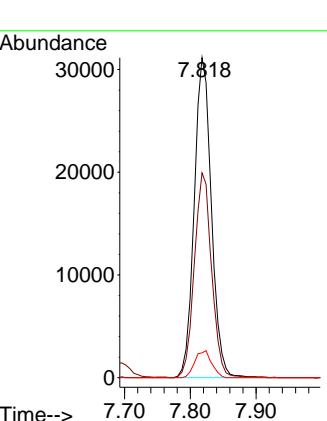 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#48

Methyl methacrylate


Concen: 42.896 ug/l







RT: 7.690 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

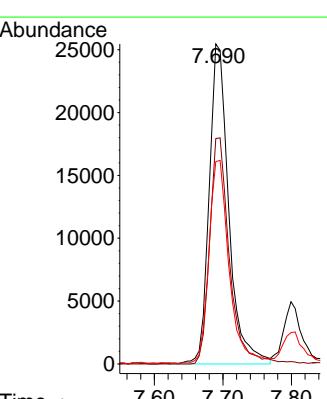 Tgt Ion: 41 Resp: 50434  
 Ion Ratio Lower Upper  
 41 100  
 69 71.5 58.2 87.2  
 39 65.7 53.6 80.4




#49

1,4-Dioxane

Concen: 868.137 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument:


MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

### Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

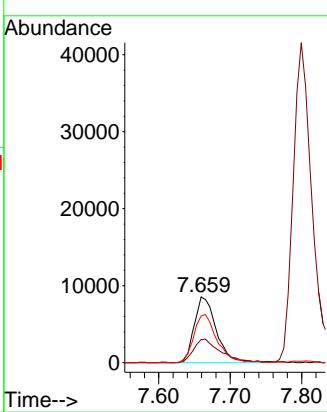

#50

Toluene-d8

Concen: 44.840 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33


Tgt Ion: 98 Resp: 138195

Ion Ratio Lower Upper


98 100

100 65.6 52.2 78.4


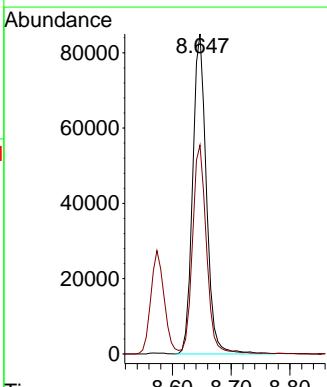





Abundance Scan 1228 (8.574 min): VX045577.D\data.ms

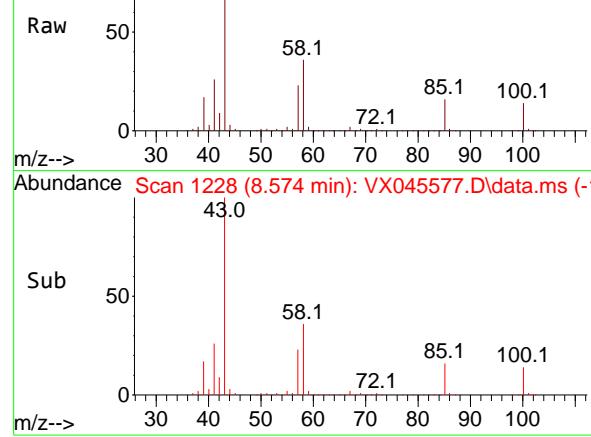


Abundance Scan 1228 (8.574 min): VX045577.D\data.ms (-1)

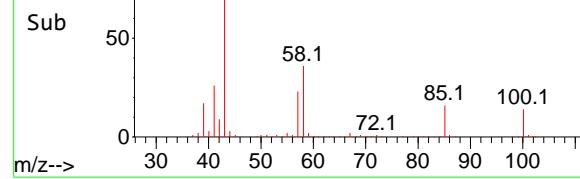

Abundance Scan 1251 (8.714 min): VX045577.D\data.ms

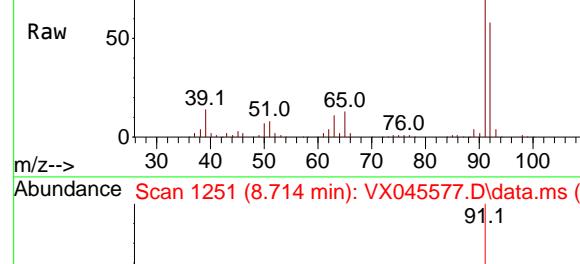

Abundance Scan 1251 (8.714 min): VX045577.D\data.ms (-1)

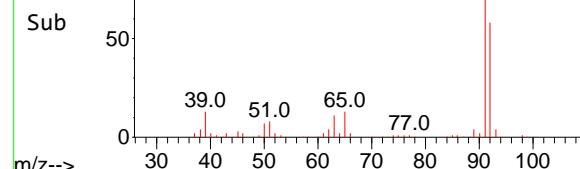

#51

4-Methyl-2-Pentanone

Concen: 216.701 ug/l

RT: 8.574 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**


 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

Tgt Ion: 43 Resp: 32712

Ion Ratio Lower Upper

43 100

58 35.2 28.5 42.7

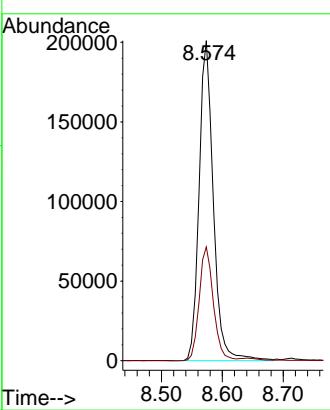

#52

Toluene

Concen: 41.527 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33




Tgt Ion: 92 Resp: 91494

Ion Ratio Lower Upper

92 100

91 171.6 138.7 208.1

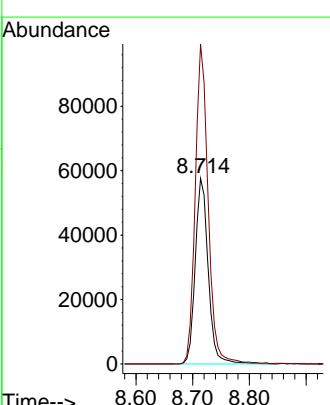

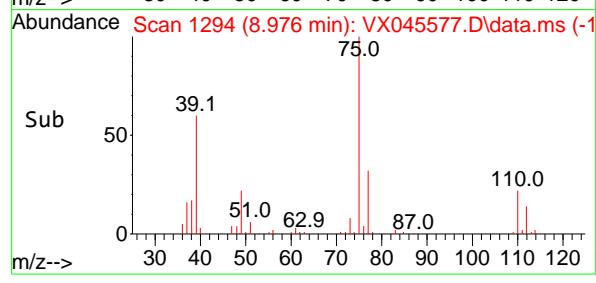





#53

t-1,3-Dichloropropene  
Concen: 36.797 ug/l  
RT: 8.976 min Scan# 1294  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument: MSVOA\_X  
ClientSampleId: MW-18B-56-040225MSD

### Manual Integrations APPROVED


Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025






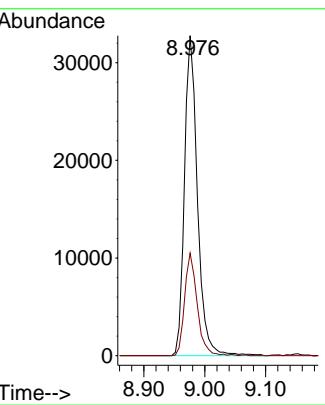


#54

cis-1,3-Dichloropropene  
Concen: 41.229 ug/l  
RT: 8.366 min Scan# 1194  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion: 75 Resp: 53960  
Ion Ratio Lower Upper  
75 100  
77 30.8 24.6 36.8  
39 62.1 48.4 72.6

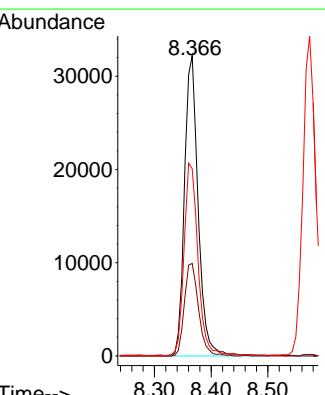



#55

1,1,2-Trichloroethane

Concen: 42.883 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min


Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

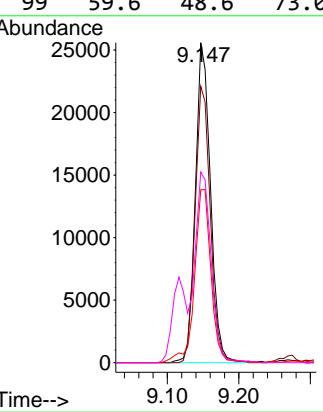

#56

Ethyl methacrylate

Concen: 42.272 ug/l


RT: 9.116 min Scan# 1317




Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt Ion: 69 Resp: 57438  
 Ion Ratio Lower Upper  
 69 100  
 41 75.5 61.3 91.9  
 39 49.8 40.2 60.2

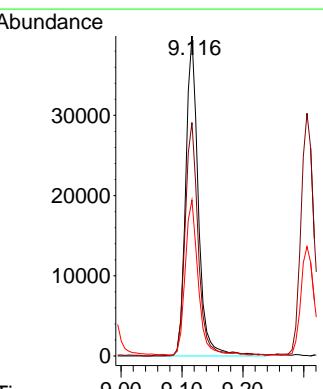



#57

1,3-Dichloropropane

Concen: 42.735 ug/l

RT: 9.305 min Scan# 1348

Delta R.T. 0.000 min




Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X

ClientSampleId : MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

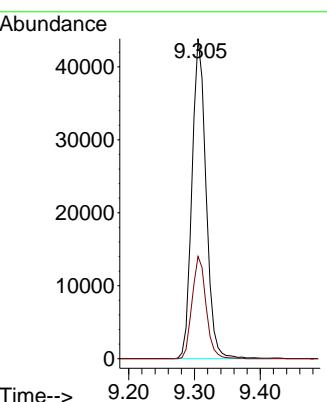 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#59

2-Hexanone


Concen: 219.150 ug/l




RT: 9.427 min Scan# 1368

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

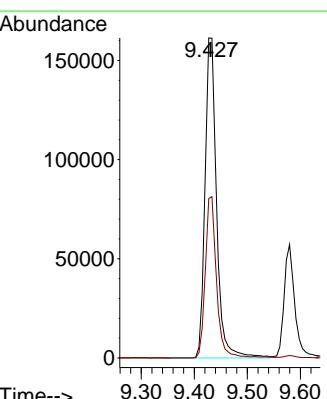 Tgt Ion: 43 Resp: 244980  
 Ion Ratio Lower Upper  
 43 100  
 58 49.4 24.9 74.6

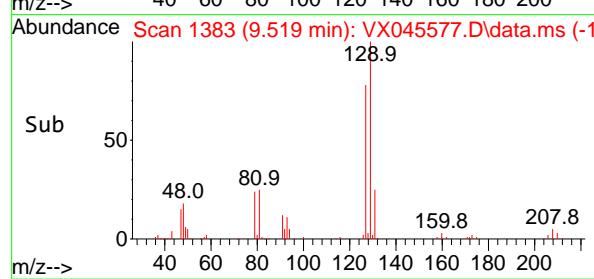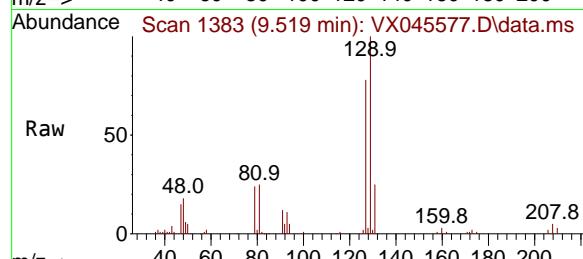


#60

Dibromochloromethane

Concen: 42.099 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X



ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

Abundance

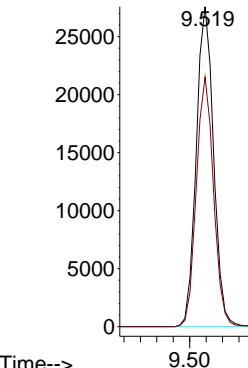

#61

1,2-Dibromoethane

Concen: 43.098 ug/l

RT: 9.610 min Scan# 1398



Delta R.T. 0.006 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33


 Tgt Ion:107 Resp: 38304  
 Ion Ratio Lower Upper  
 107 100  
 109 92.0 75.7 113.5

Abundance

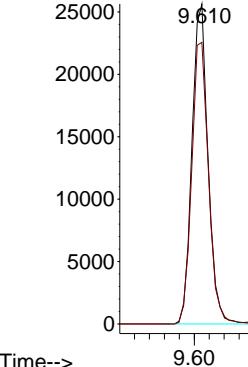

Abundance



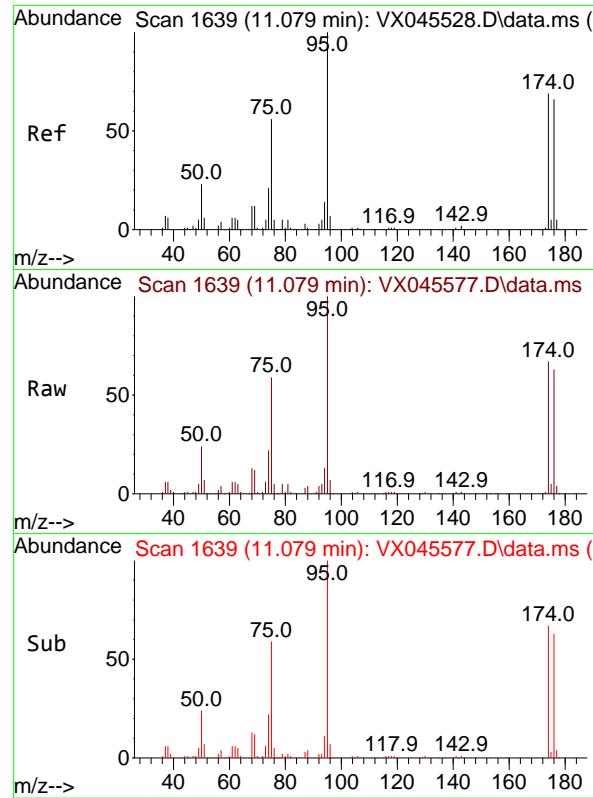

#62

4-Bromofluorobenzene

Concen: 45.976 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min



Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

**Manual Integrations**  
**APPROVED**

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

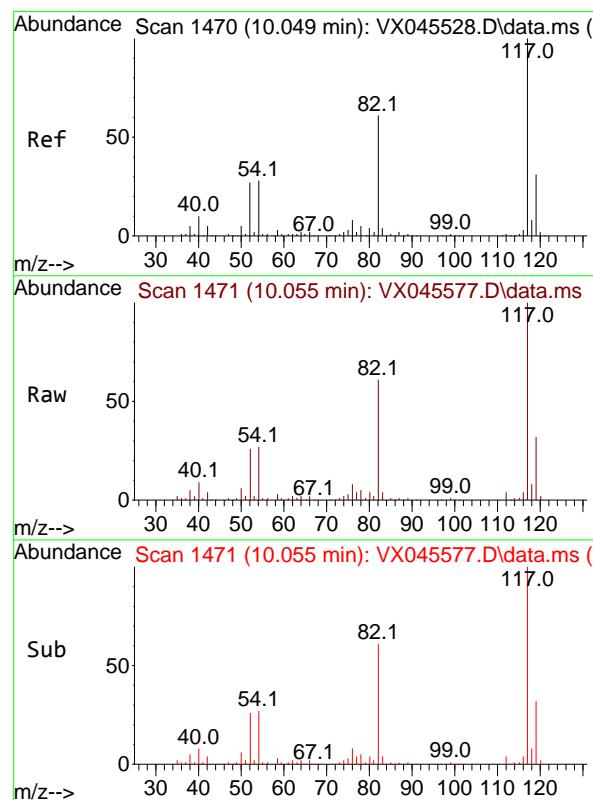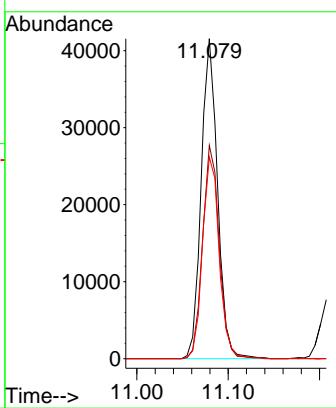

#63

Chlorobenzene-d5

Concen: 50.000 ug/l


RT: 10.055 min Scan# 1471




Delta R.T. 0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt Ion:117 Resp: 109108  
 Ion Ratio Lower Upper  
 117 100  
 82 60.8 49.2 73.8  
 119 31.8 25.1 37.7

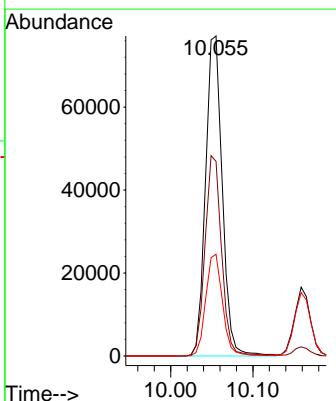



#64

Tetrachloroethene

Concen: 40.159 ug/l

RT: 9.269 min Scan# 1

Delta R.T. -0.000 min





Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

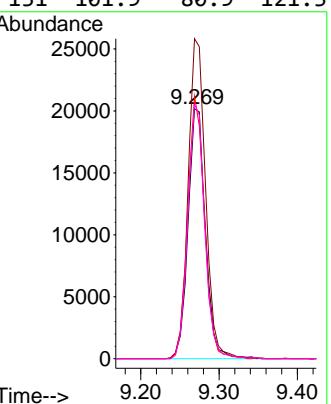

#65

Chlorobenzene

Concen: 42.027 ug/l


RT: 10.079 min Scan# 1475




Delta R.T. 0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt Ion:112 Resp: 97984  
 Ion Ratio Lower Upper  
 112 100  
 114 31.9 24.7 37.1

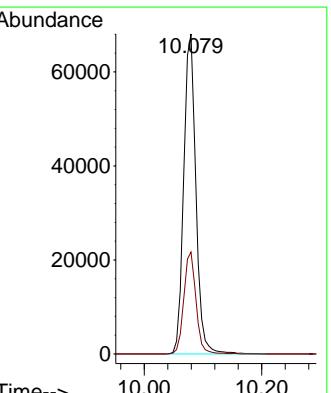



#66

1,1,1,2-Tetrachloroethane

Concen: 40.930 ug/l

RT: 10.159 min Scan# 1488

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33





Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

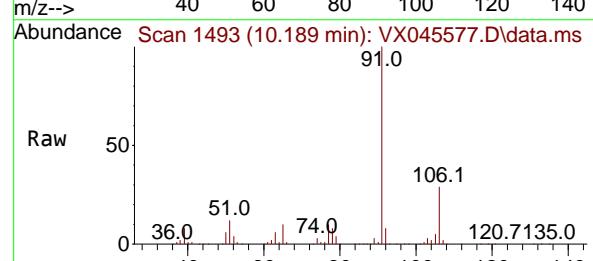 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025


#67

Ethyl Benzene

Concen: 41.892 ug/l

RT: 10.189 min Scan# 1493


Delta R.T. 0.000 min




Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt Ion: 91 Resp: 174928

Ion Ratio Lower Upper

 91 100  
 106 29.0 23.7 35.5








#68  
m/p-Xylenes  
Concen: 85.358 ug/l  
RT: 10.299 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD


### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025



#69  
o-Xylene  
Concen: 42.080 ug/l  
RT: 10.640 min Scan# 1567  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion:106 Resp: 62955  
Ion Ratio Lower Upper  
106 100  
91 232.6 113.6 340.6




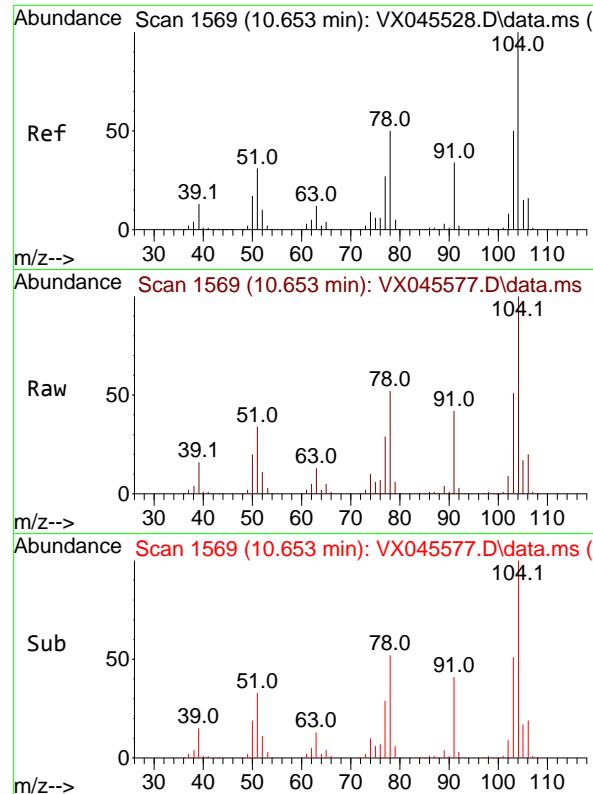


#70  
Styrene  
Concen: 43.611 ug/l  
RT: 10.653 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD


**Manual Integrations**  
**APPROVED**




Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

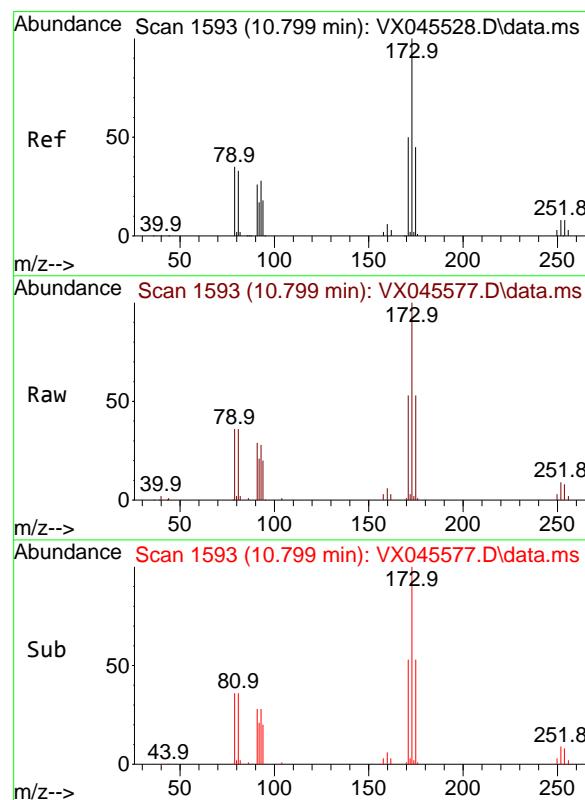

#71  
Bromoform  
Concen: 40.574 ug/l  
RT: 10.799 min Scan# 1593  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion:173 Resp: 24522  
Ion Ratio Lower Upper  
173 100  
175 50.4 23.4 70.2  
254 0.0 0.0 0.0





#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l




RT: 12.018 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD  
**Manual Integrations APPROVED**  
 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025



#73

Isopropylbenzene

Concen: 40.915 ug/l


RT: 10.957 min Scan# 1619




Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt Ion:105 Resp: 167230  
 Ion Ratio Lower Upper  
 105 100  
 120 25.4 12.7 38.0

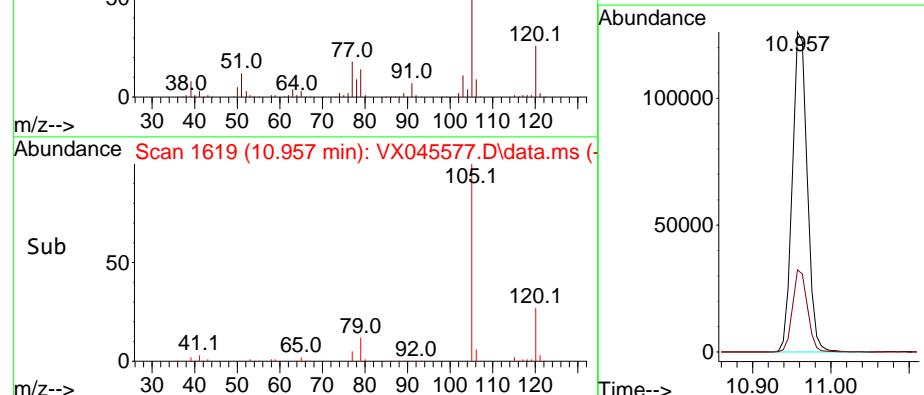



#74

N-amyl acetate

Concen: 40.809 ug/l

RT: 10.842 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

Tgt Ion: 43 Resp: 79780





Ion Ratio Lower Upper

43 100

70 37.7 30.1 45.1

55 23.0 18.3 27.5

61 21.1 17.5 26.3

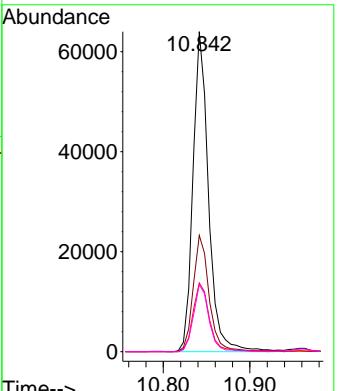

#75

1,1,2,2-Tetrachloroethane

Concen: 40.727 ug/l

RT: 11.207 min Scan# 1660

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Tgt Ion: 83 Resp: 58476




Ion Ratio Lower Upper

83 100

131 9.8 4.7 14.1

85 64.0 32.4 97.2

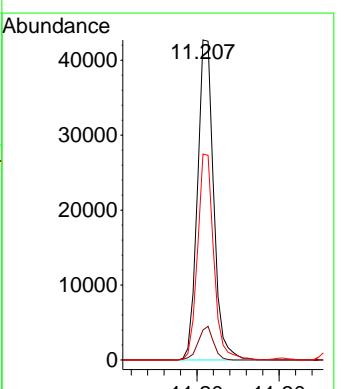

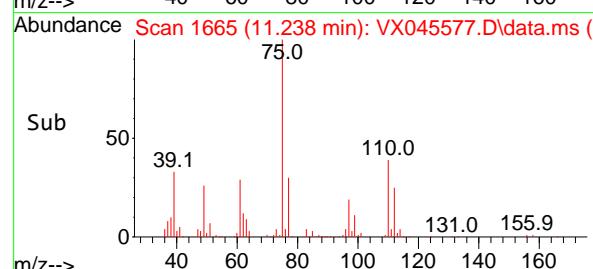

#76

1,2,3-Trichloropropane

Concen: 39.568 ug/l m

RT: 11.238 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33




Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#77

Bromobenzene

Concen: 41.322 ug/l

RT: 11.195 min Scan# 1658

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt Ion:156 Resp: 39023


Ion Ratio Lower Upper


156 100

77 182.0 92.6 277.8

158 92.9 48.1 144.4

1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16

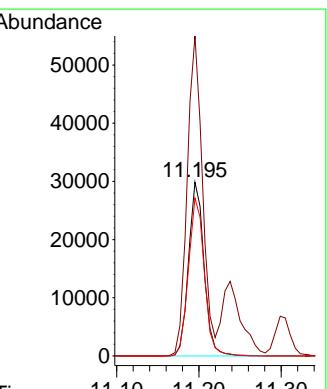

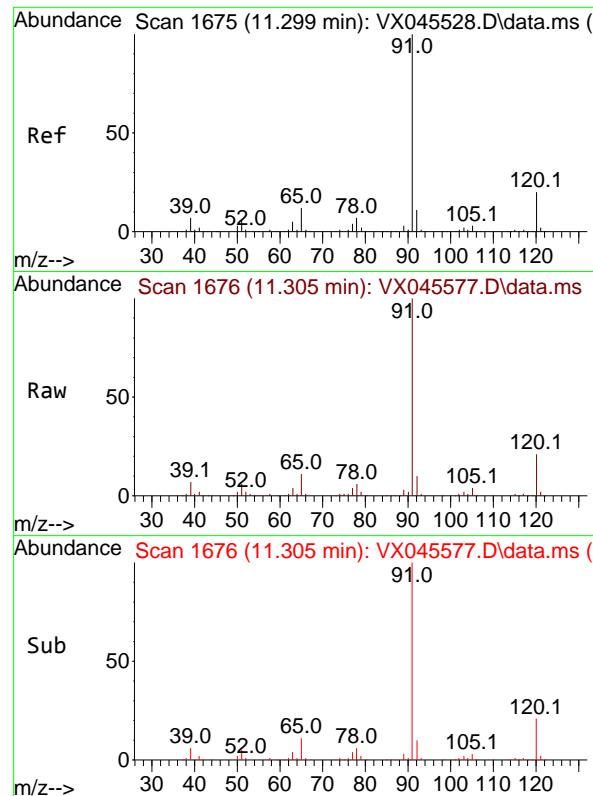

#78

n-propylbenzene

Concen: 41.291 ug/l

RT: 11.305 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

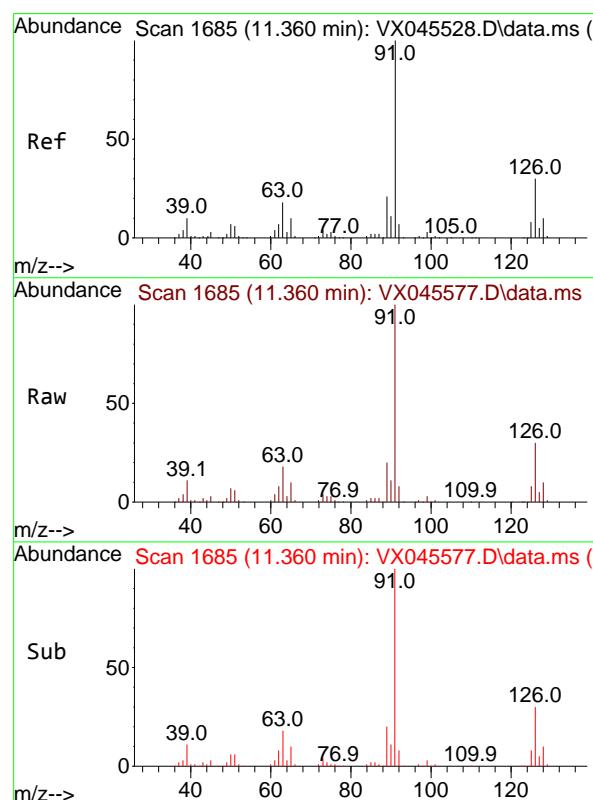 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#79

2-Chlorotoluene

Concen: 40.544 ug/l

RT: 11.360 min Scan# 1685

Delta R.T. 0.000 min

Lab File: VX045577.D


Acq: 03 Apr 2025 17:33




Tgt Ion: 91 Resp: 122025

Ion Ratio Lower Upper

91 100

126 31.7 15.8 47.4

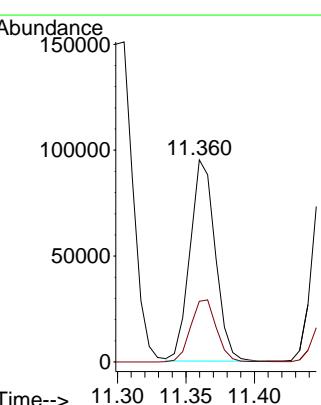







#80

1,3,5-Trimethylbenzene  
Concen: 40.958 ug/l  
RT: 11.451 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025

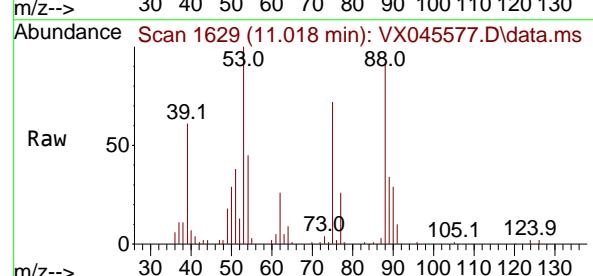




#81

trans-1,4-Dichloro-2-butene  
Concen: 36.907 ug/l  
RT: 11.018 min Scan# 1629  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion: 75 Resp: 13535  
Ion Ratio Lower Upper  
75 100  
53 143.1 101.8 152.6  
89 47.3 37.2 55.8





#82

4-Chlorotoluene

Concen: 41.866 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33





Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

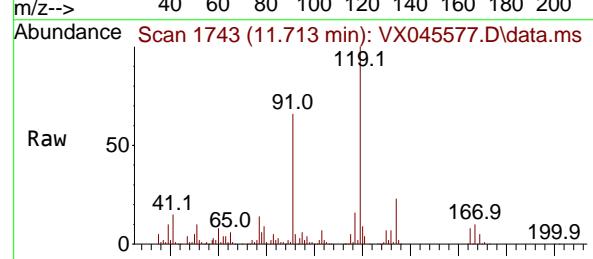 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#83

tert-Butylbenzene


Concen: 40.577 ug/l




RT: 11.713 min Scan# 1743

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

 Tgt Ion:119 Resp: 135774  
 Ion Ratio Lower Upper  
 119 100  
 91 66.6 32.4 97.2  
 134 22.9 11.5 34.5

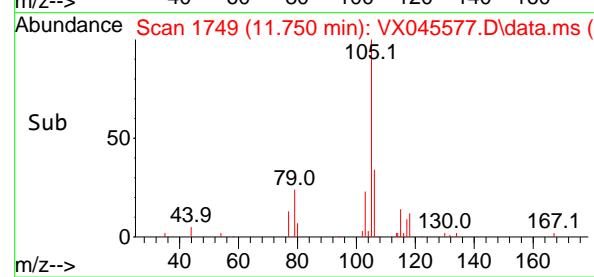





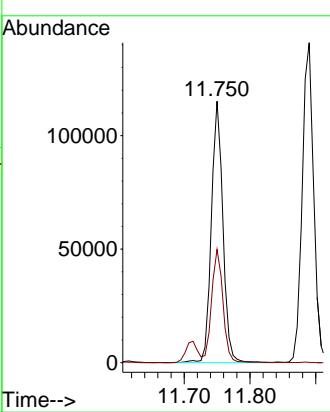
#84

1,2,4-Trimethylbenzene  
Concen: 41.550 ug/l  
RT: 11.750 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD

### Manual Integrations APPROVED


Reviewed By : Semsettin Yesilyurt 04/04/2025  
Supervised By : Mahesh Dadoda 04/04/2025






#85

sec-Butylbenzene  
Concen: 41.307 ug/l  
RT: 11.890 min Scan# 1772  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion:105 Resp: 169765  
Ion Ratio Lower Upper  
105 100  
134 18.9 9.6 28.6

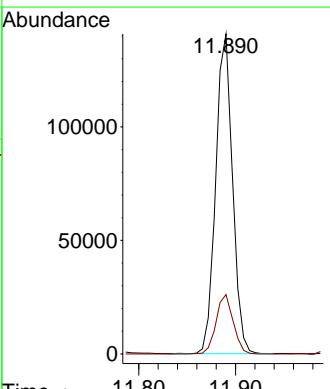



#86

p-Isopropyltoluene

Concen: 40.807 ug/l

RT: 12.006 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33





Instrument:

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

**Manual Integrations  
APPROVED**

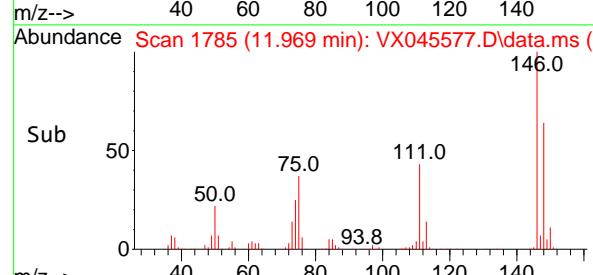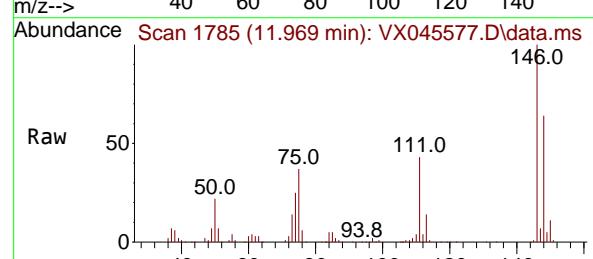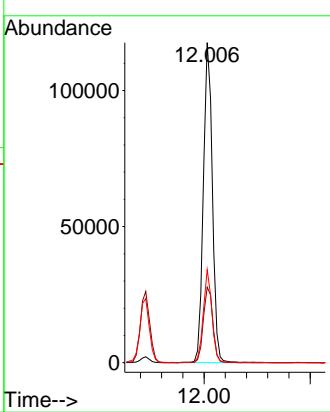 Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025


#87

1,3-Dichlorobenzene

Concen: 39.704 ug/l


RT: 11.969 min Scan# 1785


Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt	Ion:146	Resp:	68253
Ion	Ratio	Lower	Upper
146	100		
111	44.9	22.2	66.6
148	64.2	31.9	95.7

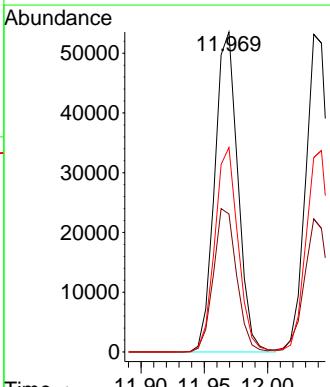

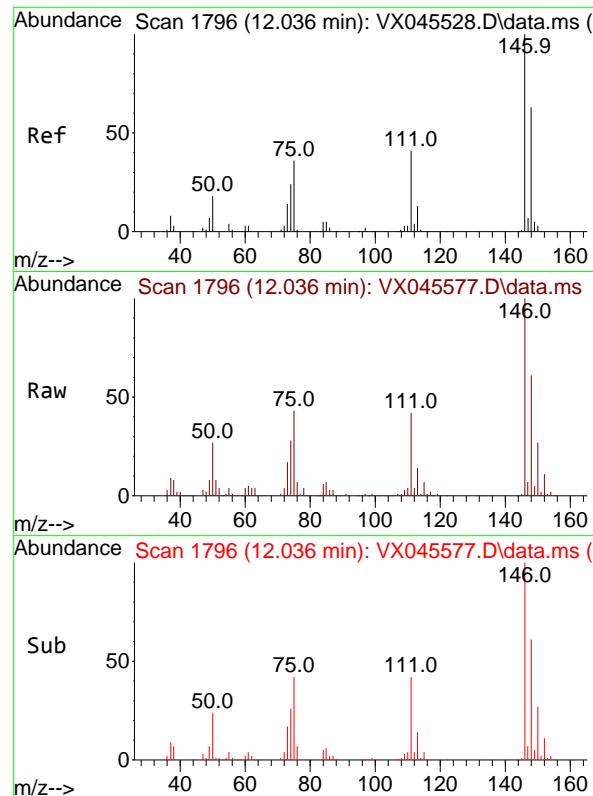

#88

1,4-Dichlorobenzene

Concen: 39.473 ug/l

RT: 12.036 min Scan# 1

Delta R.T. 0.000 min



Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD  
**Manual Integrations APPROVED**

Tgt Ion:146 Resp: 6879:  
 Ion Ratio Lower Upper  
 146 100  
 111 43.1 20.9 62.8  
 148 64.7 31.5 94.5

Reviewed By :Semsettin Yesilyurt 04/04/2025  
 Supervised By :Mahesh Dadoda 04/04/2025

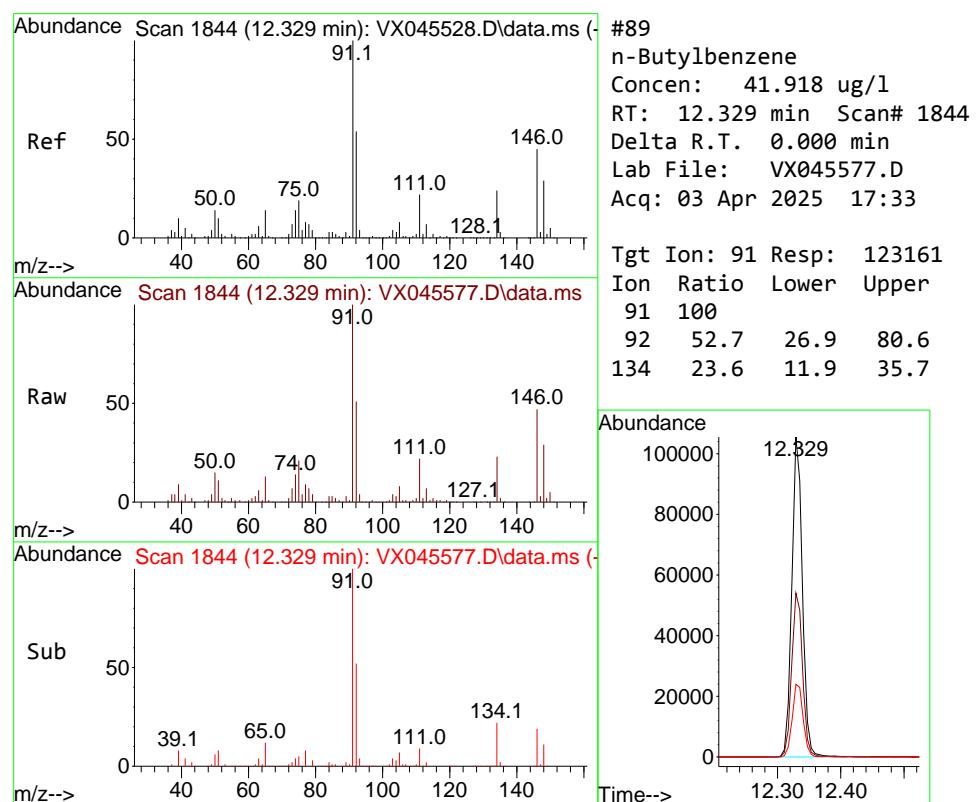

#89

n-Butylbenzene

Concen: 41.918 ug/l


RT: 12.329 min Scan# 1844




Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Tgt Ion: 91 Resp: 123161  
 Ion Ratio Lower Upper  
 91 100  
 92 52.7 26.9 80.6  
 134 23.6 11.9 35.7









#90  
Hexachloroethane  
Concen: 40.163 ug/l  
RT: 12.536 min Scan# 1  
Instrument: MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33  
ClientSampleId : MW-18B-56-040225MSD


### Manual Integrations APPROVED


Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

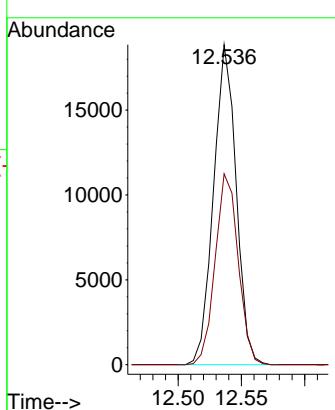

#91  
1,2-Dichlorobenzene  
Concen: 40.959 ug/l  
RT: 12.335 min Scan# 1845  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion:146 Resp: 70002  
Ion Ratio Lower Upper  
146 100  
111 45.6 22.9 68.8  
148 63.2 31.9 95.5

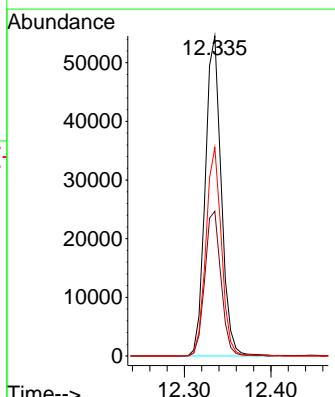


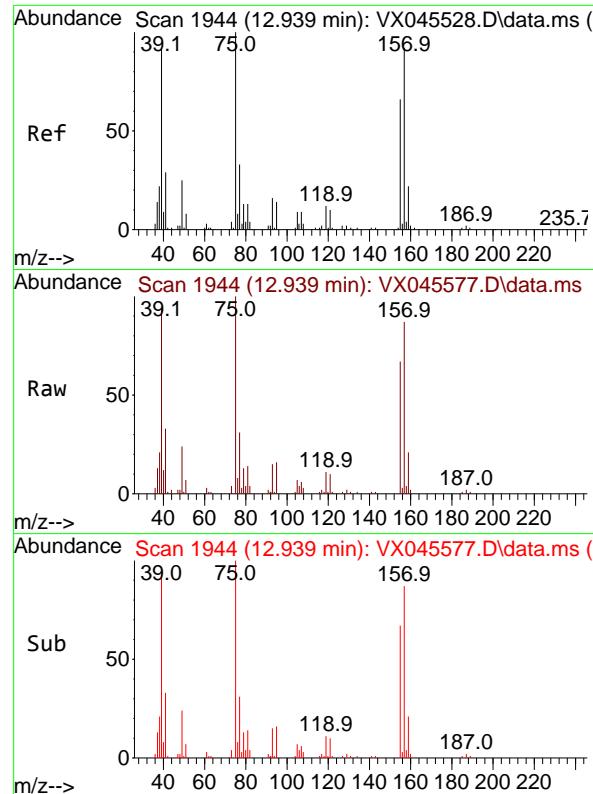


#92  
1,2-Dibromo-3-Chloropropane  
Concen: 42.015 ug/l  
RT: 12.939 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
ClientSampleId : MW-18B-56-040225MSD


### Manual Integrations APPROVED




Reviewed By :Semsettin Yesilyurt 04/04/2025  
Supervised By :Mahesh Dadoda 04/04/2025

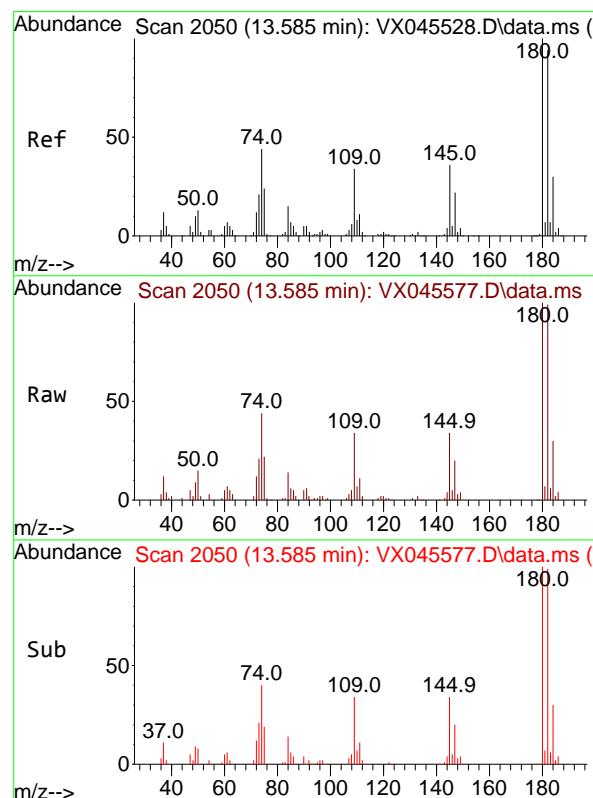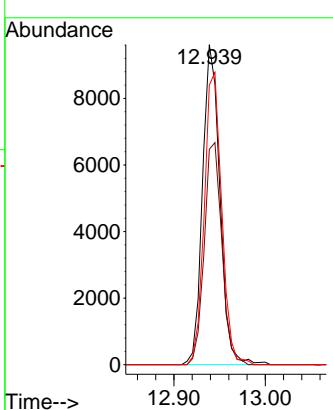

#93  
1,2,4-Trichlorobenzene  
Concen: 39.634 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX045577.D  
Acq: 03 Apr 2025 17:33

Tgt Ion:180 Resp: 37705  
Ion Ratio Lower Upper  
180 100  
182 94.8 47.9 143.6  
145 33.7 17.9 53.8



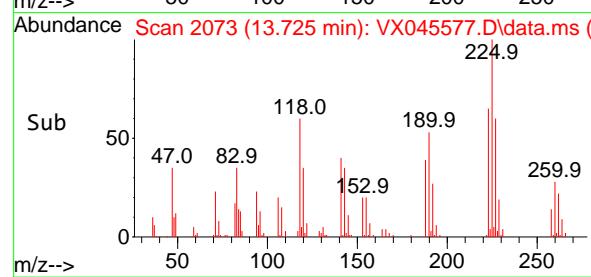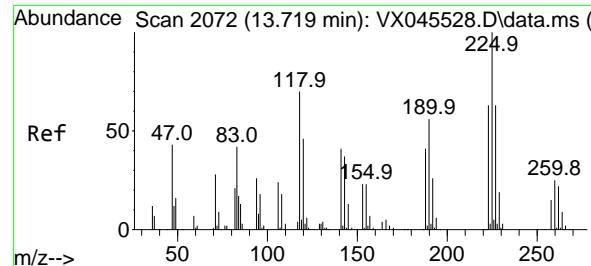

#94

Hexachlorobutadiene

Concen: 38.647 ug/l




RT: 13.725 min Scan# 2

Delta R.T. 0.006 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument : MSVOA\_X  
 ClientSampleId : MW-18B-56-040225MSD  
**Manual Integrations APPROVED**  
 Reviewed By : Semsettin Yesilyurt 04/04/2025  
 Supervised By : Mahesh Dadoda 04/04/2025

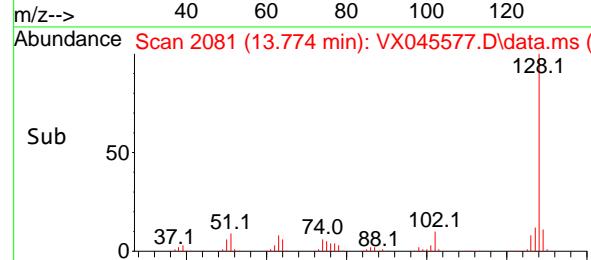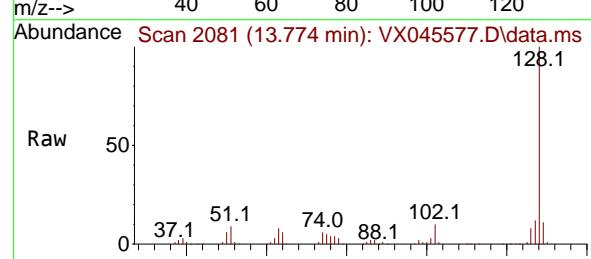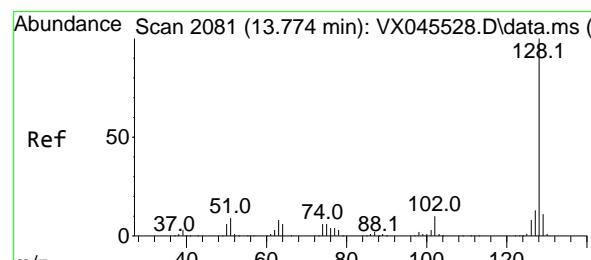

#95

Naphthalene

Concen: 40.810 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33


Tgt Ion:128 Resp: 144479

Ion Ratio Lower Upper

128 100

127 12.6 10.3 15.5

129 10.8 8.6 12.8

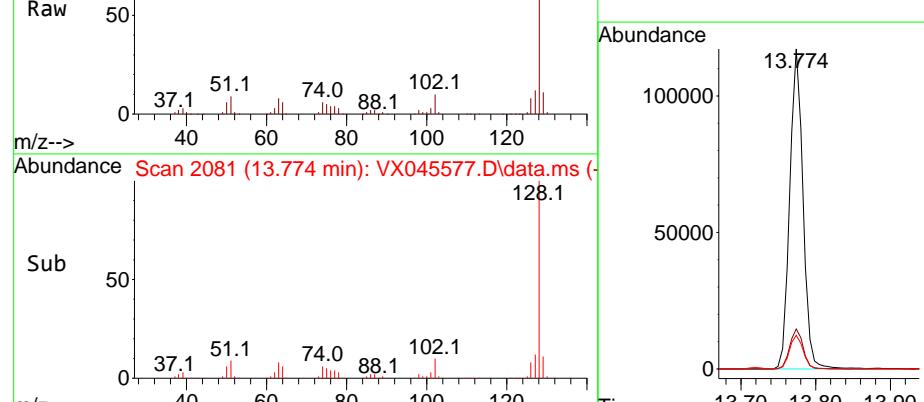

Abundance


13.774

100000

50000

0

13.70 13.75 13.80 13.90

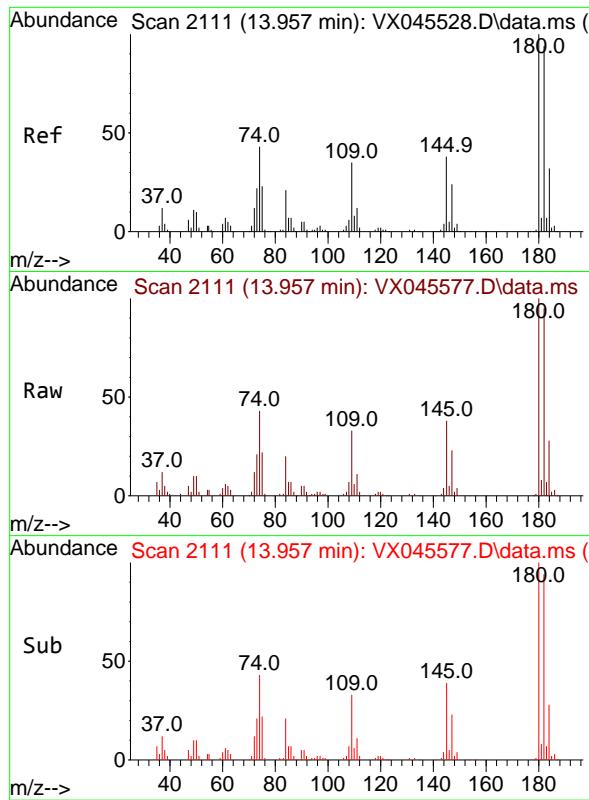

#96

1,2,3-Trichlorobenzene

Concen: 40.543 ug/l

RT: 13.957 min Scan# 2

Delta R.T. 0.000 min

Lab File: VX045577.D

Acq: 03 Apr 2025 17:33

Instrument :

MSVOA\_X

ClientSampleId :

MW-18B-56-040225MSD

Tgt Ion:180 Resp: 40388

Ion Ratio Lower Upper

180 100

182 93.9 47.3 141.8


145 36.0 18.2 54.6

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/04/2025

Supervised By :Mahesh Dadoda 04/04/2025



## Manual Integration Report

Sequence:	VX040225	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICC001	VX045525.D	1,2,3-Trichloropropane	Amit	4/2/2025 2:14:20 PM	MMDadoda	4/2/2025 2:16:05 PM	Peak Integrated by Software
VSTDICC001	VX045525.D	1,4-Dichlorobenzene	Amit	4/2/2025 2:14:20 PM	MMDadoda	4/2/2025 2:16:05 PM	Peak Integrated by Software
VSTDICC001	VX045525.D	1,4-Dioxane	Amit	4/2/2025 2:14:20 PM	MMDadoda	4/2/2025 2:16:05 PM	Peak Integrated by Software
VSTDICC001	VX045525.D	Ethyl methacrylate	Amit	4/2/2025 2:14:20 PM	MMDadoda	4/2/2025 2:16:05 PM	Peak Integrated by Software
VSTDICC001	VX045525.D	Methacrylonitrile	Amit	4/2/2025 2:14:20 PM	MMDadoda	4/2/2025 2:16:05 PM	Peak Integrated by Software
VSTDICC005	VX045526.D	1,2,3-Trichloropropane	Amit	4/2/2025 2:14:22 PM	MMDadoda	4/2/2025 2:16:07 PM	Peak Integrated by Software
VSTDICC020	VX045527.D	1,2,3-Trichloropropane	Amit	4/2/2025 2:14:25 PM	MMDadoda	4/2/2025 2:16:09 PM	Peak Integrated by Software
VSTDICCC050	VX045528.D	1,2,3-Trichloropropane	Amit	4/2/2025 2:14:26 PM	MMDadoda	4/2/2025 2:16:11 PM	Peak Integrated by Software
VSTDICC100	VX045529.D	1,2,3-Trichloropropane	Amit	4/2/2025 2:14:28 PM	MMDadoda	4/2/2025 2:16:15 PM	Peak Integrated by Software
VSTDICC150	VX045530.D	1,2,3-Trichloropropane	Amit	4/2/2025 2:14:30 PM	MMDadoda	4/2/2025 2:16:46 PM	Peak Integrated by Software
VSTDICV050	VX045532.D	1,2,3-Trichloropropane	Amit	4/2/2025 2:14:32 PM	MMDadoda	4/2/2025 2:17:50 PM	Peak Integrated by Software
VSTDCCC050	VX045534.D	1,2,3-Trichloropropane	JOHN	4/3/2025 10:04:10 AM	MMDadoda	4/3/2025 1:12:02 PM	Peak Integrated by Software
VSTDCCC050	VX045557.D	1,2,3-Trichloropropane	JOHN	4/3/2025 10:04:58 AM	MMDadoda	4/3/2025 1:12:08 PM	Peak Integrated by Software

 1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

## Manual Integration Report

Sequence:	VX040225	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
-----------	---------	-----------	-----------	-----------	---------------	---------------	--------

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

### Manual Integration Report

Sequence:	vx040325	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC050	VX045559.D	1,2,3-Trichloropropane	Sam	4/4/2025 7:55:26 AM	mmdadoda	4/4/2025 7:58:07 AM	Peak Integrated by Software
VX0403WBS01	VX045563.D	1,2,3-Trichloropropane	Sam	4/4/2025 7:55:28 AM	mmdadoda	4/4/2025 7:57:38 AM	Peak Integrated by Software
Q1711-03MSD	VX045577.D	1,2,3-Trichloropropane	Sam	4/4/2025 7:55:33 AM	mmdadoda	4/4/2025 7:57:44 AM	Peak Integrated by Software
VSTDCCC050	VX045584.D	1,2,3-Trichloropropane	Sam	4/4/2025 7:55:35 AM	mmdadoda	4/4/2025 7:57:46 AM	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

### Manual Integration Report

Sequence:	vx040425	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC050	VX045586.D	1,2,3-Trichloropropane	JOHN	4/7/2025 9:56:35 AM	MMDadoda	4/7/2025 11:32:09 AM	Peak Integrated by Software
VX0404WBS01	VX045589.D	1,2,3-Trichloropropane	JOHN	4/7/2025 9:56:40 AM	MMDadoda	4/7/2025 11:32:13 AM	Peak Integrated by Software
Q1711-02MS	VX045591.D	1,2,3-Trichloropropane	JOHN	4/7/2025 9:56:50 AM	MMDadoda	4/7/2025 11:32:21 AM	Peak Integrated by Software
VSTDCCC050	VX045612.D	1,2,3-Trichloropropane	JOHN	4/7/2025 9:57:10 AM	MMDadoda	4/7/2025 11:32:29 AM	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX040225**

Review By	John Carlone	Review On	4/2/2025 9:42:46 AM
Supervise By	Amit Patel	Supervise On	4/2/2025 2:14:39 PM
SubDirectory	VX040225	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133559,VP133563 VP133569,VP133570,VP133571,VP133572,VP133573,VP133574		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133564,VP133565 VP133575		

Sr #	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX045524.D	01 Apr 2025 16:15	JC/MD	Ok
2	VSTDICC001	VX045525.D	01 Apr 2025 17:06	JC/MD	Ok,M
3	VSTDICC005	VX045526.D	01 Apr 2025 17:29	JC/MD	Ok,M
4	VSTDICC020	VX045527.D	01 Apr 2025 17:52	JC/MD	Ok,M
5	VSTDICCC050	VX045528.D	01 Apr 2025 18:15	JC/MD	Ok,M
6	VSTDICC100	VX045529.D	01 Apr 2025 18:38	JC/MD	Ok,M
7	VSTDICC150	VX045530.D	01 Apr 2025 19:02	JC/MD	Ok,M
8	IBLK	VX045531.D	01 Apr 2025 19:25	JC/MD	Ok
9	VSTDICV050	VX045532.D	01 Apr 2025 19:48	JC/MD	Ok,M
10	BFB	VX045533.D	02 Apr 2025 09:30	JC/MD	Ok
11	VSTDCCCC050	VX045534.D	02 Apr 2025 10:02	JC/MD	Ok,M
12	VX0402MBL01	VX045535.D	02 Apr 2025 10:30	JC/MD	Ok
13	VX0402WBL01	VX045536.D	02 Apr 2025 10:53	JC/MD	Ok
14	VX0402WBS01	VX045537.D	02 Apr 2025 11:16	JC/MD	Ok,M
15	VX0402WBSD01	VX045538.D	02 Apr 2025 11:44	JC/MD	Ok,M
16	Q1697-01	VX045539.D	02 Apr 2025 12:07	JC/MD	Dilution
17	Q1697-02	VX045540.D	02 Apr 2025 12:30	JC/MD	Dilution
18	IBLK	VX045541.D	02 Apr 2025 12:54	JC/MD	Ok
19	Q1697-01DL	VX045542.D	02 Apr 2025 13:21	JC/MD	Ok
20	Q1697-02DL	VX045543.D	02 Apr 2025 13:44	JC/MD	Ok
21	Q1697-03	VX045544.D	02 Apr 2025 14:07	JC/MD	Not Ok

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX040225**

Review By	John Carlone	Review On	4/2/2025 9:42:46 AM
Supervise By	Amit Patel	Supervise On	4/2/2025 2:14:39 PM
SubDirectory	VX040225	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133559,VP133563 VP133569,VP133570,VP133571,VP133572,VP133573,VP133574		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133564,VP133565 VP133575		

22	Q1697-04	VX045545.D	02 Apr 2025 14:31	JC/MD	Not Ok
23	Q1697-05	VX045546.D	02 Apr 2025 14:54	JC/MD	Not Ok
24	Q1697-07	VX045547.D	02 Apr 2025 15:18	JC/MD	Not Ok
25	IBLK	VX045548.D	02 Apr 2025 15:41	JC/MD	Ok
26	Q1697-03	VX045549.D	02 Apr 2025 16:04	JC/MD	Ok
27	Q1697-04	VX045550.D	02 Apr 2025 16:27	JC/MD	Ok
28	Q1697-05	VX045551.D	02 Apr 2025 16:51	JC/MD	Ok
29	Q1697-06	VX045552.D	02 Apr 2025 17:14	JC/MD	ReRun
30	Q1623-01	VX045553.D	02 Apr 2025 17:37	JC/MD	Ok
31	Q1623-02	VX045554.D	02 Apr 2025 18:01	JC/MD	Ok
32	Q1623-03	VX045555.D	02 Apr 2025 18:24	JC/MD	Ok
33	Q1623-04	VX045556.D	02 Apr 2025 18:47	JC/MD	Ok
34	VSTDCCCC050	VX045557.D	02 Apr 2025 19:10	JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX040325**

Review By	Semsettin Yesilyurt	Review On	4/4/2025 7:55:43 AM
Supervise By	Mahesh Dadoda	Supervise On	4/4/2025 7:58:30 AM
SubDirectory	VX040325	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133576		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133577,VP133578		

Sr #	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX045558.D	03 Apr 2025 10:01	JC/MD	Ok
2	VSTDCCC050	VX045559.D	03 Apr 2025 10:30	JC/MD	Ok,M
3	VX0403MBL01	VX045560.D	03 Apr 2025 10:58	JC/MD	Ok
4	VX0403WBL01	VX045561.D	03 Apr 2025 11:21	JC/MD	Ok
5	Q1697-06	VX045562.D	03 Apr 2025 11:45	JC/MD	Ok
6	VX0403WBS01	VX045563.D	03 Apr 2025 12:08	JC/MD	Ok,M
7	Q1711-01	VX045564.D	03 Apr 2025 12:31	JC/MD	Not Ok
8	Q1711-04	VX045565.D	03 Apr 2025 12:54	JC/MD	Not Ok
9	Q1711-07	VX045566.D	03 Apr 2025 13:18	JC/MD	Not Ok
10	VX0403WBSD01	VX045567.D	03 Apr 2025 13:41	JC/MD	Ok,M
11	Q1711-07	VX045568.D	03 Apr 2025 14:04	JC/MD	Ok
12	Q1711-04	VX045569.D	03 Apr 2025 14:27	JC/MD	Ok
13	IBLK	VX045570.D	03 Apr 2025 14:50	JC/MD	Ok
14	Q1711-10	VX045571.D	03 Apr 2025 15:14	JC/MD	Ok
15	Q1711-08	VX045572.D	03 Apr 2025 15:37	JC/MD	Ok
16	Q1711-05	VX045573.D	03 Apr 2025 16:00	JC/MD	Not Ok
17	Q1711-06	VX045574.D	03 Apr 2025 16:23	JC/MD	Not Ok
18	Q1711-01	VX045575.D	03 Apr 2025 16:47	JC/MD	Ok
19	Q1711-02MS	VX045576.D	03 Apr 2025 17:10	JC/MD	Not Ok
20	Q1711-03MSD	VX045577.D	03 Apr 2025 17:33	JC/MD	Ok,M
21	IBLK	VX045578.D	03 Apr 2025 17:56	JC/MD	Ok

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX040325**

Review By	Semsettin Yesilyurt	Review On	4/4/2025 7:55:43 AM
Supervise By	Mahesh Dadoda	Supervise On	4/4/2025 7:58:30 AM
SubDirectory	VX040325	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133576		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133577,VP133578		

22	IBLK	VX045579.D	03 Apr 2025 18:19	JC/MD	Ok
23	Q1676-01	VX045580.D	03 Apr 2025 18:43	JC/MD	Ok
24	Q1676-02	VX045581.D	03 Apr 2025 19:06	JC/MD	Ok
25	Q1676-03	VX045582.D	03 Apr 2025 19:29	JC/MD	Ok
26	Q1676-04	VX045583.D	03 Apr 2025 19:52	JC/MD	Ok
27	VSTDCCC050	VX045584.D	03 Apr 2025 20:15	JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX040425**

Review By	John Carfone	Review On	4/7/2025 9:58:56 AM
Supervise By	Mahesh Dadoda	Supervise On	4/7/2025 12:14:08 PM
SubDirectory	VX040425	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133596		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133597,VP133598		

Sr #	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX045585.D	04 Apr 2025 09:31	JC/MD	Ok
2	VSTDCCC050	VX045586.D	04 Apr 2025 10:00	JC/MD	Ok,M
3	VX0404MBL01	VX045587.D	04 Apr 2025 10:28	JC/MD	Ok
4	VX0404WBL01	VX045588.D	04 Apr 2025 10:51	JC/MD	Ok
5	VX0404WBS01	VX045589.D	04 Apr 2025 11:14	JC/MD	Ok,M
6	VX0404WBSD01	VX045590.D	04 Apr 2025 11:40	JC/MD	Ok,M
7	Q1711-02MS	VX045591.D	04 Apr 2025 12:04	JC/MD	Ok,M
8	IBLK	VX045592.D	04 Apr 2025 12:27	JC/MD	Ok
9	Q1716-01	VX045593.D	04 Apr 2025 12:50	JC/MD	Ok
10	Q1731-04	VX045594.D	04 Apr 2025 13:13	JC/MD	Not Ok
11	Q1731-01	VX045595.D	04 Apr 2025 13:37	JC/MD	Not Ok
12	Q1731-02	VX045596.D	04 Apr 2025 14:00	JC/MD	Not Ok
13	Q1731-03	VX045597.D	04 Apr 2025 14:23	JC/MD	Not Ok
14	IBLK	VX045598.D	04 Apr 2025 14:46	JC/MD	Ok
15	Q1731-07	VX045599.D	04 Apr 2025 15:10	JC/MD	Ok
16	Q1731-05	VX045600.D	04 Apr 2025 15:33	JC/MD	Ok
17	PB167448TB	VX045601.D	04 Apr 2025 15:56	JC/MD	Ok
18	PB167448ZHE#01	VX045602.D	04 Apr 2025 16:19	JC/MD	Ok
19	PB167448ZHE#02	VX045603.D	04 Apr 2025 16:42	JC/MD	Ok
20	PB167448ZHE#03	VX045604.D	04 Apr 2025 17:06	JC/MD	Ok
21	PB167448ZHE#04	VX045605.D	04 Apr 2025 17:29	JC/MD	Ok

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX040425**

Review By	John Caralone	Review On	4/7/2025 9:58:56 AM
Supervise By	Mahesh Dadoda	Supervise On	4/7/2025 12:14:08 PM
SubDirectory	VX040425	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133596		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133597,VP133598		

22	PB167448ZHE#05	VX045606.D	04 Apr 2025 17:52	JC/MD	Ok,M
23	Q1694-04	VX045607.D	04 Apr 2025 18:15	JC/MD	Ok
24	Q1695-04	VX045608.D	04 Apr 2025 18:38	JC/MD	Ok
25	Q1695-08	VX045609.D	04 Apr 2025 19:01	JC/MD	Ok
26	Q1712-04	VX045610.D	04 Apr 2025 19:24	JC/MD	Ok
27	Q1712-08	VX045611.D	04 Apr 2025 19:48	JC/MD	Ok
28	VSTDCCC050	VX045612.D	04 Apr 2025 20:11	JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX040225

Review By	John Carlone	Review On	4/2/2025 9:42:46 AM
Supervise By	Amit Patel	Supervise On	4/2/2025 2:14:39 PM
SubDirectory	VX040225	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP133559,VP133563		
Initial Calibration Stds	VP133569,VP133570,VP133571,VP133572,VP133573,VP133574		
CCC	VP133564,VP133565		
Internal Standard/PEM	VP133575		
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr #	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX045524.D	01 Apr 2025 16:15		JC/MD	Ok
2	VSTDICCC001	VSTDICCC001	VX045525.D	01 Apr 2025 17:06	%D failed for Comp. #53 in 01PPB	JC/MD	Ok,M
3	VSTDICCC005	VSTDICCC005	VX045526.D	01 Apr 2025 17:29		JC/MD	Ok,M
4	VSTDICCC020	VSTDICCC020	VX045527.D	01 Apr 2025 17:52		JC/MD	Ok,M
5	VSTDICCC050	VSTDICCC050	VX045528.D	01 Apr 2025 18:15		JC/MD	Ok,M
6	VSTDICCC100	VSTDICCC100	VX045529.D	01 Apr 2025 18:38		JC/MD	Ok,M
7	VSTDICCC150	VSTDICCC150	VX045530.D	01 Apr 2025 19:02		JC/MD	Ok,M
8	IBLK	IBLK	VX045531.D	01 Apr 2025 19:25		JC/MD	Ok
9	VSTDICCV050	ICVVX040225	VX045532.D	01 Apr 2025 19:48		JC/MD	Ok,M
10	BFB	BFB	VX045533.D	02 Apr 2025 09:30		JC/MD	Ok
11	VSTDCCC050	VSTDCCC050	VX045534.D	02 Apr 2025 10:02	pH#Lot#V12668	JC/MD	Ok,M
12	VX0402MBL01	VX0402MBL01	VX045535.D	02 Apr 2025 10:30		JC/MD	Ok
13	VX0402WBL01	VX0402WBL01	VX045536.D	02 Apr 2025 10:53		JC/MD	Ok
14	VX0402WBS01	VX0402WBS01	VX045537.D	02 Apr 2025 11:16		JC/MD	Ok,M
15	VX0402WBSD01	VX0402WBSD01	VX045538.D	02 Apr 2025 11:44		JC/MD	Ok,M
16	Q1697-01	MW-19B-72-040125	VX045539.D	02 Apr 2025 12:07	vial A pH<2 Need 200X	JC/MD	Dilution
17	Q1697-02	IW-01-55-040125	VX045540.D	02 Apr 2025 12:30	vial A pH<2 Need 10X	JC/MD	Dilution

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX040225

Review By	John Caralone	Review On	4/2/2025 9:42:46 AM
Supervise By	Amit Patel	Supervise On	4/2/2025 2:14:39 PM
SubDirectory	VX040225	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP133559,VP133563		
Initial Calibration Stds	VP133569,VP133570,VP133571,VP133572,VP133573,VP133574		
CCC	VP133564,VP133565		
Internal Standard/PEM	VP133575		
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

18	IBLK	IBLK	VX045541.D	02 Apr 2025 12:54		JC/MD	Ok
19	Q1697-01DL	MW-19B-72-040125DL	VX045542.D	02 Apr 2025 13:21	vial B pH<2	JC/MD	Ok
20	Q1697-02DL	IW-01-55-040125DL	VX045543.D	02 Apr 2025 13:44	vial B pH<2	JC/MD	Ok
21	Q1697-03	IW-02-55-040125	VX045544.D	02 Apr 2025 14:07	Need lower dilution	JC/MD	Not Ok
22	Q1697-04	IW-02-55-040125-FD	VX045545.D	02 Apr 2025 14:31	Need lower dilution	JC/MD	Not Ok
23	Q1697-05	IW-03-55-040125	VX045546.D	02 Apr 2025 14:54	Need lower dilution	JC/MD	Not Ok
24	Q1697-07	MW-19B-72-040125	VX045547.D	02 Apr 2025 15:18	Not On Login	JC/MD	Not Ok
25	IBLK	IBLK	VX045548.D	02 Apr 2025 15:41		JC/MD	Ok
26	Q1697-03	IW-02-55-040125	VX045549.D	02 Apr 2025 16:04	vial A pH<2	JC/MD	Ok
27	Q1697-04	IW-02-55-040125-FD	VX045550.D	02 Apr 2025 16:27	vial A pH<2	JC/MD	Ok
28	Q1697-05	IW-03-55-040125	VX045551.D	02 Apr 2025 16:51	vial A pH<2	JC/MD	Ok
29	Q1697-06	TB-01-040125	VX045552.D	02 Apr 2025 17:14	vial A pH<2 TB;Hit of comp.#44	JC/MD	ReRun
30	Q1623-01	Storage-Blank-SOIL-RB	VX045553.D	02 Apr 2025 17:37	vial A pH<2	JC/MD	Ok
31	Q1623-02	Storage-Blank-WATER	VX045554.D	02 Apr 2025 18:01	vial A pH<2	JC/MD	Ok
32	Q1623-03	Storage-Blank-WATER	VX045555.D	02 Apr 2025 18:24	vial A pH<2	JC/MD	Ok
33	Q1623-04	Storage-Blank-SAMPLE	VX045556.D	02 Apr 2025 18:47	vial A pH<2	JC/MD	Ok
34	VSTDCCC050	VSTDCCC050EC	VX045557.D	02 Apr 2025 19:10		JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX040325

Review By	Semsettin Yesilyurt	Review On	4/4/2025 7:55:43 AM
Supervise By	Mahesh Dadoda	Supervise On	4/4/2025 7:58:30 AM
SubDirectory	VX040325	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133576		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133577,VP133578		

Sr #	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX045558.D	03 Apr 2025 10:01		JC/MD	Ok
2	VSTDCCC050	VSTDCCC050	VX045559.D	03 Apr 2025 10:30	pH#Lot#V12668	JC/MD	Ok,M
3	VX0403MBL01	VX0403MBL01	VX045560.D	03 Apr 2025 10:58		JC/MD	Ok
4	VX0403WBL01	VX0403WBL01	VX045561.D	03 Apr 2025 11:21		JC/MD	Ok
5	Q1697-06	TB-01-040125	VX045562.D	03 Apr 2025 11:45	vial B pH<2 TB	JC/MD	Ok
6	VX0403WBS01	VX0403WBS01	VX045563.D	03 Apr 2025 12:08		JC/MD	Ok,M
7	Q1711-01	MW-18B-56-040225	VX045564.D	03 Apr 2025 12:31	Need lower dilution	JC/MD	Not Ok
8	Q1711-04	MW-17B-55-040225	VX045565.D	03 Apr 2025 12:54	Need lower dilution	JC/MD	Not Ok
9	Q1711-07	RMW-05B-89-040225	VX045566.D	03 Apr 2025 13:18	Need Straight Run	JC/MD	Not Ok
10	VX0403WBSD01	VX0403WBSD01	VX045567.D	03 Apr 2025 13:41		JC/MD	Ok,M
11	Q1711-07	RMW-05B-89-040225	VX045568.D	03 Apr 2025 14:04	vial A pH<2	JC/MD	Ok
12	Q1711-04	MW-17B-55-040225	VX045569.D	03 Apr 2025 14:27	vial A pH<2	JC/MD	Ok
13	IBLK	IBLK	VX045570.D	03 Apr 2025 14:50		JC/MD	Ok
14	Q1711-10	TB01-040225	VX045571.D	03 Apr 2025 15:14	vial A pH<2 TB	JC/MD	Ok
15	Q1711-08	EB01-040225	VX045572.D	03 Apr 2025 15:37	vial A pH<2 EB	JC/MD	Ok
16	Q1711-05	MW-18B-56-040225-SI	VX045573.D	03 Apr 2025 16:00	screening	JC/MD	Not Ok
17	Q1711-06	MW-17B-56-040225-SI	VX045574.D	03 Apr 2025 16:23	screening	JC/MD	Not Ok
18	Q1711-01	MW-18B-56-040225	VX045575.D	03 Apr 2025 16:47	vial A pH<2	JC/MD	Ok

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX040325

Review By	Semsettin Yesilyurt	Review On	4/4/2025 7:55:43 AM
Supervise By	Mahesh Dadoda	Supervise On	4/4/2025 7:58:30 AM
SubDirectory	VX040325	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds  CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133576  VP133577,VP133578		

19	Q1711-02MS	MW-18B-56-040225MS	VX045576.D	03 Apr 2025 17:10	Internal standard fail;Surrogate fail;Recovery failed low	JC/MD	Not Ok
20	Q1711-03MSD	MW-18B-56-040225MS	VX045577.D	03 Apr 2025 17:33	vial A pH<2	JC/MD	Ok,M
21	IBLK	IBLK	VX045578.D	03 Apr 2025 17:56		JC/MD	Ok
22	IBLK	IBLK	VX045579.D	03 Apr 2025 18:19		JC/MD	Ok
23	Q1676-01	Storage-Blank-SOIL-RB	VX045580.D	03 Apr 2025 18:43	vial A pH<2	JC/MD	Ok
24	Q1676-02	Storage-Blank-WATER	VX045581.D	03 Apr 2025 19:06	vial A pH<2	JC/MD	Ok
25	Q1676-03	Storage-Blank-WATER	VX045582.D	03 Apr 2025 19:29	vial A pH<2	JC/MD	Ok
26	Q1676-04	Storage-Blank-SAMPLE	VX045583.D	03 Apr 2025 19:52	vial A pH<2	JC/MD	Ok
27	VSTDCCC050	VSTDCCC050EC	VX045584.D	03 Apr 2025 20:15		JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX040425

Review By	John Carlone	Review On	4/7/2025 9:58:56 AM
Supervise By	Mahesh Dadoda	Supervise On	4/7/2025 12:14:08 PM
SubDirectory	VX040425	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133596		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133597,VP133598		

Sr #	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX045585.D	04 Apr 2025 09:31		JC/MD	Ok
2	VSTDCCC050	VSTDCCC050	VX045586.D	04 Apr 2025 10:00	pH#Lot#V12668	JC/MD	Ok,M
3	VX0404MBL01	VX0404MBL01	VX045587.D	04 Apr 2025 10:28		JC/MD	Ok
4	VX0404WBL01	VX0404WBL01	VX045588.D	04 Apr 2025 10:51		JC/MD	Ok
5	VX0404WBS01	VX0404WBS01	VX045589.D	04 Apr 2025 11:14		JC/MD	Ok,M
6	VX0404WBSD01	VX0404WBSD01	VX045590.D	04 Apr 2025 11:40		JC/MD	Ok,M
7	Q1711-02MS	MW-18B-56-040225MS	VX045591.D	04 Apr 2025 12:04	vial A pH<2	JC/MD	Ok,M
8	IBLK	IBLK	VX045592.D	04 Apr 2025 12:27		JC/MD	Ok
9	Q1716-01	MOD-FOR-LRSA	VX045593.D	04 Apr 2025 12:50	vial A pH<2	JC/MD	Ok
10	Q1731-04	RMW-03B-90-040325	VX045594.D	04 Apr 2025 13:13	RUN@40X	JC/MD	Not Ok
11	Q1731-01	RMW-01B-82-040325	VX045595.D	04 Apr 2025 13:37	Need Straight Run	JC/MD	Not Ok
12	Q1731-02	RMW-04B-91-040325	VX045596.D	04 Apr 2025 14:00	Need Straight Run	JC/MD	Not Ok
13	Q1731-03	RMW-01B-82-040325-F	VX045597.D	04 Apr 2025 14:23	Need Straight Run	JC/MD	Not Ok
14	IBLK	IBLK	VX045598.D	04 Apr 2025 14:46		JC/MD	Ok
15	Q1731-07	TB01-040325	VX045599.D	04 Apr 2025 15:10	vial A pH<2 TB	JC/MD	Ok
16	Q1731-05	EB01-040325	VX045600.D	04 Apr 2025 15:33	vial A pH<2 EB	JC/MD	Ok
17	PB167448TB	PB167448TB	VX045601.D	04 Apr 2025 15:56		JC/MD	Ok
18	PB167448ZHE#01	PB167448ZHE#01	VX045602.D	04 Apr 2025 16:19		JC/MD	Ok

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX040425

Review By	John Caralone	Review On	4/7/2025 9:58:56 AM
Supervise By	Mahesh Dadoda	Supervise On	4/7/2025 12:14:08 PM
SubDirectory	VX040425	HP Acquire Method	HP Processing Method 82X040225W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds  CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133596  VP133597,VP133598		

19	PB167448ZHE#02	PB167448ZHE#02	VX045603.D	04 Apr 2025 16:42		JC/MD	Ok
20	PB167448ZHE#03	PB167448ZHE#03	VX045604.D	04 Apr 2025 17:06		JC/MD	Ok
21	PB167448ZHE#04	PB167448ZHE#04	VX045605.D	04 Apr 2025 17:29		JC/MD	Ok
22	PB167448ZHE#05	PB167448ZHE#05	VX045606.D	04 Apr 2025 17:52		JC/MD	Ok,M
23	Q1694-04	TP-18	VX045607.D	04 Apr 2025 18:15	vial A pH#5.0	JC/MD	Ok
24	Q1695-04	TT-2	VX045608.D	04 Apr 2025 18:38	vial A pH#5.0	JC/MD	Ok
25	Q1695-08	TT-3	VX045609.D	04 Apr 2025 19:01	vial A pH#5.0	JC/MD	Ok
26	Q1712-04	Z-05A	VX045610.D	04 Apr 2025 19:24	vial A pH#5.0	JC/MD	Ok
27	Q1712-08	TT-7	VX045611.D	04 Apr 2025 19:48	vial A pH#5.0	JC/MD	Ok
28	VSTDCCC050	VSTDCCC050EC	VX045612.D	04 Apr 2025 20:11		JC/MD	Ok,M

M : Manual Integration

## Prep Standard - Chemical Standard Summary

**Order ID :** Q1711

**Test :** VOCMS Group3

**Prepbatch ID :**

**Sequence ID/Qc Batch ID:** vx040325,VX040425,

**Standard ID :**

VP131746,VP131767,VP132035,VP132096,VP133174,VP133342,VP133544,VP133576,VP133577,VP133578,VP133596,VP133597,VP133598,

**Chemical ID :**

V13391,V13457,V13460,V13465,V13466,V13706,V14154,V14289,V14431,V14435,V14501,V14502,V14523,V14524,V14613,V14614,V14615,V14630,V14631,V14632,V14633,V14719,V14720,V14726,V14744,V14753,V14804,V14805,V14842,V14883,V14896,V14897,V14898,V14899,W3112,

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
247	8260 Internal Standard, 250PPM	<a href="#">VP131746</a>	11/22/2024	05/18/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 11/23/2024

FROM 0.50000ml of V14289 + 49.50000ml of V14154 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
218	BFB, 25PPM	<a href="#">VP131767</a>	11/22/2024	05/18/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 11/27/2024

FROM 0.50000ml of V13391 + 49.50000ml of V14154 = Final Quantity: 50.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1810	8260 Working Std(2-CVE)-800ppm	<a href="#">VP132035</a>	12/10/2024	06/10/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 12/12/2024

**FROM** 1.00000ml of V14630 + 1.00000ml of V14631 + 1.00000ml of V14632 + 1.00000ml of V14633 + 46.00000ml of V14614 = Final  
Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
719	8260 Working STD (BCM)-First source, 400PPM	<a href="#">VP132096</a>	12/12/2024	06/10/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 12/19/2024

**FROM** 1.00000ml of V13465 + 1.00000ml of V13466 + 1.50000ml of V13457 + 1.50000ml of V13460 + 20.00000ml of V14614 = Final  
Quantity: 25.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
617	8260 Surrogate, 400PPM	<a href="#">VP133174</a>	02/27/2025	08/27/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 03/04/2025

FROM 0.40000ml of V13706 + 24.60000ml of V14613 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
51	8260 Working STD (Acrolein) -first source, 800PPM	<a href="#">VP133342</a>	03/18/2025	04/17/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 03/20/2025

FROM 1.00000ml of V14896 + 1.00000ml of V14897 + 1.00000ml of V14898 + 1.00000ml of V14899 + 21.00000ml of V14883 = Final Quantity: 25.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
257	8260 Calibration Working STD Mix-First source, 160PPM	<a href="#">VP133544</a>	04/01/2025	05/10/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 04/03/2025
<b>FROM</b>	0.40000ml of V14842 + 1.00000ml of V14431 + 1.00000ml of V14435 + 1.00000ml of V14501 + 1.00000ml of V14502 + 1.00000ml of V14523 + 1.00000ml of V14524 + 1.00000ml of V14726 + 1.00000ml of V14744 + 1.00000ml of V14753 + 1.00000ml of V14804 + 1.00000ml of V14805 + 1.50000ml of V14719 + 1.50000ml of V14720 + 10.60000ml of V14615 = Final Quantity: 25.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
589	BFB TUNE CHECK	<a href="#">VP133576</a>	04/03/2025	04/04/2025	John Carlone	None	None	Mahesh Dadoda 04/05/2025
<b>FROM</b>	39.98400ml of W3112 + 0.01600ml of VP131767 = Final Quantity: 40.000 ml							

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	<a href="#">VP133577</a>	04/03/2025	04/04/2025	John Carlone	None	None	Mahesh Dadoda 04/05/2025

FROM 39.94450ml of W3112 + 0.00500ml of VP132096 + 0.00500ml of VP133174 + 0.00800ml of VP131746 + 0.01250ml of VP132035 + 0.01250ml of VP133342 + 0.01250ml of VP133544 = Final Quantity: 40.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	<a href="#">VP133578</a>	04/03/2025	04/04/2025	John Carlone	None	None	Mahesh Dadoda 04/05/2025

FROM 39.94450ml of W3112 + 0.00500ml of VP132096 + 0.00500ml of VP133174 + 0.00800ml of VP131746 + 0.01250ml of VP132035 + 0.01250ml of VP133342 + 0.01250ml of VP133544 = Final Quantity: 40.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
589	BFB TUNE CHECK	<a href="#">VP133596</a>	04/04/2025	04/05/2025	John Carlone	None	None	Mahesh Dadoda 04/07/2025

FROM 39.98400ml of W3112 + 0.01600ml of VP131767 = Final Quantity: 40.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	<a href="#">VP133597</a>	04/04/2025	04/05/2025	John Carlone	None	None	Mahesh Dadoda 04/07/2025

FROM 39.94450ml of W3112 + 0.00500ml of VP132096 + 0.00500ml of VP133174 + 0.00800ml of VP131746 + 0.01250ml of VP132035 + 0.01250ml of VP133342 + 0.01250ml of VP133544 = Final Quantity: 40.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	<a href="#">VP133598</a>	04/04/2025	04/05/2025	John Carlone	None	None	Mahesh Dadoda 04/07/2025
<u>FROM</u>	39.94450ml of W3112 + 0.00500ml of VP132096 + 0.00500ml of VP133174 + 0.00800ml of VP131746 + 0.01250ml of VP132035 + 0.01250ml of VP133342 + 0.01250ml of VP133544 = Final Quantity: 40.000 ml							

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30067 / BFB tuneing solution	A0191805	11/22/2025	11/22/2024 / SAM	01/13/2023 / SAM	V13391
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13457
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13460
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13465
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13466
Restek	555582 / Custom Mixture, 8260 A/B Surrogate Mix [CS 5179-2]	A0196865	02/27/2026	02/27/2025 / SAM	04/12/2023 / SAM	V13706

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	05/18/2025	11/18/2024 / pedro	02/06/2024 / SAM	V14154
Restek	555581 / Custom Standard, 8260 Internal Std [CS 5179-1]	A0210184	11/22/2025	11/22/2024 / SAM	04/15/2024 / SAM	V14289
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0209618	09/20/2025	03/20/2025 / SAM	08/15/2024 / SAM	V14431
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0209618	09/20/2025	03/20/2025 / SAM	08/15/2024 / SAM	V14435
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	09/20/2025	03/20/2025 / SAM	09/17/2024 / SAM	V14501
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	09/20/2025	03/20/2025 / SAM	09/17/2024 / SAM	V14502

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	09/20/2025	03/20/2025 / SAM	09/18/2024 / SAM	V14523
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	09/20/2025	03/20/2025 / SAM	09/18/2024 / SAM	V14524
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	08/27/2025	02/27/2025 / SAM	11/26/2024 / SAM	V14613
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	06/10/2025	12/10/2024 / SAM	11/26/2024 / SAM	V14614
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	09/19/2025	03/19/2025 / SAM	11/26/2024 / SAM	V14615
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14630

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14631
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14632
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14633
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	09/20/2025	03/20/2025 / SAM	12/17/2024 / SAM	V14719
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	09/20/2025	03/20/2025 / SAM	12/17/2024 / SAM	V14720
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	07/30/2025	01/30/2025 / SAM	12/17/2024 / SAM	V14726

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	08/27/2025	02/27/2025 / SAM	12/17/2024 / SAM	V14744
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	07/30/2025	01/30/2025 / SAM	12/17/2024 / SAM	V14753
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE LOTS	A0220471	09/20/2025	03/20/2025 / SAM	01/08/2025 / SAM	V14804
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE LOTS	A0220471	09/20/2025	03/20/2025 / SAM	01/08/2025 / SAM	V14805
Restek	30470 / VOA Stock Solution, tert-butanol std, 1mL, P&TM	A0217535	08/27/2025	02/27/2025 / SAM	01/21/2025 / SAM	V14842
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	10/25/2025	02/19/2025 / Jaswal	04/22/2024 / Jaswal	V14883

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	031725	04/17/2025	03/18/2025 / SAM	03/18/2025 / SAM	V14896


Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	031725	04/17/2025	03/18/2025 / SAM	03/18/2025 / SAM	V14897

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	031725	04/17/2025	03/18/2025 / SAM	03/18/2025 / SAM	V14898

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	031725	04/17/2025	03/18/2025 / SAM	03/18/2025 / SAM	V14899

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis

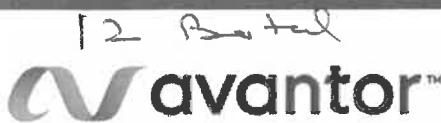

Material No.: 9077-02  
Batch No.: 22L0562016  
Manufactured Date: 2022-10-26  
Expiration Date: 2025-10-25  
Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier  
Vice President Global Quality

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis

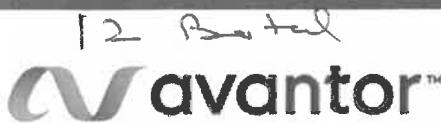

Material No.: 9077-02  
Batch No.: 22L0562016  
Manufactured Date: 2022-10-26  
Expiration Date: 2025-10-25  
Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier  
Vice President Global Quality

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis

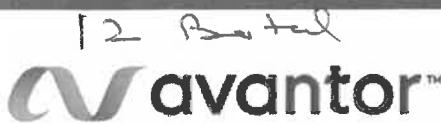

Material No.: 9077-02  
Batch No.: 22L0562016  
Manufactured Date: 2022-10-26  
Expiration Date: 2025-10-25  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier  
Vice President Global Quality

Ree 09/17/24

## CERTIFIED WEIGHT REPORT

Part Number: 95317  
 Lot Number: 021624  
 Description: Universal VOA Mixture  
 69 components

Solvent(s): Lot#  
 Methanol EG359-USQ12

Expiration Date: 02/2027  
 Recommended Storage: Freeze (0 °C)

Nominal Concentration (ug/mL): 2000NIST Test ID#: 8UTBWeight(s) shown below were combined and diluted to (mL): 100.0 0.021 Flask Uncertainty

5E-05 Balance Uncertainty

Compound	(RM#)	Lot Number	Dil. Factor	Initial Vol. (mL)	Initial Conc. (ug/mL)	Nominal Conc. (ug/mL)	Purity (%)	Purity Uncertainty	Uncertainty Pipette (mL)	Target Weight(g)	Actual Weight(g)	Actual Conc. (ug/mL)	Actual Conc. (ug/mL) (+/-) (ug/mL)	Expanded Uncertainty	SDS Information
	Part Number											CAS#	OSHA PEL (TWA)	LD50	
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8	40 ppm (70mg/m <sup>3</sup> /8H) orl-rat 2400mg/kg
2. Allyl chloride (3-Chloropropene)	(0325)	102398	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1	1 ppm (3mg/m <sup>3</sup> /8H) orl-rat 700mg/kg
3. Carbon disulfide	(0600)	MKCR8581	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.8	8.1	75-15-0	4 ppm (12mg/m <sup>3</sup> ) (skin) orl-rat 1200mg/kg
4. cis-1,4-Dichloro-2-butene	(1198)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21058	0.21069	2001.1	8.5	1478-11-6	N/A
5. trans-1,4-Dichloro-2-butene	(0486)	MKBP6041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20748	2001.7	8.4	110-57-6	N/A
6. Diethyl ether	(0153)	K18CA5000K	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7	N/A
7. Ethyl methacrylate	(0381)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2	N/A
8. Iodomethane	(0489)	SHBF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20108	0.20121	2001.5	8.2	74-88-4	5 ppm (28mg/m <sup>3</sup> /8H) (skin) orl-rat 14800mg/kg
9. 2-Methyl-1-propanol	(0445)	18241EB	NA	NA	NA	2000	99.5	0.2	NA	0.20108	0.20120	2001.4	8.1	78-83-1	50 ppm (150mg/m <sup>3</sup> /8H) orl-rat 240mg/kg
10. Methacrylonitrile	(0442)	0042ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	126-98-7	1 ppm (3mg/m <sup>3</sup> /8H) (skin) orl-rat 120mg/kg
11. Methyl acrylate	(1075)	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3	10 ppm (35mg/m <sup>3</sup> /8H) (skin) orl-rat 277mg/kg
12. Methyl methacrylate	(0404)	MKBW6137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	80-82-6	100 ppm (410mg/m <sup>3</sup> /8H) orl-rat 787mg/kg
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	98-85-3	1 ppm (5mg/m <sup>3</sup> /8H) (skin) orl-rat 780mg/kg
14. 2-Nitropropane	(0481)	14002JK	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	79-48-9	10 ppm (35mg/m <sup>3</sup> /8H) orl-rat 720mg/kg
15. Pentachloroethane	(0450)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.6	8.3	78-01-7	N/A
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18590	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1	1000 ppm (7600mg/m <sup>3</sup> /8H) orl-rat 45mg/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1988.6	22.8	75-27-4	N/A
18. Dibromochloromethane	35171	101623	0.05	5.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1	N/A
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	156-59-2	N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	23.0	156-60-5	N/A
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-09-2	500 ppm orl-rat 820mg/kg
22. 1,1-Dichloroethene	32251	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.7	20.4	75-35-4	1 ppm (4mg/m <sup>3</sup> /8H) orl-rat 200mg/kg
23. Bromoform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2	0.5 ppm (5mg/m <sup>3</sup> ) (skin) orl-rat 933mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	2 ppm (12.8mg/m <sup>3</sup> /8H) orl-rat 235mg/kg
25. Chloroform	95321	020724	0.10	10.00	20024.0	2000	NA	NA	0.042	NA	NA	1999.8	20.4	67-83-3	60 ppm (240mg/m <sup>3</sup> ) (CL) orl-rat 90mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20002.9	2000	NA	NA	0.042	NA	NA	2001.9	20.5	78-85-3	100 ppm (410mg/m <sup>3</sup> /8H) orl-rat 108mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-34-3	100 ppm orl-rat 725mg/kg
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	78-87-5	75 ppm (350mg/m <sup>3</sup> /8H) orl-rat 1847mg/kg
29. Tetrachloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	1999.8	20.8	59-20-7	N/A
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	127-18-4	25 ppm (170mg/m <sup>3</sup> /8H) (final) orl-rat 2620mg/kg
31. 1,2-Dibromo-3-chloropropane	35161	112322	0.05	5.00	40018.5	2000	NA	NA	0.017	NA	NA	1999.8	20.5	71-55-6	350 ppm (1900mg/m <sup>3</sup> /8H) orl-rat 10300mg/kg
32. 1,2-Dibromopentane	35161	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.3	22.9	98-12-8	0.001 ppm orl-rat 170mg/kg
33. 1,2-Dichloroethane	35161	112322	0.05	5.00	40018.0	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-03-4	20 ppm (8H) orl-rat 108mg/kg
34. 1,2-Dichloropropane	35161	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-06-2	50 ppm (BH) orl-rat 670mg/kg
35. 1,2-Dichloropropane	35161	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	2002.0	22.9	83-20-6	75 ppm (350mg/m <sup>3</sup> /8H) orl-mus 1847mg/kg
36. 1,1-Dichloropropene	35161	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	142-29-9	N/A orl-mus 3600mg/kg
37. cis-1,3-Dichloropropene	35161	112322	0.05	5.00	40010.0	2000	NA	NA	0.017	NA	NA	2000.1	28.7	583-56-6	N/A
38. trans-1,3-Dichloropropene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10081-01-5	N/A
39. Hexachloro-1,3-butadiene	35161	112322	0.05	5.00	40021.9	2000	NA	NA	0.017	NA	NA	2000.4	23.0	1061-02-6	N/A
40. 1,1,1,2-Tetrachloroethane	35161	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-08-3	0.02 ppm (0.24mg/m <sup>3</sup> /8H) orl-rat 82mg/kg
41. 1,1,2,2-Tetrachloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.1	22.9	830-20-6	N/A orl-rat 670mg/kg
42. 1,1,2-Tetrafluoroethane	35161	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.9	22.9	78-34-5	5 ppm (55mg/m <sup>3</sup> /8H) (skin) orl-rat 600mg/kg
43. Trichloroethene	35161	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	1999.8	23.0	78-00-5	10 ppm (45mg/m <sup>3</sup> /8H) (skin) orl-rat 833mg/kg
44. 1,2,2-Trichloropropane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.9	22.9	78-01-6	50 ppm (270mg/m <sup>3</sup> /8H) orl-mus 240mg/kg
45. Benzene	35162	050823	0.05	5.00	40005.0	2000	NA	NA	0.017	NA	NA	1999.9	22.9	98-18-4	10 ppm (60mg/m <sup>3</sup> /8H) orl-rat 149.8mg/kg
46. Bromobenzene	35162	050823	0.05	5.00	40006.9	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2	1 ppm orl-rat 480mg/kg
47. n-Butyl benzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-1	N/A orl-rat 269mg/kg
48. Ethyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8	N/A
49. p-Isopropyl tolue	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4	100 ppm (435mg/m <sup>3</sup> /8H) orl-rat >2000mg/kg
50. Naphthalene	35162	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	99-57-6	N/A orl-rat 475mg/kg
51. Styrene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3	10 ppm (50mg/m <sup>3</sup> /8H) orl-rat 490mg/kg
52. Toluene	35162	050823	0.05	5.00	40008.2	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5	100 ppm orl-rat 5000mg/kg
53. 1,2,3-Trichlorobenzene	35162	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	108-88-3	200 ppm orl-rat 5000mg/kg
54. 1,2,4-Trichlorobenzene	35162	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1	5 ppm (CL) (40mg/m <sup>3</sup> ) orl-rat 756mg/kg
55. 1,3,5-Trimethylbenzene	35162	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.6	23.0	95-63-6	N/A orl-rat 5g/kg
56. m-Xylene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-67-8	N/A orl-rat 5000mg/kg
57. <i>t</i> -Butyl benzene	35163	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-38-3	100 ppm (435mg/m <sup>3</sup> /8H) orl-rat 5g/kg
58. <i>sec</i> -Butyl benzene	35163	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.8	22.9	98-06-6	N/A orl-rat 1083mg/kg
59. <i>tert</i> -Butyl benzene	35163	101923	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	135-98-8	N/A orl-rat 2240mg/kg



Run 16, "P95317 L021624 [2000µg/mL in MeOH]"

Run Length: 60.00 min, 35998 points at 10 points/second.

Created: Sat, Feb 17, 2024 at 8:56:46 AM.

Sampled: Sequence "021624-GC5-M1", Method "GC5-M1".

Analyzed using Method "GC5-M1".

Comments

GC5-M1 Analysis by Candice Warren

Column ID SPB-Vocel 105 meter X 0.53mm X 3.0µm film thickness

Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,


Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.

Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.).

Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.

FID Signal = Edaq Channel 1

Standard injection = 0.5µL, Range=3

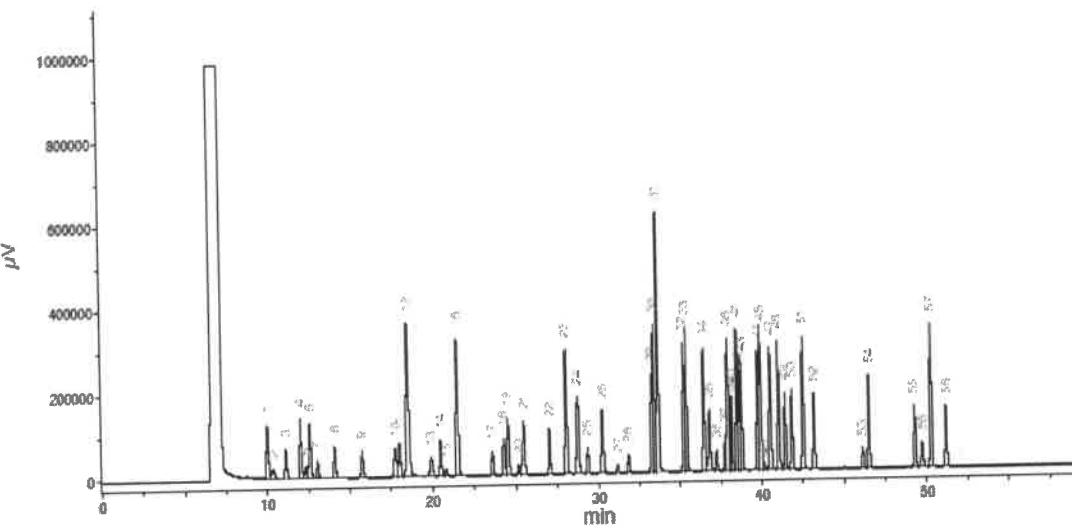

Peak #	Name	FID RT (min.)
1	Ether	0.97
2	1,1,2-Trichloro-1,2,2-trifluoroethane	10.33
3	1,1-Dichloroethane	11.10
4	Acetonitrile	12.00
5	Iodomethane	12.21
6	Allyl chloride	12.56
7	Carbon disulfide/Methylene chloride	13.74
8	trans-1,2-Dichloroethane	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,3-Dichloropropene	18.60
12	Methyl vinyl ketone/Methyl acrylate/Chloroform	18.49
13	Isobutanol/1,1,1-Trichloroethane	19.91
14	1,1-Dichloropropane	20.79
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.48
17	Trichloroethane	23.68
18	1,2-Dichloropropane	24.26
19	Methyl methacrylate	24.52
20	Bromoacetylbenzene	25.13
21	Dibromoethane/1,2-Dibromoethane	25.48
22	cis-1,3-Dichloropropene	27.07
23	Toluene	28.03
24	Ethyl methacrylate/trans-1,3-Dichloropropene	29.73
25	1,1,2-Trichloroethane	29.94
26	Toluene/butanone/1,2-Dichloropropane	30.84
27	Dibromochloromethane	31.16
28	1,2-Dibromoethane	31.89
29	Chlorobutane	33.20
30	Ethyleneglycerol,1,1,2-Tetraacetylethane	33.60
31	m-Xylene/p-Xylene	33.89
32	o-Xylene	33.93
33	Glyrene	35.94
34	Isopropylbenzene/Bromoform	36.48
35	cis-1,4-Dichloro-1-butene	36.60
36	1,1,2,2-Tetrachloroethane	37.23
37	j,2,3-Trichloropropene	37.77
38	n-Propylbenzene	37.92
39	trans-1,3-Dichloro-3-butene	38.05
40	Bromobenzene	38.14
41	1,3,5-Trimethylbenzene	38.50
42	2-Chlorotoluene	38.63
43	4-Chlorotoluene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	40.91
46	Pentachloroethane	40.17
47	tert-Butylbenzene	40.53
48	p Isopropyltoluene	41.03
49	1,3-Dichloropropane	41.13
50	1,4-Dichlorobenzene	41.83
51	n-Butylbenzene	42.62
52	1,2-Dichlorobenzene	42.16
53	1,2-Dibromo-3-chloropropane	46.17
54	Norbornane	46.49
55	1,2,4-Trimethoxybenzene	49.26
56	Hexachlorobutadiene	49.32
57	Naphthalene	50.16
58	1,2,3-Trichlorobenzene	51.16



Boiling Point	65°C	Specific Gravity (H <sub>2</sub> O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

Ree 09/17/24

## CERTIFIED WEIGHT REPORT

Part Number: 95317  
 Lot Number: 021624  
 Description: Universal VOA Mixture  
 69 components

Solvent(s): Lot#  
 Methanol EG359-USQ12

Expiration Date: 02/2027  
 Recommended Storage: Freeze (0 °C)

Nominal Concentration (ug/mL): 2000NIST Test ID#: 8UTBWeight(s) shown below were combined and diluted to (mL): 100.0 0.021 Flask Uncertainty

5E-05 Balance Uncertainty

Compound	(RM#)	Lot Number	Dil. Factor	Initial Vol. (mL)	Initial Conc. (ug/mL)	Nominal Conc. (ug/mL)	Purity (%)	Purity Uncertainty	Uncertainty Pipette (mL)	Target Weight(g)	Actual Weight(g)	Actual Conc. (ug/mL)	Actual Conc. (ug/mL) (+/-) (ug/mL)	Expanded Uncertainty	SDS Information
	Part Number											CAS#	OSHA PEL (TWA)	LD50	
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8	40 ppm (70mg/m <sup>3</sup> /8H) orl-rat 2400mg/kg
2. Allyl chloride (3-Chloropropene)	(0325)	102398	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1	1 ppm (3mg/m <sup>3</sup> /8H) orl-rat 700mg/kg
3. Carbon disulfide	(0600)	MKCR8581	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.8	8.1	75-15-0	4 ppm (12mg/m <sup>3</sup> ) (skin) orl-rat 1200mg/kg
4. cis-1,4-Dichloro-2-butene	(1198)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21058	0.21069	2001.1	8.5	1478-11-6	N/A
5. trans-1,4-Dichloro-2-butene	(0486)	MKBP6041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20748	2001.7	8.4	110-57-6	N/A
6. Diethyl ether	(0153)	K18CA5000K	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7	N/A
7. Ethyl methacrylate	(0381)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2	N/A
8. Iodomethane	(0489)	SHBF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20108	0.20121	2001.5	8.2	74-88-4	5 ppm (28mg/m <sup>3</sup> /8H) (skin) orl-rat 14800mg/kg
9. 2-Methyl-1-propanol	(0445)	18241EB	NA	NA	NA	2000	99.5	0.2	NA	0.20108	0.20120	2001.4	8.1	78-83-1	50 ppm (150mg/m <sup>3</sup> /8H) orl-rat 240mg/kg
10. Methacrylonitrile	(0442)	0042ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	126-98-7	1 ppm (3mg/m <sup>3</sup> /8H) (skin) orl-rat 120mg/kg
11. Methyl acrylate	(1075)	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3	10 ppm (35mg/m <sup>3</sup> /8H) (skin) orl-rat 277mg/kg
12. Methyl methacrylate	(0404)	MKBW6137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	80-82-6	100 ppm (410mg/m <sup>3</sup> /8H) orl-rat 787mg/kg
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	98-85-3	1 ppm (5mg/m <sup>3</sup> /8H) (skin) orl-rat 780mg/kg
14. 2-Nitropropane	(0481)	14002JK	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	79-48-9	10 ppm (35mg/m <sup>3</sup> /8H) orl-rat 720mg/kg
15. Pentachloroethane	(0450)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.6	8.3	78-01-7	N/A
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18590	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1	1000 ppm (7600mg/m <sup>3</sup> /8H) orl-rat 45mg/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1988.6	22.8	75-27-4	N/A
18. Dibromochloromethane	35171	101623	0.05	5.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1	N/A
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	156-59-2	N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	23.0	156-60-5	N/A
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.5	22.9	75-09-2	500 ppm orl-rat 820mg/kg
22. 1,1-Dichloroethene	32251	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.7	20.4	75-35-4	1 ppm (4mg/m <sup>3</sup> /8H) orl-rat 200mg/kg
23. Bromoform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2	0.5 ppm (5mg/m <sup>3</sup> ) (skin) orl-rat 933mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2	2 ppm (12.8mg/m <sup>3</sup> /8H) orl-rat 235mg/kg
25. Chloroform	95321	020724	0.10	10.00	20024.0	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	1 ppm (4mg/m <sup>3</sup> /8H) orl-rat 230mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20002.9	2000	NA	NA	0.042	NA	NA	2001.9	20.5	67-88-3	60 ppm (240mg/m <sup>3</sup> ) (CL) orl-rat 90mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-85-3	N/A
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	2002.0	22.9	75-34-3	100 ppm orl-rat 725mg/kg
29. Tetrachloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	1999.8	20.4	59-20-7	N/A
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	2018.9	20.8	127-18-4	25 ppm (170mg/m <sup>3</sup> /8H)(final) orl-rat 262mg/kg
31. 1,2-Dibromo-3-chloropropane	35161	112322	0.05	5.00	40018.5	2000	NA	NA	0.017	NA	NA	1999.8	20.5	71-55-6	350 ppm (1900mg/m <sup>3</sup> /8H) orl-rat 10300mg/kg
32. 1,2-Dibromopentane	35161	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.3	22.9	98-12-8	0.001 ppm orl-rat 170mg/kg
33. 1,2-Dichloroethane	35161	112322	0.05	5.00	40018.0	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-03-4	20 ppm (8H) orl-rat 108mg/kg
34. 1,2-Dichloropropane	35161	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-06-2	50 ppm (BH) orl-rat 670mg/kg
35. 1,2-Dichloropropane	35161	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5	75 ppm (350mg/m <sup>3</sup> /8H) orl-rat 1847mg/kg
36. 1,1-Dichloropropene	35161	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	142-29-9	N/A orl-mus 3600mg/kg
37. cis-1,3-Dichloropropene	35161	112322	0.05	5.00	40010.0	2000	NA	NA	0.017	NA	NA	2000.1	28.7	583-58-6	N/A
38. trans-1,3-Dichloropropene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10081-01-5	N/A
39. Hexachloro-1,3-butadiene	35161	112322	0.05	5.00	40021.9	2000	NA	NA	0.017	NA	NA	2000.4	23.0	106-01-2	N/A
40. 1,1,1,2-Tetrachloroethane	35161	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-08-3	0.02 ppm (0.24mg/m <sup>3</sup> /8H) orl-rat 82mg/kg
41. 1,1,2,2-Tetrachloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.1	22.9	830-20-6	N/A orl-rat 670mg/kg
42. 1,1,2-Tetrafluoroethane	35161	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.9	22.9	78-34-5	5 ppm (55mg/m <sup>3</sup> /8H) (skin) orl-rat 600mg/kg
43. Trichloroethene	35161	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	1999.8	23.0	78-00-5	10 ppm (45mg/m <sup>3</sup> /8H) (skin) orl-rat 833mg/kg
44. 1,2,2-Trichloropropane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.9	22.9	78-01-6	50 ppm (270mg/m <sup>3</sup> /8H) orl-mus 240mg/kg
45. Benzene	35162	050823	0.05	5.00	40005.0	2000	NA	NA	0.017	NA	NA	1999.9	22.9	98-18-4	10 ppm (60mg/m <sup>3</sup> /8H) orl-rat 149.8mg/kg
46. Bromobenzene	35162	050823	0.05	5.00	40006.9	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2	1 ppm orl-rat 480mg/kg
47. n-Butyl benzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-1	N/A orl-rat 269mg/kg
48. Ethyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8	N/A
49. p-Isopropyl tolue	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4	100 ppm (435mg/m <sup>3</sup> /8H) orl-rat >2000mg/kg
50. Naphthalene	35162	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	99-57-6	N/A orl-rat 475mg/kg
51. Styrene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3	10 ppm (50mg/m <sup>3</sup> /8H) orl-rat 490mg/kg
52. Toluene	35162	050823	0.05	5.00	40008.2	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5	100 ppm orl-rat 5000mg/kg
53. 1,2,3-Trichlorobenzene	35162	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-3	200 ppm orl-rat 5000mg/kg
54. 1,2,4-Trichlorobenzene	35162	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1	5 ppm (CL) (40mg/m <sup>3</sup> ) orl-rat 756mg/kg
55. 1,3,5-Trimethylbenzene	35162	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.6	23.0	95-63-6	N/A orl-rat 5g/kg
56. m-Xylene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-67-8	N/A orl-rat 5000mg/kg
57. <i>t</i> -Butyl benzene	35163	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-38-3	100 ppm (435mg/m <sup>3</sup> /8H) orl-rat 5g/kg
58. <i>sec</i> -Butyl benzene	35163	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	98-06-6	N/A orl-rat 5g/kg
59. <i>n</i> -Butyl benzene	35163	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.8	22.9	135-98-8	N/A orl-rat 2240mg/kg
60. Chlorobenzene	35163	101923													



Run 16, "P95317 L021624 [2000µg/mL in MeOH]"

Run Length: 60.00 min, 35998 points at 10 points/second.

Created: Sat, Feb 17, 2024 at 8:56:46 AM.

Sampled: Sequence "021624-GC5M1", Method "GC5-M1".

Analyzed using Method "GC5-M1".

#### Comments

##### GC5-M1 Analysis by Candice Warren

Column ID SPB-Vocel 105 meter X 0.53mm X 3.0µm film thickness

Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,


Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.

Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.).

Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.

FID Signal = Edaq Channel 1

Standard injection = 0.5µL, Range=3

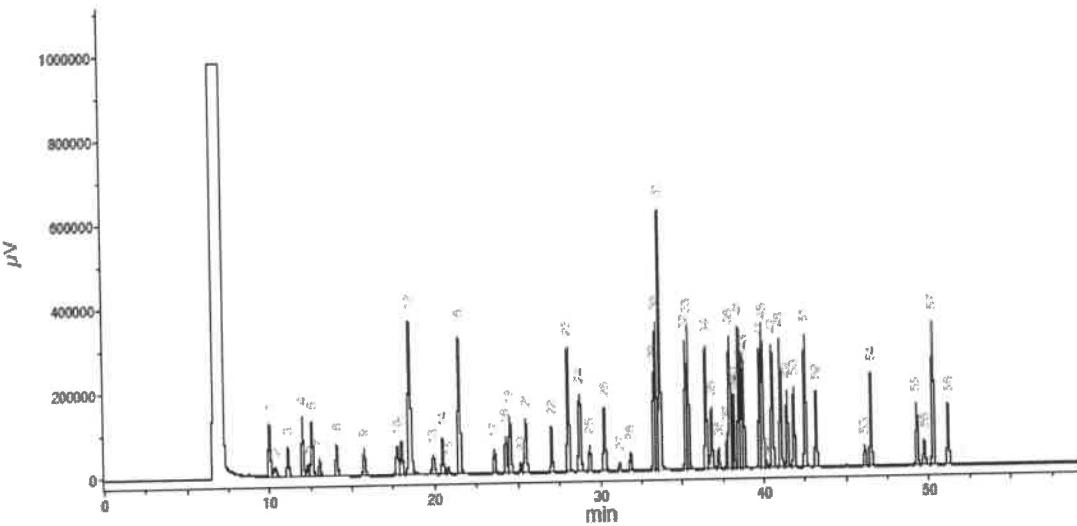

Peak #	Name	FID RT (min.)
1	Ether	0.97
2	1,1,2-Trichloro-1,2,3-trifluoropropane	10.33
3	1,1-Dichloroethane	11.10
4	Acetonitrile	12.00
5	Iodomethane	12.21
6	Allyl chloride	12.56
7	Carbon disulfide/Methylene chloride	13.74
8	trans-1,2-Dichloroethane	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,3-Dichloropropene	18.60
12	Methylacrylonitrile/Methyl acrylate/Chloroform	18.49
13	Isobutanol/1,1,1-Trichloropropane	19.91
14	1,1-Dichloropropane	20.79
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.48
17	Trichloroethane	23.68
18	1,2-Dichloropropane	24.26
19	Methyl methacrylate	24.52
20	Bromoacetylbenzene	25.13
21	Dibromoethane/1,2-Dibromoethane	25.48
22	cis-1,3-Dichloropropene	27.07
23	Toluene	28.03
24	Ethyl methacrylate/trans-1,3-Dichloropropene	29.73
25	1,1,2-Trichloroethane	29.94
26	Toluene/butanone/1,2-Dichloropropane	30.84
27	Dibromochloromethane	31.16
28	1,2-Dibromoethane	31.89
29	Chlorobutane	33.20
30	Ethylobenzenes/1,1,2-Tetrachloroethane	33.60
31	m-Xylene/p-Xylene	33.89
32	o-Xylene	33.93
33	Glyrene	35.94
34	Isopropylbenzene/Bromoform	36.48
35	cis-1,4-Dichloro-1-butene	36.60
36	1,1,2,2-Tetrachloroethane	37.23
37	j,2,3-Trichloropropene	37.77
38	n-Propylbenzene	37.92
39	trans-1,3-Dichloro-3-butene	38.05
40	Bromobenzene	38.14
41	1,3,5-Trimethylbenzene	38.50
42	2-Chlorotoluene	38.63
43	4-Chlorotoluene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	40.91
46	Pentachloroethane	40.17
47	tert-Butylbenzene	40.53
48	p Isopropyltoluene	41.03
49	1,3-Dichloropropane	41.13
50	1,4-Dichlorobenzene	41.83
51	n-Butylbenzene	42.62
52	1,2-Dichlorobenzene	42.16
53	1,2-Dibromo-3-chloropropane	46.17
54	Nitrobenzene	46.49
55	1,3,4-Trimethoxybenzene	49.26
56	Hexachlorobutadiene	49.32
57	Naphthalene	50.16
58	1,2,3-Trichlorobenzene	51.16

**Safety Data Sheet (SDS)**      GHS/OSHA Compliant**Section I Product and Company Identification****IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL**

Manufacturer's Name      ABSOLUTE STANDARDS INC  
 Address      44 Rossotto Dr.  
                   Hamden CT, 06514  
 Emergency Telephone USA & CANADA  
 Emergency Telephone International  
 Date Prepared/Revised

**1-800-535-5053**  
**1-352-323-3500**  
 January 1, 2024

**Section II - Hazards Identification****GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)**

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water

**Signal Word: DANGER****Section III - Composition**

Components (Specific Chemical Identity; Common Name(s))  
 Methanol      METHYL ALCOHOL      CAS#: 67-56-1      % (optional)  
                   > 97

**See Certified Weight Report For Other Analytes Present At Trace Quantities.****INTENDED USE: REFERENCE MATERIAL****Section IV. FIRST AID MEASURES**

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

**Section V. FIREFIGHTING MEASURES**

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media Protective equipment for fire	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide. Wear self contained breathing apparatus for fire fighting if necessary.

**Section VI. ACCIDENTAL RELEASE MEASURES**

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions Clean up	Prevent further leakage or spillage if safe to do so. Do not let product enter drains. Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

**Section VII. HANDLING AND STORAGE**

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.
Storage Conditions	Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

**Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION**

Methanol	67-56-1 TWA 200 ppm
Skin notation	TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.	
Personal protective equipment      Respiratory protection      Handle with gloves. Gloves must be inspected prior to use.      Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.	

**Section IX - Physical/Chemical Characteristics**

Boiling Point	65°C	Specific Gravity (H <sub>2</sub> O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability: Stable under recommended storage conditions.  
 Possibility of hazardous reactions: Vapours may form explosive mixture with air.  
 Conditions to avoid: Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid: Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US)  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



## Certified Reference Material CRM

Ref. 03/18/24

ANAB ISO 17034 Accredited  
AR-1539 Certificate Number  
<https://Absolutestandards.co>

## CERTIFIED WEIGHT REPORT

Part Number: 91980  
 Lot Number: 031725  
 Description: Acrolein

Solvent(s): Water Lot#  
072324Q

*5 via*  
*V14895 to*  
*V14899*

Expiration Date: 04/17/25  
 Recommended Storage: Refrigerate (4 °C)  
 Nominal Concentration ( $\mu\text{g/mL}$ ): 5000  
 NIST Test ID#: 6UTB


5E-05 Balance Uncertainty  
 0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0

<i>Lawrence Barry</i>	<u>031725</u>
Formulated By:	Lawrence Barry
<i>Pedro L. Rentas</i>	<u>031725</u>
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ( $\mu\text{g/mL}$ )	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ( $\mu\text{g/mL}$ )	Expanded Uncertainty (+/-) ( $\mu\text{g/mL}$ )	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5 $\mu\text{m}$  film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.) **Rate** = 4°C/min., **Injector Temp.** = 200°C, **Detector Temp.** = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

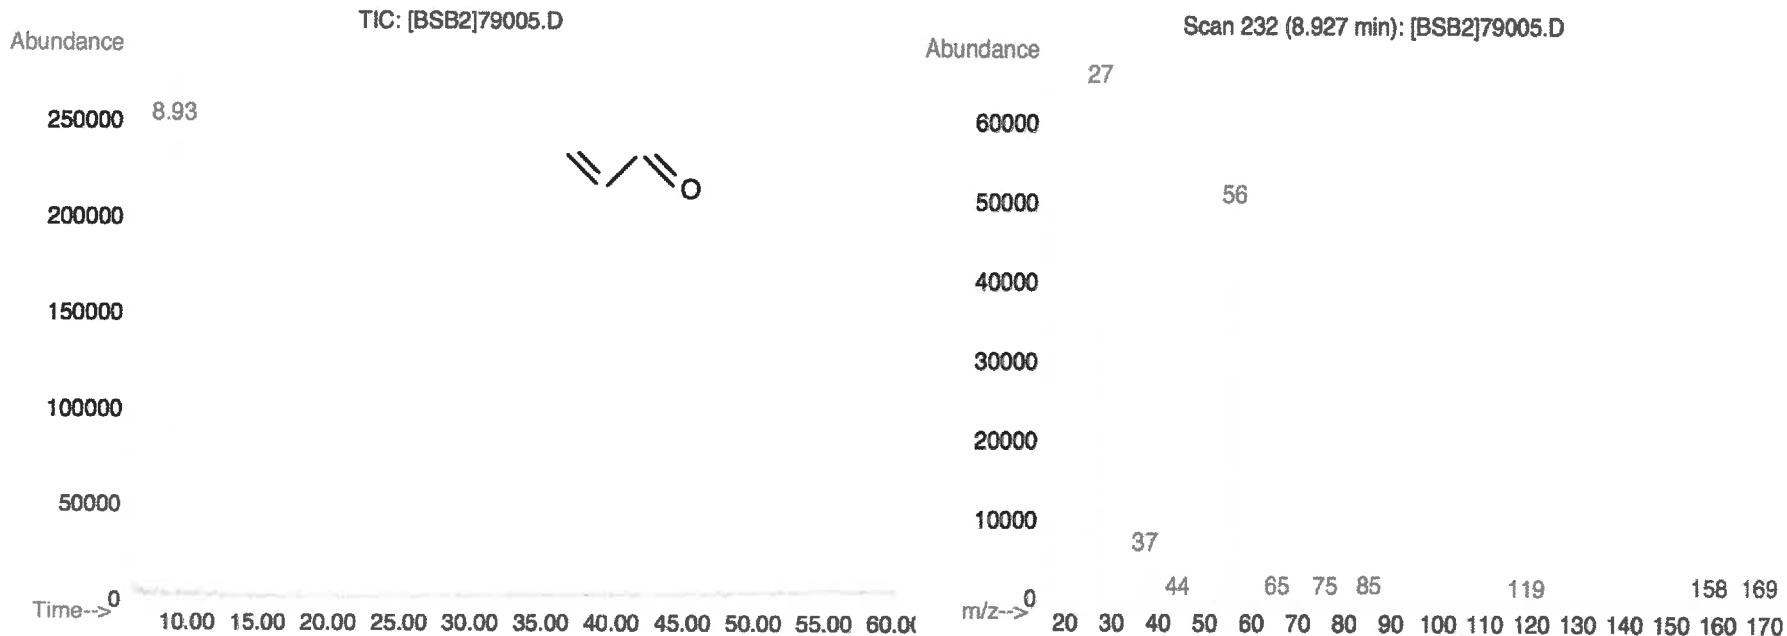

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Vapor Density (AIR = 1)	NA	Evaporation rate (Butyl Acetate = 1)	0°C
Solubility in Water	Completely miscible		NA

Appearance and Odor      CLEAR, COLORLESS LIQUID WITH SLIGHT CHEMICAL ODOR.

#### Section X. STABILITY AND REACTIVITY

Chemical stability      Stable under recommended storage conditions.  
 Possibility of hazardous reactions      NA  
 Conditions to avoid      NA  
 Materials to avoid      NA  
 Hazardous decomposition products - No data available

#### Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat      NA  
 LC50 Inhalation - Rat      NA  
 LD50 Dermal - Guinea pig      NA  
 Causes skin irritation.  
 Eye irritation

#### Section XII. ECOLOGICAL INFORMATION

LC50      NA  
 EC50      NA

#### Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

#### Section XIV. TRANSPORT INFORMATION

DOT (US)  
 Not dangerous goods  
 Proper shipping name: Water      IATA  
 Not dangerous goods  
 Proper shipping name: Water

#### Section XV. REGULATORY INFORMATION

SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

#### Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



## Certified Reference Material CRM

Ref. 03/18/24



ANAB ISO 17034 Accredited  
AR-1539 Certificate Number  
<https://Absolutestandards.co>

## CERTIFIED WEIGHT REPORT

Part Number: 91980  
Lot Number: 031725  
Description: Acrolein

Solvent(s): Water Lot# 072324Q

*5 via*  
V14895 to  
V14899

Expiration Date: 04/17/25  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration ( $\mu\text{g/mL}$ ): 5000  
NIST Test ID#: 6UTB


5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0

<i>Lawrence Barry</i>	031725
Formulated By:	Lawrence Barry
<i>Pedro L. Rentas</i>	031725
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ( $\mu\text{g/mL}$ )	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ( $\mu\text{g/mL}$ )	Expanded Uncertainty (+/-) ( $\mu\text{g/mL}$ )	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5 $\mu\text{m}$  film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.) **Rate:** 4°C/min., **Injector Temp.** = 200°C, **Detector Temp.** = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

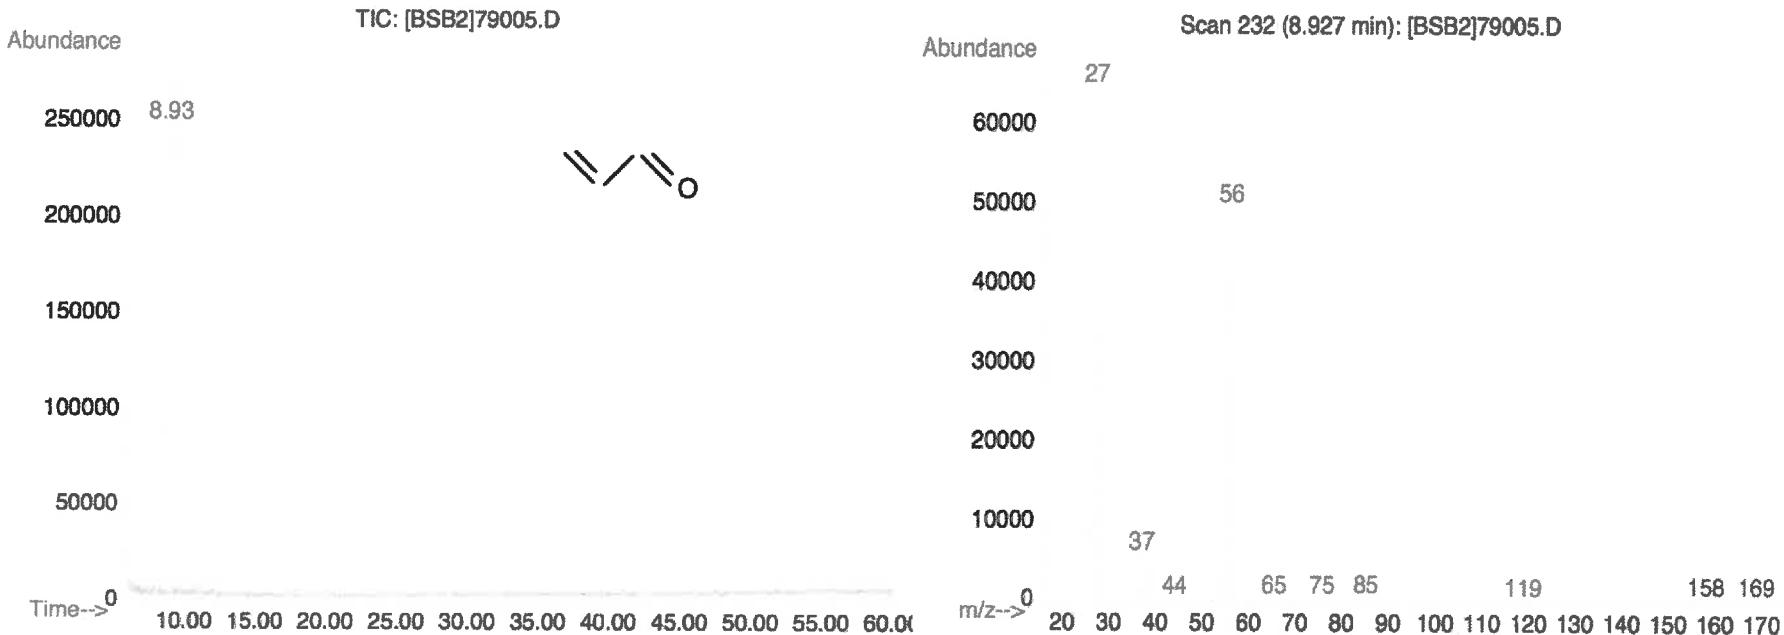

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Vapor Density (AIR = 1)	NA	Evaporation rate (Butyl Acetate = 1)	0°C
Solubility in Water	Completely miscible		NA

Appearance and Odor      CLEAR, COLORLESS LIQUID WITH SLIGHT CHEMICAL ODOR.

#### Section X. STABILITY AND REACTIVITY

Chemical stability      Stable under recommended storage conditions.  
 Possibility of hazardous reactions      NA  
 Conditions to avoid      NA  
 Materials to avoid      NA  
 Hazardous decomposition products - No data available

#### Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat      NA  
 LC50 Inhalation - Rat      NA  
 LD50 Dermal - Guinea pig      NA  
 Causes skin irritation.  
 Eye irritation

#### Section XII. ECOLOGICAL INFORMATION

LC50      NA  
 EC50      NA

#### Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

#### Section XIV. TRANSPORT INFORMATION

DOT (US)  
 Not dangerous goods  
 Proper shipping name: Water      IATA  
 Not dangerous goods  
 Proper shipping name: Water

#### Section XV. REGULATORY INFORMATION

SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

#### Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



## Certified Reference Material CRM

Ref. 03/18/24

ANAB ISO 17034 Accredited  
AR-1539 Certificate Number  
<https://Absolutestandards.co>

## CERTIFIED WEIGHT REPORT

Part Number: 91980  
 Lot Number: 031725  
 Description: Acrolein

Solvent(s): Water Lot#  
072324Q

*5 via*  
*V14895 to*  
*V14899*

Expiration Date: 04/17/25  
 Recommended Storage: Refrigerate (4 °C)  
 Nominal Concentration ( $\mu\text{g/mL}$ ): 5000  
 NIST Test ID#: 6UTB


5E-05 Balance Uncertainty  
 0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0

<i>Lawrence Barry</i>	<u>031725</u>
Formulated By:	Lawrence Barry
<i>Pedro L. Rentas</i>	<u>031725</u>
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ( $\mu\text{g/mL}$ )	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ( $\mu\text{g/mL}$ )	Expanded Uncertainty (+/-) ( $\mu\text{g/mL}$ )	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5 $\mu\text{m}$  film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.) **Rate** = 4°C/min., **Injector Temp.** = 200°C, **Detector Temp.** = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

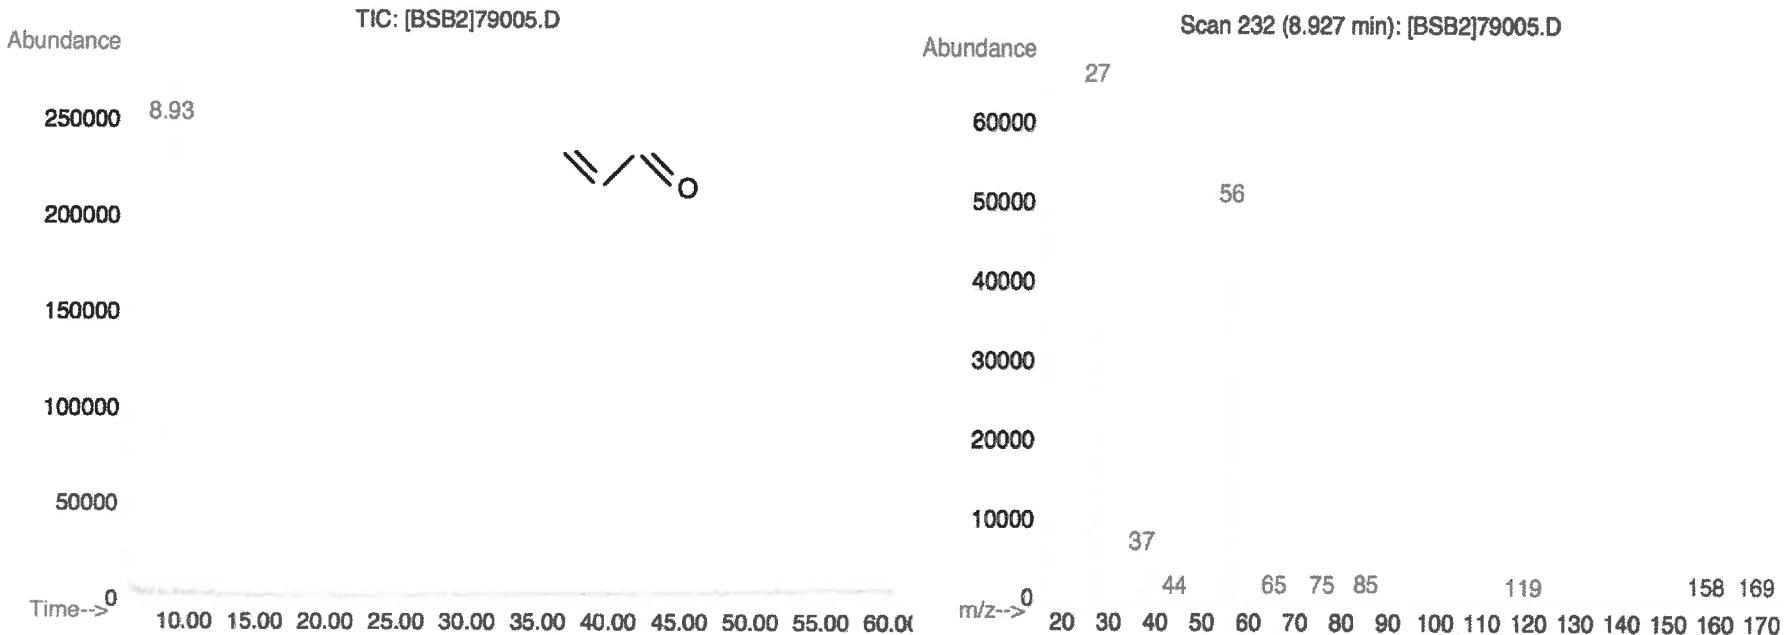

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

**Safety Data Sheet (SDS)**

GHS/OSHA Compliant

**Section I Product and Company Identification****IDENTITY ANALYTICAL STANDARD DISSOLVED IN WATER**

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	<b>1-800-535-5053</b>
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	<b>1-352-323-3500</b> January 1, 2025

**Section II - Hazards Identification****GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)**

P271	Use in ventilated area	H315	Causes skin and eye irritation.
P302,332	If on skin, wash with soap and water	P280	Use gloves, eye protection/face shield
		P305,351,338	If in eyes, remove contacts, rinse with water

**Signal Word: DANGER****Section III - Composition**

Components (Specific Chemical Identity; Common Name(s))	CAS#: 7732-18-5	% (optional) > 97
Water		

**See Certified Weight Report For Other Analytes Present At Trace Quantities.****INTENDED USE: REFERENCE MATERIAL****Section IV. FIRST AID MEASURES**

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

**Section V. FIREFIGHTING MEASURES**

Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.
Hazardous Decomposition products	Carbon oxides

**Section VI. ACCIDENTAL RELEASE MEASURES**

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.

Clean up

Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

**Section VII. HANDLING AND STORAGE**

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

**Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION**

Water	CAS#: 7732-18-5	TWA: 500 ppm
-------	-----------------	--------------

Personal protective equipment      Respiratory protection      Handle with gloves. Gloves must be inspected prior to use.      Eye protection.  
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

**Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS**

Boiling Point	100°C	Specific Gravity (H <sub>2</sub> O = 1)	1
Vapor Pressure (mm Hg)		Melting Point	

Vapor Density (AIR = 1)	NA	Evaporation rate (Butyl Acetate = 1)	0°C
Solubility in Water	Completely miscible		NA

Appearance and Odor      CLEAR, COLORLESS LIQUID WITH SLIGHT CHEMICAL ODOR.

#### Section X. STABILITY AND REACTIVITY

Chemical stability      Stable under recommended storage conditions.  
 Possibility of hazardous reactions      NA  
 Conditions to avoid      NA  
 Materials to avoid      NA  
 Hazardous decomposition products - No data available

#### Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat      NA  
 LC50 Inhalation - Rat      NA  
 LD50 Dermal - Guinea pig      NA  
 Causes skin irritation.  
 Eye irritation

#### Section XII. ECOLOGICAL INFORMATION

LC50      NA  
 EC50      NA

#### Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

#### Section XIV. TRANSPORT INFORMATION

DOT (US)  
 Not dangerous goods  
 Proper shipping name: Water      IATA  
 Not dangerous goods  
 Proper shipping name: Water

#### Section XV. REGULATORY INFORMATION

SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

#### Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



## Certified Reference Material CRM

Ref. 03/18/24

ANAB ISO 17034 Accredited  
AR-1539 Certificate Number  
<https://Absolutestandards.co>

## CERTIFIED WEIGHT REPORT

Part Number: 91980  
 Lot Number: 031725  
 Description: Acrolein

Solvent(s): Water Lot#  
072324Q

*5 via*  
*V14895 to*  
*V14899*

Expiration Date: 04/17/25  
 Recommended Storage: Refrigerate (4 °C)  
 Nominal Concentration ( $\mu\text{g/mL}$ ): 5000  
 NIST Test ID#: 6UTB


5E-05 Balance Uncertainty  
 0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0

<i>Lawrence Barry</i>	031725
Formulated By:	Lawrence Barry
<i>Pedro L. Rentas</i>	031725
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ( $\mu\text{g/mL}$ )	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ( $\mu\text{g/mL}$ )	Expanded Uncertainty (+/-) ( $\mu\text{g/mL}$ )	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5 $\mu\text{m}$  film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.) **Rate:** 4°C/min., **Injector Temp.** = 200°C, **Detector Temp.** = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

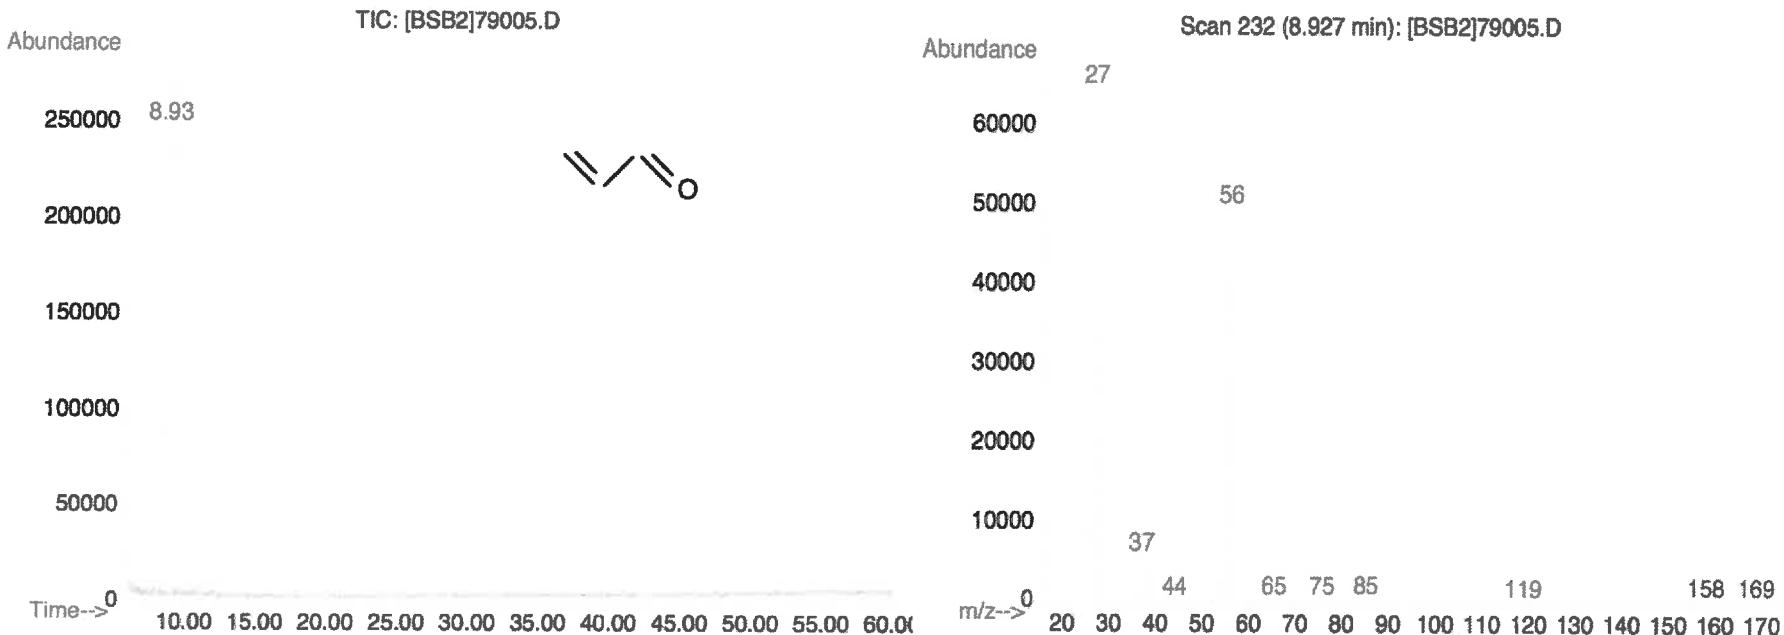

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Vapor Density (AIR = 1)	NA	Evaporation rate (Butyl Acetate = 1)	0°C
Solubility in Water	Completely miscible		NA

Appearance and Odor      CLEAR, COLORLESS LIQUID WITH SLIGHT CHEMICAL ODOR.

#### Section X. STABILITY AND REACTIVITY

Chemical stability      Stable under recommended storage conditions.  
 Possibility of hazardous reactions      NA  
 Conditions to avoid      NA  
 Materials to avoid      NA  
 Hazardous decomposition products - No data available

#### Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat      NA  
 LC50 Inhalation - Rat      NA  
 LD50 Dermal - Guinea pig      NA  
 Causes skin irritation.  
 Eye irritation

#### Section XII. ECOLOGICAL INFORMATION

LC50      NA  
 EC50      NA

#### Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

#### Section XIV. TRANSPORT INFORMATION

DOT (US)  
 Not dangerous goods  
 Proper shipping name: Water      IATA  
 Not dangerous goods  
 Proper shipping name: Water

#### Section XV. REGULATORY INFORMATION

SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

#### Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



## Certified Reference Material CRM

Dec 09/17/24

2 Uvof

ANAB ISO 17034 Accredited  
AR-1539 Certificate Num:  
<https://Absolutestandards.co...>

## CERTIFIED WEIGHT REPORT


Part Number: 91980  
 Lot Number: 091424  
 Description: Acrolein  
 Solvent(s): Water  
 Lot #: 072324Q

Expiration Date: 101424  
 Recommended Storage: Refrigerate (4 °C)  
 Nominal Concentration (µg/mL): 5000  
 NIST Test ID#: 6UTB  
 Weight(s) shown below were combined and diluted to (mL): 10.0      5E-05 Balance Uncertainty  
 0.001 Flask Uncertainty

	091424
Formulated By:	Justin Dippold
	091424
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05175	5008.9	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5µm film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.). **Rate** = 4°C/min., **Injector Temp.** = 200°C, **Detector Temp.** = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

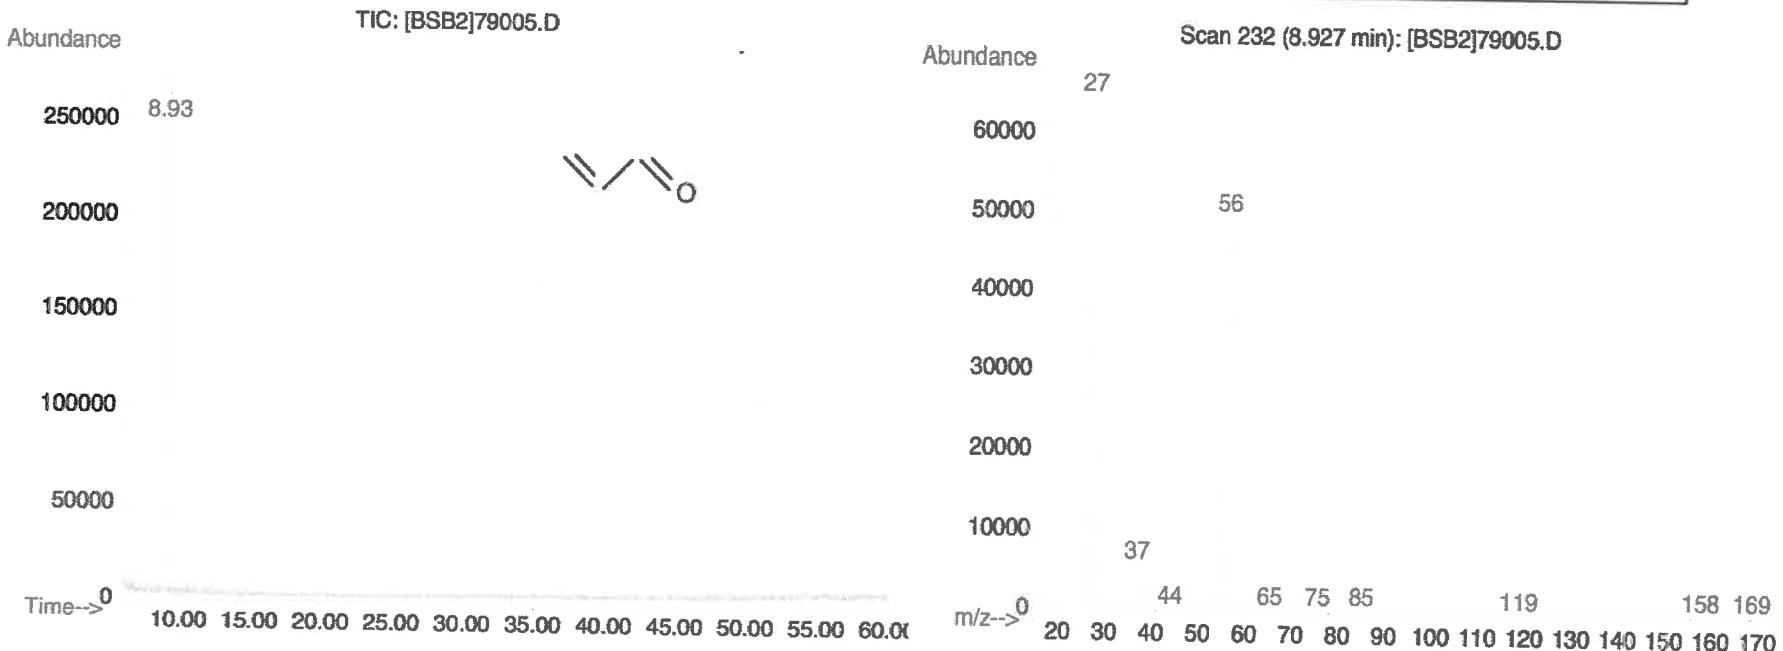

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



## Certified Reference Material CRM

Dec 09/17/24

2 Uvof

ANAB ISO 17034 Accredited  
AR-1539 Certificate Num:  
<https://Absolutestandards.co...>

## CERTIFIED WEIGHT REPORT


Part Number: 91980  
 Lot Number: 091424  
 Description: Acrolein  
 Solvent(s): Water  
 Lot #: 072324Q

Expiration Date: 101424  
 Recommended Storage: Refrigerate (4 °C)  
 Nominal Concentration (µg/mL): 5000  
 NIST Test ID#: 6UTB  
 Weight(s) shown below were combined and diluted to (mL): 10.0      5E-05 Balance Uncertainty  
 0.001 Flask Uncertainty

	091424
Formulated By: Justin Dippold	DATE
	091424
Reviewed By: Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05175	5008.9	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5µm film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.). **Rate** = 4°C/min., **Injector Temp.** = 200°C, **Detector Temp.** = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

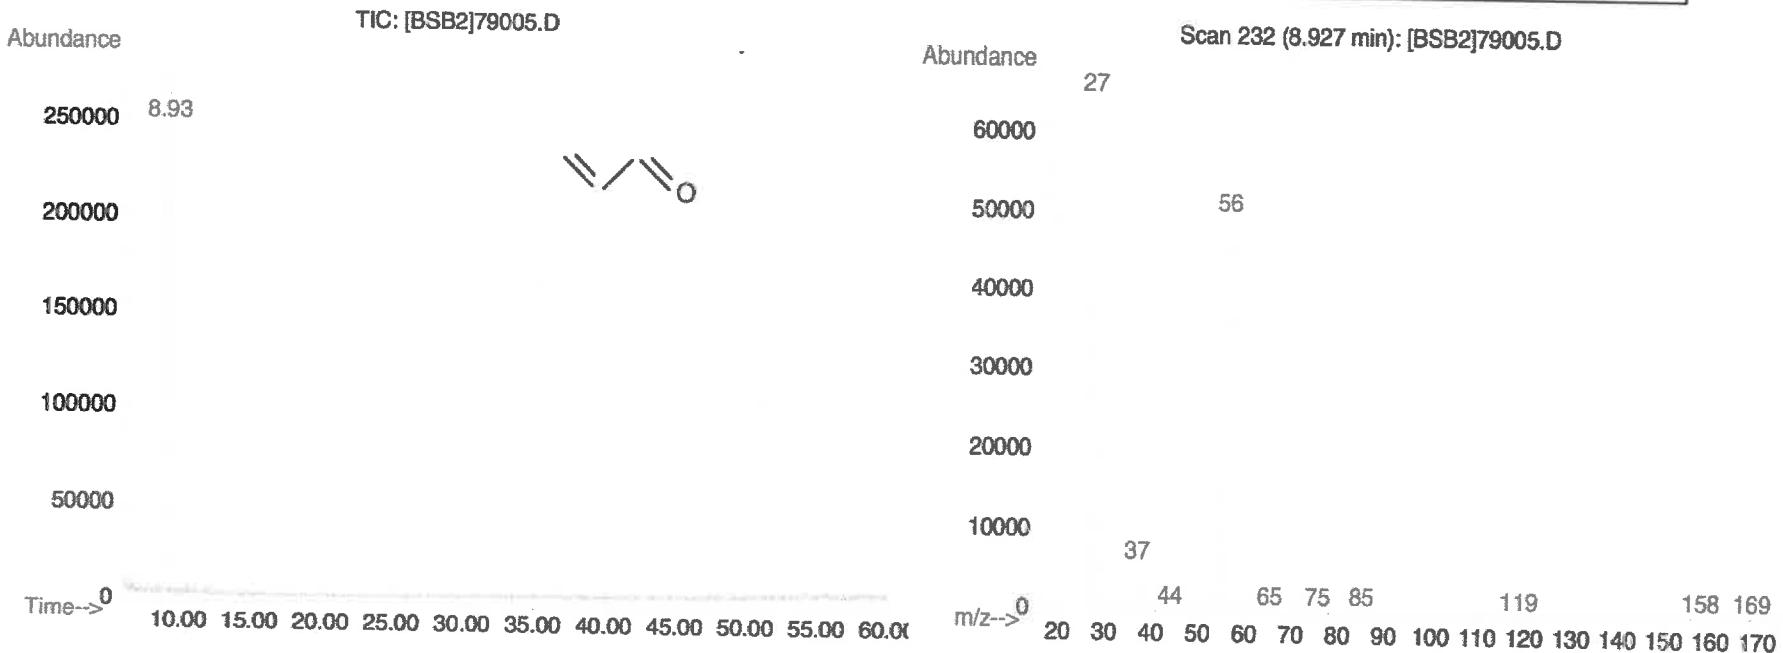

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Rec 12/16/24



CERTIFIED WEIGHT REPORT

Part Number: 95318  
Lot Number: 120524  
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#  
Methanol EJ143-US

Expiration Date: 120527  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test ID#: 6UTB




✓ 14630 to  
✓ 14649

Weight(s) shown below were combined and diluted to (mL): 50.0      5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min.,  
Injector B Temp.= 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

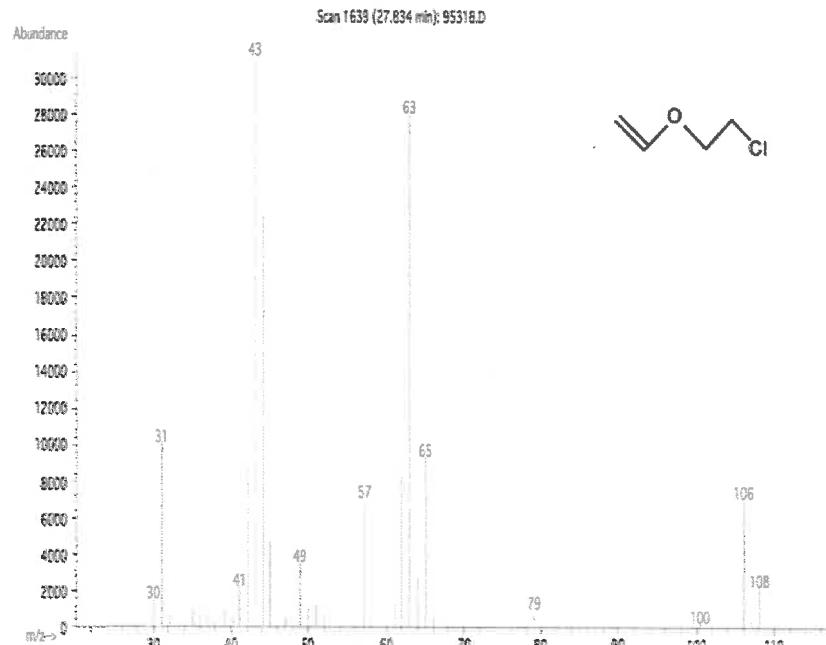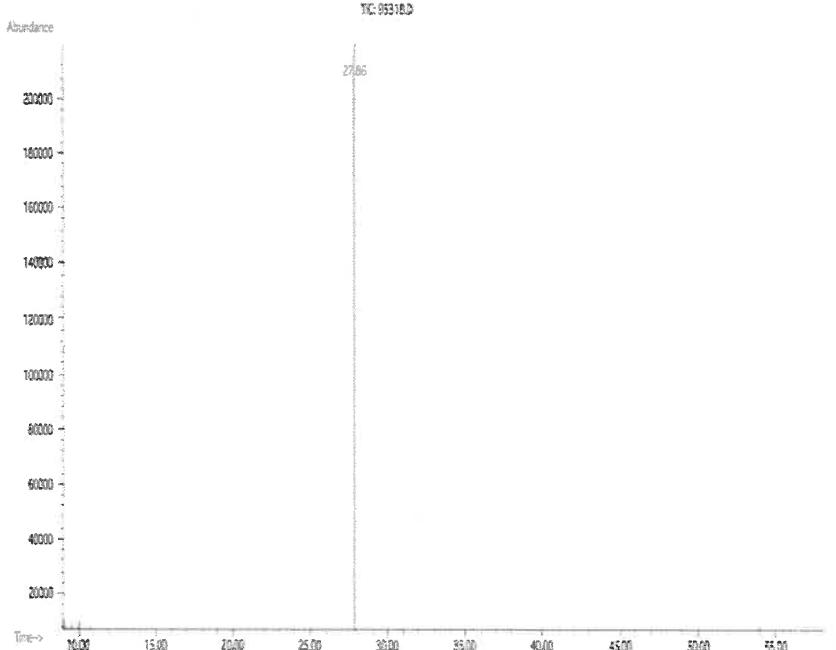

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ( $\pm$ ) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Boiling Point		Specific Gravity (H <sub>2</sub> O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24



CERTIFIED WEIGHT REPORT

Part Number: 95318  
Lot Number: 120524  
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#  
Methanol EJ143-US

Expiration Date: 120527  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test ID#: 6UTB




V14630 to  
V14649

Weight(s) shown below were combined and diluted to (mL): 50.0      5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min.,  
Injector B Temp.= 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

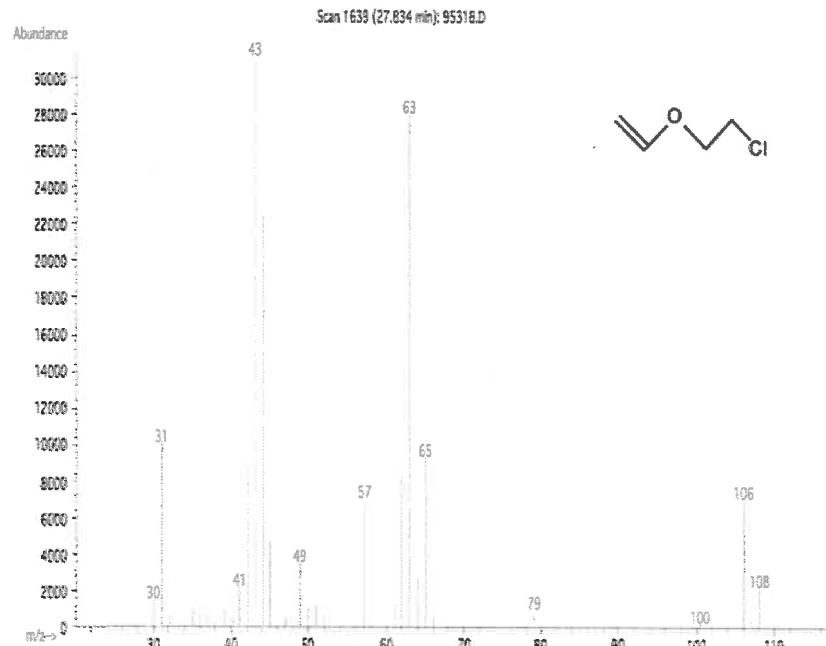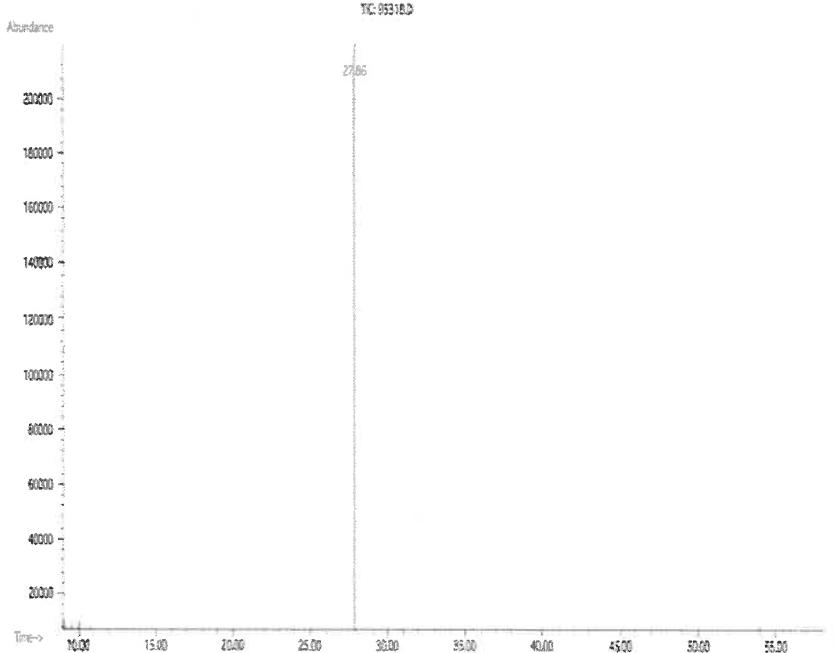

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ( $\pm$ ) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant

## **Section I Product and Company Identification**

**IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL**

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

## **Section II - Hazards Identification**

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



## **Signal Word: DANGER**

### **Section III - Composition**

**See Certified Weight Report For Other Analytes Present At Trace Quantities.**

**INTENDED USE: REFERENCE MATERIAL**

#### **Section IV. FIRST AID MEASURES**

<b>General advice</b>	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
<b>If inhaled</b>	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
<b>In case of skin contact</b>	Wash with soap and water. Consult a physician.
<b>In case of eye contact</b>	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
<b>If swallowed</b>	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

## **Section V. FIREFIGHTING MEASURES**

**Flammability** Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.  
**Suitable extinguishing media** Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.  
**Protective equipment for fire** Wear self contained breathing apparatus for fire fighting if necessary.

## **Section VI. ACCIDENTAL RELEASE MEASURES**

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

## **Section VII. HANDLING AND STORAGE**

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

## **Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION**

**Methanol** 67-56-1 TWA 200 ppm  
**Skin notation** TWA 200 ppm  
Potential for skin absorption, ingestion and inhalation.  
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

#### **Section IX - Physical/Chemical Characteristics**

Boiling Point		Specific Gravity (H <sub>2</sub> O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24



CERTIFIED WEIGHT REPORT

Part Number: 95318  
Lot Number: 120524  
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#  
Methanol EJ143-US

Expiration Date: 120527  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test ID#: 6UTB




✓ 14630 to  
✓ 14649

Weight(s) shown below were combined and diluted to (mL): 50.0      5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min.,  
Injector B Temp.= 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

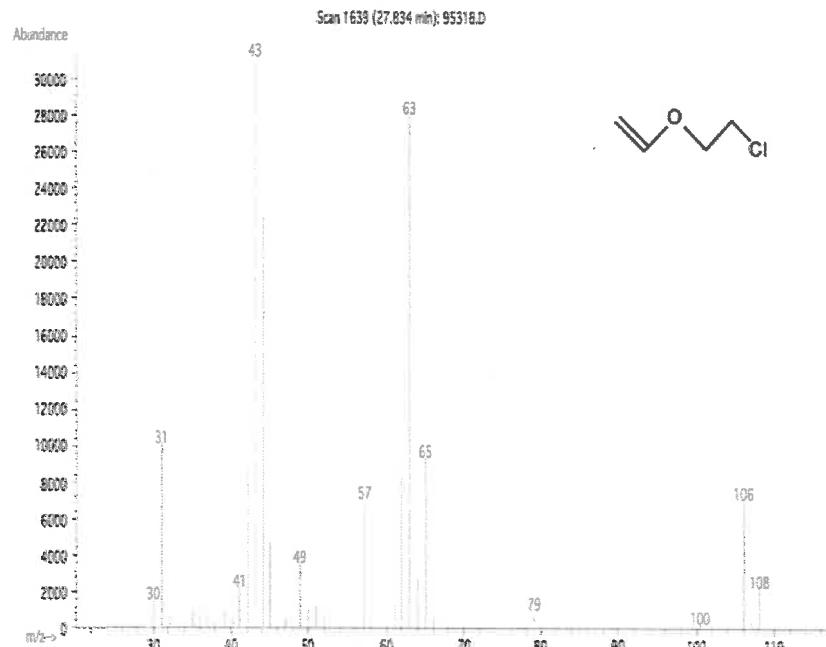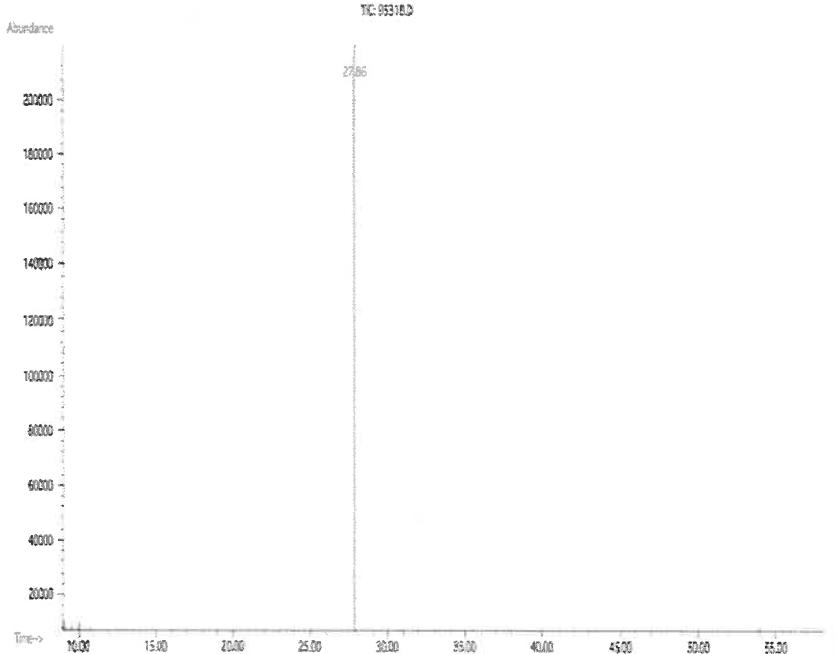

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ( $\pm$ ) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

## Safety Data Sheet (SDS) GHS/OSHA Compliant

**Section I Product and Company Identification****IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL**

Manufacturer's Name      ABSOLUTE STANDARDS INC      Emergency Telephone USA & CANADA      1-800-535-5053  
 Address      44 Rossotto Dr.      Emergency Telephone International      1-352-323-3500  
                  Hamden CT, 06514      Date Prepared/Revised      January 1, 2024

**Section II - Hazards Identification****GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)**

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water

**Signal Word: DANGER****Section III - Composition**

Components (Specific Chemical Identity; Common Name(s))      % (optional)  
 Methanol      METHYL ALCOHOL      > 97

**See Certified Weight Report For Other Analytes Present At Trace Quantities.****INTENDED USE: REFERENCE MATERIAL****Section IV. FIRST AID MEASURES**

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

**Section V. FIREFIGHTING MEASURES**

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.

Protective equipment for fire      Wear self contained breathing apparatus for fire fighting if necessary.

**Section VI. ACCIDENTAL RELEASE MEASURES**

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.

Clean up      Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

**Section VII. HANDLING AND STORAGE**

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

**Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION**

Methanol	67-56-1 TWA 200 ppm
Skin notation	TWA 200 ppm
Potential for skin absorption , ingestion and inhalation.	
Personal protective equipment	Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.	

**Section IX - Physical/Chemical Characteristics**

Boiling Point		Specific Gravity (H <sub>2</sub> O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24



CERTIFIED WEIGHT REPORT

Part Number: 95318  
Lot Number: 120524  
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#  
Methanol EJ143-US

Expiration Date: 120527  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test ID#: 6UTB




✓ 14630 to  
✓ 14649

Weight(s) shown below were combined and diluted to (mL): 50.0      5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min.,  
Injector B Temp.= 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

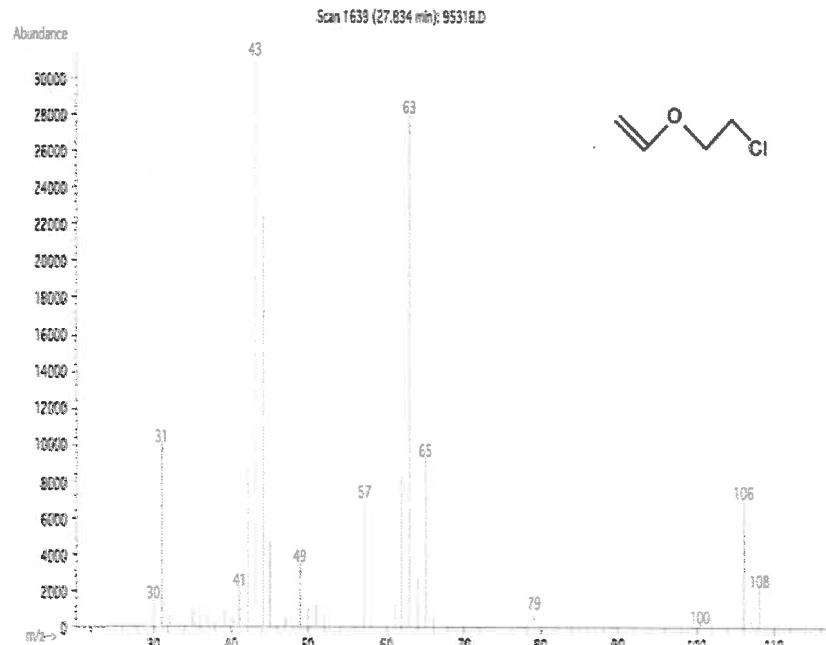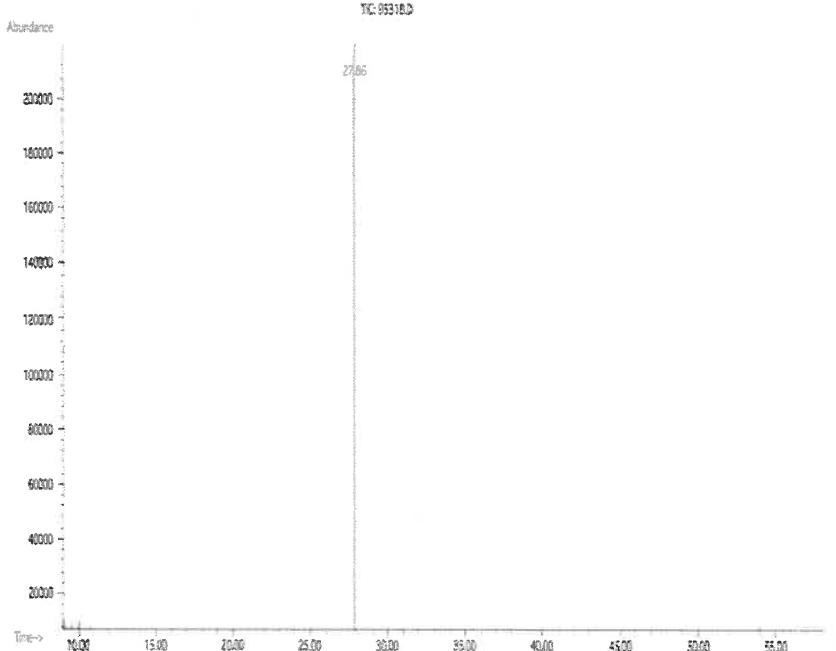

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ( $\pm$ ) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Boiling Point		Specific Gravity (H <sub>2</sub> O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30067

**Lot No.:** A0191805

**Description :** 4-Bromofluorobenzene Standard

4-Bromofluorobenzene Standard 2,500 $\mu$ g/mL, P&T Methanol,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	2,483.9 $\mu$ g/mL	+/- 139.5488

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

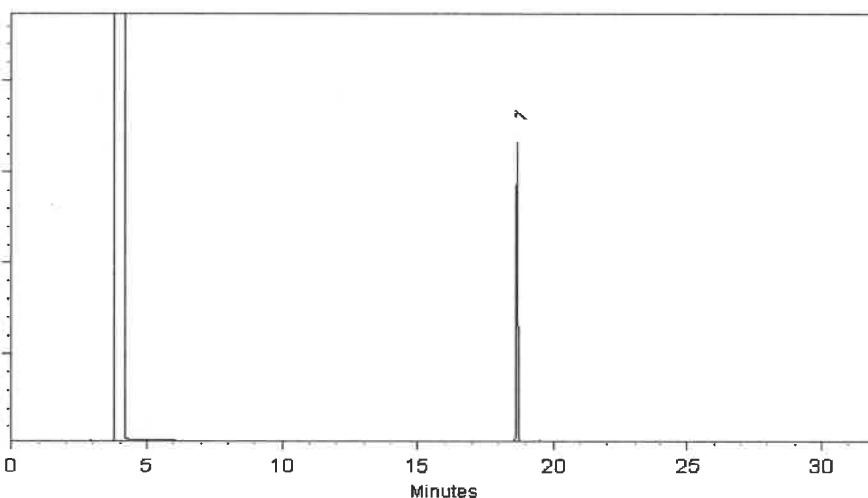

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Alicia Leathers - Operation Technician I

Date Mixed: 17-Nov-2022      Balance Serial #: B251644995

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Nov-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/pECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309  
[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30225

**Lot No.:** A0193071

**Description :** Bromochloromethane Standard

Bromochloromethane 2000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 $\mu$ g/mL	+/- 113.3890

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

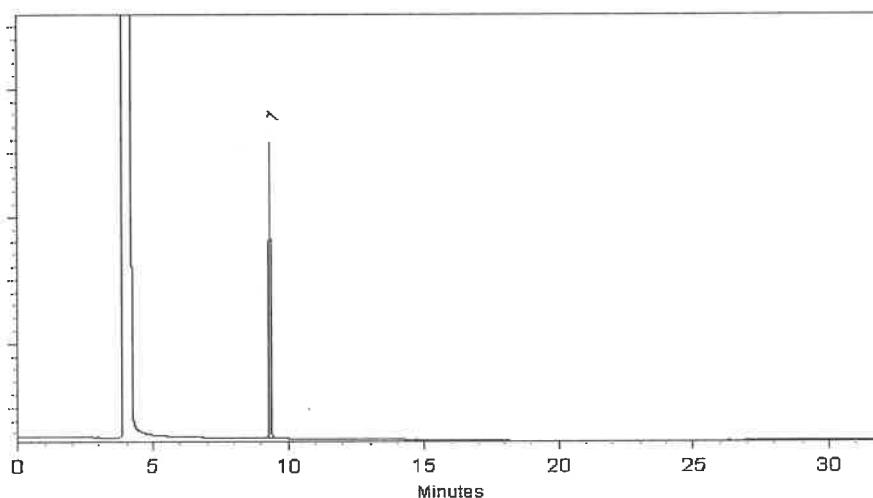

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022      Balance Serial #: B707717271

Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309  
[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30225

**Lot No.:** A0193071

**Description :** Bromochloromethane Standard

Bromochloromethane 2000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 $\mu$ g/mL	+/- 113.3890

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

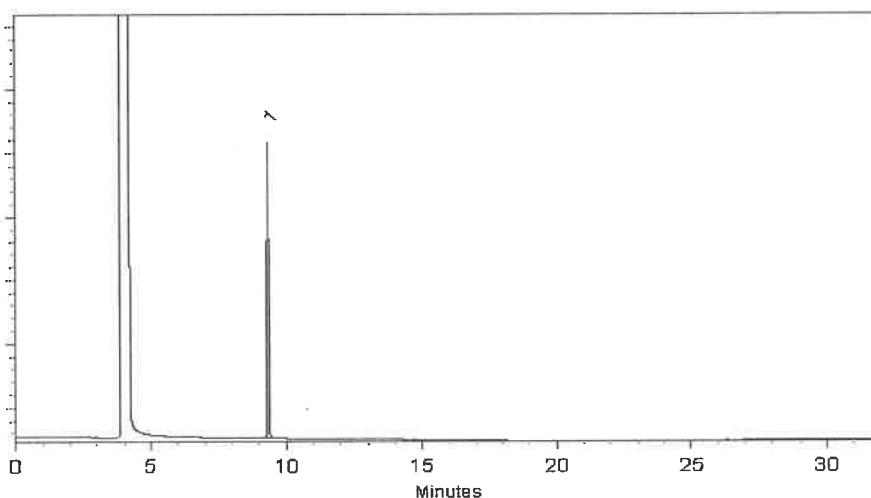

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022      Balance Serial #: B707717271

Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309  
[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30225

**Lot No.:** A0193071

**Description :** Bromochloromethane Standard

Bromochloromethane 2000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 $\mu$ g/mL	+/- 113.3890

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

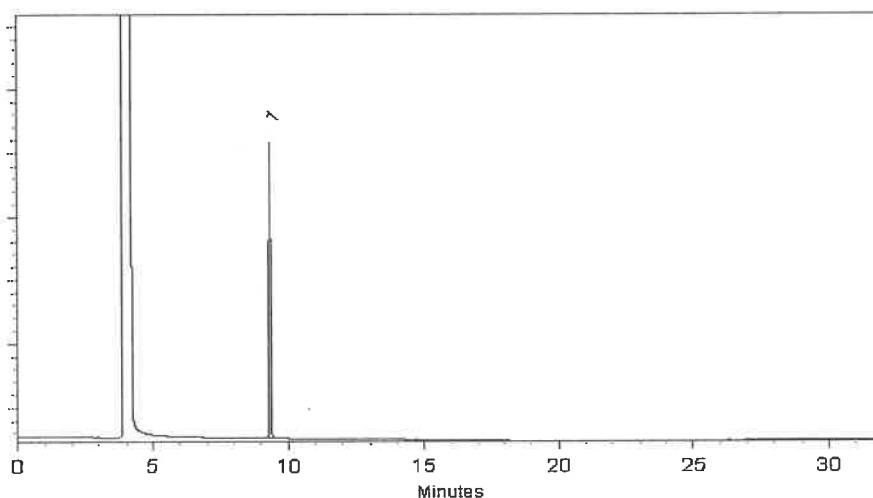

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022      Balance Serial #: B707717271

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309  
[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30225

**Lot No.:** A0193071

**Description :** Bromochloromethane Standard

Bromochloromethane 2000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 $\mu$ g/mL	+/- 113.3890

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

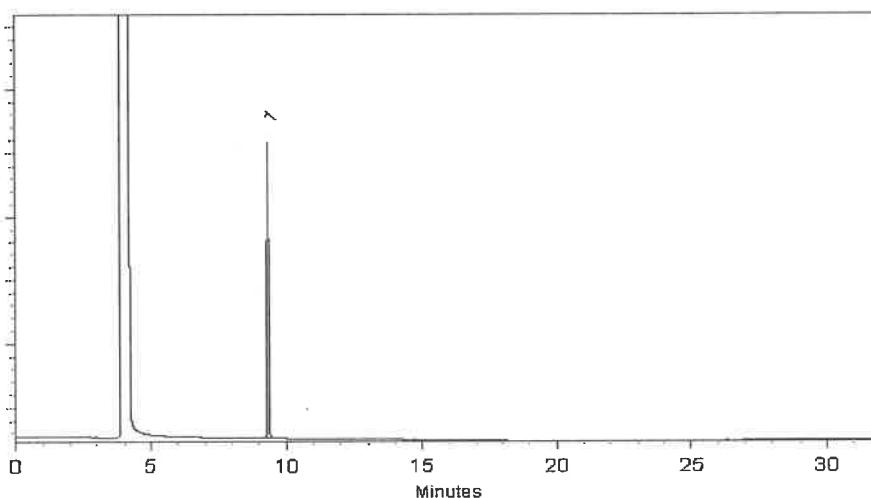

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022      Balance Serial #: B707717271

Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis *gravimetric*



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555582

**Lot No.:** A0196865

**Description :** Custom 8260A/B Surrogate Mix

Custom 8260A/B Surrogate Mix 25,000 $\mu$ g/mL, P&T Methanol,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2026

**Storage:** 10°C or colder

**Ship:** Ambient

#### C E R T I F I E D   V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2-Dichloroethane-d4	17060-07-0	PR-32845	99%	25,036.0 $\mu$ g/mL	+/- 1,417.9179
2	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	25,132.0 $\mu$ g/mL	+/- 1,423.3549
3	Dibromofluoromethane	1868-53-7	022013	99%	25,040.0 $\mu$ g/mL	+/- 1,418.1445
4	Toluene-d8	2037-26-5	PR-33397	99%	25,028.0 $\mu$ g/mL	+/- 1,417.4648

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

Russ Bookhamer - Operations Technician

Date Mixed: 11-Apr-2023 Balance: 1127510105

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



**ILAC**  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



**ILAC**  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30489

**Lot No.:** A0209618

**Description :** 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2025

**Storage:** -20°C or colder

**Handling:** This product is photosensitive.

**Ship:** On Ice

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBP3100	99%	2,019.3 µg/mL	+/- 69.7974
2	Vinyl acetate	108-05-4	RP231030CTH	98%	2,016.8 µg/mL	+/- 69.7112
3	Ethyl acetate	141-78-6	SHBQ9682	99%	2,010.7 µg/mL	+/- 69.4979
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,016.0 µg/mL	+/- 69.6822
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBP6314	99%	2,007.3 µg/mL	+/- 69.3826
7	Amyl acetate	628-63-7	41325/1	97%	2,004.7 µg/mL	+/- 69.2905

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

### Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this

reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

## Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

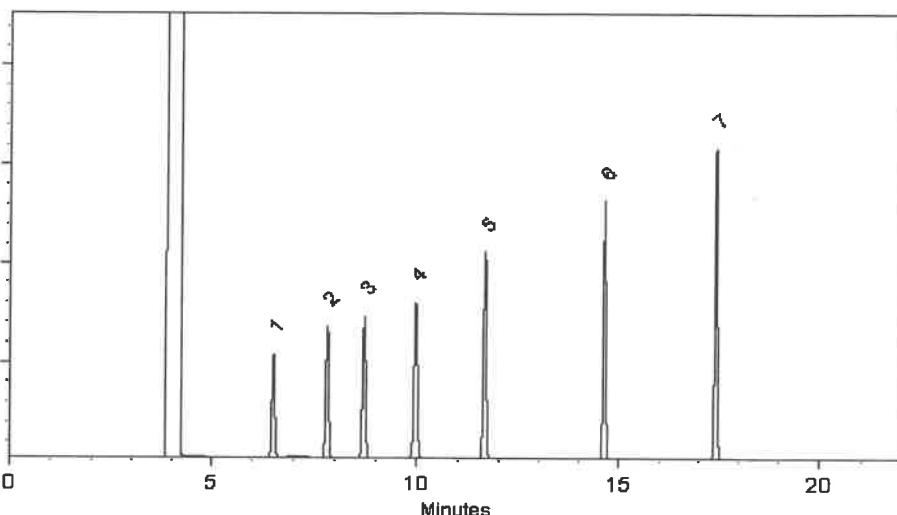

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Samuel Moodier*  
Sam Moodier - Operations Tech I

Date Mixed: 28-Mar-2024 Balance Serial #: B707717271

*Dillan Murphy*  
Dillan Murphy - Operations Technician |

Date Passed: 01-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



**ILAC**  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



**ILAC**  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30489

**Lot No.:** A0209618

**Description :** 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2025

**Storage:** -20°C or colder

**Handling:** This product is photosensitive.

**Ship:** On Ice

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBP3100	99%	2,019.3 µg/mL	+/- 69.7974
2	Vinyl acetate	108-05-4	RP231030CTH	98%	2,016.8 µg/mL	+/- 69.7112
3	Ethyl acetate	141-78-6	SHBQ9682	99%	2,010.7 µg/mL	+/- 69.4979
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,016.0 µg/mL	+/- 69.6822
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBP6314	99%	2,007.3 µg/mL	+/- 69.3826
7	Amyl acetate	628-63-7	41325/1	97%	2,004.7 µg/mL	+/- 69.2905

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

### Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this

reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

## Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

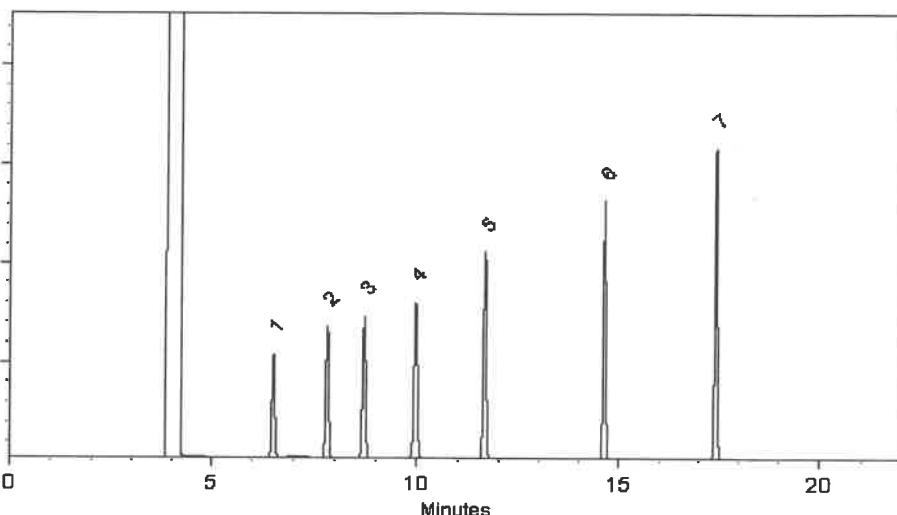

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Samuel Moodier*  
Sam Moodier - Operations Tech I

Date Mixed: 28-Mar-2024 Balance Serial #: B707717271

*Dillan Murphy*  
Dillan Murphy - Operations Technician |

Date Passed: 01-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis *gravimetric*



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 555581

**Lot No.:** A0210184

**Description :** Custom 8260 Internal Standard Mix

Custom 8260 Internal Standard Mix 25,000 $\mu$ g/mL, P&T Methanol,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2027


**Storage:** 10°C or colder

**Ship:** Ambient

#### C E R T I F I E D   V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	25,212.0 $\mu$ g/mL	+/- 1,427.8857
2	1,4-Difluorobenzene	540-36-3	MKCS8657	99%	25,220.0 $\mu$ g/mL	+/- 1,428.3388
3	Chlorobenzene-d5	3114-55-4	PR-31132	99%	25,116.0 $\mu$ g/mL	+/- 1,422.4487
4	Pentafluorobenzene	363-72-4	MKCR9383	99%	25,180.0 $\mu$ g/mL	+/- 1,426.0734

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

  
John Friedline - Operations Technician I

Date Mixed: 11-Apr-2024

Balance: 1127510105

APPROVED  
By Analyst Name: [Redacted] Date: [Redacted]

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

# Certificate of Analysis

*chromatographic plus*

V14697-to-14726



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 30006

**Lot No.:** A0210618

**Description :** VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 $\mu$ g/mL, P&T Methanol/Water(90:10),  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 $\mu$ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 $\mu$ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 $\mu$ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 $\mu$ g/mL	+/- 173.2261

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol/Water (90:10)

**CAS #** 67-56-1/7732-18-5

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**


1 $\mu$ l

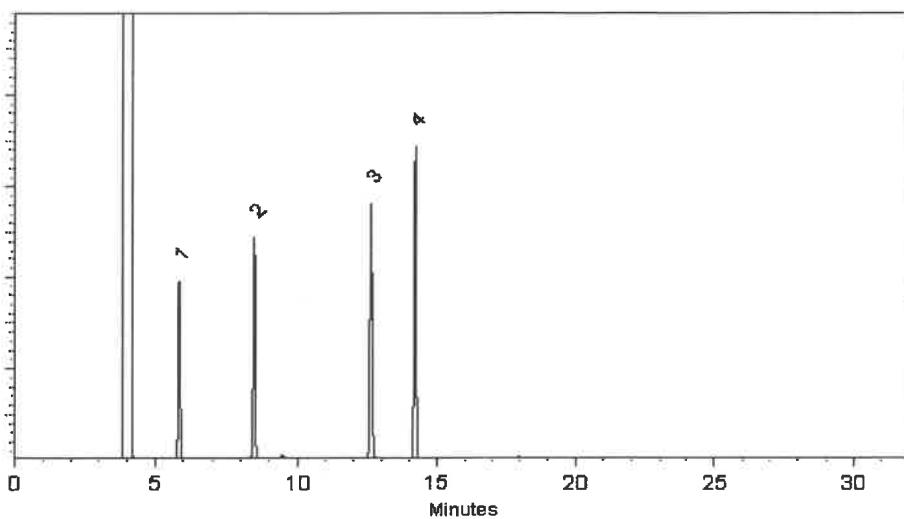

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024      Balance Serial #: B707717271

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

# Certificate of Analysis

*chromatographic plus*

V14697-to-14726



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 30006

**Lot No.:** A0210618

**Description :** VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 $\mu$ g/mL, P&T Methanol/Water(90:10),  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 $\mu$ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 $\mu$ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 $\mu$ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 $\mu$ g/mL	+/- 173.2261

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol/Water (90:10)

**CAS #** 67-56-1/7732-18-5

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**


1 $\mu$ l

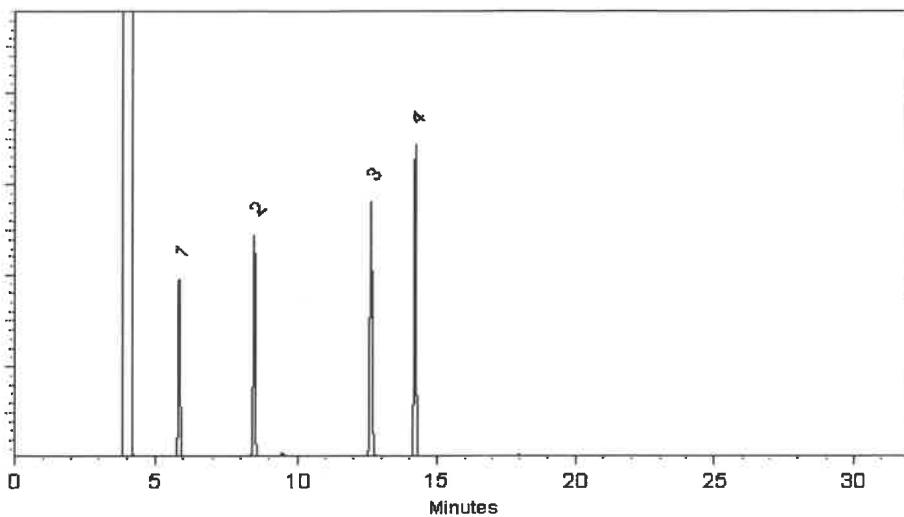

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024      Balance Serial #: B707717271

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

# Certificate of Analysis

*chromatographic plus*

V14697-to-14726



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 30006

**Lot No.:** A0210618

**Description :** VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 $\mu$ g/mL, P&T Methanol/Water(90:10),  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 $\mu$ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 $\mu$ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 $\mu$ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 $\mu$ g/mL	+/- 173.2261

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol/Water (90:10)

**CAS #** 67-56-1/7732-18-5

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**


1 $\mu$ l

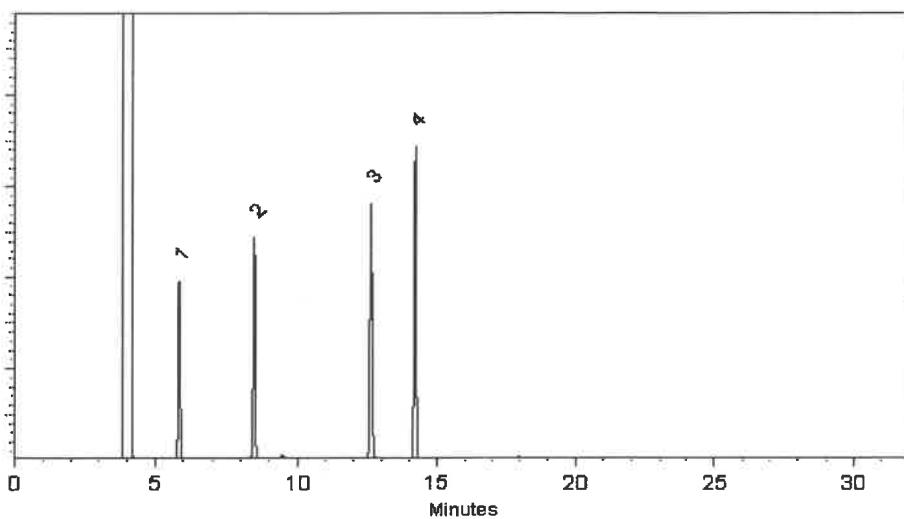

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024      Balance Serial #: B707717271

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

*Rev 12/17/24*  
**CERTIFIED REFERENCE MATERIAL**

*30 mL*



**ILAC**  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222-01



**ILAC**  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222-02

**Certificate of Analysis**  
*chromatographic plus*

*V14727 +  
V14756*

**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30042

**Lot No.:** A0216826

**Description :** 502.2 Calibration Mix #1

502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** May 31, 2031

**Storage:** 0°C or colder

**Ship:** Ambient

**C E R T I F I E D V A L U E S**

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

60m x 0.25mm x 1.4 $\mu$ m  
Rtx-502.2 (cat.#10916)

**Carrier Gas:**

helium-constant flow 2.0 mL/min.

**Temp. Program:**

40°C (hold 6 min.) to 100°C  
@ 6°C/min.

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


MSD

**Split Vent:**

Split ratio 10:1

**Inj. Vol**

1 $\mu$ l

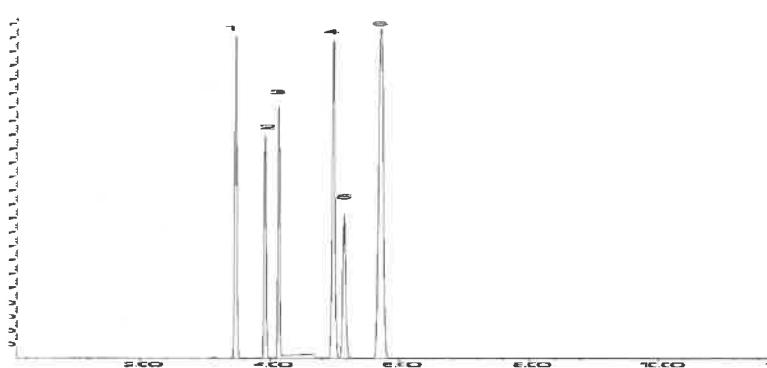

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar Mix Technician

Date Mixed: 23-Sep-2024 Balance Serial #: B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

*Rev 12/17/24*  
**CERTIFIED REFERENCE MATERIAL**

*30 mL*



**ILAC**  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222-01



**ILAC**  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222-02

**Certificate of Analysis**  
*chromatographic plus*

*V14727 +  
V14756*

**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30042

**Lot No.:** A0216826

**Description :** 502.2 Calibration Mix #1

502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** May 31, 2031

**Storage:** 0°C or colder

**Ship:** Ambient

**C E R T I F I E D   V A L U E S**

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

60m x 0.25mm x 1.4 $\mu$ m  
Rtx-502.2 (cat.#10916)

**Carrier Gas:**

helium-constant flow 2.0 mL/min.

**Temp. Program:**

40°C (hold 6 min.) to 100°C  
@ 6°C/min.

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


MSD

**Split Vent:**

Split ratio 10:1

**Inj. Vol**

1 $\mu$ l

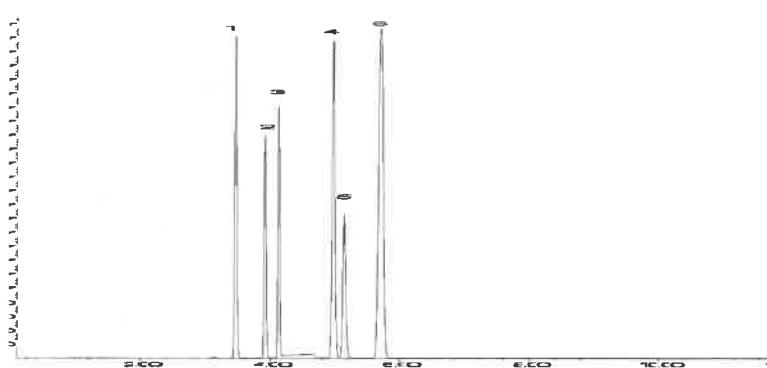

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar Mix Technician

Date Mixed: 23-Sep-2024 Balance Serial #: B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

## Certificate of Analysis

*chromatographic plus*

✓ 14842 to 14846

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 30470

**Lot No.:** A0217535

**Description :** tert-Butanol Standard

tert-Butanol Std 50,000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	tert-Butanol (TBA)	75-65-0	SHBQ8002-1	99%	50,007.5 $\mu$ g/mL	+/- 717.6137

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

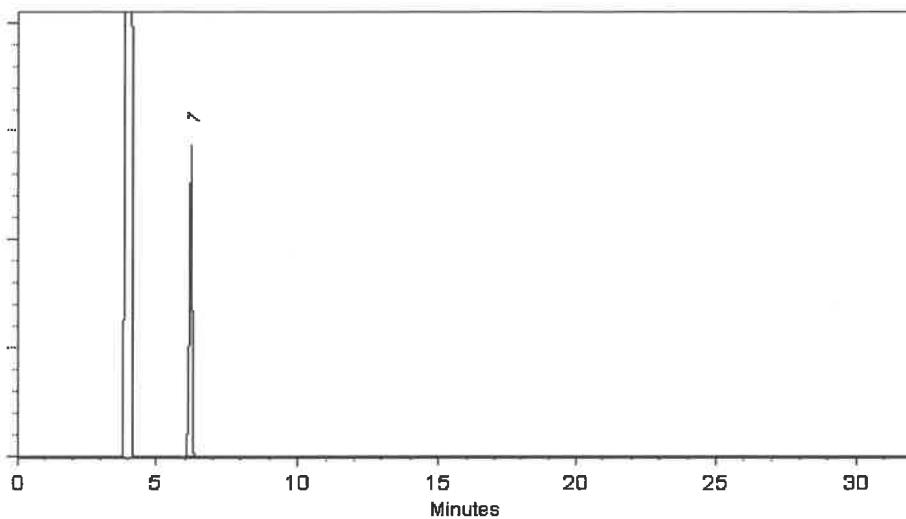

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Aaron Enyart*  
Aaron Enyart - Operations Tech I

Date Mixed: 07-Oct-2024      Balance Serial #: B251644995

*Brittany Federinko*  
Brittany Federinko - Operations Tech I

Date Passed: 09-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

2014 Dec 01 (08/21)



ILAC  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ILAC  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

## Certificate of Analysis chromatographic

J14803 - J14822

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No.:** 555408-SL

**Lot No.:** A0220471

**Description :** Custom Vinyl Acetate Standard

Custom Vinyl Acetate Standard 8,000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** June 30, 2026

**Storage:** -20°C or colder

**Handling:** This product is photosensitive.

**Ship:** On Ice

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 $\mu$ g/mL	+/- 278.7979

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

### Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

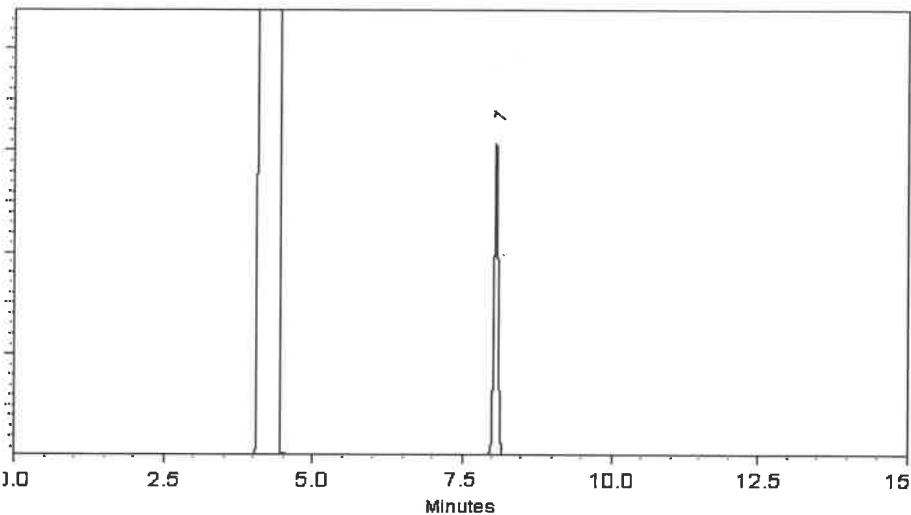

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ethan Winiarski*  
Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024      Balance Serial #: 1127510105

*Dillan Murphy*  
Dillan Murphy - Operations Technician I

Date Passed: 02-Jan-2025

REVIEWED  
By Jennifer Polson at 7:17 am, Jan 05, 2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

2014 Dec 01 (08/21)



ILAC  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ILAC  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

# Certificate of Analysis

chromatographic

J14803 - J14822

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No.:** 555408-SL

**Lot No.:** A0220471

**Description :** Custom Vinyl Acetate Standard

Custom Vinyl Acetate Standard 8,000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** June 30, 2026

**Storage:** -20°C or colder

**Handling:** This product is photosensitive.

**Ship:** On Ice

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 $\mu$ g/mL	+/- 278.7979

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

### Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

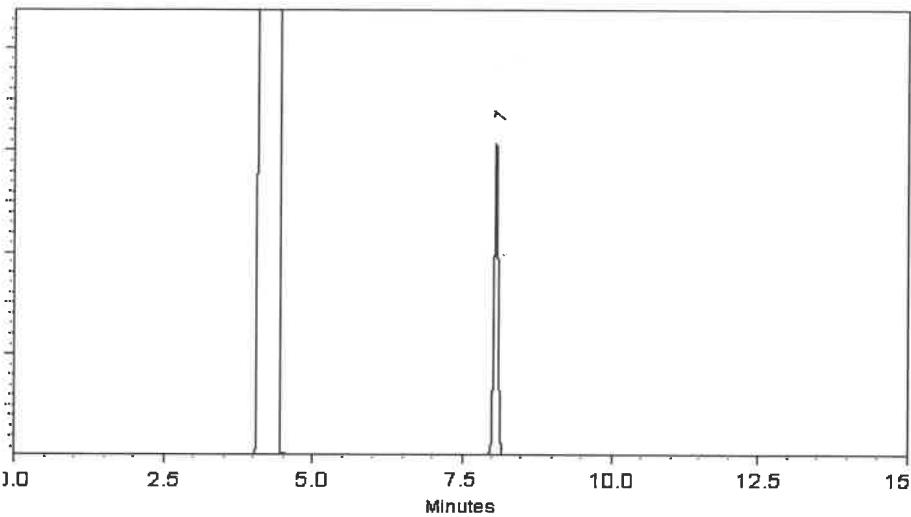

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ethan Winiarski*  
Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024 Balance Serial #: 1127510105

*Dillan Murphy*  
Dillan Murphy - Operations Technician I

Date Passed: 02-Jan-2025

REVIEWED  
By Jennifer Polson at 7:17 am, Jan 05, 2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis



Material No.: 9077-02  
Batch No.: 22L0562016  
Manufactured Date: 2022-10-26  
Expiration Date: 2025-10-25  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ( $\text{CH}_3\text{OH}$ ) (by GC, corrected for water)	$\geq 99.9 \%$	100.0 %
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.2 ppm
Titrable Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	0.2
Titrable Base ( $\mu\text{eq/g}$ )	$\leq 0.10$	0.03
Water (by KF, coulometric)	$\leq 0.08 \%$	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier  
Vice President Global Quality

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis



V14883  
V14884


Material No.: 9077-02  
Batch No.: 22L0562016  
Manufactured Date: 2022-10-26  
Expiration Date: 2025-10-25  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

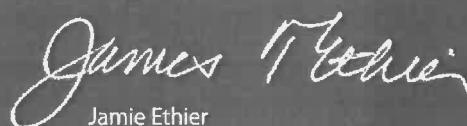  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1



# SHIPPING DOCUMENTS

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

## CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: Jacobs

ADDRESS: 412 Mt Kisco Ave Suite #100

CITY: Morristown STATE: NJ ZIP: 07960

ATTENTION: John Yufant *John.Yufant@Jacobs.com*

PHONE: FAX:

## CLIENT PROJECT INFORMATION

PROJECT NAME: STC PTC

PROJECT NO.: D3868221 LOCATION: Princeton Junction

PROJECT MANAGER: Mary Murphy

e-mail: ~~CRPT~~ Mary.Murphy@Jacobs.com

PHONE: FAX:

## CLIENT BILLING INFORMATION

BILL TO: Mary Murphy

PO#:

ADDRESS:

CITY: STATE: ZIP:

ATTENTION: PHONE:

## ANALYSIS

## DATA TURNAROUND INFORMATION

FAX (RUSH) Rush TAT (2 day) DAYS\*

HARD COPY (DATA PACKAGE): DAYS\*

EDD: DAYS\*

\*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

## DATA DELIVERABLE INFORMATION

- Level 1 (Results Only)  Level 4 (QC + Full Raw Data)  
 Level 2 (Results + QC)  NJ Reduced  US EPA CLP  
 Level 3 (Results + QC)  NYS ASP A  NYS ASP B  
+ Raw Data)  Other \_\_\_\_\_  
 EDD FORMAT

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS	
			COMP	GRAB	DATE	TIME		A/E	E	B/E	E	E	E	A/E				
								1	2	3	4	5	6	7	8	9		
1.	MW-18B-56-040225	GW	✓		4/2/25	1235	2	✓	✓	✓	✓	✓	✓	✓	✓	✓	MS/MSD !! (27 bottles)	
2.	MW-17B-55-040225	GW	✓		4/2/25	1535	0910	✓	✓	✓	✓	✓	✓	✓	✓	✓	9 bottles	
3.	MW-18B-56-040225-SIM	GW	✓		4/2/25	1235	2											
4.	MW-17B-56-040225-SIM	GW	✓		4/2/25	1535	2											
5.																		
6.																		
7.																		
8.																		
9.																		
10.																		

## SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER:

DATE/TIME: 4-2-25 1650

RECEIVED BY:

1. *D* 4-2-25

RELINQUISHED BY SAMPLER:

DATE/TIME:

RECEIVED BY:

2.

RELINQUISHED BY SAMPLER:

DATE/TIME: 4-2-25 1825

RECEIVED BY:

3.

Conditions of bottles or coolers at receipt:  COMPLIANT  NON COMPLIANT  COOLER TEMP

3.0°C

Comments: See work order for list of site specific VOCs

PRESERVE DISSOLVE IRON SAMPLES UPON ARRIVAL TO THE LAB

PO# 148064311

Temp 3.0°C (Adjusted Factor +1) IR Gun #1

Page 1 of 2 CLIENT:  Hand Delivered  Other

Shipment Complete

 YES  NO



**From:** Ynfante, John <John.Ynfante@jacobs.com>  
**Sent:** Friday, April 04, 2025 12:54 PM  
**To:** Yazmeen Gomez; Mohammad Ahmed  
**Subject:** RE: Princeton SIM/no-SIM

EXTERNAL EMAIL - This email was sent by a person from outside your organization. Exercise caution when clicking links, opening attachments or taking further action, before validating its authenticity.

Secured by Check Point

Thanks Yazmeen, but like I mentioned yesterday if you aren't able to analyze any of those 3 normal samples by SIM then I have no need for the EB to be analyzed by SIM either so please just cancel that SIM EB. I will already have EB data for VOCs from the EB you ran (or are running) by your routine low 8260D.

---

**From:** Yazmeen Gomez <Yazmeen.Gomez@alliancetg.com>  
**Sent:** Friday, April 4, 2025 11:51 AM  
**To:** Ynfante, John <John.Ynfante@jacobs.com>; Mohammad Ahmed <mohammad.ahmed@alliancetg.com>  
**Subject:** [EXTERNAL] RE: Princeton SIM/no-SIM

John,

Please see attached. SIM analysis is also not possible for MW-18B and MW-17B.

However, "EB01-040225-SIM" will be analyzed with SIM.

Best Regards,



**Yazmeen Gomez**  
**Sr. Project Manager**  
**An Alliance Technical Group Company**  
**Main:** 908-789-8900  
**Direct:** 908-728-3147  
**Address:** 284 Sheffield St, Ste 1, Mountainside, NJ 07092  
[www.alliancetg.com](http://www.alliancetg.com)

---

**From:** Ynfante, John <John.Ynfante@jacobs.com>  
**Sent:** Thursday, April 3, 2025 6:27 PM  
**To:** Mohammad Ahmed <mohammad.ahmed@alliancetg.com>; Yazmeen Gomez <Yazmeen.Gomez@alliancetg.com>  
**Subject:** RE: Princeton SIM/no-SIM

EXTERNAL EMAIL - This email was sent by a person from outside your organization. Exercise caution when clicking links, opening attachments or taking further action, before validating its authenticity.

Ok thanks for the confirmation Mohammad

---

**From:** Mohammad Ahmed <[mohammad.ahmed@alliancetg.com](mailto:mohammad.ahmed@alliancetg.com)>  
**Sent:** Thursday, April 3, 2025 5:22 PM  
**To:** Ynfante, John <[John.Ynfante@jacobs.com](mailto:John.Ynfante@jacobs.com)>; Yazmeen Gomez <[Yazmeen.Gomez@alliancetg.com](mailto:Yazmeen.Gomez@alliancetg.com)>  
**Subject:** [EXTERNAL] Re: Princeton SIM/no-SIM

Hi John ,  
I will let you know about other 2 samples regarding SIM .  
1 8oz jar is enough to run Total metals and SPLP

Get [Outlook for iOS](#)

---

**From:** Ynfante, John <[John.Ynfante@jacobs.com](mailto:John.Ynfante@jacobs.com)>  
**Sent:** Thursday, April 3, 2025 5:55:35 PM  
**To:** Yazmeen Gomez <[Yazmeen.Gomez@alliancetg.com](mailto:Yazmeen.Gomez@alliancetg.com)>; Mohammad Ahmed <[mohammad.ahmed@alliancetg.com](mailto:mohammad.ahmed@alliancetg.com)>  
**Subject:** Princeton SIM/no-SIM

EXTERNAL EMAIL - This email was sent by a person from outside your organization. Exercise caution when clicking links, opening attachments or taking further action, before validating its authenticity.

Hi Yazmeen and Mohammad, a few things:

After speaking with Mohammad I understand that the full scan 8260D run for the MW-17B sample had ~11ppm of TCE and high concs of other VOCs as well so you won't be able to run SIM on it – I understand the limitations and have passed that update on to the team so that is fine. There should also be SIM samples collected for 2 more samples - MW-18B and MW-19B so please let me know if your standard 8260 run shows similar concentrations on those as well. Note that these 3 samples are in a completely different location from the rest of the samples and their concentrations shouldn't necessarily represent the levels we will see for other samples – I understand if you have to dilute these high-conc samples I just don't want to over-dilute other samples unnecessarily.

Also, if you don't end up running any of the 3 SFAM-SIM samples then we have no need for that SIM equipment blank to be analyzed either so you can cancel that unless MW-18B or MW-19B turn out to be low enough to be run by SIM in which case I would want the SIM EB.

Finally, for the soil samples we are collecting next week the client decided today that we should also collect for SPLP silver and place it on hold pending the total silver results – I believe you sent 8oz jars for the total silver so that should be plenty to cover the initial silver analysis and then still have enough for SPLP Silver if we need to run it right? Or do you prefer a completely separate jar for the SPLP Ag?

John Ynfante  
Jacobs  
Chemist  
281-414-1719 mobile  
[John.Ynfante@jacobs.com](mailto:John.Ynfante@jacobs.com)  
[www.jacobs.com](http://www.jacobs.com)

---

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

NOTICE - This communication may contain confidential and privileged information that is for the sole use of the intended recipient. Any viewing, copying or distribution of, or reliance on this message by unintended recipients is strictly prohibited. If you have received this message in error, please notify us immediately by replying to the message and deleting it from your computer.

---

NOTICE - This communication may contain confidential and privileged information that is for the sole use of the intended recipient. Any viewing, copying or distribution of, or reliance on this message by unintended recipients is strictly prohibited. If you have received this message in error, please notify us immediately by replying to the message and deleting it from your computer.

---

NOTICE - This communication may contain confidential and privileged information that is for the sole use of the intended recipient. Any viewing, copying or distribution of, or reliance on this message by unintended recipients is strictly prohibited. If you have received this message in error, please notify us immediately by replying to the message and deleting it from your computer.

**Laboratory Certification**

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

## LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q1711 JACO05	Order Date : 4/3/2025 10:00:00 AM	Project Mgr :
Client Name : JACOBS Engineering Grou	Project Name : Former Schlumberger STC	Report Type : Level 4
Client Contact : John Ynfante	Receive DateTime : 4/2/2025 6:25:00 PM	EDD Type : CH2MHILL
Invoice Name : JACOBS Engineering Grou	Purchase Order :	Hard Copy Date :
Invoice Contact : John Ynfante		Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q1711-01	MW-18B-56-040225	Water	04/02/2025	12:35	VOCMS Group3		8260-Low	2 Bus. Days	
Q1711-02	Q1711-01MS	Water	04/02/2025	12:35	VOCMS Group3		8260-Low	2 Bus. Days	
Q1711-03	Q1711-01MSD	Water	04/02/2025	12:35	VOCMS Group3		8260-Low	2 Bus. Days	
Q1711-04	MW-17B-55-040225	Water	04/02/2025	15:35	VOCMS Group3		8260-Low	2 Bus. Days	
Q1711-05	MW-18B-56-040225-SIM	Water	04/02/2025	12:35	VOC TRACE SFAM		SFAM_Trace	2 Bus. Days	
Q1711-06	MW-17B-56-040225-SIM	Water	04/02/2025	15:35	VOC-TRACE-SFAM		SFAM_Trace	2 Bus. Days	YG 04/04/2025
Q1711-07	RMW-05B-89-040225	Water	04/02/2025	16:05	VOCMS Group3		8260-Low	2 Bus. Days	
Q1711-08	EB01-040225	Water	04/02/2025	15:50					

## LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q1711	JACO05	Order Date : 4/3/2025 10:00:00 AM	Project Mgr :
Client Name : JACOBS Engineering Grou		Project Name : Former Schlumberger STC	Report Type : Level 4
Client Contact : John Ynfante		Receive Date/Time : 4/2/2025 6:25:00 PM	EDD Type : CH2MHILL
Invoice Name : JACOBS Engineering Grou		Purchase Order :	Hard Copy Date :
Invoice Contact : John Ynfante			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q1711-09	EB01-040225-SIM	Water	04/02/2025	15:50	VOCMS Group3		8260-Low	2 Bus. Days	
Q1711-10	TB01-040225	Water	04/02/2025	16:00	VOC TRACE SFAM	SFAM_Trace	2 Bus. Days	YG	04/04/2025

Relinquished By :

CH  
Date / Time : 4-3-25 12:25

Received By :

CH  
Date / Time : 4-3-25 12:25

Storage Area : VOA Refrigerator Room