
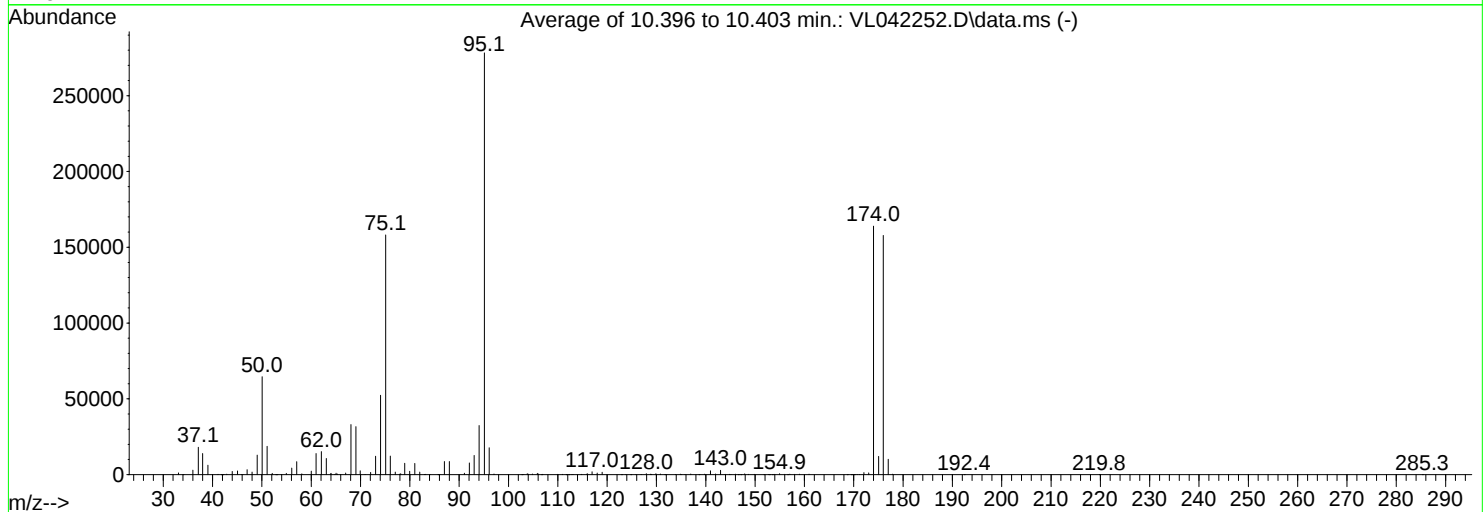


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040825\
Data File : VL042252.D
Acq On : 08 Apr 2025 07:57
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

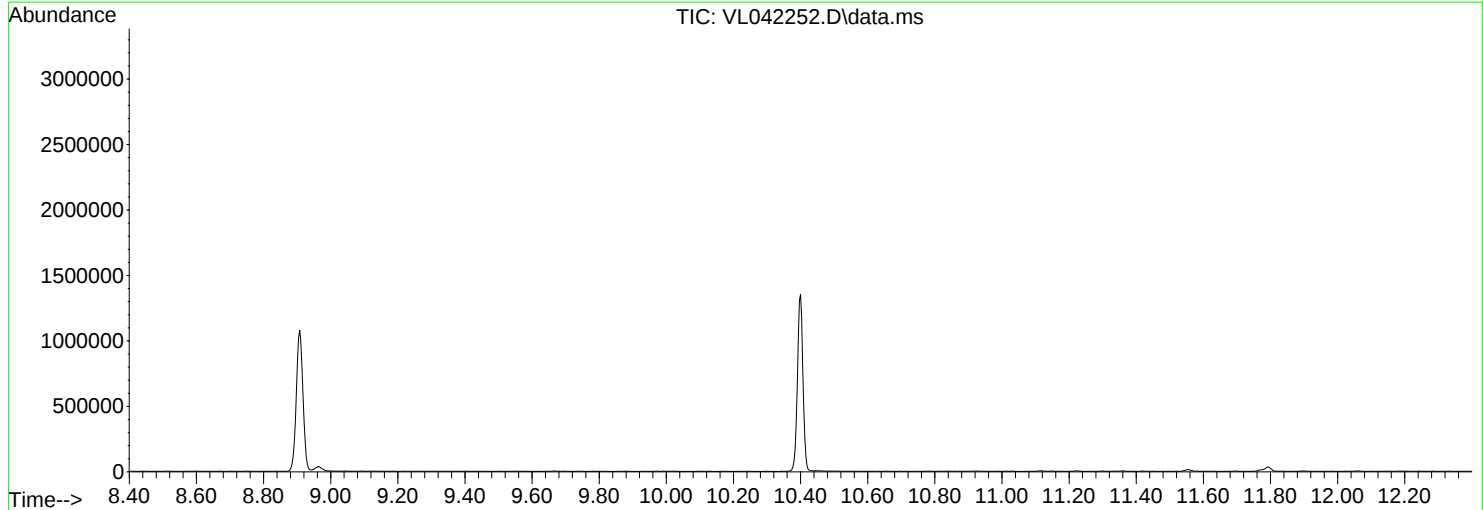

AutoFind: Scans 3185, 3186, 3187; Background Corrected with Scan 3171

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.2	64653	PASS
75	95	30	66	56.8	158080	PASS
95	95	100	100	100.0	278272	PASS
96	95	5	9	6.4	17742	PASS
173	174	0.00	2	0.7	1215	PASS
174	95	50	120	58.9	163968	PASS
175	174	4	9	7.4	12075	PASS
176	174	93	101	96.2	157760	PASS
177	176	5	9	6.5	10188	PASS

Average of 10.396 to 10.403 min.: VL042252.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1173	45.05	2396	53.95	75	64.80	20
34.00	24	45.90	94	54.95	823	65.05	96
36.00	2935	46.15	122	56.05	4327	65.30	38
37.10	18091	47.00	3288	57.05	8586	65.95	11
38.00	13985	48.00	1743	58.10	481	67.00	1033
39.05	6269	49.05	12912	60.00	2314	68.05	33005
41.10	186	50.05	64653	61.00	13978	69.05	31645
41.80	46	51.05	18675	62.05	15253	69.95	2571
42.10	53	52.10	879	63.05	10648	70.90	102
42.90	316	52.80	36	63.90	490	72.05	1487
44.00	2123	53.05	63	64.05	900	73.05	12139

Average of 10.396 to 10.403 min.: VL042252.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.05	52327	83.20	208	96.10	17742	110.00	246
75.10	158080	84.10	65	97.05	449	110.95	263
76.05	12287	85.70	23	102.70	63	111.70	44
77.05	1759	86.05	104	103.10	118	111.95	126
77.90	379	87.00	8661	103.80	694	112.20	47
78.15	661	88.00	8614	104.00	377	112.85	161
78.95	7464	91.05	1004	104.85	431	113.10	151
79.95	2195	92.05	7755	105.85	896	114.85	262
81.00	7405	93.05	12653	106.10	407	115.90	431
82.00	1757	94.05	32440	106.70	34	116.05	484
82.95	159	95.10	278272	106.95	186	116.95	1878

Average of 10.396 to 10.403 min.: VL042252.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.00	1020	130.80	423	142.00	414	151.80	26
119.00	1551	131.70	56	143.00	2904	152.70	122
122.90	25	132.10	71	143.95	209	152.90	55
123.80	172	133.85	67	144.80	270	153.50	30
124.80	33	134.85	336	145.10	108	154.00	198
125.85	168	135.10	127	146.00	338	154.95	621
126.90	65	135.80	108	146.60	18	156.00	242
127.95	700	136.95	468	147.10	28	156.60	59
128.80	316	138.60	62	147.90	513	157.05	369
129.00	248	139.80	366	148.65	229	158.00	241
129.90	615	140.95	2513	149.85	211	159.00	309

Average of 10.396 to 10.403 min.: VL042252.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.95	339	176.00	157760				
168.70	37	177.00	10188				
169.50	38	177.90	281				
169.80	43	192.40	19				
170.10	32	219.80	20				
170.70	147	285.30	19				
171.15	161						
172.05	1377						
173.05	1215						
174.00	163968						
175.05	12075						