
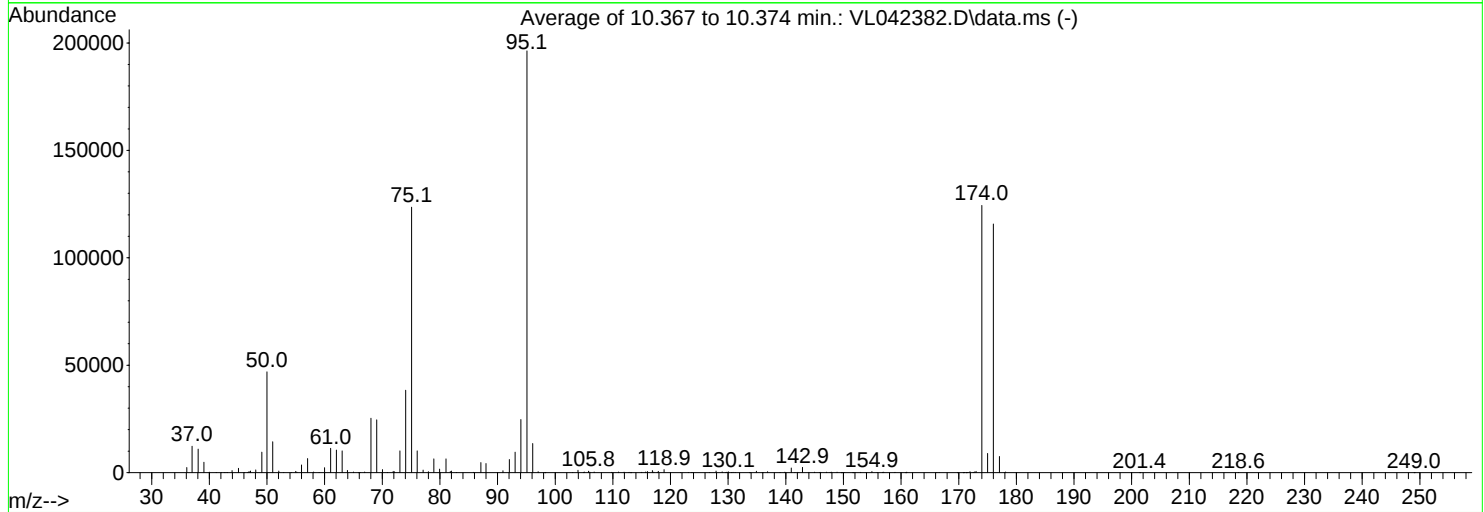


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041825\
Data File : VL042382.D
Acq On : 18 Apr 2025 07:51
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Apr 18 02:14:00 2025

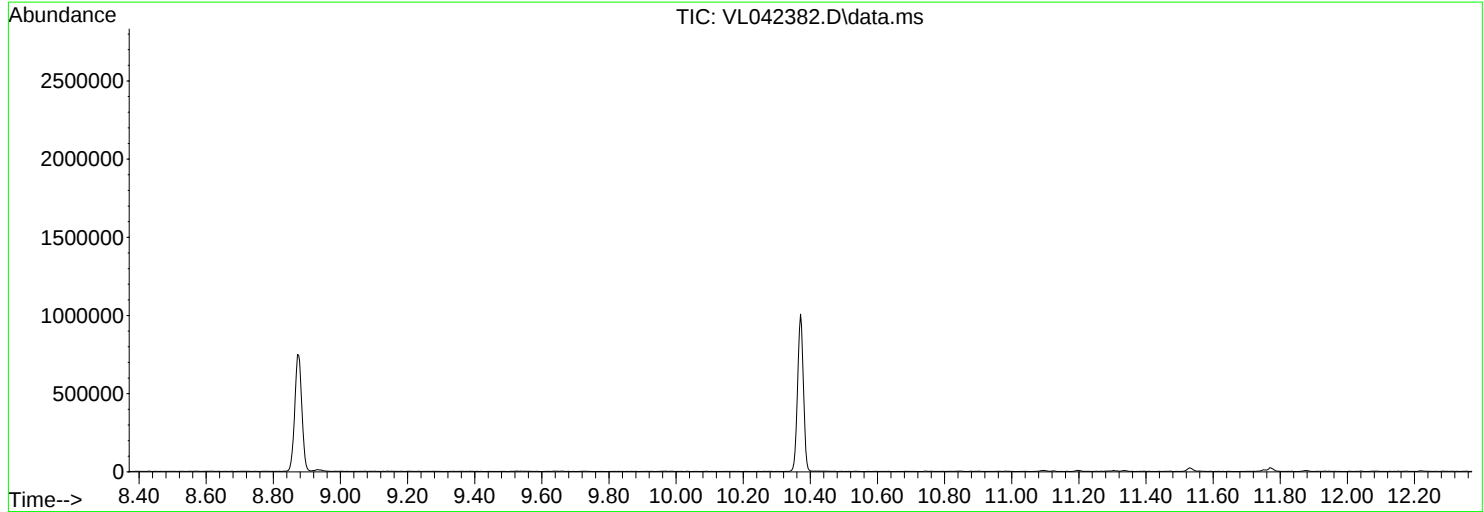

AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3162

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.9	46915	PASS
75	95	30	66	62.9	123587	PASS
95	95	100	100	100.0	196331	PASS
96	95	5	9	6.9	13533	PASS
173	174	0.00	2	0.5	606	PASS
174	95	50	120	63.4	124411	PASS
175	174	4	9	7.2	8959	PASS
176	174	93	101	93.0	115728	PASS
177	176	5	9	6.5	7500	PASS

Average of 10.367 to 10.374 min.: VL042382.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	2355	45.05	2019	54.25	90	63.95	1054
37.00	12307	46.05	107	55.00	589	65.00	271
38.05	10978	46.70	173	55.20	230	65.90	21
39.05	4844	46.90	506	56.00	3553	66.15	7
40.00	261	47.15	771	57.05	6587	66.95	333
41.20	49	48.05	1299	58.10	295	68.05	25299
42.10	50	49.10	9510	59.05	92	69.05	24557
42.60	94	50.00	46915	60.00	2328	70.05	1436
42.90	101	51.00	14396	61.05	11301	70.90	47
43.15	65	52.05	731	62.05	10485	71.90	575
43.95	949	52.90	81	63.05	10158	72.10	474

Average of 10.367 to 10.374 min.: VL042382.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	10117	82.90	116	98.20	38	112.80	160
74.05	38381	85.85	183	103.05	61	113.10	24
75.10	123587	87.10	4682	103.95	1126	115.00	168
76.05	10164	88.00	4242	104.90	76	115.70	339
77.10	1198	90.95	883	105.05	266	116.00	527
78.00	474	92.05	6079	105.80	663	116.85	942
78.95	6382	93.05	9542	106.00	214	117.10	203
79.95	1673	94.05	24704	106.75	307	117.70	167
81.05	6395	95.10	196331	109.75	167	117.90	574
81.80	488	96.10	13533	111.00	306	118.90	1428
82.00	782	97.05	482	111.95	206	121.75	40

Average of 10.367 to 10.374 min.: VL042382.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.10	44	131.20	45	144.00	139	151.60	39
123.70	84	133.70	21	145.00	253	152.00	110
123.90	45	134.90	649	145.90	116	153.00	137
126.80	62	135.90	20	146.05	165	153.95	90
127.90	722	136.85	432	147.10	201	154.95	495
128.95	344	139.00	99	147.70	124	155.85	99
129.60	95	139.85	238	147.95	236	156.80	131
129.80	216	140.95	2142	148.90	197	157.00	260
130.05	365	141.60	44	149.60	19	158.95	189
130.60	101	142.10	181	149.90	63	160.80	17
130.85	170	142.90	2426	150.10	94	161.00	227

Average of 10.367 to 10.374 min.: VL042382.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
166.20	42	174.00	124411				
166.60	84	175.00	8959				
169.80	19	176.00	115728				
170.80	24	177.05	7500				
171.00	53	177.90	86				
171.30	25	178.15	284				
171.60	65	201.40	18				
171.95	457	218.55	103				
172.50	141	249.00	24				
172.80	370						
173.00	606						