

**DATA PACKAGE  
GC SEMI-VOLATILES**

**PROJECT NAME : RAYMARK SUPERFUND SITE**

**NOBIS GROUP**

**585 Middlesex Street**

**Lowell, MA - 01851**

**Phone No: 978-683-0891**

**ORDER ID : Q1730**

**ATTENTION : Adam Roy**



**Laboratory Certification ID # 20012**



<b>1) PCB Data</b>	<b>2</b>
<b>2) Signature Page</b>	<b>4</b>
<b>3) Case Narrative</b>	<b>5</b>
<b>4) Qualifier Page</b>	<b>7</b>
<b>5) Conformance/Non Conformance</b>	<b>8</b>
<b>6) QA Checklist</b>	<b>10</b>
<b>7) Chronicle</b>	<b>11</b>
<b>8) Hit Summary</b>	<b>13</b>
<b>9) QC Data Summary For PCB</b>	<b>14</b>
<b>9.1) Deuterated Monitoring Compound Summary</b>	<b>15</b>
<b>9.2) MS/MSD Summary</b>	<b>18</b>
<b>9.3) LCS/LCSD Summary</b>	<b>20</b>
<b>9.4) Method Blank Summary</b>	<b>21</b>
<b>10) Sample Data</b>	<b>22</b>
<b>10.1) OU4-VSL-15-040325</b>	<b>23</b>
<b>10.2) OU4-VSL-16-040325</b>	<b>27</b>
<b>10.3) OU4-VSL-17-040325</b>	<b>31</b>
<b>10.4) OU4-PCS-TC-21-040325</b>	<b>35</b>
<b>10.5) OU4-PCS-TC-22-040325</b>	<b>39</b>
<b>10.6) OU4-PCS-TC-23-040325</b>	<b>43</b>
<b>10.7) OU4-PCS-TC-24-040325</b>	<b>47</b>
<b>10.8) OU4-PCS-TC-25-040325</b>	<b>51</b>
<b>10.9) OU4-PCS-TC-26-040325</b>	<b>55</b>
<b>10.10) OU4-CF-15-040325</b>	<b>59</b>
<b>11) Calibration Data Summary</b>	<b>63</b>
<b>11.1) Initial Calibration Data</b>	<b>64</b>
<b>11.1.1) PO031925</b>	<b>64</b>
<b>11.1.2) PP032725</b>	<b>283</b>
<b>11.2) Continued Calibration Data</b>	<b>502</b>
<b>11.2.1) PO110263.D</b>	<b>502</b>
<b>11.2.2) PO110278.D</b>	<b>514</b>
<b>11.2.3) PO110286.D</b>	<b>526</b>
<b>11.2.4) PO110292.D</b>	<b>538</b>
<b>11.2.5) PO110302.D</b>	<b>550</b>
<b>11.2.6) PP071136.D</b>	<b>562</b>

<b>11.2.7) PP071151.D</b>	<b>574</b>		
<b>11.3) Analytical Seq</b>	<b>586</b>		
<b>12) Compound Detection Summary</b>	<b>590</b>		
<b>13) QC Sample Data</b>	<b>593</b>		
<b>13.1) Method Blank Data</b>	<b>594</b>		
<b>13.2) PIBLK Data</b>	<b>598</b>		
<b>13.3) LCS Data</b>	<b>634</b>		
<b>13.4) MS Data</b>	<b>643</b>		
<b>13.5) MSD Data</b>	<b>652</b>		
<b>14) Manual Integration</b>	<b>661</b>		
<b>15) Analytical Runlogs</b>	<b>669</b>		
<b>16) Percent Solid</b>	<b>689</b>		
<b>17) Extraction Logs</b>	<b>693</b>		
<b>17.1) PB167469.pdf</b>	<b>693</b>		
<b>17.2) PB167469IC.pdf</b>	<b>695</b>		
<b>18) Standard Prep Logs</b>	<b>696</b>		
<b>19) Shipping Document</b>	<b>784</b>		
<b>19.1) Chain Of Custody</b>	<b>785</b>		
<b>19.2) Lab Certificate</b>	<b>786</b>		
<b>19.3) Internal COC</b>	<b>787</b>		
<b>20) Not Reviewed Data</b>	<b>789</b>		

## Cover Page

**Order ID :** Q1730

**Project ID :** Raymark Superfund Site

**Client :** Nobis Group

### Lab Sample Number

Q1730-01  
Q1730-02  
Q1730-03  
Q1730-04  
Q1730-05  
Q1730-06  
Q1730-07  
Q1730-08  
Q1730-09  
Q1730-10  
Q1730-11  
Q1730-12  
Q1730-13  
Q1730-14  
Q1730-15  
Q1730-16  
Q1730-17  
Q1730-18  
Q1730-19  
Q1730-20

### Client Sample Number

OU4-VSL-15-040325  
OU4-VSL-15-040325  
OU4-VSL-16-040325  
OU4-VSL-16-040325  
OU4-VSL-17-040325  
OU4-VSL-17-040325  
OU4-PCS-TC-21-040325  
OU4-PCS-TC-21-040325  
OU4-PCS-TC-22-040325  
OU4-PCS-TC-22-040325  
OU4-PCS-TC-23-040325  
OU4-PCS-TC-23-040325  
OU4-PCS-TC-24-040325  
OU4-PCS-TC-24-040325  
OU4-PCS-TC-25-040325  
OU4-PCS-TC-25-040325  
OU4-PCS-TC-26-040325  
OU4-PCS-TC-26-040325  
OU4-CF-15-040325  
OU4-CF-15-040325

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

**APPROVED**

Signature :



By Nimisha Pandya, QA/QC Supervisor at 9:19 am, Apr 17, 2025

Date: 4/10/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

## CASE NARRATIVE

**Nobis Group**

**Project Name:** Raymark Superfund Site

**Project # N/A**

**Chemtech Project # Q1730**

**Test Name:** PCB

### **A. Number of Samples and Date of Receipt:**

20 Solid samples were received on 04/04/2025.

### **B. Parameters**

According to the Chain of Custody document, the following analyses were requested: Cyanide, Herbicide Group1, Mercury, Metals ICP-TAL, METALS-TAL, PCB, Pesticide-TCL, SPLP Extraction, SPLP Mercury, SPLP MetalGroup3, SVOCMS Group3 and VOCMS Group3. This data package contains results for PCB.

### **C. Analytical Techniques:**

The analyses were performed on instrument GCECD\_P. The front column is ZB-MR1 which is 30 meters, 0.32 mm ID, 0.5 um df, Catalogue # 7HM-G016-17. The rear column is ZB-MR2 which is 30 meters, 0.32 mm ID, 0.25 µm; Catalogue # 7HM-G017-11. The analyses were performed on instrument GCECD\_O. The front column is ZB-MR1 which is 30 meters, 0.32 mm ID, 0.5 um df, Catalogue # 7HM-G016-17. The rear column is ZB-MR2 which is 30 meters, 0.32 mm ID, 0.25 µm; Catalogue # 7HM-G017-11. The analysis of PCBs was based on method 8082A and extraction was done based on method 3541.

### **D. QA/ QC Samples:**

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria except for OU4-CF-15-040325 [Tetrachloro-m-xylene(2) - 138%]AS per method one surrogate allowed to fail to meet the criteria per column. No further corrective action was taken.

The Retention Times were acceptable for all samples.

The MS recoveries met the requirements for all compounds.

The MSD recoveries met the acceptable requirements.

The RPD met criteria .

The Blank Spike met requirements for all samples .

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements .

The Continuous Calibration met the requirements .



284 Sheffield Street, Mountainside, NJ 07092  
Phone: 908 789 8900 Fax: 908 789 8922

**E. Additional Comments:**

The not QT review data is reported in the Miscellaneous.  
The soil samples results are based on a dry weight basis.

**F. Manual Integration Comments:**

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

---

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

**APPROVED**

*By Nimisha Pandya, QA/QC Supervisor at 9:20 am, Apr 17, 2025*

Signature \_\_\_\_\_

**DATA REPORTING QUALIFIERS- ORGANIC**

For reporting results, the following "Results Qualifiers" are used:

- Value** If the result is a value greater than or equal to the detection limit, report the value
- U** Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
- ND** Indicates the analyte was analyzed for, but not detected
- J** Indicates an estimated value. This flag is used:  
(1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.)  
(2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
- B** Indicates the analyte was found in the blank as well as the sample report as "12 B".
- E** Indicates the analyte's concentration exceeds the calibrated range of the instrument for that specific analysis.
- D** This flag identifies all compounds identified in an analysis at a secondary dilution factor.
- P** This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
- N** This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
- A** This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
- Q** Indicates the LCS did not meet the control limits requirements



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

**GC ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY**

CHEMTECH PROJECT NUMBER: Q1730

MATRIX: Solid

METHOD: 8082A/3541

	NA	NO	YES
1. Chromatograms Labeled/Compounds Identified.			✓
2. Standard Summary Submitted.			✓
3. Calibration - Initial Calibration performed within 30 days before sample analysis and continuing calibration performed within 24 hours of sample analysis, 12 HOURS IF 8000 SERIES METHOD.			✓
The Initial Calibration met the requirements .			
The Continuous Calibration met the requirements .			
4. Blank Contamination - If yes, list compounds and concentrations in each blank:			✓
5. Surrogate Recoveries Meet Criteria			✓
If not met, list those compounds and their recoveries which fall outside the acceptable ranges.			
The Surrogate recoveries met the acceptable criteria except for OU4-CF-15-040325 [Tetrachloro-m-xylene(2) - 138%]AS per method one surrogate allowed to fail to meet the criteria per column. No further corrective action was taken.			
6. Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria			✓
If not met, list those compounds and their recoveries which fall outside the acceptable range.			
The MS recoveries met the requirements for all compounds.			
The MSD recoveries met the acceptable requirements.			
The Blank Spike met requirements for all samples .			
The RPD met criteria .			
7. Retention Time Shift Meet Criteria (if applicable)			✓
Comments:			
8. Extraction Holding Time Met			✓
If not met, list number of days exceeded for each sample:			



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

**GC ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY (CONTINUED)**

NA      NO      YES

9. Analysis Holding Time Met ✓

If not met, list those compounds and their recoveries which fall outside the acceptable range.

**ADDITIONAL COMMENTS:**

The not QT review data is reported in the Miscellaneous.

The soil samples results are based on a dry weight basis.

**REVIEWED**

*By Sohil Jodhani, QA/QC Director at 9:07 am, Apr 17, 2025*

QA REVIEW

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## APPENDIX A

### QA REVIEW GENERAL DOCUMENTATION

Project #: Q1730

Completed

For thorough review, the report must have the following:

#### GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page) ✓

Check chain-of-custody for proper relinquish/return of samples ✓

Is the chain of custody signed and complete ✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts ✓

Collect information for each project id from server. Were all requirements followed ✓

#### COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page ✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody ✓

#### CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results ✓

Do requested analyses on Chain of Custody agree with the log-in page ✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody ✓

Were the samples received within hold time ✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle ✓

#### ANALYTICAL:

Was method requirement followed? ✓

Was client requirement followed? ✓

Does the case narrative summarize all QC failure? ✓

All runlogs and manual integration are reviewed for requirements ✓

All manual calculations and /or hand notations verified ✓

QA Review Signature: SOHIL JODHANI

Date: 04/10/2025

## LAB CHRONICLE

<b>OrderID:</b>	Q1730	<b>OrderDate:</b>	4/4/2025 10:51:00 AM					
<b>Client:</b>	Nobis Group	<b>Project:</b>	Raymark Superfund Site					
<b>Contact:</b>	Adam Roy	<b>Location:</b>	L31, VOA Ref. #2 Soil					
<hr/>								
LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1730-01	OU4-VSL-15-040325	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/07/25	<b>04/04/25</b>
Q1730-03	OU4-VSL-16-040325	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/07/25	<b>04/04/25</b>
Q1730-05	OU4-VSL-17-040325	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/08/25	<b>04/04/25</b>
Q1730-07	OU4-PCS-TC-21-0403 25	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/08/25	<b>04/04/25</b>
Q1730-09	OU4-PCS-TC-22-0403 25	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/08/25	<b>04/04/25</b>
Q1730-11	OU4-PCS-TC-23-0403 25	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/08/25	<b>04/04/25</b>
Q1730-13	OU4-PCS-TC-24-0403 25	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/08/25	<b>04/04/25</b>
Q1730-15	OU4-PCS-TC-25-0403 25	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/08/25	<b>04/04/25</b>
Q1730-17	OU4-PCS-TC-26-0403 25	SOIL	PCB	8082A	<b>04/03/25</b>	04/07/25	04/08/25	<b>04/04/25</b>
Q1730-19	OU4-CF-15-040325	SOIL			<b>04/03/25</b>			<b>04/04/25</b>

---

## LAB CHRONICLE

PCB

8082A

04/07/25

04/08/25

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

### Hit Summary Sheet SW-846

SDG No.: Q1730

Order ID: Q1730

Client: Nobis Group

Project ID: Raymark Superfund Site

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	LOD	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-----	-------

Client ID :

Total Concentration: 0.000

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



# QC

# SUMMARY

### Surrogate Summary

**SDG No.:** Q1730

**Client:** Nobis Group

**Analytical Method:** 8082A

Lab Sample ID	Client ID	Parameter	Limits						
			Column	Spike	Result	Rec	Qual	Low	High
I.BLK-PO109971.D	PIBLK-PO109971.D	Tetrachloro-m-xylene	1	20	18.5	93		60	140
		Decachlorobiphenyl	1	20	20.0	100		60	140
		Tetrachloro-m-xylene	2	20	18.6	93		60	140
		Decachlorobiphenyl	2	20	21.3	107		60	140
I.BLK-PO110267.D	PIBLK-PO110267.D	Tetrachloro-m-xylene	1	20	19.5	97		60	140
		Decachlorobiphenyl	1	20	18.4	92		60	140
		Tetrachloro-m-xylene	2	20	18.8	94		60	140
		Decachlorobiphenyl	2	20	15.9	79		60	140
Q1730-01	OU4-VSL-15-040325	Tetrachloro-m-xylene	1	20	20.2	101		44	130
		Decachlorobiphenyl	1	20	17.6	88		60	125
		Tetrachloro-m-xylene	2	20	19.4	97		44	130
		Decachlorobiphenyl	2	20	15.9	79		60	125
Q1730-03	OU4-VSL-16-040325	Tetrachloro-m-xylene	1	20	22.4	112		44	130
		Decachlorobiphenyl	1	20	19.4	97		60	125
		Tetrachloro-m-xylene	2	20	21.5	108		44	130
		Decachlorobiphenyl	2	20	16.8	84		60	125
Q1730-03MS	OU4-VSL-16-040325MS	Tetrachloro-m-xylene	1	20	22.8	114		44	130
		Decachlorobiphenyl	1	20	20.9	104		60	125
		Tetrachloro-m-xylene	2	20	21.8	109		44	130
		Decachlorobiphenyl	2	20	18.0	90		60	125
Q1730-03MSD	OU4-VSL-16-040325MSD	Tetrachloro-m-xylene	1	20	21.6	108		44	130
		Decachlorobiphenyl	1	20	19.8	99		60	125
		Tetrachloro-m-xylene	2	20	20.8	104		44	130
		Decachlorobiphenyl	2	20	17.3	86		60	125
I.BLK-PO110282.D	PIBLK-PO110282.D	Tetrachloro-m-xylene	1	20	19.3	97		60	140
		Decachlorobiphenyl	1	20	17.2	86		60	140
		Tetrachloro-m-xylene	2	20	18.8	94		60	140
		Decachlorobiphenyl	2	20	16.2	81		60	140
PB167469BL	PB167469BL	Tetrachloro-m-xylene	1	20	19.0	95		44	130
		Decachlorobiphenyl	1	20	17.3	86		60	125
		Tetrachloro-m-xylene	2	20	18.3	91		44	130
		Decachlorobiphenyl	2	20	16.0	80		60	125
PB167469BS	PB167469BS	Tetrachloro-m-xylene	1	20	19.9	99		44	130
		Decachlorobiphenyl	1	20	19.1	95		60	125
		Tetrachloro-m-xylene	2	20	18.9	95		44	130
		Decachlorobiphenyl	2	20	17.3	86		60	125
I.BLK-PO110290.D	PIBLK-PO110290.D	Tetrachloro-m-xylene	1	20	19.5	98		60	140
		Decachlorobiphenyl	1	20	17.7	89		60	140
		Tetrachloro-m-xylene	2	20	18.9	94		60	140
		Decachlorobiphenyl	2	20	16.2	81		60	140
I.BLK-PO110296.D	PIBLK-PO110296.D	Tetrachloro-m-xylene	1	20	18.7	93		60	140

### Surrogate Summary

**SDG No.:** Q1730

**Client:** Nobis Group

**Analytical Method:** 8082A

Lab Sample ID	Client ID	Parameter	Limits						
			Column	Spike	Result	Rec	Qual	Low	High
I.BLK-PO110296.D	PIBLK-PO110296.D	Decachlorobiphenyl	1	20	17.8	89		60	140
		Tetrachloro-m-xylene	2	20	17.7	89		60	140
		Decachlorobiphenyl	2	20	15.4	77		60	140
		Tetrachloro-m-xylene	1	20	23.2	116		44	130
		Decachlorobiphenyl	1	20	21.1	105		60	125
		Tetrachloro-m-xylene	2	20	22.1	110		44	130
Q1730-05	OU4-VSL-17-040325	Decachlorobiphenyl	2	20	18.1	91		60	125
		Tetrachloro-m-xylene	1	20	20.3	102		44	130
		Decachlorobiphenyl	1	20	17.1	85		60	125
		Tetrachloro-m-xylene	2	20	19.2	96		44	130
		Decachlorobiphenyl	2	20	14.1	71		60	125
		Tetrachloro-m-xylene	1	20	20.7	104		44	130
Q1730-07	OU4-PCS-TC-21-040325	Decachlorobiphenyl	1	20	17.9	90		60	125
		Tetrachloro-m-xylene	2	20	19.7	98		44	130
		Decachlorobiphenyl	2	20	14.8	74		60	125
		Tetrachloro-m-xylene	1	20	20.9	104		44	130
		Decachlorobiphenyl	1	20	18.0	90		60	125
		Tetrachloro-m-xylene	2	20	19.9	99		44	130
Q1730-09	OU4-PCS-TC-22-040325	Decachlorobiphenyl	2	20	14.8	74		60	125
		Tetrachloro-m-xylene	1	20	20.7	104		44	130
		Decachlorobiphenyl	1	20	17.9	90		60	125
		Tetrachloro-m-xylene	2	20	19.7	98		44	130
		Decachlorobiphenyl	2	20	14.8	74		60	125
		Tetrachloro-m-xylene	1	20	20.9	104		44	130
Q1730-11	OU4-PCS-TC-23-040325	Decachlorobiphenyl	1	20	18.0	90		60	125
		Tetrachloro-m-xylene	2	20	19.9	99		44	130
		Decachlorobiphenyl	2	20	14.8	74		60	125
		Tetrachloro-m-xylene	1	20	20.5	102		44	130
		Decachlorobiphenyl	1	20	18.9	94		60	125
		Tetrachloro-m-xylene	2	20	19.4	97		44	130
Q1730-13	OU4-PCS-TC-24-040325	Decachlorobiphenyl	2	20	14.8	74		60	125
		Tetrachloro-m-xylene	1	20	20.5	102		44	130
		Decachlorobiphenyl	1	20	18.9	94		60	125
		Tetrachloro-m-xylene	2	20	19.4	97		44	130
		Decachlorobiphenyl	2	20	15.7	78		60	125
		Tetrachloro-m-xylene	1	20	18.2	91		60	140
I.BLK-PO110306.D	PIBLK-PO110306.D	Decachlorobiphenyl	1	20	18.4	92		60	140
		Tetrachloro-m-xylene	2	20	17.4	87		60	140
		Decachlorobiphenyl	2	20	15.3	77		60	140
		Tetrachloro-m-xylene	1	20	18.8	94		60	140
		Decachlorobiphenyl	1	20	19.4	97		60	140
		Tetrachloro-m-xylene	2	20	18.1	91		60	140
I.BLK-PP070916.D	PIBLK-PP070916.D	Decachlorobiphenyl	2	20	23.4	117		60	140
		Tetrachloro-m-xylene	1	20	22.8	114		60	140
		Decachlorobiphenyl	1	20	23.9	119		60	140
		Tetrachloro-m-xylene	2	20	23.1	116		60	140
		Decachlorobiphenyl	2	20	21.5	108		60	140
		Tetrachloro-m-xylene	1	20	24.7	123		44	130
Q1730-15	OU4-PCS-TC-25-040325	Decachlorobiphenyl	1	20	23.3	116		60	125
		Tetrachloro-m-xylene	2	20	24.8	124		44	130
		Decachlorobiphenyl	2	20	20.5	102		60	125
		Tetrachloro-m-xylene	1	20	25.1	125		44	130
		Decachlorobiphenyl	1	20	24.9	124		60	125
		Tetrachloro-m-xylene	1	20	24.9	124		60	125

### Surrogate Summary

SDG No.: **Q1730**

Client: **Nobis Group**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Limits						
			Column	Spike	Result	Rec	Qual	Low	High
Q1730-17	OU4-PCS-TC-26-040325	Tetrachloro-m-xylene	2	20	24.8	124		44	130
		Decachlorobiphenyl	2	20	22.0	110		60	125
Q1730-19	OU4-CF-15-040325	Tetrachloro-m-xylene	1	20	25.8	129		44	130
		Decachlorobiphenyl	1	20	24.1	121		60	125
		Tetrachloro-m-xylene	2	20	27.5	138	*	44	130
		Decachlorobiphenyl	2	20	21.7	108		60	125
I.BLK-PP071155.D	PIBLK-PP071155.D	Tetrachloro-m-xylene	1	20	20.6	103		60	140
		Decachlorobiphenyl	1	20	21.0	105		60	140
		Tetrachloro-m-xylene	2	20	21.1	105		60	140
		Decachlorobiphenyl	2	20	18.4	92		60	140

### Matrix Spike/Matrix Spike Duplicate Summary

**SW-846**

**SDG No.:** Q1730

**Client:** Nobis Group

**Analytical Method:** 8082A

**DataFile :** PO110271.D

<b>Lab Sample ID:</b>	<b>Parameter</b>	<b>Spike</b>	Sample			<b>Rec</b>	<b>Rec Qual</b>	<b>RPD</b>	<b>RPD Qual</b>	<b>Limits</b>	
			<b>Result</b>	<b>Result</b>	<b>Units</b>					<b>Low</b>	<b>High</b>
<b>Client Sample ID:</b> <b>OU4-VSL-16-040325MS</b>											
Q1730-03MS	AR1016	176.1	0	170	ug/kg	97			47	134	
	AR1260	176.1	0	157	ug/kg	89			53	140	

### Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q1730

Client: Nobis Group

Analytical Method: 8082A

DataFile : PO110272.D

Lab Sample ID:	Parameter	Spike	Sample			Rec	Rec Qual	RPD	RPD Qual	Limits		RPD
			Result	Result	Units					Low	High	
Client Sample ID:	<b>OU4-VSL-16-040325MSD</b>											
Q1730-03MSD	AR1016	176.2	0	164	ug/kg	93		4		47	134	20
	AR1260	176.2	0	153	ug/kg	87		2		53	140	20

### Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q1730

Client: Nobis Group

Analytical Method: 8082A

Datafile : PO110284.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD	Limits		RPD	
									Qual	Low	High	
PB167469BS	AR1016	166.6	141	ug/kg	85					47	134	
	AR1260	166.6	134	ug/kg	80					53	140	

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB167469BL

Lab Name: CHEMTECH

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730

SAS No.: Q1730 SDG NO.: Q1730

Lab Sample ID: PB167469BL

Lab File ID: PO110283.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 04/07/2025

Date Analyzed (1): 04/07/2025

Date Analyzed (2): 04/07/2025

Time Analyzed (1): 19:22

Time Analyzed (2): 19:22

Instrument ID (1): ECD\_O

Instrument ID (2): ECD\_O

GC Column (1): ZB-MR1

ID: 0.32 (mm)

GC Column (2): ZB-MR2

ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
OU4-VSL-15-040325	Q1730-01	PO110269.D	04/07/2025	04/07/2025
OU4-VSL-16-040325	Q1730-03	PO110270.D	04/07/2025	04/07/2025
OU4-VSL-16-040325MS	Q1730-03MS	PO110271.D	04/07/2025	04/07/2025
OU4-VSL-16-040325MSD	Q1730-03MSD	PO110272.D	04/07/2025	04/07/2025
PB167469BS	PB167469BS	PO110284.D	04/07/2025	04/07/2025
OU4-VSL-17-040325	Q1730-05	PO110297.D	04/08/2025	04/08/2025
OU4-PCS-TC-21-040325	Q1730-07	PO110298.D	04/08/2025	04/08/2025
OU4-PCS-TC-22-040325	Q1730-09	PO110299.D	04/08/2025	04/08/2025
OU4-PCS-TC-23-040325	Q1730-11	PO110300.D	04/08/2025	04/08/2025
OU4-PCS-TC-24-040325	Q1730-13	PO110301.D	04/08/2025	04/08/2025
OU4-PCS-TC-25-040325	Q1730-15	PP071142.D	04/08/2025	04/08/2025
OU4-PCS-TC-26-040325	Q1730-17	PP071143.D	04/08/2025	04/08/2025
OU4-CF-15-040325	Q1730-19	PP071144.D	04/08/2025	04/08/2025

COMMENTS:



# SAMPLE

# DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-VSL-15-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-01			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	96.9	Decanted:
Sample Wt/Vol:	30.07	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110269.D	1	04/07/25 08:20	04/07/25 13:38	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	8.50	U	4.10	8.50	17.5	ug/kg
11104-28-2	Aroclor-1221	13.4	U	4.10	13.4	17.5	ug/kg
11141-16-5	Aroclor-1232	8.50	U	3.80	8.50	17.5	ug/kg
53469-21-9	Aroclor-1242	8.50	U	4.10	8.50	17.5	ug/kg
12672-29-6	Aroclor-1248	13.4	U	6.10	13.4	17.5	ug/kg
11097-69-1	Aroclor-1254	8.50	U	3.30	8.50	17.5	ug/kg
37324-23-5	Aroclor-1262	13.4	U	5.20	13.4	17.5	ug/kg
11100-14-4	Aroclor-1268	8.50	U	3.70	8.50	17.5	ug/kg
11096-82-5	Aroclor-1260	8.50	U	3.30	8.50	17.5	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	20.2		44 - 130		101%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.6		60 - 125		88%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110269.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 13:38  
 Operator : YP/AJ  
 Sample : Q1730-01  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-VSL-15-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 14:27:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	3.690	3.687	183.9E6	101.8E6	20.206	19.404
2) SA Decachloro...	8.741	8.690	135.7E6	38509502	17.644	15.873

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110269.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 13:38  
 Operator : YP/AJ  
 Sample : Q1730-01  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-VSL-15-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 14:27:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

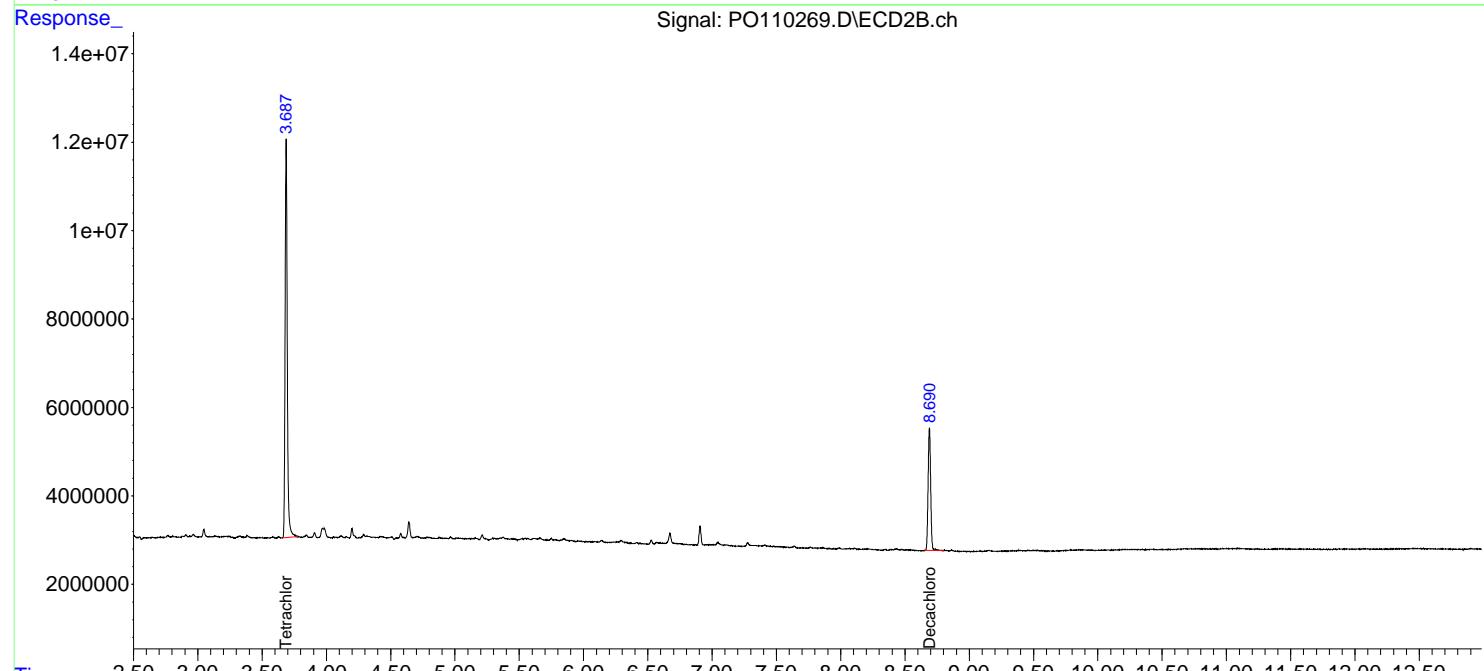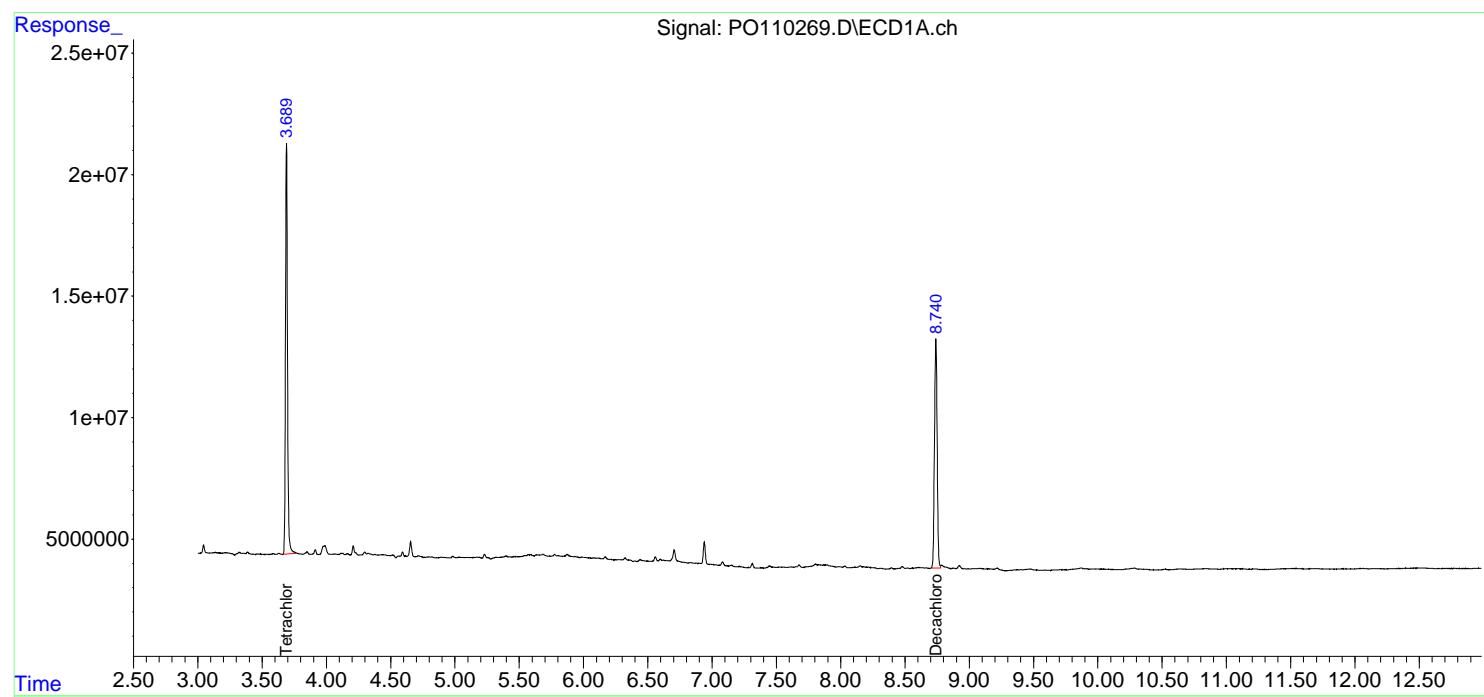

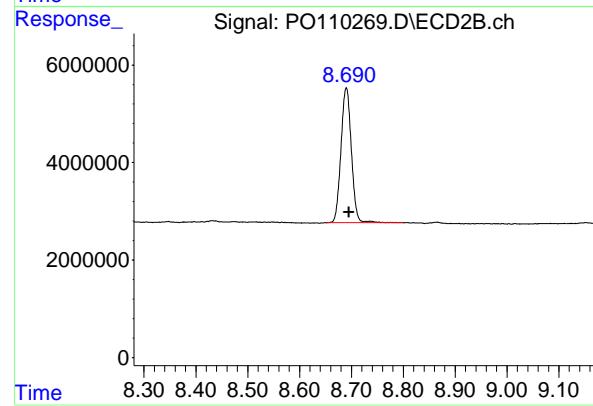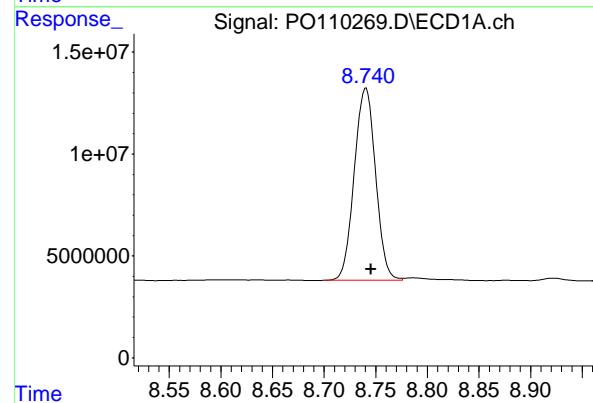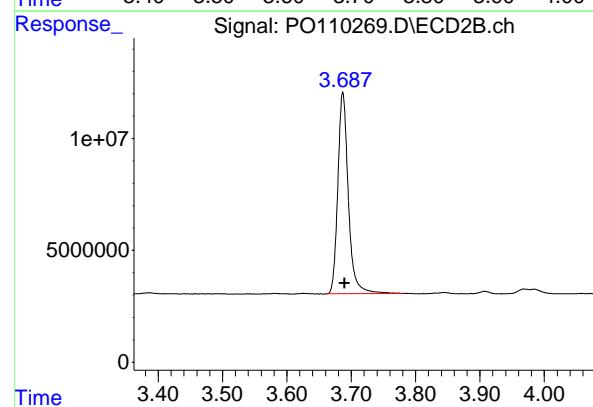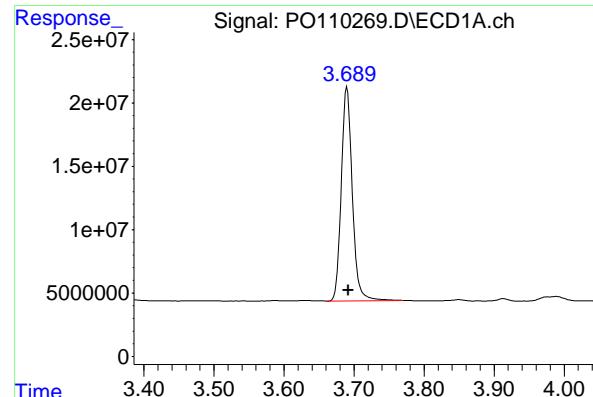

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: -0.002 min  
 Response: 183908751  
 Conc: 20.21 ng/ml

Instrument: ECD\_O  
 ClientSampleId: OU4-VSL-15-040325

## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
 Delta R.T.: -0.003 min  
 Response: 101756501  
 Conc: 19.40 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.741 min  
 Delta R.T.: -0.005 min  
 Response: 135656538  
 Conc: 17.64 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.690 min  
 Delta R.T.: -0.006 min  
 Response: 38509502  
 Conc: 15.87 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-VSL-16-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-03			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	94.5	Decanted:
Sample Wt/Vol:	30.03	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110270.D	1	04/07/25 08:20	04/07/25 13:56	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	8.80	U	4.20	8.80	18.0	ug/kg
11104-28-2	Aroclor-1221	13.7	U	4.30	13.7	18.0	ug/kg
11141-16-5	Aroclor-1232	8.80	U	3.90	8.80	18.0	ug/kg
53469-21-9	Aroclor-1242	8.80	U	4.20	8.80	18.0	ug/kg
12672-29-6	Aroclor-1248	13.7	U	6.30	13.7	18.0	ug/kg
11097-69-1	Aroclor-1254	8.80	U	3.40	8.80	18.0	ug/kg
37324-23-5	Aroclor-1262	13.7	U	5.30	13.7	18.0	ug/kg
11100-14-4	Aroclor-1268	8.80	U	3.80	8.80	18.0	ug/kg
11096-82-5	Aroclor-1260	8.80	U	3.40	8.80	18.0	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	22.4		44 - 130		112%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.4		60 - 125		97%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110270.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 13:56  
 Operator : YP/AJ  
 Sample : Q1730-03  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-VSL-16-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 14:27:50 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachlor...	3.690	3.687	203.6E6	112.9E6	22.365	21.523
2) SA Decachlor...	8.740	8.690	149.1E6	40812607	19.387	16.822

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110270.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 13:56  
 Operator : YP/AJ  
 Sample : Q1730-03  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-VSL-16-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 14:27:50 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

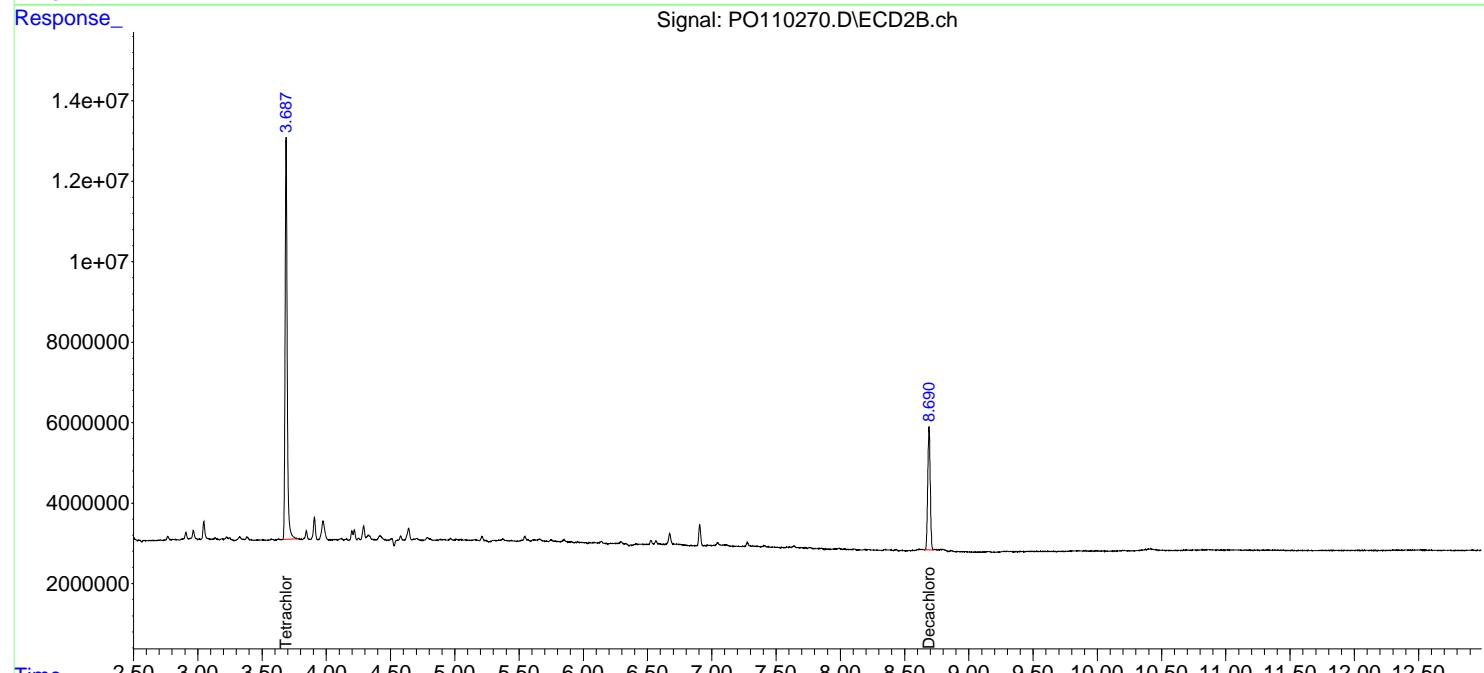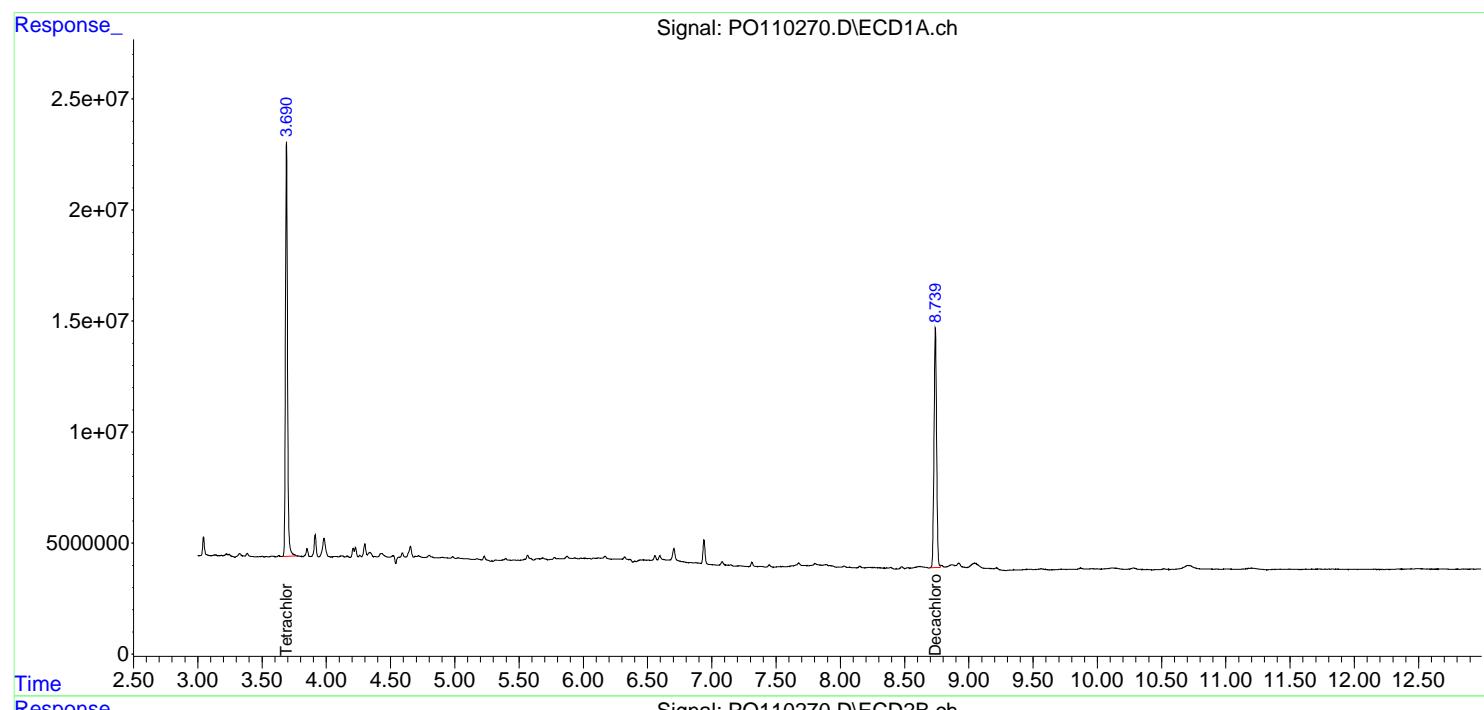

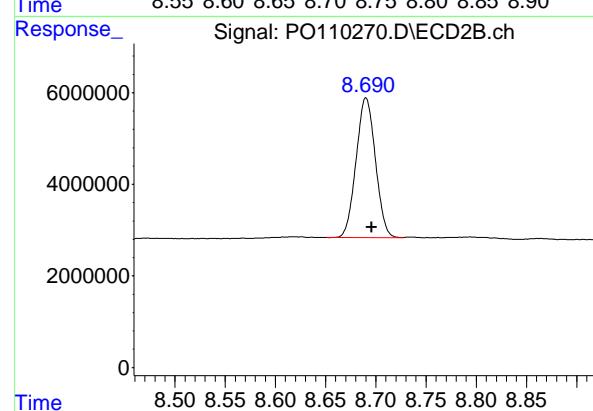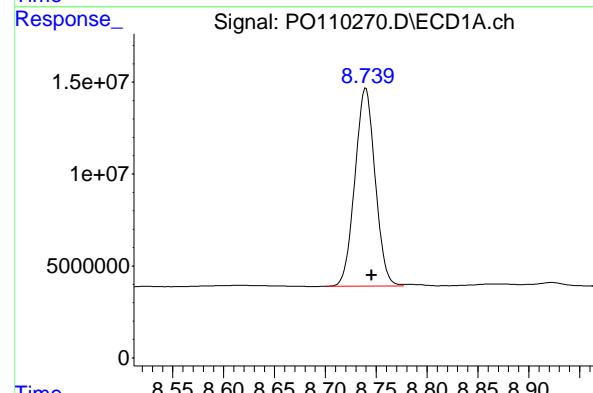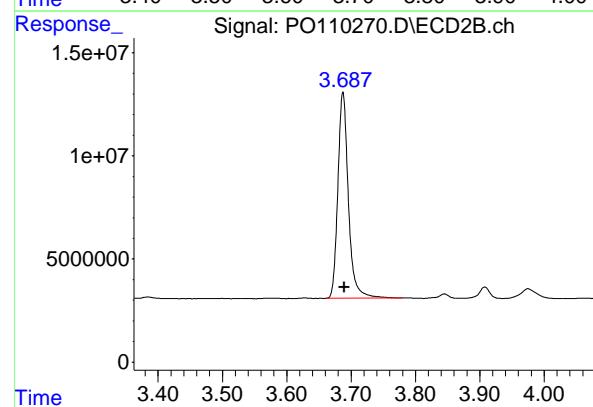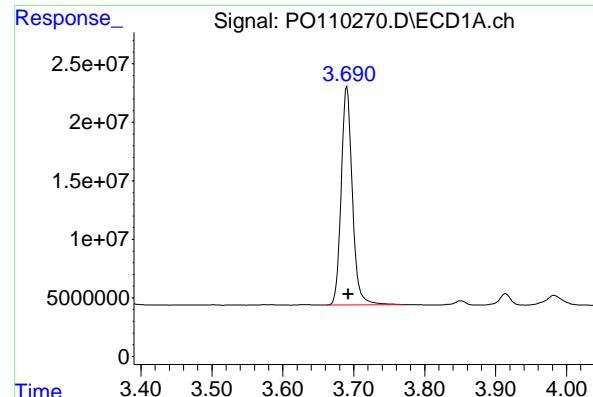

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: -0.002 min  
 Response: 203553270  
 Conc: 22.36 ng/ml

Instrument: ECD\_O  
 ClientSampleId: OU4-VSL-16-040325

## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
 Delta R.T.: -0.002 min  
 Response: 112868485  
 Conc: 21.52 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.740 min  
 Delta R.T.: -0.006 min  
 Response: 149058190  
 Conc: 19.39 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.690 min  
 Delta R.T.: -0.006 min  
 Response: 40812607  
 Conc: 16.82 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-VSL-17-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-05			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	92.4	Decanted:
Sample Wt/Vol:	30.08	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110297.D	1	04/07/25 08:20	04/08/25 10:39	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	9.00	U	4.30	9.00	18.3	ug/kg
11104-28-2	Aroclor-1221	14.0	U	4.30	14.0	18.3	ug/kg
11141-16-5	Aroclor-1232	9.00	U	4.00	9.00	18.3	ug/kg
53469-21-9	Aroclor-1242	9.00	U	4.30	9.00	18.3	ug/kg
12672-29-6	Aroclor-1248	14.0	U	6.40	14.0	18.3	ug/kg
11097-69-1	Aroclor-1254	9.00	U	3.50	9.00	18.3	ug/kg
37324-23-5	Aroclor-1262	14.0	U	5.40	14.0	18.3	ug/kg
11100-14-4	Aroclor-1268	9.00	U	3.90	9.00	18.3	ug/kg
11096-82-5	Aroclor-1260	9.00	U	3.50	9.00	18.3	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	23.2		44 - 130		116%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.1		60 - 125		105%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110297.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 10:39  
 Operator : YP/AJ  
 Sample : Q1730-05  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-VSL-17-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:13:12 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.688	211.3E6	115.8E6	23.218	22.077
2) SA Decachlor...	8.740	8.691	162.1E6	43918378	21.086	18.102

#### Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110297.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 10:39  
 Operator : YP/AJ  
 Sample : Q1730-05  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-VSL-17-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:13:12 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

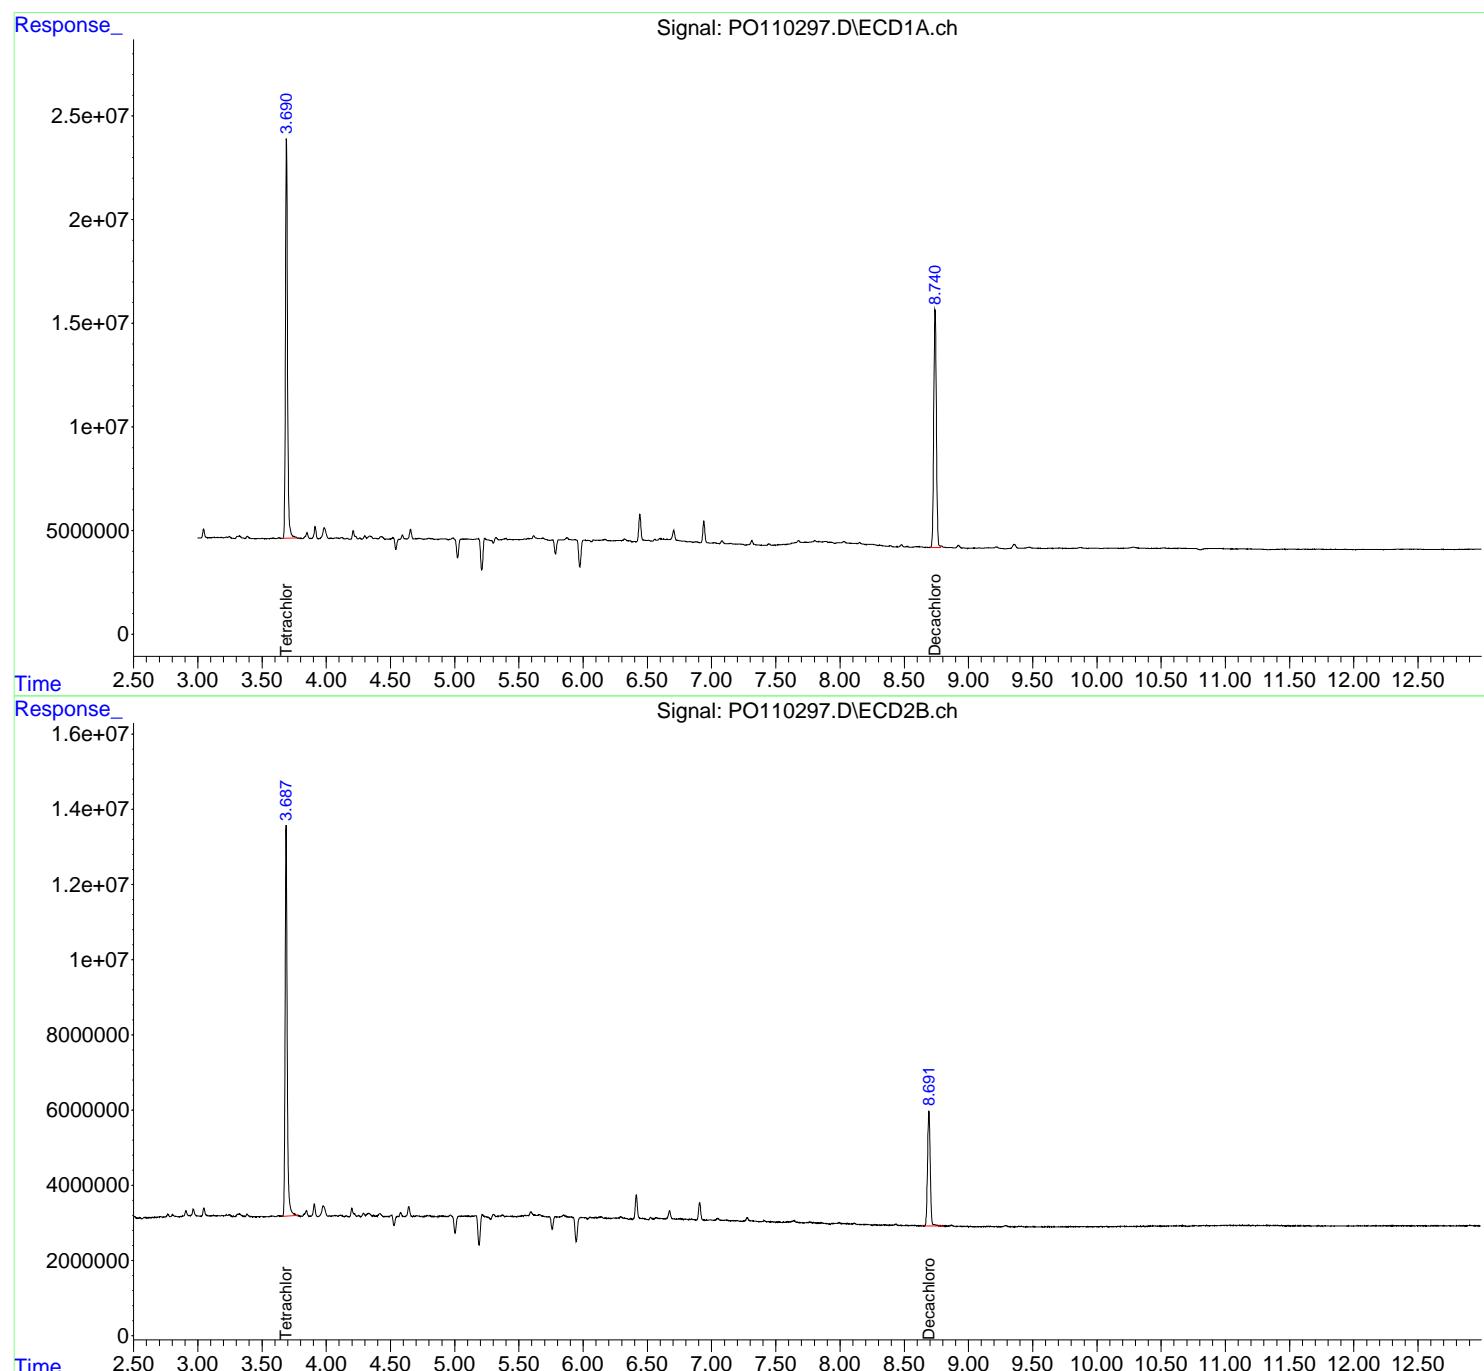

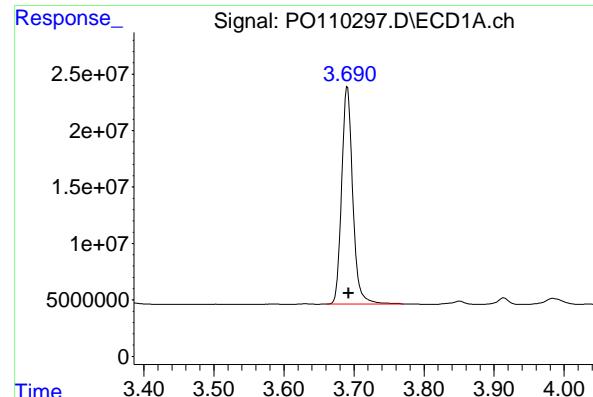


## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: -0.001 min  
 Response: 211317711 ECD\_O  
 Conc: 23.22 ng/ml ClientSampleId : OU4-VSL-17-040325

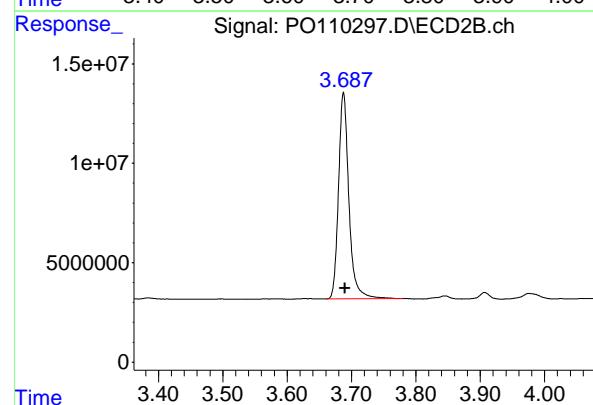


## #1 Tetrachloro-m-xylene

R.T.: 3.688 min  
 Delta R.T.: -0.002 min  
 Response: 115771341  
 Conc: 22.08 ng/ml

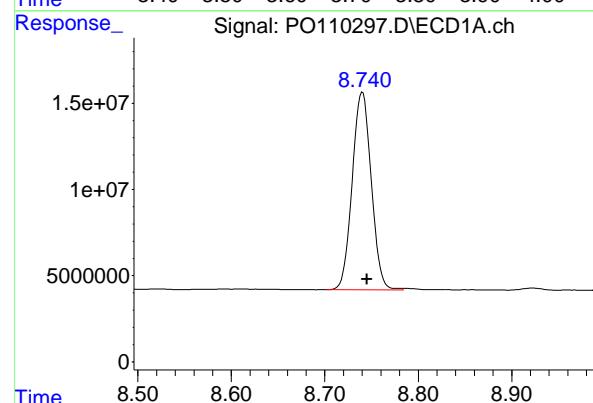

## #2 Decachlorobiphenyl

R.T.: 8.740 min  
 Delta R.T.: -0.005 min  
 Response: 162122100  
 Conc: 21.09 ng/ml

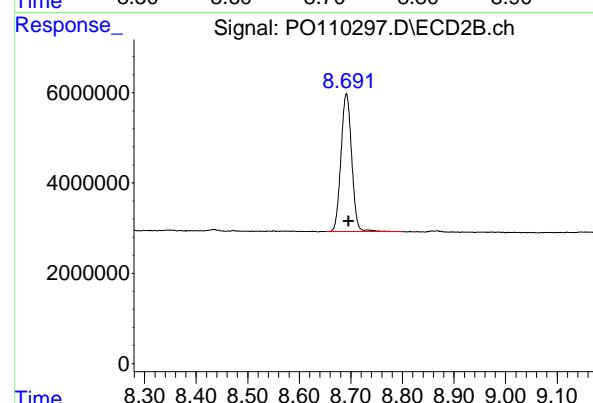

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
 Delta R.T.: -0.004 min  
 Response: 43918378  
 Conc: 18.10 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-PCS-TC-21-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-07			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	89	Decanted:
Sample Wt/Vol:	30.01	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110298.D	1	04/07/25 08:20	04/08/25 10:58	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	9.30	U	4.40	9.30	19.1	ug/kg
11104-28-2	Aroclor-1221	14.6	U	4.50	14.6	19.1	ug/kg
11141-16-5	Aroclor-1232	9.30	U	4.20	9.30	19.1	ug/kg
53469-21-9	Aroclor-1242	9.30	U	4.50	9.30	19.1	ug/kg
12672-29-6	Aroclor-1248	14.6	U	6.60	14.6	19.1	ug/kg
11097-69-1	Aroclor-1254	9.30	U	3.60	9.30	19.1	ug/kg
37324-23-5	Aroclor-1262	14.6	U	5.60	14.6	19.1	ug/kg
11100-14-4	Aroclor-1268	9.30	U	4.00	9.30	19.1	ug/kg
11096-82-5	Aroclor-1260	9.30	U	3.60	9.30	19.1	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	20.3	44 - 130		102%	SPK: 20	
2051-24-3	Decachlorobiphenyl	17.1	60 - 125		85%	SPK: 20	

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110298.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 10:58  
 Operator : YP/AJ  
 Sample : Q1730-07  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
OU4-PCS-TC-21-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:14:05 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	3.690	3.687	184.9E6	100.8E6	20.313	19.219
2) SA Decachloro...	8.741	8.692	131.1E6	34240978	17.046	14.114

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110298.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 10:58  
 Operator : YP/AJ  
 Sample : Q1730-07  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 OU4-PCS-TC-21-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:14:05 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

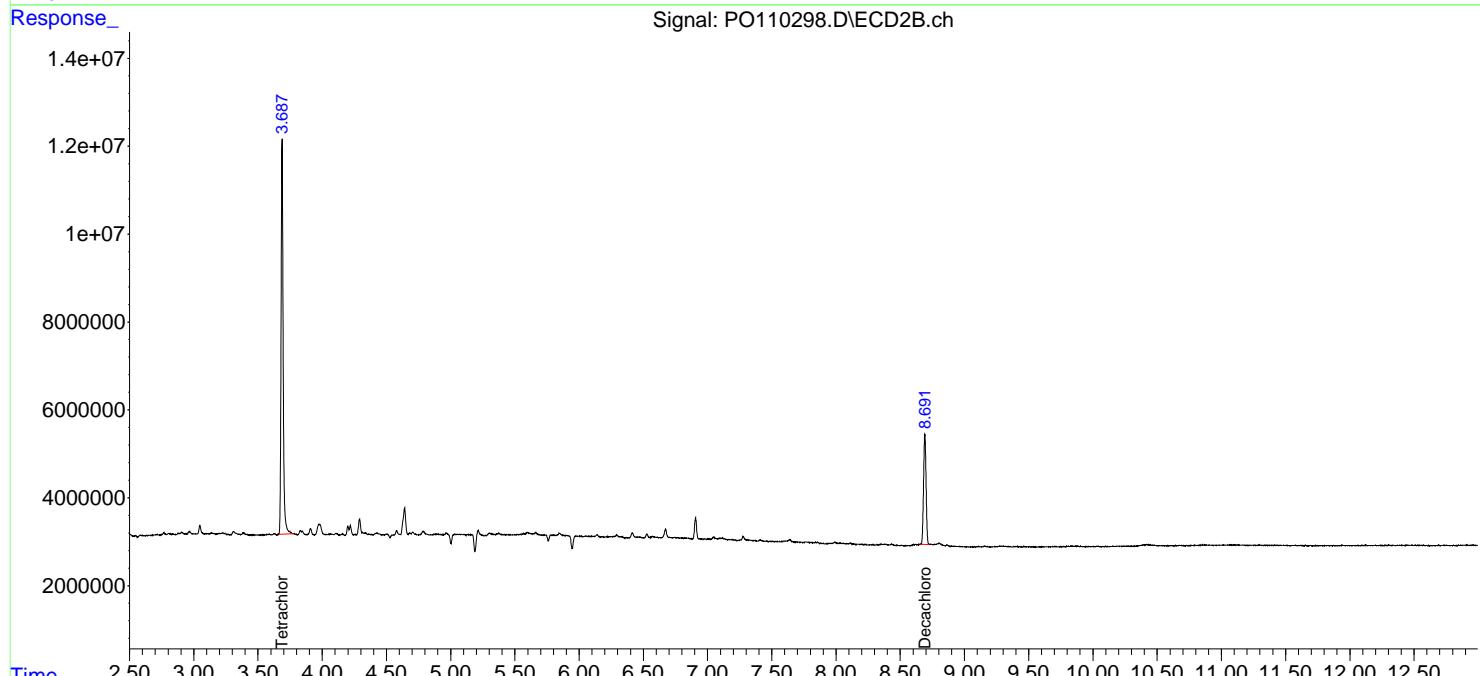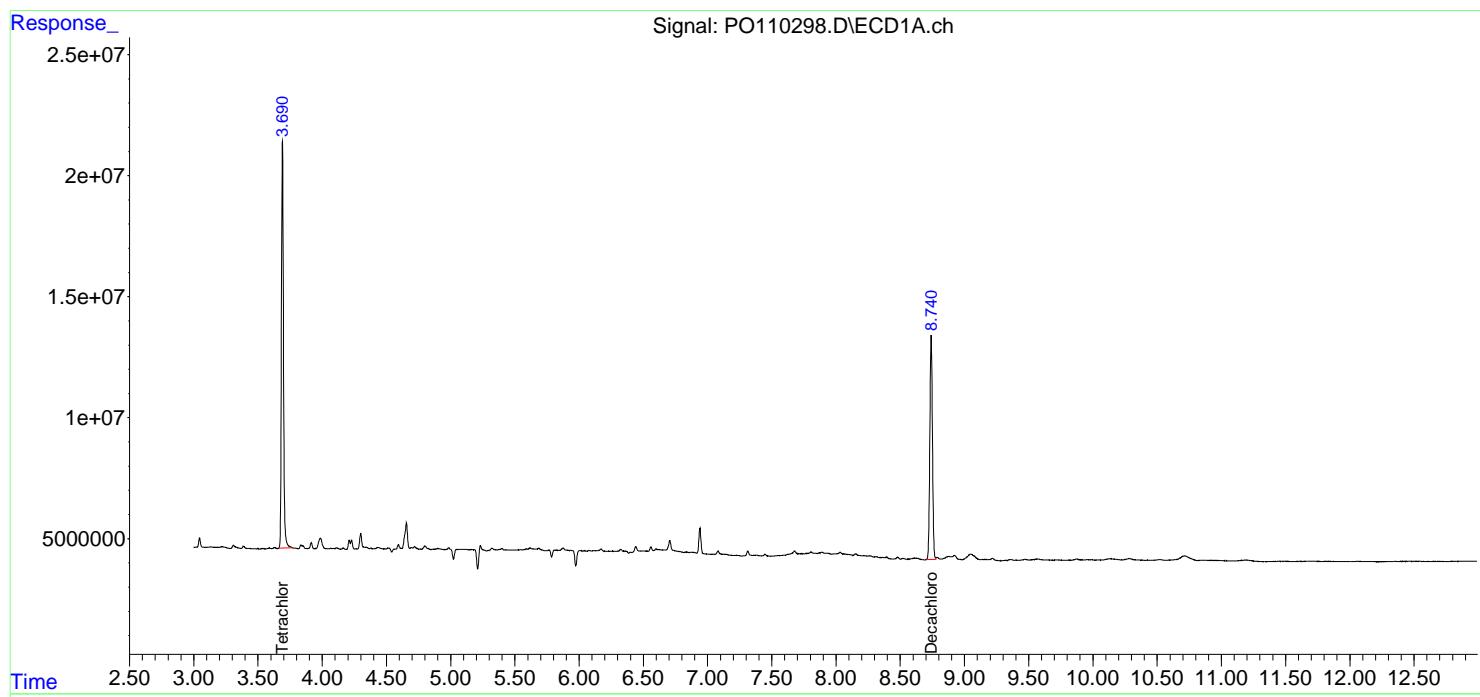

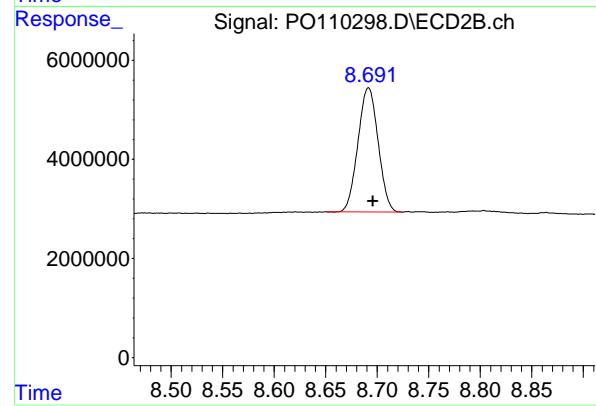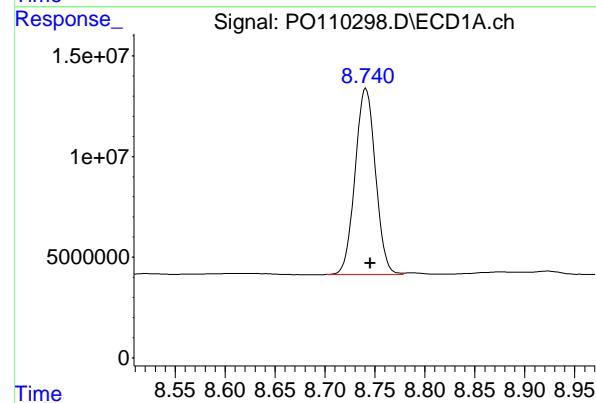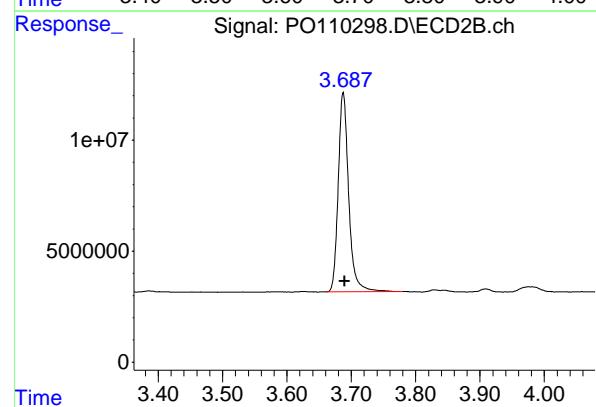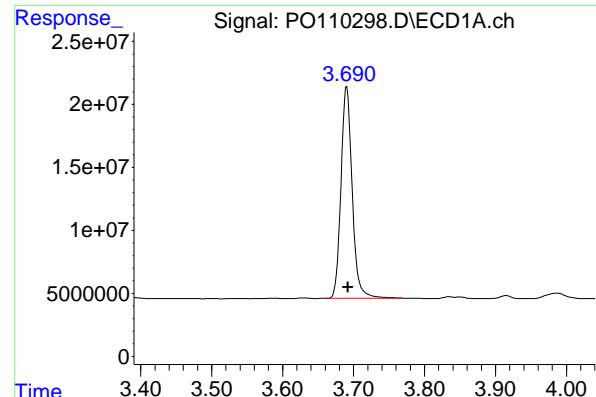

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: -0.002 min  
 Response: 184875104 ECD\_O  
 Conc: 20.31 ng/ml ClientSampleId : OU4-PCS-TC-21-040325

## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
 Delta R.T.: -0.002 min  
 Response: 100787167 ECD\_O  
 Conc: 19.22 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.741 min  
 Delta R.T.: -0.004 min  
 Response: 131063538 ECD\_O  
 Conc: 17.05 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.692 min  
 Delta R.T.: -0.004 min  
 Response: 34240978 ECD\_O  
 Conc: 14.11 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-PCS-TC-22-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-09			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	90.8	Decanted:
Sample Wt/Vol:	30.02	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110299.D	1	04/07/25 08:20	04/08/25 11:16	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	9.10	U	4.30	9.10	18.7	ug/kg
11104-28-2	Aroclor-1221	14.3	U	4.40	14.3	18.7	ug/kg
11141-16-5	Aroclor-1232	9.10	U	4.10	9.10	18.7	ug/kg
53469-21-9	Aroclor-1242	9.10	U	4.40	9.10	18.7	ug/kg
12672-29-6	Aroclor-1248	14.3	U	6.50	14.3	18.7	ug/kg
11097-69-1	Aroclor-1254	9.10	U	3.50	9.10	18.7	ug/kg
37324-23-5	Aroclor-1262	14.3	U	5.50	14.3	18.7	ug/kg
11100-14-4	Aroclor-1268	9.10	U	4.00	9.10	18.7	ug/kg
11096-82-5	Aroclor-1260	9.10	U	3.60	9.10	18.7	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	20.7		44 - 130		104%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.9		60 - 125		90%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110299.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:16  
 Operator : YP/AJ  
 Sample : Q1730-09  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
OU4-PCS-TC-22-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:32:32 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	3.690	3.688	188.8E6	103.3E6	20.743	19.690
2) SA Decachloro...	8.741	8.692	138.0E6	35929484	17.943	14.810

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110299.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:16  
 Operator : YP/AJ  
 Sample : Q1730-09  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 OU4-PCS-TC-22-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:32:32 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

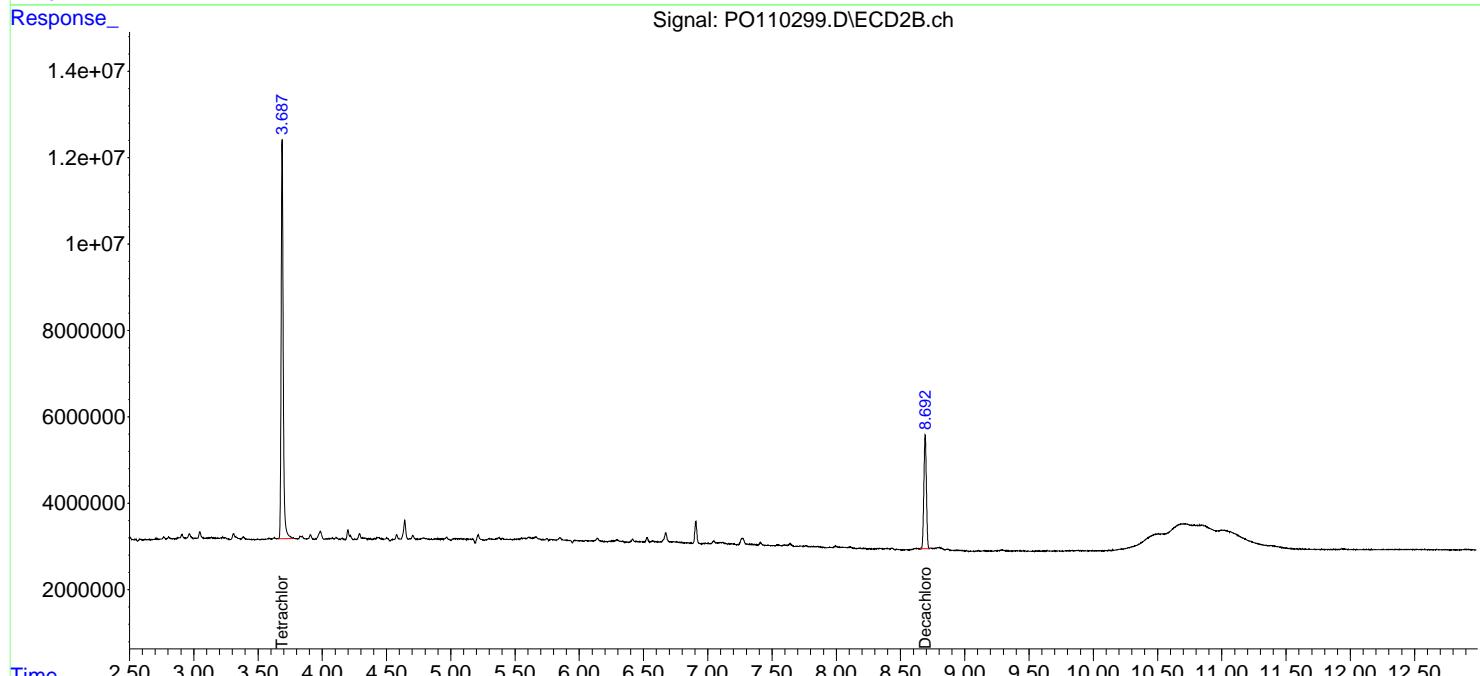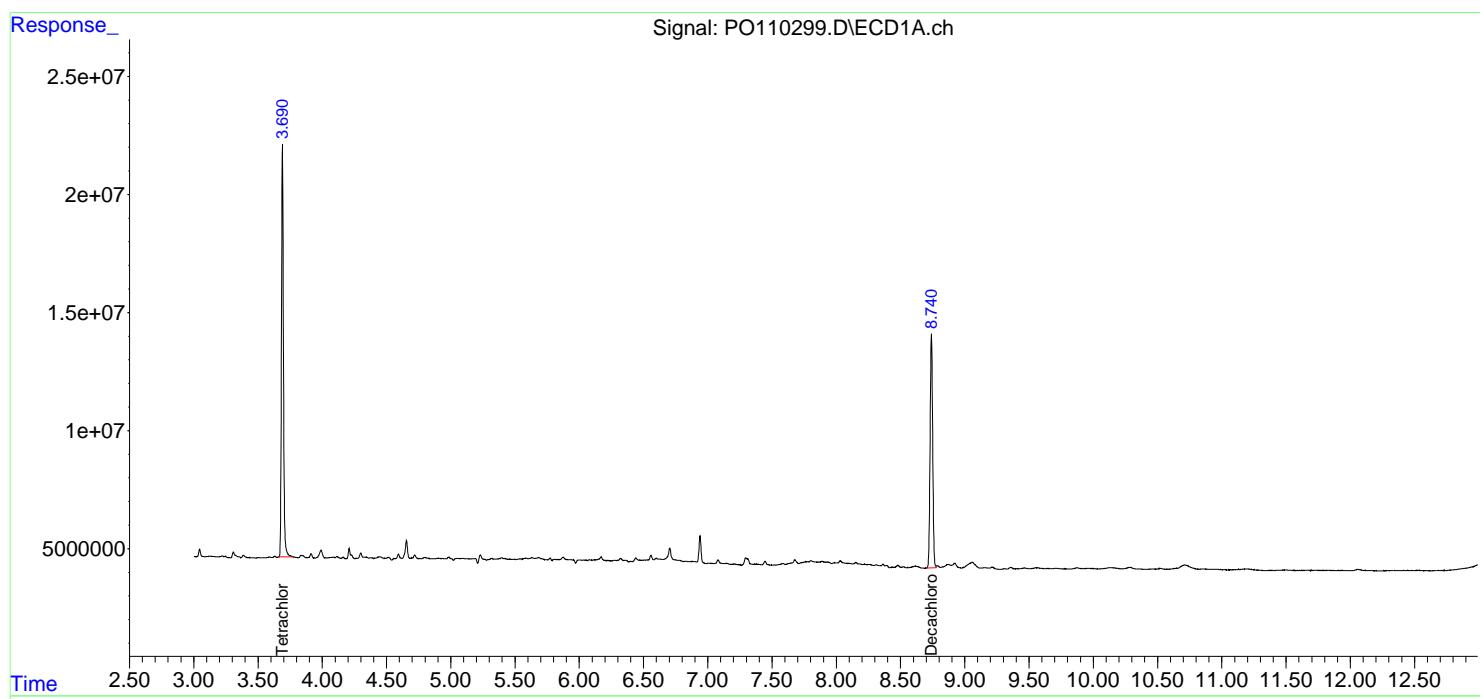

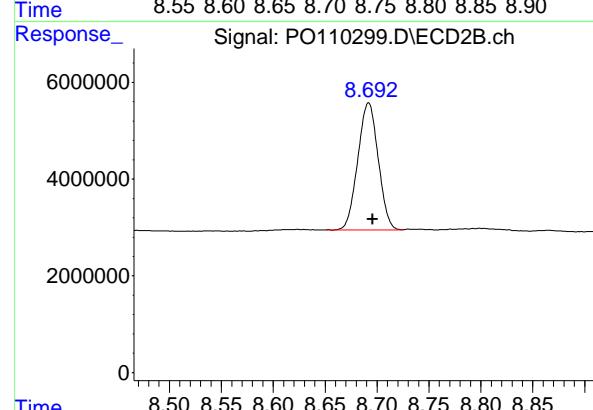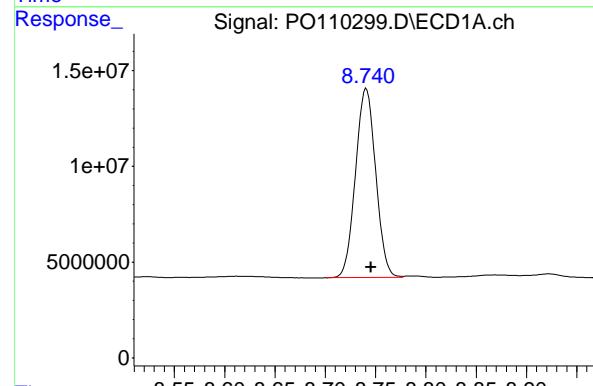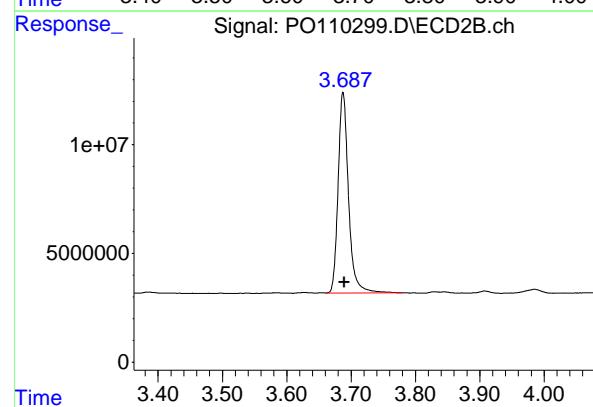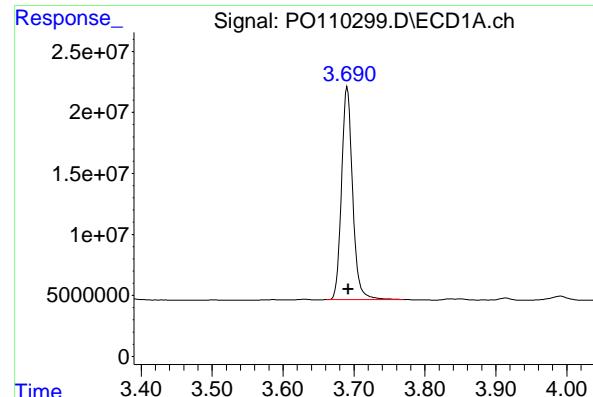

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: -0.002 min  
 Response: 188790826  
 Conc: 20.74 ng/ml

Instrument: ECD\_O  
 ClientSampleId: OU4-PCS-TC-22-040325

## #1 Tetrachloro-m-xylene

R.T.: 3.688 min  
 Delta R.T.: -0.002 min  
 Response: 103254489  
 Conc: 19.69 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.741 min  
 Delta R.T.: -0.005 min  
 Response: 137955475  
 Conc: 17.94 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.692 min  
 Delta R.T.: -0.004 min  
 Response: 35929484  
 Conc: 14.81 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-PCS-TC-23-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-11			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	90.9	Decanted:
Sample Wt/Vol:	30.05	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110300.D	1	04/07/25 08:20	04/08/25 11:35	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	9.10	U	4.30	9.10	18.7	ug/kg
11104-28-2	Aroclor-1221	14.3	U	4.40	14.3	18.7	ug/kg
11141-16-5	Aroclor-1232	9.10	U	4.10	9.10	18.7	ug/kg
53469-21-9	Aroclor-1242	9.10	U	4.40	9.10	18.7	ug/kg
12672-29-6	Aroclor-1248	14.3	U	6.50	14.3	18.7	ug/kg
11097-69-1	Aroclor-1254	9.10	U	3.50	9.10	18.7	ug/kg
37324-23-5	Aroclor-1262	14.3	U	5.50	14.3	18.7	ug/kg
11100-14-4	Aroclor-1268	9.10	U	4.00	9.10	18.7	ug/kg
11096-82-5	Aroclor-1260	9.10	U	3.50	9.10	18.7	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	20.9		44 - 130		104%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.0		60 - 125		90%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110300.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:35  
 Operator : YP/AJ  
 Sample : Q1730-11  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
OU4-PCS-TC-23-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:51:20 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	3.691	3.687	189.8E6	104.3E6	20.849	19.893
2) SA Decachloro...	8.740	8.692	138.3E6	35798912	17.988	14.756

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110300.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:35  
 Operator : YP/AJ  
 Sample : Q1730-11  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 OU4-PCS-TC-23-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:51:20 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

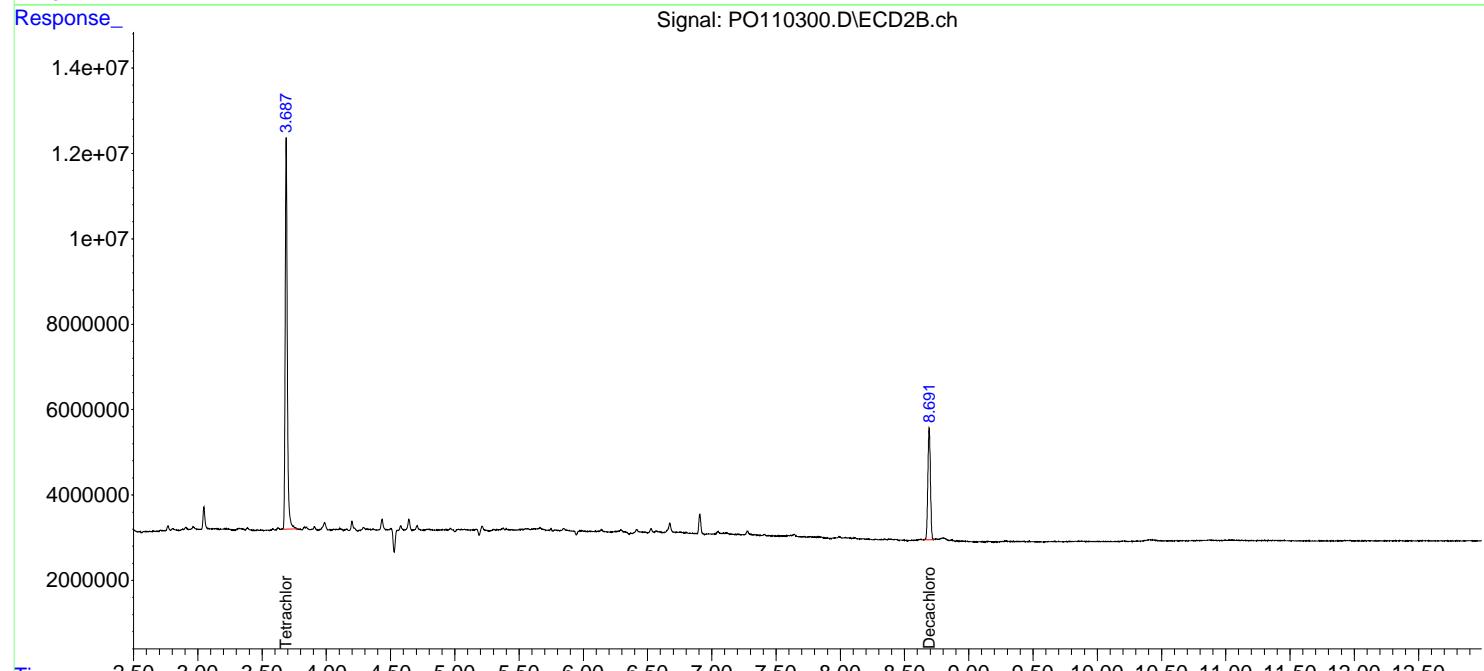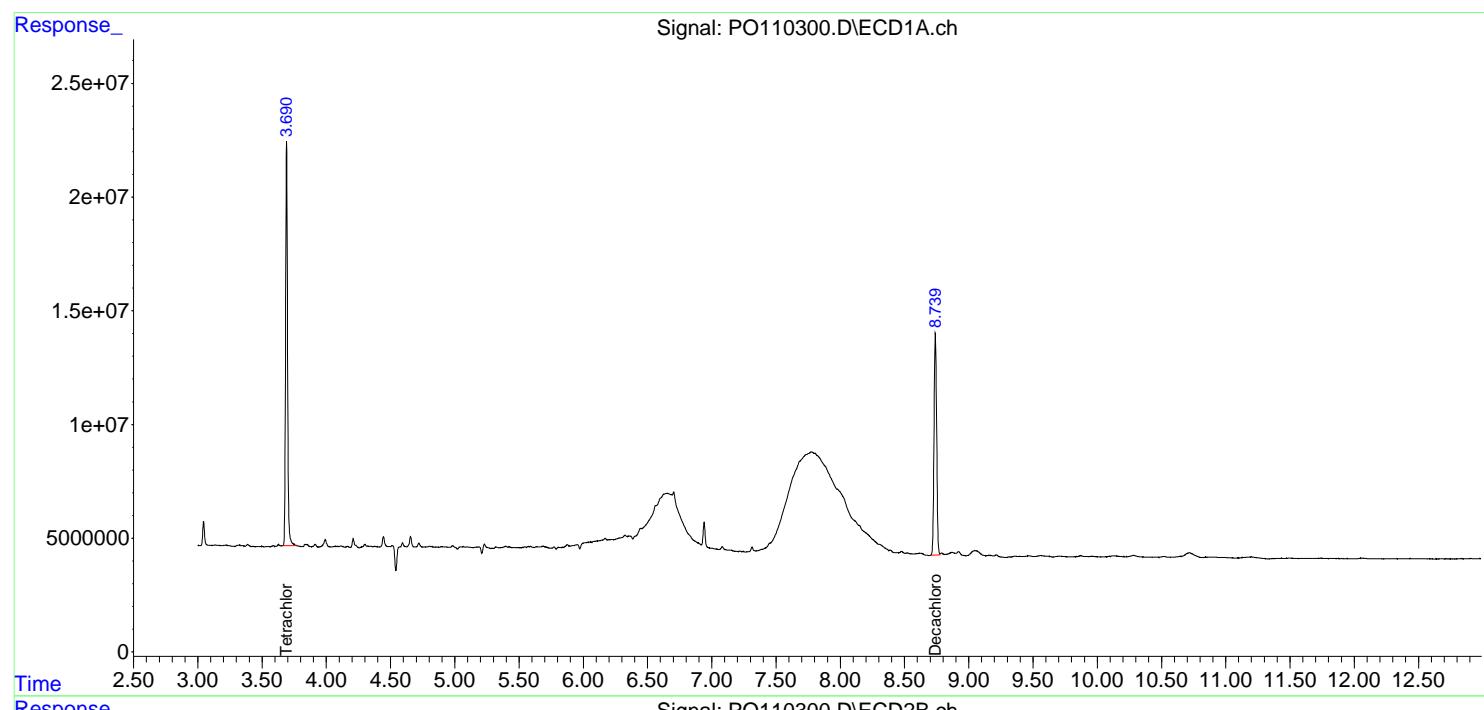

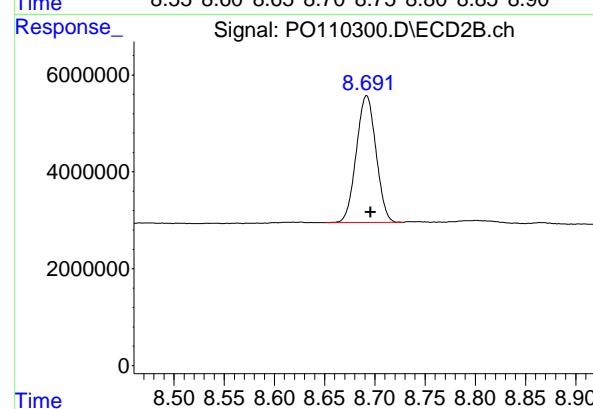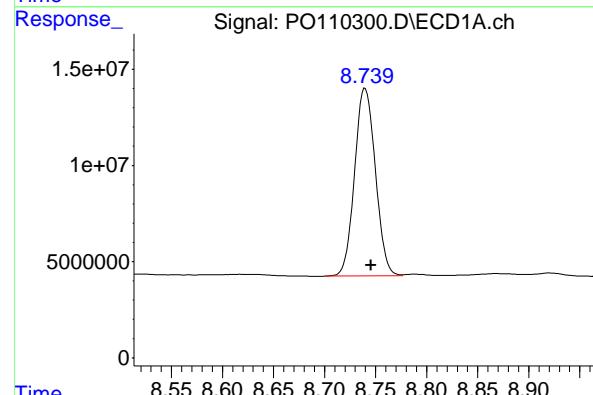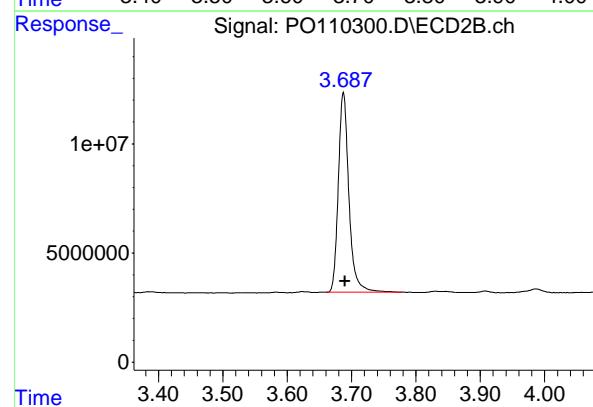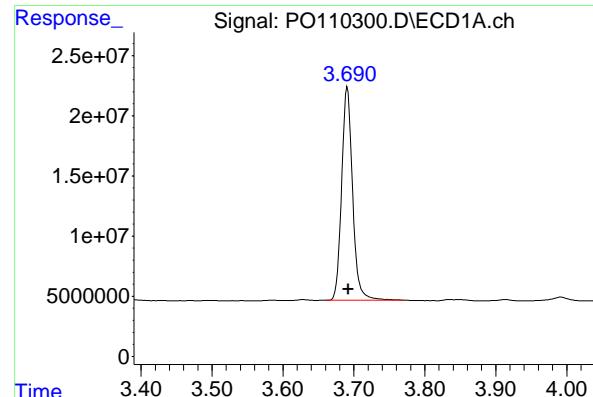

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: -0.001 min  
 Response: 189761354 ECD\_O  
 Conc: 20.85 ng/ml ClientSampleId : OU4-PCS-TC-23-040325

## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
 Delta R.T.: -0.002 min  
 Response: 104320886  
 Conc: 19.89 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.740 min  
 Delta R.T.: -0.006 min  
 Response: 138303216  
 Conc: 17.99 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.692 min  
 Delta R.T.: -0.004 min  
 Response: 35798912  
 Conc: 14.76 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-PCS-TC-24-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-13			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	91.3	Decanted:
Sample Wt/Vol:	30.08	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110301.D	1	04/07/25 08:20	04/08/25 11:53	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	9.10	U	4.30	9.10	18.6	ug/kg
11104-28-2	Aroclor-1221	14.2	U	4.40	14.2	18.6	ug/kg
11141-16-5	Aroclor-1232	9.10	U	4.10	9.10	18.6	ug/kg
53469-21-9	Aroclor-1242	9.10	U	4.40	9.10	18.6	ug/kg
12672-29-6	Aroclor-1248	14.2	U	6.50	14.2	18.6	ug/kg
11097-69-1	Aroclor-1254	9.10	U	3.50	9.10	18.6	ug/kg
37324-23-5	Aroclor-1262	14.2	U	5.50	14.2	18.6	ug/kg
11100-14-4	Aroclor-1268	9.10	U	3.90	9.10	18.6	ug/kg
11096-82-5	Aroclor-1260	9.10	U	3.50	9.10	18.6	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	20.5		44 - 130		102%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.9		60 - 125		94%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110301.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:53  
 Operator : YP/AJ  
 Sample : Q1730-13  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
OU4-PCS-TC-24-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 12:09:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	3.690	3.687	186.4E6	101.7E6	20.482	19.389
2) SA Decachloro...	8.741	8.691	145.2E6	37966376	18.886	15.649

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110301.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:53  
 Operator : YP/AJ  
 Sample : Q1730-13  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-PCS-TC-24-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 12:09:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

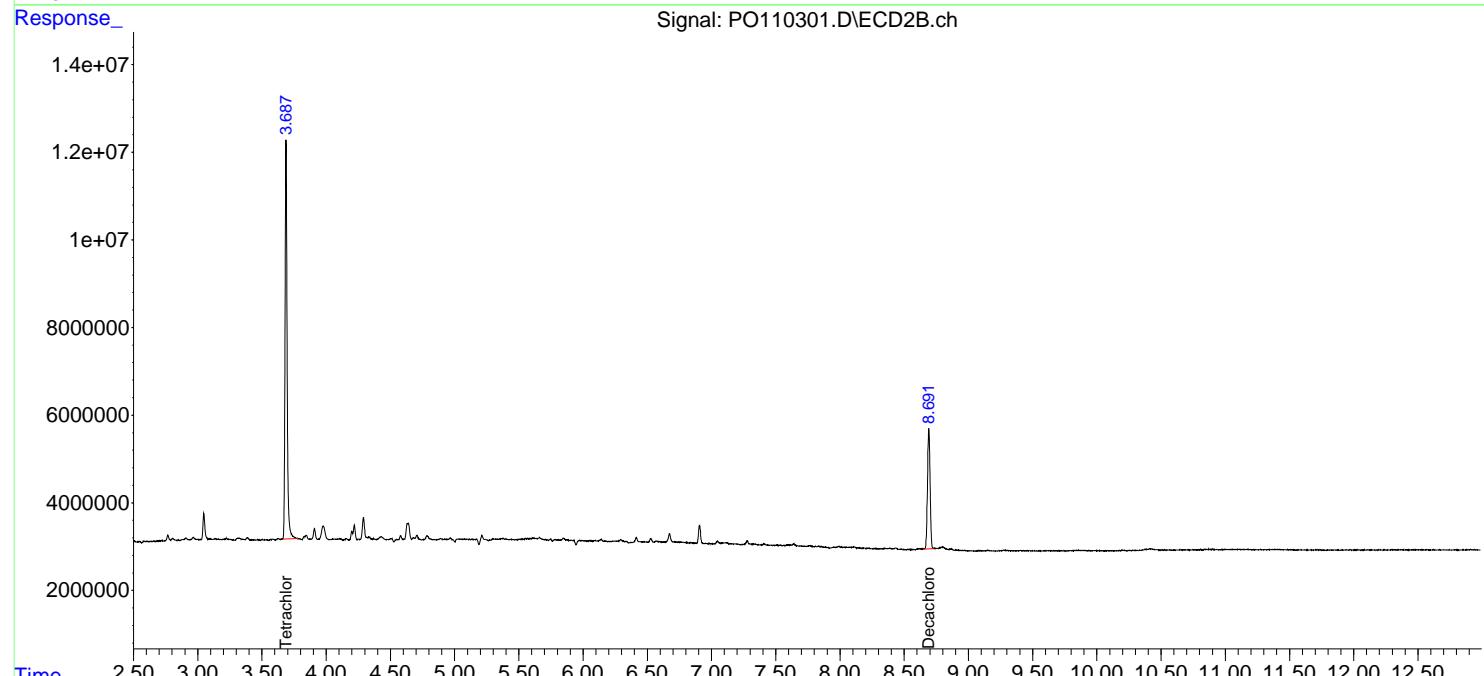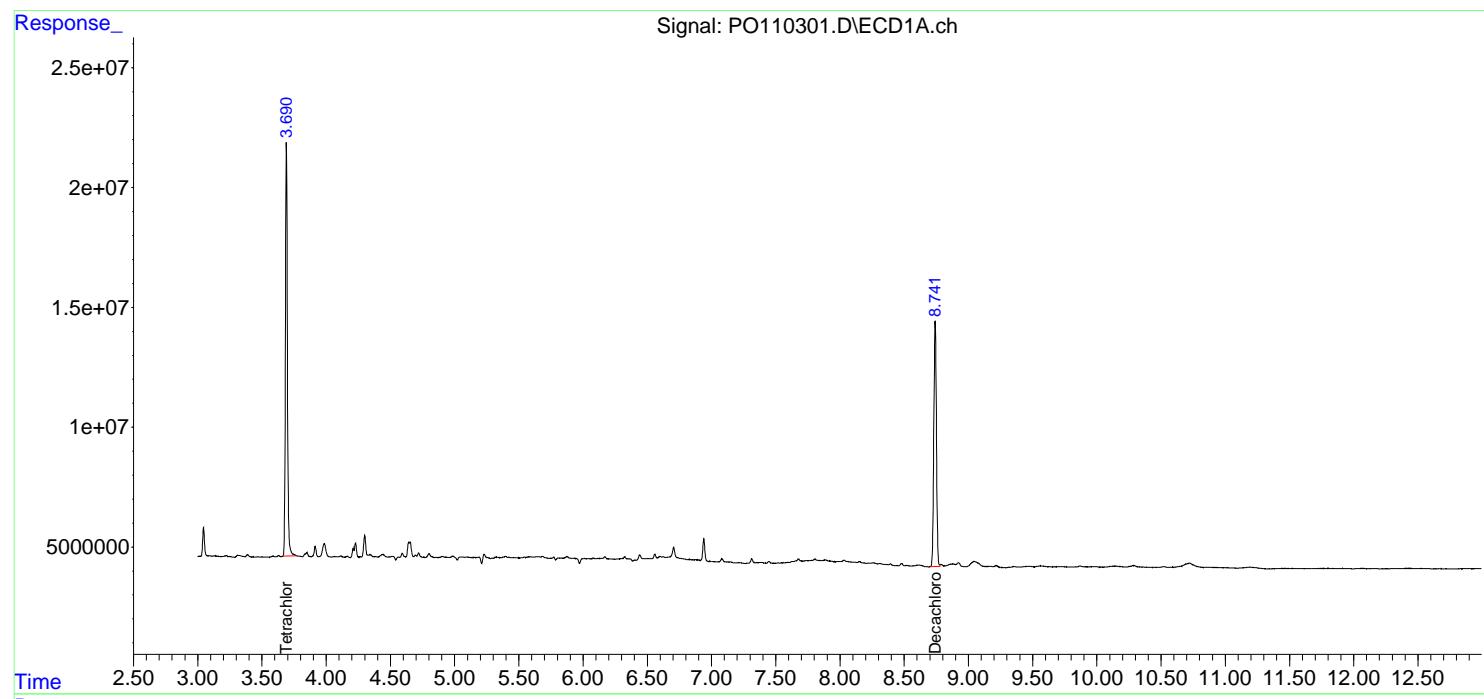

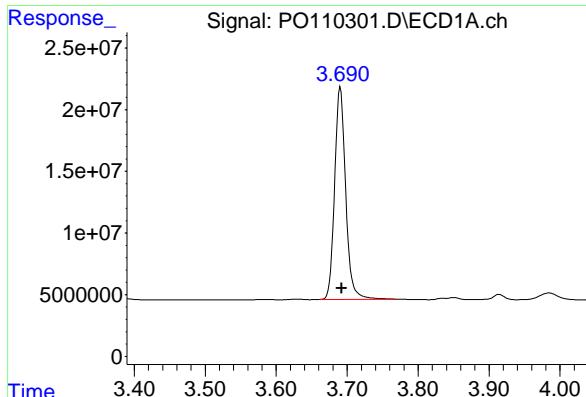


## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
Delta R.T.: -0.002 min  
Instrument: ECD\_O  
Response: 186415453  
Conc: 20.48 ng/ml  
ClientSampleId: OU4-PCS-TC-24-040325

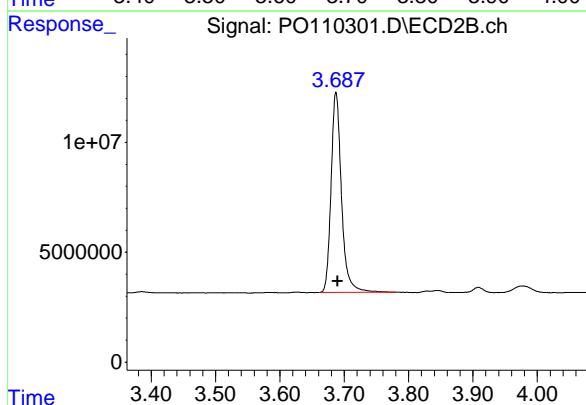


## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
Delta R.T.: -0.002 min  
Instrument: ECD\_O  
Response: 101677050  
Conc: 19.39 ng/ml

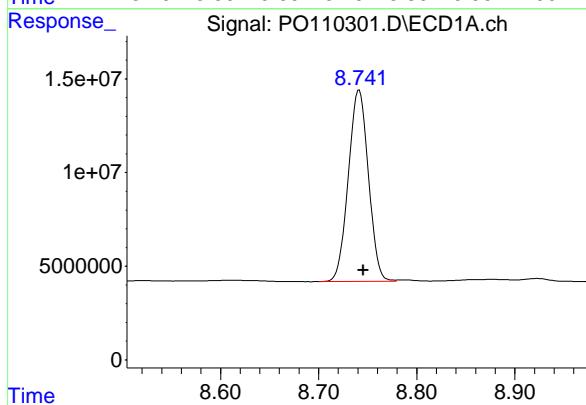

## #2 Decachlorobiphenyl

R.T.: 8.741 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_O  
Response: 145207235  
Conc: 18.89 ng/ml

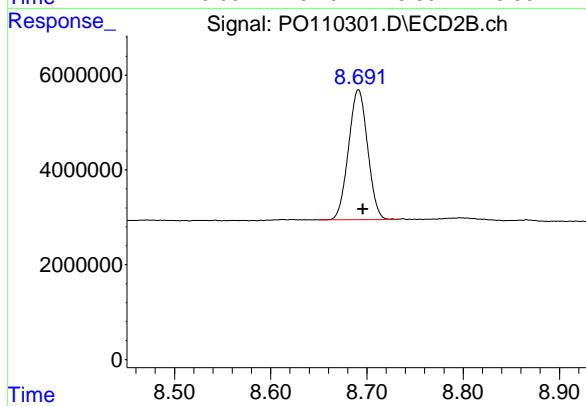

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
Delta R.T.: -0.005 min  
Instrument: ECD\_O  
Response: 37966376  
Conc: 15.65 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	04/03/25	
Project:	Raymark Superfund Site		Date Received:	04/04/25	
Client Sample ID:	OU4-PCS-TC-25-040325		SDG No.:	Q1730	
Lab Sample ID:	Q1730-15		Matrix:	SOIL	
Analytical Method:	SW8082A		% Solid:	92.5	Decanted:
Sample Wt/Vol:	30.06	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP071142.D	1	04/07/25 08:20	04/08/25 11:39	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	9.00	U	4.30	9.00	18.3	ug/kg
11104-28-2	Aroclor-1221	14.0	U	4.30	14.0	18.3	ug/kg
11141-16-5	Aroclor-1232	9.00	U	4.00	9.00	18.3	ug/kg
53469-21-9	Aroclor-1242	9.00	U	4.30	9.00	18.3	ug/kg
12672-29-6	Aroclor-1248	14.0	U	6.40	14.0	18.3	ug/kg
11097-69-1	Aroclor-1254	9.00	U	3.50	9.00	18.3	ug/kg
37324-23-5	Aroclor-1262	14.0	U	5.40	14.0	18.3	ug/kg
11100-14-4	Aroclor-1268	9.00	U	3.90	9.00	18.3	ug/kg
11096-82-5	Aroclor-1260	9.00	U	3.50	9.00	18.3	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	24.8		44 - 130		124%	SPK: 20
2051-24-3	Decachlorobiphenyl	23.3		60 - 125		116%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071142.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:39  
 Operator : YP\AJ  
 Sample : Q1730-15  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**OU4-PCS-TC-25-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 12:00:55 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	4.514	3.815	36065391	25688268	24.676	24.780
2) SA Decachloro...	10.242	8.859	24468736	16145301	23.246	20.484

#### Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071142.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:39  
 Operator : YP\AJ  
 Sample : Q1730-15  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 OU4-PCS-TC-25-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 12:00:55 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

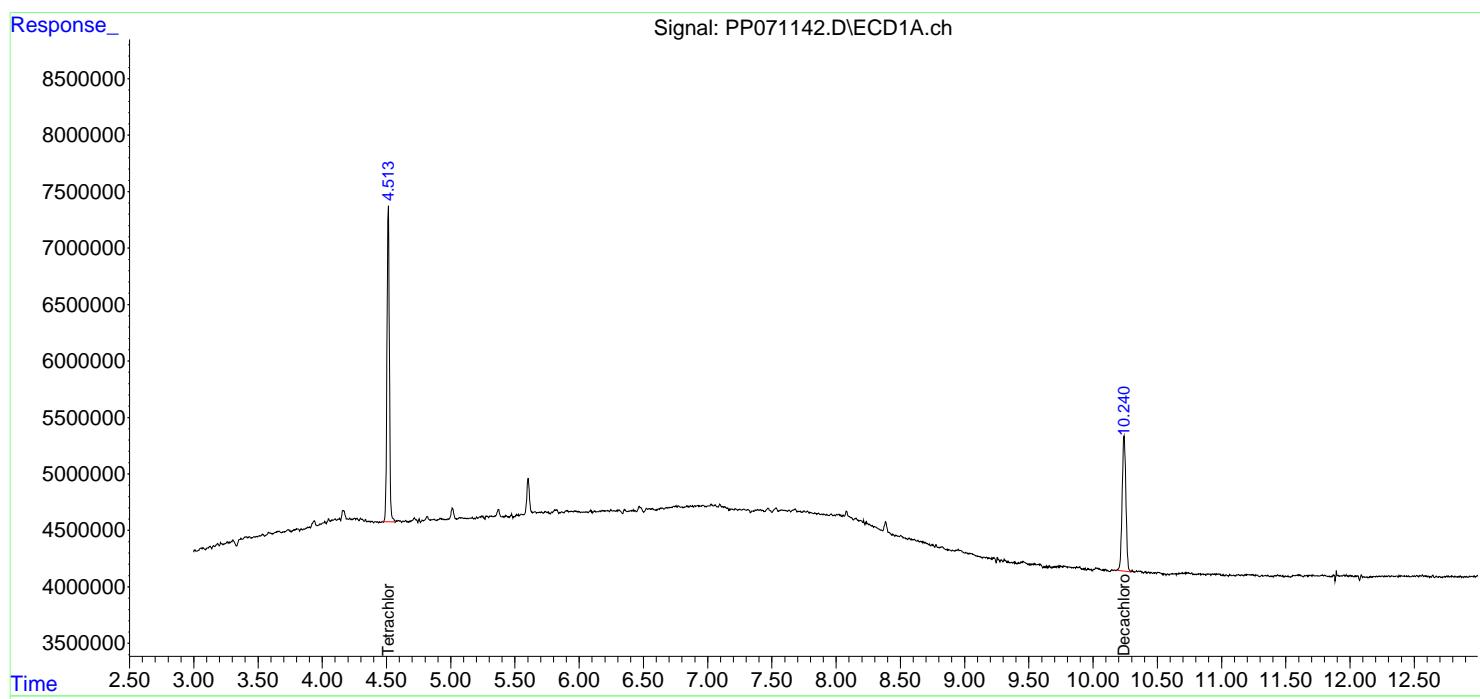

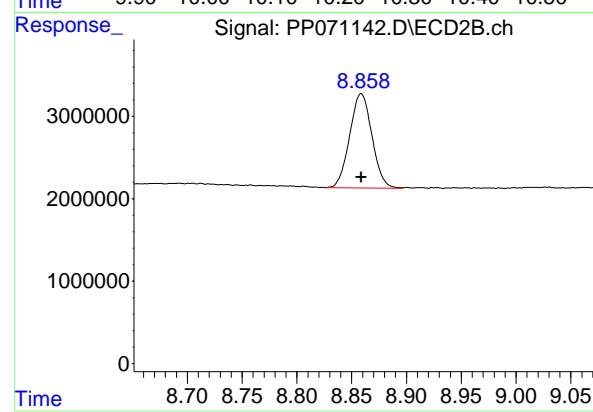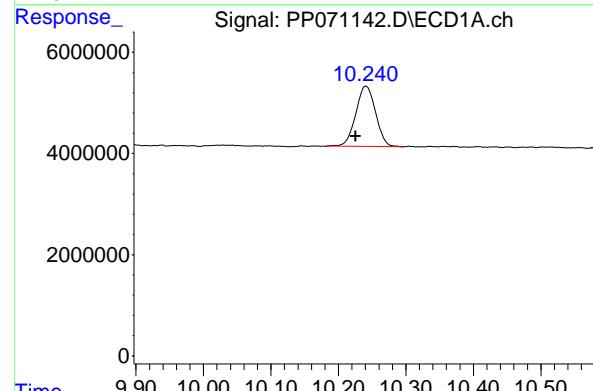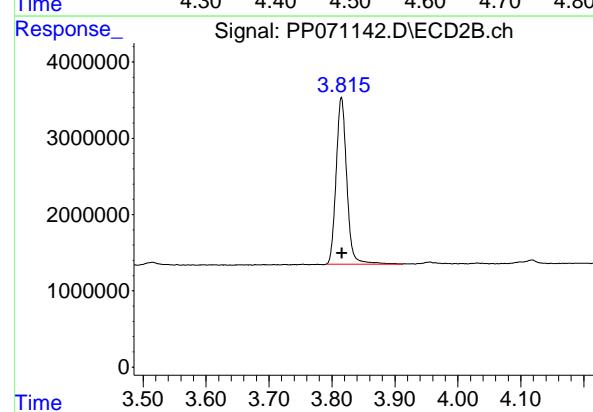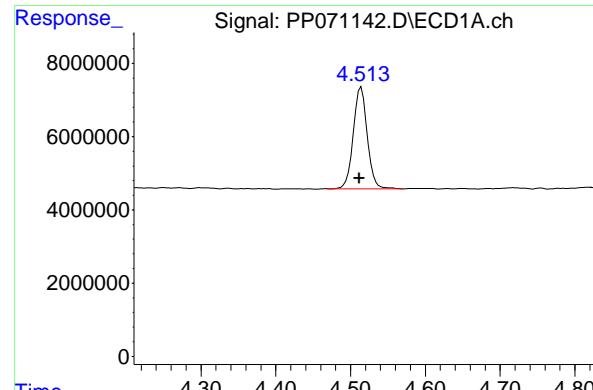

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
 Delta R.T.: 0.002 min  
 Response: 36065391 ECD\_P  
 Conc: 24.68 ng/ml ClientSampleId : OU4-PCS-TC-25-040325

## #1 Tetrachloro-m-xylene

R.T.: 3.815 min  
 Delta R.T.: 0.000 min  
 Response: 25688268  
 Conc: 24.78 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.242 min  
 Delta R.T.: 0.016 min  
 Response: 24468736  
 Conc: 23.25 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 16145301  
 Conc: 20.48 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-PCS-TC-26-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-17			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	92.1	Decanted:
Sample Wt/Vol:	30.03	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP071143.D	1	04/07/25 08:20	04/08/25 11:56	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	9.00	U	4.30	9.00	18.4	ug/kg
11104-28-2	Aroclor-1221	14.1	U	4.40	14.1	18.4	ug/kg
11141-16-5	Aroclor-1232	9.00	U	4.00	9.00	18.4	ug/kg
53469-21-9	Aroclor-1242	9.00	U	4.30	9.00	18.4	ug/kg
12672-29-6	Aroclor-1248	14.1	U	6.40	14.1	18.4	ug/kg
11097-69-1	Aroclor-1254	9.00	U	3.50	9.00	18.4	ug/kg
37324-23-5	Aroclor-1262	14.1	U	5.40	14.1	18.4	ug/kg
11100-14-4	Aroclor-1268	9.00	U	3.90	9.00	18.4	ug/kg
11096-82-5	Aroclor-1260	9.00	U	3.50	9.00	18.4	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	25.1		44 - 130		125%	SPK: 20
2051-24-3	Decachlorobiphenyl	24.9		60 - 125		124%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071143.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:56  
 Operator : YP\AJ  
 Sample : Q1730-17  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**OU4-PCS-TC-26-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 12:13:50 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	4.518	3.815	36660054	25694077	25.083	24.786
2) SA Decachloro...	10.246	8.859	26192698	17327330	24.883	21.984

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071143.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:56  
 Operator : YP\AJ  
 Sample : Q1730-17  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**OU4-PCS-TC-26-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 12:13:50 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

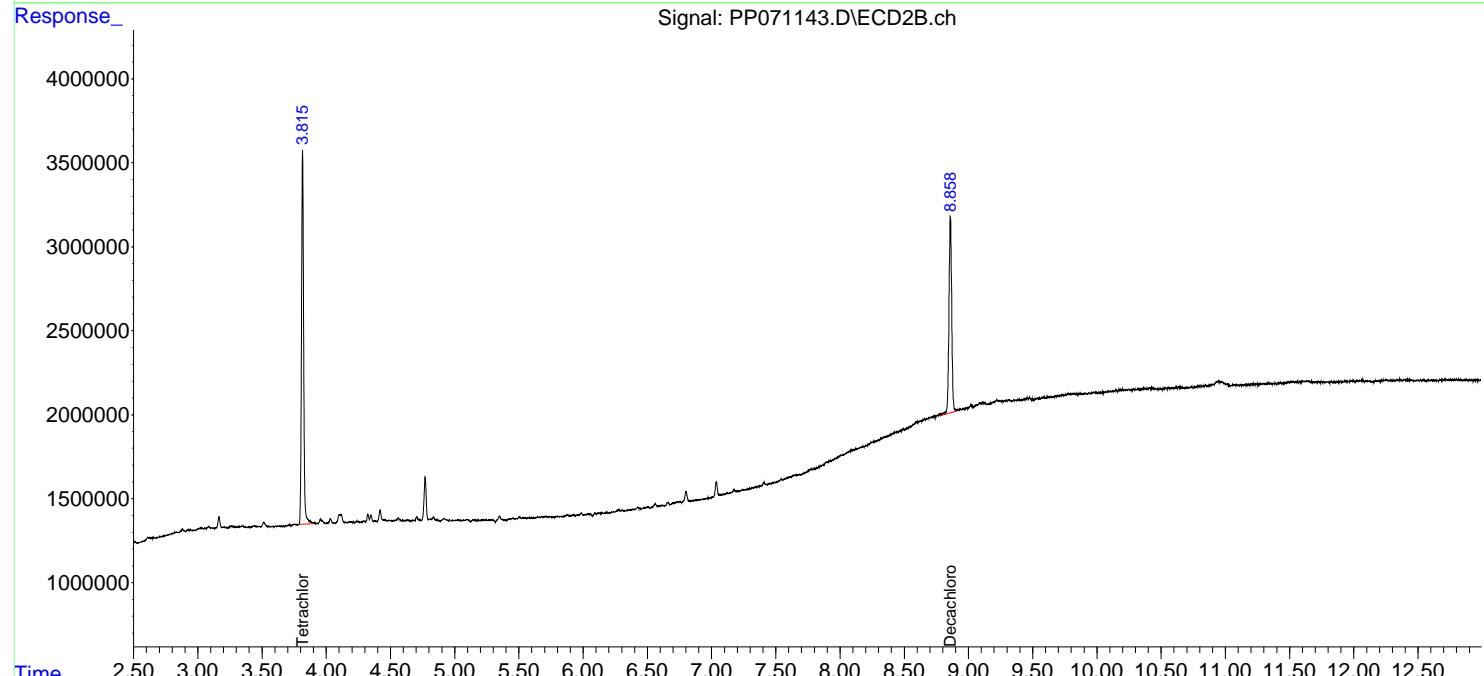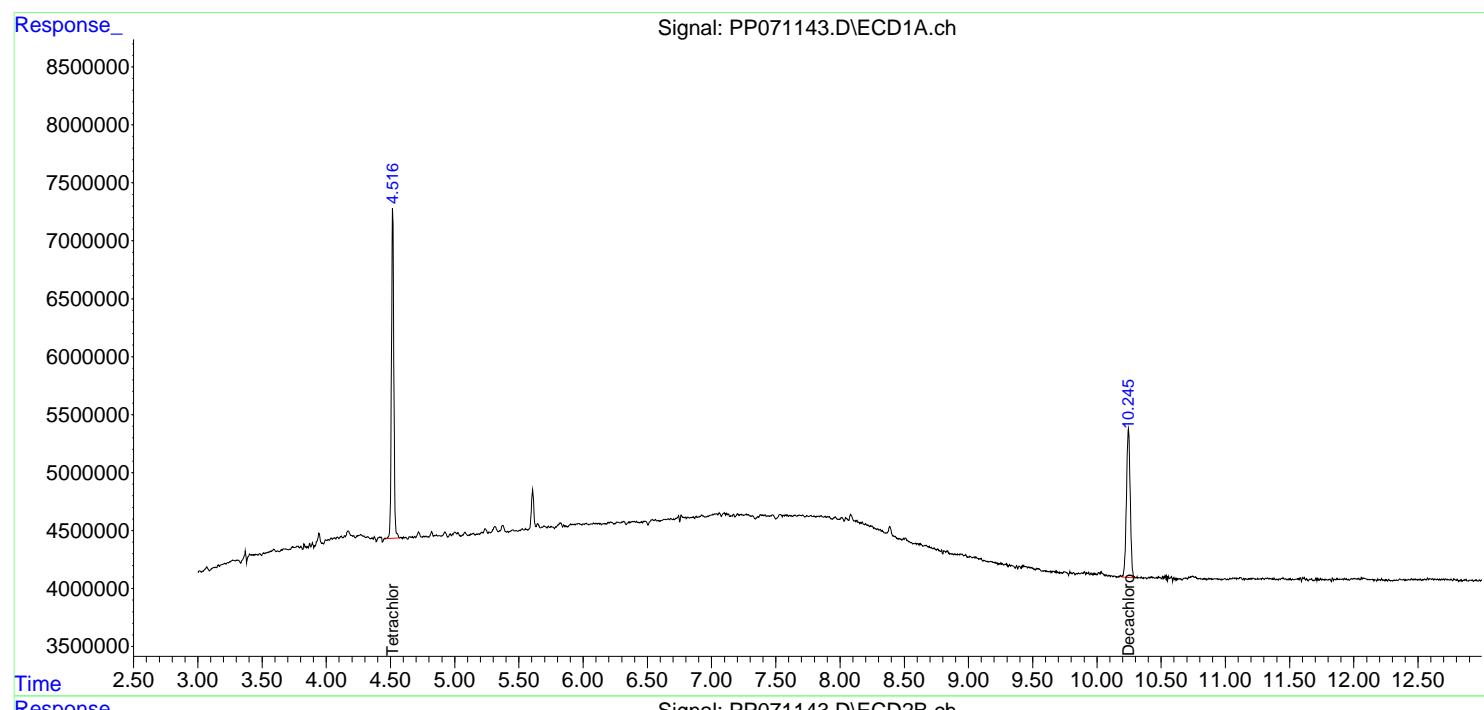

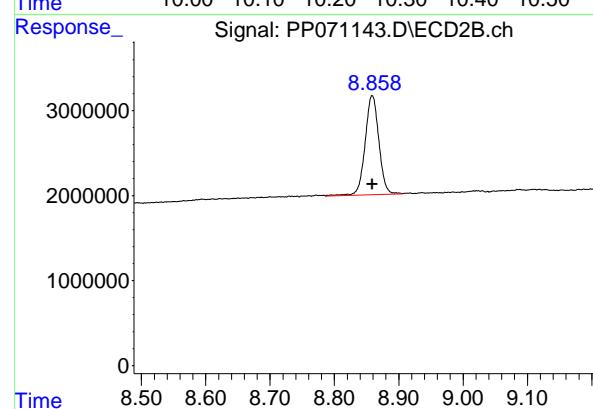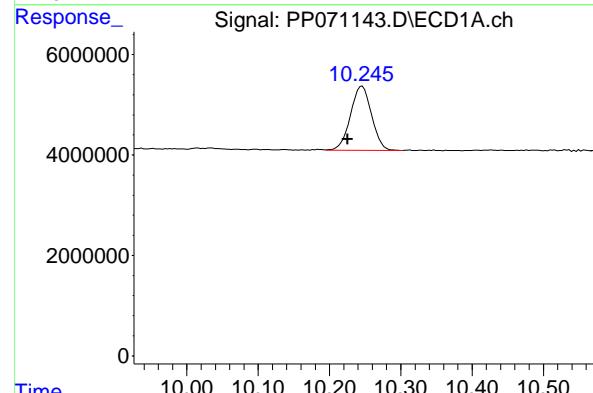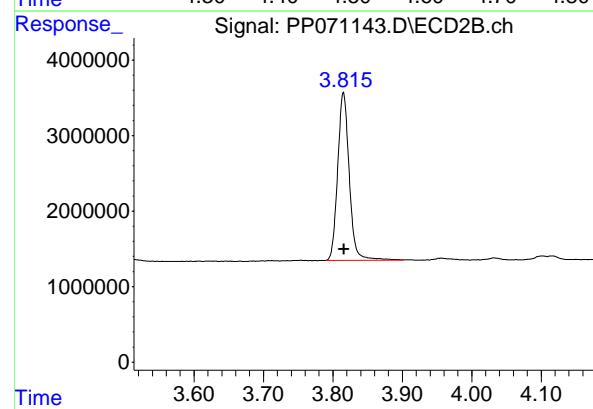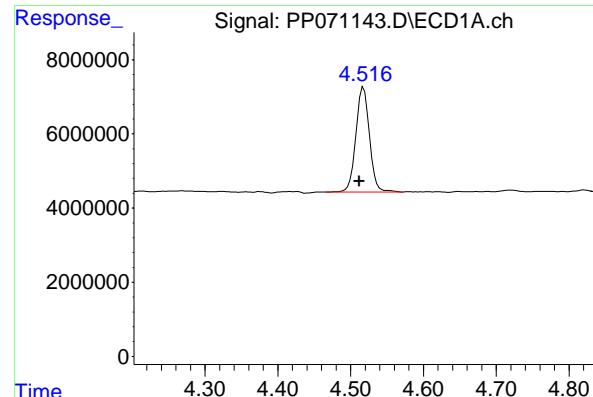

## #1 Tetrachloro-m-xylene

R.T.: 4.518 min  
Delta R.T.: 0.006 min  
Instrument: ECD\_P  
Response: 36660054  
Conc: 25.08 ng/ml  
ClientSampleId : OU4-PCS-TC-26-040325

## #1 Tetrachloro-m-xylene

R.T.: 3.815 min  
Delta R.T.: 0.000 min  
Response: 25694077  
Conc: 24.79 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.246 min  
Delta R.T.: 0.021 min  
Response: 26192698  
Conc: 24.88 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 17327330  
Conc: 21.98 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-CF-15-040325			SDG No.:	Q1730	
Lab Sample ID:	Q1730-19			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	93.9	Decanted:
Sample Wt/Vol:	30.02	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP071144.D	1	04/07/25 08:20	04/08/25 12:12	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	8.80	U	4.20	8.80	18.1	ug/kg
11104-28-2	Aroclor-1221	13.8	U	4.30	13.8	18.1	ug/kg
11141-16-5	Aroclor-1232	8.80	U	4.00	8.80	18.1	ug/kg
53469-21-9	Aroclor-1242	8.80	U	4.30	8.80	18.1	ug/kg
12672-29-6	Aroclor-1248	13.8	U	6.30	13.8	18.1	ug/kg
11097-69-1	Aroclor-1254	8.80	U	3.40	8.80	18.1	ug/kg
37324-23-5	Aroclor-1262	13.8	U	5.30	13.8	18.1	ug/kg
11100-14-4	Aroclor-1268	8.80	U	3.80	8.80	18.1	ug/kg
11096-82-5	Aroclor-1260	8.80	U	3.40	8.80	18.1	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	27.5	*	44 - 130		138%	SPK: 20
2051-24-3	Decachlorobiphenyl	24.1		60 - 125		121%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071144.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 12:12  
 Operator : YP\AJ  
 Sample : Q1730-19  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**OU4-CF-15-040325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 12:26:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	4.516	3.815	37706422	28536768	25.798	27.528
2) SA Decachloro...	10.242	8.859	25401796	17071245	24.132	21.659

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071144.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 12:12  
 Operator : YP\AJ  
 Sample : Q1730-19  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument:**  
ECD\_P  
**ClientSampleId :**  
OU4-CF-15-040325

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 12:26:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

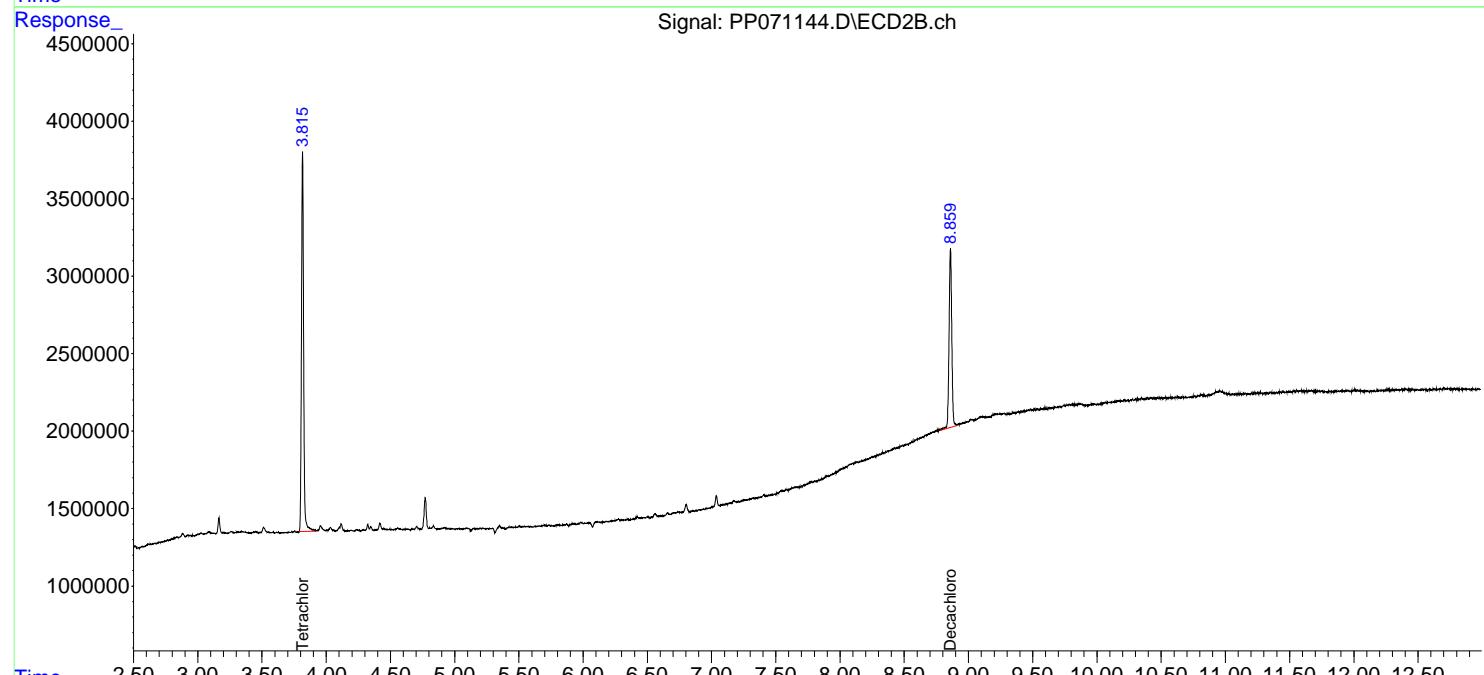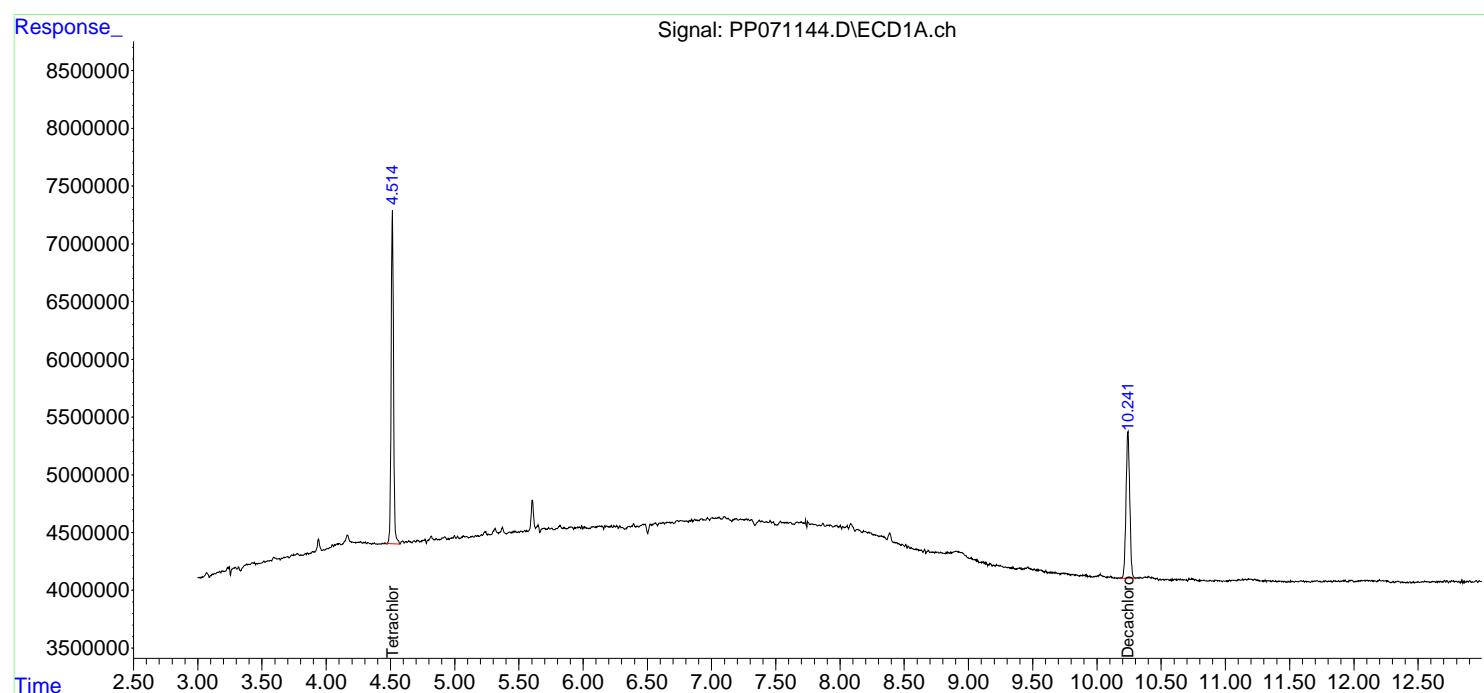

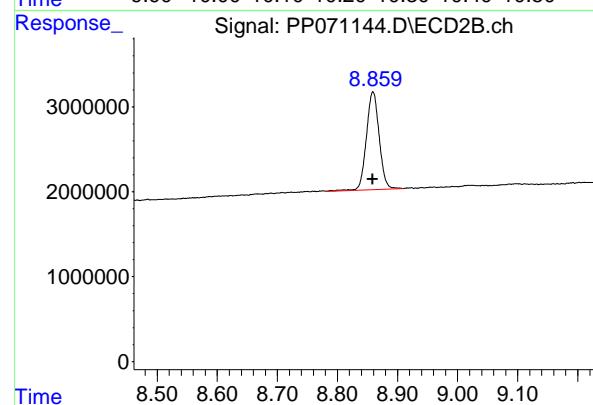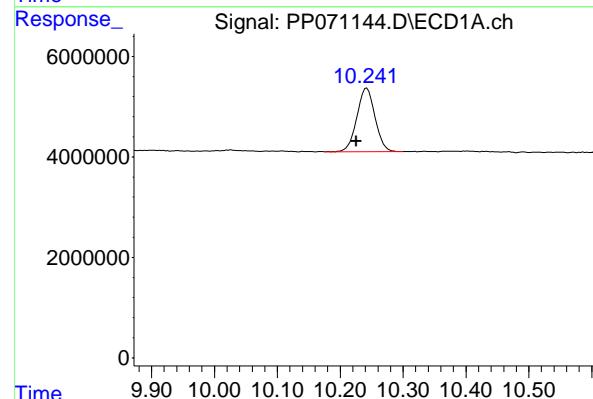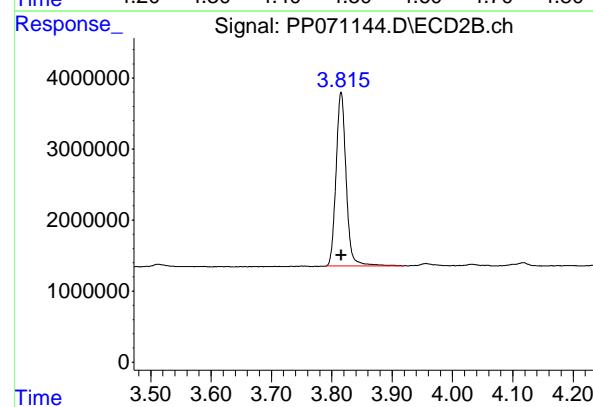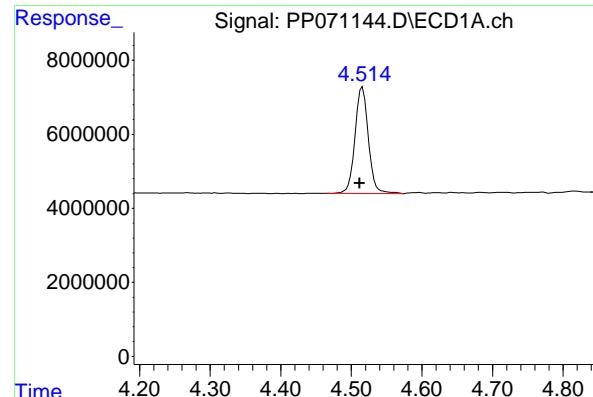

## #1 Tetrachloro-m-xylene

R.T.: 4.516 min  
 Delta R.T.: 0.004 min  
 Response: 37706422 ECD\_P  
 Conc: 25.80 ng/ml ClientSampleId : OU4-CF-15-040325

## #1 Tetrachloro-m-xylene

R.T.: 3.815 min  
 Delta R.T.: 0.000 min  
 Response: 28536768  
 Conc: 27.53 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.242 min  
 Delta R.T.: 0.017 min  
 Response: 25401796  
 Conc: 24.13 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 17071245  
 Conc: 21.66 ng/ml



# CALIBRATION

# SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>NOBI03</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1730</u>	SAS No.:	<u>Q1730</u>	SDG NO.:	<u>Q1730</u>
Instrument ID:	<u>ECD_O</u>	Calibration Date(s):		<u>03/18/2025</u>		<u>03/18/2025</u>	
		Calibration Times:		<u>14:03</u>		<u>22:15</u>	

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	<u>PO109972.D</u>	RT 750 =	<u>PO109973.D</u>
	RT 500 =	<u>PO109974.D</u>	RT 250 =	<u>PO109975.D</u>
			RT 050 =	<u>PO109976.D</u>

COMPOUND	RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW FROM	TO
Aroclor-1016-1 (1)	4.79	4.79	4.79	4.79	4.78	4.79	4.69	4.89
Aroclor-1016-2 (2)	4.81	4.81	4.80	4.80	4.80	4.80	4.70	4.90
Aroclor-1016-3 (3)	4.86	4.86	4.86	4.86	4.86	4.86	4.76	4.96
Aroclor-1016-4 (4)	4.98	4.98	4.98	4.98	4.98	4.98	4.88	5.08
Aroclor-1016-5 (5)	5.24	5.24	5.24	5.24	5.24	5.24	5.14	5.34
Aroclor-1260-1 (1)	6.28	6.28	6.28	6.28	6.28	6.28	6.18	6.38
Aroclor-1260-2 (2)	6.47	6.47	6.47	6.47	6.47	6.47	6.37	6.57
Aroclor-1260-3 (3)	6.84	6.84	6.84	6.84	6.84	6.84	6.74	6.94
Aroclor-1260-4 (4)	7.10	7.10	7.10	7.10	7.10	7.10	7.00	7.20
Aroclor-1260-5 (5)	7.34	7.34	7.34	7.34	7.34	7.34	7.24	7.44
Decachlorobiphenyl	8.75	8.75	8.75	8.75	8.74	8.75	8.65	8.85
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79
Aroclor-1242-1 (1)	4.79	4.79	4.79	4.79	4.78	4.79	4.69	4.89
Aroclor-1242-2 (2)	4.80	4.80	4.81	4.80	4.80	4.80	4.70	4.90
Aroclor-1242-3 (3)	4.86	4.86	4.86	4.86	4.86	4.86	4.76	4.96
Aroclor-1242-4 (4)	4.98	4.98	4.98	4.98	4.98	4.98	4.88	5.08
Aroclor-1242-5 (5)	5.64	5.63	5.64	5.63	5.63	5.63	5.53	5.73
Decachlorobiphenyl	8.74	8.74	8.74	8.74	8.74	8.74	8.64	8.84
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79
Aroclor-1248-1 (1)	4.78	4.79	4.79	4.78	4.78	4.78	4.68	4.88
Aroclor-1248-2 (2)	5.02	5.02	5.02	5.02	5.02	5.02	4.92	5.12
Aroclor-1248-3 (3)	5.24	5.24	5.24	5.24	5.24	5.24	5.14	5.34
Aroclor-1248-4 (4)	5.59	5.59	5.59	5.59	5.59	5.59	5.49	5.69
Aroclor-1248-5 (5)	5.63	5.64	5.63	5.63	5.63	5.63	5.53	5.73
Decachlorobiphenyl	8.74	8.74	8.74	8.74	8.74	8.74	8.64	8.84
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79
Aroclor-1254-1 (1)	5.59	5.59	5.59	5.59	5.59	5.59	5.49	5.69
Aroclor-1254-2 (2)	5.74	5.74	5.74	5.74	5.74	5.74	5.64	5.84
Aroclor-1254-3 (3)	6.15	6.15	6.15	6.15	6.15	6.15	6.05	6.25
Aroclor-1254-4 (4)	6.38	6.38	6.38	6.38	6.38	6.38	6.28	6.48
Aroclor-1254-5 (5)	6.80	6.80	6.80	6.80	6.80	6.80	6.70	6.90
Decachlorobiphenyl	8.74	8.74	8.74	8.74	8.74	8.74	8.64	8.84
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79
Aroclor-1268-1 (1)	7.62	7.62	7.62	7.62	7.62	7.62	7.52	7.72
Aroclor-1268-2 (2)	7.69	7.69	7.69	7.69	7.69	7.69	7.59	7.79
Aroclor-1268-3 (3)	7.90	7.90	7.90	7.90	7.90	7.90	7.80	8.00
Aroclor-1268-4 (4)	8.18	8.18	8.19	8.18	8.18	8.18	8.08	8.28
Aroclor-1268-5 (5)	8.48	8.48	8.48	8.48	8.48	8.48	8.38	8.58



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

#### RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	8.74	8.74	8.74	8.74	8.74	8.74	8.64	8.84	1
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79	2

3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>NOBI03</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1730</u>	SAS No.:	<u>Q1730</u>	SDG NO.:	<u>Q1730</u>
Instrument ID:	<u>ECD_O</u>	Calibration Date(s):		<u>03/18/2025</u>		<u>03/18/2025</u>	
		Calibration Times:		<u>14:03</u>		<u>22:15</u>	

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	<u>PO109972.D</u>	RT 750 =	<u>PO109973.D</u>
	RT 500 =	<u>PO109974.D</u>	RT 250 =	<u>PO109975.D</u>
			RT 050 =	<u>PO109976.D</u>

COMPOUND	RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW FROM	TO
Aroclor-1016-1 (1)	4.77	4.77	4.77	4.77	4.77	4.77	4.67	4.87
Aroclor-1016-2 (2)	4.79	4.79	4.79	4.79	4.79	4.79	4.69	4.89
Aroclor-1016-3 (3)	4.97	4.97	4.97	4.97	4.97	4.97	4.87	5.07
Aroclor-1016-4 (4)	5.01	5.01	5.01	5.01	5.01	5.01	4.91	5.11
Aroclor-1016-5 (5)	5.22	5.22	5.22	5.22	5.22	5.22	5.12	5.32
Aroclor-1260-1 (1)	6.25	6.26	6.26	6.25	6.25	6.25	6.15	6.35
Aroclor-1260-2 (2)	6.44	6.44	6.44	6.44	6.44	6.44	6.34	6.54
Aroclor-1260-3 (3)	6.60	6.60	6.60	6.59	6.59	6.59	6.49	6.69
Aroclor-1260-4 (4)	7.07	7.07	7.07	7.07	7.07	7.07	6.97	7.17
Aroclor-1260-5 (5)	7.31	7.31	7.31	7.31	7.31	7.31	7.21	7.41
Decachlorobiphenyl	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79
Aroclor-1242-1 (1)	4.77	4.77	4.77	4.77	4.77	4.77	4.67	4.87
Aroclor-1242-2 (2)	4.79	4.79	4.79	4.79	4.79	4.79	4.69	4.89
Aroclor-1242-3 (3)	4.97	4.97	4.97	4.97	4.97	4.97	4.87	5.07
Aroclor-1242-4 (4)	5.05	5.05	5.05	5.05	5.05	5.05	4.95	5.15
Aroclor-1242-5 (5)	5.57	5.57	5.57	5.57	5.57	5.57	5.47	5.67
Decachlorobiphenyl	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79
Aroclor-1248-1 (1)	4.77	4.77	4.77	4.77	4.77	4.77	4.67	4.87
Aroclor-1248-2 (2)	5.01	5.01	5.01	5.01	5.01	5.01	4.91	5.11
Aroclor-1248-3 (3)	5.05	5.05	5.05	5.05	5.05	5.05	4.95	5.15
Aroclor-1248-4 (4)	5.22	5.22	5.22	5.22	5.22	5.22	5.12	5.32
Aroclor-1248-5 (5)	5.61	5.61	5.61	5.61	5.61	5.61	5.51	5.71
Decachlorobiphenyl	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79
Aroclor-1254-1 (1)	5.57	5.57	5.57	5.57	5.57	5.57	5.47	5.67
Aroclor-1254-2 (2)	5.72	5.72	5.72	5.72	5.72	5.72	5.62	5.82
Aroclor-1254-3 (3)	6.12	6.12	6.12	6.12	6.12	6.12	6.02	6.22
Aroclor-1254-4 (4)	6.35	6.35	6.35	6.35	6.35	6.35	6.25	6.45
Aroclor-1254-5 (5)	6.77	6.77	6.77	6.77	6.77	6.77	6.67	6.87
Decachlorobiphenyl	8.69	8.70	8.70	8.70	8.69	8.70	8.60	8.80
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79
Aroclor-1268-1 (1)	7.59	7.59	7.59	7.59	7.59	7.59	7.49	7.69
Aroclor-1268-2 (2)	7.66	7.66	7.65	7.65	7.65	7.65	7.55	7.75
Aroclor-1268-3 (3)	7.86	7.86	7.86	7.86	7.86	7.86	7.76	7.96
Aroclor-1268-4 (4)	8.15	8.15	8.15	8.15	8.15	8.15	8.05	8.25
Aroclor-1268-5 (5)	8.44	8.44	8.44	8.44	8.44	8.44	8.34	8.54



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

#### RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	8.70	8.70	8.69	8.70	8.70	8.70	8.60	8.80	1
Tetrachloro-m-xylene	3.69	3.69	3.69	3.69	3.69	3.69	3.59	3.79	2

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract:	<b>NOBI03</b>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1730</u>	SAS No.:	<u>Q1730</u>	SDG NO.:	<u>Q1730</u>
Instrument ID:	<u>ECD_O</u>	Calibration Date(s):				<u>03/18/2025</u>	<u>03/18/2025</u>
		Calibration Times:				<u>14:03</u>	<u>22:15</u>
GC Column:	<u>ZB-MR1</u>	ID:	<u>0.32</u> (mm)				

LAB FILE ID:	CF 1000 =	CF 750 =	CF 500 =
	CF 500 =	CF 250 =	CF 050 =
	<u>PO109972.D</u>	<u>PO109973.D</u>	<u>PO109976.D</u>
	<u>PO109974.D</u>	<u>PO109975.D</u>	<u>PO109976.D</u>
COMPOUND	CF 1000	CF 750	CF 500
Aroclor-1016-1 (1)	318793340	329109113	342176988
Aroclor-1016-2 (2)	446388679	463709840	475172436
Aroclor-1016-3 (3)	297123739	311570976	324283686
Aroclor-1016-4 (4)	237983440	248526219	257445742
Aroclor-1016-5 (5)	250501585	263674729	272727188
Aroclor-1260-1 (1)	448474074	467586512	475904282
Aroclor-1260-2 (2)	549756400	573035712	574538170
Aroclor-1260-3 (3)	466244522	483474499	486507370
Aroclor-1260-4 (4)	395577993	413728377	429812132
Aroclor-1260-5 (5)	1037246832	1067855560	1076605366
Decachlorobiphenyl	7314268770	7585202853	7715836840
Tetrachloro-m-xylene	9191618080	9409704013	9556350980
Aroclor-1242-1 (1)	257021206	271242037	274350776
Aroclor-1242-2 (2)	361656206	376061644	380771426
Aroclor-1242-3 (3)	239272274	256595597	260500336
Aroclor-1242-4 (4)	191269111	202702439	206227546
Aroclor-1242-5 (5)	200342595	212233400	219728410
Decachlorobiphenyl	7073021470	7288055093	7382383840
Tetrachloro-m-xylene	8702773030	8995385800	8954862760
Aroclor-1248-1 (1)	203222777	210833551	219941524
Aroclor-1248-2 (2)	271717932	285234192	301067598
Aroclor-1248-3 (3)	341855080	357243465	374409124
Aroclor-1248-4 (4)	484718685	503724613	523274664
Aroclor-1248-5 (5)	341874536	354831647	369725290
Decachlorobiphenyl	7279802030	7532134600	7794766540
Tetrachloro-m-xylene	8896906280	9107530813	9275989780
Aroclor-1254-1 (1)	527461301	541865743	559314886
Aroclor-1254-2 (2)	454907170	469007857	483702014
Aroclor-1254-3 (3)	753626169	772675721	789277352
Aroclor-1254-4 (4)	465418236	477798716	486446390
Aroclor-1254-5 (5)	652046620	666447925	680525202
Decachlorobiphenyl	7506577390	7722603000	7867257780
Tetrachloro-m-xylene	9124017490	9264222013	9387241720
Aroclor-1268-1 (1)	1369838059	1374439380	1401378006



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

#### CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	1266296617	1262736967	1279632688	1321583800	1270503560	1280150726	2
Aroclor-1268-3	(3)	1019701747	1019547960	1038648586	1056461448	1003450380	1027562024	2
Aroclor-1268-4	(4)	432675859	421354135	447439086	473337560	435173000	441995928	4
Aroclor-1268-5	(5)	3202130253	3192211076	3228608174	3247761892	3036317900	3181405859	3
Decachlorobiphenyl		13640006290	13735597093	14120230440	14566780400	14594697800	14131462405	3
Tetrachloro-m-xylene		9016621250	8994153573	9277514520	9319153840	8874982800	9096485197	2

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract:	<b>NOBI03</b>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1730</u>	SAS No.:	<u>Q1730</u>	SDG NO.:	<u>Q1730</u>
Instrument ID:	<u>ECD_O</u>				Calibration Date(s):	<u>03/18/2025</u>	<u>03/18/2025</u>
					Calibration Times:	<u>14:03</u>	<u>22:15</u>
GC Column:	<u>ZB-MR2</u>	ID:	<u>0.32</u> (mm)				

LAB FILE ID:	CF 1000 =	PO109972.D	CF 750 =	PO109973.D			
	CF 500 =	<u>PO109974.D</u>	CF 250 =	<u>PO109975.D</u>	CF 050 =	<u>PO109976.D</u>	
COMPOUND	CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1 (1)	173731434	178393712	185954312	194985500	183209860	183254964	4
Aroclor-1016-2 (2)	252919767	260842944	268062016	276298580	249399140	261504489	4
Aroclor-1016-3 (3)	134029267	138651783	144331354	150165168	141715700	141778654	4
Aroclor-1016-4 (4)	107671732	112396073	118651742	125867636	125061600	117929757	7
Aroclor-1016-5 (5)	141734749	147685869	153486032	162580972	159105760	152918676	6
Aroclor-1260-1 (1)	240074381	247747439	258832620	273383796	257170920	255441831	5
Aroclor-1260-2 (2)	281757793	288999419	301276956	315867360	313526020	300285510	5
Aroclor-1260-3 (3)	267611935	278954948	288530668	305847736	303966000	288982257	6
Aroclor-1260-4 (4)	196048044	205344145	218294872	229292036	226412760	215078371	7
Aroclor-1260-5 (5)	481983300	481761991	513782868	520791536	495161780	498696295	4
Decachlorobiphenyl	2314898720	2277821173	2432747880	2620033760	2485044400	2426109187	6
Tetrachloro-m-xylene	5279380900	5378354400	5480250420	5516817960	4565680000	5244096736	7
Aroclor-1242-1 (1)	141331278	146781083	150759024	159963196	132242600	146215436	7
Aroclor-1242-2 (2)	205951481	214434265	215763772	224841412	179186640	208035514	8
Aroclor-1242-3 (3)	108828803	114341291	116166340	122887996	95840060	111612898	9
Aroclor-1242-4 (4)	107629937	113953347	117437436	126339948	114521460	115976426	6
Aroclor-1242-5 (5)	132486572	139043136	144664964	152408060	117607760	137242098	10
Decachlorobiphenyl	2177773130	2225931947	2270761420	2435729160	2067519400	2235543011	6
Tetrachloro-m-xylene	5049304150	5177204613	5163887520	5207194080	3529903800	4825498833	15
Aroclor-1248-1 (1)	111262575	115666484	120322434	126703700	133730220	121537083	7
Aroclor-1248-2 (2)	153166873	160144767	168518512	179835124	180628540	168458763	7
Aroclor-1248-3 (3)	163639212	170966695	179105274	191715488	200520960	181189526	8
Aroclor-1248-4 (4)	192034431	200649257	208567738	223057368	227978540	210457467	7
Aroclor-1248-5 (5)	189825244	196639567	203671792	215836044	233387660	207872061	8
Decachlorobiphenyl	2147083620	2251559707	2344655820	2535991200	2605882000	2377034469	8
Tetrachloro-m-xylene	5118943080	5218637120	5295153740	5366945840	5070595200	5214054996	2
Aroclor-1254-1 (1)	289813236	298739165	307722880	314204860	352998300	312695688	8
Aroclor-1254-2 (2)	250736607	259627313	268490268	271062664	307765180	271536406	8
Aroclor-1254-3 (3)	402159669	413409125	421207530	415558372	424838600	415434659	2
Aroclor-1254-4 (4)	231846868	237861840	244387952	246184552	252577700	242571782	3
Aroclor-1254-5 (5)	329301884	337898680	348664586	361298960	302328380	335898498	7
Decachlorobiphenyl	2196807900	2276377227	2418572320	2516603360	2645427200	2410757601	7
Tetrachloro-m-xylene	5207556450	5288727027	5346917000	5051956440	5061201200	5191271623	3
Aroclor-1268-1 (1)	560759375	568986040	578205714	598591620	620126960	585333942	4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

#### CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	519206129	525348819	532636024	548739284	562258340	537637719	3
Aroclor-1268-3	(3)	397648794	399556300	412917038	427809808	440374680	415661324	4
Aroclor-1268-4	(4)	153792414	154678659	162023954	168698684	166024000	161043542	4
Aroclor-1268-5	(5)	963659212	966574348	987141016	1016062428	1031847640	993056929	3
Decachlorobiphenyl		3902633900	3983566053	4144258760	4413490680	4552839600	4199357799	7
Tetrachloro-m-xylene		5158364110	5158184947	5281917420	5320423880	5129069800	5209592031	2

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Instrument ID: ECD\_O Date(s) Analyzed: 03/18/2025 03/18/2025

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.91	3.81	4.01	115828000
		2	3.99	3.89	4.09	86499800
		3	4.07	3.97	4.17	261696000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.07	3.97	4.17	215744000
		2	4.56	4.46	4.66	114786000
		3	4.81	4.71	4.91	211780000
		4	4.98	4.88	5.08	113561000
		5	5.02	4.92	5.12	80454000
Aroclor-1262	500	1	6.84	6.74	6.94	688120000
		2	7.34	7.24	7.44	1191970000
		3	7.62	7.52	7.72	470630000
		4	7.69	7.59	7.79	874576000
		5	8.18	8.08	8.28	394442000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Instrument ID: ECD\_O Date(s) Analyzed: 03/18/2025 03/18/2025

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.90	3.80	4.00	66882200
		2	3.99	3.89	4.09	49381600
		3	4.06	3.96	4.16	151684000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.06	3.96	4.16	124093000
		2	4.79	4.69	4.89	120349000
		3	4.97	4.87	5.07	63656000
		4	5.05	4.95	5.15	59341000
		5	5.22	5.12	5.32	63217800
Aroclor-1262	500	1	6.81	6.71	6.91	344312000
		2	7.31	7.21	7.41	537220000
		3	7.59	7.49	7.69	194051000
		4	7.65	7.55	7.75	361786000
		5	8.15	8.05	8.25	141162000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109972.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:03  
 Operator : YP/AJ  
 Sample : AR1660ICC1000  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:33:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.693	3.690	919.2E6	527.9E6	98.055	98.133
2) SA Decachlor...	8.745	8.696	731.4E6	231.5E6	97.328	97.518

Target Compounds

3) L1 AR-1016-1	4.786	4.772	318.8E6	173.7E6	964.622	966.018
4) L1 AR-1016-2	4.805	4.791	446.4E6	252.9E6	968.766	970.935
5) L1 AR-1016-3	4.862	4.967	297.1E6	134.0E6	956.293	962.990
6) L1 AR-1016-4	4.982	5.009	238.0E6	107.7E6	960.716	951.485
7) L1 AR-1016-5	5.240	5.222	250.5E6	141.7E6	957.522	960.195
31) L7 AR-1260-1	6.281	6.254	448.5E6	240.1E6	970.326	962.401
32) L7 AR-1260-2	6.470	6.442	549.8E6	281.8E6	977.958	966.521
33) L7 AR-1260-3	6.838	6.595	466.2E6	267.6E6	978.732	962.386
34) L7 AR-1260-4	7.098	7.066	395.6E6	196.0E6	958.524	946.308
35) L7 AR-1260-5	7.340	7.307	1037.2E6	482.0E6	981.381	968.065



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109972.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:03  
 Operator : YP/AJ  
 Sample : AR1660ICC1000  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1660ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:33:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

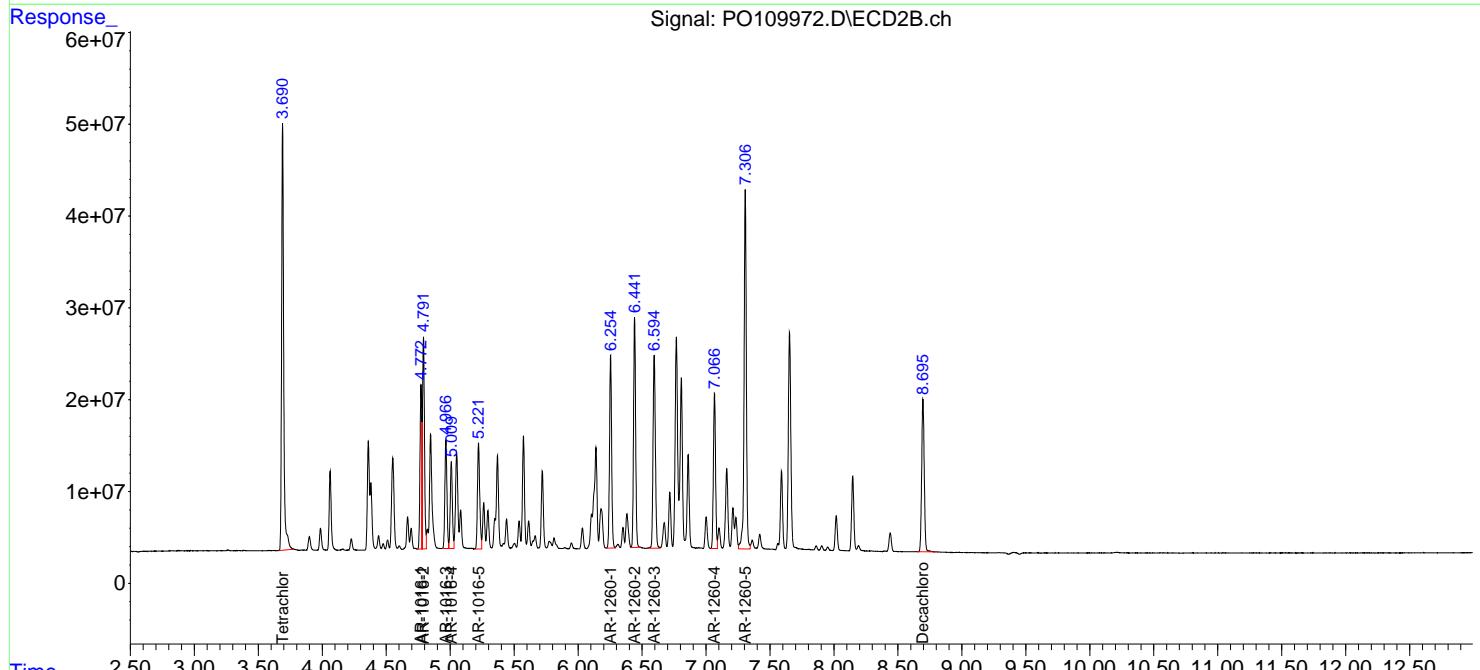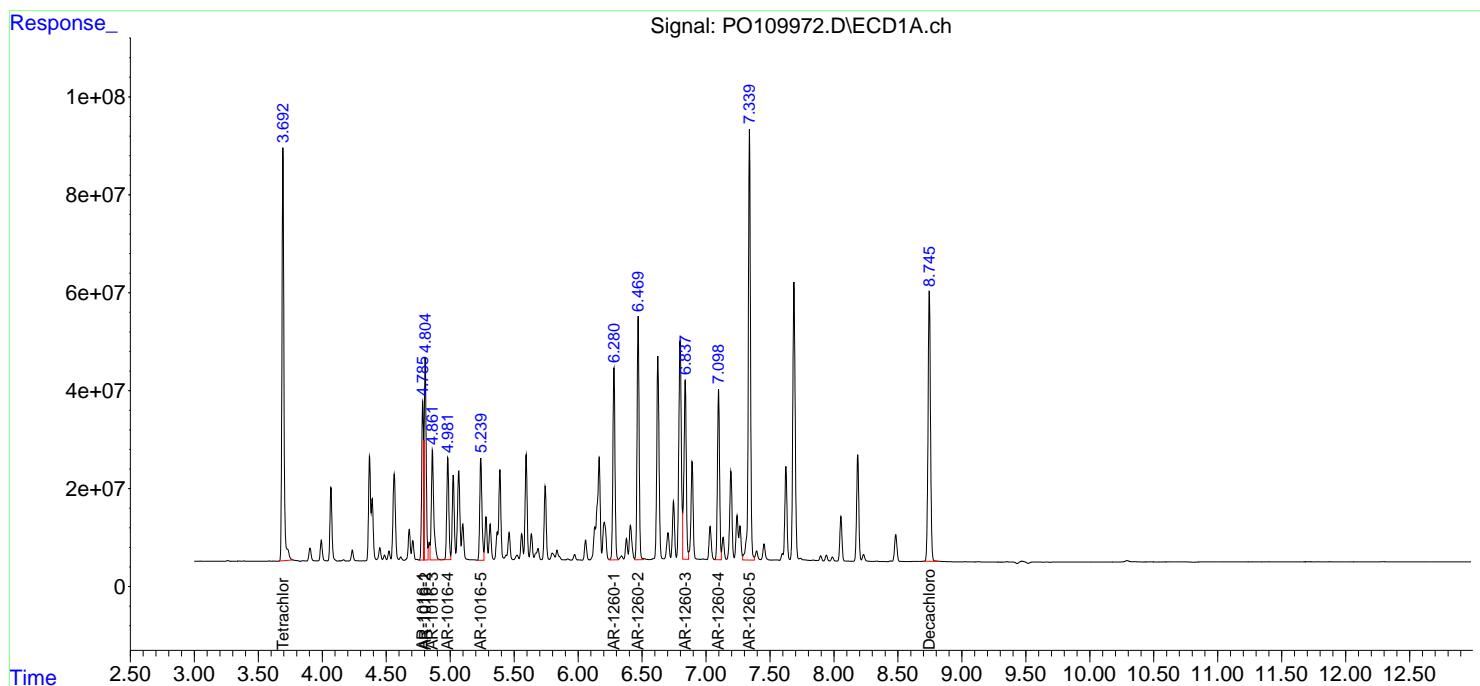

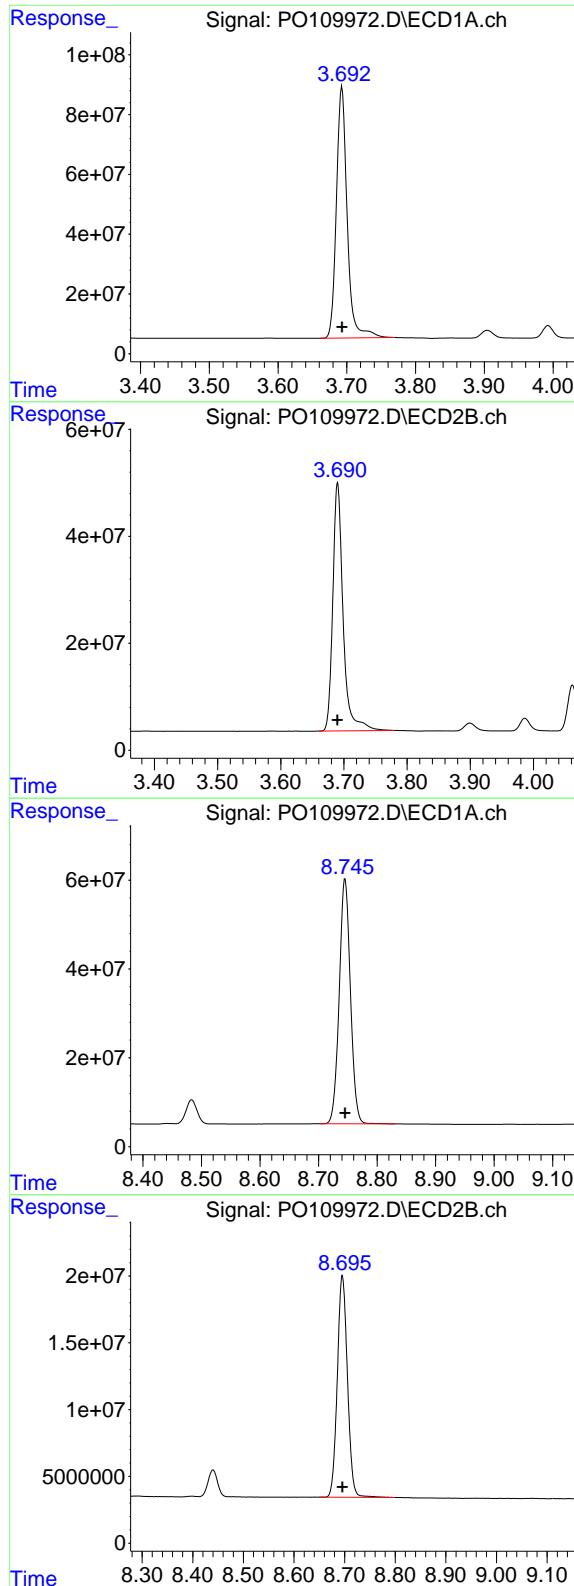

## #1 Tetrachloro-m-xylene

R.T.: 3.693 min  
Delta R.T.: 0.000 min  
Response: 919161808  
Conc: 98.05 ng/ml

Instrument:

ECD\_O

ClientSampleId :

AR1660ICC1000

## #1 Tetrachloro-m-xylene


R.T.: 3.690 min  
Delta R.T.: 0.000 min  
Response: 527938090  
Conc: 98.13 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.745 min  
Delta R.T.: 0.000 min  
Response: 731426877  
Conc: 97.33 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 231489872  
Conc: 97.52 ng/ml

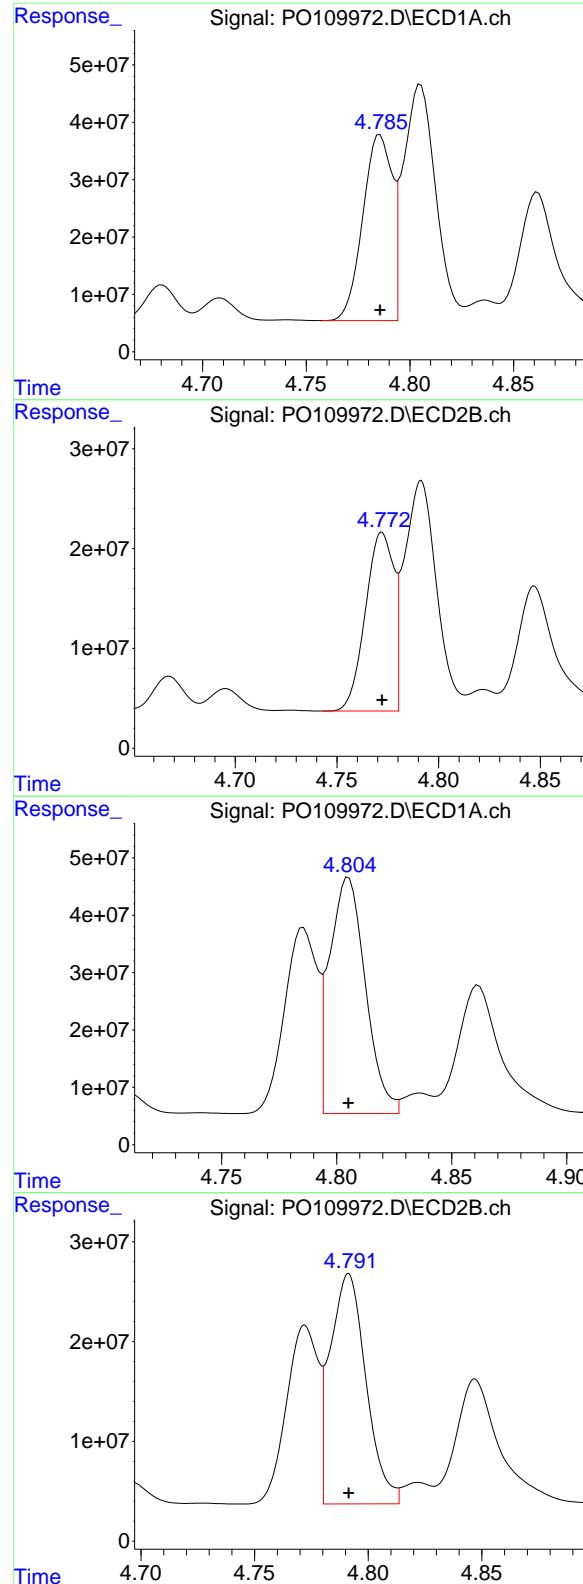

#3 AR-1016-1

R.T.: 4.786 min  
 Delta R.T.: 0.000 min  
 Response: 318793340  
 Conc: 964.62 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC1000

#3 AR-1016-1

R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 173731434  
 Conc: 966.02 ng/ml

#4 AR-1016-2

R.T.: 4.805 min  
 Delta R.T.: 0.000 min  
 Response: 446388679  
 Conc: 968.77 ng/ml


#4 AR-1016-2

R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 252919767  
 Conc: 970.94 ng/ml

#5 AR-1016-3


R.T.: 4.862 min  
 Delta R.T.: 0.000 min  
 Response: 297123739  
 Conc: 956.29 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC1000




#5 AR-1016-3

R.T.: 4.967 min  
 Delta R.T.: 0.000 min  
 Response: 134029267  
 Conc: 962.99 ng/ml

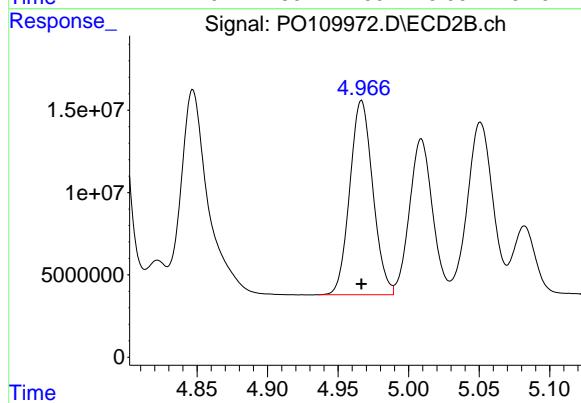


#6 AR-1016-4





R.T.: 4.982 min  
 Delta R.T.: 0.000 min  
 Response: 237983440  
 Conc: 960.72 ng/ml

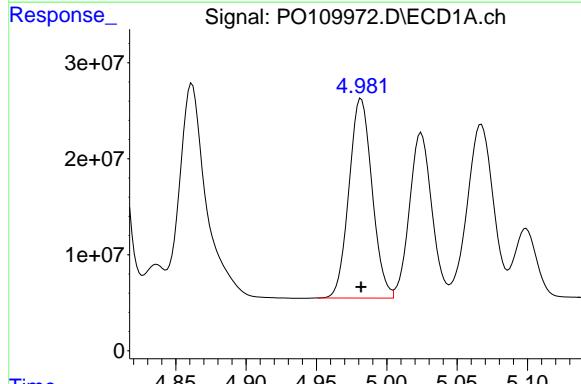

#6 AR-1016-4

R.T.: 5.009 min  
 Delta R.T.: 0.000 min  
 Response: 107671732  
 Conc: 951.49 ng/ml

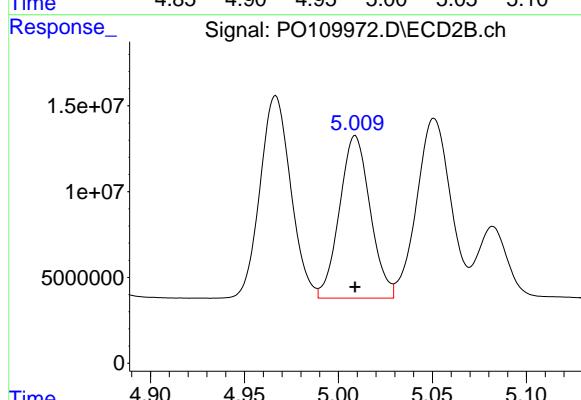

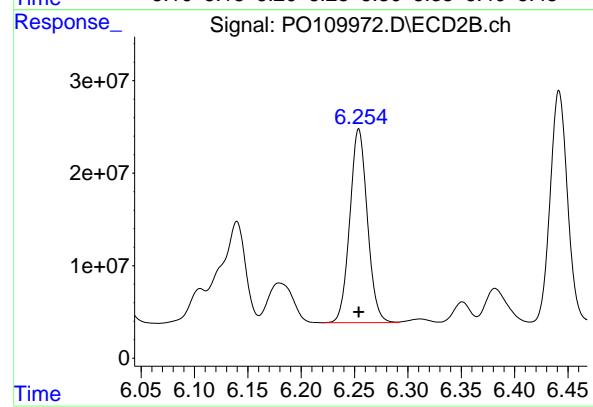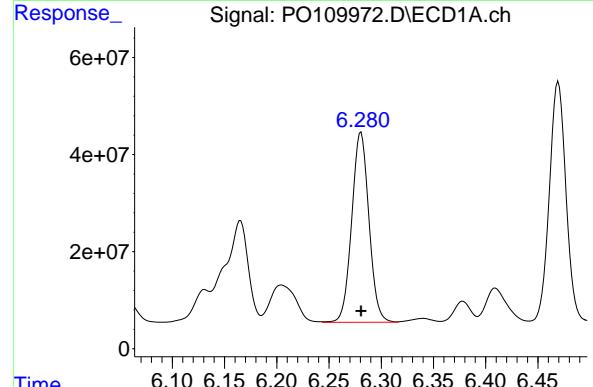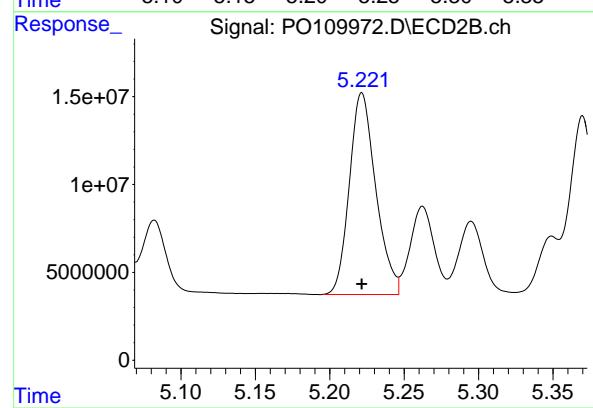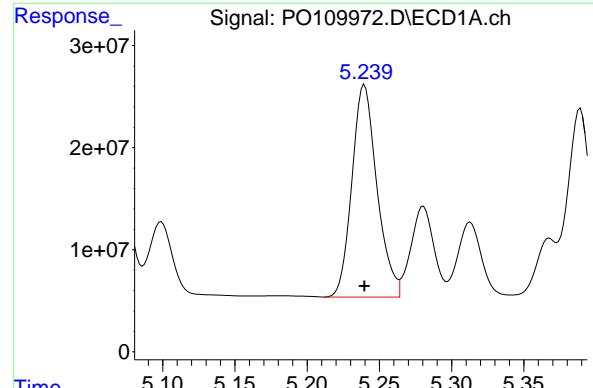

#7 AR-1016-5

R.T.: 5.240 min  
 Delta R.T.: 0.000 min  
 Response: 250501585  
 Conc: 957.52 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC1000

#7 AR-1016-5

R.T.: 5.222 min  
 Delta R.T.: 0.000 min  
 Response: 141734749  
 Conc: 960.19 ng/ml

#31 AR-1260-1

R.T.: 6.281 min  
 Delta R.T.: 0.000 min  
 Response: 448474074  
 Conc: 970.33 ng/ml





#31 AR-1260-1

R.T.: 6.254 min  
 Delta R.T.: 0.000 min  
 Response: 240074381  
 Conc: 962.40 ng/ml

#32 AR-1260-2

R.T.: 6.470 min  
 Delta R.T.: 0.000 min  
 Response: 549756400  
 Conc: 977.96 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC1000

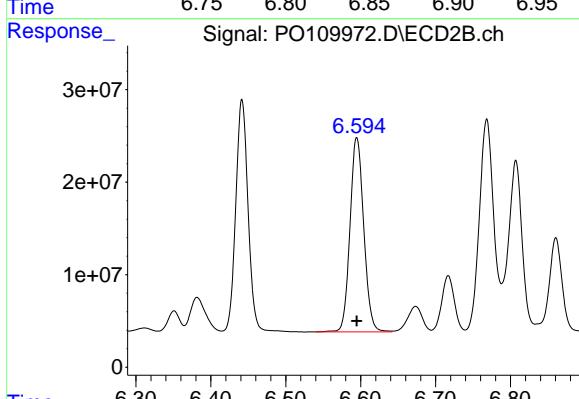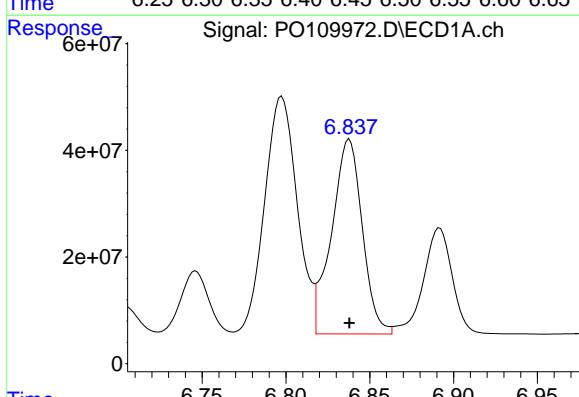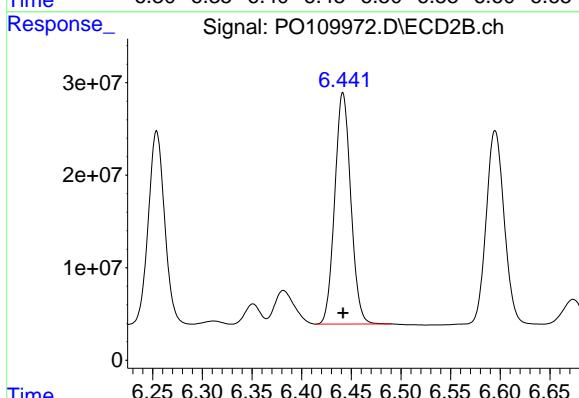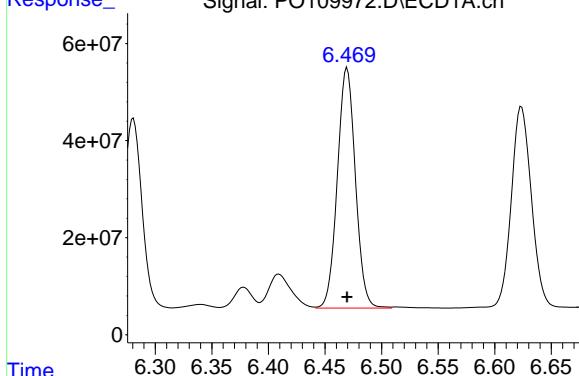

#32 AR-1260-2

R.T.: 6.442 min  
 Delta R.T.: 0.000 min  
 Response: 281757793  
 Conc: 966.52 ng/ml

#33 AR-1260-3

R.T.: 6.838 min  
 Delta R.T.: 0.000 min  
 Response: 466244522  
 Conc: 978.73 ng/ml


#33 AR-1260-3

R.T.: 6.595 min  
 Delta R.T.: 0.000 min  
 Response: 267611935  
 Conc: 962.39 ng/ml

#34 AR-1260-4


R.T.: 7.098 min  
 Delta R.T.: 0.000 min  
 Response: 395577993  
 Conc: 958.52 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC1000

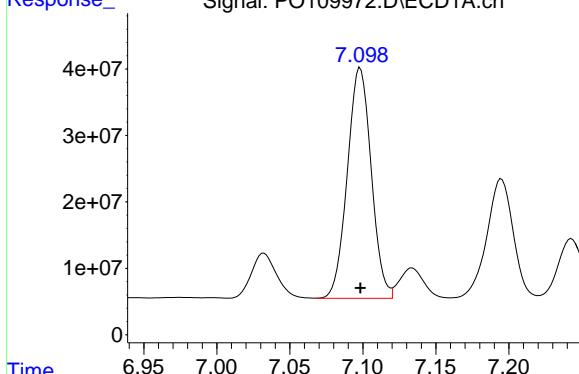


#34 AR-1260-4

R.T.: 7.066 min  
 Delta R.T.: 0.000 min  
 Response: 196048044  
 Conc: 946.31 ng/ml

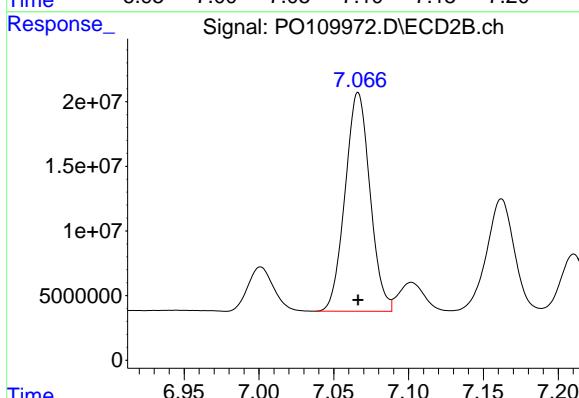


#35 AR-1260-5

R.T.: 7.340 min  
 Delta R.T.: 0.000 min  
 Response: 1037246832  
 Conc: 981.38 ng/ml

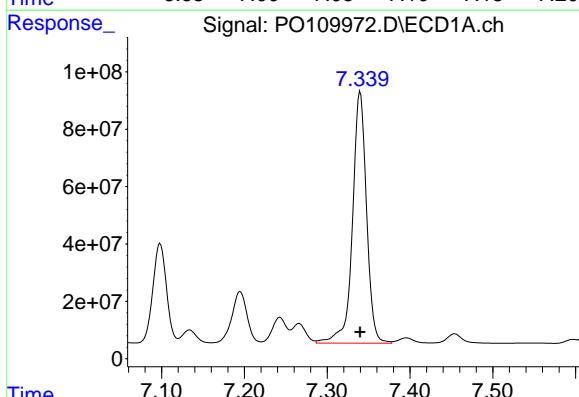

#35 AR-1260-5

R.T.: 7.307 min  
 Delta R.T.: 0.000 min  
 Response: 481983300  
 Conc: 968.07 ng/ml

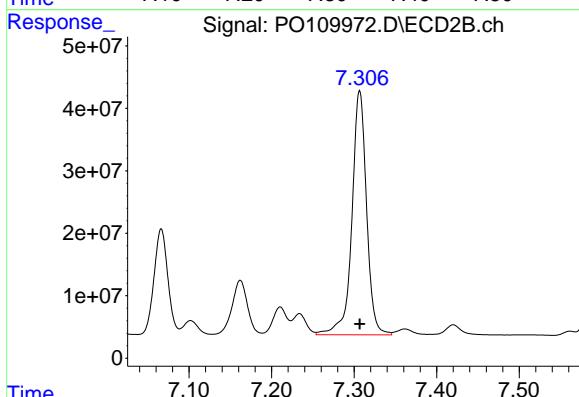

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109973.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:21  
 Operator : YP/AJ  
 Sample : AR1660ICC750  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1660ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:36:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	3.693	3.690	705.7E6	403.4E6	75.190	74.986
2) SA Decachlor...	8.745	8.696	568.9E6	170.8E6	75.465	72.950

**Target Compounds**

3) L1 AR-1016-1	4.785	4.772	246.8E6	133.8E6	747.915	745.960
4) L1 AR-1016-2	4.805	4.791	347.8E6	195.6E6	753.172	750.675
5) L1 AR-1016-3	4.862	4.967	233.7E6	104.0E6	751.394	748.099
6) L1 AR-1016-4	4.982	5.009	186.4E6	84297055	751.636	746.609
7) L1 AR-1016-5	5.239	5.222	197.8E6	110.8E6	753.927	750.256
31) L7 AR-1260-1	6.280	6.255	350.7E6	185.8E6	755.816	746.573
32) L7 AR-1260-2	6.470	6.442	429.8E6	216.7E6	759.623	745.669
33) L7 AR-1260-3	6.837	6.595	362.6E6	209.2E6	757.414	751.587
34) L7 AR-1260-4	7.098	7.067	310.3E6	154.0E6	751.251	745.577
35) L7 AR-1260-5	7.340	7.307	800.9E6	361.3E6	755.153	735.355m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109973.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:21  
 Operator : YP/AJ  
 Sample : AR1660ICC750  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:36:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_O  
 ClientSampleId :  
 AR1660ICC750

### Manual Integrations APPROVED

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

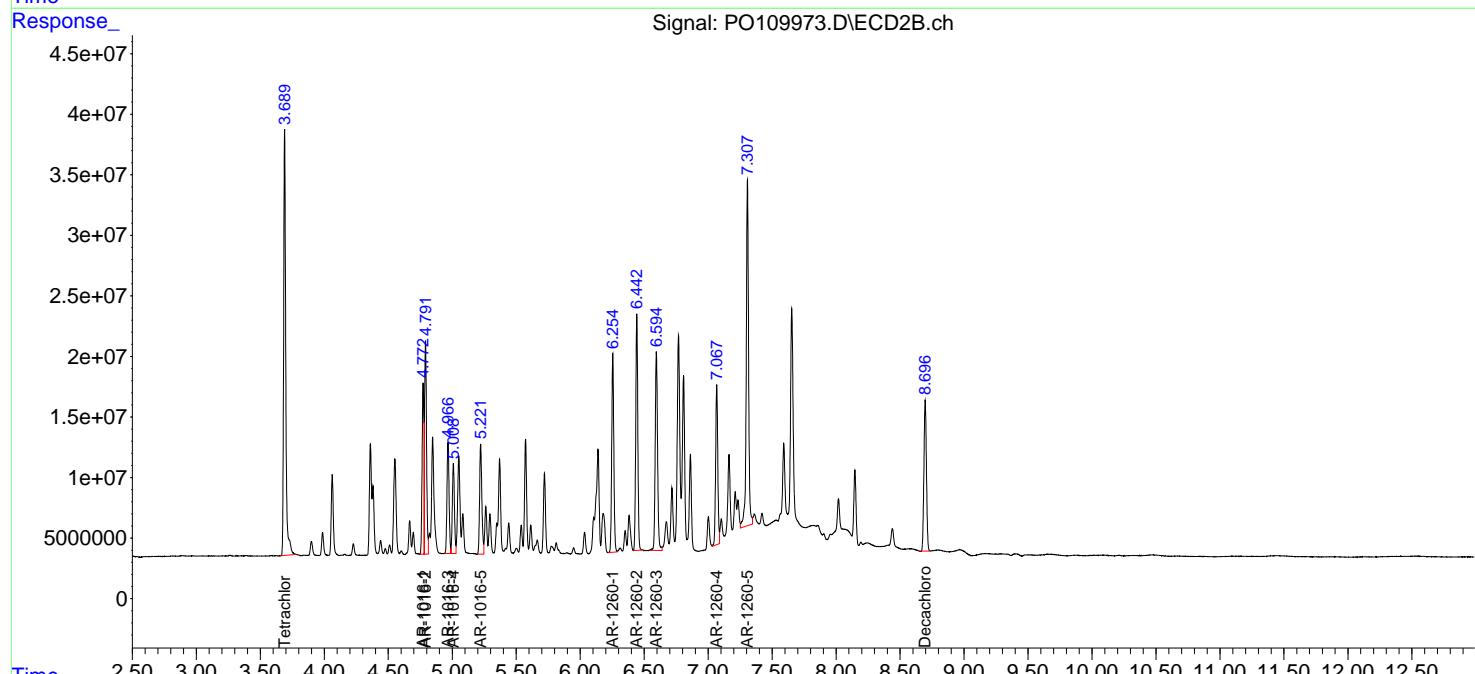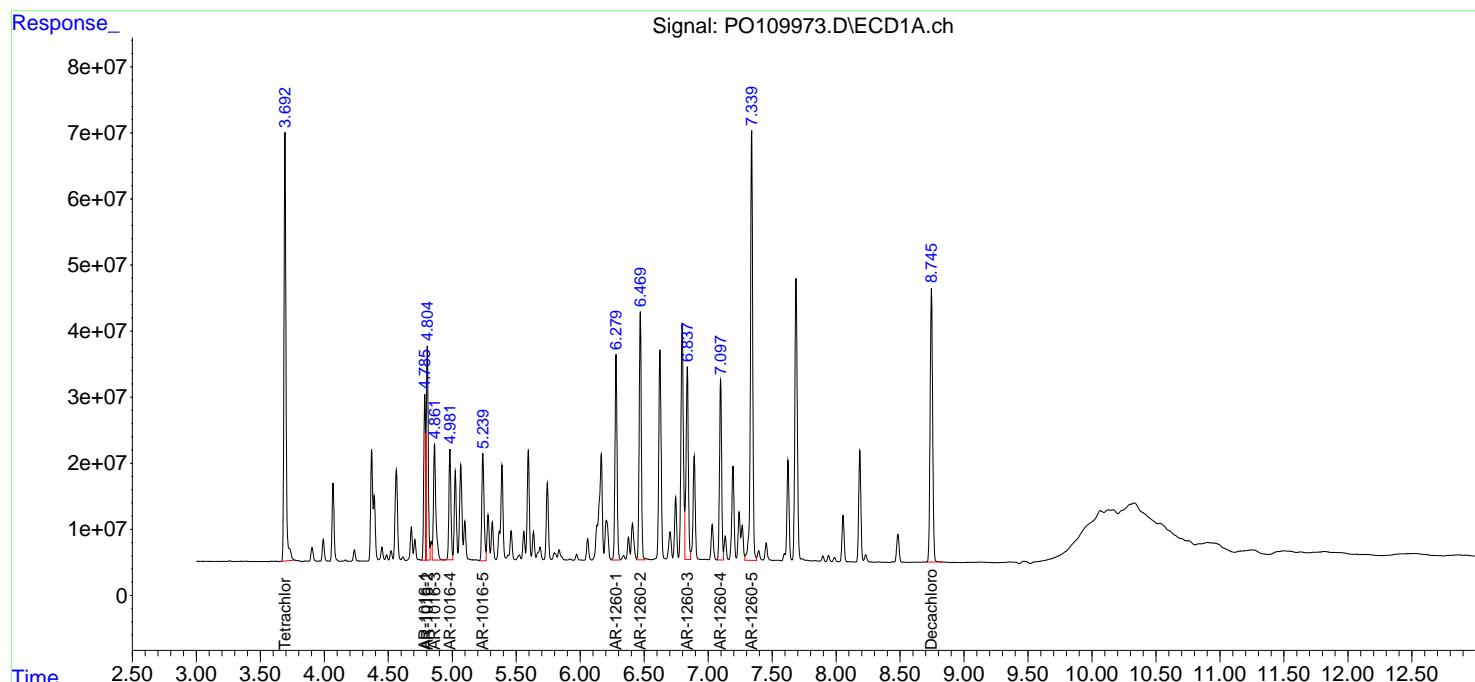

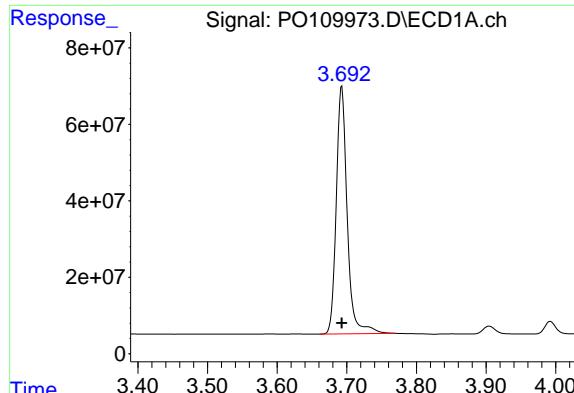


## #1 Tetrachloro-m-xylene

R.T.: 3.693 min  
Delta R.T.: 0.000 min  
Response: 705727801  
Conc: 75.19 ng/ml

**Instrument:**  
ECD\_O  
**ClientSampleId :**  
AR1660ICC750


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

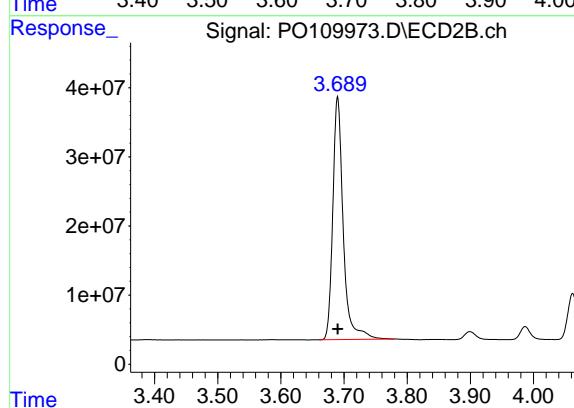


## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
Delta R.T.: 0.000 min  
Response: 403376580  
Conc: 74.99 ng/ml

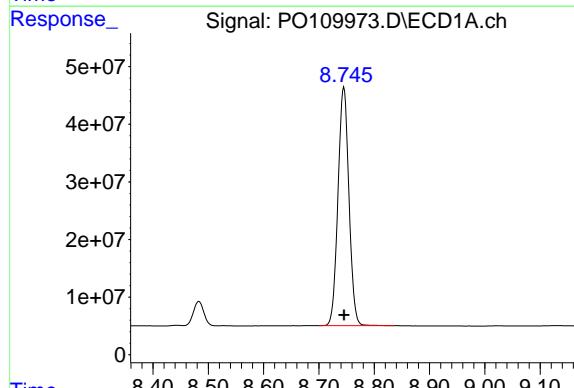

## #2 Decachlorobiphenyl

R.T.: 8.745 min  
Delta R.T.: 0.000 min  
Response: 568890214  
Conc: 75.47 ng/ml

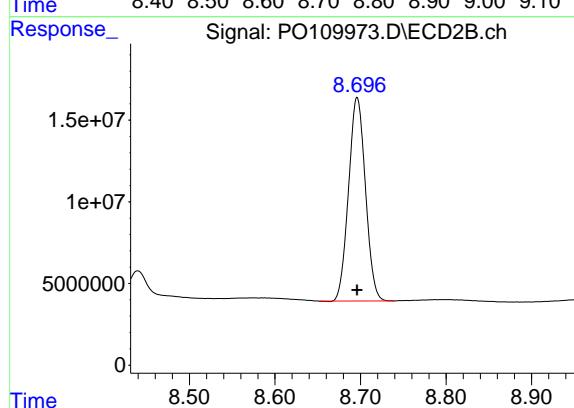

## #2 Decachlorobiphenyl

R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 170836588  
Conc: 72.95 ng/ml





#3 AR-1016-1

R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 246831835  
 Conc: 747.92 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

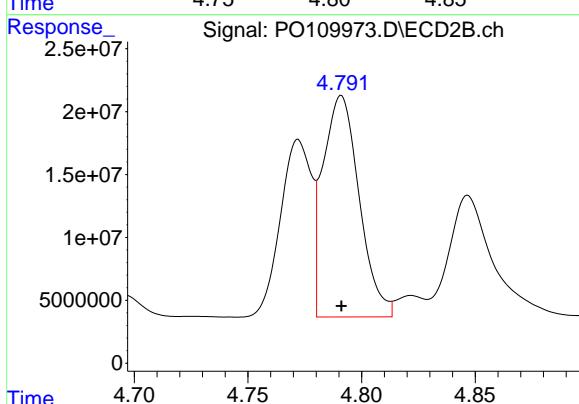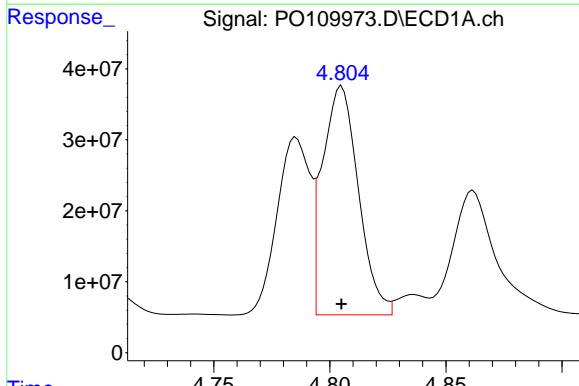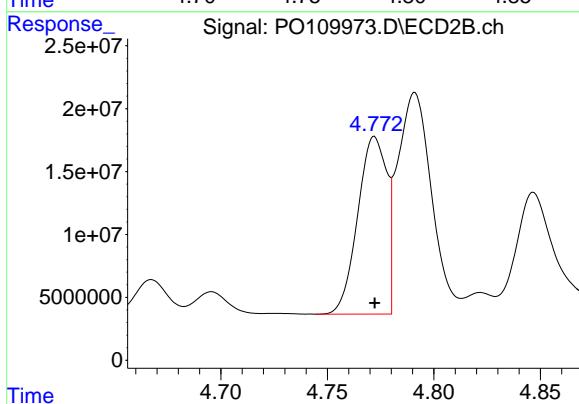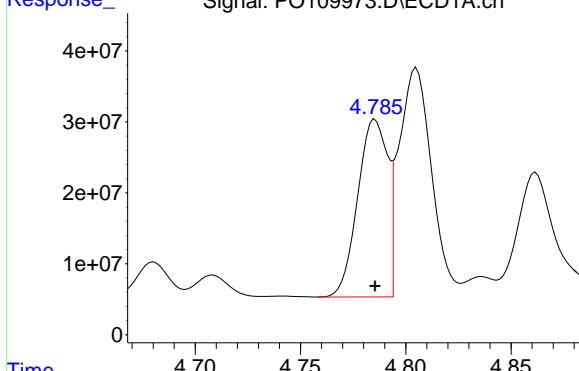

#3 AR-1016-1

R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 133795284  
 Conc: 745.96 ng/ml

#4 AR-1016-2

R.T.: 4.805 min  
 Delta R.T.: 0.000 min  
 Response: 347782380  
 Conc: 753.17 ng/ml

#4 AR-1016-2

R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 195632208  
 Conc: 750.68 ng/ml





#5 AR-1016-3

R.T.: 4.862 min  
 Delta R.T.: 0.000 min  
 Response: 233678232  
 Conc: 751.39 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

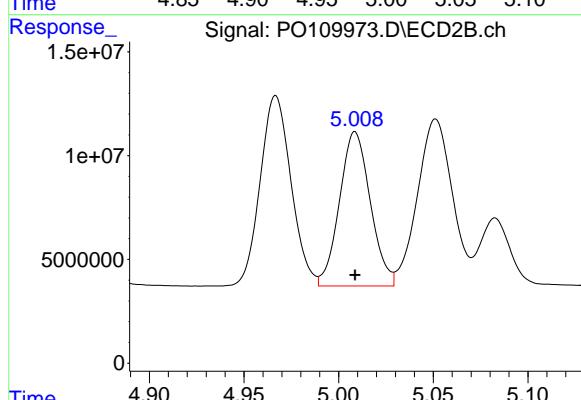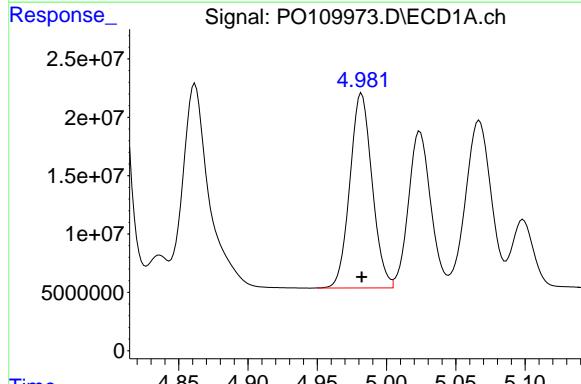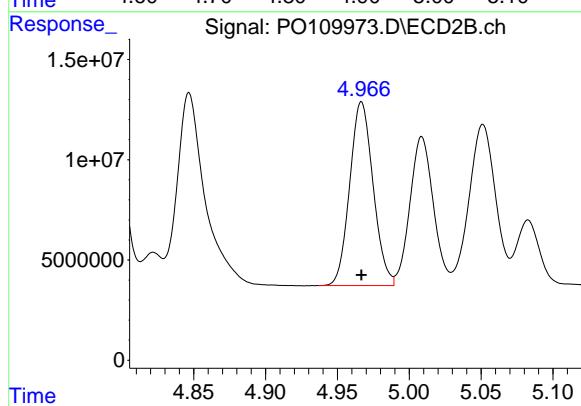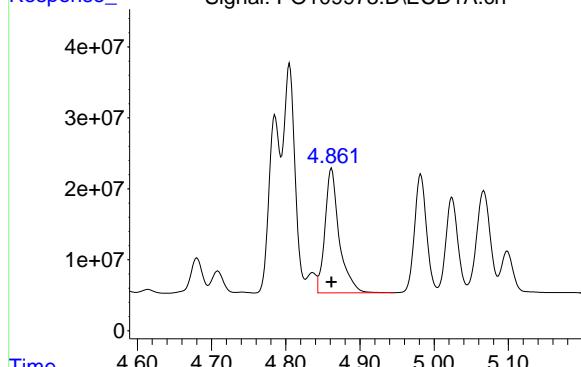

#5 AR-1016-3


R.T.: 4.967 min  
 Delta R.T.: 0.000 min  
 Response: 103988837  
 Conc: 748.10 ng/ml

#6 AR-1016-4

R.T.: 4.982 min  
 Delta R.T.: 0.000 min  
 Response: 186394664  
 Conc: 751.64 ng/ml

#6 AR-1016-4

R.T.: 5.009 min  
 Delta R.T.: 0.000 min  
 Response: 84297055  
 Conc: 746.61 ng/ml

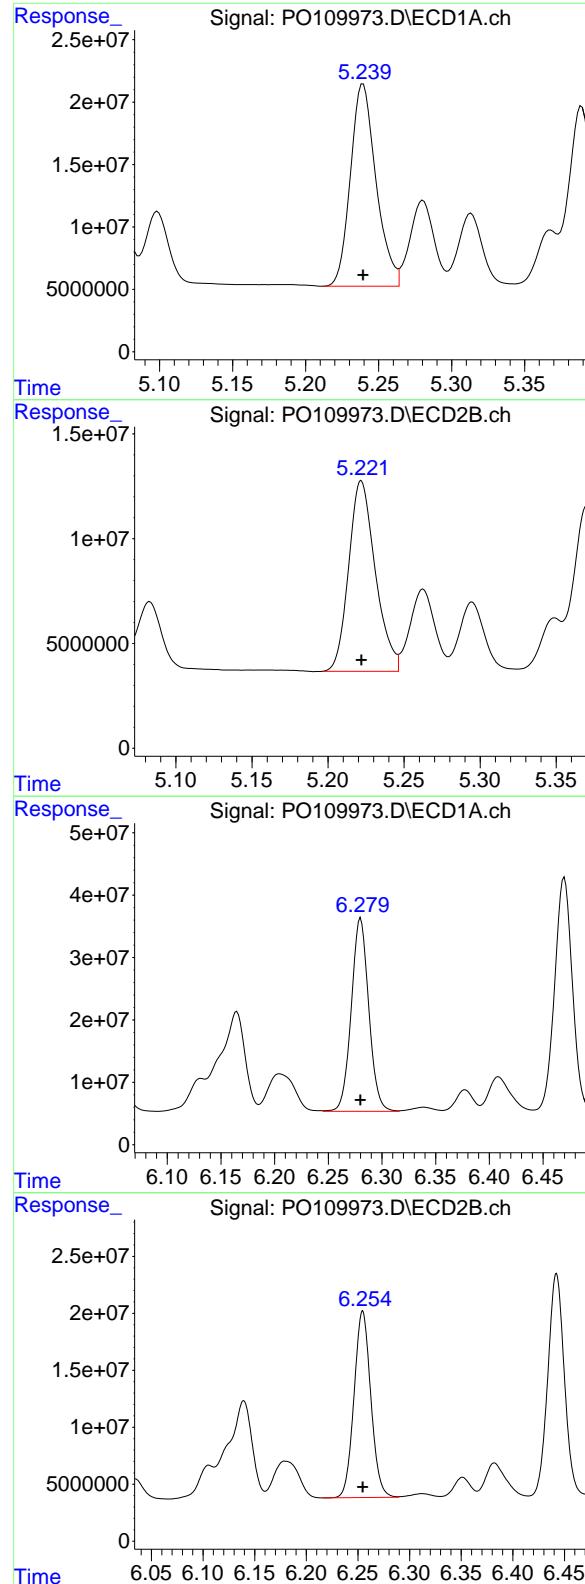

#7 AR-1016-5

R.T.: 5.239 min  
 Delta R.T.: 0.000 min  
 Response: 197756047  
 Conc: 753.93 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#7 AR-1016-5


R.T.: 5.222 min  
 Delta R.T.: 0.000 min  
 Response: 110764402  
 Conc: 750.26 ng/ml

#31 AR-1260-1

R.T.: 6.280 min  
 Delta R.T.: 0.000 min  
 Response: 350689884  
 Conc: 755.82 ng/ml

#31 AR-1260-1

R.T.: 6.255 min  
 Delta R.T.: 0.000 min  
 Response: 185810579  
 Conc: 746.57 ng/ml

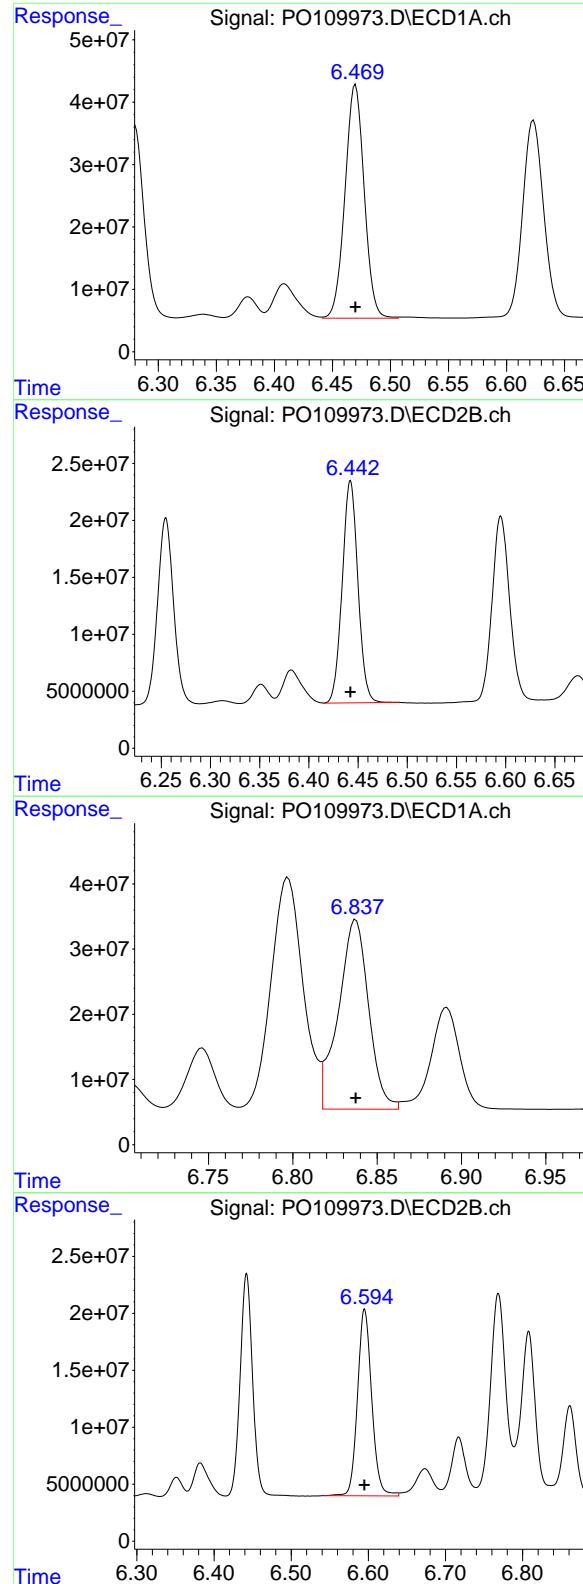

#32 AR-1260-2

R.T.: 6.470 min  
 Delta R.T.: 0.000 min  
 Response: 429776784  
 Conc: 759.62 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#32 AR-1260-2

R.T.: 6.442 min  
 Delta R.T.: 0.000 min  
 Response: 216749564  
 Conc: 745.67 ng/ml

#33 AR-1260-3

R.T.: 6.837 min  
 Delta R.T.: 0.000 min  
 Response: 362605874  
 Conc: 757.41 ng/ml

#33 AR-1260-3

R.T.: 6.595 min  
 Delta R.T.: 0.000 min  
 Response: 209216211  
 Conc: 751.59 ng/ml





#34 AR-1260-4

R.T.: 7.098 min  
 Delta R.T.: 0.000 min  
 Response: 310296283  
 Conc: 751.25 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

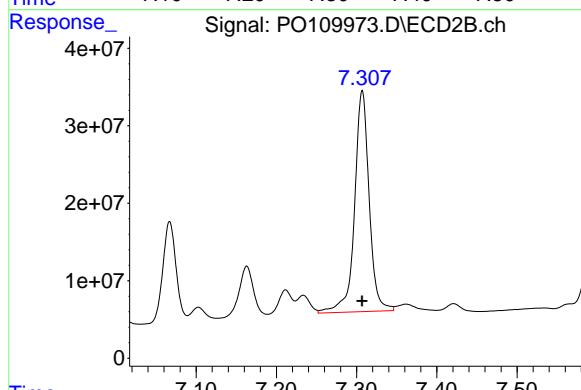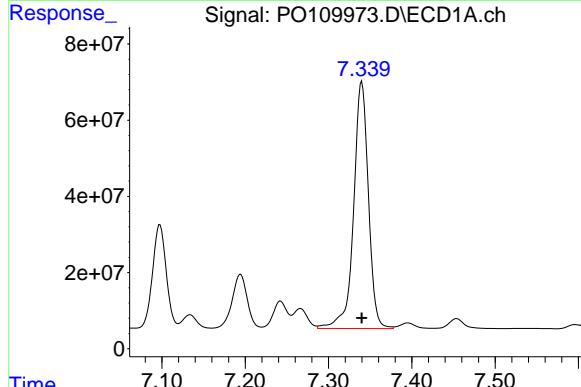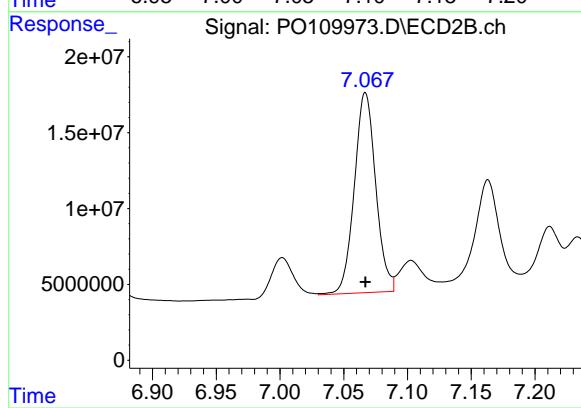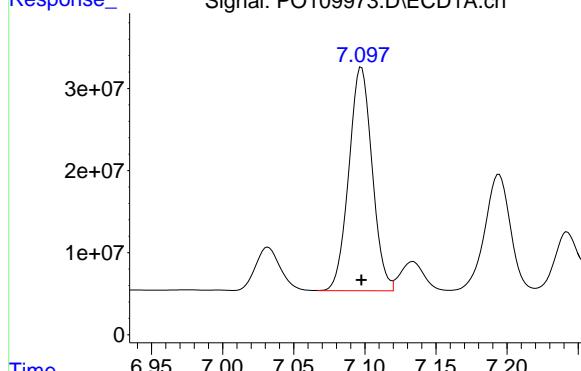

#34 AR-1260-4

R.T.: 7.067 min  
 Delta R.T.: 0.000 min  
 Response: 154008109  
 Conc: 745.58 ng/ml

#35 AR-1260-5

R.T.: 7.340 min  
 Delta R.T.: 0.000 min  
 Response: 800891670  
 Conc: 755.15 ng/ml

#35 AR-1260-5

R.T.: 7.307 min  
 Delta R.T.: 0.000 min  
 Response: 361321493  
 Conc: 735.35 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109974.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:39  
 Operator : YP/AJ  
 Sample : AR1660ICC500  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1660ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:30:52 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	477.8E6	274.0E6	50.000	50.000
2) SA Decachlor...	8.745	8.696	385.8E6	121.6E6	50.000	50.000

Target Compounds

3) L1 AR-1016-1	4.785	4.772	171.1E6	92977156	500.000	500.000
4) L1 AR-1016-2	4.804	4.791	237.6E6	134.0E6	500.000	500.000
5) L1 AR-1016-3	4.861	4.967	162.1E6	72165677	500.000	500.000
6) L1 AR-1016-4	4.981	5.009	128.7E6	59325871	500.000	500.000
7) L1 AR-1016-5	5.239	5.222	136.4E6	76743016	500.000	500.000
31) L7 AR-1260-1	6.280	6.255	238.0E6	129.4E6	500.000	500.000
32) L7 AR-1260-2	6.469	6.442	287.3E6	150.6E6	500.000	500.000
33) L7 AR-1260-3	6.837	6.595	243.3E6	144.3E6	500.000	500.000
34) L7 AR-1260-4	7.098	7.067	214.9E6	109.1E6	500.000	500.000
35) L7 AR-1260-5	7.339	7.307	538.3E6	256.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109974.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:39  
 Operator : YP/AJ  
 Sample : AR1660ICC500  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1660ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:30:52 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

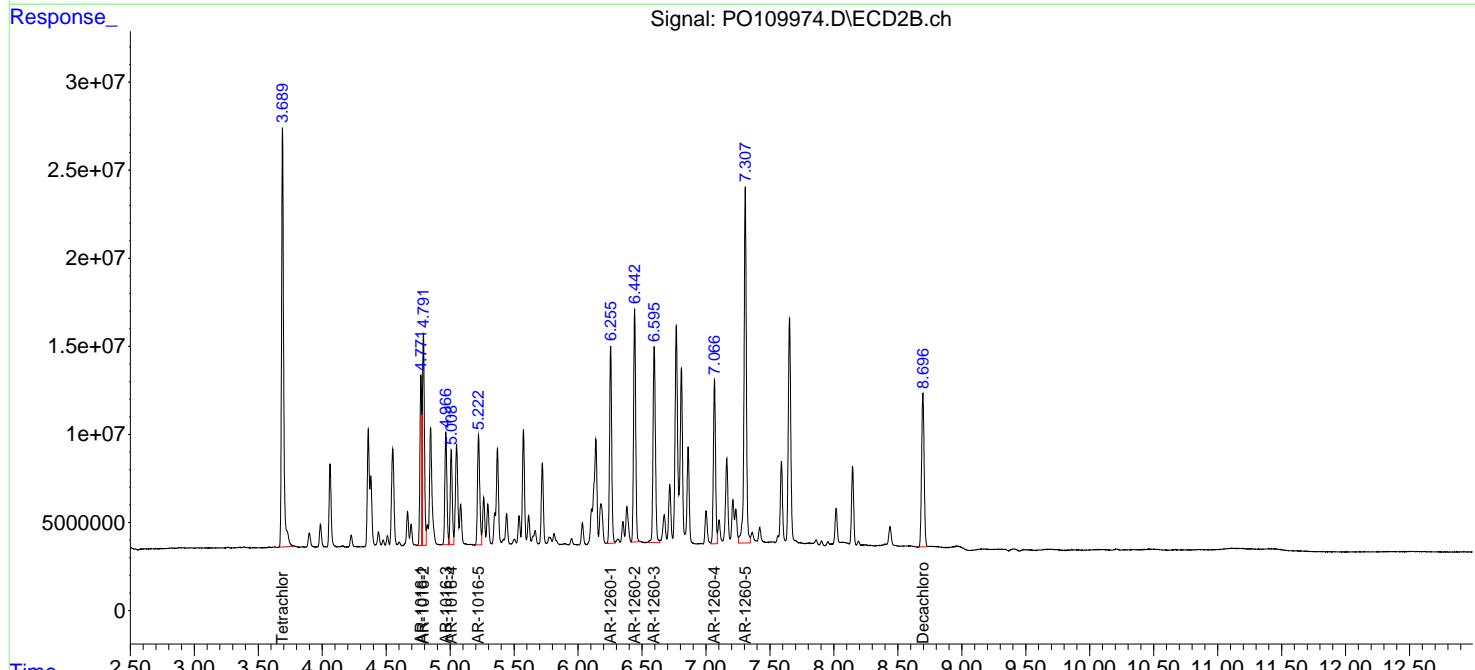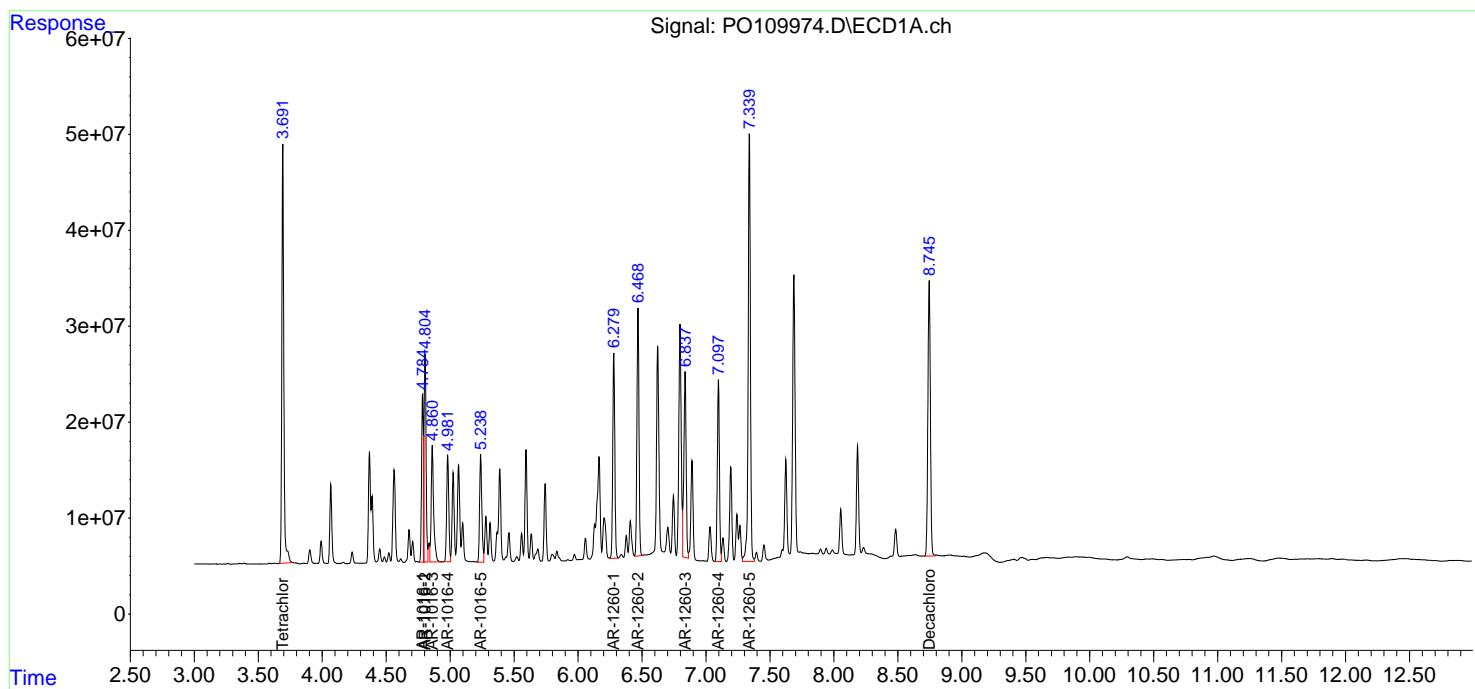

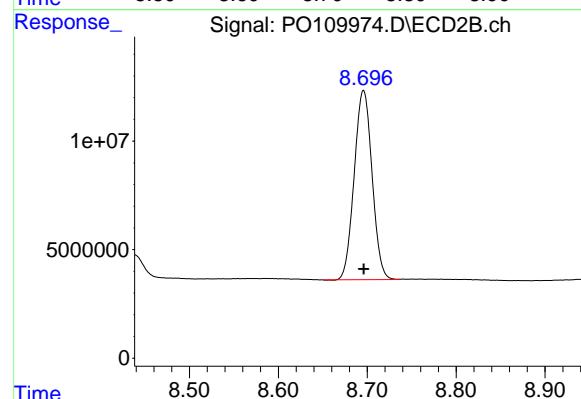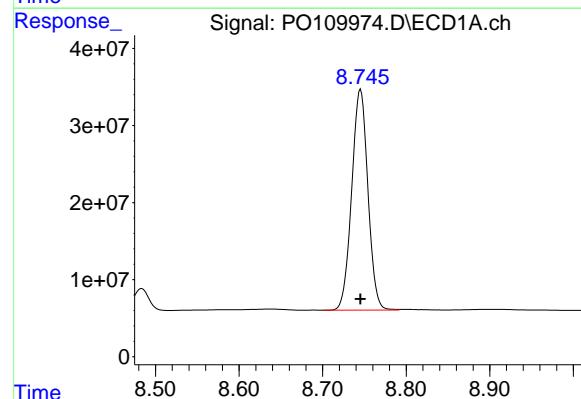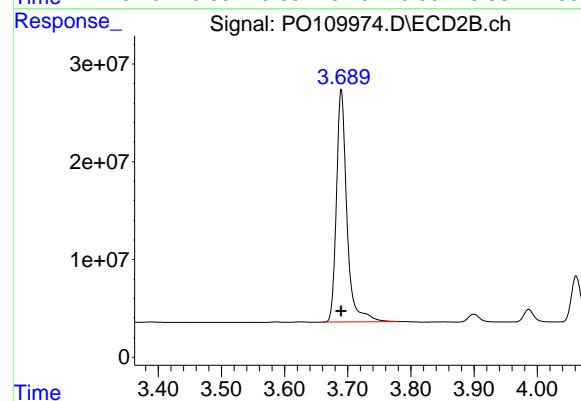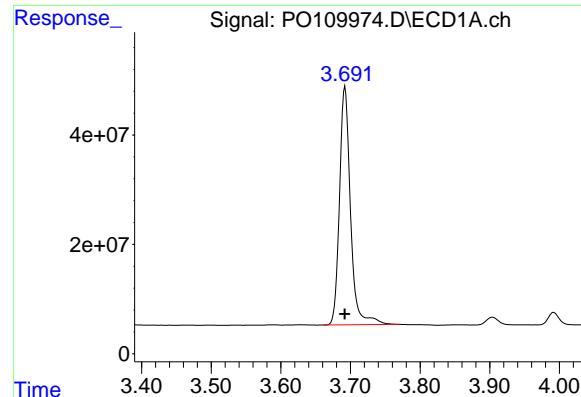

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 477817549  
Conc: 50.00 ng/ml

Instrument:

ECD\_O

ClientSampleId :

AR1660ICC500

## #1 Tetrachloro-m-xylene





R.T.: 3.690 min  
Delta R.T.: 0.000 min  
Response: 274012521  
Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.745 min  
Delta R.T.: 0.000 min  
Response: 385791842  
Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 121637394  
Conc: 50.00 ng/ml

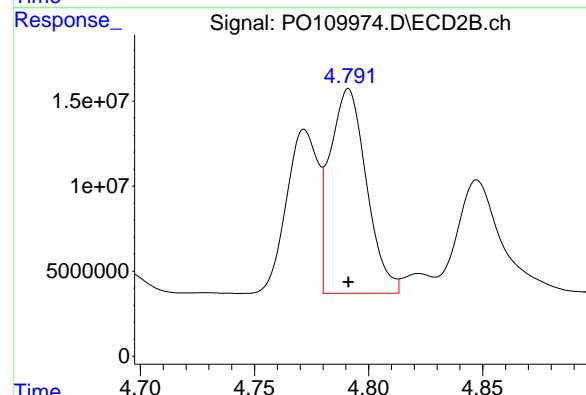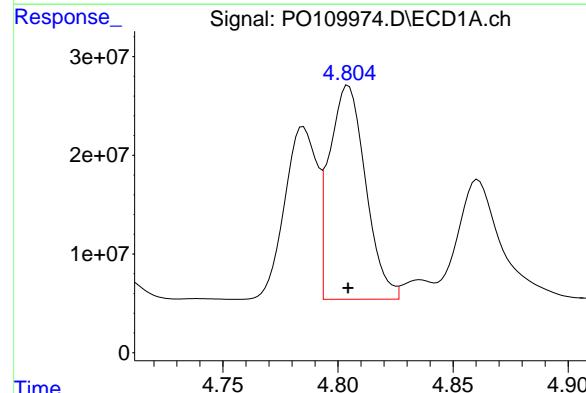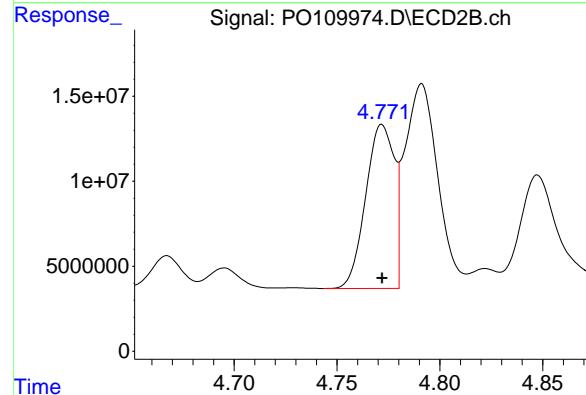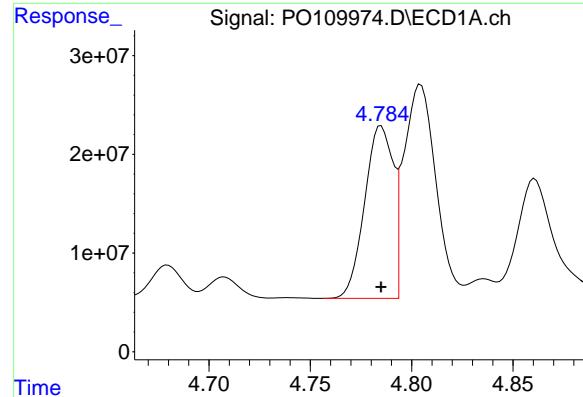

#3 AR-1016-1

R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
**Instrument:**  
 Response: 171088494 ECD\_O  
 Conc: 500.00 ng/ml ClientSampleId :  
 AR1660ICC500

#3 AR-1016-1

R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 92977156  
 Conc: 500.00 ng/ml

#4 AR-1016-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 237586218  
 Conc: 500.00 ng/ml





#4 AR-1016-2

R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 134031008  
 Conc: 500.00 ng/ml

#5 AR-1016-3

R.T.: 4.861 min  
 Delta R.T.: 0.000 min  
 Response: 162141843  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC500

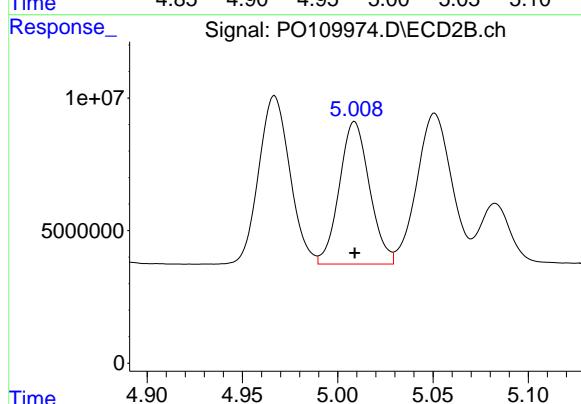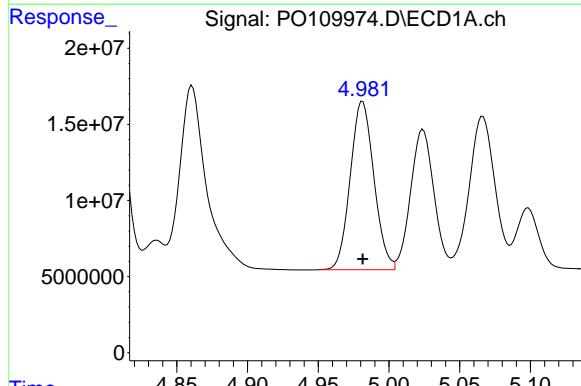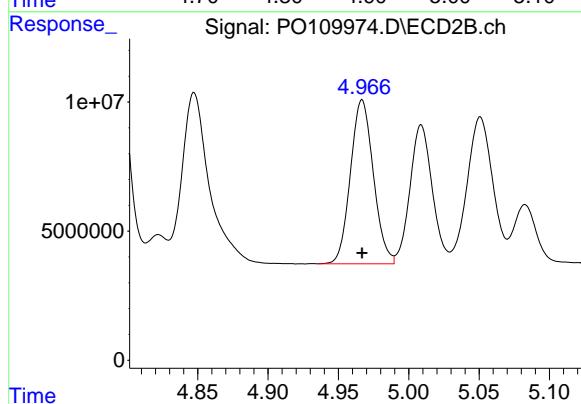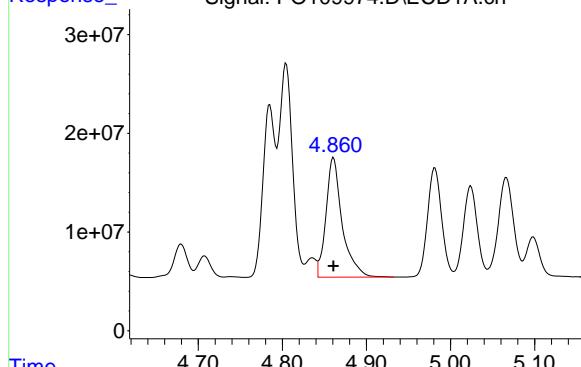

#5 AR-1016-3



R.T.: 4.967 min  
 Delta R.T.: 0.000 min  
 Response: 72165677  
 Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 128722871  
 Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 5.009 min  
 Delta R.T.: 0.000 min  
 Response: 59325871  
 Conc: 500.00 ng/ml

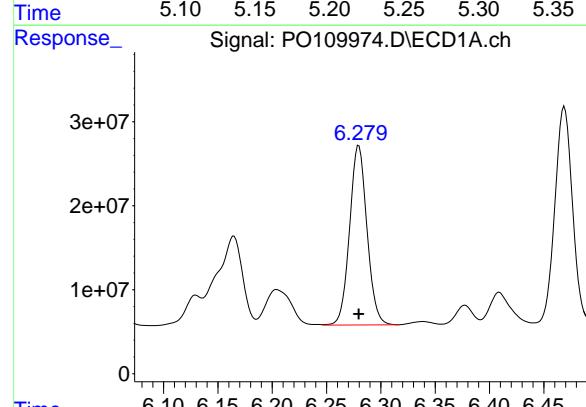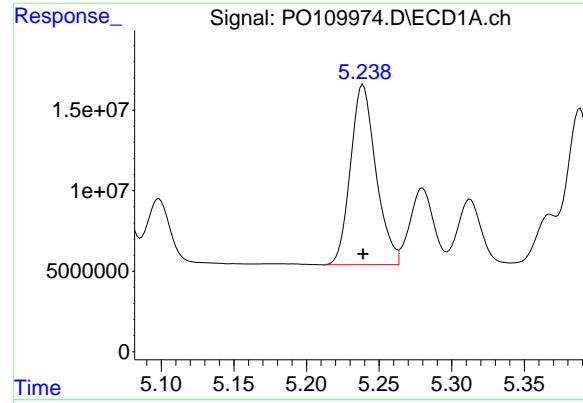

#7 AR-1016-5

R.T.: 5.239 min  
 Delta R.T.: 0.000 min  
 Response: 136363594  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC500

#7 AR-1016-5


R.T.: 5.222 min  
 Delta R.T.: 0.000 min  
 Response: 76743016  
 Conc: 500.00 ng/ml

#31 AR-1260-1

R.T.: 6.280 min  
 Delta R.T.: 0.000 min  
 Response: 237952141  
 Conc: 500.00 ng/ml

#31 AR-1260-1

R.T.: 6.255 min  
 Delta R.T.: 0.000 min  
 Response: 129416310  
 Conc: 500.00 ng/ml

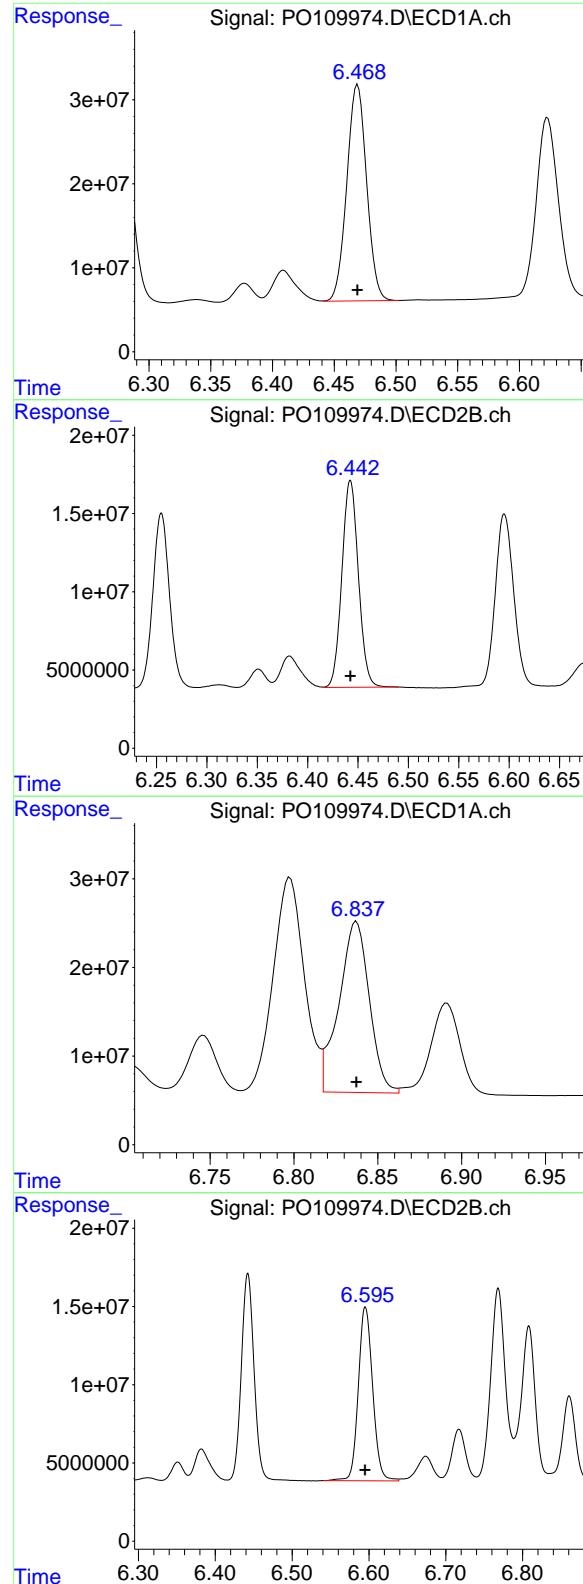

#32 AR-1260-2

R.T.: 6.469 min  
 Delta R.T.: 0.000 min  
 Response: 287269085  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC500

#32 AR-1260-2

R.T.: 6.442 min  
 Delta R.T.: 0.000 min  
 Response: 150638478  
 Conc: 500.00 ng/ml

#33 AR-1260-3

R.T.: 6.837 min  
 Delta R.T.: 0.000 min  
 Response: 243253685  
 Conc: 500.00 ng/ml





#33 AR-1260-3

R.T.: 6.595 min  
 Delta R.T.: 0.000 min  
 Response: 144265334  
 Conc: 500.00 ng/ml

#34 AR-1260-4

R.T.: 7.098 min  
 Delta R.T.: 0.000 min  
 Response: 214906066  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC500

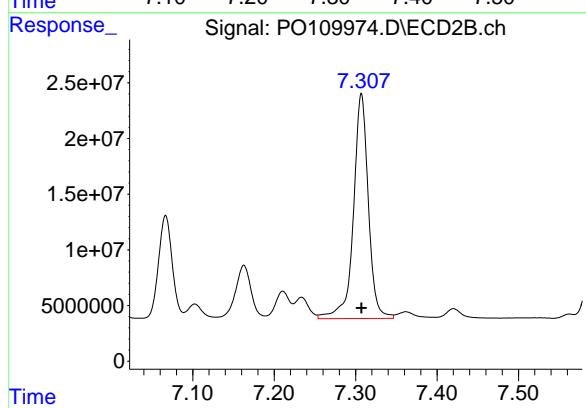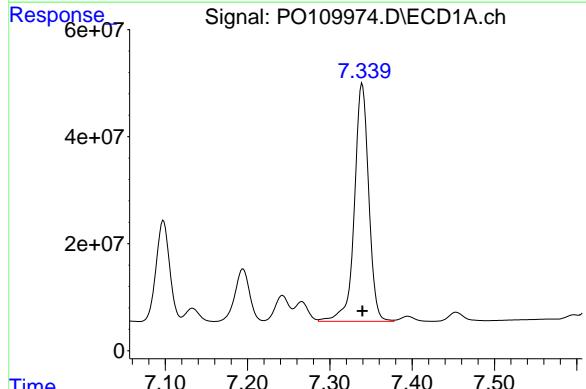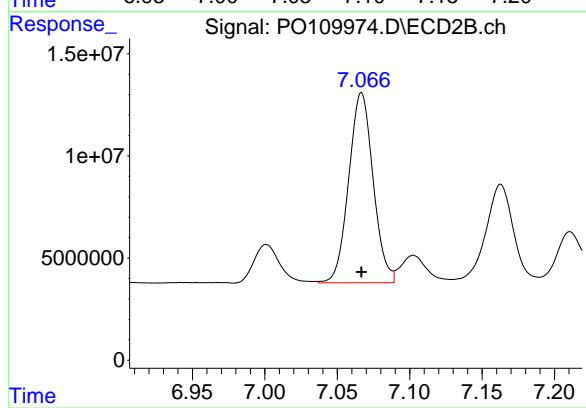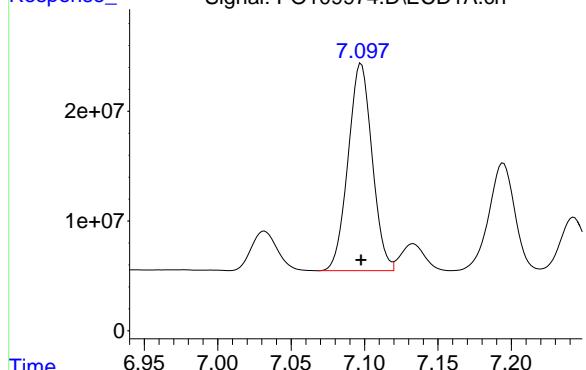

#34 AR-1260-4

R.T.: 7.067 min  
 Delta R.T.: 0.000 min  
 Response: 109147436  
 Conc: 500.00 ng/ml

#35 AR-1260-5

R.T.: 7.339 min  
 Delta R.T.: 0.000 min  
 Response: 538302683  
 Conc: 500.00 ng/ml

#35 AR-1260-5

R.T.: 7.307 min  
 Delta R.T.: 0.000 min  
 Response: 256891434  
 Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109975.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:58  
 Operator : YP/AJ  
 Sample : AR1660ICC250  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1660ICC250

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:39:25 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	233.8E6	137.9E6	24.929	25.476
2) SA Decachlor...	8.745	8.696	201.6E6	65500844	26.286	27.163

Target Compounds

3) L1 AR-1016-1	4.785	4.772	88646972	48746375	263.699	265.987
4) L1 AR-1016-2	4.804	4.791	123.1E6	69074645	262.197	261.121
5) L1 AR-1016-3	4.861	4.967	85428739	37541292	268.076	264.759
6) L1 AR-1016-4	4.981	5.009	67025370	31466909	264.908	270.924
7) L1 AR-1016-5	5.239	5.222	72404369	40645243	269.031	268.512
31) L7 AR-1260-1	6.280	6.254	125.2E6	68345949	264.643	268.013
32) L7 AR-1260-2	6.469	6.441	151.2E6	78966840	262.745	265.904
33) L7 AR-1260-3	6.837	6.594	126.6E6	76461934	260.615	268.065
34) L7 AR-1260-4	7.097	7.066	113.3E6	57323009	267.737	270.080
35) L7 AR-1260-5	7.339	7.307	272.1E6	130.2E6	254.883	260.615



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109975.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:58  
 Operator : YP/AJ  
 Sample : AR1660ICC250  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:39:25 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

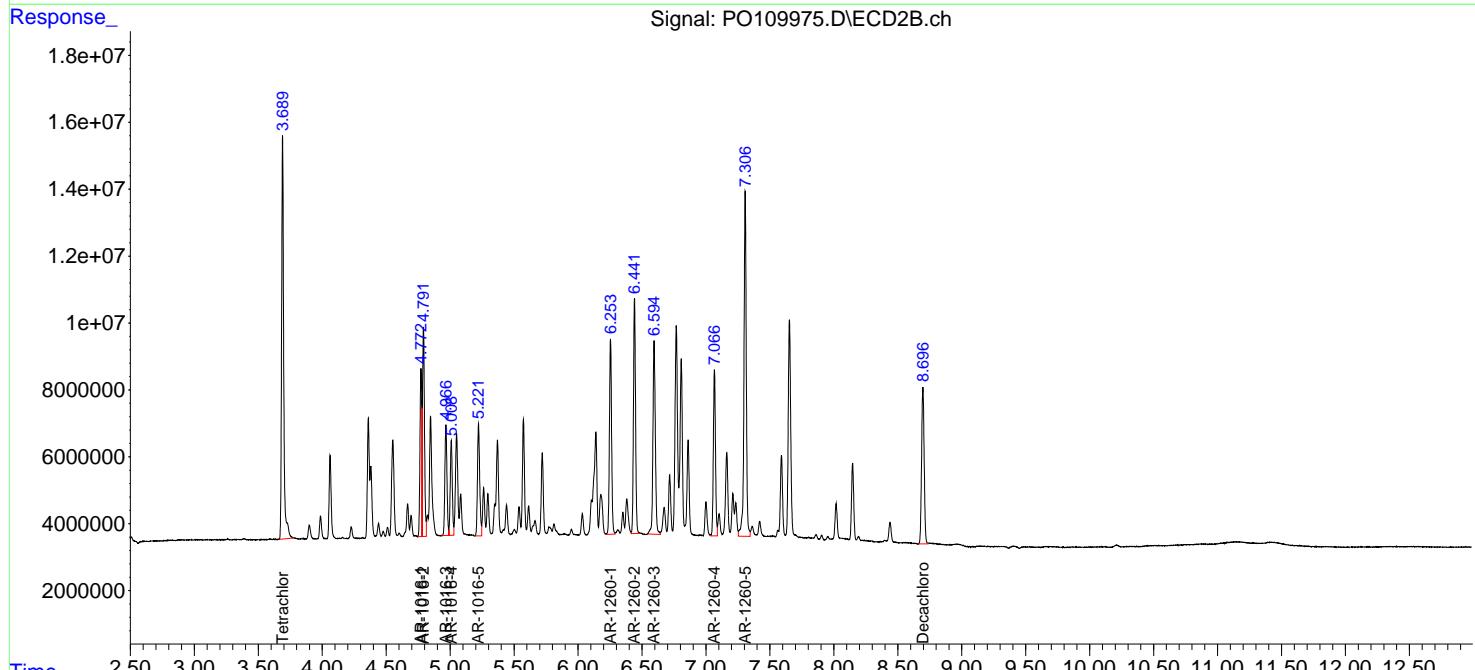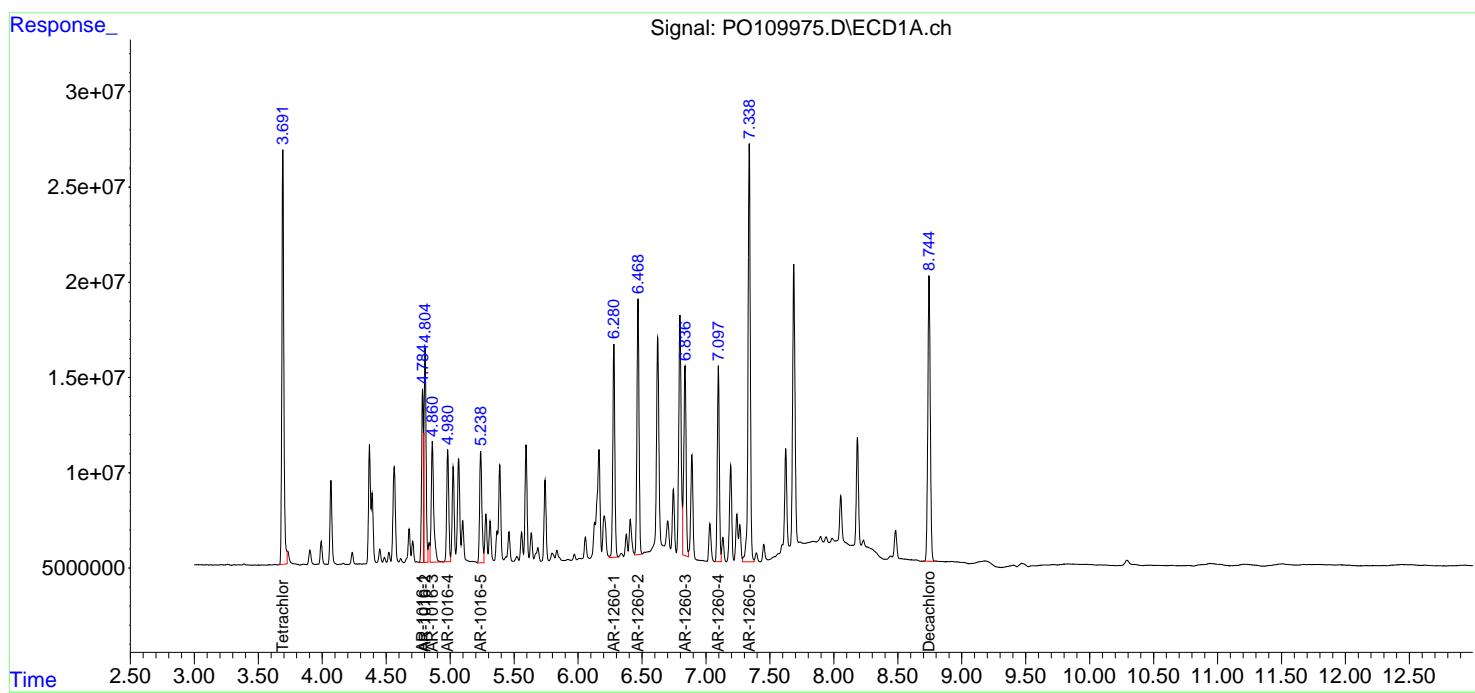

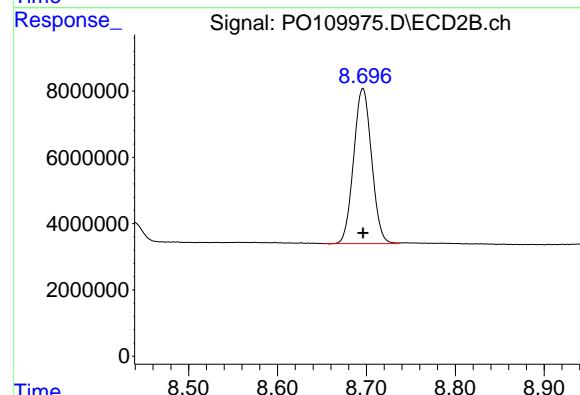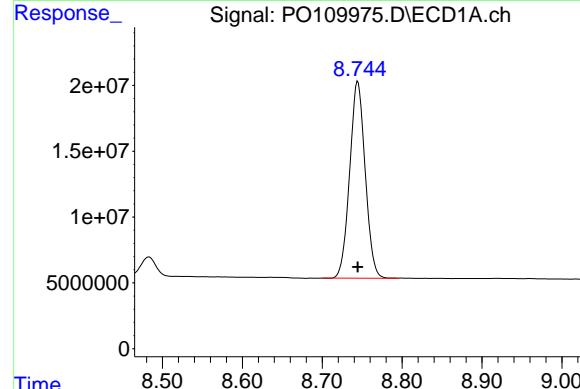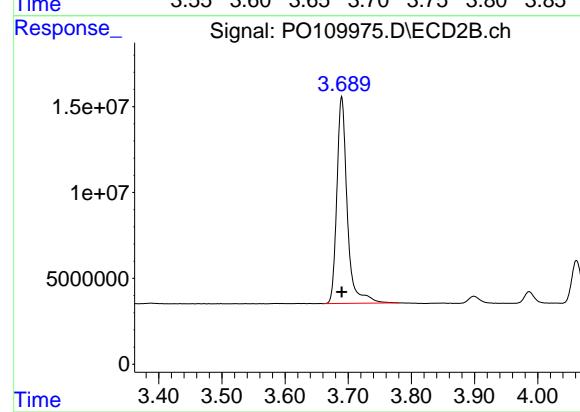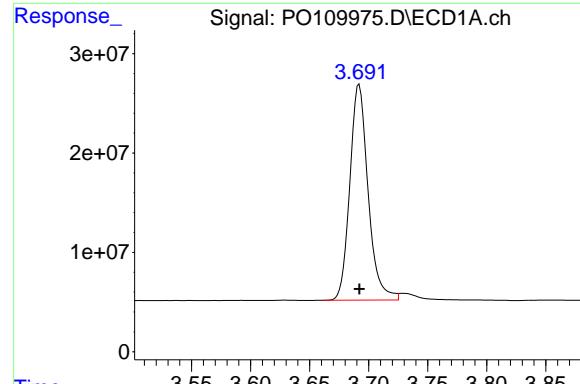

#1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 233755001  
Conc: 24.93 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1660ICC250

#1 Tetrachloro-m-xylene





R.T.: 3.690 min  
Delta R.T.: 0.000 min  
Response: 137920449  
Conc: 25.48 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.745 min  
Delta R.T.: 0.000 min  
Response: 201609663  
Conc: 26.29 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 65500844  
Conc: 27.16 ng/ml

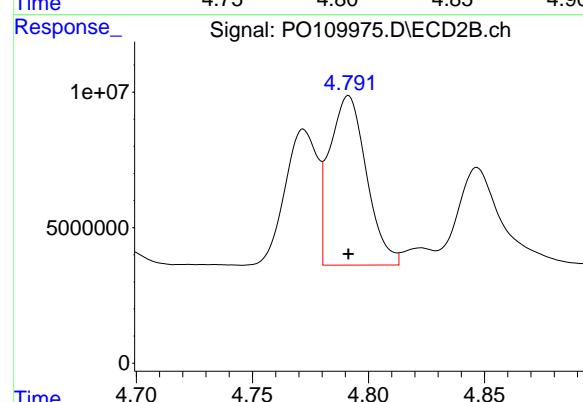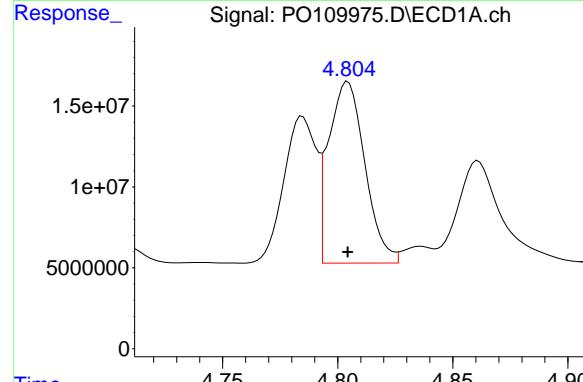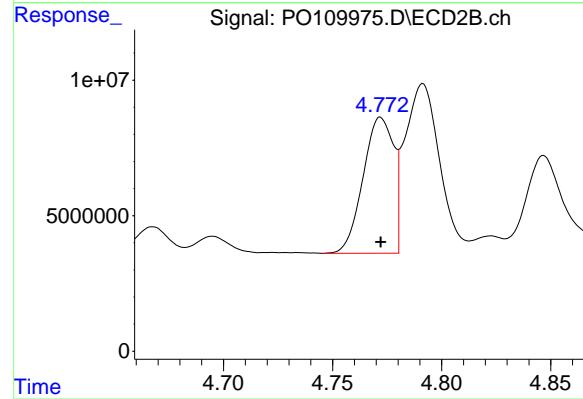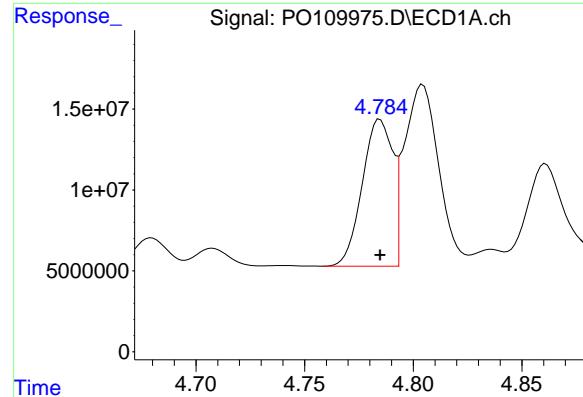

#3 AR-1016-1

R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 88646972  
 Conc: 263.70 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC250

#3 AR-1016-1

R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 48746375  
 Conc: 265.99 ng/ml

#4 AR-1016-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 123072474  
 Conc: 262.20 ng/ml


#4 AR-1016-2

R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 69074645  
 Conc: 261.12 ng/ml

#5 AR-1016-3


R.T.: 4.861 min  
 Delta R.T.: 0.000 min  
 Response: 85428739  
 Conc: 268.08 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC250

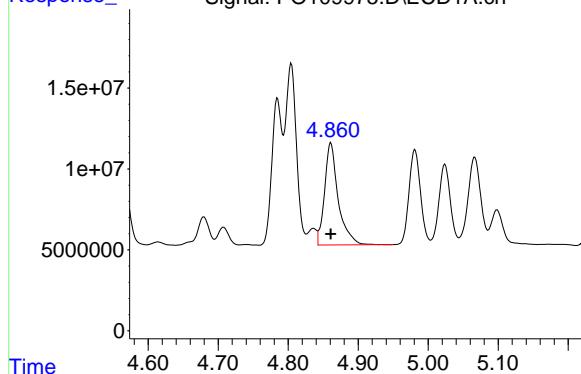


#5 AR-1016-3

R.T.: 4.967 min  
 Delta R.T.: 0.000 min  
 Response: 37541292  
 Conc: 264.76 ng/ml

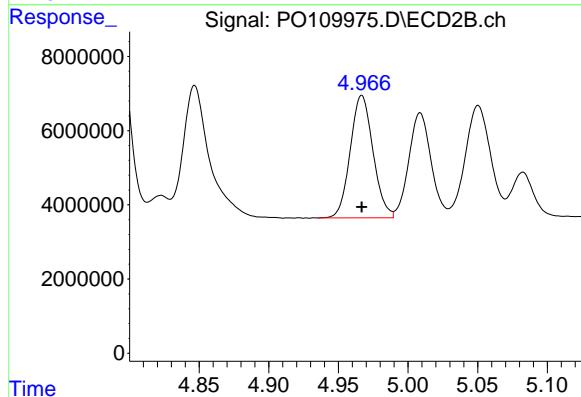


#6 AR-1016-4


R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 67025370  
 Conc: 264.91 ng/ml

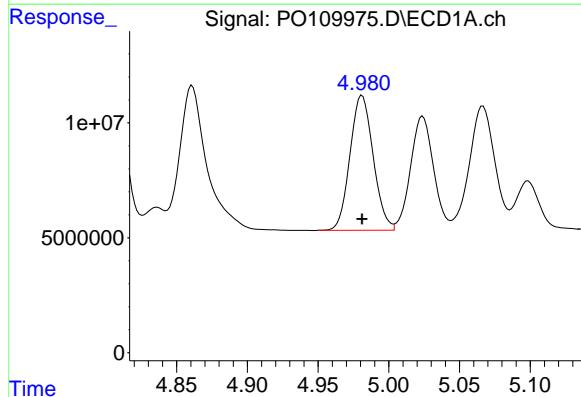

#6 AR-1016-4

R.T.: 5.009 min  
 Delta R.T.: 0.000 min  
 Response: 31466909  
 Conc: 270.92 ng/ml

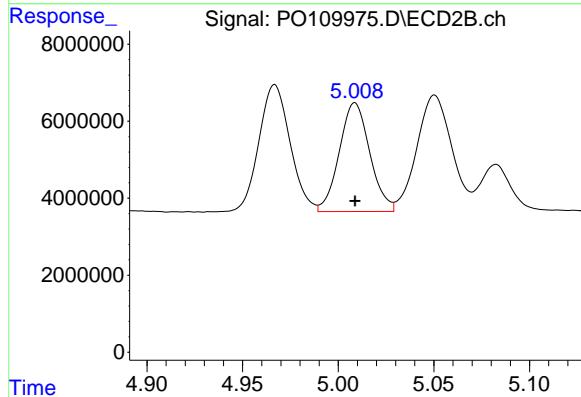

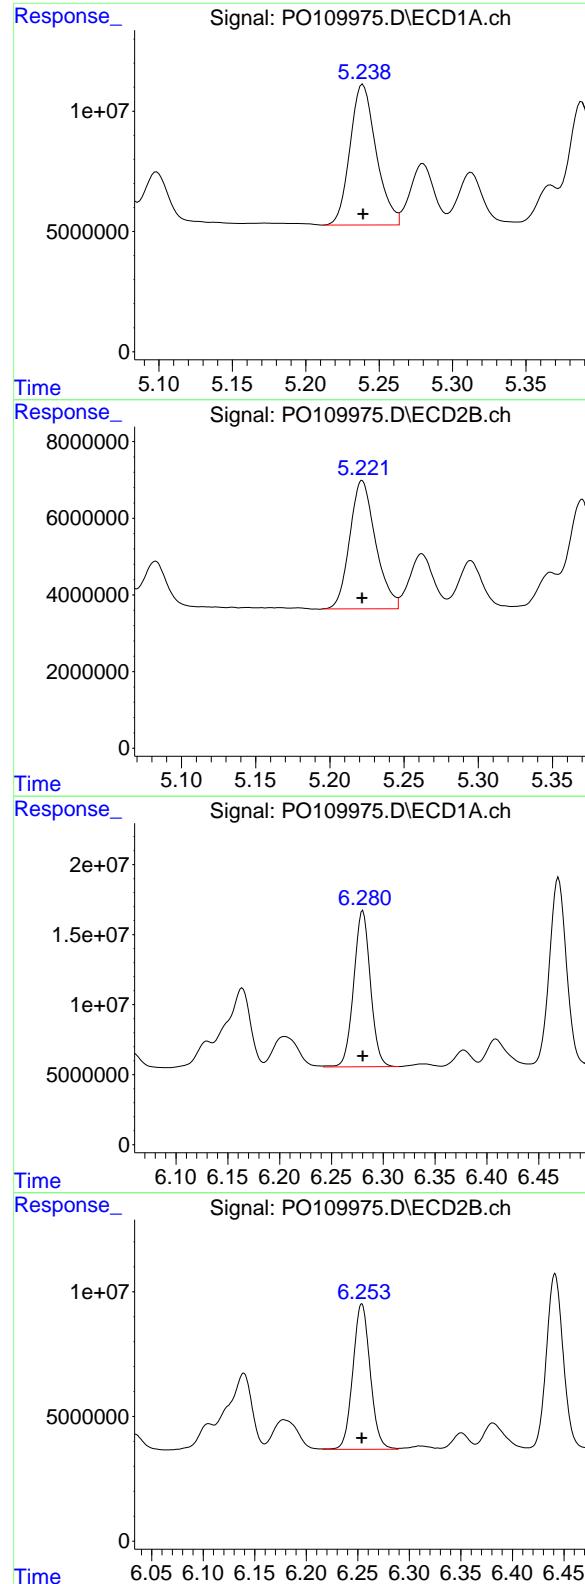

#7 AR-1016-5

R.T.: 5.239 min  
 Delta R.T.: 0.000 min  
 Response: 72404369  
 Conc: 269.03 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC250

#7 AR-1016-5

R.T.: 5.222 min  
 Delta R.T.: 0.000 min  
 Response: 40645243  
 Conc: 268.51 ng/ml

#31 AR-1260-1

R.T.: 6.280 min  
 Delta R.T.: 0.000 min  
 Response: 125236229  
 Conc: 264.64 ng/ml





#31 AR-1260-1

R.T.: 6.254 min  
 Delta R.T.: 0.000 min  
 Response: 68345949  
 Conc: 268.01 ng/ml

#32 AR-1260-2

R.T.: 6.469 min  
 Delta R.T.: 0.000 min  
 Response: 151225079  
 Conc: 262.75 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC250

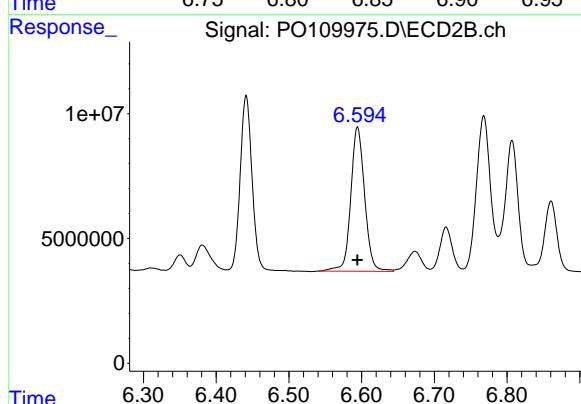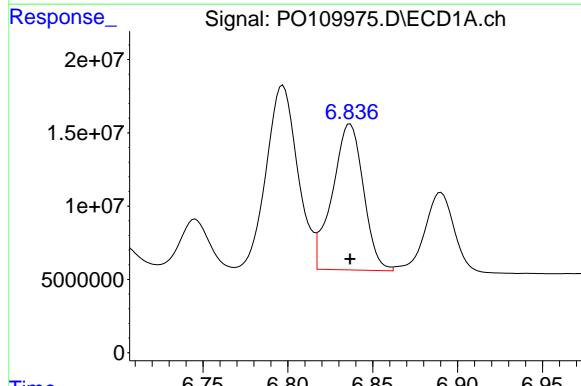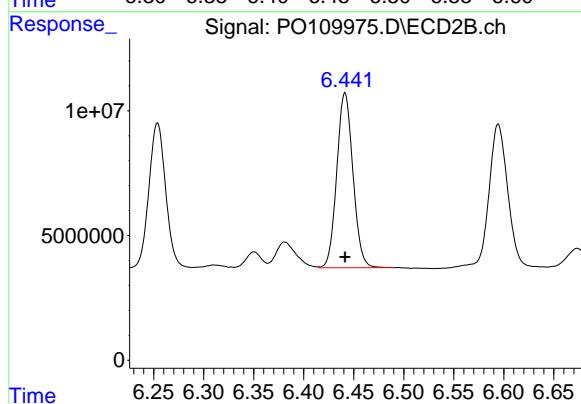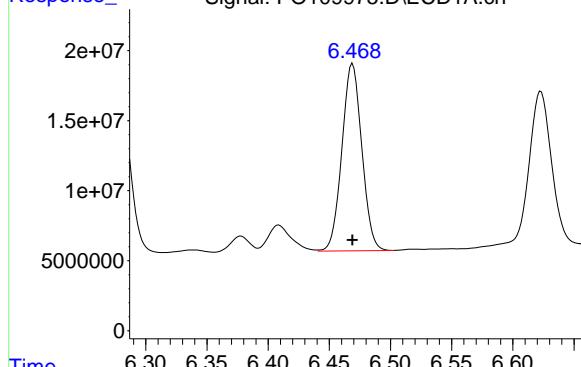

#32 AR-1260-2

R.T.: 6.441 min  
 Delta R.T.: 0.000 min  
 Response: 78966840  
 Conc: 265.90 ng/ml

#33 AR-1260-3

R.T.: 6.837 min  
 Delta R.T.: 0.000 min  
 Response: 126558412  
 Conc: 260.61 ng/ml





#33 AR-1260-3

R.T.: 6.594 min  
 Delta R.T.: 0.000 min  
 Response: 76461934  
 Conc: 268.07 ng/ml

#34 AR-1260-4

R.T.: 7.097 min  
 Delta R.T.: 0.000 min  
 Response: 113264613  
 Conc: 267.74 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC250

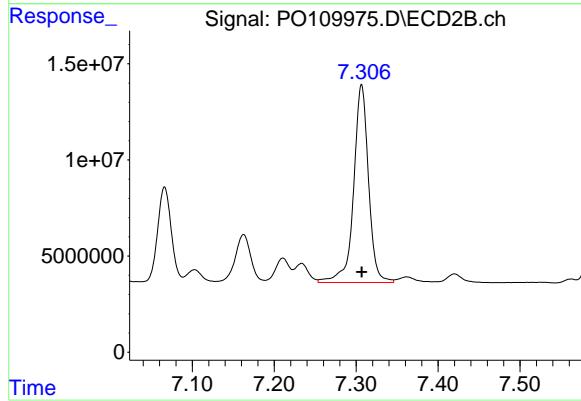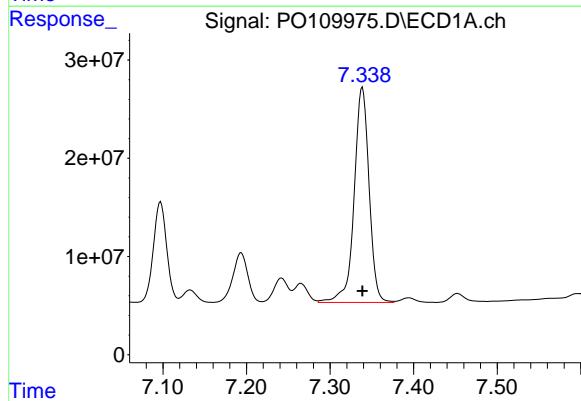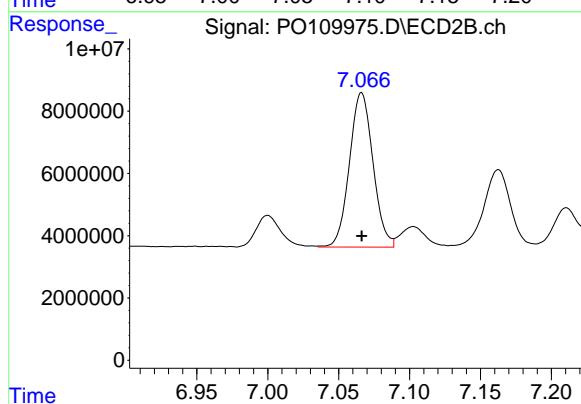

#34 AR-1260-4

R.T.: 7.066 min  
 Delta R.T.: 0.000 min  
 Response: 57323009  
 Conc: 270.08 ng/ml

#35 AR-1260-5

R.T.: 7.339 min  
 Delta R.T.: 0.000 min  
 Response: 272092445  
 Conc: 254.88 ng/ml

#35 AR-1260-5

R.T.: 7.307 min  
 Delta R.T.: 0.000 min  
 Response: 130197884  
 Conc: 260.61 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109976.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 15:16  
 Operator : YP/AJ  
 Sample : AR1660ICC050  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:42:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.688	39998137	22828400	4.395	4.353
2) SA Decachlor...	8.744	8.695	38817794	12425222	5.049	5.121

Target Compounds

3) L1 AR-1016-1	4.784	4.771	16902653	9160493	50.224	49.988
4) L1 AR-1016-2	4.804	4.790	22043406	12469957	47.540	47.685
5) L1 AR-1016-3	4.860	4.965	16411868	7085785	51.193	49.978
6) L1 AR-1016-4	4.981	5.008	12569483	6253080	49.743	53.024
7) L1 AR-1016-5	5.238	5.220	14890720	7955288	54.174	52.023
31) L7 AR-1260-1	6.278	6.252	23192253	12858546	48.956m	50.252m
32) L7 AR-1260-2	6.468	6.441	33768251	15676301	56.704	52.205
33) L7 AR-1260-3	6.836	6.593	24202394	15198300	49.871	53.072m
34) L7 AR-1260-4	7.096	7.065	21433117	11320638	50.530	52.635
35) L7 AR-1260-5	7.339	7.306	47957612	24758089	45.855	49.646

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109976.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 15:16  
 Operator : YP/AJ  
 Sample : AR1660ICC050  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:42:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

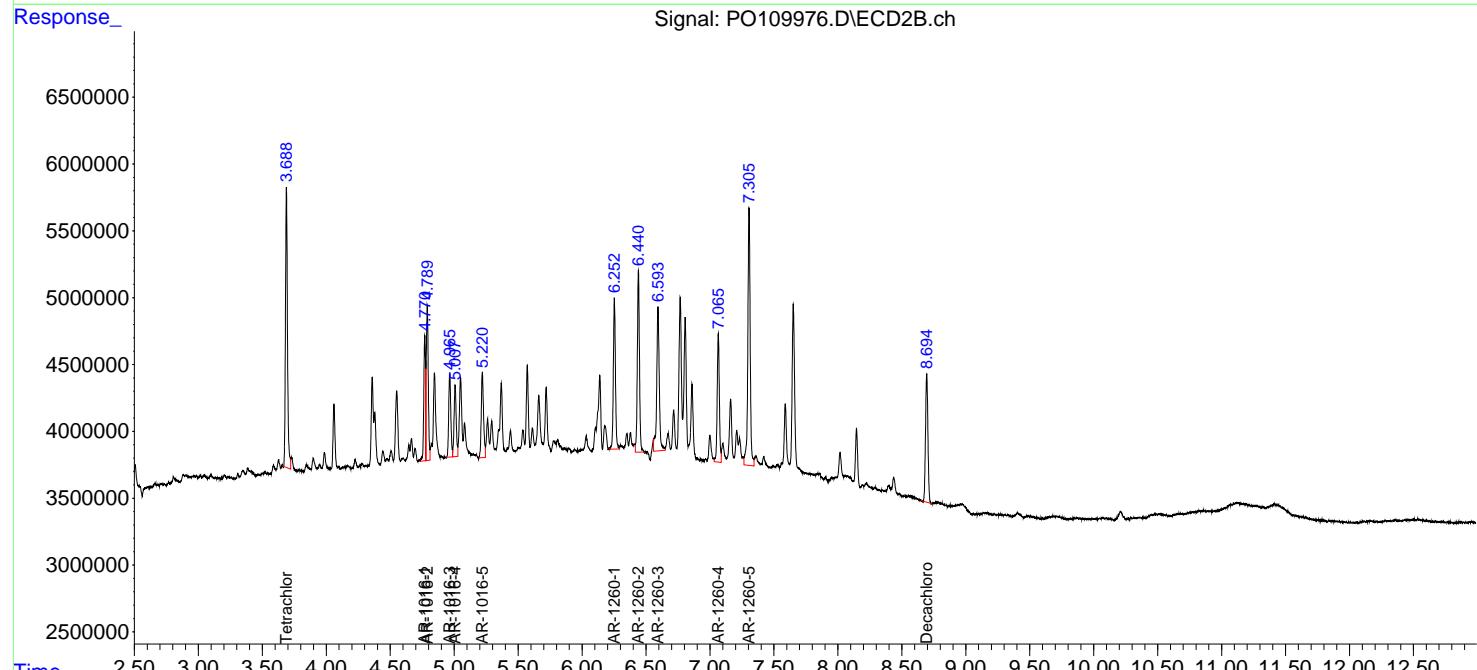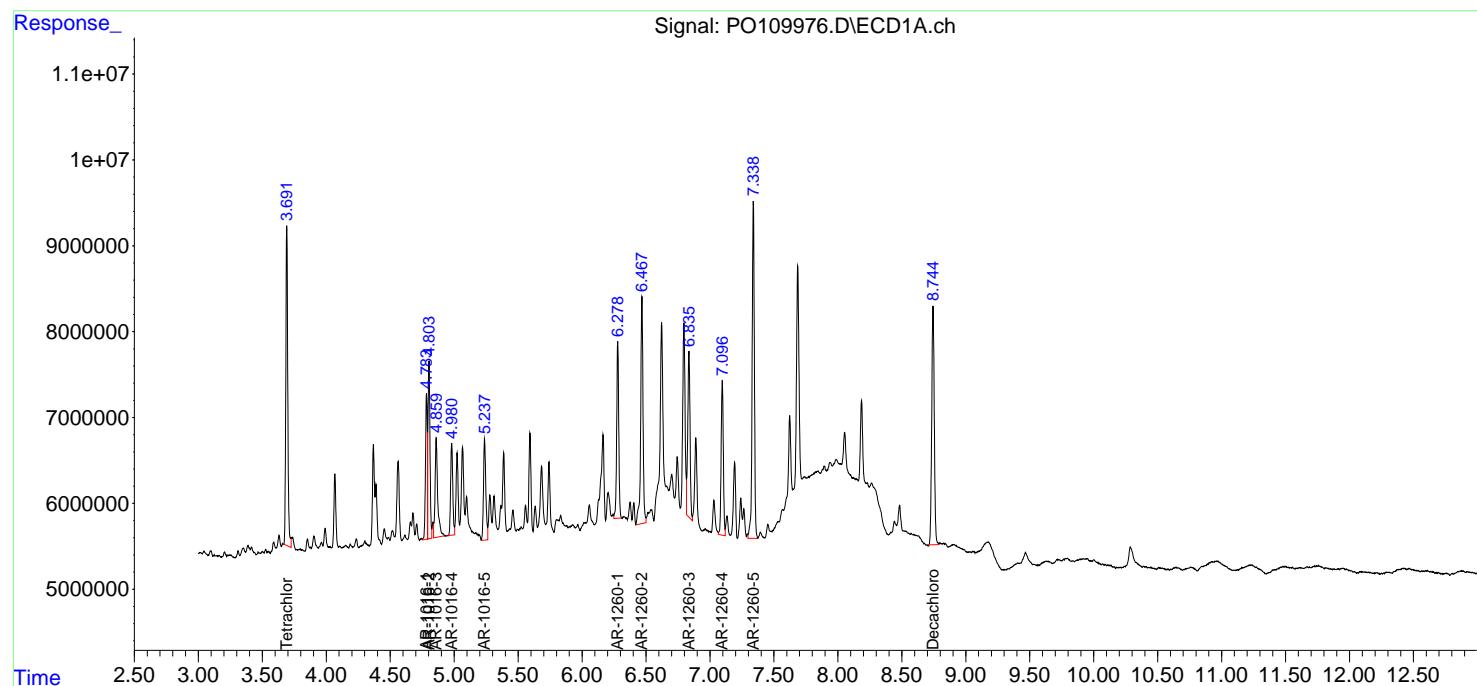

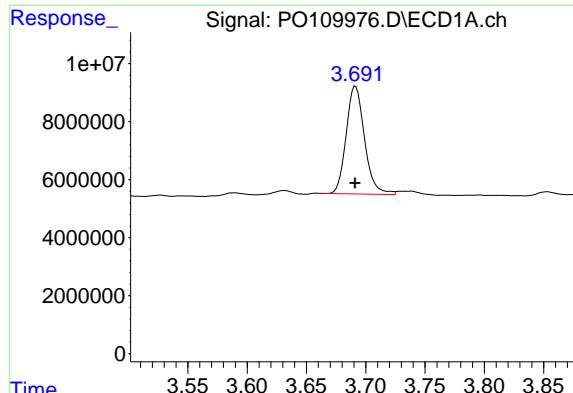


## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
Delta R.T.: 0.000 min  
Response: 39998137  
Conc: 4.39 ng/ml

**Instrument:**  
ECD\_O  
**ClientSampleId :**  
AR1660ICC050


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

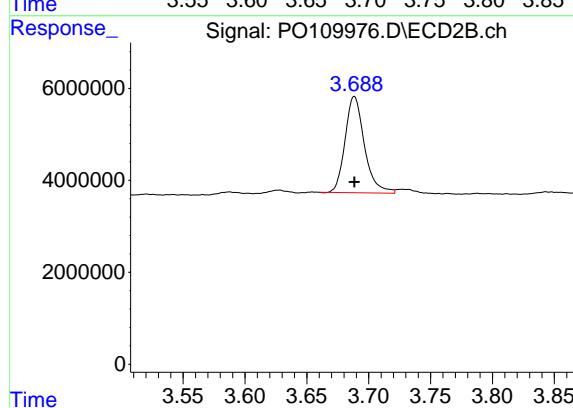


## #1 Tetrachloro-m-xylene

R.T.: 3.688 min  
Delta R.T.: 0.000 min  
Response: 22828400  
Conc: 4.35 ng/ml

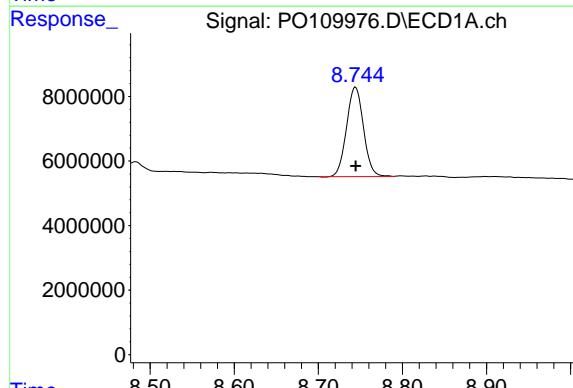

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 38817794  
Conc: 5.05 ng/ml

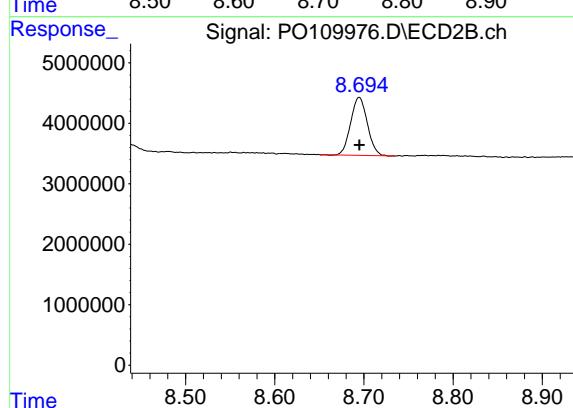

## #2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 12425222  
Conc: 5.12 ng/ml

#3 AR-1016-1

R.T.: 4.784 min  
 Delta R.T.: 0.000 min  
 Response: 16902653  
 Conc: 50.22 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#3 AR-1016-1





R.T.: 4.771 min  
 Delta R.T.: 0.000 min  
 Response: 9160493  
 Conc: 49.99 ng/ml


#4 AR-1016-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 22043406  
 Conc: 47.54 ng/ml

#4 AR-1016-2

R.T.: 4.790 min  
 Delta R.T.: 0.000 min  
 Response: 12469957  
 Conc: 47.69 ng/ml

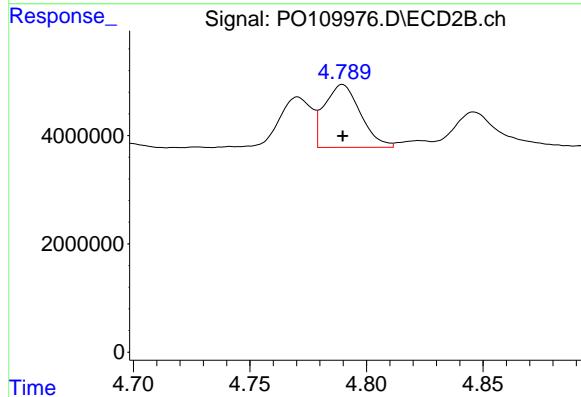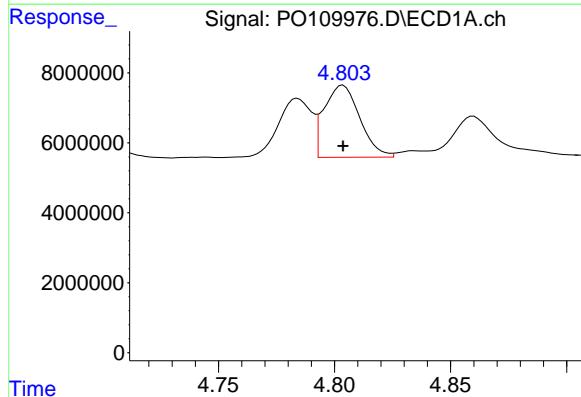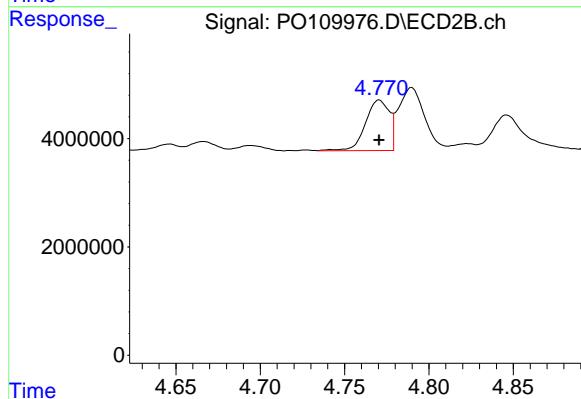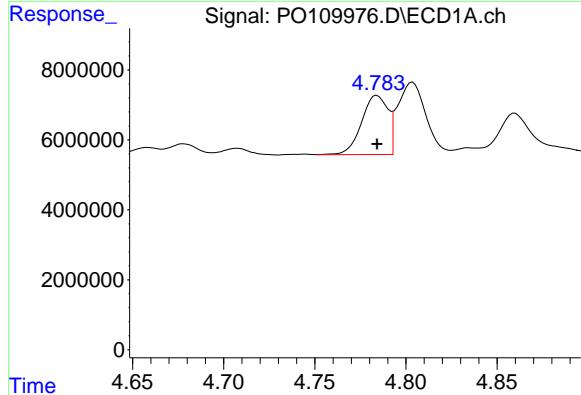

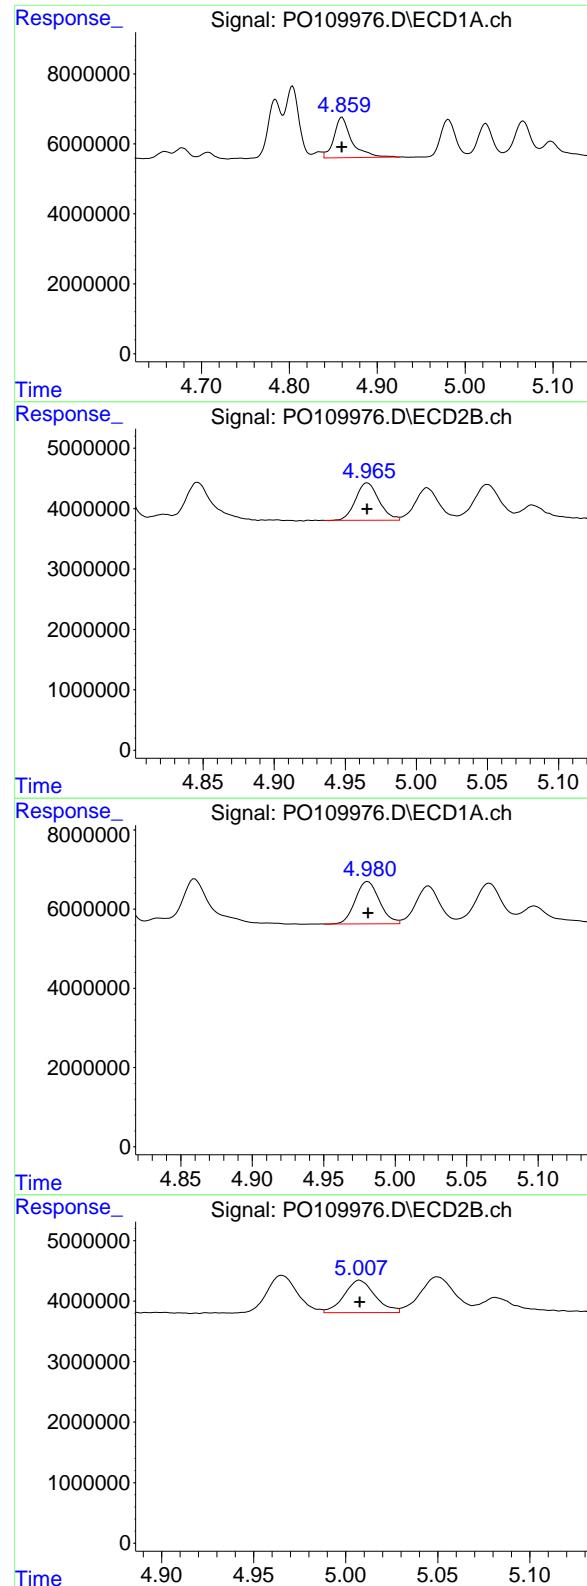

#5 AR-1016-3

R.T.: 4.860 min  
 Delta R.T.: 0.000 min  
 Response: 16411868  
 Conc: 51.19 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#5 AR-1016-3


R.T.: 4.965 min  
 Delta R.T.: 0.000 min  
 Response: 7085785  
 Conc: 49.98 ng/ml

#6 AR-1016-4

R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 12569483  
 Conc: 49.74 ng/ml

#6 AR-1016-4

R.T.: 5.008 min  
 Delta R.T.: 0.000 min  
 Response: 6253080  
 Conc: 53.02 ng/ml

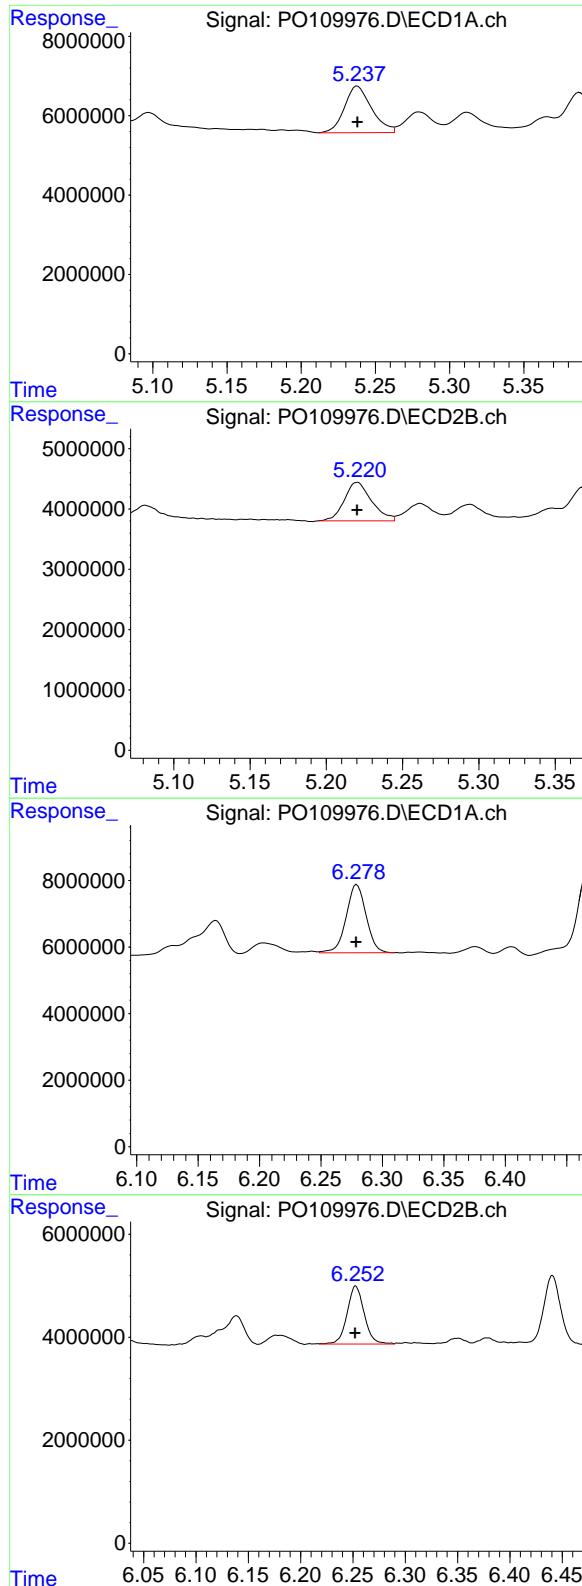

#7 AR-1016-5

R.T.: 5.238 min  
 Delta R.T.: 0.000 min  
 Response: 14890720  
 Conc: 54.17 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#7 AR-1016-5


R.T.: 5.220 min  
 Delta R.T.: 0.000 min  
 Response: 7955288  
 Conc: 52.02 ng/ml

#31 AR-1260-1

R.T.: 6.278 min  
 Delta R.T.: 0.000 min  
 Response: 23192253  
 Conc: 48.96 ng/ml

#31 AR-1260-1

R.T.: 6.252 min  
 Delta R.T.: 0.000 min  
 Response: 12858546  
 Conc: 50.25 ng/ml

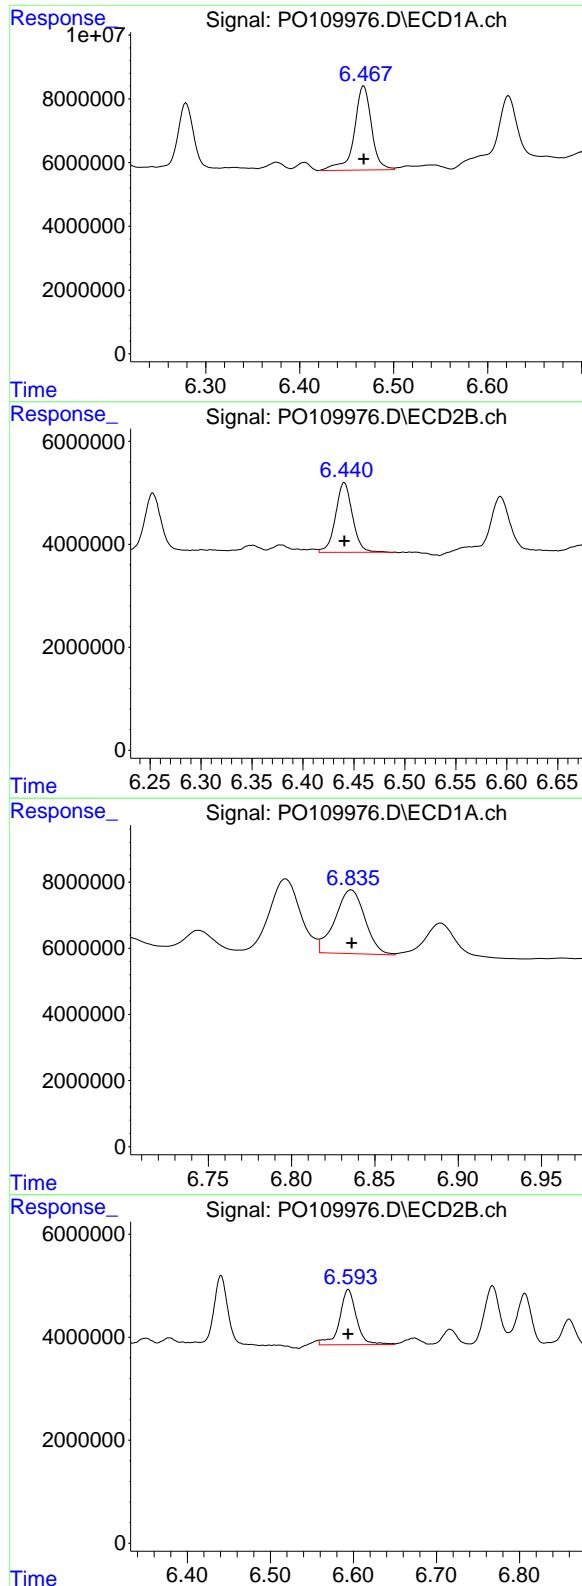

#32 AR-1260-2

R.T.: 6.468 min  
 Delta R.T.: 0.000 min  
 Response: 33768251  
 Conc: 56.70 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#32 AR-1260-2

R.T.: 6.441 min  
 Delta R.T.: 0.000 min  
 Response: 15676301  
 Conc: 52.20 ng/ml

#33 AR-1260-3

R.T.: 6.836 min  
 Delta R.T.: 0.000 min  
 Response: 24202394  
 Conc: 49.87 ng/ml

#33 AR-1260-3

R.T.: 6.593 min  
 Delta R.T.: 0.000 min  
 Response: 15198300  
 Conc: 53.07 ng/ml

#34 AR-1260-4

R.T.: 7.096 min  
 Delta R.T.: 0.000 min  
 Response: 21433117  
 Conc: 50.53 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#34 AR-1260-4





R.T.: 7.065 min  
 Delta R.T.: 0.000 min  
 Response: 11320638  
 Conc: 52.63 ng/ml

#35 AR-1260-5

R.T.: 7.339 min  
 Delta R.T.: 0.000 min  
 Response: 47957612  
 Conc: 45.86 ng/ml

#35 AR-1260-5

R.T.: 7.306 min  
 Delta R.T.: 0.000 min  
 Response: 24758089  
 Conc: 49.65 ng/ml

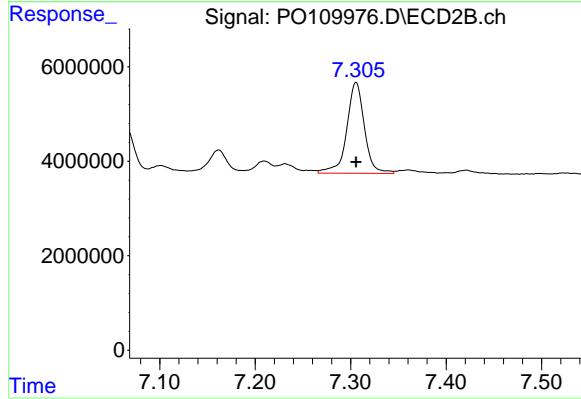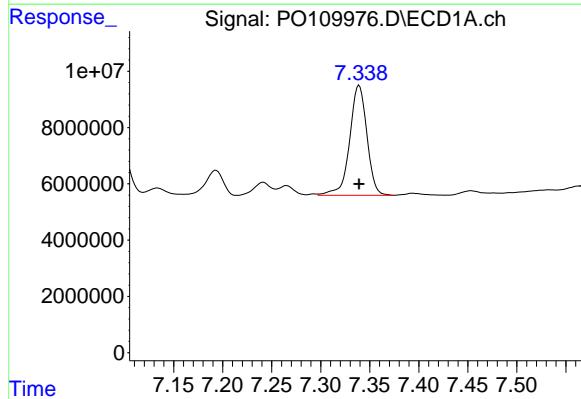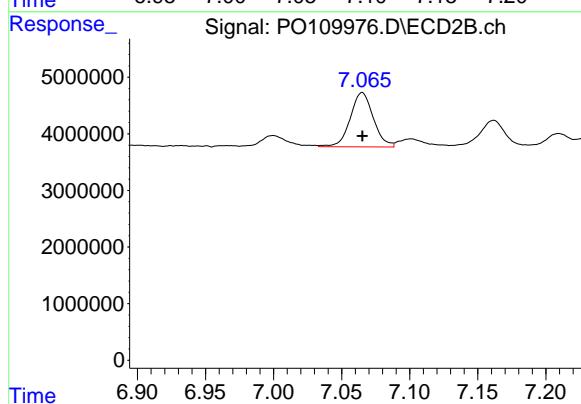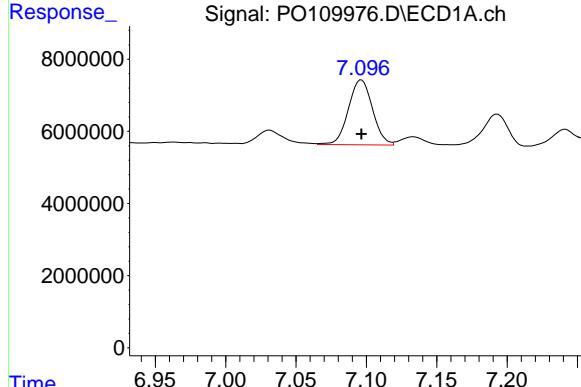

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109977.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 15:34  
 Operator : YP/AJ  
 Sample : AR1221ICC500  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1221ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:27:37 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:27:26 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	428.4E6	261.3E6	50.000	50.000
2) SA Decachlor...	8.743	8.696	367.0E6	116.0E6	50.000	50.000

Target Compounds

8) L2 AR-1221-1	3.906	3.901	57914123	33441082	500.000	500.000
9) L2 AR-1221-2	3.992	3.986	43249856	24690825	500.000	500.000
10) L2 AR-1221-3	4.069	4.062	130.8E6	75841971	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109977.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 15:34  
 Operator : YP/AJ  
 Sample : AR1221ICC500  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1221ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:27:37 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:27:26 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

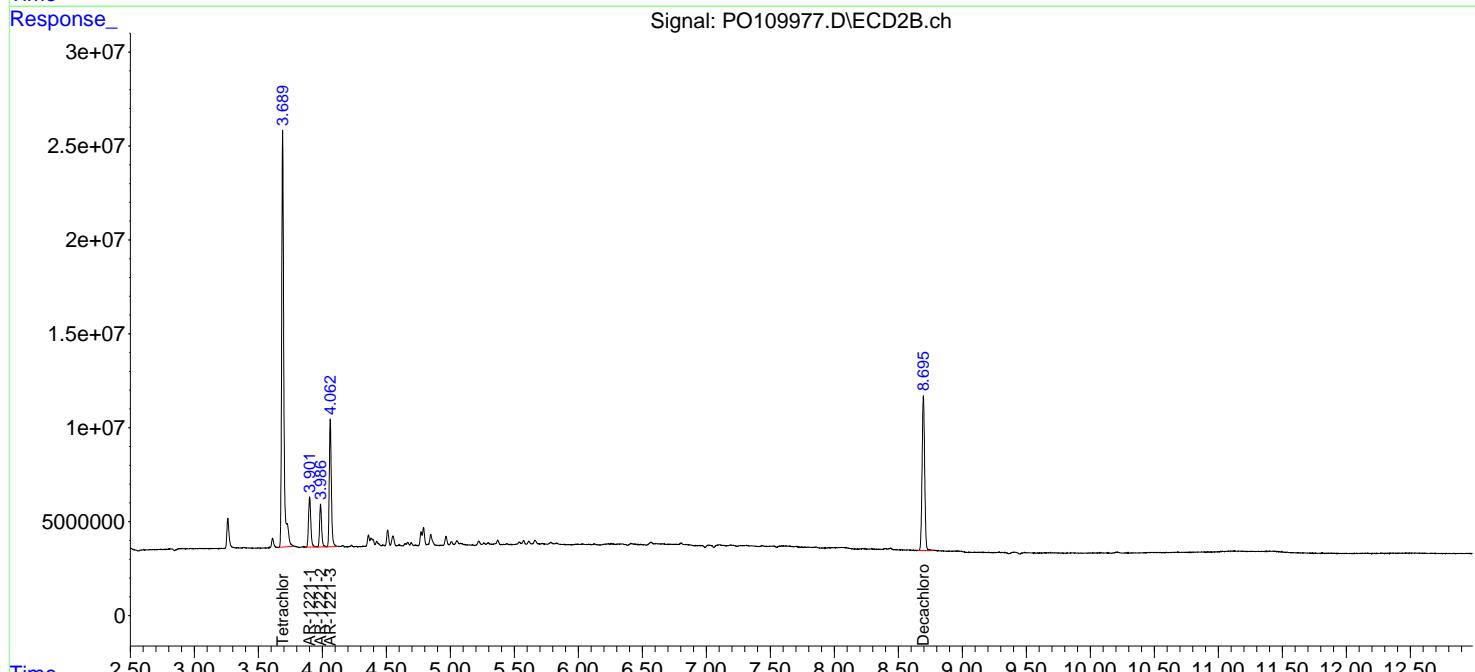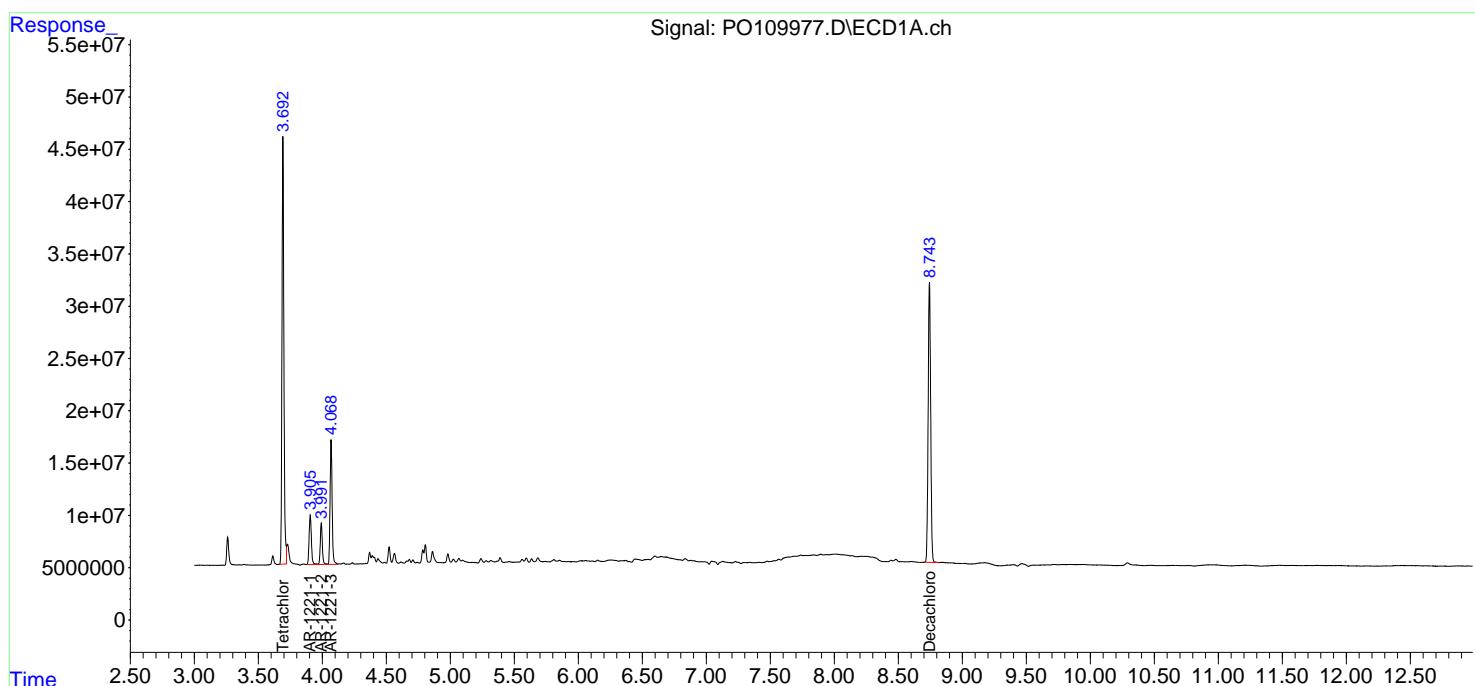

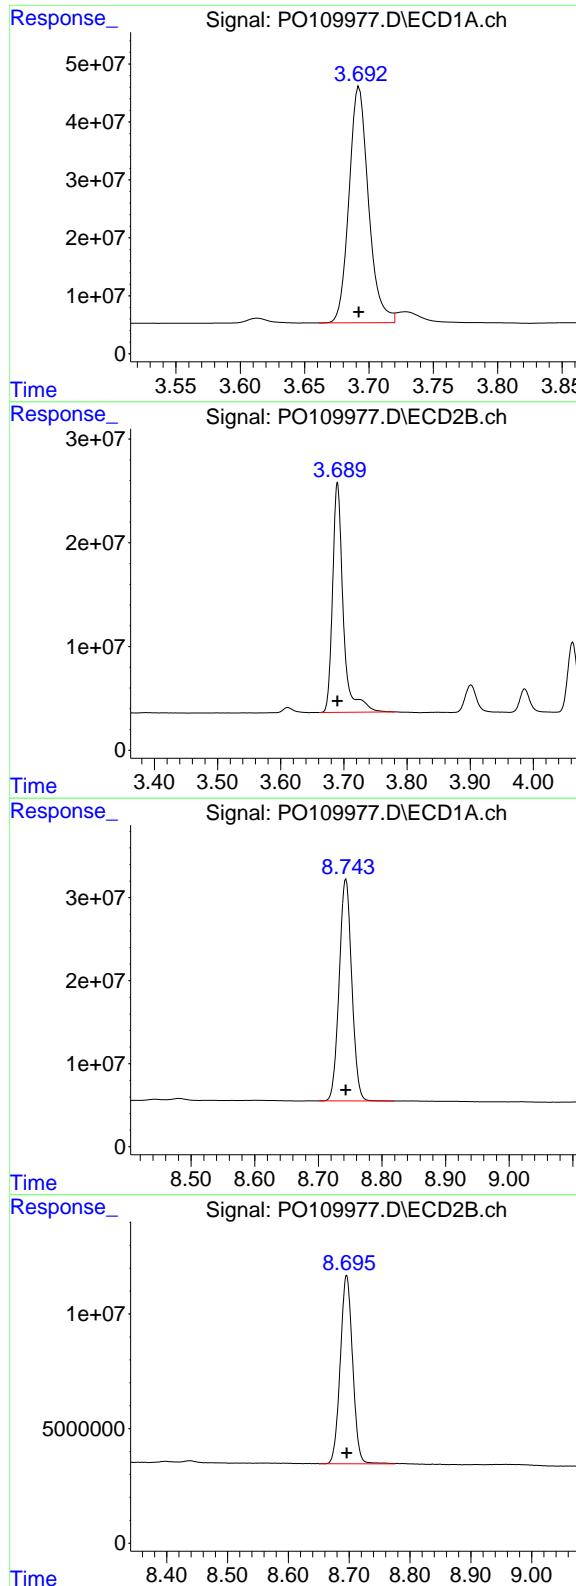

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
 Delta R.T.: 0.000 min  
 Response: 428446750  
 Conc: 50.00 ng/ml

Instrument:

ECD\_O

ClientSampleId :

AR1221ICC500

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: 0.000 min  
 Response: 261250272  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl


R.T.: 8.743 min  
 Delta R.T.: 0.000 min  
 Response: 367001269  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.696 min  
 Delta R.T.: 0.000 min  
 Response: 115987092  
 Conc: 50.00 ng/ml


#8 AR-1221-1

R.T.: 3.906 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 57914123 ECD\_O  
 Conc: 500.00 ng/ml **ClientSampleId:**  
 AR1221ICC500

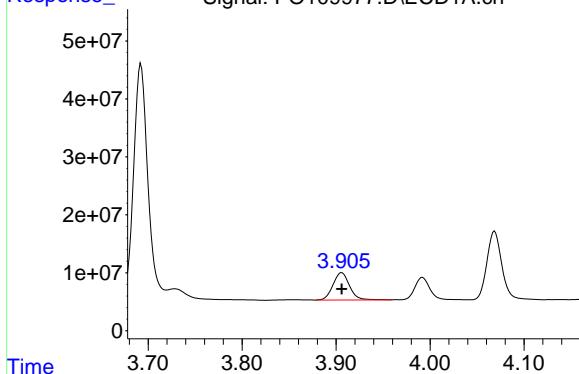


#8 AR-1221-1

R.T.: 3.901 min  
 Delta R.T.: 0.000 min  
 Response: 33441082  
 Conc: 500.00 ng/ml

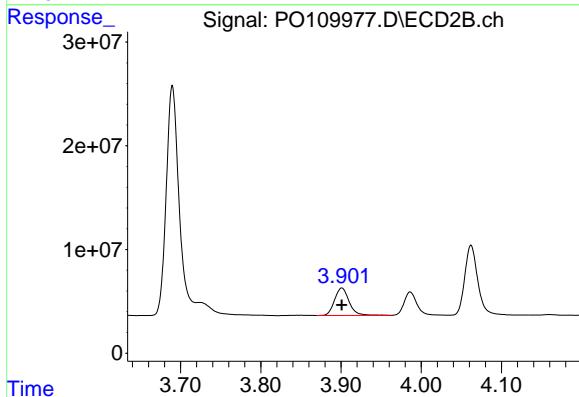


#9 AR-1221-2

R.T.: 3.992 min  
 Delta R.T.: 0.000 min  
 Response: 43249856  
 Conc: 500.00 ng/ml

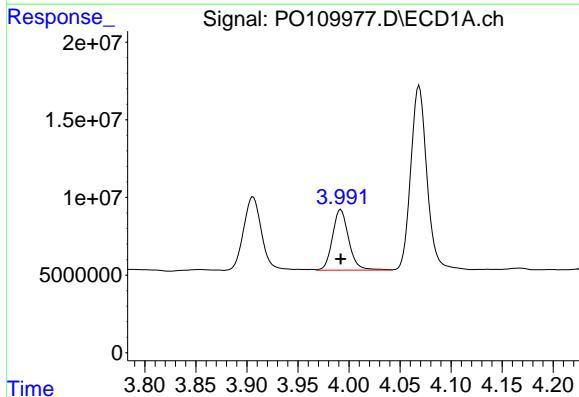



#9 AR-1221-2

R.T.: 3.986 min  
 Delta R.T.: 0.000 min  
 Response: 24690825  
 Conc: 500.00 ng/ml

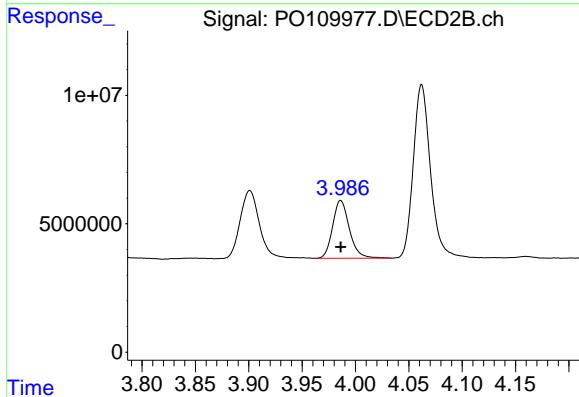

#10 AR-1221-3

R.T.: 4.069 min  
Delta R.T.: 0.000 min **Instrument:**  
Response: 130847955 ECD\_O  
Conc: 500.00 ng/ml **ClientSampleId:**  
AR1221ICC500

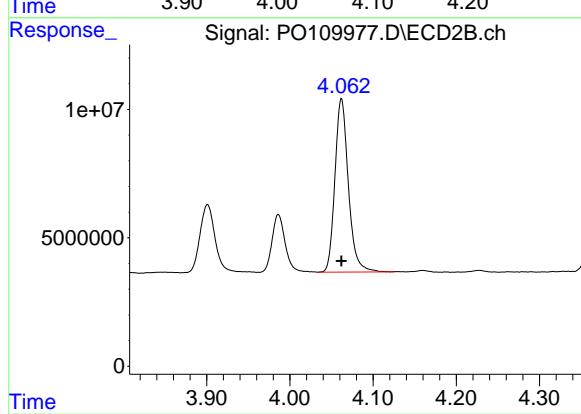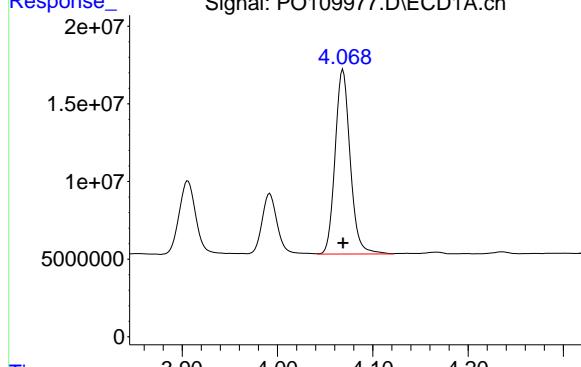

#10 AR-1221-3

R.T.: 4.062 min  
Delta R.T.: 0.000 min  
Response: 75841971  
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109978.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 15:53  
 Operator : YP/AJ  
 Sample : AR1232ICC500  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1232ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:25:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:24:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	438.9E6	262.6E6	50.000	50.000
2) SA Decachlor...	8.744	8.696	372.1E6	116.2E6	50.000	50.000

Target Compounds

11) L3 AR-1232-1	4.068	4.062	107.9E6	62046675	500.000	500.000
12) L3 AR-1232-2	4.563	4.791	57393041	60174277	500.000	500.000
13) L3 AR-1232-3	4.805	4.966	105.9E6	31828000	500.000	500.000
14) L3 AR-1232-4	4.981	5.051	56780516	29670451	500.000	500.000
15) L3 AR-1232-5	5.024	5.221	40226994	31608944	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109978.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 15:53  
 Operator : YP/AJ  
 Sample : AR1232ICC500  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1232ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:25:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:24:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

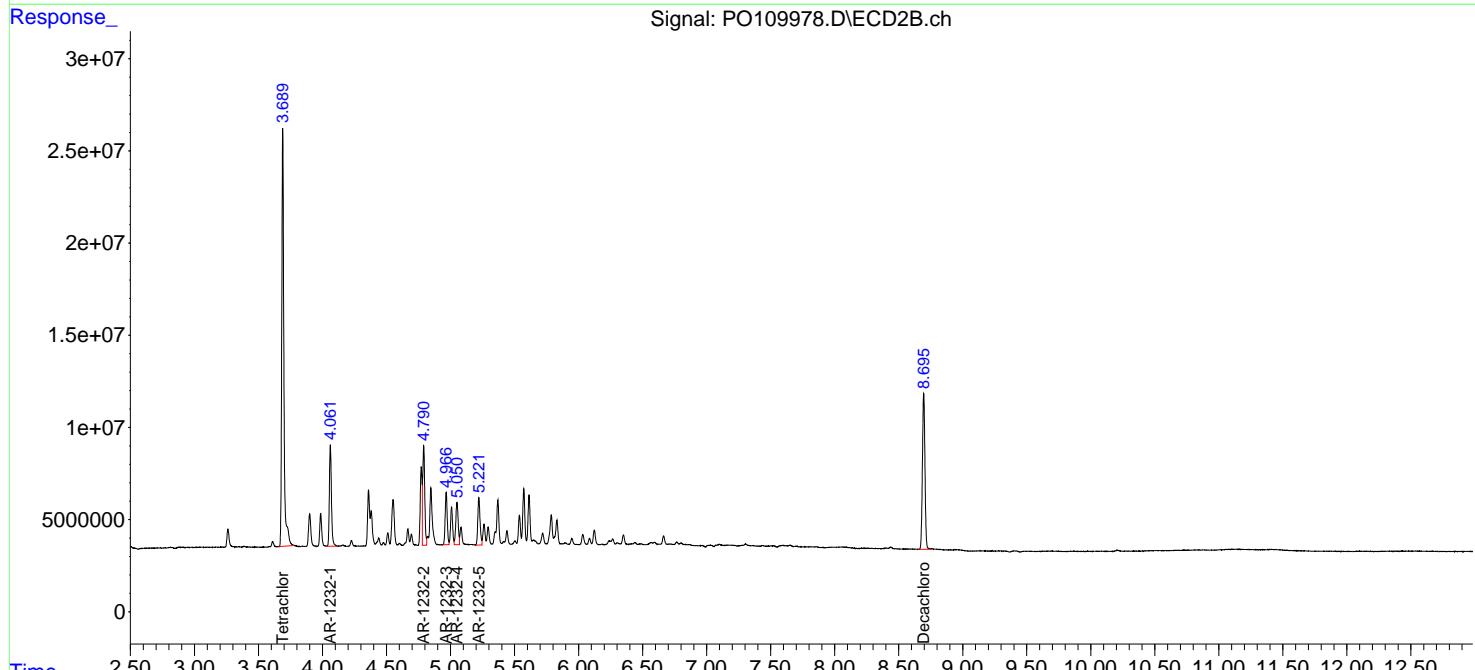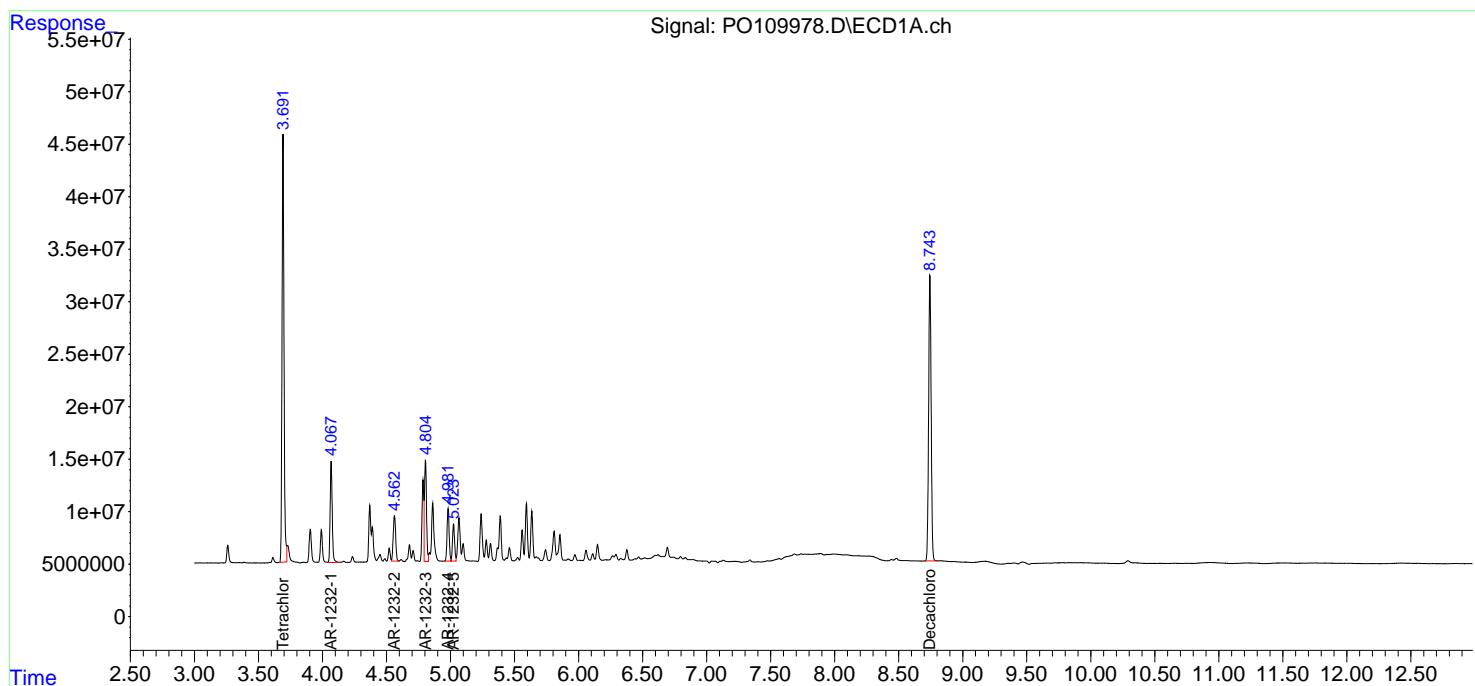

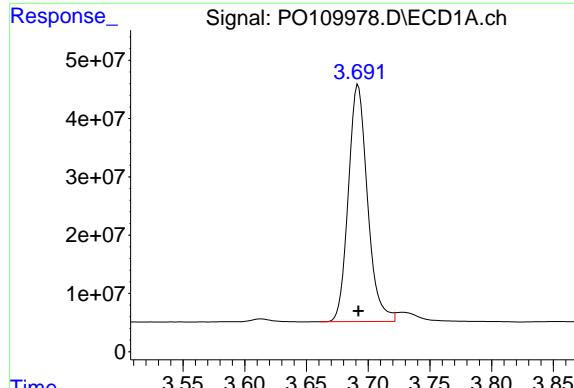

#1 Tetrachloro-m-xylene

R.T.: 3.692 min

Delta R.T.: 0.000 min


Instrument:

Response: 438922587 ECD\_O

Conc: 50.00 ng/ml

ClientSampleId:

AR1232ICC500

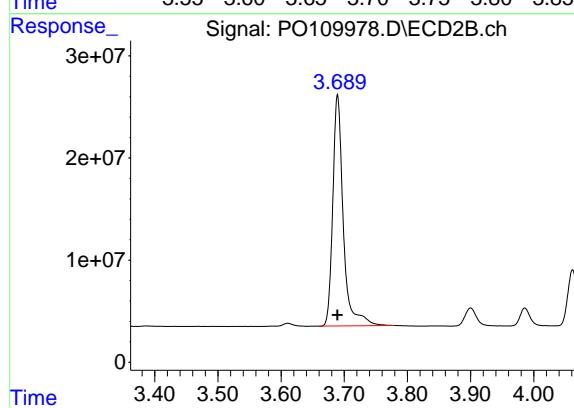


#1 Tetrachloro-m-xylene

R.T.: 3.689 min

Delta R.T.: 0.000 min

Response: 262556927

Conc: 50.00 ng/ml

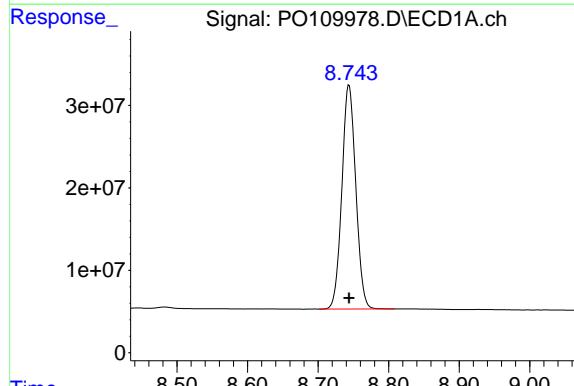


#2 Decachlorobiphenyl

R.T.: 8.744 min

Delta R.T.: 0.000 min

Response: 372070287

Conc: 50.00 ng/ml

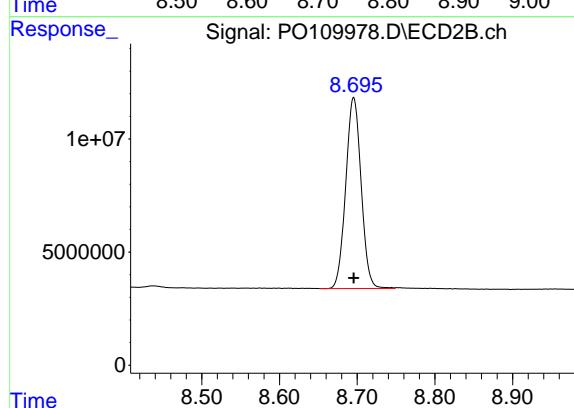

#2 Decachlorobiphenyl

R.T.: 8.696 min

Delta R.T.: 0.000 min


Response: 116151811

Conc: 50.00 ng/ml

#11 AR-1232-1


R.T.: 4.068 min  
 Delta R.T.: 0.000 min  
 Response: 107872261  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1232ICC500

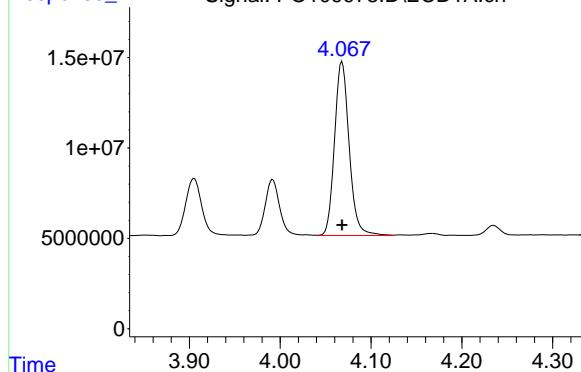


#11 AR-1232-1

R.T.: 4.062 min  
 Delta R.T.: 0.000 min  
 Response: 62046675  
 Conc: 500.00 ng/ml

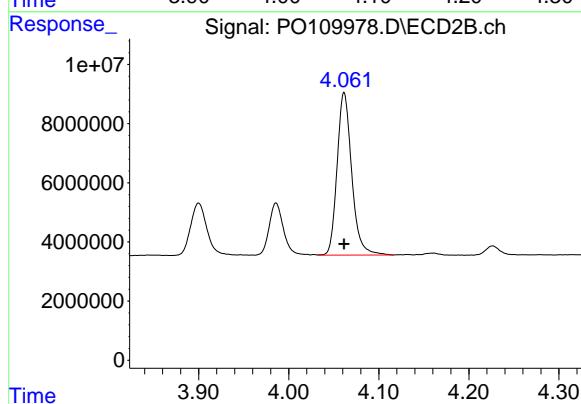


#12 AR-1232-2

R.T.: 4.563 min  
 Delta R.T.: 0.000 min  
 Response: 57393041  
 Conc: 500.00 ng/ml

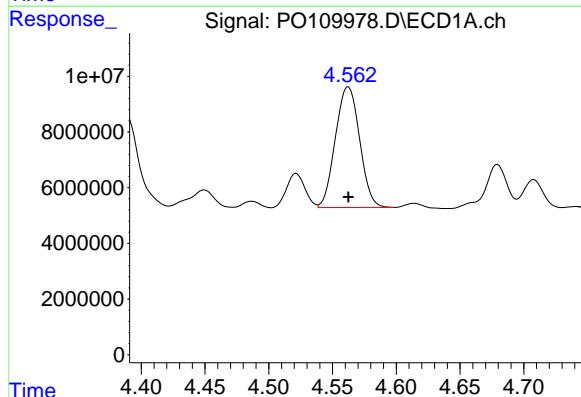

#12 AR-1232-2


R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 60174277  
 Conc: 500.00 ng/ml

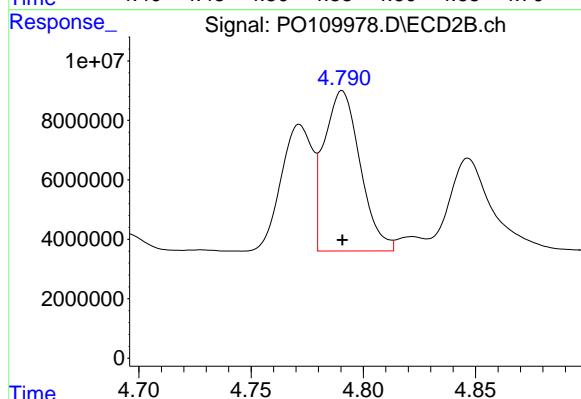

#13 AR-1232-3


R.T.: 4.805 min  
 Delta R.T.: 0.000 min  
 Response: 105889863  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1232ICC500

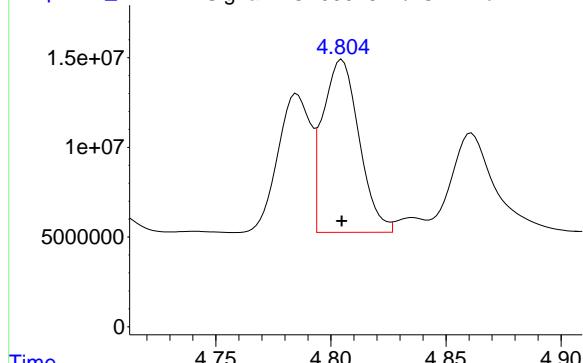


#13 AR-1232-3

R.T.: 4.966 min  
 Delta R.T.: 0.000 min  
 Response: 31828000  
 Conc: 500.00 ng/ml

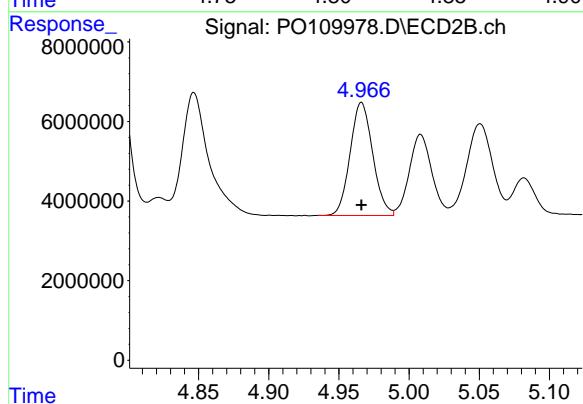


#14 AR-1232-4

R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 56780516  
 Conc: 500.00 ng/ml

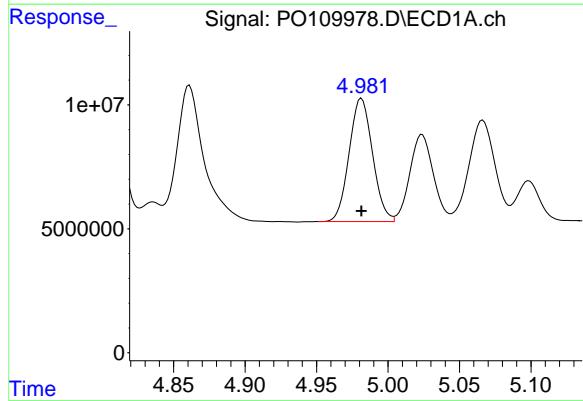

#14 AR-1232-4



R.T.: 5.051 min  
 Delta R.T.: 0.000 min  
 Response: 29670451  
 Conc: 500.00 ng/ml

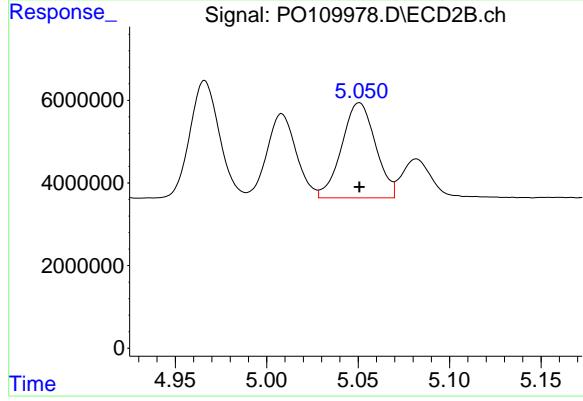

#15 AR-1232-5

R.T.: 5.024 min  
Delta R.T.: 0.000 min  
Response: 40226994  
Conc: 500.00 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1232ICC500

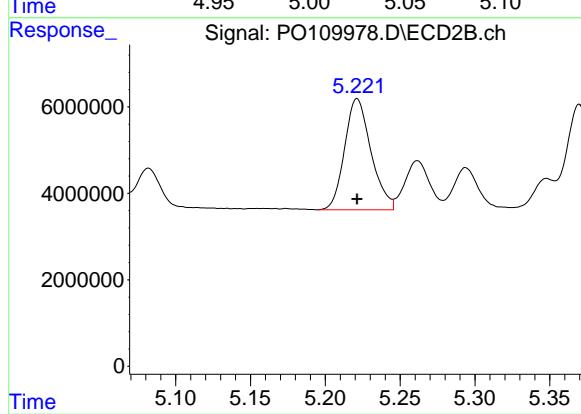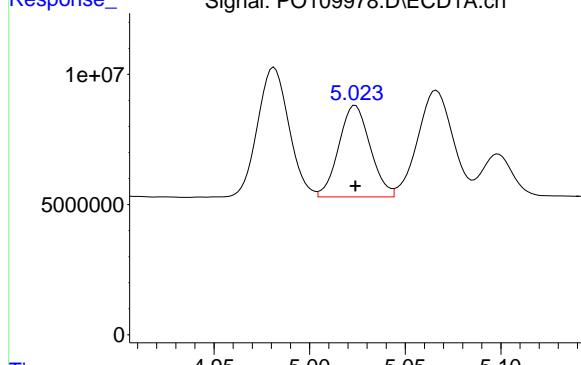

#15 AR-1232-5

R.T.: 5.221 min  
Delta R.T.: 0.000 min  
Response: 31608944  
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109979.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 16:11  
 Operator : YP/AJ  
 Sample : AR1242ICC1000  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1242ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:01:51 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:58:44 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	870.3E6	504.9E6	98.572	98.878
2) SA Decachlor...	8.744	8.697	707.3E6	217.8E6	97.860	97.910

Target Compounds

16) L4 AR-1242-1	4.785	4.772	257.0E6	141.3E6	967.387	967.723
17) L4 AR-1242-2	4.804	4.791	361.7E6	206.0E6	974.253	976.732
18) L4 AR-1242-3	4.861	4.966	239.3E6	108.8E6	957.525	967.388
19) L4 AR-1242-4	4.981	5.051	191.3E6	107.6E6	962.368	956.424
20) L4 AR-1242-5	5.635	5.572	200.3E6	132.5E6	953.851	956.059



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109979.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 16:11  
 Operator : YP/AJ  
 Sample : AR1242ICC1000  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1242ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:01:51 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:58:44 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

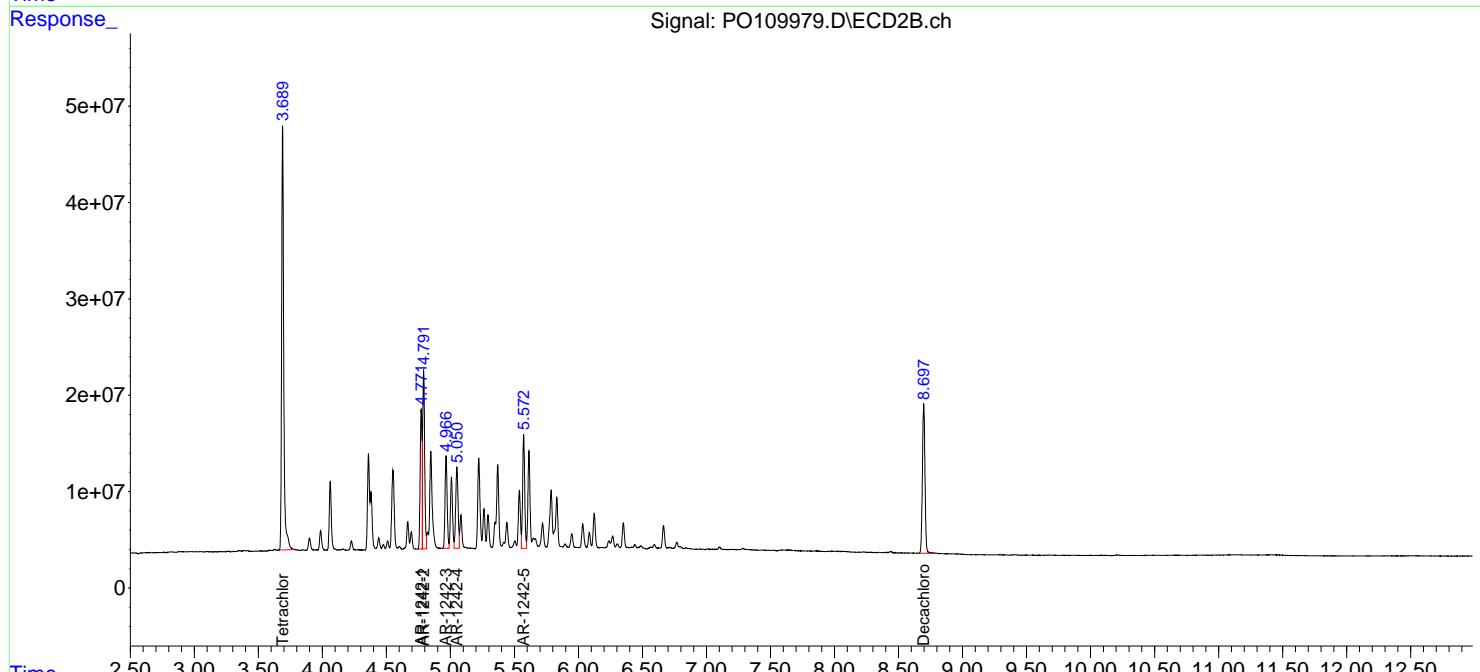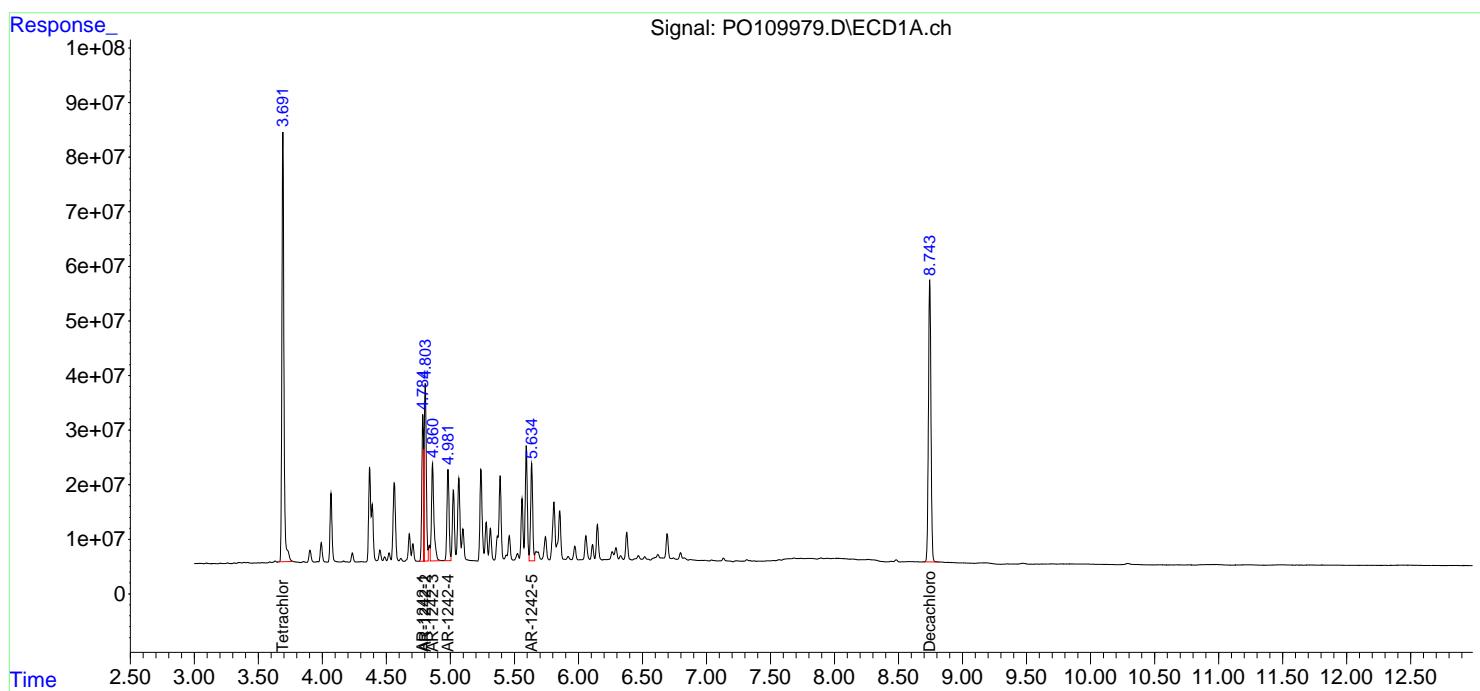

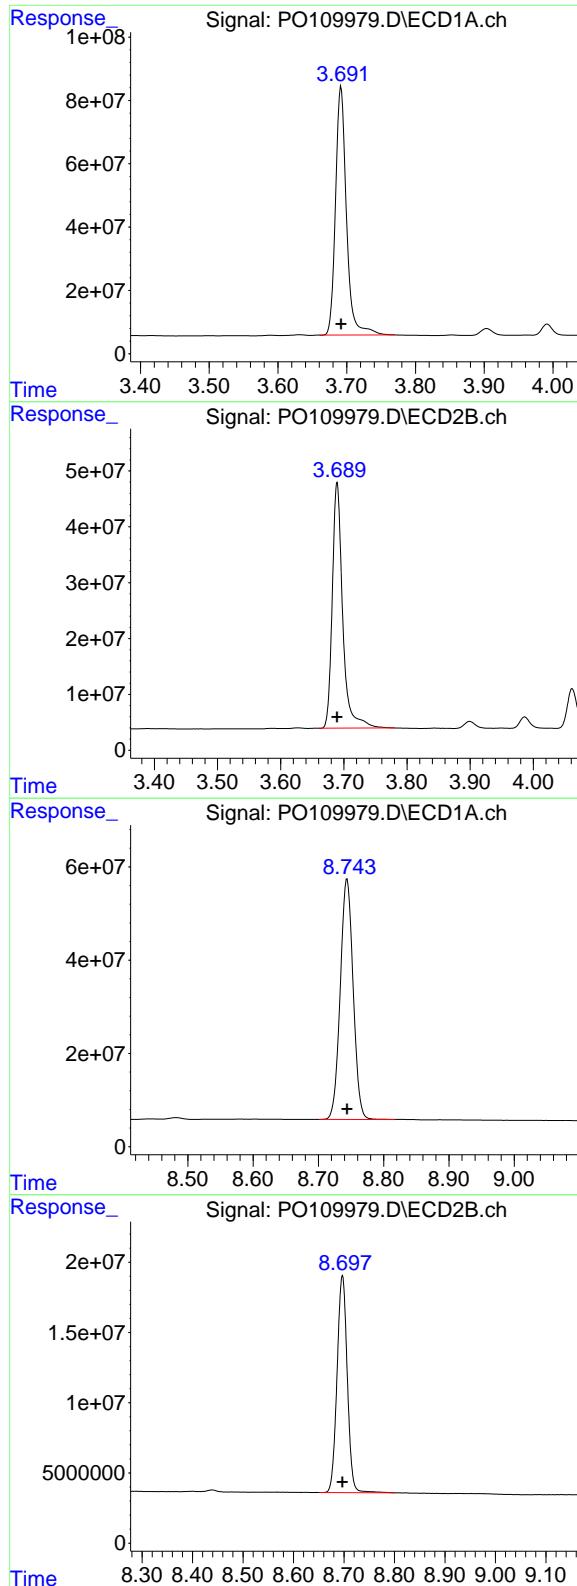

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 870277303  
Conc: 98.57 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC1000

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 504930415  
Conc: 98.88 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 707302147  
Conc: 97.86 ng/ml





## #2 Decachlorobiphenyl

R.T.: 8.697 min  
Delta R.T.: 0.000 min  
Response: 217777313  
Conc: 97.91 ng/ml

#16 AR-1242-1

R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 257021206  
 Conc: 967.39 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC1000

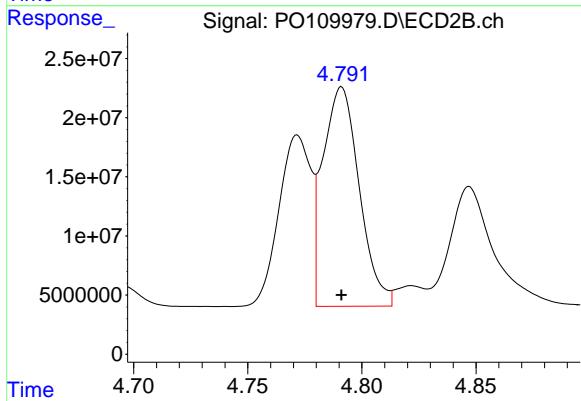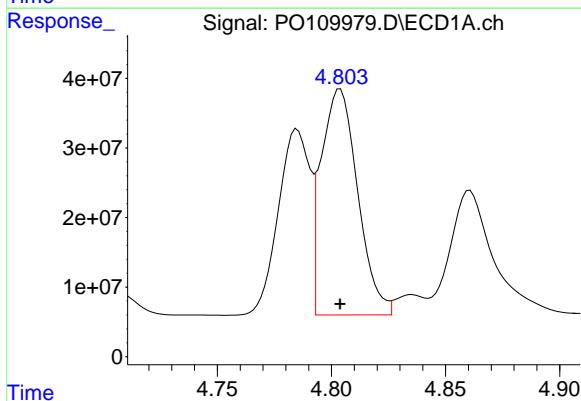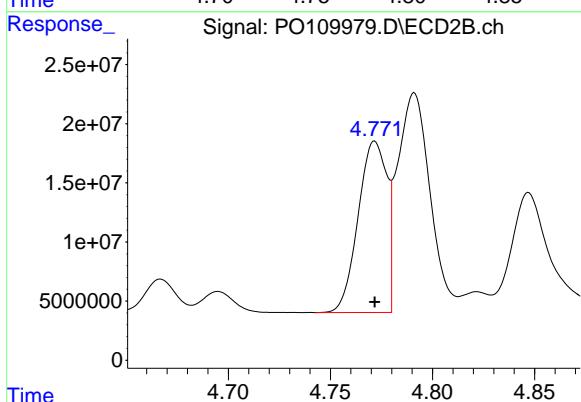

#16 AR-1242-1

R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 141331278  
 Conc: 967.72 ng/ml

#17 AR-1242-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 361656206  
 Conc: 974.25 ng/ml


#17 AR-1242-2

R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 205951481  
 Conc: 976.73 ng/ml

#18 AR-1242-3


R.T.: 4.861 min  
 Delta R.T.: 0.000 min  
 Response: 239272274  
 Conc: 957.52 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC1000

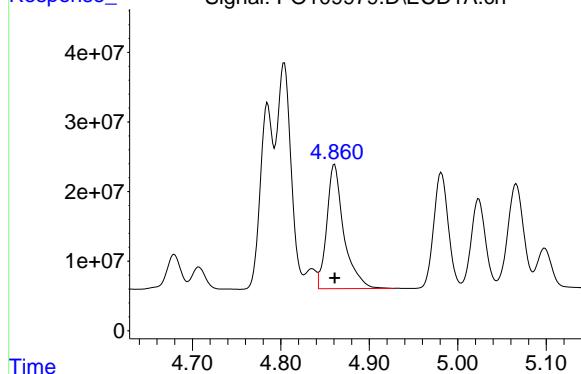


#18 AR-1242-3

R.T.: 4.966 min  
 Delta R.T.: 0.000 min  
 Response: 108828803  
 Conc: 967.39 ng/ml

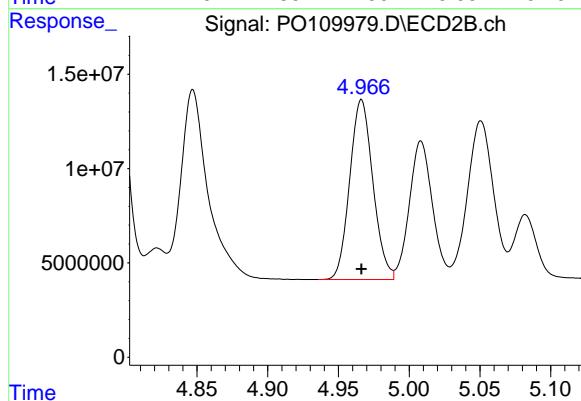


#19 AR-1242-4

R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 191269111  
 Conc: 962.37 ng/ml

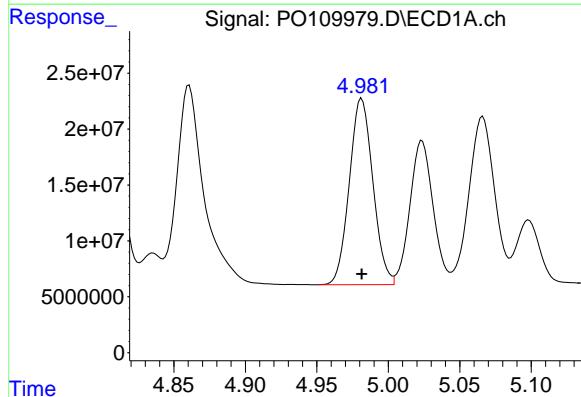

#19 AR-1242-4



R.T.: 5.051 min  
 Delta R.T.: 0.000 min  
 Response: 107629937  
 Conc: 956.42 ng/ml

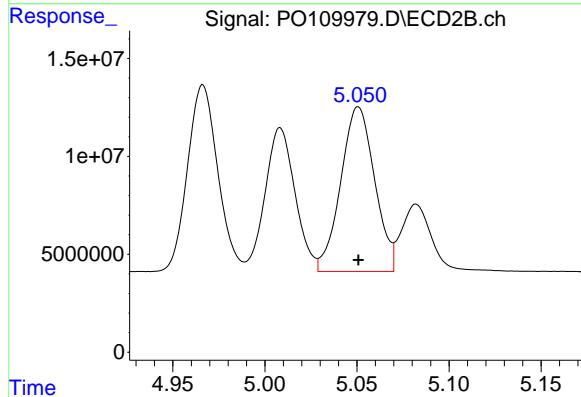

#20 AR-1242-5

R.T.: 5.635 min  
Delta R.T.: 0.000 min  
Response: 200342595  
Conc: 953.85 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1242ICC1000

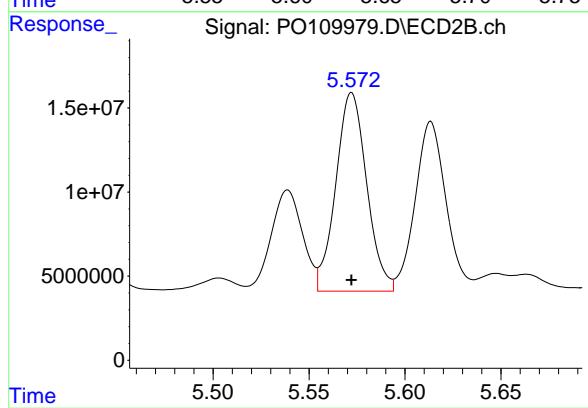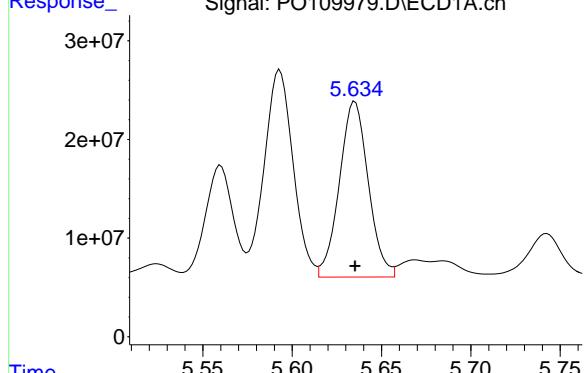

#20 AR-1242-5

R.T.: 5.572 min  
Delta R.T.: 0.000 min  
Response: 132486572  
Conc: 956.06 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109980.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 16:30  
 Operator : YP/AJ  
 Sample : AR1242ICC750  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1242ICC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:04:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:58:44 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.689	674.7E6	388.3E6	75.937	75.688
2) SA Decachlor...	8.744	8.696	546.6E6	166.9E6	75.416	75.037

Target Compounds

16) L4 AR-1242-1	4.785	4.771	203.4E6	110.1E6	760.384	752.515
17) L4 AR-1242-2	4.804	4.790	282.0E6	160.8E6	756.501	758.433
18) L4 AR-1242-3	4.860	4.966	192.4E6	85755968	763.306	758.150
19) L4 AR-1242-4	4.981	5.050	152.0E6	85465010	759.882	756.281
20) L4 AR-1242-5	5.634	5.572	159.2E6	104.3E6	755.214	751.684



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109980.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 16:30  
 Operator : YP/AJ  
 Sample : AR1242ICC750  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1242ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:04:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:58:44 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

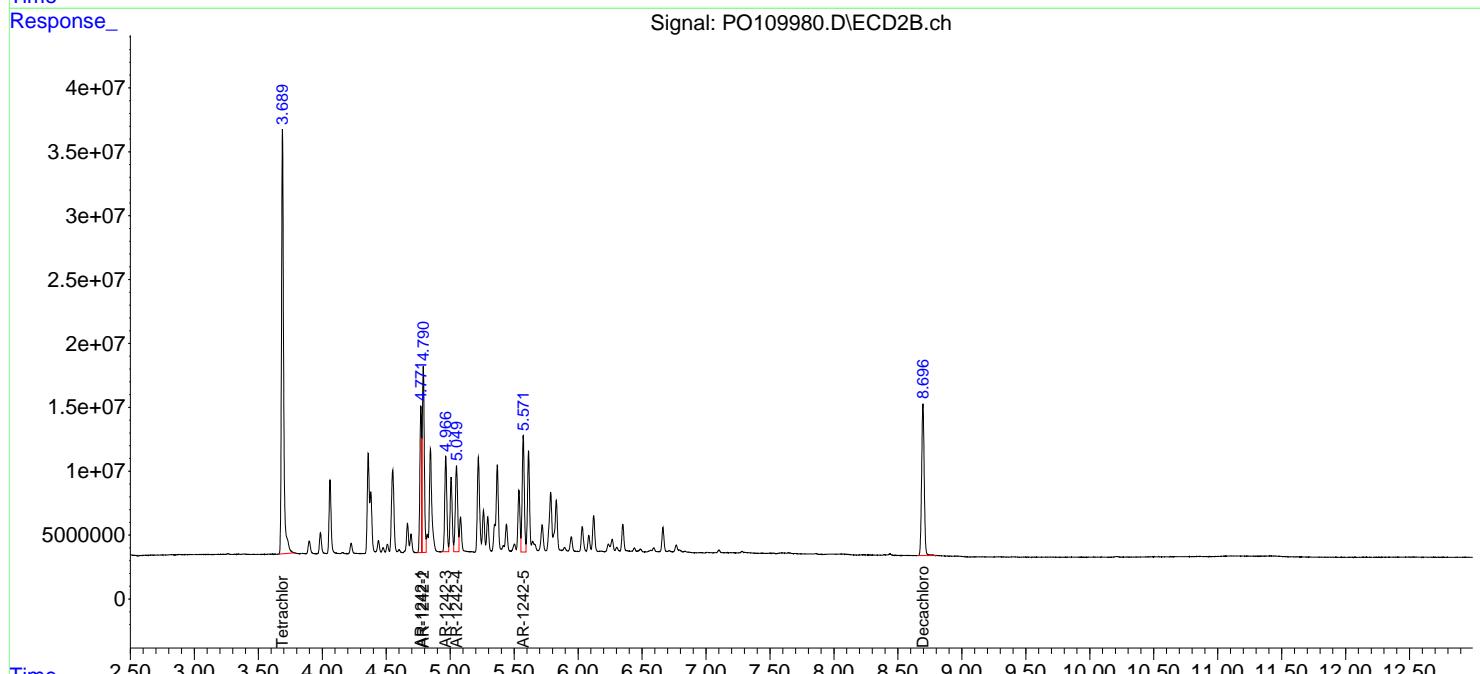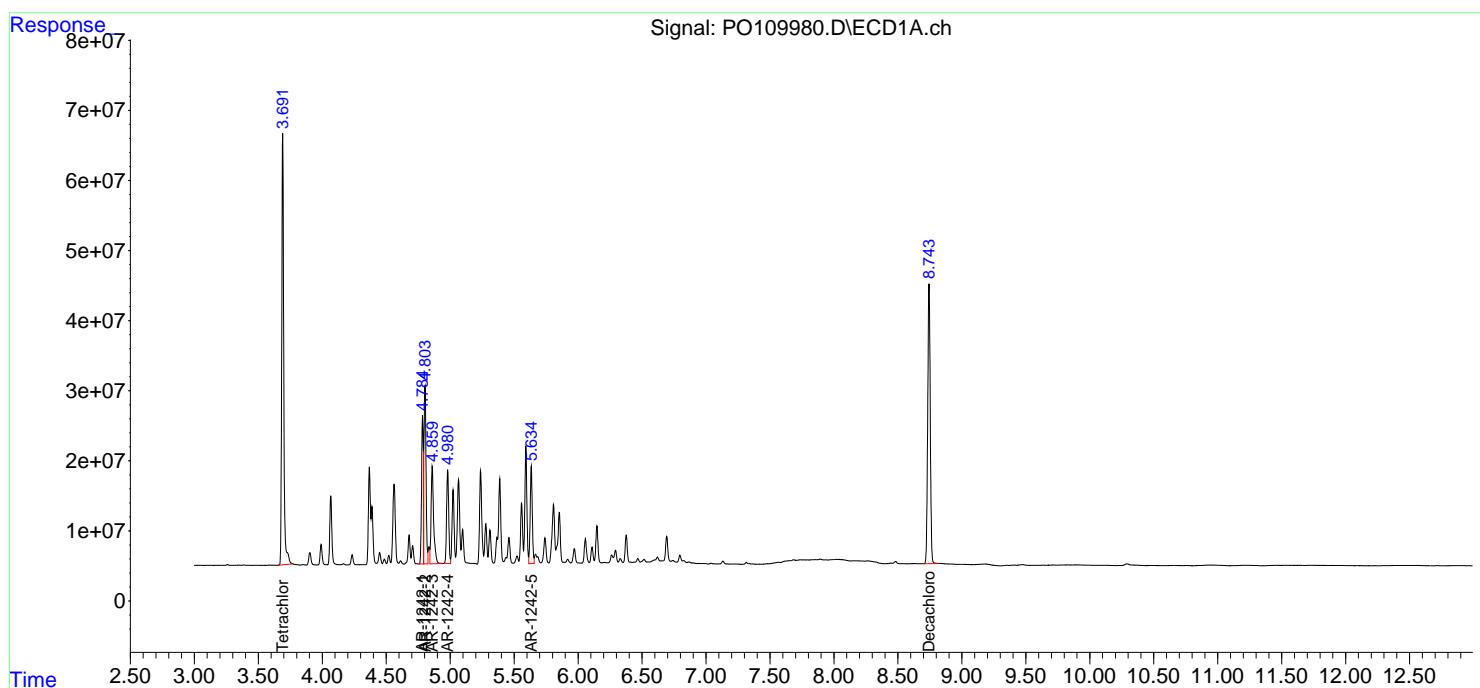

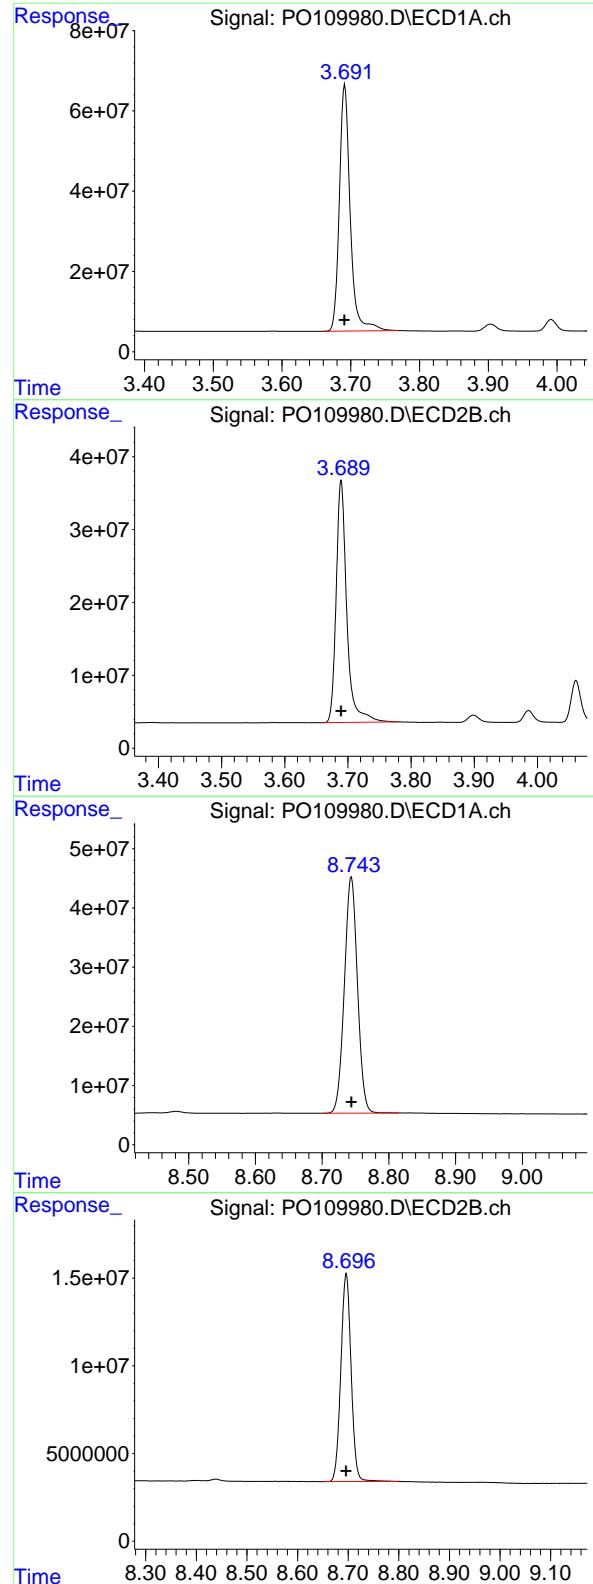

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: 0.000 min  
 Response: 674653935  
 Conc: 75.94 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC750

## #1 Tetrachloro-m-xylene


R.T.: 3.689 min  
 Delta R.T.: 0.000 min  
 Response: 388290346  
 Conc: 75.69 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
 Delta R.T.: 0.000 min  
 Response: 546604132  
 Conc: 75.42 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.696 min  
 Delta R.T.: 0.000 min  
 Response: 166944896  
 Conc: 75.04 ng/ml

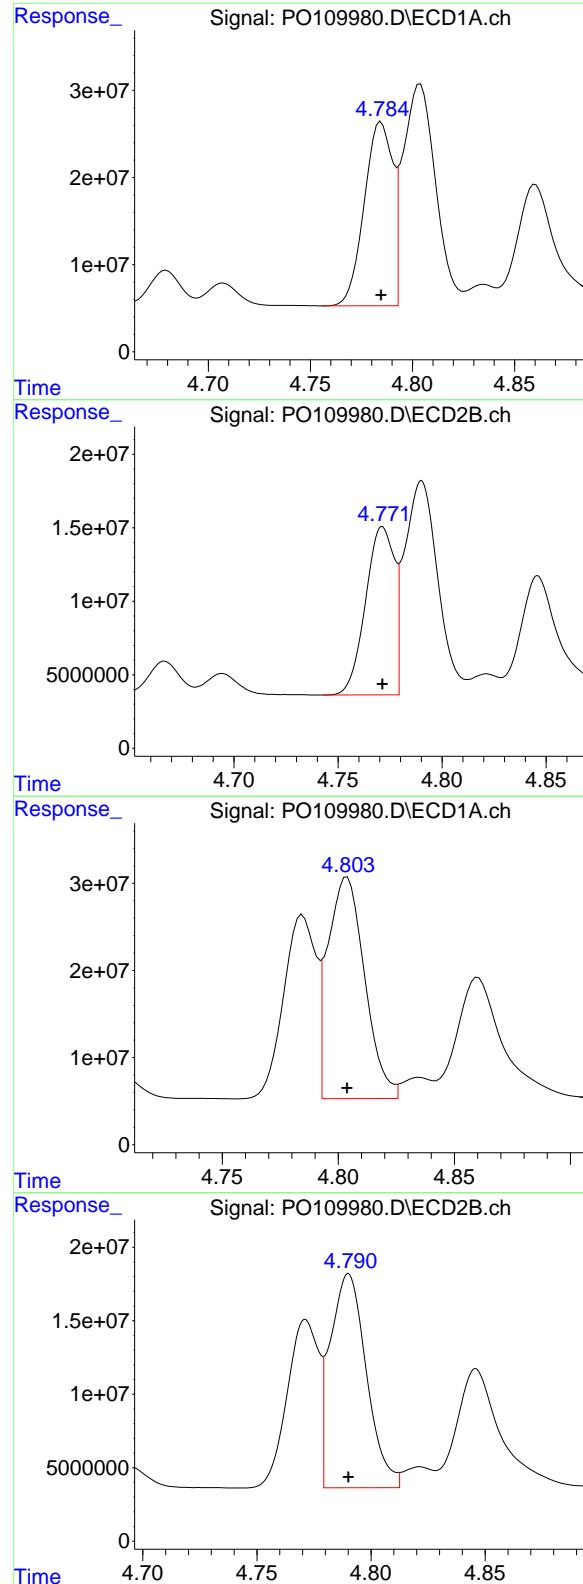

#16 AR-1242-1

R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 203431528  
 Conc: 760.38 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1242ICC750

#16 AR-1242-1


R.T.: 4.771 min  
 Delta R.T.: 0.000 min  
 Response: 110085812  
 Conc: 752.52 ng/ml

#17 AR-1242-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 282046233  
 Conc: 756.50 ng/ml

#17 AR-1242-2

R.T.: 4.790 min  
 Delta R.T.: 0.000 min  
 Response: 160825699  
 Conc: 758.43 ng/ml

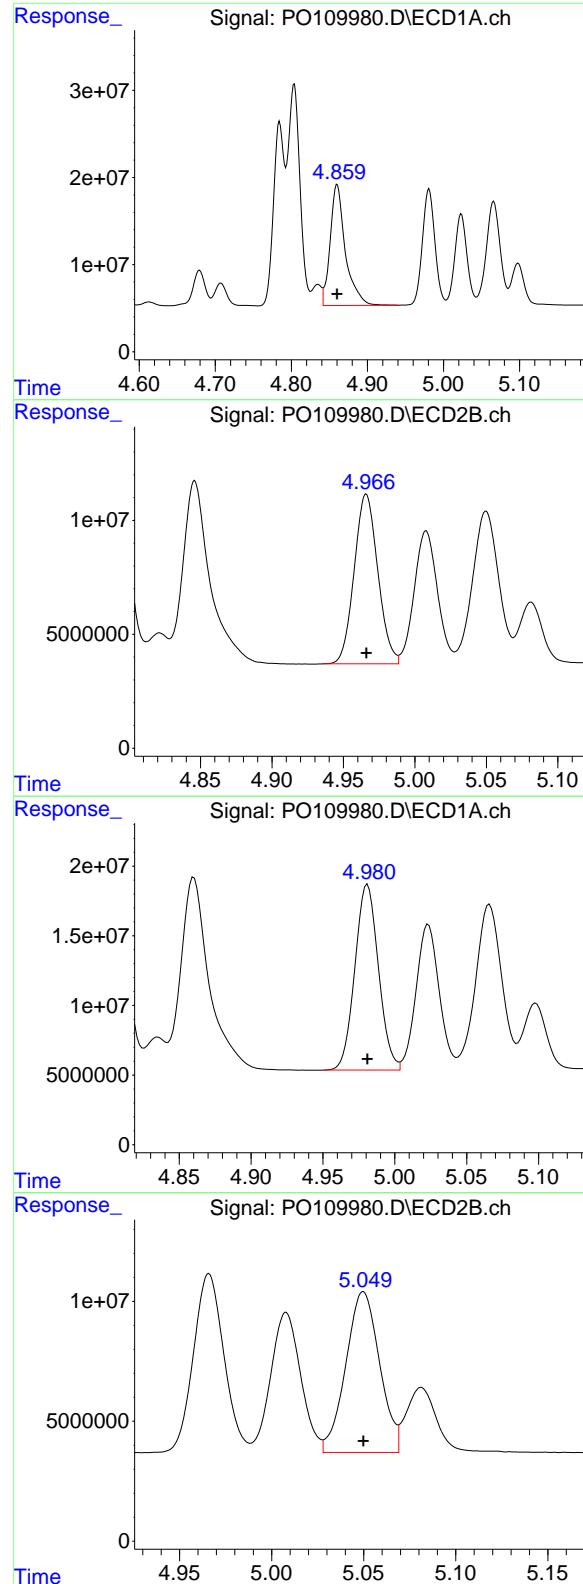

#18 AR-1242-3

R.T.: 4.860 min  
 Delta R.T.: 0.000 min  
 Response: 192446698  
 Conc: 763.31 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1242ICC750

#18 AR-1242-3

R.T.: 4.966 min  
 Delta R.T.: 0.000 min  
 Response: 85755968  
 Conc: 758.15 ng/ml

#19 AR-1242-4

R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 152026829  
 Conc: 759.88 ng/ml



#19 AR-1242-4

R.T.: 5.050 min  
 Delta R.T.: 0.000 min  
 Response: 85465010  
 Conc: 756.28 ng/ml

#20 AR-1242-5

R.T.: 5.634 min  
Delta R.T.: 0.000 min  
Response: 159175050  
Conc: 755.21 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1242ICC750

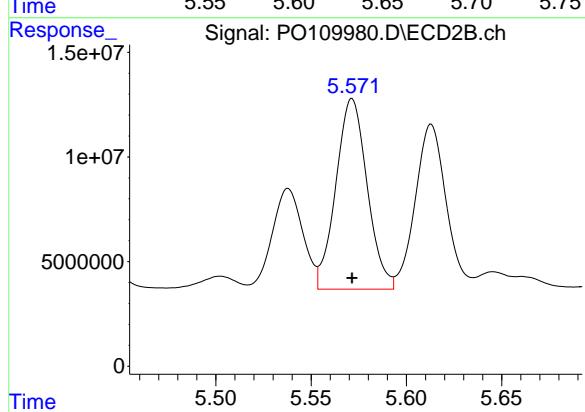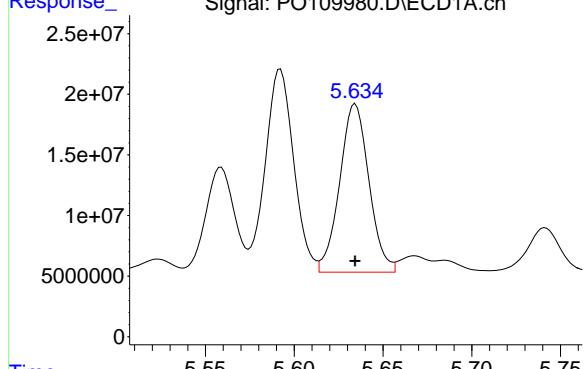

#20 AR-1242-5

R.T.: 5.572 min  
Delta R.T.: 0.000 min  
Response: 104282352  
Conc: 751.68 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109981.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 16:48  
 Operator : YP/AJ  
 Sample : AR1242ICC500  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1242ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:59:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:58:44 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	447.7E6	258.2E6	50.000	50.000
2) SA Decachlor...	8.744	8.695	369.1E6	113.5E6	50.000	50.000

Target Compounds

16) L4 AR-1242-1	4.785	4.772	137.2E6	75379512	500.000	500.000
17) L4 AR-1242-2	4.805	4.791	190.4E6	107.9E6	500.000	500.000
18) L4 AR-1242-3	4.861	4.967	130.3E6	58083170	500.000	500.000
19) L4 AR-1242-4	4.982	5.051	103.1E6	58718718	500.000	500.000
20) L4 AR-1242-5	5.635	5.573	109.9E6	72332482	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109981.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 16:48  
 Operator : YP/AJ  
 Sample : AR1242ICC500  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1242ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:59:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:58:44 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

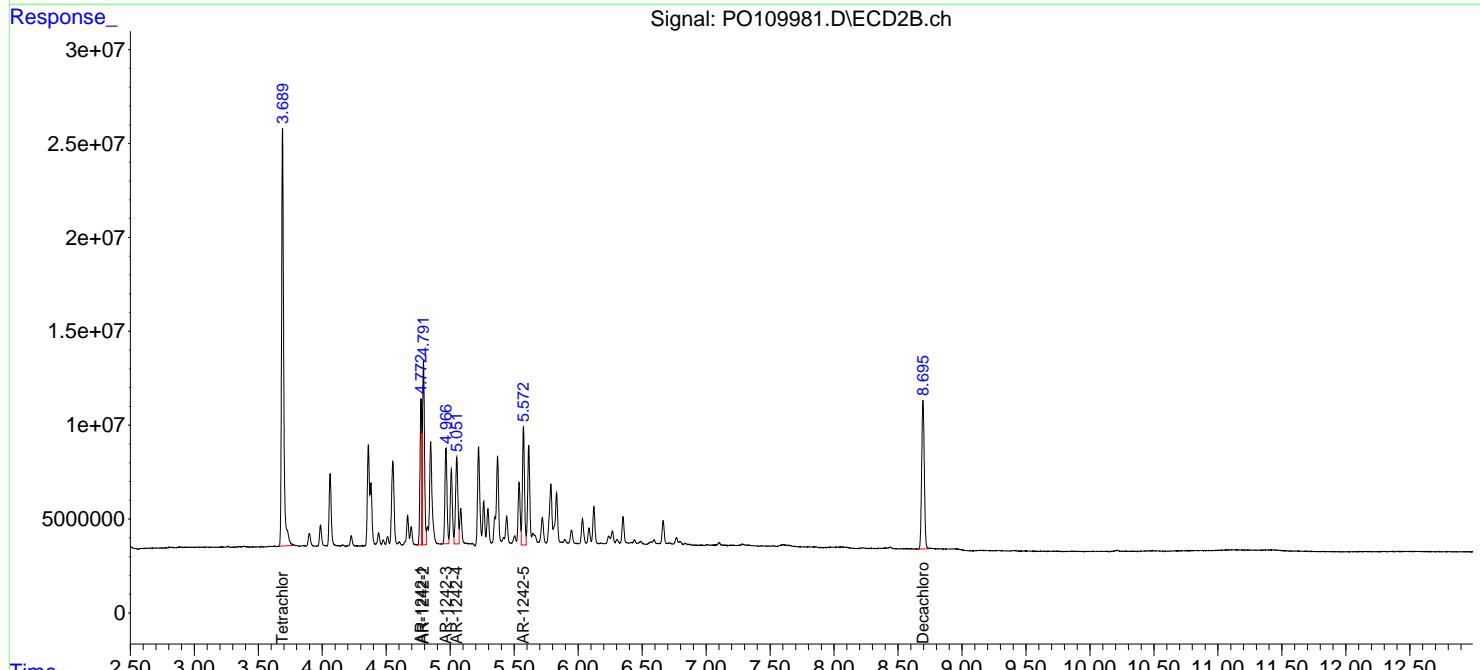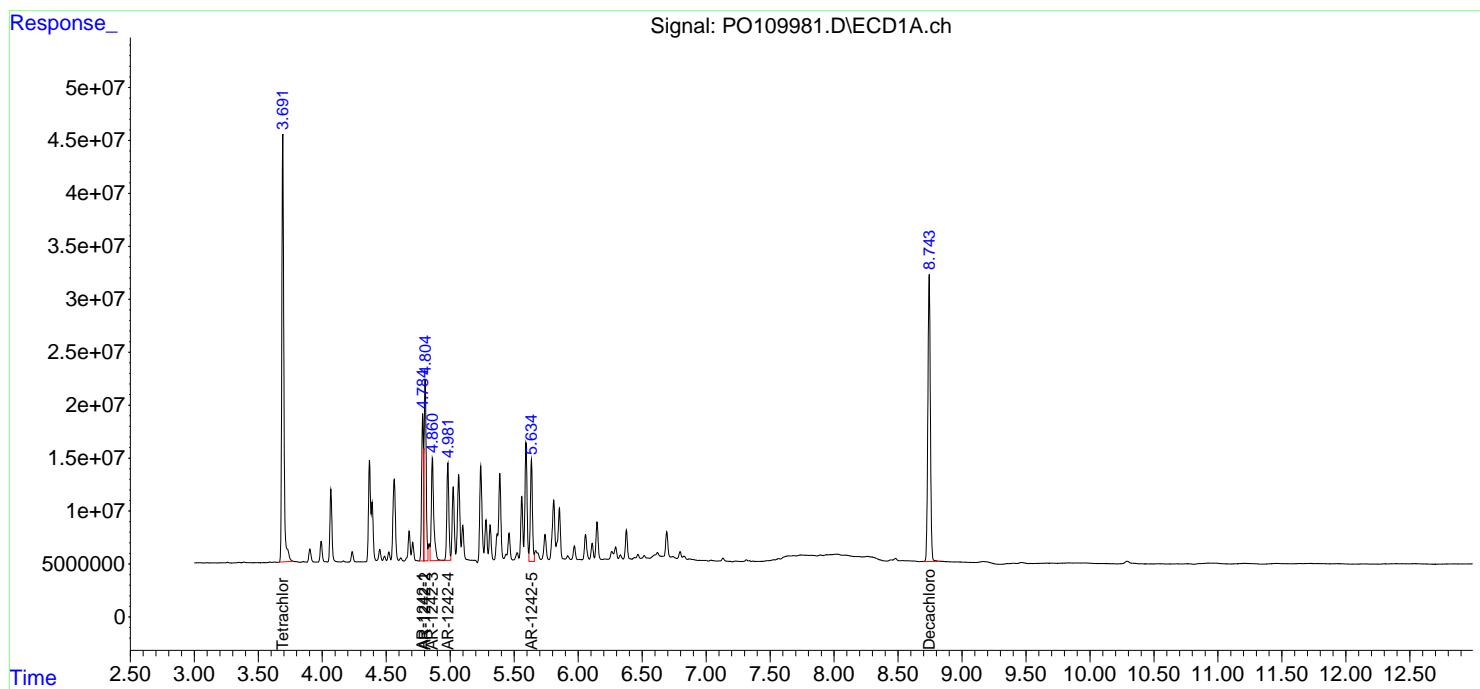

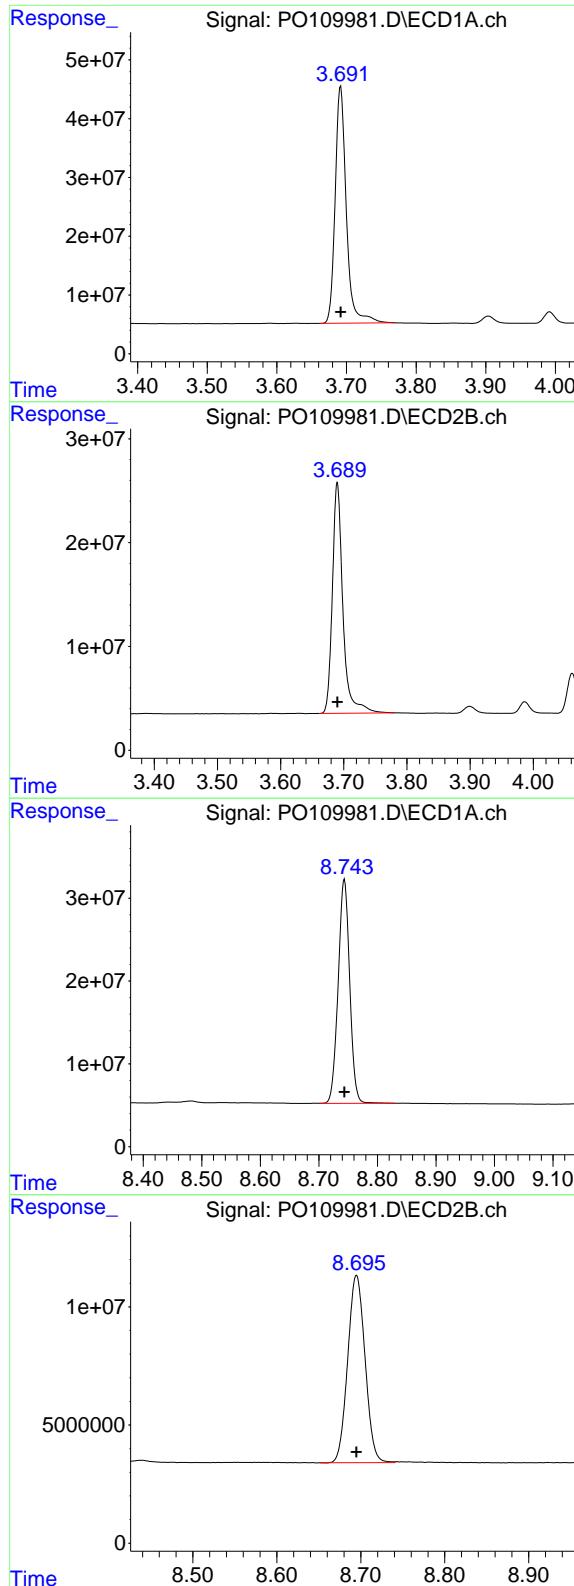

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
 Delta R.T.: 0.000 min  
 Response: 447743138  
 Conc: 50.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC500

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: 0.000 min  
 Response: 258194376  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
 Delta R.T.: 0.000 min  
 Response: 369119192  
 Conc: 50.00 ng/ml





## #2 Decachlorobiphenyl

R.T.: 8.695 min  
 Delta R.T.: 0.000 min  
 Response: 113538071  
 Conc: 50.00 ng/ml

#16 AR-1242-1

R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 137175388  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC500

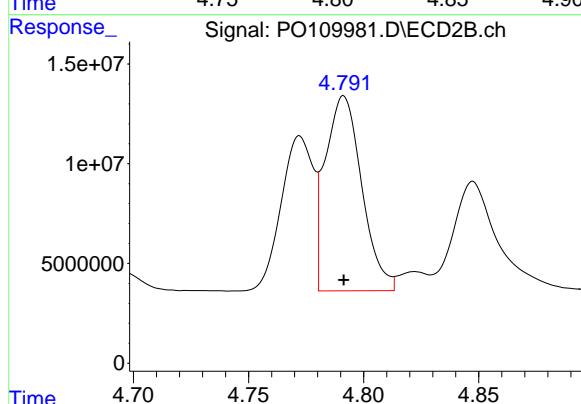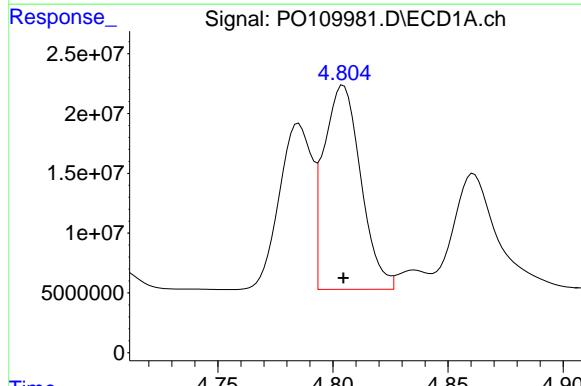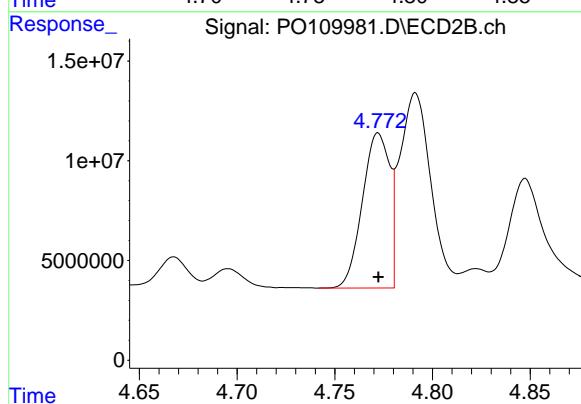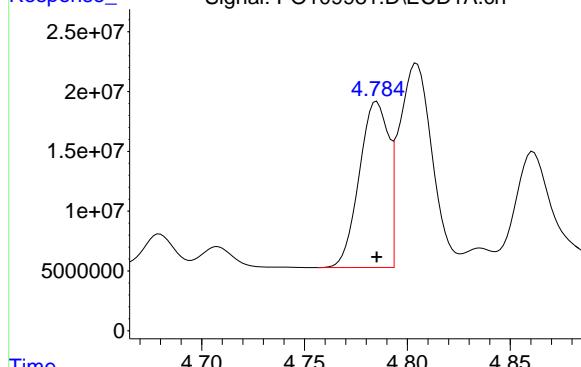

#16 AR-1242-1


R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 75379512  
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 4.805 min  
 Delta R.T.: 0.000 min  
 Response: 190385713  
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 107881886  
 Conc: 500.00 ng/ml

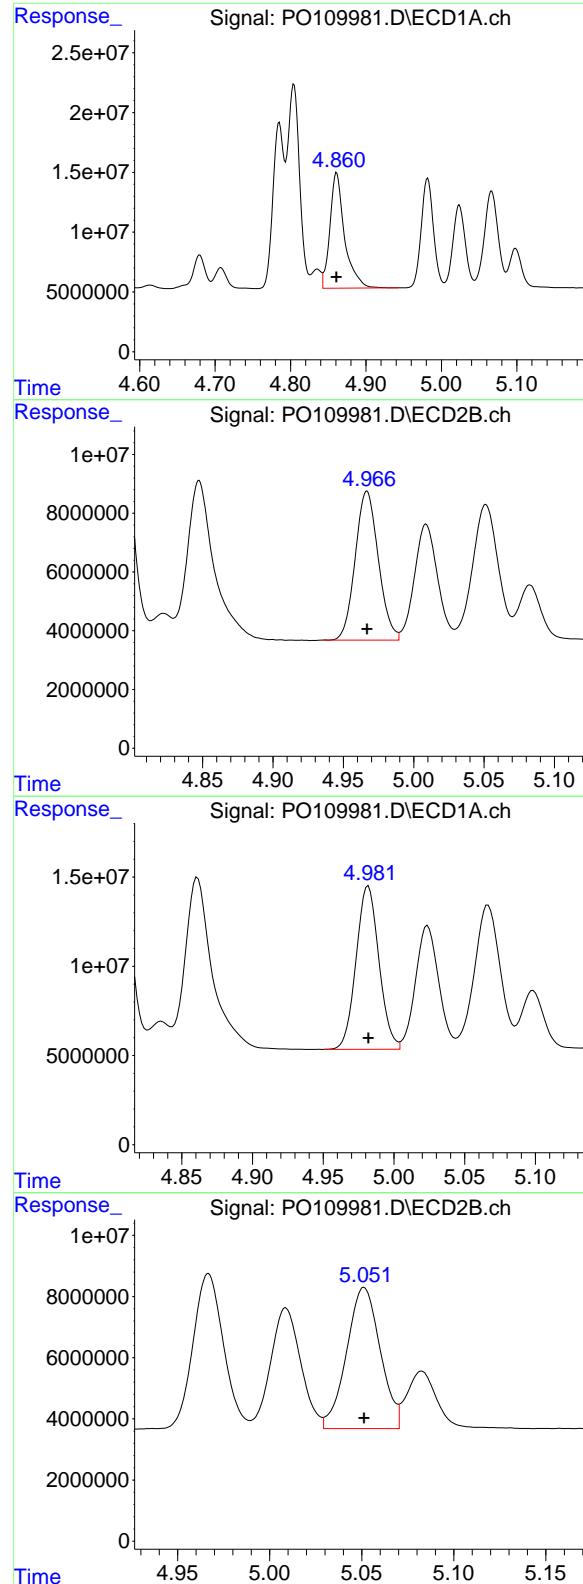

#18 AR-1242-3

R.T.: 4.861 min  
 Delta R.T.: 0.000 min  
 Response: 130250168  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC500

#18 AR-1242-3

R.T.: 4.967 min  
 Delta R.T.: 0.000 min  
 Response: 58083170  
 Conc: 500.00 ng/ml

#19 AR-1242-4

R.T.: 4.982 min  
 Delta R.T.: 0.000 min  
 Response: 103113773  
 Conc: 500.00 ng/ml



#19 AR-1242-4

R.T.: 5.051 min  
 Delta R.T.: 0.000 min  
 Response: 58718718  
 Conc: 500.00 ng/ml

#20 AR-1242-5

R.T.: 5.635 min  
Delta R.T.: 0.000 min  
Response: 109864205  
Conc: 500.00 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1242ICC500

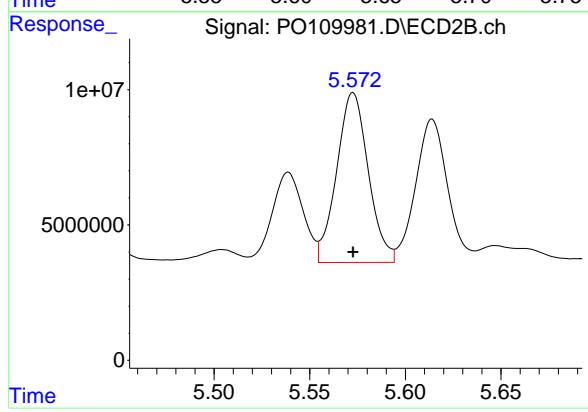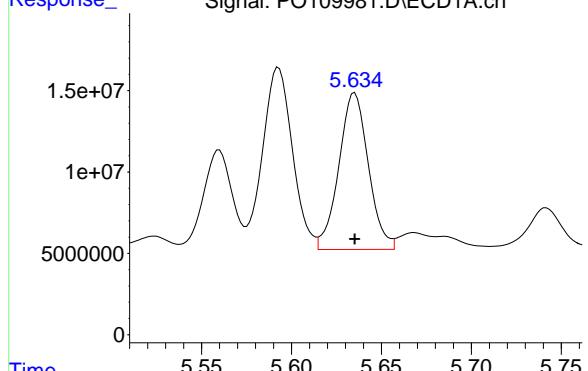

#20 AR-1242-5

R.T.: 5.573 min  
Delta R.T.: 0.000 min  
Response: 72332482  
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109982.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 17:06  
 Operator : YP/AJ  
 Sample : AR1242ICC250  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1242ICC250

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:16:15 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 17:16:03 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	226.3E6	130.2E6	25.356	25.281
2) SA Decachlor...	8.744	8.695	194.6E6	60893229	26.361	26.736

Target Compounds

16) L4 AR-1242-1	4.785	4.772	71937746	39990799	263.903	267.124
17) L4 AR-1242-2	4.804	4.791	99324236	56210353	262.106	261.143
18) L4 AR-1242-3	4.860	4.967	69326183	30721999	268.271	265.862
19) L4 AR-1242-4	4.981	5.051	53927655	31584987	264.381	271.488
20) L4 AR-1242-5	5.634	5.572	57576429	38102015	266.987	268.040



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109982.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 17:06  
 Operator : YP/AJ  
 Sample : AR1242ICC250  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1242ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:16:15 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 17:16:03 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

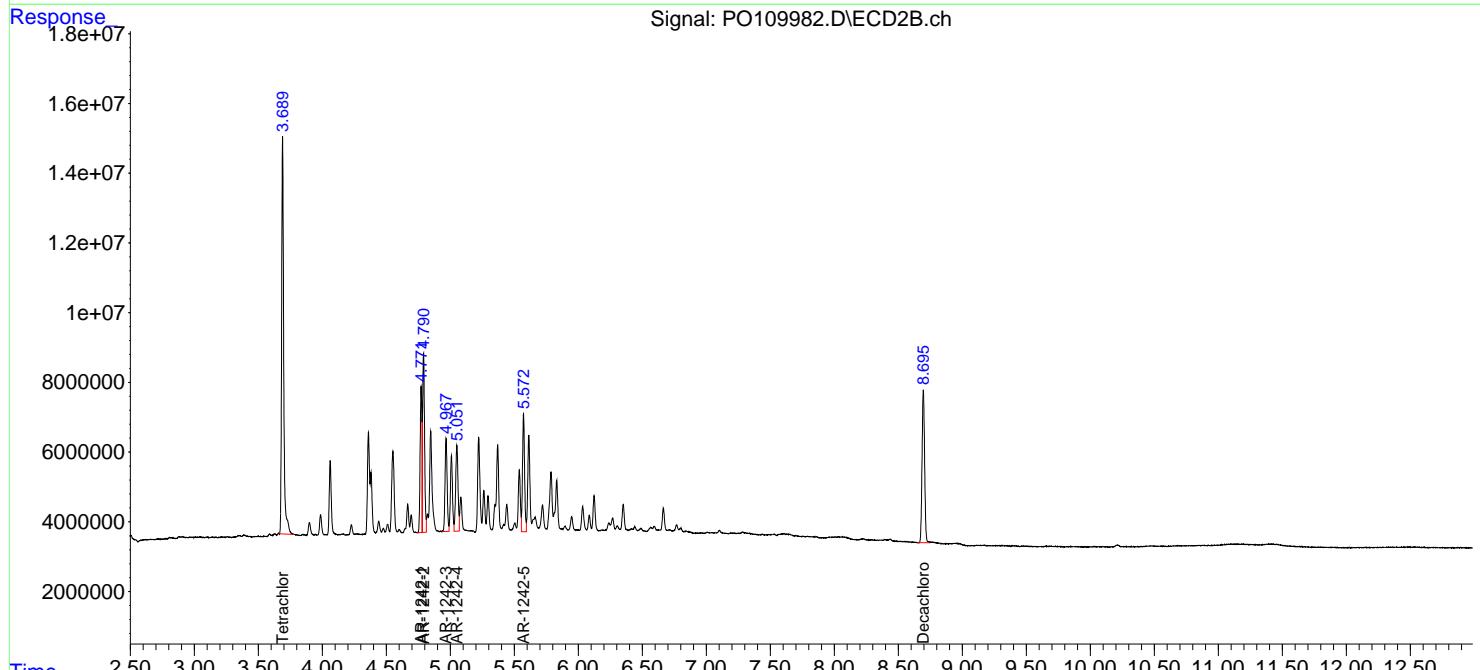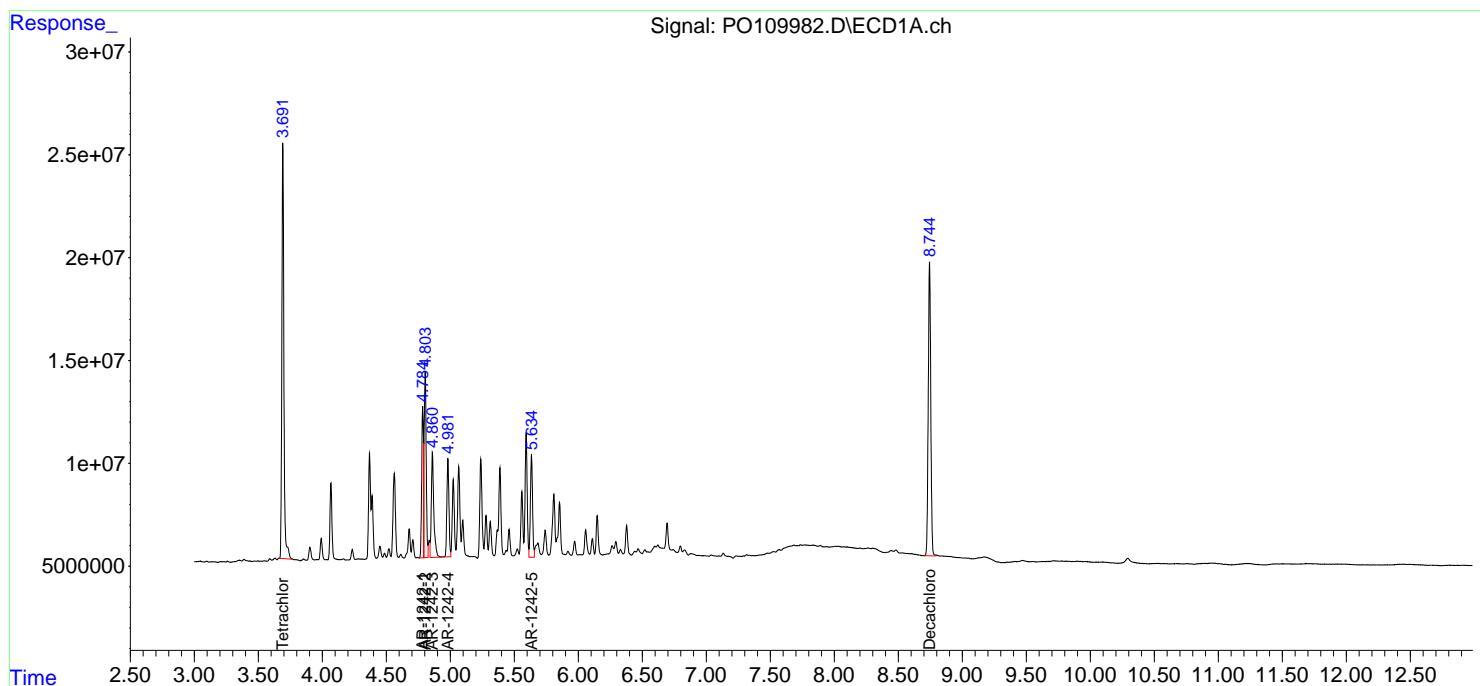

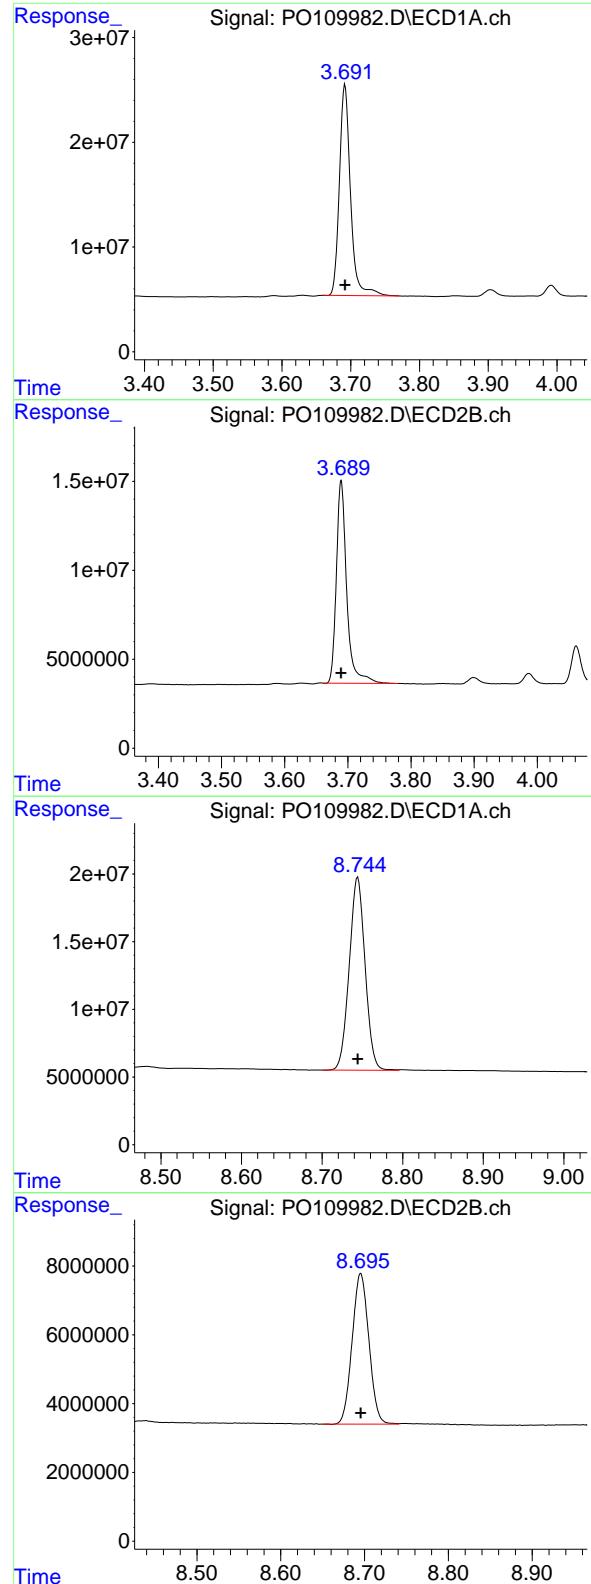

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 226344128  
Conc: 25.36 ng/ml

Instrument:

ECD\_O

ClientSampleId :

AR1242ICC250

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 130179852  
Conc: 25.28 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 194588935  
Conc: 26.36 ng/ml


## #2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 60893229  
Conc: 26.74 ng/ml

#16 AR-1242-1


R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 71937746  
 Conc: 263.90 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC250




#16 AR-1242-1

R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 39990799  
 Conc: 267.12 ng/ml

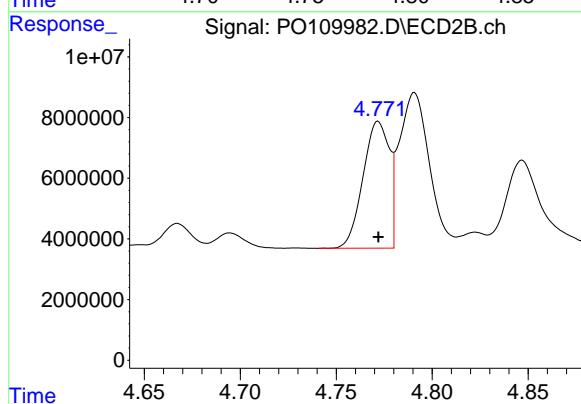


#17 AR-1242-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 99324236  
 Conc: 262.11 ng/ml

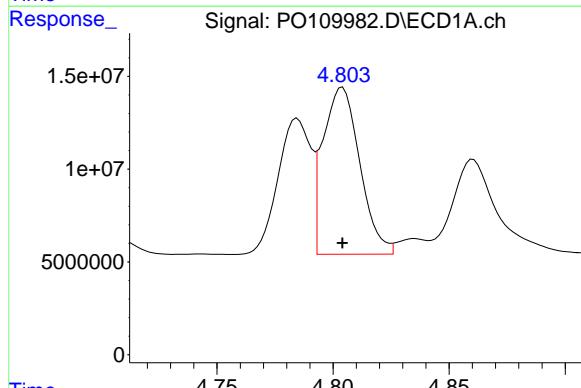

#17 AR-1242-2





R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 56210353  
 Conc: 261.14 ng/ml

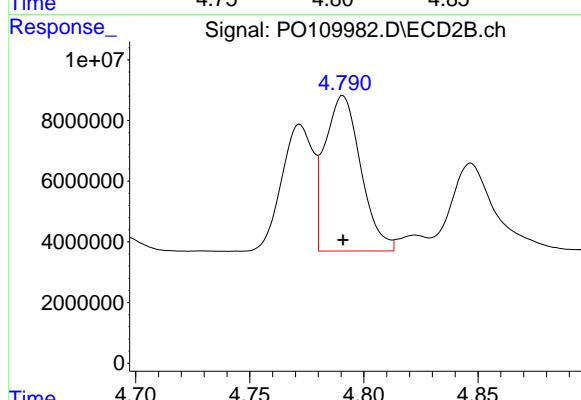

#18 AR-1242-3

R.T.: 4.860 min  
 Delta R.T.: 0.000 min  
 Response: 69326183  
 Conc: 268.27 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC250

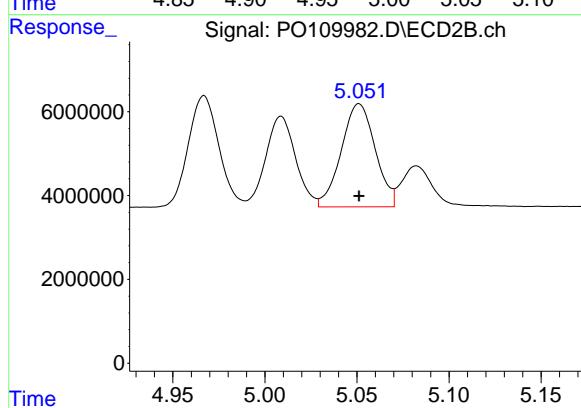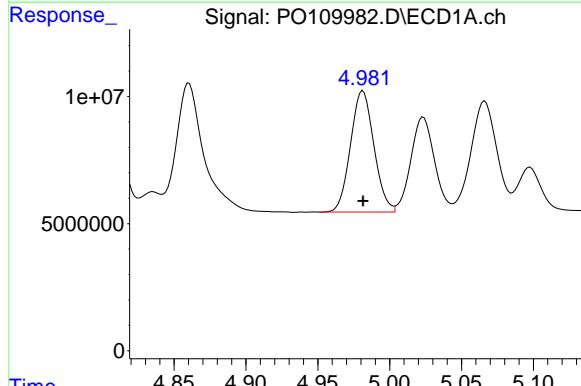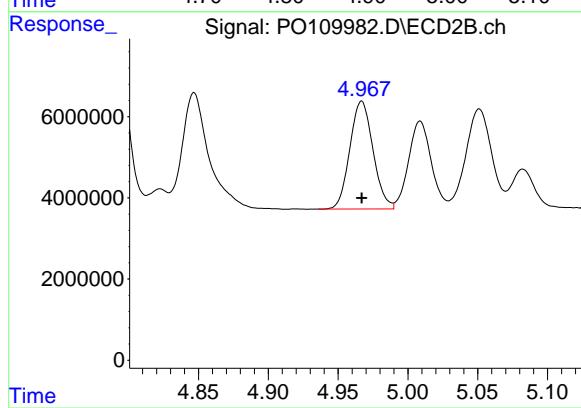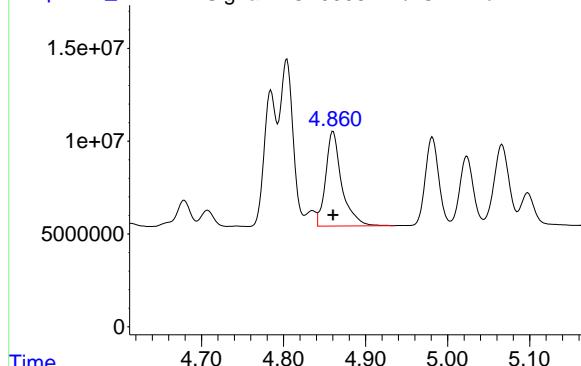

#18 AR-1242-3

R.T.: 4.967 min  
 Delta R.T.: 0.000 min  
 Response: 30721999  
 Conc: 265.86 ng/ml

#19 AR-1242-4

R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 53927655  
 Conc: 264.38 ng/ml



#19 AR-1242-4

R.T.: 5.051 min  
 Delta R.T.: 0.000 min  
 Response: 31584987  
 Conc: 271.49 ng/ml

#20 AR-1242-5

R.T.: 5.634 min  
Delta R.T.: 0.000 min  
Response: 57576429  
Conc: 266.99 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1242ICC250

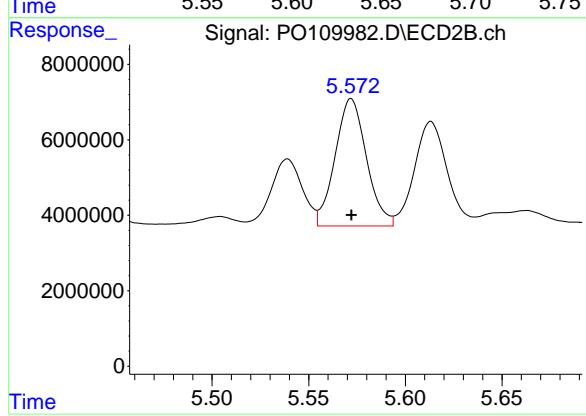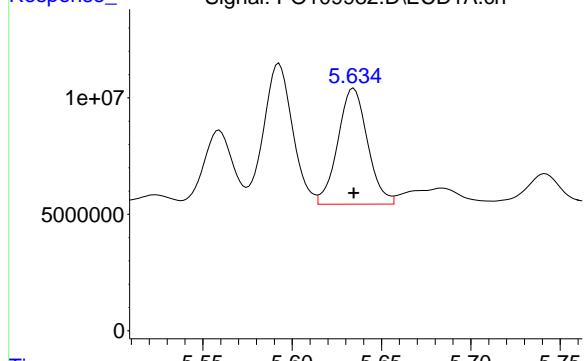

#20 AR-1242-5

R.T.: 5.572 min  
Delta R.T.: 0.000 min  
Response: 38102015  
Conc: 268.04 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109983.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 17:25  
 Operator : YP/AJ  
 Sample : AR1242ICC050  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1242ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:34:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 17:34:29 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	3.691	3.688	33275417	17649519	3.978m	3.680m
2) SA Decachlor...	8.744	8.696	32408304	10337597	4.500	4.624

**Target Compounds**

16) L4 AR-1242-1	4.784	4.772	12333502	6612130	46.123	45.222
17) L4 AR-1242-2	4.804	4.791	16261465	8959332	44.164	43.066
18) L4 AR-1242-3	4.859	4.966	12804073	4792003	49.638	42.926m
19) L4 AR-1242-4	4.980	5.051	9228050	5726073	46.259m	49.373
20) L4 AR-1242-5	5.633	5.572	9633519	5880388	45.772m	42.708m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109983.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 17:25  
 Operator : YP/AJ  
 Sample : AR1242ICC050  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1


Instrument :  
 ECD\_O  
 ClientSampleId :  
 AR1242ICC050


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:34:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 17:34:29 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

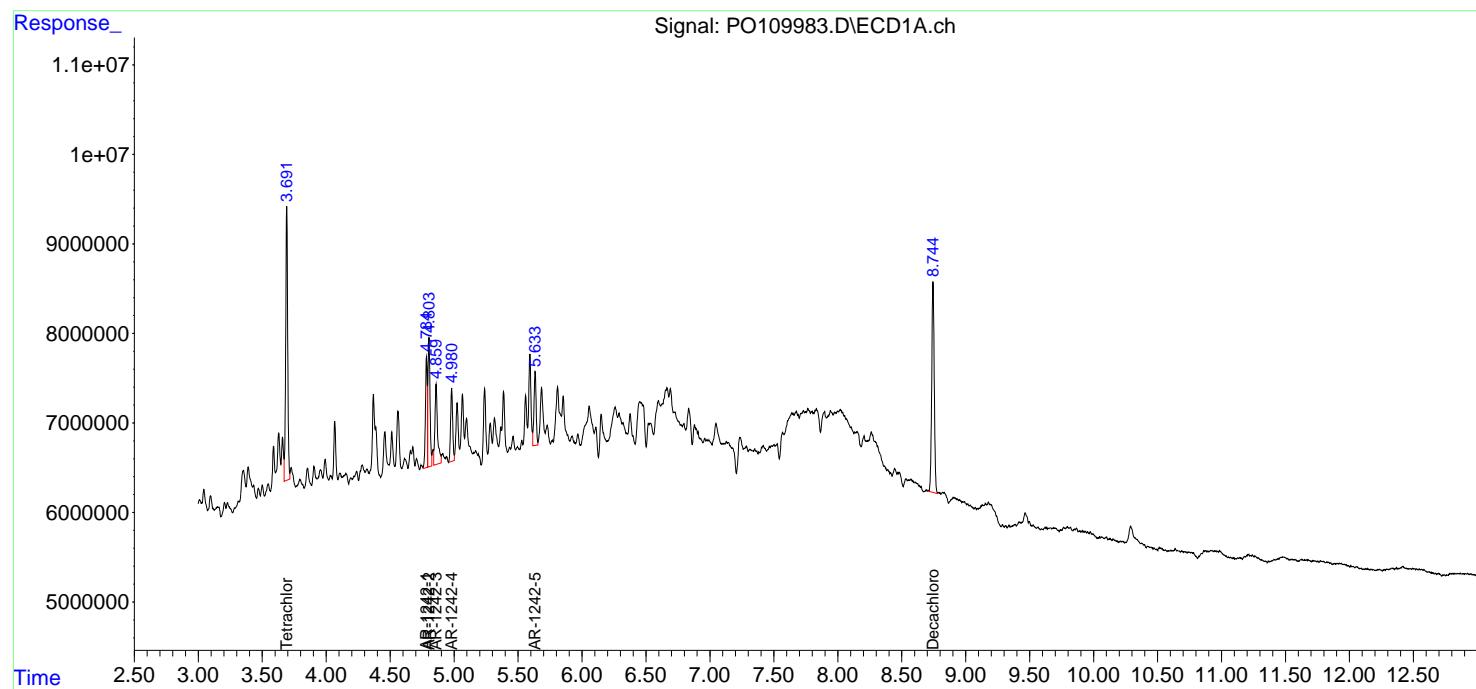

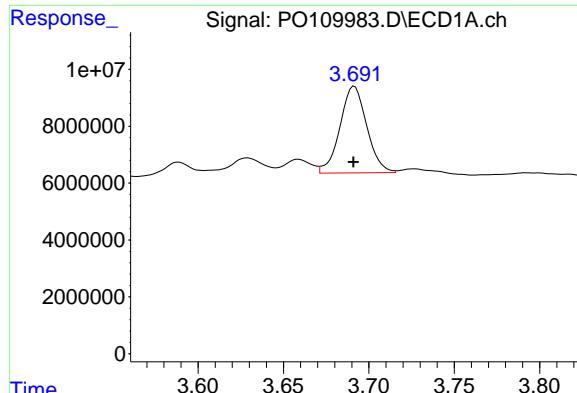


## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
Delta R.T.: 0.000 min  
Response: 33275417  
Conc: 3.98 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1242ICC050


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

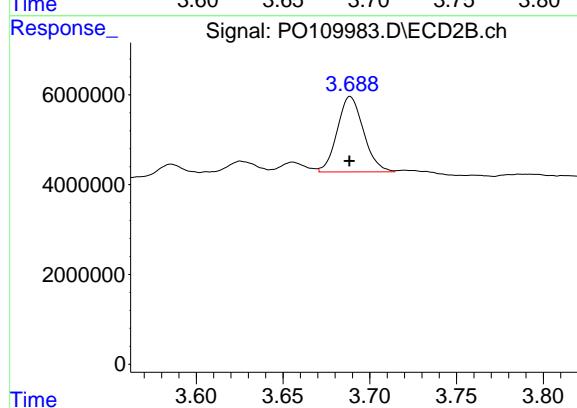


## #1 Tetrachloro-m-xylene

R.T.: 3.688 min  
Delta R.T.: 0.000 min  
Response: 17649519  
Conc: 3.68 ng/ml

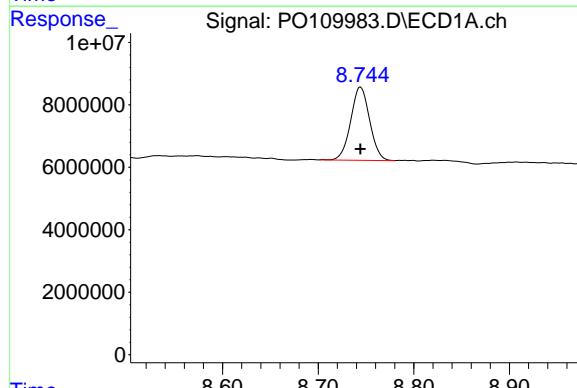


## #2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 32408304  
Conc: 4.50 ng/ml

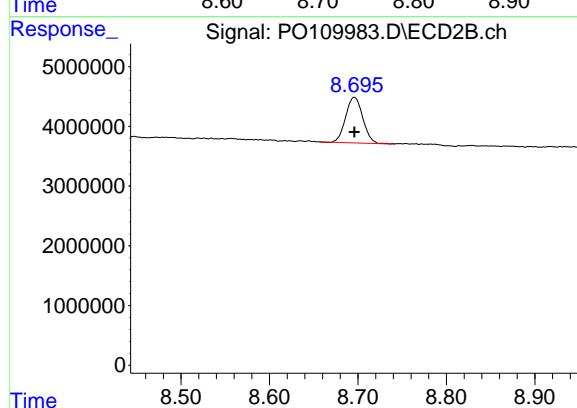

## #2 Decachlorobiphenyl

R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 10337597  
Conc: 4.62 ng/ml

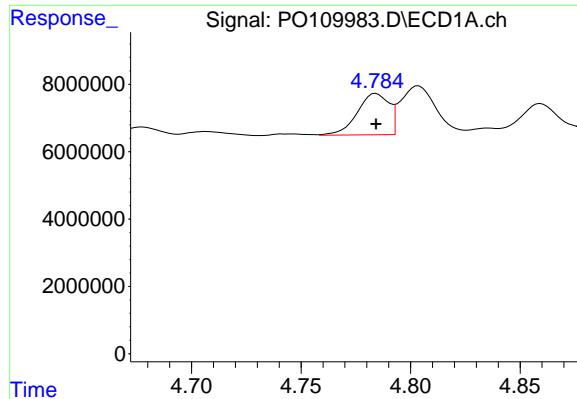


#16 AR-1242-1

R.T.: 4.784 min  
 Delta R.T.: 0.000 min  
 Response: 12333502  
 Conc: 46.12 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC050


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

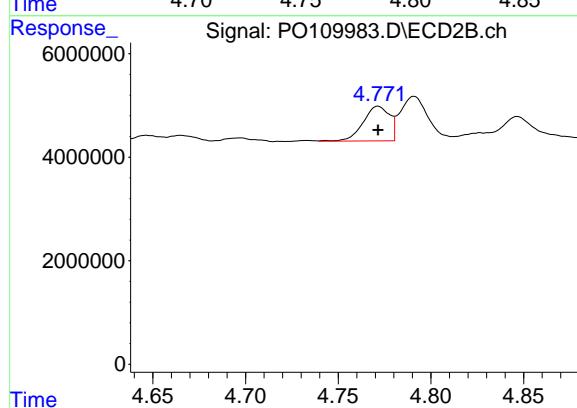


#16 AR-1242-1

R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 6612130  
 Conc: 45.22 ng/ml

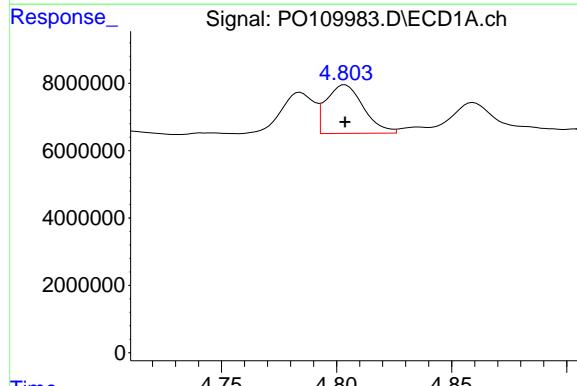



#17 AR-1242-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 16261465  
 Conc: 44.16 ng/ml

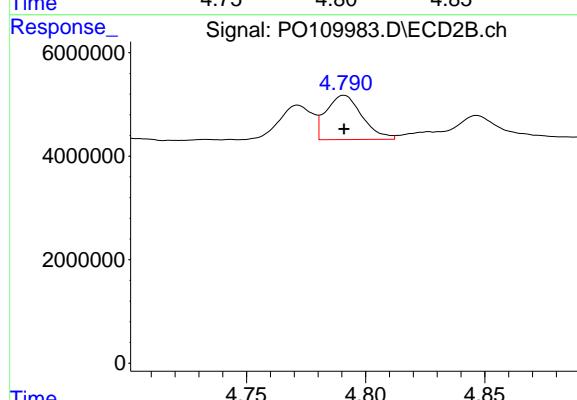

#17 AR-1242-2

R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 8959332  
 Conc: 43.07 ng/ml

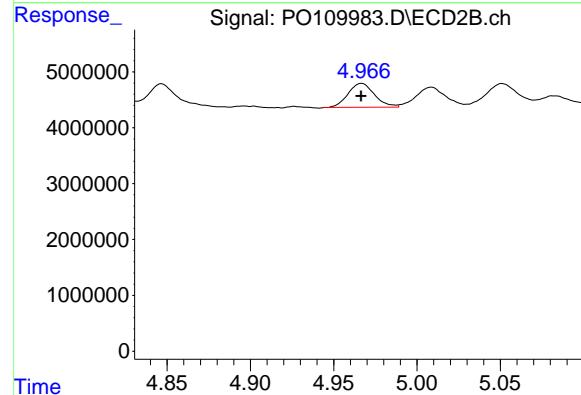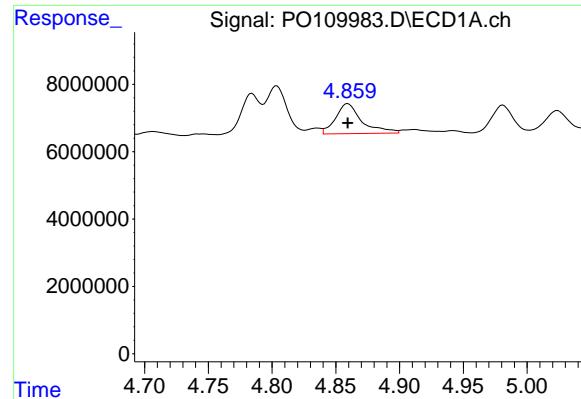


#18 AR-1242-3

R.T.: 4.859 min  
 Delta R.T.: 0.000 min  
 Response: 12804073  
 Conc: 49.64 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1242ICC050


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

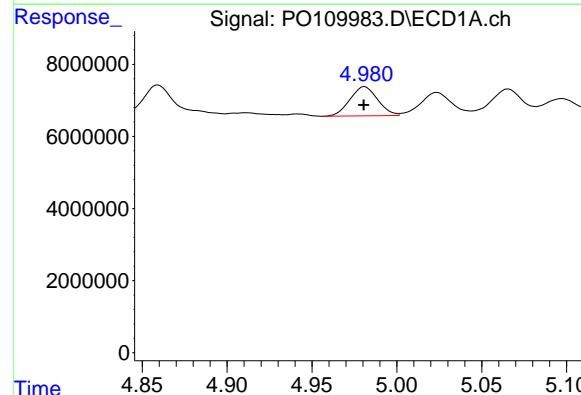

#18 AR-1242-3

R.T.: 4.966 min  
 Delta R.T.: 0.000 min  
 Response: 4792003  
 Conc: 42.93 ng/ml

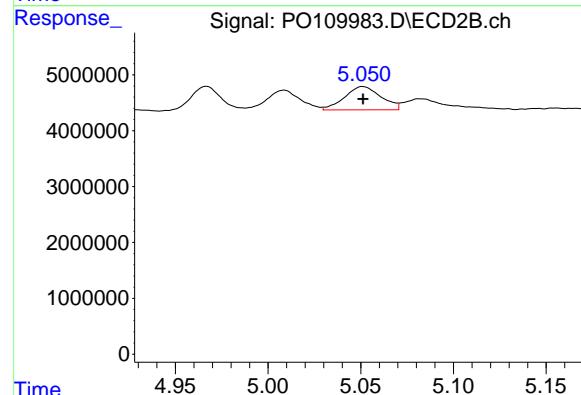


#19 AR-1242-4

R.T.: 4.980 min  
 Delta R.T.: 0.000 min  
 Response: 9228050  
 Conc: 46.26 ng/ml

#19 AR-1242-4

R.T.: 5.051 min  
 Delta R.T.: 0.000 min  
 Response: 5726073  
 Conc: 49.37 ng/ml

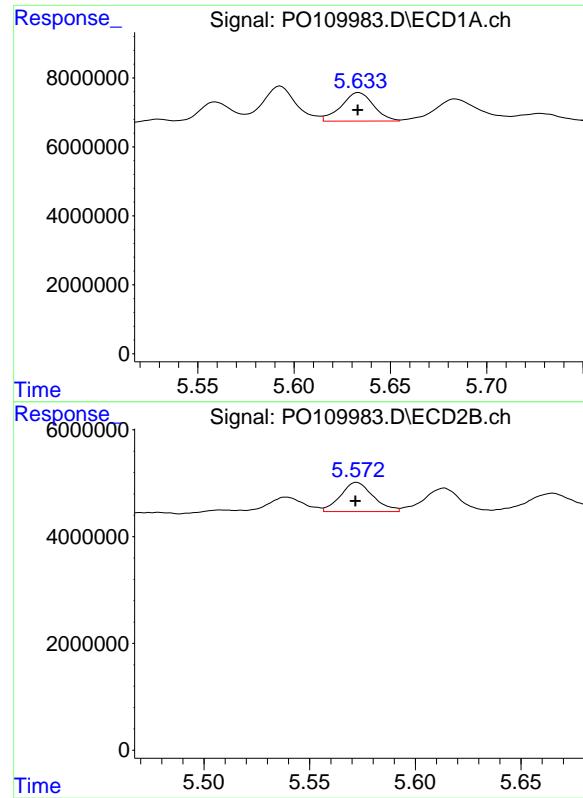

#20 AR-1242-5

R.T.: 5.633 min  
 Delta R.T.: 0.000 min  
 Response: 9633519  
 Conc: 45.77 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1242ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109984.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 17:42  
 Operator : YP/AJ  
 Sample : AR1248ICC1000  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1248ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:07 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.690	3.689	889.7E6	511.9E6	95.913	96.672
2) SA Decachlor...	8.742	8.696	728.0E6	214.7E6	93.393	91.574

Target Compounds

21) L5 AR-1248-1	4.783	4.771	203.2E6	111.3E6	923.985	924.703
22) L5 AR-1248-2	5.022	5.008	271.7E6	153.2E6	902.515	908.902
23) L5 AR-1248-3	5.237	5.050	341.9E6	163.6E6	913.052	913.648
24) L5 AR-1248-4	5.591	5.221	484.7E6	192.0E6	926.318	920.729
25) L5 AR-1248-5	5.633	5.614	341.9E6	189.8E6	924.672	932.015



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109984.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 17:42  
 Operator : YP/AJ  
 Sample : AR1248ICC1000  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1248ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:07 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

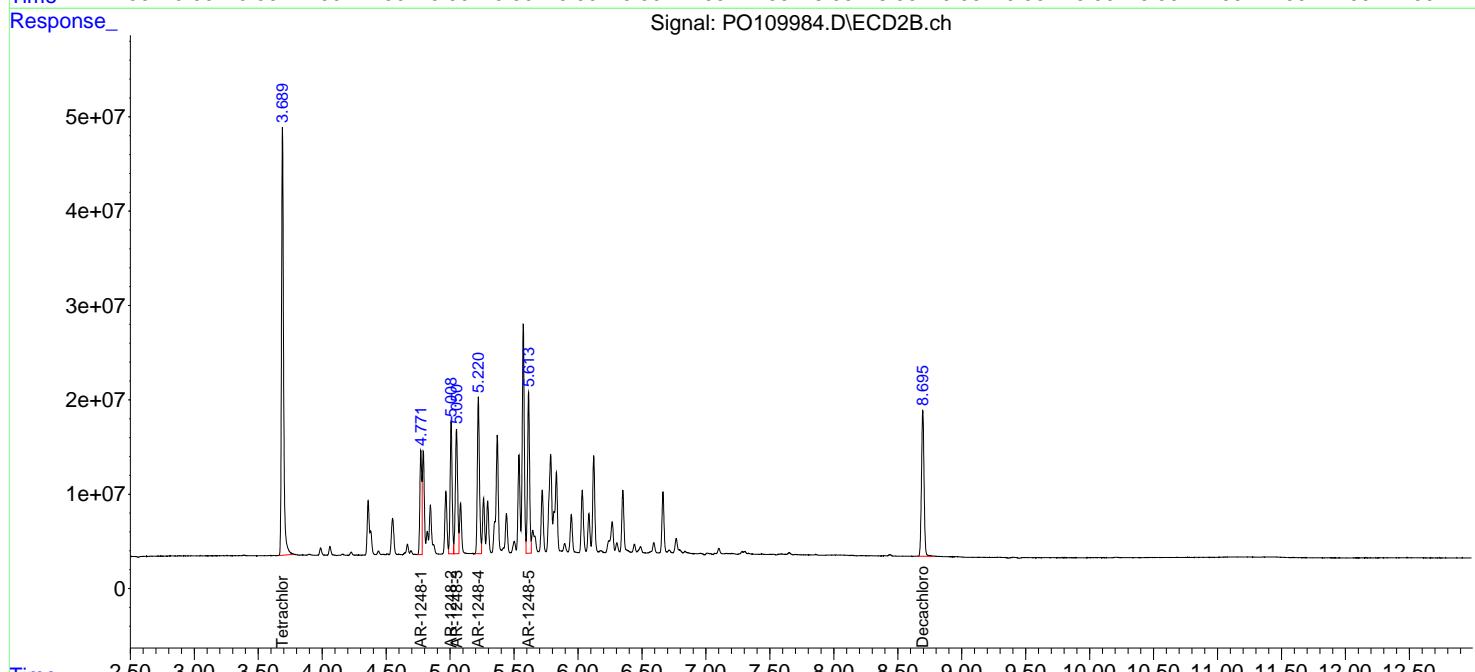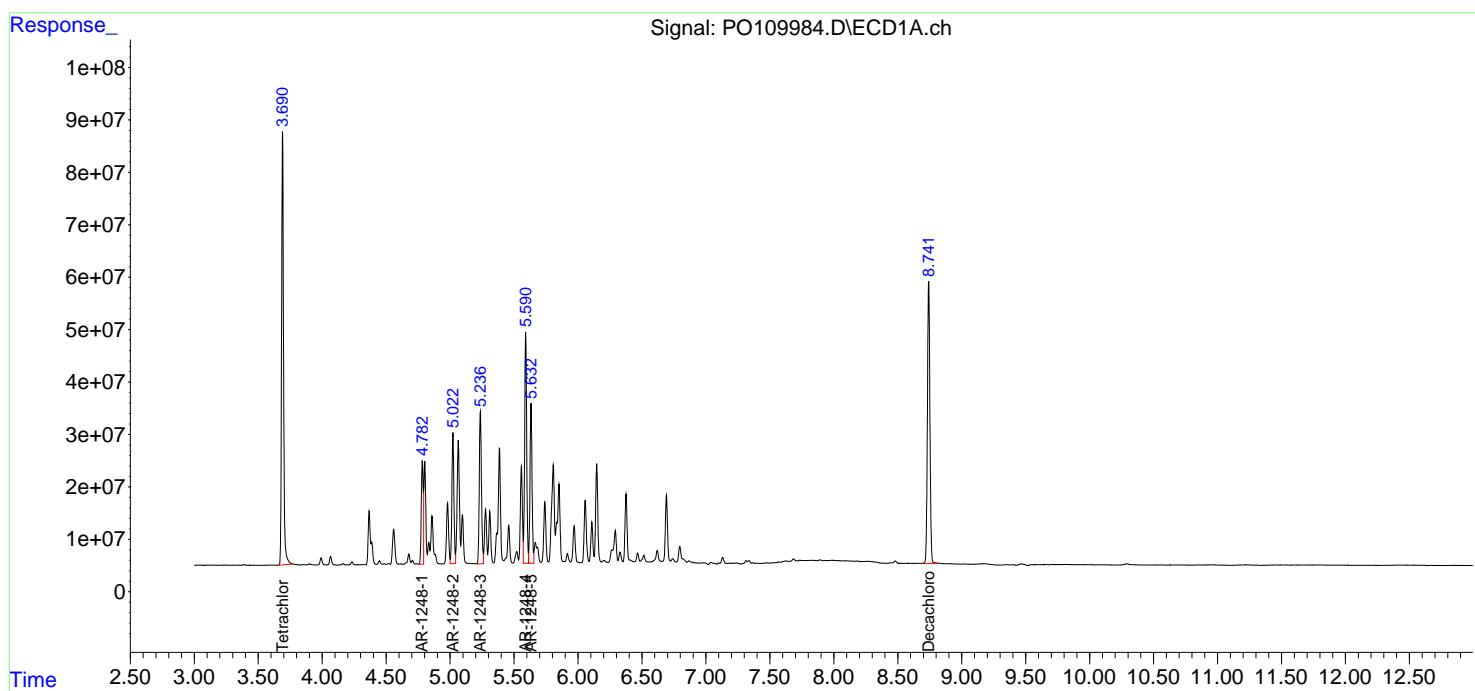

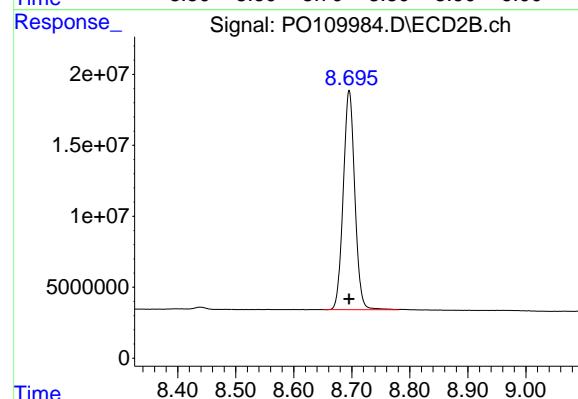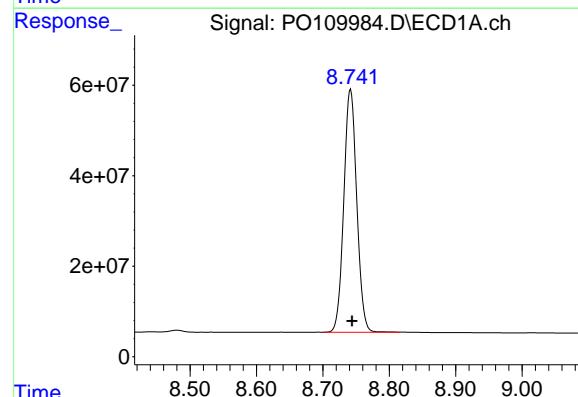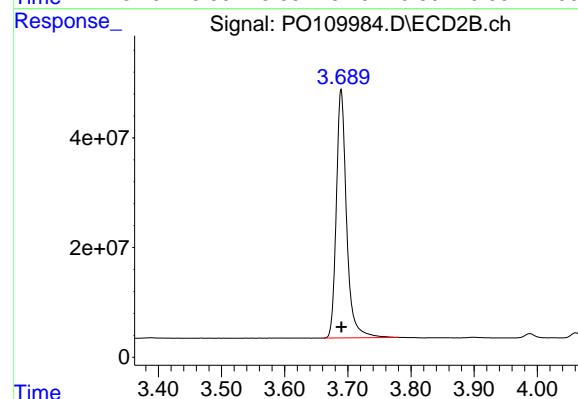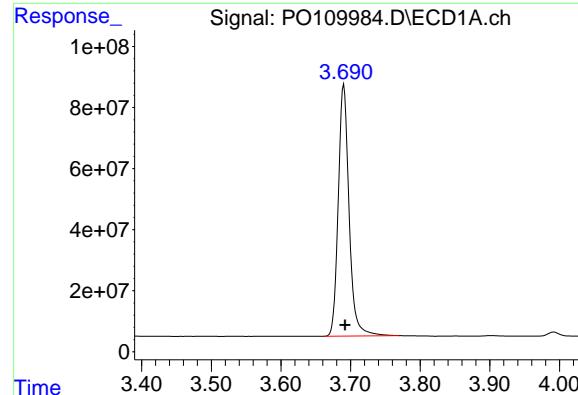

#1 Tetrachloro-m-xylene

R.T.: 3.690 min  
Delta R.T.: -0.002 min  
Response: 889690628  
Conc: 95.91 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1248ICC1000

#1 Tetrachloro-m-xylene


R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 511894308  
Conc: 96.67 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.742 min  
Delta R.T.: -0.002 min  
Response: 727980203  
Conc: 93.39 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 214708362  
Conc: 91.57 ng/ml

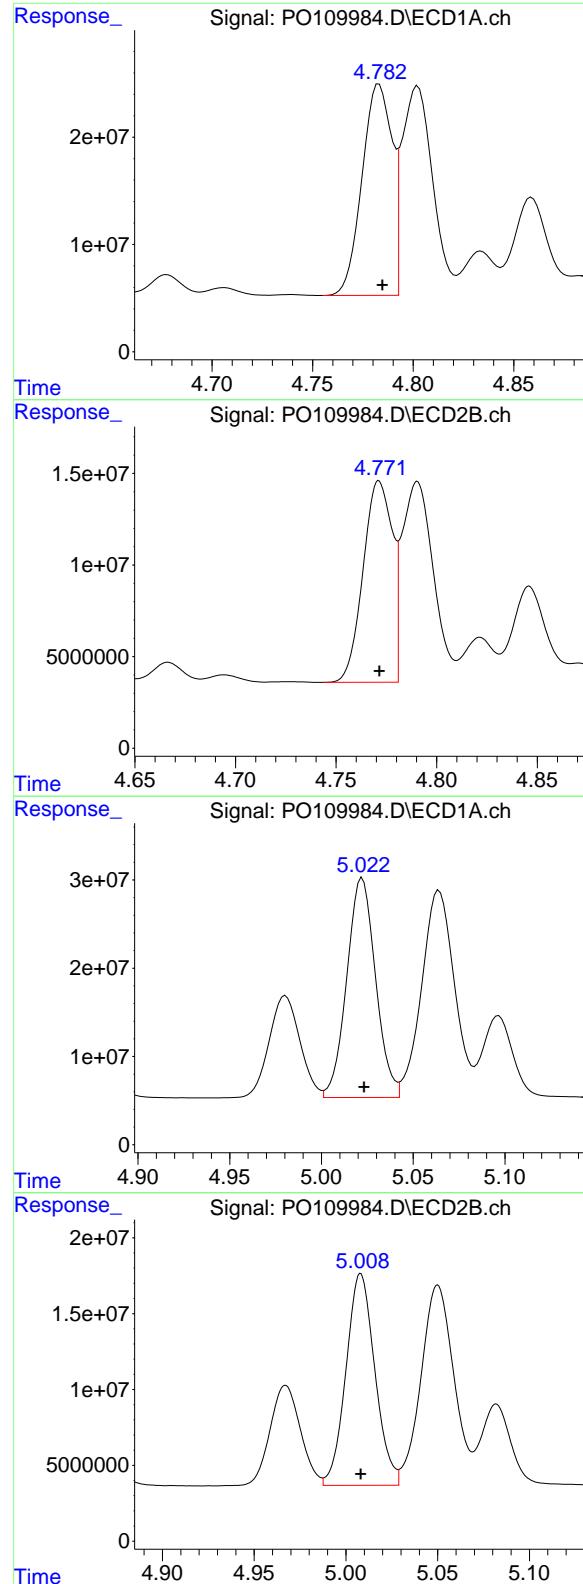

#21 AR-1248-1

R.T.: 4.783 min  
 Delta R.T.: -0.002 min  
 Response: 20322777  
 Conc: 923.99 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1248ICC1000

#21 AR-1248-1

R.T.: 4.771 min  
 Delta R.T.: 0.000 min  
 Response: 111262575  
 Conc: 924.70 ng/ml

#22 AR-1248-2

R.T.: 5.022 min  
 Delta R.T.: -0.001 min  
 Response: 271717932  
 Conc: 902.51 ng/ml


#22 AR-1248-2

R.T.: 5.008 min  
 Delta R.T.: 0.000 min  
 Response: 153166873  
 Conc: 908.90 ng/ml

#23 AR-1248-3


R.T.: 5.237 min  
 Delta R.T.: -0.002 min  
 Response: 341855080  
 Conc: 913.05 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC1000

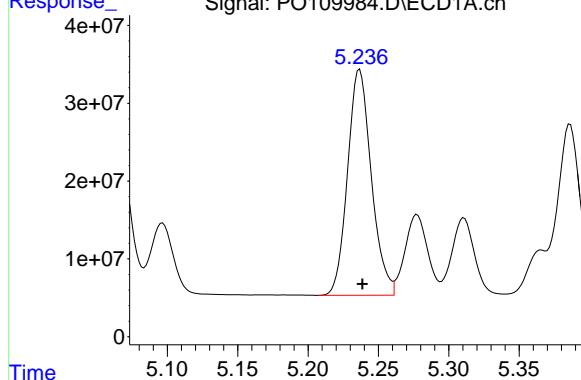


#23 AR-1248-3

R.T.: 5.050 min  
 Delta R.T.: 0.000 min  
 Response: 163639212  
 Conc: 913.65 ng/ml

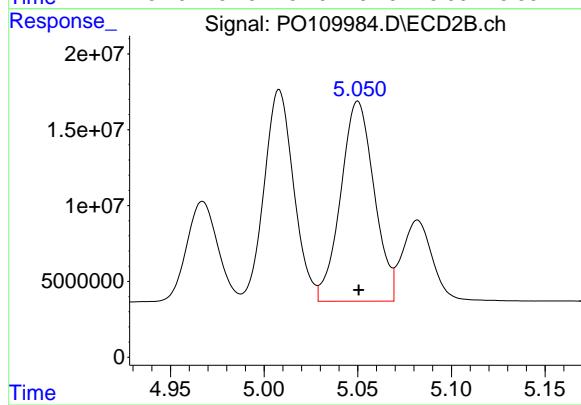


#24 AR-1248-4

R.T.: 5.591 min  
 Delta R.T.: -0.001 min  
 Response: 484718685  
 Conc: 926.32 ng/ml

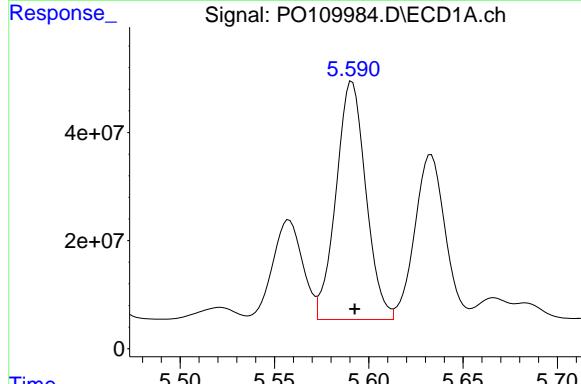

#24 AR-1248-4


R.T.: 5.221 min  
 Delta R.T.: 0.000 min  
 Response: 192034431  
 Conc: 920.73 ng/ml

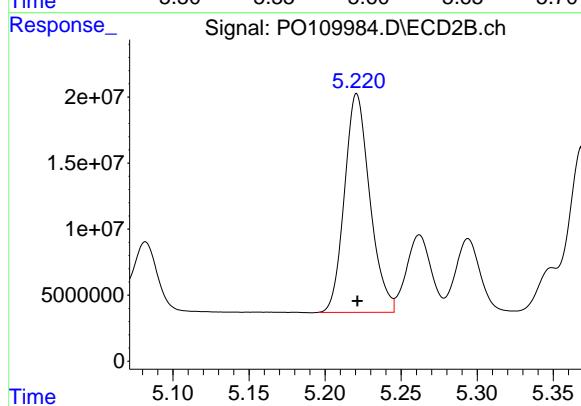

#25 AR-1248-5

R.T.: 5.633 min  
Delta R.T.: -0.001 min  
Response: 341874536  
Conc: 924.67 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1248ICC1000

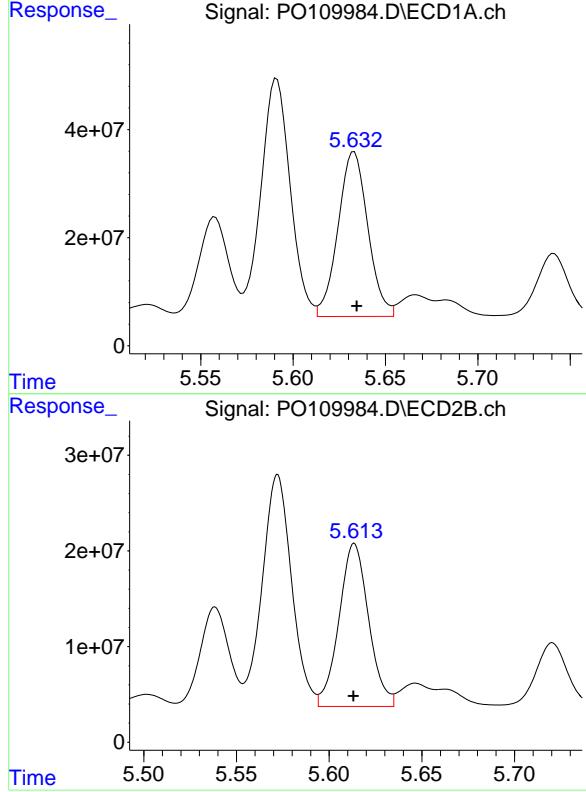

#25 AR-1248-5

R.T.: 5.614 min  
Delta R.T.: 0.000 min  
Response: 189825244  
Conc: 932.02 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109985.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:00  
 Operator : YP/AJ  
 Sample : AR1248ICC750  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1248ICC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:18 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.693	3.690	683.1E6	391.4E6	73.638	73.916
2) SA Decachlor...	8.743	8.696	564.9E6	168.9E6	72.473	72.022

Target Compounds

21) L5 AR-1248-1	4.785	4.772	158.1E6	86749863	718.942	720.978
22) L5 AR-1248-2	5.024	5.009	213.9E6	120.1E6	710.557	712.732
23) L5 AR-1248-3	5.239	5.051	267.9E6	128.2E6	715.615	715.920
24) L5 AR-1248-4	5.593	5.222	377.8E6	150.5E6	721.979	721.526
25) L5 AR-1248-5	5.635	5.614	266.1E6	147.5E6	719.788	724.105



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109985.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:00  
 Operator : YP/AJ  
 Sample : AR1248ICC750  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1248ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:18 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

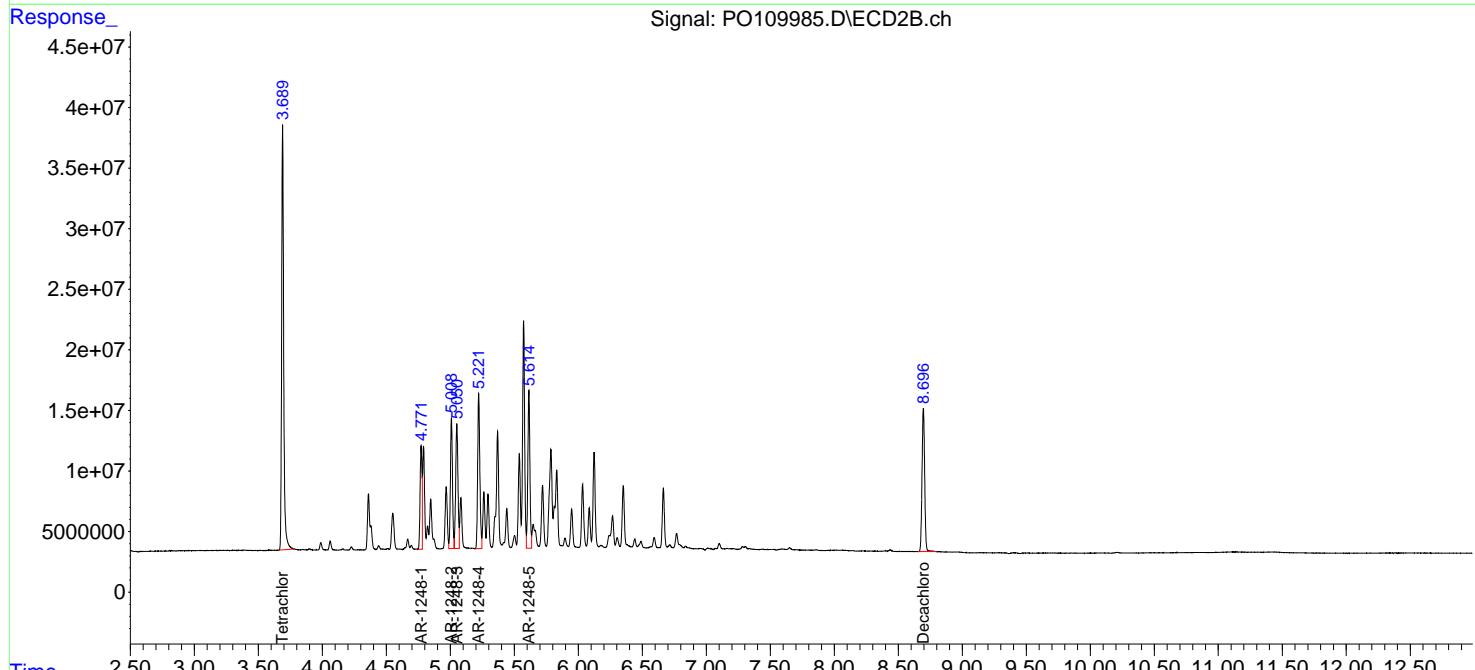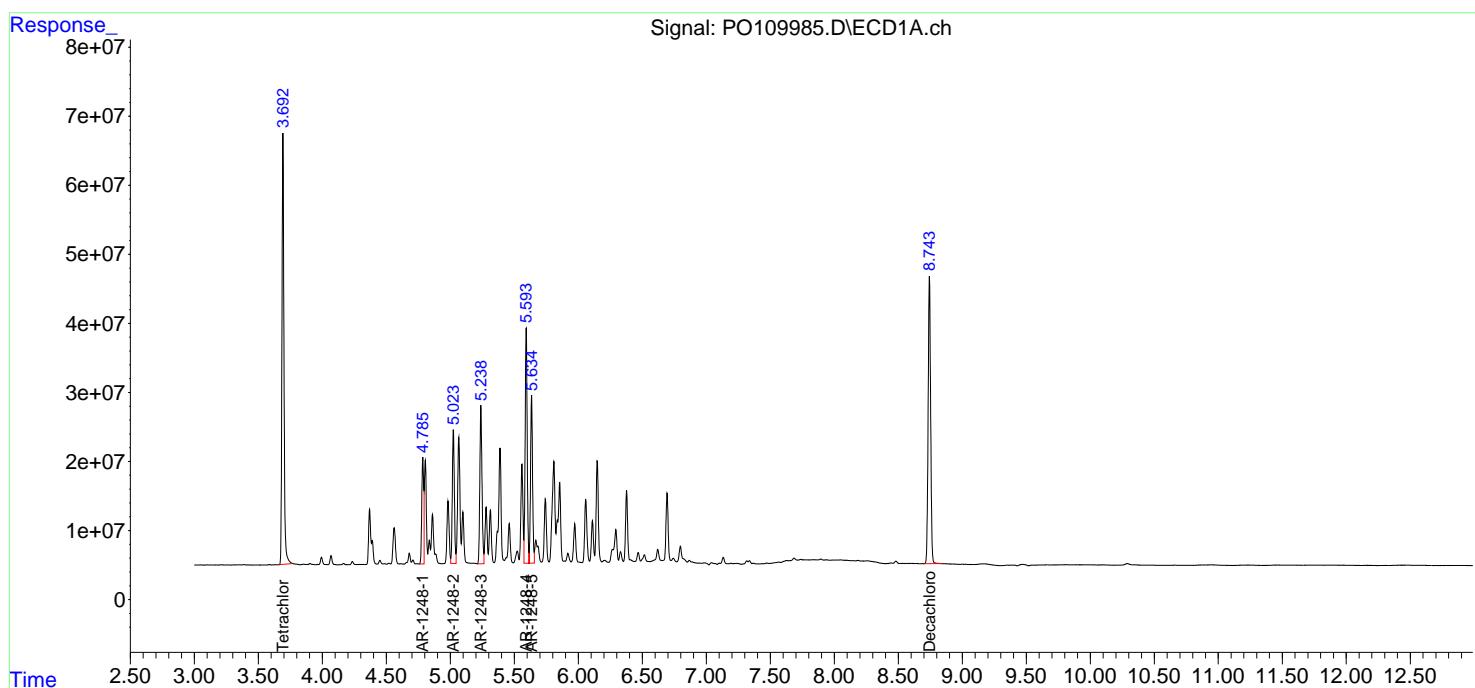

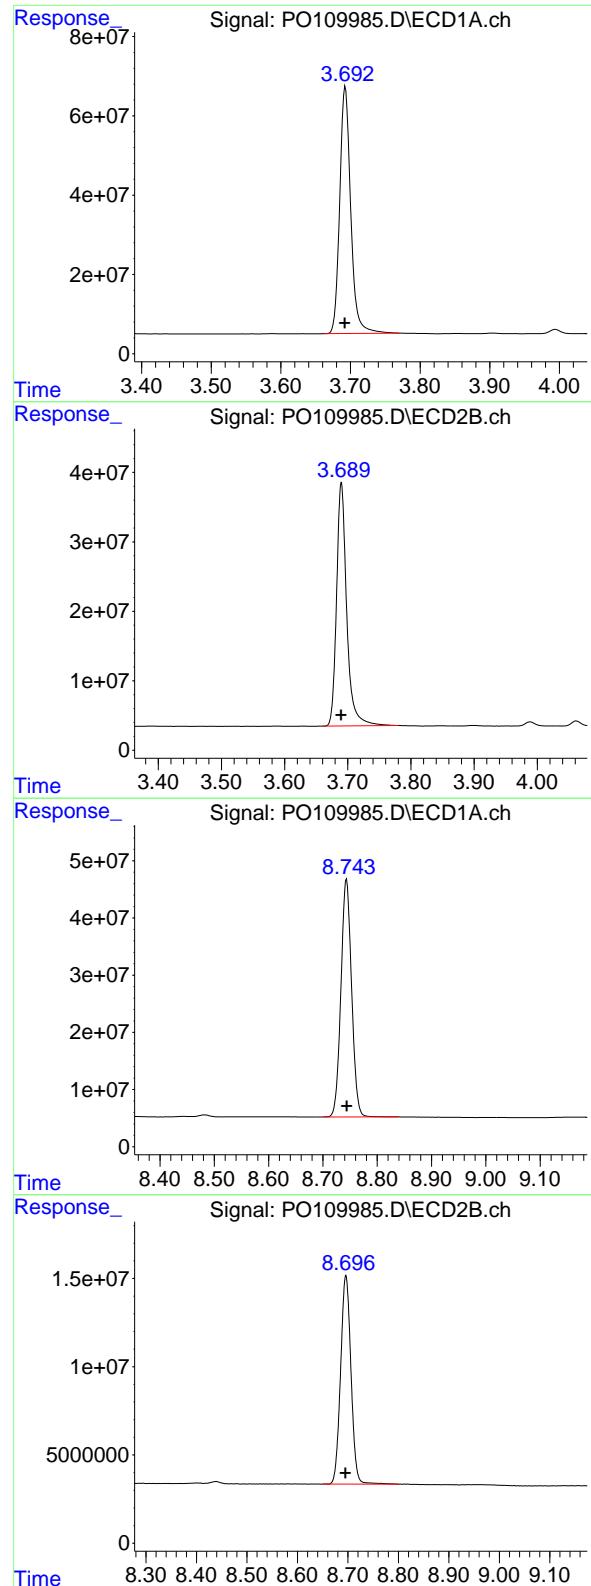

## #1 Tetrachloro-m-xylene

R.T.: 3.693 min  
 Delta R.T.: 0.000 min  
 Response: 683064811  
 Conc: 73.64 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC750

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: 0.000 min  
 Response: 391397784  
 Conc: 73.92 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.743 min  
 Delta R.T.: 0.000 min  
 Response: 564910095  
 Conc: 72.47 ng/ml


## #2 Decachlorobiphenyl

R.T.: 8.696 min  
 Delta R.T.: 0.000 min  
 Response: 168866978  
 Conc: 72.02 ng/ml

#21 AR-1248-1


R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 158125163  
 Conc: 718.94 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC750




#21 AR-1248-1

R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 86749863  
 Conc: 720.98 ng/ml

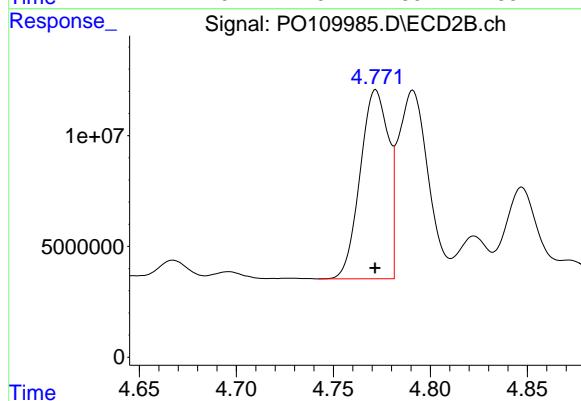


#22 AR-1248-2

R.T.: 5.024 min  
 Delta R.T.: 0.000 min  
 Response: 213925644  
 Conc: 710.56 ng/ml

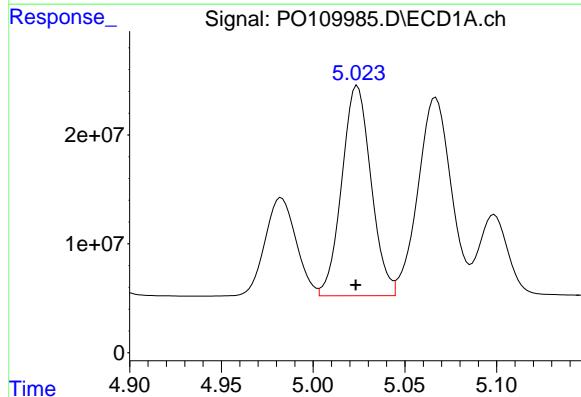

#22 AR-1248-2


R.T.: 5.009 min  
 Delta R.T.: 0.000 min  
 Response: 120108575  
 Conc: 712.73 ng/ml

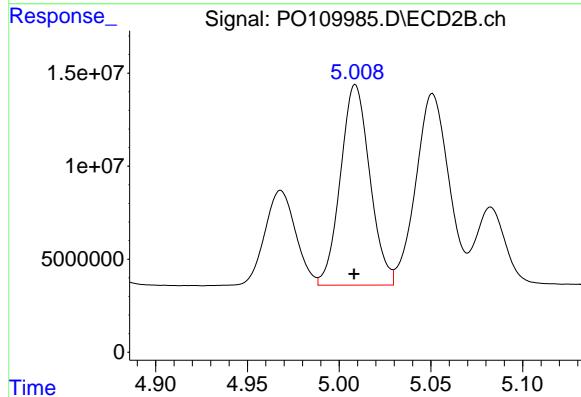

#23 AR-1248-3


R.T.: 5.239 min  
 Delta R.T.: 0.000 min  
 Response: 267932599  
 Conc: 715.61 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC750




#23 AR-1248-3

R.T.: 5.051 min  
 Delta R.T.: 0.000 min  
 Response: 128225021  
 Conc: 715.92 ng/ml

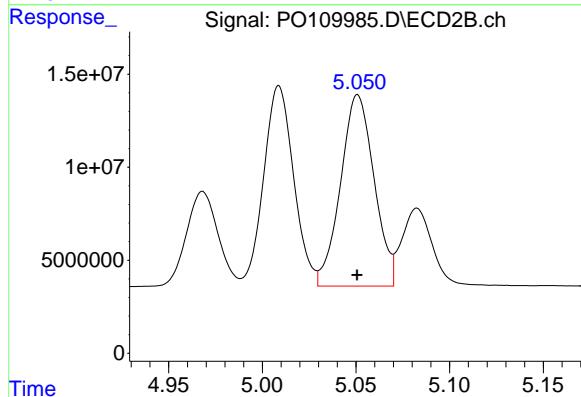


#24 AR-1248-4

R.T.: 5.593 min  
 Delta R.T.: 0.000 min  
 Response: 377793460  
 Conc: 721.98 ng/ml

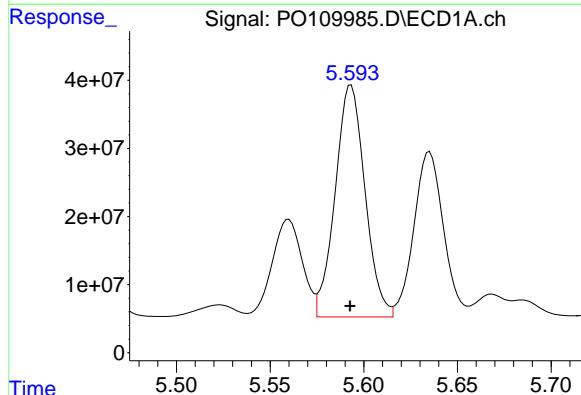

#24 AR-1248-4



R.T.: 5.222 min  
 Delta R.T.: 0.000 min  
 Response: 150486943  
 Conc: 721.53 ng/ml

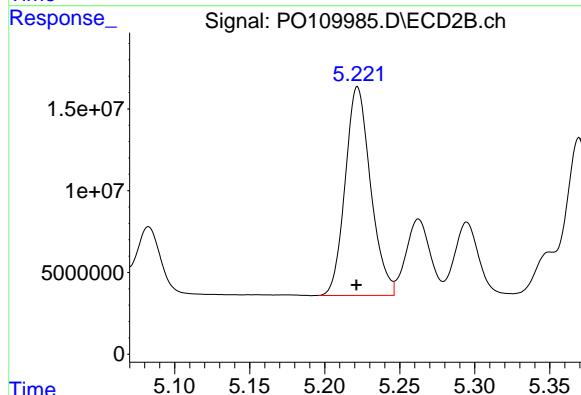

#25 AR-1248-5

R.T.: 5.635 min  
Delta R.T.: 0.000 min  
Response: 266123735  
Conc: 719.79 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1248ICC750

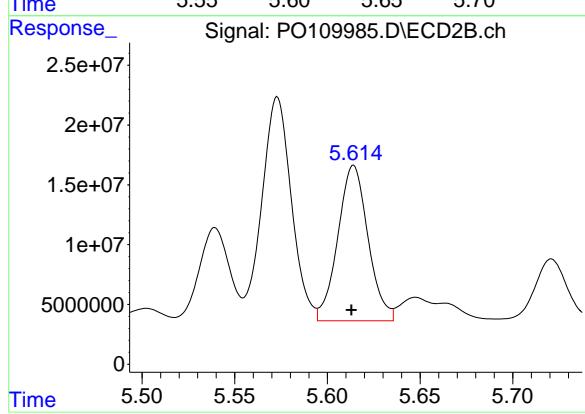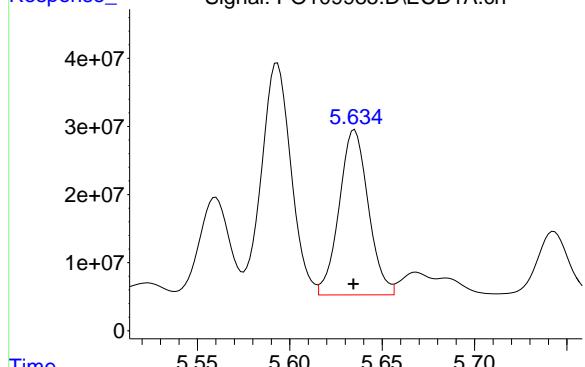

#25 AR-1248-5

R.T.: 5.614 min  
Delta R.T.: 0.001 min  
Response: 147479675  
Conc: 724.10 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109986.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:19  
 Operator : YP/AJ  
 Sample : AR1248ICC500  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1248ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:30 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	463.8E6	264.8E6	50.000	50.000
2) SA Decachlor...	8.744	8.695	389.7E6	117.2E6	50.000	50.000

Target Compounds

21) L5 AR-1248-1	4.785	4.771	110.0E6	60161217	500.000	500.000
22) L5 AR-1248-2	5.023	5.008	150.5E6	84259256	500.000	500.000
23) L5 AR-1248-3	5.239	5.051	187.2E6	89552637	500.000	500.000
24) L5 AR-1248-4	5.593	5.221	261.6E6	104.3E6	500.000	500.000
25) L5 AR-1248-5	5.634	5.613	184.9E6	101.8E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109986.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:19  
 Operator : YP/AJ  
 Sample : AR1248ICC500  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1248ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:30 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

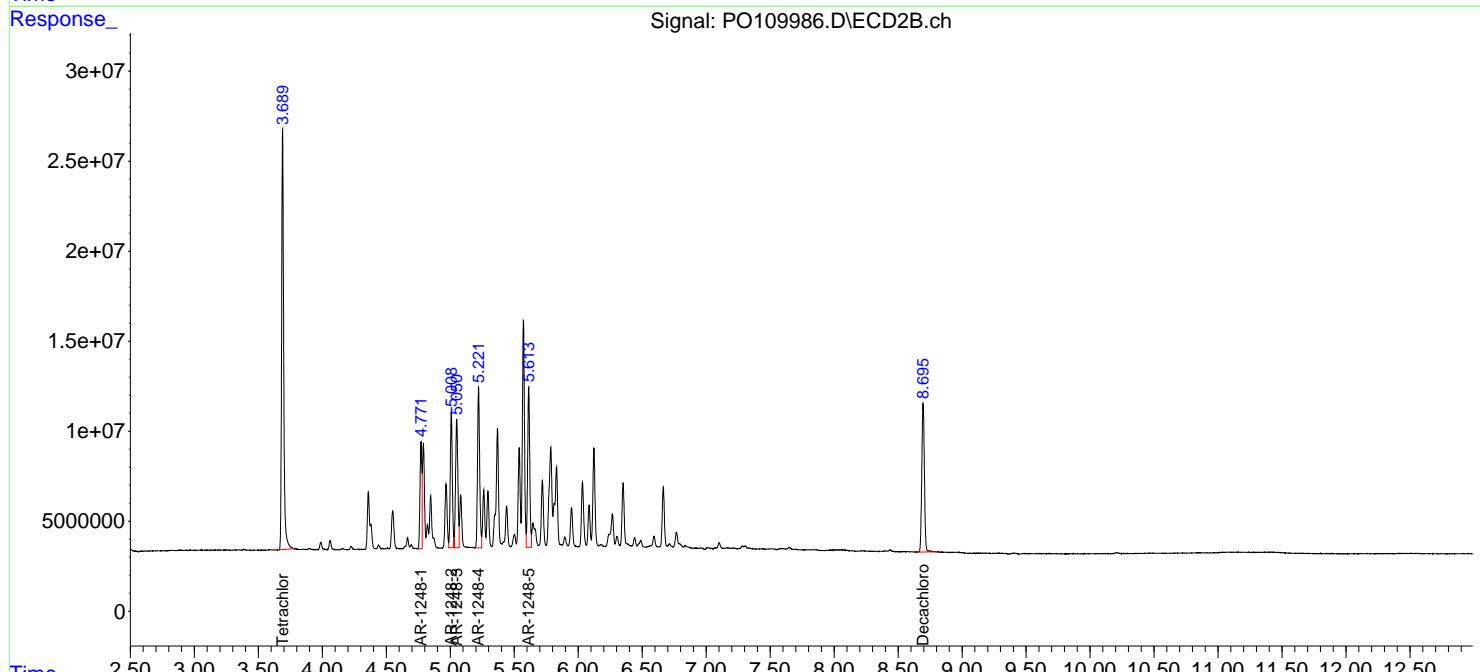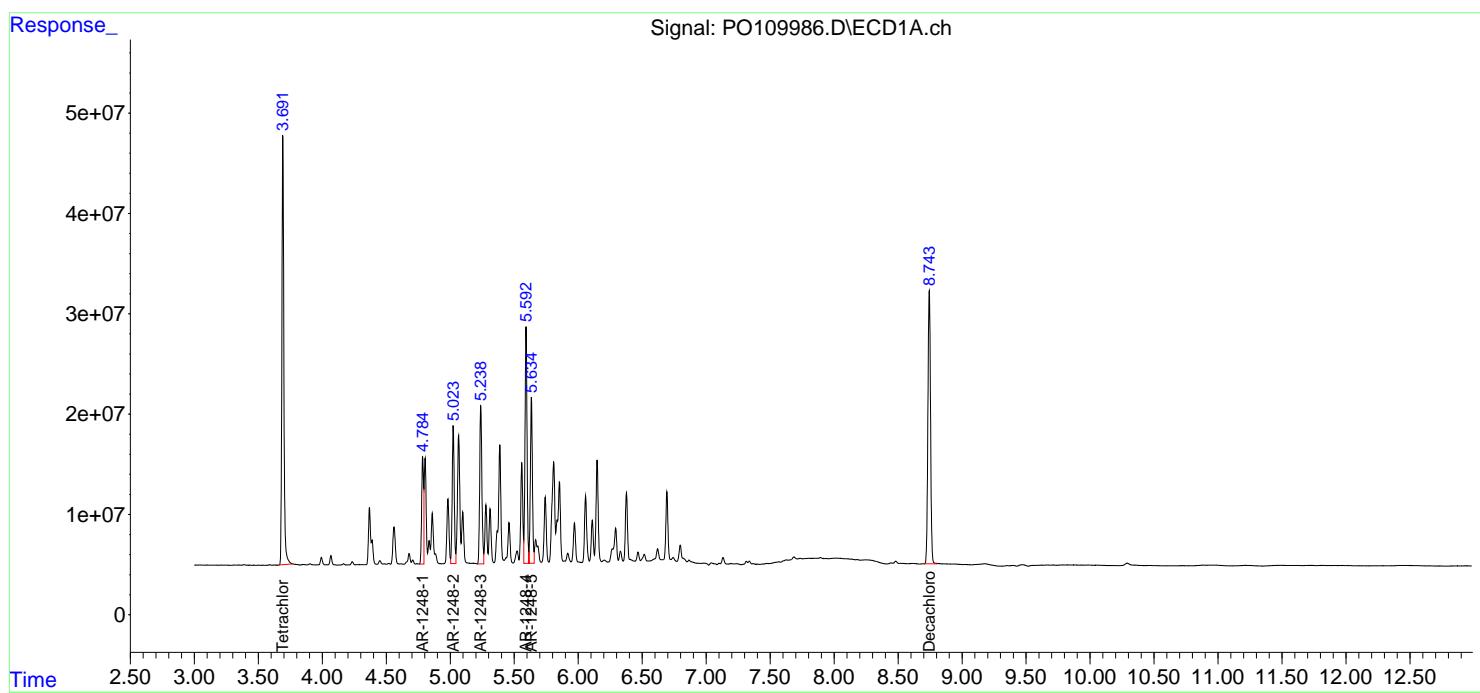

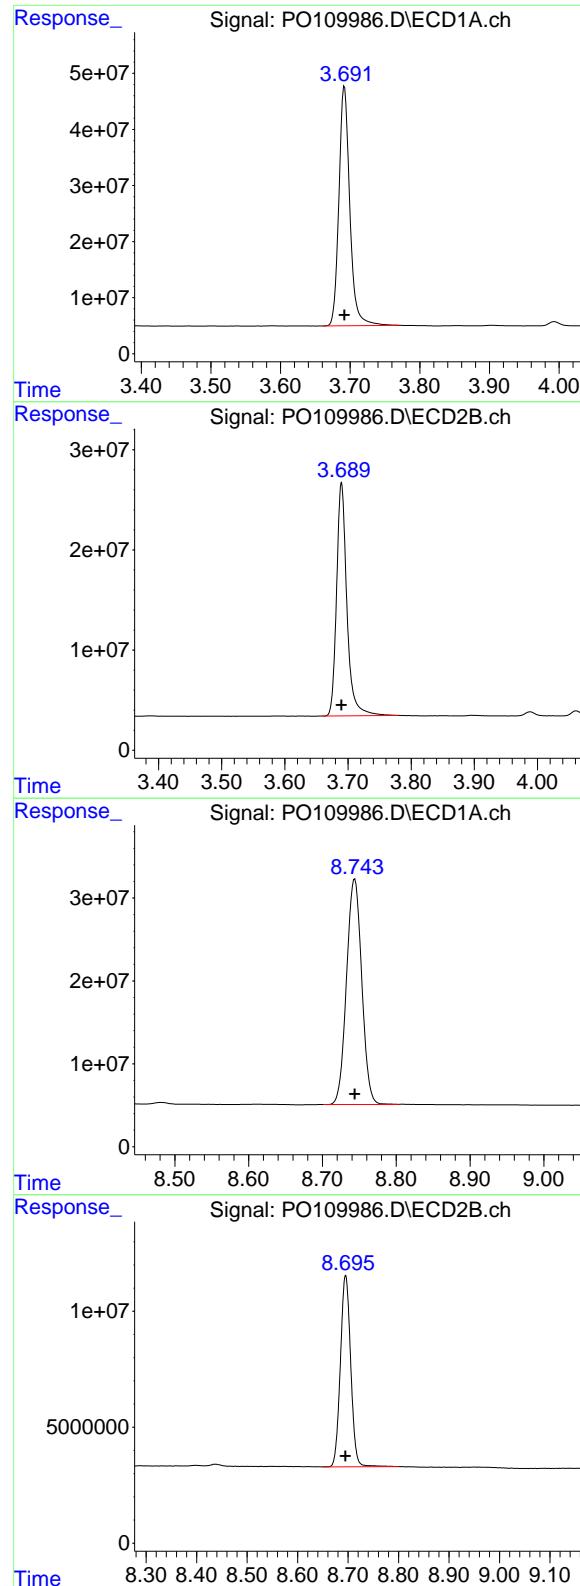

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
 Delta R.T.: 0.000 min  
 Response: 463799489  
 Conc: 50.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC500

## #1 Tetrachloro-m-xylene


R.T.: 3.690 min  
 Delta R.T.: 0.000 min  
 Response: 264757687  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
 Delta R.T.: 0.000 min  
 Response: 389738327  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.695 min  
 Delta R.T.: 0.000 min  
 Response: 117232791  
 Conc: 50.00 ng/ml

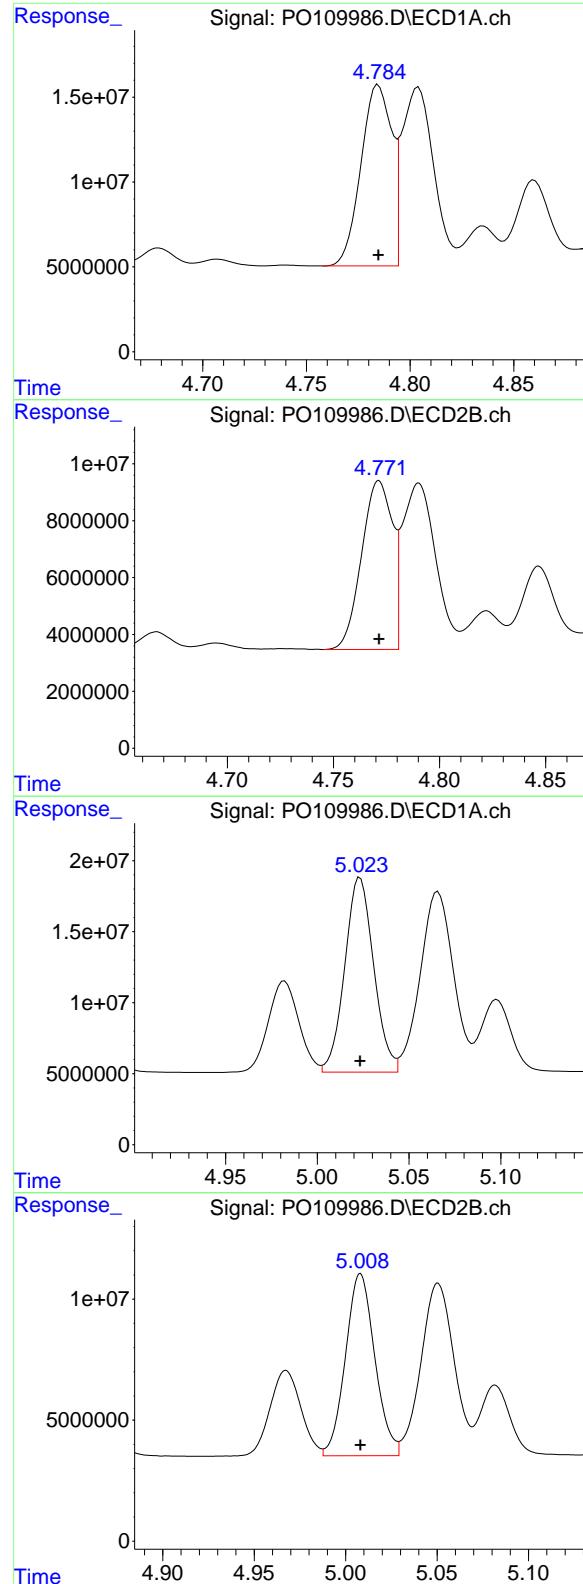

#21 AR-1248-1

R.T.: 4.785 min  
Delta R.T.: 0.000 min  
Response: 109970762  
Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC500

#21 AR-1248-1


R.T.: 4.771 min  
Delta R.T.: 0.000 min  
Response: 60161217  
Conc: 500.00 ng/ml

#22 AR-1248-2

R.T.: 5.023 min  
Delta R.T.: 0.000 min  
Response: 150533799  
Conc: 500.00 ng/ml

#22 AR-1248-2

R.T.: 5.008 min  
Delta R.T.: 0.000 min  
Response: 84259256  
Conc: 500.00 ng/ml

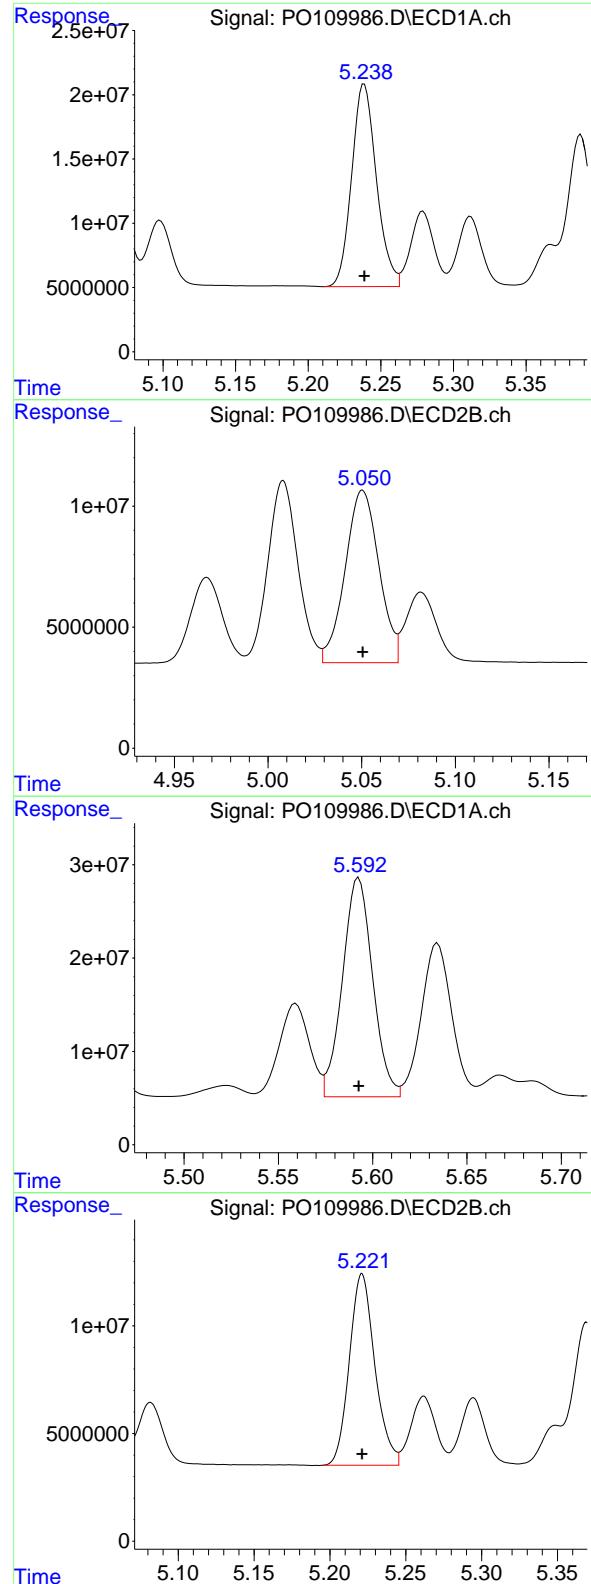

#23 AR-1248-3

R.T.: 5.239 min  
 Delta R.T.: 0.000 min  
**Instrument:**  
 Response: 187204562 ECD\_O  
 Conc: 500.00 ng/ml ClientSampleId :  
 AR1248ICC500

#23 AR-1248-3

R.T.: 5.051 min  
 Delta R.T.: 0.000 min  
 Response: 89552637  
 Conc: 500.00 ng/ml

#24 AR-1248-4

R.T.: 5.593 min  
 Delta R.T.: 0.000 min  
 Response: 261637332  
 Conc: 500.00 ng/ml


#24 AR-1248-4

R.T.: 5.221 min  
 Delta R.T.: 0.000 min  
 Response: 104283869  
 Conc: 500.00 ng/ml

#25 AR-1248-5

R.T.: 5.634 min  
Delta R.T.: 0.000 min  
Response: 184862645  
Conc: 500.00 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1248ICC500

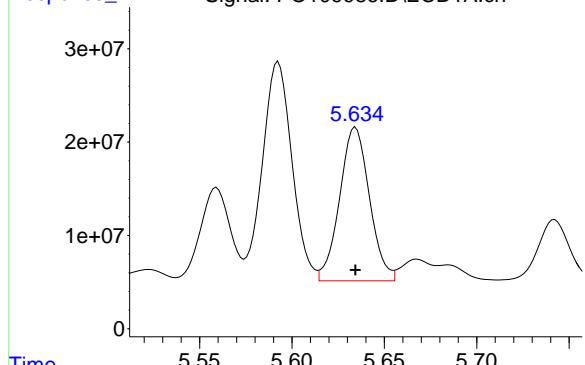

#25 AR-1248-5

R.T.: 5.613 min  
Delta R.T.: 0.000 min  
Response: 101835896  
Conc: 500.00 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109987.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:37  
 Operator : YP/AJ  
 Sample : AR1248ICC250  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1248ICC250

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:44 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.689	234.4E6	134.2E6	25.266	25.339
2) SA Decachlor...	8.744	8.695	202.8E6	63399780	26.017	27.040

Target Compounds

21) L5 AR-1248-1	4.784	4.771	57869632	31675925	263.114	263.259
22) L5 AR-1248-2	5.023	5.008	80049855	44958781	265.887	266.788
23) L5 AR-1248-3	5.238	5.050	98806066	47928872	263.899	267.602
24) L5 AR-1248-4	5.592	5.221	136.0E6	55764342	259.818	267.368
25) L5 AR-1248-5	5.634	5.613	96853624	53959011	261.961	264.931



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109987.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:37  
 Operator : YP/AJ  
 Sample : AR1248ICC250  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1248ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:44 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

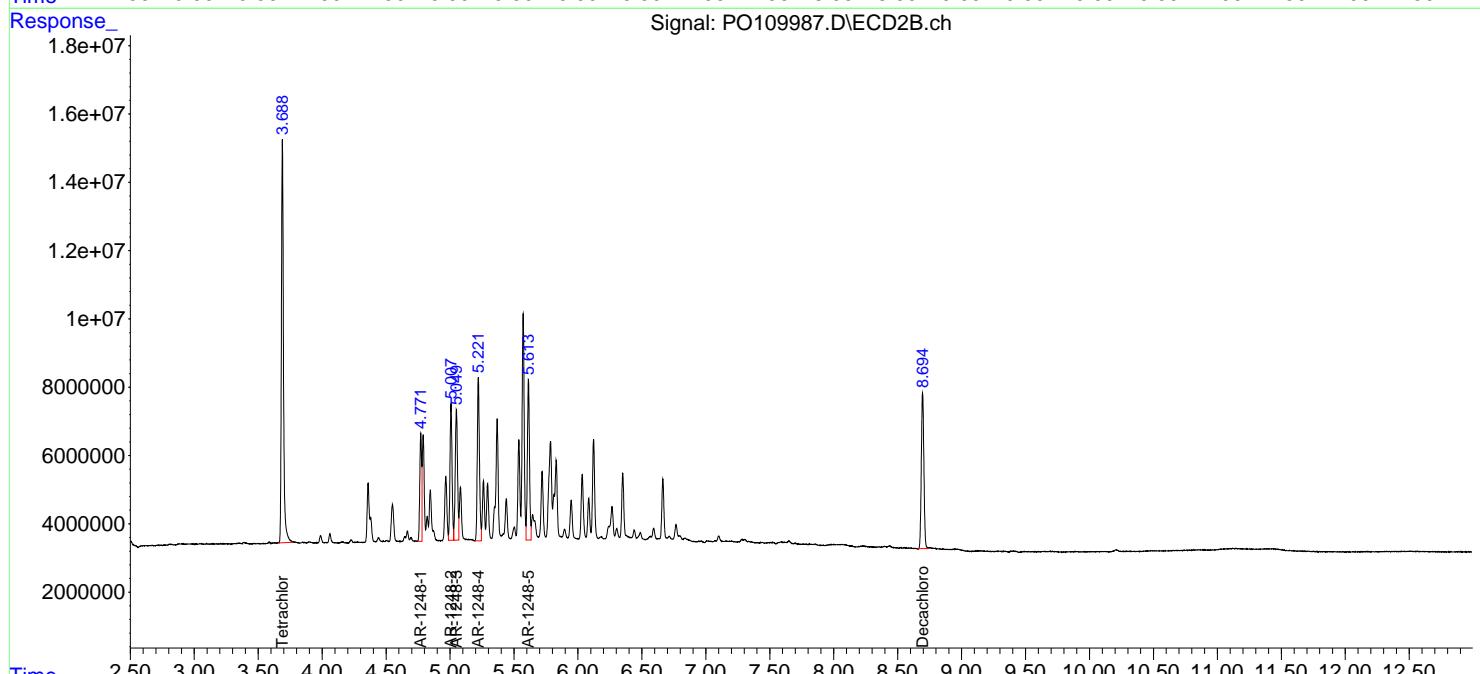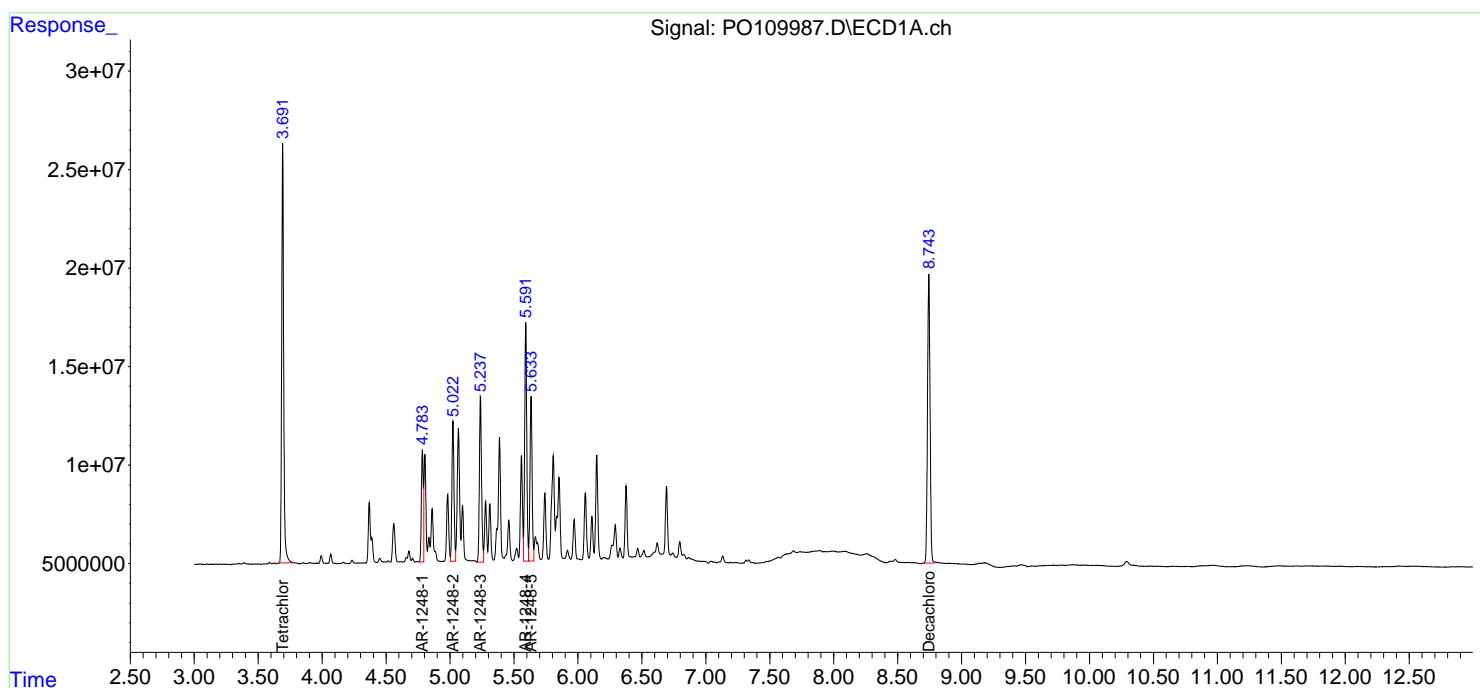

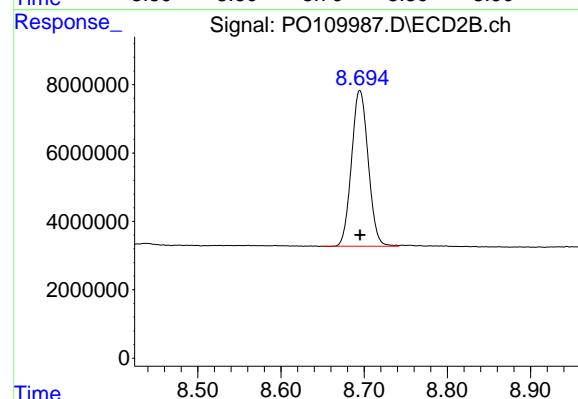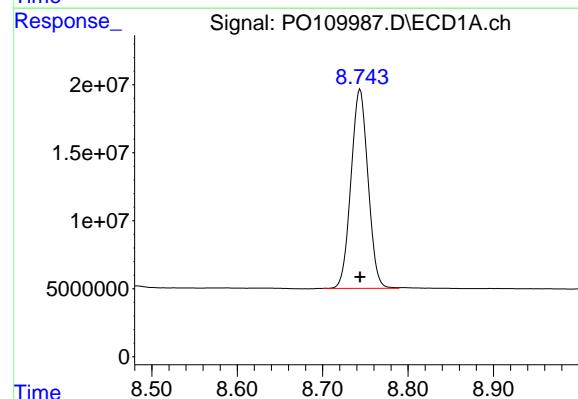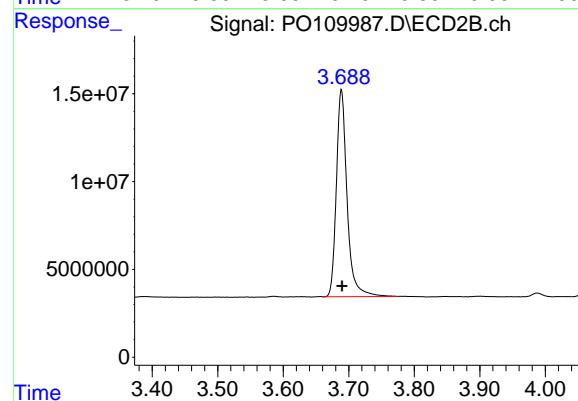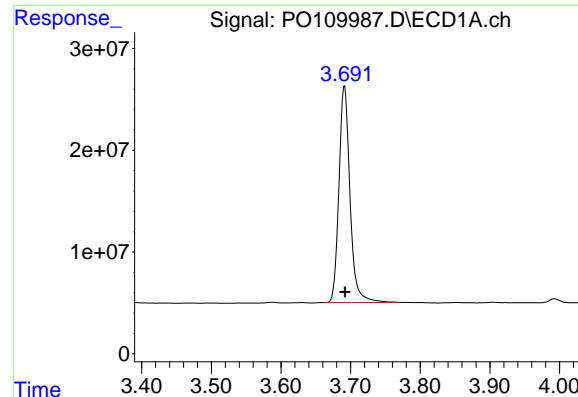

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: 0.000 min  
 Response: 234365223  
 Conc: 25.27 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1248ICC250

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
 Delta R.T.: 0.000 min  
 Response: 134173646  
 Conc: 25.34 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
 Delta R.T.: 0.000 min  
 Response: 202795797  
 Conc: 26.02 ng/ml


## #2 Decachlorobiphenyl

R.T.: 8.695 min  
 Delta R.T.: 0.000 min  
 Response: 63399780  
 Conc: 27.04 ng/ml

#21 AR-1248-1


R.T.: 4.784 min  
 Delta R.T.: 0.000 min  
 Response: 57869632  
 Conc: 263.11 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC250

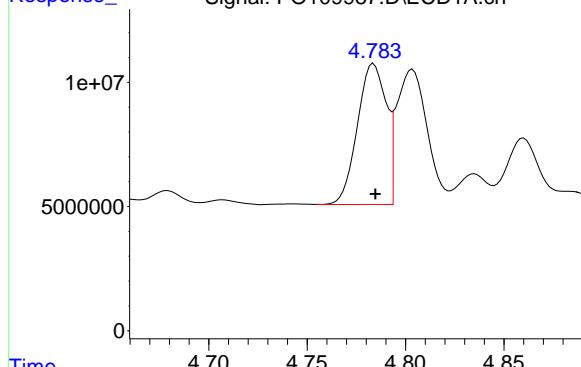


#21 AR-1248-1

R.T.: 4.771 min  
 Delta R.T.: 0.000 min  
 Response: 31675925  
 Conc: 263.26 ng/ml

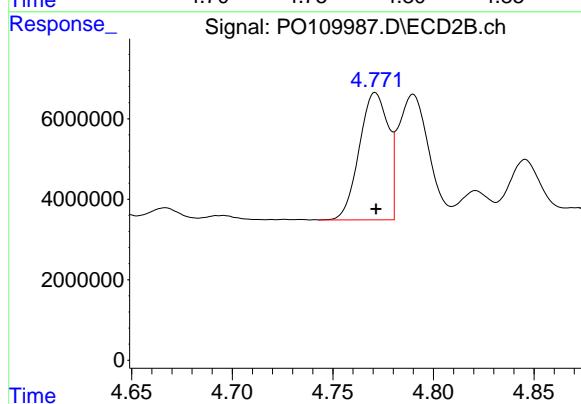


#22 AR-1248-2

R.T.: 5.023 min  
 Delta R.T.: 0.000 min  
 Response: 80049855  
 Conc: 265.89 ng/ml

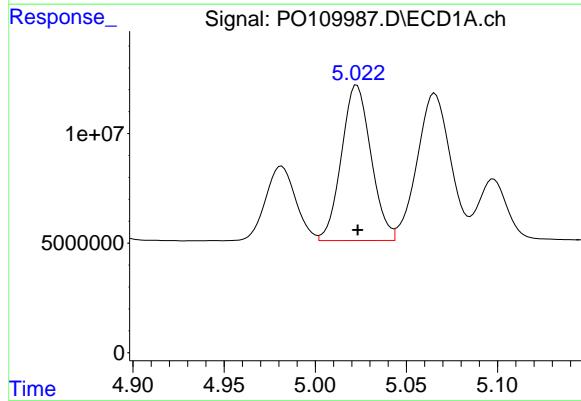

#22 AR-1248-2





R.T.: 5.008 min  
 Delta R.T.: 0.000 min  
 Response: 44958781  
 Conc: 266.79 ng/ml

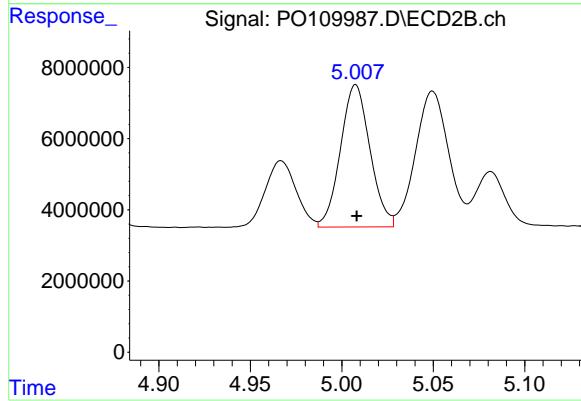

#23 AR-1248-3

R.T.: 5.238 min  
 Delta R.T.: 0.000 min  
 Response: 98806066  
 Conc: 263.90 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC250

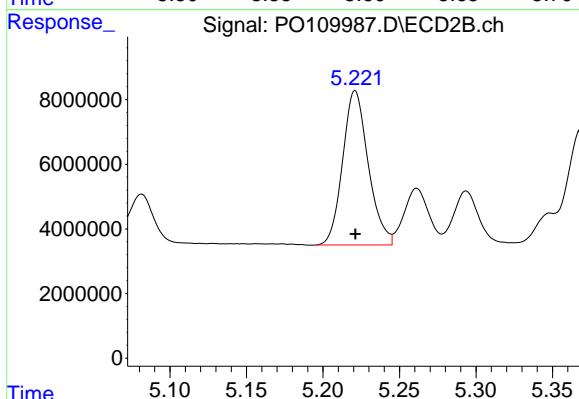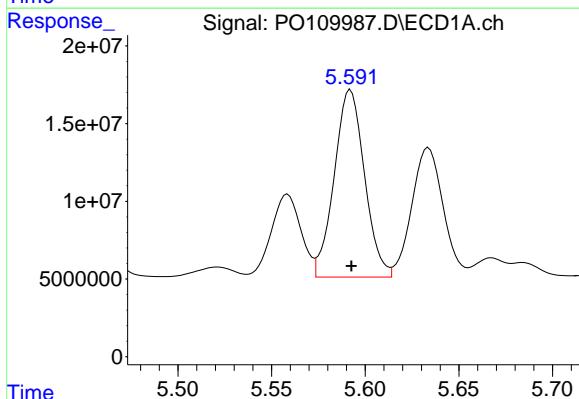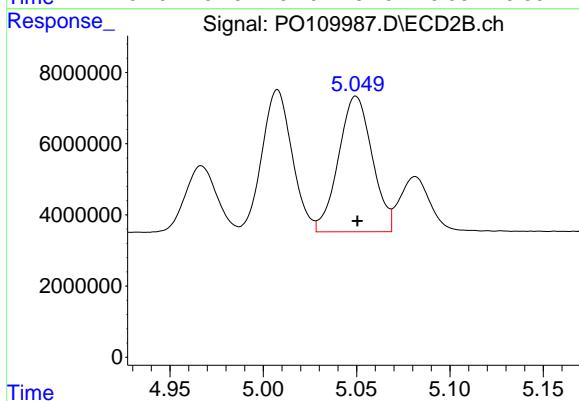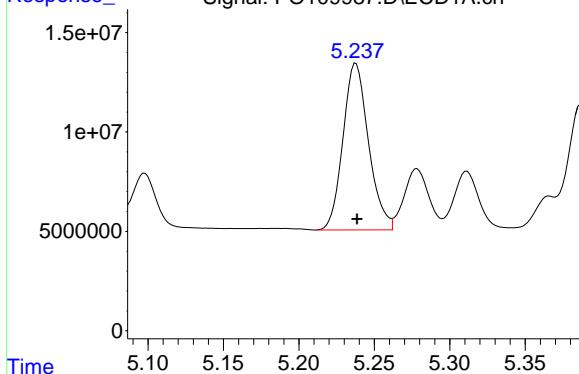

#23 AR-1248-3

R.T.: 5.050 min  
 Delta R.T.: 0.000 min  
 Response: 47928872  
 Conc: 267.60 ng/ml


#24 AR-1248-4

R.T.: 5.592 min  
 Delta R.T.: 0.000 min  
 Response: 135956218  
 Conc: 259.82 ng/ml

#24 AR-1248-4

R.T.: 5.221 min  
 Delta R.T.: 0.000 min  
 Response: 55764342  
 Conc: 267.37 ng/ml

#25 AR-1248-5

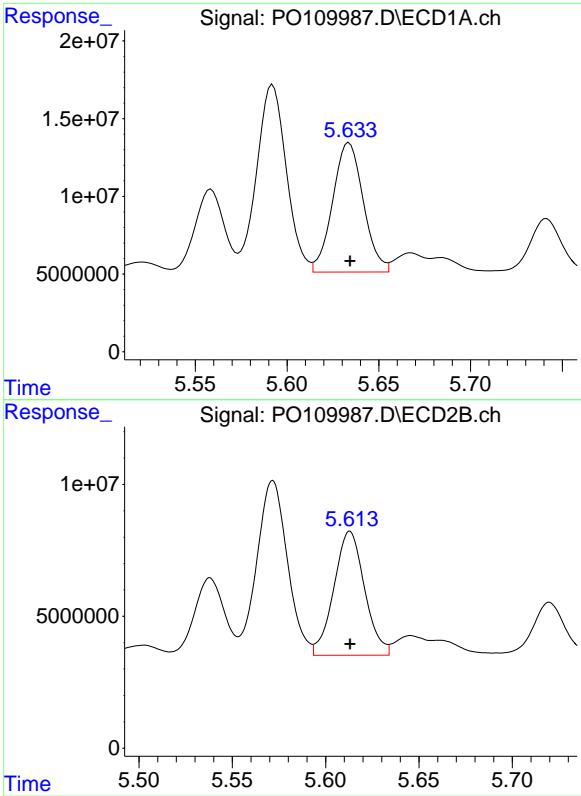

R.T.: 5.634 min  
Delta R.T.: 0.000 min  
Response: 96853624  
Conc: 261.96 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1248ICC250

#25 AR-1248-5

R.T.: 5.613 min  
Delta R.T.: 0.000 min  
Response: 53959011  
Conc: 264.93 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109988.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:54  
 Operator : YP/AJ  
 Sample : AR1248ICC050  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1248ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	3.690	3.689	43788277	25352976	4.721	4.788
2) SA Decachlor...	8.742	8.695	41310164	13029410	5.300	5.557

**Target Compounds**

21) L5 AR-1248-1	4.782	4.771	11846805	6686511	53.863	55.572
22) L5 AR-1248-2	5.021	5.008	16385888	9031427	54.426	53.593
23) L5 AR-1248-3	5.235	5.050	19860582	10026048	53.045m	55.979
24) L5 AR-1248-4	5.591	5.221	29227773	11398927	55.856	54.653m
25) L5 AR-1248-5	5.632	5.613	20545156	11669383	55.569	57.295

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109988.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:54  
 Operator : YP/AJ  
 Sample : AR1248ICC050  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 AR1248ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

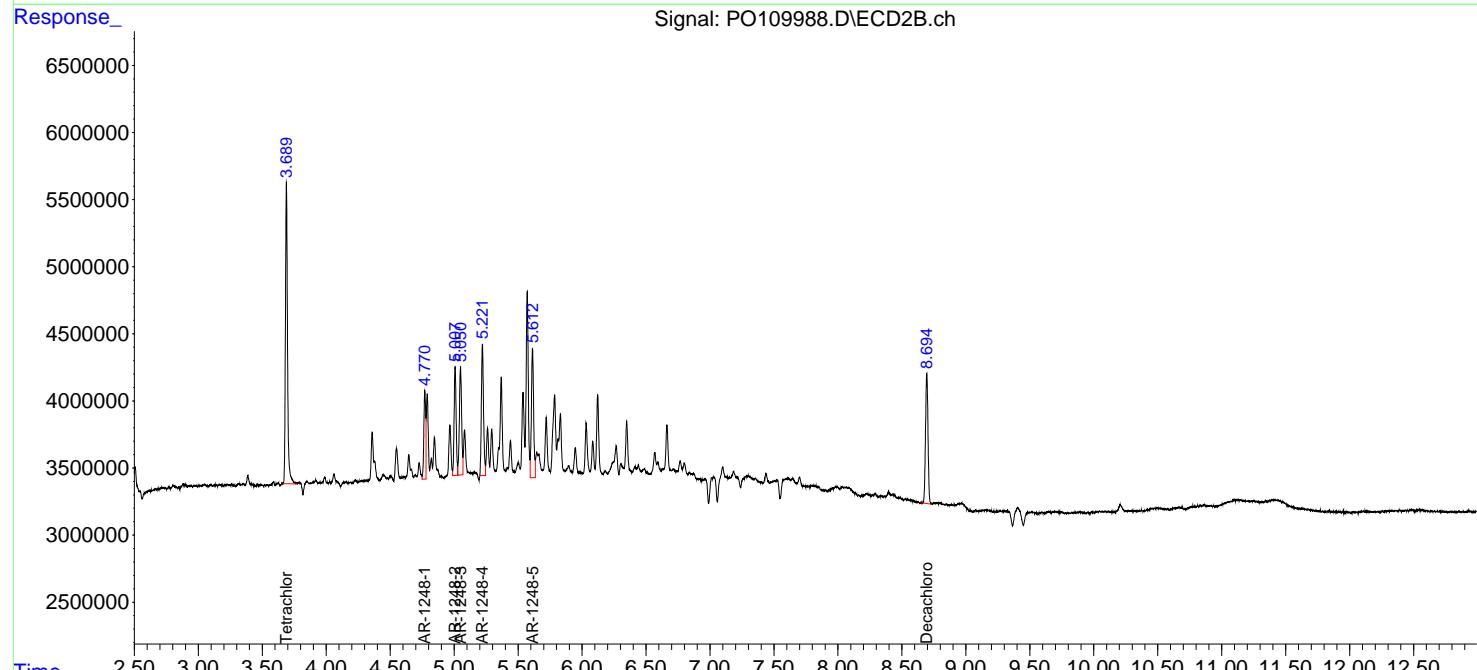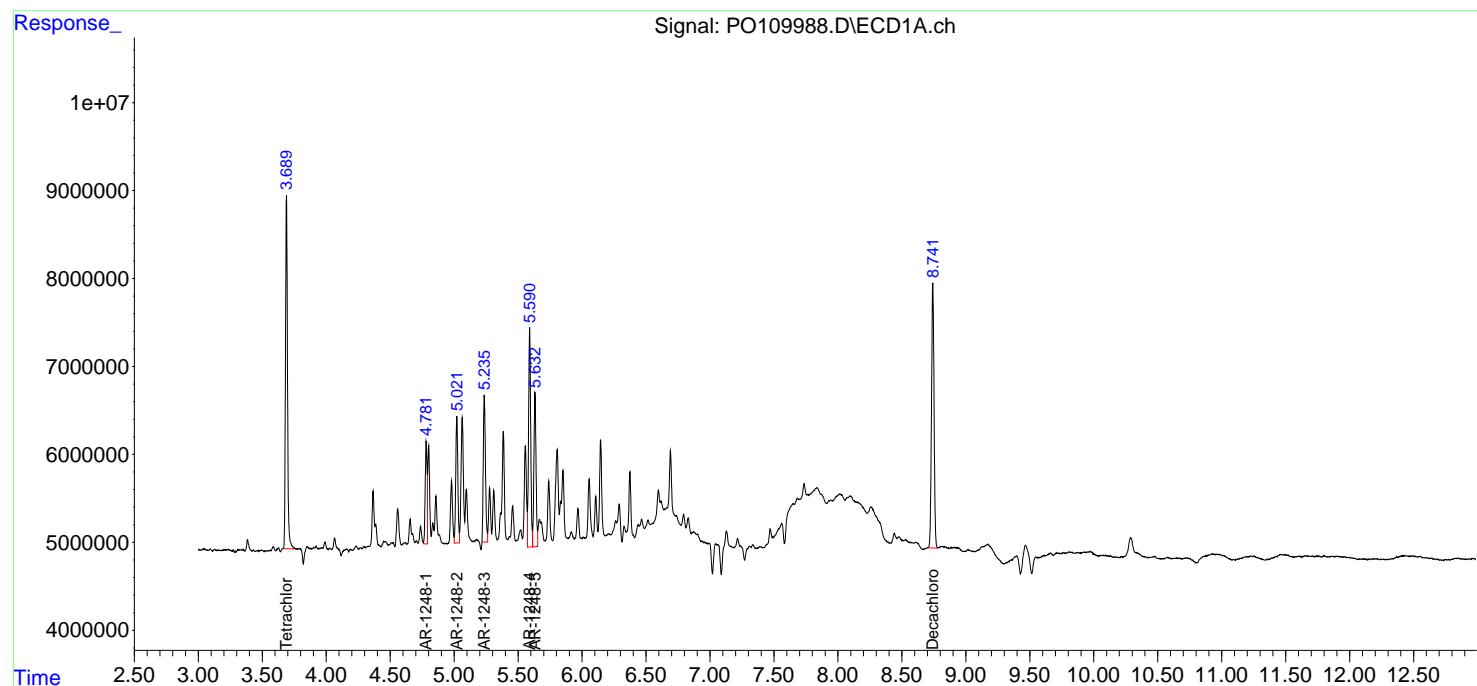




## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
Delta R.T.: -0.002 min  
Response: 43788277  
Conc: 4.72 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1248ICC050


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

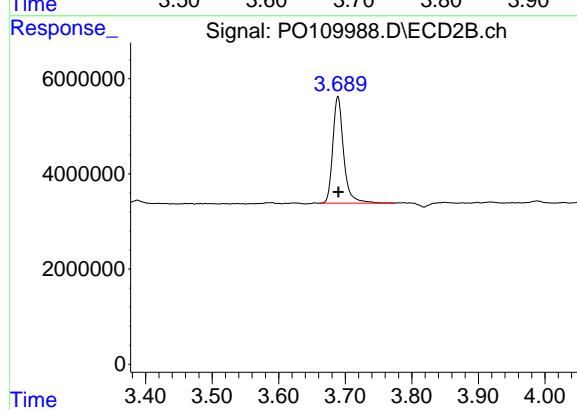


## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 25352976  
Conc: 4.79 ng/ml

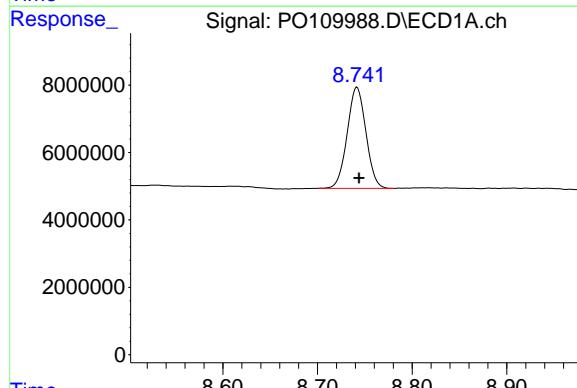


## #2 Decachlorobiphenyl

R.T.: 8.742 min  
Delta R.T.: -0.002 min  
Response: 41310164  
Conc: 5.30 ng/ml

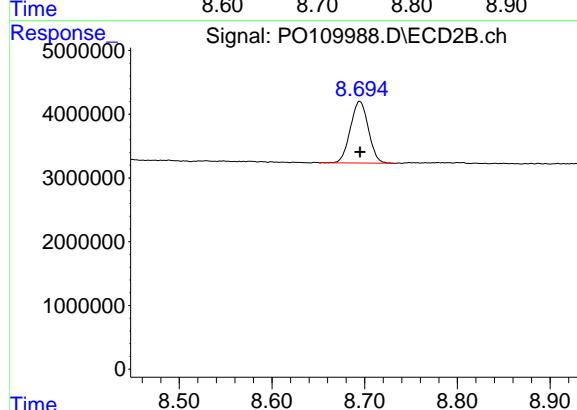

## #2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 13029410  
Conc: 5.56 ng/ml

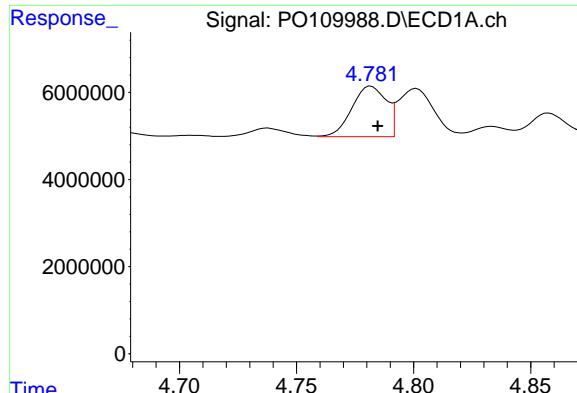


#21 AR-1248-1

R.T.: 4.782 min  
Delta R.T.: -0.003 min  
Response: 11846805  
Conc: 53.86 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC050


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

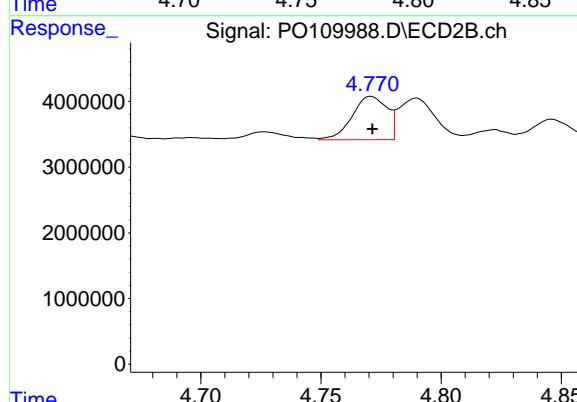


#21 AR-1248-1

R.T.: 4.771 min  
Delta R.T.: 0.000 min  
Response: 6686511  
Conc: 55.57 ng/ml

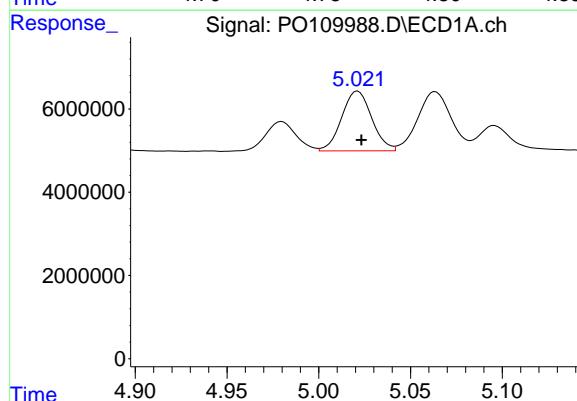


#22 AR-1248-2

R.T.: 5.021 min  
Delta R.T.: -0.002 min  
Response: 16385888  
Conc: 54.43 ng/ml

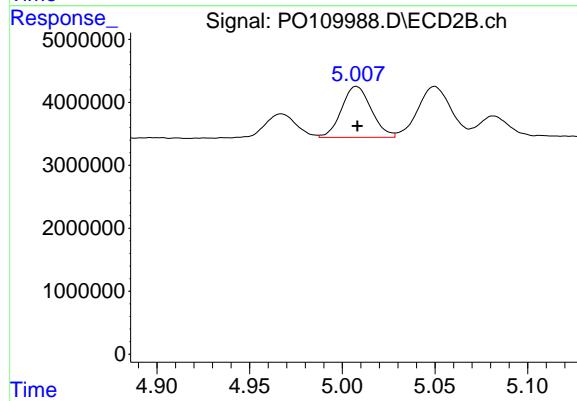

#22 AR-1248-2

R.T.: 5.008 min  
Delta R.T.: 0.000 min  
Response: 9031427  
Conc: 53.59 ng/ml

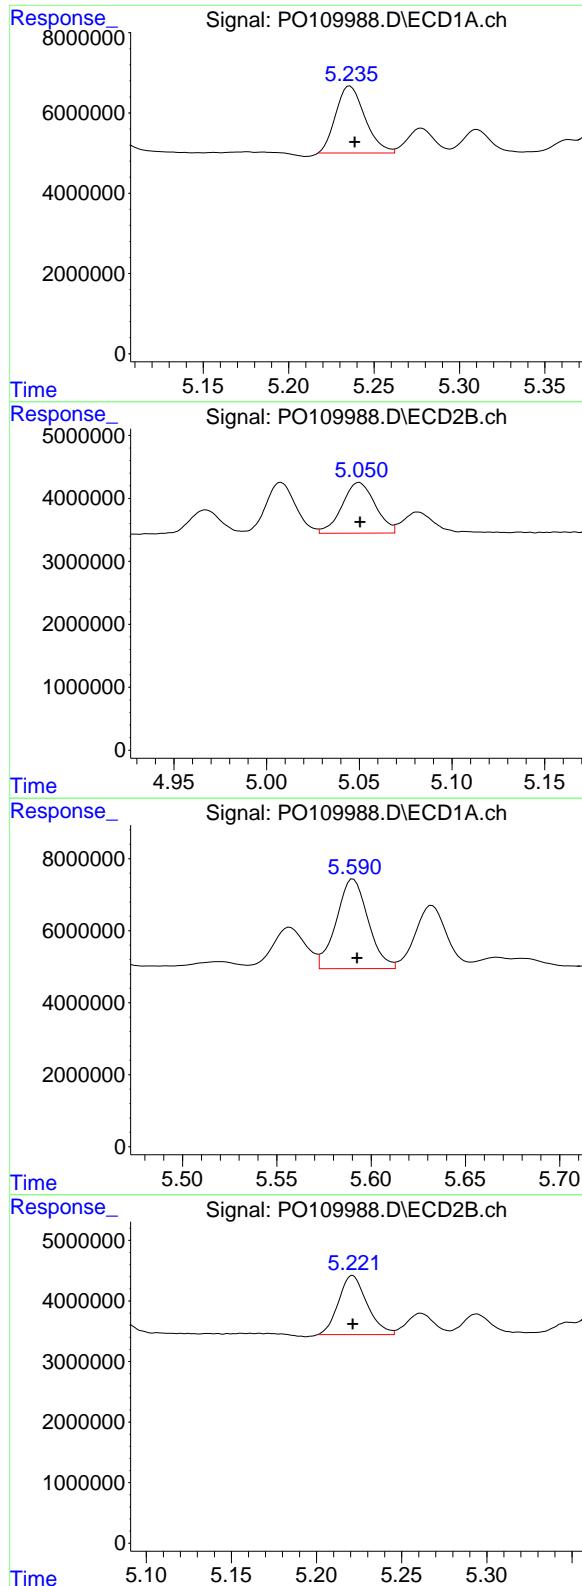

#23 AR-1248-3

R.T.: 5.235 min  
 Delta R.T.: -0.003 min  
 Response: 19860582  
 Conc: 53.05 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#23 AR-1248-3

R.T.: 5.050 min  
 Delta R.T.: 0.000 min  
 Response: 10026048  
 Conc: 55.98 ng/ml

#24 AR-1248-4

R.T.: 5.591 min  
 Delta R.T.: -0.002 min  
 Response: 29227773  
 Conc: 55.86 ng/ml

#24 AR-1248-4

R.T.: 5.221 min  
 Delta R.T.: 0.000 min  
 Response: 11398927  
 Conc: 54.65 ng/ml

#25 AR-1248-5

R.T.: 5.632 min  
 Delta R.T.: -0.002 min  
 Response: 20545156  
 Conc: 55.57 ng/ml


**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#25 AR-1248-5

R.T.: 5.613 min  
 Delta R.T.: 0.000 min  
 Response: 11669383  
 Conc: 57.30 ng/ml

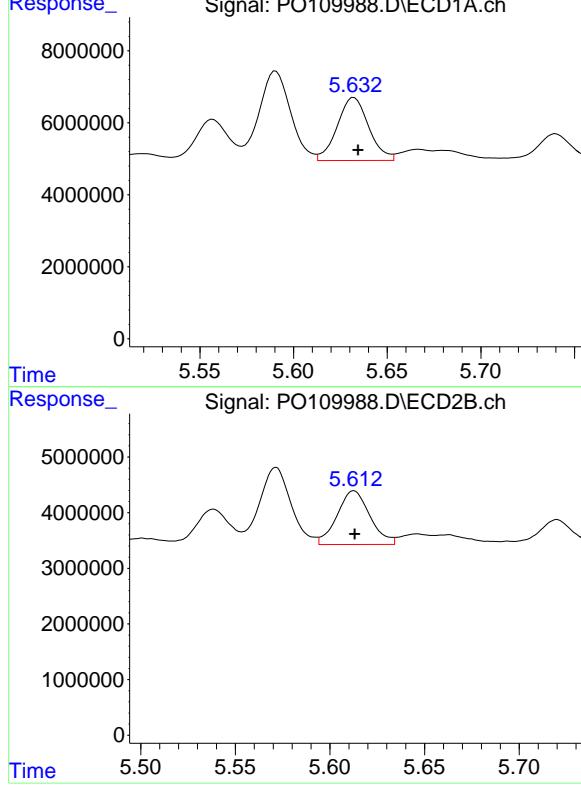

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109989.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 19:13  
 Operator : YP/AJ  
 Sample : AR1254ICC1000  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1254ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:49:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	912.4E6	520.8E6	97.196	97.394
2) SA Decachlor...	8.744	8.694	750.7E6	219.7E6	95.415	90.831

Target Compounds

26) L6 AR-1254-1	5.593	5.573	527.5E6	289.8E6	943.049	941.799
27) L6 AR-1254-2	5.742	5.721	454.9E6	250.7E6	940.470	933.876
28) L6 AR-1254-3	6.147	6.123	753.6E6	402.2E6	954.831	954.778
29) L6 AR-1254-4	6.376	6.351	465.4E6	231.8E6	956.772	948.684
30) L6 AR-1254-5	6.797	6.768	652.0E6	329.3E6	958.152	944.466



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109989.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 19:13  
 Operator : YP/AJ  
 Sample : AR1254ICC1000  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1254ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:49:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

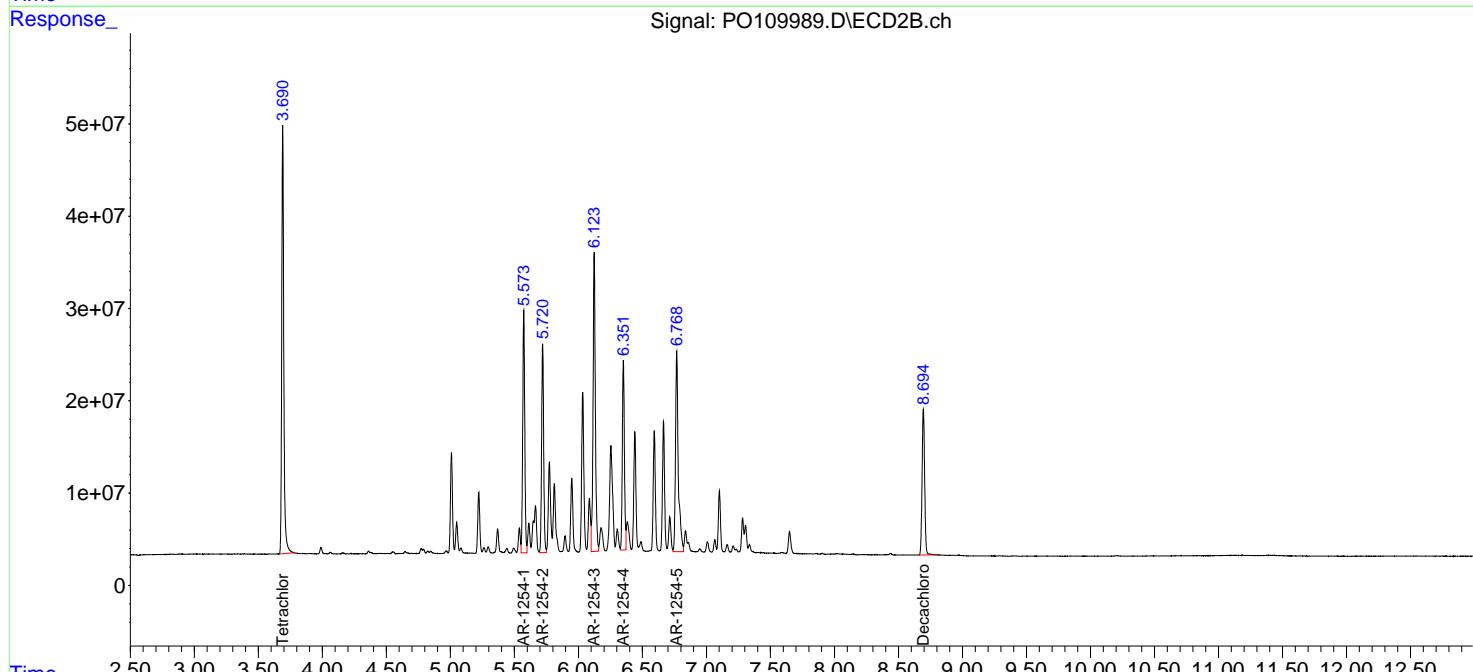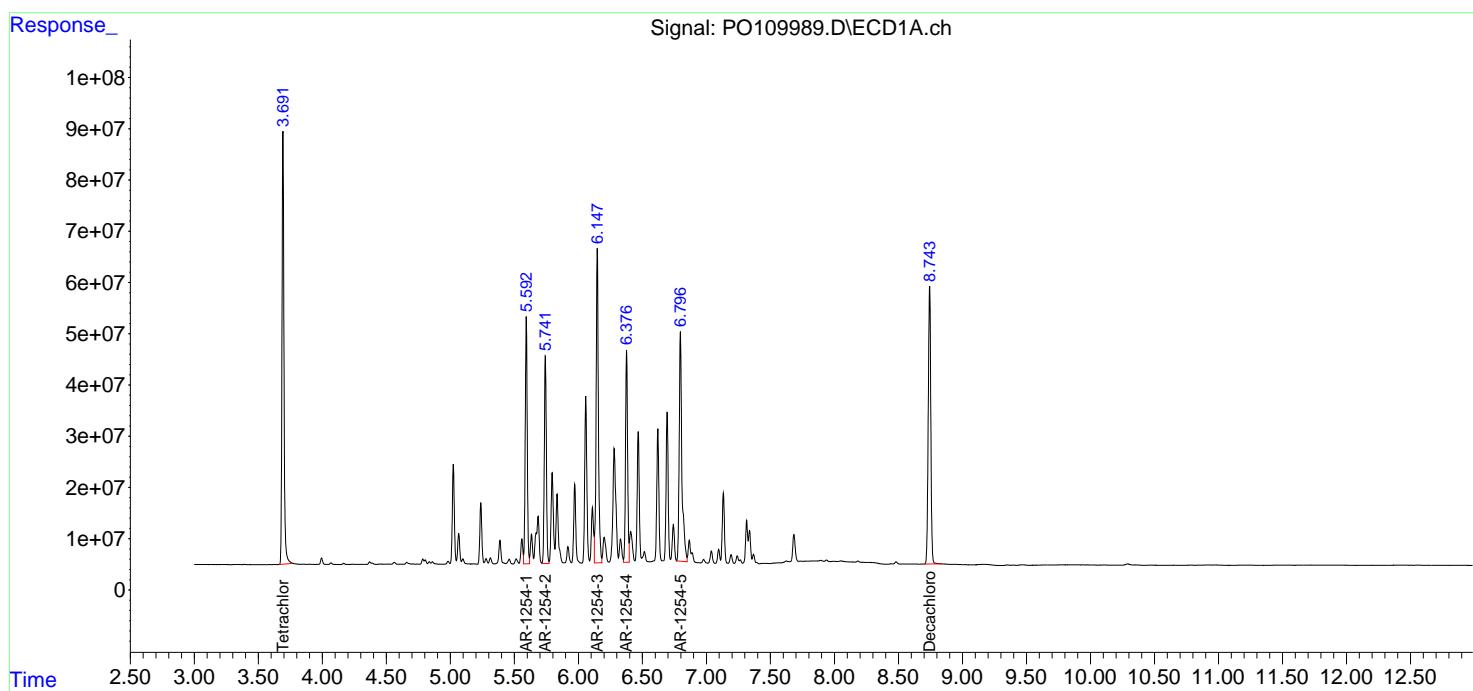

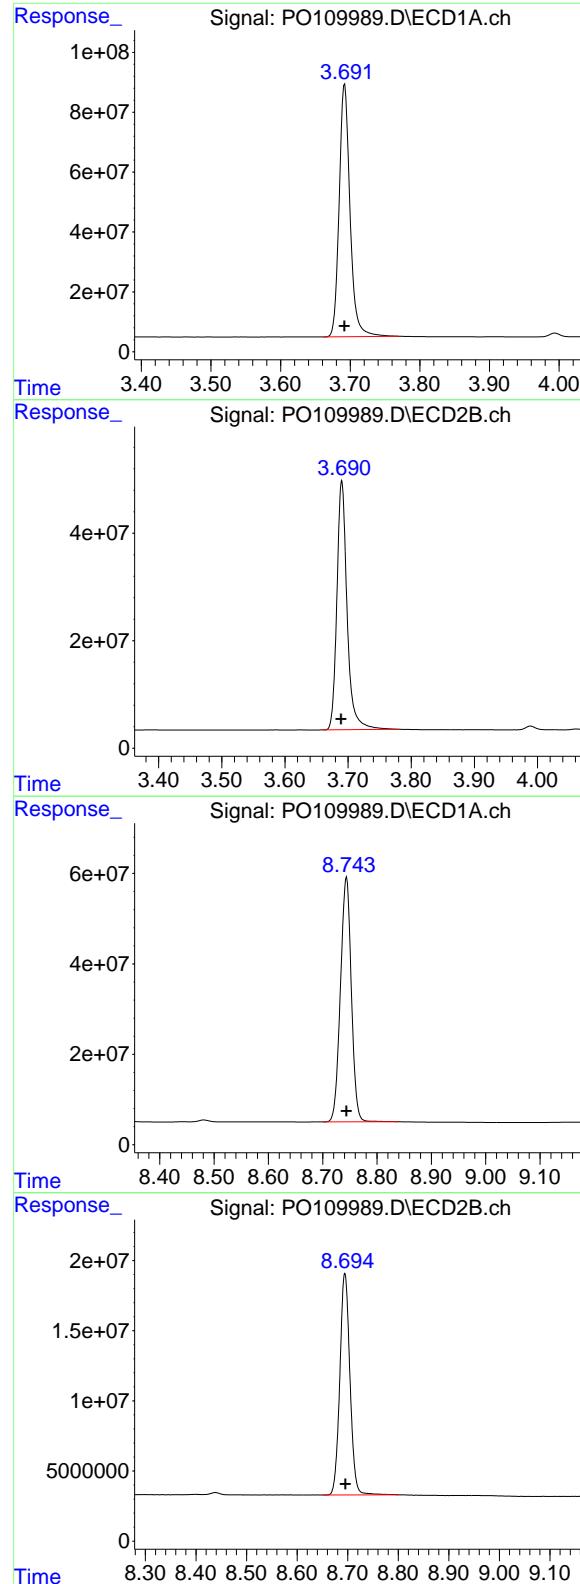

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
 Delta R.T.: 0.000 min  
 Response: 912401749  
 Conc: 97.20 ng/ml

Instrument:  
 ECD\_O  
 ClientSampleId :  
 AR1254ICC1000

## #1 Tetrachloro-m-xylene


R.T.: 3.690 min  
 Delta R.T.: 0.000 min  
 Response: 520755645  
 Conc: 97.39 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
 Delta R.T.: 0.000 min  
 Response: 750657739  
 Conc: 95.42 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.694 min  
 Delta R.T.: -0.001 min  
 Response: 219680790  
 Conc: 90.83 ng/ml

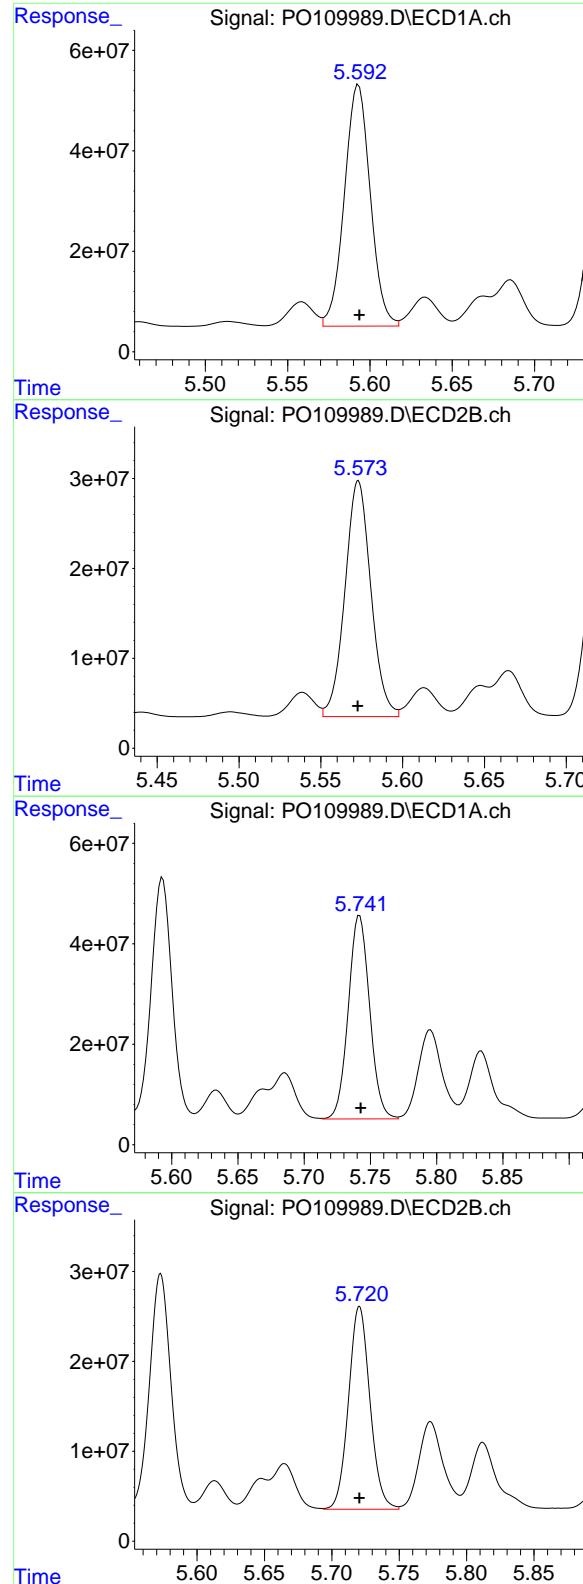

#26 AR-1254-1

R.T.: 5.593 min  
 Delta R.T.: 0.000 min  
 Response: 527461301  
 Conc: 943.05 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1254ICC1000

#26 AR-1254-1

R.T.: 5.573 min  
 Delta R.T.: 0.000 min  
 Response: 289813236  
 Conc: 941.80 ng/ml

#27 AR-1254-2

R.T.: 5.742 min  
 Delta R.T.: 0.000 min  
 Response: 454907170  
 Conc: 940.47 ng/ml





#27 AR-1254-2

R.T.: 5.721 min  
 Delta R.T.: 0.000 min  
 Response: 250736607  
 Conc: 933.88 ng/ml

#28 AR-1254-3

R.T.: 6.147 min  
 Delta R.T.: 0.000 min  
 Response: 753626169  
 Conc: 954.83 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC1000

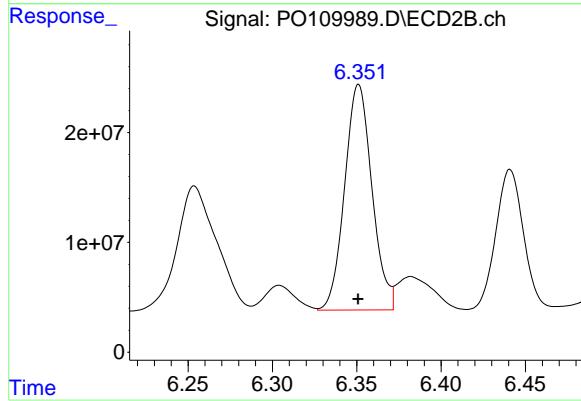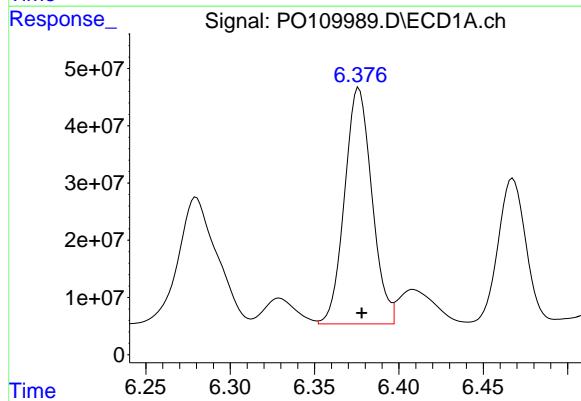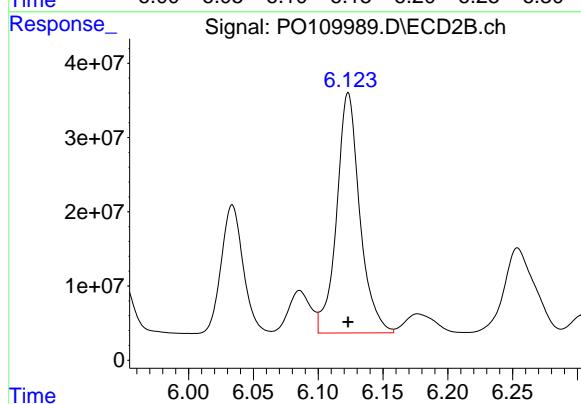

#28 AR-1254-3

R.T.: 6.123 min  
 Delta R.T.: 0.000 min  
 Response: 402159669  
 Conc: 954.78 ng/ml

#29 AR-1254-4

R.T.: 6.376 min  
 Delta R.T.: -0.002 min  
 Response: 465418236  
 Conc: 956.77 ng/ml



#29 AR-1254-4

R.T.: 6.351 min  
 Delta R.T.: 0.000 min  
 Response: 231846868  
 Conc: 948.68 ng/ml

#30 AR-1254-5

R.T.: 6.797 min  
Delta R.T.: 0.000 min  
Response: 652046620  
Conc: 958.15 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1254ICC1000

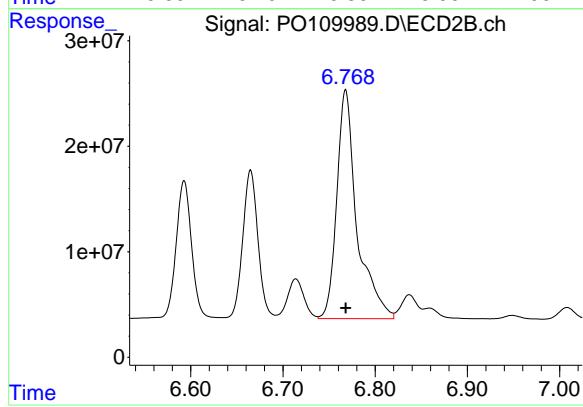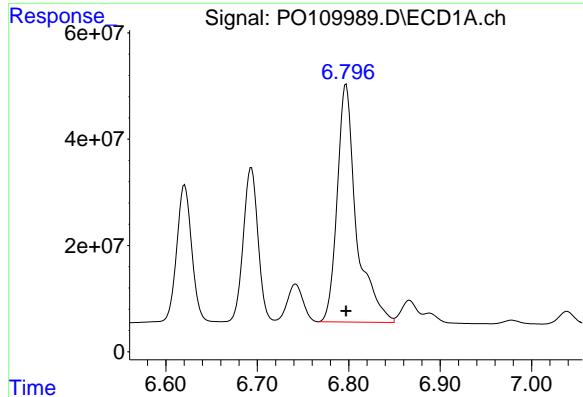

#30 AR-1254-5

R.T.: 6.768 min  
Delta R.T.: 0.000 min  
Response: 329301884  
Conc: 944.47 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109990.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 19:31  
 Operator : YP/AJ  
 Sample : AR1254ICC750  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1254ICC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:49:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.689	694.8E6	396.7E6	74.017	74.184
2) SA Decachlor...	8.742	8.695	579.2E6	170.7E6	73.621	70.591

Target Compounds

26) L6 AR-1254-1	5.593	5.572	406.4E6	224.1E6	726.602	728.104
27) L6 AR-1254-2	5.742	5.720	351.8E6	194.7E6	727.216	725.242
28) L6 AR-1254-3	6.148	6.122	579.5E6	310.1E6	734.225	736.114
29) L6 AR-1254-4	6.376	6.350	358.3E6	178.4E6	736.667	729.972
30) L6 AR-1254-5	6.796	6.768	499.8E6	253.4E6	734.486	726.842



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109990.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 19:31  
 Operator : YP/AJ  
 Sample : AR1254ICC750  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1254ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:49:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

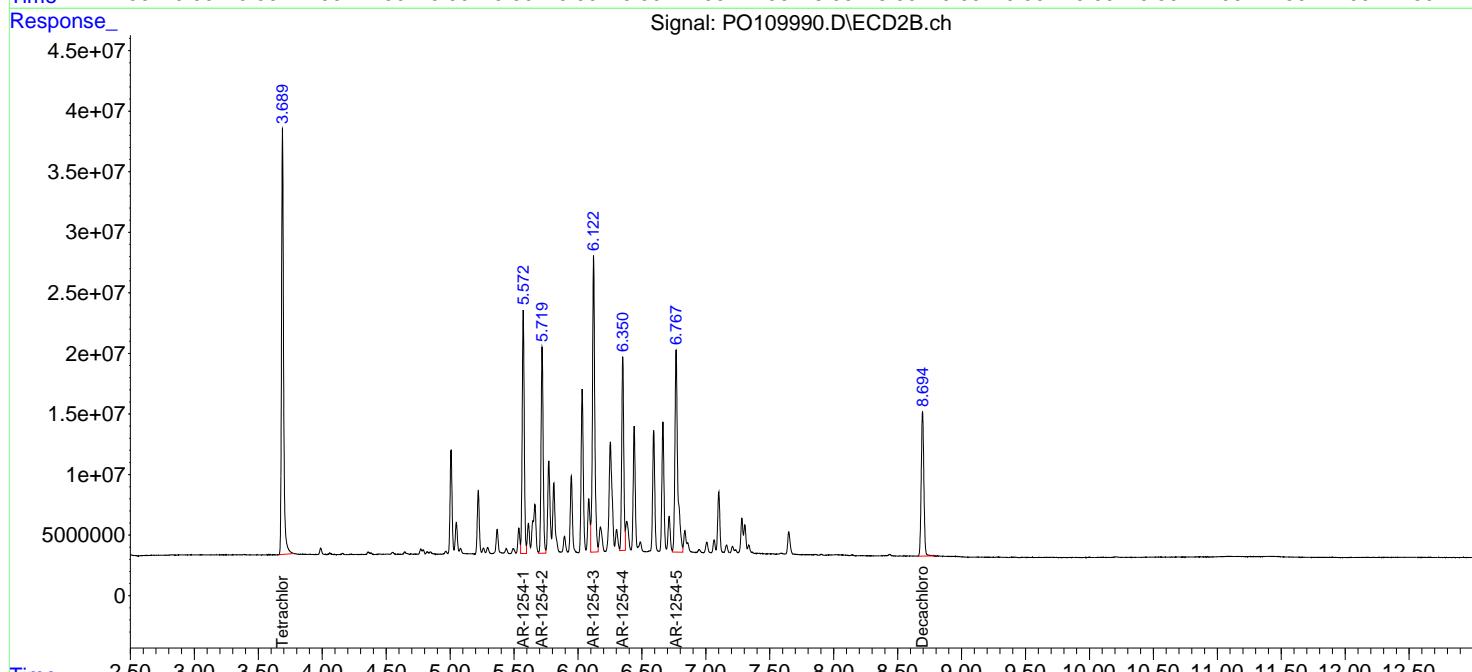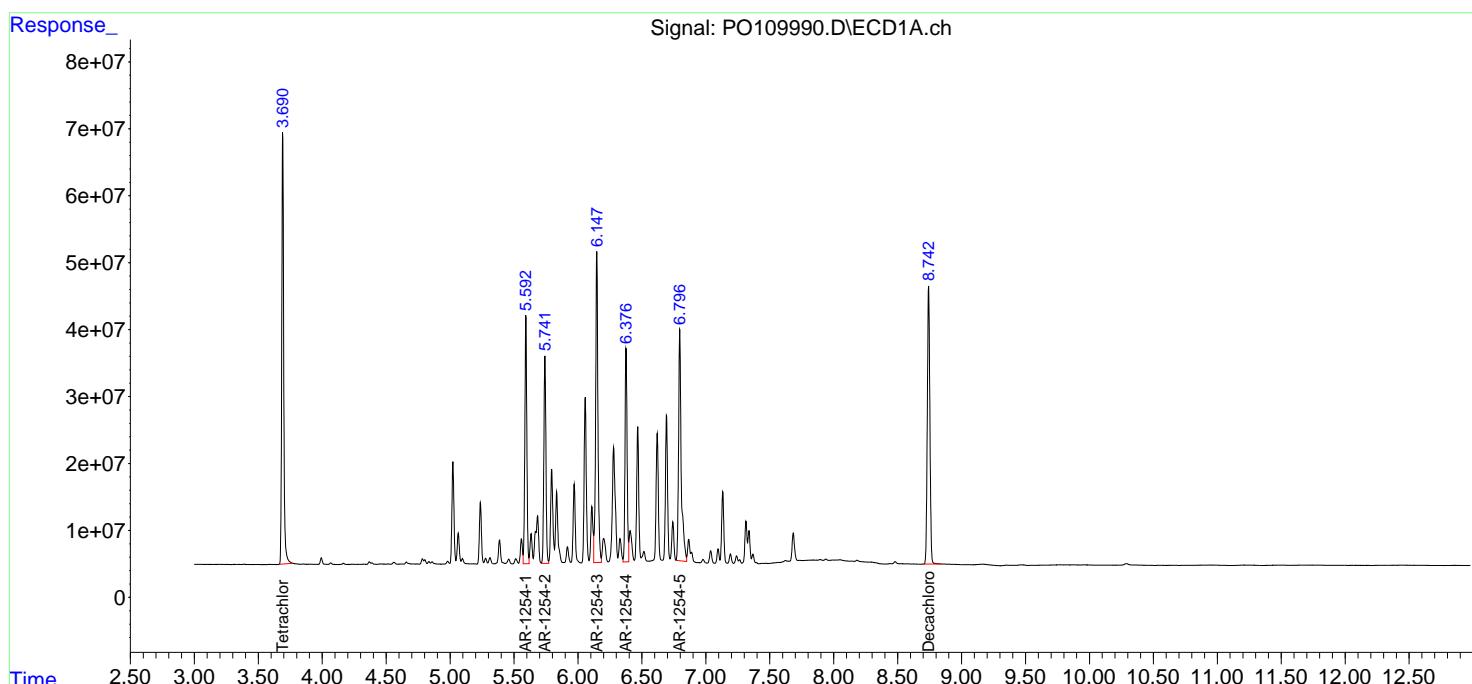

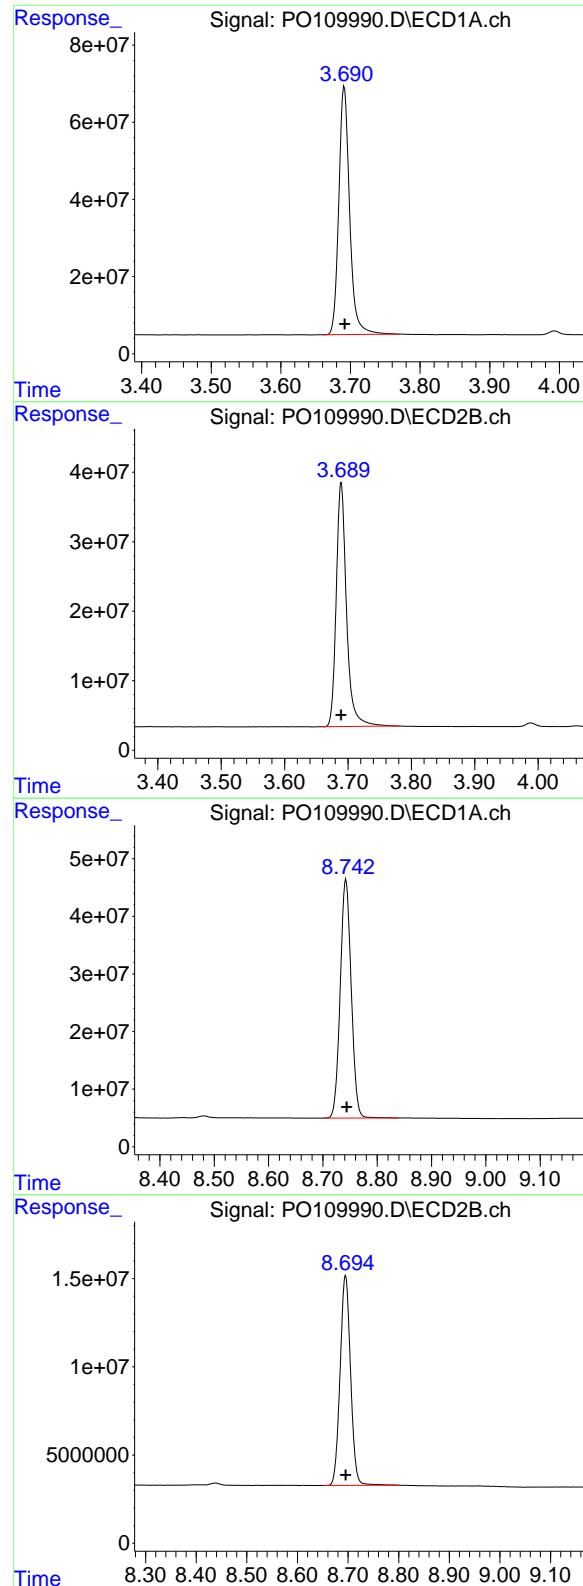

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: 0.000 min  
 Response: 694816651  
 Conc: 74.02 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC750

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
 Delta R.T.: 0.000 min  
 Response: 396654527  
 Conc: 74.18 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.742 min  
 Delta R.T.: -0.001 min  
 Response: 579195225  
 Conc: 73.62 ng/ml


## #2 Decachlorobiphenyl

R.T.: 8.695 min  
 Delta R.T.: 0.000 min  
 Response: 170728292  
 Conc: 70.59 ng/ml

#26 AR-1254-1


R.T.: 5.593 min  
 Delta R.T.: 0.000 min  
 Response: 406399307  
 Conc: 726.60 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC750

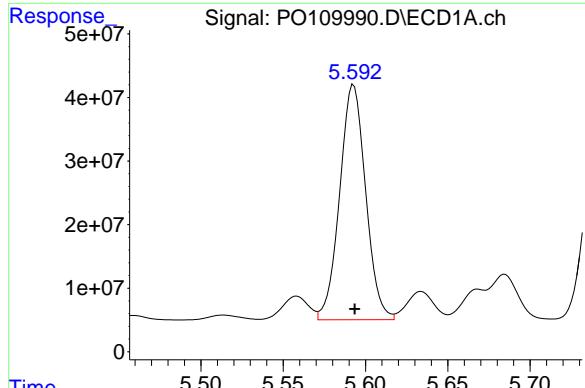


#26 AR-1254-1

R.T.: 5.572 min  
 Delta R.T.: 0.000 min  
 Response: 224054374  
 Conc: 728.10 ng/ml

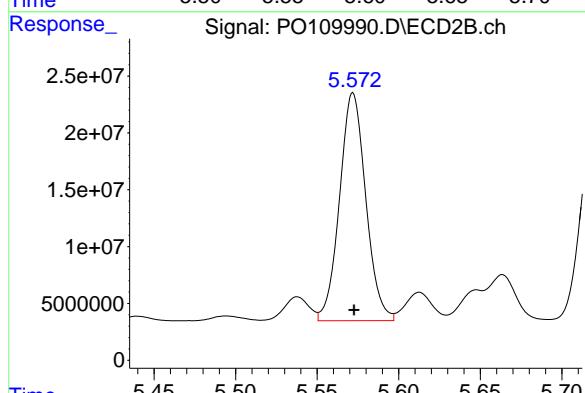


#27 AR-1254-2

R.T.: 5.742 min  
 Delta R.T.: -0.001 min  
 Response: 351755893  
 Conc: 727.22 ng/ml

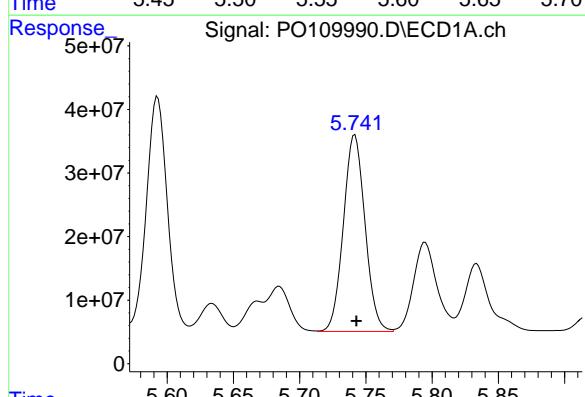

#27 AR-1254-2





R.T.: 5.720 min  
 Delta R.T.: 0.000 min  
 Response: 194720485  
 Conc: 725.24 ng/ml

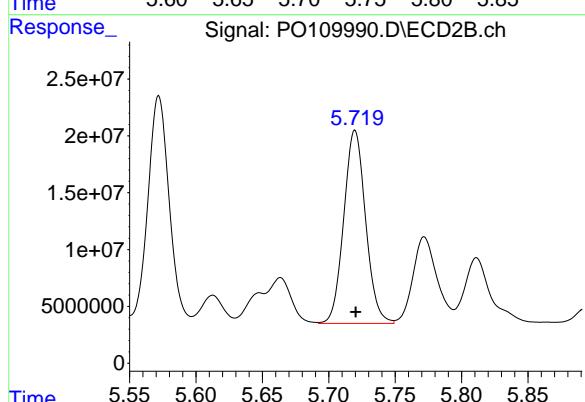

#28 AR-1254-3

R.T.: 6.148 min  
 Delta R.T.: 0.000 min  
 Response: 579506791  
 Conc: 734.22 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC750

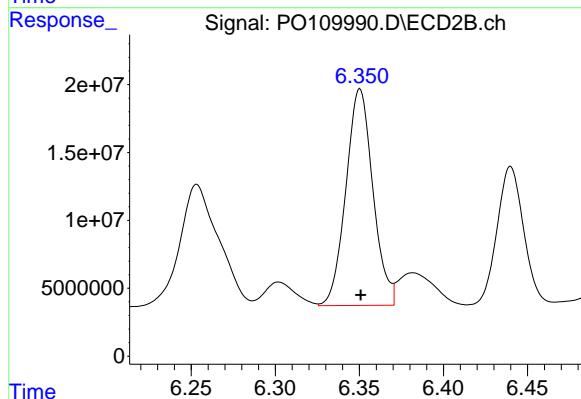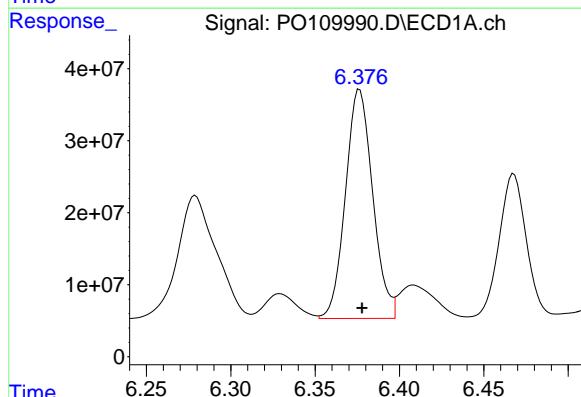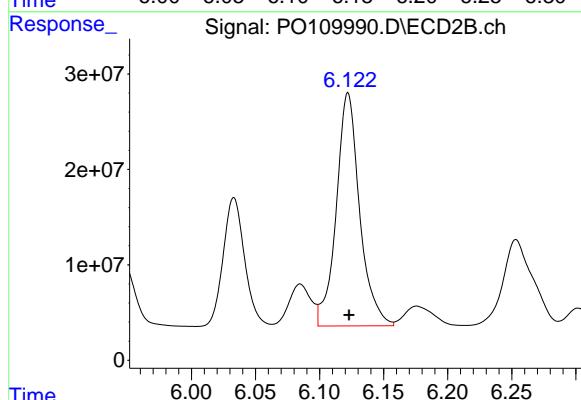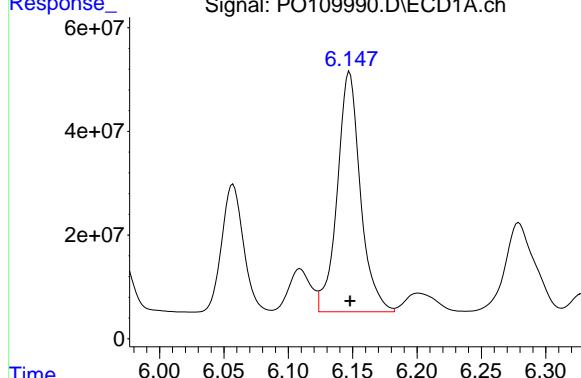

#28 AR-1254-3

R.T.: 6.122 min  
 Delta R.T.: 0.000 min  
 Response: 310056844  
 Conc: 736.11 ng/ml

#29 AR-1254-4

R.T.: 6.376 min  
 Delta R.T.: -0.001 min  
 Response: 358349037  
 Conc: 736.67 ng/ml


#29 AR-1254-4

R.T.: 6.350 min  
 Delta R.T.: 0.000 min  
 Response: 178396380  
 Conc: 729.97 ng/ml

#30 AR-1254-5


R.T.: 6.796 min  
Delta R.T.: 0.000 min  
Response: 499835944  
Conc: 734.49 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1254ICC750

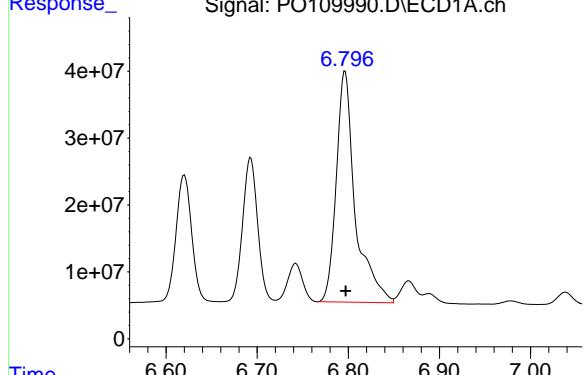

#30 AR-1254-5

R.T.: 6.768 min  
Delta R.T.: 0.000 min  
Response: 253424010  
Conc: 726.84 ng/ml

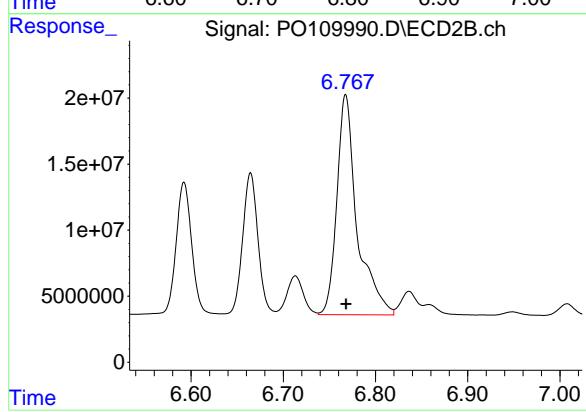

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109991.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 19:49  
 Operator : YP/AJ  
 Sample : AR1254ICC500  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1254ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:52:43 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	469.4E6	267.3E6	50.000	50.000
2) SA Decachlor...	8.744	8.695	393.4E6	120.9E6	50.000	50.000

Target Compounds

26) L6 AR-1254-1	5.594	5.573	279.7E6	153.9E6	500.000	500.000
27) L6 AR-1254-2	5.743	5.720	241.9E6	134.2E6	500.000	500.000
28) L6 AR-1254-3	6.148	6.123	394.6E6	210.6E6	500.000	500.000
29) L6 AR-1254-4	6.378	6.351	243.2E6	122.2E6	500.000	500.000
30) L6 AR-1254-5	6.797	6.768	340.3E6	174.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109991.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 19:49  
 Operator : YP/AJ  
 Sample : AR1254ICC500  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1


**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 AR1254ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:52:43 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

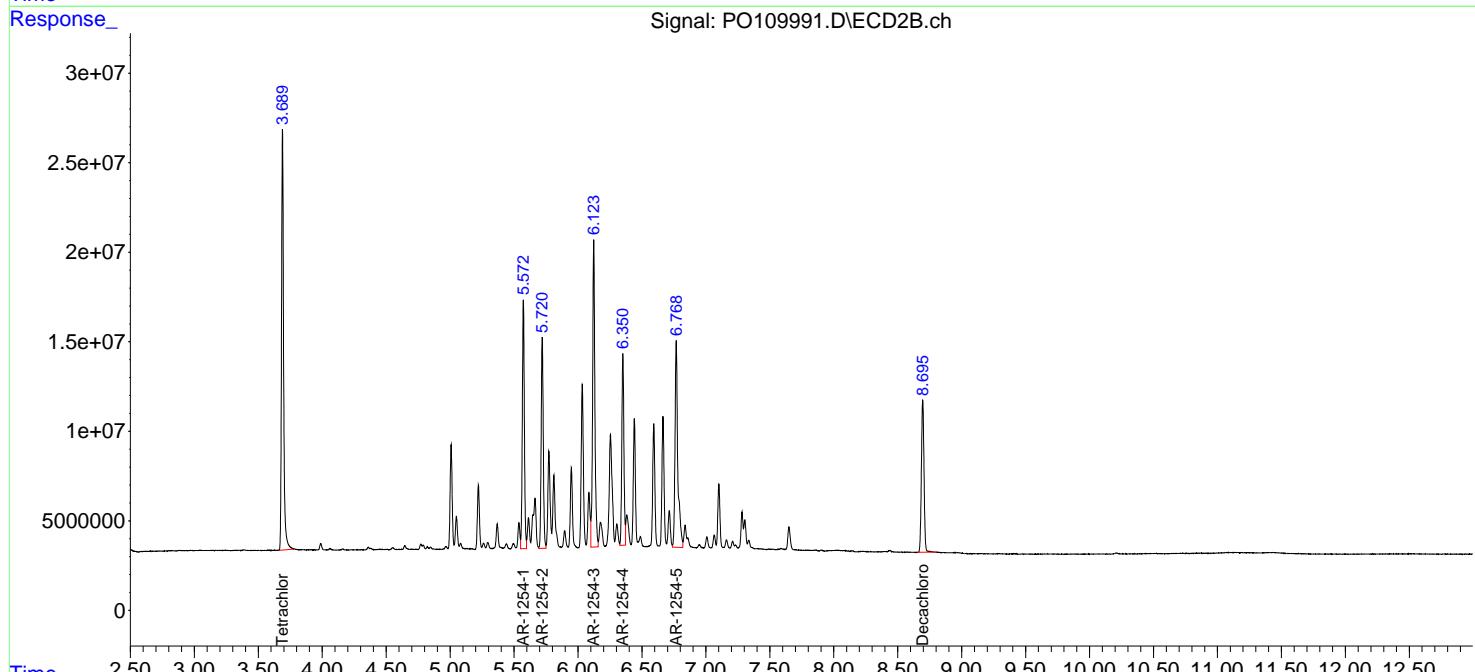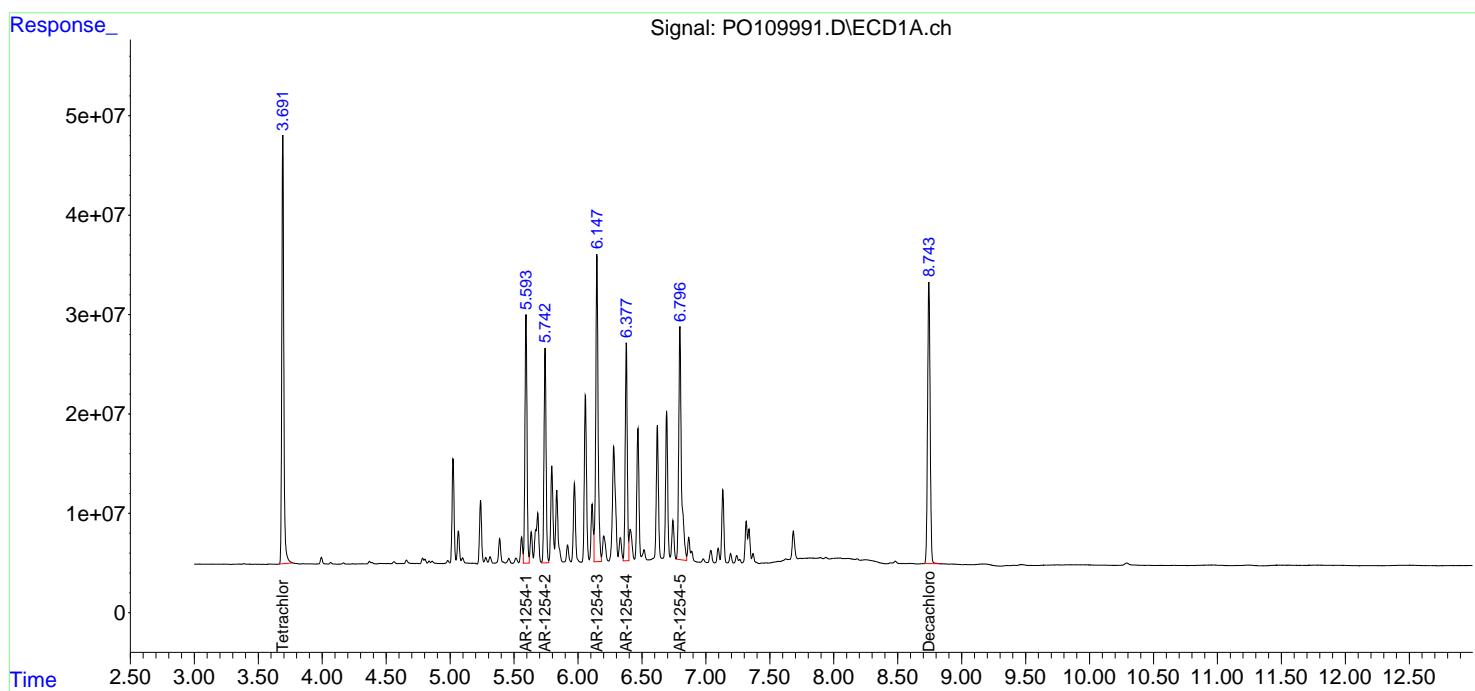

## #1 Tetrachloro-m-xylene

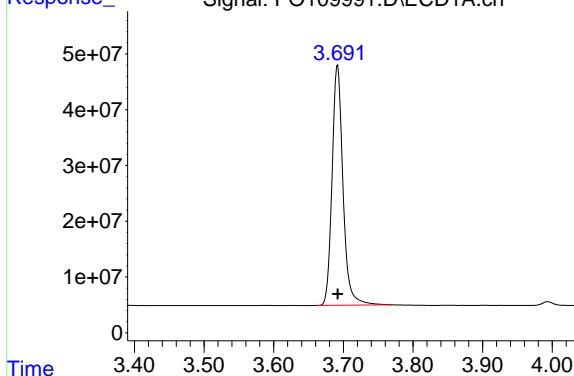

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 469362086  
Conc: 50.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC500

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 267345850  
Conc: 50.00 ng/ml



## #2 Decachlorobiphenyl


R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 393362889  
Conc: 50.00 ng/ml



## #2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 120928616  
Conc: 50.00 ng/ml



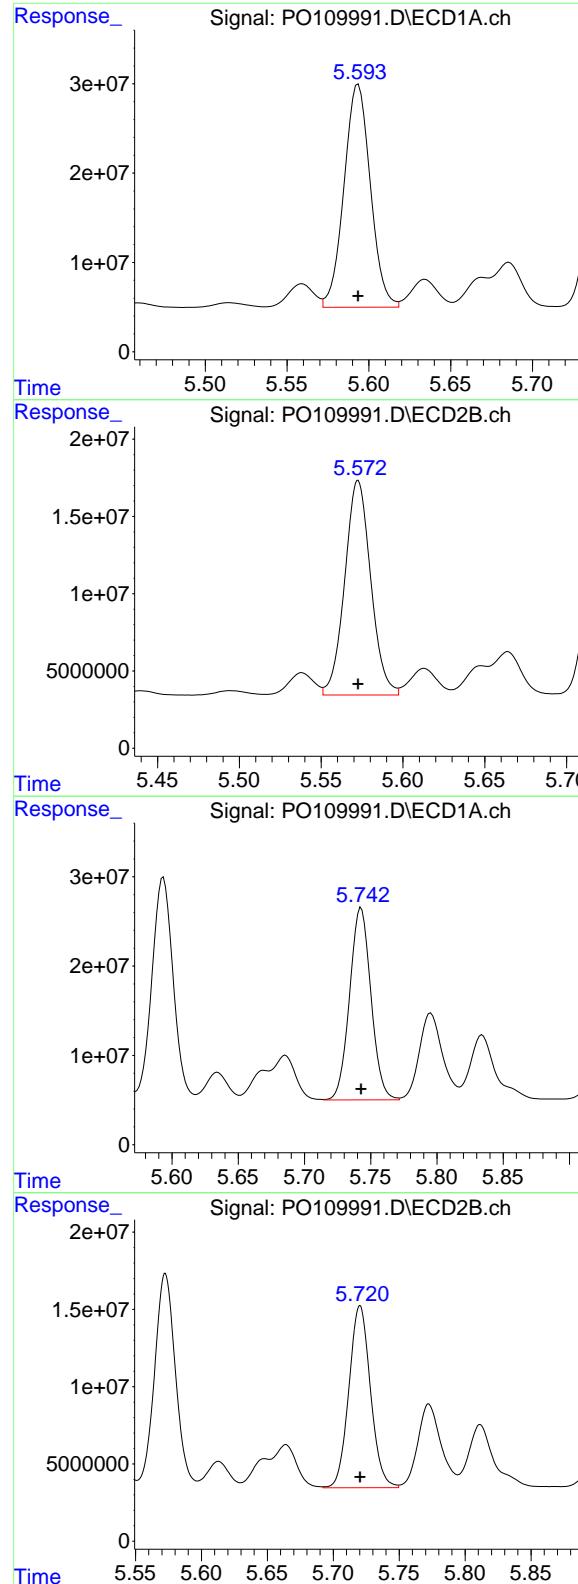

#26 AR-1254-1

R.T.: 5.594 min  
Delta R.T.: 0.000 min  
Response: 279657443  
Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC500

#26 AR-1254-1

R.T.: 5.573 min  
Delta R.T.: 0.000 min  
Response: 153861440  
Conc: 500.00 ng/ml

#27 AR-1254-2

R.T.: 5.743 min  
Delta R.T.: 0.000 min  
Response: 241851007  
Conc: 500.00 ng/ml





#27 AR-1254-2

R.T.: 5.720 min  
Delta R.T.: 0.000 min  
Response: 134245134  
Conc: 500.00 ng/ml

#28 AR-1254-3

R.T.: 6.148 min  
 Delta R.T.: 0.000 min  
 Response: 394638676  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC500

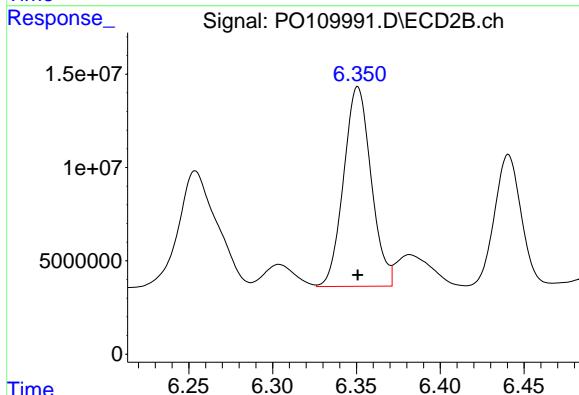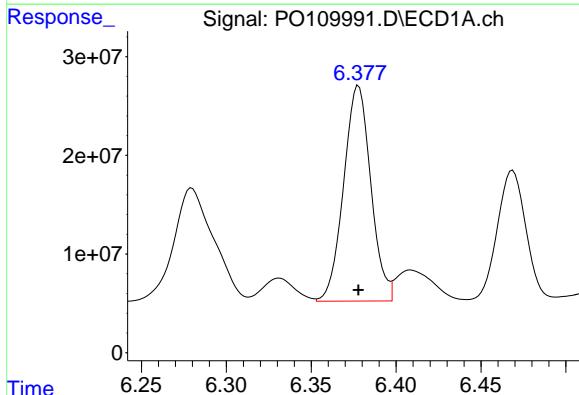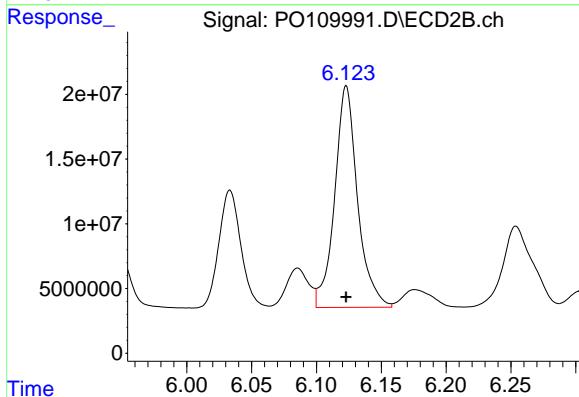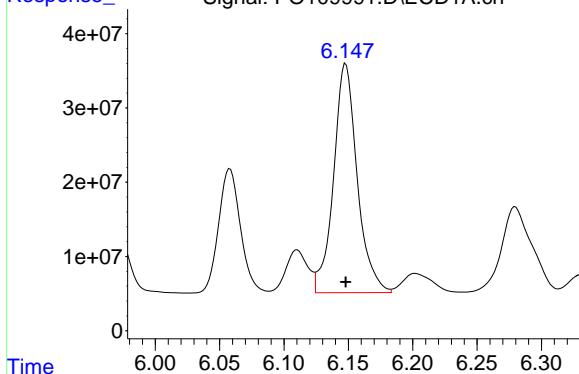

#28 AR-1254-3

R.T.: 6.123 min  
 Delta R.T.: 0.000 min  
 Response: 210603765  
 Conc: 500.00 ng/ml

#29 AR-1254-4

R.T.: 6.378 min  
 Delta R.T.: 0.000 min  
 Response: 243223195  
 Conc: 500.00 ng/ml



#29 AR-1254-4

R.T.: 6.351 min  
 Delta R.T.: 0.000 min  
 Response: 122193976  
 Conc: 500.00 ng/ml

#30 AR-1254-5

R.T.: 6.797 min  
Delta R.T.: 0.000 min  
Response: 340262601  
Conc: 500.00 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1254ICC500

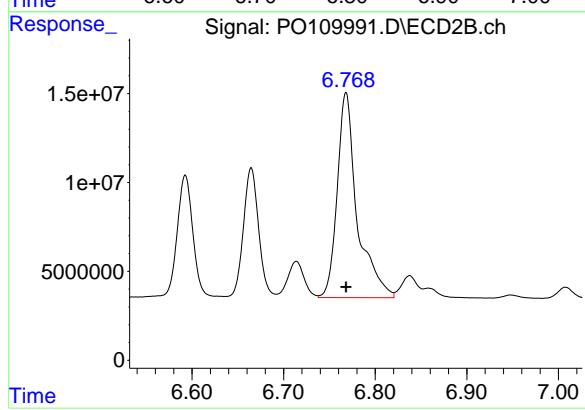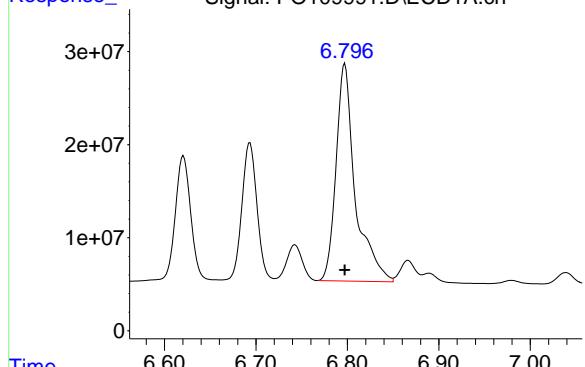

#30 AR-1254-5

R.T.: 6.768 min  
Delta R.T.: 0.000 min  
Response: 174332293  
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109992.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 20:07  
 Operator : YP/AJ  
 Sample : AR1254ICC250  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1254ICC250

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:50:17 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.690	3.689	218.3E6	126.3E6	23.256	23.621
2) SA Decachlor...	8.743	8.695	201.1E6	62915084	25.556	26.013

Target Compounds

26) L6 AR-1254-1	5.592	5.572	142.8E6	78551215	255.230	255.266
27) L6 AR-1254-2	5.741	5.720	117.7E6	67765666	243.403	252.395
28) L6 AR-1254-3	6.146	6.123	190.0E6	103.9E6	240.780	246.647
29) L6 AR-1254-4	6.376	6.351	124.9E6	61546138	256.767	251.838
30) L6 AR-1254-5	6.795	6.768	170.5E6	90324740	250.587	259.059



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109992.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 20:07  
 Operator : YP/AJ  
 Sample : AR1254ICC250  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1254ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:50:17 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

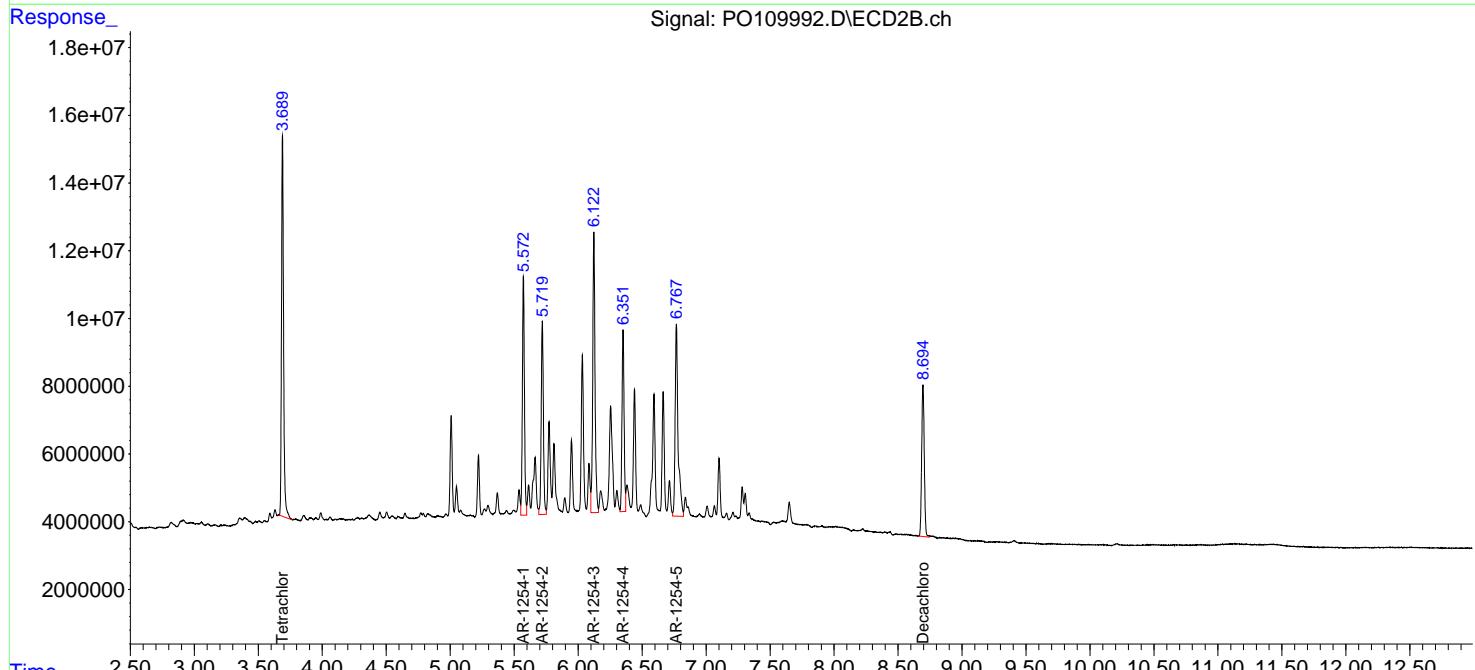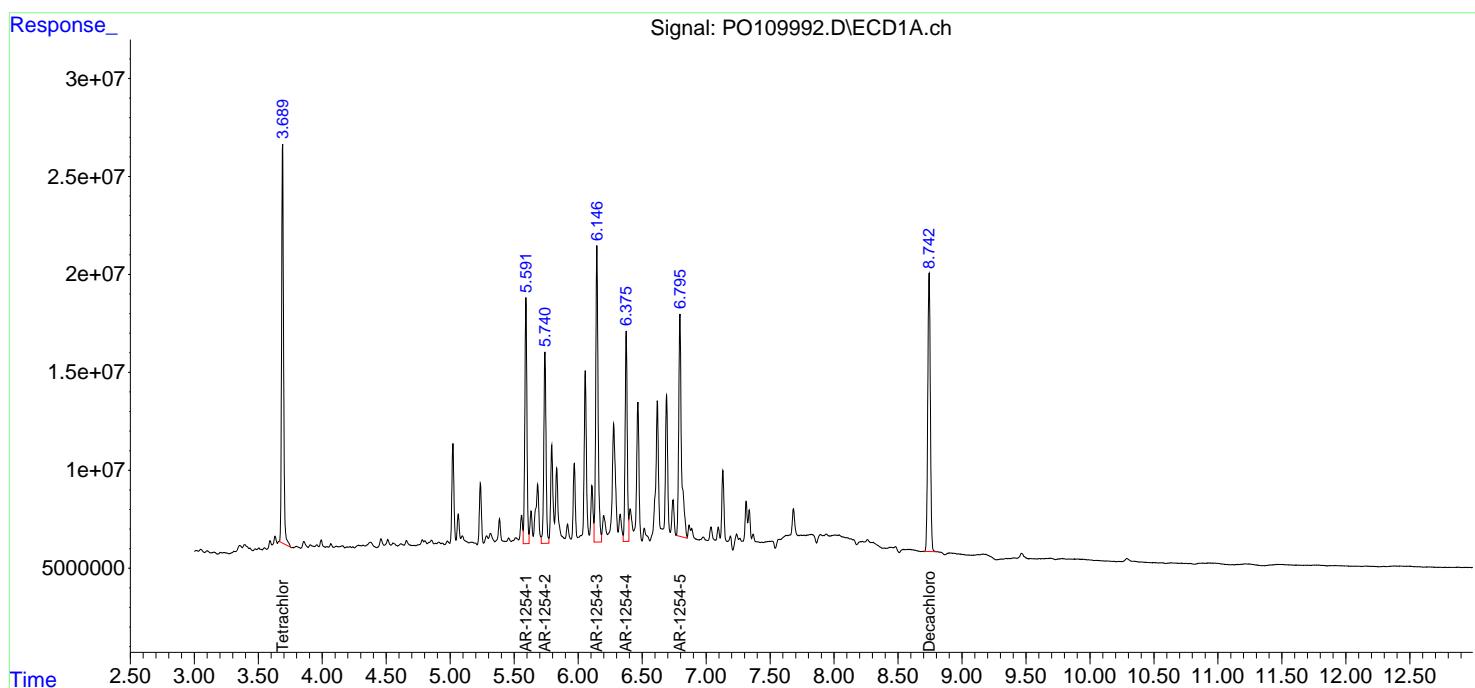

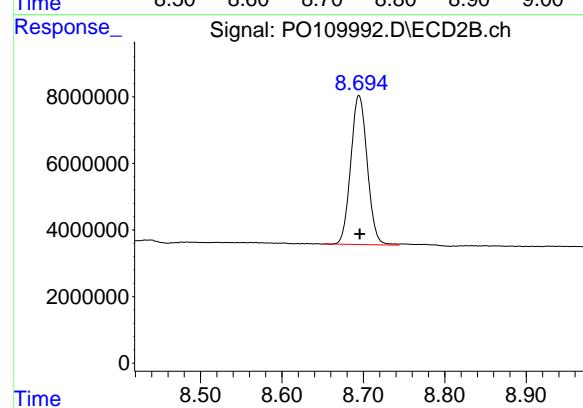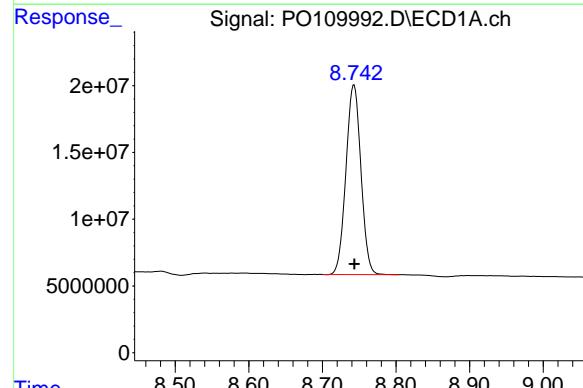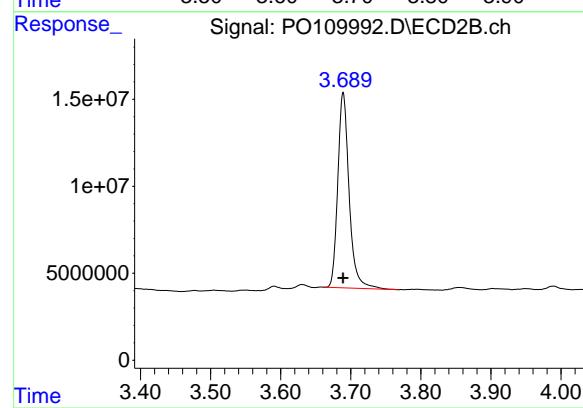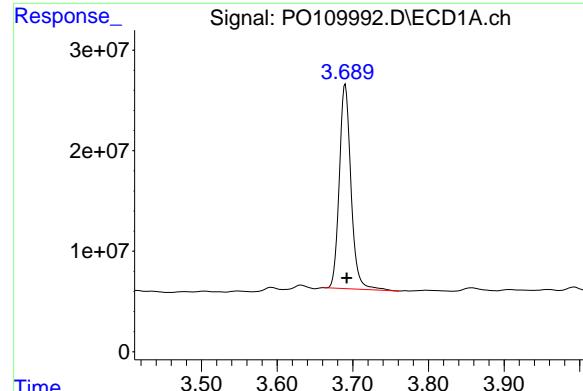

#1 Tetrachloro-m-xylene

R.T.: 3.690 min

Delta R.T.: -0.002 min

Response: 218311930

Conc: 23.26 ng/ml

Instrument:

ECD\_O

ClientSampleId :

AR1254ICC250

#1 Tetrachloro-m-xylene

R.T.: 3.689 min

Delta R.T.: 0.000 min

Response: 126298911

Conc: 23.62 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.743 min

Delta R.T.: 0.000 min

Response: 201053654

Conc: 25.56 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min

Delta R.T.: 0.000 min


Response: 62915084

Conc: 26.01 ng/ml

#26 AR-1254-1


R.T.: 5.592 min  
 Delta R.T.: -0.002 min  
 Response: 142754156  
 Conc: 255.23 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC250

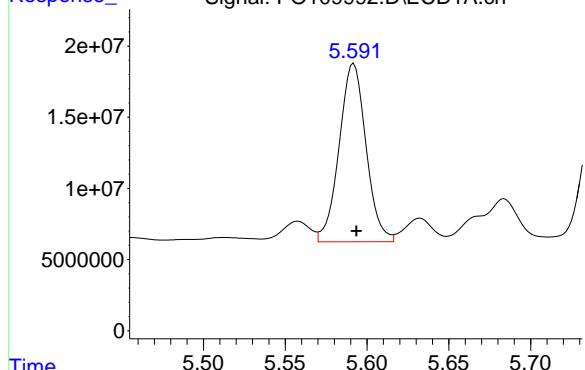


#26 AR-1254-1

R.T.: 5.572 min  
 Delta R.T.: 0.000 min  
 Response: 78551215  
 Conc: 255.27 ng/ml

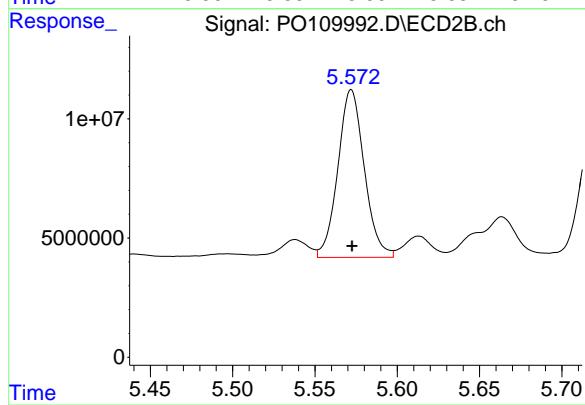


#27 AR-1254-2

R.T.: 5.741 min  
 Delta R.T.: -0.002 min  
 Response: 117734646  
 Conc: 243.40 ng/ml

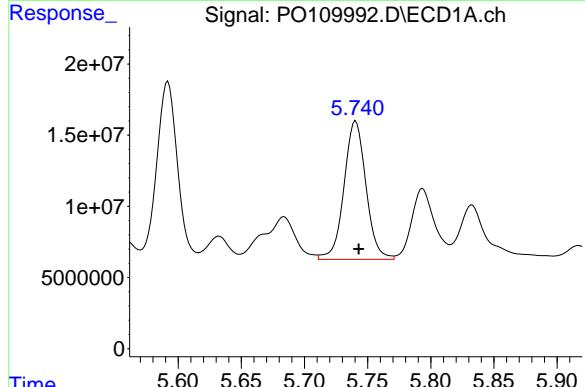

#27 AR-1254-2





R.T.: 5.720 min  
 Delta R.T.: 0.000 min  
 Response: 67765666  
 Conc: 252.40 ng/ml

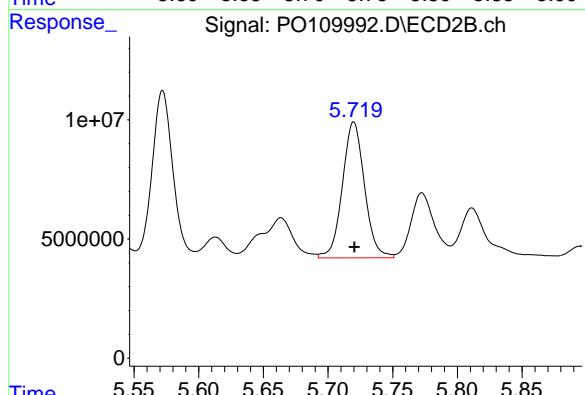

#28 AR-1254-3

R.T.: 6.146 min  
 Delta R.T.: -0.002 min  
 Response: 190042575  
 Conc: 240.78 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC250

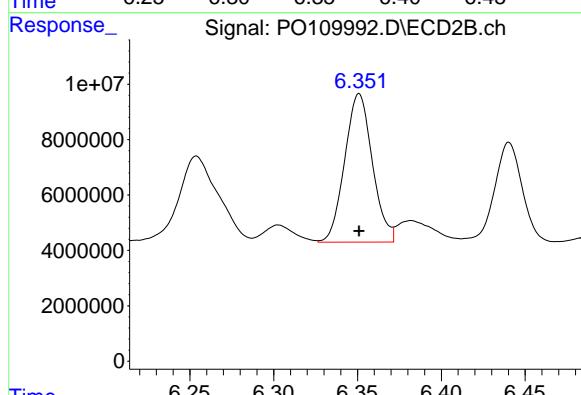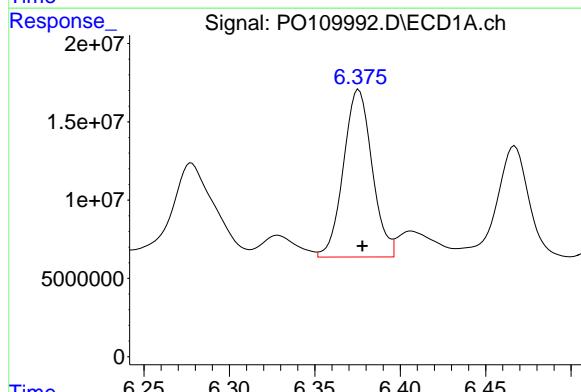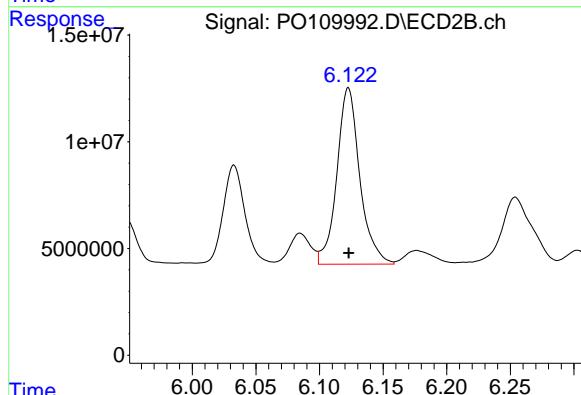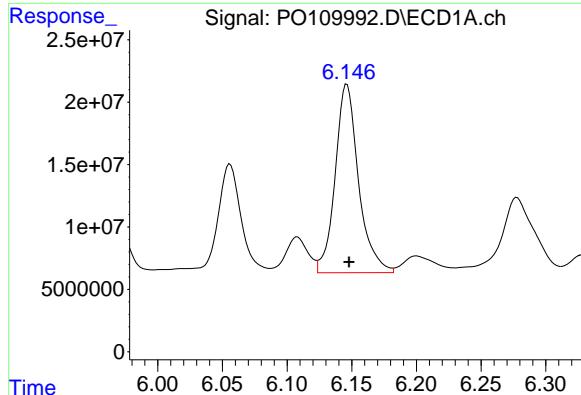

#28 AR-1254-3

R.T.: 6.123 min  
 Delta R.T.: 0.000 min  
 Response: 103889593  
 Conc: 246.65 ng/ml


#29 AR-1254-4

R.T.: 6.376 min  
 Delta R.T.: -0.002 min  
 Response: 124903516  
 Conc: 256.77 ng/ml

#29 AR-1254-4

R.T.: 6.351 min  
 Delta R.T.: 0.000 min  
 Response: 61546138  
 Conc: 251.84 ng/ml

#30 AR-1254-5




R.T.: 6.795 min  
Delta R.T.: -0.002 min  
Response: 170531002  
Conc: 250.59 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1254ICC250

#30 AR-1254-5

R.T.: 6.768 min  
Delta R.T.: 0.000 min  
Response: 90324740  
Conc: 259.06 ng/ml

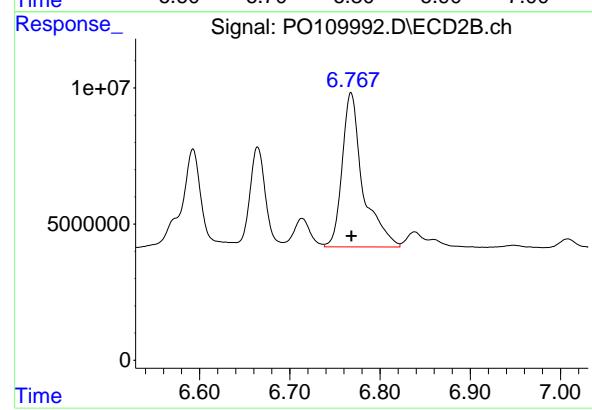

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109993.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 20:25  
 Operator : YP/AJ  
 Sample : AR1254ICC050  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1254ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:50:30 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	43445665	25306006	4.628	4.733
2) SA Decachlor...	8.743	8.694	41266656	13227136	5.245	5.469

Target Compounds

26) L6 AR-1254-1	5.593	5.573	31329450	17649915	56.014	57.357
27) L6 AR-1254-2	5.742	5.720	26381750	15388259	54.541	57.314
28) L6 AR-1254-3	6.148	6.123	39484048	21241930	50.026	50.431
29) L6 AR-1254-4	6.377	6.350	23571245	12628885	48.456	51.676
30) L6 AR-1254-5	6.797	6.768	28479203	15116419	41.849	43.355m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109993.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 20:25  
 Operator : YP/AJ  
 Sample : AR1254ICC050  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:50:30 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 AR1254ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

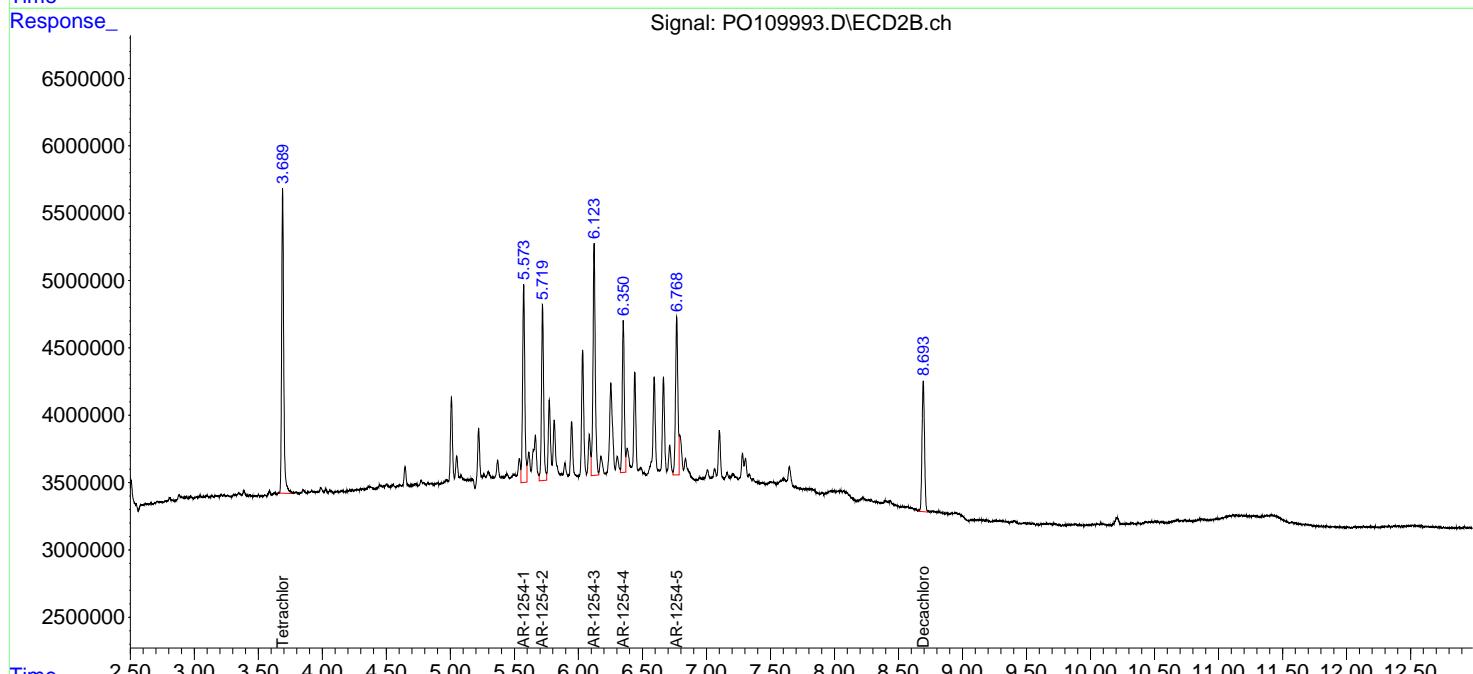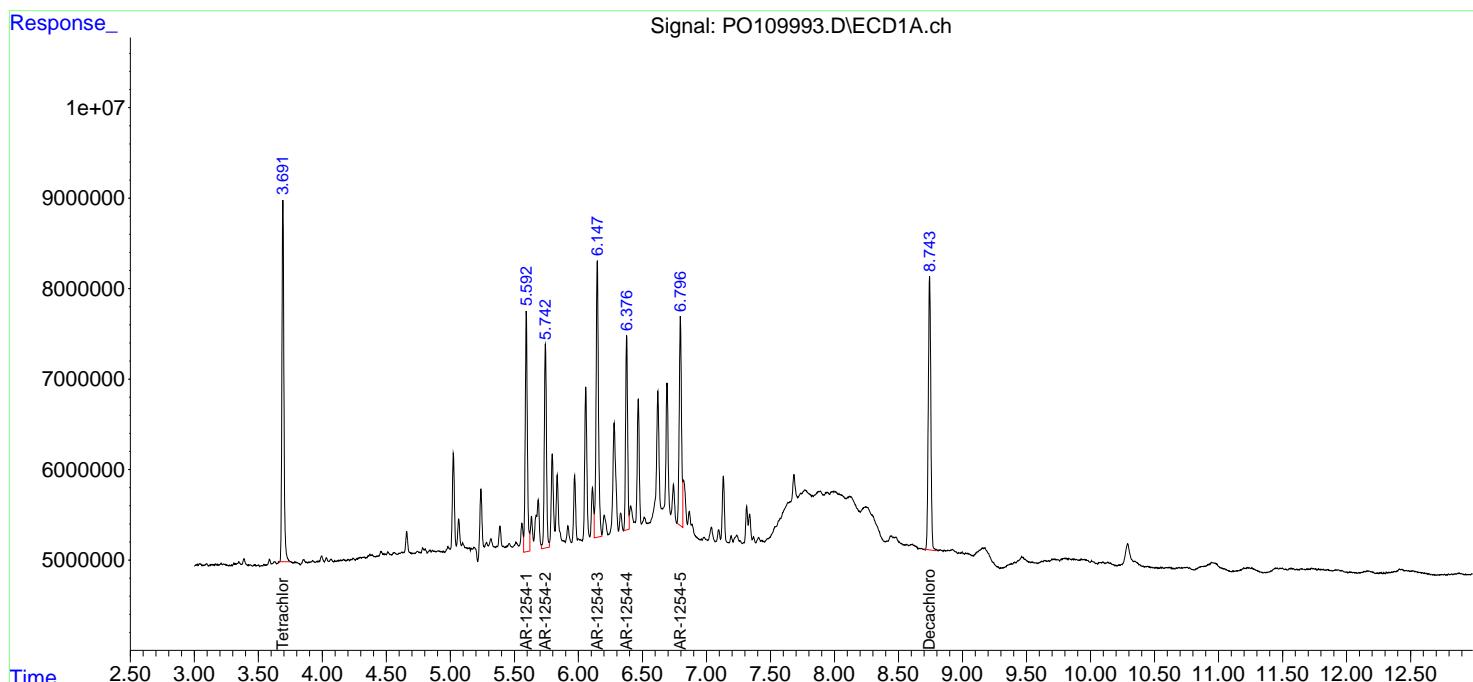




## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 43445665  
Conc: 4.63 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1254ICC050


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

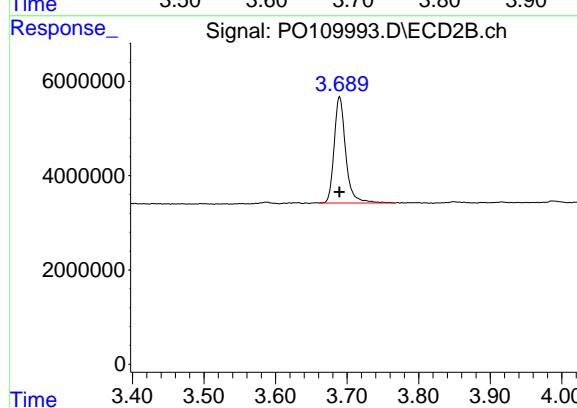


## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 25306006  
Conc: 4.73 ng/ml

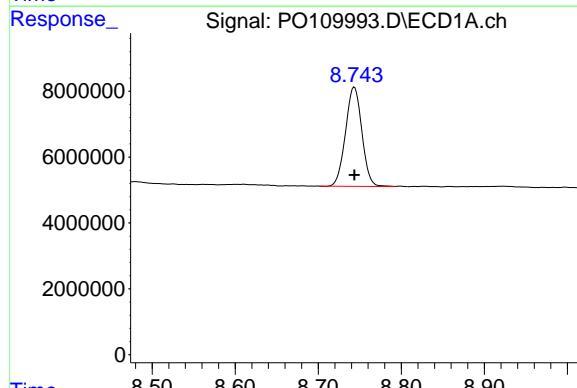

## #2 Decachlorobiphenyl

R.T.: 8.743 min  
Delta R.T.: 0.000 min  
Response: 41266656  
Conc: 5.25 ng/ml

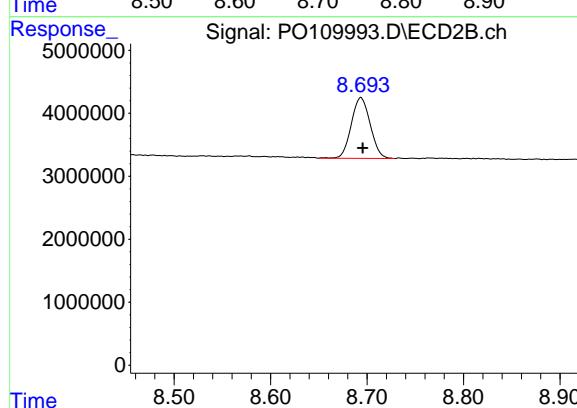

## #2 Decachlorobiphenyl

R.T.: 8.694 min  
Delta R.T.: -0.002 min  
Response: 13227136  
Conc: 5.47 ng/ml





#26 AR-1254-1

R.T.: 5.593 min  
 Delta R.T.: 0.000 min  
 Response: 31329450  
 Conc: 56.01 ng/ml

**Instrument:**  
ECD\_O  
**ClientSampleId :**  
AR1254ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

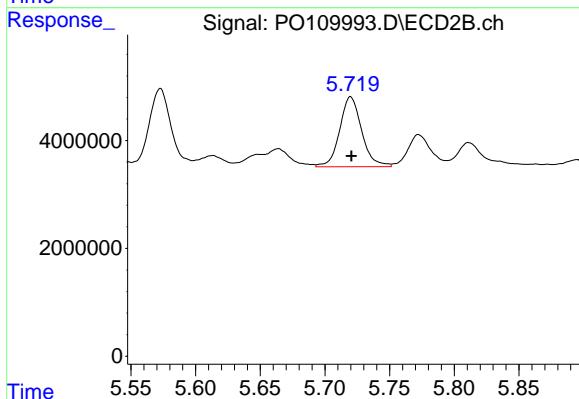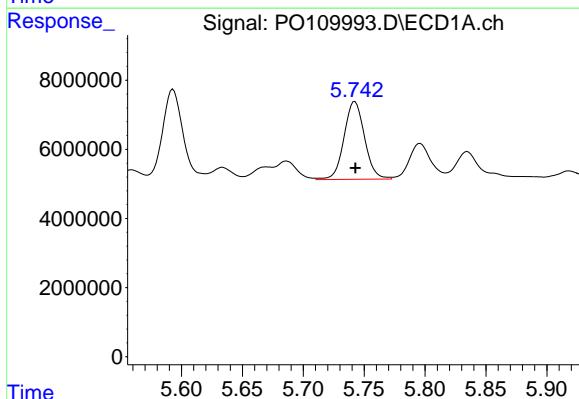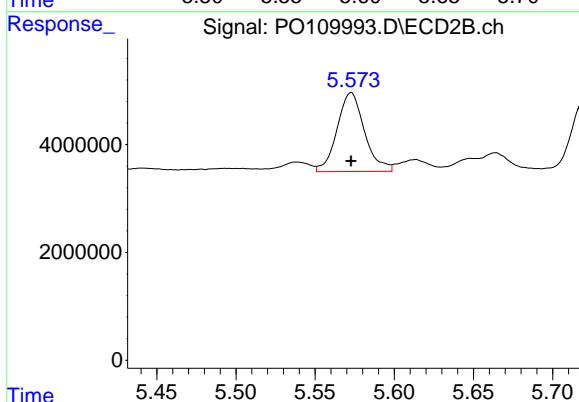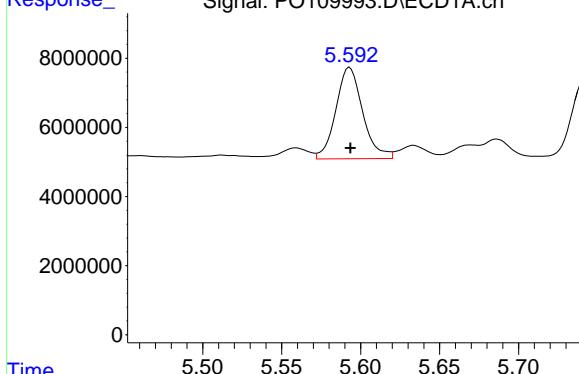

#26 AR-1254-1





R.T.: 5.573 min  
 Delta R.T.: 0.000 min  
 Response: 17649915  
 Conc: 57.36 ng/ml

#27 AR-1254-2

R.T.: 5.742 min  
 Delta R.T.: 0.000 min  
 Response: 26381750  
 Conc: 54.54 ng/ml

#27 AR-1254-2

R.T.: 5.720 min  
 Delta R.T.: 0.000 min  
 Response: 15388259  
 Conc: 57.31 ng/ml

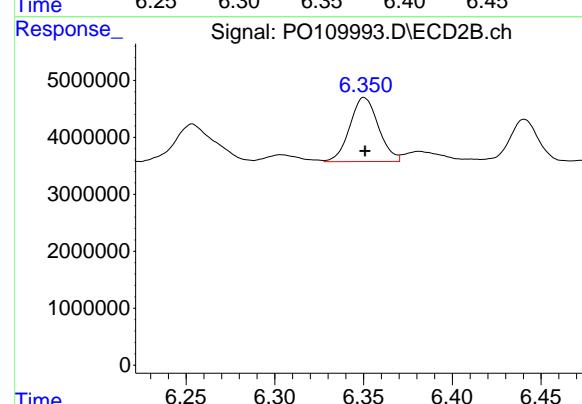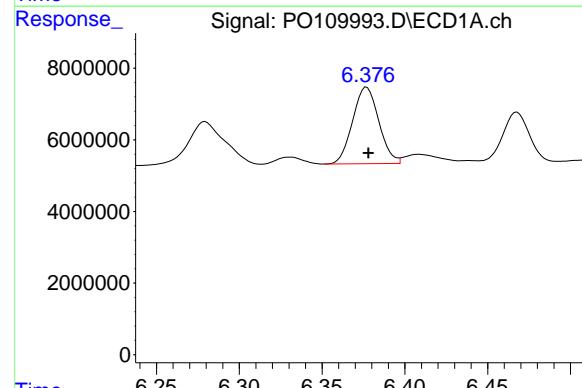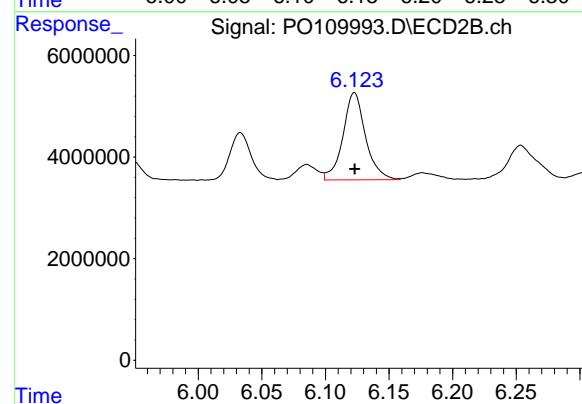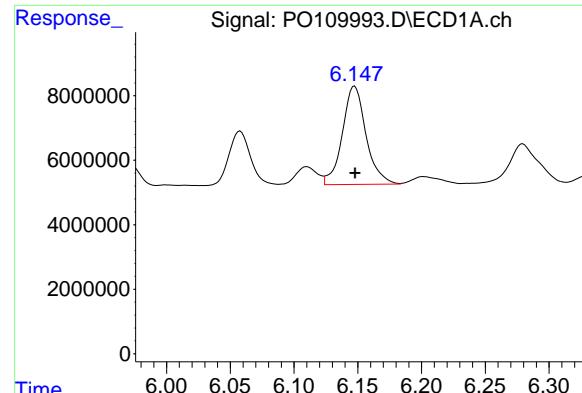

#28 AR-1254-3

R.T.: 6.148 min  
Delta R.T.: 0.000 min  
Response: 39484048  
Conc: 50.03 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

#28 AR-1254-3

R.T.: 6.123 min  
Delta R.T.: 0.000 min  
Response: 21241930  
Conc: 50.43 ng/ml

#29 AR-1254-4

R.T.: 6.377 min  
Delta R.T.: 0.000 min  
Response: 23571245  
Conc: 48.46 ng/ml

#29 AR-1254-4

R.T.: 6.350 min  
Delta R.T.: 0.000 min  
Response: 12628885  
Conc: 51.68 ng/ml



#30 AR-1254-5

R.T.: 6.797 min  
 Delta R.T.: 0.000 min  
 Response: 28479203  
 Conc: 41.85 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1254ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

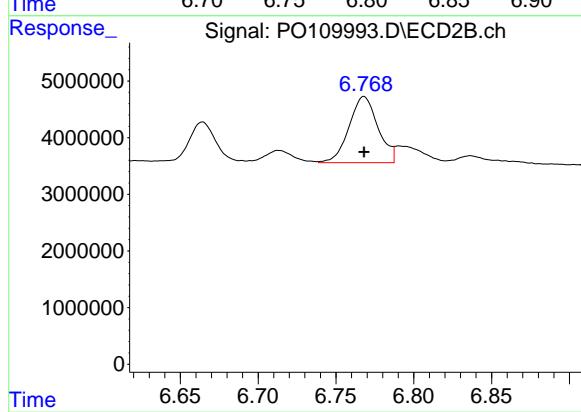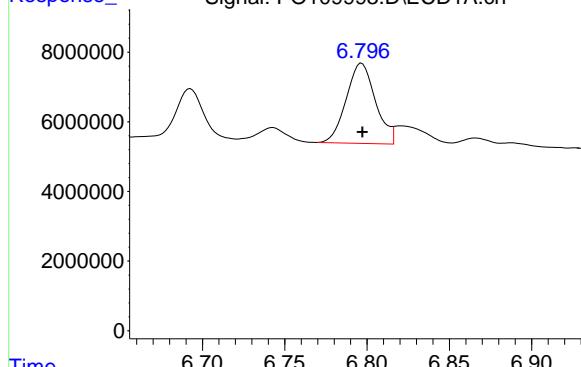

#30 AR-1254-5

R.T.: 6.768 min  
 Delta R.T.: 0.000 min  
 Response: 15116419  
 Conc: 43.36 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109994.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 20:43  
 Operator : YP/AJ  
 Sample : AR1262ICC500  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1262ICC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:59:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:59:23 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	443.4E6	253.7E6	50.000	50.000
2) SA Decachlor...	8.744	8.695	383.2E6	113.8E6	50.000	50.000

Target Compounds

36) L8 AR-1262-1	6.836	6.807	344.1E6	172.2E6	500.000	500.000
37) L8 AR-1262-2	7.338	7.306	596.0E6	268.6E6	500.000	500.000
38) L8 AR-1262-3	7.623	7.590	235.3E6	97025324	500.000	500.000
39) L8 AR-1262-4	7.687	7.654	437.3E6	180.9E6	500.000	500.000
40) L8 AR-1262-5	8.184	8.146	197.2E6	70580972	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109994.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 20:43  
 Operator : YP/AJ  
 Sample : AR1262ICC500  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1262ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:59:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:59:23 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

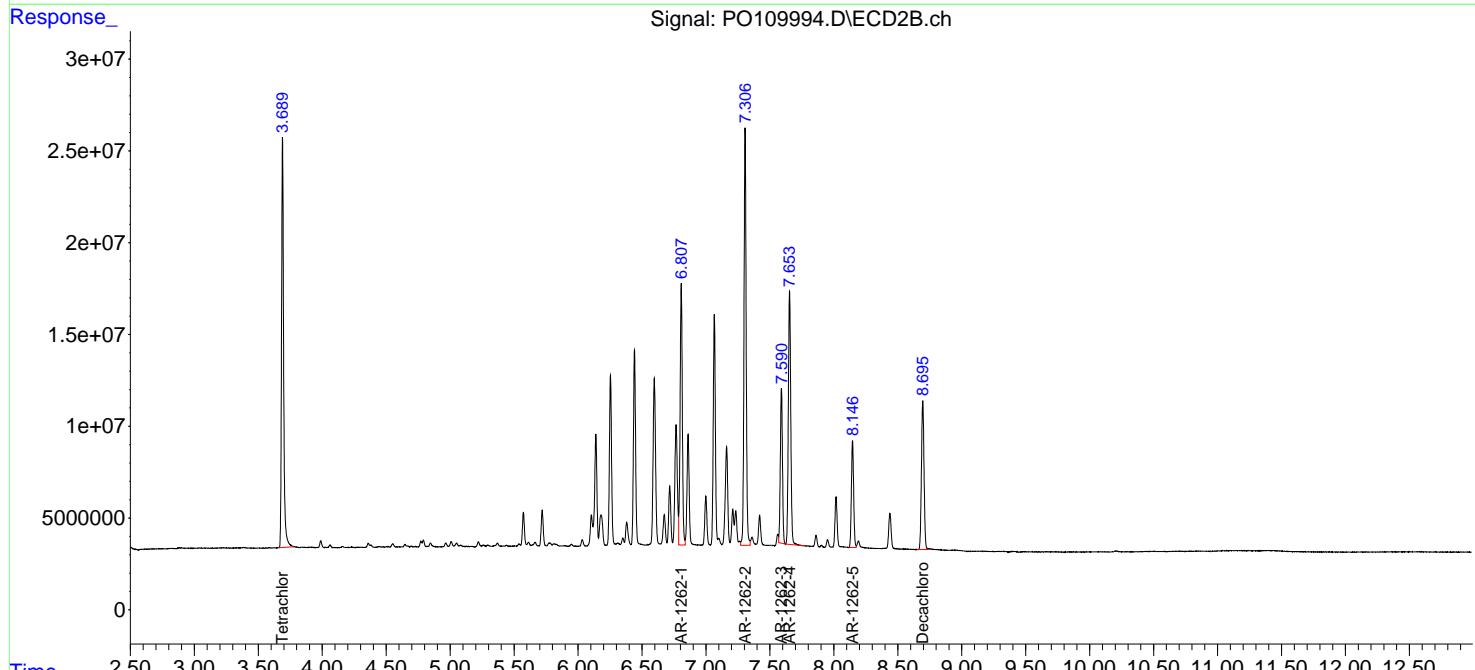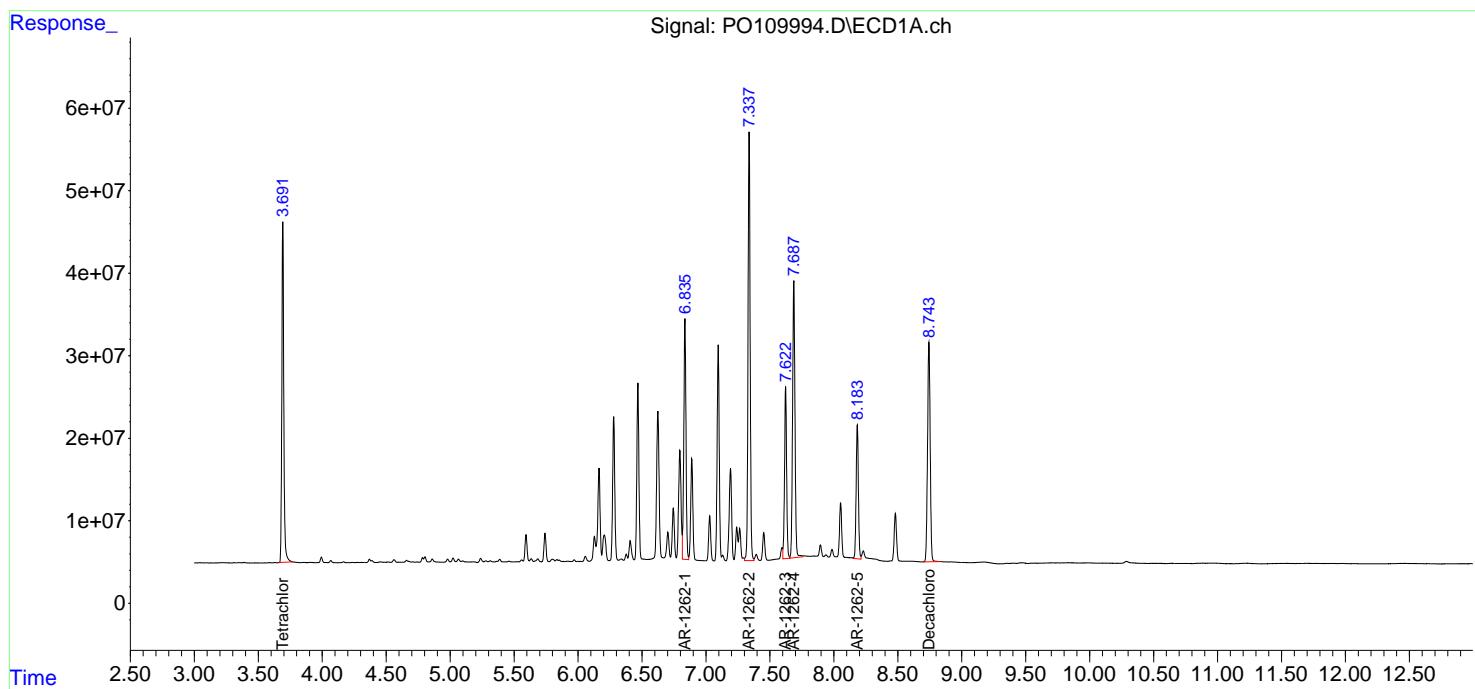

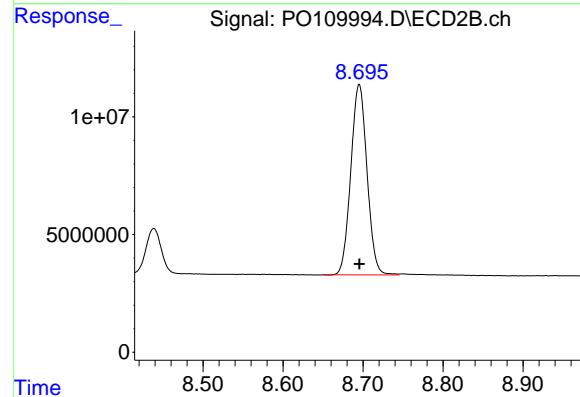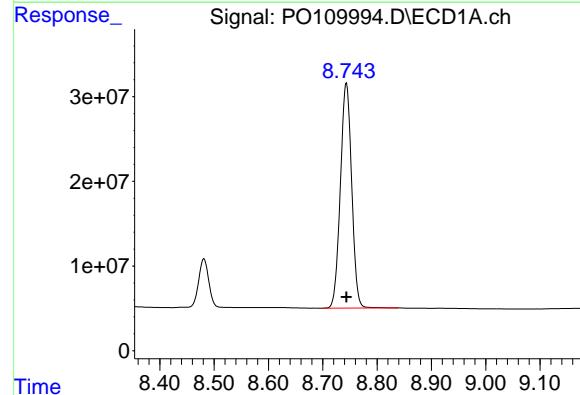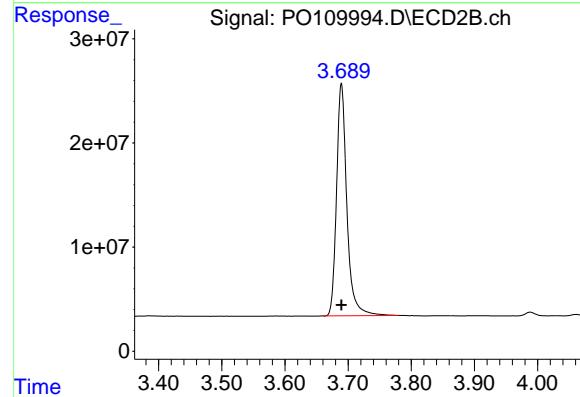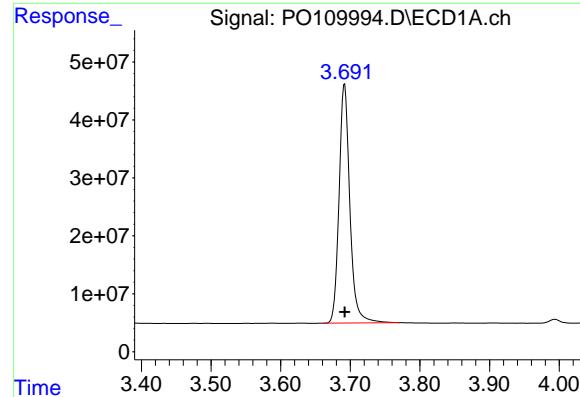

#1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 443392340  
Conc: 50.00 ng/ml

**Instrument:**  
ECD\_O  
**ClientSampleId:**  
AR1262ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 253657981  
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 383169446  
Conc: 50.00 ng/ml





#2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 113848015  
Conc: 50.00 ng/ml

#36 AR-1262-1

R.T.: 6.836 min  
 Delta R.T.: 0.000 min  
 Response: 344060290  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1262ICC500

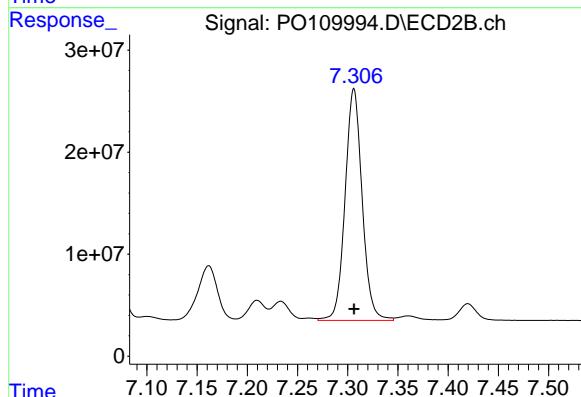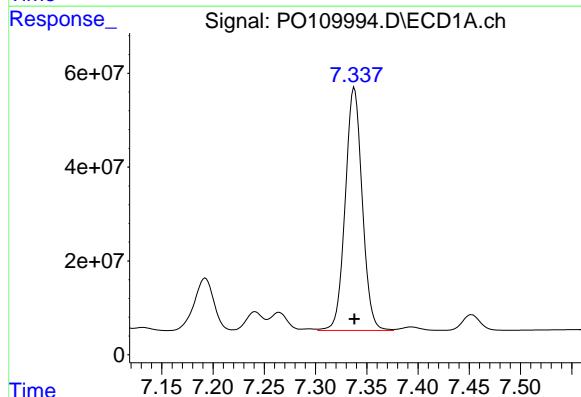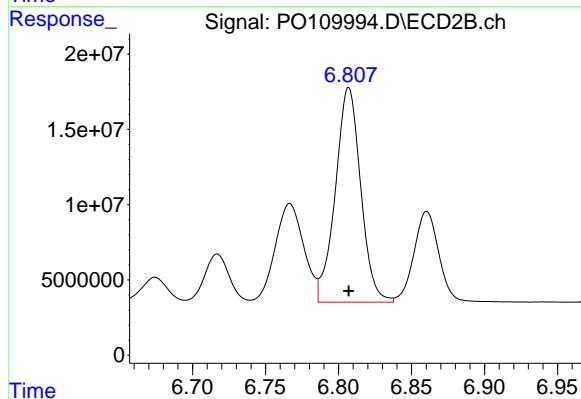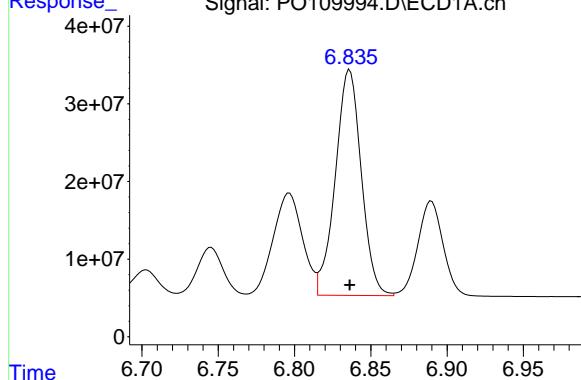

#36 AR-1262-1

R.T.: 6.807 min  
 Delta R.T.: 0.000 min  
 Response: 172156478  
 Conc: 500.00 ng/ml

#37 AR-1262-2

R.T.: 7.338 min  
 Delta R.T.: 0.000 min  
 Response: 595986678  
 Conc: 500.00 ng/ml


#37 AR-1262-2

R.T.: 7.306 min  
 Delta R.T.: 0.000 min  
 Response: 268610130  
 Conc: 500.00 ng/ml

#38 AR-1262-3


R.T.: 7.623 min  
 Delta R.T.: 0.000 min  
 Response: 235314860  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1262ICC500

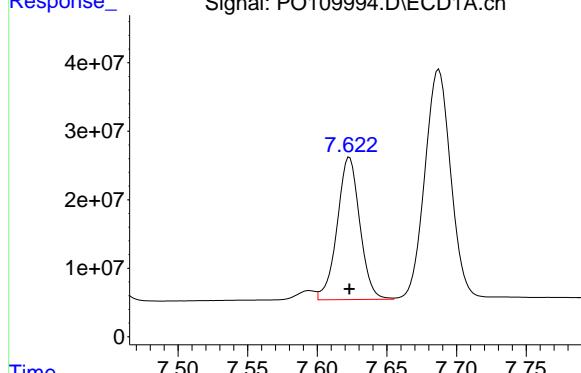


#38 AR-1262-3

R.T.: 7.590 min  
 Delta R.T.: 0.000 min  
 Response: 97025324  
 Conc: 500.00 ng/ml

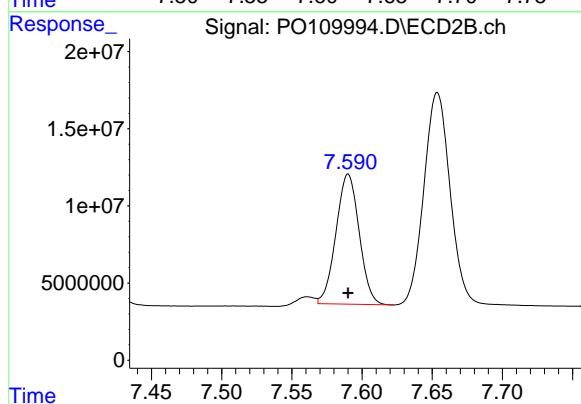


#39 AR-1262-4

R.T.: 7.687 min  
 Delta R.T.: 0.000 min  
 Response: 437287698  
 Conc: 500.00 ng/ml

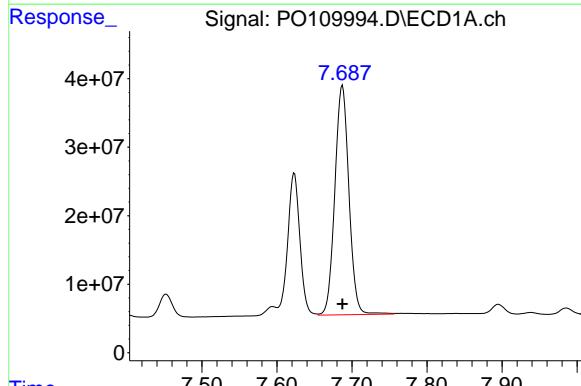

#39 AR-1262-4



R.T.: 7.654 min  
 Delta R.T.: 0.000 min  
 Response: 180893327  
 Conc: 500.00 ng/ml

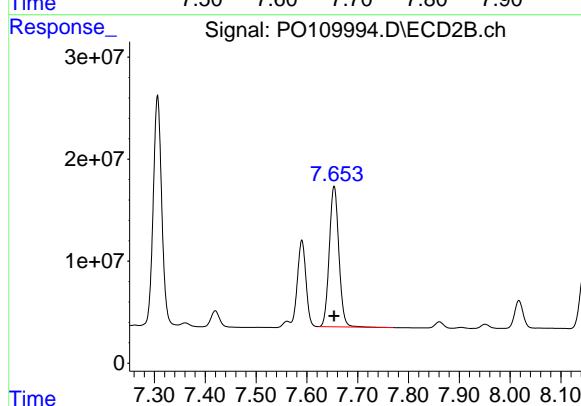

#40 AR-1262-5

R.T.: 8.184 min  
Delta R.T.: 0.000 min  
Response: 197221208  
Conc: 500.00 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1262ICC500

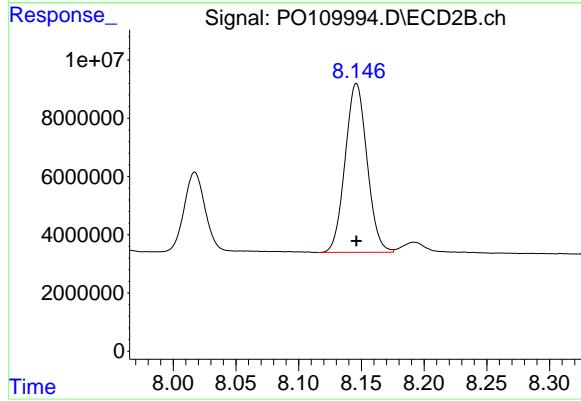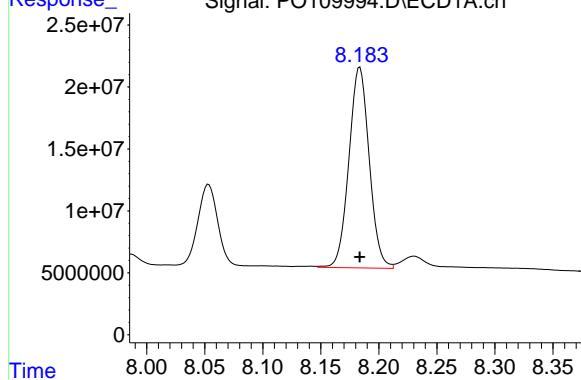

#40 AR-1262-5

R.T.: 8.146 min  
Delta R.T.: 0.000 min  
Response: 70580972  
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109995.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:02  
 Operator : YP/AJ  
 Sample : AR1268ICC1000  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1268ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:17 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	901.7E6	515.8E6	97.188	97.661
2) SA Decachlor...	8.743	8.696	1364.0E6	390.3E6	96.599	94.170

Target Compounds

41) L9 AR-1268-1	7.623	7.590	1369.8E6	560.8E6	976.135	969.827
42) L9 AR-1268-2	7.688	7.655	1266.3E6	519.2E6	989.578	974.786
43) L9 AR-1268-3	7.896	7.862	1019.7E6	397.6E6	981.758	963.023
44) L9 AR-1268-4	8.183	8.147	432.7E6	153.8E6	967.005	949.196
45) L9 AR-1268-5	8.481	8.440	3202.1E6	963.7E6	991.799	976.212



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109995.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:02  
 Operator : YP/AJ  
 Sample : AR1268ICC1000  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1268ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:17 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

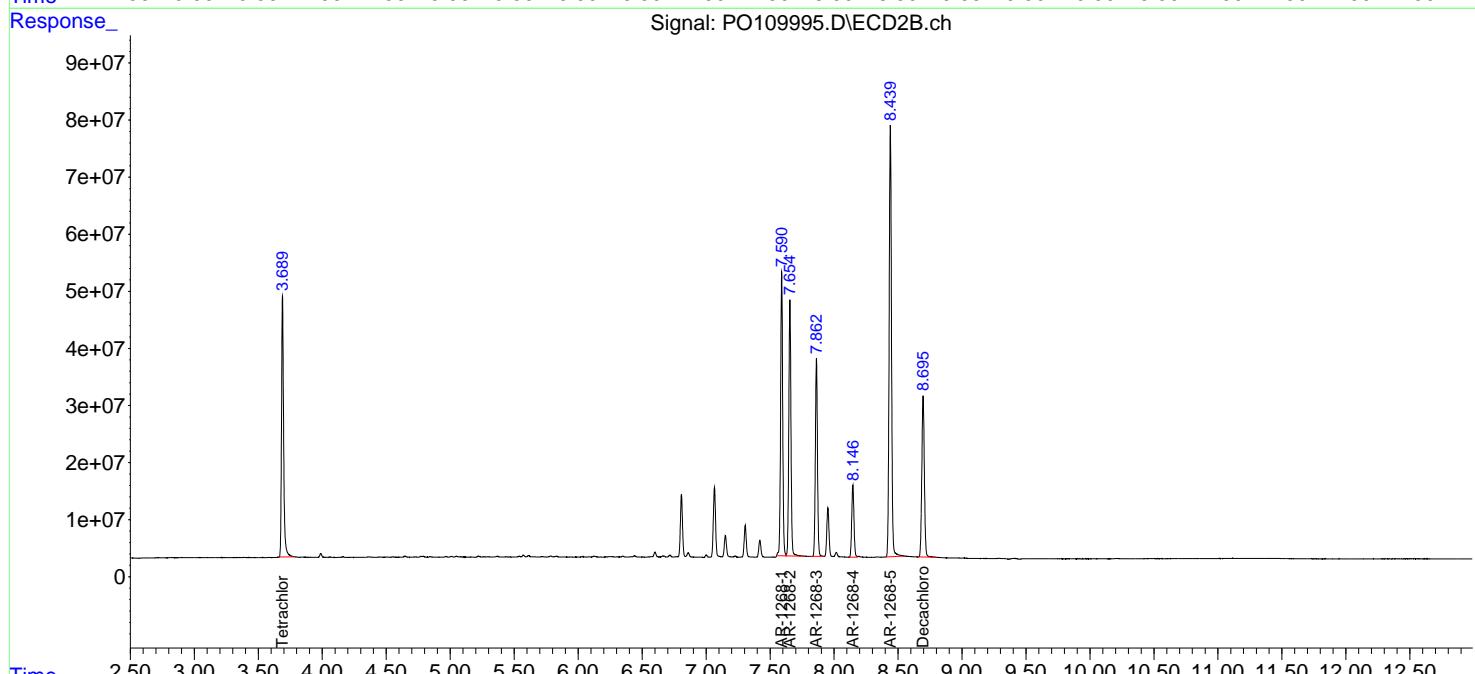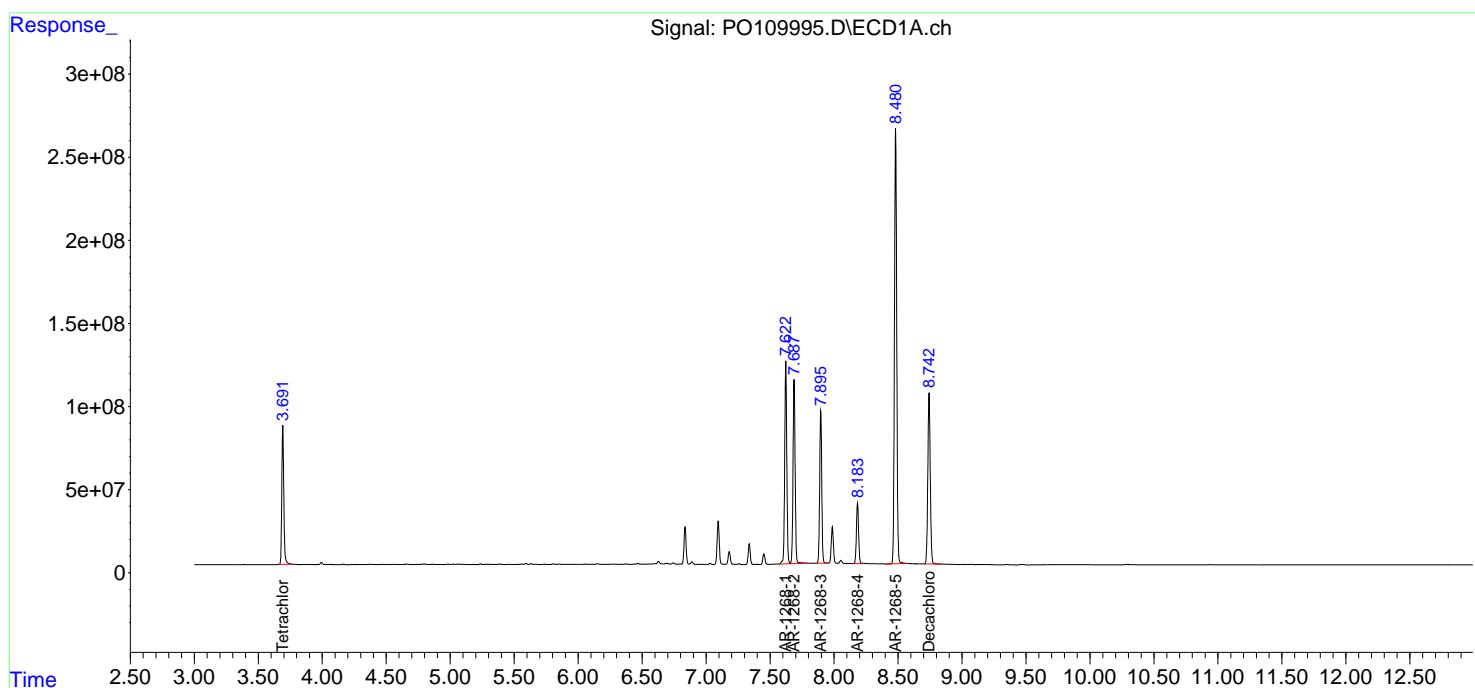

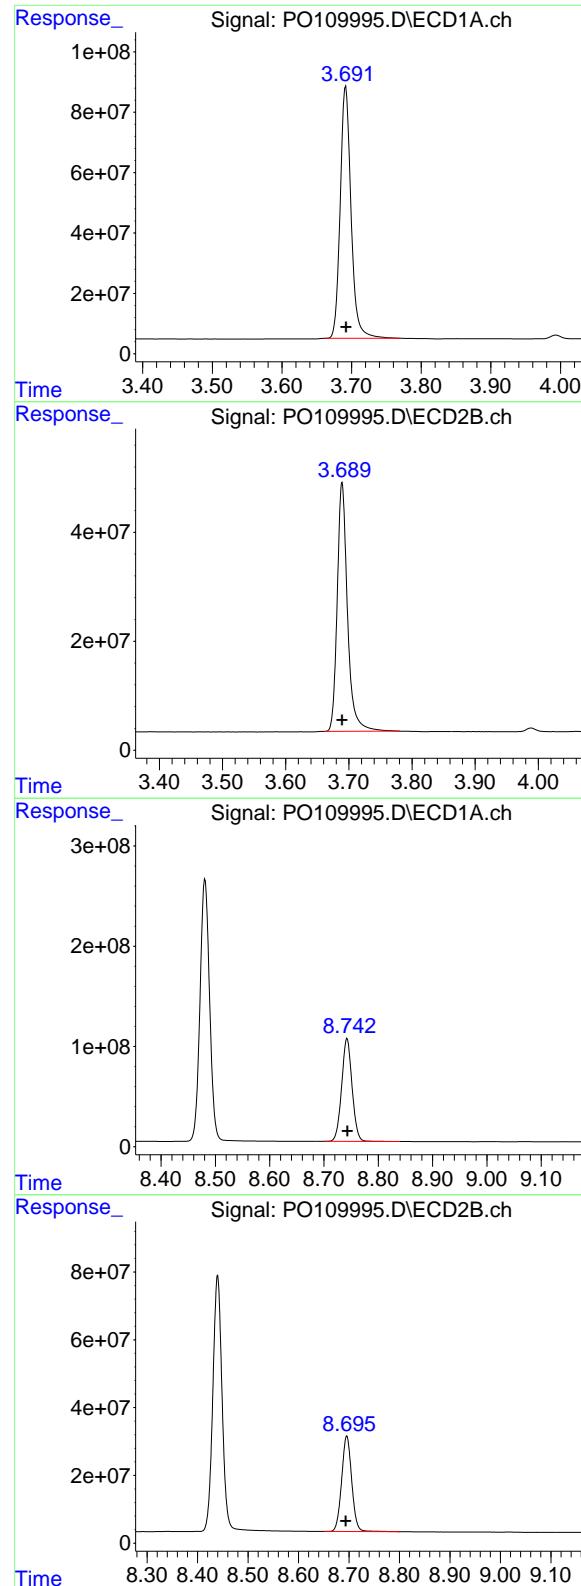

#1 Tetrachloro-m-xylene

R.T.: 3.692 min  
 Delta R.T.: 0.000 min  
 Response: 901662125  
 Conc: 97.19 ng/ml

Instrument:

ECD\_O

ClientSampleId :

AR1268ICC1000

#1 Tetrachloro-m-xylene





R.T.: 3.689 min  
 Delta R.T.: 0.000 min  
 Response: 515836411  
 Conc: 97.66 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.743 min  
 Delta R.T.: 0.000 min  
 Response: 1364000629  
 Conc: 96.60 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.696 min  
 Delta R.T.: 0.002 min  
 Response: 390263390  
 Conc: 94.17 ng/ml

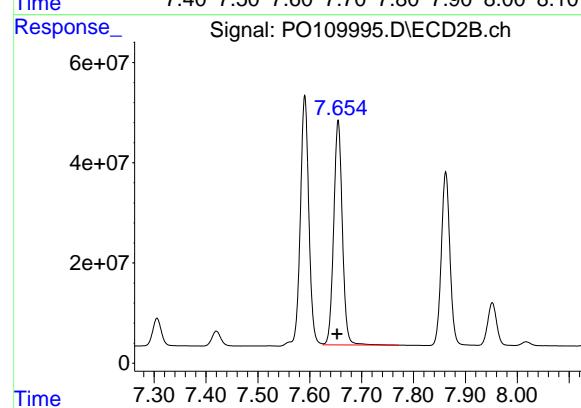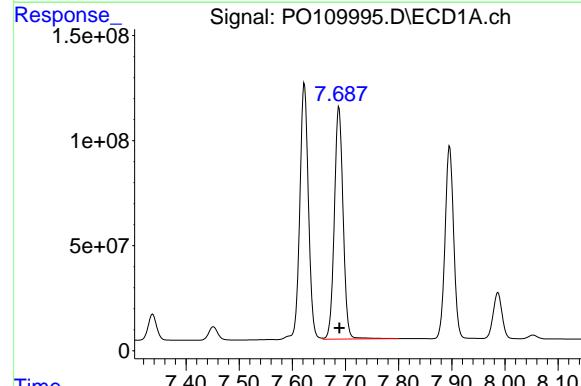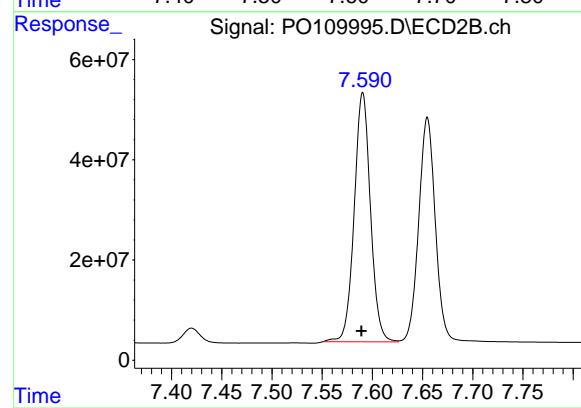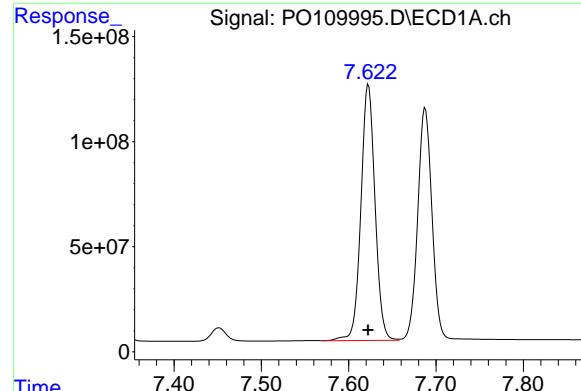

#41 AR-1268-1

R.T.: 7.623 min  
Delta R.T.: 0.000 min  
Response: 1369838059  
Conc: 976.13 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC1000

#41 AR-1268-1

R.T.: 7.590 min  
Delta R.T.: 0.001 min  
Response: 560759375  
Conc: 969.83 ng/ml


#42 AR-1268-2

R.T.: 7.688 min  
Delta R.T.: 0.000 min  
Response: 1266296617  
Conc: 989.58 ng/ml


#42 AR-1268-2

R.T.: 7.655 min  
Delta R.T.: 0.002 min  
Response: 519206129  
Conc: 974.79 ng/ml


Response\_ Signal: PO109995.D\ECD1A.ch

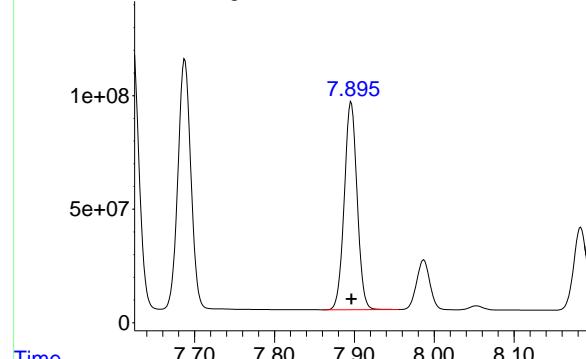


Response\_ Signal: PO109995.D\ECD2B.ch

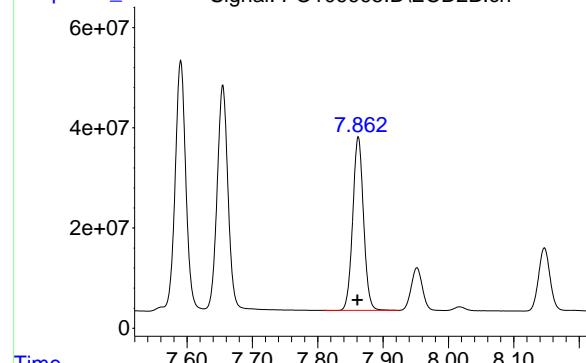

Response\_ Signal: PO109995.D\ECD1A.ch

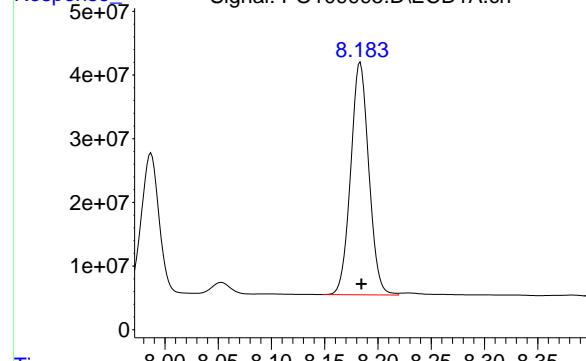

Response\_ Signal: PO109995.D\ECD2B.ch

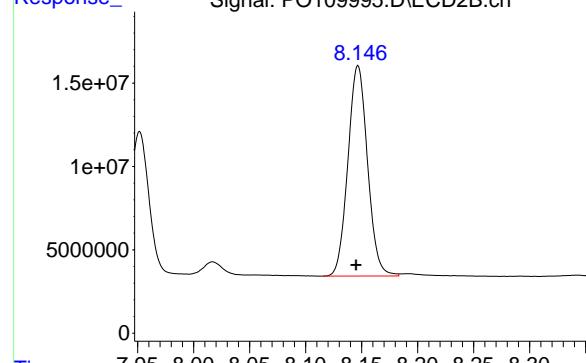

#43 AR-1268-3

R.T.: 7.896 min  
Delta R.T.: 0.000 min  
Response: 1019701747  
Conc: 981.76 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC1000

#43 AR-1268-3

R.T.: 7.862 min  
Delta R.T.: 0.001 min  
Response: 397648794  
Conc: 963.02 ng/ml

#44 AR-1268-4

R.T.: 8.183 min  
Delta R.T.: -0.001 min  
Response: 432675859  
Conc: 967.01 ng/ml



#44 AR-1268-4

R.T.: 8.147 min  
Delta R.T.: 0.002 min  
Response: 153792414  
Conc: 949.20 ng/ml

#45 AR-1268-5

R.T.: 8.481 min  
Delta R.T.: -0.001 min  
Response: 3202130253  
Conc: 991.80 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1268ICC1000

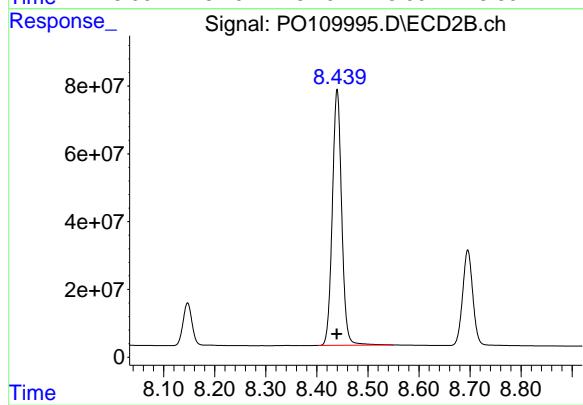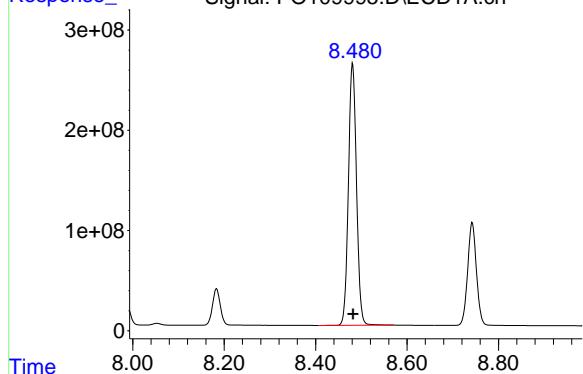

#45 AR-1268-5

R.T.: 8.440 min  
Delta R.T.: 0.001 min  
Response: 963659212  
Conc: 976.21 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109996.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:20  
 Operator : YP/AJ  
 Sample : AR1268ICC750  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1268ICC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:27 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	674.6E6	386.9E6	72.709	73.243
2) SA Decachlor...	8.743	8.696	1030.2E6	298.8E6	72.957	72.092

Target Compounds

41) L9 AR-1268-1	7.624	7.590	1030.8E6	426.7E6	734.560	738.041
42) L9 AR-1268-2	7.688	7.655	947.1E6	394.0E6	740.097	739.739
43) L9 AR-1268-3	7.897	7.862	764.7E6	299.7E6	736.208	725.732
44) L9 AR-1268-4	8.184	8.147	316.0E6	116.0E6	706.276	715.999
45) L9 AR-1268-5	8.482	8.440	2394.2E6	724.9E6	741.545	734.374



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109996.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:20  
 Operator : YP/AJ  
 Sample : AR1268ICC750  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1268ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:27 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

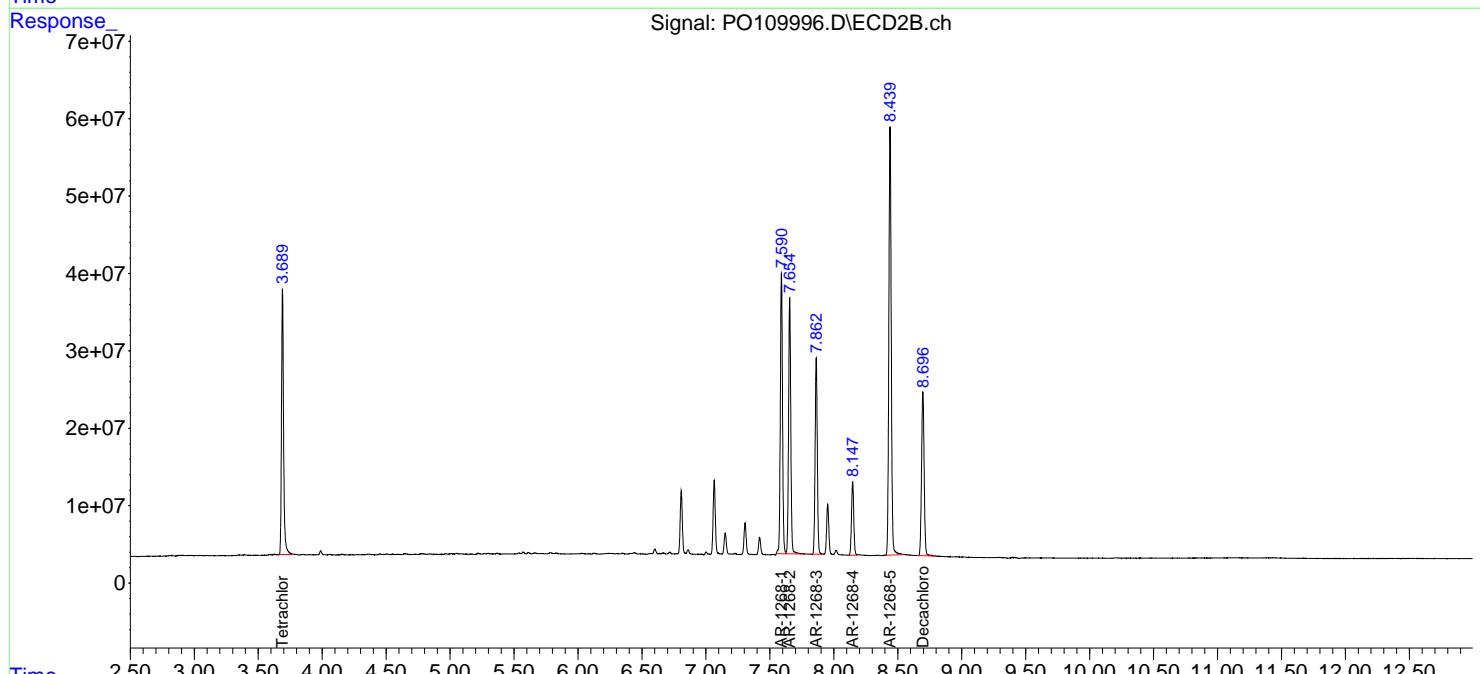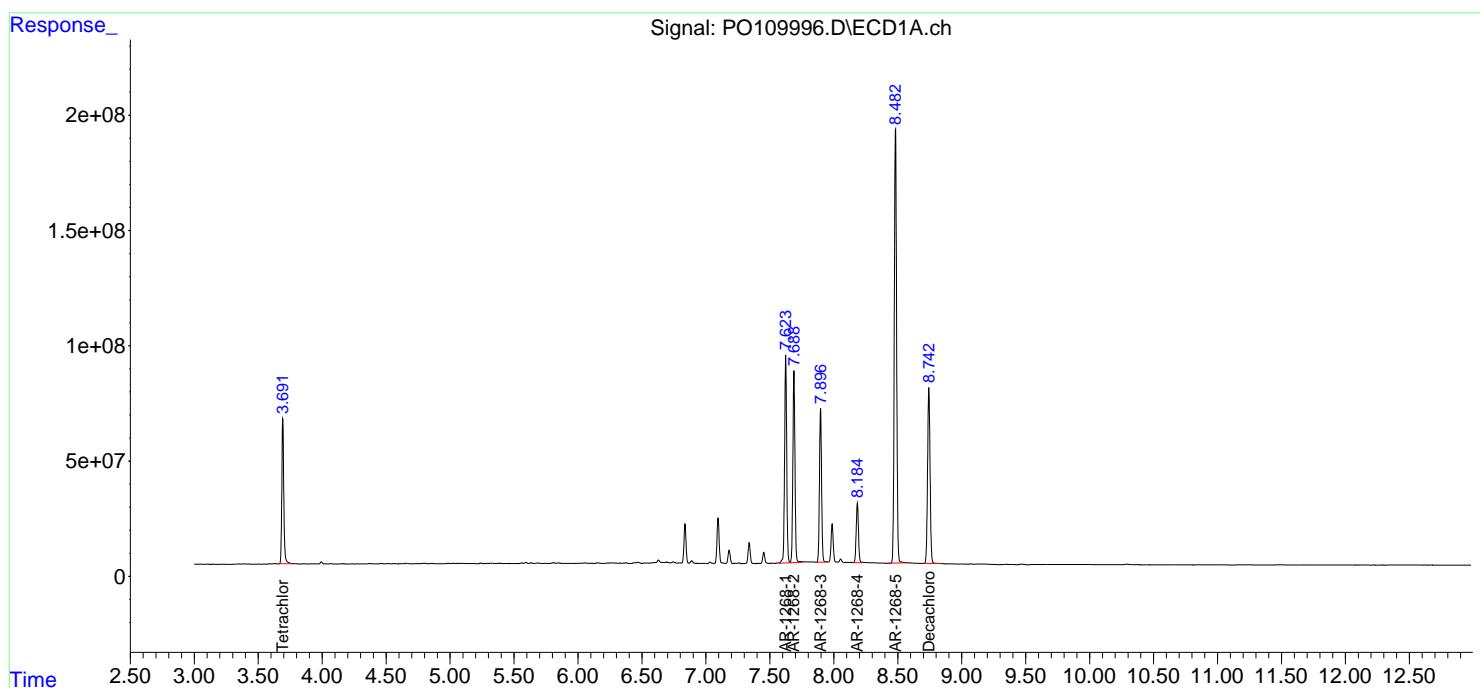

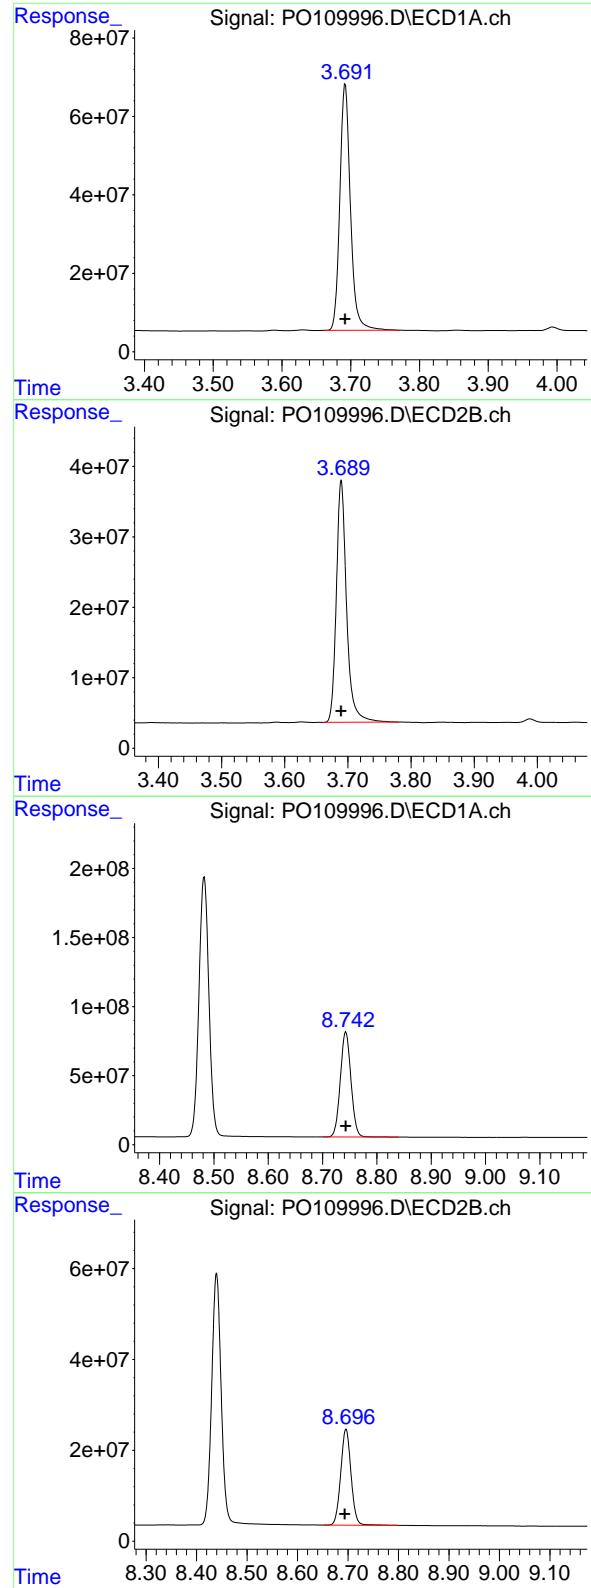

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 674561518  
Conc: 72.71 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC750

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 386863871  
Conc: 73.24 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.743 min  
Delta R.T.: 0.000 min  
Response: 1030169782  
Conc: 72.96 ng/ml


## #2 Decachlorobiphenyl

R.T.: 8.696 min  
Delta R.T.: 0.002 min  
Response: 298767454  
Conc: 72.09 ng/ml

#41 AR-1268-1


R.T.: 7.624 min  
 Delta R.T.: 0.002 min  
 Response: 1030829535  
 Conc: 734.56 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC750

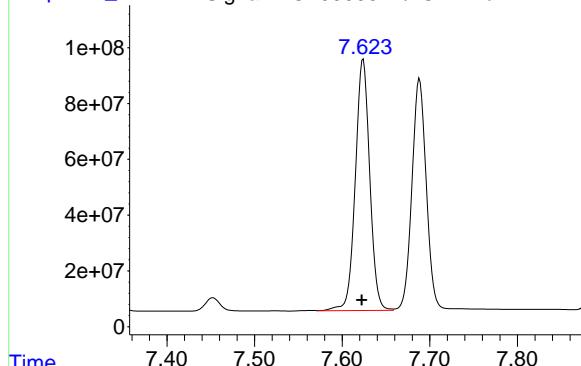


#41 AR-1268-1

R.T.: 7.590 min  
 Delta R.T.: 0.001 min  
 Response: 426739530  
 Conc: 738.04 ng/ml

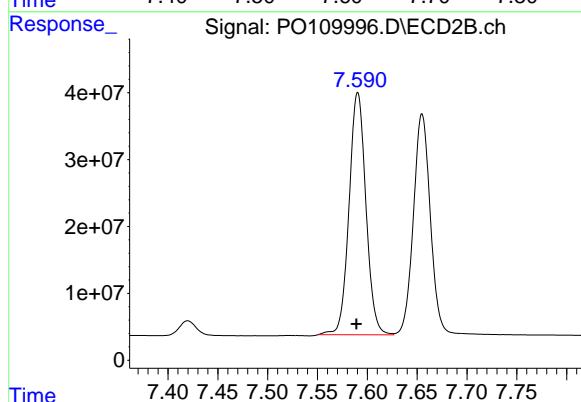


#42 AR-1268-2

R.T.: 7.688 min  
 Delta R.T.: 0.000 min  
 Response: 947052725  
 Conc: 740.10 ng/ml

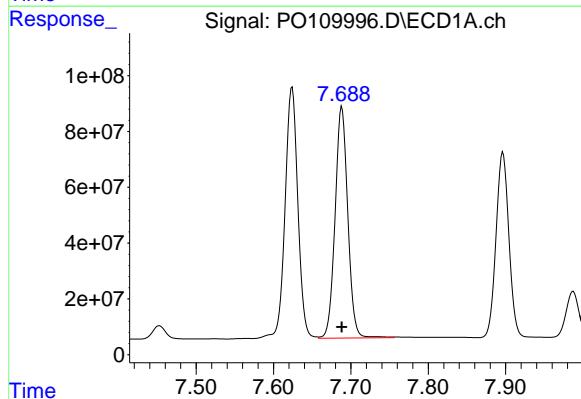

#42 AR-1268-2


R.T.: 7.655 min  
 Delta R.T.: 0.002 min  
 Response: 394011614  
 Conc: 739.74 ng/ml

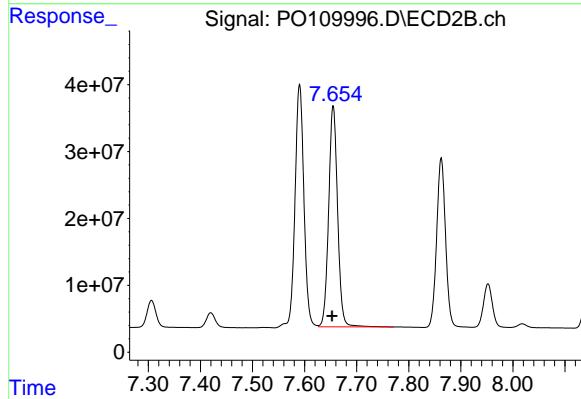

#43 AR-1268-3


R.T.: 7.897 min  
 Delta R.T.: 0.000 min  
 Response: 764660970  
 Conc: 736.21 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC750

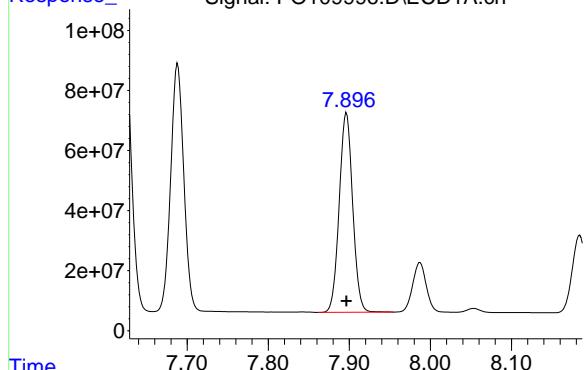


#43 AR-1268-3

R.T.: 7.862 min  
 Delta R.T.: 0.002 min  
 Response: 299667225  
 Conc: 725.73 ng/ml

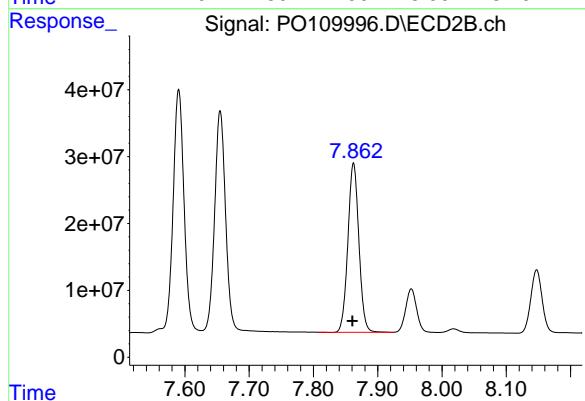


#44 AR-1268-4

R.T.: 8.184 min  
 Delta R.T.: 0.000 min  
 Response: 316015601  
 Conc: 706.28 ng/ml

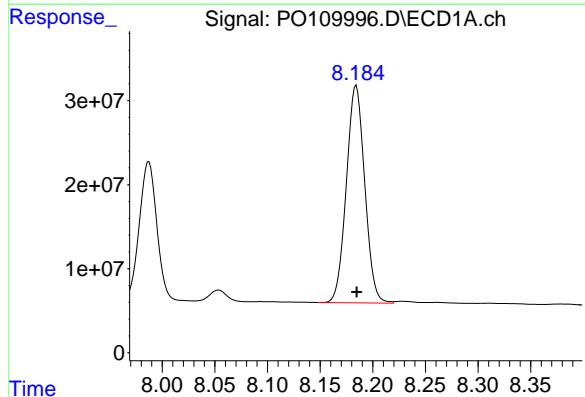

#44 AR-1268-4



R.T.: 8.147 min  
 Delta R.T.: 0.002 min  
 Response: 116008994  
 Conc: 716.00 ng/ml

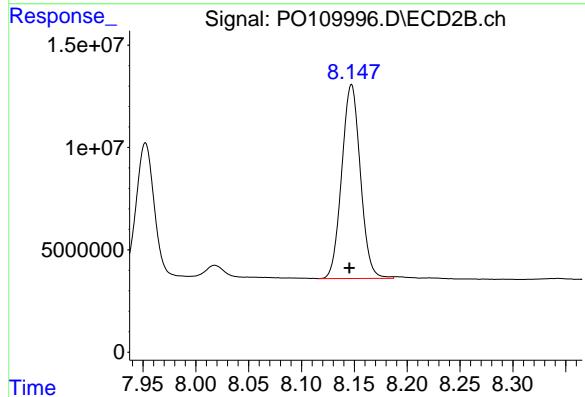

#45 AR-1268-5

R.T.: 8.482 min  
Delta R.T.: 0.000 min  
Response: 2394158307  
Conc: 741.55 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1268ICC750

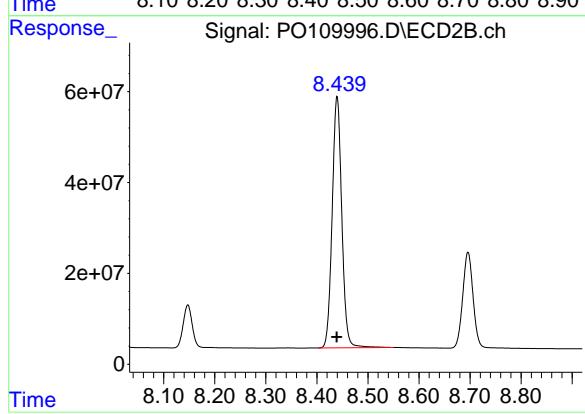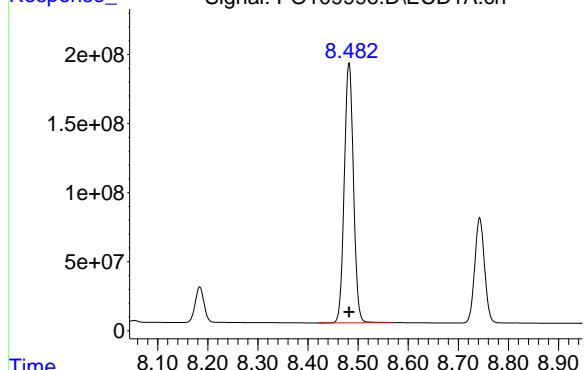

#45 AR-1268-5

R.T.: 8.440 min  
Delta R.T.: 0.000 min  
Response: 724930761  
Conc: 734.37 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109997.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:39  
 Operator : YP/AJ  
 Sample : AR1268ICC500  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1268ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	463.9E6	264.1E6	50.000	50.000
2) SA Decachlor...	8.743	8.694	706.0E6	207.2E6	50.000	50.000

Target Compounds

41) L9 AR-1268-1	7.622	7.589	700.7E6	289.1E6	499.305m	500.000
42) L9 AR-1268-2	7.688	7.653	639.8E6	266.3E6	500.000	500.000
43) L9 AR-1268-3	7.896	7.861	519.3E6	206.5E6	500.000	500.000
44) L9 AR-1268-4	8.185	8.145	223.7E6	81011977	500.000	500.000
45) L9 AR-1268-5	8.482	8.439	1614.3E6	493.6E6	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109997.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:39  
 Operator : YP/AJ  
 Sample : AR1268ICC500  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 AR1268ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

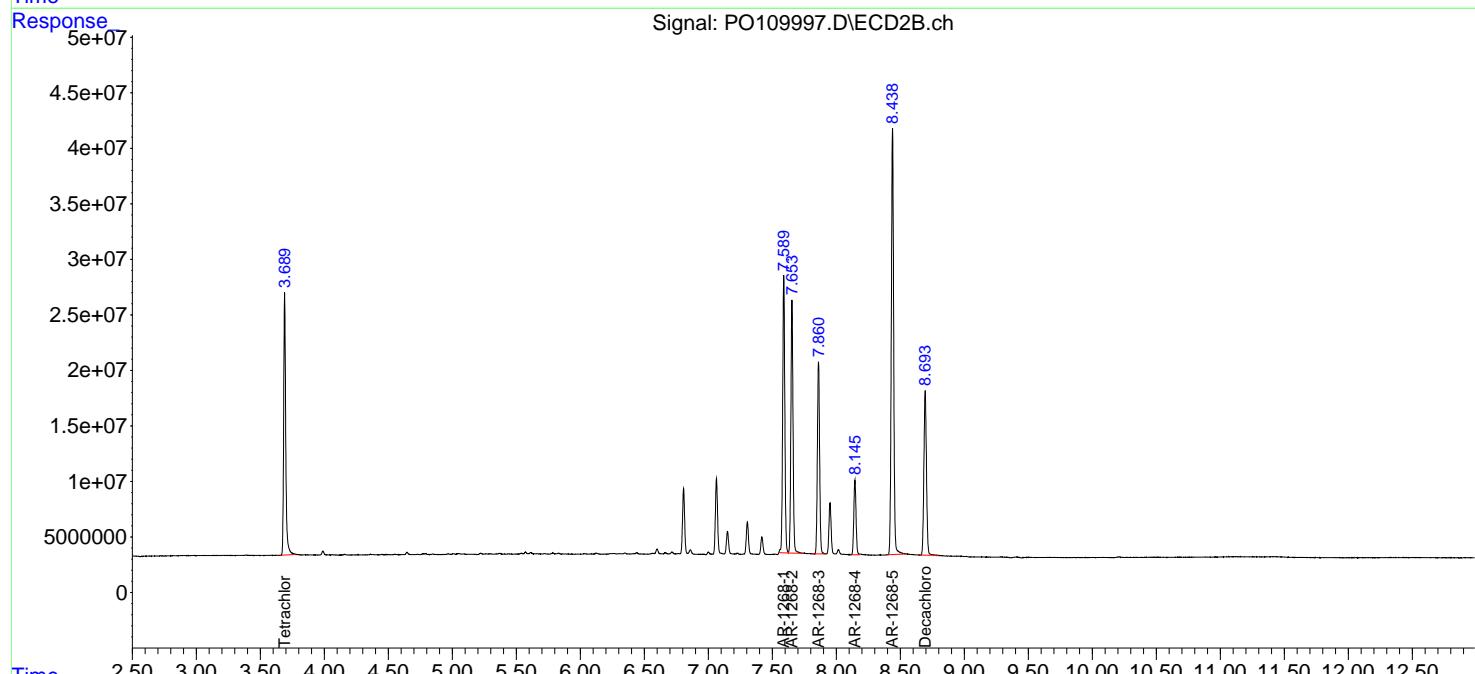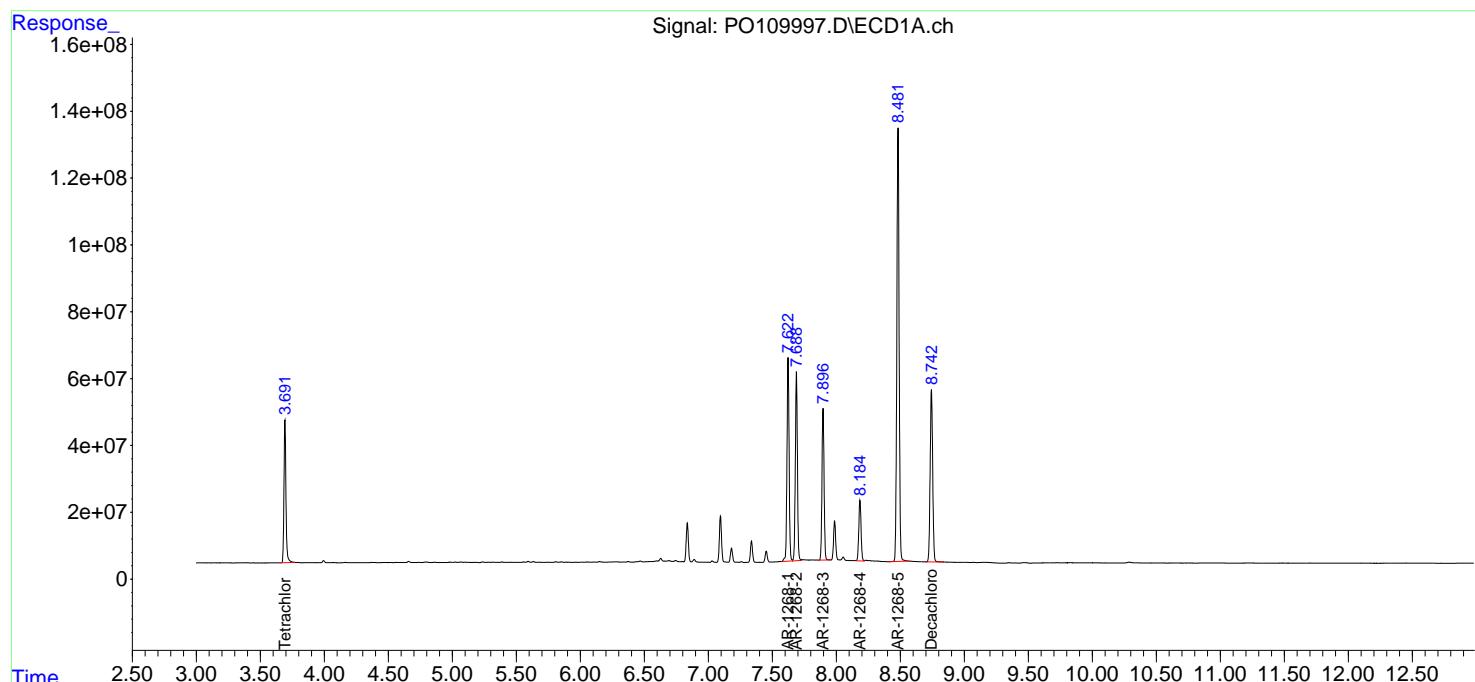

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min

Delta R.T.: 0.000 min

Response: 463875726

Conc: 50.00 ng/ml

Instrument:

ECD\_O


ClientSampleId :

AR1268ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025

Supervised By :mohammad ahmed 03/24/2025

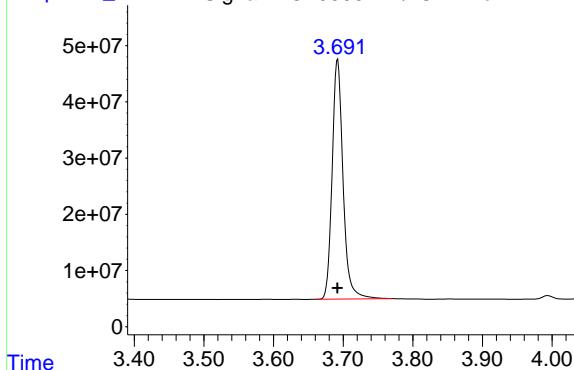


## #1 Tetrachloro-m-xylene

R.T.: 3.689 min

Delta R.T.: 0.000 min

Response: 264095871

Conc: 50.00 ng/ml

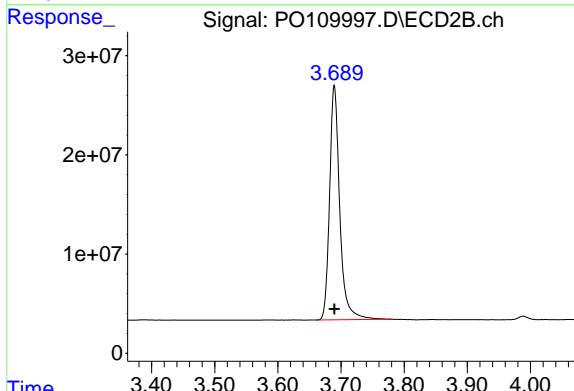


## #2 Decachlorobiphenyl

R.T.: 8.743 min

Delta R.T.: 0.000 min

Response: 706011522

Conc: 50.00 ng/ml

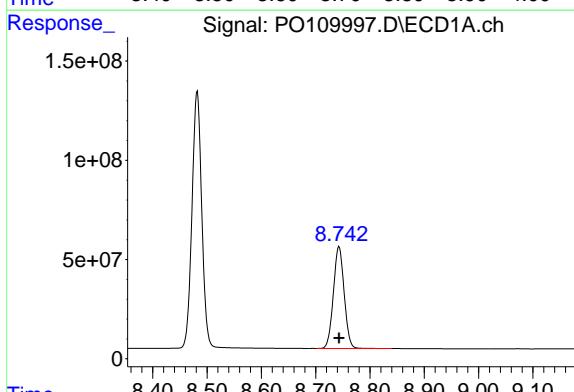


## #2 Decachlorobiphenyl

R.T.: 8.694 min

Delta R.T.: 0.000 min

Response: 207212938

Conc: 50.00 ng/ml

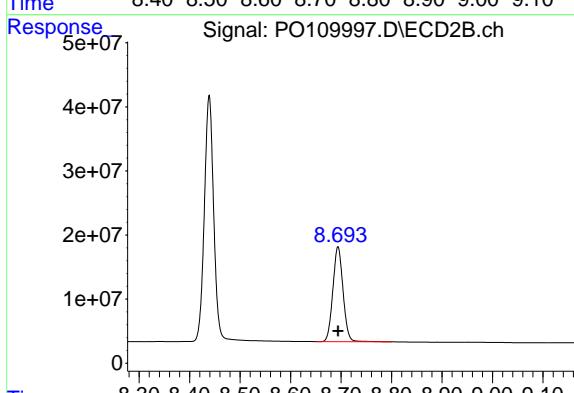

#41 AR-1268-1

R.T.: 7.622 min

Delta R.T.: 0.000 min

Response: 700689003

Conc: 499.31 ng/ml

Instrument:

ECD\_O





ClientSampleId :

AR1268ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025

Supervised By :mohammad ahmed 03/24/2025

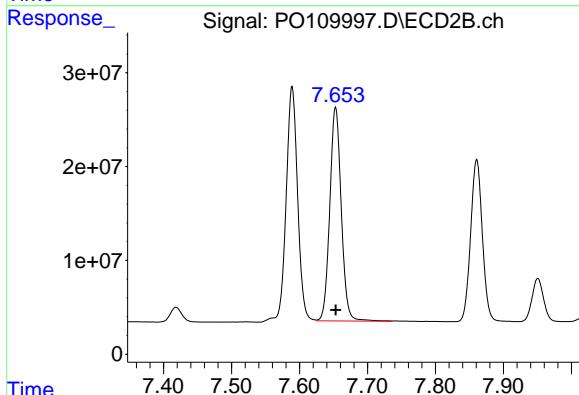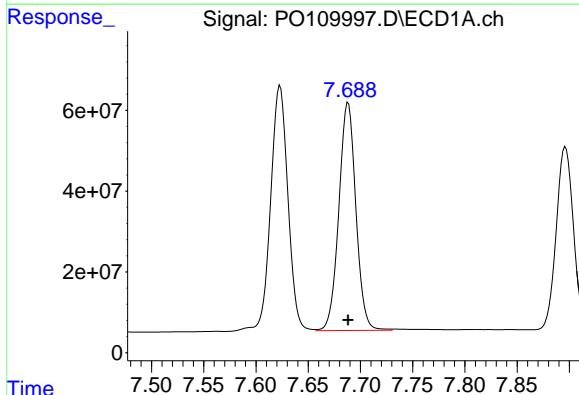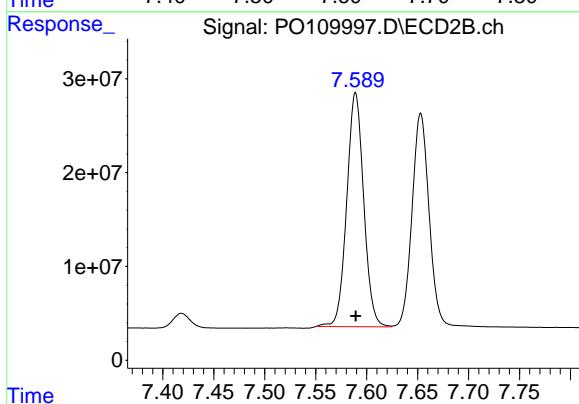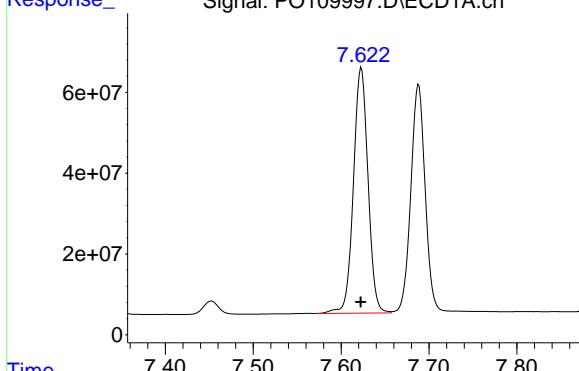

#41 AR-1268-1

R.T.: 7.589 min

Delta R.T.: 0.000 min

Response: 289102857

Conc: 500.00 ng/ml

#42 AR-1268-2

R.T.: 7.688 min

Delta R.T.: 0.000 min

Response: 639816344

Conc: 500.00 ng/ml

#42 AR-1268-2

R.T.: 7.653 min

Delta R.T.: 0.000 min

Response: 266318012

Conc: 500.00 ng/ml





#43 AR-1268-3

R.T.: 7.896 min  
 Delta R.T.: 0.000 min  
 Response: 519324293  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

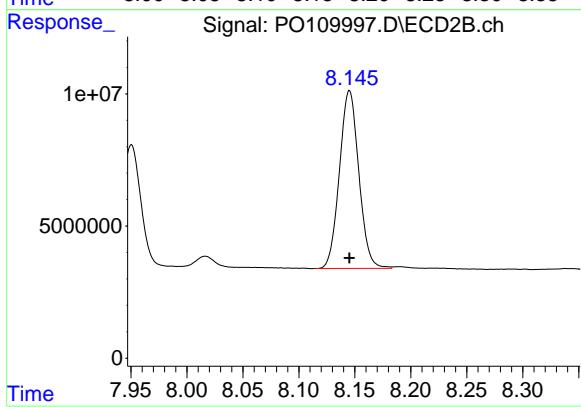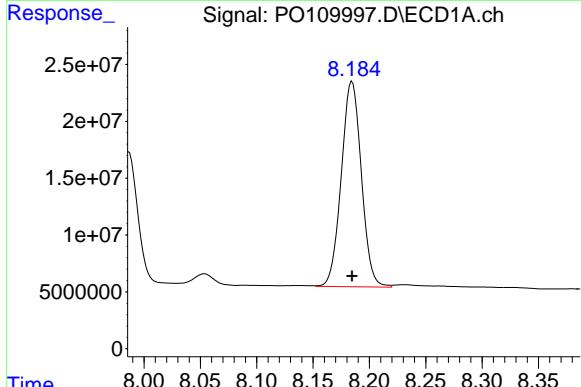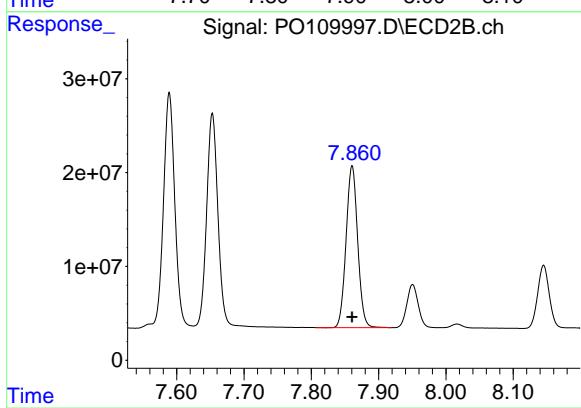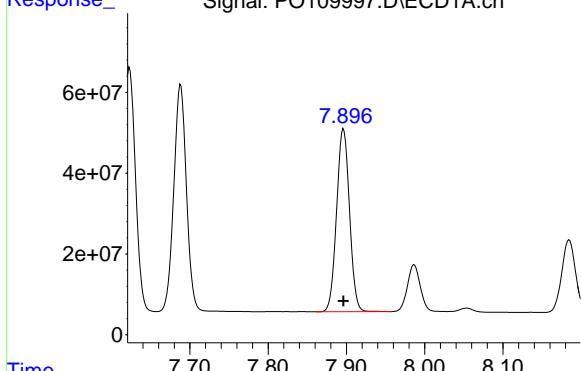

#43 AR-1268-3

R.T.: 7.861 min  
 Delta R.T.: 0.000 min  
 Response: 206458519  
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 8.185 min  
 Delta R.T.: 0.000 min  
 Response: 223719543  
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 8.145 min  
 Delta R.T.: 0.000 min  
 Response: 81011977  
 Conc: 500.00 ng/ml


#45 AR-1268-5

R.T.: 8.482 min  
 Delta R.T.: 0.000 min  
 Response: 1614304087  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

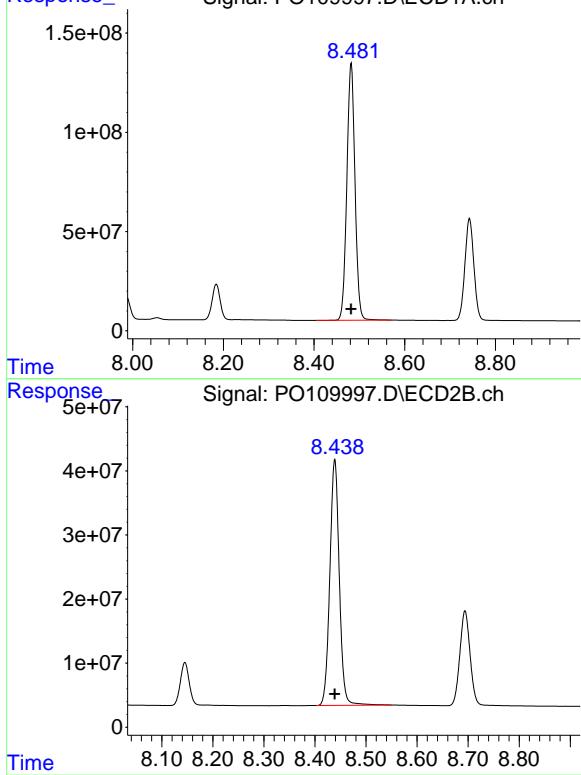

#45 AR-1268-5

R.T.: 8.439 min  
 Delta R.T.: 0.000 min  
 Response: 493570508  
 Conc: 500.00 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109998.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:57  
 Operator : YP/AJ  
 Sample : AR1268ICC250  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1268ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:56 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	233.0E6	133.0E6	25.112	25.182
2) SA Decachlor...	8.743	8.695	364.2E6	110.3E6	25.791	26.624

Target Compounds

41) L9 AR-1268-1	7.623	7.590	357.9E6	149.6E6	255.005m	258.814
42) L9 AR-1268-2	7.688	7.654	330.4E6	137.2E6	258.196	257.558
43) L9 AR-1268-3	7.897	7.861	264.1E6	107.0E6	254.288	259.017
44) L9 AR-1268-4	8.184	8.146	118.3E6	42174671	264.470	260.299
45) L9 AR-1268-5	8.482	8.439	811.9E6	254.0E6	251.483	257.325

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109998.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:57  
 Operator : YP/AJ  
 Sample : AR1268ICC250  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1



**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1268ICC250


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:56 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

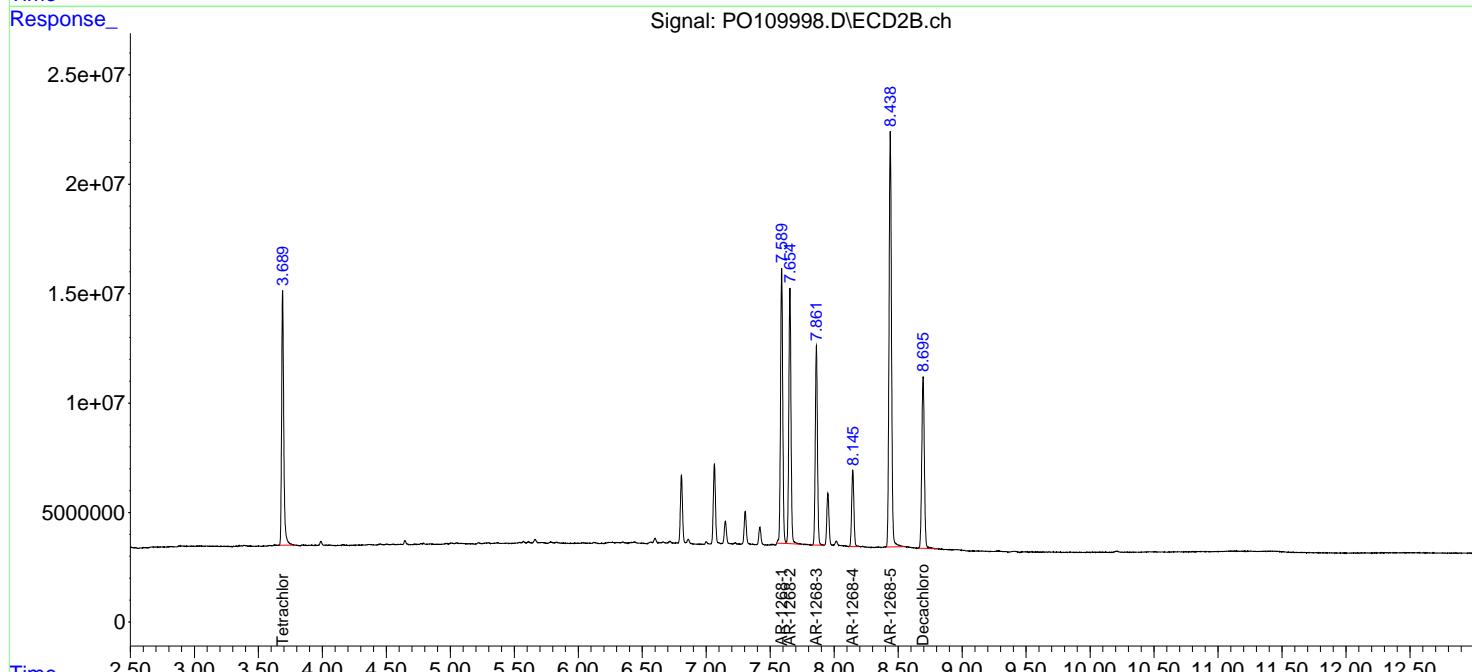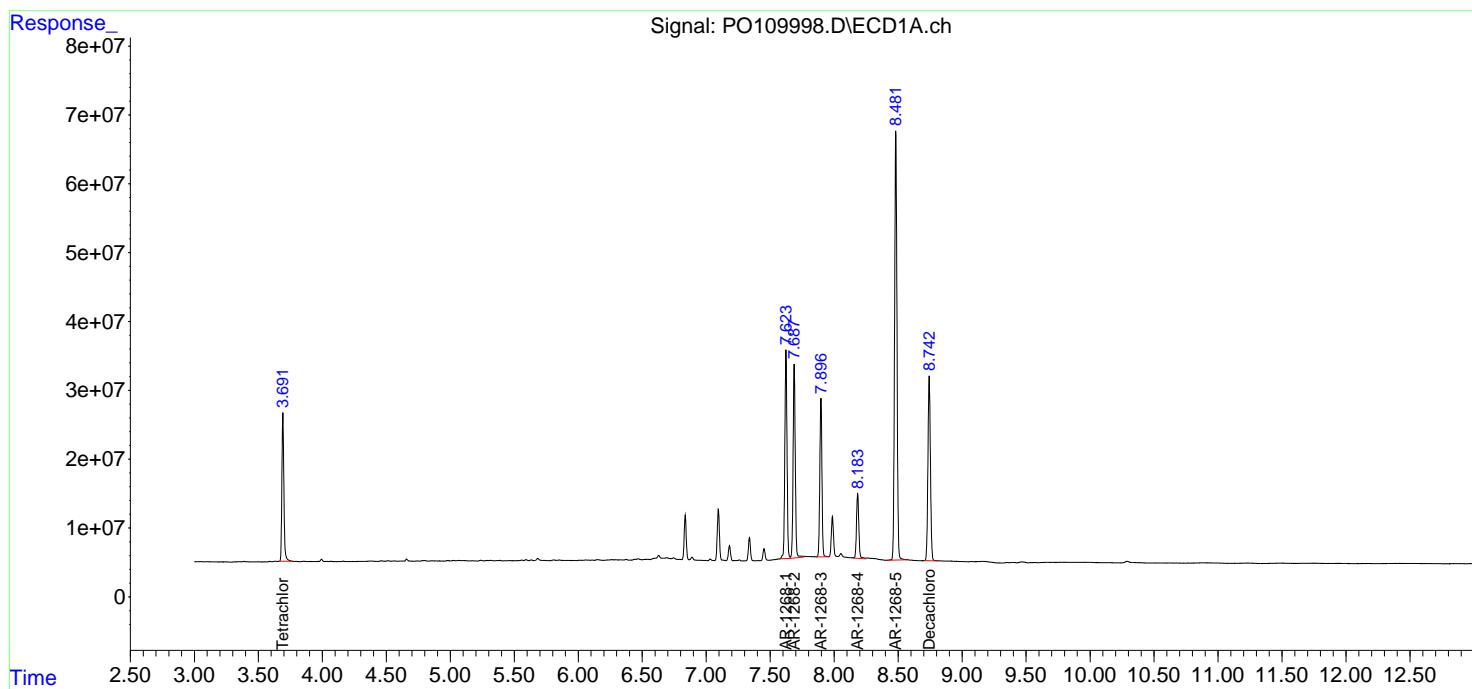

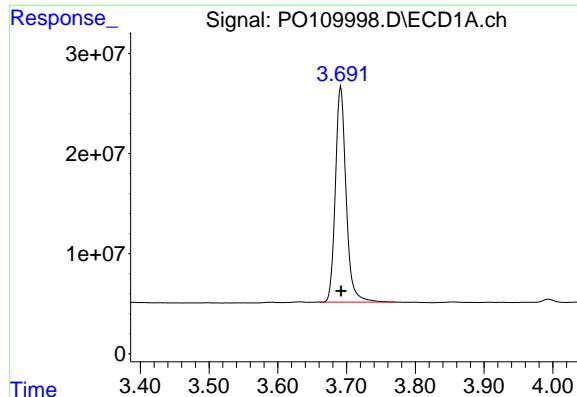


#1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 232978846  
Conc: 25.11 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1268ICC250


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

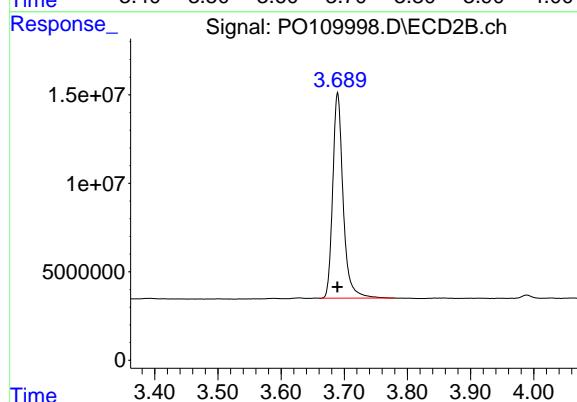


#1 Tetrachloro-m-xylene

R.T.: 3.690 min  
Delta R.T.: 0.000 min  
Response: 133010597  
Conc: 25.18 ng/ml

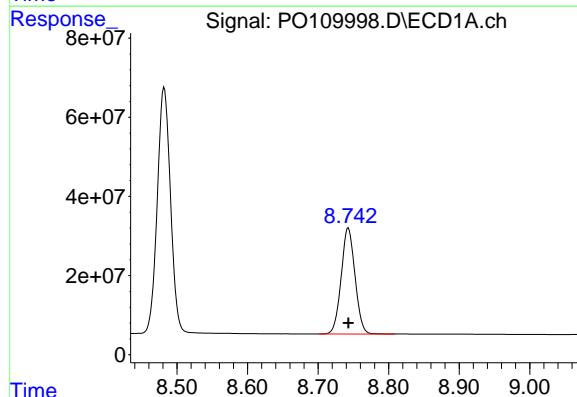

#2 Decachlorobiphenyl

R.T.: 8.743 min  
Delta R.T.: 0.000 min  
Response: 364169510  
Conc: 25.79 ng/ml

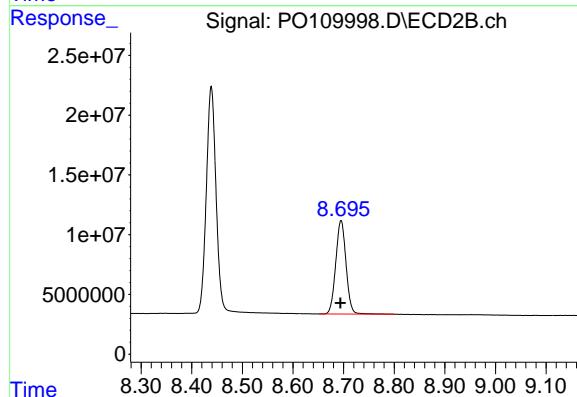

#2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.001 min  
Response: 110337267  
Conc: 26.62 ng/ml





#41 AR-1268-1

R.T.: 7.623 min  
 Delta R.T.: 0.000 min  
 Response: 357855660  
 Conc: 255.00 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

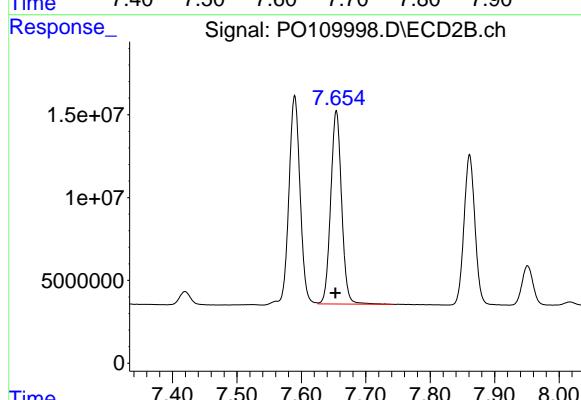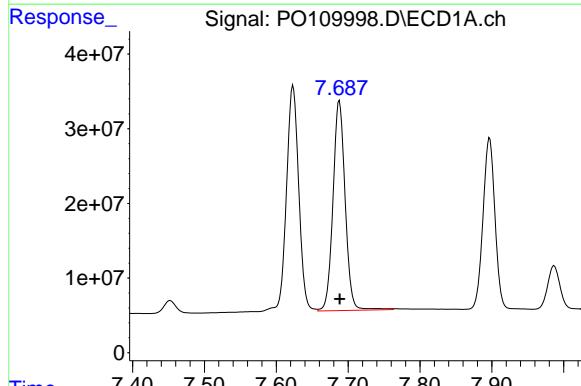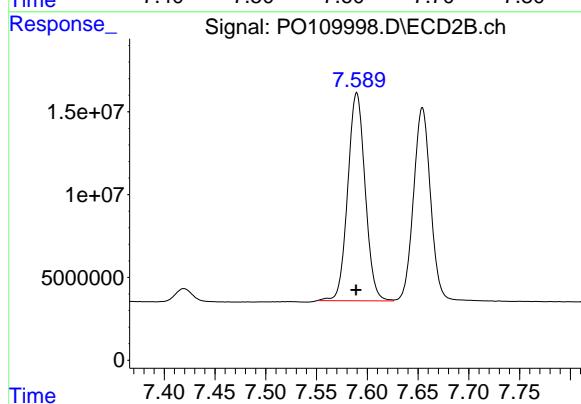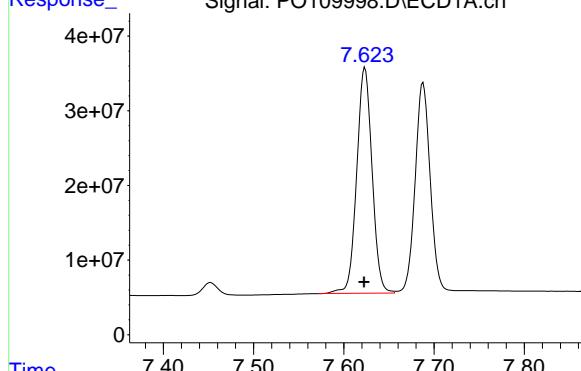

#41 AR-1268-1

R.T.: 7.590 min  
 Delta R.T.: 0.000 min  
 Response: 149647905  
 Conc: 258.81 ng/ml

#42 AR-1268-2

R.T.: 7.688 min  
 Delta R.T.: 0.000 min  
 Response: 330395950  
 Conc: 258.20 ng/ml

#42 AR-1268-2

R.T.: 7.654 min  
 Delta R.T.: 0.001 min  
 Response: 137184821  
 Conc: 257.56 ng/ml

#43 AR-1268-3

R.T.: 7.897 min  
 Delta R.T.: 0.000 min  
 Response: 264115362  
 Conc: 254.29 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#43 AR-1268-3





R.T.: 7.861 min  
 Delta R.T.: 0.000 min  
 Response: 106952452  
 Conc: 259.02 ng/ml

#44 AR-1268-4

R.T.: 8.184 min  
 Delta R.T.: 0.000 min  
 Response: 118334390  
 Conc: 264.47 ng/ml

#44 AR-1268-4

R.T.: 8.146 min  
 Delta R.T.: 0.000 min  
 Response: 42174671  
 Conc: 260.30 ng/ml

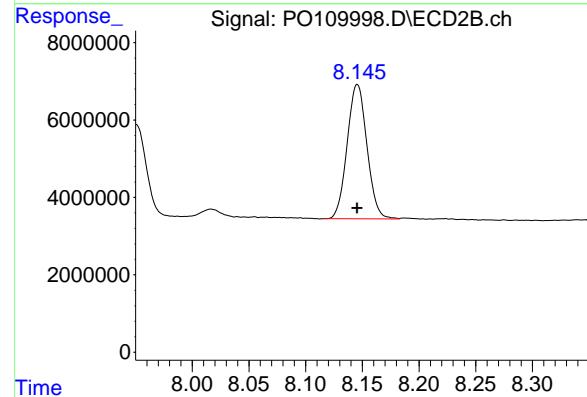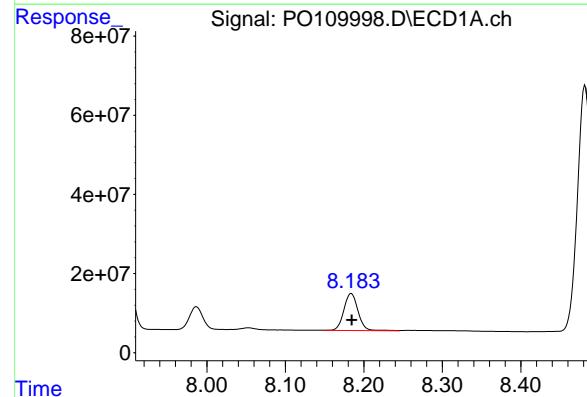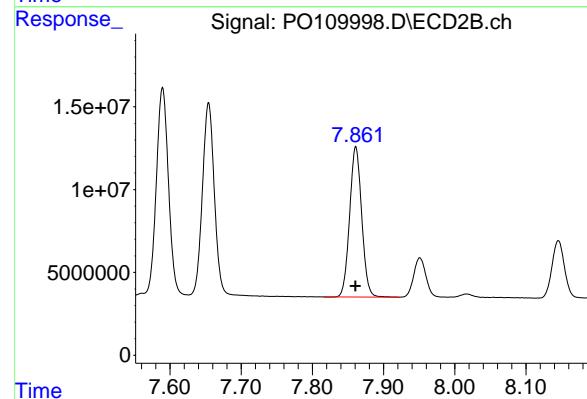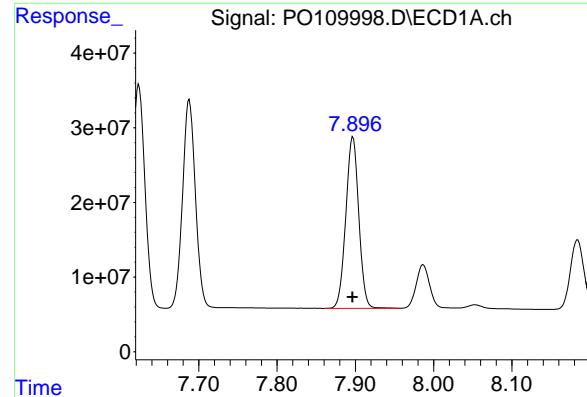


#45 AR-1268-5

R.T.: 8.482 min  
 Delta R.T.: 0.000 min  
 Response: 811940473  
 Conc: 251.48 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

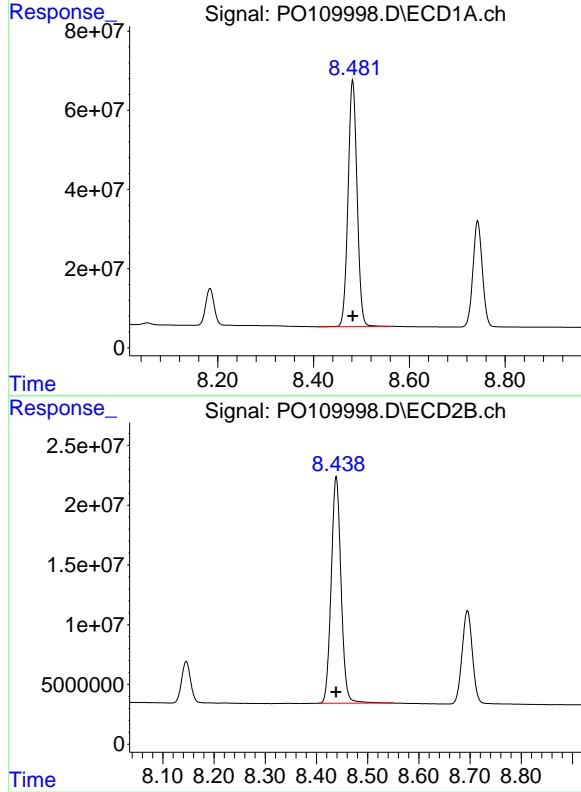

#45 AR-1268-5

R.T.: 8.439 min  
 Delta R.T.: 0.000 min  
 Response: 254015607  
 Conc: 257.32 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109999.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 22:15  
 Operator : YP/AJ  
 Sample : AR1268ICC050  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
AR1268ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:07:11 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	3.691	3.688	44374914	25645349	4.783m	4.855m
2) SA Decachlor...	8.743	8.695	72973489	22764198	5.168	5.493

**Target Compounds**

41) L9 AR-1268-1	7.622	7.590	71178847	31006348	50.721m	53.625
42) L9 AR-1268-2	7.688	7.654	63525178	28112917	49.643	52.781
43) L9 AR-1268-3	7.896	7.861	50172519	22018734	48.306	53.325
44) L9 AR-1268-4	8.183	8.146	21758650	8301200	48.629m	51.234
45) L9 AR-1268-5	8.481	8.438	151.8E6	51592382	47.022	52.264

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109999.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 22:15  
 Operator : YP/AJ  
 Sample : AR1268ICC050  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:07:11 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_O  
**ClientSampleId :**  
 AR1268ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

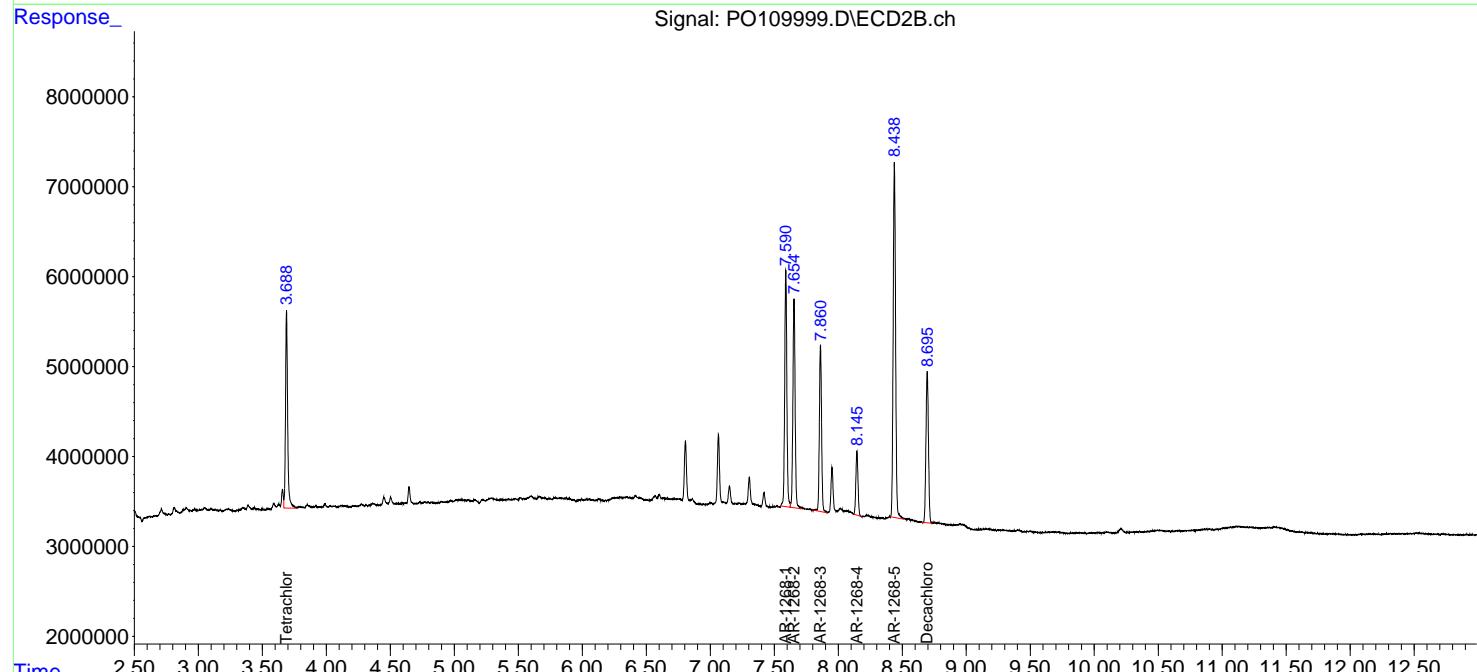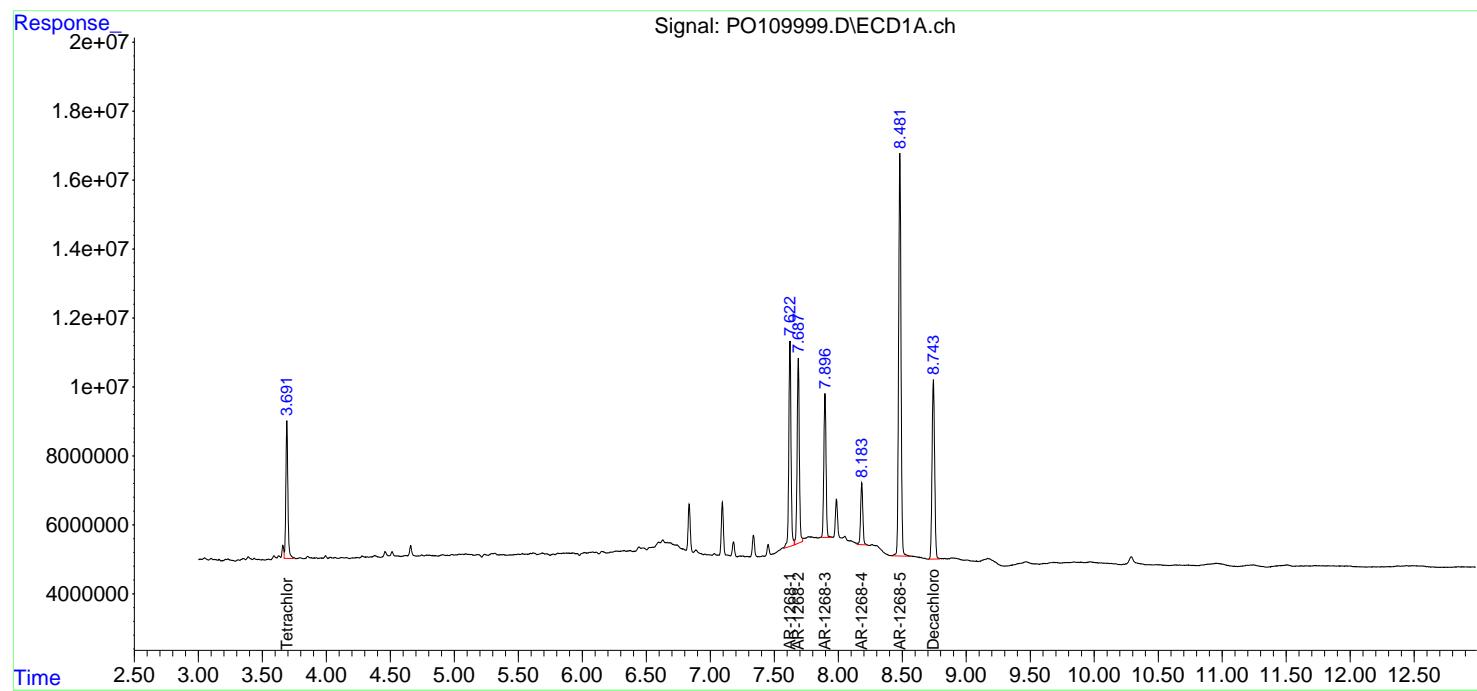

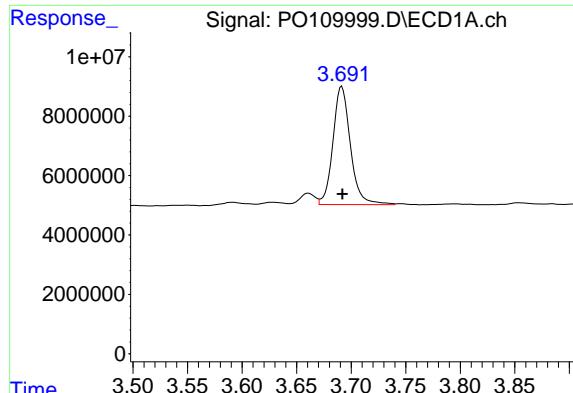


## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
Delta R.T.: -0.001 min  
Response: 44374914  
Conc: 4.78 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1268ICC050


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/19/2025  
Supervised By :mohammad ahmed 03/24/2025

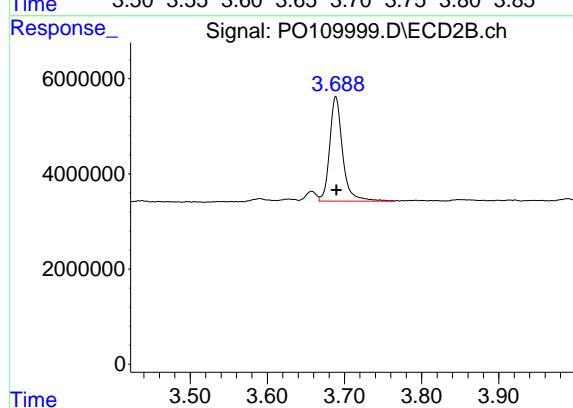


## #1 Tetrachloro-m-xylene

R.T.: 3.688 min  
Delta R.T.: -0.001 min  
Response: 25645349  
Conc: 4.86 ng/ml

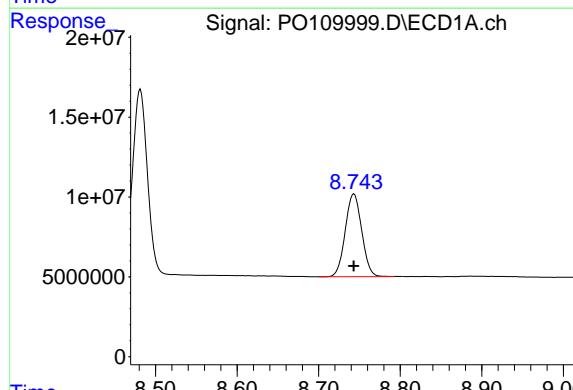

## #2 Decachlorobiphenyl

R.T.: 8.743 min  
Delta R.T.: 0.000 min  
Response: 72973489  
Conc: 5.17 ng/ml

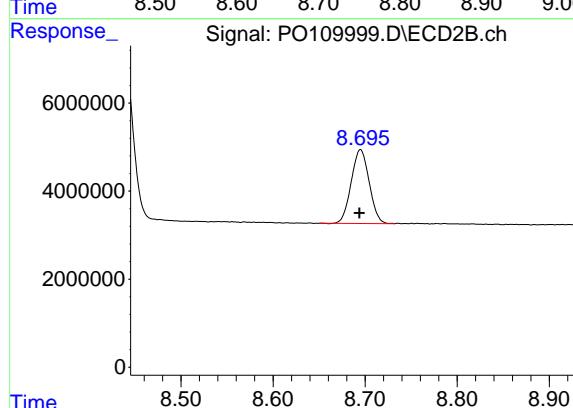

## #2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.001 min  
Response: 22764198  
Conc: 5.49 ng/ml





#41 AR-1268-1

R.T.: 7.622 min  
 Delta R.T.: 0.000 min  
 Response: 71178847  
 Conc: 50.72 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

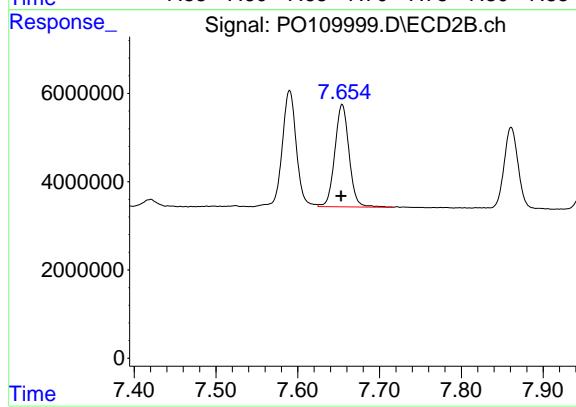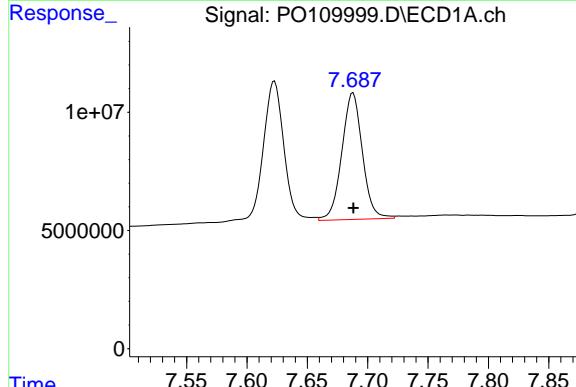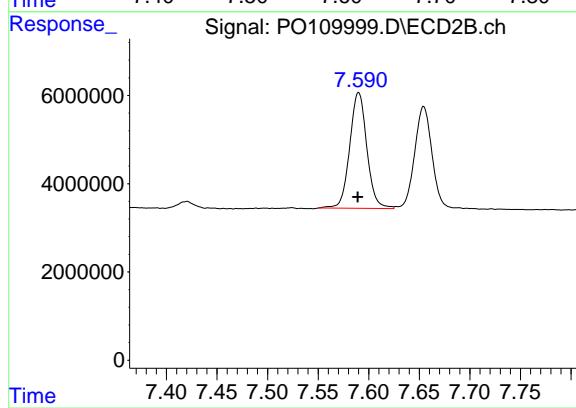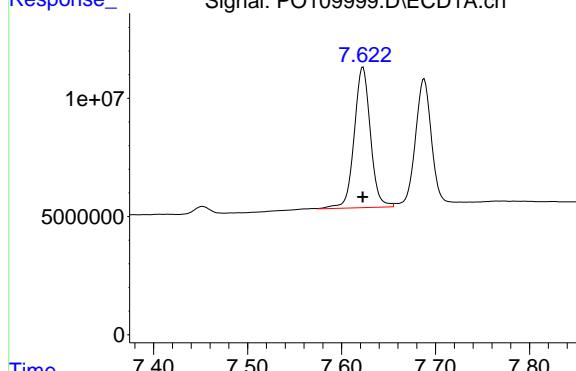

#41 AR-1268-1

R.T.: 7.590 min  
 Delta R.T.: 0.000 min  
 Response: 31006348  
 Conc: 53.63 ng/ml

#42 AR-1268-2

R.T.: 7.688 min  
 Delta R.T.: 0.000 min  
 Response: 63525178  
 Conc: 49.64 ng/ml

#42 AR-1268-2

R.T.: 7.654 min  
 Delta R.T.: 0.001 min  
 Response: 28112917  
 Conc: 52.78 ng/ml

#43 AR-1268-3

R.T.: 7.896 min  
 Delta R.T.: 0.000 min  
 Response: 50172519  
 Conc: 48.31 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

#43 AR-1268-3





R.T.: 7.861 min  
 Delta R.T.: 0.000 min  
 Response: 22018734  
 Conc: 53.32 ng/ml

#44 AR-1268-4

R.T.: 8.183 min  
 Delta R.T.: -0.001 min  
 Response: 21758650  
 Conc: 48.63 ng/ml

#44 AR-1268-4

R.T.: 8.146 min  
 Delta R.T.: 0.000 min  
 Response: 8301200  
 Conc: 51.23 ng/ml

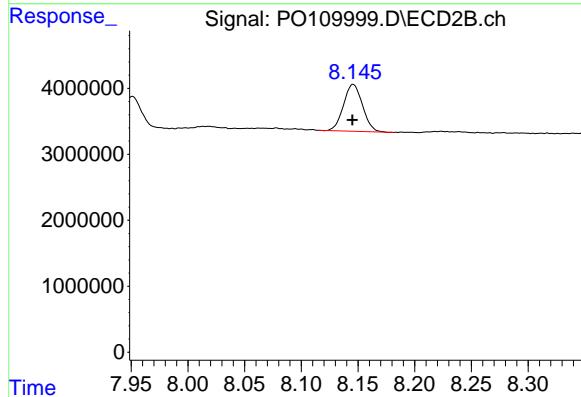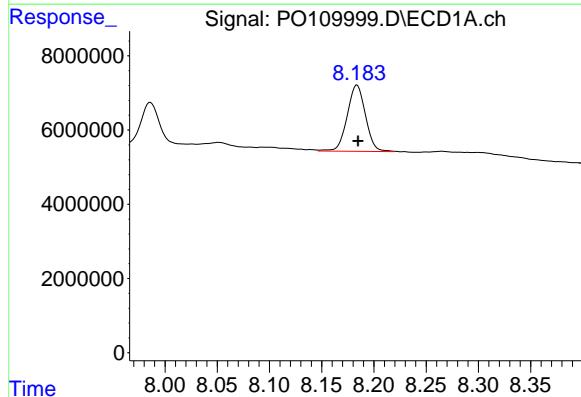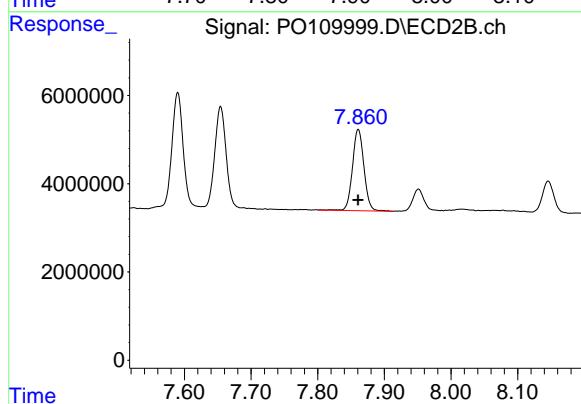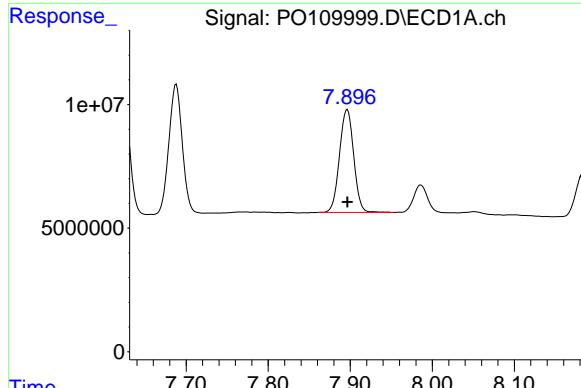



#45 AR-1268-5

R.T.: 8.481 min  
 Delta R.T.: 0.000 min  
 Response: 151815895  
 Conc: 47.02 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/19/2025  
 Supervised By :mohammad ahmed 03/24/2025

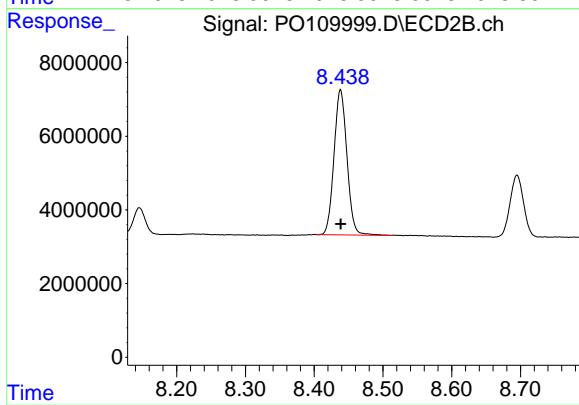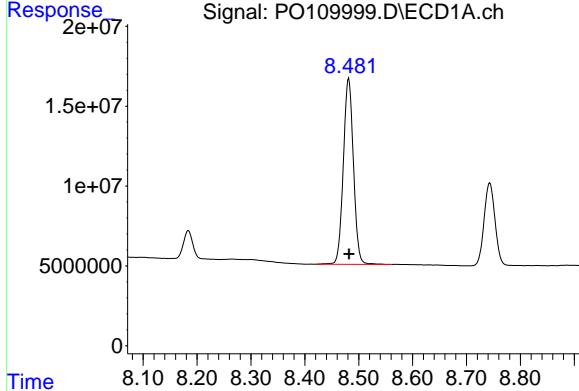

#45 AR-1268-5

R.T.: 8.438 min  
 Delta R.T.: 0.000 min  
 Response: 51592382  
 Conc: 52.26 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110000.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 22:34  
 Operator : YP/AJ  
 Sample : P0031925ICV500  
 Misc :  
 ALS Vial : 31 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
ICVPO031925

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:41:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:39:38 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	445.5E6	261.7E6	48.943	49.897
2) SA Decachlor...	8.744	8.696	386.1E6	117.6E6	50.211	48.467

Target Compounds

3) L1 AR-1016-1	4.784	4.771	165.3E6	89338991	491.286	487.512
4) L1 AR-1016-2	4.804	4.790	229.3E6	128.0E6	494.517	489.369
5) L1 AR-1016-3	4.860	4.966	158.0E6	69159098	492.753	487.796
6) L1 AR-1016-4	4.981	5.008	124.5E6	57510192	492.750	487.665
7) L1 AR-1016-5	5.238	5.221	133.3E6	74393726	484.896	486.492
31) L7 AR-1260-1	6.280	6.253	235.0E6	125.1E6	498.624	489.686
32) L7 AR-1260-2	6.469	6.441	287.0E6	145.2E6	481.955	483.545
33) L7 AR-1260-3	6.837	6.594	243.8E6	137.4E6	502.299	475.363
34) L7 AR-1260-4	7.097	7.065	212.4E6	103.8E6	500.751	482.426
35) L7 AR-1260-5	7.339	7.306	531.0E6	241.3E6	507.683	483.788



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110000.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 22:34  
 Operator : YP/AJ  
 Sample : P0031925ICV500  
 Misc :  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 ICPPO031925

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:41:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:39:38 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

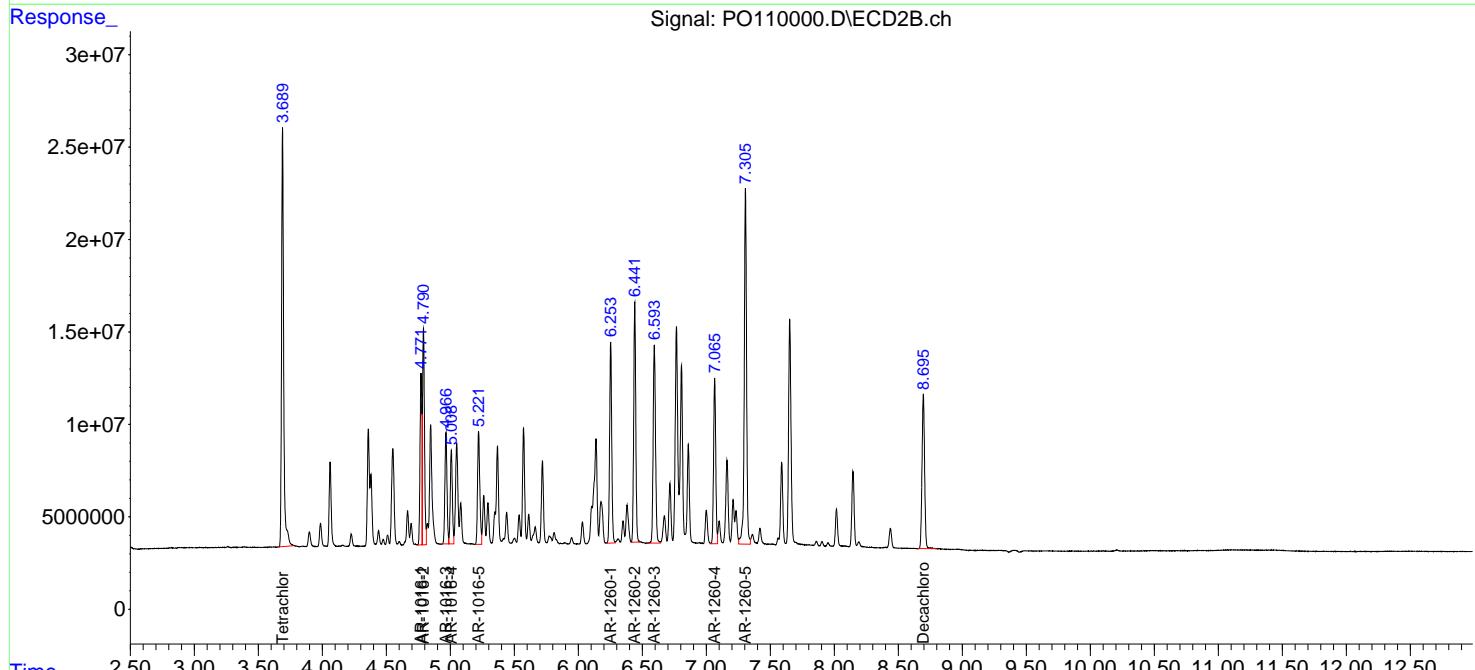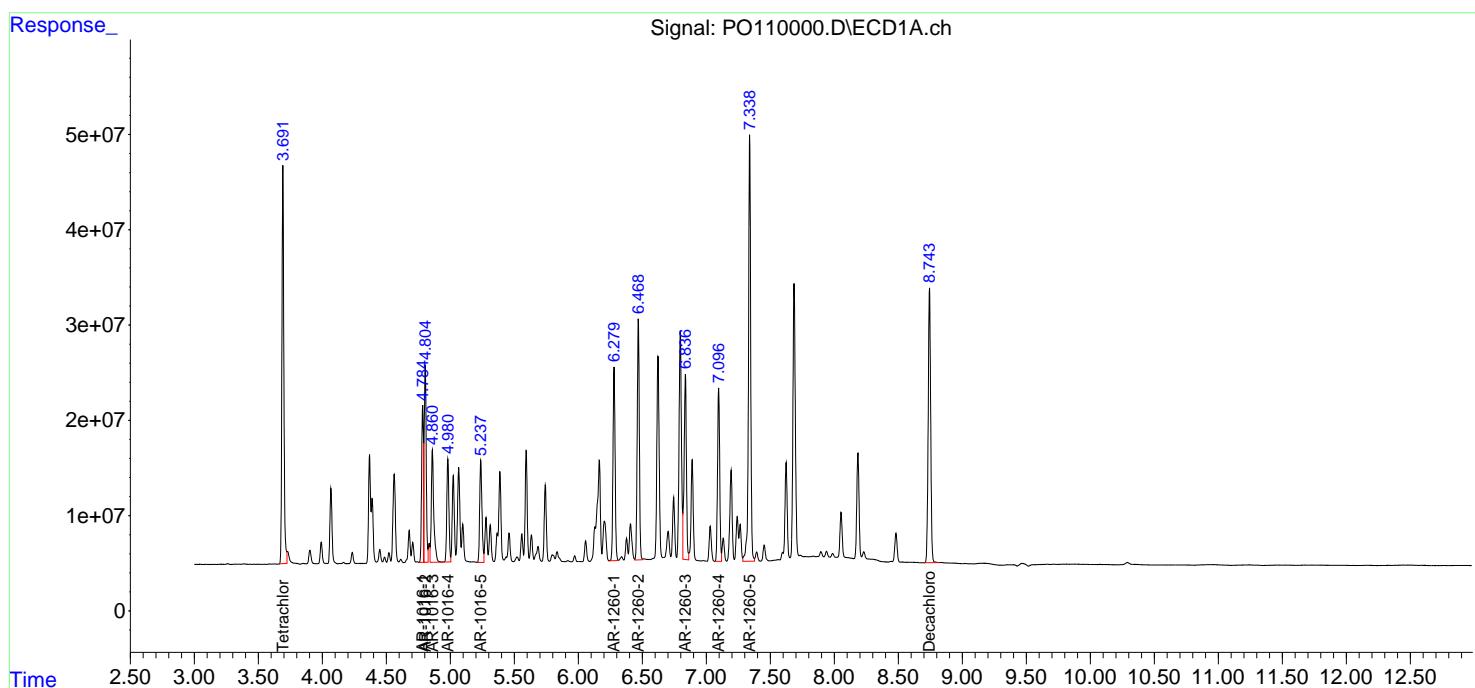

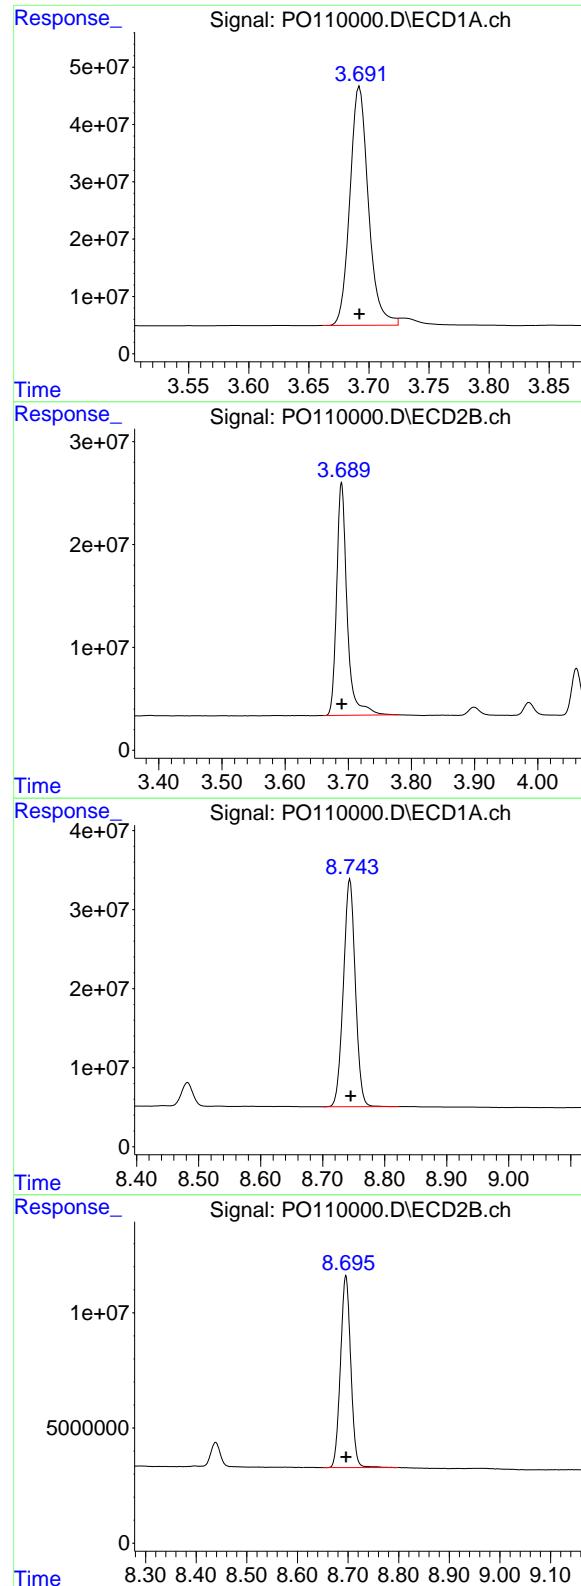

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 445455679  
Conc: 48.94 ng/ml

**Instrument:**

ECD\_O

**ClientSampleId :**

ICVPO031925

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 261663576  
Conc: 49.90 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: -0.001 min  
Response: 386058371  
Conc: 50.21 ng/ml


## #2 Decachlorobiphenyl

R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 117585250  
Conc: 48.47 ng/ml

#3 AR-1016-1


R.T.: 4.784 min  
 Delta R.T.: 0.000 min  
 Response: 165339415  
 Conc: 491.29 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925

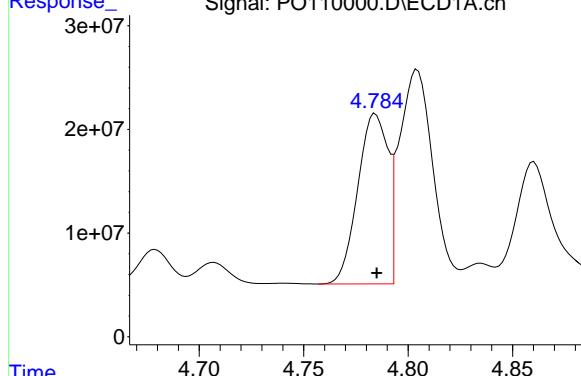


#3 AR-1016-1

R.T.: 4.771 min  
 Delta R.T.: 0.000 min  
 Response: 89338991  
 Conc: 487.51 ng/ml

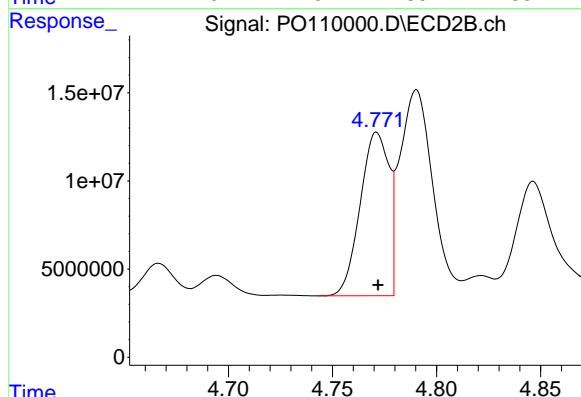


#4 AR-1016-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 229300386  
 Conc: 494.52 ng/ml

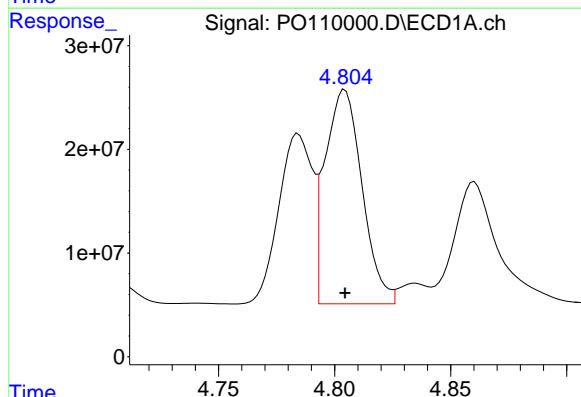


#4 AR-1016-2

R.T.: 4.790 min  
 Delta R.T.: 0.000 min  
 Response: 127972100  
 Conc: 489.37 ng/ml

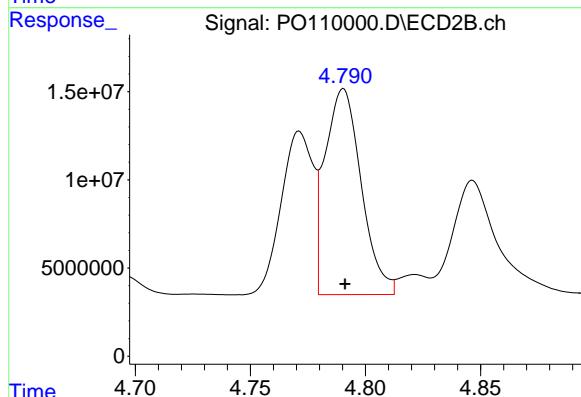


#5 AR-1016-3

R.T.: 4.860 min  
 Delta R.T.: 0.000 min  
**Instrument:**  
 Response: 157969845 ECD\_O  
 Conc: 492.75 ng/ml ClientSampleId :  
 ICVPO031925

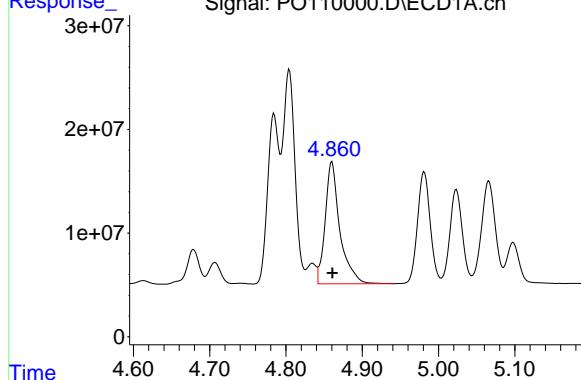


#5 AR-1016-3

R.T.: 4.966 min  
 Delta R.T.: 0.000 min  
 Response: 69159098  
 Conc: 487.80 ng/ml

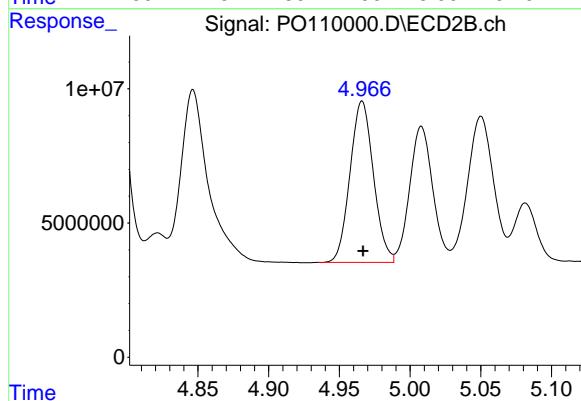


#6 AR-1016-4


R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 124512743  
 Conc: 492.75 ng/ml

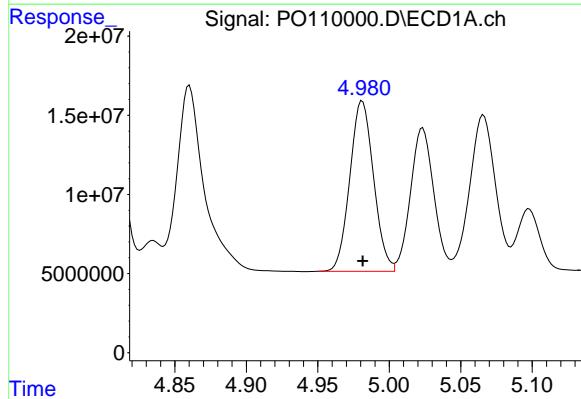

#6 AR-1016-4

R.T.: 5.008 min  
 Delta R.T.: 0.000 min  
 Response: 57510192  
 Conc: 487.66 ng/ml

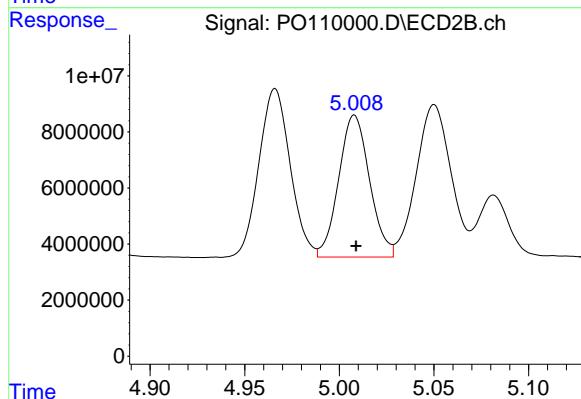

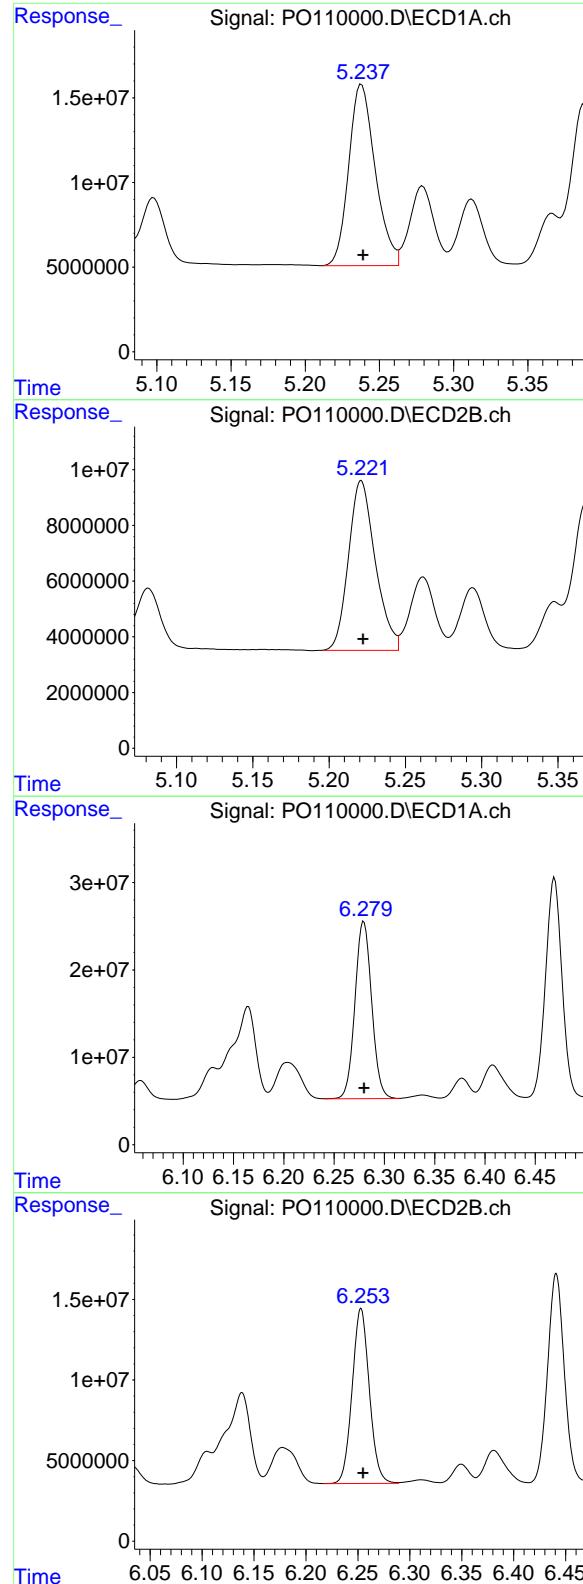

#7 AR-1016-5

R.T.: 5.238 min  
 Delta R.T.: -0.001 min  
 Response: 133281979  
 Conc: 484.90 ng/ml

Instrument: ECD\_O  
 ClientSampleId: ICVPO031925

#7 AR-1016-5

R.T.: 5.221 min  
 Delta R.T.: -0.001 min  
 Response: 74393726  
 Conc: 486.49 ng/ml

#31 AR-1260-1

R.T.: 6.280 min  
 Delta R.T.: 0.000 min  
 Response: 235026886  
 Conc: 498.62 ng/ml





#31 AR-1260-1

R.T.: 6.253 min  
 Delta R.T.: -0.002 min  
 Response: 125086324  
 Conc: 489.69 ng/ml

#32 AR-1260-2

R.T.: 6.469 min  
 Delta R.T.: 0.000 min  
 Response: 287013411  
 Conc: 481.95 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925

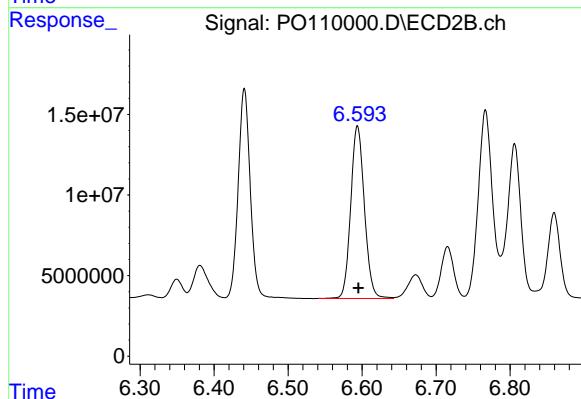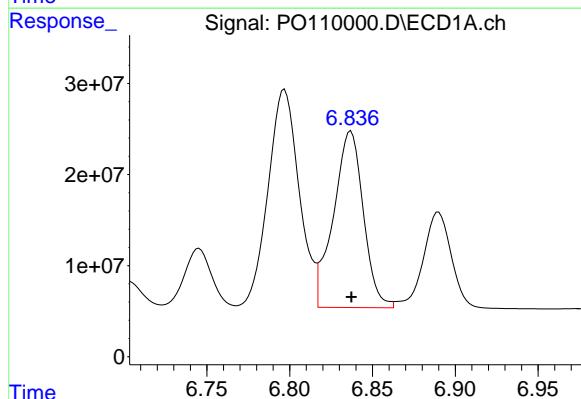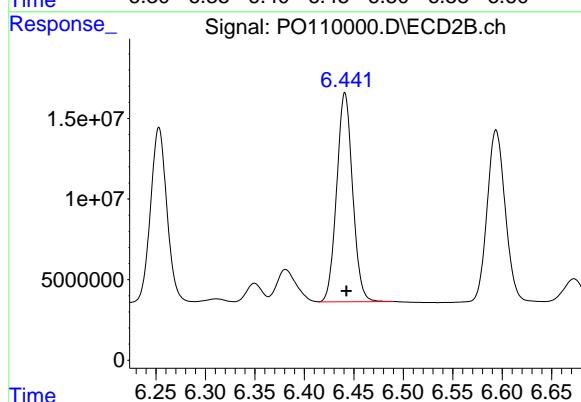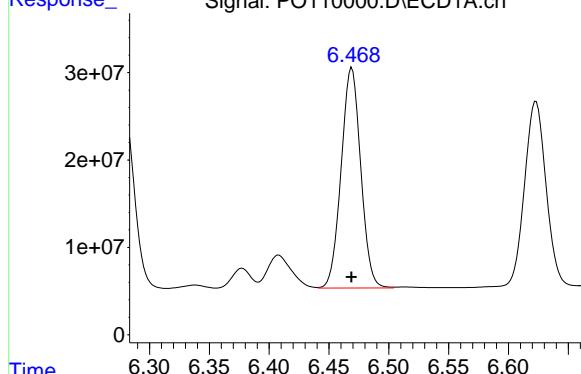

#32 AR-1260-2

R.T.: 6.441 min  
 Delta R.T.: -0.001 min  
 Response: 145201446  
 Conc: 483.54 ng/ml

#33 AR-1260-3

R.T.: 6.837 min  
 Delta R.T.: 0.000 min  
 Response: 243766592  
 Conc: 502.30 ng/ml


#33 AR-1260-3

R.T.: 6.594 min  
 Delta R.T.: -0.001 min  
 Response: 137371501  
 Conc: 475.36 ng/ml

#34 AR-1260-4


R.T.: 7.097 min  
 Delta R.T.: 0.000 min  
 Response: 212402639  
 Conc: 500.75 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925

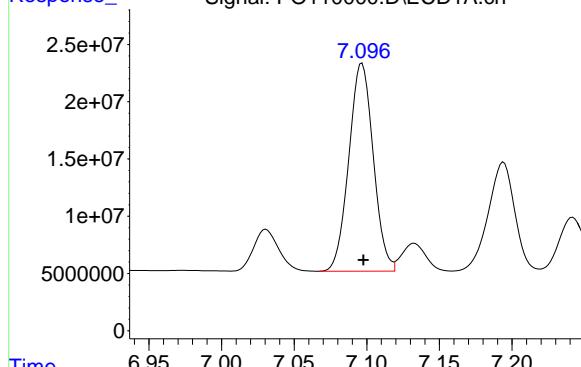


#34 AR-1260-4

R.T.: 7.065 min  
 Delta R.T.: -0.001 min  
 Response: 103759489  
 Conc: 482.43 ng/ml

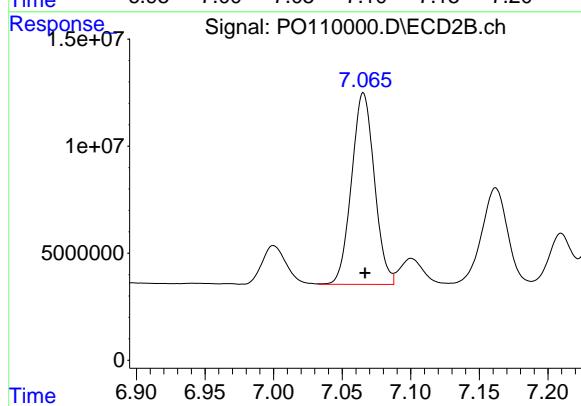


#35 AR-1260-5

R.T.: 7.339 min  
 Delta R.T.: 0.000 min  
 Response: 530958243  
 Conc: 507.68 ng/ml

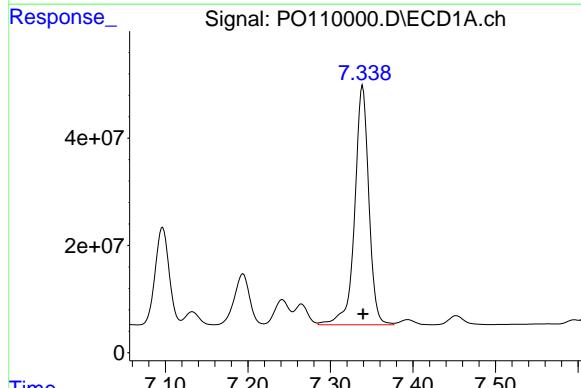

#35 AR-1260-5

R.T.: 7.306 min  
 Delta R.T.: -0.001 min  
 Response: 241263068  
 Conc: 483.79 ng/ml

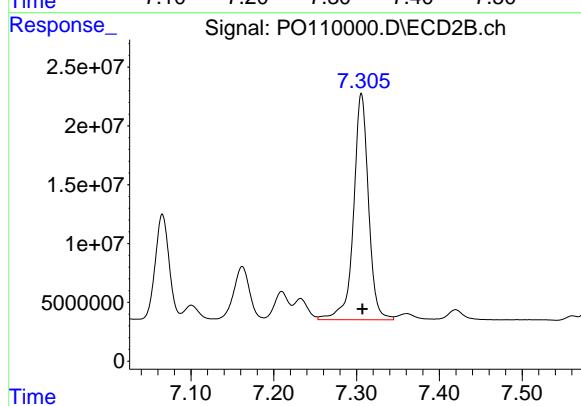

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110001.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 23:47  
 Operator : YP/AJ  
 Sample : AR1242ICV500  
 Misc :  
 ALS Vial : 32 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**ICVPO031925AR1242**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:45:06 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:43:41 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	445.5E6	254.1E6	52.578	52.663
2) SA Decachlor...	8.744	8.695	378.1E6	113.8E6	52.496	50.899

Target Compounds

16) L4 AR-1242-1	4.785	4.771	138.5E6	75308322	517.896	515.050
17) L4 AR-1242-2	4.804	4.791	190.3E6	107.0E6	516.964	514.473
18) L4 AR-1242-3	4.861	4.966	132.7E6	58059678	514.485	520.188
19) L4 AR-1242-4	4.981	5.050	104.1E6	58816332	520.236	507.140
20) L4 AR-1242-5	5.634	5.572	109.1E6	71078329	516.760	517.905



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110001.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 23:47  
 Operator : YP/AJ  
 Sample : AR1242ICV500  
 Misc :  
 ALS Vial : 32 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**ICVPO031925AR1242**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:45:06 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:43:41 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

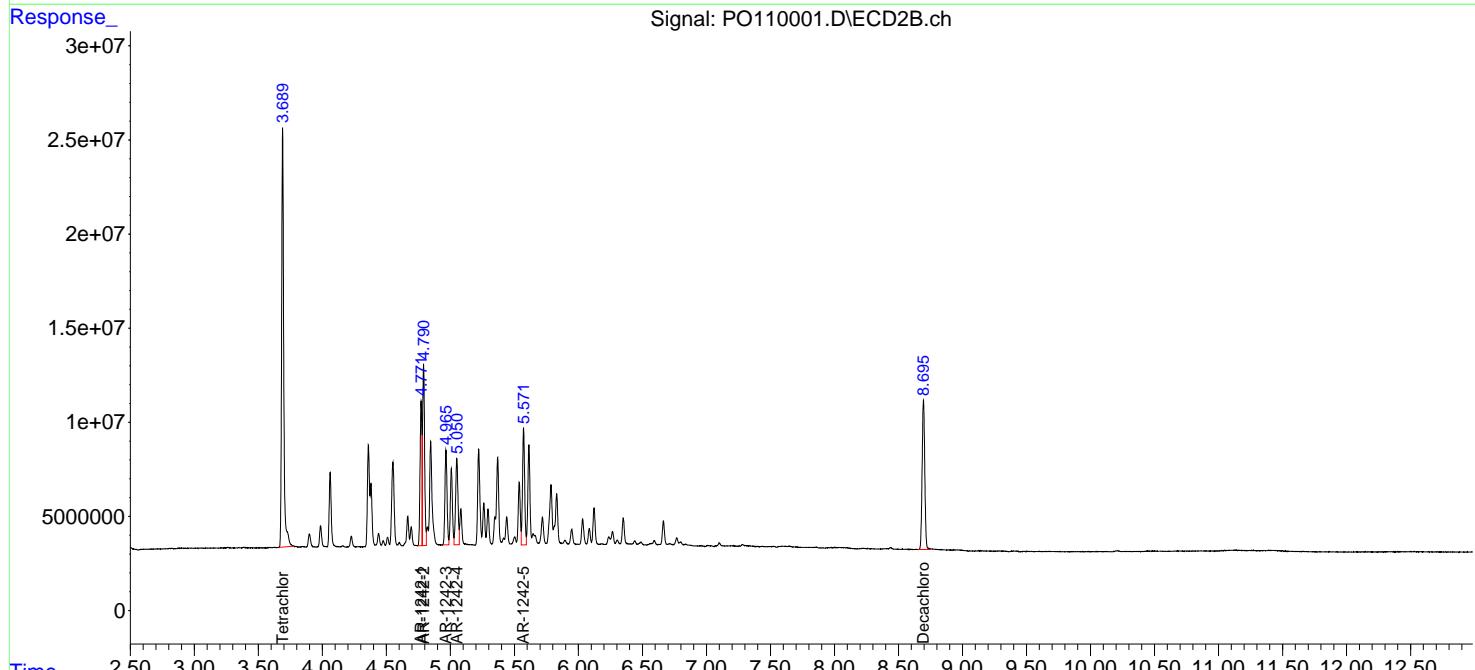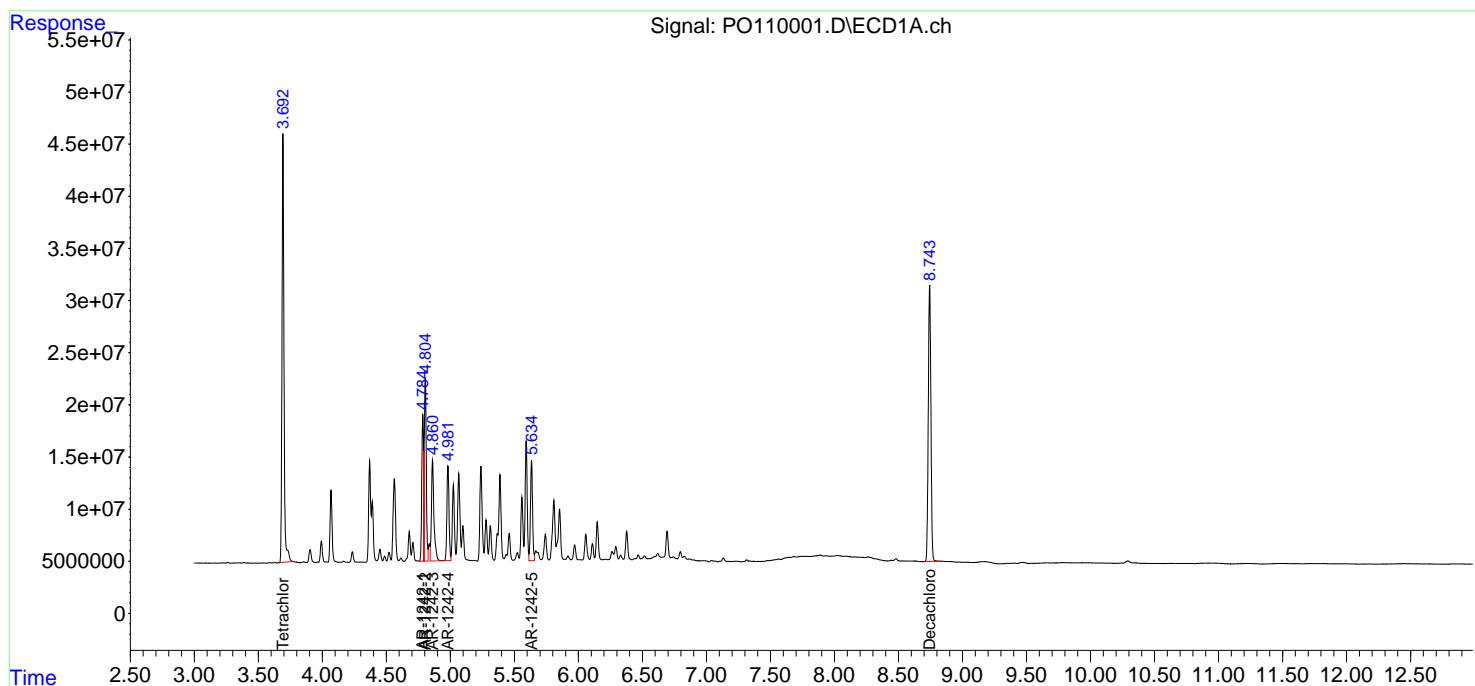

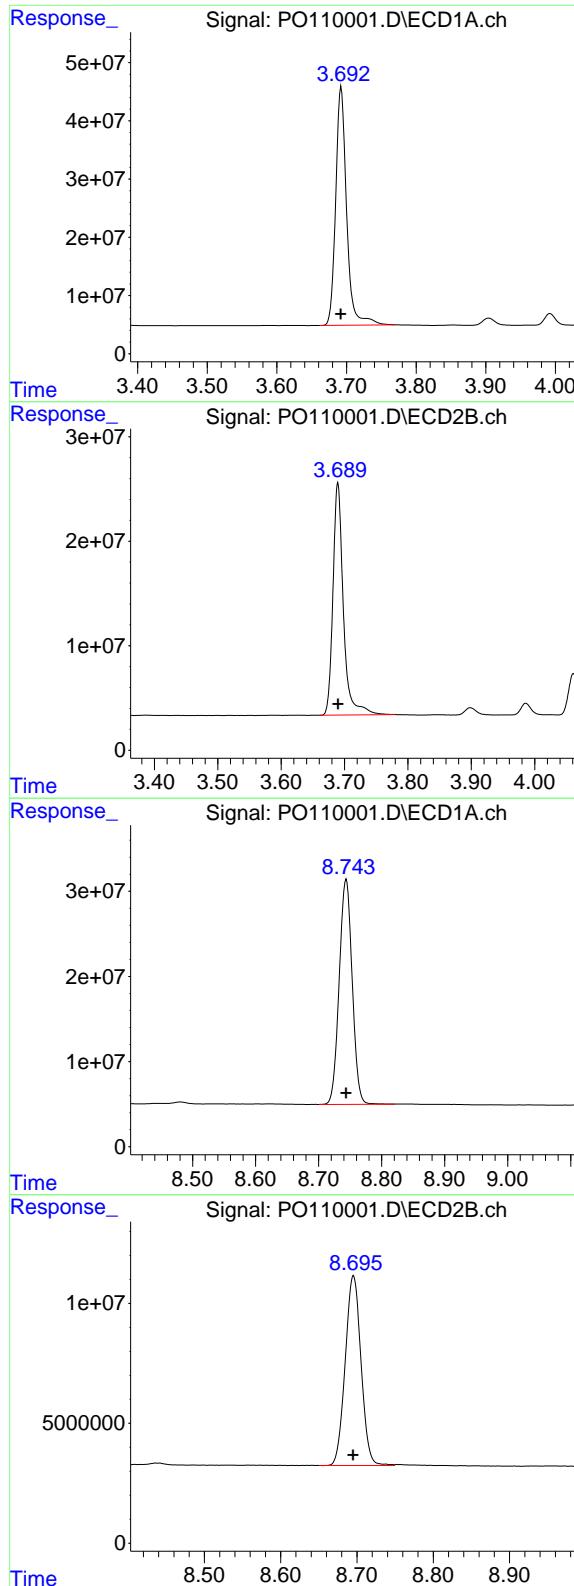

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 445457667  
Conc: 52.58 ng/ml

Instrument: ECD\_O  
ClientSampleId: ICVPO031925AR1242

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 254125961  
Conc: 52.66 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 378060054  
Conc: 52.50 ng/ml


## #2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 113786439  
Conc: 50.90 ng/ml

#16 AR-1242-1


R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 138489149  
 Conc: 517.90 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1242




#16 AR-1242-1

R.T.: 4.771 min  
 Delta R.T.: 0.000 min  
 Response: 75308322  
 Conc: 515.05 ng/ml

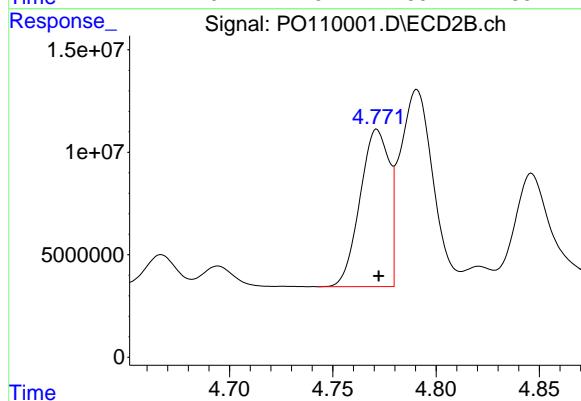


#17 AR-1242-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 190347656  
 Conc: 516.96 ng/ml

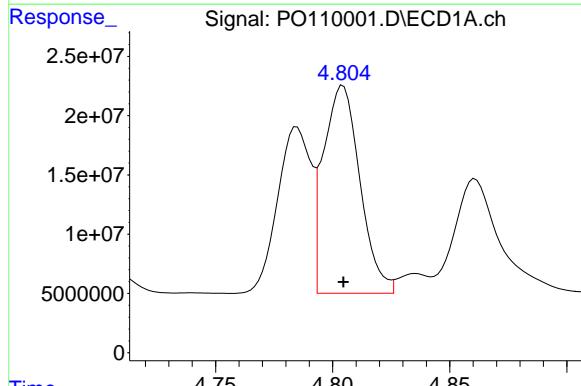

#17 AR-1242-2





R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 107028573  
 Conc: 514.47 ng/ml

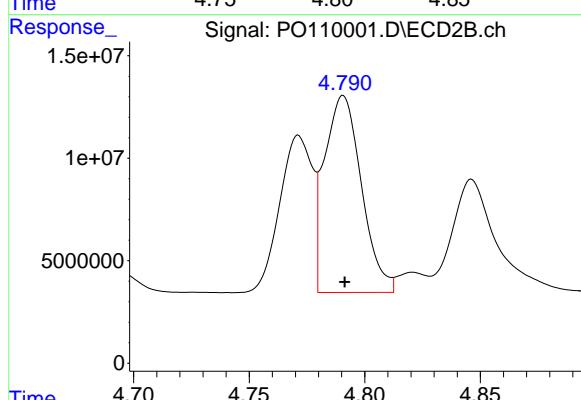

#18 AR-1242-3

R.T.: 4.861 min  
 Delta R.T.: 0.000 min  
 Response: 132711818  
 Conc: 514.48 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1242

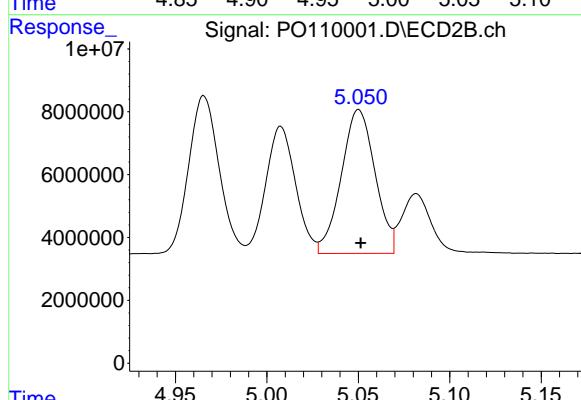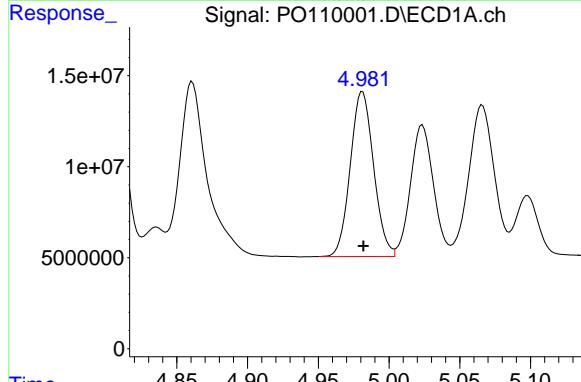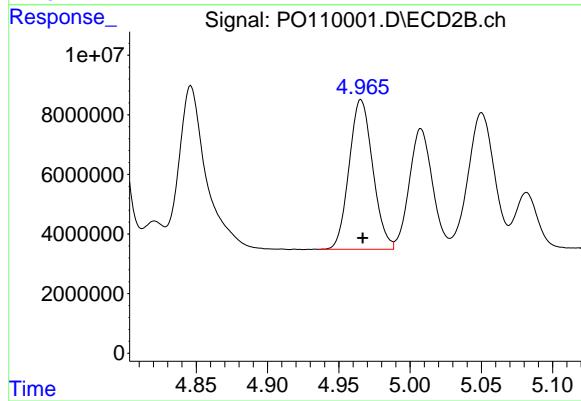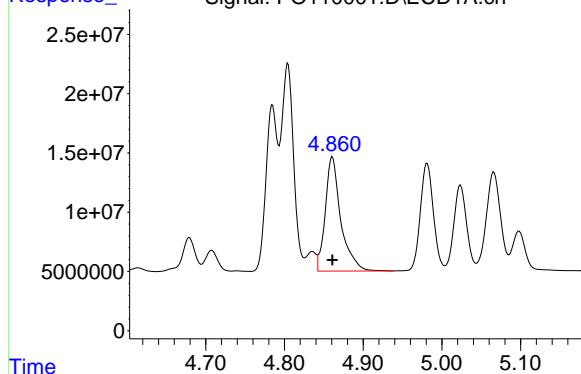

#18 AR-1242-3

R.T.: 4.966 min  
 Delta R.T.: -0.001 min  
 Response: 58059678  
 Conc: 520.19 ng/ml

#19 AR-1242-4

R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 104096142  
 Conc: 520.24 ng/ml



#19 AR-1242-4

R.T.: 5.050 min  
 Delta R.T.: -0.001 min  
 Response: 58816332  
 Conc: 507.14 ng/ml

#20 AR-1242-5

R.T.: 5.634 min  
Delta R.T.: 0.000 min  
Response: 109065446  
Conc: 516.76 ng/ml

Instrument: ECD\_O  
ClientSampleId: ICVPO031925AR1242

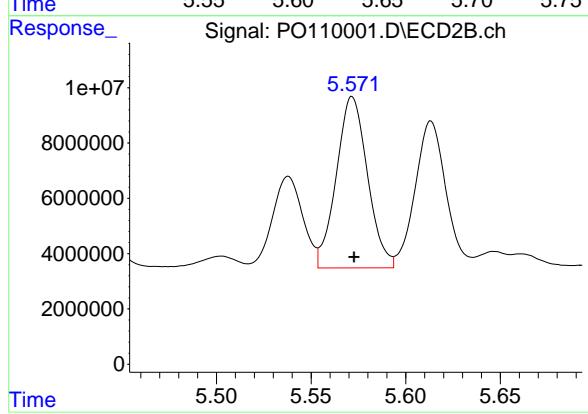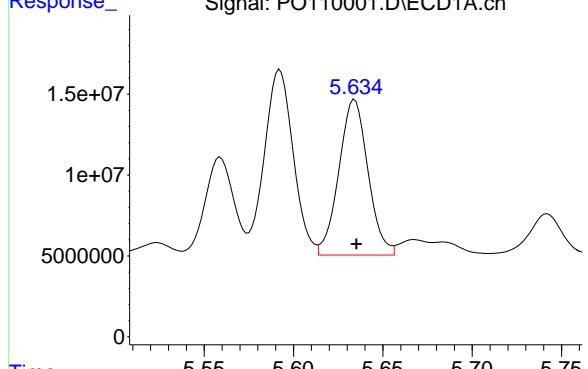

#20 AR-1242-5

R.T.: 5.572 min  
Delta R.T.: 0.000 min  
Response: 71078329  
Conc: 517.90 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110002.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Mar 2025 00:05  
 Operator : YP/AJ  
 Sample : AR1248ICV500  
 Misc :  
 ALS Vial : 33 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**ICVPO031925AR1248**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:41:11 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	453.1E6	257.7E6	48.851	48.659
2) SA Decachlor...	8.743	8.695	387.8E6	116.2E6	49.748	49.559

Target Compounds

21) L5 AR-1248-1	4.784	4.771	108.4E6	58618795	492.939	487.181
22) L5 AR-1248-2	5.023	5.008	147.5E6	82104463	489.895	487.213
23) L5 AR-1248-3	5.238	5.050	184.5E6	87652547	492.701	489.391
24) L5 AR-1248-4	5.592	5.221	258.0E6	102.0E6	493.069	489.250
25) L5 AR-1248-5	5.634	5.613	182.7E6	99745645	494.045	489.737



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110002.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Mar 2025 00:05  
 Operator : YP/AJ  
 Sample : AR12481CV500  
 Misc :  
 ALS Vial : 33 Sample Multiplier: 1


**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**ICVPO031925AR1248**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:41:11 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

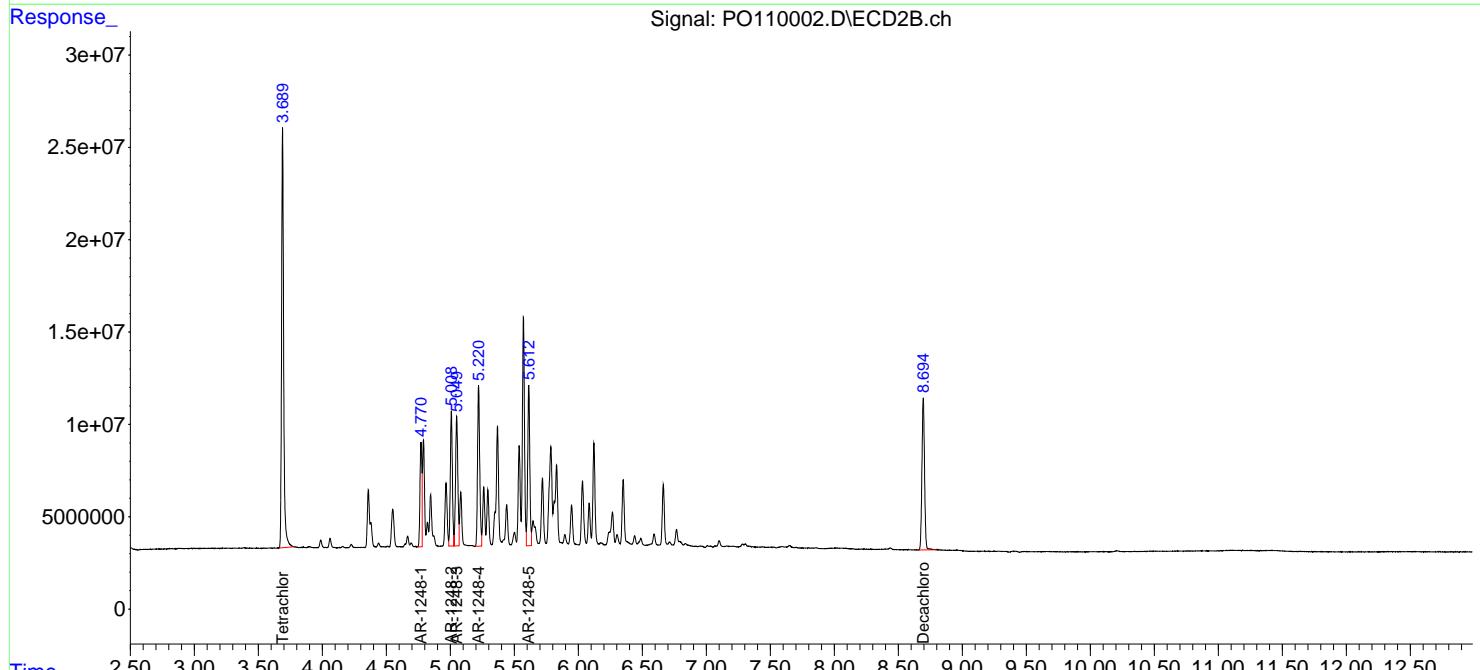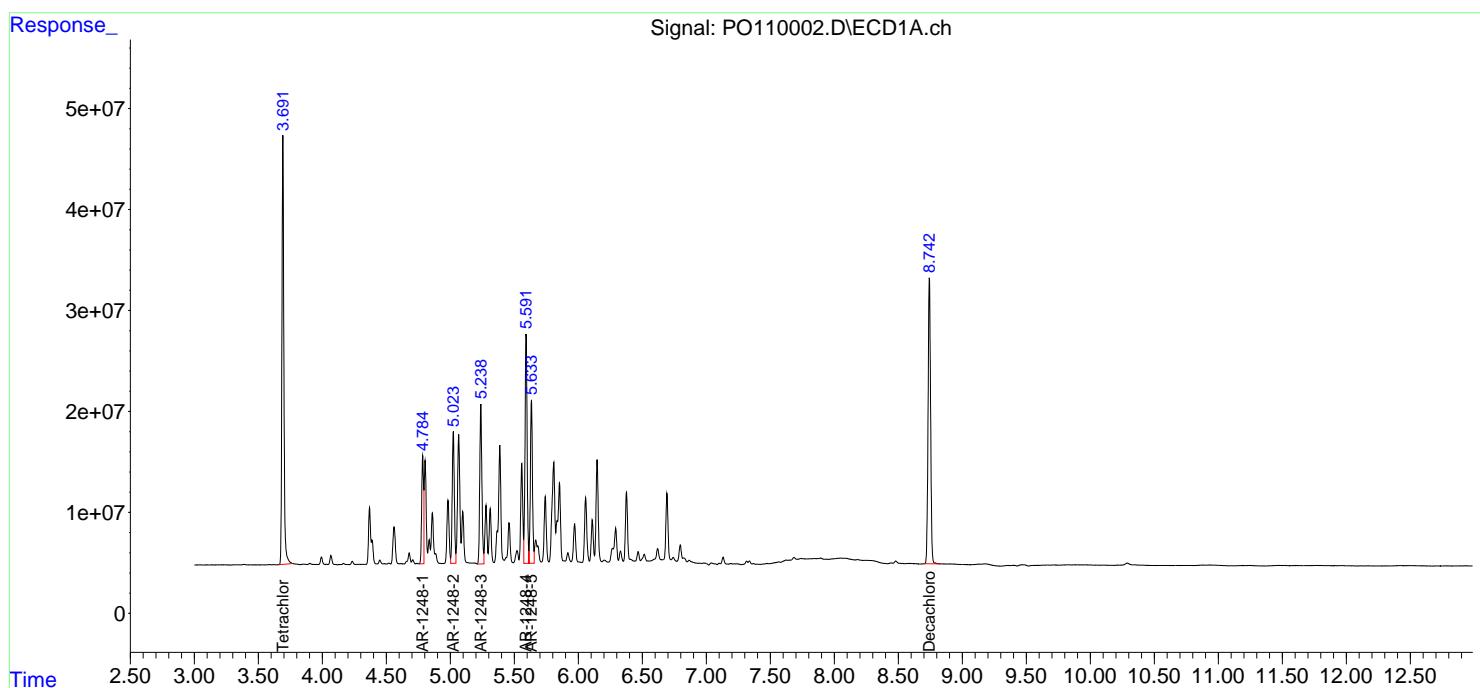

## #1 Tetrachloro-m-xylene

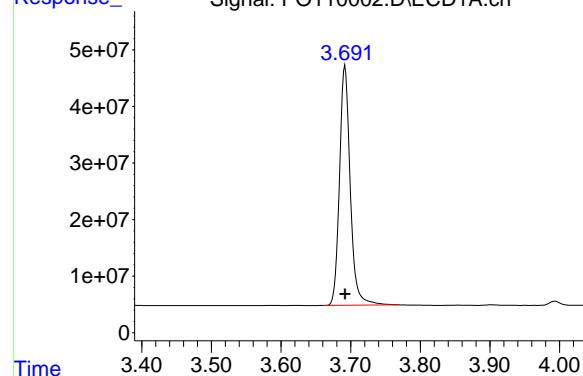

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 453137446  
Conc: 48.85 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1248

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 257654315  
Conc: 48.66 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.743 min  
Delta R.T.: -0.001 min  
Response: 387771183  
Conc: 49.75 ng/ml

## #2 Decachlorobiphenyl





R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 116199328  
Conc: 49.56 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

#21 AR-1248-1

R.T.: 4.784 min  
 Delta R.T.: 0.000 min  
 Response: 108417858  
 Conc: 492.94 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1248

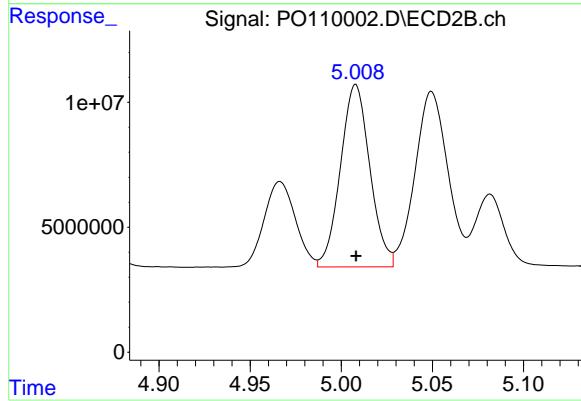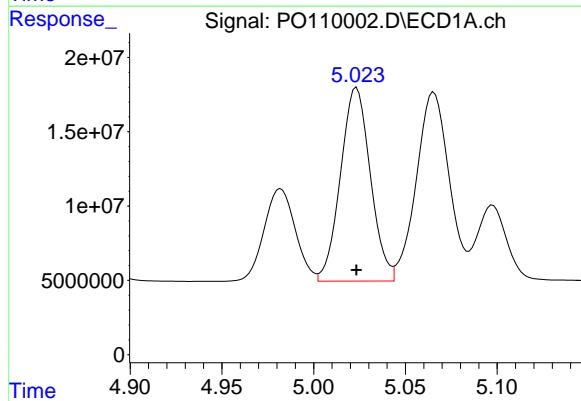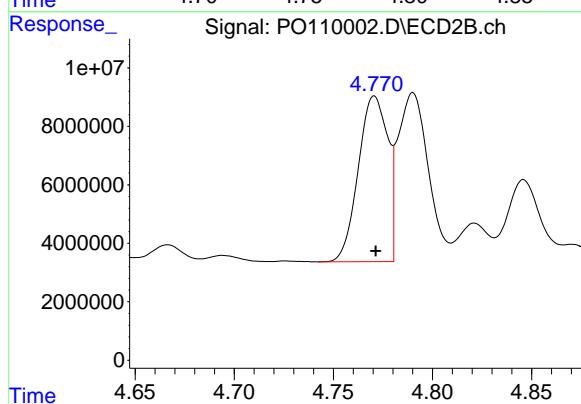

#21 AR-1248-1

R.T.: 4.771 min  
 Delta R.T.: 0.000 min  
 Response: 58618795  
 Conc: 487.18 ng/ml

#22 AR-1248-2

R.T.: 5.023 min  
 Delta R.T.: 0.000 min  
 Response: 147491637  
 Conc: 489.90 ng/ml


#22 AR-1248-2

R.T.: 5.008 min  
 Delta R.T.: 0.000 min  
 Response: 82104463  
 Conc: 487.21 ng/ml

#23 AR-1248-3


R.T.: 5.238 min  
 Delta R.T.: 0.000 min  
 Response: 184471566  
 Conc: 492.70 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1248

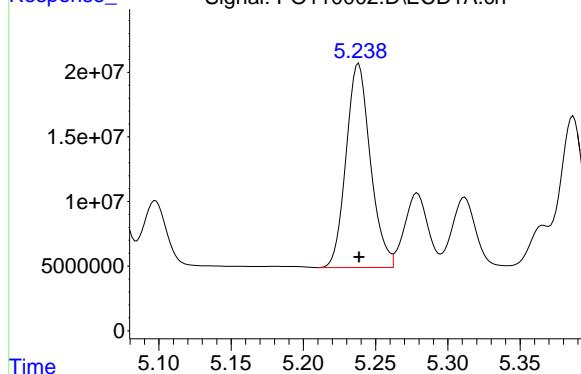


#23 AR-1248-3

R.T.: 5.050 min  
 Delta R.T.: 0.000 min  
 Response: 87652547  
 Conc: 489.39 ng/ml

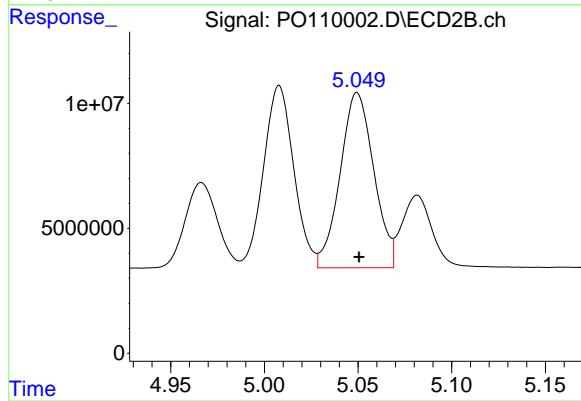


#24 AR-1248-4

R.T.: 5.592 min  
 Delta R.T.: 0.000 min  
 Response: 258010469  
 Conc: 493.07 ng/ml

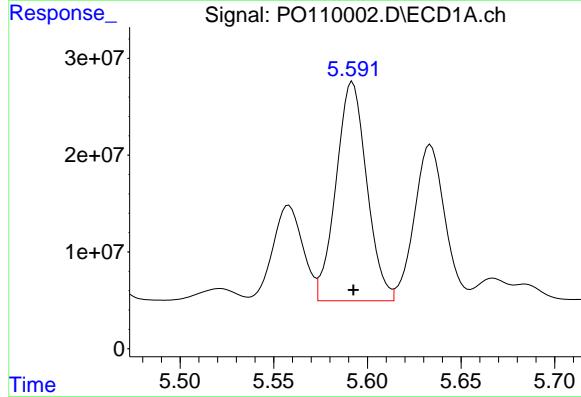

#24 AR-1248-4



R.T.: 5.221 min  
 Delta R.T.: 0.000 min  
 Response: 102041710  
 Conc: 489.25 ng/ml

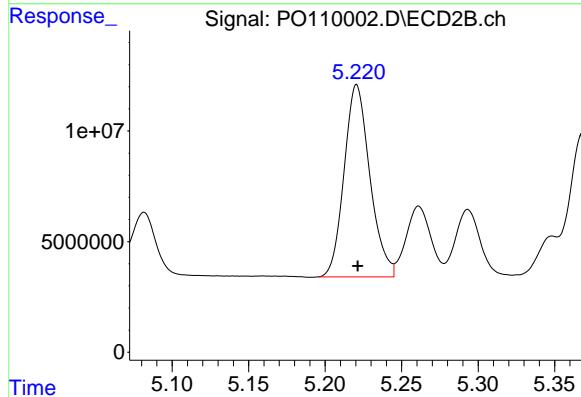

#25 AR-1248-5

R.T.: 5.634 min  
Delta R.T.: 0.000 min  
Response: 182660838  
Conc: 494.04 ng/ml

Instrument: ECD\_O  
ClientSampleId: ICVPO031925AR1248

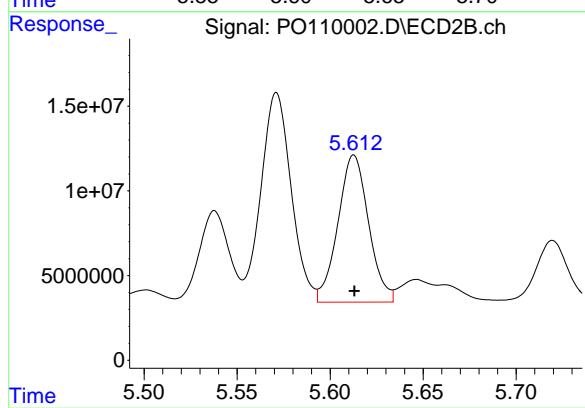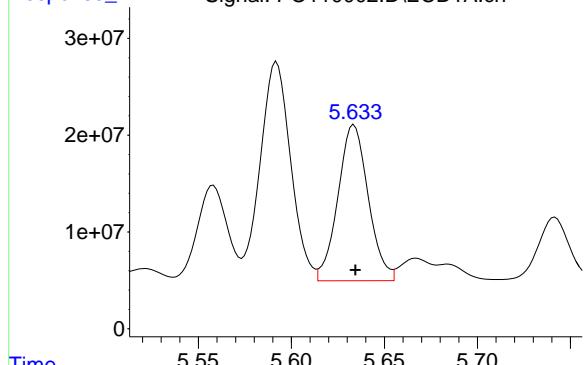

#25 AR-1248-5

R.T.: 5.613 min  
Delta R.T.: 0.000 min  
Response: 99745645  
Conc: 489.74 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110003.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Mar 2025 00:24  
 Operator : YP/AJ  
 Sample : AR1254ICV500  
 Misc :  
 ALS Vial : 34 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**ICVPO031925AR1254**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:50:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	450.3E6	255.9E6	47.966	47.857
2) SA Decachlor...	8.743	8.695	386.1E6	115.4E6	49.078	47.699

Target Compounds

26) L6 AR-1254-1	5.593	5.572	270.9E6	148.9E6	484.350	483.813
27) L6 AR-1254-2	5.743	5.720	234.3E6	129.7E6	484.326	483.086
28) L6 AR-1254-3	6.148	6.123	381.8E6	203.6E6	483.781	483.489
29) L6 AR-1254-4	6.377	6.350	236.7E6	117.7E6	486.513	481.783
30) L6 AR-1254-5	6.797	6.768	332.2E6	169.1E6	488.082	485.104



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110003.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Mar 2025 00:24  
 Operator : YP/AJ  
 Sample : AR1254ICV500  
 Misc :  
 ALS Vial : 34 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**ICVPO031925AR1254**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:50:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

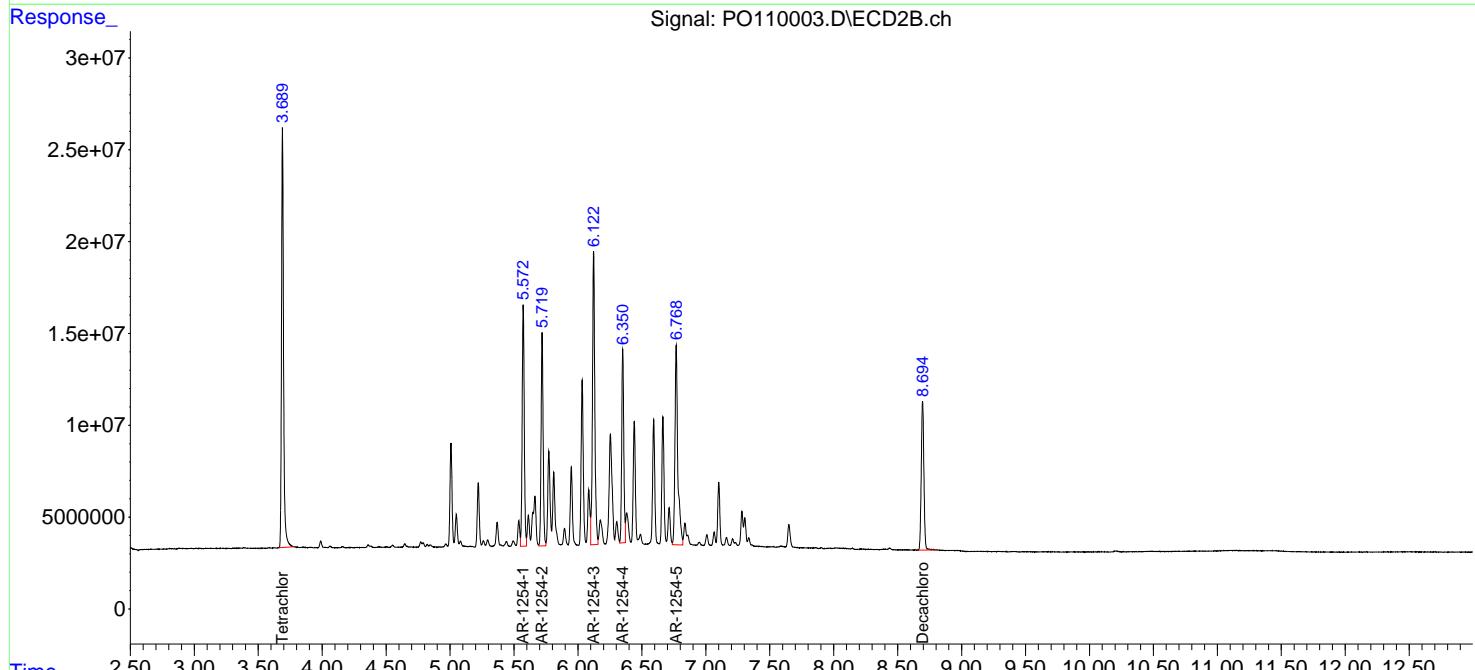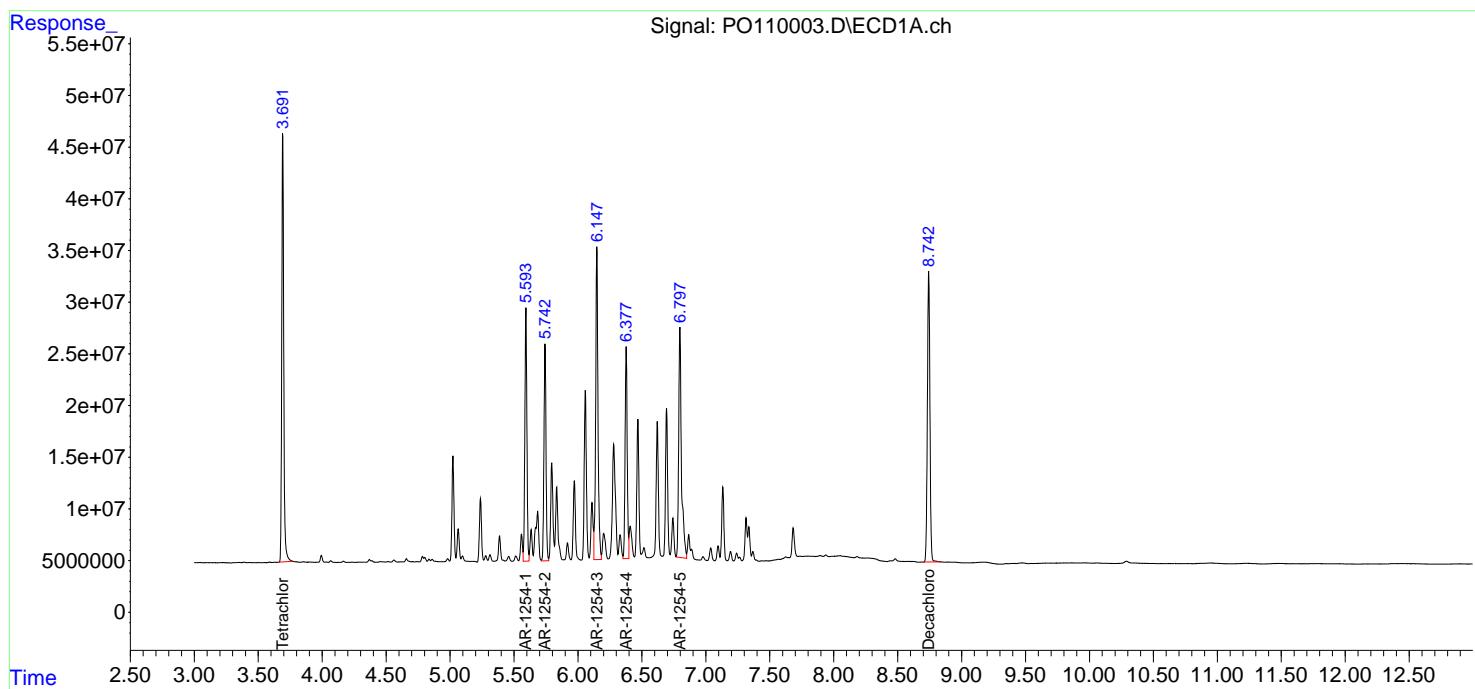

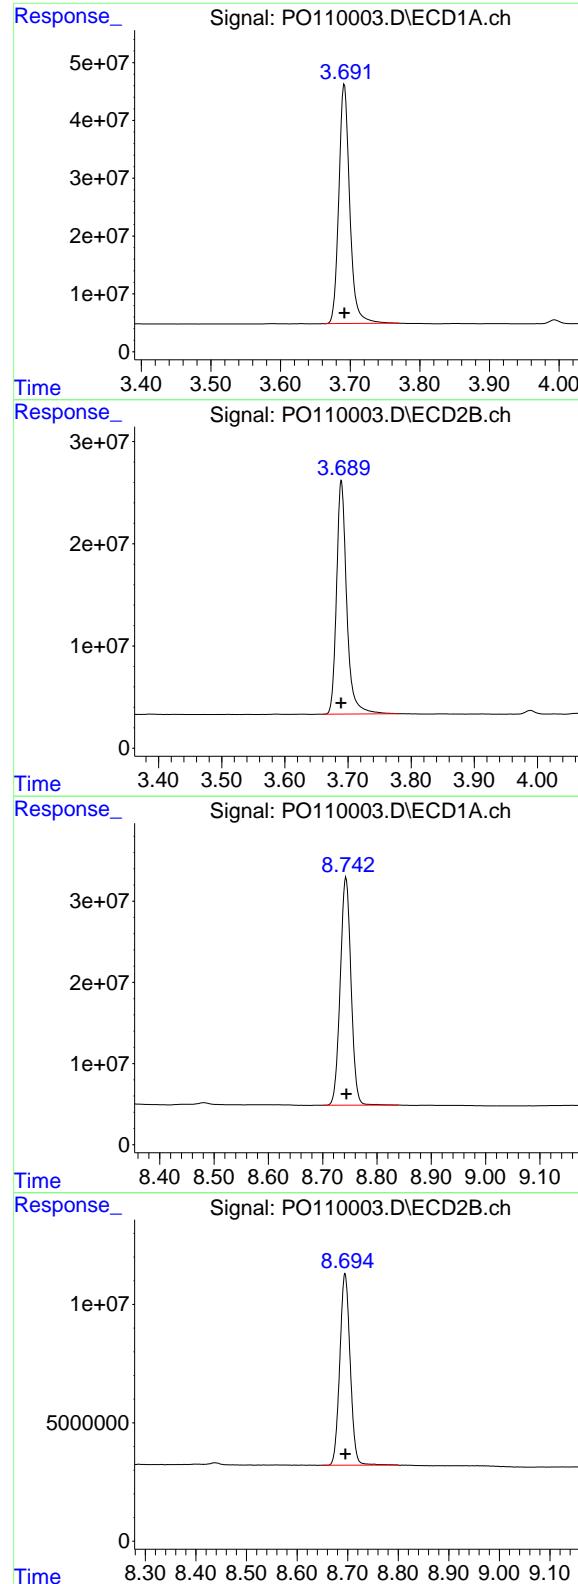

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
 Delta R.T.: 0.000 min  
 Response: 450272597  
 Conc: 47.97 ng/ml

Instrument: ECD\_O  
 ClientSampleId: ICVPO031925AR1254

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
 Delta R.T.: 0.000 min  
 Response: 255886625  
 Conc: 47.86 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.743 min  
 Delta R.T.: 0.000 min  
 Response: 386111719  
 Conc: 49.08 ng/ml


## #2 Decachlorobiphenyl

R.T.: 8.695 min  
 Delta R.T.: 0.000 min  
 Response: 115363596  
 Conc: 47.70 ng/ml

#26 AR-1254-1


R.T.: 5.593 min  
 Delta R.T.: 0.000 min  
 Response: 270904261  
 Conc: 484.35 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1254




#26 AR-1254-1

R.T.: 5.572 min  
 Delta R.T.: 0.000 min  
 Response: 148880437  
 Conc: 483.81 ng/ml

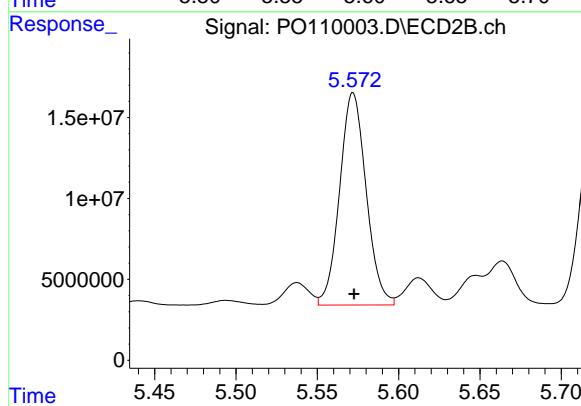


#27 AR-1254-2

R.T.: 5.743 min  
 Delta R.T.: 0.000 min  
 Response: 234269646  
 Conc: 484.33 ng/ml

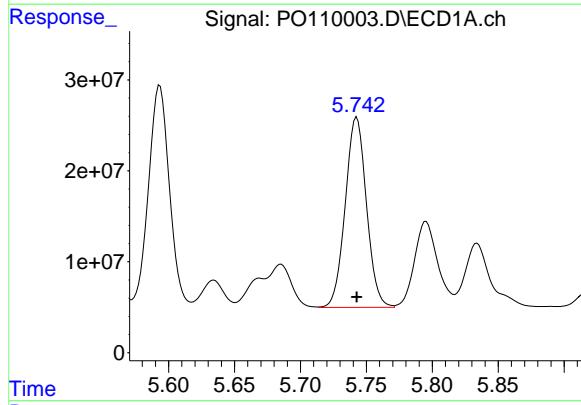

#27 AR-1254-2


R.T.: 5.720 min  
 Delta R.T.: 0.000 min  
 Response: 129704001  
 Conc: 483.09 ng/ml

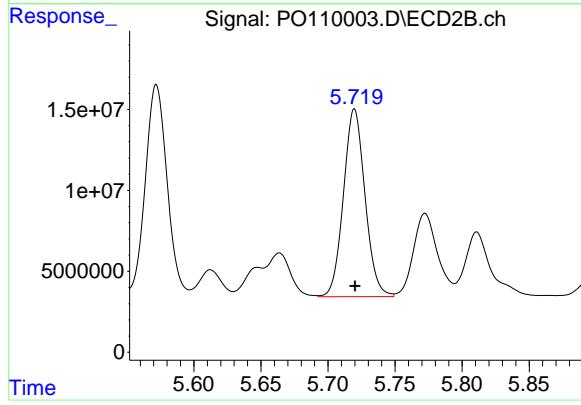

#28 AR-1254-3


R.T.: 6.148 min  
 Delta R.T.: 0.000 min  
 Response: 381837309  
 Conc: 483.78 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1254

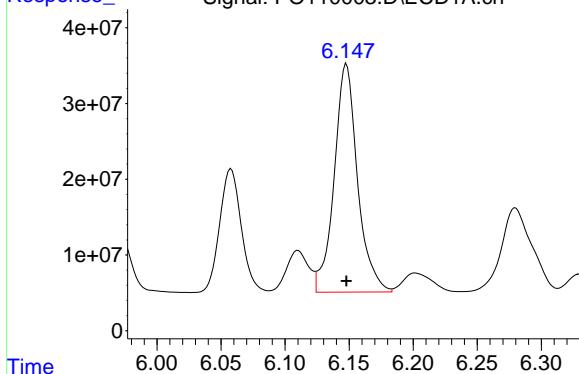


#28 AR-1254-3

R.T.: 6.123 min  
 Delta R.T.: 0.000 min  
 Response: 203649298  
 Conc: 483.49 ng/ml

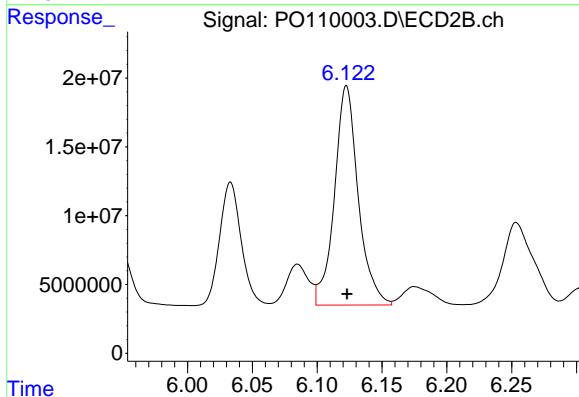


#29 AR-1254-4

R.T.: 6.377 min  
 Delta R.T.: 0.000 min  
 Response: 236662409  
 Conc: 486.51 ng/ml

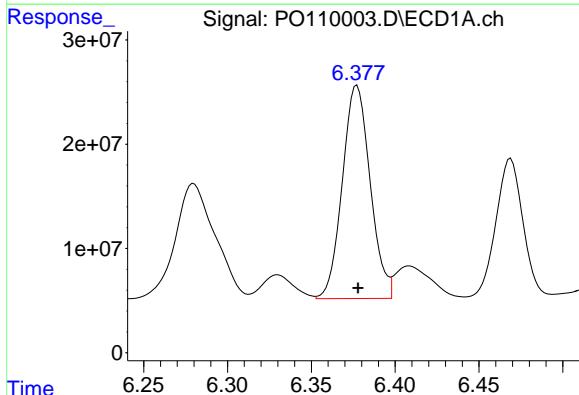

#29 AR-1254-4



R.T.: 6.350 min  
 Delta R.T.: 0.000 min  
 Response: 117742050  
 Conc: 481.78 ng/ml

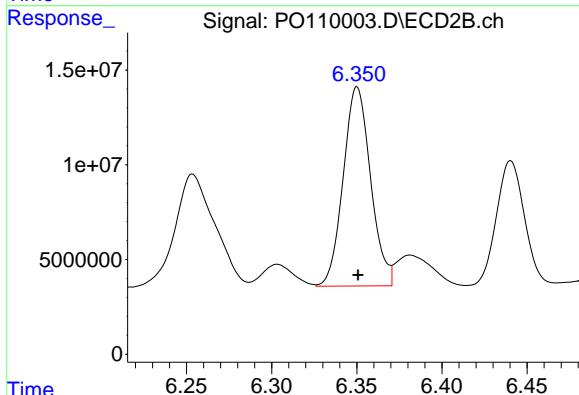

#30 AR-1254-5

R.T.: 6.797 min  
Delta R.T.: 0.000 min  
Response: 332152185  
Conc: 488.08 ng/ml

Instrument: ECD\_O  
ClientSampleId: ICVPO031925AR1254

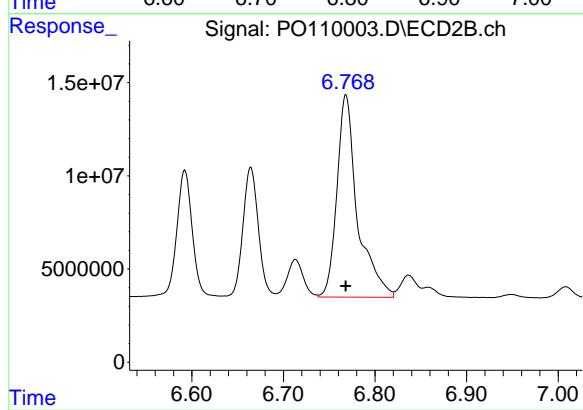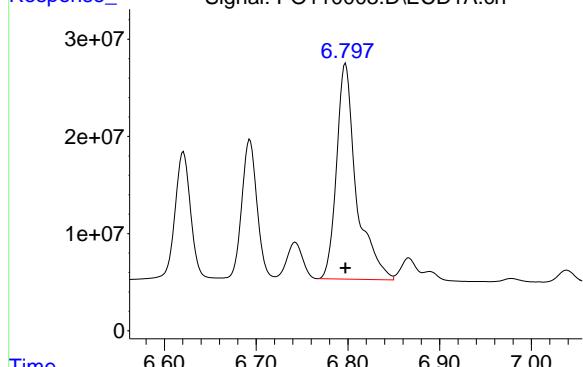

#30 AR-1254-5

R.T.: 6.768 min  
Delta R.T.: 0.000 min  
Response: 169138710  
Conc: 485.10 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110004.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Mar 2025 00:42  
 Operator : YP/AJ  
 Sample : AR1268ICV500  
 Misc :  
 ALS Vial : 35 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**ICVPO031925AR1268**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:07:25 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	450.4E6	255.9E6	48.546	48.447
2) SA Decachlor...	8.744	8.696	690.0E6	201.4E6	48.863	48.609

Target Compounds

41) L9 AR-1268-1	7.624	7.590	683.9E6	280.8E6	487.341	485.631
42) L9 AR-1268-2	7.689	7.654	622.6E6	259.1E6	486.560	486.478
43) L9 AR-1268-3	7.897	7.862	509.4E6	200.7E6	490.473	486.052
44) L9 AR-1268-4	8.184	8.146	217.2E6	79710818	485.391	491.969
45) L9 AR-1268-5	8.482	8.440	1574.6E6	478.9E6	487.695	485.135



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0110004.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Mar 2025 00:42  
 Operator : YP/AJ  
 Sample : AR1268ICV500  
 Misc :  
 ALS Vial : 35 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**ICVPO031925AR1268**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:07:25 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

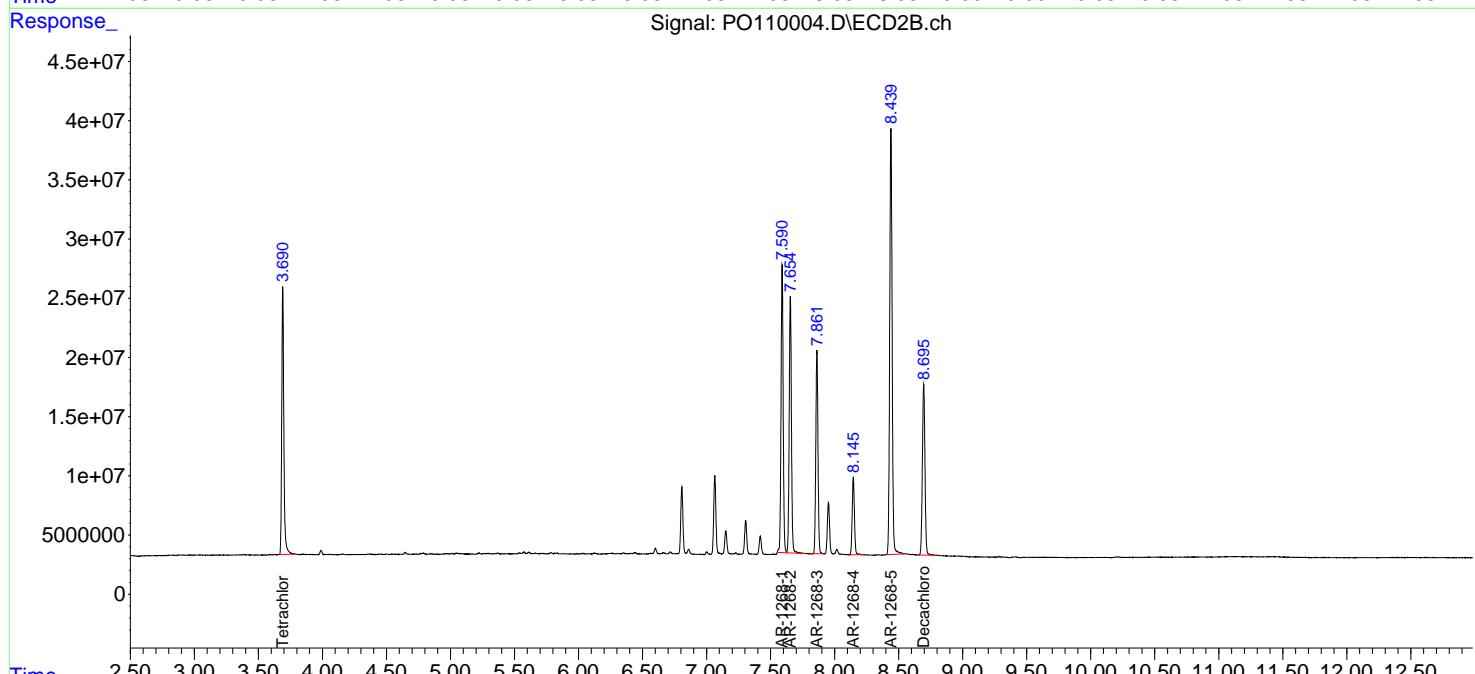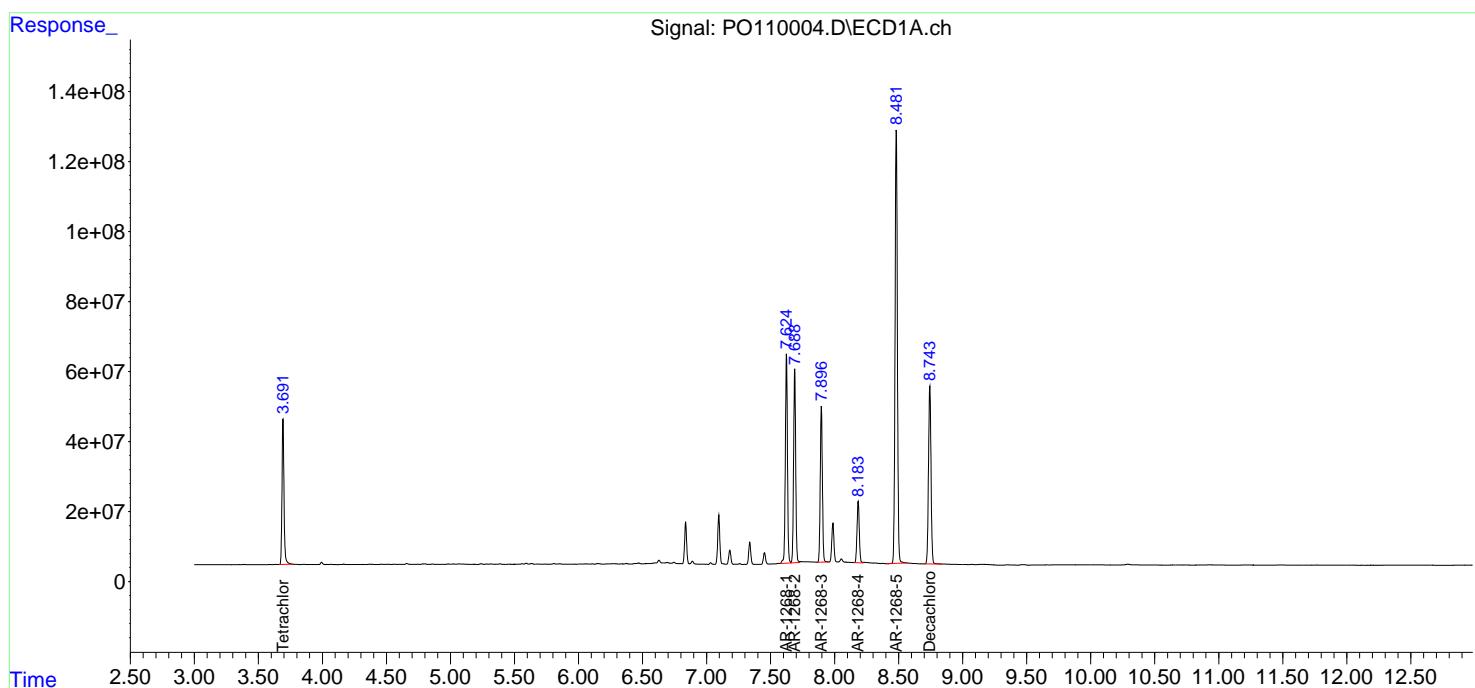

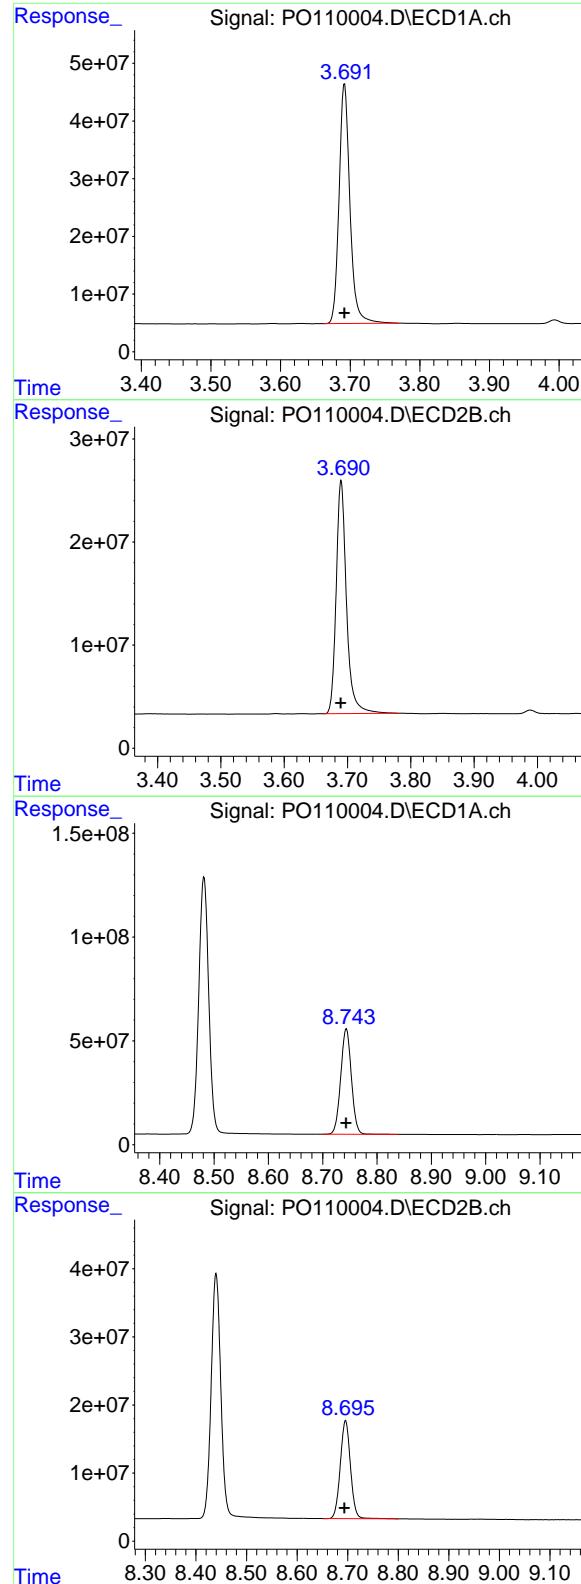

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
 Delta R.T.: 0.000 min  
 Response: 450382059  
 Conc: 48.55 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1268

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: 0.000 min  
 Response: 255894244  
 Conc: 48.45 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.744 min  
 Delta R.T.: 0.000 min  
 Response: 689957964  
 Conc: 48.86 ng/ml





## #2 Decachlorobiphenyl

R.T.: 8.696 min  
 Delta R.T.: 0.002 min  
 Response: 201448574  
 Conc: 48.61 ng/ml

#41 AR-1268-1

R.T.: 7.624 min  
 Delta R.T.: 0.002 min  
 Response: 683899311  
 Conc: 487.34 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1268

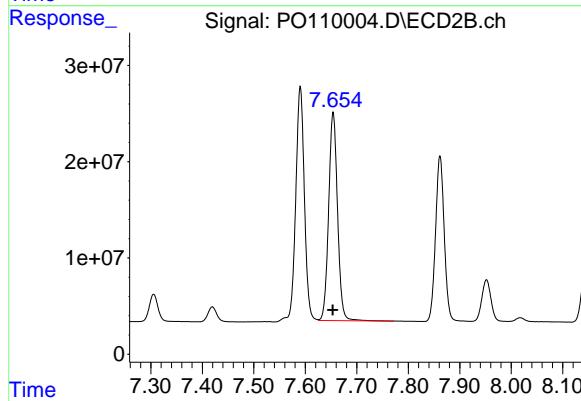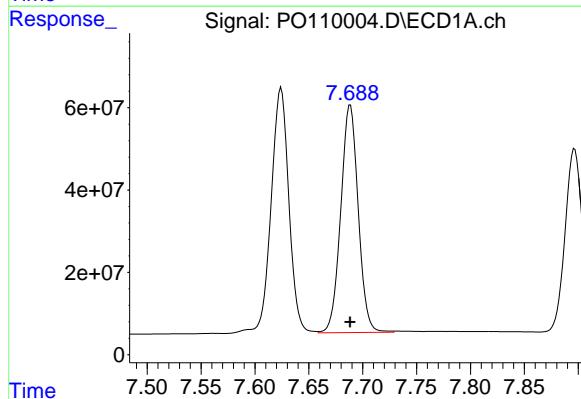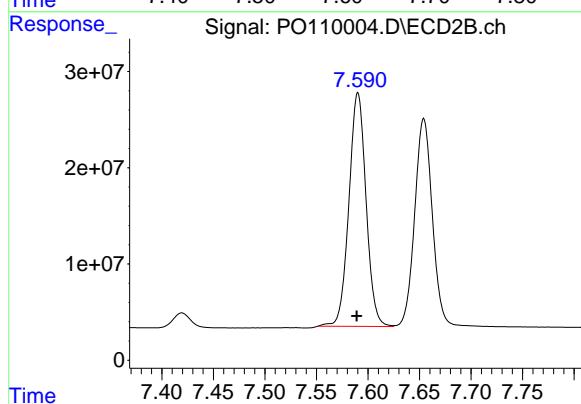

#41 AR-1268-1

R.T.: 7.590 min  
 Delta R.T.: 0.001 min  
 Response: 280794579  
 Conc: 485.63 ng/ml

#42 AR-1268-2

R.T.: 7.689 min  
 Delta R.T.: 0.000 min  
 Response: 622617772  
 Conc: 486.56 ng/ml


#42 AR-1268-2

R.T.: 7.654 min  
 Delta R.T.: 0.001 min  
 Response: 259115661  
 Conc: 486.48 ng/ml

#43 AR-1268-3


R.T.: 7.897 min  
 Delta R.T.: 0.000 min  
 Response: 509428626  
 Conc: 490.47 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** ICVPO031925AR1268

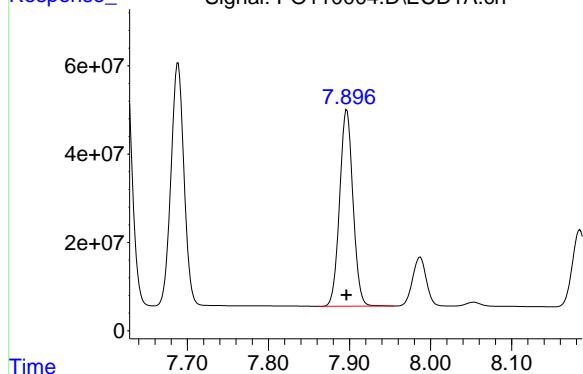


#43 AR-1268-3

R.T.: 7.862 min  
 Delta R.T.: 0.000 min  
 Response: 200699301  
 Conc: 486.05 ng/ml

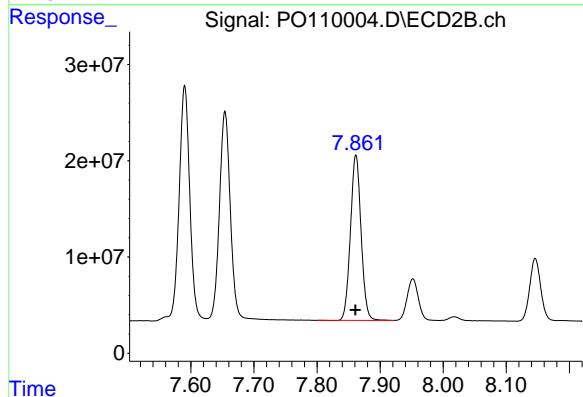


#44 AR-1268-4

R.T.: 8.184 min  
 Delta R.T.: 0.000 min  
 Response: 217182692  
 Conc: 485.39 ng/ml

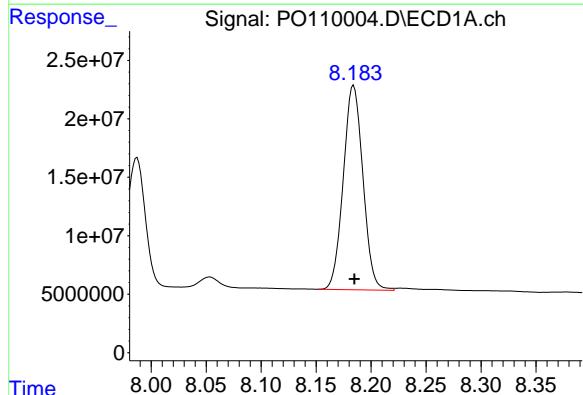

#44 AR-1268-4



R.T.: 8.146 min  
 Delta R.T.: 0.000 min  
 Response: 79710818  
 Conc: 491.97 ng/ml

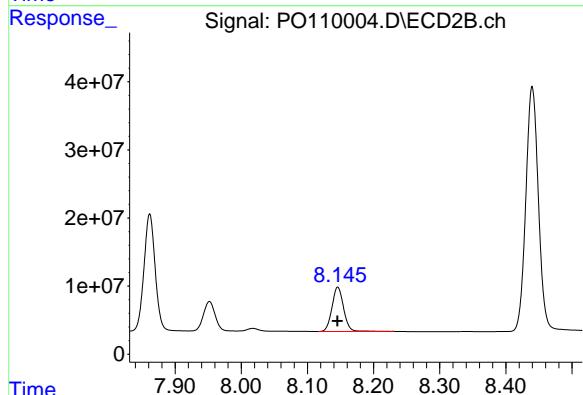

#45 AR-1268-5

R.T.: 8.482 min  
Delta R.T.: 0.000 min  
Response: 1574576275  
Conc: 487.70 ng/ml

Instrument: ECD\_O  
ClientSampleId: ICVPO031925AR1268

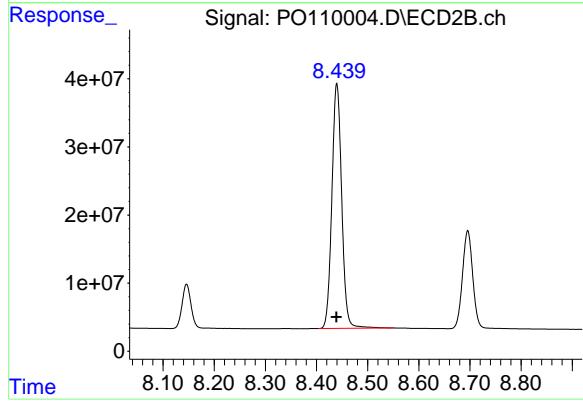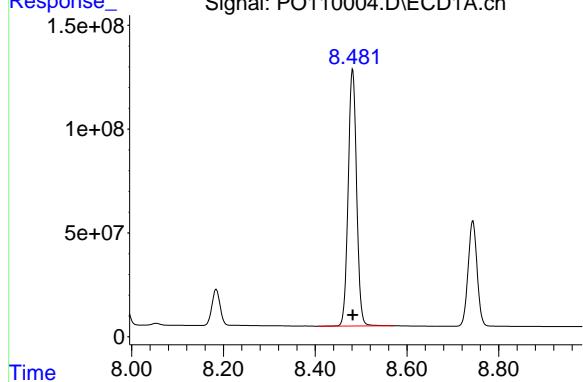

#45 AR-1268-5

R.T.: 8.440 min  
Delta R.T.: 0.000 min  
Response: 478896315  
Conc: 485.13 ng/ml

## RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<b>NOBI03</b>				
Lab Code:	<b>CHEM</b>	Case No.:	<b>Q1730</b>	SAS No.:	<b>Q1730</b>
Instrument ID:	<b>ECD_P</b>	Calibration Date(s):		<b>03/27/2025</b>	<b>03/27/2025</b>
		Calibration Times:		<b>10:30</b>	<b>17:53</b>

GC Column: **ZB-MR1** ID: **0.32** (mm)

LAB FILE ID:	RT 1000 =	<b>PP070917.D</b>	RT 750 =	<b>PP070918.D</b>
	RT 500 =	<b>PP070919.D</b>	RT 250 =	<b>PP070920.D</b>
			RT 050 =	<b>PP070921.D</b>

COMPOUND	RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW FROM	TO
Aroclor-1016-1 (1)	5.67	5.67	5.66	5.67	5.67	5.67	5.57	5.77
Aroclor-1016-2 (2)	5.69	5.69	5.69	5.69	5.69	5.69	5.59	5.79
Aroclor-1016-3 (3)	5.75	5.75	5.75	5.75	5.75	5.75	5.65	5.85
Aroclor-1016-4 (4)	5.85	5.85	5.85	5.85	5.85	5.85	5.75	5.95
Aroclor-1016-5 (5)	6.14	6.14	6.14	6.14	6.14	6.14	6.04	6.24
Aroclor-1260-1 (1)	7.26	7.26	7.26	7.26	7.26	7.26	7.16	7.36
Aroclor-1260-2 (2)	7.51	7.51	7.51	7.51	7.51	7.51	7.41	7.61
Aroclor-1260-3 (3)	7.87	7.87	7.87	7.87	7.87	7.87	7.77	7.97
Aroclor-1260-4 (4)	8.10	8.10	8.09	8.09	8.09	8.09	7.99	8.19
Aroclor-1260-5 (5)	8.41	8.42	8.41	8.41	8.41	8.41	8.31	8.51
Decachlorobiphenyl	10.23	10.23	10.23	10.23	10.23	10.23	10.13	10.33
Tetrachloro-m-xylene	4.51	4.52	4.51	4.52	4.51	4.51	4.41	4.61
Aroclor-1242-1 (1)	5.67	5.67	5.66	5.67	5.66	5.67	5.57	5.77
Aroclor-1242-2 (2)	5.69	5.69	5.69	5.69	5.69	5.69	5.59	5.79
Aroclor-1242-3 (3)	5.75	5.75	5.75	5.75	5.75	5.75	5.65	5.85
Aroclor-1242-4 (4)	5.85	5.85	5.85	5.85	5.84	5.85	5.75	5.95
Aroclor-1242-5 (5)	6.58	6.58	6.58	6.58	6.57	6.58	6.48	6.68
Decachlorobiphenyl	10.23	10.23	10.23	10.23	10.23	10.23	10.13	10.33
Tetrachloro-m-xylene	4.51	4.51	4.51	4.51	4.51	4.51	4.41	4.61
Aroclor-1248-1 (1)	5.67	5.67	5.67	5.67	5.67	5.67	5.57	5.77
Aroclor-1248-2 (2)	5.94	5.94	5.94	5.94	5.94	5.94	5.84	6.04
Aroclor-1248-3 (3)	6.14	6.14	6.14	6.14	6.14	6.14	6.04	6.24
Aroclor-1248-4 (4)	6.54	6.54	6.54	6.54	6.54	6.54	6.44	6.64
Aroclor-1248-5 (5)	6.58	6.58	6.58	6.58	6.58	6.58	6.48	6.68
Decachlorobiphenyl	10.23	10.23	10.23	10.23	10.23	10.23	10.13	10.33
Tetrachloro-m-xylene	4.51	4.51	4.51	4.52	4.51	4.51	4.41	4.61
Aroclor-1254-1 (1)	6.52	6.52	6.52	6.52	6.52	6.52	6.42	6.62
Aroclor-1254-2 (2)	6.73	6.73	6.73	6.73	6.73	6.73	6.63	6.83
Aroclor-1254-3 (3)	7.10	7.09	7.10	7.10	7.10	7.10	7.00	7.20
Aroclor-1254-4 (4)	7.38	7.38	7.38	7.38	7.38	7.38	7.28	7.48
Aroclor-1254-5 (5)	7.79	7.79	7.79	7.79	7.79	7.79	7.69	7.89
Decachlorobiphenyl	10.23	10.23	10.23	10.23	10.23	10.23	10.13	10.33
Tetrachloro-m-xylene	4.51	4.51	4.51	4.51	4.52	4.51	4.41	4.61
Aroclor-1268-1 (1)	8.73	8.73	8.73	8.73	8.73	8.73	8.63	8.83
Aroclor-1268-2 (2)	8.82	8.82	8.82	8.82	8.82	8.82	8.72	8.92
Aroclor-1268-3 (3)	9.06	9.06	9.05	9.06	9.05	9.06	8.96	9.16
Aroclor-1268-4 (4)	9.47	9.47	9.47	9.47	9.47	9.47	9.37	9.57
Aroclor-1268-5 (5)	9.89	9.89	9.89	9.89	9.89	9.89	9.79	9.99



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

#### RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	10.23	10.23	10.23	10.23	10.23	10.23	10.13	10.33	1
Tetrachloro-m-xylene	4.52	4.51	4.51	4.52	4.51	4.51	4.41	4.61	2

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>NOBI03</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1730</u>	SAS No.:	<u>Q1730</u>	SDG NO.:	<u>Q1730</u>
Instrument ID:	<u>ECD_P</u>	Calibration Date(s):			<u>03/27/2025</u>	<u>03/27/2025</u>	
		Calibration Times:			<u>10:30</u>	<u>17:53</u>	

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	<u>PP070917.D</u>	RT 750 =	<u>PP070918.D</u>
	RT 500 =	<u>PP070919.D</u>	RT 250 =	<u>PP070920.D</u>
			RT 050 =	<u>PP070921.D</u>

COMPOUND	RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW FROM	TO
Aroclor-1016-1 (1)	4.90	4.90	4.90	4.90	4.90	4.90	4.80	5.00
Aroclor-1016-2 (2)	4.92	4.92	4.92	4.92	4.92	4.92	4.82	5.02
Aroclor-1016-3 (3)	5.10	5.10	5.10	5.10	5.10	5.10	5.00	5.20
Aroclor-1016-4 (4)	5.14	5.14	5.14	5.14	5.14	5.14	5.04	5.24
Aroclor-1016-5 (5)	5.36	5.36	5.36	5.36	5.36	5.36	5.26	5.46
Aroclor-1260-1 (1)	6.39	6.39	6.39	6.39	6.39	6.39	6.29	6.49
Aroclor-1260-2 (2)	6.58	6.58	6.58	6.58	6.58	6.58	6.48	6.68
Aroclor-1260-3 (3)	6.73	6.73	6.73	6.73	6.73	6.73	6.63	6.83
Aroclor-1260-4 (4)	7.20	7.20	7.21	7.21	7.21	7.20	7.10	7.30
Aroclor-1260-5 (5)	7.45	7.44	7.45	7.45	7.45	7.45	7.35	7.55
Decachlorobiphenyl	8.86	8.86	8.86	8.86	8.86	8.86	8.76	8.96
Tetrachloro-m-xylene	3.82	3.82	3.82	3.82	3.82	3.82	3.72	3.92
Aroclor-1242-1 (1)	4.90	4.90	4.90	4.90	4.90	4.90	4.80	5.00
Aroclor-1242-2 (2)	4.92	4.92	4.92	4.92	4.92	4.92	4.82	5.02
Aroclor-1242-3 (3)	5.10	5.10	5.10	5.10	5.10	5.10	5.00	5.20
Aroclor-1242-4 (4)	5.18	5.18	5.18	5.18	5.18	5.18	5.08	5.28
Aroclor-1242-5 (5)	5.71	5.71	5.71	5.71	5.71	5.71	5.61	5.81
Decachlorobiphenyl	8.86	8.86	8.86	8.86	8.86	8.86	8.76	8.96
Tetrachloro-m-xylene	3.82	3.82	3.82	3.82	3.82	3.82	3.72	3.92
Aroclor-1248-1 (1)	4.90	4.90	4.90	4.90	4.90	4.90	4.80	5.00
Aroclor-1248-2 (2)	5.14	5.14	5.14	5.14	5.14	5.14	5.04	5.24
Aroclor-1248-3 (3)	5.18	5.18	5.18	5.18	5.18	5.18	5.08	5.28
Aroclor-1248-4 (4)	5.36	5.36	5.36	5.36	5.36	5.36	5.26	5.46
Aroclor-1248-5 (5)	5.75	5.75	5.75	5.75	5.75	5.75	5.65	5.85
Decachlorobiphenyl	8.86	8.86	8.86	8.86	8.86	8.86	8.76	8.96
Tetrachloro-m-xylene	3.82	3.82	3.82	3.82	3.82	3.82	3.72	3.92
Aroclor-1254-1 (1)	5.71	5.71	5.71	5.71	5.71	5.71	5.61	5.81
Aroclor-1254-2 (2)	5.86	5.86	5.86	5.86	5.86	5.86	5.76	5.96
Aroclor-1254-3 (3)	6.26	6.26	6.26	6.26	6.26	6.26	6.16	6.36
Aroclor-1254-4 (4)	6.49	6.49	6.49	6.49	6.49	6.49	6.39	6.59
Aroclor-1254-5 (5)	6.91	6.91	6.91	6.91	6.91	6.91	6.81	7.01
Decachlorobiphenyl	8.86	8.86	8.86	8.86	8.86	8.86	8.76	8.96
Tetrachloro-m-xylene	3.82	3.82	3.82	3.82	3.82	3.82	3.72	3.92
Aroclor-1268-1 (1)	7.73	7.73	7.73	7.73	7.73	7.73	7.63	7.83
Aroclor-1268-2 (2)	7.80	7.80	7.79	7.79	7.79	7.79	7.69	7.89
Aroclor-1268-3 (3)	8.00	8.00	8.00	8.00	8.00	8.00	7.90	8.10
Aroclor-1268-4 (4)	8.30	8.29	8.29	8.30	8.29	8.29	8.19	8.39
Aroclor-1268-5 (5)	8.60	8.60	8.60	8.60	8.60	8.60	8.50	8.70



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

**RETENTION TIMES OF INITIAL CALIBRATION**

Decachlorobiphenyl	8.86	8.86	8.86	8.86	8.86	8.86	8.76	8.96	1
Tetrachloro-m-xylene	3.82	3.82	3.82	3.82	3.82	3.82	3.72	3.92	2

3

4

5

6

7

8

9

10

11

12

13

14

15

16

17

18

19

20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract:	<b>NOBI03</b>							
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1730</u>	SAS No.:	<u>Q1730</u>	SDG NO.:	<u>Q1730</u>	
Instrument ID:	<u>ECD_P</u>				Calibration Date(s):	<u>03/27/2025</u>	<u>03/27/2025</u>	
					Calibration Times:	<u>10:30</u>	<u>17:53</u>	
GC Column:	<u>ZB-MR1</u>	ID:	<u>0.32</u> (mm)					

LAB FILE ID:	CF 1000 =	PP070917.D	CF 750 =	PP070918.D			
	CF 500 =	<u>PP070919.D</u>	CF 250 =	<u>PP070920.D</u>	CF 050 =	<u>PP070921.D</u>	
COMPOUND	CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1 (1)	47478014	49171687	50934060	54324668	52347880	50851262	5
Aroclor-1016-2 (2)	72483549	74568483	78811172	80433884	83971080	78053634	6
Aroclor-1016-3 (3)	43541298	44043953	46815864	48849960	52621940	47174603	7
Aroclor-1016-4 (4)	36661280	36602855	39014928	39212148	32287440	36755730	7
Aroclor-1016-5 (5)	32204227	33487635	35040682	36610940	32217200	33912137	5
Aroclor-1260-1 (1)	60625379	62238407	66823960	72729028	73347280	67152811	8
Aroclor-1260-2 (2)	90805769	95497569	97808710	102858984	93710780	96136362	4
Aroclor-1260-3 (3)	75946924	78957439	82970652	86114216	75601760	79918198	5
Aroclor-1260-4 (4)	67190656	75020355	81451428	78145636	91876440	78736903	11
Aroclor-1260-5 (5)	154592706	156108101	159960800	166857288	156911780	158886135	3
Decachlorobiphenyl	1019047430	1065730867	1116449000	1115108760	946747800	1052616771	7
Tetrachloro-m-xylene	1424837400	1461405720	1519248320	1595716440	1306667000	1461574976	7
Aroclor-1242-1 (1)	40990074	42746281	43432670	43984636	48732080	43977148	6
Aroclor-1242-2 (2)	64704598	63862937	67024876	68850388	57138840	64316328	7
Aroclor-1242-3 (3)	39349869	38048504	39702972	40627540	47468380	41039453	9
Aroclor-1242-4 (4)	30814559	31466187	32277086	32194644	25864220	30523339	8
Aroclor-1242-5 (5)	36006298	34981232	37334376	38560396	35669740	36510408	4
Decachlorobiphenyl	1036298130	1063489027	1106293120	1153452680	1056566000	1083219791	4
Tetrachloro-m-xylene	1443947330	1507747640	1537397120	1567165920	1326698400	1476591282	6
Aroclor-1248-1 (1)	31141042	33379292	33781538	45988760	37146900	36287506	15
Aroclor-1248-2 (2)	42399779	44979081	46192256	47122176	43999640	44938586	4
Aroclor-1248-3 (3)	48055172	50777464	51825052	50697180	51832600	50637494	3
Aroclor-1248-4 (4)	59878410	63471275	67039892	73429036	56919340	64147591	9
Aroclor-1248-5 (5)	56652876	60504408	64286140	68519384	54268440	60846250	9
Decachlorobiphenyl	1072017300	1124462173	1205136680	1167091680	1109917800	1135725127	5
Tetrachloro-m-xylene	1462181050	1544091280	1549039360	1559485200	1464932600	1515945898	3
Aroclor-1254-1 (1)	60157506	63067431	65471886	66806416	66447920	64390232	4
Aroclor-1254-2 (2)	92838442	97047215	101802392	105556104	108208740	101090579	6
Aroclor-1254-3 (3)	92334650	98055471	99416554	103841140	104991280	99727819	5
Aroclor-1254-4 (4)	84238161	87780547	86802510	88788836	85373700	86596751	2
Aroclor-1254-5 (5)	74433164	79038301	80854650	83958584	83470140	80350968	5
Decachlorobiphenyl	1095432410	1144692320	1168417220	1194330360	1035516600	1127677782	6
Tetrachloro-m-xylene	1501288360	1551275560	1575746420	1626904120	1301718600	1511386612	8
Aroclor-1268-1 (1)	226575551	237927453	239660032	247892192	225482800	235507606	4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

#### CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	190380276	198934901	200232346	204948924	182079900	195315269	4
Aroclor-1268-3	(3)	163648333	171737784	173955356	177246576	167979860	170913582	3
Aroclor-1268-4	(4)	70377008	73665913	73237284	74802952	61652780	70747187	7
Aroclor-1268-5	(5)	459553484	481598519	482514296	498456744	458756600	476175929	3
Decachlorobiphenyl		1956984350	2055290840	2095781900	2171413960	2007035400	2057301290	4
Tetrachloro-m-xylene		1523485290	1594639080	1607574540	1645012520	1440121400	1562166566	5

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract:	<b>NOBI03</b>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1730</u>	SAS No.:	<u>Q1730</u>	SDG NO.:	<u>Q1730</u>
Instrument ID:	<u>ECD_P</u>				Calibration Date(s):	<u>03/27/2025</u>	<u>03/27/2025</u>
					Calibration Times:	<u>10:30</u>	<u>17:53</u>

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:	CF 1000 =	CF 750 =	CF 500 =	CF 250 =	CF 050 =	CF	% RSD
	<u>PP070917.D</u>	<u>PP070918.D</u>	<u>PP070919.D</u>	<u>PP070920.D</u>	<u>PP070921.D</u>		
COMPOUND	CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1 (1)	34208953	37661787	37955886	45294856	45319420	40088180	12
Aroclor-1016-2 (2)	49610574	53393839	54380778	65503040	66437080	57865062	12
Aroclor-1016-3 (3)	27000462	29732755	29849058	35508136	32526120	30923306	10
Aroclor-1016-4 (4)	21229955	23465415	23793788	28635320	24655080	24355912	10
Aroclor-1016-5 (5)	26939544	29893109	30154374	37292184	37326660	32321174	14
Aroclor-1260-1 (1)	45249076	46519276	48240522	56226688	59796020	51206316	12
Aroclor-1260-2 (2)	58475471	61260192	62904038	69183788	67145740	63793846	6
Aroclor-1260-3 (3)	50913622	52312629	53920638	58739540	56547700	54486826	5
Aroclor-1260-4 (4)	42366044	44395528	47488628	49955128	54926140	47826294	10
Aroclor-1260-5 (5)	113066934	116639771	125312810	127263128	140268800	124510289	8
Decachlorobiphenyl	793547960	846236520	865016160	753569280	682611000	788196184	9
Tetrachloro-m-xylene	926488500	1023245573	1036748080	1124812280	1071924800	1036643847	7
Aroclor-1242-1 (1)	30391529	31772724	34649408	38698720	35466820	34195840	9
Aroclor-1242-2 (2)	43879042	45075739	49434800	55503780	52395240	49257720	9
Aroclor-1242-3 (3)	24103124	24630729	26618958	29833472	28035100	26644277	8
Aroclor-1242-4 (4)	23086538	23159225	25581538	28618736	31445140	26378235	13
Aroclor-1242-5 (5)	28647762	29235153	31558738	32962404	32387440	30958299	6
Decachlorobiphenyl	794686010	779465320	775544600	851493360	677466800	775731218	8
Tetrachloro-m-xylene	994474400	1020857307	1119824860	1120535680	1106593200	1072457089	6
Aroclor-1248-1 (1)	23297586	26737011	28501250	29207540	27656520	27079981	8
Aroclor-1248-2 (2)	31071420	35918237	38274460	38702620	39645560	36722459	9
Aroclor-1248-3 (3)	32592570	37701093	39964120	40477712	42561380	38659375	9
Aroclor-1248-4 (4)	38114246	43411732	47181776	48244244	48753000	45141000	9
Aroclor-1248-5 (5)	37031094	41115012	43925318	46634268	44688040	42678746	8
Decachlorobiphenyl	763432400	822192813	827097300	806313080	732328400	790272799	5
Tetrachloro-m-xylene	969522160	1045815880	1138159760	1084071480	1169729800	1081459816	7
Aroclor-1254-1 (1)	58928147	61799583	66082486	73787844	69490960	66017804	8
Aroclor-1254-2 (2)	50145967	53786207	56793554	64034708	60730300	57098147	9
Aroclor-1254-3 (3)	77448562	83642240	87764778	99090376	86260880	86841367	9
Aroclor-1254-4 (4)	49998215	54614948	55966900	64174348	55747980	56100478	9
Aroclor-1254-5 (5)	65979008	71358709	71825896	82425644	69163880	72150627	8
Decachlorobiphenyl	783483810	796181933	910832540	850283840	759277600	820011945	7
Tetrachloro-m-xylene	1042595600	1091536387	1108578240	1195164040	1067355200	1101045893	5
Aroclor-1268-1 (1)	165356134	175541800	174753666	176934688	164423820	171402022	3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

#### CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	137801505	147739099	145758868	146778256	138336660	143282878	3
Aroclor-1268-3	(3)	120132746	127507232	124391202	127247744	116467620	123149309	4
Aroclor-1268-4	(4)	51096977	54505272	53344994	55689972	49428660	52813175	5
Aroclor-1268-5	(5)	357060145	376226307	370949858	366544744	338563340	361868879	4
Decachlorobiphenyl		1484820890	1579158933	1563503220	1620729960	1432317200	1536106041	5
Tetrachloro-m-xylene		1051289840	1118865693	1118283520	1183542080	1260888000	1146573827	7

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Instrument ID: ECD\_P Date(s) Analyzed: 03/27/2025 03/27/2025

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	4.72	4.62	4.82	17353700
		2	4.80	4.70	4.90	12952900
		3	4.88	4.78	4.98	41717200
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.88	4.78	4.98	33288800
		2	5.41	5.31	5.51	15910300
		3	5.69	5.59	5.79	34270400
		4	5.85	5.75	5.95	15707600
		5	5.94	5.84	6.04	10640400
Aroclor-1262	500	1	8.09	7.99	8.19	106300000
		2	8.41	8.31	8.51	198383000
		3	8.73	8.63	8.83	131742000
		4	8.82	8.72	8.92	95614800
		5	9.47	9.37	9.57	65066400



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Instrument ID: ECD\_P Date(s) Analyzed: 03/27/2025 03/27/2025

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	4.03	3.93	4.13	15243600
		2	4.11	4.01	4.21	11436300
		3	4.19	4.09	4.29	34089000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.19	4.09	4.29	27986800
		2	4.92	4.82	5.02	28061200
		3	5.10	5.00	5.20	14889600
		4	5.19	5.09	5.29	12804400
		5	5.36	5.26	5.46	14174800
Aroclor-1262	500	1	6.95	6.85	7.05	85563600
		2	7.21	7.11	7.31	68464400
		3	7.73	7.63	7.83	60723600
		4	7.79	7.69	7.89	99406800
		5	8.29	8.19	8.39	46871600

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070917.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 10:30  
 Operator : YP\AJ  
 Sample : AR1660ICC1000  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 11:43:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.513	3.815	142.5E6	92648850	93.786	89.365
2) SA Decachloro...	10.227	8.858	101.9E6	79354796	91.276	91.738

**Target Compounds**

3) L1 AR-1016-1	5.665	4.903	47478014	34208953	932.147	901.282
4) L1 AR-1016-2	5.687	4.921	72483549	49610574	919.712	912.281
5) L1 AR-1016-3	5.749	5.098	43541298	27000462	930.054	904.567
6) L1 AR-1016-4	5.846	5.140	36661280	21229955	939.673	892.248
7) L1 AR-1016-5	6.140	5.355	32204227	26939544	919.053	893.388
31) L7 AR-1260-1	7.258	6.391	60625379	45249076	907.240	937.989
32) L7 AR-1260-2	7.512	6.579	90805769	58475471	928.402	929.598
33) L7 AR-1260-3	7.870	6.732	75946924	50913622	915.347	944.233
34) L7 AR-1260-4	8.095	7.204	67190656	42366044	824.917	892.130
35) L7 AR-1260-5	8.413	7.445	154.6E6	113.1E6	966.441	902.278


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.




Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070917.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 10:30  
 Operator : YP\AJ  
 Sample : AR1660ICC1000  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1660ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 11:43:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

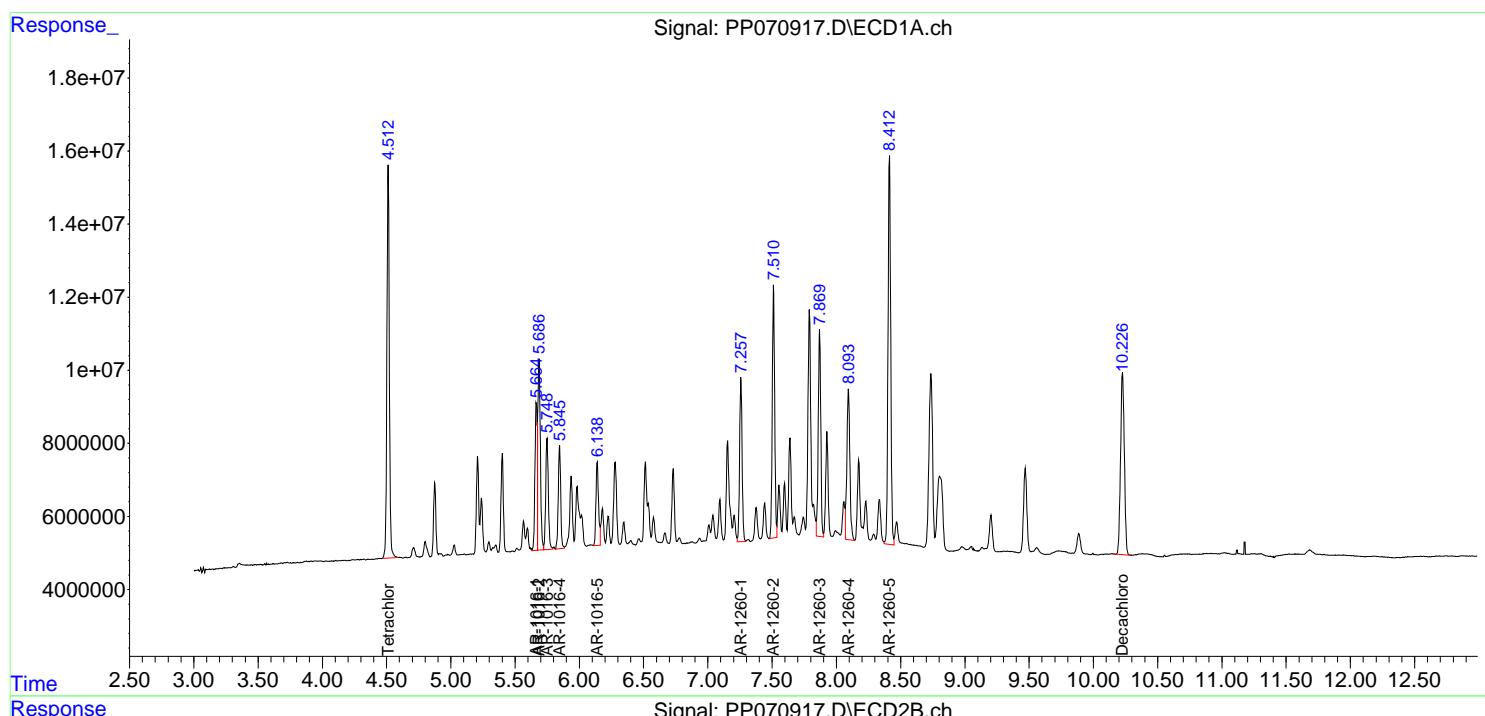

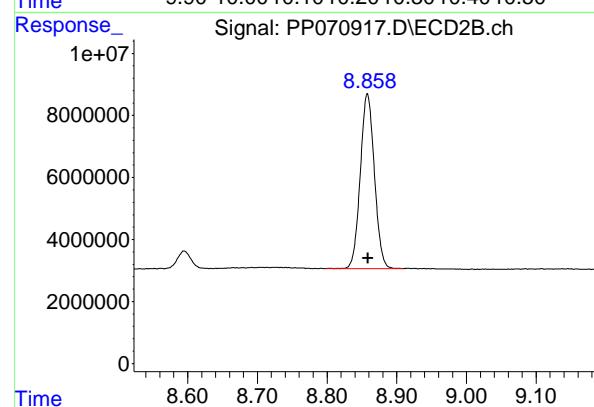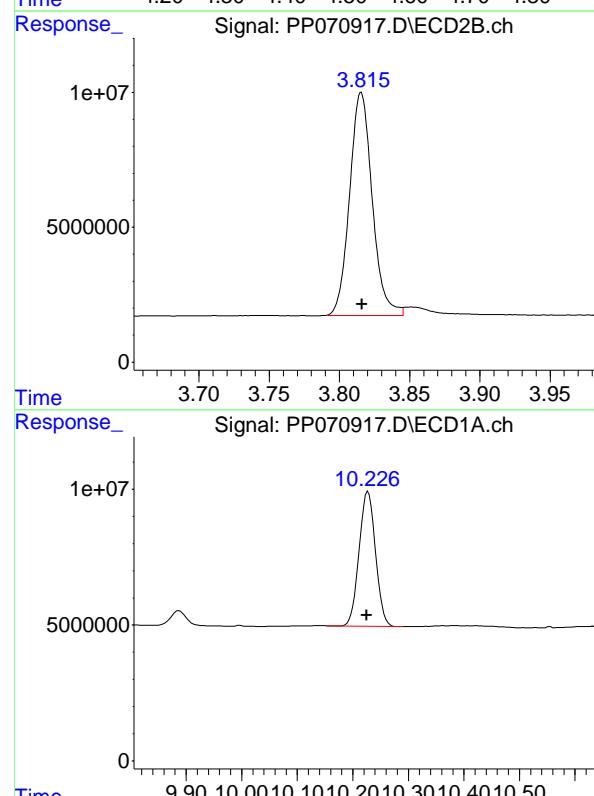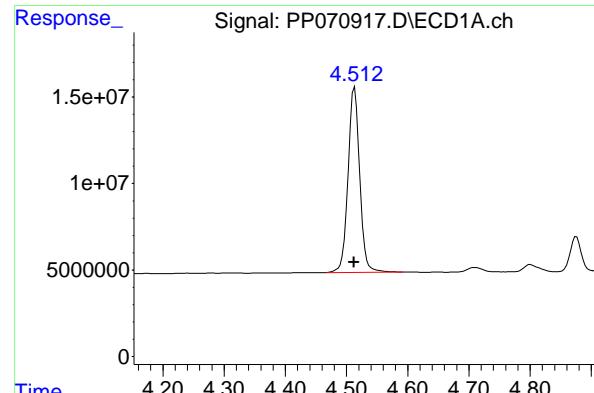

## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
 Delta R.T.: 0.001 min  
 Response: 142483740 ECD\_P  
 Conc: 93.79 ng/ml ClientSampleId : AR1660ICC1000

## #1 Tetrachloro-m-xylene

R.T.: 3.815 min  
 Delta R.T.: 0.000 min  
 Response: 92648850  
 Conc: 89.36 ng/ml

## #2 Decachlorobiphenyl


R.T.: 10.227 min  
 Delta R.T.: 0.002 min  
 Response: 101904743  
 Conc: 91.28 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.858 min  
 Delta R.T.: 0.000 min  
 Response: 79354796  
 Conc: 91.74 ng/ml


#3 AR-1016-1

R.T.: 5.665 min  
 Delta R.T.: 0.002 min  
 Response: 47478014 ECD\_P  
 Conc: 932.15 ng/ml ClientSampleId : AR1660ICC1000

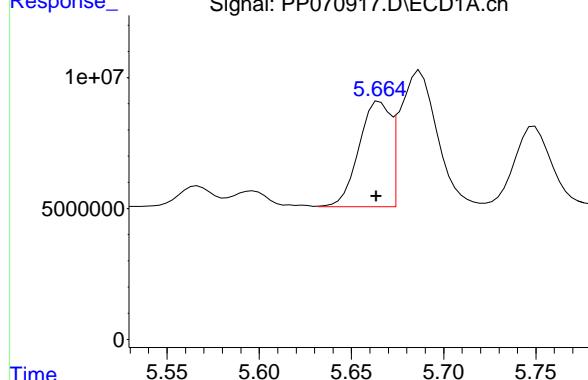


#3 AR-1016-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 34208953  
 Conc: 901.28 ng/ml

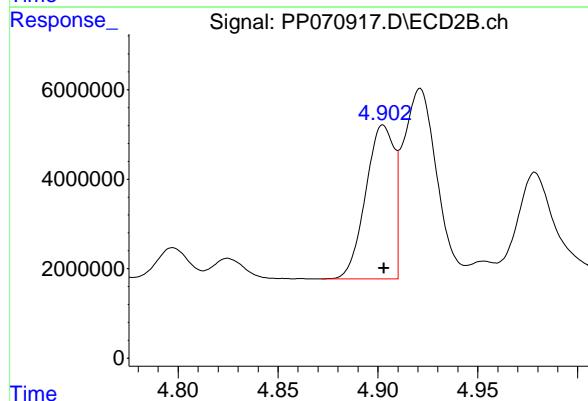


#4 AR-1016-2

R.T.: 5.687 min  
 Delta R.T.: 0.002 min  
 Response: 72483549  
 Conc: 919.71 ng/ml

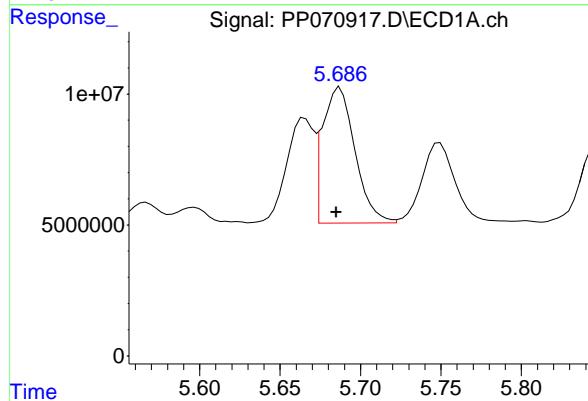


#4 AR-1016-2

R.T.: 4.921 min  
 Delta R.T.: 0.000 min  
 Response: 49610574  
 Conc: 912.28 ng/ml

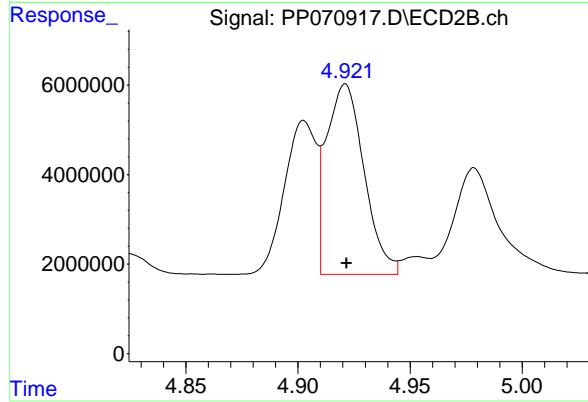


#5 AR-1016-3

R.T.: 5.749 min  
 Delta R.T.: 0.002 min  
 Response: 43541298 ECD\_P  
 Conc: 930.05 ng/ml ClientSampleId : AR1660ICC1000

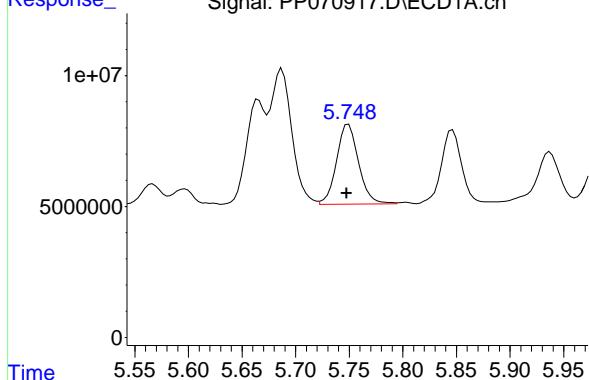


#5 AR-1016-3

R.T.: 5.098 min  
 Delta R.T.: 0.000 min  
 Response: 27000462  
 Conc: 904.57 ng/ml

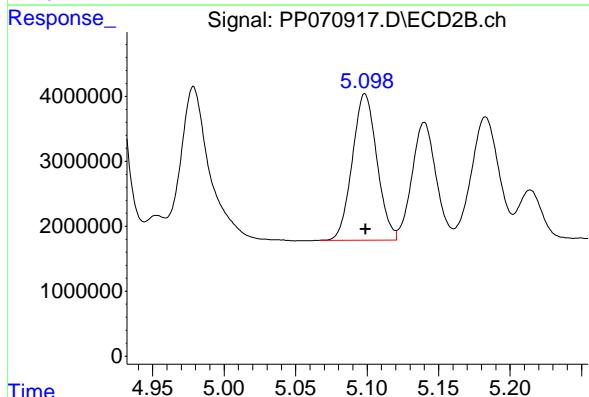


#6 AR-1016-4

R.T.: 5.846 min  
 Delta R.T.: 0.001 min  
 Response: 36661280  
 Conc: 939.67 ng/ml

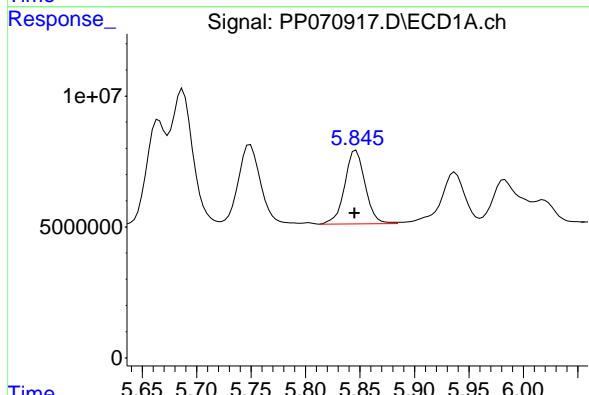


#6 AR-1016-4

R.T.: 5.140 min  
 Delta R.T.: 0.000 min  
 Response: 21229955  
 Conc: 892.25 ng/ml

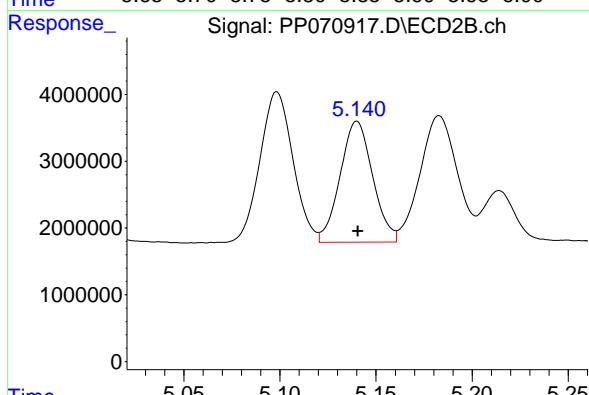


#7 AR-1016-5

R.T.: 6.140 min  
 Delta R.T.: 0.002 min  
 Response: 32204227  
 Conc: 919.05 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** AR1660ICC1000

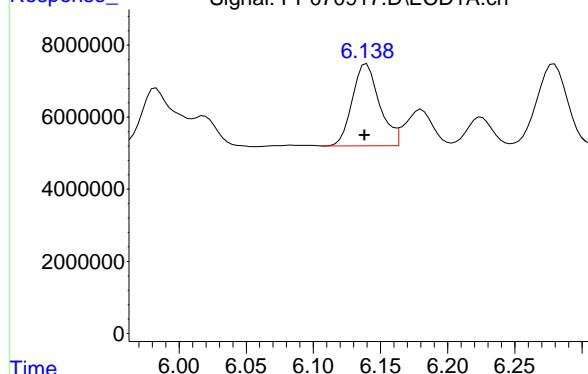


#7 AR-1016-5

R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 26939544  
 Conc: 893.39 ng/ml

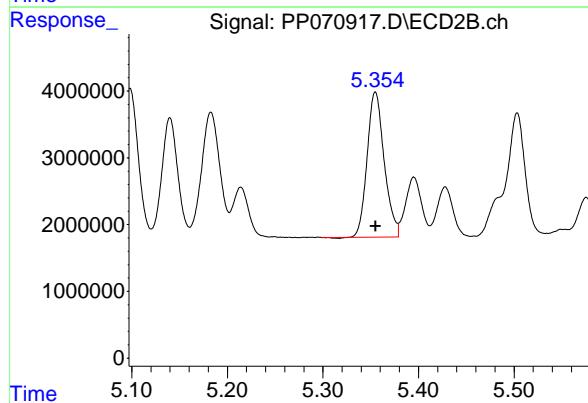


#31 AR-1260-1

R.T.: 7.258 min  
 Delta R.T.: 0.002 min  
 Response: 60625379  
 Conc: 907.24 ng/ml

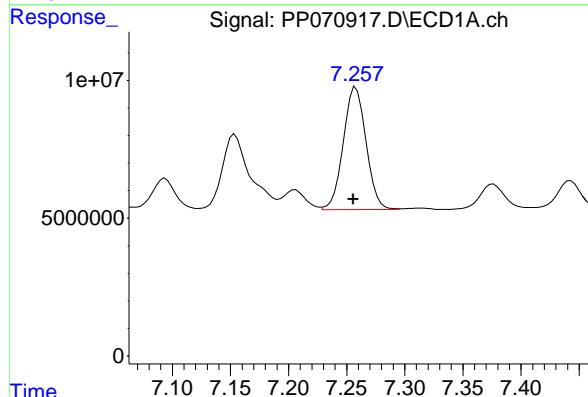


#31 AR-1260-1

R.T.: 6.391 min  
 Delta R.T.: 0.000 min  
 Response: 45249076  
 Conc: 937.99 ng/ml

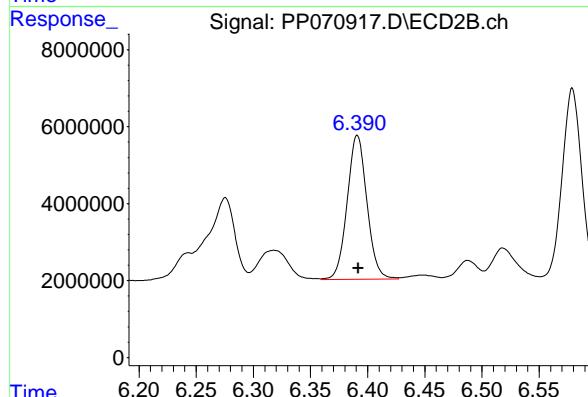


#32 AR-1260-2

R.T.: 7.512 min  
 Delta R.T.: 0.002 min  
 Response: 90805769 ECD\_P  
 Conc: 928.40 ng/ml ClientSampleId : AR1660ICC1000

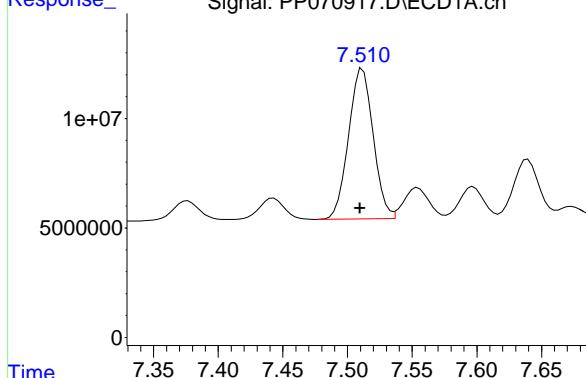


#32 AR-1260-2

R.T.: 6.579 min  
 Delta R.T.: 0.000 min  
 Response: 58475471  
 Conc: 929.60 ng/ml

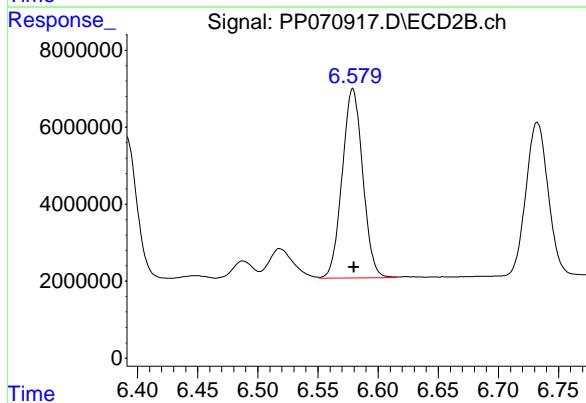


#33 AR-1260-3




R.T.: 7.870 min  
 Delta R.T.: 0.002 min  
 Response: 75946924  
 Conc: 915.35 ng/ml

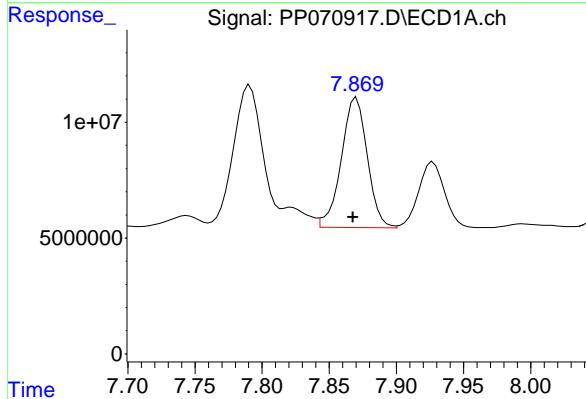

#33 AR-1260-3

R.T.: 6.732 min  
 Delta R.T.: -0.001 min  
 Response: 50913622  
 Conc: 944.23 ng/ml

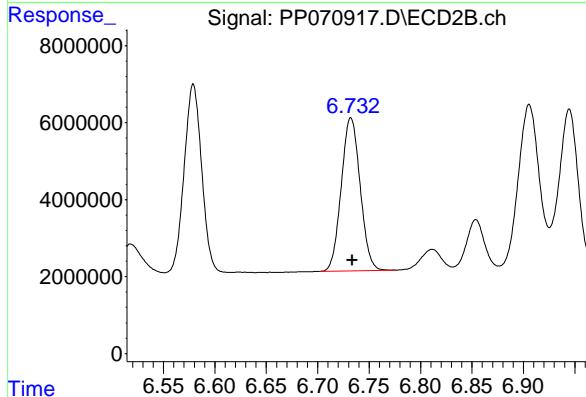

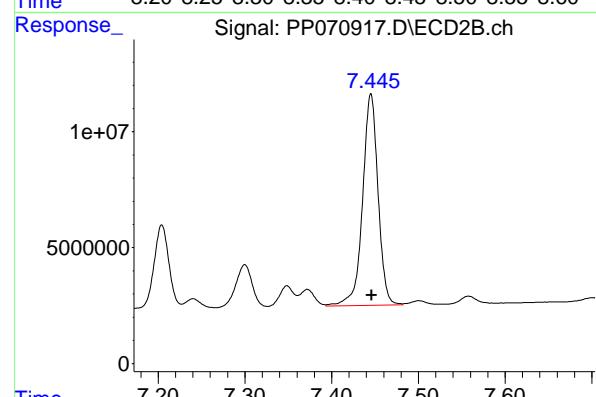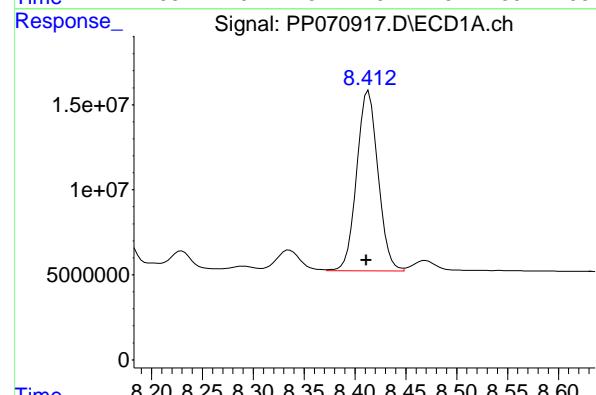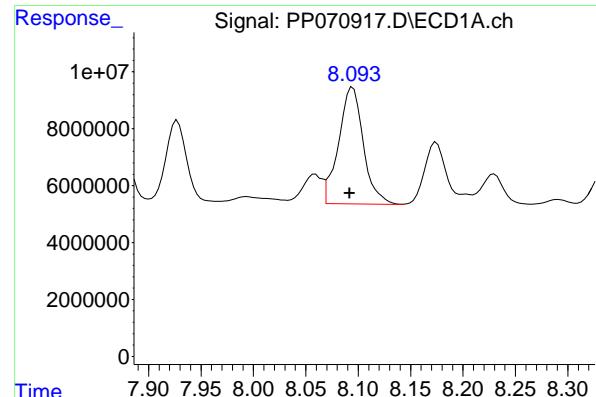

#34 AR-1260-4

R.T.: 8.095 min  
 Delta R.T.: 0.003 min  
 Response: 67190656 ClientSampleId :  
 Conc: 824.92 ng/ml AR1660ICC1000

#34 AR-1260-4

R.T.: 7.204 min  
 Delta R.T.: 0.000 min  
 Response: 42366044  
 Conc: 892.13 ng/ml

#35 AR-1260-5

R.T.: 8.413 min  
 Delta R.T.: 0.002 min  
 Response: 154592706  
 Conc: 966.44 ng/ml

#35 AR-1260-5

R.T.: 7.445 min  
 Delta R.T.: 0.000 min  
 Response: 113066934  
 Conc: 902.28 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070918.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 10:47  
 Operator : YP\AJ  
 Sample : AR1660ICC750  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 11:43:22 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.516	3.816	109.6E6	76743418	72.145	74.023
2) SA Decachloro...	10.232	8.858	79929815	63467739	71.593	73.372

**Target Compounds**

3) L1 AR-1016-1	5.668	4.903	36878765	28246340	724.049	744.189
4) L1 AR-1016-2	5.690	4.922	55926362	40045379	709.625	736.388
5) L1 AR-1016-3	5.752	5.098	33032965	22299566	705.593	747.078
6) L1 AR-1016-4	5.850	5.140	27452141	17599061	703.632	739.649
7) L1 AR-1016-5	6.142	5.355	25115726	22419832	716.759	743.502
31) L7 AR-1260-1	7.261	6.391	46678805	34889457	698.534	723.240
32) L7 AR-1260-2	7.514	6.578	71623177	45945144	732.278	730.401
33) L7 AR-1260-3	7.873	6.732	59218079	39234472	713.723	727.634
34) L7 AR-1260-4	8.097	7.203	56265266	33296646	690.783	701.150
35) L7 AR-1260-5	8.417	7.444	117.1E6	87479828	731.936	698.092



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070918.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 10:47  
 Operator : YP\AJ  
 Sample : AR1660ICC750  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 11:43:22 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

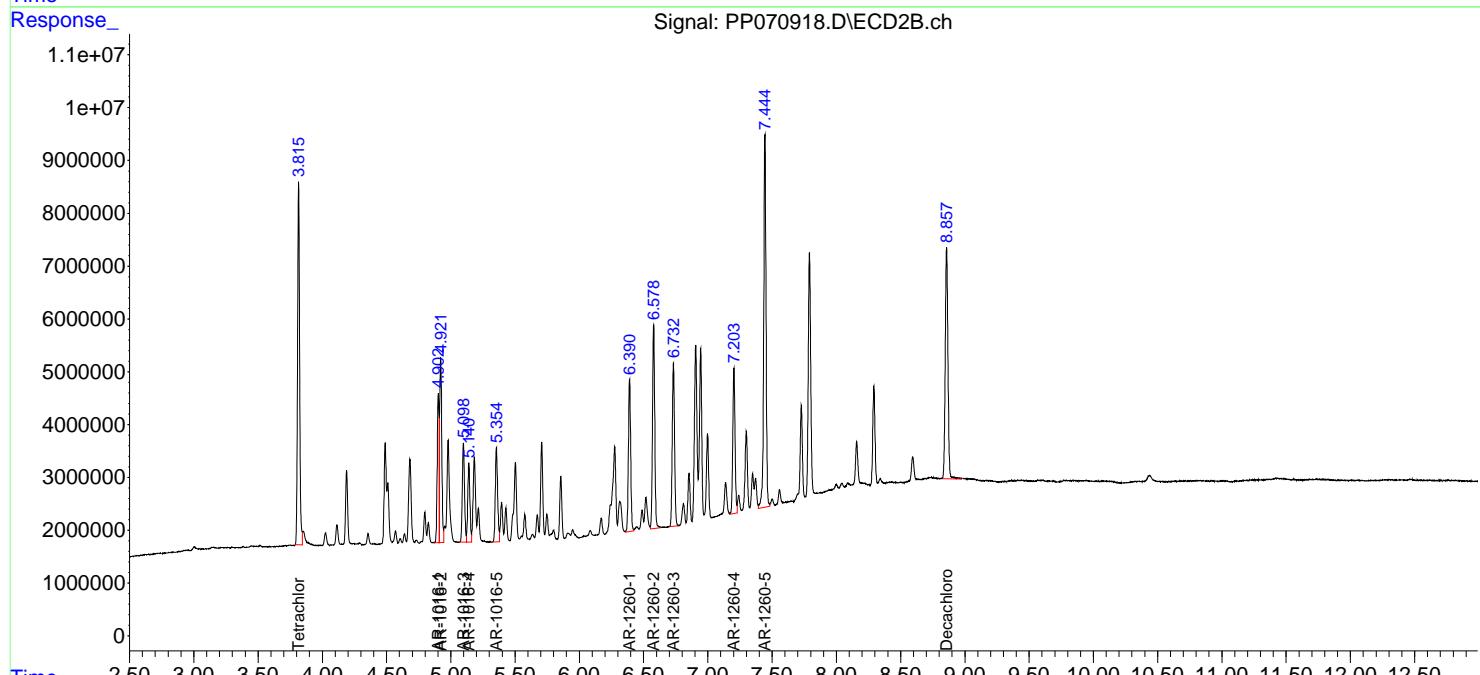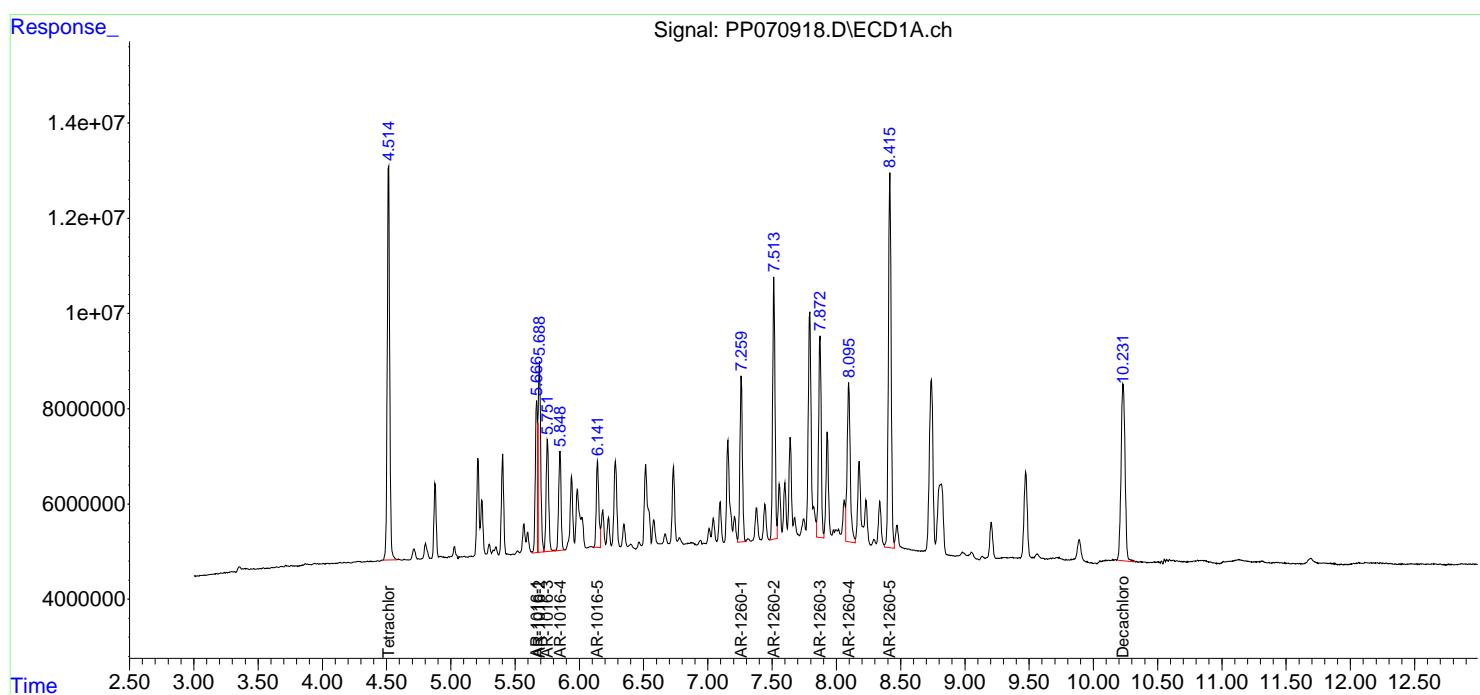

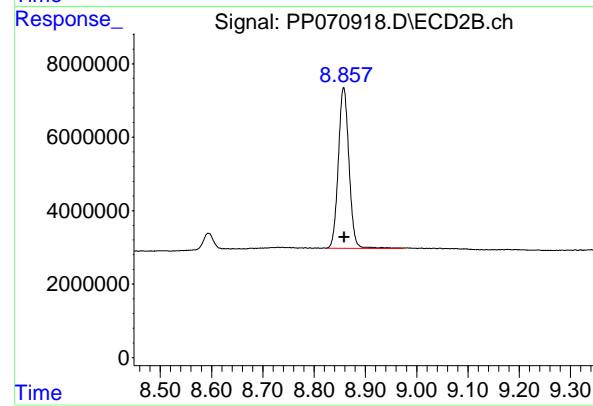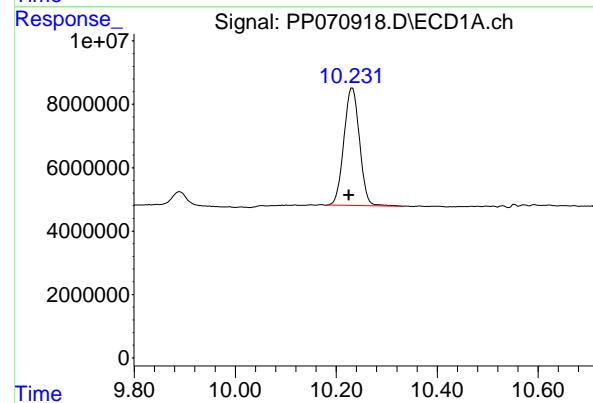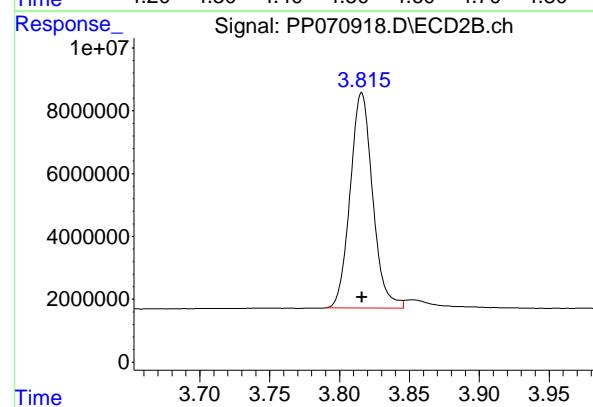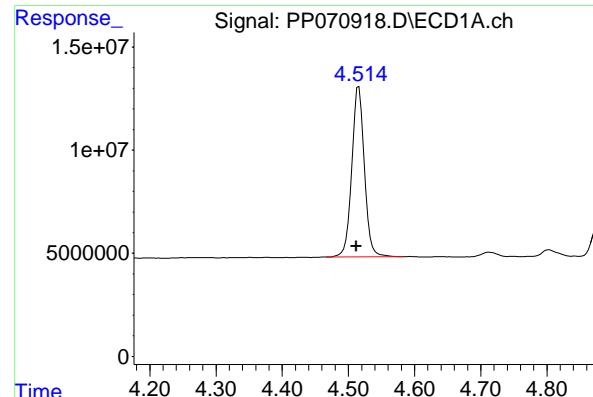

## #1 Tetrachloro-m-xylene

R.T.: 4.516 min  
Delta R.T.: 0.004 min  
Instrument: ECD\_P  
Response: 109605429  
Conc: 72.14 ng/ml ClientSampleId : AR1660ICC750

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 76743418  
Conc: 74.02 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.232 min  
Delta R.T.: 0.007 min  
Response: 79929815  
Conc: 71.59 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.858 min  
Delta R.T.: -0.001 min  
Response: 63467739  
Conc: 73.37 ng/ml

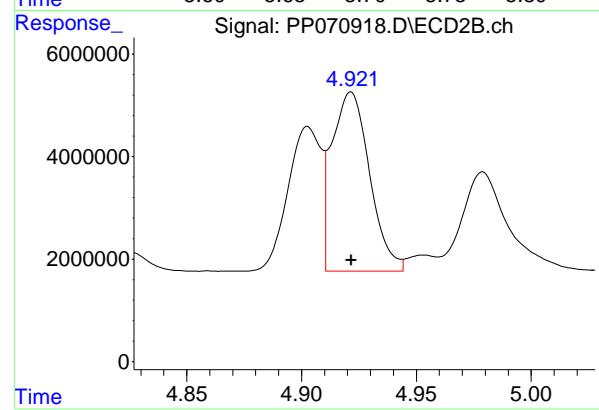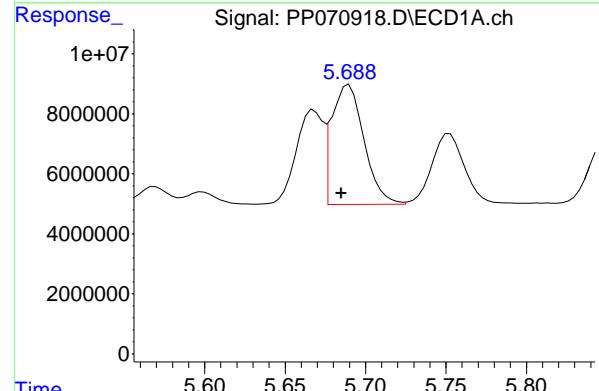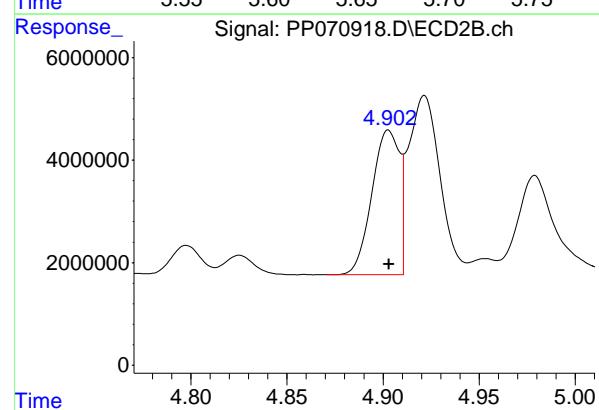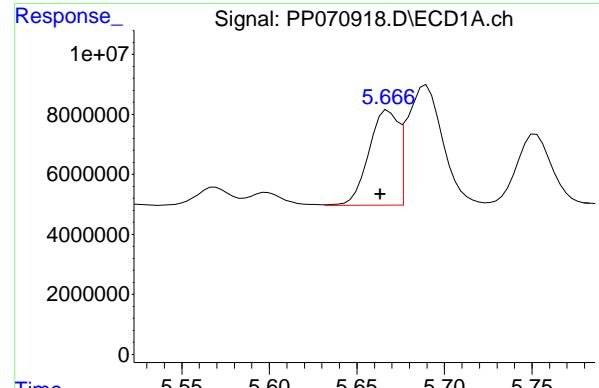

#3 AR-1016-1

R.T.: 5.668 min  
 Delta R.T.: 0.005 min  
 Response: 36878765  
 Conc: 724.05 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC750

#3 AR-1016-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 28246340  
 Conc: 744.19 ng/ml

#4 AR-1016-2


R.T.: 5.690 min  
 Delta R.T.: 0.005 min  
 Response: 55926362  
 Conc: 709.62 ng/ml

#4 AR-1016-2

R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 40045379  
 Conc: 736.39 ng/ml


#5 AR-1016-3

R.T.: 5.752 min  
 Delta R.T.: 0.005 min  
 Response: 33032965  
 Conc: 705.59 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** AR1660ICC750

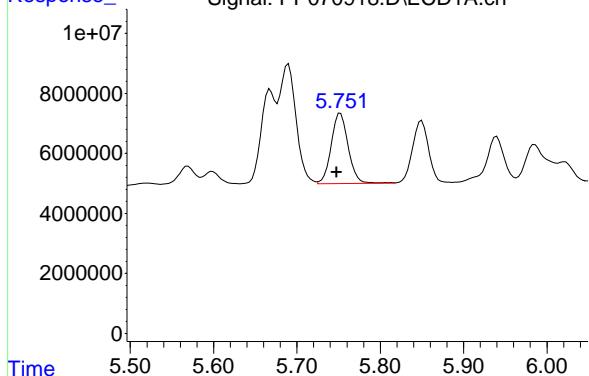


#5 AR-1016-3

R.T.: 5.098 min  
 Delta R.T.: 0.000 min  
 Response: 22299566  
 Conc: 747.08 ng/ml

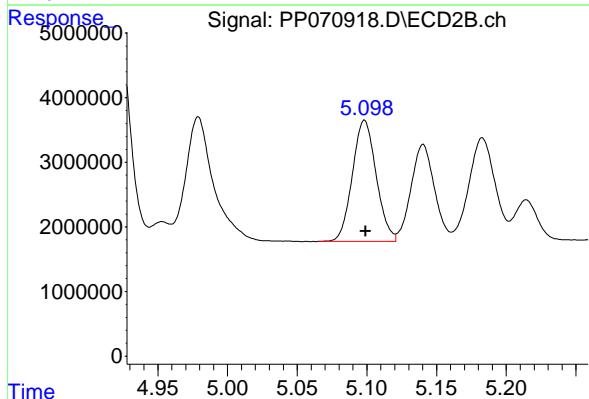


#6 AR-1016-4

R.T.: 5.850 min  
 Delta R.T.: 0.005 min  
 Response: 27452141  
 Conc: 703.63 ng/ml

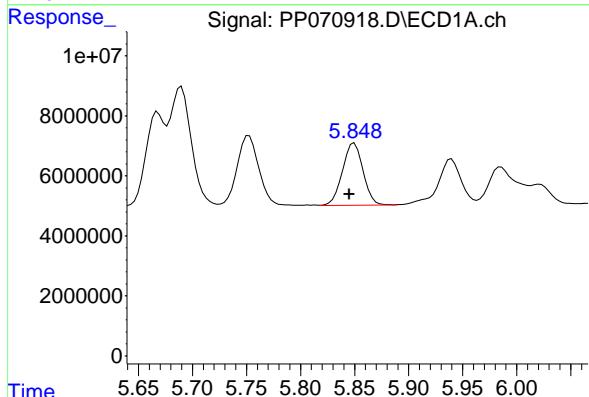


#6 AR-1016-4

R.T.: 5.140 min  
 Delta R.T.: 0.000 min  
 Response: 17599061  
 Conc: 739.65 ng/ml

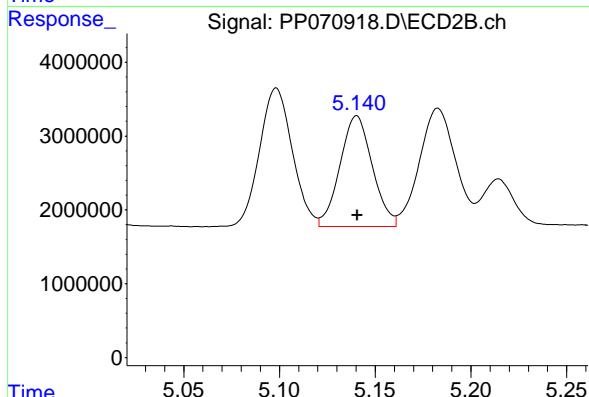


#7 AR-1016-5

R.T.: 6.142 min  
 Delta R.T.: 0.004 min  
 Response: 25115726 ECD\_P  
 Conc: 716.76 ng/ml ClientSampleId : AR1660ICC750

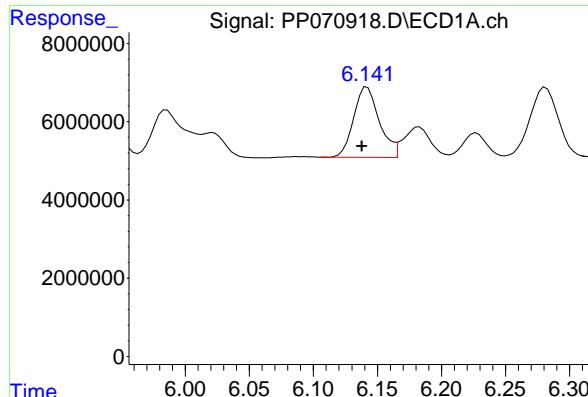


#7 AR-1016-5

R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 22419832  
 Conc: 743.50 ng/ml

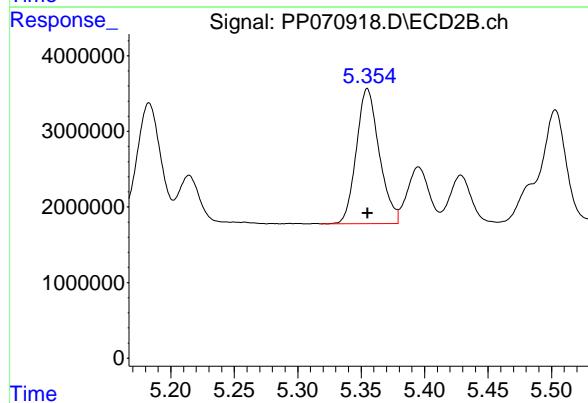


#31 AR-1260-1

R.T.: 7.261 min  
 Delta R.T.: 0.005 min  
 Response: 46678805  
 Conc: 698.53 ng/ml

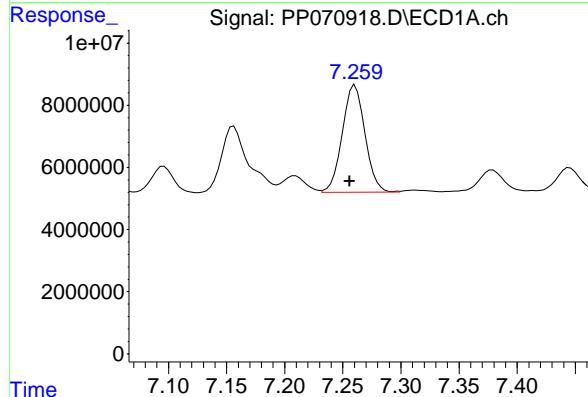


#31 AR-1260-1

R.T.: 6.391 min  
 Delta R.T.: 0.000 min  
 Response: 34889457  
 Conc: 723.24 ng/ml

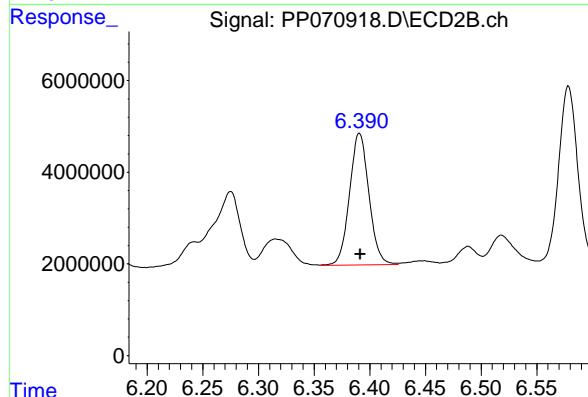


#32 AR-1260-2

R.T.: 7.514 min  
 Delta R.T.: 0.005 min  
 Response: 71623177 ECD\_P  
 Conc: 732.28 ng/ml ClientSampleId : AR1660ICC750

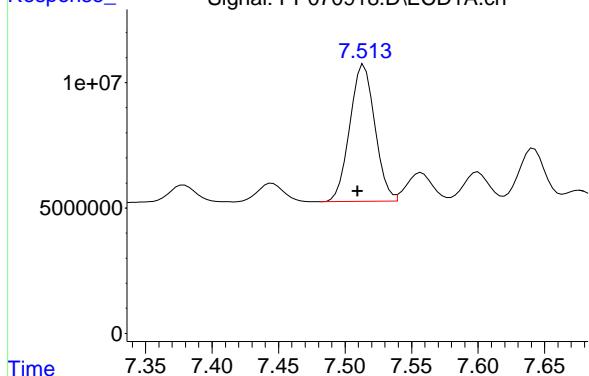

#32 AR-1260-2

R.T.: 6.578 min  
 Delta R.T.: -0.001 min  
 Response: 45945144  
 Conc: 730.40 ng/ml




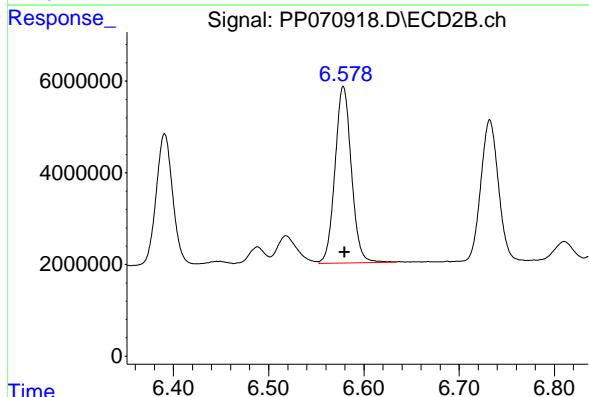


#33 AR-1260-3

R.T.: 7.873 min  
 Delta R.T.: 0.005 min  
 Response: 59218079  
 Conc: 713.72 ng/ml

#33 AR-1260-3

R.T.: 6.732 min  
 Delta R.T.: -0.001 min  
 Response: 39234472  
 Conc: 727.63 ng/ml

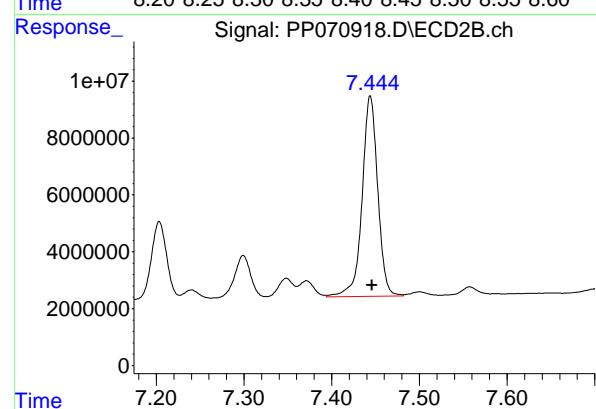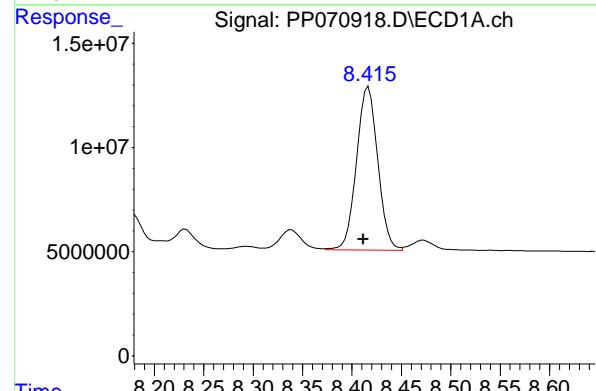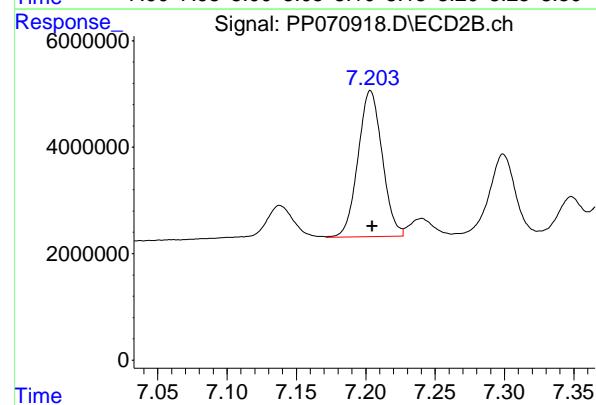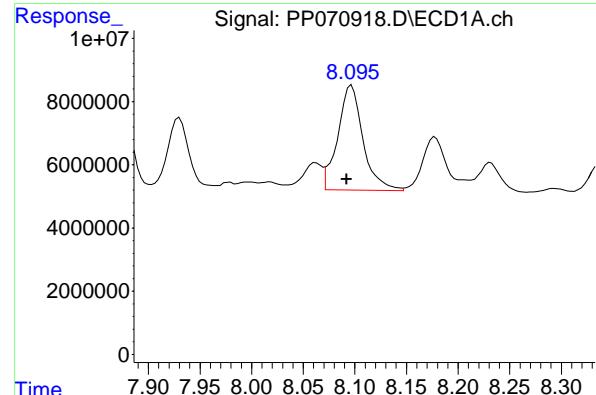

#34 AR-1260-4

R.T.: 8.097 min  
 Delta R.T.: 0.005 min  
 Response: 56265266 ECD\_P  
 Conc: 690.78 ng/ml ClientSampleId : AR1660ICC750

#34 AR-1260-4

R.T.: 7.203 min  
 Delta R.T.: -0.001 min  
 Response: 33296646  
 Conc: 701.15 ng/ml

#35 AR-1260-5

R.T.: 8.417 min  
 Delta R.T.: 0.005 min  
 Response: 117081076  
 Conc: 731.94 ng/ml

#35 AR-1260-5

R.T.: 7.444 min  
 Delta R.T.: -0.002 min  
 Response: 87479828  
 Conc: 698.09 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070919.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:03  
 Operator : YP\AJ  
 Sample : AR1660ICC500  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 11:43:35 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.512	3.816	75962416	51837404	50.000	50.000
2) SA Decachloro...	10.225	8.859	55822450	43250808	50.000	50.000

**Target Compounds**

3) L1 AR-1016-1	5.663	4.903	25467030	18977943	500.000	500.000
4) L1 AR-1016-2	5.685	4.922	39405586	27190389	500.000	500.000
5) L1 AR-1016-3	5.748	5.099	23407932	14924529	500.000	500.000
6) L1 AR-1016-4	5.845	5.141	19507464	11896894	500.000	500.000
7) L1 AR-1016-5	6.138	5.355	17520341	15077187	500.000	500.000
31) L7 AR-1260-1	7.256	6.392	33411980	24120261	500.000	500.000
32) L7 AR-1260-2	7.510	6.580	48904355	31452019	500.000	500.000
33) L7 AR-1260-3	7.868	6.734	41485326	26960319	500.000	500.000
34) L7 AR-1260-4	8.092	7.205	40725714	23744314	500.000	500.000
35) L7 AR-1260-5	8.411	7.446	79980400	62656405	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070919.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:03  
 Operator : YP\AJ  
 Sample : AR1660ICC500  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 11:43:35 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1      Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

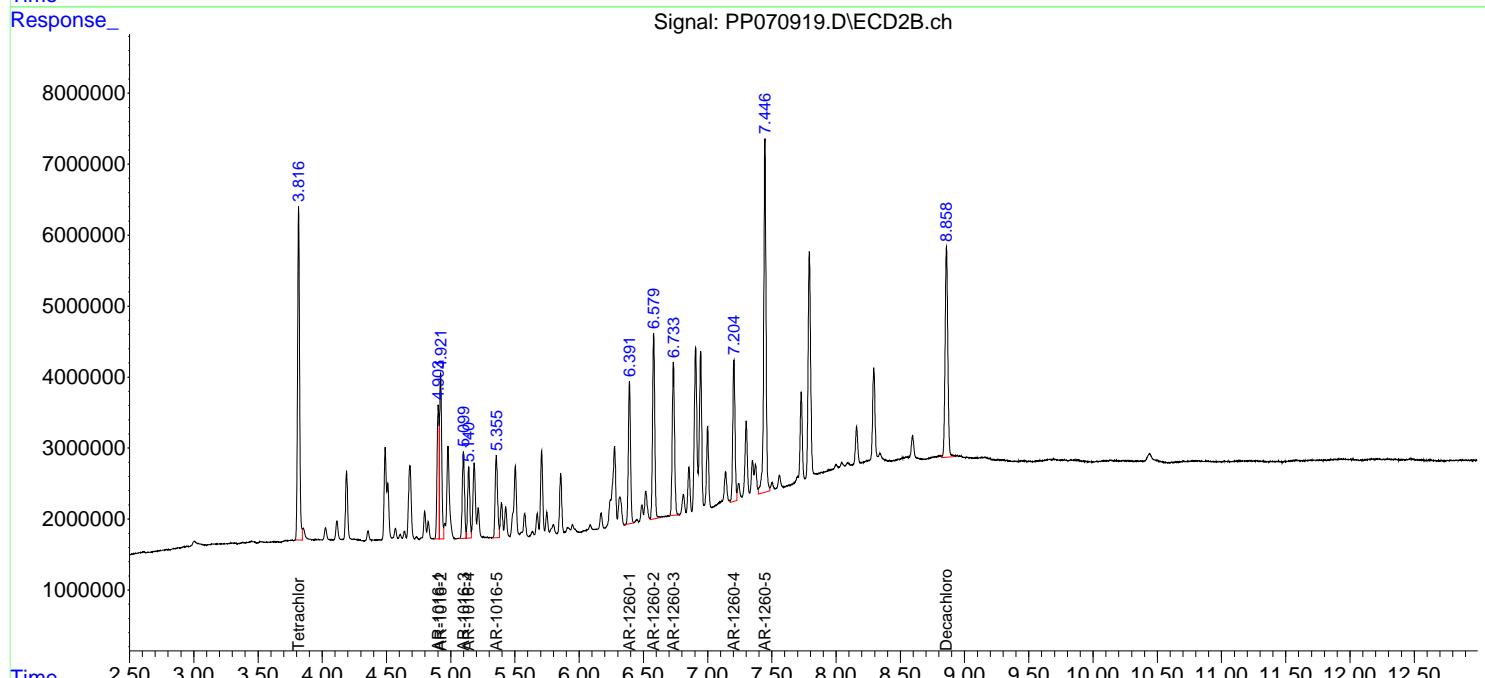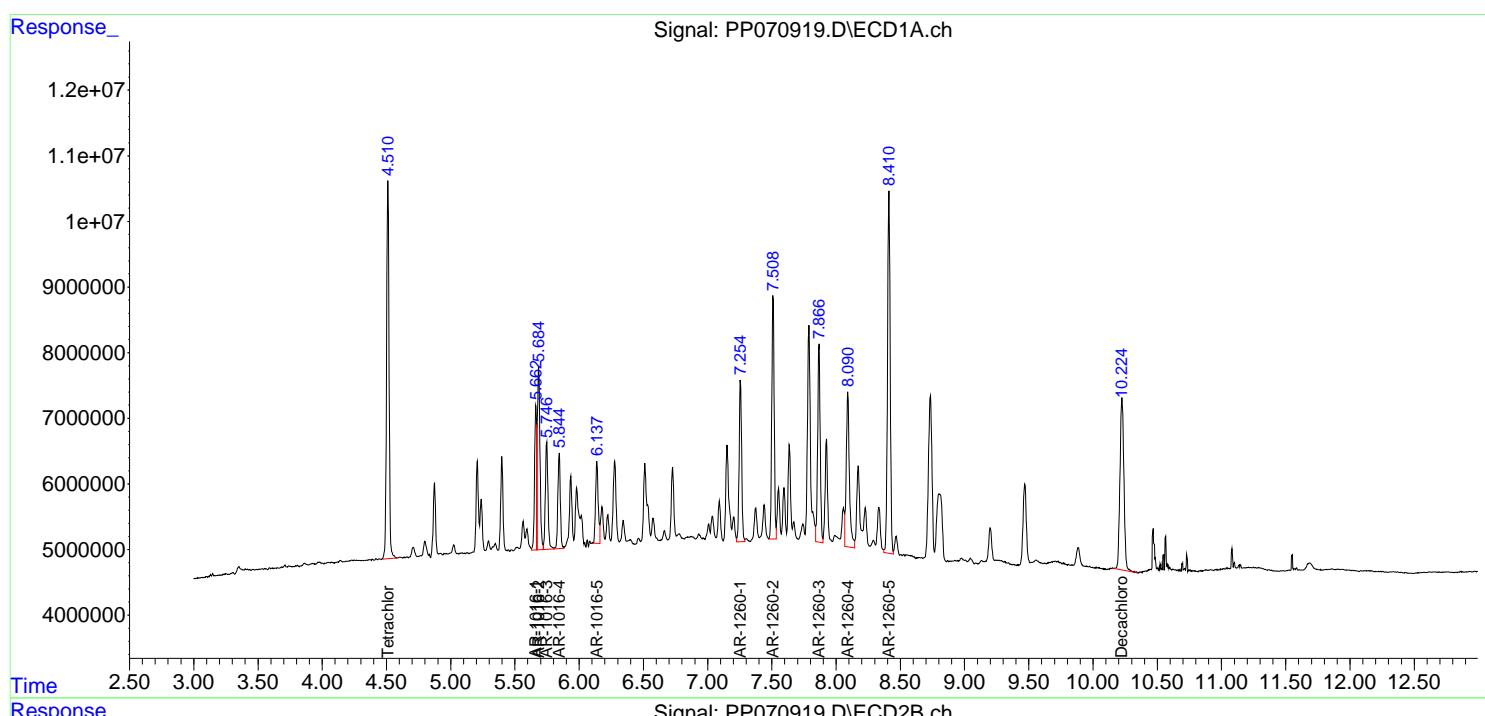

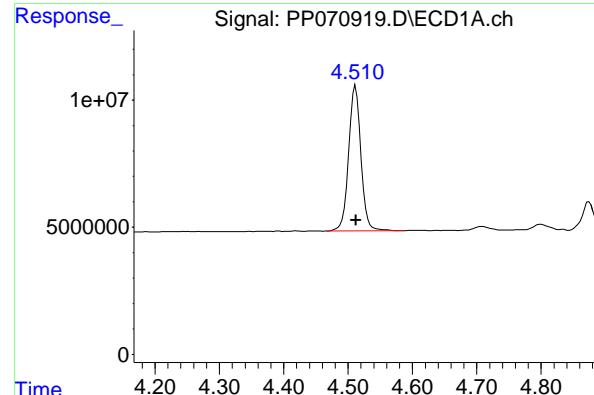


## #1 Tetrachloro-m-xylene

R.T.: 4.512 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 75962416  
Conc: 50.00 ng/ml ClientSampleId : AR1660ICC500

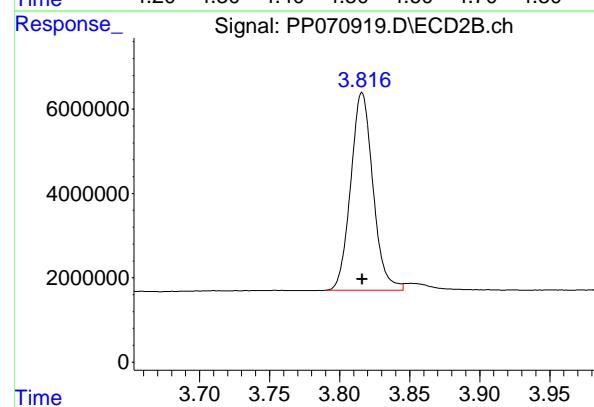


## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 51837404  
Conc: 50.00 ng/ml

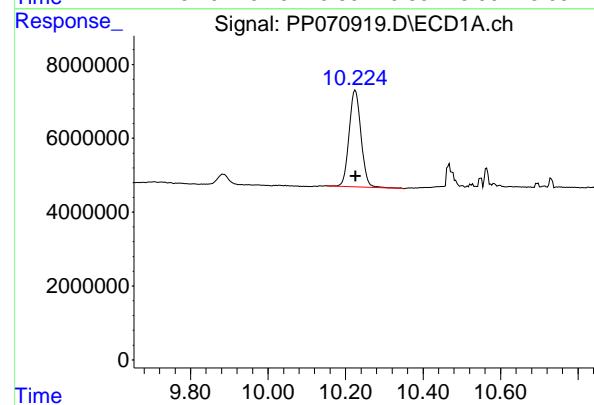





## #2 Decachlorobiphenyl

R.T.: 10.225 min  
Delta R.T.: 0.000 min  
Response: 55822450  
Conc: 50.00 ng/ml

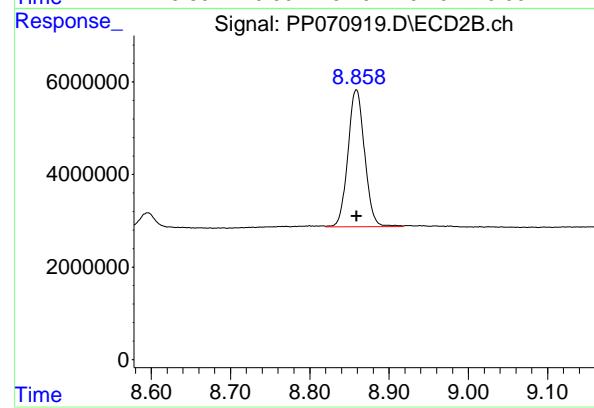

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 43250808  
Conc: 50.00 ng/ml

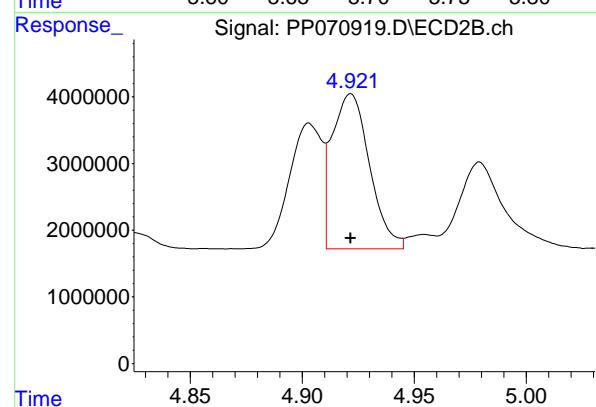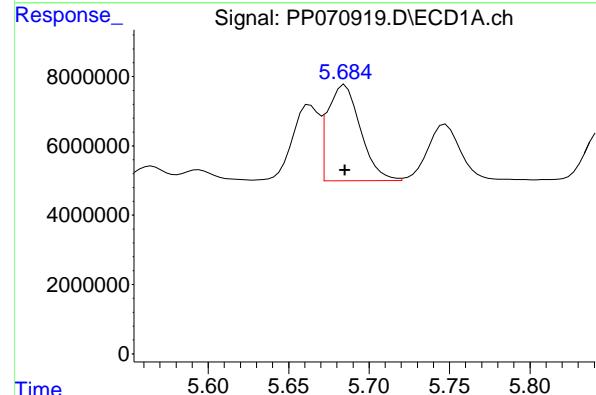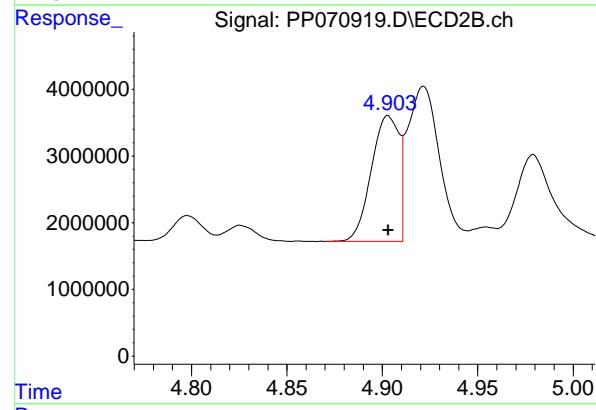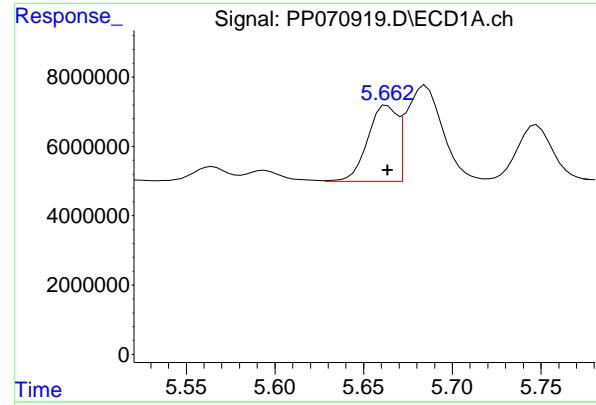

#3 AR-1016-1

R.T.: 5.663 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_P  
 Response: 25467030  
 Conc: 500.00 ng/ml  
 ClientSampleId: AR1660ICC500

#3 AR-1016-1





R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 18977943  
 Conc: 500.00 ng/ml

#4 AR-1016-2

R.T.: 5.685 min  
 Delta R.T.: 0.000 min  
 Response: 39405586  
 Conc: 500.00 ng/ml

#4 AR-1016-2

R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 27190389  
 Conc: 500.00 ng/ml

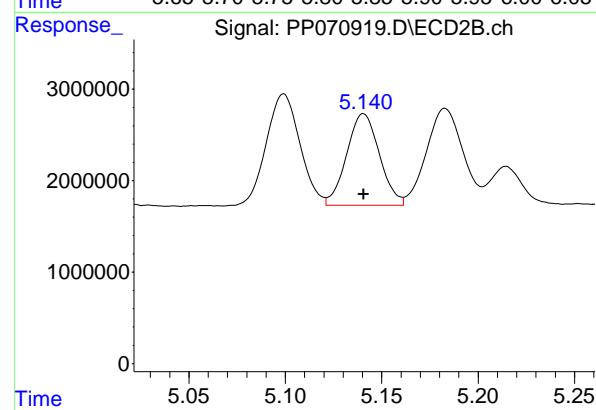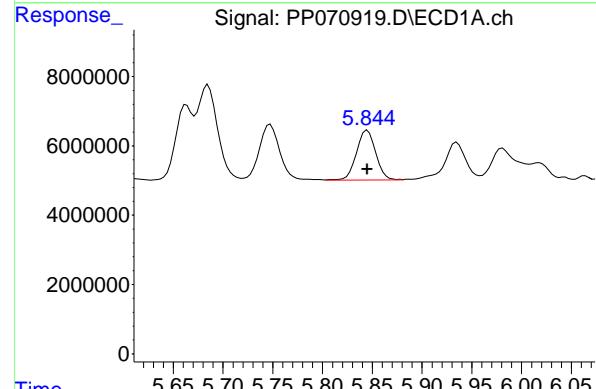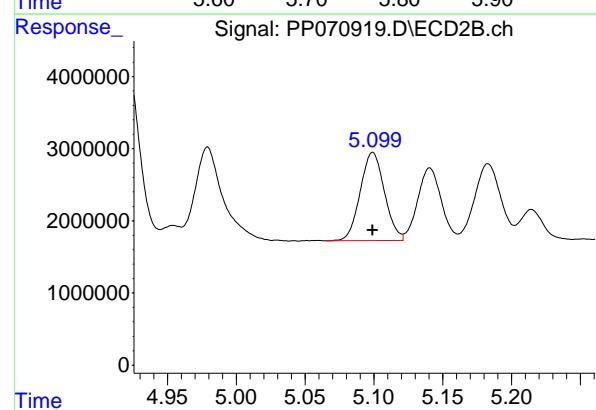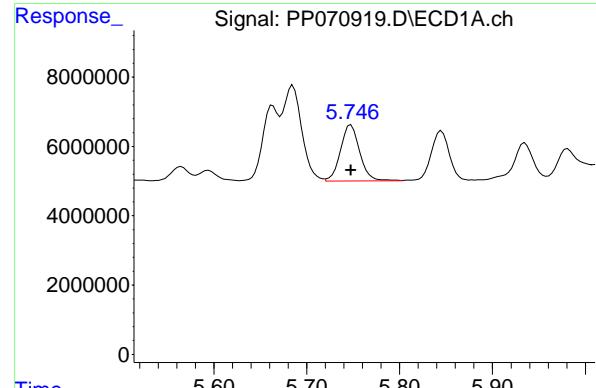

#5 AR-1016-3

R.T.: 5.748 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 23407932  
Conc: 500.00 ng/ml  
ClientSampleId : AR1660ICC500

#5 AR-1016-3


R.T.: 5.099 min  
Delta R.T.: 0.000 min  
Response: 14924529  
Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 5.845 min  
Delta R.T.: 0.000 min  
Response: 19507464  
Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 5.141 min  
Delta R.T.: 0.000 min  
Response: 11896894  
Conc: 500.00 ng/ml

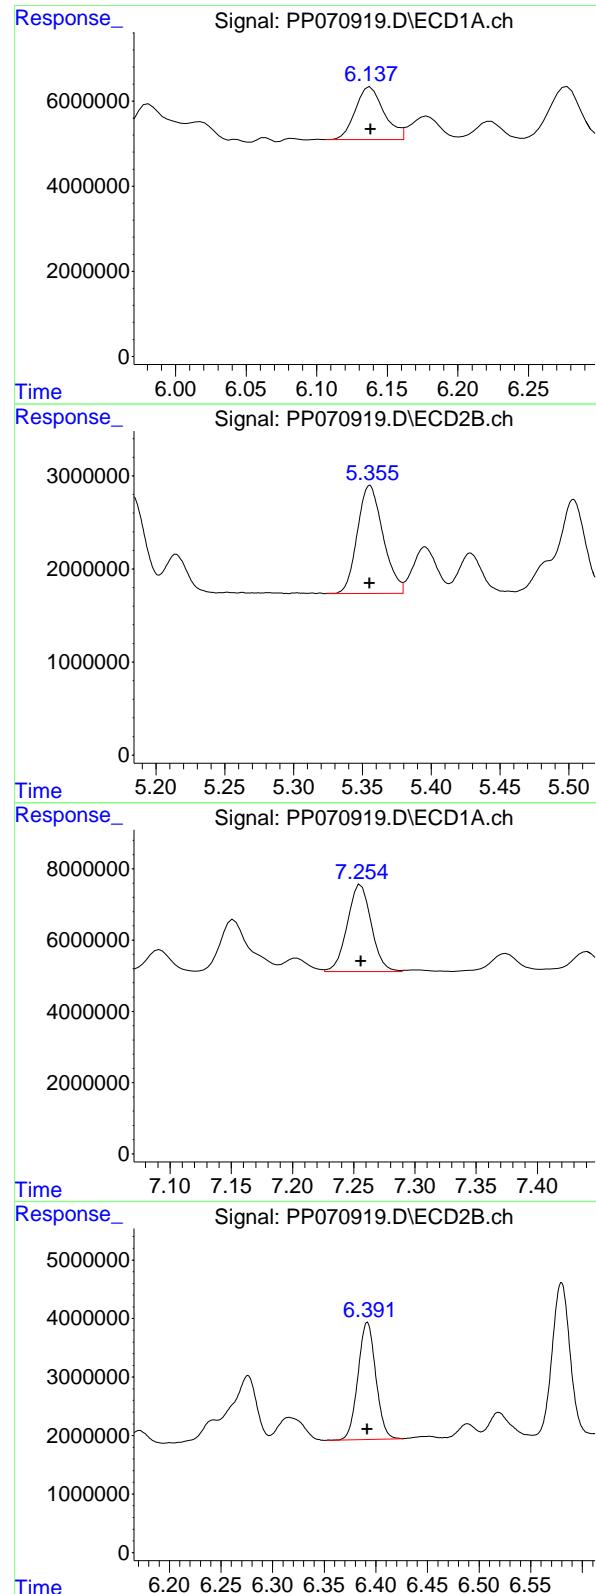

#7 AR-1016-5

R.T.: 6.138 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_P  
 Response: 17520341  
 Conc: 500.00 ng/ml  
 ClientSampleId : AR1660ICC500

#7 AR-1016-5


R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 15077187  
 Conc: 500.00 ng/ml

#31 AR-1260-1

R.T.: 7.256 min  
 Delta R.T.: 0.000 min  
 Response: 33411980  
 Conc: 500.00 ng/ml

#31 AR-1260-1

R.T.: 6.392 min  
 Delta R.T.: 0.000 min  
 Response: 24120261  
 Conc: 500.00 ng/ml

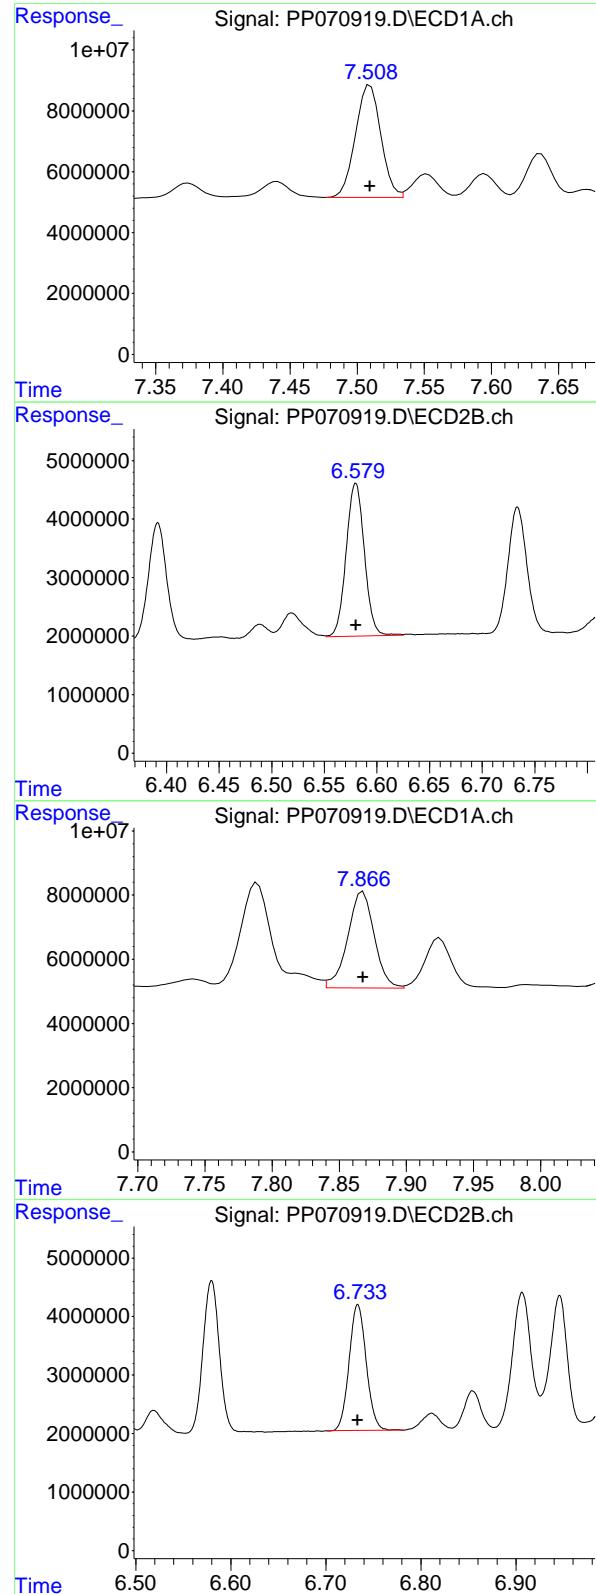

#32 AR-1260-2

R.T.: 7.510 min  
 Delta R.T.: 0.000 min  
 Response: 48904355  
 Conc: 500.00 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** AR1660ICC500

#32 AR-1260-2





R.T.: 6.580 min  
 Delta R.T.: 0.000 min  
 Response: 31452019  
 Conc: 500.00 ng/ml

#33 AR-1260-3

R.T.: 7.868 min  
 Delta R.T.: 0.000 min  
 Response: 41485326  
 Conc: 500.00 ng/ml

#33 AR-1260-3

R.T.: 6.734 min  
 Delta R.T.: 0.000 min  
 Response: 26960319  
 Conc: 500.00 ng/ml

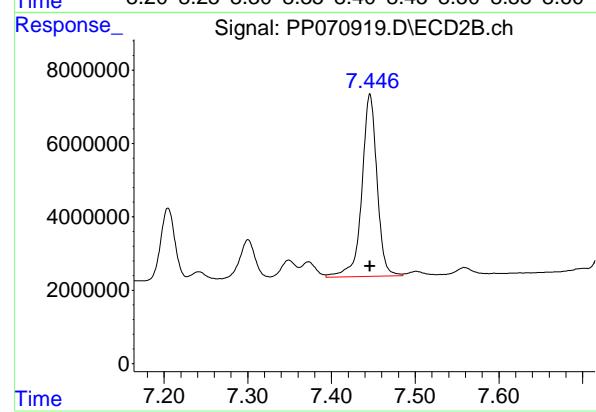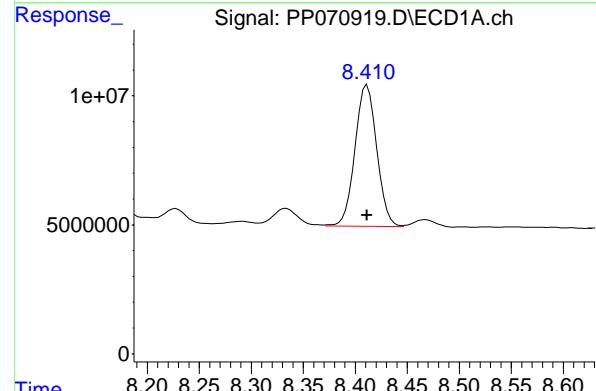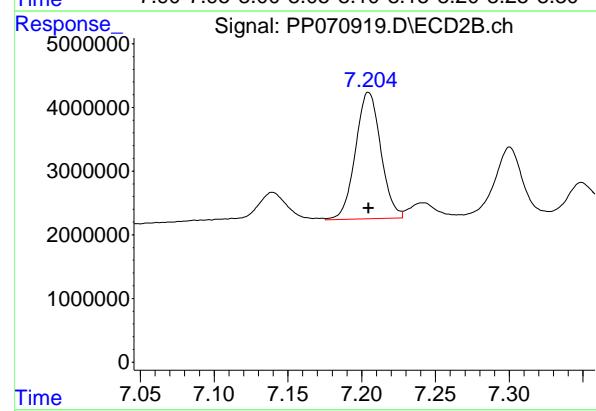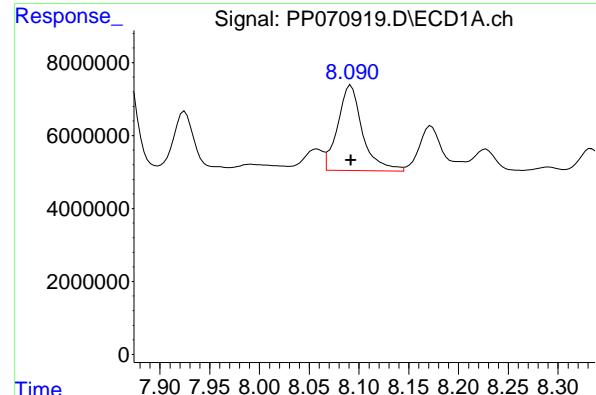

#34 AR-1260-4

R.T.: 8.092 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_P  
 Response: 40725714  
 Conc: 500.00 ng/ml  
 ClientSampleId : AR1660ICC500

#34 AR-1260-4

R.T.: 7.205 min  
 Delta R.T.: 0.000 min  
 Response: 23744314  
 Conc: 500.00 ng/ml

#35 AR-1260-5

R.T.: 8.411 min  
 Delta R.T.: 0.000 min  
 Response: 79980400  
 Conc: 500.00 ng/ml

#35 AR-1260-5

R.T.: 7.446 min  
 Delta R.T.: 0.000 min  
 Response: 62656405  
 Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:19  
 Operator : YP\AJ  
 Sample : AR1660ICC250  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1660ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:11:10 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.515	3.816	39892911	28120307	26.258	27.124
2) SA Decachloro...	10.229	8.859	27877719	18839232	24.970	21.779

**Target Compounds**

3) L1 AR-1016-1	5.667	4.903	13581167	11323714	266.642	298.339
4) L1 AR-1016-2	5.689	4.922	20108471	16375760	255.147	301.131
5) L1 AR-1016-3	5.751	5.099	12212490	8877034	260.862	297.397
6) L1 AR-1016-4	5.848	5.141	9803037	7158830	251.264	300.870
7) L1 AR-1016-5	6.141	5.355	9152735	9323046	261.203	309.177
31) L7 AR-1260-1	7.260	6.391	18182257	14056672	272.092	291.387
32) L7 AR-1260-2	7.513	6.579	25714746	17295947	262.909	274.958
33) L7 AR-1260-3	7.870	6.733	21528554	14684885	259.472m	272.343
34) L7 AR-1260-4	8.094	7.205	19536409	12488782	239.853m	262.985
35) L7 AR-1260-5	8.414	7.446	41714322	31815782	260.778m	253.891

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:19  
 Operator : YP\AJ  
 Sample : AR1660ICC250  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1



Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1660ICC250





**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:11:10 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

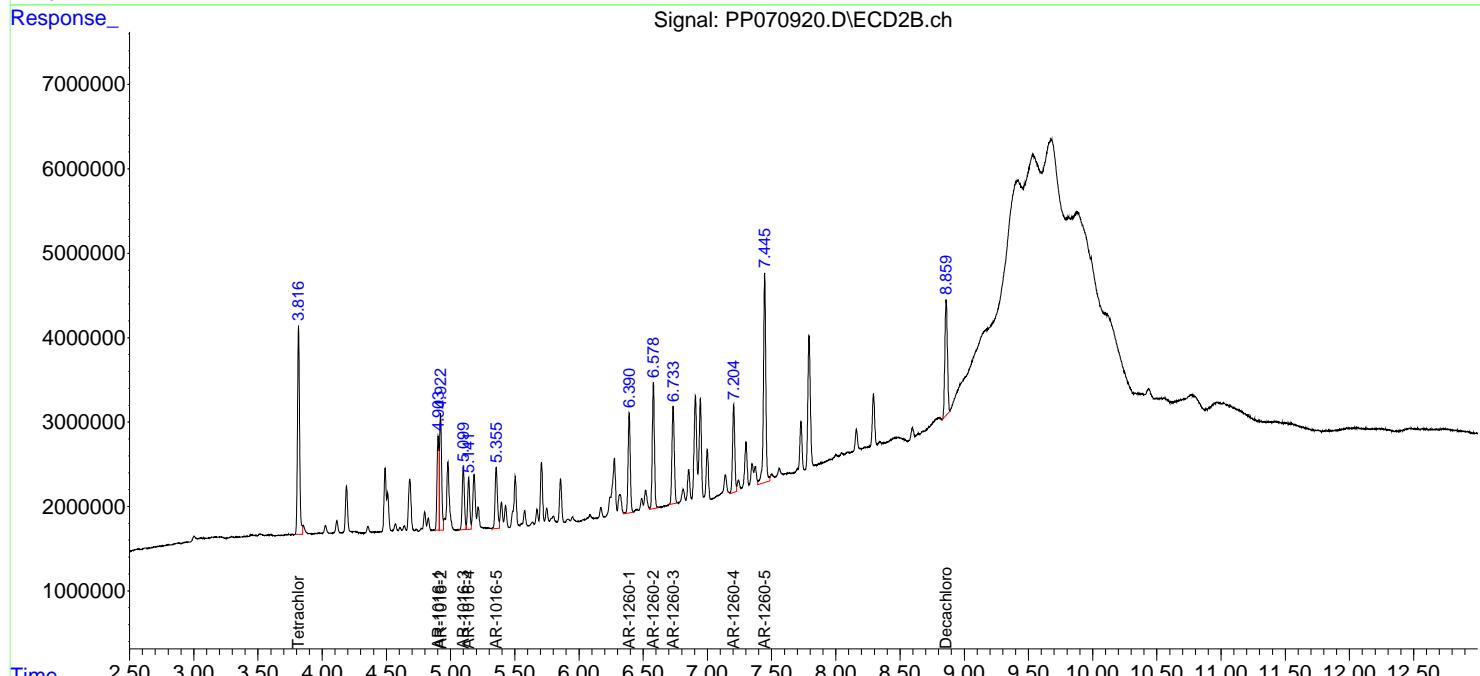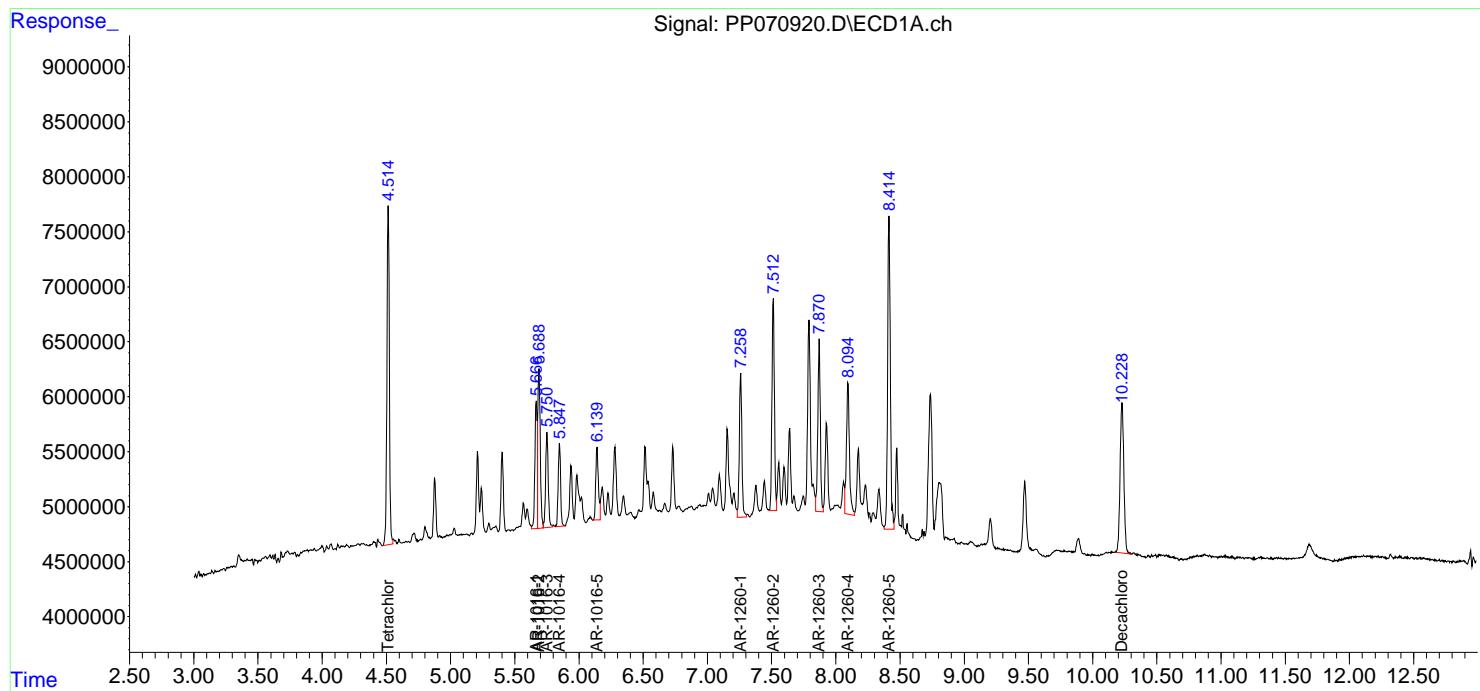

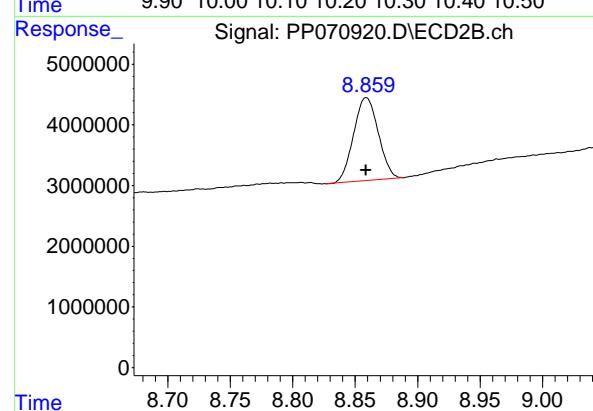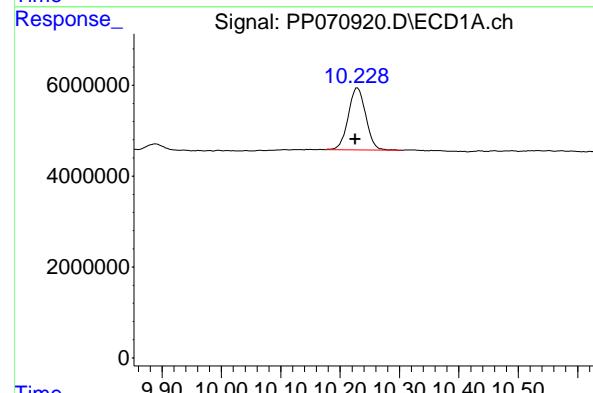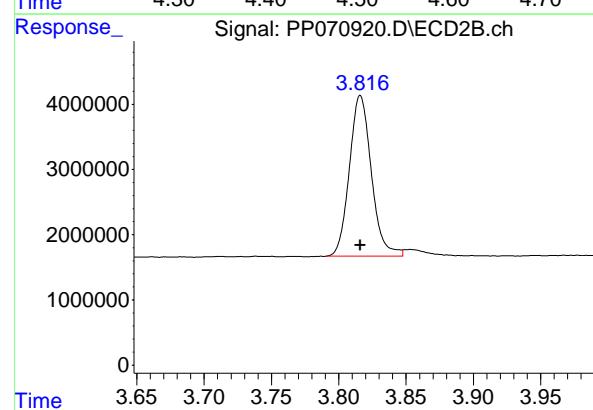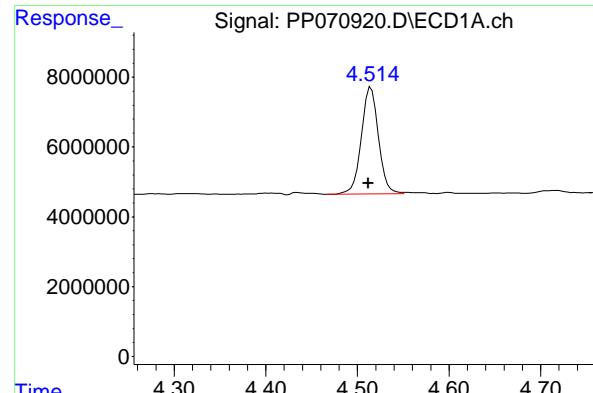

## #1 Tetrachloro-m-xylene

R.T.: 4.515 min  
 Delta R.T.: 0.003 min  
 Response: 39892911  
 Conc: 26.26 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1660ICC250

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 28120307  
 Conc: 27.12 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.229 min  
 Delta R.T.: 0.004 min  
 Response: 27877719  
 Conc: 24.97 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 18839232  
 Conc: 21.78 ng/ml

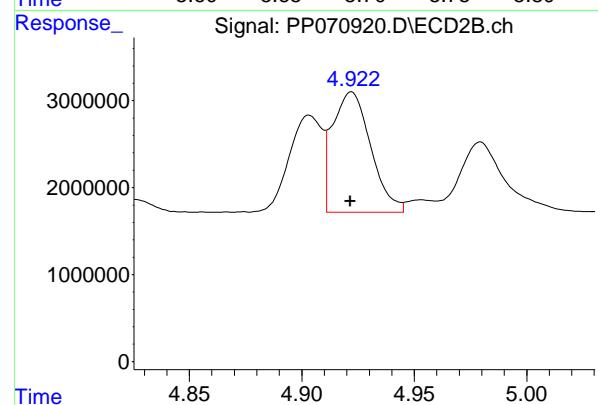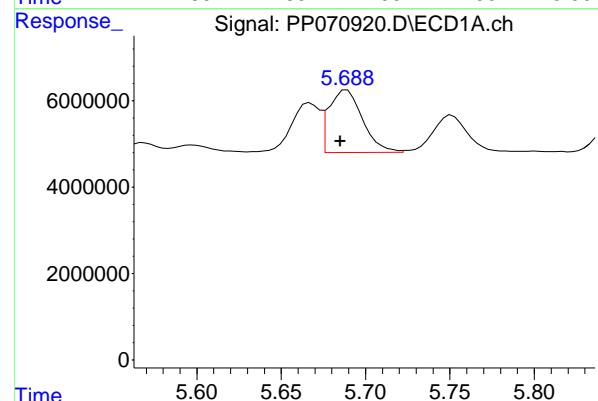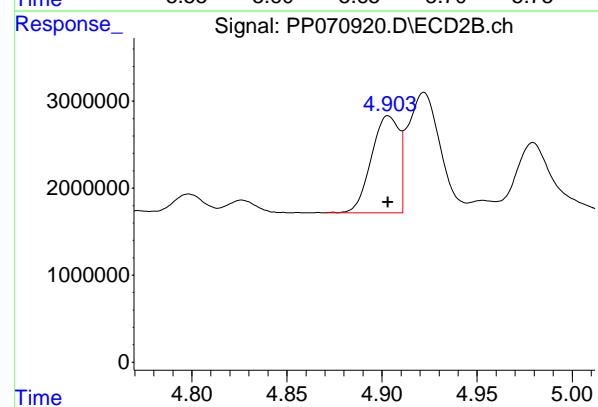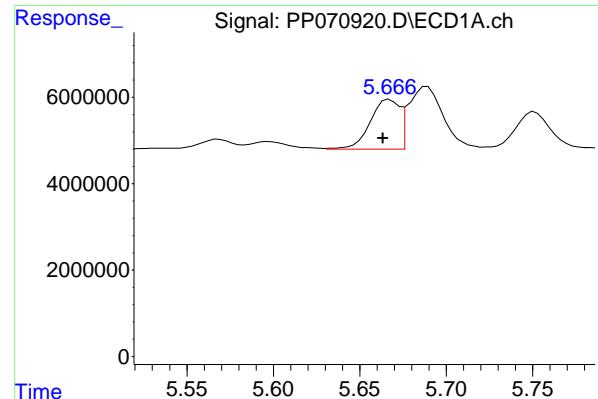

#3 AR-1016-1

R.T.: 5.667 min  
 Delta R.T.: 0.004 min  
 Response: 13581167  
 Conc: 266.64 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1660ICC250

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#3 AR-1016-1





R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 11323714  
 Conc: 298.34 ng/ml

#4 AR-1016-2

R.T.: 5.689 min  
 Delta R.T.: 0.004 min  
 Response: 20108471  
 Conc: 255.15 ng/ml

#4 AR-1016-2

R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 16375760  
 Conc: 301.13 ng/ml

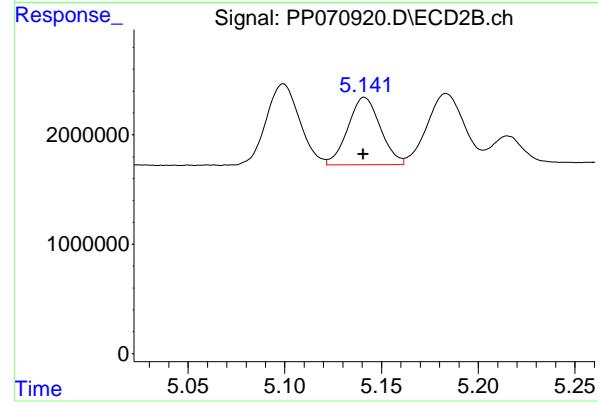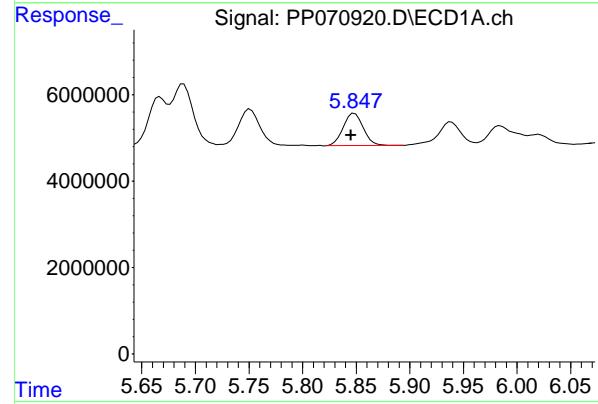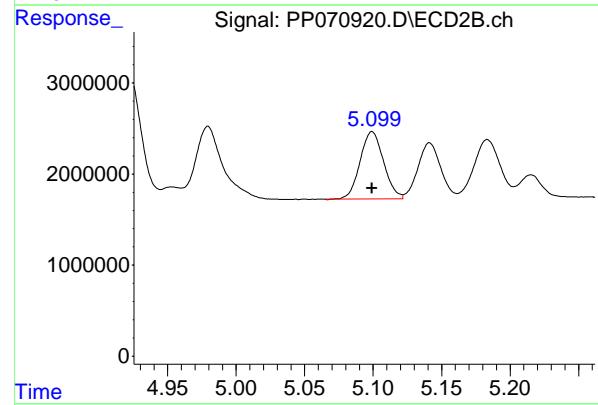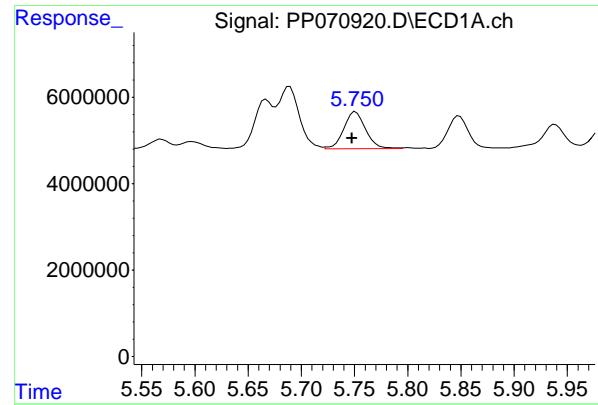

#5 AR-1016-3

R.T.: 5.751 min  
 Delta R.T.: 0.004 min  
 Response: 12212490 ECD\_P  
 Conc: 260.86 ng/ml Client SampleId : AR1660ICC250

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#5 AR-1016-3





R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 8877034  
 Conc: 297.40 ng/ml

#6 AR-1016-4

R.T.: 5.848 min  
 Delta R.T.: 0.003 min  
 Response: 9803037  
 Conc: 251.26 ng/ml

#6 AR-1016-4

R.T.: 5.141 min  
 Delta R.T.: 0.000 min  
 Response: 7158830  
 Conc: 300.87 ng/ml

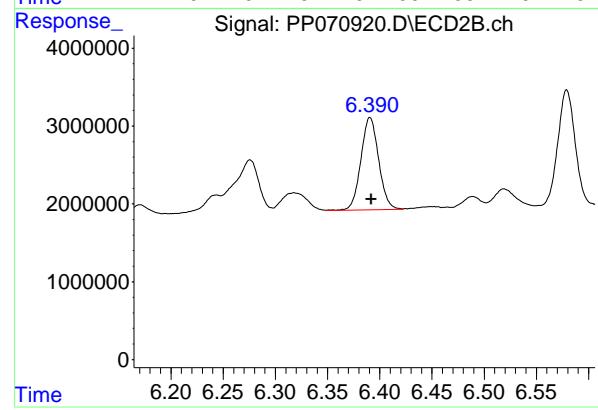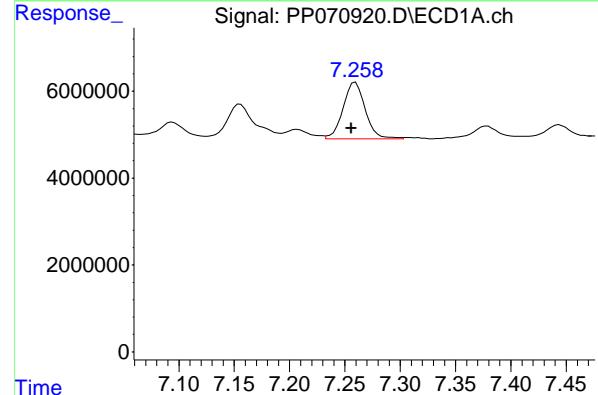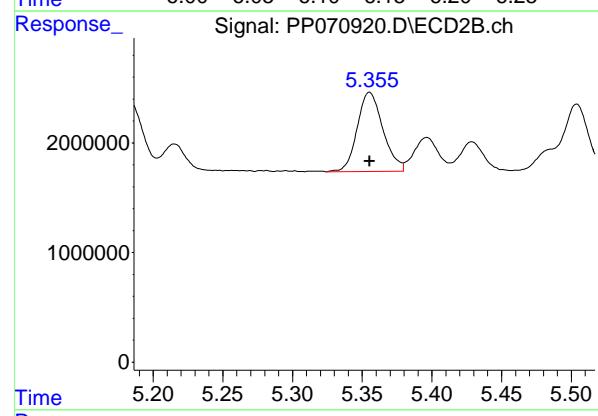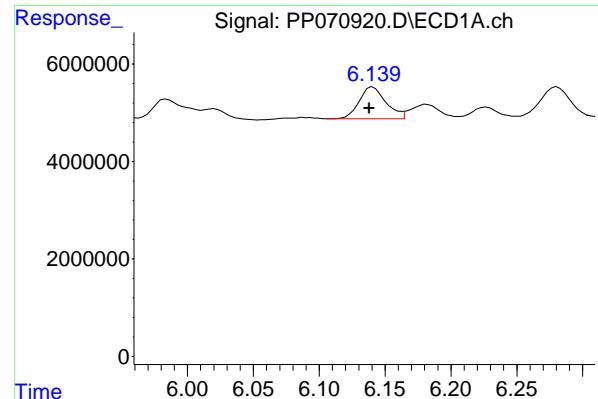

#7 AR-1016-5

R.T.: 6.141 min  
 Delta R.T.: 0.003 min  
 Response: 9152735  
 Conc: 261.20 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1660ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#7 AR-1016-5





R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 9323046  
 Conc: 309.18 ng/ml

#31 AR-1260-1

R.T.: 7.260 min  
 Delta R.T.: 0.004 min  
 Response: 18182257  
 Conc: 272.09 ng/ml

#31 AR-1260-1

R.T.: 6.391 min  
 Delta R.T.: -0.001 min  
 Response: 14056672  
 Conc: 291.39 ng/ml

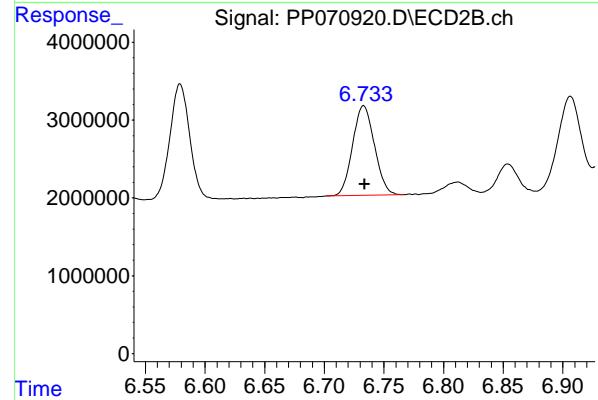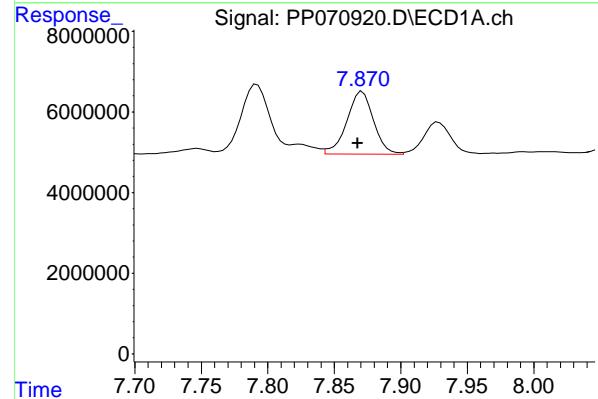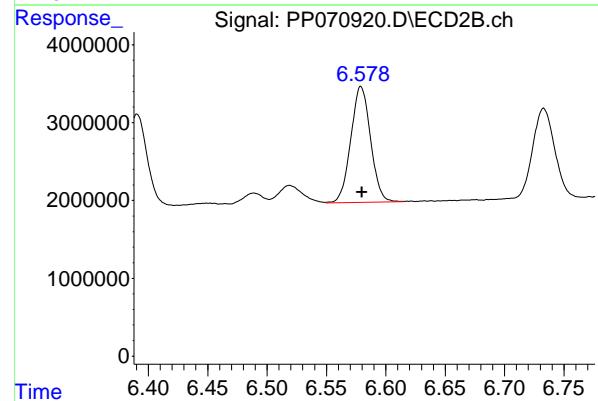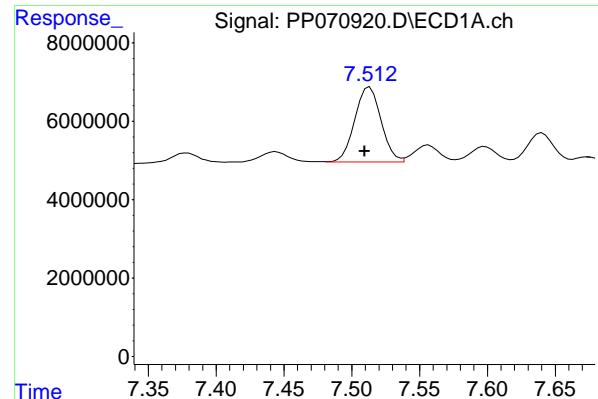

#32 AR-1260-2

R.T.: 7.513 min  
Delta R.T.: 0.004 min  
Instrument: ECD\_P  
Response: 25714746  
Conc: 262.91 ng/ml Client SampleId : AR1660ICC250

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

#32 AR-1260-2





R.T.: 6.579 min  
Delta R.T.: 0.000 min  
Response: 17295947  
Conc: 274.96 ng/ml

#33 AR-1260-3

R.T.: 7.870 min  
Delta R.T.: 0.002 min  
Response: 21528554  
Conc: 259.47 ng/ml

#33 AR-1260-3

R.T.: 6.733 min  
Delta R.T.: 0.000 min  
Response: 14684885  
Conc: 272.34 ng/ml

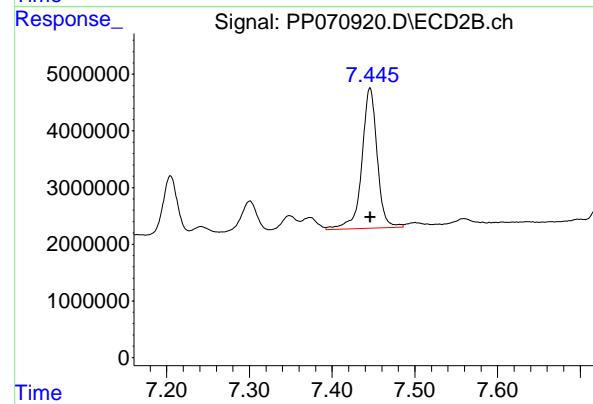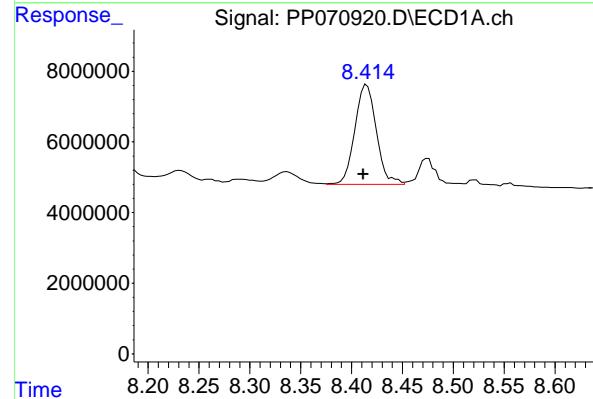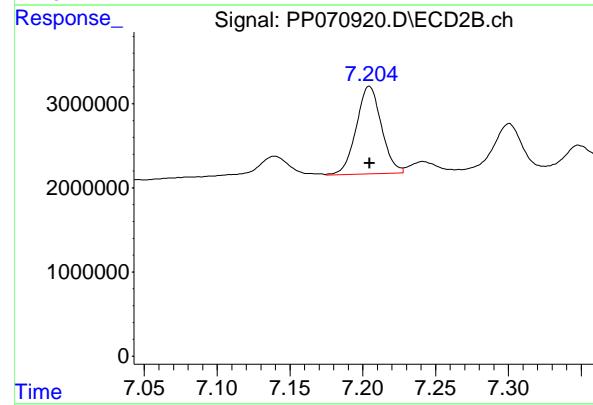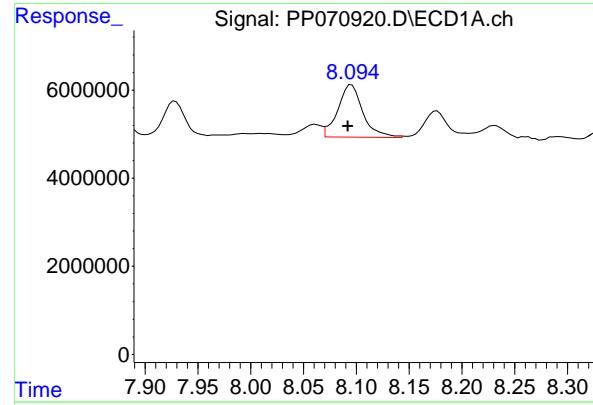

#34 AR-1260-4

R.T.: 8.094 min  
 Delta R.T.: 0.002 min  
 Response: 19536409  
 Conc: 239.85 ng/ml  
 Instrument: ECD\_P  
 ClientSampleId : AR1660ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#34 AR-1260-4

R.T.: 7.205 min  
 Delta R.T.: 0.000 min  
 Response: 12488782  
 Conc: 262.98 ng/ml

#35 AR-1260-5

R.T.: 8.414 min  
 Delta R.T.: 0.002 min  
 Response: 41714322  
 Conc: 260.78 ng/ml

#35 AR-1260-5

R.T.: 7.446 min  
 Delta R.T.: 0.000 min  
 Response: 31815782  
 Conc: 253.89 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:35  
 Operator : YP\AJ  
 Sample : AR1660ICC050  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC050**

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:09:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.513	3.816	6533335	5359624	4.300	5.170
2) SA Decachloro...	10.230	8.858	4733739	3413055	4.240	3.946

**Target Compounds**

3) L1 AR-1016-1	5.666	4.903	2617394	2265971	51.388	59.700
4) L1 AR-1016-2	5.688	4.922	4198554	3321854	53.274	61.085
5) L1 AR-1016-3	5.751	5.099	2631097	1626306	56.201	54.484
6) L1 AR-1016-4	5.848	5.140	1614372	1232754	41.378	51.810 #
7) L1 AR-1016-5	6.139	5.356	1610860	1866333	45.971m	61.893 #
31) L7 AR-1260-1	7.257	6.391	3667364	2989801	54.881m	61.977
32) L7 AR-1260-2	7.512	6.579	4685539	3357287	47.905	53.372
33) L7 AR-1260-3	7.869	6.732	3780088	2827385	45.559m	52.436
34) L7 AR-1260-4	8.094	7.205	4593822	2746307	56.400m	57.831
35) L7 AR-1260-5	8.412	7.445	7845589	7013440	49.047m	55.967

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:35  
 Operator : YP\AJ  
 Sample : AR1660ICC050  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:09:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 11:40:16 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1660ICC050

### Manual Integrations APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

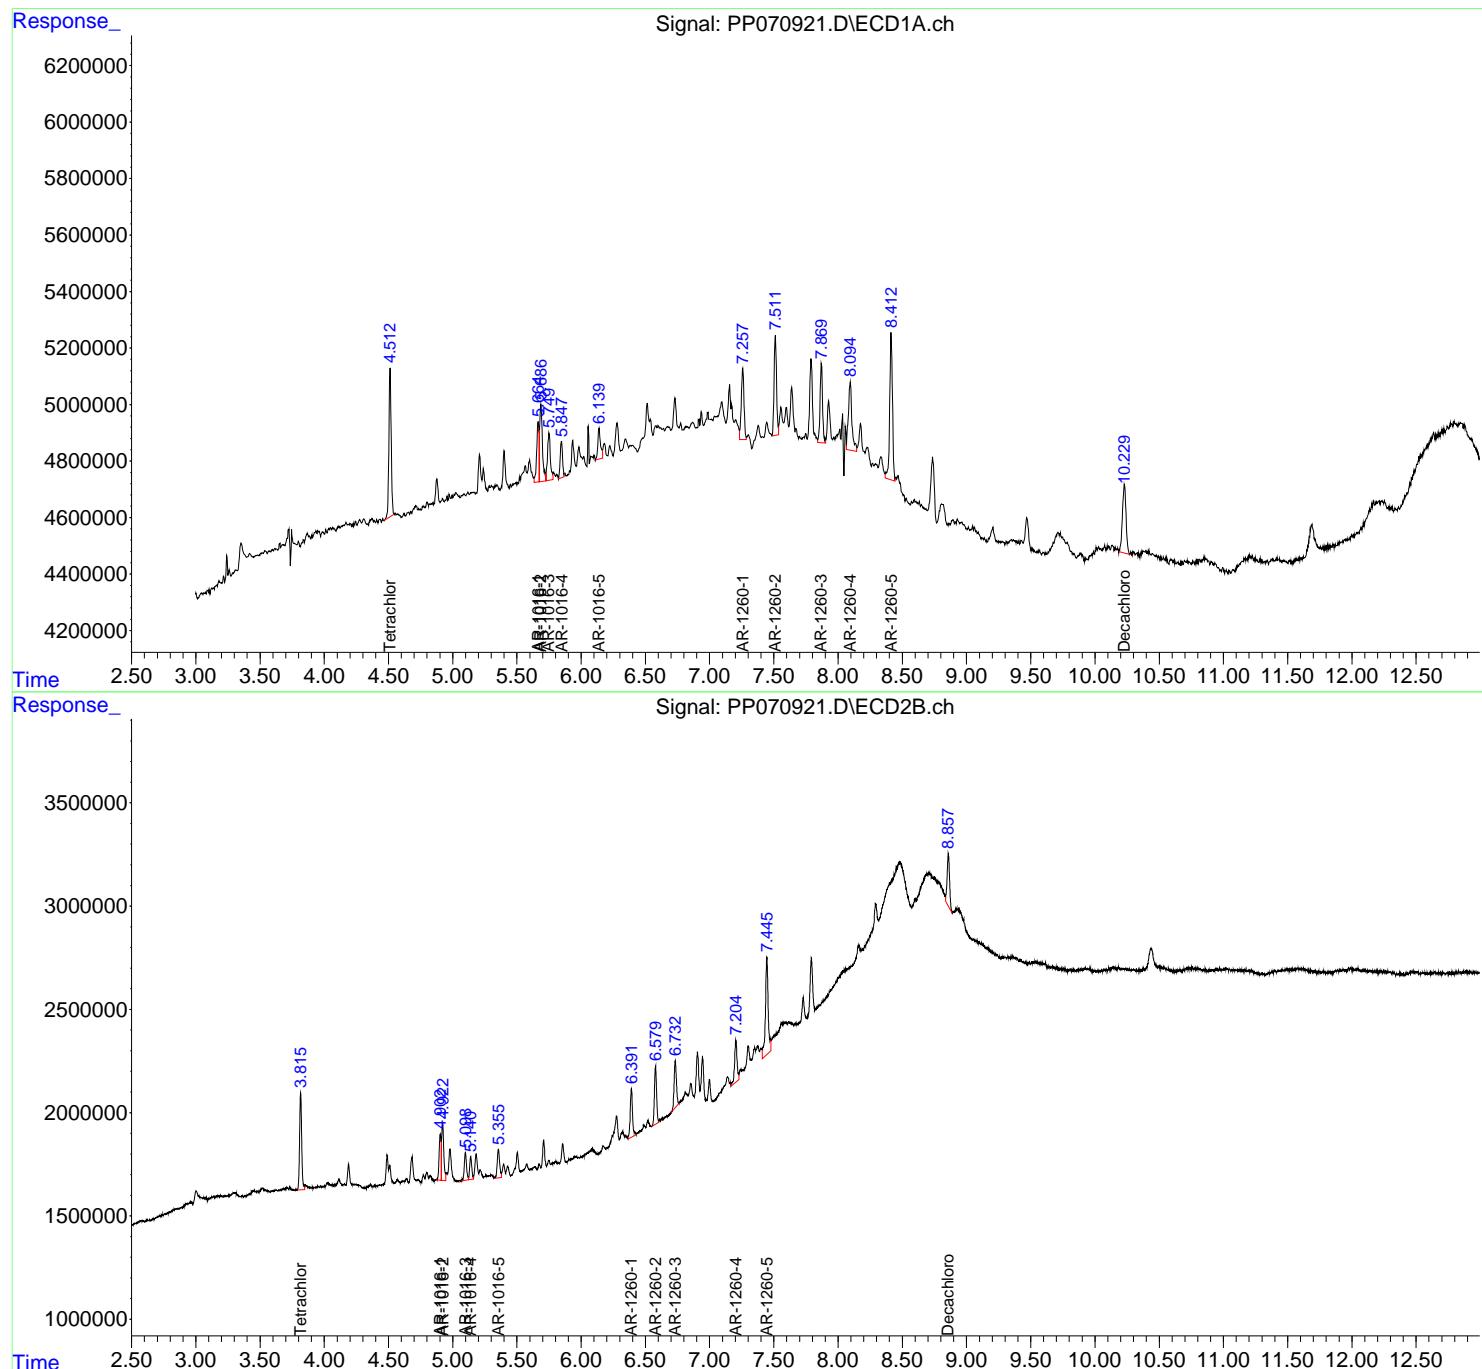

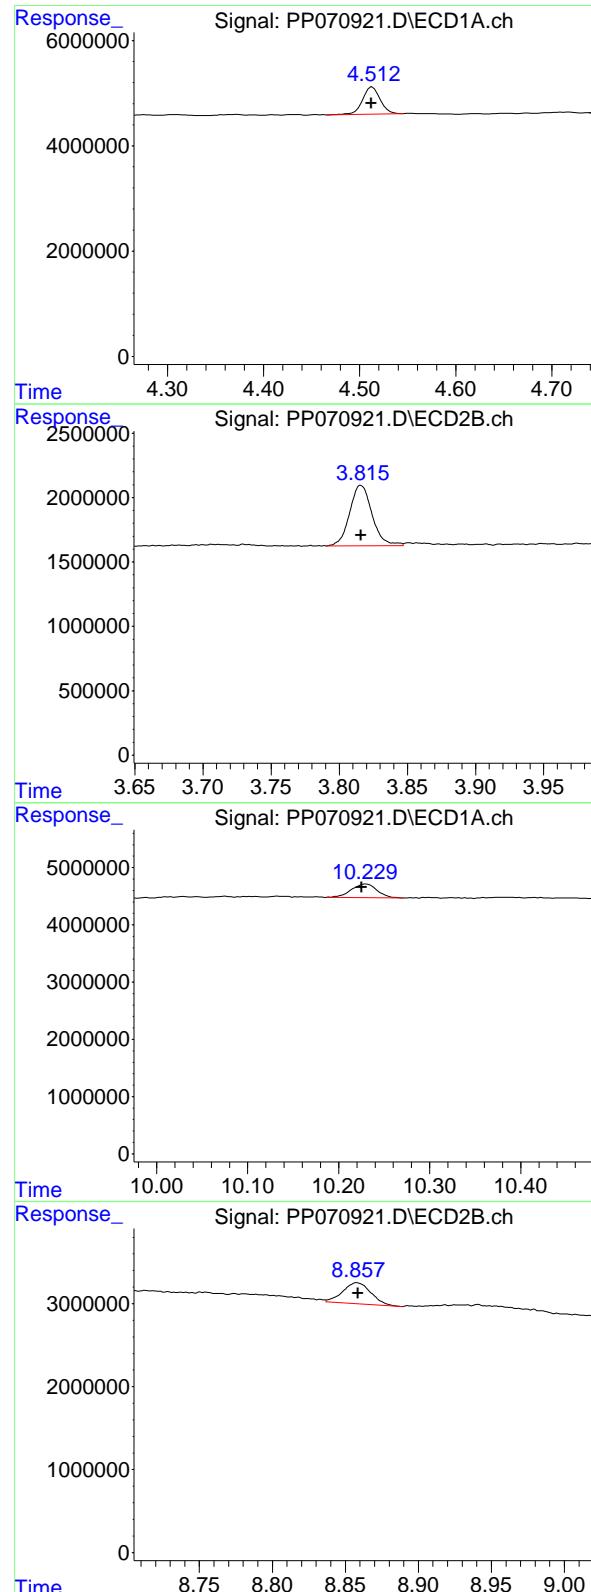

## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
 Delta R.T.: 0.001 min  
 Response: 6533335 ECD\_P  
 Conc: 4.30 ng/ml ClientSampleId : AR1660ICC050

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene


R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 5359624  
 Conc: 5.17 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.230 min  
 Delta R.T.: 0.005 min  
 Response: 4733739  
 Conc: 4.24 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.858 min  
 Delta R.T.: 0.000 min  
 Response: 3413055  
 Conc: 3.95 ng/ml

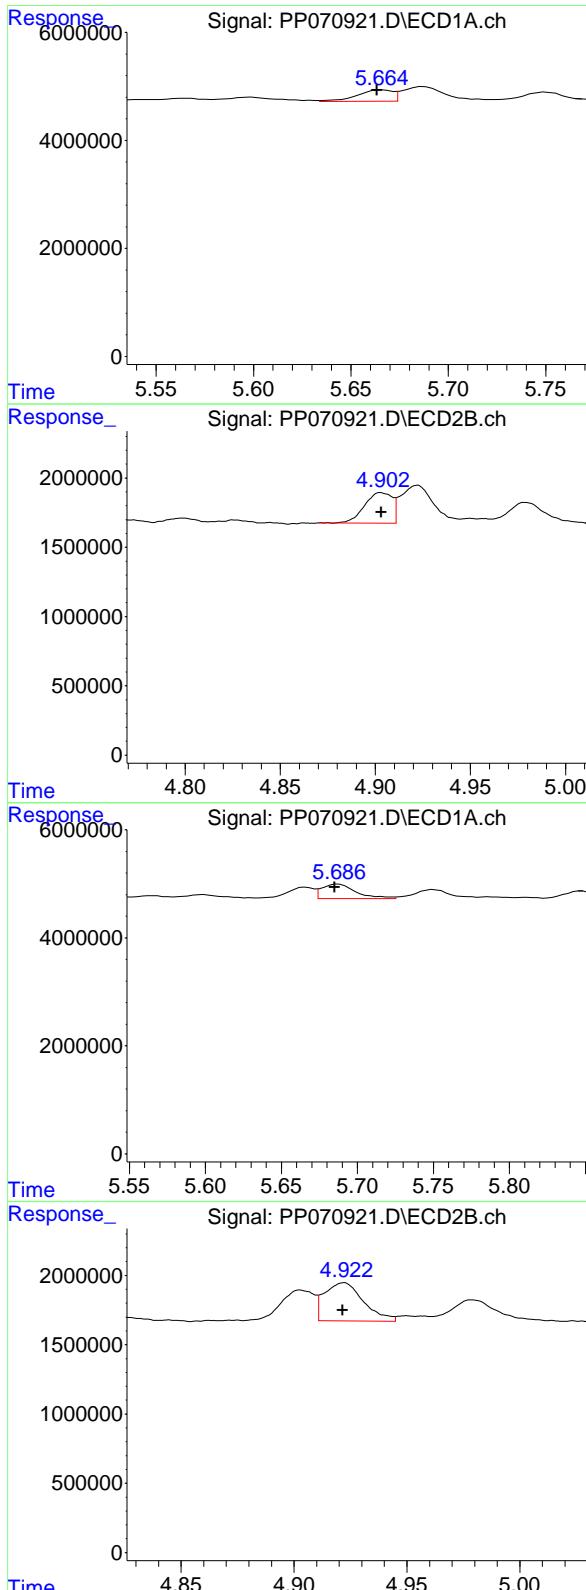

#3 AR-1016-1

R.T.: 5.666 min  
 Delta R.T.: 0.002 min  
 Response: 2617394 ECD\_P  
 Conc: 51.39 ng/ml ClientSampleId : AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#3 AR-1016-1


R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 2265971  
 Conc: 59.70 ng/ml

#4 AR-1016-2

R.T.: 5.688 min  
 Delta R.T.: 0.002 min  
 Response: 4198554  
 Conc: 53.27 ng/ml

#4 AR-1016-2

R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 3321854  
 Conc: 61.09 ng/ml

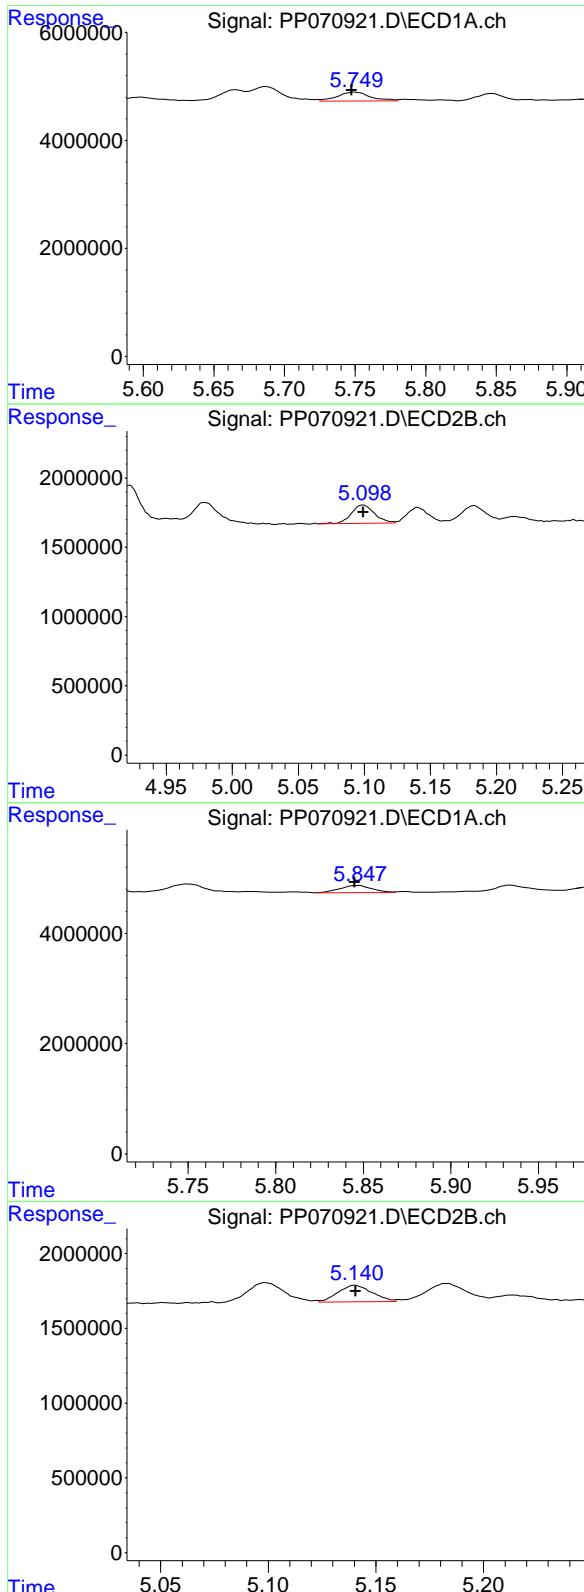

#5 AR-1016-3

R.T.: 5.751 min  
 Delta R.T.: 0.003 min  
 Response: 2631097  
 Conc: 56.20 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#5 AR-1016-3





R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 1626306  
 Conc: 54.48 ng/ml

#6 AR-1016-4

R.T.: 5.848 min  
 Delta R.T.: 0.003 min  
 Response: 1614372  
 Conc: 41.38 ng/ml

#6 AR-1016-4

R.T.: 5.140 min  
 Delta R.T.: 0.000 min  
 Response: 1232754  
 Conc: 51.81 ng/ml

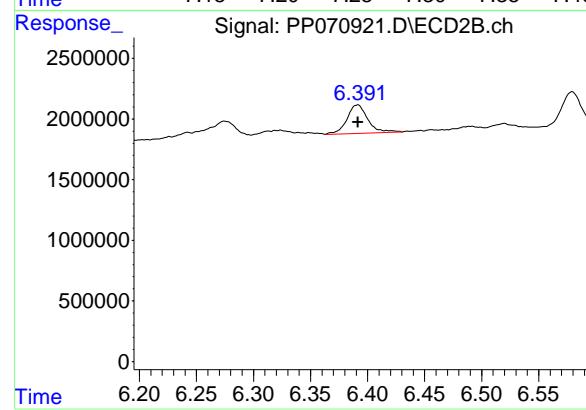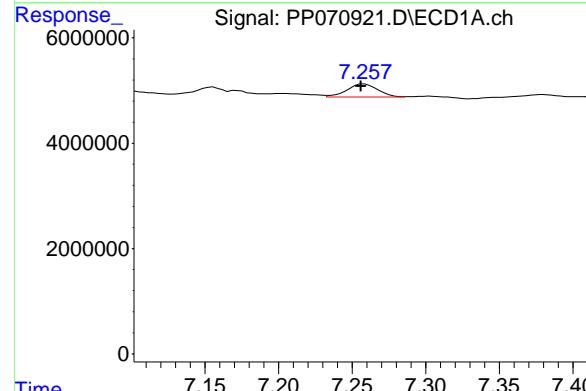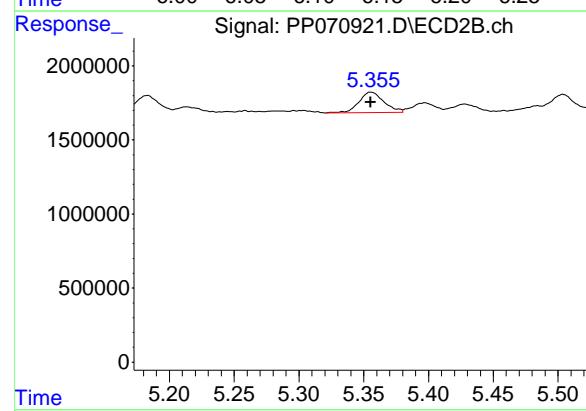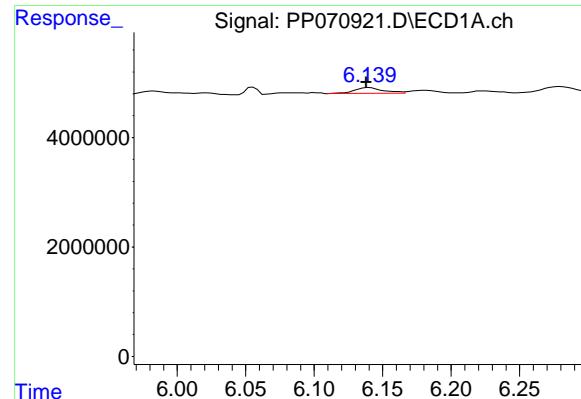

#7 AR-1016-5

R.T.: 6.139 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_P  
 Response: 1610860  
 Conc: 45.97 ng/ml  
 ClientSampleId : AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#7 AR-1016-5





R.T.: 5.356 min  
 Delta R.T.: 0.000 min  
 Response: 1866333  
 Conc: 61.89 ng/ml

#31 AR-1260-1

R.T.: 7.257 min  
 Delta R.T.: 0.001 min  
 Response: 3667364  
 Conc: 54.88 ng/ml

#31 AR-1260-1

R.T.: 6.391 min  
 Delta R.T.: 0.000 min  
 Response: 2989801  
 Conc: 61.98 ng/ml

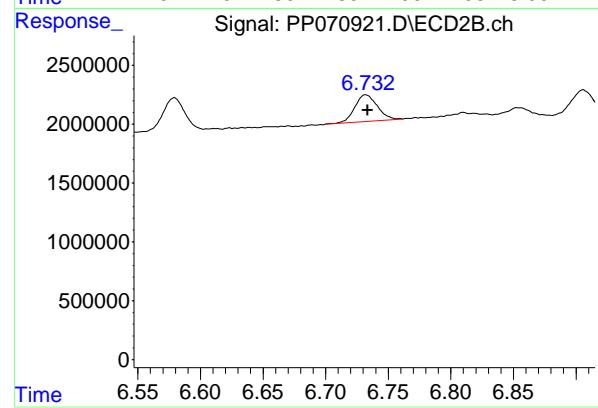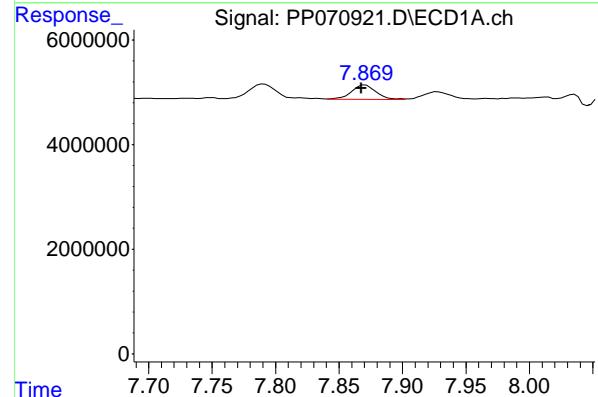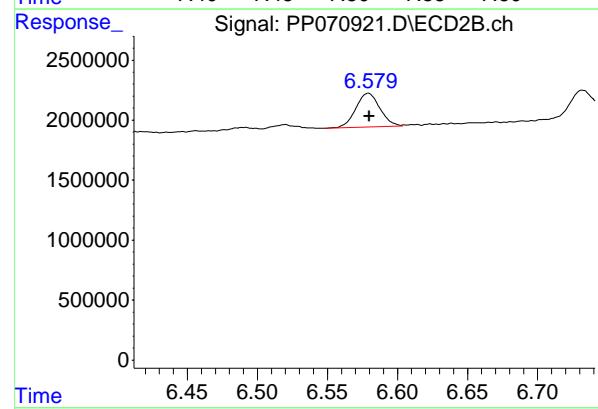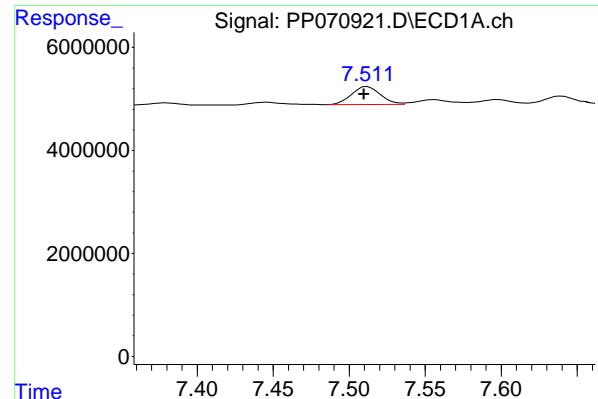

#32 AR-1260-2

R.T.: 7.512 min  
 Delta R.T.: 0.002 min  
 Response: 4685539 ECD\_P  
 Conc: 47.91 ng/ml ClientSampleId : AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#32 AR-1260-2


R.T.: 6.579 min  
 Delta R.T.: 0.000 min  
 Response: 3357287  
 Conc: 53.37 ng/ml

#33 AR-1260-3

R.T.: 7.869 min  
 Delta R.T.: 0.002 min  
 Response: 3780088  
 Conc: 45.56 ng/ml

#33 AR-1260-3

R.T.: 6.732 min  
 Delta R.T.: -0.001 min  
 Response: 2827385  
 Conc: 52.44 ng/ml

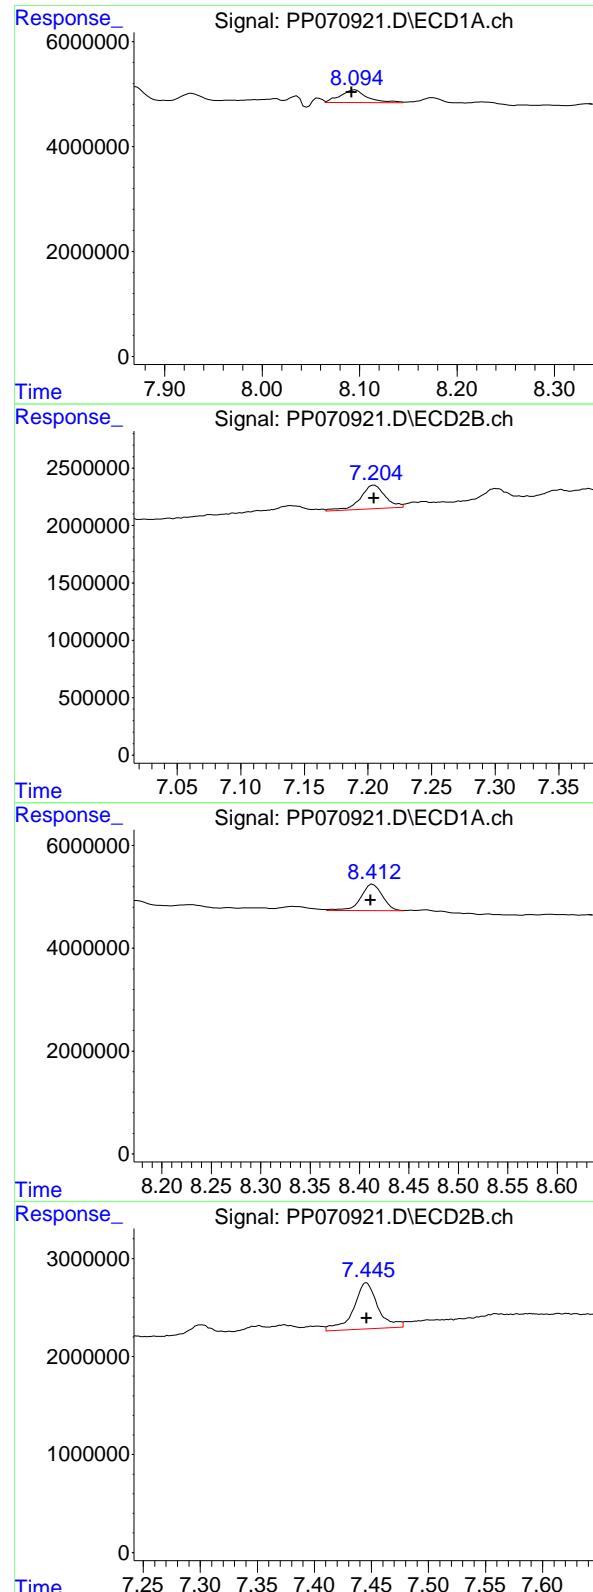

#34 AR-1260-4

R.T.: 8.094 min  
 Delta R.T.: 0.002 min  
 Response: 4593822 ECD\_P  
 Conc: 56.40 ng/ml ClientSampleId : AR1660ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#34 AR-1260-4

R.T.: 7.205 min  
 Delta R.T.: 0.000 min  
 Response: 2746307  
 Conc: 57.83 ng/ml

#35 AR-1260-5

R.T.: 8.412 min  
 Delta R.T.: 0.000 min  
 Response: 7845589  
 Conc: 49.05 ng/ml

#35 AR-1260-5

R.T.: 7.445 min  
 Delta R.T.: 0.000 min  
 Response: 7013440  
 Conc: 55.97 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070922.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:52  
 Operator : YP\AJ  
 Sample : AR1221ICC500  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1221ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:33:19 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 12:32:55 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.515	3.817	75324924	52315210	50.000	50.000
2) SA Decachloro...	10.229	8.859	52098024	39006992	50.000	50.000

**Target Compounds**

8) L2 AR-1221-1	4.716	4.027	8676827	7621792	500.000	500.000
9) L2 AR-1221-2	4.802	4.114	6476464	5718144	500.000	500.000
10) L2 AR-1221-3	4.878	4.190	20858618	17044480	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070922.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:52  
 Operator : YP\AJ  
 Sample : AR1221ICC500  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1221ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:33:19 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 12:32:55 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

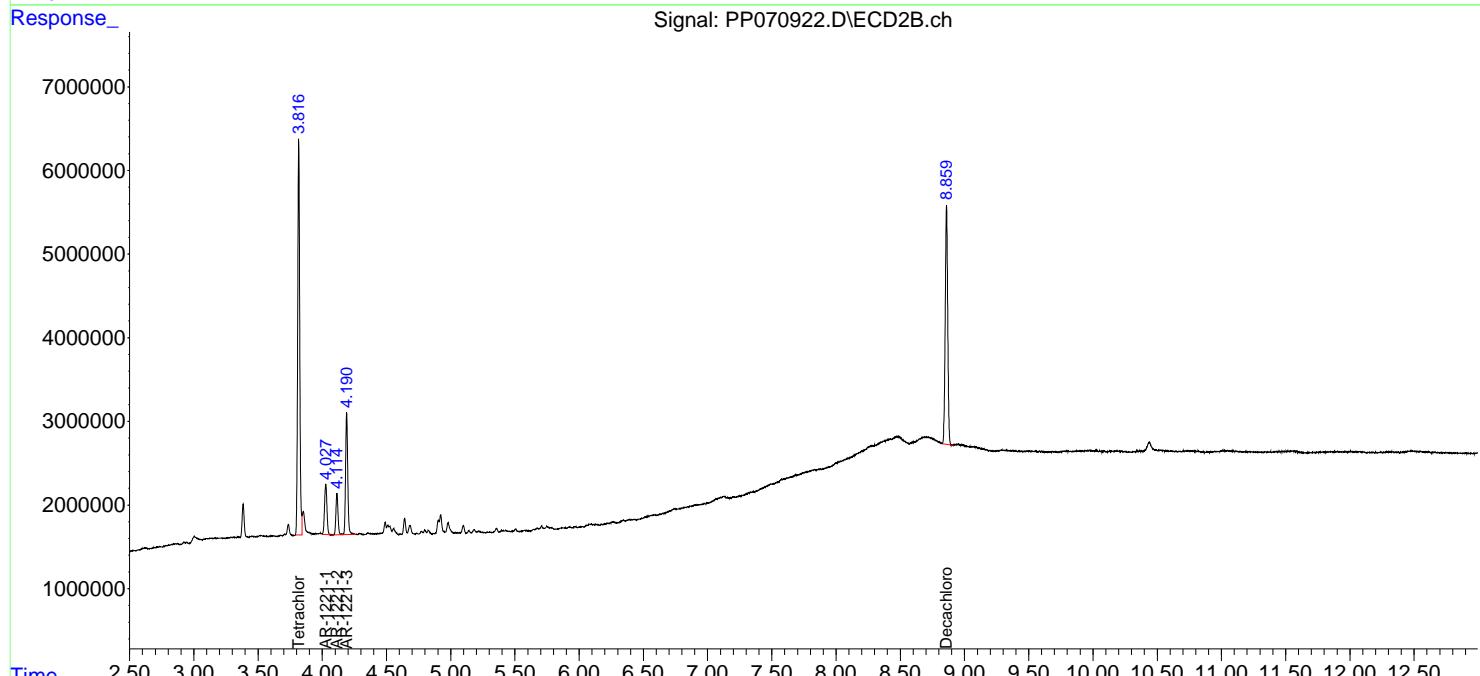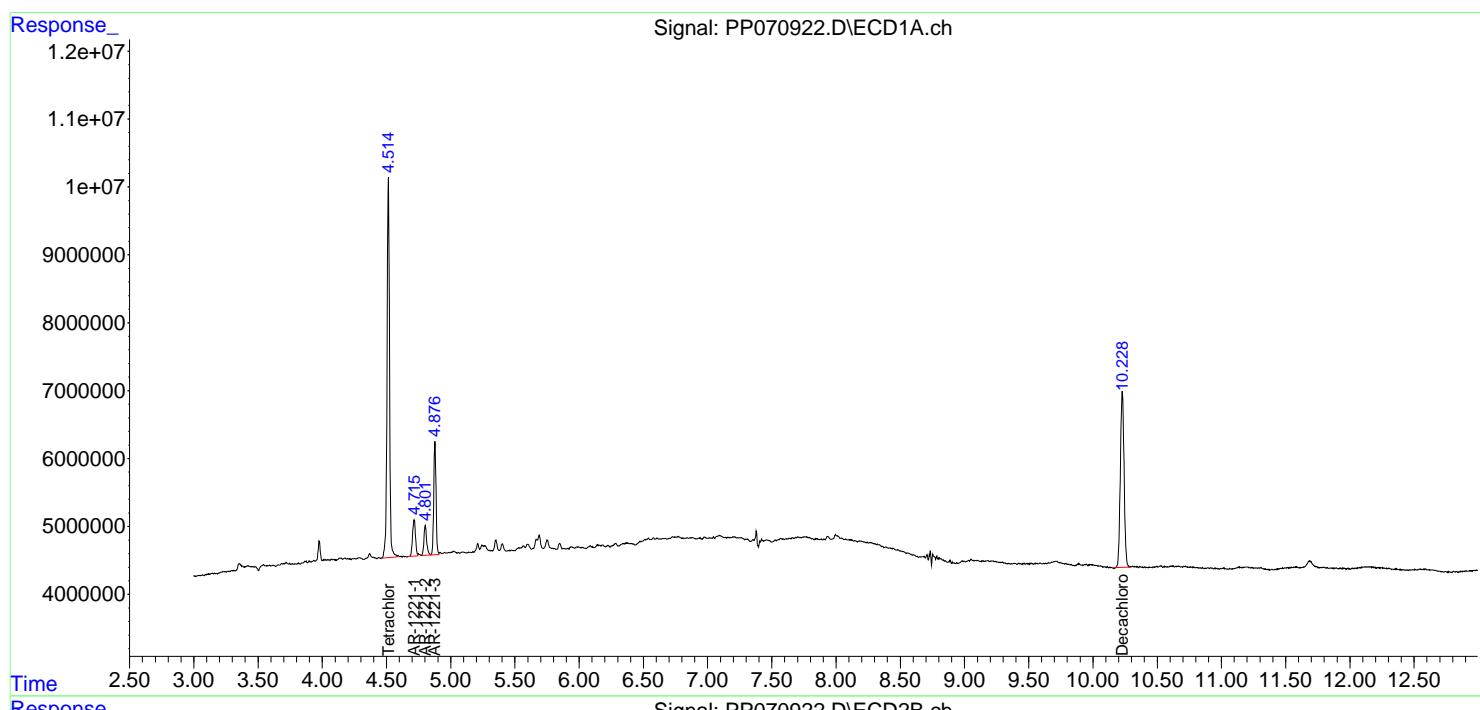

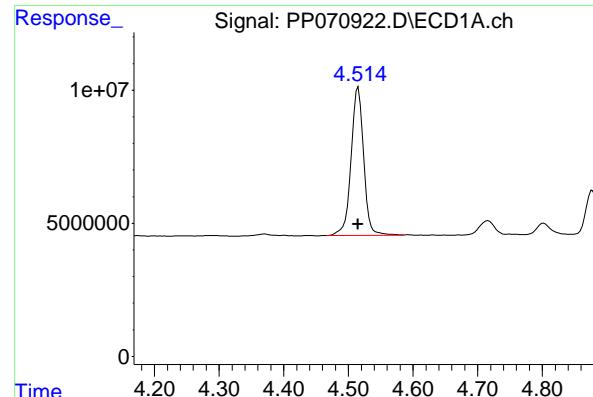


## #1 Tetrachloro-m-xylene

R.T.: 4.515 min  
 Delta R.T.: 0.000 min  
 Response: 75324924 ECD\_P  
 Conc: 50.00 ng/ml ClientSampleId : AR1221ICC500

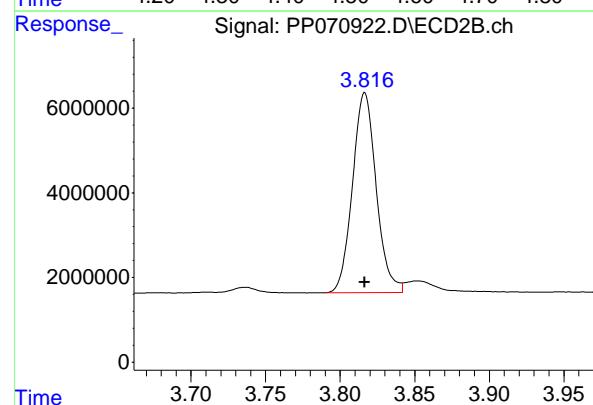


## #1 Tetrachloro-m-xylene

R.T.: 3.817 min  
 Delta R.T.: 0.000 min  
 Response: 52315210  
 Conc: 50.00 ng/ml

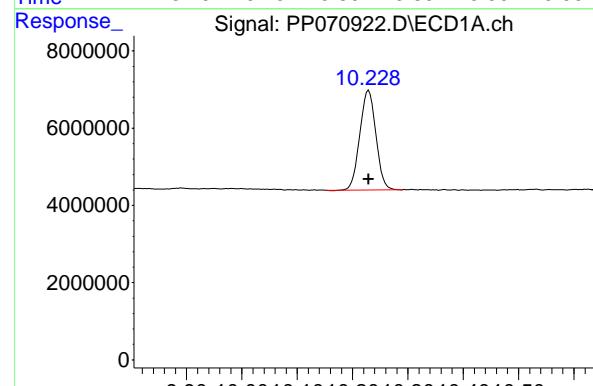




## #2 Decachlorobiphenyl

R.T.: 10.229 min  
 Delta R.T.: 0.000 min  
 Response: 52098024  
 Conc: 50.00 ng/ml

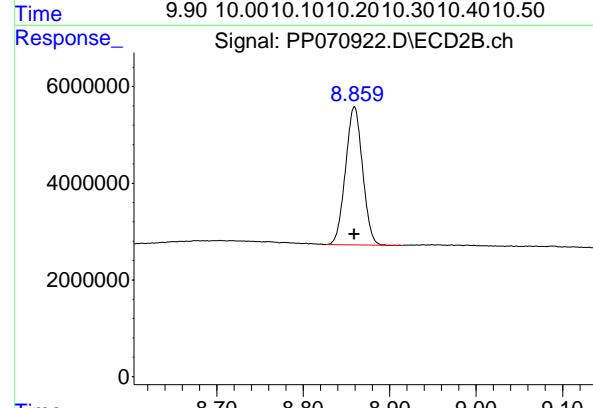

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 39006992  
 Conc: 50.00 ng/ml

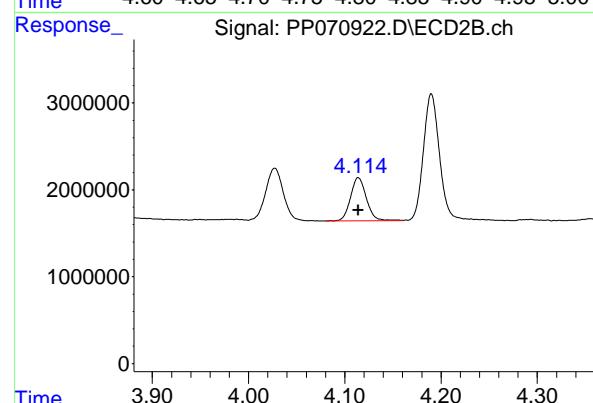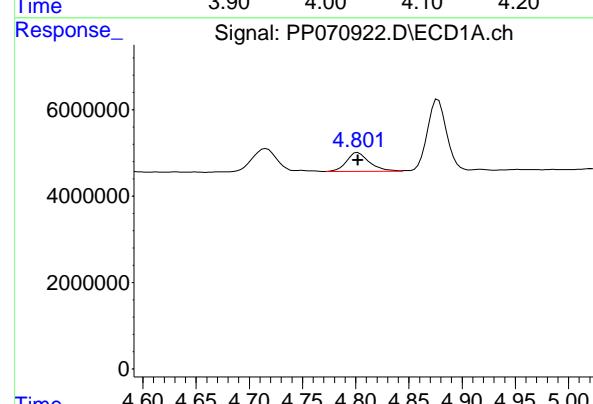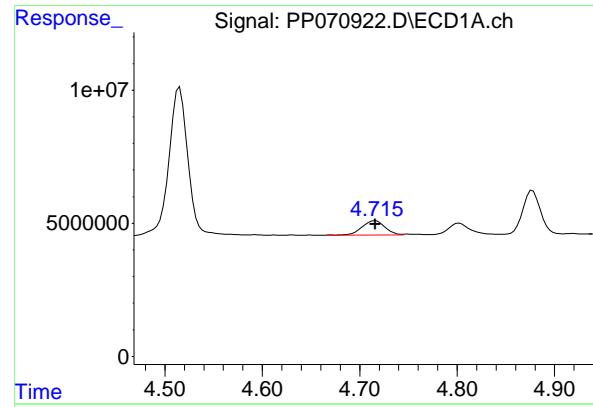

#8 AR-1221-1

R.T.: 4.716 min  
 Delta R.T.: 0.000 min  
 Response: 8676827  
 Conc: 500.00 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1221ICC500

#8 AR-1221-1

R.T.: 4.027 min  
 Delta R.T.: 0.000 min  
 Response: 7621792  
 Conc: 500.00 ng/ml

#9 AR-1221-2



R.T.: 4.802 min  
 Delta R.T.: 0.000 min  
 Response: 6476464  
 Conc: 500.00 ng/ml

#9 AR-1221-2

R.T.: 4.114 min  
 Delta R.T.: 0.000 min  
 Response: 5718144  
 Conc: 500.00 ng/ml

#10 AR-1221-3

R.T.: 4.878 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 20858618  
Conc: 500.00 ng/ml  
ClientSampleId: AR1221ICC500

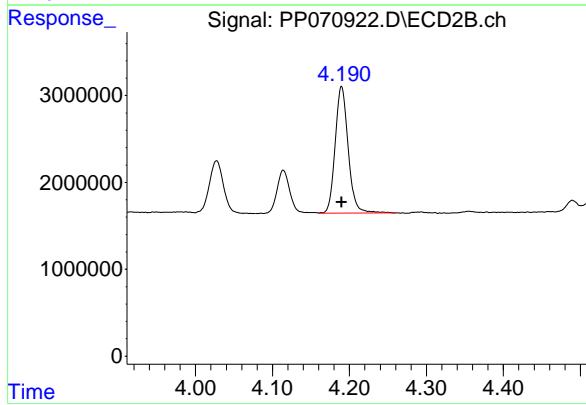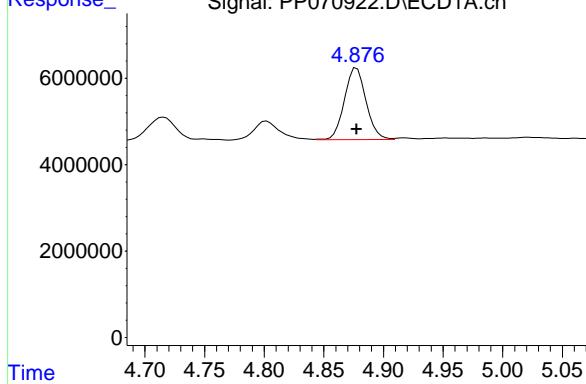

#10 AR-1221-3

R.T.: 4.190 min  
Delta R.T.: 0.000 min  
Response: 17044480  
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070923.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 12:11  
 Operator : YP\AJ  
 Sample : AR1232ICC500  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
AR1232ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:39:29 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 12:38:20 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.520	3.817	74435949	51438566	50.000	50.000
2) SA Decachloro...	10.234	8.860	46115316	40517792	51.013m	50.000

**Target Compounds**

11) L3 AR-1232-1	4.883	4.191	16644355	13993352	500.000	500.000
12) L3 AR-1232-2	5.408	4.923	7955169	14030567	500.000	500.000
13) L3 AR-1232-3	5.694	5.100	17135200	7444793	500.000	500.000
14) L3 AR-1232-4	5.854	5.185	7853790	6402183	500.000	500.000
15) L3 AR-1232-5	5.943	5.357	5320177	7087391	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070923.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 12:11  
 Operator : YP\AJ  
 Sample : AR1232ICC500  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1



Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1232ICC500





**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:39:29 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 12:38:20 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

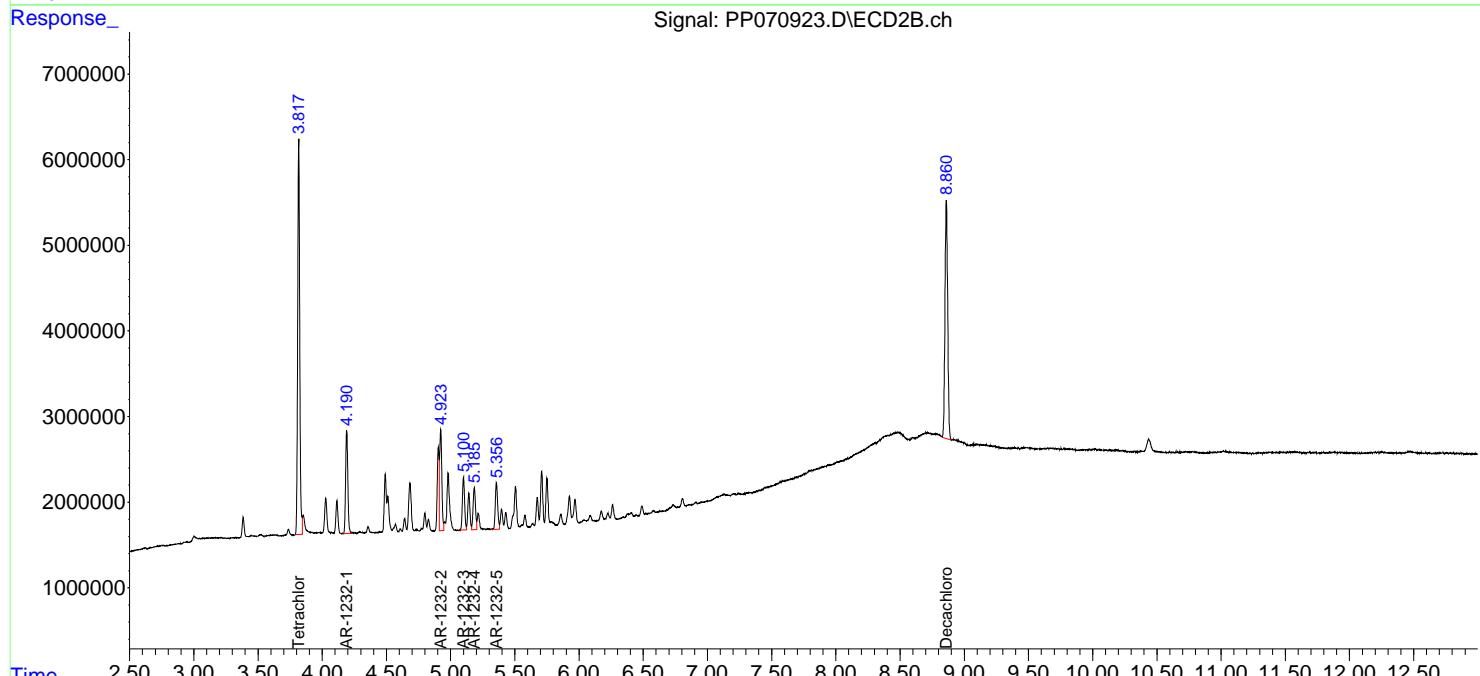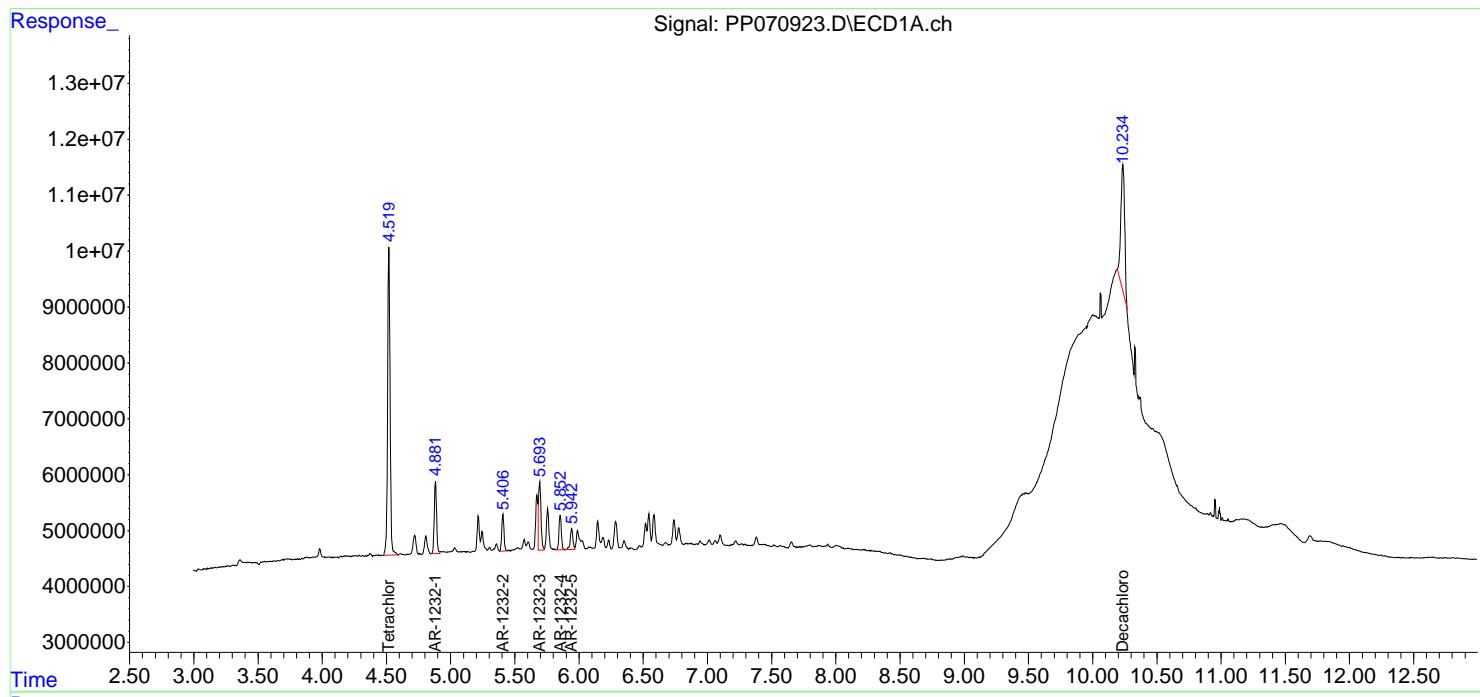

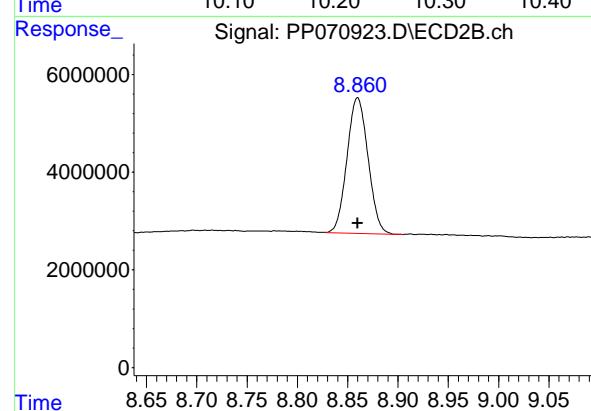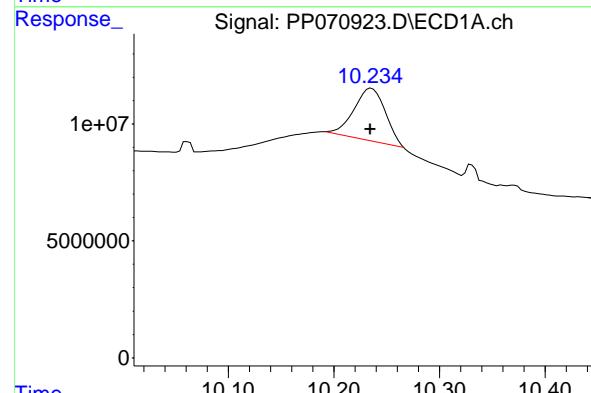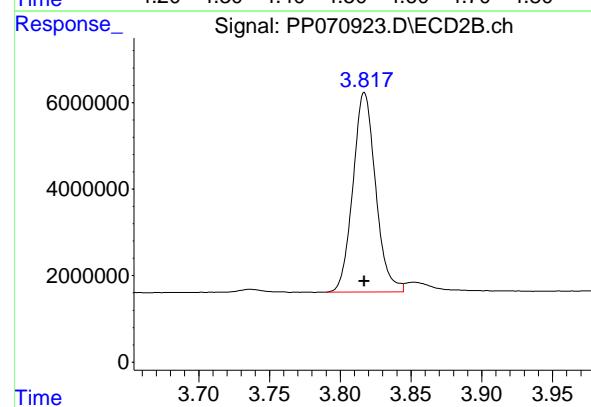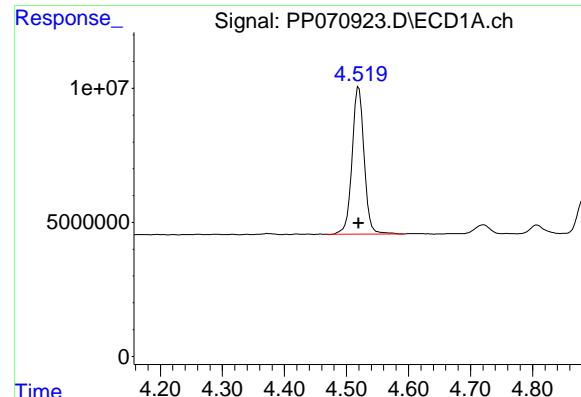

## #1 Tetrachloro-m-xylene

R.T.: 4.520 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 74435949  
Conc: 50.00 ng/ml ClientSampleId : AR1232ICC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene


R.T.: 3.817 min  
Delta R.T.: 0.000 min  
Response: 51438566  
Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.234 min  
Delta R.T.: 0.000 min  
Response: 46115316  
Conc: 51.01 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.860 min  
Delta R.T.: 0.000 min  
Response: 40517792  
Conc: 50.00 ng/ml

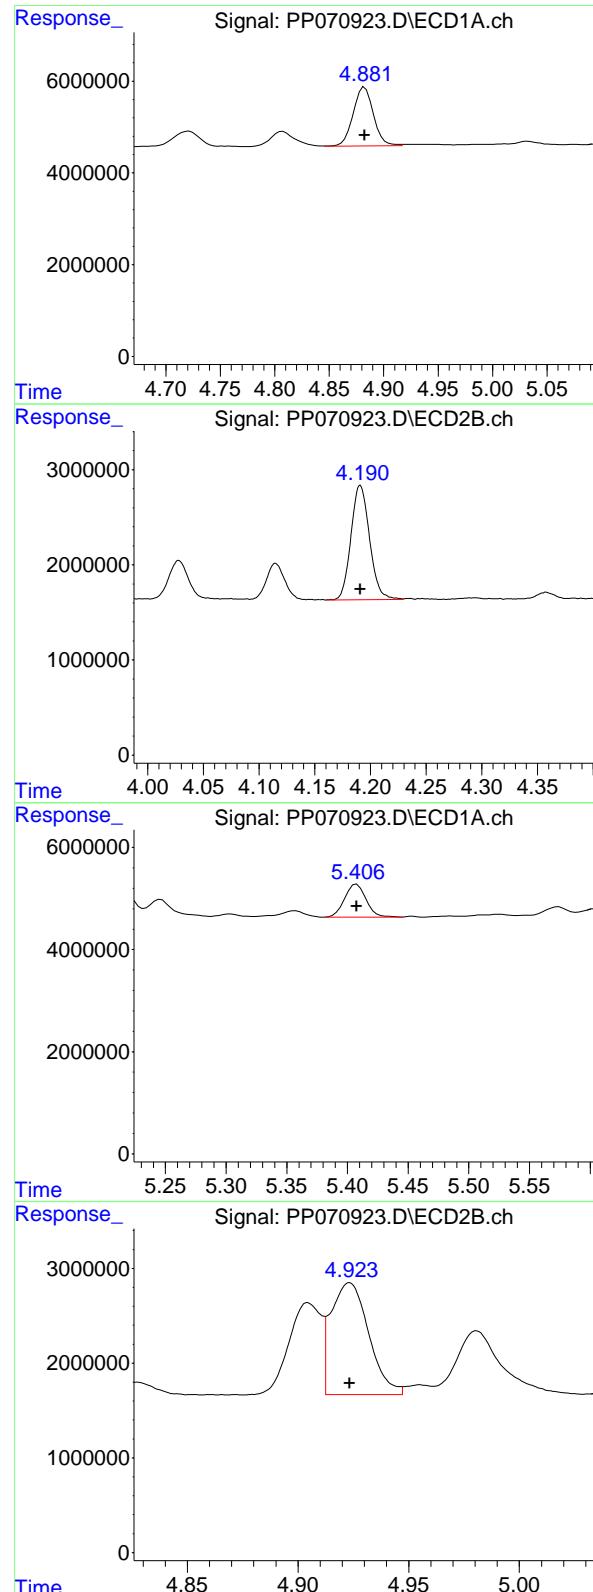

#11 AR-1232-1

R.T.: 4.883 min  
 Delta R.T.: 0.000 min  
 Response: 16644355 ECD\_P  
 Conc: 500.00 ng/ml ClientSampleId : AR1232ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#11 AR-1232-1





R.T.: 4.191 min  
 Delta R.T.: 0.000 min  
 Response: 13993352  
 Conc: 500.00 ng/ml

#12 AR-1232-2

R.T.: 5.408 min  
 Delta R.T.: 0.000 min  
 Response: 7955169  
 Conc: 500.00 ng/ml

#12 AR-1232-2

R.T.: 4.923 min  
 Delta R.T.: 0.000 min  
 Response: 14030567  
 Conc: 500.00 ng/ml

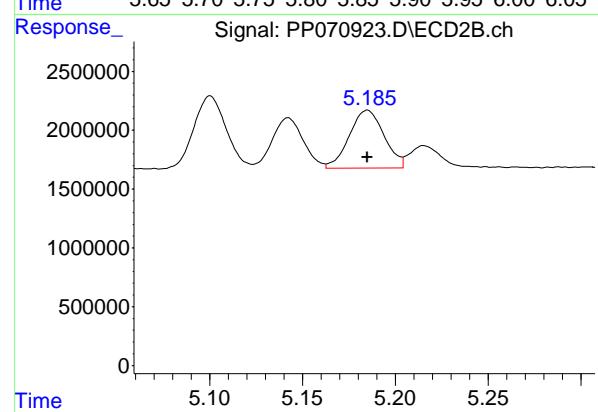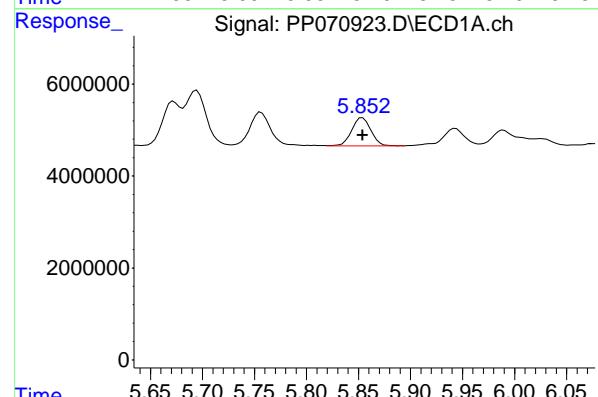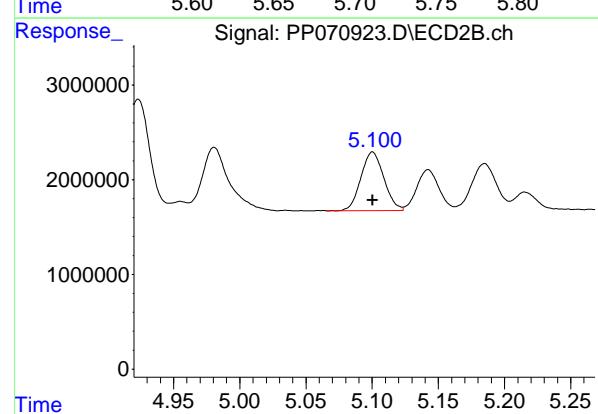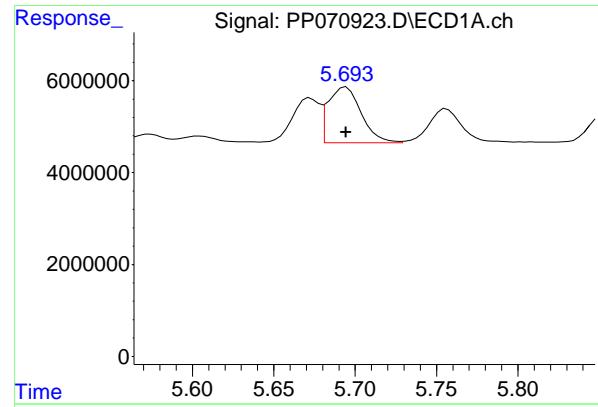

#13 AR-1232-3

R.T.: 5.694 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_P  
 Response: 17135200  
 Conc: 500.00 ng/ml  
 ClientSampleId: AR1232ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#13 AR-1232-3

R.T.: 5.100 min  
 Delta R.T.: 0.000 min  
 Response: 7444793  
 Conc: 500.00 ng/ml

#14 AR-1232-4

R.T.: 5.854 min  
 Delta R.T.: 0.000 min  
 Response: 7853790  
 Conc: 500.00 ng/ml

#14 AR-1232-4

R.T.: 5.185 min  
 Delta R.T.: 0.000 min  
 Response: 6402183  
 Conc: 500.00 ng/ml

#15 AR-1232-5


R.T.: 5.943 min  
 Delta R.T.: 0.000 min  
 Response: 5320177 ECD\_P  
 Conc: 500.00 ng/ml ClientSampleId :  
 AR1232ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#15 AR-1232-5

R.T.: 5.357 min  
 Delta R.T.: 0.000 min  
 Response: 7087391  
 Conc: 500.00 ng/ml

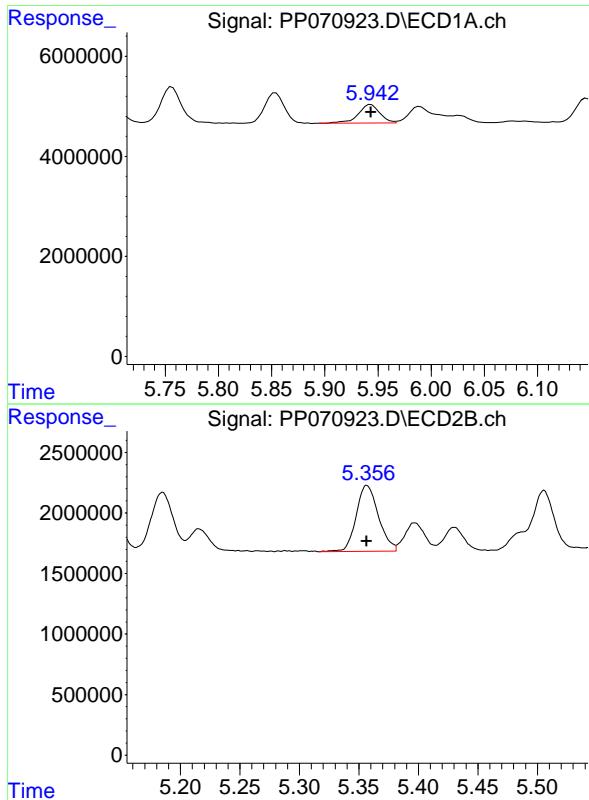

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070924.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 12:28  
 Operator : YP\AJ  
 Sample : AR1242ICC1000  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:28:07 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.513	3.816	144.4E6	99447440	93.922	88.806
2) SA Decachloro...	10.227	8.858	103.6E6	79468601	93.673	102.468

**Target Compounds**

16) L4 AR-1242-1	5.666	4.903	40990074	30391529	943.761	877.115
17) L4 AR-1242-2	5.687	4.922	64704598	43879042	965.382	887.614
18) L4 AR-1242-3	5.749	5.099	39349869	24103124	991.106	905.487
19) L4 AR-1242-4	5.846	5.183	30814559	23086538	954.688	902.469
20) L4 AR-1242-5	6.577	5.707	36006298	28647762	964.427	907.760



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.




Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070924.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 12:28  
 Operator : YP\AJ  
 Sample : AR1242ICC1000  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1242ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:28:07 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

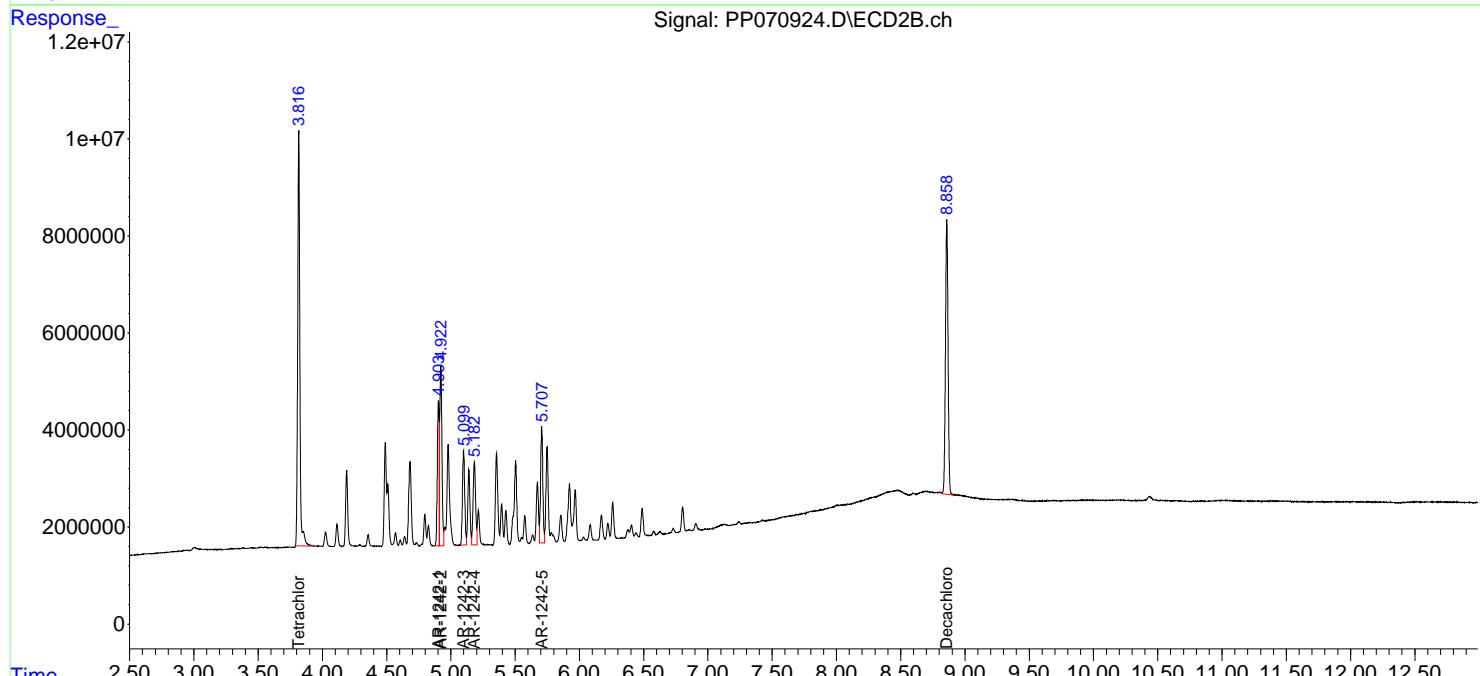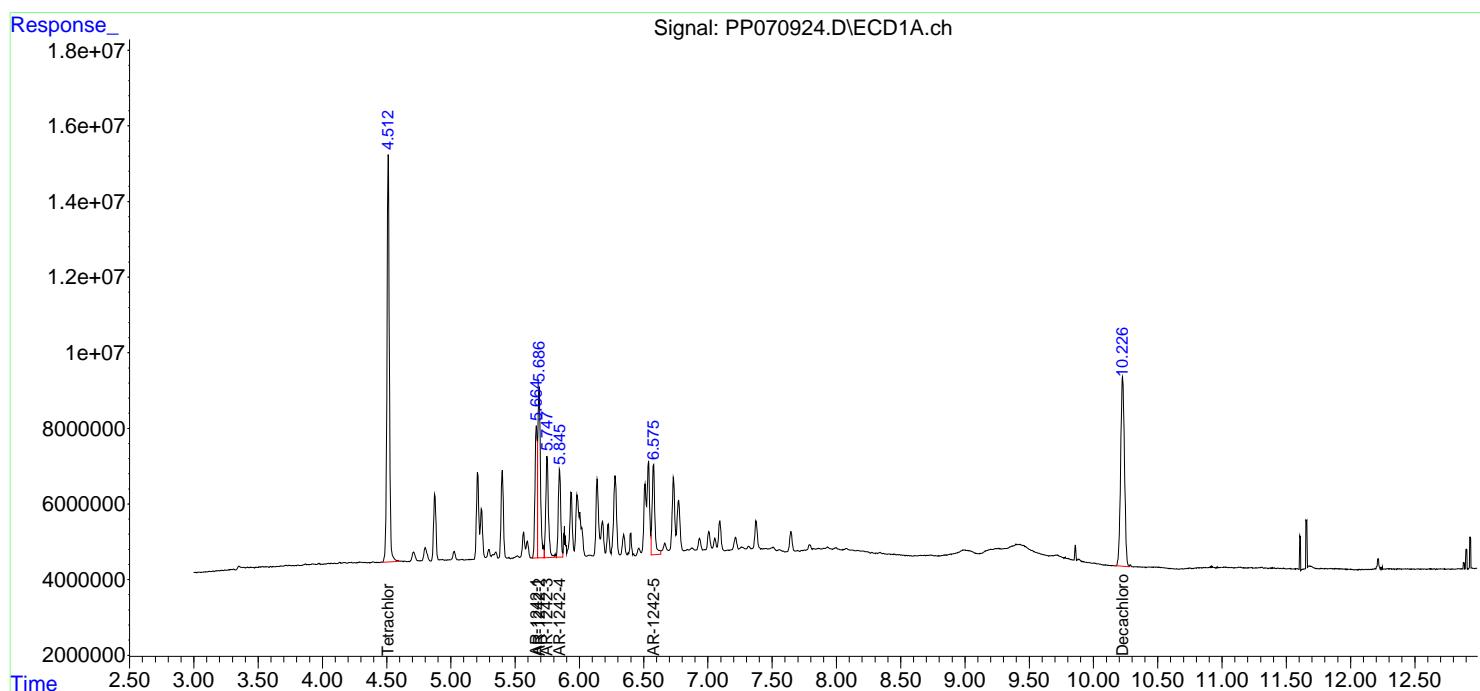

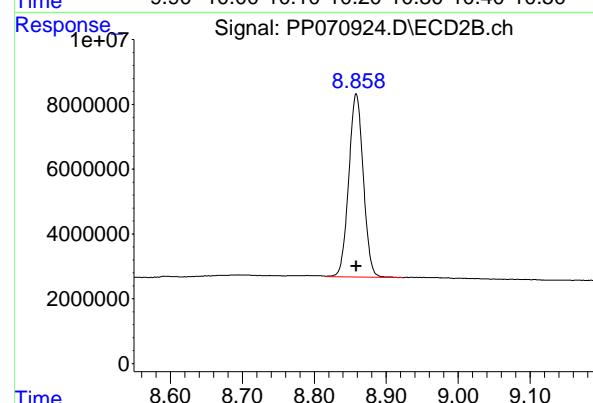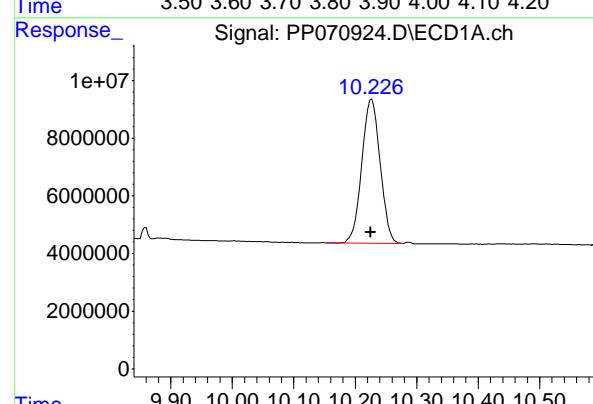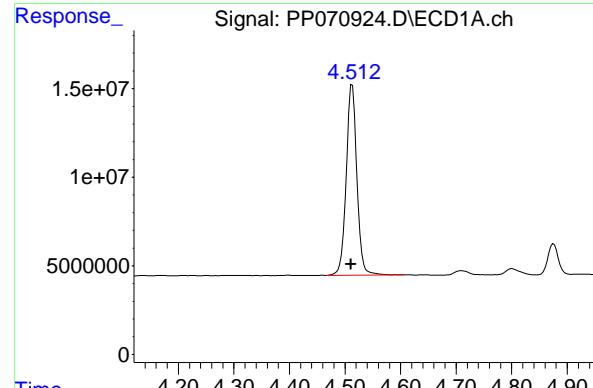

## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
 Delta R.T.: 0.002 min  
 Response: 144394733 ECD\_P  
 Conc: 93.92 ng/ml ClientSampleId : AR1242ICC1000

## #1 Tetrachloro-m-xylene



R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 99447440  
 Conc: 88.81 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.227 min  
 Delta R.T.: 0.002 min  
 Response: 103629813  
 Conc: 93.67 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.858 min  
 Delta R.T.: 0.000 min  
 Response: 79468601  
 Conc: 102.47 ng/ml

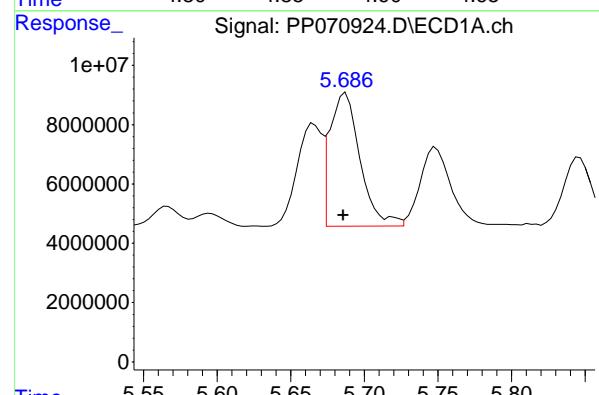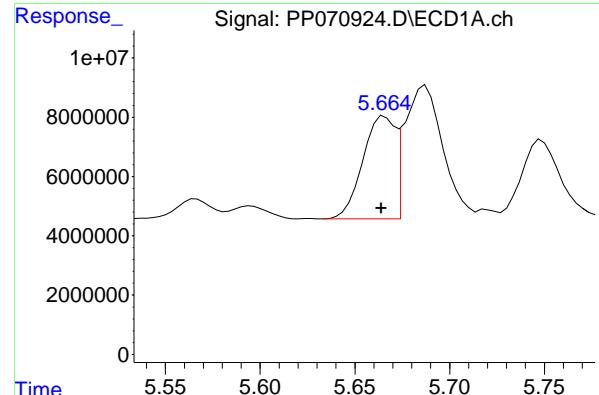

#16 AR-1242-1

R.T.: 5.666 min  
 Delta R.T.: 0.002 min  
 Response: 40990074 ECD\_P  
 Conc: 943.76 ng/ml ClientSampleId : AR1242ICC1000

#16 AR-1242-1


R.T.: 4.903 min  
 Delta R.T.: 0.001 min  
 Response: 30391529  
 Conc: 877.12 ng/ml

#17 AR-1242-2

R.T.: 5.687 min  
 Delta R.T.: 0.002 min  
 Response: 64704598  
 Conc: 965.38 ng/ml

#17 AR-1242-2

R.T.: 4.922 min  
 Delta R.T.: 0.001 min  
 Response: 43879042  
 Conc: 887.61 ng/ml

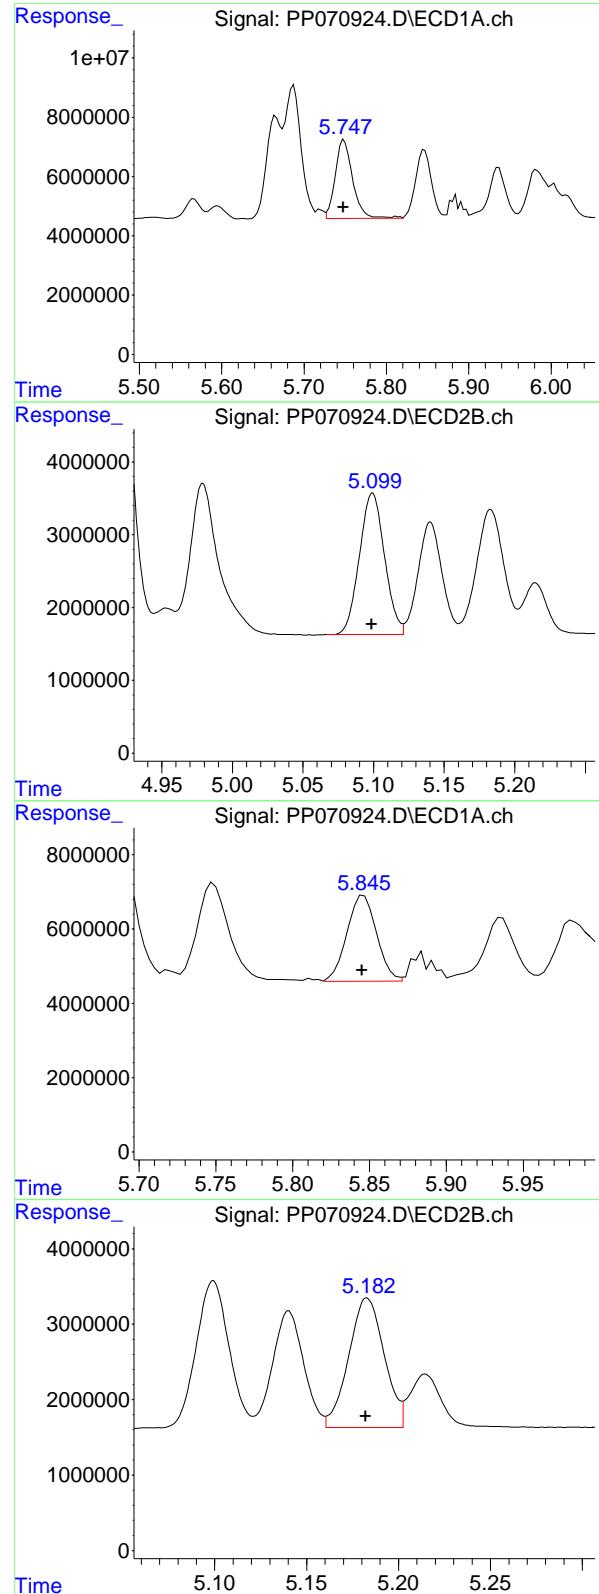

#18 AR-1242-3

R.T.: 5.749 min  
 Delta R.T.: 0.000 min  
 Response: 39349869  
 Conc: 991.11 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** AR1242ICC1000

#18 AR-1242-3

R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 24103124  
 Conc: 905.49 ng/ml

#19 AR-1242-4


R.T.: 5.846 min  
 Delta R.T.: 0.001 min  
 Response: 30814559  
 Conc: 954.69 ng/ml

#19 AR-1242-4

R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 23086538  
 Conc: 902.47 ng/ml


#20 AR-1242-5

R.T.: 6.577 min  
Delta R.T.: 0.001 min  
Instrument: ECD\_P  
Response: 36006298  
Conc: 964.43 ng/ml  
ClientSampleId: AR1242ICC1000

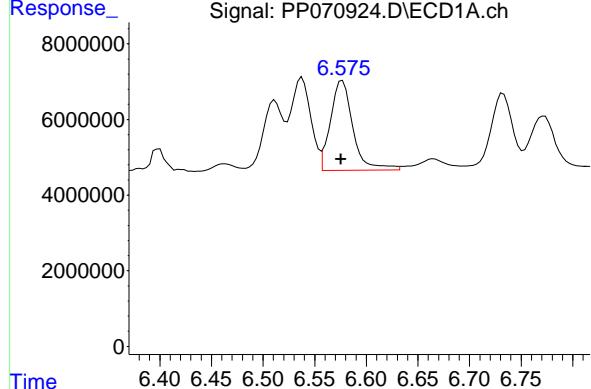

#20 AR-1242-5

R.T.: 5.707 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 28647762  
Conc: 907.76 ng/ml

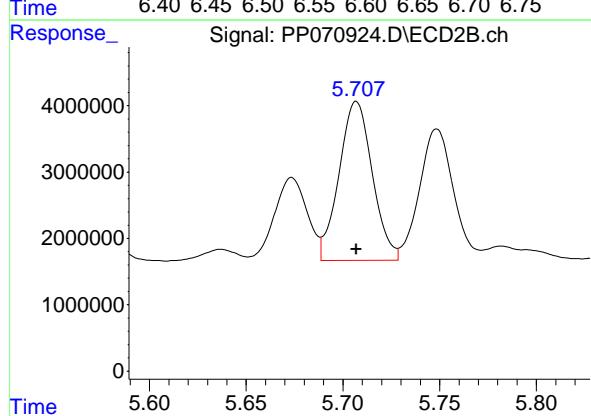

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070925.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 12:44  
 Operator : YP\AJ  
 Sample : AR1242ICC750  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:28:30 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.513	3.816	113.1E6	76564298	73.554	68.372
2) SA Decachlor...	10.229	8.859	79761677	58459899	72.098	75.379

Target Compounds

16) L4 AR-1242-1	5.666	4.903	32059711	23829543	738.147	687.733
17) L4 AR-1242-2	5.687	4.921	47897203	33806804	714.618	683.867
18) L4 AR-1242-3	5.750	5.099	28536378	18473047	718.747	693.981
19) L4 AR-1242-4	5.847	5.183	23599640	17369419	731.158	678.983
20) L4 AR-1242-5	6.577	5.707	26235924	21926365	702.728	694.780



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070925.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 12:44  
 Operator : YP\AJ  
 Sample : AR1242ICC750  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:28:30 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

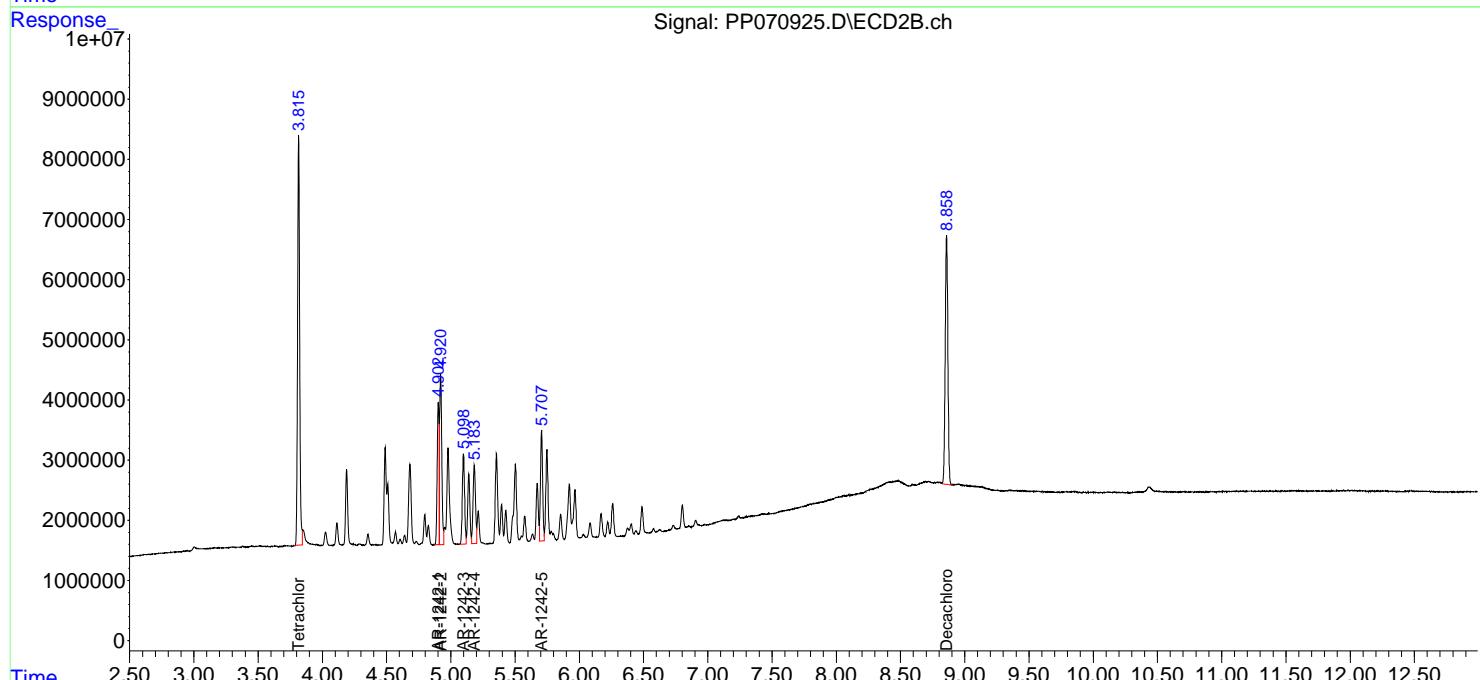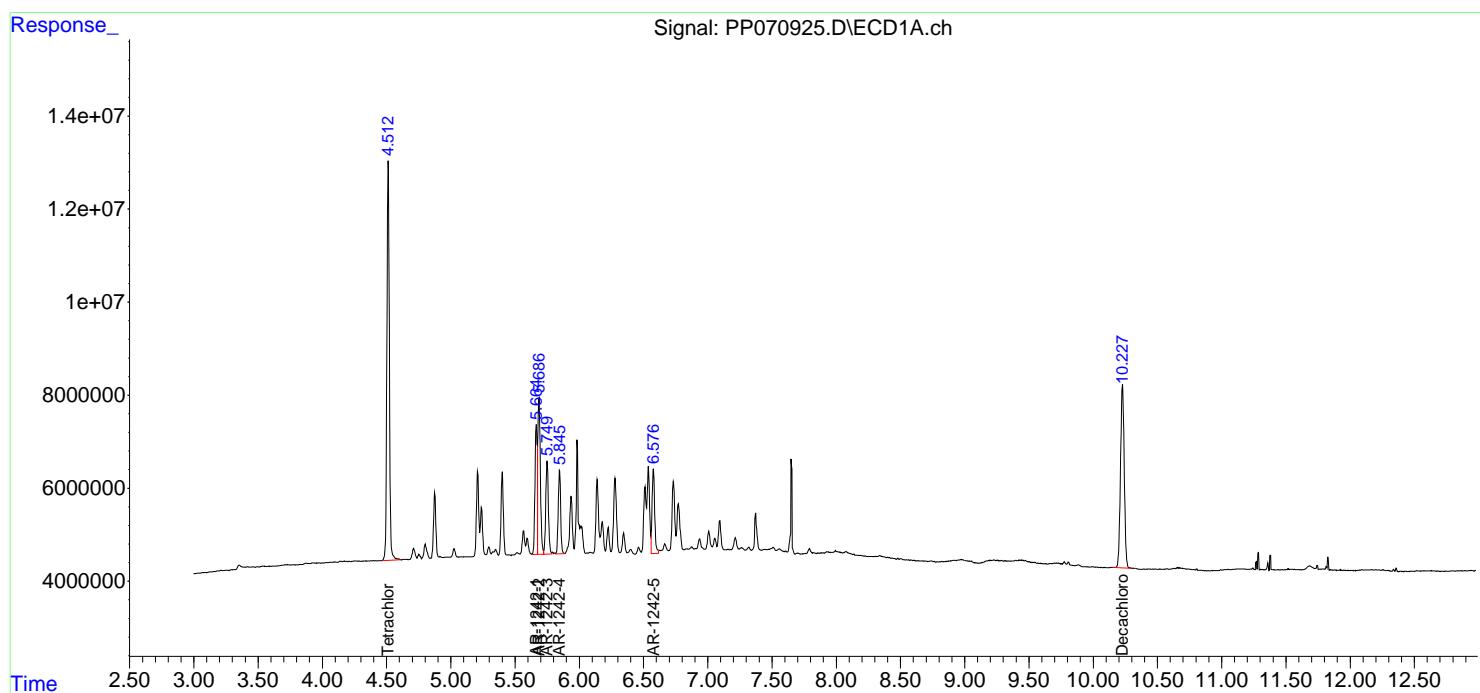

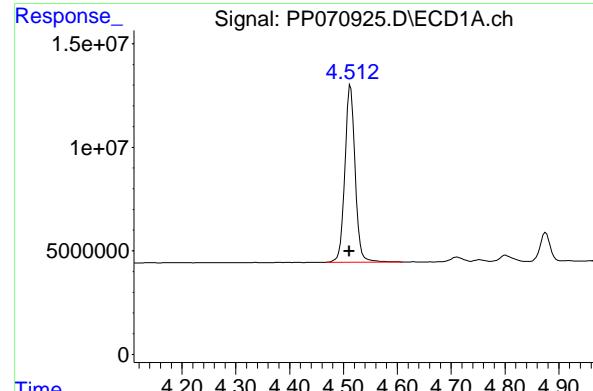


## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
Delta R.T.: 0.002 min  
Instrument: ECD\_P  
Response: 113081073  
Conc: 73.55 ng/ml  
ClientSampleId : AR1242ICC750

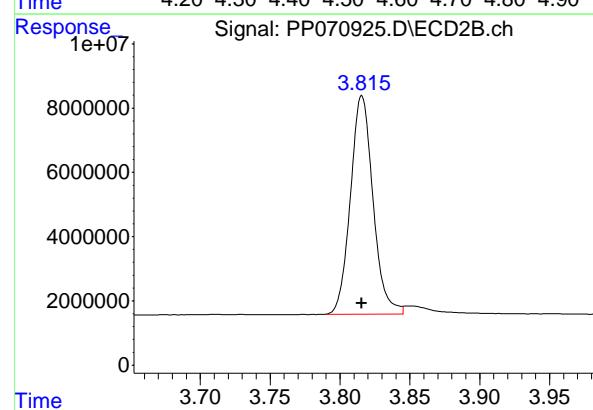


## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 76564298  
Conc: 68.37 ng/ml

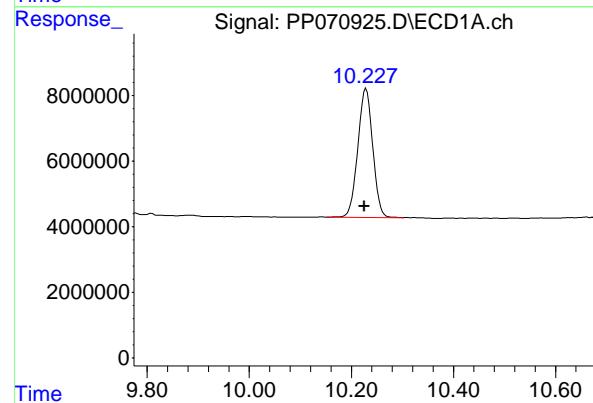





## #2 Decachlorobiphenyl

R.T.: 10.229 min  
Delta R.T.: 0.003 min  
Response: 79761677  
Conc: 72.10 ng/ml

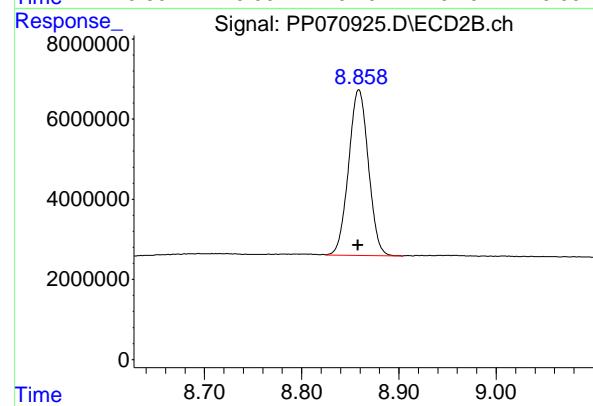

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 58459899  
Conc: 75.38 ng/ml

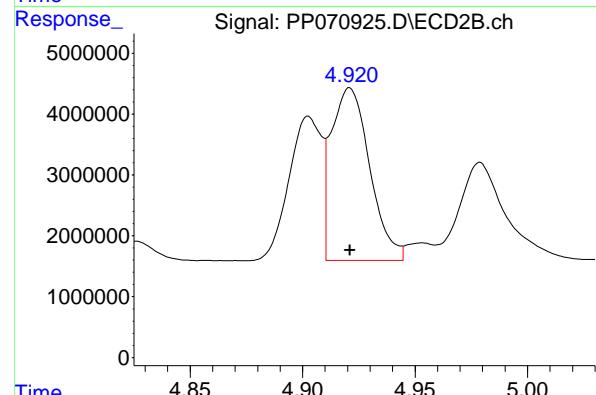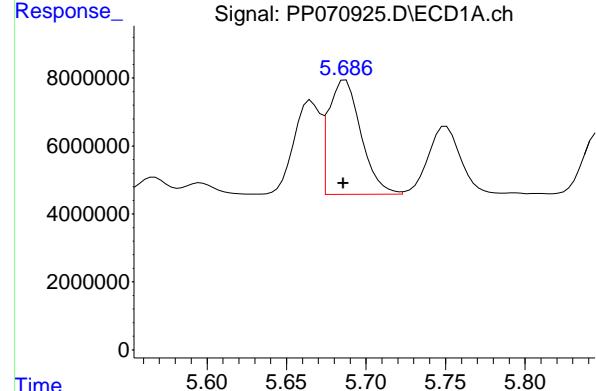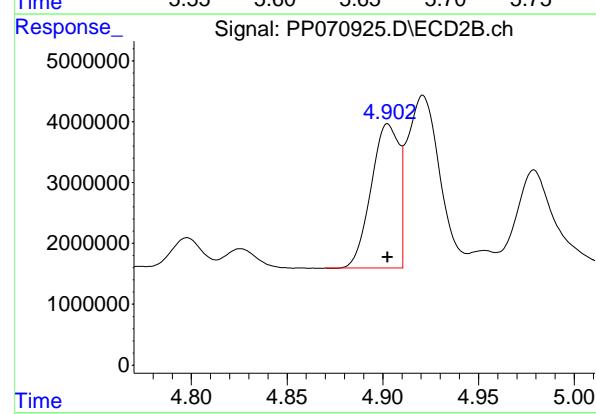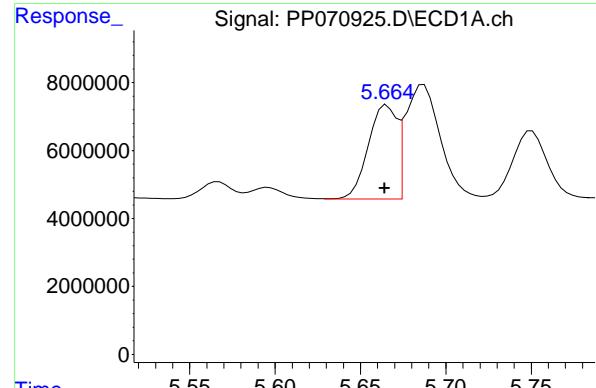

#16 AR-1242-1

R.T.: 5.666 min  
 Delta R.T.: 0.002 min  
 Instrument: ECD\_P  
 Response: 32059711  
 Conc: 738.15 ng/ml  
 ClientSampleId: AR1242ICC750

#16 AR-1242-1





R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 23829543  
 Conc: 687.73 ng/ml

#17 AR-1242-2

R.T.: 5.687 min  
 Delta R.T.: 0.001 min  
 Response: 47897203  
 Conc: 714.62 ng/ml

#17 AR-1242-2

R.T.: 4.921 min  
 Delta R.T.: 0.000 min  
 Response: 33806804  
 Conc: 683.87 ng/ml

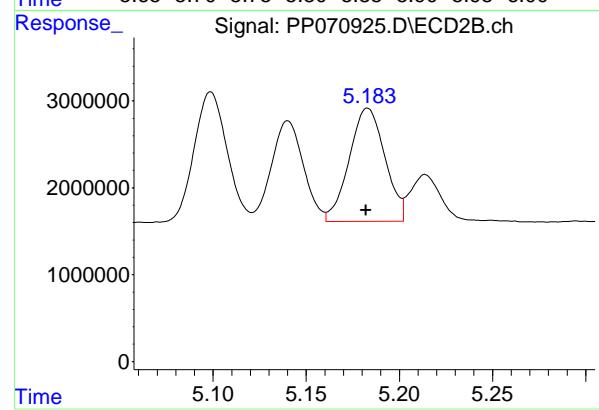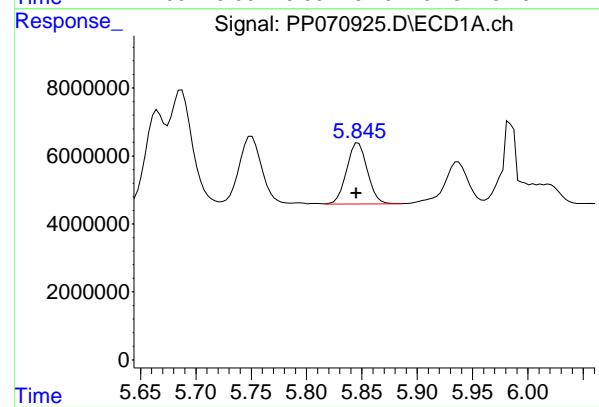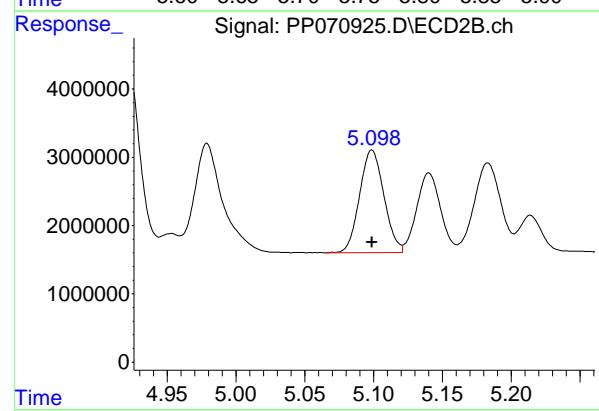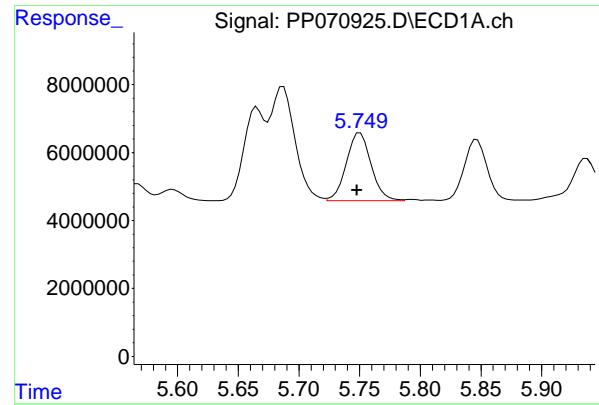

#18 AR-1242-3

R.T.: 5.750 min  
 Delta R.T.: 0.003 min  
 Response: 28536378 ECD\_P  
 Conc: 718.75 ng/ml ClientSampleId : AR1242ICC750

#18 AR-1242-3

R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 18473047  
 Conc: 693.98 ng/ml

#19 AR-1242-4



R.T.: 5.847 min  
 Delta R.T.: 0.002 min  
 Response: 23599640  
 Conc: 731.16 ng/ml

#19 AR-1242-4

R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 17369419  
 Conc: 678.98 ng/ml

#20 AR-1242-5

R.T.: 6.577 min  
Delta R.T.: 0.002 min  
Instrument: ECD\_P  
Response: 26235924  
Conc: 702.73 ng/ml  
ClientSampleId: AR1242ICC750

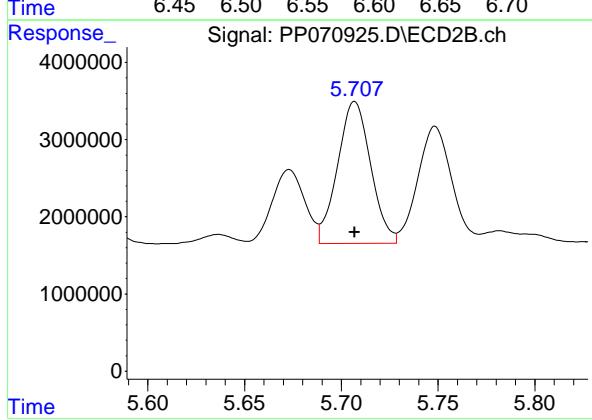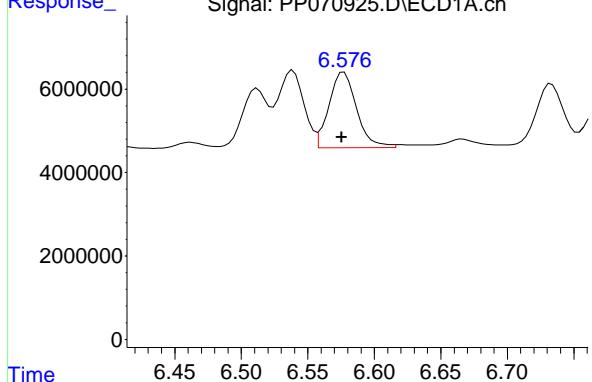

#20 AR-1242-5

R.T.: 5.707 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 21926365  
Conc: 694.78 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070926.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:00  
 Operator : YP\AJ  
 Sample : AR1242ICC500  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:28:40 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.511	3.815	76869856	55991243	50.000	50.000
2) SA Decachloro...	10.225	8.858	55314656	38777230	50.000	50.000

**Target Compounds**

16) L4 AR-1242-1	5.664	4.902	21716335	17324704	500.000	500.000
17) L4 AR-1242-2	5.686	4.921	33512438	24717400	500.000	500.000
18) L4 AR-1242-3	5.748	5.099	19851486	13309479	500.000	500.000
19) L4 AR-1242-4	5.845	5.182	16138543	12790769	500.000	500.000
20) L4 AR-1242-5	6.576	5.707	18667188	15779369	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.




Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070926.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:00  
 Operator : YP\AJ  
 Sample : AR1242ICC500  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:28:40 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

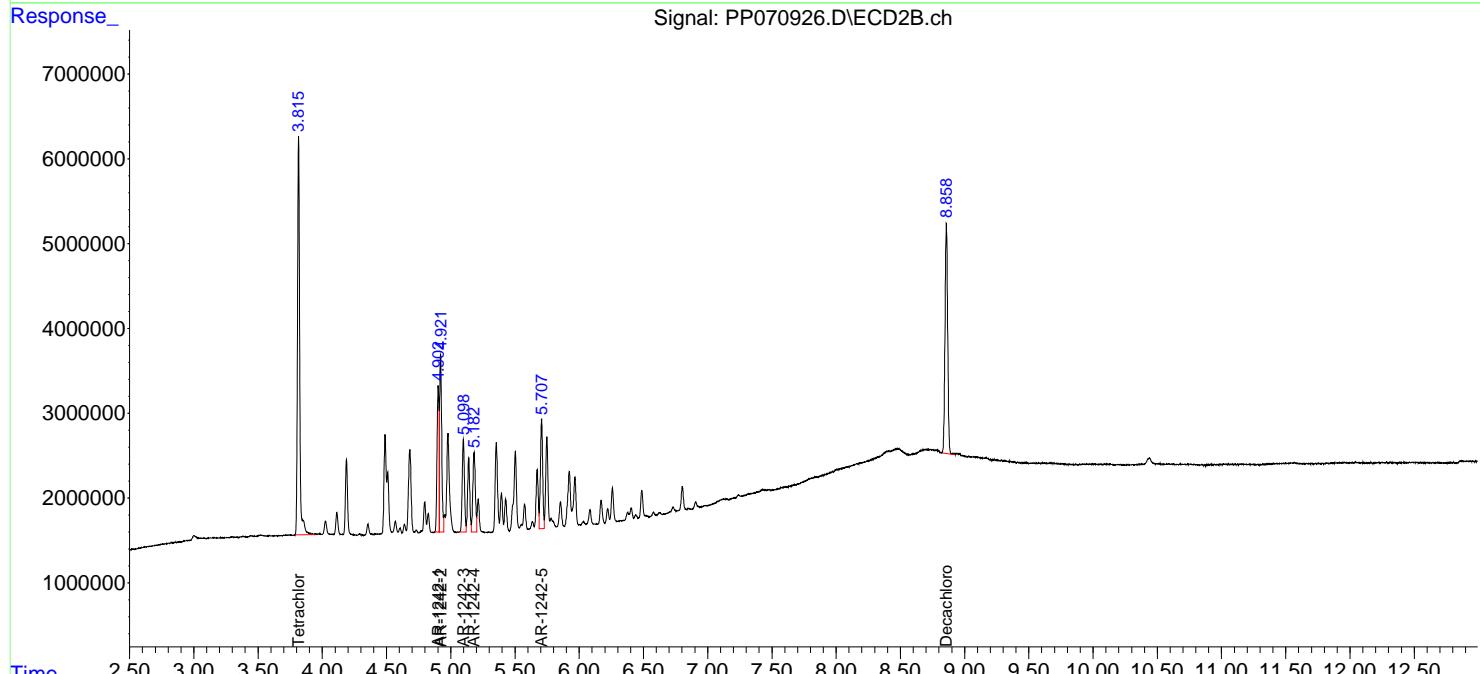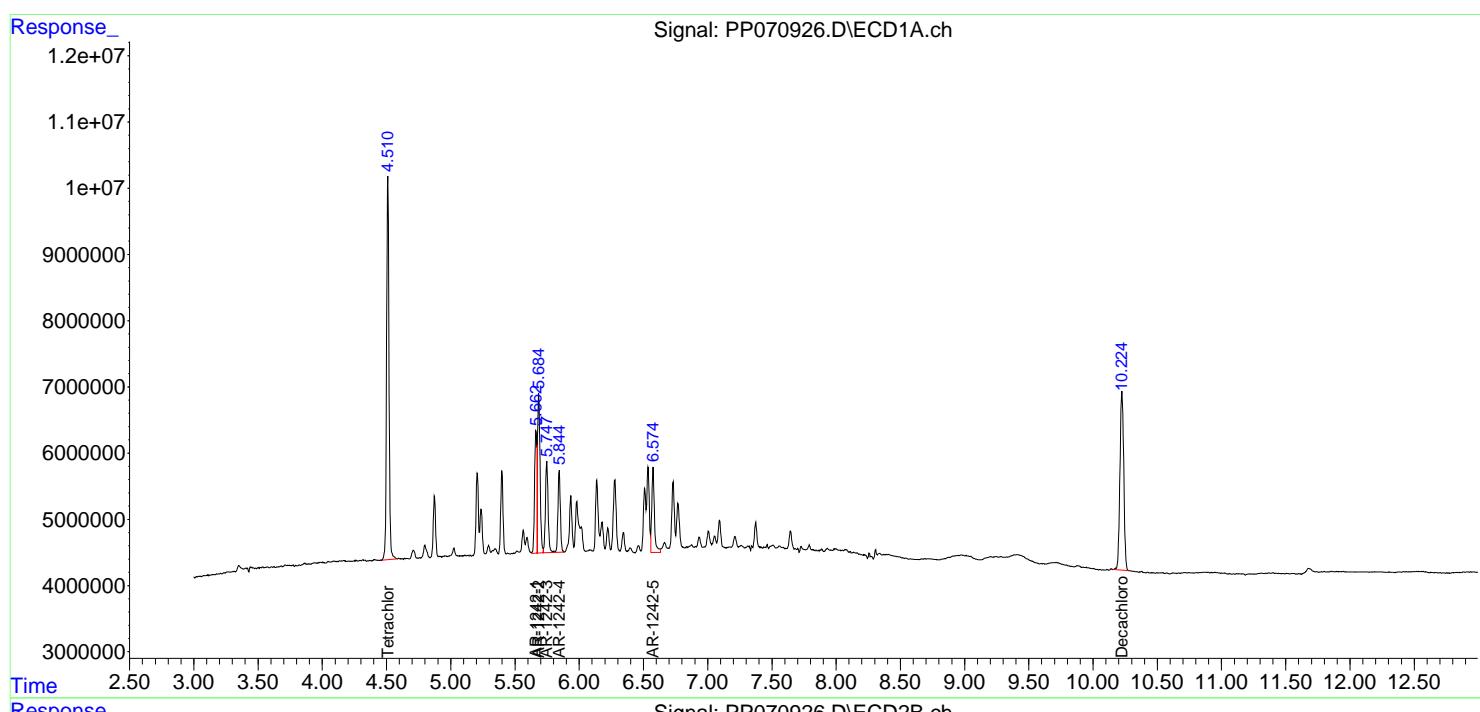

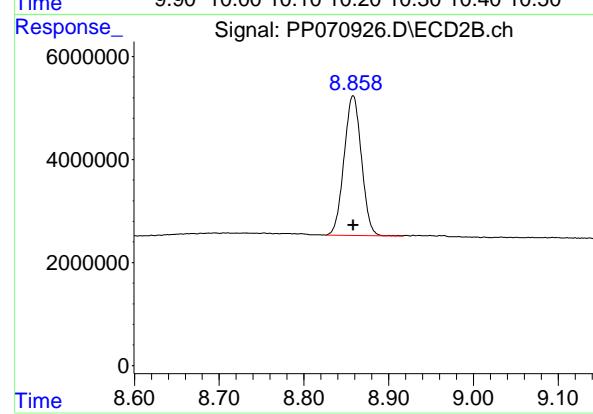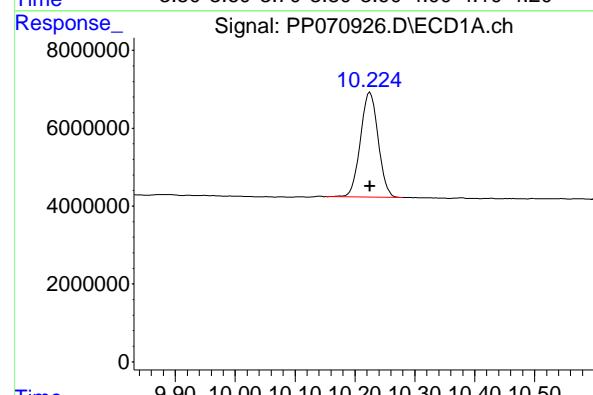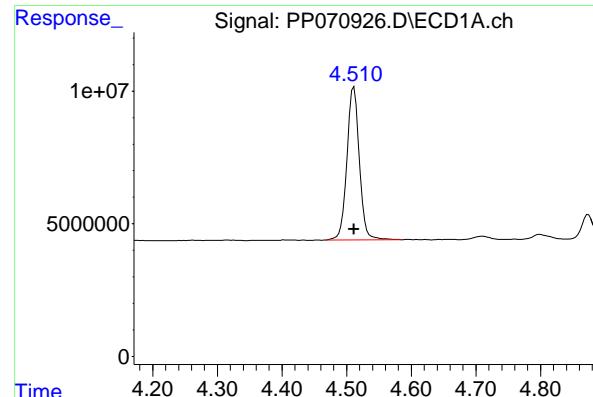

## #1 Tetrachloro-m-xylene

R.T.: 4.511 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 76869856  
Conc: 50.00 ng/ml ClientSampleId : AR1242ICC500

## #1 Tetrachloro-m-xylene





R.T.: 3.815 min  
Delta R.T.: 0.000 min  
Response: 55991243  
Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.225 min  
Delta R.T.: 0.000 min  
Response: 55314656  
Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.858 min  
Delta R.T.: 0.000 min  
Response: 38777230  
Conc: 50.00 ng/ml

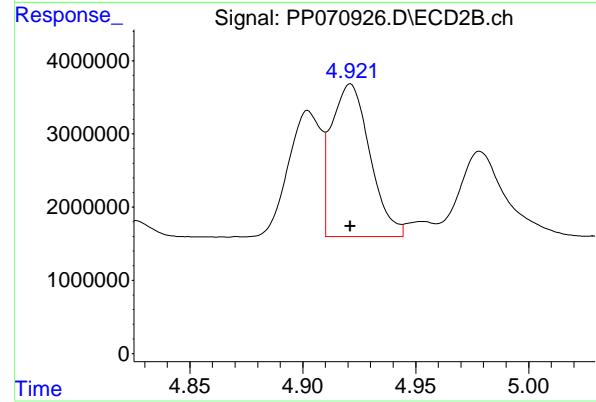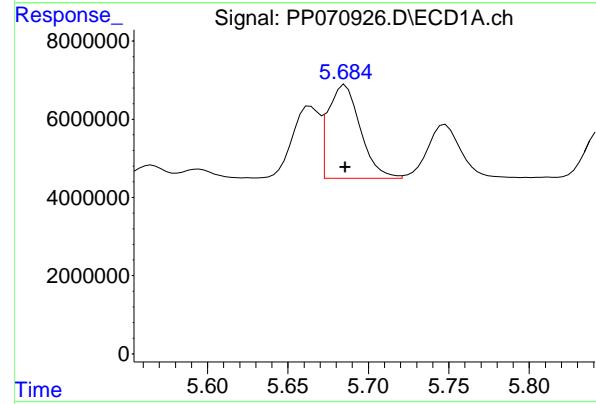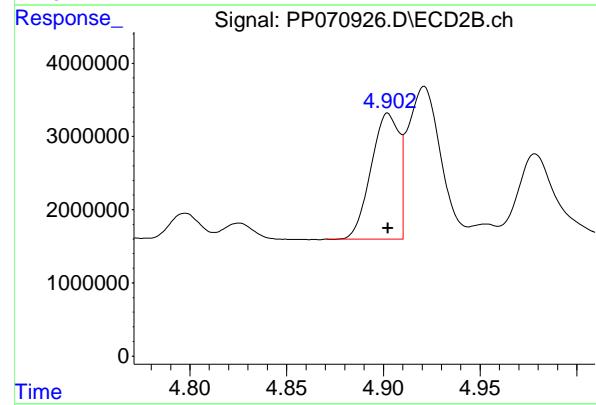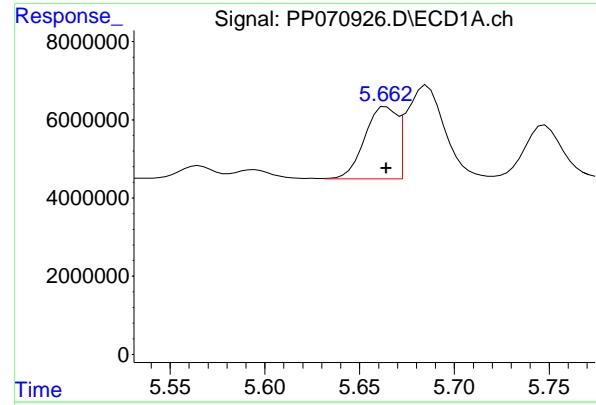

#16 AR-1242-1

R.T.: 5.664 min  
 Delta R.T.: 0.000 min  
 Response: 21716335  
 Conc: 500.00 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** AR1242ICC500

#16 AR-1242-1


R.T.: 4.902 min  
 Delta R.T.: 0.000 min  
 Response: 17324704  
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 5.686 min  
 Delta R.T.: 0.000 min  
 Response: 33512438  
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 4.921 min  
 Delta R.T.: 0.000 min  
 Response: 24717400  
 Conc: 500.00 ng/ml

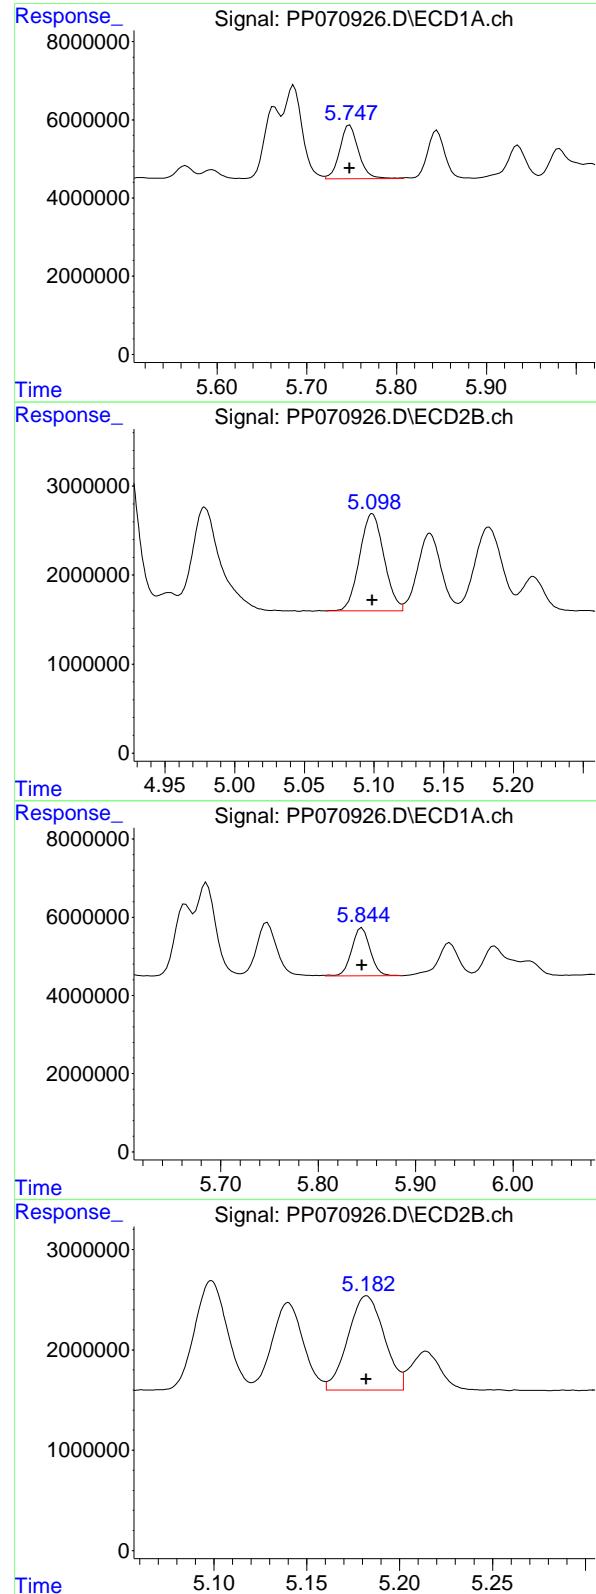

#18 AR-1242-3

R.T.: 5.748 min  
 Delta R.T.: 0.000 min  
 Response: 19851486 ECD\_P  
 Conc: 500.00 ng/ml ClientSampleId : AR1242ICC500

#18 AR-1242-3

R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 13309479  
 Conc: 500.00 ng/ml

#19 AR-1242-4


R.T.: 5.845 min  
 Delta R.T.: 0.000 min  
 Response: 16138543  
 Conc: 500.00 ng/ml

#19 AR-1242-4

R.T.: 5.182 min  
 Delta R.T.: 0.000 min  
 Response: 12790769  
 Conc: 500.00 ng/ml


#20 AR-1242-5

R.T.: 6.576 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 18667188  
Conc: 500.00 ng/ml  
ClientSampleId: AR1242ICC500

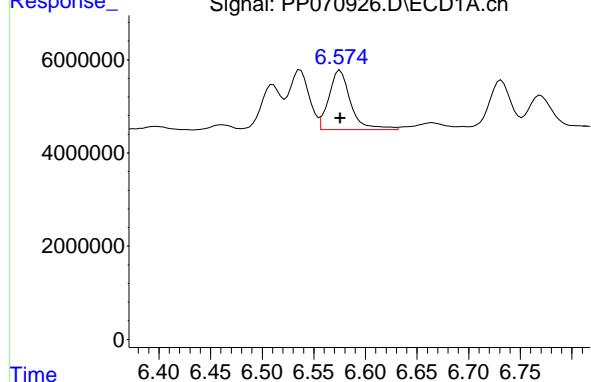

#20 AR-1242-5

R.T.: 5.707 min  
Delta R.T.: 0.000 min  
Response: 15779369  
Conc: 500.00 ng/ml

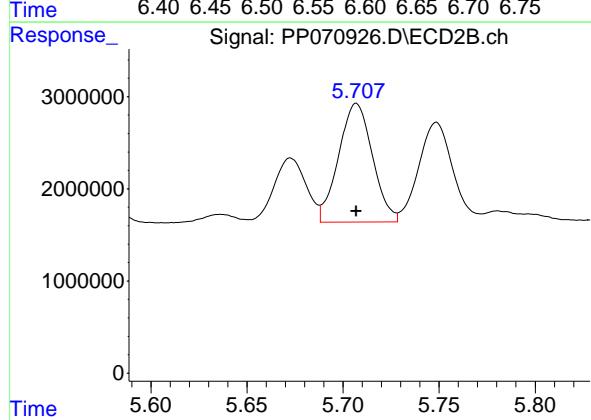

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070927.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:16  
 Operator : YP\AJ  
 Sample : AR1242ICC250  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:36:45 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.514	3.816	39179148	28013392	25.484	25.016
2) SA Decachloro...	10.230	8.858	28836317	21287334	26.066	27.448

**Target Compounds**

16) L4 AR-1242-1	5.666	4.903	10996159	9674680	253.177	279.216
17) L4 AR-1242-2	5.688	4.922	17212597	13875945	256.809	280.692
18) L4 AR-1242-3	5.750	5.099	10156885	7458368	255.822	280.190
19) L4 AR-1242-4	5.847	5.183	8048661	7154684	249.361	279.682
20) L4 AR-1242-5	6.578	5.708	9640099	8240601	258.210	261.119


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070927.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:16  
 Operator : YP\AJ  
 Sample : AR1242ICC250  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:36:45 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

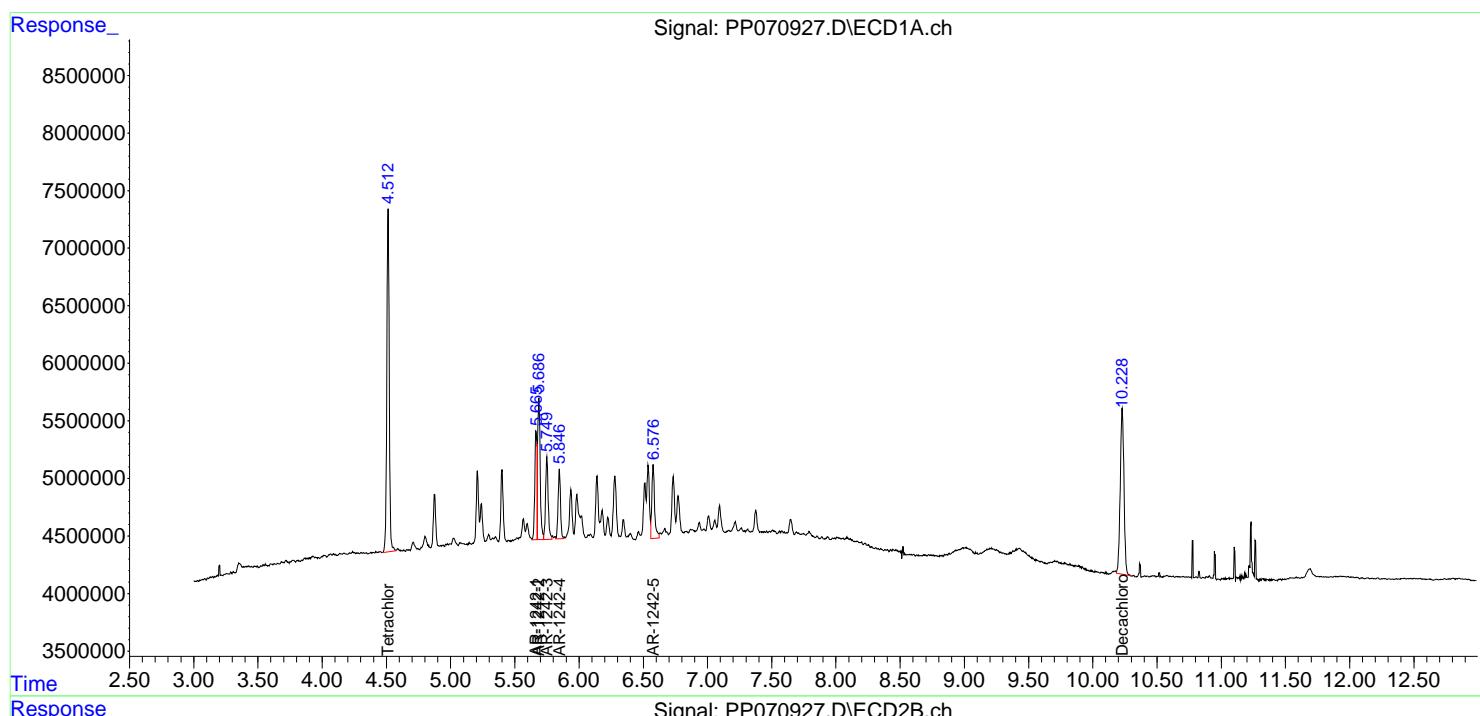

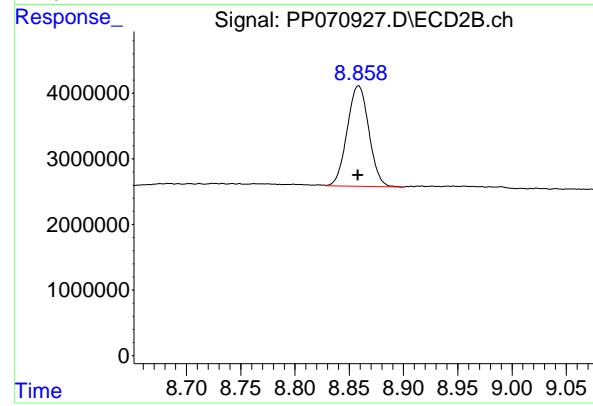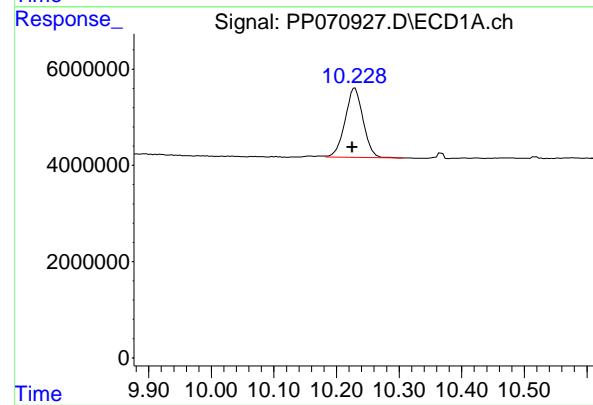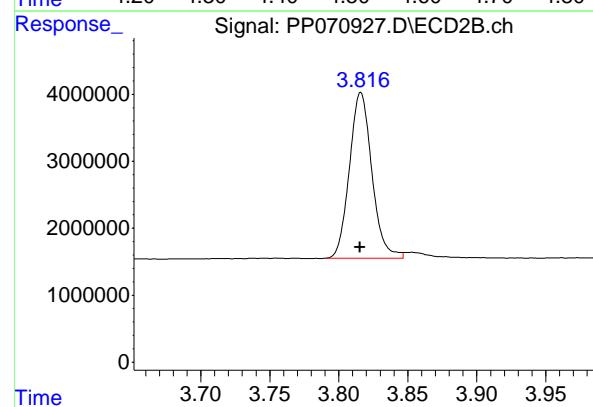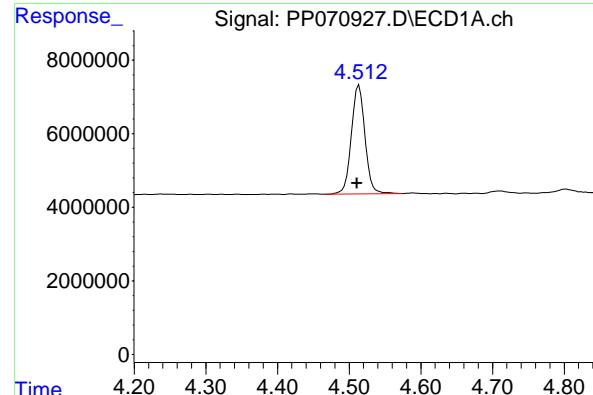

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
 Delta R.T.: 0.003 min  
 Response: 39179148 ECD\_P  
 Conc: 25.48 ng/ml ClientSampleId : AR1242ICC250

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 28013392  
 Conc: 25.02 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.230 min  
 Delta R.T.: 0.004 min  
 Response: 28836317  
 Conc: 26.07 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.858 min  
 Delta R.T.: 0.000 min  
 Response: 21287334  
 Conc: 27.45 ng/ml

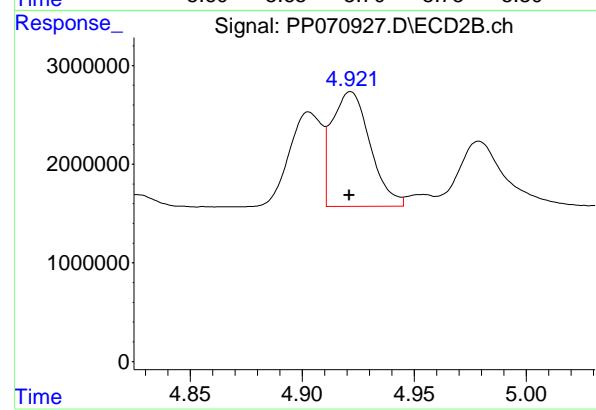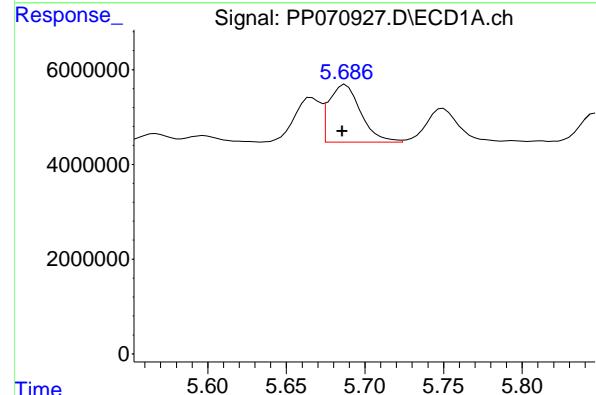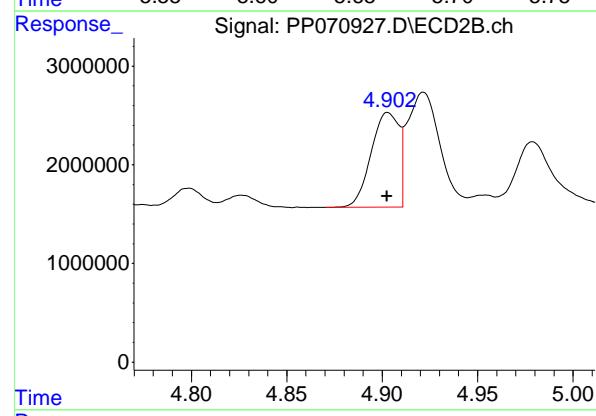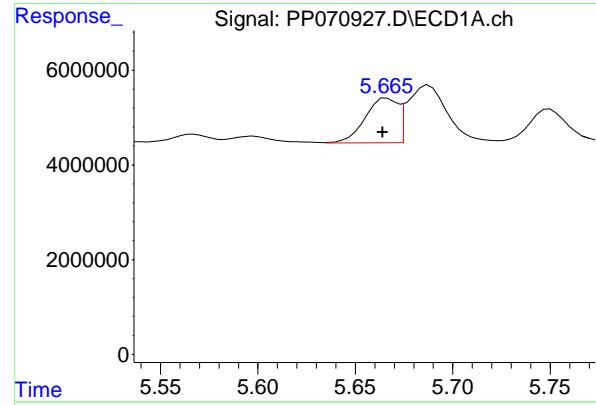

#16 AR-1242-1

R.T.: 5.666 min  
 Delta R.T.: 0.002 min  
 Response: 10996159 ECD\_P  
 Conc: 253.18 ng/ml ClientSampleId : AR1242ICC250

#16 AR-1242-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 9674680  
 Conc: 279.22 ng/ml

#17 AR-1242-2


R.T.: 5.688 min  
 Delta R.T.: 0.002 min  
 Response: 17212597  
 Conc: 256.81 ng/ml

#17 AR-1242-2

R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 13875945  
 Conc: 280.69 ng/ml


#18 AR-1242-3

R.T.: 5.750 min  
 Delta R.T.: 0.002 min  
 Response: 10156885 ECD\_P  
 Conc: 255.82 ng/ml ClientSampleId : AR1242ICC250

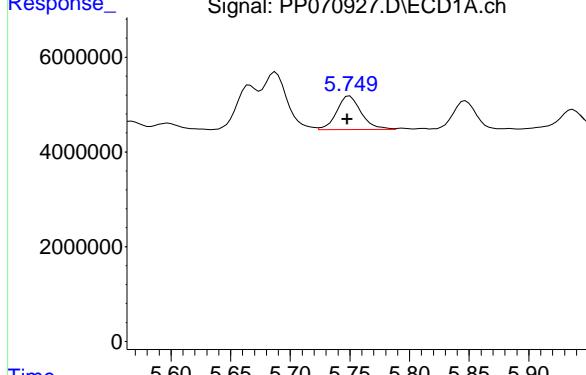


#18 AR-1242-3

R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 7458368  
 Conc: 280.19 ng/ml

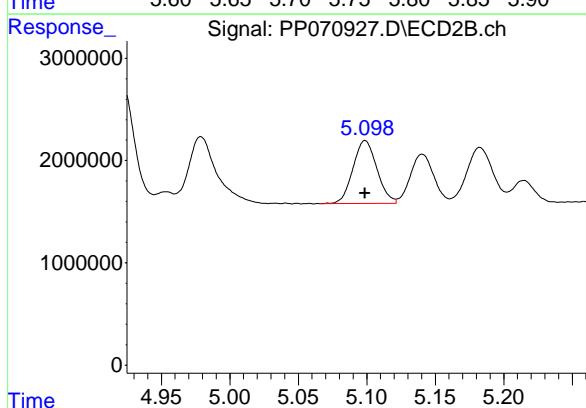


#19 AR-1242-4


R.T.: 5.847 min  
 Delta R.T.: 0.002 min  
 Response: 8048661  
 Conc: 249.36 ng/ml

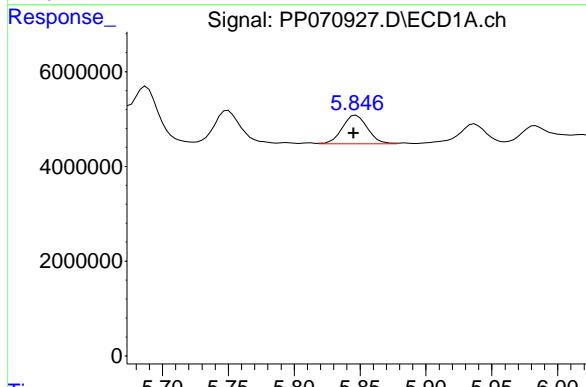

#19 AR-1242-4

R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 7154684  
 Conc: 279.68 ng/ml

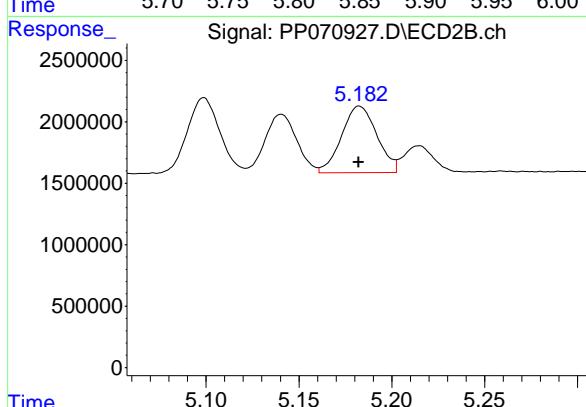

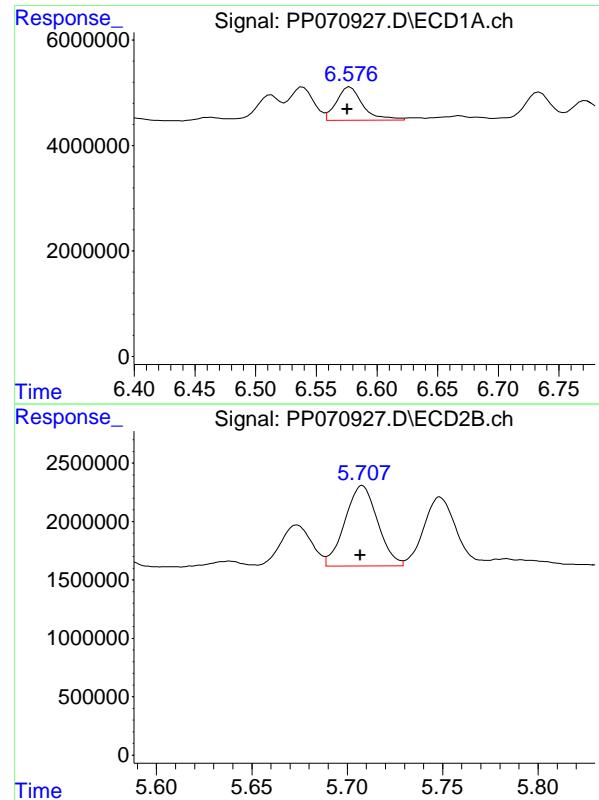

#20 AR-1242-5

R.T.: 6.578 min  
Delta R.T.: 0.002 min  
Instrument: ECD\_P  
Response: 9640099  
Conc: 258.21 ng/ml  
ClientSampleId: AR1242ICC250

#20 AR-1242-5

R.T.: 5.708 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 8240601  
Conc: 261.12 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070928.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:33  
 Operator : YP\AJ  
 Sample : AR1242ICC050  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC050**

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:57:16 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	4.512	3.815	6633492	5532966	4.273	4.939
2) SA Decachlor...	10.226	8.857	5282830	3387334	4.676	4.164

**Target Compounds**

16) L4 AR-1242-1	5.663	4.902	2436604	1773341	55.746m	48.354
17) L4 AR-1242-2	5.686	4.921	2856942	2619762	42.052m	49.929m
18) L4 AR-1242-3	5.748	5.098	2373419	1401755	59.091m	49.661
19) L4 AR-1242-4	5.843	5.181	1293211	1572257	40.117m	58.017m#
20) L4 AR-1242-5	6.574	5.705	1783487	1619372	46.999m	50.197m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070928.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:33  
 Operator : YP\AJ  
 Sample : AR1242ICC050  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1


Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1242ICC050


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:57:16 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

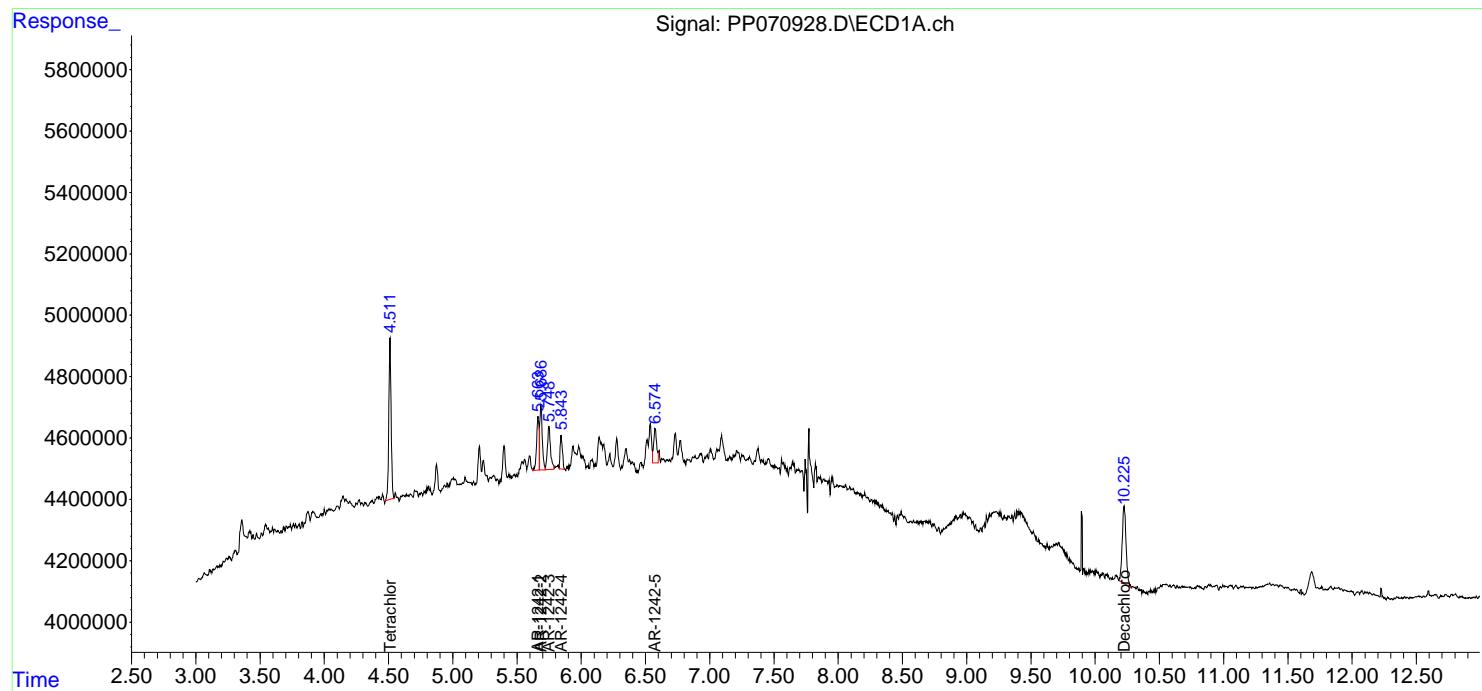

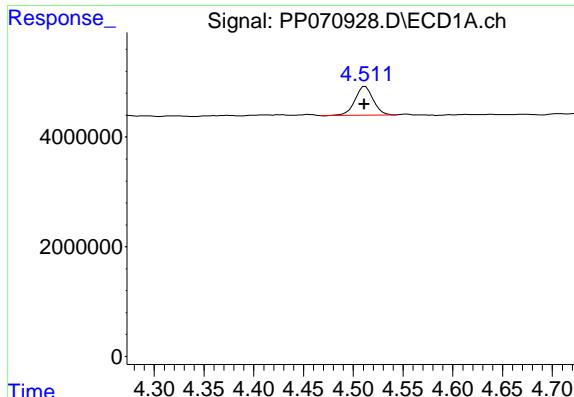


## #1 Tetrachloro-m-xylene

R.T.: 4.512 min  
Delta R.T.: 0.001 min  
Instrument:  
Response: 6633492 ECD\_P  
Conc: 4.27 ng/ml ClientSampleId : AR1242ICC050


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

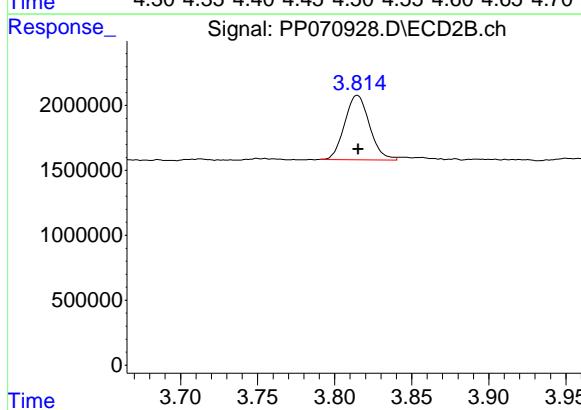


## #1 Tetrachloro-m-xylene

R.T.: 3.815 min  
Delta R.T.: 0.000 min  
Response: 5532966  
Conc: 4.94 ng/ml

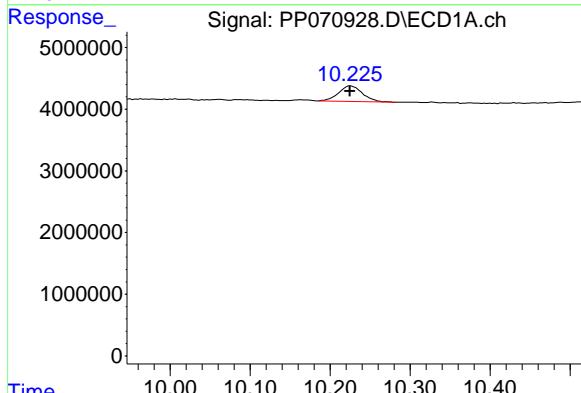


## #2 Decachlorobiphenyl

R.T.: 10.226 min  
Delta R.T.: 0.000 min  
Response: 5282830  
Conc: 4.68 ng/ml

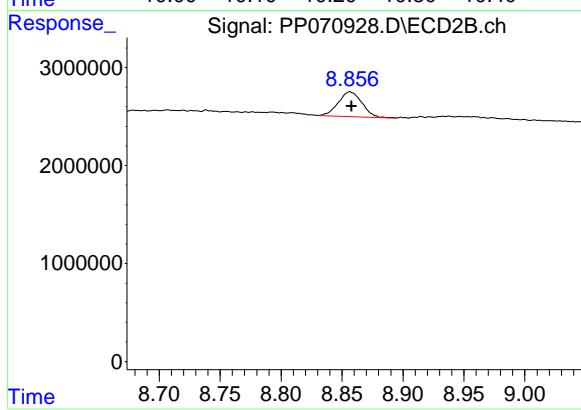

## #2 Decachlorobiphenyl

R.T.: 8.857 min  
Delta R.T.: -0.001 min  
Response: 3387334  
Conc: 4.16 ng/ml

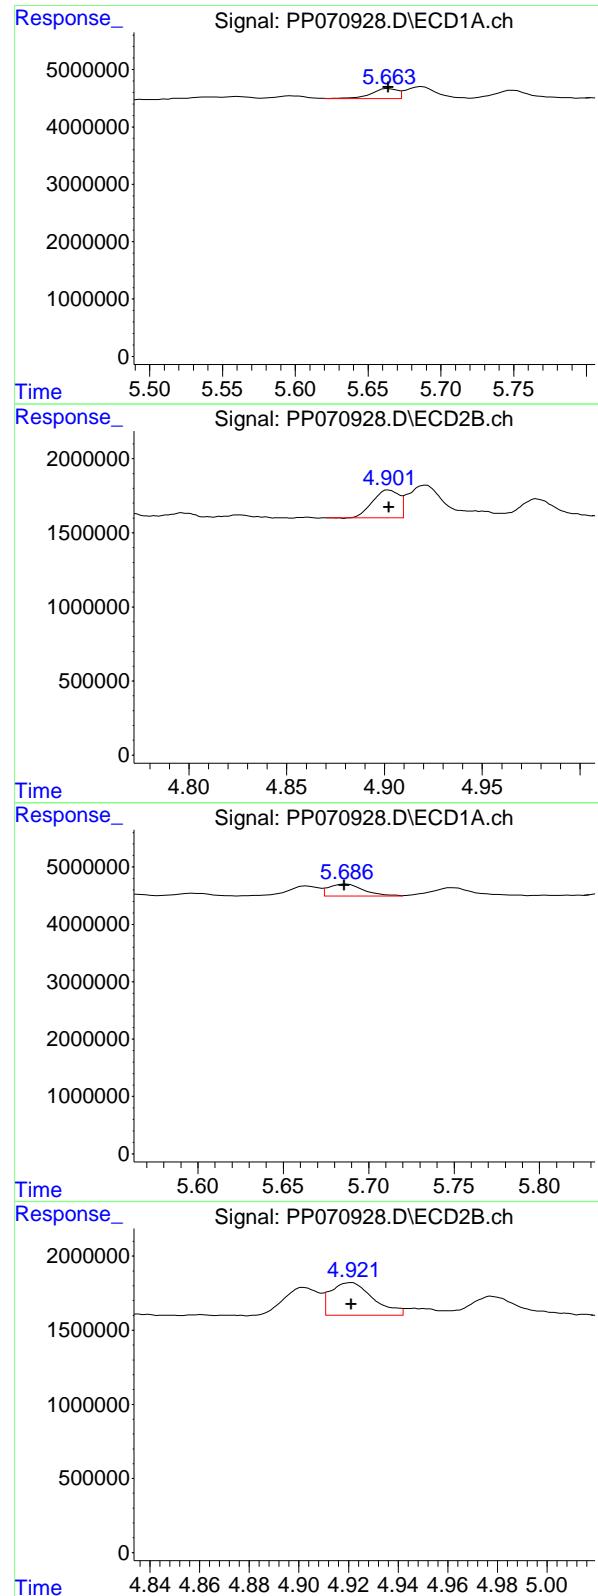

#16 AR-1242-1

R.T.: 5.663 min  
 Delta R.T.: -0.002 min  
 Response: 2436604 ECD\_P  
 Conc: 55.75 ng/ml ClientSampleId : AR1242ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#16 AR-1242-1


R.T.: 4.902 min  
 Delta R.T.: 0.000 min  
 Response: 1773341  
 Conc: 48.35 ng/ml

#17 AR-1242-2

R.T.: 5.686 min  
 Delta R.T.: 0.000 min  
 Response: 2856942  
 Conc: 42.05 ng/ml

#17 AR-1242-2

R.T.: 4.921 min  
 Delta R.T.: 0.000 min  
 Response: 2619762  
 Conc: 49.93 ng/ml

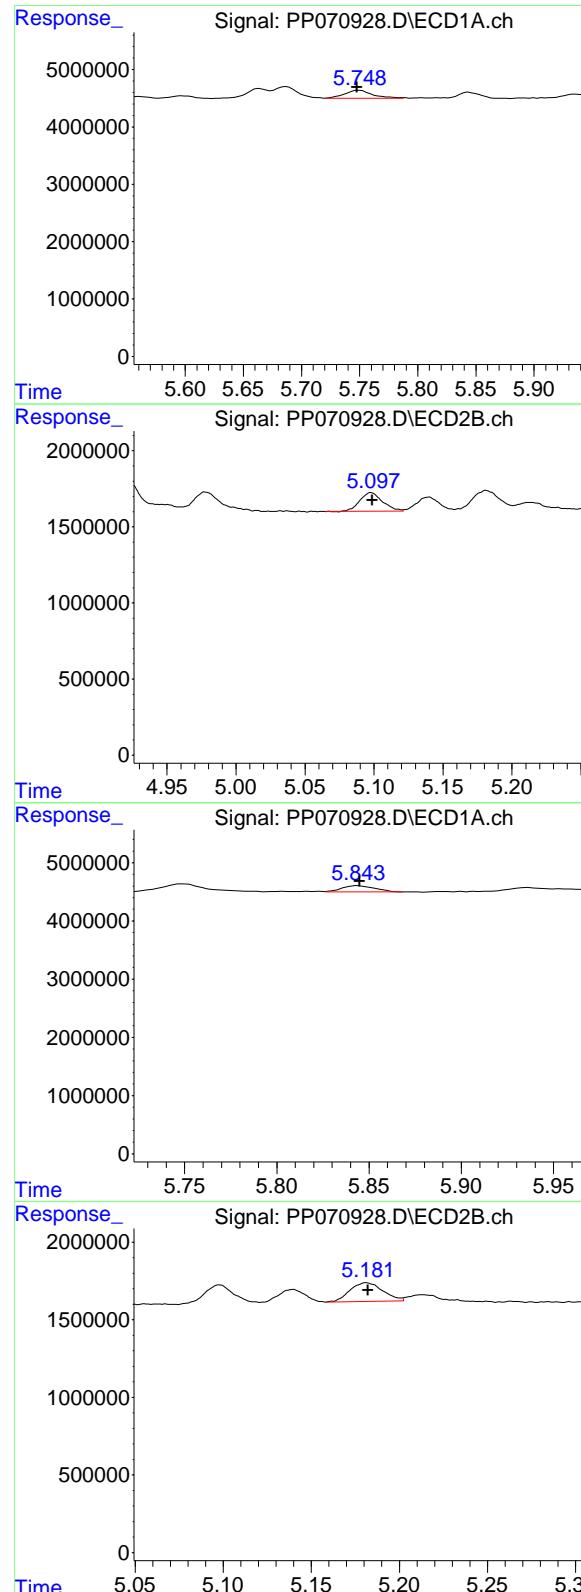

#18 AR-1242-3

R.T.: 5.748 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_P  
 Response: 2373419  
 Conc: 59.09 ng/ml Client SampleId : AR1242ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#18 AR-1242-3

R.T.: 5.098 min  
 Delta R.T.: 0.000 min  
 Response: 1401755  
 Conc: 49.66 ng/ml

#19 AR-1242-4

R.T.: 5.843 min  
 Delta R.T.: -0.002 min  
 Response: 1293211  
 Conc: 40.12 ng/ml

#19 AR-1242-4

R.T.: 5.181 min  
 Delta R.T.: -0.002 min  
 Response: 1572257  
 Conc: 58.02 ng/ml

#20 AR-1242-5


R.T.: 6.574 min  
 Delta R.T.: -0.002 min  
 Response: 1783487 ECD\_P  
 Conc: 47.00 ng/ml ClientSampleId :  
 AR1242ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#20 AR-1242-5

R.T.: 5.705 min  
 Delta R.T.: -0.001 min  
 Response: 1619372  
 Conc: 50.20 ng/ml

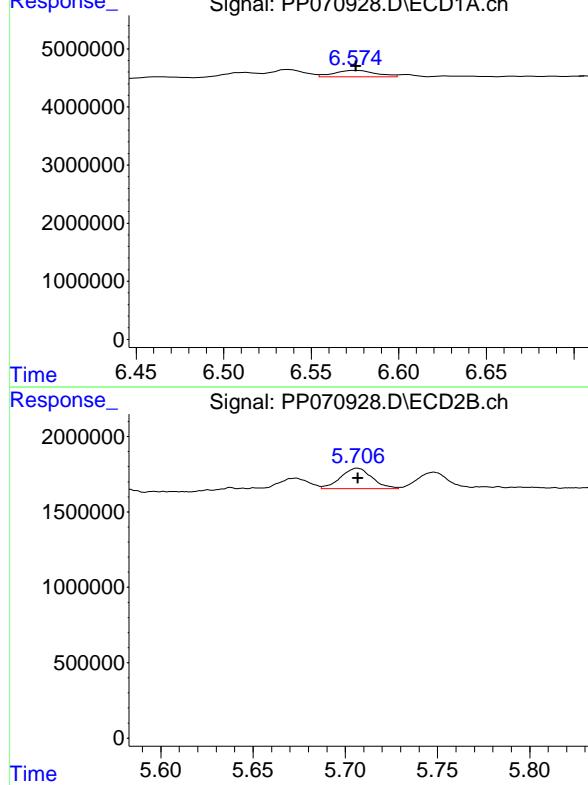

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070929.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:49  
 Operator : YP\AJ  
 Sample : AR1248ICC1000  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 14:45:43 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 14:45:17 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.514	3.816	146.2E6	96952216	94.393	85.183
2) SA Decachlor...	10.229	8.859	107.2E6	76343240	88.954	92.303

Target Compounds

21) L5 AR-1248-1	5.666	4.903	31141042	23297586	921.836	817.423
22) L5 AR-1248-2	5.938	5.141	42399779	31071420	917.898	811.806
23) L5 AR-1248-3	6.140	5.183	48055172	32592570	927.258	815.546
24) L5 AR-1248-4	6.539	5.355	59878410	38114246	893.176	807.817
25) L5 AR-1248-5	6.579	5.749	56652876	37031094	881.261	843.047


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070929.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:49  
 Operator : YP\AJ  
 Sample : AR1248ICC1000  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
AR1248ICC1000

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 14:45:43 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 14:45:17 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

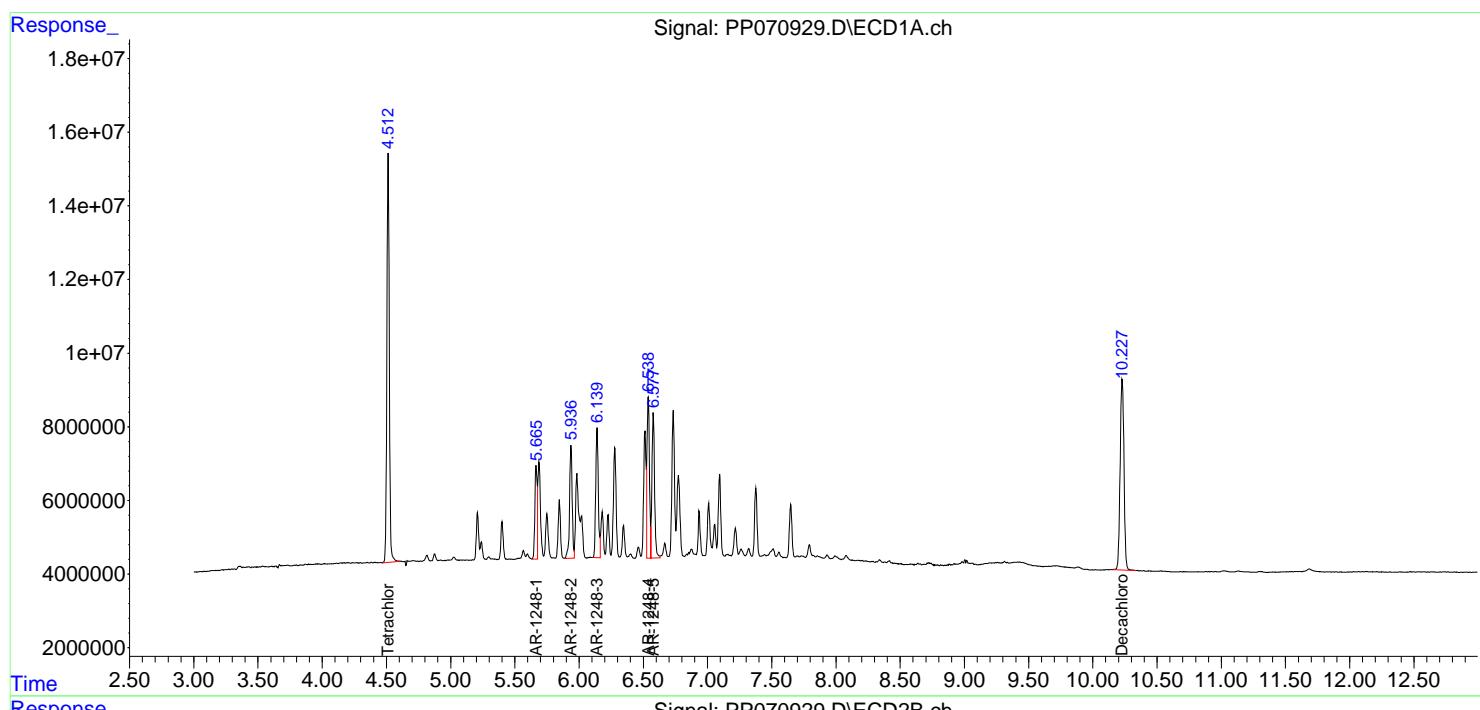

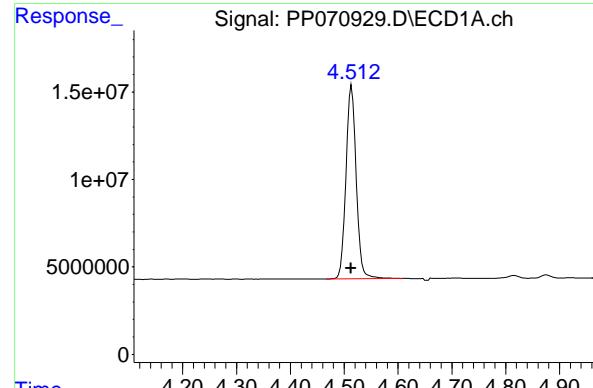


## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 146218105  
Conc: 94.39 ng/ml  
ClientSampleId: AR1248ICC1000

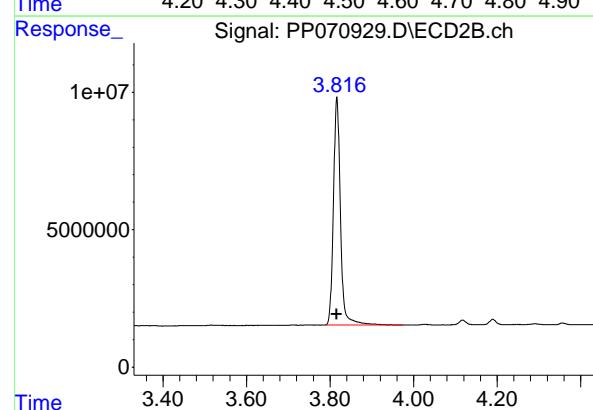


## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 96952216  
Conc: 85.18 ng/ml

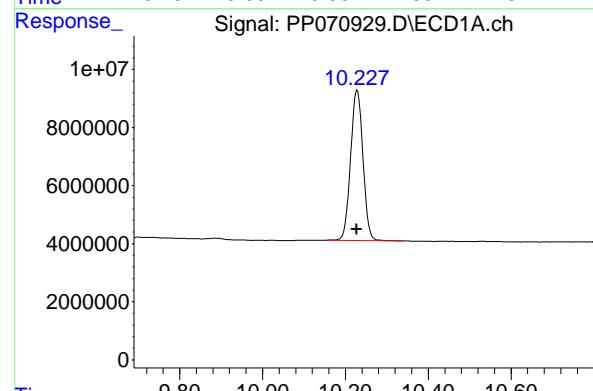





## #2 Decachlorobiphenyl

R.T.: 10.229 min  
Delta R.T.: 0.002 min  
Response: 107201730  
Conc: 88.95 ng/ml

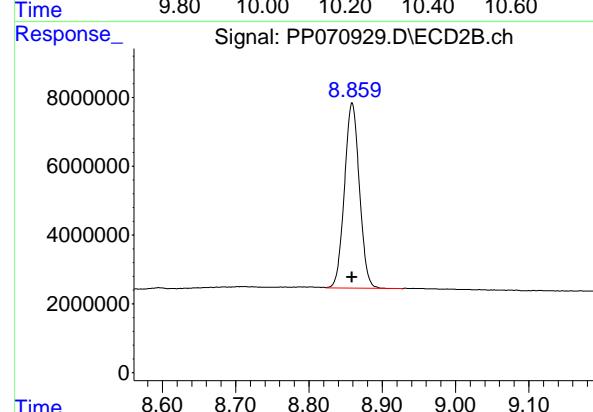

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 76343240  
Conc: 92.30 ng/ml

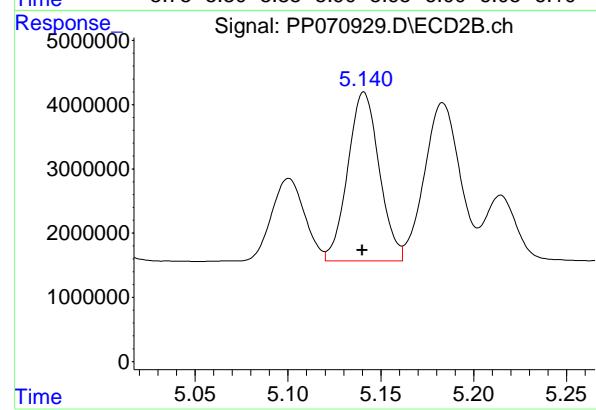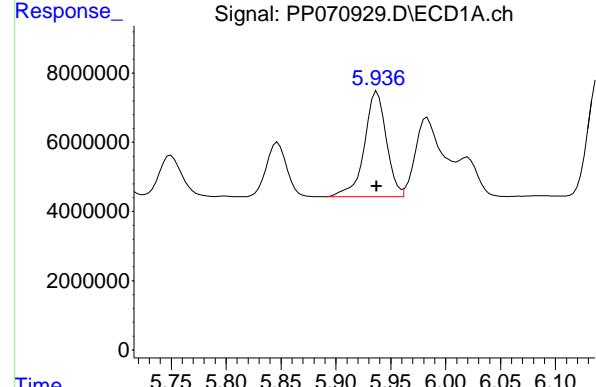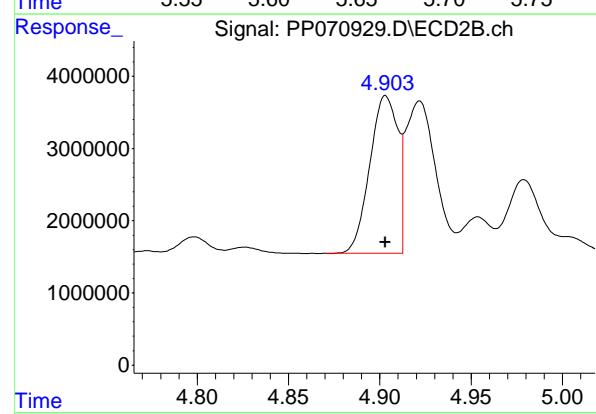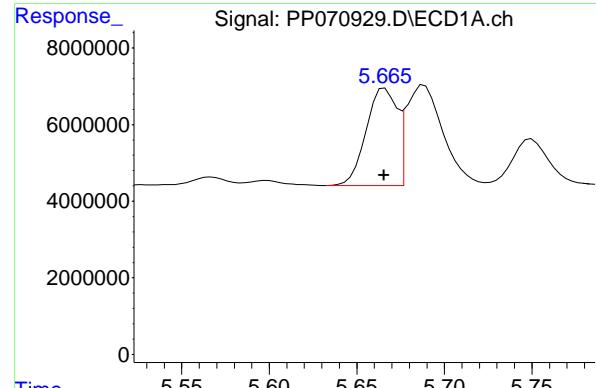

#21 AR-1248-1

R.T.: 5.666 min  
 Delta R.T.: 0.000 min  
 Response: 31141042 ECD\_P  
 Conc: 921.84 ng/ml ClientSampleId : AR1248ICC1000

#21 AR-1248-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 23297586  
 Conc: 817.42 ng/ml

#22 AR-1248-2


R.T.: 5.938 min  
 Delta R.T.: 0.000 min  
 Response: 42399779  
 Conc: 917.90 ng/ml

#22 AR-1248-2

R.T.: 5.141 min  
 Delta R.T.: 0.000 min  
 Response: 31071420  
 Conc: 811.81 ng/ml


#23 AR-1248-3

R.T.: 6.140 min  
 Delta R.T.: 0.000 min  
 Response: 48055172 ECD\_P  
 Conc: 927.26 ng/ml ClientSampleId : AR1248ICC1000

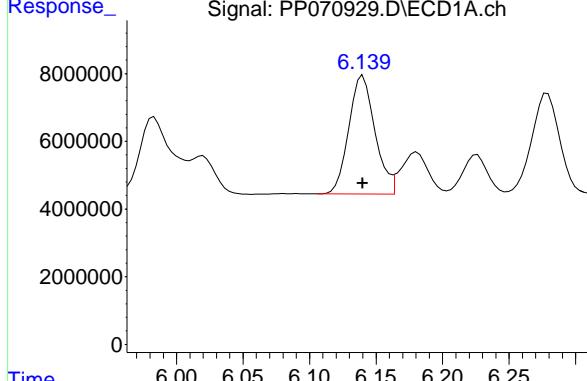


#23 AR-1248-3

R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 32592570  
 Conc: 815.55 ng/ml

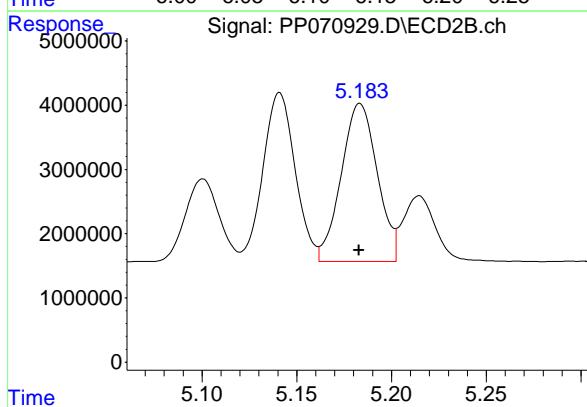


#24 AR-1248-4

R.T.: 6.539 min  
 Delta R.T.: 0.000 min  
 Response: 59878410  
 Conc: 893.18 ng/ml

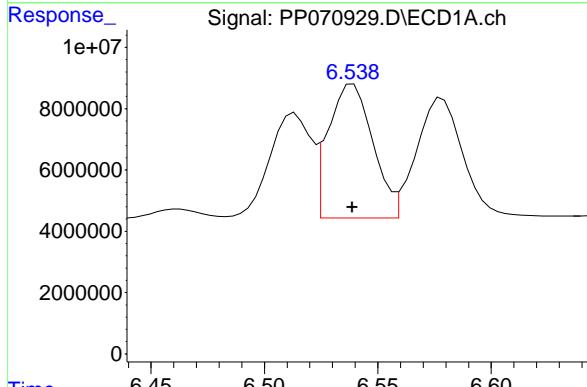


#24 AR-1248-4

R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 38114246  
 Conc: 807.82 ng/ml

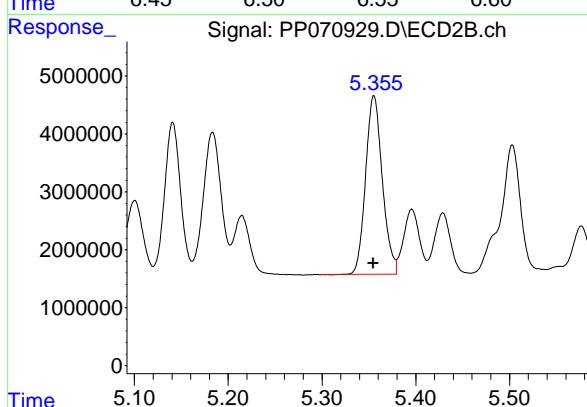


#25 AR-1248-5

R.T.: 6.579 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 56652876  
Conc: 881.26 ng/ml  
ClientSampleId: AR1248ICC1000

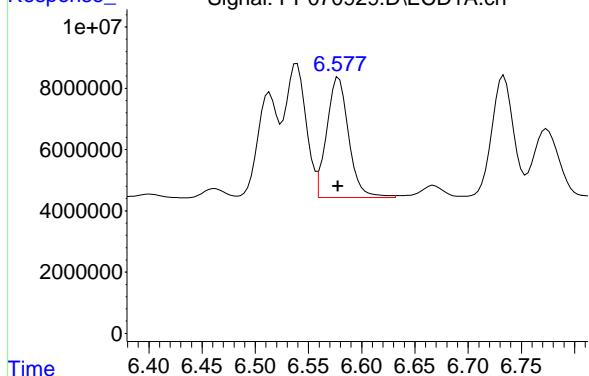

#25 AR-1248-5

R.T.: 5.749 min  
Delta R.T.: 0.000 min  
Response: 37031094  
Conc: 843.05 ng/ml

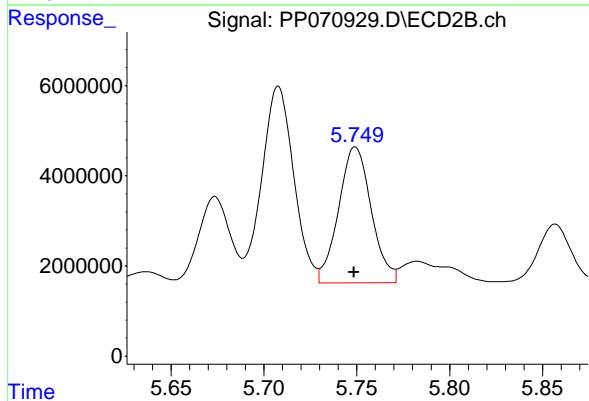

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070930.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:05  
 Operator : YP\AJ  
 Sample : AR1248ICC750  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 14:46:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 14:45:17 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	4.514	3.816	115.8E6	78436191	74.760	68.915
2) SA Decachlor...	10.229	8.860	84334663	61664461	69.979	74.555

**Target Compounds**

21) L5 AR-1248-1	5.666	4.903	25034469	20052758	741.070	703.575
22) L5 AR-1248-2	5.938	5.141	33734311	26938678	730.302	703.829
23) L5 AR-1248-3	6.140	5.183	38083098	28275820	734.840	707.530
24) L5 AR-1248-4	6.539	5.356	47603456	32558799	710.077	690.072
25) L5 AR-1248-5	6.578	5.749	45378306	30836259	705.880	702.016



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070930.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:05  
 Operator : YP\AJ  
 Sample : AR1248ICC750  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 14:46:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 14:45:17 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

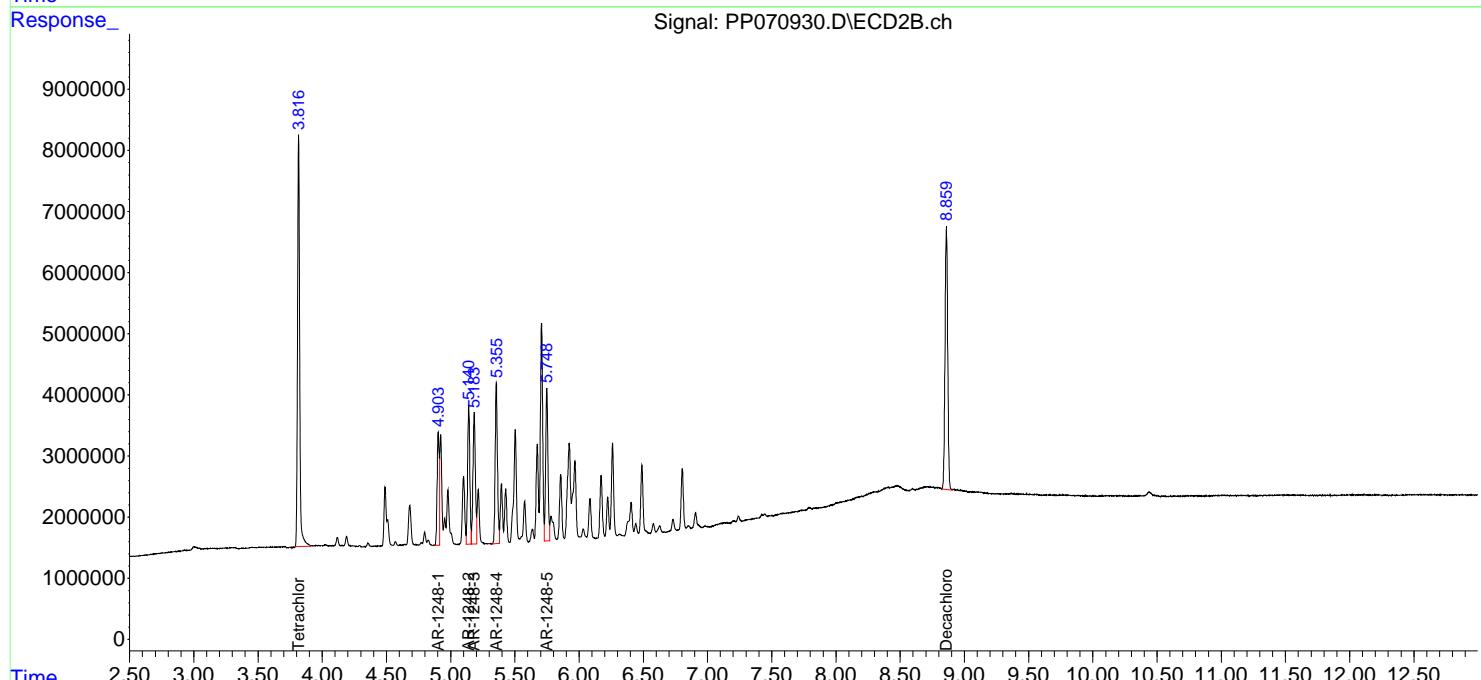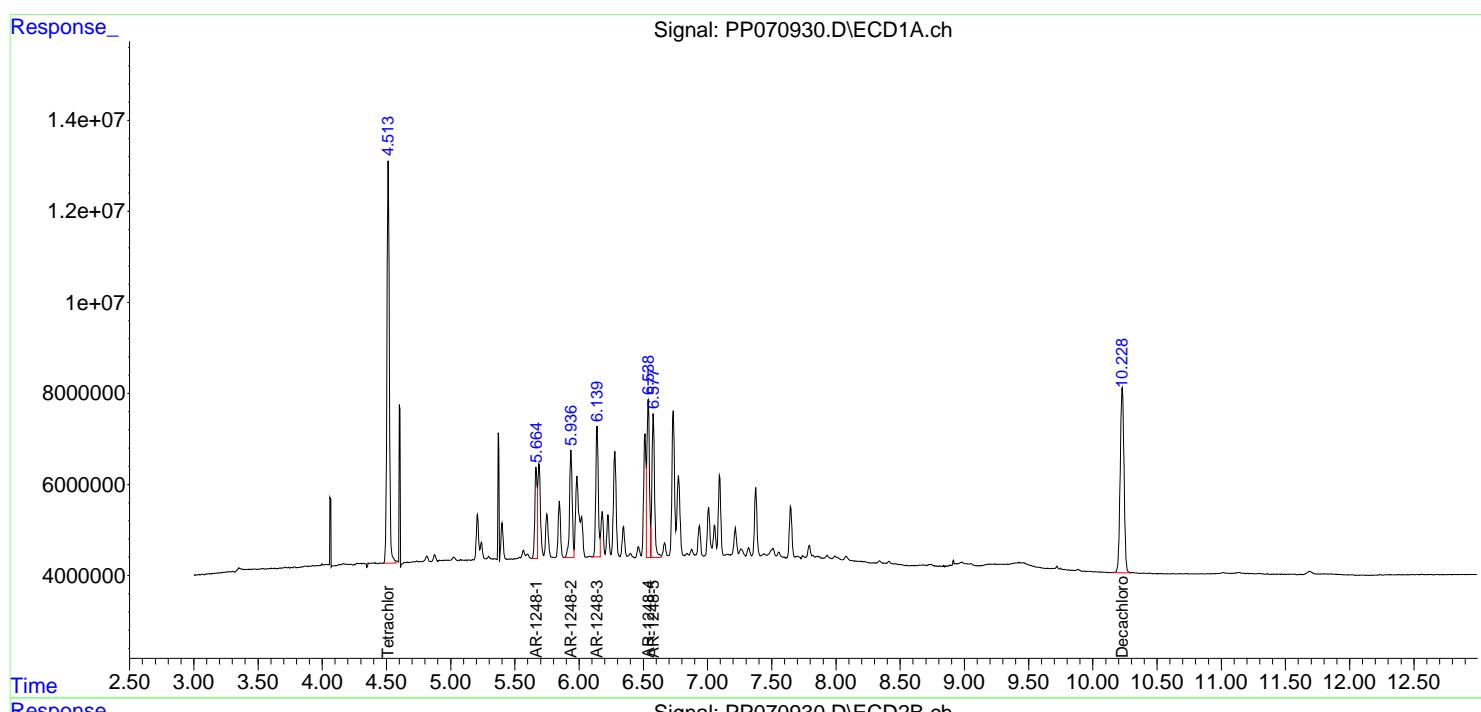

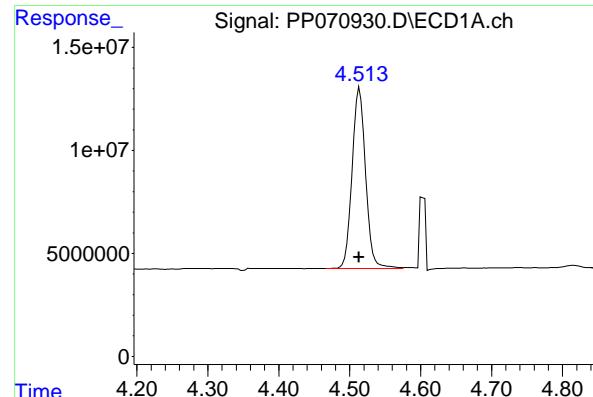


## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 115806846  
Conc: 74.76 ng/ml ClientSampleId : AR1248ICC750

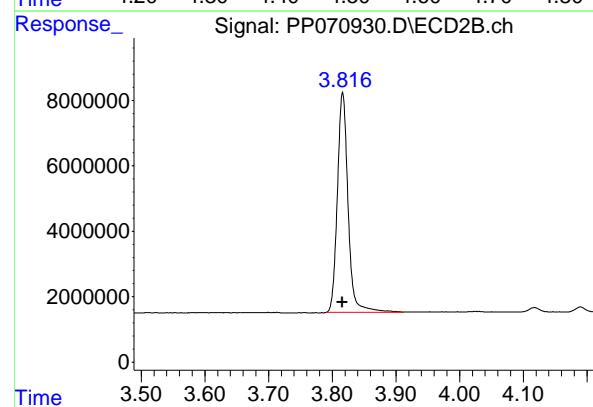


## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 78436191  
Conc: 68.91 ng/ml

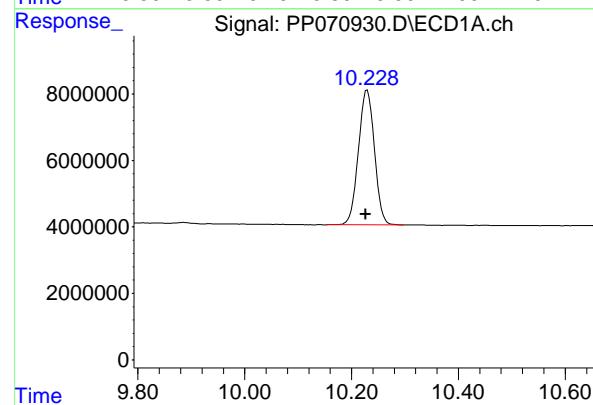





## #2 Decachlorobiphenyl

R.T.: 10.229 min  
Delta R.T.: 0.003 min  
Response: 84334663  
Conc: 69.98 ng/ml

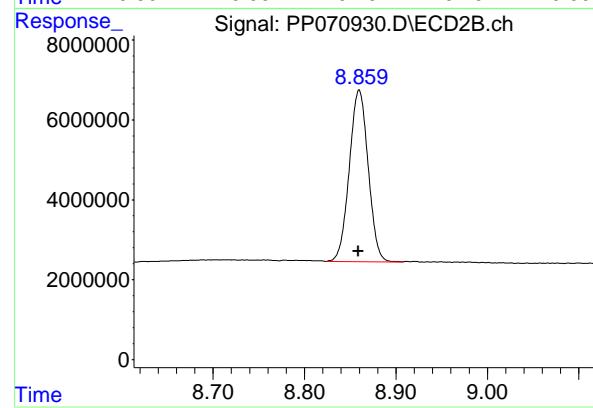

## #2 Decachlorobiphenyl

R.T.: 8.860 min  
Delta R.T.: 0.000 min  
Response: 61664461  
Conc: 74.56 ng/ml

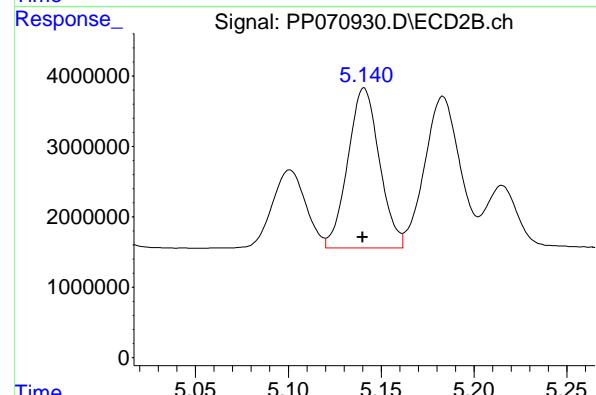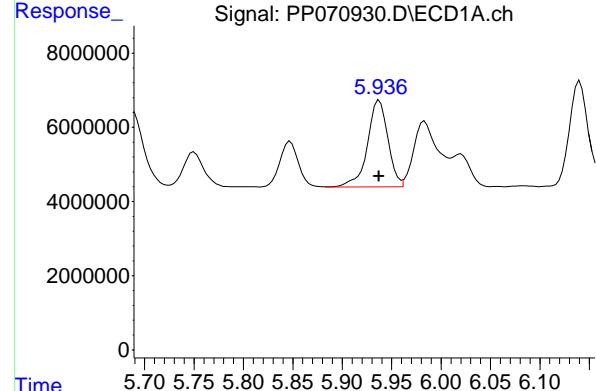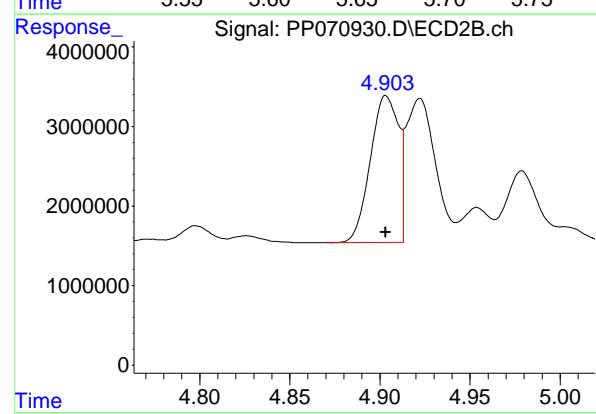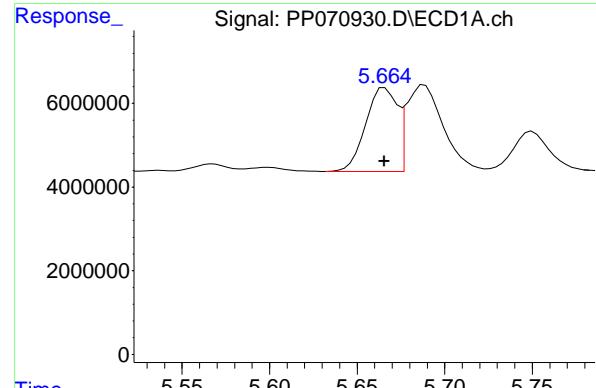

#21 AR-1248-1

R.T.: 5.666 min  
 Delta R.T.: 0.000 min  
 Response: 25034469 ECD\_P  
 Conc: 741.07 ng/ml ClientSampleId : AR1248ICC750

#21 AR-1248-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 20052758  
 Conc: 703.57 ng/ml

#22 AR-1248-2


R.T.: 5.938 min  
 Delta R.T.: 0.000 min  
 Response: 33734311  
 Conc: 730.30 ng/ml

#22 AR-1248-2

R.T.: 5.141 min  
 Delta R.T.: 0.000 min  
 Response: 26938678  
 Conc: 703.83 ng/ml


#23 AR-1248-3

R.T.: 6.140 min  
 Delta R.T.: 0.000 min  
 Response: 38083098 ECD\_P  
 Conc: 734.84 ng/ml ClientSampleId : AR1248ICC750

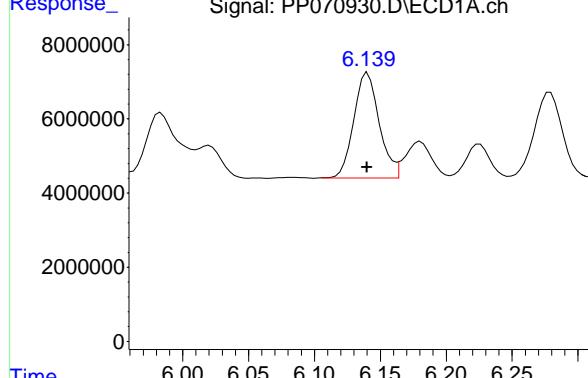


#23 AR-1248-3

R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 28275820  
 Conc: 707.53 ng/ml

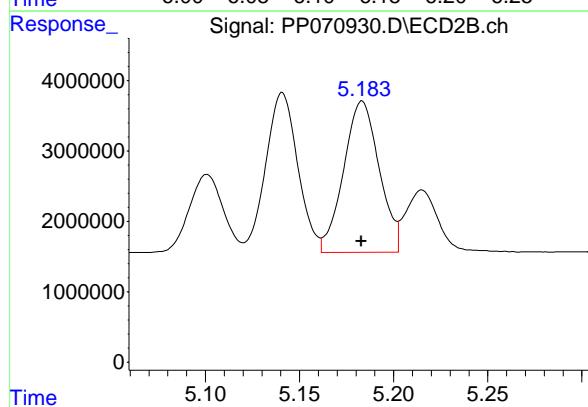


#24 AR-1248-4

R.T.: 6.539 min  
 Delta R.T.: 0.000 min  
 Response: 47603456  
 Conc: 710.08 ng/ml

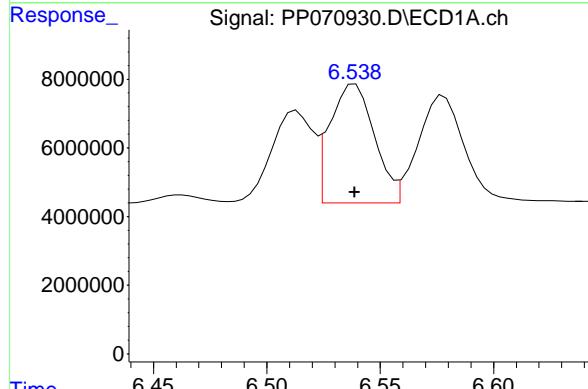


#24 AR-1248-4

R.T.: 5.356 min  
 Delta R.T.: 0.000 min  
 Response: 32558799  
 Conc: 690.07 ng/ml

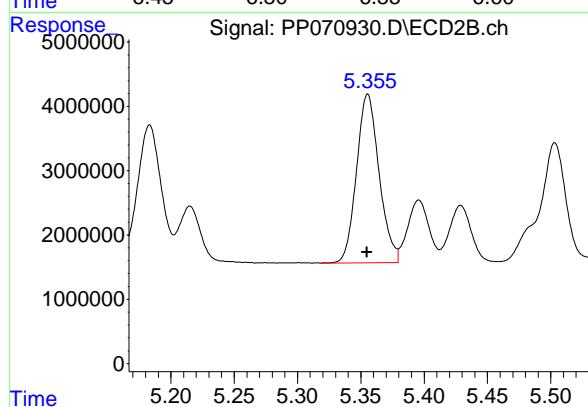


#25 AR-1248-5

R.T.: 6.578 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 45378306  
Conc: 705.88 ng/ml  
ClientSampleId: AR1248ICC750

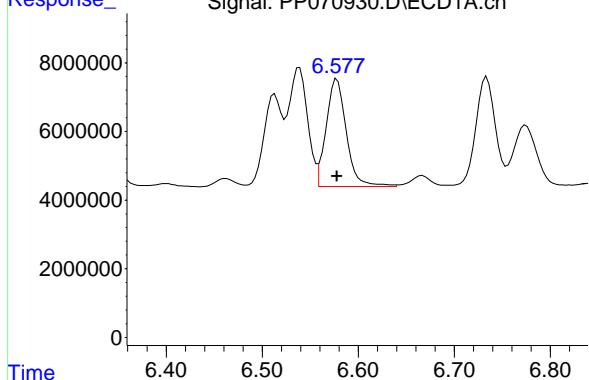

#25 AR-1248-5

R.T.: 5.749 min  
Delta R.T.: 0.000 min  
Response: 30836259  
Conc: 702.02 ng/ml

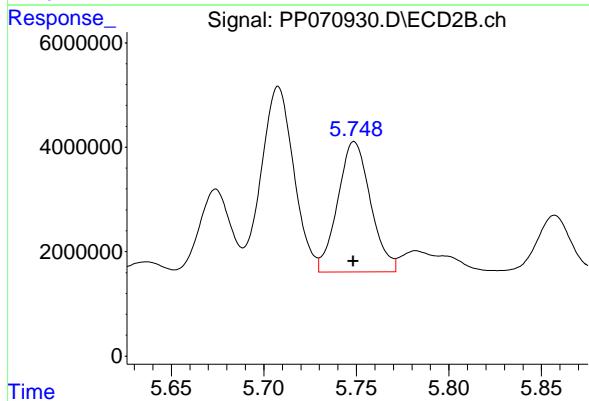

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070931.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:22  
 Operator : YP\AJ  
 Sample : AR1248ICC500  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 14:46:15 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 14:45:17 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.513	3.816	77451968	56907988	50.000	50.000
2) SA Decachlor...	10.226	8.859	60256834	41354865	50.000	50.000

Target Compounds

21) L5 AR-1248-1	5.665	4.903	16890769	14250625	500.000	500.000
22) L5 AR-1248-2	5.937	5.140	23096128	19137230	500.000	500.000
23) L5 AR-1248-3	6.140	5.183	25912526	19982060	500.000	500.000
24) L5 AR-1248-4	6.539	5.355	33519946	23590888	500.000	500.000
25) L5 AR-1248-5	6.578	5.748	32143070	21962659	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070931.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:22  
 Operator : YP\AJ  
 Sample : AR1248ICC500  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 14:46:15 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 14:45:17 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

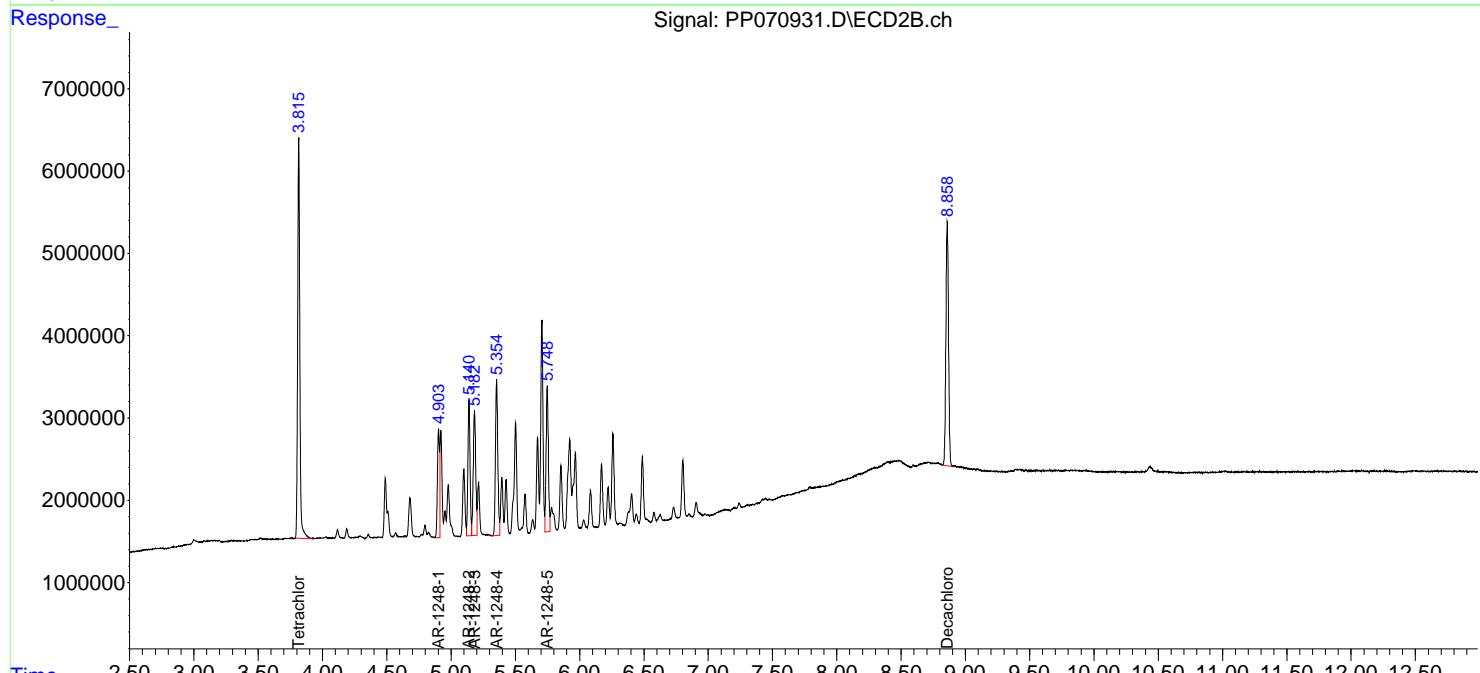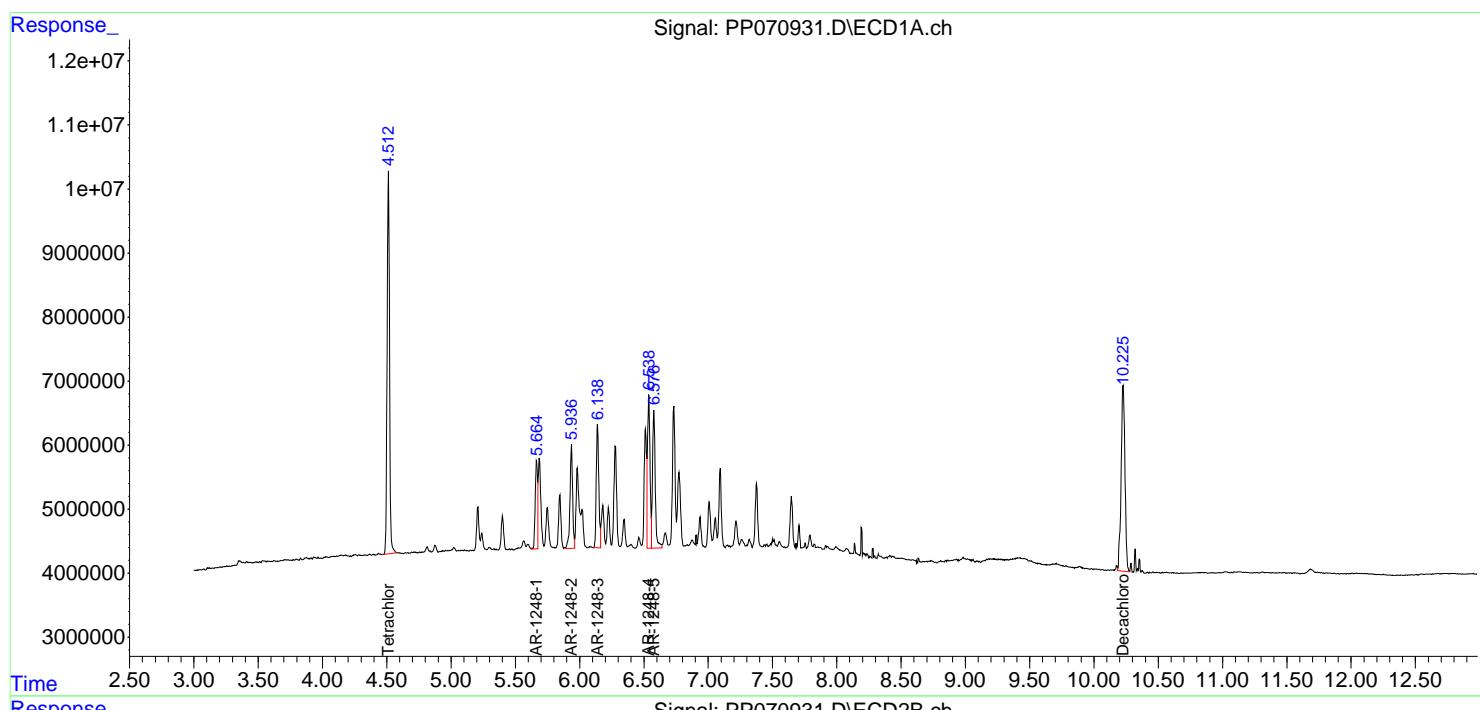

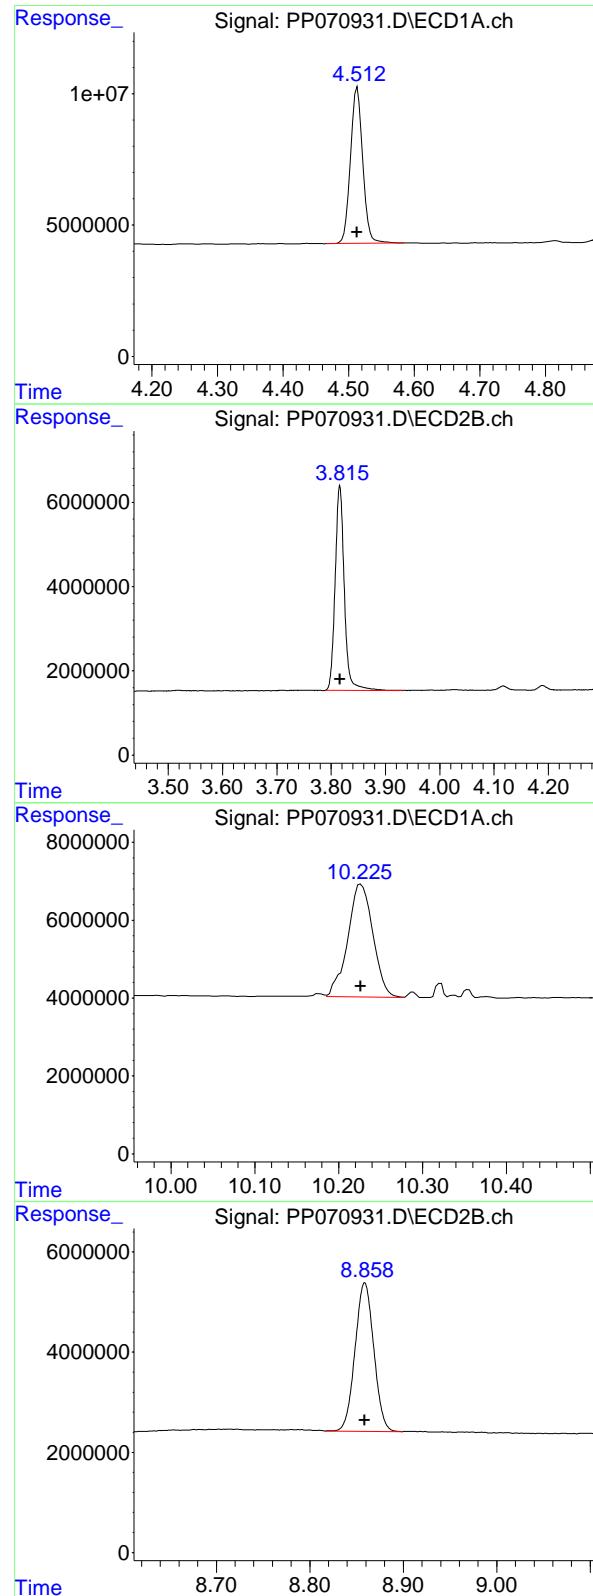

## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
 Delta R.T.: 0.000 min  
 Response: 77451968 ECD\_P  
 Conc: 50.00 ng/ml ClientSampleId : AR1248ICC500

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 56907988  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.226 min  
 Delta R.T.: 0.000 min  
 Response: 60256834  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 41354865  
 Conc: 50.00 ng/ml

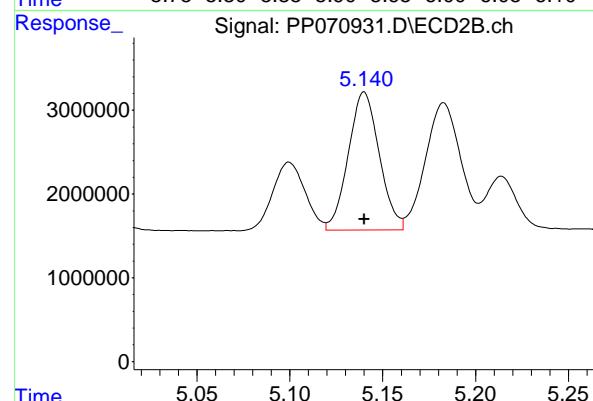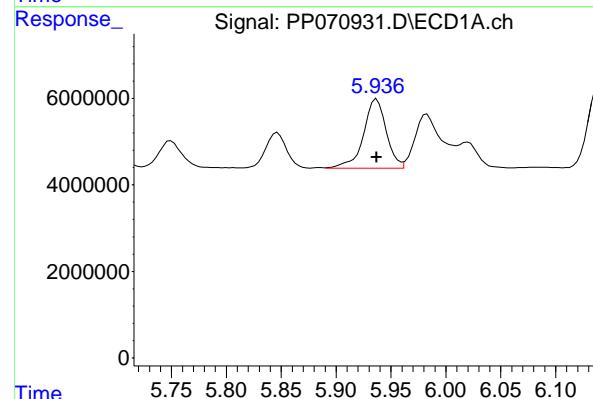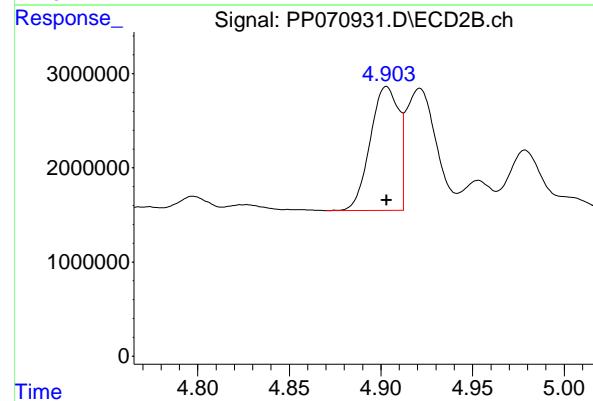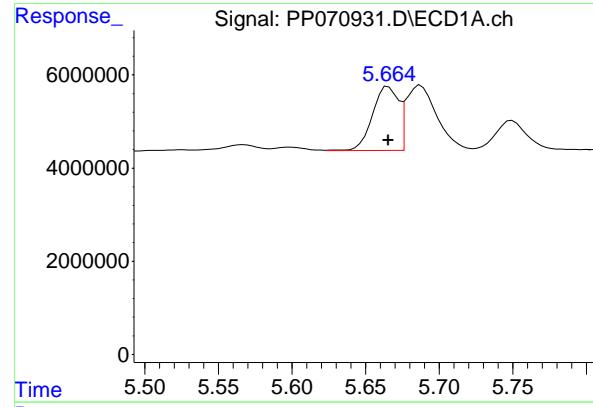

#21 AR-1248-1

R.T.: 5.665 min  
 Delta R.T.: 0.000 min  
 Response: 16890769  
 Conc: 500.00 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** AR1248ICC500

#21 AR-1248-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 14250625  
 Conc: 500.00 ng/ml

#22 AR-1248-2


R.T.: 5.937 min  
 Delta R.T.: 0.000 min  
 Response: 23096128  
 Conc: 500.00 ng/ml

#22 AR-1248-2

R.T.: 5.140 min  
 Delta R.T.: 0.000 min  
 Response: 19137230  
 Conc: 500.00 ng/ml


#23 AR-1248-3

R.T.: 6.140 min  
 Delta R.T.: 0.000 min  
 Response: 25912526  
 Conc: 500.00 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** AR1248ICC500

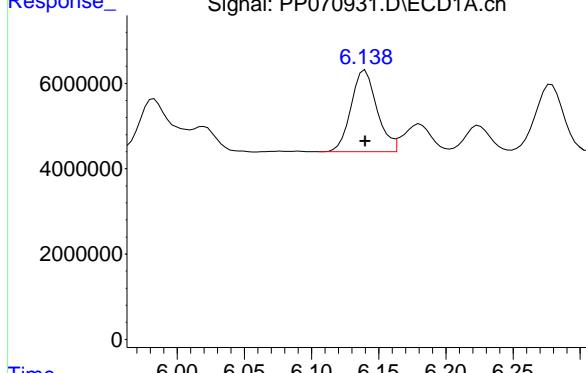


#23 AR-1248-3

R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 19982060  
 Conc: 500.00 ng/ml

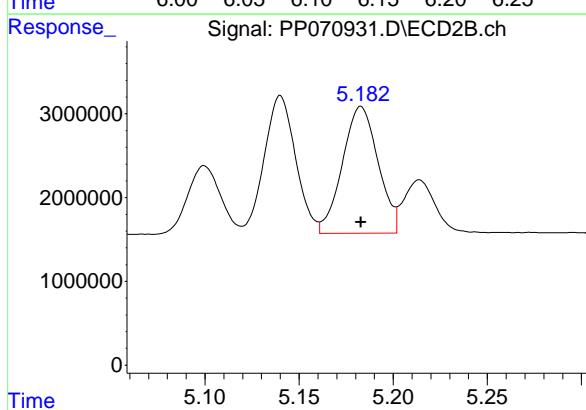


#24 AR-1248-4

R.T.: 6.539 min  
 Delta R.T.: 0.000 min  
 Response: 33519946  
 Conc: 500.00 ng/ml

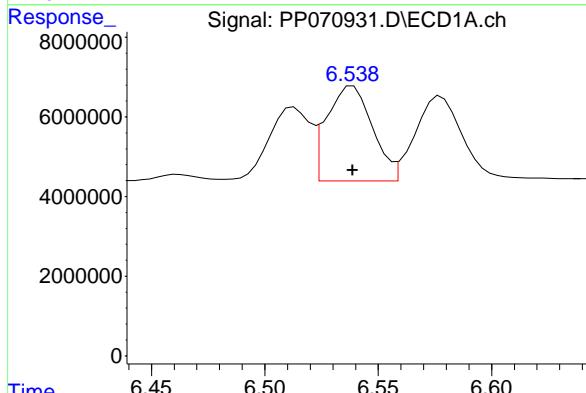


#24 AR-1248-4

R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 23590888  
 Conc: 500.00 ng/ml

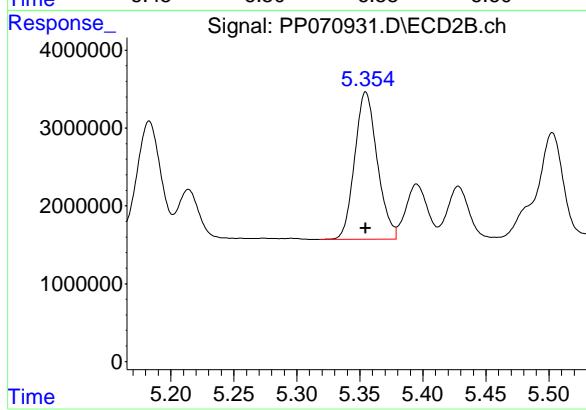


#25 AR-1248-5

R.T.: 6.578 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 32143070  
Conc: 500.00 ng/ml  
ClientSampleId: AR1248ICC500

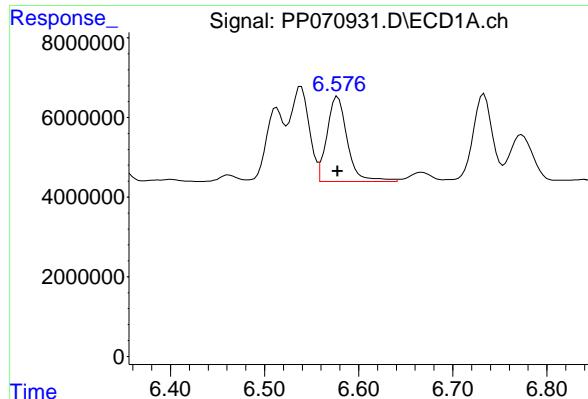

#25 AR-1248-5

R.T.: 5.748 min  
Delta R.T.: 0.000 min  
Response: 21962659  
Conc: 500.00 ng/ml

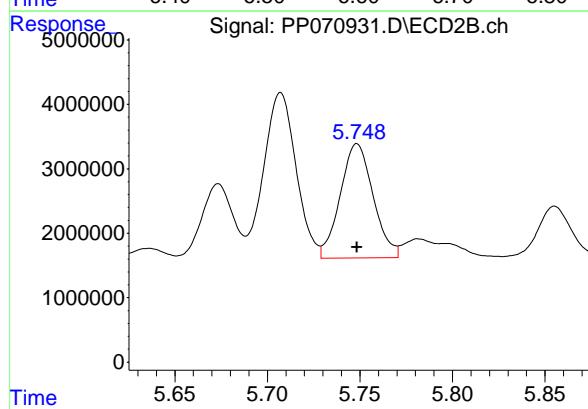

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070932.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:38  
 Operator : YP\AJ  
 Sample : AR1248ICC250  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 15:07:19 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 15:04:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.517	3.817	38987130	27101787	25.676	25.783
2) SA Decachlor...	10.232	8.860	29177292	20157827	25.732	25.064

Target Compounds

21) L5 AR-1248-1	5.672	4.904	11497190	7301885	350.874	278.926
22) L5 AR-1248-2	5.941	5.141	11780544	9675655	264.590	275.754
23) L5 AR-1248-3	6.144	5.184	12674295	10119428	252.379	275.339
24) L5 AR-1248-4	6.543	5.356	18357259	12061061	289.258	281.127
25) L5 AR-1248-5	6.582	5.750	17129846	11658567	283.226	286.518



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070932.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:38  
 Operator : YP\AJ  
 Sample : AR1248ICC250  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 15:07:19 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 15:04:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

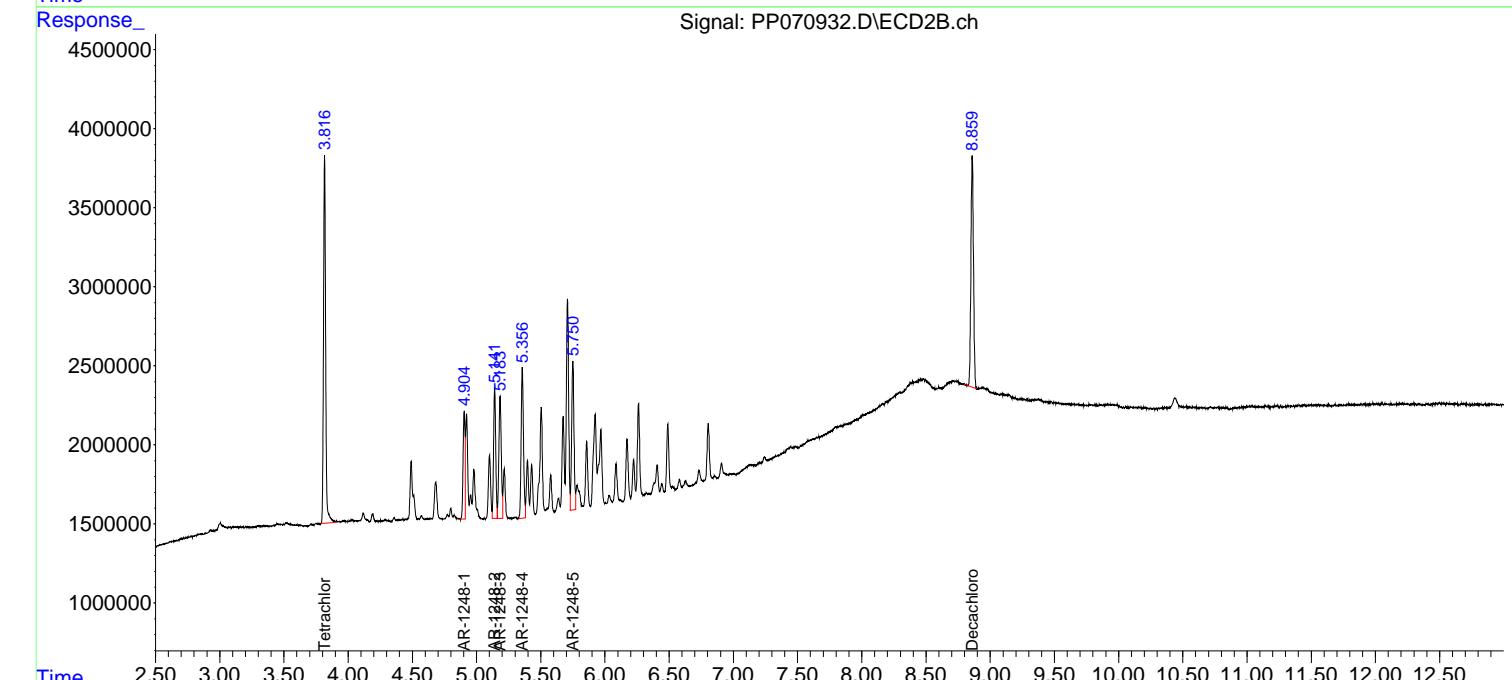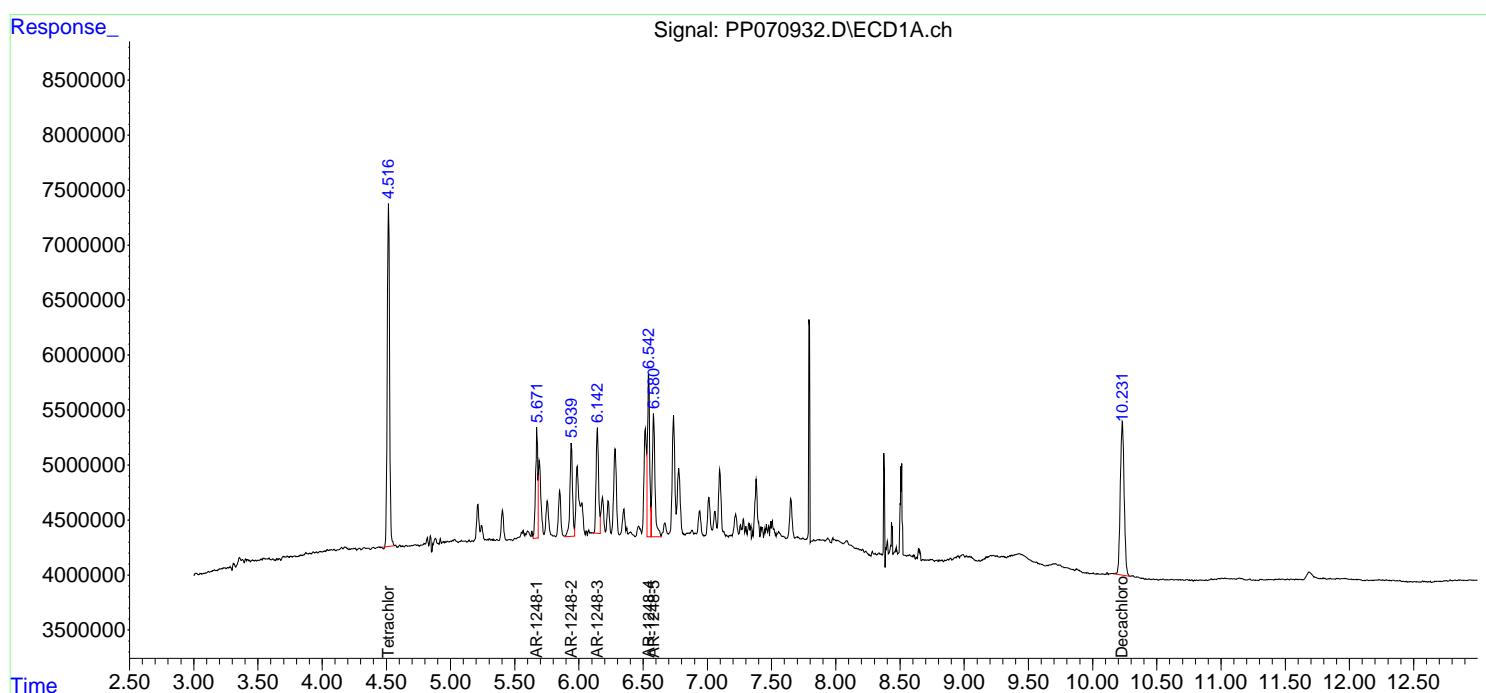

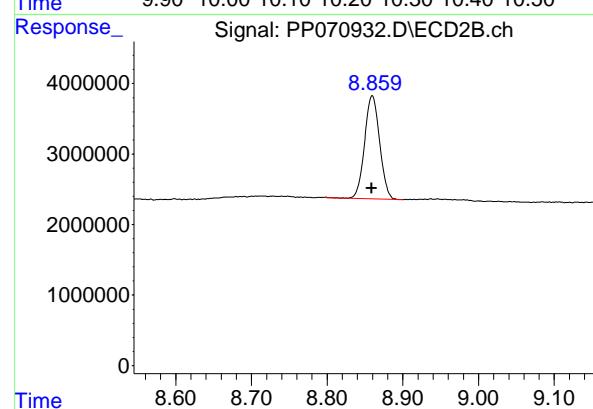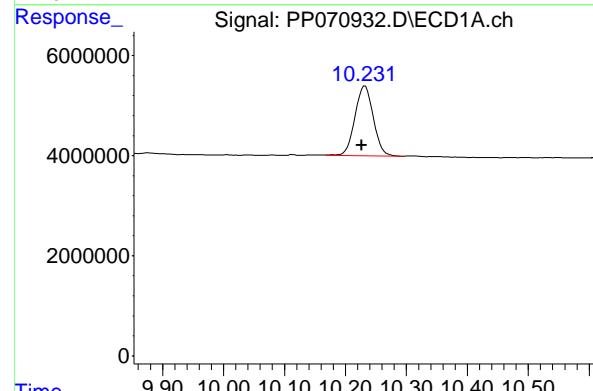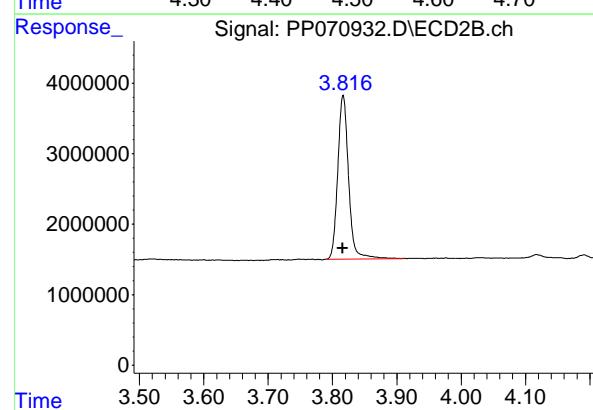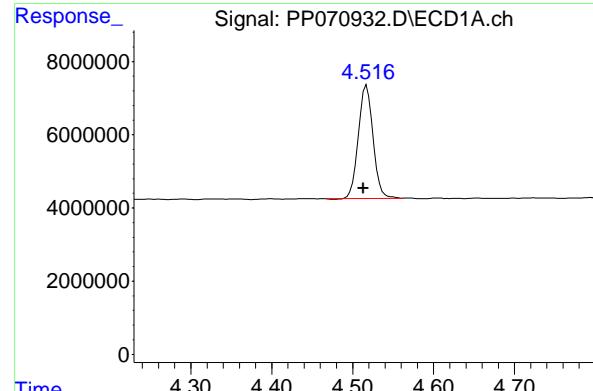

## #1 Tetrachloro-m-xylene

R.T.: 4.517 min  
 Delta R.T.: 0.004 min  
 Response: 38987130 ECD\_P  
 Conc: 25.68 ng/ml ClientSampleId : AR1248ICC250

## #1 Tetrachloro-m-xylene


R.T.: 3.817 min  
 Delta R.T.: 0.000 min  
 Response: 27101787  
 Conc: 25.78 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.232 min  
 Delta R.T.: 0.006 min  
 Response: 29177292  
 Conc: 25.73 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.860 min  
 Delta R.T.: 0.000 min  
 Response: 20157827  
 Conc: 25.06 ng/ml

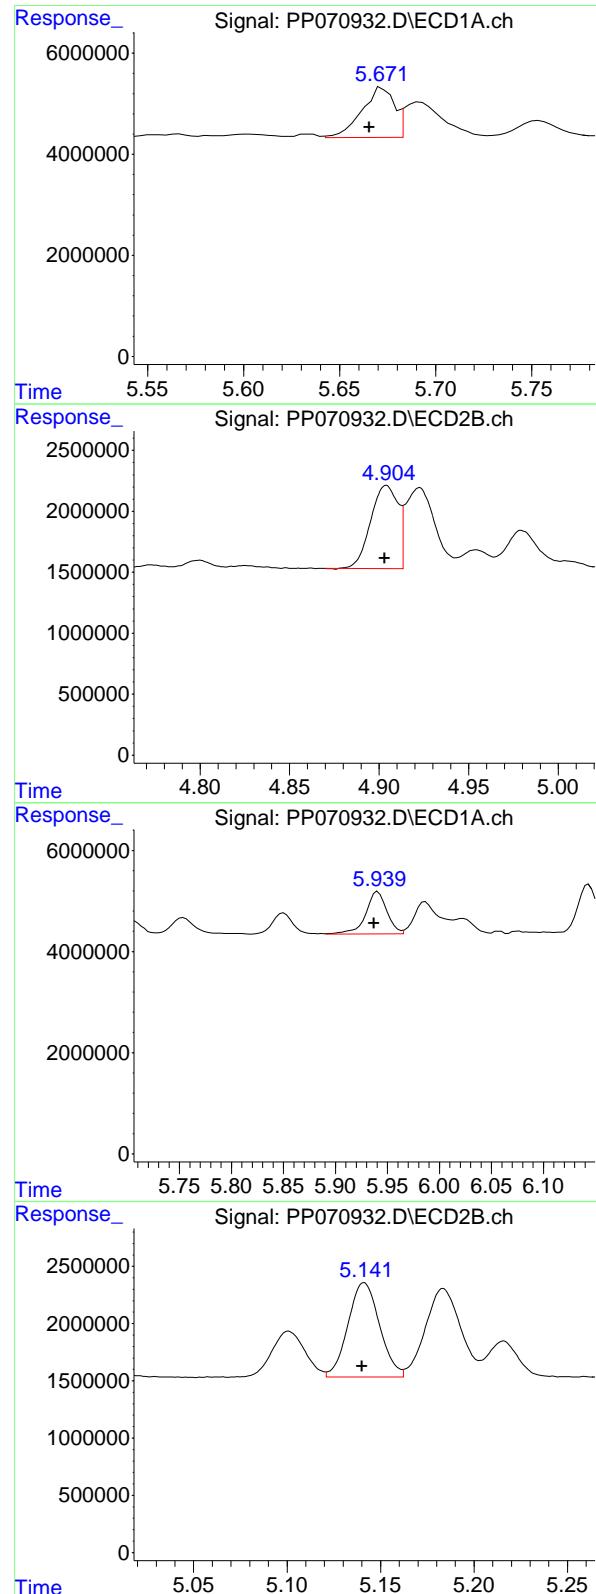

#21 AR-1248-1

R.T.: 5.672 min  
 Delta R.T.: 0.007 min  
 Response: 11497190 ECD\_P  
 Conc: 350.87 ng/ml ClientSampleId : AR1248ICC250

#21 AR-1248-1





R.T.: 4.904 min  
 Delta R.T.: 0.000 min  
 Response: 7301885  
 Conc: 278.93 ng/ml

#22 AR-1248-2

R.T.: 5.941 min  
 Delta R.T.: 0.004 min  
 Response: 11780544  
 Conc: 264.59 ng/ml

#22 AR-1248-2

R.T.: 5.141 min  
 Delta R.T.: 0.001 min  
 Response: 9675655  
 Conc: 275.75 ng/ml

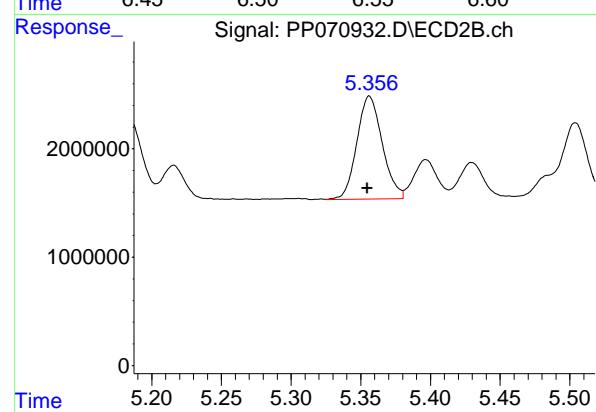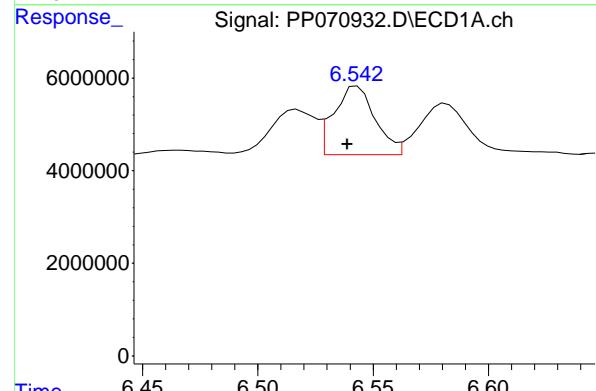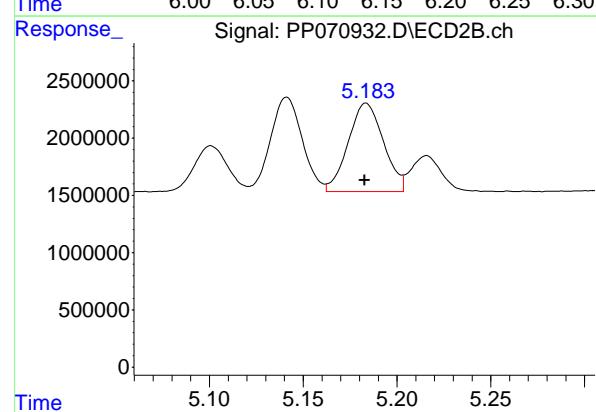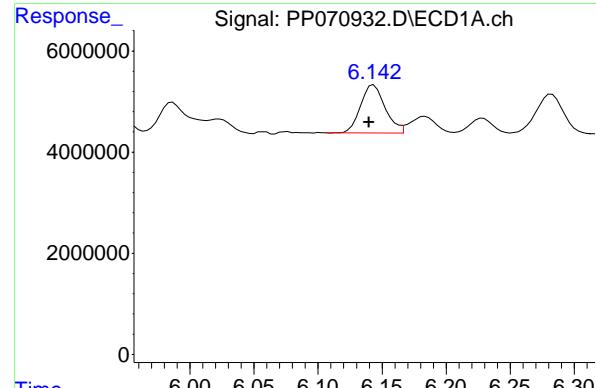

#23 AR-1248-3

R.T.: 6.144 min  
 Delta R.T.: 0.004 min  
 Response: 12674295 ECD\_P  
 Conc: 252.38 ng/ml ClientSampleId : AR1248ICC250

#23 AR-1248-3

R.T.: 5.184 min  
 Delta R.T.: 0.000 min  
 Response: 10119428  
 Conc: 275.34 ng/ml

#24 AR-1248-4



R.T.: 6.543 min  
 Delta R.T.: 0.004 min  
 Response: 18357259  
 Conc: 289.26 ng/ml

#24 AR-1248-4

R.T.: 5.356 min  
 Delta R.T.: 0.002 min  
 Response: 12061061  
 Conc: 281.13 ng/ml

#25 AR-1248-5

R.T.: 6.582 min  
Delta R.T.: 0.004 min  
Instrument: ECD\_P  
Response: 17129846  
Conc: 283.23 ng/ml  
ClientSampleId: AR1248ICC250

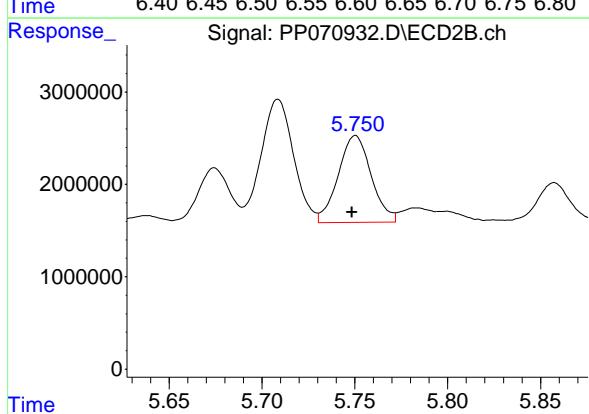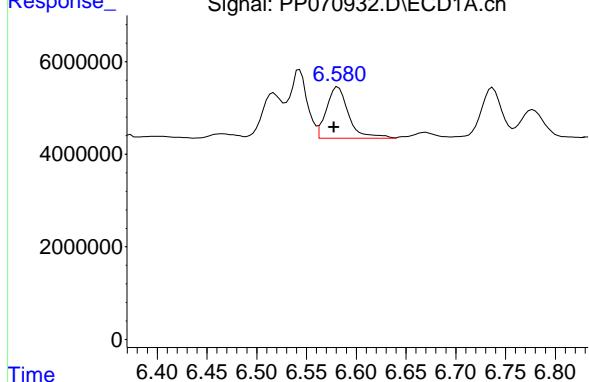

#25 AR-1248-5

R.T.: 5.750 min  
Delta R.T.: 0.002 min  
Response: 11658567  
Conc: 286.52 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070933.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:55  
 Operator : YP\AJ  
 Sample : AR1248ICC050  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC050**

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 15:16:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 15:04:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	4.513	3.815	7324663	5848649	4.791	5.521
2) SA Decachlor...	10.227	8.859	5549589	3661642	4.859	4.550

**Target Compounds**

21) L5 AR-1248-1	5.665	4.902	1857345	1382826	51.489	51.338
22) L5 AR-1248-2	5.935	5.140	2199982	1982278	48.701m	55.076
23) L5 AR-1248-3	6.137	5.182	2591630	2128069	51.484m	56.472
24) L5 AR-1248-4	6.536	5.354	2845967	2437650	43.150m	55.103 #
25) L5 AR-1248-5	6.576	5.748	2713422	2234402	43.421m	52.978

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070933.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:55  
 Operator : YP\AJ  
 Sample : AR1248ICC050  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 15:16:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 15:04:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_P  
**ClientSampleId :**  
 AR1248ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

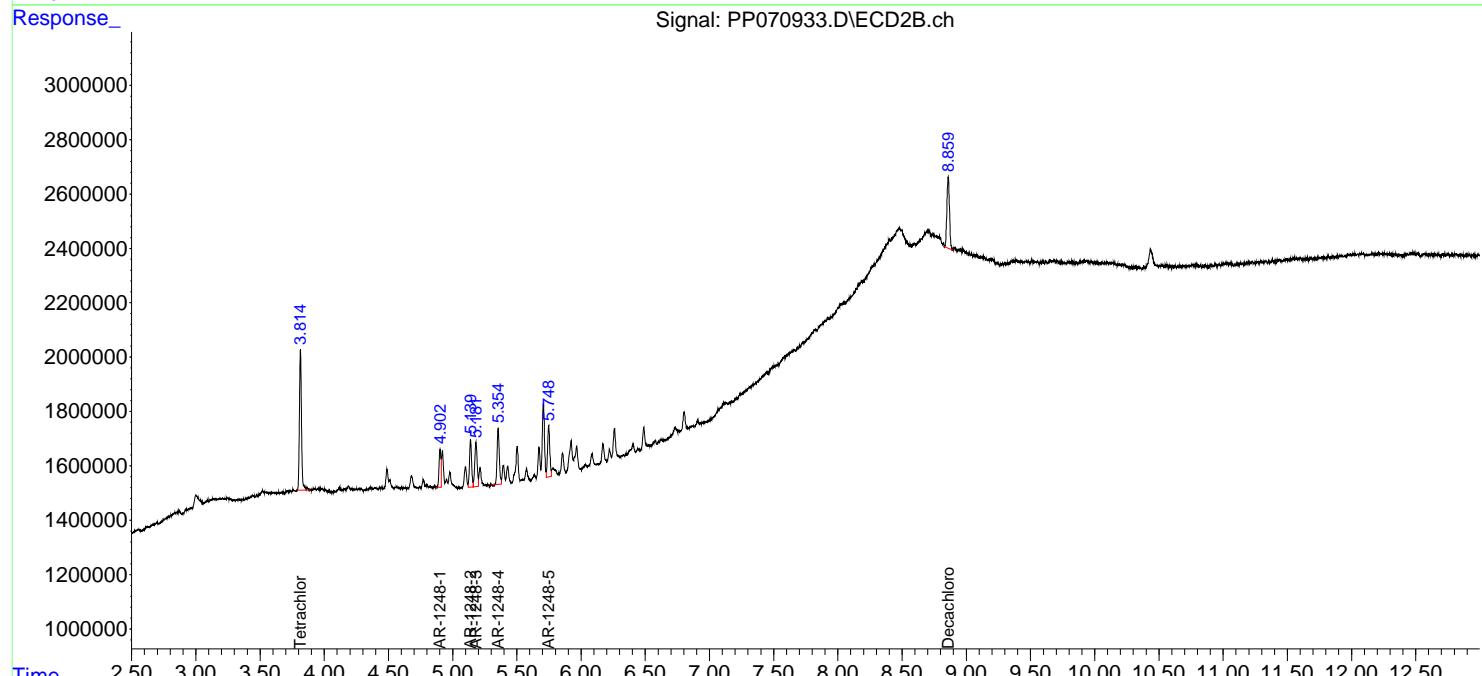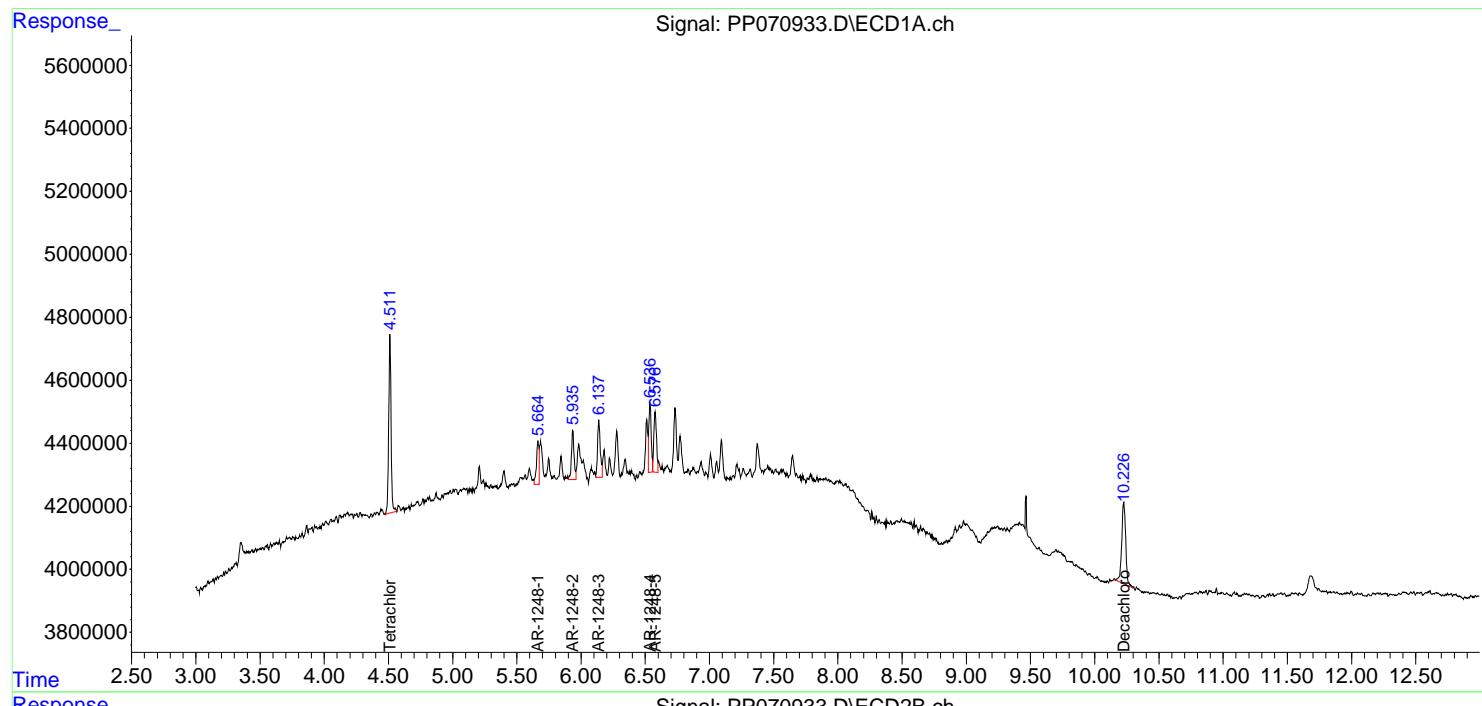

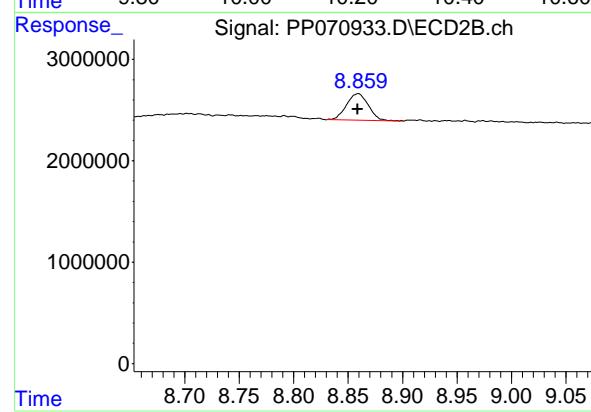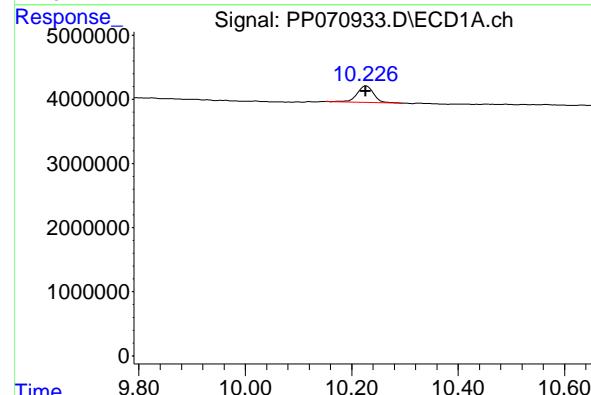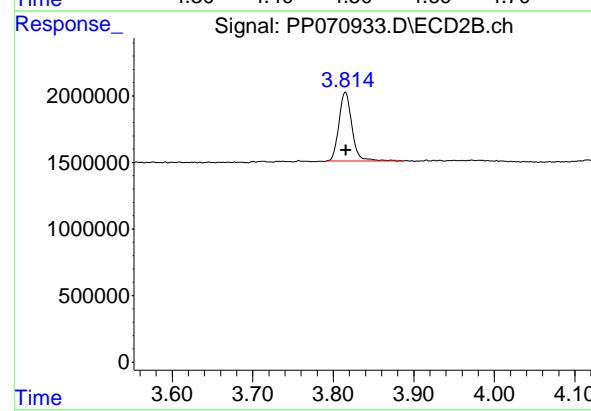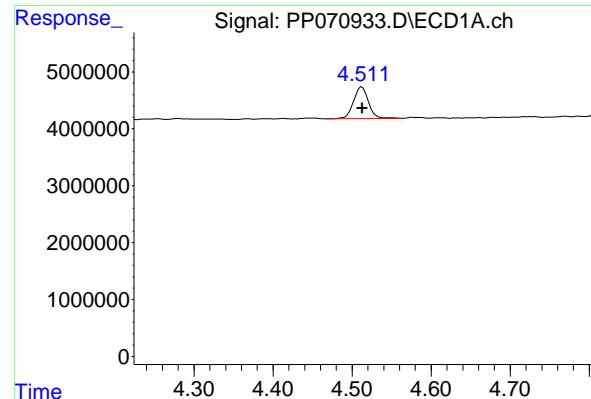

## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
 Delta R.T.: 0.000 min  
 Response: 7324663 ECD\_P  
 Conc: 4.79 ng/ml ClientSampleId : AR1248ICC050

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene


R.T.: 3.815 min  
 Delta R.T.: 0.000 min  
 Response: 5848649  
 Conc: 5.52 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.227 min  
 Delta R.T.: 0.000 min  
 Response: 5549589  
 Conc: 4.86 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 3661642  
 Conc: 4.55 ng/ml

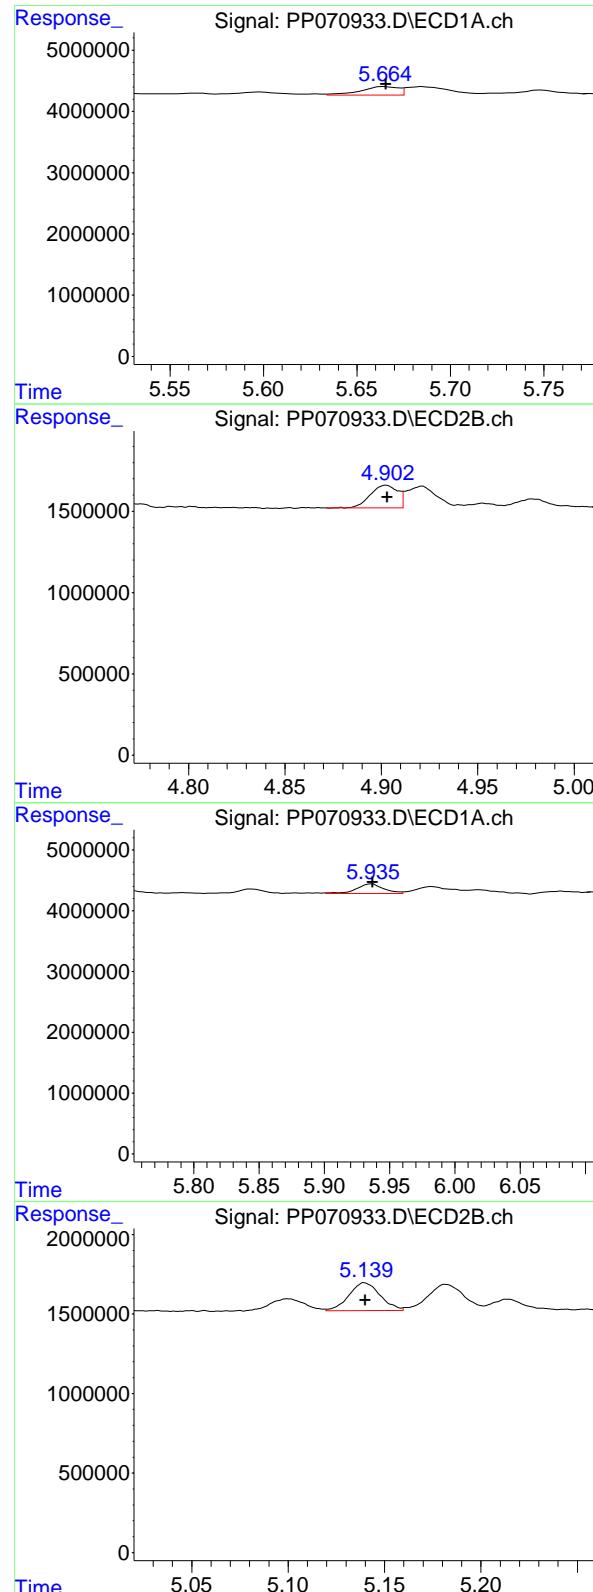

#21 AR-1248-1

R.T.: 5.665 min  
 Delta R.T.: 0.000 min  
 Response: 1857345  
 Conc: 51.49 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1248ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#21 AR-1248-1


R.T.: 4.902 min  
 Delta R.T.: 0.000 min  
 Response: 1382826  
 Conc: 51.34 ng/ml

#22 AR-1248-2

R.T.: 5.935 min  
 Delta R.T.: -0.002 min  
 Response: 2199982  
 Conc: 48.70 ng/ml

#22 AR-1248-2

R.T.: 5.140 min  
 Delta R.T.: 0.000 min  
 Response: 1982278  
 Conc: 55.08 ng/ml

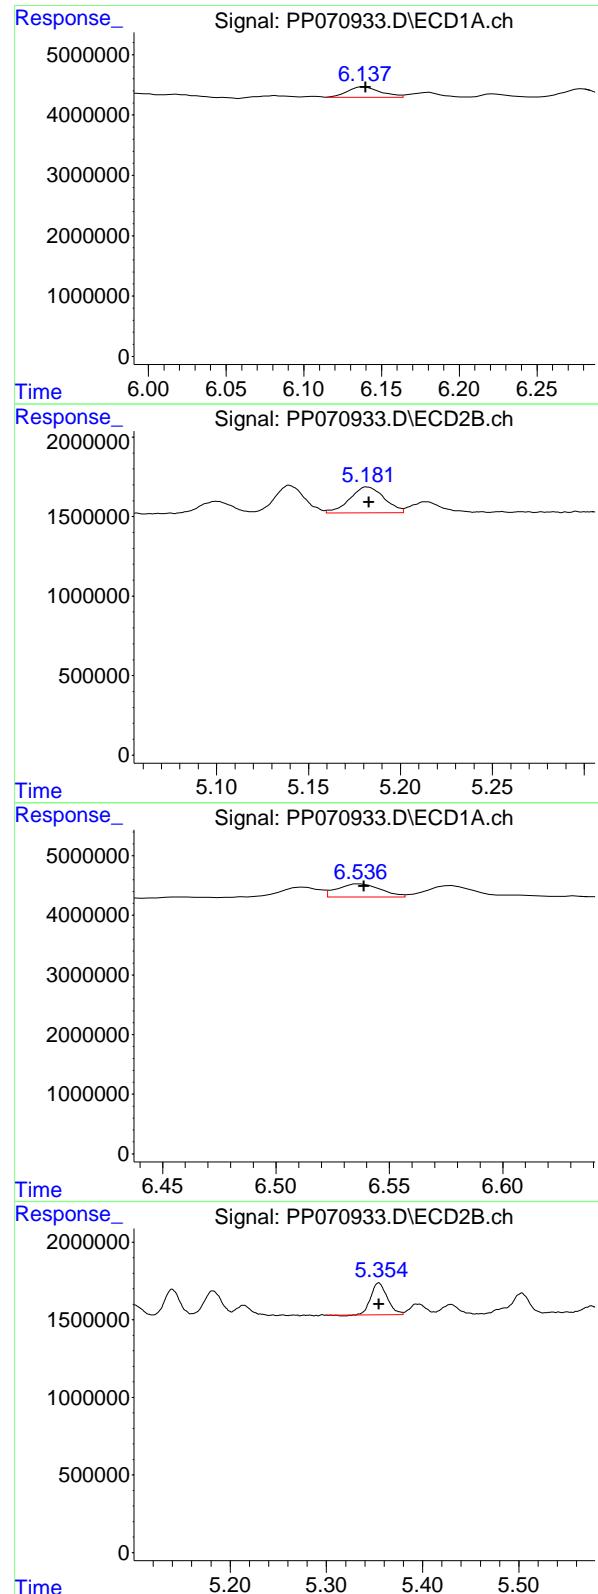

#23 AR-1248-3

R.T.: 6.137 min  
 Delta R.T.: -0.002 min  
 Response: 2591630 ECD\_P  
 Conc: 51.48 ng/ml ClientSampleId : AR1248ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#23 AR-1248-3

R.T.: 5.182 min  
 Delta R.T.: 0.000 min  
 Response: 2128069  
 Conc: 56.47 ng/ml

#24 AR-1248-4

R.T.: 6.536 min  
 Delta R.T.: -0.003 min  
 Response: 2845967  
 Conc: 43.15 ng/ml

#24 AR-1248-4

R.T.: 5.354 min  
 Delta R.T.: 0.000 min  
 Response: 2437650  
 Conc: 55.10 ng/ml

#25 AR-1248-5


R.T.: 6.576 min  
 Delta R.T.: -0.001 min  
 Response: 2713422 ECD\_P  
 Conc: 43.42 ng/ml ClientSampleId :  
 AR1248ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#25 AR-1248-5

R.T.: 5.748 min  
 Delta R.T.: 0.000 min  
 Response: 2234402  
 Conc: 52.98 ng/ml

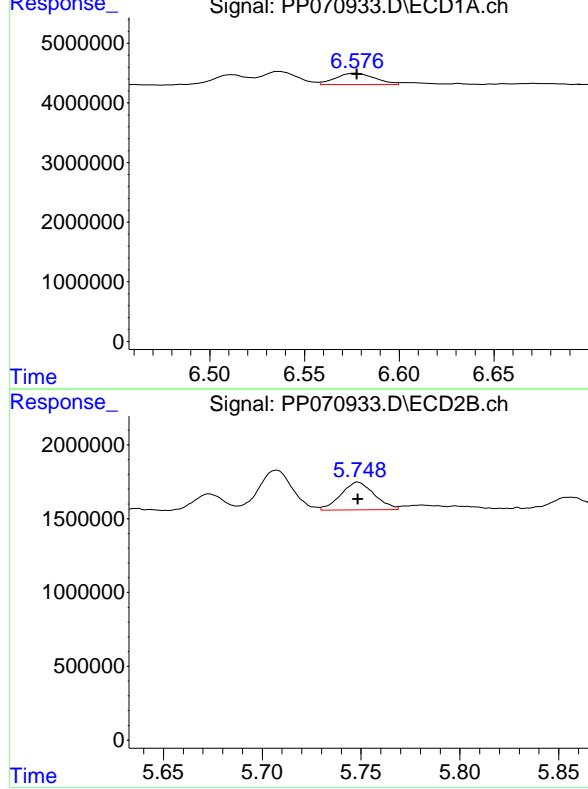

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070934.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:11  
 Operator : YP\AJ  
 Sample : AR1254ICC1000  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
AR1254ICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.514	3.816	150.1E6	104.3E6	95.275	94.048
2) SA Decachloro...	10.231	8.860	109.5E6	78348381	93.754	86.018

**Target Compounds**

26) L6 AR-1254-1	6.516	5.709	60157506	58928147	918.830	891.736
27) L6 AR-1254-2	6.732	5.857	92838442	50145967	911.948	882.952
28) L6 AR-1254-3	7.095	6.261	92334650	77448562	928.765	882.456
29) L6 AR-1254-4	7.379	6.490	84238161	49998215	970.458	893.353
30) L6 AR-1254-5	7.792	6.908	74433164	65979008	920.580m	918.596

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070934.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:11  
 Operator : YP\AJ  
 Sample : AR1254ICC1000  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1



Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1254ICC1000





**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

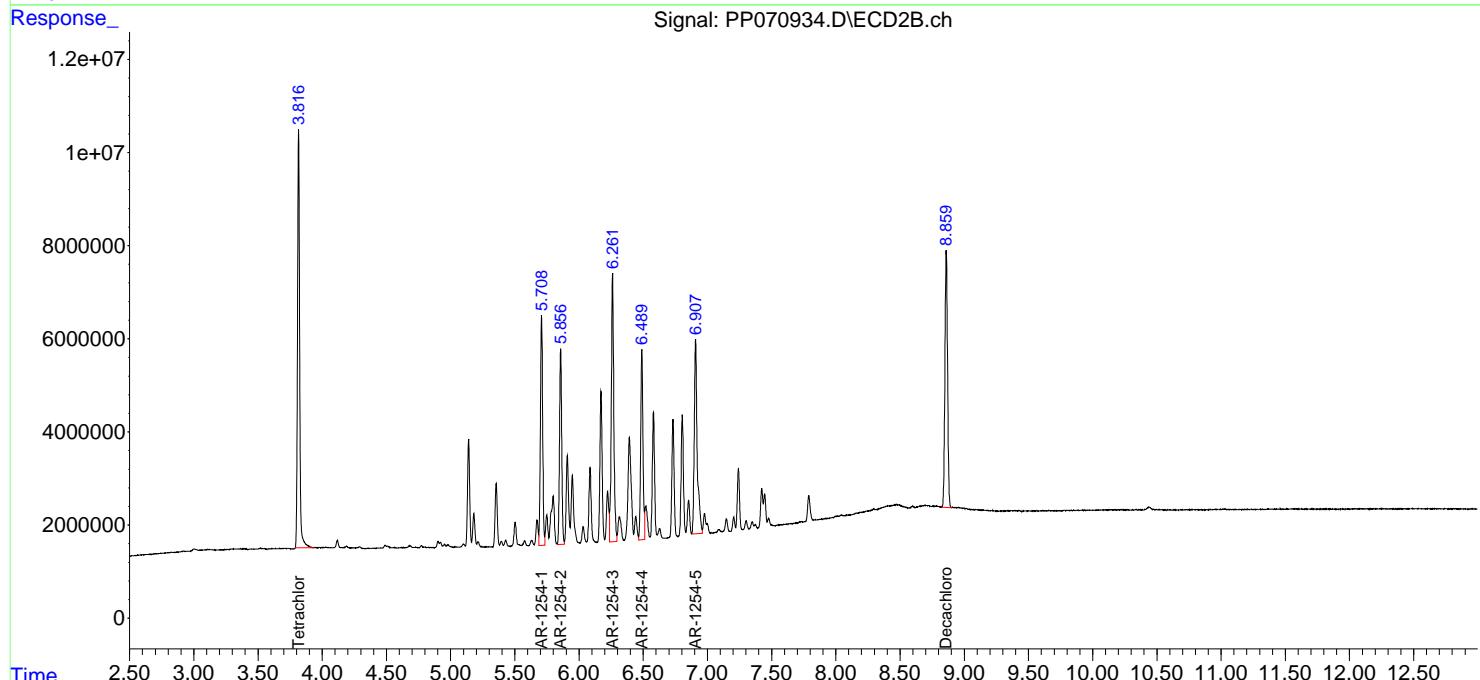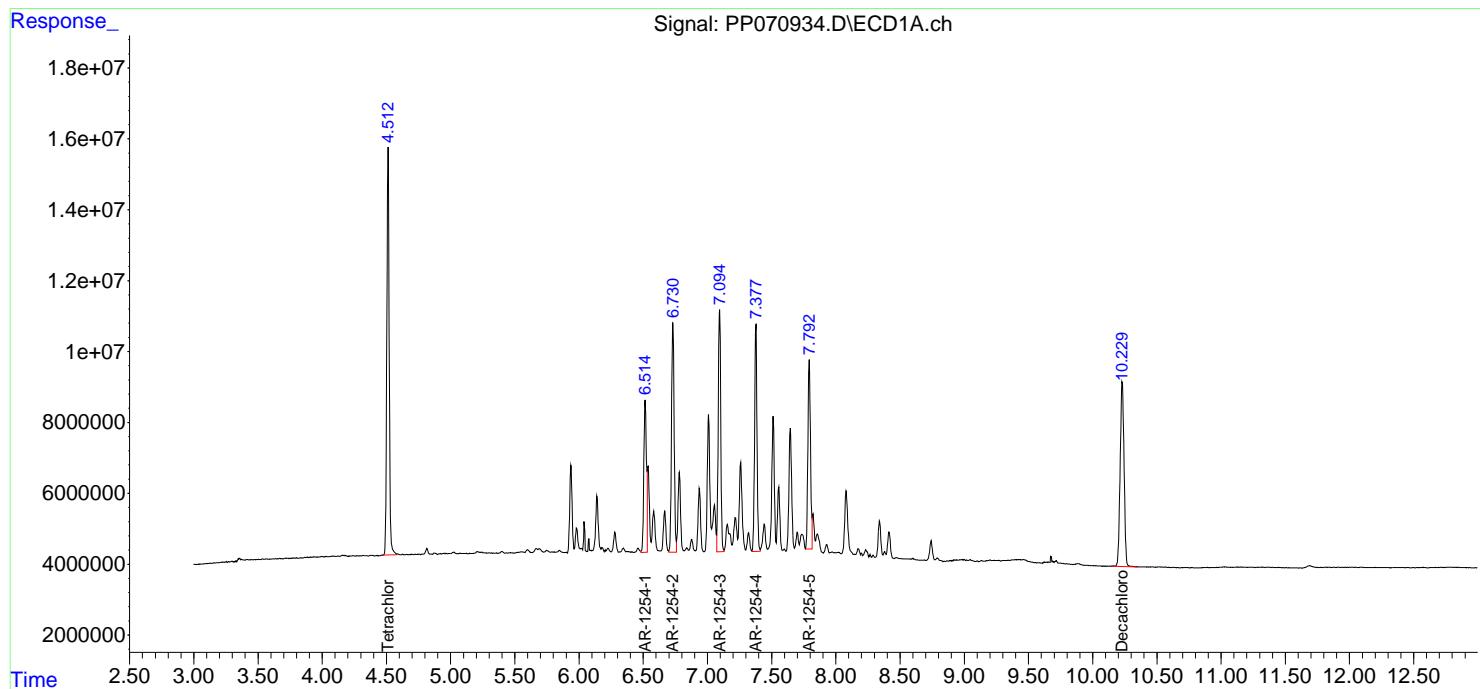

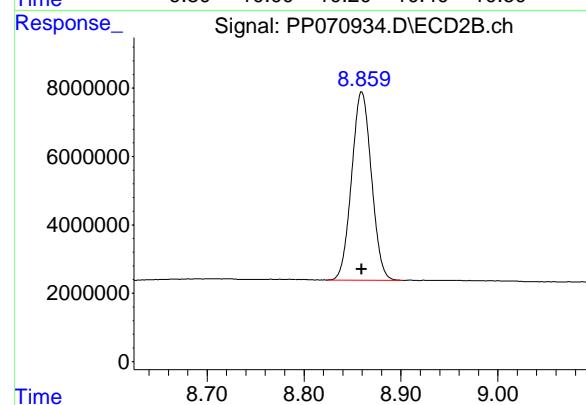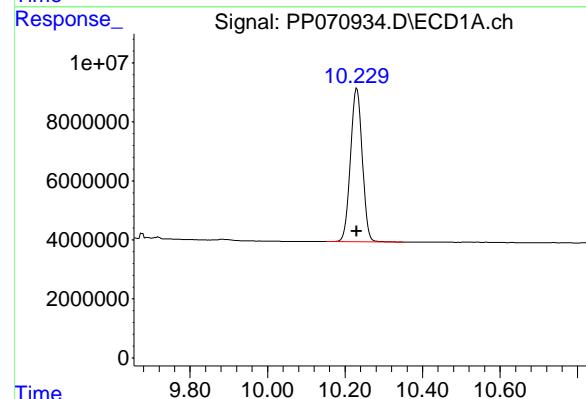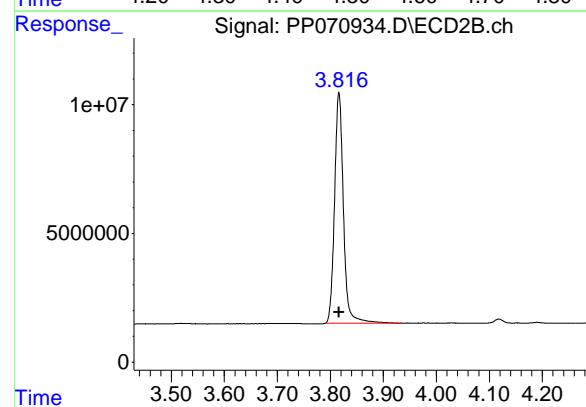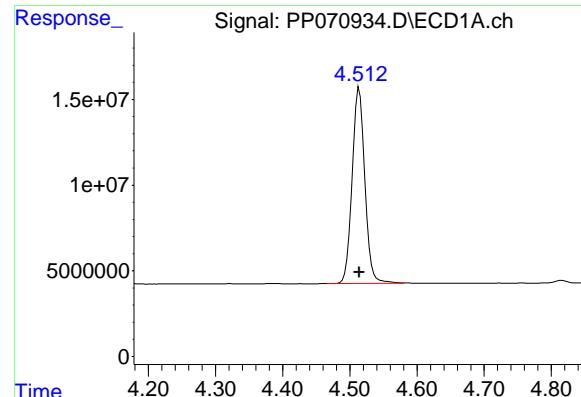

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 150128836  
Conc: 95.27 ng/ml ClientSampleId : AR1254ICC1000

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 104259560  
Conc: 94.05 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.231 min  
Delta R.T.: 0.001 min  
Response: 109543241  
Conc: 93.75 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.860 min  
Delta R.T.: 0.000 min  
Response: 78348381  
Conc: 86.02 ng/ml

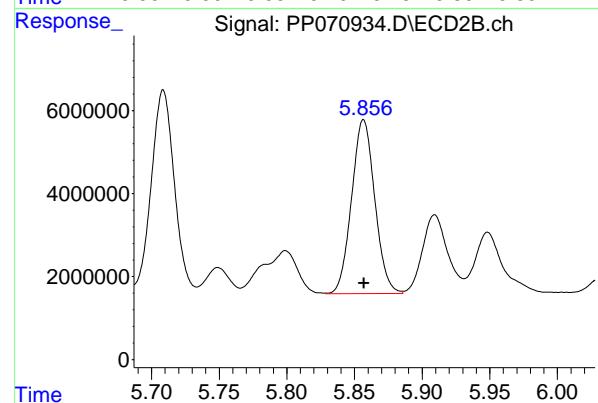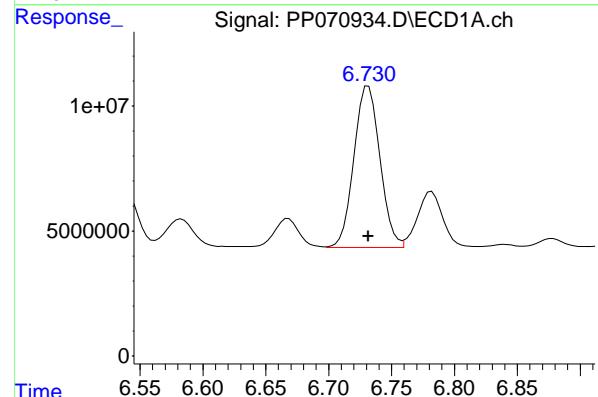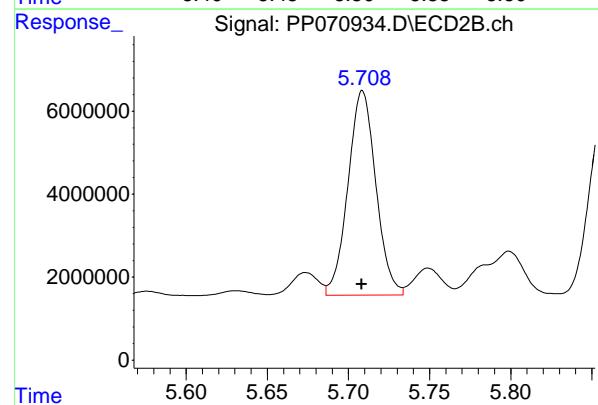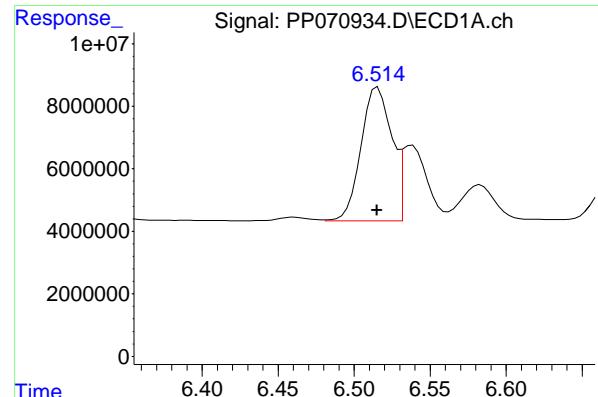

#26 AR-1254-1

R.T.: 6.516 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 60157506  
Conc: 918.83 ng/ml ClientSampleId : AR1254ICC1000

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

#26 AR-1254-1

R.T.: 5.709 min  
Delta R.T.: 0.000 min  
Response: 58928147  
Conc: 891.74 ng/ml

#27 AR-1254-2

R.T.: 6.732 min  
Delta R.T.: 0.000 min  
Response: 92838442  
Conc: 911.95 ng/ml

#27 AR-1254-2

R.T.: 5.857 min  
Delta R.T.: 0.000 min  
Response: 50145967  
Conc: 882.95 ng/ml

#28 AR-1254-3

R.T.: 7.095 min  
 Delta R.T.: 0.000 min  
 Response: 92334650 ECD\_P  
 Conc: 928.77 ng/ml ClientSampleId : AR1254ICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#28 AR-1254-3





R.T.: 6.261 min  
 Delta R.T.: 0.001 min  
 Response: 77448562  
 Conc: 882.46 ng/ml

#29 AR-1254-4

R.T.: 7.379 min  
 Delta R.T.: 0.002 min  
 Response: 84238161  
 Conc: 970.46 ng/ml

#29 AR-1254-4

R.T.: 6.490 min  
 Delta R.T.: 0.000 min  
 Response: 49998215  
 Conc: 893.35 ng/ml

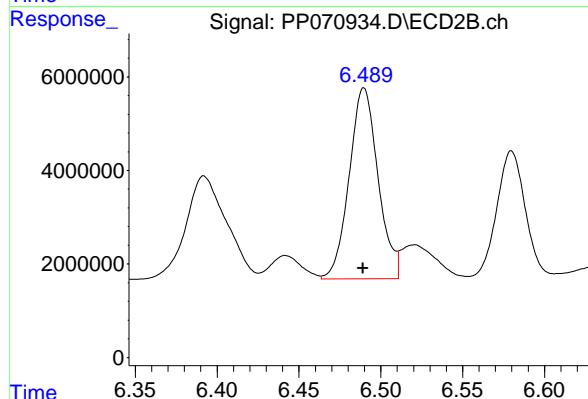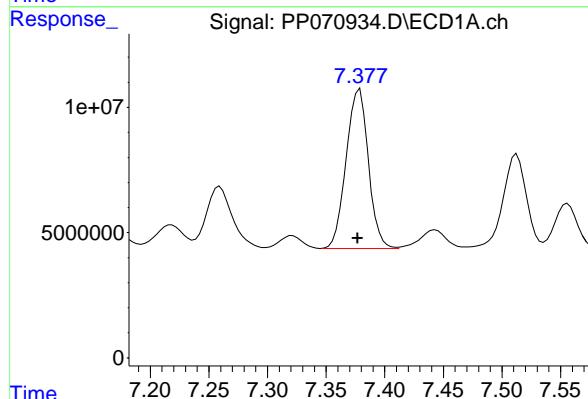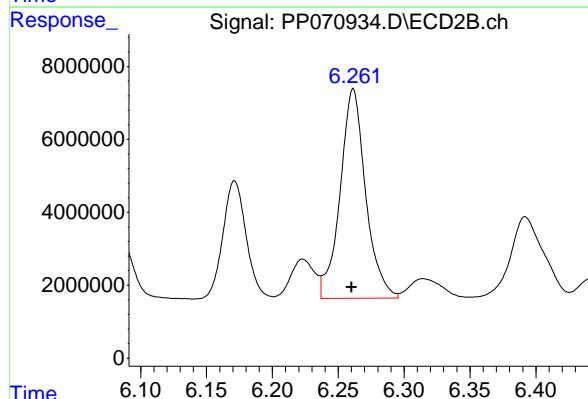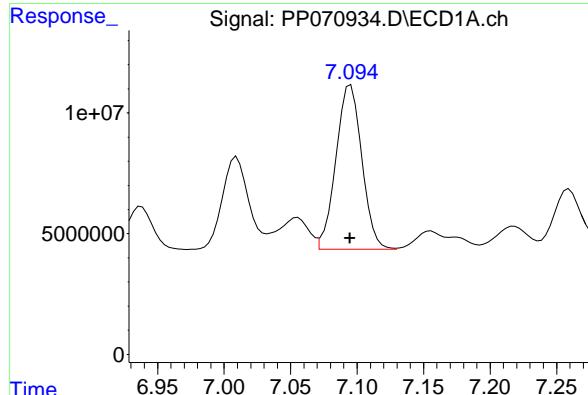

#30 AR-1254-5


R.T.: 7.792 min  
 Delta R.T.: 0.000 min  
 Response: 74433164 ECD\_P  
 Conc: 920.58 ng/ml ClientSampleId :  
 AR1254ICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#30 AR-1254-5

R.T.: 6.908 min  
 Delta R.T.: 0.000 min  
 Response: 65979008  
 Conc: 918.60 ng/ml

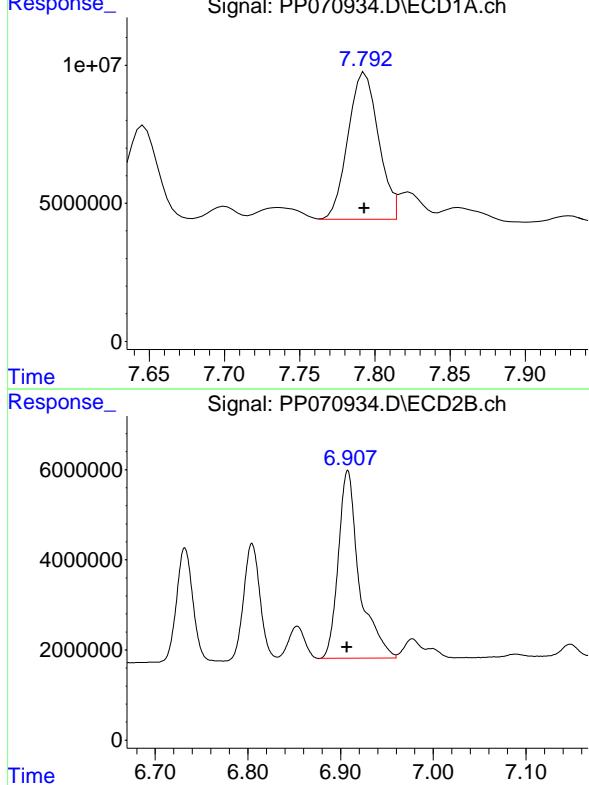

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070935.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:27  
 Operator : YP\AJ  
 Sample : AR1254ICC750  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC750**

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.514	3.816	116.3E6	81865229	73.835	73.847
2) SA Decachloro...	10.228	8.859	85851924	59713645	73.477	65.559

**Target Compounds**

26) L6 AR-1254-1	6.515	5.708	47300573	46349687	722.456	701.391
27) L6 AR-1254-2	6.731	5.856	72785411	40339655	714.968	710.286
28) L6 AR-1254-3	7.094	6.260	73541603	62731680	739.732	714.771
29) L6 AR-1254-4	7.377	6.490	65835410	40961211	758.451	731.883
30) L6 AR-1254-5	7.792	6.907	59278726	53519032	733.152m	745.122

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070935.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:27  
 Operator : YP\AJ  
 Sample : AR1254ICC750  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1



Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1254ICC750





**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

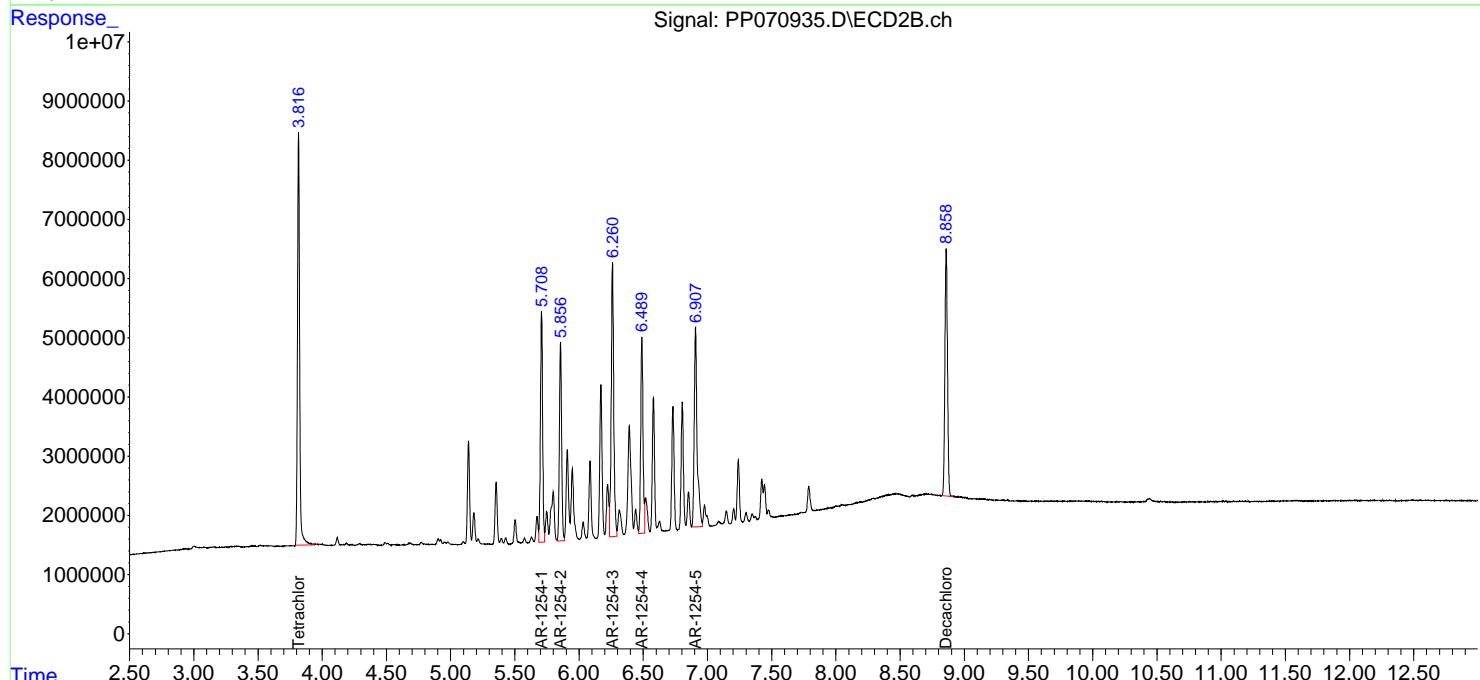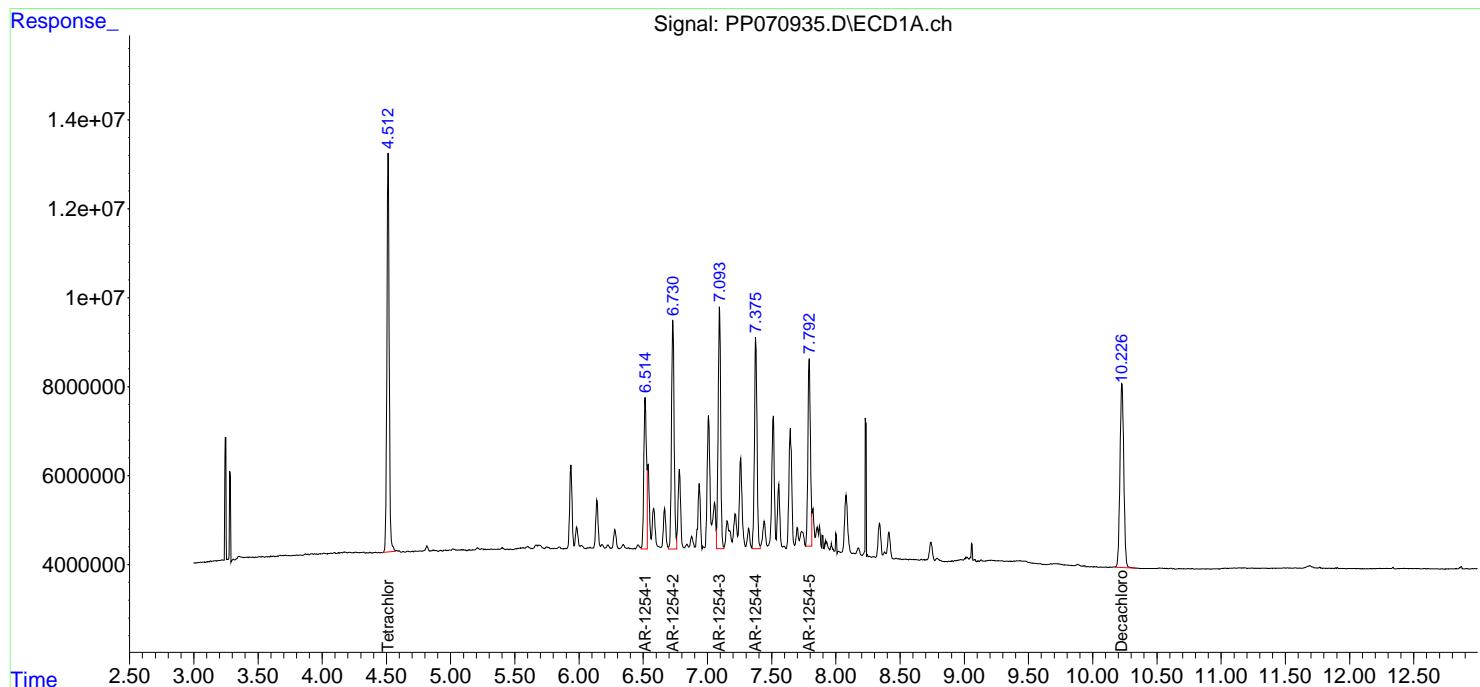

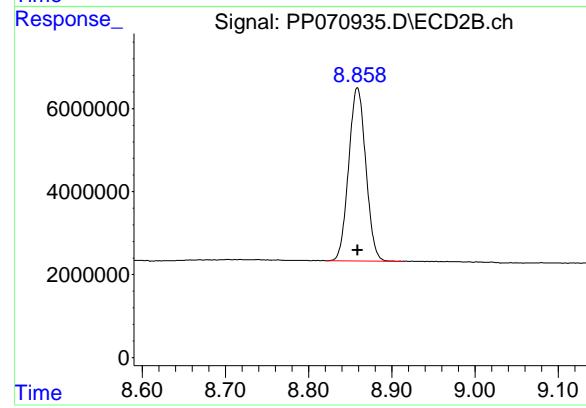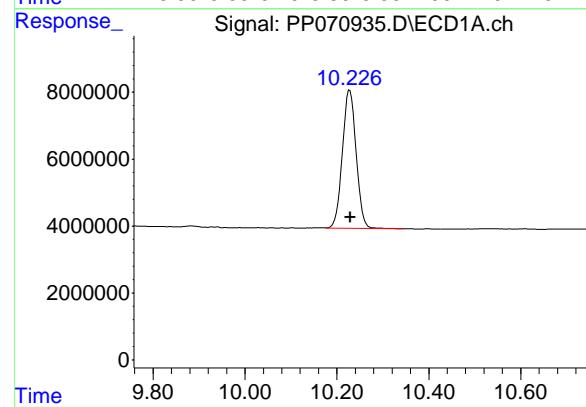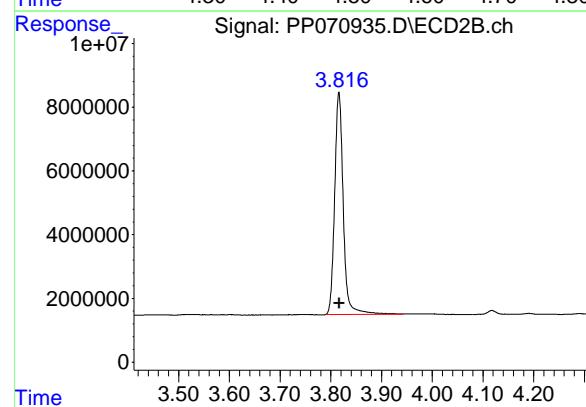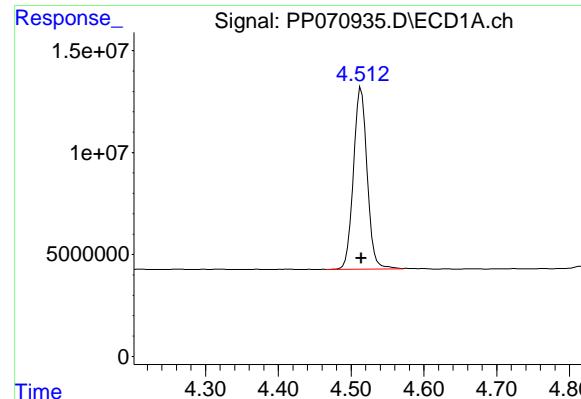

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 116345667  
Conc: 73.84 ng/ml ClientSampleId : AR1254ICC750

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 81865229  
Conc: 73.85 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.228 min  
Delta R.T.: -0.002 min  
Response: 85851924  
Conc: 73.48 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 59713645  
Conc: 65.56 ng/ml

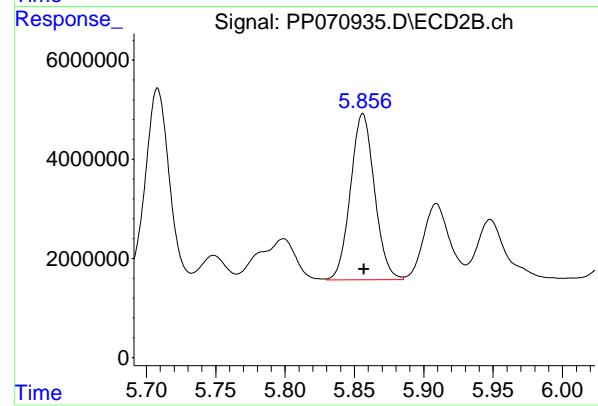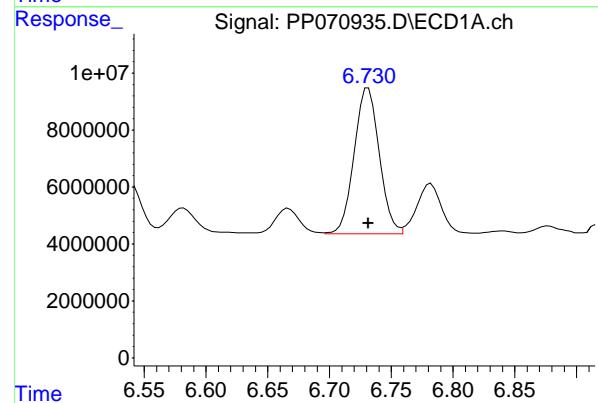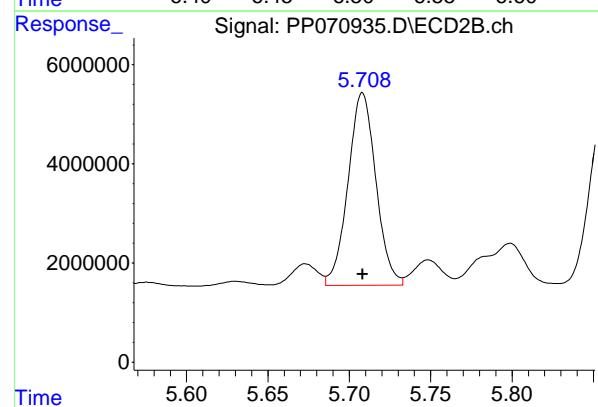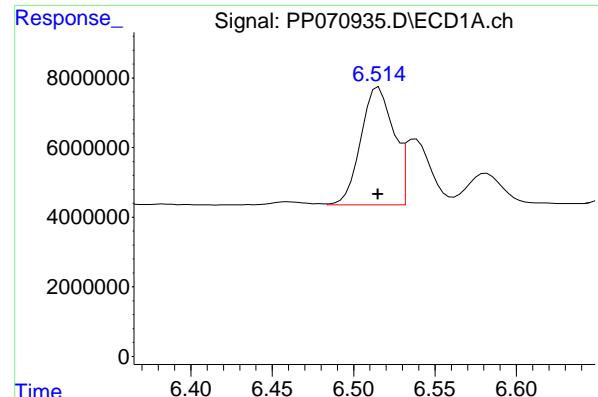

#26 AR-1254-1

R.T.: 6.515 min  
 Delta R.T.: 0.000 min  
 Response: 47300573 ECD\_P  
 Conc: 722.46 ng/ml ClientSampleId : AR1254ICC750

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#26 AR-1254-1

R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 46349687  
 Conc: 701.39 ng/ml

#27 AR-1254-2

R.T.: 6.731 min  
 Delta R.T.: 0.000 min  
 Response: 72785411  
 Conc: 714.97 ng/ml

#27 AR-1254-2

R.T.: 5.856 min  
 Delta R.T.: 0.000 min  
 Response: 40339655  
 Conc: 710.29 ng/ml

#28 AR-1254-3

R.T.: 7.094 min  
 Delta R.T.: 0.000 min  
 Response: 73541603 ECD\_P  
 Conc: 739.73 ng/ml ClientSampleId : AR1254ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#28 AR-1254-3





R.T.: 6.260 min  
 Delta R.T.: 0.000 min  
 Response: 62731680  
 Conc: 714.77 ng/ml

#29 AR-1254-4

R.T.: 7.377 min  
 Delta R.T.: 0.000 min  
 Response: 65835410  
 Conc: 758.45 ng/ml

#29 AR-1254-4

R.T.: 6.490 min  
 Delta R.T.: 0.000 min  
 Response: 40961211  
 Conc: 731.88 ng/ml

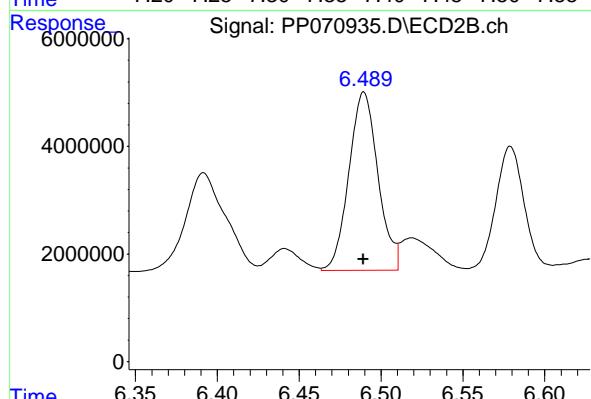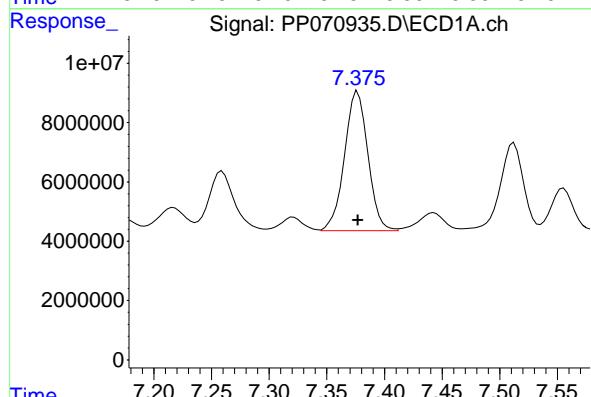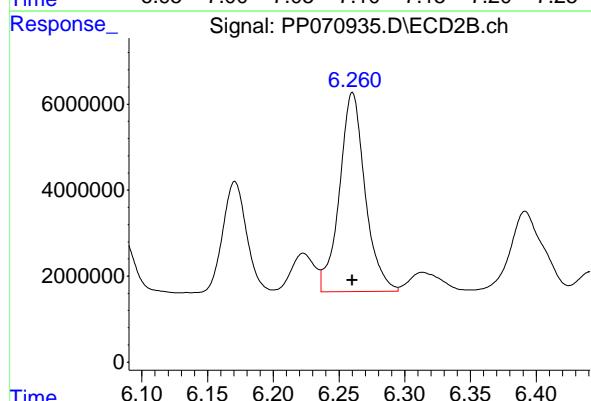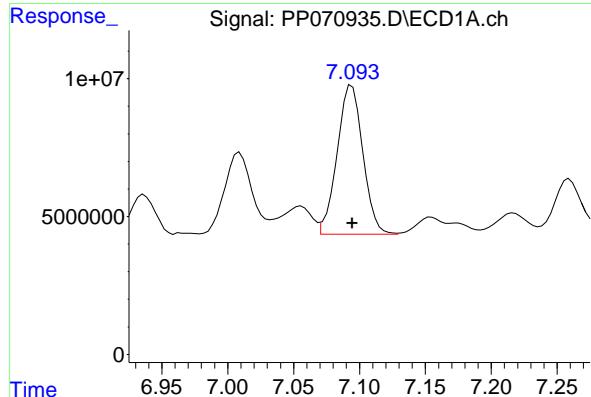

#30 AR-1254-5


R.T.: 7.792 min  
 Delta R.T.: -0.001 min  
 Response: 59278726 ECD\_P  
 Conc: 733.15 ng/ml ClientSampleId :  
 AR1254ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#30 AR-1254-5

R.T.: 6.907 min  
 Delta R.T.: 0.000 min  
 Response: 53519032  
 Conc: 745.12 ng/ml

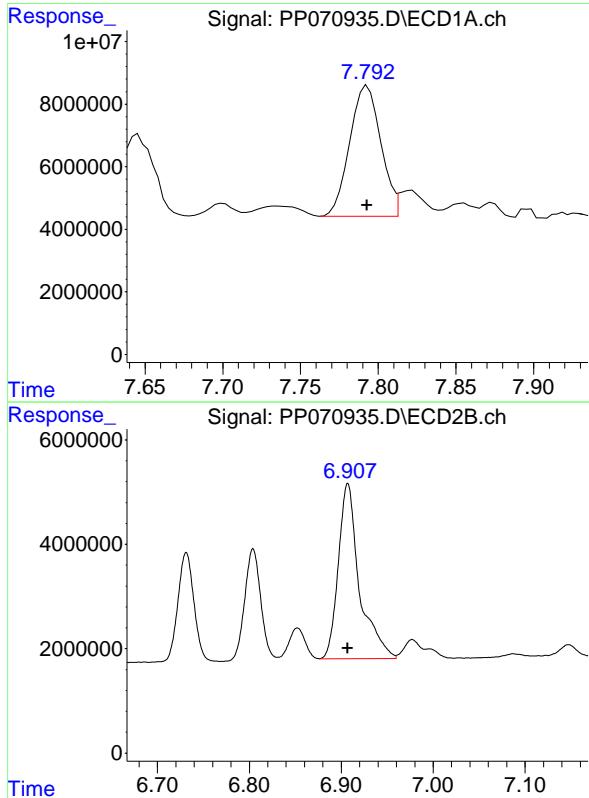

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070936.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:43  
 Operator : YP\AJ  
 Sample : AR1254ICC500  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	4.514	3.816	78787321	55428912	50.000	50.000
2) SA Decachloro...	10.230	8.859	58420861	45541627	50.000	50.000

Target Compounds

26) L6 AR-1254-1	6.515	5.708	32735943	33041243	500.000	500.000
27) L6 AR-1254-2	6.732	5.857	50901196	28396777	500.000	500.000
28) L6 AR-1254-3	7.095	6.260	49708277	43882389	500.000	500.000
29) L6 AR-1254-4	7.377	6.489	43401255	27983450	500.000	500.000
30) L6 AR-1254-5	7.793	6.907	40427325	35912948	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070936.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:43  
 Operator : YP\AJ  
 Sample : AR1254ICC500  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

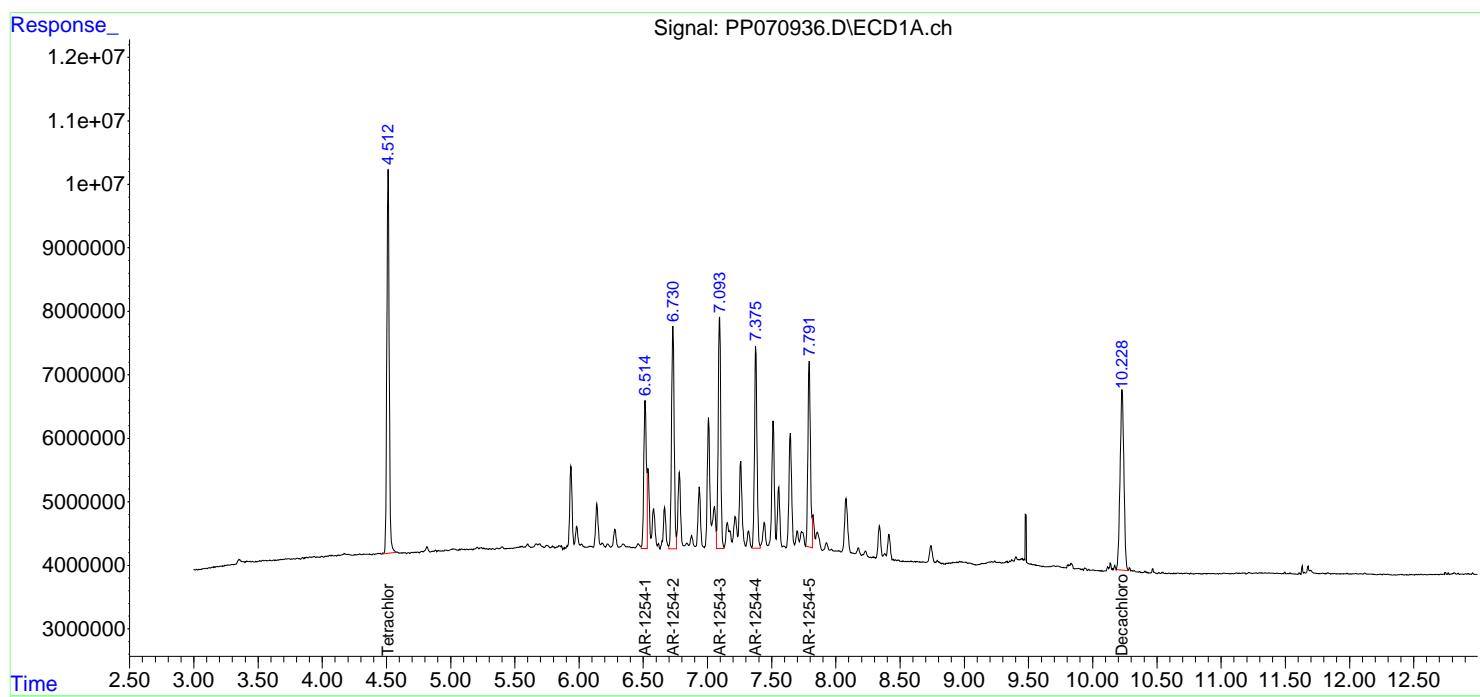

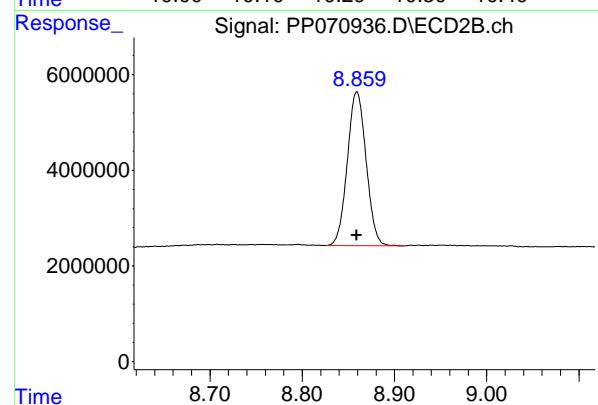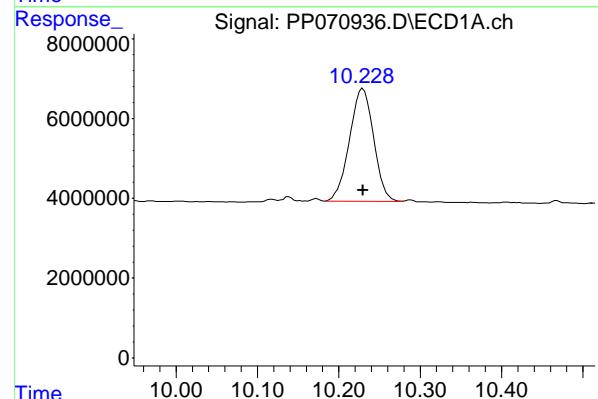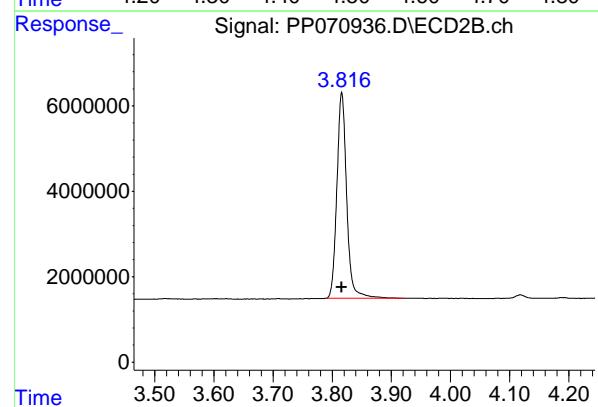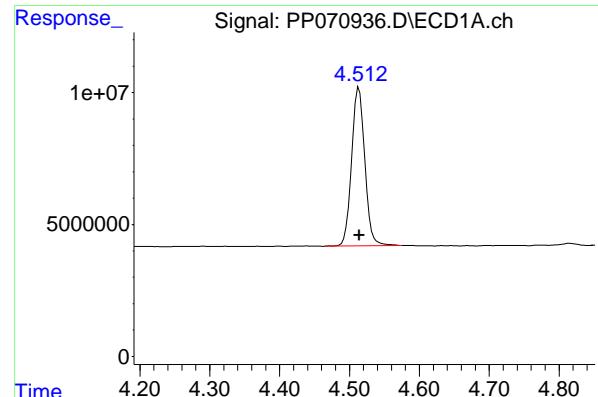

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 78787321  
Conc: 50.00 ng/ml  
ClientSampleId : AR1254ICC500

## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 55428912  
Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl


R.T.: 10.230 min  
Delta R.T.: 0.000 min  
Response: 58420861  
Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 45541627  
Conc: 50.00 ng/ml


#26 AR-1254-1

R.T.: 6.515 min  
 Delta R.T.: 0.000 min  
 Response: 32735943 ECD\_P  
 Conc: 500.00 ng/ml ClientSampleId : AR1254ICC500

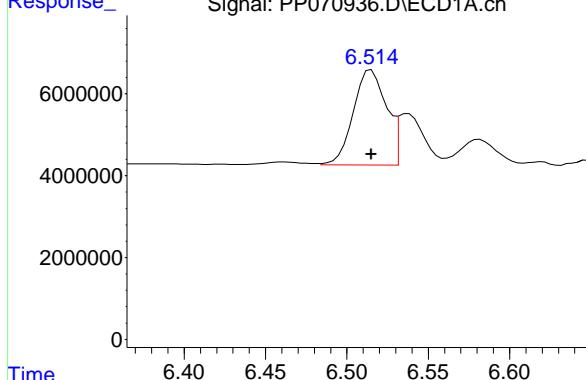


#26 AR-1254-1

R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 33041243  
 Conc: 500.00 ng/ml

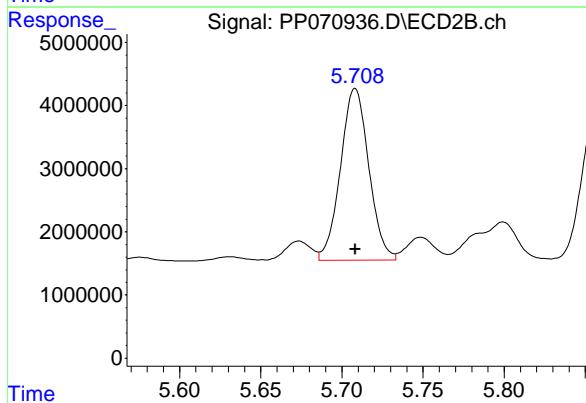


#27 AR-1254-2


R.T.: 6.732 min  
 Delta R.T.: 0.000 min  
 Response: 50901196  
 Conc: 500.00 ng/ml

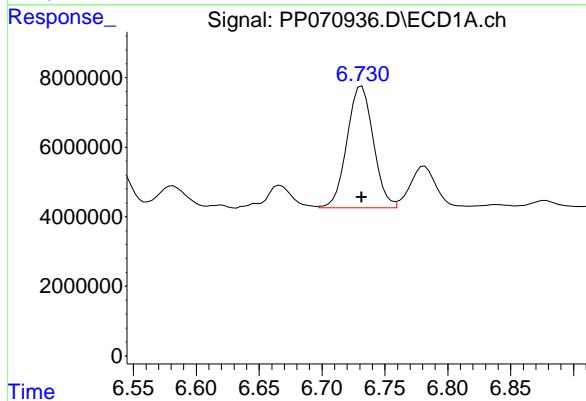

#27 AR-1254-2

R.T.: 5.857 min  
 Delta R.T.: 0.000 min  
 Response: 28396777  
 Conc: 500.00 ng/ml

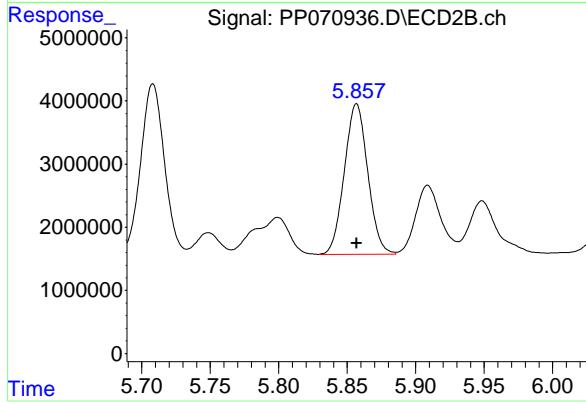

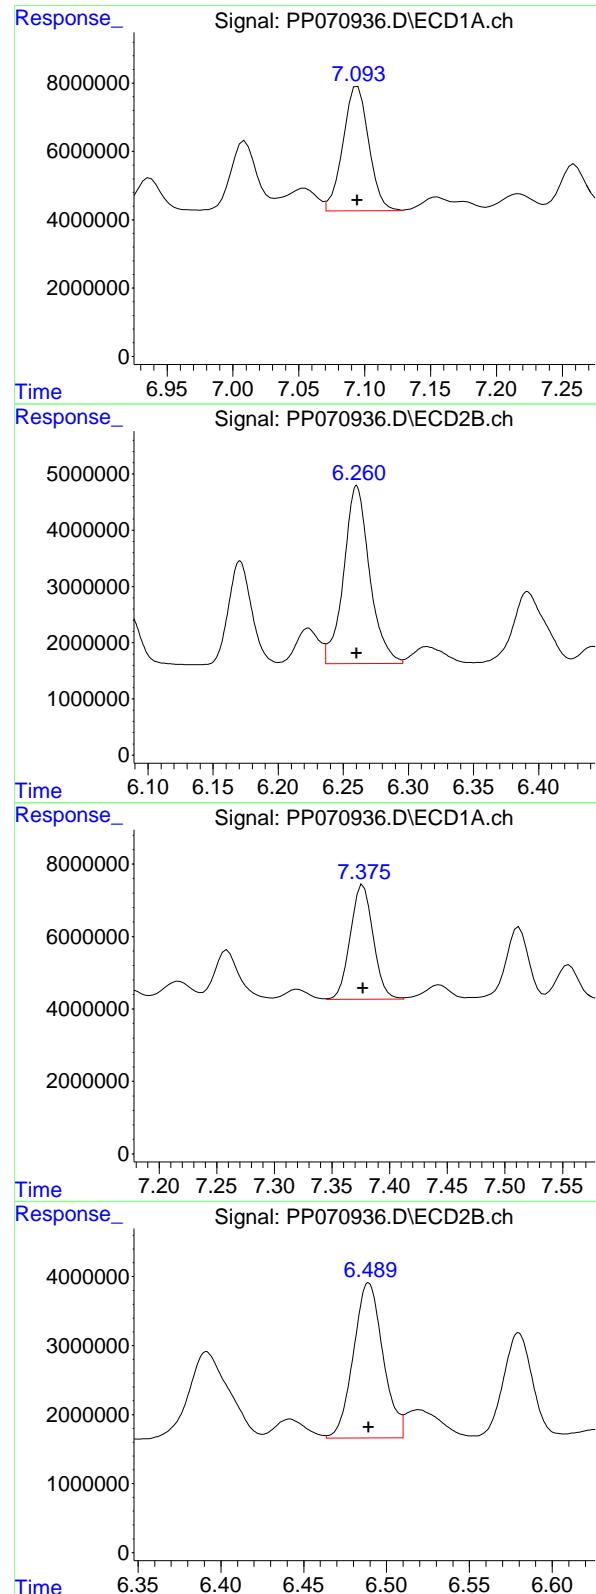

#28 AR-1254-3

R.T.: 7.095 min  
 Delta R.T.: 0.000 min  
 Response: 49708277  
 Conc: 500.00 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1254ICC500

#28 AR-1254-3

R.T.: 6.260 min  
 Delta R.T.: 0.000 min  
 Response: 43882389  
 Conc: 500.00 ng/ml

#29 AR-1254-4


R.T.: 7.377 min  
 Delta R.T.: 0.000 min  
 Response: 43401255  
 Conc: 500.00 ng/ml

#29 AR-1254-4

R.T.: 6.489 min  
 Delta R.T.: 0.000 min  
 Response: 27983450  
 Conc: 500.00 ng/ml


#30 AR-1254-5

R.T.: 7.793 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 40427325  
Conc: 500.00 ng/ml  
ClientSampleId: AR1254ICC500

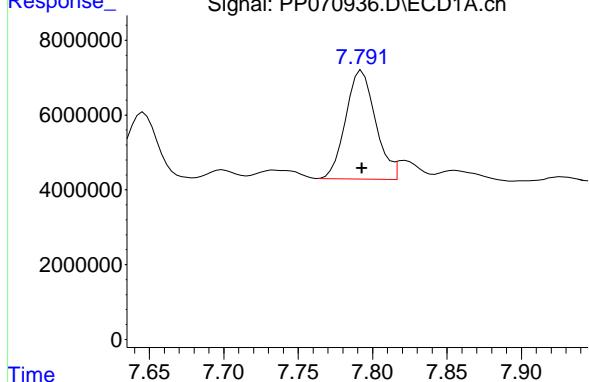

#30 AR-1254-5

R.T.: 6.907 min  
Delta R.T.: 0.000 min  
Response: 35912948  
Conc: 500.00 ng/ml

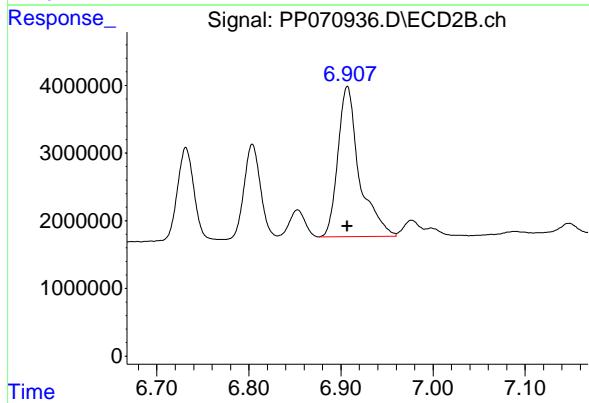

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070937.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:00  
 Operator : YP\AJ  
 Sample : AR1254ICC250  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC250**

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:20:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.514	3.816	40672603	29879101	25.812	26.953
2) SA Decachloro...	10.230	8.859	29858259	21257096	25.554	23.338

**Target Compounds**

26) L6 AR-1254-1	6.516	5.708	16701604	18446961	255.096	279.151
27) L6 AR-1254-2	6.732	5.856	26389026	16008677	259.218	281.875
28) L6 AR-1254-3	7.095	6.260	25960285	24772594	261.126	282.261
29) L6 AR-1254-4	7.377	6.489	22197209	16043587	255.721	286.662
30) L6 AR-1254-5	7.791	6.907	20989646	20606411	259.597m	286.894

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070937.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:00  
 Operator : YP\AJ  
 Sample : AR1254ICC250  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1


Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1254ICC250





**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:20:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

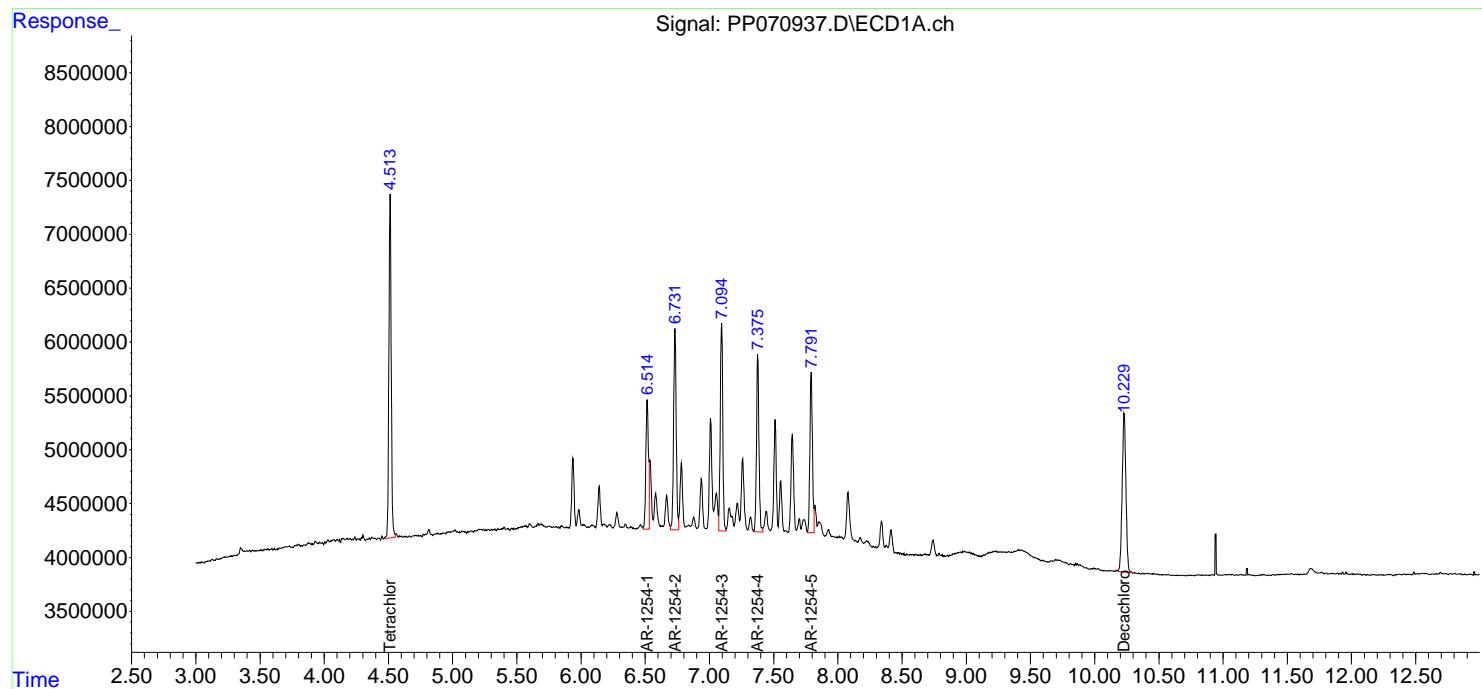

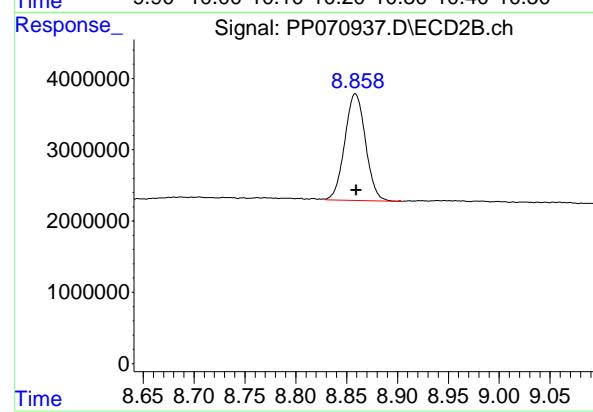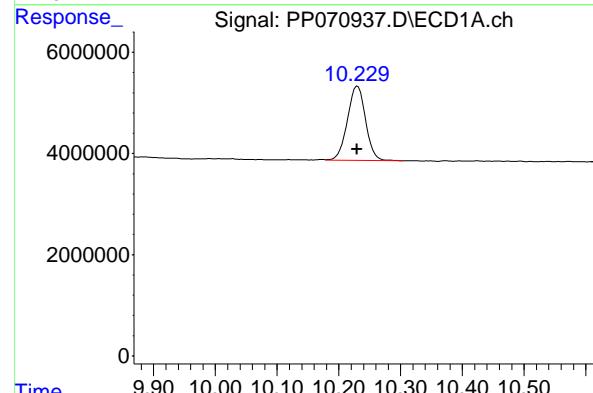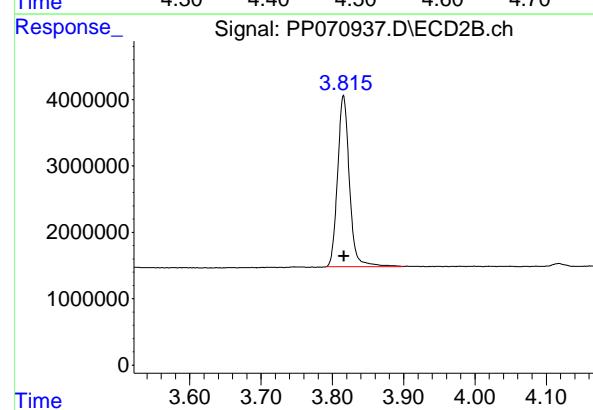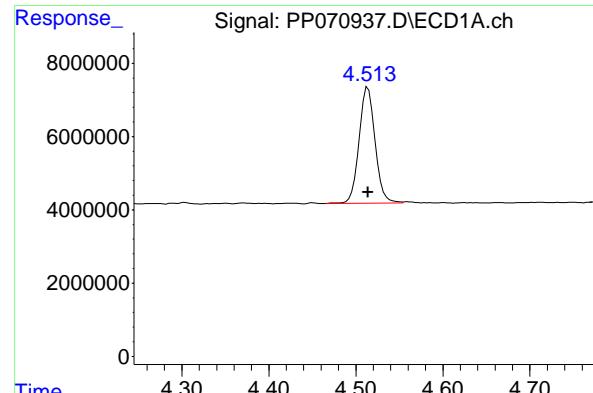

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
 Delta R.T.: 0.000 min  
 Response: 40672603 ECD\_P  
 Conc: 25.81 ng/ml ClientSampleId : AR1254ICC250

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 29879101  
 Conc: 26.95 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.230 min  
 Delta R.T.: 0.000 min  
 Response: 29858259  
 Conc: 25.55 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 21257096  
 Conc: 23.34 ng/ml

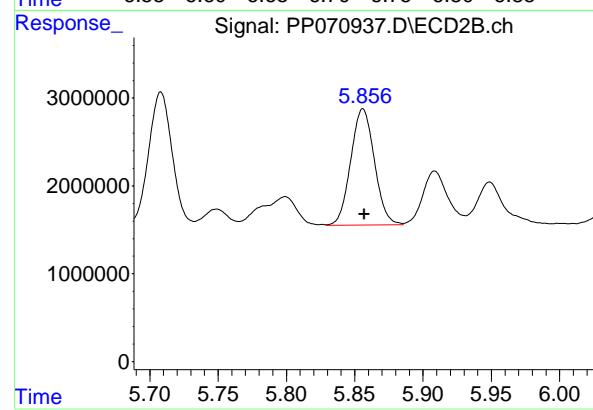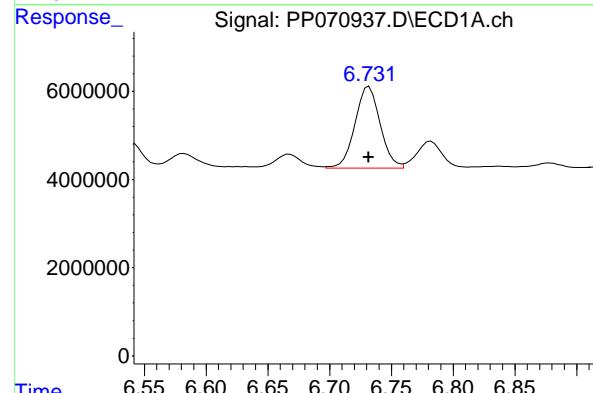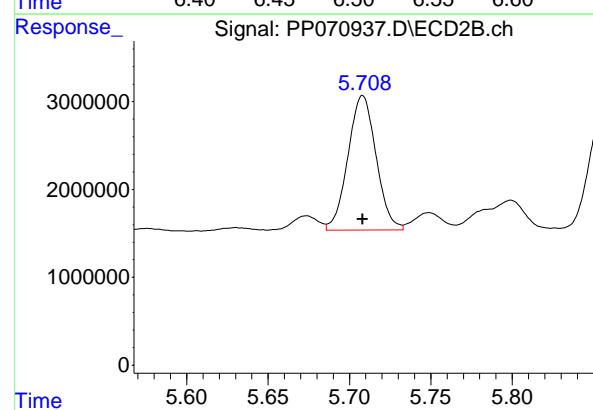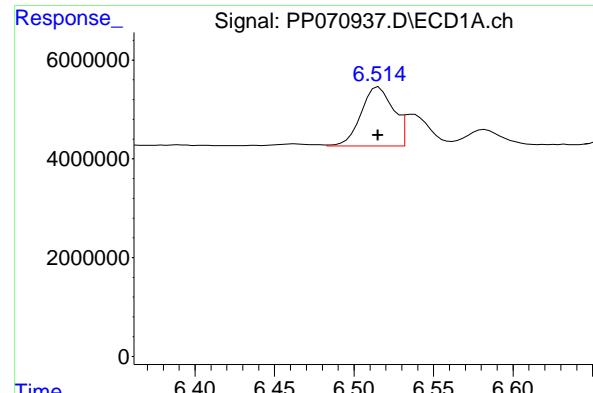

#26 AR-1254-1

R.T.: 6.516 min  
 Delta R.T.: 0.000 min  
 Response: 16701604 ECD\_P  
 Conc: 255.10 ng/ml ClientSampleId : AR1254ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#26 AR-1254-1

R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 18446961  
 Conc: 279.15 ng/ml

#27 AR-1254-2

R.T.: 6.732 min  
 Delta R.T.: 0.000 min  
 Response: 26389026  
 Conc: 259.22 ng/ml

#27 AR-1254-2

R.T.: 5.856 min  
 Delta R.T.: 0.000 min  
 Response: 16008677  
 Conc: 281.87 ng/ml

#28 AR-1254-3

R.T.: 7.095 min  
 Delta R.T.: 0.000 min  
 Response: 25960285  
 Conc: 261.13 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId :** AR1254ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#28 AR-1254-3





R.T.: 6.260 min  
 Delta R.T.: 0.000 min  
 Response: 24772594  
 Conc: 282.26 ng/ml

#29 AR-1254-4

R.T.: 7.377 min  
 Delta R.T.: 0.000 min  
 Response: 22197209  
 Conc: 255.72 ng/ml

#29 AR-1254-4

R.T.: 6.489 min  
 Delta R.T.: 0.000 min  
 Response: 16043587  
 Conc: 286.66 ng/ml

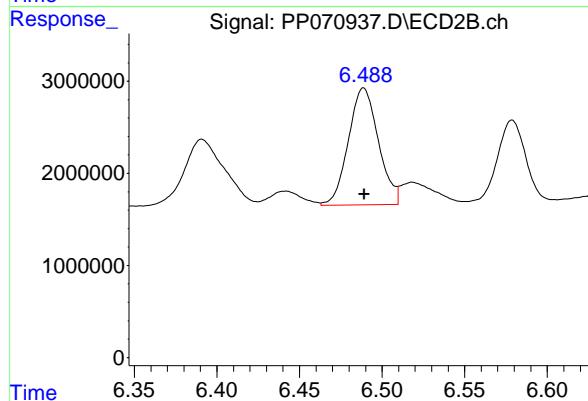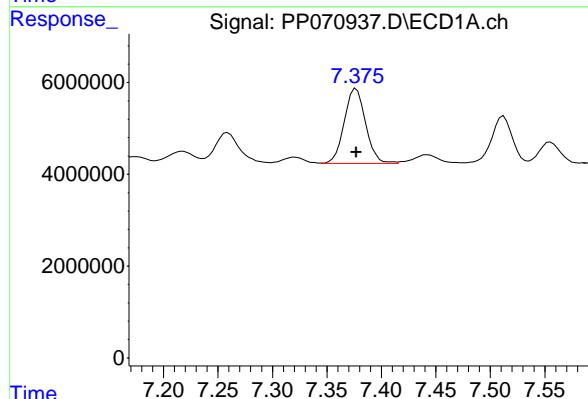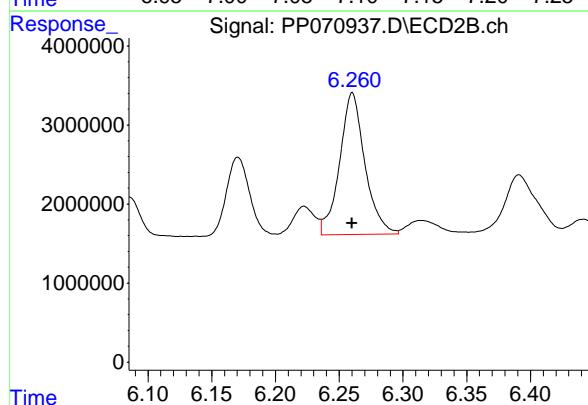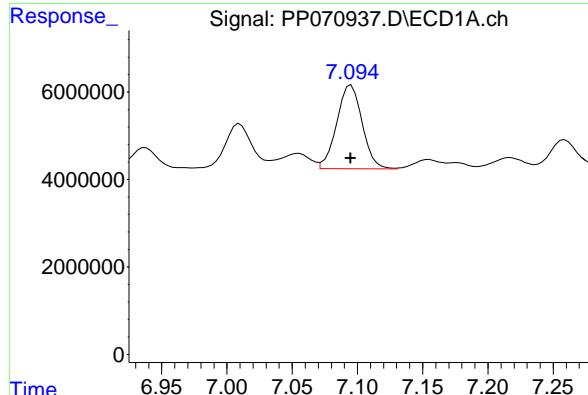

#30 AR-1254-5


R.T.: 7.791 min  
 Delta R.T.: -0.001 min  
 Response: 20989646 ECD\_P  
 Conc: 259.60 ng/ml ClientSampleId :  
 AR1254ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#30 AR-1254-5

R.T.: 6.907 min  
 Delta R.T.: 0.000 min  
 Response: 20606411  
 Conc: 286.89 ng/ml

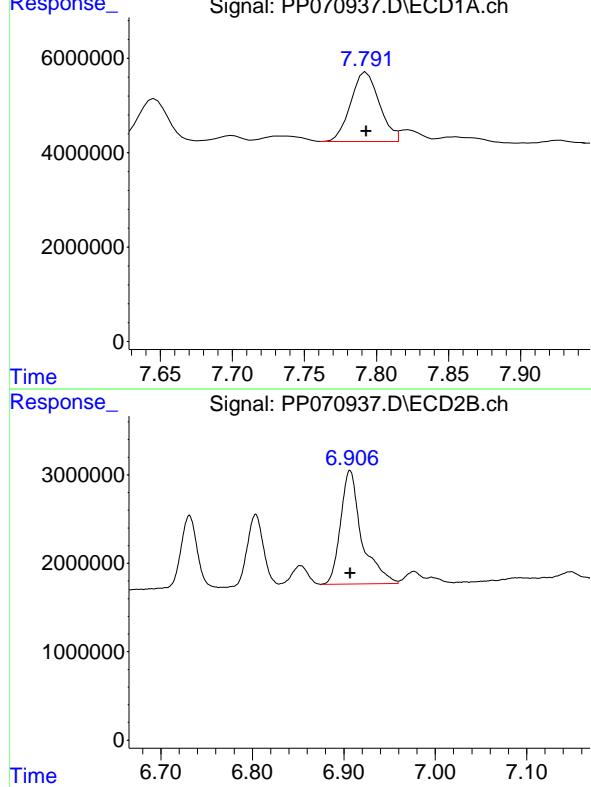

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070938.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:16  
 Operator : YP\AJ  
 Sample : AR1254ICC050  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:35:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.515	3.816	6508593	5336776	4.107	4.715
2) SA Decachlor...	10.232	8.861	5177583	3796388	4.429	4.454

Target Compounds

26) L6 AR-1254-1	6.516	5.708	3322396	3474548	51.023	51.687
27) L6 AR-1254-2	6.733	5.857	5410437	3036515	53.321	52.169
28) L6 AR-1254-3	7.096	6.261	5249564	4313044	52.267	47.835
29) L6 AR-1254-4	7.378	6.490	4268685	2787399	48.623	47.851
30) L6 AR-1254-5	7.794	6.907	4173507	3458194	51.345	45.985


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070938.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:16  
 Operator : YP\AJ  
 Sample : AR1254ICC050  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:35:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

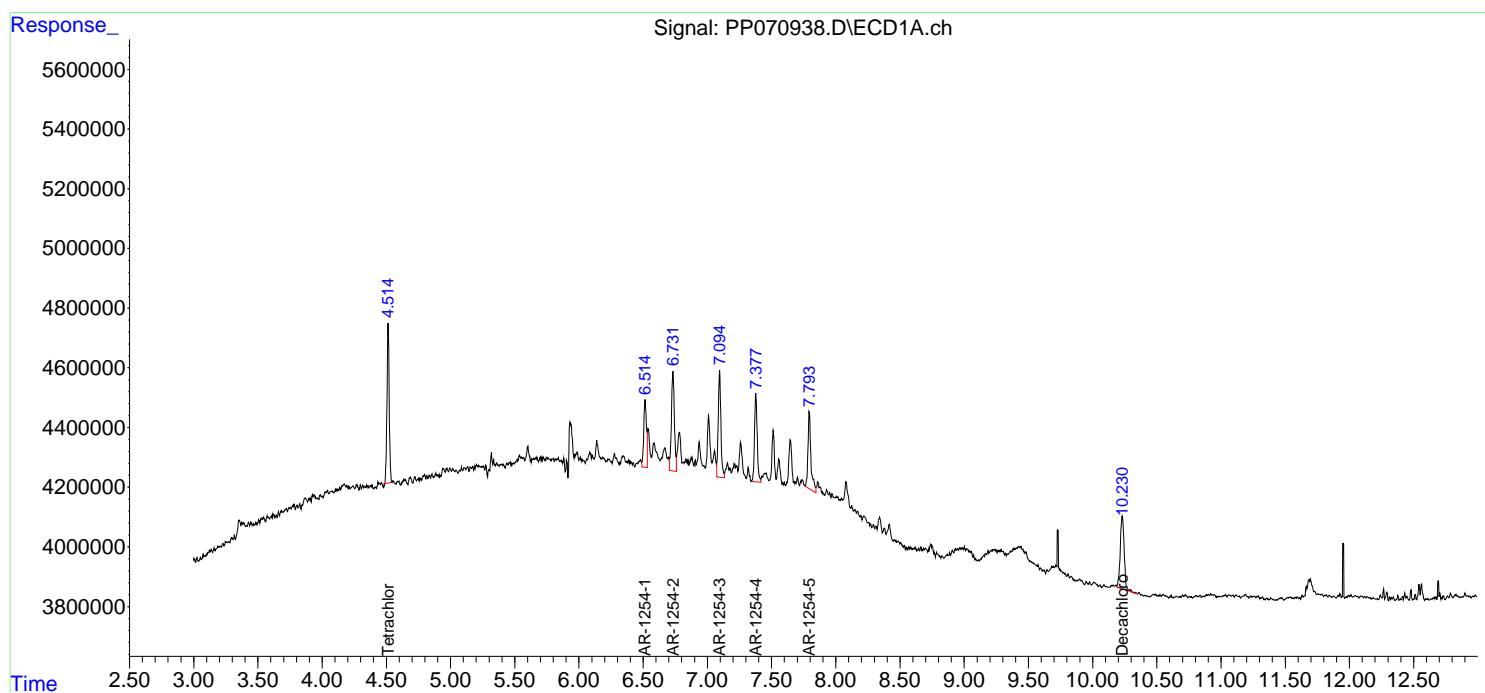

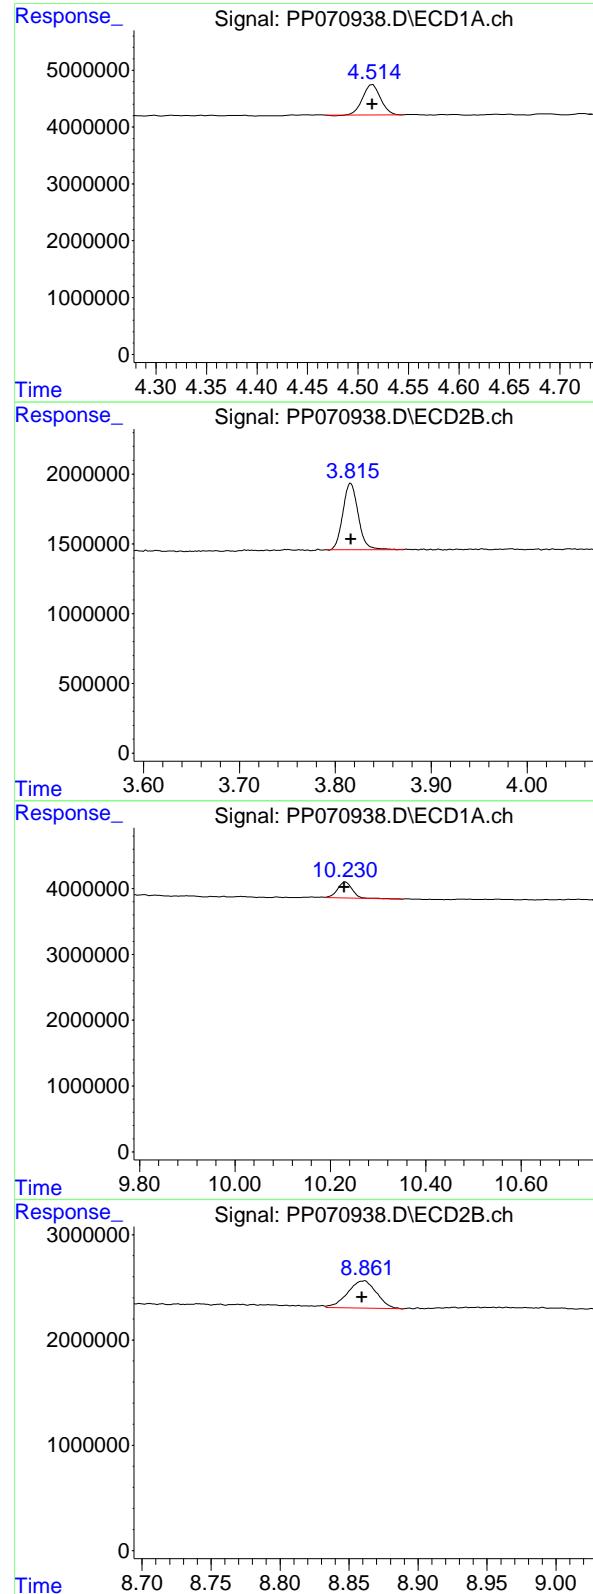

## #1 Tetrachloro-m-xylene

R.T.: 4.515 min  
Delta R.T.: 0.000 min  
Instrument:  
Response: 6508593 ECD\_P  
Conc: 4.11 ng/ml ClientSampleId : AR1254ICC050

## #1 Tetrachloro-m-xylene


R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 5336776  
Conc: 4.72 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.232 min  
Delta R.T.: 0.002 min  
Response: 5177583  
Conc: 4.43 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.861 min  
Delta R.T.: 0.001 min  
Response: 3796388  
Conc: 4.45 ng/ml

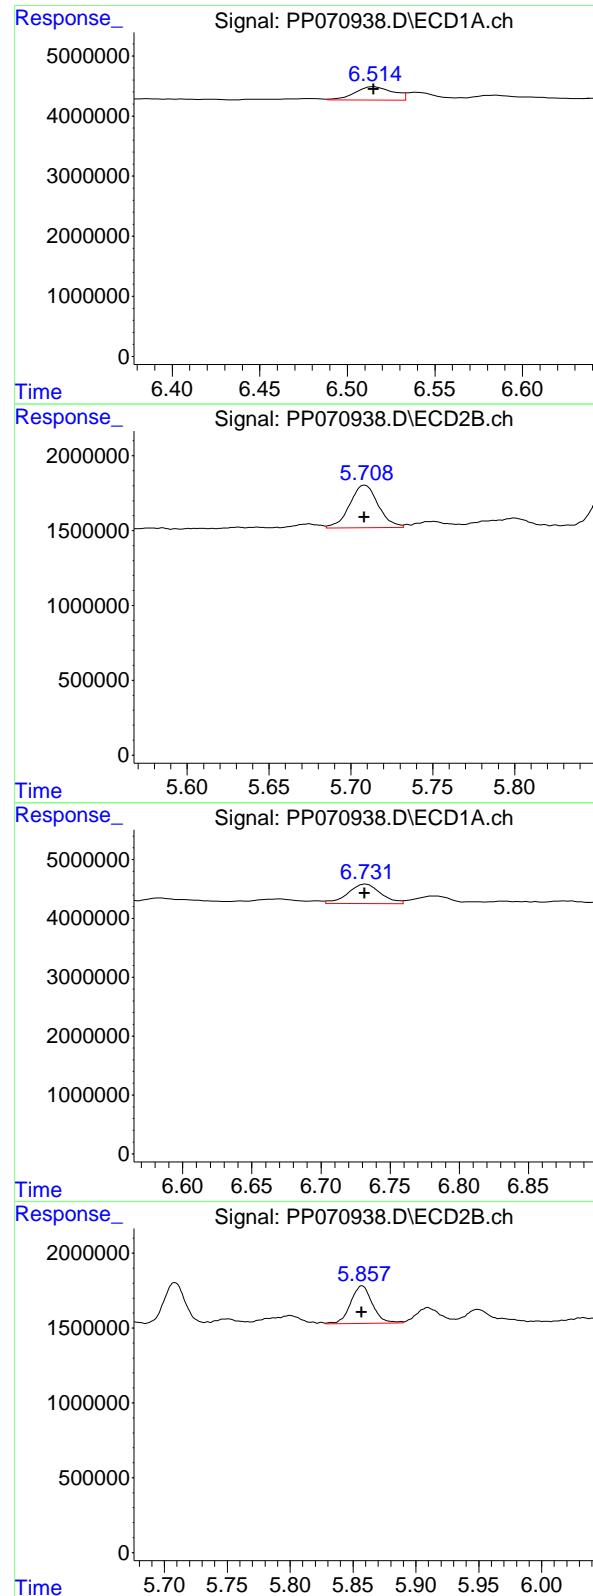

#26 AR-1254-1

R.T.: 6.516 min  
 Delta R.T.: 0.000 min  
 Response: 3322396 ECD\_P  
 Conc: 51.02 ng/ml ClientSampleId : AR1254ICC050

#26 AR-1254-1

R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 3474548  
 Conc: 51.69 ng/ml

#27 AR-1254-2


R.T.: 6.733 min  
 Delta R.T.: 0.001 min  
 Response: 5410437  
 Conc: 53.32 ng/ml

#27 AR-1254-2

R.T.: 5.857 min  
 Delta R.T.: 0.000 min  
 Response: 3036515  
 Conc: 52.17 ng/ml


#28 AR-1254-3

R.T.: 7.096 min  
 Delta R.T.: 0.001 min  
 Response: 5249564 ECD\_P  
 Conc: 52.27 ng/ml ClientSampleId : AR1254ICC050

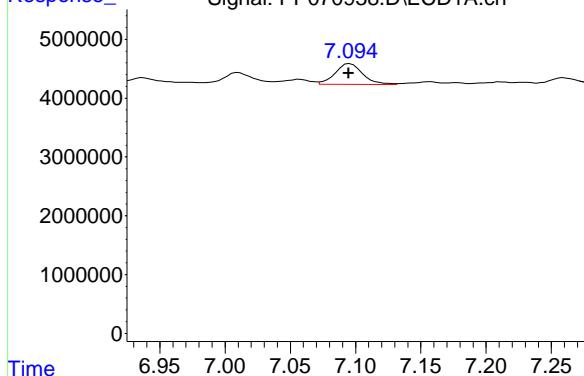


#28 AR-1254-3

R.T.: 6.261 min  
 Delta R.T.: 0.000 min  
 Response: 4313044  
 Conc: 47.83 ng/ml

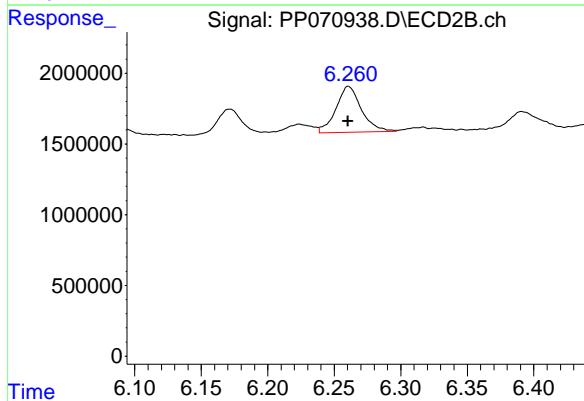


#29 AR-1254-4

R.T.: 7.378 min  
 Delta R.T.: 0.001 min  
 Response: 4268685  
 Conc: 48.62 ng/ml

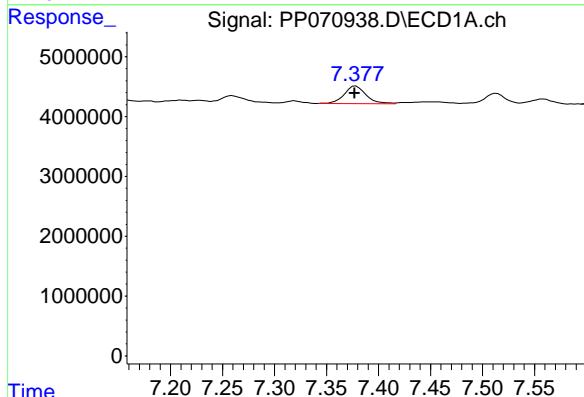


#29 AR-1254-4

R.T.: 6.490 min  
 Delta R.T.: 0.000 min  
 Response: 2787399  
 Conc: 47.85 ng/ml

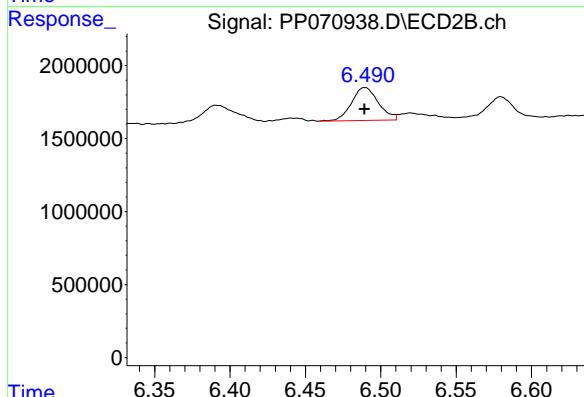


#30 AR-1254-5

R.T.: 7.794 min  
Delta R.T.: 0.002 min  
Instrument: ECD\_P  
Response: 4173507  
Conc: 51.34 ng/ml  
ClientSampleId: AR1254ICC050

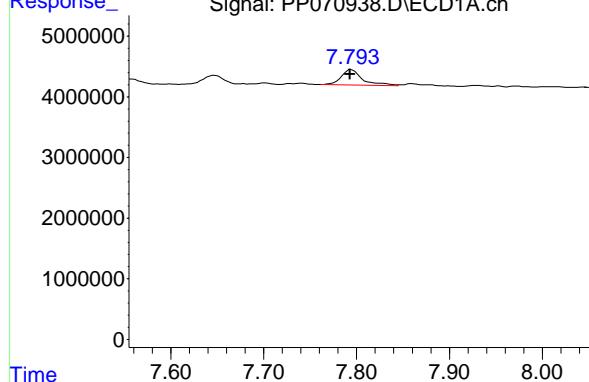

#30 AR-1254-5

R.T.: 6.907 min  
Delta R.T.: 0.000 min  
Response: 3458194  
Conc: 45.98 ng/ml

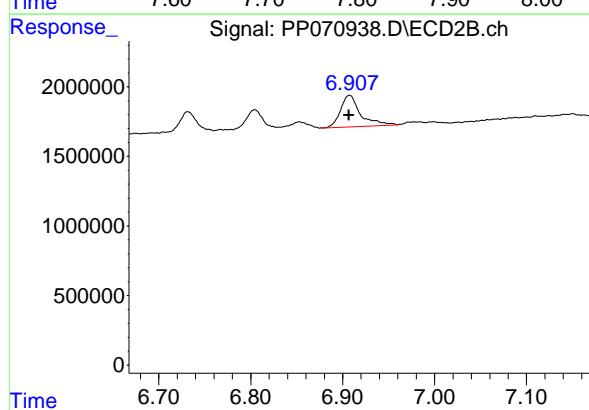

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070939.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:32  
 Operator : YP\AJ  
 Sample : AR1262ICC500  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1262ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:04:37 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.512	3.816	78302128	53762587	50.000	50.000
2) SA Decachloro...	10.226	8.859	57984668	42902548	50.000	50.000

**Target Compounds**

36) L8 AR-1262-1	8.093	6.945	53150122	42781773	500.000	500.000
37) L8 AR-1262-2	8.412	7.205	99191436	34232243	500.000	500.000
38) L8 AR-1262-3	8.729	7.729	65870896	30361758	500.000	500.000
39) L8 AR-1262-4	8.817	7.793	47807443	49703360	500.000	500.000
40) L8 AR-1262-5	9.469	8.294	32533206	23435811	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070939.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:32  
 Operator : YP\AJ  
 Sample : AR1262ICC500  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1262ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:04:37 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

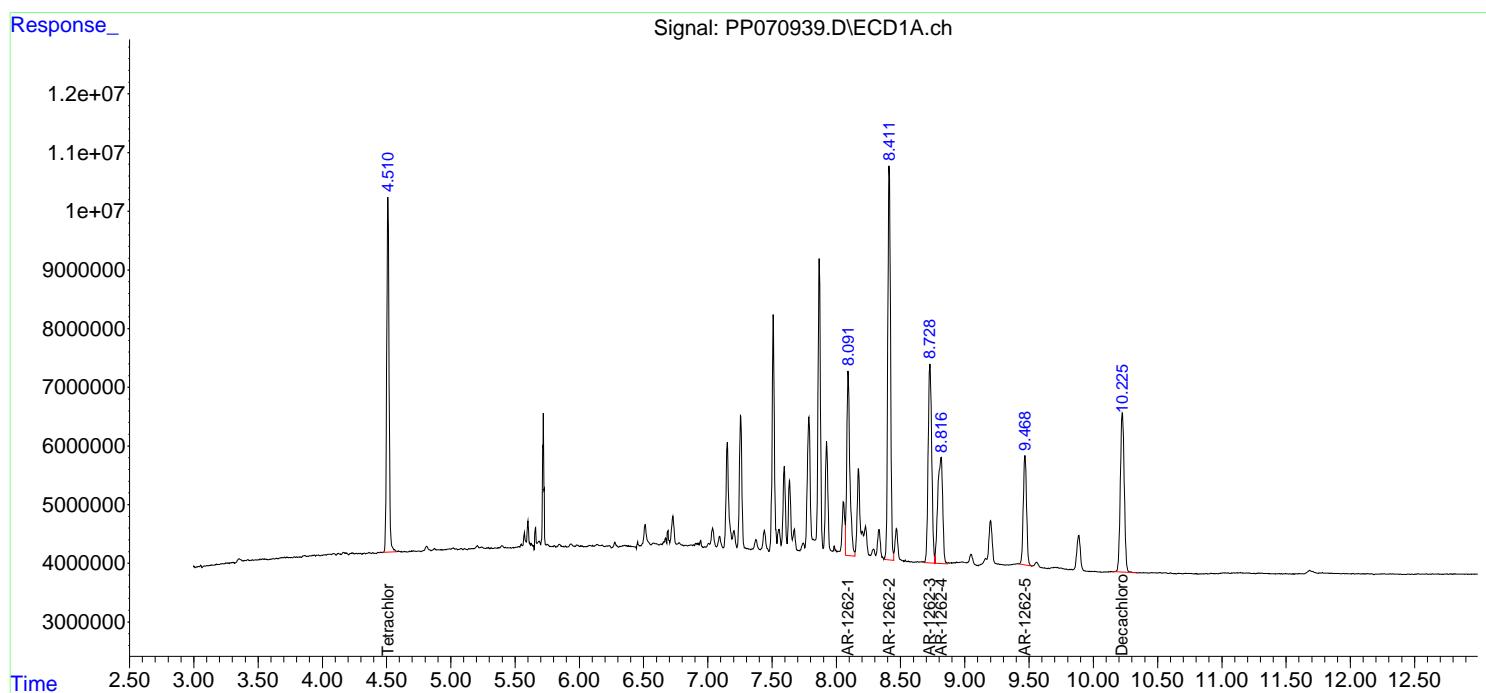

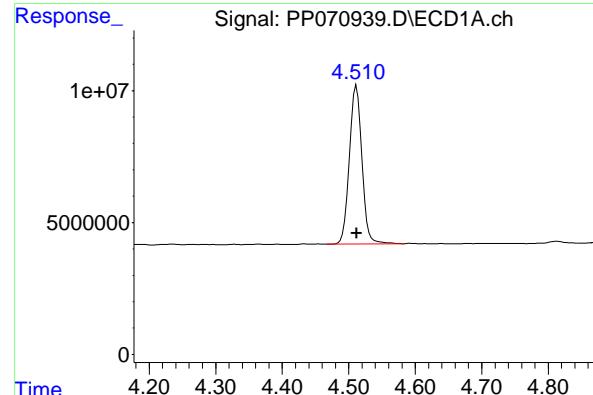


## #1 Tetrachloro-m-xylene

R.T.: 4.512 min  
 Delta R.T.: 0.000 min  
 Response: 78302128 ECD\_P  
 Conc: 50.00 ng/ml ClientSampleId : AR1262ICC500

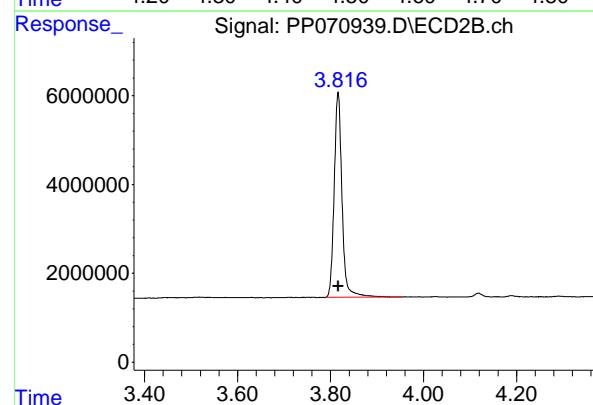


## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 53762587  
 Conc: 50.00 ng/ml

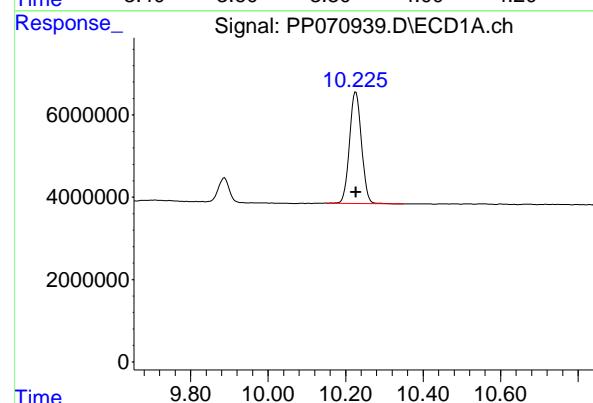


## #2 Decachlorobiphenyl

R.T.: 10.226 min  
 Delta R.T.: 0.000 min  
 Response: 57984668  
 Conc: 50.00 ng/ml

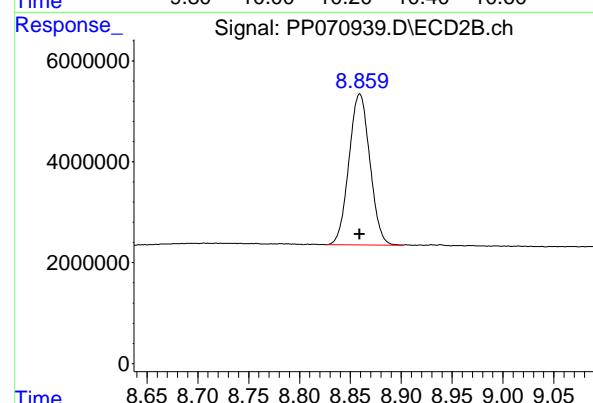

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 42902548  
 Conc: 50.00 ng/ml

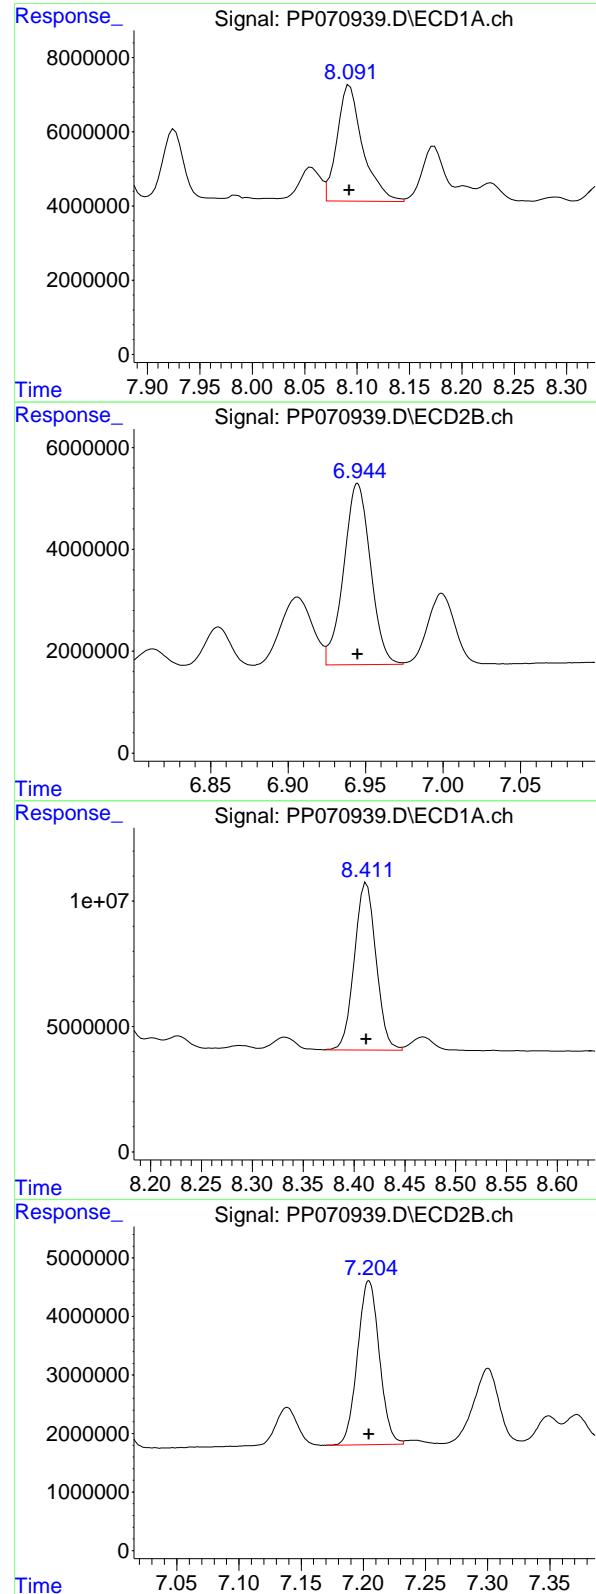

#36 AR-1262-1

R.T.: 8.093 min  
 Delta R.T.: 0.000 min  
 Response: 53150122  
 Conc: 500.00 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1262ICC500

#36 AR-1262-1

R.T.: 6.945 min  
 Delta R.T.: 0.000 min  
 Response: 42781773  
 Conc: 500.00 ng/ml

#37 AR-1262-2


R.T.: 8.412 min  
 Delta R.T.: 0.000 min  
 Response: 99191436  
 Conc: 500.00 ng/ml

#37 AR-1262-2

R.T.: 7.205 min  
 Delta R.T.: 0.000 min  
 Response: 34232243  
 Conc: 500.00 ng/ml


#38 AR-1262-3

R.T.: 8.729 min  
 Delta R.T.: 0.000 min  
 Response: 65870896 ECD\_P  
 Conc: 500.00 ng/ml ClientSampleId : AR1262ICC500

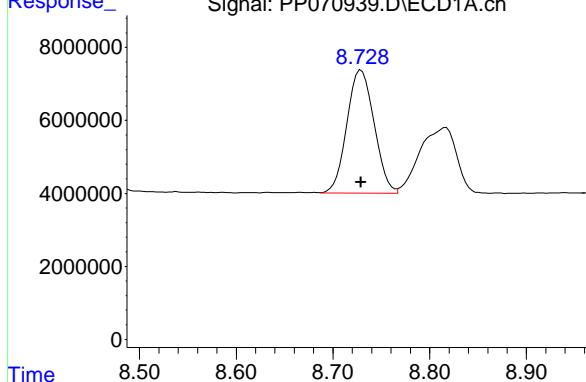


#38 AR-1262-3

R.T.: 7.729 min  
 Delta R.T.: 0.000 min  
 Response: 30361758  
 Conc: 500.00 ng/ml

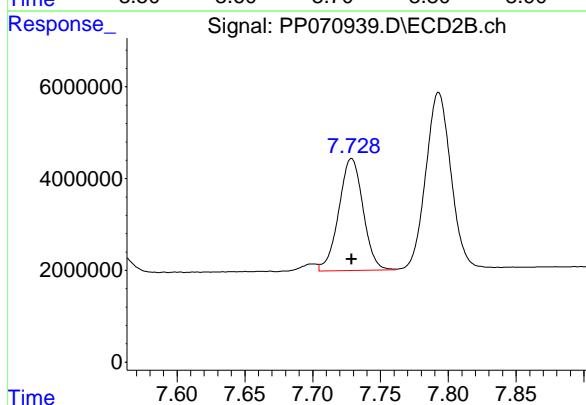


#39 AR-1262-4

R.T.: 8.817 min  
 Delta R.T.: 0.000 min  
 Response: 47807443  
 Conc: 500.00 ng/ml

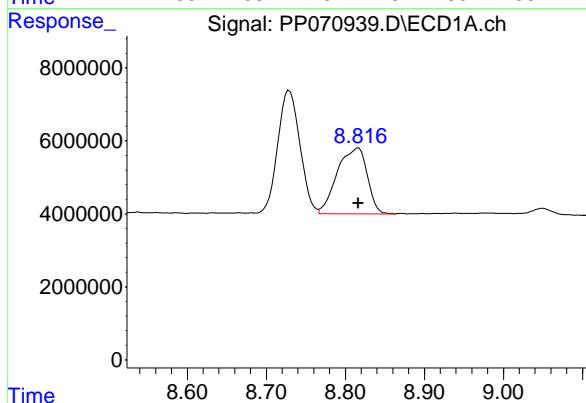


#39 AR-1262-4

R.T.: 7.793 min  
 Delta R.T.: 0.000 min  
 Response: 49703360  
 Conc: 500.00 ng/ml

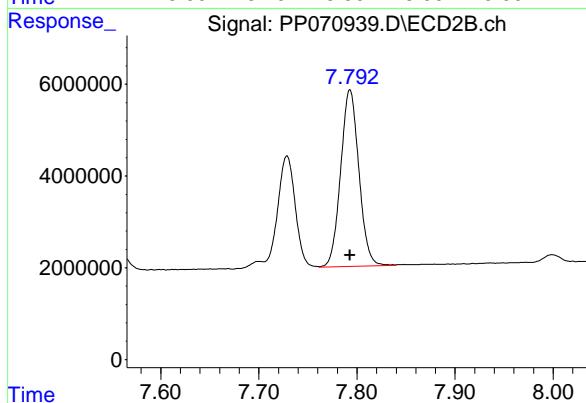


#40 AR-1262-5

R.T.: 9.469 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 32533206  
Conc: 500.00 ng/ml  
ClientSampleId: AR1262ICC500

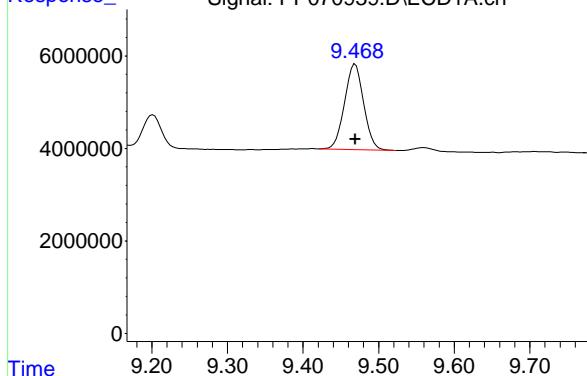

#40 AR-1262-5

R.T.: 8.294 min  
Delta R.T.: 0.000 min  
Response: 23435811  
Conc: 500.00 ng/ml

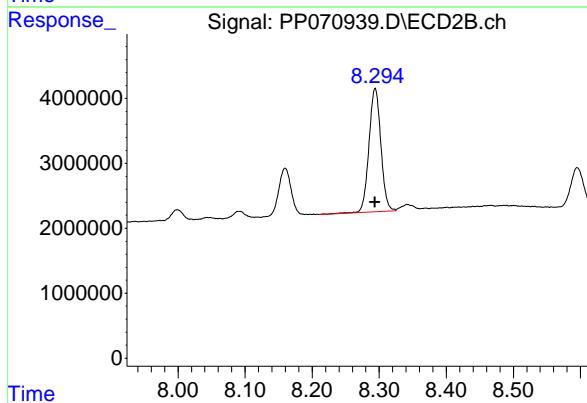

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070940.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:48  
 Operator : YP\AJ  
 Sample : AR1268ICC1000  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
AR1268ICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.516	3.817	152.3E6	105.1E6	94.769	94.009
2) SA Decachloro...	10.232	8.860	195.7E6	148.5E6	93.377	94.968

**Target Compounds**

41) L9 AR-1268-1	8.730	7.729	226.6E6	165.4E6	945.404	946.509m
42) L9 AR-1268-2	8.824	7.795	190.4E6	137.8E6	950.797	945.407
43) L9 AR-1268-3	9.056	8.001	163.6E6	120.1E6	940.749	965.766
44) L9 AR-1268-4	9.474	8.295	70377008	51096977	960.945	957.859
45) L9 AR-1268-5	9.891	8.596	459.6E6	357.1E6	952.414	962.556

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070940.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:48  
 Operator : YP\AJ  
 Sample : AR1268ICC1000  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_P  
**ClientSampleId :**  
 AR1268ICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

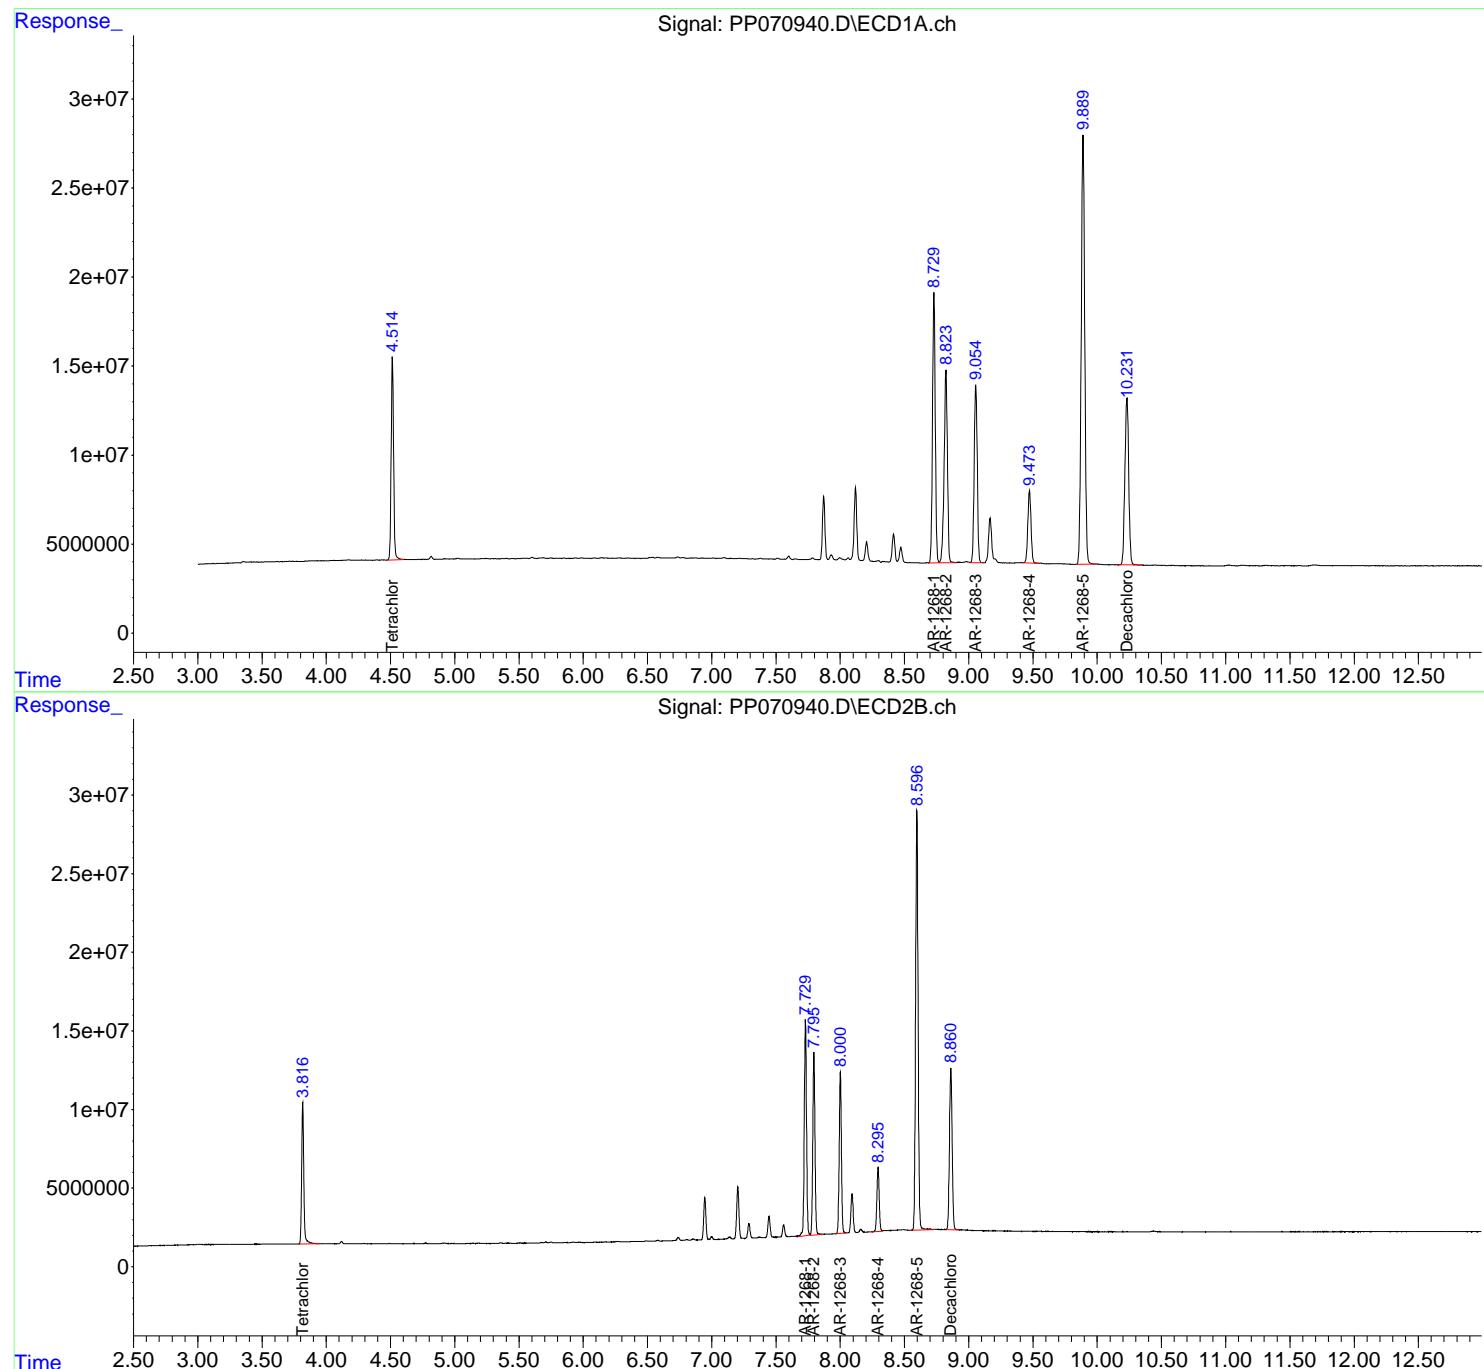

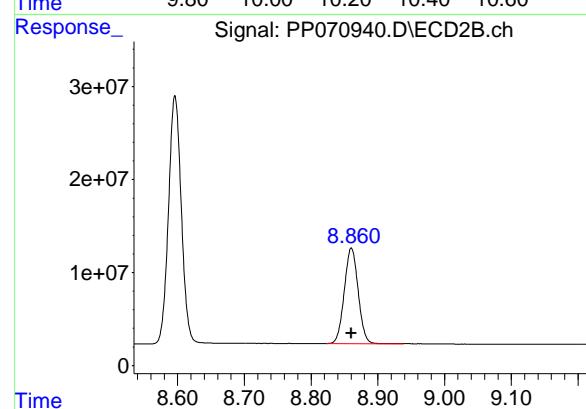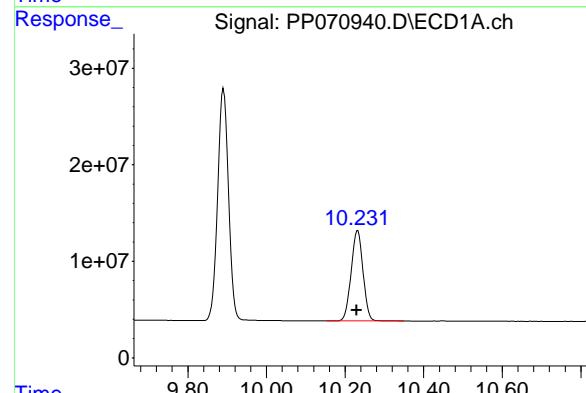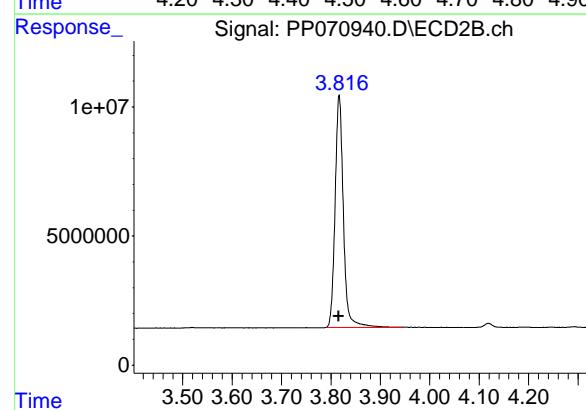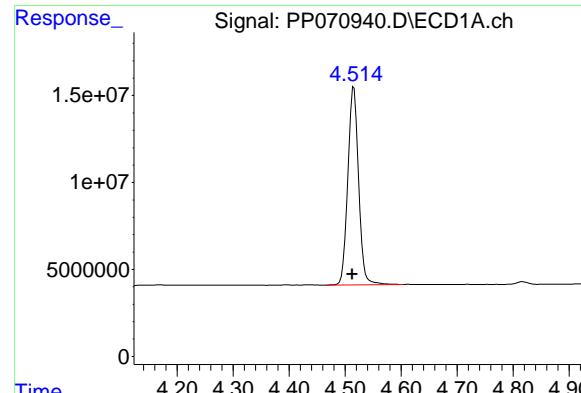

## #1 Tetrachloro-m-xylene

R.T.: 4.516 min  
Delta R.T.: 0.003 min  
Instrument:  
Response: 152348529 ECD\_P  
Conc: 94.77 ng/ml ClientSampleId : AR1268ICC1000

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene



R.T.: 3.817 min  
Delta R.T.: 0.000 min  
Response: 105128984  
Conc: 94.01 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.232 min  
Delta R.T.: 0.003 min  
Response: 195698435  
Conc: 93.38 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.860 min  
Delta R.T.: 0.000 min  
Response: 148482089  
Conc: 94.97 ng/ml

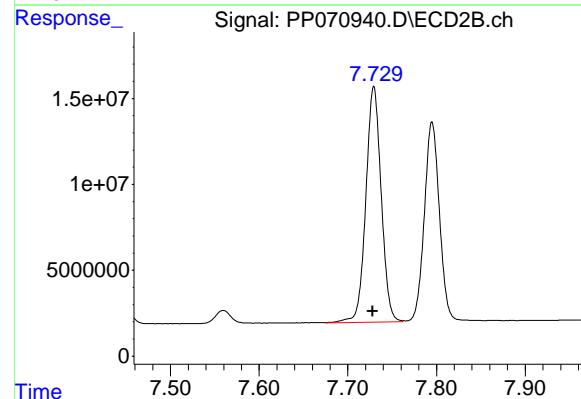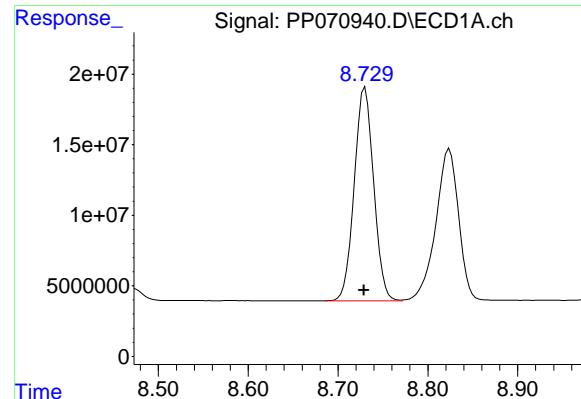

#41 AR-1268-1

R.T.: 8.730 min  
 Delta R.T.: 0.001 min  
 Response: 226575551  
 Conc: 945.40 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1268ICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#41 AR-1268-1

R.T.: 7.729 min  
 Delta R.T.: 0.001 min  
 Response: 165356134  
 Conc: 946.51 ng/ml

#42 AR-1268-2

R.T.: 8.824 min  
 Delta R.T.: 0.003 min  
 Response: 190380276  
 Conc: 950.80 ng/ml

#42 AR-1268-2

R.T.: 7.795 min  
 Delta R.T.: 0.001 min  
 Response: 137801505  
 Conc: 945.41 ng/ml

#43 AR-1268-3

R.T.: 9.056 min  
 Delta R.T.: 0.003 min  
 Response: 163648333  
 Conc: 940.75 ng/ml  
 Instrument: ECD\_P  
 ClientSampleId : AR1268ICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#43 AR-1268-3



R.T.: 8.001 min  
 Delta R.T.: 0.001 min  
 Response: 120132746  
 Conc: 965.77 ng/ml

#44 AR-1268-4

R.T.: 9.474 min  
 Delta R.T.: 0.002 min  
 Response: 70377008  
 Conc: 960.95 ng/ml

#44 AR-1268-4

R.T.: 8.295 min  
 Delta R.T.: 0.002 min  
 Response: 51096977  
 Conc: 957.86 ng/ml

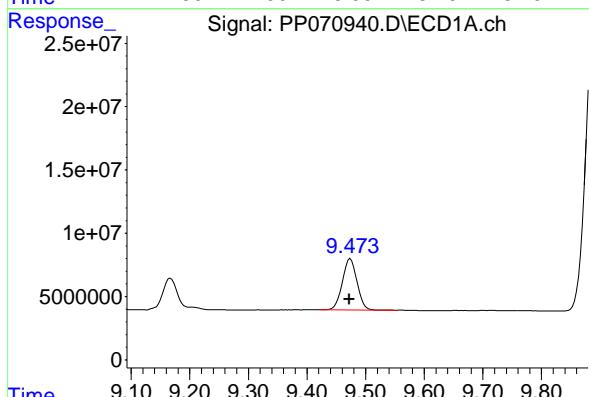
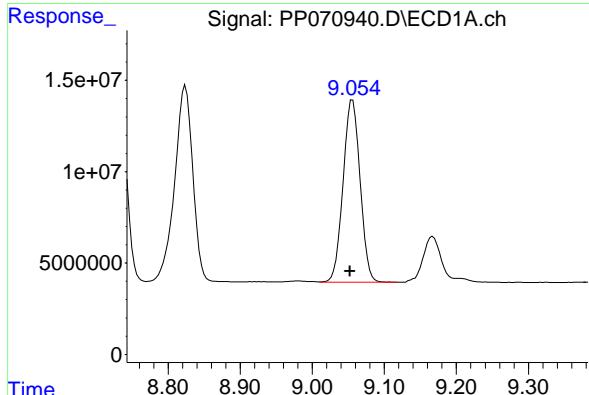


#45 AR-1268-5

R.T.: 9.891 min  
 Delta R.T.: 0.003 min  
 Response: 459553484 ECD\_P  
 Conc: 952.41 ng/ml ClientSampleId :  
 AR1268ICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

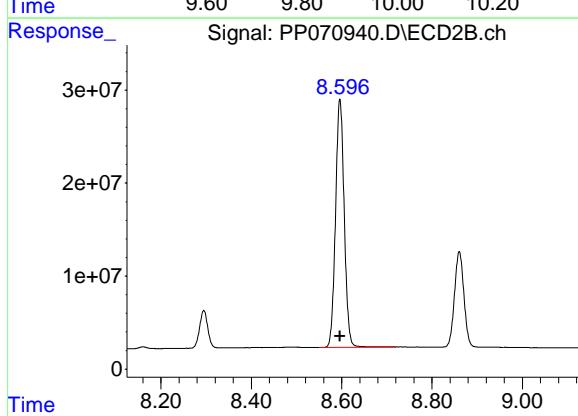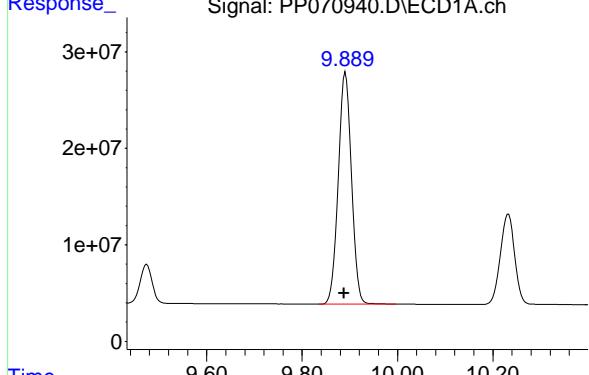

#45 AR-1268-5

R.T.: 8.596 min  
 Delta R.T.: 0.000 min  
 Response: 357060145  
 Conc: 962.56 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070941.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:05  
 Operator : YP\AJ  
 Sample : AR1268ICC750  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
AR1268ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:14 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.514	3.817	119.6E6	83914927	74.397	75.039
2) SA Decachloro...	10.230	8.861	154.1E6	118.4E6	73.551	75.751

**Target Compounds**

41) L9 AR-1268-1	8.730	7.729	178.4E6	131.7E6	744.578	753.609m
42) L9 AR-1268-2	8.823	7.795	149.2E6	110.8E6	745.140	760.189
43) L9 AR-1268-3	9.055	8.000	128.8E6	95630424	740.439	768.788
44) L9 AR-1268-4	9.473	8.294	55249435	40878954	754.389	766.313
45) L9 AR-1268-5	9.890	8.596	361.2E6	282.2E6	748.577	760.668

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070941.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:05  
 Operator : YP\AJ  
 Sample : AR1268ICC750  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1



Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1268ICC750





**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:14 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

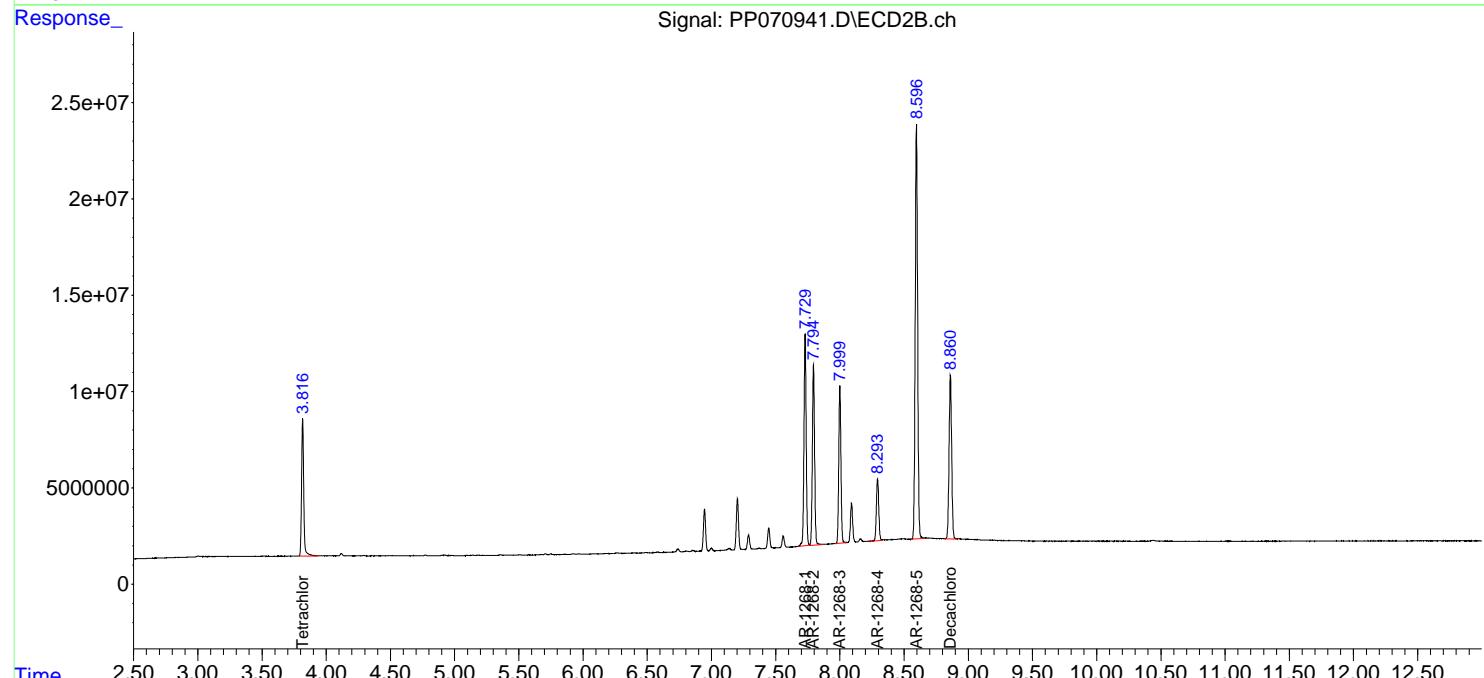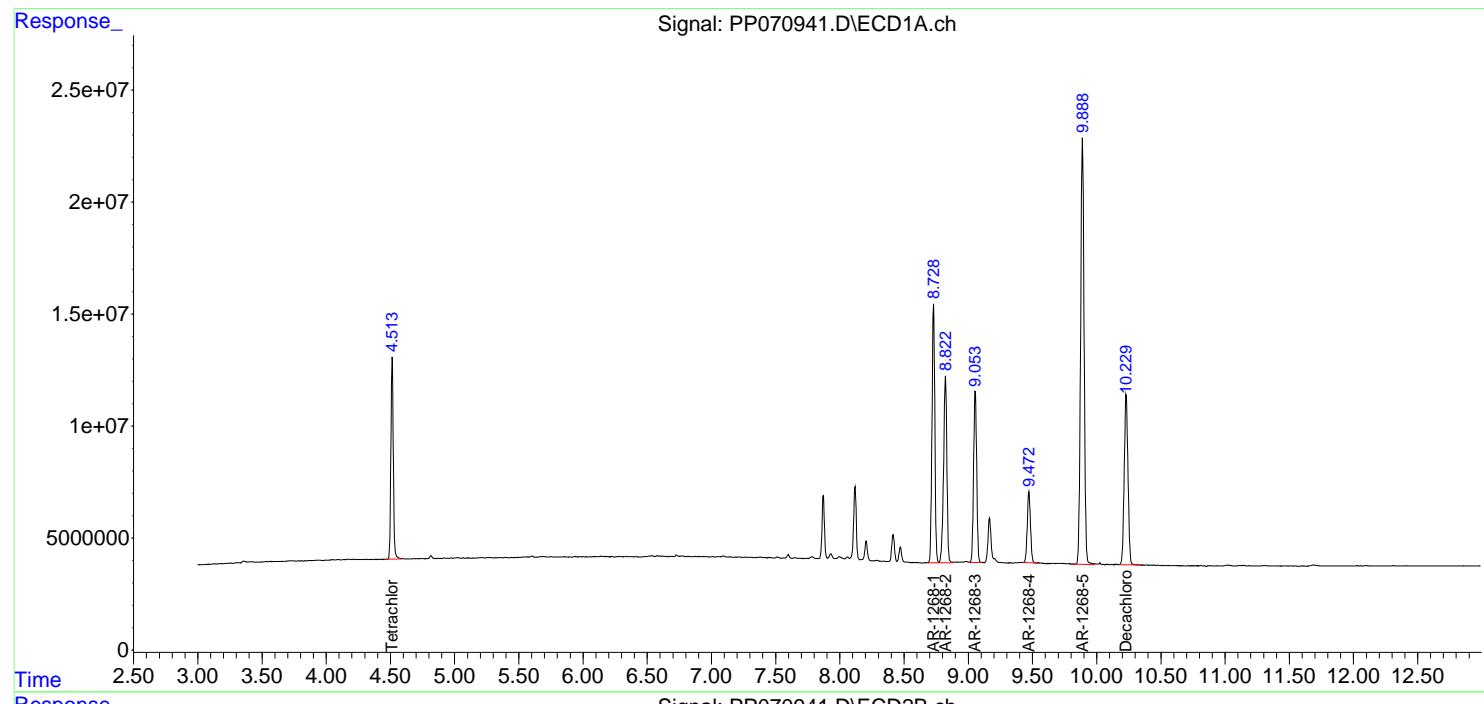

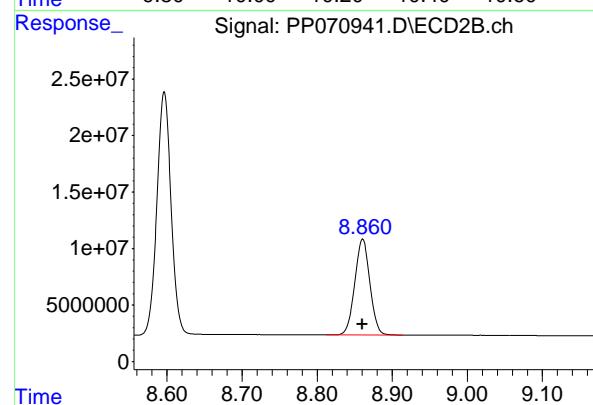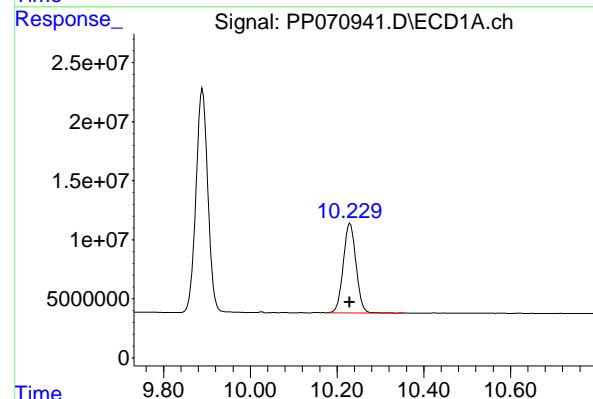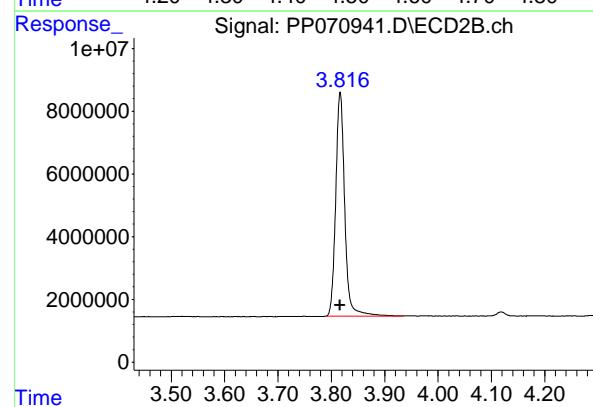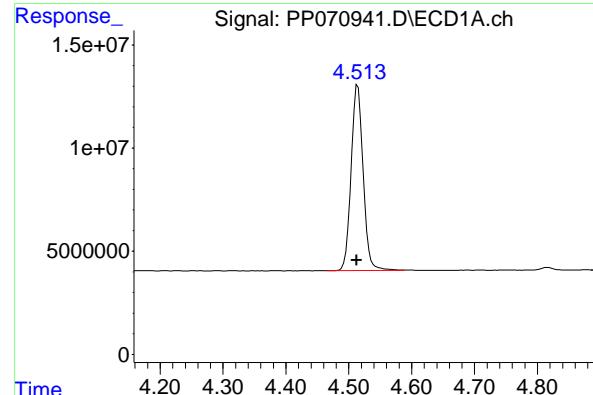

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
 Delta R.T.: 0.001 min  
 Response: 119597931  
 Conc: 74.40 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1268ICC750

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.817 min  
 Delta R.T.: 0.000 min  
 Response: 83914927  
 Conc: 75.04 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.230 min  
 Delta R.T.: 0.000 min  
 Response: 154146813  
 Conc: 73.55 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.861 min  
 Delta R.T.: 0.000 min  
 Response: 118436920  
 Conc: 75.75 ng/ml

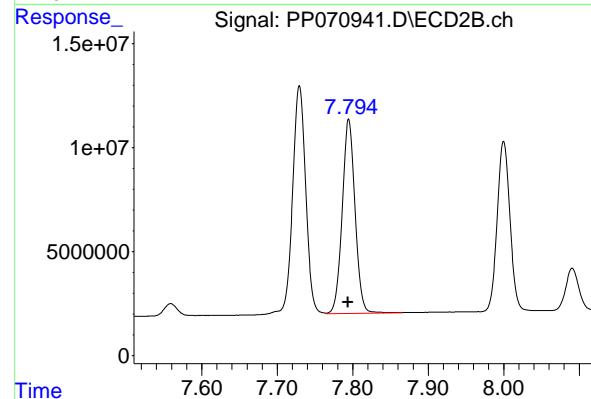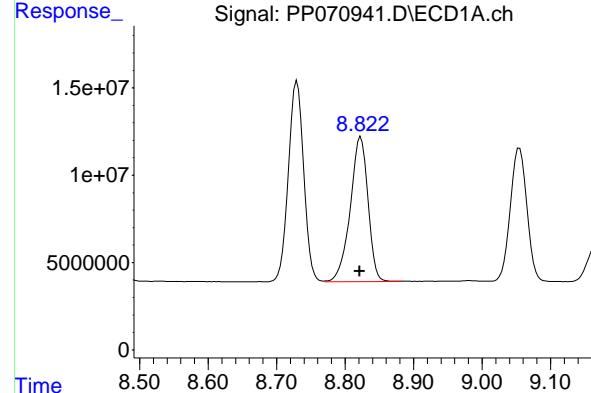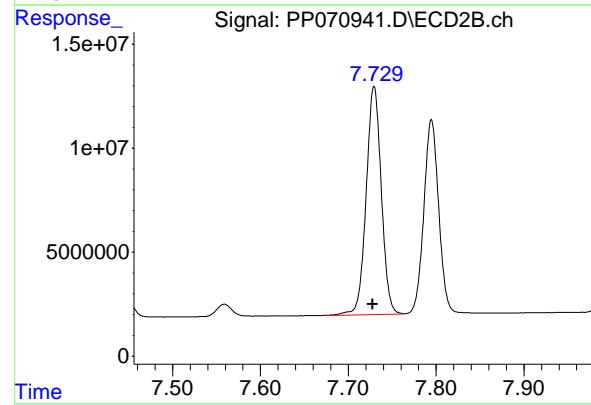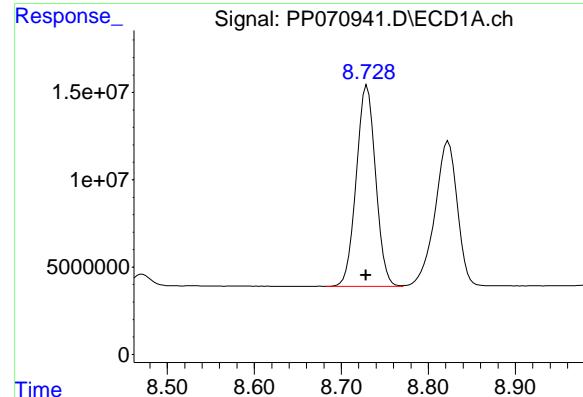

#41 AR-1268-1

R.T.: 8.730 min  
 Delta R.T.: 0.001 min  
 Response: 178445590  
 Conc: 744.58 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1268ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#41 AR-1268-1

R.T.: 7.729 min  
 Delta R.T.: 0.001 min  
 Response: 131656350  
 Conc: 753.61 ng/ml

#42 AR-1268-2

R.T.: 8.823 min  
 Delta R.T.: 0.002 min  
 Response: 149201176  
 Conc: 745.14 ng/ml

#42 AR-1268-2

R.T.: 7.795 min  
 Delta R.T.: 0.001 min  
 Response: 110804324  
 Conc: 760.19 ng/ml

#43 AR-1268-3

R.T.: 9.055 min  
 Delta R.T.: 0.002 min  
 Response: 128803338  
 Conc: 740.44 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId :** AR1268ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#43 AR-1268-3





R.T.: 8.000 min  
 Delta R.T.: 0.000 min  
 Response: 95630424  
 Conc: 768.79 ng/ml

#44 AR-1268-4

R.T.: 9.473 min  
 Delta R.T.: 0.001 min  
 Response: 55249435  
 Conc: 754.39 ng/ml

#44 AR-1268-4

R.T.: 8.294 min  
 Delta R.T.: 0.000 min  
 Response: 40878954  
 Conc: 766.31 ng/ml

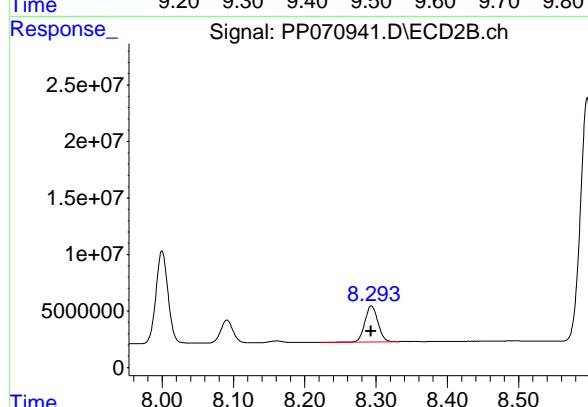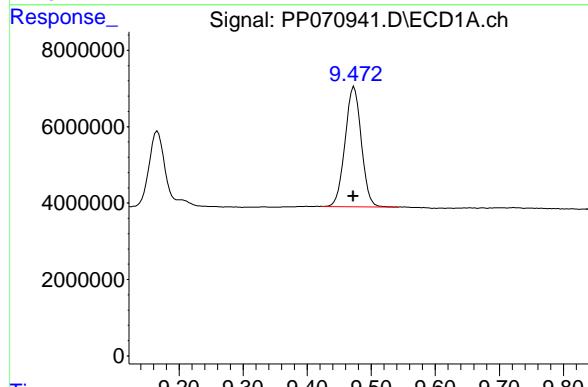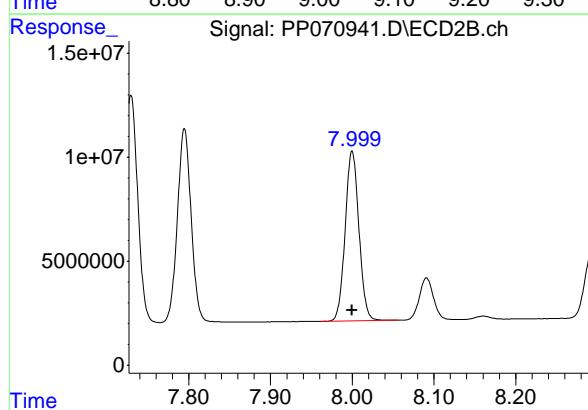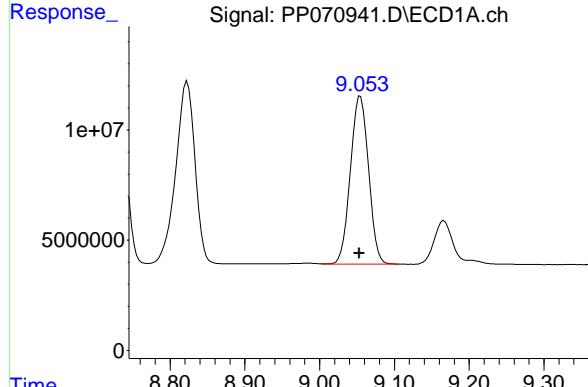

#45 AR-1268-5


R.T.: 9.890 min  
 Delta R.T.: 0.002 min  
 Response: 361198889  
 Conc: 748.58 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId :** AR1268ICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#45 AR-1268-5

R.T.: 8.596 min  
 Delta R.T.: 0.000 min  
 Response: 282169730  
 Conc: 760.67 ng/ml

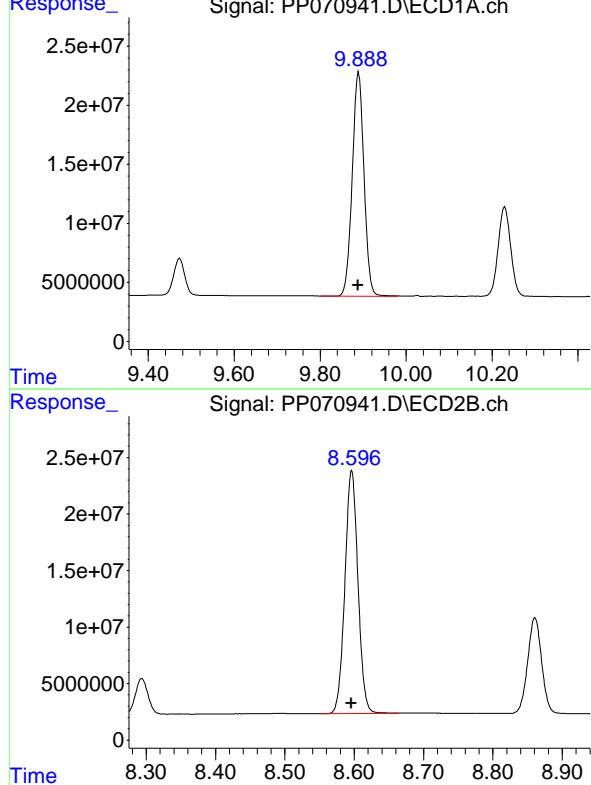

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070942.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:21  
 Operator : YP\AJ  
 Sample : AR1268ICC500  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
AR1268ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	4.513	3.816	80378727	55914176	50.000	50.000
2) SA Decachlor...	10.230	8.860	104.8E6	78175161	50.000	50.000

**Target Compounds**

41) L9 AR-1268-1	8.729	7.728	119.8E6	87376833	500.000	500.150m
42) L9 AR-1268-2	8.821	7.793	100.1E6	72879434	500.000	500.000
43) L9 AR-1268-3	9.053	8.000	86977678	62195601	500.000	500.000
44) L9 AR-1268-4	9.472	8.293	36618642	26672497	500.000	500.000
45) L9 AR-1268-5	9.888	8.596	241.3E6	185.5E6	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070942.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:21  
 Operator : YP\AJ  
 Sample : AR1268ICC500  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1268ICC500

### Manual Integrations APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

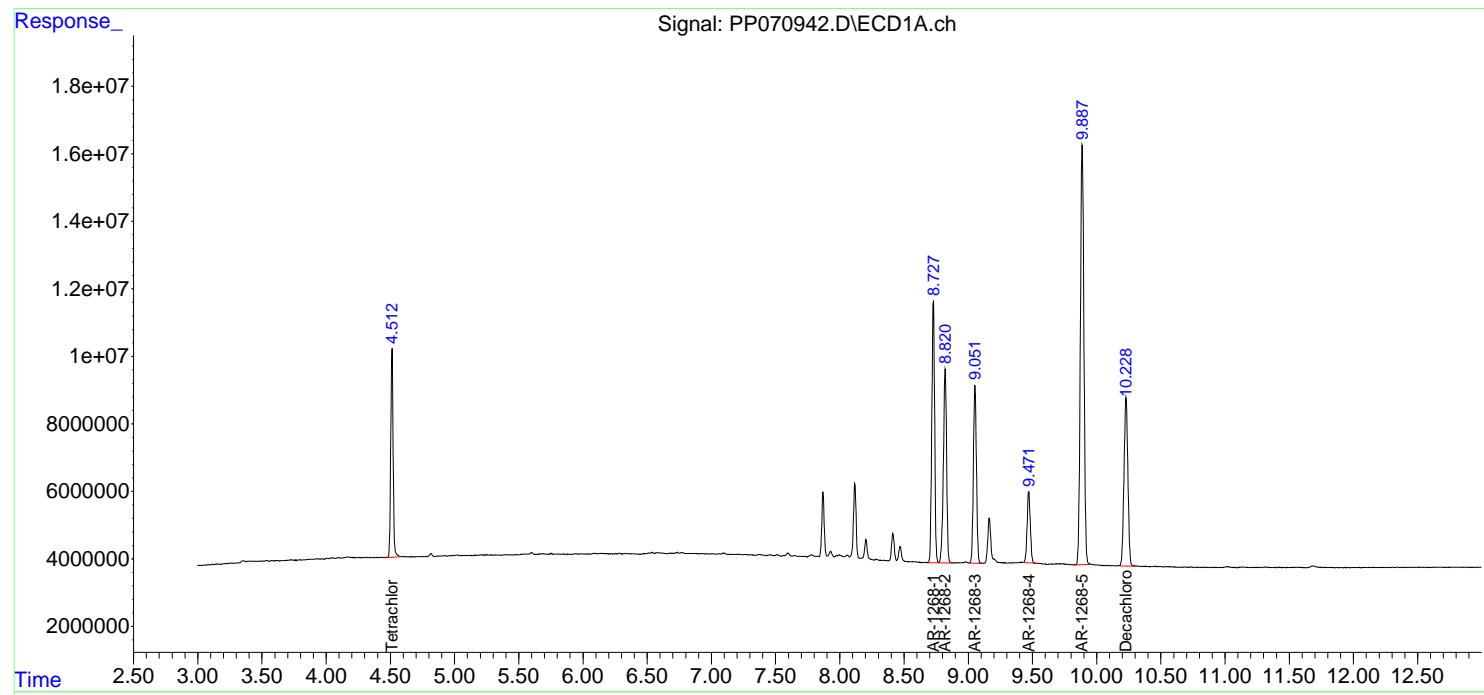

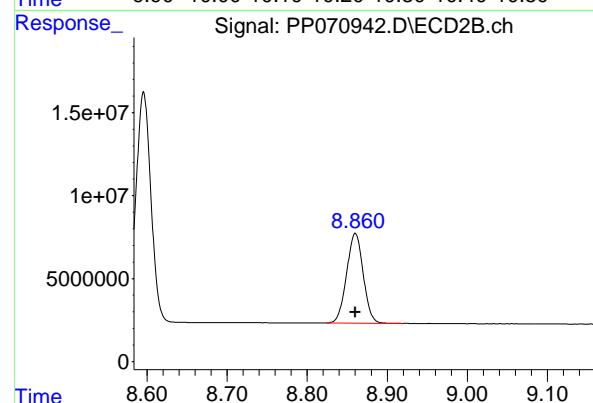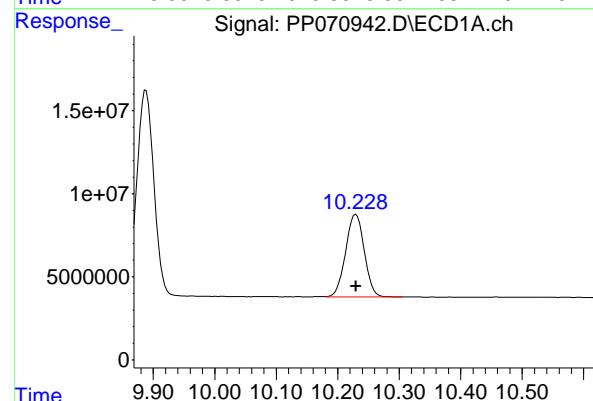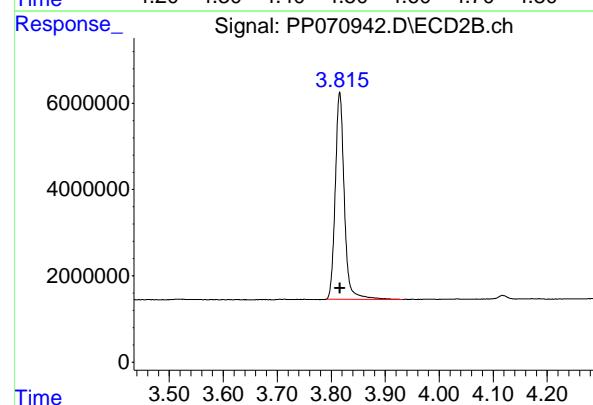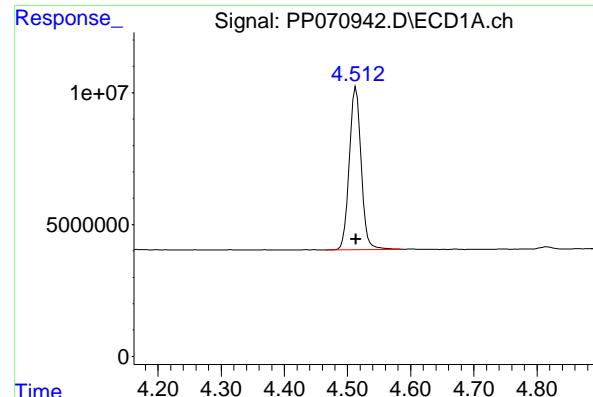

## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
 Delta R.T.: 0.000 min  
 Response: 80378727  
 Conc: 50.00 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1268ICC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 55914176  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.230 min  
 Delta R.T.: 0.000 min  
 Response: 104789095  
 Conc: 50.00 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.860 min  
 Delta R.T.: 0.000 min  
 Response: 78175161  
 Conc: 50.00 ng/ml

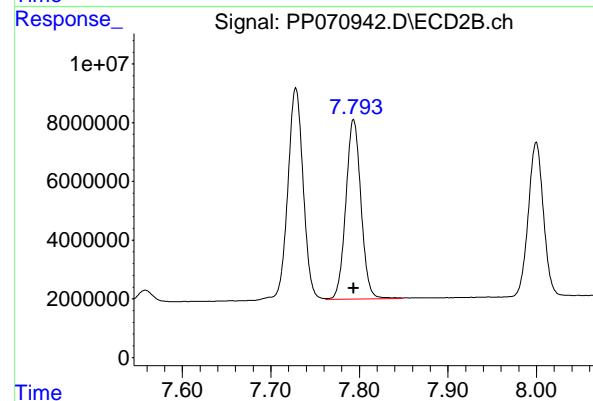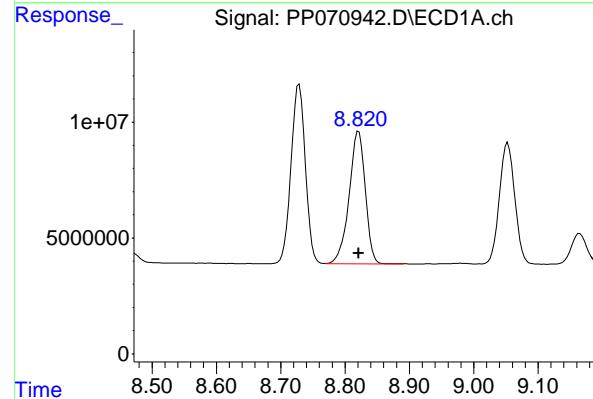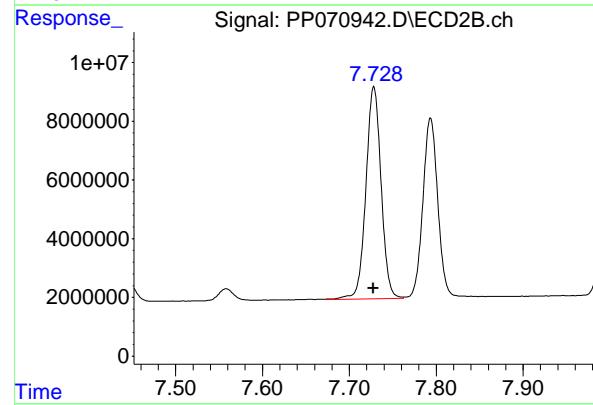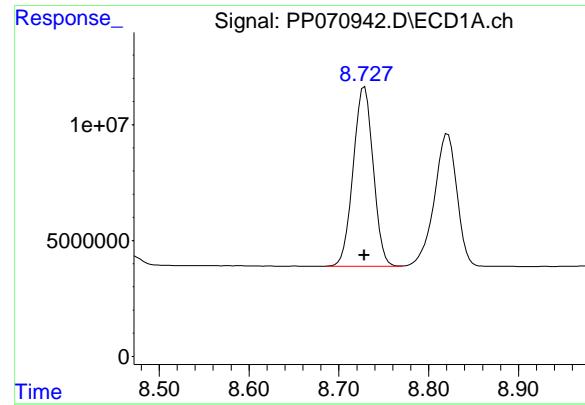

#41 AR-1268-1

R.T.: 8.729 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 119830016  
Conc: 500.00 ng/ml ClientSampleId : AR1268ICC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

#41 AR-1268-1

R.T.: 7.728 min  
Delta R.T.: 0.000 min  
Response: 87376833  
Conc: 500.15 ng/ml

#42 AR-1268-2

R.T.: 8.821 min  
Delta R.T.: 0.000 min  
Response: 100116173  
Conc: 500.00 ng/ml

#42 AR-1268-2

R.T.: 7.793 min  
Delta R.T.: 0.000 min  
Response: 72879434  
Conc: 500.00 ng/ml

#43 AR-1268-3

R.T.: 9.053 min  
 Delta R.T.: 0.000 min  
 Response: 86977678  
 Conc: 500.00 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId :** AR1268ICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#43 AR-1268-3





R.T.: 8.000 min  
 Delta R.T.: 0.000 min  
 Response: 62195601  
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 9.472 min  
 Delta R.T.: 0.000 min  
 Response: 36618642  
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 8.293 min  
 Delta R.T.: 0.000 min  
 Response: 26672497  
 Conc: 500.00 ng/ml

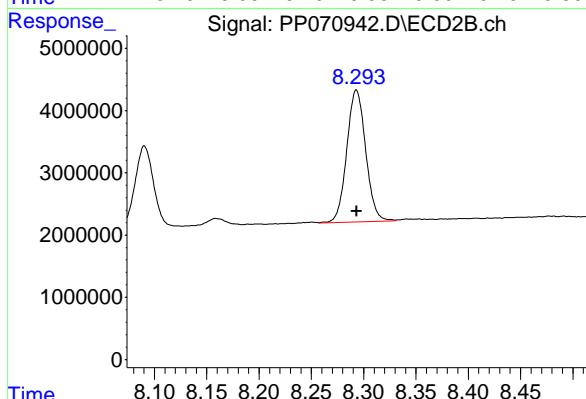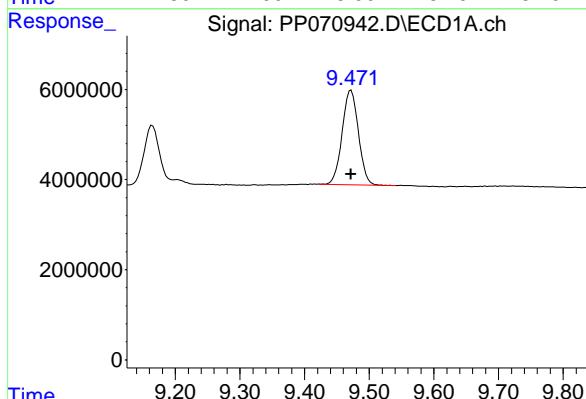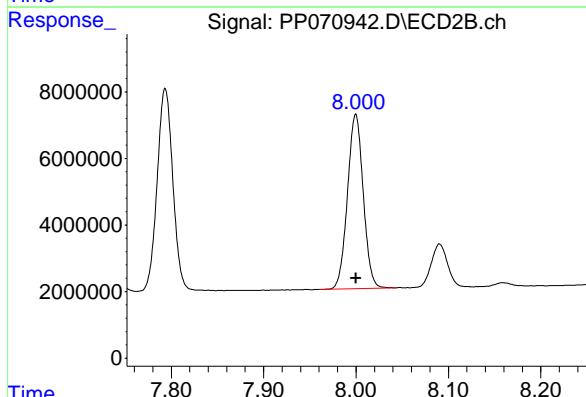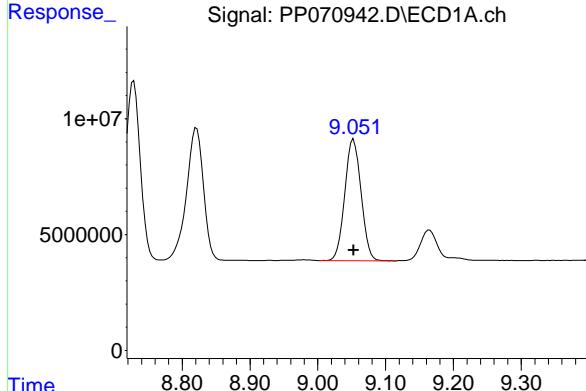

#45 AR-1268-5



R.T.: 9.888 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 241257148  
Conc: 500.00 ng/ml  
ClientSampleId: AR1268ICC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
Supervised By :mohammad ahmed 03/31/2025

#45 AR-1268-5

R.T.: 8.596 min  
Delta R.T.: 0.000 min  
Response: 185474929  
Conc: 500.00 ng/ml

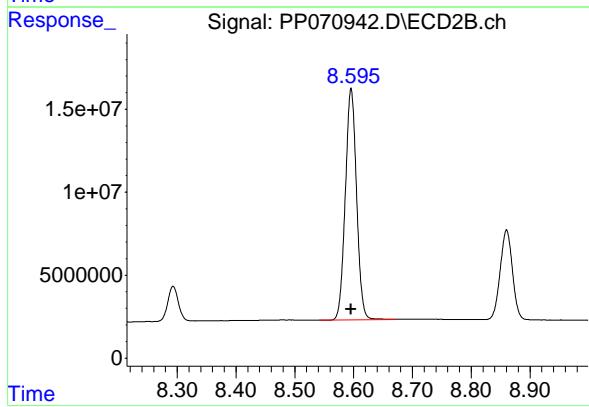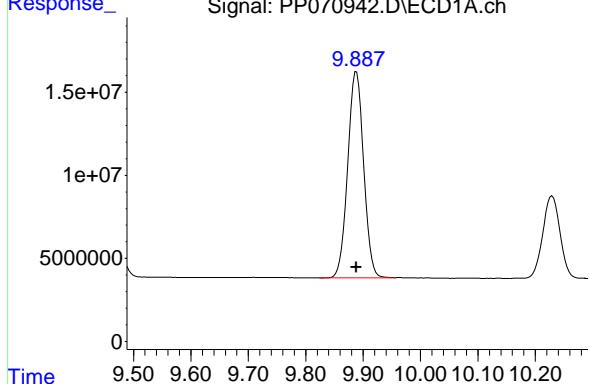

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070943.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:37  
 Operator : YP\AJ  
 Sample : AR1268ICC250  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC250**

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.515	3.817	41125313	29588552	25.582	26.459
2) SA Decachloro...	10.232	8.859	54285349	40518249	25.902	25.915

**Target Compounds**

41) L9 AR-1268-1	8.730	7.729	61973048	44233672	258.587	253.196m
42) L9 AR-1268-2	8.824	7.794	51237231	36694564	255.889	251.748
43) L9 AR-1268-3	9.055	8.000	44311644	31811936	254.730	255.741
44) L9 AR-1268-4	9.473	8.295	18700738	13922493	255.345	260.990
45) L9 AR-1268-5	9.890	8.596	124.6E6	91636186	258.260	247.031

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070943.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:37  
 Operator : YP\AJ  
 Sample : AR1268ICC250  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1


Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1268ICC250





**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

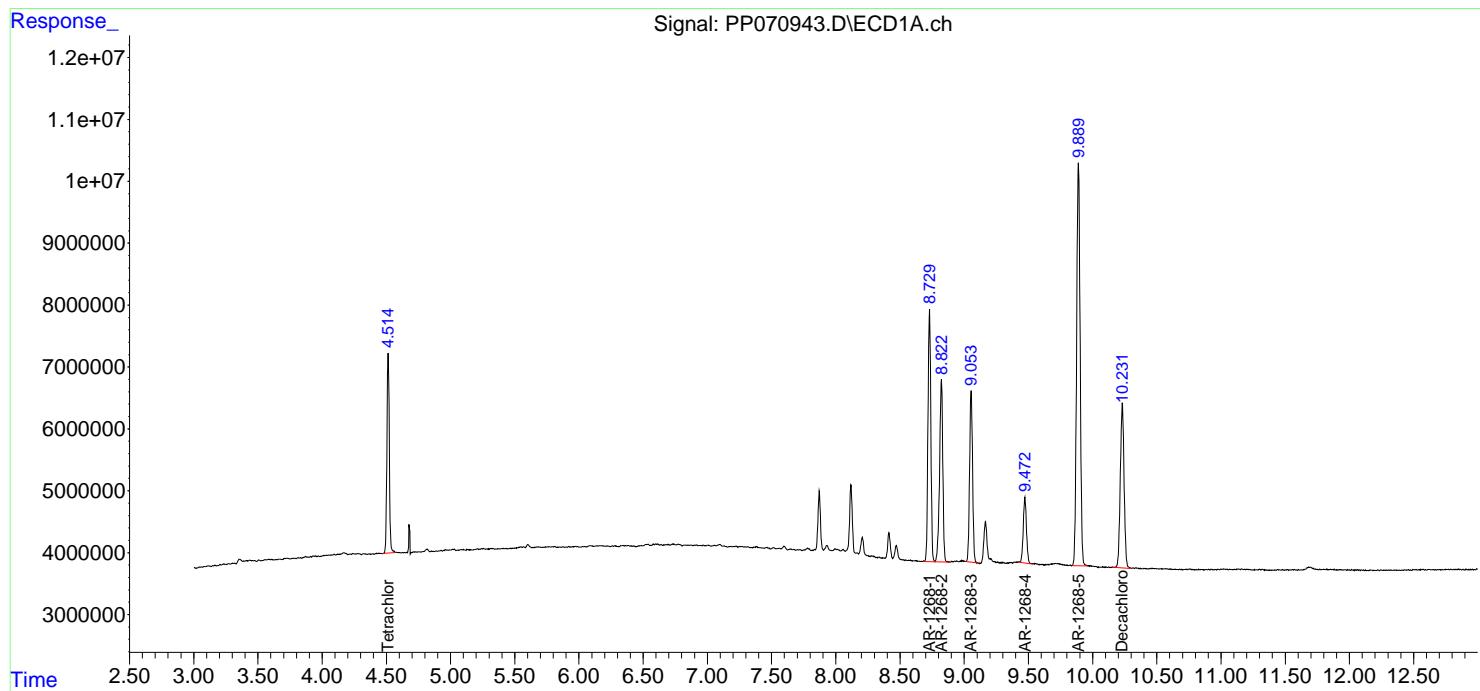

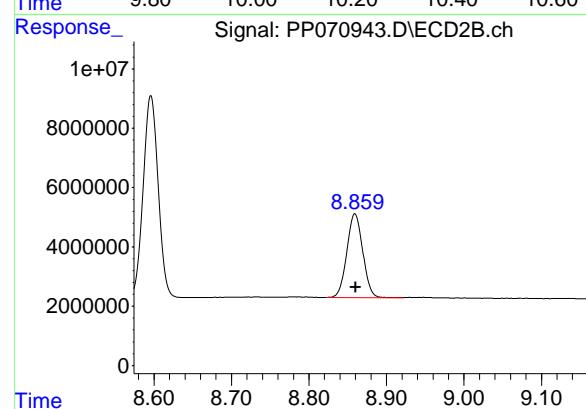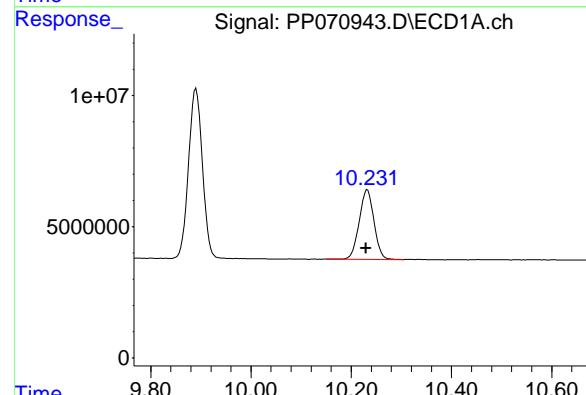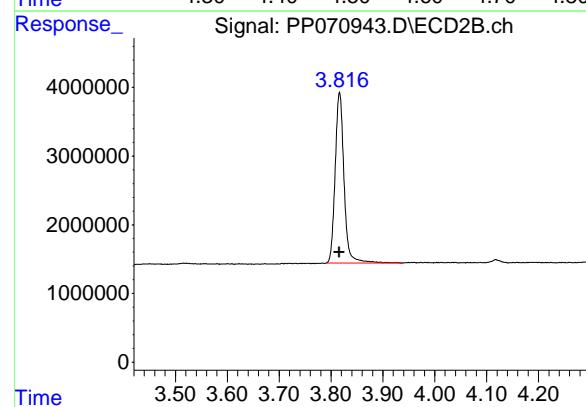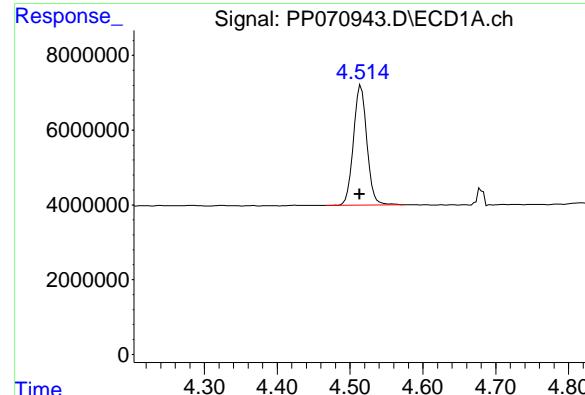

## #1 Tetrachloro-m-xylene

R.T.: 4.515 min  
 Delta R.T.: 0.002 min  
 Response: 41125313 ECD\_P  
 Conc: 25.58 ng/ml ClientSampleId : AR1268ICC250

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene



R.T.: 3.817 min  
 Delta R.T.: 0.000 min  
 Response: 29588552  
 Conc: 26.46 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.232 min  
 Delta R.T.: 0.003 min  
 Response: 54285349  
 Conc: 25.90 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 40518249  
 Conc: 25.92 ng/ml

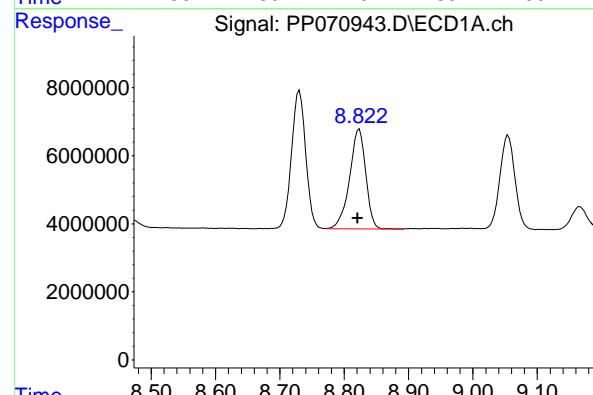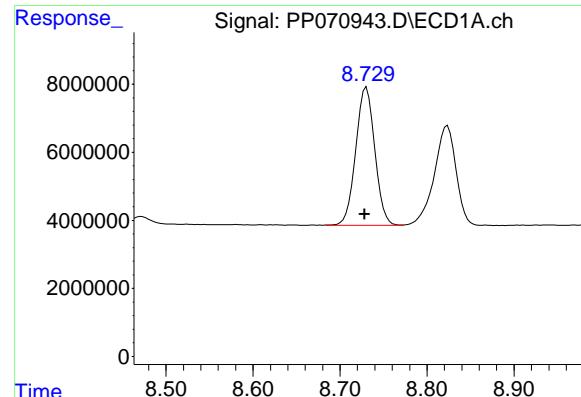

#41 AR-1268-1

R.T.: 8.730 min  
 Delta R.T.: 0.002 min  
 Response: 61973048  
 Conc: 258.59 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1268ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#41 AR-1268-1





R.T.: 7.729 min  
 Delta R.T.: 0.000 min  
 Response: 44233672  
 Conc: 253.20 ng/ml

#42 AR-1268-2

R.T.: 8.824 min  
 Delta R.T.: 0.002 min  
 Response: 51237231  
 Conc: 255.89 ng/ml

#42 AR-1268-2

R.T.: 7.794 min  
 Delta R.T.: 0.000 min  
 Response: 36694564  
 Conc: 251.75 ng/ml

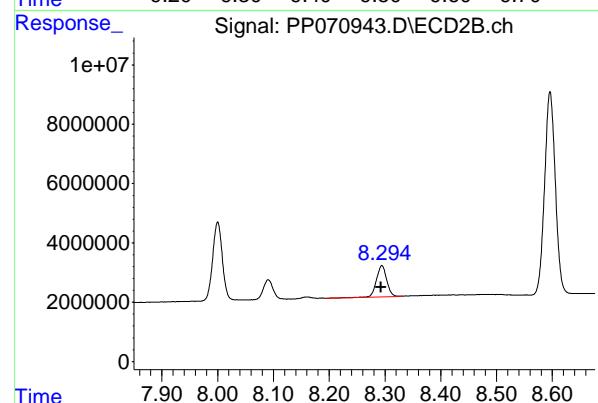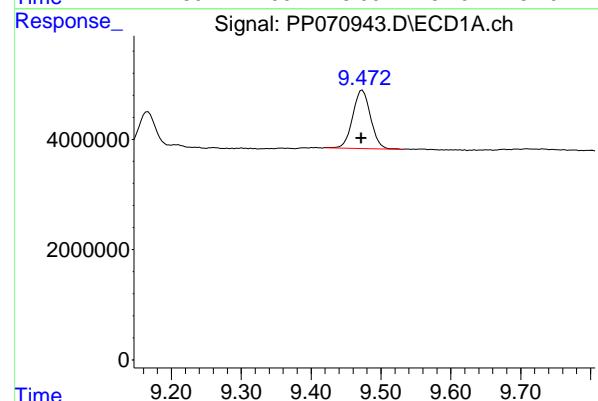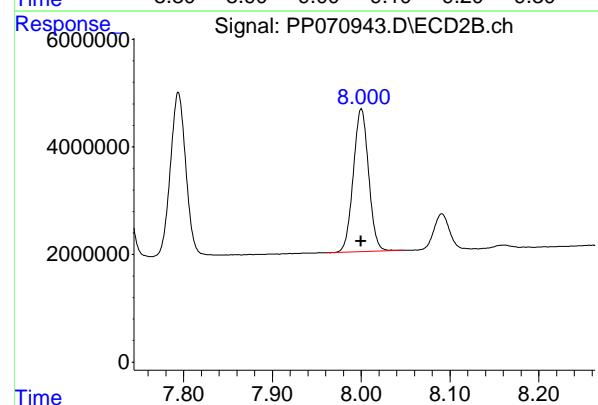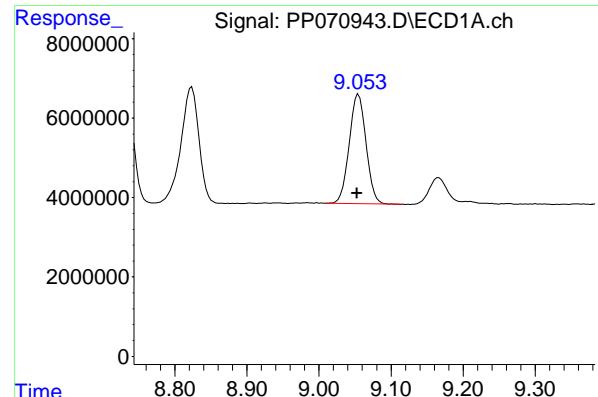

#43 AR-1268-3

R.T.: 9.055 min  
 Delta R.T.: 0.002 min  
 Instrument: ECD\_P  
 Response: 44311644  
 Conc: 254.73 ng/ml  
 ClientSampleId : AR1268ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#43 AR-1268-3

R.T.: 8.000 min  
 Delta R.T.: 0.000 min  
 Response: 31811936  
 Conc: 255.74 ng/ml

#44 AR-1268-4

R.T.: 9.473 min  
 Delta R.T.: 0.002 min  
 Response: 18700738  
 Conc: 255.34 ng/ml

#44 AR-1268-4

R.T.: 8.295 min  
 Delta R.T.: 0.002 min  
 Response: 13922493  
 Conc: 260.99 ng/ml

#45 AR-1268-5


R.T.: 9.890 min  
 Delta R.T.: 0.002 min  
 Response: 124614186  
 Conc: 258.26 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId :** AR1268ICC250

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#45 AR-1268-5

R.T.: 8.596 min  
 Delta R.T.: 0.000 min  
 Response: 91636186  
 Conc: 247.03 ng/ml

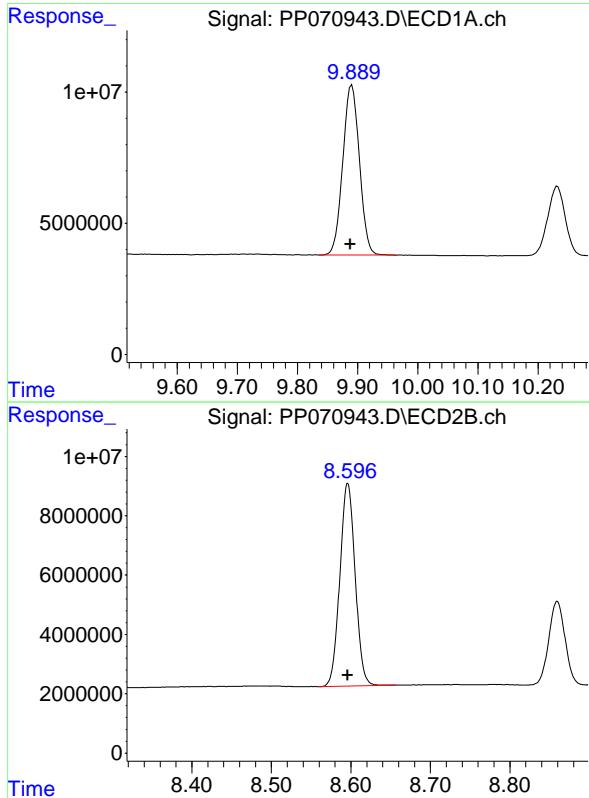

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070944.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:53  
 Operator : YP\AJ  
 Sample : AR1268ICC050  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC050**

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 18:13:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.514	3.816	7200607	6304440	4.457m	5.529
2) SA Decachloro...	10.230	8.859	10035177	7161586	4.762	4.510

**Target Compounds**

41) L9 AR-1268-1	8.729	7.728	11274140	8221191	46.621	46.780m
42) L9 AR-1268-2	8.822	7.794	9103995	6916833	45.210	47.131
43) L9 AR-1268-3	9.054	7.999	8398993	5823381	48.183	46.078
44) L9 AR-1268-4	9.471	8.293	3082639	2471433	41.712	45.336m
45) L9 AR-1268-5	9.889	8.596	22937830	16928167	47.050	45.599

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070944.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:53  
 Operator : YP\AJ  
 Sample : AR1268ICC050  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1


**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC050**





**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 18:13:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

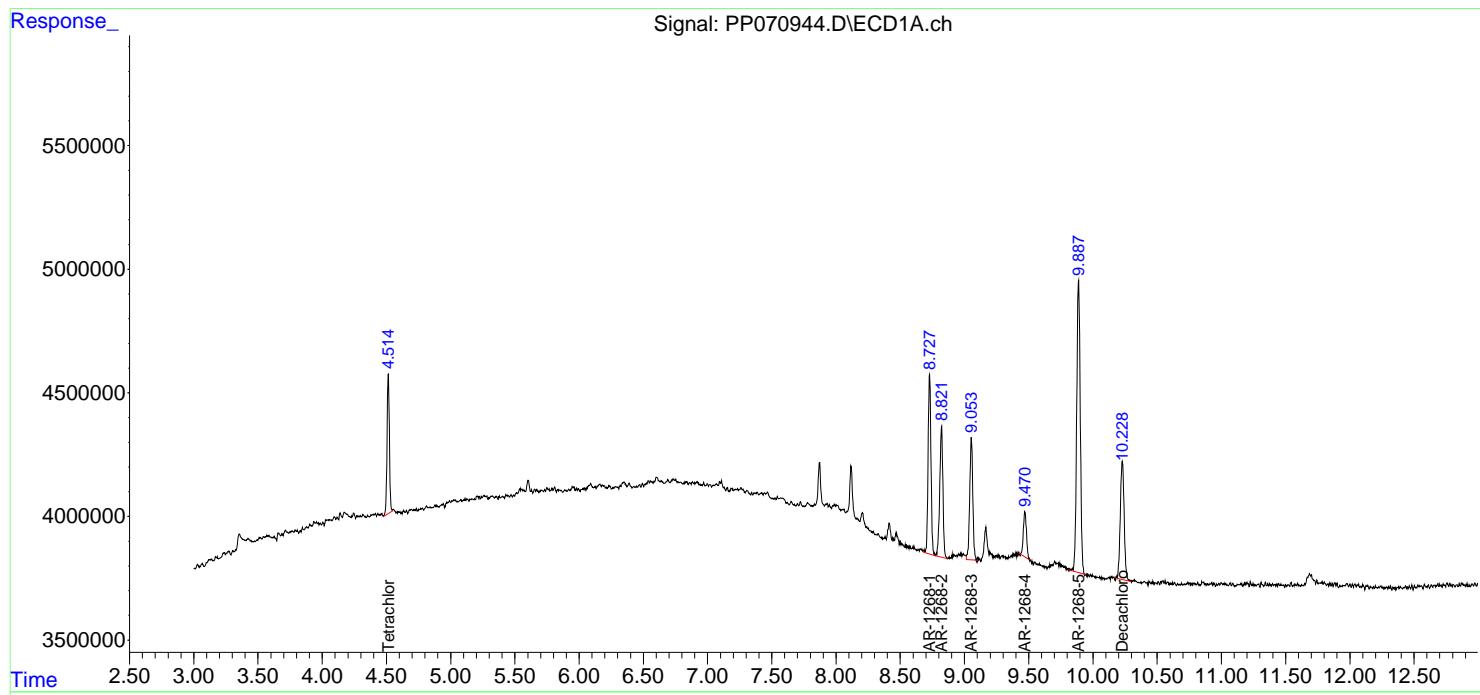

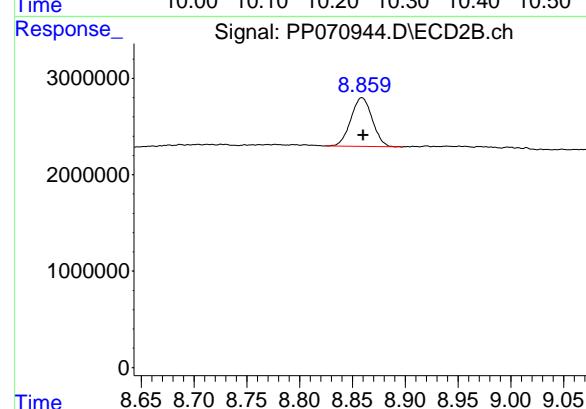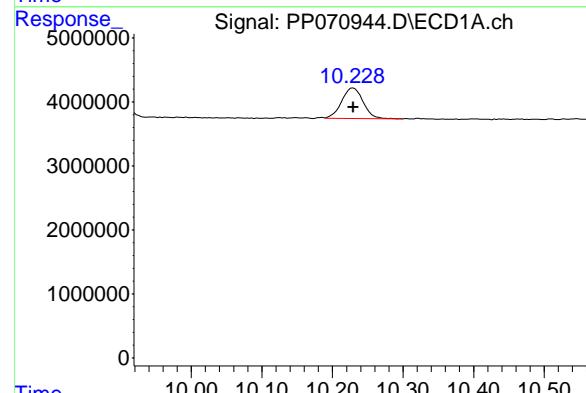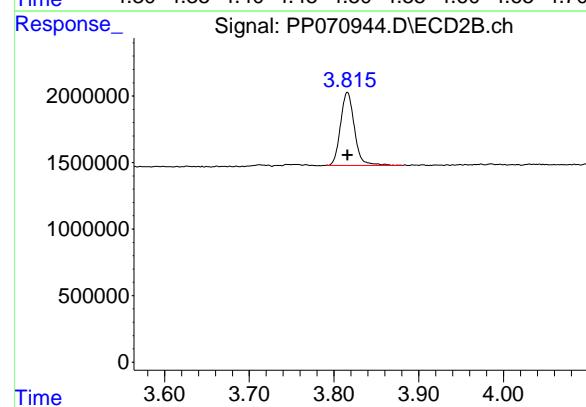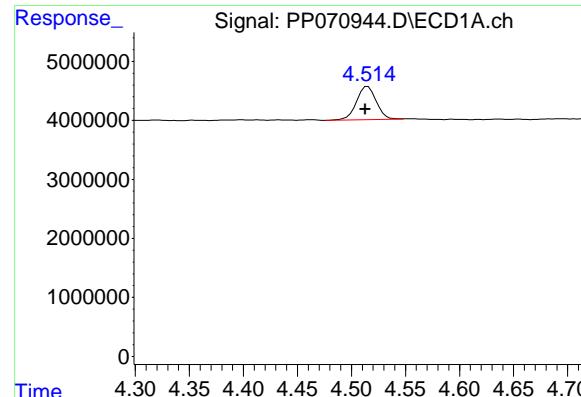

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
 Delta R.T.: 0.000 min  
 Response: 7200607  
 Conc: 4.46 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1268ICC050

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 6304440  
 Conc: 5.53 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.230 min  
 Delta R.T.: 0.000 min  
 Response: 10035177  
 Conc: 4.76 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: -0.001 min  
 Response: 7161586  
 Conc: 4.51 ng/ml

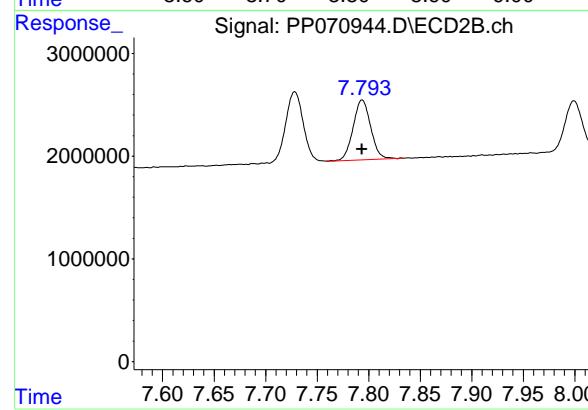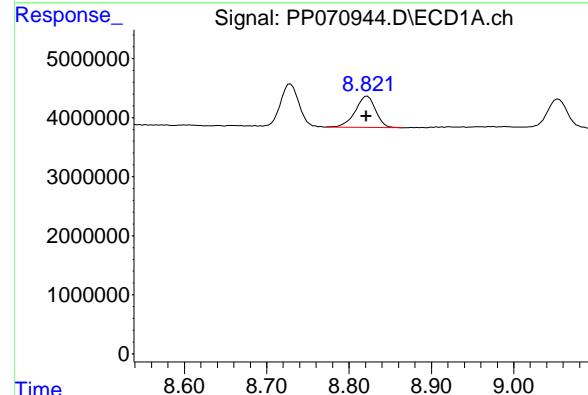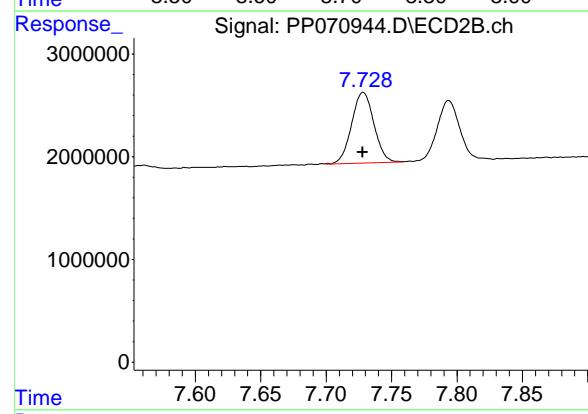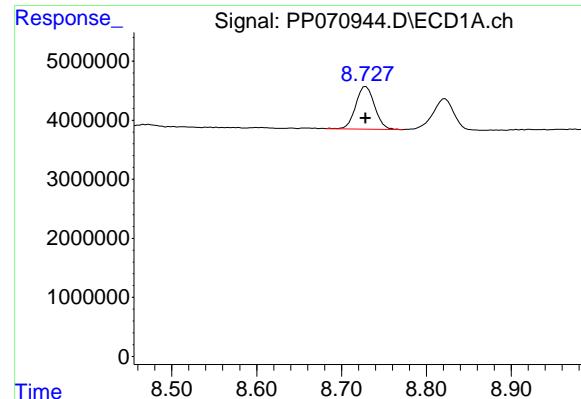

#41 AR-1268-1

R.T.: 8.729 min  
 Delta R.T.: 0.000 min  
 Response: 11274140 ECD\_P  
 Conc: 46.62 ng/ml ClientSampleId : AR1268ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#41 AR-1268-1


R.T.: 7.728 min  
 Delta R.T.: 0.000 min  
 Response: 8221191  
 Conc: 46.78 ng/ml

#42 AR-1268-2

R.T.: 8.822 min  
 Delta R.T.: 0.000 min  
 Response: 9103995  
 Conc: 45.21 ng/ml

#42 AR-1268-2

R.T.: 7.794 min  
 Delta R.T.: 0.000 min  
 Response: 6916833  
 Conc: 47.13 ng/ml

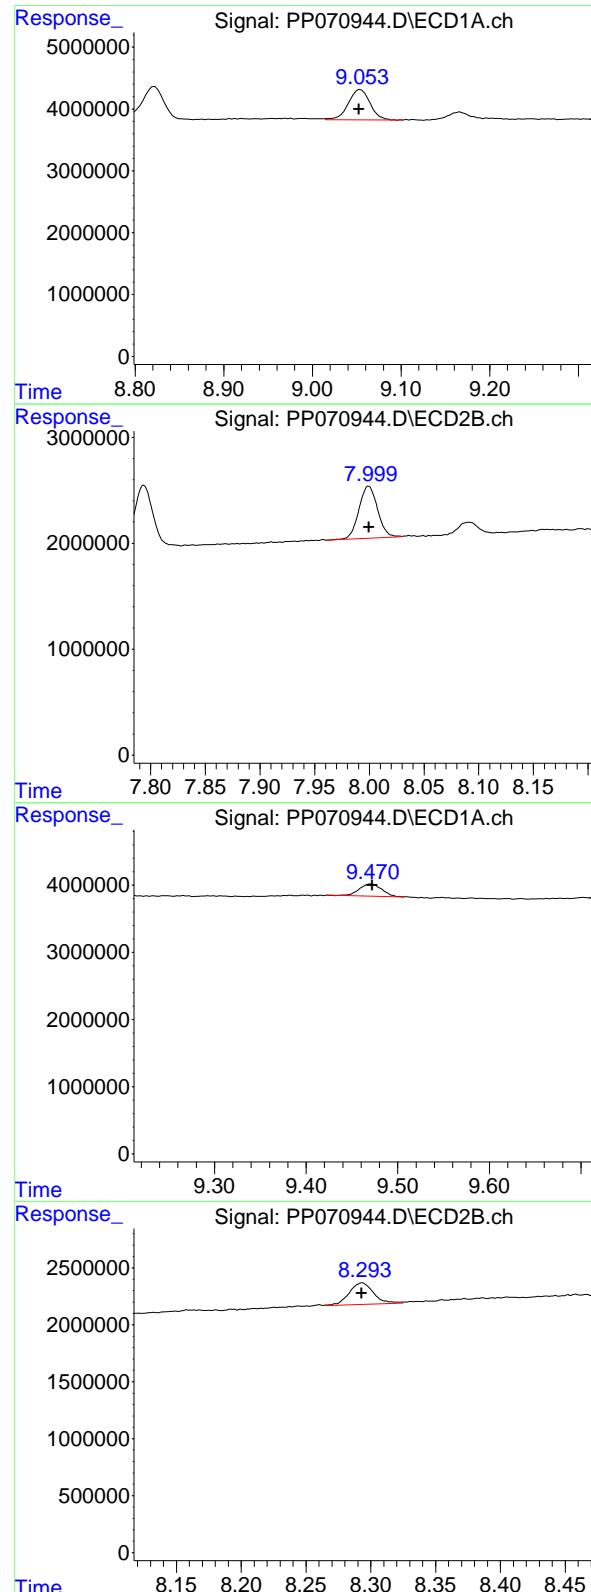

#43 AR-1268-3

R.T.: 9.054 min  
 Delta R.T.: 0.002 min  
 Response: 8398993  
 Conc: 48.18 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1268ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#43 AR-1268-3

R.T.: 7.999 min  
 Delta R.T.: 0.000 min  
 Response: 5823381  
 Conc: 46.08 ng/ml

#44 AR-1268-4

R.T.: 9.471 min  
 Delta R.T.: 0.000 min  
 Response: 3082639  
 Conc: 41.71 ng/ml

#44 AR-1268-4



R.T.: 8.293 min  
 Delta R.T.: 0.000 min  
 Response: 2471433  
 Conc: 45.34 ng/ml

#45 AR-1268-5

R.T.: 9.889 min  
 Delta R.T.: 0.000 min  
 Response: 22937830 ECD\_P  
 Conc: 47.05 ng/ml ClientSampleId :  
 AR1268ICC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

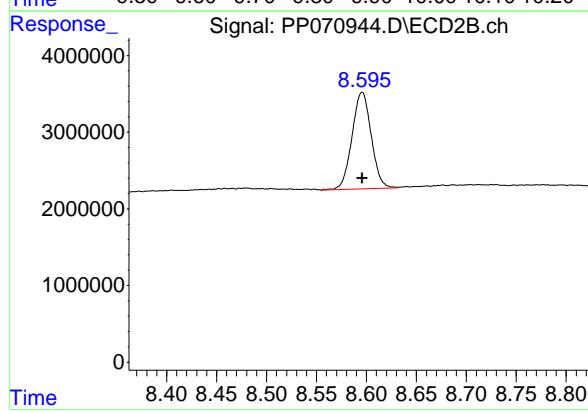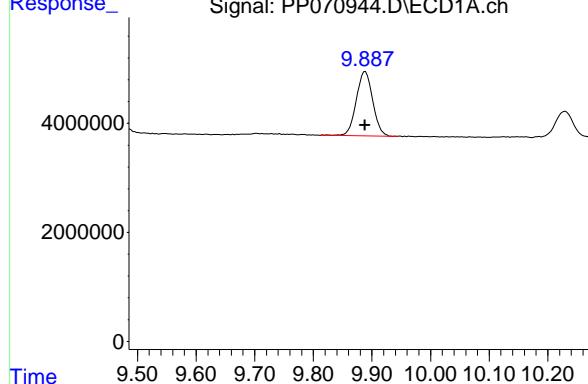

#45 AR-1268-5

R.T.: 8.596 min  
 Delta R.T.: 0.000 min  
 Response: 16928167  
 Conc: 45.60 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070945.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 18:26  
 Operator : YP\AJ  
 Sample : PP032725ICV500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 18:44:38 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 18:19:30 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	4.513	3.817	83053328	55050464	56.825	53.105
2) SA Decachlor...	10.229	8.860	60452615	44643396	57.431	56.640

**Target Compounds**

3) L1 AR-1016-1	5.666	4.904	27342824	21140954	537.702	527.361
4) L1 AR-1016-2	5.688	4.923	41229999	30414011	528.227	525.602
5) L1 AR-1016-3	5.750	5.100	25160452	16688586	533.347	539.677
6) L1 AR-1016-4	5.847	5.141	20613627	13786307	560.828	566.035
7) L1 AR-1016-5	6.140	5.356	19310102	17090774	569.416	528.779
31) L7 AR-1260-1	7.259	6.392	37489891	28161151	558.277	549.955
32) L7 AR-1260-2	7.512	6.580	54825330	35718929	570.287	559.912
33) L7 AR-1260-3	7.871	6.734	45118892	30750809	564.563	564.371
34) L7 AR-1260-4	8.095	7.206	41972897	25791995	533.078	539.285
35) L7 AR-1260-5	8.414	7.447	87345749	64063663	549.738	514.525



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070945.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 18:26  
 Operator : YP\AJ  
 Sample : PP032725ICV500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 ICVPP032725

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 18:44:38 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 18:19:30 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

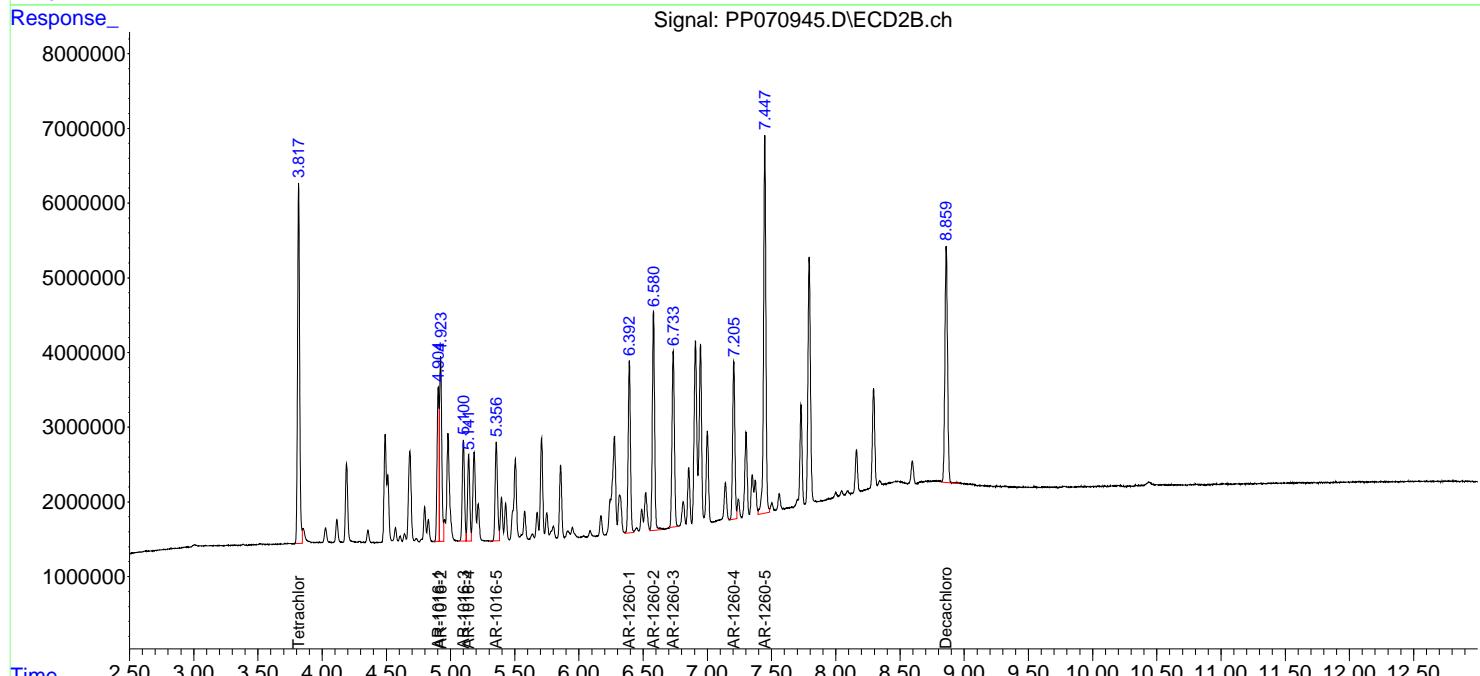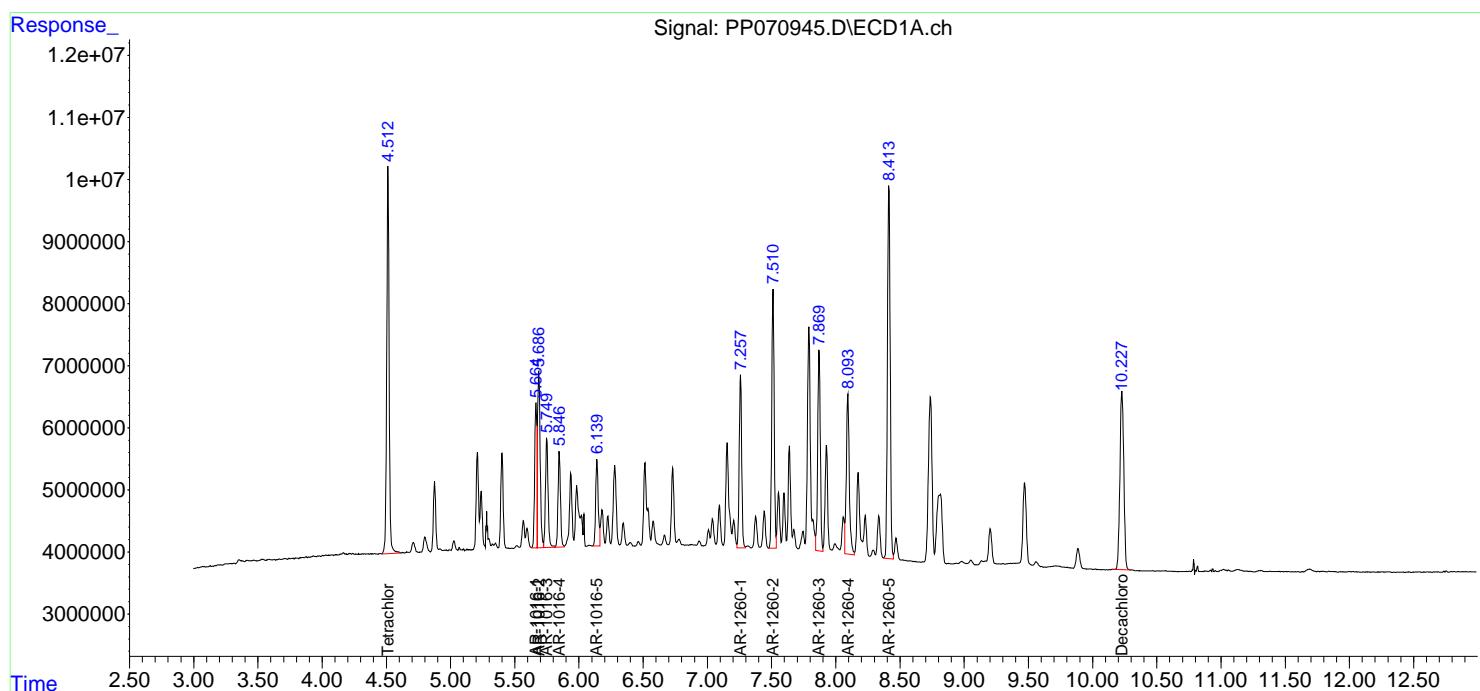

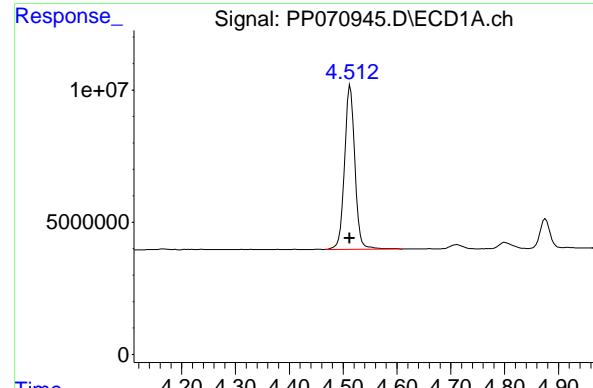


## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
Delta R.T.: 0.001 min  
Instrument: ECD\_P  
Response: 83053328  
Conc: 56.82 ng/ml  
ClientSampleId : ICVPP032725

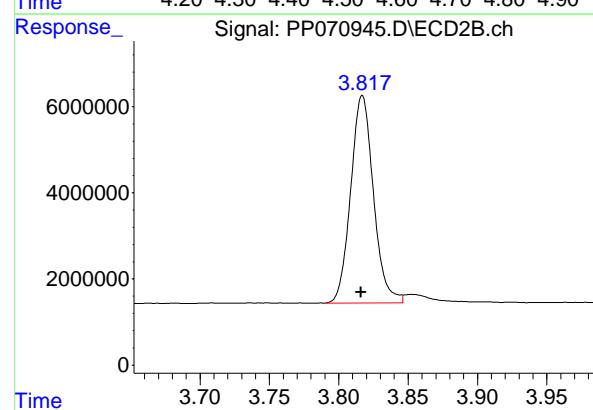


## #1 Tetrachloro-m-xylene

R.T.: 3.817 min  
Delta R.T.: 0.000 min  
Response: 55050464  
Conc: 53.10 ng/ml

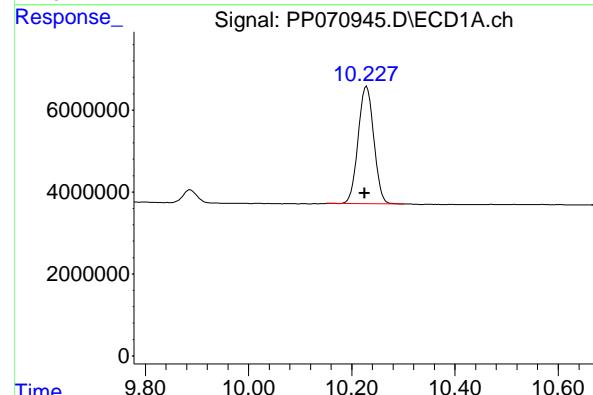

## #2 Decachlorobiphenyl

R.T.: 10.229 min  
Delta R.T.: 0.003 min  
Response: 60452615  
Conc: 57.43 ng/ml

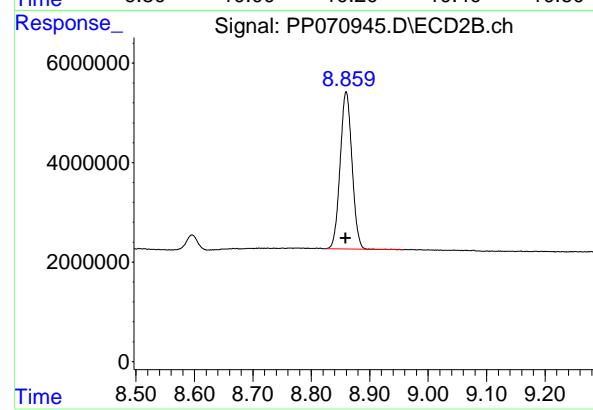


## #2 Decachlorobiphenyl

R.T.: 8.860 min  
Delta R.T.: 0.000 min  
Response: 44643396  
Conc: 56.64 ng/ml


#3 AR-1016-1

R.T.: 5.666 min  
 Delta R.T.: 0.002 min  
 Response: 27342824 ECD\_P  
 Conc: 537.70 ng/ml ClientSampleId :  
 ICVPP032725

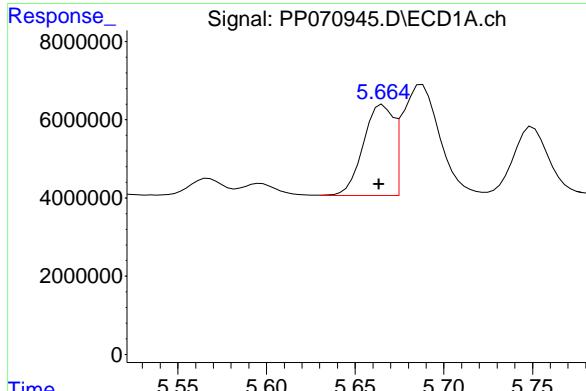


#3 AR-1016-1

R.T.: 4.904 min  
 Delta R.T.: 0.001 min  
 Response: 21140954  
 Conc: 527.36 ng/ml

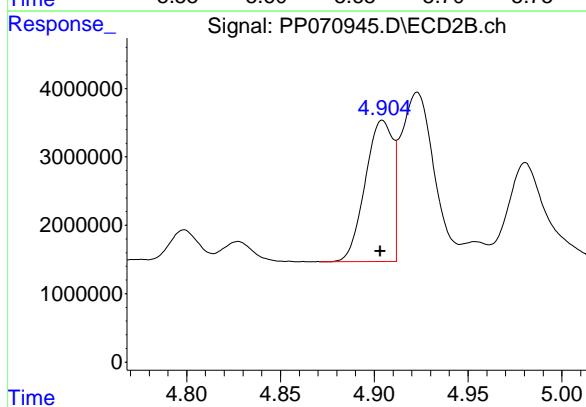


#4 AR-1016-2





R.T.: 5.688 min  
 Delta R.T.: 0.003 min  
 Response: 41229999  
 Conc: 528.23 ng/ml

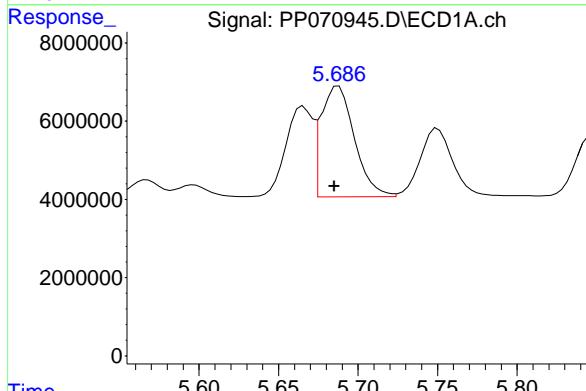

#4 AR-1016-2

R.T.: 4.923 min  
 Delta R.T.: 0.001 min  
 Response: 30414011  
 Conc: 525.60 ng/ml

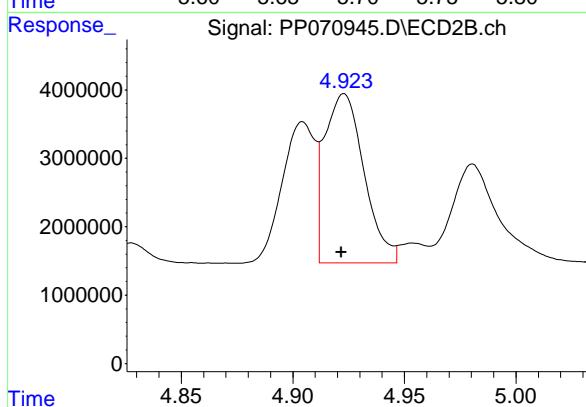

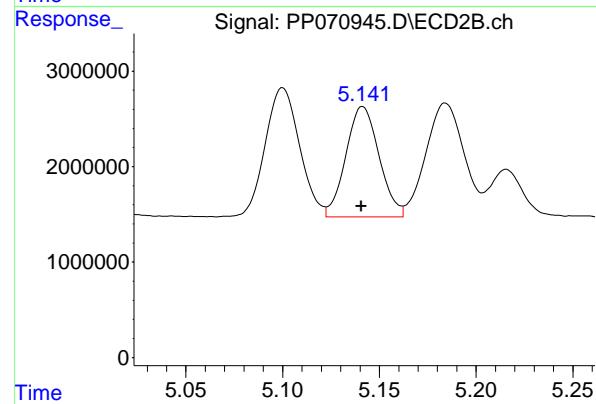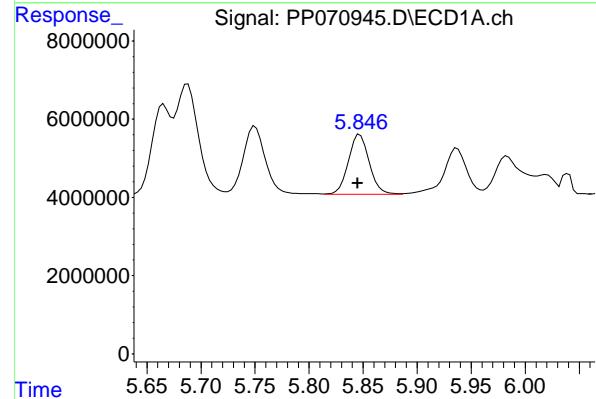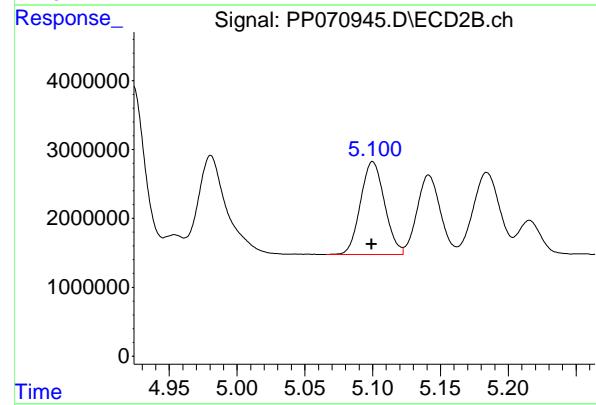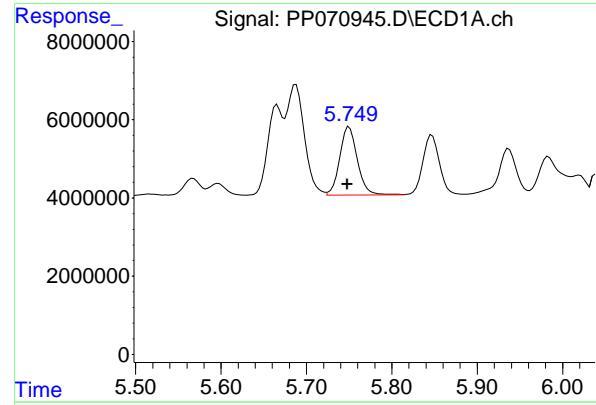

#5 AR-1016-3

R.T.: 5.750 min  
 Delta R.T.: 0.003 min  
 Instrument: ECD\_P  
 Response: 25160452  
 Conc: 533.35 ng/ml  
 ClientSampleId: ICVPP032725

#5 AR-1016-3

R.T.: 5.100 min  
 Delta R.T.: 0.000 min  
 Response: 16688586  
 Conc: 539.68 ng/ml

#6 AR-1016-4


R.T.: 5.847 min  
 Delta R.T.: 0.002 min  
 Response: 20613627  
 Conc: 560.83 ng/ml

#6 AR-1016-4

R.T.: 5.141 min  
 Delta R.T.: 0.000 min  
 Response: 13786307  
 Conc: 566.04 ng/ml


#7 AR-1016-5

R.T.: 6.140 min  
 Delta R.T.: 0.002 min  
 Response: 19310102 Instrument:  
 Conc: 569.42 ng/ml ClientSampleId :  
 ICVPP032725

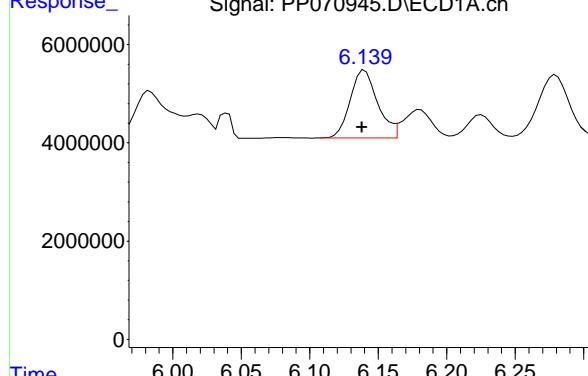


#7 AR-1016-5

R.T.: 5.356 min  
 Delta R.T.: 0.000 min  
 Response: 17090774  
 Conc: 528.78 ng/ml

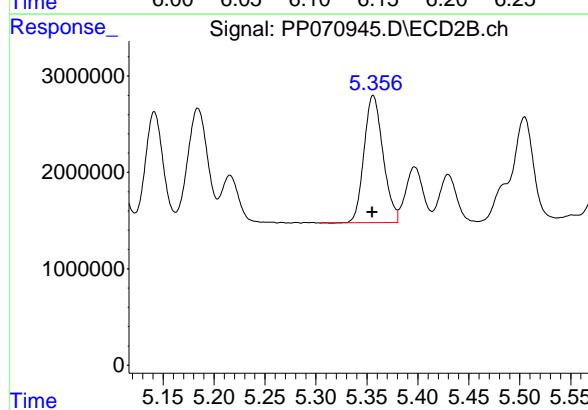


#31 AR-1260-1


R.T.: 7.259 min  
 Delta R.T.: 0.003 min  
 Response: 37489891  
 Conc: 558.28 ng/ml

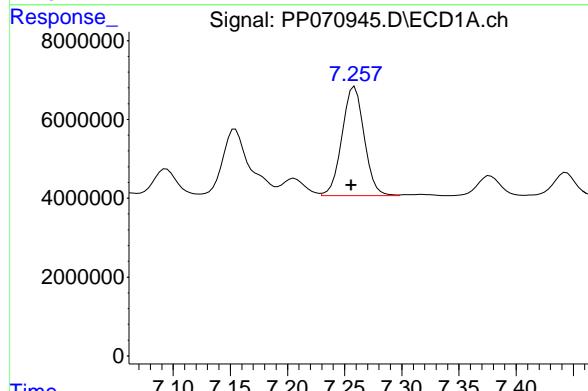

#31 AR-1260-1

R.T.: 6.392 min  
 Delta R.T.: 0.000 min  
 Response: 28161151  
 Conc: 549.95 ng/ml

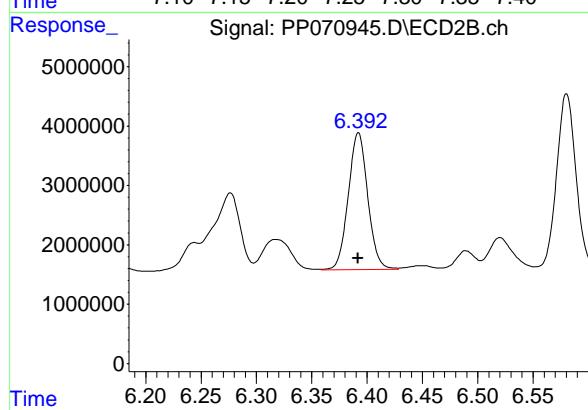

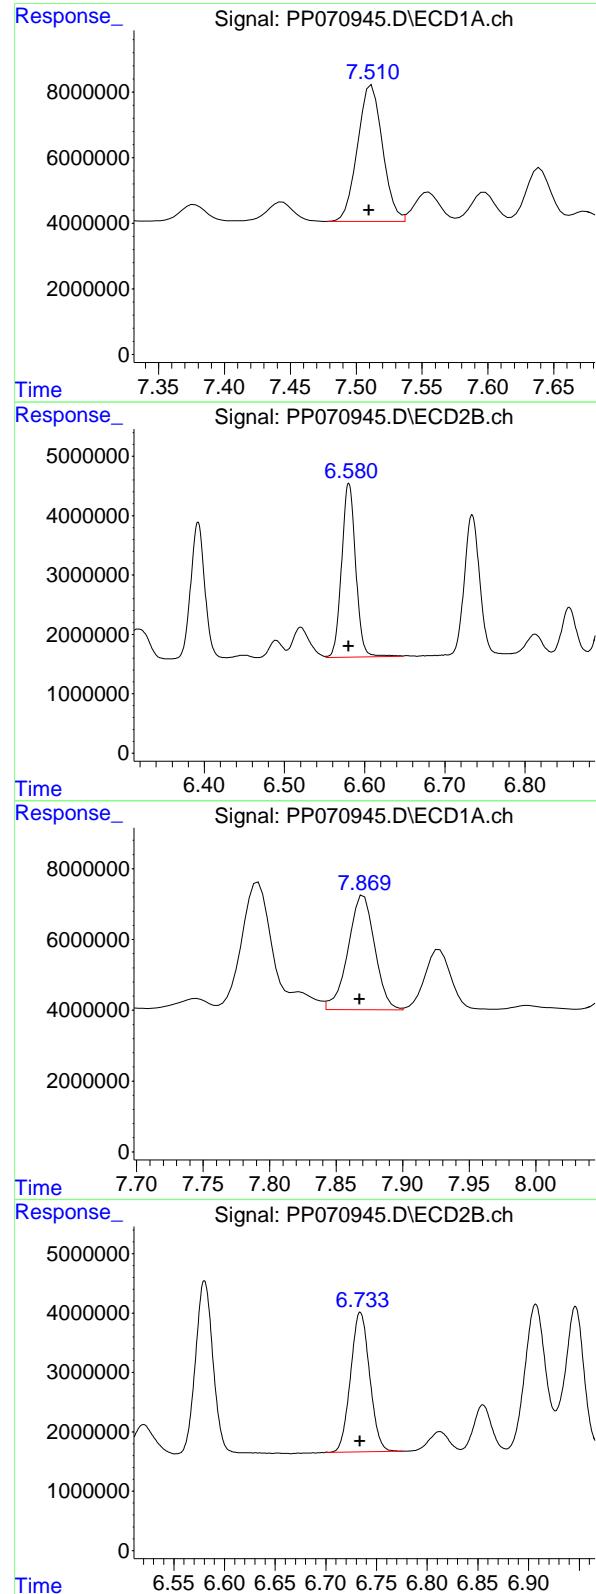

#32 AR-1260-2

R.T.: 7.512 min  
 Delta R.T.: 0.002 min  
 Response: 54825330 ECD\_P  
 Conc: 570.29 ng/ml ClientSampleId :  
 ICVPP032725

#32 AR-1260-2


R.T.: 6.580 min  
 Delta R.T.: 0.000 min  
 Response: 35718929  
 Conc: 559.91 ng/ml

#33 AR-1260-3

R.T.: 7.871 min  
 Delta R.T.: 0.003 min  
 Response: 45118892  
 Conc: 564.56 ng/ml

#33 AR-1260-3

R.T.: 6.734 min  
 Delta R.T.: 0.000 min  
 Response: 30750809  
 Conc: 564.37 ng/ml

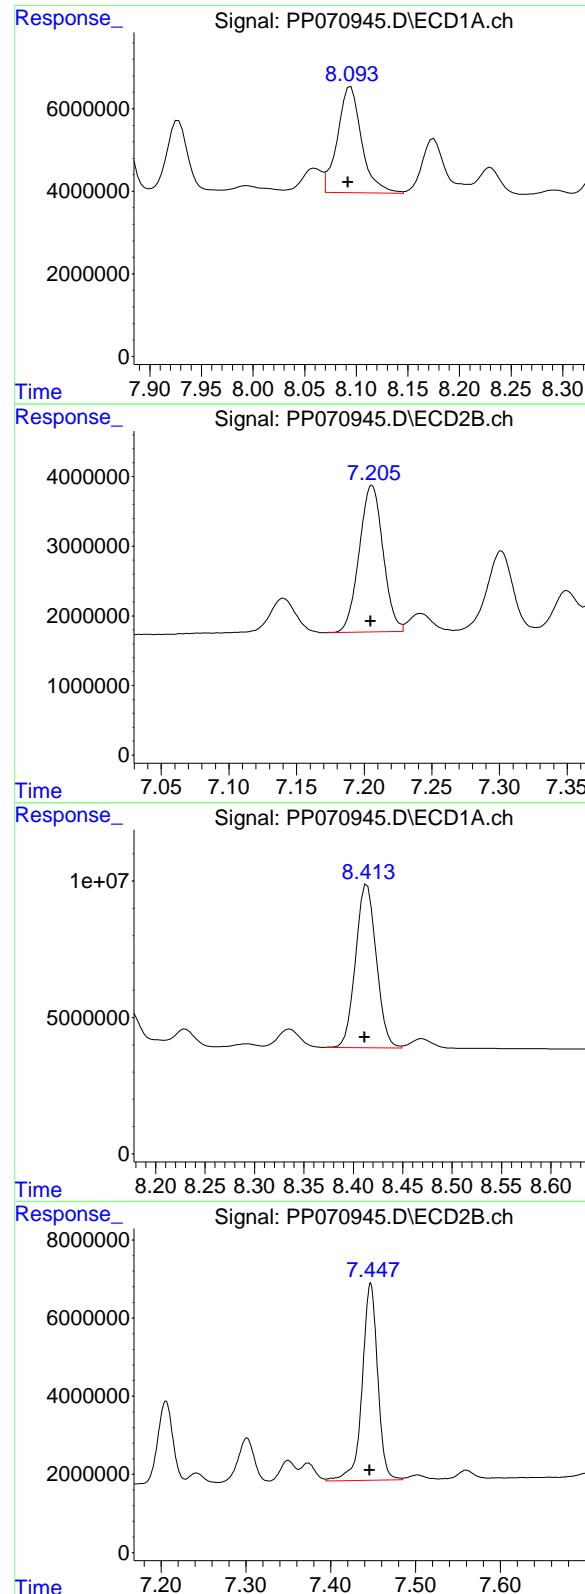

#34 AR-1260-4

R.T.: 8.095 min  
 Delta R.T.: 0.003 min  
 Response: 41972897  
 Conc: 533.08 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** ICVPP032725

#34 AR-1260-4

R.T.: 7.206 min  
 Delta R.T.: 0.000 min  
 Response: 25791995  
 Conc: 539.28 ng/ml

#35 AR-1260-5

R.T.: 8.414 min  
 Delta R.T.: 0.003 min  
 Response: 87345749  
 Conc: 549.74 ng/ml

#35 AR-1260-5

R.T.: 7.447 min  
 Delta R.T.: 0.000 min  
 Response: 64063663  
 Conc: 514.53 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070946.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 18:42  
 Operator : YP\AJ  
 Sample : AR1242ICV500  
 Misc :  
 ALS Vial : 32 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1242**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 19:00:51 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 18:58:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	4.515	3.816	78786041	55016883	53.357	51.300
2) SA Decachloro...	10.230	8.859	57489647	39612860	53.073	51.065

Target Compounds

16) L4 AR-1242-1	5.667	4.904	21998453	17657296	500.225	516.358
17) L4 AR-1242-2	5.689	4.922	33746674	24829266	524.698	504.069
18) L4 AR-1242-3	5.752	5.099	20359598	13889595	496.098	521.298
19) L4 AR-1242-4	5.849	5.183	16580558	13666228	543.209	518.087
20) L4 AR-1242-5	6.580	5.708	19203834	15992906	525.982	516.595



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070946.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 18:42  
 Operator : YP\AJ  
 Sample : AR1242ICV500  
 Misc :  
 ALS Vial : 32 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1242**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 19:00:51 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 18:58:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

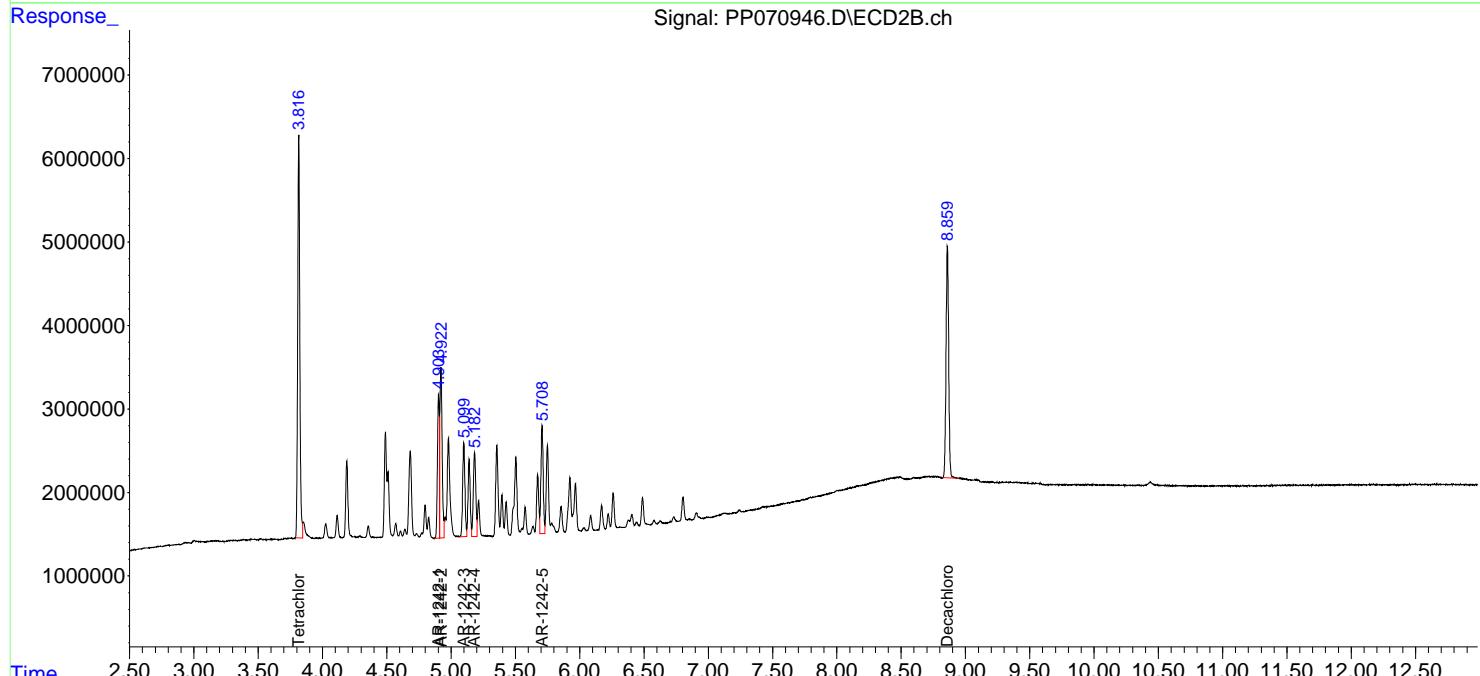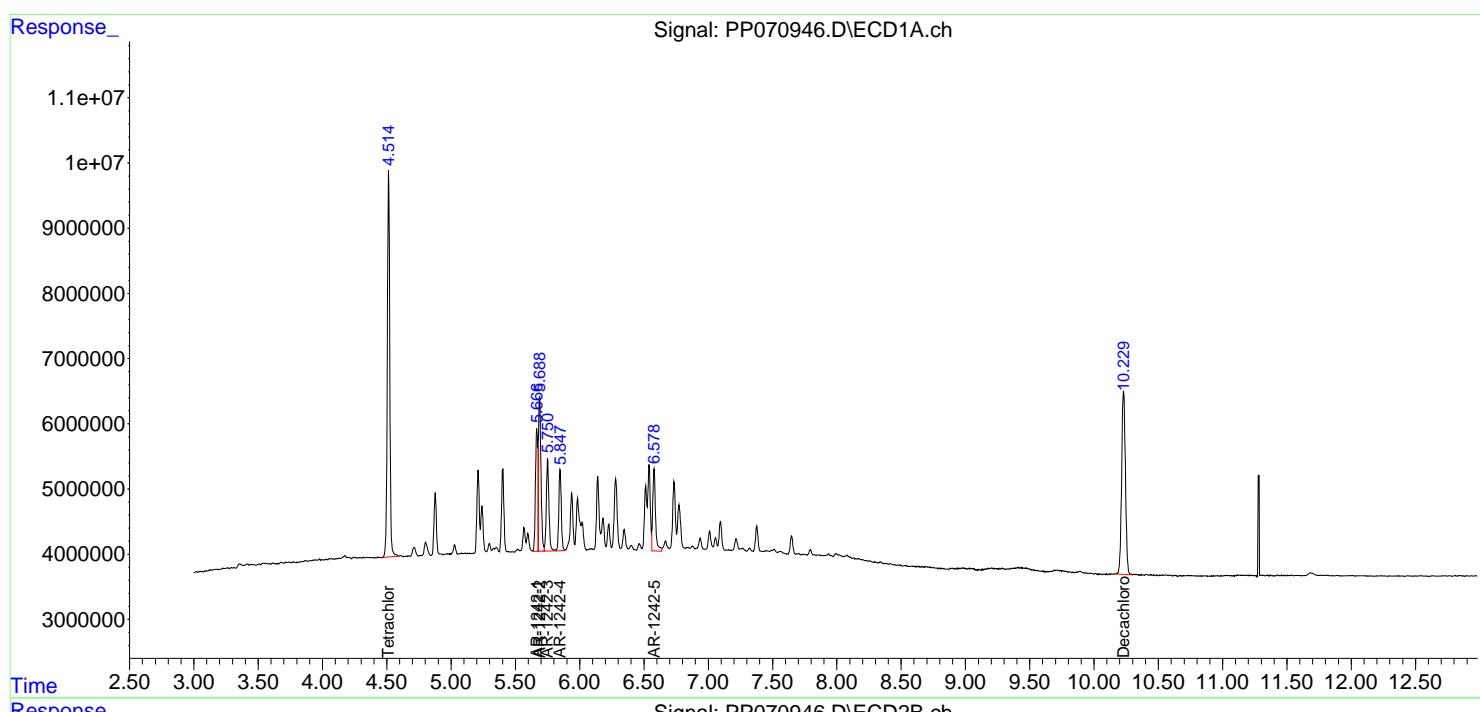

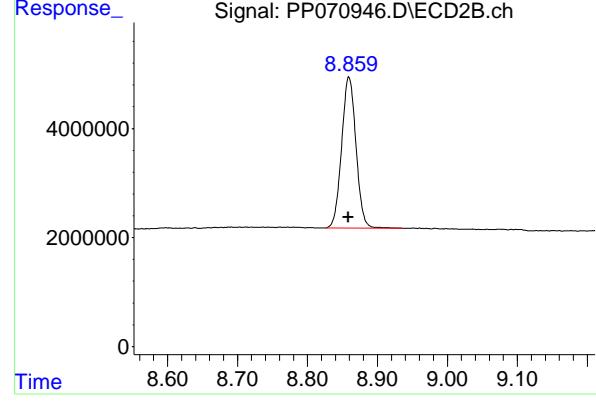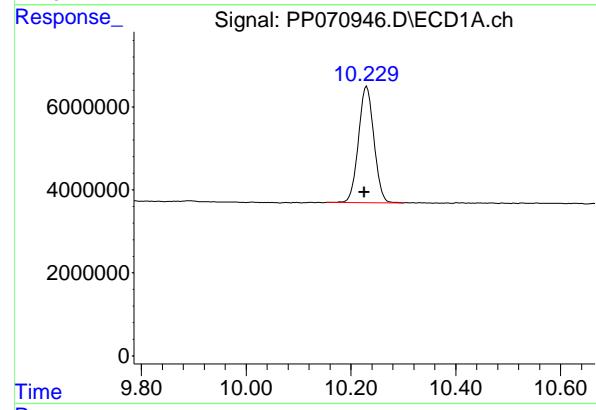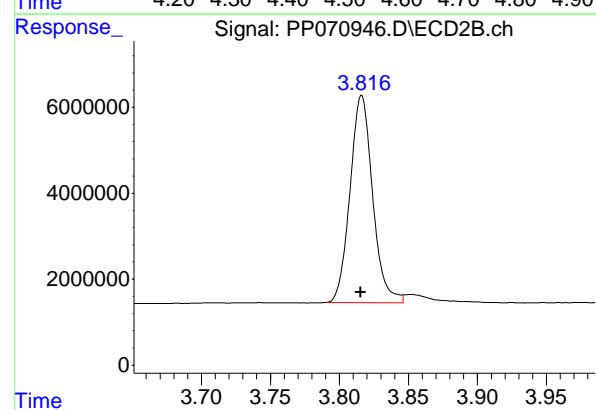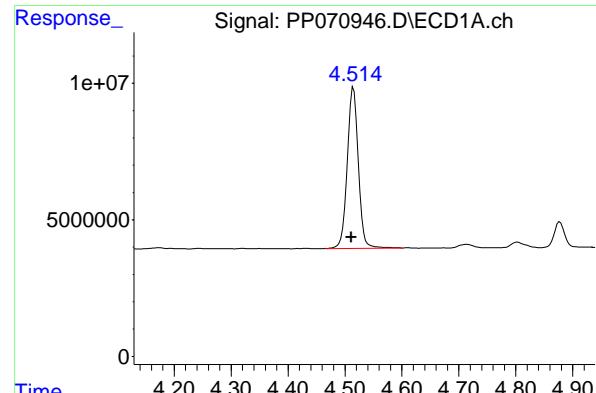

## #1 Tetrachloro-m-xylene

R.T.: 4.515 min  
Delta R.T.: 0.004 min  
Instrument: ECD\_P  
Response: 78786041  
Conc: 53.36 ng/ml ClientSampleId : ICVPP032725AR1242

## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 55016883  
Conc: 51.30 ng/ml

## #2 Decachlorobiphenyl


R.T.: 10.230 min  
Delta R.T.: 0.005 min  
Response: 57489647  
Conc: 53.07 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.001 min  
Response: 39612860  
Conc: 51.07 ng/ml


#16 AR-1242-1

R.T.: 5.667 min  
 Delta R.T.: 0.003 min  
 Response: 21998453 ECD\_P  
 Conc: 500.22 ng/ml ClientSampleId :  
 ICVPP032725AR1242

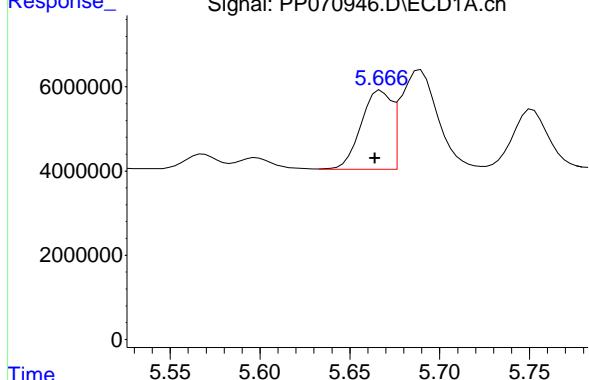


#16 AR-1242-1

R.T.: 4.904 min  
 Delta R.T.: 0.001 min  
 Response: 17657296  
 Conc: 516.36 ng/ml

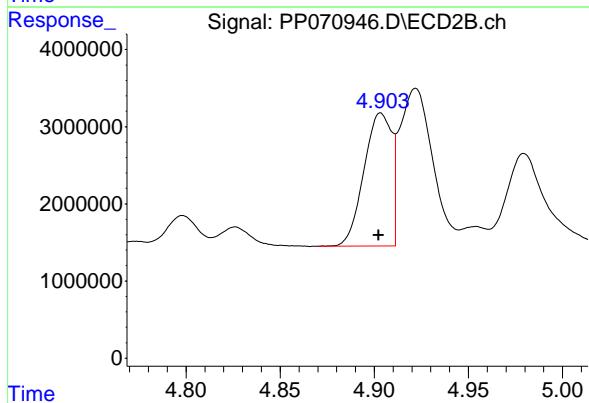


#17 AR-1242-2

R.T.: 5.689 min  
 Delta R.T.: 0.004 min  
 Response: 33746674  
 Conc: 524.70 ng/ml

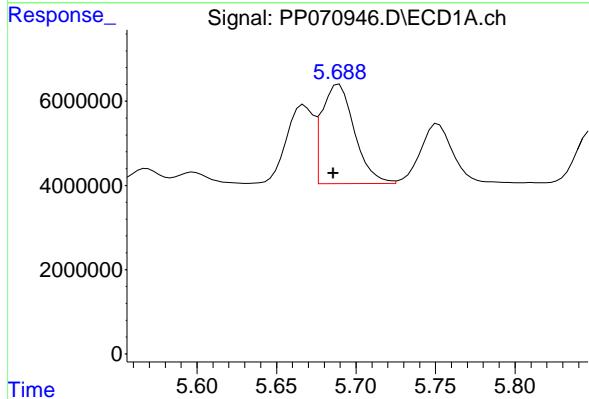


#17 AR-1242-2

R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 24829266  
 Conc: 504.07 ng/ml

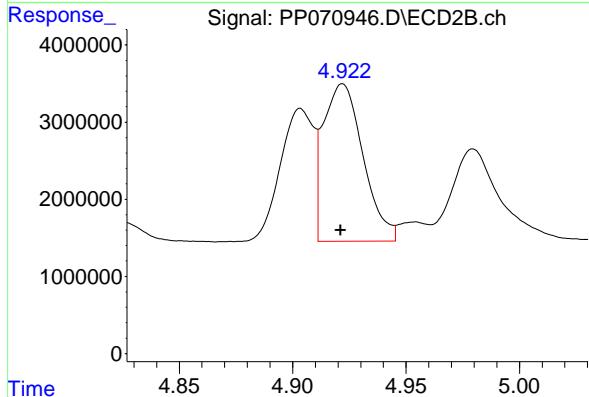


#18 AR-1242-3

R.T.: 5.752 min  
 Delta R.T.: 0.004 min  
 Response: 20359598 ECD\_P  
 Conc: 496.10 ng/ml ClientSampleId :  
 ICVPP032725AR1242

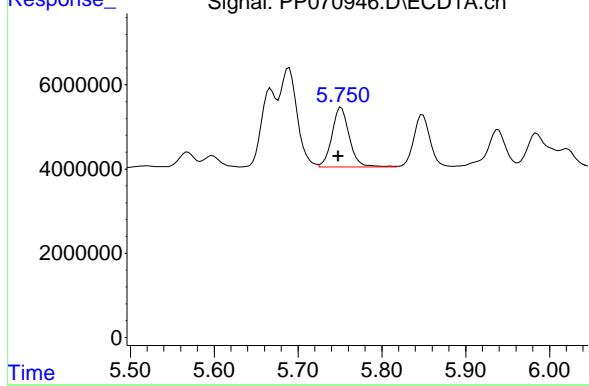


#18 AR-1242-3

R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 13889595  
 Conc: 521.30 ng/ml

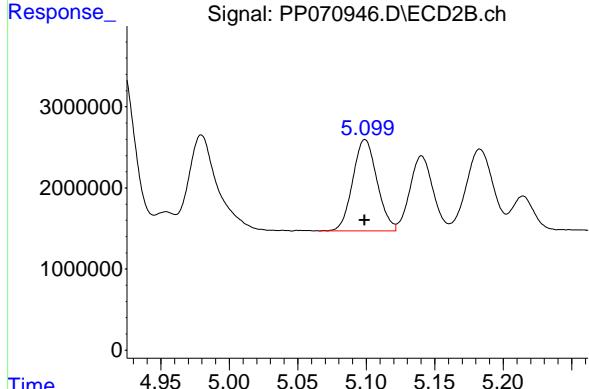


#19 AR-1242-4

R.T.: 5.849 min  
 Delta R.T.: 0.004 min  
 Response: 16580558  
 Conc: 543.21 ng/ml

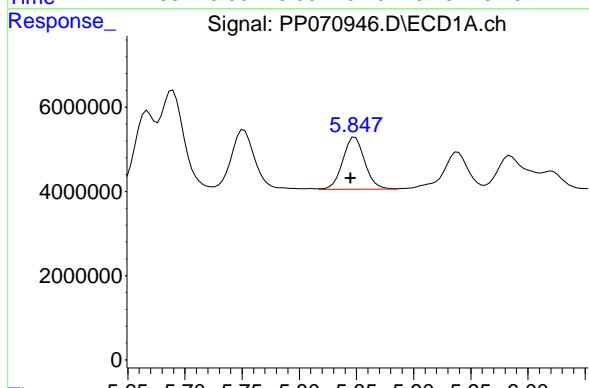



#19 AR-1242-4

R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 13666228  
 Conc: 518.09 ng/ml

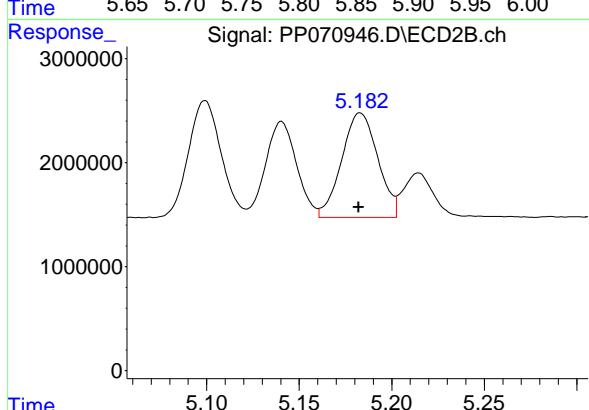

#20 AR-1242-5

R.T.: 6.580 min  
Delta R.T.: 0.004 min  
Instrument: ECD\_P  
Response: 19203834  
Conc: 525.98 ng/ml  
ClientSampleId: ICVPP032725AR1242

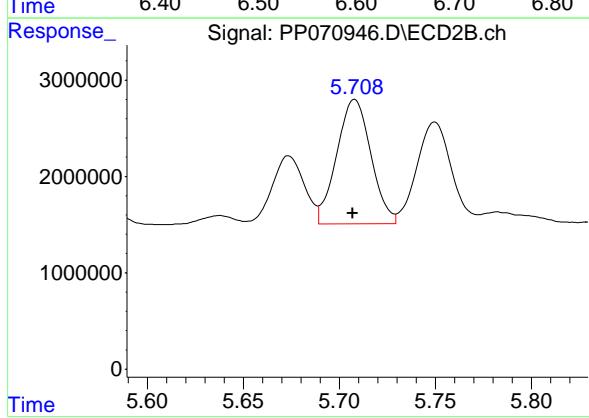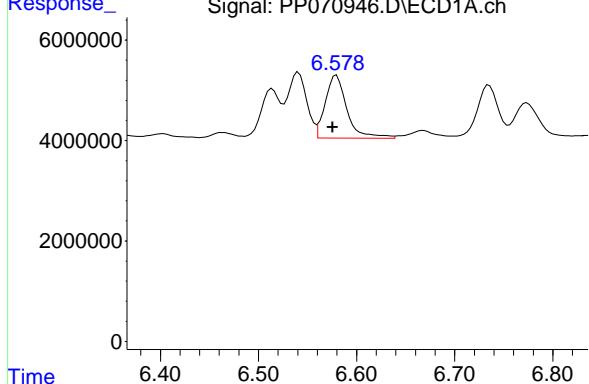

#20 AR-1242-5

R.T.: 5.708 min  
Delta R.T.: 0.000 min  
Response: 15992906  
Conc: 516.60 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070947.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 19:15  
 Operator : YP\AJ  
 Sample : AR1248ICV500  
 Misc :  
 ALS Vial : 33 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1248**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 19:34:19 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 19:07:15 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	4.514	3.817	80868018	57291573	53.345	52.976
2) SA Decachloro...	10.229	8.860	60625729	42784323	53.381	54.139

Target Compounds

21) L5 AR-1248-1	5.666	4.904	17556753	15279017	483.824	564.218
22) L5 AR-1248-2	5.937	5.141	24046455	20552003	535.096	559.658
23) L5 AR-1248-3	6.140	5.183	26863901	21355068	530.514	552.390
24) L5 AR-1248-4	6.539	5.356	33592146	24182903	523.670	535.719
25) L5 AR-1248-5	6.578	5.750	32500443	22380961	534.140	524.405



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070947.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 19:15  
 Operator : YP\AJ  
 Sample : AR1248ICV500  
 Misc :  
 ALS Vial : 33 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1248**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 19:34:19 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 19:07:15 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

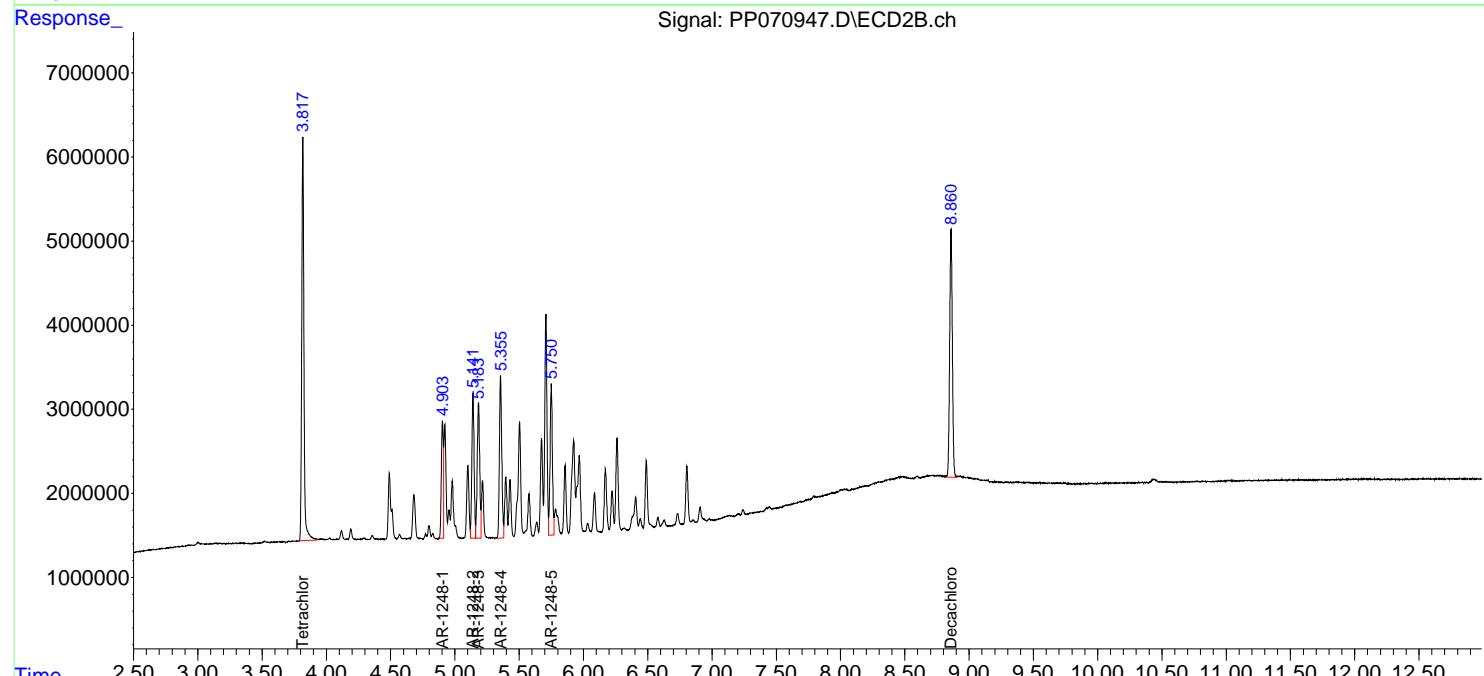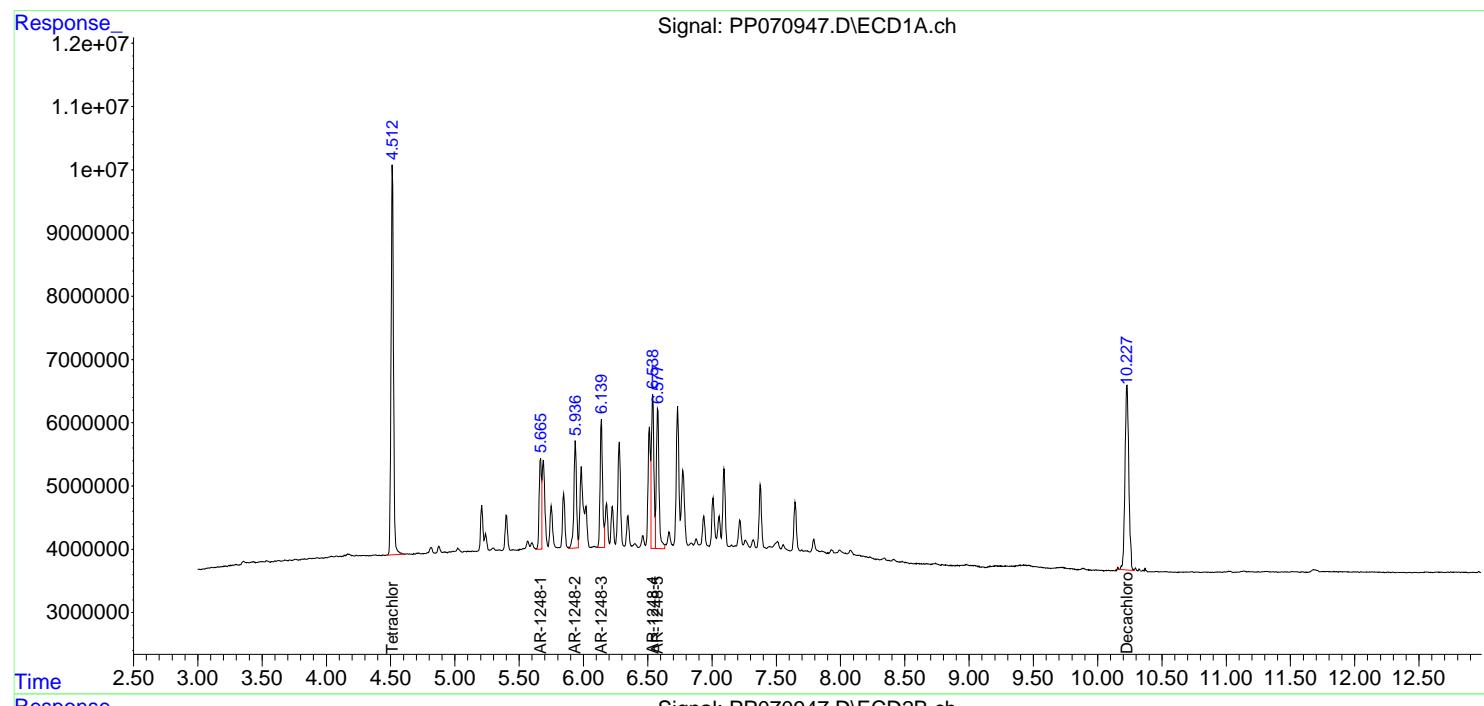

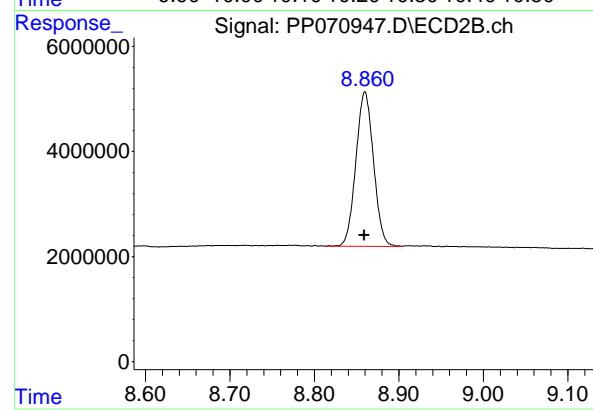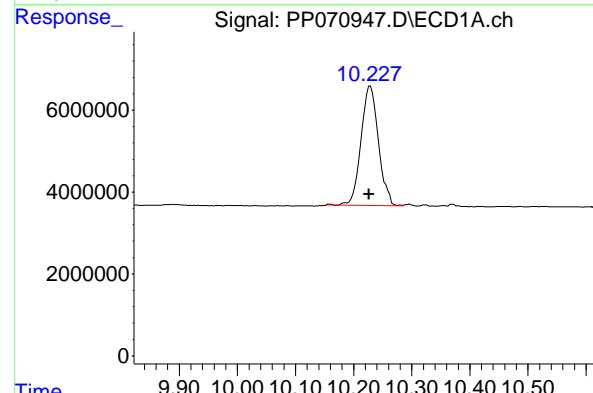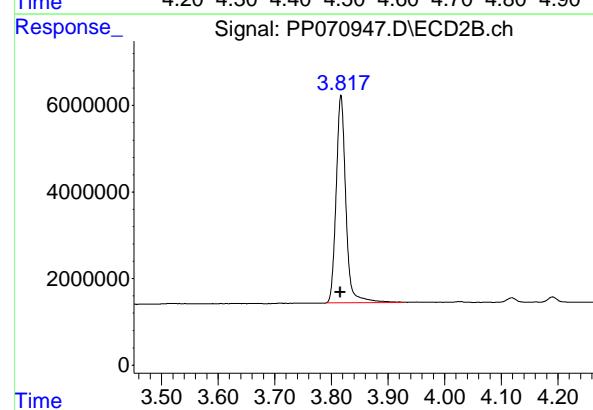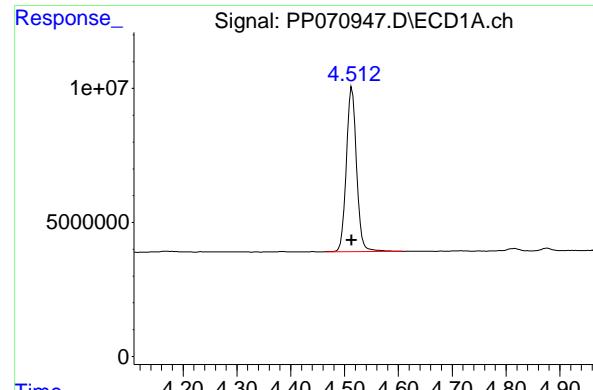

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
Delta R.T.: 0.000 min  
Instrument:  
Response: 80868018 ECD\_P  
Conc: 53.34 ng/ml ClientSampleId :  
ICVPP032725AR1248

## #1 Tetrachloro-m-xylene





R.T.: 3.817 min  
Delta R.T.: 0.001 min  
Response: 57291573  
Conc: 52.98 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.229 min  
Delta R.T.: 0.002 min  
Response: 60625729  
Conc: 53.38 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.860 min  
Delta R.T.: 0.001 min  
Response: 42784323  
Conc: 54.14 ng/ml

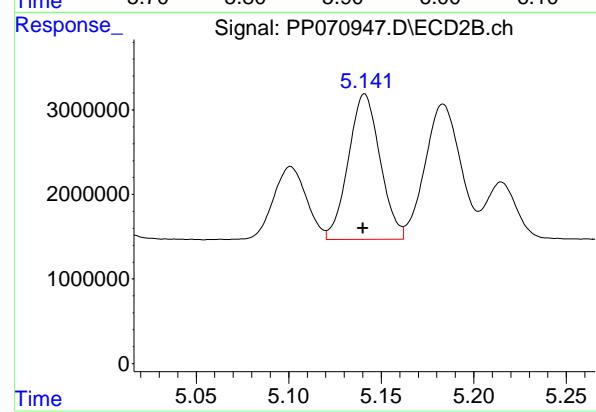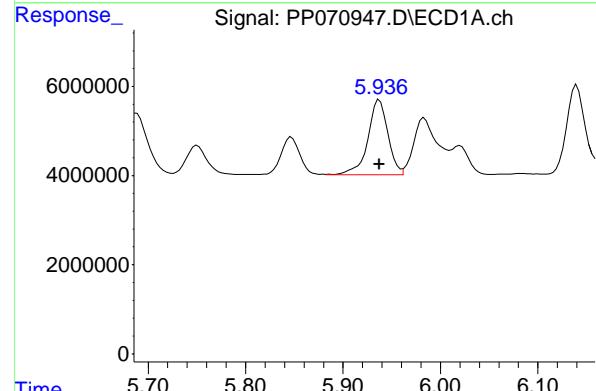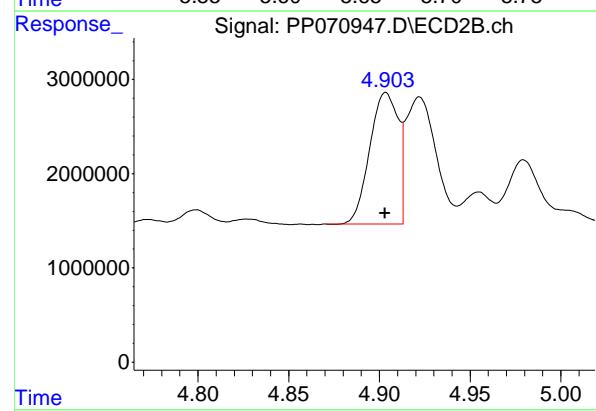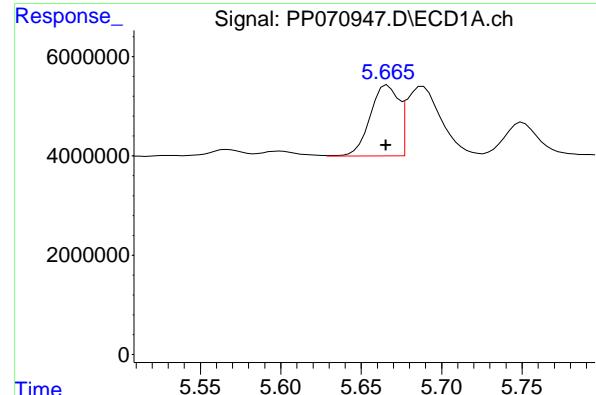

#21 AR-1248-1

R.T.: 5.666 min  
 Delta R.T.: 0.000 min  
 Response: 17556753 ECD\_P  
 Conc: 483.82 ng/ml ClientSampleId :  
 ICVPP032725AR1248

#21 AR-1248-1

R.T.: 4.904 min  
 Delta R.T.: 0.000 min  
 Response: 15279017  
 Conc: 564.22 ng/ml

#22 AR-1248-2


R.T.: 5.937 min  
 Delta R.T.: 0.000 min  
 Response: 24046455  
 Conc: 535.10 ng/ml

#22 AR-1248-2

R.T.: 5.141 min  
 Delta R.T.: 0.001 min  
 Response: 20552003  
 Conc: 559.66 ng/ml


#23 AR-1248-3

R.T.: 6.140 min  
 Delta R.T.: 0.000 min  
 Response: 26863901 ECD\_P  
 Conc: 530.51 ng/ml ClientSampleId :  
 ICVPP032725AR1248

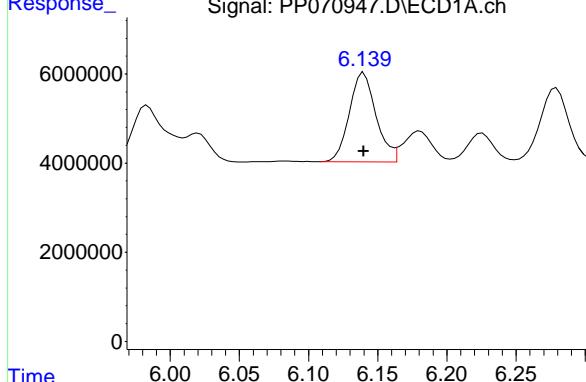


#23 AR-1248-3

R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 21355068  
 Conc: 552.39 ng/ml

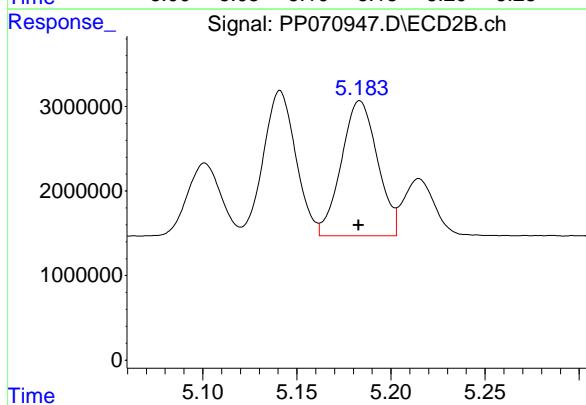


#24 AR-1248-4

R.T.: 6.539 min  
 Delta R.T.: 0.000 min  
 Response: 33592146  
 Conc: 523.67 ng/ml

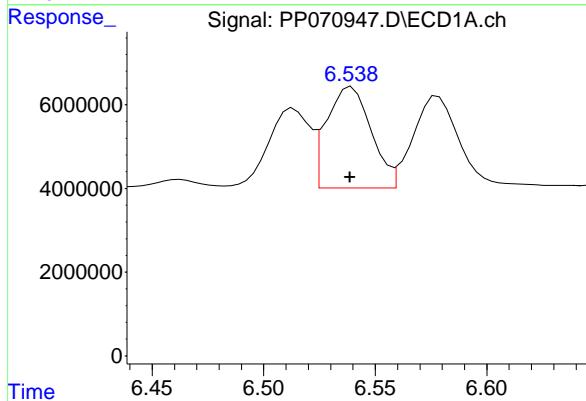



#24 AR-1248-4

R.T.: 5.356 min  
 Delta R.T.: 0.000 min  
 Response: 24182903  
 Conc: 535.72 ng/ml

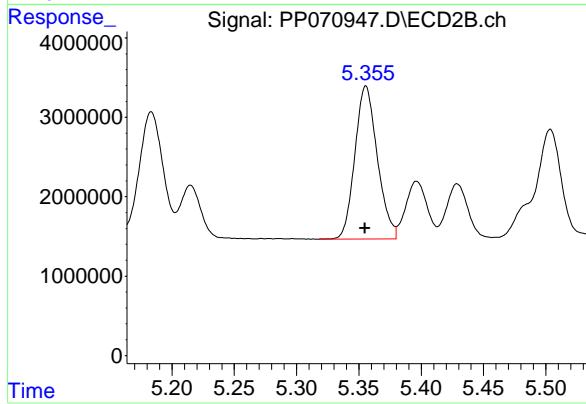

#25 AR-1248-5

R.T.: 6.578 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 32500443  
Conc: 534.14 ng/ml  
ClientSampleId: ICVPP032725AR1248

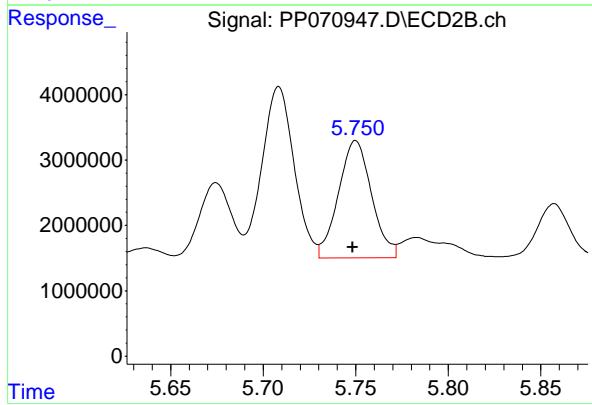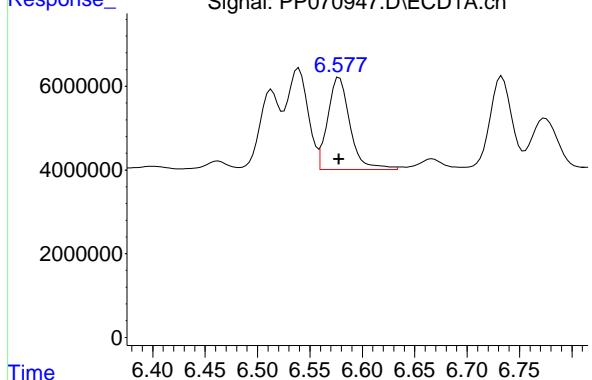

#25 AR-1248-5

R.T.: 5.750 min  
Delta R.T.: 0.002 min  
Response: 22380961  
Conc: 524.41 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070948.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 19:47  
 Operator : YP\AJ  
 Sample : AR1254ICV500  
 Misc :  
 ALS Vial : 34 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1254**

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 01:39:10 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 01:37:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachloro...	4.513	3.816	80813408	55809150	53.470	50.687
2) SA Decachloro...	10.228	8.859	60442284	44113864	53.599	53.797

**Target Compounds**

26) L6 AR-1254-1	6.514	5.708	34026950	33372474	528.449	505.507
27) L6 AR-1254-2	6.730	5.856	52171420	28060451	516.086	491.442
28) L6 AR-1254-3	7.093	6.260	52059367	42608413	522.014	490.647
29) L6 AR-1254-4	7.375	6.489	45346150	27407702	523.647	488.547
30) L6 AR-1254-5	7.790	6.907	41706053	36336253	519.049m	503.617

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070948.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 19:47  
 Operator : YP\AJ  
 Sample : AR12541CV500  
 Misc :  
 ALS Vial : 34 Sample Multiplier: 1



Instrument :  
 ECD\_P  
 ClientSampleId :  
 ICVPP032725AR1254


**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 01:39:10 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 01:37:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

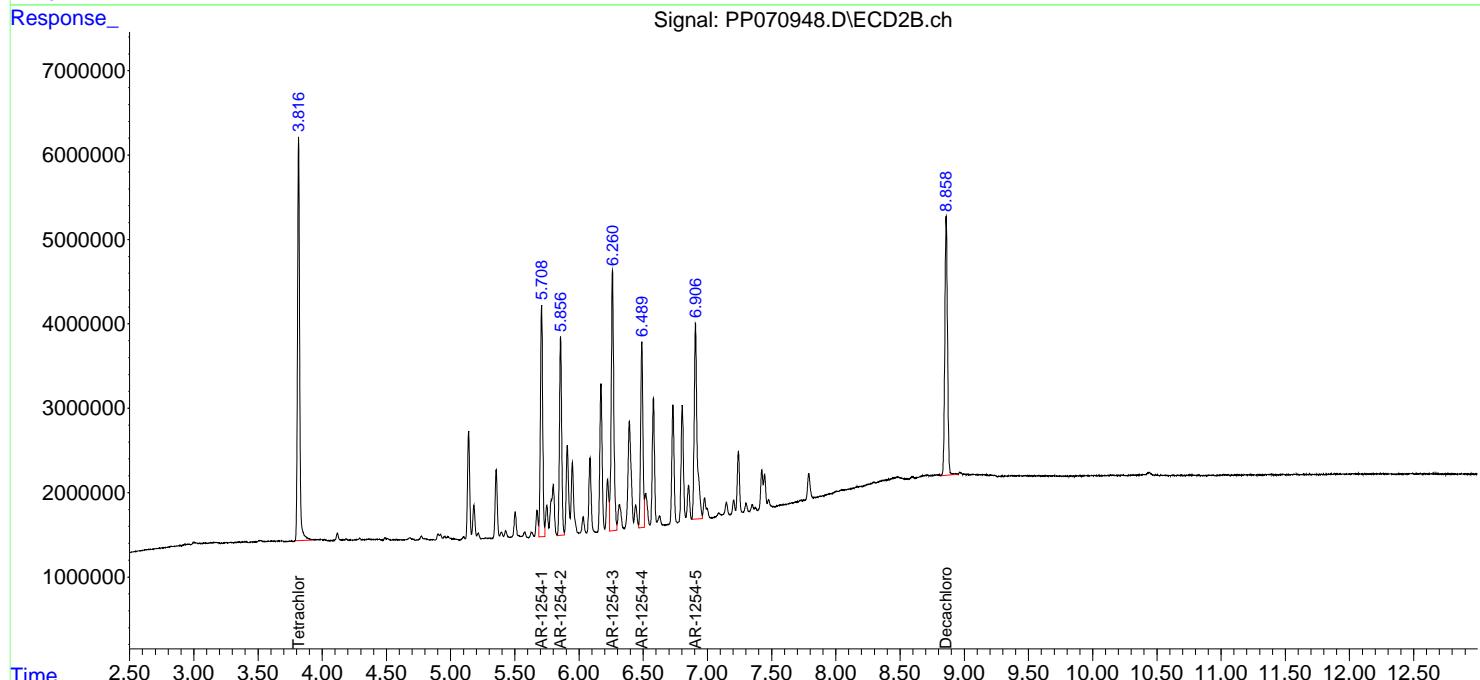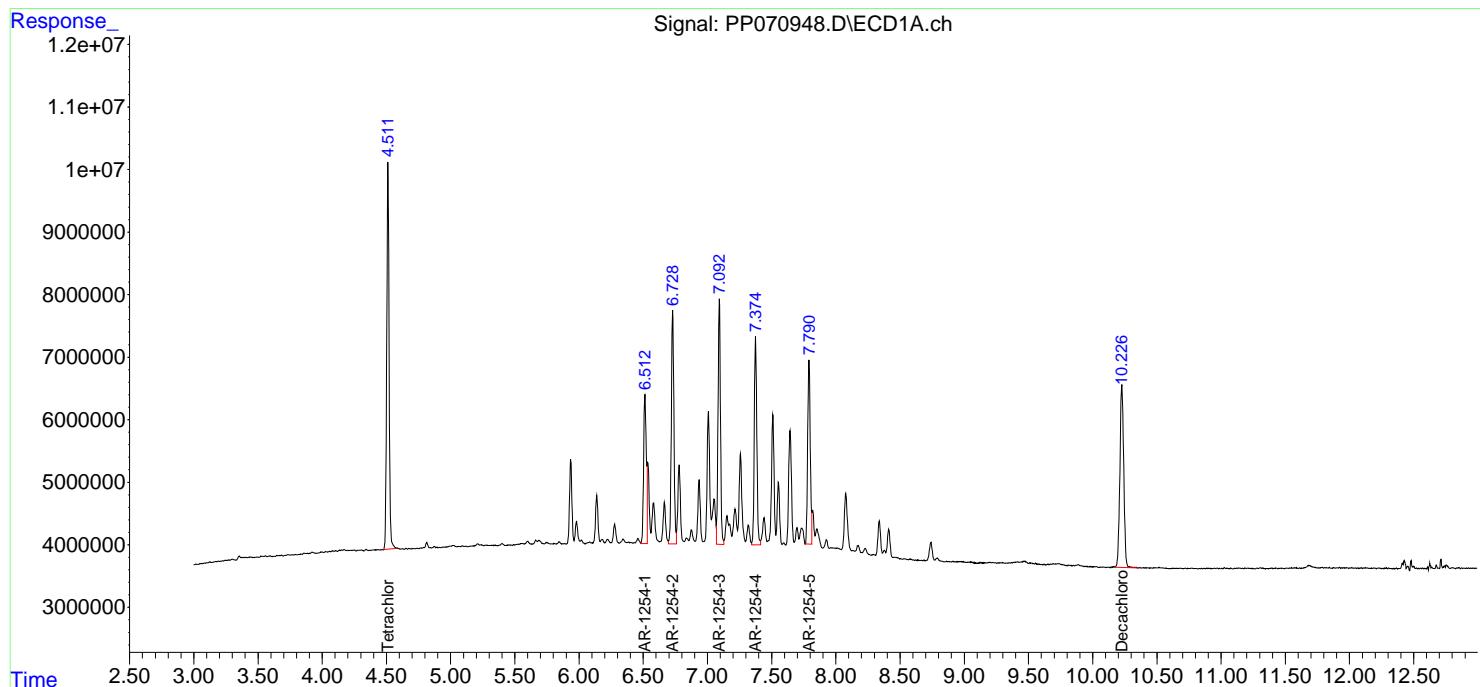

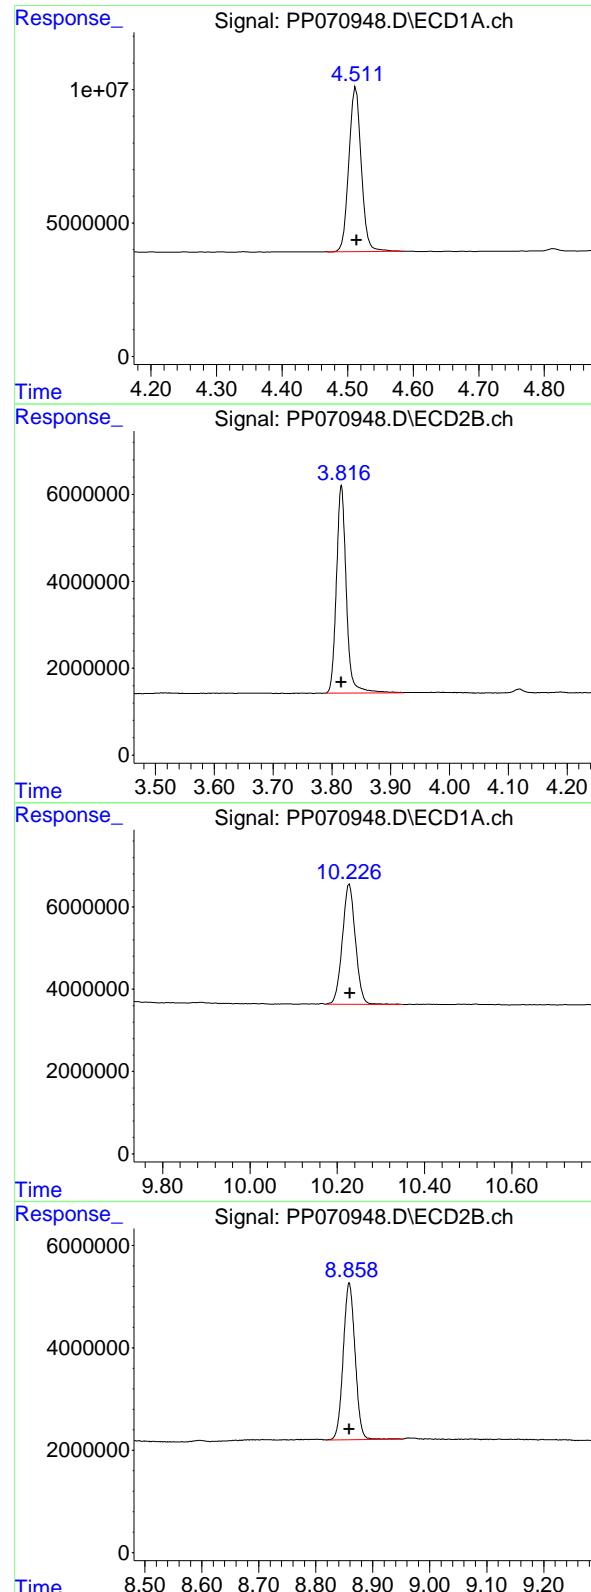

## #1 Tetrachloro-m-xylene

R.T.: 4.513 min  
 Delta R.T.: -0.001 min  
 Response: 80813408 ECD\_P  
 Conc: 53.47 ng/ml ClientSampleId :  
 ICVPP032725AR1254

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 55809150  
 Conc: 50.69 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.228 min  
 Delta R.T.: -0.002 min  
 Response: 60442284  
 Conc: 53.60 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 44113864  
 Conc: 53.80 ng/ml

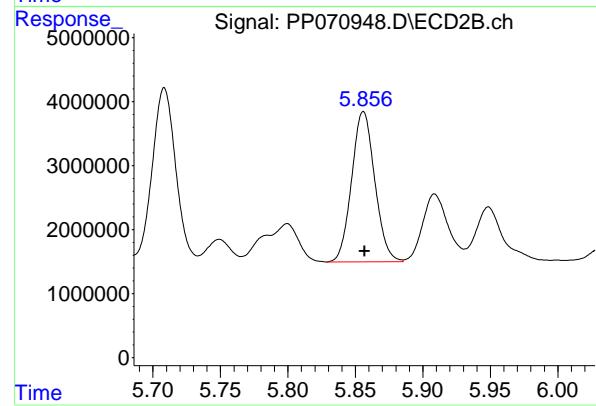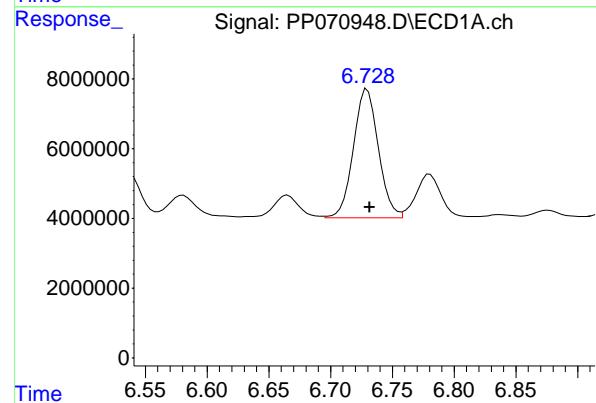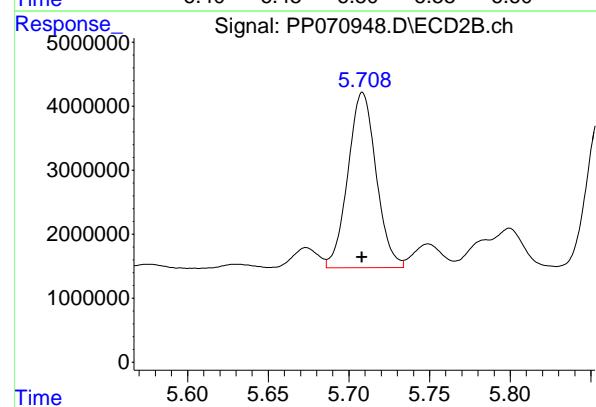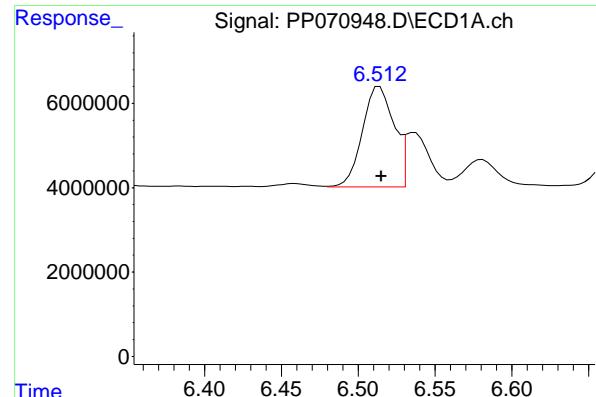

#26 AR-1254-1

R.T.: 6.514 min  
 Delta R.T.: -0.001 min  
 Response: 34026950 ECD\_P  
 Conc: 528.45 ng/ml ClientSampleId :  
 ICVPP032725AR1254

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#26 AR-1254-1





R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 33372474  
 Conc: 505.51 ng/ml

#27 AR-1254-2

R.T.: 6.730 min  
 Delta R.T.: -0.002 min  
 Response: 52171420  
 Conc: 516.09 ng/ml

#27 AR-1254-2

R.T.: 5.856 min  
 Delta R.T.: 0.000 min  
 Response: 28060451  
 Conc: 491.44 ng/ml

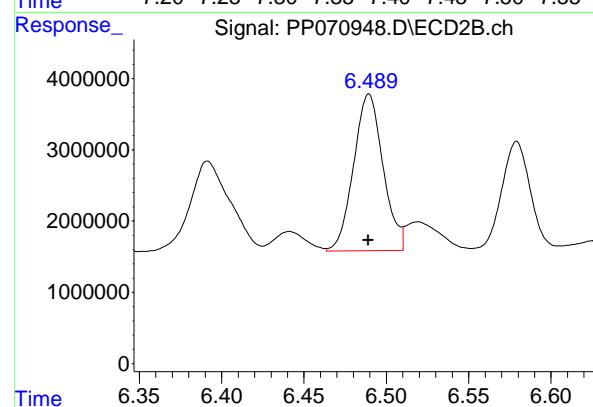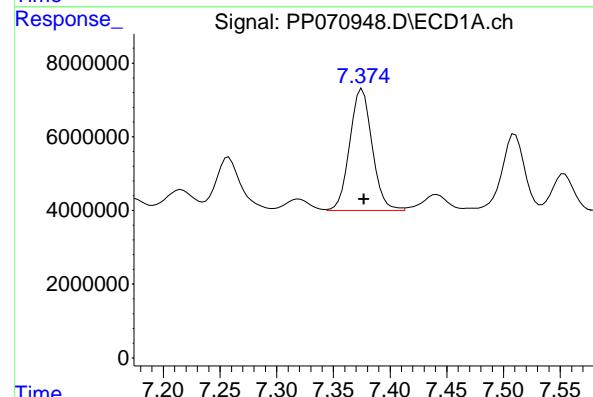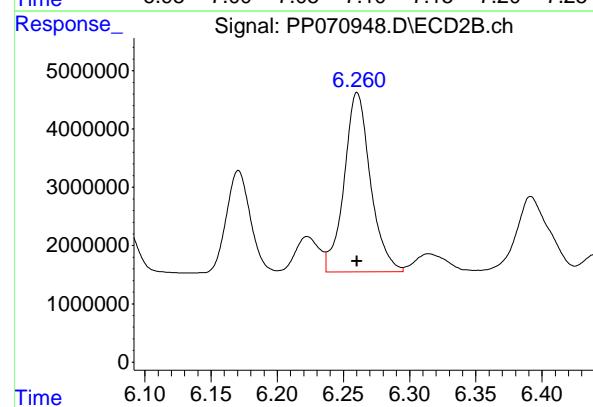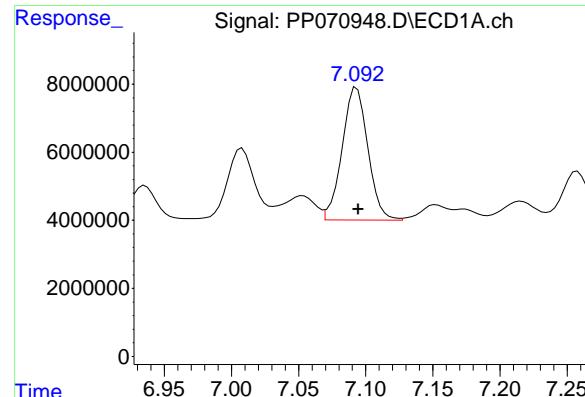

#28 AR-1254-3

R.T.: 7.093 min  
 Delta R.T.: -0.001 min  
 Response: 52059367  
 Conc: 522.01 ng/ml

Instrument: ECD\_P  
 ClientSampleId: ICVPP032725AR1254

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#28 AR-1254-3

R.T.: 6.260 min  
 Delta R.T.: 0.000 min  
 Response: 42608413  
 Conc: 490.65 ng/ml

#29 AR-1254-4

R.T.: 7.375 min  
 Delta R.T.: -0.001 min  
 Response: 45346150  
 Conc: 523.65 ng/ml

#29 AR-1254-4

R.T.: 6.489 min  
 Delta R.T.: 0.000 min  
 Response: 27407702  
 Conc: 488.55 ng/ml

#30 AR-1254-5


R.T.: 7.790 min  
 Delta R.T.: -0.003 min  
 Response: 41706053 ECD\_P  
 Conc: 519.05 ng/ml ClientSampleId :  
 ICVPP032725AR1254

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/28/2025  
 Supervised By :mohammad ahmed 03/31/2025

#30 AR-1254-5

R.T.: 6.907 min  
 Delta R.T.: 0.000 min  
 Response: 36336253  
 Conc: 503.62 ng/ml

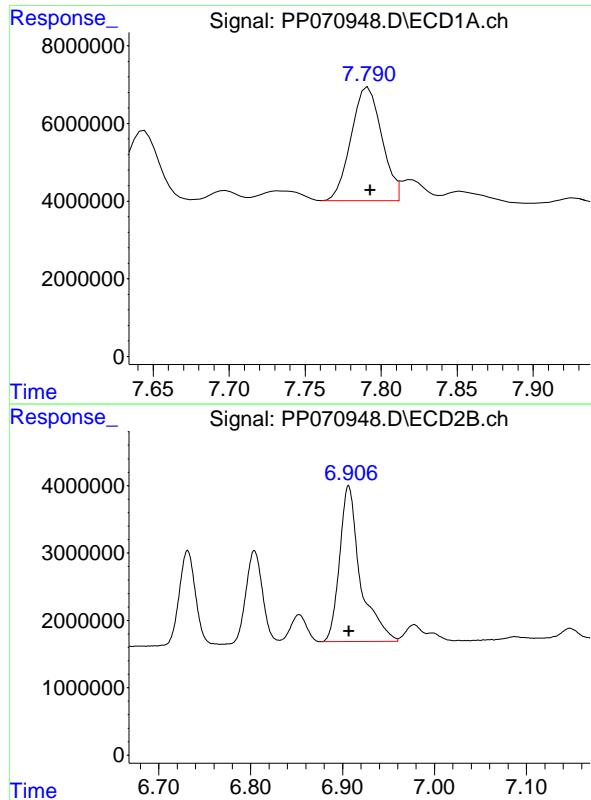

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070949.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 20:20  
 Operator : YP\AJ  
 Sample : AR1268ICV500  
 Misc :  
 ALS Vial : 35 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1268**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 01:48:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 01:43:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	4.516	3.816	81260121	54086649	52.018	47.172
2) SA Decachlor...	10.231	8.858	106.7E6	75635416	51.843	49.238

**Target Compounds**

41) L9 AR-1268-1	8.729	7.728	122.6E6	85915063	520.500	501.249
42) L9 AR-1268-2	8.822	7.793	102.3E6	71467631	523.804	498.787
43) L9 AR-1268-3	9.054	7.999	88458310	61199335	517.562	496.952
44) L9 AR-1268-4	9.472	8.292	37948087	26301297	536.390	498.006
45) L9 AR-1268-5	9.889	8.595	246.0E6	175.8E6	516.662	485.835


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070949.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 20:20  
 Operator : YP\AJ  
 Sample : AR12681CV500  
 Misc :  
 ALS Vial : 35 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1268**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 01:48:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 01:43:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

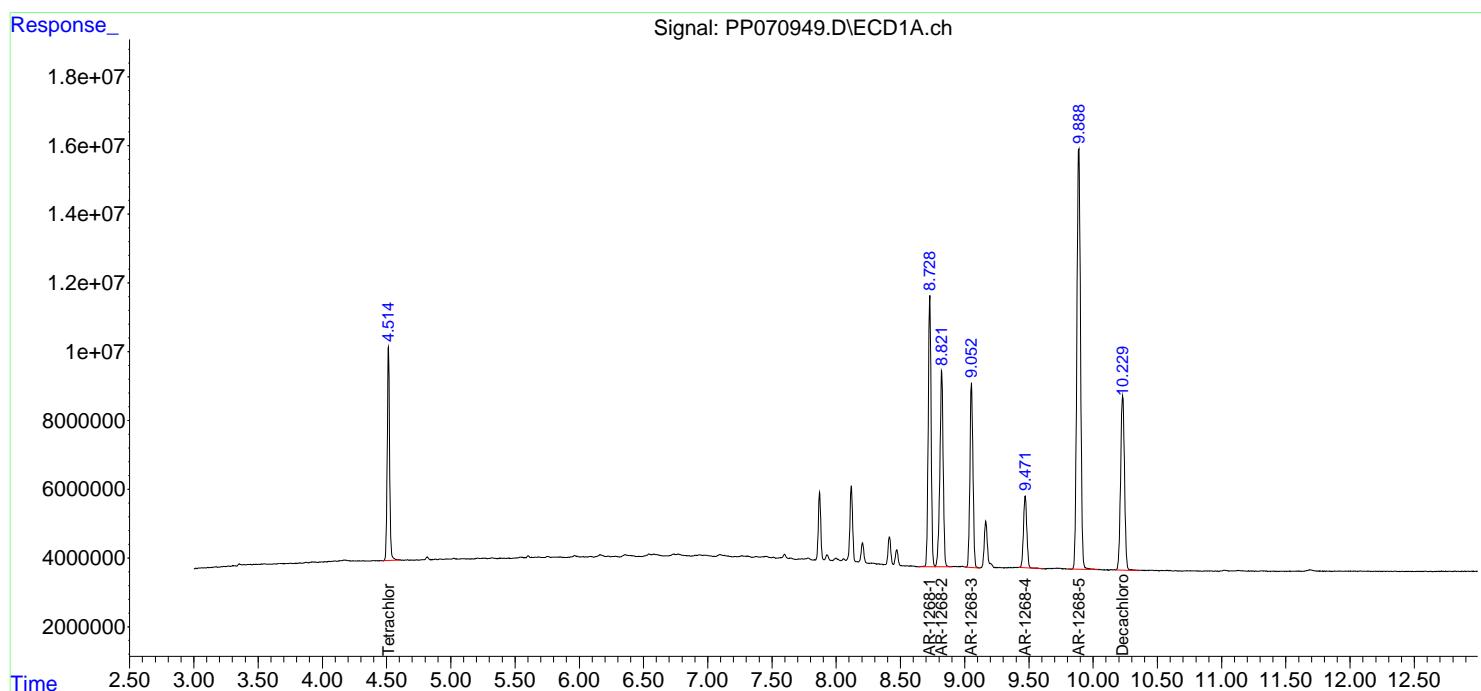

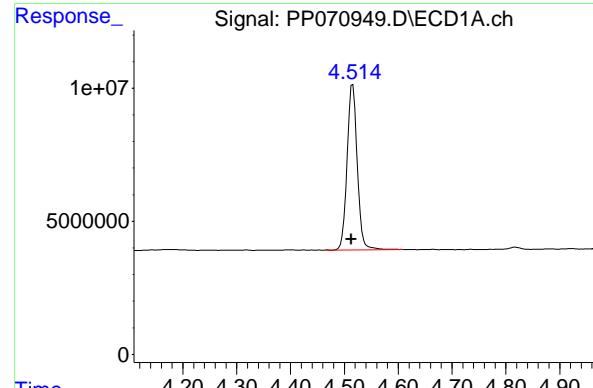


## #1 Tetrachloro-m-xylene

R.T.: 4.516 min  
Delta R.T.: 0.003 min  
Instrument:  
Response: 81260121 ECD\_P  
Conc: 52.02 ng/ml ClientSampleId :  
ICVPP032725AR1268

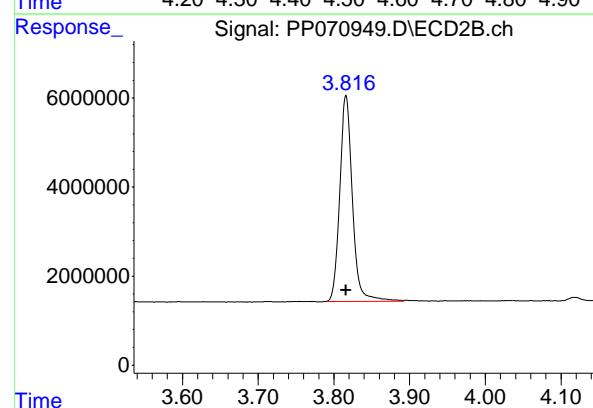


## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 54086649  
Conc: 47.17 ng/ml

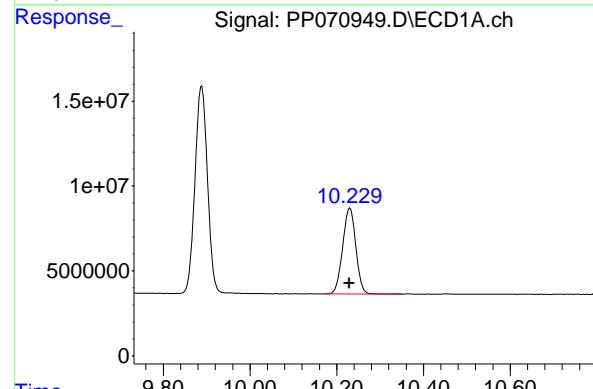

## #2 Decachlorobiphenyl

R.T.: 10.231 min  
Delta R.T.: 0.000 min  
Response: 106656431  
Conc: 51.84 ng/ml

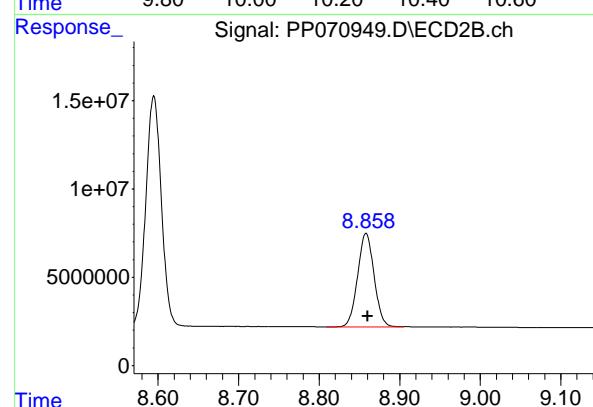


## #2 Decachlorobiphenyl

R.T.: 8.858 min  
Delta R.T.: -0.002 min  
Response: 75635416  
Conc: 49.24 ng/ml


#41 AR-1268-1

R.T.: 8.729 min  
 Delta R.T.: 0.000 min  
 Response: 122581794 ECD\_P  
 Conc: 520.50 ng/ml ClientSampleId :  
 ICVPP032725AR1268

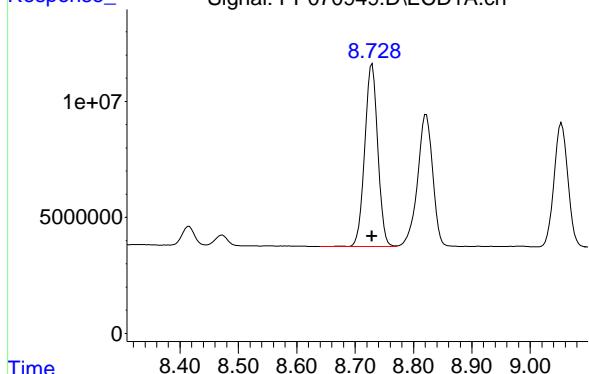


#41 AR-1268-1

R.T.: 7.728 min  
 Delta R.T.: 0.000 min  
 Response: 85915063  
 Conc: 501.25 ng/ml

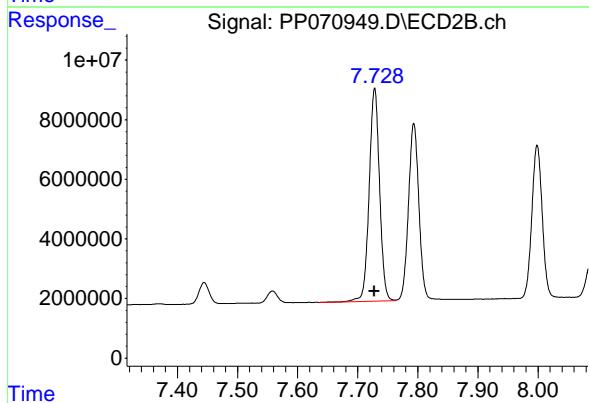


#42 AR-1268-2

R.T.: 8.822 min  
 Delta R.T.: 0.000 min  
 Response: 102307003  
 Conc: 523.80 ng/ml

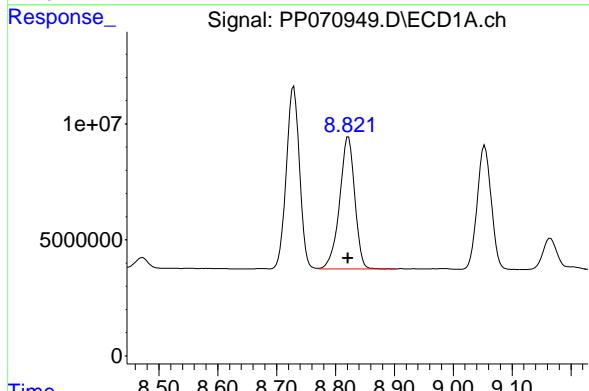


#42 AR-1268-2

R.T.: 7.793 min  
 Delta R.T.: 0.000 min  
 Response: 71467631  
 Conc: 498.79 ng/ml

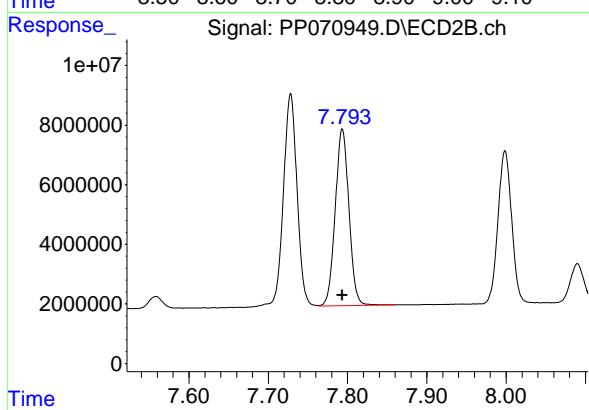


#43 AR-1268-3

R.T.: 9.054 min  
 Delta R.T.: 0.000 min  
 Response: 88458310 ECD\_P  
 Conc: 517.56 ng/ml ClientSampleId :  
 ICVPP032725AR1268

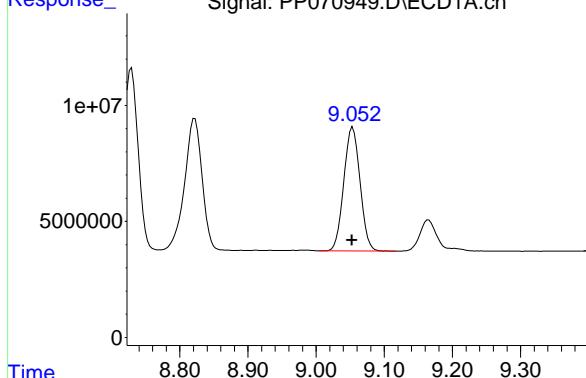


#43 AR-1268-3

R.T.: 7.999 min  
 Delta R.T.: -0.001 min  
 Response: 61199335  
 Conc: 496.95 ng/ml

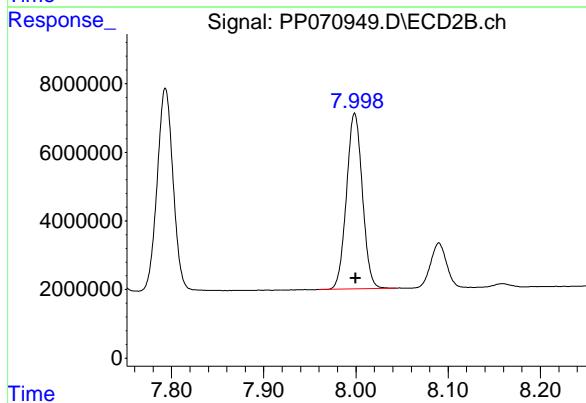


#44 AR-1268-4

R.T.: 9.472 min  
 Delta R.T.: 0.000 min  
 Response: 37948087  
 Conc: 536.39 ng/ml

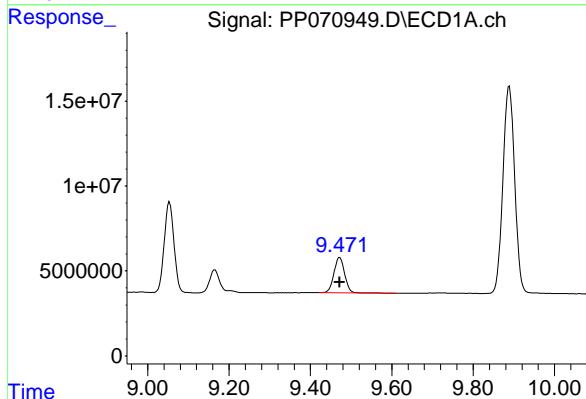


#44 AR-1268-4

R.T.: 8.292 min  
 Delta R.T.: 0.000 min  
 Response: 26301297  
 Conc: 498.01 ng/ml

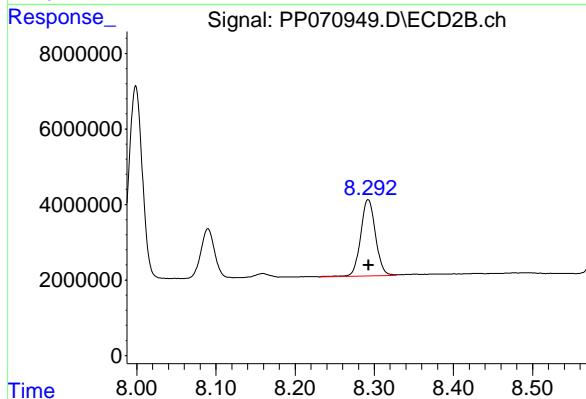


#45 AR-1268-5

R.T.: 9.889 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_P  
Response: 246021928  
Conc: 516.66 ng/ml  
ClientSampleId: ICVPP032725AR1268

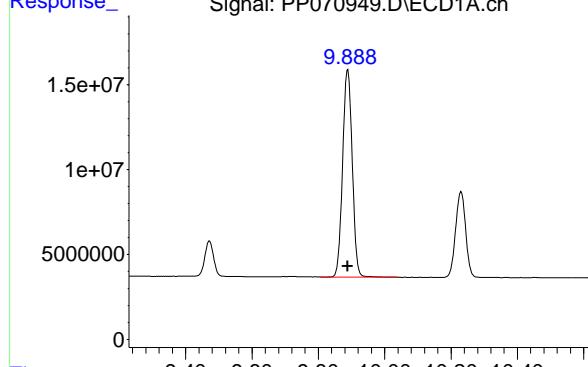

#45 AR-1268-5

R.T.: 8.595 min  
Delta R.T.: -0.001 min  
Instrument: ECD\_P  
Response: 175808654  
Conc: 485.84 ng/ml

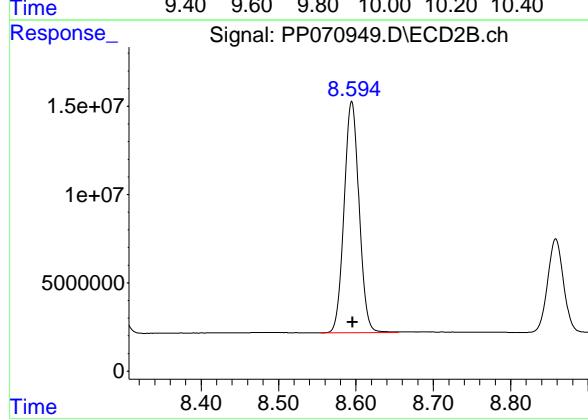



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 09:46 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-2 (2)	4.80	4.80	4.70	4.90	0.00
Aroclor-1016-3 (3)	4.86	4.86	4.76	4.96	0.00
Aroclor-1016-4 (4)	4.98	4.98	4.88	5.08	0.00
Aroclor-1016-5 (5)	5.24	5.24	5.14	5.34	0.00
Aroclor-1260-1 (1)	6.28	6.28	6.18	6.38	0.00
Aroclor-1260-2 (2)	6.47	6.47	6.37	6.57	0.00
Aroclor-1260-3 (3)	6.84	6.84	6.74	6.94	0.00
Aroclor-1260-4 (4)	7.10	7.10	7.00	7.20	0.00
Aroclor-1260-5 (5)	7.34	7.34	7.24	7.44	0.00
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.74	8.75	8.65	8.85	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 09:46 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2 (2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3 (3)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-4 (4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5 (5)	5.22	5.22	5.12	5.32	0.00
Aroclor-1260-1 (1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3 (3)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.69	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR1 ID: 0.32 (mm) Init. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL01 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110263.D Time Analyzed: 09:46

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.784	4.685	4.885	533.050	500.000	6.6
Aroclor-1016-2	4.803	4.704	4.904	532.950	500.000	6.6
Aroclor-1016-3	4.860	4.761	4.961	534.220	500.000	6.8
Aroclor-1016-4	4.980	4.881	5.081	533.580	500.000	6.7
Aroclor-1016-5	5.238	5.139	5.339	534.560	500.000	6.9
Aroclor-1260-1	6.279	6.180	6.380	540.840	500.000	8.2
Aroclor-1260-2	6.467	6.369	6.569	507.690	500.000	1.5
Aroclor-1260-3	6.835	6.737	6.937	498.120	500.000	-0.4
Aroclor-1260-4	7.096	6.998	7.198	486.870	500.000	-2.6
Aroclor-1260-5	7.337	7.239	7.439	480.250	500.000	-4.0
Decachlorobiphenyl	8.742	8.645	8.845	57.530	50.000	15.1
Tetrachloro-m-xylene	3.692	3.592	3.792	53.720	50.000	7.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR2 ID: 0.32 (mm) Init. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL01 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110263.D Time Analyzed: 09:46

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.769	4.672	4.872	509.410	500.000	1.9
Aroclor-1016-2	4.788	4.691	4.891	506.900	500.000	1.4
Aroclor-1016-3	4.964	4.867	5.067	511.350	500.000	2.3
Aroclor-1016-4	5.005	4.909	5.109	504.600	500.000	0.9
Aroclor-1016-5	5.219	5.122	5.322	510.930	500.000	2.2
Aroclor-1260-1	6.250	6.155	6.355	495.180	500.000	-1.0
Aroclor-1260-2	6.438	6.342	6.542	487.390	500.000	-2.5
Aroclor-1260-3	6.591	6.495	6.695	473.050	500.000	-5.4
Aroclor-1260-4	7.062	6.967	7.167	467.970	500.000	-6.4
Aroclor-1260-5	7.302	7.207	7.407	455.220	500.000	-9.0
Decachlorobiphenyl	8.690	8.596	8.796	48.910	50.000	-2.2
Tetrachloro-m-xylene	3.687	3.590	3.790	52.660	50.000	5.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110263.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 09:46  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 12:29:19 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.687	489.0E6	276.2E6	53.724	52.660
2) SA Decachlor...	8.742	8.690	442.3E6	118.7E6	57.530	48.907

Target Compounds

3) L1 AR-1016-1	4.784	4.769	179.4E6	93351070	533.053	509.405
4) L1 AR-1016-2	4.803	4.788	247.1E6	132.6E6	532.949	506.901
5) L1 AR-1016-3	4.860	4.964	171.3E6	72498019	534.221	511.346
6) L1 AR-1016-4	4.980	5.005	134.8E6	59506839	533.582	504.596
7) L1 AR-1016-5	5.238	5.219	146.9E6	78129978	534.558	510.925
31) L7 AR-1260-1	6.279	6.250	254.9E6	126.5E6	540.836	495.179
32) L7 AR-1260-2	6.467	6.438	302.3E6	146.4E6	507.691	487.393
33) L7 AR-1260-3	6.835	6.591	241.7E6	136.7E6	498.121	473.054
34) L7 AR-1260-4	7.096	7.062	206.5E6	100.7E6	486.872	467.969
35) L7 AR-1260-5	7.337	7.302	502.3E6	227.0E6	480.254	455.222



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110263.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 09:46  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 AR1660CCC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 12:29:19 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

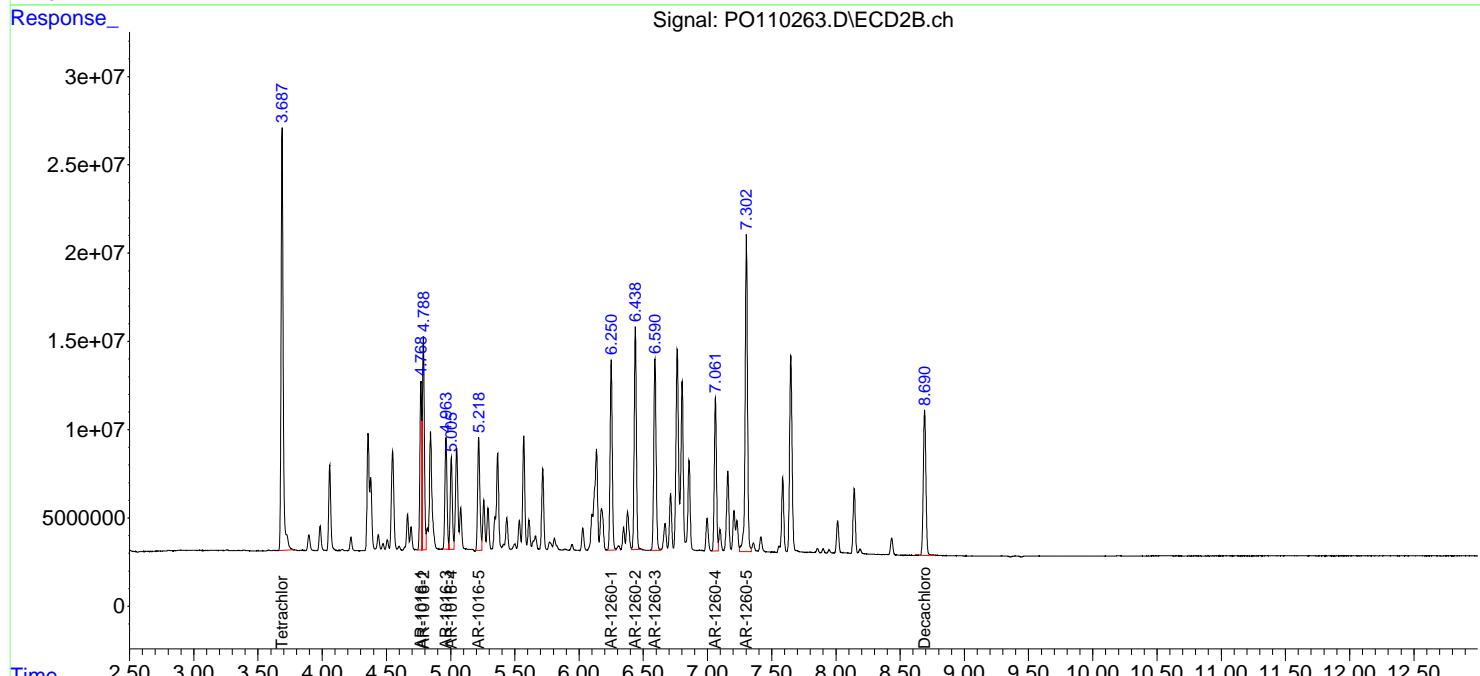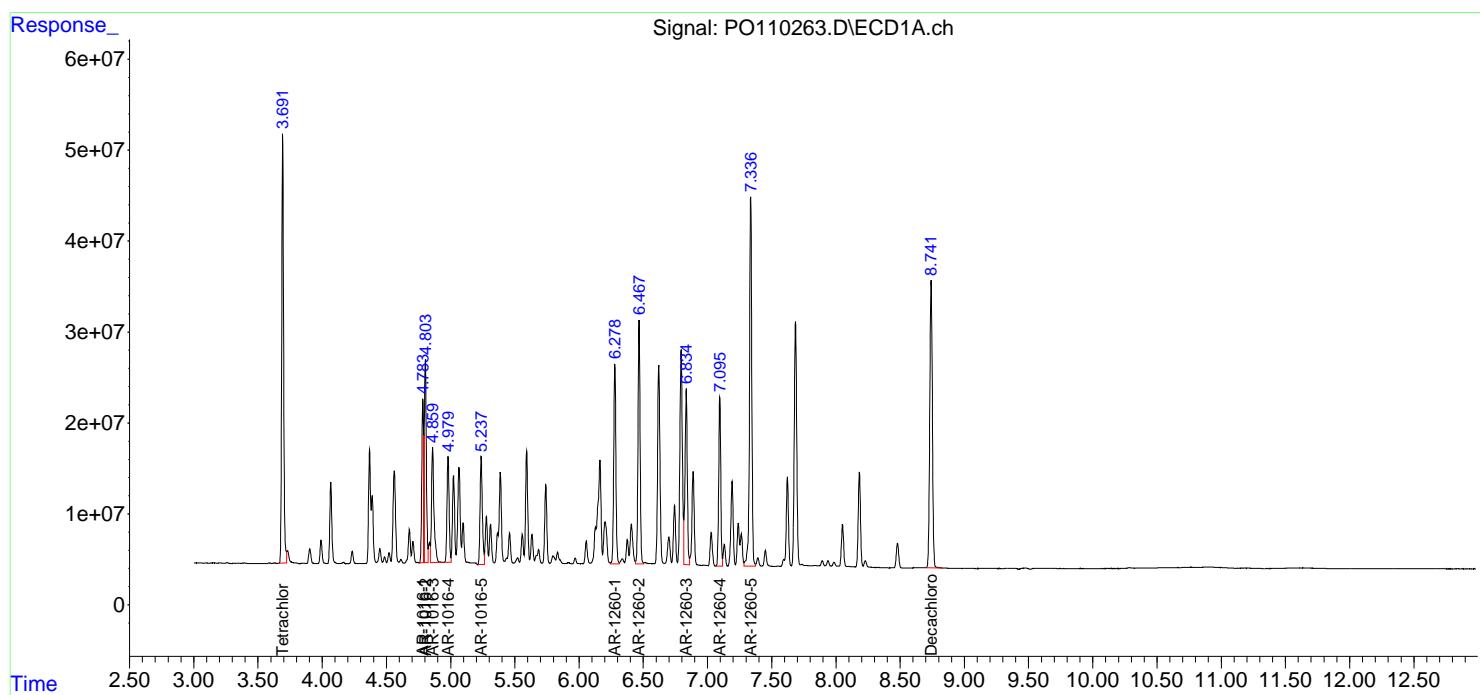

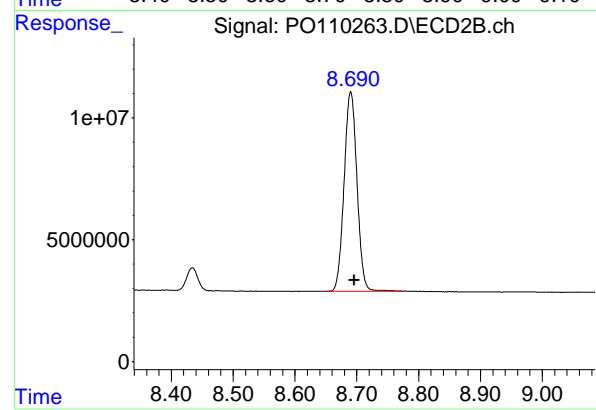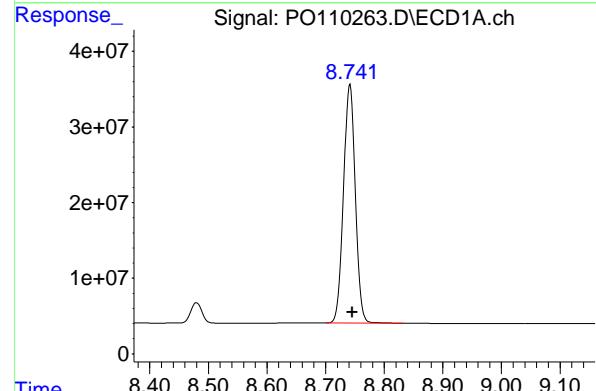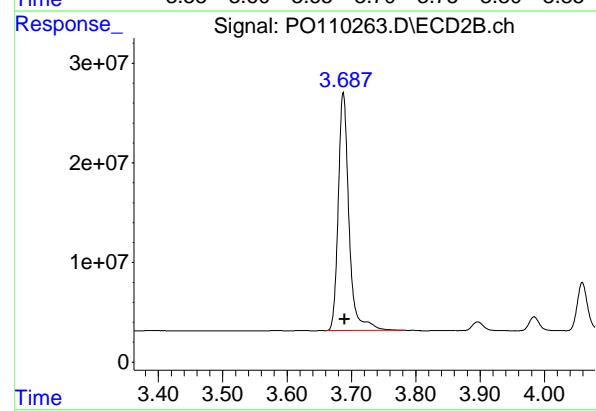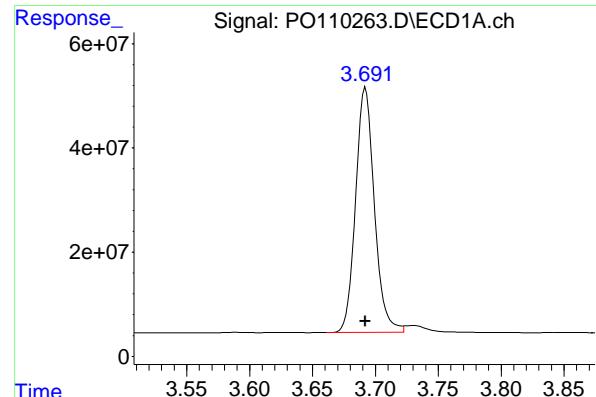

## #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
 Delta R.T.: 0.000 min  
 Response: 488973455 ECD\_O  
 Conc: 53.72 ng/ml ClientSampleId : AR1660CCC500

## #1 Tetrachloro-m-xylene





R.T.: 3.687 min  
 Delta R.T.: -0.002 min  
 Response: 276154148 Conc: 52.66 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.742 min  
 Delta R.T.: -0.004 min  
 Response: 442329479 Conc: 57.53 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.690 min  
 Delta R.T.: -0.006 min  
 Response: 118652560 Conc: 48.91 ng/ml

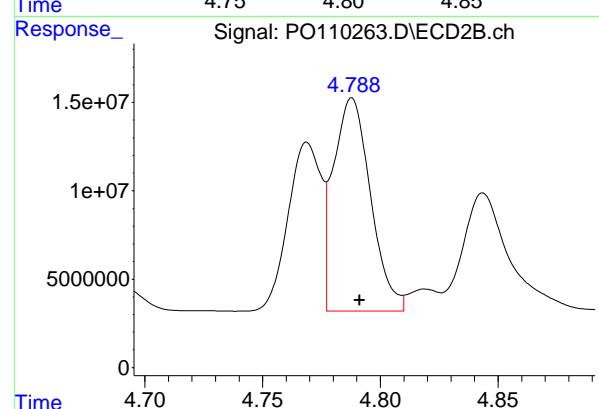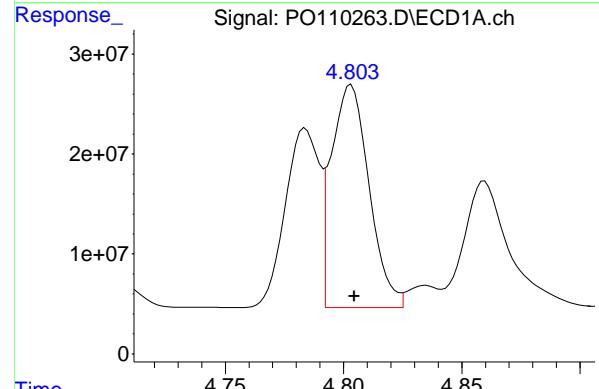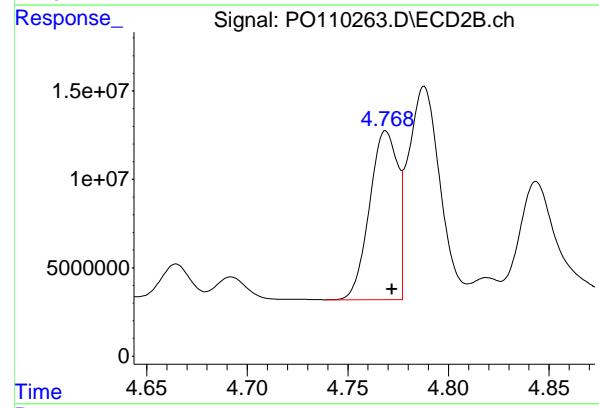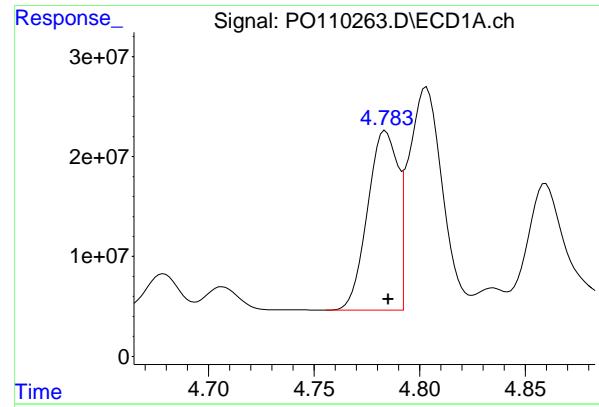

#3 AR-1016-1

R.T.: 4.784 min  
 Delta R.T.: -0.001 min  
 Instrument: ECD\_O  
 Response: 179395675  
 Conc: 533.05 ng/ml  
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.769 min  
 Delta R.T.: -0.003 min  
 Response: 93351070  
 Conc: 509.41 ng/ml

#4 AR-1016-2

R.T.: 4.803 min  
 Delta R.T.: -0.001 min  
 Response: 247120791  
 Conc: 532.95 ng/ml

#4 AR-1016-2

R.T.: 4.788 min  
 Delta R.T.: -0.003 min  
 Response: 132556824  
 Conc: 506.90 ng/ml

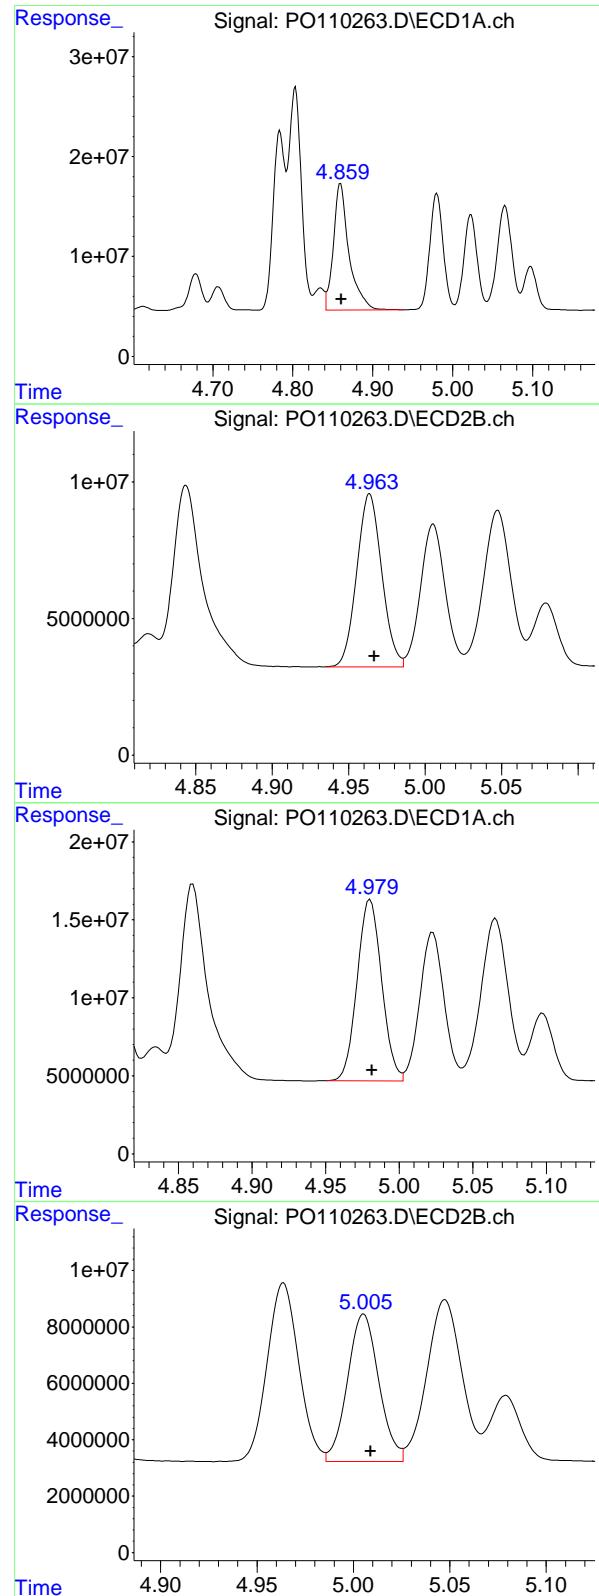

#5 AR-1016-3

R.T.: 4.860 min  
 Delta R.T.: -0.001 min  
 Response: 171263953  
 Conc: 534.22 ng/ml

Instrument: ECD\_O  
 ClientSampleId : AR1660CCC500

#5 AR-1016-3



R.T.: 4.964 min  
 Delta R.T.: -0.003 min  
 Response: 72498019  
 Conc: 511.35 ng/ml

#6 AR-1016-4

R.T.: 4.980 min  
 Delta R.T.: -0.001 min  
 Response: 134830395  
 Conc: 533.58 ng/ml

#6 AR-1016-4

R.T.: 5.005 min  
 Delta R.T.: -0.004 min  
 Response: 59506839  
 Conc: 504.60 ng/ml

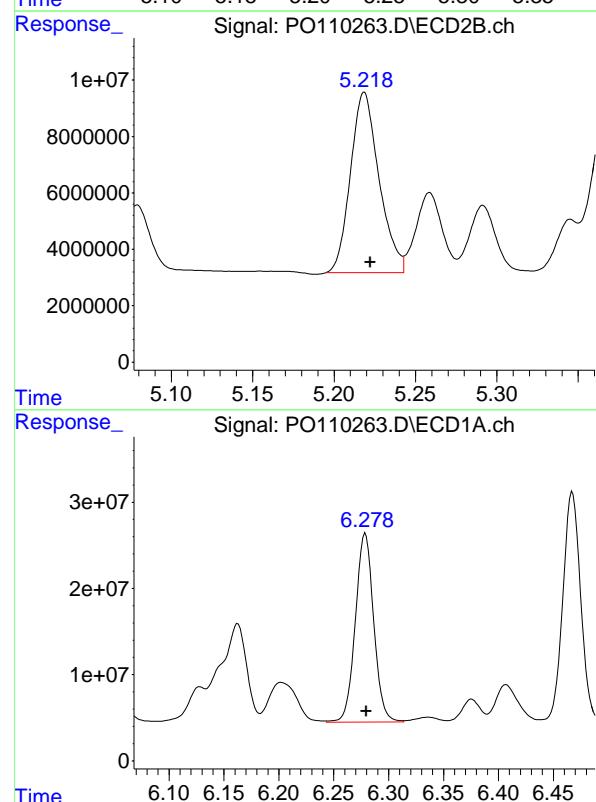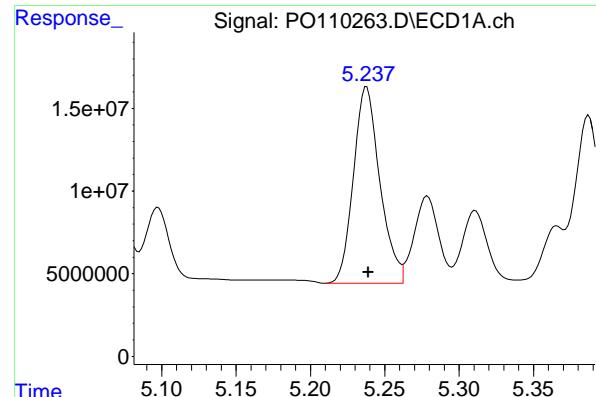

#7 AR-1016-5

R.T.: 5.238 min  
 Delta R.T.: -0.001 min  
 Response: 146932389  
 Conc: 534.56 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId :** AR1660CCC500

#7 AR-1016-5


R.T.: 5.219 min  
 Delta R.T.: -0.004 min  
 Response: 78129978  
 Conc: 510.93 ng/ml

#31 AR-1260-1

R.T.: 6.279 min  
 Delta R.T.: 0.000 min  
 Response: 254923351  
 Conc: 540.84 ng/ml

#31 AR-1260-1

R.T.: 6.250 min  
 Delta R.T.: -0.005 min  
 Response: 126489343  
 Conc: 495.18 ng/ml

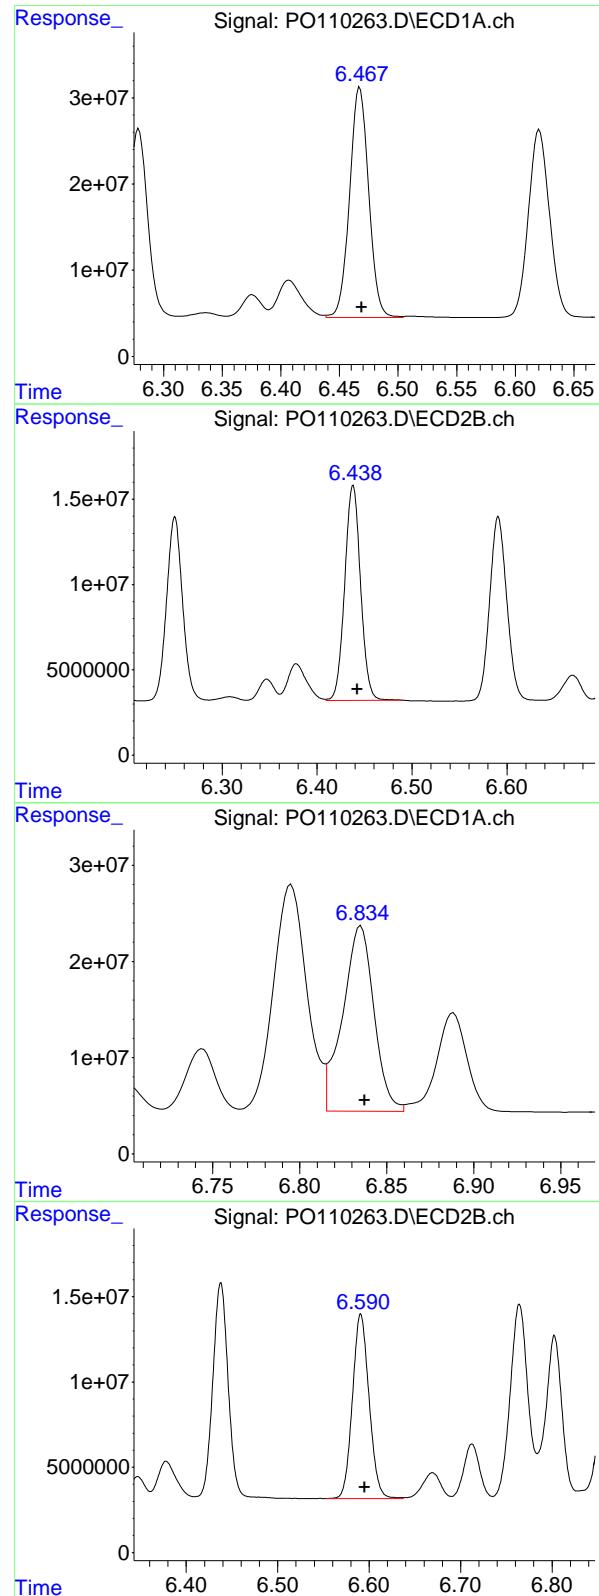

#32 AR-1260-2

R.T.: 6.467 min  
 Delta R.T.: -0.002 min  
 Response: 302339417  
 Conc: 507.69 ng/ml  
 Instrument: ECD\_O  
 ClientSampleId : AR1660CCC500

#32 AR-1260-2


R.T.: 6.438 min  
 Delta R.T.: -0.005 min  
 Response: 146357167  
 Conc: 487.39 ng/ml

#33 AR-1260-3

R.T.: 6.835 min  
 Delta R.T.: -0.002 min  
 Response: 241738750  
 Conc: 498.12 ng/ml

#33 AR-1260-3

R.T.: 6.591 min  
 Delta R.T.: -0.004 min  
 Response: 136704083  
 Conc: 473.05 ng/ml

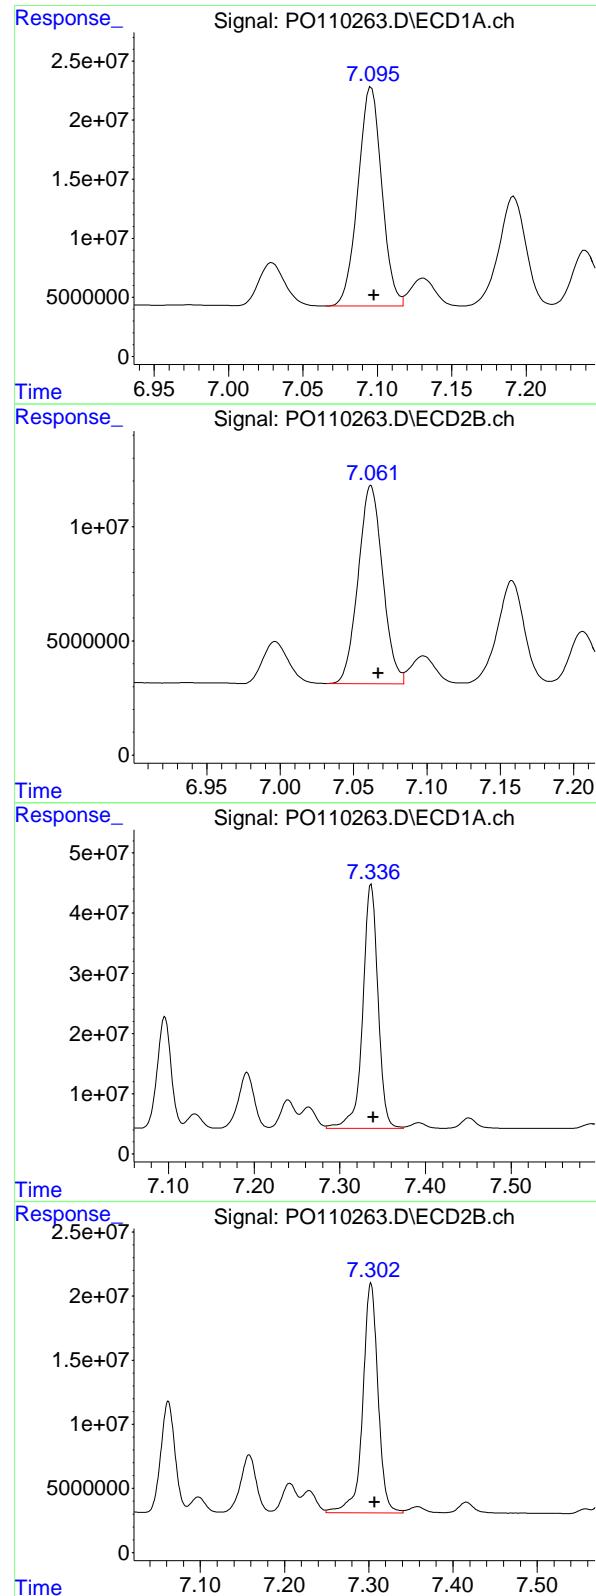

#34 AR-1260-4

R.T.: 7.096 min  
 Delta R.T.: -0.002 min  
 Response: 206515387  
 Conc: 486.87 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#34 AR-1260-4

R.T.: 7.062 min  
 Delta R.T.: -0.005 min  
 Response: 100650011  
 Conc: 467.97 ng/ml

#35 AR-1260-5

R.T.: 7.337 min  
 Delta R.T.: -0.003 min  
 Response: 502271562  
 Conc: 480.25 ng/ml

#35 AR-1260-5

R.T.: 7.302 min  
 Delta R.T.: -0.005 min  
 Response: 227017361  
 Conc: 455.22 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 17:14 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-2 (2)	4.80	4.80	4.70	4.90	0.00
Aroclor-1016-3 (3)	4.86	4.86	4.76	4.96	0.00
Aroclor-1016-4 (4)	4.98	4.98	4.88	5.08	0.00
Aroclor-1016-5 (5)	5.24	5.24	5.14	5.34	0.00
Aroclor-1260-1 (1)	6.28	6.28	6.18	6.38	0.00
Aroclor-1260-2 (2)	6.47	6.47	6.37	6.57	0.00
Aroclor-1260-3 (3)	6.83	6.84	6.74	6.94	0.01
Aroclor-1260-4 (4)	7.09	7.10	7.00	7.20	0.01
Aroclor-1260-5 (5)	7.34	7.34	7.24	7.44	0.00
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.74	8.75	8.65	8.85	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 17:14 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2 (2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3 (3)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-4 (4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5 (5)	5.22	5.22	5.12	5.32	0.00
Aroclor-1260-1 (1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3 (3)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.69	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR1 ID: 0.32 (mm) Init. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL02 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110278.D Time Analyzed: 17:14

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.782	4.685	4.885	511.900	500.000	2.4
Aroclor-1016-2	4.802	4.704	4.904	513.800	500.000	2.8
Aroclor-1016-3	4.858	4.761	4.961	513.560	500.000	2.7
Aroclor-1016-4	4.979	4.881	5.081	505.500	500.000	1.1
Aroclor-1016-5	5.236	5.139	5.339	483.610	500.000	-3.3
Aroclor-1260-1	6.276	6.180	6.380	516.970	500.000	3.4
Aroclor-1260-2	6.466	6.369	6.569	486.490	500.000	-2.7
Aroclor-1260-3	6.834	6.737	6.937	450.780	500.000	-9.8
Aroclor-1260-4	7.094	6.998	7.198	442.100	500.000	-11.6
Aroclor-1260-5	7.336	7.239	7.439	429.820	500.000	-14.0
Decachlorobiphenyl	8.741	8.645	8.845	52.440	50.000	4.9
Tetrachloro-m-xylene	3.691	3.592	3.792	52.070	50.000	4.1



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR2 ID: 0.32 (mm) Init. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL02 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110278.D Time Analyzed: 17:14

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.769	4.672	4.872	501.230	500.000	0.2
Aroclor-1016-2	4.788	4.691	4.891	505.970	500.000	1.2
Aroclor-1016-3	4.964	4.867	5.067	506.650	500.000	1.3
Aroclor-1016-4	5.006	4.909	5.109	501.000	500.000	0.2
Aroclor-1016-5	5.218	5.122	5.322	500.710	500.000	0.1
Aroclor-1260-1	6.250	6.155	6.355	459.750	500.000	-8.1
Aroclor-1260-2	6.438	6.342	6.542	450.220	500.000	-10.0
Aroclor-1260-3	6.591	6.495	6.695	435.550	500.000	-12.9
Aroclor-1260-4	7.063	6.967	7.167	432.750	500.000	-13.5
Aroclor-1260-5	7.303	7.207	7.407	419.150	500.000	-16.2
Decachlorobiphenyl	8.691	8.596	8.796	46.440	50.000	-7.1
Tetrachloro-m-xylene	3.688	3.590	3.790	52.230	50.000	4.5

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110278.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 17:14  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 17:33:50 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	3.691	3.688	473.9E6	273.9E6	52.066	52.232
2) SA Decachloro...	8.741	8.691	403.2E6	112.7E6	52.443	46.444

Target Compounds

3) L1 AR-1016-1	4.782	4.769	172.3E6	91853593	511.903	501.234
4) L1 AR-1016-2	4.802	4.788	238.2E6	132.3E6	513.796	505.969
5) L1 AR-1016-3	4.858	4.964	164.6E6	71832300	513.560	506.651
6) L1 AR-1016-4	4.979	5.006	127.7E6	59082308	505.504	500.996
7) L1 AR-1016-5	5.236	5.218	132.9E6	76567933	483.609	500.710
31) L7 AR-1260-1	6.276	6.250	243.7E6	117.4E6	516.972	459.747
32) L7 AR-1260-2	6.466	6.438	289.7E6	135.2E6	486.489	450.225
33) L7 AR-1260-3	6.834	6.591	218.8E6	125.9E6	450.781	435.554
34) L7 AR-1260-4	7.094	7.063	187.5E6	93074613	442.104	432.747
35) L7 AR-1260-5	7.336	7.303	449.5E6	209.0E6	429.819	419.151



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\PO040725\  
 Data File : PO110278.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 17:14  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 AR1660CCC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 17:33:50 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

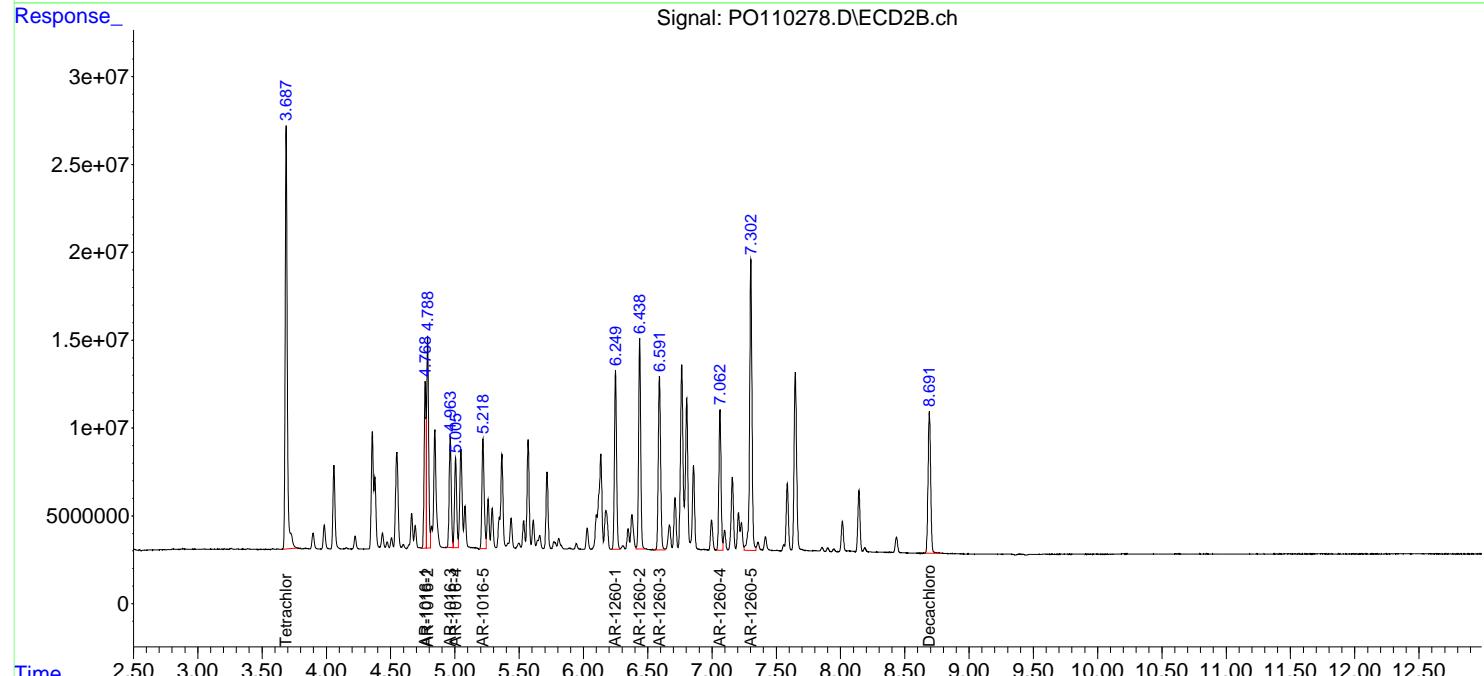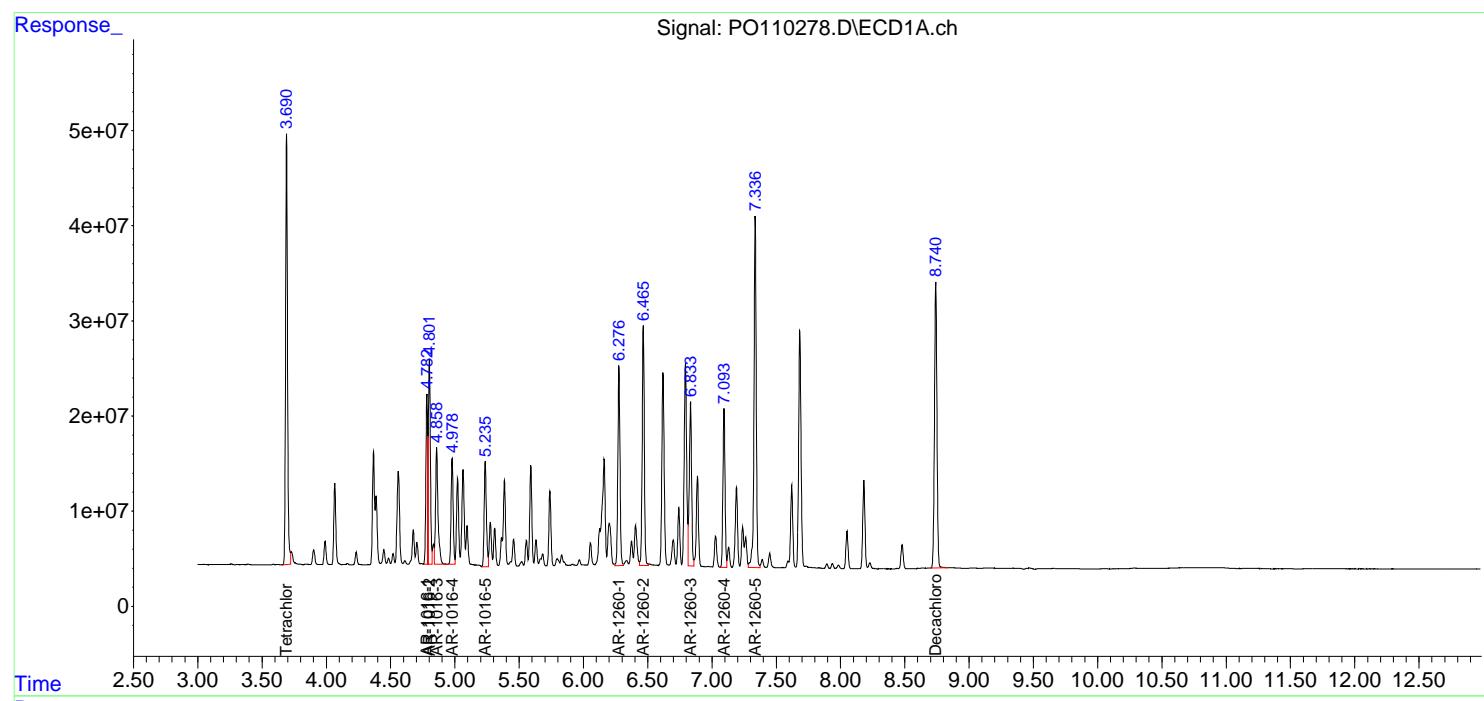

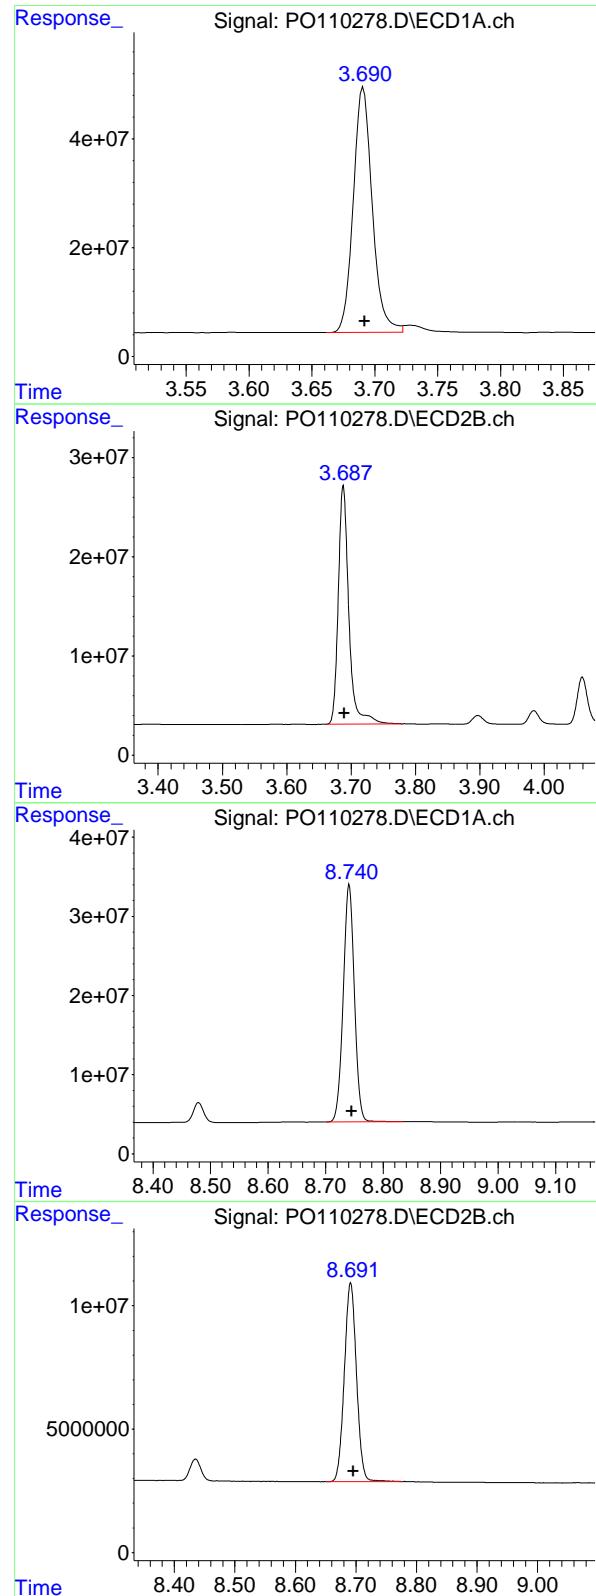

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
Delta R.T.: -0.001 min  
Response: 473883144 ECD\_O  
Conc: 52.07 ng/ml Client SampleId : AR1660CCC500

## #1 Tetrachloro-m-xylene


R.T.: 3.688 min  
Delta R.T.: -0.002 min  
Response: 273908061  
Conc: 52.23 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.741 min  
Delta R.T.: -0.004 min  
Response: 403219619  
Conc: 52.44 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
Delta R.T.: -0.005 min  
Response: 112677778  
Conc: 46.44 ng/ml

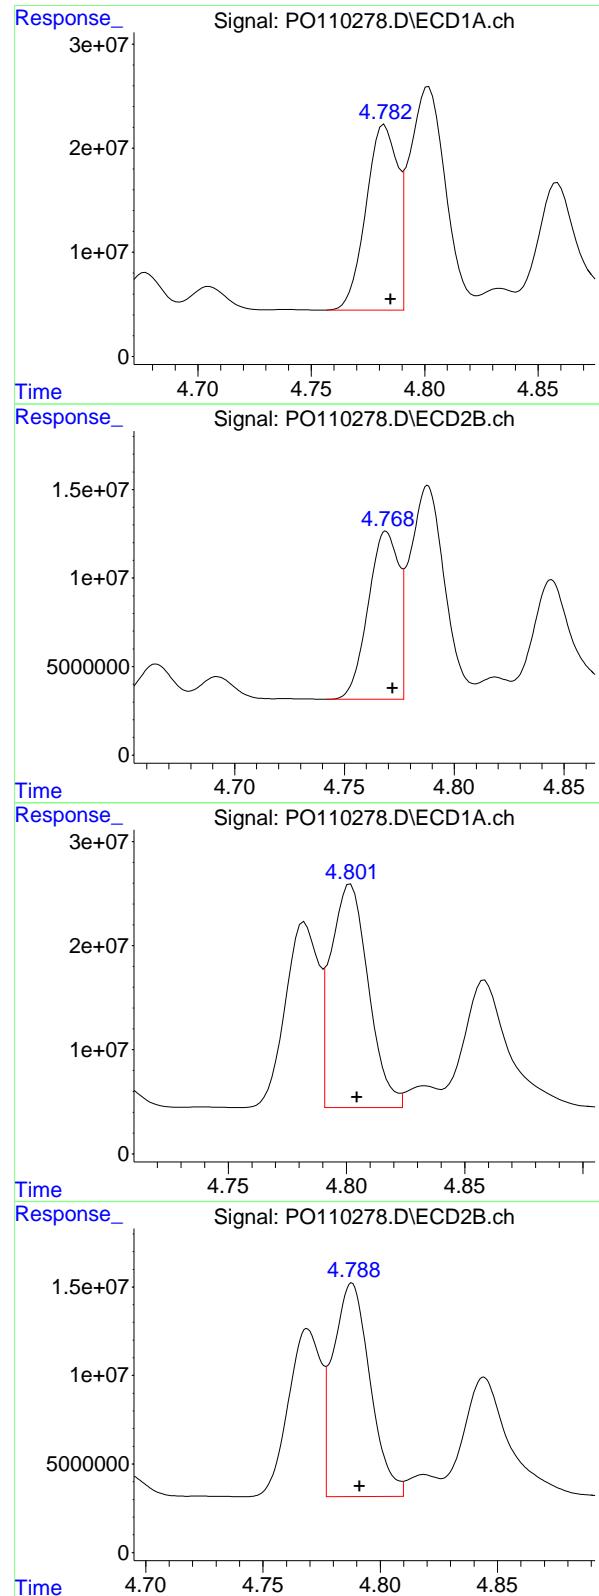

#3 AR-1016-1

R.T.: 4.782 min  
 Delta R.T.: -0.003 min  
 Response: 172277908  
 Conc: 511.90 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.769 min  
 Delta R.T.: -0.003 min  
 Response: 91853593  
 Conc: 501.23 ng/ml

#4 AR-1016-2

R.T.: 4.802 min  
 Delta R.T.: -0.003 min  
 Response: 238239899  
 Conc: 513.80 ng/ml

#4 AR-1016-2

R.T.: 4.788 min  
 Delta R.T.: -0.003 min  
 Response: 132313036  
 Conc: 505.97 ng/ml

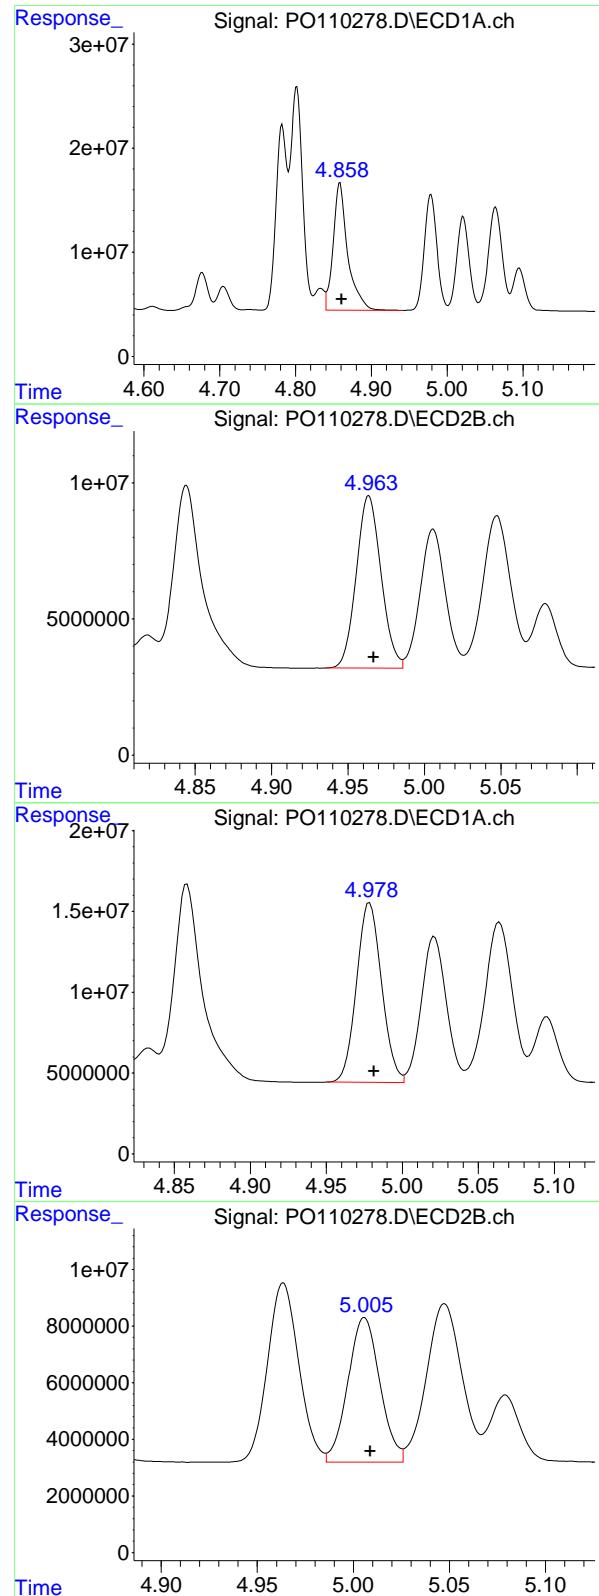

#5 AR-1016-3

R.T.: 4.858 min  
 Delta R.T.: -0.002 min  
 Response: 164640078  
 Conc: 513.56 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId :** AR1660CCC500

#5 AR-1016-3



R.T.: 4.964 min  
 Delta R.T.: -0.003 min  
 Response: 71832300  
 Conc: 506.65 ng/ml

#6 AR-1016-4

R.T.: 4.979 min  
 Delta R.T.: -0.003 min  
 Response: 127735566  
 Conc: 505.50 ng/ml

#6 AR-1016-4

R.T.: 5.006 min  
 Delta R.T.: -0.003 min  
 Response: 59082308  
 Conc: 501.00 ng/ml

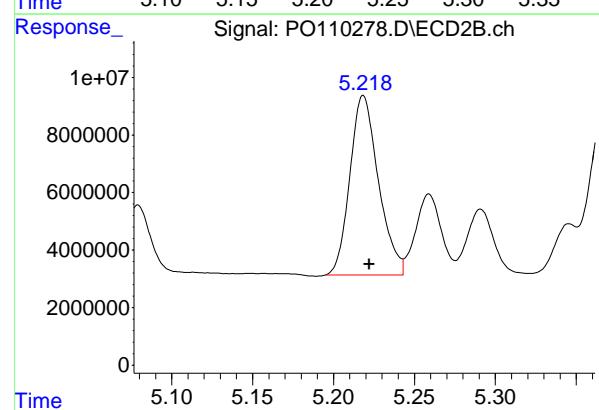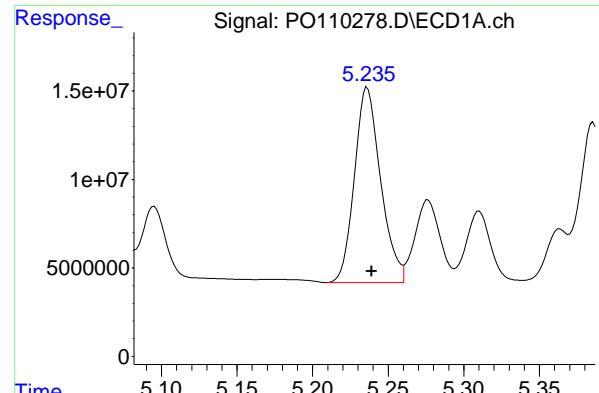

#7 AR-1016-5

R.T.: 5.236 min  
 Delta R.T.: -0.003 min  
 Response: 132928200  
 Conc: 483.61 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#7 AR-1016-5





R.T.: 5.218 min  
 Delta R.T.: -0.004 min  
 Response: 76567933  
 Conc: 500.71 ng/ml

#31 AR-1260-1

R.T.: 6.276 min  
 Delta R.T.: -0.003 min  
 Response: 243675158  
 Conc: 516.97 ng/ml

#31 AR-1260-1

R.T.: 6.250 min  
 Delta R.T.: -0.005 min  
 Response: 117438638  
 Conc: 459.75 ng/ml

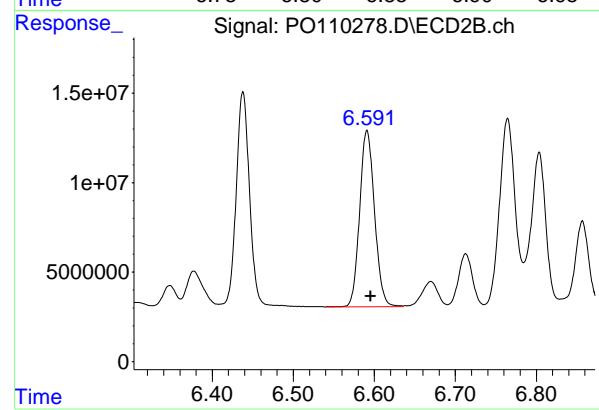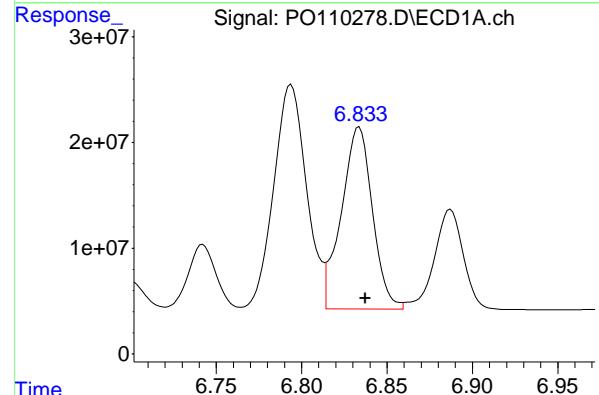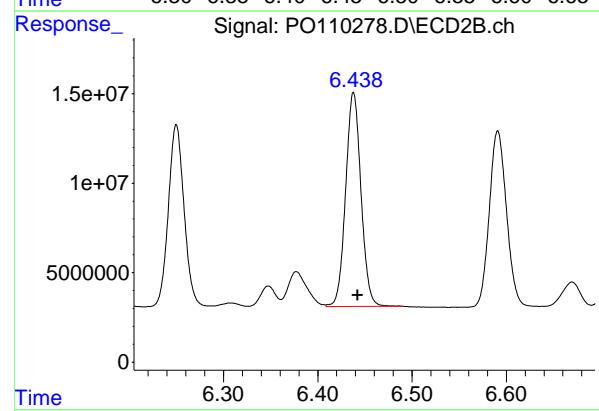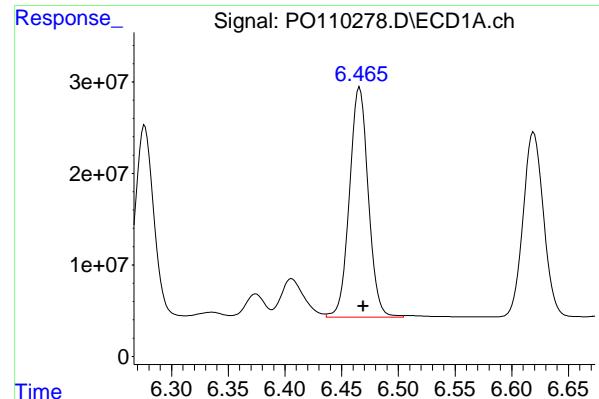

#32 AR-1260-2

R.T.: 6.466 min  
 Delta R.T.: -0.003 min  
 Instrument: ECD\_O  
 Response: 289713640  
 Conc: 486.49 ng/ml  
 ClientSampleId: AR1660CCC500

#32 AR-1260-2



R.T.: 6.438 min  
 Delta R.T.: -0.005 min  
 Response: 135195944  
 Conc: 450.22 ng/ml

#33 AR-1260-3

R.T.: 6.834 min  
 Delta R.T.: -0.004 min  
 Response: 218764620  
 Conc: 450.78 ng/ml

#33 AR-1260-3

R.T.: 6.591 min  
 Delta R.T.: -0.004 min  
 Response: 125867255  
 Conc: 435.55 ng/ml

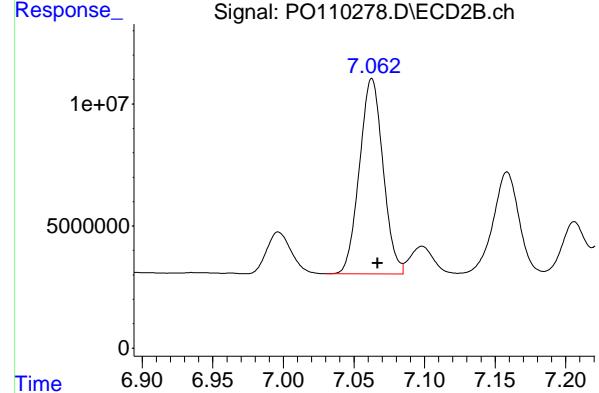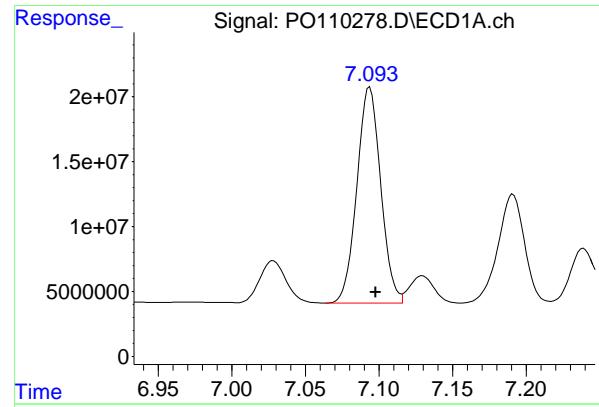

#34 AR-1260-4

R.T.: 7.094 min  
 Delta R.T.: -0.004 min  
 Response: 187526171  
 Conc: 442.10 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#34 AR-1260-4

R.T.: 7.063 min  
 Delta R.T.: -0.004 min  
 Response: 93074613  
 Conc: 432.75 ng/ml

#35 AR-1260-5

R.T.: 7.336 min  
 Delta R.T.: -0.003 min  
 Response: 449524286  
 Conc: 429.82 ng/ml

#35 AR-1260-5

R.T.: 7.303 min  
 Delta R.T.: -0.004 min  
 Response: 209028955  
 Conc: 419.15 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 21:27 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-2 (2)	4.80	4.80	4.70	4.90	0.00
Aroclor-1016-3 (3)	4.86	4.86	4.76	4.96	0.00
Aroclor-1016-4 (4)	4.98	4.98	4.88	5.08	0.00
Aroclor-1016-5 (5)	5.24	5.24	5.14	5.34	0.00
Aroclor-1260-1 (1)	6.28	6.28	6.18	6.38	0.00
Aroclor-1260-2 (2)	6.47	6.47	6.37	6.57	0.00
Aroclor-1260-3 (3)	6.83	6.84	6.74	6.94	0.01
Aroclor-1260-4 (4)	7.09	7.10	7.00	7.20	0.01
Aroclor-1260-5 (5)	7.34	7.34	7.24	7.44	0.00
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.74	8.75	8.65	8.85	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 21:27 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2 (2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3 (3)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-4 (4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5 (5)	5.22	5.22	5.12	5.32	0.00
Aroclor-1260-1 (1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3 (3)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.69	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR1 ID: 0.32 (mm) Init. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL03 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110286.D Time Analyzed: 21:27

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.783	4.685	4.885	528.320	500.000	5.7
Aroclor-1016-2	4.802	4.704	4.904	526.450	500.000	5.3
Aroclor-1016-3	4.858	4.761	4.961	529.370	500.000	5.9
Aroclor-1016-4	4.979	4.881	5.081	518.990	500.000	3.8
Aroclor-1016-5	5.236	5.139	5.339	496.090	500.000	-0.8
Aroclor-1260-1	6.277	6.180	6.380	550.160	500.000	10.0
Aroclor-1260-2	6.466	6.369	6.569	508.400	500.000	1.7
Aroclor-1260-3	6.834	6.737	6.937	481.740	500.000	-3.7
Aroclor-1260-4	7.094	6.998	7.198	471.490	500.000	-5.7
Aroclor-1260-5	7.336	7.239	7.439	462.920	500.000	-7.4
Decachlorobiphenyl	8.740	8.645	8.845	54.690	50.000	9.4
Tetrachloro-m-xylene	3.691	3.592	3.792	53.480	50.000	7.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR2 ID: 0.32 (mm) Init. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL03 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110286.D Time Analyzed: 21:27

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.769	4.672	4.872	512.420	500.000	2.5
Aroclor-1016-2	4.788	4.691	4.891	514.070	500.000	2.8
Aroclor-1016-3	4.964	4.867	5.067	515.160	500.000	3.0
Aroclor-1016-4	5.006	4.909	5.109	469.250	500.000	-6.2
Aroclor-1016-5	5.218	5.122	5.322	514.370	500.000	2.9
Aroclor-1260-1	6.251	6.155	6.355	483.370	500.000	-3.3
Aroclor-1260-2	6.439	6.342	6.542	477.180	500.000	-4.6
Aroclor-1260-3	6.591	6.495	6.695	462.160	500.000	-7.6
Aroclor-1260-4	7.063	6.967	7.167	461.970	500.000	-7.6
Aroclor-1260-5	7.303	7.207	7.407	444.510	500.000	-11.1
Decachlorobiphenyl	8.691	8.596	8.796	48.770	50.000	-2.5
Tetrachloro-m-xylene	3.688	3.590	3.790	53.150	50.000	6.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110286.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 21:27  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 AR1660CCC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 04/08/2025  
 Supervised By :mohammad ahmed 04/09/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:36:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	3.691	3.688	486.8E6	278.7E6	53.484	53.152
2) SA Decachloro...	8.740	8.691	420.5E6	118.3E6	54.690	48.766

Target Compounds

3) L1 AR-1016-1	4.783	4.769	177.8E6	93902896	528.316	512.417
4) L1 AR-1016-2	4.802	4.788	244.1E6	134.4E6	526.454	514.067
5) L1 AR-1016-3	4.858	4.964	169.7E6	73038464	529.369	515.158
6) L1 AR-1016-4	4.979	5.006	131.1E6	55338718	518.987	469.252
7) L1 AR-1016-5	5.236	5.218	136.4E6	78657229	496.086m	514.373m
31) L7 AR-1260-1	6.277	6.251	259.3E6	123.5E6	550.162	483.373
32) L7 AR-1260-2	6.466	6.439	302.8E6	143.3E6	508.402	477.179
33) L7 AR-1260-3	6.834	6.591	233.8E6	133.6E6	481.744	462.164
34) L7 AR-1260-4	7.094	7.063	200.0E6	99360275	471.486	461.972
35) L7 AR-1260-5	7.336	7.303	484.1E6	221.7E6	462.918	444.506

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\PO040725\  
 Data File : PO110286.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 21:27  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:36:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_O  
 ClientSampleId :  
 AR1660CCC500

### Manual Integrations APPROVED

Reviewed By :Yogesh Patel 04/08/2025  
 Supervised By :mohammad ahmed 04/09/2025

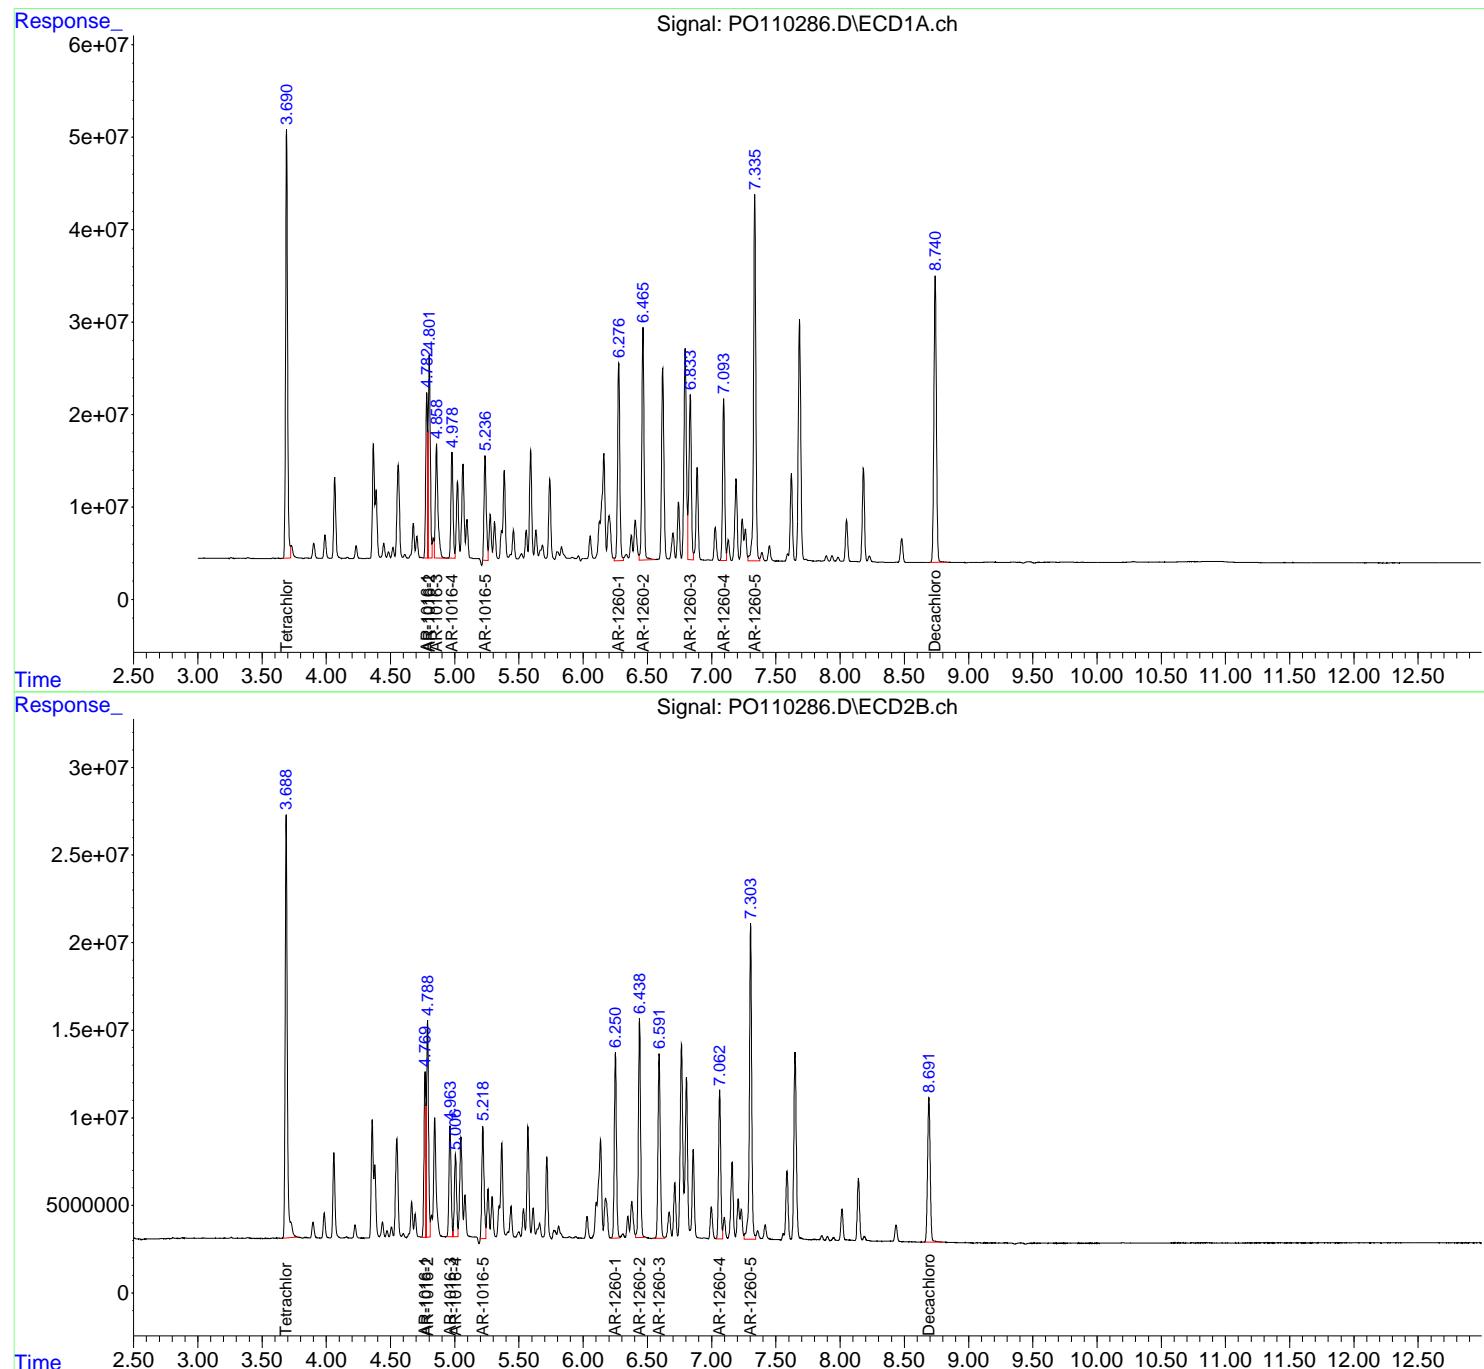

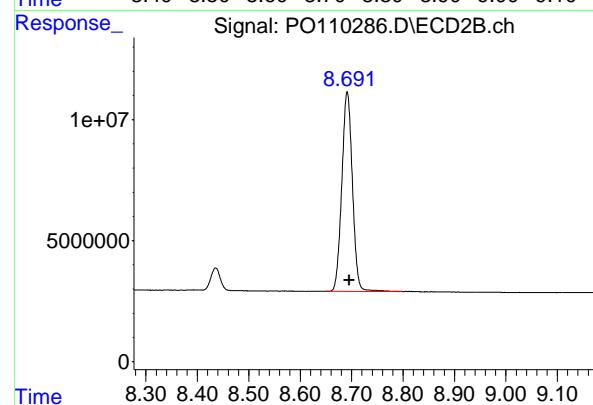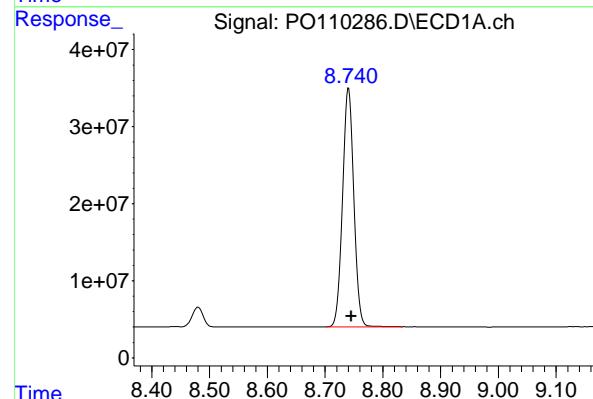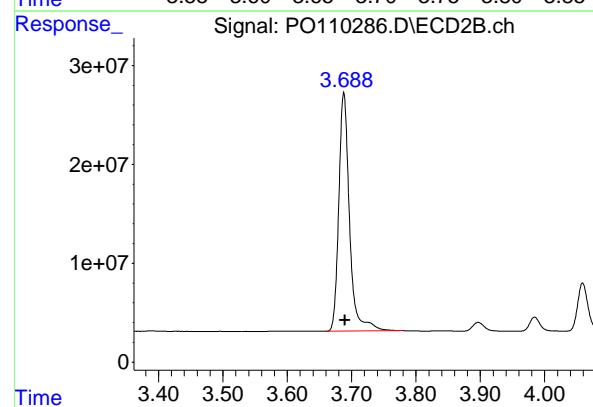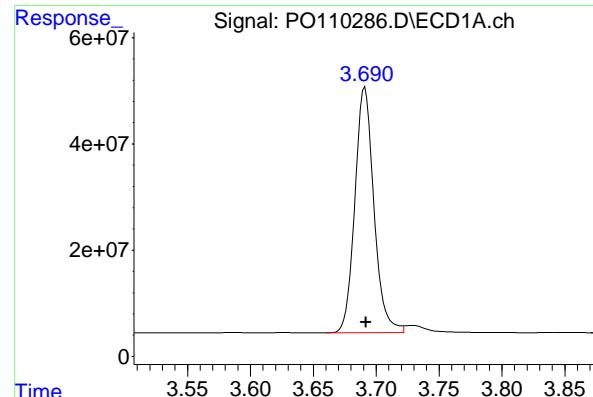

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
Delta R.T.: -0.001 min  
Instrument: ECD\_O  
Response: 486781502  
Conc: 53.48 ng/ml  
ClientSampleId : AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/08/2025  
Supervised By :mohammad ahmed 04/09/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.688 min  
Delta R.T.: -0.002 min  
Response: 278731990  
Conc: 53.15 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.740 min  
Delta R.T.: -0.005 min  
Response: 420491355  
Conc: 54.69 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
Delta R.T.: -0.004 min  
Response: 118311884  
Conc: 48.77 ng/ml

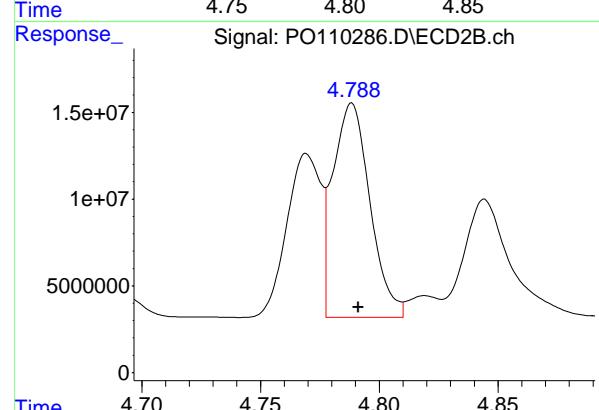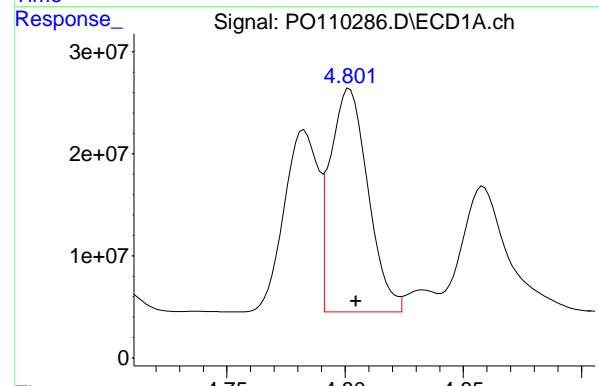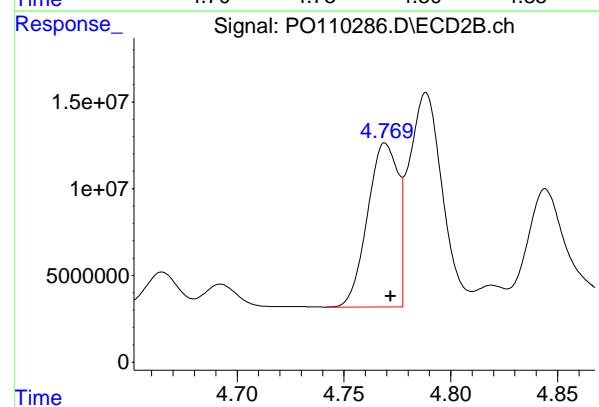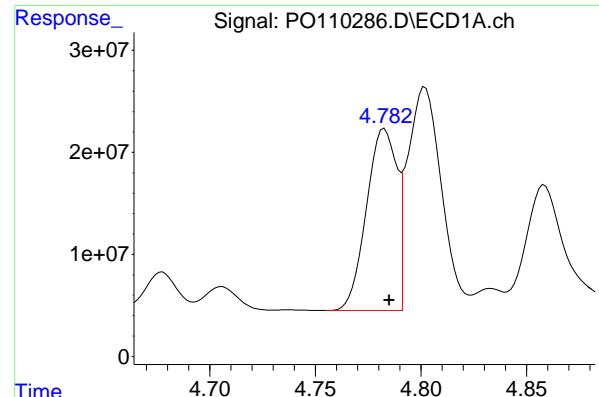

#3 AR-1016-1

R.T.: 4.783 min  
 Delta R.T.: -0.002 min  
 Response: 177801623  
 Conc: 528.32 ng/ml

Instrument: ECD\_O  
 Client SampleId : AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/08/2025  
 Supervised By :mohammad ahmed 04/09/2025

#3 AR-1016-1





R.T.: 4.769 min  
 Delta R.T.: -0.003 min  
 Response: 93902896  
 Conc: 512.42 ng/ml

#4 AR-1016-2

R.T.: 4.802 min  
 Delta R.T.: -0.003 min  
 Response: 244109403  
 Conc: 526.45 ng/ml

#4 AR-1016-2

R.T.: 4.788 min  
 Delta R.T.: -0.003 min  
 Response: 134430740  
 Conc: 514.07 ng/ml

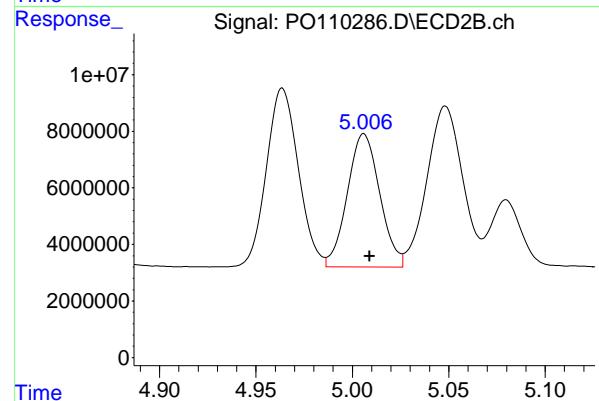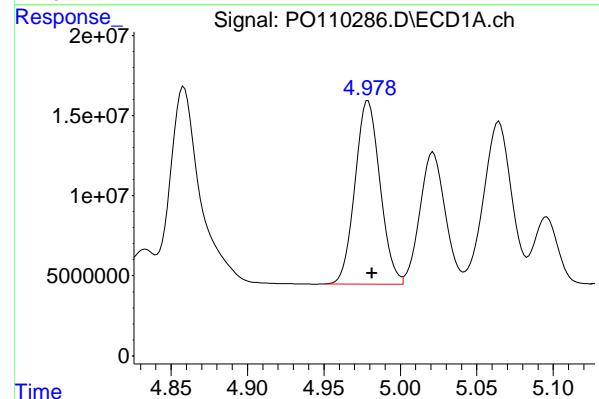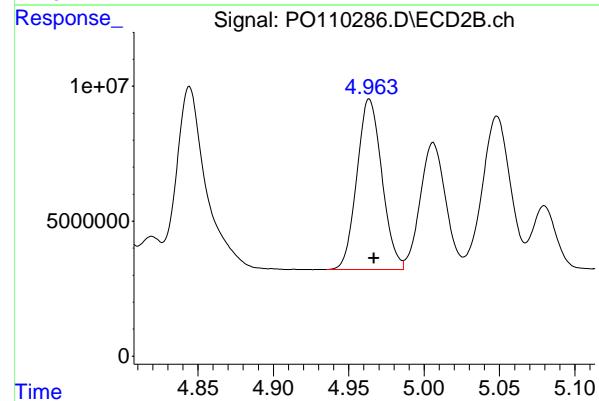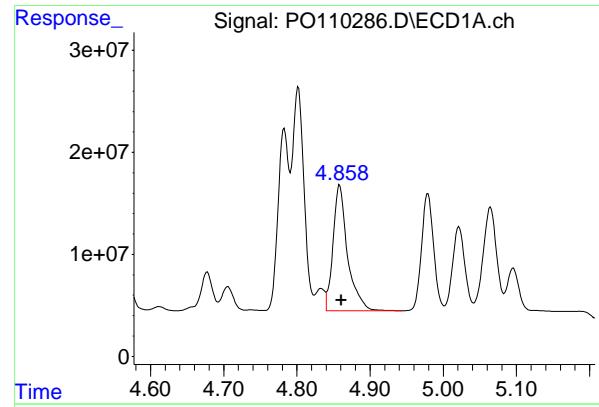

#5 AR-1016-3

R.T.: 4.858 min  
 Delta R.T.: -0.002 min  
 Response: 169708224  
 Conc: 529.37 ng/ml

Instrument: ECD\_O  
 ClientSampleId : AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/08/2025  
 Supervised By :mohammad ahmed 04/09/2025

#5 AR-1016-3





R.T.: 4.964 min  
 Delta R.T.: -0.003 min  
 Response: 73038464  
 Conc: 515.16 ng/ml

#6 AR-1016-4

R.T.: 4.979 min  
 Delta R.T.: -0.002 min  
 Response: 131142472  
 Conc: 518.99 ng/ml

#6 AR-1016-4

R.T.: 5.006 min  
 Delta R.T.: -0.003 min  
 Response: 55338718  
 Conc: 469.25 ng/ml

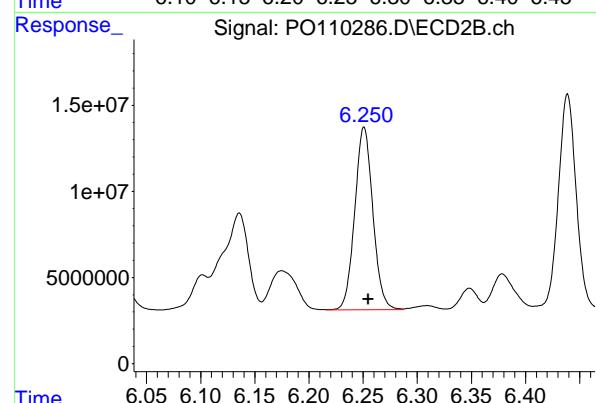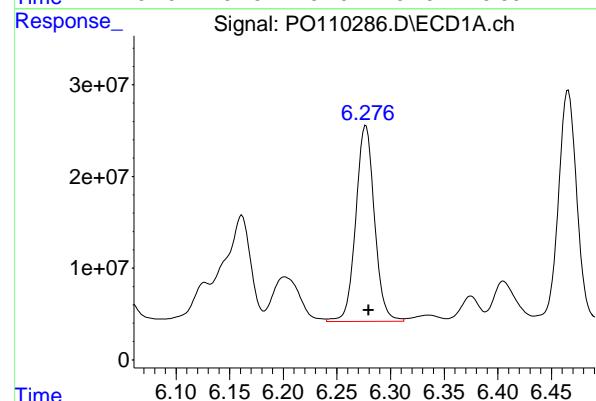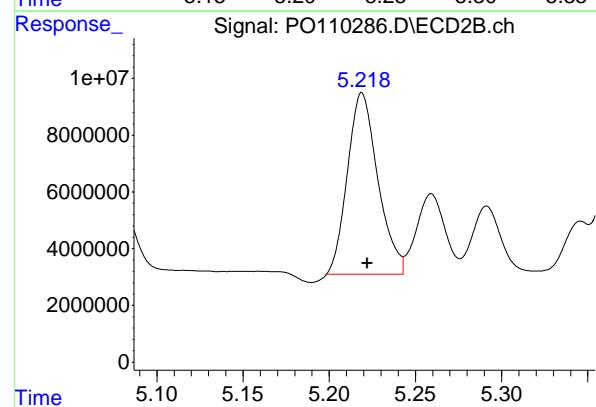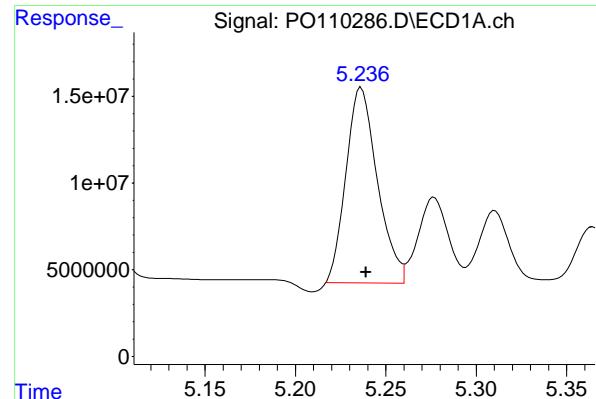

#7 AR-1016-5

R.T.: 5.236 min  
 Delta R.T.: -0.003 min  
 Response: 136357657  
 Conc: 496.09 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/08/2025  
 Supervised By :mohammad ahmed 04/09/2025

#7 AR-1016-5



R.T.: 5.218 min  
 Delta R.T.: -0.004 min  
 Response: 78657229  
 Conc: 514.37 ng/ml

#31 AR-1260-1

R.T.: 6.277 min  
 Delta R.T.: -0.003 min  
 Response: 259319565  
 Conc: 550.16 ng/ml

#31 AR-1260-1

R.T.: 6.251 min  
 Delta R.T.: -0.004 min  
 Response: 123473695  
 Conc: 483.37 ng/ml

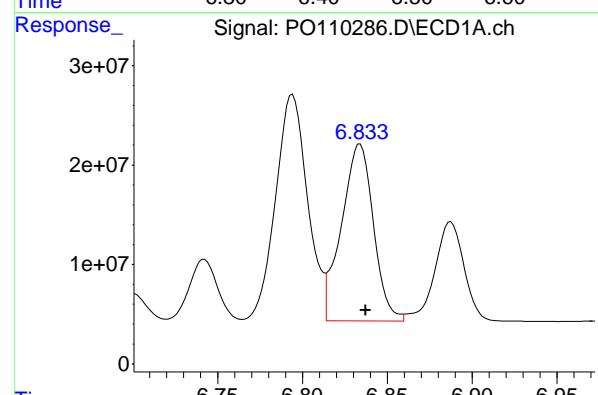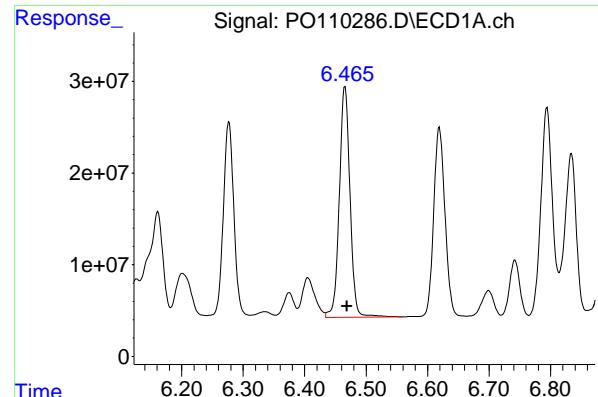

#32 AR-1260-2

R.T.: 6.466 min  
 Delta R.T.: -0.003 min  
 Response: 302763163  
 Conc: 508.40 ng/ml

Instrument: ECD\_O  
 Client Sample Id: AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/08/2025  
 Supervised By :mohammad ahmed 04/09/2025

#32 AR-1260-2


R.T.: 6.439 min  
 Delta R.T.: -0.004 min  
 Response: 143289838  
 Conc: 477.18 ng/ml

#33 AR-1260-3

R.T.: 6.834 min  
 Delta R.T.: -0.003 min  
 Response: 233791087  
 Conc: 481.74 ng/ml

#33 AR-1260-3

R.T.: 6.591 min  
 Delta R.T.: -0.004 min  
 Response: 133557256  
 Conc: 462.16 ng/ml

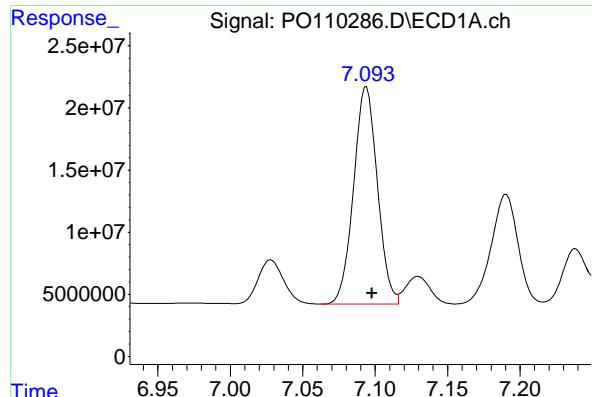


#34 AR-1260-4

R.T.: 7.094 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_O  
Response: 199989246  
Conc: 471.49 ng/ml  
ClientSampleId : AR1660CCC500


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/08/2025  
Supervised By :mohammad ahmed 04/09/2025

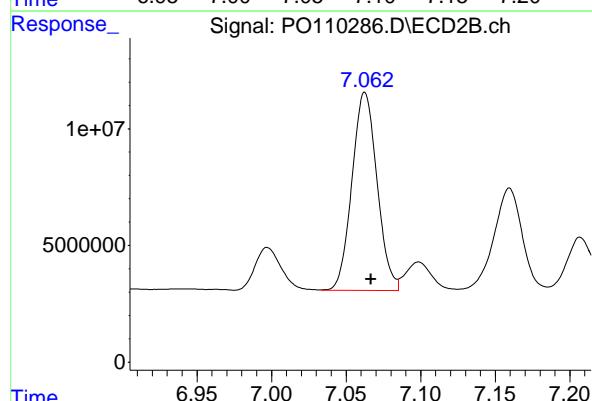


#34 AR-1260-4

R.T.: 7.063 min  
Delta R.T.: -0.004 min  
Response: 99360275  
Conc: 461.97 ng/ml

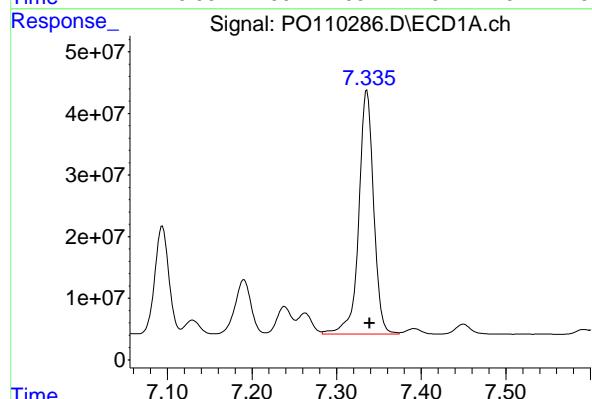

#35 AR-1260-5

R.T.: 7.336 min  
Delta R.T.: -0.004 min  
Response: 484140405  
Conc: 462.92 ng/ml

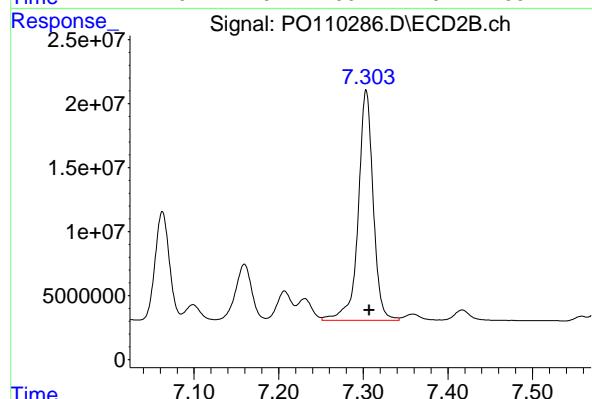

#35 AR-1260-5

R.T.: 7.303 min  
Delta R.T.: -0.004 min  
Response: 221673295  
Conc: 444.51 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/08/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 09:08 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-2 (2)	4.80	4.80	4.70	4.90	0.00
Aroclor-1016-3 (3)	4.86	4.86	4.76	4.96	0.00
Aroclor-1016-4 (4)	4.98	4.98	4.88	5.08	0.00
Aroclor-1016-5 (5)	5.24	5.24	5.14	5.34	0.00
Aroclor-1260-1 (1)	6.28	6.28	6.18	6.38	0.00
Aroclor-1260-2 (2)	6.47	6.47	6.37	6.57	0.00
Aroclor-1260-3 (3)	6.83	6.84	6.74	6.94	0.01
Aroclor-1260-4 (4)	7.09	7.10	7.00	7.20	0.01
Aroclor-1260-5 (5)	7.34	7.34	7.24	7.44	0.00
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.74	8.75	8.65	8.85	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/08/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 09:08 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2 (2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3 (3)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-4 (4)	5.00	5.01	4.91	5.11	0.01
Aroclor-1016-5 (5)	5.22	5.22	5.12	5.32	0.00
Aroclor-1260-1 (1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3 (3)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.69	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR1 ID: 0.32 (mm) Init. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL04 Date Analyzed: 04/08/2025

Lab Sample No.: AR1660CCC500 Data File : PO110292.D Time Analyzed: 09:08

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.783	4.685	4.885	490.750	500.000	-1.9
Aroclor-1016-2	4.802	4.704	4.904	490.770	500.000	-1.8
Aroclor-1016-3	4.858	4.761	4.961	494.230	500.000	-1.2
Aroclor-1016-4	4.979	4.881	5.081	493.910	500.000	-1.2
Aroclor-1016-5	5.236	5.139	5.339	541.310	500.000	8.3
Aroclor-1260-1	6.277	6.180	6.380	505.880	500.000	1.2
Aroclor-1260-2	6.467	6.369	6.569	476.430	500.000	-4.7
Aroclor-1260-3	6.834	6.737	6.937	473.120	500.000	-5.4
Aroclor-1260-4	7.094	6.998	7.198	466.380	500.000	-6.7
Aroclor-1260-5	7.337	7.239	7.439	469.070	500.000	-6.2
Decachlorobiphenyl	8.742	8.645	8.845	53.700	50.000	7.4
Tetrachloro-m-xylene	3.690	3.592	3.792	48.950	50.000	-2.1



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL04 Date Analyzed: 04/08/2025

Lab Sample No.: AR1660CCC500 Data File : PO110292.D Time Analyzed: 09:08

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.768	4.672	4.872	460.700	500.000	-7.9
Aroclor-1016-2	4.787	4.691	4.891	458.320	500.000	-8.3
Aroclor-1016-3	4.963	4.867	5.067	460.180	500.000	-8.0
Aroclor-1016-4	5.004	4.909	5.109	424.320	500.000	-15.1
Aroclor-1016-5	5.218	5.122	5.322	488.430	500.000	-2.3
Aroclor-1260-1	6.250	6.155	6.355	451.100	500.000	-9.8
Aroclor-1260-2	6.438	6.342	6.542	446.060	500.000	-10.8
Aroclor-1260-3	6.590	6.495	6.695	427.140	500.000	-14.6
Aroclor-1260-4	7.062	6.967	7.167	425.210	500.000	-15.0
Aroclor-1260-5	7.303	7.207	7.407	416.030	500.000	-16.8
Decachlorobiphenyl	8.691	8.596	8.796	44.590	50.000	-10.8
Tetrachloro-m-xylene	3.687	3.590	3.790	47.020	50.000	-6.0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110292.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 09:08  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:41:56 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	3.690	3.687	445.6E6	246.6E6	48.954	47.018
2) SA Decachloro...	8.742	8.691	412.9E6	108.2E6	53.697	44.591

Target Compounds

3) L1 AR-1016-1	4.783	4.768	165.2E6	84424795	490.747	460.696
4) L1 AR-1016-2	4.802	4.787	227.6E6	119.9E6	490.775	458.320
5) L1 AR-1016-3	4.858	4.963	158.4E6	65243266	494.235	460.177
6) L1 AR-1016-4	4.979	5.004	124.8E6	50039864	493.910	424.319
7) L1 AR-1016-5	5.236	5.218	148.8E6	74690506	541.314	488.433
31) L7 AR-1260-1	6.277	6.250	238.4E6	115.2E6	505.880	451.099
32) L7 AR-1260-2	6.467	6.438	283.7E6	133.9E6	476.430	446.059
33) L7 AR-1260-3	6.834	6.590	229.6E6	123.4E6	473.116	427.141
34) L7 AR-1260-4	7.094	7.062	197.8E6	91454142	466.378	425.213
35) L7 AR-1260-5	7.337	7.303	490.6E6	207.5E6	469.072	416.025



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110292.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 09:08  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 AR1660CCC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:41:56 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$

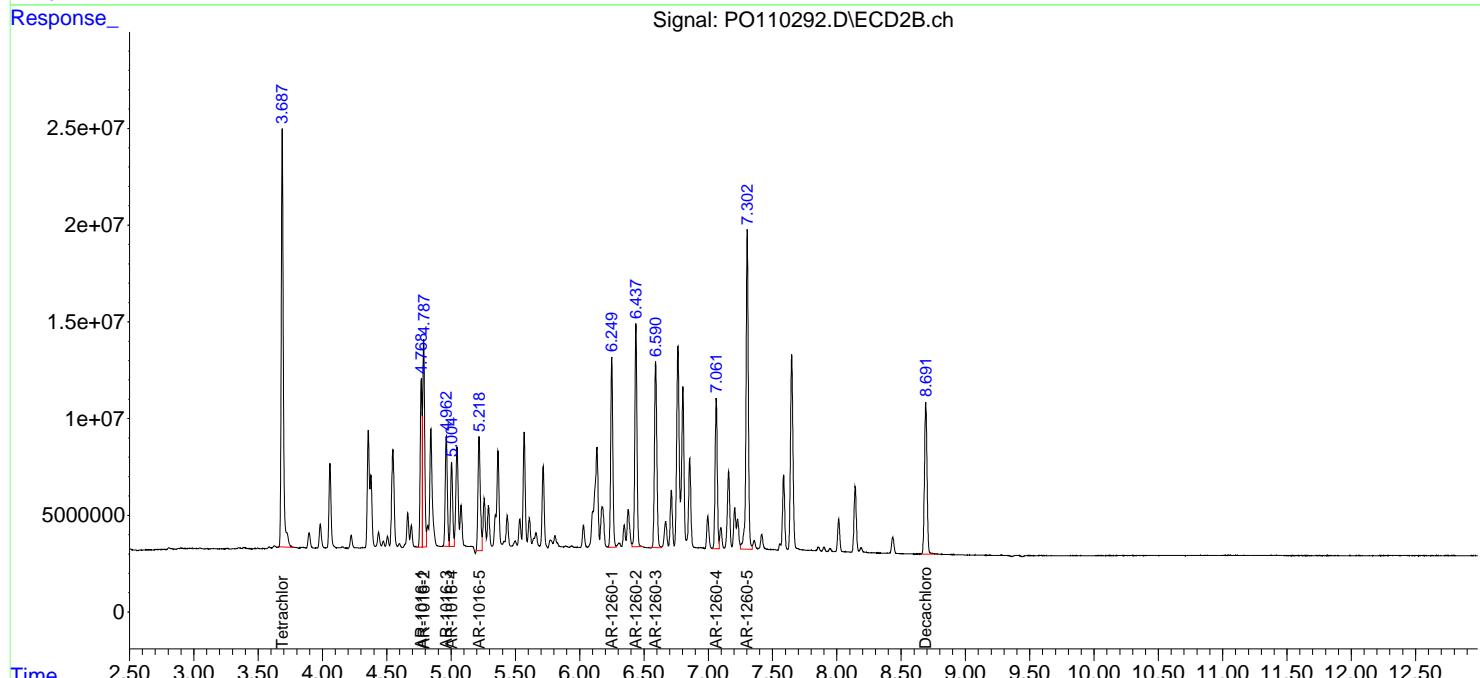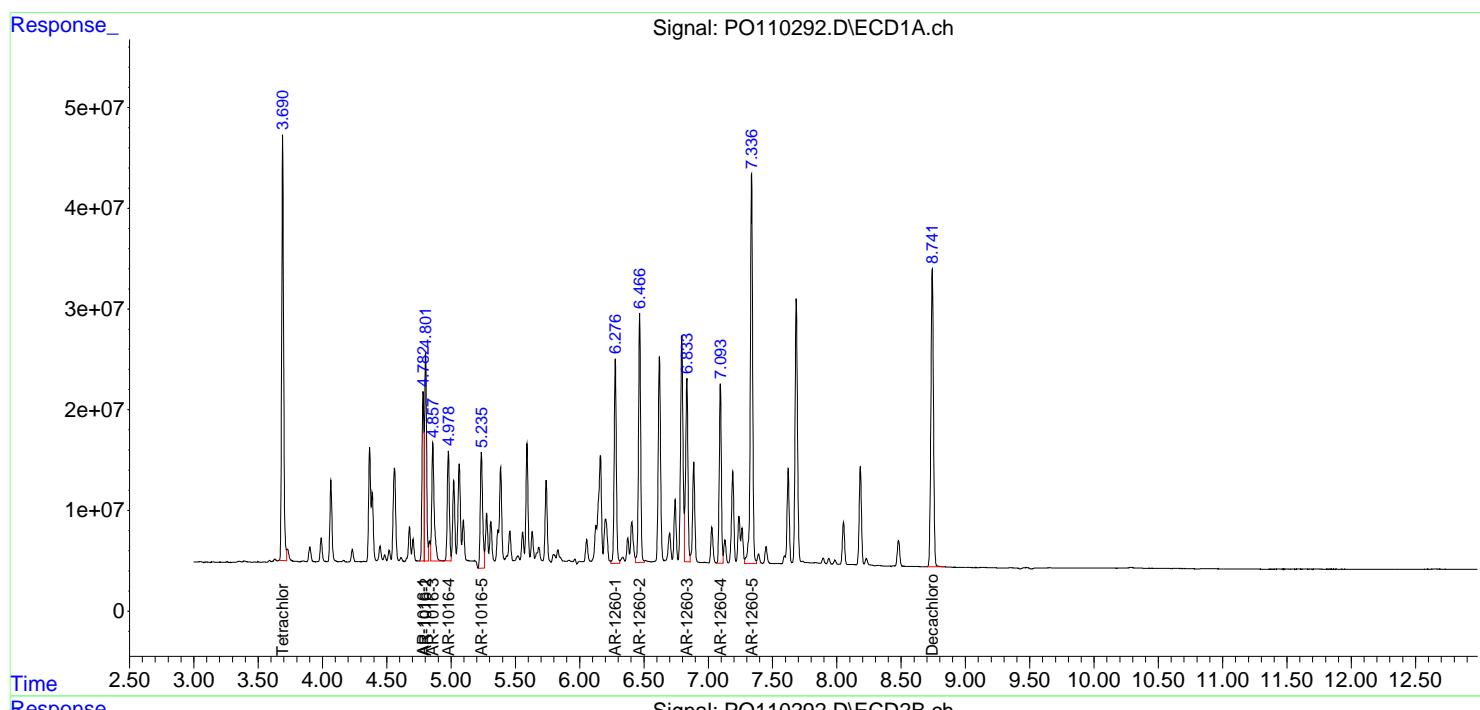

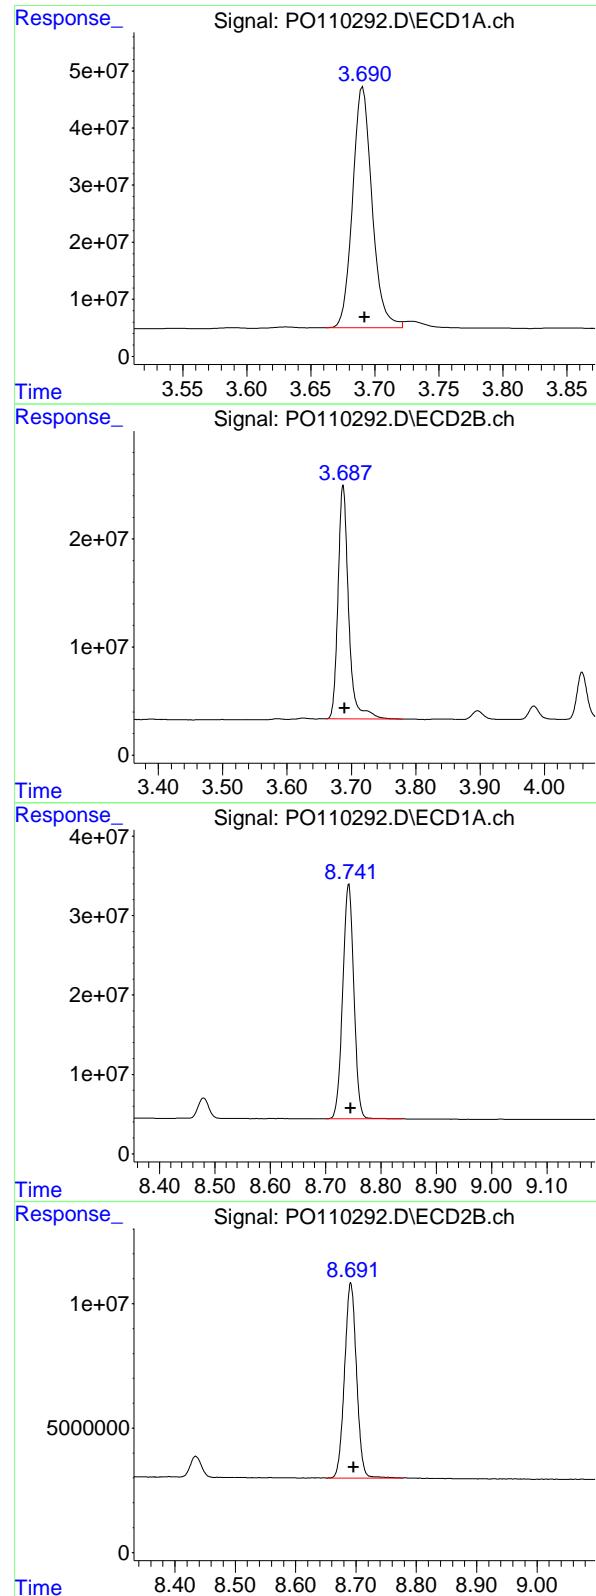

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: -0.002 min  
 Response: 445550594  
 Conc: 48.95 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

## #1 Tetrachloro-m-xylene





R.T.: 3.687 min  
 Delta R.T.: -0.003 min  
 Response: 246565424  
 Conc: 47.02 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.742 min  
 Delta R.T.: -0.004 min  
 Response: 412860287  
 Conc: 53.70 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
 Delta R.T.: -0.005 min  
 Response: 108181543  
 Conc: 44.59 ng/ml

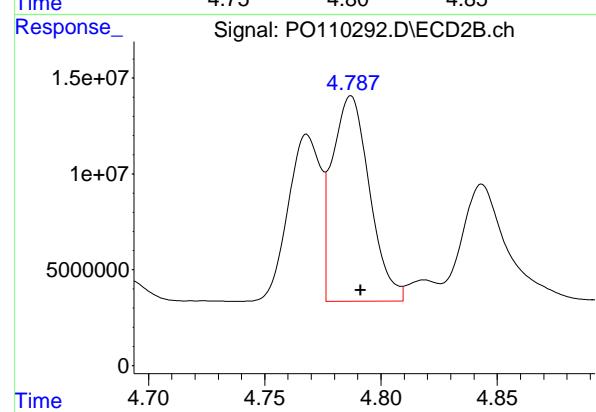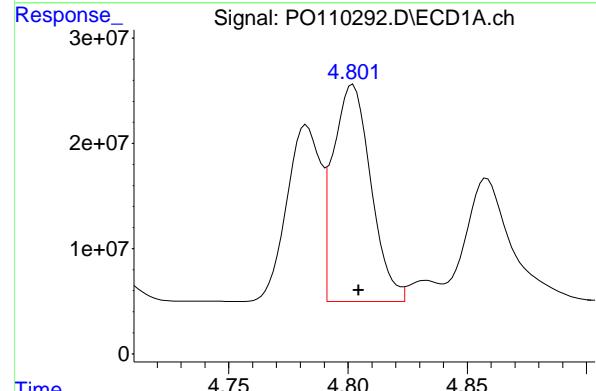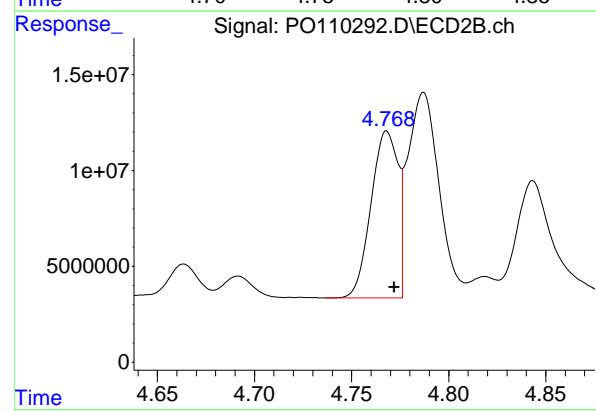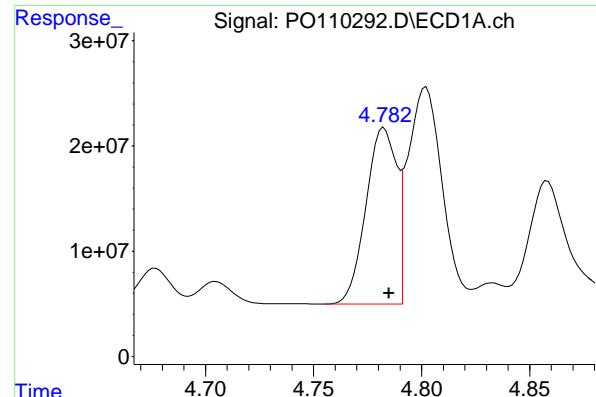

#3 AR-1016-1

R.T.: 4.783 min  
 Delta R.T.: -0.002 min  
 Instrument: ECD\_O  
 Response: 165158163  
 Conc: 490.75 ng/ml  
 ClientSampleId : AR1660CCC500

#3 AR-1016-1


R.T.: 4.768 min  
 Delta R.T.: -0.004 min  
 Response: 84424795  
 Conc: 460.70 ng/ml

#4 AR-1016-2

R.T.: 4.802 min  
 Delta R.T.: -0.002 min  
 Response: 227565206  
 Conc: 490.77 ng/ml

#4 AR-1016-2

R.T.: 4.787 min  
 Delta R.T.: -0.004 min  
 Response: 119852669  
 Conc: 458.32 ng/ml

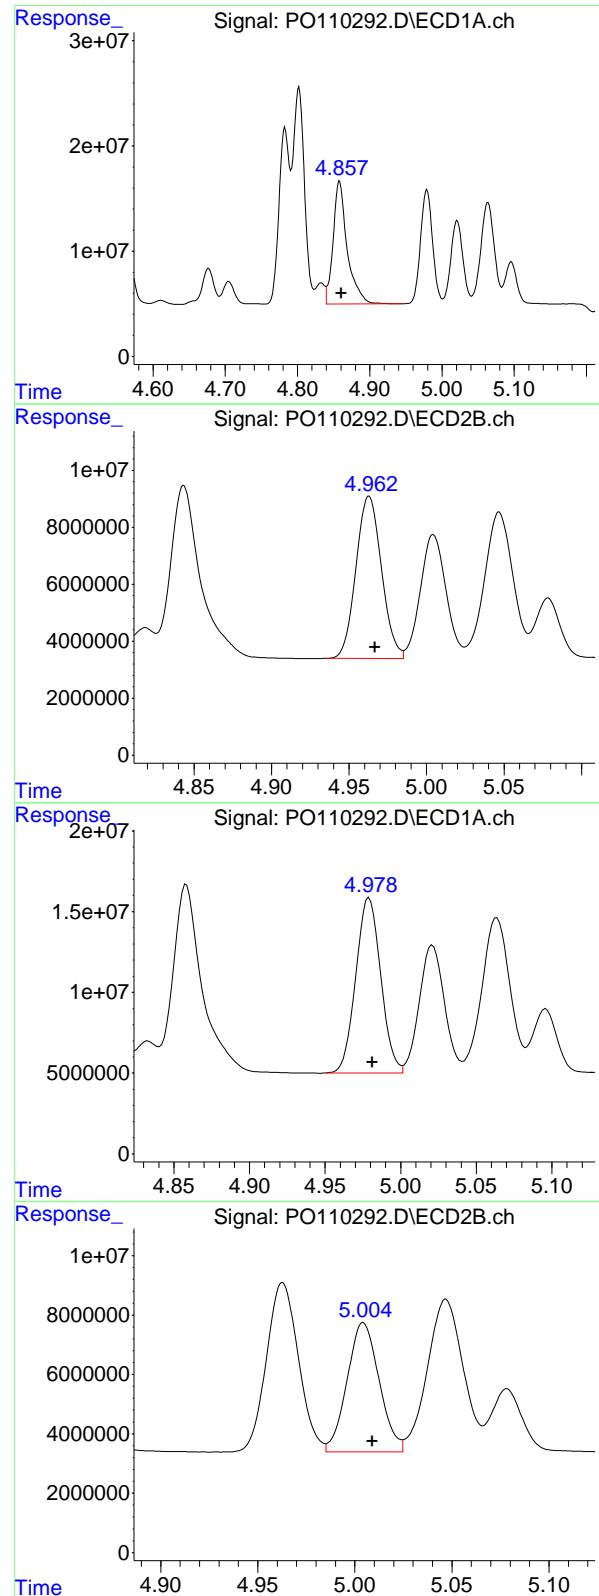

#5 AR-1016-3

R.T.: 4.858 min  
 Delta R.T.: -0.003 min  
 Instrument: ECD\_O  
 Response: 158444813  
 Conc: 494.23 ng/ml  
 ClientSampleId: AR1660CCC500

#5 AR-1016-3





R.T.: 4.963 min  
 Delta R.T.: -0.004 min  
 Response: 65243266  
 Conc: 460.18 ng/ml

#6 AR-1016-4

R.T.: 4.979 min  
 Delta R.T.: -0.002 min  
 Response: 124805818  
 Conc: 493.91 ng/ml

#6 AR-1016-4

R.T.: 5.004 min  
 Delta R.T.: -0.004 min  
 Response: 50039864  
 Conc: 424.32 ng/ml

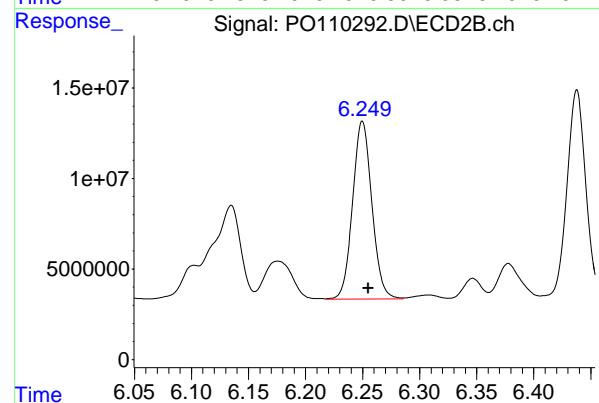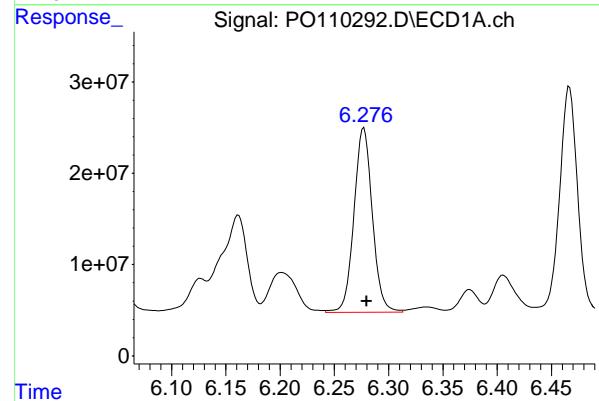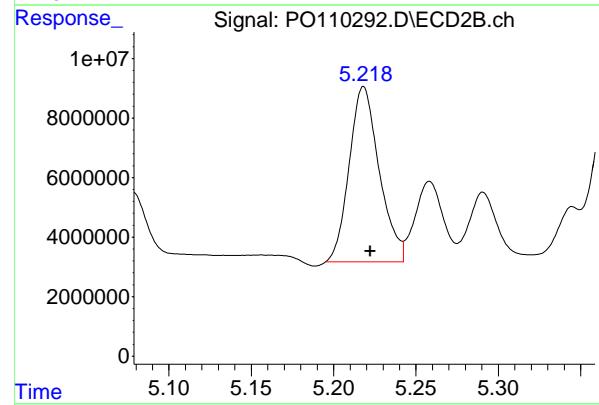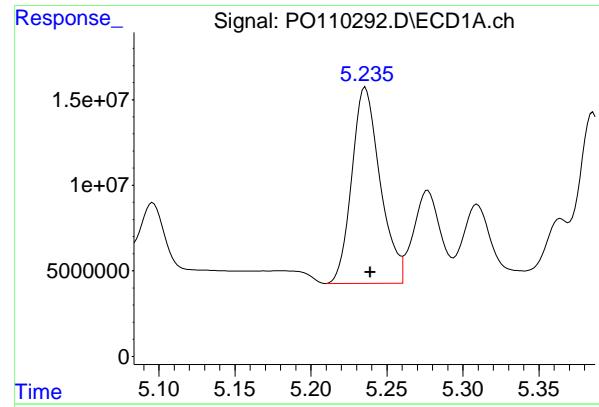

#7 AR-1016-5

R.T.: 5.236 min  
 Delta R.T.: -0.003 min  
 Response: 148789423  
 Conc: 541.31 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#7 AR-1016-5





R.T.: 5.218 min  
 Delta R.T.: -0.004 min  
 Response: 74690506  
 Conc: 488.43 ng/ml

#31 AR-1260-1

R.T.: 6.277 min  
 Delta R.T.: -0.003 min  
 Response: 238446806  
 Conc: 505.88 ng/ml

#31 AR-1260-1

R.T.: 6.250 min  
 Delta R.T.: -0.005 min  
 Response: 115229432  
 Conc: 451.10 ng/ml

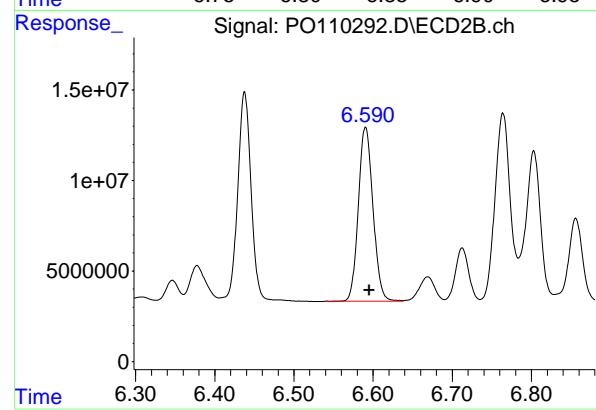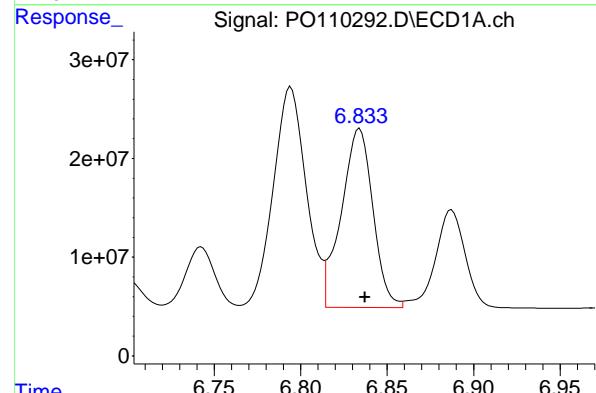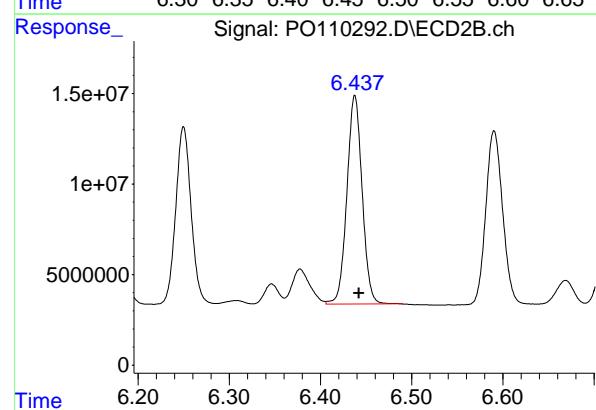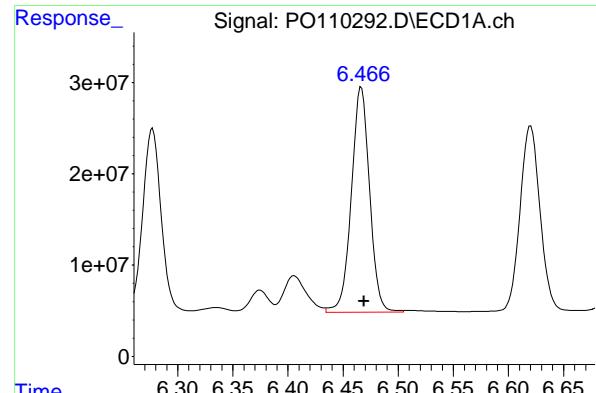

#32 AR-1260-2

R.T.: 6.467 min  
 Delta R.T.: -0.002 min  
 Instrument: ECD\_O  
 Response: 283723218  
 Conc: 476.43 ng/ml  
 ClientSampleId : AR1660CCC500

#32 AR-1260-2


R.T.: 6.438 min  
 Delta R.T.: -0.005 min  
 Response: 133944941  
 Conc: 446.06 ng/ml

#33 AR-1260-3

R.T.: 6.834 min  
 Delta R.T.: -0.003 min  
 Response: 229604002  
 Conc: 473.12 ng/ml


#33 AR-1260-3

R.T.: 6.590 min  
 Delta R.T.: -0.005 min  
 Response: 123436061  
 Conc: 427.14 ng/ml

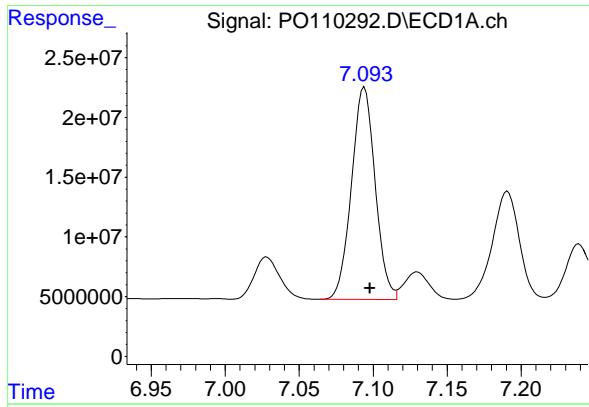


#34 AR-1260-4

R.T.: 7.094 min  
 Delta R.T.: -0.004 min  
 Response: 197822722  
 Conc: 466.38 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId :** AR1660CCC500

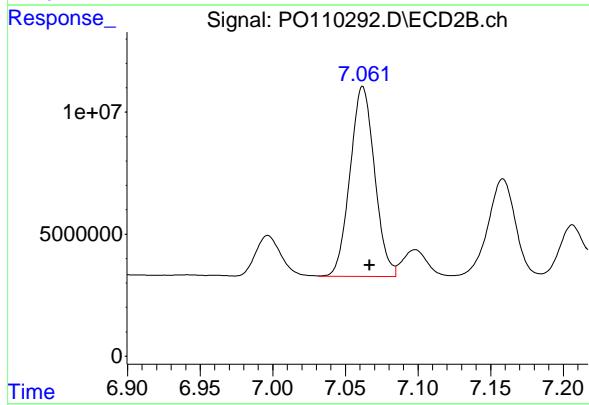


#34 AR-1260-4

R.T.: 7.062 min  
 Delta R.T.: -0.005 min  
 Response: 91454142  
 Conc: 425.21 ng/ml

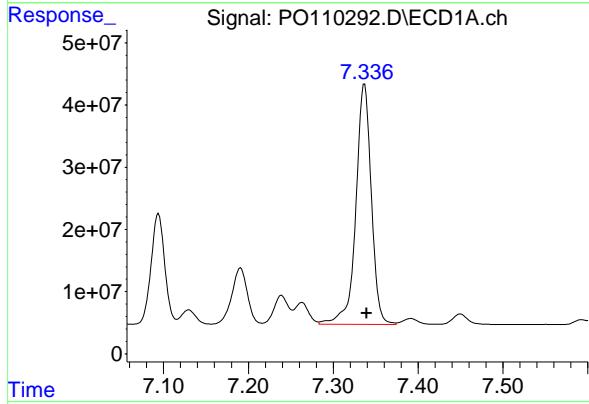

#35 AR-1260-5

R.T.: 7.337 min  
 Delta R.T.: -0.003 min  
 Response: 490577287  
 Conc: 469.07 ng/ml

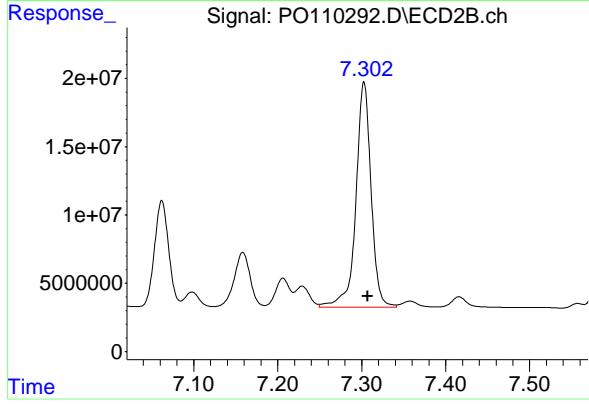

#35 AR-1260-5

R.T.: 7.303 min  
 Delta R.T.: -0.004 min  
 Response: 207470142  
 Conc: 416.03 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/08/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 12:58 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-2 (2)	4.80	4.80	4.70	4.90	0.00
Aroclor-1016-3 (3)	4.86	4.86	4.76	4.96	0.00
Aroclor-1016-4 (4)	4.98	4.98	4.88	5.08	0.00
Aroclor-1016-5 (5)	5.24	5.24	5.14	5.34	0.00
Aroclor-1260-1 (1)	6.28	6.28	6.18	6.38	0.00
Aroclor-1260-2 (2)	6.47	6.47	6.37	6.57	0.00
Aroclor-1260-3 (3)	6.83	6.84	6.74	6.94	0.01
Aroclor-1260-4 (4)	7.09	7.10	7.00	7.20	0.01
Aroclor-1260-5 (5)	7.34	7.34	7.24	7.44	0.00
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.74	8.75	8.65	8.85	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/08/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 12:58 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2 (2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3 (3)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-4 (4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5 (5)	5.22	5.22	5.12	5.32	0.00
Aroclor-1260-1 (1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2 (2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3 (3)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-4 (4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5 (5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene	3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl	8.69	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR1 ID: 0.32 (mm) Init. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL05 Date Analyzed: 04/08/2025

Lab Sample No.: AR1660CCC500 Data File : PO110302.D Time Analyzed: 12:58

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.783	4.685	4.885	478.010	500.000	-4.4
Aroclor-1016-2	4.802	4.704	4.904	481.930	500.000	-3.6
Aroclor-1016-3	4.858	4.761	4.961	488.150	500.000	-2.4
Aroclor-1016-4	4.979	4.881	5.081	483.730	500.000	-3.3
Aroclor-1016-5	5.237	5.139	5.339	484.580	500.000	-3.1
Aroclor-1260-1	6.277	6.180	6.380	484.710	500.000	-3.1
Aroclor-1260-2	6.466	6.369	6.569	466.260	500.000	-6.7
Aroclor-1260-3	6.834	6.737	6.937	478.180	500.000	-4.4
Aroclor-1260-4	7.094	6.998	7.198	469.910	500.000	-6.0
Aroclor-1260-5	7.336	7.239	7.439	460.630	500.000	-7.9
Decachlorobiphenyl	8.739	8.645	8.845	56.540	50.000	13.1
Tetrachloro-m-xylene	3.691	3.592	3.792	47.860	50.000	-4.3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL05 Date Analyzed: 04/08/2025

Lab Sample No.: AR1660CCC500 Data File : PO110302.D Time Analyzed: 12:58

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.769	4.672	4.872	459.150	500.000	-8.2
Aroclor-1016-2	4.788	4.691	4.891	461.630	500.000	-7.7
Aroclor-1016-3	4.963	4.867	5.067	464.240	500.000	-7.2
Aroclor-1016-4	5.005	4.909	5.109	462.280	500.000	-7.5
Aroclor-1016-5	5.218	5.122	5.322	459.630	500.000	-8.1
Aroclor-1260-1	6.250	6.155	6.355	447.090	500.000	-10.6
Aroclor-1260-2	6.438	6.342	6.542	439.930	500.000	-12.0
Aroclor-1260-3	6.591	6.495	6.695	426.390	500.000	-14.7
Aroclor-1260-4	7.063	6.967	7.167	425.830	500.000	-14.8
Aroclor-1260-5	7.303	7.207	7.407	416.620	500.000	-16.7
Decachlorobiphenyl	8.692	8.596	8.796	45.310	50.000	-9.4
Tetrachloro-m-xylene	3.688	3.590	3.790	47.270	50.000	-5.5

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110302.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 12:58  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 13:41:57 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	3.691	3.688	435.6E6	247.9E6	47.860	47.272
2) SA Decachloro...	8.739	8.692	434.7E6	109.9E6	56.541	45.308

Target Compounds

3) L1 AR-1016-1	4.783	4.769	160.9E6	84140877	478.015	459.147
4) L1 AR-1016-2	4.802	4.788	223.5E6	120.7E6	481.932	461.633
5) L1 AR-1016-3	4.858	4.963	156.5E6	65819182	488.147	464.239
6) L1 AR-1016-4	4.979	5.005	122.2E6	54516660	483.727	462.281
7) L1 AR-1016-5	5.237	5.218	133.2E6	70285787	484.577	459.629
31) L7 AR-1260-1	6.277	6.250	228.5E6	114.2E6	484.705	447.094
32) L7 AR-1260-2	6.466	6.438	277.7E6	132.1E6	466.258	439.928
33) L7 AR-1260-3	6.834	6.591	232.1E6	123.2E6	478.181	426.386
34) L7 AR-1260-4	7.094	7.063	199.3E6	91586397	469.907	425.828
35) L7 AR-1260-5	7.336	7.303	481.7E6	207.8E6	460.625	416.615



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110302.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 12:58  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 AR1660CCC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 13:41:57 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

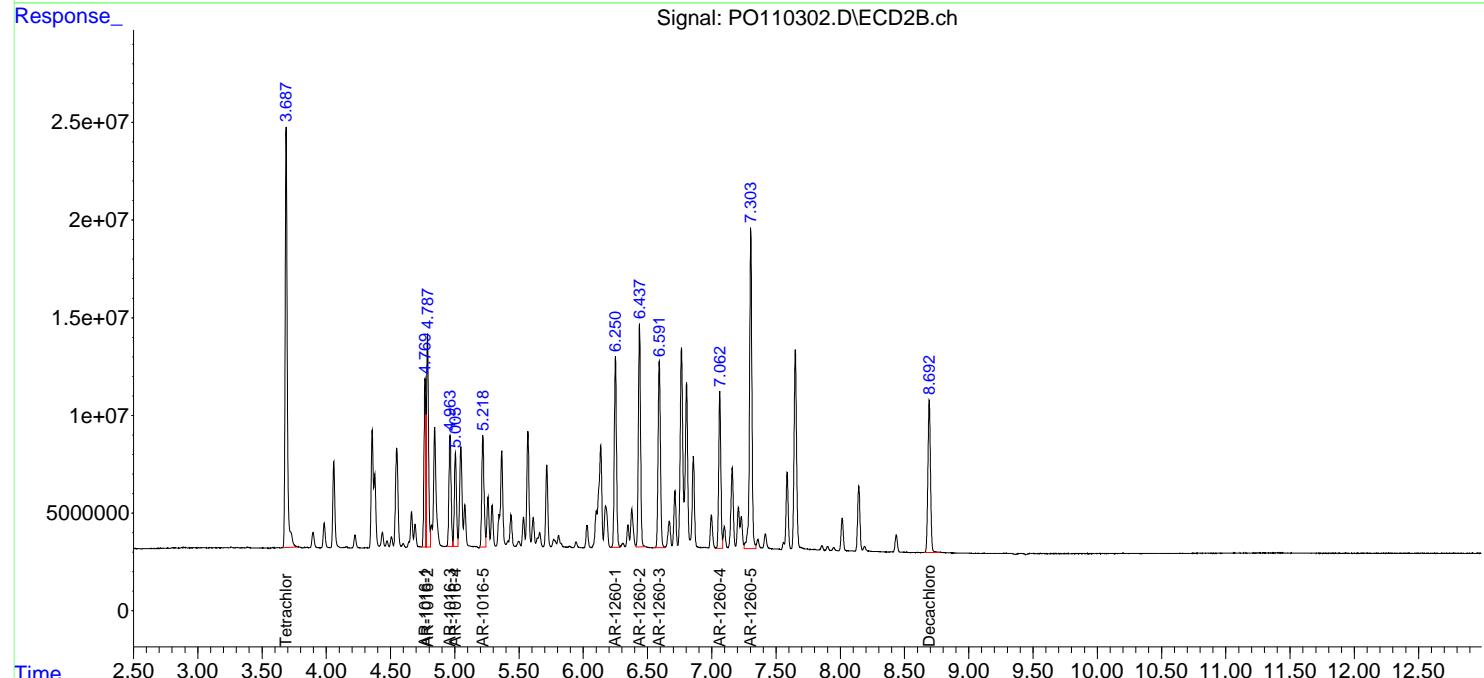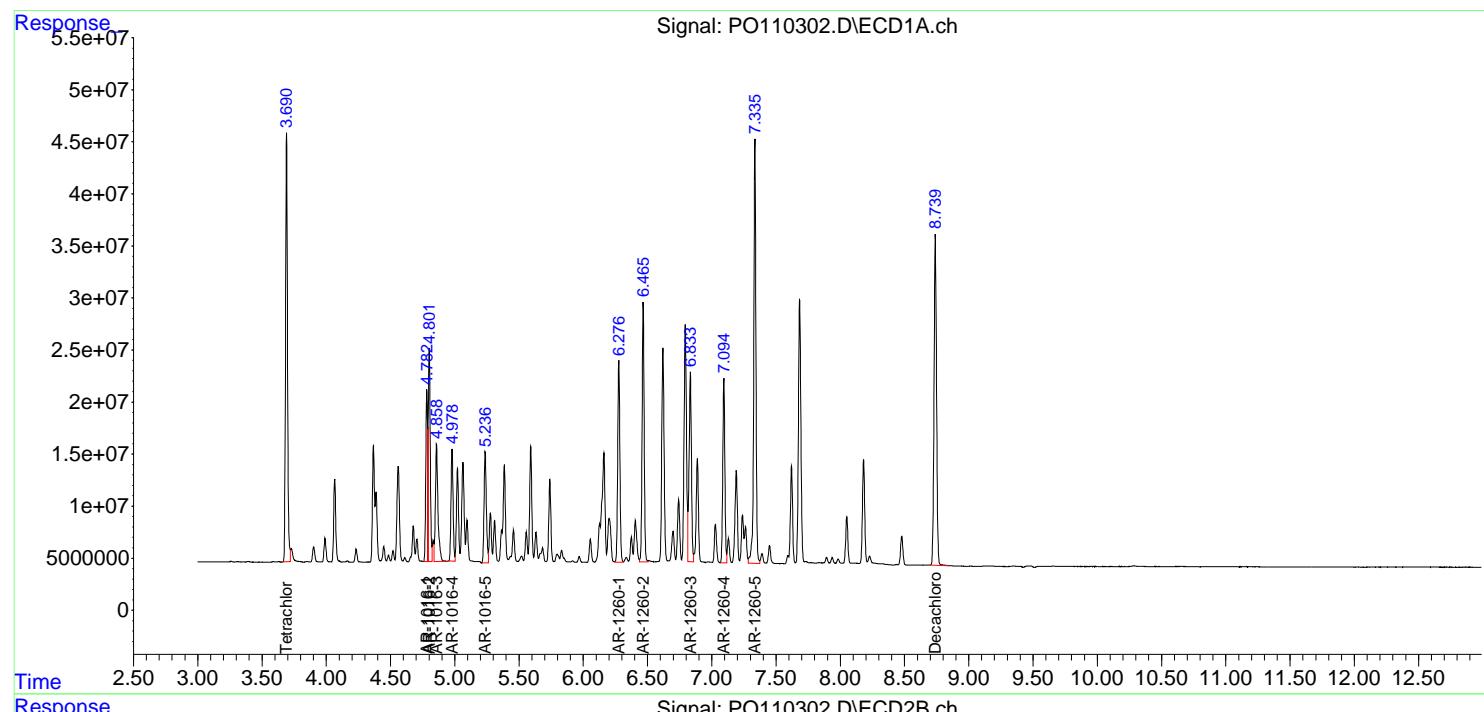

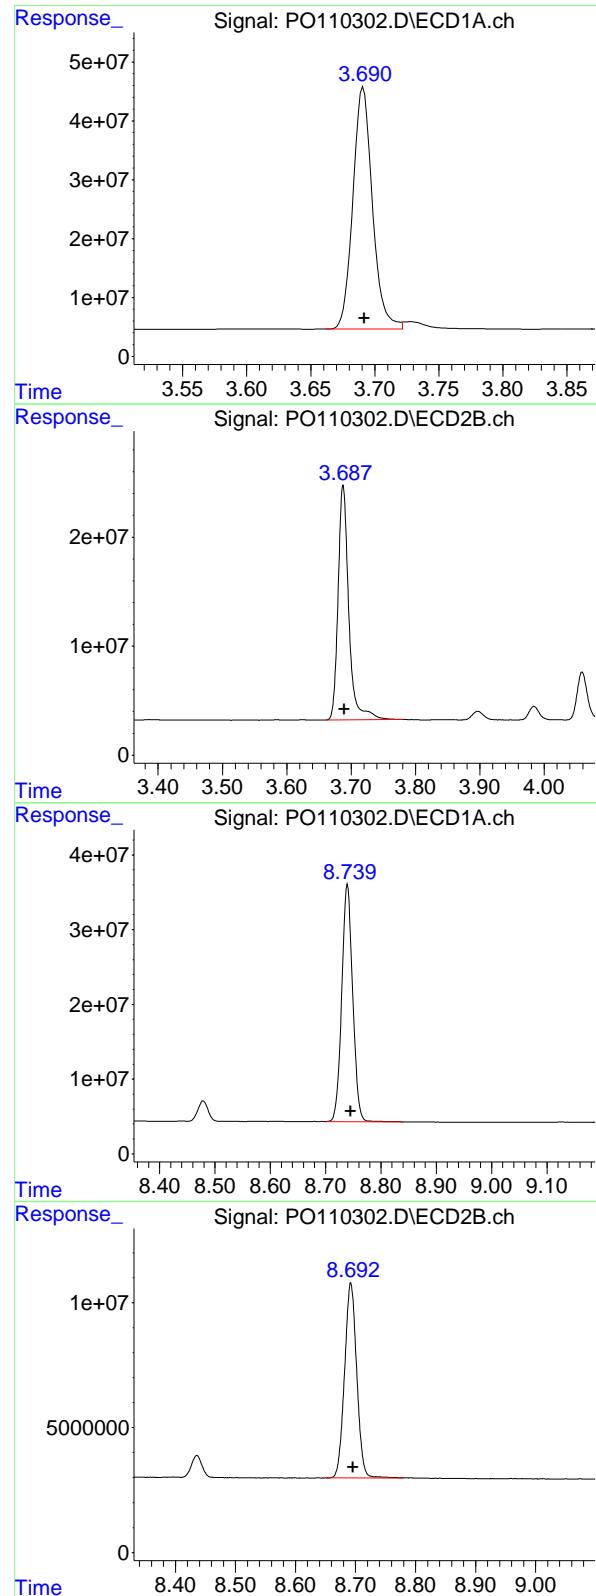

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: -0.001 min  
 Response: 435598852  
 Conc: 47.86 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

## #1 Tetrachloro-m-xylene


R.T.: 3.688 min  
 Delta R.T.: -0.002 min  
 Response: 247897432  
 Conc: 47.27 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.739 min  
 Delta R.T.: -0.006 min  
 Response: 434722533  
 Conc: 56.54 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.692 min  
 Delta R.T.: -0.004 min  
 Response: 109921655  
 Conc: 45.31 ng/ml

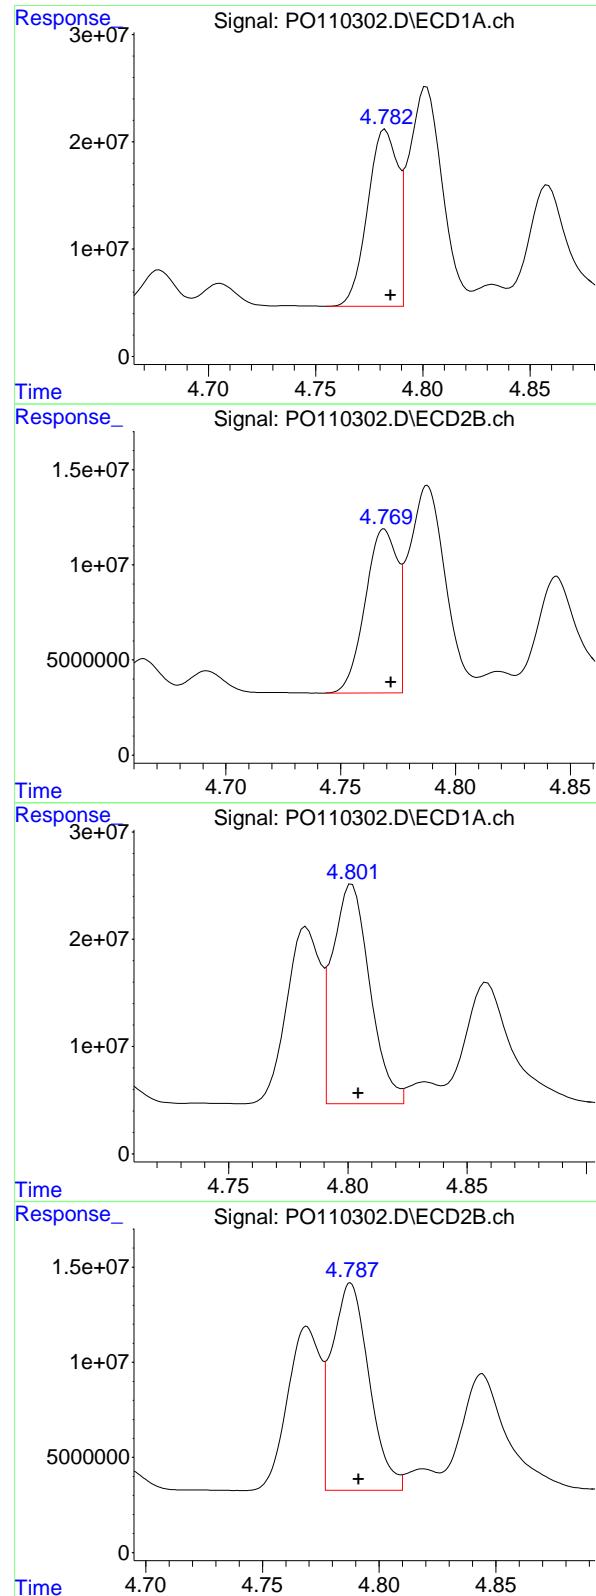

#3 AR-1016-1

R.T.: 4.783 min  
 Delta R.T.: -0.002 min  
 Instrument: ECD\_O  
 Response: 160873001  
 Conc: 478.01 ng/ml  
 ClientSampleId : AR1660CCC500

#3 AR-1016-1


R.T.: 4.769 min  
 Delta R.T.: -0.003 min  
 Response: 84140877  
 Conc: 459.15 ng/ml

#4 AR-1016-2

R.T.: 4.802 min  
 Delta R.T.: -0.003 min  
 Response: 223464953  
 Conc: 481.93 ng/ml

#4 AR-1016-2

R.T.: 4.788 min  
 Delta R.T.: -0.003 min  
 Response: 120719056  
 Conc: 461.63 ng/ml

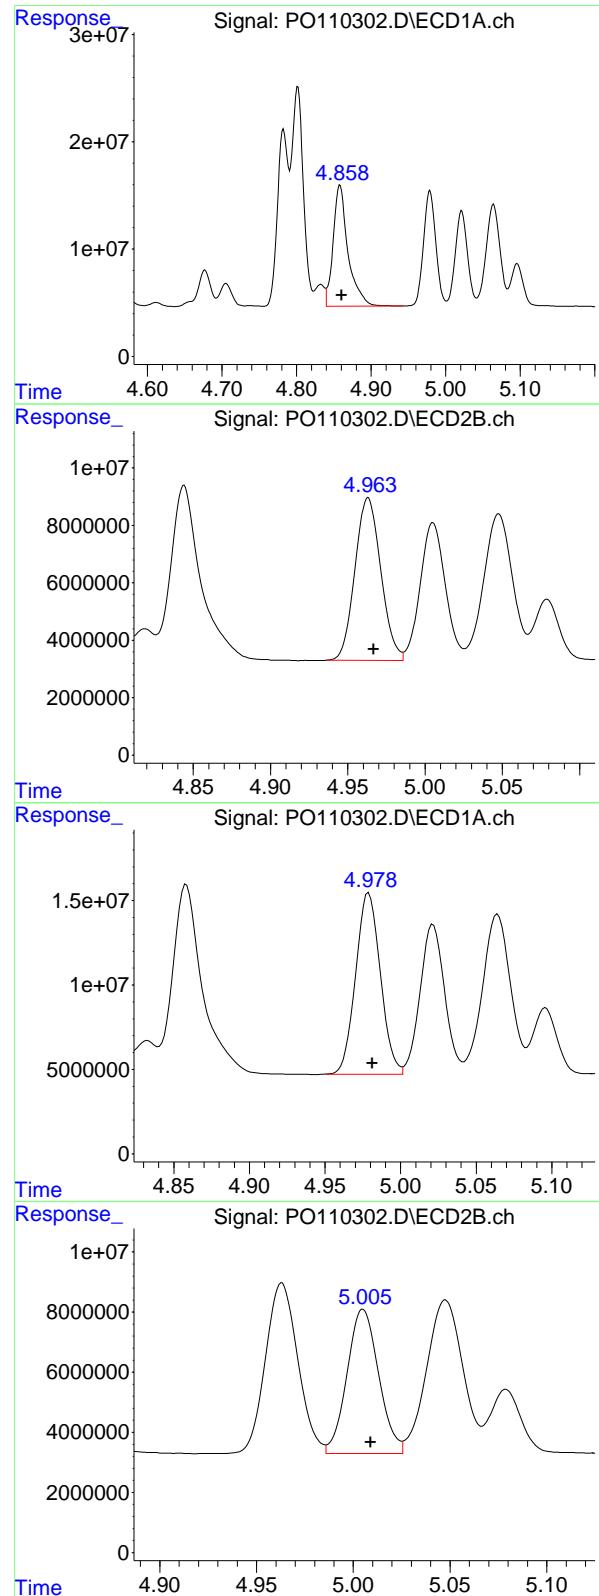

#5 AR-1016-3

R.T.: 4.858 min  
 Delta R.T.: -0.003 min  
 Instrument: ECD\_O  
 Response: 156493158  
 Conc: 488.15 ng/ml  
 ClientSampleId: AR1660CCC500

#5 AR-1016-3



R.T.: 4.963 min  
 Delta R.T.: -0.004 min  
 Response: 65819182  
 Conc: 464.24 ng/ml

#6 AR-1016-4

R.T.: 4.979 min  
 Delta R.T.: -0.002 min  
 Response: 122232752  
 Conc: 483.73 ng/ml

#6 AR-1016-4

R.T.: 5.005 min  
 Delta R.T.: -0.004 min  
 Response: 54516660  
 Conc: 462.28 ng/ml

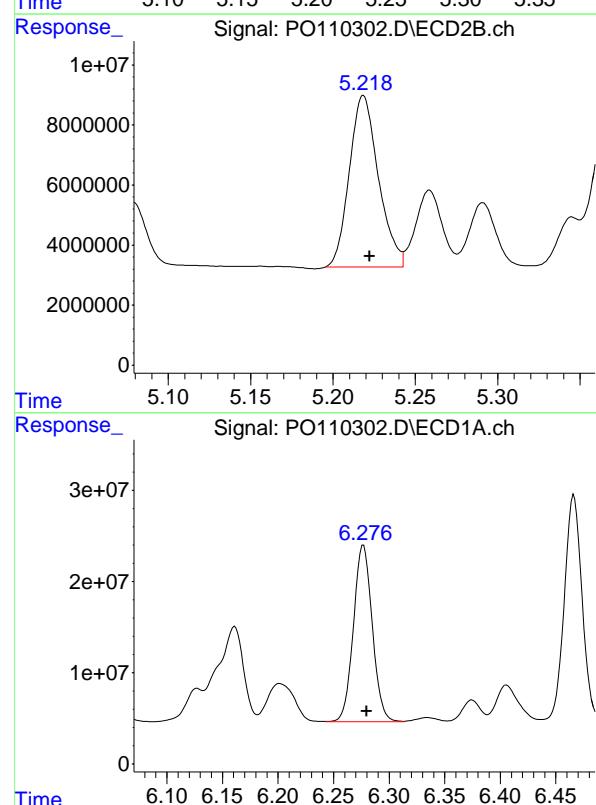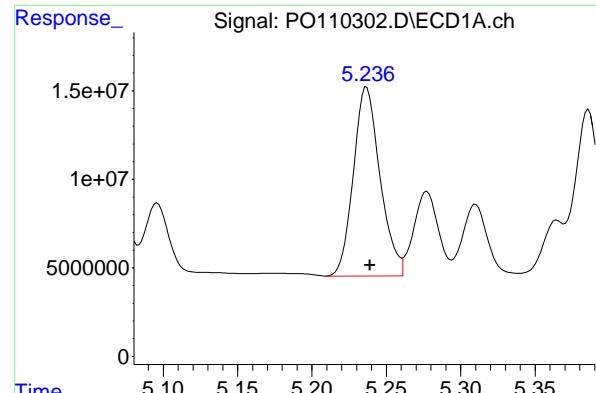

#7 AR-1016-5

R.T.: 5.237 min  
 Delta R.T.: -0.002 min  
 Response: 133194313  
 Conc: 484.58 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId :** AR1660CCC500

#7 AR-1016-5





R.T.: 5.218 min  
 Delta R.T.: -0.004 min  
 Response: 70285787  
 Conc: 459.63 ng/ml

#31 AR-1260-1

R.T.: 6.277 min  
 Delta R.T.: -0.003 min  
 Response: 228466177  
 Conc: 484.71 ng/ml

#31 AR-1260-1

R.T.: 6.250 min  
 Delta R.T.: -0.005 min  
 Response: 114206424  
 Conc: 447.09 ng/ml

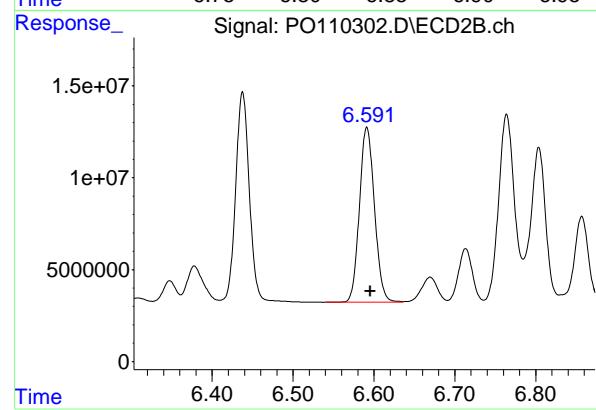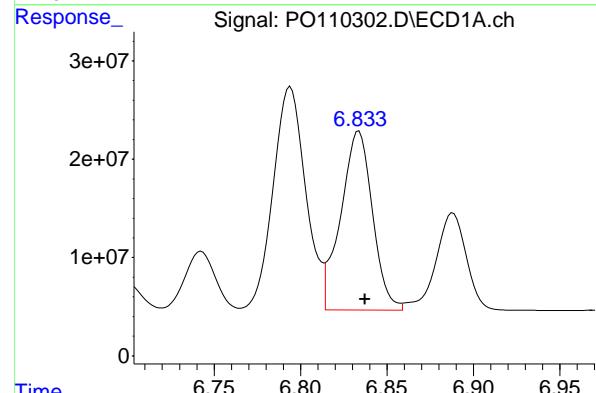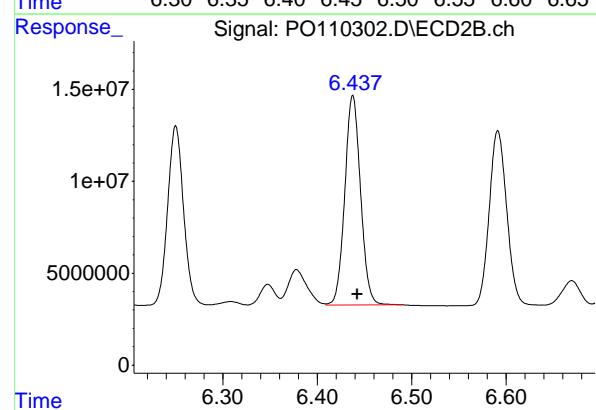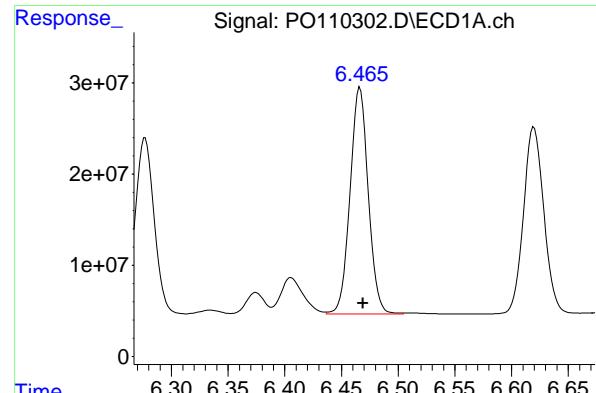

#32 AR-1260-2

R.T.: 6.466 min  
 Delta R.T.: -0.003 min  
 Response: 277665605  
 Conc: 466.26 ng/ml  
 Instrument: ECD\_O  
 ClientSampleId : AR1660CCC500

#32 AR-1260-2


R.T.: 6.438 min  
 Delta R.T.: -0.005 min  
 Response: 132103988  
 Conc: 439.93 ng/ml

#33 AR-1260-3

R.T.: 6.834 min  
 Delta R.T.: -0.004 min  
 Response: 232062227  
 Conc: 478.18 ng/ml

#33 AR-1260-3

R.T.: 6.591 min  
 Delta R.T.: -0.004 min  
 Response: 123217994  
 Conc: 426.39 ng/ml

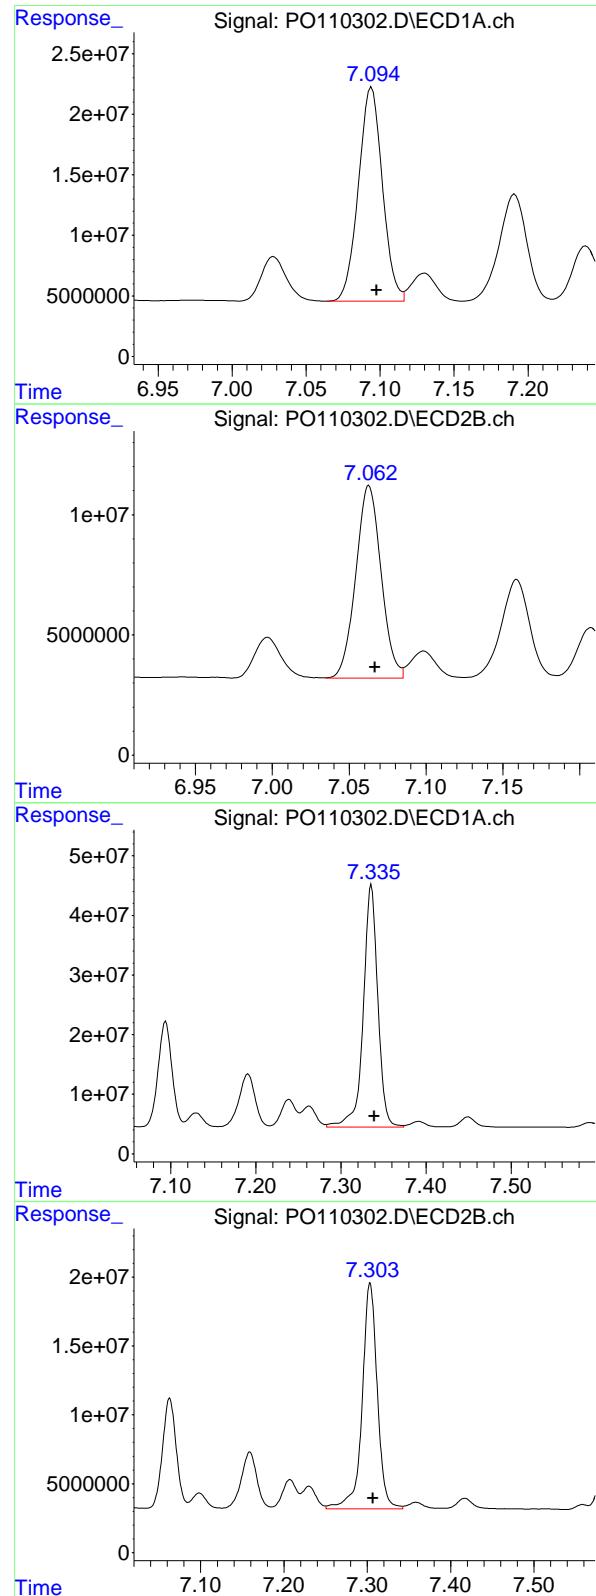

#34 AR-1260-4

R.T.: 7.094 min  
 Delta R.T.: -0.003 min  
 Response: 199319657  
 Conc: 469.91 ng/ml  
 Instrument: ECD\_O  
 ClientSampleId : AR1660CCC500

#34 AR-1260-4

R.T.: 7.063 min  
 Delta R.T.: -0.004 min  
 Response: 91586397  
 Conc: 425.83 ng/ml

#35 AR-1260-5

R.T.: 7.336 min  
 Delta R.T.: -0.004 min  
 Response: 481743144  
 Conc: 460.63 ng/ml

#35 AR-1260-5

R.T.: 7.303 min  
 Delta R.T.: -0.004 min  
 Response: 207764421  
 Conc: 416.62 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/08/2025 Initial Calibration Date(s): 03/27/2025 03/27/2025

Continuing Calib Time: 09:37 Initial Calibration Time(s): 10:30 17:53

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	Avg RT	RT Window From	To	Diff RT
Aroclor-1016-1 (1)	5.68	5.66	5.56	5.76	-0.02
Aroclor-1016-2 (2)	5.70	5.69	5.59	5.79	-0.01
Aroclor-1016-3 (3)	5.76	5.75	5.65	5.85	-0.01
Aroclor-1016-4 (4)	5.86	5.85	5.75	5.95	-0.01
Aroclor-1016-5 (5)	6.15	6.14	6.04	6.24	-0.01
Aroclor-1260-1 (1)	7.27	7.26	7.16	7.36	-0.01
Aroclor-1260-2 (2)	7.53	7.51	7.41	7.61	-0.02
Aroclor-1260-3 (3)	7.89	7.87	7.77	7.97	-0.02
Aroclor-1260-4 (4)	8.11	8.09	7.99	8.19	-0.02
Aroclor-1260-5 (5)	8.43	8.41	8.31	8.51	-0.02
Tetrachloro-m-xylene	4.52	4.51	4.41	4.61	-0.01
Decachlorobiphenyl	10.26	10.23	10.13	10.33	-0.03



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/08/2025 Initial Calibration Date(s): 03/27/2025 03/27/2025

Continuing Calib Time: 09:37 Initial Calibration Time(s): 10:30 17:53

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.90	4.90	4.80	5.00	0.00
Aroclor-1016-2 (2)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-3 (3)	5.10	5.10	5.00	5.20	0.00
Aroclor-1016-4 (4)	5.14	5.14	5.04	5.24	0.00
Aroclor-1016-5 (5)	5.36	5.36	5.26	5.46	0.00
Aroclor-1260-1 (1)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-2 (2)	6.58	6.58	6.48	6.68	0.00
Aroclor-1260-3 (3)	6.74	6.73	6.63	6.83	-0.01
Aroclor-1260-4 (4)	7.21	7.21	7.11	7.31	0.00
Aroclor-1260-5 (5)	7.45	7.45	7.35	7.55	0.00
Tetrachloro-m-xylene	3.82	3.82	3.72	3.92	0.00
Decachlorobiphenyl	8.86	8.86	8.76	8.96	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 03/27/2025 03/27/2025

Client Sample No.: CCAL06 Date Analyzed: 04/08/2025

Lab Sample No.: AR1660CCC500 Data File : PP071136.D Time Analyzed: 09:37

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	5.679	5.563	5.763	504.230	500.000	0.8
Aroclor-1016-2	5.700	5.585	5.785	472.510	500.000	-5.5
Aroclor-1016-3	5.763	5.648	5.848	488.820	500.000	-2.2
Aroclor-1016-4	5.861	5.745	5.945	525.740	500.000	5.1
Aroclor-1016-5	6.154	6.038	6.238	539.860	500.000	8.0
Aroclor-1260-1	7.273	7.156	7.356	518.030	500.000	3.6
Aroclor-1260-2	7.527	7.410	7.610	536.780	500.000	7.4
Aroclor-1260-3	7.885	7.768	7.968	503.360	500.000	0.7
Aroclor-1260-4	8.109	7.992	8.192	501.370	500.000	0.3
Aroclor-1260-5	8.431	8.311	8.511	506.740	500.000	1.3
Decachlorobiphenyl	10.255	10.125	10.325	51.060	50.000	2.1
Tetrachloro-m-xylene	4.524	4.412	4.612	51.340	50.000	2.7



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/27/2025 03/27/2025

Client Sample No.: CCAL06 Date Analyzed: 04/08/2025

Lab Sample No.: AR1660CCC500 Data File : PP071136.D Time Analyzed: 09:37

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.904	4.803	5.003	491.030	500.000	-1.8
Aroclor-1016-2	4.923	4.822	5.022	483.510	500.000	-3.3
Aroclor-1016-3	5.101	4.999	5.199	522.710	500.000	4.5
Aroclor-1016-4	5.142	5.041	5.241	542.480	500.000	8.5
Aroclor-1016-5	5.357	5.255	5.455	530.130	500.000	6.0
Aroclor-1260-1	6.393	6.292	6.492	547.620	500.000	9.5
Aroclor-1260-2	6.582	6.480	6.680	534.460	500.000	6.9
Aroclor-1260-3	6.735	6.634	6.834	546.870	500.000	9.4
Aroclor-1260-4	7.207	7.105	7.305	489.720	500.000	-2.1
Aroclor-1260-5	7.448	7.346	7.546	462.070	500.000	-7.6
Decachlorobiphenyl	8.862	8.759	8.959	43.790	50.000	-12.4
Tetrachloro-m-xylene	3.817	3.716	3.916	47.940	50.000	-4.1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071136.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 09:37  
 Operator : YP\AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1660CCC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 04/09/2025  
 Supervised By :mohammad ahmed 04/10/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:57:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	4.524	3.817	75031562	49693990	51.336	47.937
2) SA Decachloro...	10.255	8.862	53747529	34514110	51.061	43.789

Target Compounds

3) L1 AR-1016-1	5.679	4.904	25640835	19684563	504.232	491.032
4) L1 AR-1016-2	5.700	4.923	36881275	27978272	472.512m	483.509
5) L1 AR-1016-3	5.763	5.101	23060044	16163902	488.823	522.709
6) L1 AR-1016-4	5.861	5.142	19323906	13212574	525.739	542.479
7) L1 AR-1016-5	6.154	5.357	18307730	17134433	539.858	530.130
31) L7 AR-1260-1	7.273	6.393	34786874	28041460	518.026	547.617
32) L7 AR-1260-2	7.527	6.582	51604417	34095263	536.784	534.460
33) L7 AR-1260-3	7.885	6.735	40227656	29796945	503.360	546.865
34) L7 AR-1260-4	8.109	7.207	39475978	23421548	501.366m	489.721
35) L7 AR-1260-5	8.431	7.448	80513512	57532352	506.737	462.069

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071136.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 09:37  
 Operator : YP\AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:57:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1660CCC500

### Manual Integrations APPROVED

Reviewed By :Yogesh Patel 04/09/2025  
 Supervised By :mohammad ahmed 04/10/2025

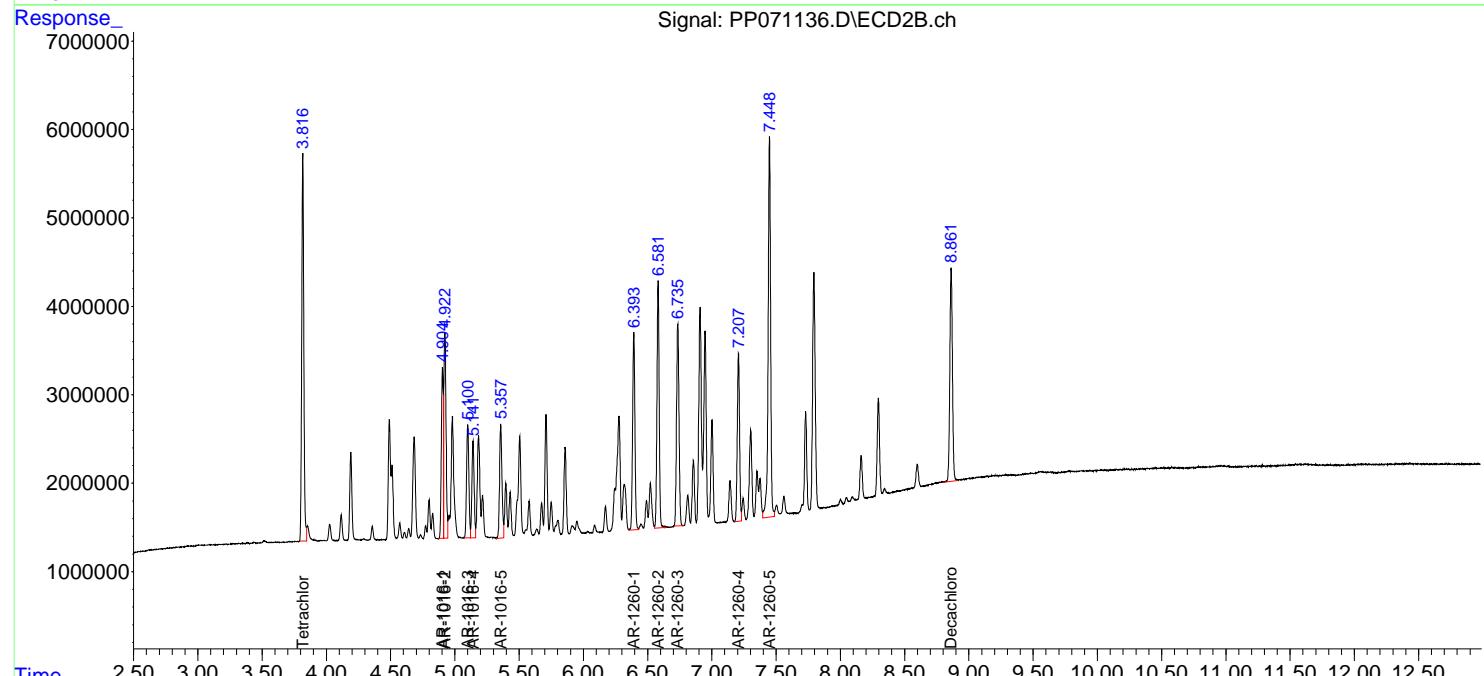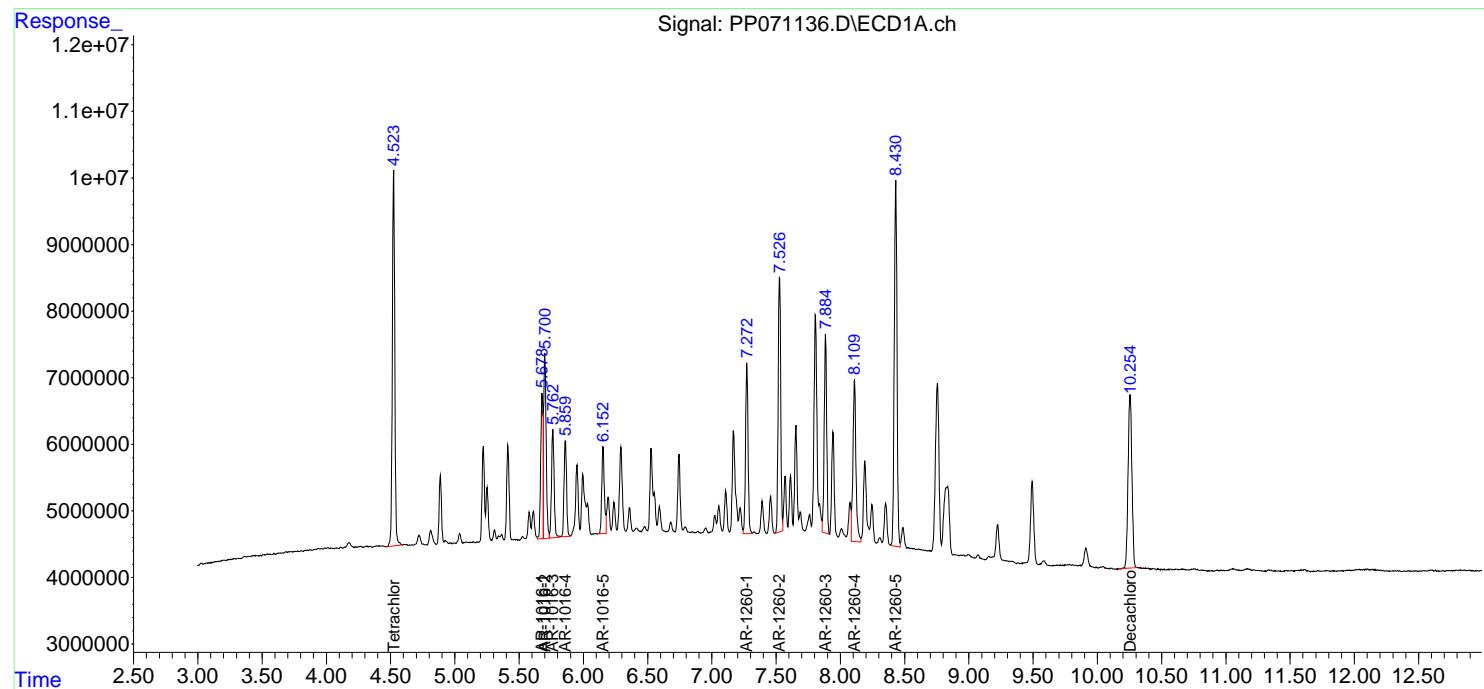

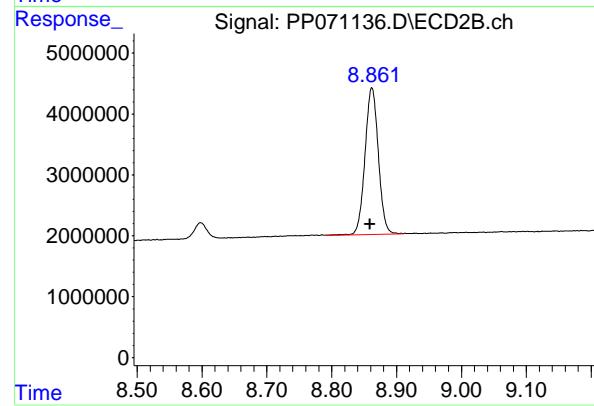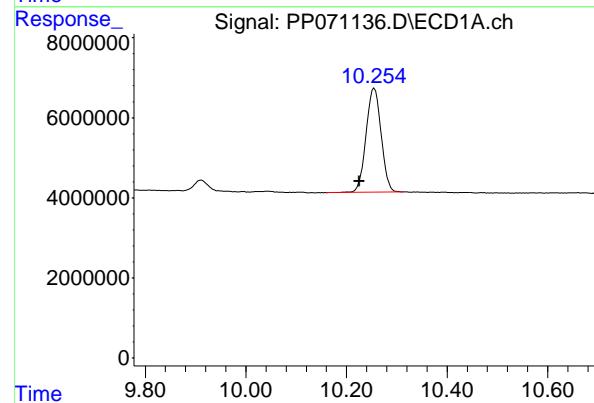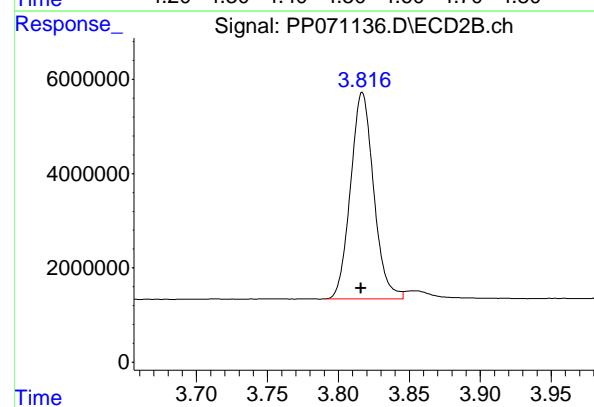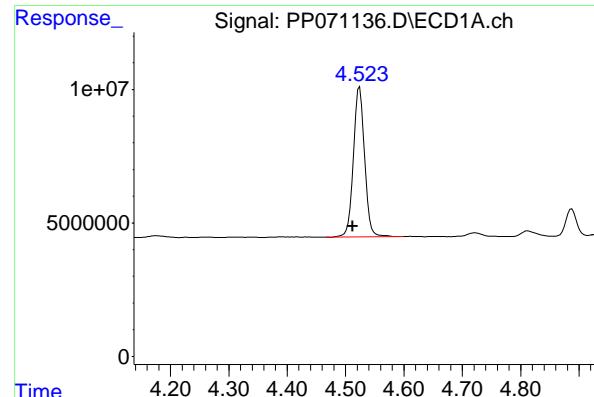

## #1 Tetrachloro-m-xylene

R.T.: 4.524 min  
Delta R.T.: 0.012 min  
Instrument: ECD\_P  
Response: 75031562  
Conc: 51.34 ng/ml Client SampleId : AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/09/2025  
Supervised By :mohammad ahmed 04/10/2025

## #1 Tetrachloro-m-xylene





R.T.: 3.817 min  
Delta R.T.: 0.000 min  
Response: 49693990  
Conc: 47.94 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.255 min  
Delta R.T.: 0.030 min  
Response: 53747529  
Conc: 51.06 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.862 min  
Delta R.T.: 0.003 min  
Response: 34514110  
Conc: 43.79 ng/ml

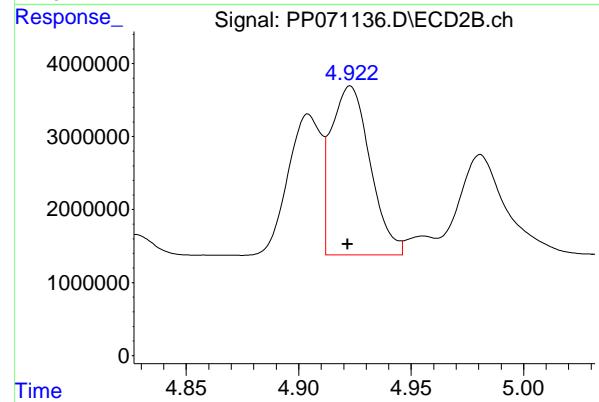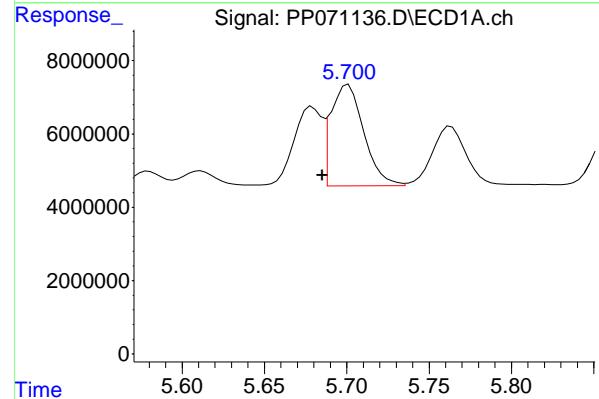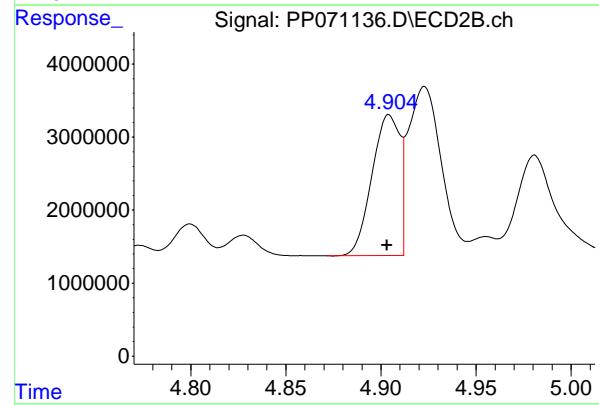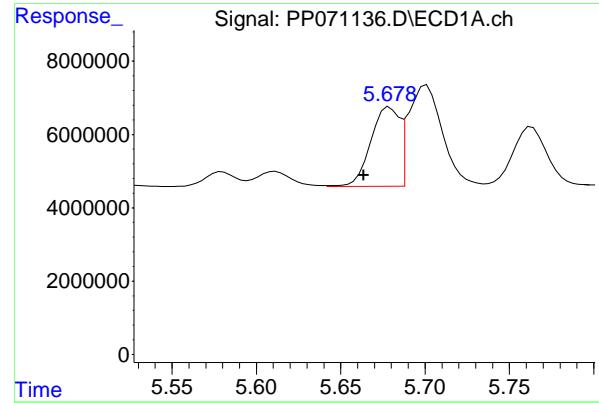

#3 AR-1016-1

R.T.: 5.679 min  
 Delta R.T.: 0.016 min  
 Response: 25640835  
 Conc: 504.23 ng/ml

Instrument: ECD\_P  
 Client SampleId: AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/09/2025  
 Supervised By :mohammad ahmed 04/10/2025

#3 AR-1016-1





R.T.: 4.904 min  
 Delta R.T.: 0.001 min  
 Response: 19684563  
 Conc: 491.03 ng/ml

#4 AR-1016-2

R.T.: 5.700 min  
 Delta R.T.: 0.015 min  
 Response: 36881275  
 Conc: 472.51 ng/ml

#4 AR-1016-2

R.T.: 4.923 min  
 Delta R.T.: 0.001 min  
 Response: 27978272  
 Conc: 483.51 ng/ml

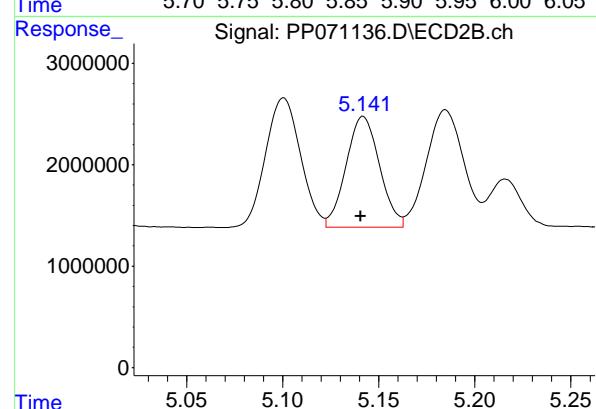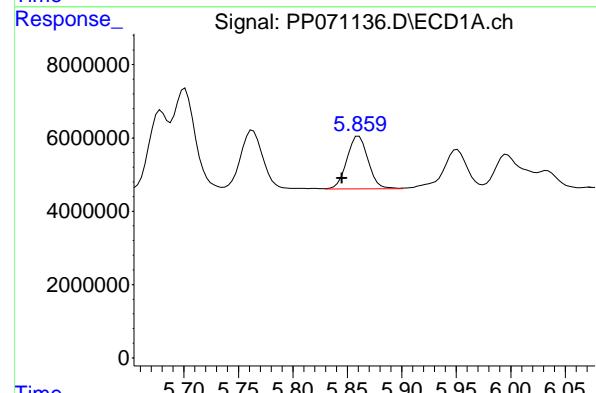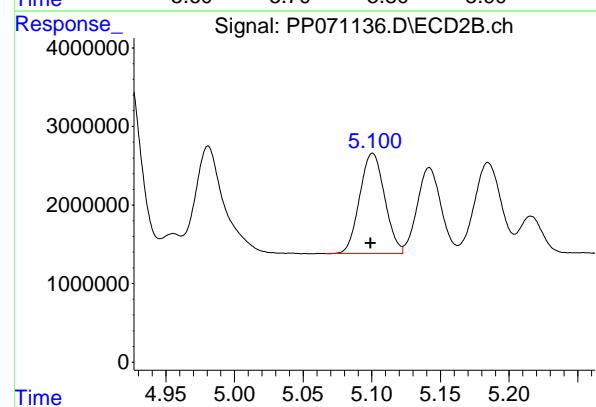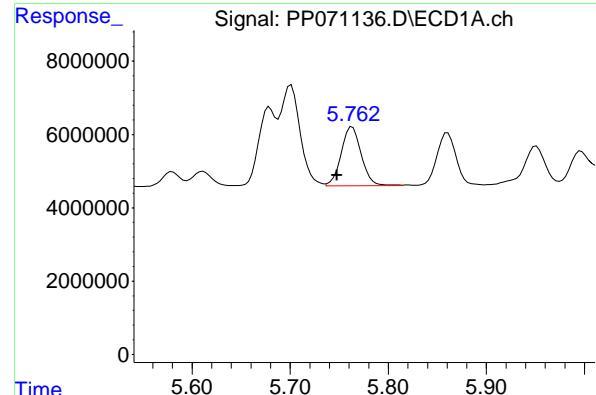

#5 AR-1016-3

R.T.: 5.763 min  
Delta R.T.: 0.016 min  
Instrument: ECD\_P  
Response: 23060044  
Conc: 488.82 ng/ml  
Client Sample Id: AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/09/2025  
Supervised By :mohammad ahmed 04/10/2025

#5 AR-1016-3


R.T.: 5.101 min  
Delta R.T.: 0.001 min  
Response: 16163902  
Conc: 522.71 ng/ml

#6 AR-1016-4

R.T.: 5.861 min  
Delta R.T.: 0.015 min  
Response: 19323906  
Conc: 525.74 ng/ml

#6 AR-1016-4

R.T.: 5.142 min  
Delta R.T.: 0.001 min  
Response: 13212574  
Conc: 542.48 ng/ml

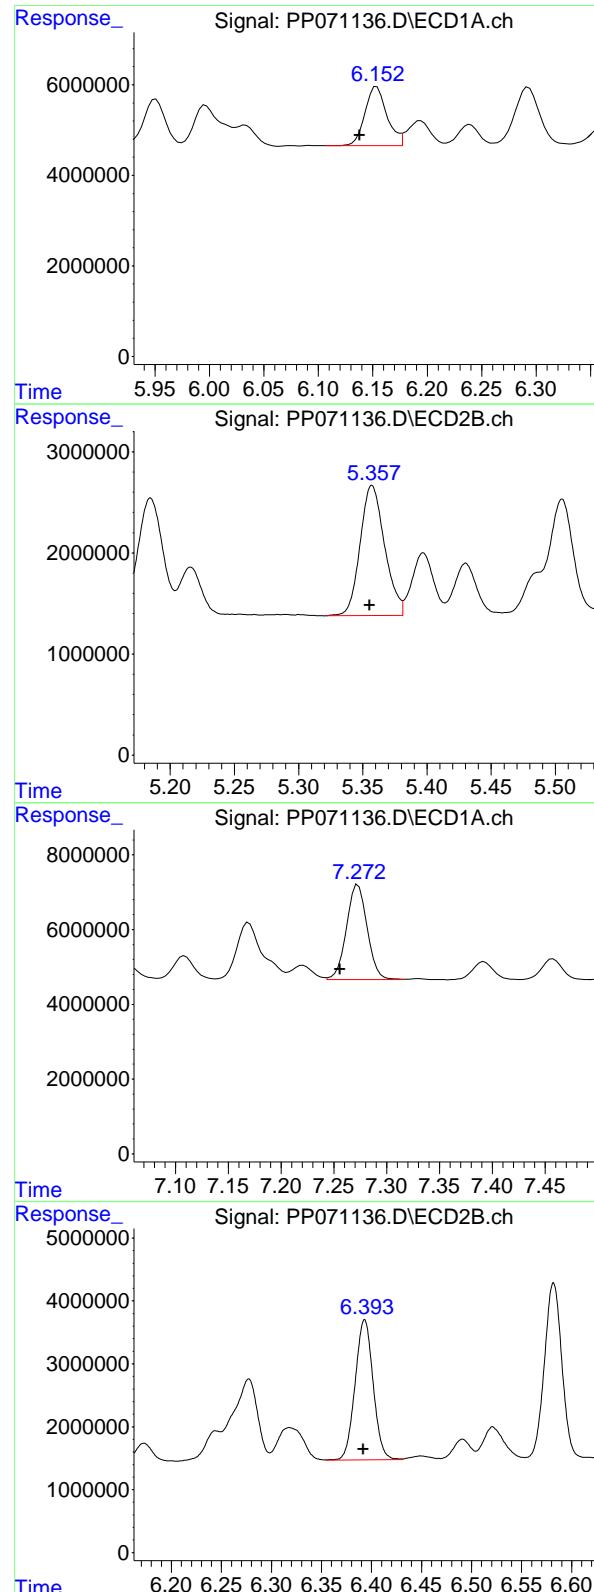

#7 AR-1016-5

R.T.: 6.154 min  
 Delta R.T.: 0.016 min  
 Response: 18307730  
 Conc: 539.86 ng/ml

Instrument: ECD\_P  
 Client SampleId: AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/09/2025  
 Supervised By :mohammad ahmed 04/10/2025

#7 AR-1016-5





R.T.: 5.357 min  
 Delta R.T.: 0.002 min  
 Response: 17134433  
 Conc: 530.13 ng/ml

#31 AR-1260-1

R.T.: 7.273 min  
 Delta R.T.: 0.017 min  
 Response: 34786874  
 Conc: 518.03 ng/ml

#31 AR-1260-1

R.T.: 6.393 min  
 Delta R.T.: 0.001 min  
 Response: 28041460  
 Conc: 547.62 ng/ml

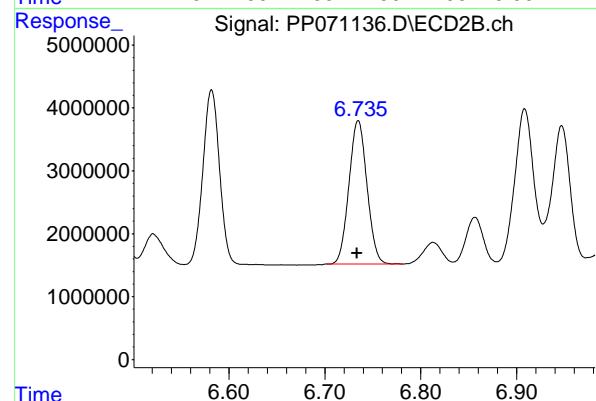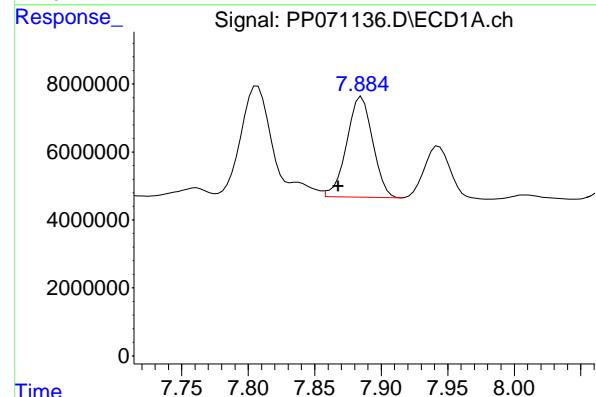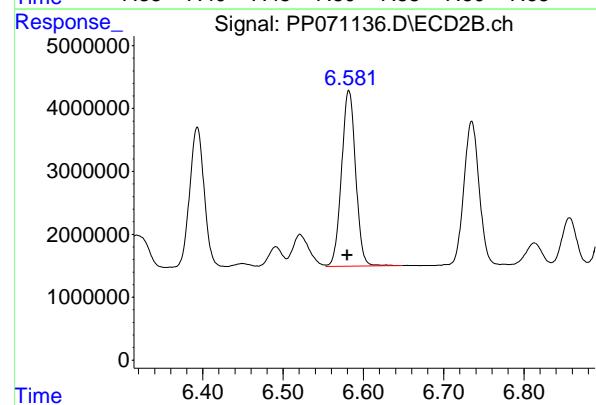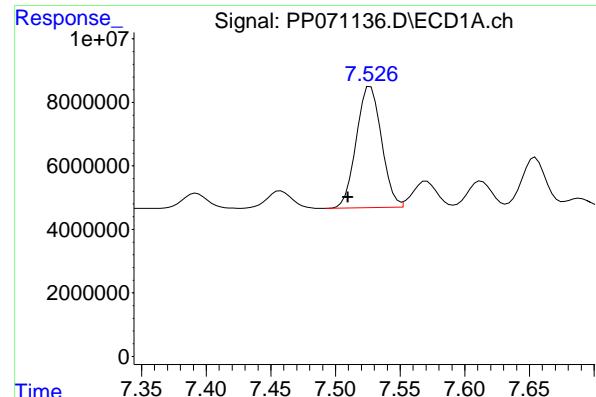

#32 AR-1260-2

R.T.: 7.527 min  
 Delta R.T.: 0.017 min  
 Response: 51604417 ECD\_P  
 Conc: 536.78 ng/ml Client SampleId : AR1660CCC500

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/09/2025  
 Supervised By :mohammad ahmed 04/10/2025

#32 AR-1260-2


R.T.: 6.582 min  
 Delta R.T.: 0.002 min  
 Response: 34095263  
 Conc: 534.46 ng/ml

#33 AR-1260-3

R.T.: 7.885 min  
 Delta R.T.: 0.018 min  
 Response: 40227656  
 Conc: 503.36 ng/ml

#33 AR-1260-3

R.T.: 6.735 min  
 Delta R.T.: 0.001 min  
 Response: 29796945  
 Conc: 546.87 ng/ml

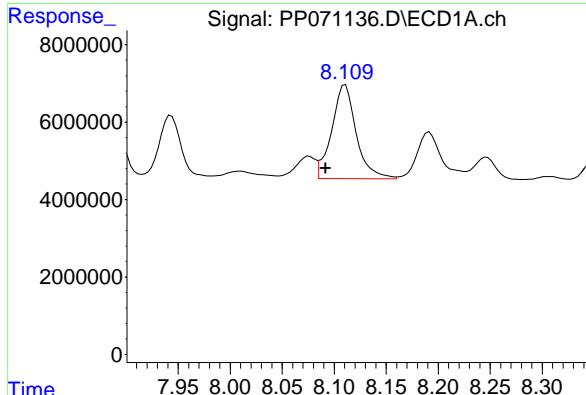


#34 AR-1260-4

R.T.: 8.109 min  
 Delta R.T.: 0.018 min  
 Response: 39475978  
 Conc: 501.37 ng/ml

Instrument: ECD\_P  
 Client SampleId: AR1660CCC500


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/09/2025  
 Supervised By :mohammad ahmed 04/10/2025

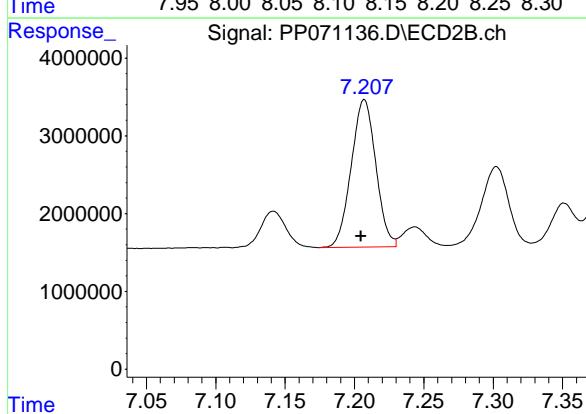


#34 AR-1260-4

R.T.: 7.207 min  
 Delta R.T.: 0.002 min  
 Response: 23421548  
 Conc: 489.72 ng/ml

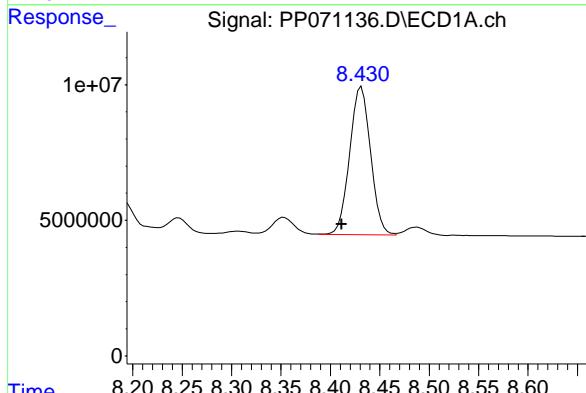

#35 AR-1260-5

R.T.: 8.431 min  
 Delta R.T.: 0.020 min  
 Response: 80513512  
 Conc: 506.74 ng/ml

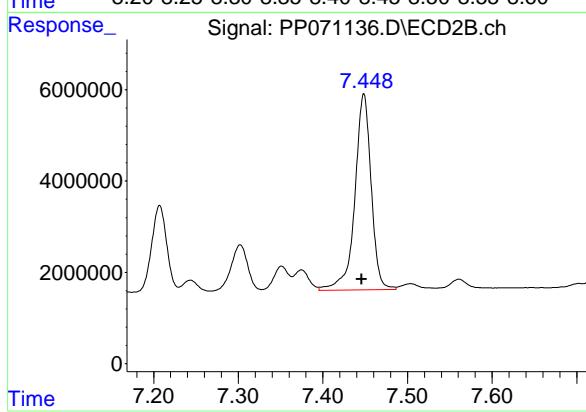

#35 AR-1260-5

R.T.: 7.448 min  
 Delta R.T.: 0.002 min  
 Response: 57532352  
 Conc: 462.07 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/08/2025 Initial Calibration Date(s): 03/27/2025 03/27/2025

Continuing Calib Time: 15:29 Initial Calibration Time(s): 10:30 17:53

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	5.67	5.66	5.56	5.76	-0.01
Aroclor-1016-2 (2)	5.69	5.69	5.59	5.79	0.00
Aroclor-1016-3 (3)	5.76	5.75	5.65	5.85	-0.01
Aroclor-1016-4 (4)	5.85	5.85	5.75	5.95	0.00
Aroclor-1016-5 (5)	6.15	6.14	6.04	6.24	-0.01
Aroclor-1260-1 (1)	7.27	7.26	7.16	7.36	0.00
Aroclor-1260-2 (2)	7.52	7.51	7.41	7.61	-0.01
Aroclor-1260-3 (3)	7.88	7.87	7.77	7.97	-0.01
Aroclor-1260-4 (4)	8.10	8.09	7.99	8.19	-0.01
Aroclor-1260-5 (5)	8.42	8.41	8.31	8.51	-0.01
Tetrachloro-m-xylene	4.52	4.51	4.41	4.61	-0.01
Decachlorobiphenyl	10.24	10.23	10.13	10.33	-0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

Continuing Calib Date: 04/08/2025 Initial Calibration Date(s): 03/27/2025 03/27/2025

Continuing Calib Time: 15:29 Initial Calibration Time(s): 10:30 17:53

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
Aroclor-1016-1 (1)	4.90	4.90	4.80	5.00	0.00
Aroclor-1016-2 (2)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-3 (3)	5.10	5.10	5.00	5.20	0.00
Aroclor-1016-4 (4)	5.14	5.14	5.04	5.24	0.00
Aroclor-1016-5 (5)	5.36	5.36	5.26	5.46	0.00
Aroclor-1260-1 (1)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-2 (2)	6.58	6.58	6.48	6.68	0.00
Aroclor-1260-3 (3)	6.73	6.73	6.63	6.83	0.00
Aroclor-1260-4 (4)	7.20	7.21	7.11	7.31	0.01
Aroclor-1260-5 (5)	7.45	7.45	7.35	7.55	0.00
Tetrachloro-m-xylene	3.82	3.82	3.72	3.92	0.00
Decachlorobiphenyl	8.86	8.86	8.76	8.96	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR1 ID: 0.32 (mm) Init. Calib. Date(s): 03/27/2025 03/27/2025

Client Sample No.: CCAL07 Date Analyzed: 04/08/2025

Lab Sample No.: AR1660CCC500 Data File : PP071151.D Time Analyzed: 15:29

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	5.671	5.563	5.763	484.620	500.000	-3.1
Aroclor-1016-2	5.692	5.585	5.785	482.920	500.000	-3.4
Aroclor-1016-3	5.755	5.648	5.848	470.770	500.000	-5.8
Aroclor-1016-4	5.852	5.745	5.945	505.800	500.000	1.2
Aroclor-1016-5	6.146	6.038	6.238	510.370	500.000	2.1
Aroclor-1260-1	7.265	7.156	7.356	508.140	500.000	1.6
Aroclor-1260-2	7.519	7.410	7.610	516.880	500.000	3.4
Aroclor-1260-3	7.879	7.768	7.968	504.190	500.000	0.8
Aroclor-1260-4	8.103	7.992	8.192	470.830	500.000	-5.8
Aroclor-1260-5	8.424	8.311	8.511	486.490	500.000	-2.7
Decachlorobiphenyl	10.243	10.125	10.325	49.190	50.000	-1.6
Tetrachloro-m-xylene	4.516	4.412	4.612	50.490	50.000	1.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG NO.: Q1730

GC Column: ZB-MR2 ID: 0.32 (mm) Init. Calib. Date(s): 03/27/2025 03/27/2025

Client Sample No.: CCAL07 Date Analyzed: 04/08/2025

Lab Sample No.: AR1660CCC500 Data File : PP071151.D Time Analyzed: 15:29

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.902	4.803	5.003	520.460	500.000	4.1
Aroclor-1016-2	4.921	4.822	5.022	507.900	500.000	1.6
Aroclor-1016-3	5.098	4.999	5.199	543.550	500.000	8.7
Aroclor-1016-4	5.140	5.041	5.241	556.220	500.000	11.2
Aroclor-1016-5	5.355	5.255	5.455	535.660	500.000	7.1
Aroclor-1260-1	6.390	6.292	6.492	521.040	500.000	4.2
Aroclor-1260-2	6.579	6.480	6.680	514.470	500.000	2.9
Aroclor-1260-3	6.732	6.634	6.834	529.510	500.000	5.9
Aroclor-1260-4	7.204	7.105	7.305	494.430	500.000	-1.1
Aroclor-1260-5	7.446	7.346	7.546	448.730	500.000	-10.3
Decachlorobiphenyl	8.859	8.759	8.959	40.800	50.000	-18.4
Tetrachloro-m-xylene	3.816	3.716	3.916	47.690	50.000	-4.6

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071151.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 15:29  
 Operator : YP\AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 15:40:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.516	3.816	73793328	49435615	50.489	47.688
2) SA Decachlor...	10.243	8.859	51773119	32161650	49.185	40.804

Target Compounds

3) L1 AR-1016-1	5.671	4.902	24643519	20864142	484.620	520.456
4) L1 AR-1016-2	5.692	4.921	37693781	29389805	482.922	507.902
5) L1 AR-1016-3	5.755	5.098	22208174	16808495	470.765	543.554
6) L1 AR-1016-4	5.852	5.140	18590980	13547316	505.798	556.223
7) L1 AR-1016-5	6.146	5.355	17307697	17313298	510.369	535.664
31) L7 AR-1260-1	7.265	6.390	34122856	26680779	508.137	521.045
32) L7 AR-1260-2	7.519	6.579	49691070	32819802	516.881	514.467
33) L7 AR-1260-3	7.879	6.732	40293738	28851540	504.187	529.514
34) L7 AR-1260-4	8.103	7.204	37071987	23646683	470.834	494.429
35) L7 AR-1260-5	8.424	7.446	77297206	55871530	486.494	448.730



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071151.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 15:29  
 Operator : YP\AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1660CCC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 15:40:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

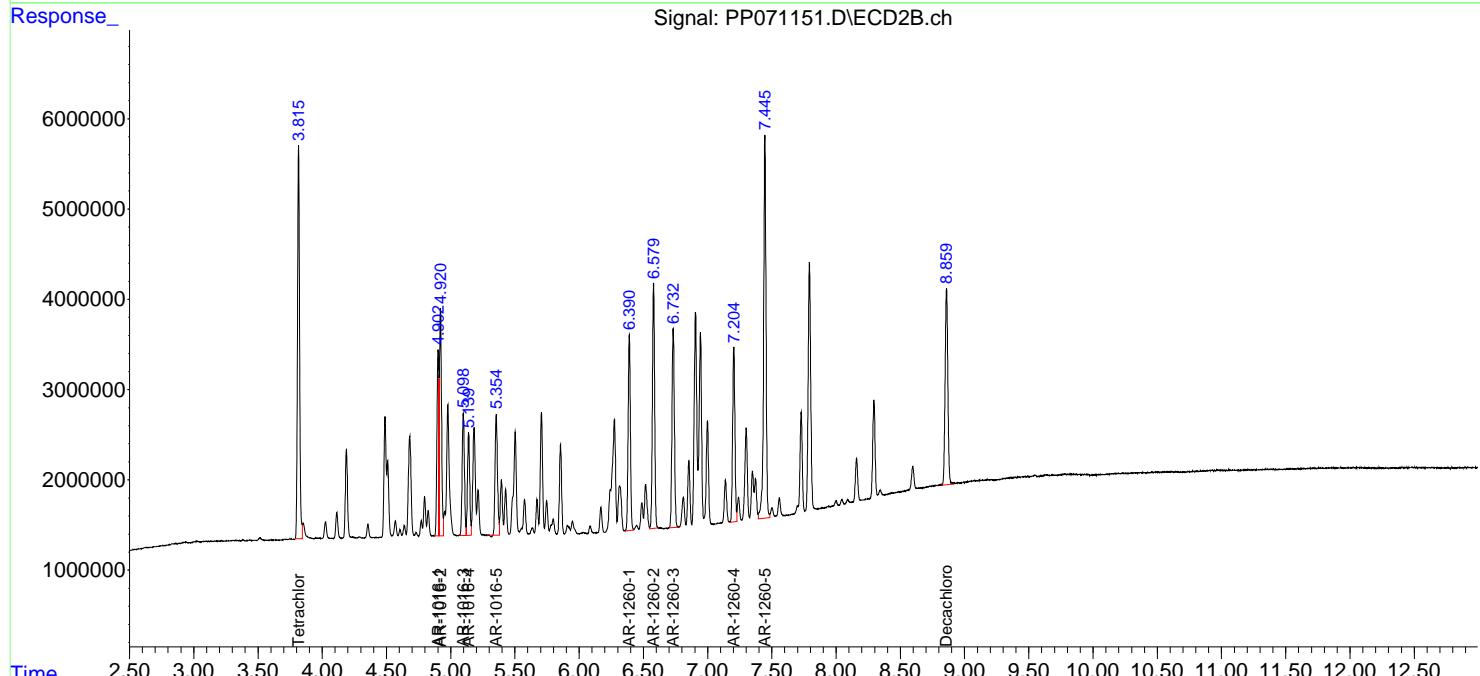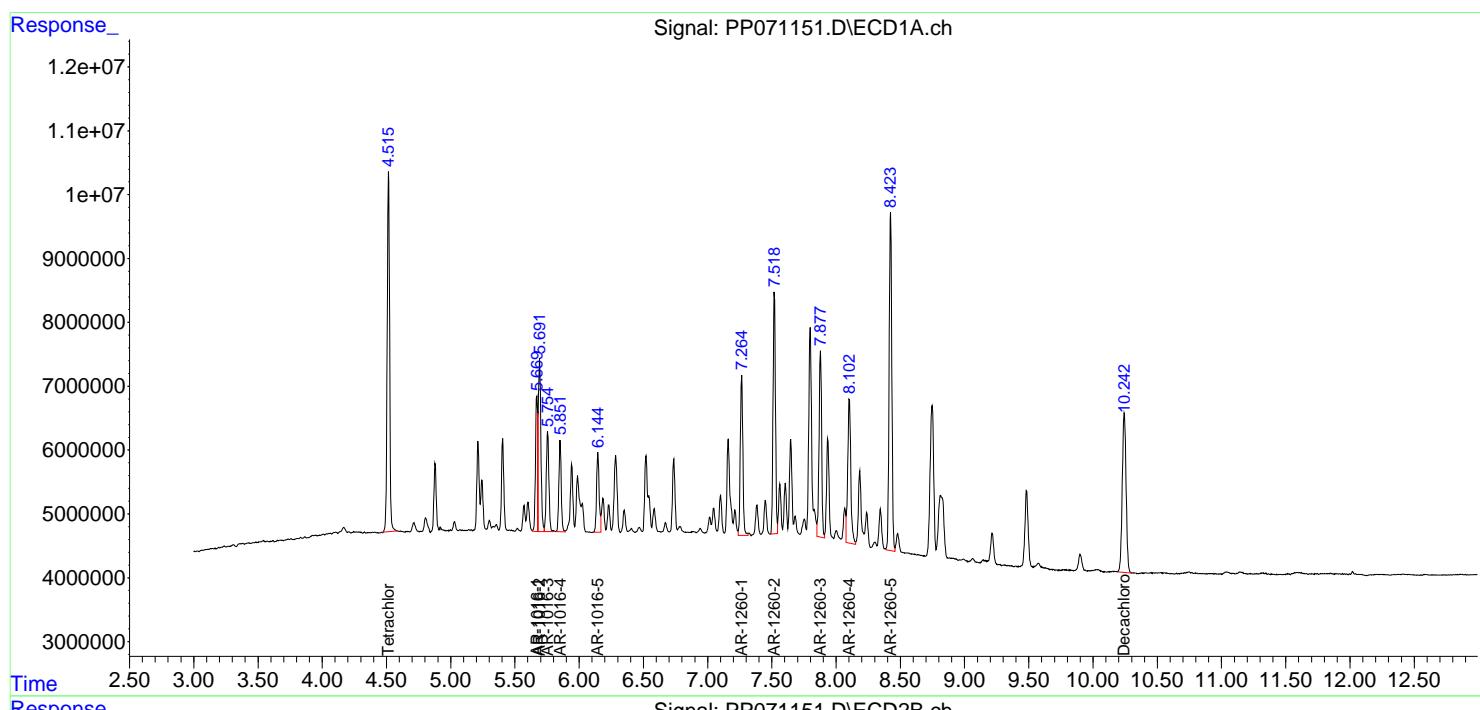

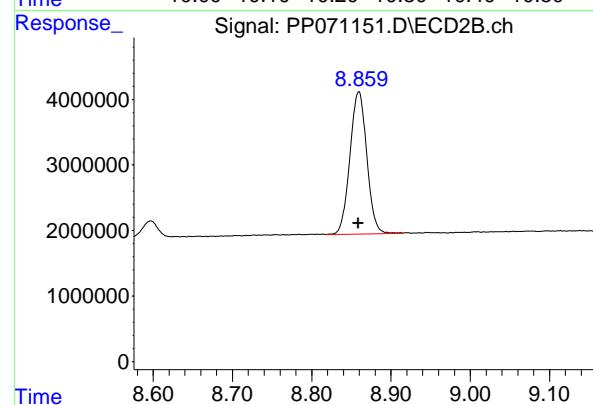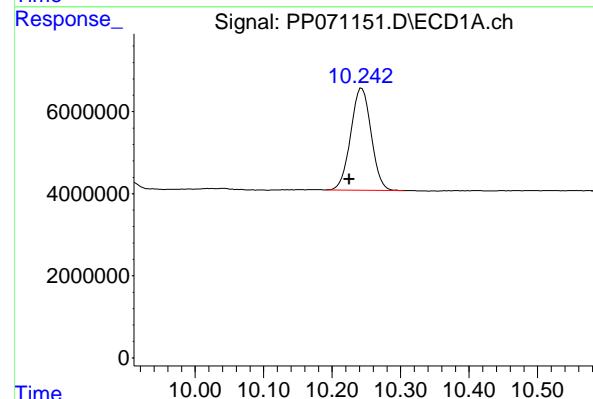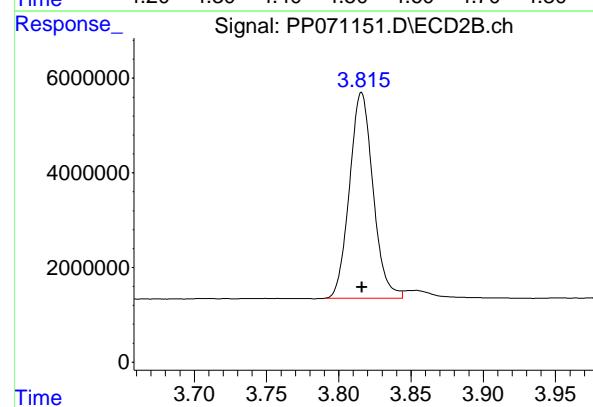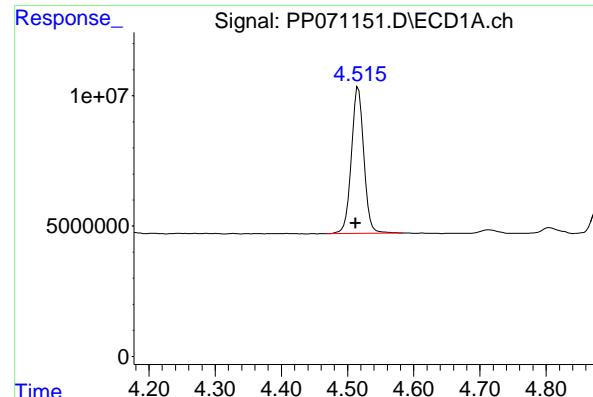

## #1 Tetrachloro-m-xylene

R.T.: 4.516 min  
Delta R.T.: 0.004 min  
Instrument: ECD\_P  
Response: 73793328  
Conc: 50.49 ng/ml  
ClientSampleId: AR1660CCC500

## #1 Tetrachloro-m-xylene





R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 49435615  
Conc: 47.69 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.243 min  
Delta R.T.: 0.018 min  
Response: 51773119  
Conc: 49.19 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 32161650  
Conc: 40.80 ng/ml

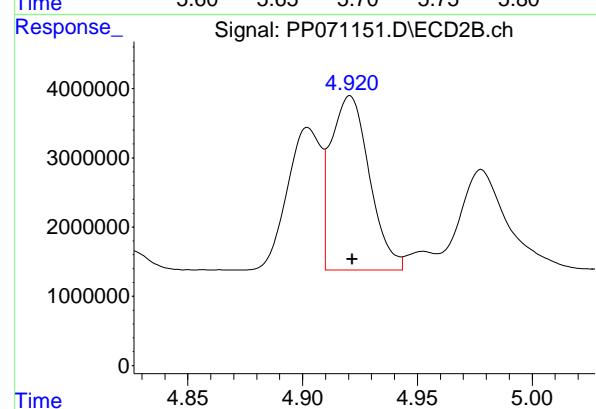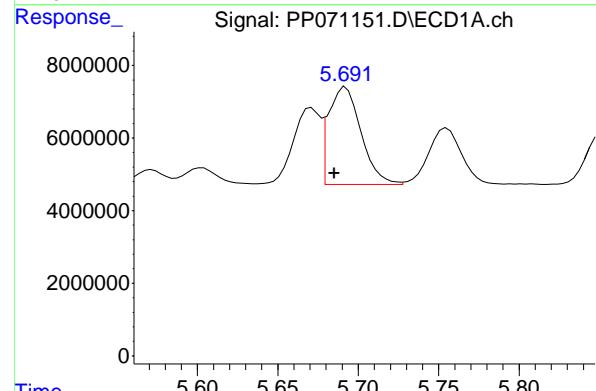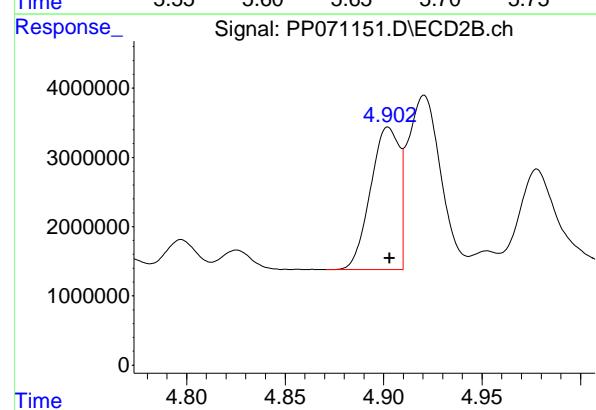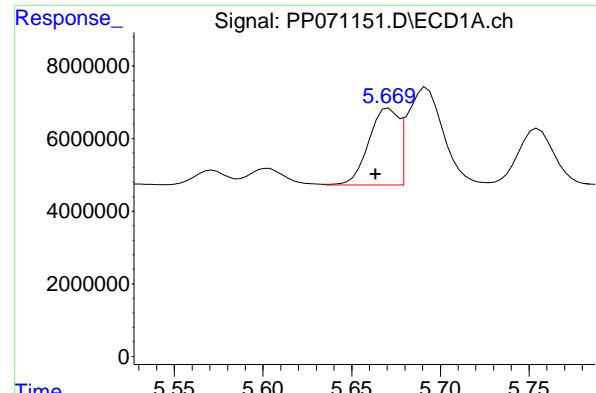

#3 AR-1016-1

R.T.: 5.671 min  
 Delta R.T.: 0.007 min  
 Response: 24643519  
 Conc: 484.62 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#3 AR-1016-1





R.T.: 4.902 min  
 Delta R.T.: 0.000 min  
 Response: 20864142  
 Conc: 520.46 ng/ml

#4 AR-1016-2

R.T.: 5.692 min  
 Delta R.T.: 0.007 min  
 Response: 37693781  
 Conc: 482.92 ng/ml

#4 AR-1016-2

R.T.: 4.921 min  
 Delta R.T.: 0.000 min  
 Response: 29389805  
 Conc: 507.90 ng/ml

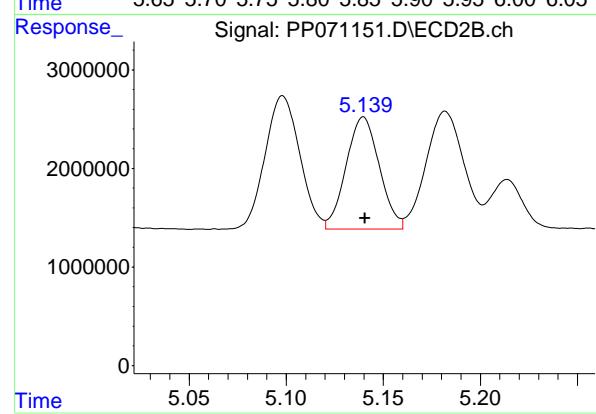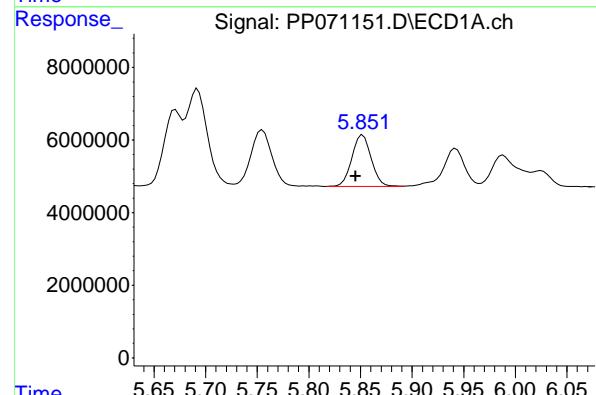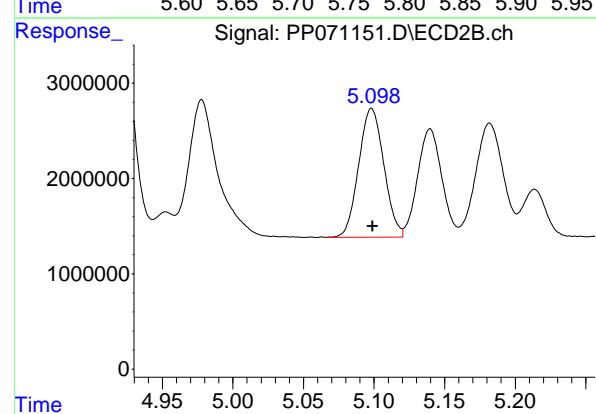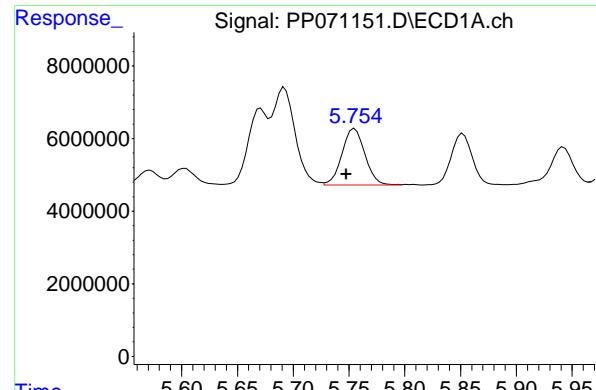

#5 AR-1016-3

R.T.: 5.755 min  
 Delta R.T.: 0.007 min  
 Response: 22208174 ECD\_P  
 Conc: 470.77 ng/ml Client SampleId : AR1660CCC500

#5 AR-1016-3





R.T.: 5.098 min  
 Delta R.T.: 0.000 min  
 Response: 16808495  
 Conc: 543.55 ng/ml

#6 AR-1016-4

R.T.: 5.852 min  
 Delta R.T.: 0.007 min  
 Response: 18590980  
 Conc: 505.80 ng/ml

#6 AR-1016-4

R.T.: 5.140 min  
 Delta R.T.: 0.000 min  
 Response: 13547316  
 Conc: 556.22 ng/ml

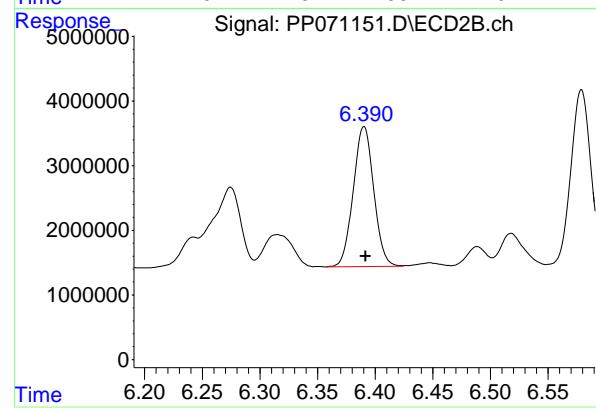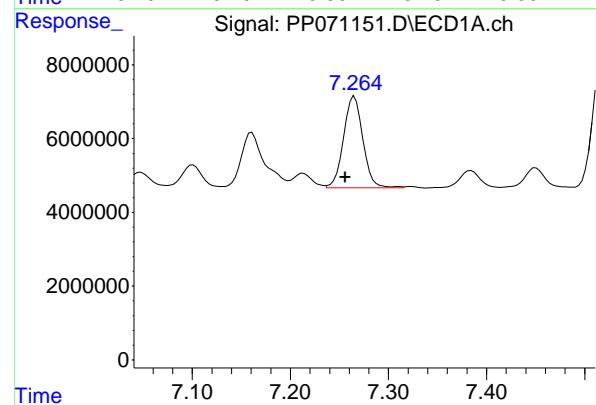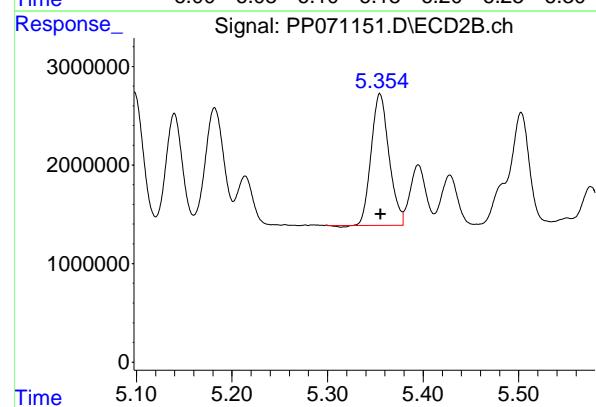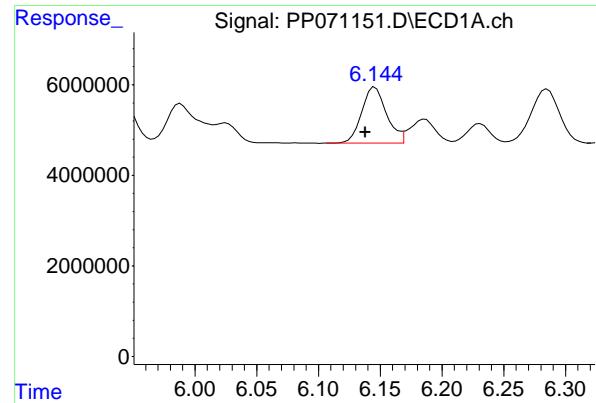

#7 AR-1016-5

R.T.: 6.146 min  
 Delta R.T.: 0.008 min  
 Response: 17307697  
 Conc: 510.37 ng/ml  
**Instrument:** ECD\_P  
**ClientSampleId:** AR1660CCC500

#7 AR-1016-5


R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 17313298  
 Conc: 535.66 ng/ml

#31 AR-1260-1

R.T.: 7.265 min  
 Delta R.T.: 0.009 min  
 Response: 34122856  
 Conc: 508.14 ng/ml

#31 AR-1260-1

R.T.: 6.390 min  
 Delta R.T.: -0.002 min  
 Response: 26680779  
 Conc: 521.04 ng/ml

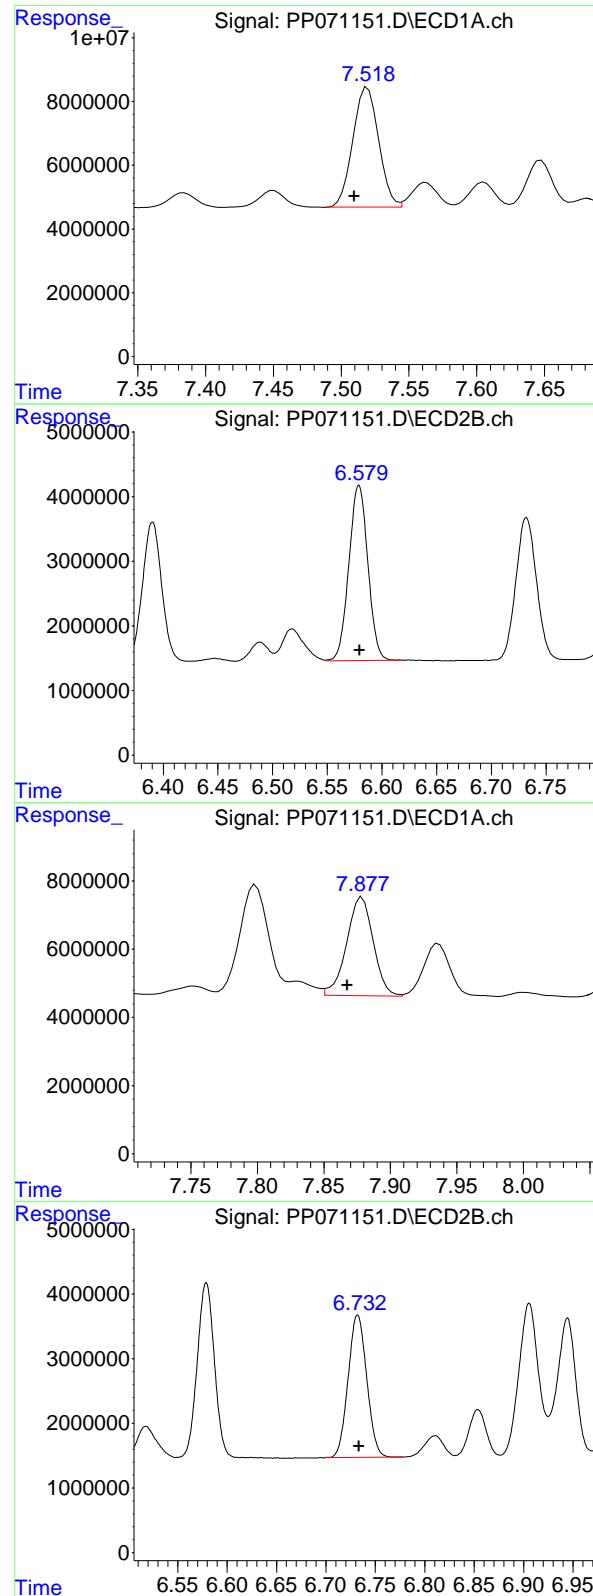

#32 AR-1260-2

R.T.: 7.519 min  
 Delta R.T.: 0.010 min  
 Response: 49691070 ECD\_P  
 Conc: 516.88 ng/ml ClientSampleId : AR1660CCC500

#32 AR-1260-2


R.T.: 6.579 min  
 Delta R.T.: 0.000 min  
 Response: 32819802  
 Conc: 514.47 ng/ml

#33 AR-1260-3

R.T.: 7.879 min  
 Delta R.T.: 0.011 min  
 Response: 40293738  
 Conc: 504.19 ng/ml


#33 AR-1260-3

R.T.: 6.732 min  
 Delta R.T.: -0.002 min  
 Response: 28851540  
 Conc: 529.51 ng/ml

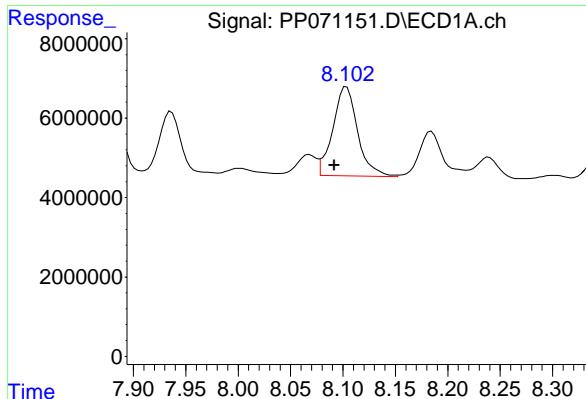


#34 AR-1260-4

R.T.: 8.103 min  
 Delta R.T.: 0.012 min  
 Response: 37071987 ECD\_P  
 Conc: 470.83 ng/ml ClientSampleId : AR1660CCC500

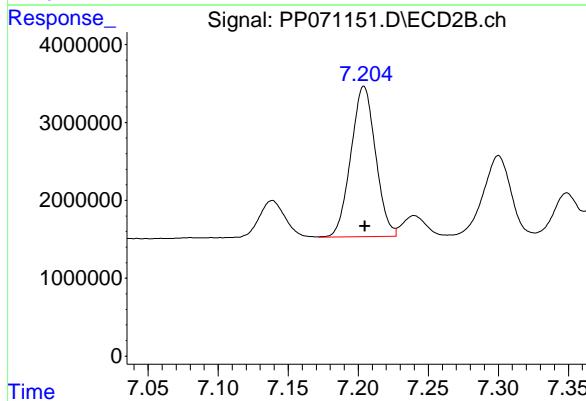


#34 AR-1260-4

R.T.: 7.204 min  
 Delta R.T.: 0.000 min  
 Response: 23646683  
 Conc: 494.43 ng/ml

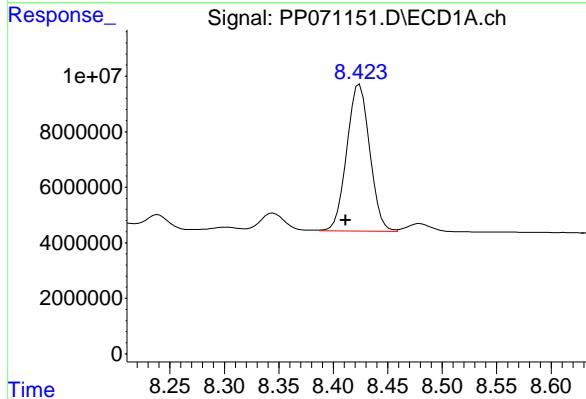

#35 AR-1260-5

R.T.: 8.424 min  
 Delta R.T.: 0.013 min  
 Response: 77297206  
 Conc: 486.49 ng/ml

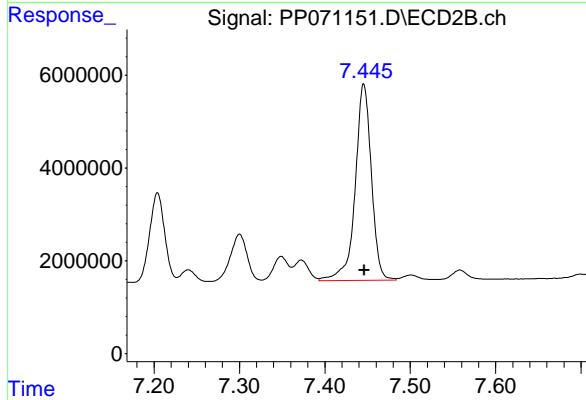

#35 AR-1260-5

R.T.: 7.446 min  
 Delta R.T.: 0.000 min  
 Response: 55871530  
 Conc: 448.73 ng/ml

## Analytical Sequence

Client: Nobis Group	SDG No.: Q1730		
Project: Raymark Superfund Site	Instrument ID: ECD_O		
GC Column: ZB-MR1	ID: 0.32 (mm)	Inst. Calib. Date(s): 03/18/2025	03/18/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES, AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
I.BLK	I.BLK	03/18/2025	13:44	PO109971.D	8.74	3.69
AR1660ICC1000	AR1660ICC1000	03/18/2025	14:03	PO109972.D	8.75	3.69
AR1660ICC750	AR1660ICC750	03/18/2025	14:21	PO109973.D	8.75	3.69
AR1660ICC500	AR1660ICC500	03/18/2025	14:39	PO109974.D	8.75	3.69
AR1660ICC250	AR1660ICC250	03/18/2025	14:58	PO109975.D	8.75	3.69
AR1660ICC050	AR1660ICC050	03/18/2025	15:16	PO109976.D	8.74	3.69
AR1221ICC500	AR1221ICC500	03/18/2025	15:34	PO109977.D	8.74	3.69
AR1232ICC500	AR1232ICC500	03/18/2025	15:53	PO109978.D	8.74	3.69
AR1242ICC1000	AR1242ICC1000	03/18/2025	16:11	PO109979.D	8.74	3.69
AR1242ICC750	AR1242ICC750	03/18/2025	16:30	PO109980.D	8.74	3.69
AR1242ICC500	AR1242ICC500	03/18/2025	16:48	PO109981.D	8.74	3.69
AR1242ICC250	AR1242ICC250	03/18/2025	17:06	PO109982.D	8.74	3.69
AR1242ICC050	AR1242ICC050	03/18/2025	17:25	PO109983.D	8.74	3.69
AR1248ICC1000	AR1248ICC1000	03/18/2025	17:42	PO109984.D	8.74	3.69
AR1248ICC750	AR1248ICC750	03/18/2025	18:00	PO109985.D	8.74	3.69
AR1248ICC500	AR1248ICC500	03/18/2025	18:19	PO109986.D	8.74	3.69
AR1248ICC250	AR1248ICC250	03/18/2025	18:37	PO109987.D	8.74	3.69
AR1248ICC050	AR1248ICC050	03/18/2025	18:54	PO109988.D	8.74	3.69
AR1254ICC1000	AR1254ICC1000	03/18/2025	19:13	PO109989.D	8.74	3.69
AR1254ICC750	AR1254ICC750	03/18/2025	19:31	PO109990.D	8.74	3.69
AR1254ICC500	AR1254ICC500	03/18/2025	19:49	PO109991.D	8.74	3.69
AR1254ICC250	AR1254ICC250	03/18/2025	20:07	PO109992.D	8.74	3.69
AR1254ICC050	AR1254ICC050	03/18/2025	20:25	PO109993.D	8.74	3.69
AR1262ICC500	AR1262ICC500	03/18/2025	20:43	PO109994.D	8.74	3.69
AR1268ICC1000	AR1268ICC1000	03/18/2025	21:02	PO109995.D	8.74	3.69
AR1268ICC750	AR1268ICC750	03/18/2025	21:20	PO109996.D	8.74	3.69
AR1268ICC500	AR1268ICC500	03/18/2025	21:39	PO109997.D	8.74	3.69
AR1268ICC250	AR1268ICC250	03/18/2025	21:57	PO109998.D	8.74	3.69
AR1268ICC050	AR1268ICC050	03/18/2025	22:15	PO109999.D	8.74	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	09:46	PO110263.D	8.74	3.69
I.BLK	I.BLK	04/07/2025	11:36	PO110267.D	8.74	3.69
OU4-VSL-15-040325	Q1730-01	04/07/2025	13:38	PO110269.D	8.74	3.69
OU4-VSL-16-040325	Q1730-03	04/07/2025	13:56	PO110270.D	8.74	3.69
OU4-VSL-16-040325MS	Q1730-03MS	04/07/2025	14:15	PO110271.D	8.74	3.69
OU4-VSL-16-040325MSD	Q1730-03MSD	04/07/2025	14:33	PO110272.D	8.74	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	17:14	PO110278.D	8.74	3.69
I.BLK	I.BLK	04/07/2025	19:04	PO110282.D	8.74	3.69
PB167469BL	PB167469BL	04/07/2025	19:22	PO110283.D	8.74	3.69
PB167469BS	PB167469BS	04/07/2025	19:41	PO110284.D	8.74	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	21:27	PO110286.D	8.74	3.69
I.BLK	I.BLK	04/07/2025	23:17	PO110290.D	8.74	3.69
AR1660CCC500	AR1660CCC500	04/08/2025	09:08	PO110292.D	8.74	3.69

### Analytical Sequence

I.BLK	I.BLK	04/08/2025	10:21	PO110296.D	8.74	3.69
OU4-VSL-17-040325	Q1730-05	04/08/2025	10:39	PO110297.D	8.74	3.69
OU4-PCS-TC-21-040325	Q1730-07	04/08/2025	10:58	PO110298.D	8.74	3.69
OU4-PCS-TC-22-040325	Q1730-09	04/08/2025	11:16	PO110299.D	8.74	3.69
OU4-PCS-TC-23-040325	Q1730-11	04/08/2025	11:35	PO110300.D	8.74	3.69
OU4-PCS-TC-24-040325	Q1730-13	04/08/2025	11:53	PO110301.D	8.74	3.69
AR1660CCC500	AR1660CCC500	04/08/2025	12:58	PO110302.D	8.74	3.69
I.BLK	I.BLK	04/08/2025	14:12	PO110306.D	8.74	3.69
I.BLK	I.BLK	03/27/2025	10:14	PP070916.D	10.23	4.51
AR1660ICC1000	AR1660ICC1000	03/27/2025	10:30	PP070917.D	10.23	4.51
AR1660ICC750	AR1660ICC750	03/27/2025	10:47	PP070918.D	10.23	4.52
AR1660ICC500	AR1660ICC500	03/27/2025	11:03	PP070919.D	10.23	4.51
AR1660ICC250	AR1660ICC250	03/27/2025	11:19	PP070920.D	10.23	4.52
AR1660ICC050	AR1660ICC050	03/27/2025	11:35	PP070921.D	10.23	4.51
AR1221ICC500	AR1221ICC500	03/27/2025	11:52	PP070922.D	10.23	4.52
AR1232ICC500	AR1232ICC500	03/27/2025	12:11	PP070923.D	10.23	4.52
AR1242ICC1000	AR1242ICC1000	03/27/2025	12:28	PP070924.D	10.23	4.51
AR1242ICC750	AR1242ICC750	03/27/2025	12:44	PP070925.D	10.23	4.51
AR1242ICC500	AR1242ICC500	03/27/2025	13:00	PP070926.D	10.23	4.51
AR1242ICC250	AR1242ICC250	03/27/2025	13:16	PP070927.D	10.23	4.51
AR1242ICC050	AR1242ICC050	03/27/2025	13:33	PP070928.D	10.23	4.51
AR1248ICC1000	AR1248ICC1000	03/27/2025	13:49	PP070929.D	10.23	4.51
AR1248ICC750	AR1248ICC750	03/27/2025	14:05	PP070930.D	10.23	4.51
AR1248ICC500	AR1248ICC500	03/27/2025	14:22	PP070931.D	10.23	4.51
AR1248ICC250	AR1248ICC250	03/27/2025	14:38	PP070932.D	10.23	4.52
AR1248ICC050	AR1248ICC050	03/27/2025	14:55	PP070933.D	10.23	4.51
AR1254ICC1000	AR1254ICC1000	03/27/2025	15:11	PP070934.D	10.23	4.51
AR1254ICC750	AR1254ICC750	03/27/2025	15:27	PP070935.D	10.23	4.51
AR1254ICC500	AR1254ICC500	03/27/2025	15:43	PP070936.D	10.23	4.51
AR1254ICC250	AR1254ICC250	03/27/2025	16:00	PP070937.D	10.23	4.51
AR1254ICC050	AR1254ICC050	03/27/2025	16:16	PP070938.D	10.23	4.52
AR1262ICC500	AR1262ICC500	03/27/2025	16:32	PP070939.D	10.23	4.51
AR1268ICC1000	AR1268ICC1000	03/27/2025	16:48	PP070940.D	10.23	4.52
AR1268ICC750	AR1268ICC750	03/27/2025	17:05	PP070941.D	10.23	4.51
AR1268ICC500	AR1268ICC500	03/27/2025	17:21	PP070942.D	10.23	4.51
AR1268ICC250	AR1268ICC250	03/27/2025	17:37	PP070943.D	10.23	4.52
AR1268ICC050	AR1268ICC050	03/27/2025	17:53	PP070944.D	10.23	4.51
AR1660CCC500	AR1660CCC500	04/08/2025	09:37	PP071136.D	10.26	4.52
I.BLK	I.BLK	04/08/2025	11:05	PP071140.D	10.25	4.52
OU4-PCS-TC-25-040325	Q1730-15	04/08/2025	11:39	PP071142.D	10.24	4.51
OU4-PCS-TC-26-040325	Q1730-17	04/08/2025	11:56	PP071143.D	10.25	4.52
OU4-CF-15-040325	Q1730-19	04/08/2025	12:12	PP071144.D	10.24	4.52
AR1660CCC500	AR1660CCC500	04/08/2025	15:29	PP071151.D	10.24	4.52
I.BLK	I.BLK	04/08/2025	16:51	PP071155.D	10.24	4.52

## Analytical Sequence

Client: Nobis Group	SDG No.: Q1730		
Project: Raymark Superfund Site	Instrument ID: ECD_O		
GC Column: ZB-MR2	ID: 0.32 (mm)	Inst. Calib. Date(s): 03/18/2025	03/18/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES, AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
I.BLK	I.BLK	03/18/2025	13:44	PO109971.D	8.70	3.69
AR1660ICC1000	AR1660ICC1000	03/18/2025	14:03	PO109972.D	8.70	3.69
AR1660ICC750	AR1660ICC750	03/18/2025	14:21	PO109973.D	8.70	3.69
AR1660ICC500	AR1660ICC500	03/18/2025	14:39	PO109974.D	8.70	3.69
AR1660ICC250	AR1660ICC250	03/18/2025	14:58	PO109975.D	8.70	3.69
AR1660ICC050	AR1660ICC050	03/18/2025	15:16	PO109976.D	8.70	3.69
AR1221ICC500	AR1221ICC500	03/18/2025	15:34	PO109977.D	8.70	3.69
AR1232ICC500	AR1232ICC500	03/18/2025	15:53	PO109978.D	8.70	3.69
AR1242ICC1000	AR1242ICC1000	03/18/2025	16:11	PO109979.D	8.70	3.69
AR1242ICC750	AR1242ICC750	03/18/2025	16:30	PO109980.D	8.70	3.69
AR1242ICC500	AR1242ICC500	03/18/2025	16:48	PO109981.D	8.70	3.69
AR1242ICC250	AR1242ICC250	03/18/2025	17:06	PO109982.D	8.70	3.69
AR1242ICC050	AR1242ICC050	03/18/2025	17:25	PO109983.D	8.70	3.69
AR1248ICC1000	AR1248ICC1000	03/18/2025	17:42	PO109984.D	8.70	3.69
AR1248ICC750	AR1248ICC750	03/18/2025	18:00	PO109985.D	8.70	3.69
AR1248ICC500	AR1248ICC500	03/18/2025	18:19	PO109986.D	8.70	3.69
AR1248ICC250	AR1248ICC250	03/18/2025	18:37	PO109987.D	8.70	3.69
AR1248ICC050	AR1248ICC050	03/18/2025	18:54	PO109988.D	8.70	3.69
AR1254ICC1000	AR1254ICC1000	03/18/2025	19:13	PO109989.D	8.69	3.69
AR1254ICC750	AR1254ICC750	03/18/2025	19:31	PO109990.D	8.70	3.69
AR1254ICC500	AR1254ICC500	03/18/2025	19:49	PO109991.D	8.70	3.69
AR1254ICC250	AR1254ICC250	03/18/2025	20:07	PO109992.D	8.70	3.69
AR1254ICC050	AR1254ICC050	03/18/2025	20:25	PO109993.D	8.69	3.69
AR1262ICC500	AR1262ICC500	03/18/2025	20:43	PO109994.D	8.70	3.69
AR1268ICC1000	AR1268ICC1000	03/18/2025	21:02	PO109995.D	8.70	3.69
AR1268ICC750	AR1268ICC750	03/18/2025	21:20	PO109996.D	8.70	3.69
AR1268ICC500	AR1268ICC500	03/18/2025	21:39	PO109997.D	8.69	3.69
AR1268ICC250	AR1268ICC250	03/18/2025	21:57	PO109998.D	8.70	3.69
AR1268ICC050	AR1268ICC050	03/18/2025	22:15	PO109999.D	8.70	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	09:46	PO110263.D	8.69	3.69
I.BLK	I.BLK	04/07/2025	11:36	PO110267.D	8.69	3.69
OU4-VSL-15-040325	Q1730-01	04/07/2025	13:38	PO110269.D	8.69	3.69
OU4-VSL-16-040325	Q1730-03	04/07/2025	13:56	PO110270.D	8.69	3.69
OU4-VSL-16-040325MS	Q1730-03MS	04/07/2025	14:15	PO110271.D	8.69	3.69
OU4-VSL-16-040325MSD	Q1730-03MSD	04/07/2025	14:33	PO110272.D	8.69	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	17:14	PO110278.D	8.69	3.69
I.BLK	I.BLK	04/07/2025	19:04	PO110282.D	8.69	3.69
PB167469BL	PB167469BL	04/07/2025	19:22	PO110283.D	8.69	3.69
PB167469BS	PB167469BS	04/07/2025	19:41	PO110284.D	8.69	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	21:27	PO110286.D	8.69	3.69
I.BLK	I.BLK	04/07/2025	23:17	PO110290.D	8.69	3.69
AR1660CCC500	AR1660CCC500	04/08/2025	09:08	PO110292.D	8.69	3.69

### Analytical Sequence

I.BLK	I.BLK	04/08/2025	10:21	PO110296.D	8.69	3.69
OU4-VSL-17-040325	Q1730-05	04/08/2025	10:39	PO110297.D	8.69	3.69
OU4-PCS-TC-21-040325	Q1730-07	04/08/2025	10:58	PO110298.D	8.69	3.69
OU4-PCS-TC-22-040325	Q1730-09	04/08/2025	11:16	PO110299.D	8.69	3.69
OU4-PCS-TC-23-040325	Q1730-11	04/08/2025	11:35	PO110300.D	8.69	3.69
OU4-PCS-TC-24-040325	Q1730-13	04/08/2025	11:53	PO110301.D	8.69	3.69
AR1660CCC500	AR1660CCC500	04/08/2025	12:58	PO110302.D	8.69	3.69
I.BLK	I.BLK	04/08/2025	14:12	PO110306.D	8.69	3.69
I.BLK	I.BLK	03/27/2025	10:14	PP070916.D	8.86	3.82
AR1660ICC1000	AR1660ICC1000	03/27/2025	10:30	PP070917.D	8.86	3.82
AR1660ICC750	AR1660ICC750	03/27/2025	10:47	PP070918.D	8.86	3.82
AR1660ICC500	AR1660ICC500	03/27/2025	11:03	PP070919.D	8.86	3.82
AR1660ICC250	AR1660ICC250	03/27/2025	11:19	PP070920.D	8.86	3.82
AR1660ICC050	AR1660ICC050	03/27/2025	11:35	PP070921.D	8.86	3.82
AR1221ICC500	AR1221ICC500	03/27/2025	11:52	PP070922.D	8.86	3.82
AR1232ICC500	AR1232ICC500	03/27/2025	12:11	PP070923.D	8.86	3.82
AR1242ICC1000	AR1242ICC1000	03/27/2025	12:28	PP070924.D	8.86	3.82
AR1242ICC750	AR1242ICC750	03/27/2025	12:44	PP070925.D	8.86	3.82
AR1242ICC500	AR1242ICC500	03/27/2025	13:00	PP070926.D	8.86	3.82
AR1242ICC250	AR1242ICC250	03/27/2025	13:16	PP070927.D	8.86	3.82
AR1242ICC050	AR1242ICC050	03/27/2025	13:33	PP070928.D	8.86	3.82
AR1248ICC1000	AR1248ICC1000	03/27/2025	13:49	PP070929.D	8.86	3.82
AR1248ICC750	AR1248ICC750	03/27/2025	14:05	PP070930.D	8.86	3.82
AR1248ICC500	AR1248ICC500	03/27/2025	14:22	PP070931.D	8.86	3.82
AR1248ICC250	AR1248ICC250	03/27/2025	14:38	PP070932.D	8.86	3.82
AR1248ICC050	AR1248ICC050	03/27/2025	14:55	PP070933.D	8.86	3.82
AR1254ICC1000	AR1254ICC1000	03/27/2025	15:11	PP070934.D	8.86	3.82
AR1254ICC750	AR1254ICC750	03/27/2025	15:27	PP070935.D	8.86	3.82
AR1254ICC500	AR1254ICC500	03/27/2025	15:43	PP070936.D	8.86	3.82
AR1254ICC250	AR1254ICC250	03/27/2025	16:00	PP070937.D	8.86	3.82
AR1254ICC050	AR1254ICC050	03/27/2025	16:16	PP070938.D	8.86	3.82
AR1262ICC500	AR1262ICC500	03/27/2025	16:32	PP070939.D	8.86	3.82
AR1268ICC1000	AR1268ICC1000	03/27/2025	16:48	PP070940.D	8.86	3.82
AR1268ICC750	AR1268ICC750	03/27/2025	17:05	PP070941.D	8.86	3.82
AR1268ICC500	AR1268ICC500	03/27/2025	17:21	PP070942.D	8.86	3.82
AR1268ICC250	AR1268ICC250	03/27/2025	17:37	PP070943.D	8.86	3.82
AR1268ICC050	AR1268ICC050	03/27/2025	17:53	PP070944.D	8.86	3.82
AR1660CCC500	AR1660CCC500	04/08/2025	09:37	PP071136.D	8.86	3.82
I.BLK	I.BLK	04/08/2025	11:05	PP071140.D	8.86	3.82
OU4-PCS-TC-25-040325	Q1730-15	04/08/2025	11:39	PP071142.D	8.86	3.82
OU4-PCS-TC-26-040325	Q1730-17	04/08/2025	11:56	PP071143.D	8.86	3.82
OU4-CF-15-040325	Q1730-19	04/08/2025	12:12	PP071144.D	8.86	3.82
AR1660CCC500	AR1660CCC500	04/08/2025	15:29	PP071151.D	8.86	3.82
I.BLK	I.BLK	04/08/2025	16:51	PP071155.D	8.86	3.82



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

IDENTIFICATION SUMMARY  
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

OU4-VSL-16-040325MS

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG No.: Q1730  
Lab Sample ID: Q1730-03MS Date(s) Analyzed: 04/07/2025 04/07/2025  
Instrument ID (1): ECD\_O Instrument ID (2): ECD\_O  
GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)  
Data file PO110271.D

ANALYTE	COL	RT	RT WINDOW FROM	TO	CONCENTRATION	MEAN CONCENTRATION	%RPD
Aroclor-1016	1	4.782	4.732	4.832	171	170	3.59
	2	4.802	4.752	4.852	172		
	3	4.858	4.808	4.908	172		
	4	4.978	4.928	5.028	171		
	5	5.236	5.186	5.286	163		
COLUMN 1	1	4.768	4.718	4.818	166	164	3.59
	2	4.787	4.737	4.837	166		
	3	4.963	4.913	5.013	166		
	4	5.005	4.955	5.055	163		
	5	5.218	5.168	5.268	159		
Aroclor-1260	1	6.276	6.226	6.326	178	157	3.9
	2	6.466	6.416	6.516	169		
	3	6.833	6.783	6.883	144		
	4	7.094	7.044	7.144	152		
	5	7.335	7.285	7.385	141		
COLUMN 1	1	6.25	6.2	6.3	164	151	3.9
	2	6.438	6.388	6.488	160		
	3	6.591	6.541	6.641	155		
	4	7.062	7.012	7.112	142		
	5	7.303	7.253	7.353	133		
COLUMN 2	1	6.25	6.2	6.3	164	151	3.9
	2	6.438	6.388	6.488	160		
	3	6.591	6.541	6.641	155		
	4	7.062	7.012	7.112	142		
	5	7.303	7.253	7.353	133		

**IDENTIFICATION SUMMARY  
FOR MULTICOMPONENT ANALYTES**

SAMPLE NO.

OU4-VSL-16-040325MSI

Contract: NOBI03

Lab Code: CHEM Case No.: Q1730 SAS No.: Q1730 SDG No.: Q1730

Lab Sample ID: Q1730-03MSD Date(s) Analyzed: 04/07/2025 04/07/2025

Instrument ID (1): ECD\_O Instrument ID (2): ECD\_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO110272.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.782	4.732	4.832	163	164	3.73
	2	4.801	4.751	4.851	167		
	3	4.857	4.807	4.907	167		
	4	4.978	4.928	5.028	166		
	5	5.235	5.185	5.285	159		
COLUMN 1	1	4.768	4.718	4.818	159	158	4.68
	2	4.788	4.738	4.838	160		
	3	4.963	4.913	5.013	160		
	4	5.005	4.955	5.055	157		
	5	5.217	5.167	5.267	154		
Aroclor-1260	1	6.276	6.226	6.326	169	153	4.68
	2	6.466	6.416	6.516	163		
	3	6.833	6.783	6.883	143		
	4	7.093	7.043	7.143	150		
	5	7.335	7.285	7.385	138		
COLUMN 2	1	6.25	6.2	6.3	159	146	4.68
	2	6.438	6.388	6.488	156		
	3	6.59	6.54	6.64	150		
	4	7.061	7.011	7.111	138		
	5	7.302	7.252	7.352	129		

IDENTIFICATION SUMMARY  
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB167469BS

Contract: NOBI03

Lab Code:	CHEM	Case No.:	Q1730	SAS No.:	Q1730	SDG No.:	Q1730
Lab Sample ID:	PB167469BS			Date(s) Analyzed:	04/07/2025	04/07/2025	
Instrument ID (1):	ECD_O			Instrument ID (2):	ECD_O		
GC Column: (1):	ZB-MR1	ID:	0.32 (mm)	GC Column: (2):	ZB-MR2	ID:	0.32 (mm)
Data file	PO110284.D						

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD	
			FROM	TO				
Aroclor-1016	1	4.782	4.732	4.832	141	141	5.09	
	2	4.802	4.752	4.852	143			
	3	4.858	4.808	4.908	142			
	4	4.978	4.928	5.028	142			
	5	5.236	5.186	5.286	138			
	1	4.769	4.719	4.819	136	134		
	2	4.788	4.738	4.838	134			
	3	4.964	4.914	5.014	136			
	4	5.005	4.955	5.055	135			
	5	5.218	5.168	5.268	131			
Aroclor-1260	1	6.277	6.227	6.327	149	134	4.58	
	2	6.465	6.415	6.515	141			
	3	6.833	6.783	6.883	119			
	4	7.093	7.043	7.143	131			
	5	7.336	7.286	7.386	129			
	1	6.25	6.2	6.3	140	128		
	2	6.438	6.388	6.488	138			
	3	6.59	6.54	6.64	133			
	4	7.062	7.012	7.112	119			
	5	7.303	7.253	7.353	113			



# QC SAMPLE

# DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	
Project:	Raymark Superfund Site			Date Received:	
Client Sample ID:	PB167469BL			SDG No.:	Q1730
Lab Sample ID:	PB167469BL			Matrix:	SOIL
Analytical Method:	SW8082A			% Solid:	100 Decanted:
Sample Wt/Vol:	30.01	Units:	g	Final Vol:	10000 uL
Soil Aliquot Vol:			uL	Test:	PCB
Extraction Type:				Injection Volume :	
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110283.D	1	04/07/25 08:20	04/07/25 19:22	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	8.30	U	3.90	8.30	17.0	ug/kg
11104-28-2	Aroclor-1221	13.0	U	4.00	13.0	17.0	ug/kg
11141-16-5	Aroclor-1232	8.30	U	3.70	8.30	17.0	ug/kg
53469-21-9	Aroclor-1242	8.30	U	4.00	8.30	17.0	ug/kg
12672-29-6	Aroclor-1248	13.0	U	5.90	13.0	17.0	ug/kg
11097-69-1	Aroclor-1254	8.30	U	3.20	8.30	17.0	ug/kg
37324-23-5	Aroclor-1262	13.0	U	5.00	13.0	17.0	ug/kg
11100-14-4	Aroclor-1268	8.30	U	3.60	8.30	17.0	ug/kg
11096-82-5	Aroclor-1260	8.30	U	3.20	8.30	17.0	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	19.0		44 - 130		95%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.3		60 - 125		86%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110283.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 19:22  
 Operator : YP/AJ  
 Sample : PB167469BL  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**PB167469BL**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:35:40 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	3.691	3.688	173.1E6	95749355	19.020	18.259
2) SA Decachloro...	8.741	8.691	133.0E6	38862706	17.297	16.019

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110283.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 19:22  
 Operator : YP/AJ  
 Sample : PB167469BL  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 PB167469BL

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:35:40 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

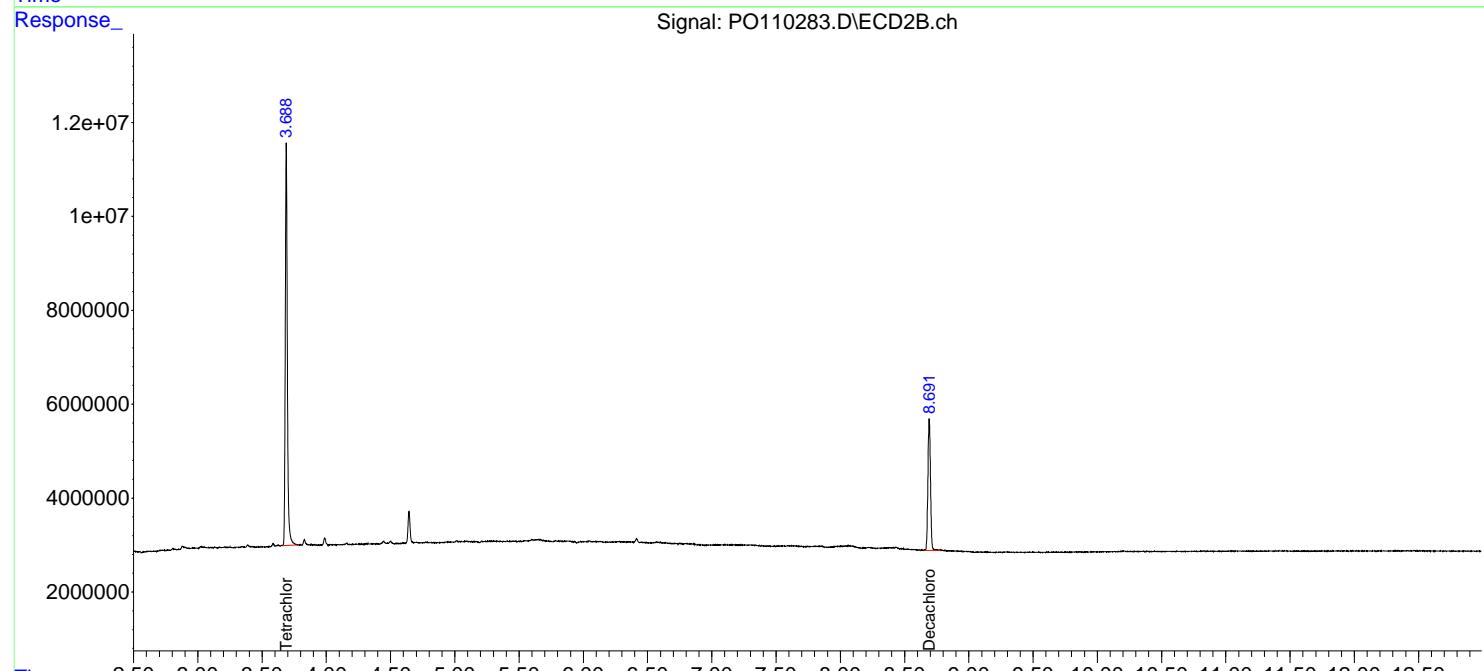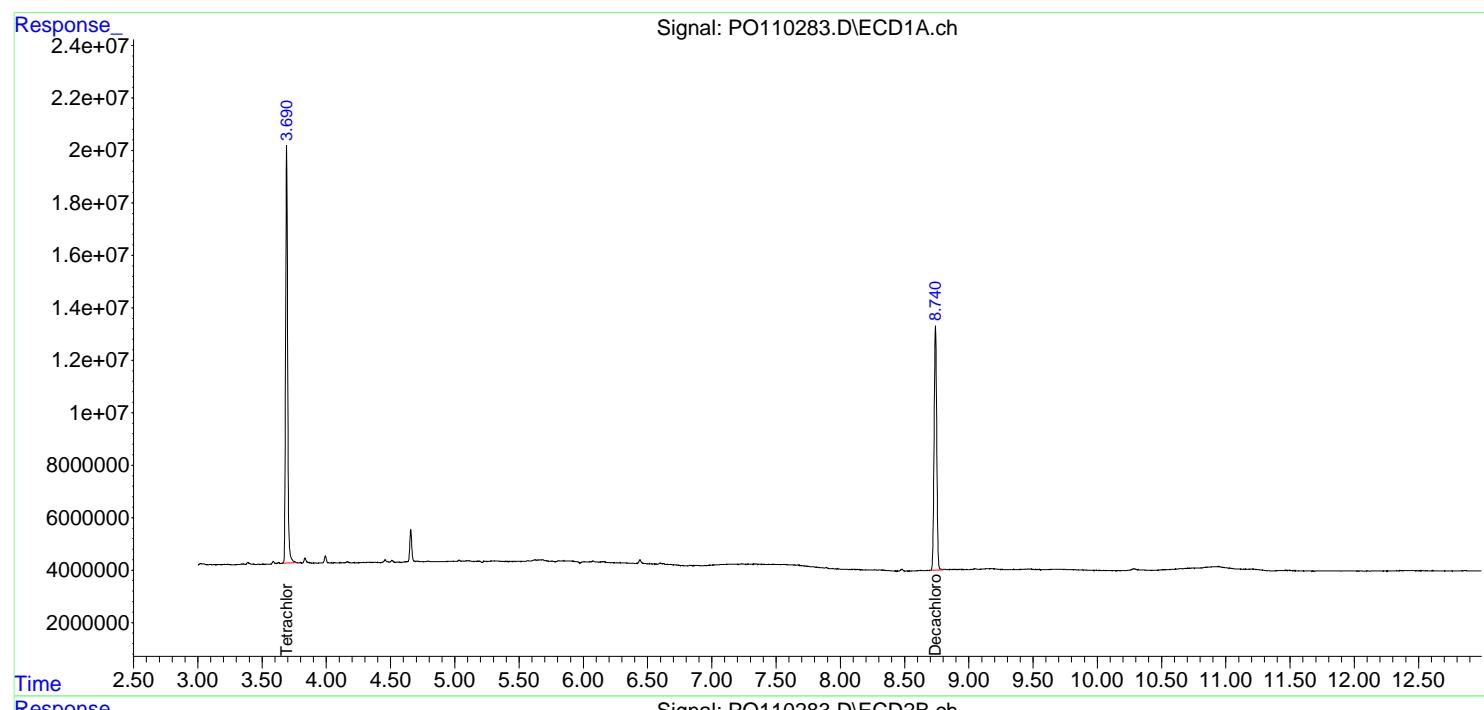


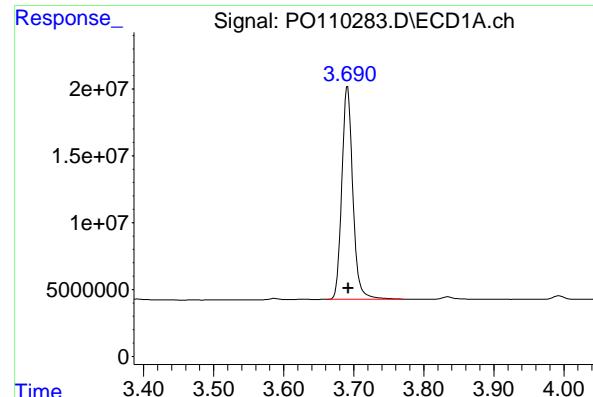

## #1 Tetrachloro-m-xylene


R.T.: 3.691 min  
 Delta R.T.: 0.000 min  
 Response: 173109300  
 Conc: 19.02 ng/ml

Instrument: ECD\_O  
 ClientSampleId: PB167469BL

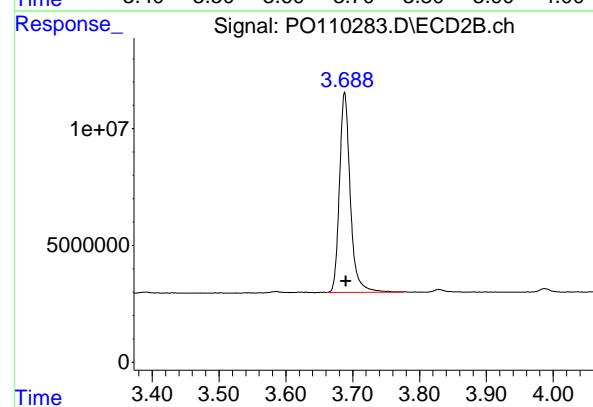


## #1 Tetrachloro-m-xylene

R.T.: 3.688 min  
 Delta R.T.: -0.002 min  
 Response: 95749355  
 Conc: 18.26 ng/ml

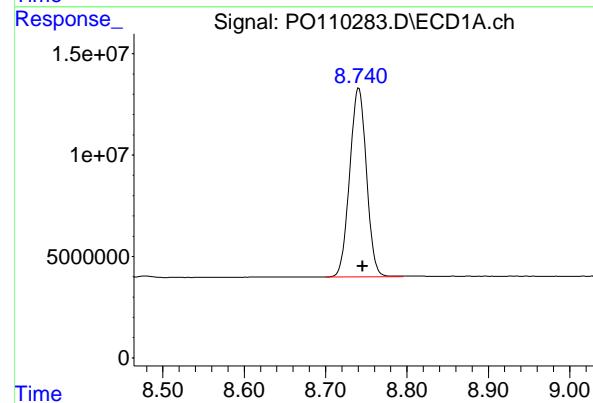

## #2 Decachlorobiphenyl

R.T.: 8.741 min  
 Delta R.T.: -0.005 min  
 Response: 132989663  
 Conc: 17.30 ng/ml

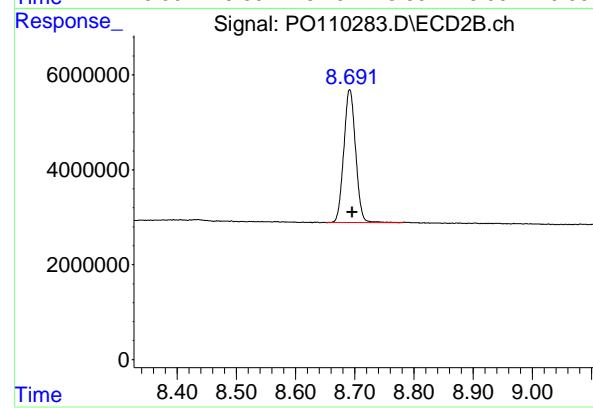

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
 Delta R.T.: -0.004 min  
 Response: 38862706  
 Conc: 16.02 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	03/18/25			
Project:	Raymark Superfund Site			Date Received:	03/18/25			
Client Sample ID:	PIBLK-PO109971.D			SDG No.:	Q1730			
Lab Sample ID:	I.BLK-PO109971.D			Matrix:	WATER			
Analytical Method:	SW8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109971.D	1		03/18/25	PO031925

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	18.5		60 - 140		93%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.0		60 - 140		100%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
Data File : P0109971.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Mar 2025 13:44  
Operator : YP/AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 19 03:44:56 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Mar 19 02:52:01 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

---

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	168.3E6	97603621	18.495	18.612
2) SA Decachlor...	8.744	8.695	153.9E6	51783076	20.014	21.344

Target Compounds

---



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109971.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 13:44  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 03:44:56 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$

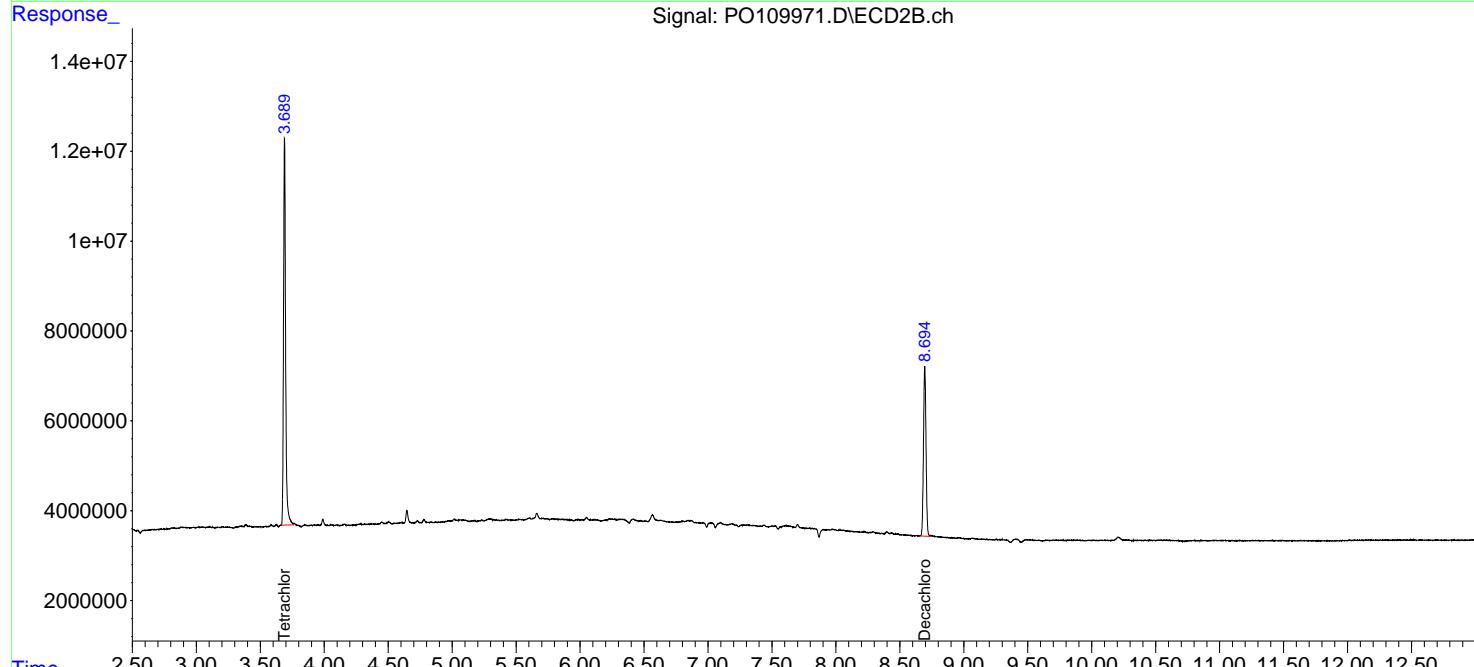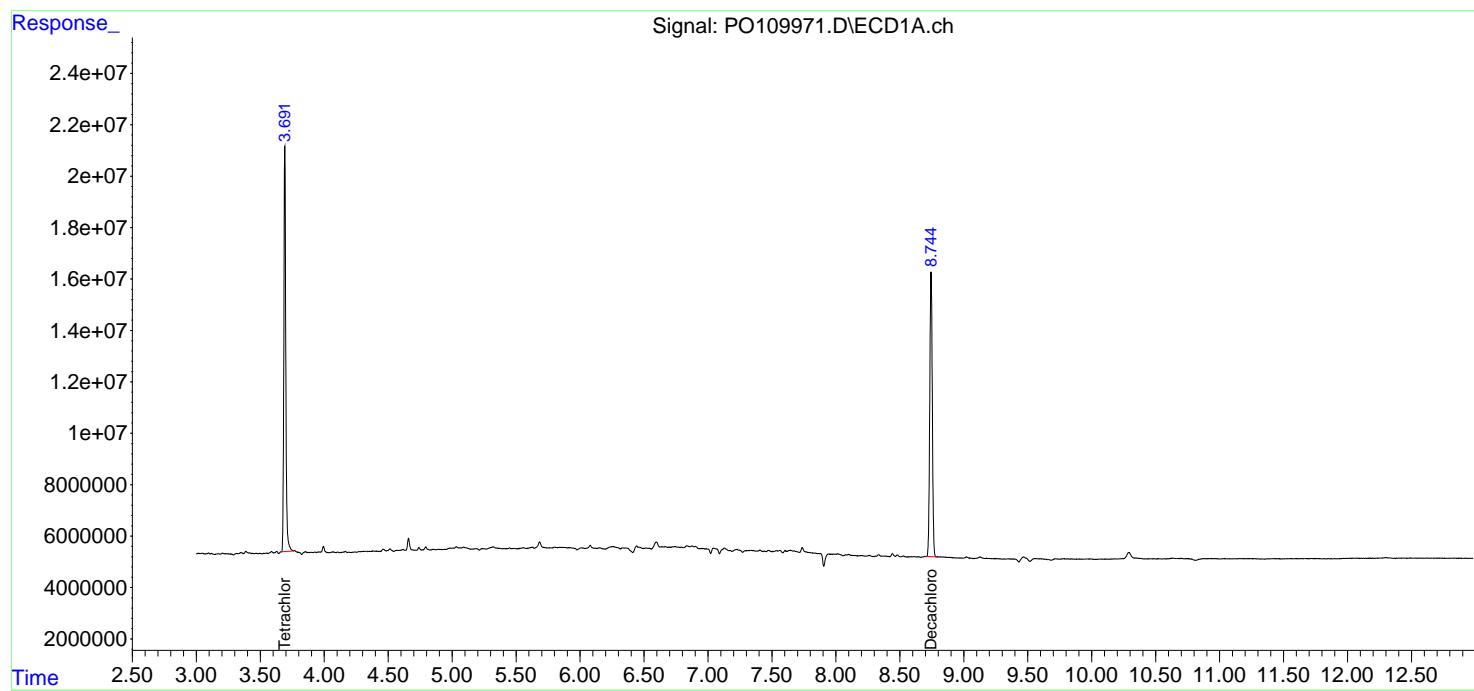




#1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 168336707  
Conc: 18.50 ng/ml


Instrument:

ECD\_O

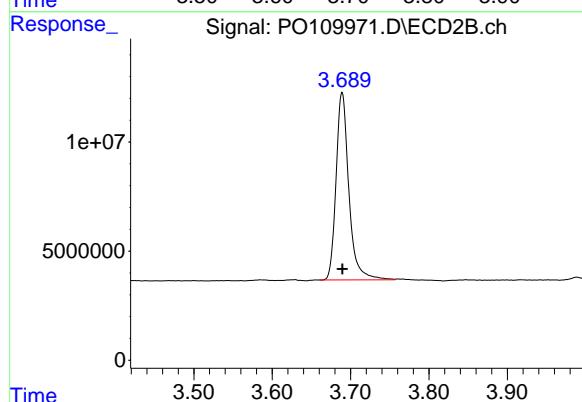ClientSampleId:  
I.BLK


#1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 97603621  
Conc: 18.61 ng/ml

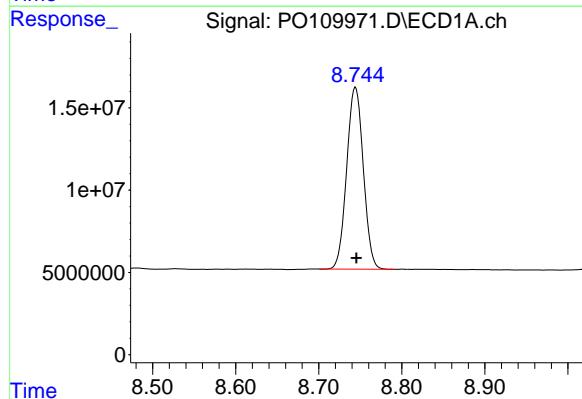

#2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: -0.001 min  
Response: 153882781  
Conc: 20.01 ng/ml

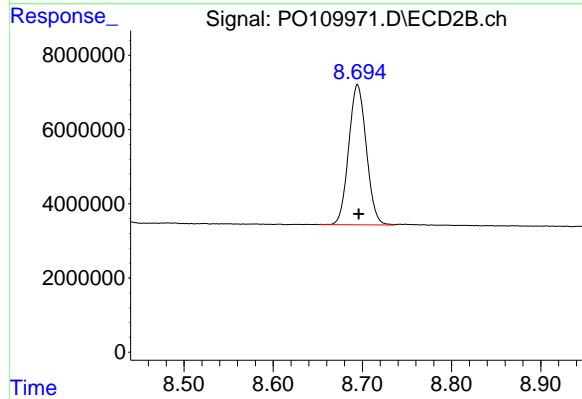

#2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: -0.001 min  
Response: 51783076  
Conc: 21.34 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/07/25	
Project:	Raymark Superfund Site			Date Received:	04/07/25	
Client Sample ID:	PIBLK-PO110267.D			SDG No.:	Q1730	
Lab Sample ID:	I.BLK-PO110267.D			Matrix:	WATER	
Analytical Method:	SW8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110267.D	1		04/07/25	PO040725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	18.8		60 - 140		94%	SPK: 20
2051-24-3	Decachlorobiphenyl	15.9		60 - 140		79%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110267.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 11:36  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 12:31:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	3.689	3.687	177.4E6	98699299	19.494	18.821
2) SA Decachloro...	8.737	8.690	141.7E6	38504154	18.426	15.871

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110267.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 11:36  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 12:31:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

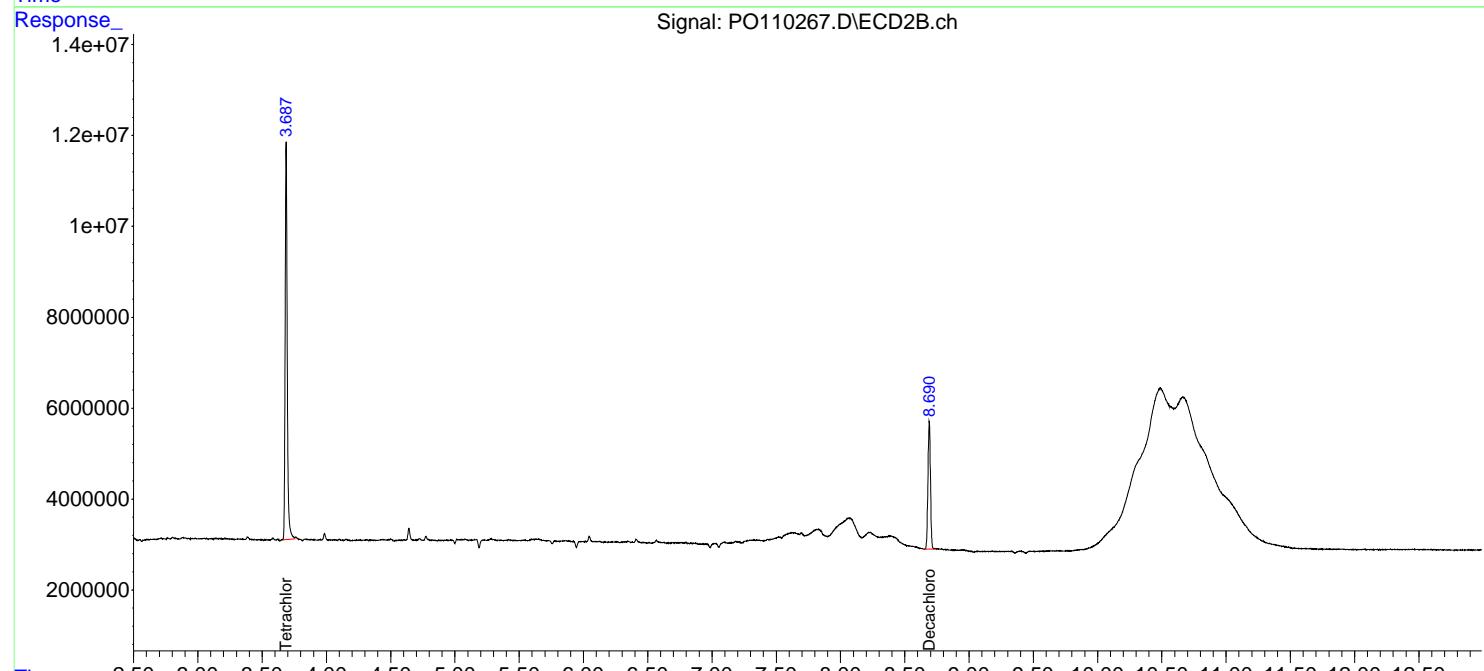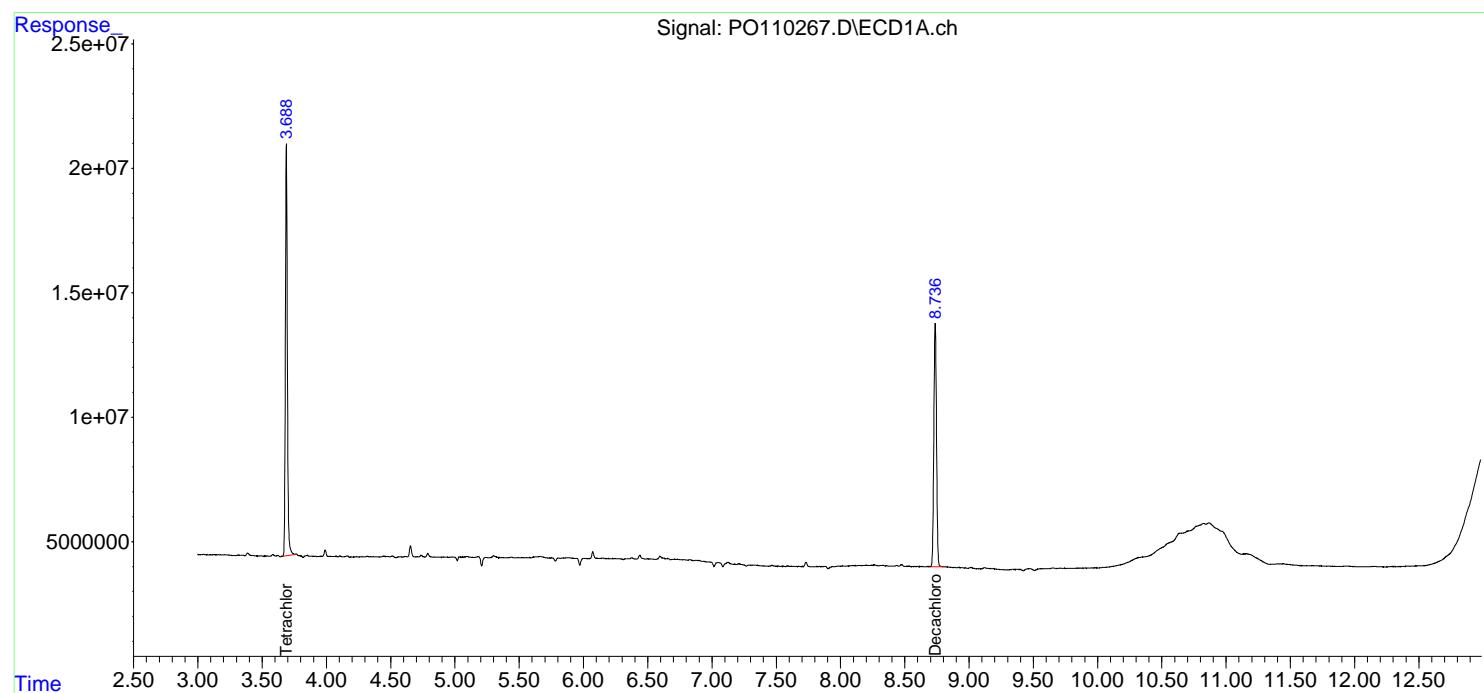

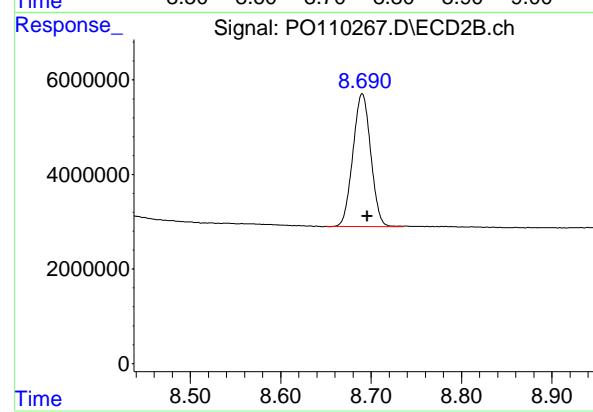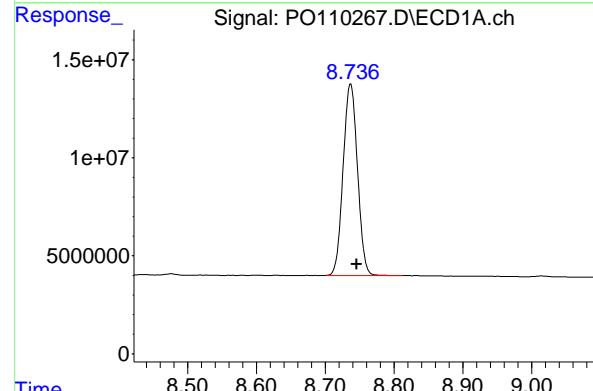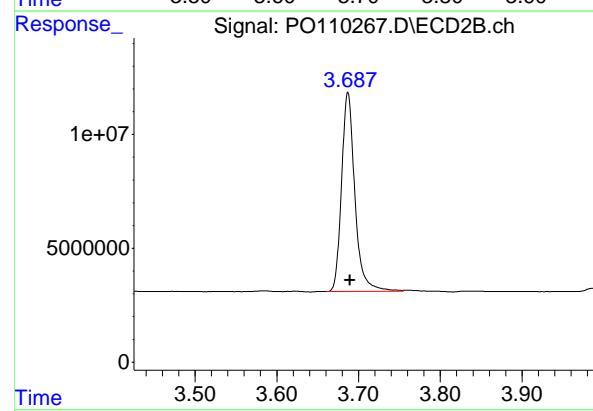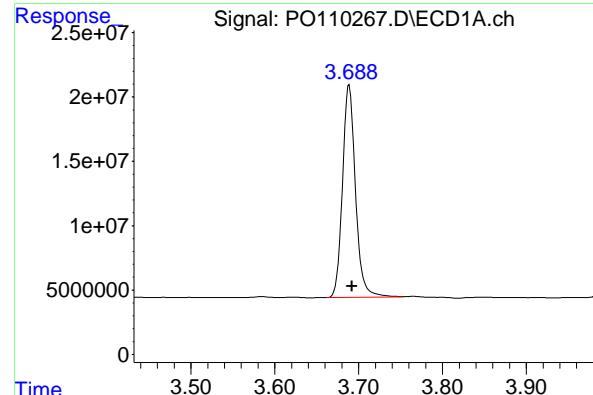

## #1 Tetrachloro-m-xylene

R.T.: 3.689 min  
 Delta R.T.: -0.003 min  
 Response: 177426113 ECD\_O  
 Conc: 19.49 ng/ml ClientSampleId : I.BLK

## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
 Delta R.T.: -0.003 min  
 Response: 98699299 ECD\_O  
 Conc: 18.82 ng/ml ClientSampleId : I.BLK

## #2 Decachlorobiphenyl

R.T.: 8.737 min  
 Delta R.T.: -0.008 min  
 Response: 141670453 ECD\_O  
 Conc: 18.43 ng/ml ClientSampleId : I.BLK

## #2 Decachlorobiphenyl

R.T.: 8.690 min  
 Delta R.T.: -0.006 min  
 Response: 38504154 ECD\_O  
 Conc: 15.87 ng/ml ClientSampleId : I.BLK



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/07/25	
Project:	Raymark Superfund Site			Date Received:	04/07/25	
Client Sample ID:	PIBLK-PO110282.D			SDG No.:	Q1730	
Lab Sample ID:	I.BLK-PO110282.D			Matrix:	WATER	
Analytical Method:	SW8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110282.D	1		04/07/25	PO040725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	18.8		60 - 140		94%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.2		60 - 140		81%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110282.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 19:04  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:35:20 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	3.691	3.688	176.0E6	98785740	19.334	18.838
2) SA Decachloro...	8.740	8.692	132.1E6	39381036	17.185	16.232

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110282.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 19:04  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:35:20 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

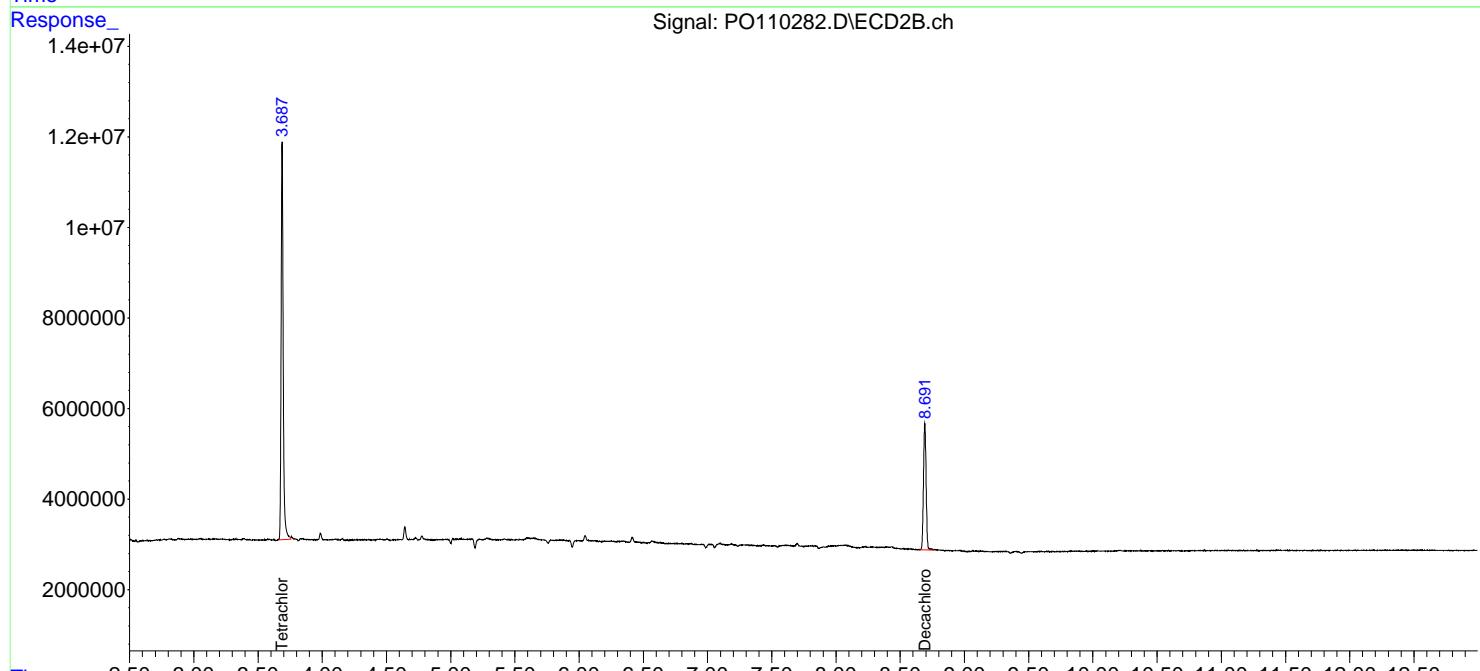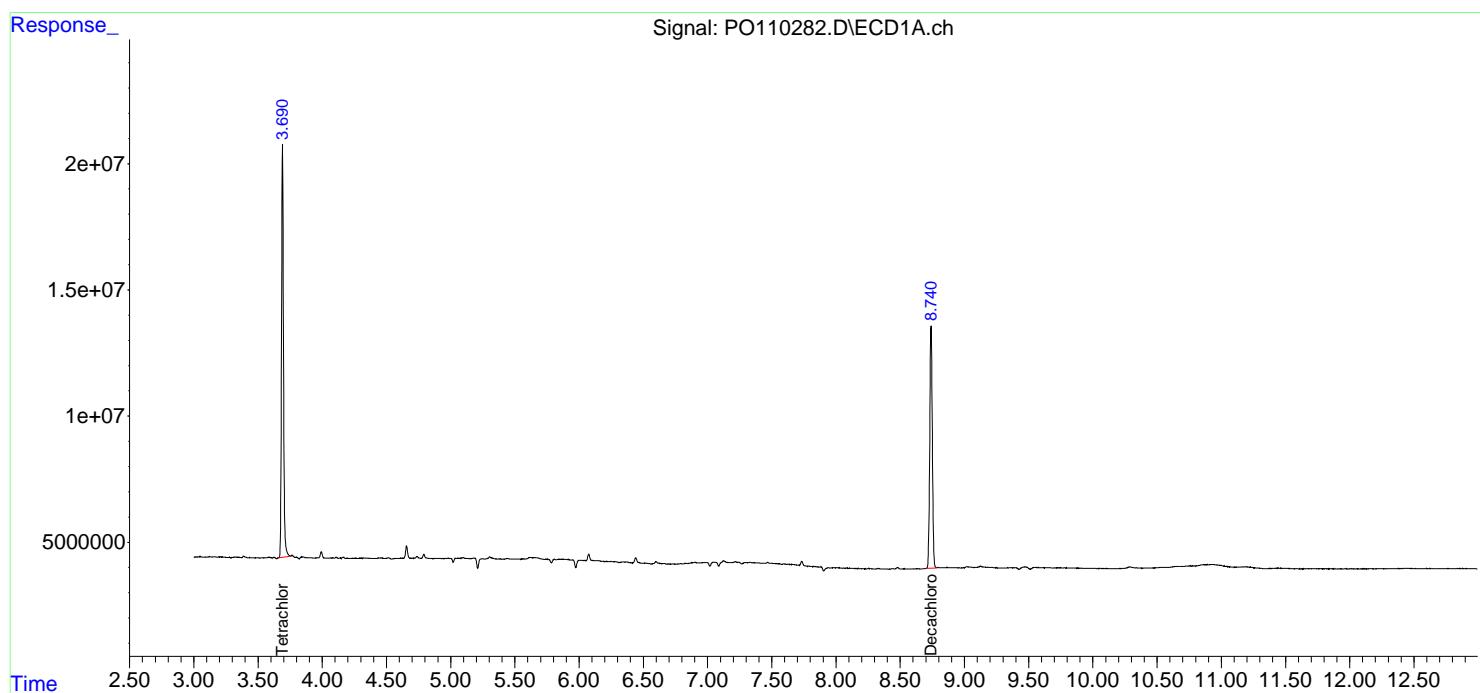

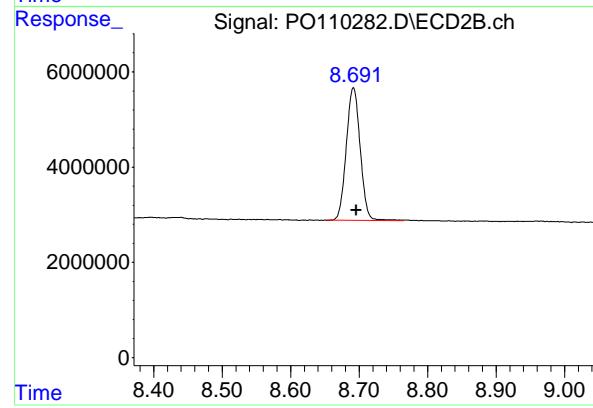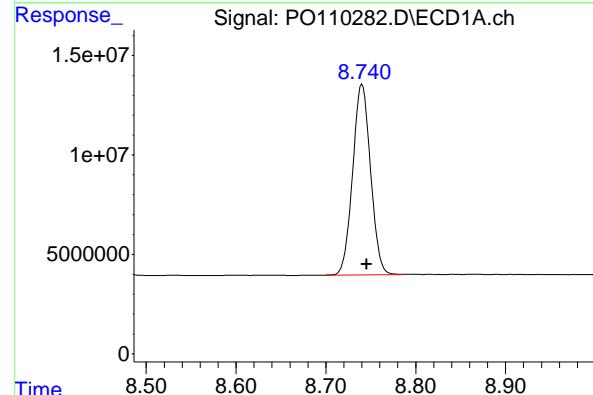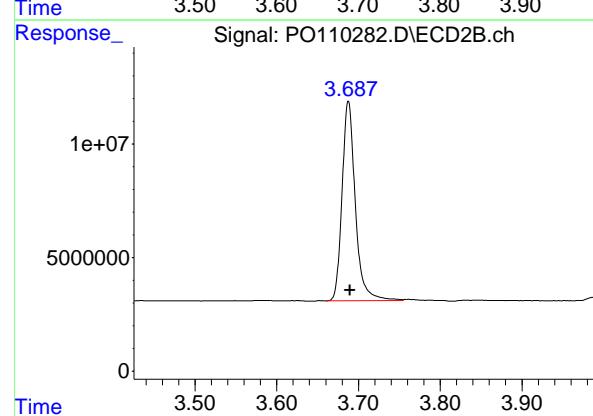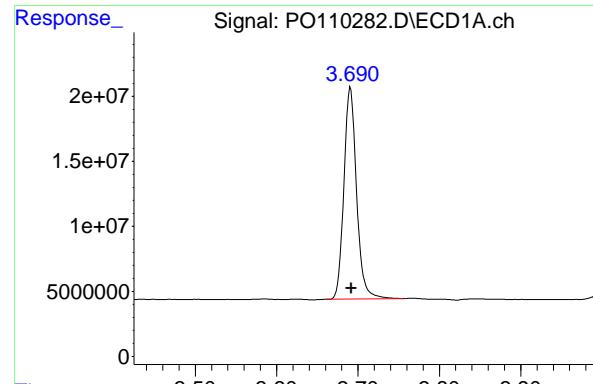

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: -0.001 min  
 Response: 175966498 ECD\_O  
 Conc: 19.33 ng/ml ClientSampleId : I.BLK

## #1 Tetrachloro-m-xylene

R.T.: 3.688 min  
 Delta R.T.: -0.002 min  
 Response: 98785740  
 Conc: 18.84 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.740 min  
 Delta R.T.: -0.005 min  
 Response: 132132646  
 Conc: 17.19 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.692 min  
 Delta R.T.: -0.004 min  
 Response: 39381036  
 Conc: 16.23 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/07/25	
Project:	Raymark Superfund Site			Date Received:	04/07/25	
Client Sample ID:	PIBLK-PO110290.D			SDG No.:	Q1730	
Lab Sample ID:	I.BLK-PO110290.D			Matrix:	WATER	
Analytical Method:	SW8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110290.D	1		04/07/25	PO040725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	18.9		60 - 140		94%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.2		60 - 140		81%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110290.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 23:17  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:38:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	3.691	3.687	177.5E6	98959783	19.499	18.871
2) SA Decachloro...	8.742	8.692	136.3E6	39361941	17.725	16.224

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110290.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 23:17  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:38:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

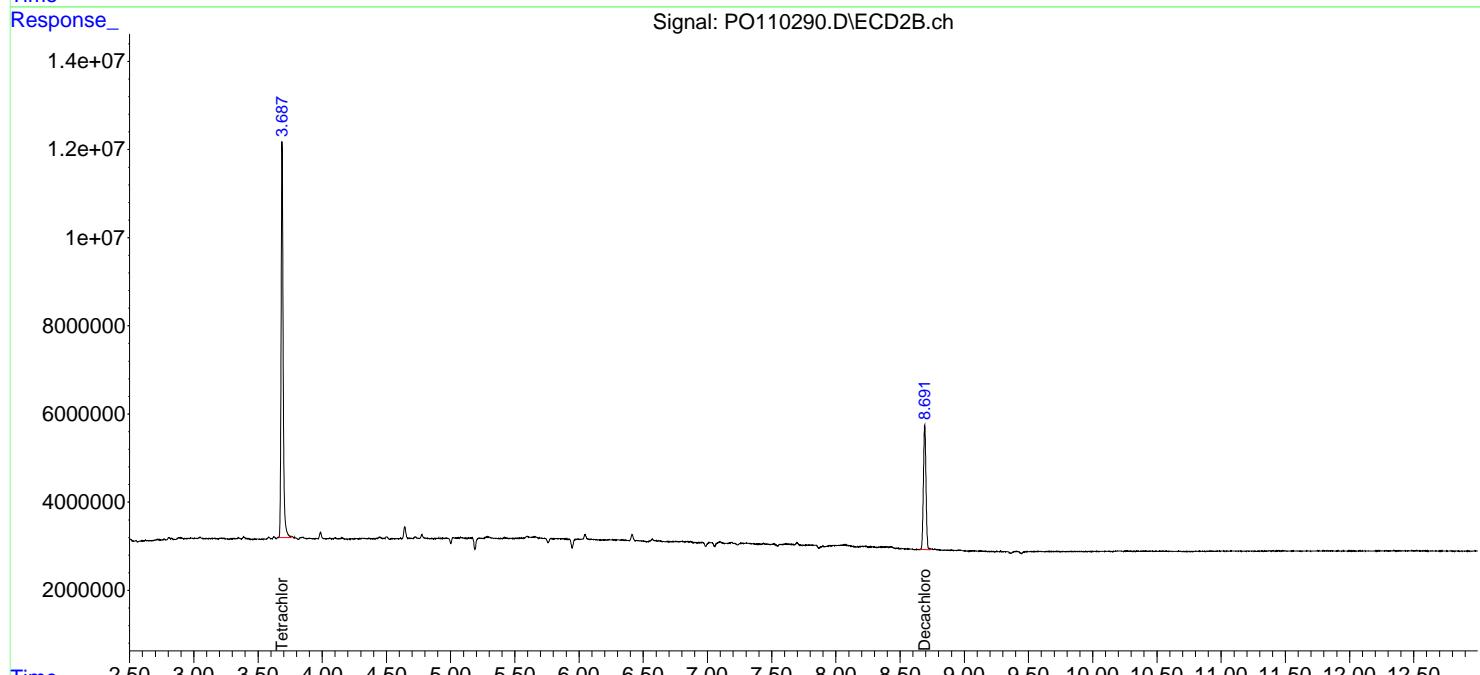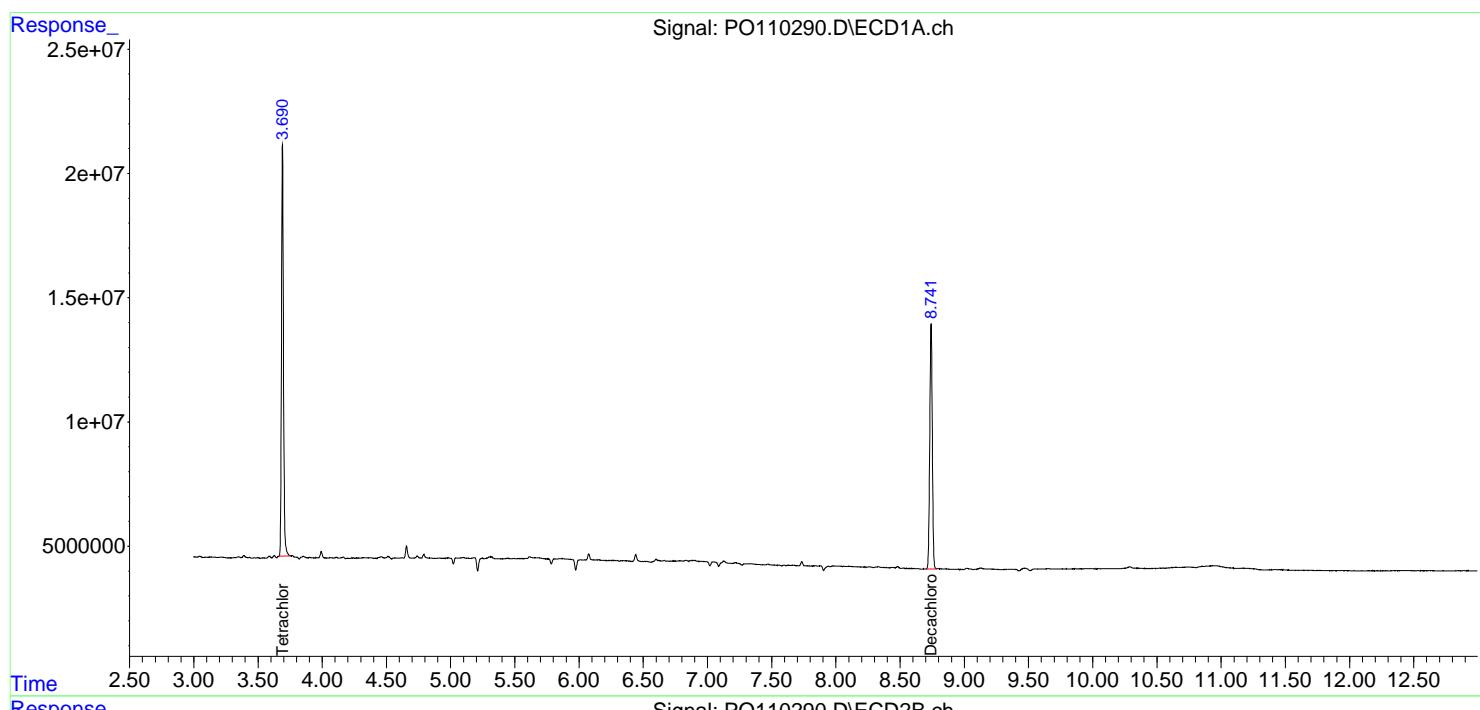

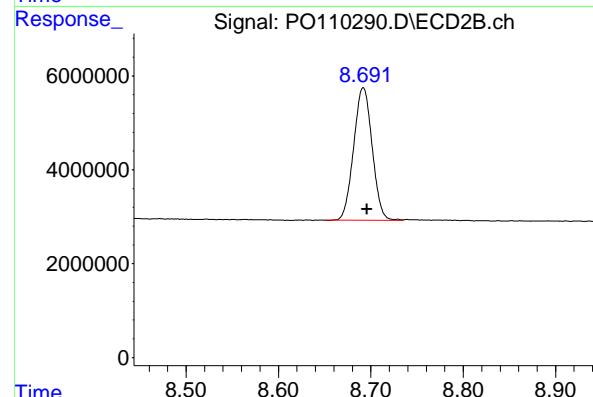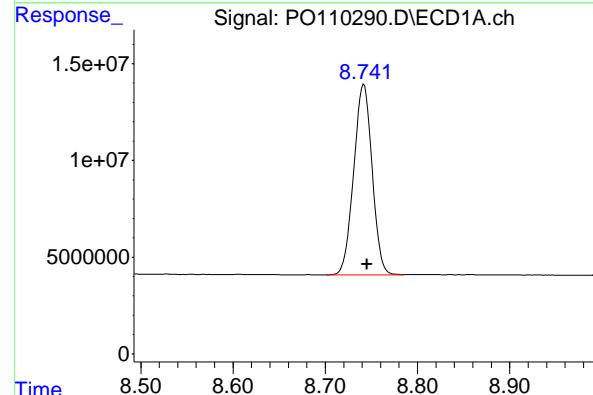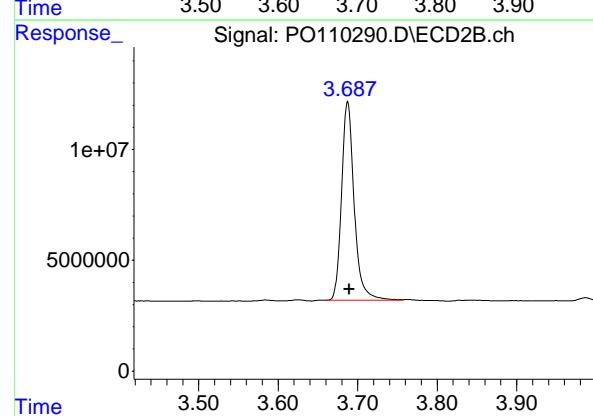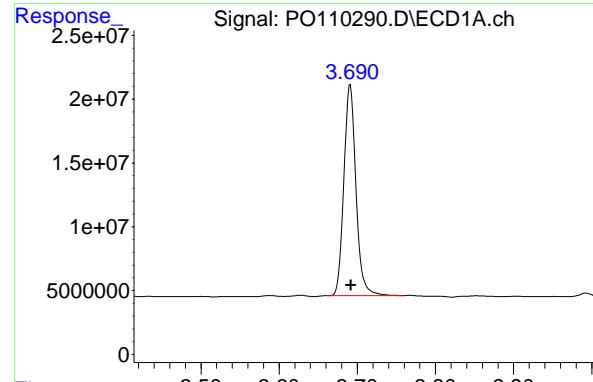

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: -0.001 min  
 Response: 177471328 ECD\_O  
 Conc: 19.50 ng/ml ClientSampleId : I.BLK

## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
 Delta R.T.: -0.002 min  
 Response: 98959783 ECD\_O  
 Conc: 18.87 ng/ml ClientSampleId : I.BLK

## #2 Decachlorobiphenyl

R.T.: 8.742 min  
 Delta R.T.: -0.004 min  
 Response: 136281296 ECD\_O  
 Conc: 17.72 ng/ml ClientSampleId : I.BLK

## #2 Decachlorobiphenyl

R.T.: 8.692 min  
 Delta R.T.: -0.004 min  
 Response: 39361941 ECD\_O  
 Conc: 16.22 ng/ml ClientSampleId : I.BLK



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/08/25	
Project:	Raymark Superfund Site			Date Received:	04/08/25	
Client Sample ID:	PIBLK-PO110296.D			SDG No.:	Q1730	
Lab Sample ID:	I.BLK-PO110296.D			Matrix:	WATER	
Analytical Method:	SW8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110296.D	1		04/08/25	PO040825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	17.7		60 - 140		89%	SPK: 20
2051-24-3	Decachlorobiphenyl	15.4		60 - 140		77%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110296.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 10:21  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:44:40 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	3.688	3.687	169.9E6	93006368	18.670	17.735
2) SA Decachloro...	8.738	8.690	136.7E6	37456258	17.778	15.439

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110296.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 10:21  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:44:40 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

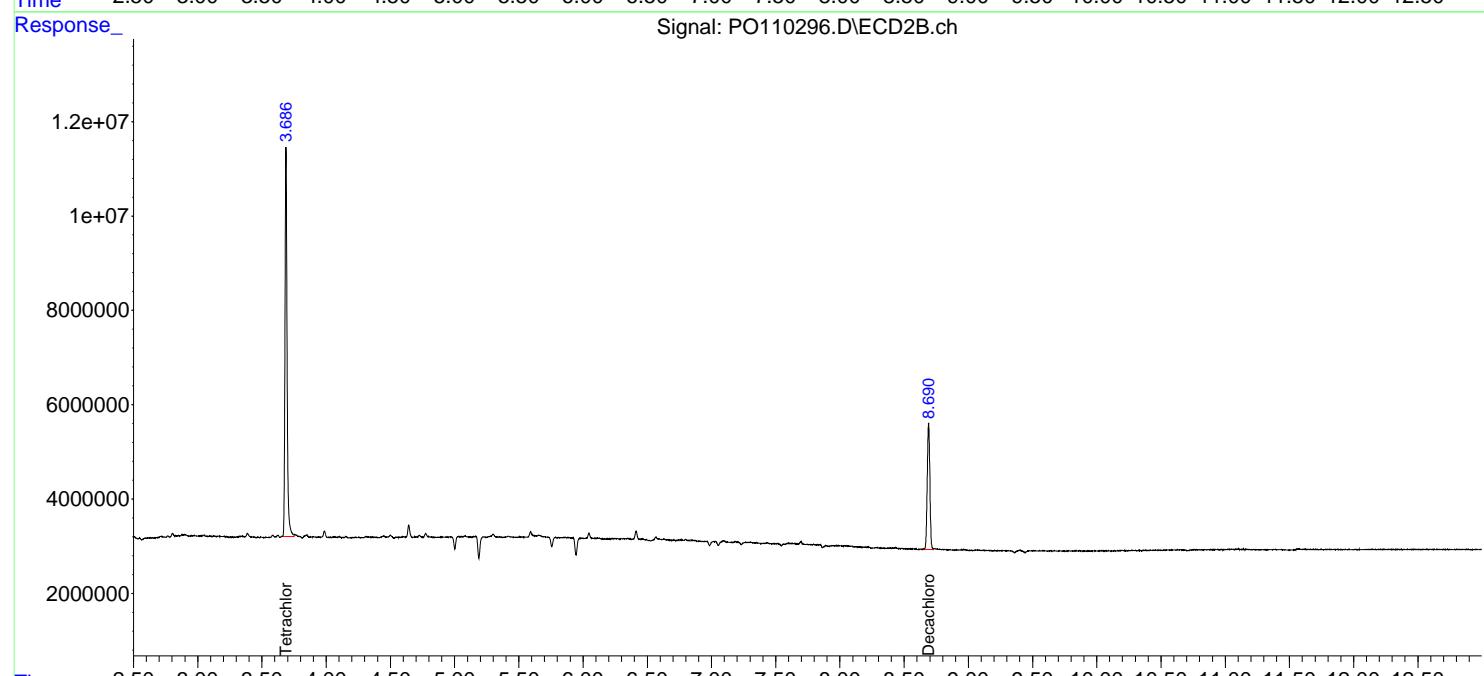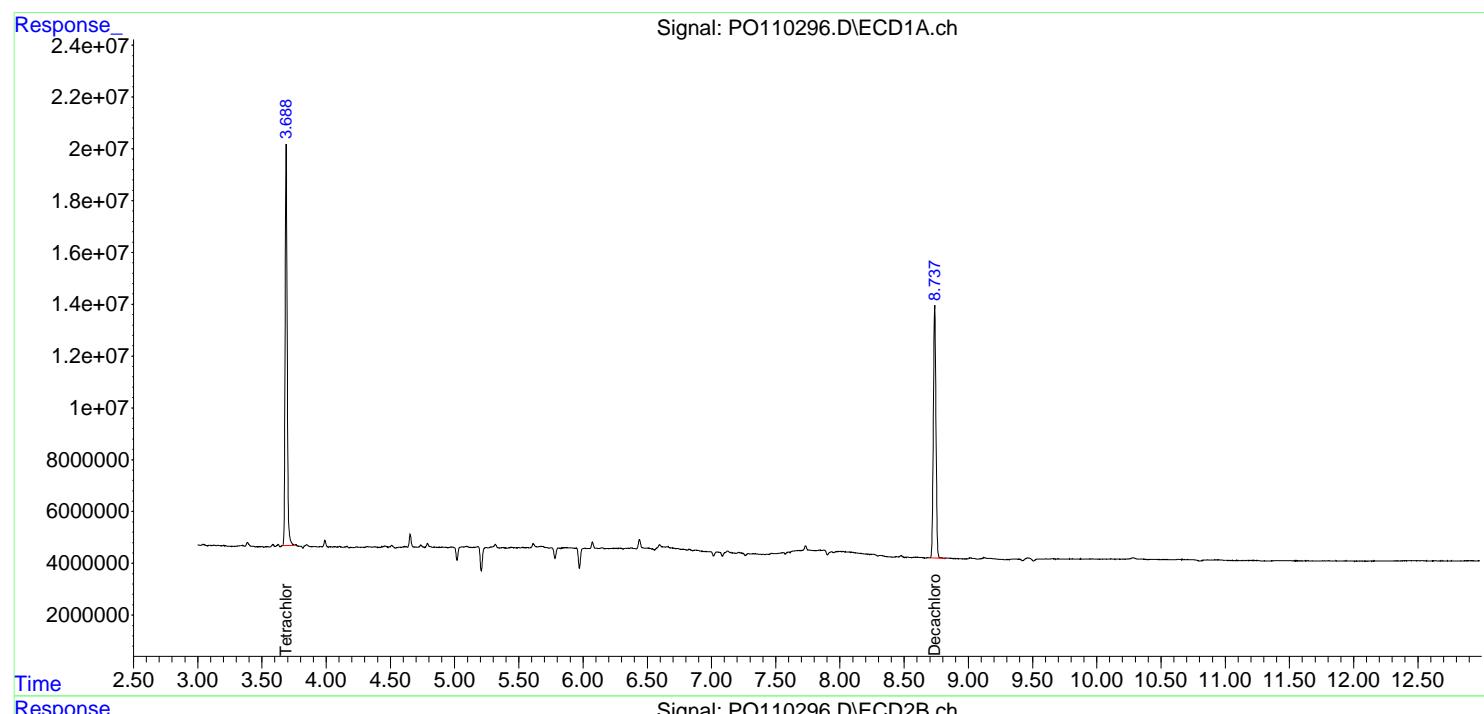

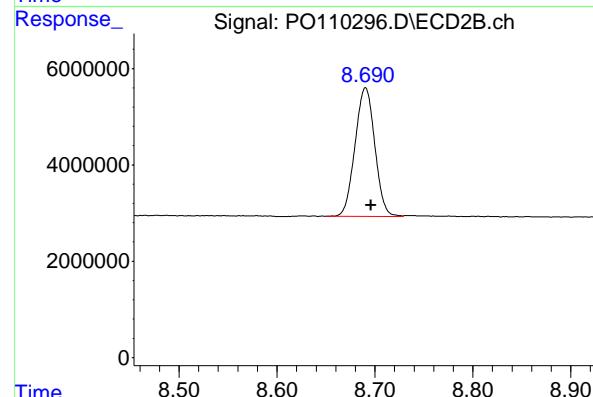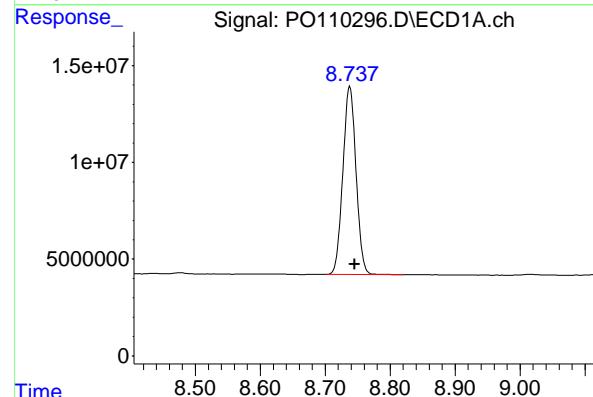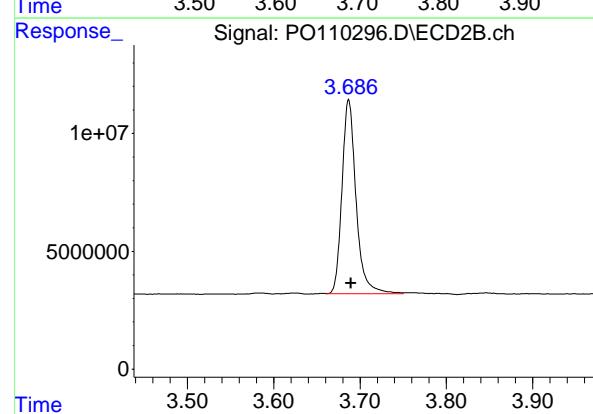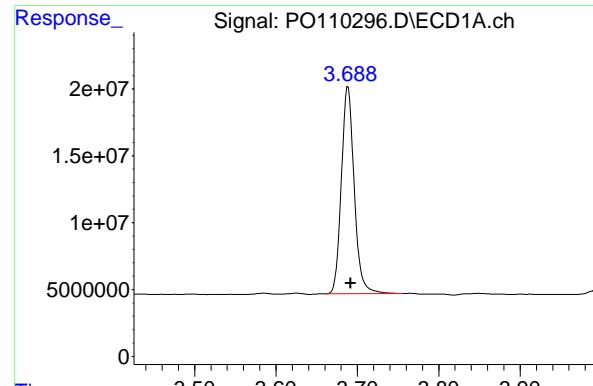

## #1 Tetrachloro-m-xylene

R.T.: 3.688 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_O  
Response: 169928217  
Conc: 18.67 ng/ml  
ClientSampleId : I.BLK

## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_O  
Response: 93006368  
Conc: 17.74 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.738 min  
Delta R.T.: -0.008 min  
Instrument: ECD\_O  
Response: 136688438  
Conc: 17.78 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.690 min  
Delta R.T.: -0.005 min  
Instrument: ECD\_O  
Response: 37456258  
Conc: 15.44 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/08/25			
Project:	Raymark Superfund Site			Date Received:	04/08/25			
Client Sample ID:	PIBLK-PO110306.D			SDG No.:	Q1730			
Lab Sample ID:	I.BLK-PO110306.D			Matrix:	WATER			
Analytical Method:	SW8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110306.D	1		04/08/25	PO040825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	17.4		60 - 140		87%	SPK: 20
2051-24-3	Decachlorobiphenyl	15.3		60 - 140		77%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110306.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 14:12  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_O  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 14:20:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachloro...	3.690	3.687	165.6E6	91042032	18.193	17.361
2) SA Decachloro...	8.739	8.691	141.3E6	37124521	18.373	15.302

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040825\  
 Data File : P0110306.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 14:12  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 14:20:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

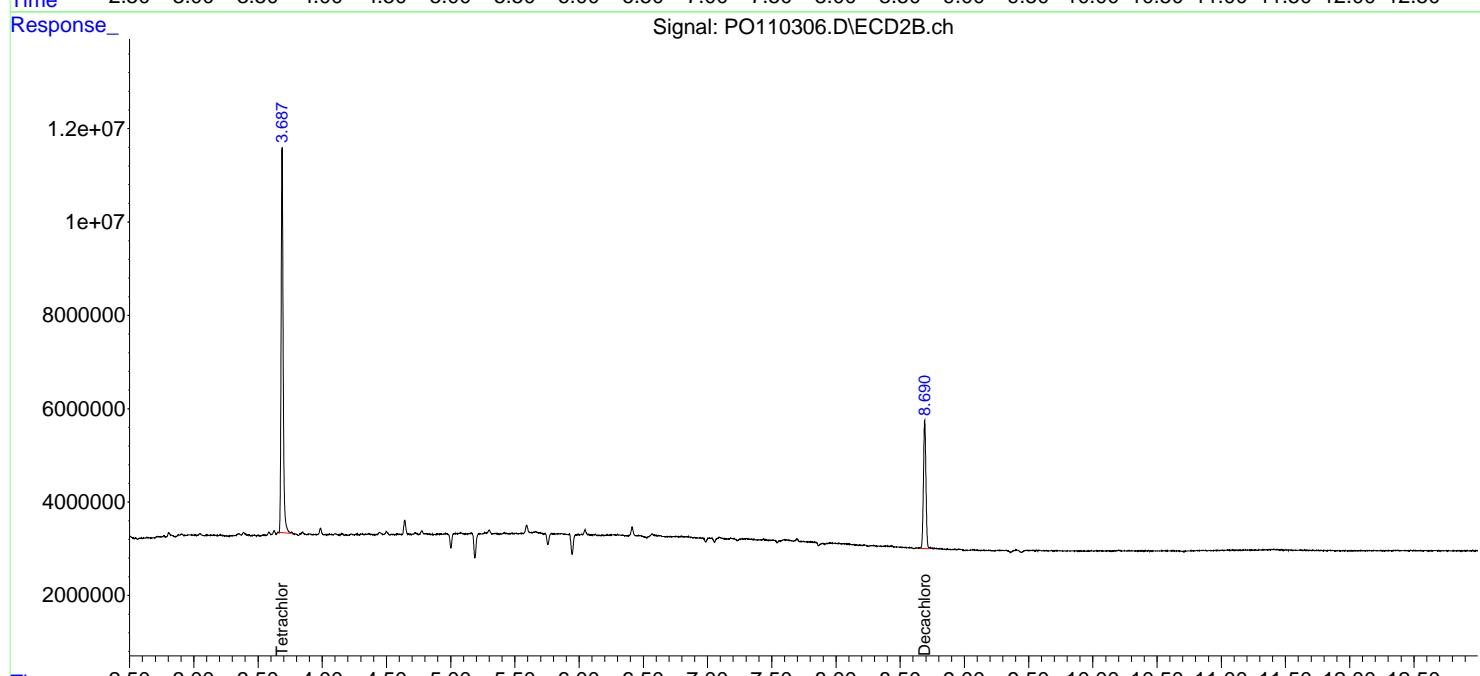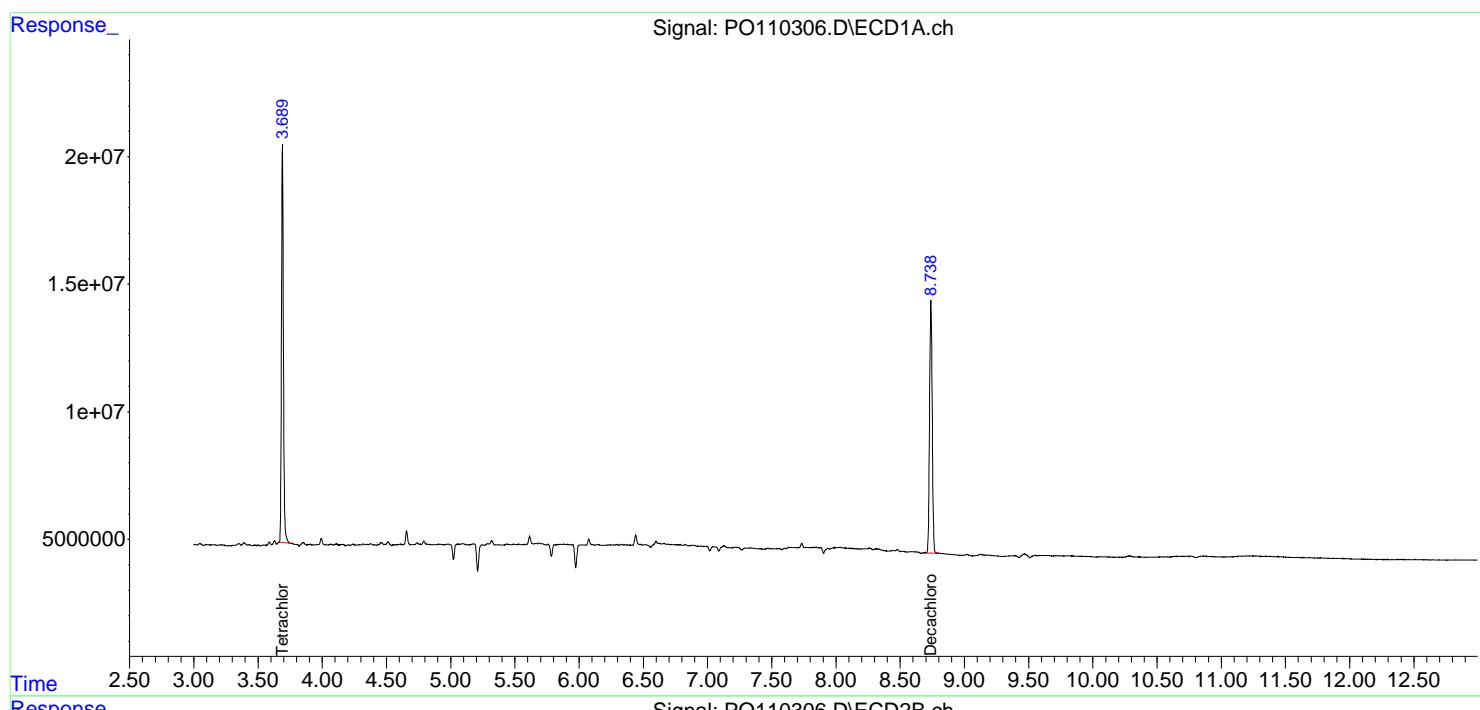

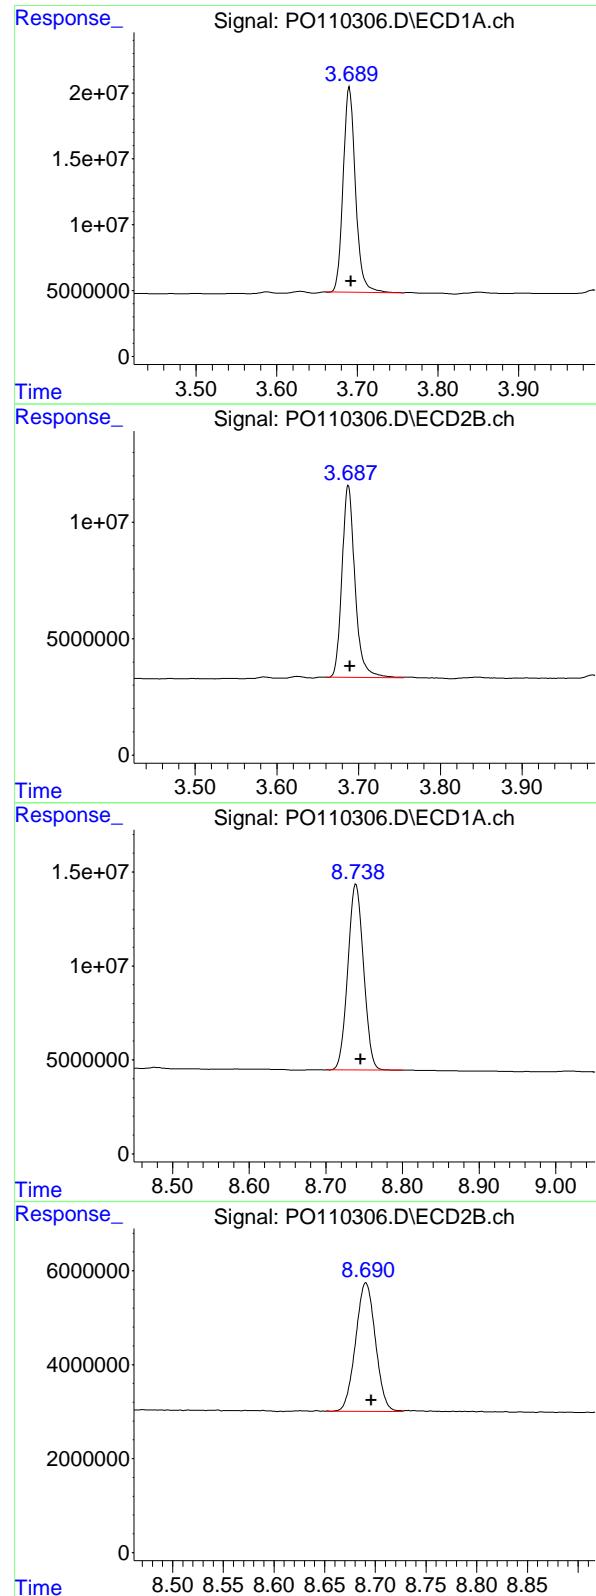

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: -0.002 min  
 Response: 165584494 ECD\_O  
 Conc: 18.19 ng/ml ClientSampleId : I.BLK

## #1 Tetrachloro-m-xylene

R.T.: 3.687 min  
 Delta R.T.: -0.002 min  
 Response: 91042032 ECD\_O  
 Conc: 17.36 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.739 min  
 Delta R.T.: -0.006 min  
 Response: 141264866 ECD\_O  
 Conc: 18.37 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
 Delta R.T.: -0.005 min  
 Response: 37124521 ECD\_O  
 Conc: 15.30 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	03/27/25	
Project:	Raymark Superfund Site			Date Received:	03/27/25	
Client Sample ID:	PIBLK-PP070916.D			SDG No.:	Q1730	
Lab Sample ID:	I.BLK-PP070916.D			Matrix:	WATER	
Analytical Method:	SW8082A			% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	5030					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070916.D	1		03/27/25	PP032725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	18.1		60 - 140		91%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.4		60 - 140		97%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070916.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 10:14  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 06:35:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	4.514	3.816	27521844	18794888	18.830	18.131
2) SA Decachloro...	10.229	8.858	20399611	18404317	19.380	23.350

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070916.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 10:14  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 06:35:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

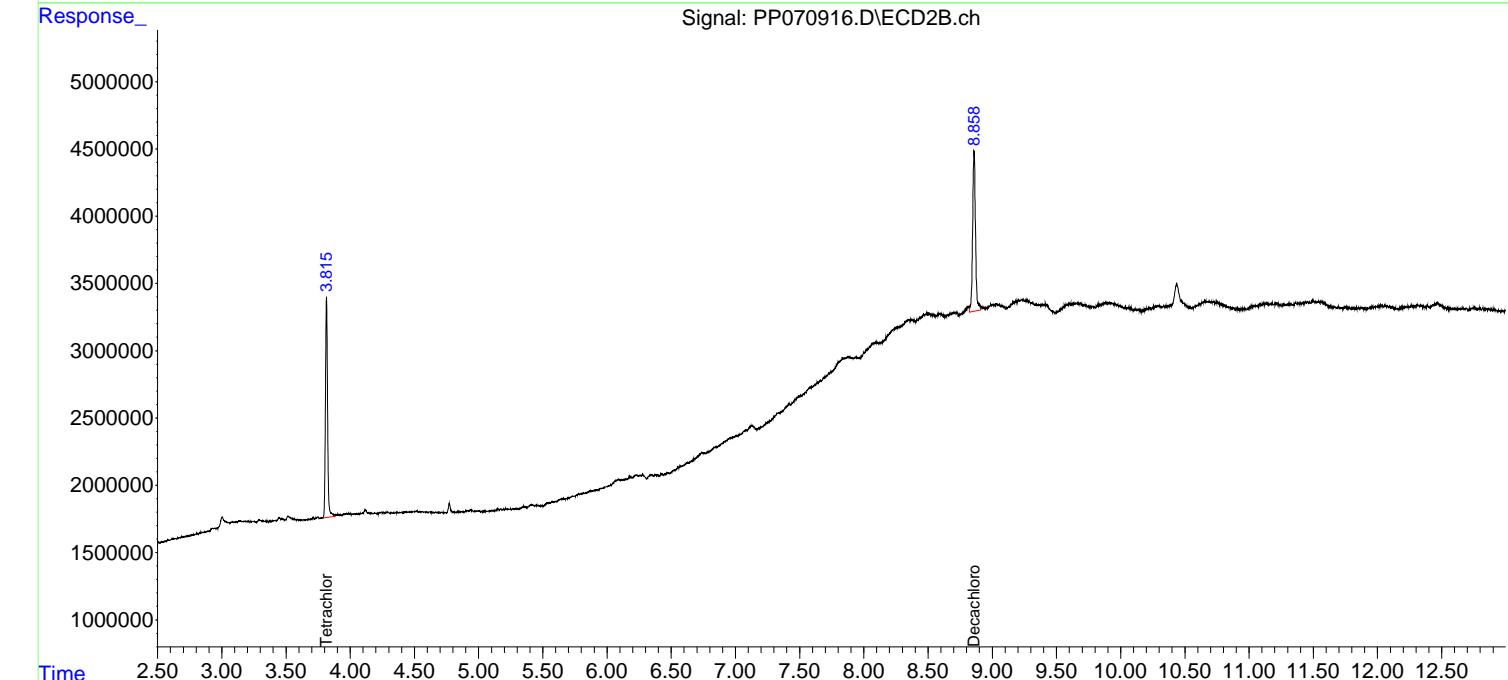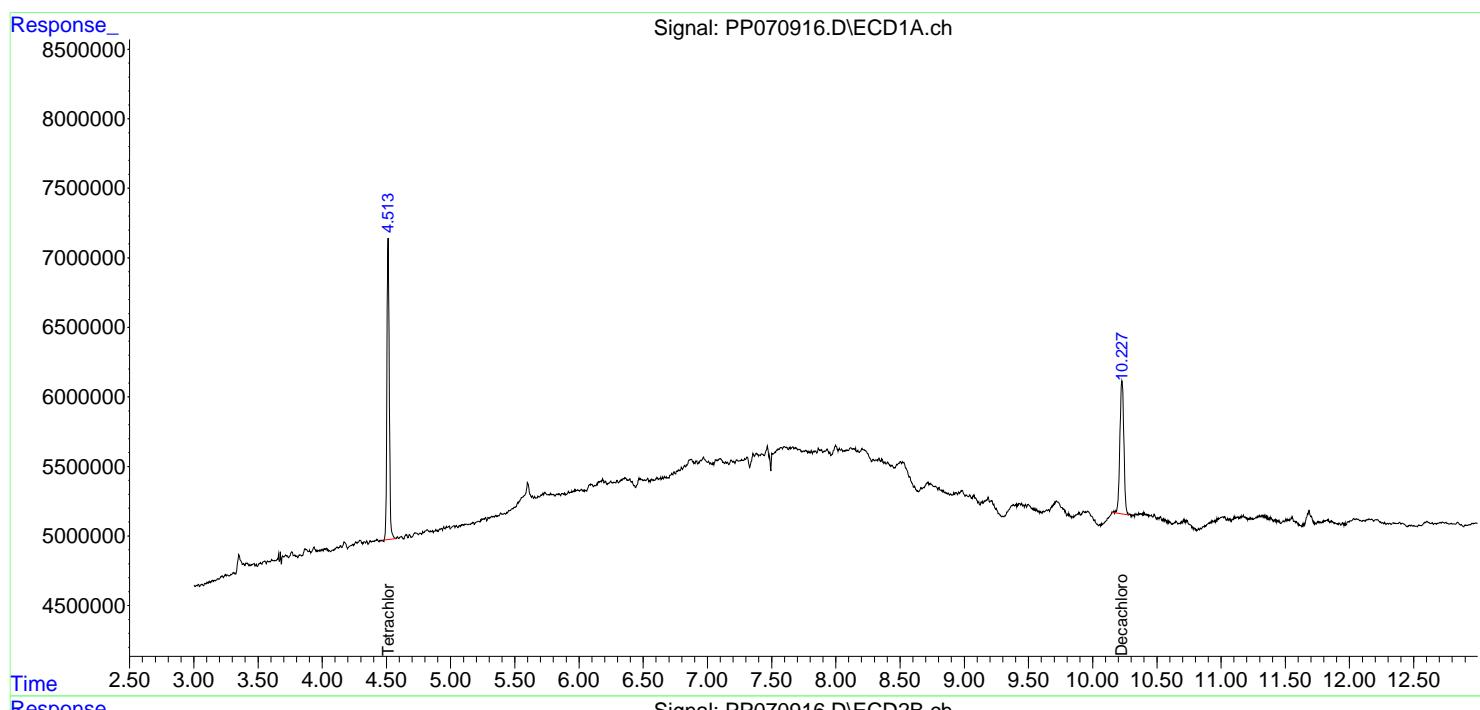

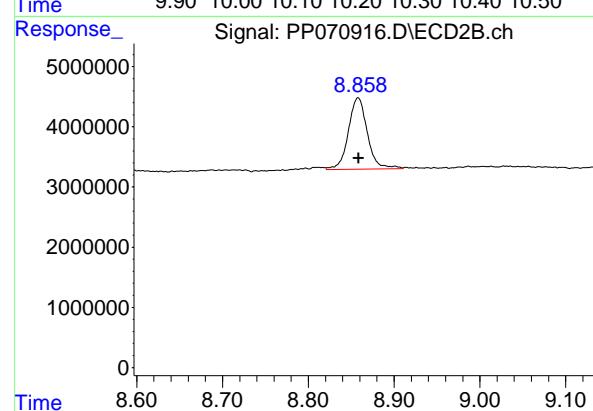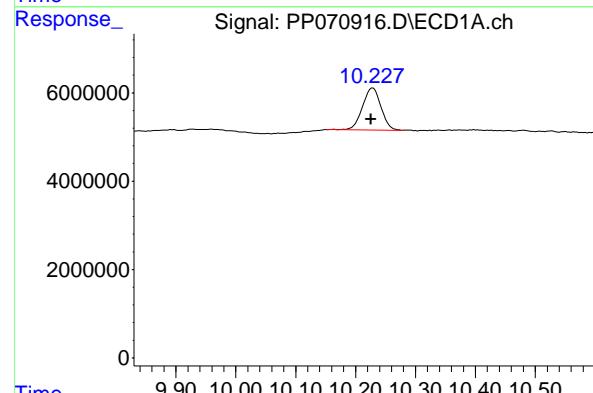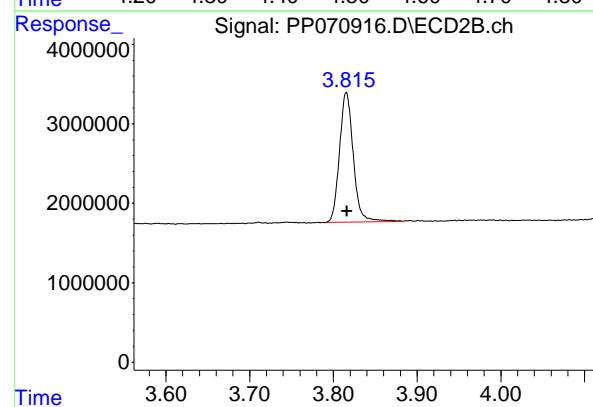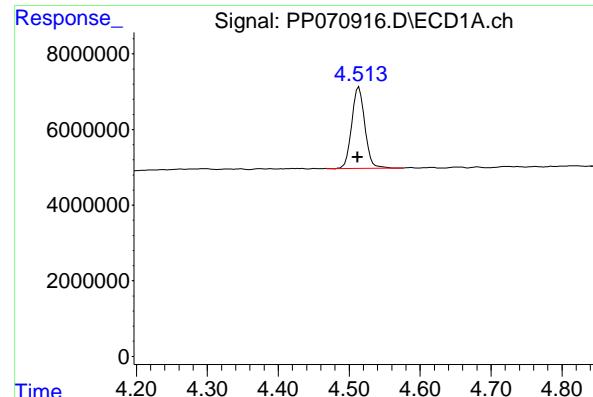

## #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
 Delta R.T.: 0.002 min  
 Response: 27521844 ECD\_P  
 Conc: 18.83 ng/ml ClientSampleId : I.BLK

## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 18794888  
 Conc: 18.13 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.229 min  
 Delta R.T.: 0.003 min  
 Response: 20399611  
 Conc: 19.38 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.858 min  
 Delta R.T.: 0.000 min  
 Response: 18404317  
 Conc: 23.35 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/08/25			
Project:	Raymark Superfund Site			Date Received:	04/08/25			
Client Sample ID:	PIBLK-PP071140.D			SDG No.:	Q1730			
Lab Sample ID:	I.BLK-PP071140.D			Matrix:	WATER			
Analytical Method:	SW8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP071140.D	1		04/08/25	PP040825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	22.8		60 - 140		114%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.5		60 - 140		108%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071140.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:05  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:17:07 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	4.518	3.815	33330770	23969414	22.805	23.122
2) SA Decachloro...	10.246	8.859	25105022	16966968	23.850	21.526

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071140.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 11:05  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 11:17:07 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

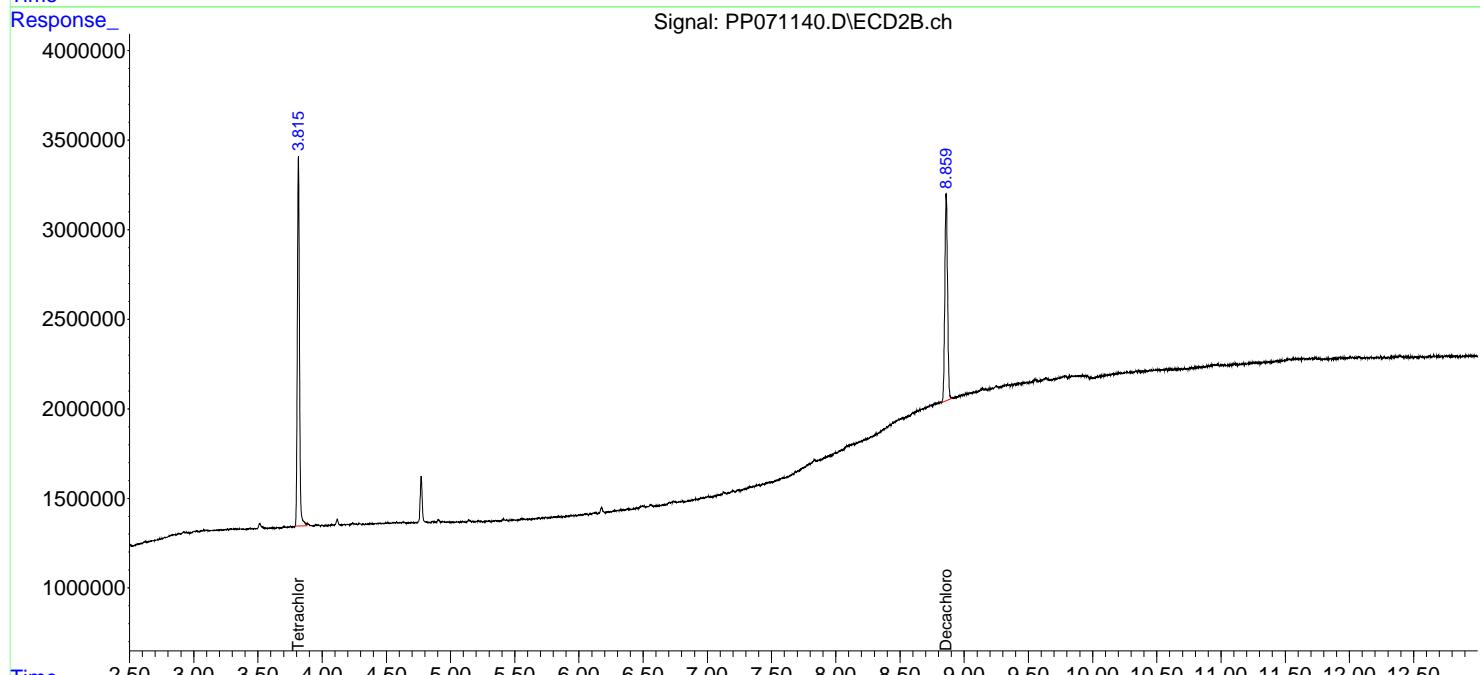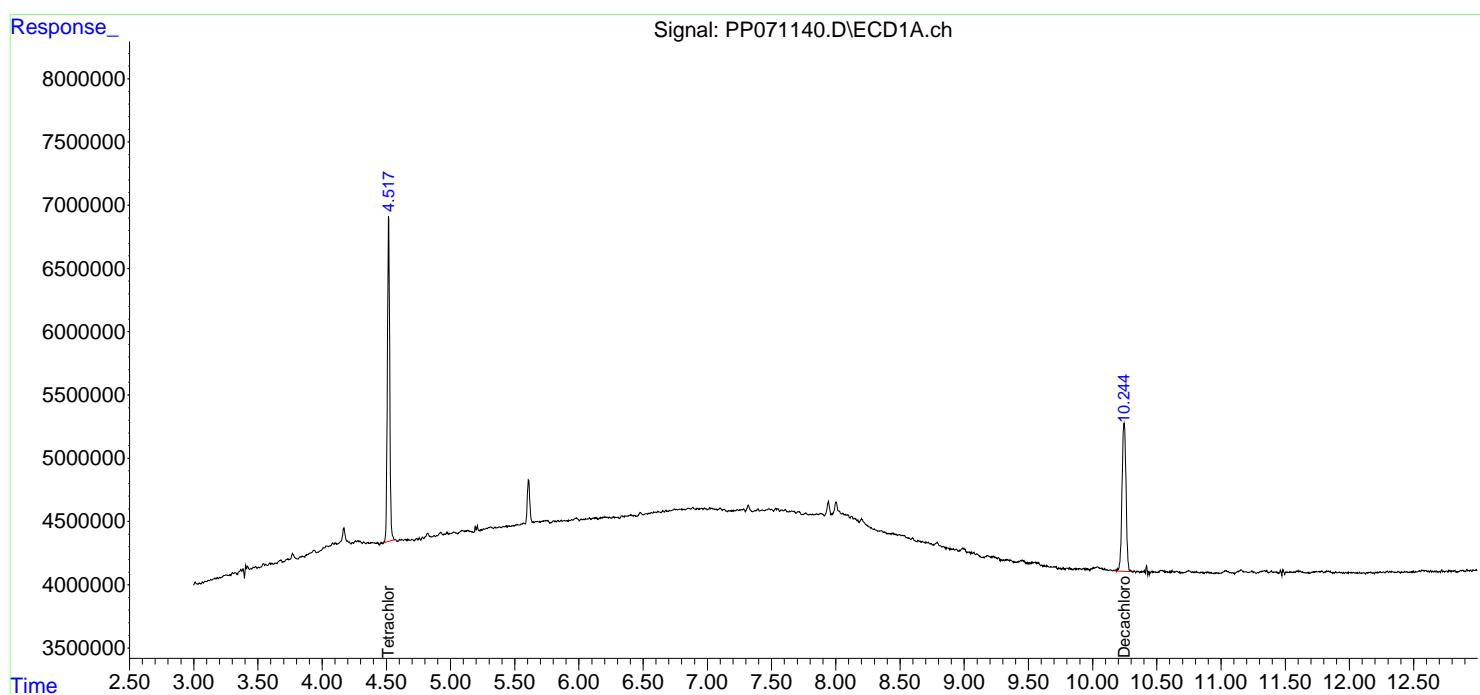

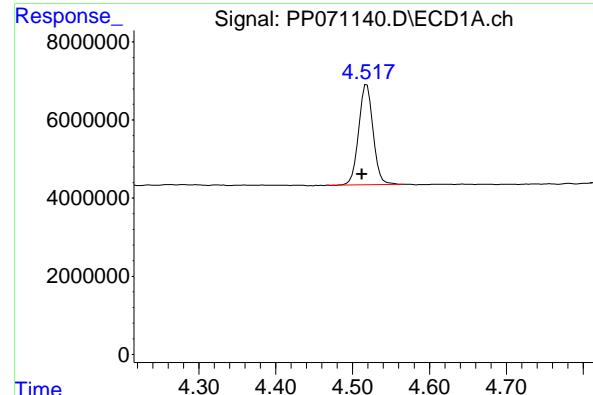


## #1 Tetrachloro-m-xylene

R.T.: 4.518 min  
Delta R.T.: 0.006 min  
Instrument: ECD\_P  
Response: 33330770  
Conc: 22.80 ng/ml ClientSampleId : I.BLK

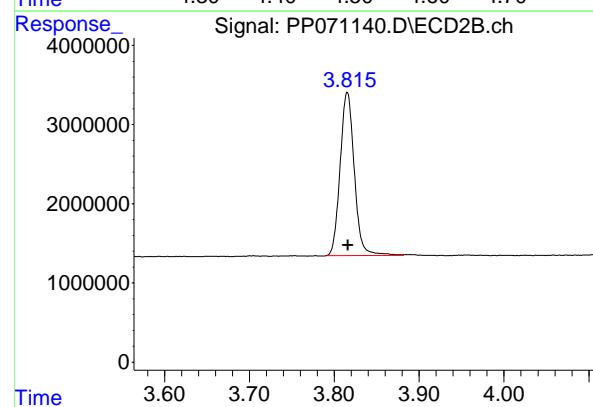


## #1 Tetrachloro-m-xylene

R.T.: 3.815 min  
Delta R.T.: 0.000 min  
Response: 23969414  
Conc: 23.12 ng/ml

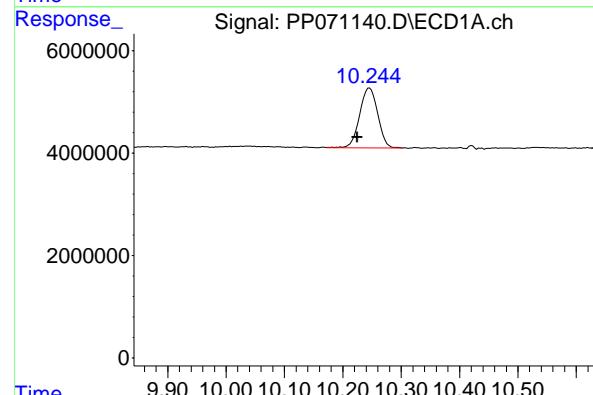

## #2 Decachlorobiphenyl

R.T.: 10.246 min  
Delta R.T.: 0.020 min  
Response: 25105022  
Conc: 23.85 ng/ml

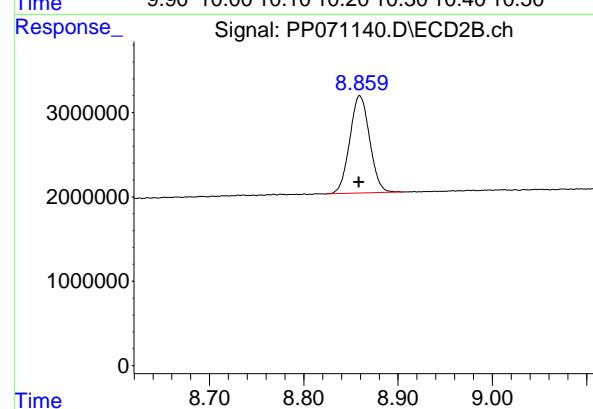

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 16966968  
Conc: 21.53 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/08/25			
Project:	Raymark Superfund Site			Date Received:	04/08/25			
Client Sample ID:	PIBLK-PP071155.D			SDG No.:	Q1730			
Lab Sample ID:	I.BLK-PP071155.D			Matrix:	WATER			
Analytical Method:	SW8082A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	PCB			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	5030							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP071155.D	1		04/08/25	PP040825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	0.25	U	0.097	0.25	0.50	ug/L
11104-28-2	Aroclor-1221	0.40	U	0.13	0.40	0.50	ug/L
11141-16-5	Aroclor-1232	0.25	U	0.096	0.25	0.50	ug/L
53469-21-9	Aroclor-1242	0.25	U	0.12	0.25	0.50	ug/L
12672-29-6	Aroclor-1248	0.25	U	0.071	0.25	0.50	ug/L
11097-69-1	Aroclor-1254	0.25	U	0.094	0.25	0.50	ug/L
11096-82-5	Aroclor-1260	0.25	U	0.081	0.25	0.50	ug/L
37324-23-5	Aroclor-1262	0.40	U	0.14	0.40	0.50	ug/L
11100-14-4	Aroclor-1268	0.25	U	0.11	0.25	0.50	ug/L
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	20.6		60 - 140		103%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.4		60 - 140		92%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071155.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 16:51  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 17:04:32 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachloro...	4.516	3.816	30070321	21846080	20.574	21.074
2) SA Decachloro...	10.242	8.859	22060594	14463728	20.958	18.350

#### Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071155.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 16:51  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 17:04:32 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

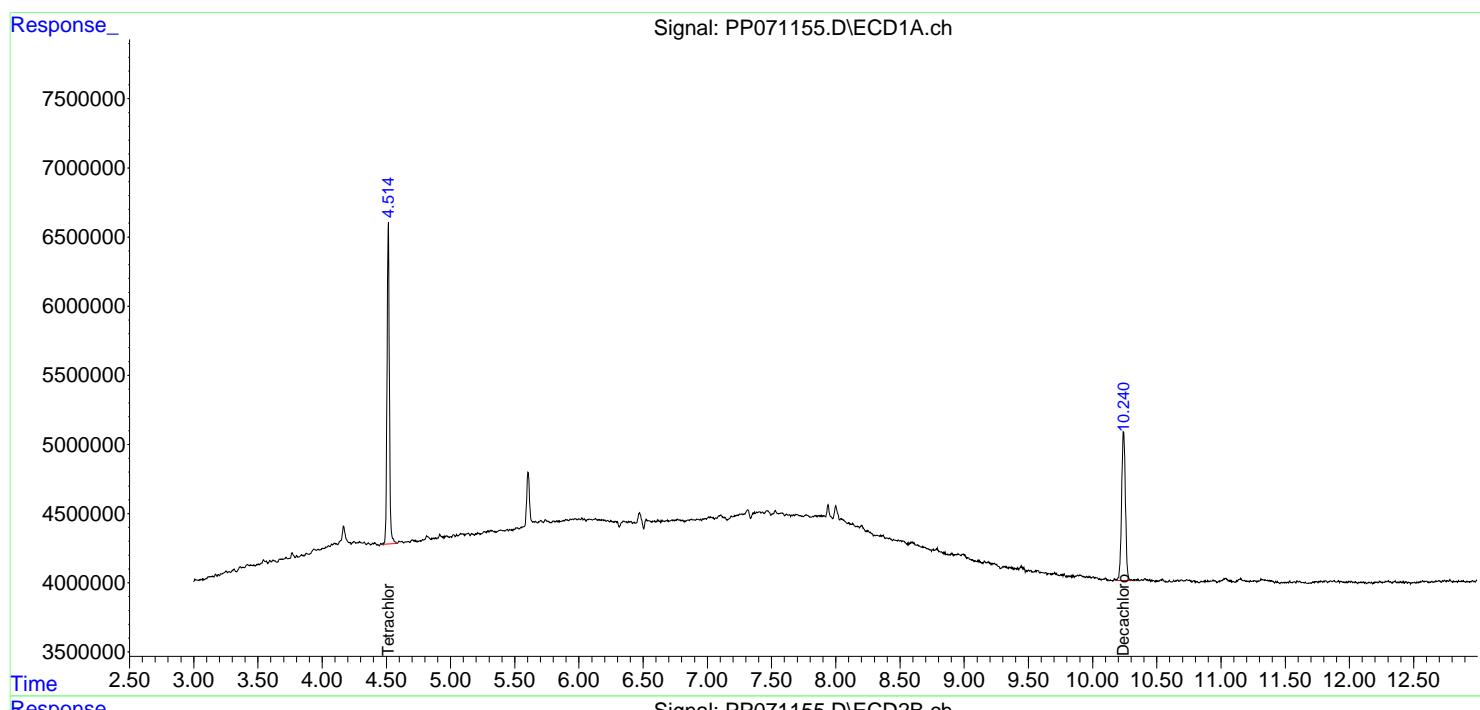

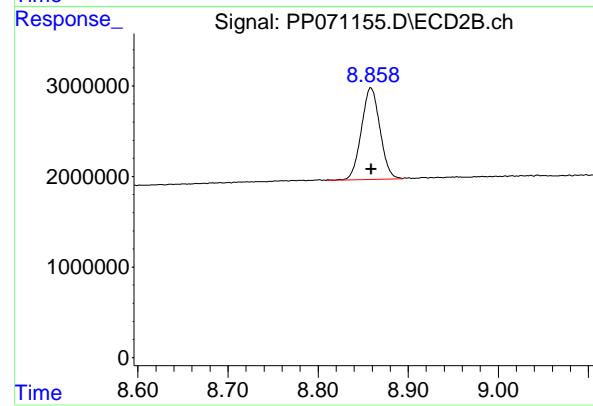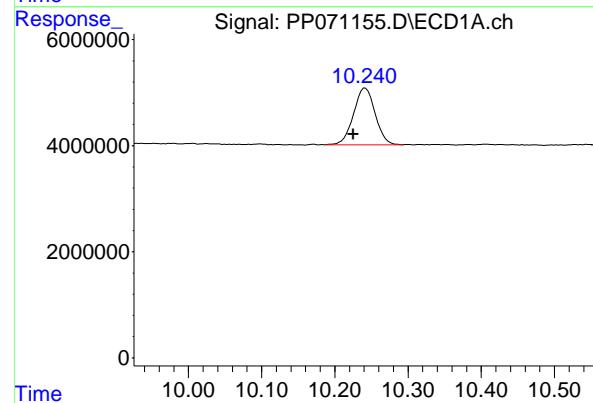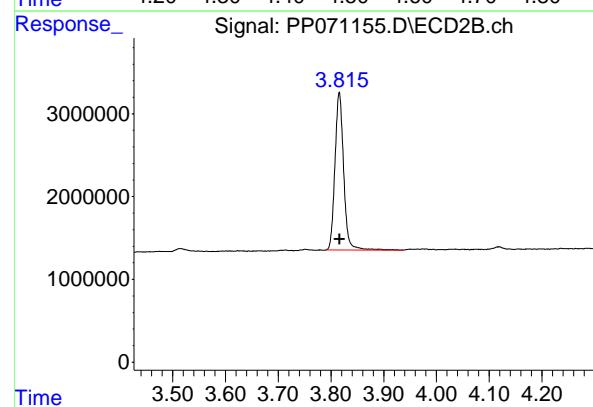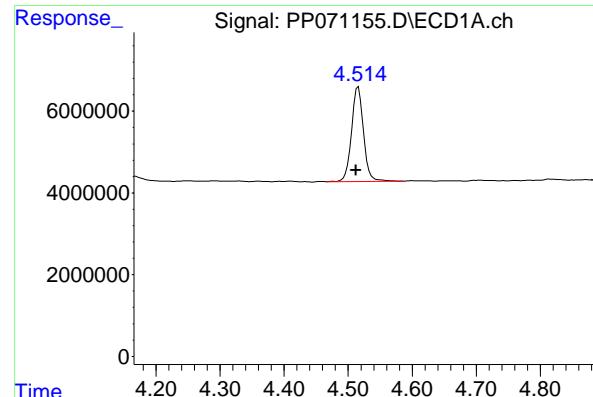

## #1 Tetrachloro-m-xylene

R.T.: 4.516 min  
 Delta R.T.: 0.004 min  
 Response: 30070321 ECD\_P  
 Conc: 20.57 ng/ml ClientSampleId : I.BLK

## #1 Tetrachloro-m-xylene

R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 21846080  
 Conc: 21.07 ng/ml

## #2 Decachlorobiphenyl

R.T.: 10.242 min  
 Delta R.T.: 0.016 min  
 Response: 22060594  
 Conc: 20.96 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.859 min  
 Delta R.T.: 0.000 min  
 Response: 14463728  
 Conc: 18.35 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	
Project:	Raymark Superfund Site			Date Received:	
Client Sample ID:	PB167469BS			SDG No.:	Q1730
Lab Sample ID:	PB167469BS			Matrix:	SOIL
Analytical Method:	SW8082A			% Solid:	100 Decanted:
Sample Wt/Vol:	30.02	Units:	g	Final Vol:	10000 uL
Soil Aliquot Vol:			uL	Test:	PCB
Extraction Type:				Injection Volume :	
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110284.D	1	04/07/25 08:20	04/07/25 19:41	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	141		3.90	8.30	17.0	ug/kg
11104-28-2	Aroclor-1221	13.0	U	4.00	13.0	17.0	ug/kg
11141-16-5	Aroclor-1232	8.30	U	3.70	8.30	17.0	ug/kg
53469-21-9	Aroclor-1242	8.30	U	4.00	8.30	17.0	ug/kg
12672-29-6	Aroclor-1248	13.0	U	5.90	13.0	17.0	ug/kg
11097-69-1	Aroclor-1254	8.30	U	3.20	8.30	17.0	ug/kg
37324-23-5	Aroclor-1262	13.0	U	5.00	13.0	17.0	ug/kg
11100-14-4	Aroclor-1268	8.30	U	3.60	8.30	17.0	ug/kg
11096-82-5	Aroclor-1260	134		3.20	8.30	17.0	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	19.9		44 - 130		99%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.1		60 - 125		95%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110284.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 19:41  
 Operator : YP/AJ  
 Sample : PB167469BS  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**PB167469BS**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:36:05 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.688	180.6E6	99143578	19.847	18.906
2) SA Decachlor...	8.740	8.691	146.7E6	41863016	19.080	17.255

Target Compounds

3) L1 AR-1016-1	4.782	4.769	142.0E6	74923264	421.865	408.847
4) L1 AR-1016-2	4.802	4.788	199.0E6	105.5E6	429.173	403.452
5) L1 AR-1016-3	4.858	4.964	137.1E6	57705339	427.778	407.010
6) L1 AR-1016-4	4.978	5.005	107.7E6	47781418	426.066	405.168
7) L1 AR-1016-5	5.236	5.218	113.5E6	60210398	412.871	393.741
31) L7 AR-1260-1	6.277	6.250	210.2E6	107.2E6	446.044	419.635
32) L7 AR-1260-2	6.465	6.438	251.9E6	124.0E6	422.920	413.030
33) L7 AR-1260-3	6.833	6.590	173.8E6	115.3E6	358.056	399.028
34) L7 AR-1260-4	7.093	7.062	166.9E6	76919777	393.513	357.636
35) L7 AR-1260-5	7.336	7.303	405.0E6	168.5E6	387.245	337.822



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\PO040725\  
 Data File : PO110284.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 19:41  
 Operator : YP/AJ  
 Sample : PB167469BS  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 PB167469BS

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:36:05 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

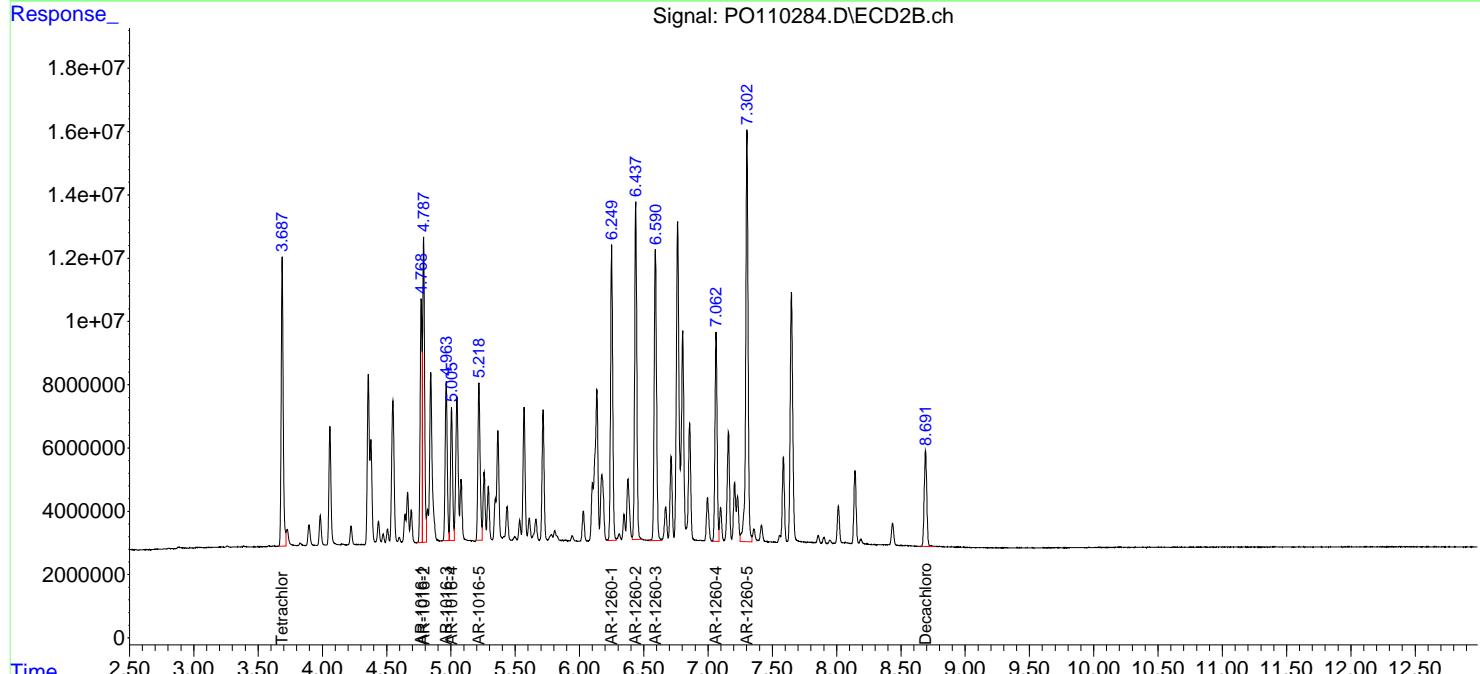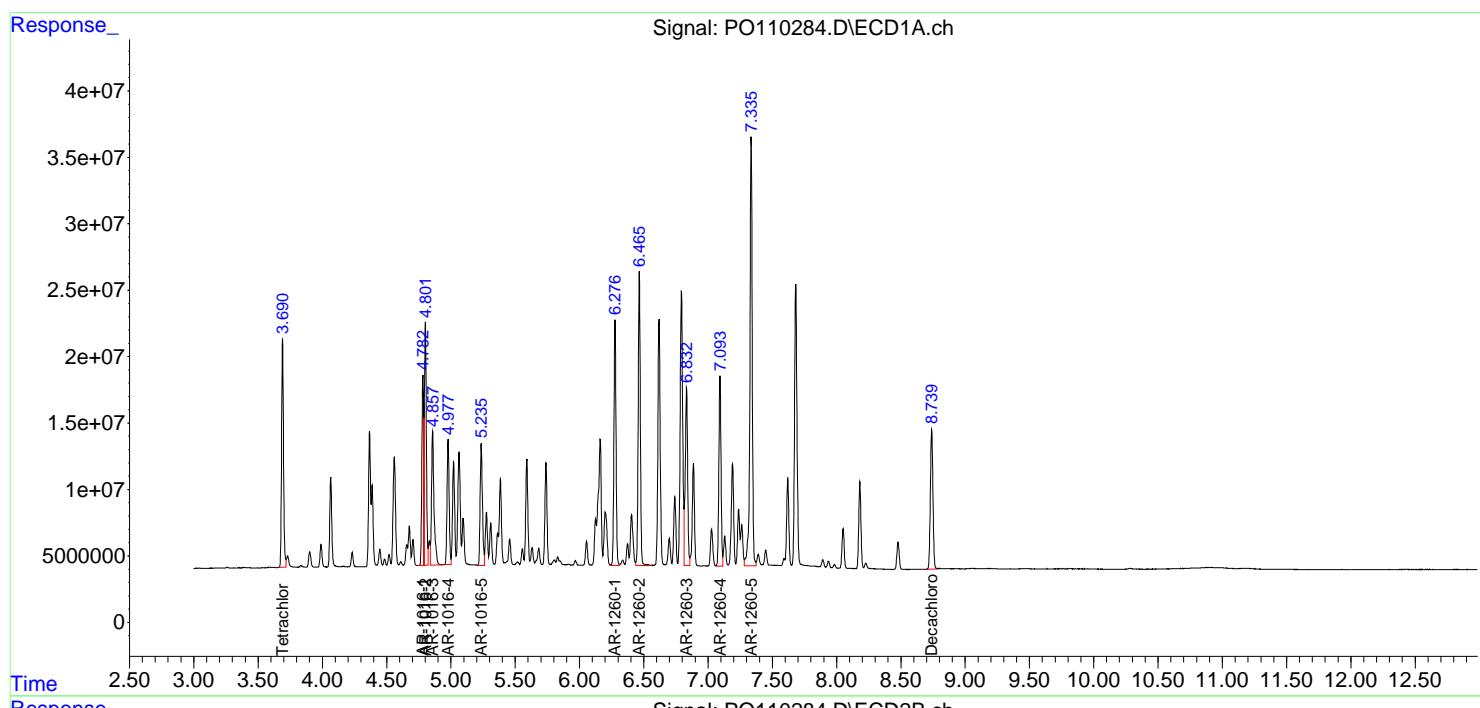

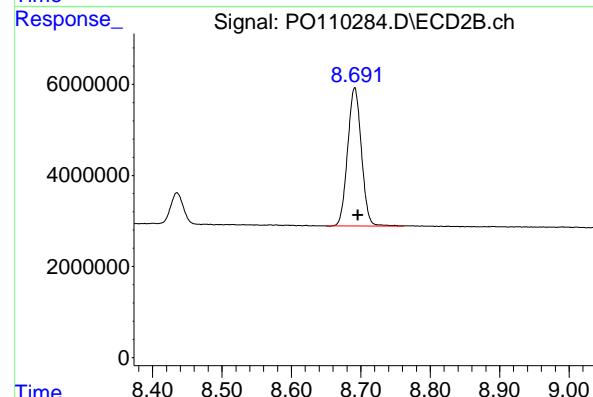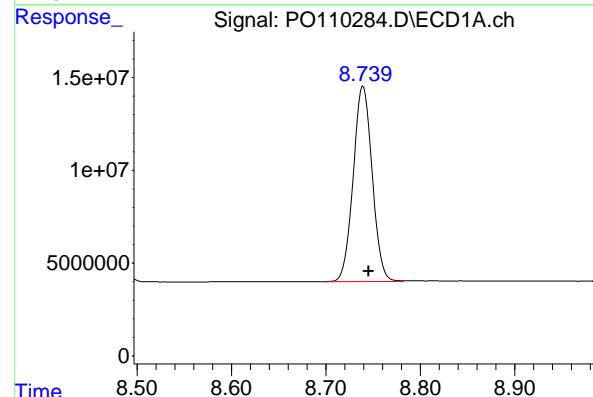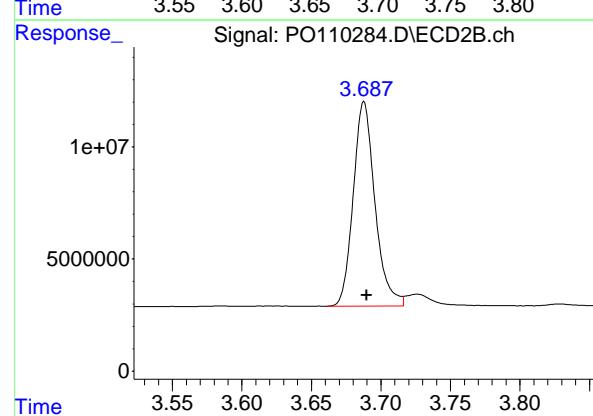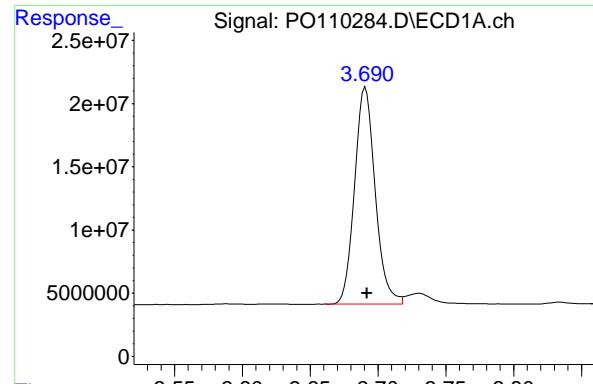

## #1 Tetrachloro-m-xylene

R.T.: 3.691 min  
 Delta R.T.: -0.001 min  
 Response: 180638940  
 Conc: 19.85 ng/ml

Instrument: ECD\_O  
 ClientSampleId: PB167469BS

## #1 Tetrachloro-m-xylene


R.T.: 3.688 min  
 Delta R.T.: -0.002 min  
 Response: 99143578  
 Conc: 18.91 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.740 min  
 Delta R.T.: -0.006 min  
 Response: 146698953  
 Conc: 19.08 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
 Delta R.T.: -0.005 min  
 Response: 41863016  
 Conc: 17.26 ng/ml

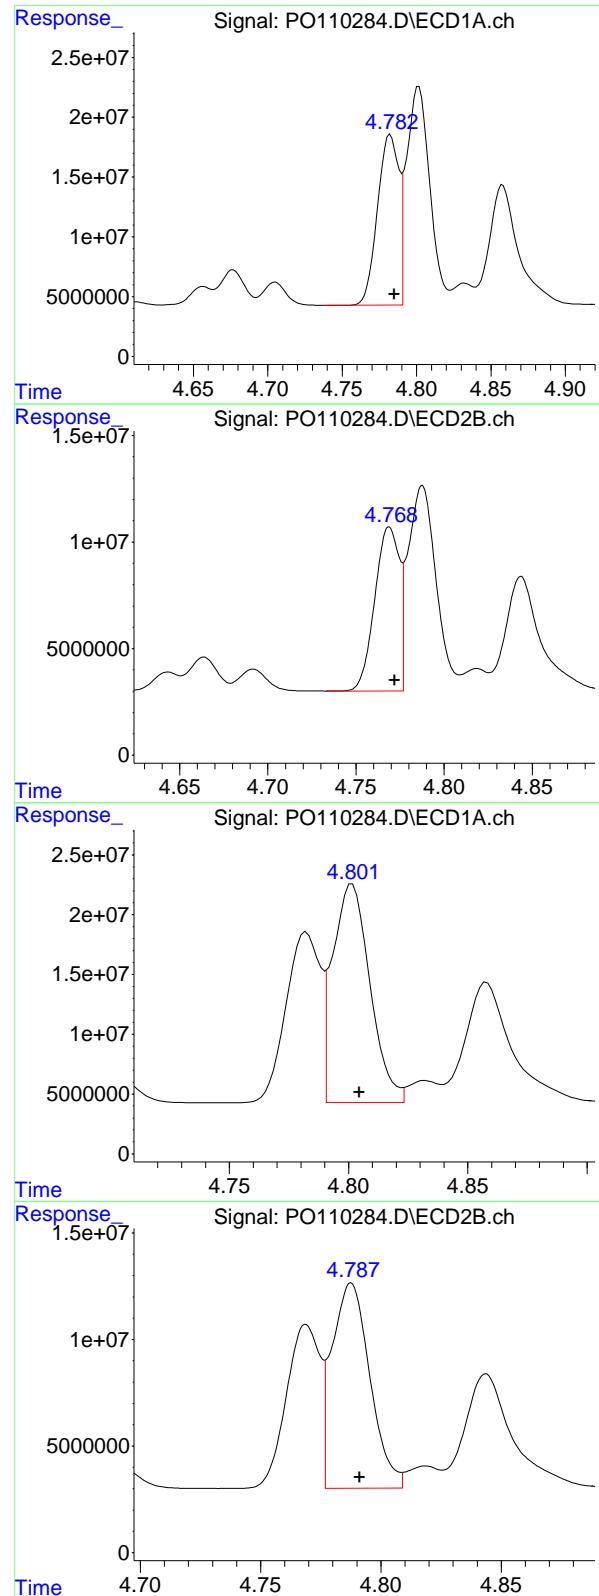

#3 AR-1016-1

R.T.: 4.782 min  
 Delta R.T.: -0.003 min  
 Response: 141976321  
 Conc: 421.87 ng/ml  
 Instrument: ECD\_O  
 ClientSampleId : PB167469BS

#3 AR-1016-1


R.T.: 4.769 min  
 Delta R.T.: -0.003 min  
 Response: 74923264  
 Conc: 408.85 ng/ml

#4 AR-1016-2

R.T.: 4.802 min  
 Delta R.T.: -0.003 min  
 Response: 199001347  
 Conc: 429.17 ng/ml

#4 AR-1016-2

R.T.: 4.788 min  
 Delta R.T.: -0.003 min  
 Response: 105504424  
 Conc: 403.45 ng/ml

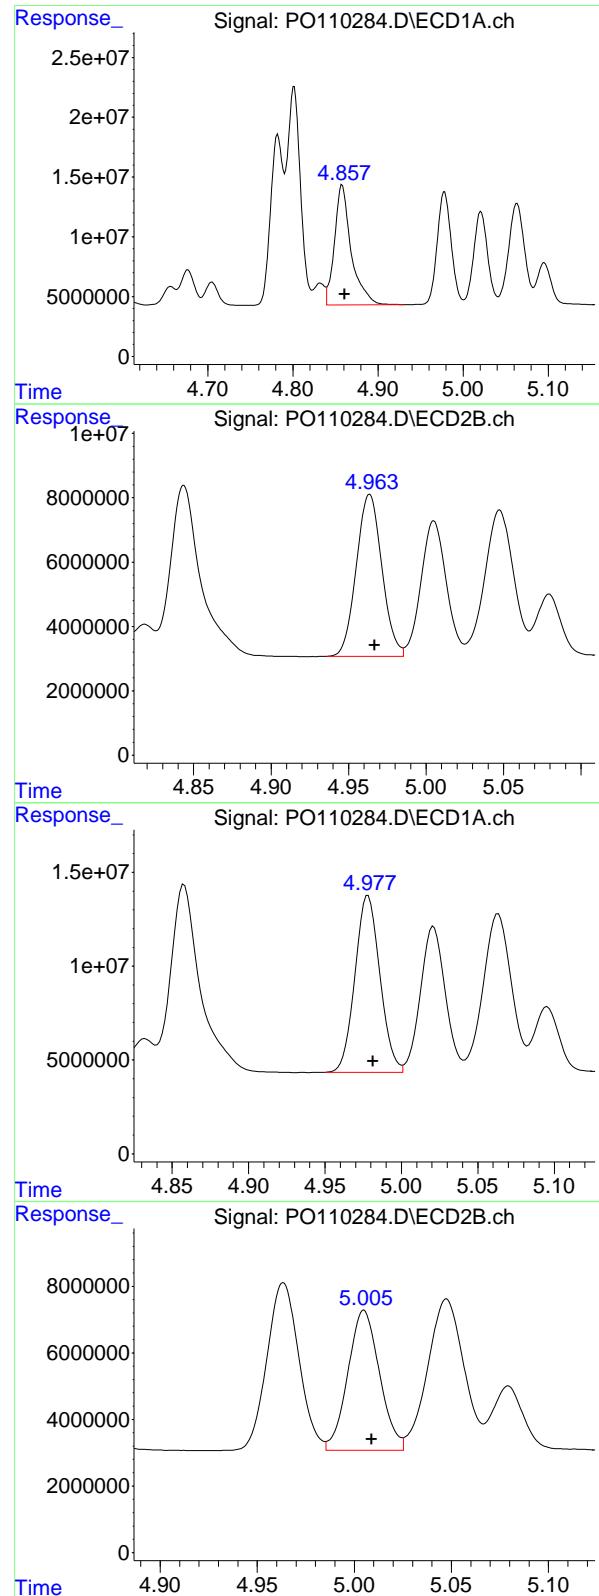

#5 AR-1016-3

R.T.: 4.858 min  
 Delta R.T.: -0.003 min  
 Response: 137139634  
 Conc: 427.78 ng/ml  
 Instrument: ECD\_O  
 ClientSampleId : PB167469BS

#5 AR-1016-3


R.T.: 4.964 min  
 Delta R.T.: -0.003 min  
 Response: 57705339  
 Conc: 407.01 ng/ml

#6 AR-1016-4

R.T.: 4.978 min  
 Delta R.T.: -0.003 min  
 Response: 107662297  
 Conc: 426.07 ng/ml

#6 AR-1016-4

R.T.: 5.005 min  
 Delta R.T.: -0.004 min  
 Response: 47781418  
 Conc: 405.17 ng/ml

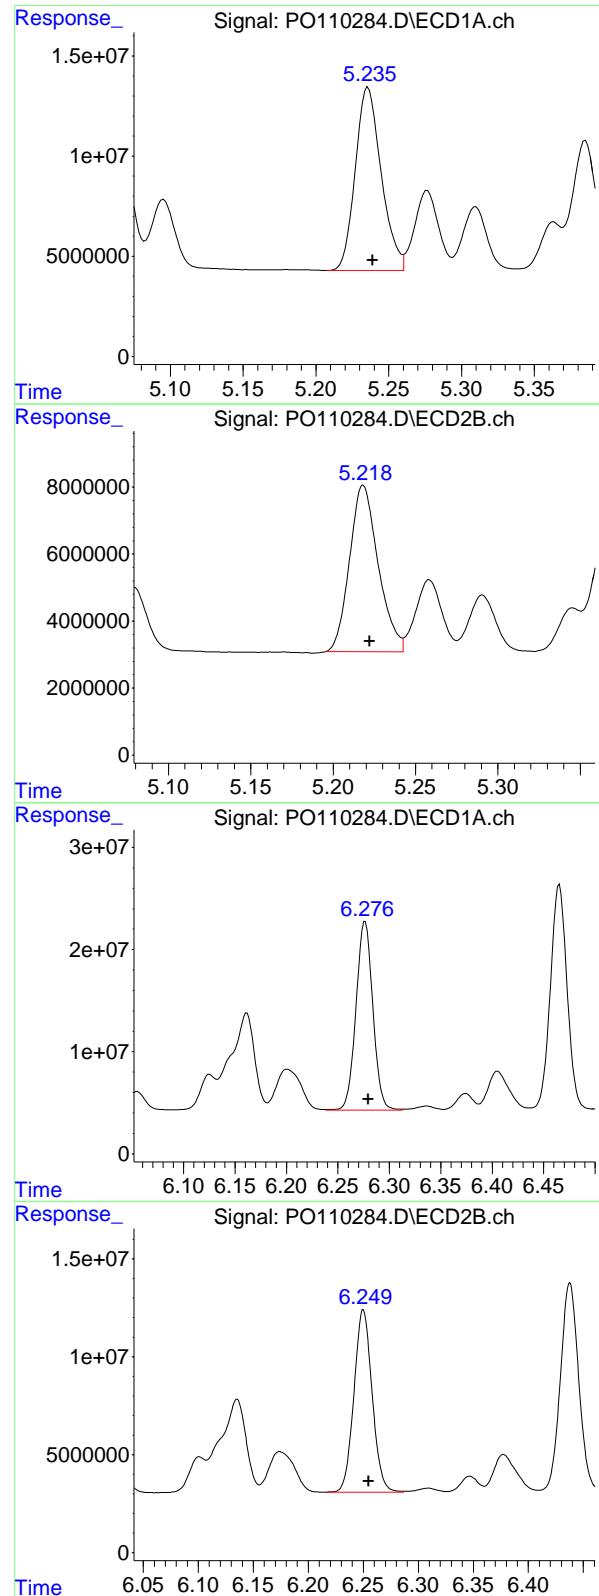

#7 AR-1016-5

R.T.: 5.236 min  
 Delta R.T.: -0.003 min  
 Response: 113484662 ECD\_O  
 Conc: 412.87 ng/ml ClientSampleId : PB167469BS

#7 AR-1016-5


R.T.: 5.218 min  
 Delta R.T.: -0.004 min  
 Response: 60210398  
 Conc: 393.74 ng/ml

#31 AR-1260-1

R.T.: 6.277 min  
 Delta R.T.: -0.003 min  
 Response: 210243094  
 Conc: 446.04 ng/ml

#31 AR-1260-1

R.T.: 6.250 min  
 Delta R.T.: -0.005 min  
 Response: 107192380  
 Conc: 419.64 ng/ml

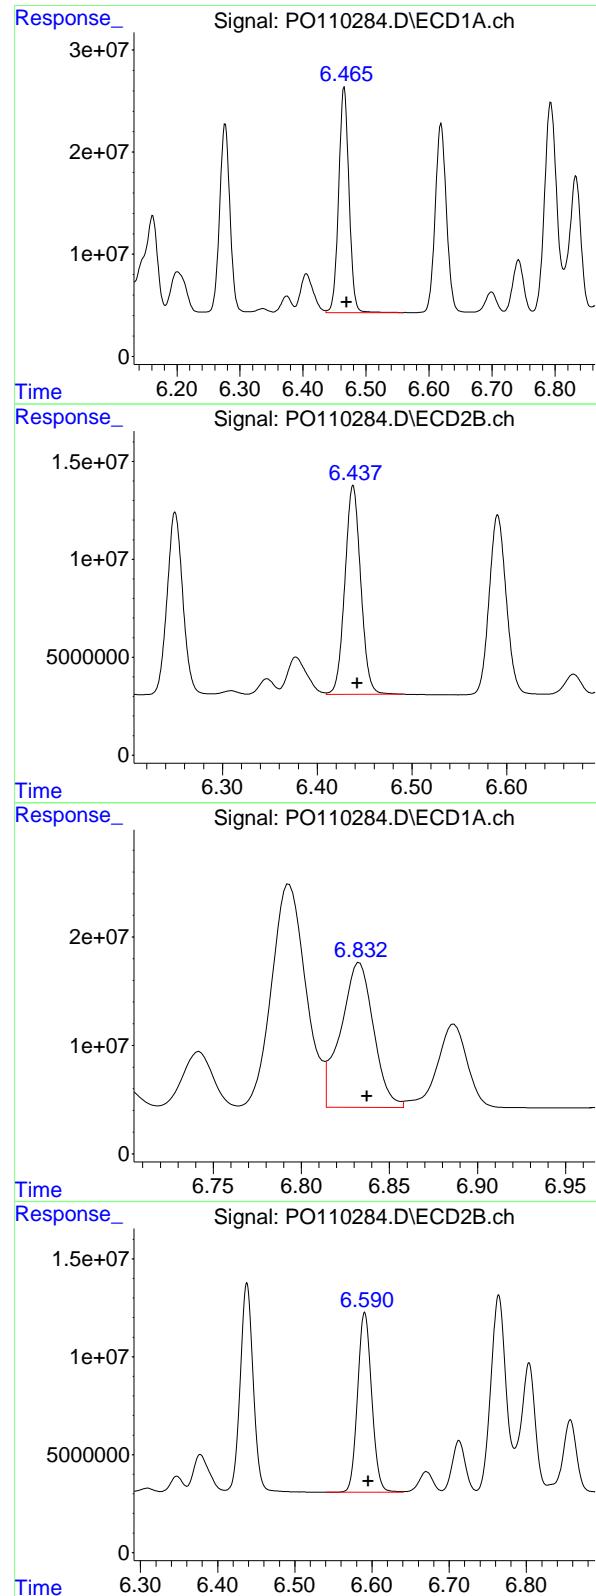

#32 AR-1260-2

R.T.: 6.465 min  
 Delta R.T.: -0.004 min  
 Response: 251857024  
 Conc: 422.92 ng/ml  
 Instrument: ECD\_O  
 ClientSampleId : PB167469BS

#32 AR-1260-2





R.T.: 6.438 min  
 Delta R.T.: -0.005 min  
 Response: 124026961  
 Conc: 413.03 ng/ml

#33 AR-1260-3

R.T.: 6.833 min  
 Delta R.T.: -0.004 min  
 Response: 173765242  
 Conc: 358.06 ng/ml

#33 AR-1260-3

R.T.: 6.590 min  
 Delta R.T.: -0.005 min  
 Response: 115311965  
 Conc: 399.03 ng/ml

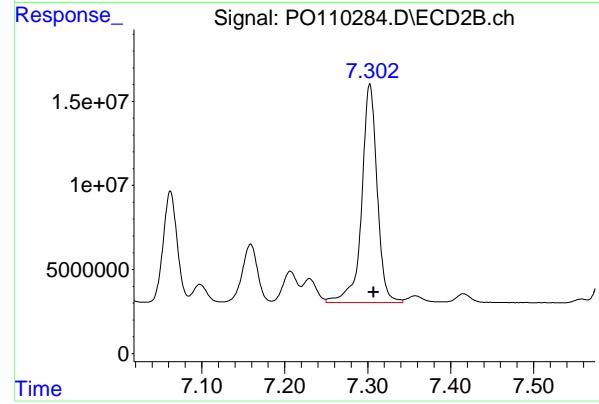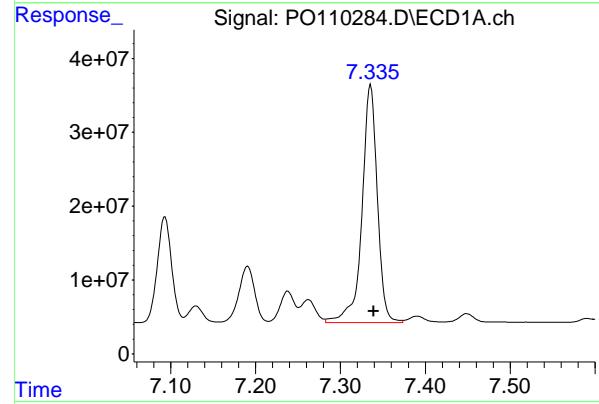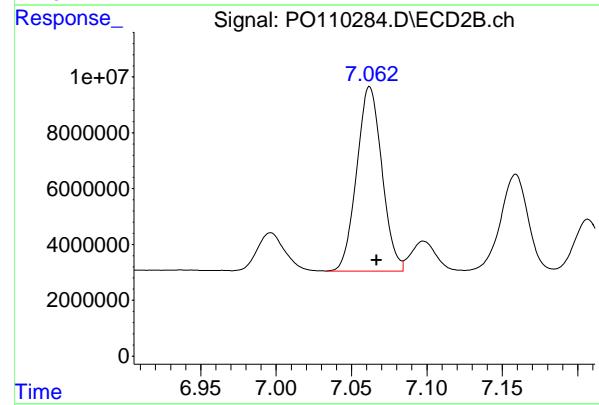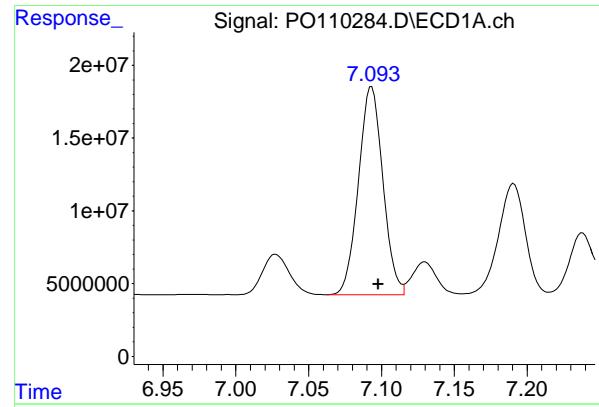

#34 AR-1260-4

R.T.: 7.093 min  
 Delta R.T.: -0.004 min  
 Response: 166915626  
 Conc: 393.51 ng/ml  
 Instrument: ECD\_O  
 ClientSampleId : PB167469BS

#34 AR-1260-4

R.T.: 7.062 min  
 Delta R.T.: -0.005 min  
 Response: 76919777  
 Conc: 357.64 ng/ml

#35 AR-1260-5

R.T.: 7.336 min  
 Delta R.T.: -0.004 min  
 Response: 404998251  
 Conc: 387.24 ng/ml

#35 AR-1260-5

R.T.: 7.303 min  
 Delta R.T.: -0.005 min  
 Response: 168470492  
 Conc: 337.82 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-VSL-16-040325MS			SDG No.:	Q1730	
Lab Sample ID:	Q1730-03MS			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	94.5	Decanted:
Sample Wt/Vol:	30.05	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110271.D	1	04/07/25 08:20	04/07/25 14:15	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	170		4.20	8.80	18.0	ug/kg
11104-28-2	Aroclor-1221	13.7	U	4.30	13.7	18.0	ug/kg
11141-16-5	Aroclor-1232	8.80	U	3.90	8.80	18.0	ug/kg
53469-21-9	Aroclor-1242	8.80	U	4.20	8.80	18.0	ug/kg
12672-29-6	Aroclor-1248	13.7	U	6.30	13.7	18.0	ug/kg
11097-69-1	Aroclor-1254	8.80	U	3.40	8.80	18.0	ug/kg
37324-23-5	Aroclor-1262	13.7	U	5.30	13.7	18.0	ug/kg
11100-14-4	Aroclor-1268	8.80	U	3.80	8.80	18.0	ug/kg
11096-82-5	Aroclor-1260	157		3.40	8.80	18.0	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	22.8		44 - 130		114%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.9		60 - 125		104%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110271.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 14:15  
 Operator : YP/AJ  
 Sample : Q1730-03MS  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-VSL-16-040325MS**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 14:28:33 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.690	3.687	207.8E6	114.5E6	22.829	21.843
2) SA Decachlor...	8.740	8.691	160.6E6	43661585	20.882	17.997

Target Compounds

3) L1 AR-1016-1	4.782	4.768	163.4E6	86371640	485.641	471.320
4) L1 AR-1016-2	4.802	4.787	226.9E6	123.3E6	489.395	471.405
5) L1 AR-1016-3	4.858	4.963	156.9E6	66829797	489.339	471.367
6) L1 AR-1016-4	4.978	5.005	122.7E6	54685236	485.623	463.710
7) L1 AR-1016-5	5.236	5.218	127.1E6	69082264	462.402	451.758
31) L7 AR-1260-1	6.276	6.250	237.9E6	119.0E6	504.637	465.860
32) L7 AR-1260-2	6.466	6.438	285.8E6	136.5E6	479.876	454.662
33) L7 AR-1260-3	6.833	6.591	199.0E6	126.8E6	409.960	438.894
34) L7 AR-1260-4	7.094	7.062	183.3E6	86758507	432.156	403.381
35) L7 AR-1260-5	7.335	7.303	418.2E6	188.7E6	399.895	378.330



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110271.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 14:15  
 Operator : YP/AJ  
 Sample : Q1730-03MS  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 OU4-VSL-16-040325MS

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 14:28:33 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

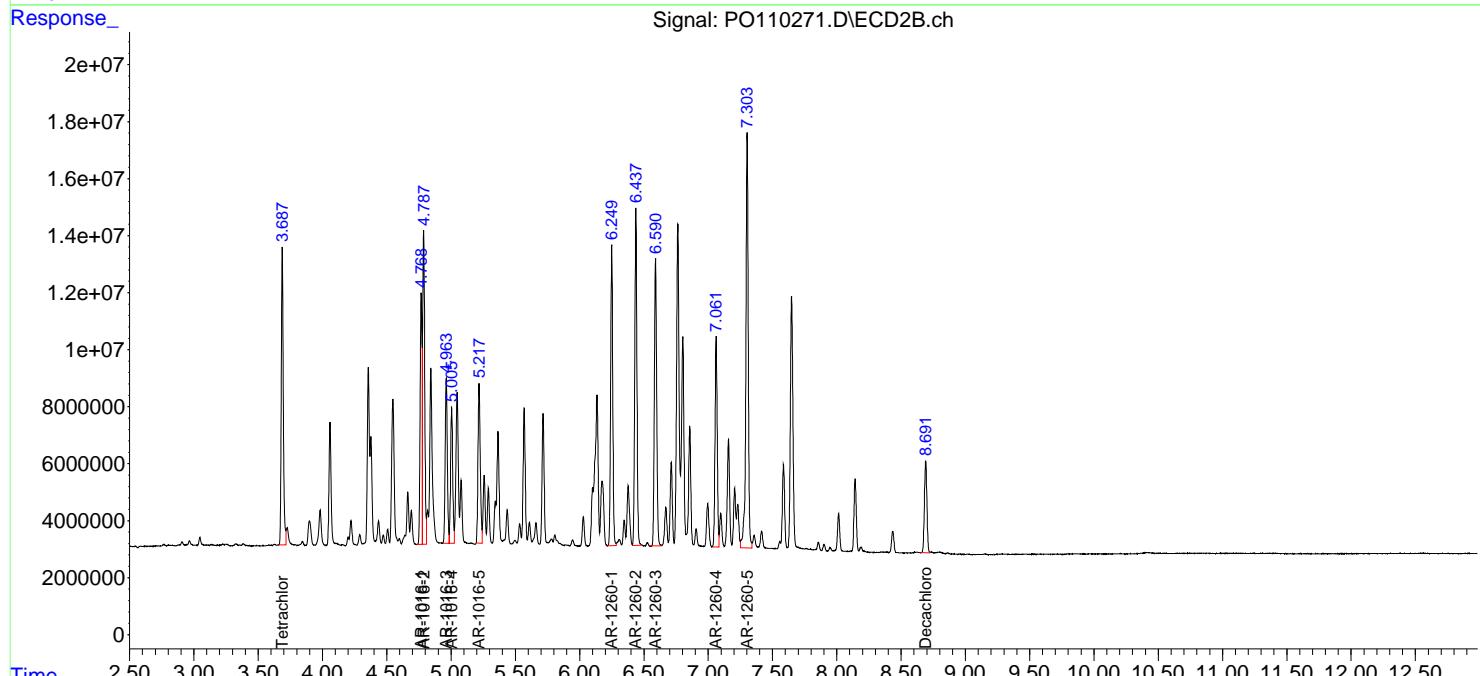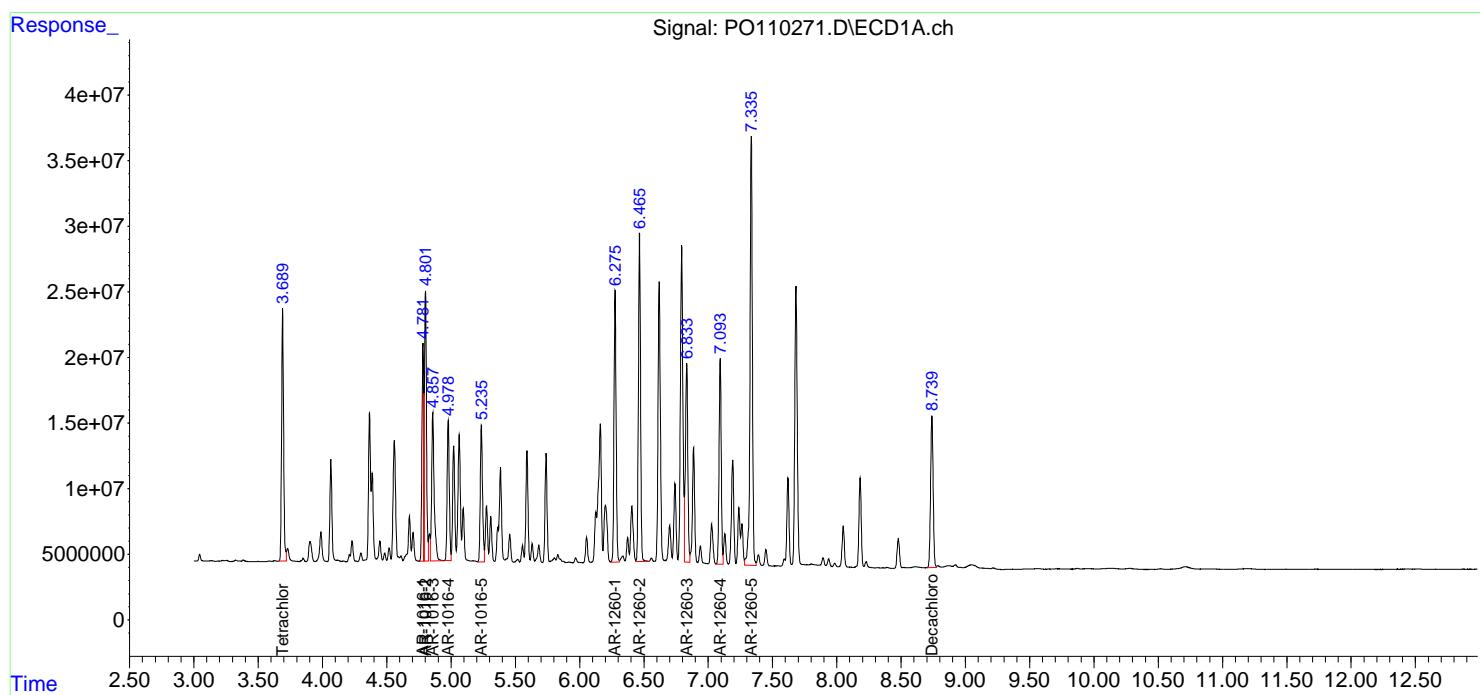

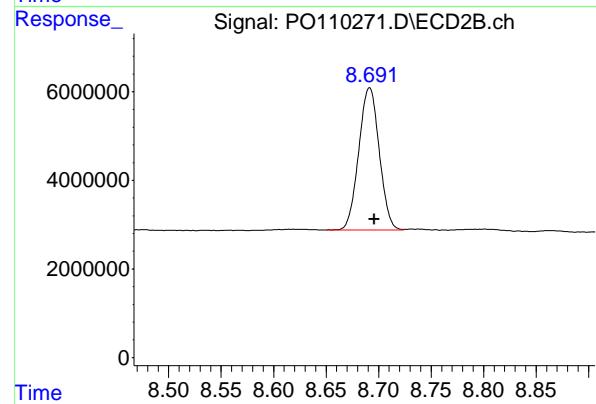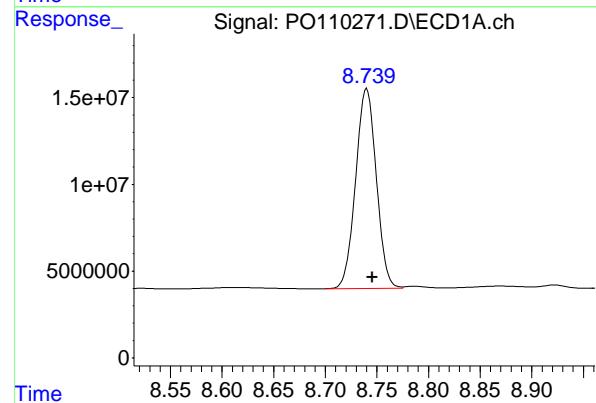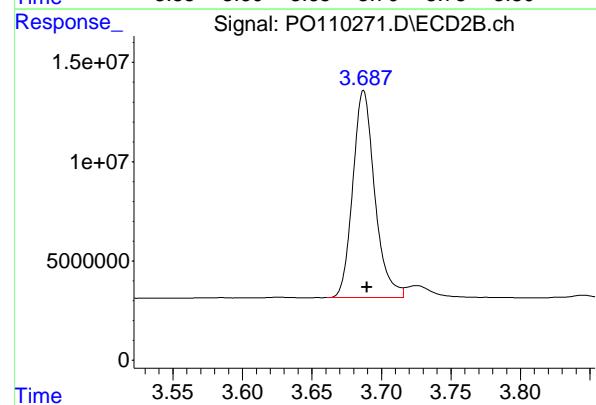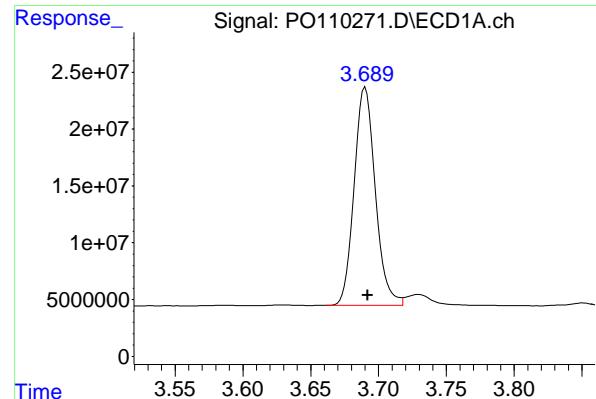

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: -0.002 min  
 Response: 207776497  
 Conc: 22.83 ng/ml

Instrument: ECD\_O  
 ClientSampleId: OU4-VSL-16-040325MS

## #1 Tetrachloro-m-xylene


R.T.: 3.687 min  
 Delta R.T.: -0.003 min  
 Response: 114548641  
 Conc: 21.84 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.740 min  
 Delta R.T.: -0.005 min  
 Response: 160555921  
 Conc: 20.88 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.691 min  
 Delta R.T.: -0.004 min  
 Response: 43661585  
 Conc: 18.00 ng/ml

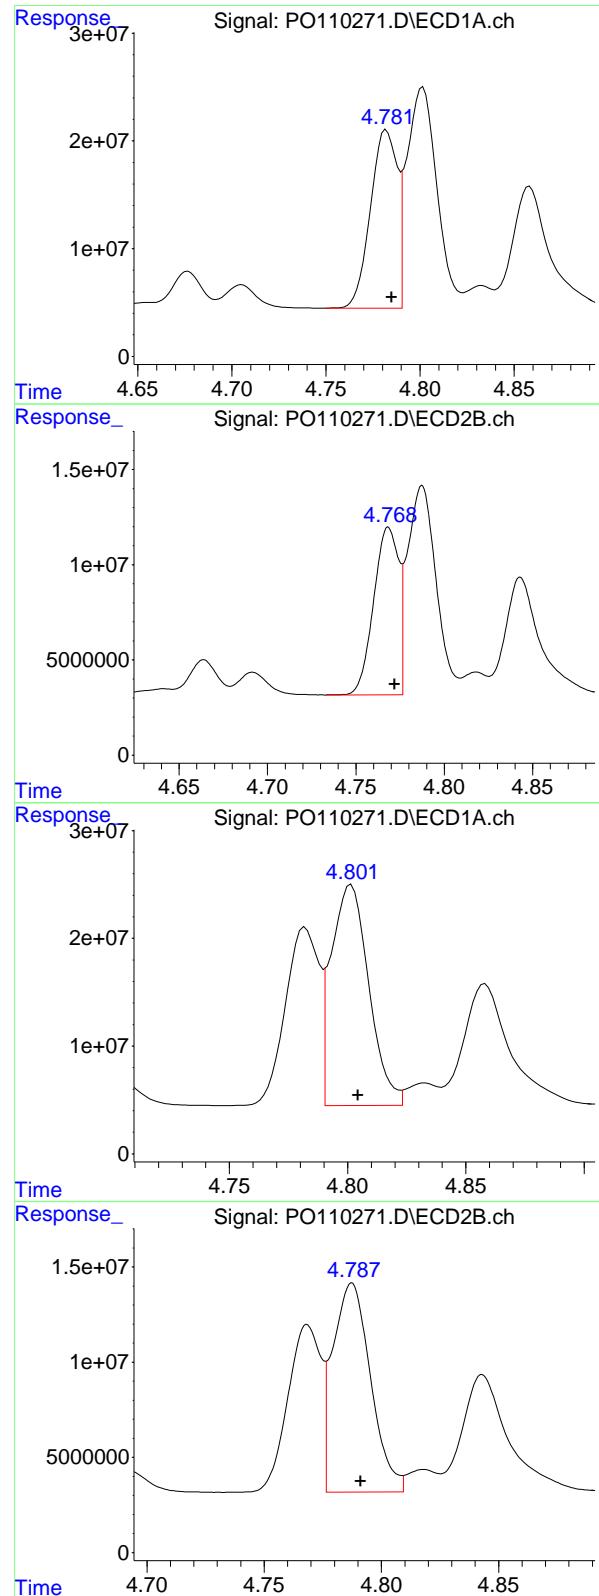

#3 AR-1016-1

R.T.: 4.782 min  
 Delta R.T.: -0.003 min  
 Response: 163439503  
 Conc: 485.64 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId :** OU4-VSL-16-040325MS

#3 AR-1016-1


R.T.: 4.768 min  
 Delta R.T.: -0.003 min  
 Response: 86371640  
 Conc: 471.32 ng/ml

#4 AR-1016-2

R.T.: 4.802 min  
 Delta R.T.: -0.003 min  
 Response: 226925626  
 Conc: 489.40 ng/ml

#4 AR-1016-2

R.T.: 4.787 min  
 Delta R.T.: -0.004 min  
 Response: 123274570  
 Conc: 471.41 ng/ml

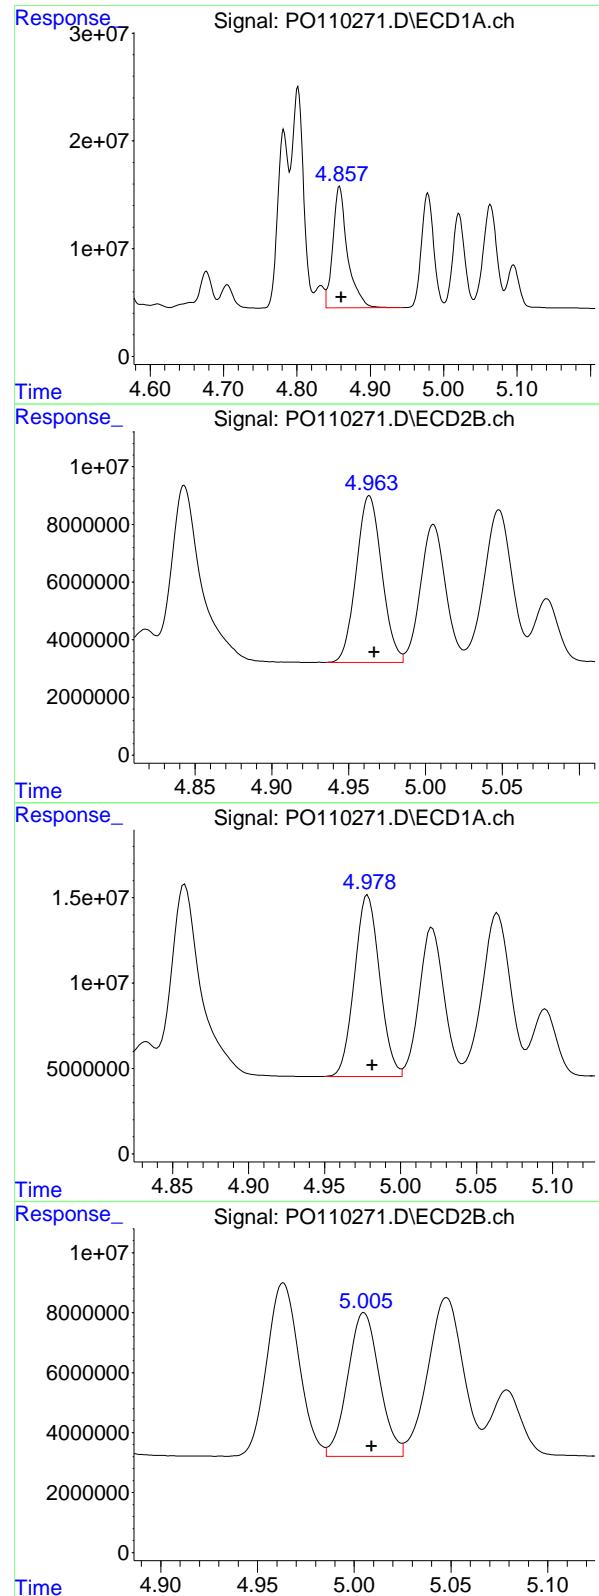

#5 AR-1016-3

R.T.: 4.858 min  
 Delta R.T.: -0.003 min  
 Response: 156875297  
 Conc: 489.34 ng/ml  
**Instrument:** ECD\_O  
**ClientSampleId :** OU4-VSL-16-040325MS

#5 AR-1016-3



R.T.: 4.963 min  
 Delta R.T.: -0.003 min  
 Response: 66829797  
 Conc: 471.37 ng/ml

#6 AR-1016-4

R.T.: 4.978 min  
 Delta R.T.: -0.003 min  
 Response: 122711855  
 Conc: 485.62 ng/ml

#6 AR-1016-4

R.T.: 5.005 min  
 Delta R.T.: -0.004 min  
 Response: 54685236  
 Conc: 463.71 ng/ml

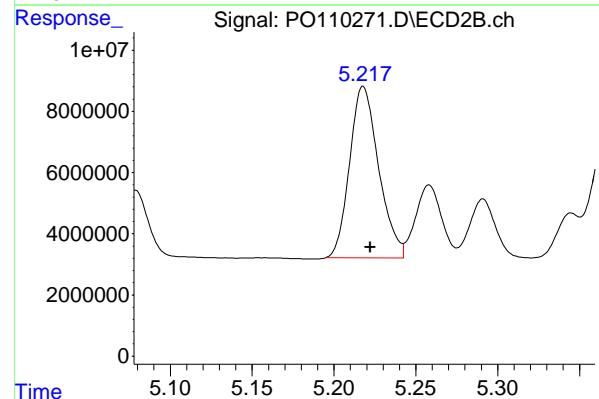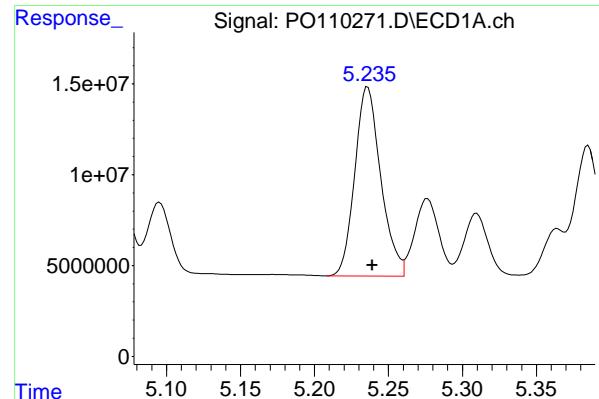

#7 AR-1016-5

R.T.: 5.236 min  
 Delta R.T.: -0.003 min  
 Response: 127098994 ECD\_O  
 Conc: 462.40 ng/ml ClientSampleId : OU4-VSL-16-040325MS

#7 AR-1016-5


R.T.: 5.218 min  
 Delta R.T.: -0.004 min  
 Response: 69082264  
 Conc: 451.76 ng/ml

#31 AR-1260-1

R.T.: 6.276 min  
 Delta R.T.: -0.004 min  
 Response: 237861115  
 Conc: 504.64 ng/ml

#31 AR-1260-1

R.T.: 6.250 min  
 Delta R.T.: -0.005 min  
 Response: 119000242  
 Conc: 465.86 ng/ml

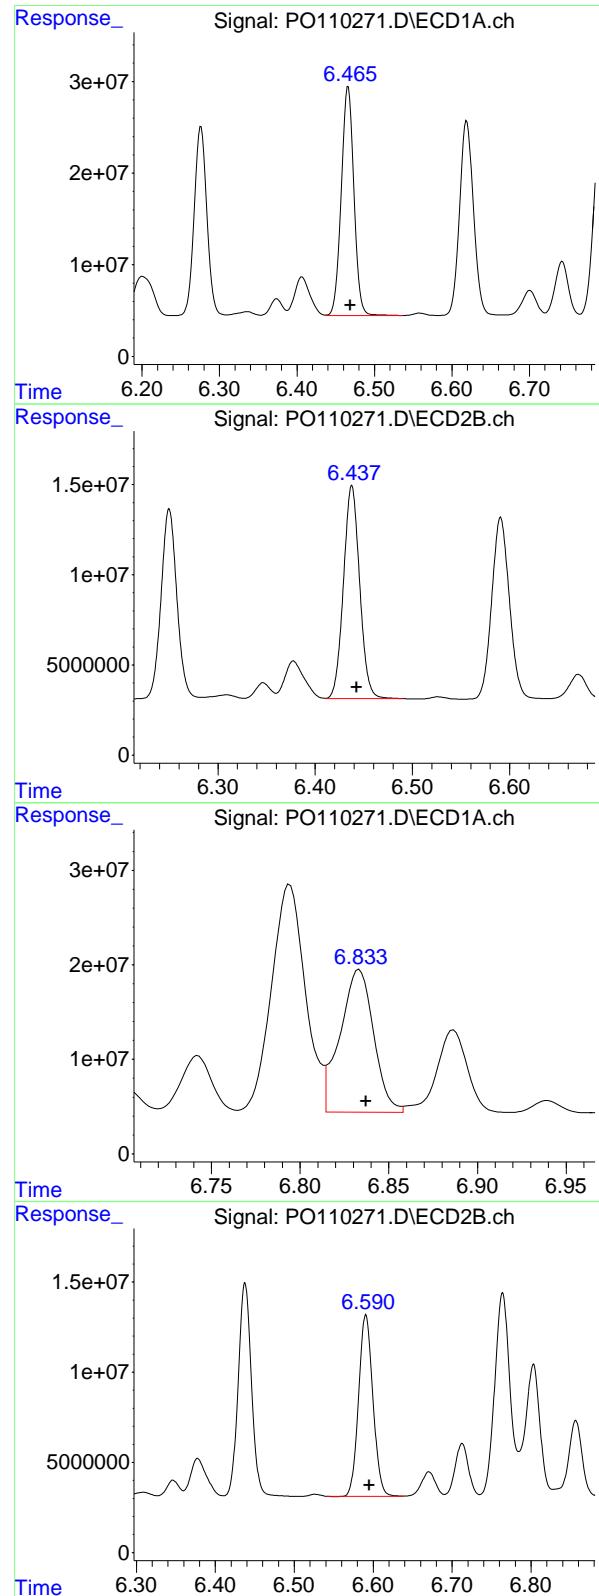

#32 AR-1260-2

R.T.: 6.466 min  
 Delta R.T.: -0.003 min  
 Response: 285775432 ECD\_O  
 Conc: 479.88 ng/ml ClientSampleId : OU4-VSL-16-040325MS

#32 AR-1260-2





R.T.: 6.438 min  
 Delta R.T.: -0.005 min  
 Response: 136528501  
 Conc: 454.66 ng/ml

#33 AR-1260-3

R.T.: 6.833 min  
 Delta R.T.: -0.004 min  
 Response: 198954290  
 Conc: 409.96 ng/ml

#33 AR-1260-3

R.T.: 6.591 min  
 Delta R.T.: -0.005 min  
 Response: 126832599  
 Conc: 438.89 ng/ml

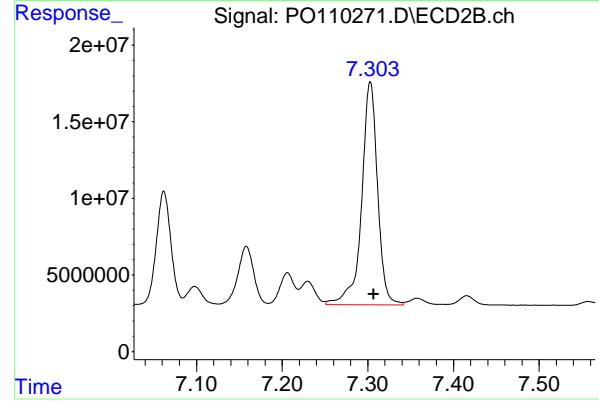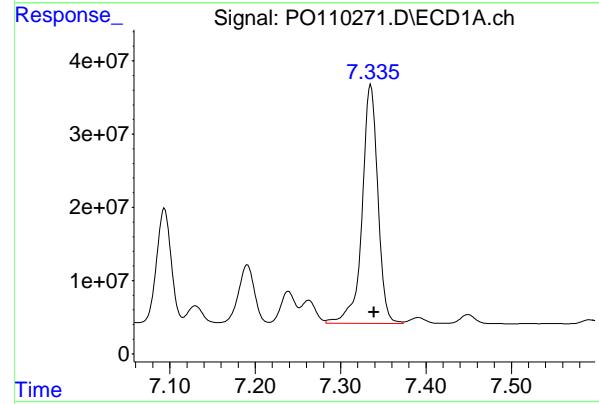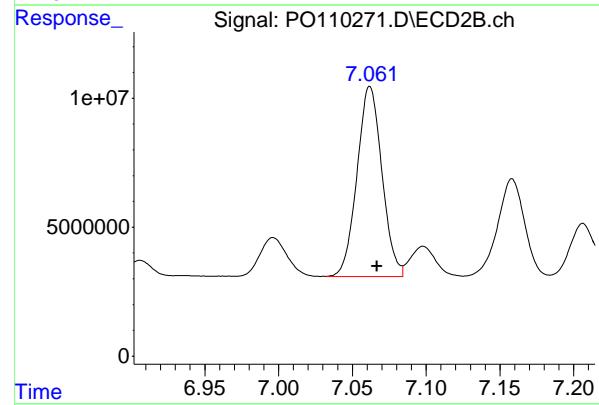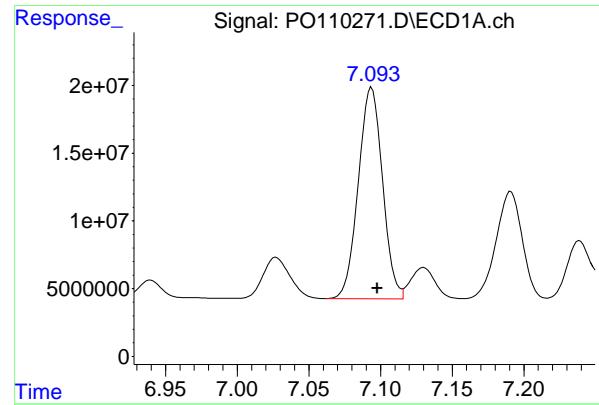

#34 AR-1260-4

R.T.: 7.094 min  
 Delta R.T.: -0.004 min  
 Response: 183306711 ECD\_O  
 Conc: 432.16 ng/ml ClientSampleId : OU4-VSL-16-040325MS

#34 AR-1260-4

R.T.: 7.062 min  
 Delta R.T.: -0.005 min  
 Response: 86758507  
 Conc: 403.38 ng/ml

#35 AR-1260-5

R.T.: 7.335 min  
 Delta R.T.: -0.004 min  
 Response: 418228862  
 Conc: 399.90 ng/ml

#35 AR-1260-5

R.T.: 7.303 min  
 Delta R.T.: -0.004 min  
 Response: 188671824  
 Conc: 378.33 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/03/25	
Project:	Raymark Superfund Site			Date Received:	04/04/25	
Client Sample ID:	OU4-VSL-16-040325MSD			SDG No.:	Q1730	
Lab Sample ID:	Q1730-03MSD			Matrix:	SOIL	
Analytical Method:	SW8082A			% Solid:	94.5	Decanted:
Sample Wt/Vol:	30.02	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	PCB	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	SW3541B					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110272.D	1	04/07/25 08:20	04/07/25 14:33	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
12674-11-2	Aroclor-1016	164		4.20	8.80	18.0	ug/kg
11104-28-2	Aroclor-1221	13.7	U	4.30	13.7	18.0	ug/kg
11141-16-5	Aroclor-1232	8.80	U	3.90	8.80	18.0	ug/kg
53469-21-9	Aroclor-1242	8.80	U	4.20	8.80	18.0	ug/kg
12672-29-6	Aroclor-1248	13.7	U	6.30	13.7	18.0	ug/kg
11097-69-1	Aroclor-1254	8.80	U	3.40	8.80	18.0	ug/kg
37324-23-5	Aroclor-1262	13.7	U	5.30	13.7	18.0	ug/kg
11100-14-4	Aroclor-1268	8.80	U	3.80	8.80	18.0	ug/kg
11096-82-5	Aroclor-1260	153		3.40	8.80	18.0	ug/kg
<b>SURROGATES</b>							
877-09-8	Tetrachloro-m-xylene	21.6		44 - 130		108%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.8		60 - 125		99%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110272.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 14:33  
 Operator : YP/AJ  
 Sample : Q1730-03MSD  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**OU4-VSL-16-040325MSD**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 14:58:52 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

1) SA Tetrachlor...	3.690	3.687	196.9E6	109.1E6	21.633	20.795
2) SA Decachlor...	8.739	8.690	152.2E6	41848584	19.800	17.249

**Target Compounds**

3) L1 AR-1016-1	4.782	4.768	156.1E6	82580554	463.781	450.632
4) L1 AR-1016-2	4.801	4.788	219.3E6	118.8E6	472.954	454.443
5) L1 AR-1016-3	4.857	4.963	151.9E6	64490825	473.697	454.870
6) L1 AR-1016-4	4.978	5.005	118.8E6	52631687	470.083	446.297
7) L1 AR-1016-5	5.235	5.217	123.9E6	66656091	450.663	435.892
31) L7 AR-1260-1	6.276	6.250	225.9E6	115.3E6	479.366	451.204
32) L7 AR-1260-2	6.466	6.438	276.1E6	132.5E6	463.567	441.258
33) L7 AR-1260-3	6.833	6.590	196.5E6	122.9E6	404.805	425.130
34) L7 AR-1260-4	7.093	7.061	180.2E6	84267581	424.947	391.799
35) L7 AR-1260-5	7.335	7.302	409.9E6	182.8E6	391.944	366.611



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110272.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 14:33  
 Operator : YP/AJ  
 Sample : Q1730-03MSD  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 OU4-VSL-16-040325MSD

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 07 14:58:52 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mm x 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

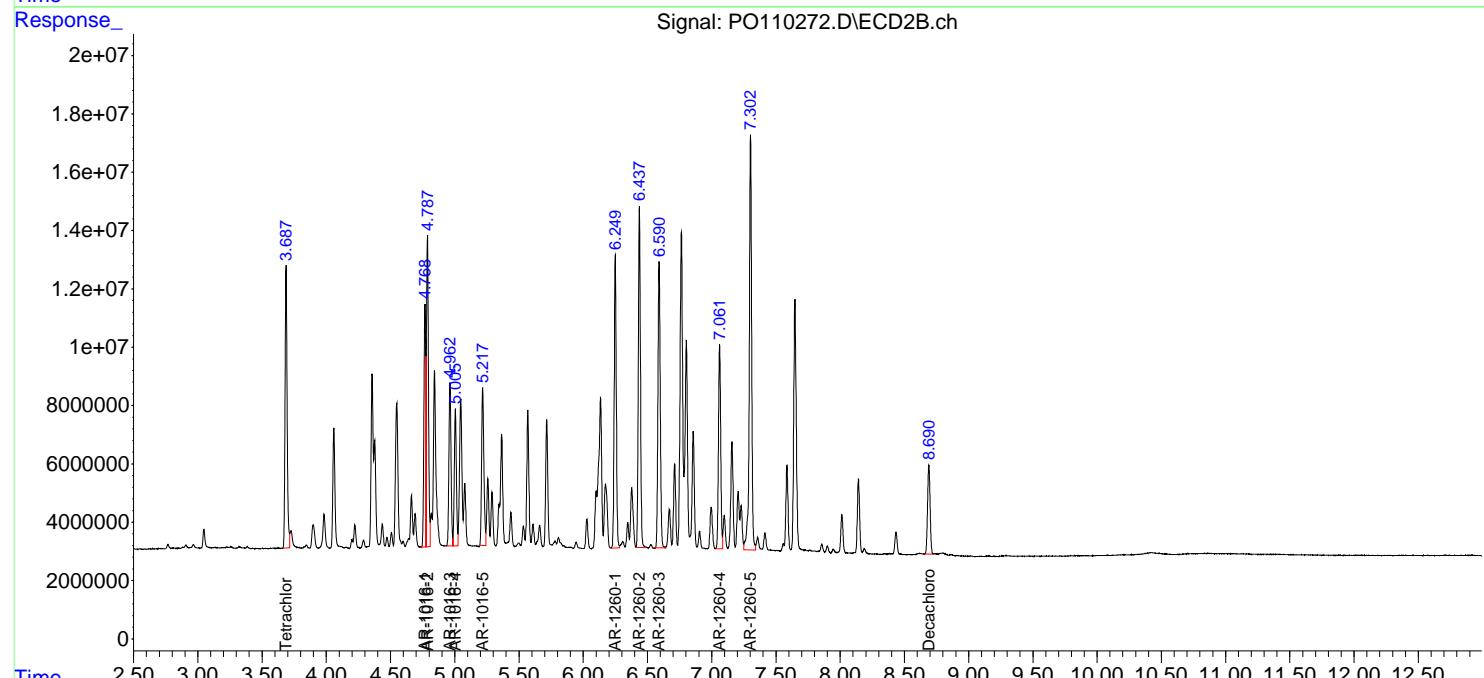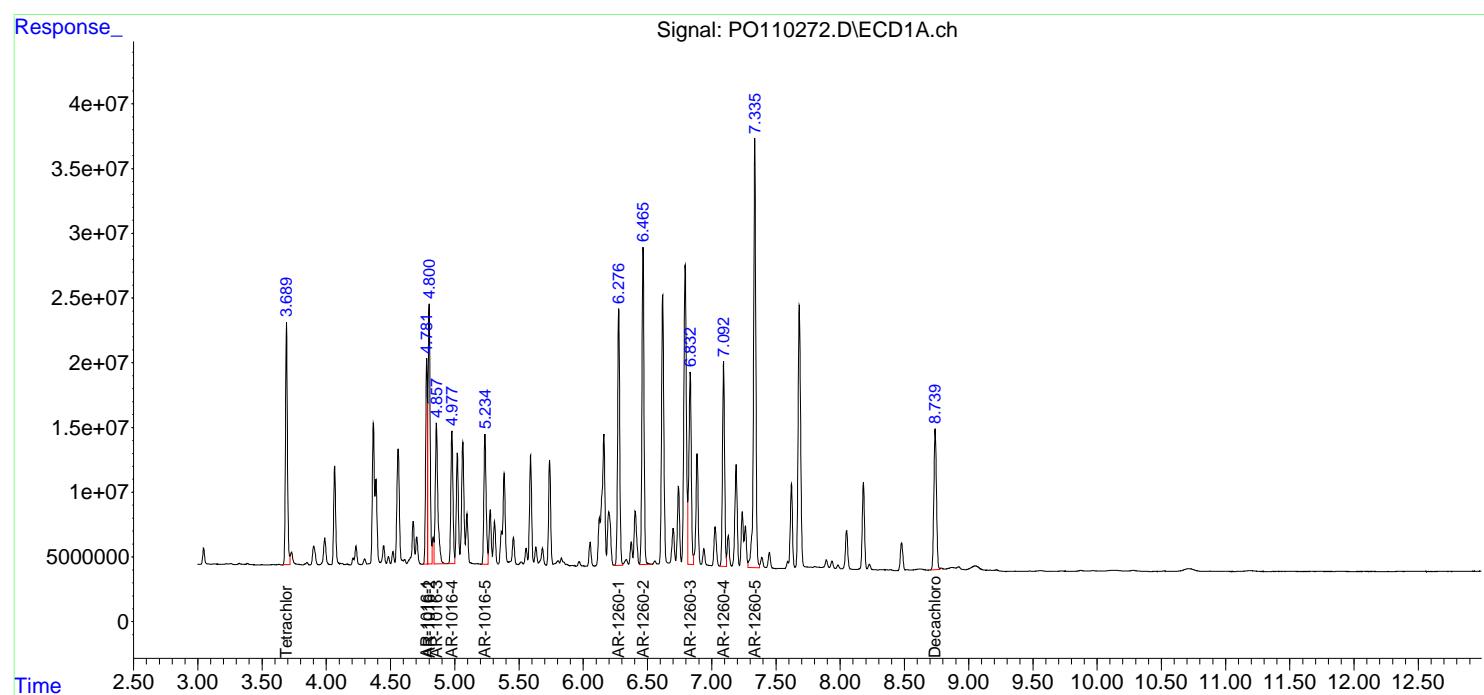

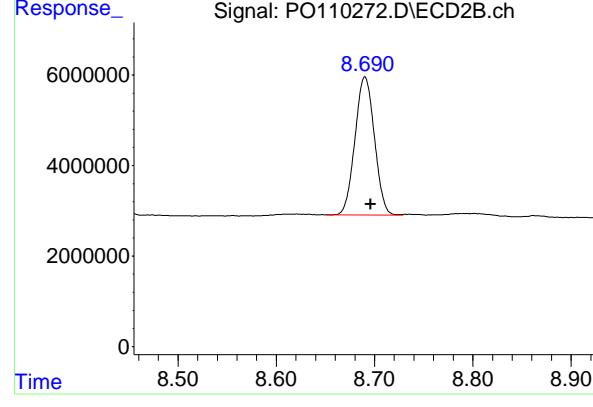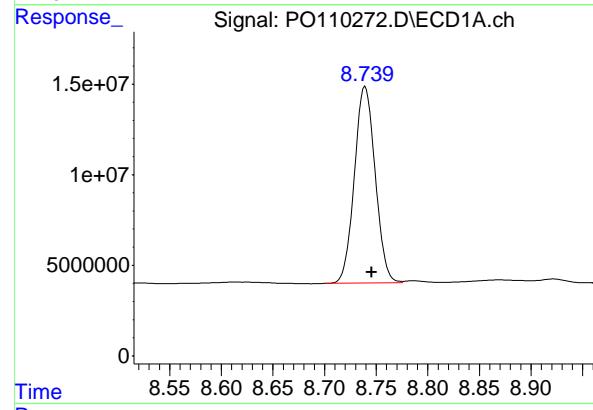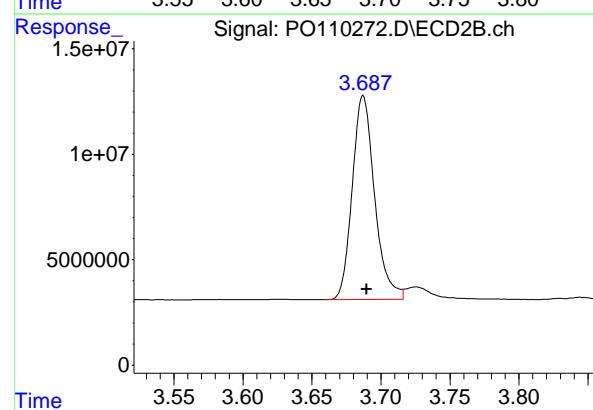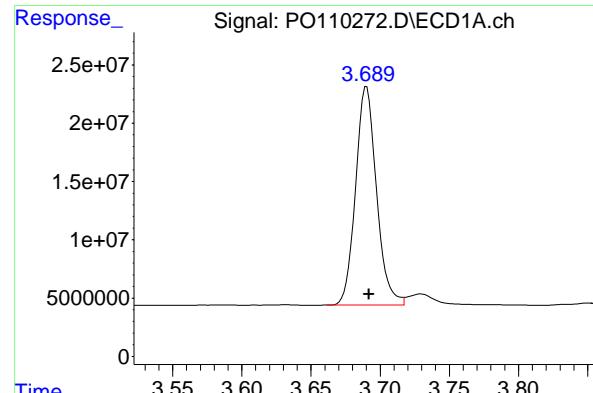

## #1 Tetrachloro-m-xylene

R.T.: 3.690 min  
 Delta R.T.: -0.002 min  
 Response: 196895453 ECD\_O  
 Conc: 21.63 ng/ml ClientSampleId : OU4-VSL-16-040325MSD

## #1 Tetrachloro-m-xylene





R.T.: 3.687 min  
 Delta R.T.: -0.003 min  
 Response: 109050960 ECD\_O  
 Conc: 20.79 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.739 min  
 Delta R.T.: -0.006 min  
 Response: 152232950 ECD\_O  
 Conc: 19.80 ng/ml

## #2 Decachlorobiphenyl

R.T.: 8.690 min  
 Delta R.T.: -0.006 min  
 Response: 41848584 ECD\_O  
 Conc: 17.25 ng/ml

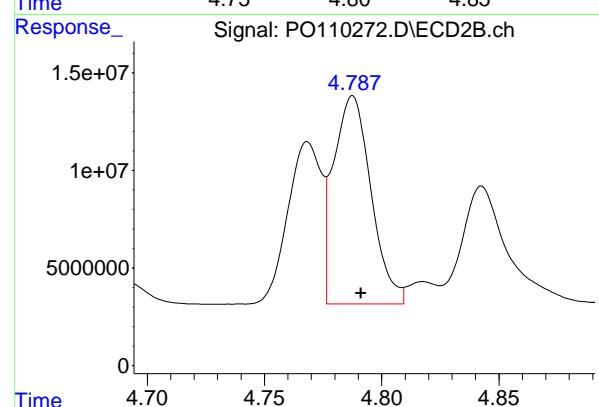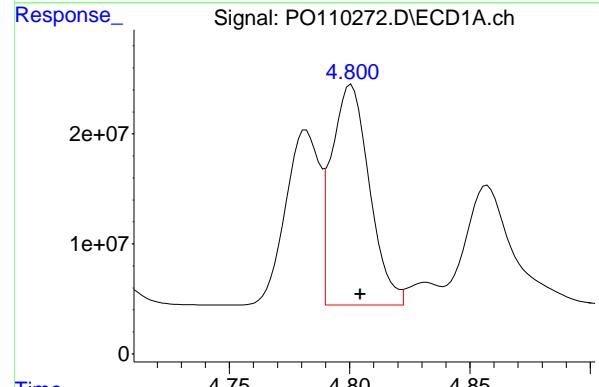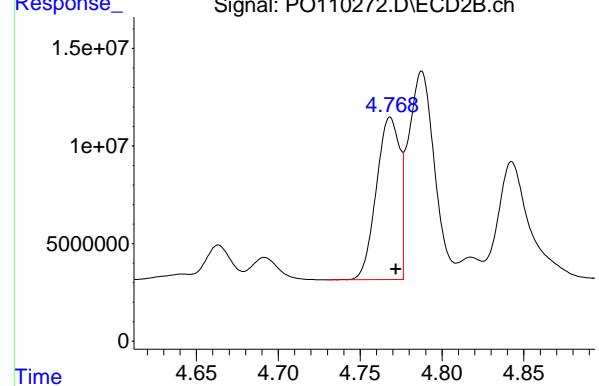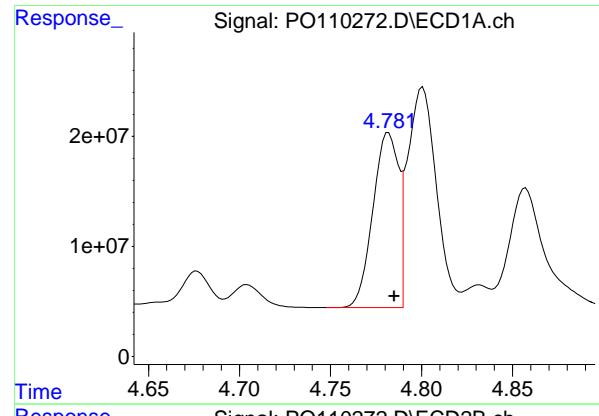

#3 AR-1016-1

R.T.: 4.782 min  
 Delta R.T.: -0.003 min  
 Instrument: ECD\_O  
 Response: 156082810  
 Conc: 463.78 ng/ml  
 ClientSampleId: OU4-VSL-16-040325MSD

#3 AR-1016-1





R.T.: 4.768 min  
 Delta R.T.: -0.004 min  
 Response: 82580554  
 Conc: 450.63 ng/ml

#4 AR-1016-2

R.T.: 4.801 min  
 Delta R.T.: -0.004 min  
 Response: 219302002  
 Conc: 472.95 ng/ml

#4 AR-1016-2

R.T.: 4.788 min  
 Delta R.T.: -0.004 min  
 Response: 118838816  
 Conc: 454.44 ng/ml

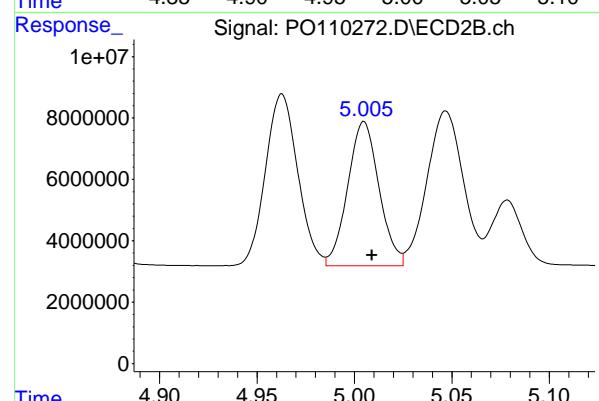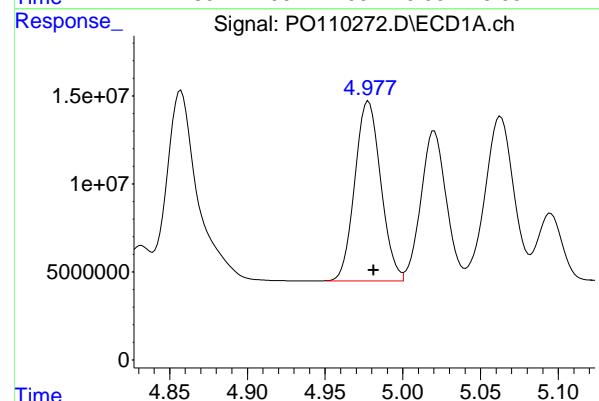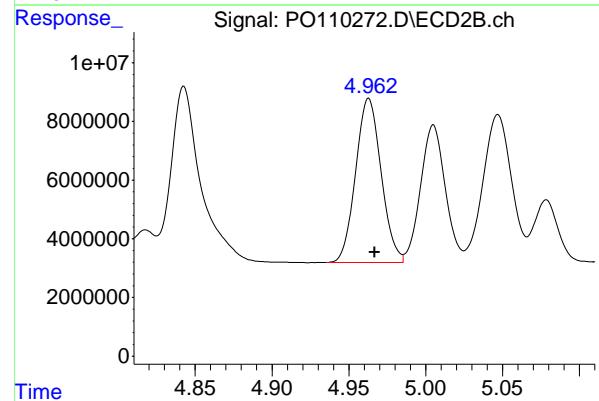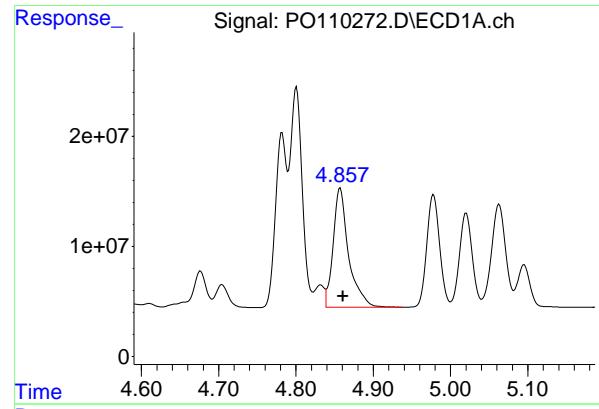

#5 AR-1016-3

R.T.: 4.857 min  
 Delta R.T.: -0.004 min  
 Response: 151860738 ECD\_O  
 Conc: 473.70 ng/ml ClientSampleId : OU4-VSL-16-040325MSD

#5 AR-1016-3


R.T.: 4.963 min  
 Delta R.T.: -0.004 min  
 Response: 64490825  
 Conc: 454.87 ng/ml

#6 AR-1016-4

R.T.: 4.978 min  
 Delta R.T.: -0.004 min  
 Response: 118784963  
 Conc: 470.08 ng/ml

#6 AR-1016-4

R.T.: 5.005 min  
 Delta R.T.: -0.004 min  
 Response: 52631687  
 Conc: 446.30 ng/ml

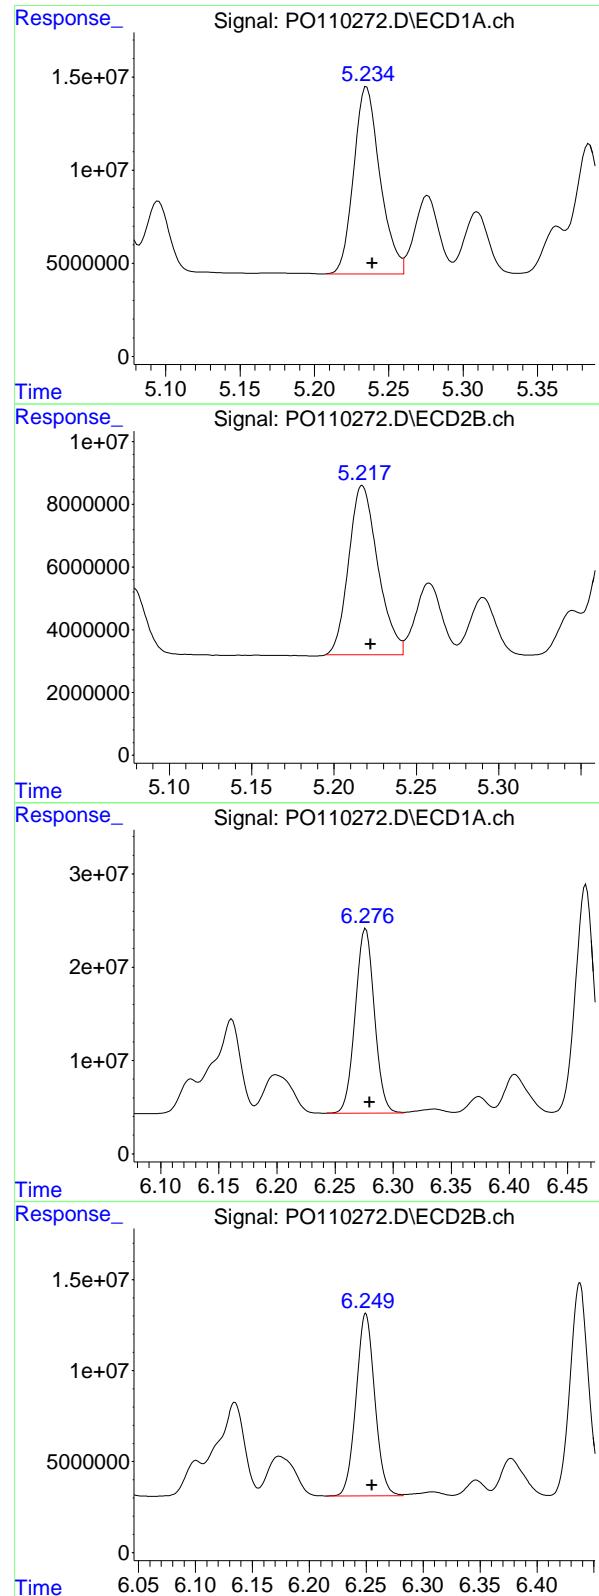

#7 AR-1016-5

R.T.: 5.235 min  
 Delta R.T.: -0.004 min  
 Instrument: ECD\_O  
 Response: 123872515  
 Conc: 450.66 ng/ml  
 ClientSampleId: OU4-VSL-16-040325MSD

#7 AR-1016-5


R.T.: 5.217 min  
 Delta R.T.: -0.005 min  
 Response: 66656091  
 Conc: 435.89 ng/ml

#31 AR-1260-1

R.T.: 6.276 min  
 Delta R.T.: -0.003 min  
 Response: 225949528  
 Conc: 479.37 ng/ml

#31 AR-1260-1

R.T.: 6.250 min  
 Delta R.T.: -0.005 min  
 Response: 115256374  
 Conc: 451.20 ng/ml

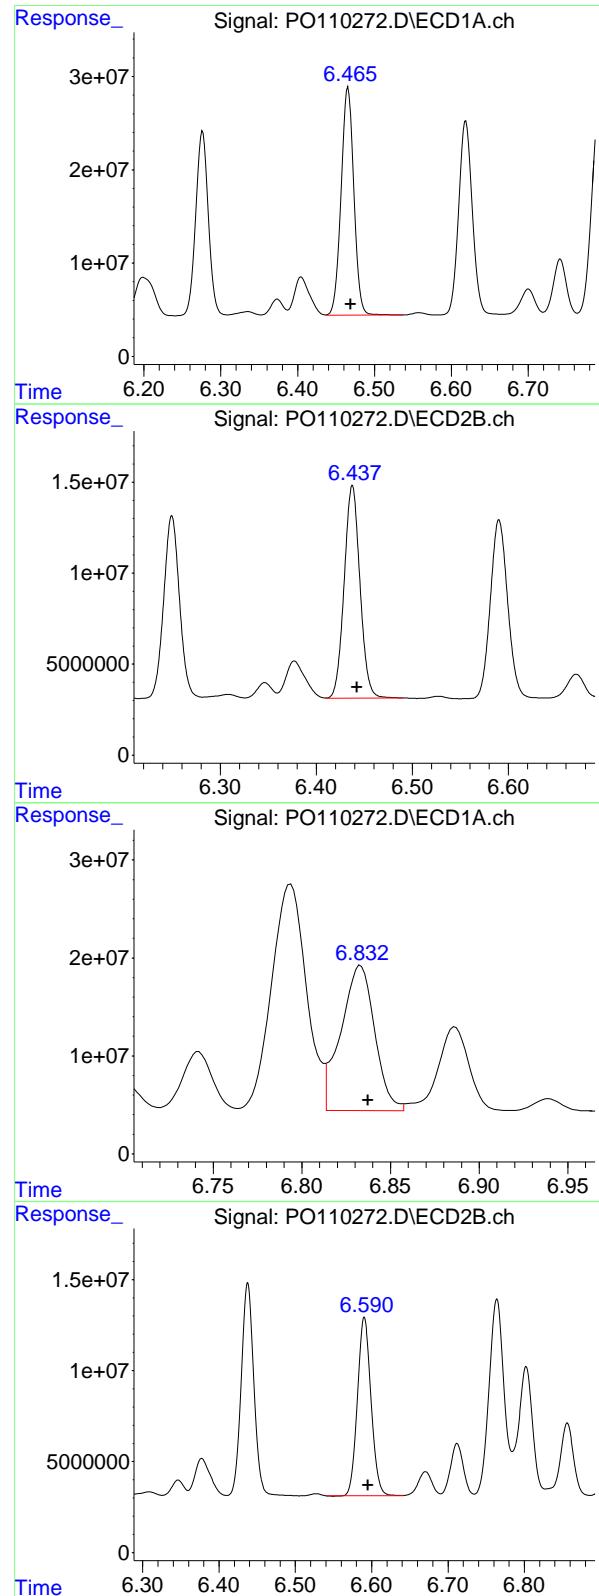

#32 AR-1260-2

R.T.: 6.466 min  
 Delta R.T.: -0.003 min  
 Response: 276063046 ECD\_O  
 Conc: 463.57 ng/ml ClientSampleId : OU4-VSL-16-040325MSD

#32 AR-1260-2



R.T.: 6.438 min  
 Delta R.T.: -0.005 min  
 Response: 132503405  
 Conc: 441.26 ng/ml

#33 AR-1260-3

R.T.: 6.833 min  
 Delta R.T.: -0.004 min  
 Response: 196452347  
 Conc: 404.80 ng/ml

#33 AR-1260-3

R.T.: 6.590 min  
 Delta R.T.: -0.005 min  
 Response: 122855008  
 Conc: 425.13 ng/ml

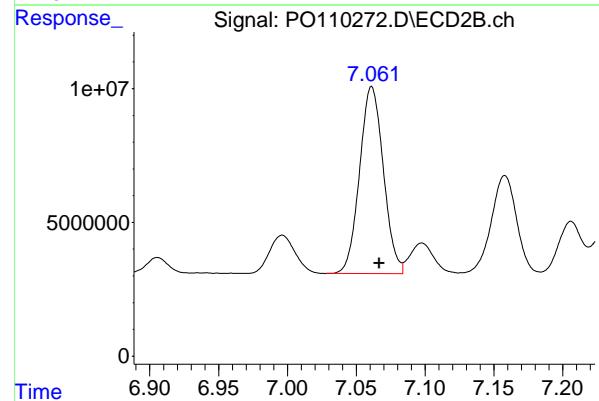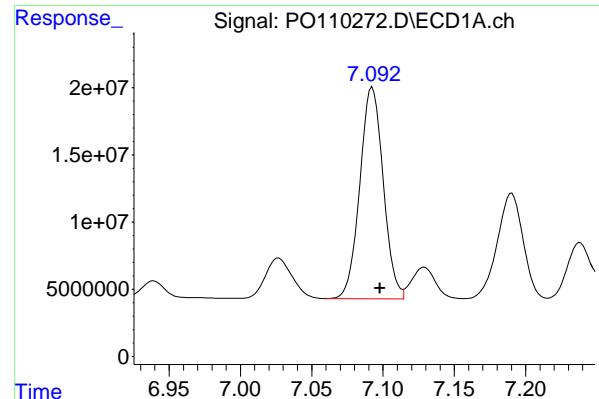

#34 AR-1260-4

R.T.: 7.093 min  
 Delta R.T.: -0.005 min  
 Response: 180248679  
 Conc: 424.95 ng/ml

Instrument: ECD\_O  
 ClientSampleId: OU4-VSL-16-040325MSD

#34 AR-1260-4

R.T.: 7.061 min  
 Delta R.T.: -0.006 min  
 Response: 84267581  
 Conc: 391.80 ng/ml

#35 AR-1260-5

R.T.: 7.335 min  
 Delta R.T.: -0.004 min  
 Response: 409913112  
 Conc: 391.94 ng/ml

#35 AR-1260-5

R.T.: 7.302 min  
 Delta R.T.: -0.005 min  
 Response: 182827616  
 Conc: 366.61 ng/ml

### Manual Integration Report

Sequence:	PO031925	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC750	PO109973.D	AR-1260-5 #2	yogesh	3/19/2025 8:01:07 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1660ICC050	PO109976.D	AR-1260-1	yogesh	3/19/2025 8:01:25 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1660ICC050	PO109976.D	AR-1260-1 #2	yogesh	3/19/2025 8:01:25 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1660ICC050	PO109976.D	AR-1260-3 #2	yogesh	3/19/2025 8:01:25 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	AR-1242-3 #2	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	AR-1242-4	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	AR-1242-5	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	AR-1242-5 #2	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	Tetrachloro-m-xylene	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	Tetrachloro-m-xylene #2	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1248ICC050	PO109988.D	AR-1248-3	yogesh	3/19/2025 8:01:10 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1248ICC050	PO109988.D	AR-1248-4 #2	yogesh	3/19/2025 8:01:10 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1254ICC050	PO109993.D	AR-1254-5 #2	yogesh	3/19/2025 8:01:12 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

### Manual Integration Report

Sequence:	PO031925	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1268ICC500	PO109997.D	AR-1268-1	yogesh	3/19/2025 8:01:13 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC250	PO109998.D	AR-1268-1	yogesh	3/19/2025 8:01:15 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC050	PO109999.D	AR-1268-1	yogesh	3/19/2025 8:01:16 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC050	PO109999.D	AR-1268-4	yogesh	3/19/2025 8:01:16 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC050	PO109999.D	Tetrachloro-m-xylene	yogesh	3/19/2025 8:01:16 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC050	PO109999.D	Tetrachloro-m-xylene #2	yogesh	3/19/2025 8:01:16 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

### Manual Integration Report

Sequence:	PO040725	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO110286.D	AR-1016-5	yogesh	4/8/2025 7:46:34 AM	mohammad	4/9/2025 2:57:57	Peak Integrated by Software
AR1660CCC500	PO110286.D	AR-1016-5 #2	yogesh	4/8/2025 7:46:34 AM	mohammad	4/9/2025 2:57:57	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## Manual Integration Report

Sequence:	PO040825	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254CCC500	PO110295.D	AR-1254-1	yogesh	4/8/2025 2:56:17 PM	mohammad	4/10/2025 5:29:43	Peak Integrated by Software
AR1254CCC500	PO110295.D	AR-1254-2	yogesh	4/8/2025 2:56:17 PM	mohammad	4/10/2025 5:29:43	Peak Integrated by Software
AR1254CCC500	PO110295.D	AR-1254-4 #2	yogesh	4/8/2025 2:56:17 PM	mohammad	4/10/2025 5:29:43	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

### Manual Integration Report

Sequence:	PP032725	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC250	PP070920.D	AR-1260-3	yogesh	3/28/2025 7:37:36 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1660ICC250	PP070920.D	AR-1260-4	yogesh	3/28/2025 7:37:36 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1660ICC250	PP070920.D	AR-1260-5	yogesh	3/28/2025 7:37:36 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1660ICC050	PP070921.D	AR-1016-5	yogesh	3/28/2025 7:37:38 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1660ICC050	PP070921.D	AR-1260-1	yogesh	3/28/2025 7:37:38 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1660ICC050	PP070921.D	AR-1260-3	yogesh	3/28/2025 7:37:38 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1660ICC050	PP070921.D	AR-1260-4	yogesh	3/28/2025 7:37:38 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1660ICC050	PP070921.D	AR-1260-5	yogesh	3/28/2025 7:37:38 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1232ICC500	PP070923.D	Decachlorobiphenyl	yogesh	3/28/2025 7:37:40 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1242ICC050	PP070928.D	AR-1242-1	yogesh	3/28/2025 7:37:42 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1242ICC050	PP070928.D	AR-1242-2	yogesh	3/28/2025 7:37:42 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1242ICC050	PP070928.D	AR-1242-2 #2	yogesh	3/28/2025 7:37:42 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1242ICC050	PP070928.D	AR-1242-3	yogesh	3/28/2025 7:37:42 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

### Manual Integration Report

Sequence:	PP032725	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1242ICC050	PP070928.D	AR-1242-4	yogesh	3/28/2025 7:37:42 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1242ICC050	PP070928.D	AR-1242-4 #2	yogesh	3/28/2025 7:37:42 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1242ICC050	PP070928.D	AR-1242-5	yogesh	3/28/2025 7:37:42 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1242ICC050	PP070928.D	AR-1242-5 #2	yogesh	3/28/2025 7:37:42 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1248ICC050	PP070933.D	AR-1248-2	yogesh	3/28/2025 7:37:44 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1248ICC050	PP070933.D	AR-1248-3	yogesh	3/28/2025 7:37:44 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1248ICC050	PP070933.D	AR-1248-4	yogesh	3/28/2025 7:37:44 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1248ICC050	PP070933.D	AR-1248-5	yogesh	3/28/2025 7:37:44 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1254ICC100	PP070934.D	AR-1254-5	yogesh	3/28/2025 7:37:45 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1254ICC750	PP070935.D	AR-1254-5	yogesh	3/28/2025 7:37:47 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1254ICC250	PP070937.D	AR-1254-5	yogesh	3/28/2025 7:37:48 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1268ICC100	PP070940.D	AR-1268-1 #2	yogesh	3/28/2025 7:37:50 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1268ICC750	PP070941.D	AR-1268-1 #2	yogesh	3/28/2025 7:37:51 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

### Manual Integration Report

Sequence:	PP032725	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1268ICC500	PP070942.D	AR-1268-1 #2	yogesh	3/28/2025 7:37:53 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1268ICC250	PP070943.D	AR-1268-1 #2	yogesh	3/28/2025 7:37:55 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1268ICC050	PP070944.D	AR-1268-1 #2	yogesh	3/28/2025 7:37:56 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1268ICC050	PP070944.D	AR-1268-4 #2	yogesh	3/28/2025 7:37:56 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1268ICC050	PP070944.D	Tetrachloro-m-xylene	yogesh	3/28/2025 7:37:56 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software
AR1254ICV500	PP070948.D	AR-1254-5	yogesh	3/28/2025 7:37:58 AM	mohammad	3/31/2025 1:17:13	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

**Manual Integration Report**

Sequence:	PP040825	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PP071136.D	AR-1260-4	yogesh	4/9/2025 9:18:11 AM	mohammad	4/10/2025 5:29:57	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Instrument ID: ECD\_O

**Daily Analysis Runlog For Sequence/QCBatch ID # PO031925**

Review By	yogesh	Review On	3/18/2025 3:19:21 PM
Supervise By	mohammad	Supervise On	3/24/2025 3:02:46 AM
SubDirectory	PO031925	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschck  Initial Calibration Stds  CCC  Internal Standard/PEM ICV/I.BLK  Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369  PP24332,PP24347,PP24352,PP24357  PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO109970.D	18 Mar 2025 13:26	YP/AJ	Ok
2	I.BLK	PO109971.D	18 Mar 2025 13:44	YP/AJ	Ok
3	AR1660ICC1000	PO109972.D	18 Mar 2025 14:03	YP/AJ	Ok
4	AR1660ICC750	PO109973.D	18 Mar 2025 14:21	YP/AJ	Ok,M
5	AR1660ICC500	PO109974.D	18 Mar 2025 14:39	YP/AJ	Ok
6	AR1660ICC250	PO109975.D	18 Mar 2025 14:58	YP/AJ	Ok
7	AR1660ICC050	PO109976.D	18 Mar 2025 15:16	YP/AJ	Ok,M
8	AR1221ICC500	PO109977.D	18 Mar 2025 15:34	YP/AJ	Ok
9	AR1232ICC500	PO109978.D	18 Mar 2025 15:53	YP/AJ	Ok
10	AR1242ICC1000	PO109979.D	18 Mar 2025 16:11	YP/AJ	Ok
11	AR1242ICC750	PO109980.D	18 Mar 2025 16:30	YP/AJ	Ok
12	AR1242ICC500	PO109981.D	18 Mar 2025 16:48	YP/AJ	Ok
13	AR1242ICC250	PO109982.D	18 Mar 2025 17:06	YP/AJ	Ok
14	AR1242ICC050	PO109983.D	18 Mar 2025 17:25	YP/AJ	Ok,M
15	AR1248ICC1000	PO109984.D	18 Mar 2025 17:42	YP/AJ	Ok
16	AR1248ICC750	PO109985.D	18 Mar 2025 18:00	YP/AJ	Ok
17	AR1248ICC500	PO109986.D	18 Mar 2025 18:19	YP/AJ	Ok
18	AR1248ICC250	PO109987.D	18 Mar 2025 18:37	YP/AJ	Ok
19	AR1248ICC050	PO109988.D	18 Mar 2025 18:54	YP/AJ	Ok,M
20	AR1254ICC1000	PO109989.D	18 Mar 2025 19:13	YP/AJ	Ok
21	AR1254ICC750	PO109990.D	18 Mar 2025 19:31	YP/AJ	Ok

Instrument ID: ECD\_O

**Daily Analysis Runlog For Sequence/QCBatch ID # PO031925**

Review By	yogesh	Review On	3/18/2025 3:19:21 PM		
Supervise By	mohammad	Supervise On	3/24/2025 3:02:46 AM		
SubDirectory	PO031925	HP Acquire Method		HP Processing Method	PO031925
STD. NAME	STD REF.#				
Tune/Reschk					
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369				
CCC	PP24332,PP24347,PP24352,PP24357				
Internal Standard/PEM					
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2				
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

22	AR1254ICC500	PO109991.D	18 Mar 2025 19:49	YP/AJ	Ok
23	AR1254ICC250	PO109992.D	18 Mar 2025 20:07	YP/AJ	Ok
24	AR1254ICC050	PO109993.D	18 Mar 2025 20:25	YP/AJ	Ok,M
25	AR1262ICC500	PO109994.D	18 Mar 2025 20:43	YP/AJ	Ok
26	AR1268ICC1000	PO109995.D	18 Mar 2025 21:02	YP/AJ	Ok
27	AR1268ICC750	PO109996.D	18 Mar 2025 21:20	YP/AJ	Ok
28	AR1268ICC500	PO109997.D	18 Mar 2025 21:39	YP/AJ	Ok,M
29	AR1268ICC250	PO109998.D	18 Mar 2025 21:57	YP/AJ	Ok,M
30	AR1268ICC050	PO109999.D	18 Mar 2025 22:15	YP/AJ	Ok,M
31	PO031925ICV500	PO110000.D	18 Mar 2025 22:34	YP/AJ	Ok
32	AR1242ICV500	PO110001.D	18 Mar 2025 23:47	YP/AJ	Ok
33	AR1248ICV500	PO110002.D	19 Mar 2025 00:05	YP/AJ	Ok
34	AR1254ICV500	PO110003.D	19 Mar 2025 00:24	YP/AJ	Ok
35	AR1268ICV500	PO110004.D	19 Mar 2025 00:42	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD\_O

**Daily Analysis Runlog For Sequence/QCBatch ID # PO040725**

Review By	yogesh	Review On	4/7/2025 11:16:09 AM
Supervise By	mohammad	Supervise On	4/9/2025 2:57:57 AM
SubDirectory	PO040725	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO110262.D	07 Apr 2025 09:08	YP/AJ	Ok
2	AR1660CCC500	PO110263.D	07 Apr 2025 09:46	YP/AJ	Ok
3	AR1242CCC500	PO110264.D	07 Apr 2025 10:05	YP/AJ	Ok
4	AR1248CCC500	PO110265.D	07 Apr 2025 10:23	YP/AJ	Ok
5	AR1254CCC500	PO110266.D	07 Apr 2025 11:18	YP/AJ	Ok
6	I.BLK	PO110267.D	07 Apr 2025 11:36	YP/AJ	Ok
7	Q1723-04DL	PO110268.D	07 Apr 2025 12:14	YP/AJ	Ok
8	Q1730-01	PO110269.D	07 Apr 2025 13:38	YP/AJ	Ok
9	Q1730-03	PO110270.D	07 Apr 2025 13:56	YP/AJ	Ok
10	Q1730-03MS	PO110271.D	07 Apr 2025 14:15	YP/AJ	Ok
11	Q1730-03MSD	PO110272.D	07 Apr 2025 14:33	YP/AJ	Ok
12	Q1736-01	PO110273.D	07 Apr 2025 14:51	YP/AJ	Ok
13	Q1736-02	PO110274.D	07 Apr 2025 15:10	YP/AJ	Ok
14	Q1737-01	PO110275.D	07 Apr 2025 15:28	YP/AJ	Ok,M
15	Q1733-01	PO110276.D	07 Apr 2025 15:47	YP/AJ	Ok,M
16	Q1735-01	PO110277.D	07 Apr 2025 16:05	YP/AJ	Ok
17	AR1660CCC500	PO110278.D	07 Apr 2025 17:14	YP/AJ	Ok
18	AR1242CCC500	PO110279.D	07 Apr 2025 18:09	YP/AJ	Ok
19	AR1248CCC500	PO110280.D	07 Apr 2025 18:27	YP/AJ	Ok
20	AR1254CCC500	PO110281.D	07 Apr 2025 18:45	YP/AJ	Ok
21	I.BLK	PO110282.D	07 Apr 2025 19:04	YP/AJ	Ok

Instrument ID: ECD\_O

**Daily Analysis Runlog For Sequence/QCBatch ID # PO040725**

Review By	yogesh	Review On	4/7/2025 11:16:09 AM		
Supervise By	mohammad	Supervise On	4/9/2025 2:57:57 AM		
SubDirectory	PO040725	HP Acquire Method		HP Processing Method	PO031925
STD. NAME	STD REF.#				
Tune/Reschk Initial Calibration Stds  CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369  PP24332,PP24347,PP24352,PP24357  PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2				

22	PB167469BL	PO110283.D	07 Apr 2025 19:22	YP/AJ	Ok
23	PB167469BS	PO110284.D	07 Apr 2025 19:41	YP/AJ	Ok
24	Q1738-01	PO110285.D	07 Apr 2025 19:59	YP/AJ	Ok
25	AR1660CCC500	PO110286.D	07 Apr 2025 21:27	YP/AJ	Ok,M
26	AR1242CCC500	PO110287.D	07 Apr 2025 22:22	YP/AJ	Ok
27	AR1248CCC500	PO110288.D	07 Apr 2025 22:40	YP/AJ	Ok
28	AR1254CCC500	PO110289.D	07 Apr 2025 22:59	YP/AJ	Ok
29	I.BLK	PO110290.D	07 Apr 2025 23:17	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD\_O

**Daily Analysis Runlog For Sequence/QCBatch ID # PO040825**

Review By	yogesh	Review On	4/8/2025 10:42:21 AM
Supervise By	mohammad	Supervise On	4/10/2025 5:29:43 AM
SubDirectory	PO040825	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO110291.D	08 Apr 2025 08:31	YP/AJ	Ok
2	AR1660CCC500	PO110292.D	08 Apr 2025 09:08	YP/AJ	Ok
3	AR1242CCC500	PO110293.D	08 Apr 2025 09:27	YP/AJ	Ok
4	AR1248CCC500	PO110294.D	08 Apr 2025 09:45	YP/AJ	Ok
5	AR1254CCC500	PO110295.D	08 Apr 2025 10:04	YP/AJ	Ok,M
6	I.BLK	PO110296.D	08 Apr 2025 10:21	YP/AJ	Ok
7	Q1730-05	PO110297.D	08 Apr 2025 10:39	YP/AJ	Ok
8	Q1730-07	PO110298.D	08 Apr 2025 10:58	YP/AJ	Ok
9	Q1730-09	PO110299.D	08 Apr 2025 11:16	YP/AJ	Ok
10	Q1730-11	PO110300.D	08 Apr 2025 11:35	YP/AJ	Ok
11	Q1730-13	PO110301.D	08 Apr 2025 11:53	YP/AJ	Ok
12	AR1660CCC500	PO110302.D	08 Apr 2025 12:58	YP/AJ	Ok
13	AR1242CCC500	PO110303.D	08 Apr 2025 13:17	YP/AJ	Ok
14	AR1248CCC500	PO110304.D	08 Apr 2025 13:35	YP/AJ	Ok
15	AR1254CCC500	PO110305.D	08 Apr 2025 13:53	YP/AJ	Ok
16	I.BLK	PO110306.D	08 Apr 2025 14:12	YP/AJ	Ok
17	PB167515BL	PO110307.D	08 Apr 2025 14:30	YP/AJ	Ok
18	PB167515BS	PO110308.D	08 Apr 2025 14:49	YP/AJ	Ok
19	PB167515BSD	PO110309.D	08 Apr 2025 15:07	YP/AJ	Ok
20	Q1735-04	PO110310.D	08 Apr 2025 15:25	YP/AJ	Ok
21	Q1746-05	PO110311.D	08 Apr 2025 15:44	YP/AJ	Ok

Instrument ID: ECD\_O

**Daily Analysis Runlog For Sequence/QCBatch ID # PO040825**

Review By	yogesh	Review On	4/8/2025 10:42:21 AM
Supervise By	mohammad	Supervise On	4/10/2025 5:29:43 AM
SubDirectory	PO040825	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds  CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369  PP24332,PP24347,PP24352,PP24357  PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		

22	Q1746-06	PO110312.D	08 Apr 2025 16:02	YP/AJ	Ok
23	Q1746-07	PO110313.D	08 Apr 2025 16:20	YP/AJ	Ok
24	Q1739-01	PO110314.D	08 Apr 2025 16:39	YP/AJ	Ok,M
25	AR1660CCC500	PO110315.D	08 Apr 2025 17:54	YP/AJ	Ok
26	AR1242CCC500	PO110316.D	08 Apr 2025 18:49	YP/AJ	Ok
27	AR1248CCC500	PO110317.D	08 Apr 2025 19:08	YP/AJ	Ok
28	AR1254CCC500	PO110318.D	08 Apr 2025 19:25	YP/AJ	Ok
29	I.BLK	PO110319.D	08 Apr 2025 19:43	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD\_P

**Daily Analysis Runlog For Sequence/QCBatch ID # PP032725**

Review By	yogesh	Review On	3/27/2025 12:19:10 PM
Supervise By	mohammad	Supervise On	3/31/2025 1:17:13 AM
SubDirectory	PP032725	HP Acquire Method	HP Processing Method      PP032725
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PP070915.D	27 Mar 2025 09:58	YP\AJ	Ok
2	I.BLK	PP070916.D	27 Mar 2025 10:14	YP\AJ	Ok
3	AR1660ICC1000	PP070917.D	27 Mar 2025 10:30	YP\AJ	Ok
4	AR1660ICC750	PP070918.D	27 Mar 2025 10:47	YP\AJ	Ok
5	AR1660ICC500	PP070919.D	27 Mar 2025 11:03	YP\AJ	Ok
6	AR1660ICC250	PP070920.D	27 Mar 2025 11:19	YP\AJ	Ok,M
7	AR1660ICC050	PP070921.D	27 Mar 2025 11:35	YP\AJ	Ok,M
8	AR1221ICC500	PP070922.D	27 Mar 2025 11:52	YP\AJ	Ok
9	AR1232ICC500	PP070923.D	27 Mar 2025 12:11	YP\AJ	Ok,M
10	AR1242ICC1000	PP070924.D	27 Mar 2025 12:28	YP\AJ	Ok
11	AR1242ICC750	PP070925.D	27 Mar 2025 12:44	YP\AJ	Ok
12	AR1242ICC500	PP070926.D	27 Mar 2025 13:00	YP\AJ	Ok
13	AR1242ICC250	PP070927.D	27 Mar 2025 13:16	YP\AJ	Ok
14	AR1242ICC050	PP070928.D	27 Mar 2025 13:33	YP\AJ	Ok,M
15	AR1248ICC1000	PP070929.D	27 Mar 2025 13:49	YP\AJ	Ok
16	AR1248ICC750	PP070930.D	27 Mar 2025 14:05	YP\AJ	Ok
17	AR1248ICC500	PP070931.D	27 Mar 2025 14:22	YP\AJ	Ok
18	AR1248ICC250	PP070932.D	27 Mar 2025 14:38	YP\AJ	Ok
19	AR1248ICC050	PP070933.D	27 Mar 2025 14:55	YP\AJ	Ok,M
20	AR1254ICC1000	PP070934.D	27 Mar 2025 15:11	YP\AJ	Ok,M
21	AR1254ICC750	PP070935.D	27 Mar 2025 15:27	YP\AJ	Ok,M

Instrument ID: ECD\_P

**Daily Analysis Runlog For Sequence/QCBatch ID # PP032725**

Review By	yogesh	Review On	3/27/2025 12:19:10 PM		
Supervise By	mohammad	Supervise On	3/31/2025 1:17:13 AM		
SubDirectory	PP032725	HP Acquire Method		HP Processing Method	PP032725
STD. NAME	STD REF.#				
Tune/Reschk					
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369				
CCC	PP24332,PP24347,PP24352,PP24357				
Internal Standard/PEM					
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2				
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

22	AR1254ICC500	PP070936.D	27 Mar 2025 15:43	YP\AJ	Ok
23	AR1254ICC250	PP070937.D	27 Mar 2025 16:00	YP\AJ	Ok,M
24	AR1254ICC050	PP070938.D	27 Mar 2025 16:16	YP\AJ	Ok
25	AR1262ICC500	PP070939.D	27 Mar 2025 16:32	YP\AJ	Ok
26	AR1268ICC1000	PP070940.D	27 Mar 2025 16:48	YP\AJ	Ok,M
27	AR1268ICC750	PP070941.D	27 Mar 2025 17:05	YP\AJ	Ok,M
28	AR1268ICC500	PP070942.D	27 Mar 2025 17:21	YP\AJ	Ok,M
29	AR1268ICC250	PP070943.D	27 Mar 2025 17:37	YP\AJ	Ok,M
30	AR1268ICC050	PP070944.D	27 Mar 2025 17:53	YP\AJ	Ok,M
31	PP032725ICV500	PP070945.D	27 Mar 2025 18:26	YP\AJ	Ok
32	AR1242ICV500	PP070946.D	27 Mar 2025 18:42	YP\AJ	Ok
33	AR1248ICV500	PP070947.D	27 Mar 2025 19:15	YP\AJ	Ok
34	AR1254ICV500	PP070948.D	27 Mar 2025 19:47	YP\AJ	Ok,M
35	AR1268ICV500	PP070949.D	27 Mar 2025 20:20	YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD\_P

**Daily Analysis Runlog For Sequence/QCBatch ID # PP040825**

Review By	yogesh	Review On	4/8/2025 3:06:55 PM
Supervise By	mohammad	Supervise On	4/10/2025 5:29:57 AM
SubDirectory	PP040825	HP Acquire Method	HP Processing Method      PP032725
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds  CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PP071135.D	08 Apr 2025 08:39	YP\AJ	Ok
2	AR1660CCC500	PP071136.D	08 Apr 2025 09:37	YP\AJ	Ok,M
3	AR1242CCC500	PP071137.D	08 Apr 2025 09:56	YP\AJ	Ok
4	AR1248CCC500	PP071138.D	08 Apr 2025 10:33	YP\AJ	Ok
5	AR1254CCC500	PP071139.D	08 Apr 2025 10:49	YP\AJ	Ok
6	I.BLK	PP071140.D	08 Apr 2025 11:05	YP\AJ	Ok
7	PB167469BL	PP071141.D	08 Apr 2025 11:23	YP\AJ	Not Ok
8	Q1730-15	PP071142.D	08 Apr 2025 11:39	YP\AJ	Ok
9	Q1730-17	PP071143.D	08 Apr 2025 11:56	YP\AJ	Ok
10	Q1730-19	PP071144.D	08 Apr 2025 12:12	YP\AJ	Ok
11	Q1740-01	PP071145.D	08 Apr 2025 13:08	YP\AJ	Ok
12	Q1742-01	PP071146.D	08 Apr 2025 13:25	YP\AJ	Ok,M
13	Q1742-01MS	PP071147.D	08 Apr 2025 13:41	YP\AJ	Ok,M
14	Q1742-01MSD	PP071148.D	08 Apr 2025 13:57	YP\AJ	Ok,M
15	Q1743-01	PP071149.D	08 Apr 2025 14:14	YP\AJ	Ok,M
16	Q1744-01	PP071150.D	08 Apr 2025 14:30	YP\AJ	Ok
17	AR1660CCC500	PP071151.D	08 Apr 2025 15:29	YP\AJ	Ok
18	AR1242CCC500	PP071152.D	08 Apr 2025 16:02	YP\AJ	Ok
19	AR1248CCC500	PP071153.D	08 Apr 2025 16:18	YP\AJ	Ok
20	AR1254CCC500	PP071154.D	08 Apr 2025 16:34	YP\AJ	Ok
21	I.BLK	PP071155.D	08 Apr 2025 16:51	YP\AJ	Ok

Instrument ID: ECD\_P

**Daily Analysis Runlog For Sequence/QCBatch ID # PP040825**

Review By	yogesh	Review On	4/8/2025 3:06:55 PM		
Supervise By	mohammad	Supervise On	4/10/2025 5:29:57 AM		
SubDirectory	PP040825	HP Acquire Method		HP Processing Method	PP032725
STD. NAME	STD REF.#				
Tune/Reschk					
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369				
CCC	PP24332,PP24347,PP24352,PP24357				
Internal Standard/PEM					
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2				
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

22	PB167507BL	PP071156.D	08 Apr 2025 17:07	YP\AJ	Ok
23	PB167507BS	PP071157.D	08 Apr 2025 17:23	YP\AJ	Ok
24	Q1744-03	PP071158.D	08 Apr 2025 17:40	YP\AJ	Ok
25	Q1745-01	PP071159.D	08 Apr 2025 17:56	YP\AJ	Ok,M
26	Q1745-09	PP071160.D	08 Apr 2025 18:12	YP\AJ	Ok,M
27	Q1746-01	PP071161.D	08 Apr 2025 18:28	YP\AJ	Ok
28	Q1746-03	PP071162.D	08 Apr 2025 18:45	YP\AJ	Ok
29	Q1747-01	PP071163.D	08 Apr 2025 19:01	YP\AJ	Ok,M
30	AR1660CCC500	PP071164.D	08 Apr 2025 20:28	YP\AJ	Ok
31	AR1242CCC500	PP071165.D	08 Apr 2025 21:17	YP\AJ	Ok
32	AR1248CCC500	PP071166.D	08 Apr 2025 21:33	YP\AJ	Ok
33	AR1254CCC500	PP071167.D	08 Apr 2025 21:49	YP\AJ	Ok
34	I.BLK	PP071168.D	08 Apr 2025 22:05	YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD\_O

### Daily Analysis Runlog For Sequence/QCBatch ID # PO031925

Review By	yogesh	Review On	3/18/2025 3:19:21 PM	
Supervise By	mohammad	Supervise On	3/24/2025 3:02:46 AM	
SubDirectory	PO031925	HP Acquire Method	HP Processing Method	PO031925
STD. NAME	STD REF.#			
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369			
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24332,PP24347,PP24352,PP24357  PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO109970.D	18 Mar 2025 13:26		YP/AJ	Ok
2	I.BLK	I.BLK	PO109971.D	18 Mar 2025 13:44		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO109972.D	18 Mar 2025 14:03		YP/AJ	Ok
4	AR1660ICC750	AR1660ICC750	PO109973.D	18 Mar 2025 14:21		YP/AJ	Ok,M
5	AR1660ICC500	AR1660ICC500	PO109974.D	18 Mar 2025 14:39		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO109975.D	18 Mar 2025 14:58		YP/AJ	Ok
7	AR1660ICC050	AR1660ICC050	PO109976.D	18 Mar 2025 15:16		YP/AJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PO109977.D	18 Mar 2025 15:34		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO109978.D	18 Mar 2025 15:53		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO109979.D	18 Mar 2025 16:11		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO109980.D	18 Mar 2025 16:30		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO109981.D	18 Mar 2025 16:48		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO109982.D	18 Mar 2025 17:06		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO109983.D	18 Mar 2025 17:25		YP/AJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PO109984.D	18 Mar 2025 17:42		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO109985.D	18 Mar 2025 18:00		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO109986.D	18 Mar 2025 18:19		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO109987.D	18 Mar 2025 18:37		YP/AJ	Ok

Instrument ID: ECD\_O

### Daily Analysis Runlog For Sequence/QCBatch ID # PO031925

Review By	yogesh	Review On	3/18/2025 3:19:21 PM
Supervise By	mohammad	Supervise On	3/24/2025 3:02:46 AM
SubDirectory	PO031925	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1248ICC050	AR1248ICC050	PO109988.D	18 Mar 2025 18:54		YP/AJ	Ok,M
20	AR1254ICC1000	AR1254ICC1000	PO109989.D	18 Mar 2025 19:13		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO109990.D	18 Mar 2025 19:31		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO109991.D	18 Mar 2025 19:49		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO109992.D	18 Mar 2025 20:07		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO109993.D	18 Mar 2025 20:25		YP/AJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PO109994.D	18 Mar 2025 20:43		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO109995.D	18 Mar 2025 21:02		YP/AJ	Ok
27	AR1268ICC750	AR1268ICC750	PO109996.D	18 Mar 2025 21:20		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO109997.D	18 Mar 2025 21:39		YP/AJ	Ok,M
29	AR1268ICC250	AR1268ICC250	PO109998.D	18 Mar 2025 21:57		YP/AJ	Ok,M
30	AR1268ICC050	AR1268ICC050	PO109999.D	18 Mar 2025 22:15		YP/AJ	Ok,M
31	PO031925ICV500	ICVPO031925	PO110000.D	18 Mar 2025 22:34		YP/AJ	Ok
32	AR1242ICV500	ICVPO031925AR1242	PO110001.D	18 Mar 2025 23:47		YP/AJ	Ok
33	AR1248ICV500	ICVPO031925AR1248	PO110002.D	19 Mar 2025 00:05		YP/AJ	Ok
34	AR1254ICV500	ICVPO031925AR1254	PO110003.D	19 Mar 2025 00:24		YP/AJ	Ok
35	AR1268ICV500	ICVPO031925AR1268	PO110004.D	19 Mar 2025 00:42		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD\_O

### Daily Analysis Runlog For Sequence/QCBatch ID # PO040725

Review By	yogesh	Review On	4/7/2025 11:16:09 AM	
Supervise By	mohammad	Supervise On	4/9/2025 2:57:57 AM	
SubDirectory	PO040725	HP Acquire Method	HP Processing Method	PO031925
STD. NAME	STD REF.#			
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369			
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24332,PP24347,PP24352,PP24357  PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO110262.D	07 Apr 2025 09:08		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO110263.D	07 Apr 2025 09:46		YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO110264.D	07 Apr 2025 10:05		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO110265.D	07 Apr 2025 10:23		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO110266.D	07 Apr 2025 11:18		YP/AJ	Ok
6	I.BLK	I.BLK	PO110267.D	07 Apr 2025 11:36		YP/AJ	Ok
7	Q1723-04DL	GAS-AUD-25-0037DL	PO110268.D	07 Apr 2025 12:14	AR1254 Hit	YP/AJ	Ok
8	Q1730-01	OU4-VSL-15-040325	PO110269.D	07 Apr 2025 13:38		YP/AJ	Ok
9	Q1730-03	OU4-VSL-16-040325	PO110270.D	07 Apr 2025 13:56		YP/AJ	Ok
10	Q1730-03MS	OU4-VSL-16-040325M	PO110271.D	07 Apr 2025 14:15		YP/AJ	Ok
11	Q1730-03MSD	OU4-VSL-16-040325M	PO110272.D	07 Apr 2025 14:33		YP/AJ	Ok
12	Q1736-01	GST1	PO110273.D	07 Apr 2025 14:51		YP/AJ	Ok
13	Q1736-02	GST2	PO110274.D	07 Apr 2025 15:10		YP/AJ	Ok
14	Q1737-01	RT3069	PO110275.D	07 Apr 2025 15:28	AR1260 hit	YP/AJ	Ok,M
15	Q1733-01	ETGI-328	PO110276.D	07 Apr 2025 15:47		YP/AJ	Ok,M
16	Q1735-01	50660-50661-50662-56	PO110277.D	07 Apr 2025 16:05		YP/AJ	Ok
17	AR1660CCC500	AR1660CCC500	PO110278.D	07 Apr 2025 17:14		YP/AJ	Ok
18	AR1242CCC500	AR1242CCC500	PO110279.D	07 Apr 2025 18:09		YP/AJ	Ok

Instrument ID: ECD\_O

### Daily Analysis Runlog For Sequence/QCBatch ID # PO040725

Review By	yogesh	Review On	4/7/2025 11:16:09 AM
Supervise By	mohammad	Supervise On	4/9/2025 2:57:57 AM
SubDirectory	PO040725	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1248CCC500	AR1248CCC500	PO110280.D	07 Apr 2025 18:27		YP/AJ	Ok
20	AR1254CCC500	AR1254CCC500	PO110281.D	07 Apr 2025 18:45		YP/AJ	Ok
21	I.BLK	I.BLK	PO110282.D	07 Apr 2025 19:04		YP/AJ	Ok
22	PB167469BL	PB167469BL	PO110283.D	07 Apr 2025 19:22		YP/AJ	Ok
23	PB167469BS	PB167469BS	PO110284.D	07 Apr 2025 19:41		YP/AJ	Ok
24	Q1738-01	OK-02-040425	PO110285.D	07 Apr 2025 19:59		YP/AJ	Ok
25	AR1660CCC500	AR1660CCC500	PO110286.D	07 Apr 2025 21:27		YP/AJ	Ok,M
26	AR1242CCC500	AR1242CCC500	PO110287.D	07 Apr 2025 22:22		YP/AJ	Ok
27	AR1248CCC500	AR1248CCC500	PO110288.D	07 Apr 2025 22:40		YP/AJ	Ok
28	AR1254CCC500	AR1254CCC500	PO110289.D	07 Apr 2025 22:59		YP/AJ	Ok
29	I.BLK	I.BLK	PO110290.D	07 Apr 2025 23:17		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD\_O

### Daily Analysis Runlog For Sequence/QCBatch ID # PO040825

Review By	yogesh	Review On	4/8/2025 10:42:21 AM
Supervise By	mohammad	Supervise On	4/10/2025 5:29:43 AM
SubDirectory	PO040825	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO110291.D	08 Apr 2025 08:31		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO110292.D	08 Apr 2025 09:08		YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO110293.D	08 Apr 2025 09:27		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO110294.D	08 Apr 2025 09:45		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO110295.D	08 Apr 2025 10:04		YP/AJ	Ok,M
6	I.BLK	I.BLK	PO110296.D	08 Apr 2025 10:21		YP/AJ	Ok
7	Q1730-05	OU4-VSL-17-040325	PO110297.D	08 Apr 2025 10:39		YP/AJ	Ok
8	Q1730-07	OU4-PCS-TC-21-04032	PO110298.D	08 Apr 2025 10:58		YP/AJ	Ok
9	Q1730-09	OU4-PCS-TC-22-04032	PO110299.D	08 Apr 2025 11:16		YP/AJ	Ok
10	Q1730-11	OU4-PCS-TC-23-04032	PO110300.D	08 Apr 2025 11:35		YP/AJ	Ok
11	Q1730-13	OU4-PCS-TC-24-04032	PO110301.D	08 Apr 2025 11:53		YP/AJ	Ok
12	AR1660CCC500	AR1660CCC500	PO110302.D	08 Apr 2025 12:58		YP/AJ	Ok
13	AR1242CCC500	AR1242CCC500	PO110303.D	08 Apr 2025 13:17		YP/AJ	Ok
14	AR1248CCC500	AR1248CCC500	PO110304.D	08 Apr 2025 13:35		YP/AJ	Ok
15	AR1254CCC500	AR1254CCC500	PO110305.D	08 Apr 2025 13:53		YP/AJ	Ok
16	I.BLK	I.BLK	PO110306.D	08 Apr 2025 14:12		YP/AJ	Ok
17	PB167515BL	PB167515BL	PO110307.D	08 Apr 2025 14:30		YP/AJ	Ok
18	PB167515BS	PB167515BS	PO110308.D	08 Apr 2025 14:49		YP/AJ	Ok

Instrument ID: ECD\_O

### Daily Analysis Runlog For Sequence/QCBatch ID # PO040825

Review By	yogesh	Review On	4/8/2025 10:42:21 AM
Supervise By	mohammad	Supervise On	4/10/2025 5:29:43 AM
SubDirectory	PO040825	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,P P24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP 24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369  PP24332,PP24347,PP24352,PP24357  PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	PB167515BSD	PB167515BSD	PO110309.D	08 Apr 2025 15:07		YP/AJ	Ok
20	Q1735-04	0401-A-0401-B-COMP	PO110310.D	08 Apr 2025 15:25		YP/AJ	Ok
21	Q1746-05	B-158-GW01	PO110311.D	08 Apr 2025 15:44		YP/AJ	Ok
22	Q1746-06	B-149-GW01	PO110312.D	08 Apr 2025 16:02		YP/AJ	Ok
23	Q1746-07	EB-2025-4-7	PO110313.D	08 Apr 2025 16:20		YP/AJ	Ok
24	Q1739-01	WC-LIQUID-20250404	PO110314.D	08 Apr 2025 16:39	AR1254 Hit	YP/AJ	Ok,M
25	AR1660CCC500	AR1660CCC500	PO110315.D	08 Apr 2025 17:54		YP/AJ	Ok
26	AR1242CCC500	AR1242CCC500	PO110316.D	08 Apr 2025 18:49		YP/AJ	Ok
27	AR1248CCC500	AR1248CCC500	PO110317.D	08 Apr 2025 19:08		YP/AJ	Ok
28	AR1254CCC500	AR1254CCC500	PO110318.D	08 Apr 2025 19:25		YP/AJ	Ok
29	I.BLK	I.BLK	PO110319.D	08 Apr 2025 19:43		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD\_P

### Daily Analysis Runlog For Sequence/QCBatch ID # PP032725

Review By	yogesh	Review On	3/27/2025 12:19:10 PM
Supervise By	mohammad	Supervise On	3/31/2025 1:17:13 AM
SubDirectory	PP032725	HP Acquire Method	HP Processing Method PP032725
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24332,PP24347,PP24352,PP24357  PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PP070915.D	27 Mar 2025 09:58		YPAJ	Ok
2	I.BLK	I.BLK	PP070916.D	27 Mar 2025 10:14		YPAJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PP070917.D	27 Mar 2025 10:30		YPAJ	Ok
4	AR1660ICC750	AR1660ICC750	PP070918.D	27 Mar 2025 10:47		YPAJ	Ok
5	AR1660ICC500	AR1660ICC500	PP070919.D	27 Mar 2025 11:03		YPAJ	Ok
6	AR1660ICC250	AR1660ICC250	PP070920.D	27 Mar 2025 11:19		YPAJ	Ok,M
7	AR1660ICC050	AR1660ICC050	PP070921.D	27 Mar 2025 11:35		YPAJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PP070922.D	27 Mar 2025 11:52		YPAJ	Ok
9	AR1232ICC500	AR1232ICC500	PP070923.D	27 Mar 2025 12:11		YPAJ	Ok,M
10	AR1242ICC1000	AR1242ICC1000	PP070924.D	27 Mar 2025 12:28		YPAJ	Ok
11	AR1242ICC750	AR1242ICC750	PP070925.D	27 Mar 2025 12:44		YPAJ	Ok
12	AR1242ICC500	AR1242ICC500	PP070926.D	27 Mar 2025 13:00		YPAJ	Ok
13	AR1242ICC250	AR1242ICC250	PP070927.D	27 Mar 2025 13:16		YPAJ	Ok
14	AR1242ICC050	AR1242ICC050	PP070928.D	27 Mar 2025 13:33		YPAJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PP070929.D	27 Mar 2025 13:49		YPAJ	Ok
16	AR1248ICC750	AR1248ICC750	PP070930.D	27 Mar 2025 14:05		YPAJ	Ok
17	AR1248ICC500	AR1248ICC500	PP070931.D	27 Mar 2025 14:22		YPAJ	Ok
18	AR1248ICC250	AR1248ICC250	PP070932.D	27 Mar 2025 14:38		YPAJ	Ok

Instrument ID: ECD\_P

### Daily Analysis Runlog For Sequence/QCBatch ID # PP032725

Review By	yogesh	Review On	3/27/2025 12:19:10 PM
Supervise By	mohammad	Supervise On	3/31/2025 1:17:13 AM
SubDirectory	PP032725	HP Acquire Method	HP Processing Method
<b>STD. NAME</b>	<b>STD REF.#</b>		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1248ICC050	AR1248ICC050	PP070933.D	27 Mar 2025 14:55		YPAJ	Ok,M
20	AR1254ICC1000	AR1254ICC1000	PP070934.D	27 Mar 2025 15:11		YPAJ	Ok,M
21	AR1254ICC750	AR1254ICC750	PP070935.D	27 Mar 2025 15:27		YPAJ	Ok,M
22	AR1254ICC500	AR1254ICC500	PP070936.D	27 Mar 2025 15:43		YPAJ	Ok
23	AR1254ICC250	AR1254ICC250	PP070937.D	27 Mar 2025 16:00		YPAJ	Ok,M
24	AR1254ICC050	AR1254ICC050	PP070938.D	27 Mar 2025 16:16		YPAJ	Ok
25	AR1262ICC500	AR1262ICC500	PP070939.D	27 Mar 2025 16:32		YPAJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PP070940.D	27 Mar 2025 16:48		YPAJ	Ok,M
27	AR1268ICC750	AR1268ICC750	PP070941.D	27 Mar 2025 17:05		YPAJ	Ok,M
28	AR1268ICC500	AR1268ICC500	PP070942.D	27 Mar 2025 17:21		YPAJ	Ok,M
29	AR1268ICC250	AR1268ICC250	PP070943.D	27 Mar 2025 17:37		YPAJ	Ok,M
30	AR1268ICC050	AR1268ICC050	PP070944.D	27 Mar 2025 17:53		YPAJ	Ok,M
31	PP032725ICV500	ICVPP032725	PP070945.D	27 Mar 2025 18:26		YPAJ	Ok
32	AR1242ICV500	ICVPP032725AR1242	PP070946.D	27 Mar 2025 18:42		YPAJ	Ok
33	AR1248ICV500	ICVPP032725AR1248	PP070947.D	27 Mar 2025 19:15		YPAJ	Ok
34	AR1254ICV500	ICVPP032725AR1254	PP070948.D	27 Mar 2025 19:47		YPAJ	Ok,M
35	AR1268ICV500	ICVPP032725AR1268	PP070949.D	27 Mar 2025 20:20		YPAJ	Ok

M : Manual Integration

Instrument ID: ECD\_P

### Daily Analysis Runlog For Sequence/QCBatch ID # PP040825

Review By	yogesh	Review On	4/8/2025 3:06:55 PM
Supervise By	mohammad	Supervise On	4/10/2025 5:29:57 AM
SubDirectory	PP040825	HP Acquire Method	HP Processing Method PP032725
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24332,PP24347,PP24352,PP24357  PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PP071135.D	08 Apr 2025 08:39		YPAJ	Ok
2	AR1660CCC500	AR1660CCC500	PP071136.D	08 Apr 2025 09:37		YPAJ	Ok,M
3	AR1242CCC500	AR1242CCC500	PP071137.D	08 Apr 2025 09:56		YPAJ	Ok
4	AR1248CCC500	AR1248CCC500	PP071138.D	08 Apr 2025 10:33		YPAJ	Ok
5	AR1254CCC500	AR1254CCC500	PP071139.D	08 Apr 2025 10:49		YPAJ	Ok
6	I.BLK	I.BLK	PP071140.D	08 Apr 2025 11:05		YPAJ	Ok
7	PB167469BL	PB167469BL	PP071141.D	08 Apr 2025 11:23	not required	YPAJ	Not Ok
8	Q1730-15	OU4-PCS-TC-25-0403	PP071142.D	08 Apr 2025 11:39		YPAJ	Ok
9	Q1730-17	OU4-PCS-TC-26-0403	PP071143.D	08 Apr 2025 11:56		YPAJ	Ok
10	Q1730-19	OU4-CF-15-040325	PP071144.D	08 Apr 2025 12:12	DCB High in 2ND column	YPAJ	Ok
11	Q1740-01	TP-20	PP071145.D	08 Apr 2025 13:08		YPAJ	Ok
12	Q1742-01	TR-06-040725	PP071146.D	08 Apr 2025 13:25		YPAJ	Ok,M
13	Q1742-01MS	TR-06-040725MS	PP071147.D	08 Apr 2025 13:41		YPAJ	Ok,M
14	Q1742-01MSD	TR-06-040725MSD	PP071148.D	08 Apr 2025 13:57		YPAJ	Ok,M
15	Q1743-01	TP-16	PP071149.D	08 Apr 2025 14:14	AR1260 Hit	YPAJ	Ok,M
16	Q1744-01	B-158-SB01	PP071150.D	08 Apr 2025 14:30	TCMX High in 2nd column	YPAJ	Ok
17	AR1660CCC500	AR1660CCC500	PP071151.D	08 Apr 2025 15:29		YPAJ	Ok
18	AR1242CCC500	AR1242CCC500	PP071152.D	08 Apr 2025 16:02		YPAJ	Ok

Instrument ID: ECD\_P

### Daily Analysis Runlog For Sequence/QCBatch ID # PP040825

Review By	yogesh	Review On	4/8/2025 3:06:55 PM
Supervise By	mohammad	Supervise On	4/10/2025 5:29:57 AM
SubDirectory	PP040825	HP Acquire Method	HP Processing Method PP032725
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1248CCC500	AR1248CCC500	PP071153.D	08 Apr 2025 16:18		YPAJ	Ok
20	AR1254CCC500	AR1254CCC500	PP071154.D	08 Apr 2025 16:34		YPAJ	Ok
21	I.BLK	I.BLK	PP071155.D	08 Apr 2025 16:51		YPAJ	Ok
22	PB167507BL	PB167507BL	PP071156.D	08 Apr 2025 17:07		YPAJ	Ok
23	PB167507BS	PB167507BS	PP071157.D	08 Apr 2025 17:23		YPAJ	Ok
24	Q1744-03	B-158-SB02	PP071158.D	08 Apr 2025 17:40		YPAJ	Ok
25	Q1745-01	IB-6A-WC	PP071159.D	08 Apr 2025 17:56		YPAJ	Ok,M
26	Q1745-09	IB-6.5-WC	PP071160.D	08 Apr 2025 18:12		YPAJ	Ok,M
27	Q1746-01	B-149-SB01	PP071161.D	08 Apr 2025 18:28		YPAJ	Ok
28	Q1746-03	B-149-SB02	PP071162.D	08 Apr 2025 18:45		YPAJ	Ok
29	Q1747-01	ARS20-0008	PP071163.D	08 Apr 2025 19:01		YPAJ	Ok,M
30	AR1660CCC500	AR1660CCC500	PP071164.D	08 Apr 2025 20:28		YPAJ	Ok
31	AR1242CCC500	AR1242CCC500	PP071165.D	08 Apr 2025 21:17		YPAJ	Ok
32	AR1248CCC500	AR1248CCC500	PP071166.D	08 Apr 2025 21:33		YPAJ	Ok
33	AR1254CCC500	AR1254CCC500	PP071167.D	08 Apr 2025 21:49		YPAJ	Ok
34	I.BLK	I.BLK	PP071168.D	08 Apr 2025 22:05		YPAJ	Ok

M : Manual Integration

**PERCENT SOLID**

**Supervisor:** Iwona  
**Analyst:** jignesh  
**Date:** 4/7/2025

**OVENTEMP IN Celsius(°C):** 107  
**Time IN:** 17:00  
**In Date:** 04/04/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**OvenID:** M OVEN#1

**OVENTEMP OUT Celsius(°C):** 103  
**Time OUT:** 08:25  
**Out Date:** 04/05/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**BalanceID:** M SC-4  
**Thermometer ID:** % SOLID- OVEN

QC:LB135307

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1729-05	SVOC-GPC-BLANK	1	1.00	1.00	2.00	2.00	100.0	
Q1729-06	PEST-GPC-BLANK	2	1.00	1.00	2.00	2.00	100.0	
Q1729-07	PEST-GPC-BLANK-SPIKE	3	1.00	1.00	2.00	2.00	100.0	
Q1729-08	PCB-GPC-BLANK	4	1.00	1.00	2.00	2.00	100.0	
Q1729-09	PCB-GPC-BLANK-SPIKE	5	1.00	1.00	2.00	2.00	100.0	
Q1729-10	SVOC-GPC2-BLANK	6	1.00	1.00	2.00	2.00	100.0	
Q1729-11	PEST-GPC2-BLANK	7	1.00	1.00	2.00	2.00	100.0	
Q1729-12	PEST-GPC2-BLANK-SPIKE	8	1.00	1.00	2.00	2.00	100.0	
Q1729-13	PCB-GPC2-BLANK	9	1.00	1.00	2.00	2.00	100.0	
Q1729-14	PCB-GPC2-BLANK-SPIKE	10	1.00	1.00	2.00	2.00	100.0	
Q1730-01	OU4-VSL-15-040325	11	1.14	10.58	11.72	11.39	96.9	
Q1730-03	OU4-VSL-16-040325	12	1.15	10.28	11.43	10.86	94.5	
Q1730-05	OU4-VSL-17-040325	13	1.16	11.32	12.48	11.62	92.4	
Q1730-07	OU4-PCS-TC-21-040325	14	1.18	10.92	12.1	10.9	89.0	
Q1730-09	OU4-PCS-TC-22-040325	15	1.16	11.79	12.95	11.87	90.8	
Q1730-11	OU4-PCS-TC-23-040325	16	1.19	11.24	12.43	11.41	90.9	
Q1730-13	OU4-PCS-TC-24-040325	17	1.18	10.42	11.6	10.69	91.3	
Q1730-15	OU4-PCS-TC-25-040325	18	1.14	11.13	12.27	11.43	92.5	
Q1730-17	OU4-PCS-TC-26-040325	19	1.15	10.84	11.99	11.13	92.1	
Q1730-19	OU4-CF-15-040325	20	1.15	10.74	11.89	11.23	93.9	
Q1732-01	TT-8	21	1.15	10.40	11.55	10.48	89.7	
Q1732-02	TT-8-EPH	22	1.15	10.33	11.48	10.34	89.0	
Q1732-03	TT-8-VOC	23	1.19	10.01	11.2	10.11	89.1	
Q1733-01	ETGI-328	24	1.18	10.19	11.37	8.37	70.6	
Q1733-02	ETGI-328-E2	25	1.18	10.29	11.47	8.27	68.9	
Q1734-01	HEH6237-1-1	26	1.00	1.00	2.00	2.00	100.0	pilc
Q1734-02	HEH6237-1-2	27	1.00	1.00	2.00	2.00	100.0	pilc
Q1734-03	STJ23-1-1	28	1.00	1.00	2.00	2.00	100.0	pilc

**PERCENT SOLID**

**Supervisor:** Iwona  
**Analyst:** jignesh  
**Date:** 4/7/2025

**OVENTEMP IN Celsius(°C):** 107  
**Time IN:** 17:00  
**In Date:** 04/04/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**OvenID:** M OVEN#1

**OVENTEMP OUT Celsius(°C):** 103  
**Time OUT:** 08:25  
**Out Date:** 04/05/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**BalanceID:** M SC-4  
**Thermometer ID:** % SOLID- OVEN

QC:LB135307

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1734-04	STJ23-1-2	29	1.00	1.00	2.00	2.00	100.0	pilc
Q1734-05	HIA989S-1-1	30	1.00	1.00	2.00	2.00	100.0	pilc
Q1734-06	HIA989S-1-2	31	1.00	1.00	2.00	2.00	100.0	pilc
Q1734-07	HED302R-1-1	32	1.00	1.00	2.00	2.00	100.0	pilc
Q1734-08	HED302R-1-2	33	1.00	1.00	2.00	2.00	100.0	pilc
Q1734-09	HED302R-2-1	34	1.00	1.00	2.00	2.00	100.0	pilc
Q1734-10	HED302R-2-2	35	1.00	1.00	2.00	2.00	100.0	pilc
Q1735-01	50660-50661-50662-5663 -COMP	36	1.18	10.92	12.1	10.42	84.6	
Q1736-01	GST1	37	1.18	10.04	11.22	9.07	78.6	
Q1736-02	GST2	38	1.18	10.93	12.11	9.98	80.5	
Q1737-01	RT3069	39	1.19	11.58	12.77	11.34	87.7	
Q1738-01	OK-02-040425	40	1.16	10.34	11.5	10.06	86.1	
Q1738-02	OK-02-040425-E2	41	1.19	10.54	11.73	10.37	87.1	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

## WORKLIST(Hardcopy Internal Chain)

WorkList Name : %1-040425

WorkList ID : 188724

Department : Wet-Chemistry

Date : 04-04-2025 08:12:22

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1736-01	GST1	Solid	Percent Solids	Cool 4 deg C	GENV01	L21	04/04/2025	Chemtech -SO
Q1736-02	GST2	Solid	Percent Solids	Cool 4 deg C	GENV01	L21	04/04/2025	Chemtech -SO
Q1730-01	OU4-VSL-15-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-03	OU4-VSL-16-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-05	OU4-VSL-17-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-07	OU4-PCS-TC-21-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-09	OU4-PCS-TC-22-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-11	OU4-PCS-TC-23-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-13	OU4-PCS-TC-24-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-15	OU4-PCS-TC-25-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-17	OU4-PCS-TC-26-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-19	OU4-CF-15-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1729-05	SVOC-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1729-06	PEST-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-07	PEST-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-08	PCB-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-09	PCB-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-10	SVOC-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-11	PEST-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-12	PEST-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-13	PCB-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO

Date/Time 04/04/15 15:20

Raw Sample Received by: John Smith

691 of 1015

Date/Time 04/04/15

Raw Sample Relinquished by:

John Smith

Raw Sample Received by:

John Smith

Page 1 of 2

Raw Sample Relinquished by:

John Smith

Raw Sample Received by:

John Smith

Raw Sample Relinquished by:

John Smith

14

15

16

17

18

19

20

11

12

13

14

15

16

17

18

19

20

## WORKLIST(Hardcopy Internal Chain)

Q1730-PCB

WorkList Name : %1-040425

WorkList ID : 188724

Department : Wet-Chemistry

Date : 04-04-2025 08:12:22

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1729-14	PCB-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1732-01	TT-8	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1732-02	TT-8-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1732-03	TT-8-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1733-01	ETGI-328	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1733-02	ETGI-328-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	I31	04/04/2025	Chemtech -SO
Q1734-01	HEH6237-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	I31	04/04/2025	Chemtech -SO
Q1734-08	HED302R-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-09	HED302R-2-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-10	HED302R-2-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1735-01	50660-50661-50662-5663-COM	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1737-01	RT3069	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-02	HEH6237-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-03	STJ23-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-04	STJ23-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-05	HIA989S-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-06	HIA989S-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-07	HED302R-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1738-01	OK-02-040425	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1738-02	OK-02-040425-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L31	04/04/2025	Chemtech -SO
					PSEG05	L31	04/04/2025	Chemtech -SO

Date/Time 04/04/15 15:20

Raw Sample Received by: JGRaw Sample Relinquished by: SA

Date/Time 04/04/15

Raw Sample Received by:

Raw Sample Relinquished by:

Page 2 of 2



SOP ID:	M3541-ASE Extraction-14		
Clean Up SOP #:	Acid Cleanup	Extraction Start Date :	04/07/2025
Matrix :	Solid	Extraction Start Time :	08:20
Weigh By:	EH	Extraction End Date :	04/07/2025
Balance check:	RJ	Extraction End Time :	11:30
Balance ID:	EX-SC-2	pH Meter ID:	N/A
pH Strip Lot#:	N/A	Hood ID:	3,7
Extraction Method:	<input type="checkbox"/> Separatory Funnel <input type="checkbox"/> Continous Liquid/Liquid <input type="checkbox"/> Sonication <input type="checkbox"/> Waste Dilution <input checked="" type="checkbox"/> Soxhlet		

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24328
Surrogate	1.0ML	200 PPB	PP24217
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2592
Baked Na2SO4	N/A	EP2597
Sand	N/A	E2865
Hexane	N/A	E3916
H2SO4 1:1	N/A	EP2565
N/A	N/A	N/A

**Extraction Conformance/Non-Conformance Comments:**

40 ML Vial lot# 03-40 BTS721. Q1735-01 Limited volume used as sample is Oily matrix.

KD Bath ID: N/A Envap ID: NEVAP-02  
 KD Bath Temperature: N/A Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
04/07/25 11:35	R.P (Est - 245)	Y.P. Pest I PCB
	Preparation Group	Analysis Group

**Analytical Method:** M3541-ASE Extraction-14

**Concentration Date:** 04/07/2025

Sample ID	Client Sample ID	Test	(g) / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB167469BL	ABLK469	PCB	30.01	N/A	ritesh	Evelyn	10			U7-1
PB167469BS	ALCS469	PCB	30.02	N/A	ritesh	Evelyn	10			2
Q1730-01	OU4-VSL-15-040325	PCB	30.07	N/A	ritesh	Evelyn	10	E		3
Q1730-03	OU4-VSL-16-040325	PCB	30.03	N/A	ritesh	Evelyn	10	E		4
Q1730-03MS	OU4-VSL-16-040325MS	PCB	30.05	N/A	ritesh	Evelyn	10	E		5
Q1730-03MSD	OU4-VSL-16-040325MSD	PCB	30.02	N/A	ritesh	Evelyn	10	E		6
Q1730-05	OU4-VSL-17-040325	PCB	30.08	N/A	ritesh	Evelyn	10	E		U2-1
Q1730-07	OU4-PCS-TC-21-040325	PCB	30.01	N/A	ritesh	Evelyn	10	E		2
Q1730-09	OU4-PCS-TC-22-040325	PCB	30.02	N/A	ritesh	Evelyn	10	E		3
Q1730-11	OU4-PCS-TC-23-040325	PCB	30.05	N/A	ritesh	Evelyn	10	E		4
Q1730-13	OU4-PCS-TC-24-040325	PCB	30.08	N/A	ritesh	Evelyn	10	E		5
Q1730-15	OU4-PCS-TC-25-040325	PCB	30.06	N/A	ritesh	Evelyn	10	E		6
Q1730-17	OU4-PCS-TC-26-040325	PCB	30.03	N/A	ritesh	Evelyn	10	E		U3-1
Q1730-19	OU4-CF-15-040325	PCB	30.02	N/A	ritesh	Evelyn	10	E		2
Q1732-01	TT-8	PCB	30.04	N/A	ritesh	Evelyn	10	D		3
Q1733-01	ETGI-328	PCB	30.06	N/A	ritesh	Evelyn	10	E	Small Particle	4
Q1735-01	50660-50661-50662-566 3-COMP	PCB	5.06	N/A	ritesh	Evelyn	10	E	Oily Debris	5
Q1736-01	GST1	PCB	30.07	N/A	ritesh	Evelyn	10			6
Q1736-02	GST2	PCB	30.03	N/A	ritesh	Evelyn	10			U6-1
Q1737-01	RT3069	PCB	30.05	N/A	ritesh	Evelyn	10	D		2
Q1738-01	OK-02-040425	PCB	30.01	N/A	ritesh	Evelyn	10	E		3

\* Extracts relinquished on the same date as received.

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q11732 WorkList ID : 188759 Department : Extraction Date : 04-07-2025 08:15:59

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample	Storage Location	Collect Date	Method
Q11730-01	OU4-VSL-15-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-03	OU4-VSL-16-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-05	OU4-VSL-17-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-07	OU4-PCS-TC-21-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-09	OU4-PCS-TC-22-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-11	OU4-PCS-TC-23-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-13	OU4-PCS-TC-24-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-15	OU4-PCS-TC-25-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-17	OU4-PCS-TC-26-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11730-19	OU4-CF-15-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B	
Q11732-01	TT-8	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	L31	04/04/2025	8081B	
Q11733-01	ETGI-328	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	L31	04/04/2025	8081B	
Q11737-01	RT3069	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	L31	04/04/2025	8081B	
Q11738-01	OK-02-040425	Solid	Pesticide-TCL	Cool 4 deg C	PSEG05	L31	04/04/2025	8081B	

Date/Time 04/07/25 08:17  
 Raw Sample Received by: J. C. S.  
 Raw Sample Relinquished by: J. C. S.

Date/Time 04/07/25 08:17  
 Raw Sample Received by: DR SM  
 Raw Sample Relinquished by: RJ (not 1st)

Page 1 of 1

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## Prep Standard - Chemical Standard Summary

**Order ID :** Q1730

**Test :** PCB

**Prepbatch ID :** PB167469,

**Sequence ID/Qc Batch ID:** PO040725,PO040825,PP040825,

**Standard ID :**

EP2565,EP2592,EP2597,PP24217,PP24328,PP24329,PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369,PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387,

**Chemical ID :**

E2865,E3551,E3804,E3876,E3877,E3916,M5173,P11522,P12699,P12702,P12931,P12936,P12948,P12949,P12957,P13354,P13356,P13373,P13381,P13589,P13591,P13697,P13702,P13830,P13878,P13883,W3112,W3177,

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	<a href="#">EP2565</a>	11/20/2024	05/20/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/20/2024

FROM 1000.00000ml of M5173 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	<a href="#">EP2592</a>	02/27/2025	08/12/2025	RUPESHKUMA R SHAH	None	None	Riteshkumar Patel 02/27/2025

FROM 4000.00000ml of E3876 + 4000.00000ml of E3877 = Final Quantity: 8000.000 ml

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	<a href="#">EP2597</a>	03/28/2025	07/01/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	Evelyn Huang 03/28/2025

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	<a href="#">PP24217</a>	03/05/2025	08/25/2025	Abdul Mirza	None	None	Yogesh Patel 03/06/2025

FROM 1.00000ml of P13354 + 999.00000ml of E3876 = Final Quantity: 1000.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	<a href="#">PP24328</a>	03/17/2025	08/25/2025	Abdul Mirza	None	None	Yogesh Patel 04/02/2025

FROM 0.50000ml of P12948 + 99.50000ml of E3876 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	<a href="#">PP24329</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13356 + 9.00000ml of W3177 = Final Quantity: 10.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	<a href="#">PP24330</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13697 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	<a href="#">PP24331</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24330 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	<a href="#">PP24332</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24330 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	<a href="#">PP24333</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24330 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	<a href="#">PP24334</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24332 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	<a href="#">PP24335</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13702 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	<a href="#">PP24336</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24335 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	<a href="#">PP24337</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24335 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	<a href="#">PP24338</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24335 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	<a href="#">PP24339</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24337 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	<a href="#">PP24340</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13878 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	<a href="#">PP24341</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24340 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	<a href="#">PP24342</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24340 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	<a href="#">PP24343</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24340 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	<a href="#">PP24344</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24342 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	<a href="#">PP24345</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P12931 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	<a href="#">PP24346</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.75000ml of PP24345 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	<a href="#">PP24347</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24345 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	<a href="#">PP24348</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24345 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	<a href="#">PP24349</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24347 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	<a href="#">PP24350</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P12936 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	<a href="#">PP24351</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24350 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	<a href="#">PP24352</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24350 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	<a href="#">PP24353</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24350 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	<a href="#">PP24354</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24352 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	<a href="#">PP24355</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13830 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	<a href="#">PP24356</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24355 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	<a href="#">PP24357</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24355 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	<a href="#">PP24358</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24355 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	<a href="#">PP24359</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24357 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	<a href="#">PP24360</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13883 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	<a href="#">PP24361</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24360 = Final Quantity: 1.000 ml

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	<a href="#">PP24362</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24360 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	<a href="#">PP24363</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24360 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	<a href="#">PP24364</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24362 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	<a href="#">PP24365</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.10000ml of P13381 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	<a href="#">PP24366</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24365 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	<a href="#">PP24367</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24365 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	<a href="#">PP24368</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24365 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	<a href="#">PP24369</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24367 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	<a href="#">PP24370</a>	03/18/2025	09/18/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12949 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	<a href="#">PP24371</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 98.50000ml of W3177 + 0.50000ml of PP24329 + 1.00000ml of PP24370 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	<a href="#">PP24372</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24371 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	<a href="#">PP24373</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13373 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1886	AR1221 500 PPB ICV	<a href="#">PP24374</a>	03/18/2025	08/12/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of E3877 + 0.50000ml of W3177 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	<a href="#">PP24375</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12699 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	<a href="#">PP24376</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24375 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	<a href="#">PP24377</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13589 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	<a href="#">PP24378</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24377 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	<a href="#">PP24379</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13591 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	<a href="#">PP24380</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24379 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	<a href="#">PP24381</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12957 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	<a href="#">PP24382</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24381 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	<a href="#">PP24384</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12702 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	<a href="#">PP24385</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24384 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	<a href="#">PP24386</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P11522 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	<a href="#">PP24387</a>	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24386 = Final Quantity: 1.000 ml

### CHEMICAL RECEIPT LOG BOOK

<b>Supplier</b>	<b>ItemCode / ItemName</b>	<b>Lot #</b>	<b>Expiration Date</b>	<b>Date Opened / Opened By</b>	<b>Received Date / Received By</b>	<b>Chemtech Lot #</b>
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	06/30/2025	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	08/25/2025	02/25/2025 / Rajesh	02/12/2025 / Rajesh	E3876
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	08/12/2025	02/12/2025 / Rajesh	02/12/2025 / Rajesh	E3877
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	10/03/2025	04/03/2025 / Rajesh	03/31/2025 / Rajesh	E3916

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	06/02/2025	06/01/2022 /	04/05/2022 / william	M5173
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	09/18/2025	03/18/2025 / yogesh	02/21/2022 / Ankita	P11522
Absolute Standards,Inc	91867 / Aroclor 1232 100 ug/mL	020823	09/18/2025	03/18/2025 / yogesh	08/07/2023 / Ankita	P12699
Absolute Standards,Inc	x9166 / Aroclor 1262 100 ug/mL	060523	09/18/2025	03/18/2025 / yogesh	08/07/2023 / Ankita	P12702
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	09/18/2025	03/18/2025 / yogesh	12/07/2023 / Ankita	P12931
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	09/18/2025	03/18/2025 / yogesh	12/07/2023 / Ankita	P12936

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	08/27/2025	02/27/2025 / Ankita	12/20/2023 / Yogesh	P12948
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	09/18/2025	03/18/2025 / yogesh	12/20/2023 / Yogesh	P12949
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/05/2025	03/05/2025 / Abdul	04/22/2024 / Abdul	P13354
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/18/2025	03/18/2025 / yogesh	04/22/2024 / Abdul	P13356
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	09/18/2025	03/18/2025 / yogesh	05/02/2024 / Ankita	P13373

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0207475	09/18/2025	03/18/2025 / yogesh	05/03/2024 / Abdul	P13381
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	09/18/2025	03/18/2025 / yogesh	10/14/2024 / Ankita	P13589
Agilent Technologies	PP-342-1 / Aroclor 1248	0006726317	09/18/2025	03/18/2025 / yogesh	10/14/2024 / Ankita	P13591
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0210629	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13697
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0215270	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13702
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0217391	09/18/2025	03/18/2025 / yogesh	12/09/2024 / Ankita	P13830

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0219655	09/18/2025	03/18/2025 / yogesh	01/23/2025 / Ankita	P13878
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0220950	09/18/2025	03/18/2025 / yogesh	01/23/2025 / Ankita	P13883
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177

Sand  
Purified  
Washed and Ignited



Material No.: 3382-05  
Batch No.: 0000243821  
Manufactured Date: 2018/04/09  
Retest Date: 2025/04/07  
Revision No: 1

## Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	<= 0.16 %	0.01

For Laboratory, Research or Manufacturing Use  
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US  
Packaging Site: Paris Mfg Ctr & DC

E 2865

*James T. Ethier*  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700  
Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreing matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

### COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/29/23 [E 3551]

RC-02-01, Ed. 3

Material No.: 9005-05  
Batch No.: 24E0761004  
Manufactured Date: 2024-05-02  
Retest Date: 2029-05-01  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.1
Titrable Base (μeq/g)	≤ 0.5	0.1
Water (H <sub>2</sub> O)	≤ 0.5 %	0.1 %
Solubility in H <sub>2</sub> O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO <sub>4</sub> )	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Rec'd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone  
CMOS



Material No.: 9005-05  
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

## Acetone CMOS



Material No.: 9005-05  
Batch No.: 24E0761004

For Microelectronic Use

**Country of Origin: USA  
Packaging Site: Paris Mfg Ctr & DC**

*Michelle Bales*  
Michelle Bales  
Sr. Manager, Quality Assurance



## Certificate of Analysis

1 Reagent Lane  
 Fair Lawn, NJ 07410  
 201.796.7100 tel  
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A

Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Recd - by RP on 2/12/25

E3877

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.

If there are any questions with this certificate, please call at (800) 227-6701.

\*Based on suggested storage condition.

## Certificate of Analysis

1 Reagent Lane  
Fair Lawn, NJ 07410  
201.796.7100 tel  
201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System  
Standard ISO9001:2015 by SAI Global Certificate Number CERT - 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A

Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H <sub>2</sub> O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

  
Harout Sahagian - Quality Control Manager - Fair Lawn

Rec'd. by RP on 3/31/25

E 3946

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.  
If there are any questions with this certificate, please call at (800) 227-6701.  
\*Based on suggested storage condition.

Hydrochloric Acid, 36.5-38.0%  
 BAKER INSTRUMENTS ANALYZED® Reagent  
 For Trace Metal Analysis



Material No.: 9530-33  
 Batch No.: 0000281827  
 Manufactured Date: 2021/03/30  
 Retest Date: 2026/03/29  
 Revision No.: 1

## Certificate of Analysis

Test	Specification	Result
ACS - Assay (as HCl) (by acid-base titrn)	36.5 – 38.0 %	37.6
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	1
ACS - Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS - Bromide (Br)	<= 0.005 %	< 0.005
ACS - Extractable Organic Substances	<= 5 ppm	< 1
ACS - Free Chlorine (as Cl <sub>2</sub> )	<= 0.5 ppm	< 0.5
Phosphate (PO <sub>4</sub> )	<= 0.05 ppm	< 0.03
Sulfate (SO <sub>4</sub> )	<= 0.5 ppm	< 0.3
Sulfite (SO <sub>3</sub> )	<= 0.8 ppm	0.3
Ammonium (NH <sub>4</sub> )	<= 3 ppm	< 1
Trace Impurities - Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities - Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities - Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities - Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities - Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities - Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities - Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities - Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities - Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities - Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities - Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities - Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



# Certificate of Analysis

P11518  
↓  
P11522  
02/21/22

**Product Name:** Aroclor 1268 Standard

**Product Number:** PP-382-1

**Lot Issue Date:** 09-Feb-2021

**Lot Number:** 0006587800

**Expiration Date:** 31-Mar-2029

**Description:**

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

**Matrix:** isoctane (2,2,4-trimethylpentane)

**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Intended Use:**

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Hazards:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this RM.

**Expiration of Certification:**

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

Monica Bourgeois  
QMS Representative



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 1 of 1

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



**CERTIFIED WEIGHT REPORT**

Part Number:	<u>91867</u>	Solvent#	10	
Lot Number:	<u>020823</u>	Acet	11	
Description:	WP 037 - Aroclor 1232		12	
Expiration Date:	PCB Technical Mixture		13	
Recommended Storage:	020833		14	
Nominal Concentration ( $\mu\text{g/mL}$ ):	Ambient (20 °C)		15	
NIST Test ID#:	100	Balance Uncertainty	16	
Weight(s) shown below were combined and diluted to (mL):	6UTB	0.057	Flask Uncertainty	17
	100.0			

Compound	RM#	Lot Number	Nominal Conc ( $\mu\text{g/mL}$ )	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurements," Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

**Comments**

GC3-M1 Analysis by Melissa Storier

Column ID SPB-608 30 meter X 0.53mm X 5 $\mu\text{m}$  film thickness

Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min


Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min

Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)

Rate = 8°C/min, Total run time = 35 min

Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1

Standard injection = 1.5 $\mu\text{L}$ , Range=3

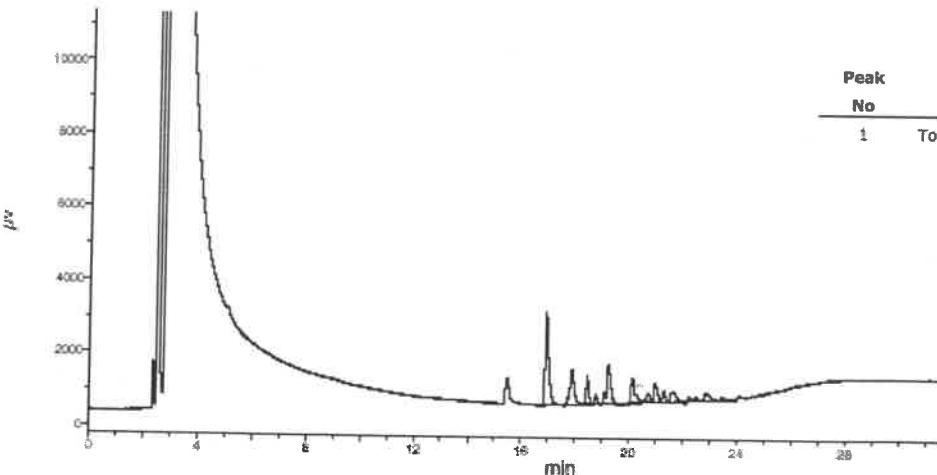





## CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## Certificate of Analysis

*chromatographic plus*

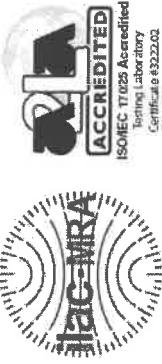

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. :	32009	Lot No.:	A0203672
Description :	Aroclor® 1242 Standard		
Container Size :	2 mL	Pkg Amt:	> 1 mL
Expiration Date :	January 31, 2030	Storage:	25°C nominal
Handling:	This product contains PCBs.	Ship:	Ambient

912928

X

912932

AJ  
12/07/23

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane  
**CAS #** 110-54-3  
**Purity** 99%

\* Expanded Uncertainty displayed in same units as Grav. Conc.

## Quality Confirmation Test

**Column:**  
30m x .25mm x 2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**  
helium-constant pressure 20 psi.

**Temp. Program:**  
200°C to 300°C  
@ 25°C/min. ( hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
300°C

**Det. Type:**  
ECD

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
0.2µl

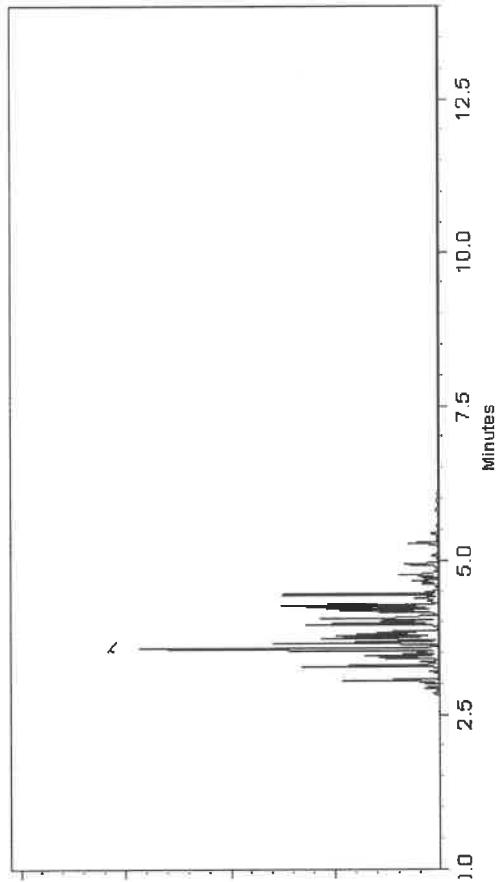

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boethamer - Operations Technician I

Date Mixed: 26-Oct-2023 Balance Serial # B442140311

Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FIM 80397



## CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010  
Description: Aroclor® 1248 Standard  
Container Size: 2 mL  
Expiration Date: January 31, 2030  
Handling: This product contains PCBs.

Lot No.: A0202803

Pkg Amt: > 1 mL

Storage: 25°C nominal

Ship: Ambient

*P12939  
P12939-X  
P12939-X  
P12939-X  
P12939-X  
P12939-X*

### CERTIFIED VALUES

Elation Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	—%	1,001.7 µg/mL	+/- 55.5850

Solvent: Hexane  
CAS # 110-54-3  
Purity 99%

\* Expanded Uncertainty displayed in same units as Grav. Conc.

## Quality Confirmation Test

**Column:**  
30m x .25mm x 2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**  
helium-constant pressure 20 psi.

**Temp. Program:**  
200°C to 300°C  
@ 25°C/min. ( hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
300°C

**Det. Type:**  
ECD

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
0.2µl

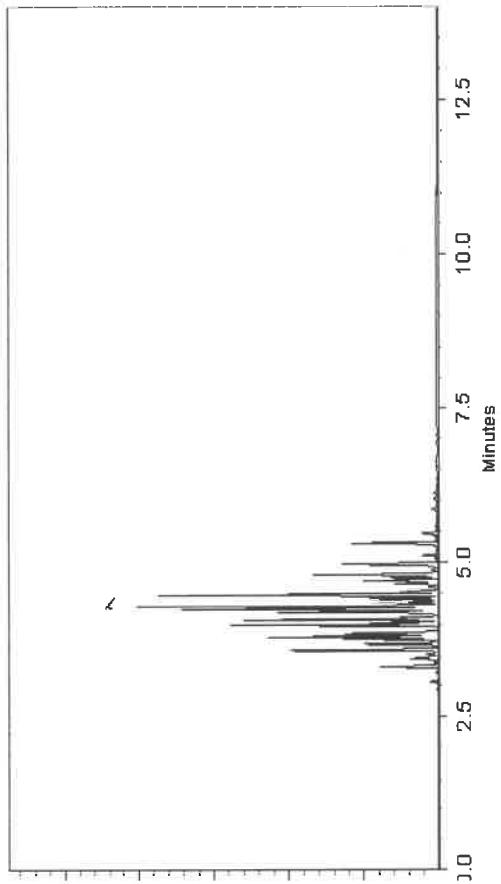

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Laith Clemente - Operations Technician |

Date Mixed: 03-Oct-2023 Balance Serial #: 1128360905

Jennifer Polino - Operations Tech II - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



### Certified Reference Material CRM



### CERTIFIED WEIGHT REPORT

Part Number:	20064	Solvent(s):	Lot#
Lot Number:	022023	Hexane	273615
Description:	CLP PCBIS - Aroclor Mix		
Aroclors 1016 & 1260			
Expiration Date:	022023	Formulated By:	Benson Chan DATE 12/19/23
Recommended Storage:	Ambient (20 °C)		
Nominal Concentration (µg/mL):	1000		
NIST Test ID#:	6UTB		
Weights(s) shown below were combined and diluted to (mL):	200.0	5E-05 Balance Uncertainty	
		0.010 Flask Uncertainty	

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty (%)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (Solvent Safety Info. On Attached pg.)		
									(+/−) (µg/mL)	CAS#	OSHA PEL (TWA)
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11096-82-5	0.5mg/m3 orl-rat 1315mg/kg

\*The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.

\*Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).

\*Standards are certified (</>).5% of the stated value, unless otherwise stated.

\*All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.

\*Uncertainty Reference: Taylor, B.N. and Kuyet, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

### Comments

GC3-M1 Analysis by Melissa Skinner

Column ID: SP8-608 30 meter X 0.53mm X 5um film thickness

Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min


Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min

Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)

Rate = 8°C/min, Total run time = 35 min

Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Edaq Channel 1

Standard injection = 1.5µL, Range=3

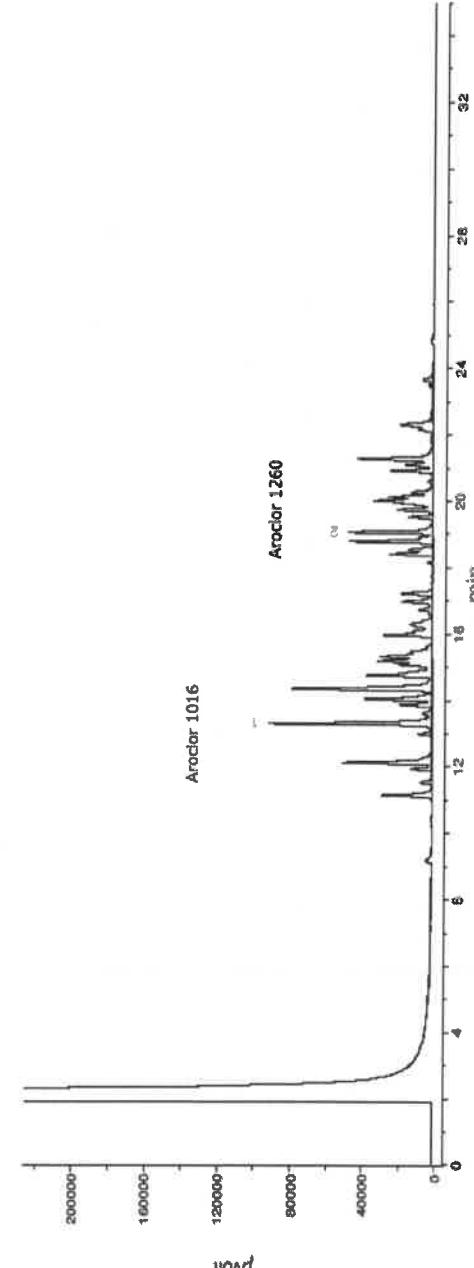

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



### Certified Reference Material CRM



#### CERTIFIED WEIGHT REPORT

Part Number:	20064	Solvent(s):	Lot#
Lot Number:	022023	Hexane	273615
Description:	CLP PCBIS - Aroclor Mix		
Aroclors 1016 & 1260			
Expiration Date:	022023	Formulated By:	Benson Chan DATE 12/19/23
Recommended Storage:	Ambient (20 °C)		
Nominal Concentration (µg/mL):	1000		
NIST Test ID#:	6UTB		
Weights(s) shown below were combined and diluted to (mL):	200.0	5E-05 Balance Uncertainty	
		0.010 Flask Uncertainty	

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty (%)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±t) (µg/mL)	SDS Information
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2 N/A N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11096-82-5 0.5mg/m3 orl-rat 1315mg/kg

\*The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.

\*Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).

\*Standards are certified (<+/>) 0.5% of the stated value, unless otherwise stated.

\*All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.

\*Uncertainty Reference: Taylor, B.N. and Kuyet, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

#### Comments

GC3-M1 Analysis by Melissa Skinner

Column ID: SPB-608 30 meter X 0.53mm X5um film thickness

Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min


Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min

Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)

Rate = 8°C/min, Total run time = 35 min

Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Edaq Channel 1

Standard injection = 1.5µL, Range=3

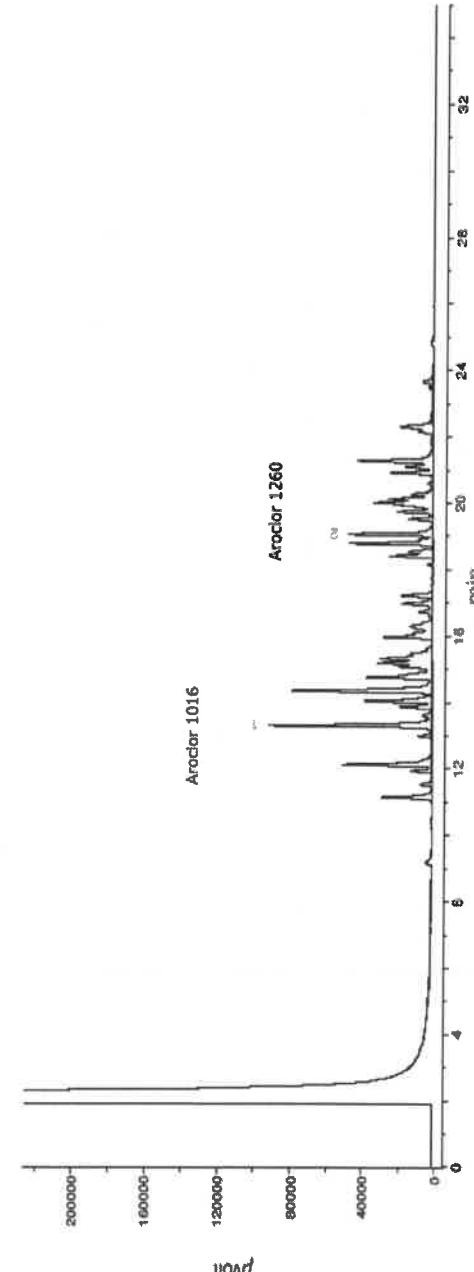

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



## Certified Reference Material CRM



### CERTIFIED WEIGHT REPORT

Part Number:	<u>99139</u>	Solvent(s):	<u>Iso-octane</u>	Lot#	<u>82227</u>
Lot Number:	<u>121823</u>				
Description:	<u>Arcoletor 1254</u>				
Expiration Date:	<u>12/18/23</u>				
Recommended Storage:	<u>Ambient (20 °C)</u>				
Nominal Concentration ( $\mu\text{g/mL}$ ):	<u>100</u>	5E-05	Balance Uncertainty		
NIST Test ID#:	<u>6UTB</u>	<u>20.0</u>	<u>0.003</u>	Flask Uncertainty	
Volume(s) shown below were combined and diluted to (mL):					

Note: Arcoletor 1254 is a mix of isomers.

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Final Conc. ( $\mu\text{g/mL}$ )	Initial Conc. ( $\mu\text{g/mL}$ )	Final Conc. ( $\mu\text{g/mL}$ )	Uncertainty (+/-) ( $\mu\text{g/mL}$ )	(Solvent Safety Info. On Attached pg.)	SDS Information
1. Arcoletor 1254	<u>79100</u>	<u>121823</u>	<u>0.10</u>	<u>2.00</u>	<u>0.017</u>	<u>1003.3</u>	<u>100.1</u>	<u>1.8</u>	<u>11097.69-1</u>	<u>0.56ng/m3 (skin)</u>	<u>or rat 1295mg/kg</u>

\* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.

\* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).

\* All Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.

\* All Standards, after opening ampoule, should be stored with caps tight and under appropriate laboratory conditions.

\* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results," NIST Technical Note 1297. U.S. Government Printing Office, Washington, DC, (1994).

### Comments

GC3-MI Analysis by Melissa Storier

Column ID SPB-30 meter X 0.5mm X 0.3um film thickness

Flow rates: Helium (carrier) = 5ml/min, Helium (make-up) = 25ml/min

Hydrogen (make-up) = 30ml/min, Air (make-up) = 350ml/min

Rate = 5°C/min, Total run time = 25 min


Oven: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 260 °C (Time 2 = 13.5 min)

Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = E丝q Channel 1

Standard injection = 1.5μL, Range=3

Peak No. Name FID RT (min.)

1	Total Arcoletor 1254	16.12
---	----------------------	-------

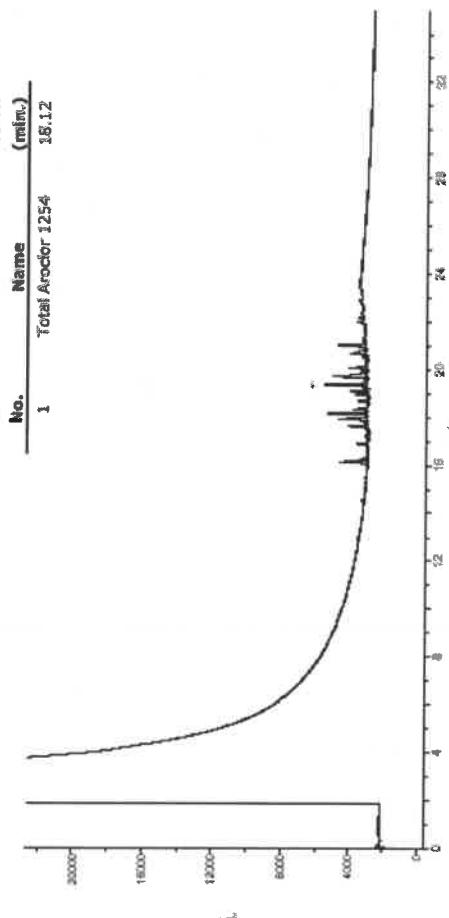

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 32000

**Lot No.:** A0206810

**Description:** Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

**Container Size:** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date:** April 30, 2030

**Storage:** 10°C or colder

**Handling:** Contains PCBs - sonicate prior to use.

**Ship:** Ambient

P13348  
P13357  
DAU  
04/25/2024

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone

**CAS #** 67-64-1  
**Purity** 99%

### Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isoctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

# Quality Confirmation Test

**Column:**30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**200°C to 300°C  
@ 25°C/min. ( hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

10 ml/min.

**Inj. Vol**


1µl

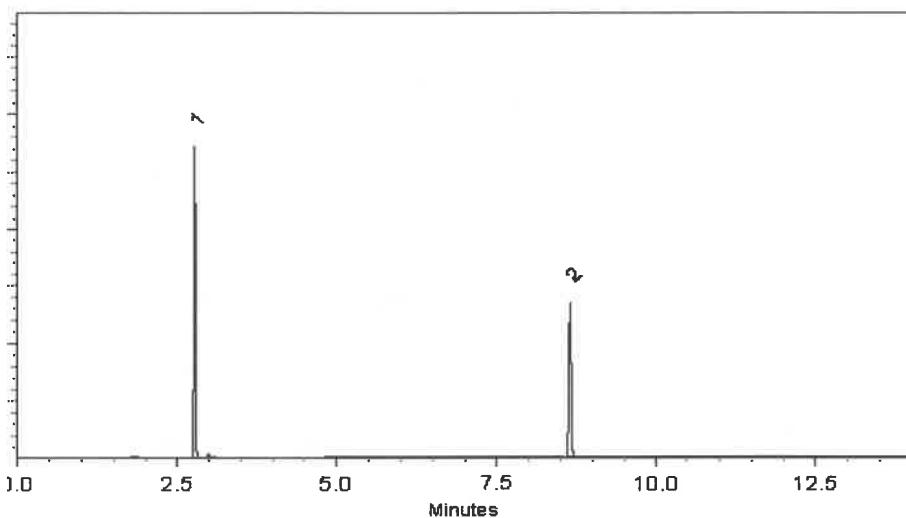

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024 Balance Serial #: 1128360905

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

P 13348  
↓  
P 13357  
S AUF  
04/25/2025



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 32000

**Lot No.:** A0206810

**Description:** Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

**Container Size:** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date:** April 30, 2030

**Storage:** 10°C or colder

**Handling:** Contains PCBs - sonicate prior to use.

**Ship:** Ambient

P13348  
P13357  
DAU  
04/25/2024

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone

**CAS #** 67-64-1  
**Purity** 99%

### Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isoctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

# Quality Confirmation Test

**Column:**30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**200°C to 300°C  
@ 25°C/min. ( hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

10 ml/min.

**Inj. Vol**


1µl

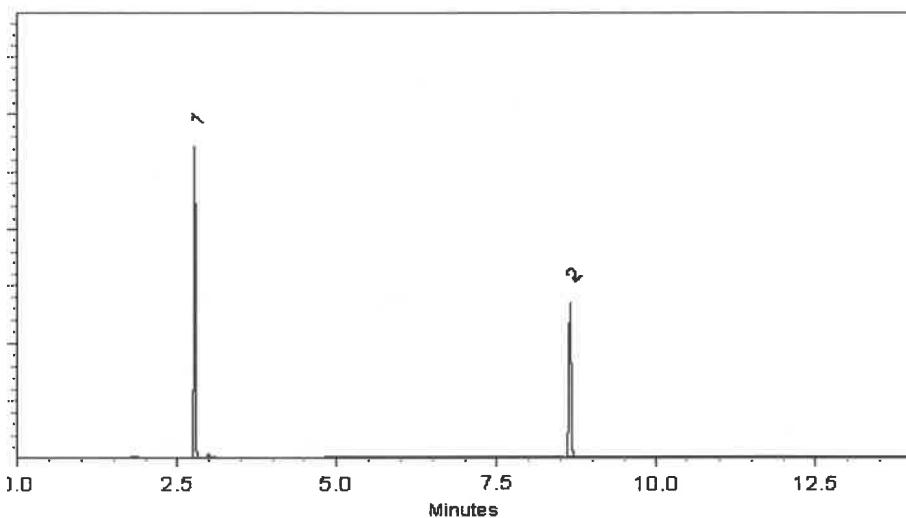

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024 Balance Serial #: 1128360905

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

P 13348  
↓  
P 13357  
S AUF  
04/25/2025



Trusted Answers

ISO 17034

## Reference Material Certificate

### Product Information Sheet

Product Name:	Aroclor 1221 Standard		
Product Number:	PP-292-1		
Storage Conditions:	Store at Room Temperature (15° to 30°C).		
Component Name	Concentration	Uncertainty	CAS#
Aroclor 1221	100.3 ±	0.5 µg/ml	011104-28-2
			NT01017

**Matrix:** isoctane (2,2,4-trimethylpentane)

#### Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

#### Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

#### Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

#### Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

#### Safety:

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

#### Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

#### Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342  
J  
P13343  
05/06/24  
AJ

Page: 1 of 2

CSD-QA-015.2

ISO 17025


Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 [www.agilent.com/quality](http://www.agilent.com/quality)



**Maintenance of Certification:**  
If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

  
Monica Bougeois  
QMS Representative



ISO 17034  
Cert No. AR-1936

250 Smith Street North Kingstown, Rhode Island 02852 [www.agilent.com/quality](http://www.agilent.com/quality)

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015 Quality Management System. Cert# 95121532

Page: 2 of 2

[www.agilent.com/quality/  
CSD-QA-015.2](http://www.agilent.com/quality/CSD-QA-015.2)

ISO 17025  
Cert No. AT-1937

6 7 8 9 10 11 12 13 14 15 16 17 18 19 20



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



ILAC-MRA  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ILAC-MRA  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

## Certificate of Analysis *chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 32410

**Lot No.:** A0207475

**Description:** Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

**Container Size:** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date:** May 31, 2030

**Storage:** 25°C nominal

**Handling:** This product contains PCBs.

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1268	11100-14-4	10947000	----%	1,000.0 µg/mL	+/- 55.4925

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

P 13386  
P 13381  
2  
J. STAN  
05/01/2024

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

# Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. ( hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

Split ratio 500:1

**Inj. Vol**

0.2µl

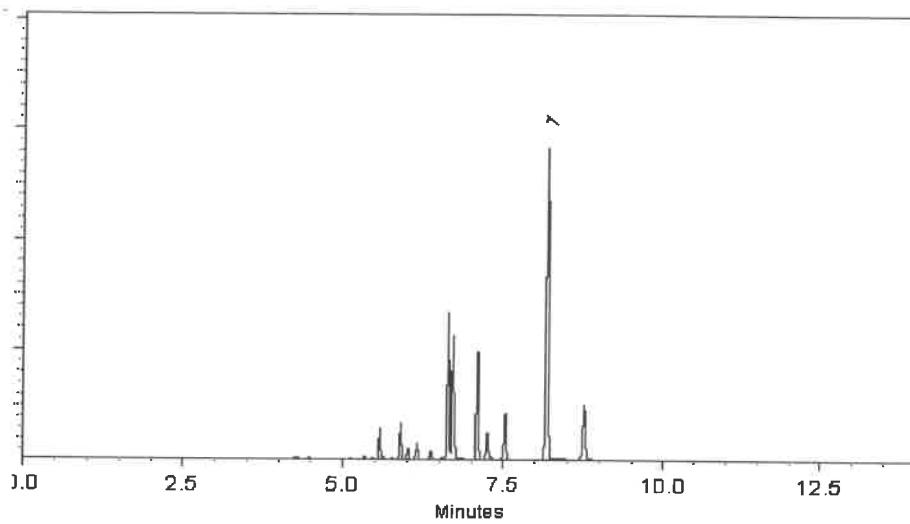

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*michael maye*  
**Michael Maye - Operations Tech I**

Date Mixed: 06-Feb-2024      Balance Serial #: B442140311


*Dillan Murphy*  
**Dillan Murphy - Operations Technician I**

Date Passed: 09-Feb-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

P13380  
↓  
P13381  
②  
Dated 05/6/2024

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



## Reference Material Certificate

**Product Name:** Aroclor 1242 Standard      **Lot Number:** 0006665550  
**Product Number:** PP-312-1      **Lot Issue Date:** 08-Feb-2022  
**Storage Conditions:** Store at Room Temperature (15° to 30°C).      **Expiration Date:** 31-Jan-2027

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
Aroclor 1242	100.4	± 0.5 µg/mL		053469-21-9	NT01020

**Matrix:** isoctane (2,2,4-trimethylpentane)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Safety:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

**Intended Use:**


This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Expiration of Certification:**

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

p13589  
↓  
p13590

AJ  
10/11/12/14

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

Monica Bourgeois  
QMS Representative



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015  
Quality Management System. Cert# 951215321

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)

CSD-QA-015.1



ISO 17025  
Cert No. AT-

**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Aroclor 1248 Standard

**Lot Number:** 0006726317

**Product Number:** PP-342-1

**Lot Issue Date:** 27-Jan-2023

**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Expiration Date:** 28-Feb-2031

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1248	100.3	± 0.5 µg/mL	012672-29-6	NT01582

**Matrix:** isoctane (2,2,4-trimethylpentane)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material (RM) standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above. Purity values are taken from approved vendor raw material certificates.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference (RM) standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Safety:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

**Intended Use:**

This analytical reference (RM) standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Expiration of Certification:**

The certification of this analytical reference standard (RM) is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13591

↓


P13592

AJ  
10/14/2024

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

  
Monica Bourgeois  
QMS Representative



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO  
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1

ISO 17025



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



## Certificate of Analysis *chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32039

**Lot No.:** A0210629

P13697  
↓  
P13701 } Y.P.  
} 10/19/24

**Description :** Aroclor® 1016/1260 Mix

Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2030

**Storage:** 25°C nominal

**Handling:** This product contains PCBs.

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1016	12674-11-2	07	----%	1,005.3 µg/mL	+/- 55.7809
2	Aroclor 1260	11096-82-5	1320657	----%	1,000.0 µg/mL	+/- 55.4850

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane

**CAS #** 110-54-3

**Purity** 99%

# Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. ( hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

10 ml/min.

**Inj. Vol**


0.2µl

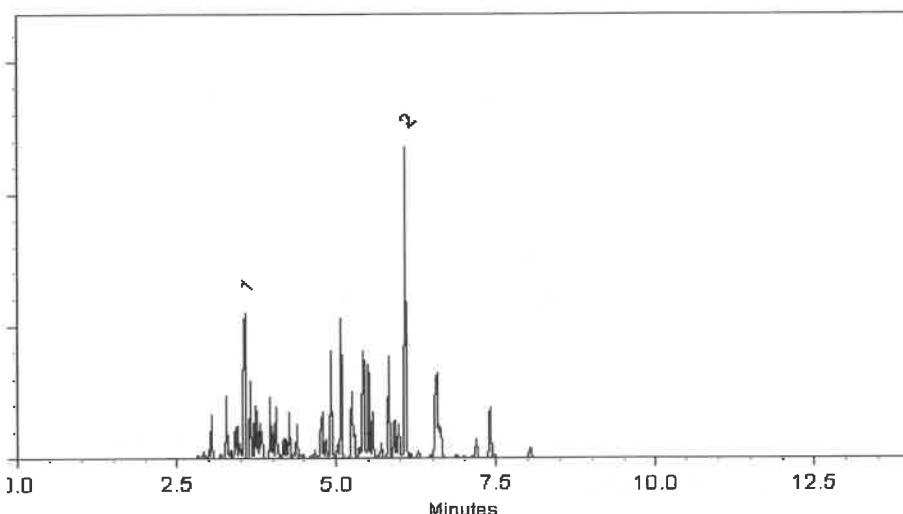

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Laith Clemente - Operations Technician I

Date Mixed: 22-Apr-2024 Balance Serial #: B442140311

  
Dillon Murphy - Operations Technician I

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 32007

**Lot No.:** A0215270

**Description:** Aroclor® 1221 Standard

Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul

**Container Size:** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date:** November 30, 2030

**Storage:** 25°C nominal

**Handling:** This product contains PCBs.

**Ship:** Ambient

P13902 }  
P13903 } Y.P.  
10/17/24

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1221	11104-28-2	14969200	----%	1,005.0 µg/mL	+/- 55.7700

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

# Quality Confirmation Test

**Column:**

30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**

200°C to 300°C  
@ 25°C/min. ( hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

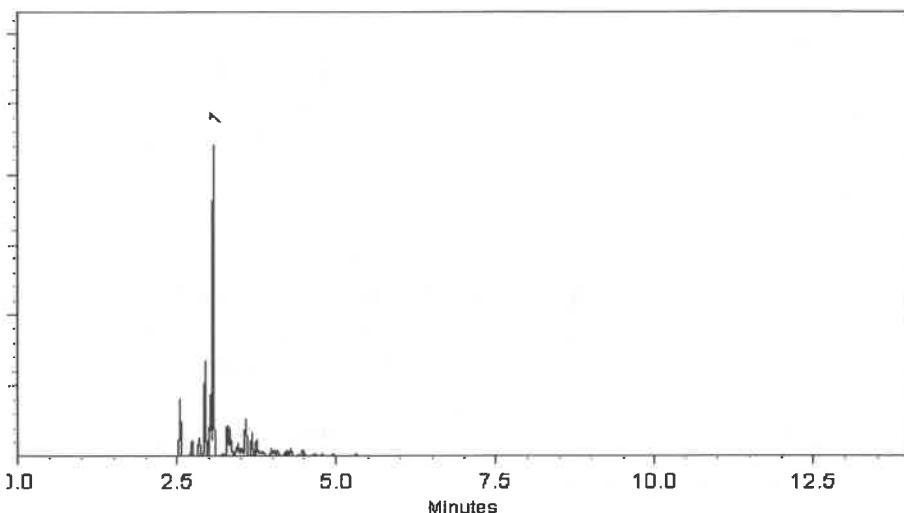

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
Michael Maye - Operations Tech I

Date Mixed: 16-Aug-2024 Balance Serial #: 1128360905

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Aug-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



21  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



22  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

## Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32011

**Lot No.:** A0217391

**Description :** Aroclor® 1254 Standard

Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** January 31, 2031

**Storage:** 25°C nominal

**Handling:** This product contains PCBs.

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1254	11097-69-1	124-191-B	----%	1,004.7 µg/mL	+/- 55.7515

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane

**CAS #** 110-54-3

**Purity** 99%

P13830  
↓  
P13832 12/09/24 AJ

# Quality Confirmation Test

**Column:**30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

**Temp. Program:**200°C to 300°C  
@ 25°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

300°C

**Det. Type:**


ECD

**Split Vent:**

300 ml/min.

**Inj. Vol**

1µl

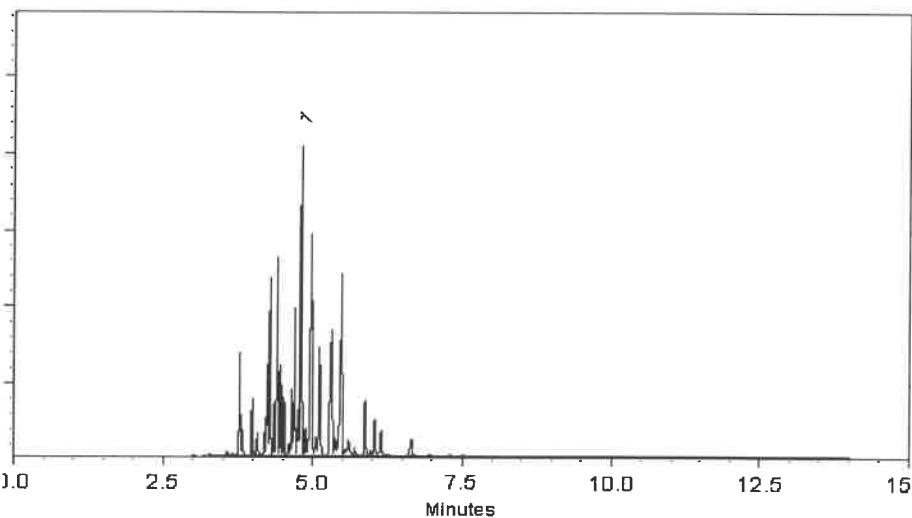

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*michael maye*  
**Michael Maye - Operations Tech I**

Date Mixed: 02-Oct-2024      Balance Serial #: C322230531

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

Date Passed: 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397





## CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## Certificate of Analysis

*chromatographic plus*



**ACCREDITED**  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01

**ACCREDITED**  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :**

32008

**Description :**

Aroclor® 1232 Standard

**Container Size :**

2 mL

**Pkg Amt:**

> 1 mL

**Expiration Date :**

March 31, 2031

**Handling:**

This product contains PCBs.

### C E R T I F I E D   V A L U E S

Elation Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1232	11141-16-5	15665-01	----%	1,007.0 µg/mL	+/- 55.8810

**Solvent:**

Hexane

**CAS #**

110-54-3

**Purity**

99%

\* Expanded Uncertainty displayed in same units as Grav. Conc.

P19848

↓

P19850

AJ  
01/28/25

## Quality Confirmation Test

**Column:**  
30m x .25mm x .2um  
Rtx-CLP II (cat.# 11323)

**Carrier Gas:**  
helium-constant pressure 20 psi.

**Temp. Program:**  
200°C to 300°C  
@ 25°C/min. ( hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
300°C

**Det. Type:**  
ECD

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
1μl

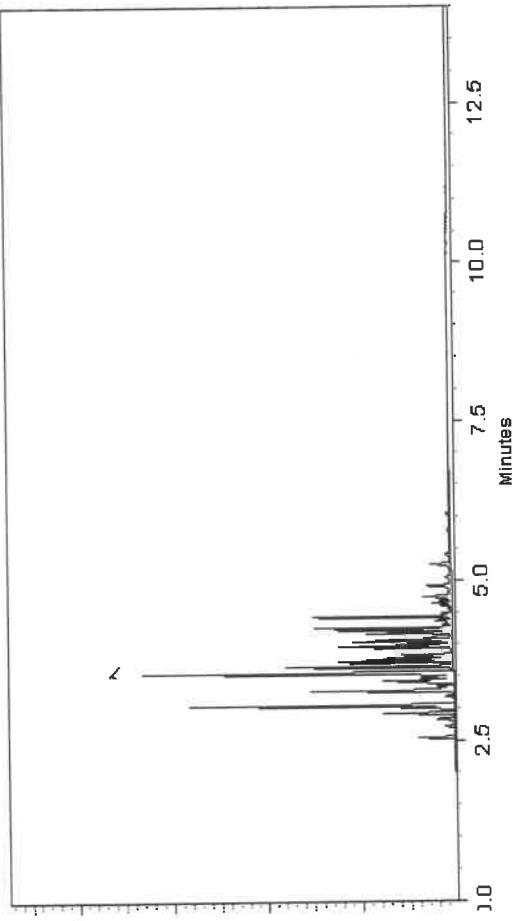

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*michael maye*  
**Michael Maye - Operations Tech I**

Date Mixed: 02-Dec-2024      Balance Serial # C322230531

*Brittany Federino*  
**Brittany Federino - Operations Tech I**

Date Passed: 05-Dec-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397




## CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellevonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32409

**Lot No.:** A0220950

**Description :** Aroclor® 1262 Standard

Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2031

**Storage:** 25°C nominal

**Handling:** This product contains PCBs.

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elation Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1262	37324-23-5	10849100	----%	1,002.0 µg/mL	+/- 55.6035

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

P138862  
AJ  
01/28/25  
P138863  
AJ  
01/28/25

6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## Quality Confirmation Test

Q1730-PCB  
**Column:**  
30m x .25mm x 2um  
Rtx-CLP I (cat.# 11323)

**Carrier Gas:**  
helium-constant pressure 20 psi.

**Temp. Program:**  
200°C to 300°C  
@ 25°C/min. (hold 10 min.)

**Inj. Temp:**  
250°C

**Def. Temp:**  
300°C

**Det. Type:**  
ECD

**Split Vent:**  
300 ml/min.

**Inj. Vol**  
0.2µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 09-Jan-2025

Balance Serial # C322230531

  
Brittany Federenko - Operations Tech

Date Passed: 14-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis



Material No.: 9262-03  
Batch No.: 24G1962003  
Manufactured Date: 2024-05-23  
Expiration Date: 2025-08-22  
Revision No.: 0

W314X  
W314X  
CPLTE. 02/03/2023  
SP

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak

Director Quality Operations, Biosciences



# SHIPPING DOCUMENTS

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



### Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## LOGIN REPORT/SAMPLE TRANSFER

**Order ID :** Q1730      **NOBI03**

**Order Date :** 4/4/2025 10:51:00 AM

**Project Mgr :** Yazmeen

**Client Name :** Nobis Group

**Project Name :** Raymark Superfund Site

**Report Type :** Level 4

**Client Contact :** Adam Roy

**Receive DateTime :** 4/4/2025 10:45:00 AM

**EDD Type :** EQUIS

**Invoice Name :** Nobis Group

**Purchase Order :**

**Hard Copy Date :**

**Invoice Contact :** Adam Roy

**Date Signoff :** 4/4/2025 11:24:53 AM

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUUE DATES
Q1730-01	OU4-VSL-15-040325	Solid	04/03/2025	12:10	VOCMS Group3	8260D	10 Bus. Days		
Q1730-03	OU4-VSL-16-040325	Solid	04/03/2025	12:20	VOCMS Group3	8260D	10 Bus. Days		
Q1730-05	OU4-VSL-17-040325	Solid	04/03/2025	12:30	VOCMS Group3	8260D	10 Bus. Days		
Q1730-07	OU4-PCS-TC-21-040325	Solid	04/03/2025	13:45	VOCMS Group3	8260D	10 Bus. Days		
Q1730-09	OU4-PCS-TC-22-040325	Solid	04/03/2025	13:50	VOCMS Group3	8260D	10 Bus. Days		
Q1730-11	OU4-PCS-TC-23-040325	Solid	04/03/2025	13:55	VOCMS Group3	8260D	10 Bus. Days		
Q1730-13	OU4-PCS-TC-24-040325	Solid	04/03/2025	14:00	VOCMS Group3	8260D	10 Bus. Days		
Q1730-15	OU4-PCS-TC-25-040325	Solid	04/03/2025	14:05	VOCMS Group3	8260D	10 Bus. Days		

## LOGIN REPORT/SAMPLE TRANSFER

**Order ID :** Q1730      **NOBI03**

**Order Date :** 4/4/2025 10:51:00 AM

**Project Mgr :** Yazmeen

**Client Name :** Nobis Group

**Project Name :** Raymark Superfund Site

**Report Type :** Level 4

**Client Contact :** Adam Roy

**Receive DateTime :** 4/4/2025 10:45:00 AM

**EDD Type :** EQUIS

**Invoice Name :** Nobis Group

**Purchase Order :**


**Hard Copy Date :**

**Invoice Contact :** Adam Roy

**Date Signoff :** 4/4/2025 11:24:53 AM


LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DU <sup>E</sup> DATES
Q1730-17	OU4-PCS-TC-26-040325	Solid	04/03/2025	14:10	VOCMS Group3		8260D	10 Bus. Days	
Q1730-19	OU4-CF-15-040325	Solid	04/03/2025	13:00	VOCMS Group3		8260D	10 Bus. Days	
					VOCMS Group3		8260D	10 Bus. Days	

**Relinquished By :**



**Date / Time :** 4/4/25 14:15

**Received By :**

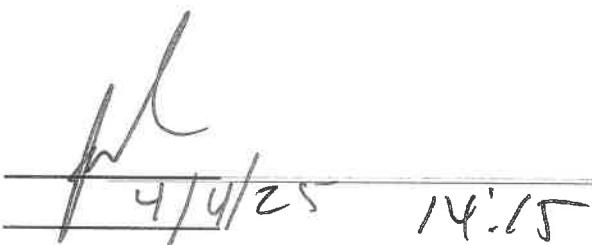

**Date / Time :** 4/4/25 14:15

**Storage Area :** VOA Refrigerator Room

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109973.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:21  
 Operator : YP/AJ  
 Sample : AR1660ICC750  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:36:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.693	3.690	705.7E6	403.4E6	75.190	74.986
2) SA Decachlor...	8.745	8.696	568.9E6	170.8E6	75.465	72.950

Target Compounds

3) L1 AR-1016-1	4.785	4.772	246.8E6	133.8E6	747.915	745.960
4) L1 AR-1016-2	4.805	4.791	347.8E6	195.6E6	753.172	750.675
5) L1 AR-1016-3	4.862	4.967	233.7E6	104.0E6	751.394	748.099
6) L1 AR-1016-4	4.982	5.009	186.4E6	84297055	751.636	746.609
7) L1 AR-1016-5	5.239	5.222	197.8E6	110.8E6	753.927	750.256
31) L7 AR-1260-1	6.280	6.255	350.7E6	185.8E6	755.816	746.573
32) L7 AR-1260-2	6.470	6.442	429.8E6	216.7E6	759.623	745.669
33) L7 AR-1260-3	6.837	6.595	362.6E6	209.2E6	757.414	751.587
34) L7 AR-1260-4	7.098	7.067	310.3E6	154.0E6	751.251	745.577
35) L7 AR-1260-5	7.340	7.307	800.9E6	394.6E6	755.153	803.094



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109973.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 14:21  
 Operator : YP/AJ  
 Sample : AR1660ICC750  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:36:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

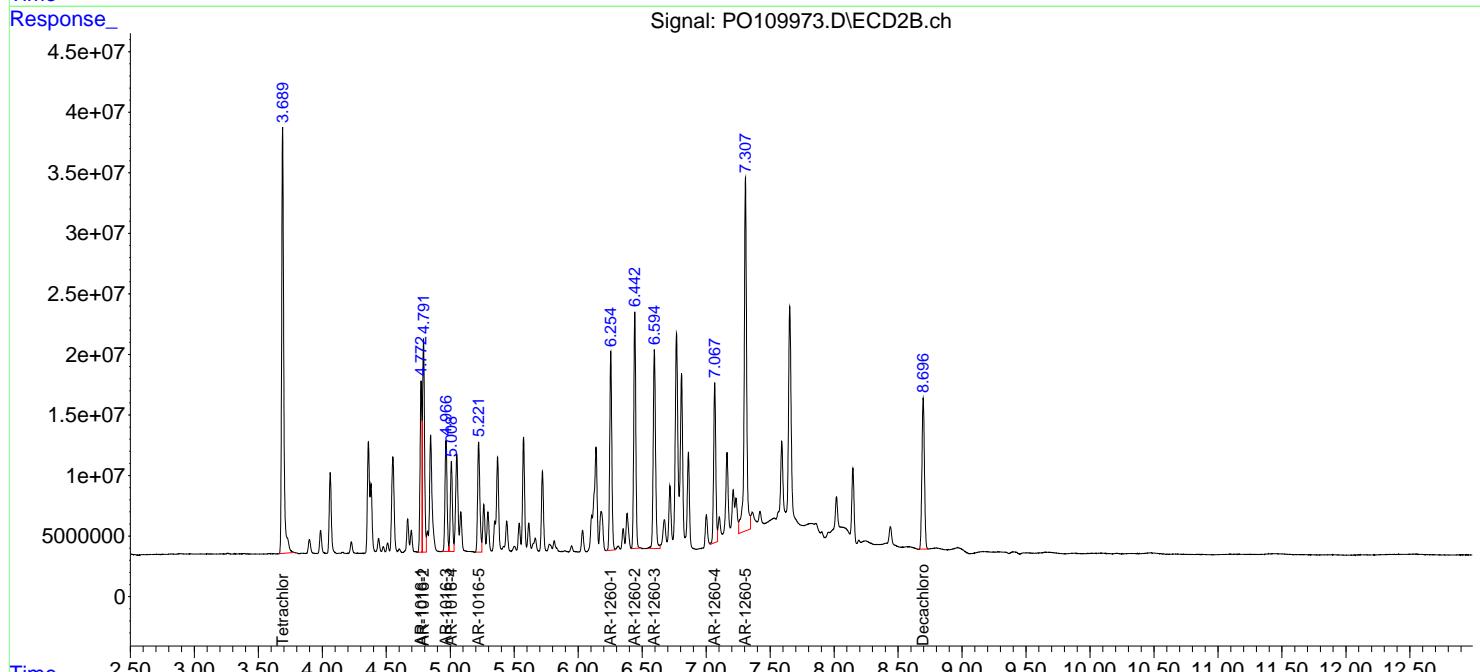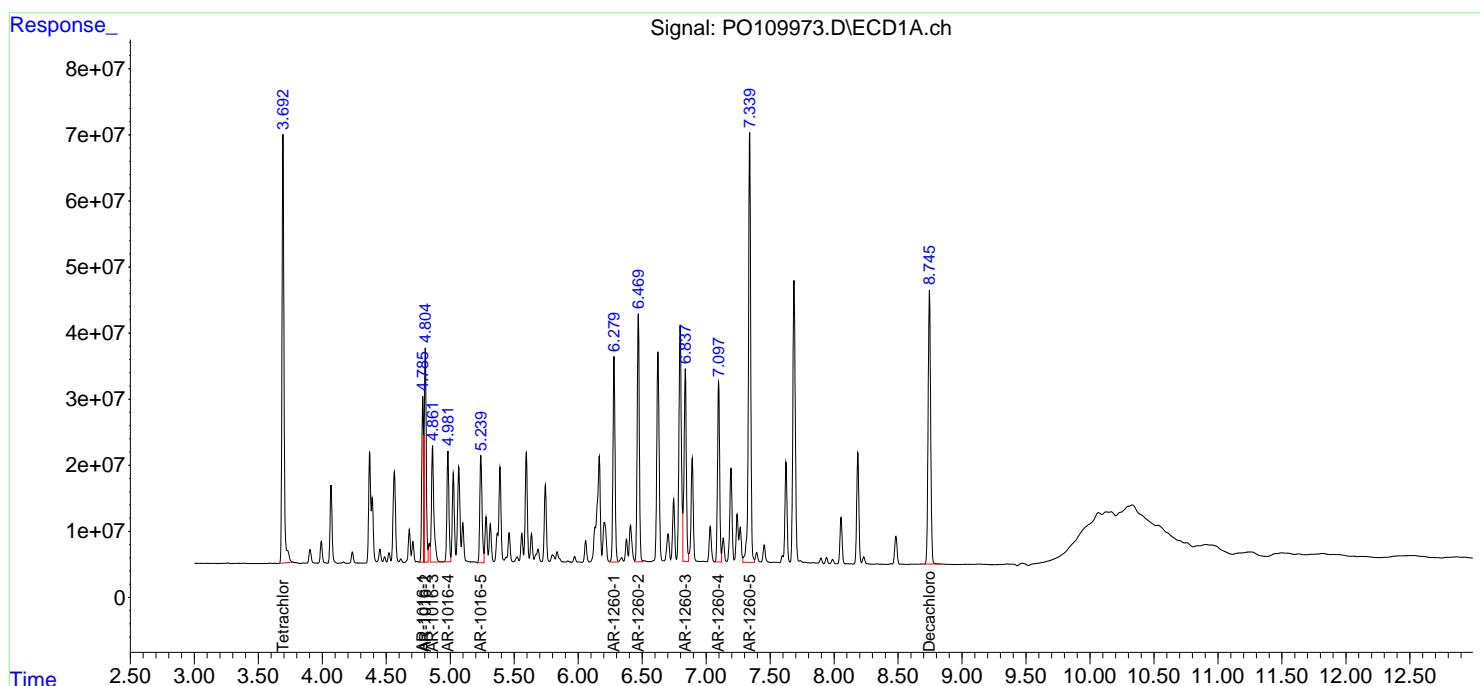

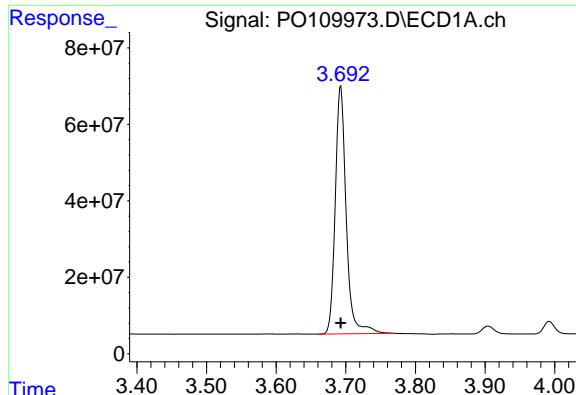


#1 Tetrachloro-m-xylene  
R.T.: 3.693 min  
Delta R.T.: 0.000 min  
Response: 705727801  
Conc: 75.19 ng/ml


**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC750

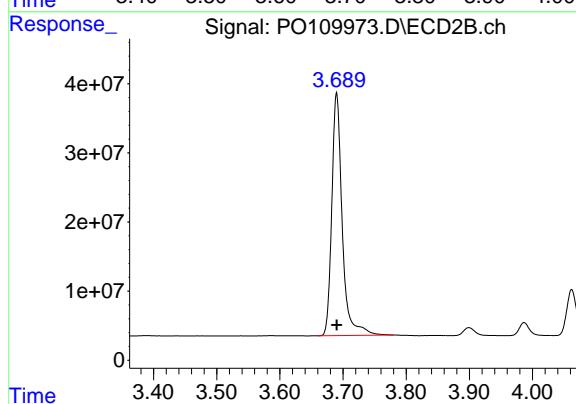


#1 Tetrachloro-m-xylene  
R.T.: 3.690 min  
Delta R.T.: 0.000 min  
Response: 403376580  
Conc: 74.99 ng/ml

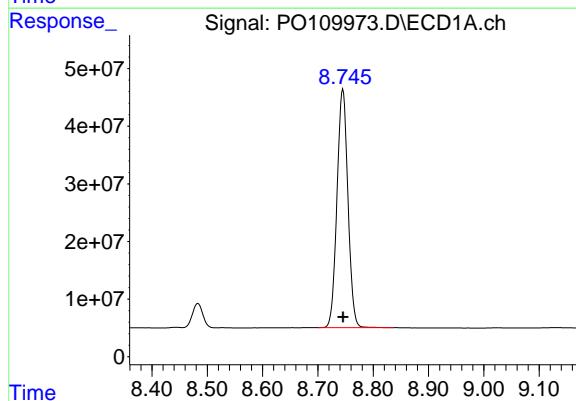

#2 Decachlorobiphenyl  
R.T.: 8.745 min  
Delta R.T.: 0.000 min  
Response: 568890214  
Conc: 75.47 ng/ml

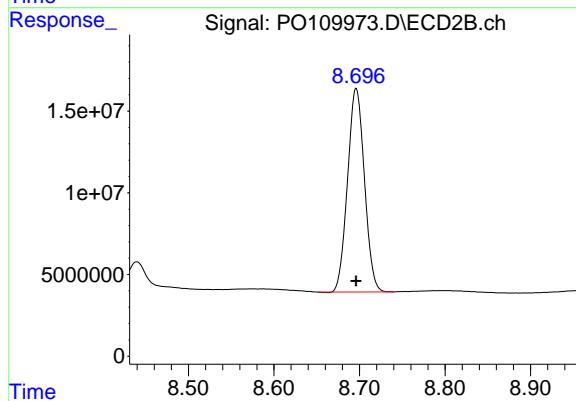

#2 Decachlorobiphenyl  
R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 170836588  
Conc: 72.95 ng/ml

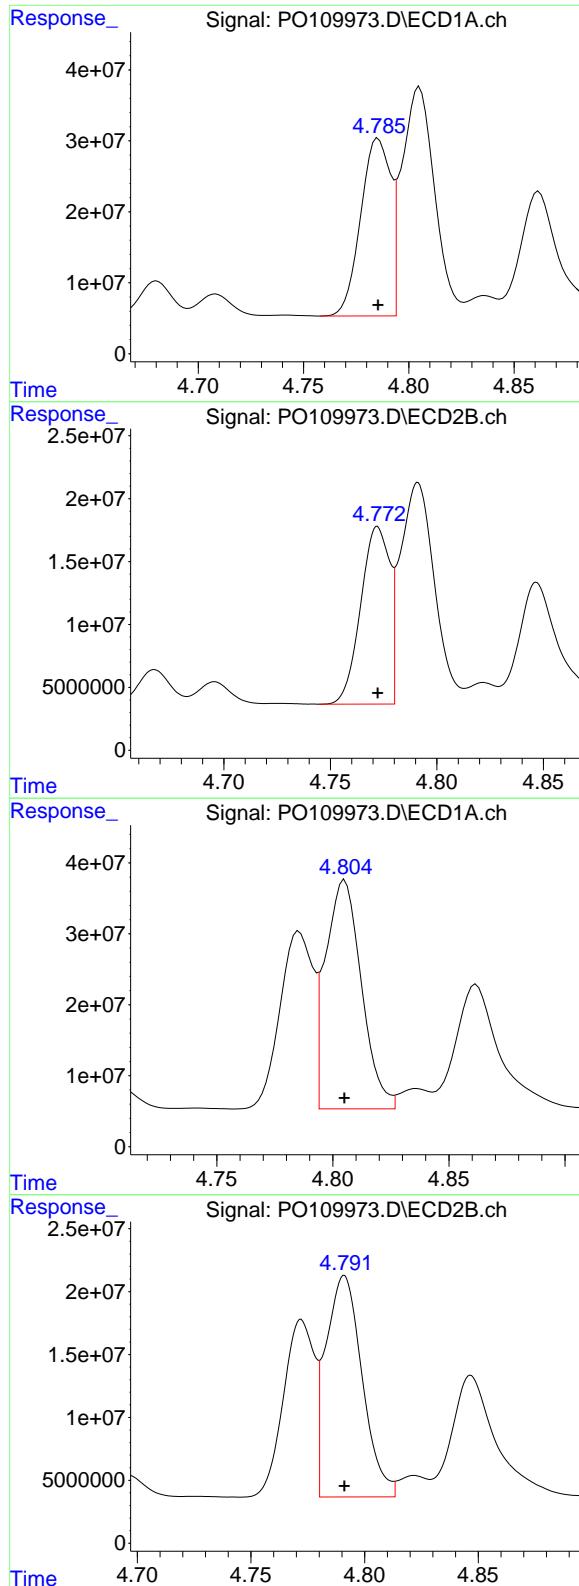

#3 AR-1016-1

R.T.: 4.785 min  
 Delta R.T.: 0.000 min  
 Response: 246831835  
 Conc: 747.92 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660ICC750

#3 AR-1016-1


R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 133795284  
 Conc: 745.96 ng/ml

#4 AR-1016-2

R.T.: 4.805 min  
 Delta R.T.: 0.000 min  
 Response: 347782380  
 Conc: 753.17 ng/ml

#4 AR-1016-2

R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 195632208  
 Conc: 750.68 ng/ml

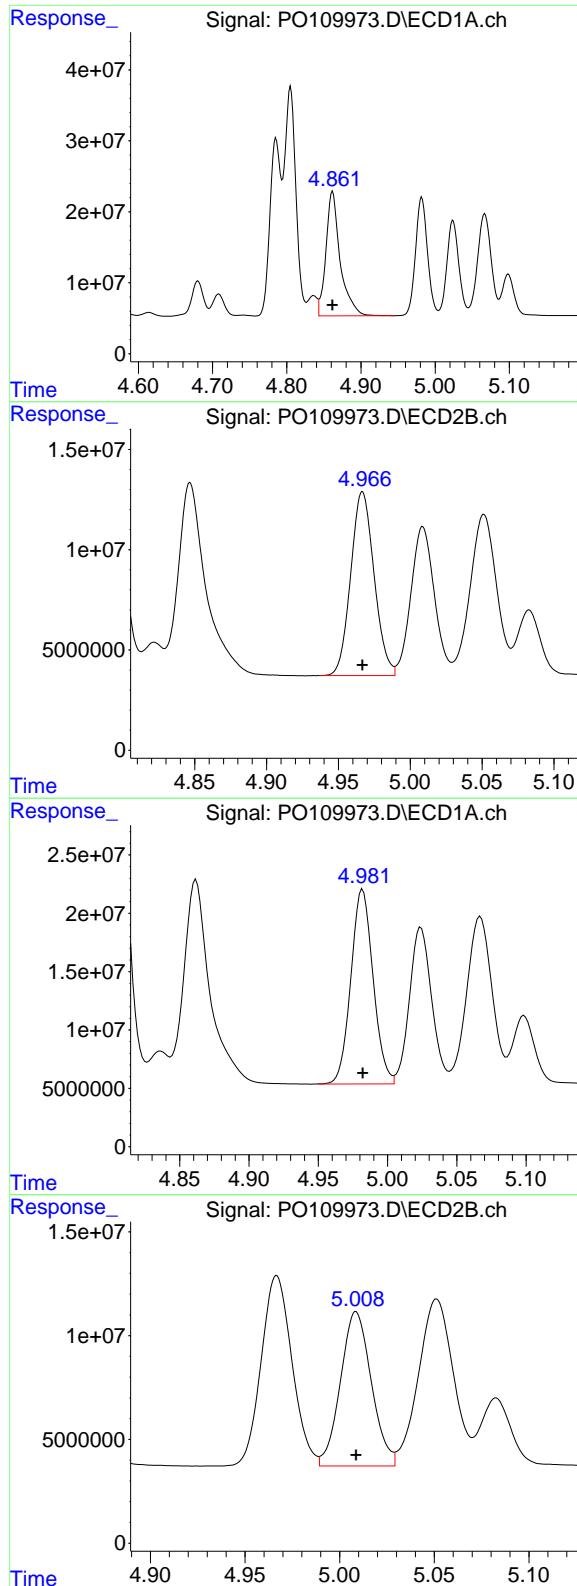

#5 AR-1016-3

R.T.: 4.862 min  
 Delta R.T.: 0.000 min  
 Response: 233678232  
 Conc: 751.39 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660ICC750

#5 AR-1016-3


R.T.: 4.967 min  
 Delta R.T.: 0.000 min  
 Response: 103988837  
 Conc: 748.10 ng/ml

#6 AR-1016-4

R.T.: 4.982 min  
 Delta R.T.: 0.000 min  
 Response: 186394664  
 Conc: 751.64 ng/ml

#6 AR-1016-4

R.T.: 5.009 min  
 Delta R.T.: 0.000 min  
 Response: 84297055  
 Conc: 746.61 ng/ml

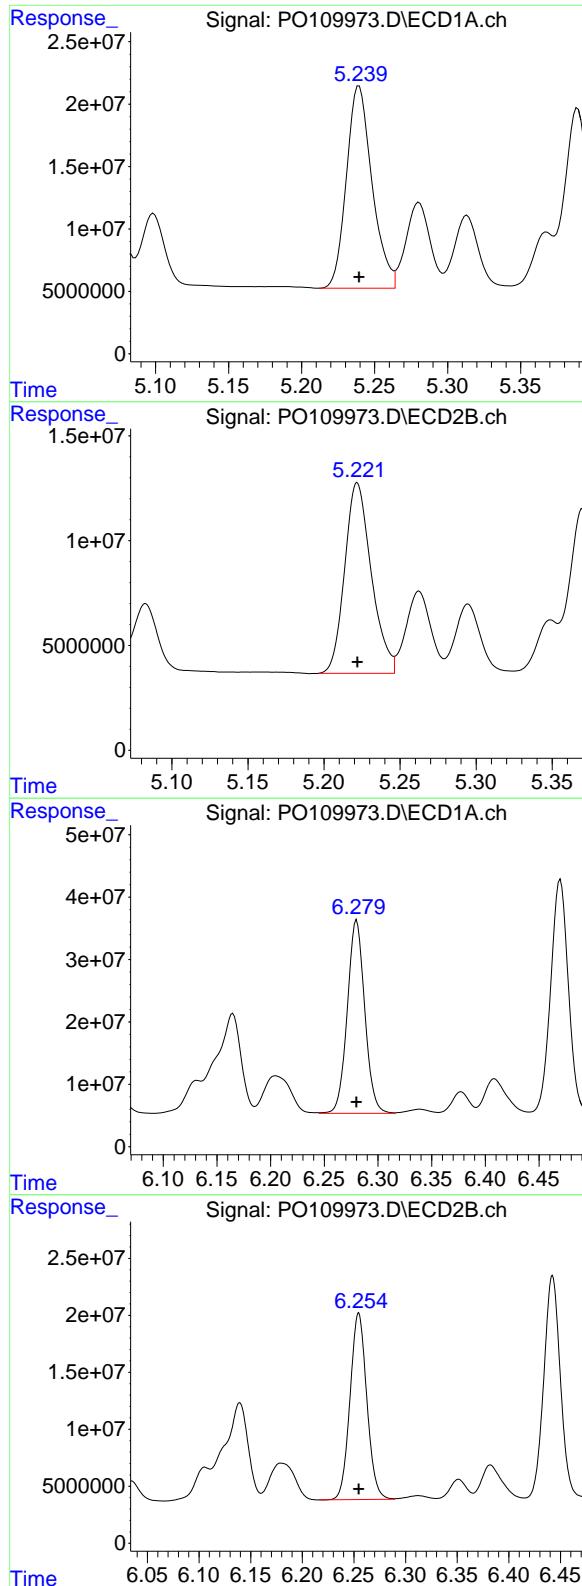

#7 AR-1016-5

R.T.: 5.239 min  
 Delta R.T.: 0.000 min  
 Response: 197756047  
 Conc: 753.93 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660ICC750

#7 AR-1016-5


R.T.: 5.222 min  
 Delta R.T.: 0.000 min  
 Response: 110764402  
 Conc: 750.26 ng/ml

#31 AR-1260-1

R.T.: 6.280 min  
 Delta R.T.: 0.000 min  
 Response: 350689884  
 Conc: 755.82 ng/ml

#31 AR-1260-1

R.T.: 6.255 min  
 Delta R.T.: 0.000 min  
 Response: 185810579  
 Conc: 746.57 ng/ml

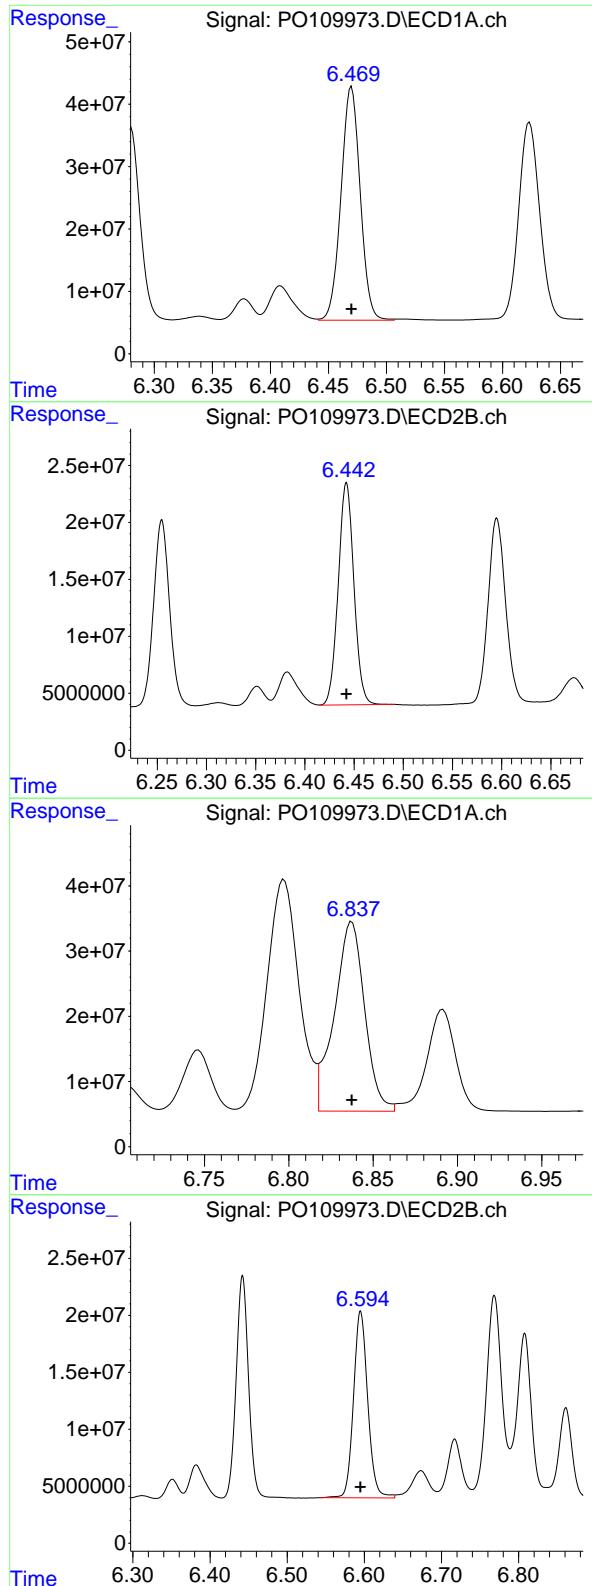

#32 AR-1260-2

R.T.: 6.470 min  
 Delta R.T.: 0.000 min  
 Response: 429776784  
 Conc: 759.62 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC750

#32 AR-1260-2


R.T.: 6.442 min  
 Delta R.T.: 0.000 min  
 Response: 216749564  
 Conc: 745.67 ng/ml

#33 AR-1260-3

R.T.: 6.837 min  
 Delta R.T.: 0.000 min  
 Response: 362605874  
 Conc: 757.41 ng/ml

#33 AR-1260-3

R.T.: 6.595 min  
 Delta R.T.: 0.000 min  
 Response: 209216211  
 Conc: 751.59 ng/ml

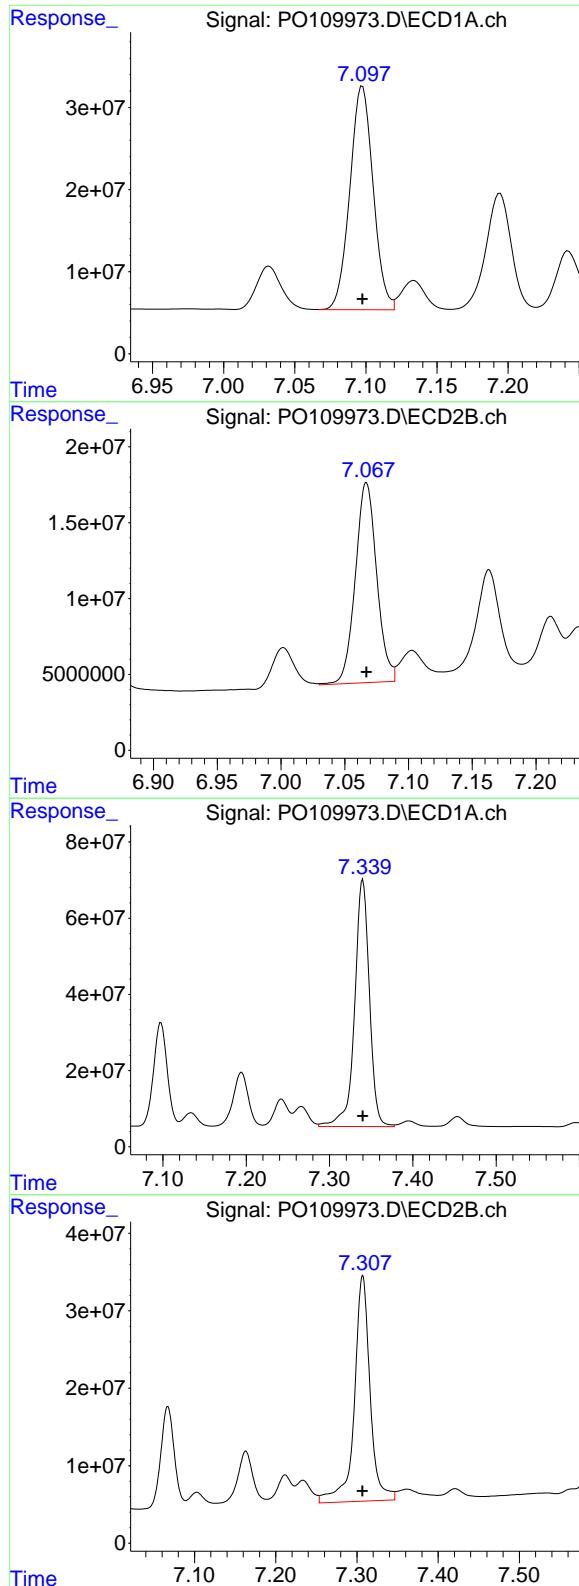

#34 AR-1260-4

R.T.: 7.098 min  
 Delta R.T.: 0.000 min  
 Response: 310296283  
 Conc: 751.25 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660ICC750

#34 AR-1260-4

R.T.: 7.067 min  
 Delta R.T.: 0.000 min  
 Response: 154008109  
 Conc: 745.58 ng/ml

#35 AR-1260-5

R.T.: 7.340 min  
 Delta R.T.: 0.000 min  
 Response: 800891670  
 Conc: 755.15 ng/ml

#35 AR-1260-5

R.T.: 7.307 min  
 Delta R.T.: 0.000 min  
 Response: 394605629  
 Conc: 803.09 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109976.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 15:16  
 Operator : YP/AJ  
 Sample : AR1660ICC050  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:42:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.688	39998137	22828400	4.395	4.353
2) SA Decachlor...	8.744	8.695	38817794	12425222	5.049	5.121

Target Compounds

3) L1 AR-1016-1	4.784	4.771	16902653	9160493	50.224	49.988
4) L1 AR-1016-2	4.804	4.790	22043406	12469957	47.540	47.685
5) L1 AR-1016-3	4.860	4.965	16411868	7085785	51.193	49.978
6) L1 AR-1016-4	4.981	5.008	12569483	6253080	49.743	53.024
7) L1 AR-1016-5	5.238	5.220	14890720	7955288	54.174	52.023
31) L7 AR-1260-1	6.279	6.253	27190975	14406182	57.396	56.300
32) L7 AR-1260-2	6.468	6.441	33768251	15676301	56.704	52.205
33) L7 AR-1260-3	6.836	6.594	24202394	18027606	49.871	62.952 #
34) L7 AR-1260-4	7.096	7.065	21433117	11320638	50.530	52.635
35) L7 AR-1260-5	7.339	7.306	47957612	24758089	45.855	49.646



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109976.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 15:16  
 Operator : YP/AJ  
 Sample : AR1660ICC050  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 16:42:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 16:30:31 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

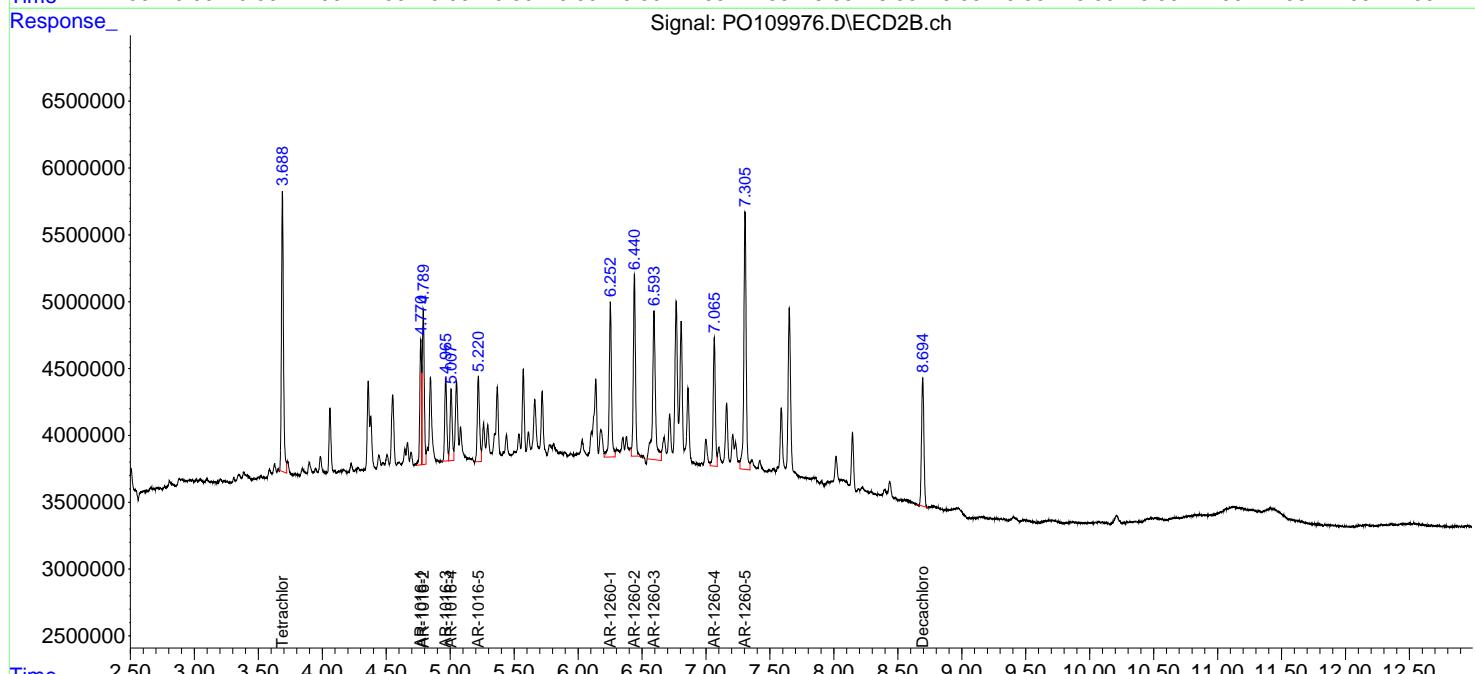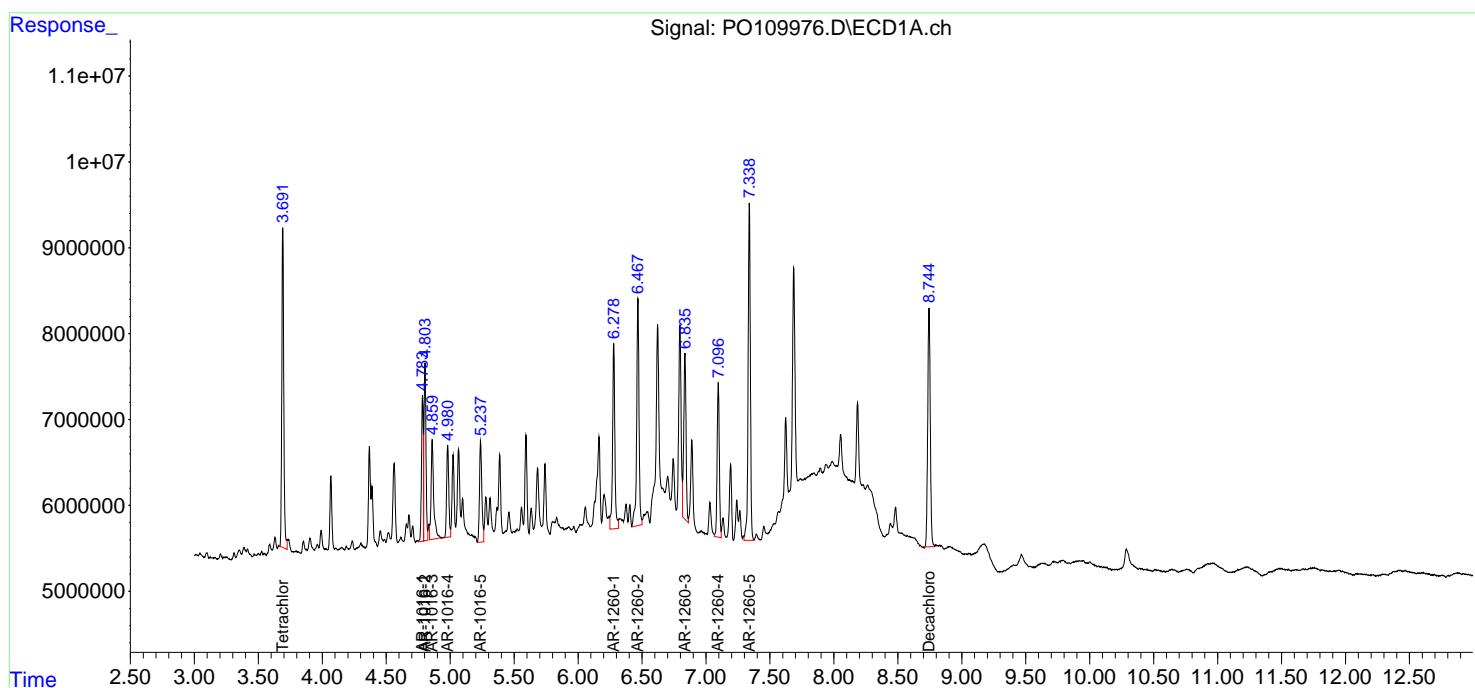


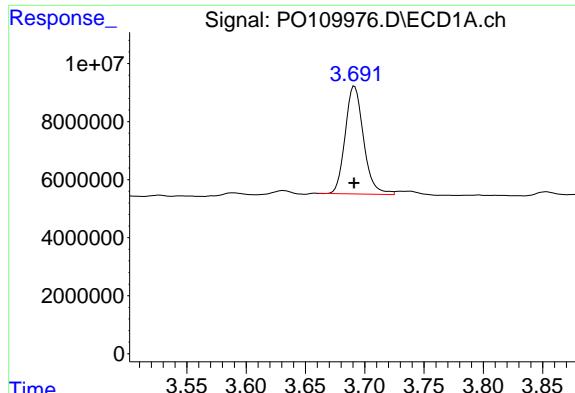

#1 Tetrachloro-m-xylene


R.T.: 3.691 min  
Delta R.T.: 0.000 min  
Response: 39998137  
Conc: 4.39 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1660ICC050

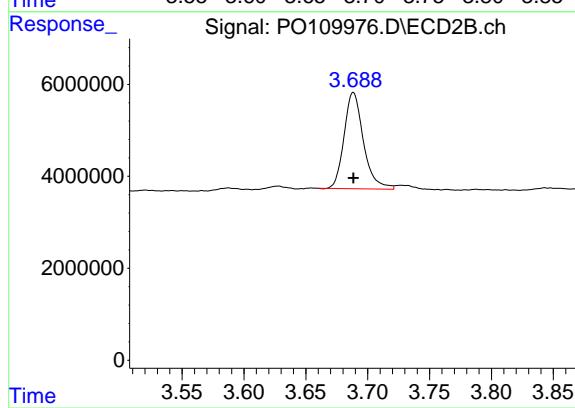


#1 Tetrachloro-m-xylene

R.T.: 3.688 min  
Delta R.T.: 0.000 min  
Response: 22828400  
Conc: 4.35 ng/ml

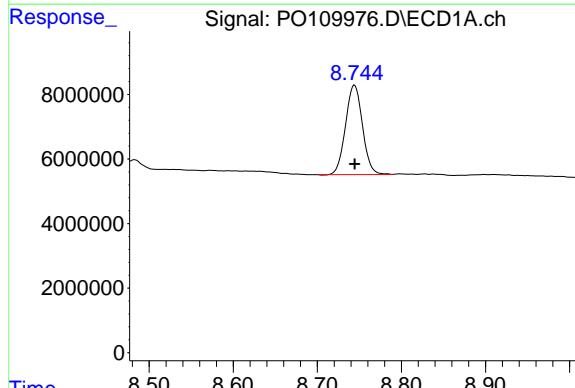


#2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 38817794  
Conc: 5.05 ng/ml

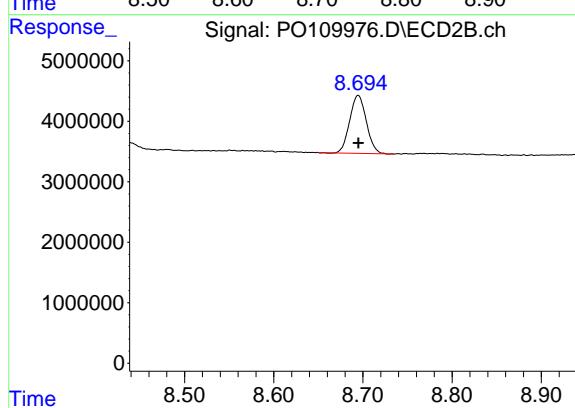

#2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 12425222  
Conc: 5.12 ng/ml

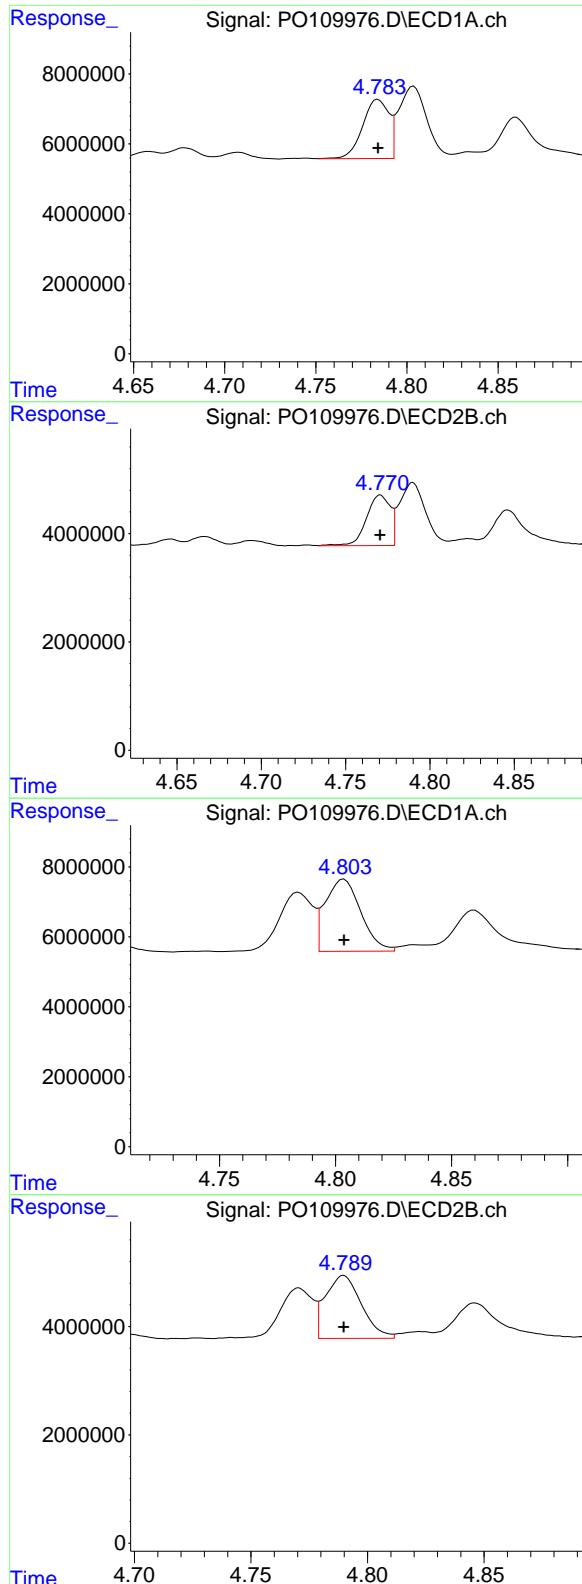

#3 AR-1016-1

R.T.: 4.784 min  
Delta R.T.: 0.000 min **Instrument:**  
Response: 16902653 ECD\_O  
Conc: 50.22 ng/ml **ClientSampleId:**  
AR1660ICC050

#3 AR-1016-1


R.T.: 4.771 min  
Delta R.T.: 0.000 min  
Response: 9160493  
Conc: 49.99 ng/ml

#4 AR-1016-2

R.T.: 4.804 min  
Delta R.T.: 0.000 min  
Response: 22043406  
Conc: 47.54 ng/ml

#4 AR-1016-2

R.T.: 4.790 min  
Delta R.T.: 0.000 min  
Response: 12469957  
Conc: 47.69 ng/ml

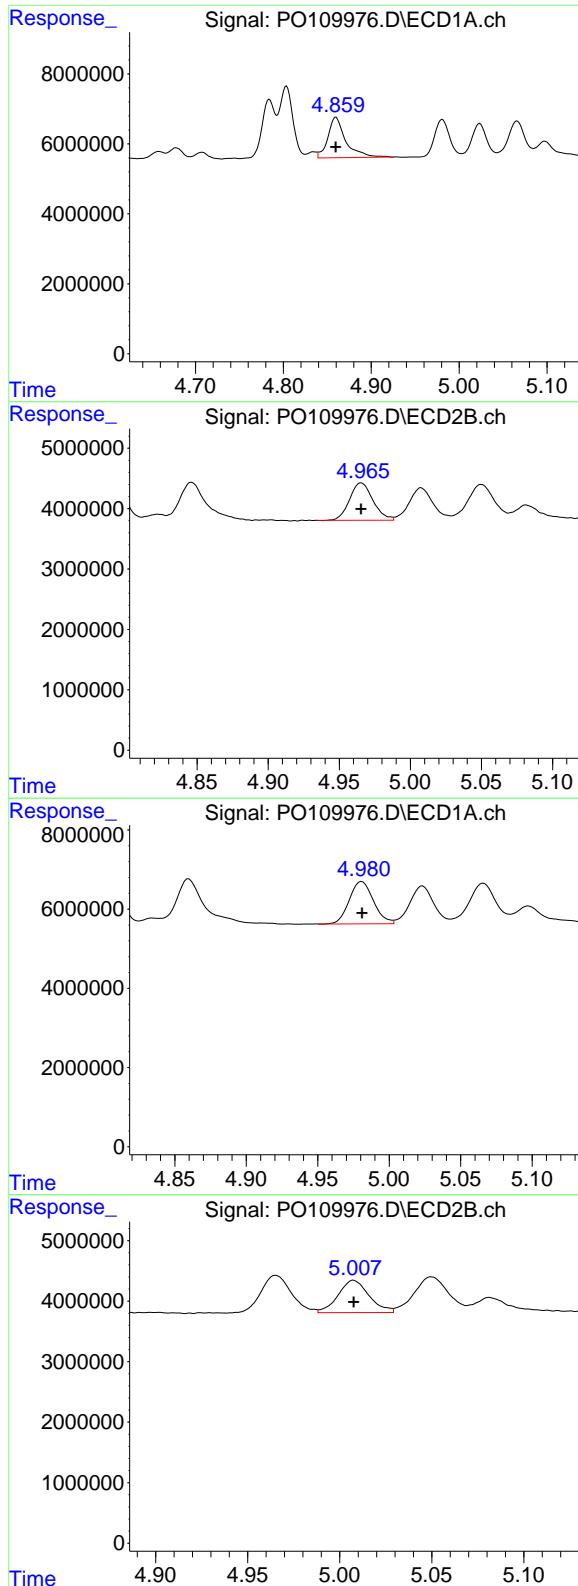

#5 AR-1016-3

R.T.: 4.860 min  
 Delta R.T.: 0.000 min  
 Response: 16411868  
 Conc: 51.19 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660ICC050

#5 AR-1016-3


R.T.: 4.965 min  
 Delta R.T.: 0.000 min  
 Response: 7085785  
 Conc: 49.98 ng/ml

#6 AR-1016-4

R.T.: 4.981 min  
 Delta R.T.: 0.000 min  
 Response: 12569483  
 Conc: 49.74 ng/ml

#6 AR-1016-4

R.T.: 5.008 min  
 Delta R.T.: 0.000 min  
 Response: 6253080  
 Conc: 53.02 ng/ml

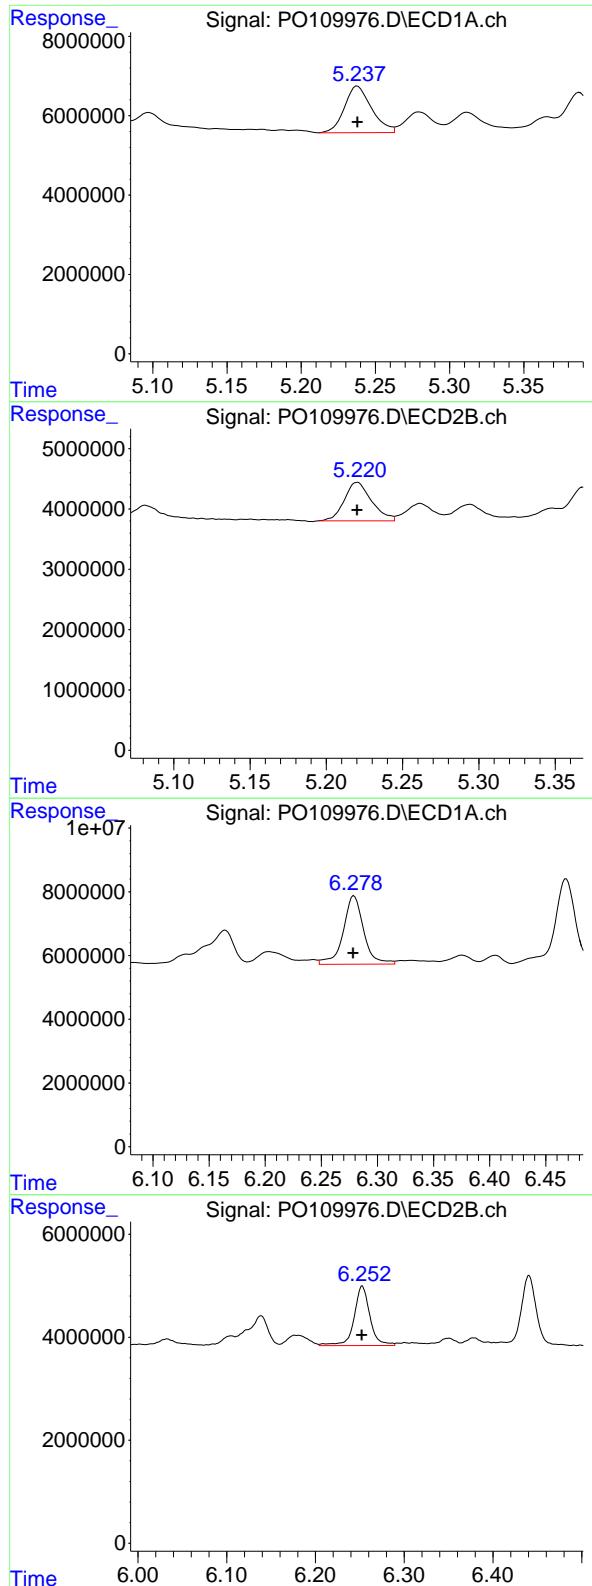

#7 AR-1016-5

R.T.: 5.238 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 14890720 ECD\_O  
 Conc: 54.17 ng/ml **ClientSampleId:**  
 AR1660ICC050

#7 AR-1016-5


R.T.: 5.220 min  
 Delta R.T.: 0.000 min  
 Response: 7955288  
 Conc: 52.02 ng/ml

#31 AR-1260-1

R.T.: 6.279 min  
 Delta R.T.: 0.000 min  
 Response: 27190975  
 Conc: 57.40 ng/ml

#31 AR-1260-1

R.T.: 6.253 min  
 Delta R.T.: 0.000 min  
 Response: 14406182  
 Conc: 56.30 ng/ml

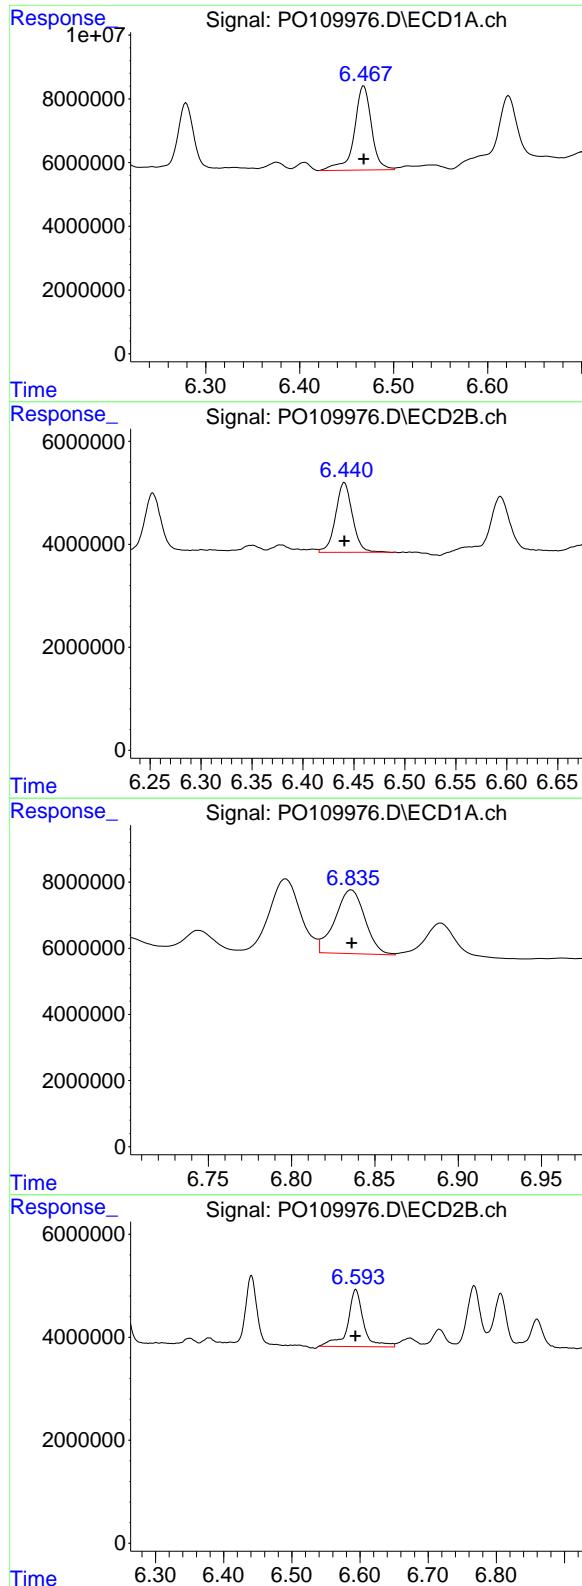

#32 AR-1260-2

R.T.: 6.468 min  
 Delta R.T.: 0.000 min  
 Response: 33768251  
 Conc: 56.70 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660ICC050

#32 AR-1260-2


R.T.: 6.441 min  
 Delta R.T.: 0.000 min  
 Response: 15676301  
 Conc: 52.20 ng/ml

#33 AR-1260-3

R.T.: 6.836 min  
 Delta R.T.: 0.000 min  
 Response: 24202394  
 Conc: 49.87 ng/ml

#33 AR-1260-3

R.T.: 6.594 min  
 Delta R.T.: 0.000 min  
 Response: 18027606  
 Conc: 62.95 ng/ml

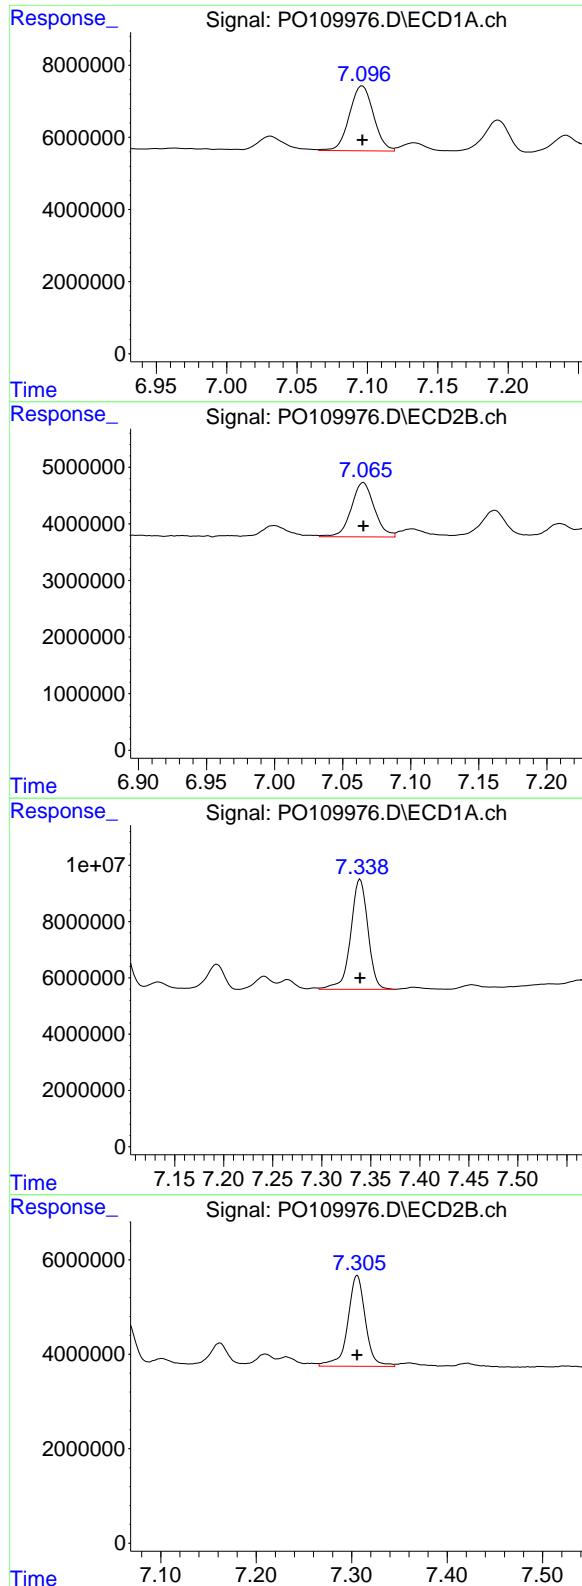

#34 AR-1260-4

R.T.: 7.096 min  
 Delta R.T.: 0.000 min  
 Response: 21433117  
 Conc: 50.53 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660ICC050

#34 AR-1260-4

R.T.: 7.065 min  
 Delta R.T.: 0.000 min  
 Response: 11320638  
 Conc: 52.63 ng/ml

#35 AR-1260-5

R.T.: 7.339 min  
 Delta R.T.: 0.000 min  
 Response: 47957612  
 Conc: 45.86 ng/ml

#35 AR-1260-5

R.T.: 7.306 min  
 Delta R.T.: 0.000 min  
 Response: 24758089  
 Conc: 49.65 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109983.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 17:25  
 Operator : YP/AJ  
 Sample : AR1242ICC050  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1242ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:34:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 17:34:29 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	27043743	15260251	3.233	3.182
2) SA Decachlor...	8.744	8.696	32408304	10337597	4.500	4.624

Target Compounds

16) L4 AR-1242-1	4.784	4.772	12333502	6612130	46.123	45.222
17) L4 AR-1242-2	4.804	4.791	16261465	8959332	44.164	43.066
18) L4 AR-1242-3	4.859	4.967	12804073	4612927	49.638	41.322
19) L4 AR-1242-4	4.981	5.051	8657409	5726073	43.398	49.373
20) L4 AR-1242-5	5.634	5.572	14229681	8157544	67.609	59.247



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109983.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 17:25  
 Operator : YP/AJ  
 Sample : AR1242ICC050  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1242ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 17:34:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 18 17:34:29 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

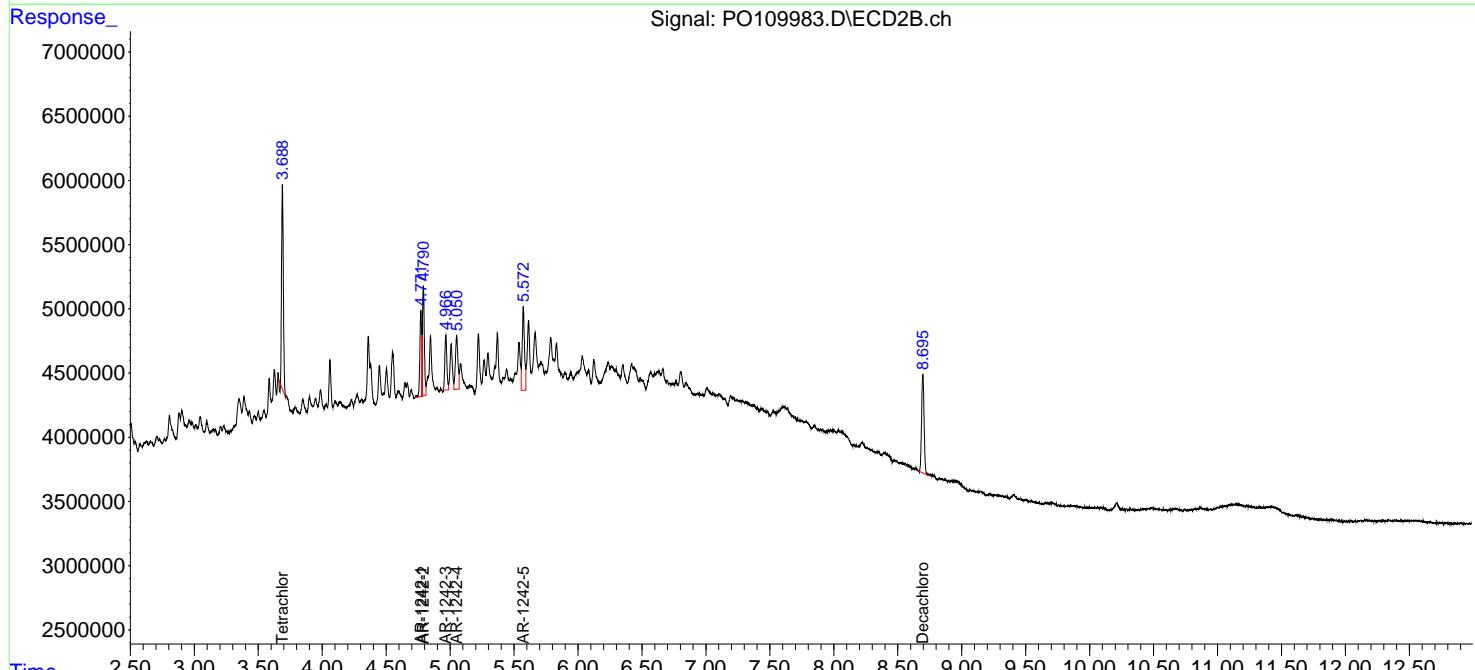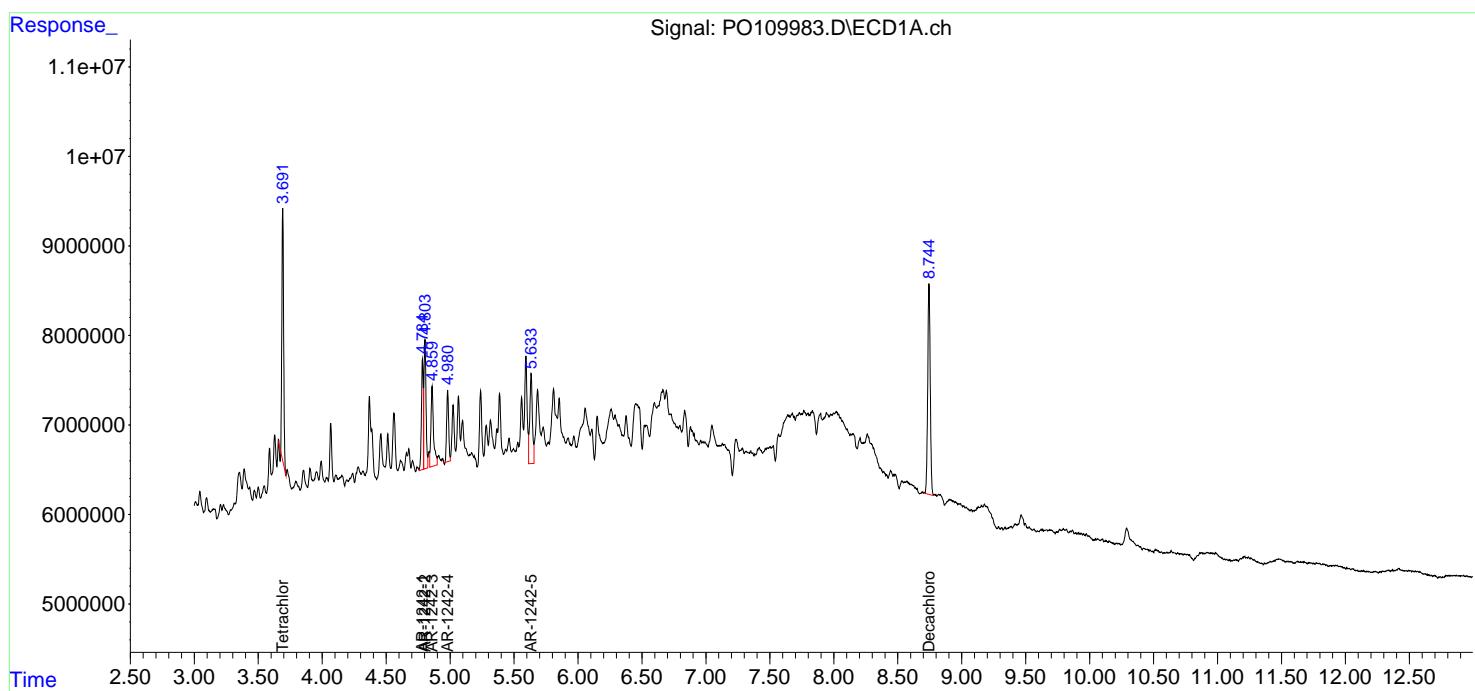

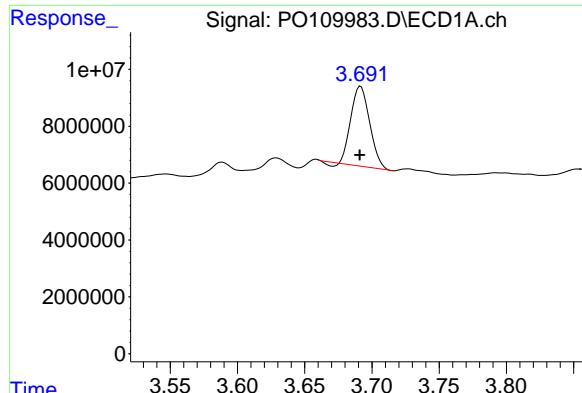


#1 Tetrachloro-m-xylene  
R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 27043743  
Conc: 3.23 ng/ml


Instrument: ECD\_O  
ClientSampleId: AR1242ICC050

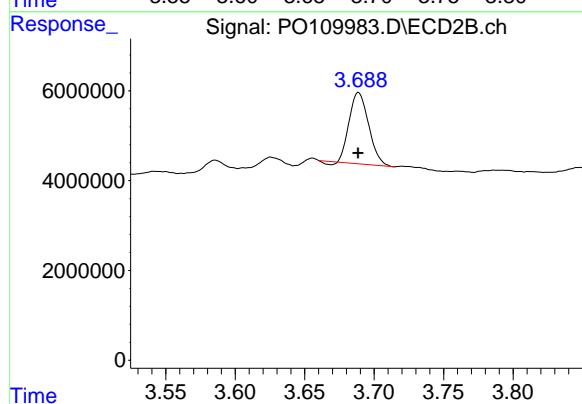


#1 Tetrachloro-m-xylene  
R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 15260251  
Conc: 3.18 ng/ml

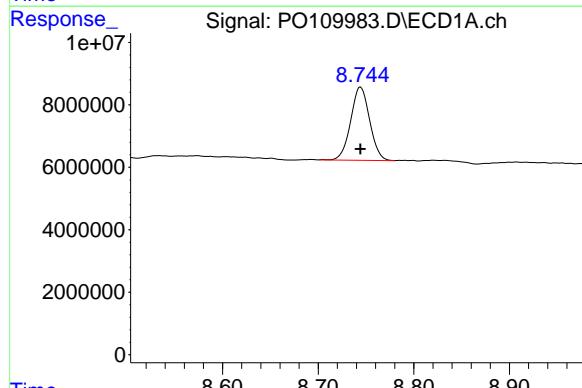

#2 Decachlorobiphenyl  
R.T.: 8.744 min  
Delta R.T.: 0.000 min  
Response: 32408304  
Conc: 4.50 ng/ml

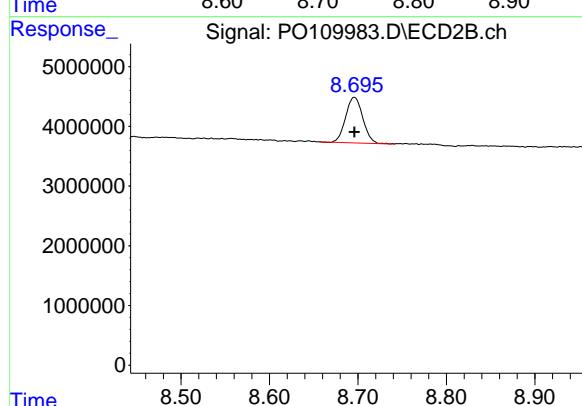

#2 Decachlorobiphenyl  
R.T.: 8.696 min  
Delta R.T.: 0.000 min  
Response: 10337597  
Conc: 4.62 ng/ml

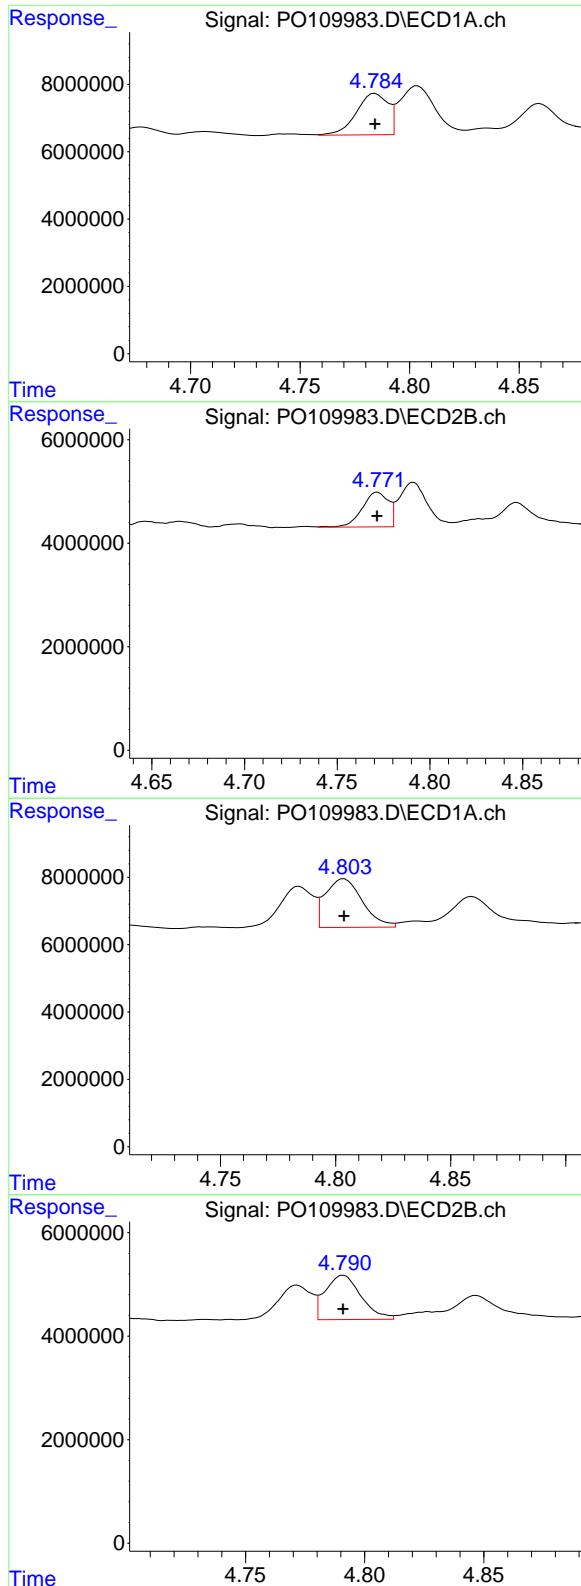

#16 AR-1242-1

R.T.: 4.784 min  
 Delta R.T.: 0.000 min  
 Response: 12333502  
 Conc: 46.12 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1242ICC050

#16 AR-1242-1


R.T.: 4.772 min  
 Delta R.T.: 0.000 min  
 Response: 6612130  
 Conc: 45.22 ng/ml

#17 AR-1242-2

R.T.: 4.804 min  
 Delta R.T.: 0.000 min  
 Response: 16261465  
 Conc: 44.16 ng/ml

#17 AR-1242-2


R.T.: 4.791 min  
 Delta R.T.: 0.000 min  
 Response: 8959332  
 Conc: 43.07 ng/ml

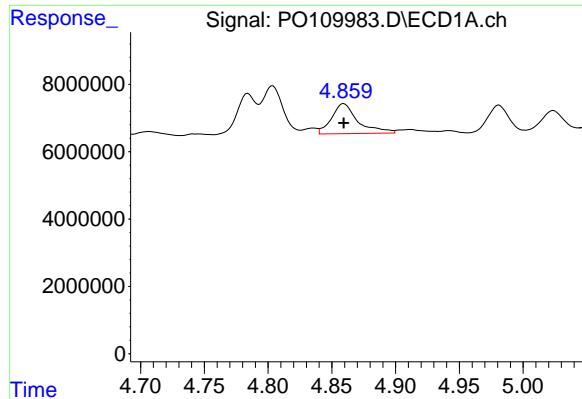

#18 AR-1242-3


R.T.: 4.859 min  
Delta R.T.: 0.000 min  
Response: 12804073  
Conc: 49.64 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1242ICC050

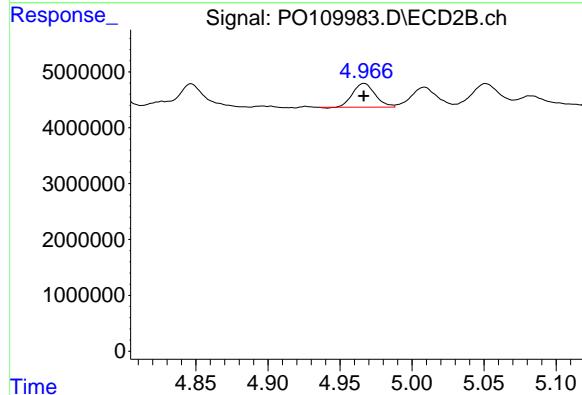


#18 AR-1242-3

R.T.: 4.967 min  
Delta R.T.: 0.000 min  
Response: 4612927  
Conc: 41.32 ng/ml

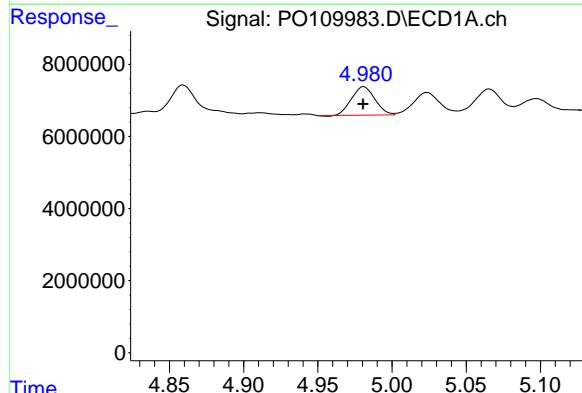


#19 AR-1242-4

R.T.: 4.981 min  
Delta R.T.: 0.000 min  
Response: 8657409  
Conc: 43.40 ng/ml

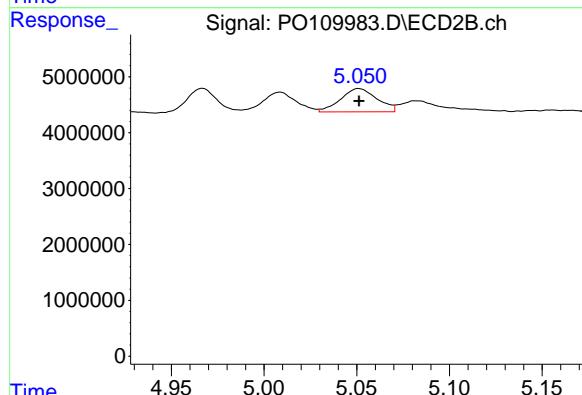

#19 AR-1242-4

R.T.: 5.051 min  
Delta R.T.: 0.000 min  
Response: 5726073  
Conc: 49.37 ng/ml

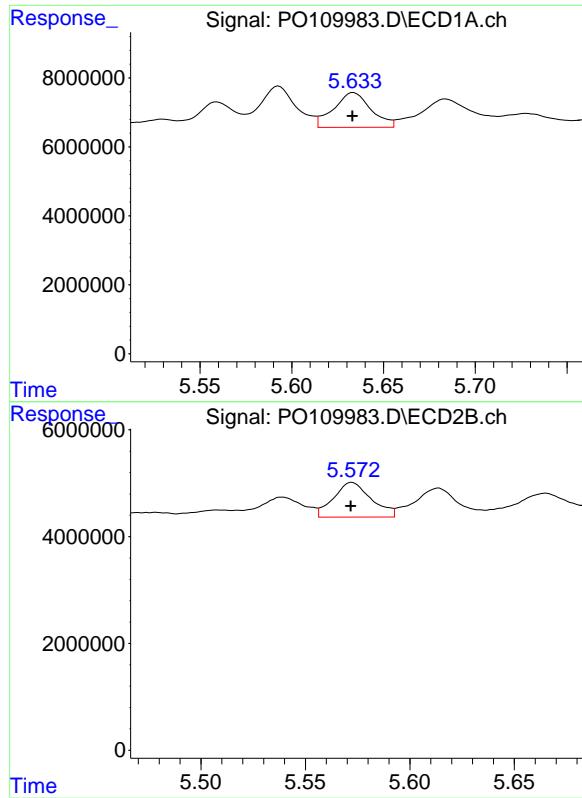

#20 AR-1242-5

R.T.: 5.634 min  
Delta R.T.: 0.000 min  
Response: 14229681  
Conc: 67.61 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1242ICC050

#20 AR-1242-5

R.T.: 5.572 min  
Delta R.T.: 0.000 min  
Response: 8157544  
Conc: 59.25 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109988.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:54  
 Operator : YP/AJ  
 Sample : AR1248ICC050  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1248ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.690	3.689	43788277	25352976	4.721	4.788
2) SA Decachlor...	8.742	8.695	41310164	13029410	5.300	5.557

Target Compounds

21) L5 AR-1248-1	4.782	4.771	11846805	6686511	53.863	55.572
22) L5 AR-1248-2	5.021	5.008	16385888	9031427	54.426	53.593
23) L5 AR-1248-3	5.236	5.050	22145957	10026048	59.149	55.979
24) L5 AR-1248-4	5.591	5.221	29227773	12176632	55.856	58.382
25) L5 AR-1248-5	5.632	5.613	20545156	11669383	55.569	57.295



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109988.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 18:54  
 Operator : YP/AJ  
 Sample : AR1248ICC050  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1248ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:40:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:38:33 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

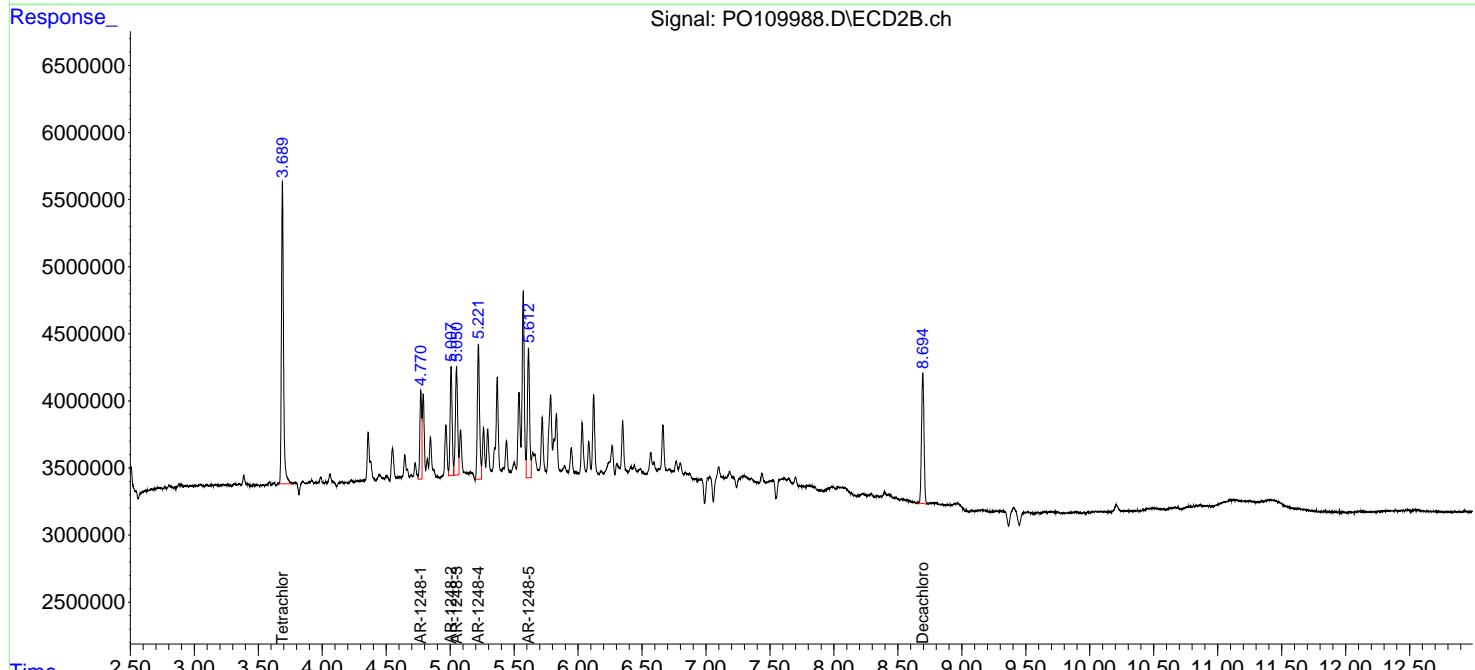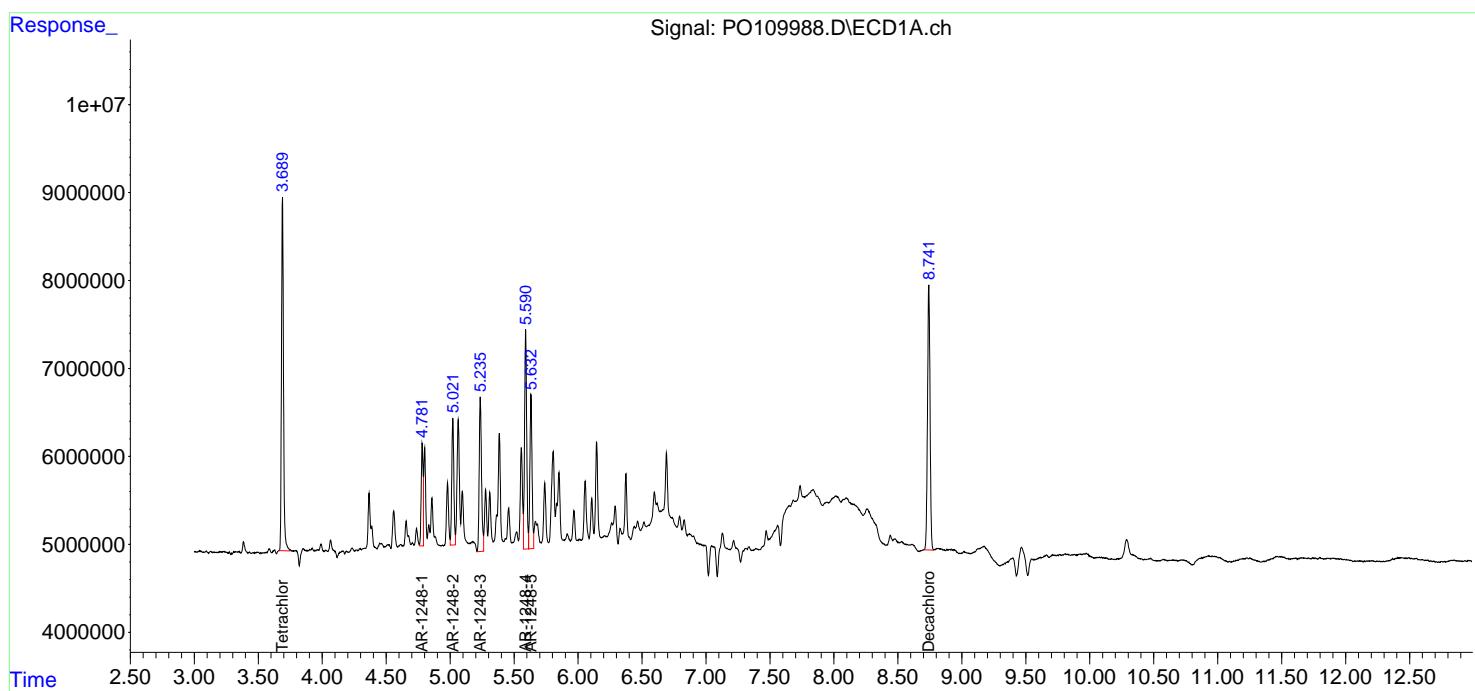

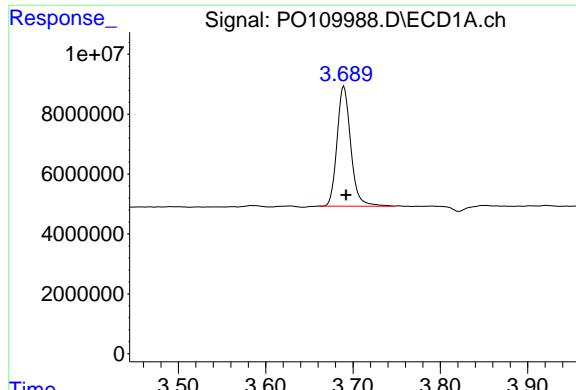

#1 Tetrachloro-m-xylene


R.T.: 3.690 min  
Delta R.T.: -0.002 min  
Response: 43788277  
Conc: 4.72 ng/ml

Instrument:

ECD\_O


ClientSampleId :

AR1248ICC050

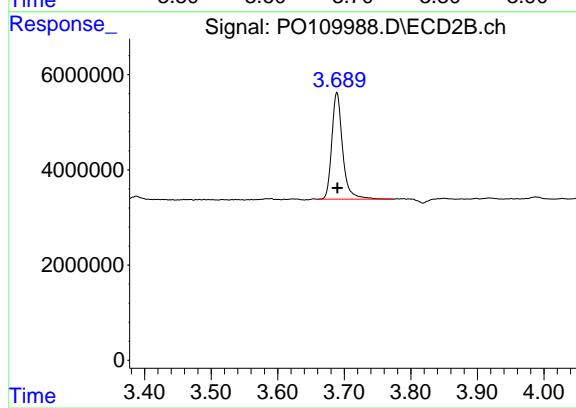


#1 Tetrachloro-m-xylene

R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 25352976  
Conc: 4.79 ng/ml

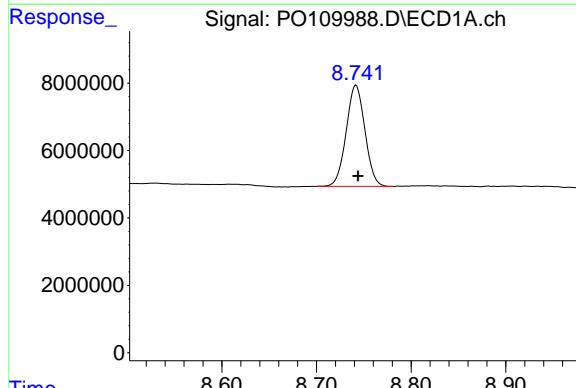


#2 Decachlorobiphenyl

R.T.: 8.742 min  
Delta R.T.: -0.002 min  
Response: 41310164  
Conc: 5.30 ng/ml

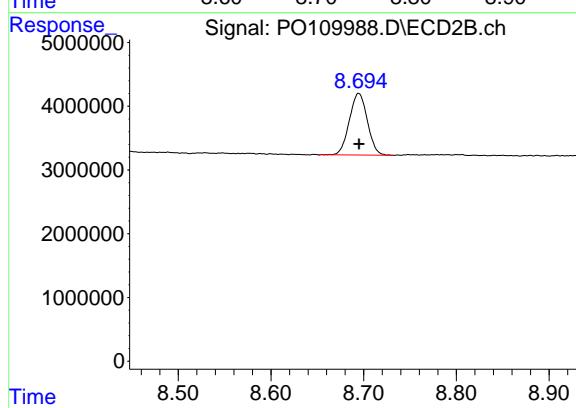

#2 Decachlorobiphenyl

R.T.: 8.695 min  
Delta R.T.: 0.000 min  
Response: 13029410  
Conc: 5.56 ng/ml

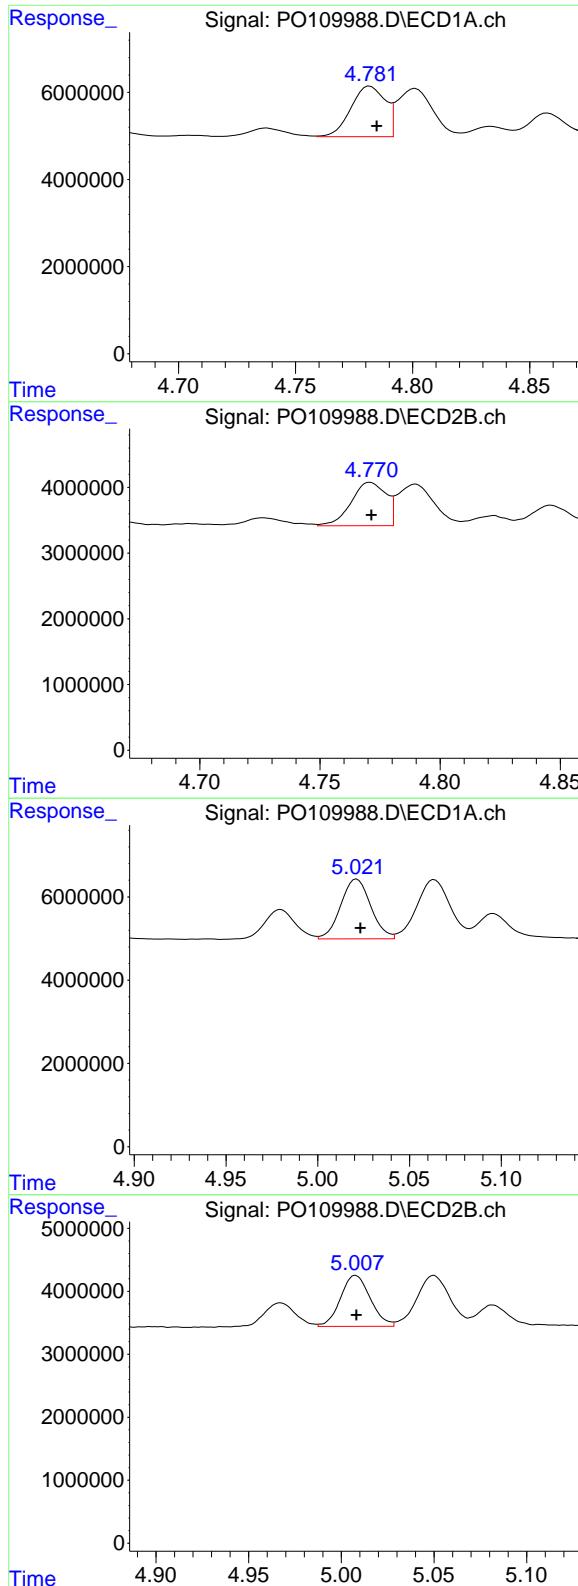

#21 AR-1248-1

R.T.: 4.782 min  
 Delta R.T.: -0.003 min  
 Response: 11846805  
 Conc: 53.86 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1248ICC050

#21 AR-1248-1


R.T.: 4.771 min  
 Delta R.T.: 0.000 min  
 Response: 6686511  
 Conc: 55.57 ng/ml

#22 AR-1248-2

R.T.: 5.021 min  
 Delta R.T.: -0.002 min  
 Response: 16385888  
 Conc: 54.43 ng/ml

#22 AR-1248-2

R.T.: 5.008 min  
 Delta R.T.: 0.000 min  
 Response: 9031427  
 Conc: 53.59 ng/ml

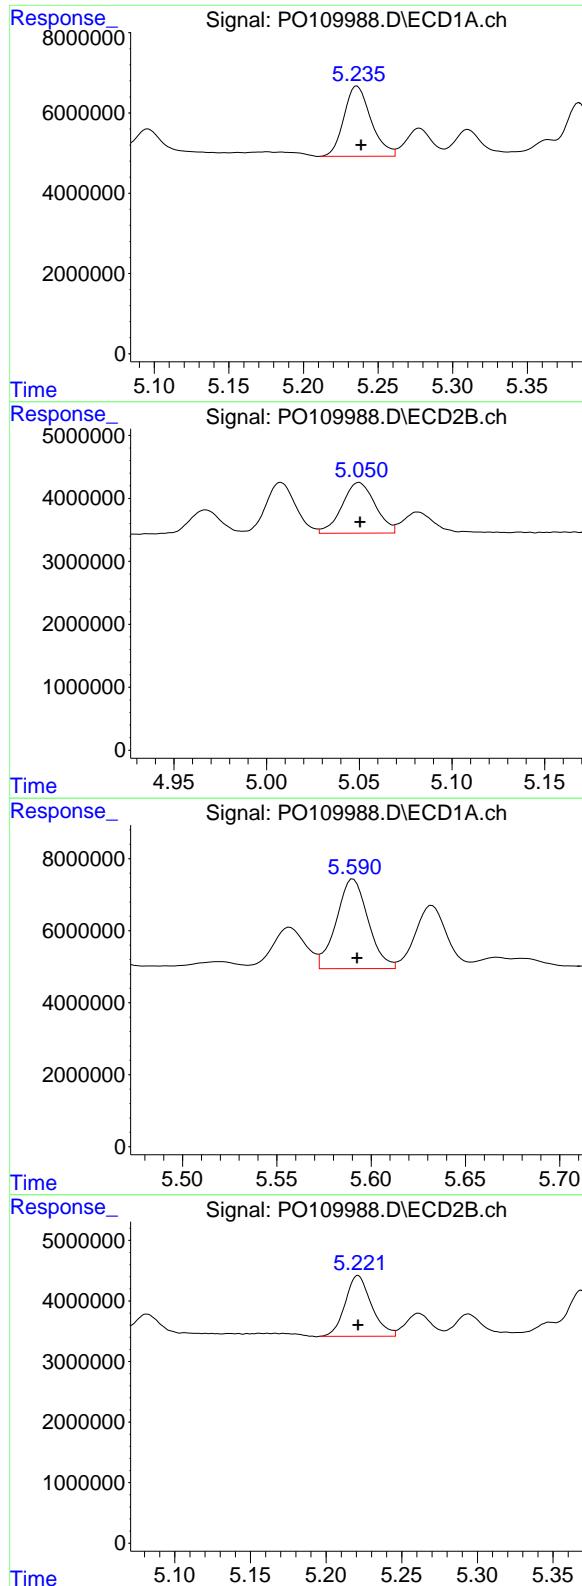

#23 AR-1248-3

R.T.: 5.236 min  
 Delta R.T.: -0.003 min  
 Response: 22145957  
 Conc: 59.15 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1248ICC050

#23 AR-1248-3


R.T.: 5.050 min  
 Delta R.T.: 0.000 min  
 Response: 10026048  
 Conc: 55.98 ng/ml

#24 AR-1248-4

R.T.: 5.591 min  
 Delta R.T.: -0.002 min  
 Response: 29227773  
 Conc: 55.86 ng/ml

#24 AR-1248-4

R.T.: 5.221 min  
 Delta R.T.: 0.000 min  
 Response: 12176632  
 Conc: 58.38 ng/ml

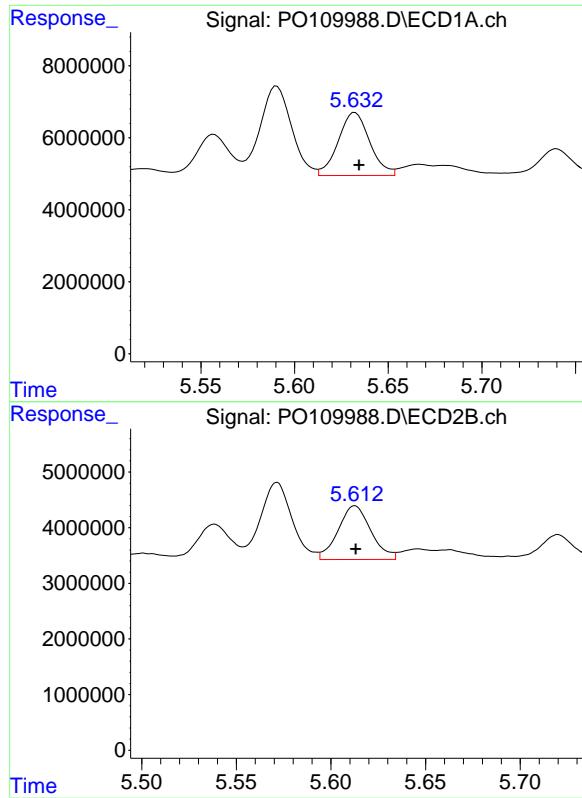

#25 AR-1248-5

R.T.: 5.632 min  
Delta R.T.: -0.002 min  
Response: 20545156  
Conc: 55.57 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1248ICC050

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109993.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 20:25  
 Operator : YP/AJ  
 Sample : AR1254ICC050  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1254ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:50:30 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	43445665	25306006	4.628	4.733
2) SA Decachlor...	8.743	8.694	41266656	13227136	5.245	5.469

Target Compounds

26) L6 AR-1254-1	5.593	5.573	31329450	17649915	56.014	57.357
27) L6 AR-1254-2	5.742	5.720	26381750	15388259	54.541	57.314
28) L6 AR-1254-3	6.148	6.123	39484048	21241930	50.026	50.431
29) L6 AR-1254-4	6.377	6.350	23571245	12628885	48.456	51.676
30) L6 AR-1254-5	6.797	6.768	28479203	19977415	41.849	57.297 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109993.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 20:25  
 Operator : YP/AJ  
 Sample : AR1254ICC050  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1254ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 01:50:30 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 01:48:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

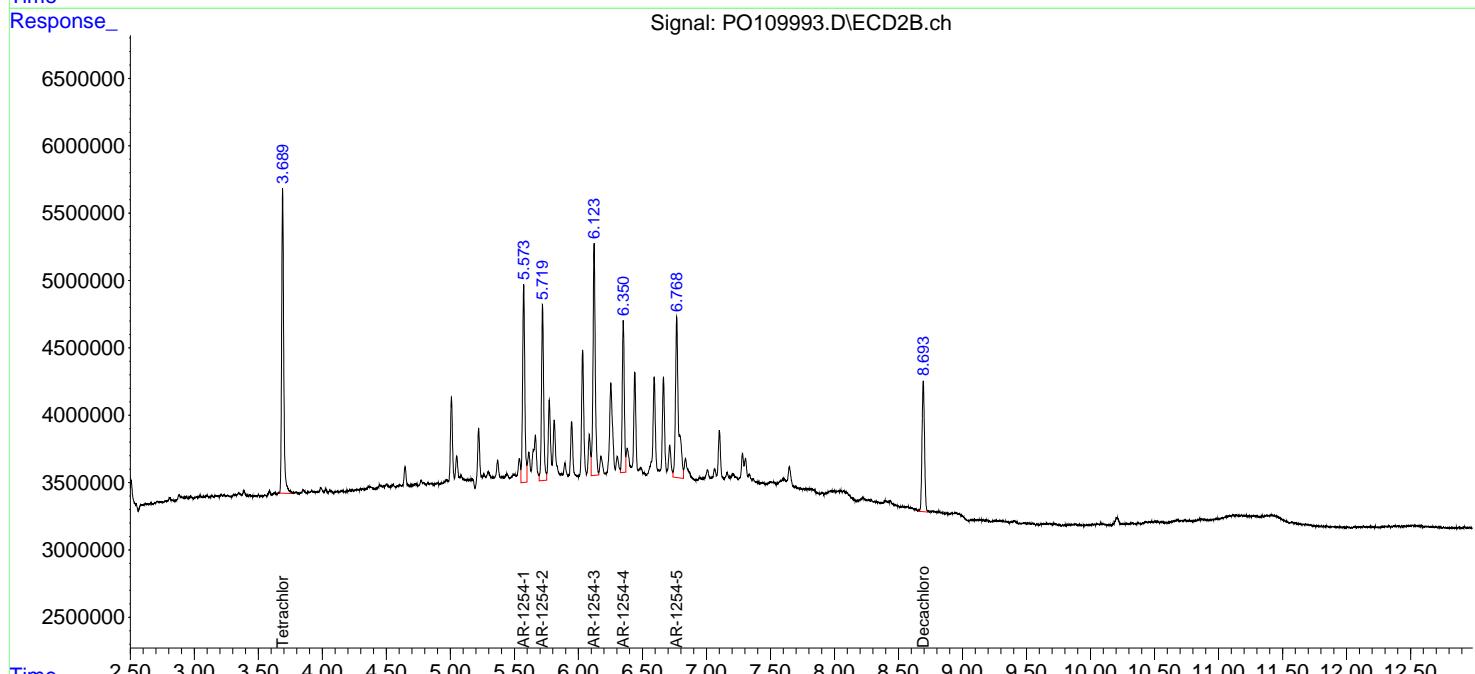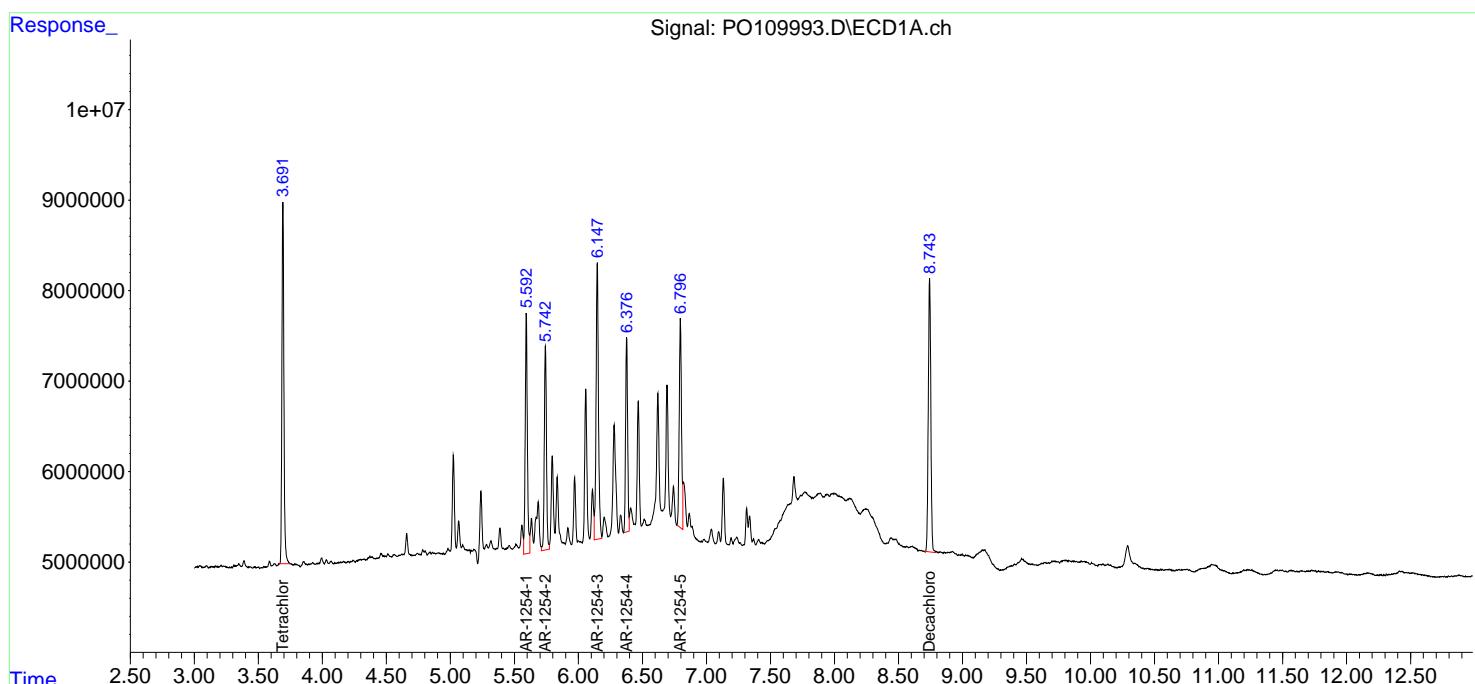

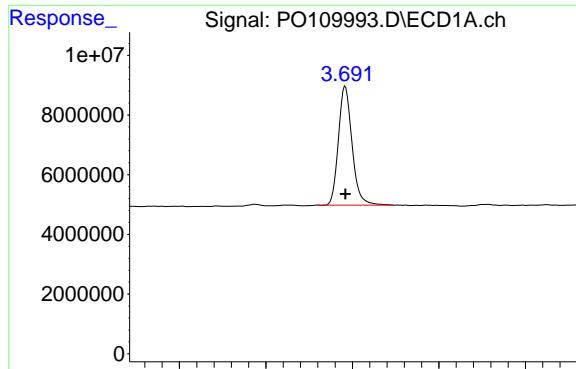


#1 Tetrachloro-m-xylene  
R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 43445665  
Conc: 4.63 ng/ml


Instrument: ECD\_O  
ClientSampleId: AR1254ICC050

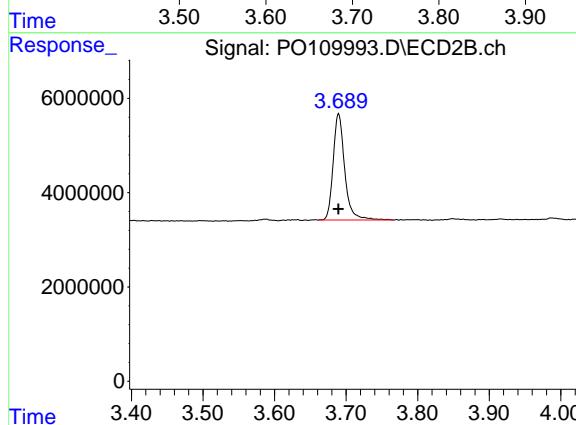


#1 Tetrachloro-m-xylene  
R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 25306006  
Conc: 4.73 ng/ml

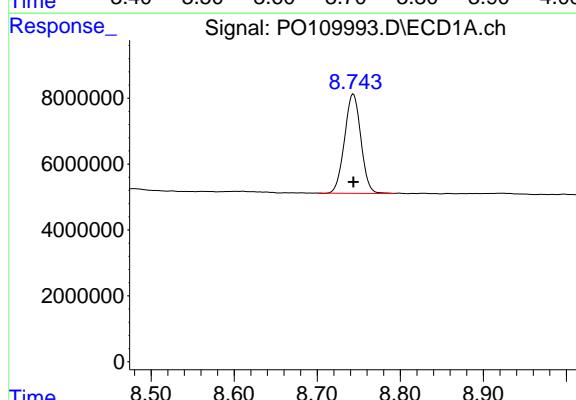

#2 Decachlorobiphenyl  
R.T.: 8.743 min  
Delta R.T.: 0.000 min  
Response: 41266656  
Conc: 5.25 ng/ml

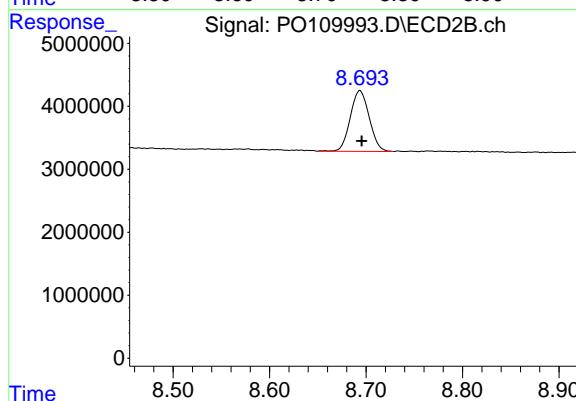

#2 Decachlorobiphenyl  
R.T.: 8.694 min  
Delta R.T.: -0.002 min  
Response: 13227136  
Conc: 5.47 ng/ml

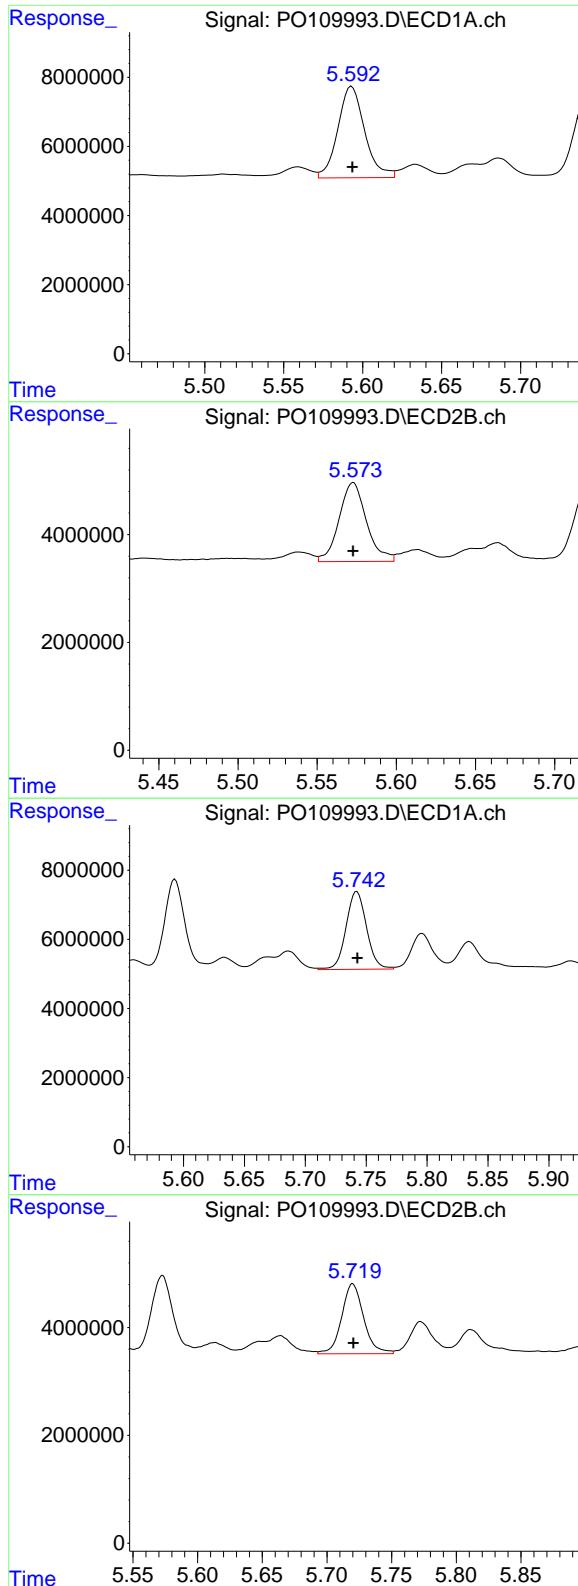

#26 AR-1254-1

R.T.: 5.593 min  
 Delta R.T.: 0.000 min  
 Response: 31329450  
 Conc: 56.01 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1254ICC050

#26 AR-1254-1


R.T.: 5.573 min  
 Delta R.T.: 0.000 min  
 Response: 17649915  
 Conc: 57.36 ng/ml

#27 AR-1254-2

R.T.: 5.742 min  
 Delta R.T.: 0.000 min  
 Response: 26381750  
 Conc: 54.54 ng/ml

#27 AR-1254-2


R.T.: 5.720 min  
 Delta R.T.: 0.000 min  
 Response: 15388259  
 Conc: 57.31 ng/ml



#28 AR-1254-3


R.T.: 6.148 min  
Delta R.T.: 0.000 min  
Response: 39484048  
Conc: 50.03 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1254ICC050

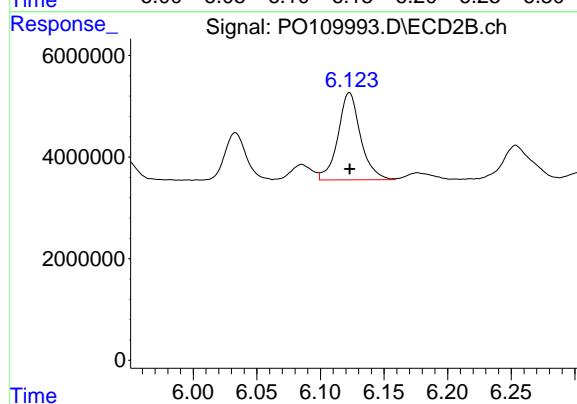


#28 AR-1254-3

R.T.: 6.123 min  
Delta R.T.: 0.000 min  
Response: 21241930  
Conc: 50.43 ng/ml

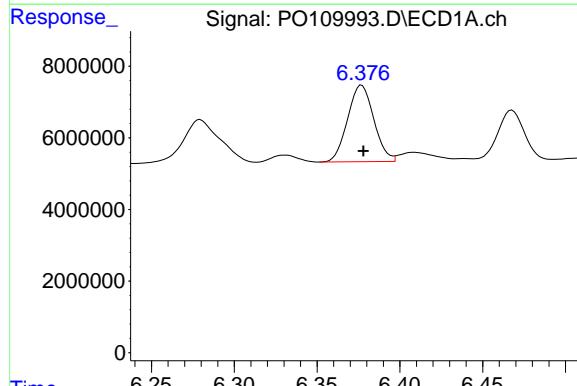


#29 AR-1254-4

R.T.: 6.377 min  
Delta R.T.: 0.000 min  
Response: 23571245  
Conc: 48.46 ng/ml

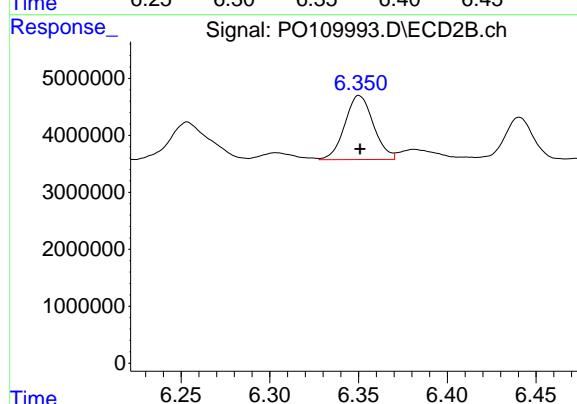

#29 AR-1254-4


R.T.: 6.350 min  
Delta R.T.: 0.000 min  
Response: 12628885  
Conc: 51.68 ng/ml

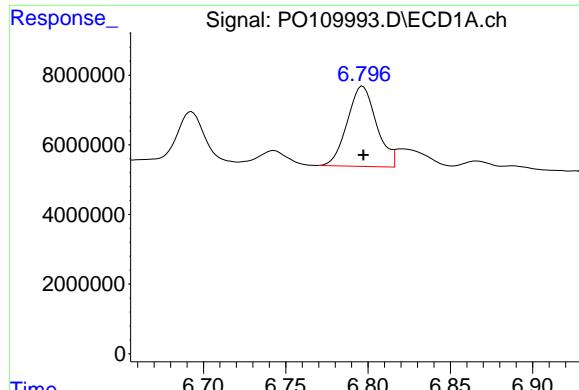

#30 AR-1254-5

R.T.: 6.797 min  
Delta R.T.: 0.000 min  
Response: 28479203  
Conc: 41.85 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1254ICC050

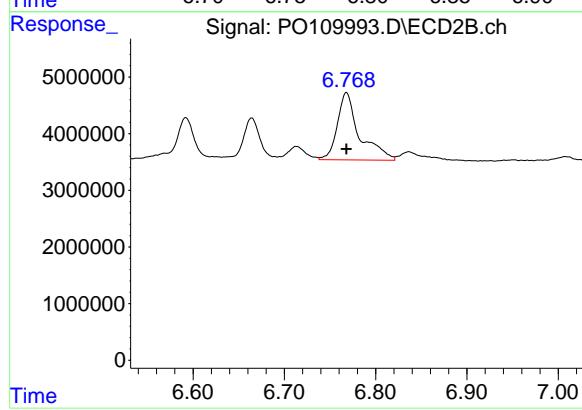

#30 AR-1254-5

R.T.: 6.768 min  
Delta R.T.: 0.000 min  
Response: 19977415  
Conc: 57.30 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109997.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:39  
 Operator : YP/AJ  
 Sample : AR1268ICC500  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1268ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.689	463.9E6	264.1E6	50.000	50.000
2) SA Decachlor...	8.743	8.694	706.0E6	207.2E6	50.000	50.000

Target Compounds

41) L9 AR-1268-1	7.623	7.589	699.8E6	289.1E6	498.680	500.000
42) L9 AR-1268-2	7.688	7.653	639.8E6	266.3E6	500.000	500.000
43) L9 AR-1268-3	7.896	7.861	519.3E6	206.5E6	500.000	500.000
44) L9 AR-1268-4	8.185	8.145	223.7E6	81011977	500.000	500.000
45) L9 AR-1268-5	8.482	8.439	1614.3E6	493.6E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109997.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:39  
 Operator : YP/AJ  
 Sample : AR1268ICC500  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1268ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

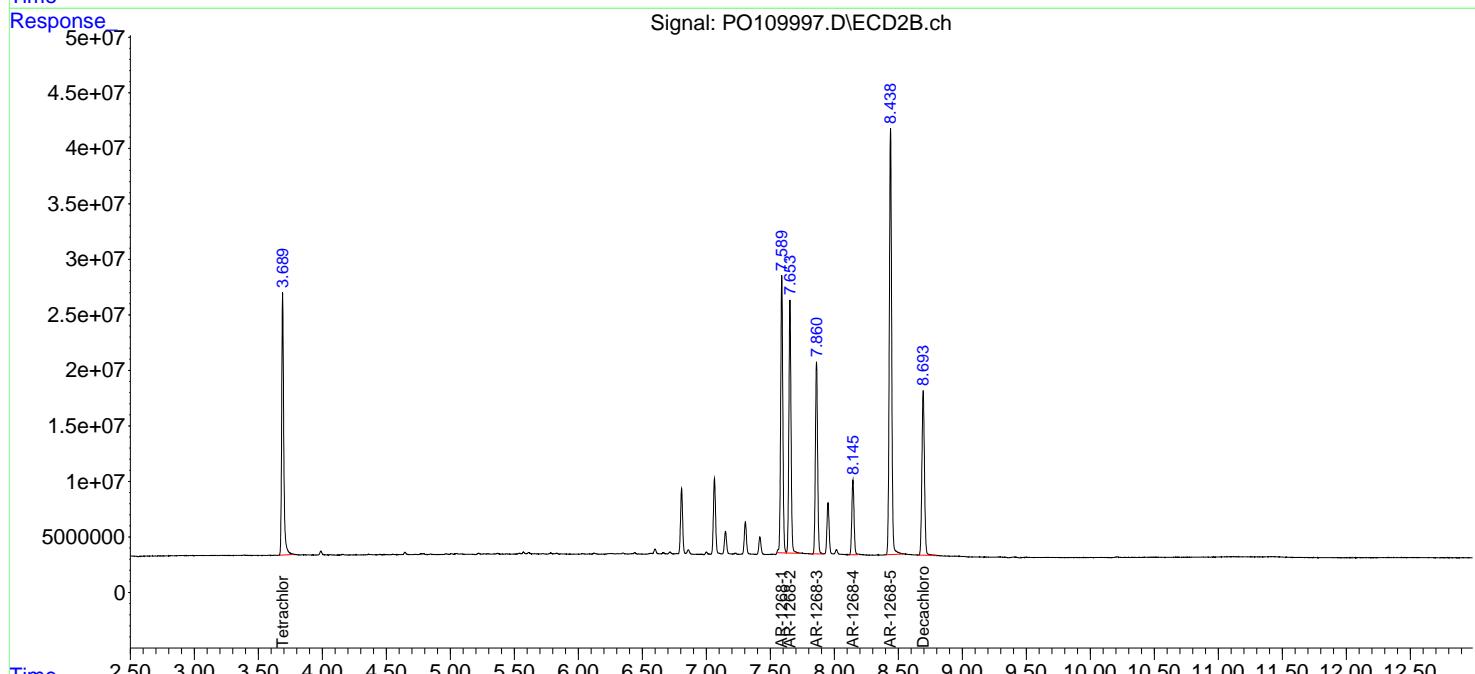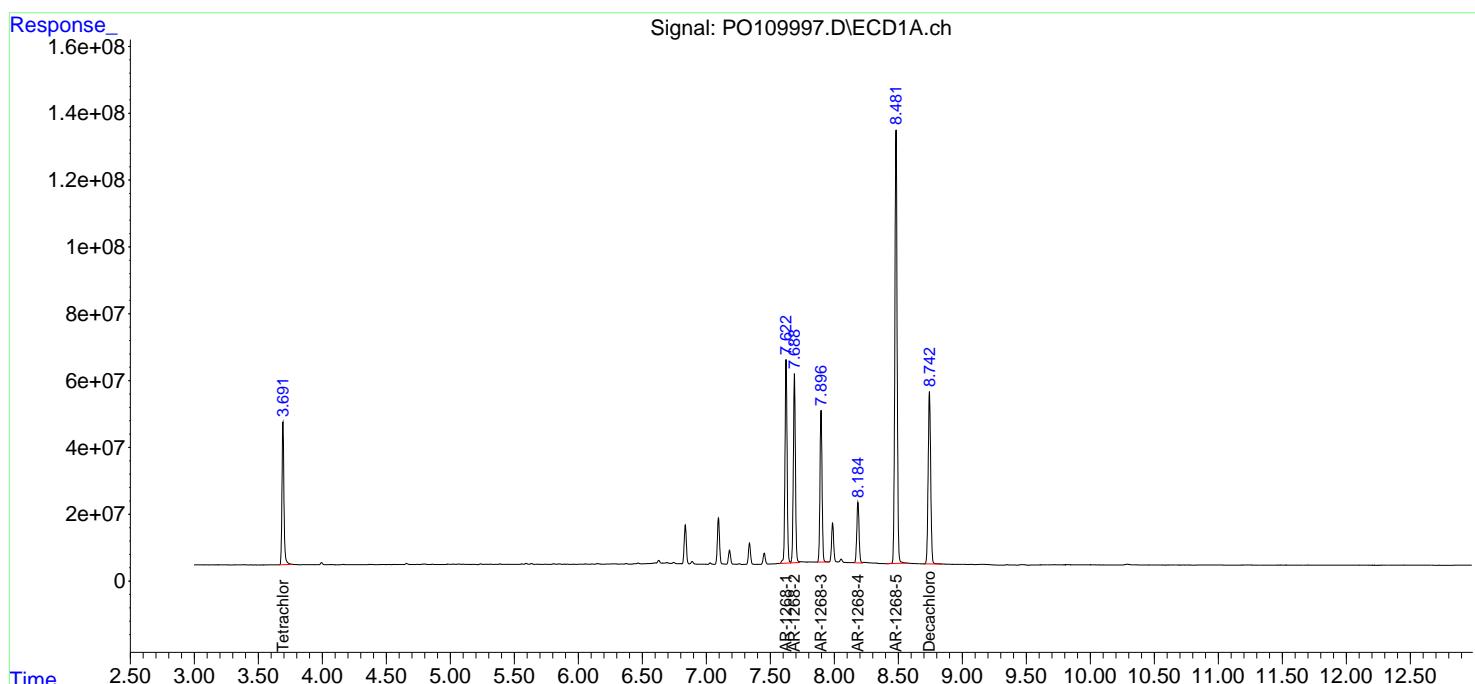

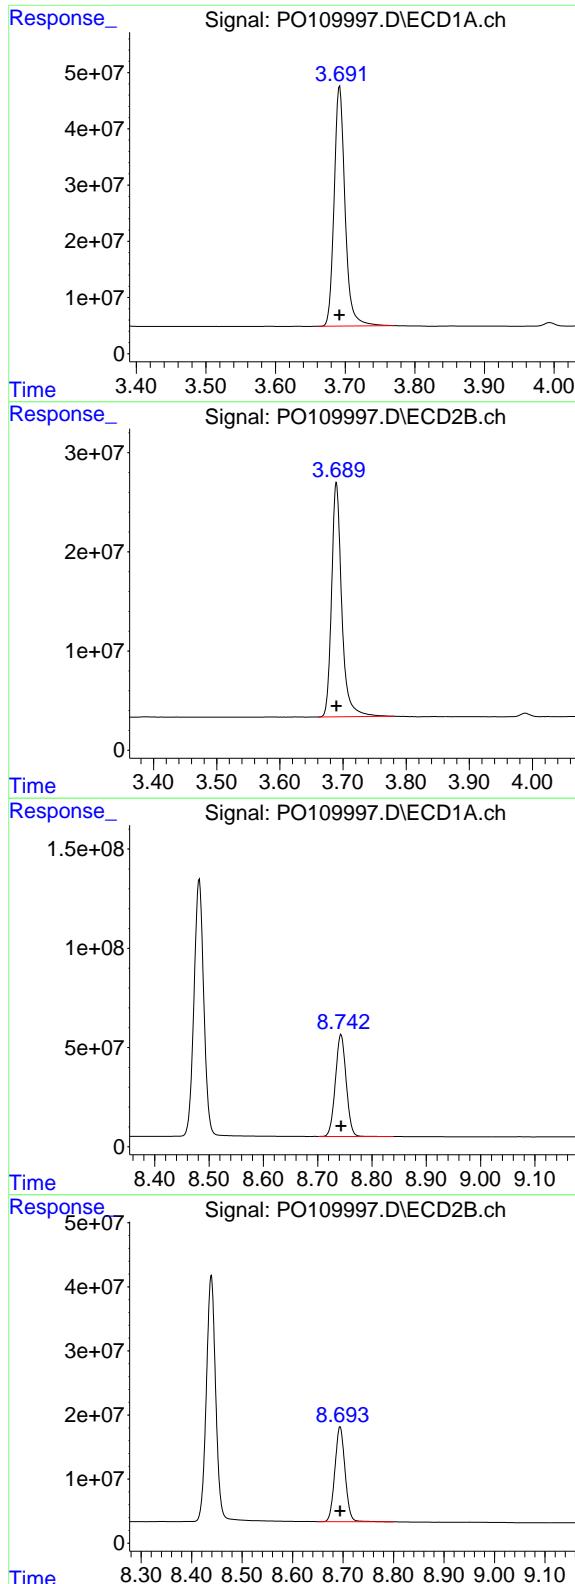

### #1 Tetrachloro-m-xylene

R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 463875726  
Conc: 50.00 ng/ml

Instrument:

ECD\_O

ClientSampleId:

AR1268ICC500

### #1 Tetrachloro-m-xylene


R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 264095871  
Conc: 50.00 ng/ml

### #2 Decachlorobiphenyl

R.T.: 8.743 min  
Delta R.T.: 0.000 min  
Response: 706011522  
Conc: 50.00 ng/ml

### #2 Decachlorobiphenyl

R.T.: 8.694 min  
Delta R.T.: 0.000 min  
Response: 207212938  
Conc: 50.00 ng/ml

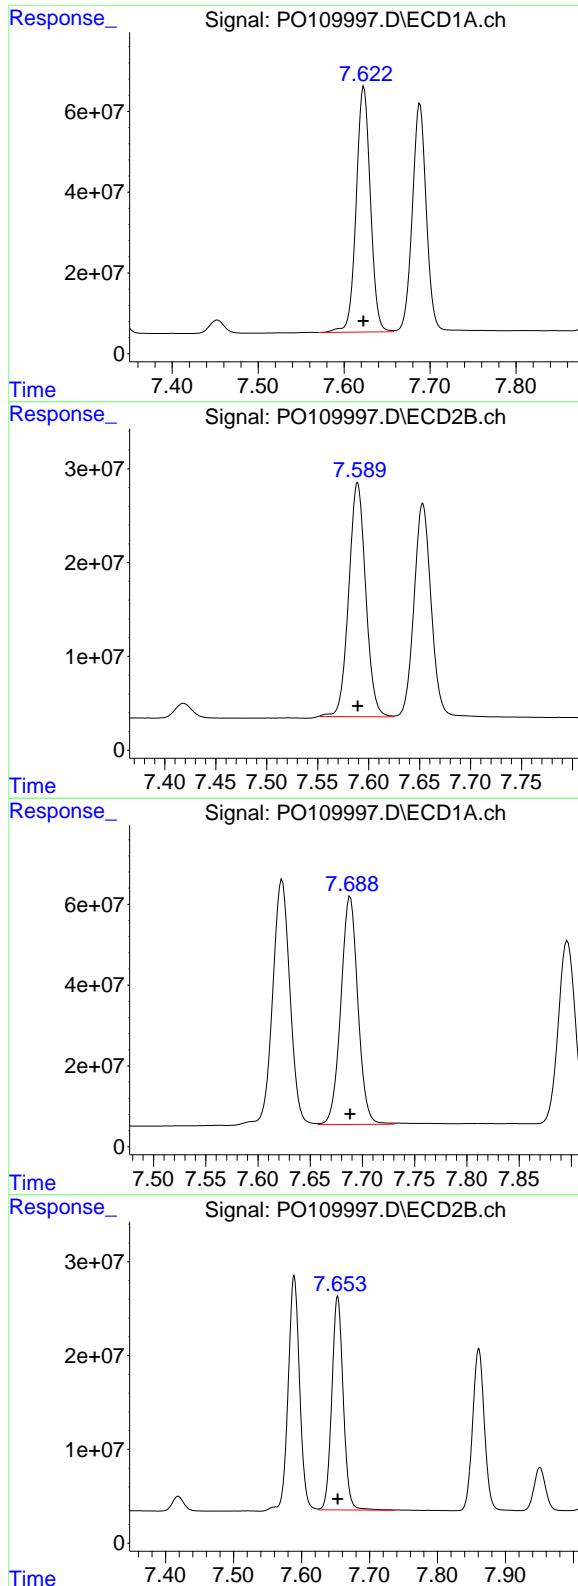

#41 AR-1268-1

R.T.: 7.623 min  
 Delta R.T.: 0.000 min  
 Response: 699811647  
 Conc: 498.68 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1268ICC500

#41 AR-1268-1


R.T.: 7.589 min  
 Delta R.T.: 0.000 min  
 Response: 289102857  
 Conc: 500.00 ng/ml

#42 AR-1268-2

R.T.: 7.688 min  
 Delta R.T.: 0.000 min  
 Response: 639816344  
 Conc: 500.00 ng/ml

#42 AR-1268-2

R.T.: 7.653 min  
 Delta R.T.: 0.000 min  
 Response: 266318012  
 Conc: 500.00 ng/ml

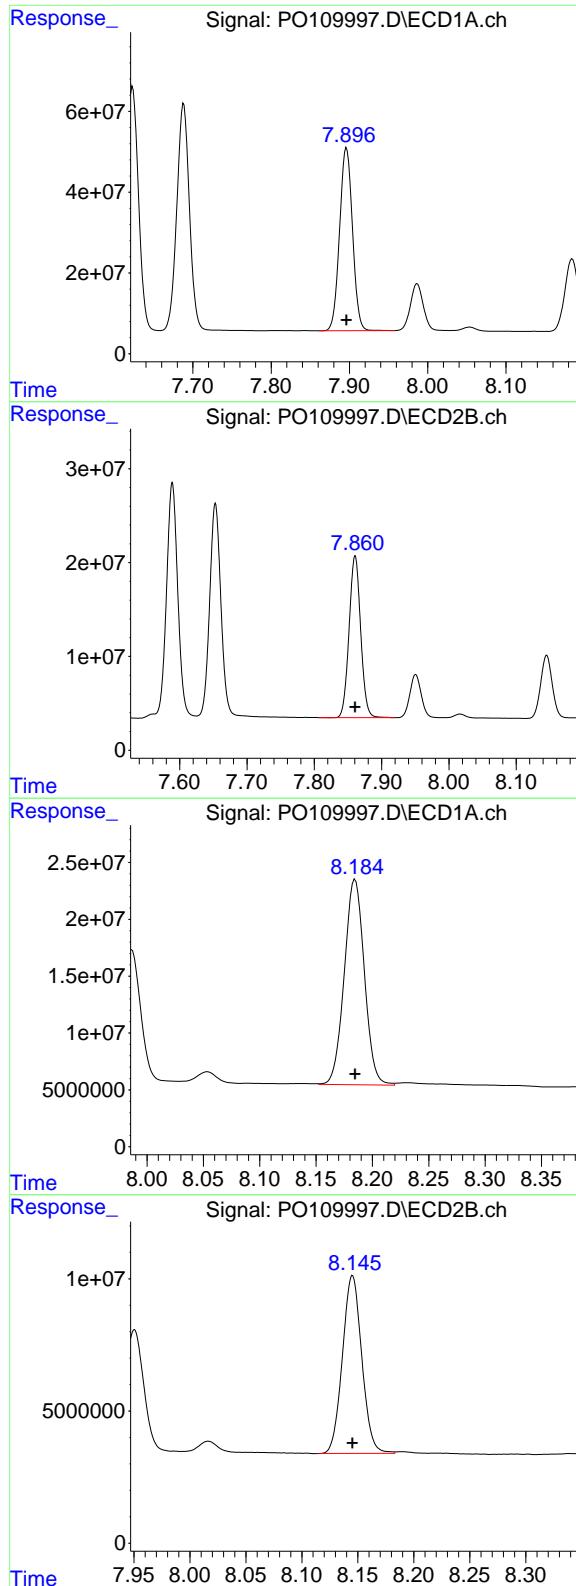

#43 AR-1268-3

R.T.: 7.896 min  
 Delta R.T.: 0.000 min  
 Response: 519324293  
 Conc: 500.00 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1268ICC500

#43 AR-1268-3


R.T.: 7.861 min  
 Delta R.T.: 0.000 min  
 Response: 206458519  
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 8.185 min  
 Delta R.T.: 0.000 min  
 Response: 223719543  
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 8.145 min  
 Delta R.T.: 0.000 min  
 Response: 81011977  
 Conc: 500.00 ng/ml

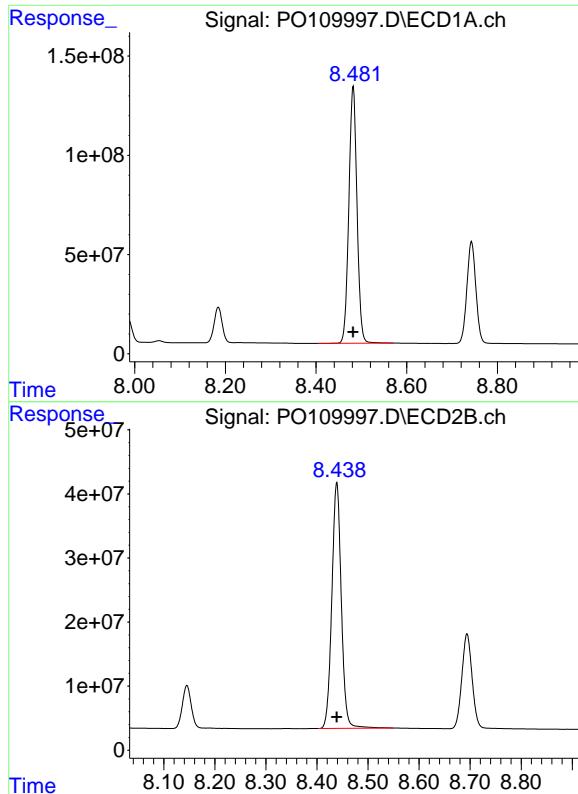

#45 AR-1268-5

R.T.: 8.482 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 1614304087 ECD\_O  
 Conc: 500.00 ng/ml **ClientSampleId :**  
 AR1268ICC500

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109998.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:57  
 Operator : YP/AJ  
 Sample : AR1268ICC250  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1268ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:56 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.692	3.690	233.0E6	133.0E6	25.112	25.182
2) SA Decachlor...	8.743	8.695	364.2E6	110.3E6	25.791	26.624

Target Compounds

41) L9 AR-1268-1	7.623	7.590	361.1E6	149.6E6	257.304	258.814
42) L9 AR-1268-2	7.688	7.654	330.4E6	137.2E6	258.196	257.558
43) L9 AR-1268-3	7.897	7.861	264.1E6	107.0E6	254.288	259.017
44) L9 AR-1268-4	8.184	8.146	118.3E6	42174671	264.470	260.299
45) L9 AR-1268-5	8.482	8.439	811.9E6	254.0E6	251.483	257.325



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109998.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 21:57  
 Operator : YP/AJ  
 Sample : AR1268ICC250  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1268ICC250**


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:06:56 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

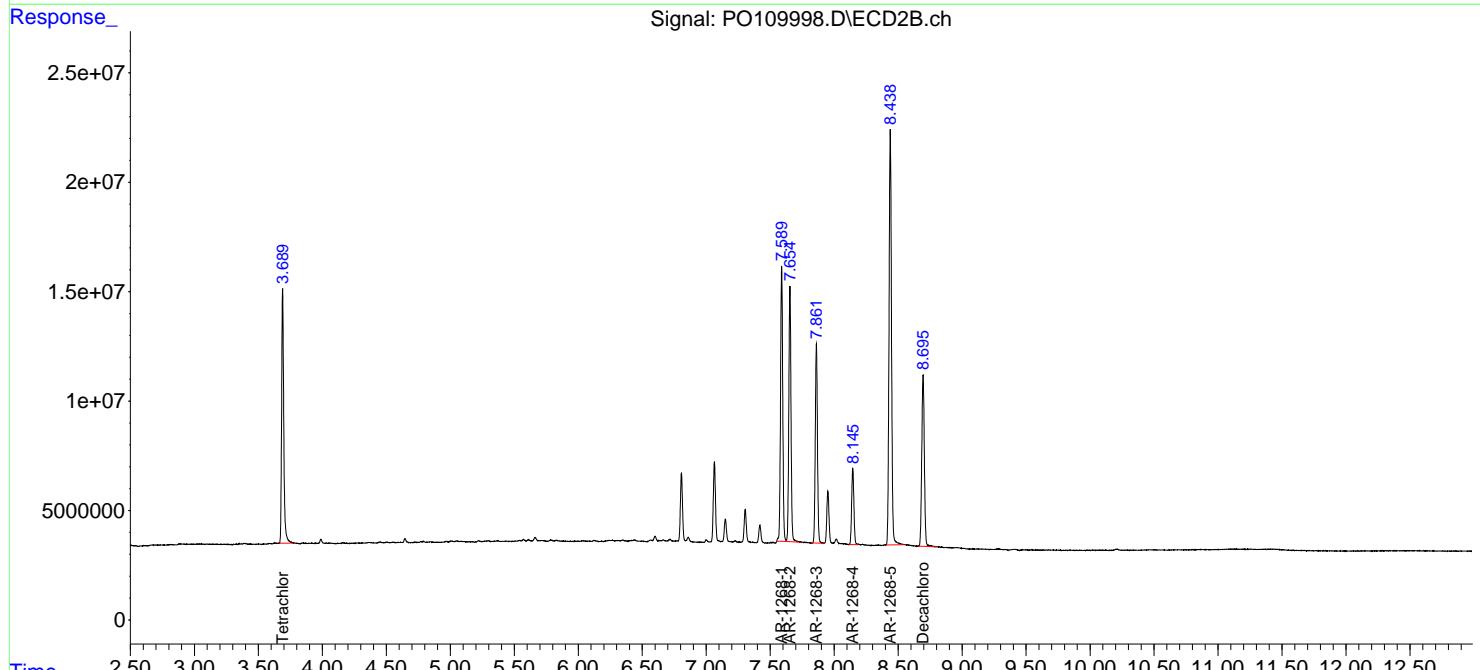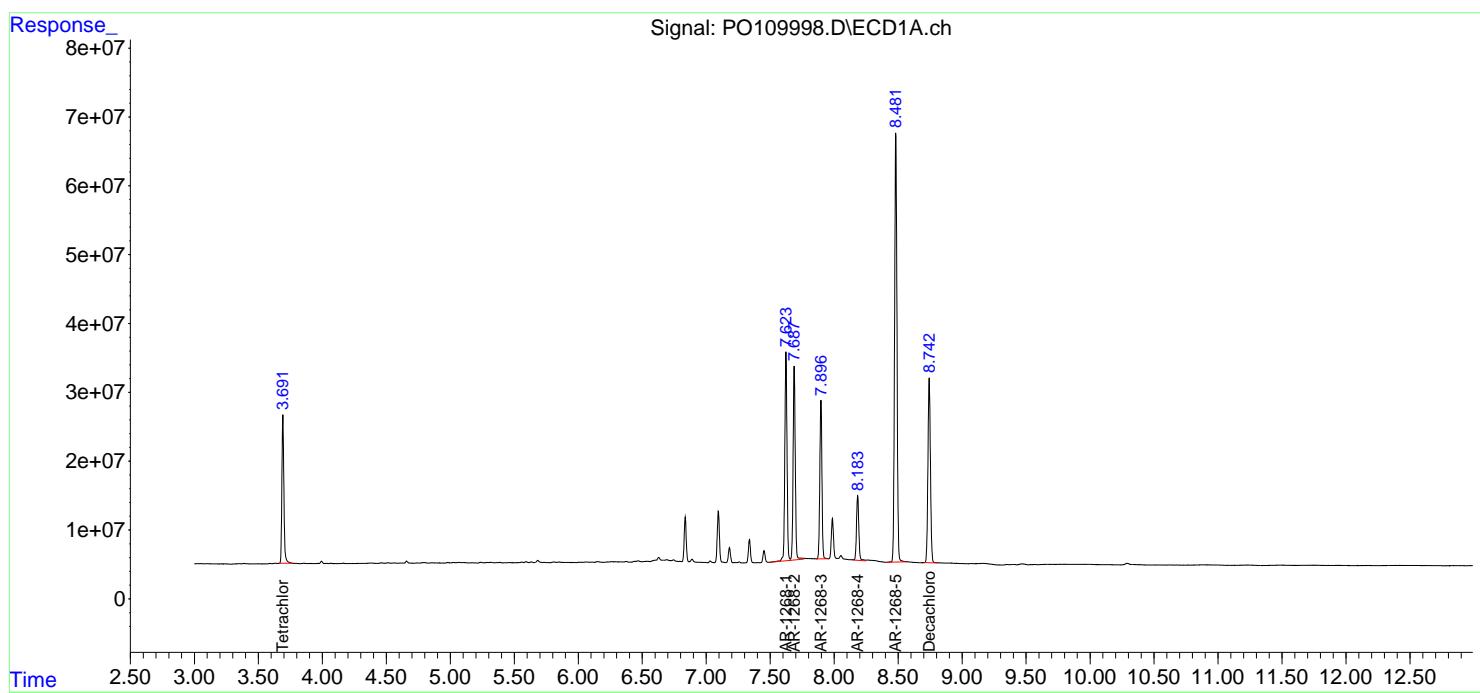


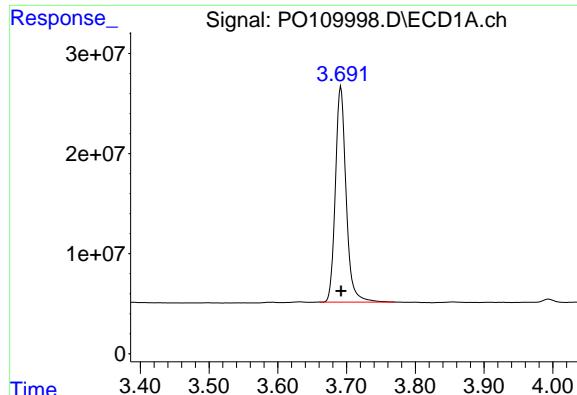


#1 Tetrachloro-m-xylene  
R.T.: 3.692 min  
Delta R.T.: 0.000 min  
Response: 232978846  
Conc: 25.11 ng/ml  
Instrument: ECD\_O  
ClientSampleId: AR1268ICC250

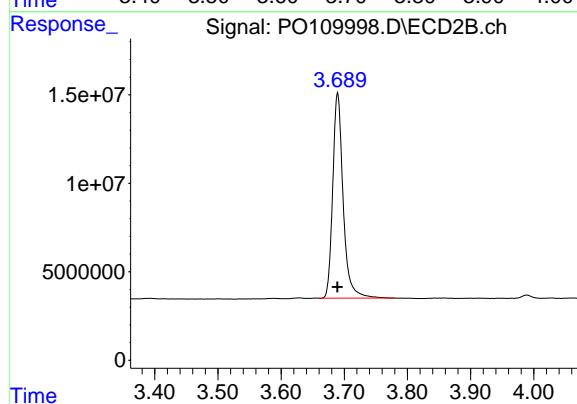


#1 Tetrachloro-m-xylene  
R.T.: 3.690 min  
Delta R.T.: 0.000 min  
Response: 133010597  
Conc: 25.18 ng/ml

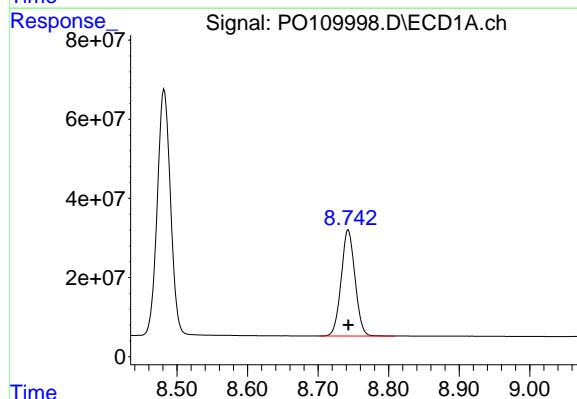

#2 Decachlorobiphenyl  
R.T.: 8.743 min  
Delta R.T.: 0.000 min  
Response: 364169510  
Conc: 25.79 ng/ml

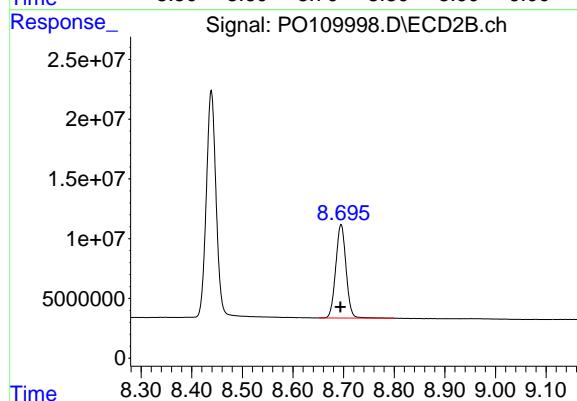

#2 Decachlorobiphenyl  
R.T.: 8.695 min  
Delta R.T.: 0.001 min  
Response: 110337267  
Conc: 26.62 ng/ml

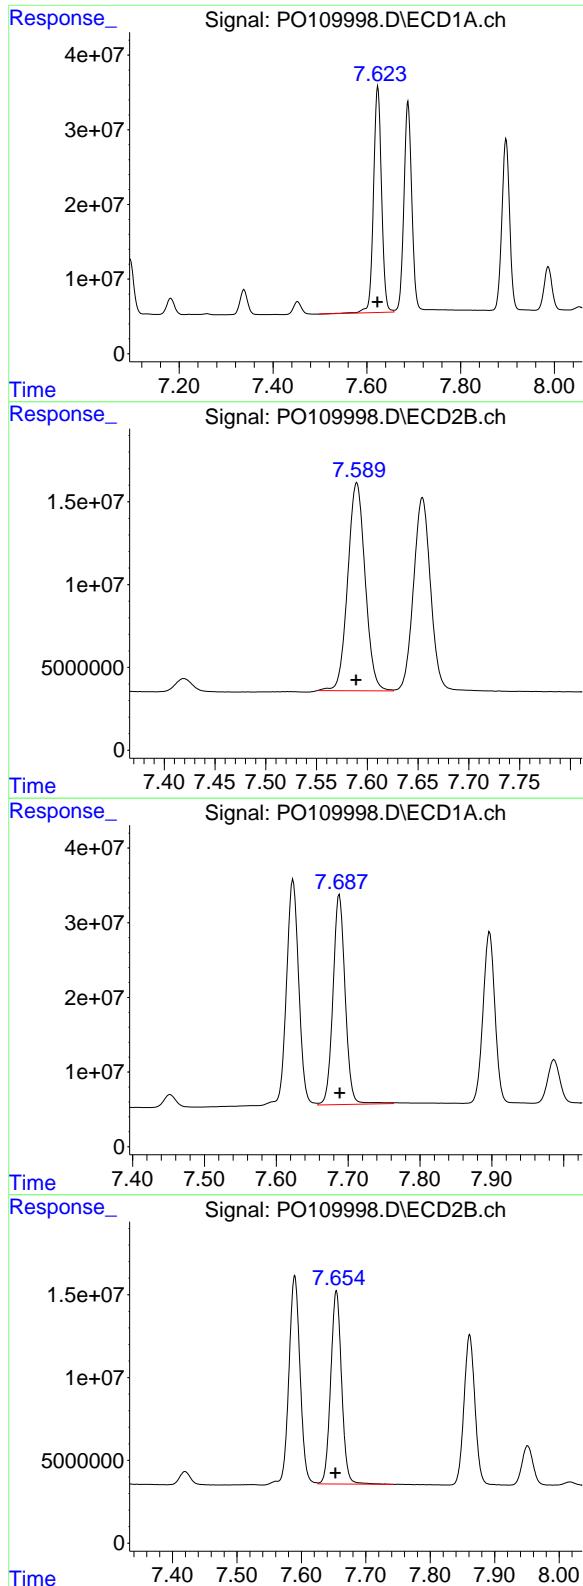

#41 AR-1268-1

R.T.: 7.623 min  
 Delta R.T.: 0.001 min  
 Response: 361082289  
 Conc: 257.30 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1268ICC250

#41 AR-1268-1


R.T.: 7.590 min  
 Delta R.T.: 0.000 min  
 Response: 149647905  
 Conc: 258.81 ng/ml

#42 AR-1268-2

R.T.: 7.688 min  
 Delta R.T.: 0.000 min  
 Response: 330395950  
 Conc: 258.20 ng/ml

#42 AR-1268-2

R.T.: 7.654 min  
 Delta R.T.: 0.001 min  
 Response: 137184821  
 Conc: 257.56 ng/ml

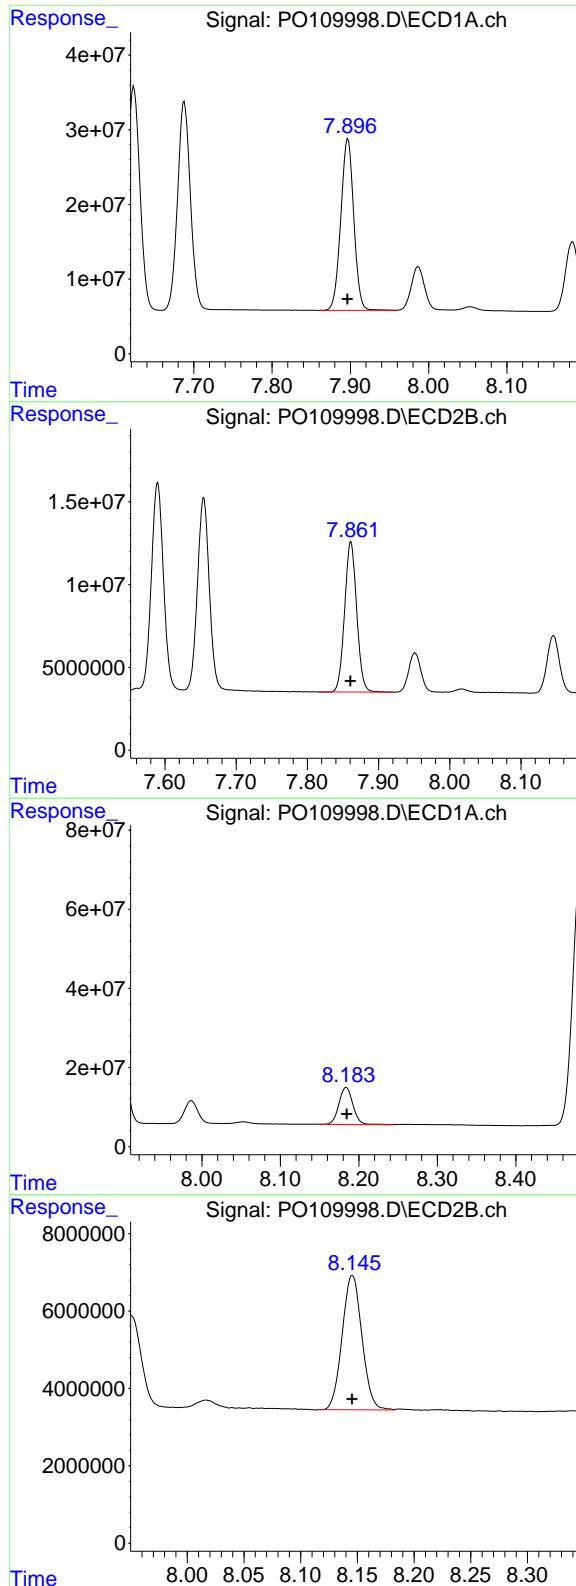

#43 AR-1268-3

R.T.: 7.897 min  
 Delta R.T.: 0.000 min  
 Response: 264115362  
 Conc: 254.29 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1268ICC250

#43 AR-1268-3


R.T.: 7.861 min  
 Delta R.T.: 0.000 min  
 Response: 106952452  
 Conc: 259.02 ng/ml

#44 AR-1268-4

R.T.: 8.184 min  
 Delta R.T.: 0.000 min  
 Response: 118334390  
 Conc: 264.47 ng/ml

#44 AR-1268-4

R.T.: 8.146 min  
 Delta R.T.: 0.000 min  
 Response: 42174671  
 Conc: 260.30 ng/ml

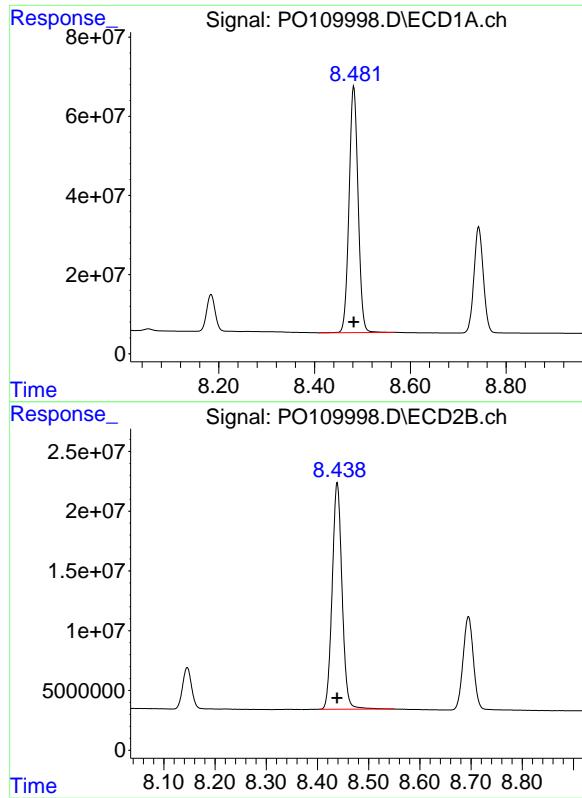

#45 AR-1268-5

R.T.: 8.482 min  
Delta R.T.: 0.000 min  
Response: 811940473  
Conc: 251.48 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1268ICC250

#45 AR-1268-5

R.T.: 8.439 min  
Delta R.T.: 0.000 min  
Response: 254015607  
Conc: 257.32 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109999.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 22:15  
 Operator : YP/AJ  
 Sample : AR1268ICC050  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1268ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:07:11 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.689	36859656	18867712	3.973	3.572
2) SA Decachlor...	8.743	8.695	72973489	22764198	5.168	5.493

Target Compounds

41) L9 AR-1268-1	7.623	7.590	72851126	31006348	51.913	53.625
42) L9 AR-1268-2	7.688	7.654	63525178	28112917	49.643	52.781
43) L9 AR-1268-3	7.896	7.861	50172519	22018734	48.306	53.325
44) L9 AR-1268-4	8.184	8.146	23615947	8301200	52.780	51.234
45) L9 AR-1268-5	8.481	8.438	151.8E6	51592382	47.022	52.264


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0031925\  
 Data File : P0109999.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Mar 2025 22:15  
 Operator : YP/AJ  
 Sample : AR1268ICC050  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1268ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:07:11 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:04:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

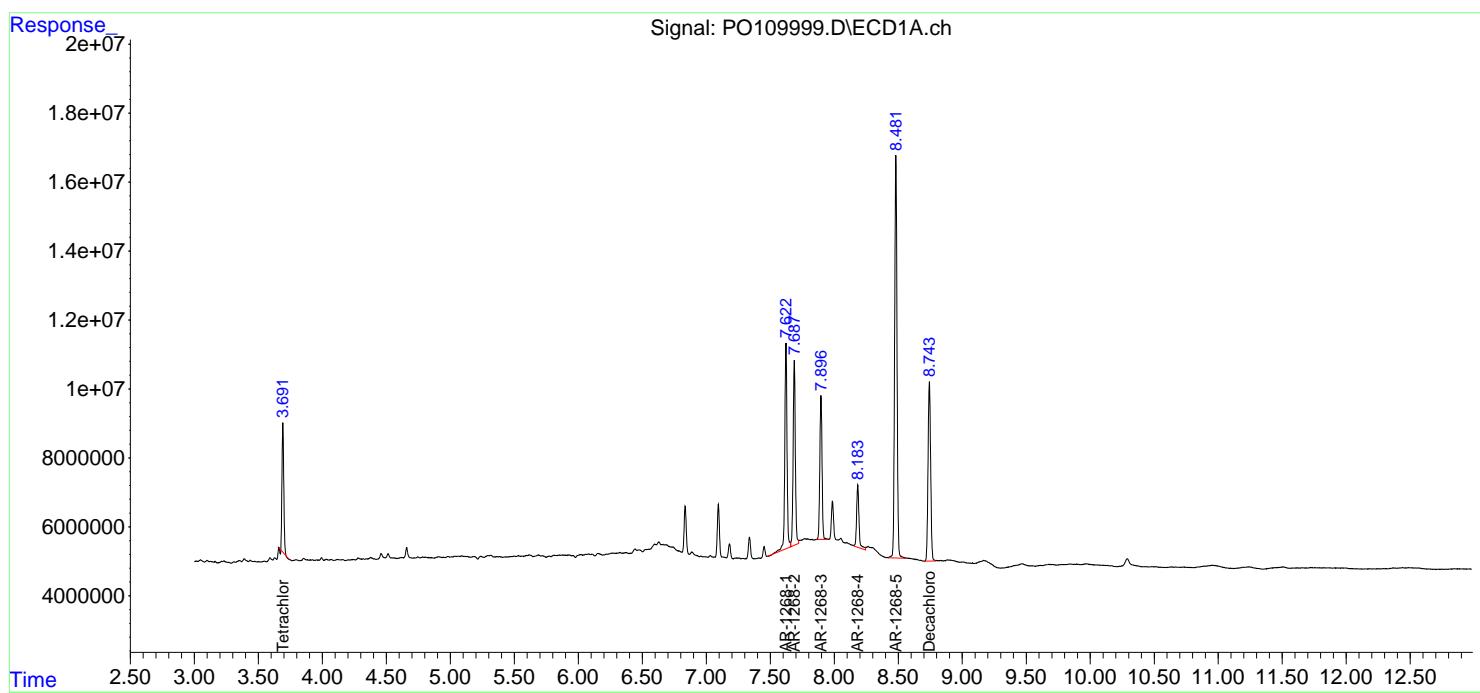




#1 Tetrachloro-m-xylene  
R.T.: 3.691 min  
Delta R.T.: 0.000 min  
Response: 36859656  
Conc: 3.97 ng/ml


Instrument: ECD\_O  
ClientSampleId: AR1268ICC050

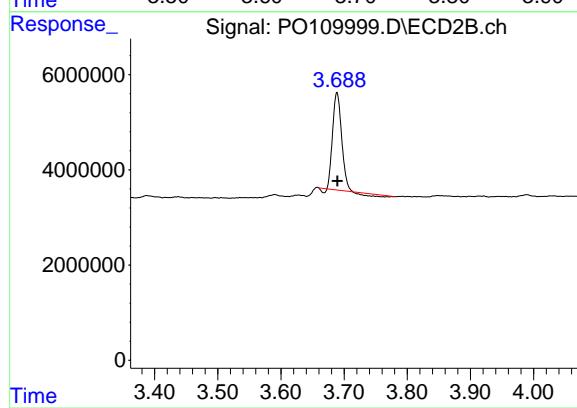


#1 Tetrachloro-m-xylene  
R.T.: 3.689 min  
Delta R.T.: 0.000 min  
Response: 18867712  
Conc: 3.57 ng/ml

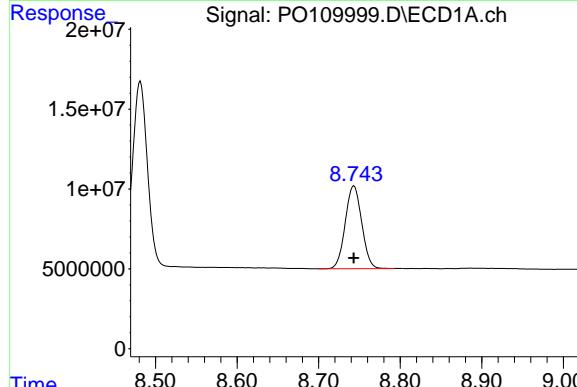

#2 Decachlorobiphenyl  
R.T.: 8.743 min  
Delta R.T.: 0.000 min  
Response: 72973489  
Conc: 5.17 ng/ml

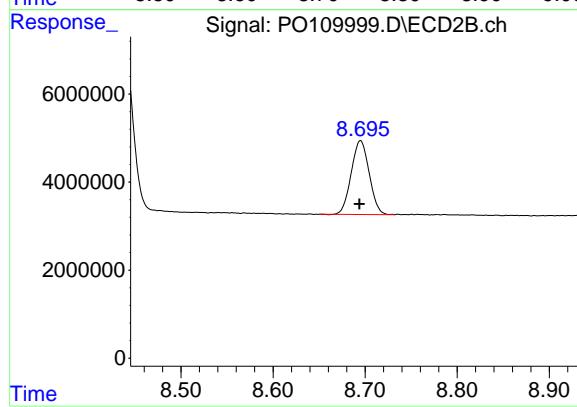


#2 Decachlorobiphenyl  
R.T.: 8.695 min  
Delta R.T.: 0.001 min  
Response: 22764198  
Conc: 5.49 ng/ml

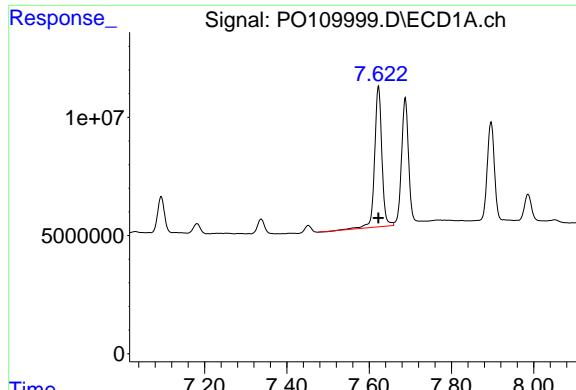


#41 AR-1268-1

R.T.: 7.623 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 72851126 ECD\_O  
 Conc: 51.91 ng/ml **ClientSampleId :**  
 AR1268ICC050

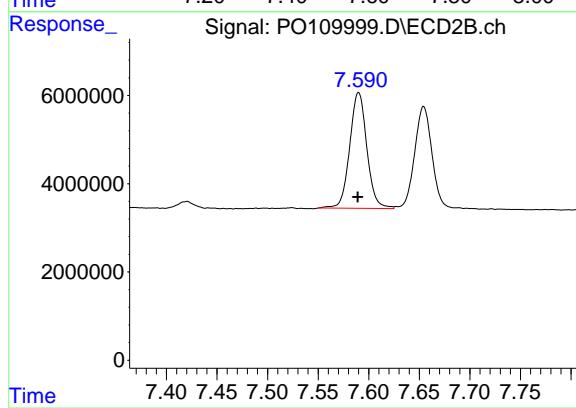


#41 AR-1268-1

R.T.: 7.590 min  
 Delta R.T.: 0.000 min  
 Response: 31006348  
 Conc: 53.63 ng/ml

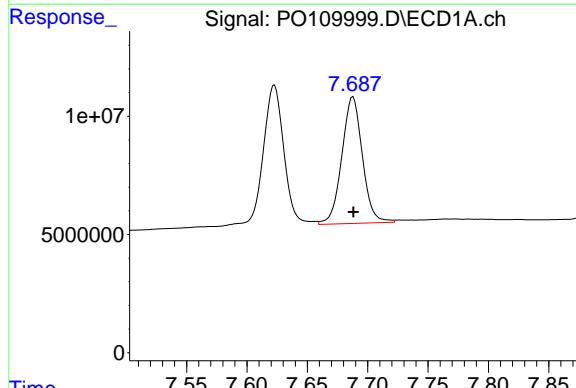


#42 AR-1268-2

R.T.: 7.688 min  
 Delta R.T.: 0.000 min  
 Response: 63525178  
 Conc: 49.64 ng/ml

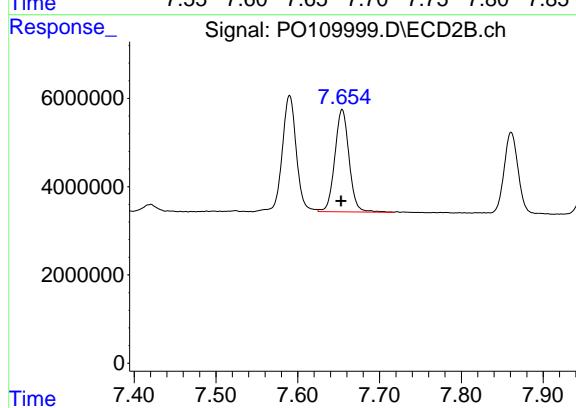

#42 AR-1268-2

R.T.: 7.654 min  
 Delta R.T.: 0.001 min  
 Response: 28112917  
 Conc: 52.78 ng/ml

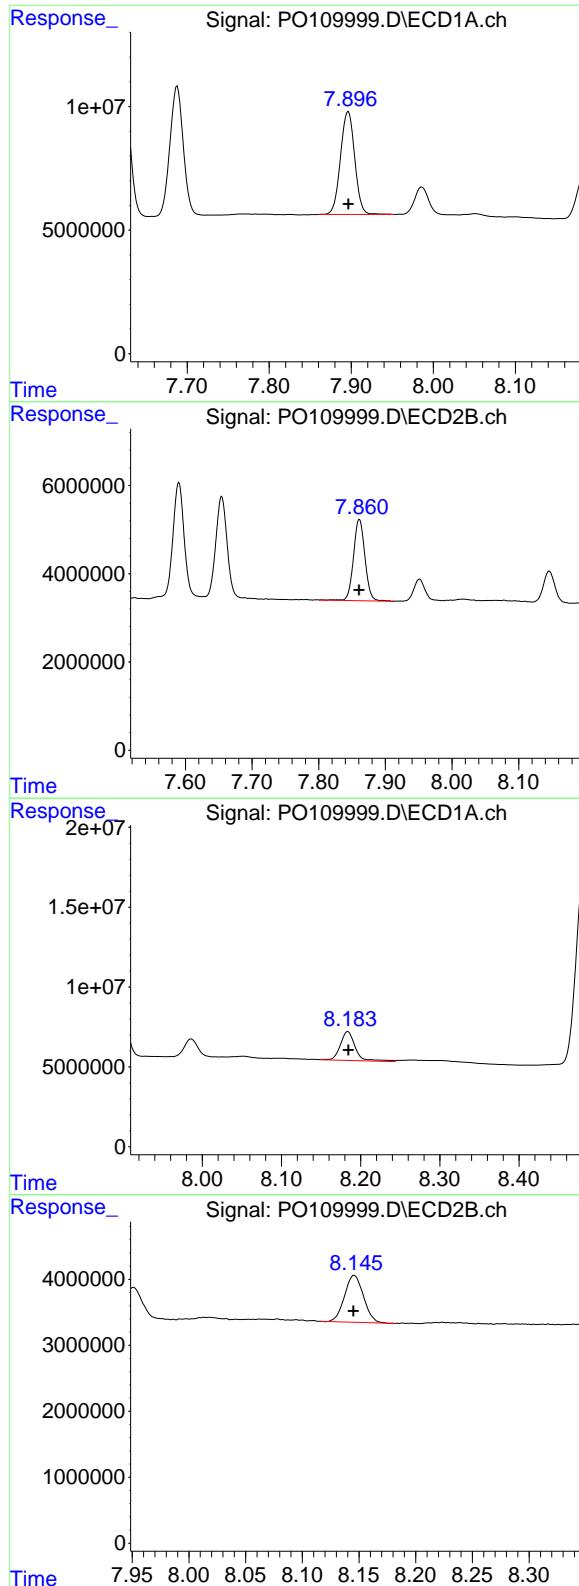

#43 AR-1268-3

R.T.: 7.896 min  
Delta R.T.: 0.000 min **Instrument:**  
Response: 50172519 ECD\_O  
Conc: 48.31 ng/ml **ClientSampleId :**  
AR1268ICC050

#43 AR-1268-3


R.T.: 7.861 min  
Delta R.T.: 0.000 min  
Response: 22018734  
Conc: 53.32 ng/ml

#44 AR-1268-4

R.T.: 8.184 min  
Delta R.T.: 0.000 min  
Response: 23615947  
Conc: 52.78 ng/ml

#44 AR-1268-4

R.T.: 8.146 min  
Delta R.T.: 0.000 min  
Response: 8301200  
Conc: 51.23 ng/ml

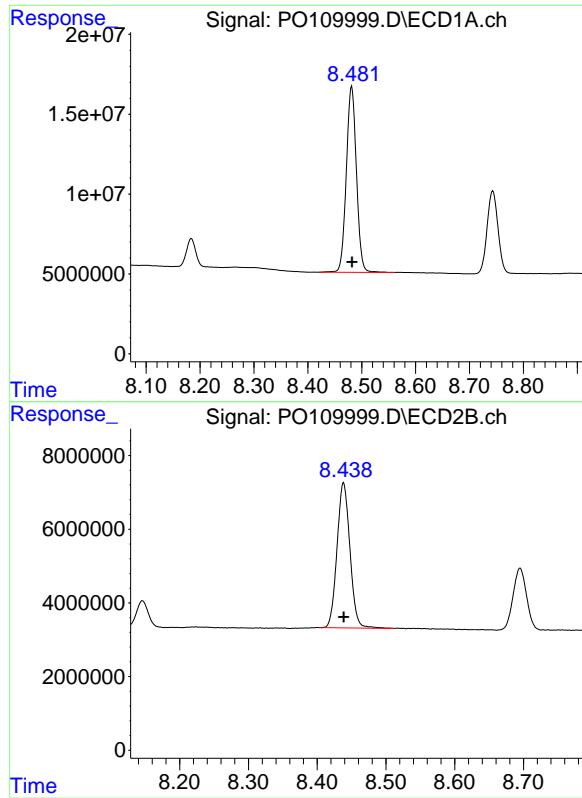

#45 AR-1268-5

R.T.: 8.481 min  
 Delta R.T.: 0.000 min  
 Response: 151815895  
 Conc: 47.02 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1268ICC050

#45 AR-1268-5

R.T.: 8.438 min  
 Delta R.T.: 0.000 min  
 Response: 51592382  
 Conc: 52.26 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110286.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 21:27  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:36:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	3.691	3.688	486.8E6	278.7E6	53.484	53.152
2) SA Decachlor...	8.740	8.691	420.5E6	118.3E6	54.690	48.766

Target Compounds

3) L1 AR-1016-1	4.783	4.769	177.8E6	93902896	528.316	512.417
4) L1 AR-1016-2	4.802	4.788	244.1E6	134.4E6	526.454	514.067
5) L1 AR-1016-3	4.858	4.964	169.7E6	73038464	529.369	515.158
6) L1 AR-1016-4	4.979	5.006	131.1E6	55338718	518.987	469.252
7) L1 AR-1016-5	5.236	5.219	150.5E6	83969338	547.465	549.111
8) L2 AR-1221-1	3.903	3.897	19462416	11025922	168.028	164.856
9) L2 AR-1221-2	3.990	3.984	28148560	15829281	325.418	320.550
10) L2 AR-1221-3	4.066	4.059	98013268	55109401	374.531	363.317
11) L3 AR-1232-1	4.066	4.059	98013268	55109401	454.302	444.096
12) L3 AR-1232-2	4.560	4.788	132.9E6	134.4E6	1157.840	1117.012
13) L3 AR-1232-3	4.802	4.964	244.1E6	73038464	1152.657	1147.393
14) L3 AR-1232-4	4.979	5.048	131.1E6	73350252	1154.819	1236.083
15) L3 AR-1232-5	5.021	5.219	95769846	83969338	1190.368	1328.253
16) L4 AR-1242-1	4.783	4.769	177.8E6	93902896	664.910	642.223
17) L4 AR-1242-2	4.802	4.788	244.1E6	134.4E6	662.975	646.191
18) L4 AR-1242-3	4.858	4.964	169.7E6	73038464	657.909	654.391
19) L4 AR-1242-4	4.979	5.048	131.1E6	73350252	655.404	632.458
20) L4 AR-1242-5	5.632	5.570	47210124	77845170	223.685	567.211 #
21) L5 AR-1248-1	4.783	4.769	177.8E6	93902896	806.421	772.628
22) L5 AR-1248-2	5.021	5.006	95769846	55338718	317.974	328.500
23) L5 AR-1248-3	5.236	5.048	150.5E6	73350252	403.228	404.826
24) L5 AR-1248-4	5.591	5.219	148.5E6	83969338	281.330	398.985 #
25) L5 AR-1248-5	5.632	5.611	47210124	22863074	126.586	109.986
26) L6 AR-1254-1	5.591	5.570	148.5E6	77845170	262.801	248.949
27) L6 AR-1254-2	5.740	5.717	117.1E6	57497390	243.333	211.748
28) L6 AR-1254-3	6.161	6.136	199.8E6	94798356	258.500	228.191
29) L6 AR-1254-4	6.375	6.348	32159525	13331170	66.979	54.958
30) L6 AR-1254-5	6.794	6.765	299.0E6	152.0E6	459.925	452.452
31) L7 AR-1260-1	6.277	6.251	259.3E6	123.5E6	550.162	483.373
32) L7 AR-1260-2	6.466	6.439	302.8E6	143.3E6	508.402	477.179
33) L7 AR-1260-3	6.834	6.591	233.8E6	133.6E6	481.744	462.164
34) L7 AR-1260-4	7.094	7.063	200.0E6	99360275	471.486	461.972
35) L7 AR-1260-5	7.336	7.303	484.1E6	221.7E6	462.918	444.506
36) L8 AR-1262-1	6.834	6.804	233.8E6	118.1E6	339.753	342.880
37) L8 AR-1262-2	7.336	7.303	484.1E6	221.7E6	406.167	412.630
38) L8 AR-1262-3	7.621	7.587	112.7E6	45025623	239.417	232.030
39) L8 AR-1262-4	7.684	7.649	350.3E6	141.7E6	400.497	391.534
40) L8 AR-1262-5	8.182	8.143	121.0E6	43223300	306.815	306.197
41) L9 AR-1268-1	7.621	7.587	112.7E6	45025623	80.476	76.923

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110286.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 21:27  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:36:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	7.684	7.649	350.3E6	141.7E6	273.612	263.471
43) L9 AR-1268-3	7.893	7.857	6384140	2701969	6.213	6.500
44) L9 AR-1268-4	8.182	8.143	121.0E6	43223300	273.806	268.395
45) L9 AR-1268-5	8.480	8.436	34068238	11602754	10.709	11.684



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0040725\  
 Data File : P0110286.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Apr 2025 21:27  
 Operator : YP/AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_O**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 01:36:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0031925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 19 02:52:01 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

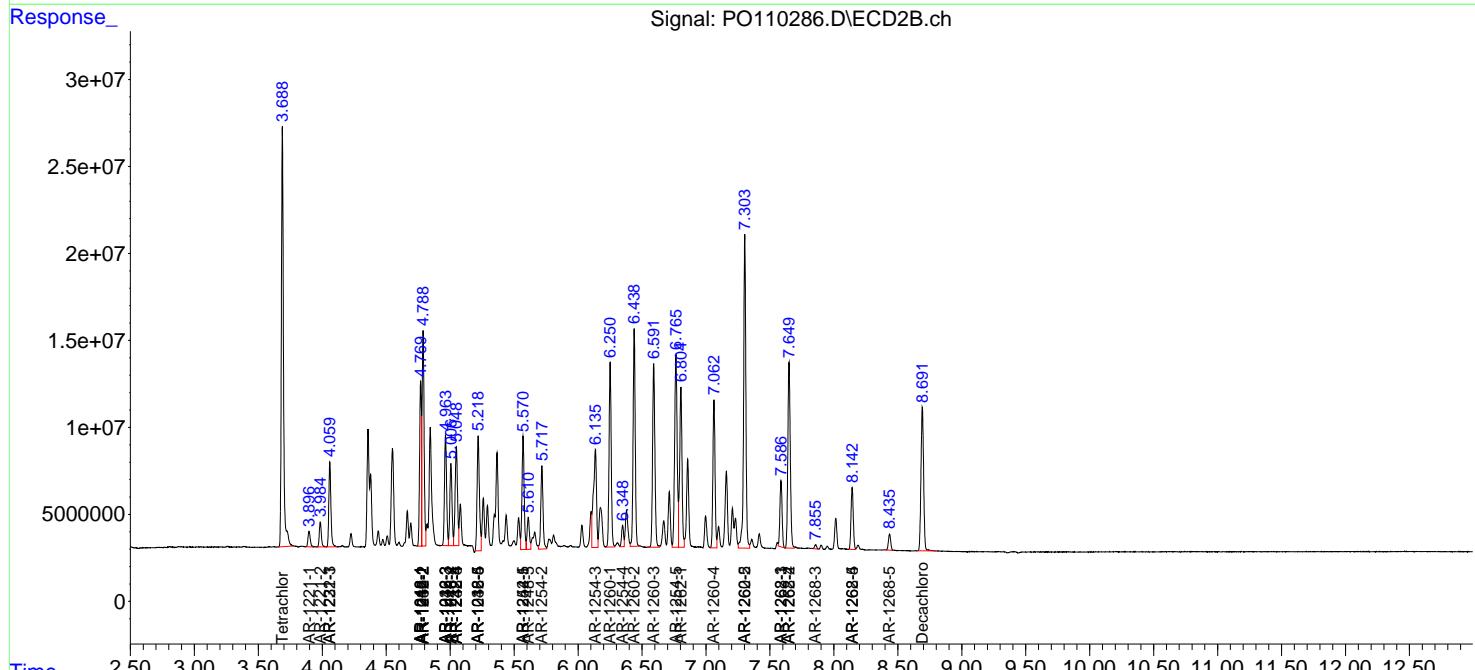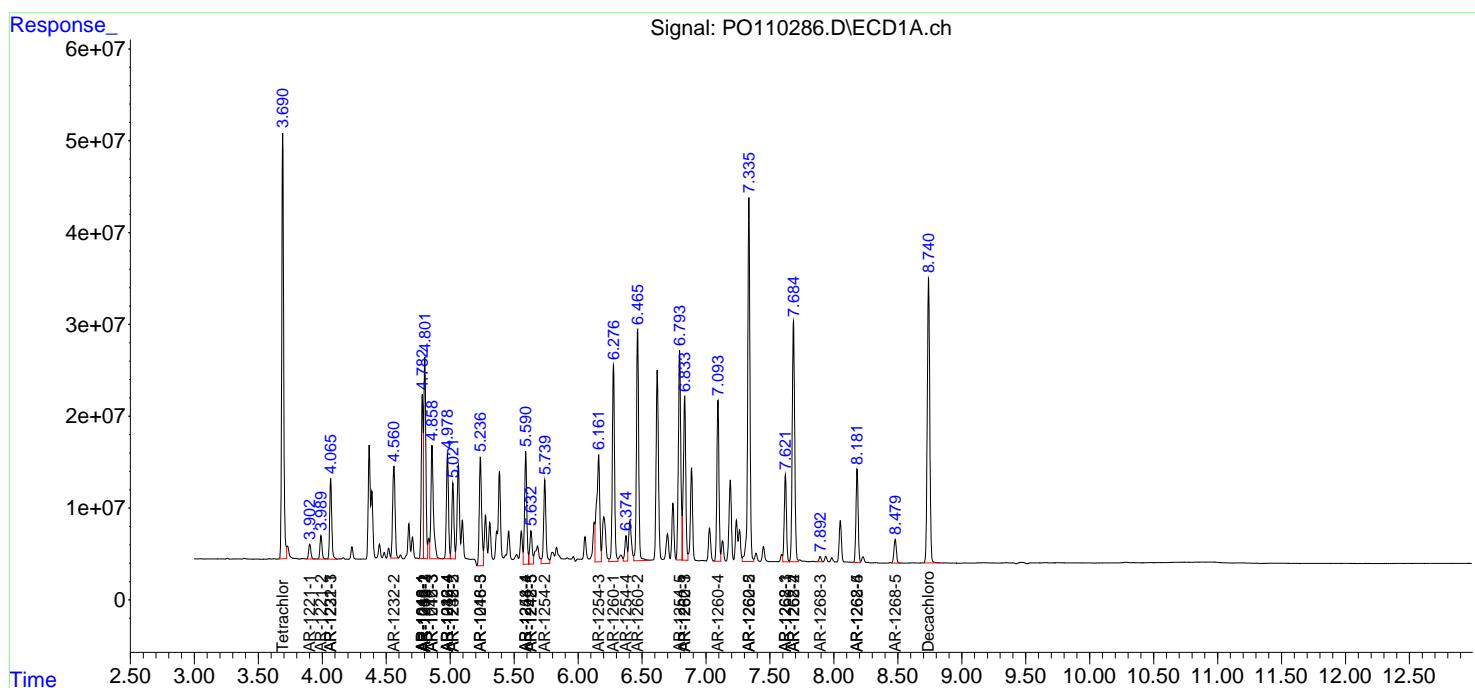

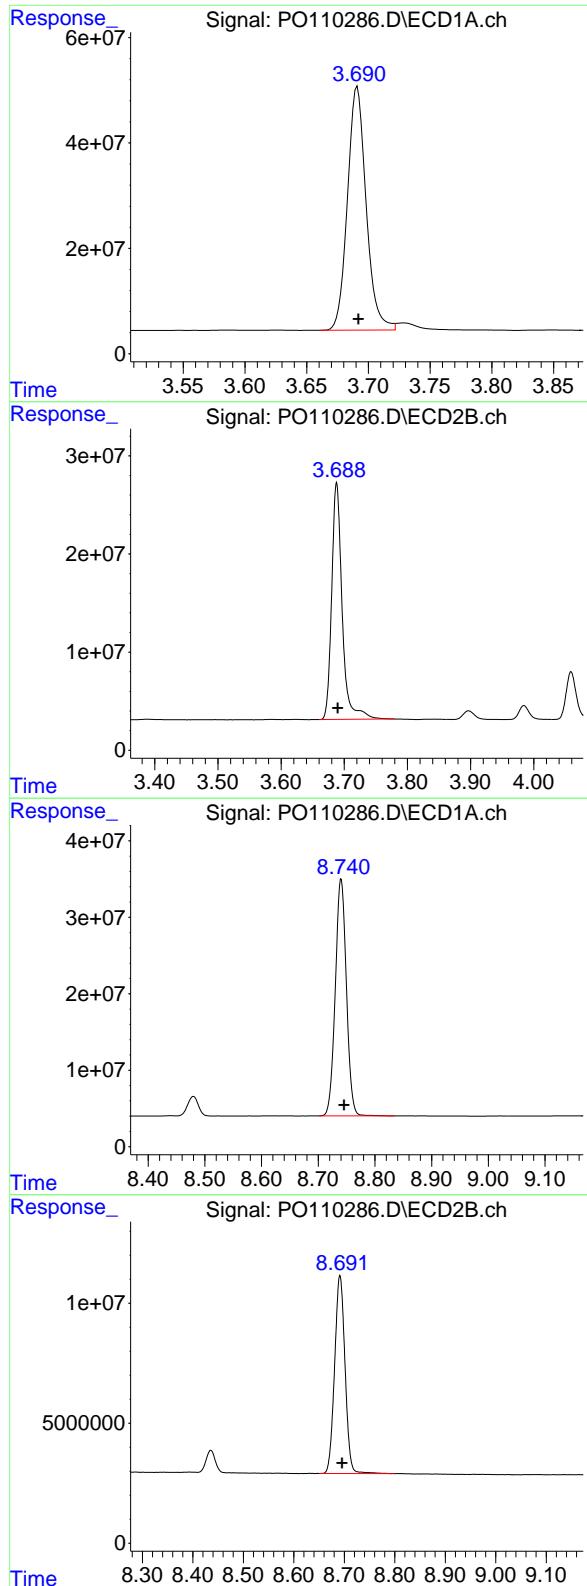

#1 Tetrachloro-m-xylene

R.T.: 3.691 min  
Delta R.T.: -0.001 min  
Response: 486781502  
Conc: 53.48 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#1 Tetrachloro-m-xylene


R.T.: 3.688 min  
Delta R.T.: -0.002 min  
Response: 278731990  
Conc: 53.15 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.740 min  
Delta R.T.: -0.005 min  
Response: 420491355  
Conc: 54.69 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.691 min  
Delta R.T.: -0.004 min  
Response: 118311884  
Conc: 48.77 ng/ml

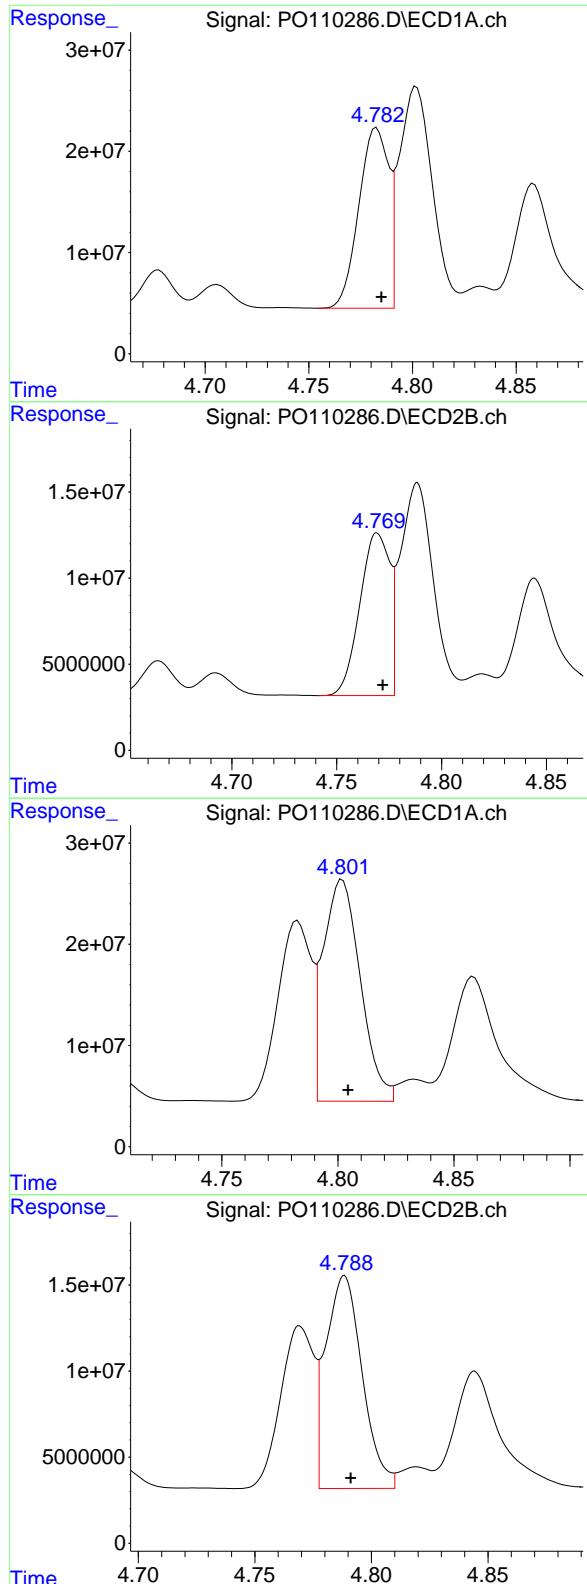

#3 AR-1016-1

R.T.: 4.783 min  
 Delta R.T.: -0.002 min  
 Response: 177801623  
 Conc: 528.32 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.769 min  
 Delta R.T.: -0.003 min  
 Response: 93902896  
 Conc: 512.42 ng/ml

#4 AR-1016-2

R.T.: 4.802 min  
 Delta R.T.: -0.003 min  
 Response: 244109403  
 Conc: 526.45 ng/ml

#4 AR-1016-2

R.T.: 4.788 min  
 Delta R.T.: -0.003 min  
 Response: 134430740  
 Conc: 514.07 ng/ml

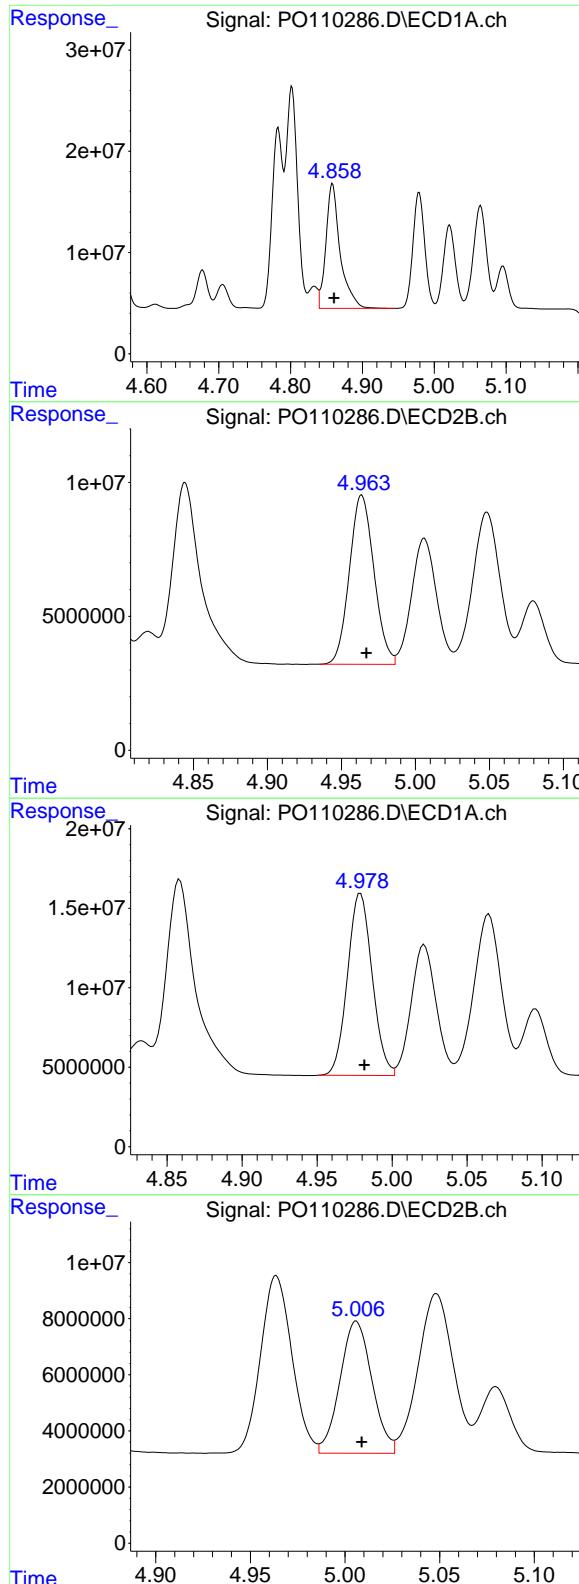

#5 AR-1016-3

R.T.: 4.858 min  
 Delta R.T.: -0.002 min  
 Response: 169708224  
 Conc: 529.37 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#5 AR-1016-3


R.T.: 4.964 min  
 Delta R.T.: -0.003 min  
 Response: 73038464  
 Conc: 515.16 ng/ml

#6 AR-1016-4

R.T.: 4.979 min  
 Delta R.T.: -0.002 min  
 Response: 131142472  
 Conc: 518.99 ng/ml

#6 AR-1016-4

R.T.: 5.006 min  
 Delta R.T.: -0.003 min  
 Response: 55338718  
 Conc: 469.25 ng/ml

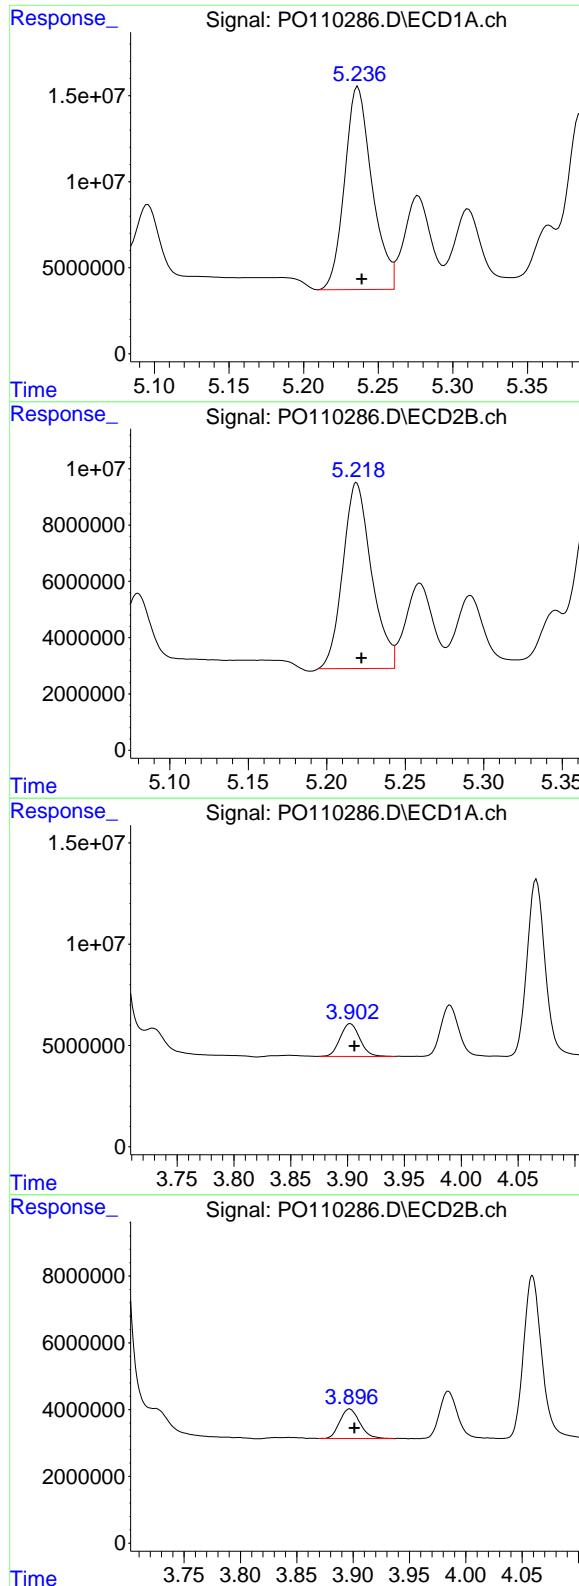

#7 AR-1016-5

R.T.: 5.236 min  
 Delta R.T.: -0.003 min  
 Response: 150479994  
 Conc: 547.46 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#7 AR-1016-5


R.T.: 5.219 min  
 Delta R.T.: -0.003 min  
 Response: 83969338  
 Conc: 549.11 ng/ml

#8 AR-1221-1

R.T.: 3.903 min  
 Delta R.T.: -0.003 min  
 Response: 19462416  
 Conc: 168.03 ng/ml

#8 AR-1221-1

R.T.: 3.897 min  
 Delta R.T.: -0.004 min  
 Response: 11025922  
 Conc: 164.86 ng/ml

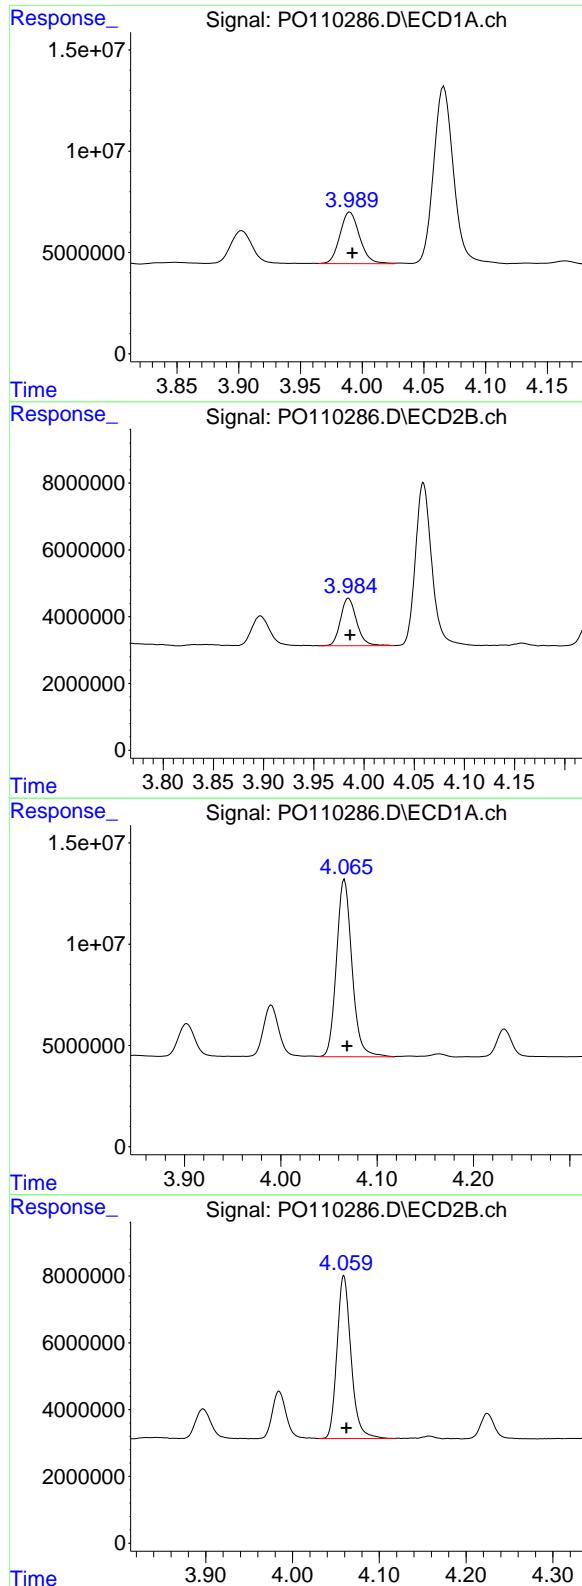

#9 AR-1221-2

R.T.: 3.990 min  
 Delta R.T.: -0.002 min  
 Response: 28148560  
 Conc: 325.42 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#9 AR-1221-2


R.T.: 3.984 min  
 Delta R.T.: -0.002 min  
 Response: 15829281  
 Conc: 320.55 ng/ml

#10 AR-1221-3

R.T.: 4.066 min  
 Delta R.T.: -0.003 min  
 Response: 98013268  
 Conc: 374.53 ng/ml

#10 AR-1221-3


R.T.: 4.059 min  
 Delta R.T.: -0.003 min  
 Response: 55109401  
 Conc: 363.32 ng/ml



#11 AR-1232-1

R.T.: 4.066 min  
 Delta R.T.: -0.002 min  
 Response: 98013268  
 Conc: 454.30 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

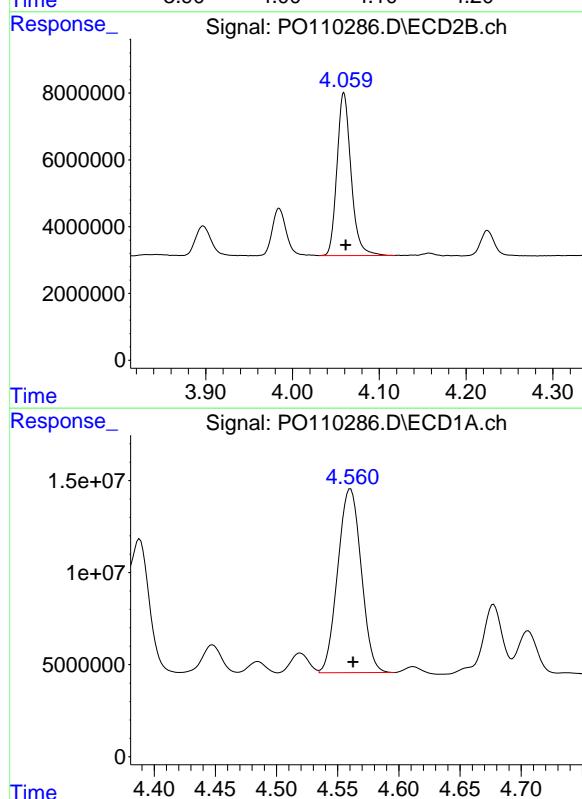


#12 AR-1232-2

R.T.: 4.560 min  
 Delta R.T.: -0.002 min  
 Response: 132903875  
 Conc: 1157.84 ng/ml

#12 AR-1232-2

R.T.: 4.788 min  
 Delta R.T.: -0.002 min  
 Response: 134430740  
 Conc: 1117.01 ng/ml

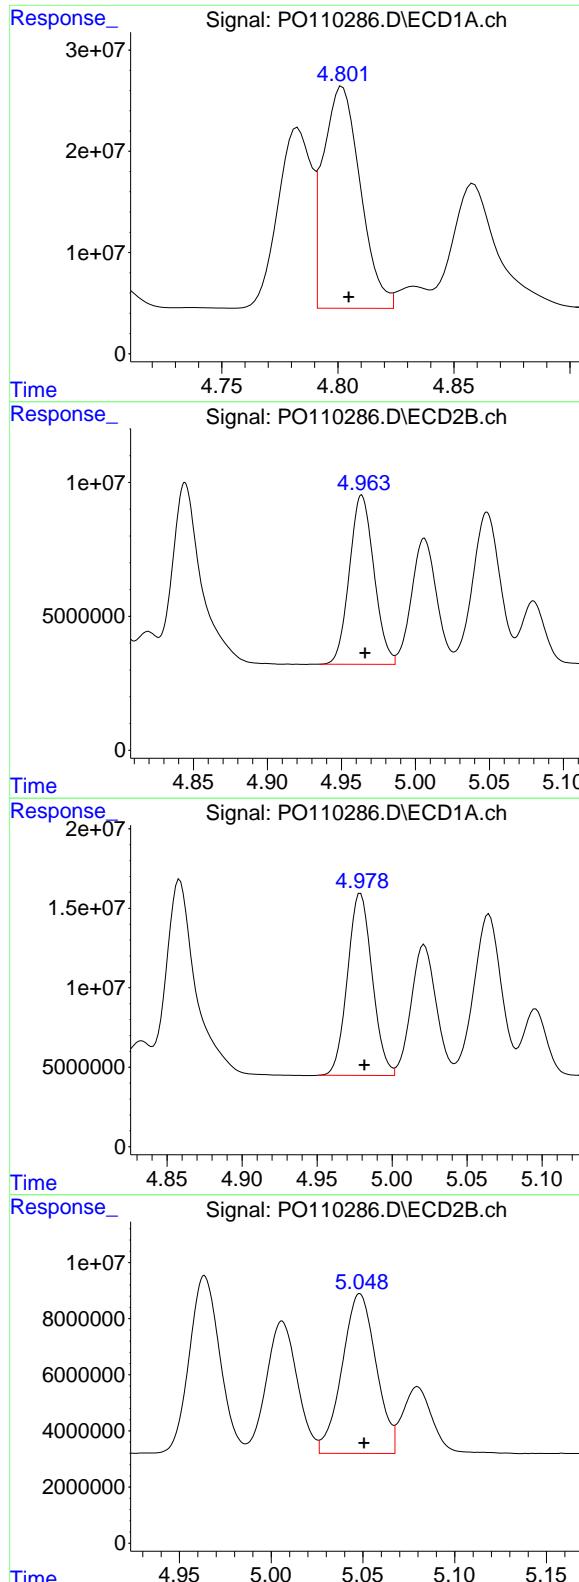

#13 AR-1232-3

R.T.: 4.802 min  
 Delta R.T.: -0.003 min  
**Instrument:**  
 Response: 244109403  
 Conc: 1152.66 ng/ml  
**ClientSampleId :**  
 AR1660CCC500

#13 AR-1232-3


R.T.: 4.964 min  
 Delta R.T.: -0.002 min  
 Response: 73038464  
 Conc: 1147.39 ng/ml

#14 AR-1232-4

R.T.: 4.979 min  
 Delta R.T.: -0.003 min  
 Response: 131142472  
 Conc: 1154.82 ng/ml

#14 AR-1232-4


R.T.: 5.048 min  
 Delta R.T.: -0.002 min  
 Response: 73350252  
 Conc: 1236.08 ng/ml

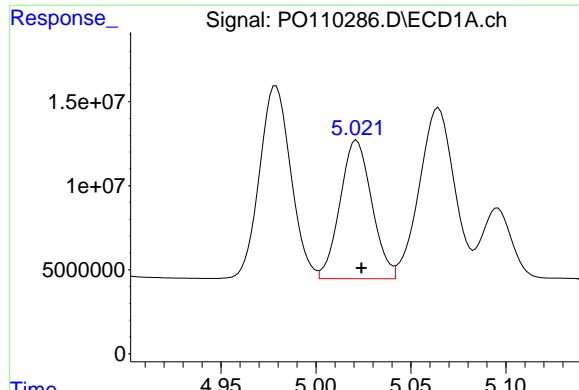

#15 AR-1232-5


R.T.: 5.021 min  
 Delta R.T.: -0.002 min  
 Response: 95769846  
 Conc: 1190.37 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

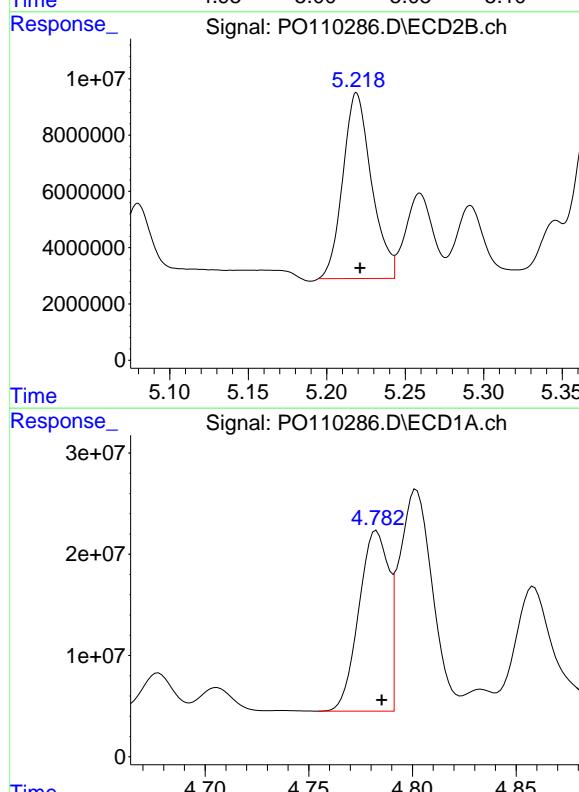


#16 AR-1242-1

R.T.: 4.783 min  
 Delta R.T.: -0.002 min  
 Response: 177801623  
 Conc: 664.91 ng/ml

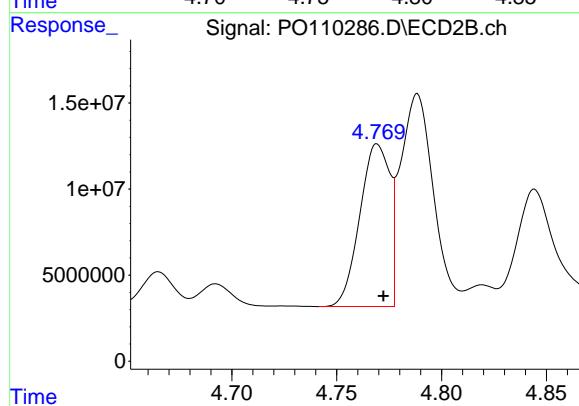

#16 AR-1242-1

R.T.: 4.769 min  
 Delta R.T.: -0.003 min  
 Response: 93902896  
 Conc: 642.22 ng/ml

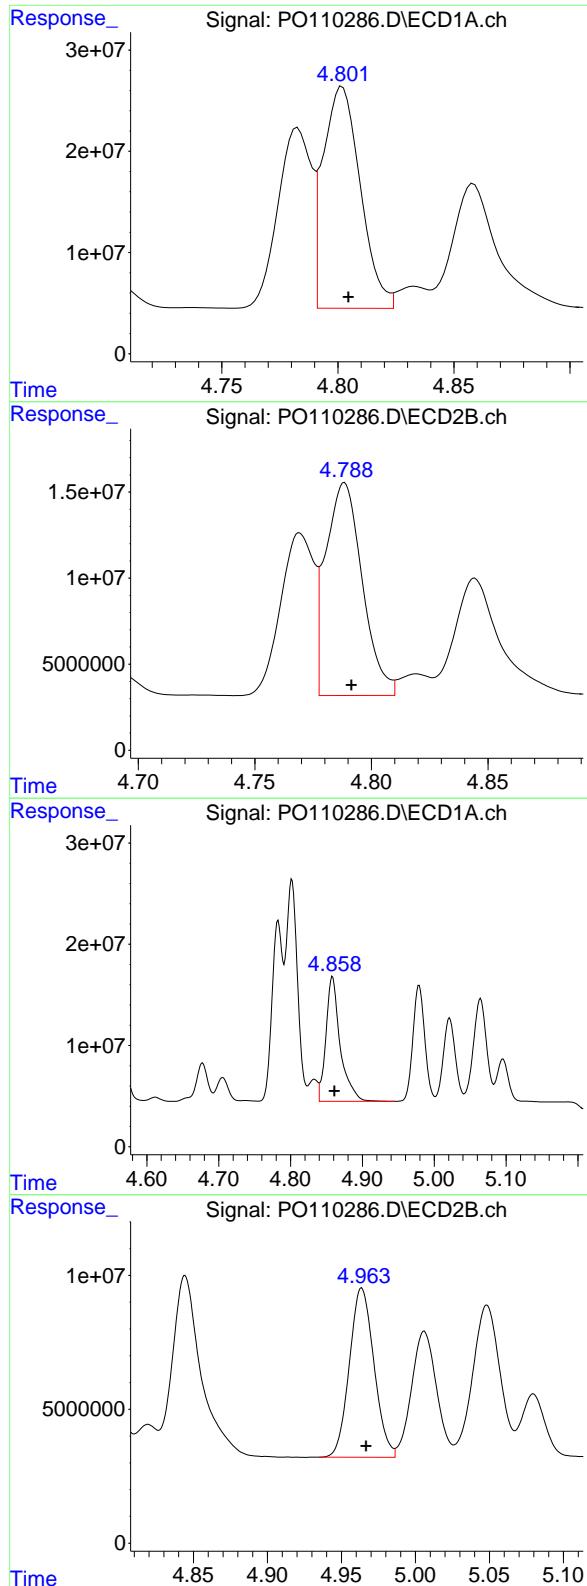

#17 AR-1242-2

R.T.: 4.802 min  
 Delta R.T.: -0.003 min  
 Response: 244109403  
 Conc: 662.97 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#17 AR-1242-2


R.T.: 4.788 min  
 Delta R.T.: -0.003 min  
 Response: 134430740  
 Conc: 646.19 ng/ml

#18 AR-1242-3

R.T.: 4.858 min  
 Delta R.T.: -0.003 min  
 Response: 169708224  
 Conc: 657.91 ng/ml

#18 AR-1242-3

R.T.: 4.964 min  
 Delta R.T.: -0.003 min  
 Response: 73038464  
 Conc: 654.39 ng/ml

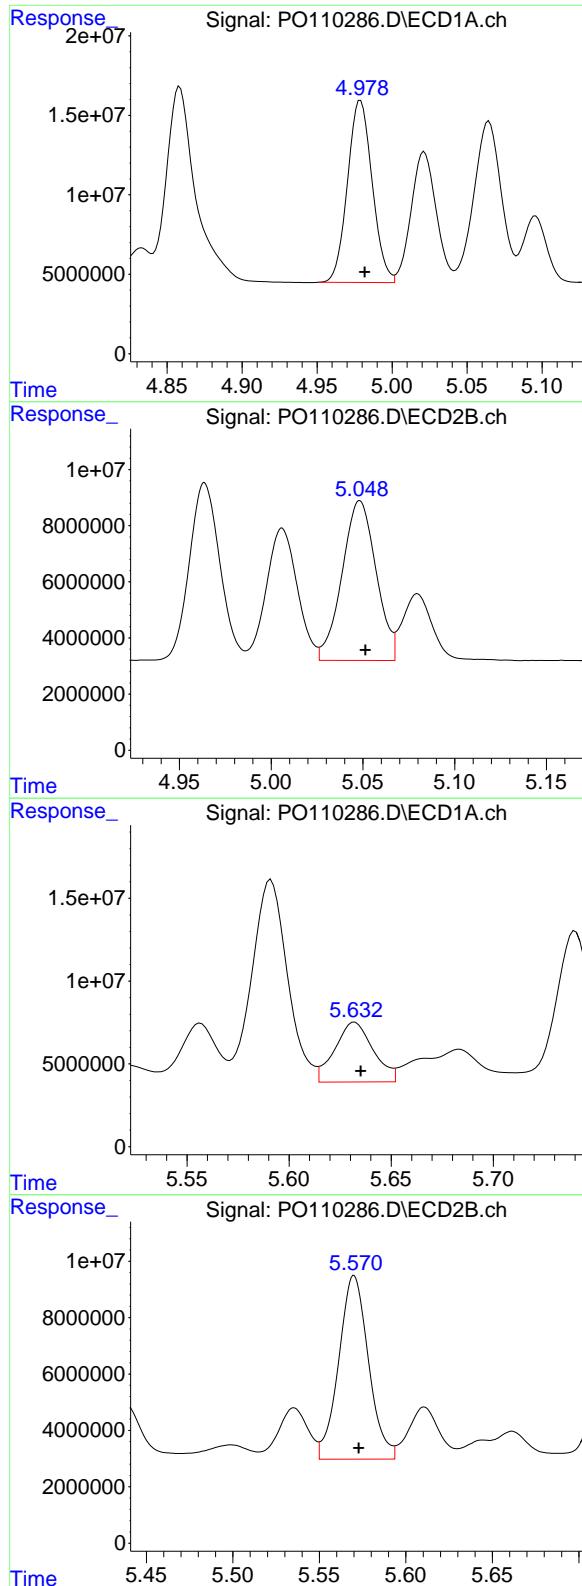

#19 AR-1242-4

R.T.: 4.979 min  
 Delta R.T.: -0.003 min  
 Response: 131142472  
 Conc: 655.40 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#19 AR-1242-4


R.T.: 5.048 min  
 Delta R.T.: -0.003 min  
 Response: 73350252  
 Conc: 632.46 ng/ml

#20 AR-1242-5

R.T.: 5.632 min  
 Delta R.T.: -0.003 min  
 Response: 47210124  
 Conc: 223.69 ng/ml

#20 AR-1242-5

R.T.: 5.570 min  
 Delta R.T.: -0.003 min  
 Response: 77845170  
 Conc: 567.21 ng/ml

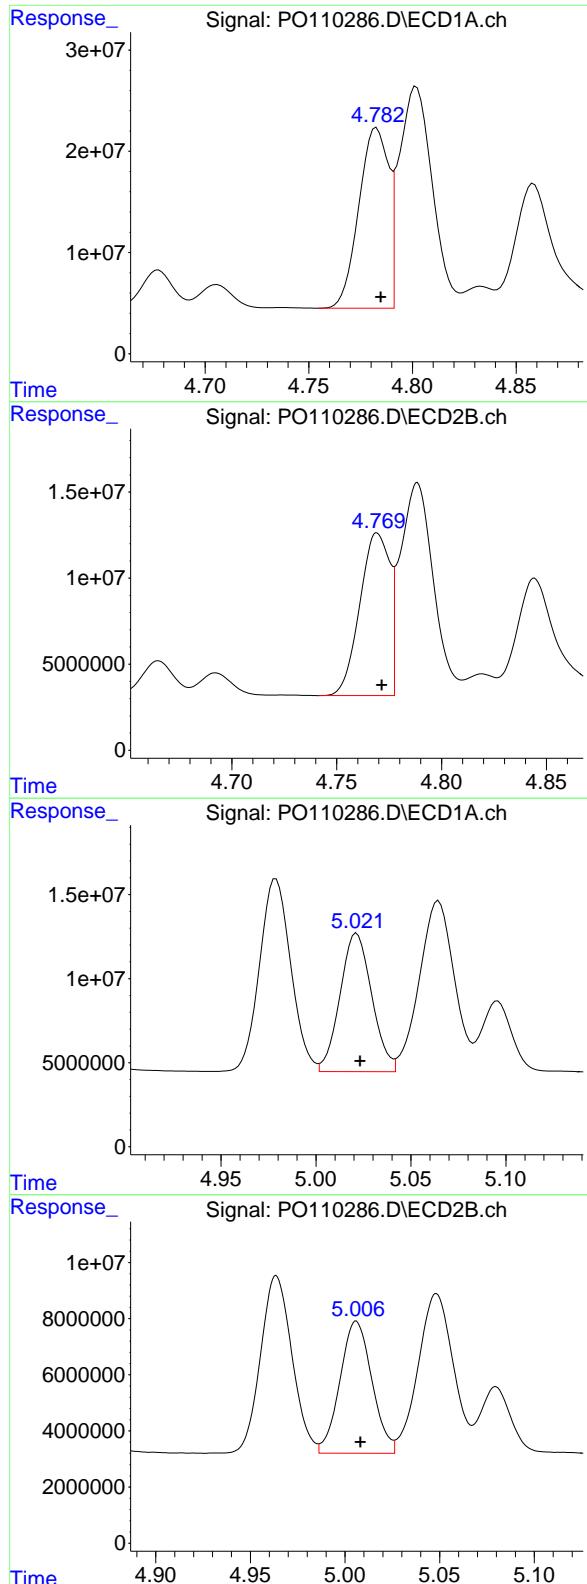

#21 AR-1248-1

R.T.: 4.783 min  
 Delta R.T.: -0.002 min  
 Response: 177801623  
 Conc: 806.42 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#21 AR-1248-1


R.T.: 4.769 min  
 Delta R.T.: -0.002 min  
 Response: 93902896  
 Conc: 772.63 ng/ml

#22 AR-1248-2

R.T.: 5.021 min  
 Delta R.T.: -0.002 min  
 Response: 95769846  
 Conc: 317.97 ng/ml

#22 AR-1248-2


R.T.: 5.006 min  
 Delta R.T.: -0.002 min  
 Response: 55338718  
 Conc: 328.50 ng/ml

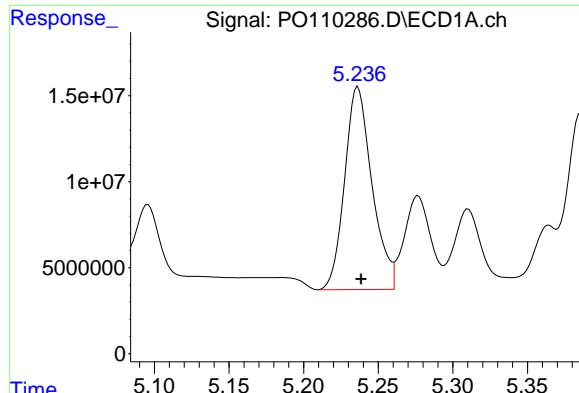

#23 AR-1248-3


R.T.: 5.236 min  
 Delta R.T.: -0.002 min  
 Response: 150479994  
 Conc: 403.23 ng/ml

Instrument : ECD\_O  
 ClientSampleId : AR1660CCC500

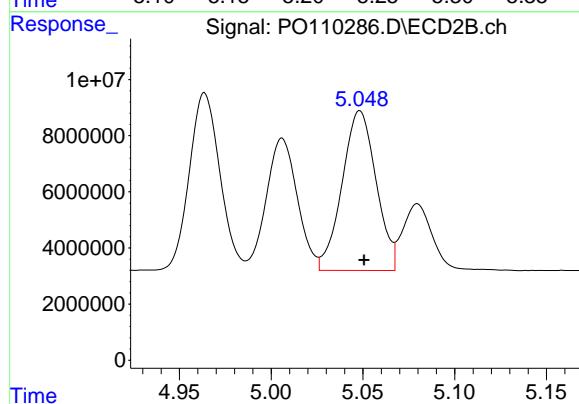


#23 AR-1248-3

R.T.: 5.048 min  
 Delta R.T.: -0.002 min  
 Response: 73350252  
 Conc: 404.83 ng/ml

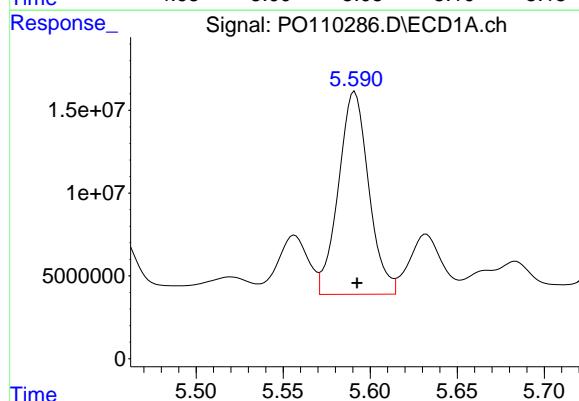


#24 AR-1248-4

R.T.: 5.591 min  
 Delta R.T.: -0.001 min  
 Response: 148547870  
 Conc: 281.33 ng/ml

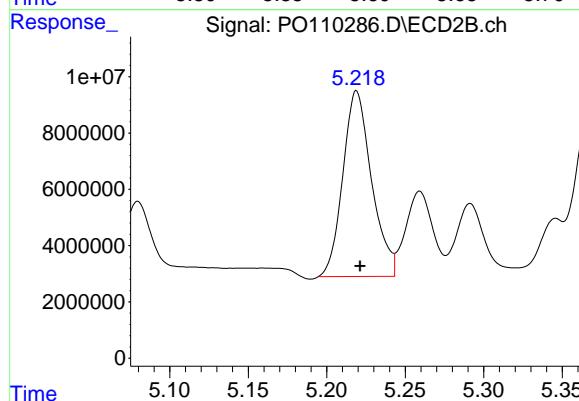

#24 AR-1248-4

R.T.: 5.219 min  
 Delta R.T.: -0.002 min  
 Response: 83969338  
 Conc: 398.98 ng/ml

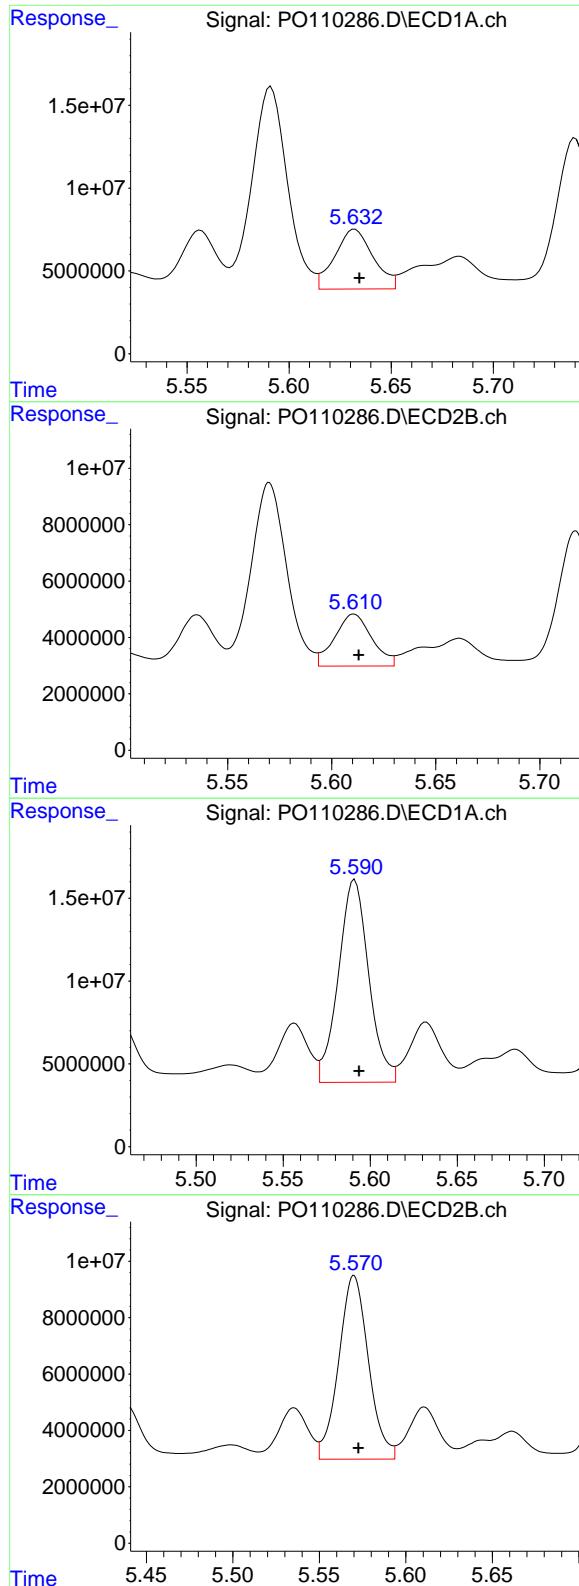

#25 AR-1248-5

R.T.: 5.632 min  
 Delta R.T.: -0.002 min  
 Response: 47210124  
 Conc: 126.59 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#25 AR-1248-5


R.T.: 5.611 min  
 Delta R.T.: -0.002 min  
 Response: 22863074  
 Conc: 109.99 ng/ml

#26 AR-1254-1

R.T.: 5.591 min  
 Delta R.T.: -0.002 min  
 Response: 148547870  
 Conc: 262.80 ng/ml

#26 AR-1254-1

R.T.: 5.570 min  
 Delta R.T.: -0.003 min  
 Response: 77845170  
 Conc: 248.95 ng/ml

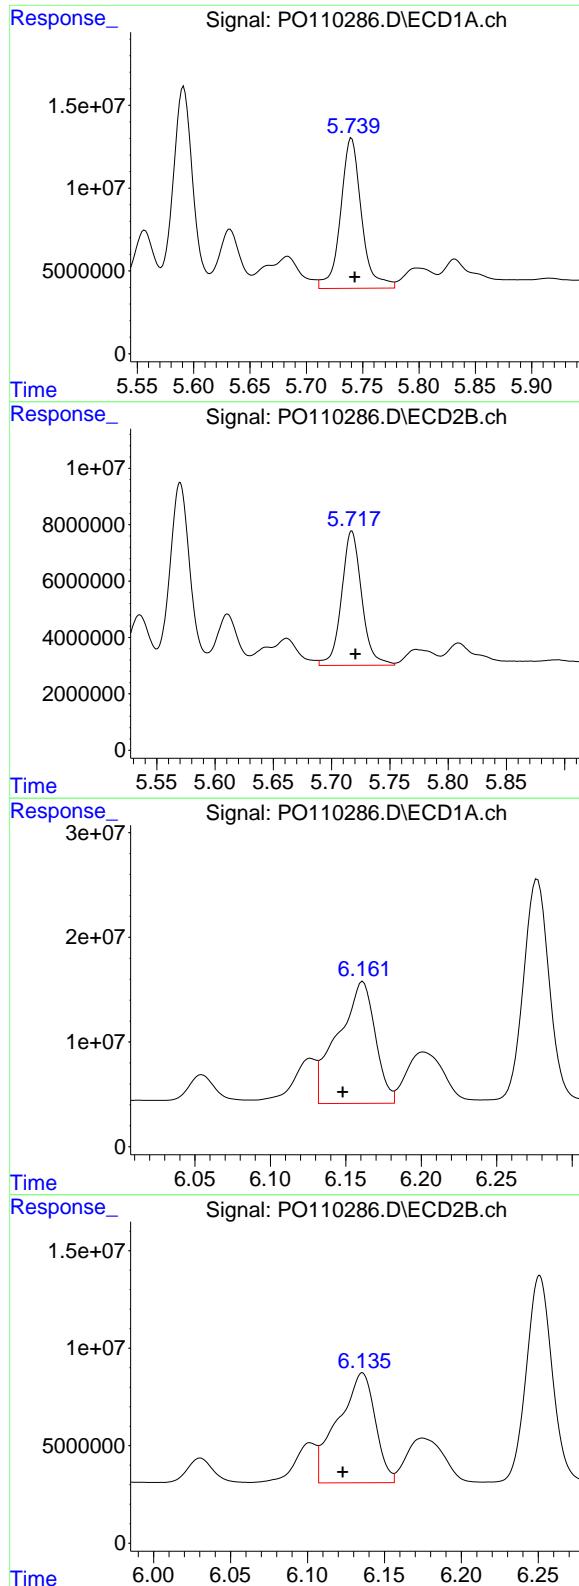

#27 AR-1254-2

R.T.: 5.740 min  
 Delta R.T.: -0.003 min  
 Response: 117101241  
 Conc: 243.33 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#27 AR-1254-2


R.T.: 5.717 min  
 Delta R.T.: -0.003 min  
 Response: 57497390  
 Conc: 211.75 ng/ml

#28 AR-1254-3

R.T.: 6.161 min  
 Delta R.T.: 0.013 min  
 Response: 199842623  
 Conc: 258.50 ng/ml

#28 AR-1254-3

R.T.: 6.136 min  
 Delta R.T.: 0.013 min  
 Response: 94798356  
 Conc: 228.19 ng/ml

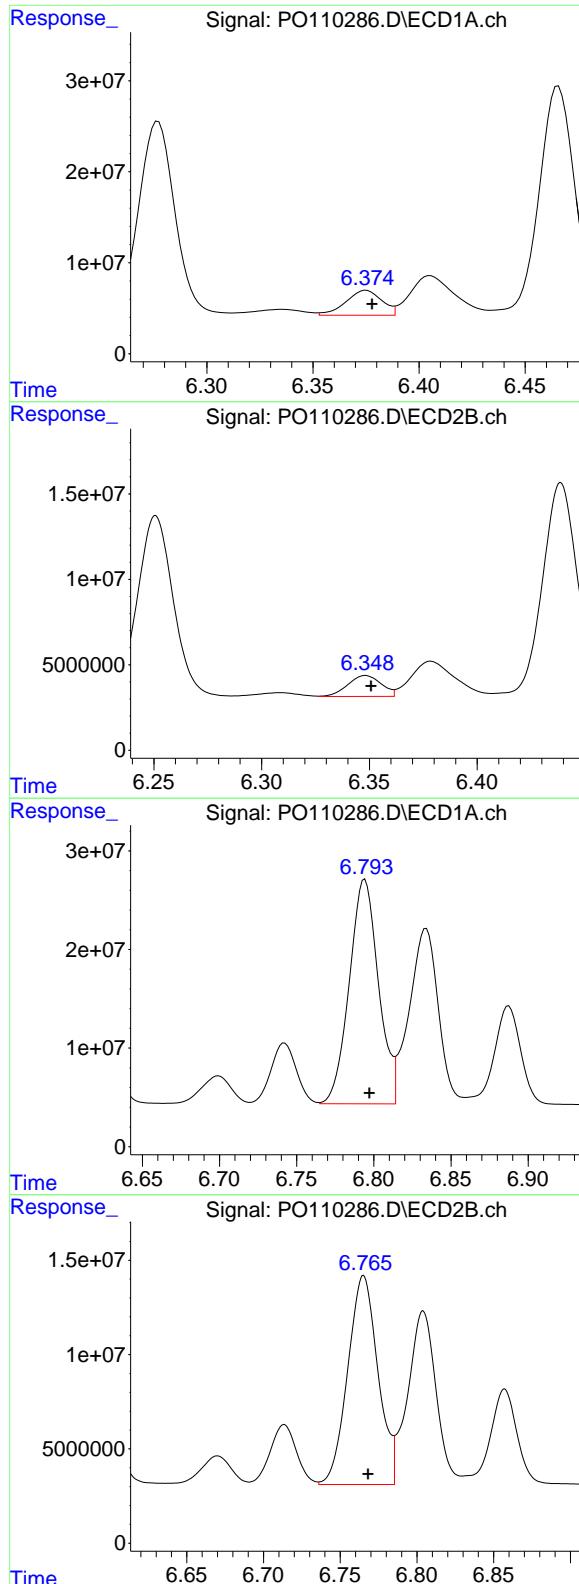

#29 AR-1254-4

R.T.: 6.375 min  
 Delta R.T.: -0.003 min  
 Response: 32159525  
 Conc: 66.98 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#29 AR-1254-4


R.T.: 6.348 min  
 Delta R.T.: -0.003 min  
 Response: 13331170  
 Conc: 54.96 ng/ml

#30 AR-1254-5

R.T.: 6.794 min  
 Delta R.T.: -0.003 min  
 Response: 299018131  
 Conc: 459.92 ng/ml

#30 AR-1254-5

R.T.: 6.765 min  
 Delta R.T.: -0.003 min  
 Response: 151977984  
 Conc: 452.45 ng/ml

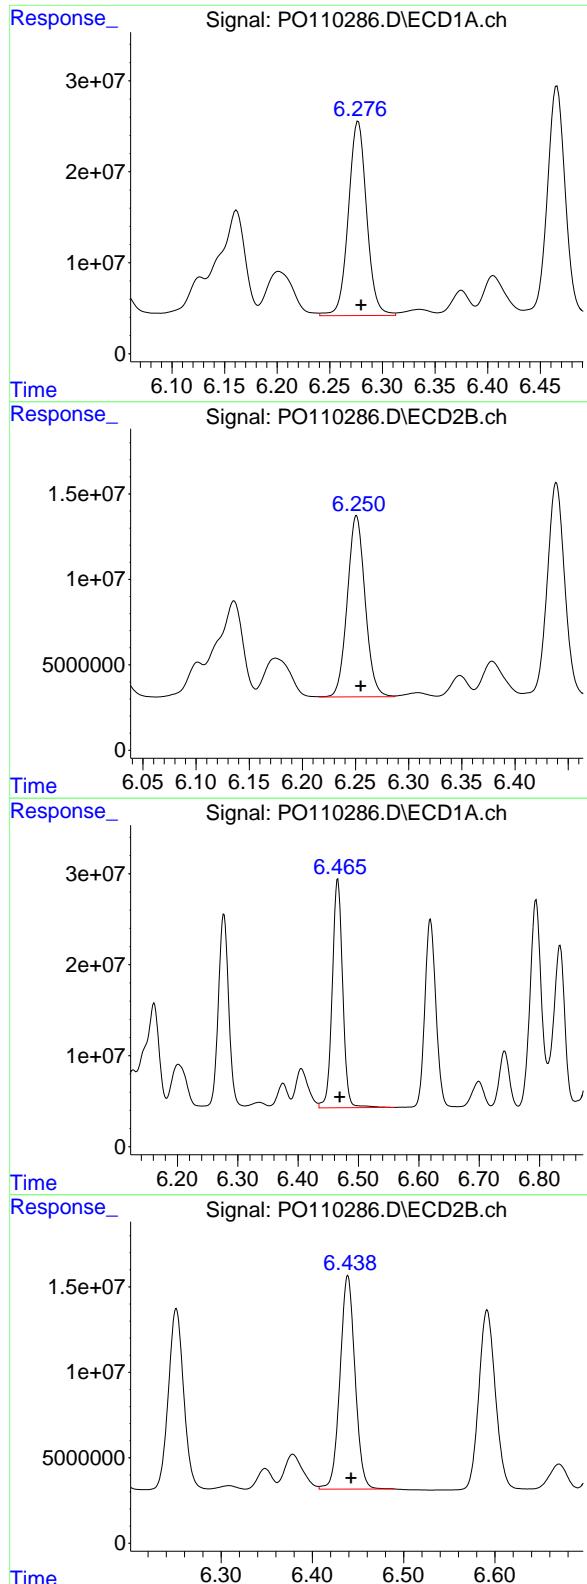

#31 AR-1260-1

R.T.: 6.277 min  
 Delta R.T.: -0.003 min  
 Response: 259319565  
 Conc: 550.16 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#31 AR-1260-1


R.T.: 6.251 min  
 Delta R.T.: -0.004 min  
 Response: 123473695  
 Conc: 483.37 ng/ml

#32 AR-1260-2

R.T.: 6.466 min  
 Delta R.T.: -0.003 min  
 Response: 302763163  
 Conc: 508.40 ng/ml

#32 AR-1260-2


R.T.: 6.439 min  
 Delta R.T.: -0.004 min  
 Response: 143289838  
 Conc: 477.18 ng/ml

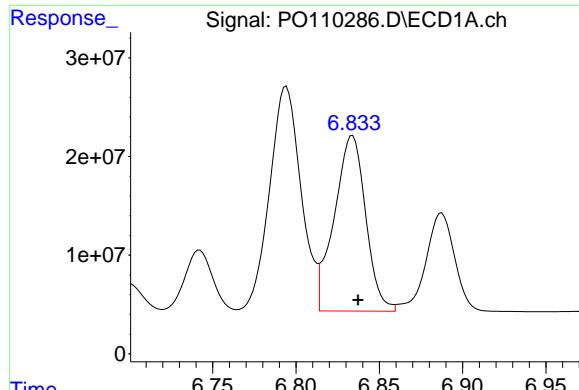

#33 AR-1260-3


R.T.: 6.834 min  
 Delta R.T.: -0.003 min  
 Response: 233791087  
 Conc: 481.74 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

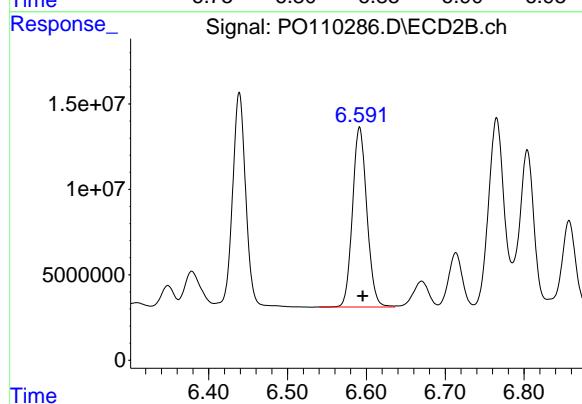


#33 AR-1260-3

R.T.: 6.591 min  
 Delta R.T.: -0.004 min  
 Response: 133557256  
 Conc: 462.16 ng/ml

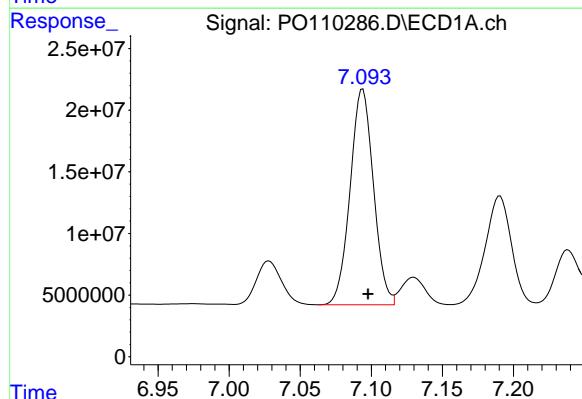


#34 AR-1260-4

R.T.: 7.094 min  
 Delta R.T.: -0.004 min  
 Response: 199989246  
 Conc: 471.49 ng/ml

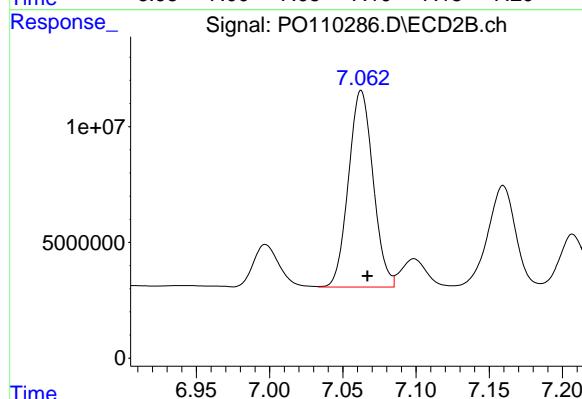

#34 AR-1260-4

R.T.: 7.063 min  
 Delta R.T.: -0.004 min  
 Response: 99360275  
 Conc: 461.97 ng/ml

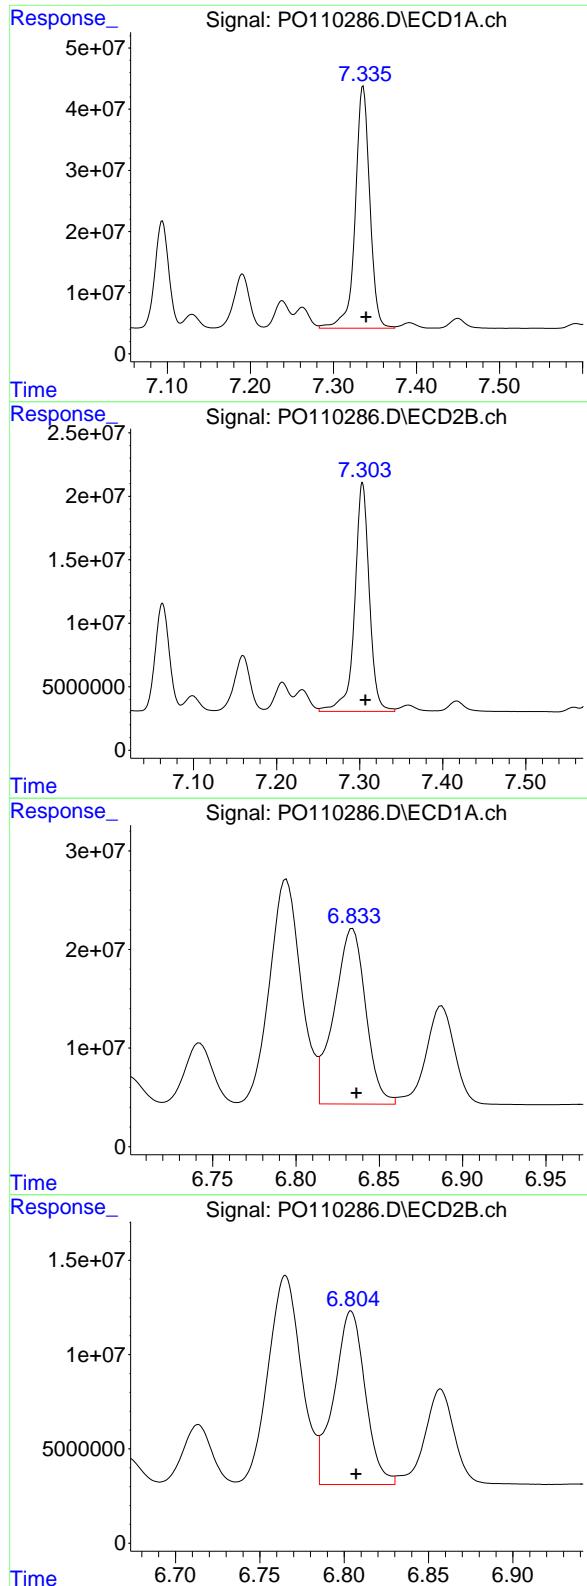

#35 AR-1260-5

R.T.: 7.336 min  
Delta R.T.: -0.004 min  
Response: 484140405  
Conc: 462.92 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#35 AR-1260-5


R.T.: 7.303 min  
Delta R.T.: -0.004 min  
Response: 221673295  
Conc: 444.51 ng/ml

#36 AR-1262-1

R.T.: 6.834 min  
Delta R.T.: -0.002 min  
Response: 233791087  
Conc: 339.75 ng/ml

#36 AR-1262-1

R.T.: 6.804 min  
Delta R.T.: -0.003 min  
Response: 118057901  
Conc: 342.88 ng/ml

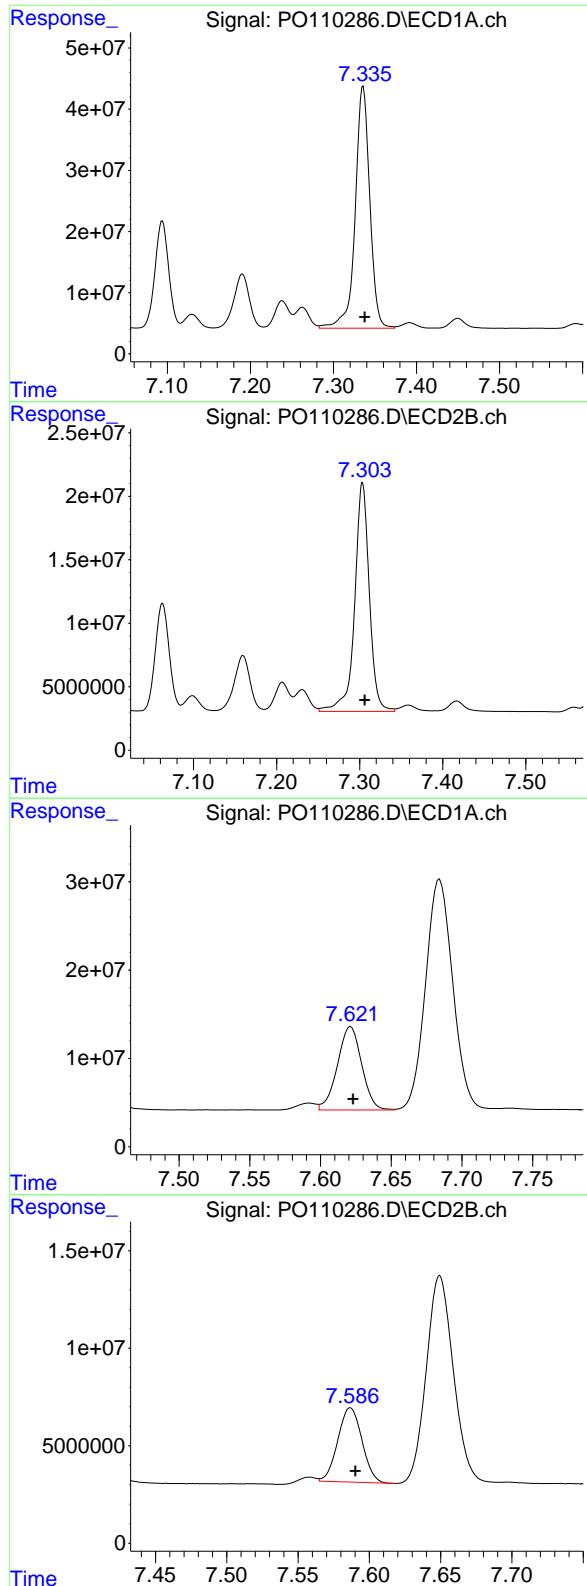

#37 AR-1262-2

R.T.: 7.336 min  
 Delta R.T.: -0.002 min  
 Response: 484140405  
 Conc: 406.17 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#37 AR-1262-2


R.T.: 7.303 min  
 Delta R.T.: -0.003 min  
 Response: 221673295  
 Conc: 412.63 ng/ml

#38 AR-1262-3

R.T.: 7.621 min  
 Delta R.T.: -0.002 min  
 Response: 112676982  
 Conc: 239.42 ng/ml

#38 AR-1262-3

R.T.: 7.587 min  
 Delta R.T.: -0.003 min  
 Response: 45025623  
 Conc: 232.03 ng/ml

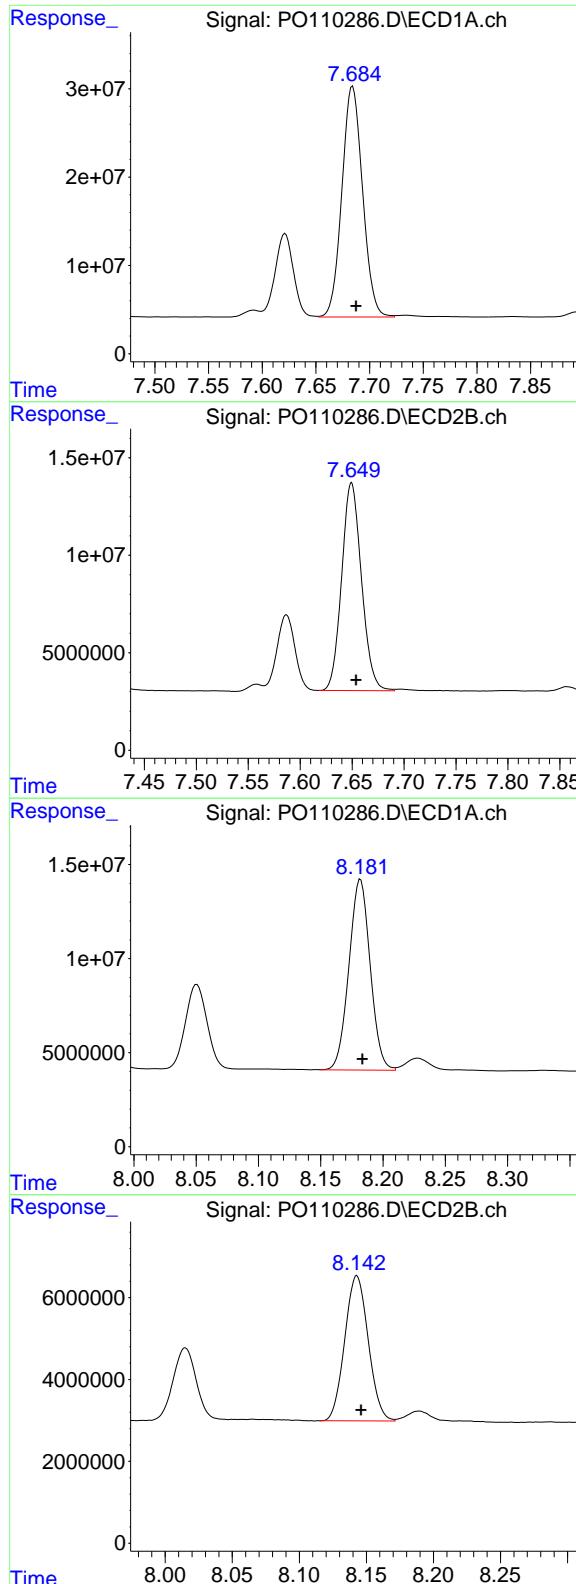

#39 AR-1262-4

R.T.: 7.684 min  
 Delta R.T.: -0.003 min  
 Response: 350265107  
 Conc: 400.50 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#39 AR-1262-4


R.T.: 7.649 min  
 Delta R.T.: -0.004 min  
 Response: 141651763  
 Conc: 391.53 ng/ml

#40 AR-1262-5

R.T.: 8.182 min  
 Delta R.T.: -0.002 min  
 Response: 121020918  
 Conc: 306.82 ng/ml

#40 AR-1262-5

R.T.: 8.143 min  
 Delta R.T.: -0.003 min  
 Response: 43223300  
 Conc: 306.20 ng/ml

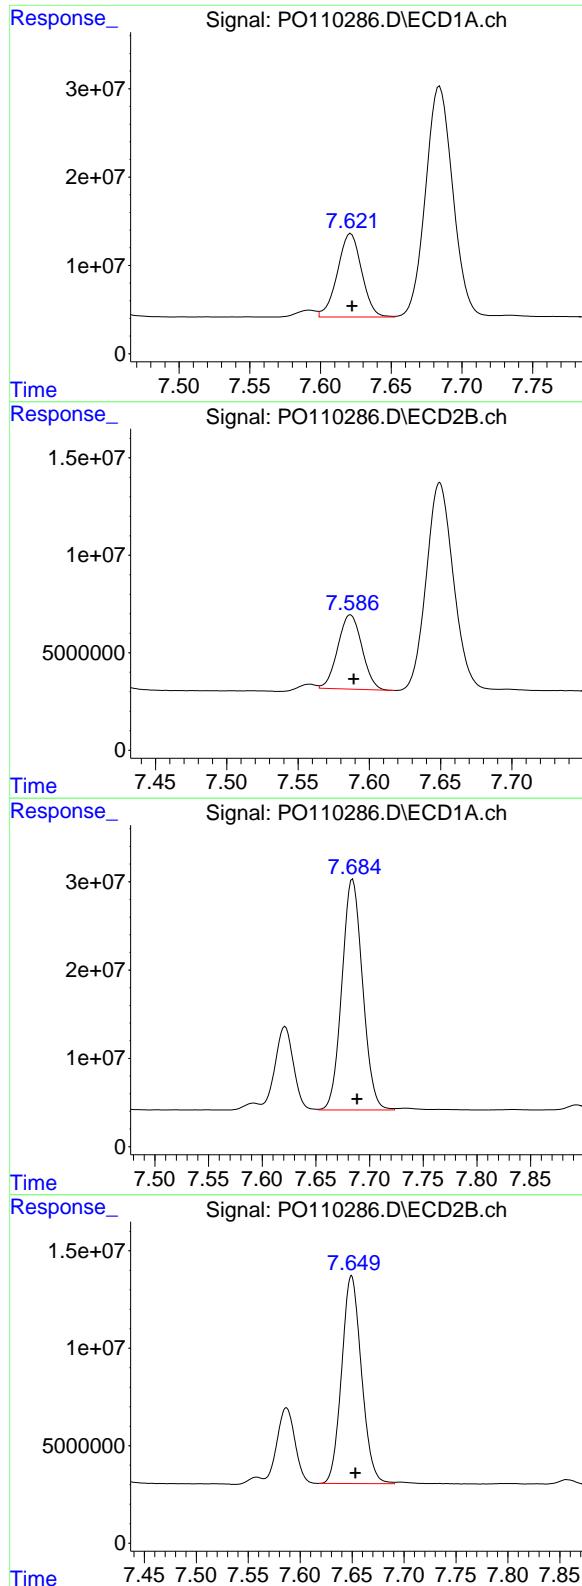

#41 AR-1268-1

R.T.: 7.621 min  
 Delta R.T.: 0.000 min  
 Response: 112676982  
 Conc: 80.48 ng/ml

**Instrument:** ECD\_O  
**ClientSampleId:** AR1660CCC500

#41 AR-1268-1


R.T.: 7.587 min  
 Delta R.T.: -0.002 min  
 Response: 45025623  
 Conc: 76.92 ng/ml

#42 AR-1268-2

R.T.: 7.684 min  
 Delta R.T.: -0.004 min  
 Response: 350265107  
 Conc: 273.61 ng/ml

#42 AR-1268-2

R.T.: 7.649 min  
 Delta R.T.: -0.004 min  
 Response: 141651763  
 Conc: 263.47 ng/ml

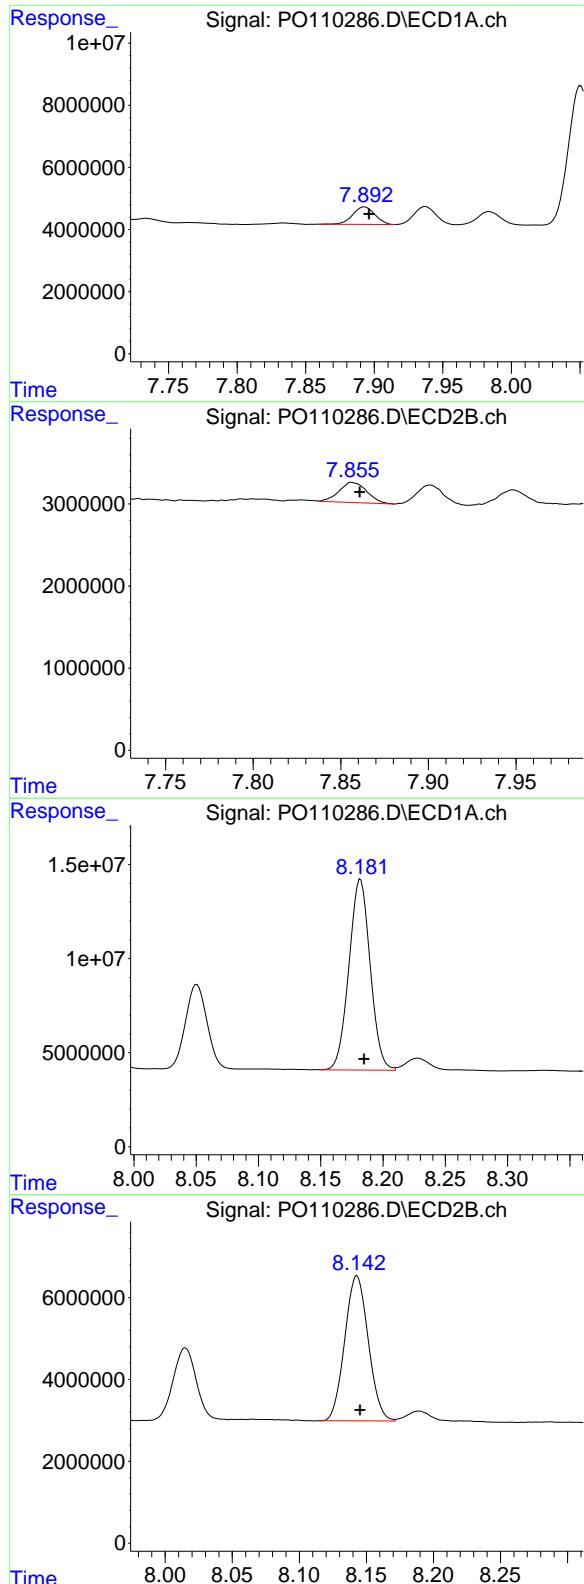

#43 AR-1268-3

R.T.: 7.893 min  
 Delta R.T.: -0.003 min  
 Response: 6384140  
 Conc: 6.21 ng/ml

Instrument: ECD\_O  
 ClientSampleId: AR1660CCC500

#43 AR-1268-3


R.T.: 7.857 min  
 Delta R.T.: -0.004 min  
 Response: 2701969  
 Conc: 6.50 ng/ml

#44 AR-1268-4

R.T.: 8.182 min  
 Delta R.T.: -0.003 min  
 Response: 121020918  
 Conc: 273.81 ng/ml

#44 AR-1268-4

R.T.: 8.143 min  
 Delta R.T.: -0.002 min  
 Response: 43223300  
 Conc: 268.40 ng/ml

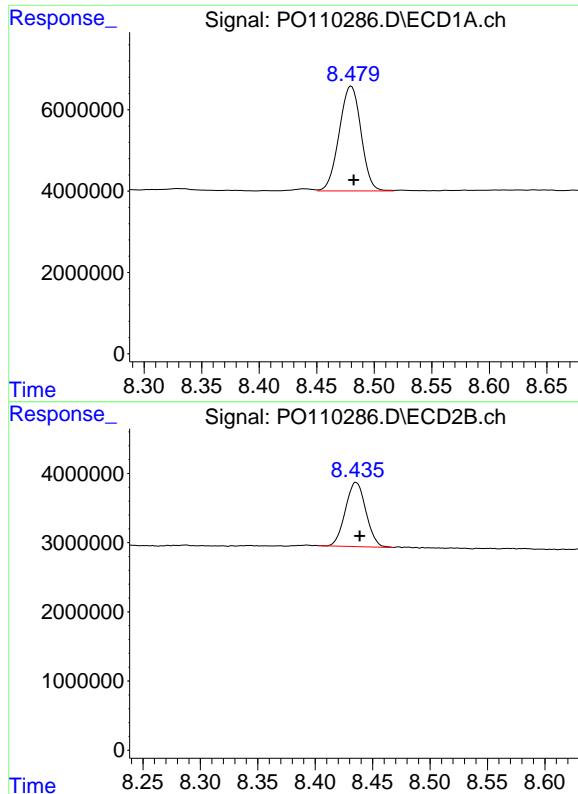

#45 AR-1268-5

R.T.: 8.480 min  
Delta R.T.: -0.002 min  
Response: 34068238  
Conc: 10.71 ng/ml

Instrument: ECD\_O  
ClientSampleId: AR1660CCC500

#45 AR-1268-5

R.T.: 8.436 min  
Delta R.T.: -0.003 min  
Response: 11602754  
Conc: 11.68 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:19  
 Operator : YP\AJ  
 Sample : AR1660ICC250  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 31 03:02:22 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.515	3.816	39892911	28120307	27.294	27.126
2) SA Decachlor...	10.229	8.859	27877719	18839232	26.484	23.902

Target Compounds

3) L1 AR-1016-1	5.667	4.903	13581167	11323714	267.076	282.470
4) L1 AR-1016-2	5.689	4.922	20108471	16375760	257.624	282.999
5) L1 AR-1016-3	5.751	5.099	12212490	8877034	258.878	287.066
6) L1 AR-1016-4	5.848	5.141	9803037	7158830	266.708	293.926
7) L1 AR-1016-5	6.141	5.355	9152735	9323046	269.896	288.450
8) L2 AR-1221-1	4.717	4.026	1321625	1122384	76.158	73.630
9) L2 AR-1221-2	4.802	4.115	2090814	1735253	161.416	151.732
10) L2 AR-1221-3	4.877	4.190	7052777	6326573	169.061	185.590
11) L3 AR-1232-1	4.877	4.190	7052777	6326573	211.867	226.056
12) L3 AR-1232-2	5.402	4.922	9379837	16375760	589.544	583.574
13) L3 AR-1232-3	5.689	5.099	20108471	8877034	586.759	596.191
14) L3 AR-1232-4	5.848	5.183	9803037	8604427	624.096	671.992
15) L3 AR-1232-5	5.939	5.355	7957300	9323046	747.842	657.721
16) L4 AR-1242-1	5.667	4.903	13581167	11323714	308.823	331.143
17) L4 AR-1242-2	5.689	4.922	20108471	16375760	312.650	332.451
18) L4 AR-1242-3	5.751	5.099	12212490	8877034	297.579	333.169
19) L4 AR-1242-4	5.848	5.183	9803037	8604427	321.165	326.194
20) L4 AR-1242-5	6.579	5.708	4761571	8766943	130.417	283.186 #
21) L5 AR-1248-1	5.667	4.903	13581167	11323714	374.266	418.158
22) L5 AR-1248-2	5.939	5.141	7957300	7158830	177.071	194.944
23) L5 AR-1248-3	6.141	5.183	9152735	8604427	180.750	222.570
24) L5 AR-1248-4	6.539	5.355	4049391	9323046	63.126	206.532 #
25) L5 AR-1248-5	6.579	5.749	4761571	2416322	78.256	56.617 #
26) L6 AR-1254-1	6.515	5.708	10069870	8766943	156.388	132.797
27) L6 AR-1254-2	6.731	5.856	10106718	6407649	99.977	112.222
28) L6 AR-1254-3	7.094	6.276	7072472	11091003	70.918	127.716 #
29) L6 AR-1254-4	7.379	6.489	4686448	1684678	54.118	30.030 #
30) L6 AR-1254-5	7.792	6.906	26750553	17034582	332.921	236.097 #
31) L7 AR-1260-1	7.260	6.391	18182257	14056672	270.759	274.511
32) L7 AR-1260-2	7.513	6.579	26780079	17295947	278.563	271.122
33) L7 AR-1260-3	7.871	6.733	23122222	14684885	289.324	269.513
34) L7 AR-1260-4	8.095	7.205	23709378	12488782	301.122	261.128
35) L7 AR-1260-5	8.415	7.446	43743345	31815782	275.313	255.527
36) L8 AR-1262-1	8.095	6.945	23709378	15226146	223.042	177.951
37) L8 AR-1262-2	8.415	7.205	43743345	12488782	220.500	182.413
38) L8 AR-1262-3	8.737	7.728	26257171	6907710	199.308	113.757 #
39) L8 AR-1262-4	8.806	7.792	15776574	20963428	165.001	210.885 #
40) L8 AR-1262-5	9.472	8.293	11555188	7670514	177.591	163.649
41) L9 AR-1268-1	8.737	7.728	26257171	6907710	111.492	40.301 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:19  
 Operator : YP\AJ  
 Sample : AR1660ICC250  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 31 03:02:22 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	8.806	7.792	15776574	20963428	80.775	146.308 #
43) L9 AR-1268-3	0.000	8.001	0	412782	N.D.	3.352 #
44) L9 AR-1268-4	9.472	8.293	11555188	7670514	163.331	145.239
45) L9 AR-1268-5	9.890	8.596	2482779	969431	5.214	2.679 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:19  
 Operator : YP\AJ  
 Sample : AR1660ICC250  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 31 03:02:22 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

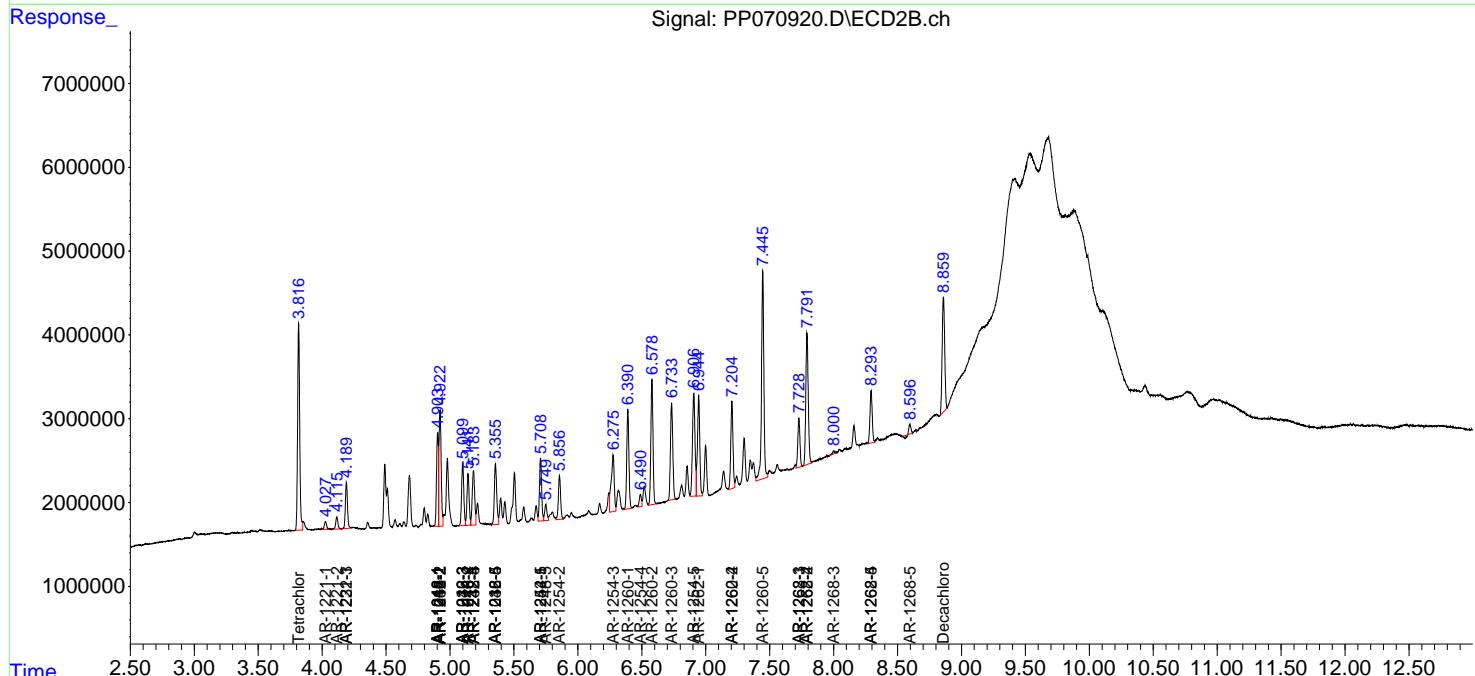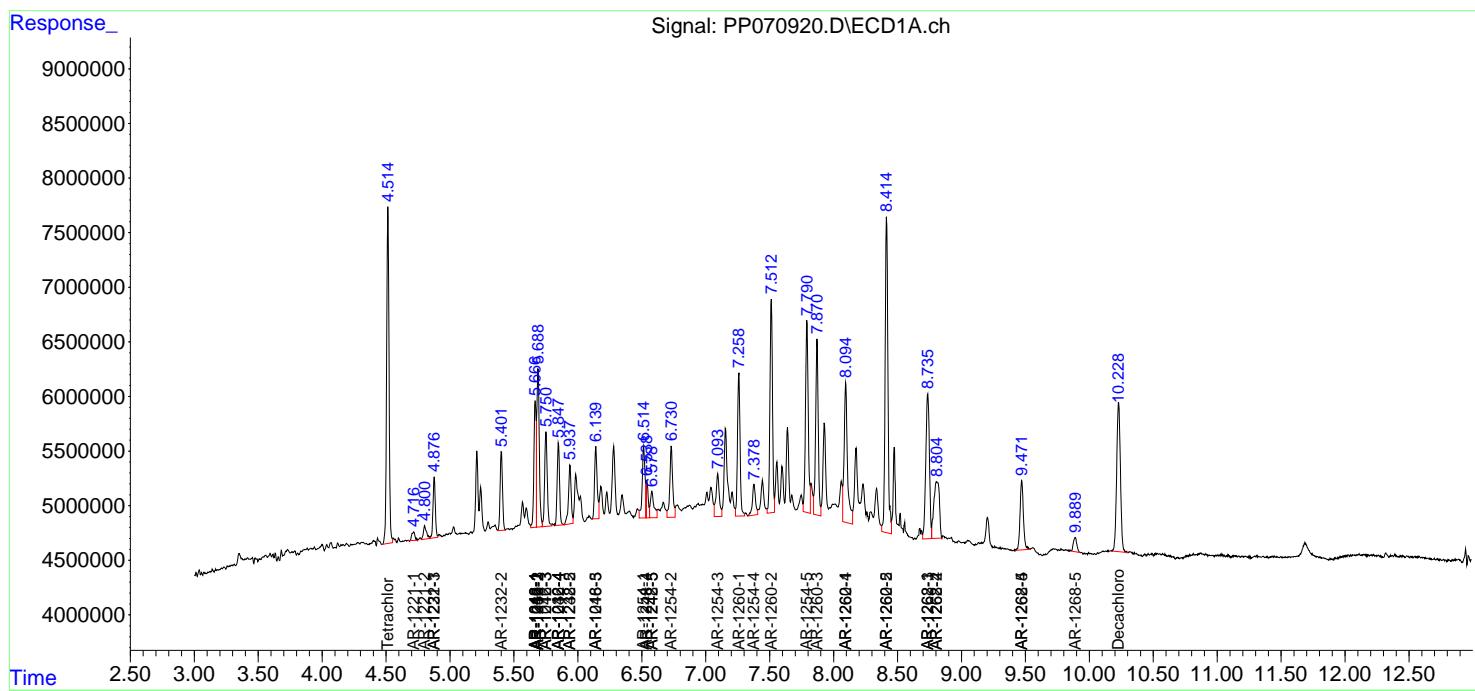

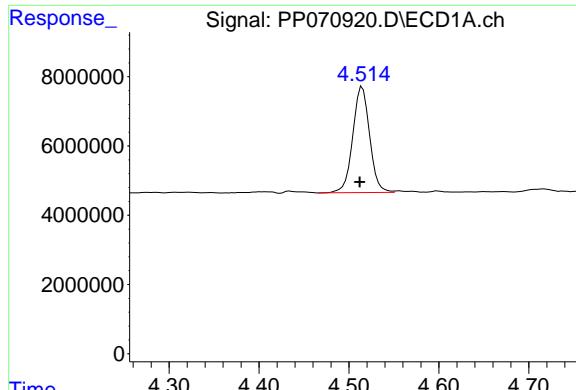

#1 Tetrachloro-m-xylene


R.T.: 4.515 min  
Delta R.T.: 0.003 min  
Response: 39892911  
Conc: 27.29 ng/ml

Instrument:

ECD\_P


ClientSampleId :

AR1660ICC250

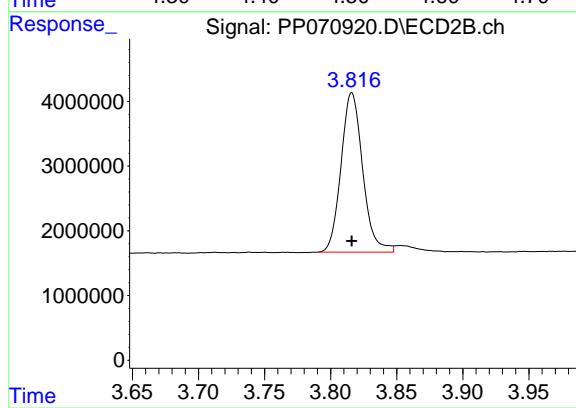


#1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 28120307  
Conc: 27.13 ng/ml

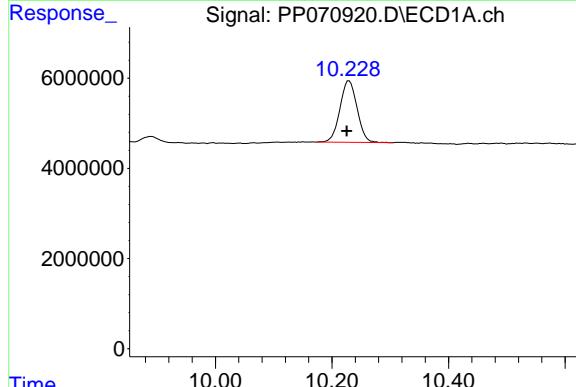


#2 Decachlorobiphenyl

R.T.: 10.229 min  
Delta R.T.: 0.004 min  
Response: 27877719  
Conc: 26.48 ng/ml

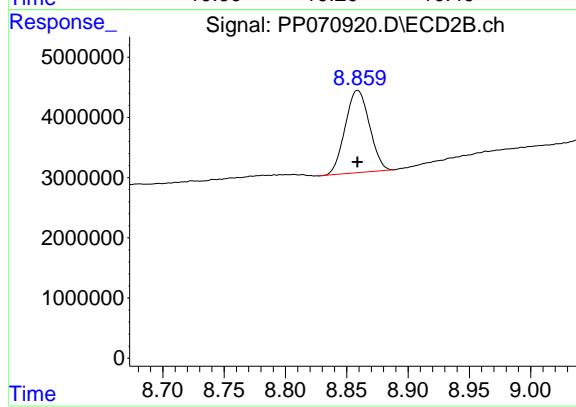

#2 Decachlorobiphenyl


R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 18839232  
Conc: 23.90 ng/ml

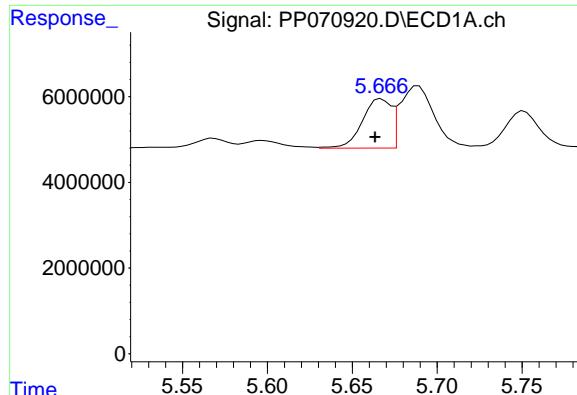

#3 AR-1016-1


R.T.: 5.667 min  
 Delta R.T.: 0.004 min  
 Response: 13581167  
 Conc: 267.08 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

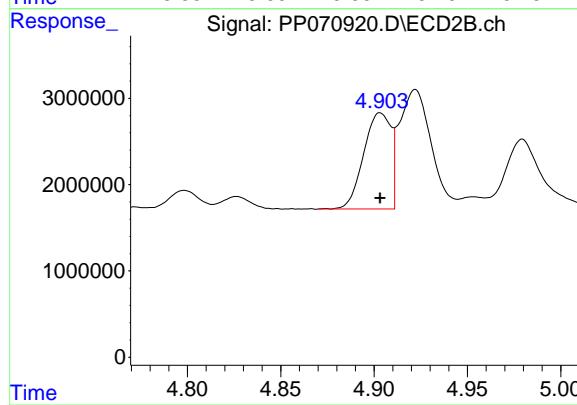


#3 AR-1016-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 11323714  
 Conc: 282.47 ng/ml

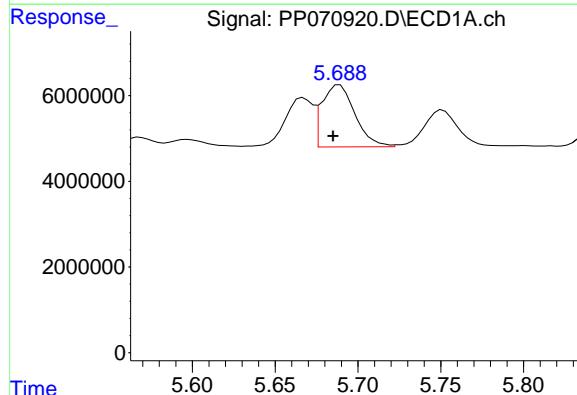


#4 AR-1016-2

R.T.: 5.689 min  
 Delta R.T.: 0.004 min  
 Response: 20108471  
 Conc: 257.62 ng/ml

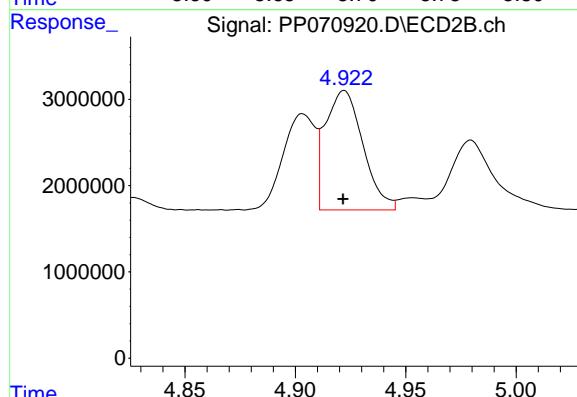

#4 AR-1016-2


R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 16375760  
 Conc: 283.00 ng/ml

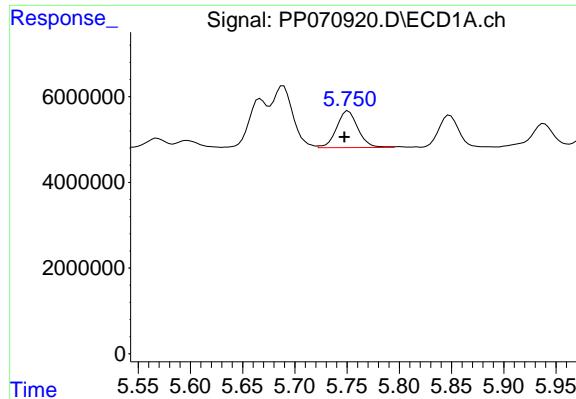

#5 AR-1016-3


R.T.: 5.751 min  
Delta R.T.: 0.004 min  
Response: 12212490  
Conc: 258.88 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660ICC250

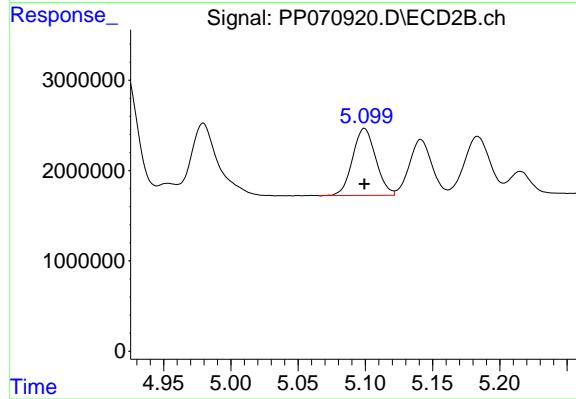


#5 AR-1016-3

R.T.: 5.099 min  
Delta R.T.: 0.000 min  
Response: 8877034  
Conc: 287.07 ng/ml

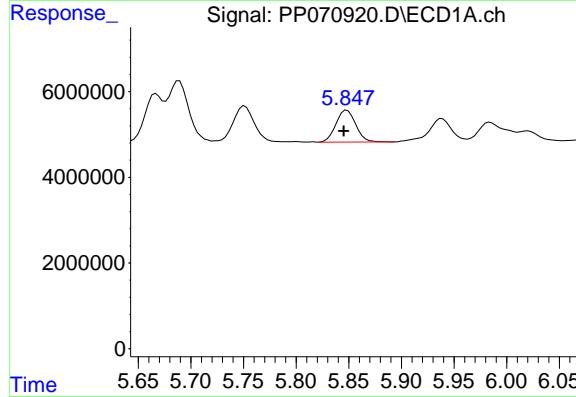


#6 AR-1016-4

R.T.: 5.848 min  
Delta R.T.: 0.003 min  
Response: 9803037  
Conc: 266.71 ng/ml

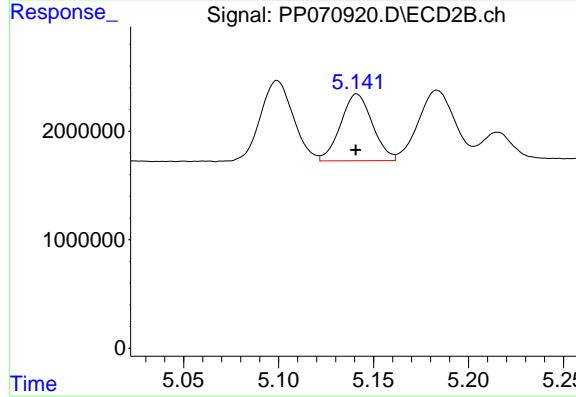

#6 AR-1016-4

R.T.: 5.141 min  
Delta R.T.: 0.000 min  
Response: 7158830  
Conc: 293.93 ng/ml

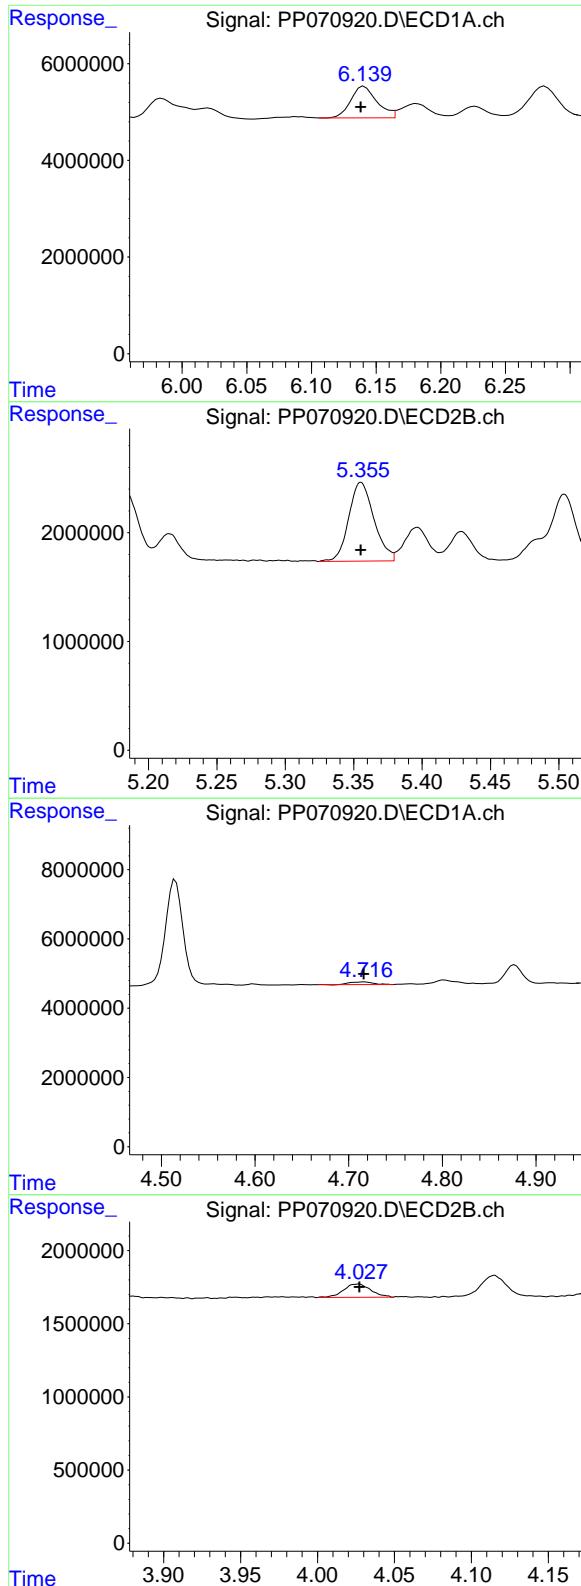

#7 AR-1016-5

R.T.: 6.141 min  
 Delta R.T.: 0.003 min  
 Response: 9152735  
 Conc: 269.90 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#7 AR-1016-5


R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 9323046  
 Conc: 288.45 ng/ml

#8 AR-1221-1

R.T.: 4.717 min  
 Delta R.T.: 0.000 min  
 Response: 1321625  
 Conc: 76.16 ng/ml

#8 AR-1221-1


R.T.: 4.026 min  
 Delta R.T.: 0.000 min  
 Response: 1122384  
 Conc: 73.63 ng/ml



#9 AR-1221-2


R.T.: 4.802 min  
Delta R.T.: 0.000 min  
Response: 2090814  
Conc: 161.42 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660ICC250

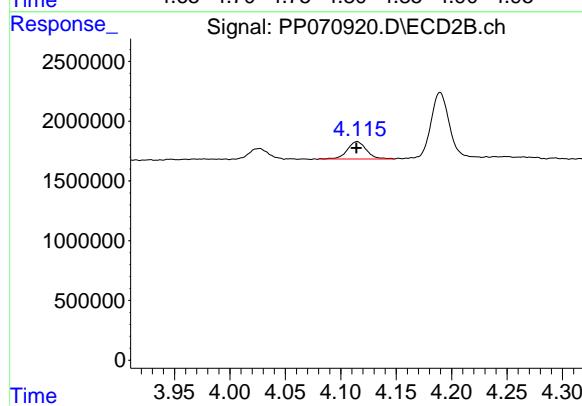


#9 AR-1221-2

R.T.: 4.115 min  
Delta R.T.: 0.000 min  
Response: 1735253  
Conc: 151.73 ng/ml




#10 AR-1221-3

R.T.: 4.877 min  
Delta R.T.: 0.000 min  
Response: 7052777  
Conc: 169.06 ng/ml

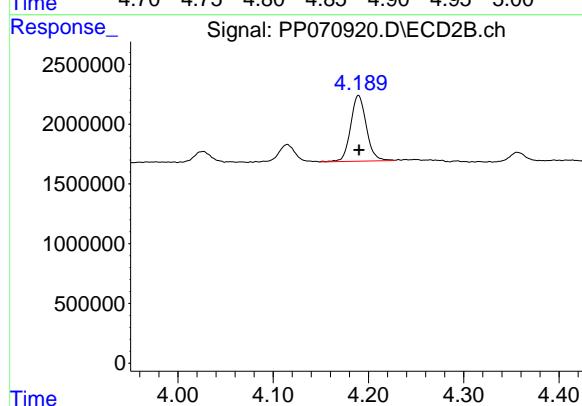

#10 AR-1221-3


R.T.: 4.190 min  
Delta R.T.: 0.000 min  
Response: 6326573  
Conc: 185.59 ng/ml

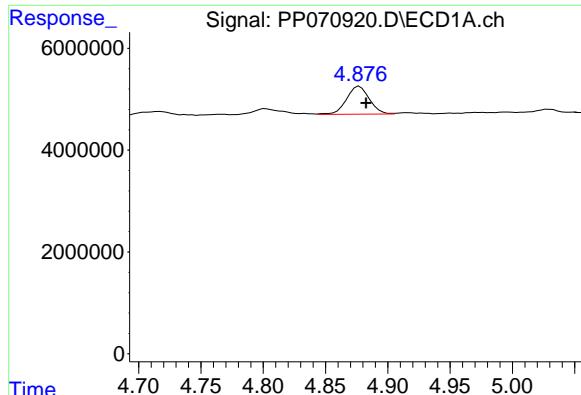

#11 AR-1232-1


R.T.: 4.877 min  
Delta R.T.: -0.005 min  
Response: 7052777  
Conc: 211.87 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660ICC250

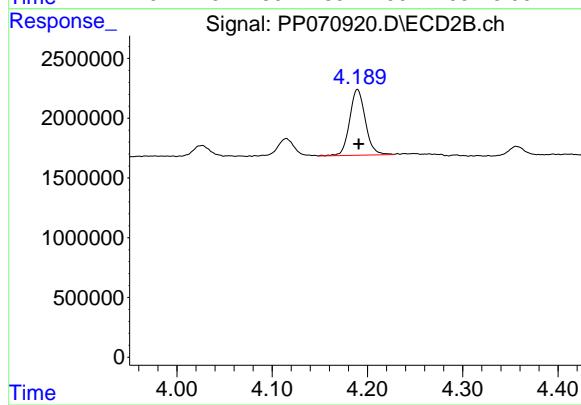


#11 AR-1232-1

R.T.: 4.190 min  
Delta R.T.: -0.001 min  
Response: 6326573  
Conc: 226.06 ng/ml

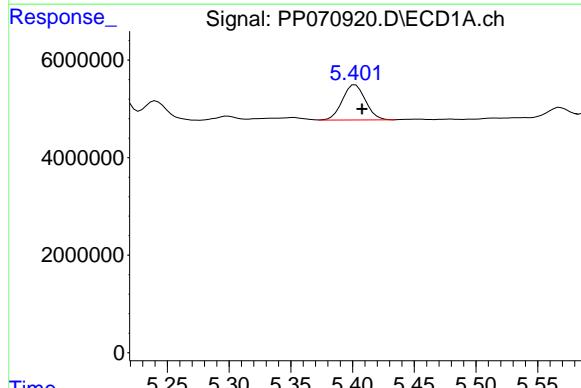


#12 AR-1232-2

R.T.: 5.402 min  
Delta R.T.: -0.005 min  
Response: 9379837  
Conc: 589.54 ng/ml

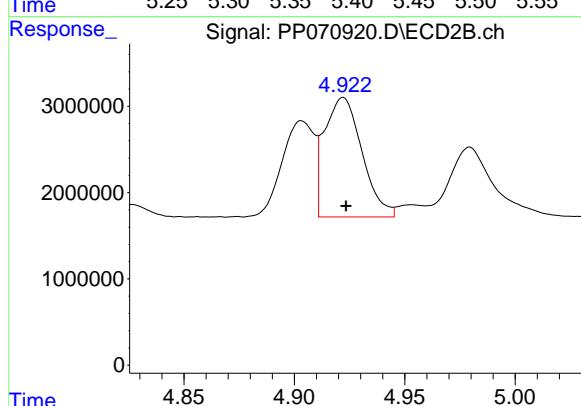

#12 AR-1232-2


R.T.: 4.922 min  
Delta R.T.: -0.001 min  
Response: 16375760  
Conc: 583.57 ng/ml

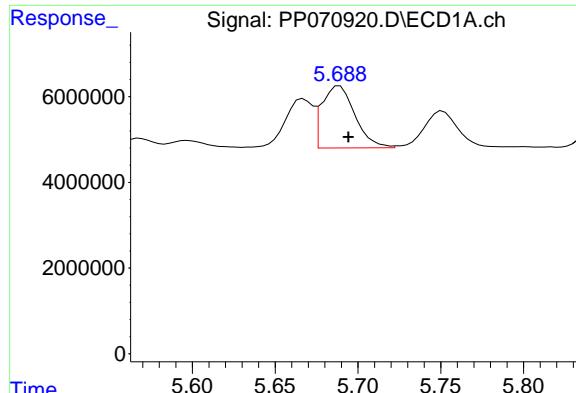

#13 AR-1232-3


R.T.: 5.689 min  
 Delta R.T.: -0.005 min  
 Response: 20108471  
 Conc: 586.76 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

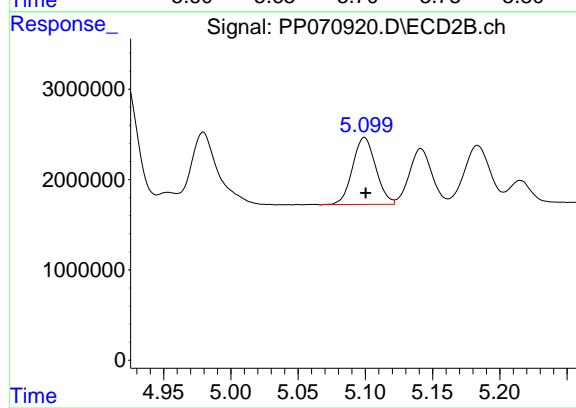


#13 AR-1232-3

R.T.: 5.099 min  
 Delta R.T.: -0.001 min  
 Response: 8877034  
 Conc: 596.19 ng/ml

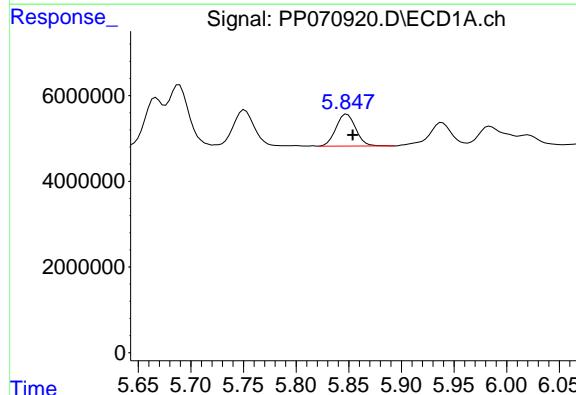


#14 AR-1232-4

R.T.: 5.848 min  
 Delta R.T.: -0.006 min  
 Response: 9803037  
 Conc: 624.10 ng/ml

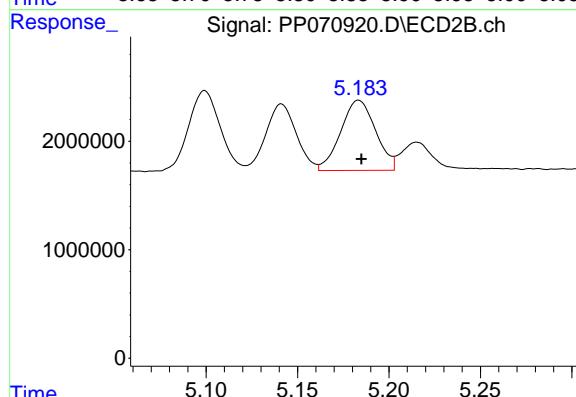

#14 AR-1232-4

R.T.: 5.183 min  
 Delta R.T.: -0.001 min  
 Response: 8604427  
 Conc: 671.99 ng/ml

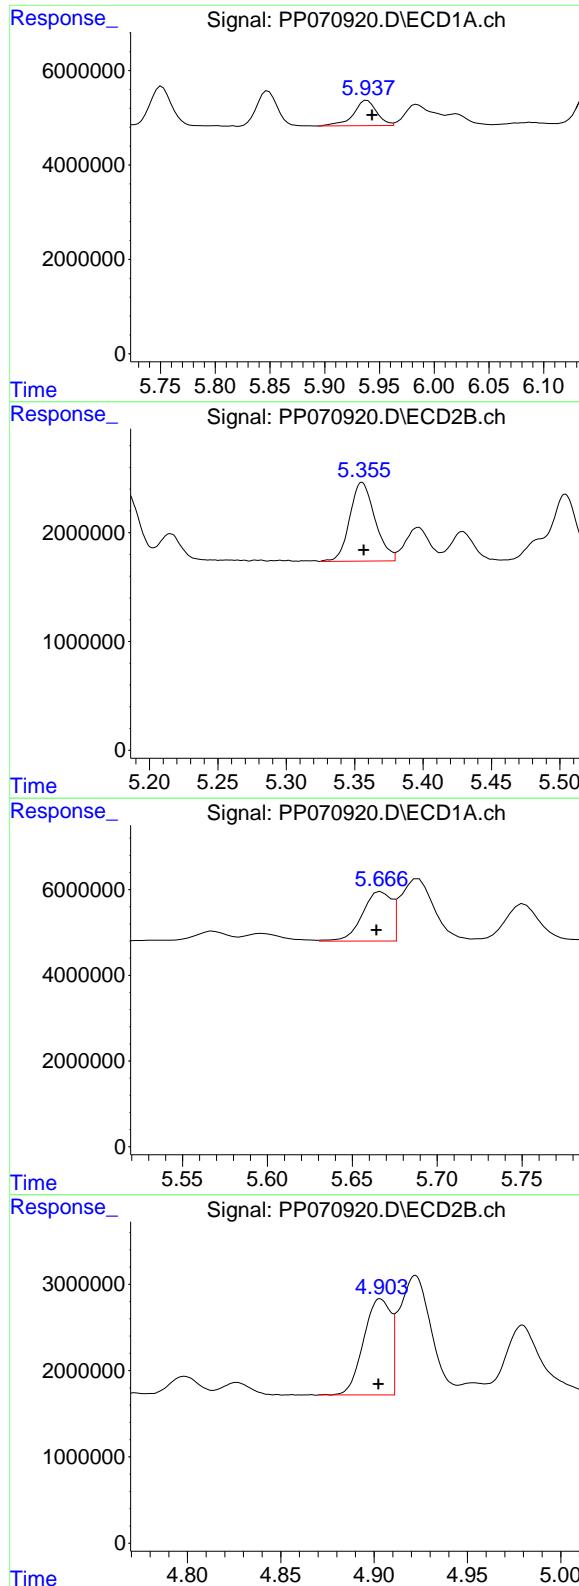

#15 AR-1232-5

R.T.: 5.939 min  
 Delta R.T.: -0.005 min  
 Response: 7957300  
 Conc: 747.84 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#15 AR-1232-5


R.T.: 5.355 min  
 Delta R.T.: -0.001 min  
 Response: 9323046  
 Conc: 657.72 ng/ml

#16 AR-1242-1

R.T.: 5.667 min  
 Delta R.T.: 0.003 min  
 Response: 13581167  
 Conc: 308.82 ng/ml

#16 AR-1242-1


R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 11323714  
 Conc: 331.14 ng/ml

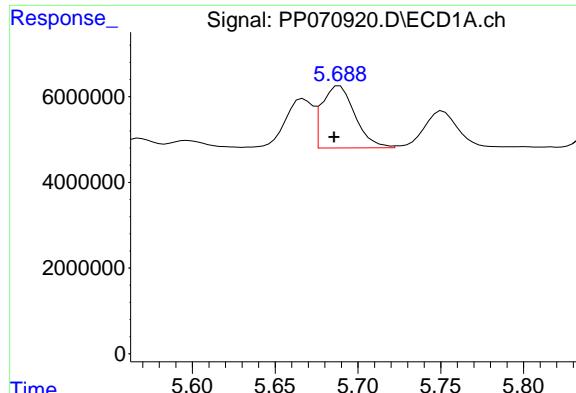

#17 AR-1242-2


R.T.: 5.689 min  
 Delta R.T.: 0.003 min  
 Response: 20108471  
 Conc: 312.65 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

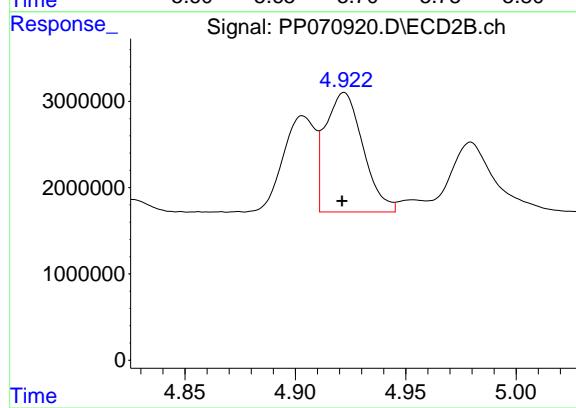


#17 AR-1242-2

R.T.: 4.922 min  
 Delta R.T.: 0.001 min  
 Response: 16375760  
 Conc: 332.45 ng/ml

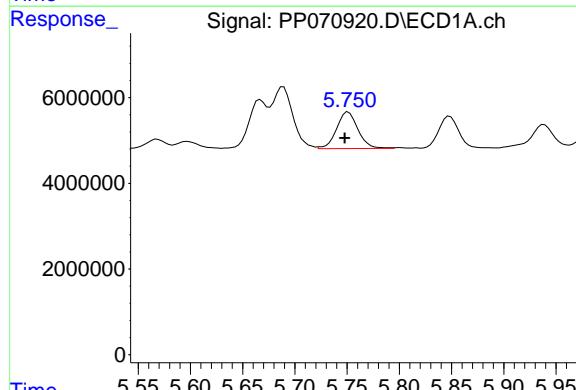


#18 AR-1242-3

R.T.: 5.751 min  
 Delta R.T.: 0.003 min  
 Response: 12212490  
 Conc: 297.58 ng/ml

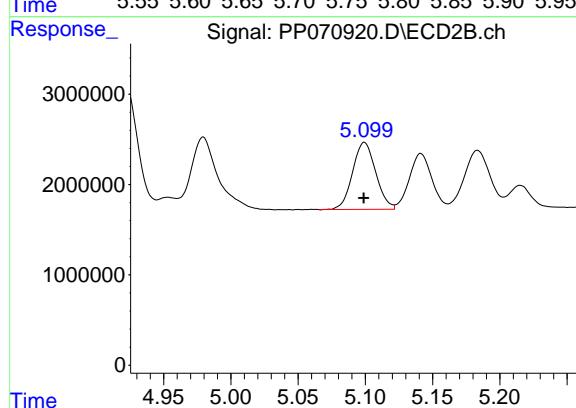

#18 AR-1242-3

R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 8877034  
 Conc: 333.17 ng/ml

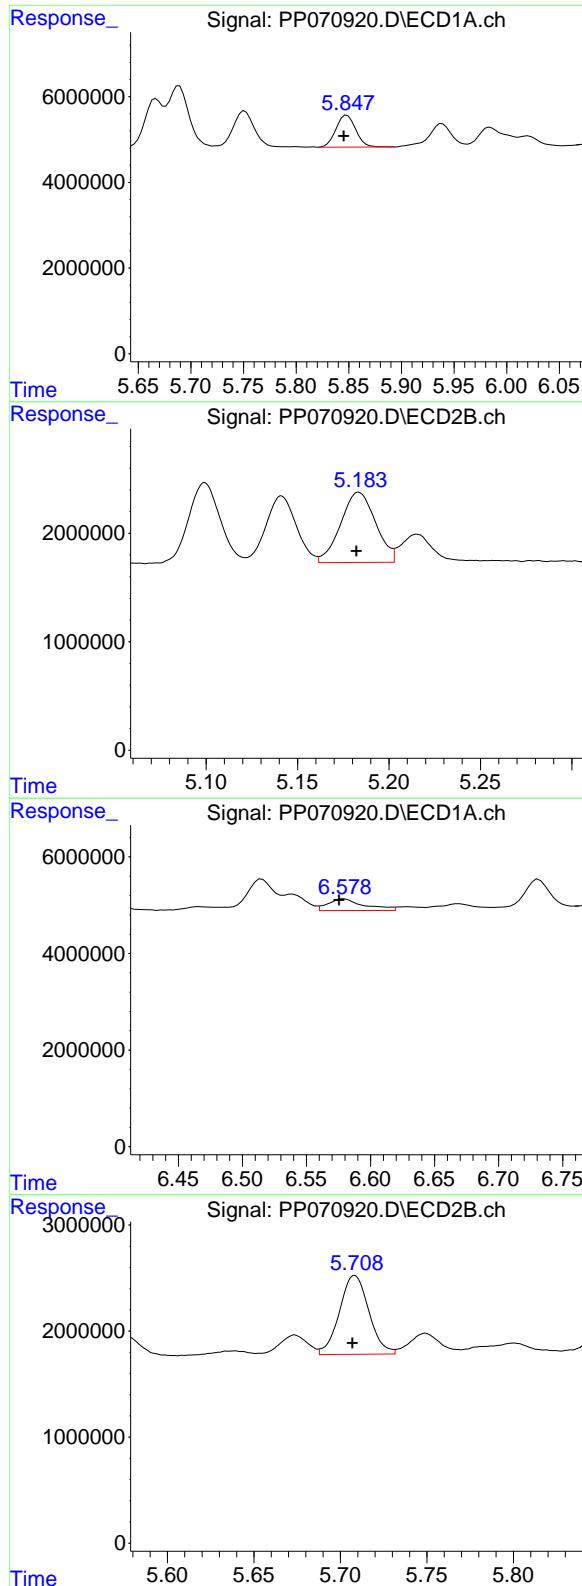

#19 AR-1242-4

R.T.: 5.848 min  
 Delta R.T.: 0.003 min  
 Response: 9803037  
 Conc: 321.17 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#19 AR-1242-4


R.T.: 5.183 min  
 Delta R.T.: 0.001 min  
 Response: 8604427  
 Conc: 326.19 ng/ml

#20 AR-1242-5

R.T.: 6.579 min  
 Delta R.T.: 0.004 min  
 Response: 4761571  
 Conc: 130.42 ng/ml

#20 AR-1242-5


R.T.: 5.708 min  
 Delta R.T.: 0.001 min  
 Response: 8766943  
 Conc: 283.19 ng/ml

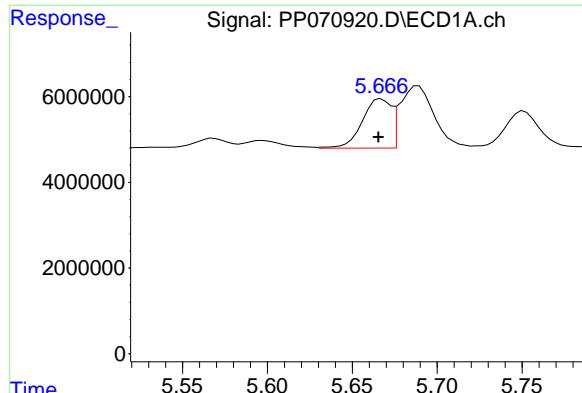

#21 AR-1248-1


R.T.: 5.667 min  
 Delta R.T.: 0.002 min  
 Response: 13581167  
 Conc: 374.27 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

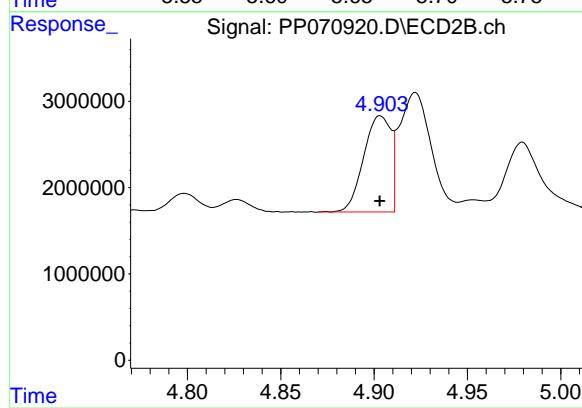


#21 AR-1248-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 11323714  
 Conc: 418.16 ng/ml

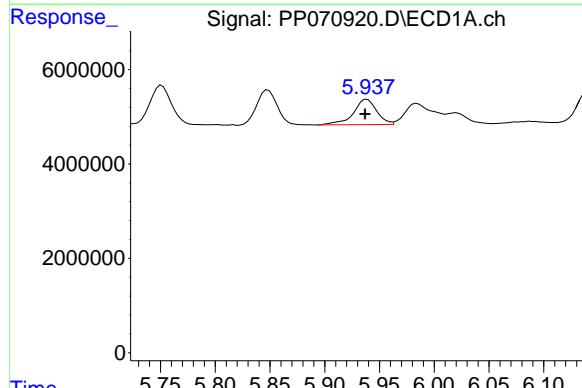


#22 AR-1248-2

R.T.: 5.939 min  
 Delta R.T.: 0.002 min  
 Response: 7957300  
 Conc: 177.07 ng/ml

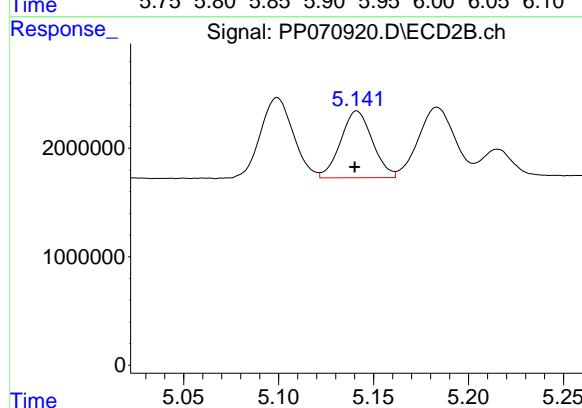

#22 AR-1248-2

R.T.: 5.141 min  
 Delta R.T.: 0.001 min  
 Response: 7158830  
 Conc: 194.94 ng/ml

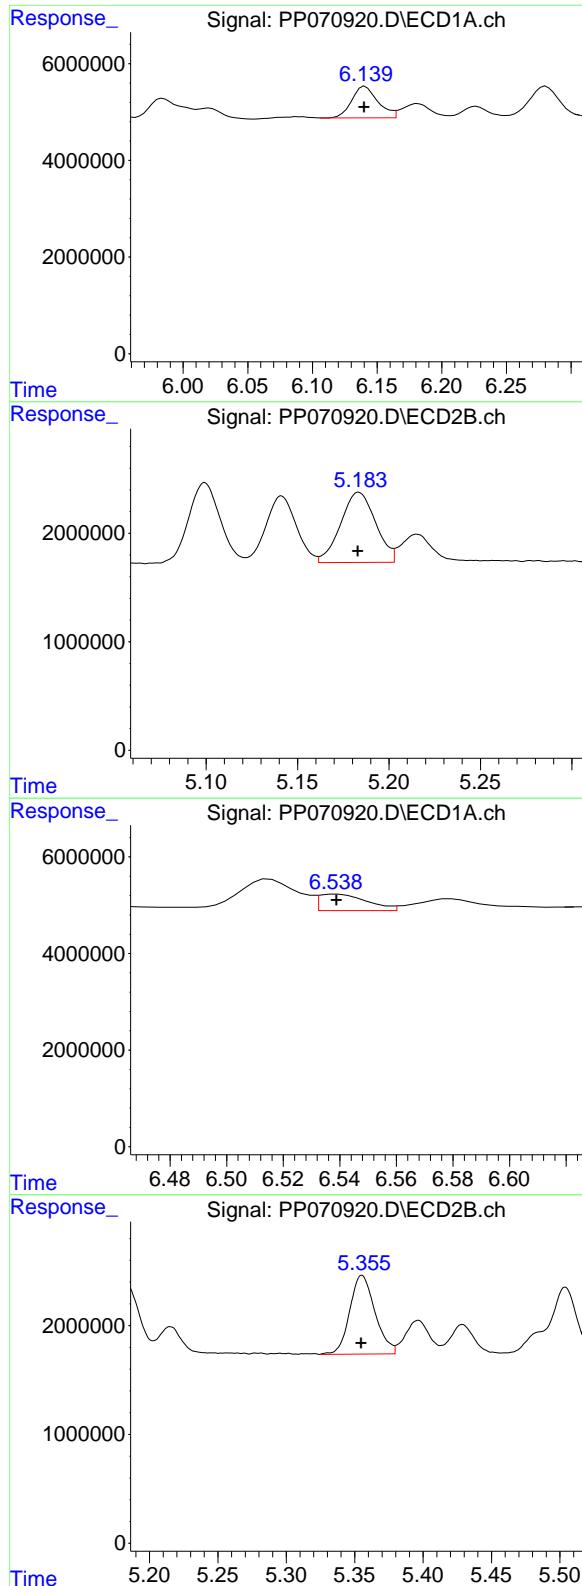

#23 AR-1248-3

R.T.: 6.141 min  
 Delta R.T.: 0.000 min  
 Response: 9152735  
 Conc: 180.75 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#23 AR-1248-3


R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 8604427  
 Conc: 222.57 ng/ml

#24 AR-1248-4

R.T.: 6.539 min  
 Delta R.T.: 0.000 min  
 Response: 4049391  
 Conc: 63.13 ng/ml

#24 AR-1248-4

R.T.: 5.355 min  
 Delta R.T.: 0.000 min  
 Response: 9323046  
 Conc: 206.53 ng/ml

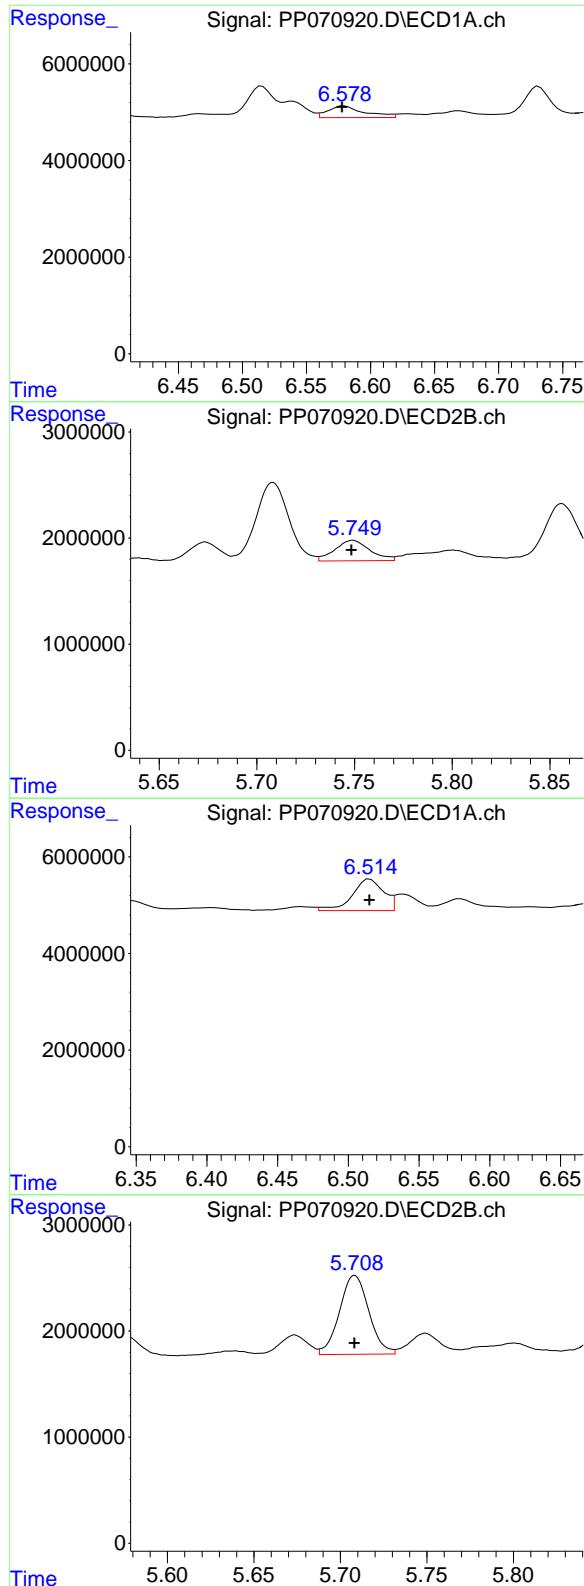

#25 AR-1248-5

R.T.: 6.579 min  
 Delta R.T.: 0.002 min  
 Response: 4761571  
 Conc: 78.26 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#25 AR-1248-5


R.T.: 5.749 min  
 Delta R.T.: 0.000 min  
 Response: 2416322  
 Conc: 56.62 ng/ml

#26 AR-1254-1

R.T.: 6.515 min  
 Delta R.T.: 0.000 min  
 Response: 10069870  
 Conc: 156.39 ng/ml

#26 AR-1254-1

R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 8766943  
 Conc: 132.80 ng/ml

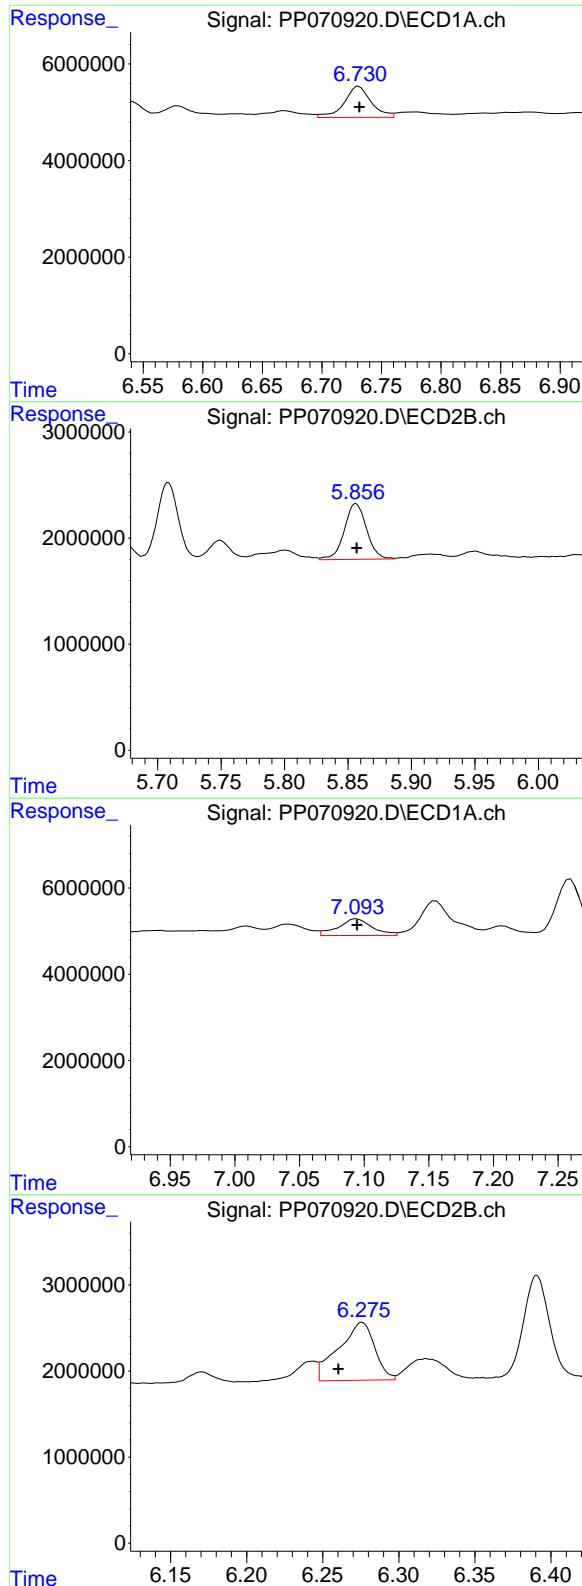

#27 AR-1254-2

R.T.: 6.731 min  
 Delta R.T.: 0.000 min  
 Response: 10106718  
 Conc: 99.98 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#27 AR-1254-2


R.T.: 5.856 min  
 Delta R.T.: 0.000 min  
 Response: 6407649  
 Conc: 112.22 ng/ml

#28 AR-1254-3

R.T.: 7.094 min  
 Delta R.T.: 0.000 min  
 Response: 7072472  
 Conc: 70.92 ng/ml

#28 AR-1254-3

R.T.: 6.276 min  
 Delta R.T.: 0.016 min  
 Response: 11091003  
 Conc: 127.72 ng/ml

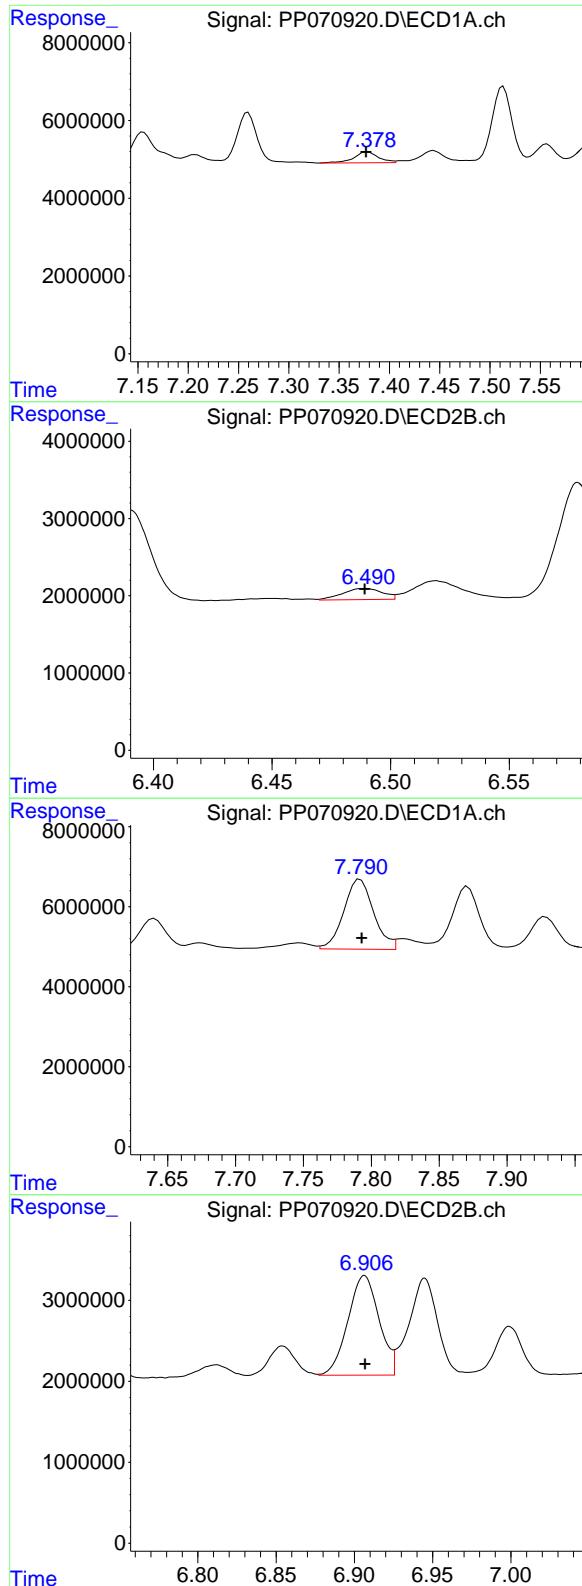

#29 AR-1254-4

R.T.: 7.379 min  
 Delta R.T.: 0.002 min  
 Response: 4686448  
 Conc: 54.12 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#29 AR-1254-4





R.T.: 6.489 min  
 Delta R.T.: 0.000 min  
 Response: 1684678  
 Conc: 30.03 ng/ml

#30 AR-1254-5

R.T.: 7.792 min  
 Delta R.T.: -0.001 min  
 Response: 26750553  
 Conc: 332.92 ng/ml

#30 AR-1254-5

R.T.: 6.906 min  
 Delta R.T.: 0.000 min  
 Response: 17034582  
 Conc: 236.10 ng/ml

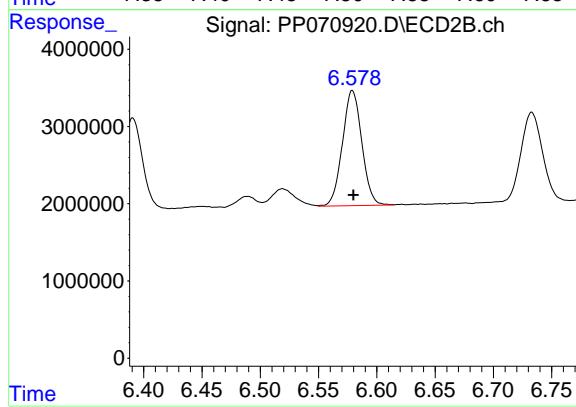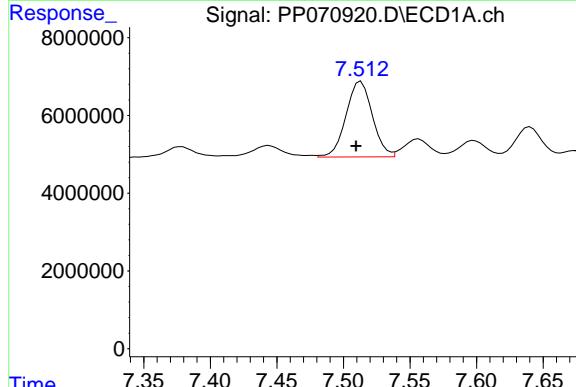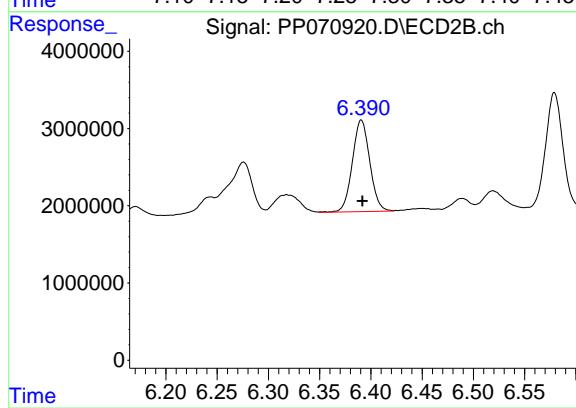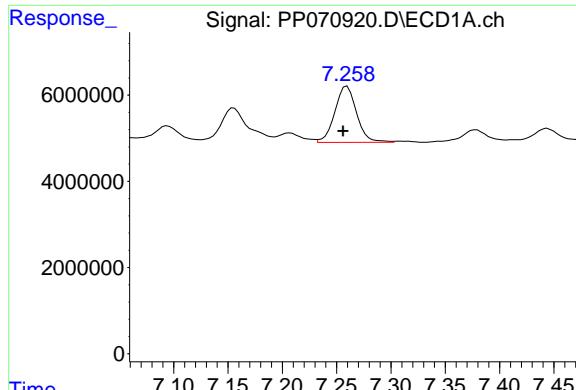

#31 AR-1260-1

R.T.: 7.260 min  
 Delta R.T.: 0.004 min  
 Response: 18182257  
 Conc: 270.76 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#31 AR-1260-1


R.T.: 6.391 min  
 Delta R.T.: -0.001 min  
 Response: 14056672  
 Conc: 274.51 ng/ml

#32 AR-1260-2

R.T.: 7.513 min  
 Delta R.T.: 0.004 min  
 Response: 26780079  
 Conc: 278.56 ng/ml

#32 AR-1260-2

R.T.: 6.579 min  
 Delta R.T.: 0.000 min  
 Response: 17295947  
 Conc: 271.12 ng/ml

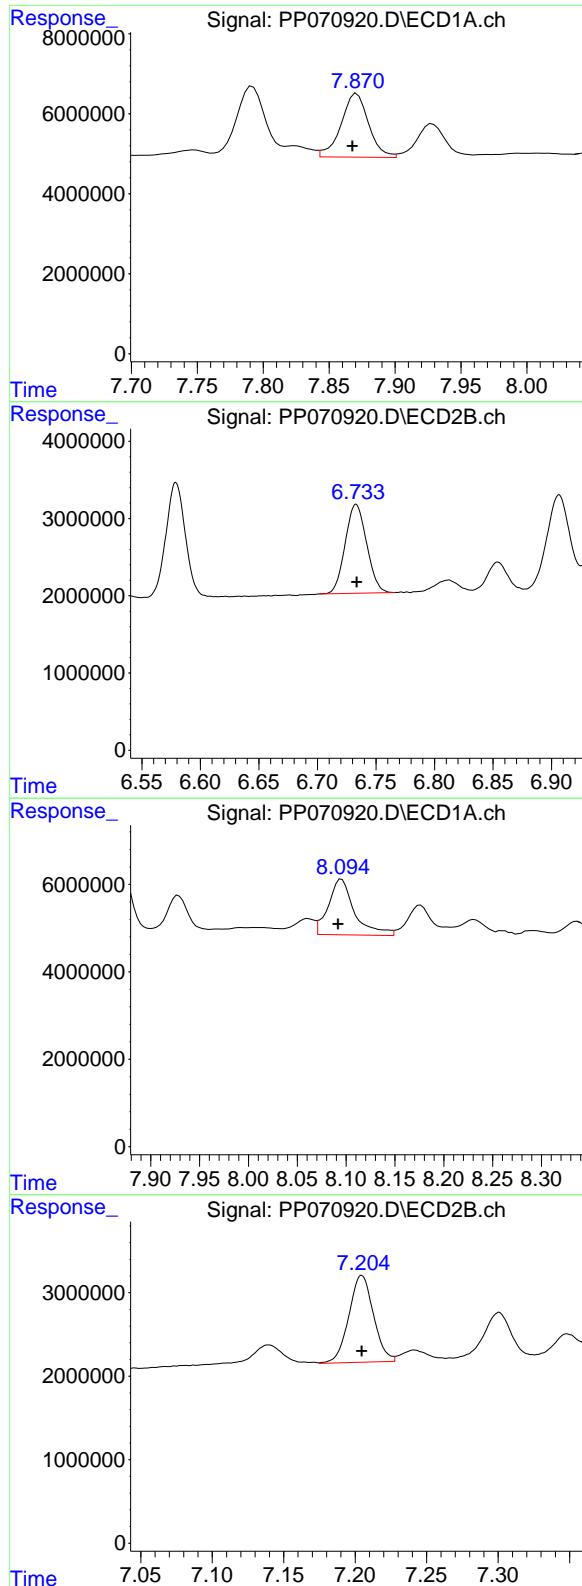

#33 AR-1260-3

R.T.: 7.871 min  
 Delta R.T.: 0.003 min  
 Response: 23122222  
 Conc: 289.32 ng/ml

**Instrument:** ECD\_P  
**ClientSampleId:** AR1660ICC250

#33 AR-1260-3


R.T.: 6.733 min  
 Delta R.T.: 0.000 min  
 Response: 14684885  
 Conc: 269.51 ng/ml

#34 AR-1260-4

R.T.: 8.095 min  
 Delta R.T.: 0.004 min  
 Response: 23709378  
 Conc: 301.12 ng/ml

#34 AR-1260-4


R.T.: 7.205 min  
 Delta R.T.: 0.000 min  
 Response: 12488782  
 Conc: 261.13 ng/ml

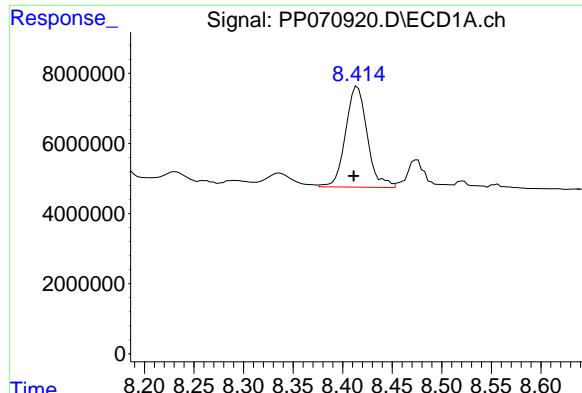

#35 AR-1260-5


R.T.: 8.415 min  
 Delta R.T.: 0.004 min  
 Response: 43743345  
 Conc: 275.31 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

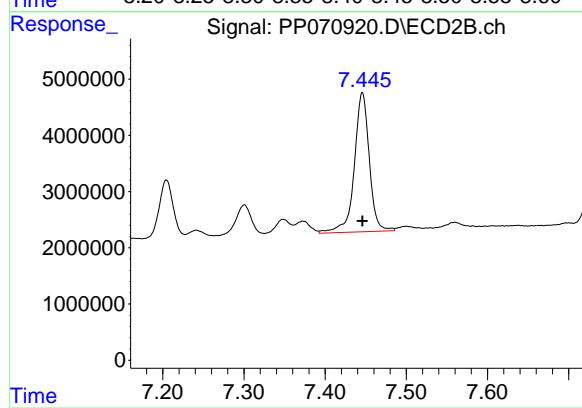


#35 AR-1260-5

R.T.: 7.446 min  
 Delta R.T.: 0.000 min  
 Response: 31815782  
 Conc: 255.53 ng/ml

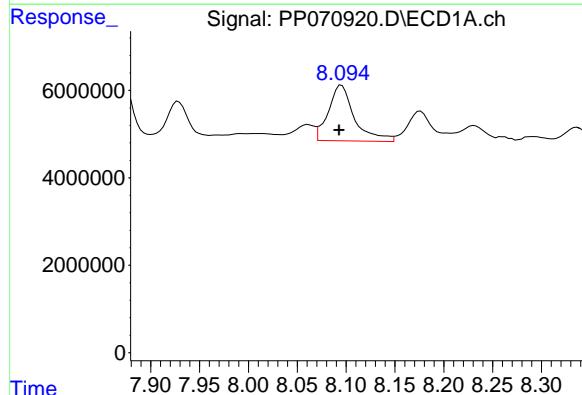


#36 AR-1262-1

R.T.: 8.095 min  
 Delta R.T.: 0.003 min  
 Response: 23709378  
 Conc: 223.04 ng/ml

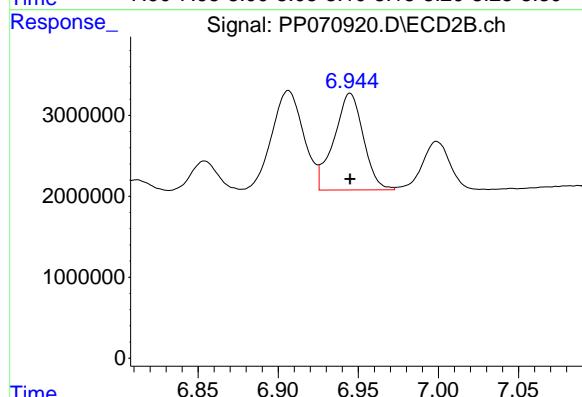

#36 AR-1262-1

R.T.: 6.945 min  
 Delta R.T.: 0.000 min  
 Response: 15226146  
 Conc: 177.95 ng/ml

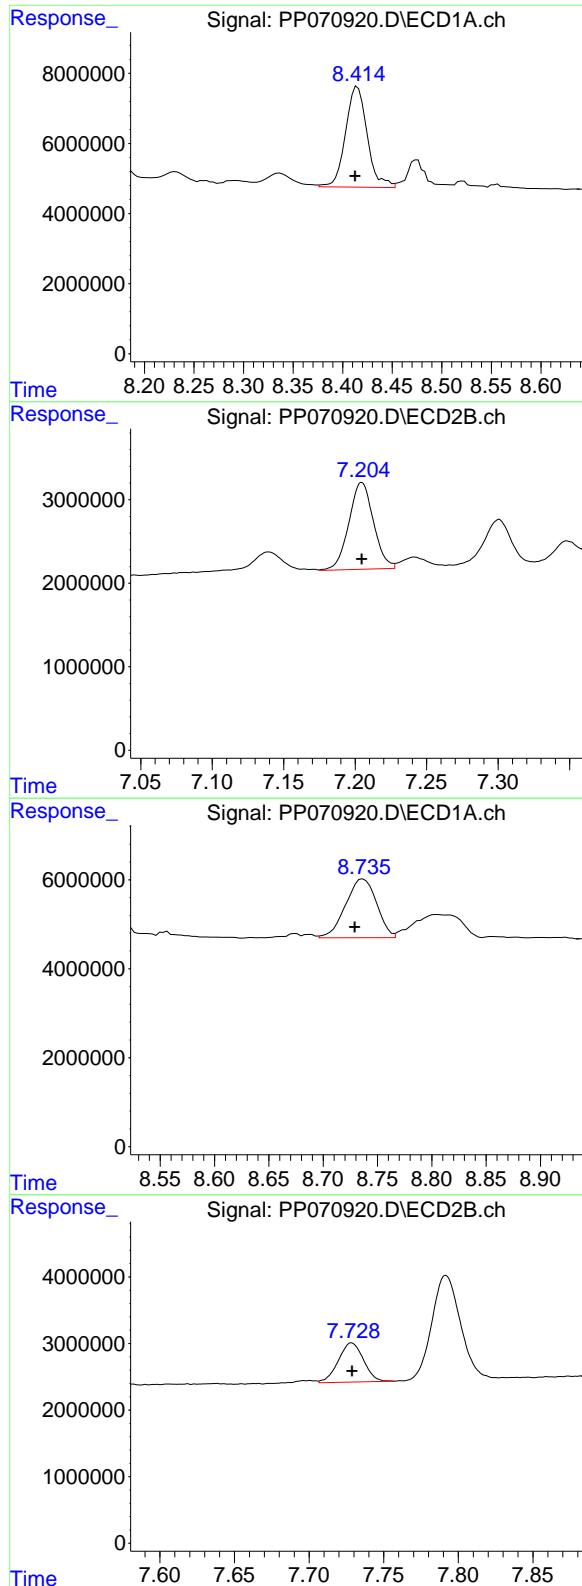

#37 AR-1262-2

R.T.: 8.415 min  
 Delta R.T.: 0.003 min  
 Response: 43743345  
 Conc: 220.50 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#37 AR-1262-2


R.T.: 7.205 min  
 Delta R.T.: 0.000 min  
 Response: 12488782  
 Conc: 182.41 ng/ml

#38 AR-1262-3

R.T.: 8.737 min  
 Delta R.T.: 0.008 min  
 Response: 26257171  
 Conc: 199.31 ng/ml

#38 AR-1262-3


R.T.: 7.728 min  
 Delta R.T.: 0.000 min  
 Response: 6907710  
 Conc: 113.76 ng/ml

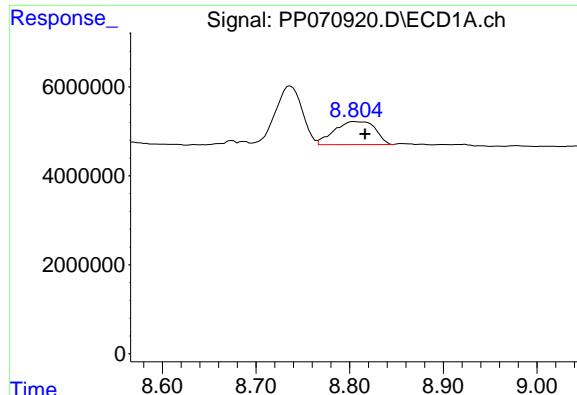

#39 AR-1262-4


R.T.: 8.806 min  
 Delta R.T.: -0.011 min  
 Response: 15776574  
 Conc: 165.00 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

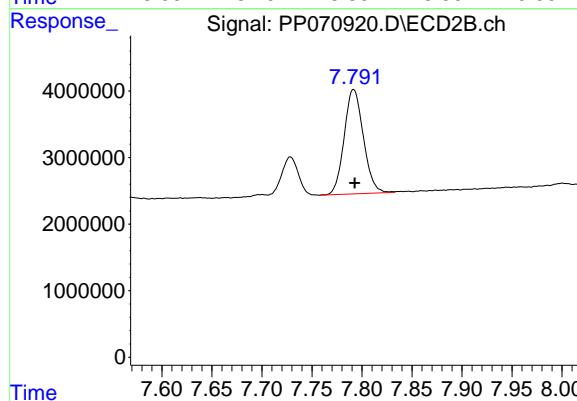


#39 AR-1262-4

R.T.: 7.792 min  
 Delta R.T.: -0.001 min  
 Response: 20963428  
 Conc: 210.89 ng/ml

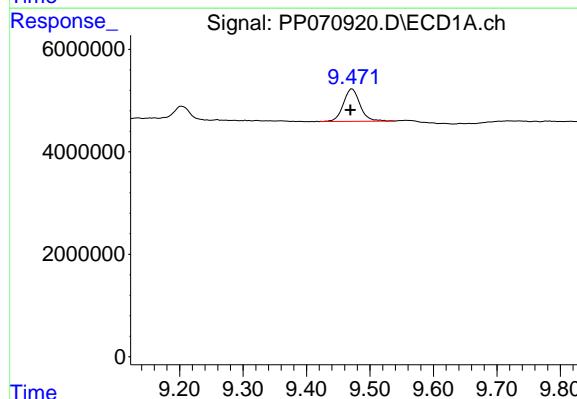


#40 AR-1262-5

R.T.: 9.472 min  
 Delta R.T.: 0.003 min  
 Response: 11555188  
 Conc: 177.59 ng/ml

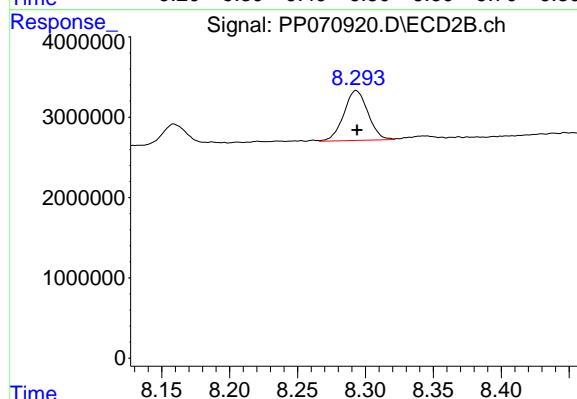

#40 AR-1262-5

R.T.: 8.293 min  
 Delta R.T.: 0.000 min  
 Response: 7670514  
 Conc: 163.65 ng/ml

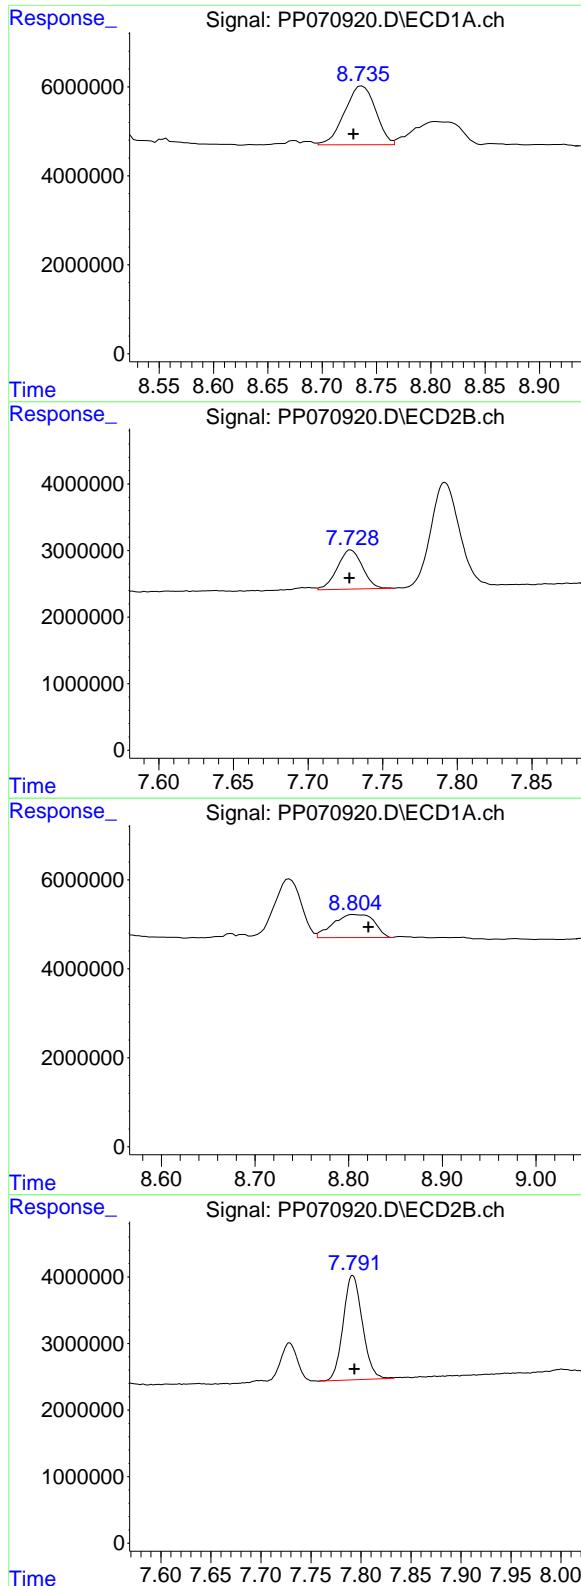

#41 AR-1268-1

R.T.: 8.737 min  
 Delta R.T.: 0.008 min  
 Response: 26257171  
 Conc: 111.49 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC250

#41 AR-1268-1


R.T.: 7.728 min  
 Delta R.T.: 0.000 min  
 Response: 6907710  
 Conc: 40.30 ng/ml

#42 AR-1268-2

R.T.: 8.806 min  
 Delta R.T.: -0.016 min  
 Response: 15776574  
 Conc: 80.77 ng/ml


#42 AR-1268-2

R.T.: 7.792 min  
 Delta R.T.: -0.002 min  
 Response: 20963428  
 Conc: 146.31 ng/ml

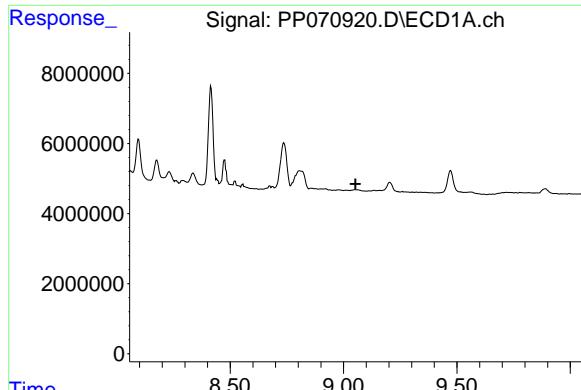


#43 AR-1268-3

R.T.: 0.000 min  
 Exp R.T. : 9.053 min **Instrument:**  
 Response: 0 ECD\_P  
 Conc: N.D. ClientSampleId :  
 AR1660ICC250

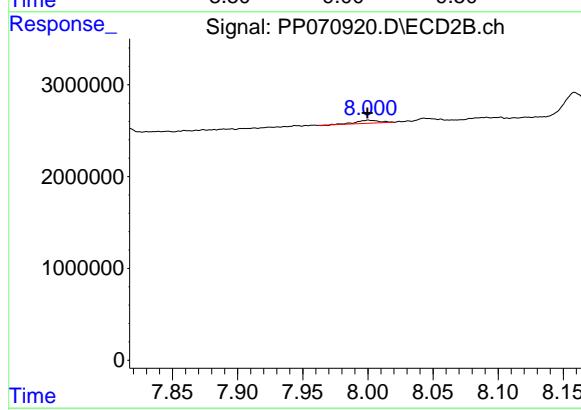


#43 AR-1268-3

R.T.: 8.001 min  
 Delta R.T.: 0.000 min  
 Response: 412782  
 Conc: 3.35 ng/ml

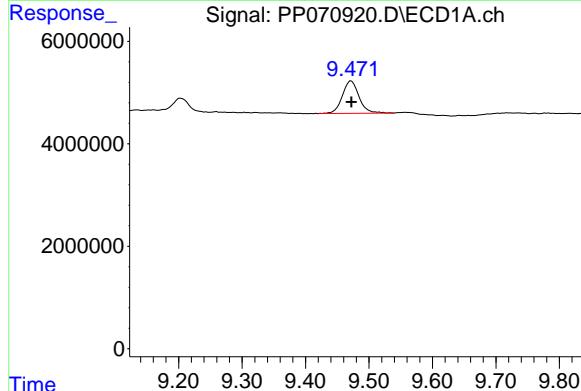


#44 AR-1268-4

R.T.: 9.472 min  
 Delta R.T.: 0.000 min  
 Response: 11555188  
 Conc: 163.33 ng/ml

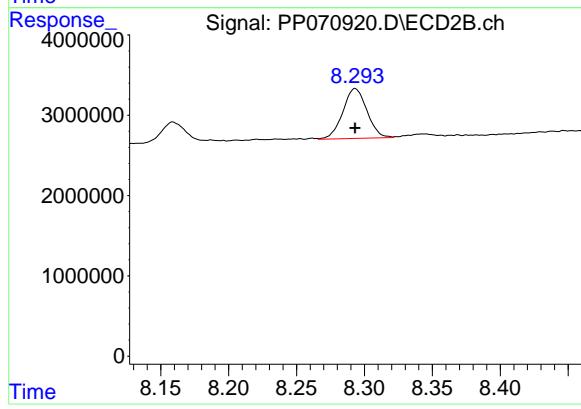

#44 AR-1268-4


R.T.: 8.293 min  
 Delta R.T.: 0.000 min  
 Response: 7670514  
 Conc: 145.24 ng/ml

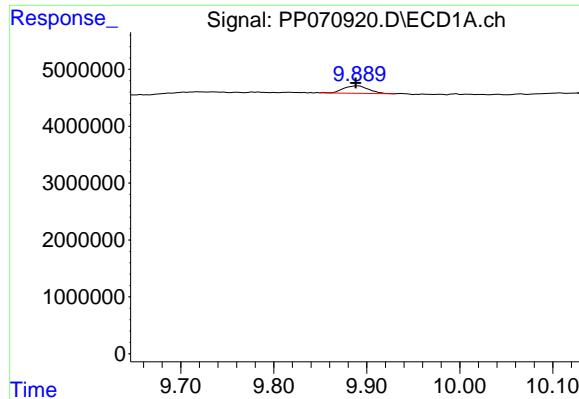

#45 AR-1268-5

R.T.: 9.890 min  
Delta R.T.: 0.002 min  
Response: 2482779  
Conc: 5.21 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660ICC250

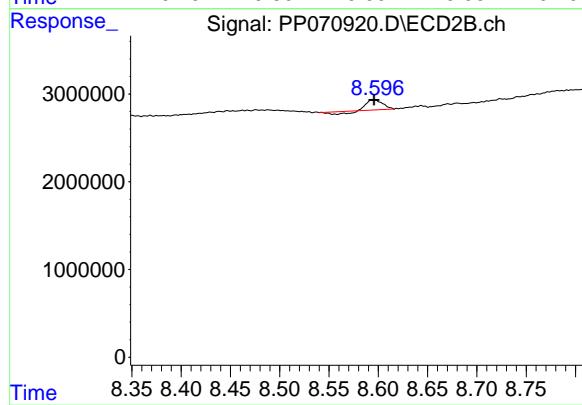

#45 AR-1268-5

R.T.: 8.596 min  
Delta R.T.: 0.000 min  
Response: 969431  
Conc: 2.68 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
Data File : PP070921.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 27 Mar 2025 11:35  
Operator : YP\AJ  
Sample : AR1660ICC050  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
ECD\_P  
**ClientSampleId :**  
AR1660ICC050

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 31 03:04:09 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Mar 28 03:13:46 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

1) SA Tetrachlor...	4.513	3.816	6533335	5359624	4.470	5.170
2) SA Decachlor...	10.230	8.858	4733739	3413055	4.497	4.330

#### Target Compounds

3) L1 AR-1016-1	5.666	4.903	2617394	2265971	51.472	56.525
4) L1 AR-1016-2	5.688	4.922	4198554	3321854	53.791	57.407
5) L1 AR-1016-3	5.751	5.099	2631097	1626306	55.774	52.592
6) L1 AR-1016-4	5.848	5.140	1614372	1232754	43.922	50.614
7) L1 AR-1016-5	6.140	5.356	1323106	1866333	39.016	57.743 #
8) L2 AR-1221-1	4.717	4.024	421830	114713	24.308	7.525 #
9) L2 AR-1221-2	4.801	4.115	218742	388578	16.887	33.978 #
10) L2 AR-1221-3	4.877	4.189	1349629	1162778	32.352	34.110
11) L3 AR-1232-1	4.877	4.189	1349629	1162778	40.543	41.548
12) L3 AR-1232-2	5.401	4.922	1794886	3321854	112.813	118.379
13) L3 AR-1232-3	5.688	5.099	4198554	1626306	122.513	109.224
14) L3 AR-1232-4	5.848	5.183	1614372	1568895	102.777	122.528
15) L3 AR-1232-5	5.935	5.356	1663453	1866333	156.334	131.666
16) L4 AR-1242-1	5.666	4.903	2617394	2265971	59.517	66.265
17) L4 AR-1242-2	5.688	4.922	4198554	3321854	65.280	67.438
18) L4 AR-1242-3	5.751	5.099	2631097	1626306	64.111	61.038
19) L4 AR-1242-4	5.848	5.183	1614372	1568895	52.890	59.477
20) L4 AR-1242-5	6.582	5.708	1738801	1466013	47.625	47.354
21) L5 AR-1248-1	5.666	4.903	2617394	2265971	72.129	83.677
22) L5 AR-1248-2	5.935	5.140	1663453	1232754	37.016	33.569
23) L5 AR-1248-3	6.140	5.183	1323106	1568895	26.129	40.583 #
24) L5 AR-1248-4	6.539	5.356	1621071	1866333	25.271	41.345 #
25) L5 AR-1248-5	6.582	5.748	1738801	371096	28.577	8.695 #
26) L6 AR-1254-1	6.515	5.708	3489366	1466013	54.191	22.206 #
27) L6 AR-1254-2	6.731	5.857	4772204	1146779	47.207	20.084 #
28) L6 AR-1254-3	7.095	6.275	7925059	3163207	79.467	36.425 #
29) L6 AR-1254-4	7.380	6.490	1640237	349900	18.941	6.237 #
30) L6 AR-1254-5	7.791	6.906	5692306	2994420	70.843	41.502 #
31) L7 AR-1260-1	7.258	6.391	4772844	2989801	71.074	58.387
32) L7 AR-1260-2	7.512	6.579	5123964	3357287	53.299	52.627
33) L7 AR-1260-3	7.871	6.732	5463057	2827385	68.358	51.891
34) L7 AR-1260-4	8.095	7.205	9380427	2746307	119.136	57.423 #
35) L7 AR-1260-5	8.414	7.445	11051960	7013440	69.559	56.328
36) L8 AR-1262-1	8.095	6.945	9380427	2613596	88.245	30.546 #
37) L8 AR-1262-2	8.414	7.205	11051960	2746307	55.710	40.113 #
38) L8 AR-1262-3	8.737	7.729	4423235	1556480	33.575	25.632
39) L8 AR-1262-4	8.806	7.792	1951193	3771123	20.407	37.936 #
40) L8 AR-1262-5	9.470	8.292	1729860	1260427	26.586	26.891
41) L9 AR-1268-1	8.737	7.729	4423235	1556480	18.782	9.081 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:35  
 Operator : YP\AJ  
 Sample : AR1660ICC050  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 31 03:04:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	8.806	7.792	1951193	3771123	9.990	26.319 #
43) L9 AR-1268-3	0.000	8.026	0	152620	N.D.	1.239 #
44) L9 AR-1268-4	9.470	8.292	1729860	1260427	24.451	23.866



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 11:35  
 Operator : YP\AJ  
 Sample : AR1660ICC050  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 31 03:04:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

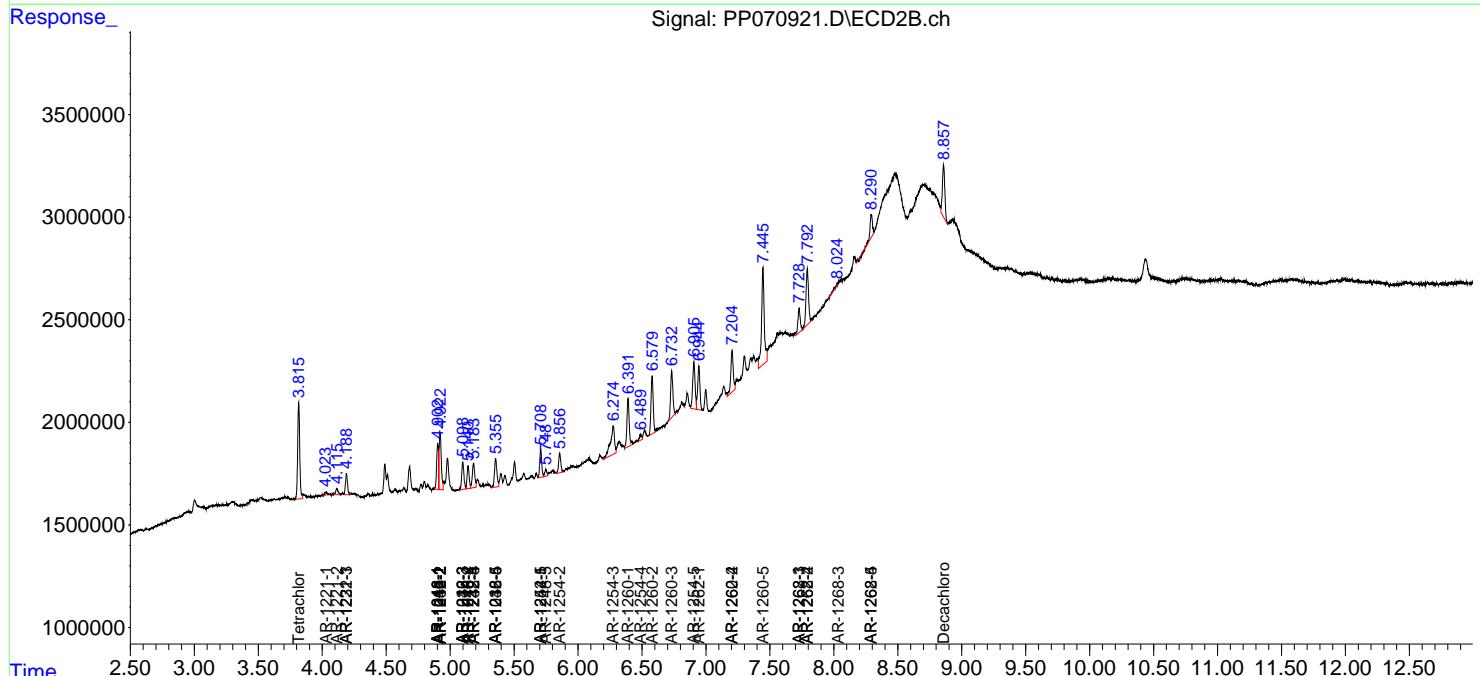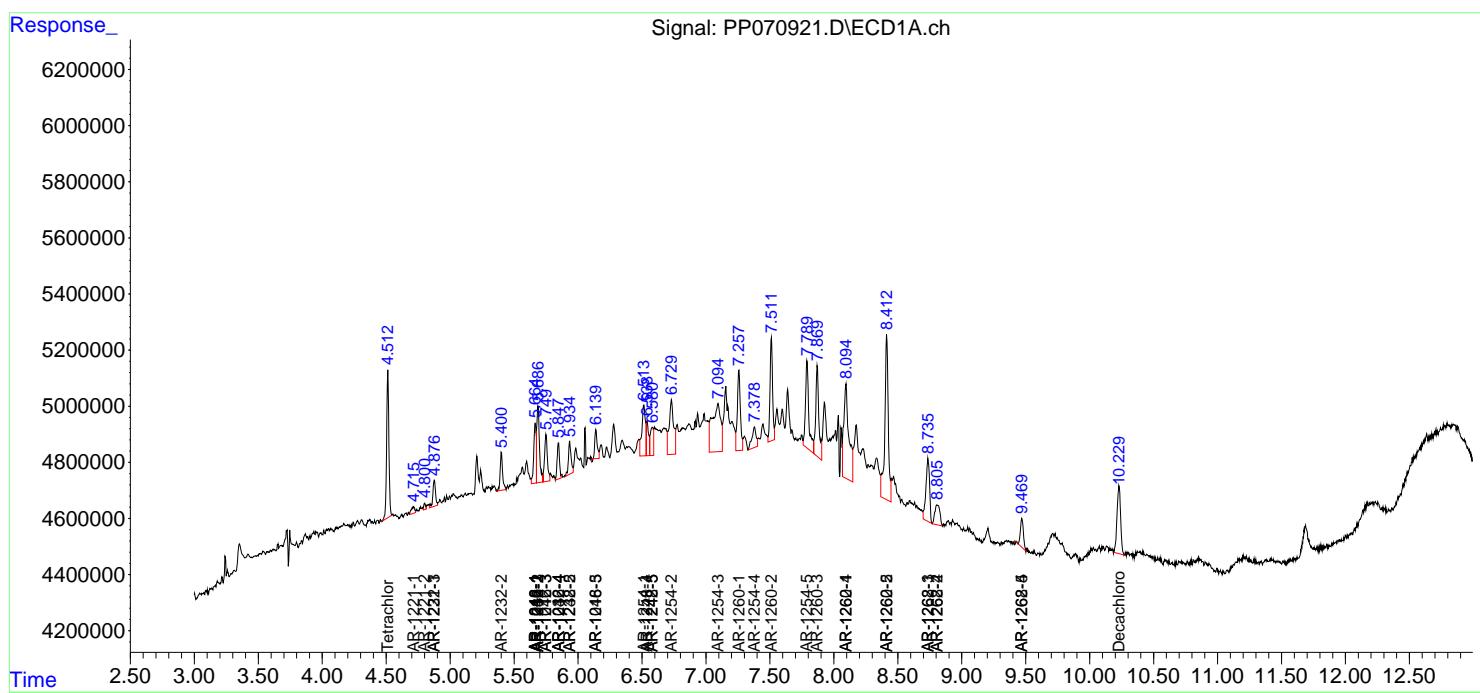



#1 Tetrachloro-m-xylene


R.T.: 4.513 min  
Delta R.T.: 0.001 min  
Response: 6533335  
Conc: 4.47 ng/ml

Instrument:

ECD\_P


ClientSampleId :

AR1660ICC050

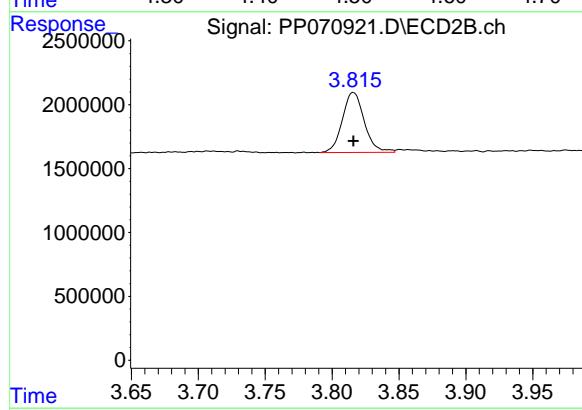


#1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 5359624  
Conc: 5.17 ng/ml

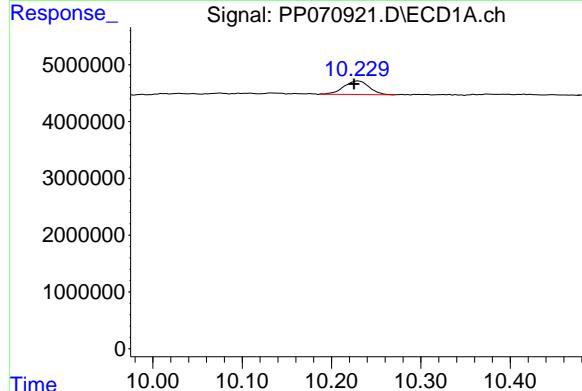


#2 Decachlorobiphenyl

R.T.: 10.230 min  
Delta R.T.: 0.005 min  
Response: 4733739  
Conc: 4.50 ng/ml

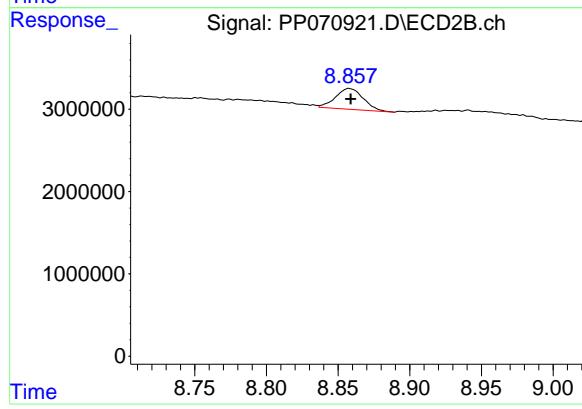

#2 Decachlorobiphenyl

R.T.: 8.858 min  
Delta R.T.: 0.000 min  
Response: 3413055  
Conc: 4.33 ng/ml

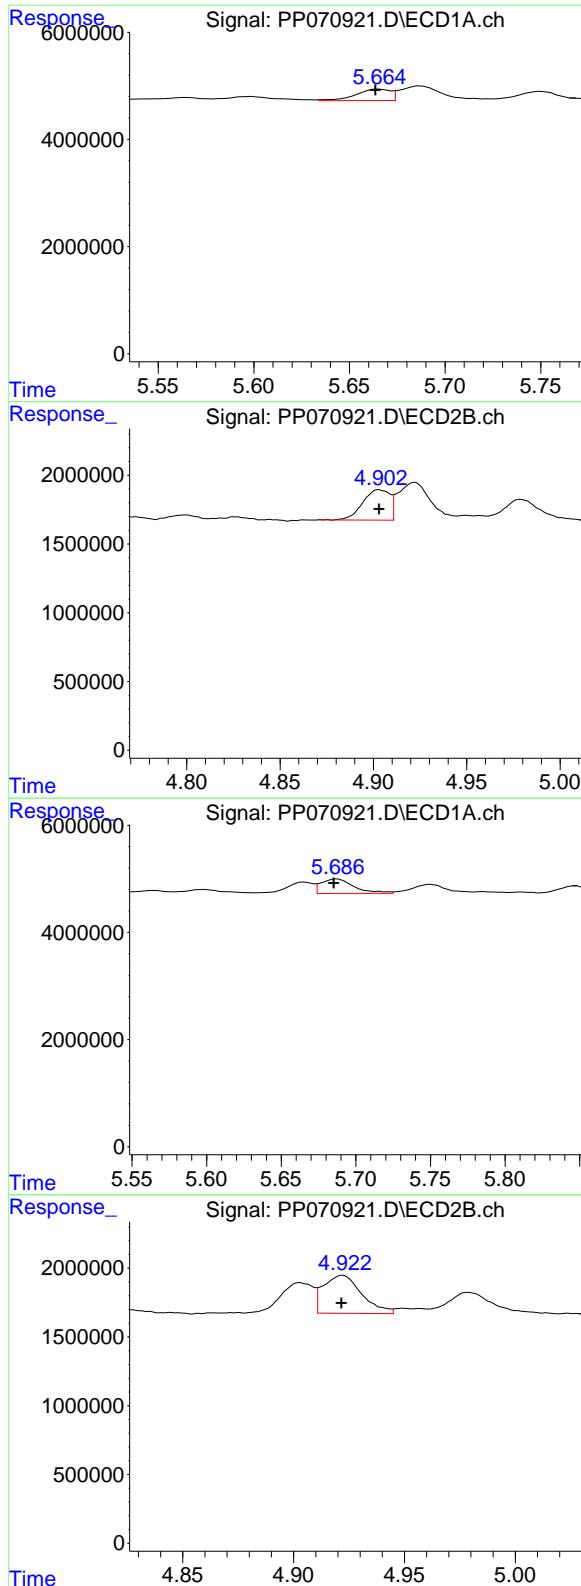

#3 AR-1016-1

R.T.: 5.666 min  
 Delta R.T.: 0.002 min **Instrument:**  
 Response: 2617394 ECD\_P  
 Conc: 51.47 ng/ml **ClientSampleId:**  
 AR1660ICC050

#3 AR-1016-1


R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 2265971  
 Conc: 56.52 ng/ml

#4 AR-1016-2

R.T.: 5.688 min  
 Delta R.T.: 0.002 min  
 Response: 4198554  
 Conc: 53.79 ng/ml

#4 AR-1016-2

R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 3321854  
 Conc: 57.41 ng/ml

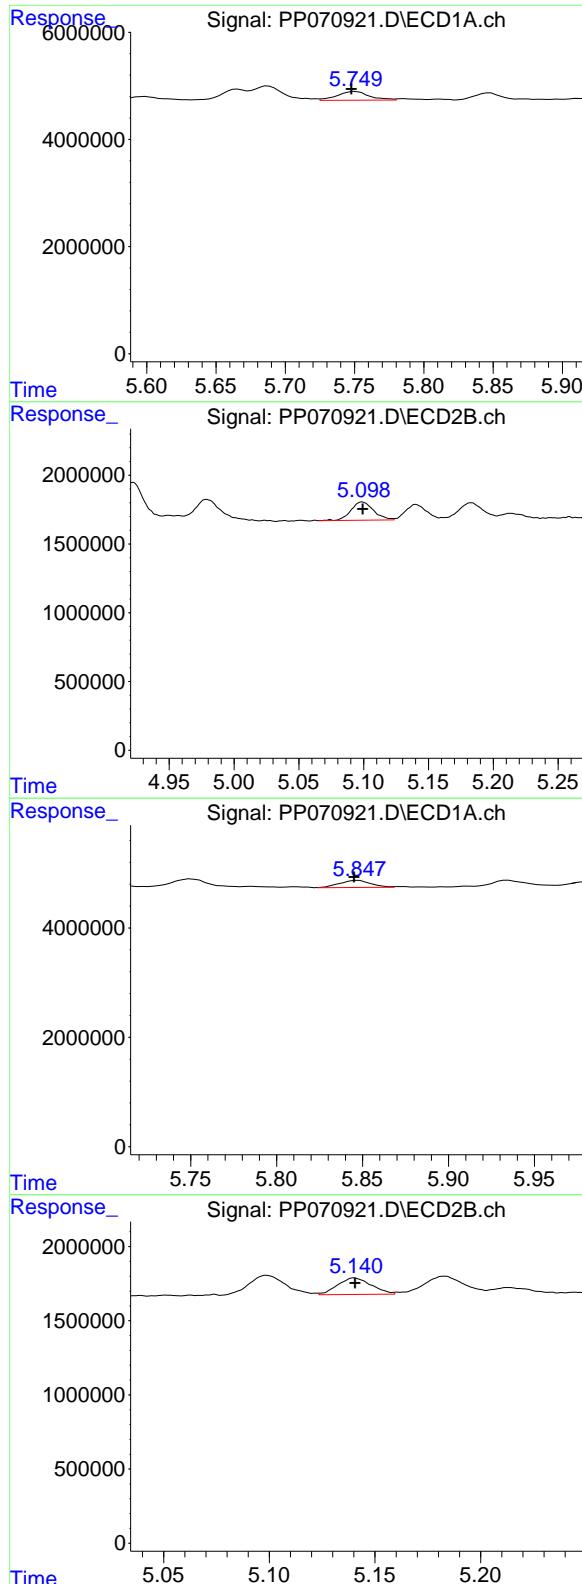

#5 AR-1016-3

R.T.: 5.751 min  
 Delta R.T.: 0.003 min  
 Response: 2631097  
 Conc: 55.77 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#5 AR-1016-3


R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 1626306  
 Conc: 52.59 ng/ml

#6 AR-1016-4

R.T.: 5.848 min  
 Delta R.T.: 0.003 min  
 Response: 1614372  
 Conc: 43.92 ng/ml

#6 AR-1016-4

R.T.: 5.140 min  
 Delta R.T.: 0.000 min  
 Response: 1232754  
 Conc: 50.61 ng/ml

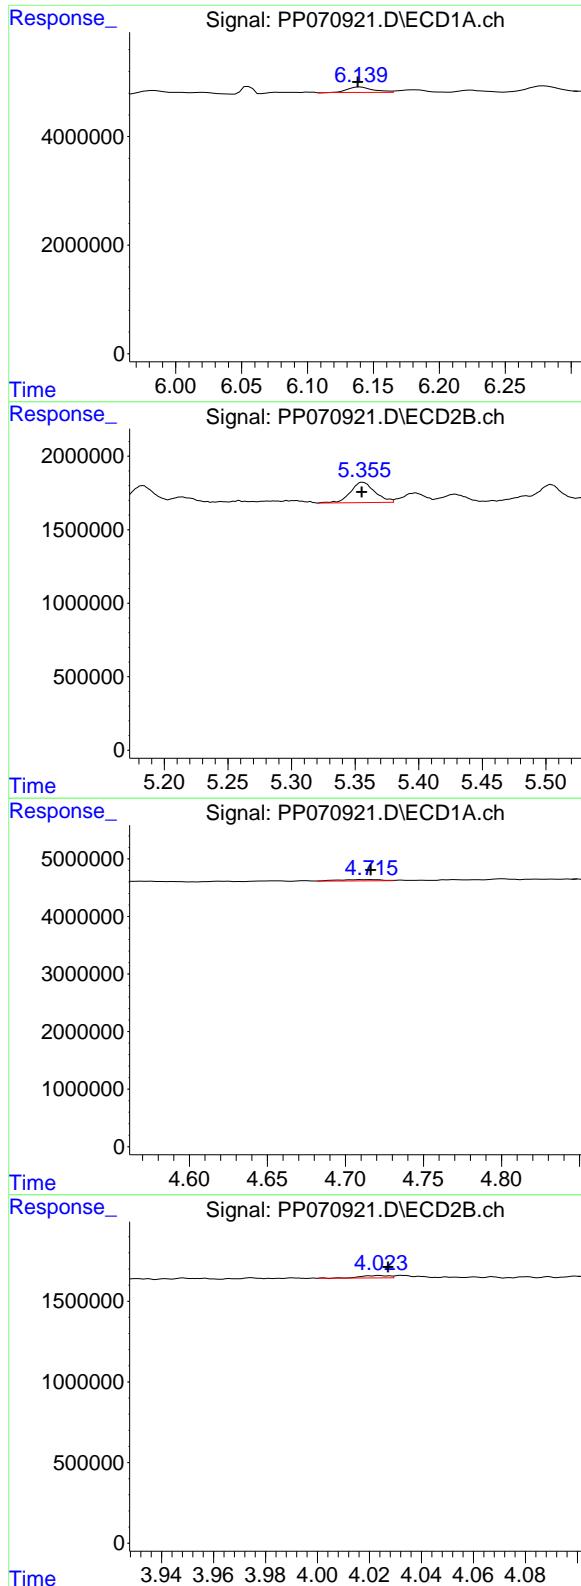

#7 AR-1016-5

R.T.: 6.140 min  
 Delta R.T.: 0.002 min  
 Response: 1323106  
 Conc: 39.02 ng/ml

Instrument: ECD\_P  
 ClientSampleId : AR1660ICC050

#7 AR-1016-5


R.T.: 5.356 min  
 Delta R.T.: 0.000 min  
 Response: 1866333  
 Conc: 57.74 ng/ml

#8 AR-1221-1

R.T.: 4.717 min  
 Delta R.T.: 0.000 min  
 Response: 421830  
 Conc: 24.31 ng/ml

#8 AR-1221-1

R.T.: 4.024 min  
 Delta R.T.: -0.004 min  
 Response: 114713  
 Conc: 7.53 ng/ml

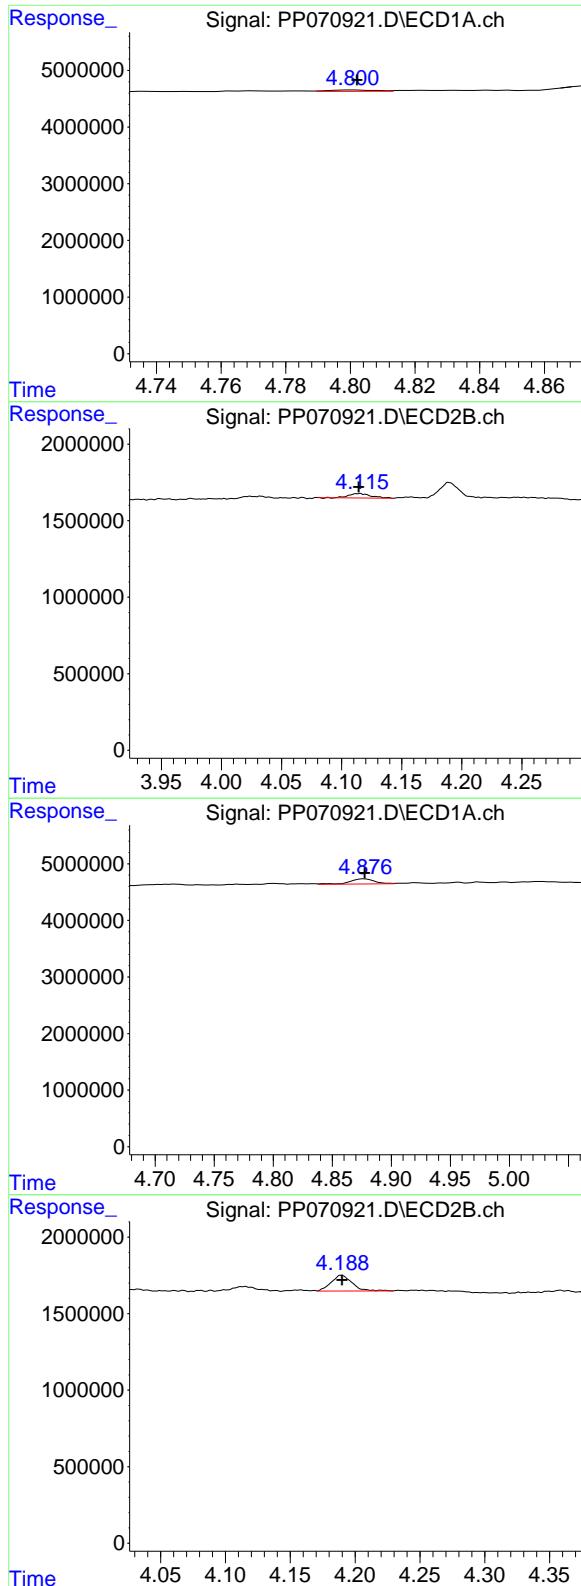

#9 AR-1221-2

R.T.: 4.801 min  
 Delta R.T.: -0.001 min Instrument:  
 Response: 218742 ECD\_P  
 Conc: 16.89 ng/ml ClientSampleId :  
 AR1660ICC050

#9 AR-1221-2


R.T.: 4.115 min  
 Delta R.T.: 0.000 min  
 Response: 388578  
 Conc: 33.98 ng/ml

#10 AR-1221-3

R.T.: 4.877 min  
 Delta R.T.: 0.000 min  
 Response: 1349629  
 Conc: 32.35 ng/ml

#10 AR-1221-3

R.T.: 4.189 min  
 Delta R.T.: 0.000 min  
 Response: 1162778  
 Conc: 34.11 ng/ml

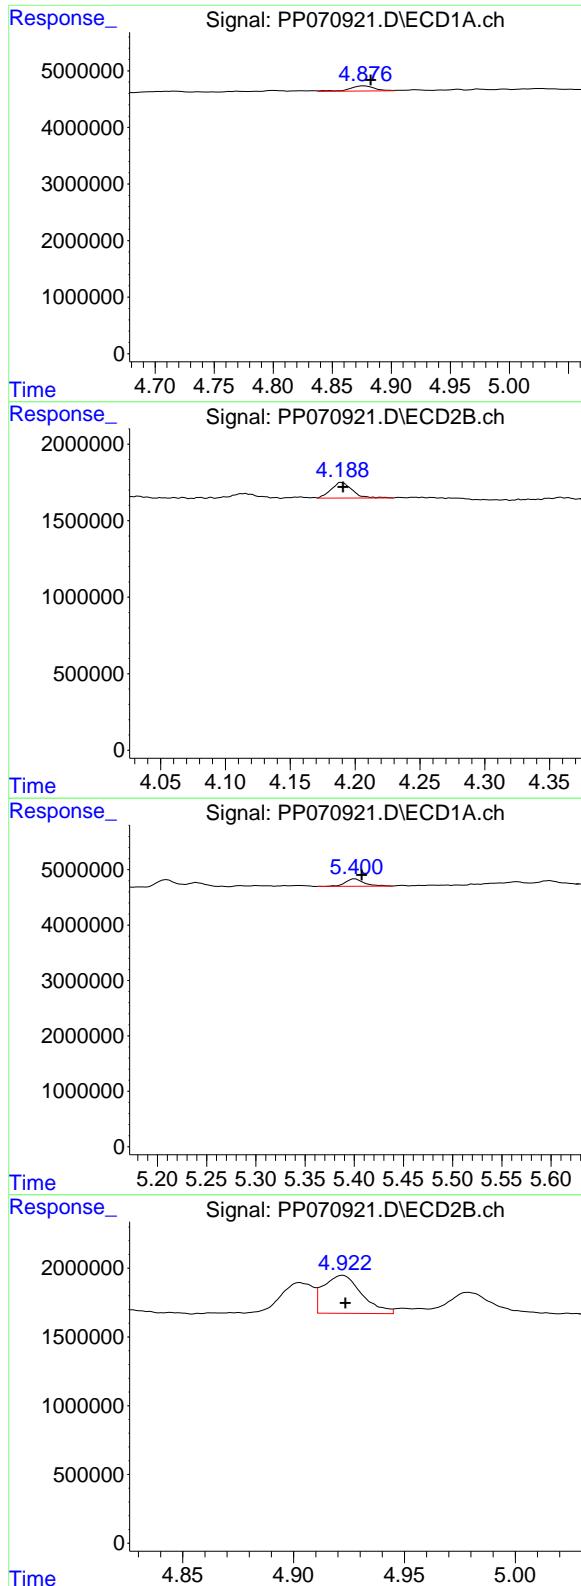

#11 AR-1232-1

R.T.: 4.877 min  
 Delta R.T.: -0.005 min  
 Response: 1349629  
 Conc: 40.54 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#11 AR-1232-1


R.T.: 4.189 min  
 Delta R.T.: -0.001 min  
 Response: 1162778  
 Conc: 41.55 ng/ml

#12 AR-1232-2

R.T.: 5.401 min  
 Delta R.T.: -0.007 min  
 Response: 1794886  
 Conc: 112.81 ng/ml

#12 AR-1232-2

R.T.: 4.922 min  
 Delta R.T.: -0.001 min  
 Response: 3321854  
 Conc: 118.38 ng/ml

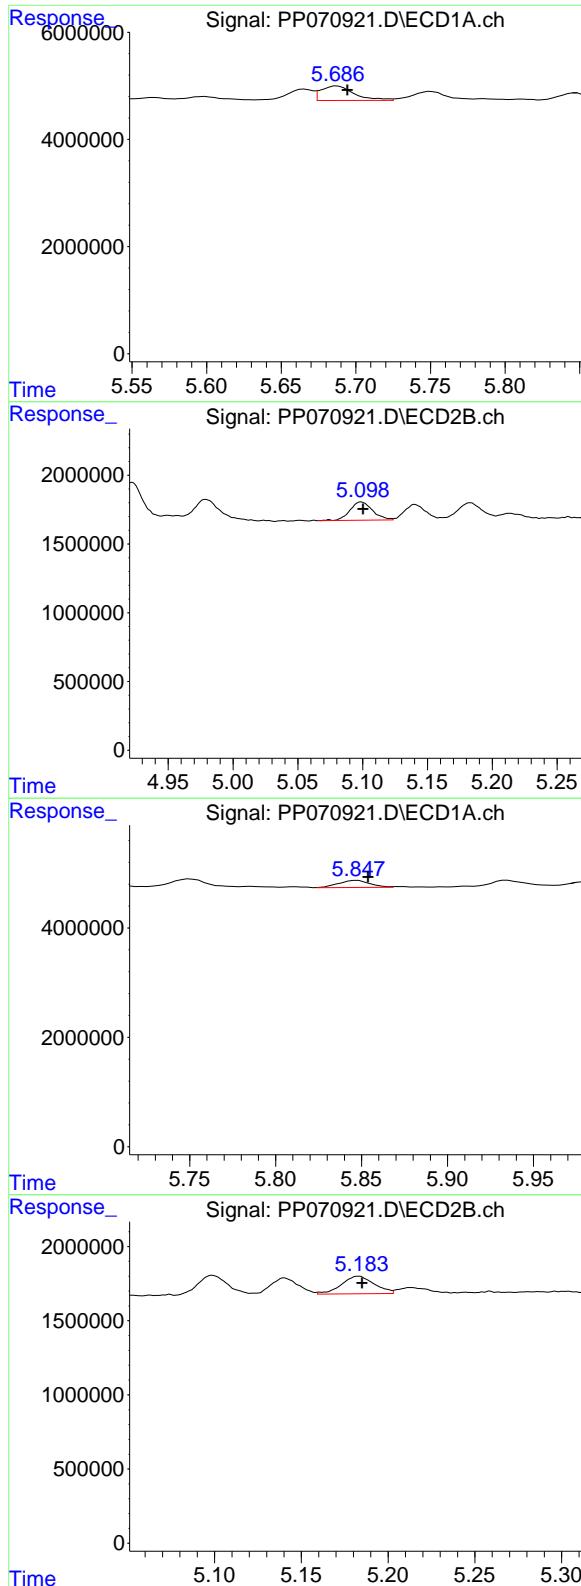

#13 AR-1232-3

R.T.: 5.688 min  
 Delta R.T.: -0.007 min  
 Response: 4198554  
 Conc: 122.51 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#13 AR-1232-3


R.T.: 5.099 min  
 Delta R.T.: -0.002 min  
 Response: 1626306  
 Conc: 109.22 ng/ml

#14 AR-1232-4

R.T.: 5.848 min  
 Delta R.T.: -0.006 min  
 Response: 1614372  
 Conc: 102.78 ng/ml

#14 AR-1232-4

R.T.: 5.183 min  
 Delta R.T.: -0.002 min  
 Response: 1568895  
 Conc: 122.53 ng/ml

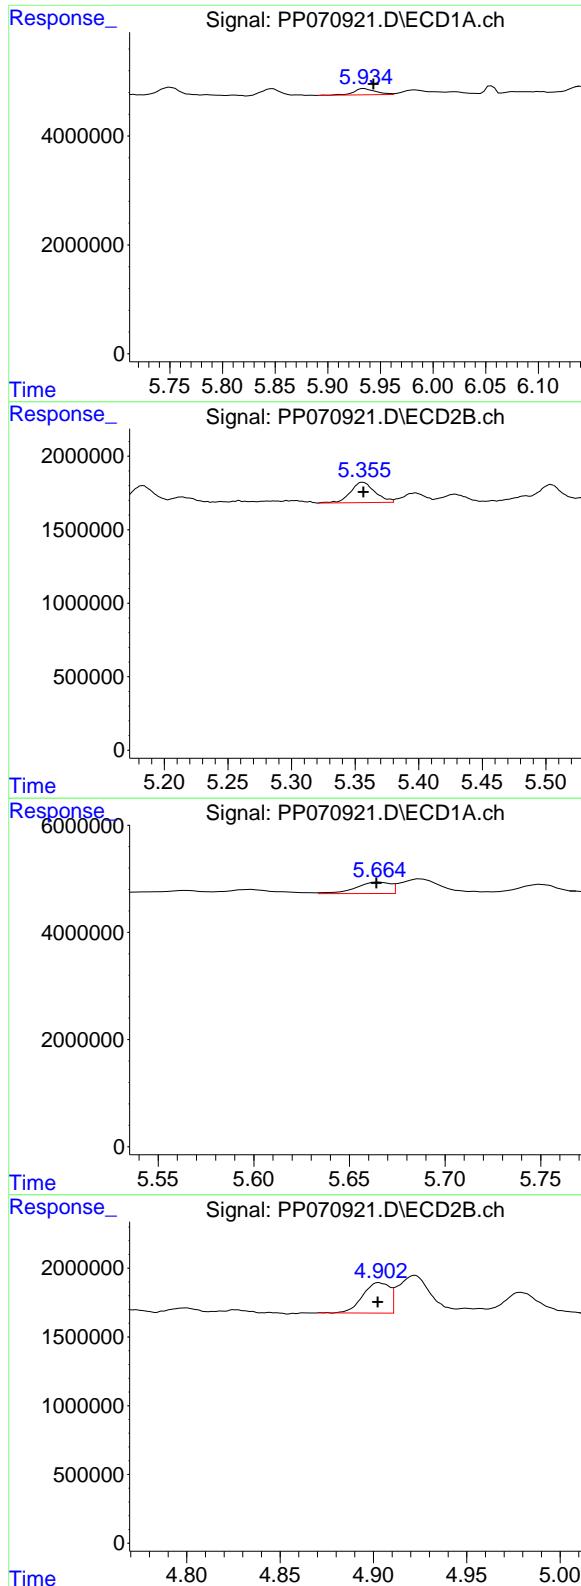

#15 AR-1232-5

R.T.: 5.935 min  
 Delta R.T.: -0.009 min  
 Response: 1663453  
 Conc: 156.33 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#15 AR-1232-5


R.T.: 5.356 min  
 Delta R.T.: 0.000 min  
 Response: 1866333  
 Conc: 131.67 ng/ml

#16 AR-1242-1

R.T.: 5.666 min  
 Delta R.T.: 0.002 min  
 Response: 2617394  
 Conc: 59.52 ng/ml

#16 AR-1242-1

R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 2265971  
 Conc: 66.26 ng/ml

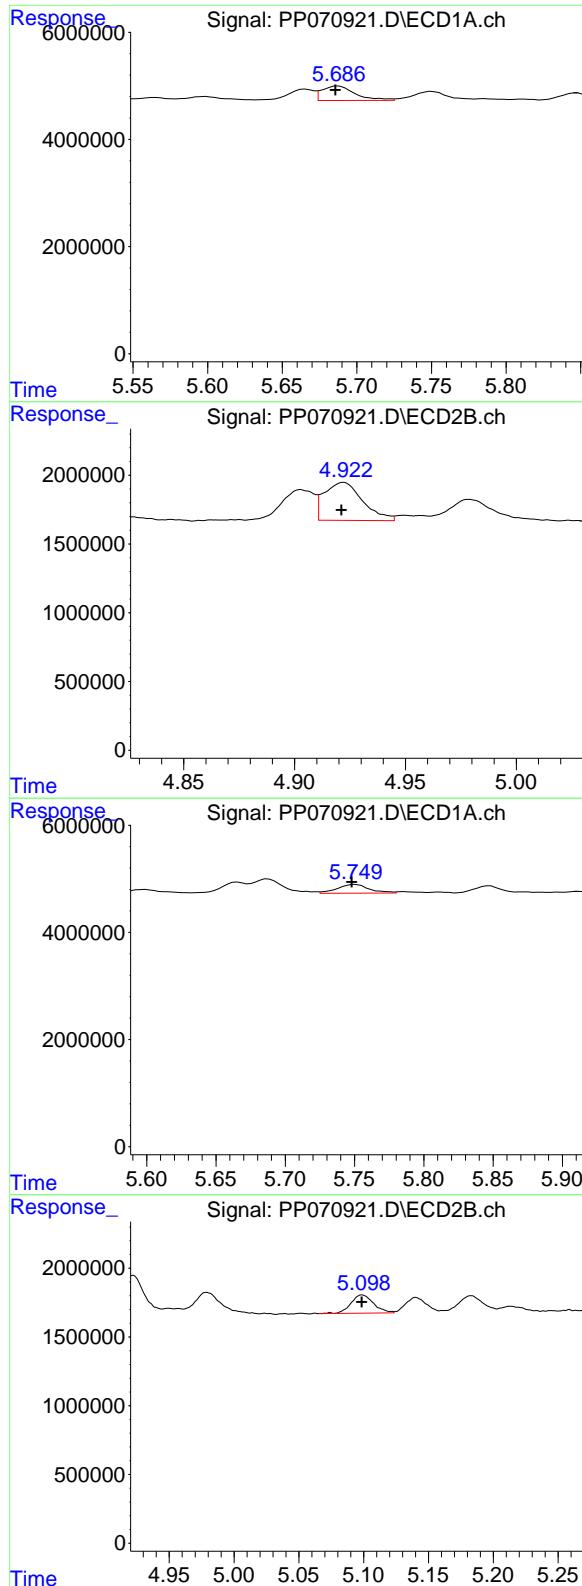

#17 AR-1242-2

R.T.: 5.688 min  
 Delta R.T.: 0.002 min  
 Response: 4198554  
 Conc: 65.28 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#17 AR-1242-2


R.T.: 4.922 min  
 Delta R.T.: 0.000 min  
 Response: 3321854  
 Conc: 67.44 ng/ml

#18 AR-1242-3

R.T.: 5.751 min  
 Delta R.T.: 0.003 min  
 Response: 2631097  
 Conc: 64.11 ng/ml

#18 AR-1242-3

R.T.: 5.099 min  
 Delta R.T.: 0.000 min  
 Response: 1626306  
 Conc: 61.04 ng/ml

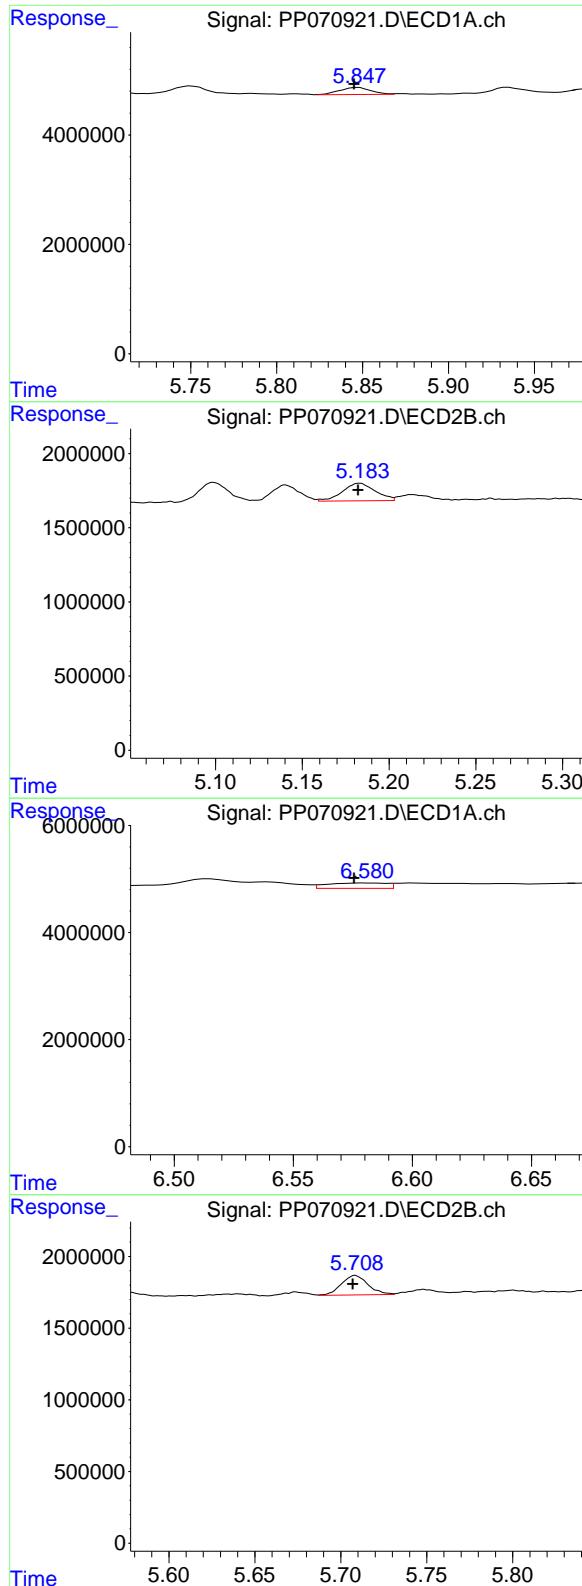

#19 AR-1242-4

R.T.: 5.848 min  
 Delta R.T.: 0.003 min  
 Response: 1614372  
 Conc: 52.89 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#19 AR-1242-4


R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 1568895  
 Conc: 59.48 ng/ml

#20 AR-1242-5

R.T.: 6.582 min  
 Delta R.T.: 0.006 min  
 Response: 1738801  
 Conc: 47.62 ng/ml

#20 AR-1242-5

R.T.: 5.708 min  
 Delta R.T.: 0.001 min  
 Response: 1466013  
 Conc: 47.35 ng/ml

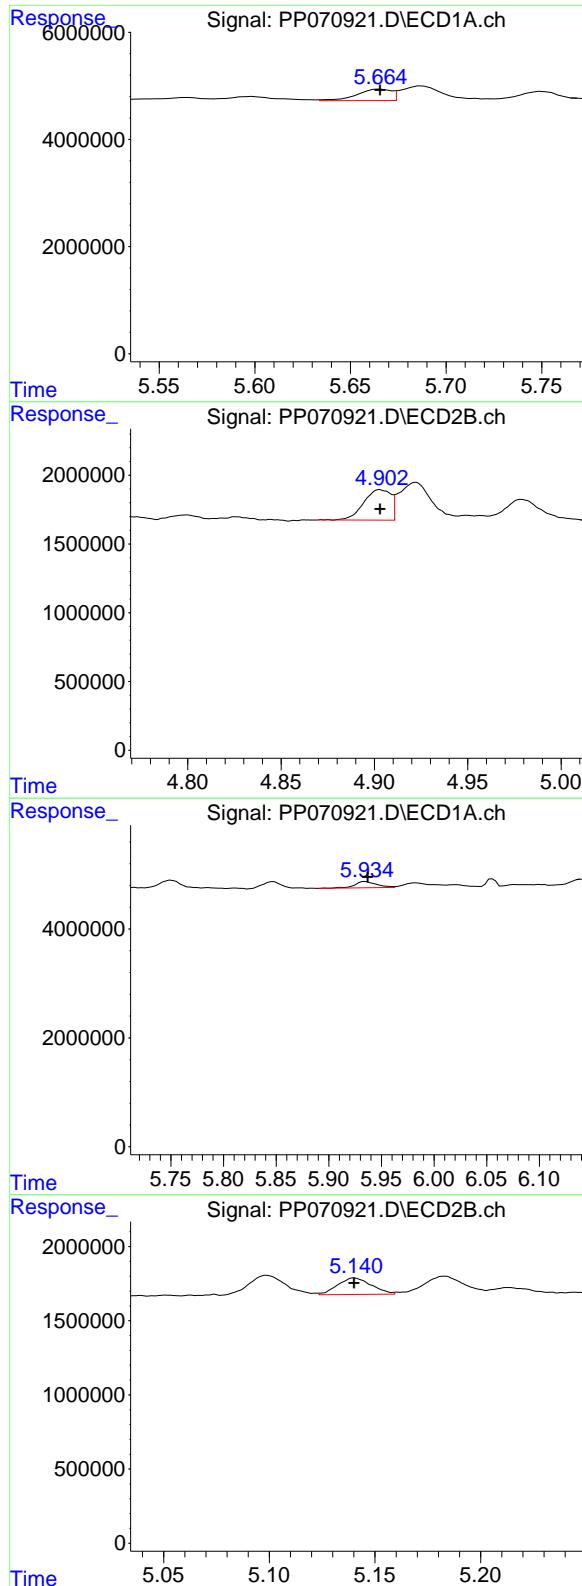

#21 AR-1248-1

R.T.: 5.666 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 2617394 ECD\_P  
 Conc: 72.13 ng/ml **ClientSampleId:**  
 AR1660ICC050

#21 AR-1248-1


R.T.: 4.903 min  
 Delta R.T.: 0.000 min  
 Response: 2265971  
 Conc: 83.68 ng/ml

#22 AR-1248-2

R.T.: 5.935 min  
 Delta R.T.: -0.002 min  
 Response: 1663453  
 Conc: 37.02 ng/ml

#22 AR-1248-2

R.T.: 5.140 min  
 Delta R.T.: 0.000 min  
 Response: 1232754  
 Conc: 33.57 ng/ml

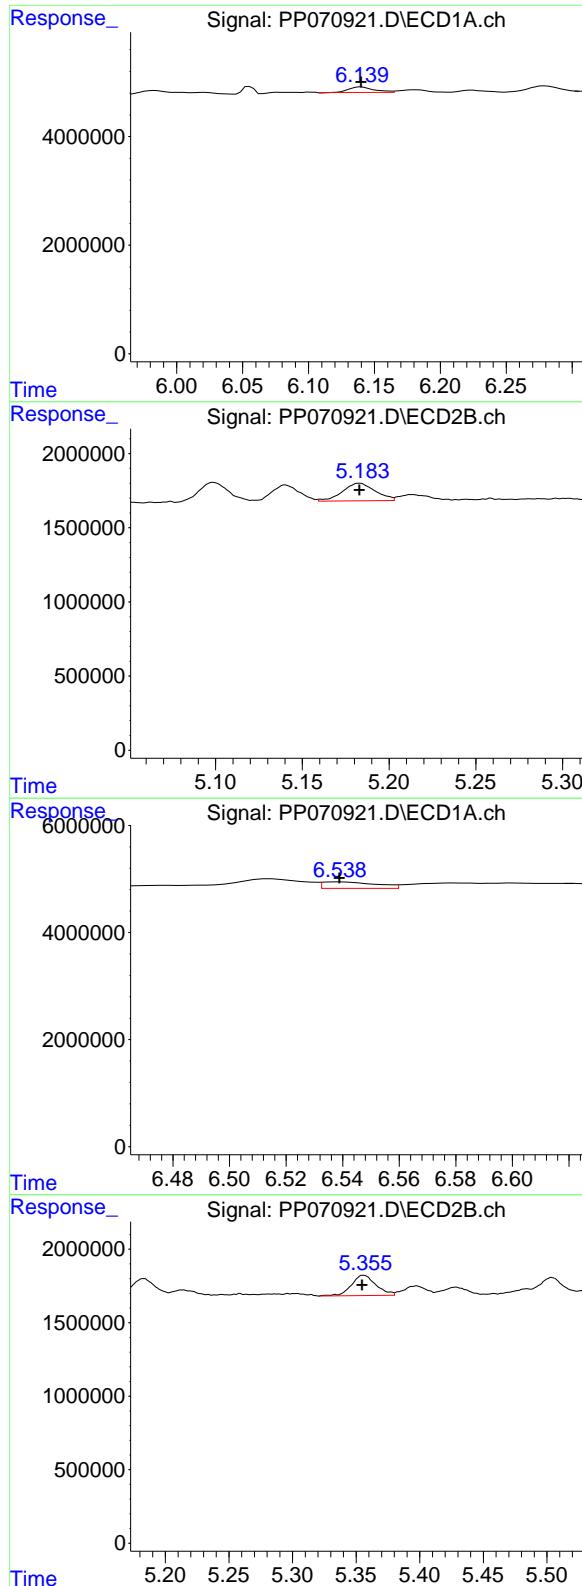

#23 AR-1248-3

R.T.: 6.140 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 1323106 ECD\_P  
 Conc: 26.13 ng/ml **ClientSampleId:**  
 AR1660ICC050

#23 AR-1248-3


R.T.: 5.183 min  
 Delta R.T.: 0.000 min  
 Response: 1568895  
 Conc: 40.58 ng/ml

#24 AR-1248-4

R.T.: 6.539 min  
 Delta R.T.: 0.000 min  
 Response: 1621071  
 Conc: 25.27 ng/ml

#24 AR-1248-4


R.T.: 5.356 min  
 Delta R.T.: 0.001 min  
 Response: 1866333  
 Conc: 41.34 ng/ml

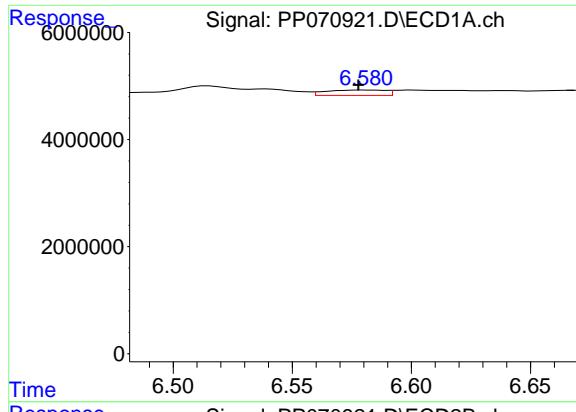

#25 AR-1248-5


R.T.: 6.582 min  
Delta R.T.: 0.004 min  
Response: 1738801  
Conc: 28.58 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660ICC050

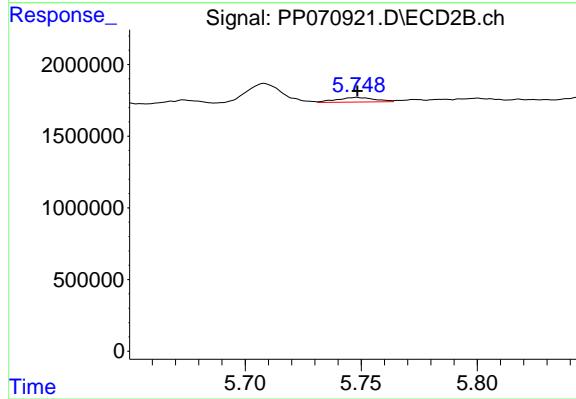


#25 AR-1248-5

R.T.: 5.748 min  
Delta R.T.: 0.000 min  
Response: 371096  
Conc: 8.70 ng/ml

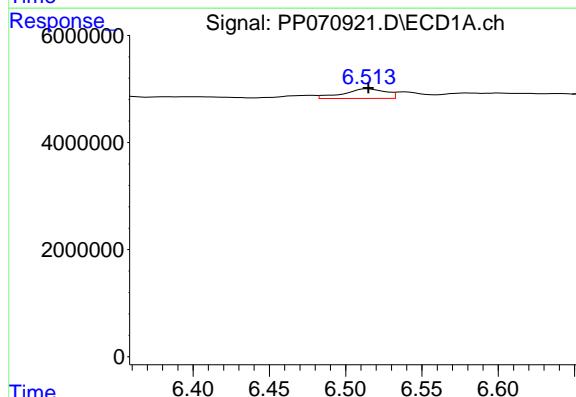


#26 AR-1254-1

R.T.: 6.515 min  
Delta R.T.: 0.000 min  
Response: 3489366  
Conc: 54.19 ng/ml

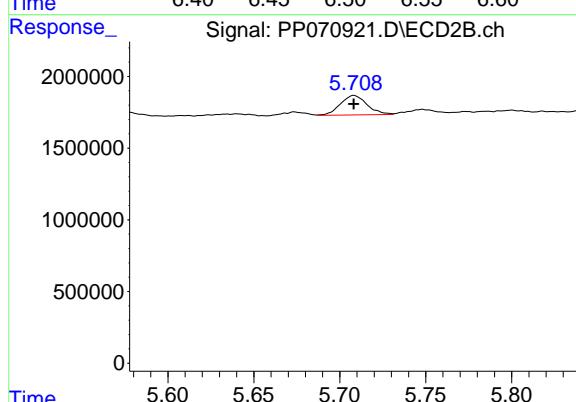

#26 AR-1254-1

R.T.: 5.708 min  
Delta R.T.: 0.000 min  
Response: 1466013  
Conc: 22.21 ng/ml

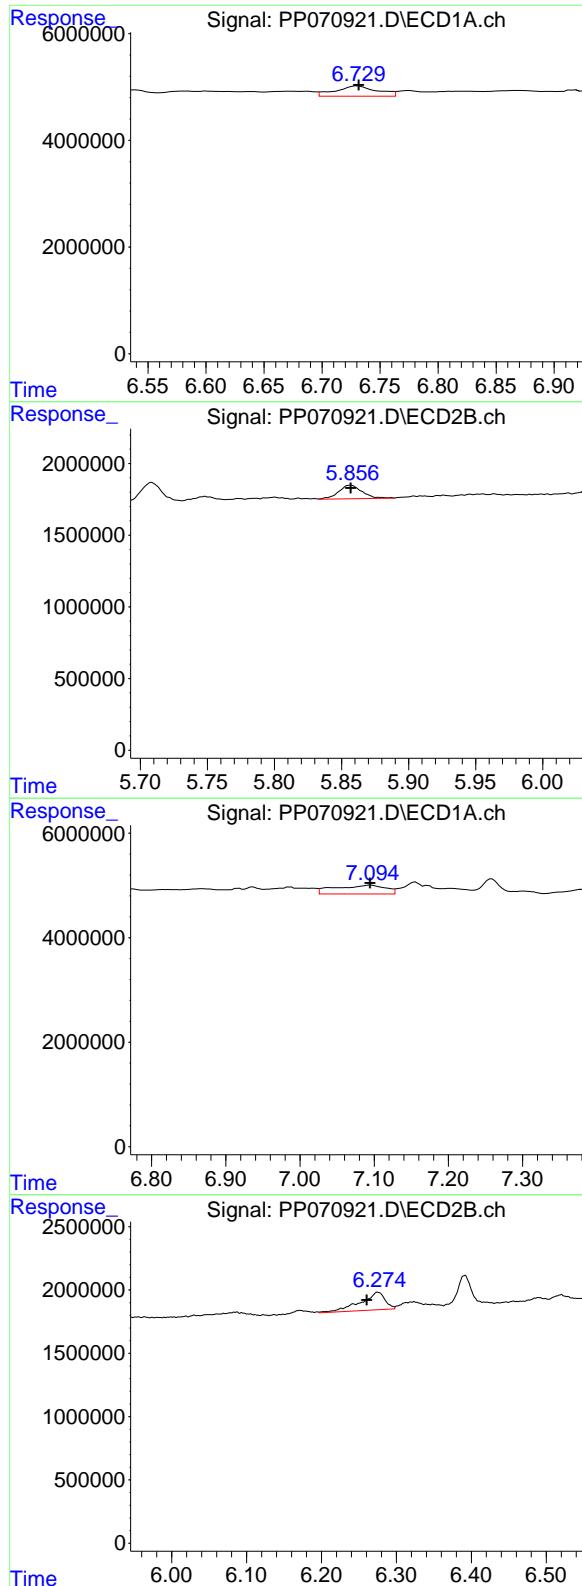

#27 AR-1254-2

R.T.: 6.731 min  
 Delta R.T.: 0.000 min  
 Response: 4772204  
 Conc: 47.21 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#27 AR-1254-2


R.T.: 5.857 min  
 Delta R.T.: 0.000 min  
 Response: 1146779  
 Conc: 20.08 ng/ml

#28 AR-1254-3

R.T.: 7.095 min  
 Delta R.T.: 0.000 min  
 Response: 7925059  
 Conc: 79.47 ng/ml

#28 AR-1254-3

R.T.: 6.275 min  
 Delta R.T.: 0.015 min  
 Response: 3163207  
 Conc: 36.43 ng/ml

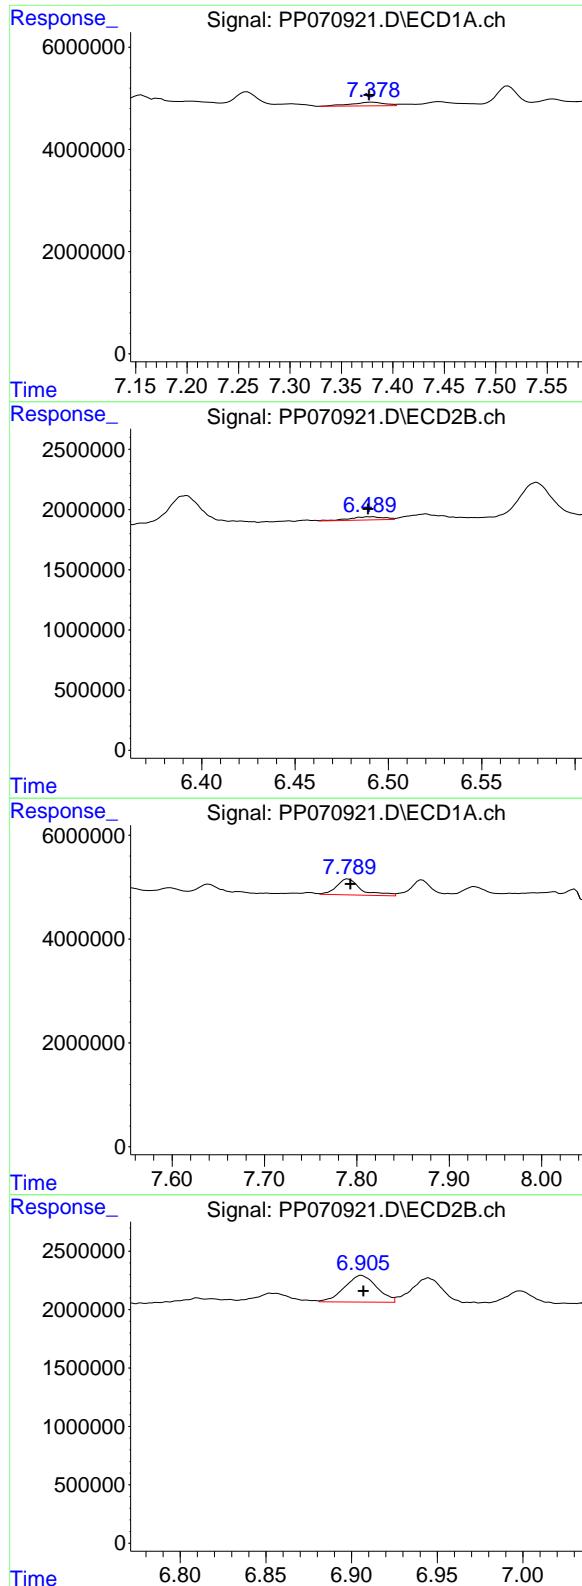

#29 AR-1254-4

R.T.: 7.380 min  
 Delta R.T.: 0.003 min  
 Response: 1640237  
 Conc: 18.94 ng/ml

**Instrument:** ECD\_P  
**ClientSampleId:** AR1660ICC050

#29 AR-1254-4


R.T.: 6.490 min  
 Delta R.T.: 0.001 min  
 Response: 349900  
 Conc: 6.24 ng/ml

#30 AR-1254-5

R.T.: 7.791 min  
 Delta R.T.: -0.002 min  
 Response: 5692306  
 Conc: 70.84 ng/ml

#30 AR-1254-5

R.T.: 6.906 min  
 Delta R.T.: -0.001 min  
 Response: 2994420  
 Conc: 41.50 ng/ml

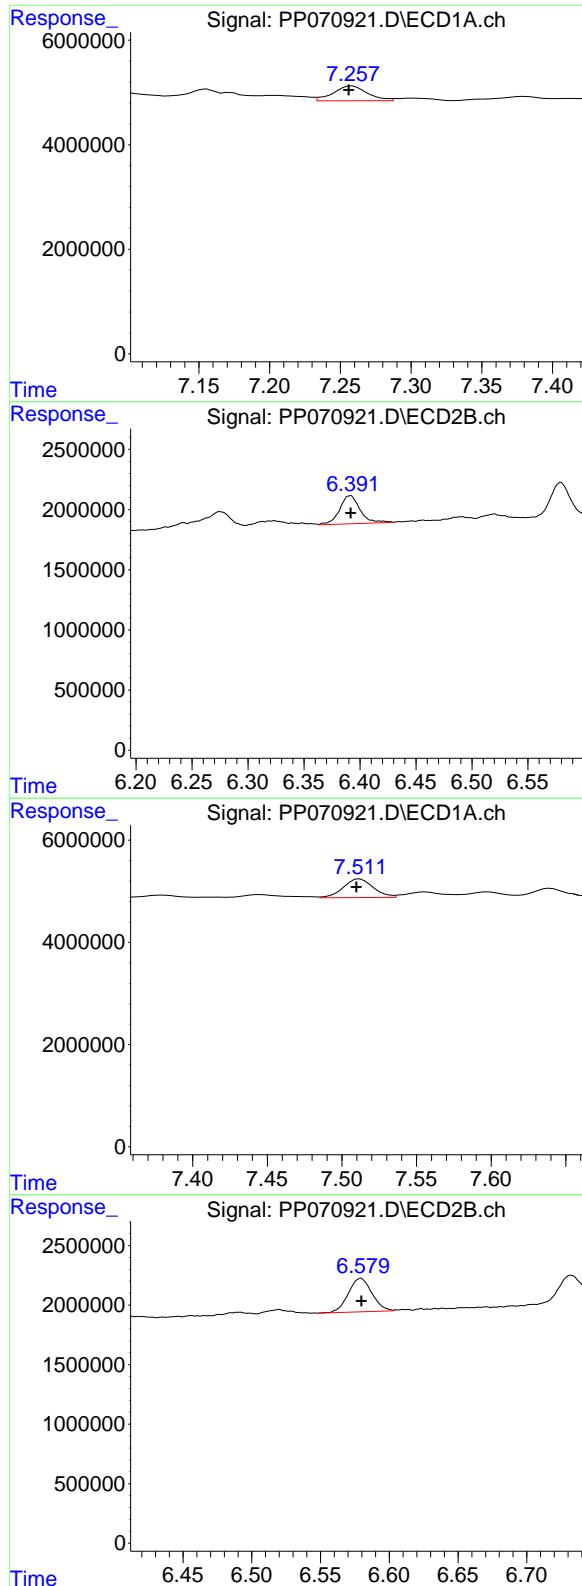

#31 AR-1260-1

R.T.: 7.258 min  
 Delta R.T.: 0.003 min  
 Response: 4772844  
 Conc: 71.07 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#31 AR-1260-1


R.T.: 6.391 min  
 Delta R.T.: 0.000 min  
 Response: 2989801  
 Conc: 58.39 ng/ml

#32 AR-1260-2

R.T.: 7.512 min  
 Delta R.T.: 0.002 min  
 Response: 5123964  
 Conc: 53.30 ng/ml

#32 AR-1260-2

R.T.: 6.579 min  
 Delta R.T.: 0.000 min  
 Response: 3357287  
 Conc: 52.63 ng/ml

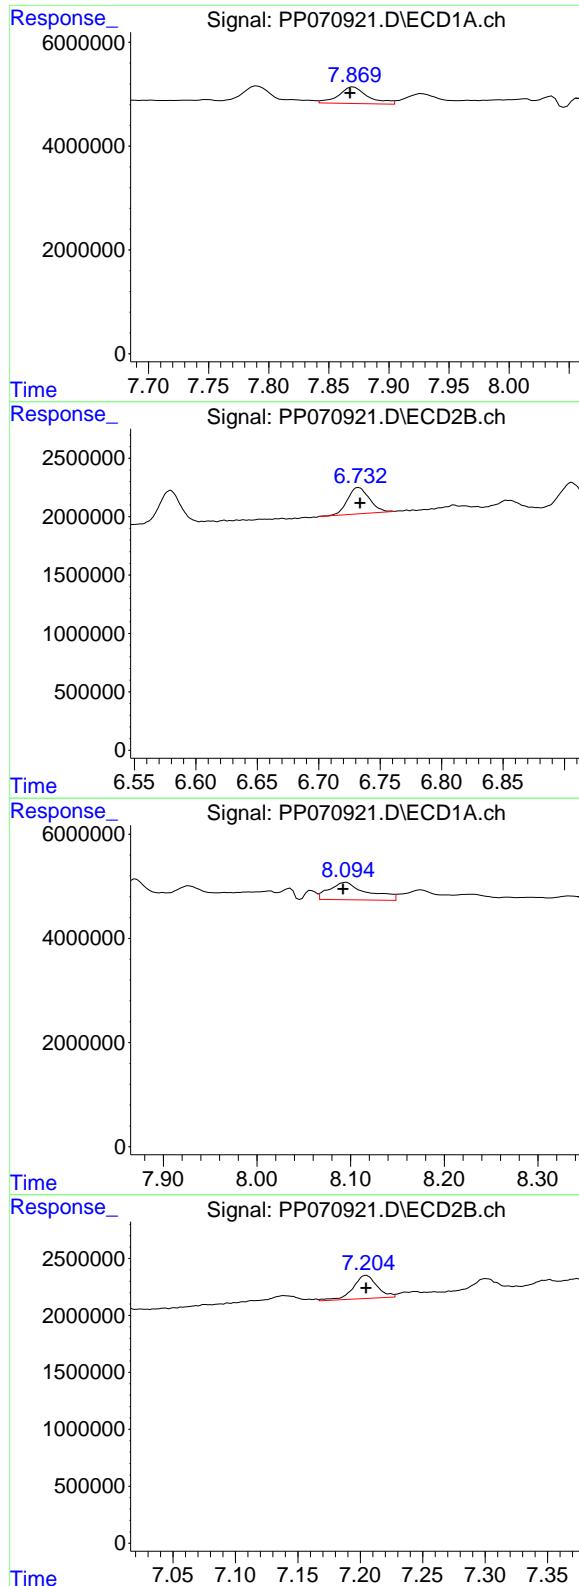

#33 AR-1260-3

R.T.: 7.871 min  
 Delta R.T.: 0.003 min  
 Response: 5463057  
 Conc: 68.36 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660ICC050

#33 AR-1260-3


R.T.: 6.732 min  
 Delta R.T.: -0.001 min  
 Response: 2827385  
 Conc: 51.89 ng/ml

#34 AR-1260-4

R.T.: 8.095 min  
 Delta R.T.: 0.004 min  
 Response: 9380427  
 Conc: 119.14 ng/ml

#34 AR-1260-4


R.T.: 7.205 min  
 Delta R.T.: 0.000 min  
 Response: 2746307  
 Conc: 57.42 ng/ml

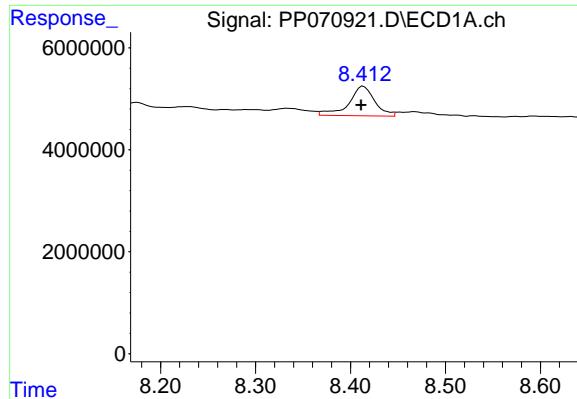

#35 AR-1260-5


R.T.: 8.414 min  
Delta R.T.: 0.002 min  
Response: 11051960  
Conc: 69.56 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660ICC050

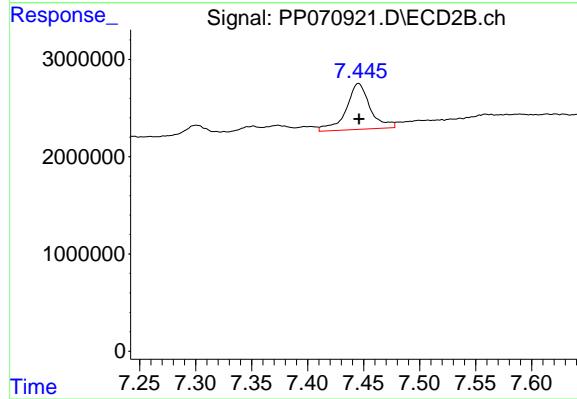


#35 AR-1260-5

R.T.: 7.445 min  
Delta R.T.: 0.000 min  
Response: 7013440  
Conc: 56.33 ng/ml

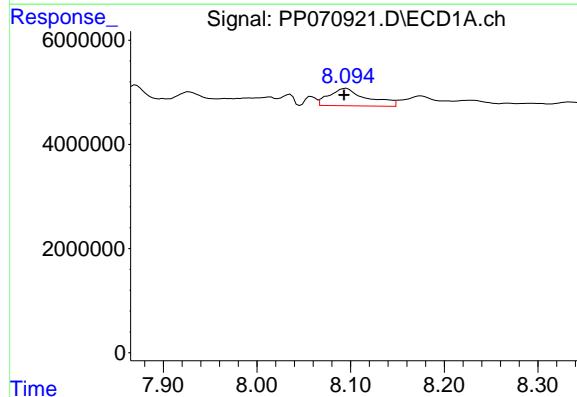


#36 AR-1262-1

R.T.: 8.095 min  
Delta R.T.: 0.003 min  
Response: 9380427  
Conc: 88.24 ng/ml

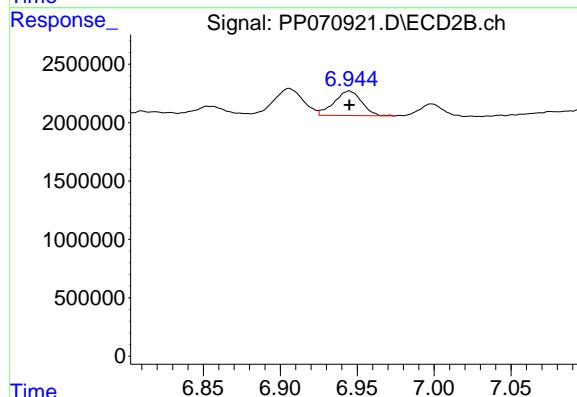

#36 AR-1262-1


R.T.: 6.945 min  
Delta R.T.: 0.000 min  
Response: 2613596  
Conc: 30.55 ng/ml

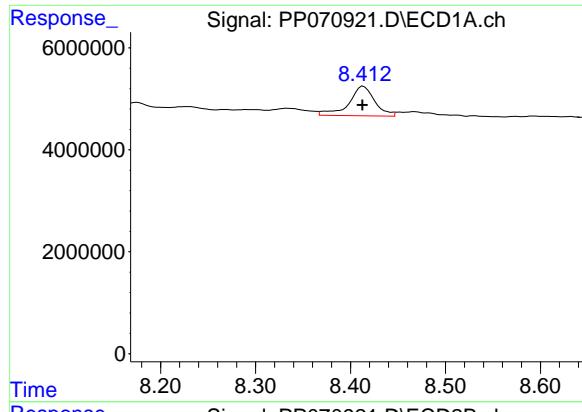

#37 AR-1262-2


R.T.: 8.414 min  
Delta R.T.: 0.001 min  
Response: 11051960  
Conc: 55.71 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660ICC050

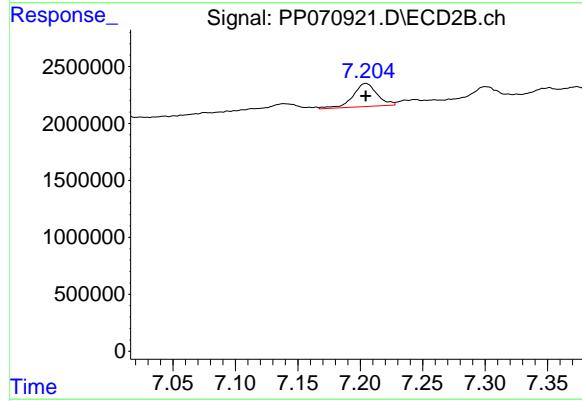


#37 AR-1262-2

R.T.: 7.205 min  
Delta R.T.: 0.000 min  
Response: 2746307  
Conc: 40.11 ng/ml

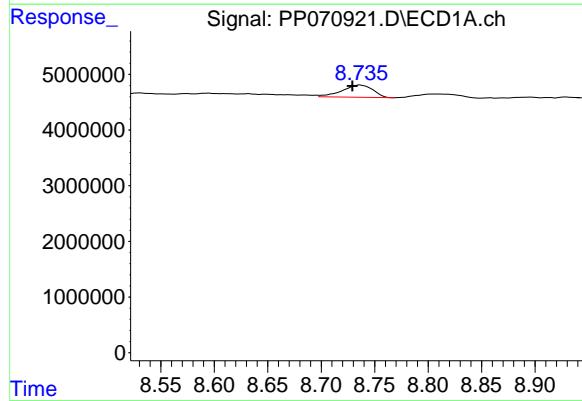


#38 AR-1262-3

R.T.: 8.737 min  
Delta R.T.: 0.008 min  
Response: 4423235  
Conc: 33.58 ng/ml

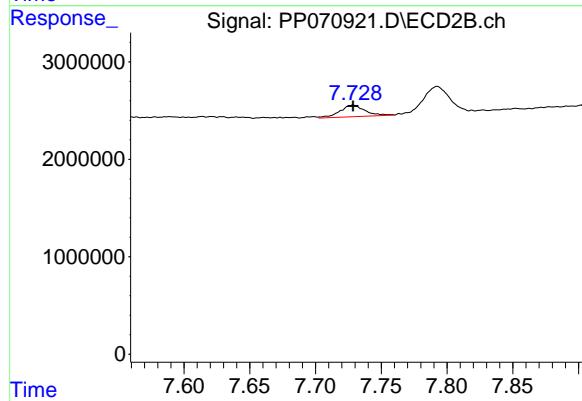

#38 AR-1262-3

R.T.: 7.729 min  
Delta R.T.: 0.000 min  
Response: 1556480  
Conc: 25.63 ng/ml

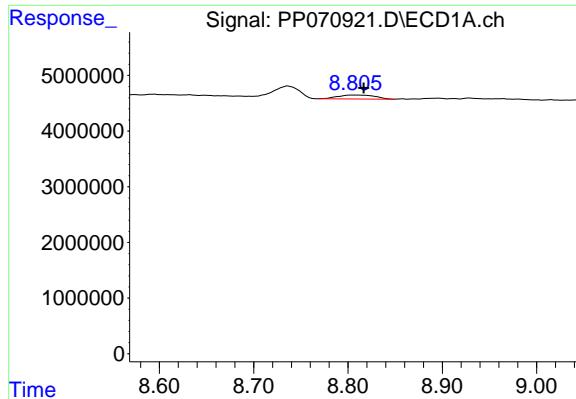

#39 AR-1262-4


R.T.: 8.806 min  
Delta R.T.: -0.011 min  
Response: 1951193  
Conc: 20.41 ng/ml

Instrument:

ECD\_P


ClientSampleId :

AR1660ICC050

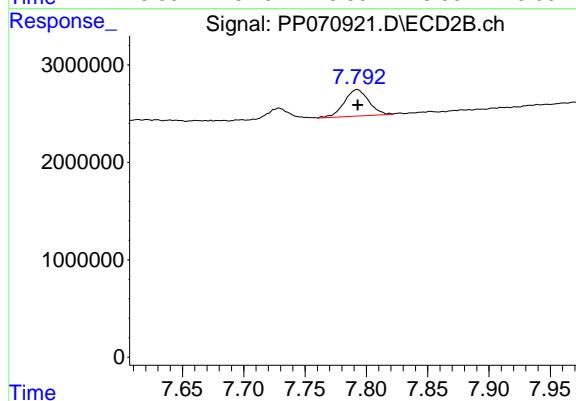


#39 AR-1262-4

R.T.: 7.792 min  
Delta R.T.: 0.000 min  
Response: 3771123  
Conc: 37.94 ng/ml

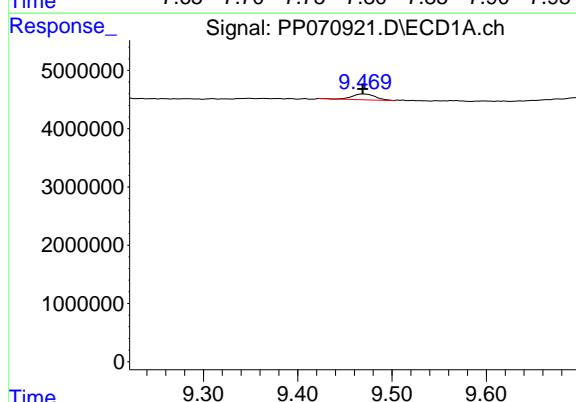


#40 AR-1262-5

R.T.: 9.470 min  
Delta R.T.: 0.001 min  
Response: 1729860  
Conc: 26.59 ng/ml

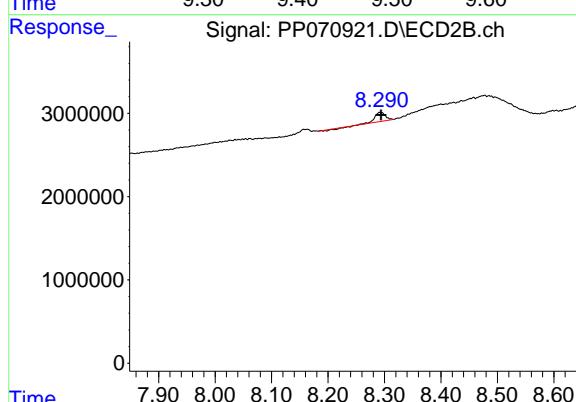

#40 AR-1262-5


R.T.: 8.292 min  
Delta R.T.: -0.002 min  
Response: 1260427  
Conc: 26.89 ng/ml

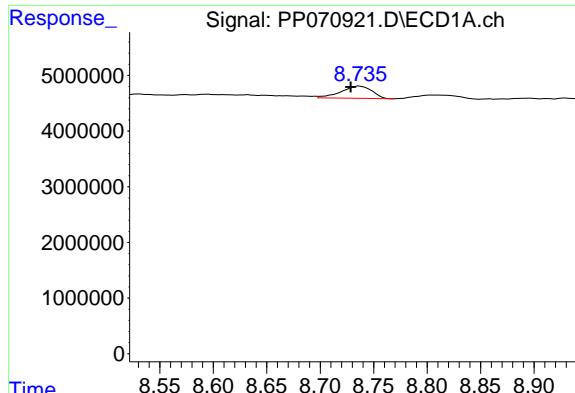

#41 AR-1268-1


R.T.: 8.737 min  
Delta R.T.: 0.008 min  
Response: 4423235  
Conc: 18.78 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660ICC050

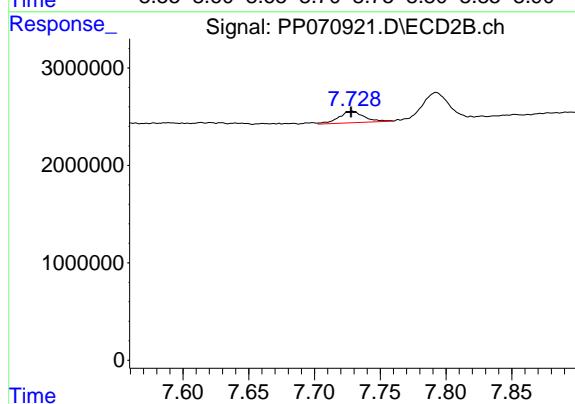


#41 AR-1268-1

R.T.: 7.729 min  
Delta R.T.: 0.001 min  
Response: 1556480  
Conc: 9.08 ng/ml

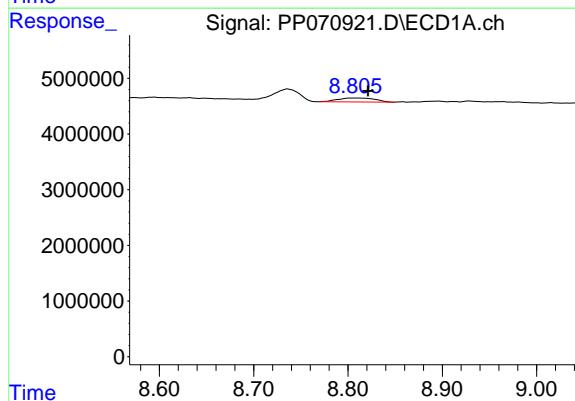


#42 AR-1268-2

R.T.: 8.806 min  
Delta R.T.: -0.016 min  
Response: 1951193  
Conc: 9.99 ng/ml

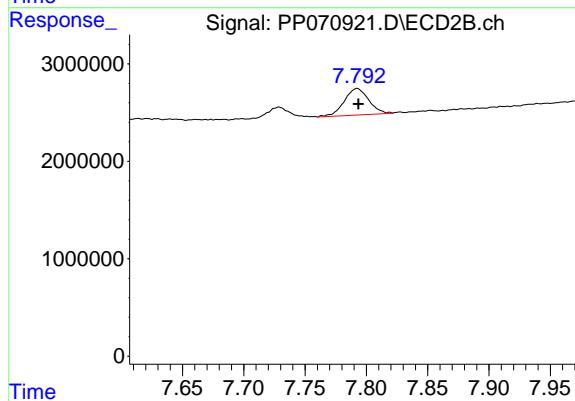


#42 AR-1268-2

R.T.: 7.792 min  
Delta R.T.: -0.001 min  
Response: 3771123  
Conc: 26.32 ng/ml




#43 AR-1268-3

R.T.: 0.000 min  
Exp R.T. : 9.053 min Instrument:  
Response: 0 ECD\_P  
Conc: N.D. ClientSampleId :  
AR1660ICC050

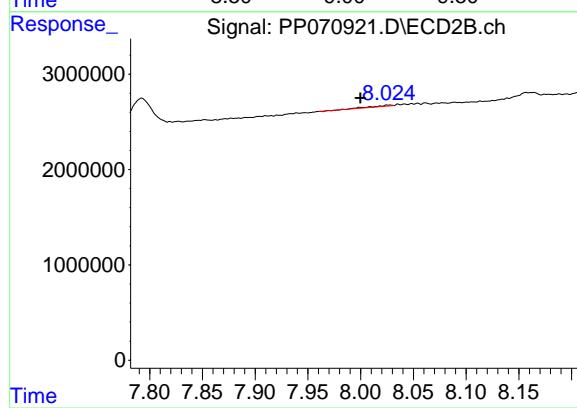


#43 AR-1268-3

R.T.: 8.026 min  
Delta R.T.: 0.026 min  
Response: 152620  
Conc: 1.24 ng/ml

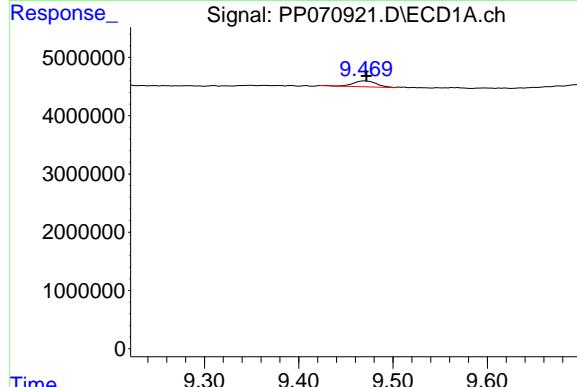

#44 AR-1268-4

R.T.: 9.470 min  
Delta R.T.: -0.002 min  
Response: 1729860  
Conc: 24.45 ng/ml

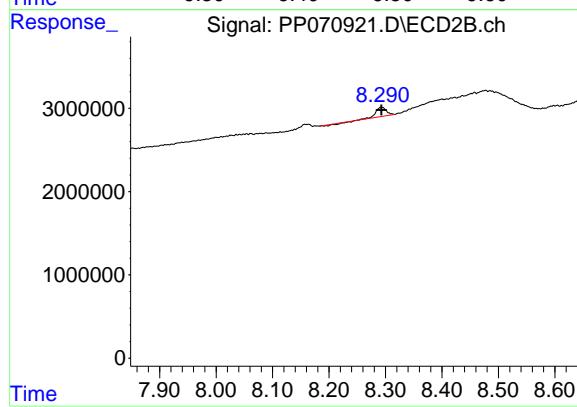

#44 AR-1268-4

R.T.: 8.292 min  
Delta R.T.: -0.001 min  
Response: 1260427  
Conc: 23.87 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070923.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 12:11  
 Operator : YP\AJ  
 Sample : AR1232ICC500  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1232ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:39:29 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 12:38:20 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.520	3.817	74435949	51438566	50.000	50.000
2) SA Decachlor...	10.236	8.860	99828492	40517792	110.430	50.000 #

Target Compounds

11) L3 AR-1232-1	4.883	4.191	16644355	13993352	500.000	500.000
12) L3 AR-1232-2	5.408	4.923	7955169	14030567	500.000	500.000
13) L3 AR-1232-3	5.694	5.100	17135200	7444793	500.000	500.000
14) L3 AR-1232-4	5.854	5.185	7853790	6402183	500.000	500.000
15) L3 AR-1232-5	5.943	5.357	5320177	7087391	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070923.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 12:11  
 Operator : YP\AJ  
 Sample : AR1232ICC500  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1232ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 12:39:29 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 12:38:20 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

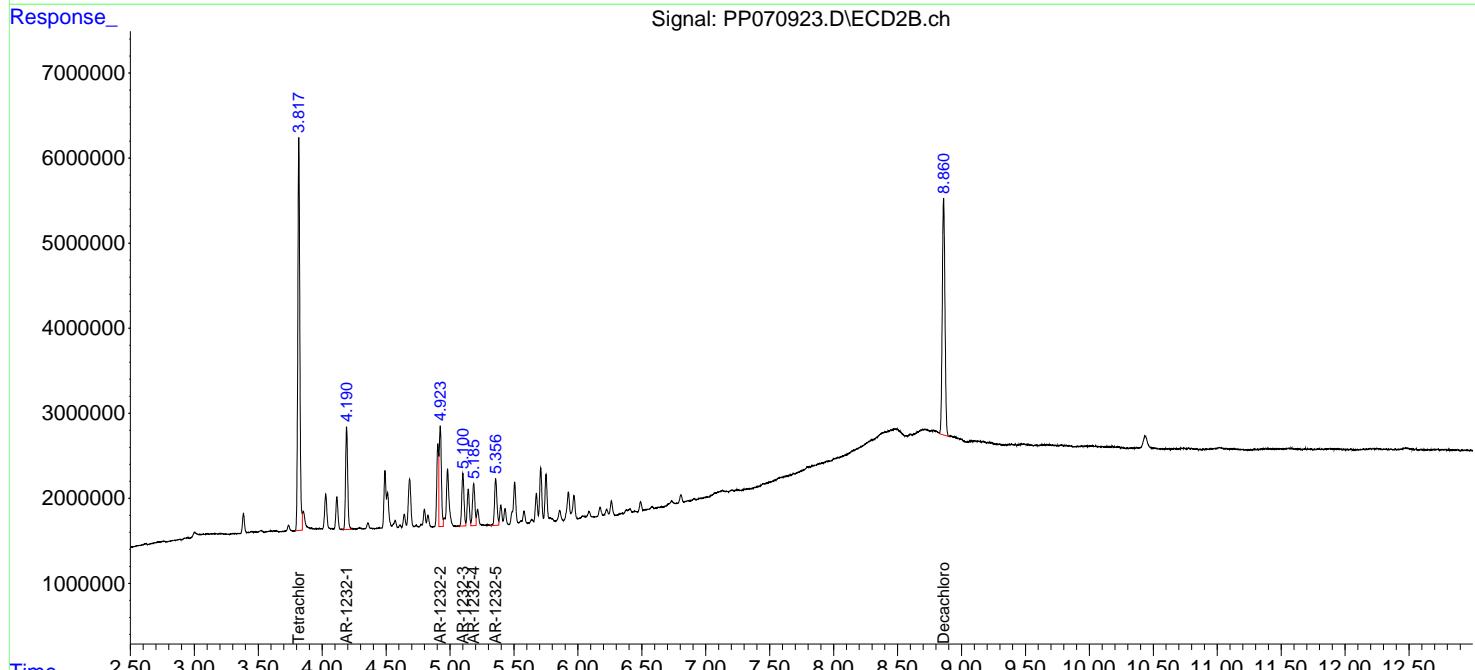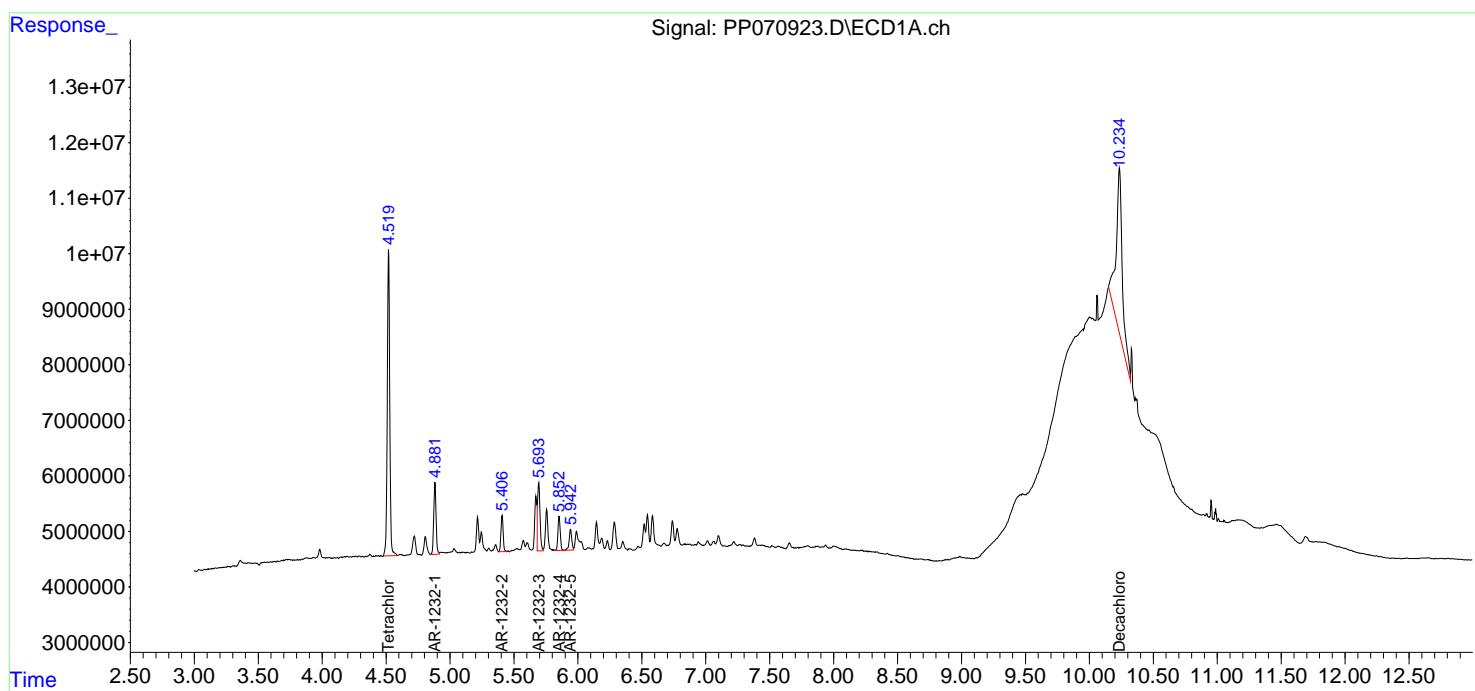

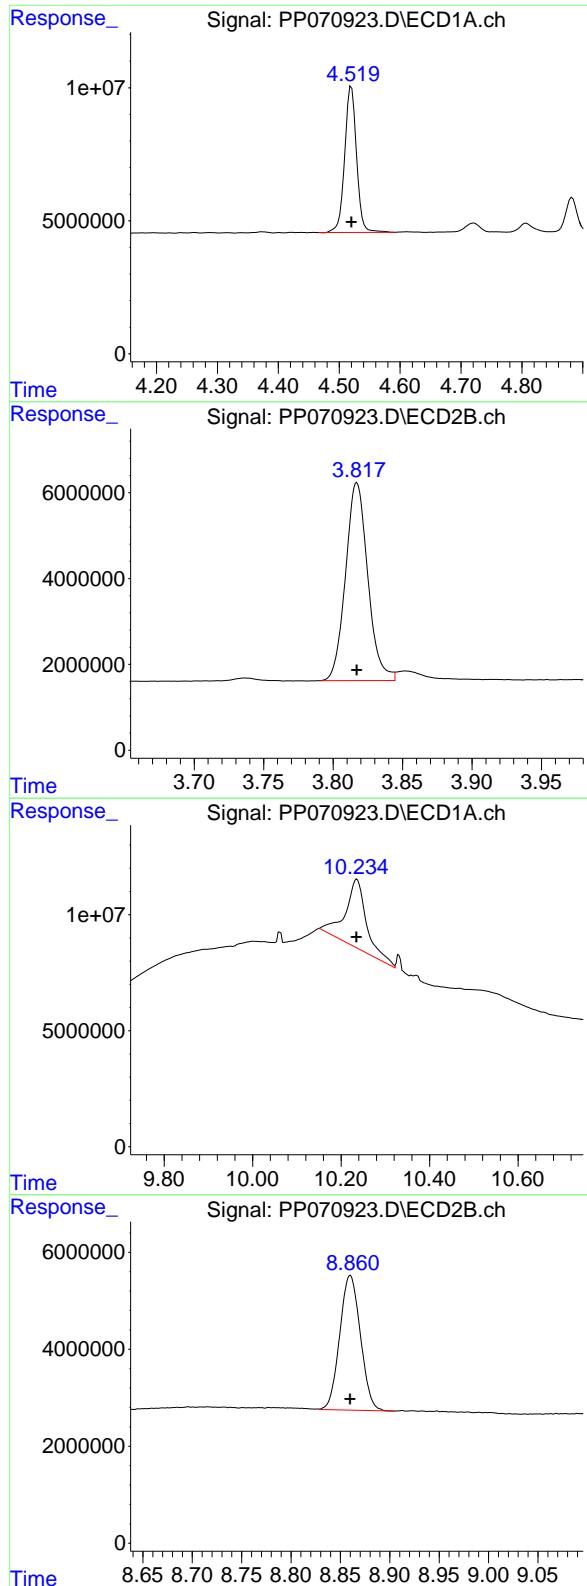

#1 Tetrachloro-m-xylene

R.T.: 4.520 min  
 Delta R.T.: 0.000 min  
 Response: 74435949  
 Conc: 50.00 ng/ml

Instrument:

ECD\_P

ClientSampleId :

AR1232ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.817 min  
 Delta R.T.: 0.000 min  
 Response: 51438566  
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.236 min  
 Delta R.T.: 0.001 min  
 Response: 99828492  
 Conc: 110.43 ng/ml

#2 Decachlorobiphenyl


R.T.: 8.860 min  
 Delta R.T.: 0.000 min  
 Response: 40517792  
 Conc: 50.00 ng/ml



#11 AR-1232-1


R.T.: 4.883 min  
 Delta R.T.: 0.000 min  
 Response: 16644355  
 Conc: 500.00 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1232ICC500

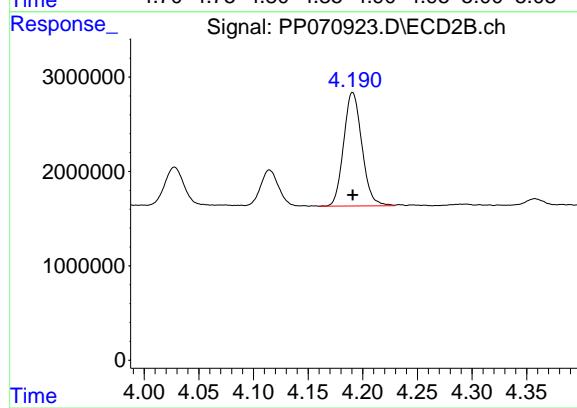


#11 AR-1232-1

R.T.: 4.191 min  
 Delta R.T.: 0.000 min  
 Response: 13993352  
 Conc: 500.00 ng/ml

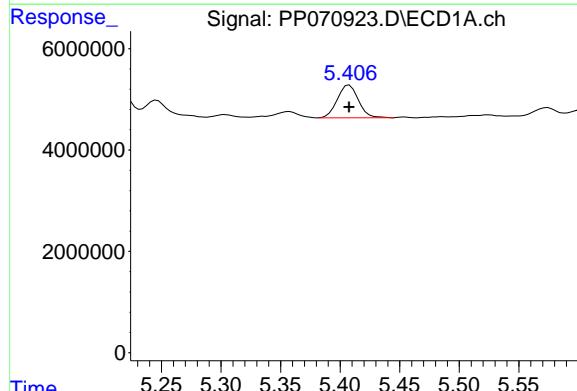


#12 AR-1232-2

R.T.: 5.408 min  
 Delta R.T.: 0.000 min  
 Response: 7955169  
 Conc: 500.00 ng/ml

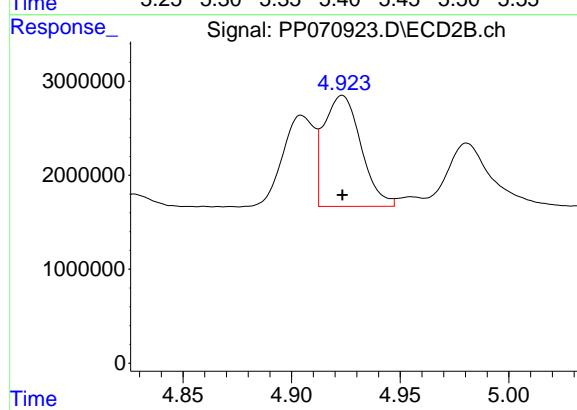

#12 AR-1232-2

R.T.: 4.923 min  
 Delta R.T.: 0.000 min  
 Response: 14030567  
 Conc: 500.00 ng/ml

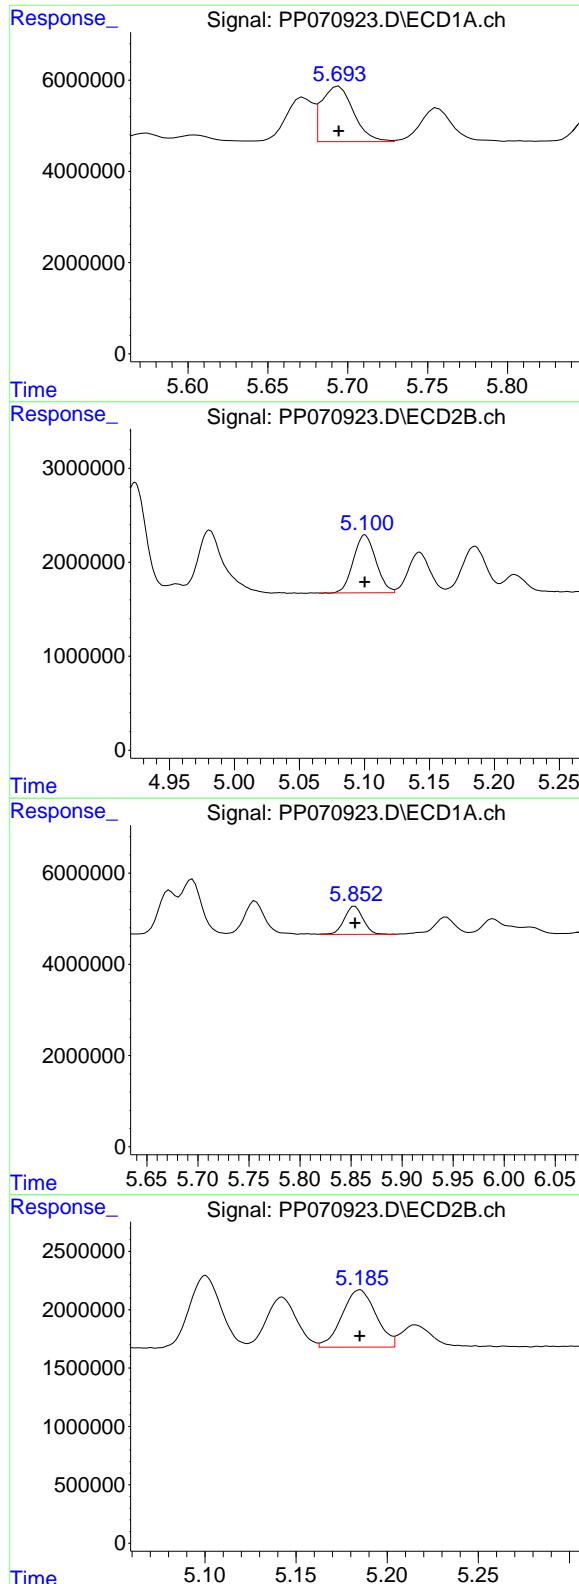

#13 AR-1232-3

R.T.: 5.694 min  
Delta R.T.: 0.000 min  
Response: 17135200  
Conc: 500.00 ng/ml

**Instrument:** ECD\_P  
**ClientSampleId:** AR1232ICC500

#13 AR-1232-3


R.T.: 5.100 min  
Delta R.T.: 0.000 min  
Response: 7444793  
Conc: 500.00 ng/ml

#14 AR-1232-4

R.T.: 5.854 min  
Delta R.T.: 0.000 min  
Response: 7853790  
Conc: 500.00 ng/ml

#14 AR-1232-4

R.T.: 5.185 min  
Delta R.T.: 0.000 min  
Response: 6402183  
Conc: 500.00 ng/ml

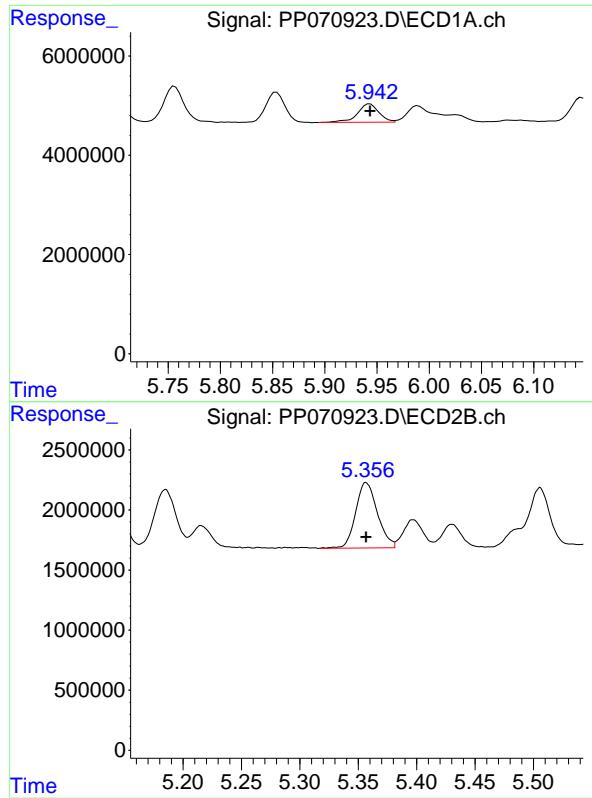

#15 AR-1232-5

R.T.: 5.943 min  
Delta R.T.: 0.000 min  
Response: 5320177  
Conc: 500.00 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1232ICC500

#15 AR-1232-5

R.T.: 5.357 min  
Delta R.T.: 0.000 min  
Response: 7087391  
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070928.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:33  
 Operator : YP\AJ  
 Sample : AR1242ICC050  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:57:16 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.512	3.815	6633492	5532966	4.273	4.939
2) SA Decachlor...	10.226	8.857	5282830	3387334	4.676	4.164

Target Compounds

16) L4 AR-1242-1	5.664	4.902	2665542	1773341	60.984	48.354
17) L4 AR-1242-2	5.687	4.921	3354217	3201456	49.372	61.016
18) L4 AR-1242-3	5.750	5.098	2977988	1401755	74.143	49.661 #
19) L4 AR-1242-4	5.844	5.181	1598185	1807177	49.578	66.685 #
20) L4 AR-1242-5	6.576	5.707	2292388	1930099	60.410	59.828



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070928.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 13:33  
 Operator : YP\AJ  
 Sample : AR1242ICC050  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1242ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 13:57:16 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 13:24:34 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

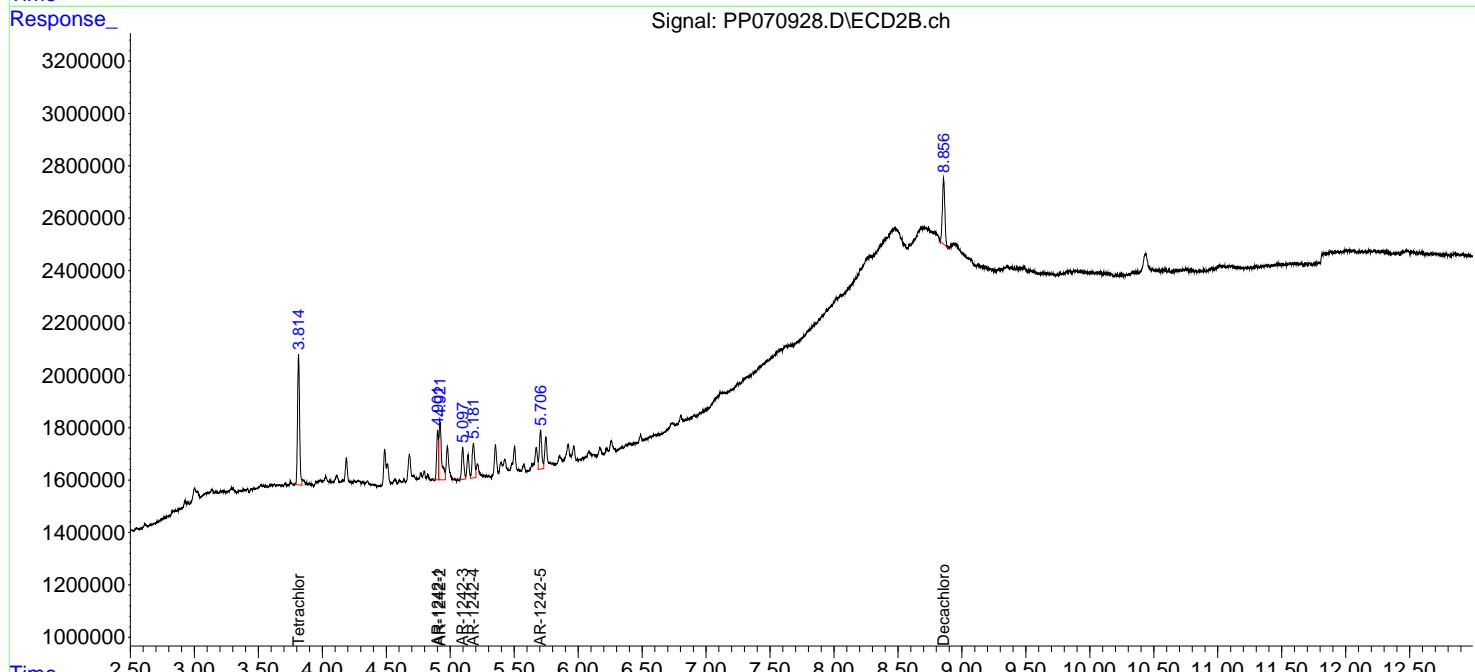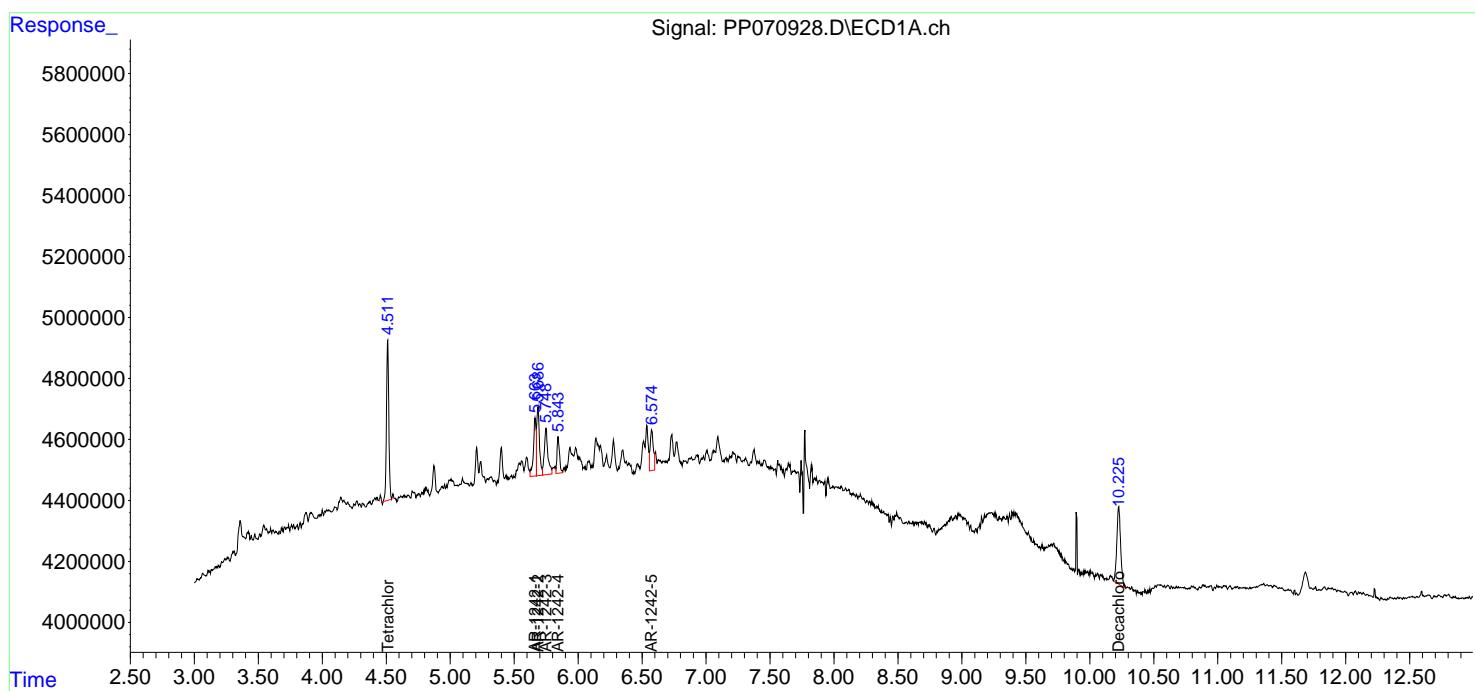

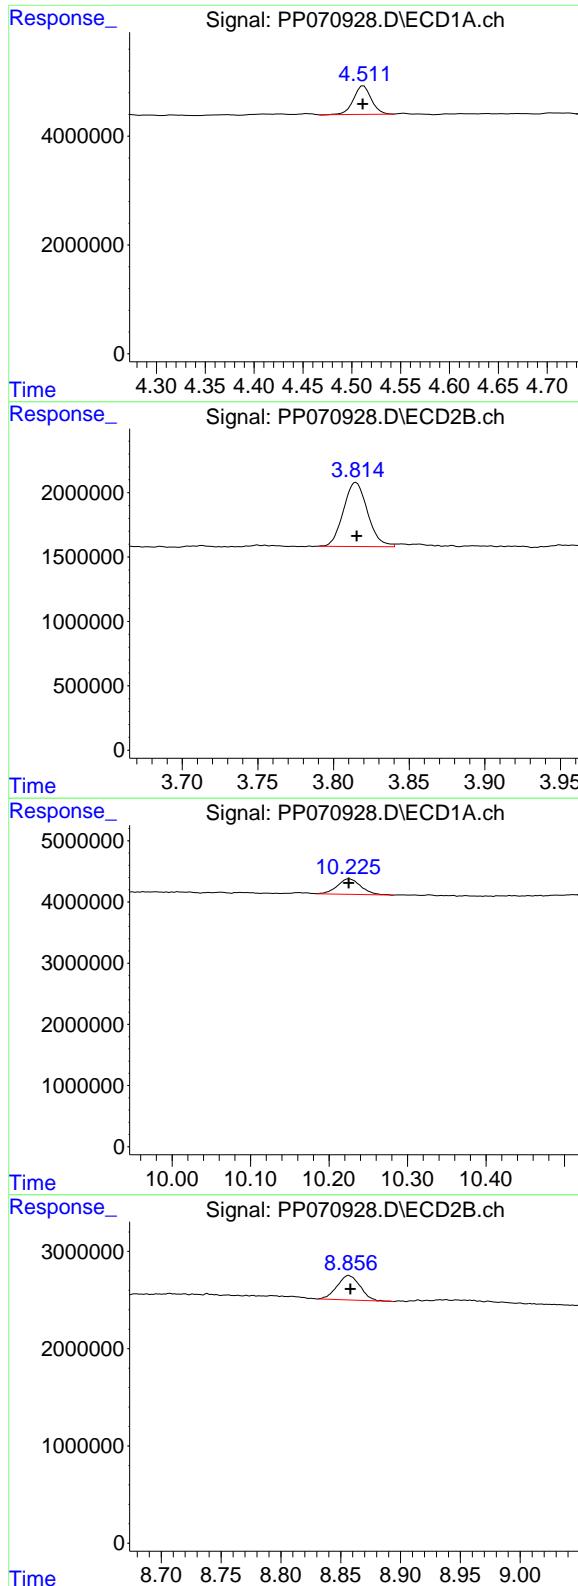

### #1 Tetrachloro-m-xylene

R.T.: 4.512 min  
 Delta R.T.: 0.001 min  
 Response: 6633492  
 Conc: 4.27 ng/ml

Instrument:

ECD\_P

ClientSampleId :

AR1242ICC050

### #1 Tetrachloro-m-xylene


R.T.: 3.815 min  
 Delta R.T.: 0.000 min  
 Response: 5532966  
 Conc: 4.94 ng/ml

### #2 Decachlorobiphenyl

R.T.: 10.226 min  
 Delta R.T.: 0.000 min  
 Response: 5282830  
 Conc: 4.68 ng/ml

### #2 Decachlorobiphenyl

R.T.: 8.857 min  
 Delta R.T.: -0.001 min  
 Response: 3387334  
 Conc: 4.16 ng/ml

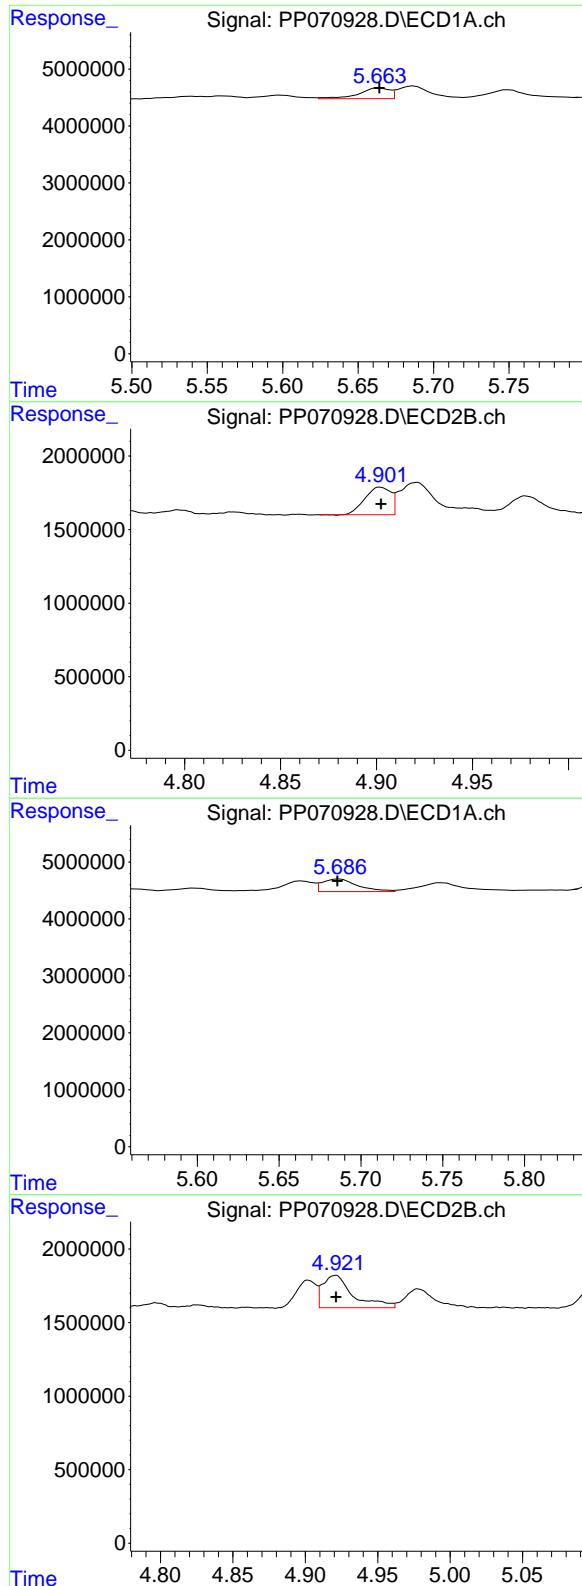

#16 AR-1242-1

R.T.: 5.664 min  
 Delta R.T.: 0.000 min  
 Response: 2665542  
 Conc: 60.98 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1242ICC050

#16 AR-1242-1


R.T.: 4.902 min  
 Delta R.T.: 0.000 min  
 Response: 1773341  
 Conc: 48.35 ng/ml

#17 AR-1242-2

R.T.: 5.687 min  
 Delta R.T.: 0.001 min  
 Response: 3354217  
 Conc: 49.37 ng/ml

#17 AR-1242-2

R.T.: 4.921 min  
 Delta R.T.: 0.000 min  
 Response: 3201456  
 Conc: 61.02 ng/ml

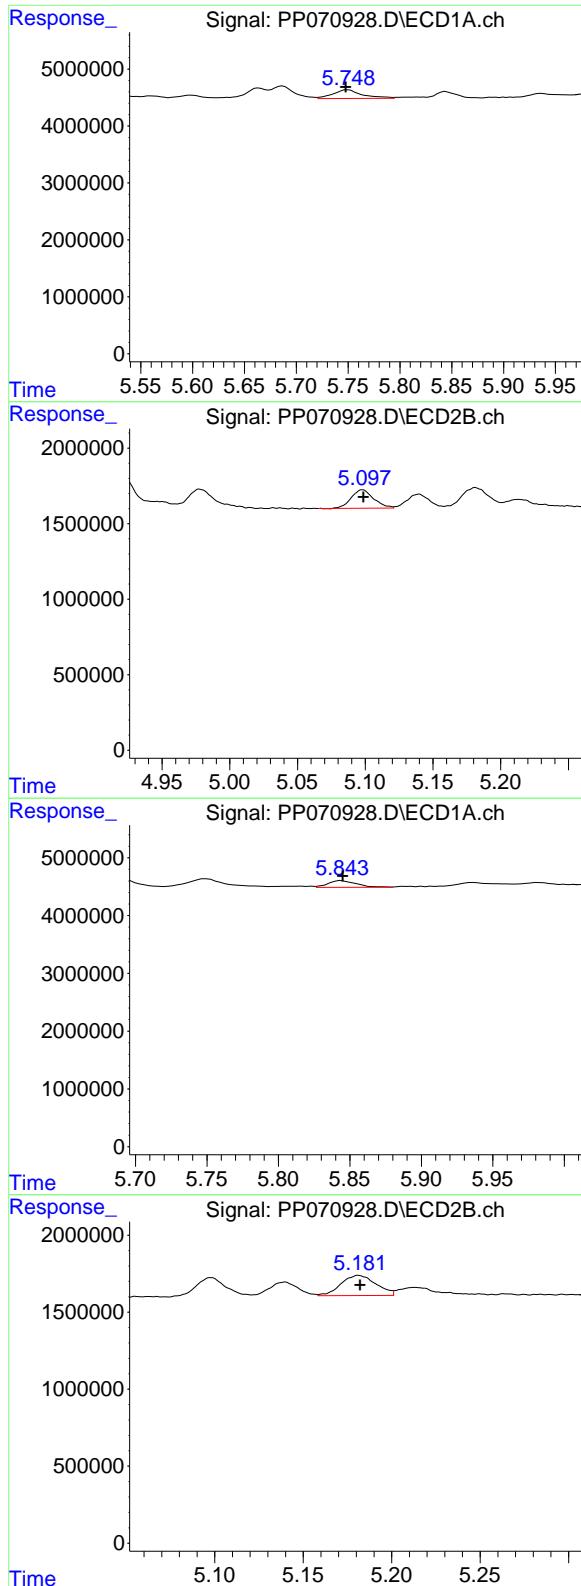

#18 AR-1242-3

R.T.: 5.750 min  
 Delta R.T.: 0.002 min  
 Response: 2977988  
 Conc: 74.14 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1242ICC050

#18 AR-1242-3


R.T.: 5.098 min  
 Delta R.T.: 0.000 min  
 Response: 1401755  
 Conc: 49.66 ng/ml

#19 AR-1242-4

R.T.: 5.844 min  
 Delta R.T.: 0.000 min  
 Response: 1598185  
 Conc: 49.58 ng/ml

#19 AR-1242-4

R.T.: 5.181 min  
 Delta R.T.: 0.000 min  
 Response: 1807177  
 Conc: 66.69 ng/ml

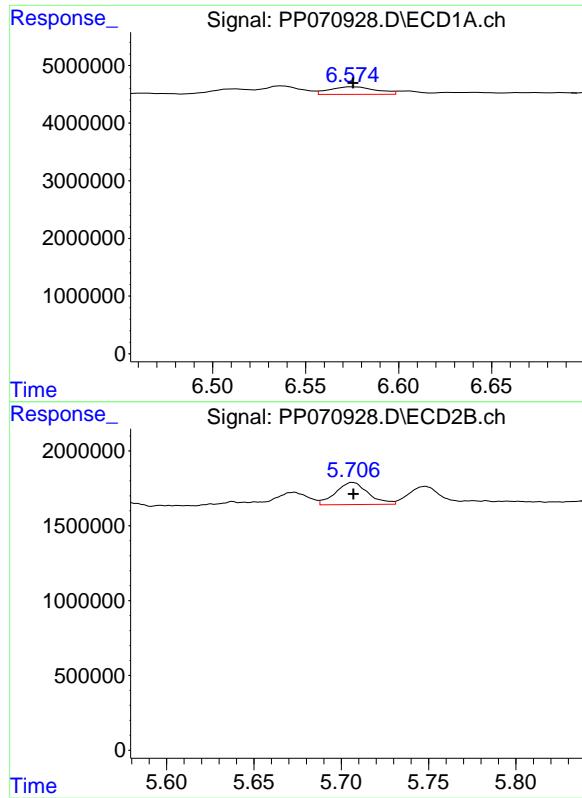

#20 AR-1242-5

R.T.: 6.576 min  
Delta R.T.: 0.000 min  
Response: 2292388  
Conc: 60.41 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1242ICC050

#20 AR-1242-5

R.T.: 5.707 min  
Delta R.T.: 0.000 min  
Response: 1930099  
Conc: 59.83 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070933.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:55  
 Operator : YP\AJ  
 Sample : AR1248ICC050  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 15:16:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 15:04:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.513	3.815	7324663	5848649	4.791	5.521
2) SA Decachlor...	10.227	8.859	5549589	3661642	4.859	4.550

Target Compounds

21) L5 AR-1248-1	5.665	4.902	1857345	1382826	51.489	51.338
22) L5 AR-1248-2	5.936	5.140	2633031	1982278	58.287	55.076
23) L5 AR-1248-3	6.139	5.182	2192198	2128069	43.549	56.472 #
24) L5 AR-1248-4	6.538	5.354	3237397	2437650	49.085	55.103
25) L5 AR-1248-5	6.578	5.748	3690931	2234402	59.064	52.978



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070933.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 14:55  
 Operator : YP\AJ  
 Sample : AR1248ICC050  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1248ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 15:16:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 15:04:54 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

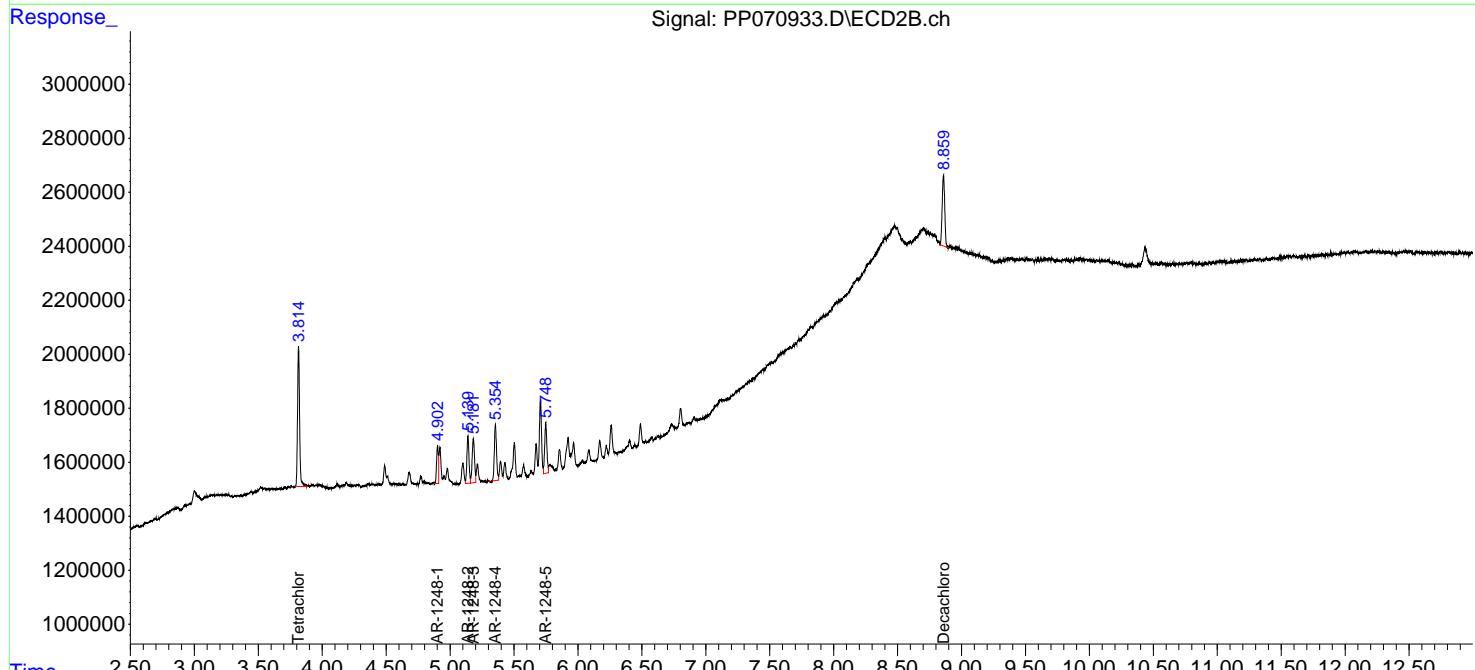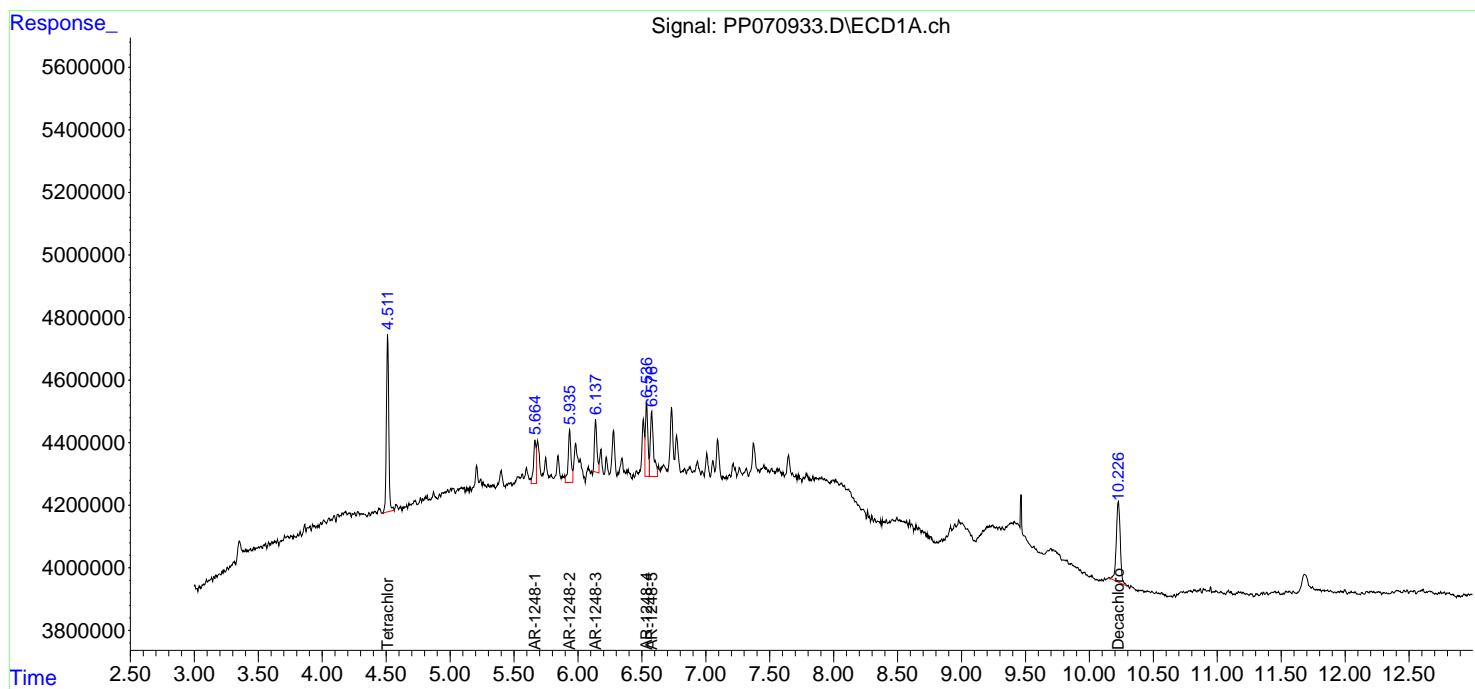

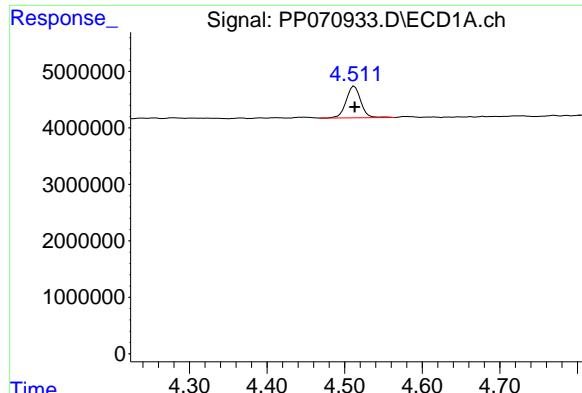


#1 Tetrachloro-m-xylene

R.T.: 4.513 min  
Delta R.T.: 0.000 min  
Response: 7324663  
Conc: 4.79 ng/ml

Instrument:


ECD\_P

ClientSampleId :  
AR1248ICC050

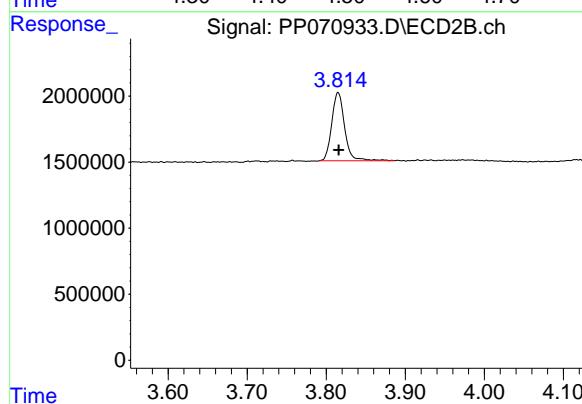


#1 Tetrachloro-m-xylene

R.T.: 3.815 min  
Delta R.T.: 0.000 min  
Response: 5848649  
Conc: 5.52 ng/ml

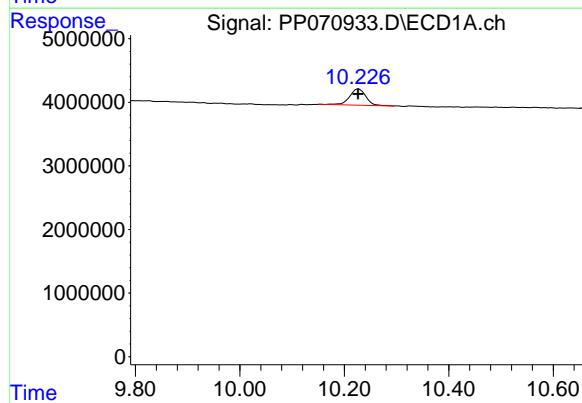


#2 Decachlorobiphenyl

R.T.: 10.227 min  
Delta R.T.: 0.000 min  
Response: 5549589  
Conc: 4.86 ng/ml

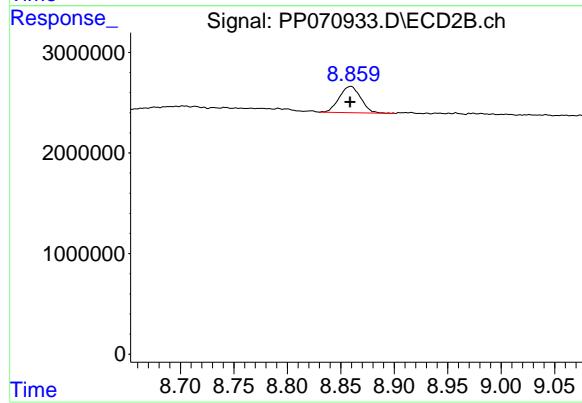

#2 Decachlorobiphenyl


R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 3661642  
Conc: 4.55 ng/ml

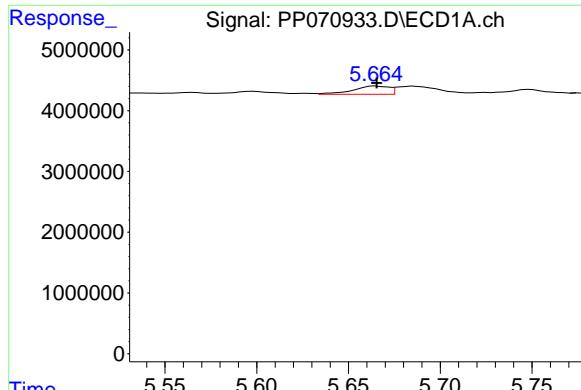

#21 AR-1248-1


R.T.: 5.665 min  
Delta R.T.: 0.000 min  
Response: 1857345  
Conc: 51.49 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1248ICC050

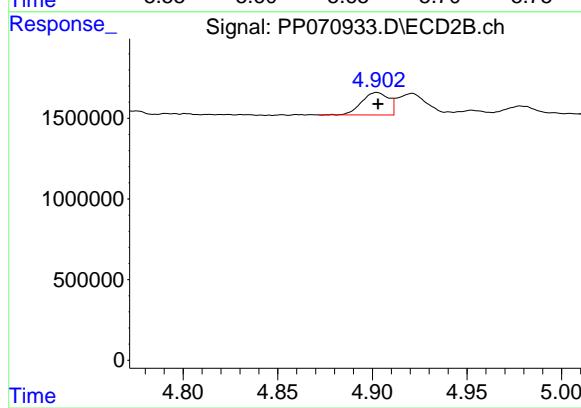


#21 AR-1248-1

R.T.: 4.902 min  
Delta R.T.: 0.000 min  
Response: 1382826  
Conc: 51.34 ng/ml

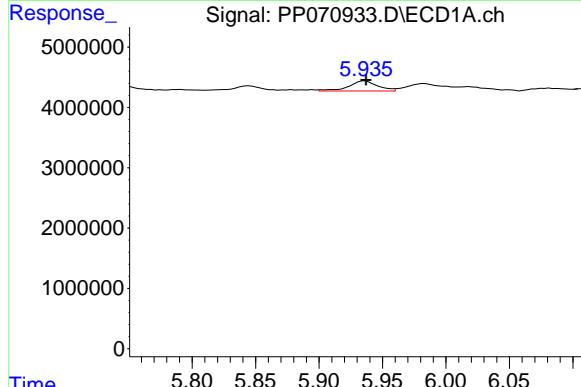


#22 AR-1248-2

R.T.: 5.936 min  
Delta R.T.: 0.000 min  
Response: 2633031  
Conc: 58.29 ng/ml

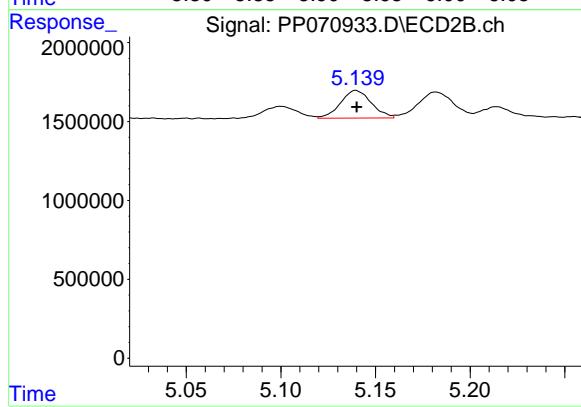

#22 AR-1248-2

R.T.: 5.140 min  
Delta R.T.: 0.000 min  
Response: 1982278  
Conc: 55.08 ng/ml

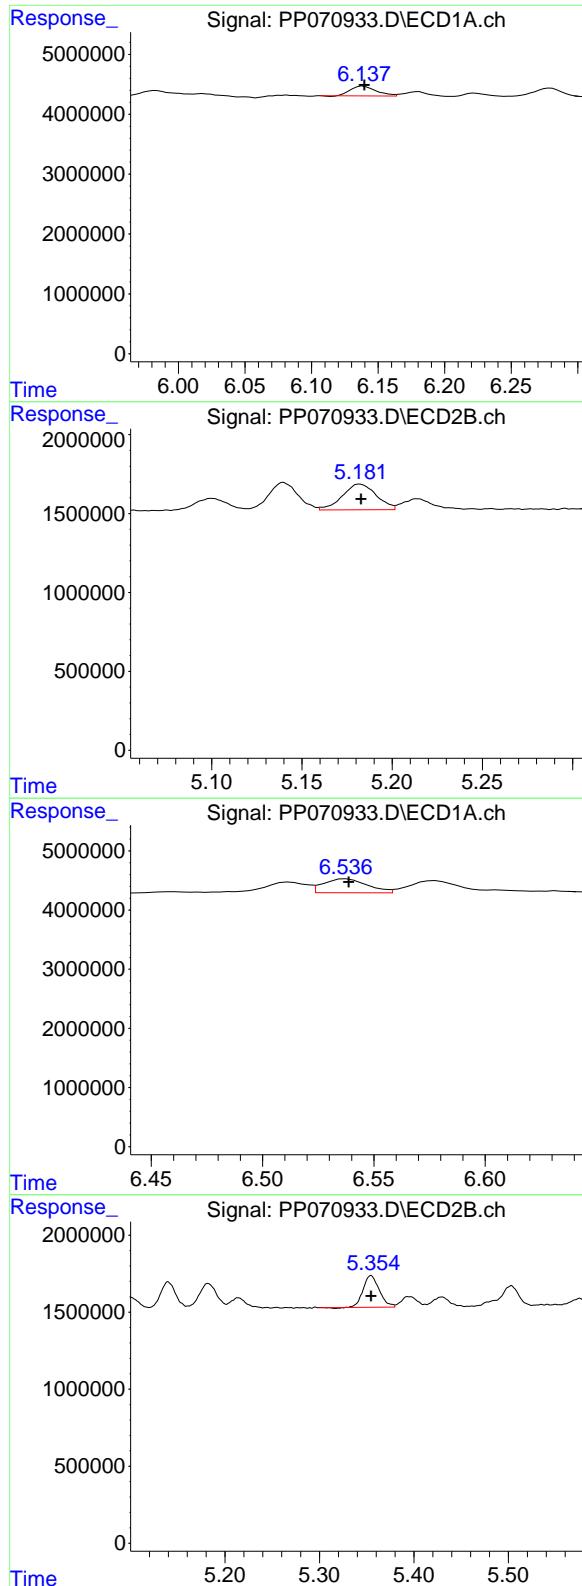

#23 AR-1248-3

R.T.: 6.139 min  
 Delta R.T.: 0.000 min  
 Response: 2192198  
 Conc: 43.55 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1248ICC050

#23 AR-1248-3


R.T.: 5.182 min  
 Delta R.T.: 0.000 min  
 Response: 2128069  
 Conc: 56.47 ng/ml

#24 AR-1248-4

R.T.: 6.538 min  
 Delta R.T.: -0.001 min  
 Response: 3237397  
 Conc: 49.09 ng/ml

#24 AR-1248-4


R.T.: 5.354 min  
 Delta R.T.: 0.000 min  
 Response: 2437650  
 Conc: 55.10 ng/ml

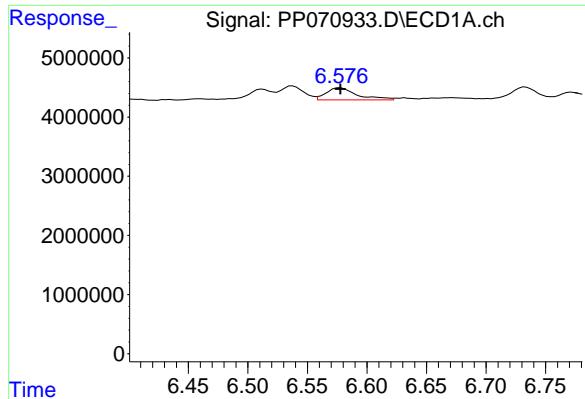

#25 AR-1248-5

R.T.: 6.578 min  
Delta R.T.: 0.000 min  
Response: 3690931  
Conc: 59.06 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1248ICC050

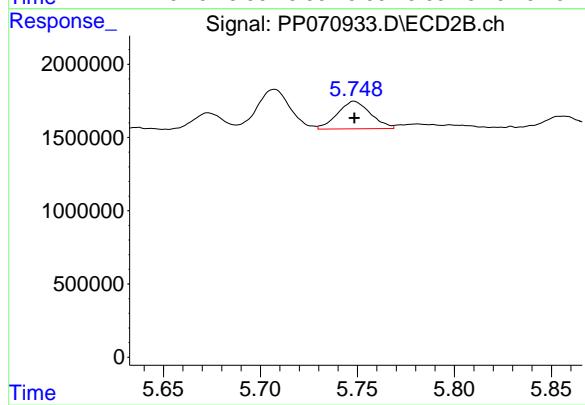

#25 AR-1248-5

R.T.: 5.748 min  
Delta R.T.: 0.000 min  
Response: 2234402  
Conc: 52.98 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070934.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:11  
 Operator : YP\AJ  
 Sample : AR1254ICC1000  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.514	3.816	150.1E6	104.3E6	95.275	94.048
2) SA Decachlor...	10.231	8.860	109.5E6	78348381	93.754	86.018

Target Compounds

26) L6 AR-1254-1	6.516	5.709	60157506	58928147	918.830	891.736
27) L6 AR-1254-2	6.732	5.857	92838442	50145967	911.948	882.952
28) L6 AR-1254-3	7.095	6.261	92334650	77448562	928.765	882.456
29) L6 AR-1254-4	7.379	6.490	84238161	49998215	970.458	893.353
30) L6 AR-1254-5	7.793	6.908	87302185	65979008	1079.742	918.596



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070934.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:11  
 Operator : YP\AJ  
 Sample : AR1254ICC1000  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

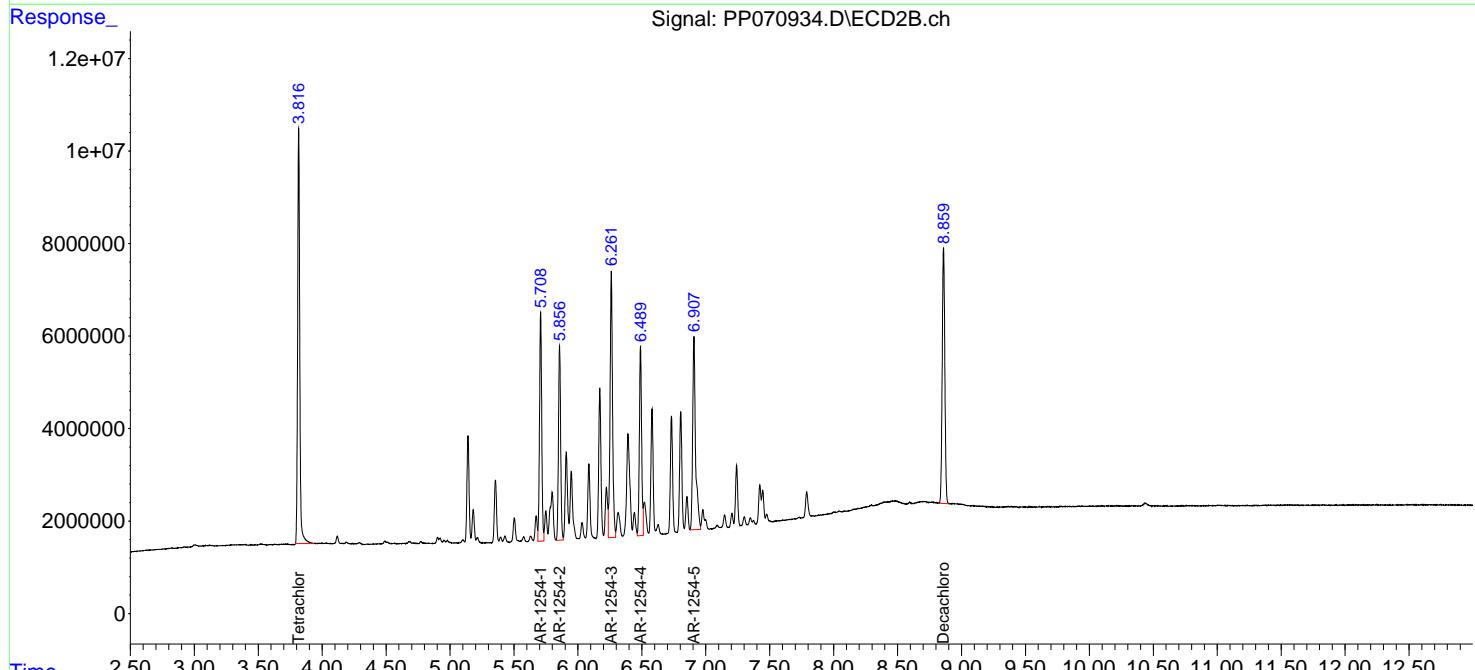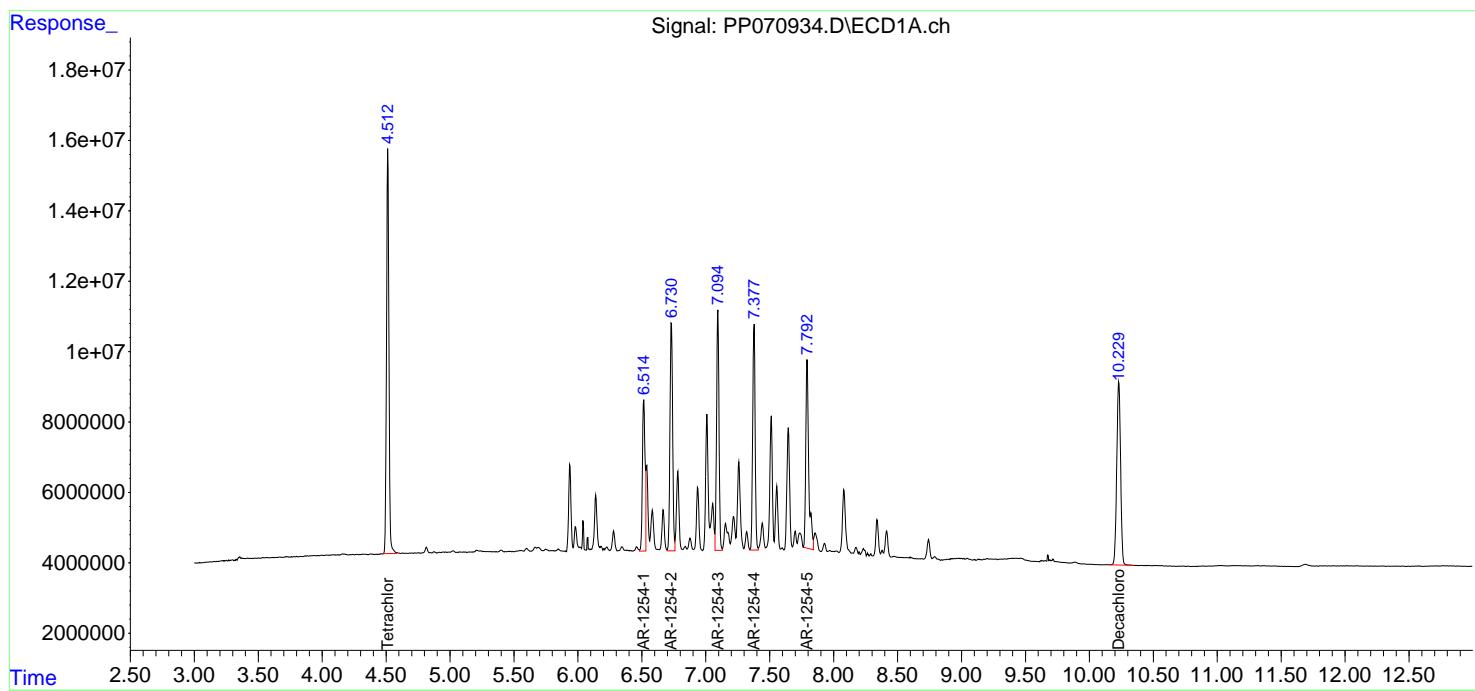

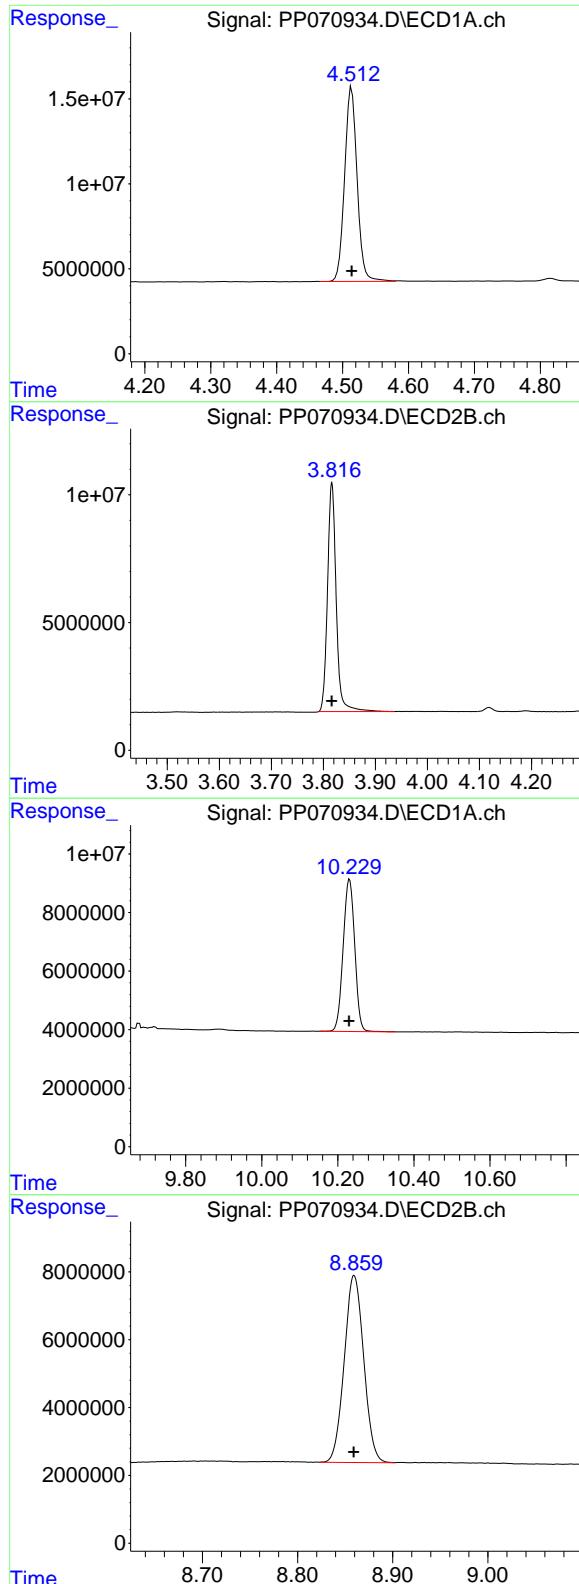

### #1 Tetrachloro-m-xylene

R.T.: 4.514 min  
 Delta R.T.: 0.000 min  
 Response: 150128836  
 Conc: 95.27 ng/ml

**Instrument:** ECD\_P  
**ClientSampleId:** AR1254ICC1000

### #1 Tetrachloro-m-xylene


R.T.: 3.816 min  
 Delta R.T.: 0.000 min  
 Response: 104259560  
 Conc: 94.05 ng/ml

### #2 Decachlorobiphenyl

R.T.: 10.231 min  
 Delta R.T.: 0.001 min  
 Response: 109543241  
 Conc: 93.75 ng/ml

### #2 Decachlorobiphenyl

R.T.: 8.860 min  
 Delta R.T.: 0.000 min  
 Response: 78348381  
 Conc: 86.02 ng/ml

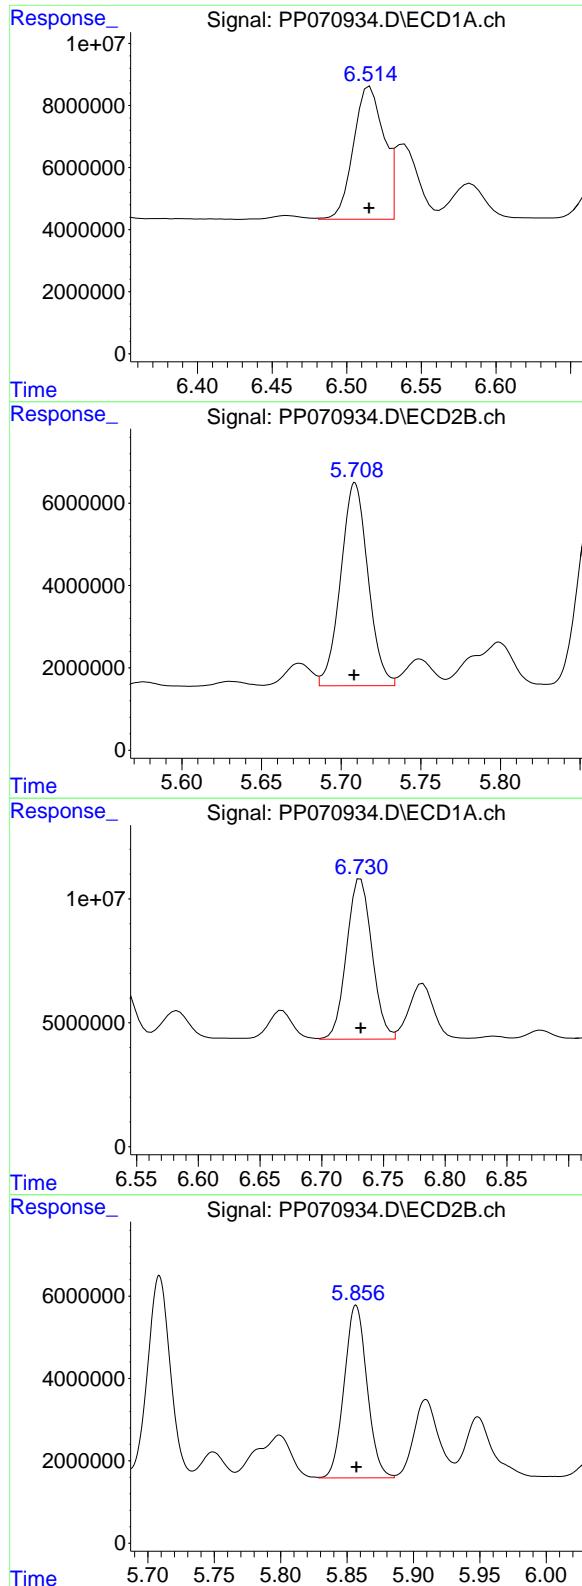

#26 AR-1254-1

R.T.: 6.516 min  
Delta R.T.: 0.000 min  
Response: 60157506  
Conc: 918.83 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1254ICC1000

#26 AR-1254-1


R.T.: 5.709 min  
Delta R.T.: 0.000 min  
Response: 58928147  
Conc: 891.74 ng/ml

#27 AR-1254-2

R.T.: 6.732 min  
Delta R.T.: 0.000 min  
Response: 92838442  
Conc: 911.95 ng/ml

#27 AR-1254-2

R.T.: 5.857 min  
Delta R.T.: 0.000 min  
Response: 50145967  
Conc: 882.95 ng/ml

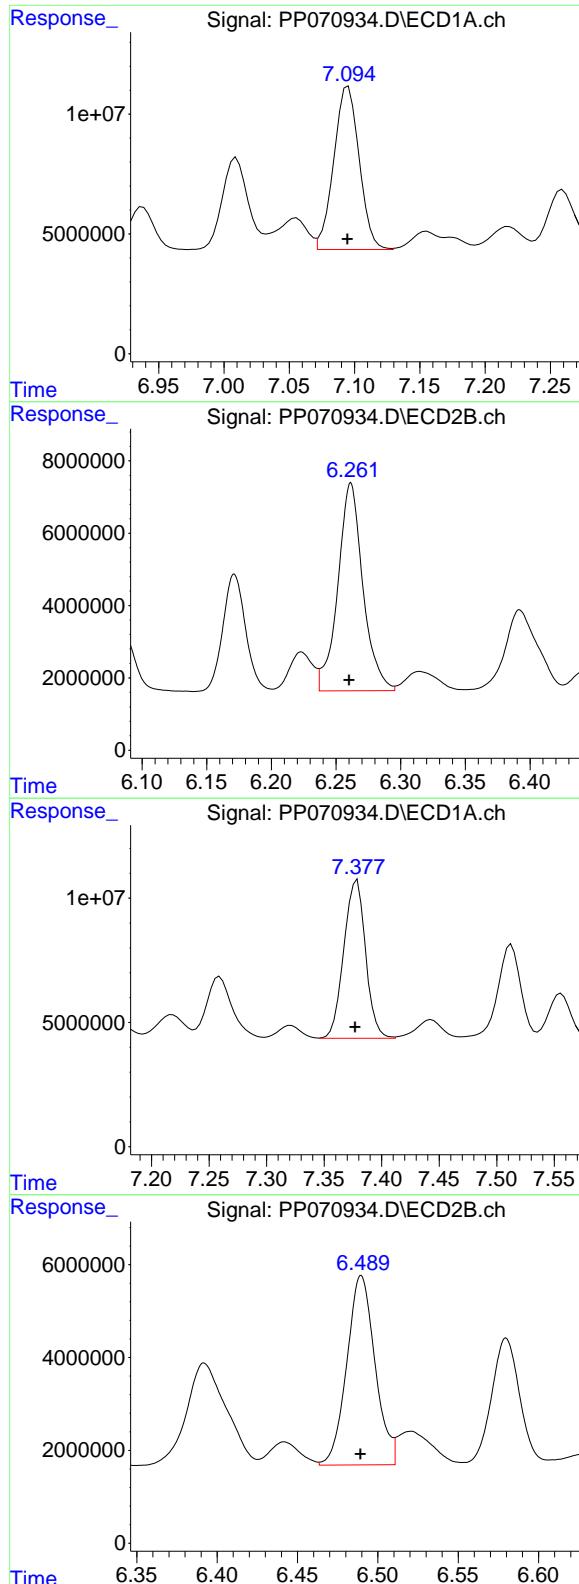

#28 AR-1254-3

R.T.: 7.095 min  
 Delta R.T.: 0.000 min  
 Response: 92334650  
 Conc: 928.77 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1254ICC1000

#28 AR-1254-3


R.T.: 6.261 min  
 Delta R.T.: 0.001 min  
 Response: 77448562  
 Conc: 882.46 ng/ml

#29 AR-1254-4

R.T.: 7.379 min  
 Delta R.T.: 0.002 min  
 Response: 84238161  
 Conc: 970.46 ng/ml

#29 AR-1254-4

R.T.: 6.490 min  
 Delta R.T.: 0.000 min  
 Response: 49998215  
 Conc: 893.35 ng/ml

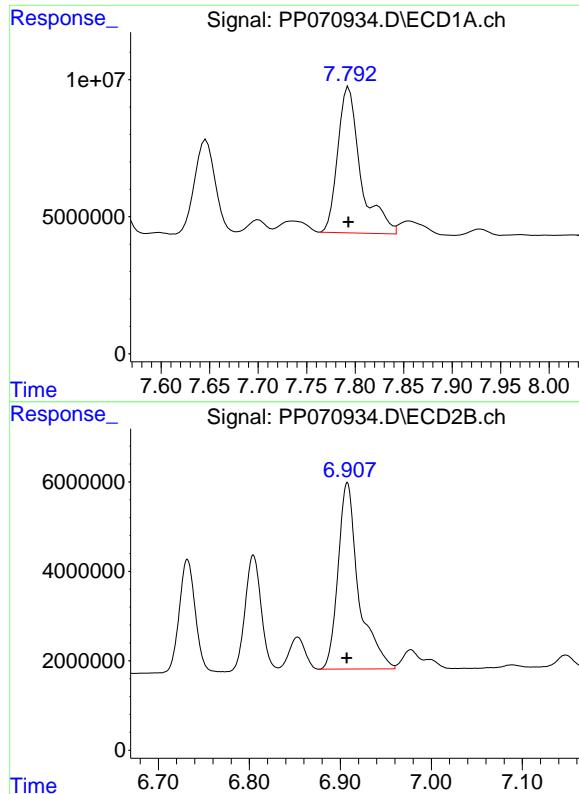

#30 AR-1254-5

R.T.: 7.793 min  
Delta R.T.: 0.000 min  
Response: 87302185  
Conc: 1079.74 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1254ICC1000

#30 AR-1254-5

R.T.: 6.908 min  
Delta R.T.: 0.000 min  
Response: 65979008  
Conc: 918.60 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070935.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:27  
 Operator : YP\AJ  
 Sample : AR1254ICC750  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.514	3.816	116.3E6	81865229	73.835	73.847
2) SA Decachlor...	10.228	8.859	85851924	59713645	73.477	65.559

Target Compounds

26) L6 AR-1254-1	6.515	5.708	47300573	46349687	722.456	701.391
27) L6 AR-1254-2	6.731	5.856	72785411	40339655	714.968	710.286
28) L6 AR-1254-3	7.094	6.260	73541603	62731680	739.732	714.771
29) L6 AR-1254-4	7.377	6.490	65835410	40961211	758.451	731.883
30) L6 AR-1254-5	7.793	6.907	68599534	53519032	848.430	745.122



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070935.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 15:27  
 Operator : YP\AJ  
 Sample : AR1254ICC750  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:19:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

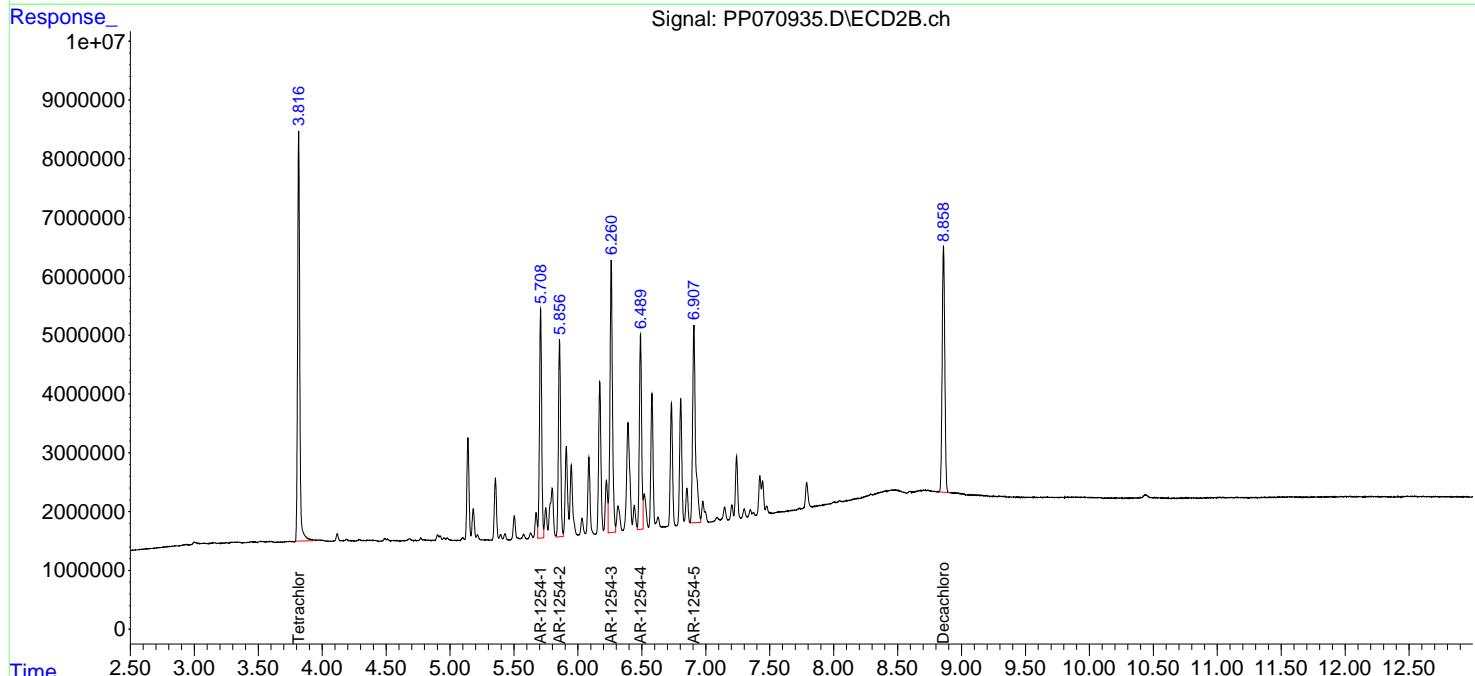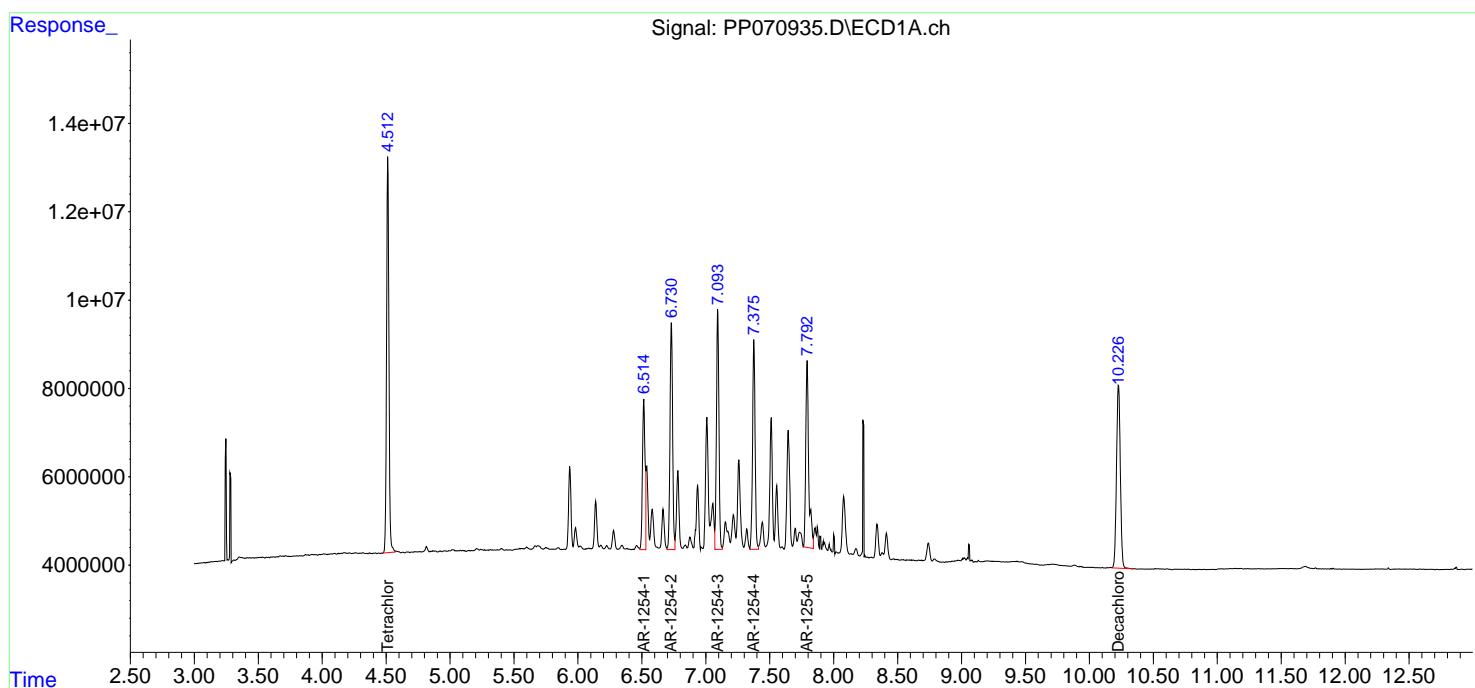

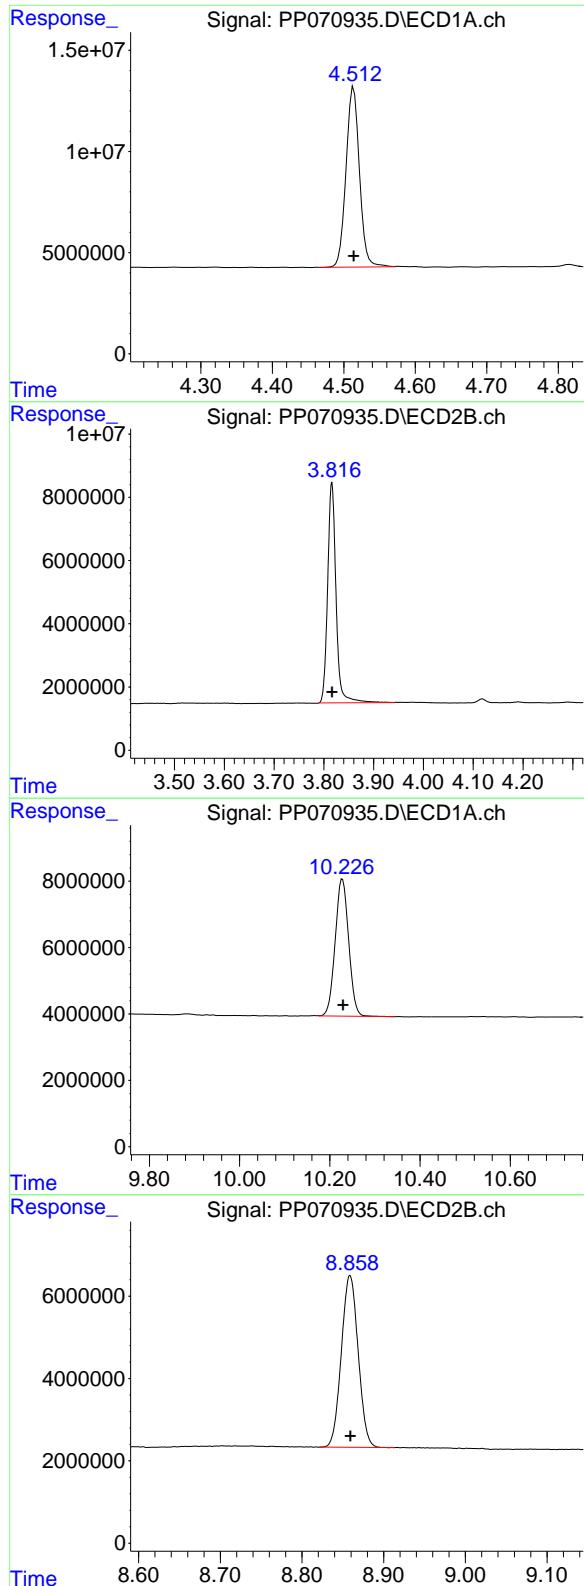

#1 Tetrachloro-m-xylene

R.T.: 4.514 min  
Delta R.T.: 0.000 min  
Response: 116345667  
Conc: 73.84 ng/ml

Instrument:

ECD\_P

ClientSampleId :

AR1254ICC750

#1 Tetrachloro-m-xylene


R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 81865229  
Conc: 73.85 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.228 min  
Delta R.T.: -0.002 min  
Response: 85851924  
Conc: 73.48 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 59713645  
Conc: 65.56 ng/ml

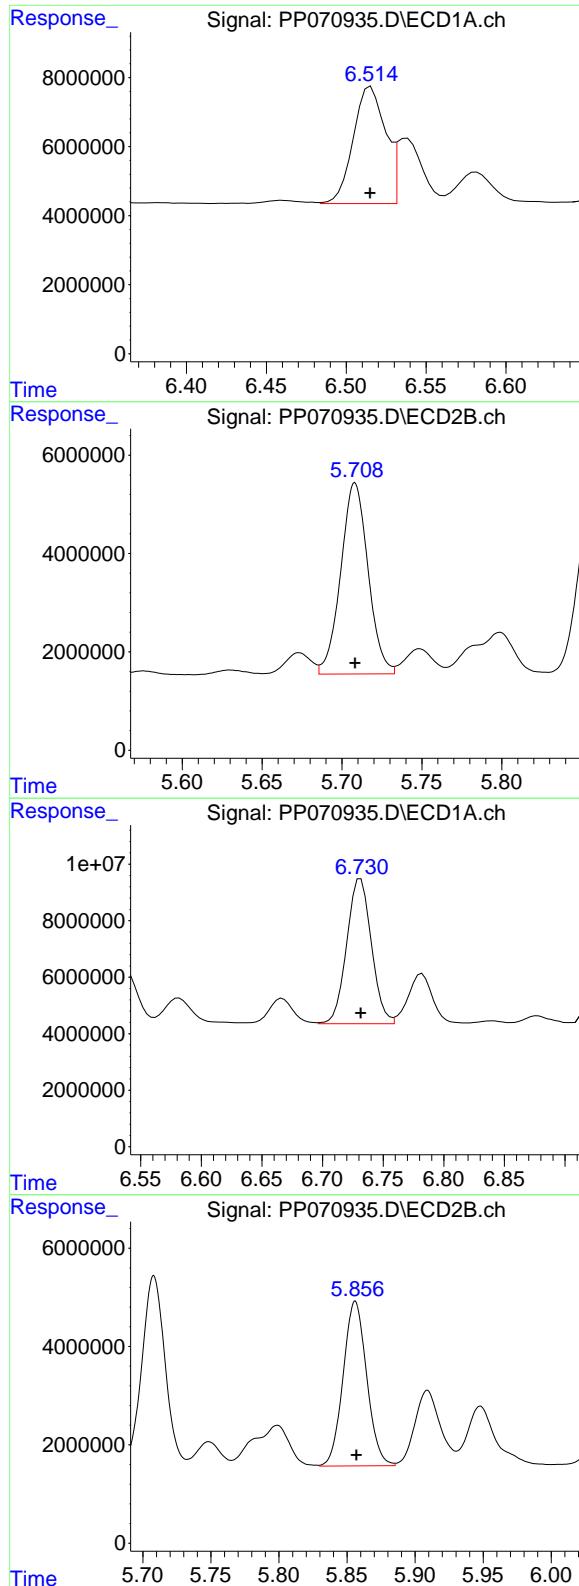

#26 AR-1254-1

R.T.: 6.515 min  
 Delta R.T.: 0.000 min  
 Response: 47300573  
 Conc: 722.46 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1254ICC750

#26 AR-1254-1


R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 46349687  
 Conc: 701.39 ng/ml

#27 AR-1254-2

R.T.: 6.731 min  
 Delta R.T.: 0.000 min  
 Response: 72785411  
 Conc: 714.97 ng/ml

#27 AR-1254-2

R.T.: 5.856 min  
 Delta R.T.: 0.000 min  
 Response: 40339655  
 Conc: 710.29 ng/ml

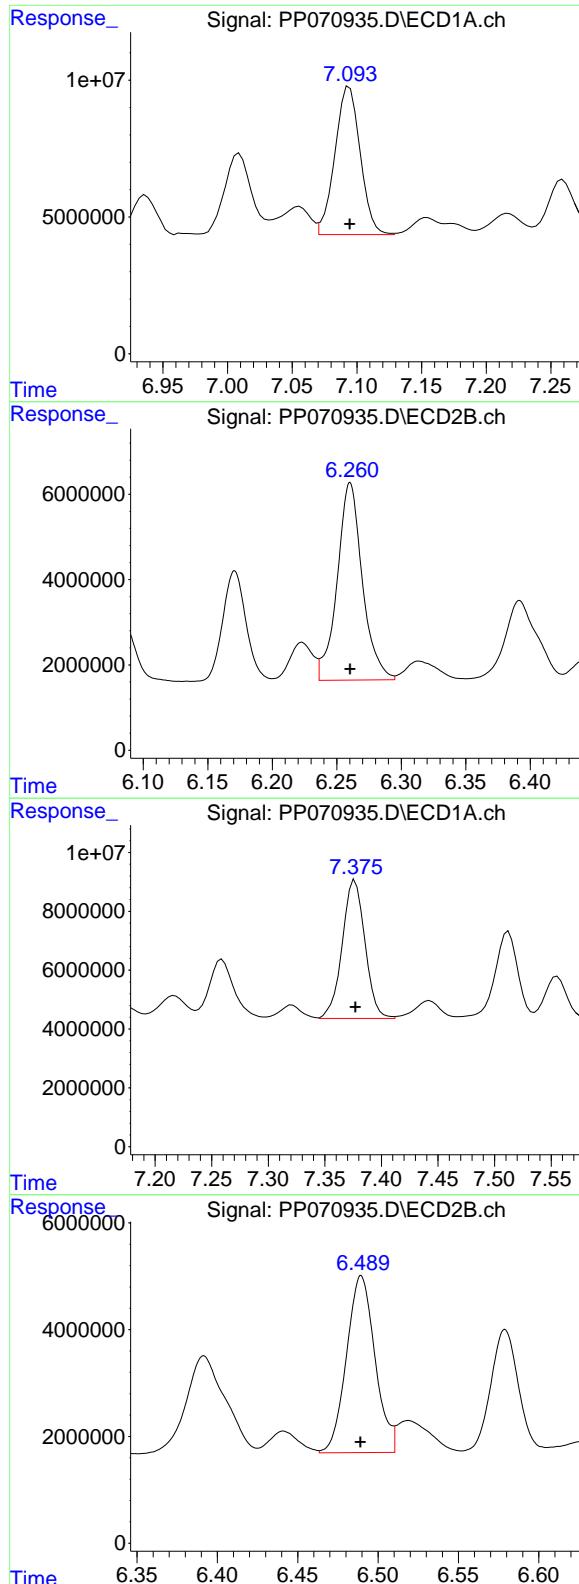

#28 AR-1254-3

R.T.: 7.094 min  
 Delta R.T.: 0.000 min  
 Response: 73541603  
 Conc: 739.73 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1254ICC750

#28 AR-1254-3


R.T.: 6.260 min  
 Delta R.T.: 0.000 min  
 Response: 62731680  
 Conc: 714.77 ng/ml

#29 AR-1254-4

R.T.: 7.377 min  
 Delta R.T.: 0.000 min  
 Response: 65835410  
 Conc: 758.45 ng/ml

#29 AR-1254-4

R.T.: 6.490 min  
 Delta R.T.: 0.000 min  
 Response: 40961211  
 Conc: 731.88 ng/ml

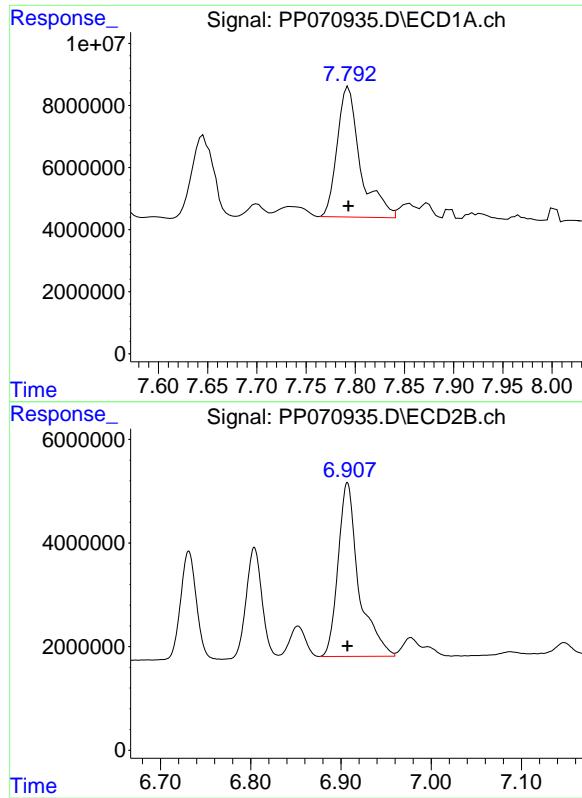

#30 AR-1254-5

R.T.: 7.793 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 68599534 ECD\_P  
 Conc: 848.43 ng/ml **ClientSampleId:**  
 AR1254ICC750

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070937.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:00  
 Operator : YP\AJ  
 Sample : AR1254ICC250  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:20:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.514	3.816	40672603	29879101	25.812	26.953
2) SA Decachlor...	10.230	8.859	29858259	21257096	25.554	23.338

Target Compounds

26) L6 AR-1254-1	6.516	5.708	16701604	18446961	255.096	279.151
27) L6 AR-1254-2	6.732	5.856	26389026	16008677	259.218	281.875
28) L6 AR-1254-3	7.095	6.260	25960285	24772594	261.126	282.261
29) L6 AR-1254-4	7.377	6.489	22197209	16043587	255.721	286.662
30) L6 AR-1254-5	7.793	6.907	23415043	20606411	289.594	286.894



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070937.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:00  
 Operator : YP\AJ  
 Sample : AR1254ICC250  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1254ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 16:20:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 16:07:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

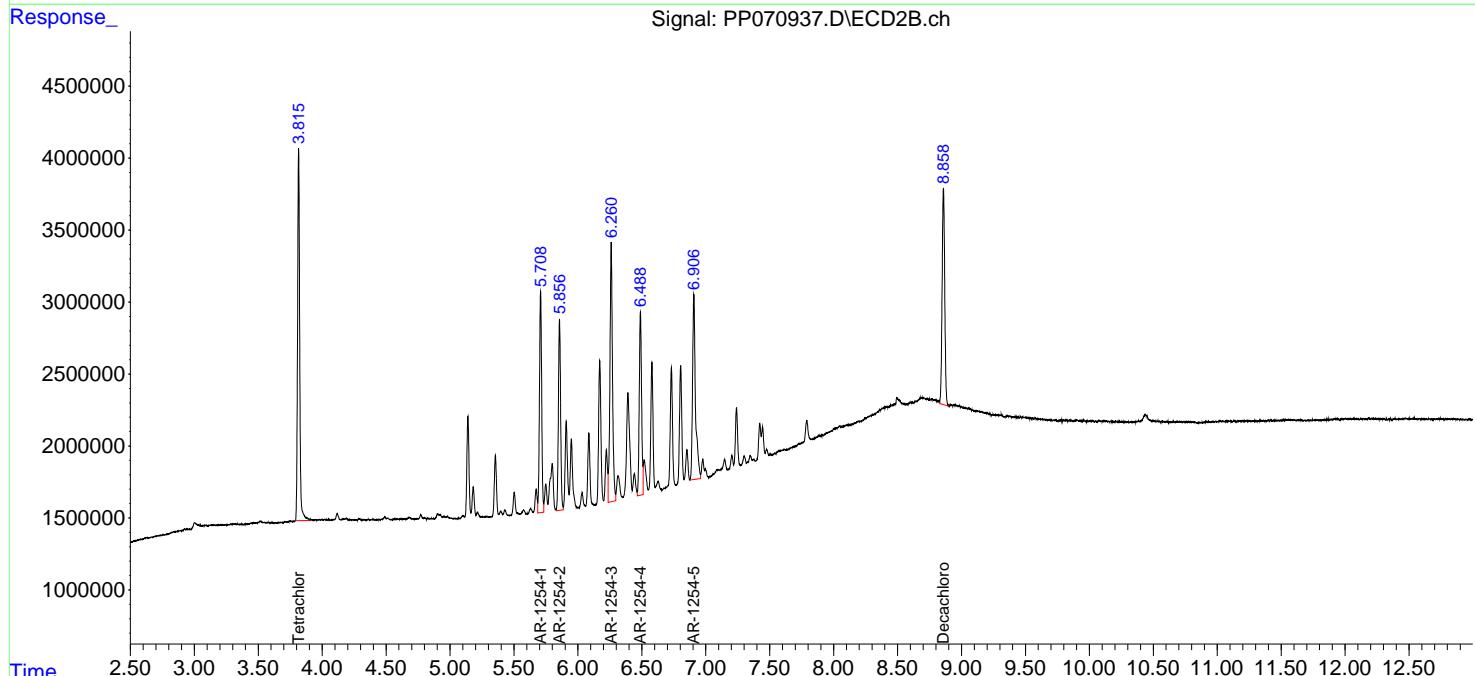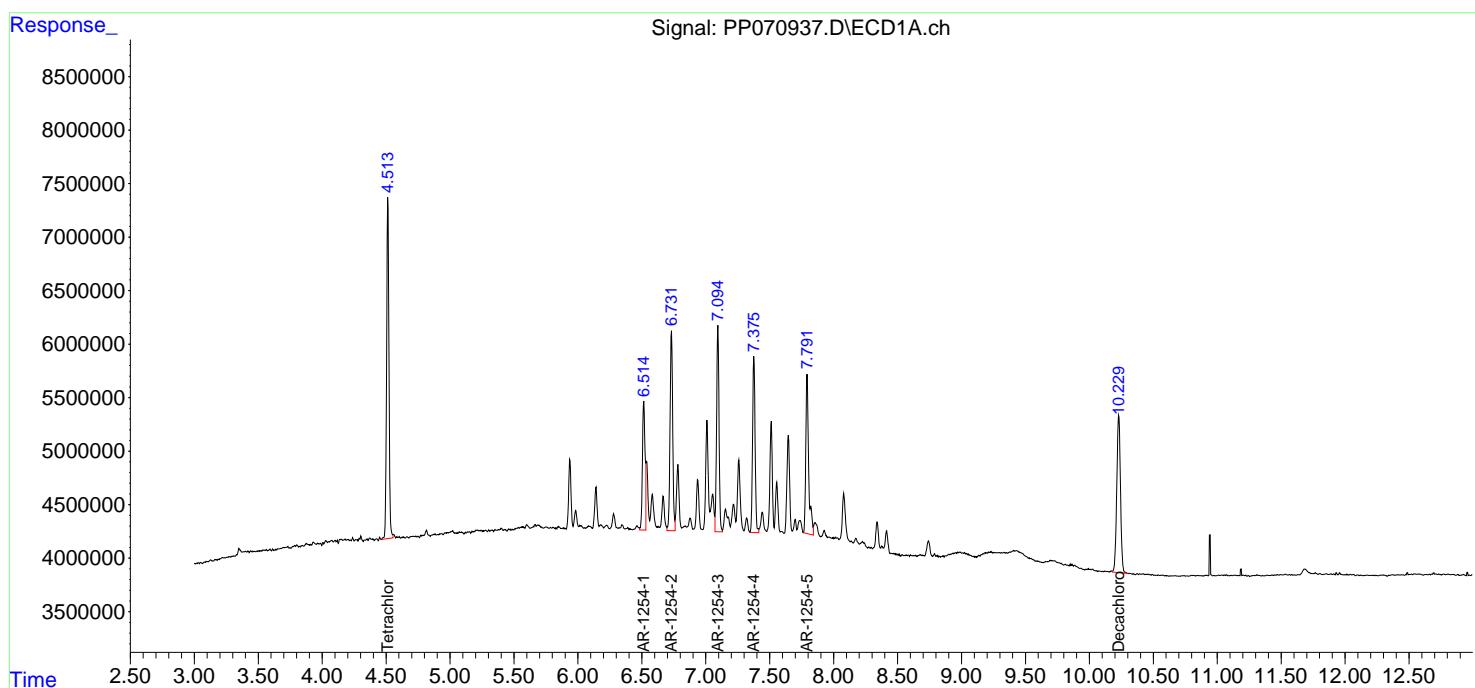

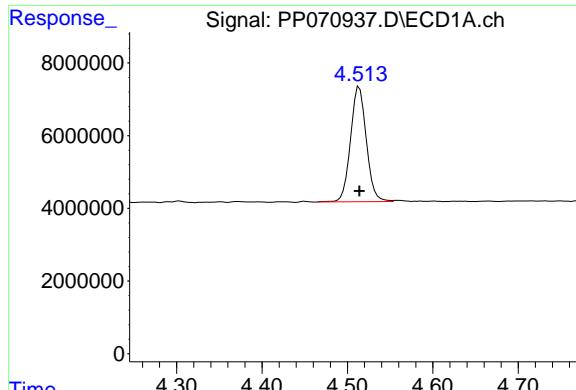

#1 Tetrachloro-m-xylene


R.T.: 4.514 min  
Delta R.T.: 0.000 min  
Response: 40672603  
Conc: 25.81 ng/ml

Instrument:

ECD\_P


ClientSampleId :

AR1254ICC250

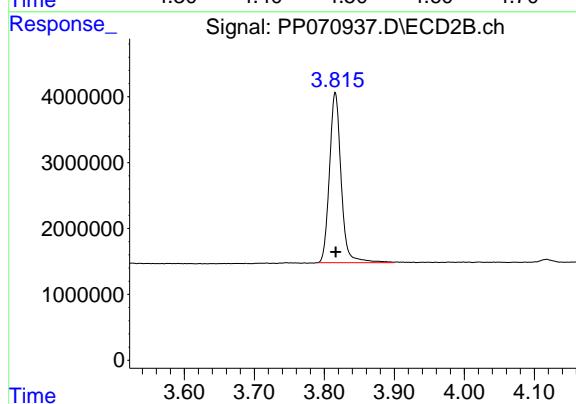


#1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 29879101  
Conc: 26.95 ng/ml

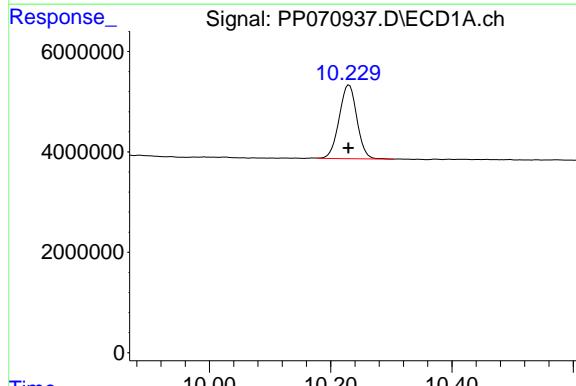


#2 Decachlorobiphenyl

R.T.: 10.230 min  
Delta R.T.: 0.000 min  
Response: 29858259  
Conc: 25.55 ng/ml

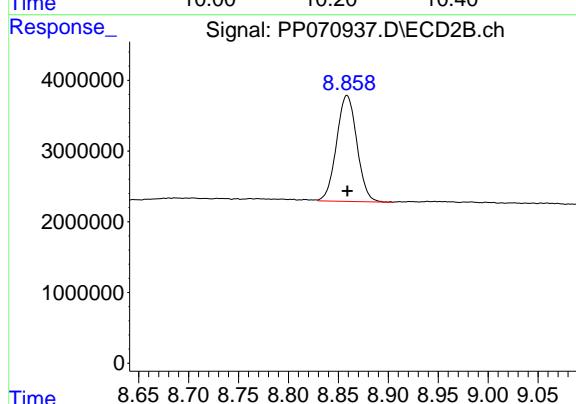

#2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 21257096  
Conc: 23.34 ng/ml

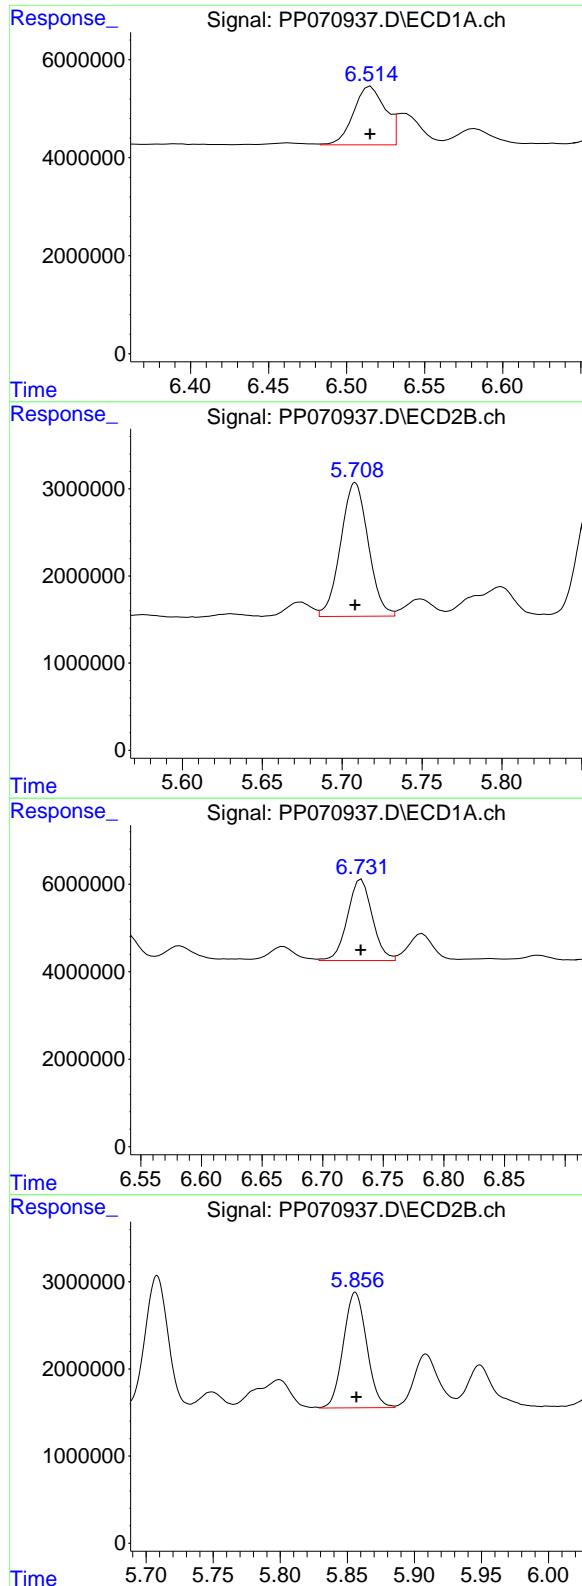

#26 AR-1254-1

R.T.: 6.516 min  
 Delta R.T.: 0.000 min  
 Response: 16701604  
 Conc: 255.10 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1254ICC250

#26 AR-1254-1


R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 18446961  
 Conc: 279.15 ng/ml

#27 AR-1254-2

R.T.: 6.732 min  
 Delta R.T.: 0.000 min  
 Response: 26389026  
 Conc: 259.22 ng/ml

#27 AR-1254-2

R.T.: 5.856 min  
 Delta R.T.: 0.000 min  
 Response: 16008677  
 Conc: 281.87 ng/ml

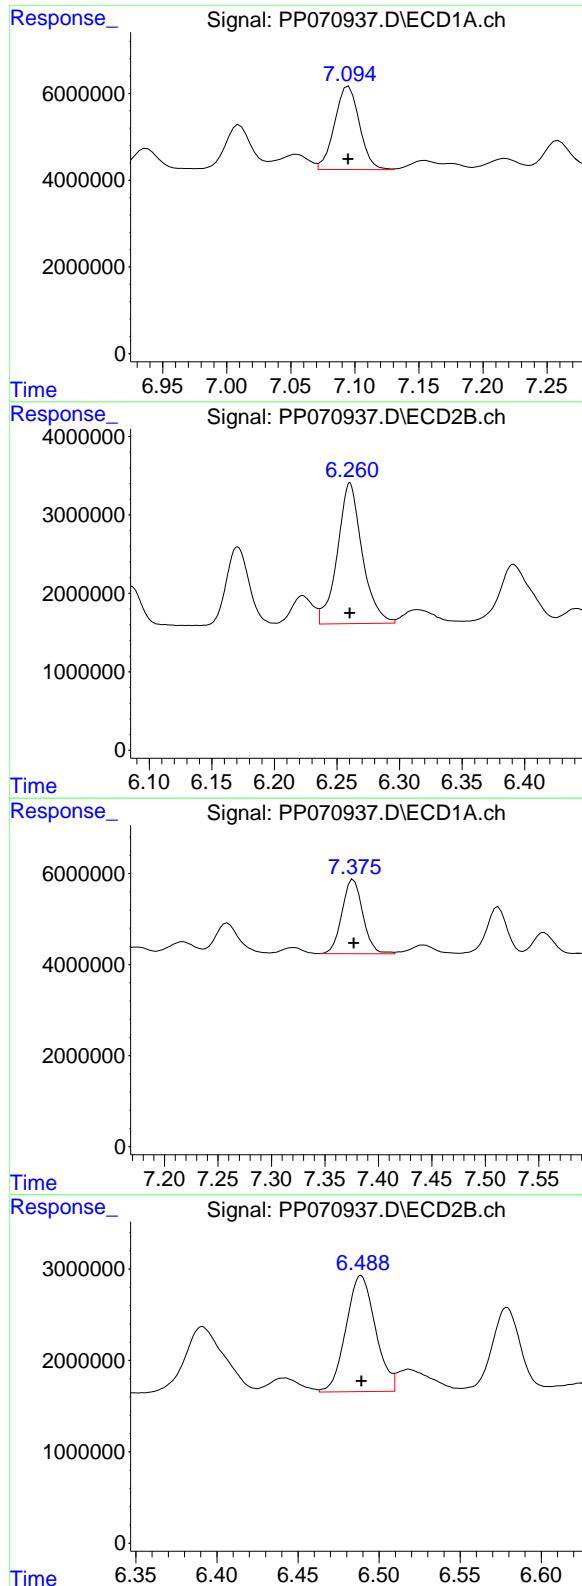

#28 AR-1254-3

R.T.: 7.095 min  
 Delta R.T.: 0.000 min  
 Response: 25960285  
 Conc: 261.13 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1254ICC250

#28 AR-1254-3


R.T.: 6.260 min  
 Delta R.T.: 0.000 min  
 Response: 24772594  
 Conc: 282.26 ng/ml

#29 AR-1254-4

R.T.: 7.377 min  
 Delta R.T.: 0.000 min  
 Response: 22197209  
 Conc: 255.72 ng/ml

#29 AR-1254-4


R.T.: 6.489 min  
 Delta R.T.: 0.000 min  
 Response: 16043587  
 Conc: 286.66 ng/ml

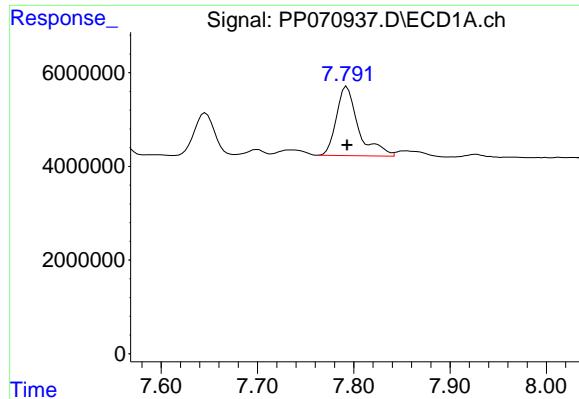

#30 AR-1254-5

R.T.: 7.793 min  
Delta R.T.: 0.000 min  
Response: 23415043  
Conc: 289.59 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1254ICC250

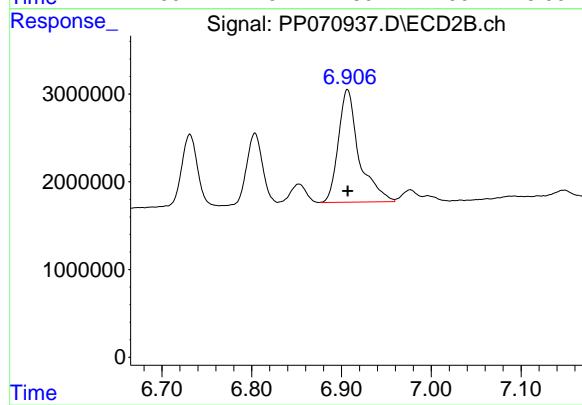

#30 AR-1254-5

R.T.: 6.907 min  
Delta R.T.: 0.000 min  
Response: 20606411  
Conc: 286.89 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070940.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:48  
 Operator : YP\AJ  
 Sample : AR1268ICC1000  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.516	3.817	152.3E6	105.1E6	94.769	94.009
2) SA Decachlor...	10.232	8.860	195.7E6	148.5E6	93.377	94.968

Target Compounds

41) L9 AR-1268-1	8.730	7.729	226.6E6	165.2E6	945.404	945.364
42) L9 AR-1268-2	8.824	7.795	190.4E6	137.8E6	950.797	945.407
43) L9 AR-1268-3	9.056	8.001	163.6E6	120.1E6	940.749	965.766
44) L9 AR-1268-4	9.474	8.295	70377008	51096977	960.945	957.859
45) L9 AR-1268-5	9.891	8.596	459.6E6	357.1E6	952.414	962.556



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070940.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 16:48  
 Operator : YP\AJ  
 Sample : AR1268ICC1000  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC1000**


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

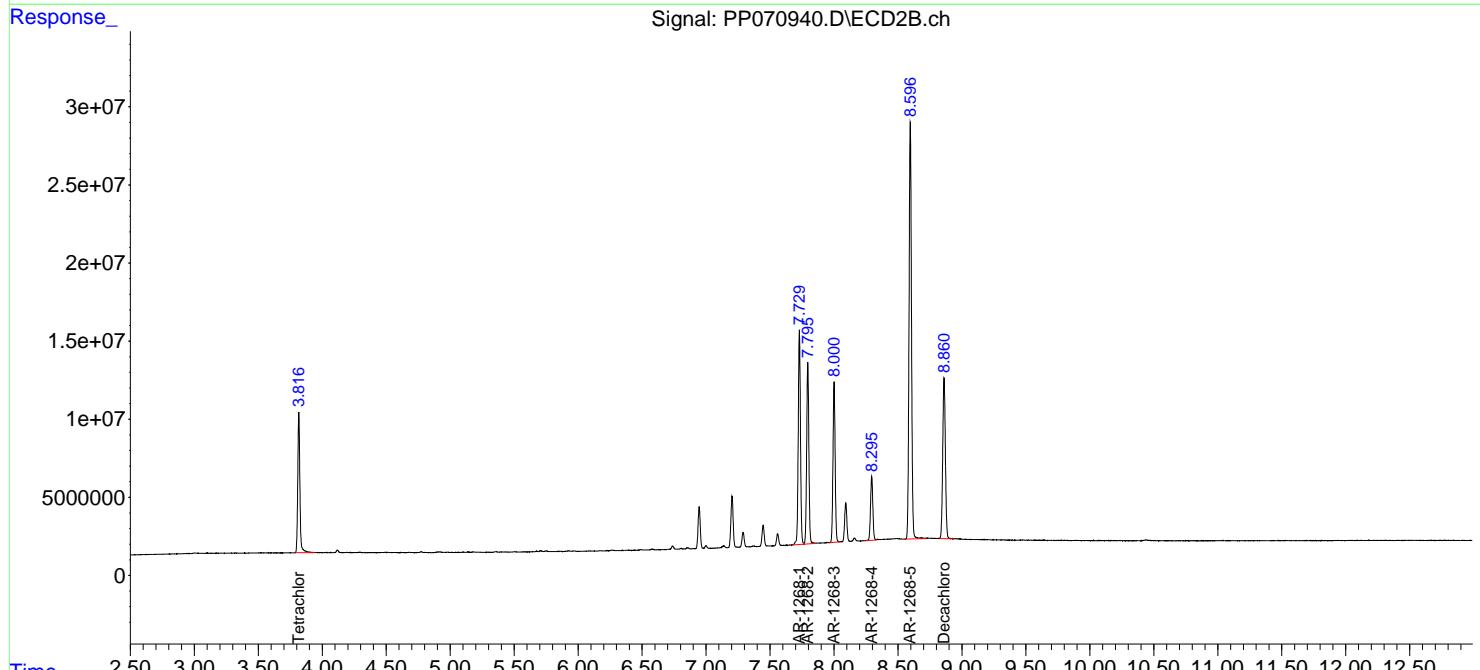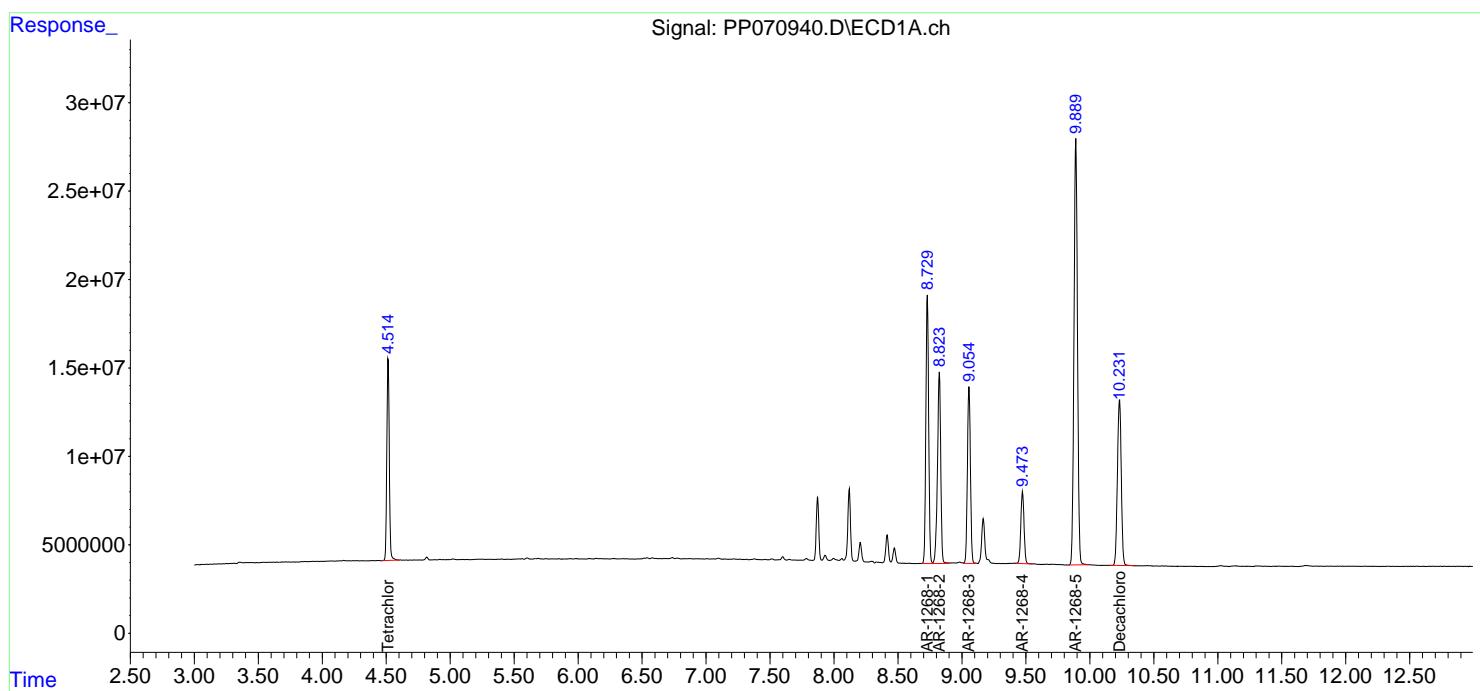





#1 Tetrachloro-m-xylene  
R.T.: 4.516 min  
Delta R.T.: 0.003 min  
Response: 152348529  
Conc: 94.77 ng/ml  
Instrument: ECD\_P  
ClientSampleId: AR1268ICC1000

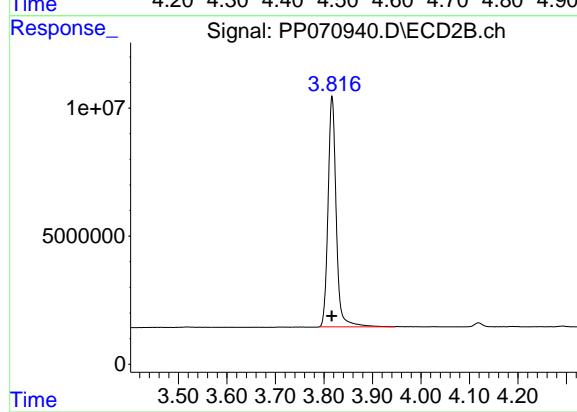


#1 Tetrachloro-m-xylene  
R.T.: 3.817 min  
Delta R.T.: 0.000 min  
Response: 105128984  
Conc: 94.01 ng/ml



#2 Decachlorobiphenyl  
R.T.: 10.232 min  
Delta R.T.: 0.003 min  
Response: 195698435  
Conc: 93.38 ng/ml

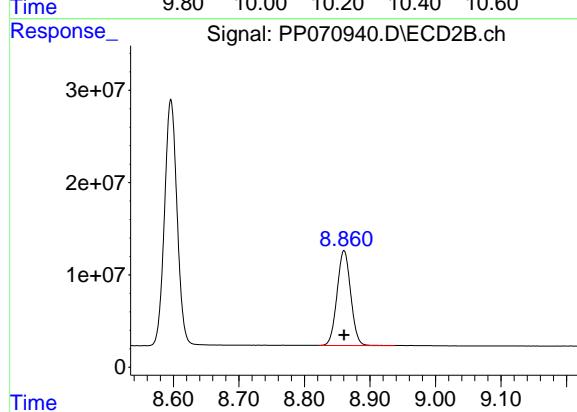

#2 Decachlorobiphenyl  
R.T.: 8.860 min  
Delta R.T.: 0.000 min  
Response: 148482089  
Conc: 94.97 ng/ml

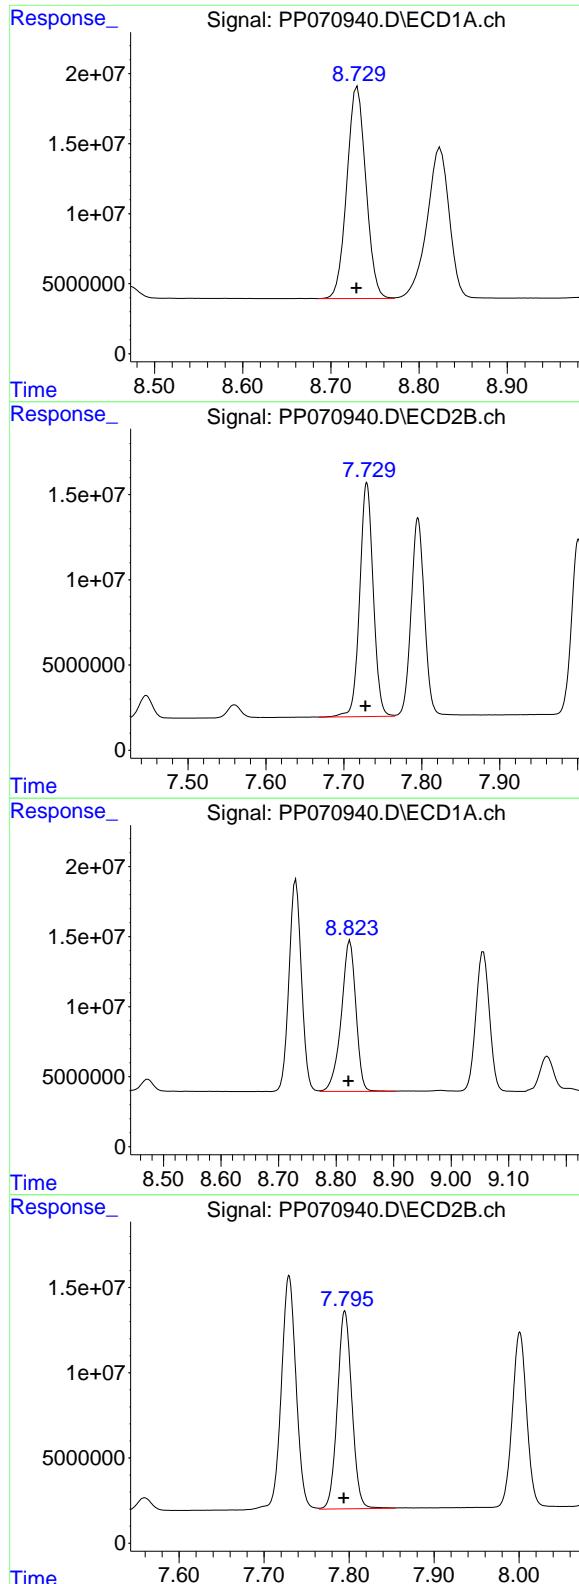

#41 AR-1268-1

R.T.: 8.730 min  
 Delta R.T.: 0.001 min  
 Response: 226575551  
 Conc: 945.40 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1268ICC1000

#41 AR-1268-1


R.T.: 7.729 min  
 Delta R.T.: 0.002 min  
 Response: 165156091  
 Conc: 945.36 ng/ml

#42 AR-1268-2

R.T.: 8.824 min  
 Delta R.T.: 0.003 min  
 Response: 190380276  
 Conc: 950.80 ng/ml

#42 AR-1268-2


R.T.: 7.795 min  
 Delta R.T.: 0.001 min  
 Response: 137801505  
 Conc: 945.41 ng/ml



#43 AR-1268-3


R.T.: 9.056 min  
 Delta R.T.: 0.003 min  
 Response: 163648333  
 Conc: 940.75 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1268ICC1000

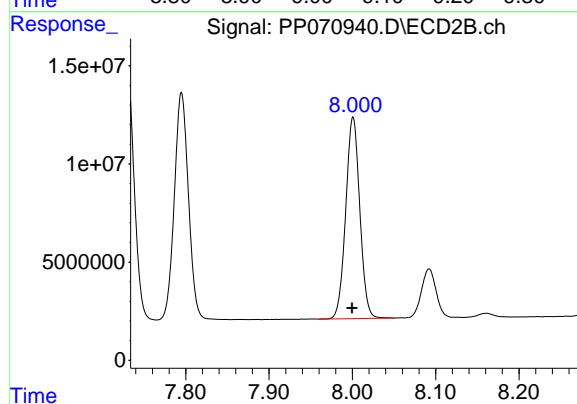


#43 AR-1268-3

R.T.: 8.001 min  
 Delta R.T.: 0.001 min  
 Response: 120132746  
 Conc: 965.77 ng/ml

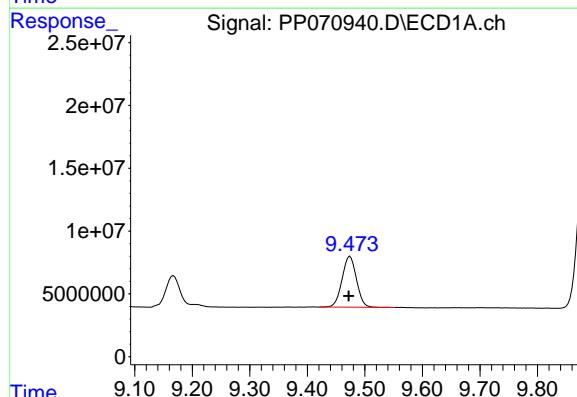


#44 AR-1268-4

R.T.: 9.474 min  
 Delta R.T.: 0.002 min  
 Response: 70377008  
 Conc: 960.95 ng/ml

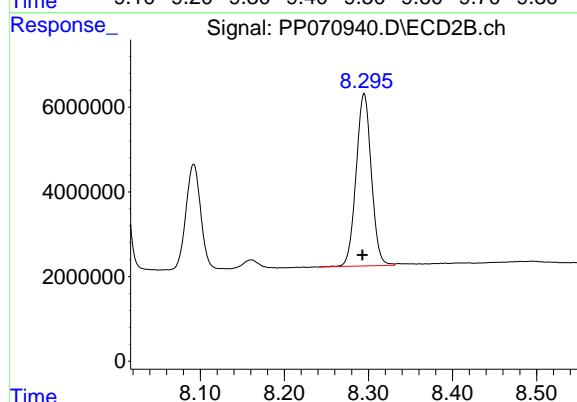

#44 AR-1268-4

R.T.: 8.295 min  
 Delta R.T.: 0.002 min  
 Response: 51096977  
 Conc: 957.86 ng/ml

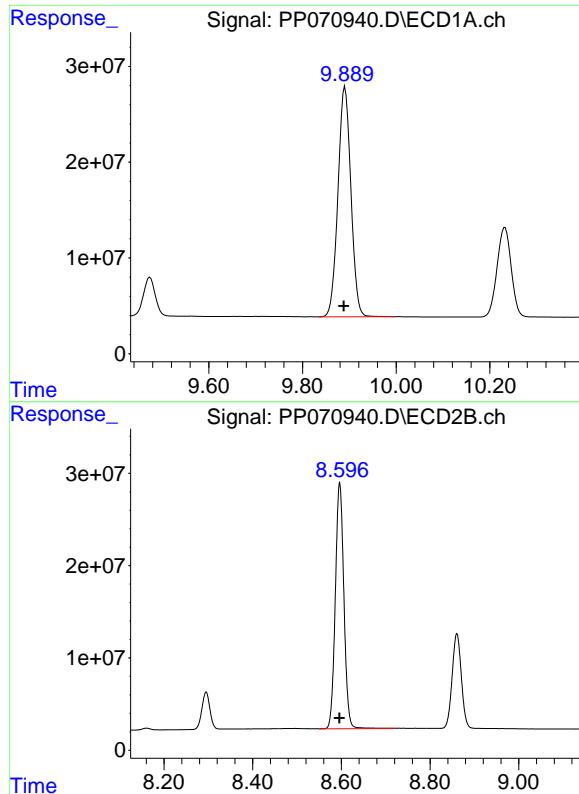

#45 AR-1268-5

R.T.: 9.891 min  
Delta R.T.: 0.003 min  
Response: 459553484  
Conc: 952.41 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1268ICC1000

#45 AR-1268-5

R.T.: 8.596 min  
Delta R.T.: 0.000 min  
Response: 357060145  
Conc: 962.56 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070941.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:05  
 Operator : YP\AJ  
 Sample : AR1268ICC750  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:14 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.514	3.817	119.6E6	83914927	74.397	75.039
2) SA Decachlor...	10.230	8.861	154.1E6	118.4E6	73.551	75.751

Target Compounds

41) L9 AR-1268-1	8.730	7.729	178.4E6	132.1E6	744.578	755.945
42) L9 AR-1268-2	8.823	7.795	149.2E6	110.8E6	745.140	760.189
43) L9 AR-1268-3	9.055	8.000	128.8E6	95630424	740.439	768.788
44) L9 AR-1268-4	9.473	8.294	55249435	40878954	754.389	766.313
45) L9 AR-1268-5	9.890	8.596	361.2E6	282.2E6	748.577	760.668



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070941.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:05  
 Operator : YP\AJ  
 Sample : AR1268ICC750  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC750**


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:14 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

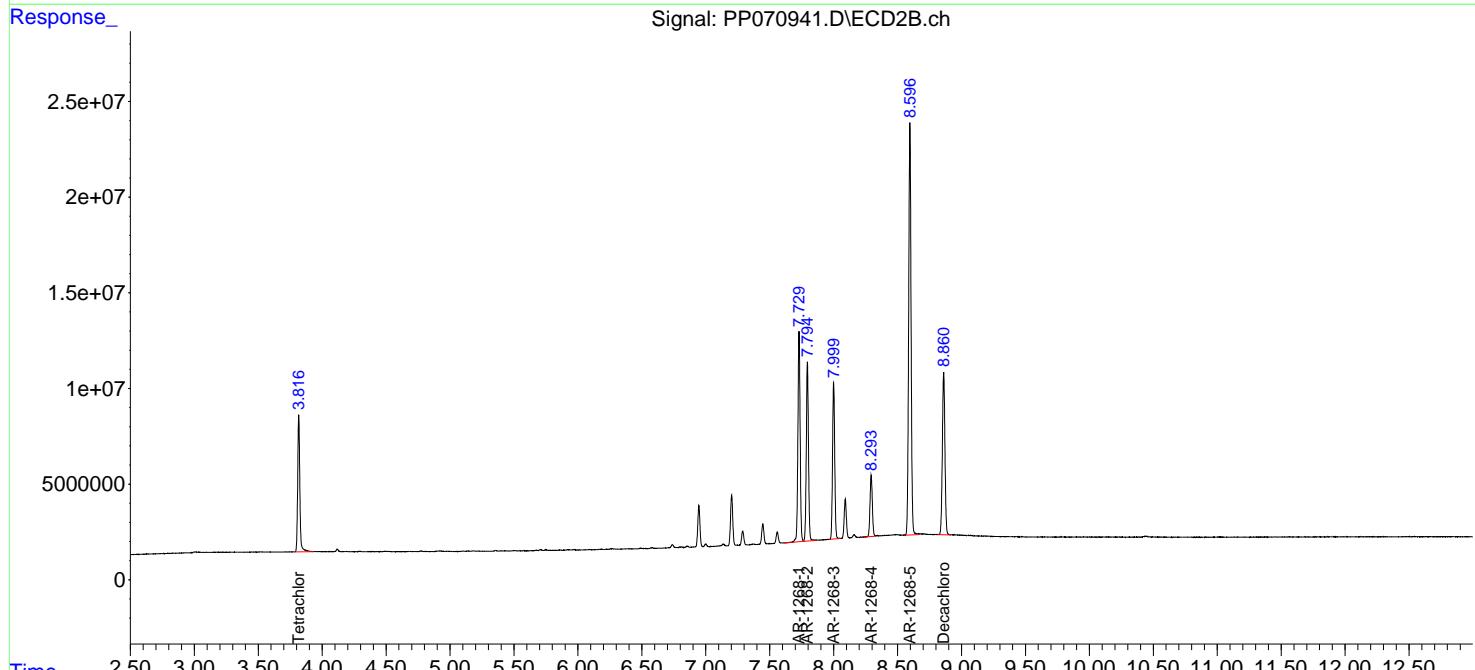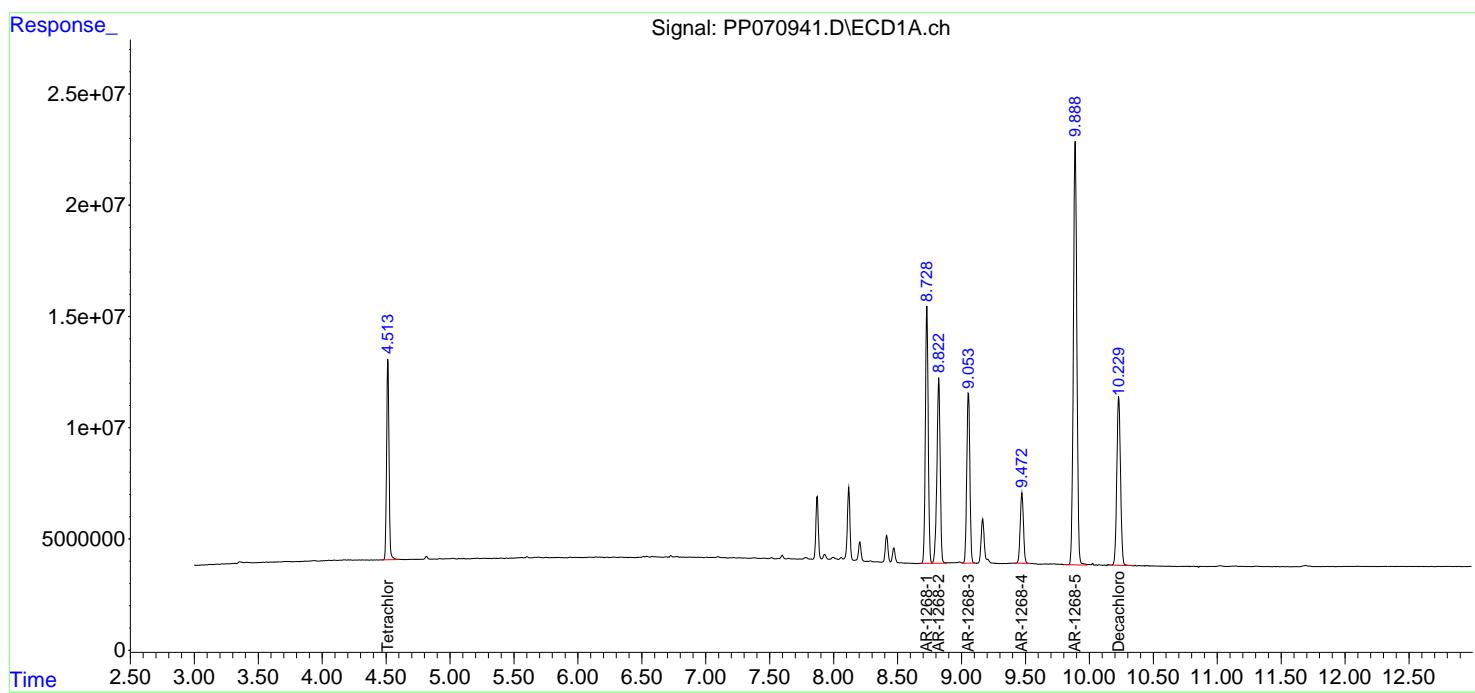





#1 Tetrachloro-m-xylene  
R.T.: 4.514 min  
Delta R.T.: 0.001 min  
Response: 119597931  
Conc: 74.40 ng/ml  
Instrument: ECD\_P  
ClientSampleId: AR1268ICC750

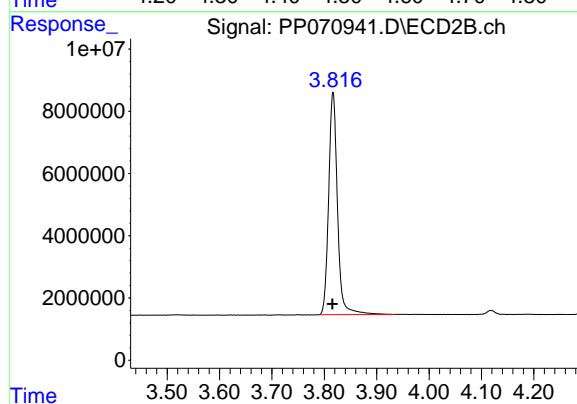


#1 Tetrachloro-m-xylene  
R.T.: 3.817 min  
Delta R.T.: 0.000 min  
Response: 83914927  
Conc: 75.04 ng/ml

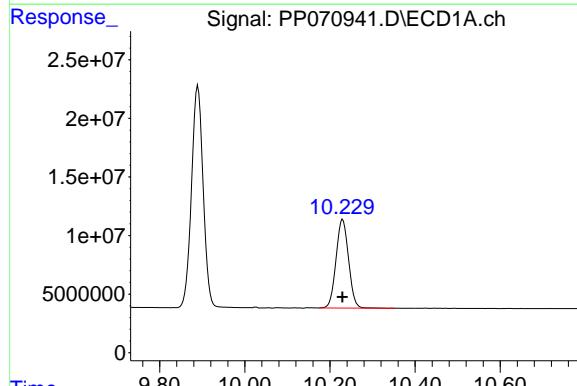

#2 Decachlorobiphenyl  
R.T.: 10.230 min  
Delta R.T.: 0.000 min  
Response: 154146813  
Conc: 73.55 ng/ml

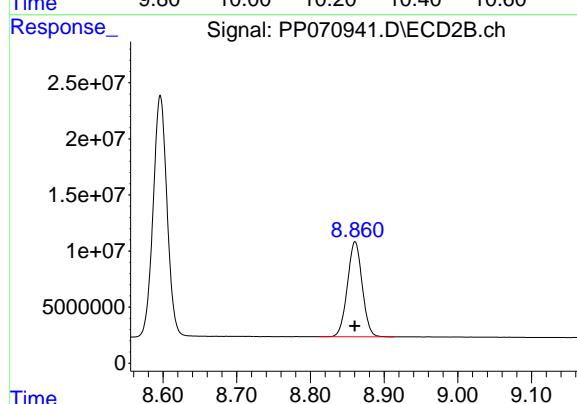


#2 Decachlorobiphenyl  
R.T.: 8.861 min  
Delta R.T.: 0.000 min  
Response: 118436920  
Conc: 75.75 ng/ml



#41 AR-1268-1


R.T.: 8.730 min  
 Delta R.T.: 0.001 min  
 Response: 178445590  
 Conc: 744.58 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1268ICC750

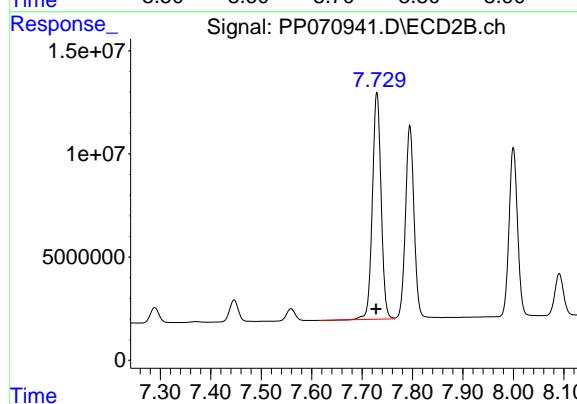


#41 AR-1268-1

R.T.: 7.729 min  
 Delta R.T.: 0.002 min  
 Response: 132064453  
 Conc: 755.95 ng/ml

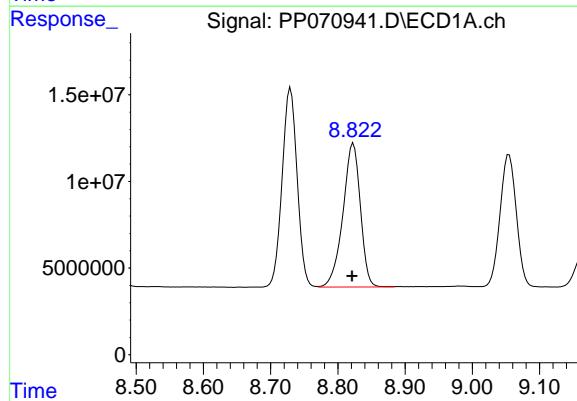


#42 AR-1268-2

R.T.: 8.823 min  
 Delta R.T.: 0.002 min  
 Response: 149201176  
 Conc: 745.14 ng/ml

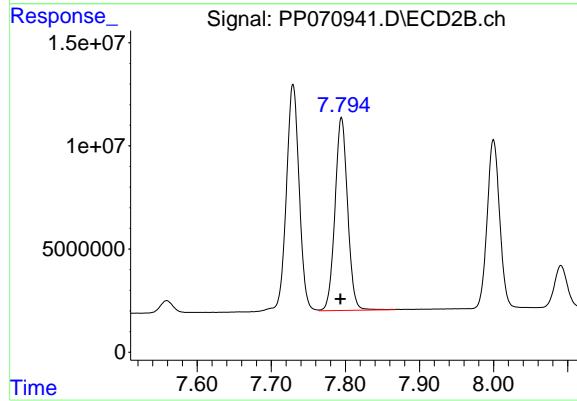

#42 AR-1268-2

R.T.: 7.795 min  
 Delta R.T.: 0.001 min  
 Response: 110804324  
 Conc: 760.19 ng/ml

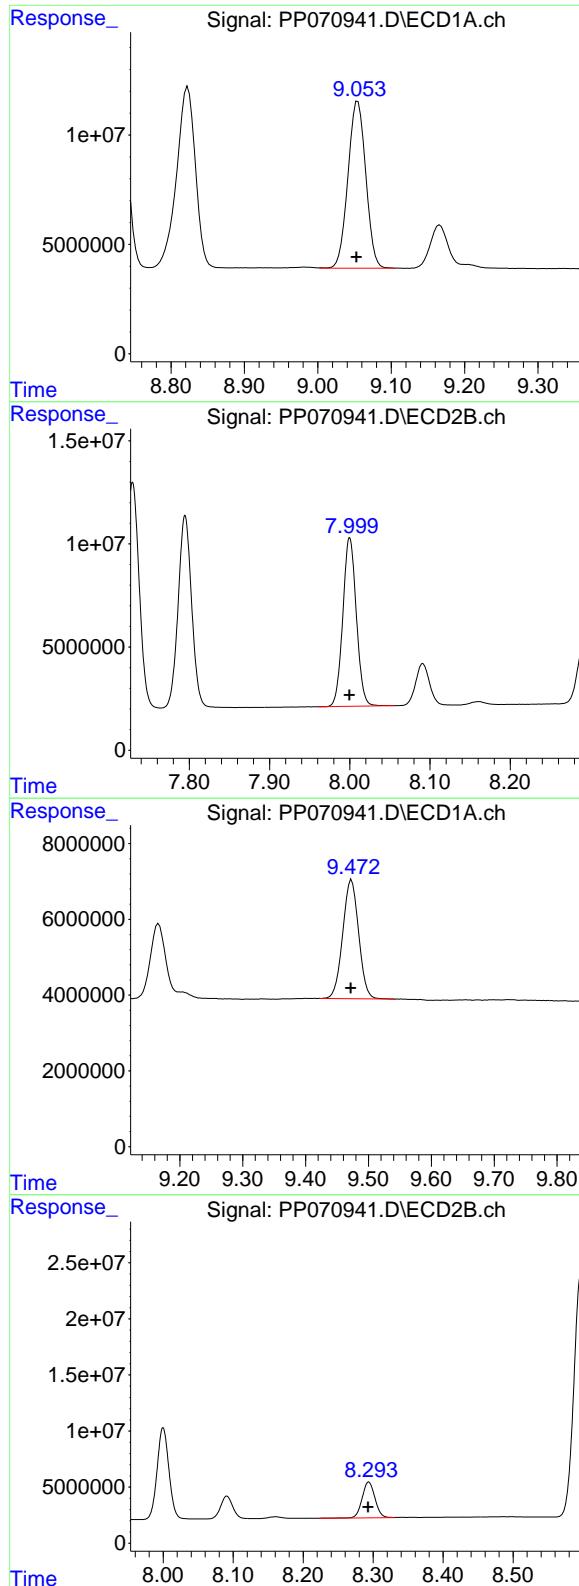

#43 AR-1268-3

R.T.: 9.055 min  
 Delta R.T.: 0.002 min  
 Response: 128803338  
 Conc: 740.44 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1268ICC750

#43 AR-1268-3


R.T.: 8.000 min  
 Delta R.T.: 0.000 min  
 Response: 95630424  
 Conc: 768.79 ng/ml

#44 AR-1268-4

R.T.: 9.473 min  
 Delta R.T.: 0.001 min  
 Response: 55249435  
 Conc: 754.39 ng/ml

#44 AR-1268-4

R.T.: 8.294 min  
 Delta R.T.: 0.000 min  
 Response: 40878954  
 Conc: 766.31 ng/ml

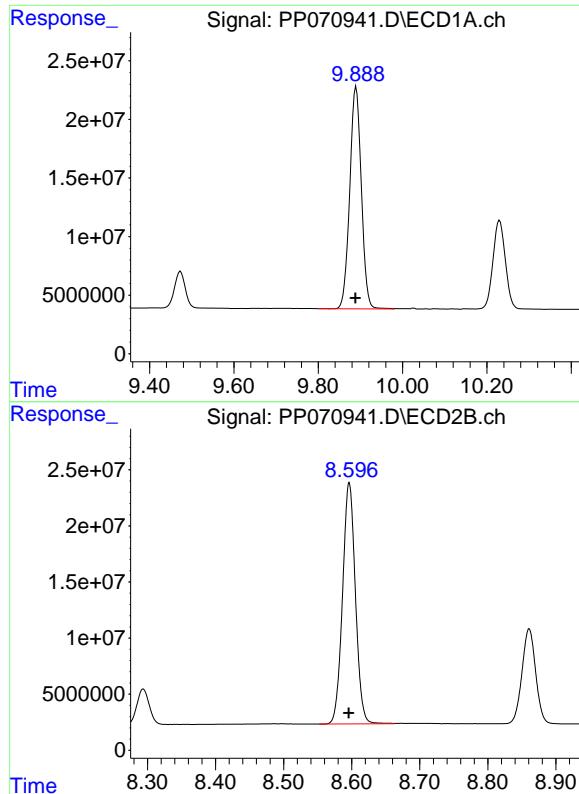

#45 AR-1268-5

R.T.: 9.890 min  
Delta R.T.: 0.002 min  
Response: 361198889  
Conc: 748.58 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1268ICC750

#45 AR-1268-5

R.T.: 8.596 min  
Delta R.T.: 0.000 min  
Response: 282169730  
Conc: 760.67 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070942.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:21  
 Operator : YP\AJ  
 Sample : AR1268ICC500  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.513	3.816	80378727	55914176	50.000	50.000
2) SA Decachlor...	10.230	8.860	104.8E6	78175161	50.000	50.000

Target Compounds

41) L9 AR-1268-1	8.729	7.728	119.8E6	87398242	500.000	500.273
42) L9 AR-1268-2	8.821	7.793	100.1E6	72879434	500.000	500.000
43) L9 AR-1268-3	9.053	8.000	86977678	62195601	500.000	500.000
44) L9 AR-1268-4	9.472	8.293	36618642	26672497	500.000	500.000
45) L9 AR-1268-5	9.888	8.596	241.3E6	185.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070942.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:21  
 Operator : YP\AJ  
 Sample : AR1268ICC500  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC500**


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:28 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

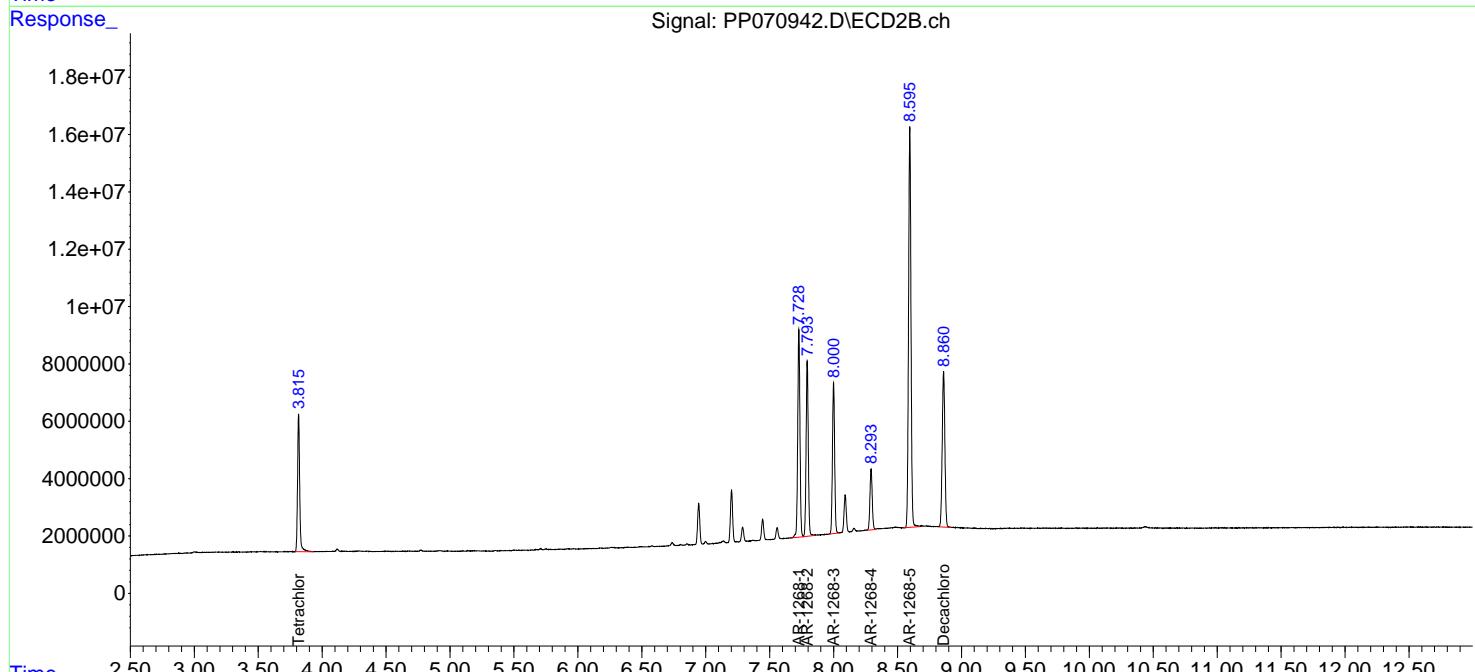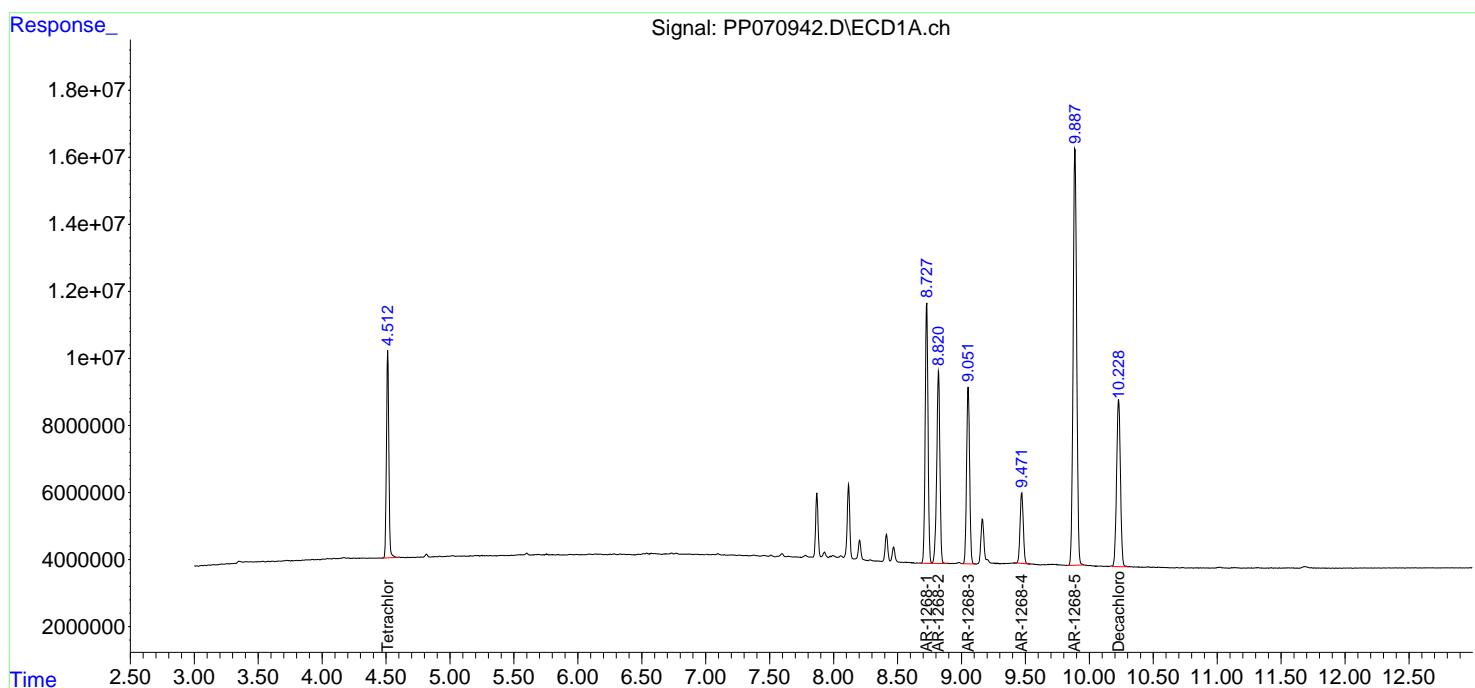





#1 Tetrachloro-m-xylene  
R.T.: 4.513 min  
Delta R.T.: 0.000 min  
Response: 80378727  
Conc: 50.00 ng/ml  
Instrument: ECD\_P  
ClientSampleId: AR1268ICC500

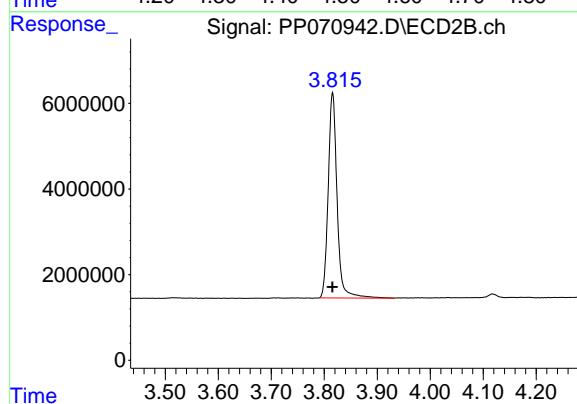


#1 Tetrachloro-m-xylene  
R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 55914176  
Conc: 50.00 ng/ml

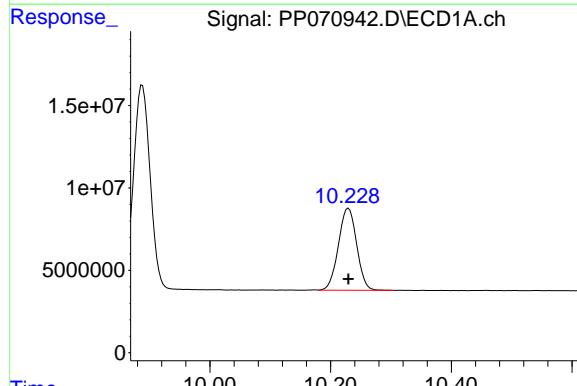

#2 Decachlorobiphenyl  
R.T.: 10.230 min  
Delta R.T.: 0.000 min  
Response: 104789095  
Conc: 50.00 ng/ml

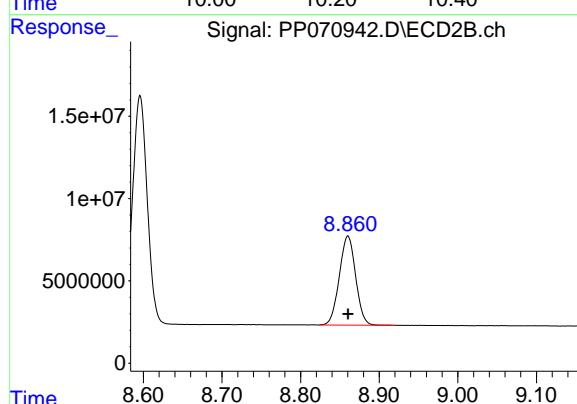

#2 Decachlorobiphenyl  
R.T.: 8.860 min  
Delta R.T.: 0.000 min  
Response: 78175161  
Conc: 50.00 ng/ml

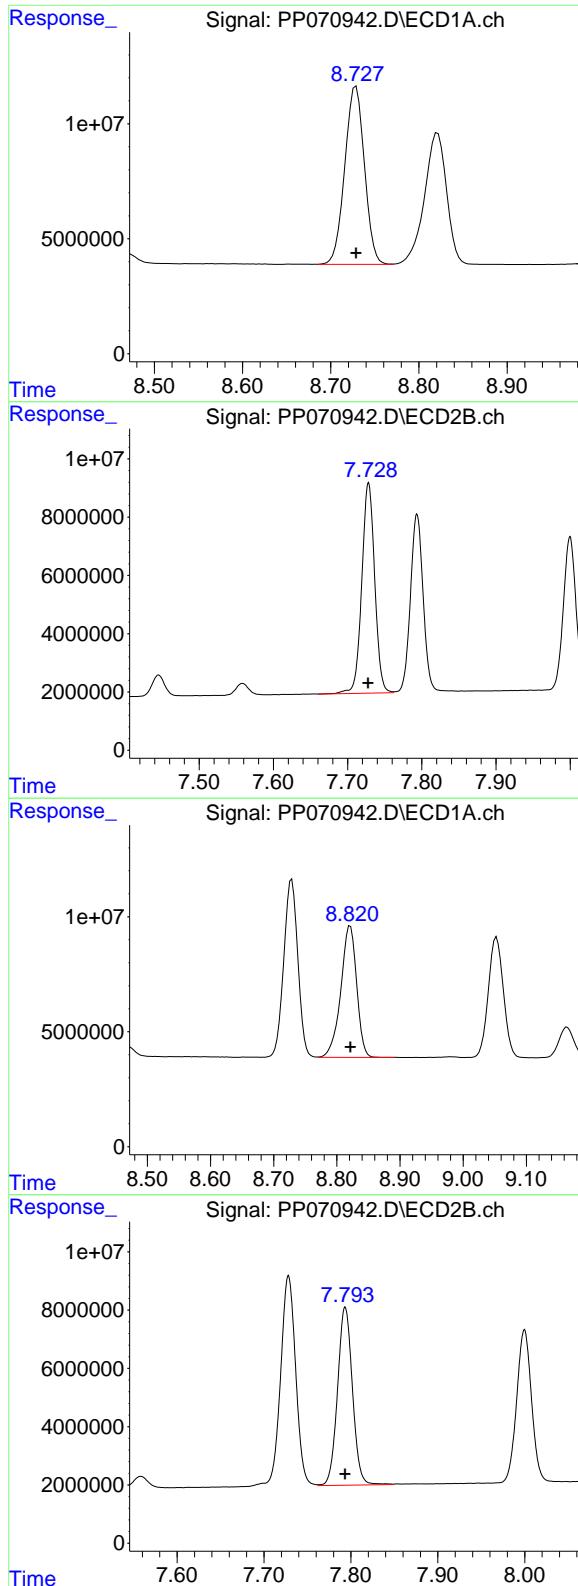

#41 AR-1268-1

R.T.: 8.729 min  
 Delta R.T.: 0.000 min  
 Response: 119830016  
 Conc: 500.00 ng/ml

**Instrument:** ECD\_P  
**ClientSampleId:** AR1268ICC500

#41 AR-1268-1


R.T.: 7.728 min  
 Delta R.T.: 0.000 min  
 Response: 87398242  
 Conc: 500.27 ng/ml

#42 AR-1268-2

R.T.: 8.821 min  
 Delta R.T.: 0.000 min  
 Response: 100116173  
 Conc: 500.00 ng/ml


#42 AR-1268-2

R.T.: 7.793 min  
 Delta R.T.: 0.000 min  
 Response: 72879434  
 Conc: 500.00 ng/ml




#43 AR-1268-3

R.T.: 9.053 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 86977678 ECD\_P  
 Conc: 500.00 ng/ml **ClientSampleId:**  
 AR1268ICC500

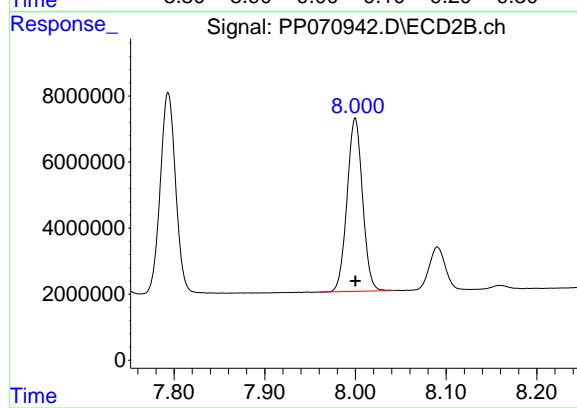


#43 AR-1268-3

R.T.: 8.000 min  
 Delta R.T.: 0.000 min  
 Response: 62195601  
 Conc: 500.00 ng/ml

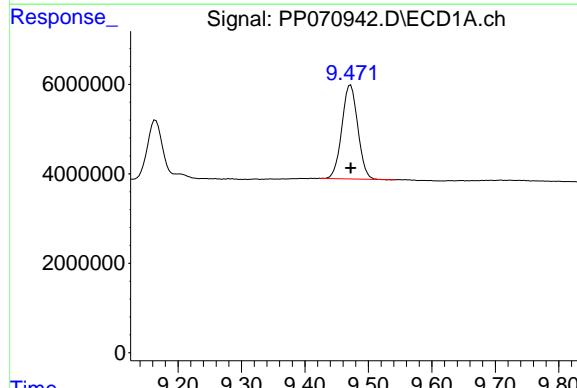


#44 AR-1268-4

R.T.: 9.472 min  
 Delta R.T.: 0.000 min  
 Response: 36618642  
 Conc: 500.00 ng/ml

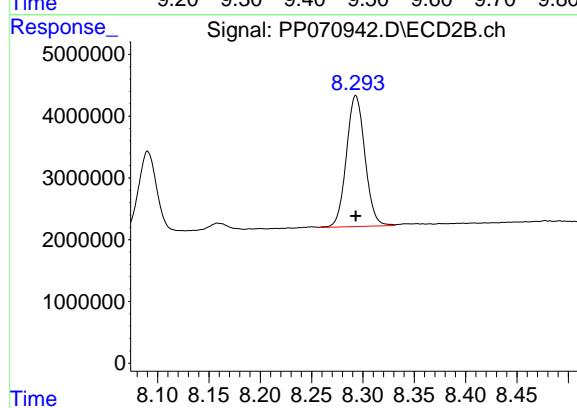

#44 AR-1268-4

R.T.: 8.293 min  
 Delta R.T.: 0.000 min  
 Response: 26672497  
 Conc: 500.00 ng/ml

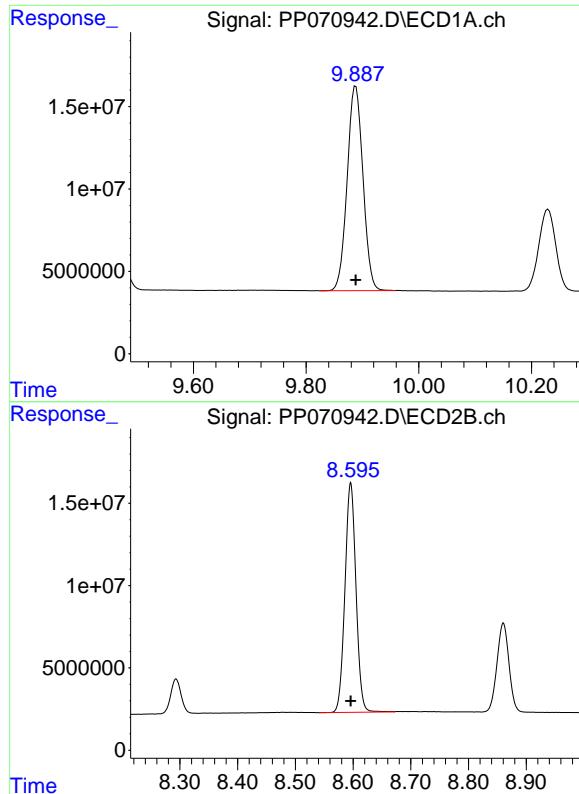

#45 AR-1268-5

R.T.: 9.888 min  
Delta R.T.: 0.000 min  
Response: 241257148  
Conc: 500.00 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1268ICC500

#45 AR-1268-5

R.T.: 8.596 min  
Delta R.T.: 0.000 min  
Response: 185474929  
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070943.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:37  
 Operator : YP\AJ  
 Sample : AR1268ICC250  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.515	3.817	41125313	29588552	25.582	26.459
2) SA Decachlor...	10.232	8.859	54285349	40518249	25.902	25.915

Target Compounds

41) L9 AR-1268-1	8.730	7.729	61973048	44387893	258.587	254.079
42) L9 AR-1268-2	8.824	7.794	51237231	36694564	255.889	251.748
43) L9 AR-1268-3	9.055	8.000	44311644	31811936	254.730	255.741
44) L9 AR-1268-4	9.473	8.295	18700738	13922493	255.345	260.990
45) L9 AR-1268-5	9.890	8.596	124.6E6	91636186	258.260	247.031



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070943.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:37  
 Operator : YP\AJ  
 Sample : AR1268ICC250  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC250**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 17:58:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

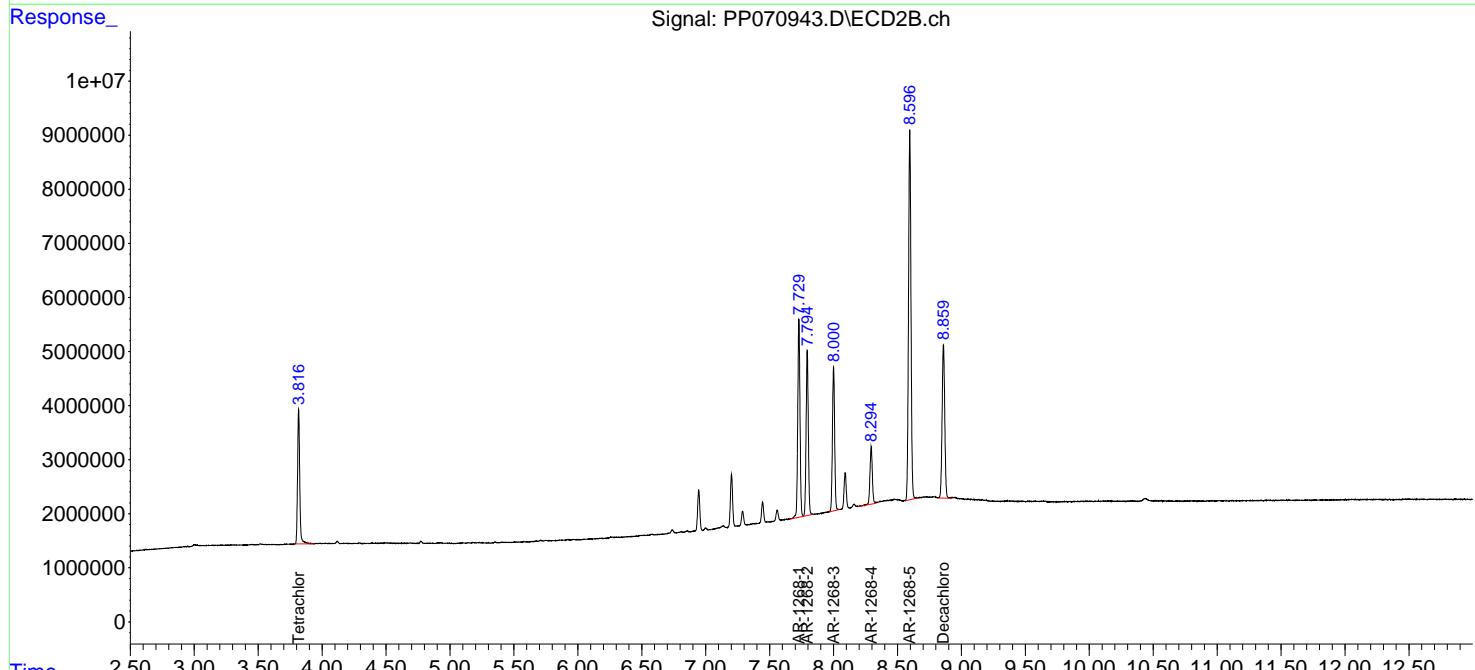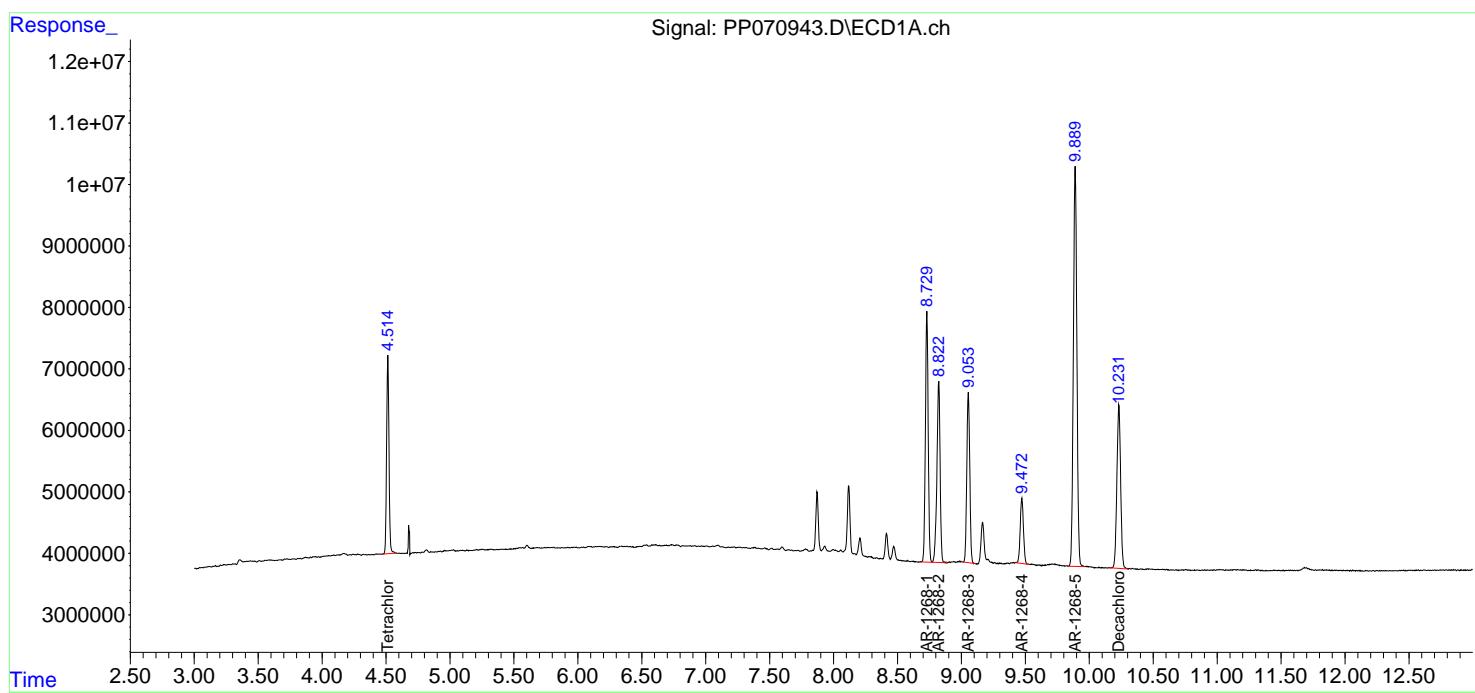




#1 Tetrachloro-m-xylene  
R.T.: 4.515 min  
Delta R.T.: 0.002 min  
Response: 41125313  
Conc: 25.58 ng/ml


Instrument: ECD\_P  
ClientSampleId: AR1268ICC250

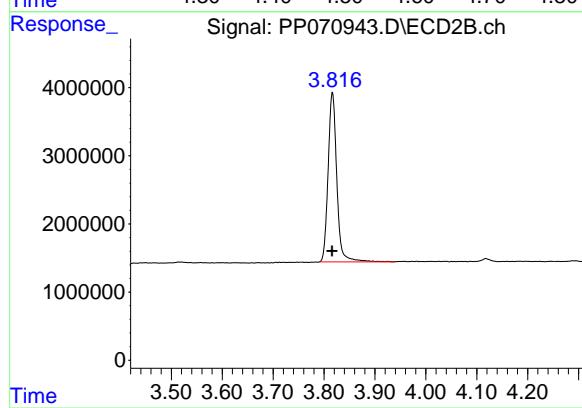


#1 Tetrachloro-m-xylene  
R.T.: 3.817 min  
Delta R.T.: 0.000 min  
Response: 29588552  
Conc: 26.46 ng/ml



#2 Decachlorobiphenyl  
R.T.: 10.232 min  
Delta R.T.: 0.003 min  
Response: 54285349  
Conc: 25.90 ng/ml

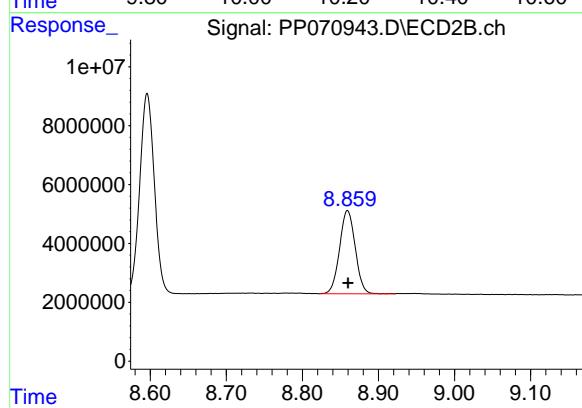

#2 Decachlorobiphenyl  
R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 40518249  
Conc: 25.92 ng/ml

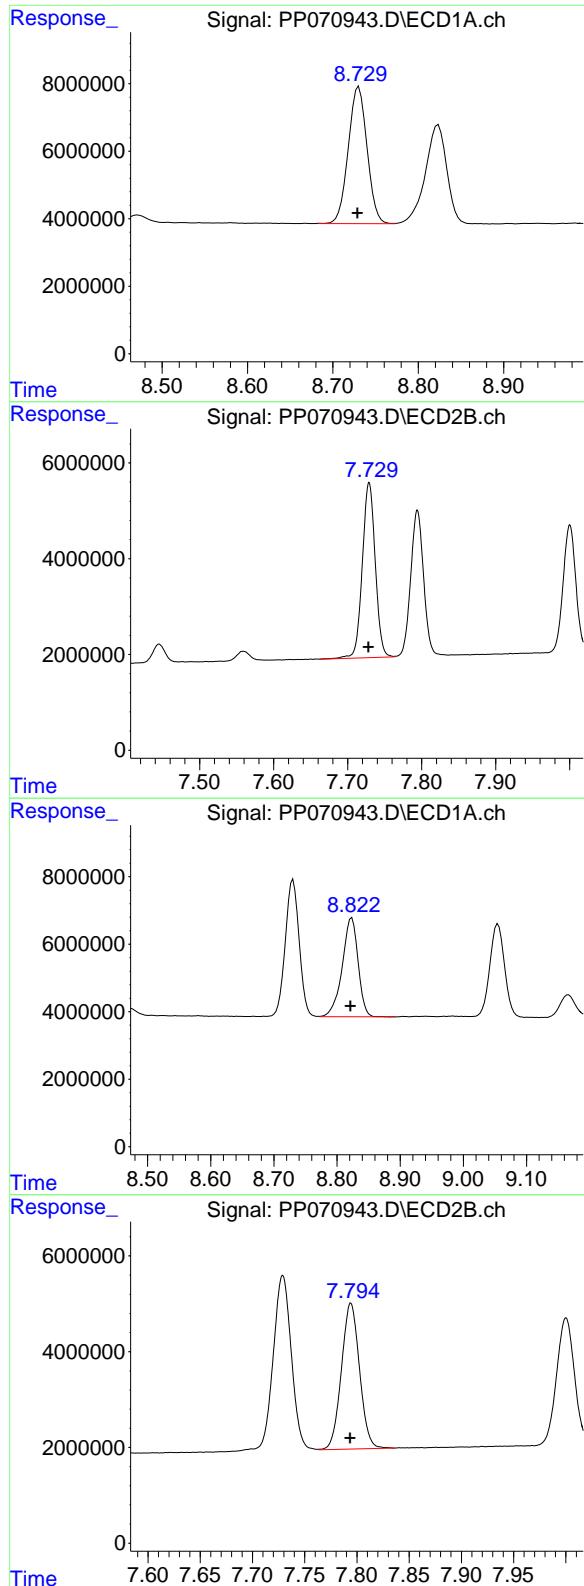

#41 AR-1268-1

R.T.: 8.730 min  
 Delta R.T.: 0.002 min  
 Response: 61973048  
 Conc: 258.59 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1268ICC250

#41 AR-1268-1


R.T.: 7.729 min  
 Delta R.T.: 0.001 min  
 Response: 44387893  
 Conc: 254.08 ng/ml

#42 AR-1268-2

R.T.: 8.824 min  
 Delta R.T.: 0.002 min  
 Response: 51237231  
 Conc: 255.89 ng/ml

#42 AR-1268-2


R.T.: 7.794 min  
 Delta R.T.: 0.000 min  
 Response: 36694564  
 Conc: 251.75 ng/ml

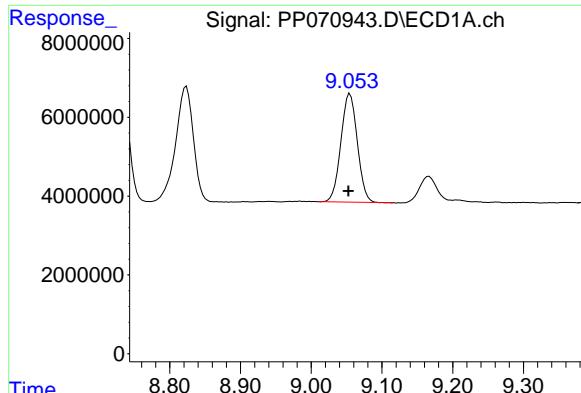

#43 AR-1268-3


R.T.: 9.055 min  
Delta R.T.: 0.002 min  
Response: 44311644  
Conc: 254.73 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1268ICC250

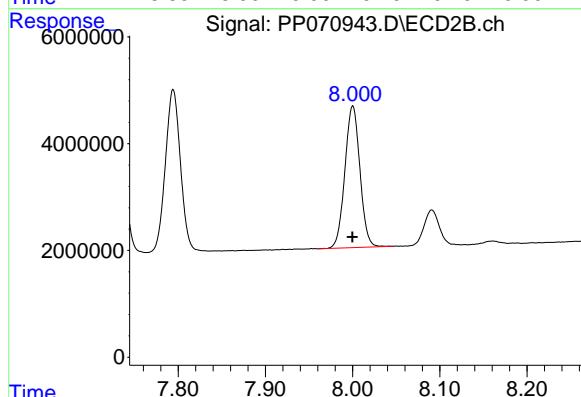


#43 AR-1268-3

R.T.: 8.000 min  
Delta R.T.: 0.000 min  
Response: 31811936  
Conc: 255.74 ng/ml

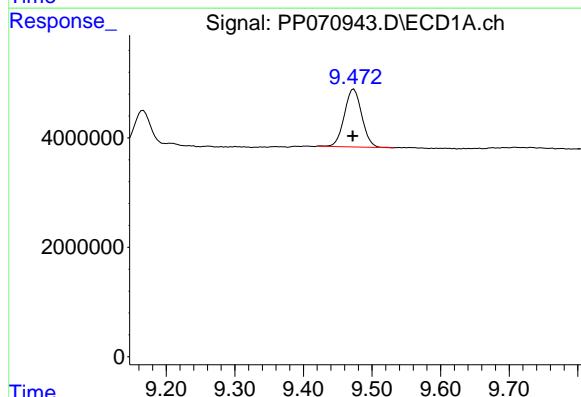


#44 AR-1268-4

R.T.: 9.473 min  
Delta R.T.: 0.002 min  
Response: 18700738  
Conc: 255.34 ng/ml

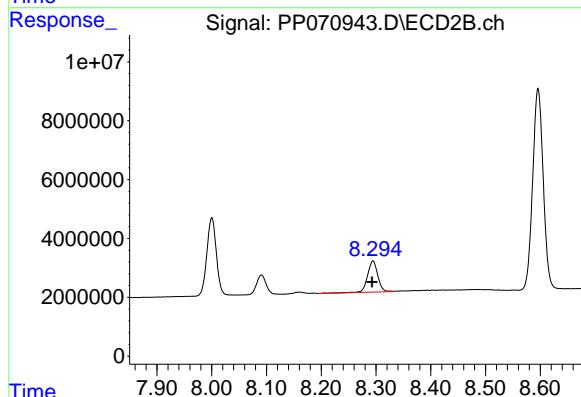

#44 AR-1268-4


R.T.: 8.295 min  
Delta R.T.: 0.002 min  
Response: 13922493  
Conc: 260.99 ng/ml

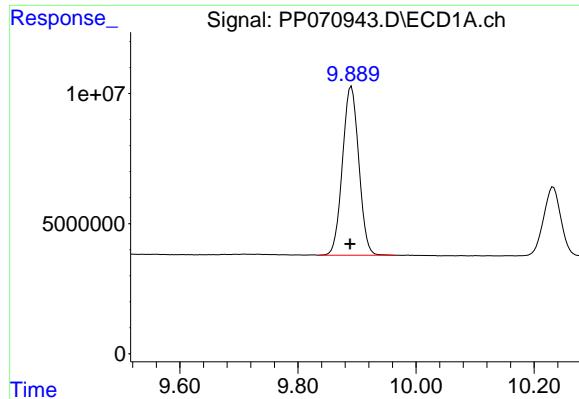

#45 AR-1268-5

R.T.: 9.890 min  
Delta R.T.: 0.002 min  
Response: 124614186  
Conc: 258.26 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1268ICC250

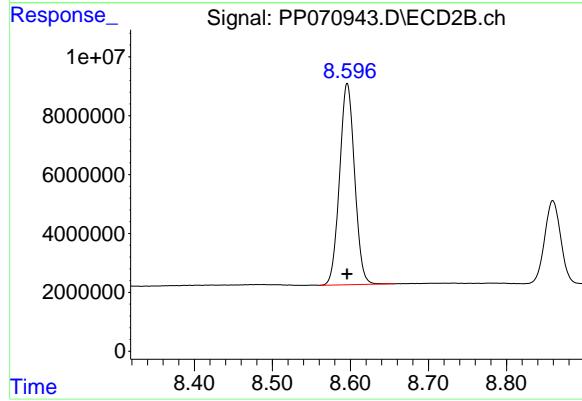

#45 AR-1268-5

R.T.: 8.596 min  
Delta R.T.: 0.000 min  
Response: 91636186  
Conc: 247.03 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070944.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:53  
 Operator : YP\AJ  
 Sample : AR1268ICC050  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 18:13:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.515	3.816	6795391	6304440	4.206	5.529 #
2) SA Decachlor...	10.230	8.859	10035177	7161586	4.762	4.510

Target Compounds

41) L9 AR-1268-1	8.729	7.728	11274140	8298716	46.621	47.221
42) L9 AR-1268-2	8.822	7.794	9103995	6916833	45.210	47.131
43) L9 AR-1268-3	9.054	7.999	8398993	5823381	48.183	46.078
44) L9 AR-1268-4	9.471	8.293	3082639	2842824	41.712	52.149 #
45) L9 AR-1268-5	9.889	8.596	22937830	16928167	47.050	45.599



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070944.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 17:53  
 Operator : YP\AJ  
 Sample : AR1268ICC050  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1268ICC050**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 27 18:13:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Mar 27 17:56:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

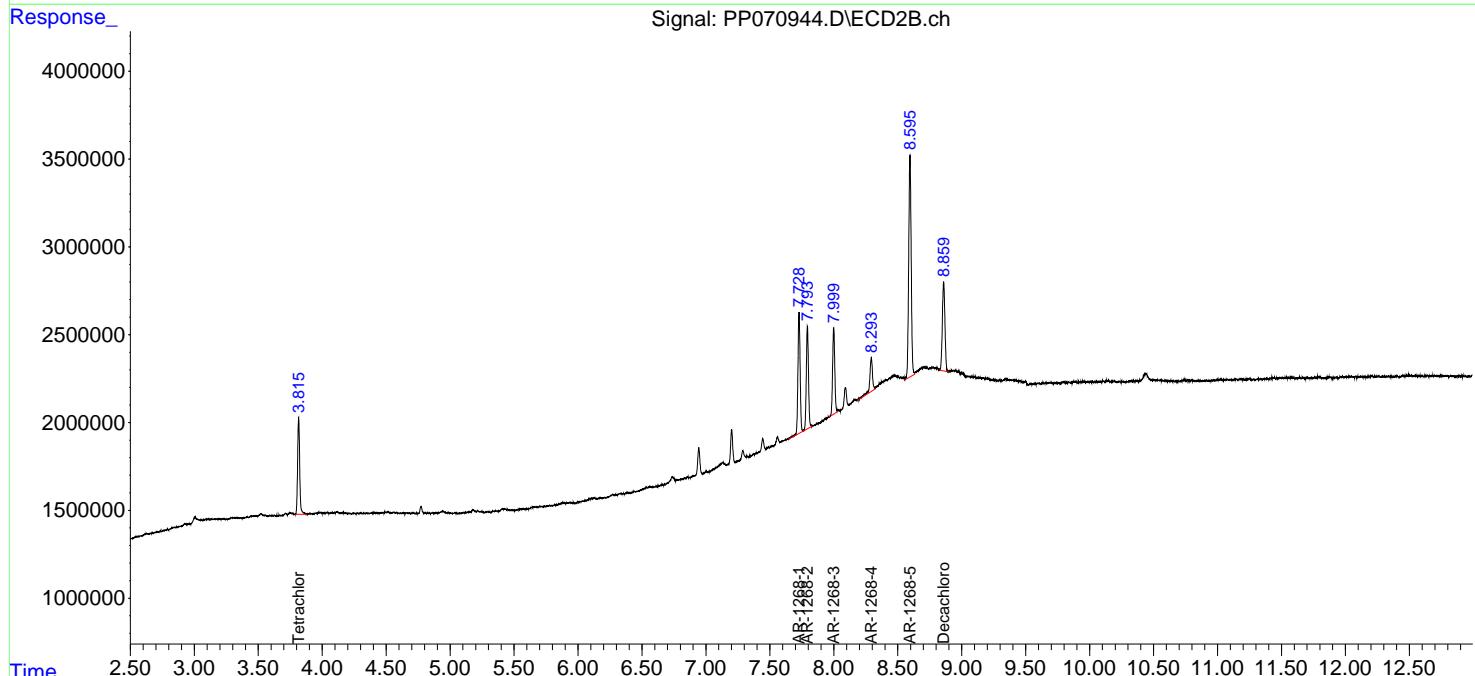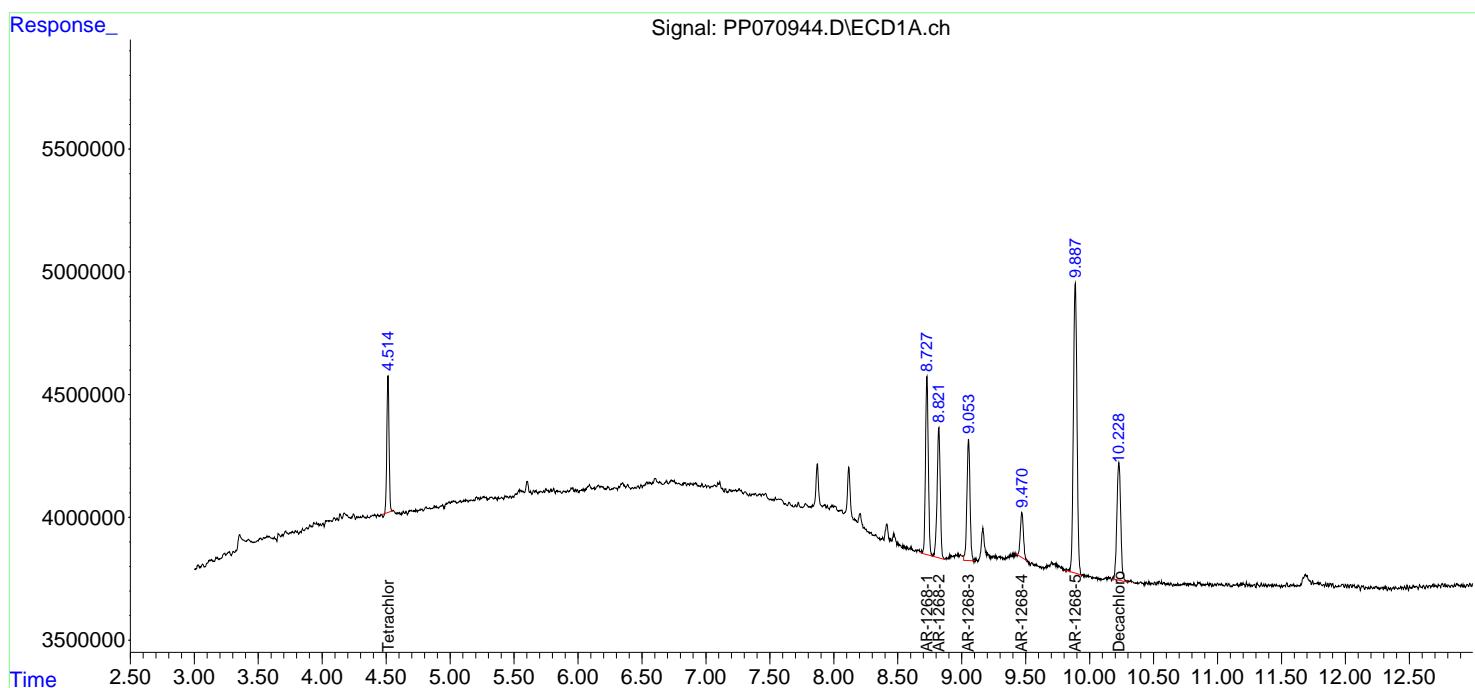

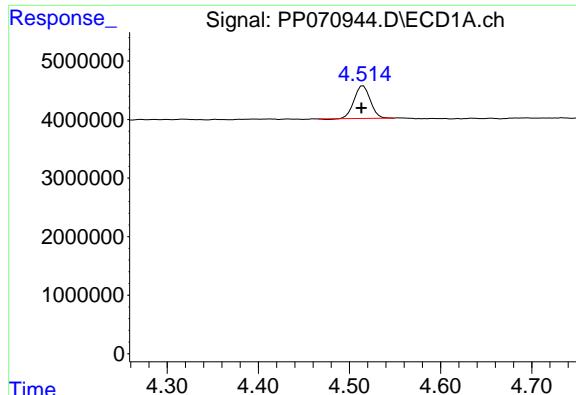

#1 Tetrachloro-m-xylene


R.T.: 4.515 min  
Delta R.T.: 0.002 min  
Response: 6795391  
Conc: 4.21 ng/ml

Instrument:

ECD\_P


ClientSampleId :

AR1268ICC050

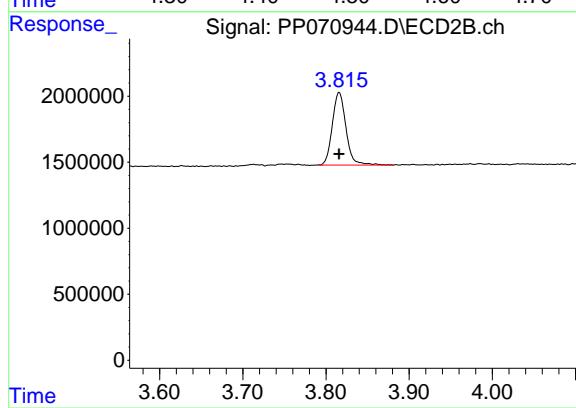


#1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 6304440  
Conc: 5.53 ng/ml

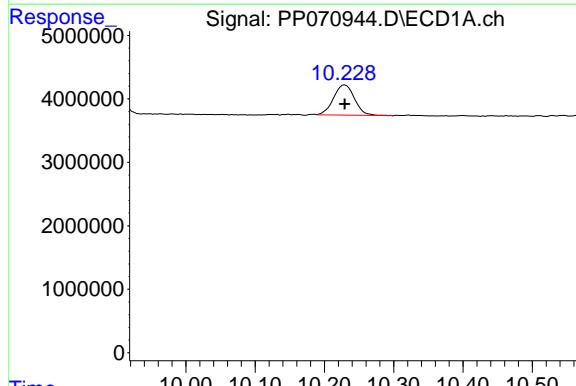


#2 Decachlorobiphenyl

R.T.: 10.230 min  
Delta R.T.: 0.000 min  
Response: 10035177  
Conc: 4.76 ng/ml

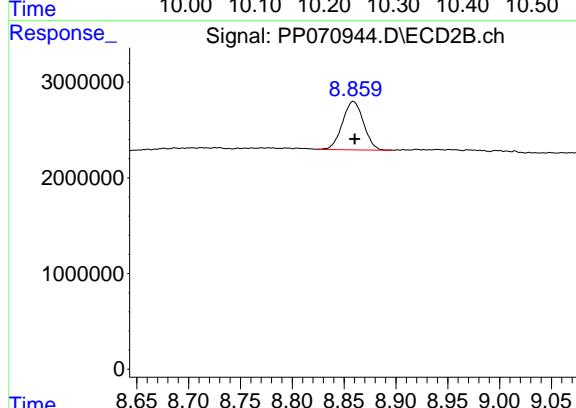

#2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: -0.001 min  
Response: 7161586  
Conc: 4.51 ng/ml

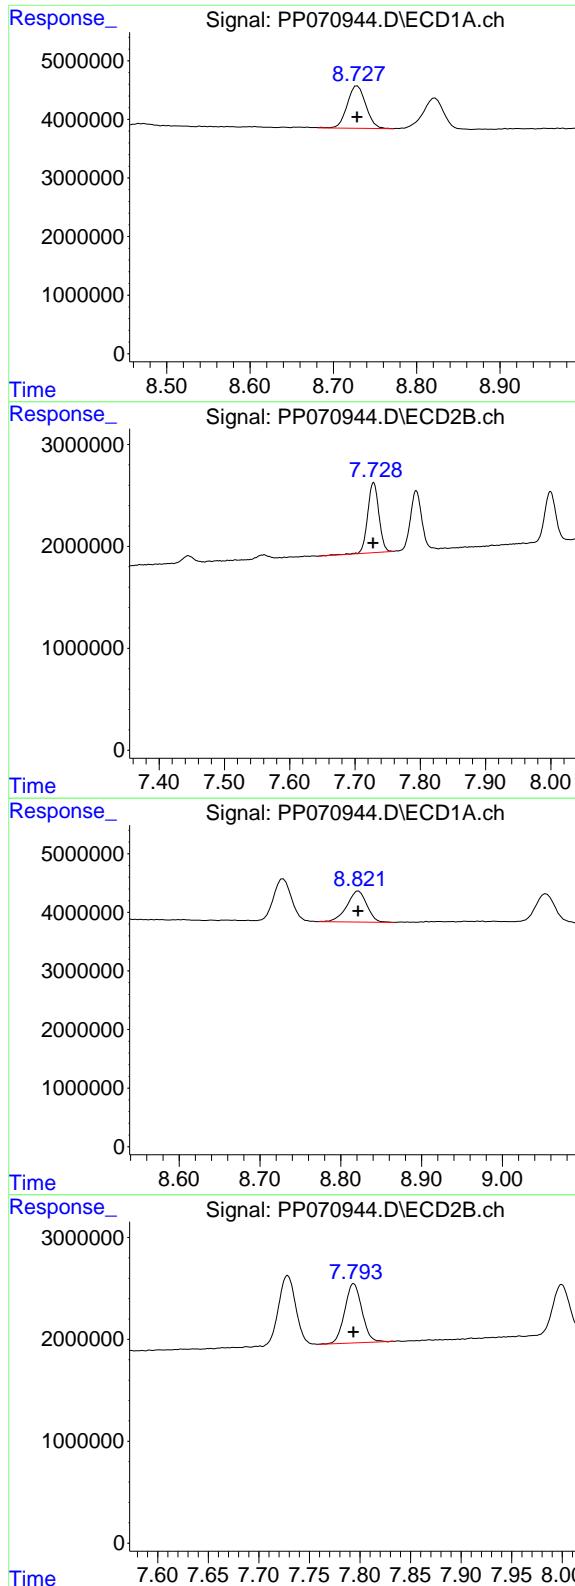

#41 AR-1268-1

R.T.: 8.729 min  
 Delta R.T.: 0.000 min  
 Response: 11274140  
 Conc: 46.62 ng/ml

**Instrument:** ECD\_P  
**ClientSampleId:** AR1268ICC050

#41 AR-1268-1


R.T.: 7.728 min  
 Delta R.T.: 0.000 min  
 Response: 8298716  
 Conc: 47.22 ng/ml

#42 AR-1268-2

R.T.: 8.822 min  
 Delta R.T.: 0.000 min  
 Response: 9103995  
 Conc: 45.21 ng/ml

#42 AR-1268-2

R.T.: 7.794 min  
 Delta R.T.: 0.000 min  
 Response: 6916833  
 Conc: 47.13 ng/ml

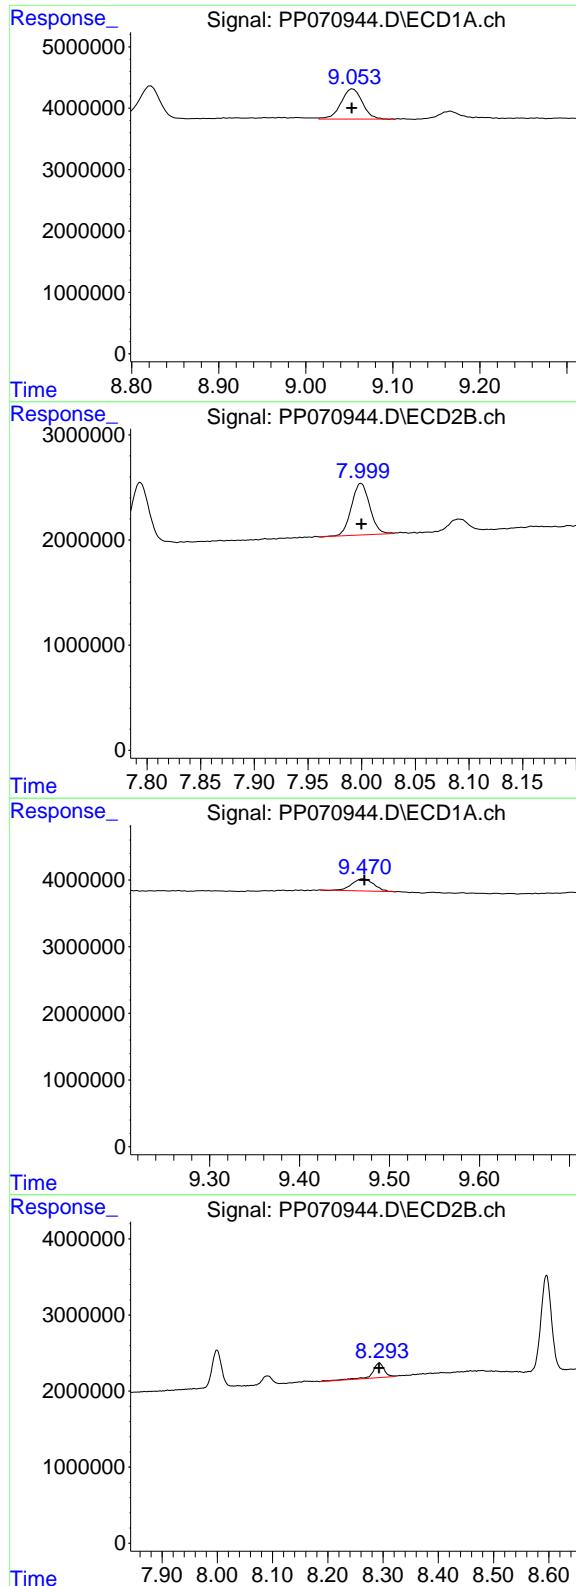

#43 AR-1268-3

R.T.: 9.054 min  
 Delta R.T.: 0.002 min  
 Response: 8398993  
 Conc: 48.18 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1268ICC050

#43 AR-1268-3



R.T.: 7.999 min  
 Delta R.T.: 0.000 min  
 Response: 5823381  
 Conc: 46.08 ng/ml

#44 AR-1268-4

R.T.: 9.471 min  
 Delta R.T.: 0.000 min  
 Response: 3082639  
 Conc: 41.71 ng/ml

#44 AR-1268-4

R.T.: 8.293 min  
 Delta R.T.: 0.000 min  
 Response: 2842824  
 Conc: 52.15 ng/ml

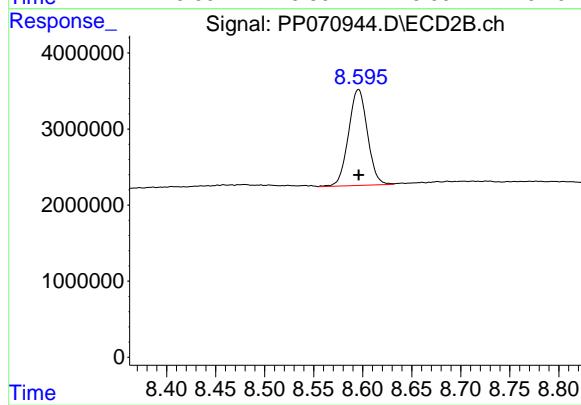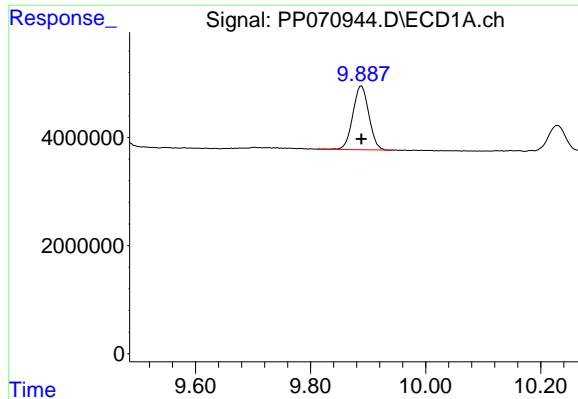

#45 AR-1268-5

R.T.: 9.889 min  
Delta R.T.: 0.000 min  
Response: 22937830  
Conc: 47.05 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1268ICC050

#45 AR-1268-5

R.T.: 8.596 min  
Delta R.T.: 0.000 min  
Response: 16928167  
Conc: 45.60 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070948.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 19:47  
 Operator : YP\AJ  
 Sample : AR1254ICV500  
 Misc :  
 ALS Vial : 34 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1254**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 01:39:10 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 01:37:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.513	3.816	80813408	55809150	53.470	50.687
2) SA Decachlor...	10.228	8.859	60442284	44113864	53.599	53.797

Target Compounds

26) L6 AR-1254-1	6.514	5.708	34026950	33372474	528.449	505.507
27) L6 AR-1254-2	6.730	5.856	52171420	28060451	516.086	491.442
28) L6 AR-1254-3	7.093	6.260	52059367	42608413	522.014	490.647
29) L6 AR-1254-4	7.375	6.489	45346150	27407702	523.647	488.547
30) L6 AR-1254-5	7.792	6.907	48183080	36336253	599.658	503.617



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP032725\  
 Data File : PP070948.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Mar 2025 19:47  
 Operator : YP\AJ  
 Sample : AR1254ICV500  
 Misc :  
 ALS Vial : 34 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**ICVPP032725AR1254**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 28 01:39:10 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 01:37:11 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$ m Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

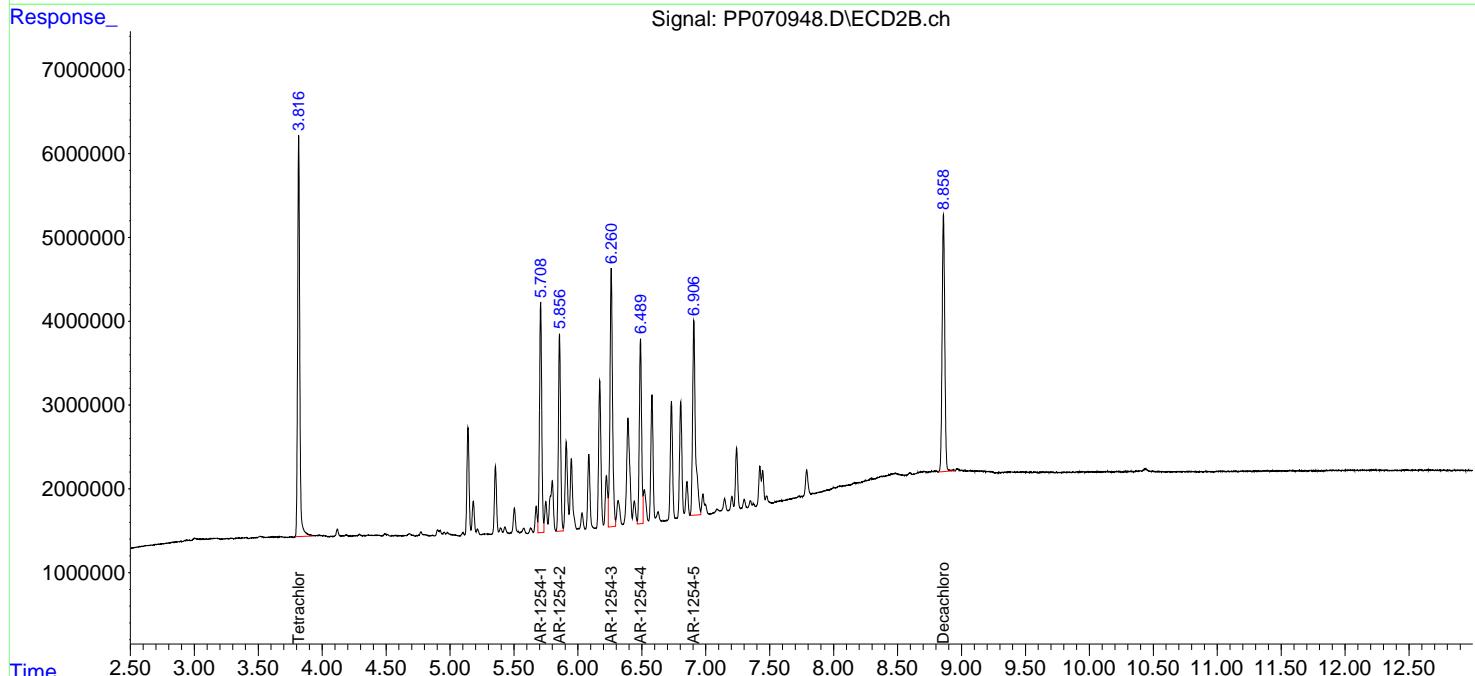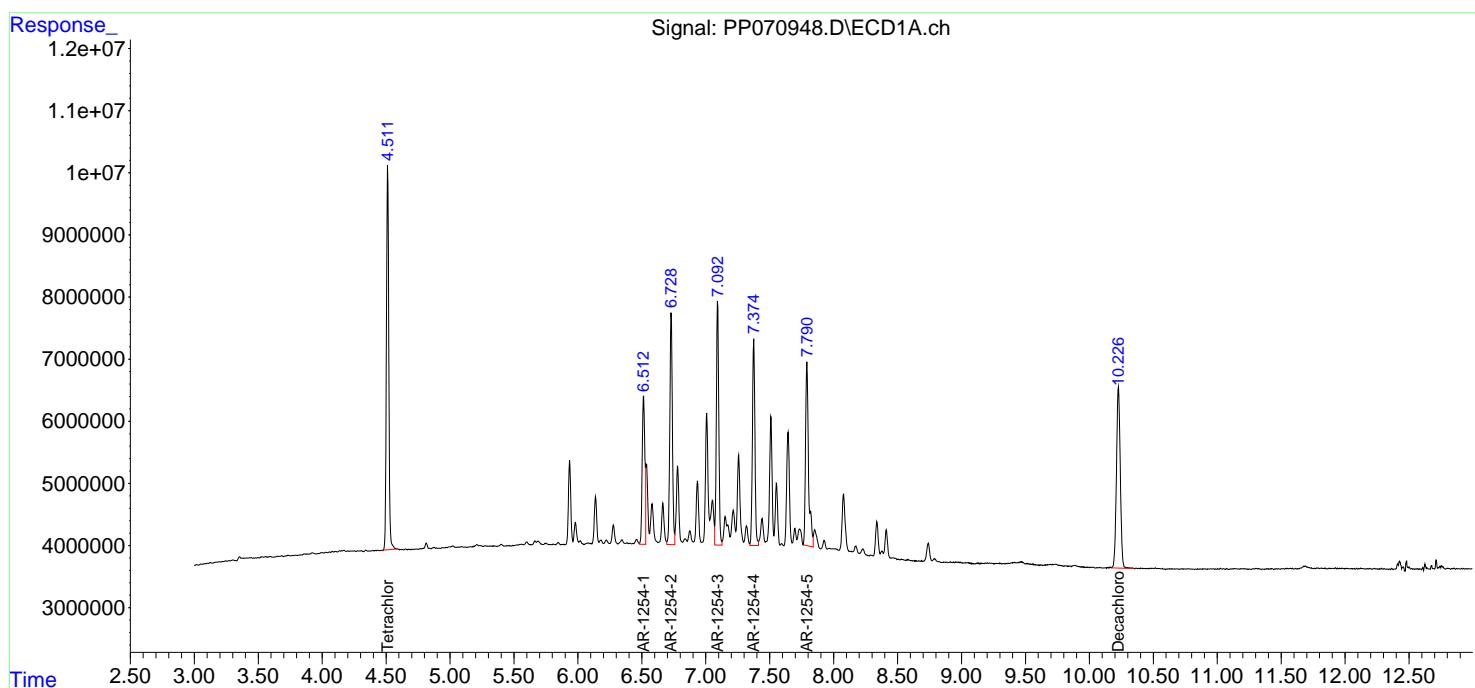




#1 Tetrachloro-m-xylene


R.T.: 4.513 min  
Delta R.T.: -0.001 min  
Response: 80813408  
Conc: 53.47 ng/ml

Instrument: ECD\_P  
ClientSampleId: ICVPP032725AR1254

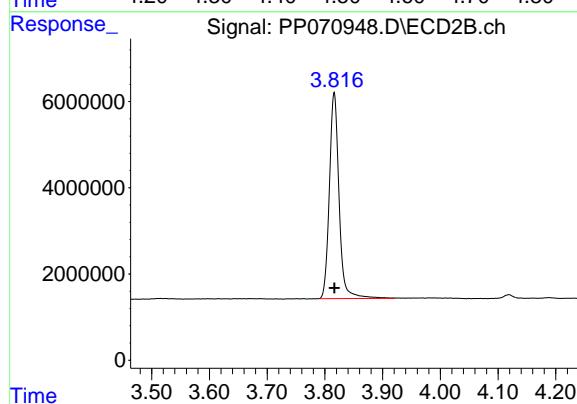


#1 Tetrachloro-m-xylene

R.T.: 3.816 min  
Delta R.T.: 0.000 min  
Response: 55809150  
Conc: 50.69 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.228 min  
Delta R.T.: -0.002 min  
Response: 60442284  
Conc: 53.60 ng/ml

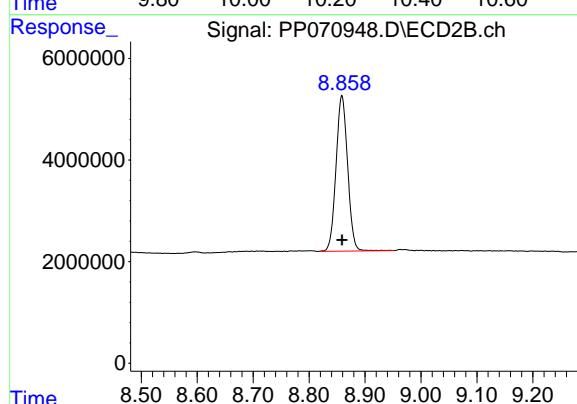

#2 Decachlorobiphenyl

R.T.: 8.859 min  
Delta R.T.: 0.000 min  
Response: 44113864  
Conc: 53.80 ng/ml

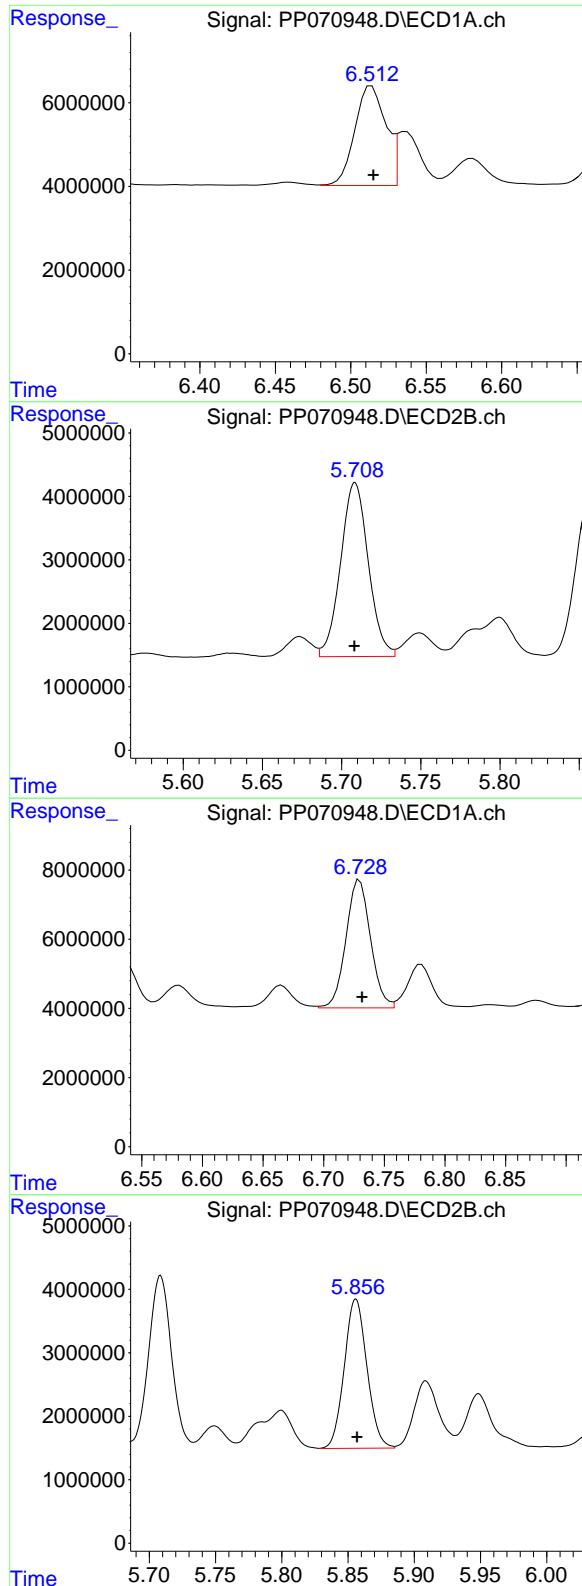

#26 AR-1254-1

R.T.: 6.514 min  
 Delta R.T.: -0.001 min  
 Response: 34026950  
 Conc: 528.45 ng/ml

Instrument: ECD\_P  
 ClientSampleId: ICVPP032725AR1254

#26 AR-1254-1


R.T.: 5.708 min  
 Delta R.T.: 0.000 min  
 Response: 33372474  
 Conc: 505.51 ng/ml

#27 AR-1254-2

R.T.: 6.730 min  
 Delta R.T.: -0.002 min  
 Response: 52171420  
 Conc: 516.09 ng/ml

#27 AR-1254-2

R.T.: 5.856 min  
 Delta R.T.: 0.000 min  
 Response: 28060451  
 Conc: 491.44 ng/ml

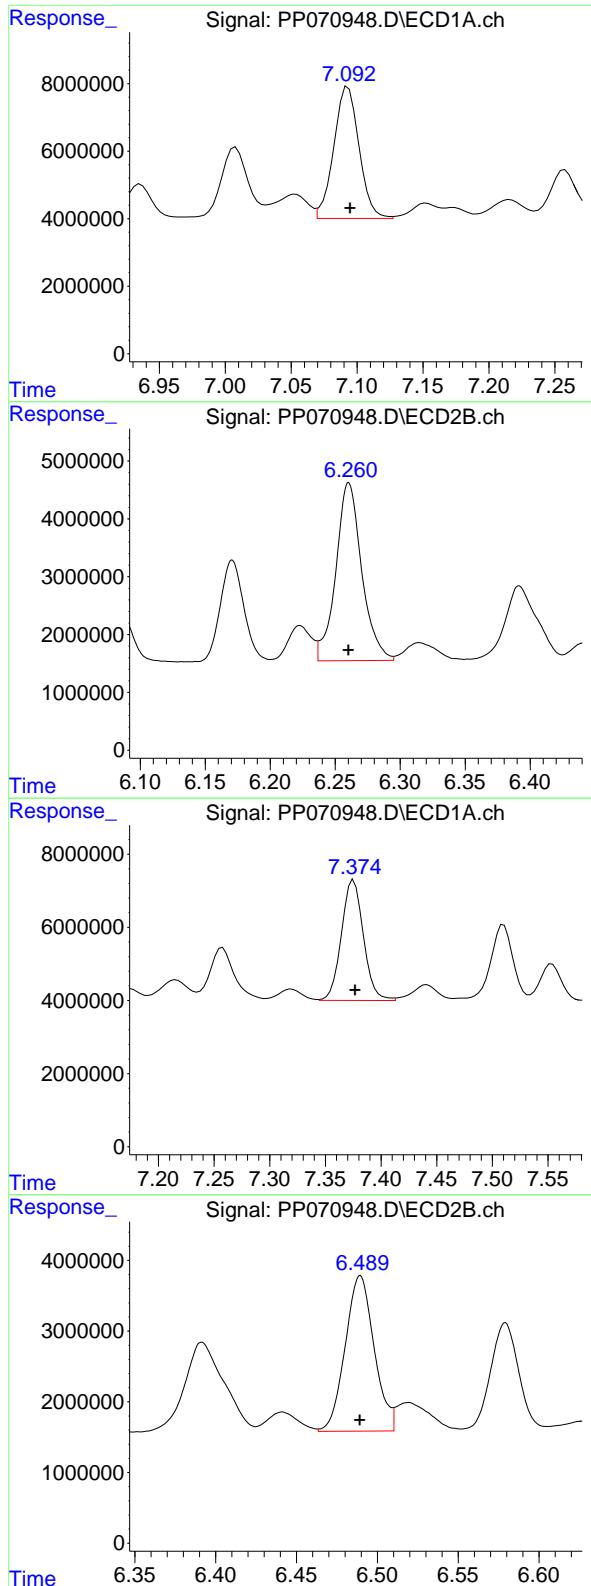

#28 AR-1254-3

R.T.: 7.093 min  
 Delta R.T.: -0.001 min  
 Response: 52059367  
 Conc: 522.01 ng/ml

**Instrument:** ECD\_P  
**ClientSampleId:** ICVPP032725AR1254

#28 AR-1254-3


R.T.: 6.260 min  
 Delta R.T.: 0.000 min  
 Response: 42608413  
 Conc: 490.65 ng/ml

#29 AR-1254-4

R.T.: 7.375 min  
 Delta R.T.: -0.001 min  
 Response: 45346150  
 Conc: 523.65 ng/ml

#29 AR-1254-4

R.T.: 6.489 min  
 Delta R.T.: 0.000 min  
 Response: 27407702  
 Conc: 488.55 ng/ml

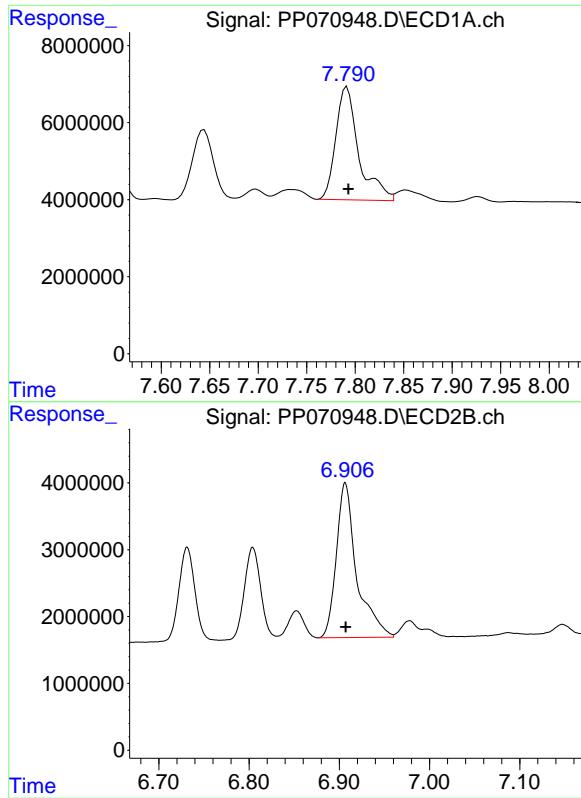

#30 AR-1254-5

R.T.: 7.792 min  
Delta R.T.: -0.001 min  
Response: 48183080  
Conc: 599.66 ng/ml

Instrument: ECD\_P  
ClientSampleId: ICVPP032725AR1254

#30 AR-1254-5

R.T.: 6.907 min  
Delta R.T.: 0.000 min  
Response: 36336253  
Conc: 503.62 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071136.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 09:37  
 Operator : YP\AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:57:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlor...	4.524	3.817	75031562	49693990	51.336	47.937
2) SA Decachlor...	10.255	8.862	53747529	34514110	51.061	43.789

Target Compounds

3) L1 AR-1016-1	5.679	4.904	25640835	19684563	504.232	491.032
4) L1 AR-1016-2	5.679	4.923	25640835	27978272	328.503	483.509 #
5) L1 AR-1016-3	5.763	5.101	23060044	16163902	488.823	522.709
6) L1 AR-1016-4	5.861	5.142	19323906	13212574	525.739	542.479
7) L1 AR-1016-5	6.154	5.357	18307730	17134433	539.858	530.130
8) L2 AR-1221-1	4.723	4.026	24566666	2180640	141.565	143.053
9) L2 AR-1221-2	4.813	4.115	3663977	3206249	282.869	280.357
10) L2 AR-1221-3	4.888	4.191	13293050	11445681	318.646	335.759
11) L3 AR-1232-1	4.888	4.191	13293050	11445681	399.326	408.969
12) L3 AR-1232-2	5.414	4.923	18281252	27978272	1149.017	997.047
13) L3 AR-1232-3	5.701	5.101	38706585	16163902	1129.447	1085.584
14) L3 AR-1232-4	5.861	5.185	19323906	15635898	1230.228	1221.138
15) L3 AR-1232-5	5.951	5.357	15905498	17134433	1494.828	1208.797
16) L4 AR-1242-1	5.679	4.904	25640835	19684563	583.049	575.642
17) L4 AR-1242-2	5.679	4.923	25640835	27978272	398.668	567.998 #
18) L4 AR-1242-3	5.763	5.101	23060044	16163902	561.899	606.656
19) L4 AR-1242-4	5.861	5.185	19323906	15635898	633.086	592.757
20) L4 AR-1242-5	6.592	5.710	6855876	16691995	187.779	539.177 #
21) L5 AR-1248-1	5.679	4.904	25640835	19684563	706.602	726.905
22) L5 AR-1248-2	5.951	5.142	15905498	13212574	353.939	359.795
23) L5 AR-1248-3	6.154	5.185	18307730	15635898	361.545	404.453
24) L5 AR-1248-4	6.528	5.357	18184937	17134433	283.486	379.576 #
25) L5 AR-1248-5	6.592	5.750	6855876	4488455	112.675	105.168
26) L6 AR-1254-1	6.528	5.710	18184937	16691995	282.418	252.841
27) L6 AR-1254-2	6.745	5.858	16493060	11838446	163.151	207.335 #
28) L6 AR-1254-3	7.109	6.244	8745572	4764413	87.694	54.863 #
29) L6 AR-1254-4	7.392	6.491	6515054	3701399	75.234	65.978
30) L6 AR-1254-5	7.807	6.908	49428901	33433766	615.162	463.388
31) L7 AR-1260-1	7.273	6.393	34786874	28041460	518.026	547.617
32) L7 AR-1260-2	7.527	6.582	51604417	34095263	536.784	534.460
33) L7 AR-1260-3	7.885	6.735	40227656	29796945	503.360	546.865
34) L7 AR-1260-4	8.076	7.207	7015115	23421548	89.096	489.721 #
35) L7 AR-1260-5	8.431	7.448	80513512	57532352	506.737	462.069
36) L8 AR-1262-1	8.076	6.947	7015115	28743067	65.993	335.927 #
37) L8 AR-1262-2	8.431	7.207	80513512	23421548	405.849	342.098
38) L8 AR-1262-3	8.756	7.730	49500185	13610298	375.736	224.136 #
39) L8 AR-1262-4	8.835	7.794	29791065	37704999	311.574	379.300
40) L8 AR-1262-5	9.493	8.296	21754078	14122672	334.337	301.305
41) L9 AR-1268-1	8.756	7.730	49500185	13610298	210.185	79.406 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071136.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 09:37  
 Operator : YP\AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_P**  
**ClientSampleId :**  
**AR1660CCC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:57:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9 AR-1268-2	8.835	7.794	29791065	37704999	152.528	263.151 #
43) L9 AR-1268-3	9.071	8.001	324667	608932	1.900	4.945 #
44) L9 AR-1268-4	9.493	8.296	21754078	14122672	307.490	267.408
45) L9 AR-1268-5	9.911	8.598	5287089	3490210	11.103	9.645



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP040825\  
 Data File : PP071136.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Apr 2025 09:37  
 Operator : YP\AJ  
 Sample : AR1660CCC500  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 AR1660CCC500

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 08 10:57:00 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP032725.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 28 03:13:46 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50 $\mu$  Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

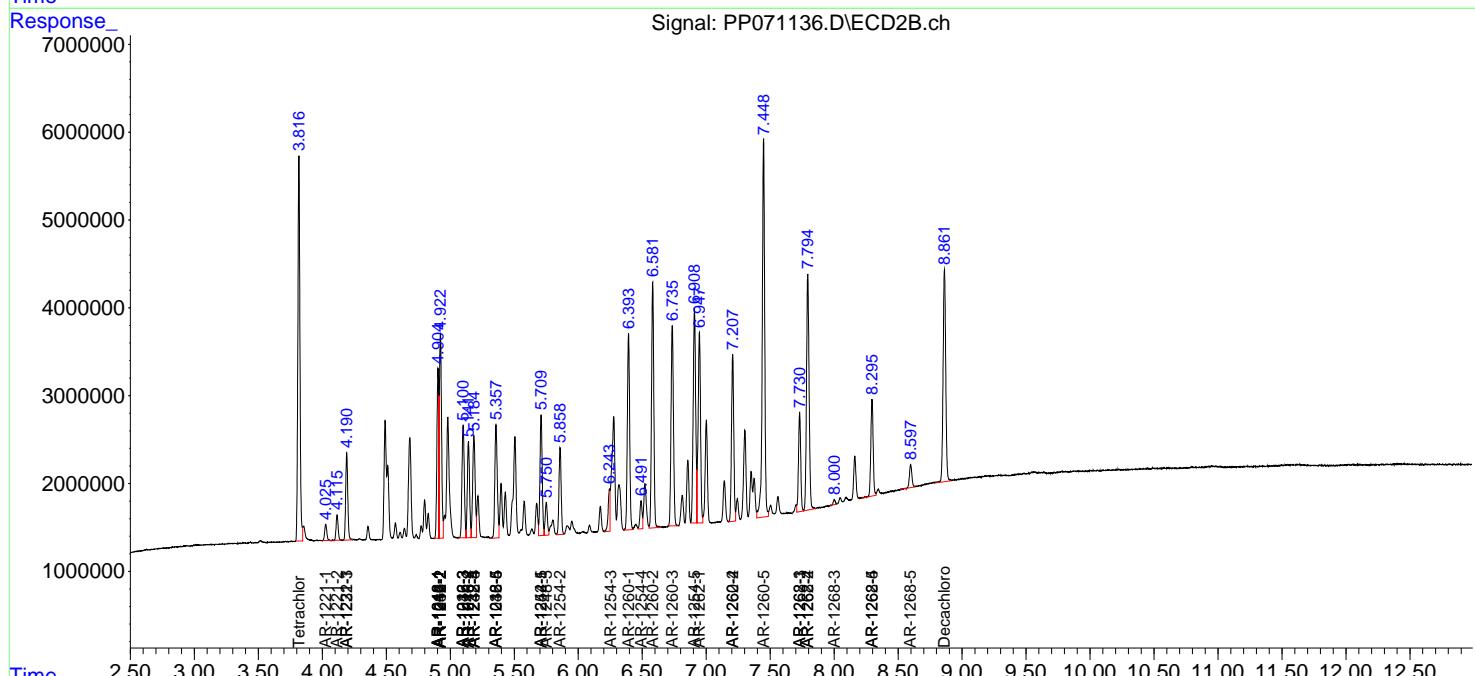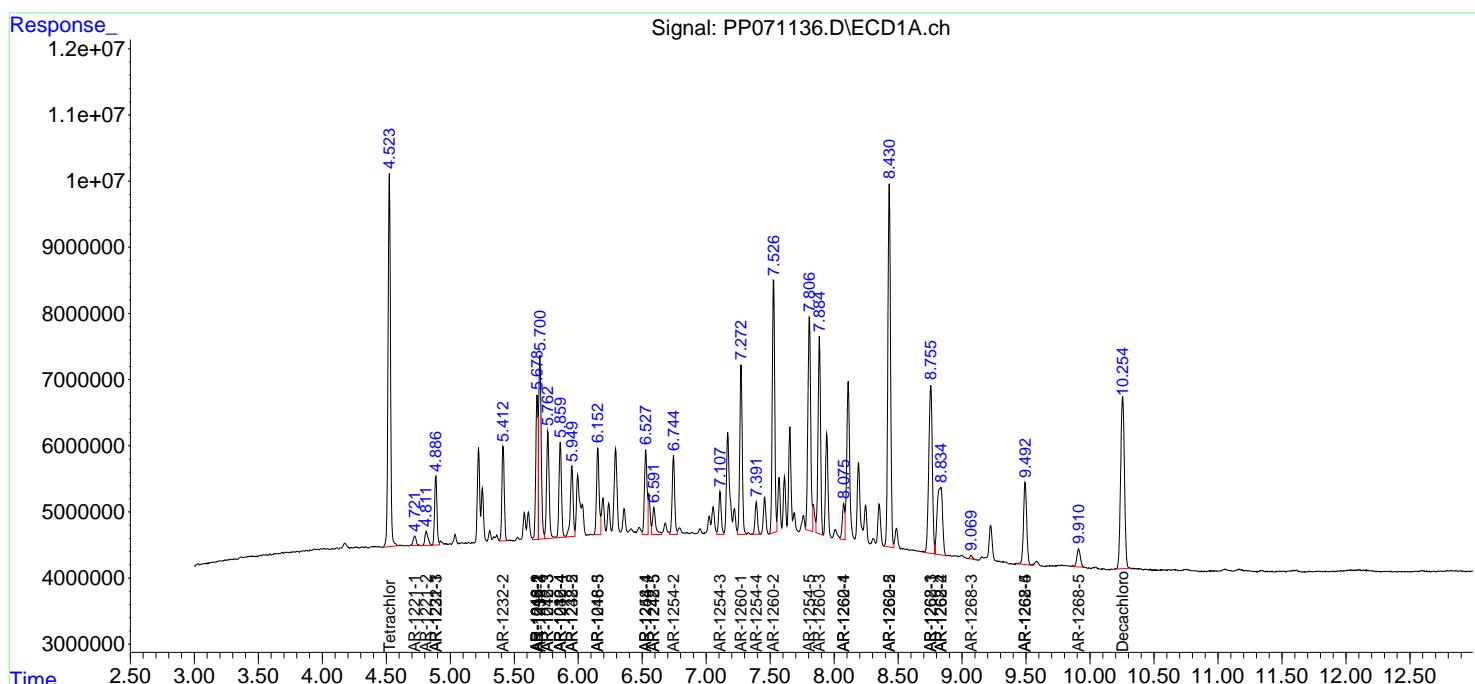

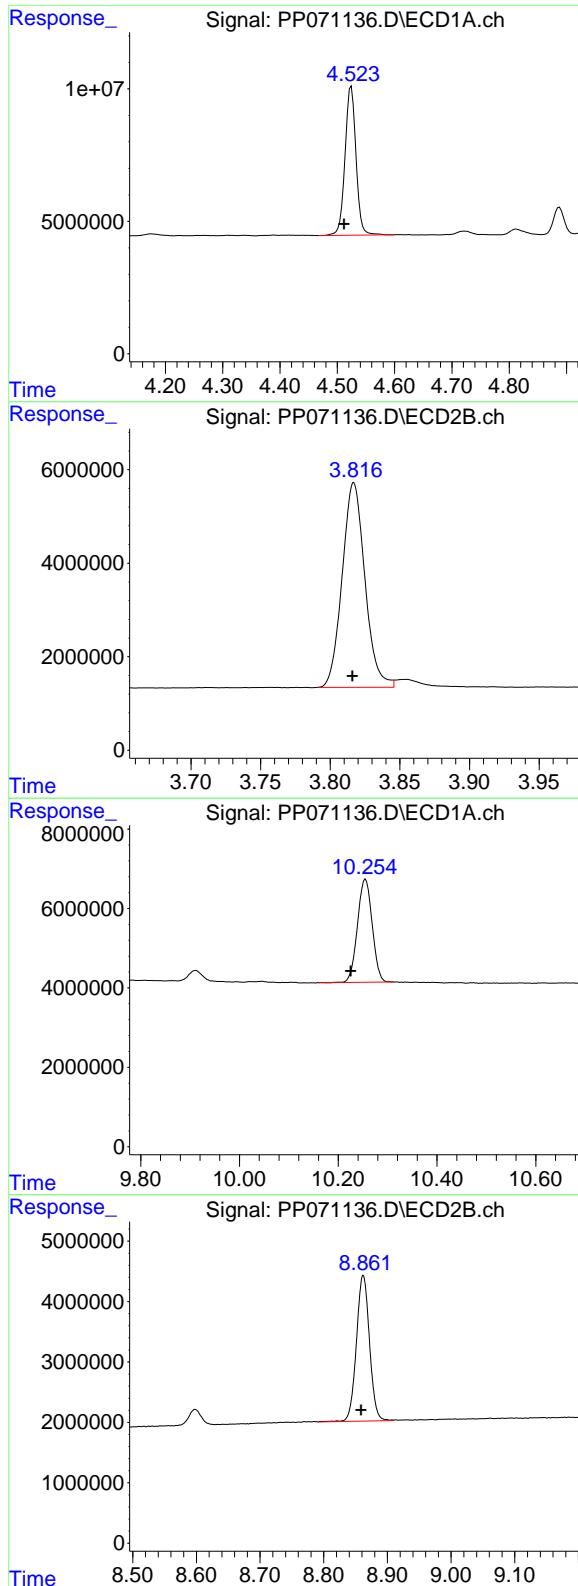

### #1 Tetrachloro-m-xylene

R.T.: 4.524 min  
 Delta R.T.: 0.012 min  
 Response: 75031562  
 Conc: 51.34 ng/ml

Instrument:

ECD\_P

ClientSampleId :

AR1660CCC500

### #1 Tetrachloro-m-xylene


R.T.: 3.817 min  
 Delta R.T.: 0.000 min  
 Response: 49693990  
 Conc: 47.94 ng/ml

### #2 Decachlorobiphenyl

R.T.: 10.255 min  
 Delta R.T.: 0.030 min  
 Response: 53747529  
 Conc: 51.06 ng/ml

### #2 Decachlorobiphenyl


R.T.: 8.862 min  
 Delta R.T.: 0.003 min  
 Response: 34514110  
 Conc: 43.79 ng/ml

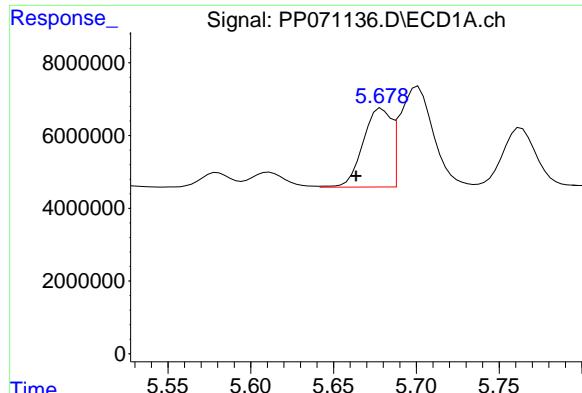

#3 AR-1016-1


R.T.: 5.679 min  
 Delta R.T.: 0.016 min  
 Response: 25640835  
 Conc: 504.23 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

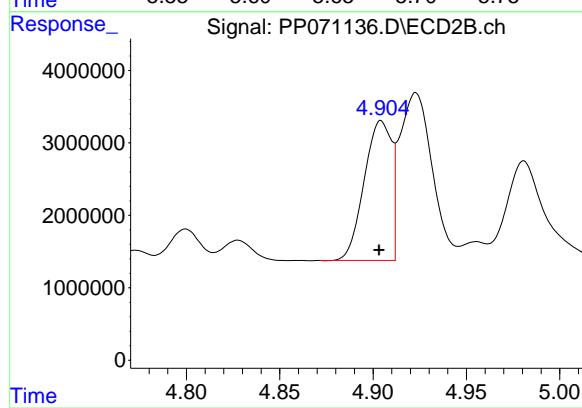


#3 AR-1016-1

R.T.: 4.904 min  
 Delta R.T.: 0.001 min  
 Response: 19684563  
 Conc: 491.03 ng/ml

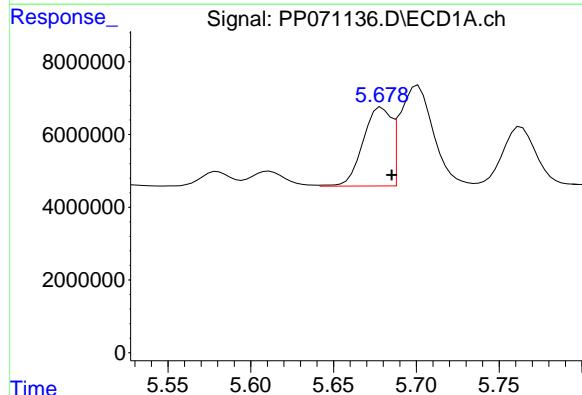


#4 AR-1016-2

R.T.: 5.679 min  
 Delta R.T.: -0.006 min  
 Response: 25640835  
 Conc: 328.50 ng/ml

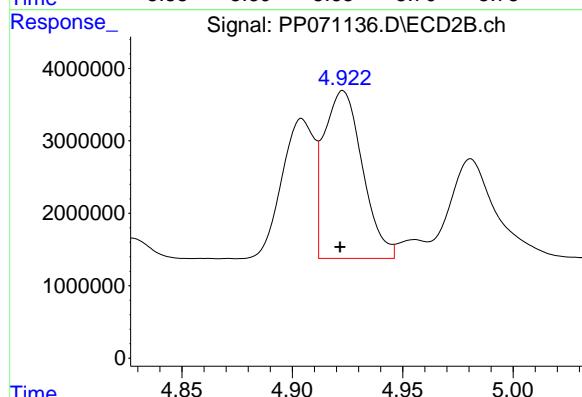

#4 AR-1016-2


R.T.: 4.923 min  
 Delta R.T.: 0.001 min  
 Response: 27978272  
 Conc: 483.51 ng/ml

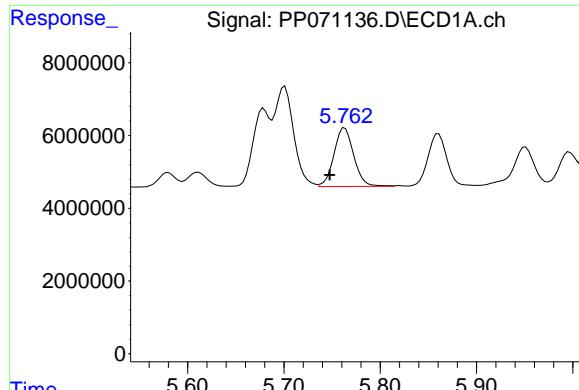

#5 AR-1016-3


R.T.: 5.763 min  
 Delta R.T.: 0.016 min  
 Response: 23060044  
 Conc: 488.82 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

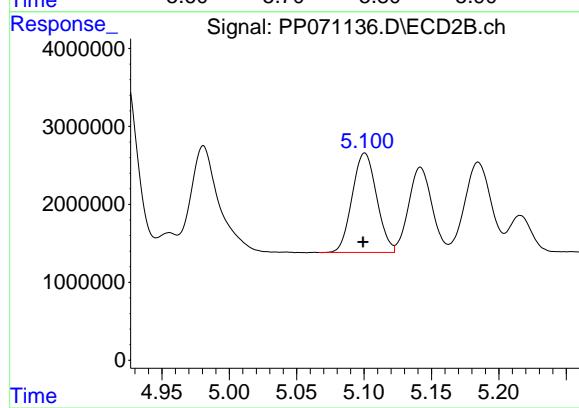


#5 AR-1016-3

R.T.: 5.101 min  
 Delta R.T.: 0.001 min  
 Response: 16163902  
 Conc: 522.71 ng/ml

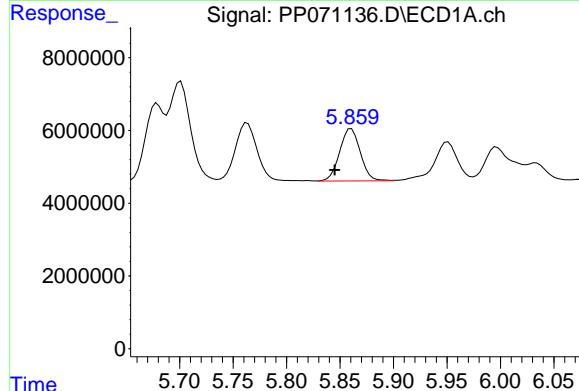


#6 AR-1016-4

R.T.: 5.861 min  
 Delta R.T.: 0.015 min  
 Response: 19323906  
 Conc: 525.74 ng/ml

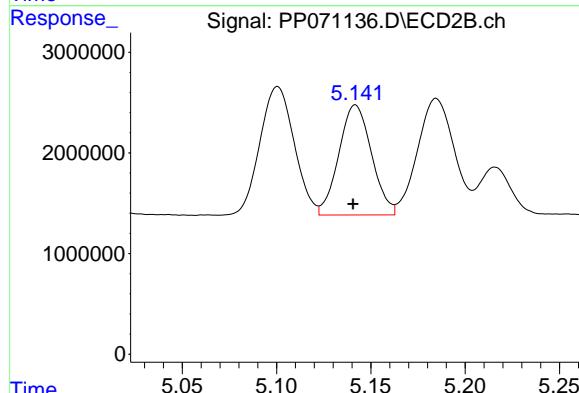

#6 AR-1016-4

R.T.: 5.142 min  
 Delta R.T.: 0.001 min  
 Response: 13212574  
 Conc: 542.48 ng/ml

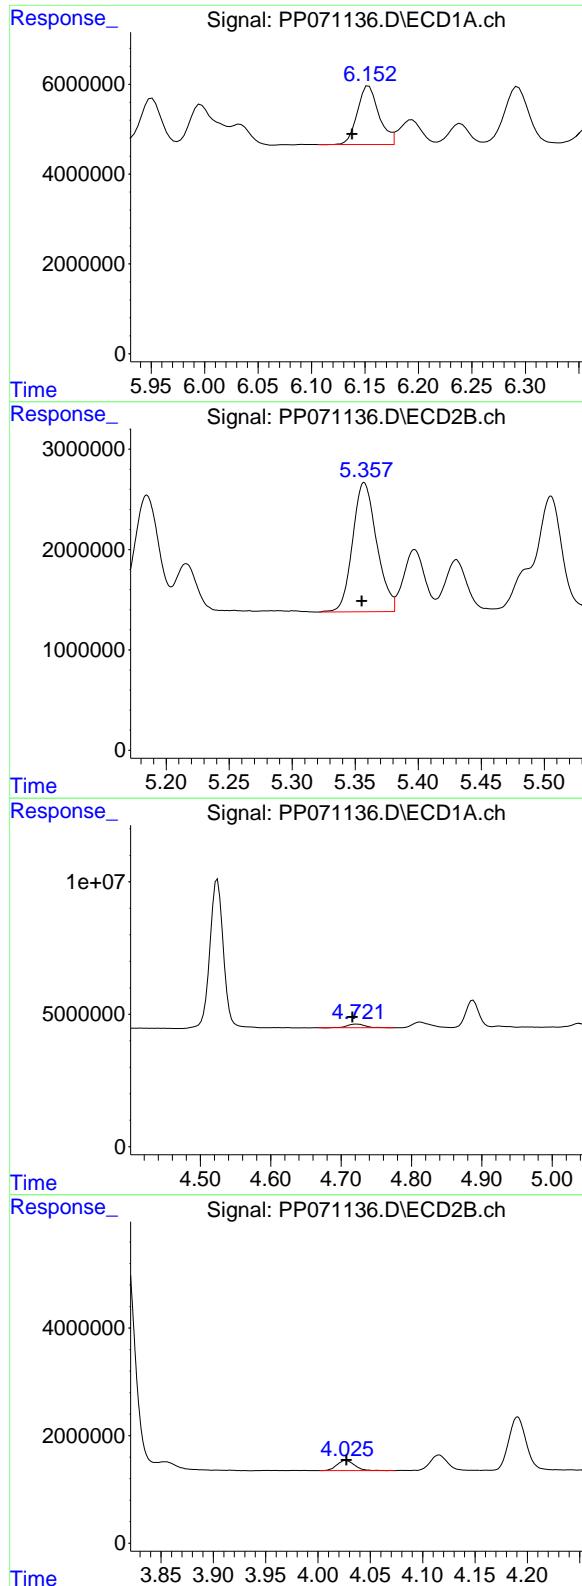

#7 AR-1016-5

R.T.: 6.154 min  
 Delta R.T.: 0.016 min  
 Response: 18307730  
 Conc: 539.86 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#7 AR-1016-5


R.T.: 5.357 min  
 Delta R.T.: 0.002 min  
 Response: 17134433  
 Conc: 530.13 ng/ml

#8 AR-1221-1

R.T.: 4.723 min  
 Delta R.T.: 0.007 min  
 Response: 2456666  
 Conc: 141.56 ng/ml

#8 AR-1221-1

R.T.: 4.026 min  
 Delta R.T.: 0.000 min  
 Response: 2180640  
 Conc: 143.05 ng/ml

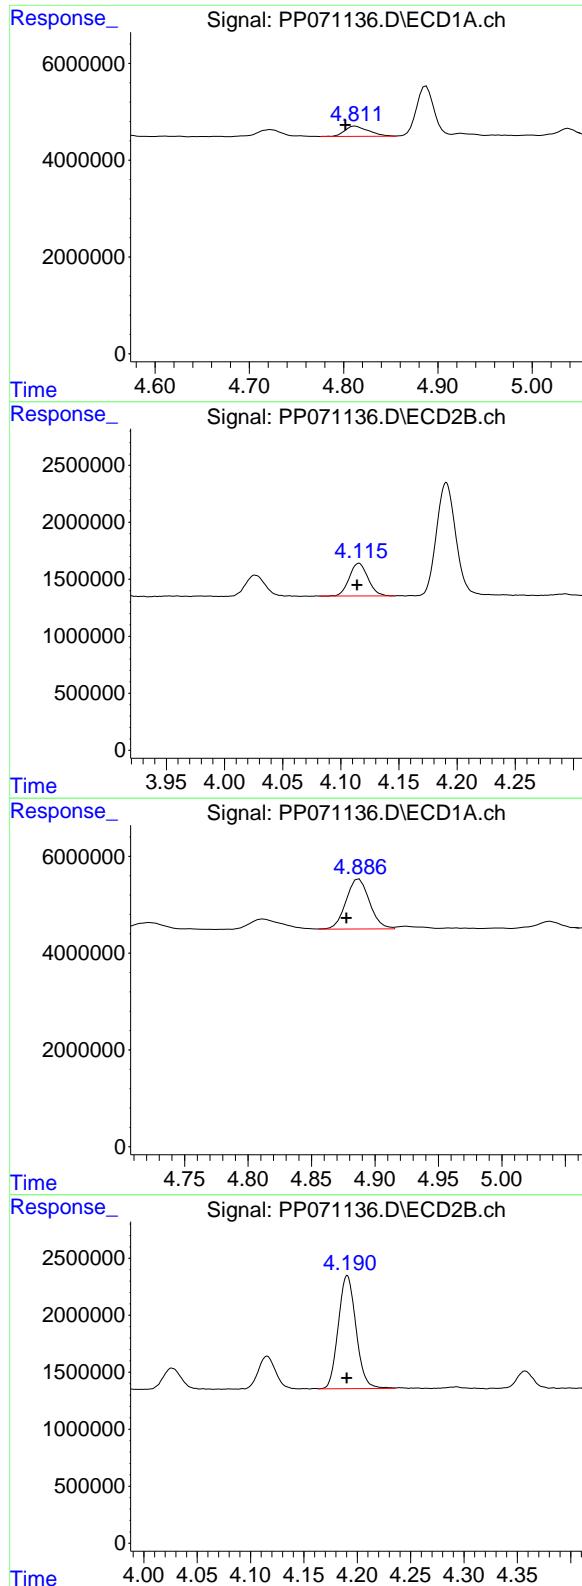

#9 AR-1221-2

R.T.: 4.813 min  
 Delta R.T.: 0.010 min  
 Response: 3663977  
 Conc: 282.87 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#9 AR-1221-2


R.T.: 4.115 min  
 Delta R.T.: 0.001 min  
 Response: 3206249  
 Conc: 280.36 ng/ml

#10 AR-1221-3

R.T.: 4.888 min  
 Delta R.T.: 0.010 min  
 Response: 13293050  
 Conc: 318.65 ng/ml

#10 AR-1221-3


R.T.: 4.191 min  
 Delta R.T.: 0.000 min  
 Response: 11445681  
 Conc: 335.76 ng/ml



#11 AR-1232-1


R.T.: 4.888 min  
Delta R.T.: 0.005 min  
Response: 13293050  
Conc: 399.33 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660CCC500

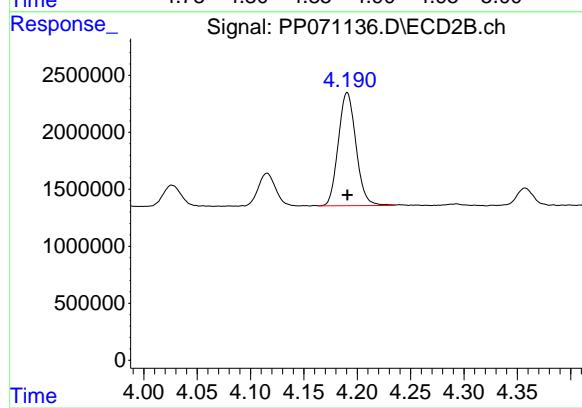


#11 AR-1232-1

R.T.: 4.191 min  
Delta R.T.: 0.000 min  
Response: 11445681  
Conc: 408.97 ng/ml

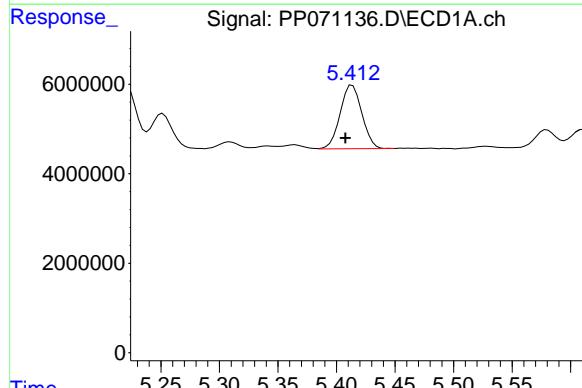


#12 AR-1232-2

R.T.: 5.414 min  
Delta R.T.: 0.006 min  
Response: 18281252  
Conc: 1149.02 ng/ml

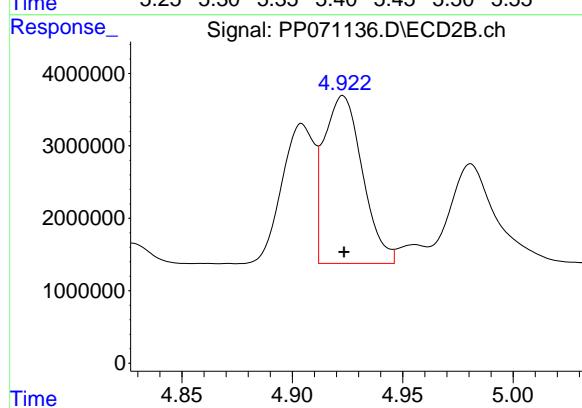

#12 AR-1232-2


R.T.: 4.923 min  
Delta R.T.: 0.000 min  
Response: 27978272  
Conc: 997.05 ng/ml

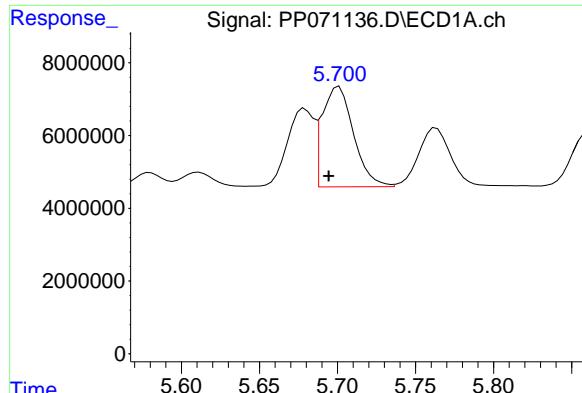

#13 AR-1232-3


R.T.: 5.701 min  
 Delta R.T.: 0.007 min  
 Response: 38706585  
 Conc: 1129.45 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

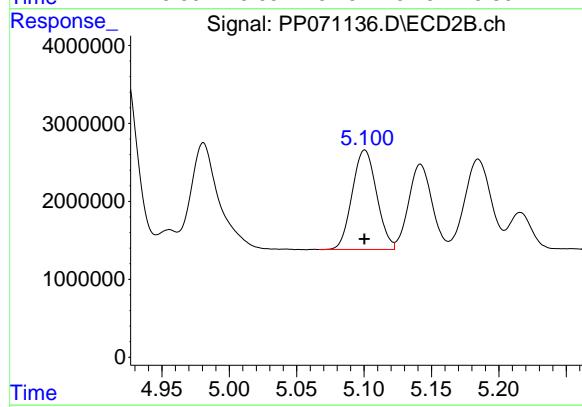


#13 AR-1232-3

R.T.: 5.101 min  
 Delta R.T.: 0.000 min  
 Response: 16163902  
 Conc: 1085.58 ng/ml

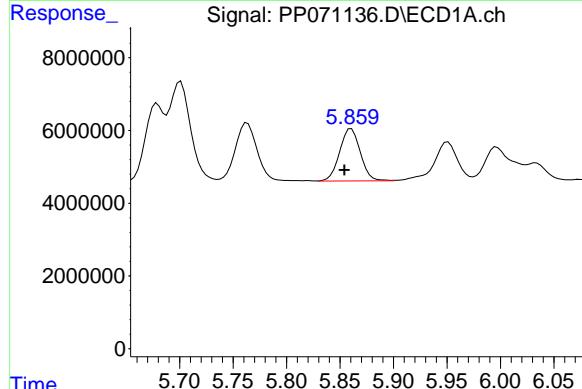


#14 AR-1232-4

R.T.: 5.861 min  
 Delta R.T.: 0.007 min  
 Response: 19323906  
 Conc: 1230.23 ng/ml

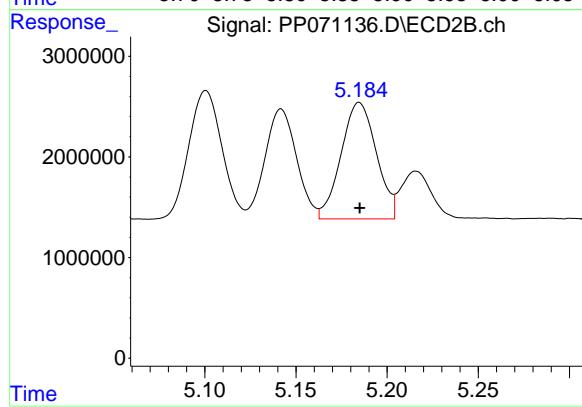

#14 AR-1232-4


R.T.: 5.185 min  
 Delta R.T.: 0.000 min  
 Response: 15635898  
 Conc: 1221.14 ng/ml

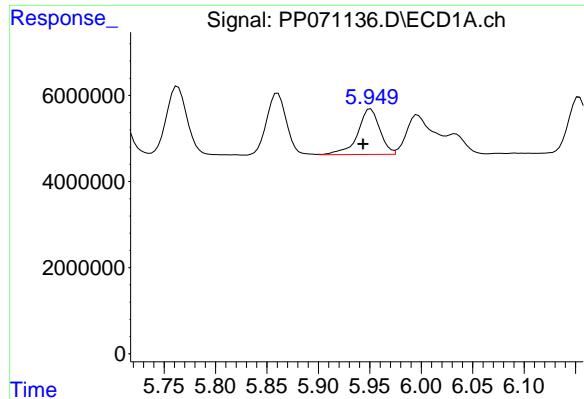

#15 AR-1232-5


R.T.: 5.951 min  
 Delta R.T.: 0.008 min  
 Response: 15905498  
 Conc: 1494.83 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

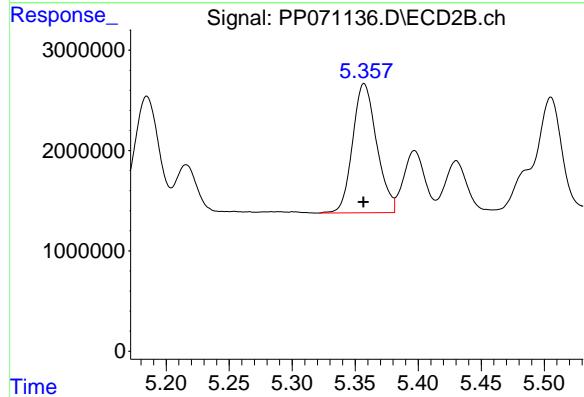


#15 AR-1232-5

R.T.: 5.357 min  
 Delta R.T.: 0.000 min  
 Response: 17134433  
 Conc: 1208.80 ng/ml

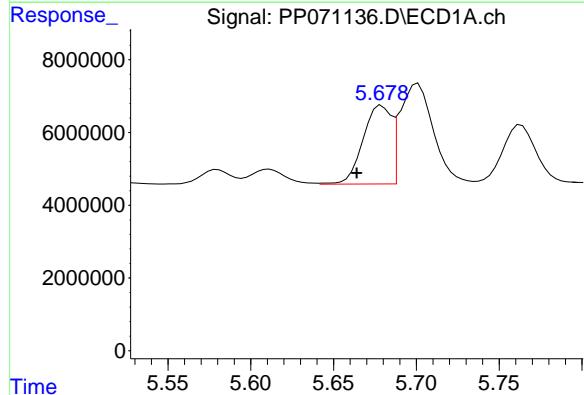


#16 AR-1242-1

R.T.: 5.679 min  
 Delta R.T.: 0.015 min  
 Response: 25640835  
 Conc: 583.05 ng/ml

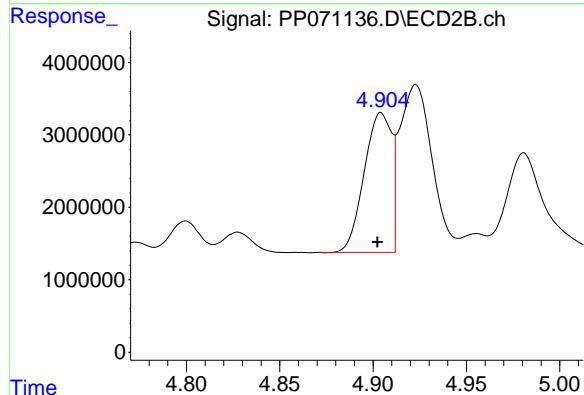

#16 AR-1242-1


R.T.: 4.904 min  
 Delta R.T.: 0.002 min  
 Response: 19684563  
 Conc: 575.64 ng/ml

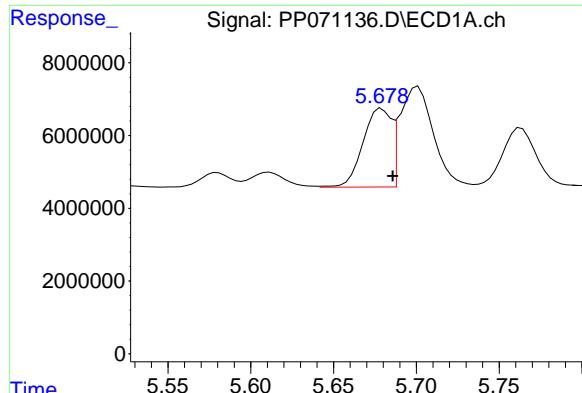

#17 AR-1242-2


R.T.: 5.679 min  
 Delta R.T.: -0.007 min  
 Response: 25640835  
 Conc: 398.67 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

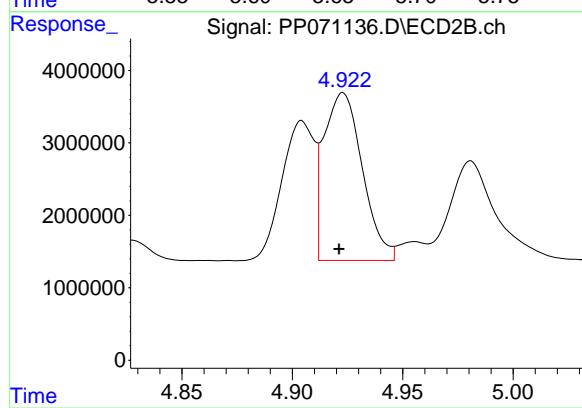


#17 AR-1242-2

R.T.: 4.923 min  
 Delta R.T.: 0.002 min  
 Response: 27978272  
 Conc: 568.00 ng/ml

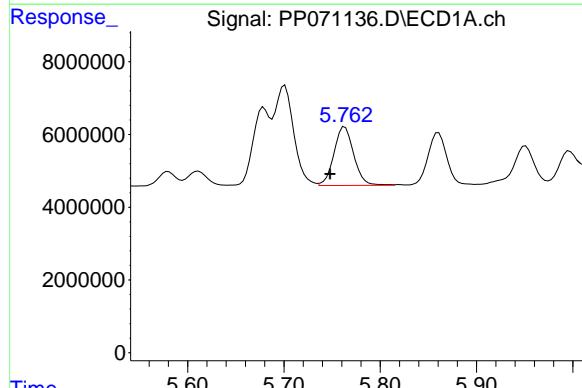


#18 AR-1242-3

R.T.: 5.763 min  
 Delta R.T.: 0.015 min  
 Response: 23060044  
 Conc: 561.90 ng/ml

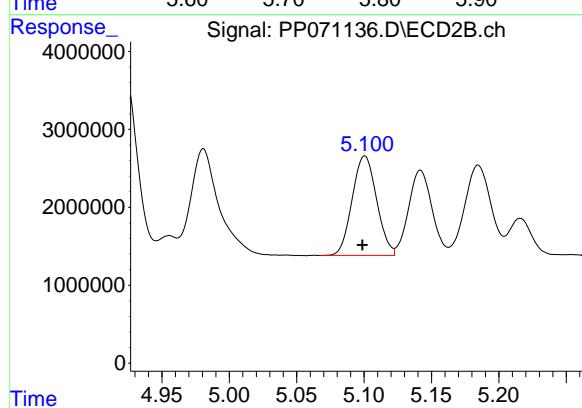

#18 AR-1242-3

R.T.: 5.101 min  
 Delta R.T.: 0.002 min  
 Response: 16163902  
 Conc: 606.66 ng/ml

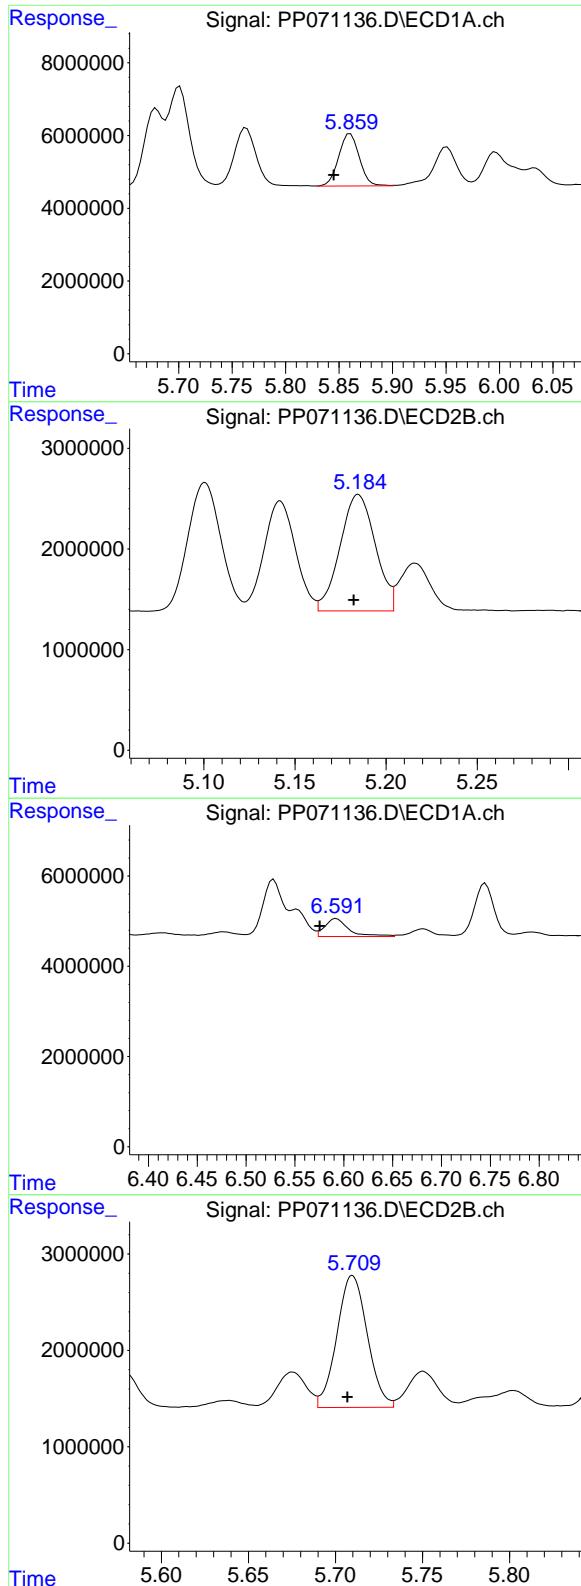

#19 AR-1242-4

R.T.: 5.861 min  
Delta R.T.: 0.015 min  
Response: 19323906  
Conc: 633.09 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660CCC500

#19 AR-1242-4


R.T.: 5.185 min  
Delta R.T.: 0.003 min  
Response: 15635898  
Conc: 592.76 ng/ml

#20 AR-1242-5

R.T.: 6.592 min  
Delta R.T.: 0.017 min  
Response: 6855876  
Conc: 187.78 ng/ml

#20 AR-1242-5


R.T.: 5.710 min  
Delta R.T.: 0.003 min  
Response: 16691995  
Conc: 539.18 ng/ml

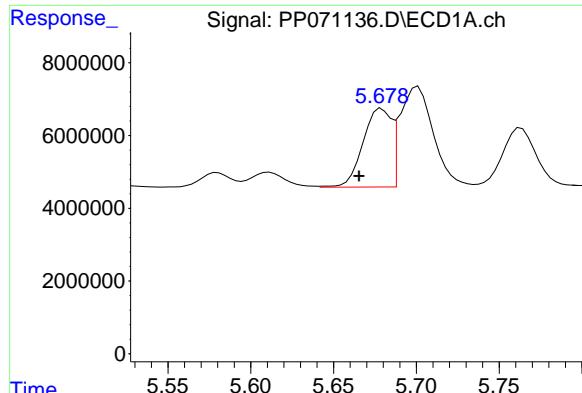

#21 AR-1248-1

R.T.: 5.679 min  
 Delta R.T.: 0.014 min  
 Response: 25640835  
 Conc: 706.60 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

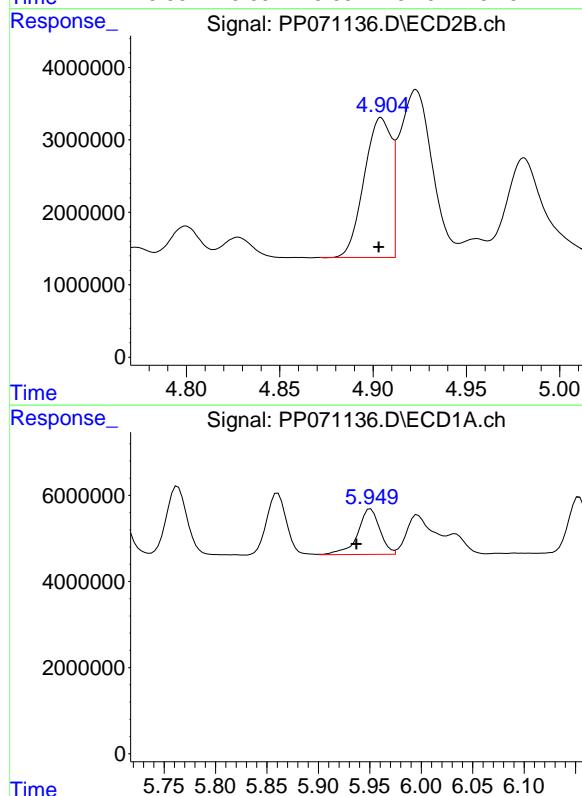


#22 AR-1248-2

R.T.: 5.951 min  
 Delta R.T.: 0.014 min  
 Response: 15905498  
 Conc: 353.94 ng/ml

#22 AR-1248-2

R.T.: 5.142 min  
 Delta R.T.: 0.002 min  
 Response: 13212574  
 Conc: 359.80 ng/ml

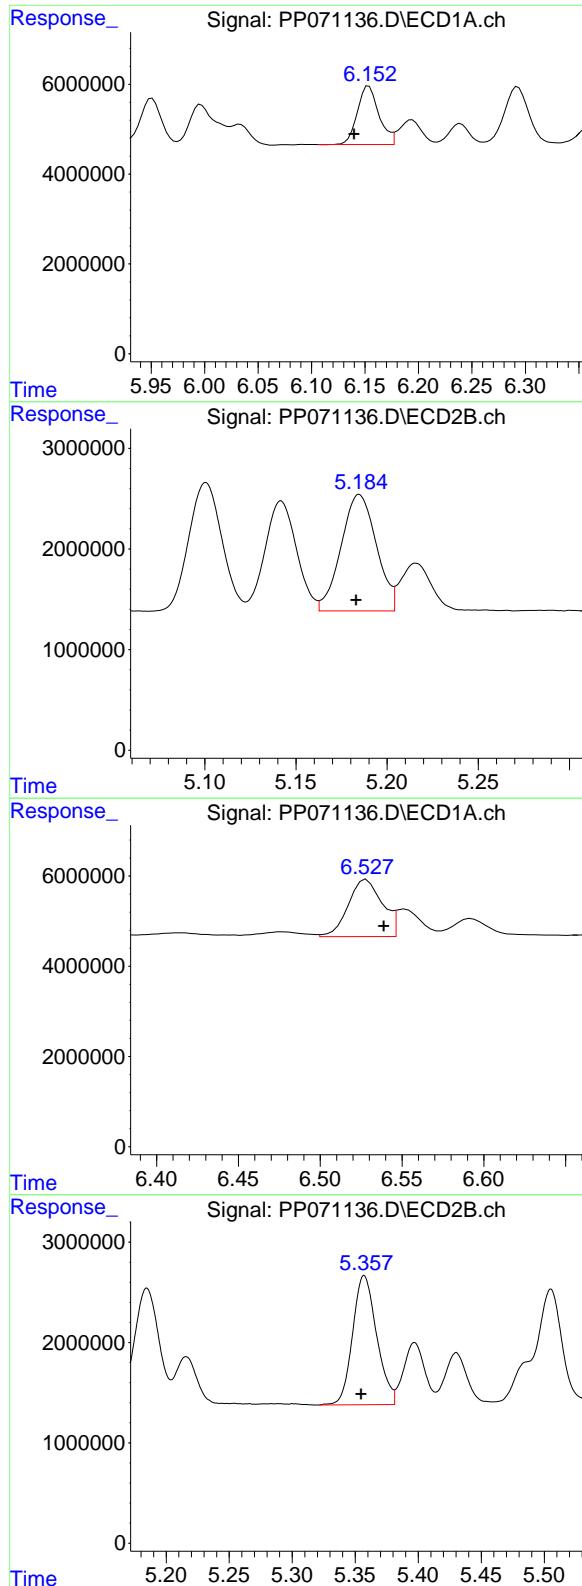

#23 AR-1248-3

R.T.: 6.154 min  
 Delta R.T.: 0.014 min  
 Response: 18307730  
 Conc: 361.54 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#23 AR-1248-3


R.T.: 5.185 min  
 Delta R.T.: 0.002 min  
 Response: 15635898  
 Conc: 404.45 ng/ml

#24 AR-1248-4

R.T.: 6.528 min  
 Delta R.T.: -0.010 min  
 Response: 18184937  
 Conc: 283.49 ng/ml

#24 AR-1248-4

R.T.: 5.357 min  
 Delta R.T.: 0.002 min  
 Response: 17134433  
 Conc: 379.58 ng/ml

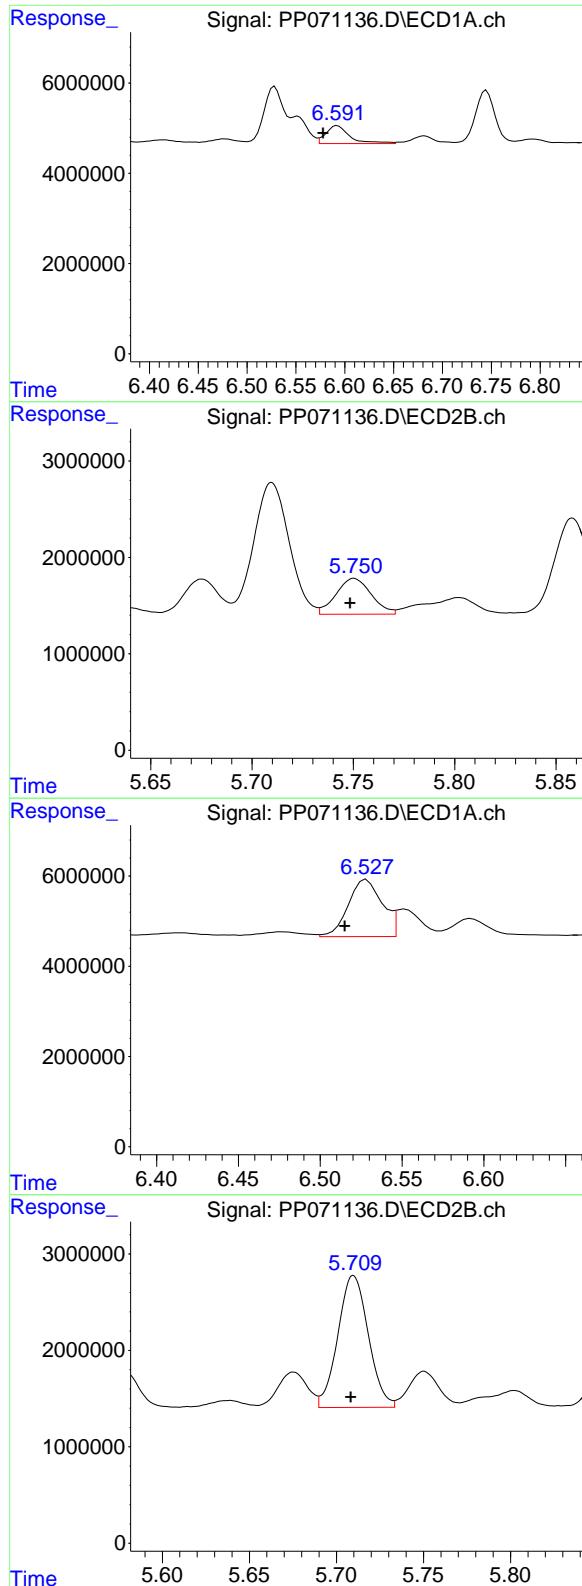

#25 AR-1248-5

R.T.: 6.592 min  
 Delta R.T.: 0.015 min  
 Response: 6855876  
 Conc: 112.68 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#25 AR-1248-5


R.T.: 5.750 min  
 Delta R.T.: 0.002 min  
 Response: 4488455  
 Conc: 105.17 ng/ml

#26 AR-1254-1

R.T.: 6.528 min  
 Delta R.T.: 0.013 min  
 Response: 18184937  
 Conc: 282.42 ng/ml

#26 AR-1254-1


R.T.: 5.710 min  
 Delta R.T.: 0.002 min  
 Response: 16691995  
 Conc: 252.84 ng/ml



#27 AR-1254-2


R.T.: 6.745 min  
Delta R.T.: 0.013 min  
Response: 16493060  
Conc: 163.15 ng/ml

Instrument: ECD\_P  
ClientSampleId: AR1660CCC500

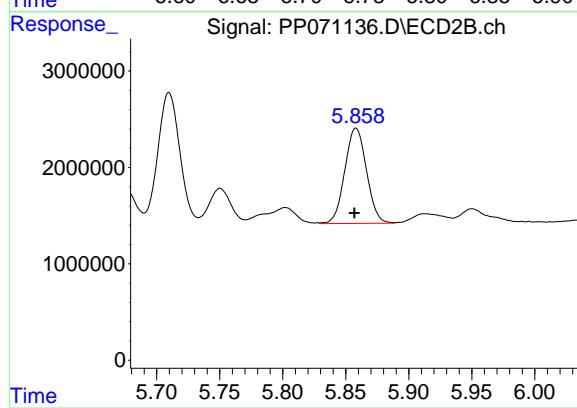


#27 AR-1254-2

R.T.: 5.858 min  
Delta R.T.: 0.001 min  
Response: 11838446  
Conc: 207.34 ng/ml

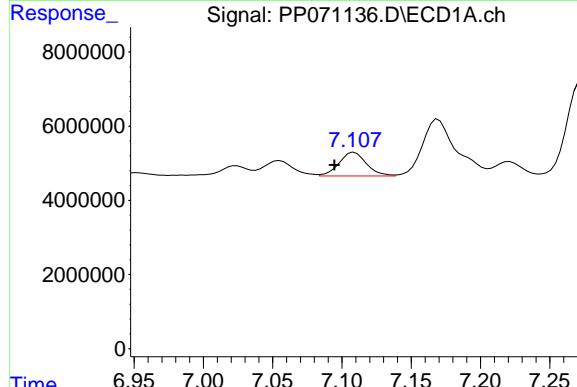


#28 AR-1254-3

R.T.: 7.109 min  
Delta R.T.: 0.014 min  
Response: 8745572  
Conc: 87.69 ng/ml

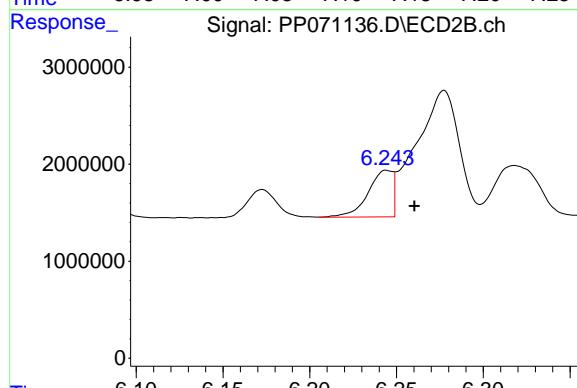

#28 AR-1254-3

R.T.: 6.244 min  
Delta R.T.: -0.016 min  
Response: 4764413  
Conc: 54.86 ng/ml

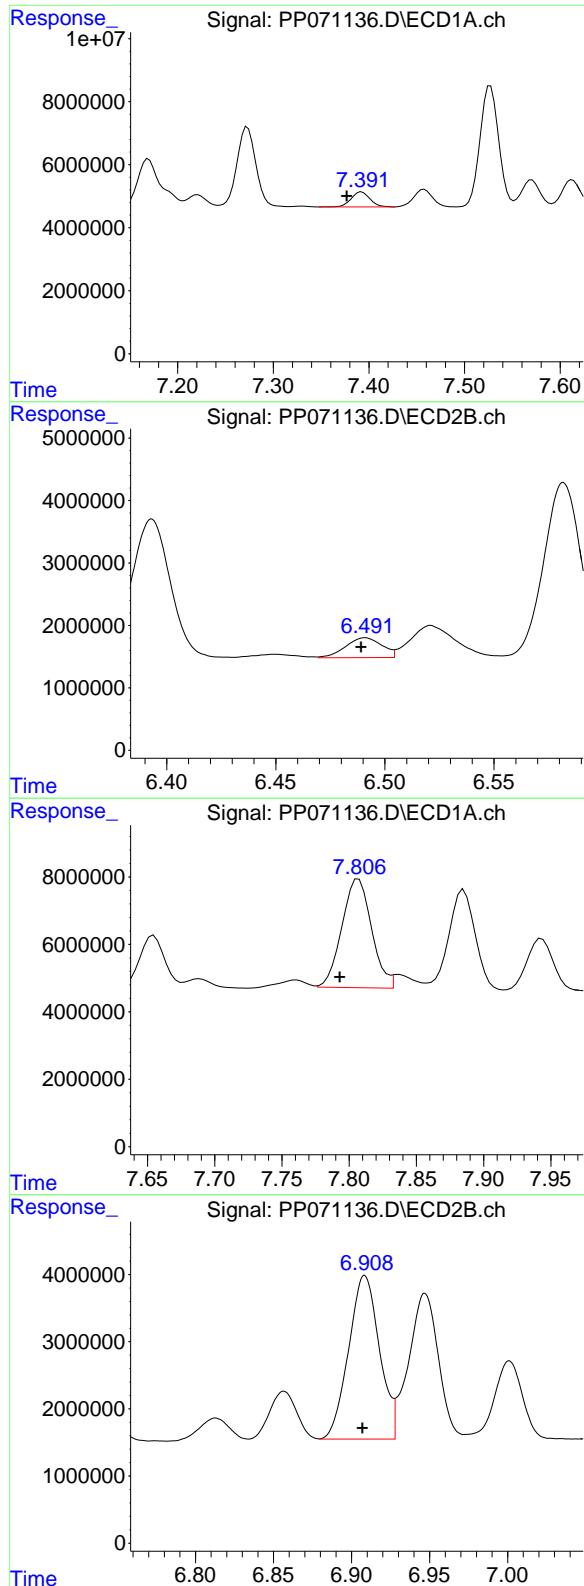

#29 AR-1254-4

R.T.: 7.392 min  
 Delta R.T.: 0.015 min  
 Response: 6515054  
 Conc: 75.23 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#29 AR-1254-4


R.T.: 6.491 min  
 Delta R.T.: 0.002 min  
 Response: 3701399  
 Conc: 65.98 ng/ml

#30 AR-1254-5

R.T.: 7.807 min  
 Delta R.T.: 0.014 min  
 Response: 49428901  
 Conc: 615.16 ng/ml

#30 AR-1254-5


R.T.: 6.908 min  
 Delta R.T.: 0.001 min  
 Response: 33433766  
 Conc: 463.39 ng/ml



#31 AR-1260-1


R.T.: 7.273 min  
 Delta R.T.: 0.017 min  
 Response: 34786874  
 Conc: 518.03 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

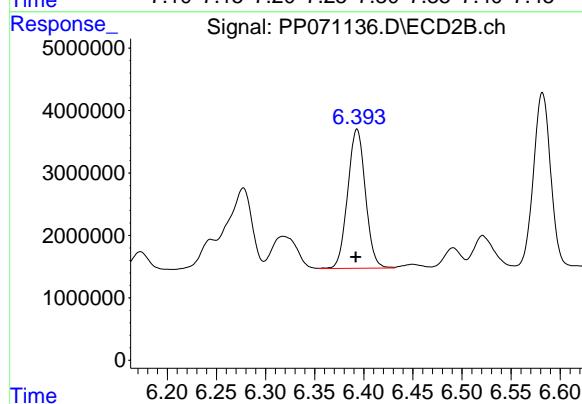


#31 AR-1260-1

R.T.: 6.393 min  
 Delta R.T.: 0.001 min  
 Response: 28041460  
 Conc: 547.62 ng/ml

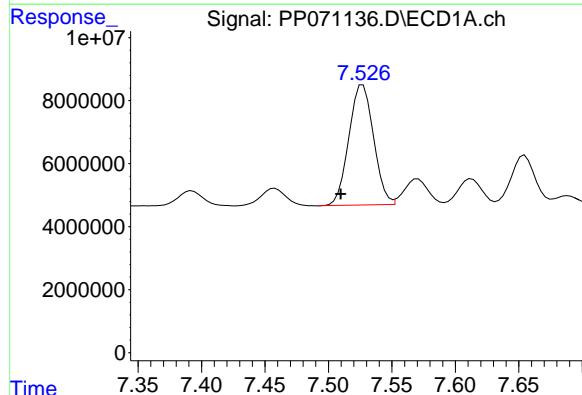


#32 AR-1260-2

R.T.: 7.527 min  
 Delta R.T.: 0.017 min  
 Response: 51604417  
 Conc: 536.78 ng/ml

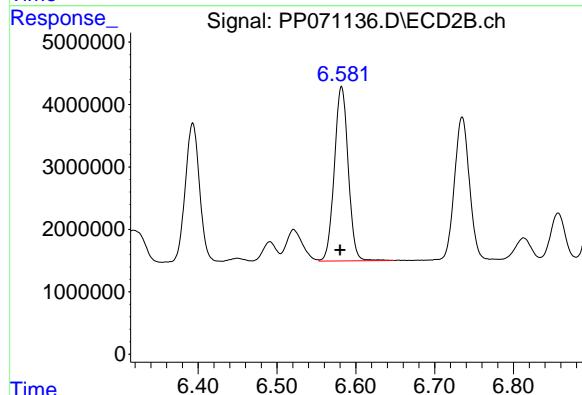

#32 AR-1260-2

R.T.: 6.582 min  
 Delta R.T.: 0.002 min  
 Response: 34095263  
 Conc: 534.46 ng/ml

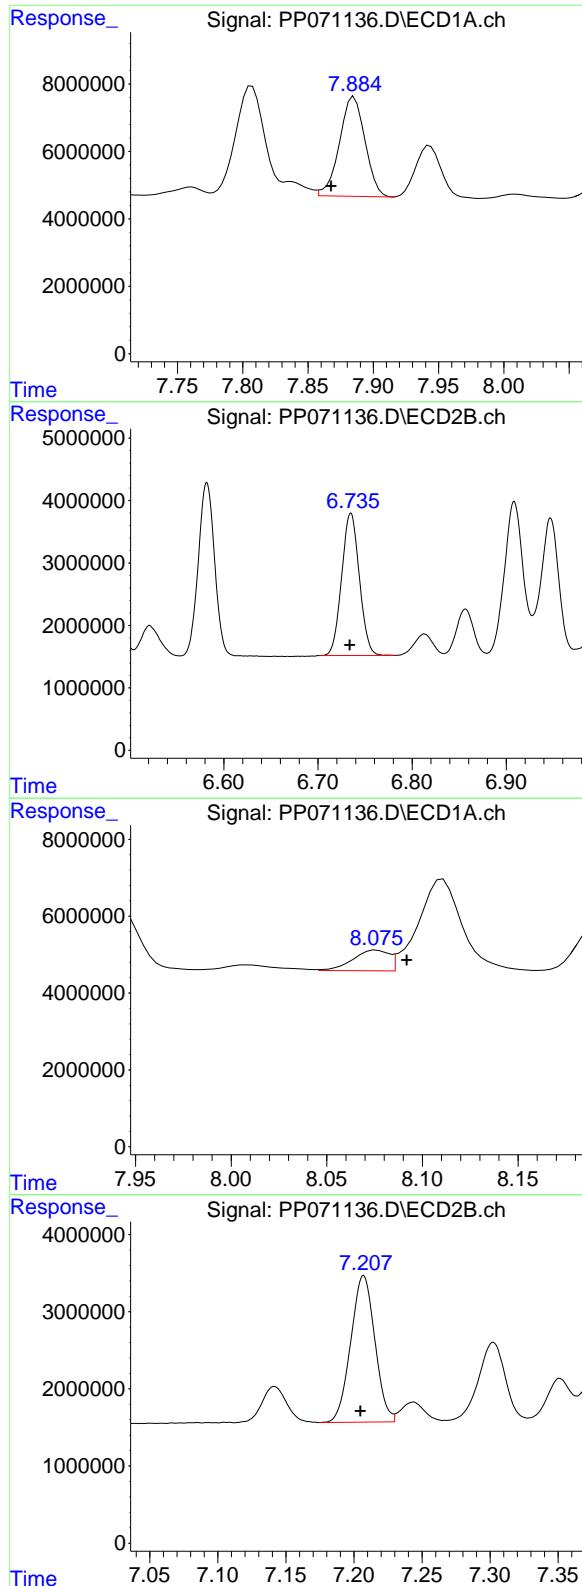

#33 AR-1260-3

R.T.: 7.885 min  
 Delta R.T.: 0.018 min  
 Response: 40227656  
 Conc: 503.36 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#33 AR-1260-3


R.T.: 6.735 min  
 Delta R.T.: 0.001 min  
 Response: 29796945  
 Conc: 546.87 ng/ml

#34 AR-1260-4

R.T.: 8.076 min  
 Delta R.T.: -0.016 min  
 Response: 7015115  
 Conc: 89.10 ng/ml

#34 AR-1260-4

R.T.: 7.207 min  
 Delta R.T.: 0.002 min  
 Response: 23421548  
 Conc: 489.72 ng/ml

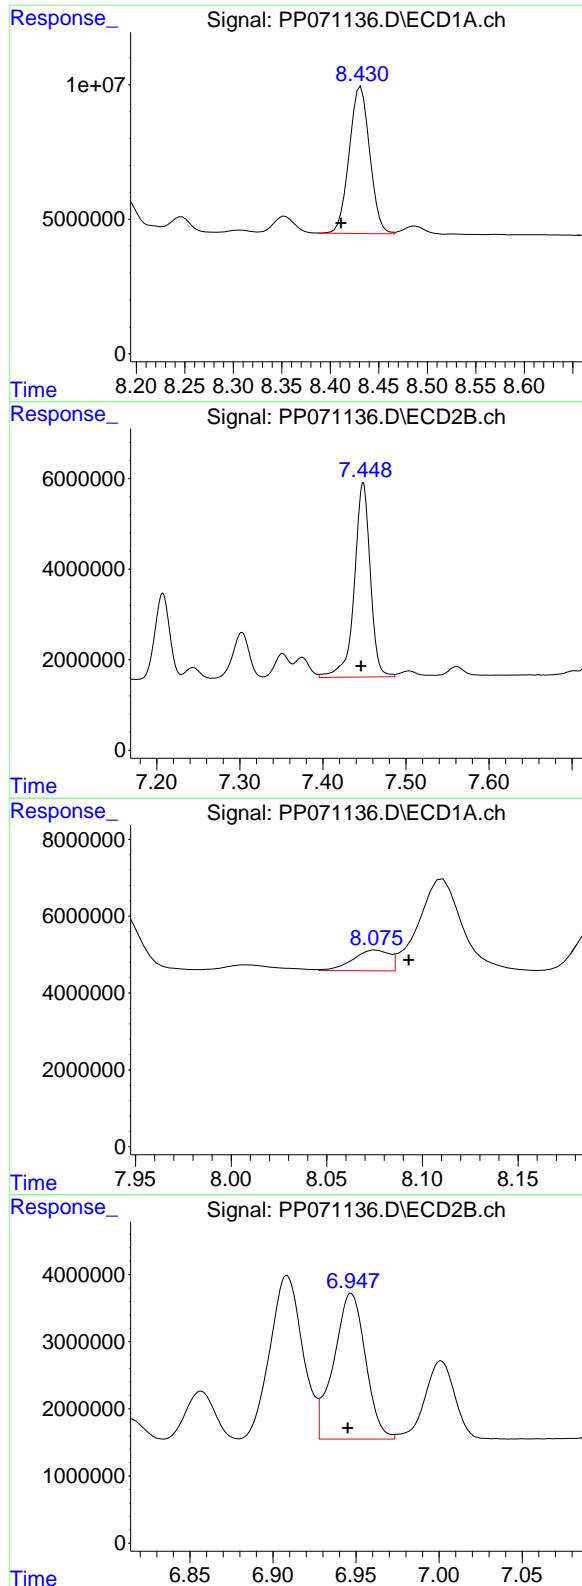

#35 AR-1260-5

R.T.: 8.431 min  
 Delta R.T.: 0.020 min  
 Response: 80513512  
 Conc: 506.74 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#35 AR-1260-5


R.T.: 7.448 min  
 Delta R.T.: 0.002 min  
 Response: 57532352  
 Conc: 462.07 ng/ml

#36 AR-1262-1

R.T.: 8.076 min  
 Delta R.T.: -0.017 min  
 Response: 7015115  
 Conc: 65.99 ng/ml

#36 AR-1262-1

R.T.: 6.947 min  
 Delta R.T.: 0.002 min  
 Response: 28743067  
 Conc: 335.93 ng/ml

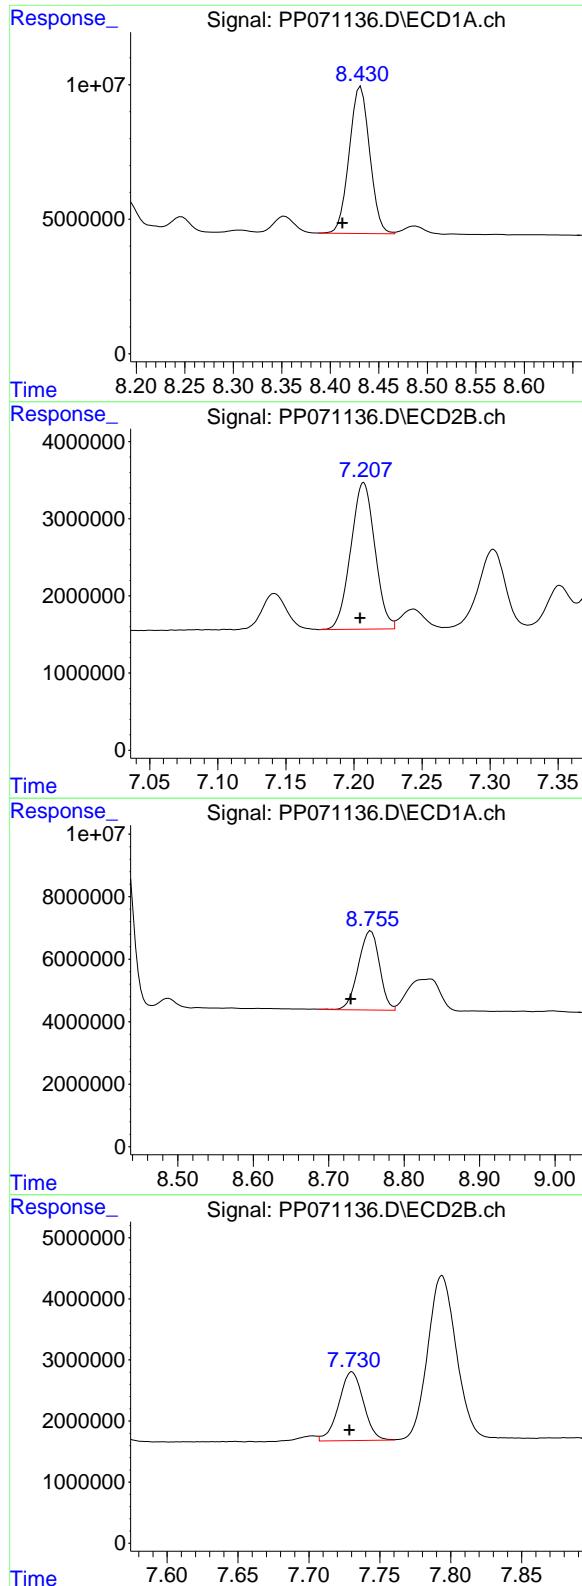

#37 AR-1262-2

R.T.: 8.431 min  
 Delta R.T.: 0.019 min  
 Response: 80513512  
 Conc: 405.85 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#37 AR-1262-2


R.T.: 7.207 min  
 Delta R.T.: 0.003 min  
 Response: 23421548  
 Conc: 342.10 ng/ml

#38 AR-1262-3

R.T.: 8.756 min  
 Delta R.T.: 0.027 min  
 Response: 49500185  
 Conc: 375.74 ng/ml

#38 AR-1262-3

R.T.: 7.730 min  
 Delta R.T.: 0.002 min  
 Response: 13610298  
 Conc: 224.14 ng/ml

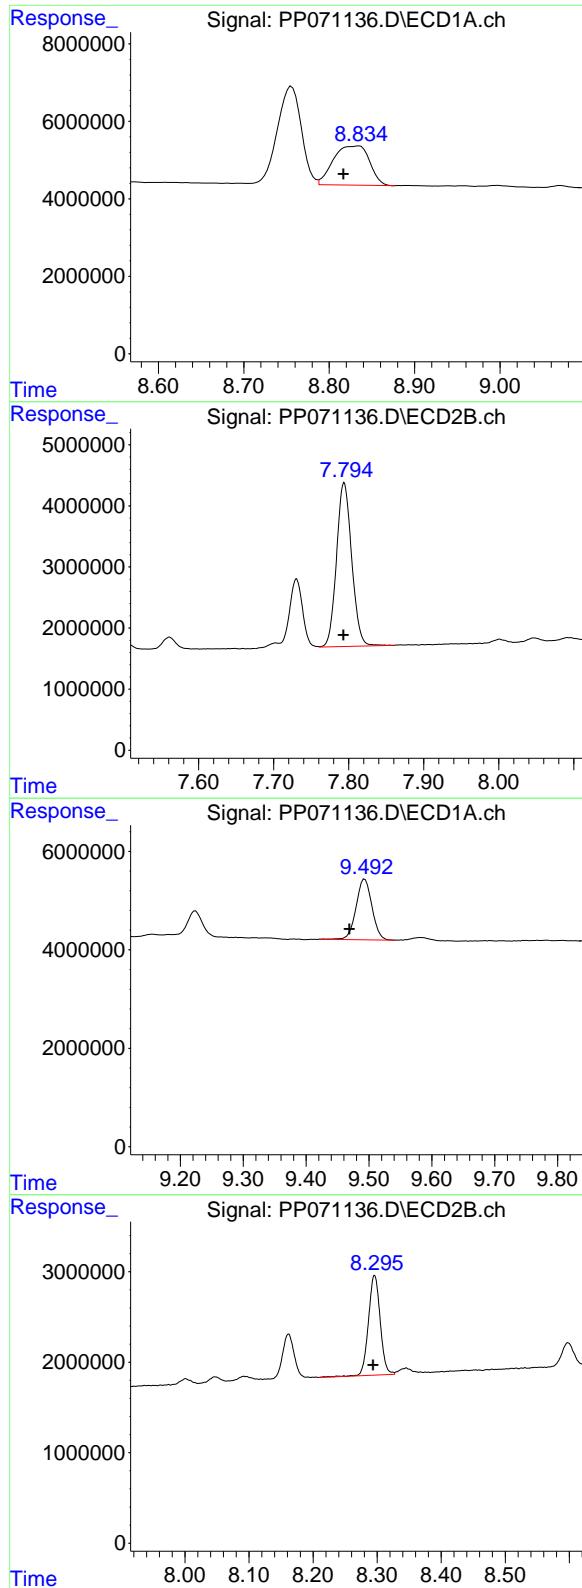

#39 AR-1262-4

R.T.: 8.835 min  
 Delta R.T.: 0.019 min  
 Response: 29791065  
 Conc: 311.57 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#39 AR-1262-4


R.T.: 7.794 min  
 Delta R.T.: 0.000 min  
 Response: 37704999  
 Conc: 379.30 ng/ml

#40 AR-1262-5

R.T.: 9.493 min  
 Delta R.T.: 0.024 min  
 Response: 21754078  
 Conc: 334.34 ng/ml

#40 AR-1262-5

R.T.: 8.296 min  
 Delta R.T.: 0.002 min  
 Response: 14122672  
 Conc: 301.31 ng/ml

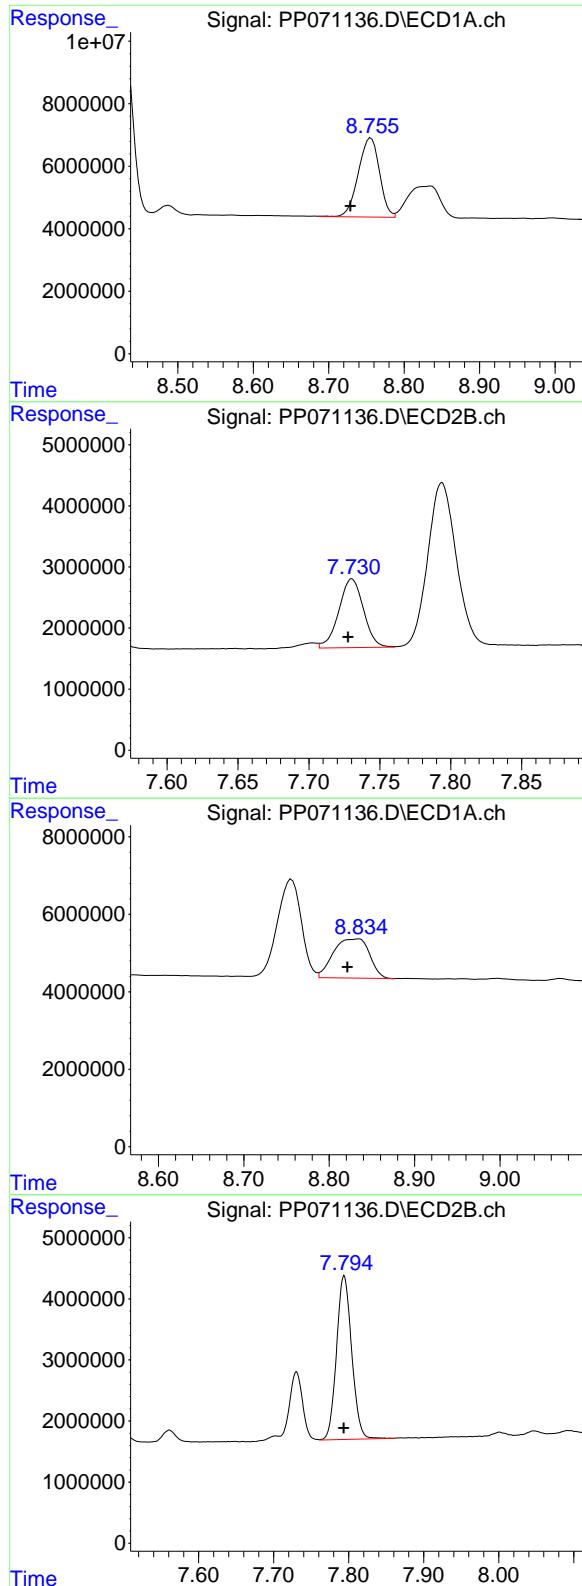

#41 AR-1268-1

R.T.: 8.756 min  
 Delta R.T.: 0.027 min  
 Response: 49500185  
 Conc: 210.19 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#41 AR-1268-1


R.T.: 7.730 min  
 Delta R.T.: 0.002 min  
 Response: 13610298  
 Conc: 79.41 ng/ml

#42 AR-1268-2

R.T.: 8.835 min  
 Delta R.T.: 0.014 min  
 Response: 29791065  
 Conc: 152.53 ng/ml

#42 AR-1268-2

R.T.: 7.794 min  
 Delta R.T.: 0.000 min  
 Response: 37704999  
 Conc: 263.15 ng/ml

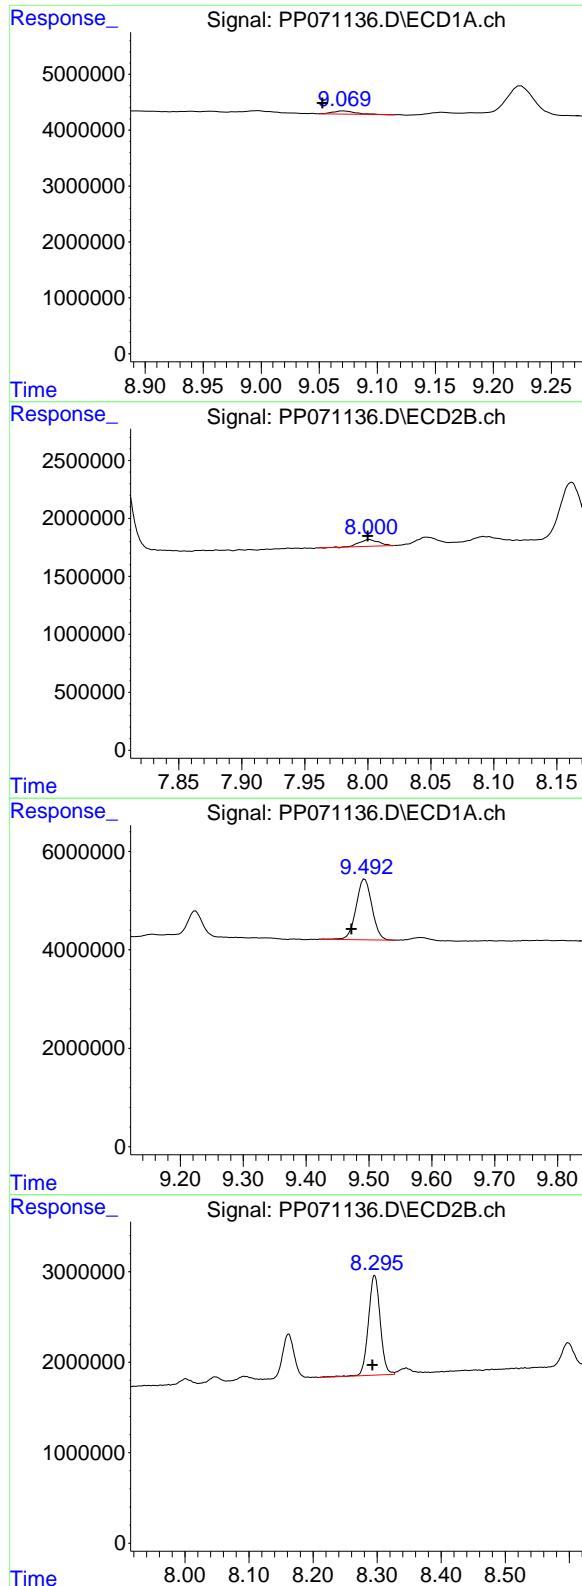

#43 AR-1268-3

R.T.: 9.071 min  
 Delta R.T.: 0.019 min  
 Response: 324667  
 Conc: 1.90 ng/ml

Instrument: ECD\_P  
 ClientSampleId: AR1660CCC500

#43 AR-1268-3


R.T.: 8.001 min  
 Delta R.T.: 0.001 min  
 Response: 608932  
 Conc: 4.94 ng/ml

#44 AR-1268-4

R.T.: 9.493 min  
 Delta R.T.: 0.021 min  
 Response: 21754078  
 Conc: 307.49 ng/ml

#44 AR-1268-4

R.T.: 8.296 min  
 Delta R.T.: 0.003 min  
 Response: 14122672  
 Conc: 267.41 ng/ml

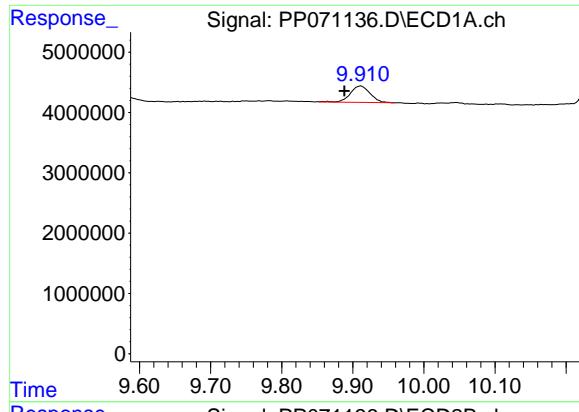

#45 AR-1268-5


R.T.: 9.911 min  
Delta R.T.: 0.023 min  
Response: 5287089  
Conc: 11.10 ng/ml

Instrument:

ECD\_P

ClientSampleId :

AR1660CCC500

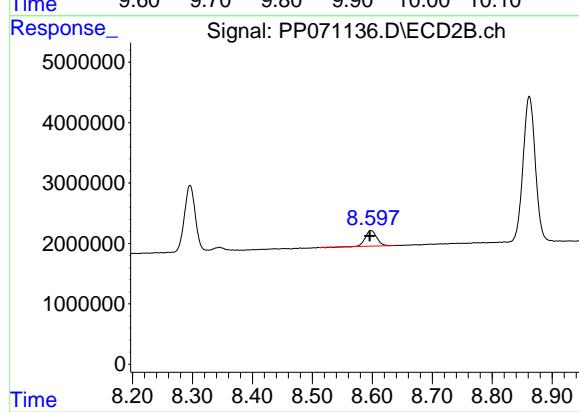

#45 AR-1268-5

R.T.: 8.598 min  
Delta R.T.: 0.002 min  
Response: 3490210  
Conc: 9.64 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20