

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
 Data File : PL094568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 10:22
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/12/2025
 Supervised By : Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 17:37:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:31:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.771	53468086	65423025	18.889	18.330
28)	SA Decachlor...	9.053	7.905	42521417	78359154	20.177	19.399
Target Compounds							
9)	A Endosulfan I	6.067	5.092	29402034	37055598	9.577	8.443
10)	B gamma-Chl...	5.937	4.971	33232558	42863759	9.863	8.877m
12)	B 4,4'-DDE	6.191	5.225	60170599	86039267	20.452	18.509
13)	MA Dieldrin	6.343	5.356	61616040	87035875	19.266	17.939
19)	B Endosulfa...	7.158	6.330	48427242	76018164	19.912	18.662
20)	A Methoxychlor	7.500	6.606	108.5E6	193.4E6	90.602	91.159
21)	B Endrin ke...	7.643	6.835	53103007	96817803	20.090	20.286

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
Data File : PL094568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 10:22
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

RESCHK

Manual Integrations



APPROVED


Reviewed By :Abdul Mirza 03/12/2025

Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 17:37:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:31:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

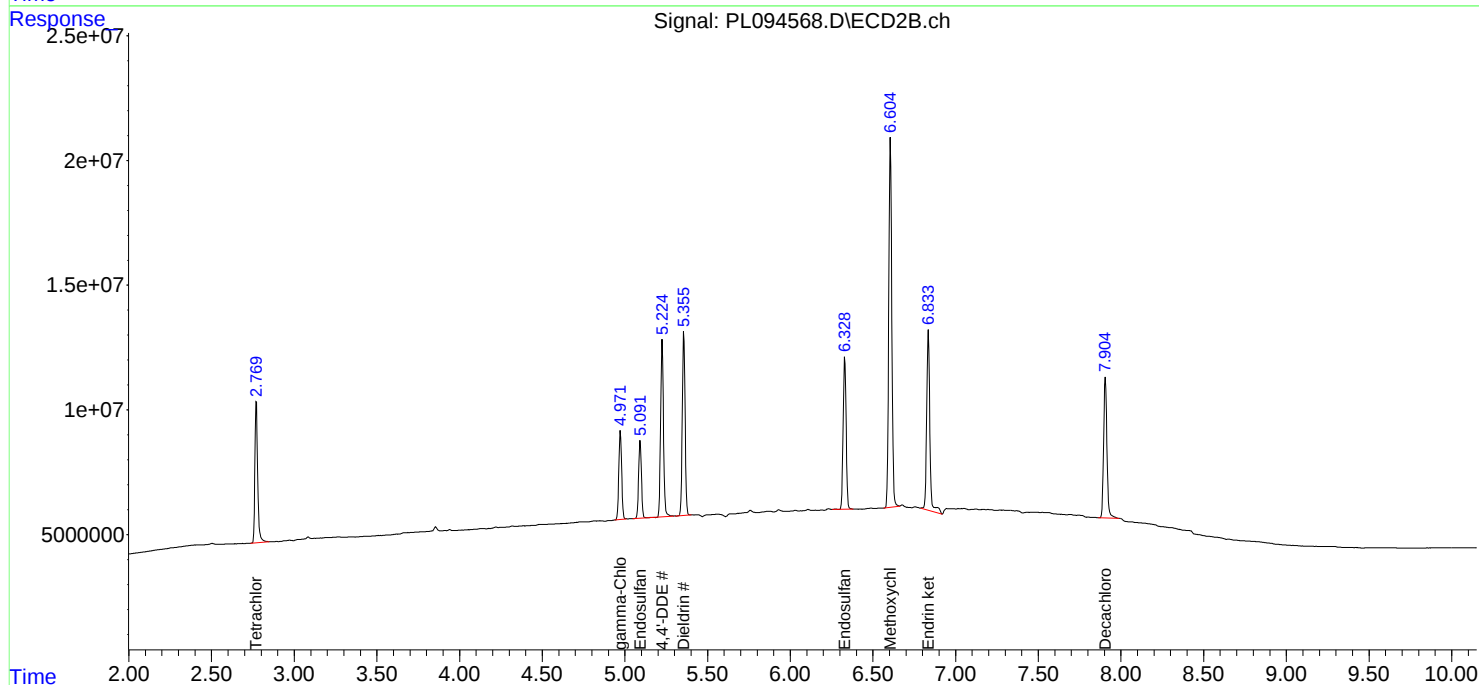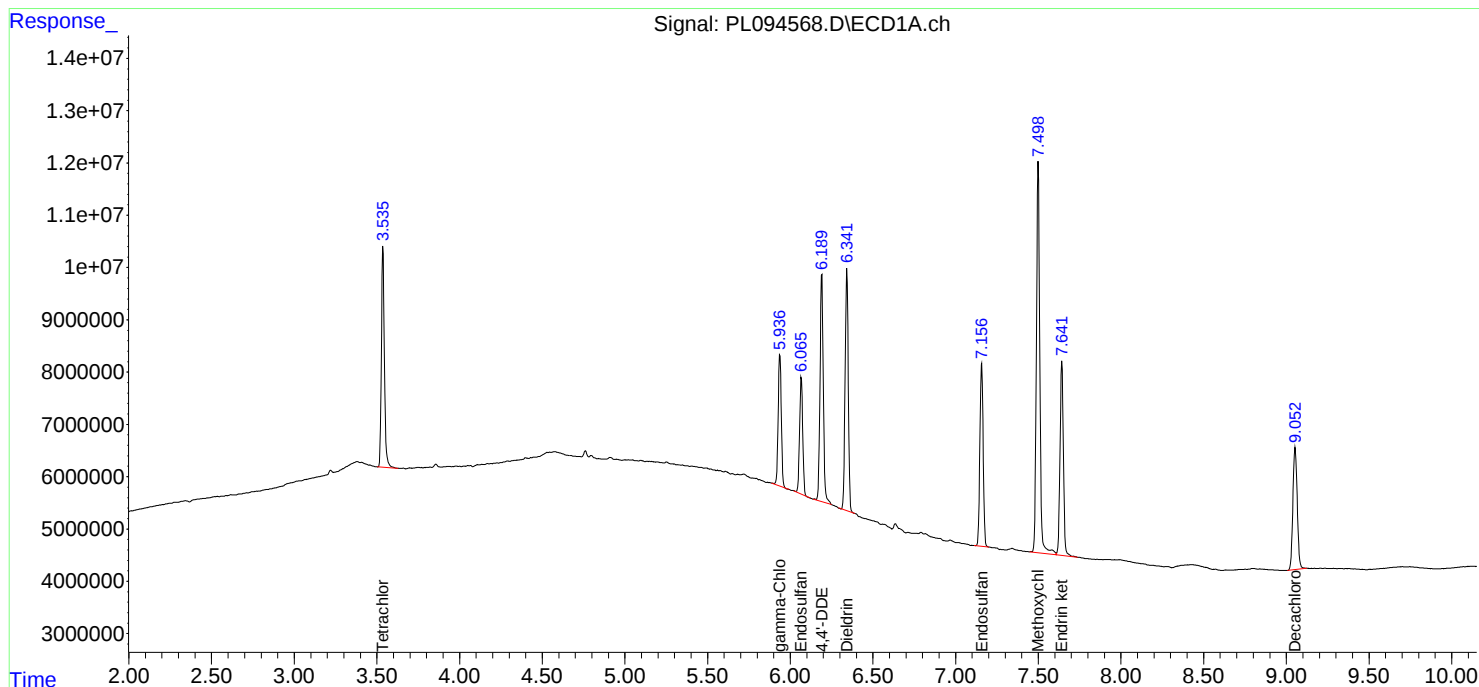

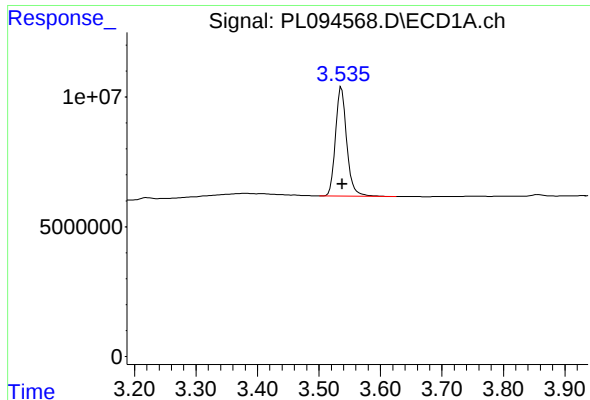


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.001 min
Response: 53468086
Conc: 18.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

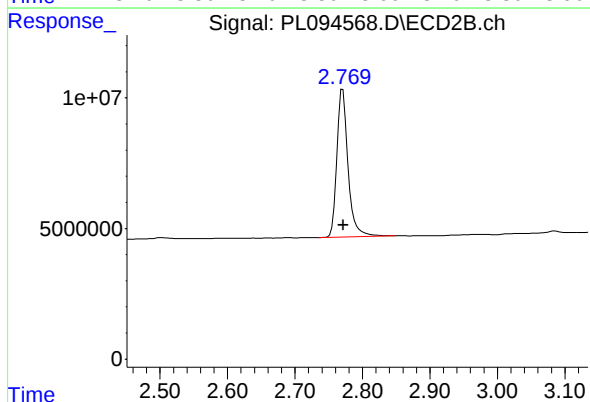


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: -0.001 min
Response: 65423025
Conc: 18.33 ng/ml

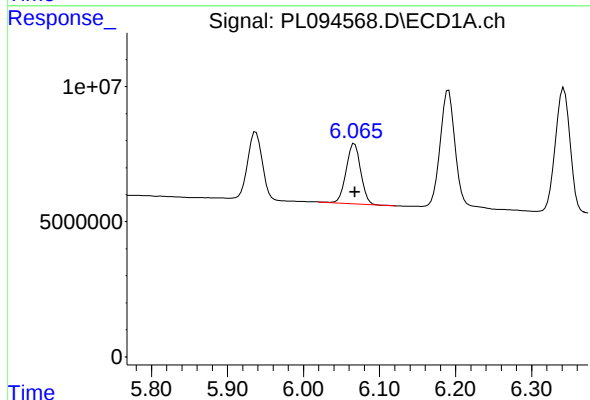


#9 Endosulfan I

R.T.: 6.067 min
Delta R.T.: 0.000 min
Response: 29402034
Conc: 9.58 ng/ml

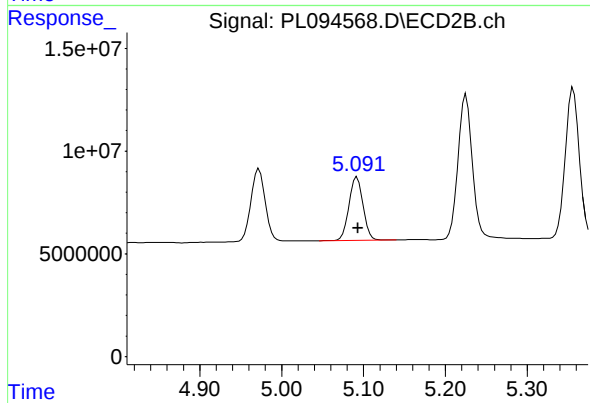

#9 Endosulfan I

R.T.: 5.092 min
Delta R.T.: -0.001 min
Response: 37055598
Conc: 8.44 ng/ml

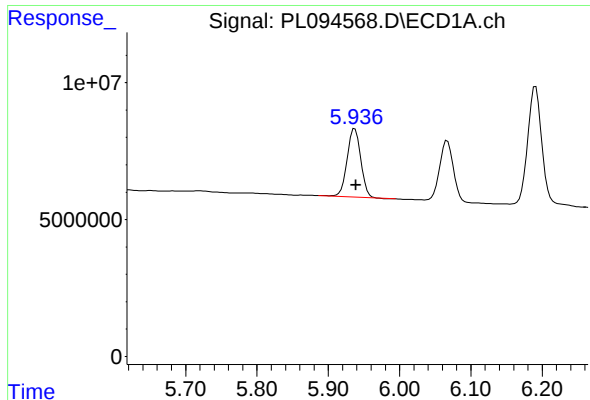


#10 gamma-Chlordane

R.T.: 5.937 min
Delta R.T.: -0.002 min
Response: 33232558
Conc: 9.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

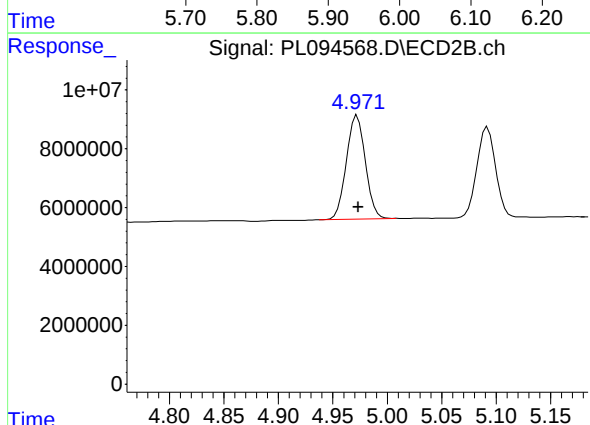


#10 gamma-Chlordane

R.T.: 4.971 min
Delta R.T.: -0.003 min
Response: 42863759
Conc: 8.88 ng/ml

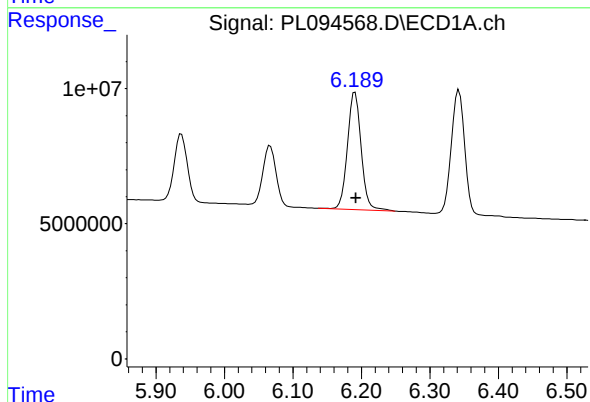


#12 4,4'-DDE

R.T.: 6.191 min
Delta R.T.: -0.001 min
Response: 60170599
Conc: 20.45 ng/ml

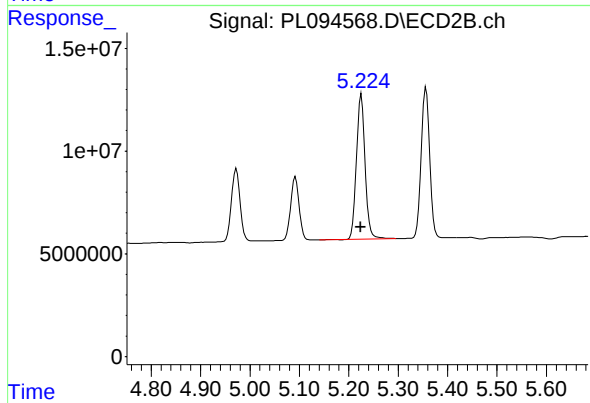

#12 4,4'-DDE

R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 86039267
Conc: 18.51 ng/ml

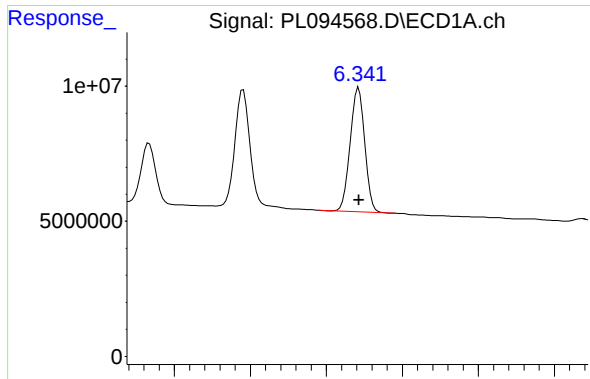


#13 Dieldrin

R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 61616040
Conc: 19.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

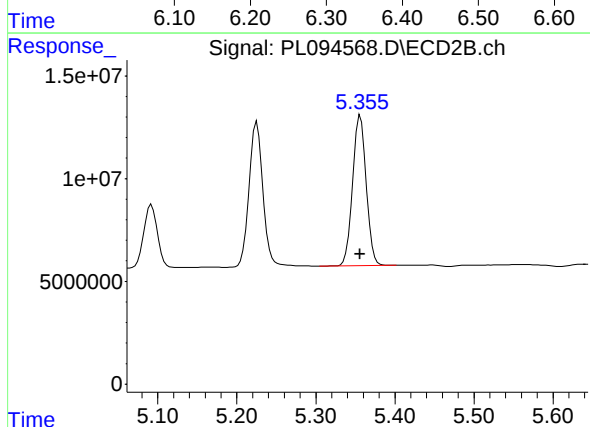


#13 Dieldrin

R.T.: 5.356 min
Delta R.T.: 0.000 min
Response: 87035875
Conc: 17.94 ng/ml

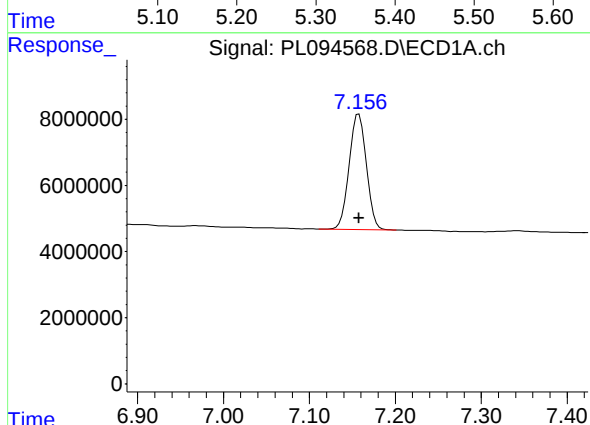


#19 Endosulfan Sulfate

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 48427242
Conc: 19.91 ng/ml

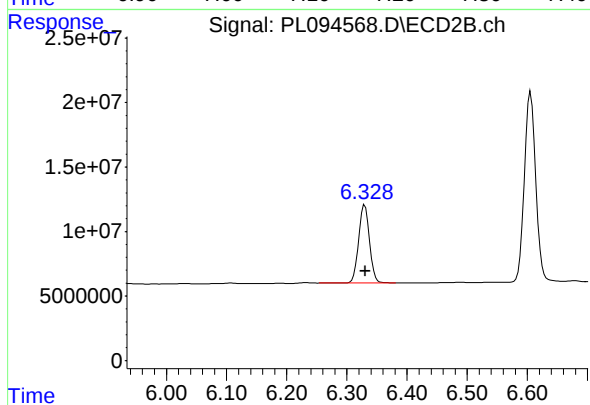

#19 Endosulfan Sulfate

R.T.: 6.330 min
Delta R.T.: 0.000 min
Response: 76018164
Conc: 18.66 ng/ml

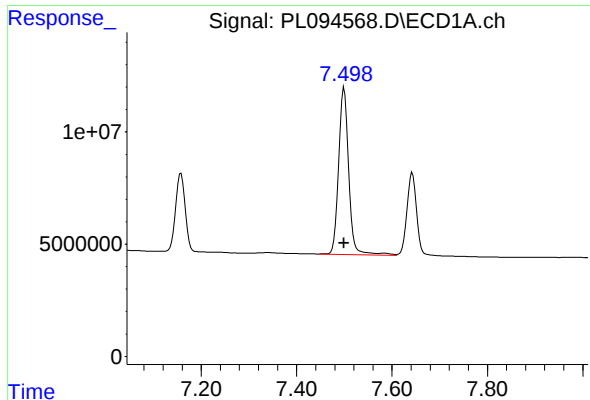


#20 Methoxychlor

R.T.: 7.500 min
Delta R.T.: 0.000 min
Response: 108457351
Conc: 90.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

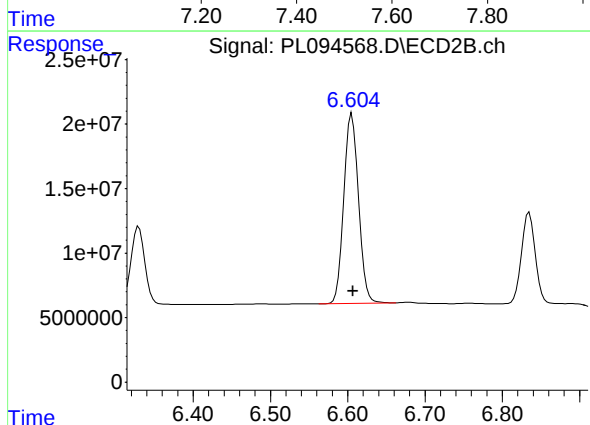


#20 Methoxychlor

R.T.: 6.606 min
Delta R.T.: -0.001 min
Response: 193354717
Conc: 91.16 ng/ml

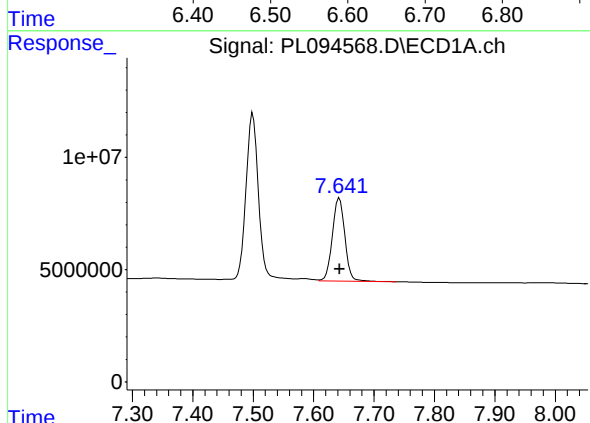


#21 Endrin ketone

R.T.: 7.643 min
Delta R.T.: 0.000 min
Response: 53103007
Conc: 20.09 ng/ml

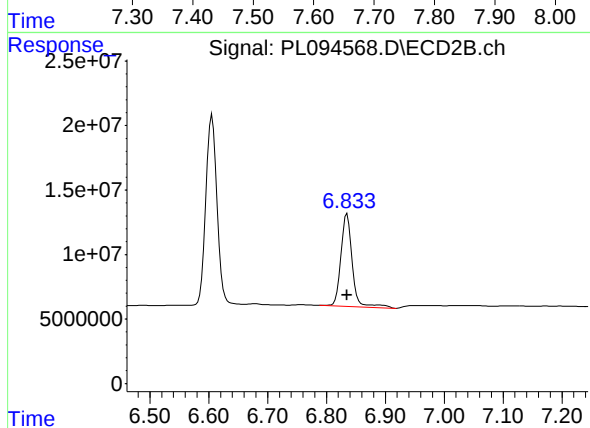

#21 Endrin ketone

R.T.: 6.835 min
Delta R.T.: 0.000 min
Response: 96817803
Conc: 20.29 ng/ml

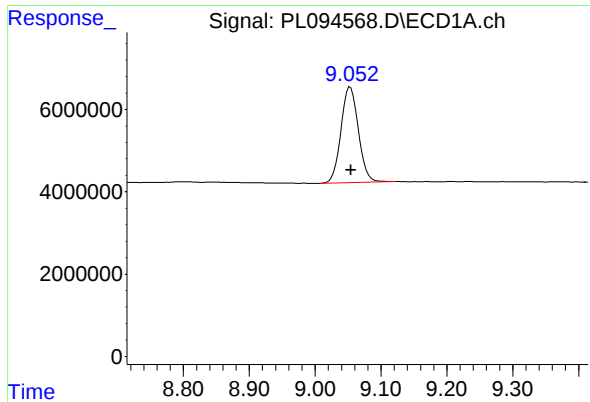


#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.001 min
Response: 42521417
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

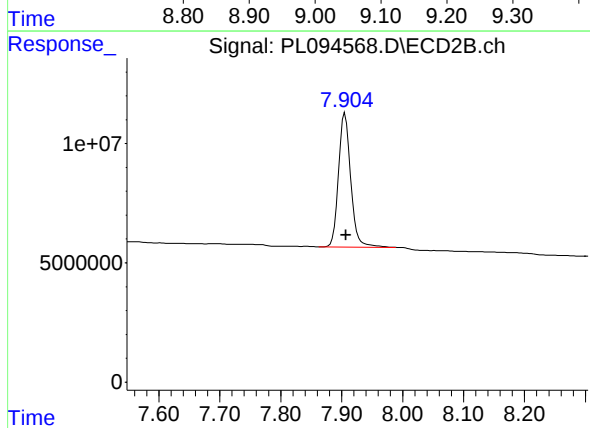

#28 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: -0.002 min
Response: 78359154
Conc: 19.40 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
Data File : PL094568.D
Acq On : 11 Mar 2025 10:22
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Title : GC Extractables
Last Update : Tue Mar 11 17:42:21 2025
Integrator: ChemStation

RT#1	RT#2	Resolution
3.537	5.937	100.00%
5.937	6.067	100.00%
6.067	6.191	100.00%
6.191	6.343	100.00%
6.343	7.158	100.00%
7.158	7.500	100.00%
7.500	7.643	100.00%
7.643	9.053	100.00%

Signal #2

2.771	4.972	100.00%
4.972	5.092	100.00%
5.092	5.225	100.00%
5.225	5.356	100.00%
5.356	6.330	100.00%
6.330	6.606	100.00%
6.606	6.835	100.00%
6.835	7.905	100.00%

PL031125.M Mon Mar 17 09:39:54 2025