

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
 Data File : PL094569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 10:35
 Operator : AR\AJ
 Sample : PSTDICC100
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC100

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 17:23:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:20:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.771	267.8E6	357.3E6	99.165	100.991
28)	SA Decachlor...	9.054	7.905	193.9E6	395.0E6	97.943	100.590
Target Compounds							
2)	A alpha-BHC	3.994	3.274	405.1E6	569.7E6	100.552	102.608
3)	MA gamma-BHC...	4.327	3.604	388.6E6	537.2E6	100.578	102.282
4)	MA Heptachlor	4.914	3.942	364.6E6	536.3E6	99.021	101.268
5)	MB Aldrin	5.256	4.221	348.7E6	504.3E6	99.355	102.086
6)	B beta-BHC	4.525	3.904	167.3E6	219.0E6	97.941	100.407
7)	B delta-BHC	4.772	4.133	373.2E6	524.5E6	100.154	102.450
8)	B Heptachlo...	5.682	4.724	312.8E6	461.9E6	98.900	100.980
9)	A Endosulfan I	6.069	5.093	285.6E6	445.6E6	98.821	101.246
10)	B gamma-Chl...	5.939	4.974	315.2E6	494.7E6	99.127	101.813
11)	B alpha-Chl...	6.018	5.037	307.8E6	484.8E6	98.919	101.428
12)	B 4,4'-DDE	6.191	5.226	280.1E6	475.6E6	99.232	101.777
13)	MA Dieldrin	6.344	5.357	299.9E6	499.1E6	99.313	102.045
14)	MA Endrin	6.573	5.634	258.6E6	443.5E6	99.178	101.238
15)	B Endosulfa...	6.794	5.928	251.0E6	434.7E6	98.634	101.059
16)	A 4,4'-DDD	6.710	5.781	205.5E6	374.5E6	98.978	102.209
17)	MA 4,4'-DDT	7.022	6.031	225.1E6	420.6E6	99.295	102.337
18)	B Endrin al...	6.924	6.108	189.9E6	330.1E6	97.545	100.338
19)	B Endosulfa...	7.158	6.330	220.3E6	411.4E6	97.946	101.002
20)	A Methoxychlor	7.498	6.606	110.9E6	208.9E6	98.022m	99.757
21)	B Endrin ke...	7.643	6.836	248.5E6	478.7E6	99.610	100.842
22)	Mirex	8.115	7.015	184.4E6	365.6E6	96.823m	99.620

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
Data File : PL094569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 10:35
Operator : AR\AJ
Sample : PSTDICC100
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

PSTDICC100



Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 17:23:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:20:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

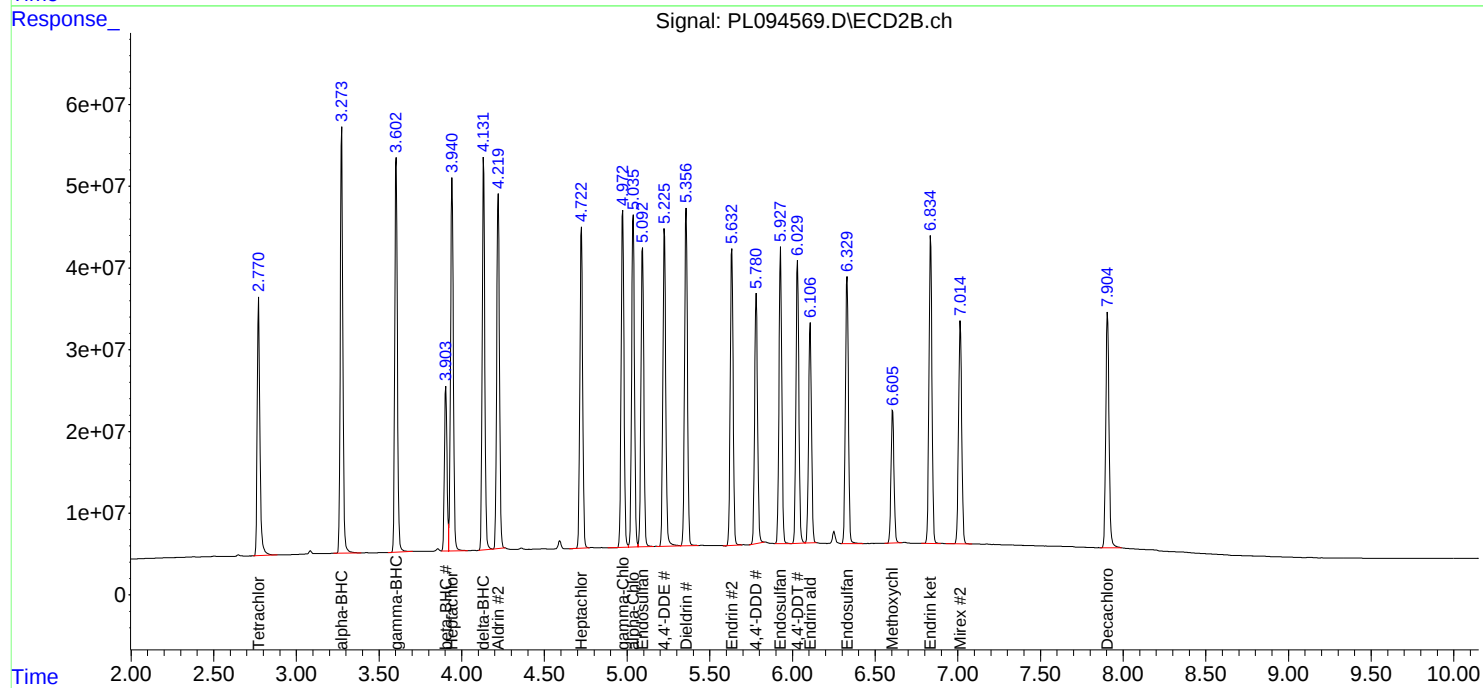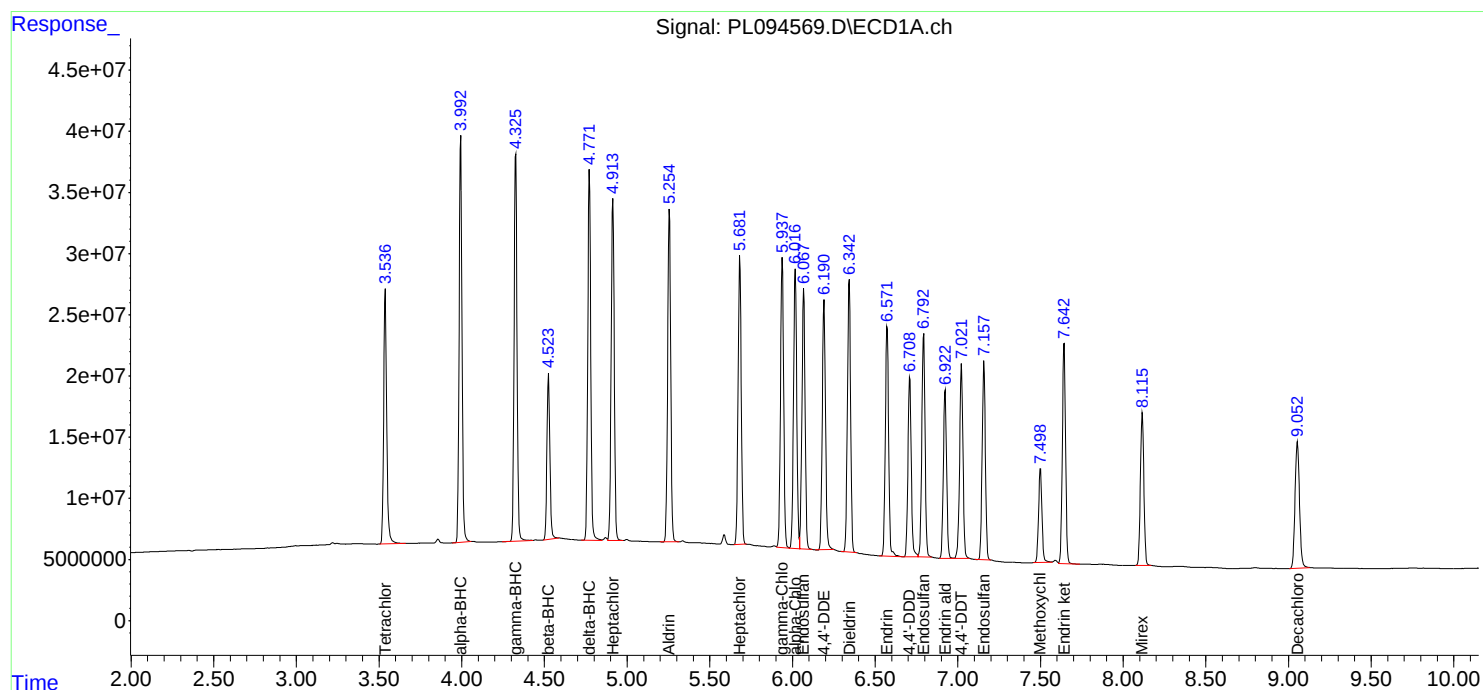

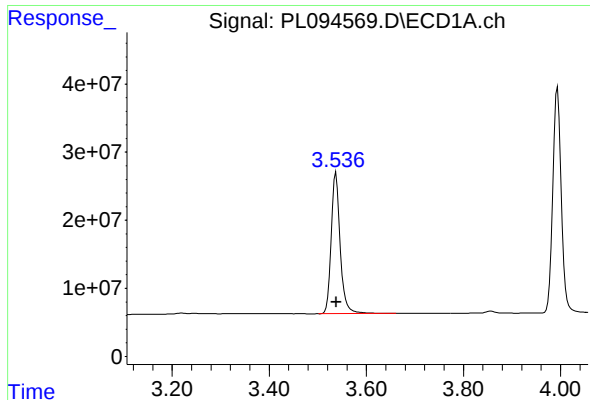


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 267763168
Conc: 99.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

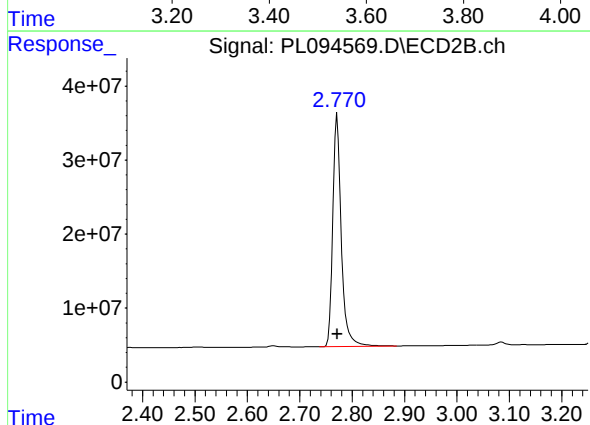


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 357251635
Conc: 100.99 ng/ml

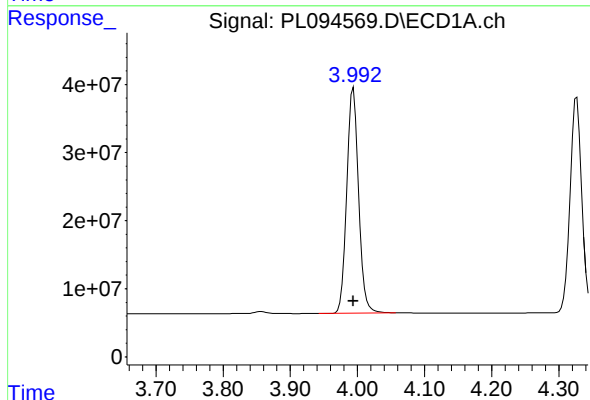


#2 alpha-BHC

R.T.: 3.994 min
Delta R.T.: 0.000 min
Response: 405083205
Conc: 100.55 ng/ml

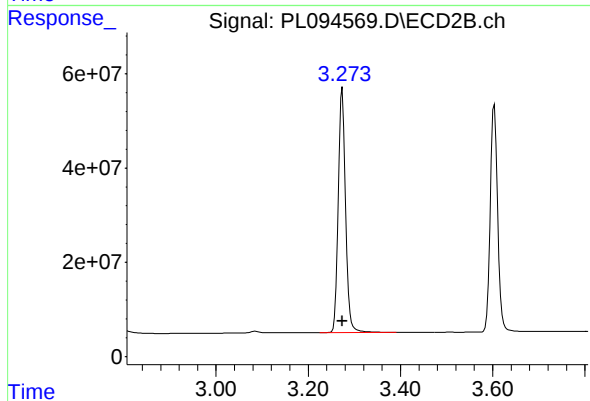

#2 alpha-BHC

R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 569673035
Conc: 102.61 ng/ml

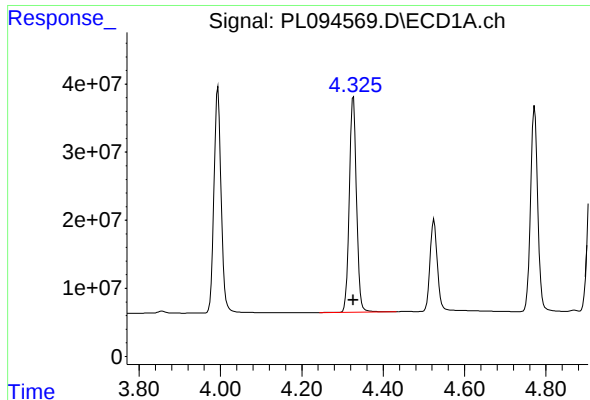


#3 gamma-BHC (Lindane)

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 388608790
Conc: 100.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

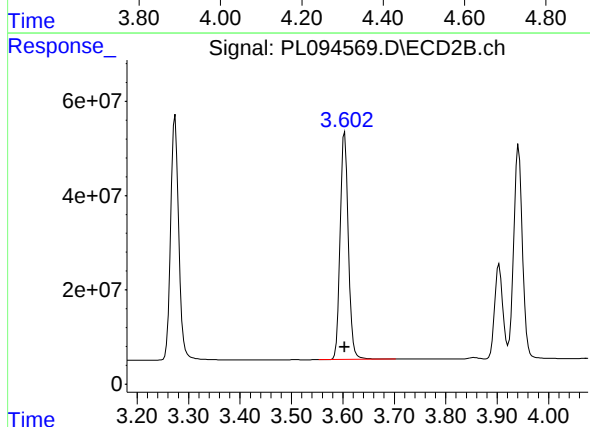


#3 gamma-BHC (Lindane)

R.T.: 3.604 min
Delta R.T.: 0.000 min
Response: 537223278
Conc: 102.28 ng/ml

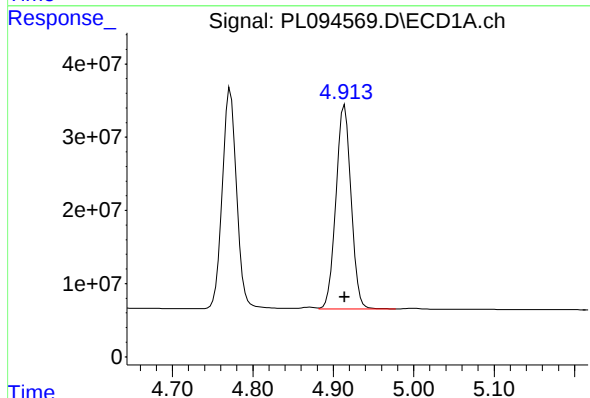


#4 Heptachlor

R.T.: 4.914 min
Delta R.T.: 0.000 min
Response: 364573075
Conc: 99.02 ng/ml

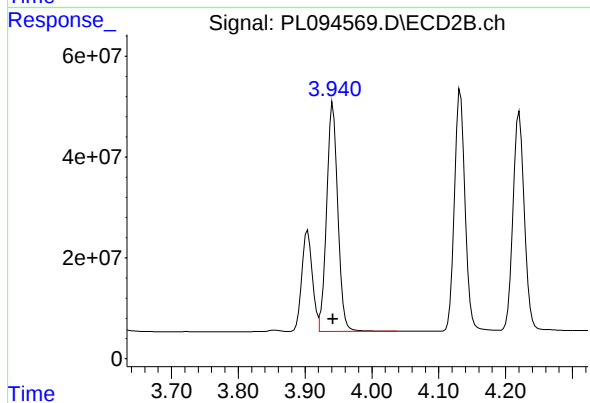

#4 Heptachlor

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 536306132
Conc: 101.27 ng/ml

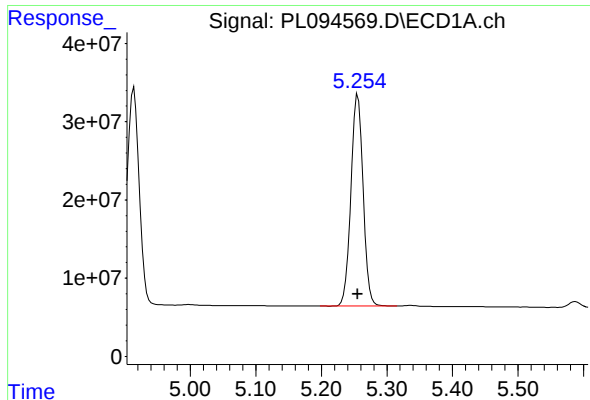


#5 Aldrin

R.T.: 5.256 min
Delta R.T.: 0.000 min
Response: 348651471
Conc: 99.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

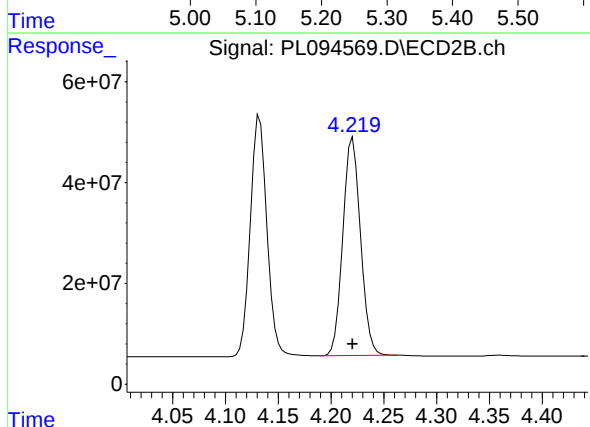


#5 Aldrin

R.T.: 4.221 min
Delta R.T.: 0.000 min
Response: 504334831
Conc: 102.09 ng/ml

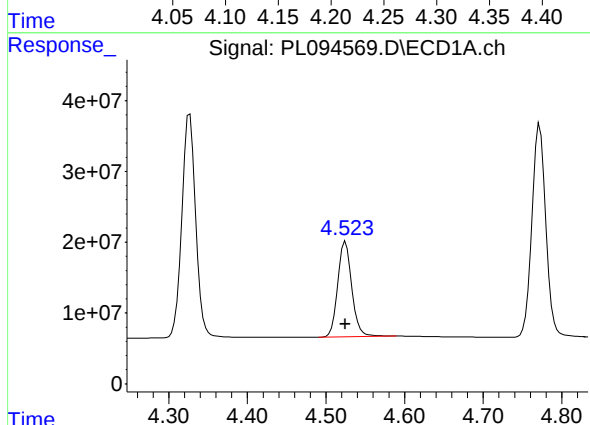


#6 beta-BHC

R.T.: 4.525 min
Delta R.T.: 0.000 min
Response: 167259580
Conc: 97.94 ng/ml

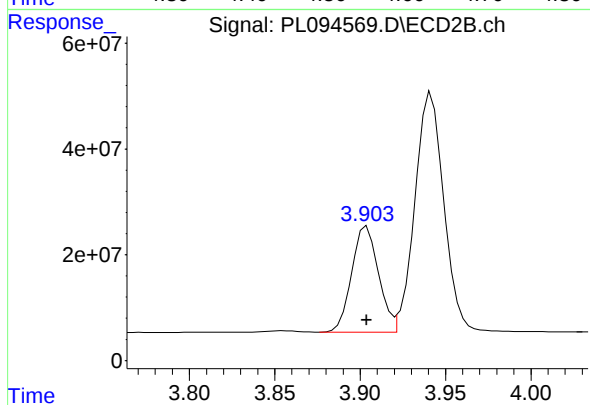

#6 beta-BHC

R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 218990788
Conc: 100.41 ng/ml

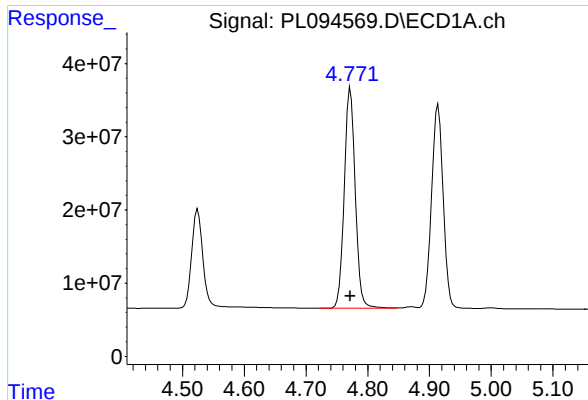


#7 delta-BHC

R.T.: 4.772 min
Delta R.T.: 0.000 min
Response: 373153307
Conc: 100.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

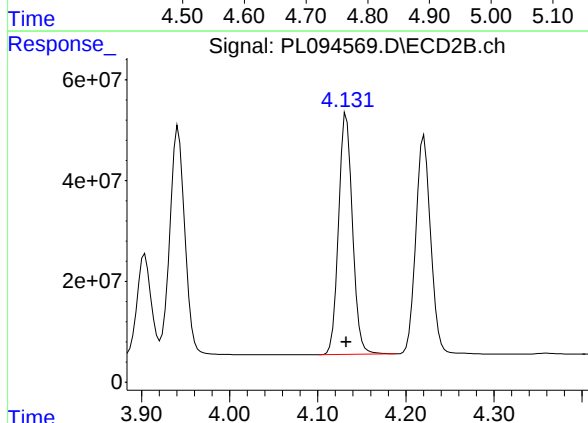


#7 delta-BHC

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 524542093
Conc: 102.45 ng/ml

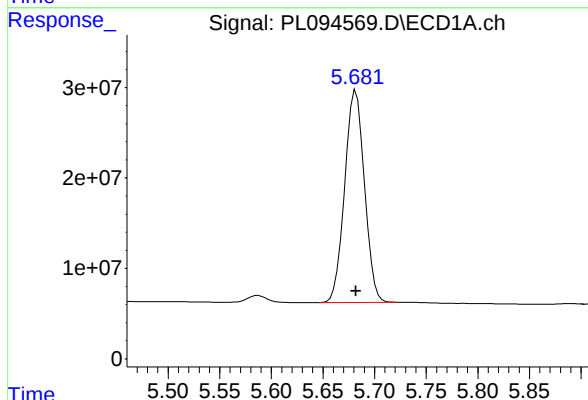


#8 Heptachlor epoxide

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 312768417
Conc: 98.90 ng/ml

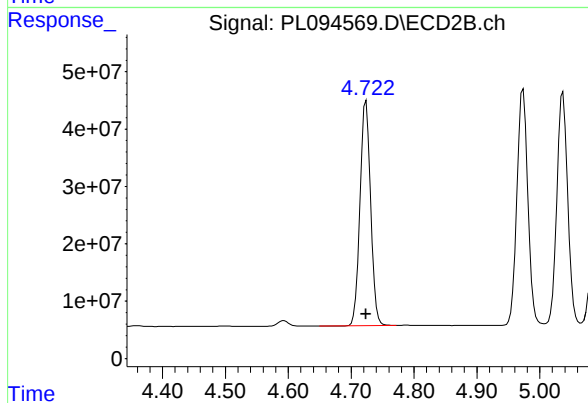

#8 Heptachlor epoxide

R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 461918591
Conc: 100.98 ng/ml

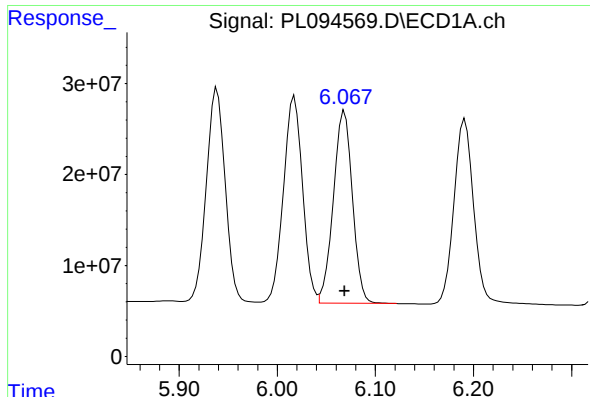


#9 Endosulfan I

R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 285605332
Conc: 98.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

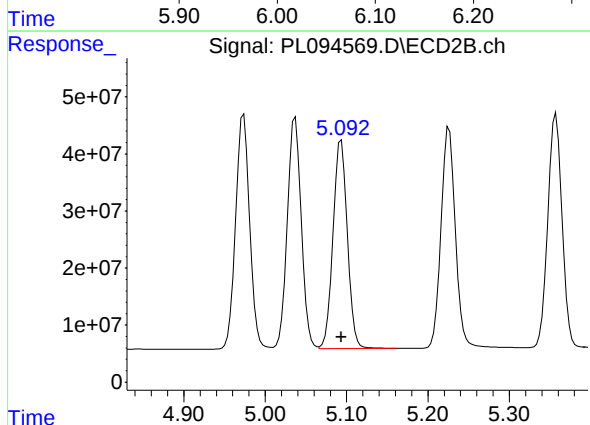


#9 Endosulfan I

R.T.: 5.093 min
Delta R.T.: 0.000 min
Response: 445594192
Conc: 101.25 ng/ml

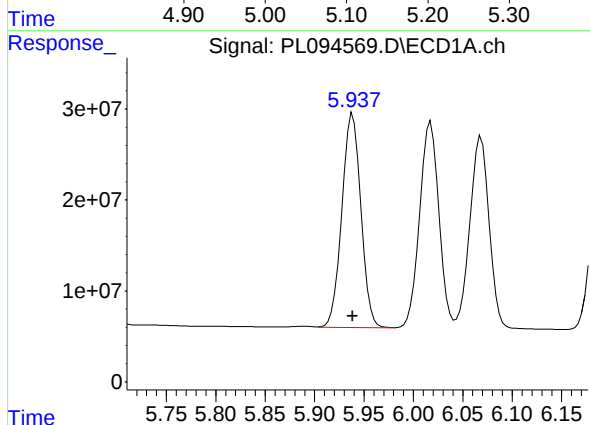


#10 gamma-Chlordane

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 315231814
Conc: 99.13 ng/ml

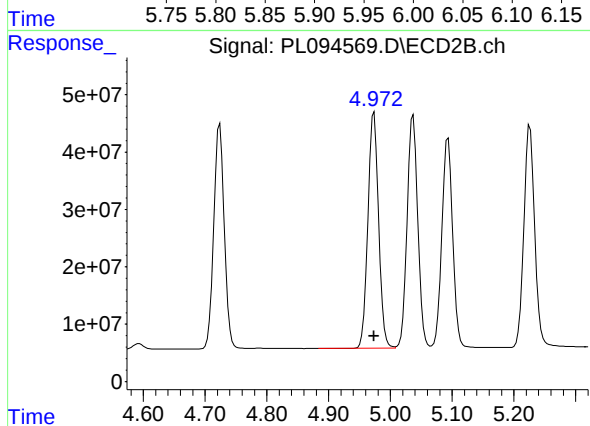

#10 gamma-Chlordane

R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 494683451
Conc: 101.81 ng/ml

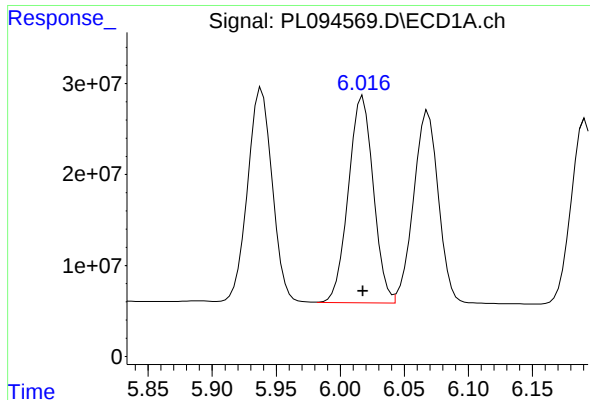


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 307825063
Conc: 98.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

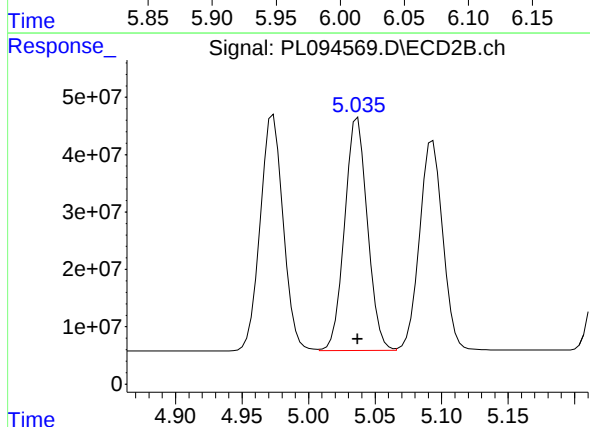


#11 alpha-Chlordane

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 484791380
Conc: 101.43 ng/ml

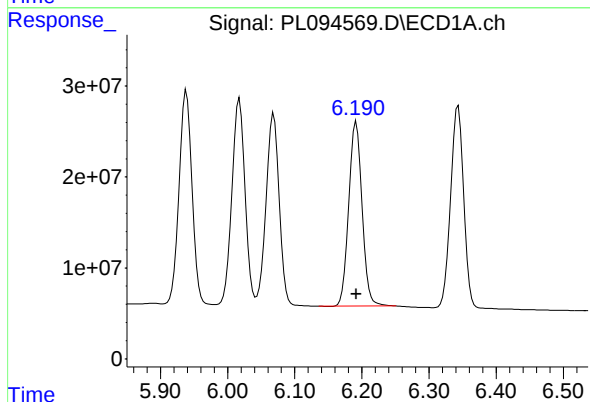


#12 4,4'-DDE

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 280081824
Conc: 99.23 ng/ml

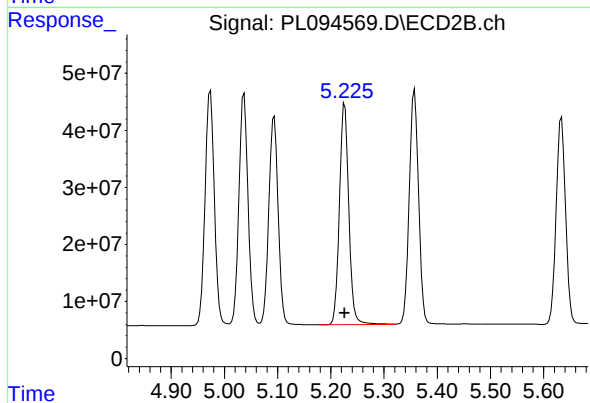

#12 4,4'-DDE

R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 475560692
Conc: 101.78 ng/ml

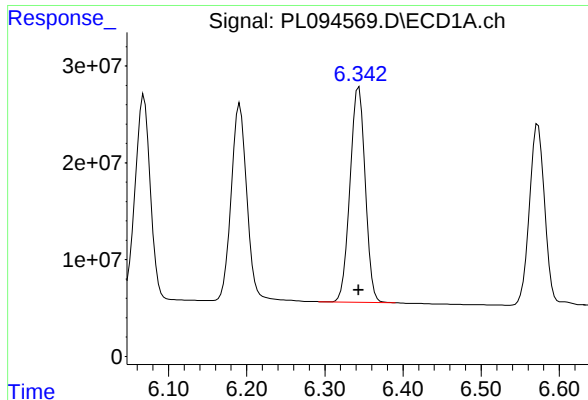


#13 Dieldrin

R.T.: 6.344 min
Delta R.T.: 0.000 min
Response: 299891748
Conc: 99.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

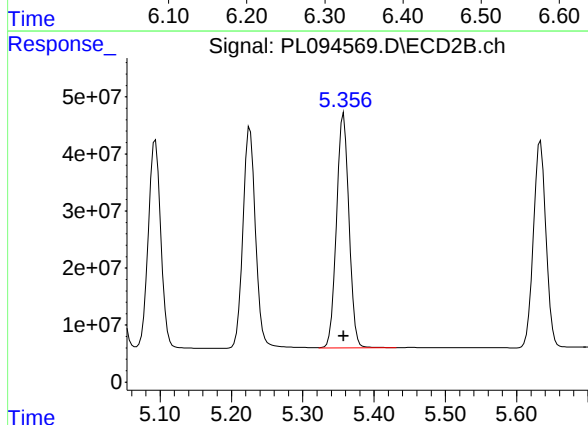


#13 Dieldrin

R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 499116818
Conc: 102.04 ng/ml

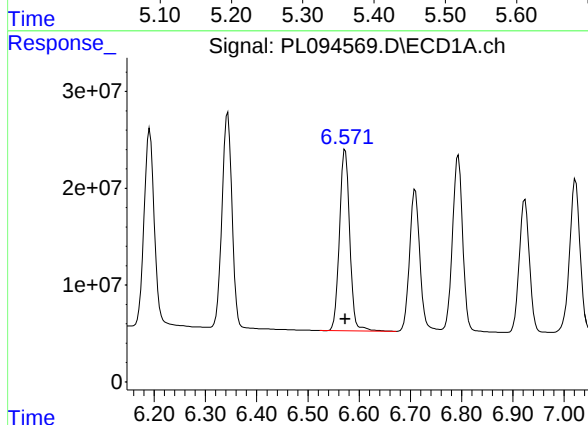


#14 Endrin

R.T.: 6.573 min
Delta R.T.: 0.000 min
Response: 258594013
Conc: 99.18 ng/ml

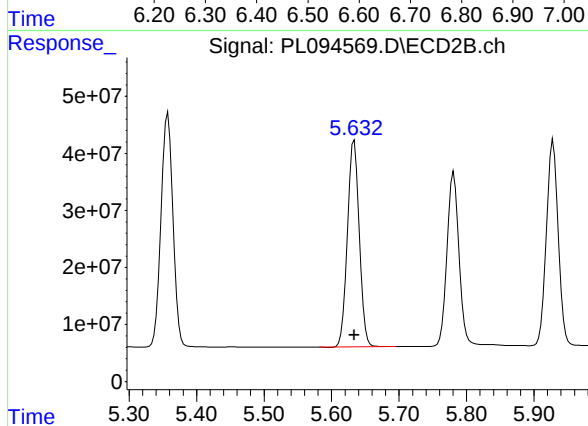

#14 Endrin

R.T.: 5.634 min
Delta R.T.: 0.000 min
Response: 443455460
Conc: 101.24 ng/ml

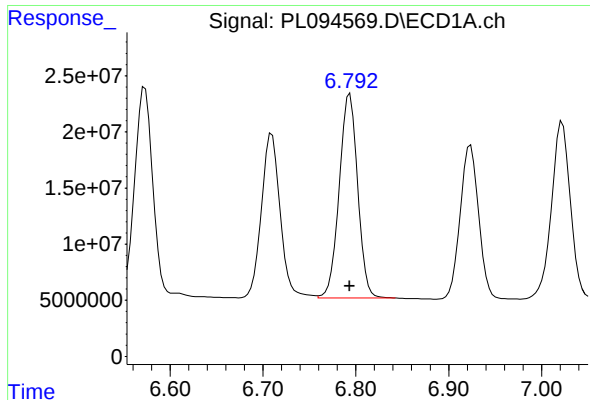


#15 Endosulfan II

R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 250994889
Conc: 98.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

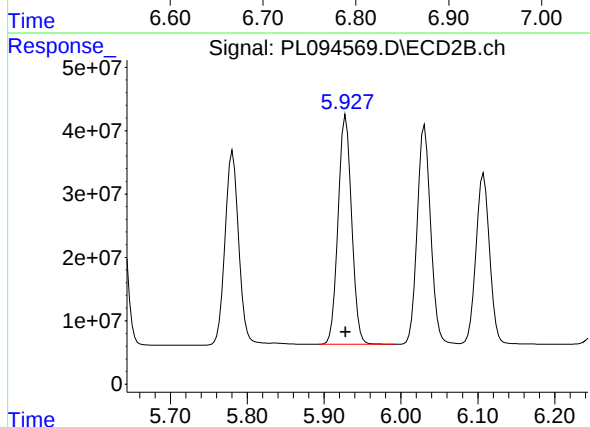


#15 Endosulfan II

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 434672686
Conc: 101.06 ng/ml

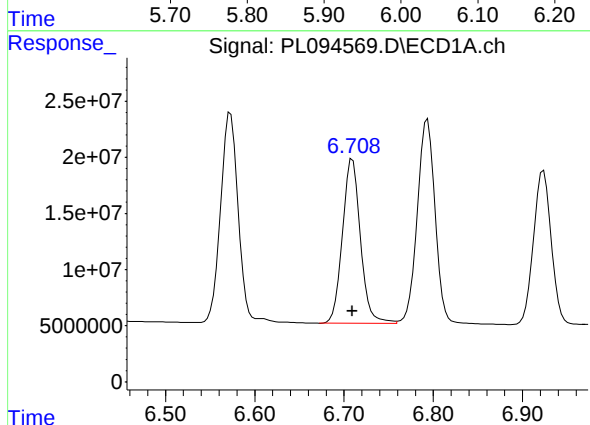


#16 4,4'-DDD

R.T.: 6.710 min
Delta R.T.: 0.000 min
Response: 205479047
Conc: 98.98 ng/ml

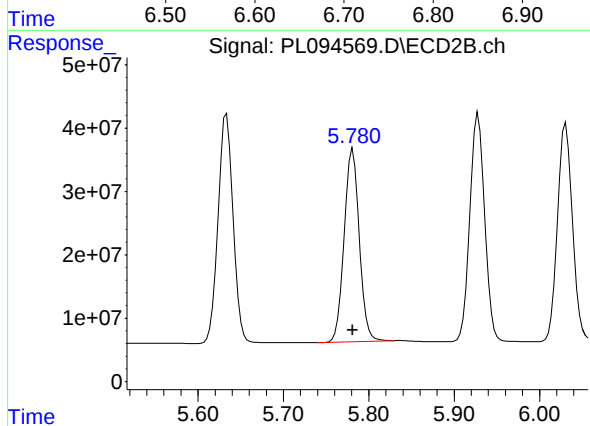

#16 4,4'-DDD

R.T.: 5.781 min
Delta R.T.: 0.000 min
Response: 374466215
Conc: 102.21 ng/ml

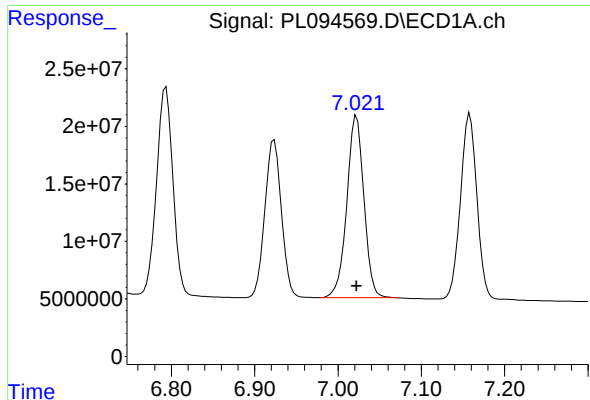


#17 4,4'-DDT

R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 225075617
Conc: 99.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

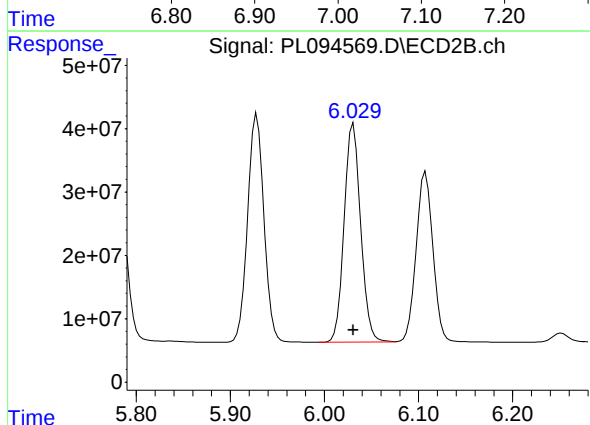


#17 4,4'-DDT

R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 420641323
Conc: 102.34 ng/ml

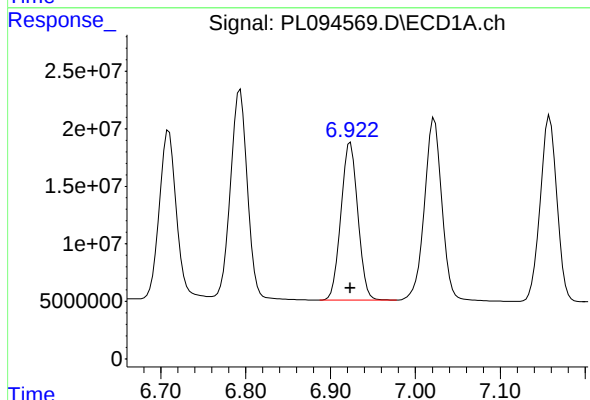


#18 Endrin aldehyde

R.T.: 6.924 min
Delta R.T.: 0.000 min
Response: 189940982
Conc: 97.54 ng/ml

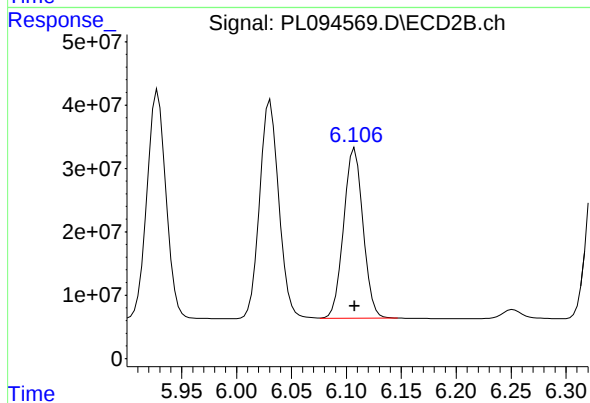

#18 Endrin aldehyde

R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 330131461
Conc: 100.34 ng/ml

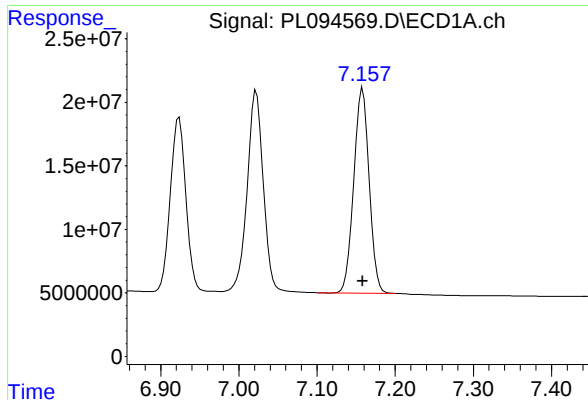


#19 Endosulfan Sulfate

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 220288726
Conc: 97.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

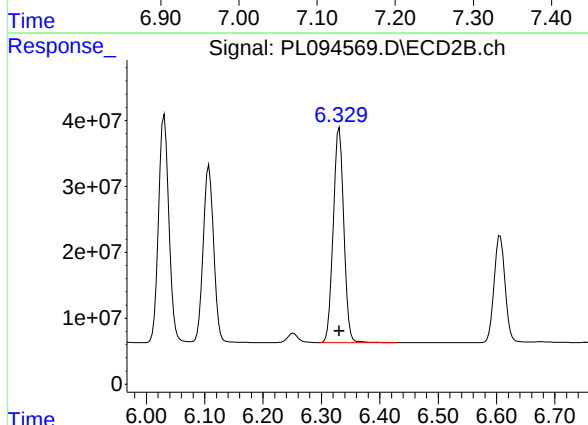


#19 Endosulfan Sulfate

R.T.: 6.330 min
Delta R.T.: 0.000 min
Response: 411435976
Conc: 101.00 ng/ml

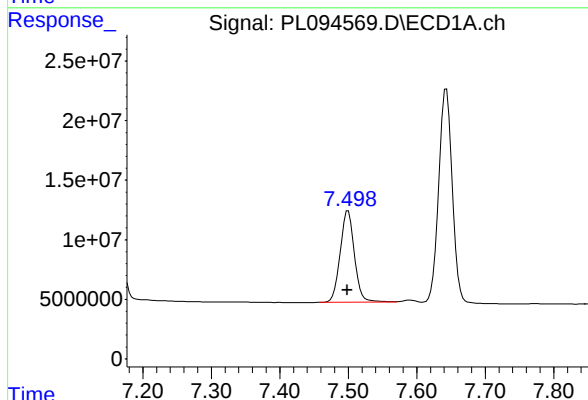


#20 Methoxychlor

R.T.: 7.498 min
Delta R.T.: 0.000 min
Response: 110916911
Conc: 98.02 ng/ml m

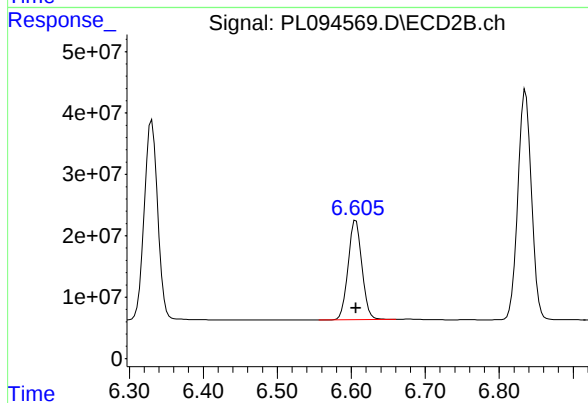

#20 Methoxychlor

R.T.: 6.606 min
Delta R.T.: 0.000 min
Response: 208916485
Conc: 99.76 ng/ml

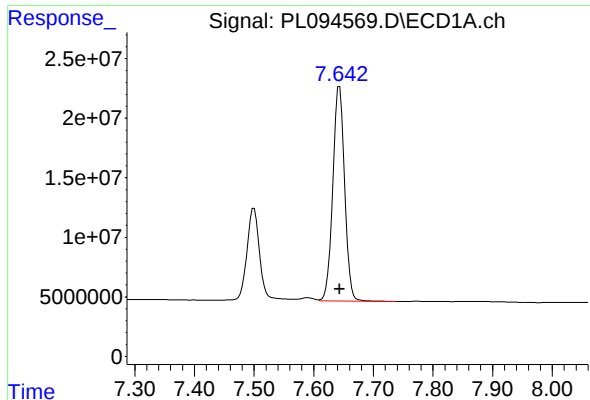


#21 Endrin ketone

R.T.: 7.643 min
Delta R.T.: 0.000 min
Response: 248530773
Conc: 99.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

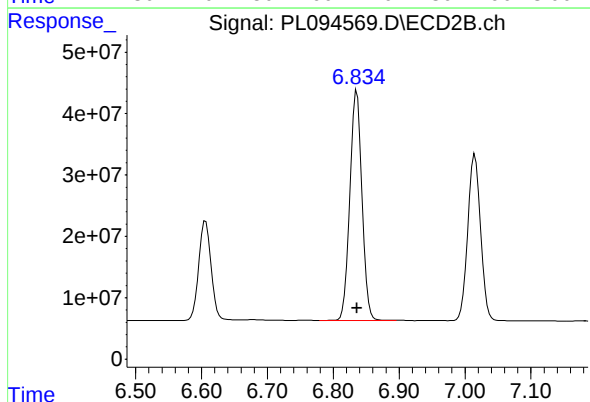


#21 Endrin ketone

R.T.: 6.836 min
Delta R.T.: 0.000 min
Response: 478749237
Conc: 100.84 ng/ml

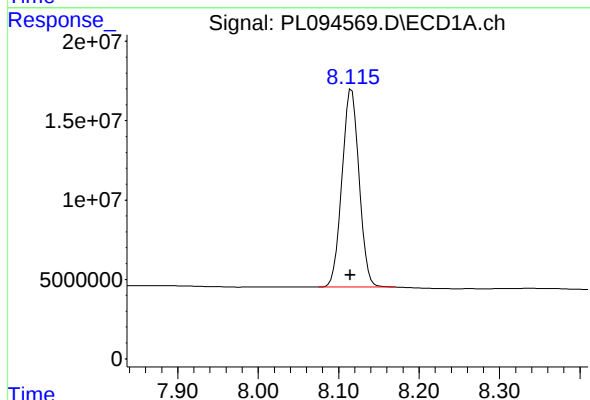


#22 Mirex

R.T.: 8.115 min
Delta R.T.: 0.000 min
Response: 184356457
Conc: 96.82 ng/ml m

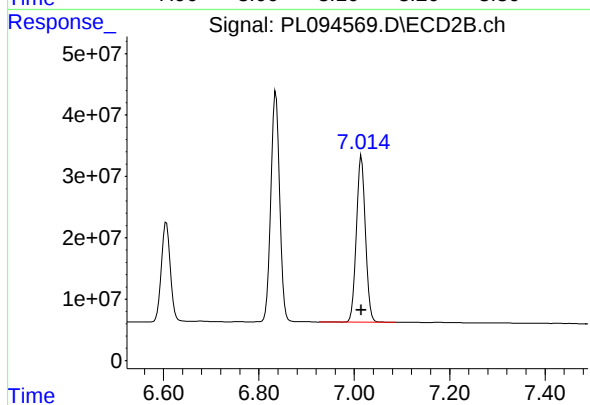

#22 Mirex

R.T.: 7.015 min
Delta R.T.: 0.000 min
Response: 365572908
Conc: 99.62 ng/ml

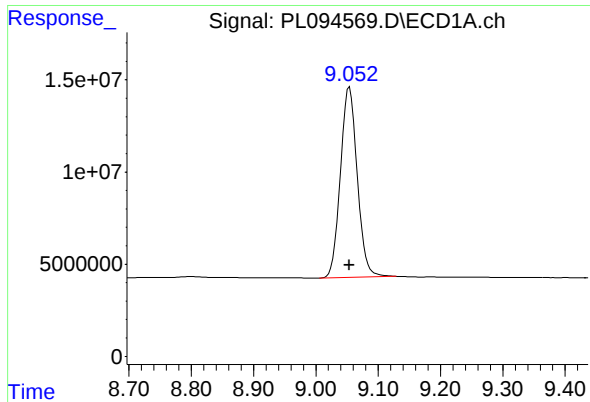


#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 193896231
Conc: 97.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC100

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

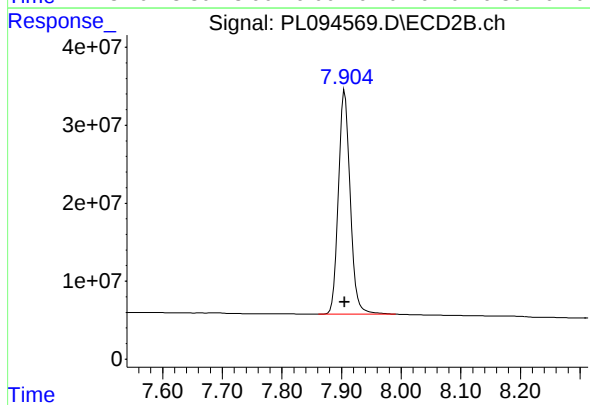

#28 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: 0.000 min
Response: 395031656
Conc: 100.59 ng/ml