
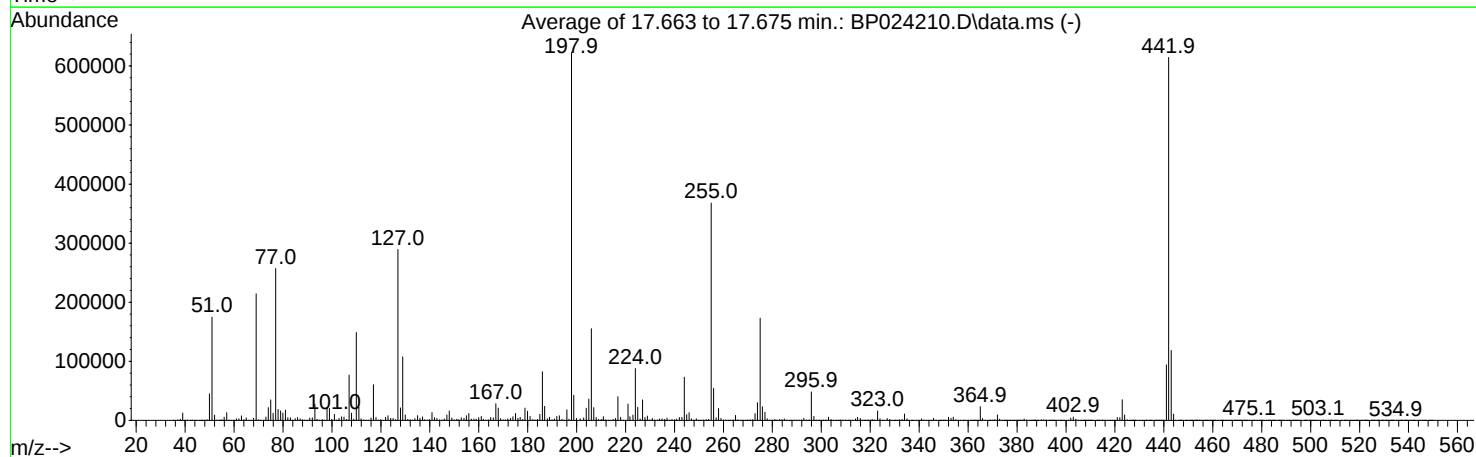


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024210.D
Acq On : 08 Apr 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 05:55:58 2025

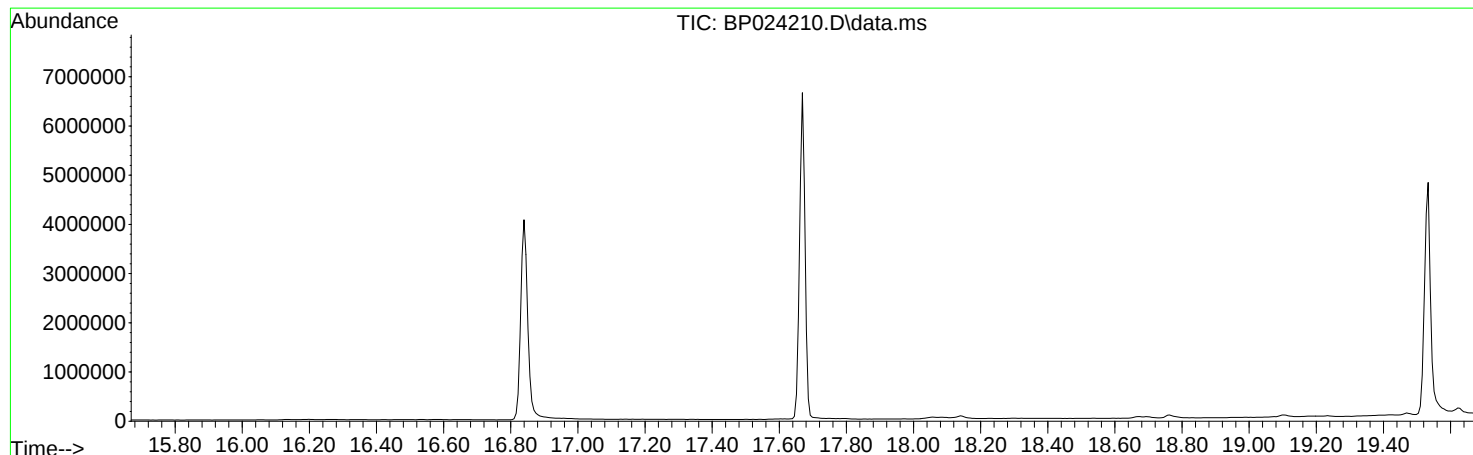




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	174652	PASS
68	69	0.00	2	1.7	3637	PASS
69	198	0.00	100	34.4	214278	PASS
70	69	0.00	2	0.6	1205	PASS
127	198	10	80	46.5	289331	PASS
197	198	0.00	2	0.3	1809	PASS
198	198	100	100	100.0	622847	PASS
199	198	5	9	6.8	42471	PASS
275	198	10	60	27.8	173014	PASS
365	198	1	100	3.7	23221	PASS
441	198	0.01	100	15.1	94130	PASS
442	442	100	100	100.0	614391	PASS
443	442	15	24	19.3	118355	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024210.D
Acq On : 08 Apr 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 08 18:25:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

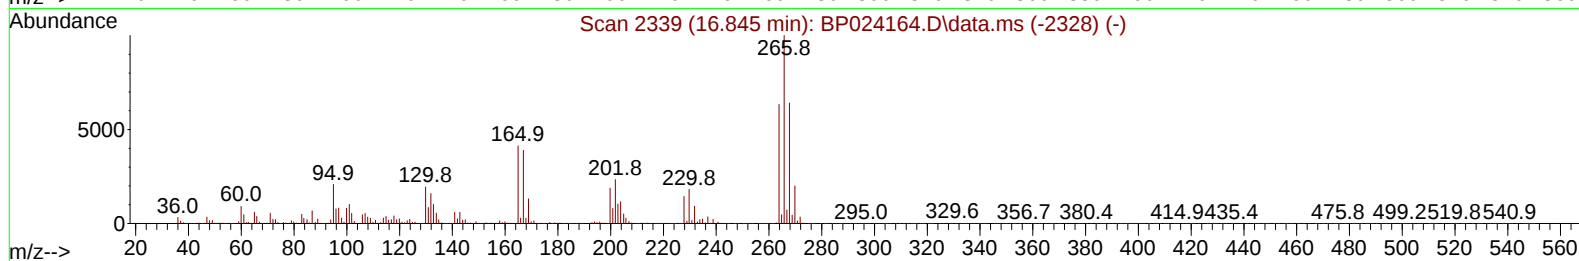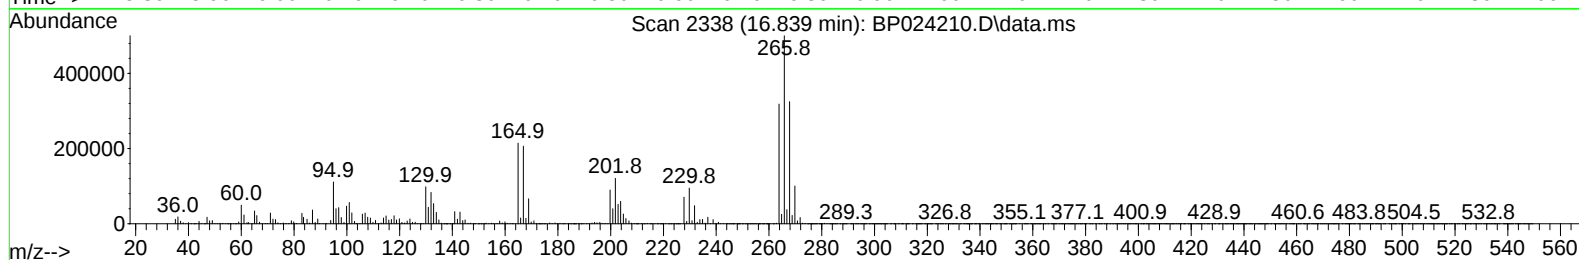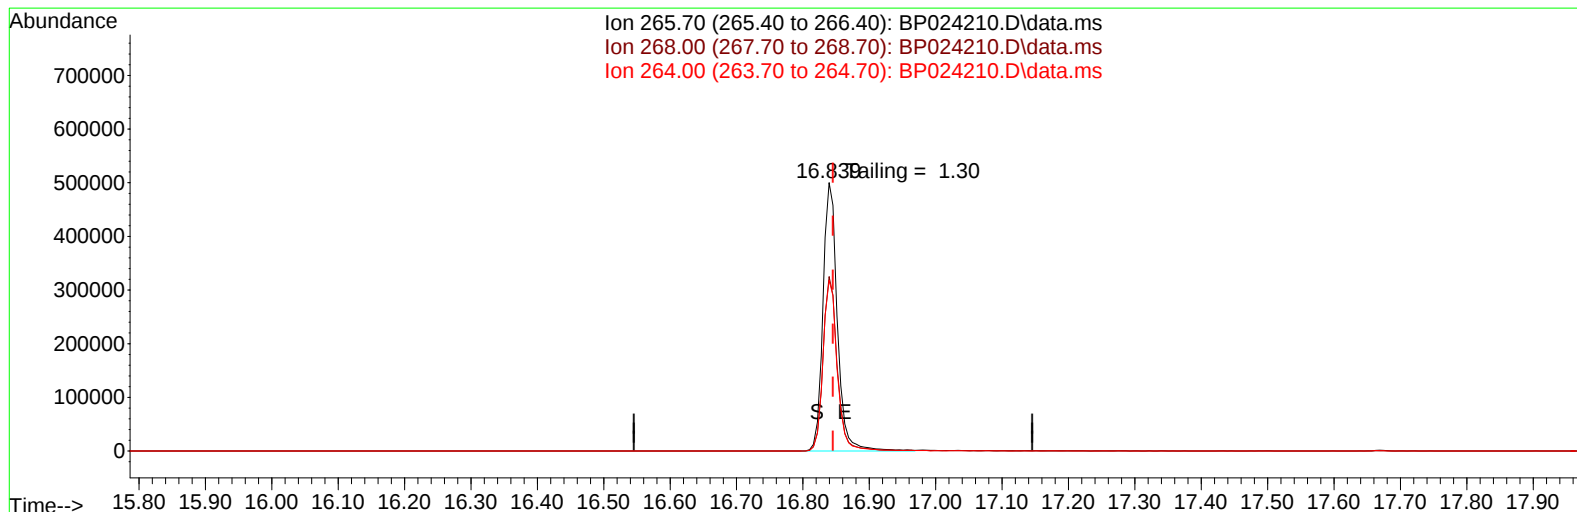

TIC: BP024210.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.006) 277531.82 ng




response **753321**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.97
264.00	63.30	63.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024210.D
Acq On : 08 Apr 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 08 18:25:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

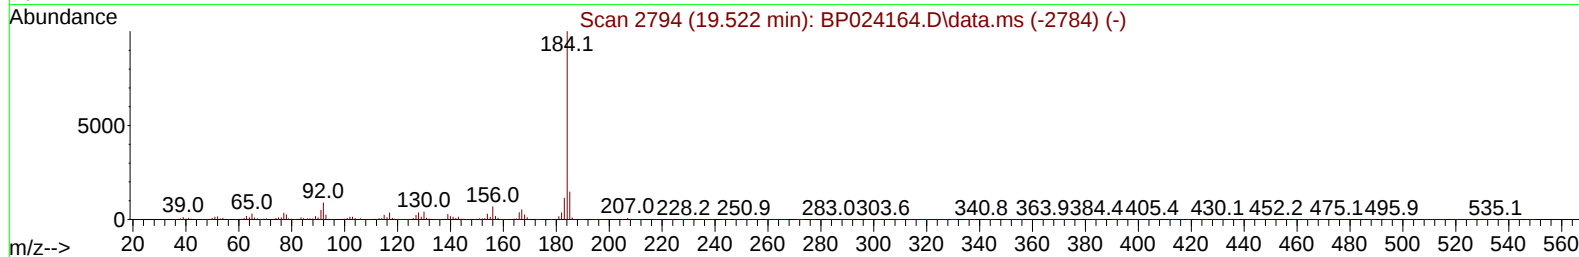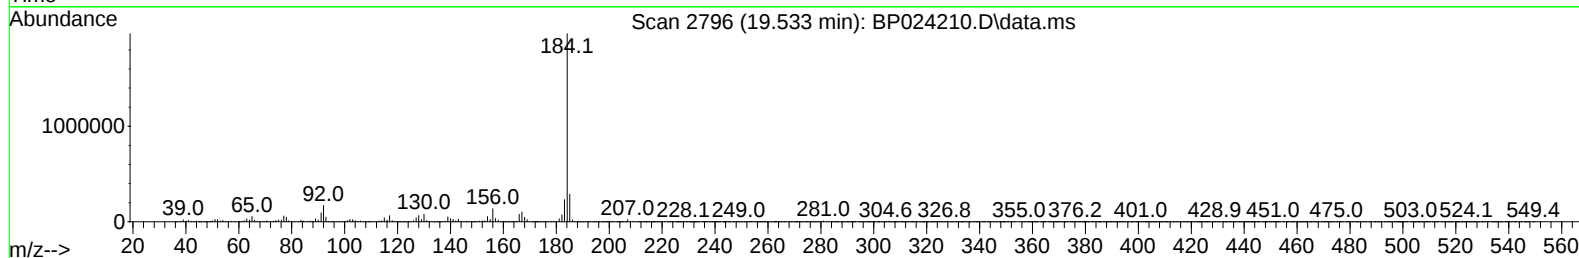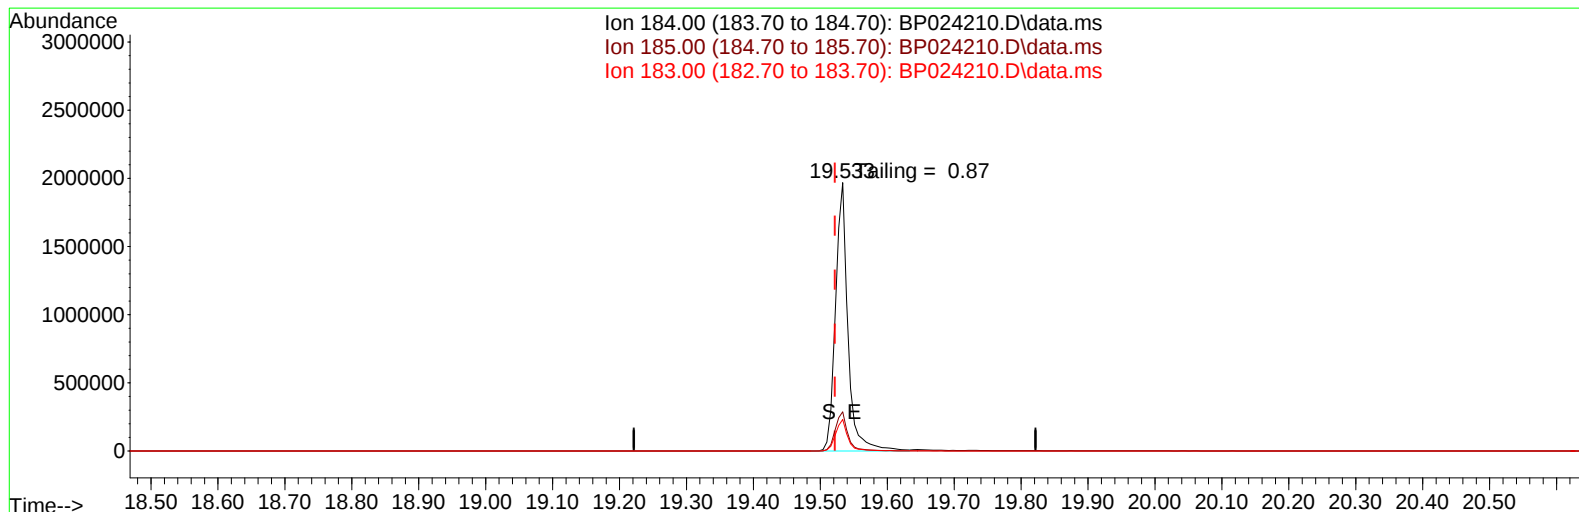

TIC: BP024210.D\data.ms

(77) Benzidine

19.533min (+ 0.012) 6521.01 ng

response 2548937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.65
183.00	11.40	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2025	BNA_P	<u>BP024210.D</u>
Compound Name	Response	Retention Time
DDT	2066235	20.833
DDD	33084	20.369
DDE	4231	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37315	2103550	1.77

Instrument :
BNA_P
ClientSampleId :
DFTPP