

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following "Results Qualifiers" are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as "12 B".
E	Indicates the analyte 's concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	Q1736	OrderDate:	4/4/2025 1:39:00 PM
Client:	G Environmental	Project:	Stockton
Contact:	Gary Landis	Location:	L21

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1736-01	GST1	SOIL	PCB	8082A	04/04/25	04/07/25	04/07/25	04/04/25
Q1736-02	GST2	SOIL	PCB	8082A	04/04/25	04/07/25	04/07/25	04/04/25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q1736

Order ID: Q1736

Client: G Environmental

Project ID: Stockton

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: **Q1736**

Client: **G Environmental**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PO109971.D	PIBLK-PO109971.D	Tetrachloro-m-xylene	1	20	18.5	93		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	20.0	100		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	18.6	93		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	21.3	107		70 (60)	130 (140)
I.BLK-PO110267.D	PIBLK-PO110267.D	Tetrachloro-m-xylene	1	20	19.5	97		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	18.4	92		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	18.8	94		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	15.9	79		70 (60)	130 (140)
Q1730-03MS	OU4-VSL-16-040325MS	Tetrachloro-m-xylene	1	20	22.8	114		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	20.9	104		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	21.8	109		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	18.0	90		30 (32)	150 (175)
Q1730-03MSD	OU4-VSL-16-040325MSD	Tetrachloro-m-xylene	1	20	21.6	108		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	19.8	99		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	20.8	104		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	17.3	86		30 (32)	150 (175)
Q1736-01	GST1	Tetrachloro-m-xylene	1	20	15.2	76		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	9.68	48		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	15.1	75		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	8.71	44		30 (32)	150 (175)
Q1736-02	GST2	Tetrachloro-m-xylene	1	20	20.1	100		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	14.9	75		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	18.6	93		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	13.6	68		30 (32)	150 (175)
I.BLK-PO110282.D	PIBLK-PO110282.D	Tetrachloro-m-xylene	1	20	19.3	97		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	17.2	86		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	18.8	94		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	16.2	81		70 (60)	130 (140)
PB167469BL	PB167469BL	Tetrachloro-m-xylene	1	20	19.0	95		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	17.3	86		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	18.3	91		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	16.0	80		30 (32)	150 (175)
PB167469BS	PB167469BS	Tetrachloro-m-xylene	1	20	19.9	99		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	19.1	95		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	18.9	95		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	17.3	86		30 (32)	150 (175)
I.BLK-PO110290.D	PIBLK-PO110290.D	Tetrachloro-m-xylene	1	20	19.5	98		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	17.7	89		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	18.9	94		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	16.2	81		70 (60)	130 (140)

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q1736

Client: G Environmental

Analytical Method: 8082A

DataFile : PO110271.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID: OU4-VSL-16-040325MS												
Q1730-03MS	AR1016	176.1	0	170	ug/kg	97				40 (55)	140 (146)	
	AR1260	176.1	0	157	ug/kg	89				40 (31)	140 (146)	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q1736

Client: G Environmental

Analytical Method: 8082A

DataFile : PO110272.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	OU4-VSL-16-040325MSD											
Q1730-03MSD	AR1016	176.2	0	164	ug/kg	93		4		40 (55)	140 (146)	30 (20)
	AR1260	176.2	0	153	ug/kg	87		2		40 (31)	140 (146)	30 (20)



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q1736

Client: G Environmental

Analytical Method: 8082A **Datafile :** PO110284.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB167469BS	AR1016	166.6	141	ug/kg	85				40 (71)	140 (120)	
	AR1260	166.6	134	ug/kg	80				40 (65)	140 (130)	

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB167469BL

Lab Name: CHEMTECH

Contract: GENV01

Lab Code: CHEM Case No.: Q1736

SAS No.: Q1736 SDG NO.: Q1736

Lab Sample ID: PB167469BL

Lab File ID: PO110283.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 04/07/2025

Date Analyzed (1): 04/07/2025

Date Analyzed (2): 04/07/2025

Time Analyzed (1): 19:22

Time Analyzed (2): 19:22

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
OU4-VSL-16-040325MS	Q1730-03MS	PO110271.D	04/07/2025	04/07/2025
OU4-VSL-16-040325MSD	Q1730-03MSD	PO110272.D	04/07/2025	04/07/2025
GST1	Q1736-01	PO110273.D	04/07/2025	04/07/2025
GST2	Q1736-02	PO110274.D	04/07/2025	04/07/2025
PB167469BS	PB167469BS	PO110284.D	04/07/2025	04/07/2025

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	G Environmental	Date Collected:	04/04/25
Project:	Stockton	Date Received:	04/04/25
Client Sample ID:	GST1	SDG No.:	Q1736
Lab Sample ID:	Q1736-01	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	78.6
Sample Wt/Vol:	30.07	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110273.D	1	04/07/25 08:20	04/07/25 14:51	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	5.00	U	5.00	21.6	ug/kg
11104-28-2	Aroclor-1221	5.10	U	5.10	21.6	ug/kg
11141-16-5	Aroclor-1232	4.70	U	4.70	21.6	ug/kg
53469-21-9	Aroclor-1242	5.10	U	5.10	21.6	ug/kg
12672-29-6	Aroclor-1248	7.50	U	7.50	21.6	ug/kg
11097-69-1	Aroclor-1254	4.10	U	4.10	21.6	ug/kg
37324-23-5	Aroclor-1262	6.40	U	6.40	21.6	ug/kg
11100-14-4	Aroclor-1268	4.60	U	4.60	21.6	ug/kg
11096-82-5	Aroclor-1260	4.10	U	4.10	21.6	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	15.2		30 (32) - 150 (144)	76%	SPK: 20
2051-24-3	Decachlorobiphenyl	9.68		30 (32) - 150 (175)	48%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
Data File : P0110273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 14:51
Operator : YP/AJ
Sample : Q1736-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
GST1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 16:23:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.688	138.0E6	78987499	15.161	15.062
2) SA Decachlor...	8.741	8.692	74450560	21138313	9.683	8.713

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 14:51
Operator : YP/AJ
Sample : Q1736-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
GST1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 16:23:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

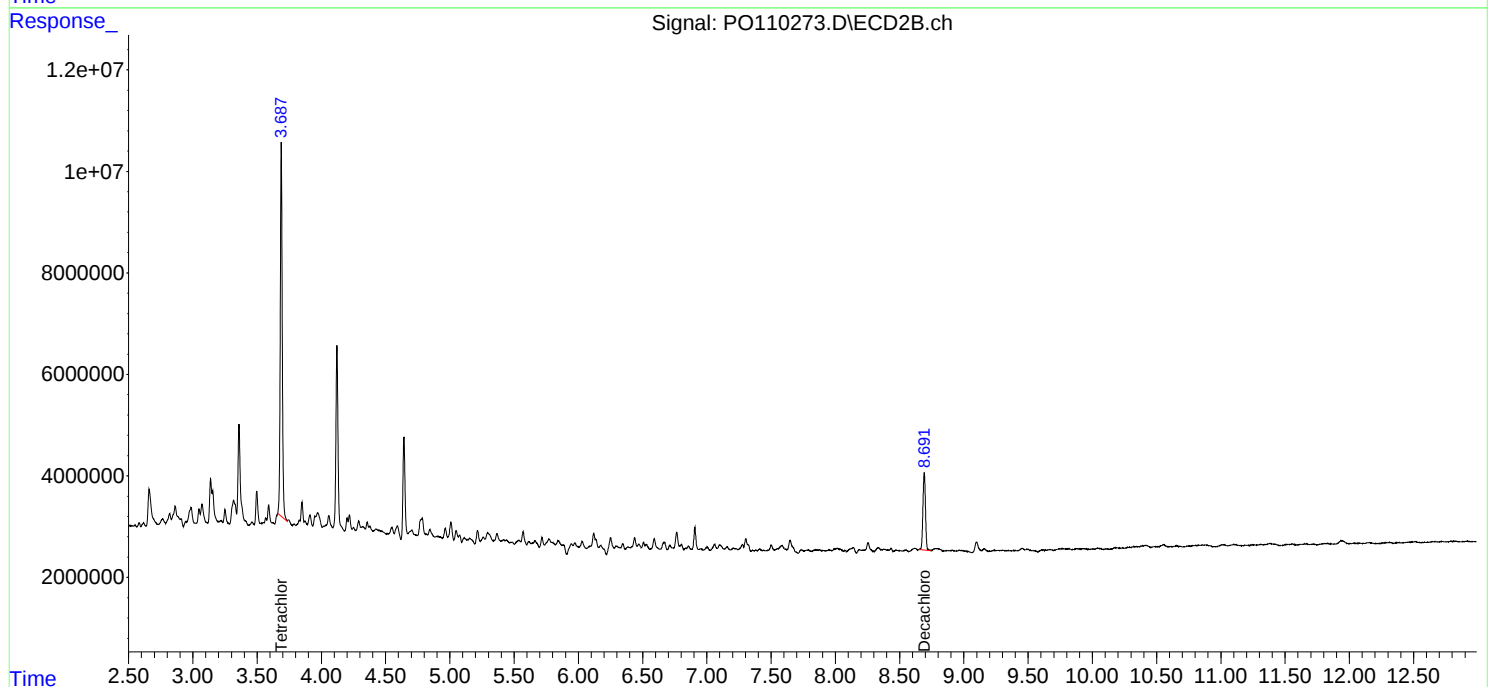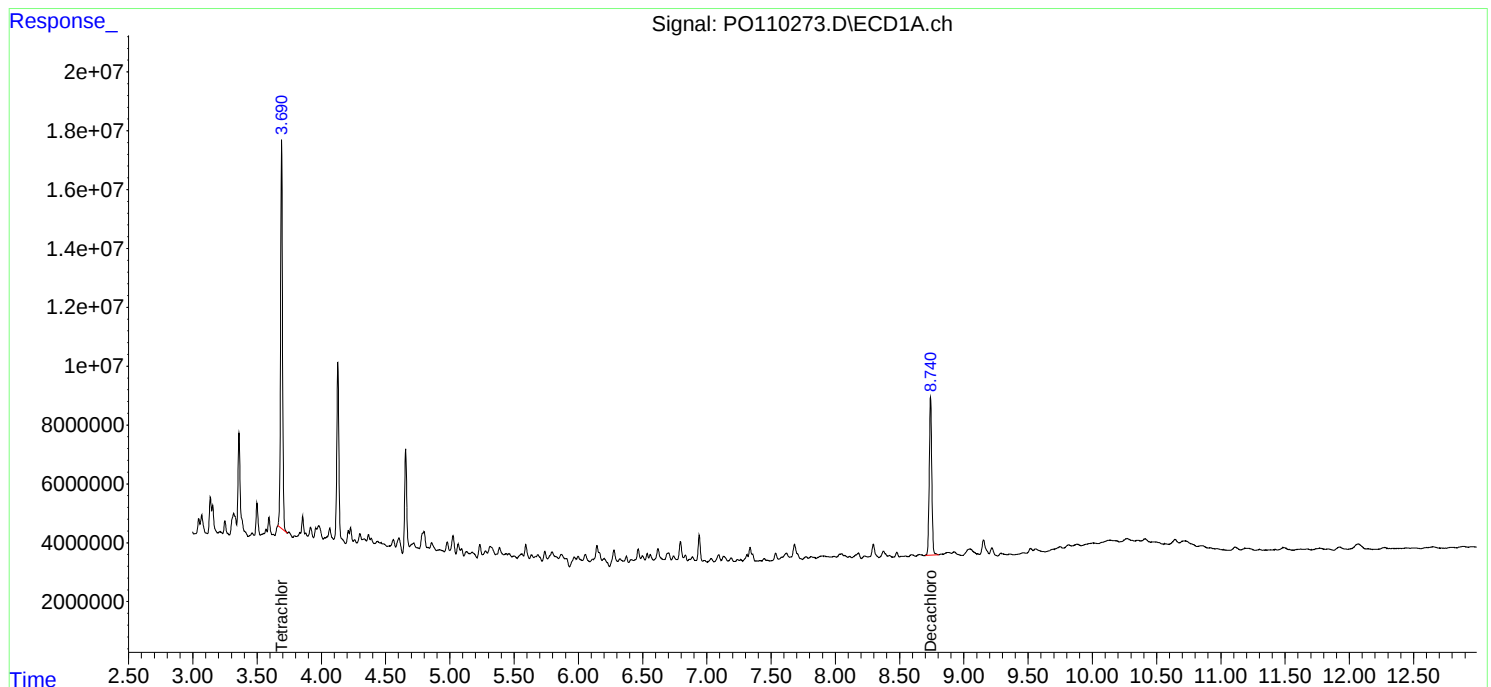


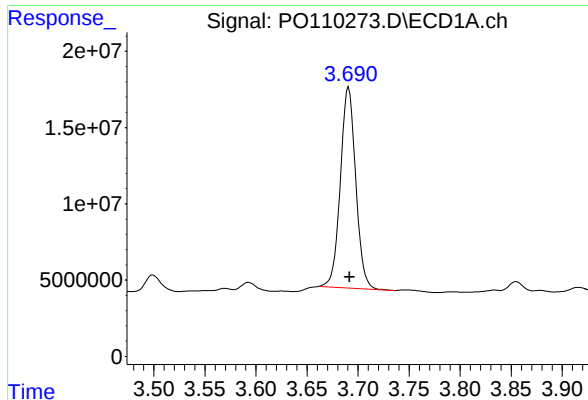

#1 Tetrachloro-m-xylene


R.T.: 3.691 min
Delta R.T.: -0.001 min
Response: 137986145
Conc: 15.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
GST1

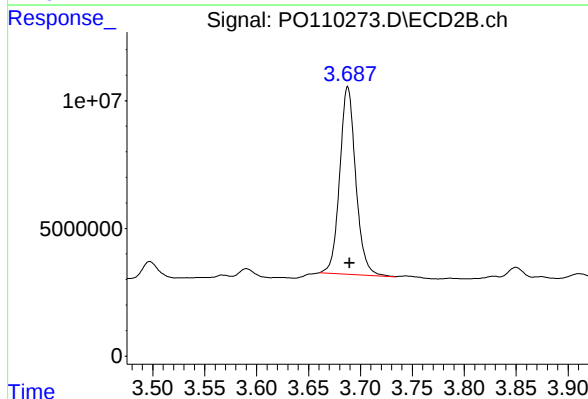


#1 Tetrachloro-m-xylene

R.T.: 3.688 min
Delta R.T.: -0.002 min
Response: 78987499
Conc: 15.06 ng/ml

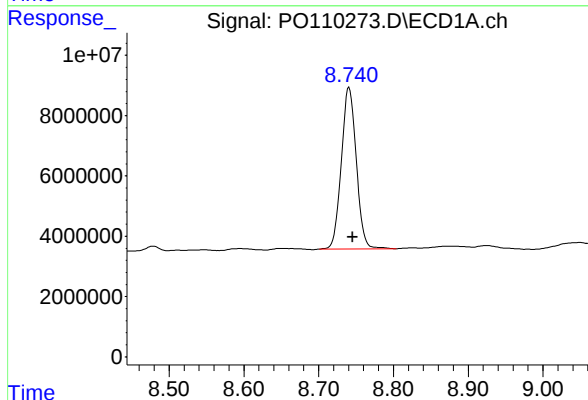

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.005 min
Response: 74450560
Conc: 9.68 ng/ml

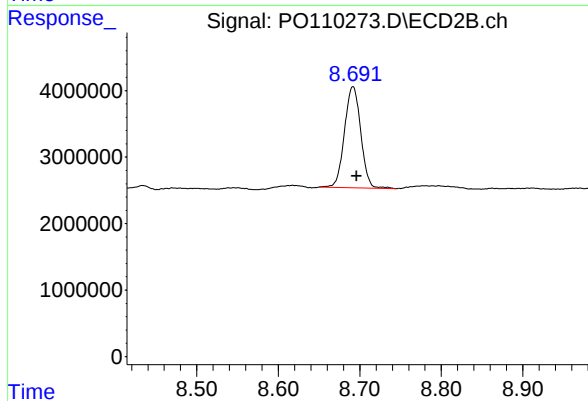

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: -0.004 min
Response: 21138313
Conc: 8.71 ng/ml

Report of Analysis

Client:	G Environmental		Date Collected:	04/04/25	
Project:	Stockton		Date Received:	04/04/25	
Client Sample ID:	GST2		SDG No.:	Q1736	
Lab Sample ID:	Q1736-02		Matrix:	SOIL	
Analytical Method:	SW8082A		% Solid:	80.5	Decanted:
Sample Wt/Vol:	30.03	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110274.D	1	04/07/25 08:20	04/07/25 15:10	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.90	U	4.90	21.1	ug/kg
11104-28-2	Aroclor-1221	5.00	U	5.00	21.1	ug/kg
11141-16-5	Aroclor-1232	4.60	U	4.60	21.1	ug/kg
53469-21-9	Aroclor-1242	5.00	U	5.00	21.1	ug/kg
12672-29-6	Aroclor-1248	7.30	U	7.30	21.1	ug/kg
11097-69-1	Aroclor-1254	4.00	U	4.00	21.1	ug/kg
37324-23-5	Aroclor-1262	6.20	U	6.20	21.1	ug/kg
11100-14-4	Aroclor-1268	4.50	U	4.50	21.1	ug/kg
11096-82-5	Aroclor-1260	4.00	U	4.00	21.1	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.1		30 (32) - 150 (144)	100%	SPK: 20
2051-24-3	Decachlorobiphenyl	14.9		30 (32) - 150 (175)	75%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 15:10
 Operator : YP/AJ
 Sample : Q1736-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GST2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 16:24:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	3.688	182.9E6	97720958	20.095	18.634
2) SA Decachlor...	8.741	8.692	114.6E6	32972583	14.911	13.591

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 15:10
Operator : YP/AJ
Sample : Q1736-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
GST2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 16:24:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

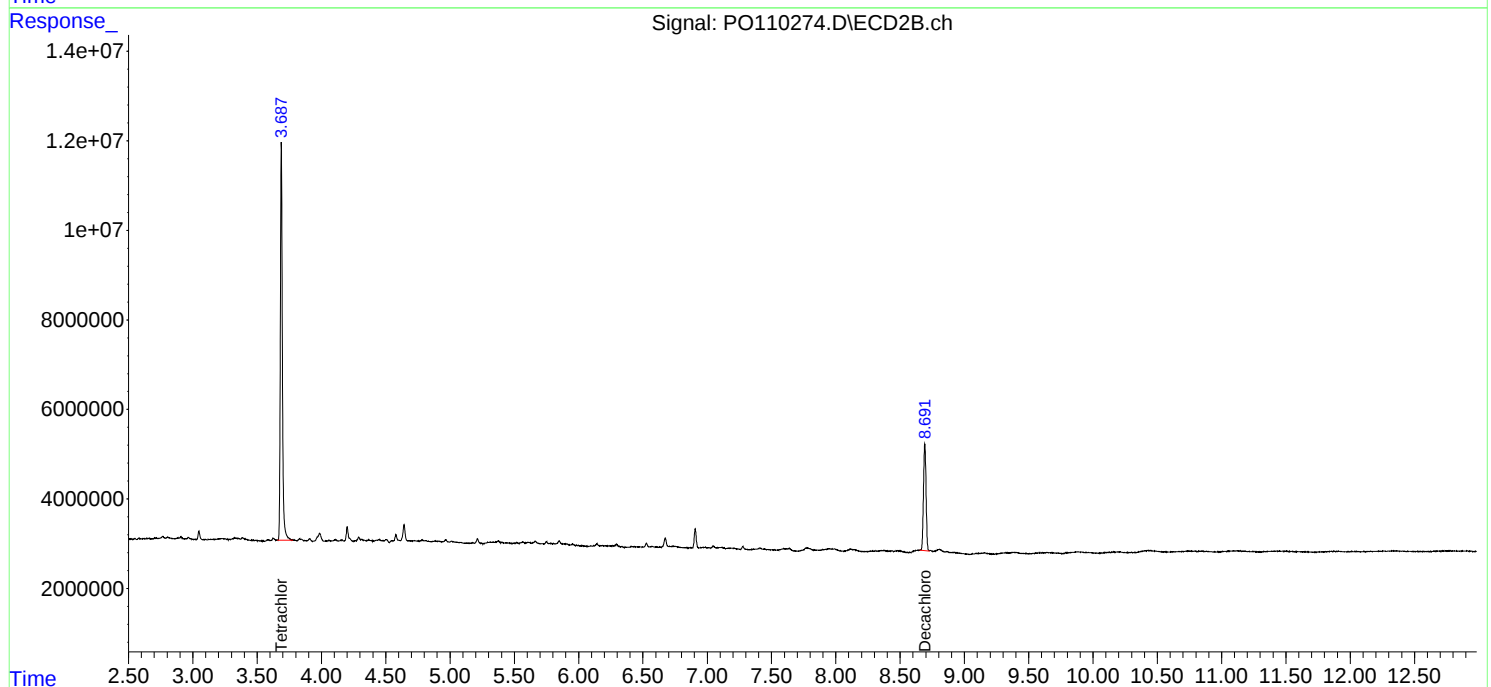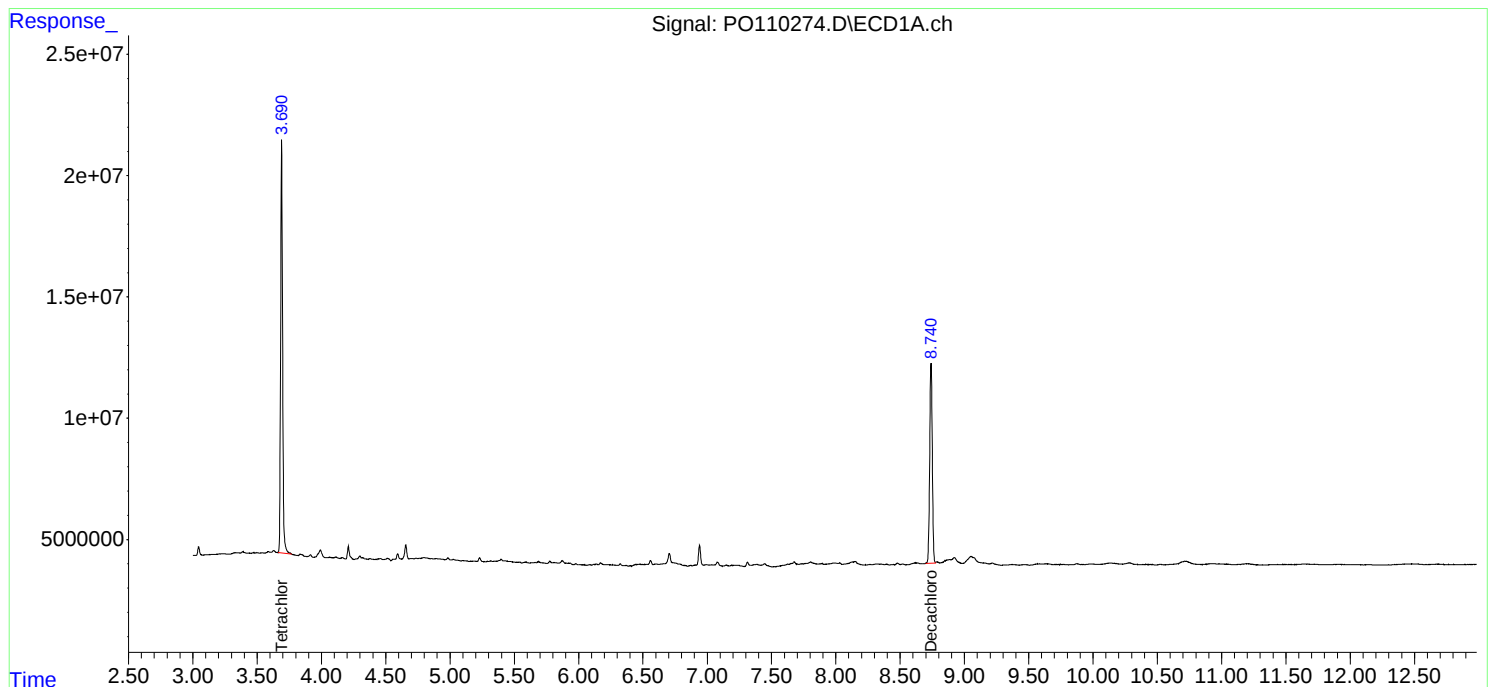


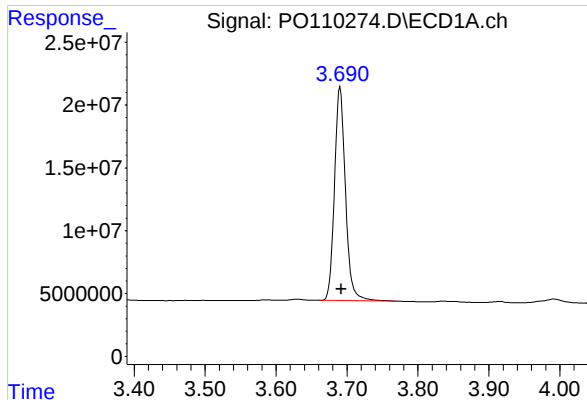

#1 Tetrachloro-m-xylene


R.T.: 3.690 min
Delta R.T.: -0.002 min
Response: 182892057
Conc: 20.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
GST2

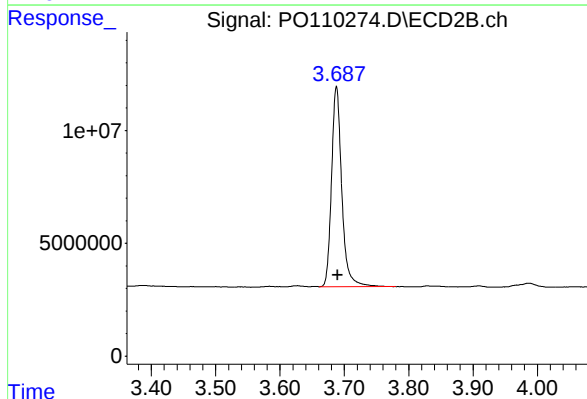


#1 Tetrachloro-m-xylene

R.T.: 3.688 min
Delta R.T.: -0.002 min
Response: 97720958
Conc: 18.63 ng/ml

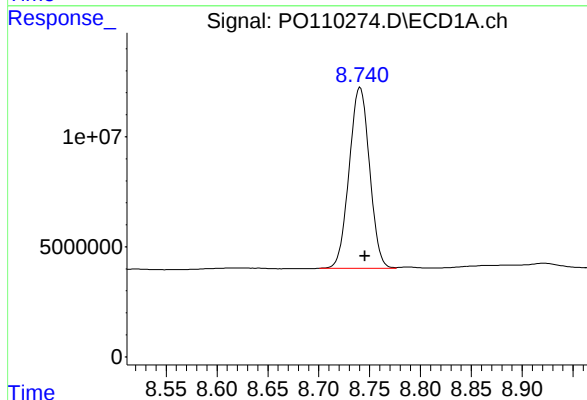

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.005 min
Response: 114647248
Conc: 14.91 ng/ml

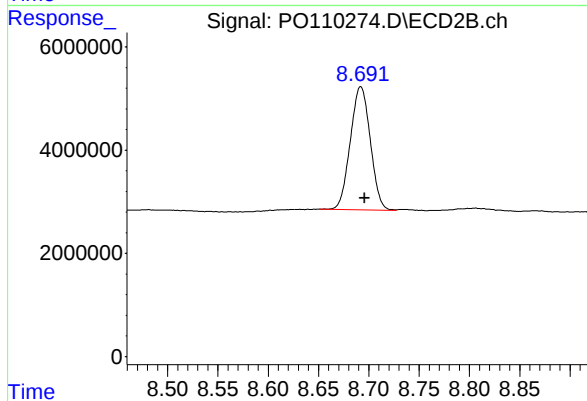

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: -0.004 min
Response: 32972583
Conc: 13.59 ng/ml



CALIBRATION SUMMARY

GC Column: ZB-MR1 ID: 0.32 (mm)

[illegible]

[illegible]

GC Column: ZB-MR2 ID: 0.32 (mm)

[illegible]

[illegible]

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: GENV01
Lab Code: CHEM **Case No.:** Q1736 **SAS No.:** Q1736 **SDG NO.:** Q1736
Instrument ID: ECD_O **Calibration Date(s):** 03/18/2025 03/18/2025
Calibration Times: 14:03 22:15

GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO109972.D</u>		CF 750 = <u>PO109973.D</u>			
CF 500 = <u>PO109974.D</u>		CF 250 = <u>PO109975.D</u>		CF 050 = <u>PO109976.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	318793340	329109113	342176988	354587888	338053060	336544078
Aroclor-1016-2	(2)	446388679	463709840	475172436	492289896	440868120	463685794
Aroclor-1016-3	(3)	297123739	311570976	324283686	341714956	328237360	320586143
Aroclor-1016-4	(4)	237983440	248526219	257445742	268101480	251389660	252689308
Aroclor-1016-5	(5)	250501585	263674729	272727188	289617476	297814400	274867076
Aroclor-1260-1	(1)	448474074	467586512	475904282	500944916	463845060	471350969
Aroclor-1260-2	(2)	549756400	573035712	574538170	604900316	675365020	595519124
Aroclor-1260-3	(3)	466244522	483474499	486507370	506233648	484047880	485301584
Aroclor-1260-4	(4)	395577993	413728377	429812132	453058452	428662340	424167859
Aroclor-1260-5	(5)	1037246832	1067855560	1076605366	1088369780	959152240	1045845956
Decachlorobiphenyl		7314268770	7585202853	7715836840	8064386520	7763558800	7688650757
Tetrachloro-m-xylene		9191618080	9409704013	9556350980	9350200040	7999627400	9101500103
Aroclor-1242-1	(1)	257021206	271242037	274350776	287750984	246670040	267407009
Aroclor-1242-2	(2)	361656206	376061644	380771426	397296944	325229300	368203104
Aroclor-1242-3	(3)	239272274	256595597	260500336	277304732	256081460	257950880
Aroclor-1242-4	(4)	191269111	202702439	206227546	215710620	184561000	200094143
Aroclor-1242-5	(5)	200342595	212233400	219728410	230305716	192670380	211056100
Decachlorobiphenyl		7073021470	7288055093	7382383840	7783557400	6481660800	7201735721
Tetrachloro-m-xylene		8702773030	8995385800	8954862760	9053765120	6655083400	8472374022
Aroclor-1248-1	(1)	203222777	210833551	219941524	231478528	236936100	220482496
Aroclor-1248-2	(2)	271717932	285234192	301067598	320199420	327717760	301187380
Aroclor-1248-3	(3)	341855080	357243465	374409124	395224264	397211640	373188715
Aroclor-1248-4	(4)	484718685	503724613	523274664	543824872	584555460	528019659
Aroclor-1248-5	(5)	341874536	354831647	369725290	387414496	410903120	372949818
Decachlorobiphenyl		7279802030	7532134600	7794766540	8111831880	8262032800	7796113570
Tetrachloro-m-xylene		8896906280	9107530813	9275989780	9374608920	8757655400	9082538239
Aroclor-1254-1	(1)	527461301	541865743	559314886	571016624	626589000	565249511
Aroclor-1254-2	(2)	454907170	469007857	483702014	470938584	527635000	481238125
Aroclor-1254-3	(3)	753626169	772675721	789277352	760170300	789680960	773086100
Aroclor-1254-4	(4)	465418236	477798716	486446390	499614064	471424900	480140461
Aroclor-1254-5	(5)	652046620	666447925	680525202	682124008	569584060	650145563
Decachlorobiphenyl		7506577390	7722603000	7867257780	8042146160	8253331200	7878383106
Tetrachloro-m-xylene		9124017490	9264222013	9387241720	8732477200	8689133000	9039418285
Aroclor-1268-1	(1)	1369838059	1374439380	1401378006	1431422640	1423576940	1400131005



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	1266296617	1262736967	1279632688	1321583800	1270503560	1280150726	2
Aroclor-1268-3	(3)	1019701747	1019547960	1038648586	1056461448	1003450380	1027562024	2
Aroclor-1268-4	(4)	432675859	421354135	447439086	473337560	435173000	441995928	4
Aroclor-1268-5	(5)	3202130253	3192211076	3228608174	3247761892	3036317900	3181405859	3
Decachlorobiphenyl		13640006290	13735597093	14120230440	14566780400	14594697800	14131462405	3
Tetrachloro-m-xylene		9016621250	8994153573	9277514520	9319153840	8874982800	9096485197	2



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Instrument ID: ECD_O

Calibration Date(s): 03/18/2025 03/18/2025

Calibration Times: 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO109972.D</u>		CF 750 = <u>PO109973.D</u>			
CF 500 = <u>PO109974.D</u>		CF 250 = <u>PO109975.D</u>		CF 050 = <u>PO109976.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	173731434	178393712	185954312	194985500	183209860	4
Aroclor-1016-2	(2)	252919767	260842944	268062016	276298580	249399140	4
Aroclor-1016-3	(3)	134029267	138651783	144331354	150165168	141715700	4
Aroclor-1016-4	(4)	107671732	112396073	118651742	125867636	125061600	7
Aroclor-1016-5	(5)	141734749	147685869	153486032	162580972	159105760	6
Aroclor-1260-1	(1)	240074381	247747439	258832620	273383796	257170920	5
Aroclor-1260-2	(2)	281757793	288999419	301276956	315867360	313526020	5
Aroclor-1260-3	(3)	267611935	278954948	288530668	305847736	303966000	6
Aroclor-1260-4	(4)	196048044	205344145	218294872	229292036	226412760	7
Aroclor-1260-5	(5)	481983300	481761991	513782868	520791536	495161780	4
Decachlorobiphenyl		2314898720	2277821173	2432747880	2620033760	2485044400	6
Tetrachloro-m-xylene		5279380900	5378354400	5480250420	5516817960	4565680000	7
Aroclor-1242-1	(1)	141331278	146781083	150759024	159963196	132242600	7
Aroclor-1242-2	(2)	205951481	214434265	215763772	224841412	179186640	8
Aroclor-1242-3	(3)	108828803	114341291	116166340	122887996	95840060	9
Aroclor-1242-4	(4)	107629937	113953347	117437436	126339948	114521460	6
Aroclor-1242-5	(5)	132486572	139043136	144664964	152408060	117607760	10
Decachlorobiphenyl		2177773130	2225931947	2270761420	2435729160	2067519400	6
Tetrachloro-m-xylene		5049304150	5177204613	5163887520	5207194080	3529903800	15
Aroclor-1248-1	(1)	111262575	115666484	120322434	126703700	133730220	7
Aroclor-1248-2	(2)	153166873	160144767	168518512	179835124	180628540	7
Aroclor-1248-3	(3)	163639212	170966695	179105274	191715488	200520960	8
Aroclor-1248-4	(4)	192034431	200649257	208567738	223057368	227978540	7
Aroclor-1248-5	(5)	189825244	196639567	203671792	215836044	233387660	8
Decachlorobiphenyl		2147083620	2251559707	2344655820	2535991200	2605882000	8
Tetrachloro-m-xylene		5118943080	5218637120	5295153740	5366945840	5070595200	2
Aroclor-1254-1	(1)	289813236	298739165	307722880	314204860	352998300	8
Aroclor-1254-2	(2)	250736607	259627313	268490268	271062664	307765180	8
Aroclor-1254-3	(3)	402159669	413409125	421207530	415558372	424838600	2
Aroclor-1254-4	(4)	231846868	237861840	244387952	246184552	252577700	3
Aroclor-1254-5	(5)	329301884	337898680	348664586	361298960	302328380	7
Decachlorobiphenyl		2196807900	2276377227	2418572320	2516603360	2645427200	7
Tetrachloro-m-xylene		5207556450	5288727027	5346917000	5051956440	5061201200	3
Aroclor-1268-1	(1)	560759375	568986040	578205714	598591620	620126960	4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	519206129	525348819	532636024	548739284	562258340	537637719	3
Aroclor-1268-3	(3)	397648794	399556300	412917038	427809808	440374680	415661324	4
Aroclor-1268-4	(4)	153792414	154678659	162023954	168698684	166024000	161043542	4
Aroclor-1268-5	(5)	963659212	966574348	987141016	1016062428	1031847640	993056929	3
Decachlorobiphenyl		3902633900	3983566053	4144258760	4413490680	4552839600	4199357799	7
Tetrachloro-m-xylene		5158364110	5158184947	5281917420	5320423880	5129069800	5209592031	2



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Instrument ID: ECD_O Date(s) Analyzed: 03/18/2025 03/18/2025

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.91	3.81	4.01	115828000
		2	3.99	3.89	4.09	86499800
		3	4.07	3.97	4.17	261696000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.07	3.97	4.17	215744000
		2	4.56	4.46	4.66	114786000
		3	4.81	4.71	4.91	211780000
		4	4.98	4.88	5.08	113561000
		5	5.02	4.92	5.12	80454000
Aroclor-1262	500	1	6.84	6.74	6.94	688120000
		2	7.34	7.24	7.44	1191970000
		3	7.62	7.52	7.72	470630000
		4	7.69	7.59	7.79	874576000
		5	8.18	8.08	8.28	394442000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Instrument ID: ECD_O Date(s) Analyzed: 03/18/2025 03/18/2025

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.90	3.80	4.00	66882200
		2	3.99	3.89	4.09	49381600
		3	4.06	3.96	4.16	151684000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.06	3.96	4.16	124093000
		2	4.79	4.69	4.89	120349000
		3	4.97	4.87	5.07	63656000
		4	5.05	4.95	5.15	59341000
		5	5.22	5.12	5.32	63217800
Aroclor-1262	500	1	6.81	6.71	6.91	344312000
		2	7.31	7.21	7.41	537220000
		3	7.59	7.49	7.69	194051000
		4	7.65	7.55	7.75	361786000
		5	8.15	8.05	8.25	141162000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 14:03
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:33:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:30:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.693	3.690	919.2E6	527.9E6	98.055	98.133
2)	SA Decachlor...	8.745	8.696	731.4E6	231.5E6	97.328	97.518
Target Compounds							
3)	L1 AR-1016-1	4.786	4.772	318.8E6	173.7E6	964.622	966.018
4)	L1 AR-1016-2	4.805	4.791	446.4E6	252.9E6	968.766	970.935
5)	L1 AR-1016-3	4.862	4.967	297.1E6	134.0E6	956.293	962.990
6)	L1 AR-1016-4	4.982	5.009	238.0E6	107.7E6	960.716	951.485
7)	L1 AR-1016-5	5.240	5.222	250.5E6	141.7E6	957.522	960.195
31)	L7 AR-1260-1	6.281	6.254	448.5E6	240.1E6	970.326	962.401
32)	L7 AR-1260-2	6.470	6.442	549.8E6	281.8E6	977.958	966.521
33)	L7 AR-1260-3	6.838	6.595	466.2E6	267.6E6	978.732	962.386
34)	L7 AR-1260-4	7.098	7.066	395.6E6	196.0E6	958.524	946.308
35)	L7 AR-1260-5	7.340	7.307	1037.2E6	482.0E6	981.381	968.065


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 14:03
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:33:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:30:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

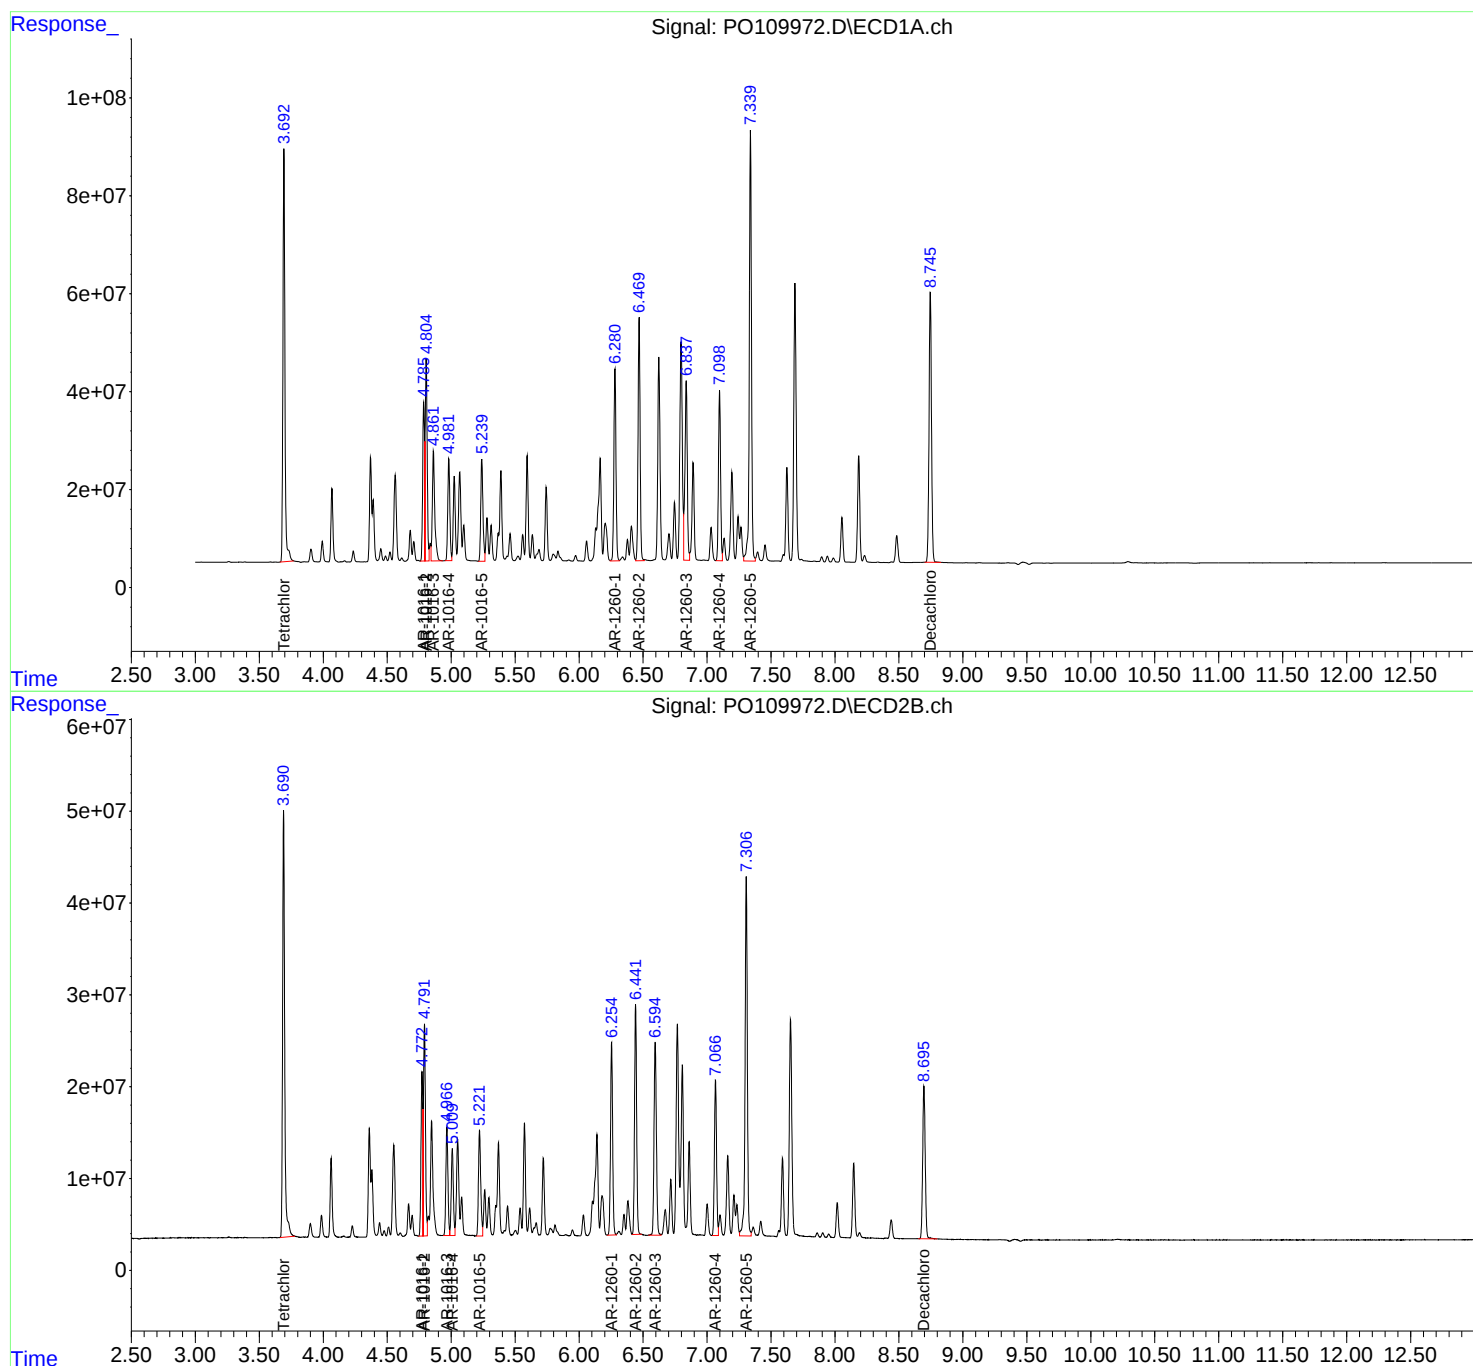

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031925\
 Data File : P0109973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 14:21
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1660ICC750

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:36:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:30:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.693	3.690	705.7E6	403.4E6	75.190	74.986
2) SA Decachlor...	8.745	8.696	568.9E6	170.8E6	75.465	72.950
Target Compounds						
3) L1 AR-1016-1	4.785	4.772	246.8E6	133.8E6	747.915	745.960
4) L1 AR-1016-2	4.805	4.791	347.8E6	195.6E6	753.172	750.675
5) L1 AR-1016-3	4.862	4.967	233.7E6	104.0E6	751.394	748.099
6) L1 AR-1016-4	4.982	5.009	186.4E6	84297055	751.636	746.609
7) L1 AR-1016-5	5.239	5.222	197.8E6	110.8E6	753.927	750.256
31) L7 AR-1260-1	6.280	6.255	350.7E6	185.8E6	755.816	746.573
32) L7 AR-1260-2	6.470	6.442	429.8E6	216.7E6	759.623	745.669
33) L7 AR-1260-3	6.837	6.595	362.6E6	209.2E6	757.414	751.587
34) L7 AR-1260-4	7.098	7.067	310.3E6	154.0E6	751.251	745.577
35) L7 AR-1260-5	7.340	7.307	800.9E6	361.3E6	755.153	735.355m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
Data File : P0109973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 14:21
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:36:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:30:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

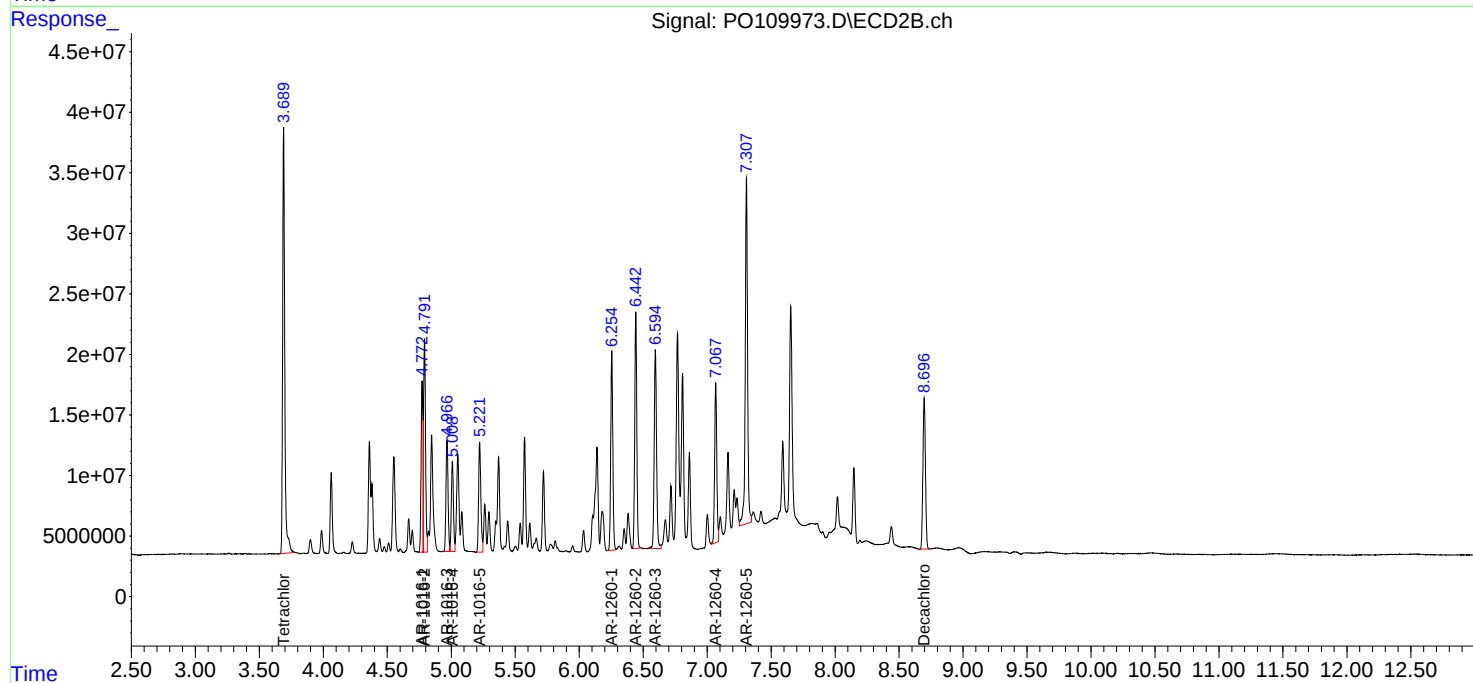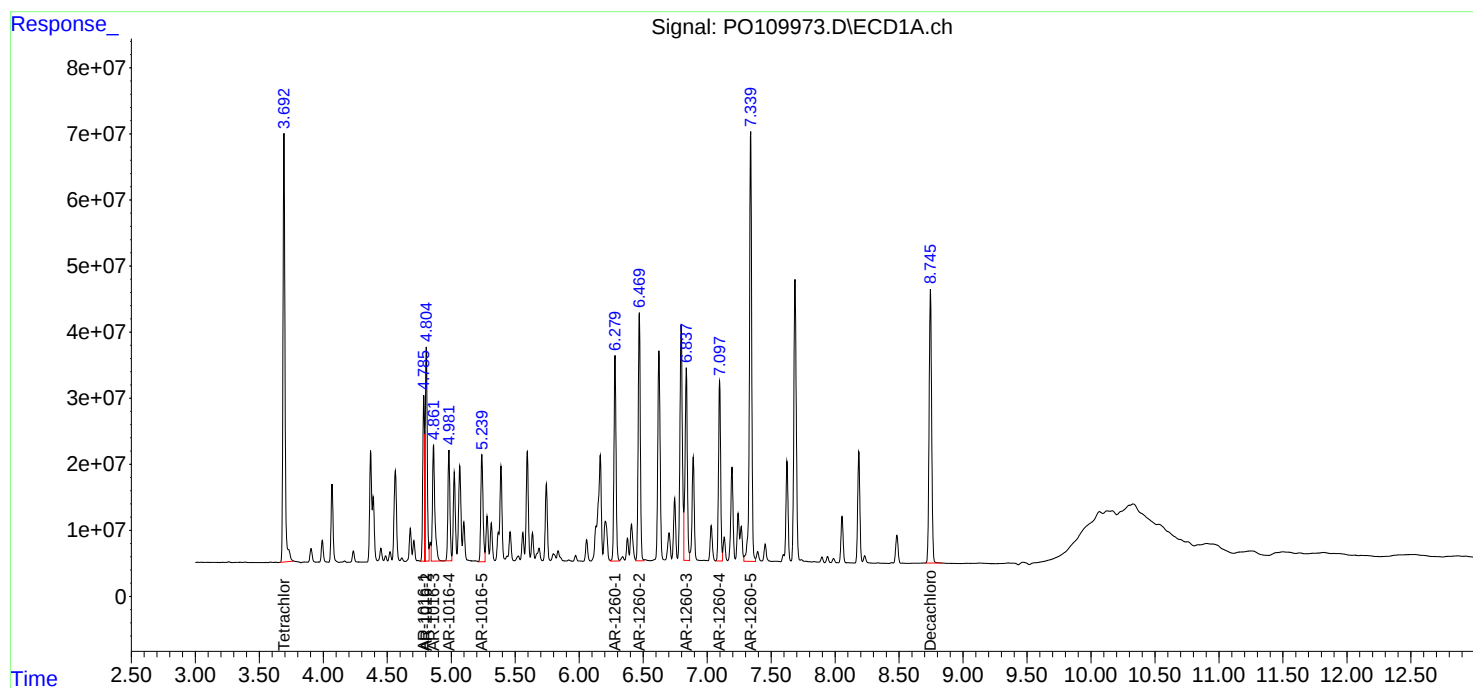

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 14:39
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:30:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:30:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.690	477.8E6	274.0E6	50.000	50.000
2) SA Decachlor...	8.745	8.696	385.8E6	121.6E6	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	4.785	4.772	171.1E6	92977156	500.000	500.000
4) L1 AR-1016-2	4.804	4.791	237.6E6	134.0E6	500.000	500.000
5) L1 AR-1016-3	4.861	4.967	162.1E6	72165677	500.000	500.000
6) L1 AR-1016-4	4.981	5.009	128.7E6	59325871	500.000	500.000
7) L1 AR-1016-5	5.239	5.222	136.4E6	76743016	500.000	500.000
31) L7 AR-1260-1	6.280	6.255	238.0E6	129.4E6	500.000	500.000
32) L7 AR-1260-2	6.469	6.442	287.3E6	150.6E6	500.000	500.000
33) L7 AR-1260-3	6.837	6.595	243.3E6	144.3E6	500.000	500.000
34) L7 AR-1260-4	7.098	7.067	214.9E6	109.1E6	500.000	500.000
35) L7 AR-1260-5	7.339	7.307	538.3E6	256.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
Data File : P0109974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 14:39
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:30:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:30:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

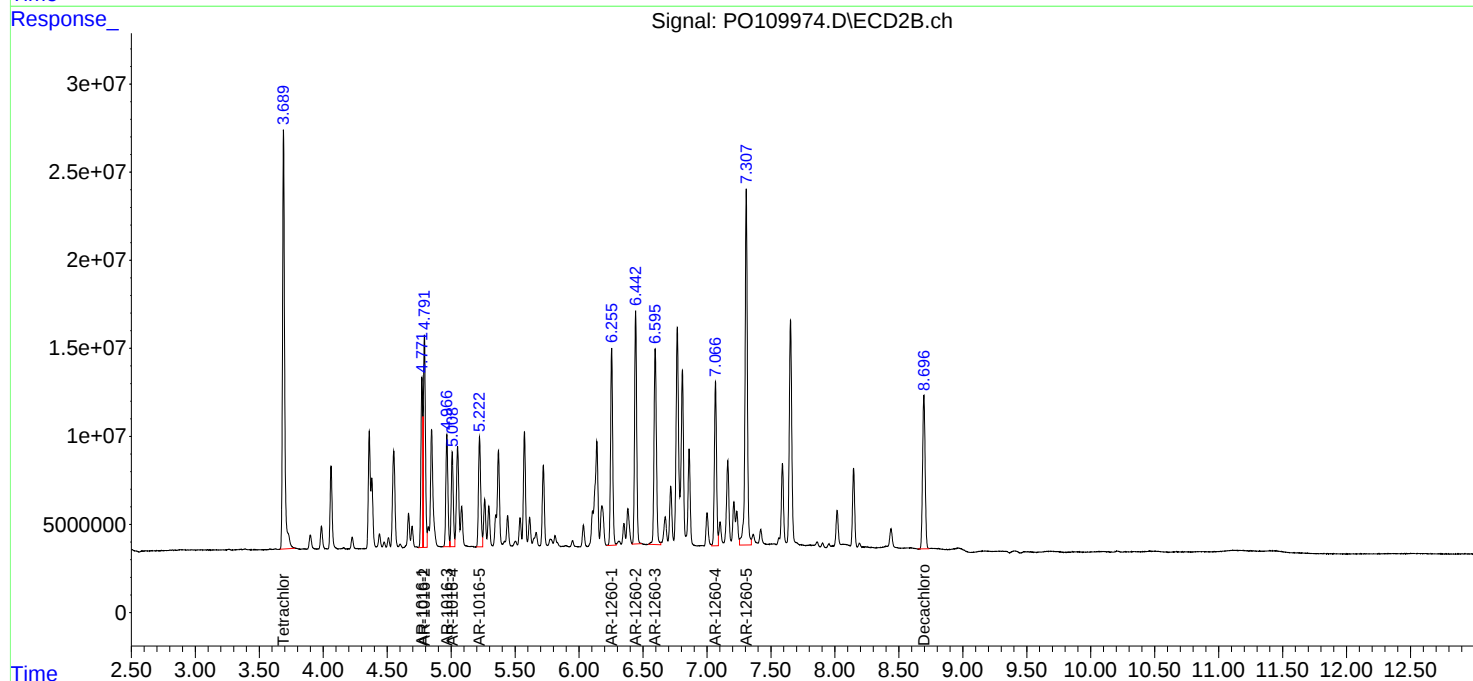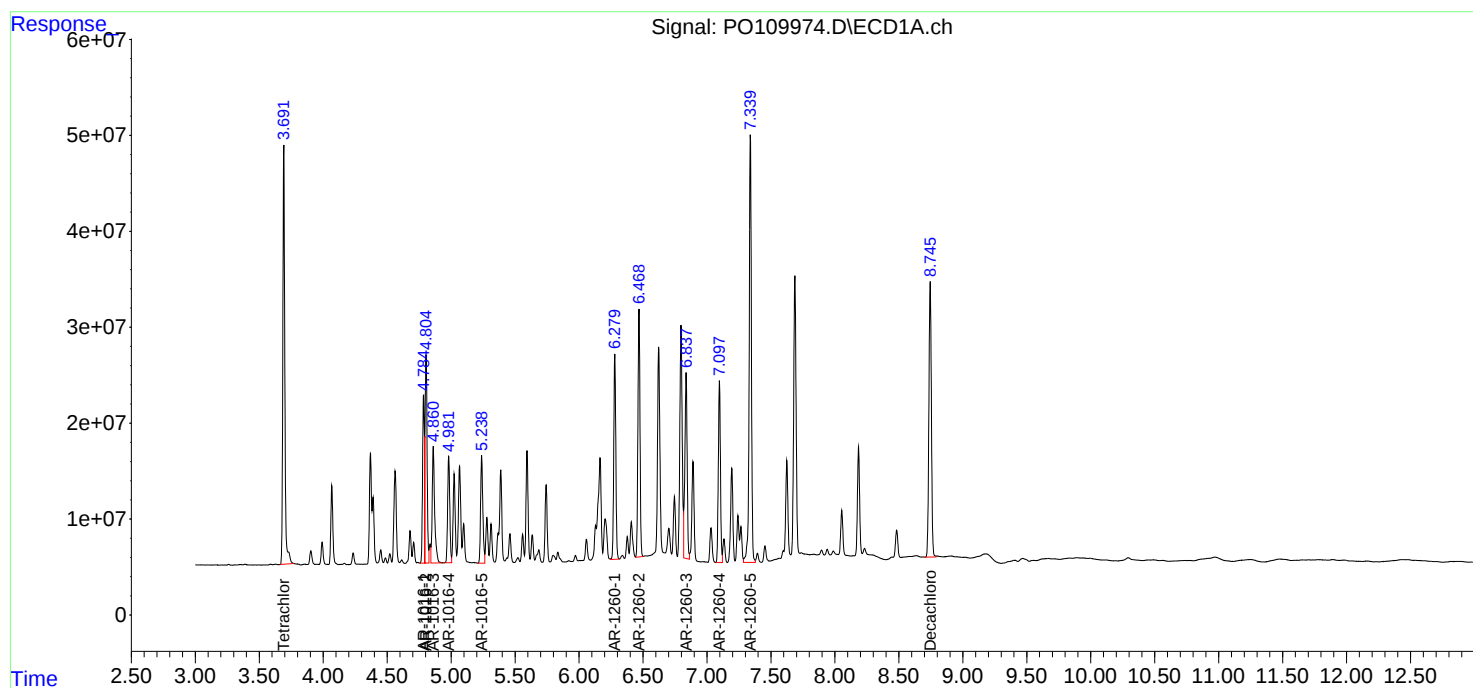

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 14:58
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:39:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:30:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.690	233.8E6	137.9E6	24.929	25.476
2) SA Decachlor...	8.745	8.696	201.6E6	65500844	26.286	27.163
Target Compounds						
3) L1 AR-1016-1	4.785	4.772	88646972	48746375	263.699	265.987
4) L1 AR-1016-2	4.804	4.791	123.1E6	69074645	262.197	261.121
5) L1 AR-1016-3	4.861	4.967	85428739	37541292	268.076	264.759
6) L1 AR-1016-4	4.981	5.009	67025370	31466909	264.908	270.924
7) L1 AR-1016-5	5.239	5.222	72404369	40645243	269.031	268.512
31) L7 AR-1260-1	6.280	6.254	125.2E6	68345949	264.643	268.013
32) L7 AR-1260-2	6.469	6.441	151.2E6	78966840	262.745	265.904
33) L7 AR-1260-3	6.837	6.594	126.6E6	76461934	260.615	268.065
34) L7 AR-1260-4	7.097	7.066	113.3E6	57323009	267.737	270.080
35) L7 AR-1260-5	7.339	7.307	272.1E6	130.2E6	254.883	260.615



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 14:58
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:39:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:30:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

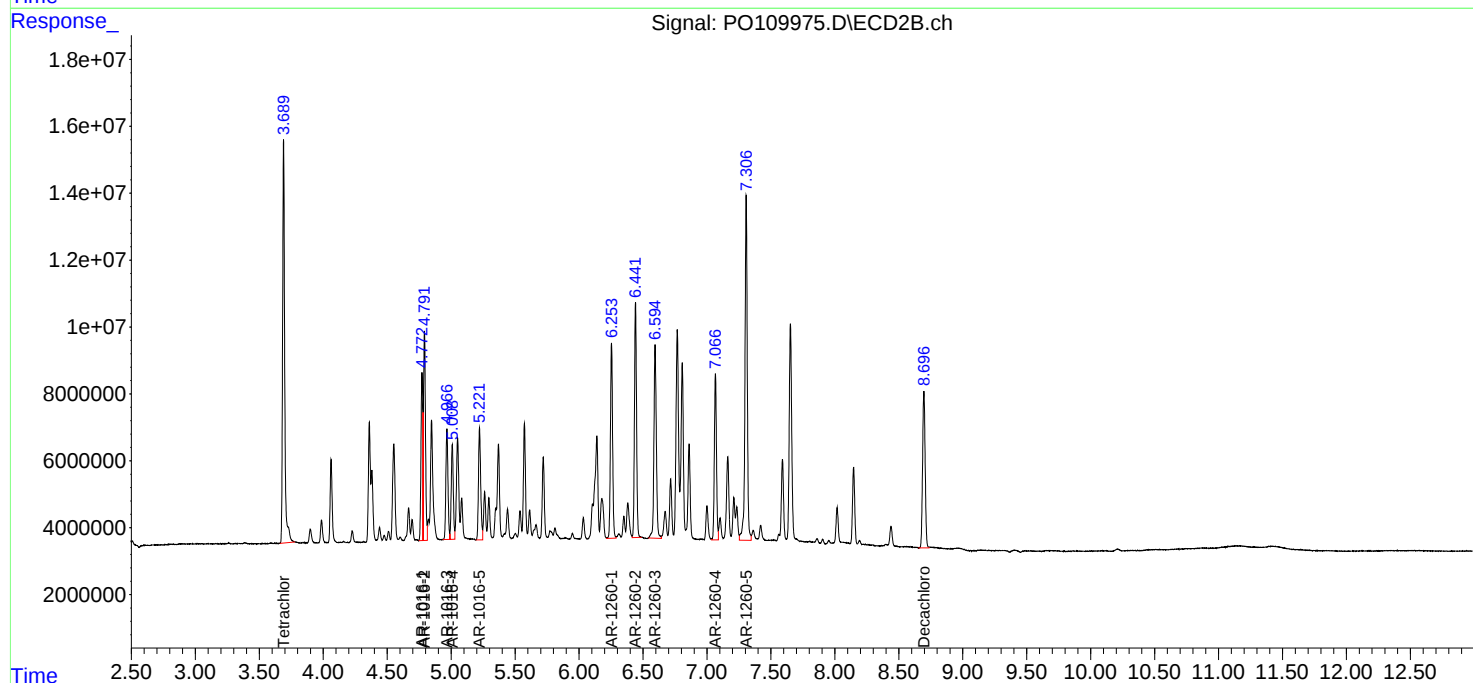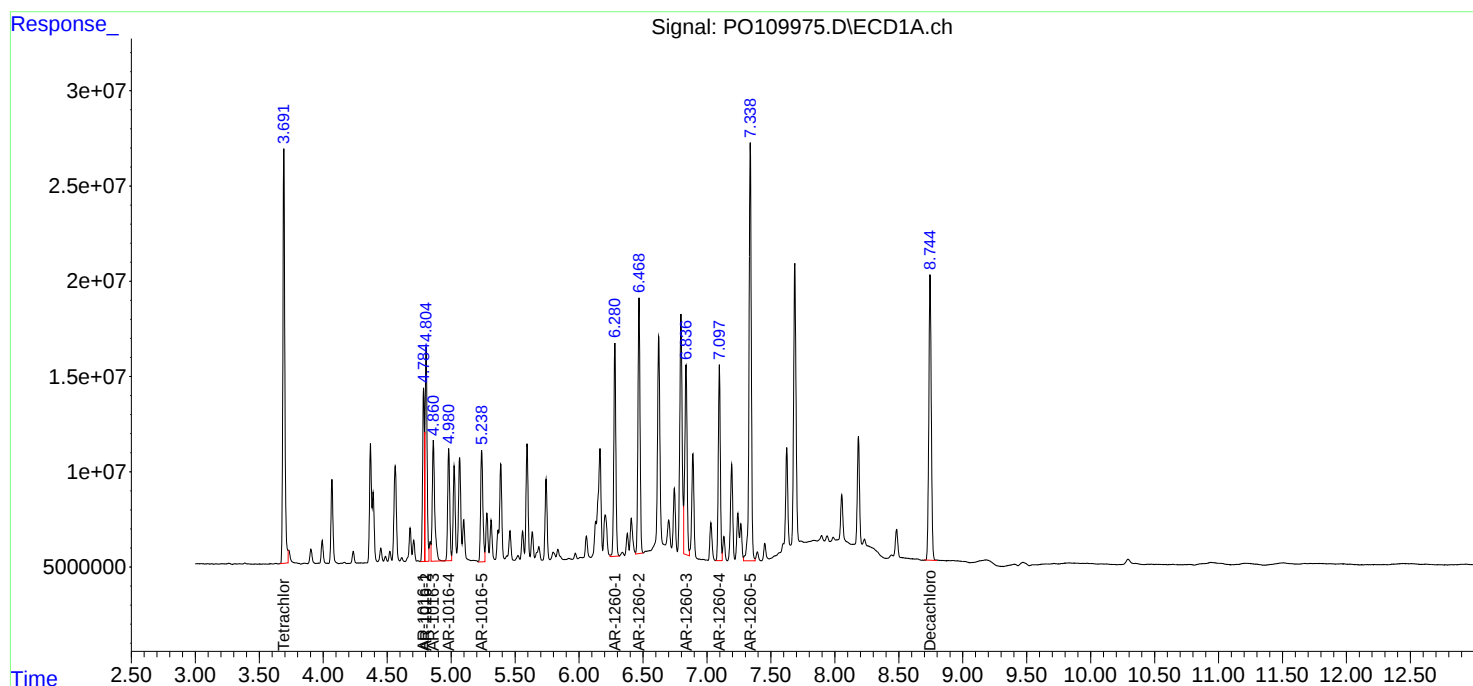

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 15:16
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:42:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:30:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.691	3.688	39998137	22828400	4.395	4.353
2)	SA Decachlor...	8.744	8.695	38817794	12425222	5.049	5.121
Target Compounds							
3)	L1 AR-1016-1	4.784	4.771	16902653	9160493	50.224	49.988
4)	L1 AR-1016-2	4.804	4.790	22043406	12469957	47.540	47.685
5)	L1 AR-1016-3	4.860	4.965	16411868	7085785	51.193	49.978
6)	L1 AR-1016-4	4.981	5.008	12569483	6253080	49.743	53.024
7)	L1 AR-1016-5	5.238	5.220	14890720	7955288	54.174	52.023
31)	L7 AR-1260-1	6.278	6.252	23192253	12858546	48.956m	50.252m
32)	L7 AR-1260-2	6.468	6.441	33768251	15676301	56.704	52.205
33)	L7 AR-1260-3	6.836	6.593	24202394	15198300	49.871	53.072m
34)	L7 AR-1260-4	7.096	7.065	21433117	11320638	50.530	52.635
35)	L7 AR-1260-5	7.339	7.306	47957612	24758089	45.855	49.646

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 15:16
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:42:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:30:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

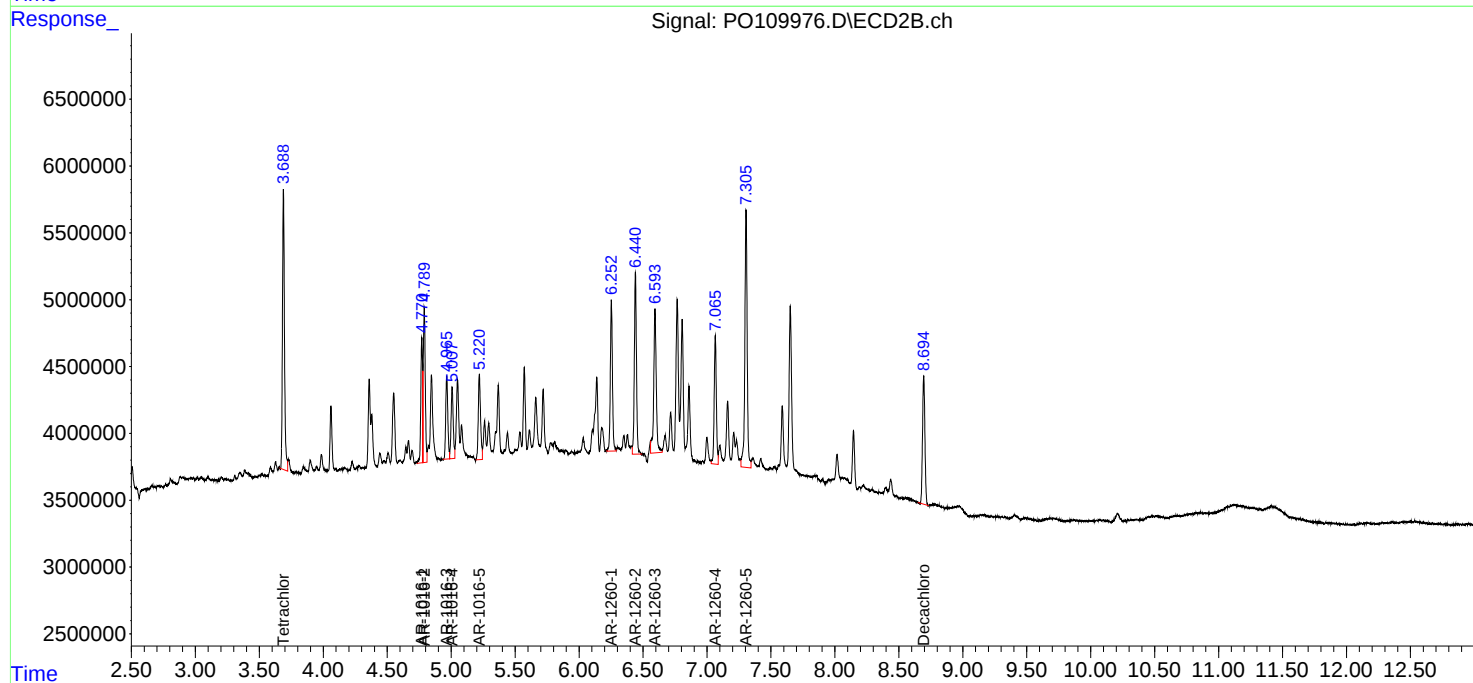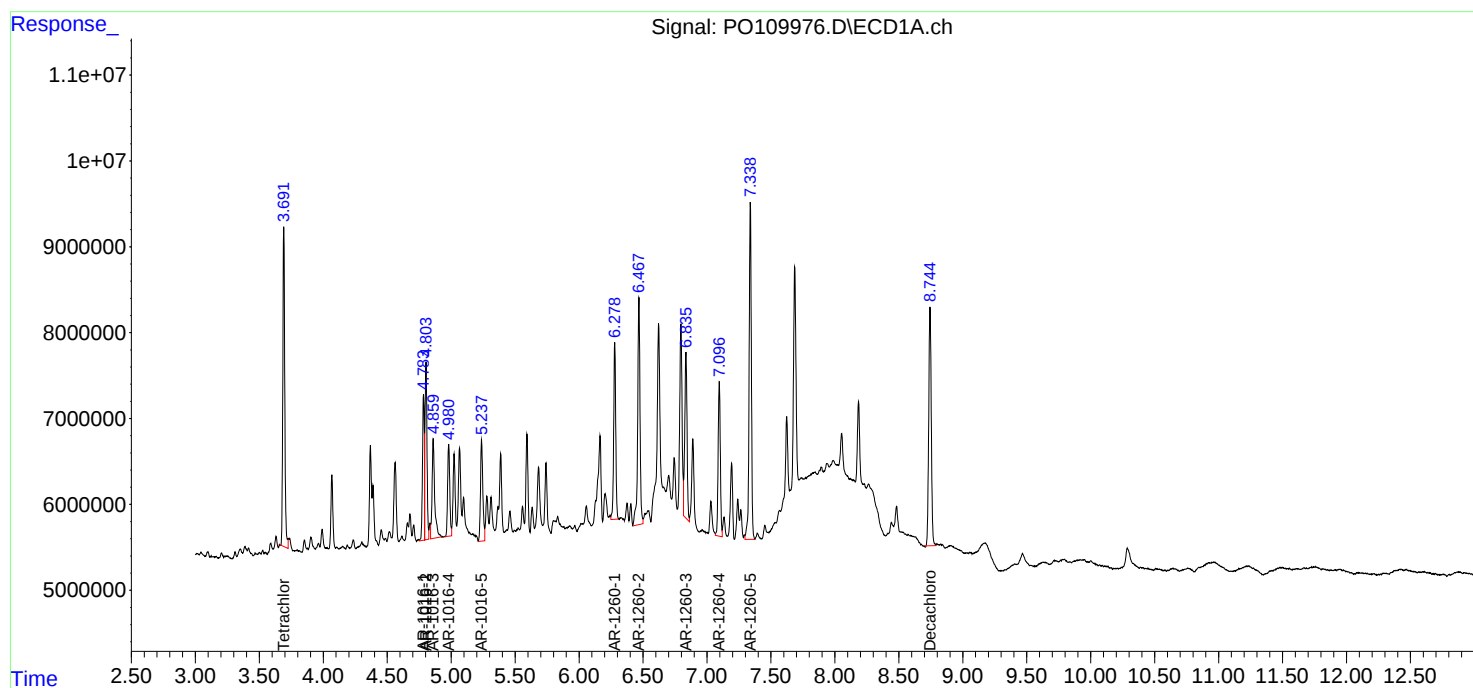

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 15:34
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:27:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:27:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.690	428.4E6	261.3E6	50.000	50.000
2) SA Decachlor...	8.743	8.696	367.0E6	116.0E6	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	3.906	3.901	57914123	33441082	500.000	500.000
9) L2 AR-1221-2	3.992	3.986	43249856	24690825	500.000	500.000
10) L2 AR-1221-3	4.069	4.062	130.8E6	75841971	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 15:34
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:27:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:27:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

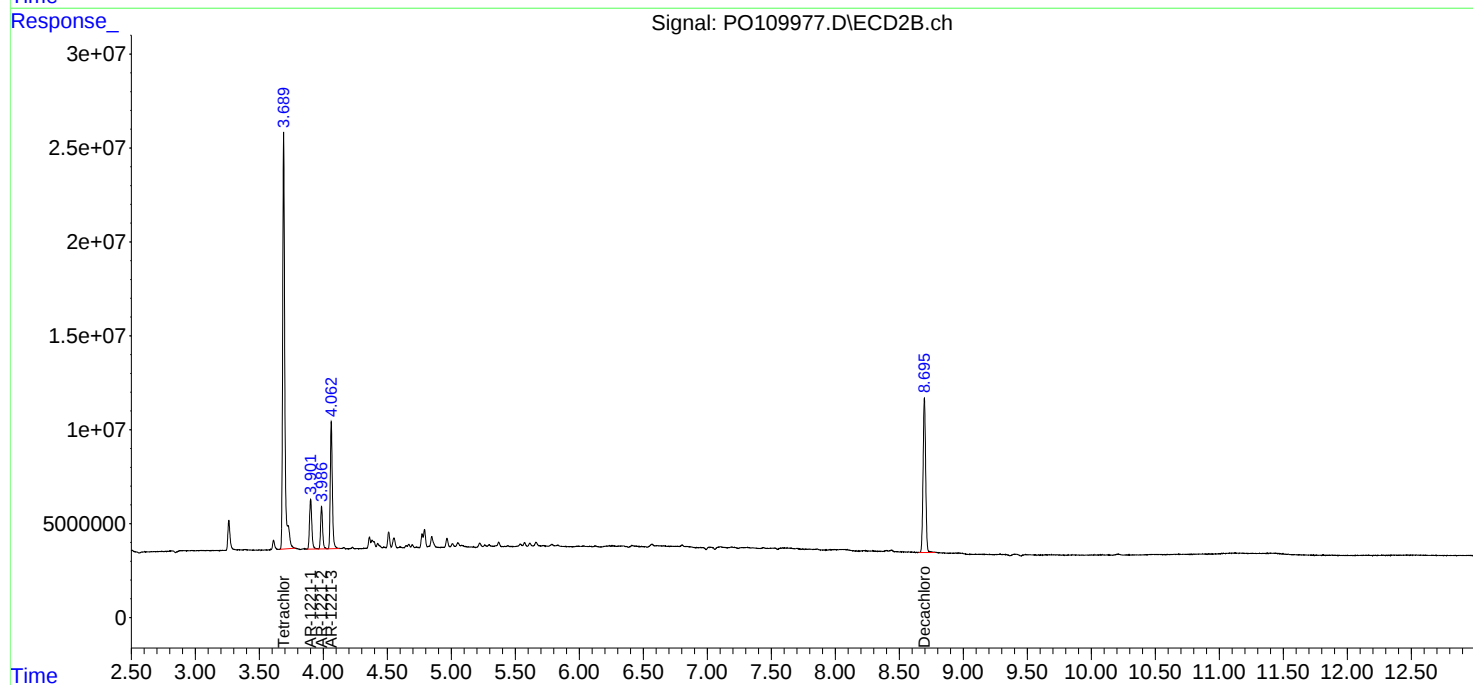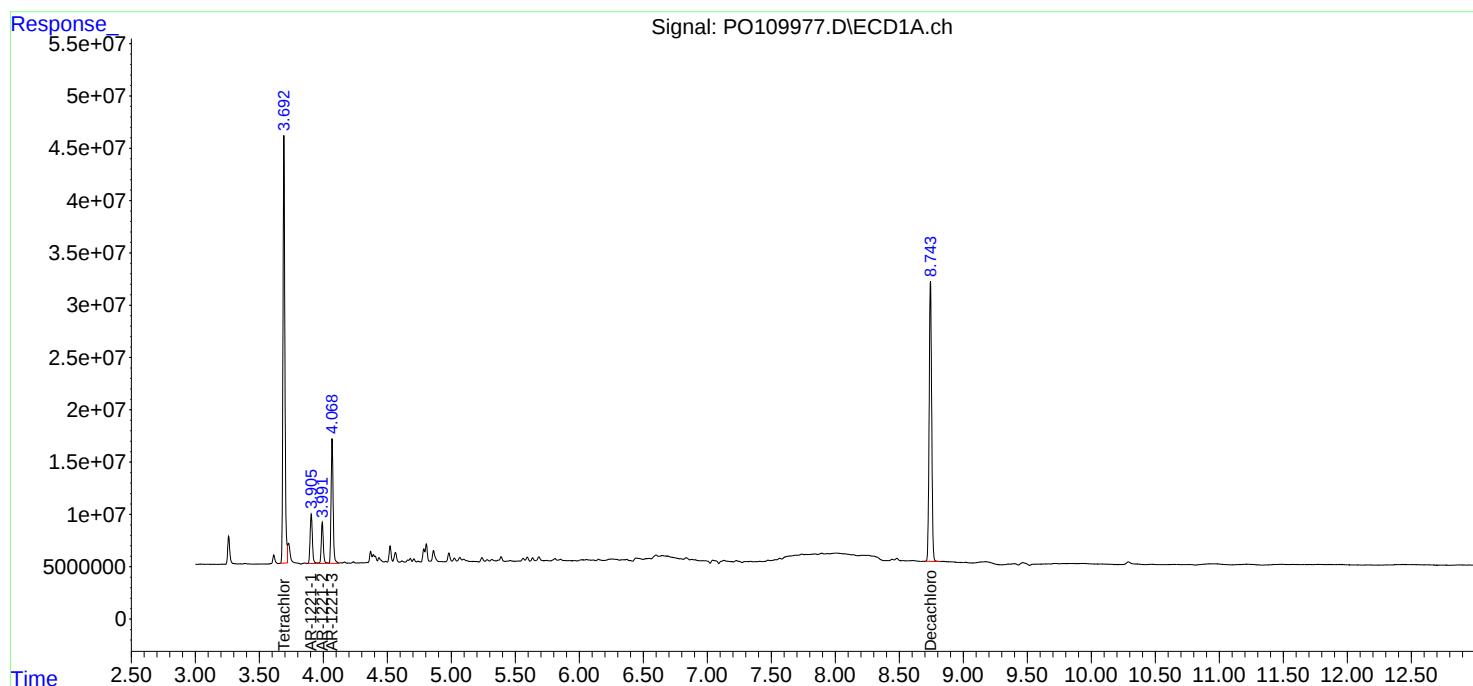

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 15:53
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:25:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:24:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	438.9E6	262.6E6	50.000	50.000
2) SA Decachlor...	8.744	8.696	372.1E6	116.2E6	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.068	4.062	107.9E6	62046675	500.000	500.000
12) L3 AR-1232-2	4.563	4.791	57393041	60174277	500.000	500.000
13) L3 AR-1232-3	4.805	4.966	105.9E6	31828000	500.000	500.000
14) L3 AR-1232-4	4.981	5.051	56780516	29670451	500.000	500.000
15) L3 AR-1232-5	5.024	5.221	40226994	31608944	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 15:53
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:25:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:24:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

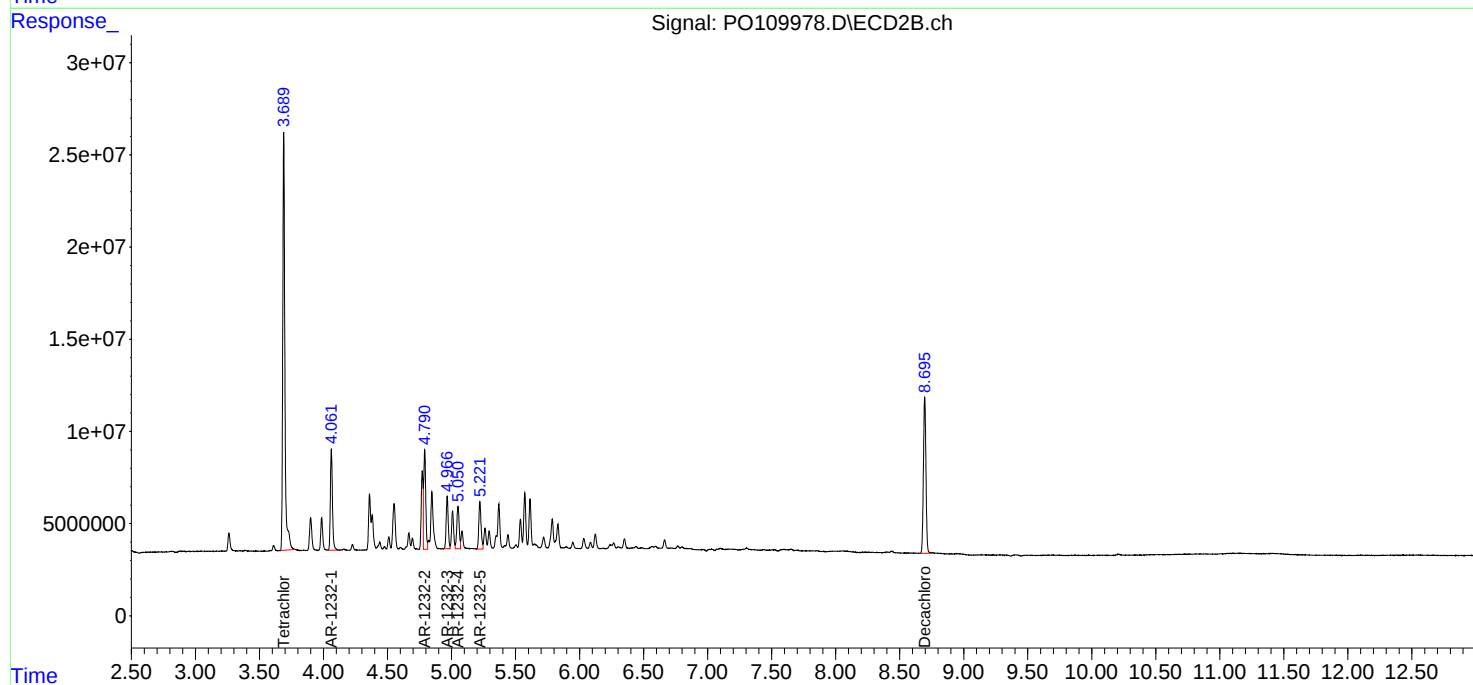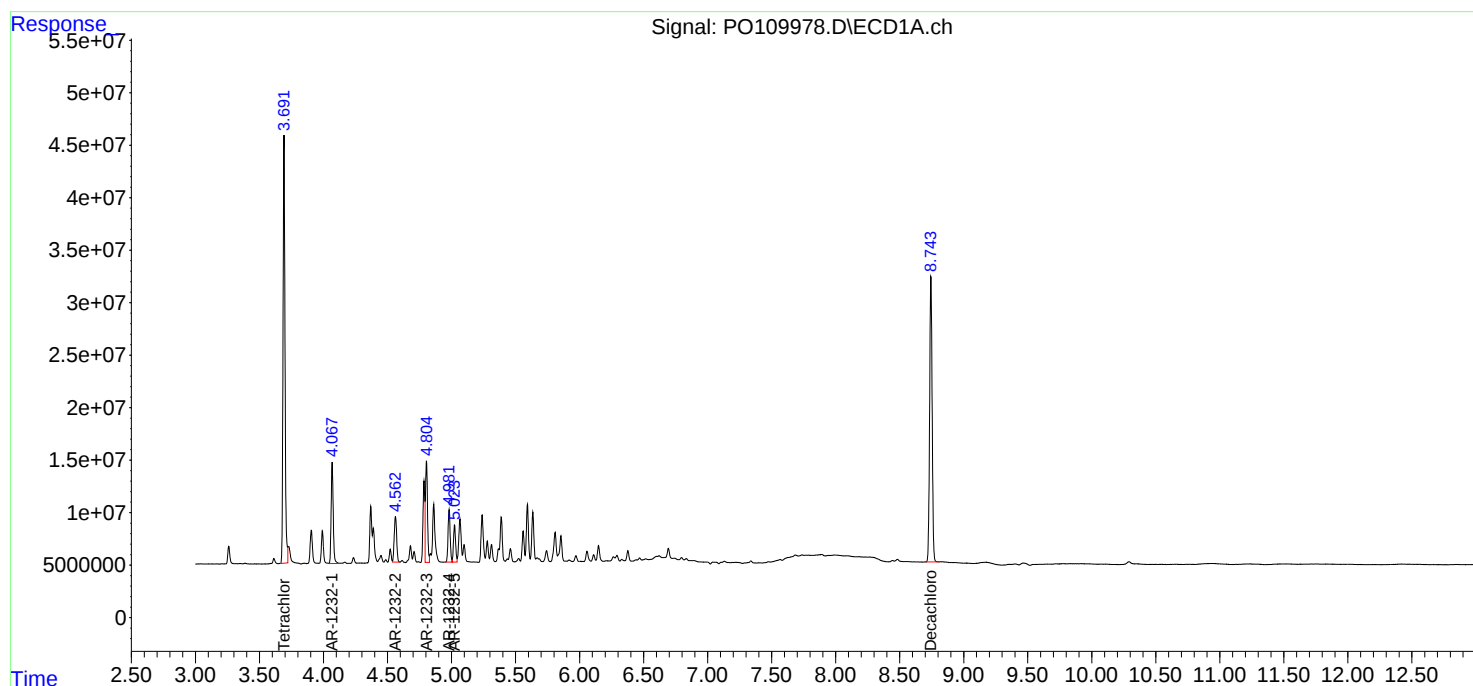

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 16:11
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 17:01:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:58:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	870.3E6	504.9E6	98.572	98.878
2) SA Decachlor...	8.744	8.697	707.3E6	217.8E6	97.860	97.910
Target Compounds						
16) L4 AR-1242-1	4.785	4.772	257.0E6	141.3E6	967.387	967.723
17) L4 AR-1242-2	4.804	4.791	361.7E6	206.0E6	974.253	976.732
18) L4 AR-1242-3	4.861	4.966	239.3E6	108.8E6	957.525	967.388
19) L4 AR-1242-4	4.981	5.051	191.3E6	107.6E6	962.368	956.424
20) L4 AR-1242-5	5.635	5.572	200.3E6	132.5E6	953.851	956.059



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 16:11
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 17:01:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:58:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

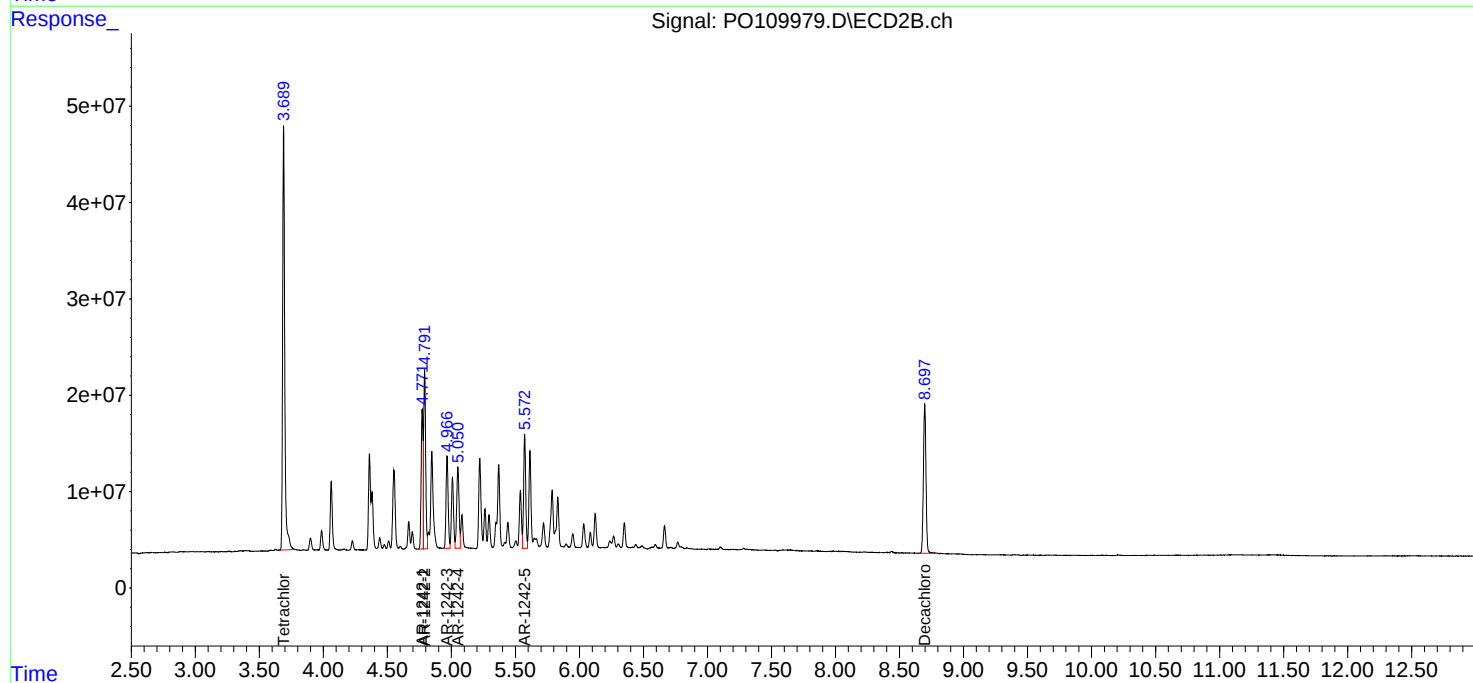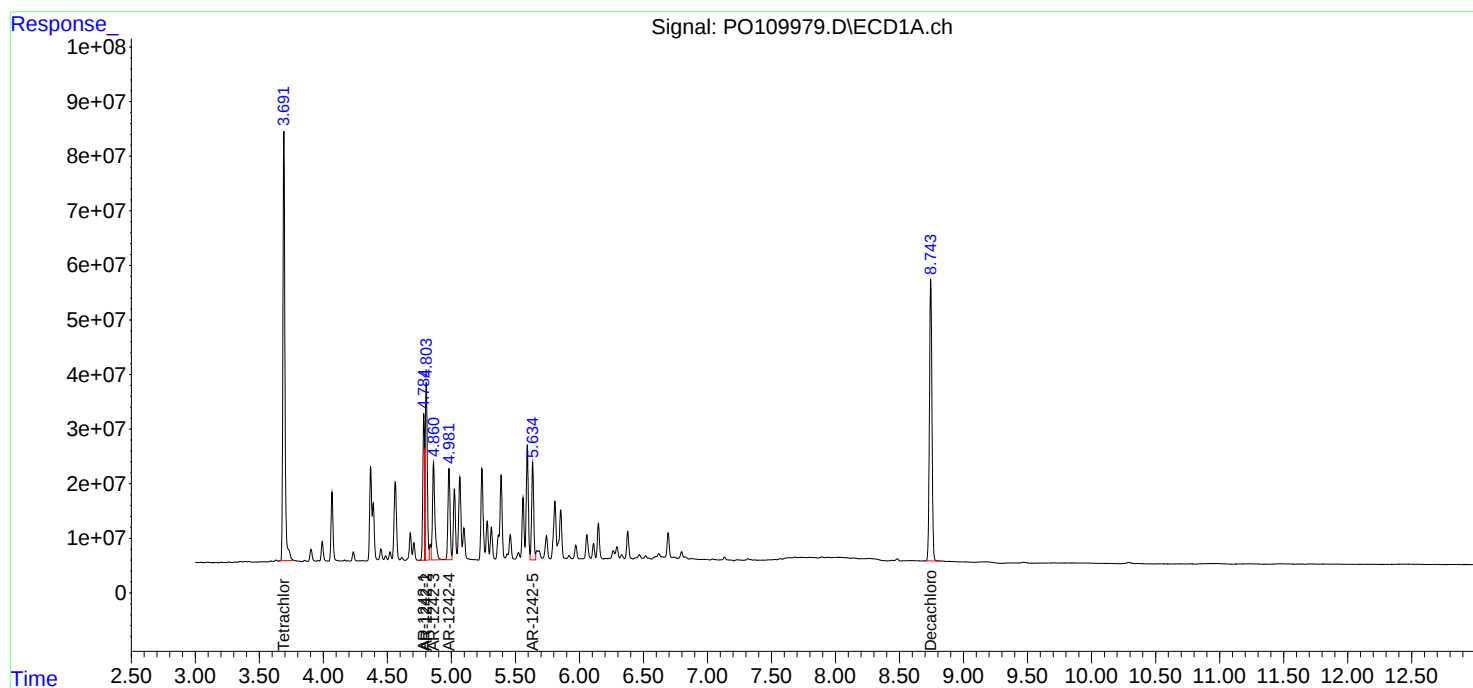

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 16:30
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 17:04:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:58:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.689	674.7E6	388.3E6	75.937	75.688
2) SA Decachlor...	8.744	8.696	546.6E6	166.9E6	75.416	75.037
Target Compounds						
16) L4 AR-1242-1	4.785	4.771	203.4E6	110.1E6	760.384	752.515
17) L4 AR-1242-2	4.804	4.790	282.0E6	160.8E6	756.501	758.433
18) L4 AR-1242-3	4.860	4.966	192.4E6	85755968	763.306	758.150
19) L4 AR-1242-4	4.981	5.050	152.0E6	85465010	759.882	756.281
20) L4 AR-1242-5	5.634	5.572	159.2E6	104.3E6	755.214	751.684



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
Data File : P0109980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 16:30
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 17:04:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:58:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

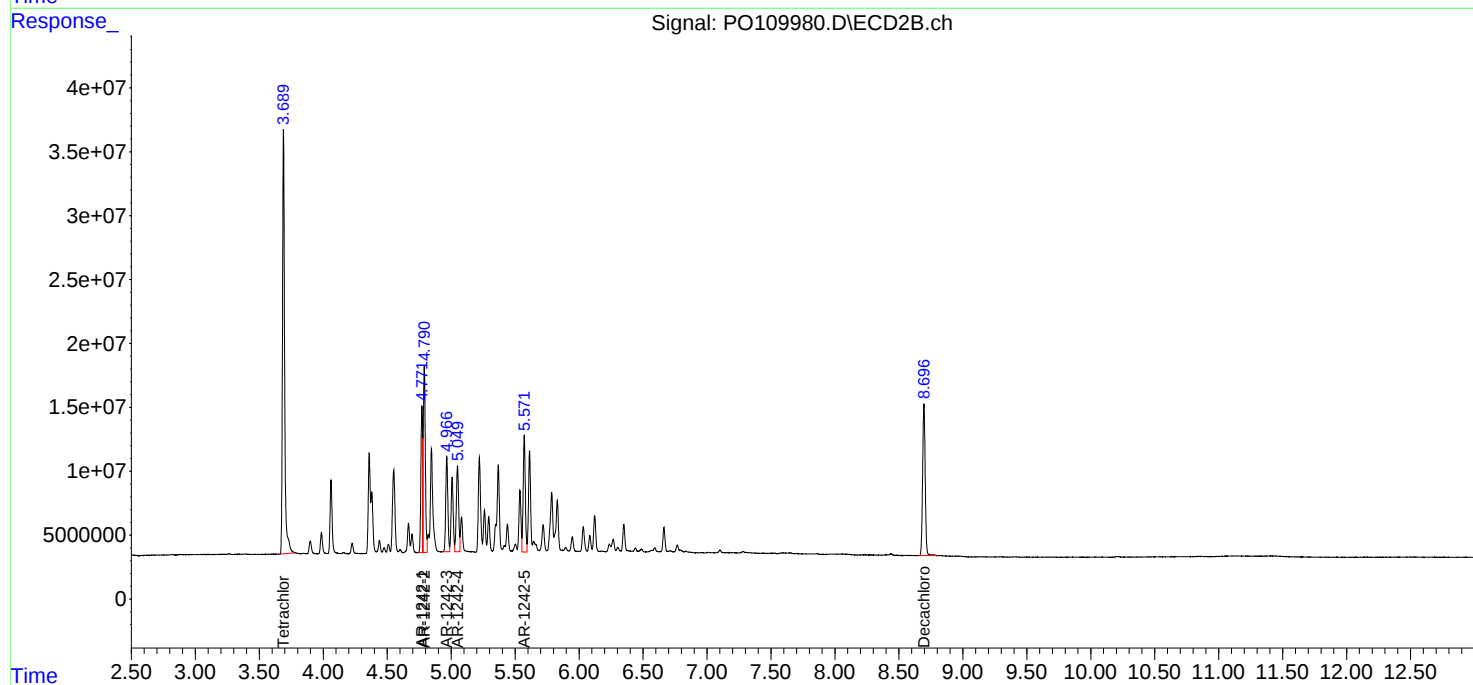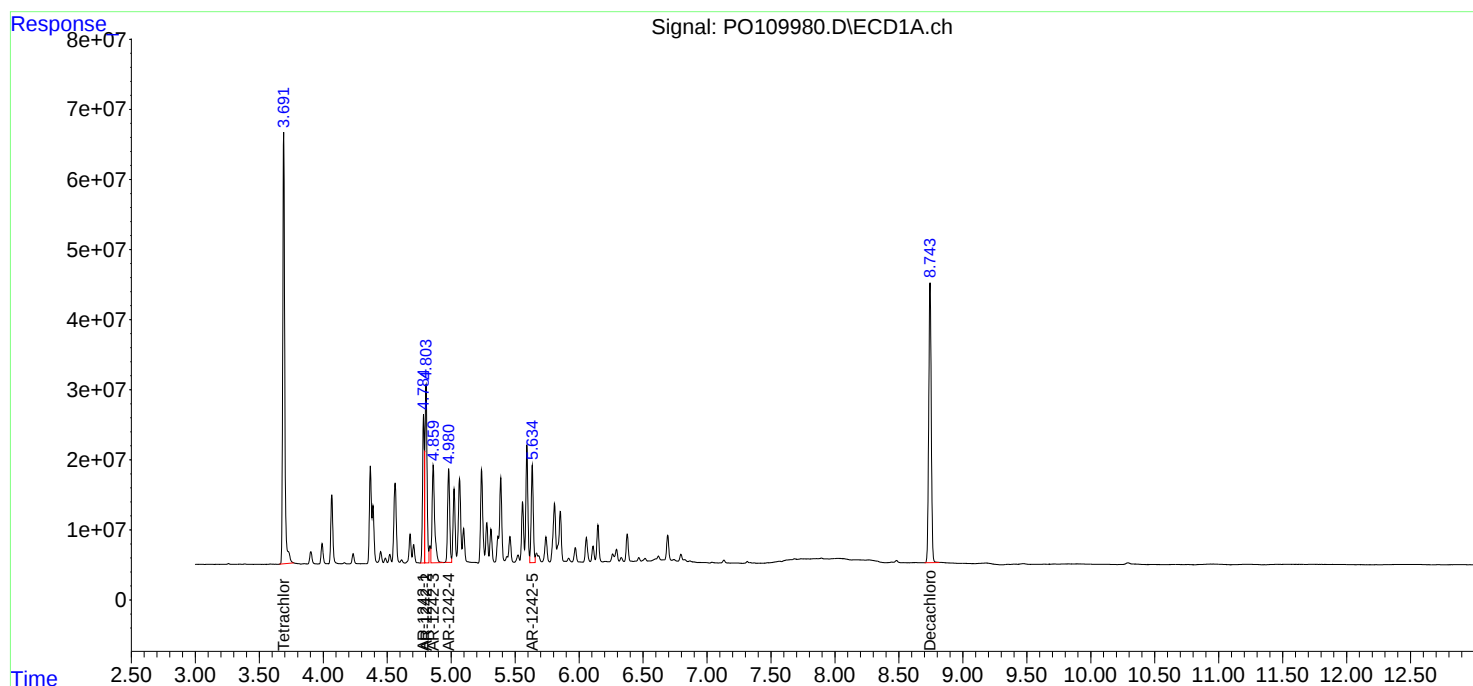

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 16:48
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:59:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 16:58:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.690	447.7E6	258.2E6	50.000	50.000
2) SA Decachlor...	8.744	8.695	369.1E6	113.5E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	4.785	4.772	137.2E6	75379512	500.000	500.000
17) L4 AR-1242-2	4.805	4.791	190.4E6	107.9E6	500.000	500.000
18) L4 AR-1242-3	4.861	4.967	130.3E6	58083170	500.000	500.000
19) L4 AR-1242-4	4.982	5.051	103.1E6	58718718	500.000	500.000
20) L4 AR-1242-5	5.635	5.573	109.9E6	72332482	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 16:48
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:59:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 16:58:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

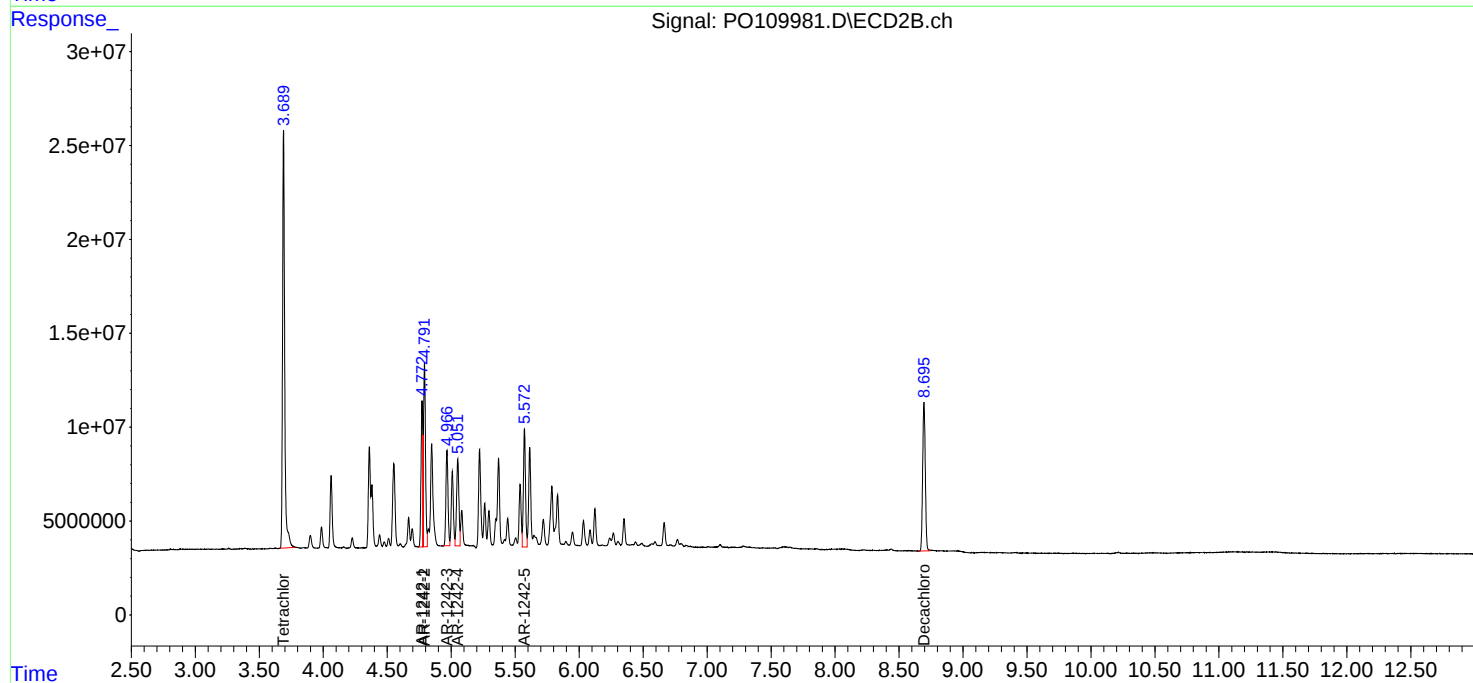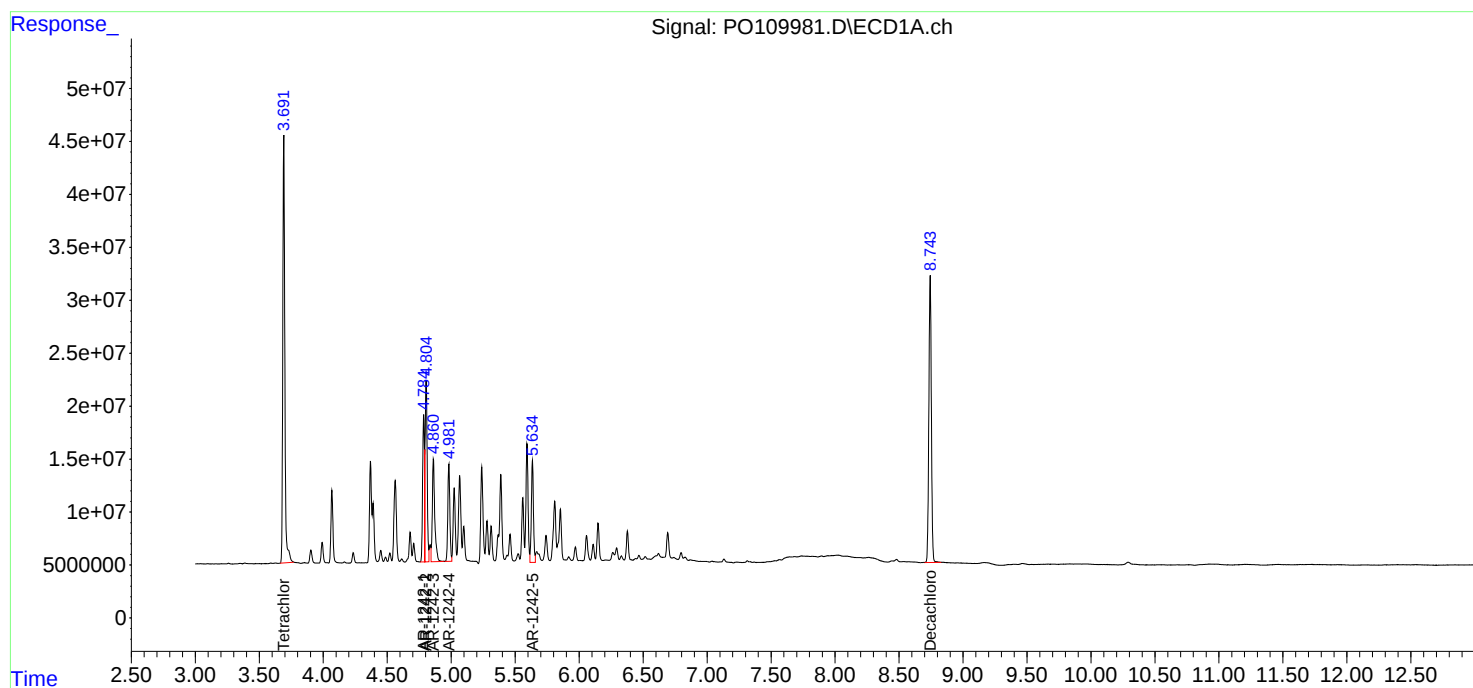

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 17:06
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 17:16:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 17:16:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	226.3E6	130.2E6	25.356	25.281
2) SA Decachlor...	8.744	8.695	194.6E6	60893229	26.361	26.736
Target Compounds						
16) L4 AR-1242-1	4.785	4.772	71937746	39990799	263.903	267.124
17) L4 AR-1242-2	4.804	4.791	99324236	56210353	262.106	261.143
18) L4 AR-1242-3	4.860	4.967	69326183	30721999	268.271	265.862
19) L4 AR-1242-4	4.981	5.051	53927655	31584987	264.381	271.488
20) L4 AR-1242-5	5.634	5.572	57576429	38102015	266.987	268.040



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 17:06
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 17:16:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 17:16:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

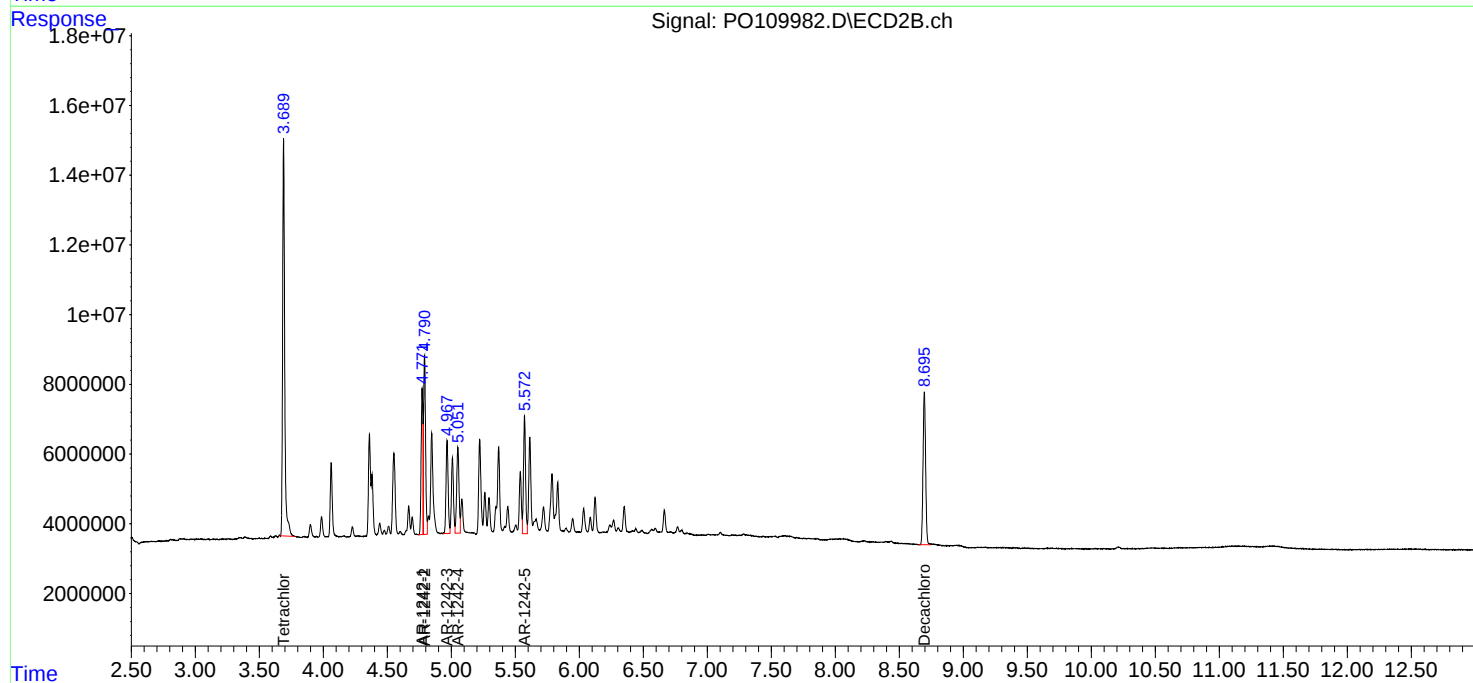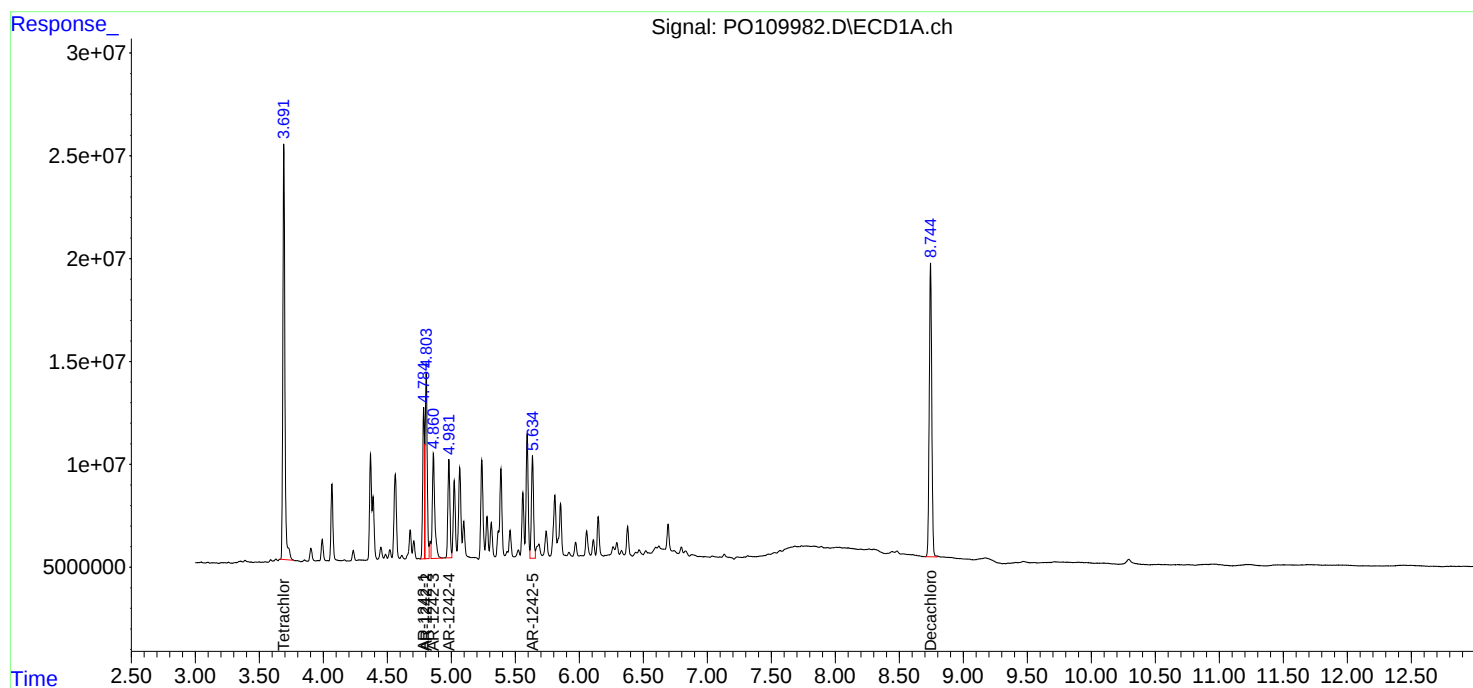

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 17:25
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 17:34:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 18 17:34:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.688	33275417	17649519	3.978m	3.680m
2) SA Decachlor...	8.744	8.696	32408304	10337597	4.500	4.624
Target Compounds						
16) L4 AR-1242-1	4.784	4.772	12333502	6612130	46.123	45.222
17) L4 AR-1242-2	4.804	4.791	16261465	8959332	44.164	43.066
18) L4 AR-1242-3	4.859	4.966	12804073	4792003	49.638	42.926m
19) L4 AR-1242-4	4.980	5.051	9228050	5726073	46.259m	49.373
20) L4 AR-1242-5	5.633	5.572	9633519	5880388	45.772m	42.708m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 17:25
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 17:34:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 18 17:34:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

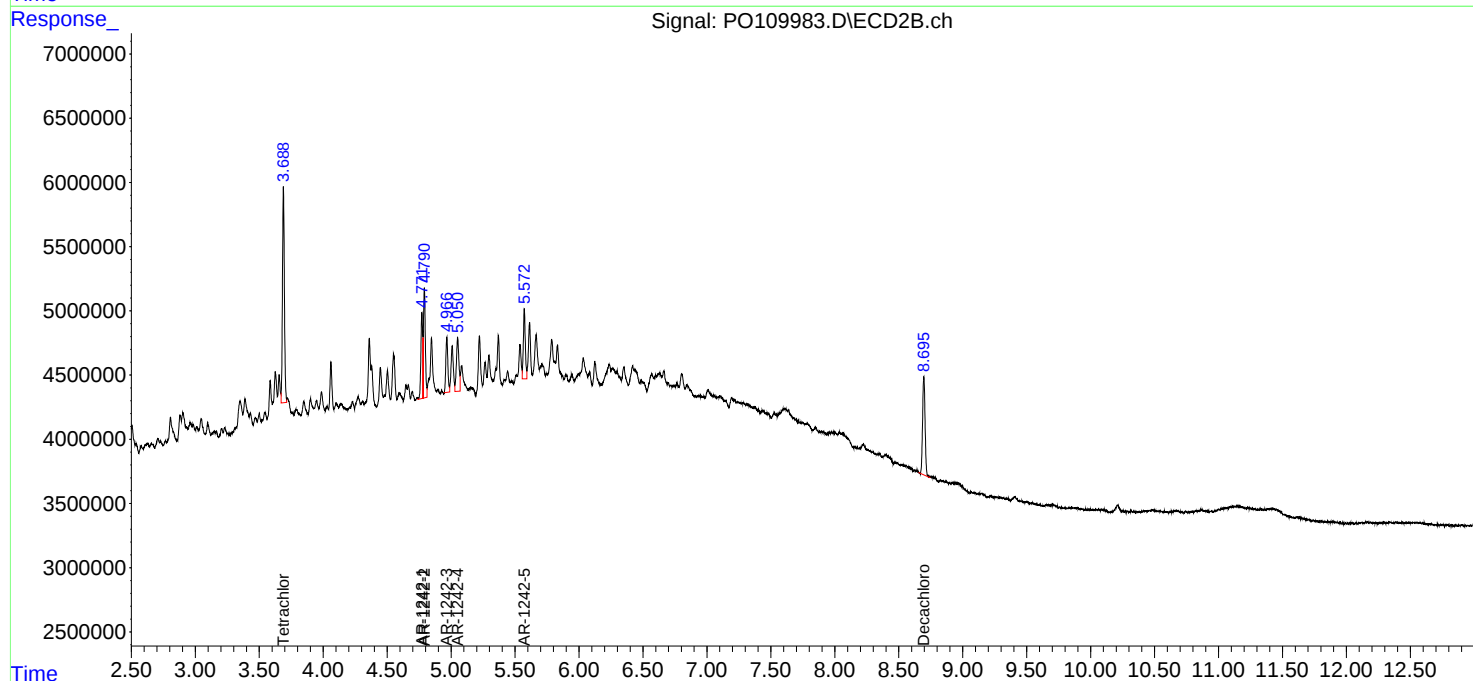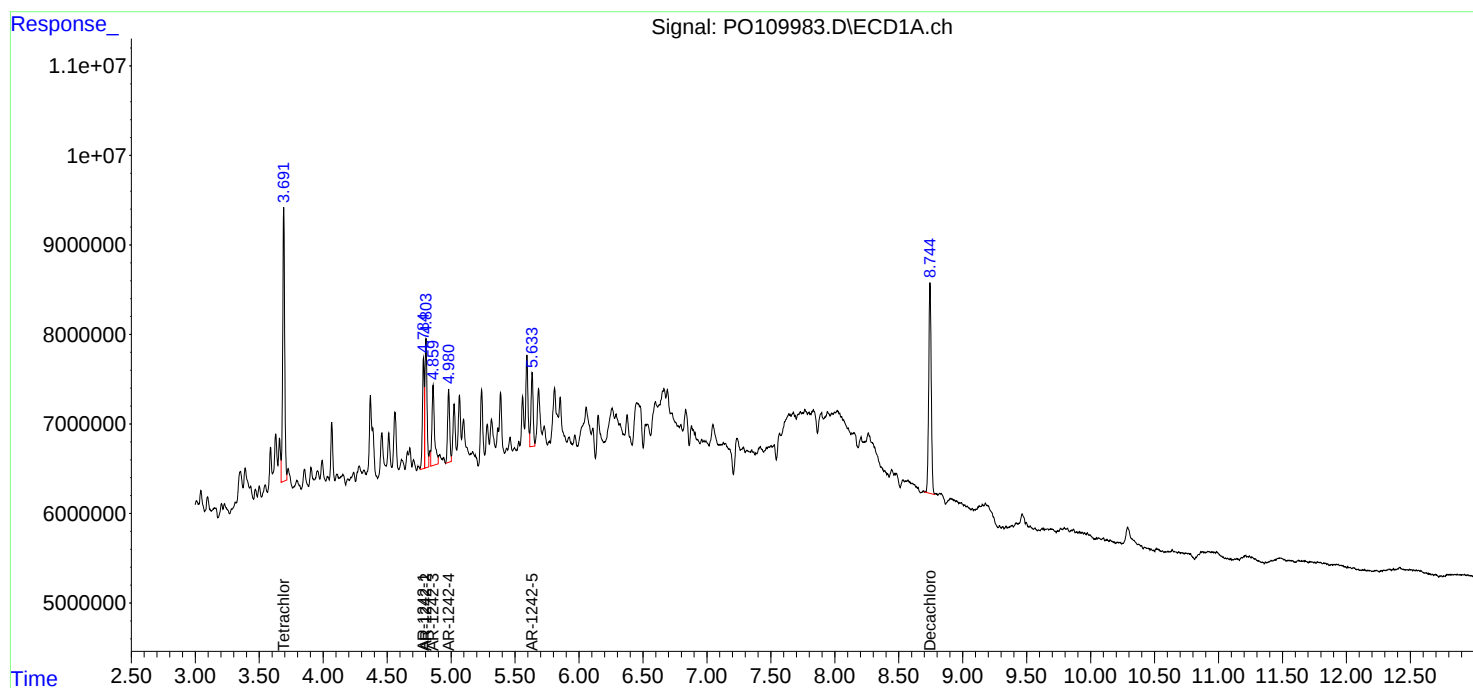

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 17:42
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:40:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:38:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	3.689	889.7E6	511.9E6	95.913	96.672
2) SA Decachlor...	8.742	8.696	728.0E6	214.7E6	93.393	91.574
Target Compounds						
21) L5 AR-1248-1	4.783	4.771	203.2E6	111.3E6	923.985	924.703
22) L5 AR-1248-2	5.022	5.008	271.7E6	153.2E6	902.515	908.902
23) L5 AR-1248-3	5.237	5.050	341.9E6	163.6E6	913.052	913.648
24) L5 AR-1248-4	5.591	5.221	484.7E6	192.0E6	926.318	920.729
25) L5 AR-1248-5	5.633	5.614	341.9E6	189.8E6	924.672	932.015



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 17:42
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:40:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:38:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

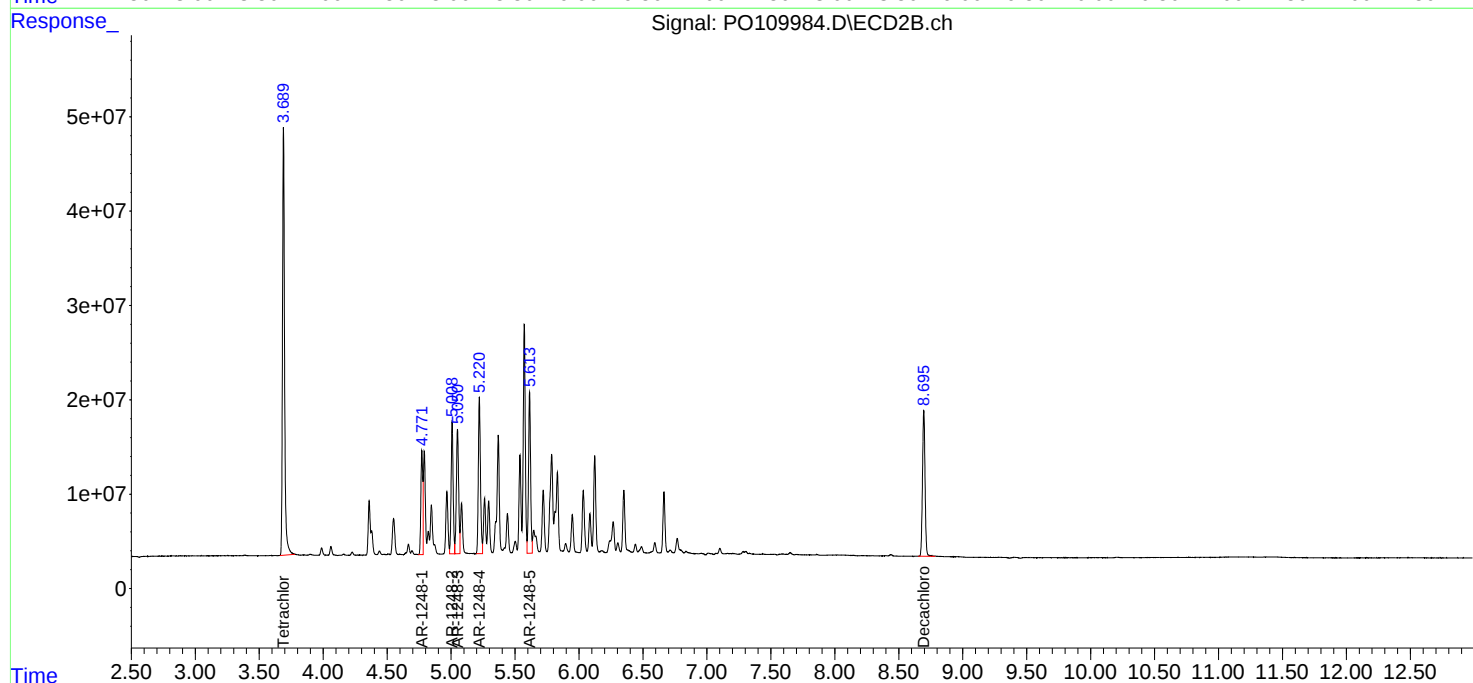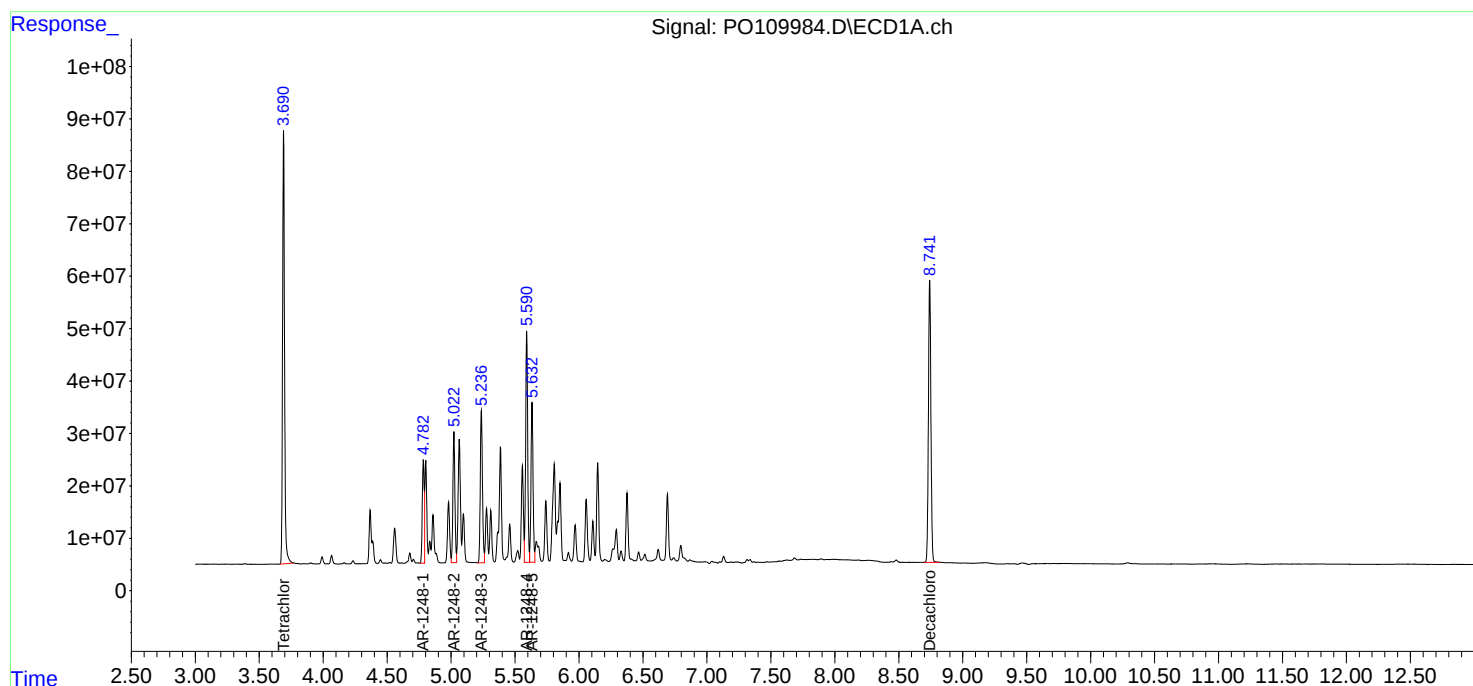

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 18:00
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:40:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:38:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.693	3.690	683.1E6	391.4E6	73.638	73.916
2) SA Decachlor...	8.743	8.696	564.9E6	168.9E6	72.473	72.022
Target Compounds						
21) L5 AR-1248-1	4.785	4.772	158.1E6	86749863	718.942	720.978
22) L5 AR-1248-2	5.024	5.009	213.9E6	120.1E6	710.557	712.732
23) L5 AR-1248-3	5.239	5.051	267.9E6	128.2E6	715.615	715.920
24) L5 AR-1248-4	5.593	5.222	377.8E6	150.5E6	721.979	721.526
25) L5 AR-1248-5	5.635	5.614	266.1E6	147.5E6	719.788	724.105



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 18:00
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:40:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:38:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

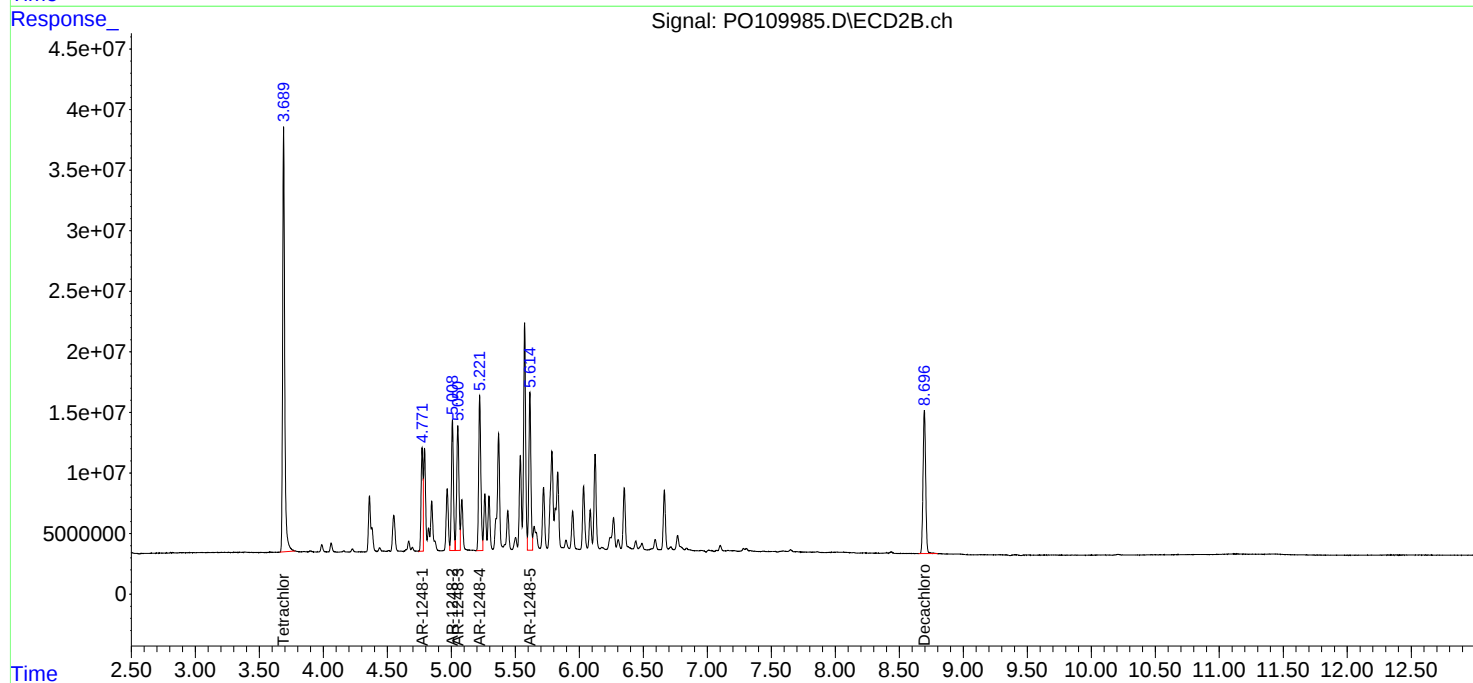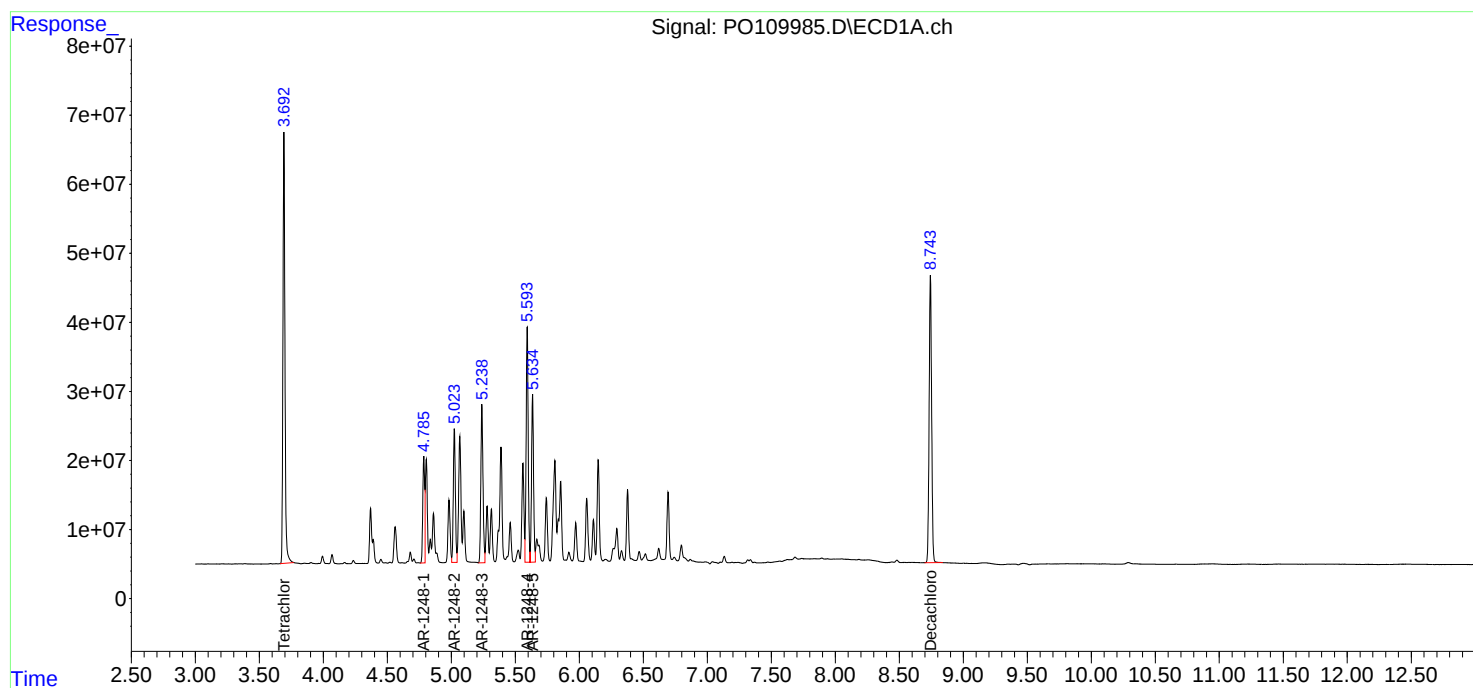

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 18:19
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:40:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:38:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.692	3.690	463.8E6	264.8E6	50.000	50.000
2)	SA Decachlor...	8.744	8.695	389.7E6	117.2E6	50.000	50.000
Target Compounds							
21)	L5 AR-1248-1	4.785	4.771	110.0E6	60161217	500.000	500.000
22)	L5 AR-1248-2	5.023	5.008	150.5E6	84259256	500.000	500.000
23)	L5 AR-1248-3	5.239	5.051	187.2E6	89552637	500.000	500.000
24)	L5 AR-1248-4	5.593	5.221	261.6E6	104.3E6	500.000	500.000
25)	L5 AR-1248-5	5.634	5.613	184.9E6	101.8E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 18:19
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:40:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:38:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

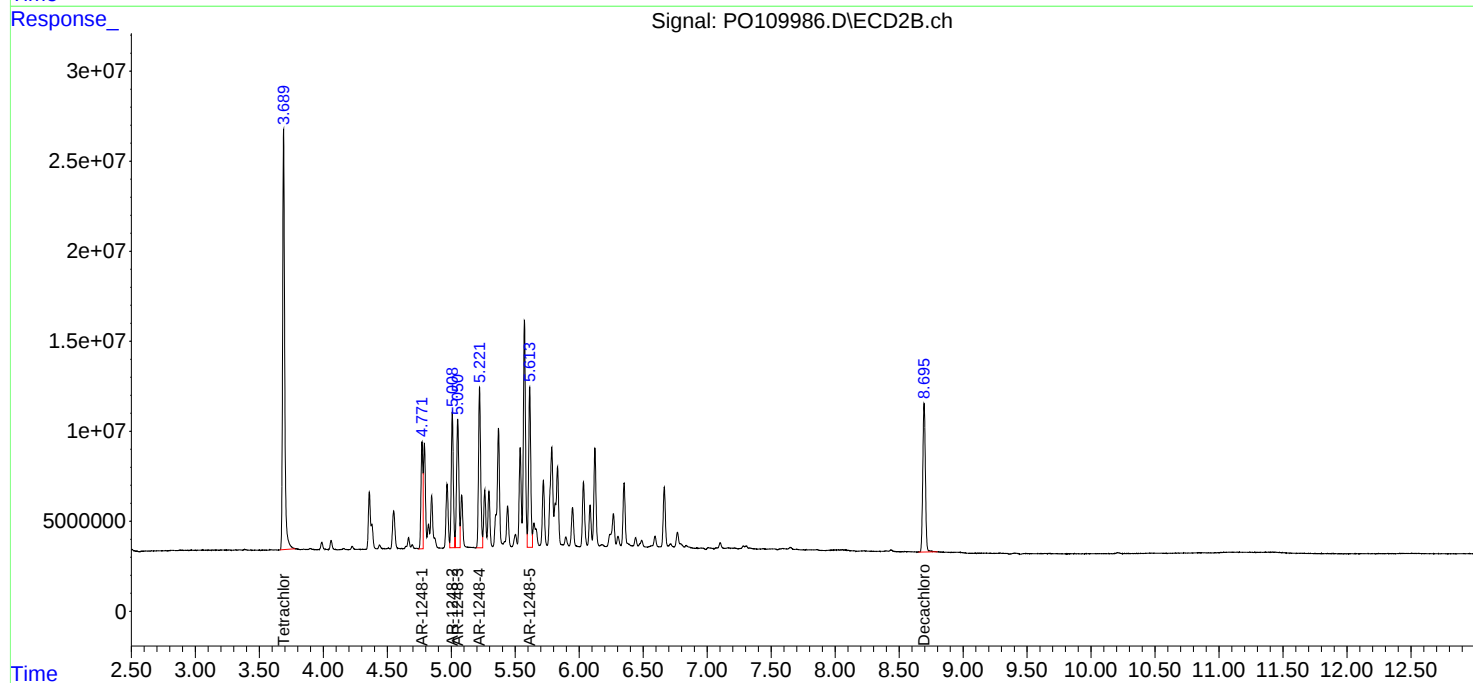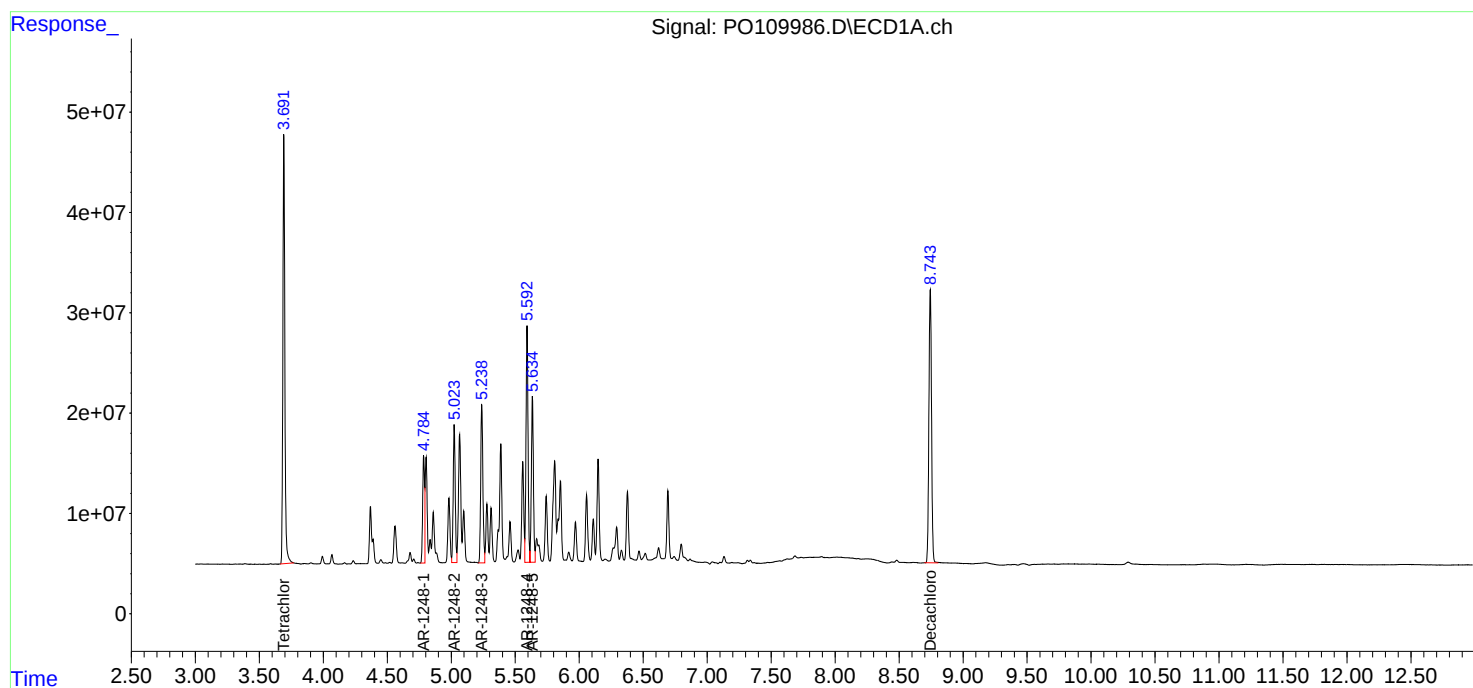

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 18:37
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:40:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:38:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.691	3.689	234.4E6	134.2E6	25.266	25.339
2)	SA Decachlor...	8.744	8.695	202.8E6	63399780	26.017	27.040
Target Compounds							
21)	L5 AR-1248-1	4.784	4.771	57869632	31675925	263.114	263.259
22)	L5 AR-1248-2	5.023	5.008	80049855	44958781	265.887	266.788
23)	L5 AR-1248-3	5.238	5.050	98806066	47928872	263.899	267.602
24)	L5 AR-1248-4	5.592	5.221	136.0E6	55764342	259.818	267.368
25)	L5 AR-1248-5	5.634	5.613	96853624	53959011	261.961	264.931



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 18:37
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:40:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:38:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

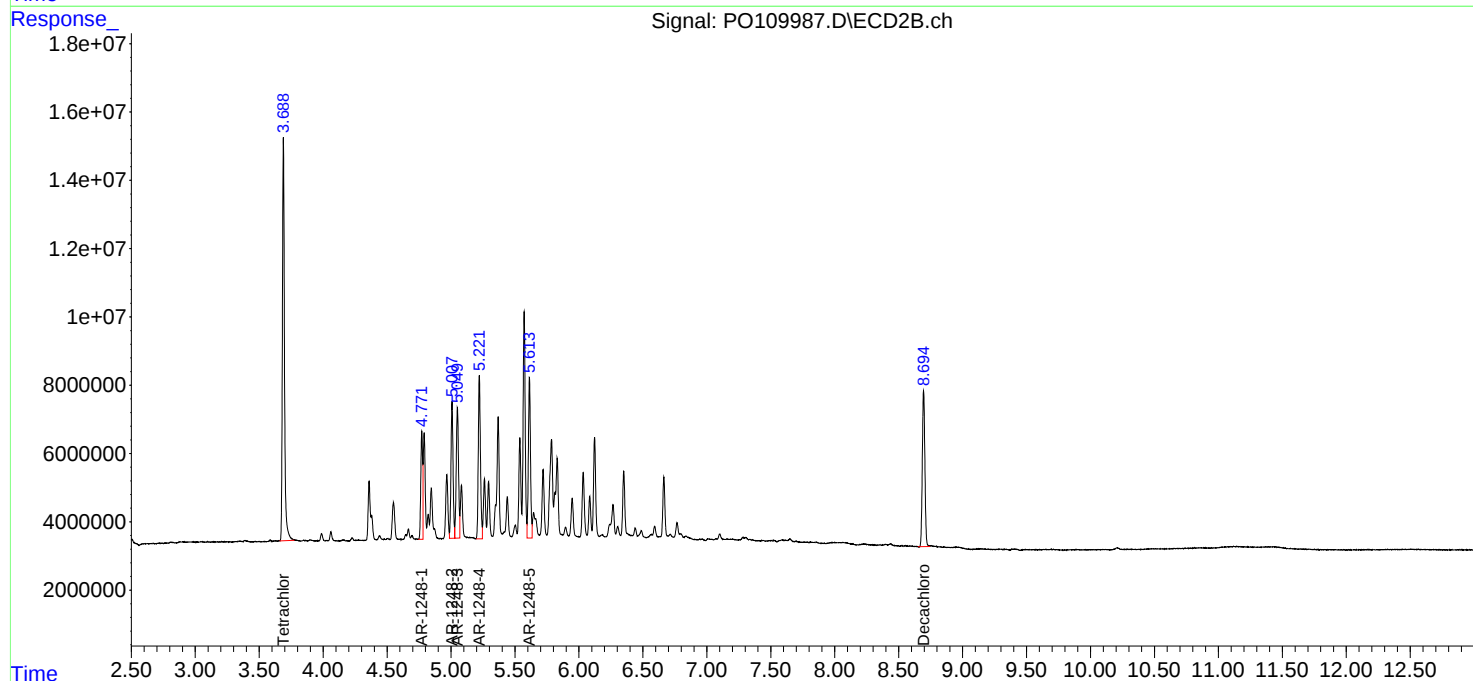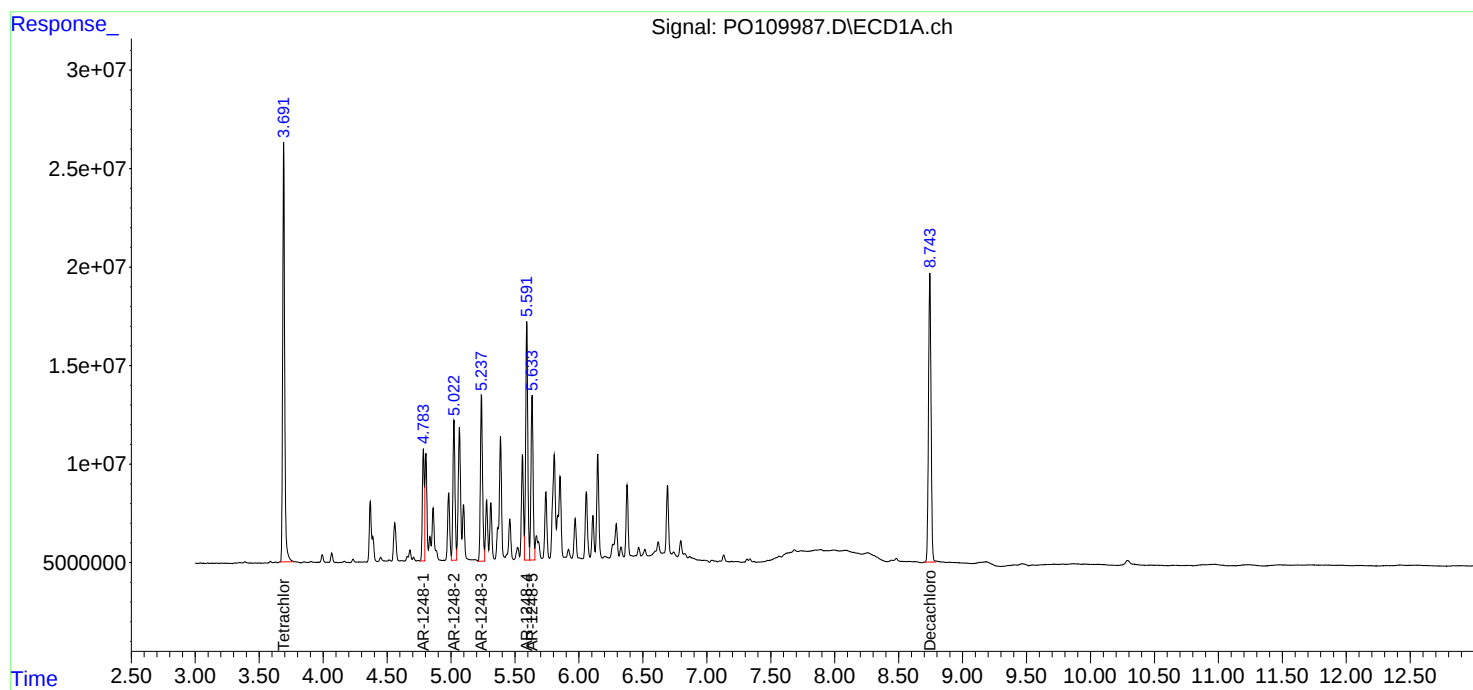

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031925\
 Data File : P0109988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 18:54
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:40:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:38:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	3.689	43788277	25352976	4.721	4.788
2) SA Decachlor...	8.742	8.695	41310164	13029410	5.300	5.557
Target Compounds						
21) L5 AR-1248-1	4.782	4.771	11846805	6686511	53.863	55.572
22) L5 AR-1248-2	5.021	5.008	16385888	9031427	54.426	53.593
23) L5 AR-1248-3	5.235	5.050	19860582	10026048	53.045m	55.979
24) L5 AR-1248-4	5.591	5.221	29227773	11398927	55.856	54.653m
25) L5 AR-1248-5	5.632	5.613	20545156	11669383	55.569	57.295

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 18:54
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:40:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:38:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

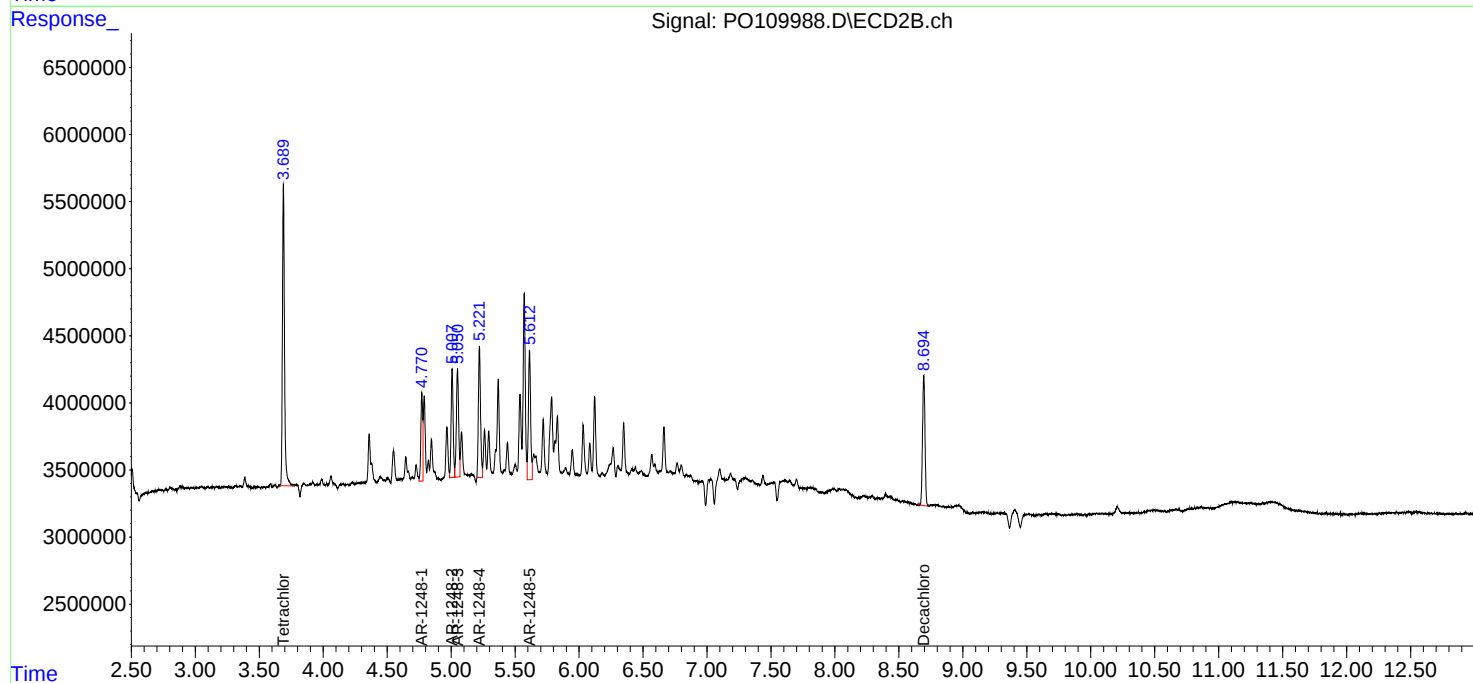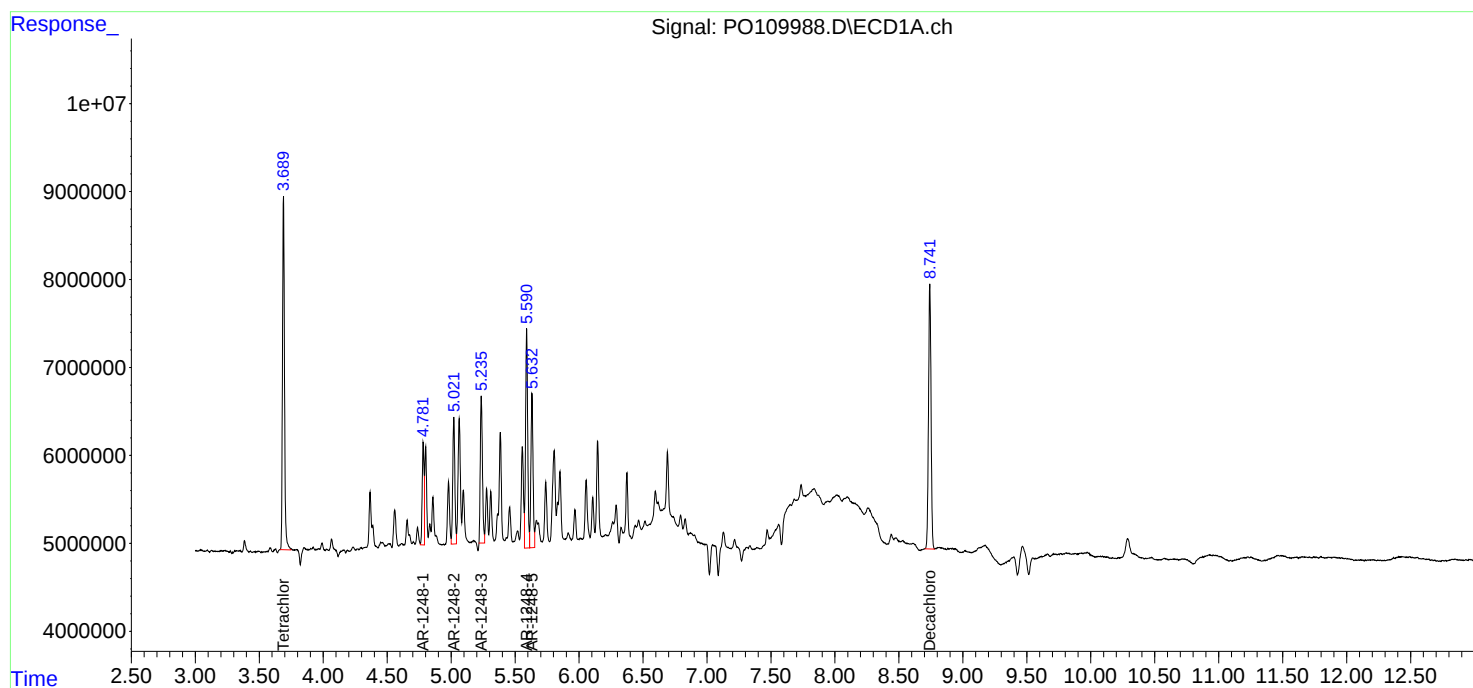

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 19:13
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:49:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:48:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.690	912.4E6	520.8E6	97.196	97.394
2) SA Decachlor...	8.744	8.694	750.7E6	219.7E6	95.415	90.831
Target Compounds						
26) L6 AR-1254-1	5.593	5.573	527.5E6	289.8E6	943.049	941.799
27) L6 AR-1254-2	5.742	5.721	454.9E6	250.7E6	940.470	933.876
28) L6 AR-1254-3	6.147	6.123	753.6E6	402.2E6	954.831	954.778
29) L6 AR-1254-4	6.376	6.351	465.4E6	231.8E6	956.772	948.684
30) L6 AR-1254-5	6.797	6.768	652.0E6	329.3E6	958.152	944.466



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 19:13
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:49:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:48:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

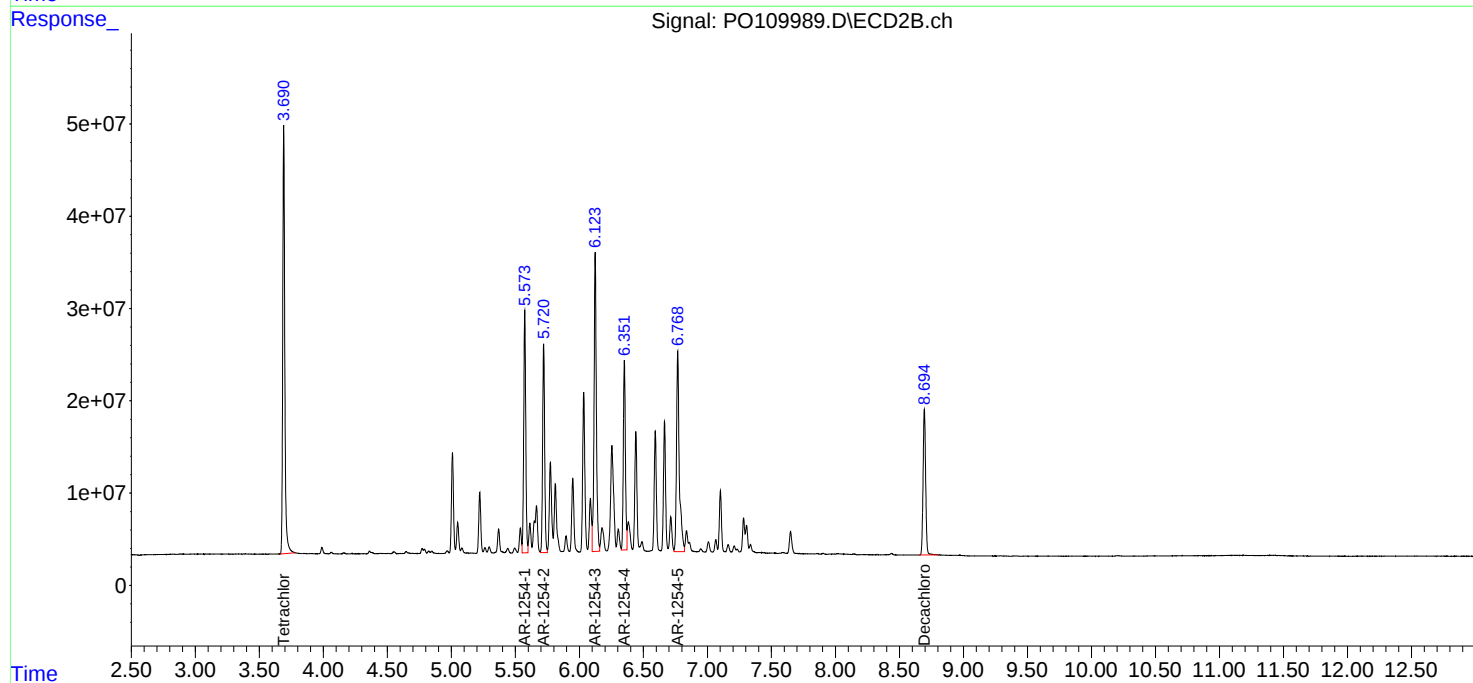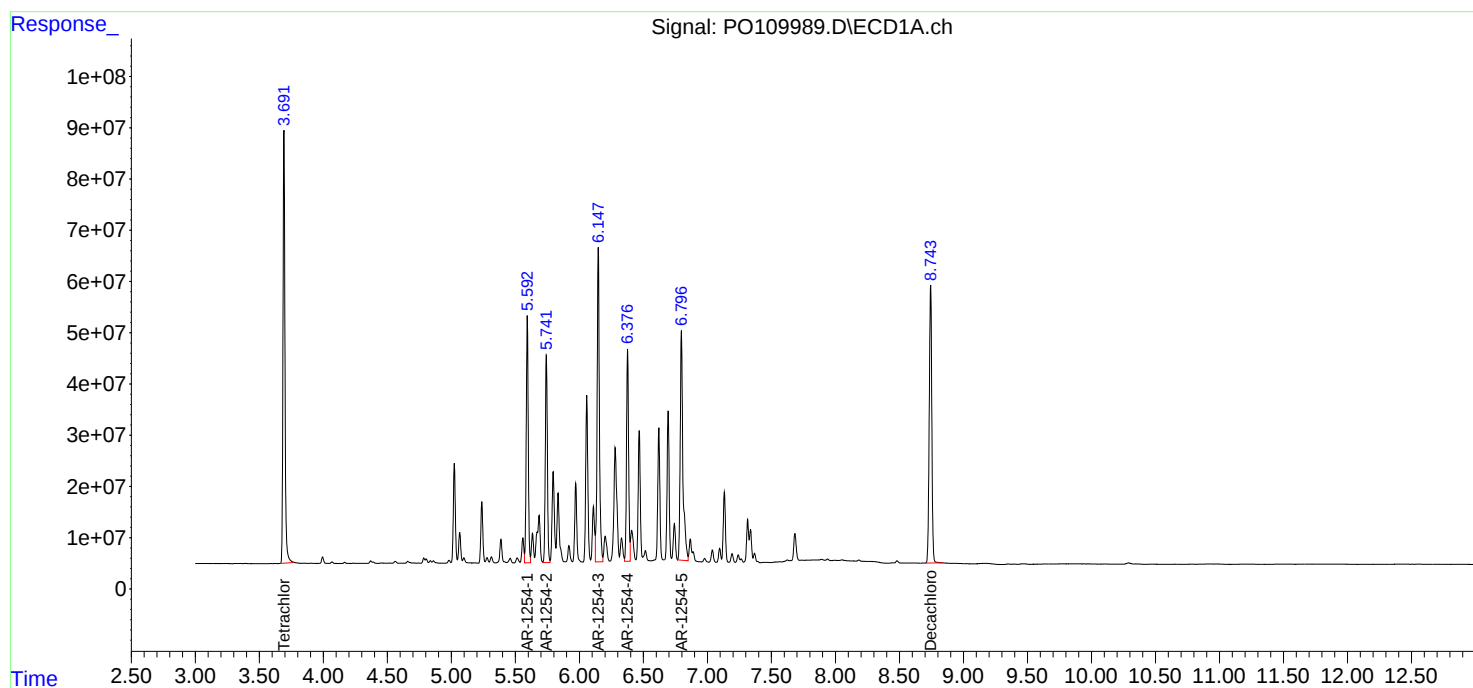

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 19:31
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:49:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:48:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.689	694.8E6	396.7E6	74.017	74.184
2) SA Decachlor...	8.742	8.695	579.2E6	170.7E6	73.621	70.591
Target Compounds						
26) L6 AR-1254-1	5.593	5.572	406.4E6	224.1E6	726.602	728.104
27) L6 AR-1254-2	5.742	5.720	351.8E6	194.7E6	727.216	725.242
28) L6 AR-1254-3	6.148	6.122	579.5E6	310.1E6	734.225	736.114
29) L6 AR-1254-4	6.376	6.350	358.3E6	178.4E6	736.667	729.972
30) L6 AR-1254-5	6.796	6.768	499.8E6	253.4E6	734.486	726.842



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 19:31
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:49:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:48:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

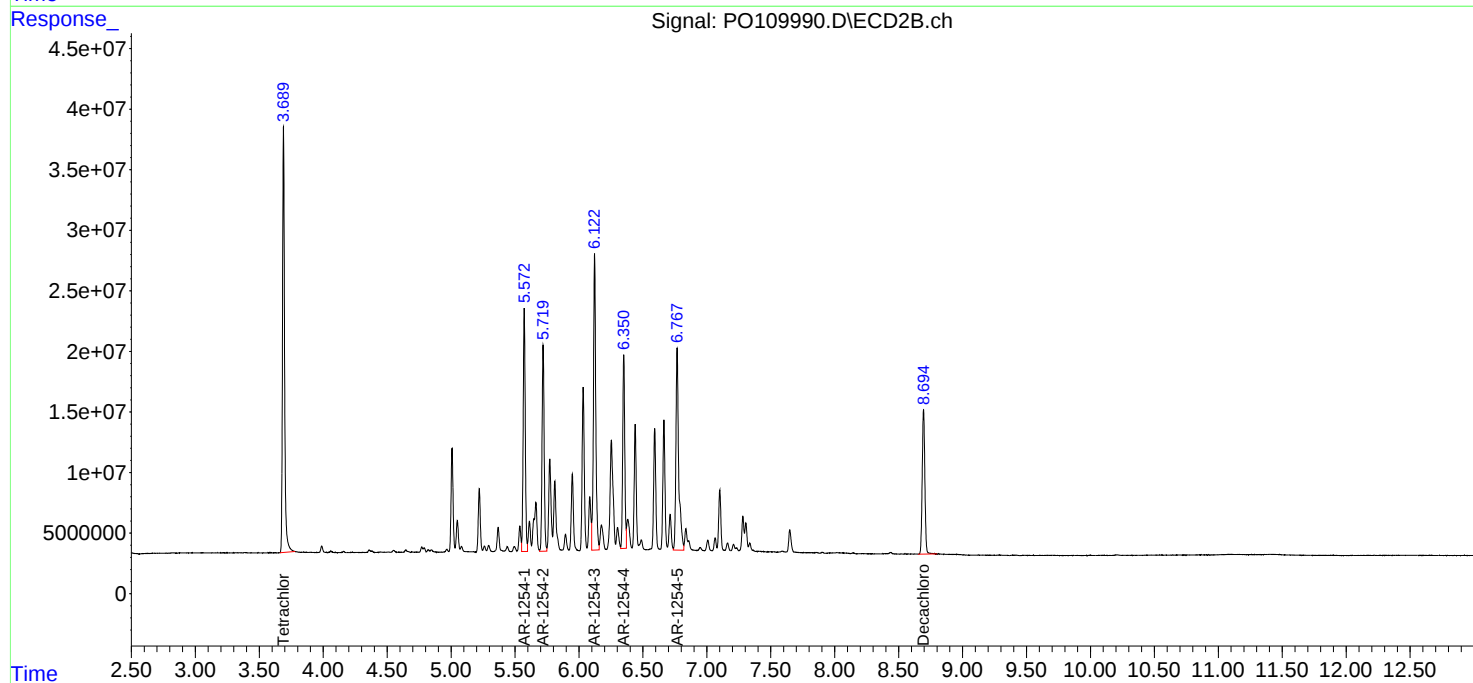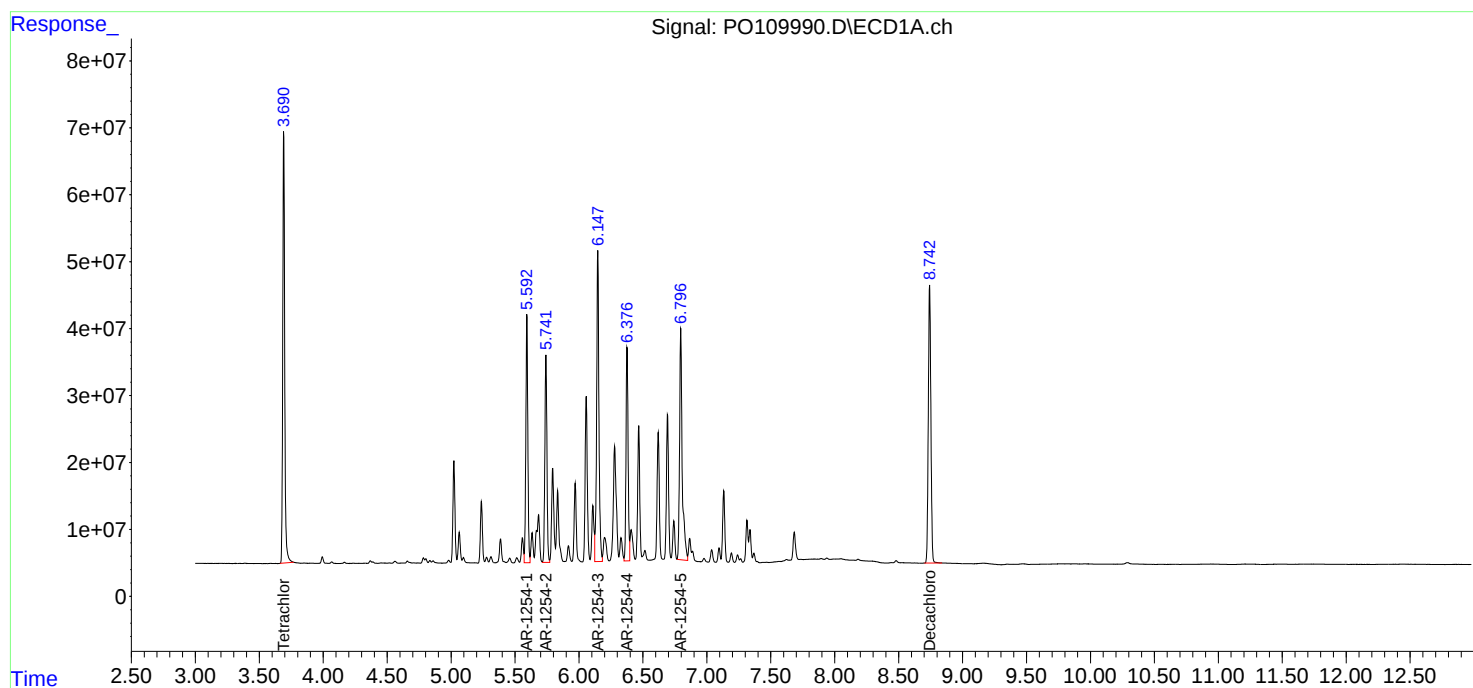

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 19:49
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:52:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:48:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	469.4E6	267.3E6	50.000	50.000
2) SA Decachlor...	8.744	8.695	393.4E6	120.9E6	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	5.594	5.573	279.7E6	153.9E6	500.000	500.000
27) L6 AR-1254-2	5.743	5.720	241.9E6	134.2E6	500.000	500.000
28) L6 AR-1254-3	6.148	6.123	394.6E6	210.6E6	500.000	500.000
29) L6 AR-1254-4	6.378	6.351	243.2E6	122.2E6	500.000	500.000
30) L6 AR-1254-5	6.797	6.768	340.3E6	174.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO031925\
Data File : PO109991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 19:49
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:52:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:48:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

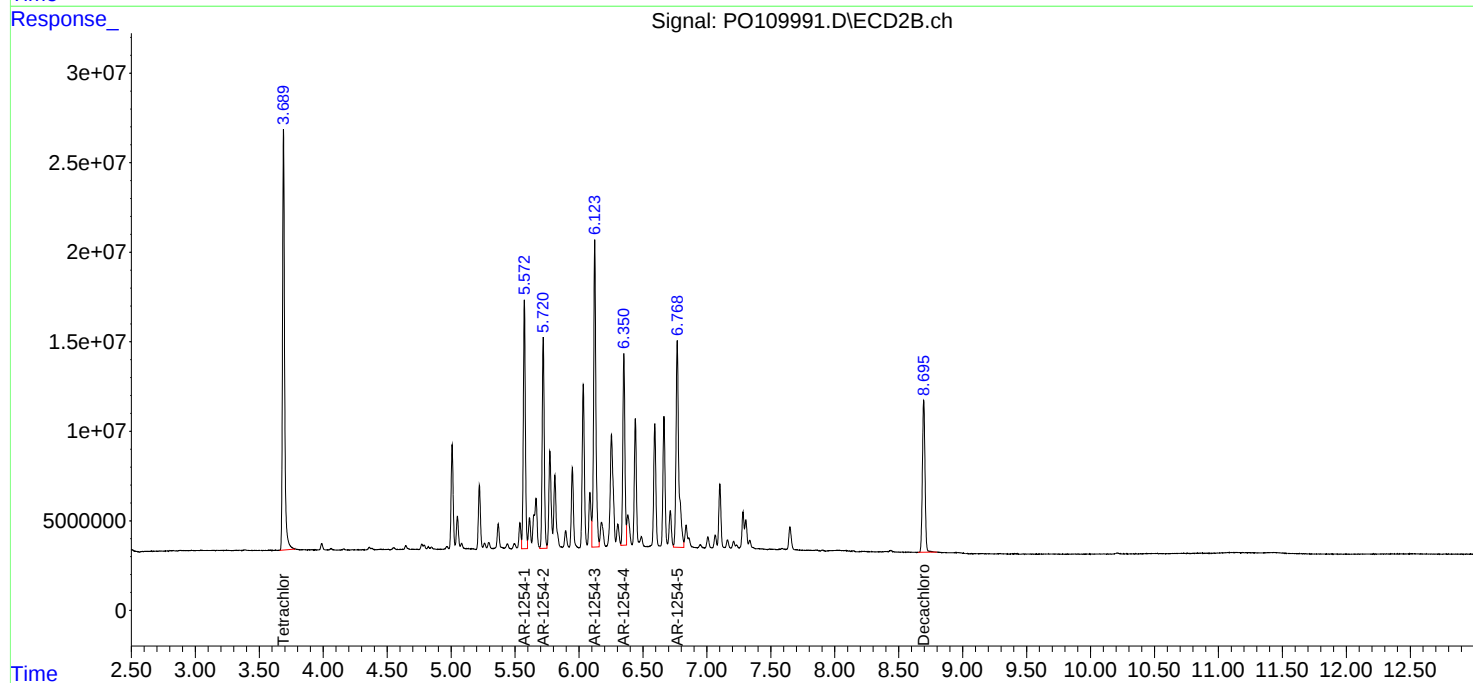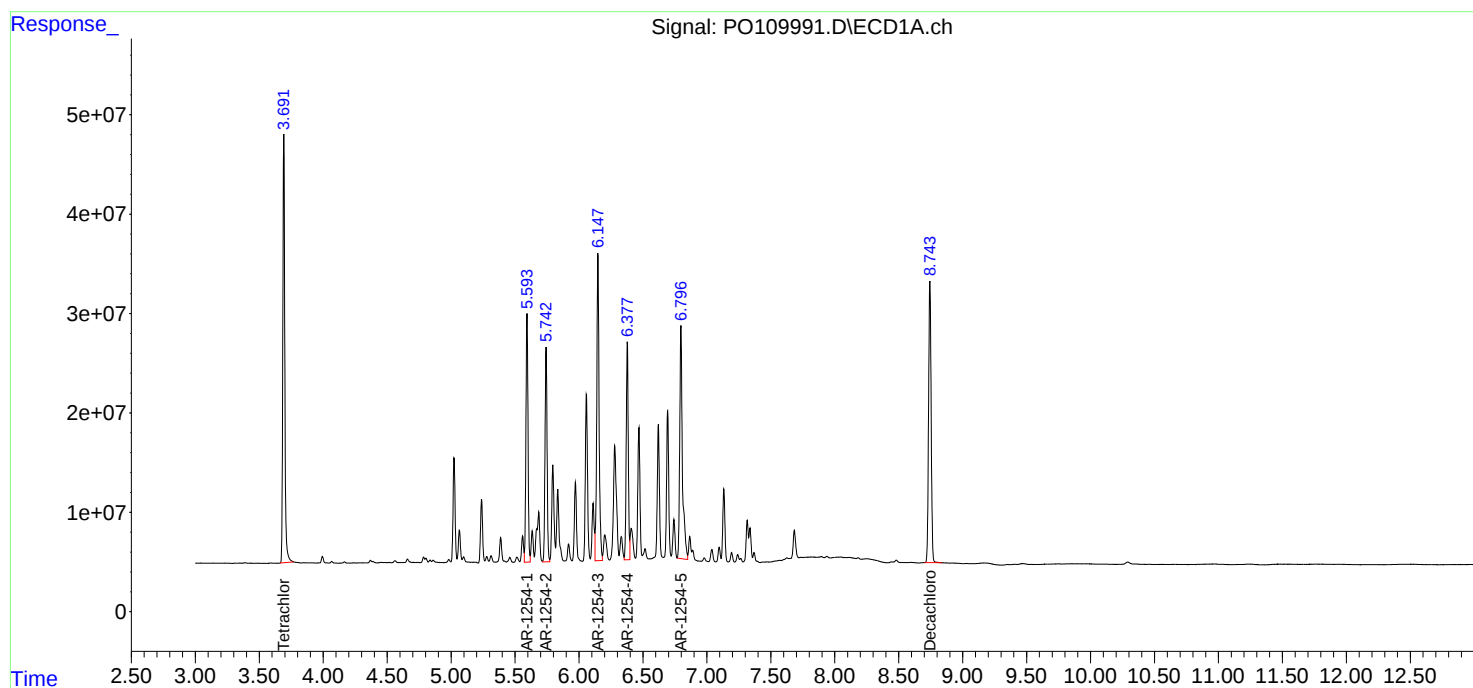

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 20:07
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:50:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:48:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	3.689	218.3E6	126.3E6	23.256	23.621
2) SA Decachlor...	8.743	8.695	201.1E6	62915084	25.556	26.013
Target Compounds						
26) L6 AR-1254-1	5.592	5.572	142.8E6	78551215	255.230	255.266
27) L6 AR-1254-2	5.741	5.720	117.7E6	67765666	243.403	252.395
28) L6 AR-1254-3	6.146	6.123	190.0E6	103.9E6	240.780	246.647
29) L6 AR-1254-4	6.376	6.351	124.9E6	61546138	256.767	251.838
30) L6 AR-1254-5	6.795	6.768	170.5E6	90324740	250.587	259.059



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 20:07
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:50:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:48:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

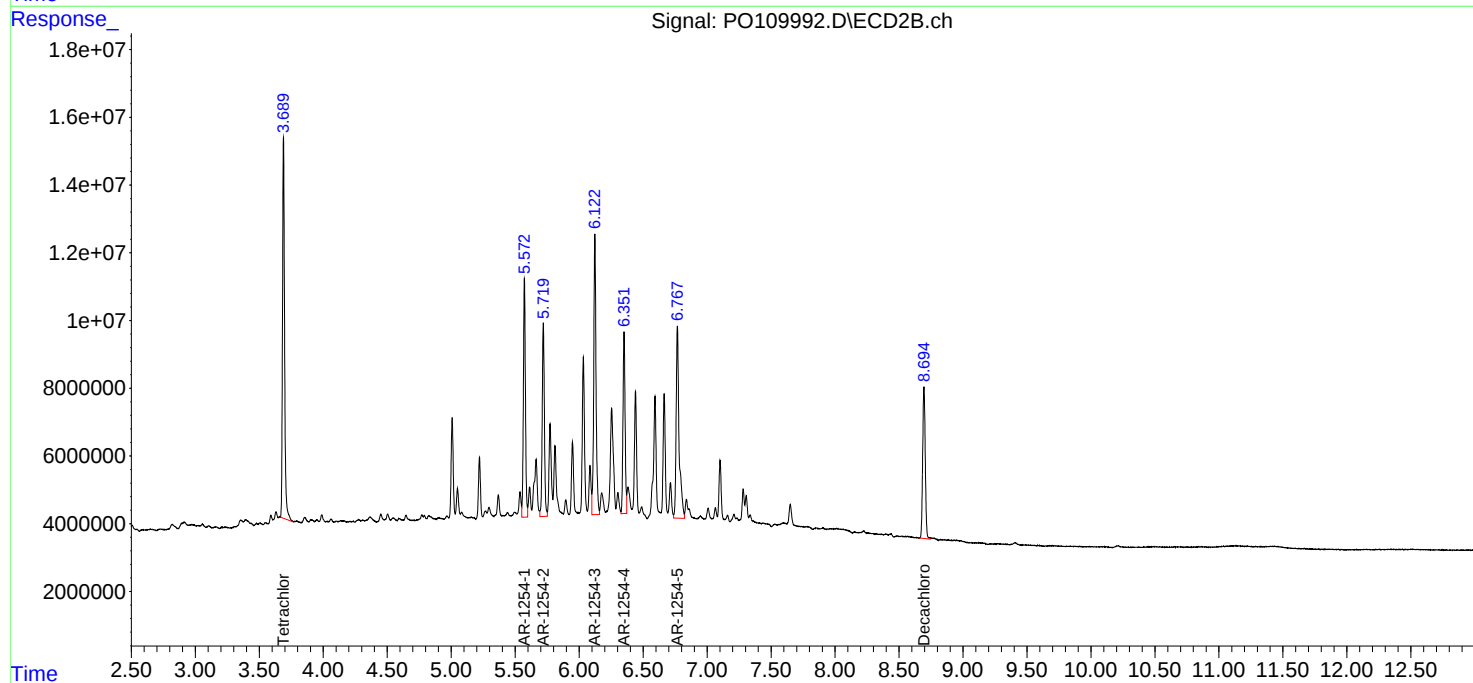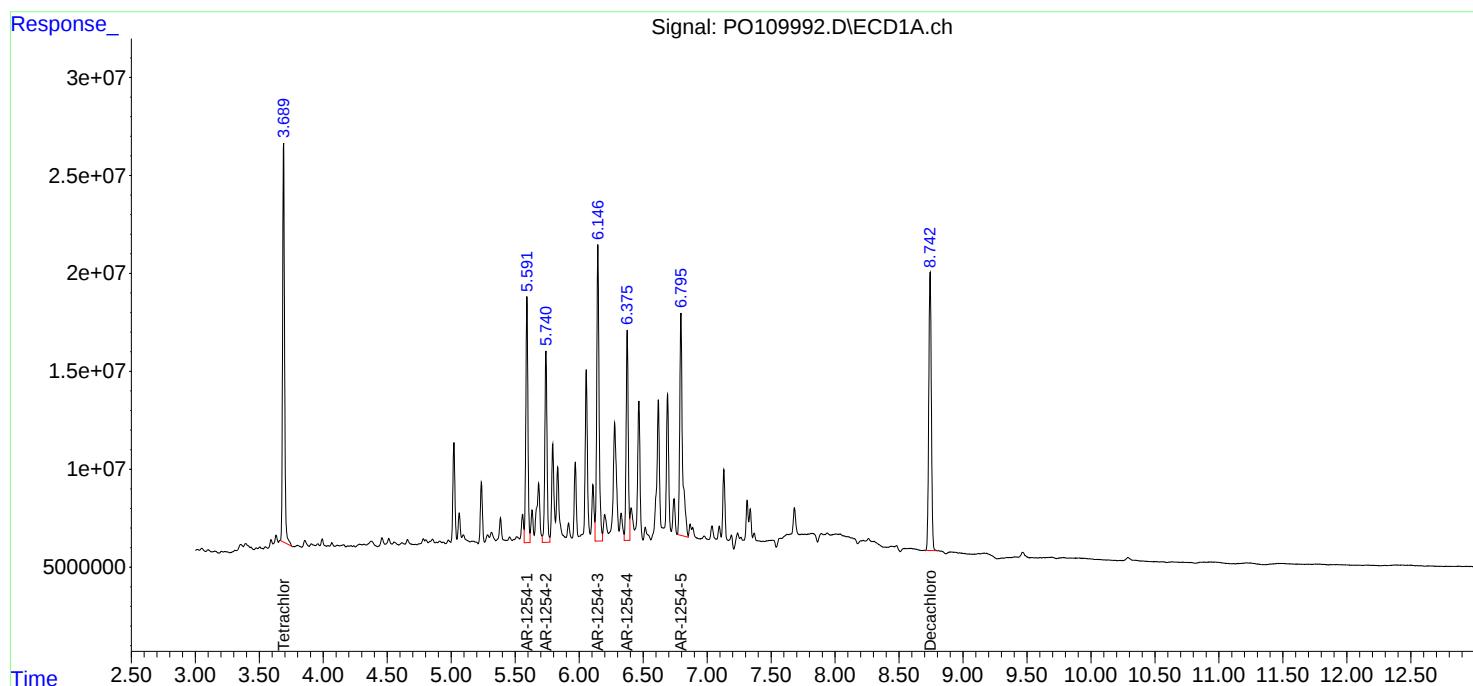

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 20:25
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:50:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:48:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	43445665	25306006	4.628	4.733
2) SA Decachlor...	8.743	8.694	41266656	13227136	5.245	5.469
Target Compounds						
26) L6 AR-1254-1	5.593	5.573	31329450	17649915	56.014	57.357
27) L6 AR-1254-2	5.742	5.720	26381750	15388259	54.541	57.314
28) L6 AR-1254-3	6.148	6.123	39484048	21241930	50.026	50.431
29) L6 AR-1254-4	6.377	6.350	23571245	12628885	48.456	51.676
30) L6 AR-1254-5	6.797	6.768	28479203	15116419	41.849	43.355m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 20:25
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:50:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:48:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

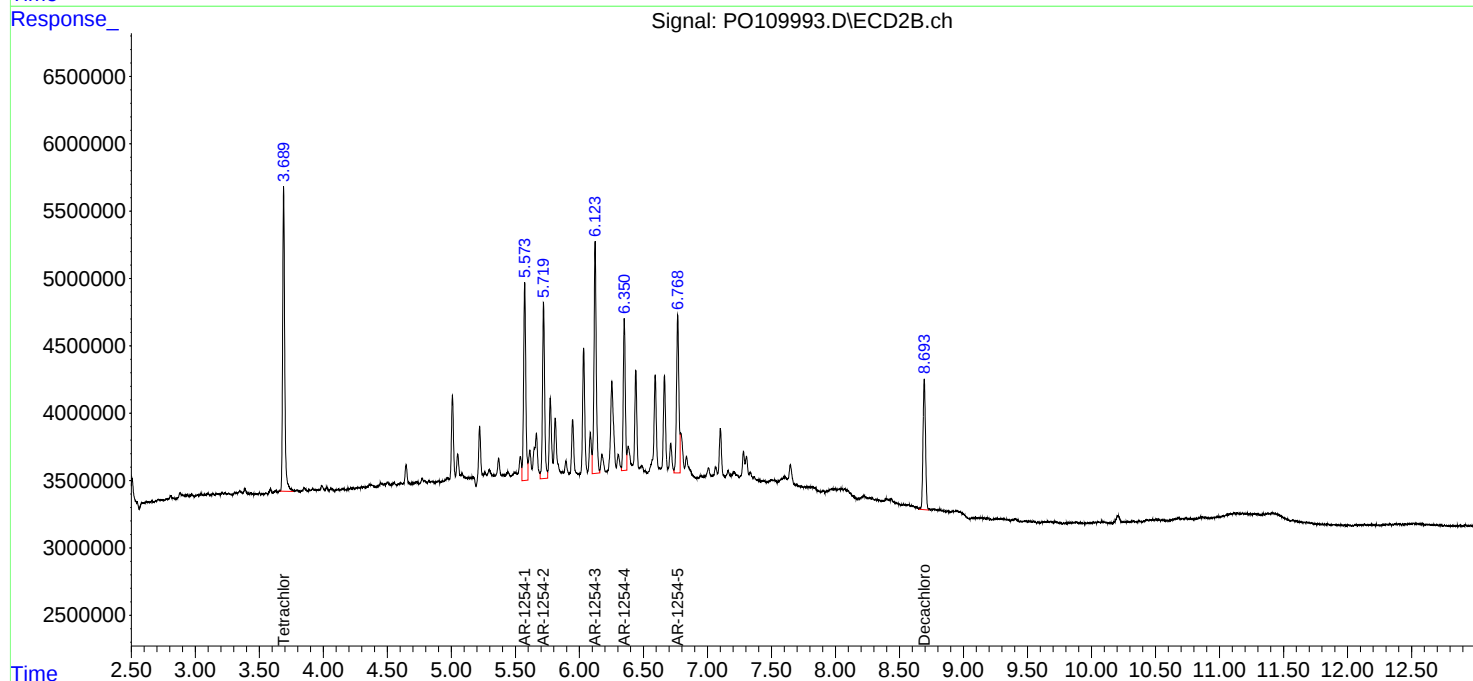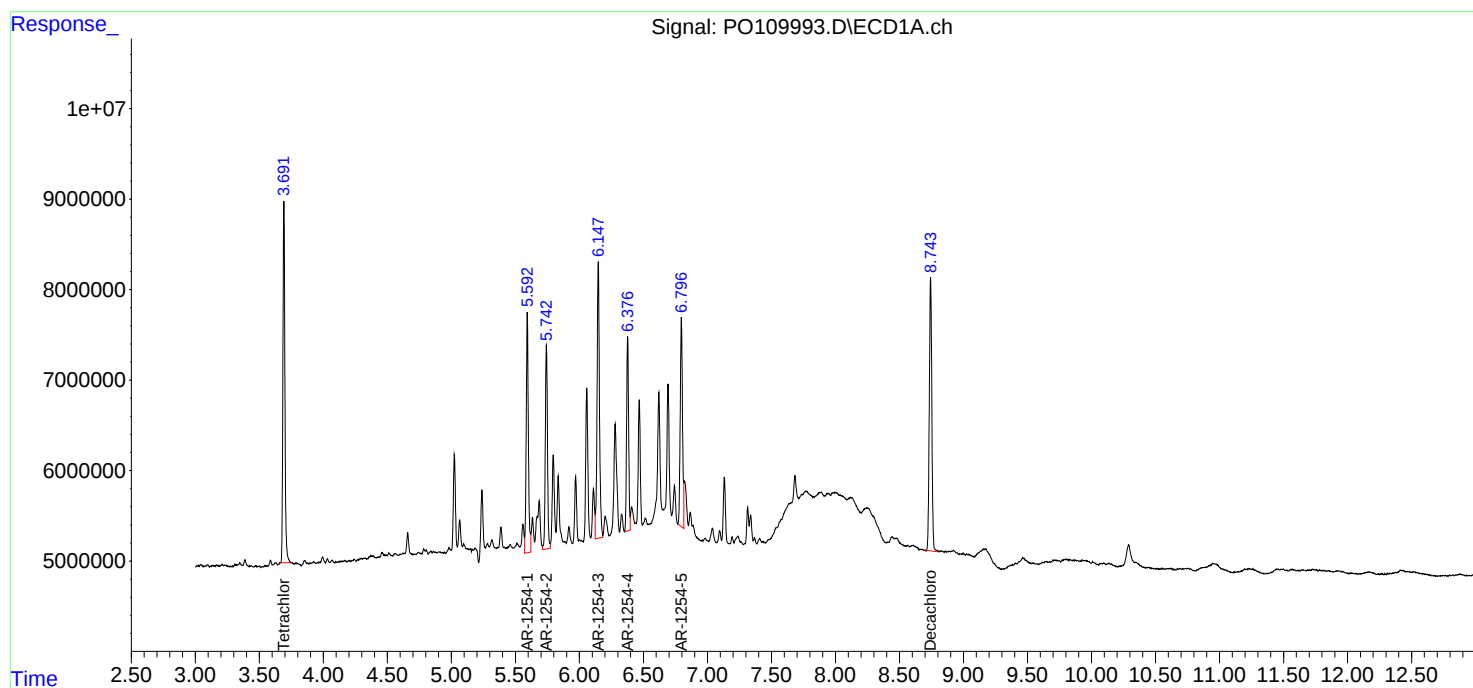

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031925\
 Data File : P0109994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 20:43
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:59:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:59:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	443.4E6	253.7E6	50.000	50.000
2) SA Decachlor...	8.744	8.695	383.2E6	113.8E6	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	6.836	6.807	344.1E6	172.2E6	500.000	500.000
37) L8 AR-1262-2	7.338	7.306	596.0E6	268.6E6	500.000	500.000
38) L8 AR-1262-3	7.623	7.590	235.3E6	97025324	500.000	500.000
39) L8 AR-1262-4	7.687	7.654	437.3E6	180.9E6	500.000	500.000
40) L8 AR-1262-5	8.184	8.146	197.2E6	70580972	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 20:43
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:59:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:59:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

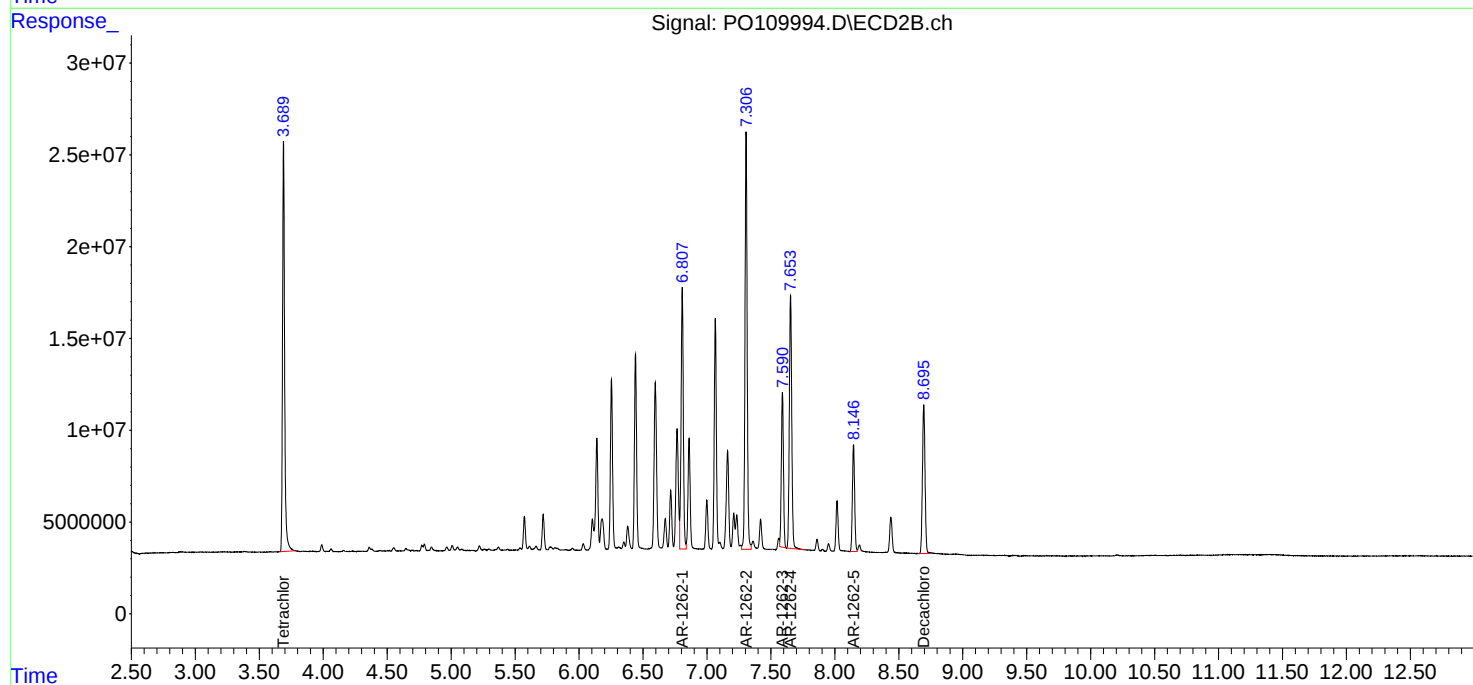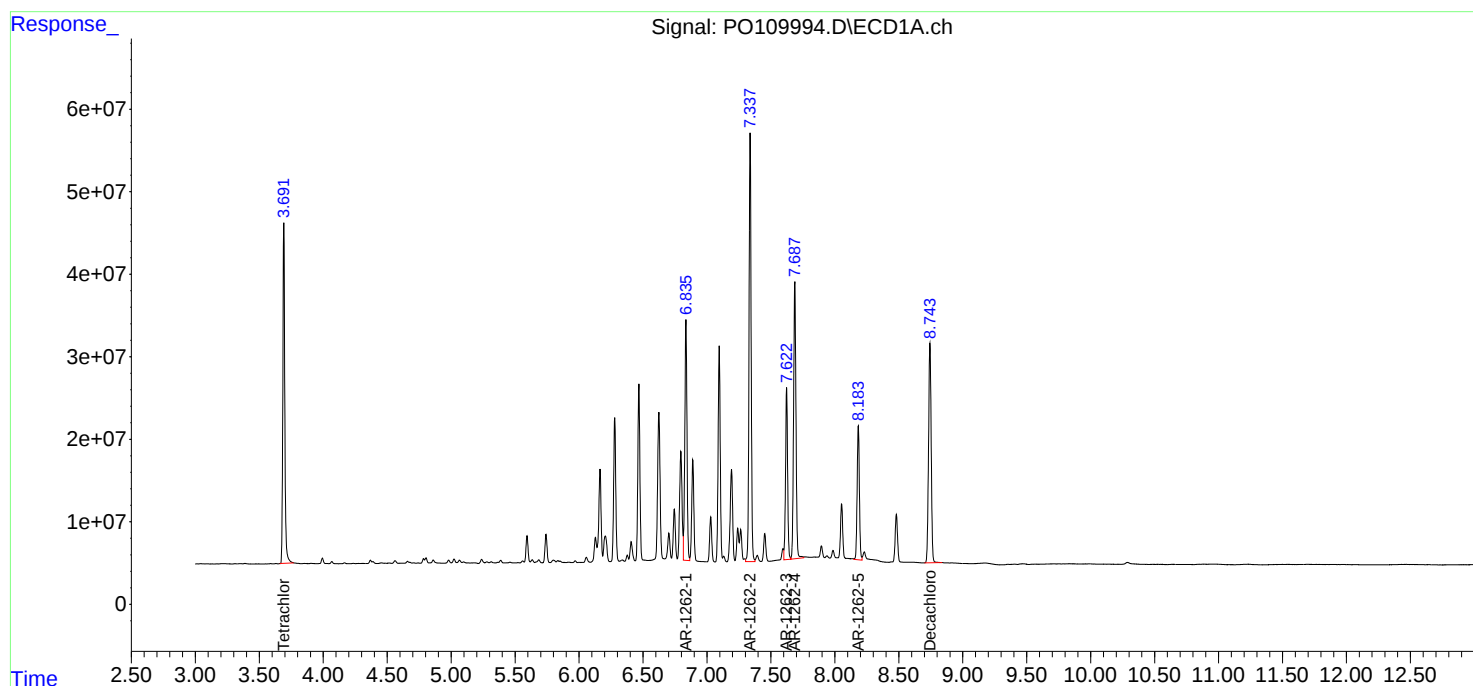

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 21:02
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:06:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:04:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	901.7E6	515.8E6	97.188	97.661
2) SA Decachlor...	8.743	8.696	1364.0E6	390.3E6	96.599	94.170
Target Compounds						
41) L9 AR-1268-1	7.623	7.590	1369.8E6	560.8E6	976.135	969.827
42) L9 AR-1268-2	7.688	7.655	1266.3E6	519.2E6	989.578	974.786
43) L9 AR-1268-3	7.896	7.862	1019.7E6	397.6E6	981.758	963.023
44) L9 AR-1268-4	8.183	8.147	432.7E6	153.8E6	967.005	949.196
45) L9 AR-1268-5	8.481	8.440	3202.1E6	963.7E6	991.799	976.212



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 21:02
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:06:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:04:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

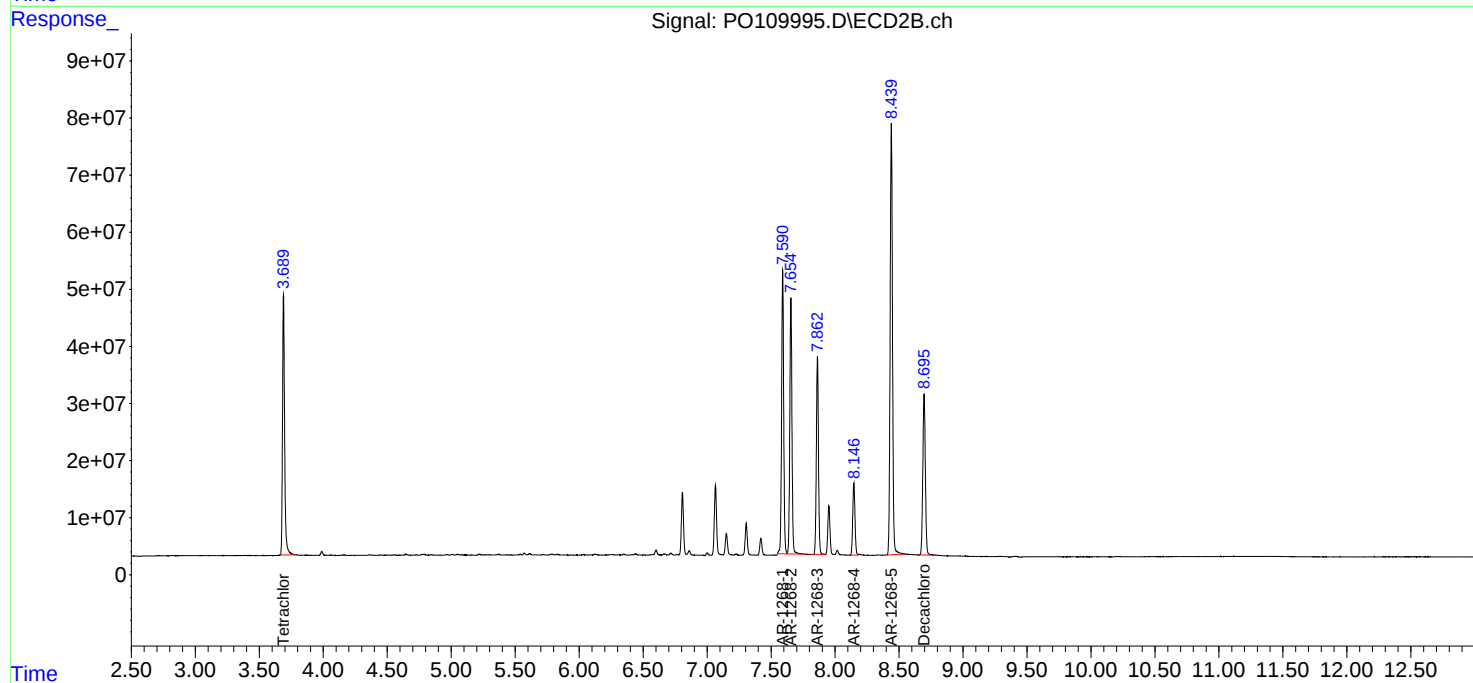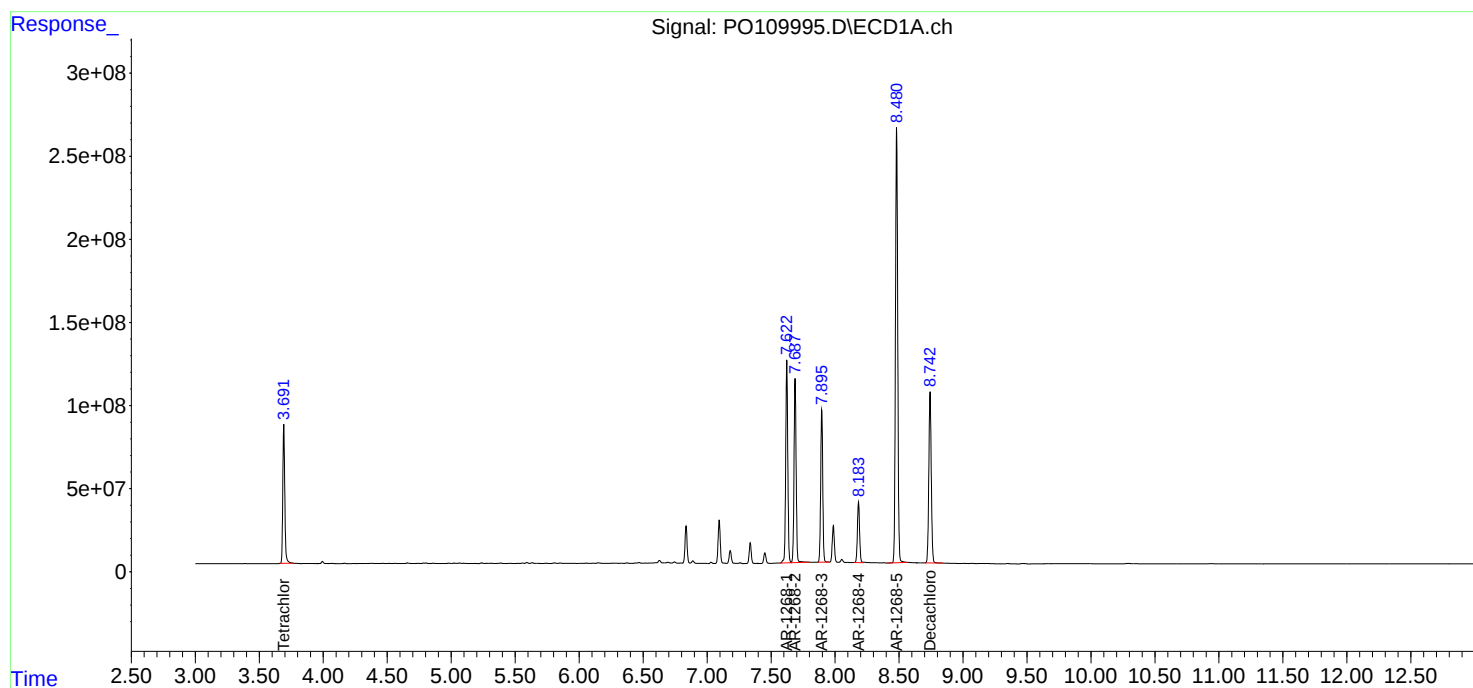

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0109996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 21:20
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:06:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:04:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	674.6E6	386.9E6	72.709	73.243
2) SA Decachlor...	8.743	8.696	1030.2E6	298.8E6	72.957	72.092
Target Compounds						
41) L9 AR-1268-1	7.624	7.590	1030.8E6	426.7E6	734.560	738.041
42) L9 AR-1268-2	7.688	7.655	947.1E6	394.0E6	740.097	739.739
43) L9 AR-1268-3	7.897	7.862	764.7E6	299.7E6	736.208	725.732
44) L9 AR-1268-4	8.184	8.147	316.0E6	116.0E6	706.276	715.999
45) L9 AR-1268-5	8.482	8.440	2394.2E6	724.9E6	741.545	734.374


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 21:20
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:06:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:04:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

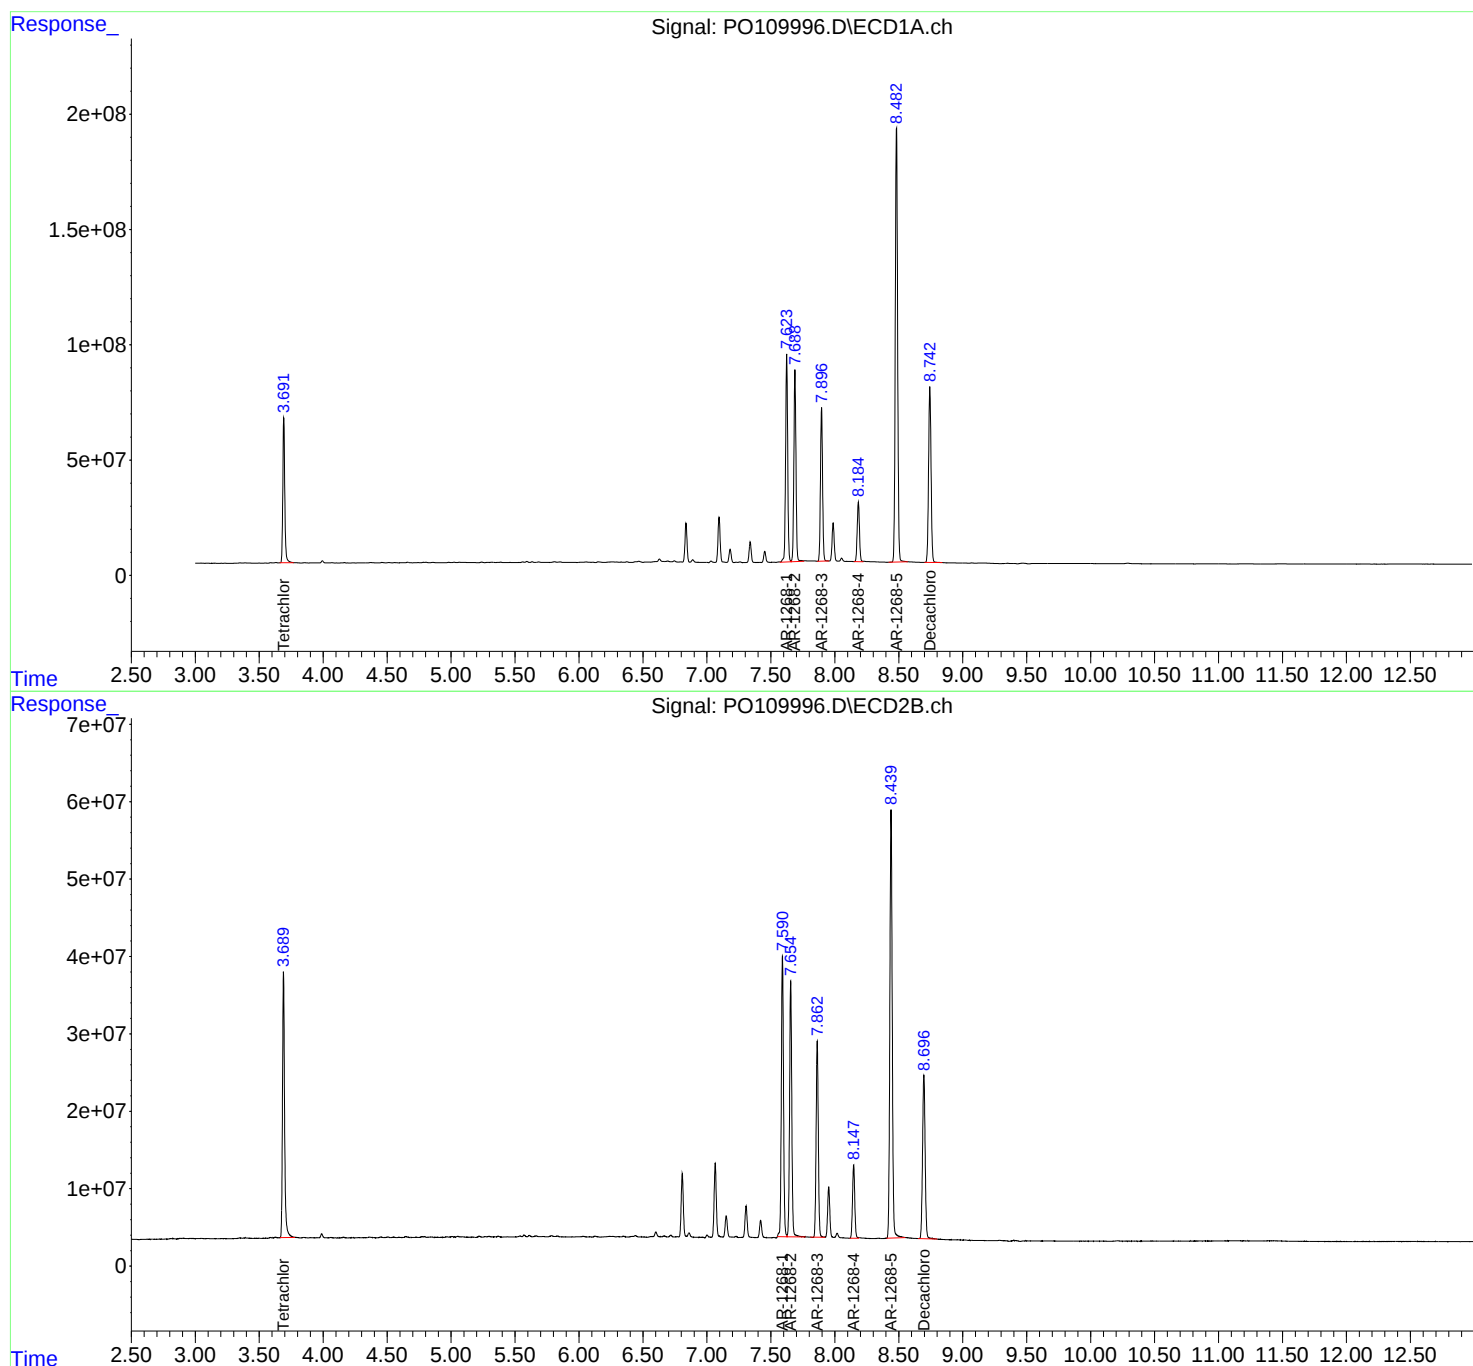

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031925\
 Data File : P0109997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 21:39
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1268ICC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:06:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:04:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	463.9E6	264.1E6	50.000	50.000
2) SA Decachlor...	8.743	8.694	706.0E6	207.2E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	7.622	7.589	700.7E6	289.1E6	499.305m	500.000
42) L9 AR-1268-2	7.688	7.653	639.8E6	266.3E6	500.000	500.000
43) L9 AR-1268-3	7.896	7.861	519.3E6	206.5E6	500.000	500.000
44) L9 AR-1268-4	8.185	8.145	223.7E6	81011977	500.000	500.000
45) L9 AR-1268-5	8.482	8.439	1614.3E6	493.6E6	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 21:39
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:06:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:04:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

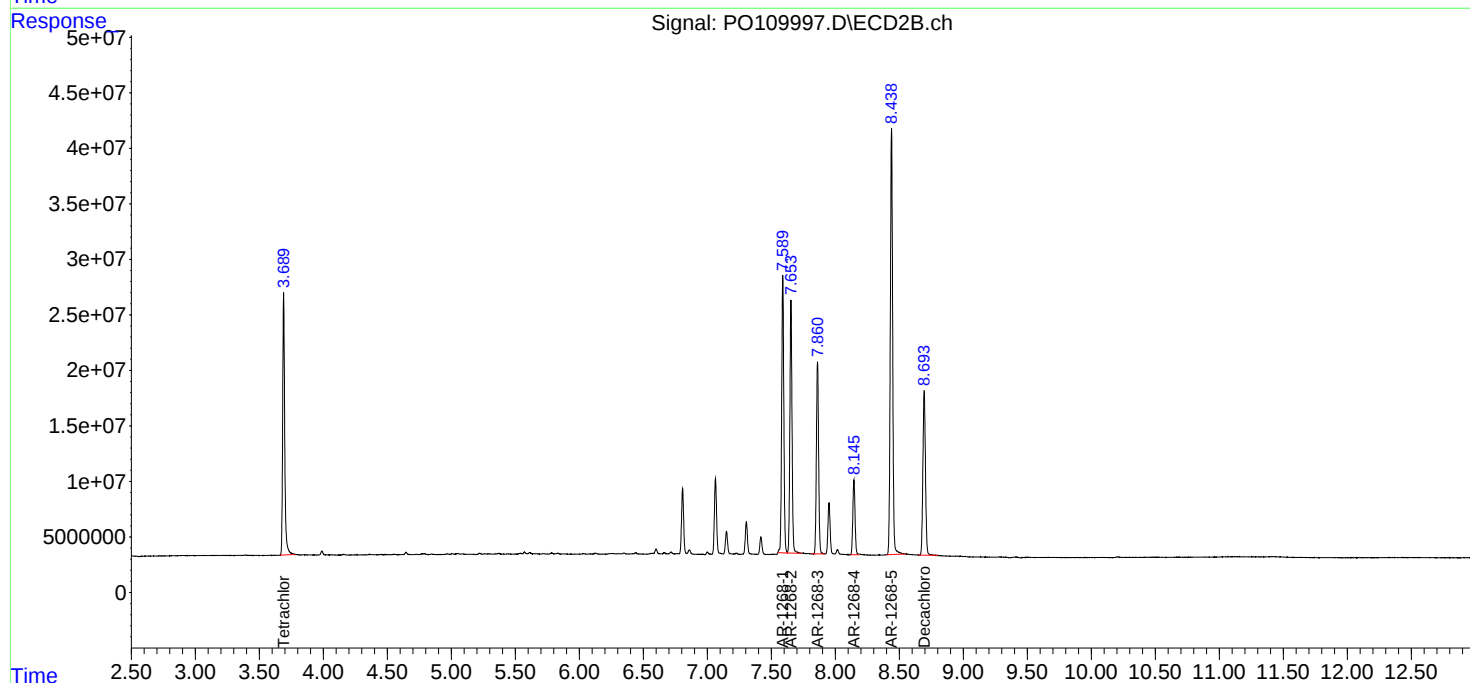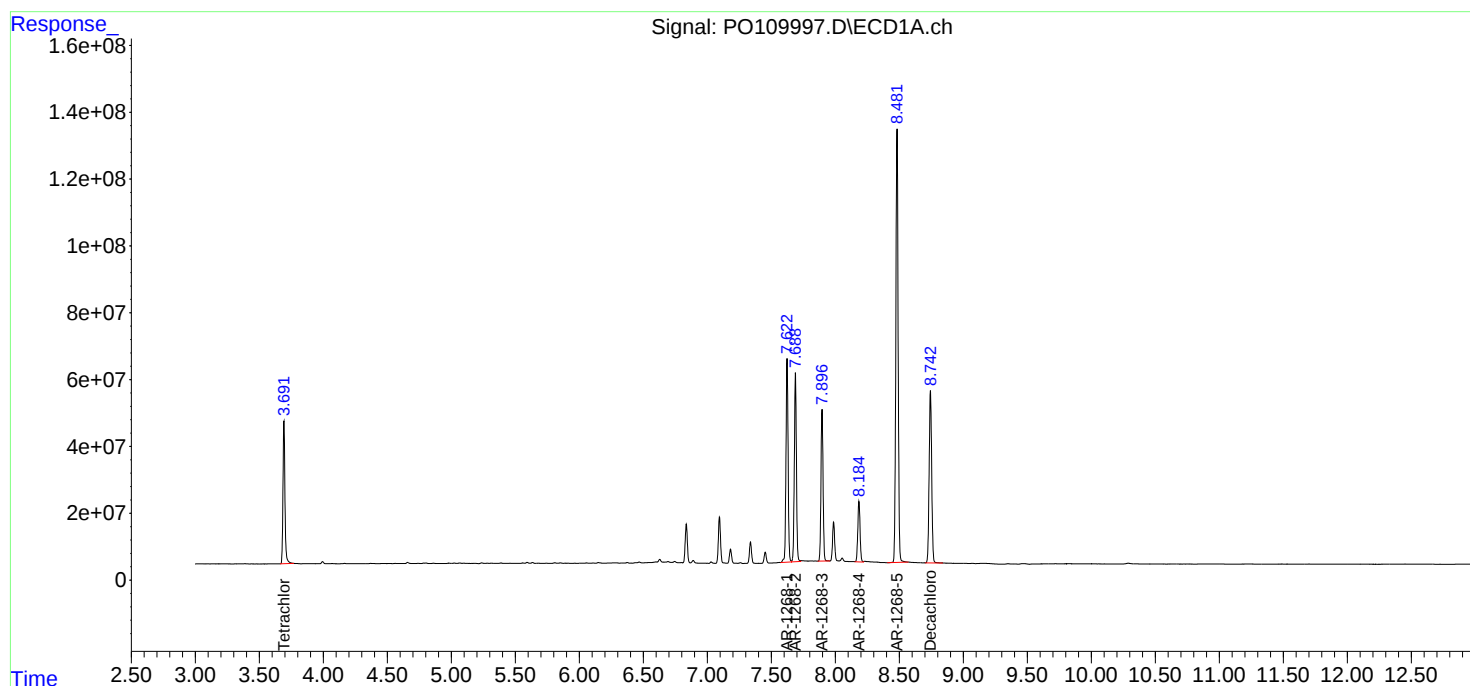

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031925\
 Data File : P0109998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 21:57
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1268ICC250

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:06:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:04:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.690	233.0E6	133.0E6	25.112	25.182
2) SA Decachlor...	8.743	8.695	364.2E6	110.3E6	25.791	26.624
Target Compounds						
41) L9 AR-1268-1	7.623	7.590	357.9E6	149.6E6	255.005m	258.814
42) L9 AR-1268-2	7.688	7.654	330.4E6	137.2E6	258.196	257.558
43) L9 AR-1268-3	7.897	7.861	264.1E6	107.0E6	254.288	259.017
44) L9 AR-1268-4	8.184	8.146	118.3E6	42174671	264.470	260.299
45) L9 AR-1268-5	8.482	8.439	811.9E6	254.0E6	251.483	257.325

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO109998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 21:57
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:06:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:04:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

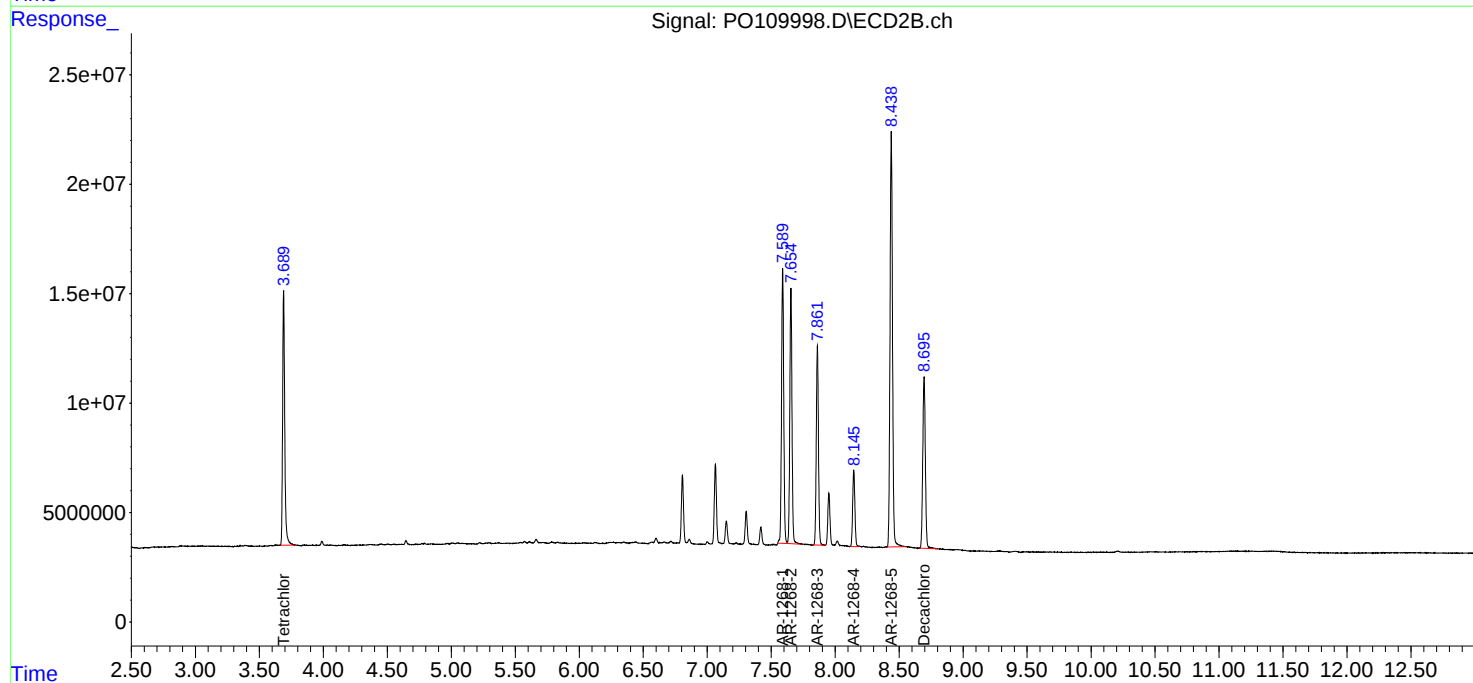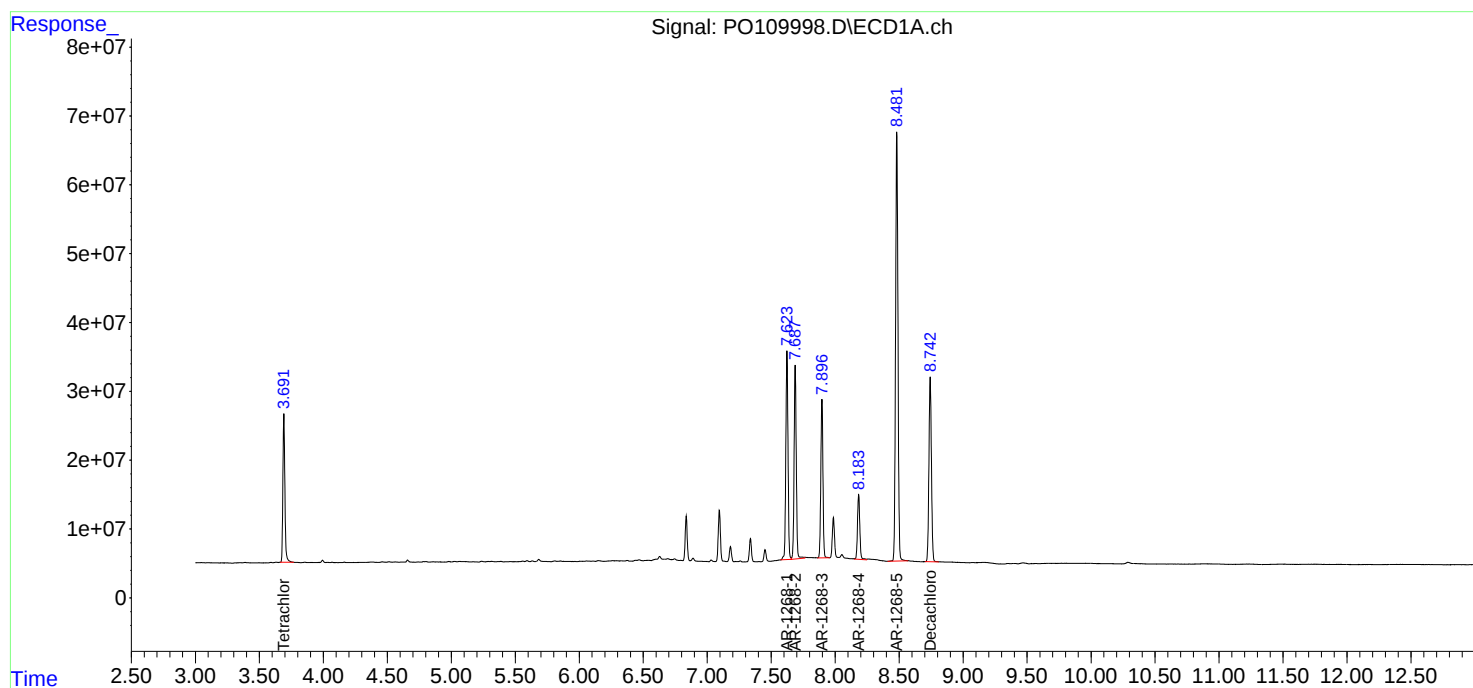

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031925\
 Data File : P0109999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 22:15
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/19/2025
 Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:07:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:04:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.688	44374914	25645349	4.783m	4.855m
2) SA Decachlor...	8.743	8.695	72973489	22764198	5.168	5.493
Target Compounds						
41) L9 AR-1268-1	7.622	7.590	71178847	31006348	50.721m	53.625
42) L9 AR-1268-2	7.688	7.654	63525178	28112917	49.643	52.781
43) L9 AR-1268-3	7.896	7.861	50172519	22018734	48.306	53.325
44) L9 AR-1268-4	8.183	8.146	21758650	8301200	48.629m	51.234
45) L9 AR-1268-5	8.481	8.438	151.8E6	51592382	47.022	52.264

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO031925\
Data File : PO109999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 22:15
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/19/2025
Supervised By :mohammad ahmed 03/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:07:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:04:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

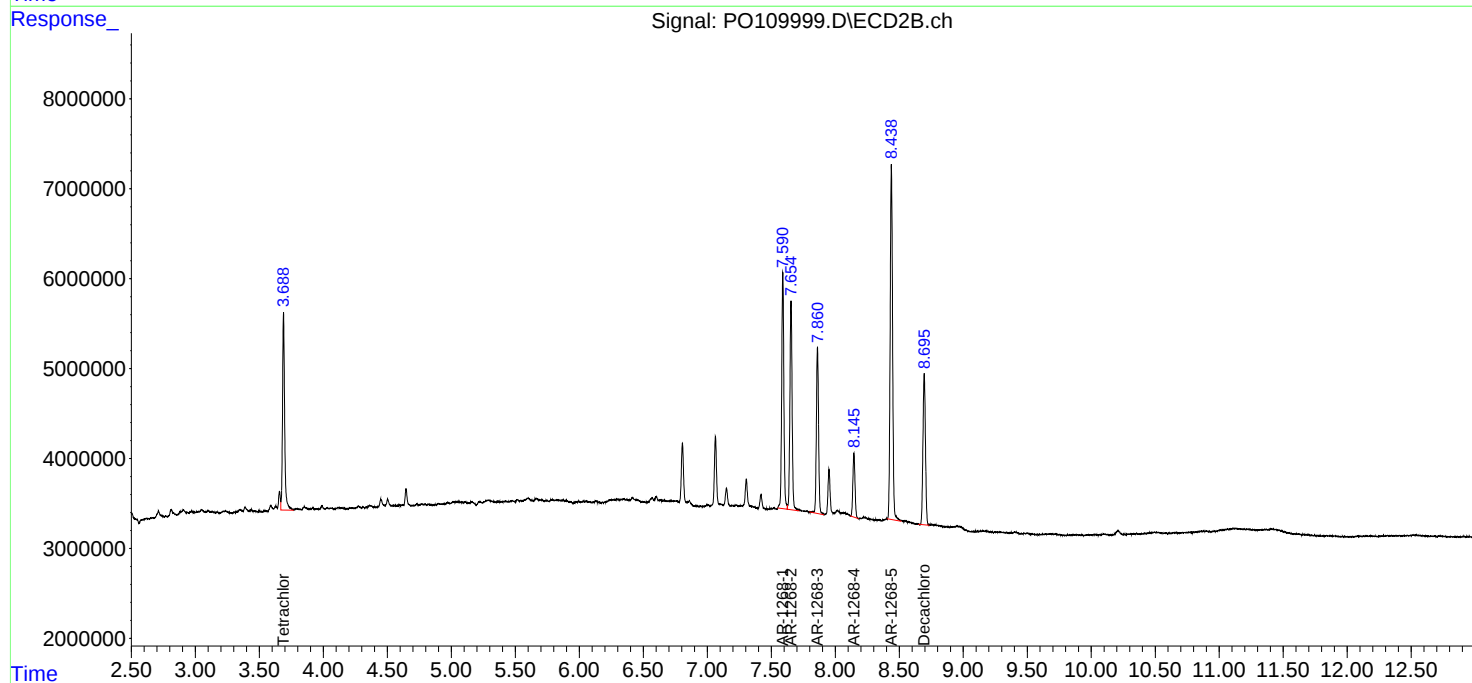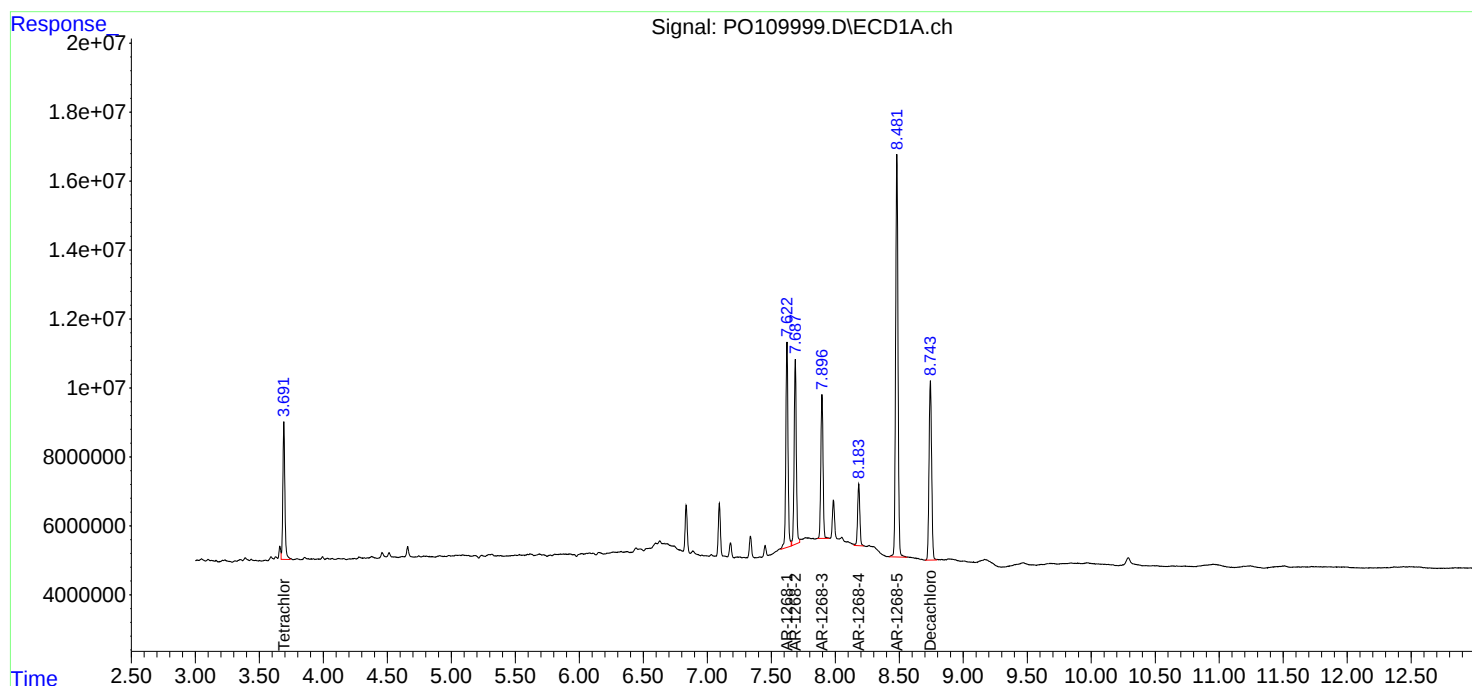

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0110000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 22:34
 Operator : YP/AJ
 Sample : P0031925ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO031925

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:41:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:39:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	445.5E6	261.7E6	48.943	49.897
2) SA Decachlor...	8.744	8.696	386.1E6	117.6E6	50.211	48.467
Target Compounds						
3) L1 AR-1016-1	4.784	4.771	165.3E6	89338991	491.286	487.512
4) L1 AR-1016-2	4.804	4.790	229.3E6	128.0E6	494.517	489.369
5) L1 AR-1016-3	4.860	4.966	158.0E6	69159098	492.753	487.796
6) L1 AR-1016-4	4.981	5.008	124.5E6	57510192	492.750	487.665
7) L1 AR-1016-5	5.238	5.221	133.3E6	74393726	484.896	486.492
31) L7 AR-1260-1	6.280	6.253	235.0E6	125.1E6	498.624	489.686
32) L7 AR-1260-2	6.469	6.441	287.0E6	145.2E6	481.955	483.545
33) L7 AR-1260-3	6.837	6.594	243.8E6	137.4E6	502.299	475.363
34) L7 AR-1260-4	7.097	7.065	212.4E6	103.8E6	500.751	482.426
35) L7 AR-1260-5	7.339	7.306	531.0E6	241.3E6	507.683	483.788



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
Data File : P0110000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 22:34
Operator : YP/AJ
Sample : P0031925ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO031925

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:41:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:39:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

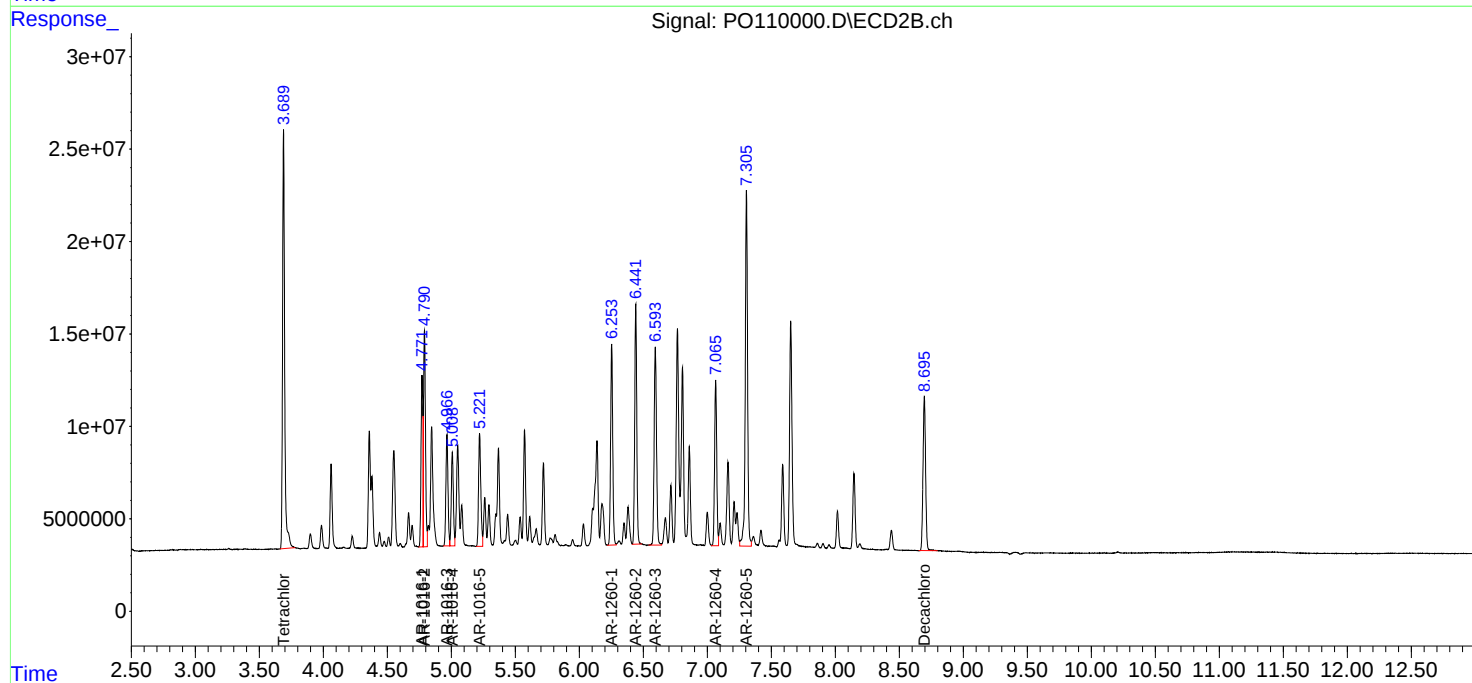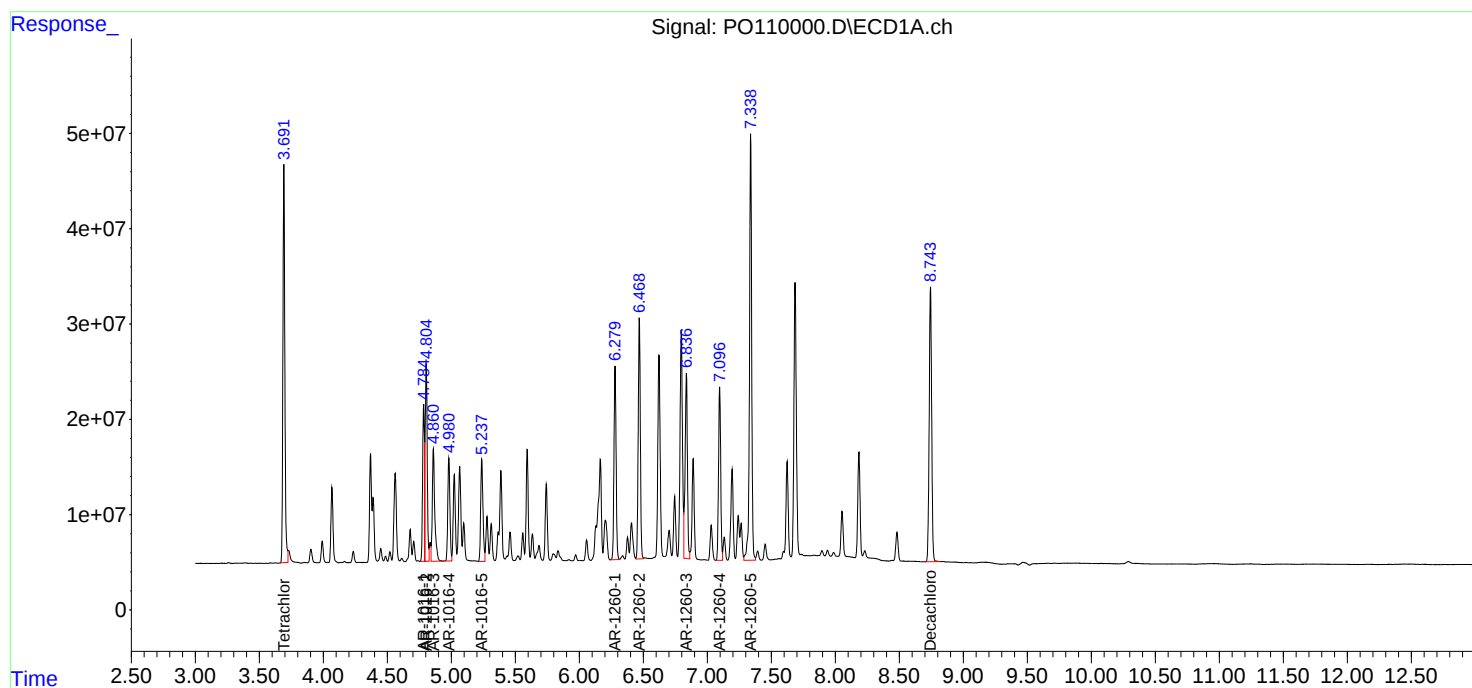

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0110001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 23:47
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO031925AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:45:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:43:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.692	3.689	445.5E6	254.1E6	52.578	52.663
2)	SA Decachlor...	8.744	8.695	378.1E6	113.8E6	52.496	50.899
Target Compounds							
16)	L4 AR-1242-1	4.785	4.771	138.5E6	75308322	517.896	515.050
17)	L4 AR-1242-2	4.804	4.791	190.3E6	107.0E6	516.964	514.473
18)	L4 AR-1242-3	4.861	4.966	132.7E6	58059678	514.485	520.188
19)	L4 AR-1242-4	4.981	5.050	104.1E6	58816332	520.236	507.140
20)	L4 AR-1242-5	5.634	5.572	109.1E6	71078329	516.760	517.905



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
Data File : P0110001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 23:47
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO031925AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:45:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:43:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

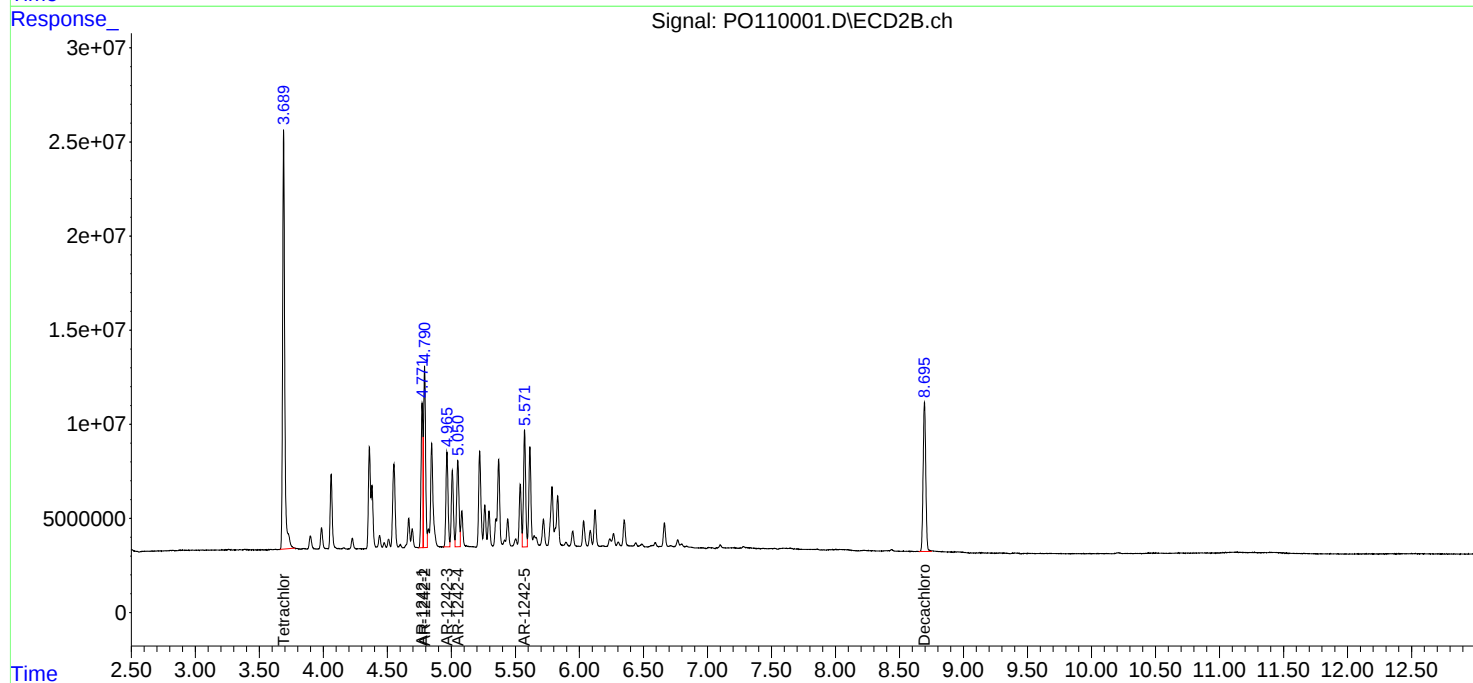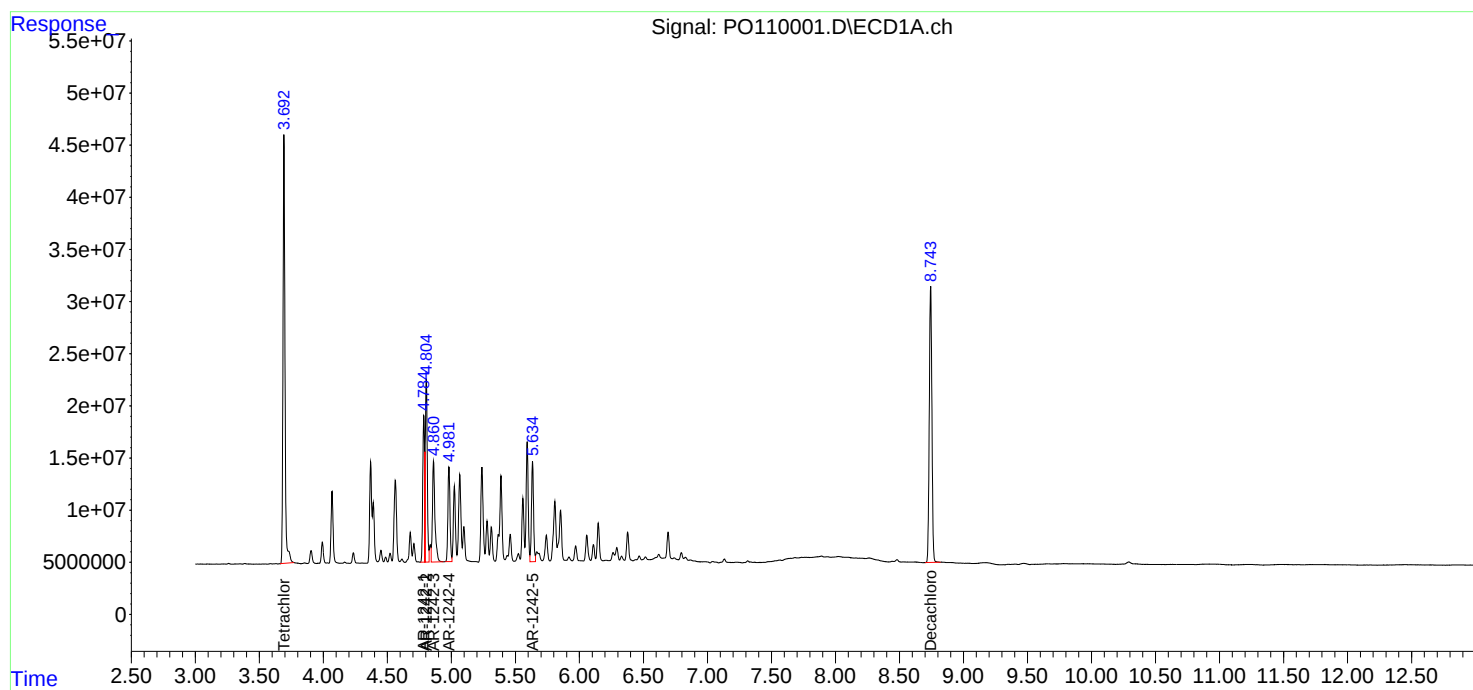

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0110002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2025 00:05
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO031925AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:41:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:38:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.692	3.689	453.1E6	257.7E6	48.851	48.659
2)	SA Decachlor...	8.743	8.695	387.8E6	116.2E6	49.748	49.559
Target Compounds							
21)	L5 AR-1248-1	4.784	4.771	108.4E6	58618795	492.939	487.181
22)	L5 AR-1248-2	5.023	5.008	147.5E6	82104463	489.895	487.213
23)	L5 AR-1248-3	5.238	5.050	184.5E6	87652547	492.701	489.391
24)	L5 AR-1248-4	5.592	5.221	258.0E6	102.0E6	493.069	489.250
25)	L5 AR-1248-5	5.634	5.613	182.7E6	99745645	494.045	489.737



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO110002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2025 00:05
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO031925AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:41:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:38:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

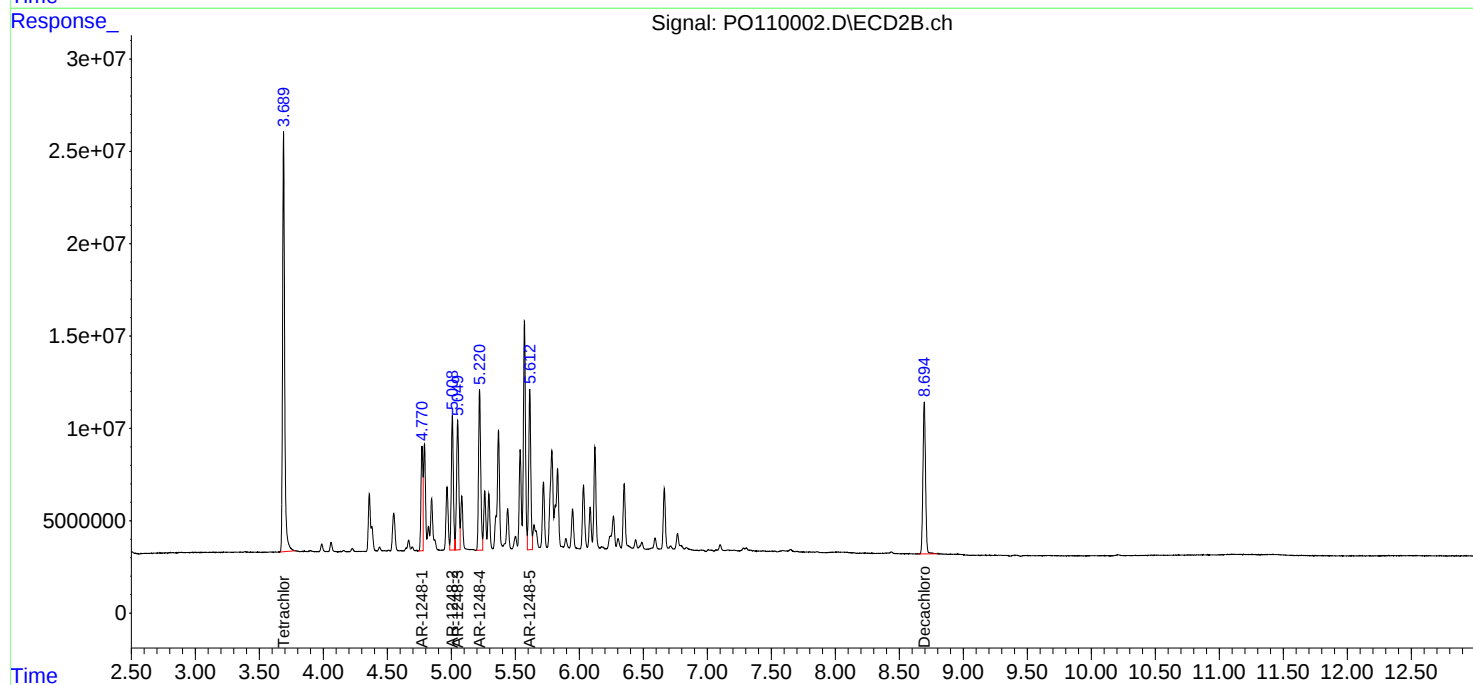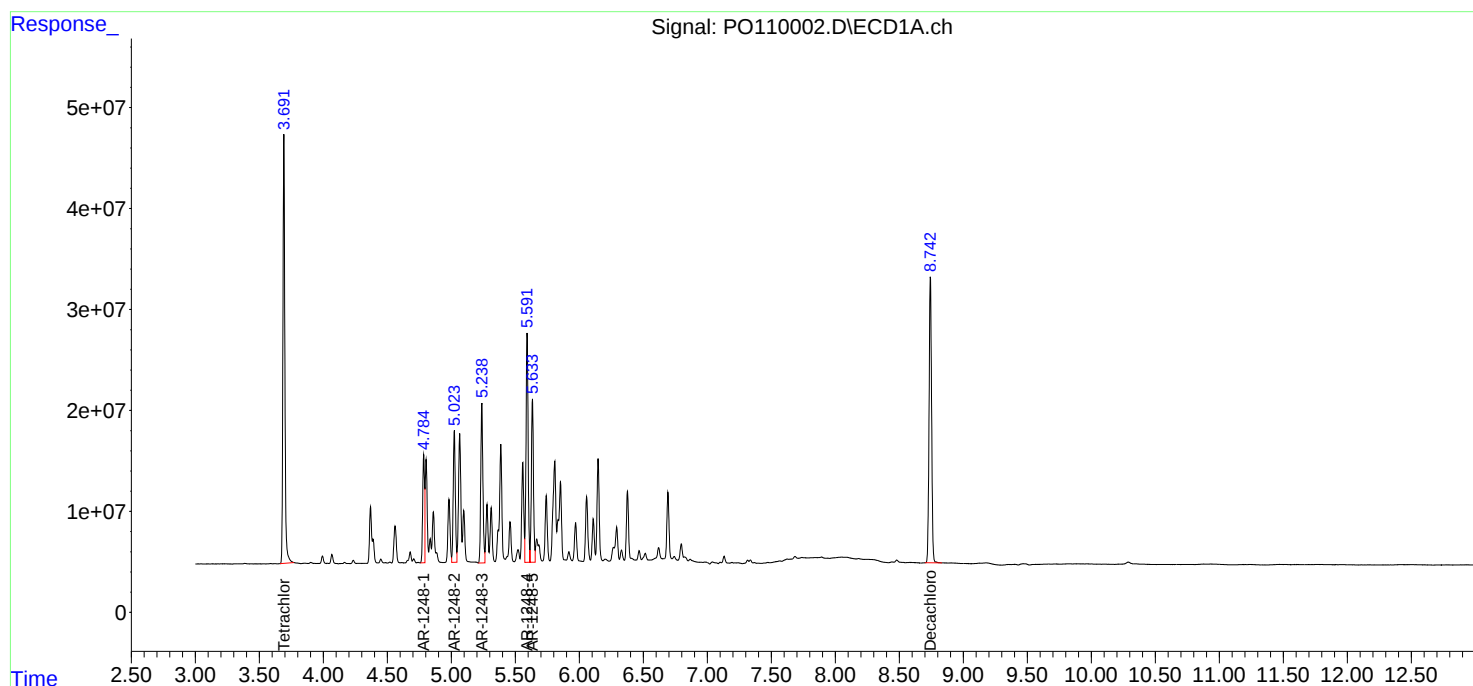

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0110003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2025 00:24
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO031925AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:50:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 01:48:40 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	450.3E6	255.9E6	47.966	47.857
2) SA Decachlor...	8.743	8.695	386.1E6	115.4E6	49.078	47.699
Target Compounds						
26) L6 AR-1254-1	5.593	5.572	270.9E6	148.9E6	484.350	483.813
27) L6 AR-1254-2	5.743	5.720	234.3E6	129.7E6	484.326	483.086
28) L6 AR-1254-3	6.148	6.123	381.8E6	203.6E6	483.781	483.489
29) L6 AR-1254-4	6.377	6.350	236.7E6	117.7E6	486.513	481.783
30) L6 AR-1254-5	6.797	6.768	332.2E6	169.1E6	488.082	485.104



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031925\
Data File : PO110003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2025 00:24
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO031925AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:50:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 01:48:40 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

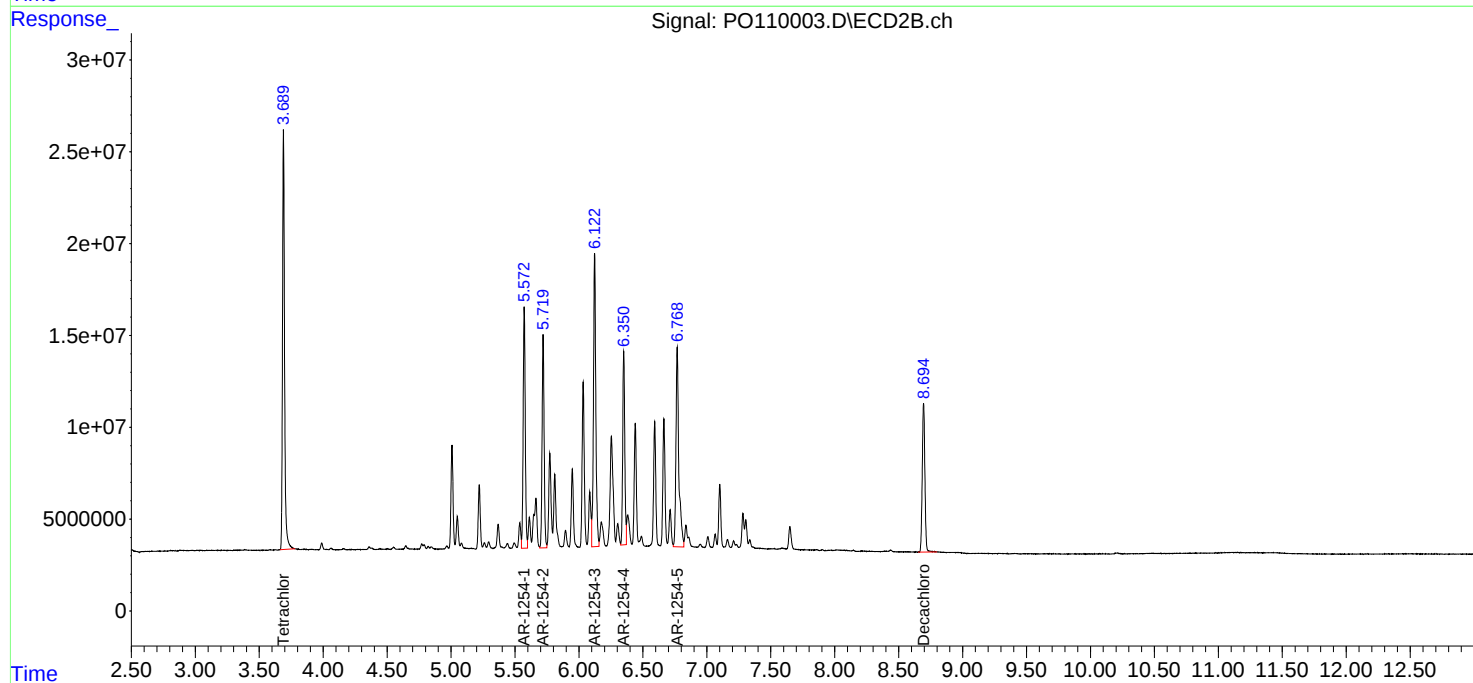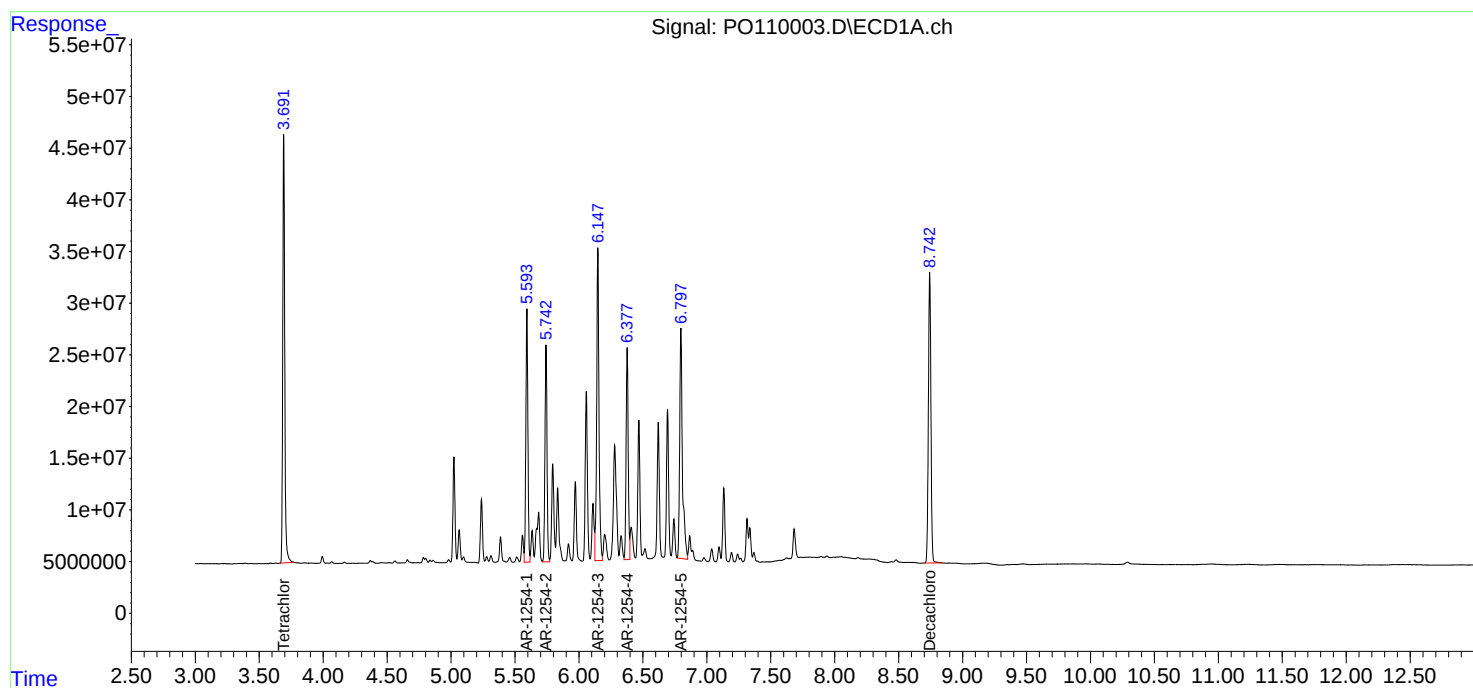

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : P0110004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2025 00:42
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO031925AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:07:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:04:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.690	450.4E6	255.9E6	48.546	48.447
2) SA Decachlor...	8.744	8.696	690.0E6	201.4E6	48.863	48.609
Target Compounds						
41) L9 AR-1268-1	7.624	7.590	683.9E6	280.8E6	487.341	485.631
42) L9 AR-1268-2	7.689	7.654	622.6E6	259.1E6	486.560	486.478
43) L9 AR-1268-3	7.897	7.862	509.4E6	200.7E6	490.473	486.052
44) L9 AR-1268-4	8.184	8.146	217.2E6	79710818	485.391	491.969
45) L9 AR-1268-5	8.482	8.440	1574.6E6	478.9E6	487.695	485.135



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO031925\
Data File : PO110004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2025 00:42
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
ICVPO031925AR1268

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:07:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:04:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

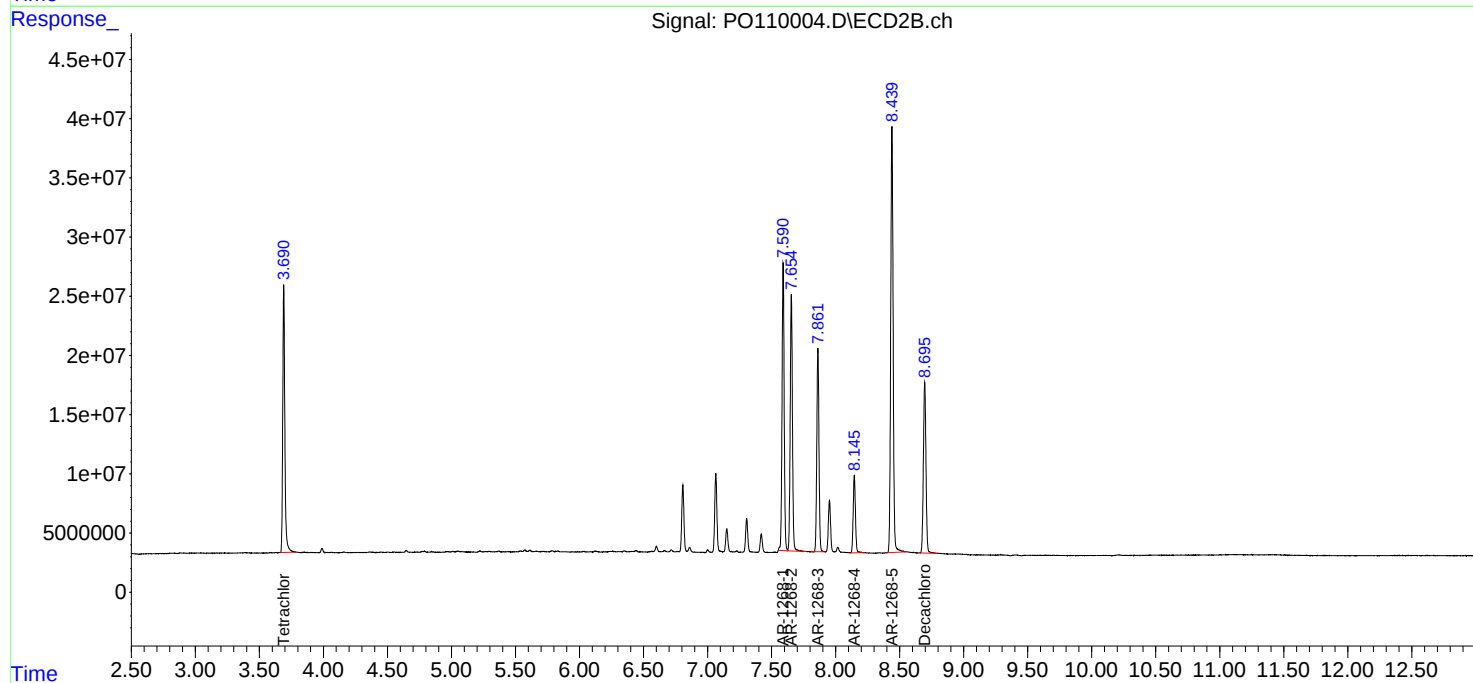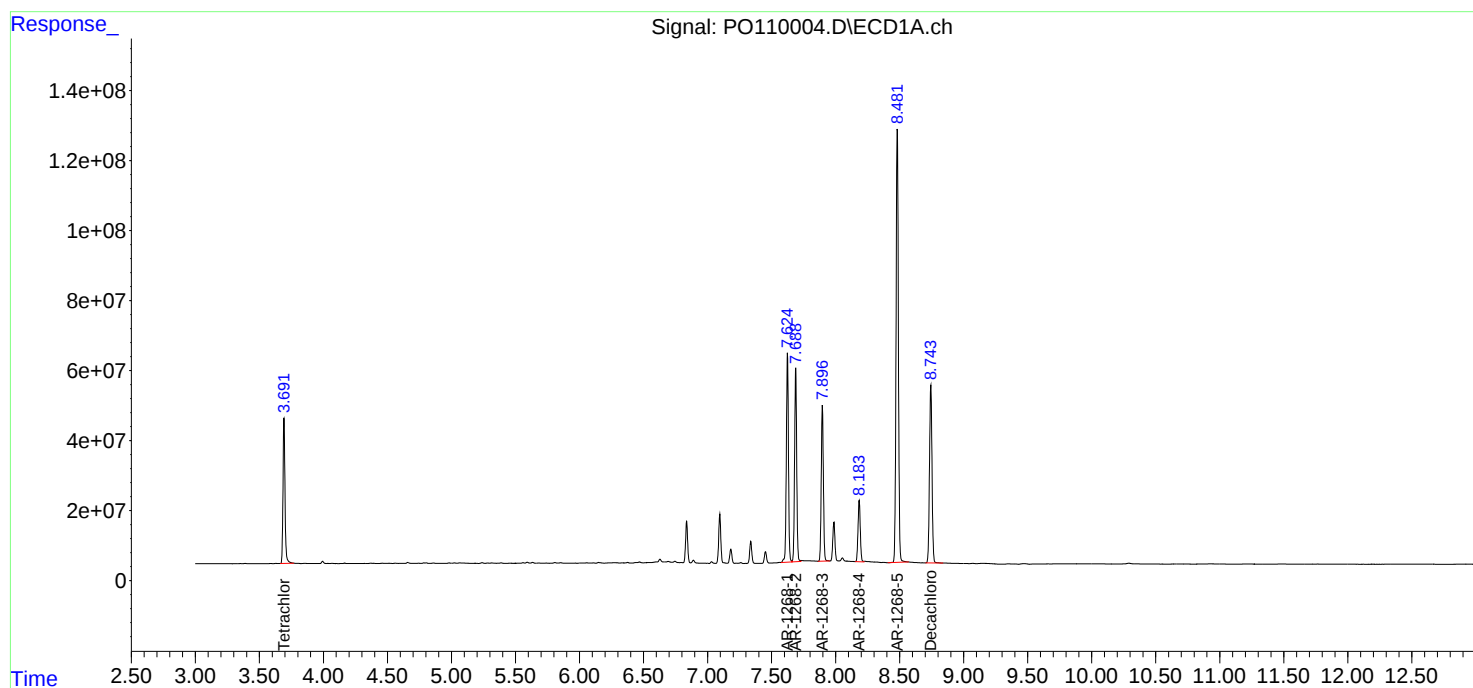



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 09:46 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-2	(2)	4.80	4.80	4.70	4.90	0.00
Aroclor-1016-3	(3)	4.86	4.86	4.76	4.96	0.00
Aroclor-1016-4	(4)	4.98	4.98	4.88	5.08	0.00
Aroclor-1016-5	(5)	5.24	5.24	5.14	5.34	0.00
Aroclor-1260-1	(1)	6.28	6.28	6.18	6.38	0.00
Aroclor-1260-2	(2)	6.47	6.47	6.37	6.57	0.00
Aroclor-1260-3	(3)	6.84	6.84	6.74	6.94	0.00
Aroclor-1260-4	(4)	7.10	7.10	7.00	7.20	0.00
Aroclor-1260-5	(5)	7.34	7.34	7.24	7.44	0.00
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.74	8.75	8.65	8.85	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 09:46 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2	(2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3	(3)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-4	(4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5	(5)	5.22	5.22	5.12	5.32	0.00
Aroclor-1260-1	(1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2	(2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3	(3)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-4	(4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5	(5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.69	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL01 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110263.D Time Analyzed: 09:46

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.784	4.685	4.885	533.050	500.000	6.6
Aroclor-1016-2	4.803	4.704	4.904	532.950	500.000	6.6
Aroclor-1016-3	4.860	4.761	4.961	534.220	500.000	6.8
Aroclor-1016-4	4.980	4.881	5.081	533.580	500.000	6.7
Aroclor-1016-5	5.238	5.139	5.339	534.560	500.000	6.9
Aroclor-1260-1	6.279	6.180	6.380	540.840	500.000	8.2
Aroclor-1260-2	6.467	6.369	6.569	507.690	500.000	1.5
Aroclor-1260-3	6.835	6.737	6.937	498.120	500.000	-0.4
Aroclor-1260-4	7.096	6.998	7.198	486.870	500.000	-2.6
Aroclor-1260-5	7.337	7.239	7.439	480.250	500.000	-4.0
Decachlorobiphenyl	8.742	8.645	8.845	57.530	50.000	15.1
Tetrachloro-m-xylene	3.692	3.592	3.792	53.720	50.000	7.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL01 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110263.D Time Analyzed: 09:46

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.769	4.672	4.872	509.410	500.000	1.9
Aroclor-1016-2	4.788	4.691	4.891	506.900	500.000	1.4
Aroclor-1016-3	4.964	4.867	5.067	511.350	500.000	2.3
Aroclor-1016-4	5.005	4.909	5.109	504.600	500.000	0.9
Aroclor-1016-5	5.219	5.122	5.322	510.930	500.000	2.2
Aroclor-1260-1	6.250	6.155	6.355	495.180	500.000	-1.0
Aroclor-1260-2	6.438	6.342	6.542	487.390	500.000	-2.5
Aroclor-1260-3	6.591	6.495	6.695	473.050	500.000	-5.4
Aroclor-1260-4	7.062	6.967	7.167	467.970	500.000	-6.4
Aroclor-1260-5	7.302	7.207	7.407	455.220	500.000	-9.0
Decachlorobiphenyl	8.690	8.596	8.796	48.910	50.000	-2.2
Tetrachloro-m-xylene	3.687	3.590	3.790	52.660	50.000	5.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 09:46
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 12:29:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.687	489.0E6	276.2E6	53.724	52.660
2) SA Decachlor...	8.742	8.690	442.3E6	118.7E6	57.530	48.907
Target Compounds						
3) L1 AR-1016-1	4.784	4.769	179.4E6	93351070	533.053	509.405
4) L1 AR-1016-2	4.803	4.788	247.1E6	132.6E6	532.949	506.901
5) L1 AR-1016-3	4.860	4.964	171.3E6	72498019	534.221	511.346
6) L1 AR-1016-4	4.980	5.005	134.8E6	59506839	533.582	504.596
7) L1 AR-1016-5	5.238	5.219	146.9E6	78129978	534.558	510.925
31) L7 AR-1260-1	6.279	6.250	254.9E6	126.5E6	540.836	495.179
32) L7 AR-1260-2	6.467	6.438	302.3E6	146.4E6	507.691	487.393
33) L7 AR-1260-3	6.835	6.591	241.7E6	136.7E6	498.121	473.054
34) L7 AR-1260-4	7.096	7.062	206.5E6	100.7E6	486.872	467.969
35) L7 AR-1260-5	7.337	7.302	502.3E6	227.0E6	480.254	455.222



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 09:46
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 12:29:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

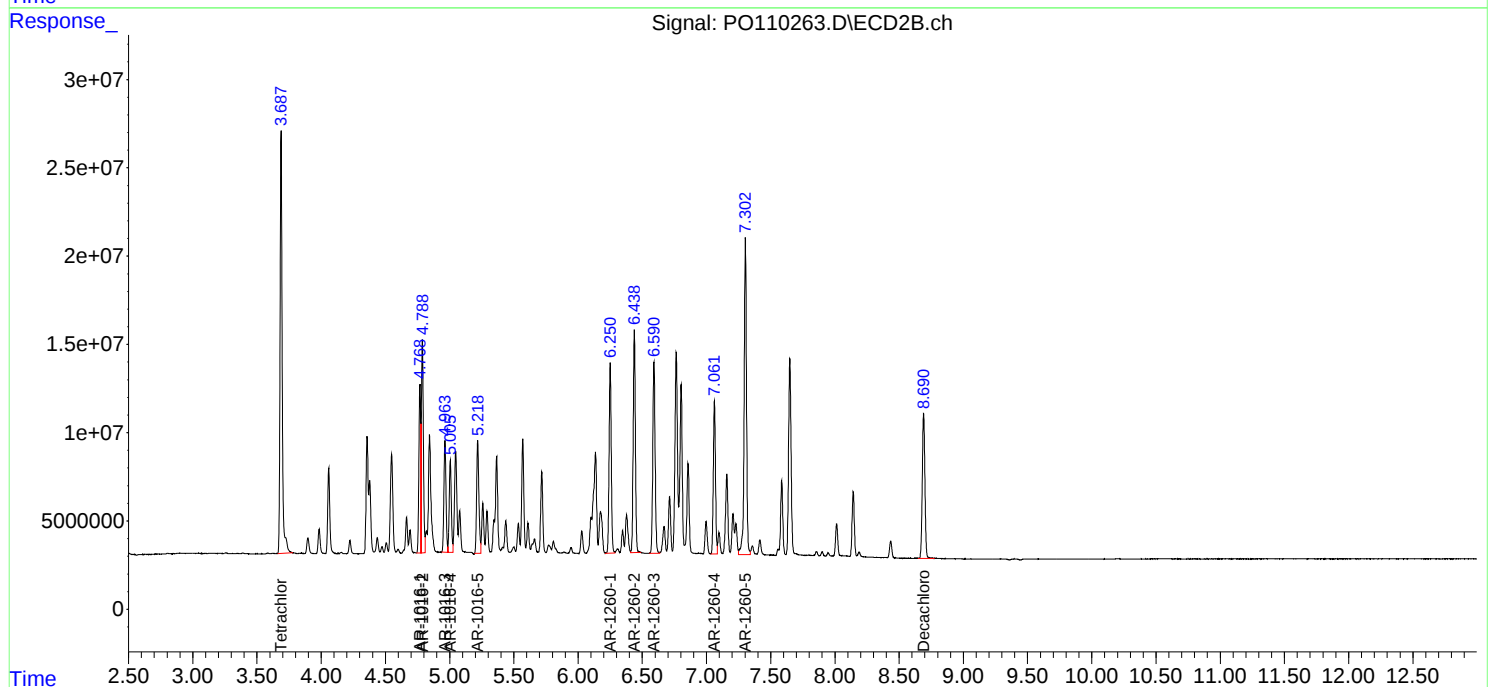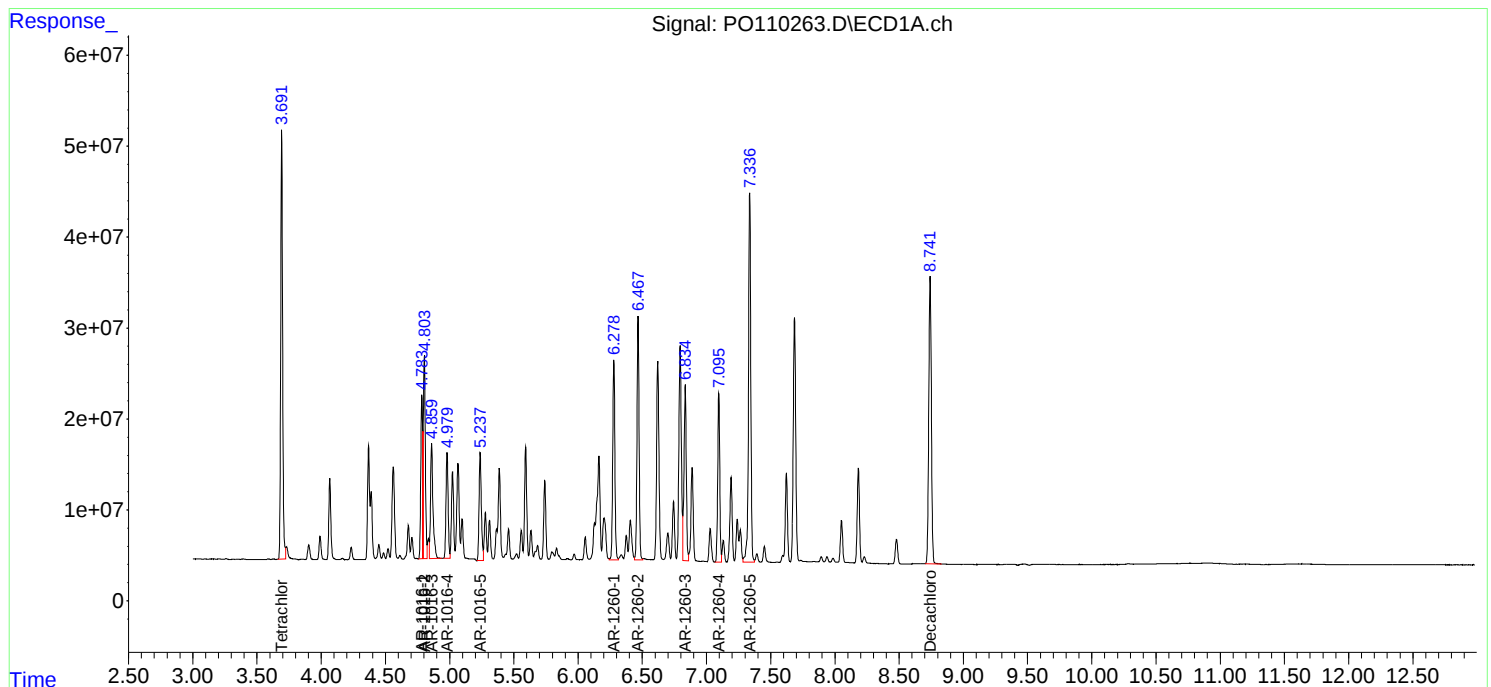



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 17:14 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-2	(2)	4.80	4.80	4.70	4.90	0.00
Aroclor-1016-3	(3)	4.86	4.86	4.76	4.96	0.00
Aroclor-1016-4	(4)	4.98	4.98	4.88	5.08	0.00
Aroclor-1016-5	(5)	5.24	5.24	5.14	5.34	0.00
Aroclor-1260-1	(1)	6.28	6.28	6.18	6.38	0.00
Aroclor-1260-2	(2)	6.47	6.47	6.37	6.57	0.00
Aroclor-1260-3	(3)	6.83	6.84	6.74	6.94	0.01
Aroclor-1260-4	(4)	7.09	7.10	7.00	7.20	0.01
Aroclor-1260-5	(5)	7.34	7.34	7.24	7.44	0.00
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.74	8.75	8.65	8.85	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 17:14 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2	(2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3	(3)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-4	(4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5	(5)	5.22	5.22	5.12	5.32	0.00
Aroclor-1260-1	(1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2	(2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3	(3)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-4	(4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5	(5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.69	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL02 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110278.D Time Analyzed: 17:14

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.782	4.685	4.885	511.900	500.000	2.4
Aroclor-1016-2	4.802	4.704	4.904	513.800	500.000	2.8
Aroclor-1016-3	4.858	4.761	4.961	513.560	500.000	2.7
Aroclor-1016-4	4.979	4.881	5.081	505.500	500.000	1.1
Aroclor-1016-5	5.236	5.139	5.339	483.610	500.000	-3.3
Aroclor-1260-1	6.276	6.180	6.380	516.970	500.000	3.4
Aroclor-1260-2	6.466	6.369	6.569	486.490	500.000	-2.7
Aroclor-1260-3	6.834	6.737	6.937	450.780	500.000	-9.8
Aroclor-1260-4	7.094	6.998	7.198	442.100	500.000	-11.6
Aroclor-1260-5	7.336	7.239	7.439	429.820	500.000	-14.0
Decachlorobiphenyl	8.741	8.645	8.845	52.440	50.000	4.9
Tetrachloro-m-xylene	3.691	3.592	3.792	52.070	50.000	4.1



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL02 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110278.D Time Analyzed: 17:14

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.769	4.672	4.872	501.230	500.000	0.2
Aroclor-1016-2	4.788	4.691	4.891	505.970	500.000	1.2
Aroclor-1016-3	4.964	4.867	5.067	506.650	500.000	1.3
Aroclor-1016-4	5.006	4.909	5.109	501.000	500.000	0.2
Aroclor-1016-5	5.218	5.122	5.322	500.710	500.000	0.1
Aroclor-1260-1	6.250	6.155	6.355	459.750	500.000	-8.1
Aroclor-1260-2	6.438	6.342	6.542	450.220	500.000	-10.0
Aroclor-1260-3	6.591	6.495	6.695	435.550	500.000	-12.9
Aroclor-1260-4	7.063	6.967	7.167	432.750	500.000	-13.5
Aroclor-1260-5	7.303	7.207	7.407	419.150	500.000	-16.2
Decachlorobiphenyl	8.691	8.596	8.796	46.440	50.000	-7.1
Tetrachloro-m-xylene	3.688	3.590	3.790	52.230	50.000	4.5

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 17:14
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 17:33:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.688	473.9E6	273.9E6	52.066	52.232
2) SA Decachlor...	8.741	8.691	403.2E6	112.7E6	52.443	46.444
Target Compounds						
3) L1 AR-1016-1	4.782	4.769	172.3E6	91853593	511.903	501.234
4) L1 AR-1016-2	4.802	4.788	238.2E6	132.3E6	513.796	505.969
5) L1 AR-1016-3	4.858	4.964	164.6E6	71832300	513.560	506.651
6) L1 AR-1016-4	4.979	5.006	127.7E6	59082308	505.504	500.996
7) L1 AR-1016-5	5.236	5.218	132.9E6	76567933	483.609	500.710
31) L7 AR-1260-1	6.276	6.250	243.7E6	117.4E6	516.972	459.747
32) L7 AR-1260-2	6.466	6.438	289.7E6	135.2E6	486.489	450.225
33) L7 AR-1260-3	6.834	6.591	218.8E6	125.9E6	450.781	435.554
34) L7 AR-1260-4	7.094	7.063	187.5E6	93074613	442.104	432.747
35) L7 AR-1260-5	7.336	7.303	449.5E6	209.0E6	429.819	419.151



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110278.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 17:14
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 17:33:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

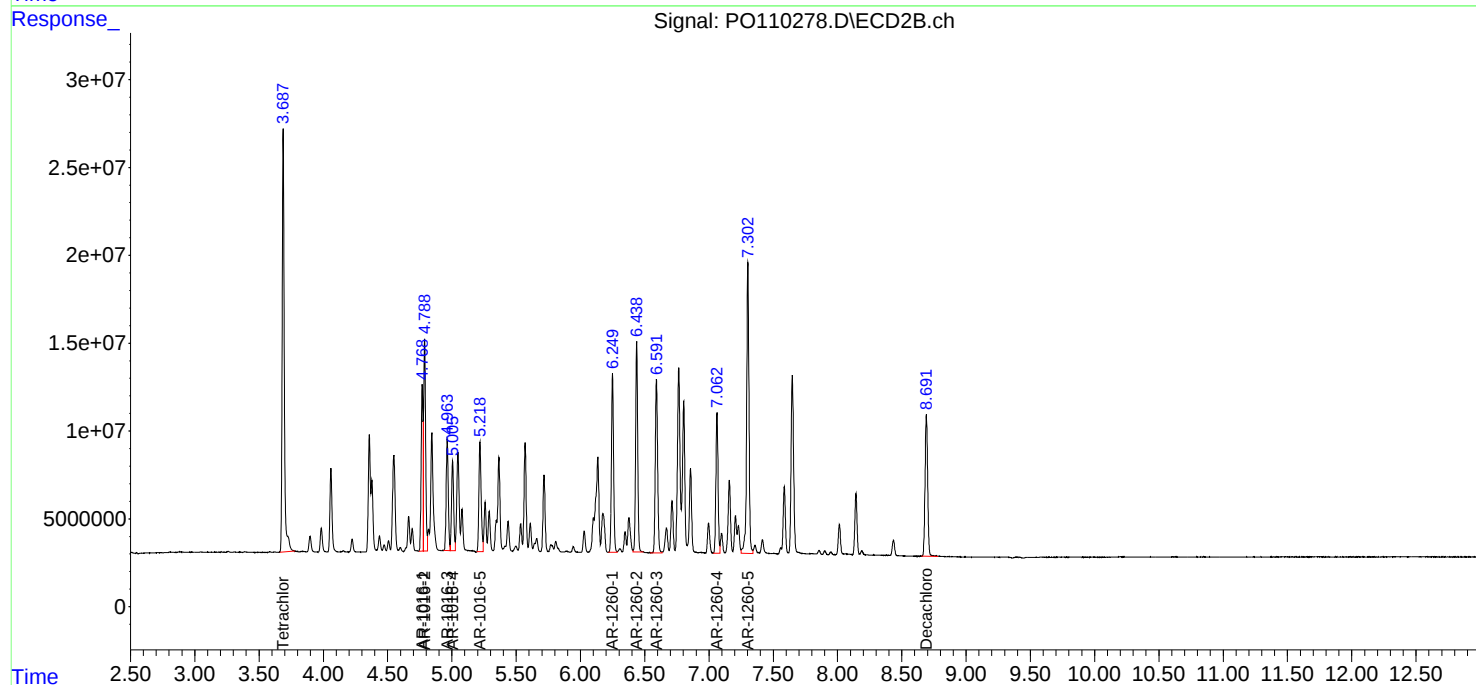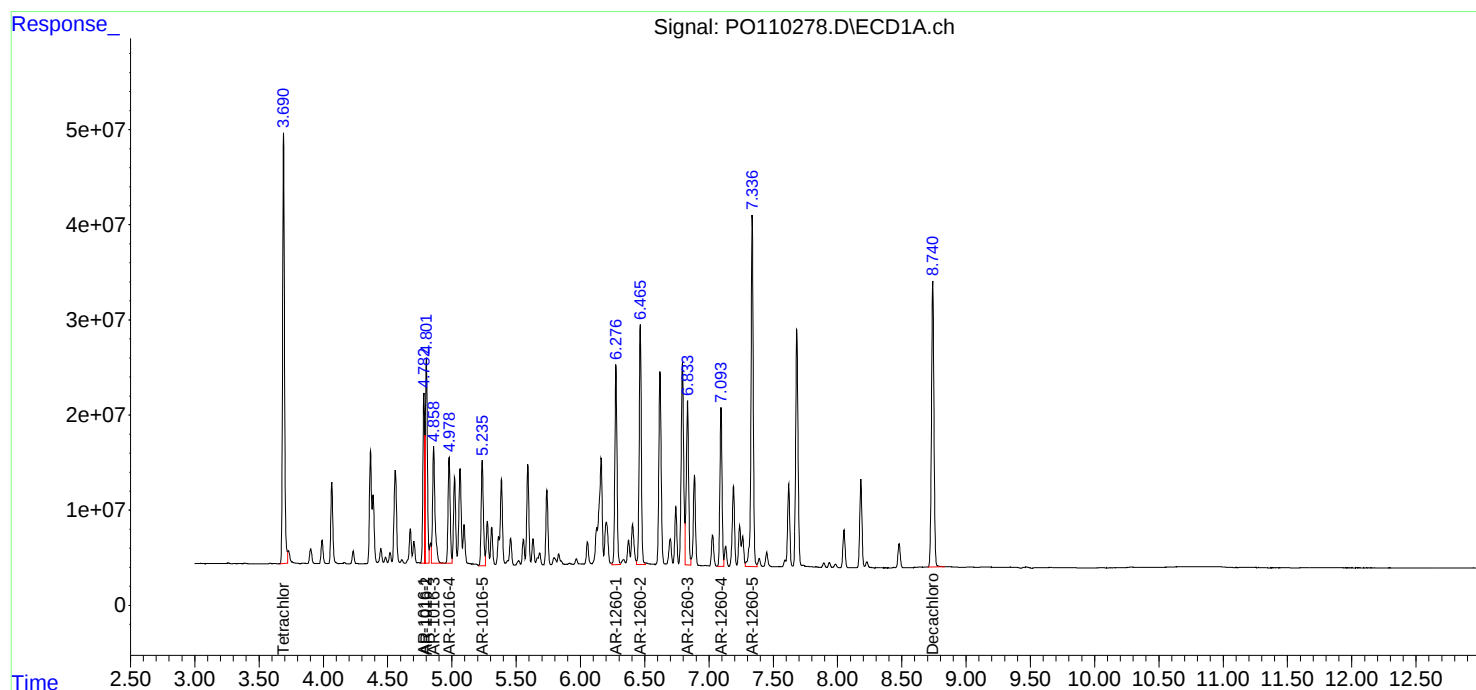



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 21:27 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-2	(2)	4.80	4.80	4.70	4.90	0.00
Aroclor-1016-3	(3)	4.86	4.86	4.76	4.96	0.00
Aroclor-1016-4	(4)	4.98	4.98	4.88	5.08	0.00
Aroclor-1016-5	(5)	5.24	5.24	5.14	5.34	0.00
Aroclor-1260-1	(1)	6.28	6.28	6.18	6.38	0.00
Aroclor-1260-2	(2)	6.47	6.47	6.37	6.57	0.00
Aroclor-1260-3	(3)	6.83	6.84	6.74	6.94	0.01
Aroclor-1260-4	(4)	7.09	7.10	7.00	7.20	0.01
Aroclor-1260-5	(5)	7.34	7.34	7.24	7.44	0.00
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.74	8.75	8.65	8.85	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Continuing Calib Date: 04/07/2025 Initial Calibration Date(s): 03/18/2025 03/18/2025

Continuing Calib Time: 21:27 Initial Calibration Time(s): 14:03 22:15

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2	(2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3	(3)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-4	(4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5	(5)	5.22	5.22	5.12	5.32	0.00
Aroclor-1260-1	(1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2	(2)	6.44	6.44	6.34	6.54	0.00
Aroclor-1260-3	(3)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-4	(4)	7.06	7.07	6.97	7.17	0.01
Aroclor-1260-5	(5)	7.30	7.31	7.21	7.41	0.01
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.69	8.70	8.60	8.80	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL03 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110286.D Time Analyzed: 21:27

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.783	4.685	4.885	528.320	500.000	5.7
Aroclor-1016-2	4.802	4.704	4.904	526.450	500.000	5.3
Aroclor-1016-3	4.858	4.761	4.961	529.370	500.000	5.9
Aroclor-1016-4	4.979	4.881	5.081	518.990	500.000	3.8
Aroclor-1016-5	5.236	5.139	5.339	496.090	500.000	-0.8
Aroclor-1260-1	6.277	6.180	6.380	550.160	500.000	10.0
Aroclor-1260-2	6.466	6.369	6.569	508.400	500.000	1.7
Aroclor-1260-3	6.834	6.737	6.937	481.740	500.000	-3.7
Aroclor-1260-4	7.094	6.998	7.198	471.490	500.000	-5.7
Aroclor-1260-5	7.336	7.239	7.439	462.920	500.000	-7.4
Decachlorobiphenyl	8.740	8.645	8.845	54.690	50.000	9.4
Tetrachloro-m-xylene	3.691	3.592	3.792	53.480	50.000	7.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/18/2025 03/18/2025

Client Sample No.: CCAL03 Date Analyzed: 04/07/2025

Lab Sample No.: AR1660CCC500 Data File : PO110286.D Time Analyzed: 21:27

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.769	4.672	4.872	512.420	500.000	2.5
Aroclor-1016-2	4.788	4.691	4.891	514.070	500.000	2.8
Aroclor-1016-3	4.964	4.867	5.067	515.160	500.000	3.0
Aroclor-1016-4	5.006	4.909	5.109	469.250	500.000	-6.2
Aroclor-1016-5	5.218	5.122	5.322	514.370	500.000	2.9
Aroclor-1260-1	6.251	6.155	6.355	483.370	500.000	-3.3
Aroclor-1260-2	6.439	6.342	6.542	477.180	500.000	-4.6
Aroclor-1260-3	6.591	6.495	6.695	462.160	500.000	-7.6
Aroclor-1260-4	7.063	6.967	7.167	461.970	500.000	-7.6
Aroclor-1260-5	7.303	7.207	7.407	444.510	500.000	-11.1
Decachlorobiphenyl	8.691	8.596	8.796	48.770	50.000	-2.5
Tetrachloro-m-xylene	3.688	3.590	3.790	53.150	50.000	6.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 21:27
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/08/2025
 Supervised By :mohammad ahmed 04/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:36:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.688	486.8E6	278.7E6	53.484	53.152
2) SA Decachlor...	8.740	8.691	420.5E6	118.3E6	54.690	48.766
Target Compounds						
3) L1 AR-1016-1	4.783	4.769	177.8E6	93902896	528.316	512.417
4) L1 AR-1016-2	4.802	4.788	244.1E6	134.4E6	526.454	514.067
5) L1 AR-1016-3	4.858	4.964	169.7E6	73038464	529.369	515.158
6) L1 AR-1016-4	4.979	5.006	131.1E6	55338718	518.987	469.252
7) L1 AR-1016-5	5.236	5.218	136.4E6	78657229	496.086m	514.373m
31) L7 AR-1260-1	6.277	6.251	259.3E6	123.5E6	550.162	483.373
32) L7 AR-1260-2	6.466	6.439	302.8E6	143.3E6	508.402	477.179
33) L7 AR-1260-3	6.834	6.591	233.8E6	133.6E6	481.744	462.164
34) L7 AR-1260-4	7.094	7.063	200.0E6	99360275	471.486	461.972
35) L7 AR-1260-5	7.336	7.303	484.1E6	221.7E6	462.918	444.506

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 21:27
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2025
Supervised By :mohammad ahmed 04/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:36:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

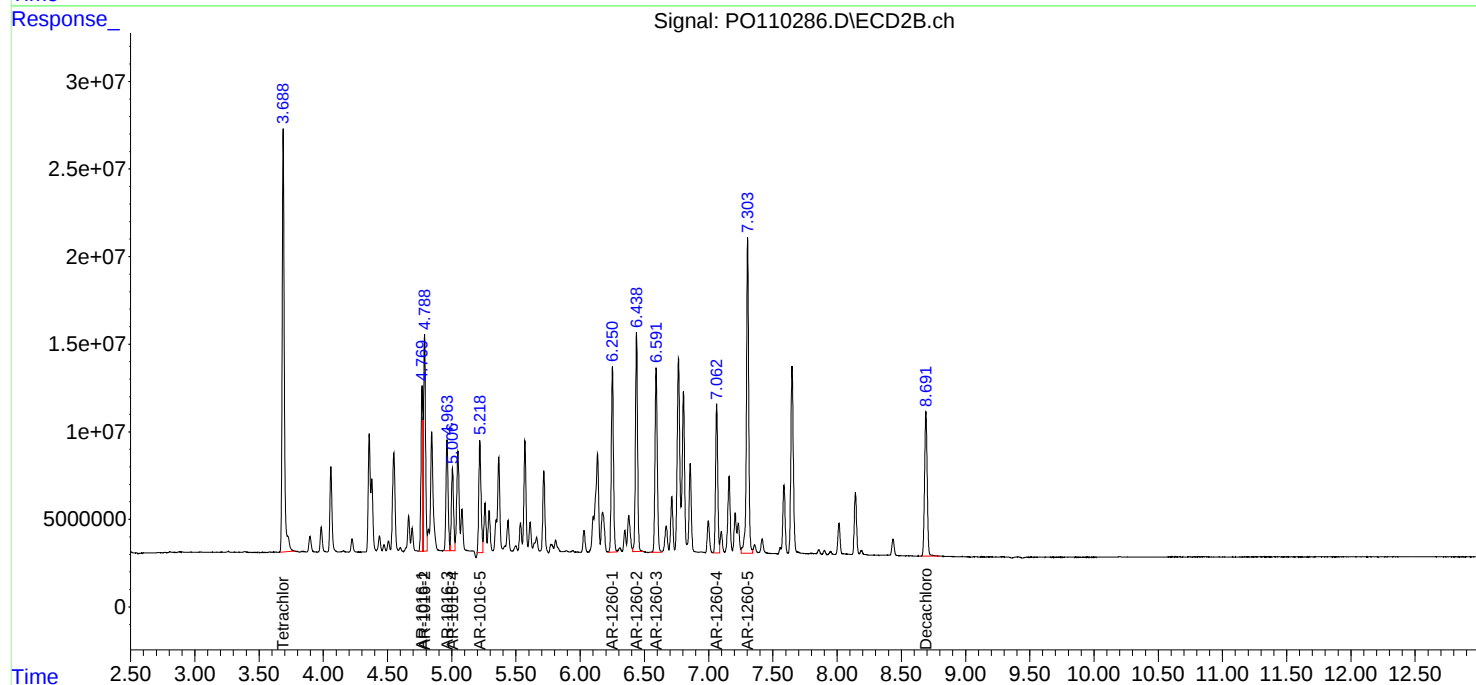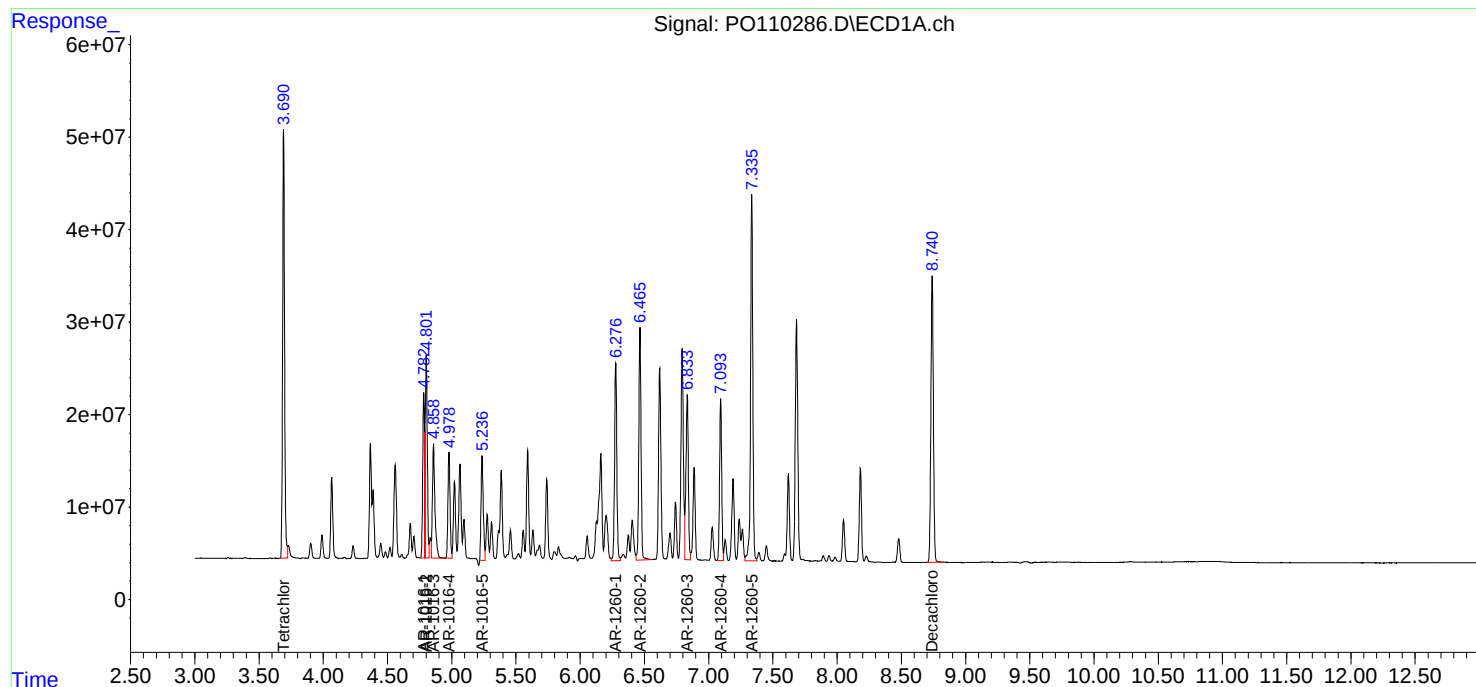

Analytical Sequence

Client: G Environmental

SDG No.: Q1736

Project: Stockton

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 03/18/2025 03/18/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	03/18/2025	13:44	PO109971.D	8.74	3.69
AR1660ICC1000	AR1660ICC1000	03/18/2025	14:03	PO109972.D	8.75	3.69
AR1660ICC750	AR1660ICC750	03/18/2025	14:21	PO109973.D	8.75	3.69
AR1660ICC500	AR1660ICC500	03/18/2025	14:39	PO109974.D	8.75	3.69
AR1660ICC250	AR1660ICC250	03/18/2025	14:58	PO109975.D	8.75	3.69
AR1660ICC050	AR1660ICC050	03/18/2025	15:16	PO109976.D	8.74	3.69
AR1221ICC500	AR1221ICC500	03/18/2025	15:34	PO109977.D	8.74	3.69
AR1232ICC500	AR1232ICC500	03/18/2025	15:53	PO109978.D	8.74	3.69
AR1242ICC1000	AR1242ICC1000	03/18/2025	16:11	PO109979.D	8.74	3.69
AR1242ICC750	AR1242ICC750	03/18/2025	16:30	PO109980.D	8.74	3.69
AR1242ICC500	AR1242ICC500	03/18/2025	16:48	PO109981.D	8.74	3.69
AR1242ICC250	AR1242ICC250	03/18/2025	17:06	PO109982.D	8.74	3.69
AR1242ICC050	AR1242ICC050	03/18/2025	17:25	PO109983.D	8.74	3.69
AR1248ICC1000	AR1248ICC1000	03/18/2025	17:42	PO109984.D	8.74	3.69
AR1248ICC750	AR1248ICC750	03/18/2025	18:00	PO109985.D	8.74	3.69
AR1248ICC500	AR1248ICC500	03/18/2025	18:19	PO109986.D	8.74	3.69
AR1248ICC250	AR1248ICC250	03/18/2025	18:37	PO109987.D	8.74	3.69
AR1248ICC050	AR1248ICC050	03/18/2025	18:54	PO109988.D	8.74	3.69
AR1254ICC1000	AR1254ICC1000	03/18/2025	19:13	PO109989.D	8.74	3.69
AR1254ICC750	AR1254ICC750	03/18/2025	19:31	PO109990.D	8.74	3.69
AR1254ICC500	AR1254ICC500	03/18/2025	19:49	PO109991.D	8.74	3.69
AR1254ICC250	AR1254ICC250	03/18/2025	20:07	PO109992.D	8.74	3.69
AR1254ICC050	AR1254ICC050	03/18/2025	20:25	PO109993.D	8.74	3.69
AR1262ICC500	AR1262ICC500	03/18/2025	20:43	PO109994.D	8.74	3.69
AR1268ICC1000	AR1268ICC1000	03/18/2025	21:02	PO109995.D	8.74	3.69
AR1268ICC750	AR1268ICC750	03/18/2025	21:20	PO109996.D	8.74	3.69
AR1268ICC500	AR1268ICC500	03/18/2025	21:39	PO109997.D	8.74	3.69
AR1268ICC250	AR1268ICC250	03/18/2025	21:57	PO109998.D	8.74	3.69
AR1268ICC050	AR1268ICC050	03/18/2025	22:15	PO109999.D	8.74	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	09:46	PO110263.D	8.74	3.69
IBLK	IBLK	04/07/2025	11:36	PO110267.D	8.74	3.69
OU4-VSL-16-040325MS	Q1730-03MS	04/07/2025	14:15	PO110271.D	8.74	3.69
OU4-VSL-16-040325MSD	Q1730-03MSD	04/07/2025	14:33	PO110272.D	8.74	3.69
GST1	Q1736-01	04/07/2025	14:51	PO110273.D	8.74	3.69
GST2	Q1736-02	04/07/2025	15:10	PO110274.D	8.74	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	17:14	PO110278.D	8.74	3.69
IBLK	IBLK	04/07/2025	19:04	PO110282.D	8.74	3.69
PB167469BL	PB167469BL	04/07/2025	19:22	PO110283.D	8.74	3.69
PB167469BS	PB167469BS	04/07/2025	19:41	PO110284.D	8.74	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	21:27	PO110286.D	8.74	3.69
IBLK	IBLK	04/07/2025	23:17	PO110290.D	8.74	3.69

Analytical Sequence

Analytical Sequence

Client: G Environmental

SDG No.: Q1736

Project: Stockton

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 03/18/2025 03/18/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	03/18/2025	13:44	PO109971.D	8.70	3.69
AR1660ICC1000	AR1660ICC1000	03/18/2025	14:03	PO109972.D	8.70	3.69
AR1660ICC750	AR1660ICC750	03/18/2025	14:21	PO109973.D	8.70	3.69
AR1660ICC500	AR1660ICC500	03/18/2025	14:39	PO109974.D	8.70	3.69
AR1660ICC250	AR1660ICC250	03/18/2025	14:58	PO109975.D	8.70	3.69
AR1660ICC050	AR1660ICC050	03/18/2025	15:16	PO109976.D	8.70	3.69
AR1221ICC500	AR1221ICC500	03/18/2025	15:34	PO109977.D	8.70	3.69
AR1232ICC500	AR1232ICC500	03/18/2025	15:53	PO109978.D	8.70	3.69
AR1242ICC1000	AR1242ICC1000	03/18/2025	16:11	PO109979.D	8.70	3.69
AR1242ICC750	AR1242ICC750	03/18/2025	16:30	PO109980.D	8.70	3.69
AR1242ICC500	AR1242ICC500	03/18/2025	16:48	PO109981.D	8.70	3.69
AR1242ICC250	AR1242ICC250	03/18/2025	17:06	PO109982.D	8.70	3.69
AR1242ICC050	AR1242ICC050	03/18/2025	17:25	PO109983.D	8.70	3.69
AR1248ICC1000	AR1248ICC1000	03/18/2025	17:42	PO109984.D	8.70	3.69
AR1248ICC750	AR1248ICC750	03/18/2025	18:00	PO109985.D	8.70	3.69
AR1248ICC500	AR1248ICC500	03/18/2025	18:19	PO109986.D	8.70	3.69
AR1248ICC250	AR1248ICC250	03/18/2025	18:37	PO109987.D	8.70	3.69
AR1248ICC050	AR1248ICC050	03/18/2025	18:54	PO109988.D	8.70	3.69
AR1254ICC1000	AR1254ICC1000	03/18/2025	19:13	PO109989.D	8.69	3.69
AR1254ICC750	AR1254ICC750	03/18/2025	19:31	PO109990.D	8.70	3.69
AR1254ICC500	AR1254ICC500	03/18/2025	19:49	PO109991.D	8.70	3.69
AR1254ICC250	AR1254ICC250	03/18/2025	20:07	PO109992.D	8.70	3.69
AR1254ICC050	AR1254ICC050	03/18/2025	20:25	PO109993.D	8.69	3.69
AR1262ICC500	AR1262ICC500	03/18/2025	20:43	PO109994.D	8.70	3.69
AR1268ICC1000	AR1268ICC1000	03/18/2025	21:02	PO109995.D	8.70	3.69
AR1268ICC750	AR1268ICC750	03/18/2025	21:20	PO109996.D	8.70	3.69
AR1268ICC500	AR1268ICC500	03/18/2025	21:39	PO109997.D	8.69	3.69
AR1268ICC250	AR1268ICC250	03/18/2025	21:57	PO109998.D	8.70	3.69
AR1268ICC050	AR1268ICC050	03/18/2025	22:15	PO109999.D	8.70	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	09:46	PO110263.D	8.69	3.69
IBLK	IBLK	04/07/2025	11:36	PO110267.D	8.69	3.69
OU4-VSL-16-040325MS	Q1730-03MS	04/07/2025	14:15	PO110271.D	8.69	3.69
OU4-VSL-16-040325MSD	Q1730-03MSD	04/07/2025	14:33	PO110272.D	8.69	3.69
GST1	Q1736-01	04/07/2025	14:51	PO110273.D	8.69	3.69
GST2	Q1736-02	04/07/2025	15:10	PO110274.D	8.69	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	17:14	PO110278.D	8.69	3.69
IBLK	IBLK	04/07/2025	19:04	PO110282.D	8.69	3.69
PB167469BL	PB167469BL	04/07/2025	19:22	PO110283.D	8.69	3.69
PB167469BS	PB167469BS	04/07/2025	19:41	PO110284.D	8.69	3.69
AR1660CCC500	AR1660CCC500	04/07/2025	21:27	PO110286.D	8.69	3.69
IBLK	IBLK	04/07/2025	23:17	PO110290.D	8.69	3.69

Analytical Sequence

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

OU4-VSL-16-040325MS

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Lab Sample ID: Q1730-03MS Date(s) Analyzed: 04/07/2025 04/07/2025

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO110271.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.782	4.732	4.832	171	170	3.59
COLUMN 1	2	4.802	4.752	4.852	172		
	3	4.858	4.808	4.908	172		
	4	4.978	4.928	5.028	171		
	5	5.236	5.186	5.286	163		
	1	4.768	4.718	4.818	166		
COLUMN 2	2	4.787	4.737	4.837	166	164	
	3	4.963	4.913	5.013	166		
	4	5.005	4.955	5.055	163		
	5	5.218	5.168	5.268	159		
Aroclor-1260	1	6.276	6.226	6.326	178	157	3.9
COLUMN 1	2	6.466	6.416	6.516	169		
	3	6.833	6.783	6.883	144		
	4	7.094	7.044	7.144	152		
	5	7.335	7.285	7.385	141		
	1	6.25	6.2	6.3	164		
COLUMN 2	2	6.438	6.388	6.488	160	151	
	3	6.591	6.541	6.641	155		
	4	7.062	7.012	7.112	142		
	5	7.303	7.253	7.353	133		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

OU4-VSL-16-040325MSI

Contract: GENV01

Lab Code: CHEM Case No.: Q1736 SAS No.: Q1736 SDG NO.: Q1736

Lab Sample ID: Q1730-03MSD Date(s) Analyzed: 04/07/2025 04/07/2025

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO110272.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.782	4.732	4.832	163	164	3.73
COLUMN 1	2	4.801	4.751	4.851	167		
	3	4.857	4.807	4.907	167		
	4	4.978	4.928	5.028	166		
	5	5.235	5.185	5.285	159		
	1	4.768	4.718	4.818	159		
COLUMN 2	2	4.788	4.738	4.838	160	158	
	3	4.963	4.913	5.013	160		
	4	5.005	4.955	5.055	157		
	5	5.217	5.167	5.267	154		
Aroclor-1260	1	6.276	6.226	6.326	169	153	4.68
COLUMN 1	2	6.466	6.416	6.516	163		
	3	6.833	6.783	6.883	143		
	4	7.093	7.043	7.143	150		
	5	7.335	7.285	7.385	138		
	1	6.25	6.2	6.3	159		
COLUMN 2	2	6.438	6.388	6.488	156	146	
	3	6.59	6.54	6.64	150		
	4	7.061	7.011	7.111	138		
	5	7.302	7.252	7.352	129		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB167469BS

Contract: GENV01

Lab Code: CHEM

Case No.: Q1736

SAS No.: Q1736

SDG NO.: Q1736

Lab Sample ID: PB167469BS

Date(s) Analyzed: 04/07/2025

04/07/2025

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO110284.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.782	4.732	4.832	141	141	5.09
COLUMN 1	2	4.802	4.752	4.852	143		
	3	4.858	4.808	4.908	142		
	4	4.978	4.928	5.028	142		
	5	5.236	5.186	5.286	138		
	1	4.769	4.719	4.819	136		
COLUMN 2	2	4.788	4.738	4.838	134	134	
	3	4.964	4.914	5.014	136		
	4	5.005	4.955	5.055	135		
	5	5.218	5.168	5.268	131		
Aroclor-1260	1	6.277	6.227	6.327	149	134	4.58
COLUMN 1	2	6.465	6.415	6.515	141		
	3	6.833	6.783	6.883	119		
	4	7.093	7.043	7.143	131		
	5	7.336	7.286	7.386	129		
	1	6.25	6.2	6.3	140	128	
COLUMN 2	2	6.438	6.388	6.488	138		
	3	6.59	6.54	6.64	133		
	4	7.062	7.012	7.112	119		
	5	7.303	7.253	7.353	113		



QC SAMPLE DATA

Report of Analysis

Client:	G Environmental	Date Collected:	
Project:	Stockton	Date Received:	
Client Sample ID:	PB167469BL	SDG No.:	Q1736
Lab Sample ID:	PB167469BL	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	100 Decanted:
Sample Wt/Vol:	30.01 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110283.D	1	04/07/25 08:20	04/07/25 19:22	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	3.90	U	3.90	17.0	ug/kg
11104-28-2	Aroclor-1221	4.00	U	4.00	17.0	ug/kg
11141-16-5	Aroclor-1232	3.70	U	3.70	17.0	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	17.0	ug/kg
12672-29-6	Aroclor-1248	5.90	U	5.90	17.0	ug/kg
11097-69-1	Aroclor-1254	3.20	U	3.20	17.0	ug/kg
37324-23-5	Aroclor-1262	5.00	U	5.00	17.0	ug/kg
11100-14-4	Aroclor-1268	3.60	U	3.60	17.0	ug/kg
11096-82-5	Aroclor-1260	3.20	U	3.20	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.0		30 (32) - 150 (144)	95%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.3		30 (32) - 150 (175)	86%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 19:22
 Operator : YP/AJ
 Sample : PB167469BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB167469BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:35:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.688	173.1E6	95749355	19.020	18.259
2) SA Decachlor...	8.741	8.691	133.0E6	38862706	17.297	16.019

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 19:22
Operator : YP/AJ
Sample : PB167469BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB167469BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:35:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

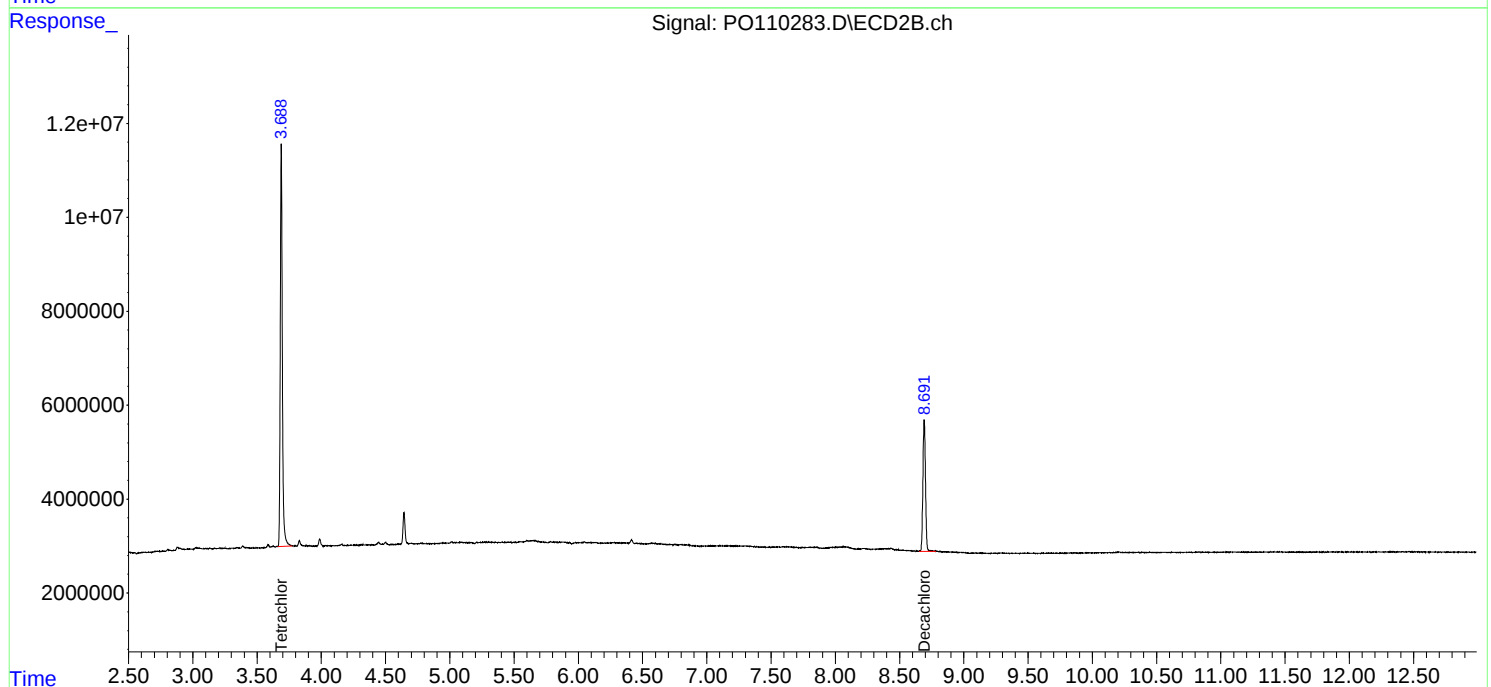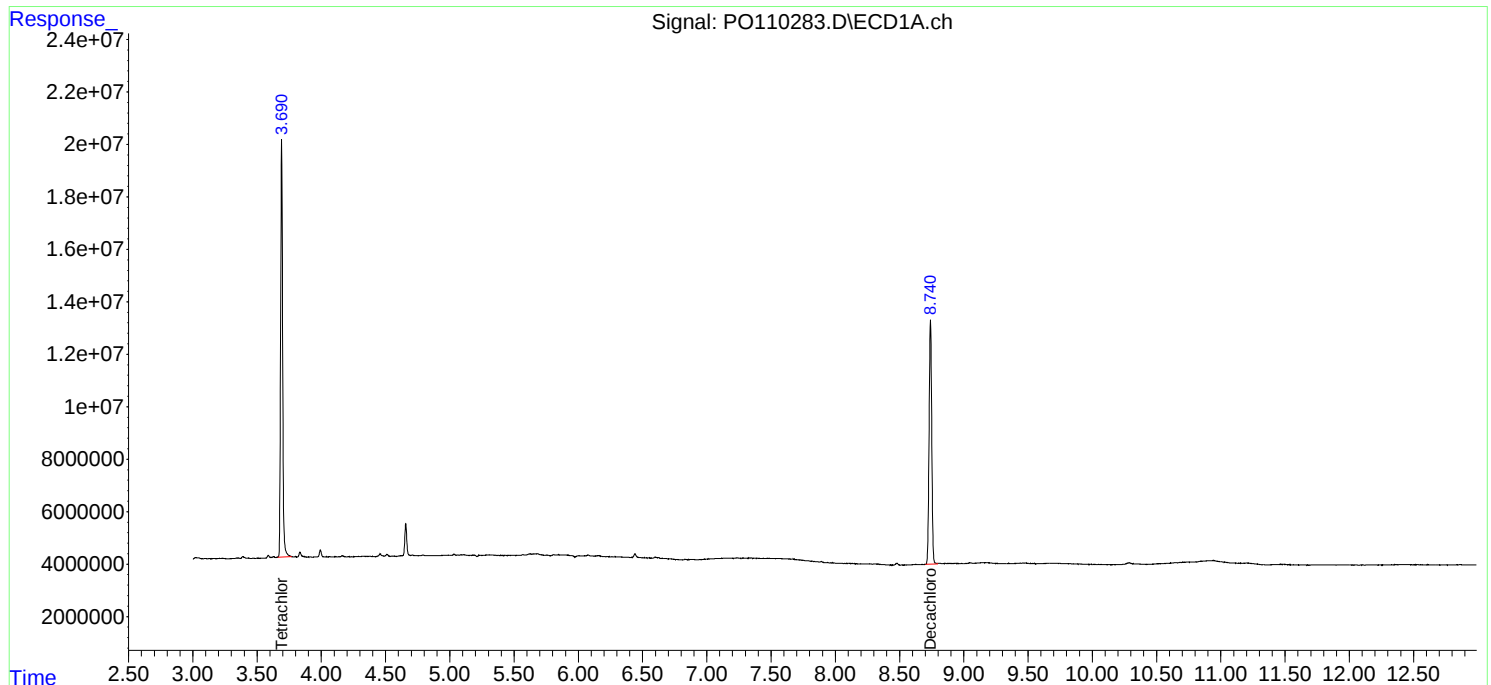


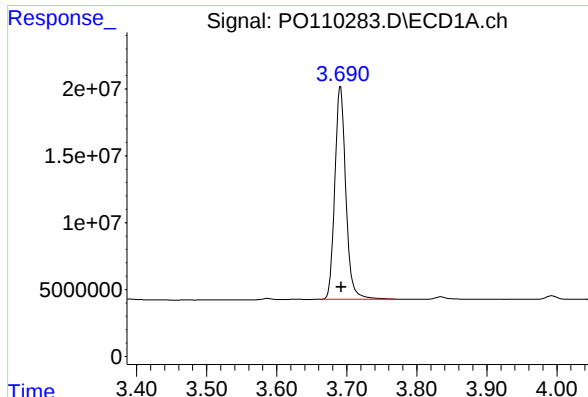

#1 Tetrachloro-m-xylene


R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 173109300
Conc: 19.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB167469BL

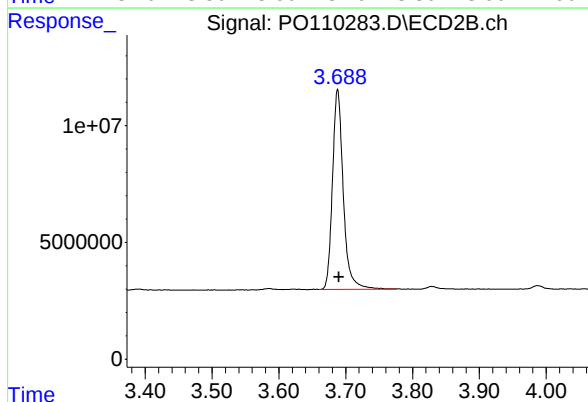


#1 Tetrachloro-m-xylene

R.T.: 3.688 min
Delta R.T.: -0.002 min
Response: 95749355
Conc: 18.26 ng/ml

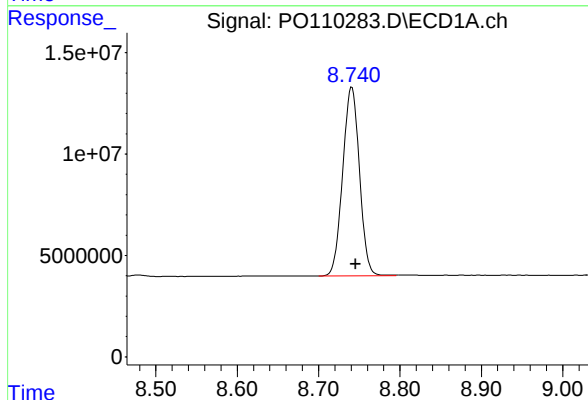

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.005 min
Response: 132989663
Conc: 17.30 ng/ml

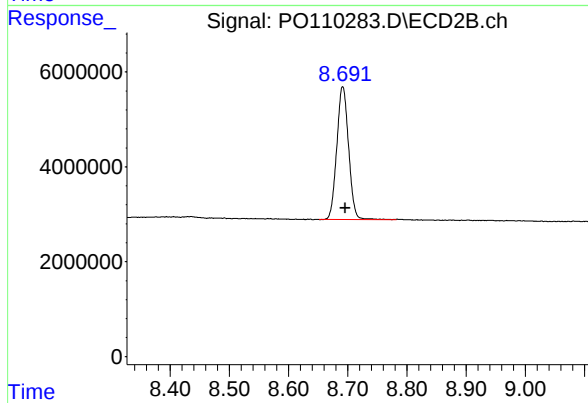

#2 Decachlorobiphenyl

R.T.: 8.691 min
Delta R.T.: -0.004 min
Response: 38862706
Conc: 16.02 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	03/18/25
Project:	Stockton	Date Received:	03/18/25
Client Sample ID:	PIBLK-PO109971.D	SDG No.:	Q1736
Lab Sample ID:	I.BLK-PO109971.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109971.D	1		03/18/25	PO031925

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.5		70 (60) - 130 (140)	93%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.0		70 (60) - 130 (140)	100%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031925\
 Data File : PO109971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2025 13:44
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 03:44:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.689	168.3E6	97603621	18.495	18.612
2) SA Decachlor...	8.744	8.695	153.9E6	51783076	20.014	21.344

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO031925\
Data File : PO109971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2025 13:44
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 03:44:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

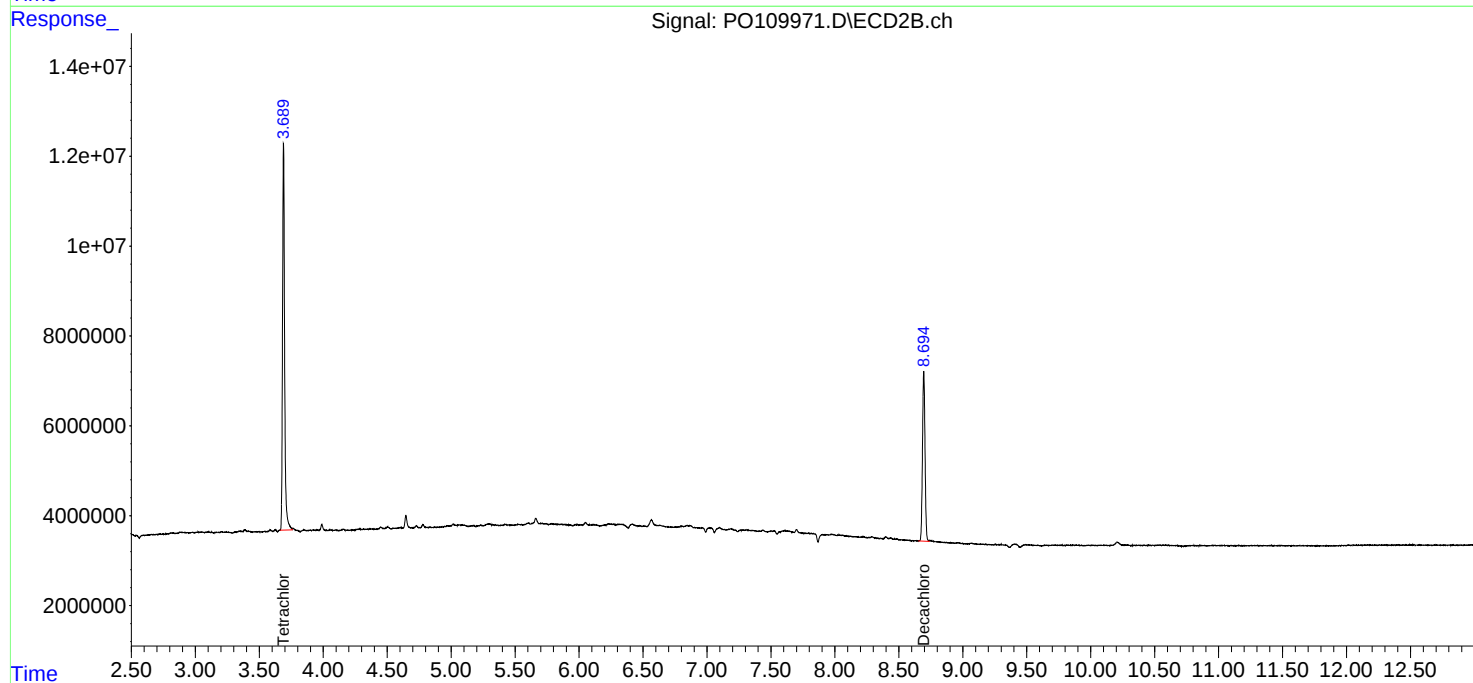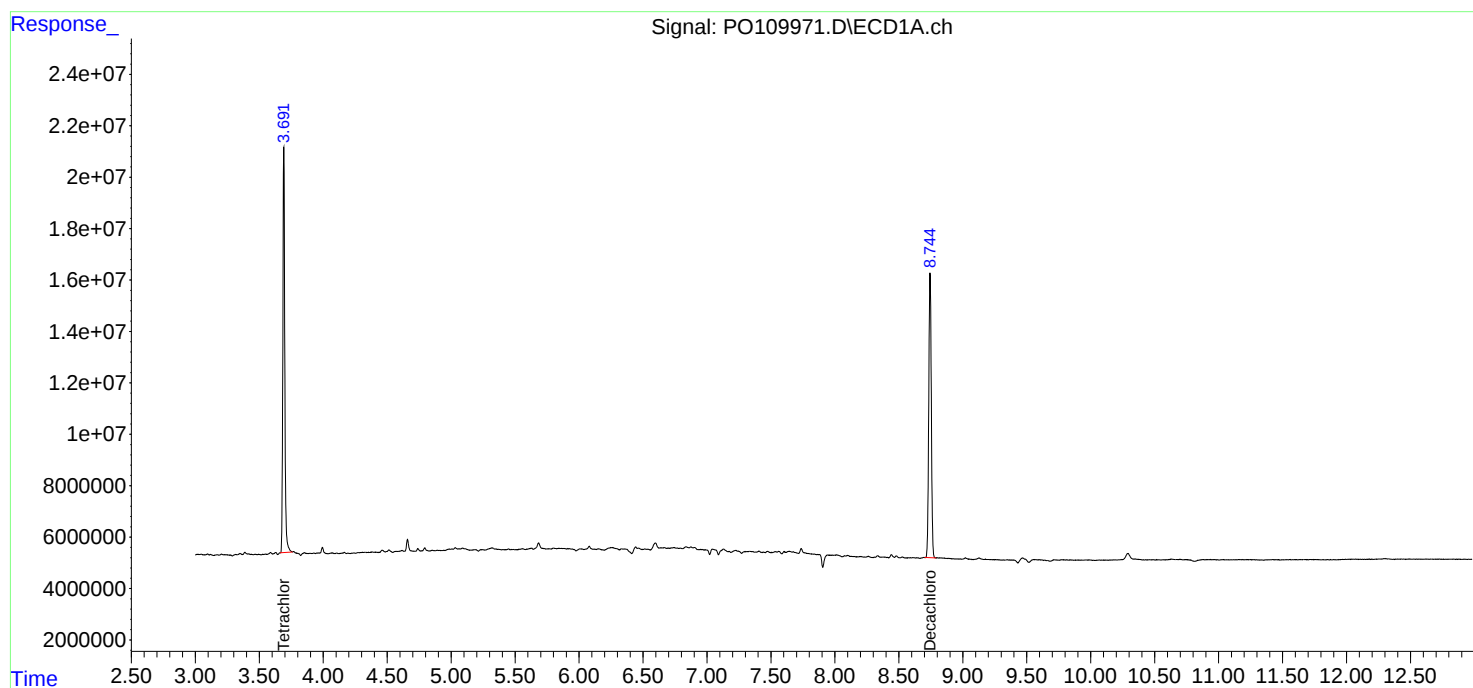


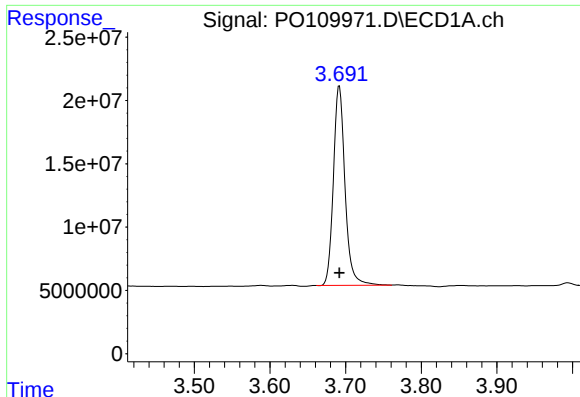

#1 Tetrachloro-m-xylene


R.T.: 3.692 min
Delta R.T.: 0.000 min
Response: 168336707
Conc: 18.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

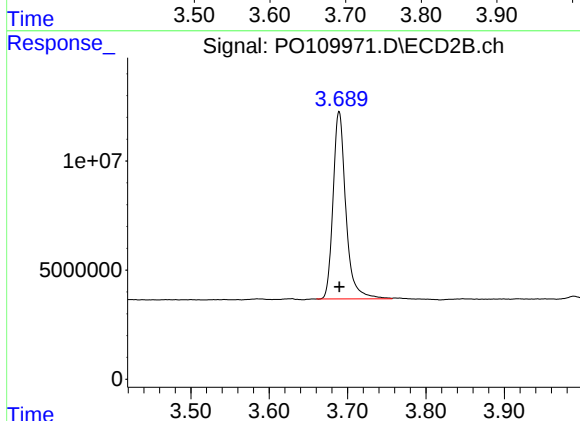


#1 Tetrachloro-m-xylene

R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 97603621
Conc: 18.61 ng/ml

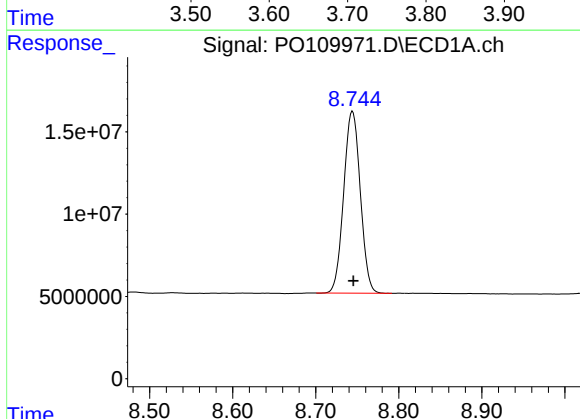

#2 Decachlorobiphenyl

R.T.: 8.744 min
Delta R.T.: -0.001 min
Response: 153882781
Conc: 20.01 ng/ml

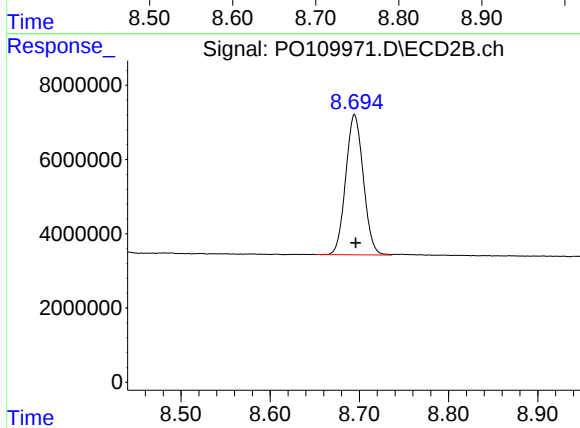

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: -0.001 min
Response: 51783076
Conc: 21.34 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	04/07/25
Project:	Stockton	Date Received:	04/07/25
Client Sample ID:	PIBLK-PO110267.D	SDG No.:	Q1736
Lab Sample ID:	I.BLK-PO110267.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110267.D	1		04/07/25	PO040725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.8		70 (60) - 130 (140)	94%	SPK: 20
2051-24-3	Decachlorobiphenyl	15.9		70 (60) - 130 (140)	79%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 11:36
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 12:31:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.689	3.687	177.4E6	98699299	19.494	18.821
2) SA Decachlor...	8.737	8.690	141.7E6	38504154	18.426	15.871

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 11:36
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 12:31:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

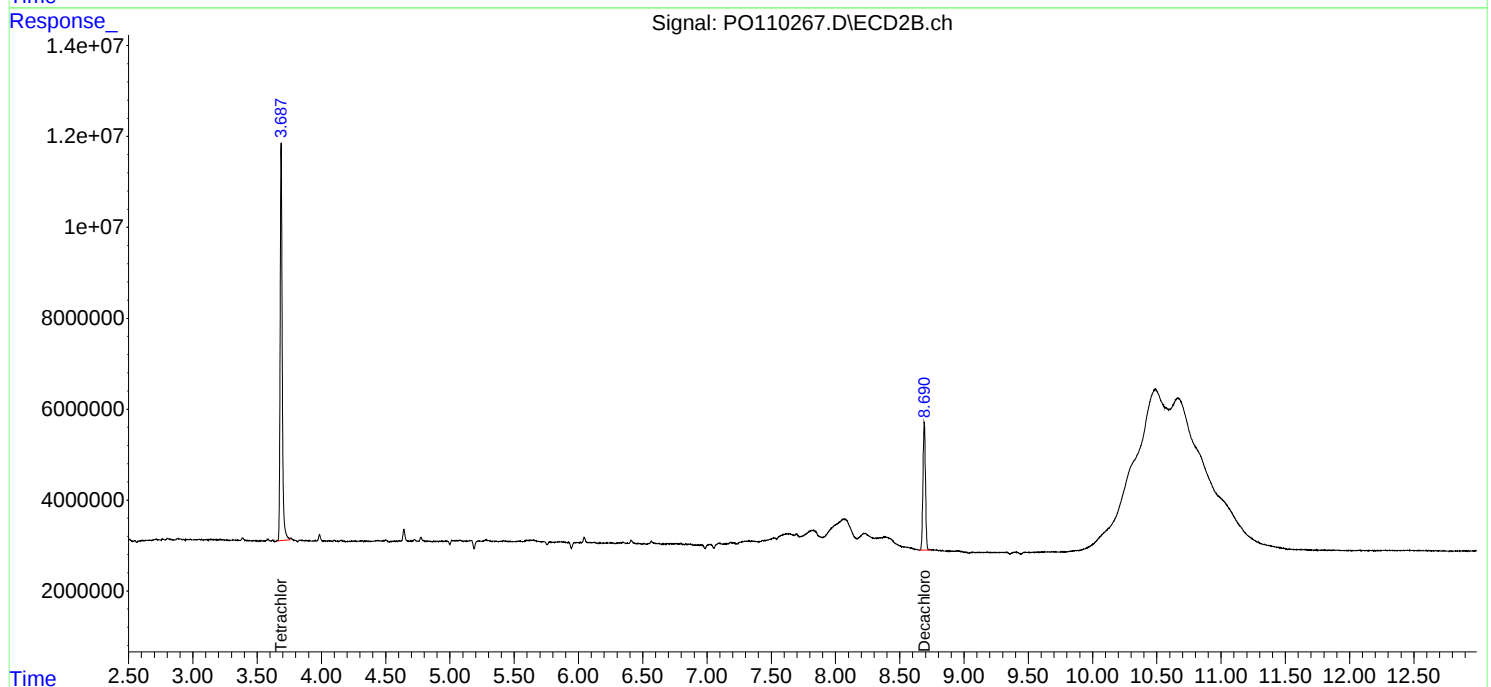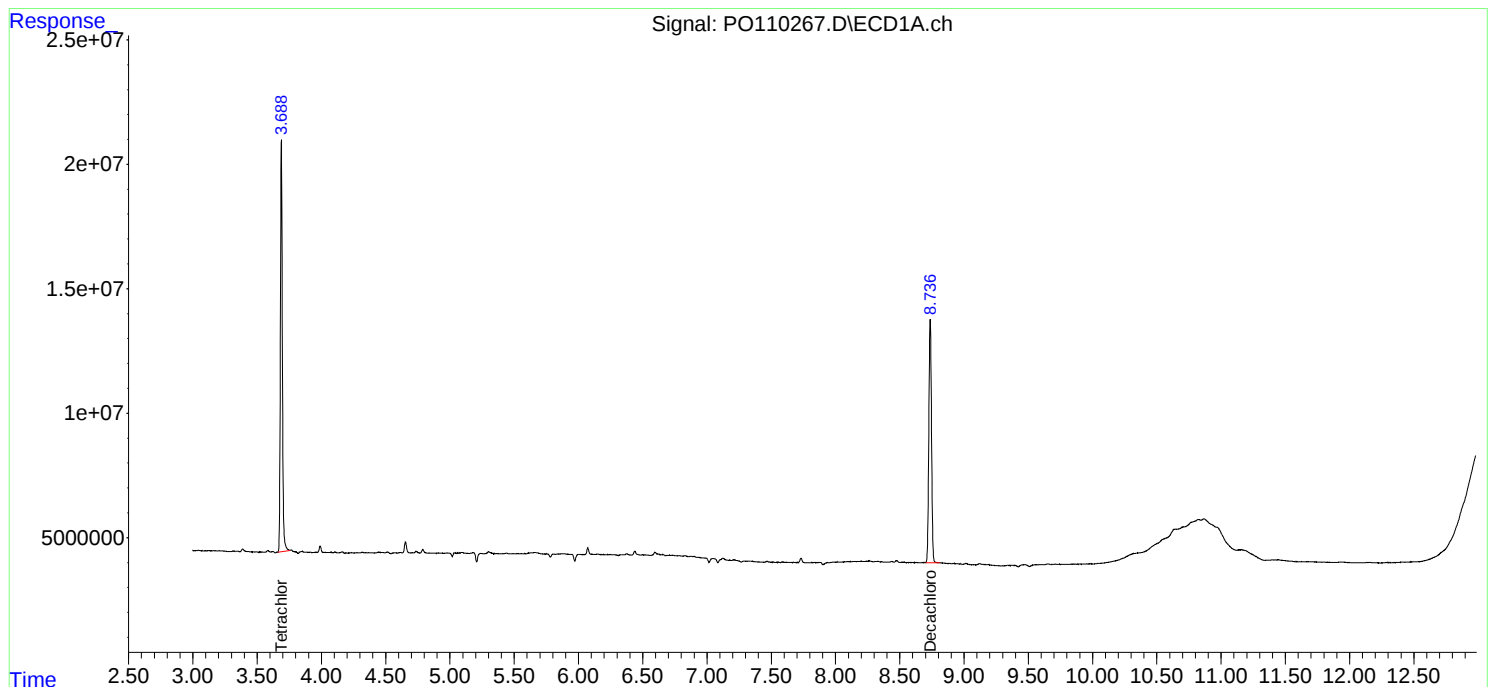


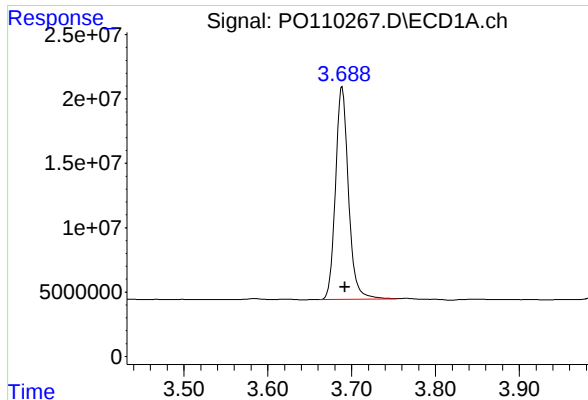

#1 Tetrachloro-m-xylene


R.T.: 3.689 min
Delta R.T.: -0.003 min
Response: 177426113
Conc: 19.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

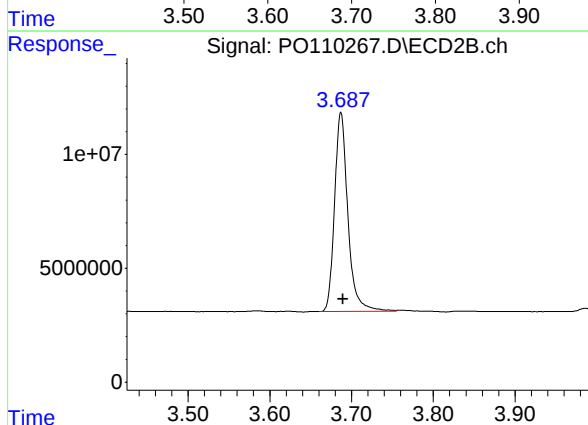


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: -0.003 min
Response: 98699299
Conc: 18.82 ng/ml

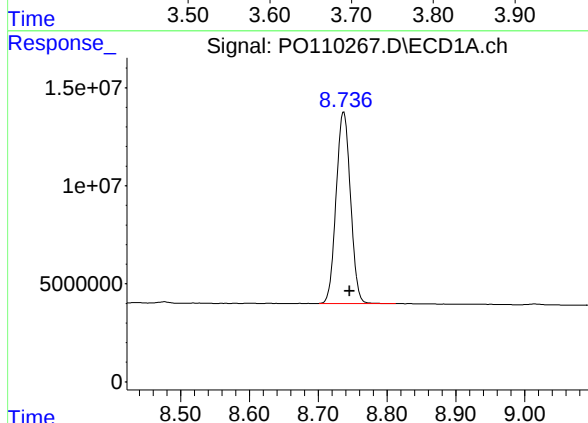

#2 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.008 min
Response: 141670453
Conc: 18.43 ng/ml

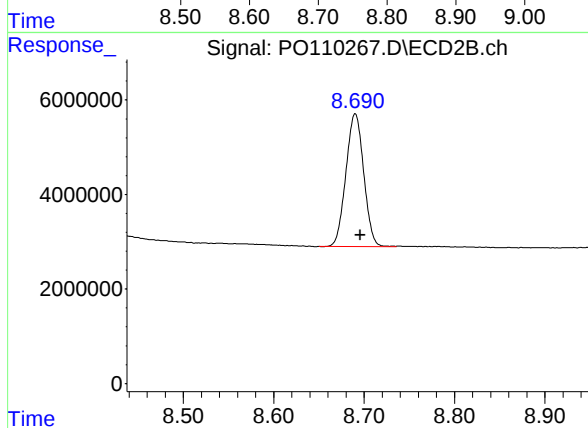

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.006 min
Response: 38504154
Conc: 15.87 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	04/07/25
Project:	Stockton	Date Received:	04/07/25
Client Sample ID:	PIBLK-PO110282.D	SDG No.:	Q1736
Lab Sample ID:	I.BLK-PO110282.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110282.D	1		04/07/25	PO040725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.8		70 (60) - 130 (140)	94%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.2		70 (60) - 130 (140)	81%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 19:04
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:35:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.688	176.0E6	98785740	19.334	18.838
2) SA Decachlor...	8.740	8.692	132.1E6	39381036	17.185	16.232

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 19:04
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:35:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

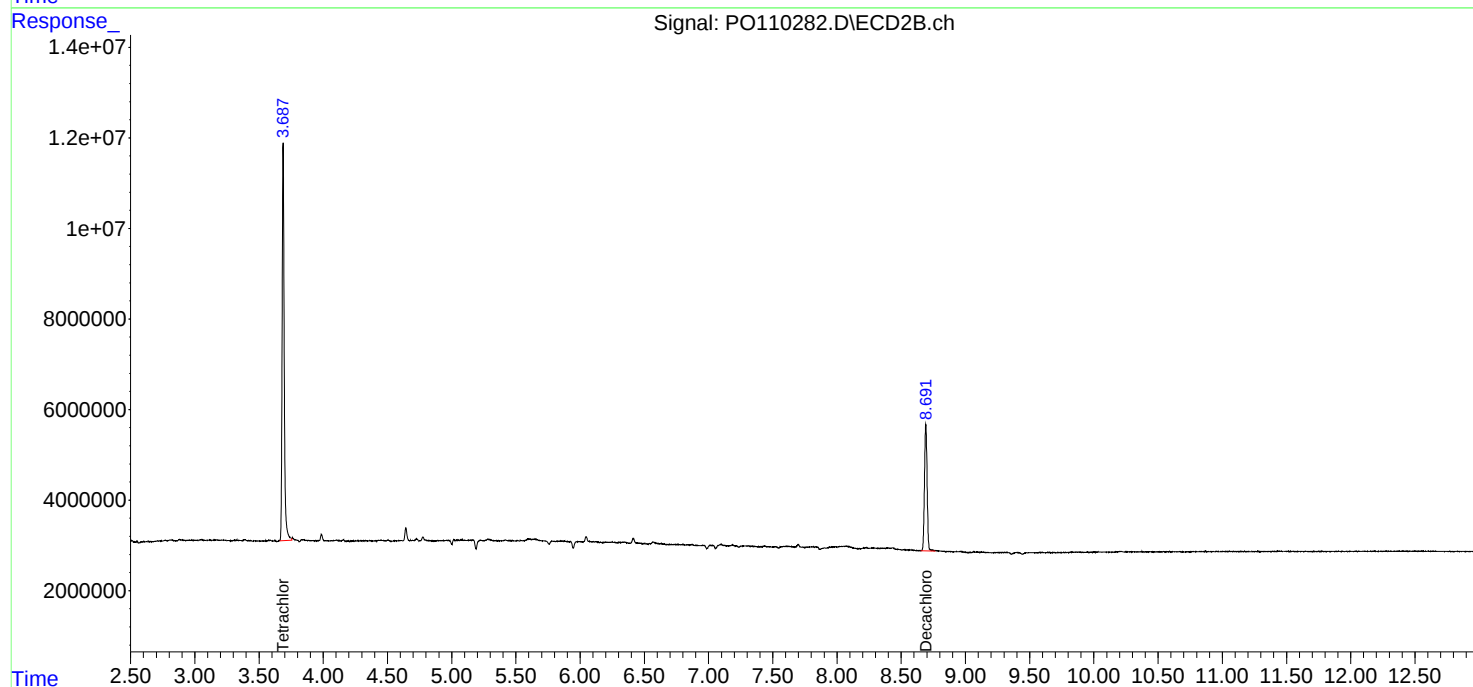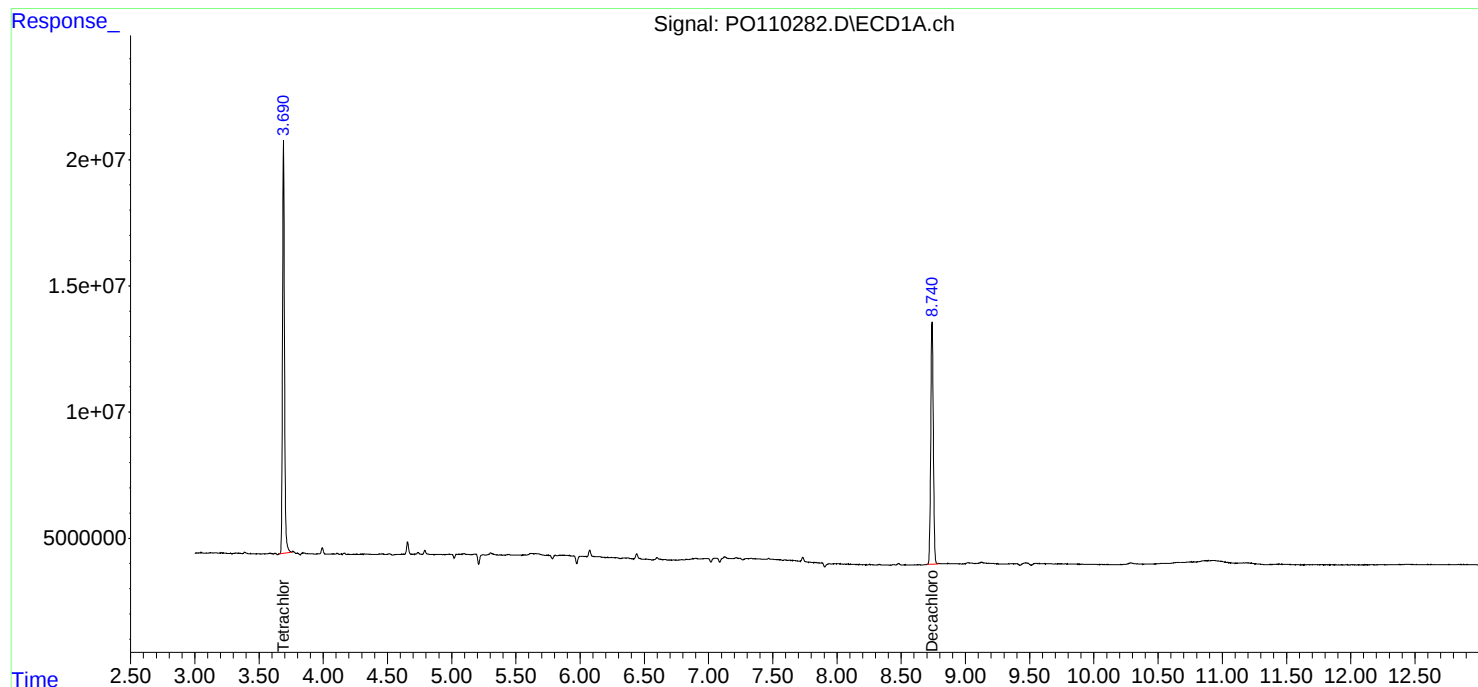


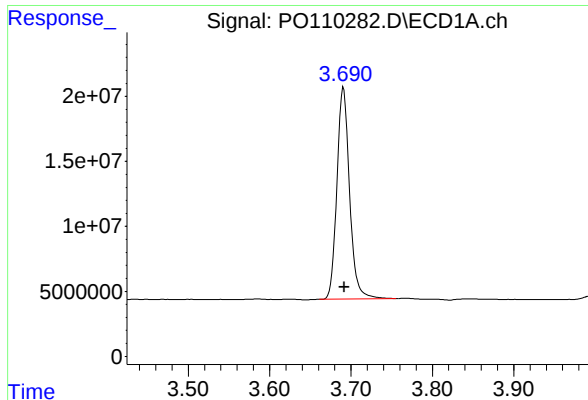

#1 Tetrachloro-m-xylene


R.T.: 3.691 min
Delta R.T.: -0.001 min
Response: 175966498
Conc: 19.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

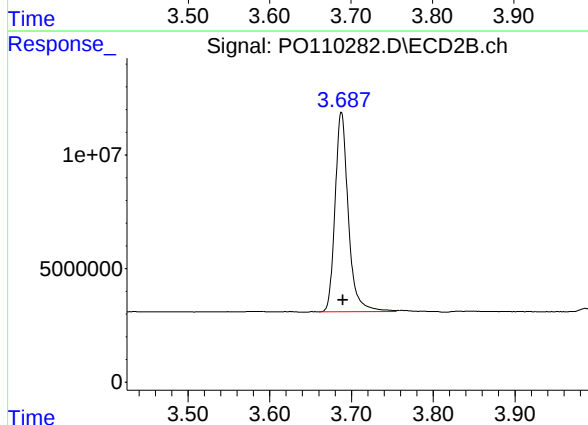


#1 Tetrachloro-m-xylene

R.T.: 3.688 min
Delta R.T.: -0.002 min
Response: 98785740
Conc: 18.84 ng/ml

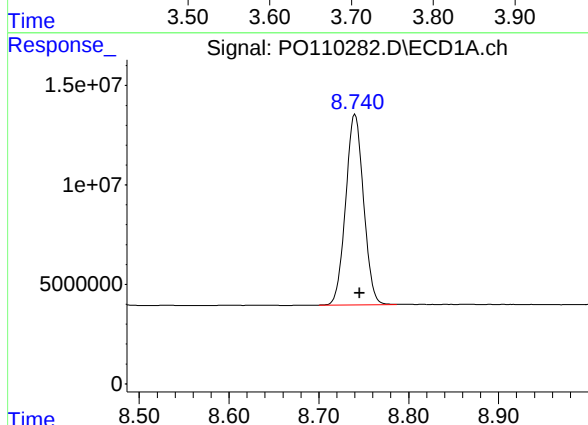

#2 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: -0.005 min
Response: 132132646
Conc: 17.19 ng/ml

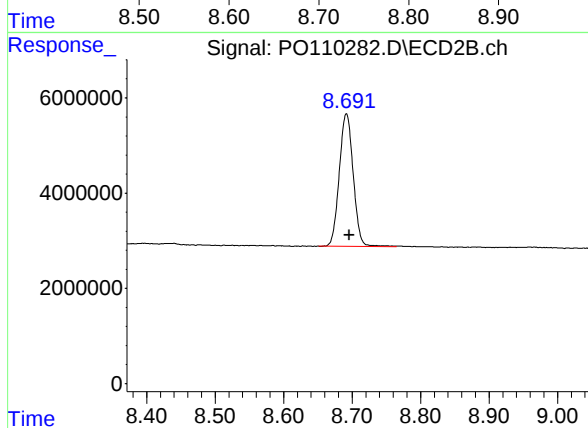

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: -0.004 min
Response: 39381036
Conc: 16.23 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	04/07/25
Project:	Stockton	Date Received:	04/07/25
Client Sample ID:	PIBLK-PO110290.D	SDG No.:	Q1736
Lab Sample ID:	I.BLK-PO110290.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110290.D	1		04/07/25	PO040725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.9		70 (60) - 130 (140)	94%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.2		70 (60) - 130 (140)	81%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 23:17
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:38:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.687	177.5E6	98959783	19.499	18.871
2) SA Decachlor...	8.742	8.692	136.3E6	39361941	17.725	16.224

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 23:17
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:38:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

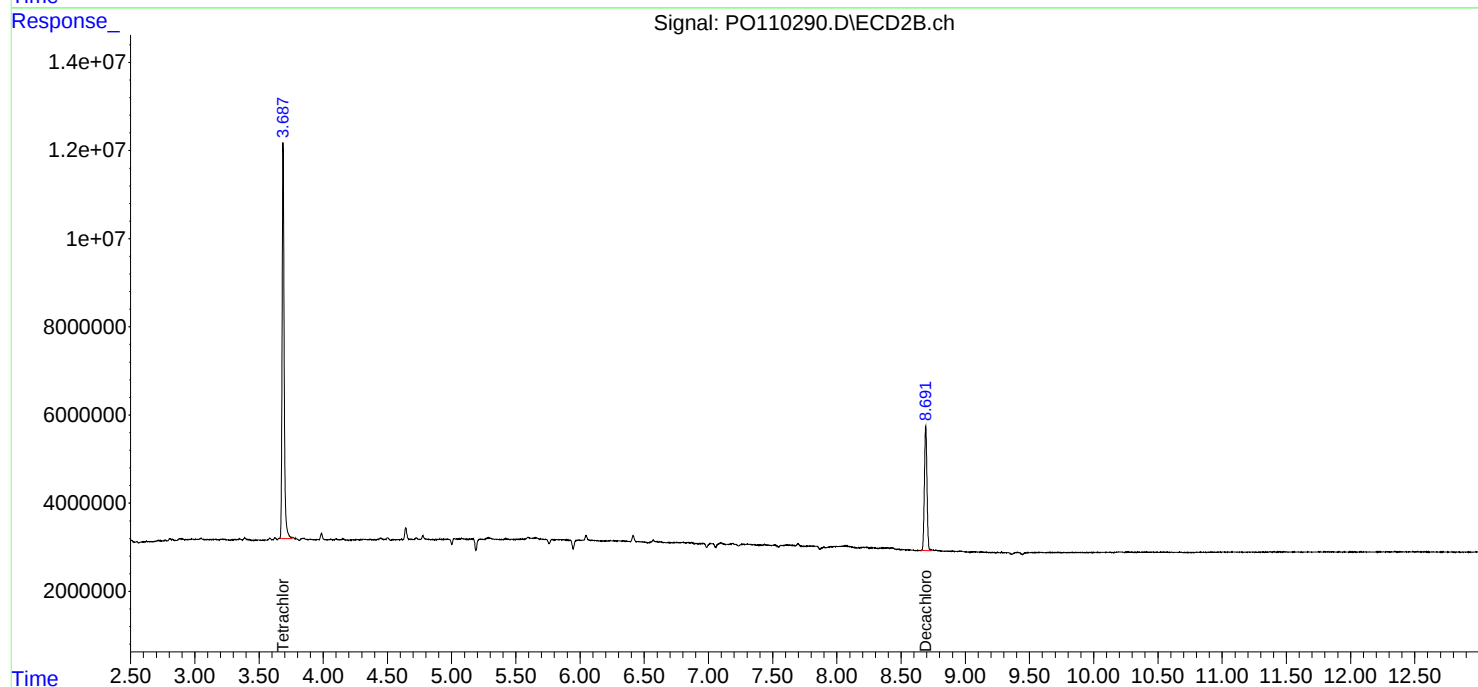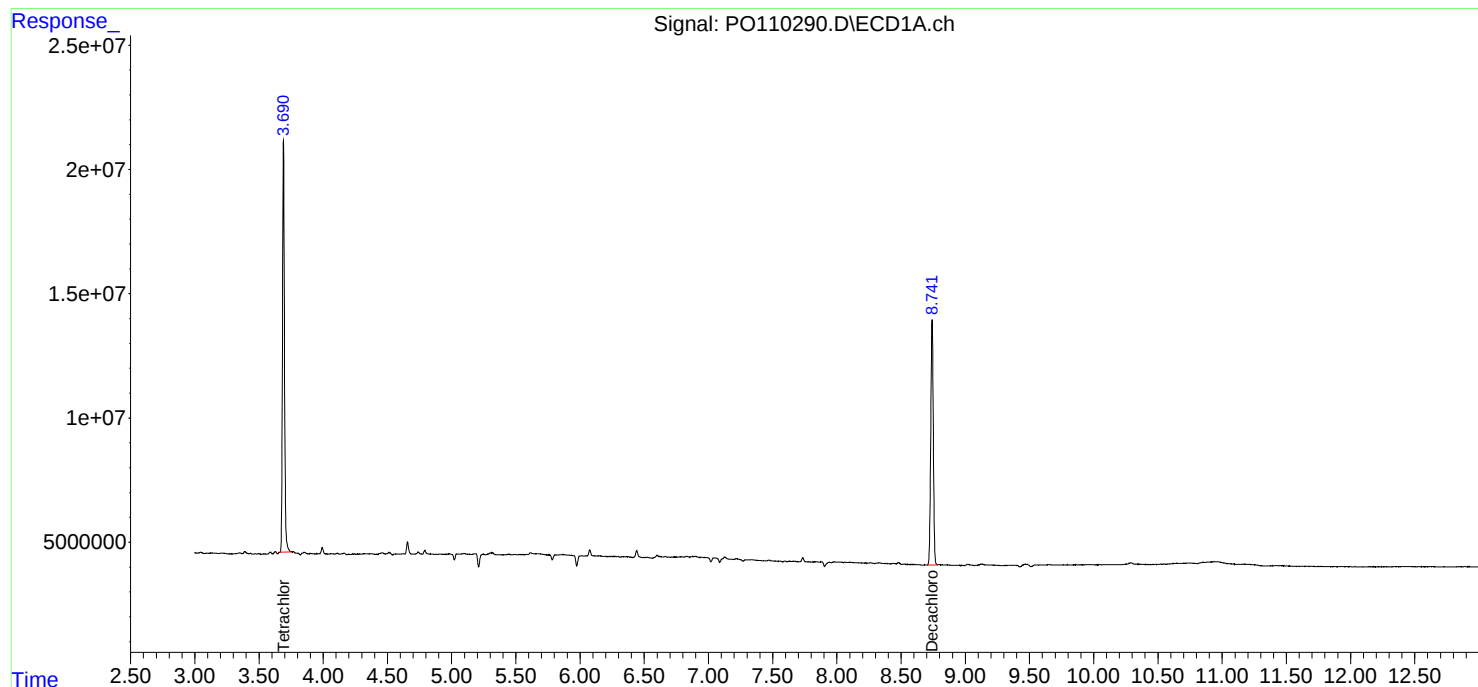


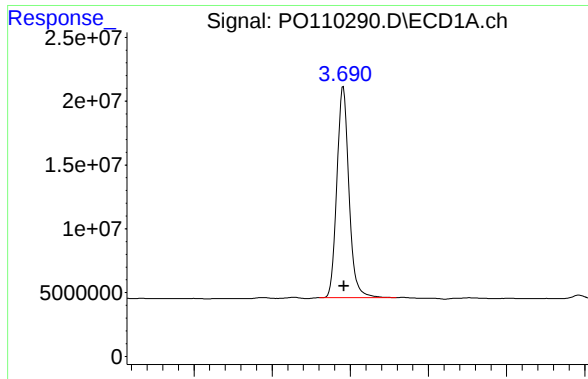

#1 Tetrachloro-m-xylene


R.T.: 3.691 min
Delta R.T.: -0.001 min
Response: 177471328
Conc: 19.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

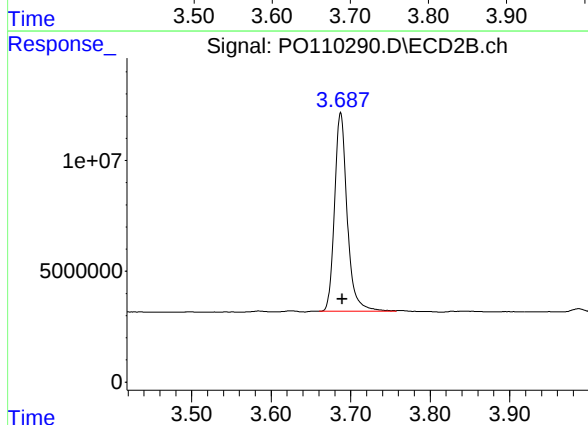


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: -0.002 min
Response: 98959783
Conc: 18.87 ng/ml

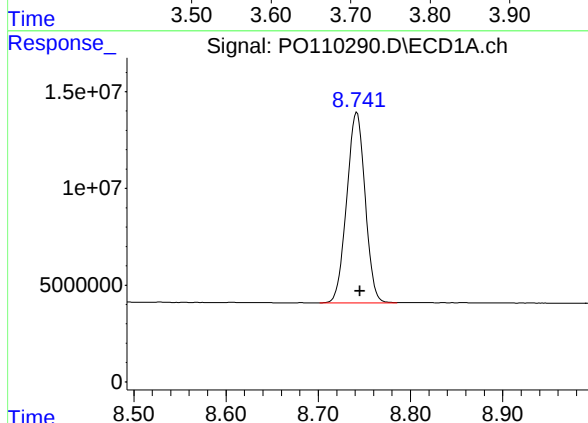

#2 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: -0.004 min
Response: 136281296
Conc: 17.72 ng/ml

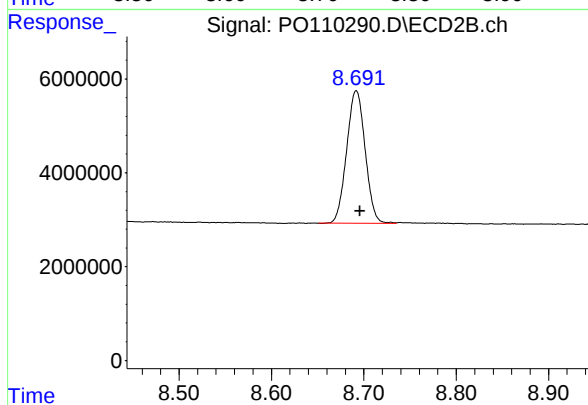

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: -0.004 min
Response: 39361941
Conc: 16.22 ng/ml

Report of Analysis

Client:	G Environmental		Date Collected:		
Project:	Stockton		Date Received:		
Client Sample ID:	PB167469BS		SDG No.:	Q1736	
Lab Sample ID:	PB167469BS		Matrix:	SOIL	
Analytical Method:	SW8082A		% Solid:	100	Decanted:
Sample Wt/Vol:	30.02	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110284.D	1	04/07/25 08:20	04/07/25 19:41	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	141		3.90	17.0	ug/kg
11104-28-2	Aroclor-1221	4.00	U	4.00	17.0	ug/kg
11141-16-5	Aroclor-1232	3.70	U	3.70	17.0	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	17.0	ug/kg
12672-29-6	Aroclor-1248	5.90	U	5.90	17.0	ug/kg
11097-69-1	Aroclor-1254	3.20	U	3.20	17.0	ug/kg
37324-23-5	Aroclor-1262	5.00	U	5.00	17.0	ug/kg
11100-14-4	Aroclor-1268	3.60	U	3.60	17.0	ug/kg
11096-82-5	Aroclor-1260	134		3.20	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.9		30 (32) - 150 (144)	99%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.1		30 (32) - 150 (175)	95%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
 Data File : PO110284.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 19:41
 Operator : YP/AJ
 Sample : PB167469BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB167469BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:36:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.688	180.6E6	99143578	19.847	18.906
2) SA Decachlor...	8.740	8.691	146.7E6	41863016	19.080	17.255
Target Compounds						
3) L1 AR-1016-1	4.782	4.769	142.0E6	74923264	421.865	408.847
4) L1 AR-1016-2	4.802	4.788	199.0E6	105.5E6	429.173	403.452
5) L1 AR-1016-3	4.858	4.964	137.1E6	57705339	427.778	407.010
6) L1 AR-1016-4	4.978	5.005	107.7E6	47781418	426.066	405.168
7) L1 AR-1016-5	5.236	5.218	113.5E6	60210398	412.871	393.741
31) L7 AR-1260-1	6.277	6.250	210.2E6	107.2E6	446.044	419.635
32) L7 AR-1260-2	6.465	6.438	251.9E6	124.0E6	422.920	413.030
33) L7 AR-1260-3	6.833	6.590	173.8E6	115.3E6	358.056	399.028
34) L7 AR-1260-4	7.093	7.062	166.9E6	76919777	393.513	357.636
35) L7 AR-1260-5	7.336	7.303	405.0E6	168.5E6	387.245	337.822



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110284.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 19:41
Operator : YP/AJ
Sample : PB167469BS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB167469BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:36:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

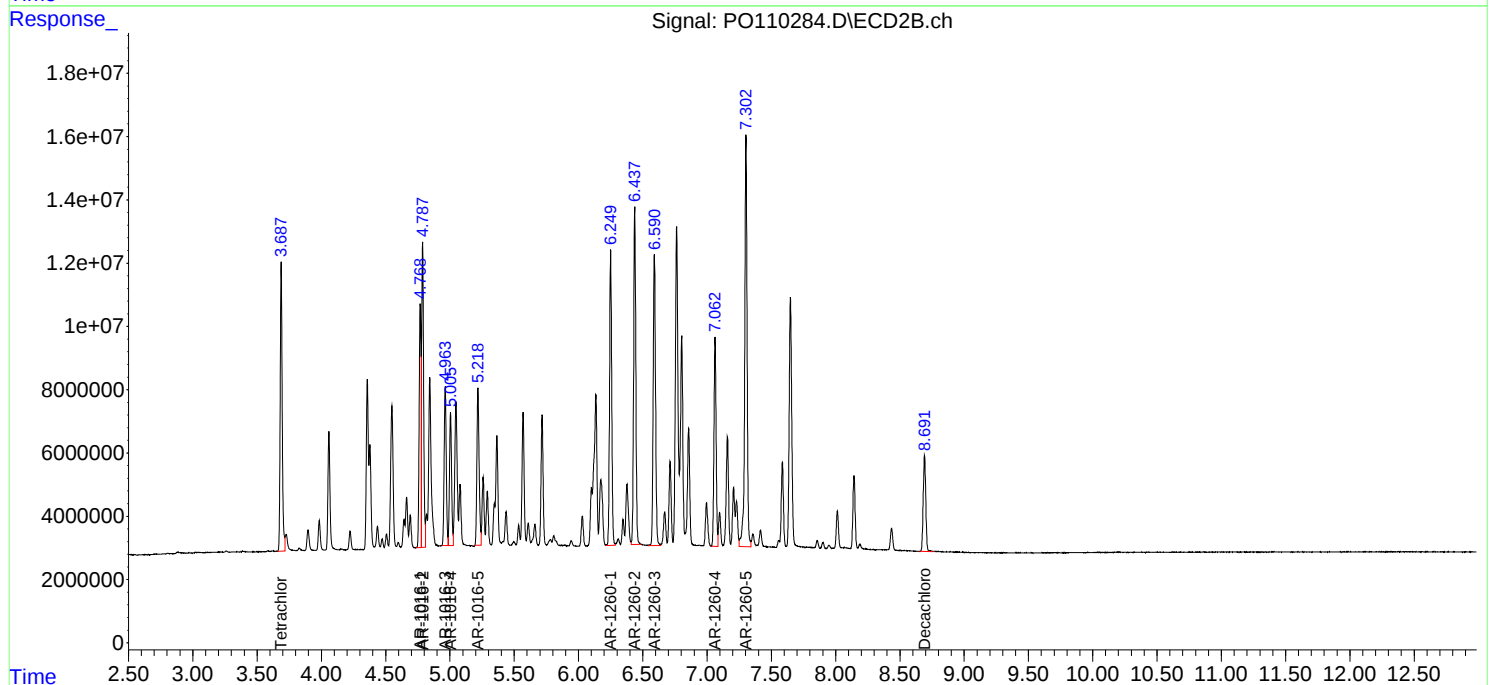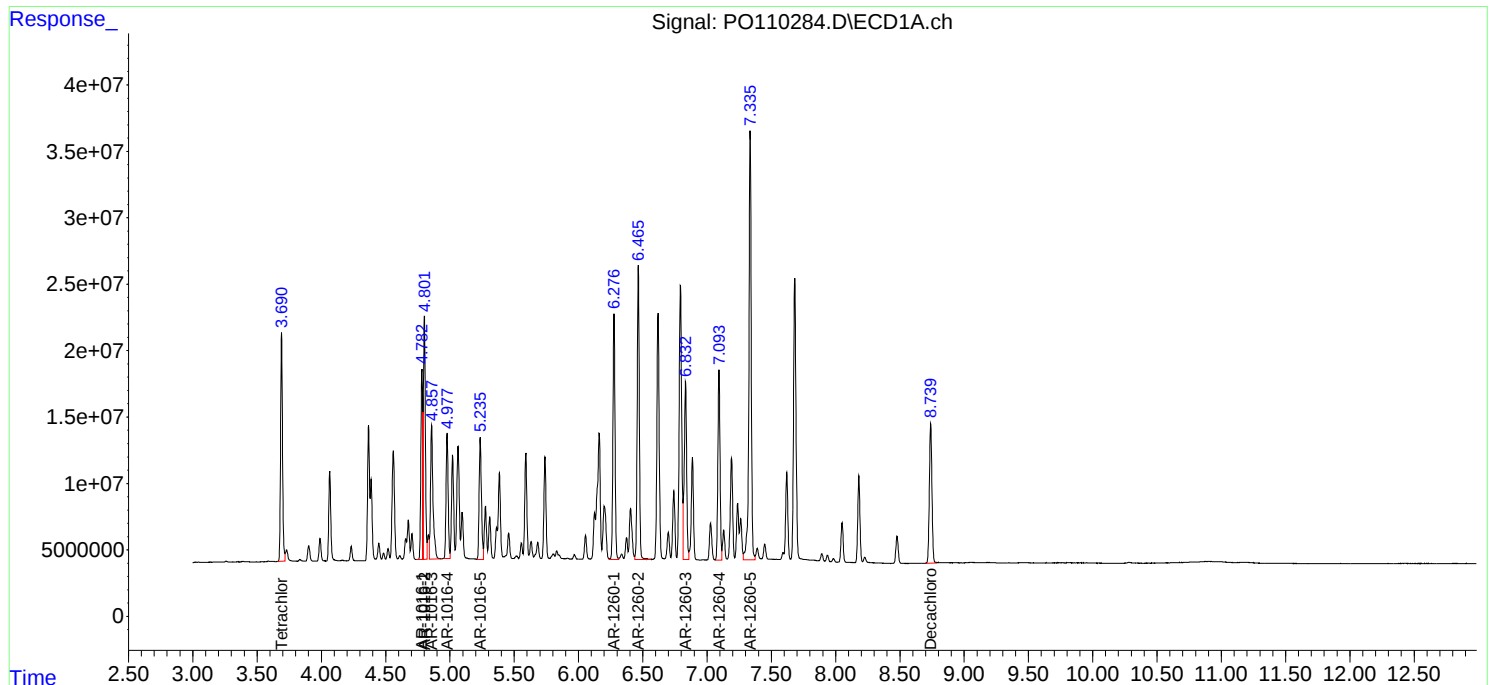

Report of Analysis

Client:	G Environmental	Date Collected:	04/03/25
Project:	Stockton	Date Received:	04/04/25
Client Sample ID:	OU4-VSL-16-040325MS	SDG No.:	Q1736
Lab Sample ID:	Q1730-03MS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	94.5
Sample Wt/Vol:	30.05	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110271.D	1	04/07/25 08:20	04/07/25 14:15	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	170		4.20	18.0	ug/kg
11104-28-2	Aroclor-1221	4.30	U	4.30	18.0	ug/kg
11141-16-5	Aroclor-1232	3.90	U	3.90	18.0	ug/kg
53469-21-9	Aroclor-1242	4.20	U	4.20	18.0	ug/kg
12672-29-6	Aroclor-1248	6.30	U	6.30	18.0	ug/kg
11097-69-1	Aroclor-1254	3.40	U	3.40	18.0	ug/kg
37324-23-5	Aroclor-1262	5.30	U	5.30	18.0	ug/kg
11100-14-4	Aroclor-1268	3.80	U	3.80	18.0	ug/kg
11096-82-5	Aroclor-1260	157		3.40	18.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.8		30 (32) - 150 (144)	114%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.9		30 (32) - 150 (175)	104%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 14:15
 Operator : YP/AJ
 Sample : Q1730-03MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU4-VSL-16-040325MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 14:28:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	3.687	207.8E6	114.5E6	22.829	21.843
2) SA Decachlor...	8.740	8.691	160.6E6	43661585	20.882	17.997
Target Compounds						
3) L1 AR-1016-1	4.782	4.768	163.4E6	86371640	485.641	471.320
4) L1 AR-1016-2	4.802	4.787	226.9E6	123.3E6	489.395	471.405
5) L1 AR-1016-3	4.858	4.963	156.9E6	66829797	489.339	471.367
6) L1 AR-1016-4	4.978	5.005	122.7E6	54685236	485.623	463.710
7) L1 AR-1016-5	5.236	5.218	127.1E6	69082264	462.402	451.758
31) L7 AR-1260-1	6.276	6.250	237.9E6	119.0E6	504.637	465.860
32) L7 AR-1260-2	6.466	6.438	285.8E6	136.5E6	479.876	454.662
33) L7 AR-1260-3	6.833	6.591	199.0E6	126.8E6	409.960	438.894
34) L7 AR-1260-4	7.094	7.062	183.3E6	86758507	432.156	403.381
35) L7 AR-1260-5	7.335	7.303	418.2E6	188.7E6	399.895	378.330



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 14:15
Operator : YP/AJ
Sample : Q1730-03MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-VSL-16-040325MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 14:28:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

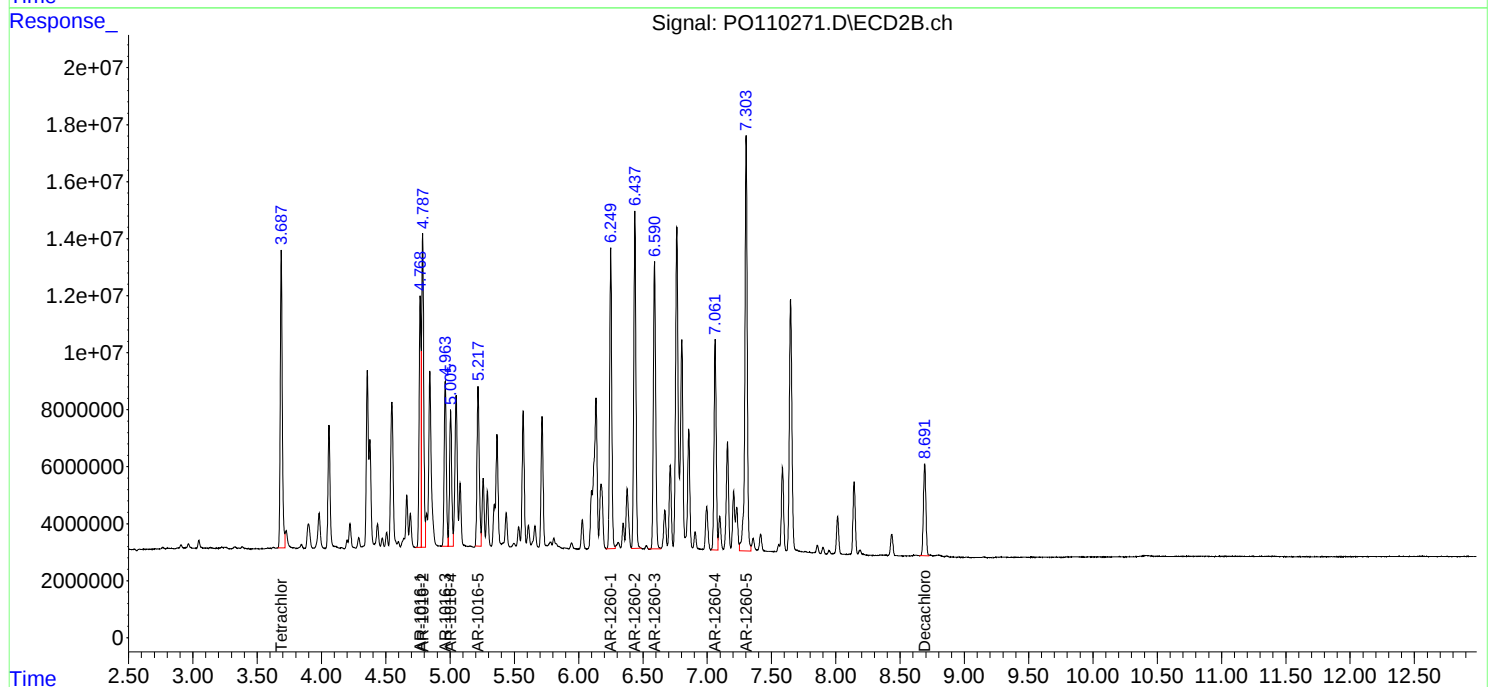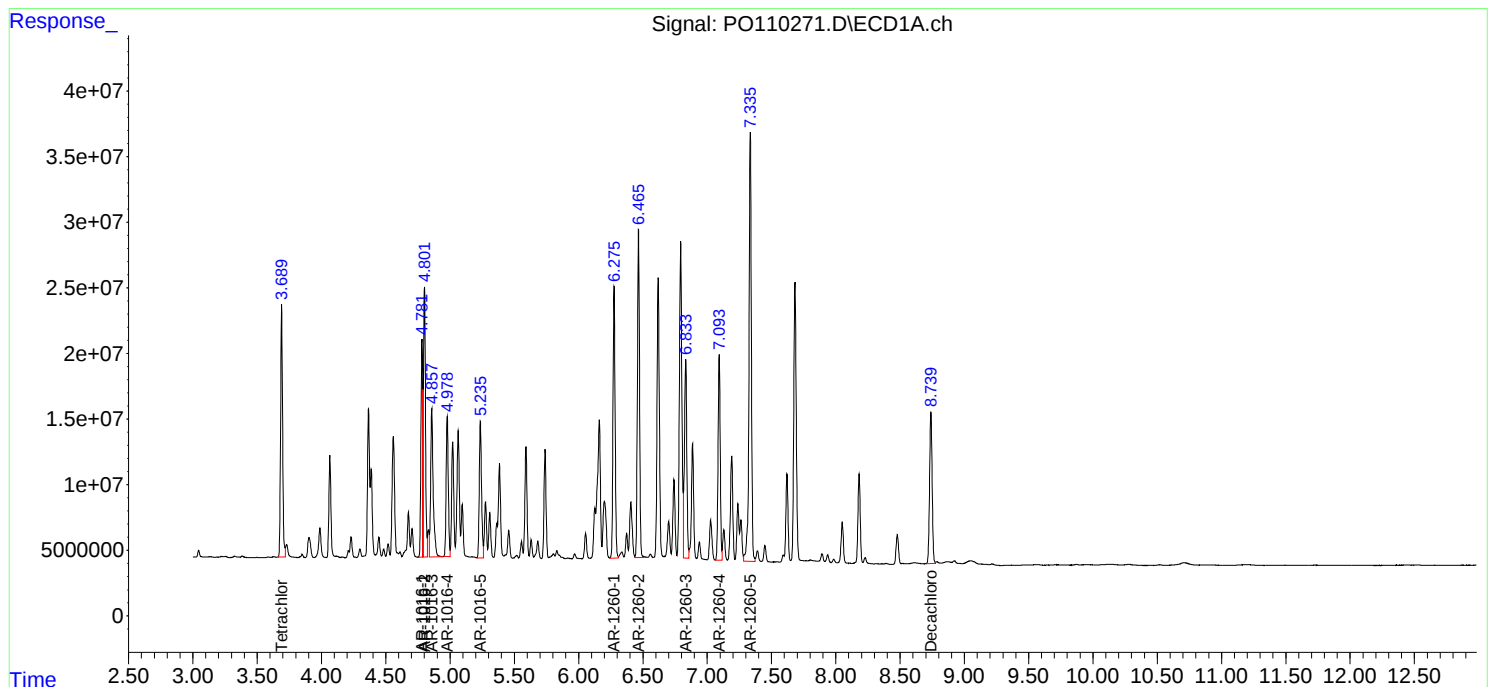

Report of Analysis

Client:	G Environmental	Date Collected:	04/03/25
Project:	Stockton	Date Received:	04/04/25
Client Sample ID:	OU4-VSL-16-040325MSD	SDG No.:	Q1736
Lab Sample ID:	Q1730-03MSD	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	94.5
Sample Wt/Vol:	30.02	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO110272.D	1	04/07/25 08:20	04/07/25 14:33	PB167469

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	164		4.20	18.0	ug/kg
11104-28-2	Aroclor-1221	4.30	U	4.30	18.0	ug/kg
11141-16-5	Aroclor-1232	3.90	U	3.90	18.0	ug/kg
53469-21-9	Aroclor-1242	4.20	U	4.20	18.0	ug/kg
12672-29-6	Aroclor-1248	6.30	U	6.30	18.0	ug/kg
11097-69-1	Aroclor-1254	3.40	U	3.40	18.0	ug/kg
37324-23-5	Aroclor-1262	5.30	U	5.30	18.0	ug/kg
11100-14-4	Aroclor-1268	3.80	U	3.80	18.0	ug/kg
11096-82-5	Aroclor-1260	153		3.40	18.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.6		30 (32) - 150 (144)	108%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.8		30 (32) - 150 (175)	99%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : PO110272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 14:33
 Operator : YP/AJ
 Sample : Q1730-03MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU4-VSL-16-040325MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 14:58:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	3.687	196.9E6	109.1E6	21.633	20.795
2) SA Decachlor...	8.739	8.690	152.2E6	41848584	19.800	17.249
Target Compounds						
3) L1 AR-1016-1	4.782	4.768	156.1E6	82580554	463.781	450.632
4) L1 AR-1016-2	4.801	4.788	219.3E6	118.8E6	472.954	454.443
5) L1 AR-1016-3	4.857	4.963	151.9E6	64490825	473.697	454.870
6) L1 AR-1016-4	4.978	5.005	118.8E6	52631687	470.083	446.297
7) L1 AR-1016-5	5.235	5.217	123.9E6	66656091	450.663	435.892
31) L7 AR-1260-1	6.276	6.250	225.9E6	115.3E6	479.366	451.204
32) L7 AR-1260-2	6.466	6.438	276.1E6	132.5E6	463.567	441.258
33) L7 AR-1260-3	6.833	6.590	196.5E6	122.9E6	404.805	425.130
34) L7 AR-1260-4	7.093	7.061	180.2E6	84267581	424.947	391.799
35) L7 AR-1260-5	7.335	7.302	409.9E6	182.8E6	391.944	366.611



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 14:33
Operator : YP/AJ
Sample : Q1730-03MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-VSL-16-040325MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 14:58:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

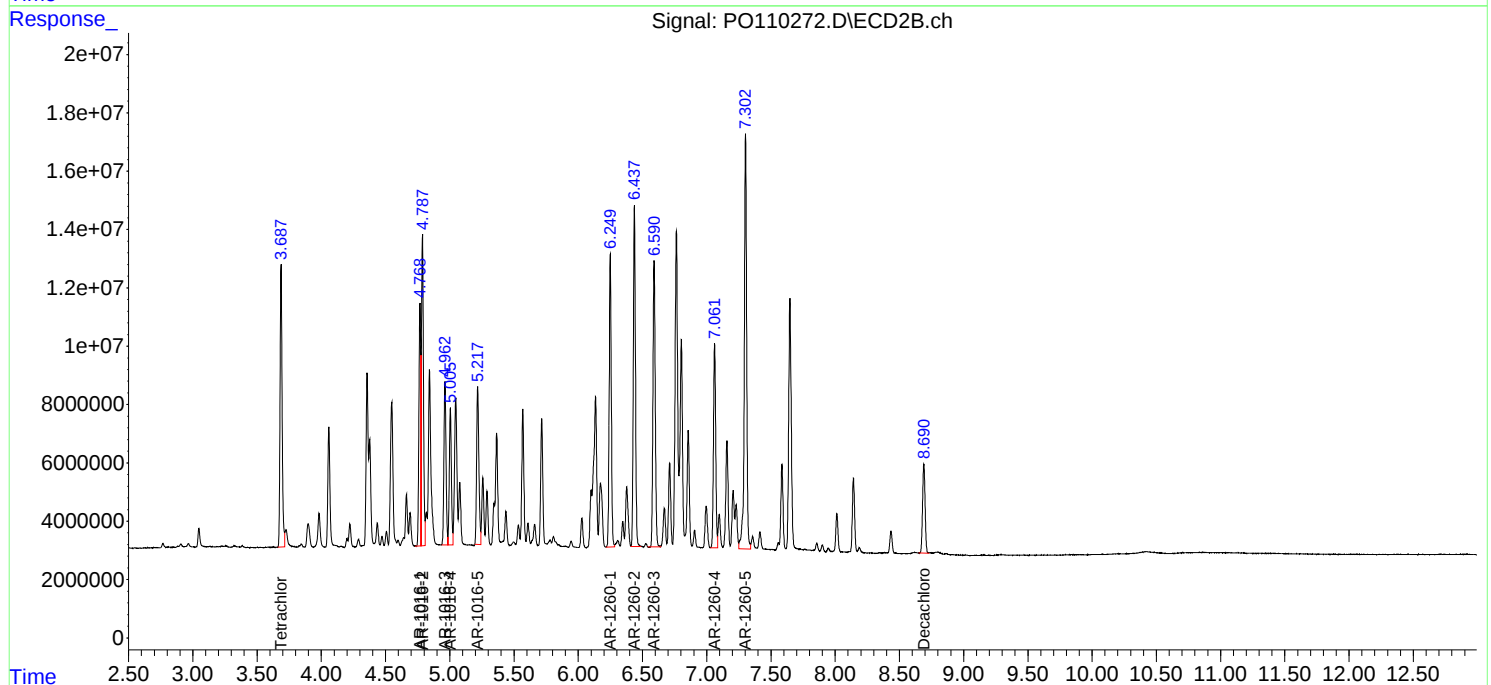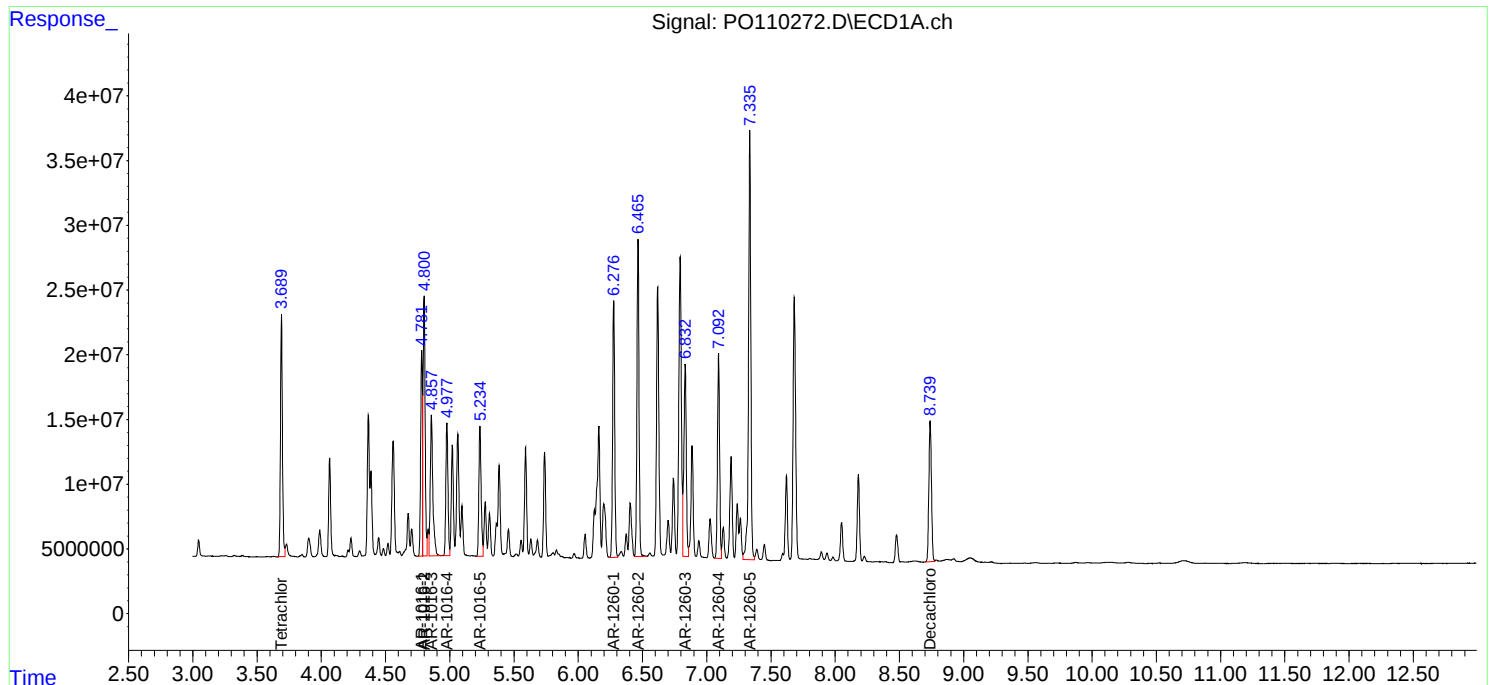

Manual Integration Report

Sequence:	PO031925	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC750	PO109973.D	AR-1260-5 #2	yogesh	3/19/2025 8:01:07 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1660ICC050	PO109976.D	AR-1260-1	yogesh	3/19/2025 8:01:25 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1660ICC050	PO109976.D	AR-1260-1 #2	yogesh	3/19/2025 8:01:25 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1660ICC050	PO109976.D	AR-1260-3 #2	yogesh	3/19/2025 8:01:25 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	AR-1242-3 #2	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	AR-1242-4	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	AR-1242-5	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	AR-1242-5 #2	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	Tetrachloro-m-xylene	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1242ICC050	PO109983.D	Tetrachloro-m-xylene #2	yogesh	3/19/2025 8:01:09 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1248ICC050	PO109988.D	AR-1248-3	yogesh	3/19/2025 8:01:10 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1248ICC050	PO109988.D	AR-1248-4 #2	yogesh	3/19/2025 8:01:10 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1254ICC050	PO109993.D	AR-1254-5 #2	yogesh	3/19/2025 8:01:12 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software

Manual Integration Report

Sequence:	PO031925	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1268ICC500	PO109997.D	AR-1268-1	yogesh	3/19/2025 8:01:13 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC250	PO109998.D	AR-1268-1	yogesh	3/19/2025 8:01:15 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC050	PO109999.D	AR-1268-1	yogesh	3/19/2025 8:01:16 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC050	PO109999.D	AR-1268-4	yogesh	3/19/2025 8:01:16 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC050	PO109999.D	Tetrachloro-m-xylene	yogesh	3/19/2025 8:01:16 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software
AR1268ICC050	PO109999.D	Tetrachloro-m-xylene #2	yogesh	3/19/2025 8:01:16 AM	mohammad	3/24/2025 3:02:46	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	PO040725	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO110286.D	AR-1016-5	yogesh	4/8/2025 7:46:34 AM	mohammad	4/9/2025 2:57:57	Peak Integrated by Software
AR1660CCC500	PO110286.D	AR-1016-5 #2	yogesh	4/8/2025 7:46:34 AM	mohammad	4/9/2025 2:57:57	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031925

Review By	yogesh	Review On	3/18/2025 3:19:21 PM
Supervise By	mohammad	Supervise On	3/24/2025 3:02:46 AM
SubDirectory	PO031925	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	Sampleld	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO109970.D	18 Mar 2025 13:26	YP/AJ	Ok
2	I.BLK	PO109971.D	18 Mar 2025 13:44	YP/AJ	Ok
3	AR1660ICC1000	PO109972.D	18 Mar 2025 14:03	YP/AJ	Ok
4	AR1660ICC750	PO109973.D	18 Mar 2025 14:21	YP/AJ	Ok,M
5	AR1660ICC500	PO109974.D	18 Mar 2025 14:39	YP/AJ	Ok
6	AR1660ICC250	PO109975.D	18 Mar 2025 14:58	YP/AJ	Ok
7	AR1660ICC050	PO109976.D	18 Mar 2025 15:16	YP/AJ	Ok,M
8	AR1221ICC500	PO109977.D	18 Mar 2025 15:34	YP/AJ	Ok
9	AR1232ICC500	PO109978.D	18 Mar 2025 15:53	YP/AJ	Ok
10	AR1242ICC1000	PO109979.D	18 Mar 2025 16:11	YP/AJ	Ok
11	AR1242ICC750	PO109980.D	18 Mar 2025 16:30	YP/AJ	Ok
12	AR1242ICC500	PO109981.D	18 Mar 2025 16:48	YP/AJ	Ok
13	AR1242ICC250	PO109982.D	18 Mar 2025 17:06	YP/AJ	Ok
14	AR1242ICC050	PO109983.D	18 Mar 2025 17:25	YP/AJ	Ok,M
15	AR1248ICC1000	PO109984.D	18 Mar 2025 17:42	YP/AJ	Ok
16	AR1248ICC750	PO109985.D	18 Mar 2025 18:00	YP/AJ	Ok
17	AR1248ICC500	PO109986.D	18 Mar 2025 18:19	YP/AJ	Ok
18	AR1248ICC250	PO109987.D	18 Mar 2025 18:37	YP/AJ	Ok
19	AR1248ICC050	PO109988.D	18 Mar 2025 18:54	YP/AJ	Ok,M
20	AR1254ICC1000	PO109989.D	18 Mar 2025 19:13	YP/AJ	Ok
21	AR1254ICC750	PO109990.D	18 Mar 2025 19:31	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031925

Review By	yogesh	Review On	3/18/2025 3:19:21 PM
Supervise By	mohammad	Supervise On	3/24/2025 3:02:46 AM
SubDirectory	PO031925	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC500	PO109991.D	18 Mar 2025 19:49	YP/AJ	Ok
23	AR1254ICC250	PO109992.D	18 Mar 2025 20:07	YP/AJ	Ok
24	AR1254ICC050	PO109993.D	18 Mar 2025 20:25	YP/AJ	Ok,M
25	AR1262ICC500	PO109994.D	18 Mar 2025 20:43	YP/AJ	Ok
26	AR1268ICC1000	PO109995.D	18 Mar 2025 21:02	YP/AJ	Ok
27	AR1268ICC750	PO109996.D	18 Mar 2025 21:20	YP/AJ	Ok
28	AR1268ICC500	PO109997.D	18 Mar 2025 21:39	YP/AJ	Ok,M
29	AR1268ICC250	PO109998.D	18 Mar 2025 21:57	YP/AJ	Ok,M
30	AR1268ICC050	PO109999.D	18 Mar 2025 22:15	YP/AJ	Ok,M
31	PO031925ICV500	PO110000.D	18 Mar 2025 22:34	YP/AJ	Ok
32	AR1242ICV500	PO110001.D	18 Mar 2025 23:47	YP/AJ	Ok
33	AR1248ICV500	PO110002.D	19 Mar 2025 00:05	YP/AJ	Ok
34	AR1254ICV500	PO110003.D	19 Mar 2025 00:24	YP/AJ	Ok
35	AR1268ICV500	PO110004.D	19 Mar 2025 00:42	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO040725

Review By	yogesh	Review On	4/7/2025 11:16:09 AM
Supervise By	mohammad	Supervise On	4/9/2025 2:57:57 AM
SubDirectory	PO040725	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	Sampleld	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO110262.D	07 Apr 2025 09:08	YP/AJ	Ok
2	AR1660CCC500	PO110263.D	07 Apr 2025 09:46	YP/AJ	Ok
3	AR1242CCC500	PO110264.D	07 Apr 2025 10:05	YP/AJ	Ok
4	AR1248CCC500	PO110265.D	07 Apr 2025 10:23	YP/AJ	Ok
5	AR1254CCC500	PO110266.D	07 Apr 2025 11:18	YP/AJ	Ok
6	I.BLK	PO110267.D	07 Apr 2025 11:36	YP/AJ	Ok
7	Q1723-04DL	PO110268.D	07 Apr 2025 12:14	YP/AJ	Ok
8	Q1730-01	PO110269.D	07 Apr 2025 13:38	YP/AJ	Ok
9	Q1730-03	PO110270.D	07 Apr 2025 13:56	YP/AJ	Ok
10	Q1730-03MS	PO110271.D	07 Apr 2025 14:15	YP/AJ	Ok
11	Q1730-03MSD	PO110272.D	07 Apr 2025 14:33	YP/AJ	Ok
12	Q1736-01	PO110273.D	07 Apr 2025 14:51	YP/AJ	Ok
13	Q1736-02	PO110274.D	07 Apr 2025 15:10	YP/AJ	Ok
14	Q1737-01	PO110275.D	07 Apr 2025 15:28	YP/AJ	Ok,M
15	Q1733-01	PO110276.D	07 Apr 2025 15:47	YP/AJ	Ok,M
16	Q1735-01	PO110277.D	07 Apr 2025 16:05	YP/AJ	Ok
17	AR1660CCC500	PO110278.D	07 Apr 2025 17:14	YP/AJ	Ok
18	AR1242CCC500	PO110279.D	07 Apr 2025 18:09	YP/AJ	Ok
19	AR1248CCC500	PO110280.D	07 Apr 2025 18:27	YP/AJ	Ok
20	AR1254CCC500	PO110281.D	07 Apr 2025 18:45	YP/AJ	Ok
21	I.BLK	PO110282.D	07 Apr 2025 19:04	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO040725

Review By	yogesh	Review On	4/7/2025 11:16:09 AM
Supervise By	mohammad	Supervise On	4/9/2025 2:57:57 AM
SubDirectory	PO040725	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	PB167469BL	PO110283.D	07 Apr 2025 19:22	YP/AJ	Ok
23	PB167469BS	PO110284.D	07 Apr 2025 19:41	YP/AJ	Ok
24	Q1738-01	PO110285.D	07 Apr 2025 19:59	YP/AJ	Ok
25	AR1660CCC500	PO110286.D	07 Apr 2025 21:27	YP/AJ	Ok,M
26	AR1242CCC500	PO110287.D	07 Apr 2025 22:22	YP/AJ	Ok
27	AR1248CCC500	PO110288.D	07 Apr 2025 22:40	YP/AJ	Ok
28	AR1254CCC500	PO110289.D	07 Apr 2025 22:59	YP/AJ	Ok
29	I.BLK	PO110290.D	07 Apr 2025 23:17	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031925

Review By	yogesh	Review On	3/18/2025 3:19:21 PM
Supervise By	mohammad	Supervise On	3/24/2025 3:02:46 AM
SubDirectory	PO031925	HP Acquire Method	HP Processing Method PO031925

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369
CCC	PP24332,PP24347,PP24352,PP24357
Internal Standard/PEM	
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO109970.D	18 Mar 2025 13:26		YP/AJ	Ok
2	I.BLK	I.BLK	PO109971.D	18 Mar 2025 13:44		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO109972.D	18 Mar 2025 14:03		YP/AJ	Ok
4	AR1660ICC750	AR1660ICC750	PO109973.D	18 Mar 2025 14:21		YP/AJ	Ok,M
5	AR1660ICC500	AR1660ICC500	PO109974.D	18 Mar 2025 14:39		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO109975.D	18 Mar 2025 14:58		YP/AJ	Ok
7	AR1660ICC050	AR1660ICC050	PO109976.D	18 Mar 2025 15:16		YP/AJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PO109977.D	18 Mar 2025 15:34		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO109978.D	18 Mar 2025 15:53		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO109979.D	18 Mar 2025 16:11		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO109980.D	18 Mar 2025 16:30		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO109981.D	18 Mar 2025 16:48		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO109982.D	18 Mar 2025 17:06		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO109983.D	18 Mar 2025 17:25		YP/AJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PO109984.D	18 Mar 2025 17:42		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO109985.D	18 Mar 2025 18:00		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO109986.D	18 Mar 2025 18:19		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO109987.D	18 Mar 2025 18:37		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031925

Review By	yogesh	Review On	3/18/2025 3:19:21 PM
Supervise By	mohammad	Supervise On	3/24/2025 3:02:46 AM
SubDirectory	PO031925	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,P P24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP 24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248ICC050	AR1248ICC050	PO109988.D	18 Mar 2025 18:54		YP/AJ	Ok,M
20	AR1254ICC1000	AR1254ICC1000	PO109989.D	18 Mar 2025 19:13		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO109990.D	18 Mar 2025 19:31		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO109991.D	18 Mar 2025 19:49		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO109992.D	18 Mar 2025 20:07		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO109993.D	18 Mar 2025 20:25		YP/AJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PO109994.D	18 Mar 2025 20:43		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO109995.D	18 Mar 2025 21:02		YP/AJ	Ok
27	AR1268ICC750	AR1268ICC750	PO109996.D	18 Mar 2025 21:20		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO109997.D	18 Mar 2025 21:39		YP/AJ	Ok,M
29	AR1268ICC250	AR1268ICC250	PO109998.D	18 Mar 2025 21:57		YP/AJ	Ok,M
30	AR1268ICC050	AR1268ICC050	PO109999.D	18 Mar 2025 22:15		YP/AJ	Ok,M
31	PO031925ICV500	ICVPO031925	PO110000.D	18 Mar 2025 22:34		YP/AJ	Ok
32	AR1242ICV500	ICVPO031925AR1242	PO110001.D	18 Mar 2025 23:47		YP/AJ	Ok
33	AR1248ICV500	ICVPO031925AR1248	PO110002.D	19 Mar 2025 00:05		YP/AJ	Ok
34	AR1254ICV500	ICVPO031925AR1254	PO110003.D	19 Mar 2025 00:24		YP/AJ	Ok
35	AR1268ICV500	ICVPO031925AR1268	PO110004.D	19 Mar 2025 00:42		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO040725

Review By	yogesh	Review On	4/7/2025 11:16:09 AM
Supervise By	mohammad	Supervise On	4/9/2025 2:57:57 AM
SubDirectory	PO040725	HP Acquire Method	HP Processing Method PO031925

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369
CCC	PP24332,PP24347,PP24352,PP24357
Internal Standard/PEM	
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO110262.D	07 Apr 2025 09:08		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO110263.D	07 Apr 2025 09:46		YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO110264.D	07 Apr 2025 10:05		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO110265.D	07 Apr 2025 10:23		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO110266.D	07 Apr 2025 11:18		YP/AJ	Ok
6	I.BLK	I.BLK	PO110267.D	07 Apr 2025 11:36		YP/AJ	Ok
7	Q1723-04DL	GAS-AUD-25-0037DL	PO110268.D	07 Apr 2025 12:14	AR1254 Hit	YP/AJ	Ok
8	Q1730-01	OU4-VSL-15-040325	PO110269.D	07 Apr 2025 13:38		YP/AJ	Ok
9	Q1730-03	OU4-VSL-16-040325	PO110270.D	07 Apr 2025 13:56		YP/AJ	Ok
10	Q1730-03MS	OU4-VSL-16-040325M	PO110271.D	07 Apr 2025 14:15		YP/AJ	Ok
11	Q1730-03MSD	OU4-VSL-16-040325M	PO110272.D	07 Apr 2025 14:33		YP/AJ	Ok
12	Q1736-01	GST1	PO110273.D	07 Apr 2025 14:51		YP/AJ	Ok
13	Q1736-02	GST2	PO110274.D	07 Apr 2025 15:10		YP/AJ	Ok
14	Q1737-01	RT3069	PO110275.D	07 Apr 2025 15:28	AR1260 hit	YP/AJ	Ok,M
15	Q1733-01	ETGI-328	PO110276.D	07 Apr 2025 15:47		YP/AJ	Ok,M
16	Q1735-01	50660-50661-50662-50663	PO110277.D	07 Apr 2025 16:05		YP/AJ	Ok
17	AR1660CCC500	AR1660CCC500	PO110278.D	07 Apr 2025 17:14		YP/AJ	Ok
18	AR1242CCC500	AR1242CCC500	PO110279.D	07 Apr 2025 18:09		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO040725

Review By	yogesh	Review On	4/7/2025 11:16:09 AM
Supervise By	mohammad	Supervise On	4/9/2025 2:57:57 AM
SubDirectory	PO040725	HP Acquire Method	HP Processing Method PO031925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,P P24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP 24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248CCC500	AR1248CCC500	PO110280.D	07 Apr 2025 18:27		YP/AJ	Ok
20	AR1254CCC500	AR1254CCC500	PO110281.D	07 Apr 2025 18:45		YP/AJ	Ok
21	I.BLK	I.BLK	PO110282.D	07 Apr 2025 19:04		YP/AJ	Ok
22	PB167469BL	PB167469BL	PO110283.D	07 Apr 2025 19:22		YP/AJ	Ok
23	PB167469BS	PB167469BS	PO110284.D	07 Apr 2025 19:41		YP/AJ	Ok
24	Q1738-01	OK-02-040425	PO110285.D	07 Apr 2025 19:59		YP/AJ	Ok
25	AR1660CCC500	AR1660CCC500	PO110286.D	07 Apr 2025 21:27		YP/AJ	Ok,M
26	AR1242CCC500	AR1242CCC500	PO110287.D	07 Apr 2025 22:22		YP/AJ	Ok
27	AR1248CCC500	AR1248CCC500	PO110288.D	07 Apr 2025 22:40		YP/AJ	Ok
28	AR1254CCC500	AR1254CCC500	PO110289.D	07 Apr 2025 22:59		YP/AJ	Ok
29	I.BLK	I.BLK	PO110290.D	07 Apr 2025 23:17		YP/AJ	Ok

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 4/7/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:00
In Date: 04/04/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 103
Time OUT: 08:25
Out Date: 04/05/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB135307

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1729-05	SVOC-GPC-BLANK	1	1.00	1.00	2.00	2.00	100.0	
Q1729-06	PEST-GPC-BLANK	2	1.00	1.00	2.00	2.00	100.0	
Q1729-07	PEST-GPC-BLANK-SPIKE	3	1.00	1.00	2.00	2.00	100.0	
Q1729-08	PCB-GPC-BLANK	4	1.00	1.00	2.00	2.00	100.0	
Q1729-09	PCB-GPC-BLANK-SPIKE	5	1.00	1.00	2.00	2.00	100.0	
Q1729-10	SVOC-GPC2-BLANK	6	1.00	1.00	2.00	2.00	100.0	
Q1729-11	PEST-GPC2-BLANK	7	1.00	1.00	2.00	2.00	100.0	
Q1729-12	PEST-GPC2-BLANK-SPIKE	8	1.00	1.00	2.00	2.00	100.0	
Q1729-13	PCB-GPC2-BLANK	9	1.00	1.00	2.00	2.00	100.0	
Q1729-14	PCB-GPC2-BLANK-SPIKE	10	1.00	1.00	2.00	2.00	100.0	
Q1730-01	OU4-VSL-15-040325	11	1.14	10.58	11.72	11.39	96.9	
Q1730-03	OU4-VSL-16-040325	12	1.15	10.28	11.43	10.86	94.5	
Q1730-05	OU4-VSL-17-040325	13	1.16	11.32	12.48	11.62	92.4	
Q1730-07	OU4-PCS-TC-21-040325	14	1.18	10.92	12.1	10.9	89.0	
Q1730-09	OU4-PCS-TC-22-040325	15	1.16	11.79	12.95	11.87	90.8	
Q1730-11	OU4-PCS-TC-23-040325	16	1.19	11.24	12.43	11.41	90.9	
Q1730-13	OU4-PCS-TC-24-040325	17	1.18	10.42	11.6	10.69	91.3	
Q1730-15	OU4-PCS-TC-25-040325	18	1.14	11.13	12.27	11.43	92.5	
Q1730-17	OU4-PCS-TC-26-040325	19	1.15	10.84	11.99	11.13	92.1	
Q1730-19	OU4-CF-15-040325	20	1.15	10.74	11.89	11.23	93.9	
Q1732-01	TT-8	21	1.15	10.40	11.55	10.48	89.7	
Q1732-02	TT-8-EPH	22	1.15	10.33	11.48	10.34	89.0	
Q1732-03	TT-8-VOC	23	1.19	10.01	11.2	10.11	89.1	
Q1733-01	ETGI-328	24	1.18	10.19	11.37	8.37	70.6	
Q1733-02	ETGI-328-E2	25	1.18	10.29	11.47	8.27	68.9	
Q1734-01	HEH6237-1-1	26	1.00	1.00	2.00	2.00	100.0	pile
Q1734-02	HEH6237-1-2	27	1.00	1.00	2.00	2.00	100.0	pile
Q1734-03	STJ23-1-1	28	1.00	1.00	2.00	2.00	100.0	pile



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 4/7/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:00
In Date: 04/04/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 103
Time OUT: 08:25
Out Date: 04/05/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB135307

Lab ID	Client SampleID	Dish #	Dish Wt (g) (A)	Sample Wt (g)	Dish + Sample Wt (g) (B)	Dish+Dry Sample Wt (g) (C)	% Solid	Comments
Q1734-04	STJ23-1-2	29	1.00	1.00	2.00	2.00	100.0	oilc
Q1734-05	HIA989S-1-1	30	1.00	1.00	2.00	2.00	100.0	oilc
Q1734-06	HIA989S-1-2	31	1.00	1.00	2.00	2.00	100.0	oilc
Q1734-07	HED302R-1-1	32	1.00	1.00	2.00	2.00	100.0	oilc
Q1734-08	HED302R-1-2	33	1.00	1.00	2.00	2.00	100.0	oilc
Q1734-09	HED302R-2-1	34	1.00	1.00	2.00	2.00	100.0	oilc
Q1734-10	HED302R-2-2	35	1.00	1.00	2.00	2.00	100.0	oilc
Q1735-01	50660-50661-50662-5663-COMP	36	1.18	10.92	12.1	10.42	84.6	
Q1736-01	GST1	37	1.18	10.04	11.22	9.07	78.6	
Q1736-02	GST2	38	1.18	10.93	12.11	9.98	80.5	
Q1737-01	RT3069	39	1.19	11.58	12.77	11.34	87.7	
Q1738-01	OK-02-040425	40	1.16	10.34	11.5	10.06	86.1	
Q1738-02	OK-02-040425-E2	41	1.19	10.54	11.73	10.37	87.1	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

VB 135307

WorkList Name : %1-040425

WorkList ID : 188724

Department : Wet-Chemistry

Date : 04-04-2025 08:12:22

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1736-01	GST1	Solid	Percent Solids	Cool 4 deg C	GENV01	L21	04/04/2025	Chemtech -SO
Q1736-02	GST2	Solid	Percent Solids	Cool 4 deg C	GENV01	L21	04/04/2025	Chemtech -SO
Q1730-01	OU4-VSL-15-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-03	OU4-VSL-16-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-05	OU4-VSL-17-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-07	OU4-PCS-TC-21-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-09	OU4-PCS-TC-22-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-11	OU4-PCS-TC-23-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-13	OU4-PCS-TC-24-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-15	OU4-PCS-TC-25-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-17	OU4-PCS-TC-26-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1730-19	OU4-CF-15-040325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1729-05	SVOC-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	NOBI03	L31	04/03/2025	Chemtech -SO
Q1729-06	PEST-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-07	PEST-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-08	PCB-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-09	PCB-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-10	SVOC-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-11	PEST-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-12	PEST-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1729-13	PCB-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO

Date/Time 04/04/25 15:20

Raw Sample Received by: JB 0001

Raw Sample Relinquished by: JB 0001

Date/Time 04/04/25

Raw Sample Received by: JB 0001

Raw Sample Relinquished by: JB 0001

WORKLIST(Hardcopy Internal Chain)

107135307

WorkList Name : %1-040425

WorkList ID : 188724

Department : Wet-Chemistry

Date : 04-04-2025 08:12:22

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1729-14	PCB-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	04/04/2025	Chemtech -SO
Q1732-01	TT-8	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1732-02	TT-8-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1732-03	TT-8-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1733-01	ETGI-328	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1733-02	ETGI-328-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	I31	04/04/2025	Chemtech -SO
Q1734-01	HEH6237-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	I31	04/04/2025	Chemtech -SO
Q1734-08	HED302R-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-09	HED302R-2-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-10	HED302R-2-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1735-01	50660-50661-50662-5663-COM	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1737-01	RT3069	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-02	HEH6237-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-03	STJ23-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-04	STJ23-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-05	HIA989S-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-06	HIA989S-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1734-07	HED302R-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/04/2025	Chemtech -SO
Q1738-01	OK-02-040425	Solid	Percent Solids	Cool 4 deg C	PSEG05	L31	04/04/2025	Chemtech -SO
Q1738-02	OK-02-040425-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L31	04/04/2025	Chemtech -SO

Date/Time 04/04/25 15:20

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: [Signature]

Date/Time 04/04/25 17:15

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: [Signature]

SOP ID: M3541-ASE Extraction-14

Clean Up SOP #: Acid Cleanup **Extraction Start Date :** 04/07/2025

Matrix : Solid **Extraction Start Time :** 08:20

Weigh By: EH **Extraction By:** RJ **Extraction End Date :** 04/07/2025

Balance check: RJ **Filter By:** RJ **Extraction End Time :** 11:30

Balance ID: EX-SC-2 **pH Meter ID:** N/A **Concentration By:** EH

pH Strip Lot#: N/A **Hood ID:** 3,7 **Supervisor By :** rajesh

Extraction Method: ☐ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24328
Surrogate	1.0ML	200 PPB	PP24217
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2592
Baked Na2SO4	N/A	EP2597
Sand	N/A	E2865
Hexane	N/A	E3916
H2SO4 1:1	N/A	EP2565
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40 BTS721. Q1735-01 Limited volume used as sample is Oily matrix.

KD Bath ID: N/A **Envap ID:** NEVAP-02

KD Bath Temperature: N/A **Envap Temperature:** 40 °C


Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
04/04/25 11:35	RP (Entr 245)	Y.P. Pest + IPCB.
	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-14

Concentration Date: 04/07/2025

Sample ID	Client Sample ID	Test	g/ mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB167469BL	ABLK469	PCB	30.01	N/A	ritesh	Evelyn	10			U7-1
PB167469BS	ALCS469	PCB	30.02	N/A	ritesh	Evelyn	10			2
Q1730-01	OU4-VSL-15-040325	PCB	30.07	N/A	ritesh	Evelyn	10	E		3
Q1730-03	OU4-VSL-16-040325	PCB	30.03	N/A	ritesh	Evelyn	10	E		4
Q1730-03MS	OU4-VSL-16-040325MS	PCB	30.05	N/A	ritesh	Evelyn	10	E		5
Q1730-03MS D	OU4-VSL-16-040325MSD	PCB	30.02	N/A	ritesh	Evelyn	10	E		6
Q1730-05	OU4-VSL-17-040325	PCB	30.08	N/A	ritesh	Evelyn	10	E		U2-1
Q1730-07	OU4-PCS-TC-21-040325	PCB	30.01	N/A	ritesh	Evelyn	10	E		2
Q1730-09	OU4-PCS-TC-22-040325	PCB	30.02	N/A	ritesh	Evelyn	10	E		3
Q1730-11	OU4-PCS-TC-23-040325	PCB	30.05	N/A	ritesh	Evelyn	10	E		4
Q1730-13	OU4-PCS-TC-24-040325	PCB	30.08	N/A	ritesh	Evelyn	10	E		5
Q1730-15	OU4-PCS-TC-25-040325	PCB	30.06	N/A	ritesh	Evelyn	10	E		6
Q1730-17	OU4-PCS-TC-26-040325	PCB	30.03	N/A	ritesh	Evelyn	10	E		U3-1
Q1730-19	OU4-CF-15-040325	PCB	30.02	N/A	ritesh	Evelyn	10	E		2
Q1732-01	TT-8	PCB	30.04	N/A	ritesh	Evelyn	10	D		3
Q1733-01	ETGI-328	PCB	30.06	N/A	ritesh	Evelyn	10	E	Small Particle	4
Q1735-01	50660-50661-50662-566 3-COMP	PCB	5.06	N/A	ritesh	Evelyn	10	E	Oily Debris	5
Q1736-01	GST1	PCB	30.07	N/A	ritesh	Evelyn	10			6
Q1736-02	GST2	PCB	30.03	N/A	ritesh	Evelyn	10			U6-1
Q1737-01	RT3069	PCB	30.05	N/A	ritesh	Evelyn	10	D		2
Q1738-01	OK-02-040425	PCB	30.01	N/A	ritesh	Evelyn	10	E		3

* Extracts relinquished on the same date as received.



WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q1732 WorkList ID : 188759 Department : Extraction Date : 04-07-2025 08:15:59

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1730-01	OU4-VSL-15-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-03	OU4-VSL-16-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-05	OU4-VSL-17-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-07	OU4-PCS-TC-21-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-09	OU4-PCS-TC-22-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-11	OU4-PCS-TC-23-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-13	OU4-PCS-TC-24-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-15	OU4-PCS-TC-25-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-17	OU4-PCS-TC-26-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1730-19	OU4-CF-15-040325	Solid	Pesticide-TCL	Cool 4 deg C	NOBI03	L31	04/03/2025	8081B
Q1732-01	TT-8	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	L31	04/04/2025	8081B
Q1733-01	ETGI-328	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	I31	04/04/2025	8081B
Q1737-01	RT3069	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	L31	04/04/2025	8081B
Q1738-01	OK-02-040425	Solid	Pesticide-TCL	Cool 4 deg C	PSEG05	L31	04/04/2025	8081B

Date/Time 04/07/25 8:17
Raw Sample Received by: RJ Fed (03)
Raw Sample Relinquished by: OP SM

Date/Time 04/07/25 3:00
Raw Sample Received by: OP SM
Raw Sample Relinquished by: RJ Fed (03)

Prep Standard - Chemical Standard Summary

Order ID : Q1736

Test : PCB

Prepbatch ID : PB167469,

Sequence ID/Qc Batch ID: PO040725,

Standard ID :

EP2565,EP2592,EP2597,PP24217,PP24328,PP24329,PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369,PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387,

Chemical ID :

E2865,E3551,E3804,E3876,E3877,E3916,M5173,P11522,P12699,P12702,P12931,P12936,P12948,P12949,P12957,P13354,P13356,P13373,P13381,P13589,P13591,P13697,P13702,P13830,P13878,P13883,W3112,W3177,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2565	11/20/2024	05/20/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/20/2024

FROM 1000.00000ml of M5173 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2592	02/27/2025	08/12/2025	RUPESHKUMAR SHAH	None	None	Riteshkumar Patel 02/27/2025

FROM 4000.00000ml of E3876 + 4000.00000ml of E3877 = Final Quantity: 8000.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2597	03/28/2025	07/01/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	Evelyn Huang 03/28/2025
<u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP24217	03/05/2025	08/25/2025	Abdul Mirza	None	None	Yogesh Patel 03/06/2025
<u>FROM</u> 1.00000ml of P13354 + 999.00000ml of E3876 = Final Quantity: 1000.000 ml								

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP24328	03/17/2025	08/25/2025	Abdul Mirza	None	None	Yogesh Patel
								04/02/2025

FROM 0.50000ml of P12948 + 99.50000ml of E3876 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24329	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P13356 + 9.00000ml of W3177 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP24330	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13697 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP24331	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP24332	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24330 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP24333	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP24334	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24332 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP24335	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13702 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP24336	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24335 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP24337	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24335 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP24338	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24335 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP24339	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24337 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP24340	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13878 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP24341	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24340 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP24342	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24340 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP24343	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24340 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP24344	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24342 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP24345	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P12931 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP24346	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.75000ml of PP24345 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP24347	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24345 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP24348	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24345 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP24349	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24347 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP24350	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P12936 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP24351	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24350 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP24352	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24350 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP24353	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24350 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP24354	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24352 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP24355	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13830 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP24356	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24355 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP24357	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24355 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP24358	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24355 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP24359	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24357 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP24360	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13883 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP24361	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24360 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP24362	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24360 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP24363	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24360 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP24364	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24362 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP24365	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13381 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP24366	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24365 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP24367	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24365 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP24368	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24365 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP24369	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24367 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP24370	03/18/2025	09/18/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12949 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP24371	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 98.50000ml of W3177 + 0.50000ml of PP24329 + 1.00000ml of PP24370 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP24372	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24371 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP24373	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P13373 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1886	AR1221 500 PPB ICV	PP24374	03/18/2025	08/12/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of E3877 + 0.50000ml of W3177 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP24375	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P12699 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP24376	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24375 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP24377	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P13589 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP24378	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24377 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP24379	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P13591 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP24380	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24379 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP24381	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P12957 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP24382	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24381 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP24384	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P12702 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP24385	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24384 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP24386	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P11522 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP24387	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025
<u>FROM</u> 0.50000ml of W3177 + 0.50000ml of PP24386 = Final Quantity: 1.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	06/30/2025	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	08/25/2025	02/25/2025 / Rajesh	02/12/2025 / Rajesh	E3876

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	08/12/2025	02/12/2025 / Rajesh	02/12/2025 / Rajesh	E3877

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	10/03/2025	04/03/2025 / Rajesh	03/31/2025 / Rajesh	E3916

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	06/02/2025	06/01/2022 /	04/05/2022 / william	M5173

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	09/18/2025	03/18/2025 / yogesh	02/21/2022 / Ankita	P11522

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	09/18/2025	03/18/2025 / yogesh	08/07/2023 / Ankita	P12699

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	x9166 / Aroclor 1262 100 ug/mL	060523	09/18/2025	03/18/2025 / yogesh	08/07/2023 / Ankita	P12702

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	09/18/2025	03/18/2025 / yogesh	12/07/2023 / Ankita	P12931

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	09/18/2025	03/18/2025 / yogesh	12/07/2023 / Ankita	P12936

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	08/27/2025	02/27/2025 / Ankita	12/20/2023 / Yogesh	P12948

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	09/18/2025	03/18/2025 / yogesh	12/20/2023 / Yogesh	P12949

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/05/2025	03/05/2025 / Abdul	04/22/2024 / Abdul	P13354

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/18/2025	03/18/2025 / yogesh	04/22/2024 / Abdul	P13356

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	09/18/2025	03/18/2025 / yogesh	05/02/2024 / Ankita	P13373

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0207475	09/18/2025	03/18/2025 / yogesh	05/03/2024 / Abdul	P13381

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	09/18/2025	03/18/2025 / yogesh	10/14/2024 / Ankita	P13589

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006726317	09/18/2025	03/18/2025 / yogesh	10/14/2024 / Ankita	P13591

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0210629	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13697

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0215270	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13702

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0217391	09/18/2025	03/18/2025 / yogesh	12/09/2024 / Ankita	P13830

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0219655	09/18/2025	03/18/2025 / yogesh	01/23/2025 / Ankita	P13878

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0220950	09/18/2025	03/18/2025 / yogesh	01/23/2025 / Ankita	P13883

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1


Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865

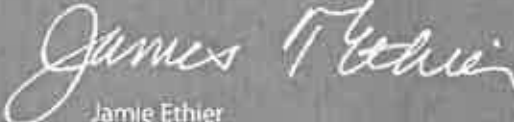
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Recd. by RP on 2/12/25

 E3877

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.

If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT - 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A

Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Harout Sahagian

Harout Sahagian - Quality Control Manager - Fair Lawn

Recd by RP on 3/31/25

E 3946

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.
 If there are any questions with this certificate, please call at (800) 227-6701.
 *Based on suggested storage condition.

Hydrochloric Acid, 36.5–38.0%
 BAKER INSTRA-ANALYZED® Reagent
 For Trace Metal Analysis



Material No.: 9530-33
 Batch No.: 0000281827
 Manufactured Date: 2021/03/30
 Retest Date: 2026/03/29
 Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
 Avantor Performance Materials, LLC
 100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality



Certificate of Analysis

P11518
↓
P11522
AJ
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isooctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026
Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration (µg/mL): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5µL, Range=3

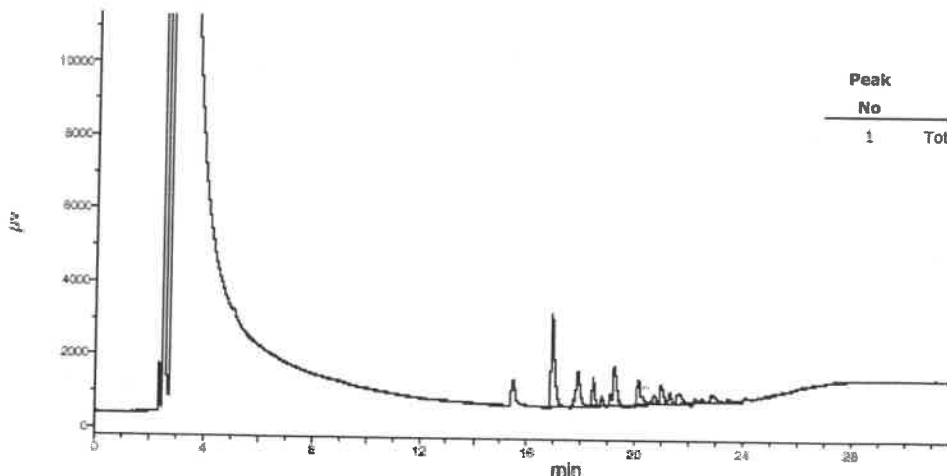




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32009 **Lot No.:** A0203672

Description: Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

p12928

→

p12932

AJ

12/27/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

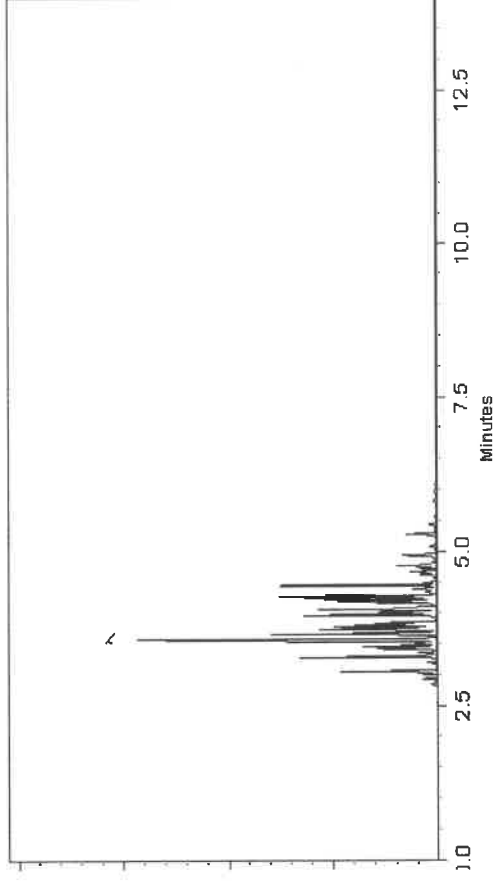

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boothamer

Russ Boothamer - Operations Technician I

Date Mixed: 26-Oct-2023

Balance Serial #

B442140311

Jennifer Polino

Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010 **Lot No.:** A0202803

Description: Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P1219697
P1219697
AF
12104123

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 µg/mL	+/- 55.5850

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

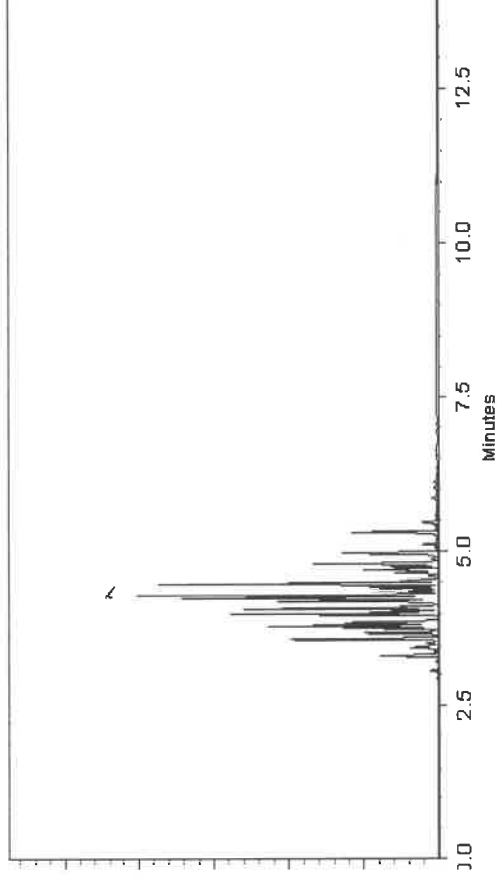

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 03-Oct-2023

Balance Serial # 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty


Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

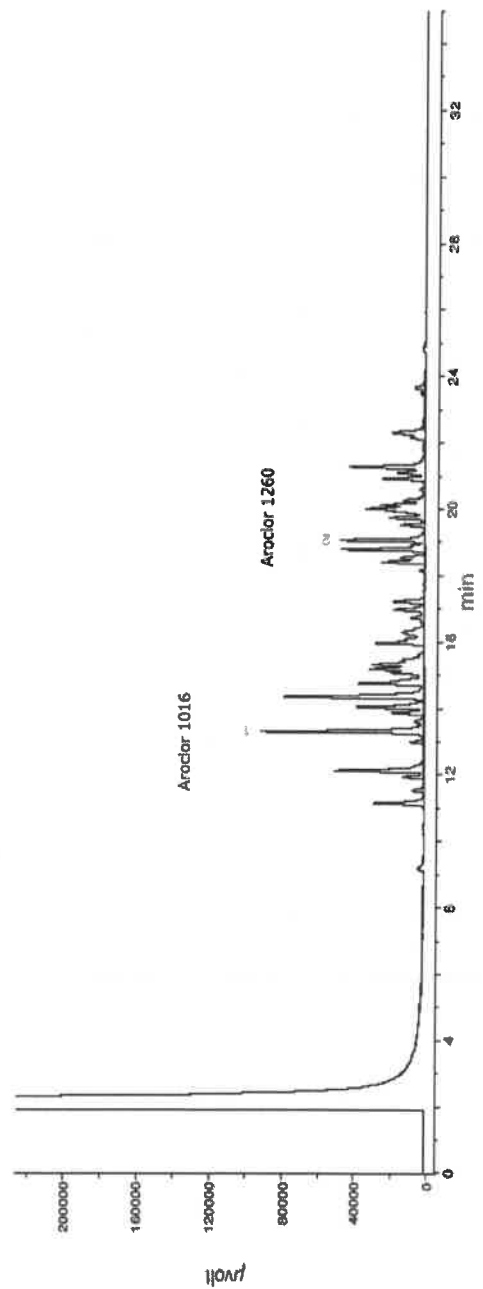



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number: 20084
Lot Number: 022023
Description: CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260
022033
Expiration Date: Ambient (20 °C)
Recommended Storage: 1000
Nominal Concentration (µg/mL): 6UTB
NIST Test ID#: 200.0

Solvent(s): Hexane
Lot#: 273615

Formulated By: Benson Chan
Reviewed By: Pedro L. Rentas

022023
DATE

022023
DATE


5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

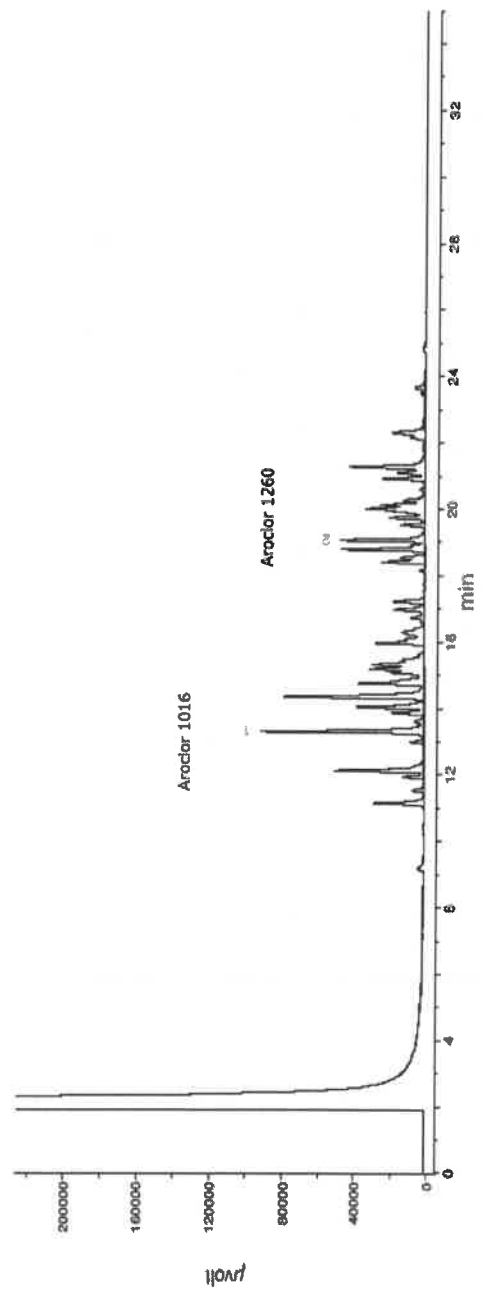



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

Solvent(s): Iso-octane
Lot#: 82227

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE


P12956 / Y.P.
12/18/23
P12957

Compound	Part Number	Lot Number	Dilution Factor	Initial Volume (mL)	Initial Uncertainty	Pipette (mL)	Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
											(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA) LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	0.017	1003.3	100.1	1.8	11097-69-1	0.5mg/m3 (skin)		or-rat 1295mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 280 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = EDAQ Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

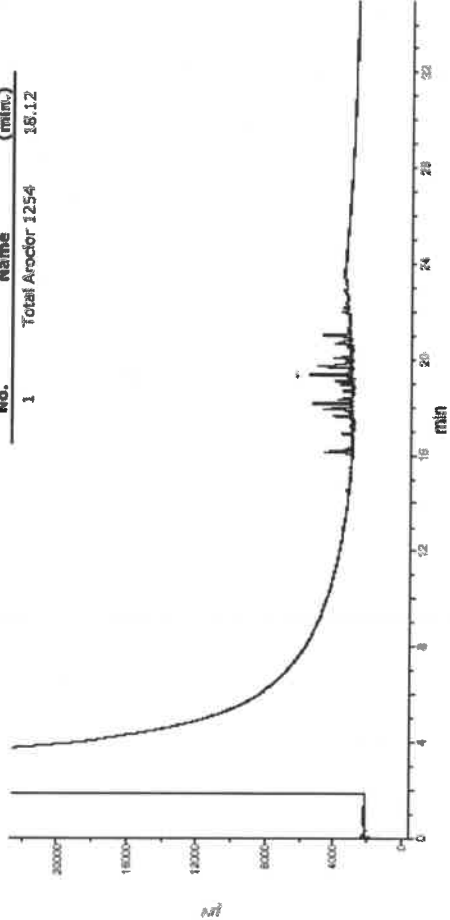



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

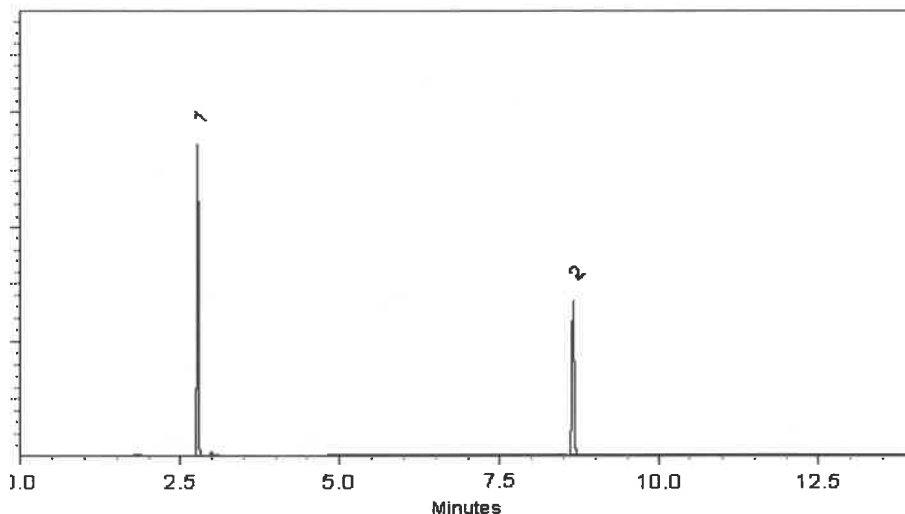


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
BAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

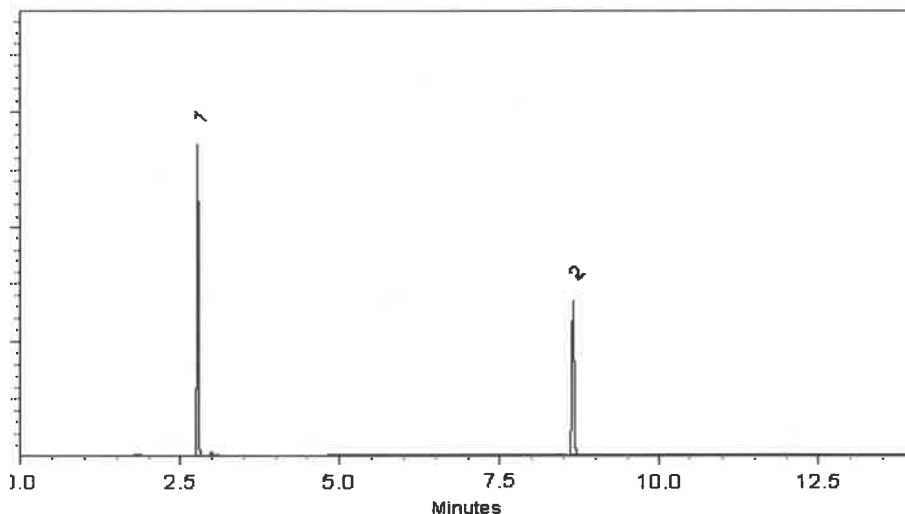


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name: Aroclor 1221 Standard
Product Number: PP-292-1
Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006783205
Lot Issue Date: 20-Feb-2024
Expiration Date: 31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ±	0.5 µg/mL	011104-28-2	NT01017

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342
AJ
05106124
P13343

Page: 1 of 2

CSD-QA-015.2

ISO 17025
Cert No. AT-1937


250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410 **Lot No.:** A0207475

Description : Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : May 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1268	11100-14-4	10947000	---%	1,000.0 µg/mL	+/- 55.4925

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 13380
↓
P 13381
↓
SAZU
05/6/2024

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

Split ratio 500:1

Inj. Vol

0.2µl

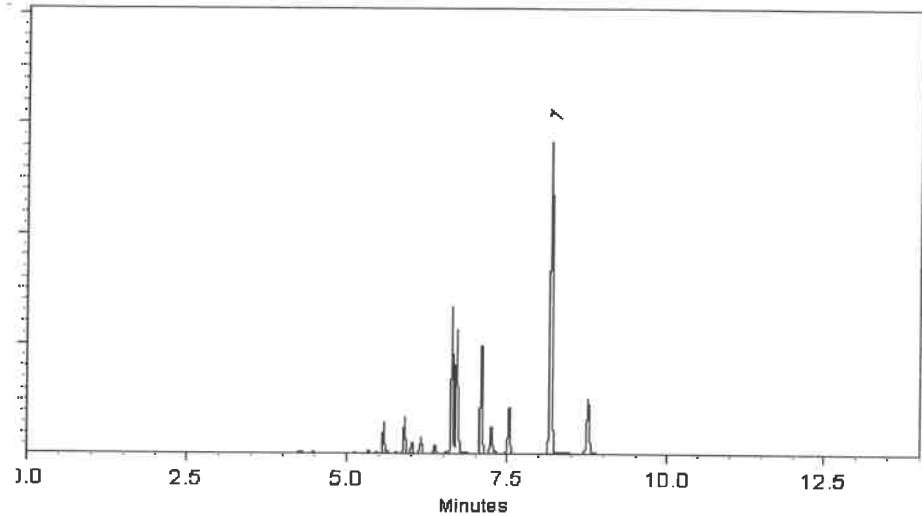

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 06-Feb-2024

Balance Serial # B442140311

Dylan Murphy
Dylan Murphy - Operations Technician I


Date Passed: 09-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P13380 } ②
↓
P13381
1

[Signature]
05/6/2024

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1242	100.4	± 0.5 µg/mL	053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13589
↓
P13590AJ
10/14/24

ISO 17034



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

Reference Material Certificate
Product Information Sheet

Product Name: Aroclor 1248 Standard

Lot Number: 0006726317

Product Number: PP-342-1

Lot Issue Date: 27-Jan-2023

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 28-Feb-2031

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1248	100.3 ±	0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material (RM) standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above. Purity values are taken from approved vendor raw material certificates.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference (RM) standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference (RM) standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard (RM) is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13591
↓
P13592

AS
10/14/2024



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1

ISO 17025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 **Lot No.:** A0210629

Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P13697
↓
P13701 } Y.P.
10/19/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1016	12674-11-2	07	----%	1,005.3 µg/mL	+/- 55.7809
2	Aroclor 1260	11096-82-5	1320657	----%	1,000.0 µg/mL	+/- 55.4850

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

0.2µl

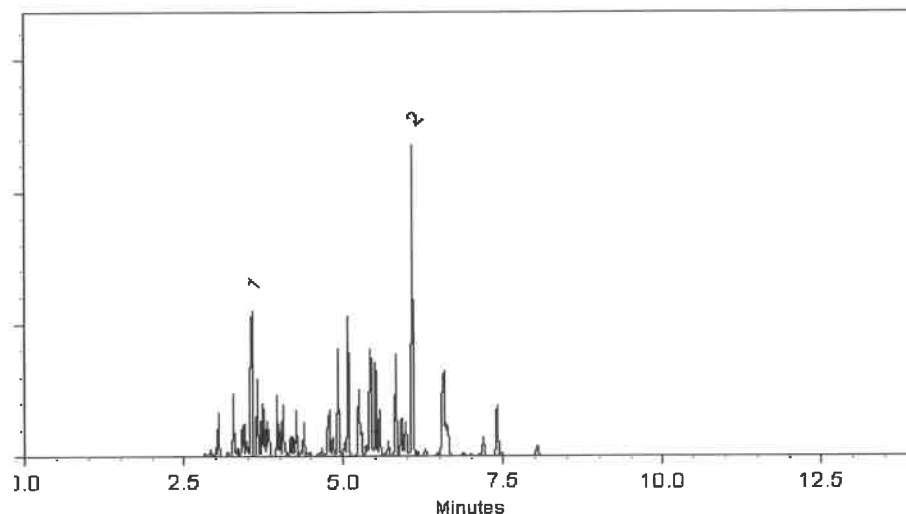


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Apr-2024

Balance Serial # B442140311


Dillan Murphy - Operations Technician I

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 **Lot No.:** A0215270

Description : Aroclor® 1221 Standard
Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P13902
P13703 } Y.P.
10/17/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1221	11104-28-2	14969200	----%	1,005.0 µg/mL	+/- 55.7700

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

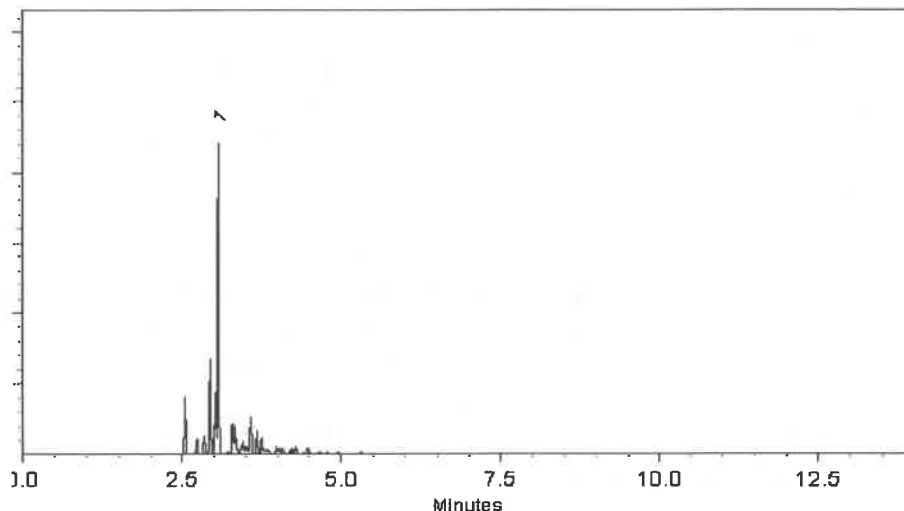

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 16-Aug-2024

Balance Serial # 1128360905

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 **Lot No.:** A0217391

Description : Aroclor® 1254 Standard

Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2031 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1254	11097-69-1	124-191-B	----%	1,004.7 µg/mL	+/- 55.7515

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P13830
↓
P13832
AJ
12/09/24

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

1µl

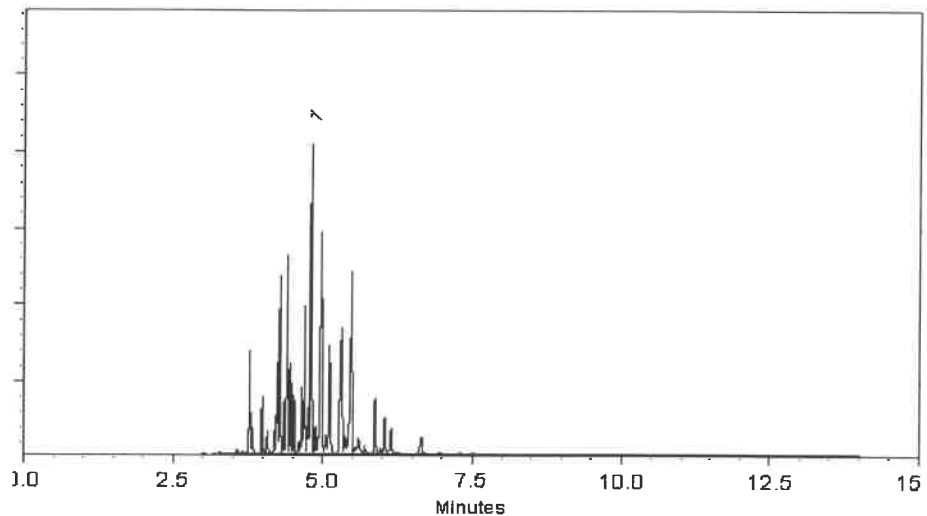

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 02-Oct-2024

Balance Serial # C322230531

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 07-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008 **Lot No.:** A0219655

Description : Aroclor® 1232 Standard

Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2031 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1232	11141-16-5	15665-01	---%	1,007.0 µg/mL	+/- 55.8810

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13878
↓
P13880

AJ
01/28/25

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

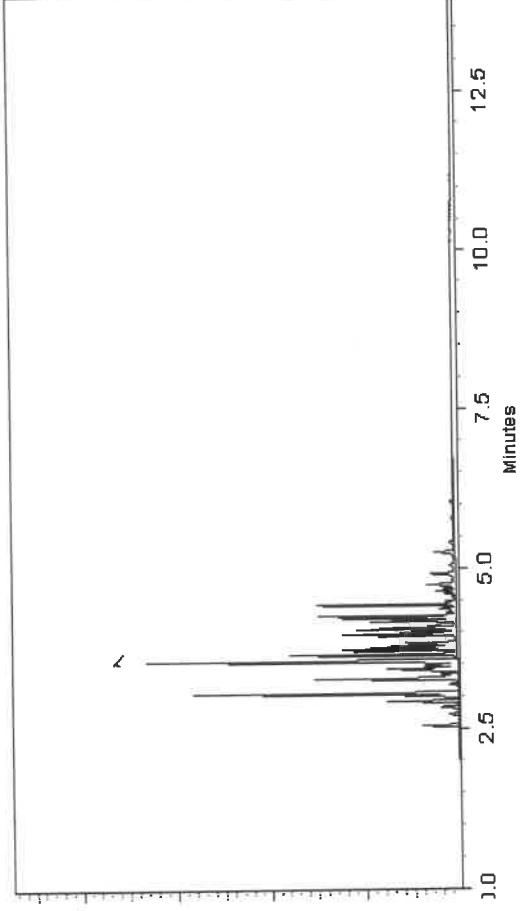

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 02-Dec-2024

Balance Serial #

C322230531

Brittany Federhik

Brittany Federhiko - Operations Tech I

Date Passed: 05-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32409 **Lot No.:** A0220950

Description: Aroclor® 1262 Standard

Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: April 30, 2031 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1262	37324-23-5	10849100	----%	1,002.0 µg/mL	+/- 55.6035

Solvent: Hexane

CAS # 110-54-3
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13882

↓

AJ
01/28/25

P13883

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

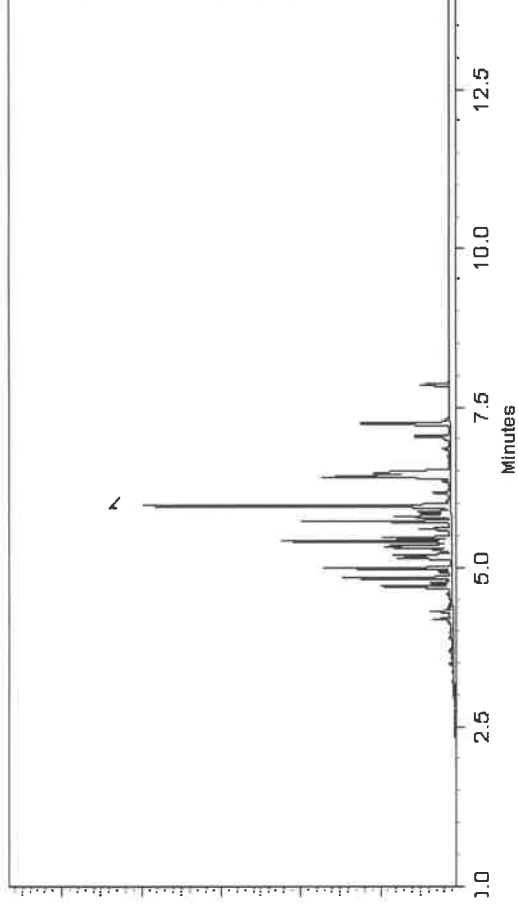

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckal - Mix Technician

Date Mixed: 09-Jan-2025 Balance Serial # C322230531



Britiany Federinko - Operations Tech I

Date Passed: 14-Jan-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak
Director Quality Operations, Bioscience Production



SHIPPING DOCUMENTS

CLIENT INFORMATION

COMPANY: Geop Inc
ADDRESS: 8 CARRIAGE
CITY: Juccasville STATE: NJ ZIP: 07876
ATTENTION:
PHONE: FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Stockton
PROJECT NO.: LOCATION: NJ
PROJECT MANAGER: GL
e-mail:
PHONE: 973 294 1771 FAX:

CLIENT BILLING INFORMATION

BILL TO: Geop Inc PO#:
ADDRESS: 8 CARRIAGE
CITY: Juccasville STATE: NJ ZIP: 07876
ATTENTION: PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) STANDARD DAYS*
HARDCOPY (DATA PACKAGE) DAYS*
EDD: DAYS*
*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☒ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data Excel
☒ EDD FORMAT MS Excel

PCB's
TRC Metals
EDH Cat 2
1,4 Dioxane

PRESERVATIVES

COMMENTS

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES										COMMENTS
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9	
1.	GST1	S01	X	X	4/4/25	1230	1	X	X	X	X						
2.	GST2	S01	X	X	4/4/25	1248	1	X	X	X	X						
3.																	
4.																	
5.																	
6.																	
7.																	
8.																	
9.																	
10.																	

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. <u>MA</u>	DATE/TIME: <u>4/4/25</u>	RECEIVED BY: 1. <u>[Signature]</u> <u>4/4/25</u> <u>1234</u>	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP <u>2.8</u> °C Comments: <u>(Adjust FACTOR H)</u> <u>IR gun #1</u>
RELINQUISHED BY SAMPLER: 2.	DATE/TIME:	RECEIVED BY: 2.	
RELINQUISHED BY SAMPLER: 3.	DATE/TIME:	RECEIVED BY: 3.	

Page ____ of CLIENT: ☐ Hand Delivered ☐ Other Shipment Complete ☐ YES ☐ NO

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488