
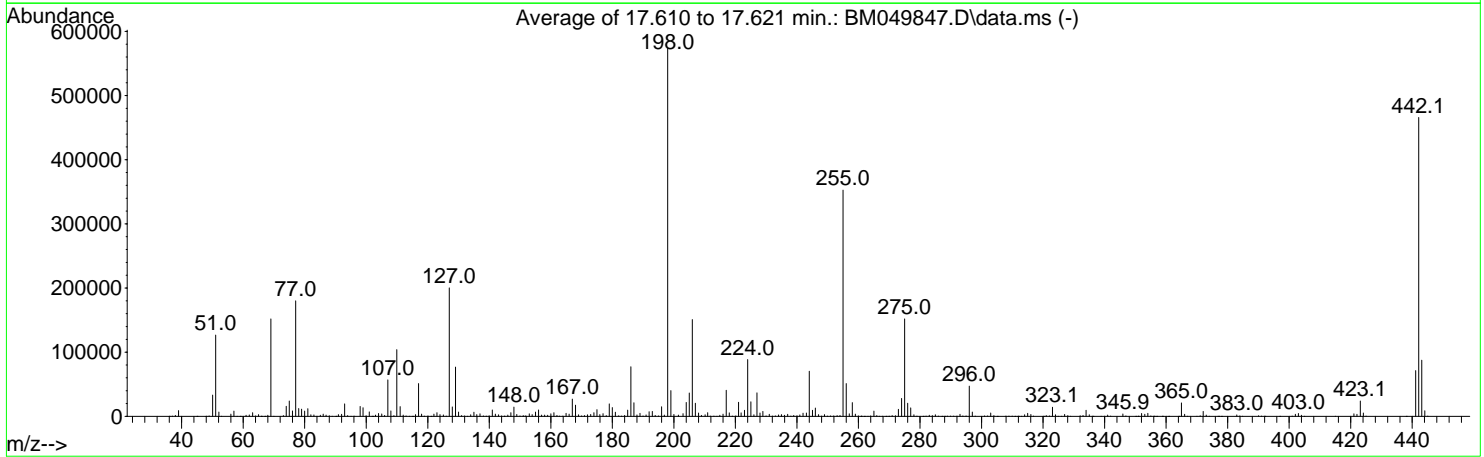


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040825\  
 Data File : BM049847.D  
 Acq On : 08 Apr 2025 12:55  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM040825.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Apr 09 04:00:55 2025

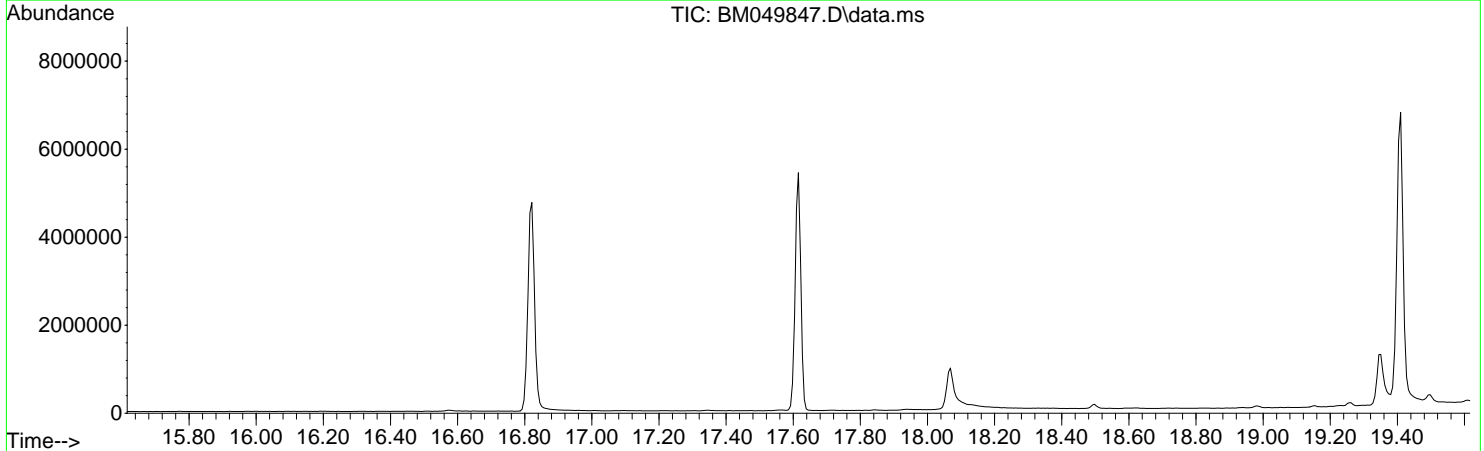




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.1	126723	PASS
68	69	0.00	2	1.2	1886	PASS
69	198	0.00	100	26.5	151989	PASS
70	69	0.00	2	0.3	382	PASS
127	198	10	80	34.9	200277	PASS
197	198	0.00	2	0.4	2141	PASS
198	198	100	100	100.0	573312	PASS
199	198	5	9	7.0	40037	PASS
275	198	10	60	26.5	151747	PASS
365	198	1	100	3.7	21032	PASS
441	198	0.01	100	12.4	71269	PASS
442	442	50	100	100.0	465813	PASS
443	442	15	24	18.8	87675	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040825\  
 Data File : BM049847.D  
 Acq On : 08 Apr 2025 12:55  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Apr 09 04:09:54 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM040825.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Apr 09 04:00:55 2025  
 Response via : Initial Calibration

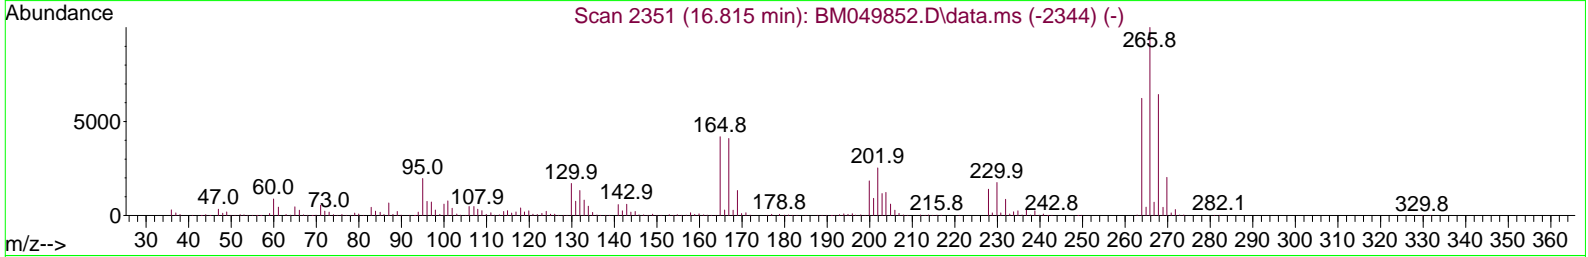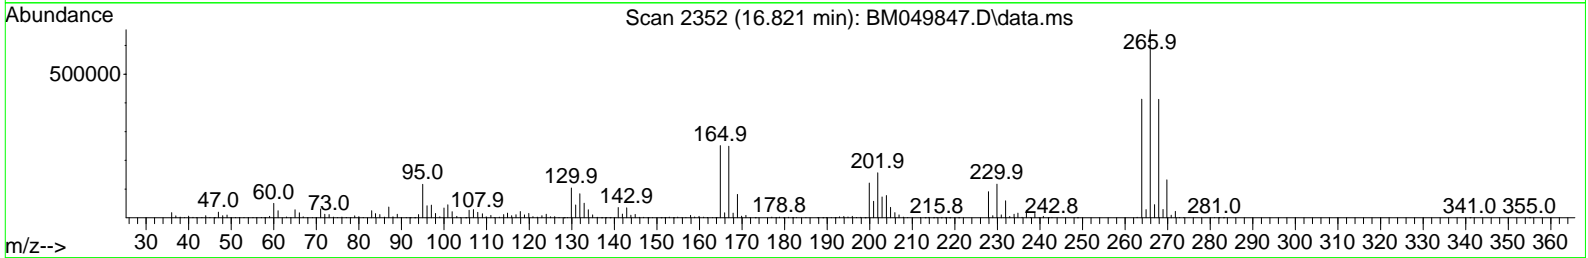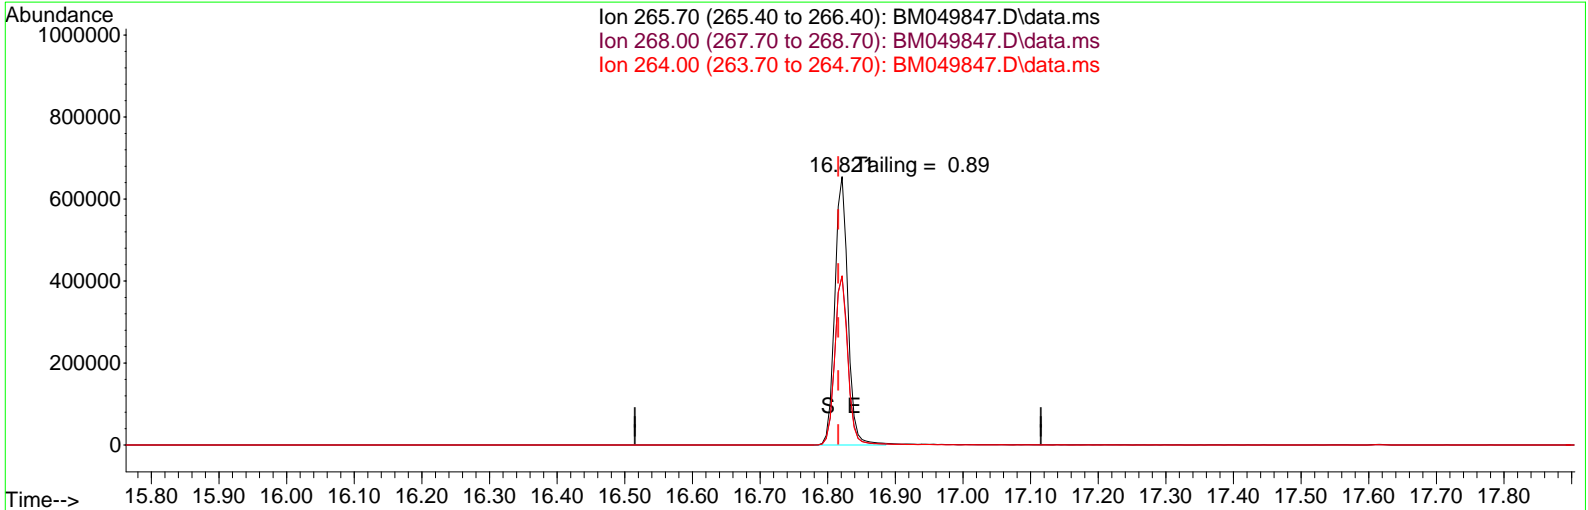

TIC: BM049847.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.006) 230006.58 ng m




response 888392

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	62.99
264.00	62.30	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM040825\  
 Data File : BM049847.D  
 Acq On : 08 Apr 2025 12:55  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Apr 09 04:09:54 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM040825.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Apr 09 04:00:55 2025  
 Response via : Initial Calibration

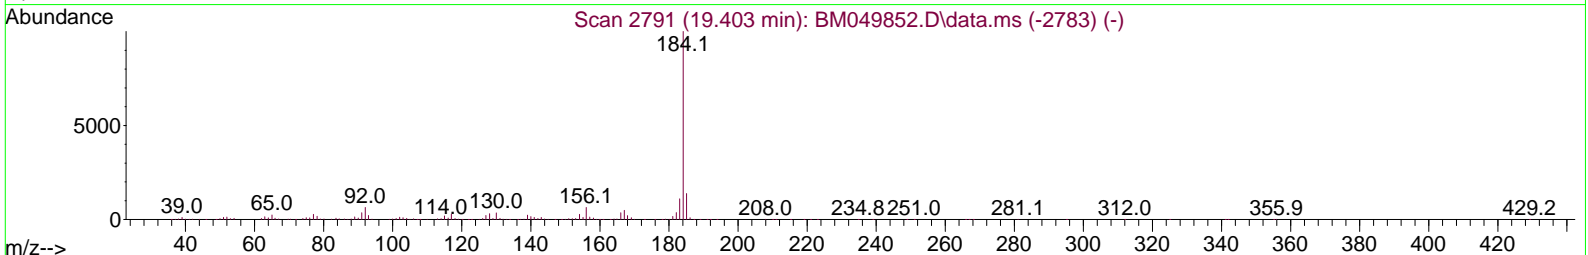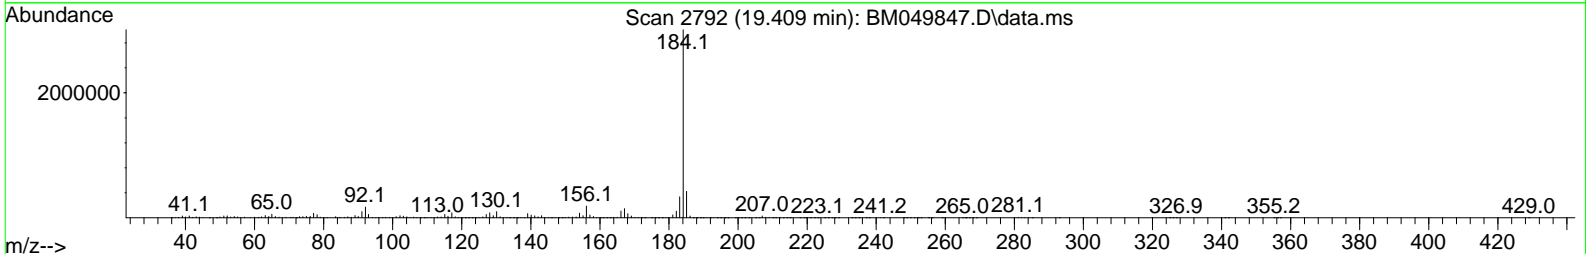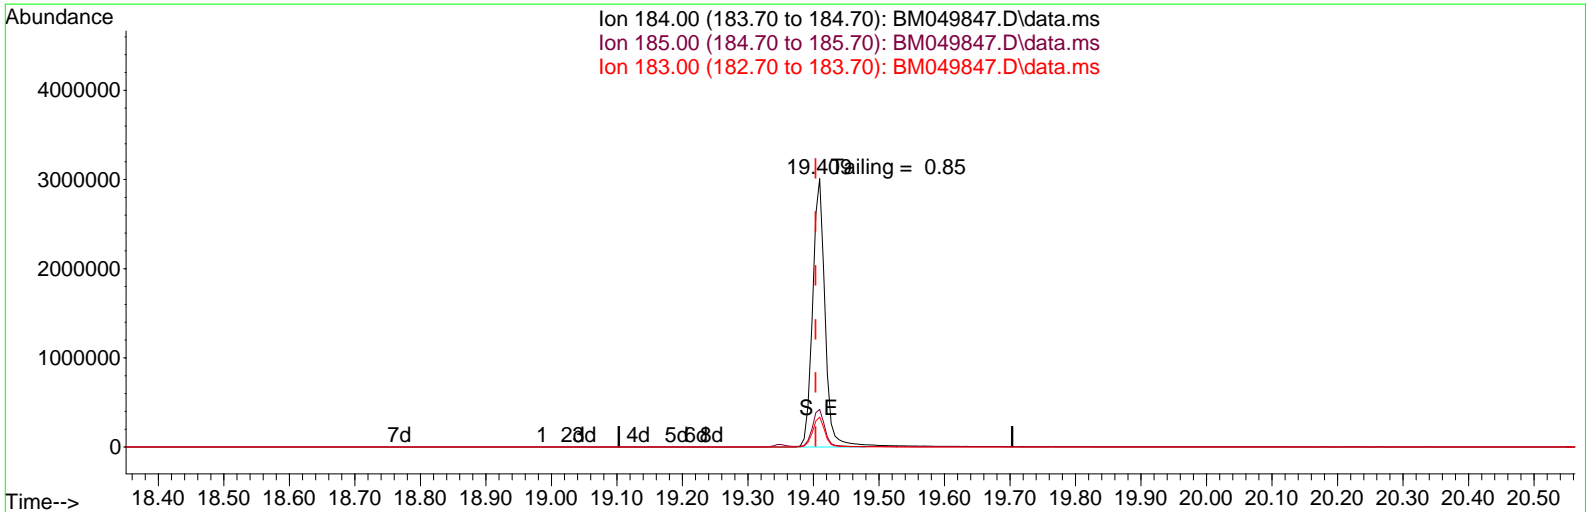

TIC: BM049847.D\data.ms

(77) Benzidine

19.409min (+ 0.006) 842986.98 ng m

response 4014847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.02
183.00	11.00	11.14
0.00	0.00	0.00

**DDT Breakdown**

Date	Instrument Name	DFTPP Data File
4/8/2025	BNA_M	<u>BM049847.D</u>
Compound Name	Response	Retention Time
DDT	1953764	20.645
DDD	24016	20.262
DDE	1854	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25870	1979634	1.31

Instrument :  
 BNA\_M  
 Client:Sampled :  
 DFTPP