
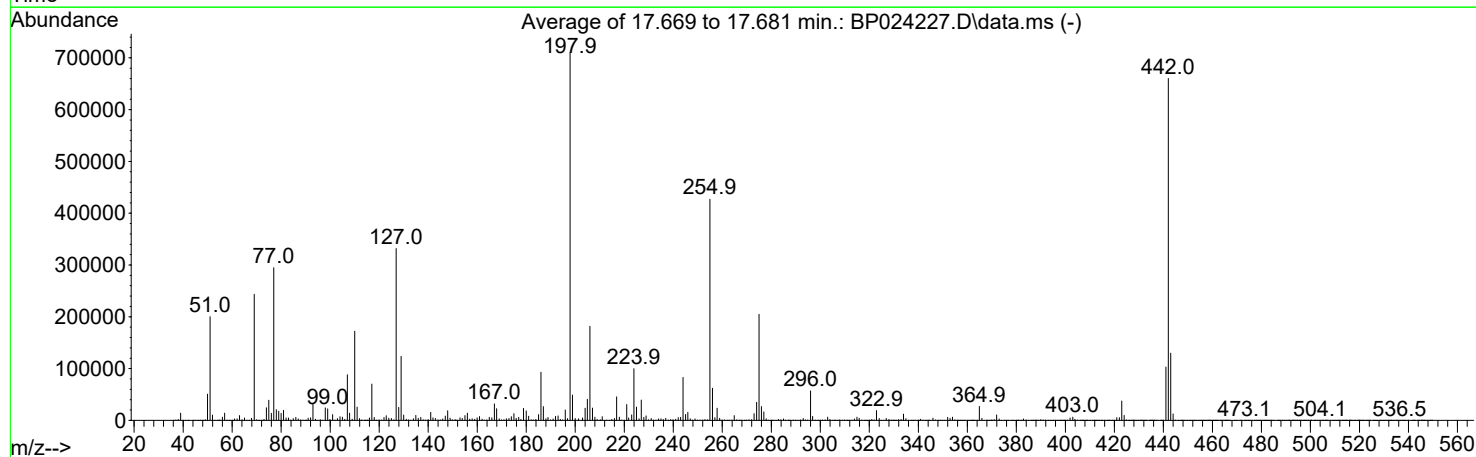


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP040925\  
Data File : BP024227.D  
Acq On : 09 Apr 2025 08:42  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031225.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Mar 13 05:55:58 2025

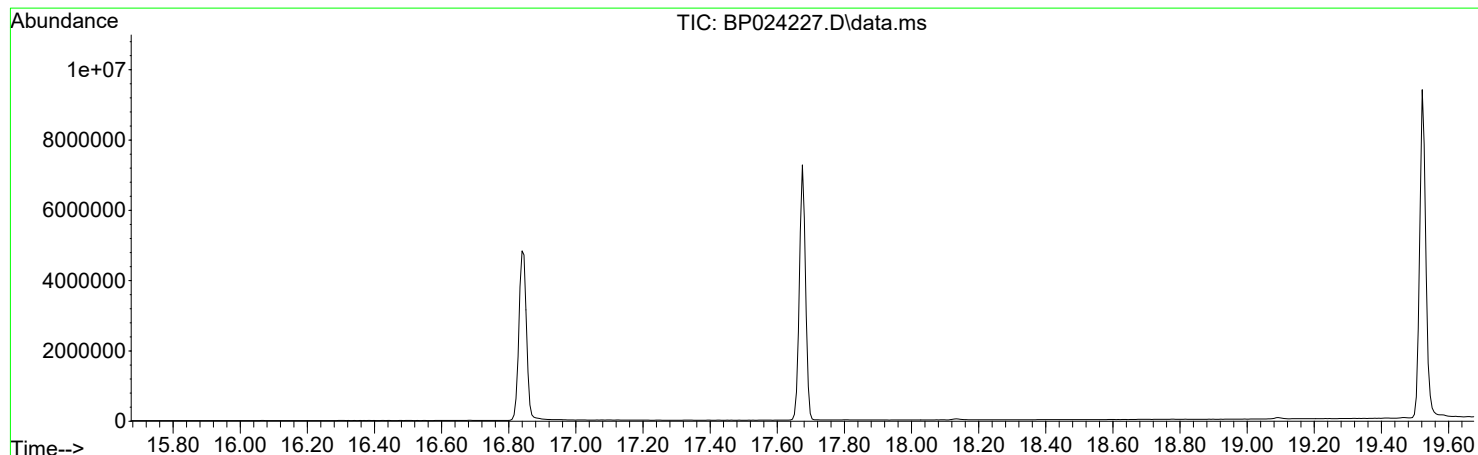

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2470

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 28.2      | 200115  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 3921    | PASS             |
| 69          | 198          | 0.00         | 100          | 34.3      | 243587  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 1251    | PASS             |
| 127         | 198          | 10           | 80           | 46.7      | 331923  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 3371    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 710336  | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 48868   | PASS             |
| 275         | 198          | 10           | 60           | 28.9      | 204948  | PASS             |
| 365         | 198          | 1            | 100          | 3.8       | 26873   | PASS             |
| 441         | 198          | 0.01         | 100          | 14.5      | 102902  | PASS             |
| 442         | 442          | 100          | 100          | 100.0     | 660181  | PASS             |
| 443         | 442          | 15           | 24           | 19.7      | 129757  | PASS             |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/9/2025      | BNA_P            | <u>BP024227.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 2570370          | 20.816             |
| DDD           | 50806            | 20.363             |
| DDE           | 1633             | 19.827             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 52439         | 2622809          | 2.00               |
|               |                  |                    |




Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP



Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP040925\  
Data File : BP024227.D  
Acq On : 09 Apr 2025 08:42  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Apr 09 12:31:59 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 13 05:55:58 2025  
Response via : Initial Calibration

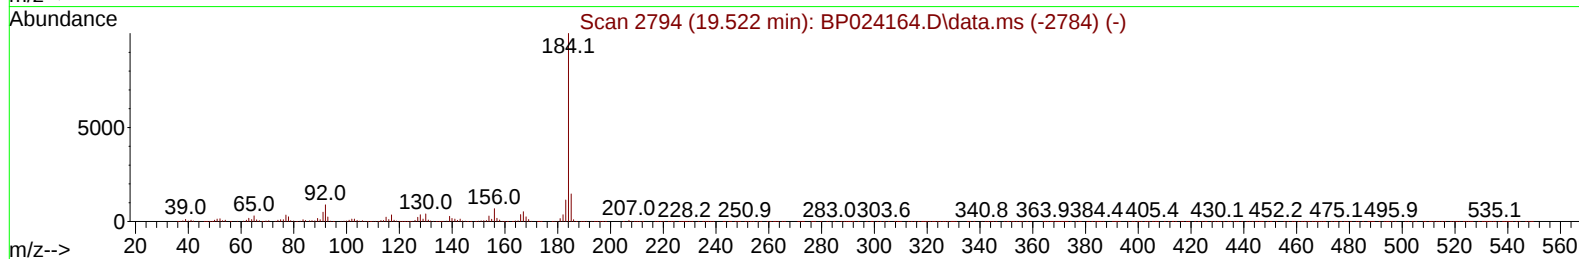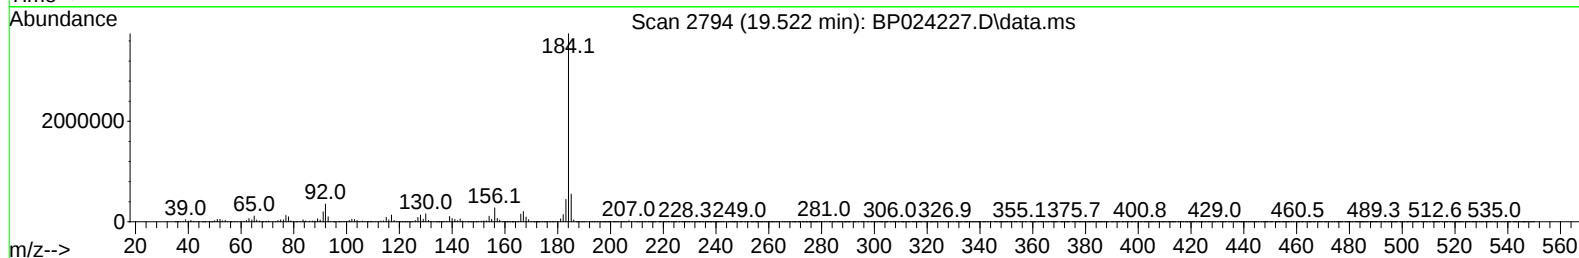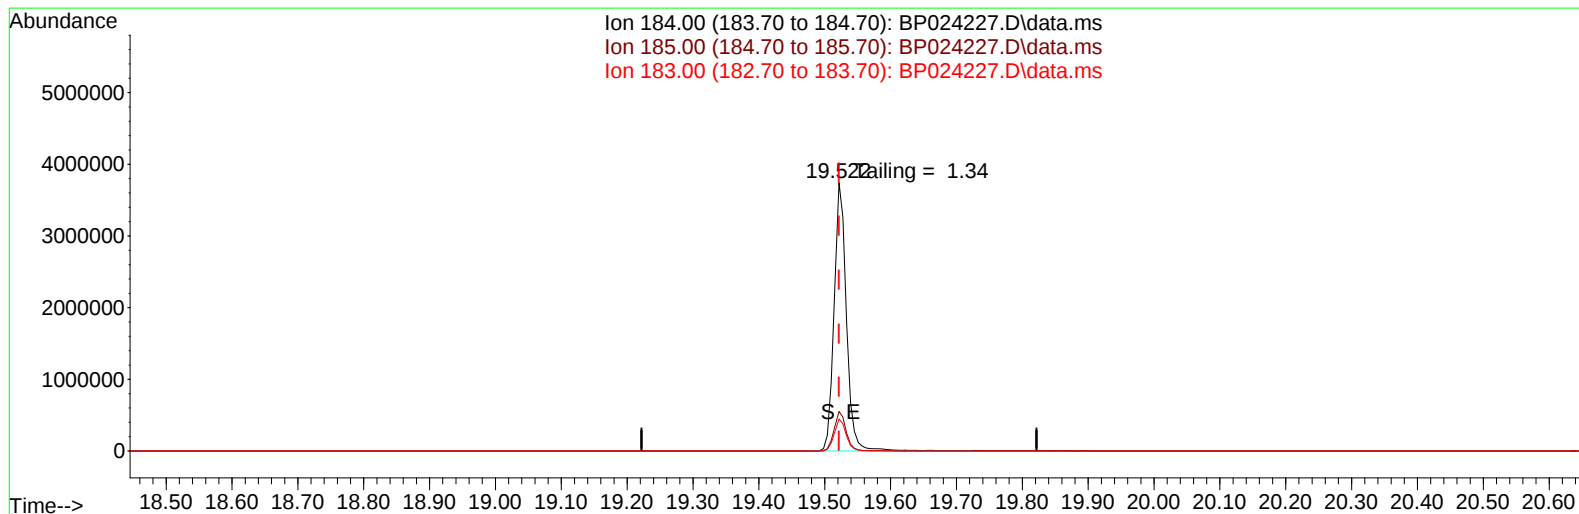

TIC: BP024227.D\data.ms

**(77) Benzidine**

**19.522min (-0.000) 108823.90 ng m**

**response 4912759**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 14.74  |
| 183.00 | 11.40  | 11.93  |
| 0.00   | 0.00   | 0.00   |