

DATA PACKAGE SEMI-VOLATILE ORGANICS

PROJECT NAME : FORMER SCHLUMBERGER STC PTC SITE D3868221

JACOBS ENGINEERING GROUP, INC.

412 Mt. Kemble Ave

Downtown Building

Morristown, NJ - 07960

Phone No: 9732670555

ORDER ID : Q1741

ATTENTION : John Ynfante



Laboratory Certification ID # 20012



1) SEMI-VOLATILE DATA	2
2) Signature Page	4
3) Case Narrative	5
4) Qualifier Page	7
5) Conformance/Non Conformance	8
6) QA Checklist	10
7) Chronicle	11
8) Hit Summary	12
9) QC Data Summary For SVOC-SIMGroup1	13
9.1) Deuterated Monitoring Compound Summary	14
9.2) LCS/LCSD Summary	15
9.3) Method Blank Summary	17
9.4) GS/MS Tune Summary	18
9.5) Internal Standard Area and RT Summary	21
10) Sample Data	25
10.1) RMW-02B-66-040425	26
10.2) RMW-02B-66-040425DL	38
10.3) RMW-06B-74-040425	49
10.4) FB01-040425	60
11) Calibration Data Summary	72
11.1) Initial Calibration Data	72
11.1.1) BN041125	72
11.1.2) BN041425	259
11.2) Continued Calibration Data	446
11.2.1) BN036884.D	446
12) QC Sample Data	472
12.1) Tune Raw Data	473
12.2) Method Blank Data	485
12.3) LCS Data	495
12.4) LCSD Data	519
13) Manual Integration	543
14) Analytical Runlogs	545
15) Extraction Logs	551
15.1) PB167519.pdf	551
15.2) PB167519IC.pdf	553

Table Of Contents for Q1741

16) Standard Prep Logs	554
17) Shipping Document	610
17.1) Chain Of Custody	611
17.2) Lab Certificate	612
17.3) Internal COC	613

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17

Cover Page

Order ID : Q1741

Project ID : Former Schlumberger STC PTC Site D3868221

Client : JACOBS Engineering Group, Inc.

Lab Sample Number

Q1741-01
Q1741-02
Q1741-03
Q1741-04

Client Sample Number

RMW-02B-66-040425
RMW-06B-74-040425
FB01-040425
TB01-040425

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature :

APPROVED

By Nimisha Pandya, QA/QC Supervisor at 12:00 pm, Apr 17, 2025

Date: 4/17/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

CASE NARRATIVE

JACOBS Engineering Group, Inc.

Project Name: Former Schlumberger STC PTC Site D3868221

Project # N/A

Chemtech Project # Q1741

Test Name: SVOC-SIMGroup1

A. Number of Samples and Date of Receipt:

4 Water samples were received on 04/04/2025.

B. Parameters

According to the Chain of Custody document, the following analyses were requested: SVOC-SIMGroup1 and VOCMS Group3. This data package contains results for SVOC-SIMGroup1.

C. Analytical Techniques:

The samples were analyzed on instrument BNA_N using GC Column ZB-SemiVolatiles Guardian which is 30 meters, 0.25 mm ID, 0.5 um df, Catalog # 7HG-G027-17-GGAThe analysis of SVOC-SIMGroup1 was based on method 8270-Modified and extraction was done based on method 3510.

D. QA/ QC Samples:

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria.

The Internal Standards Areas met the acceptable requirements except for PB167519BL
The above failure Internal standard not associated with the client parameters list,
therefore no corrective action was taken.

The Retention Times were acceptable for all samples.

The RPD met criteria .

The Blank Spike met requirements for all samples .

The Blank Spike Duplicate met requirements for all samples .

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements .

The Continuous Calibration met the requirements .

The Tuning criteria met requirements.

Sample RMW-02B-66-040425 was diluted due to high concentration.

E. Additional Comments:

The Form 6 is not included in the data package because the Initial Calibration was performed using 7 points.

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

F. Manual Integration Comments:

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature_____

APPROVED

By Nimisha Pandya, QA/QC Supervisor at 12:00 pm, Apr 17, 2025

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

GC/MS SEMI-VOLATILE ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY

CHEMTECH PROJECT NUMBER: Q1741

MATRIX: Water

METHOD: 8270-Modified/3510

		NA	NO	YES
1.	Chromatograms Labeled/Compounds Identified. (Field samples and Method Blanks)			✓
2.	GC/MS Tuning Specifications. DFTPP Meet Criteria. (NOTE THAT THERE ARE DIFFERENT CRITERIA FOR NY ASP CLP, CLP AND NJ)			✓
3.	GC/MS Tuning Frequency - Performed every 24 hours for 600 series and 12 hours for 8000 Series.			✓
4.	GC/MS Calibration - Initial Calibration performed within 30 days before sample analysis and continuing calibration performed within 24 hours of sample analysis for 600 series and 12 hours for 8000 serizes.			✓
5.	GC/MS Calibration Requirements.			✓
	The Initial Calibration met the requirements .			
	The Continuous Calibration met the requirements .			
6.	Blank Contamination - If yes, list compounds and concentrations in each blank:		✓	
7.	Surrogate Recoveries Meet Criteria		✓	
	If not met, list those compounds and their recoveries which fall outside the acceptable ranges.			
	The Surrogate recoveries met the acceptable criteria.			
8.	Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria			✓
	If not met, list those compounds and their recoveries which fall outside the acceptable range.			
	The Blank Spike met requirements for all samples .			
	The Blank Spike Duplicate met requirements for all samples .			
9.	Internal Standard Area/Retention Time Shift Meet Criteria			✓
	The Internal Standards Areas met the acceptable requirements except for PB167519BL The above failure Internal standard not associated with the client parameters list, therefore no corrective action was taken.			

Comments:

GC/MS SEMI-VOLATILE ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY
(CONTINUED)

		NA	NO	YES
10.	Extraction Holding Time Met			✓
	If not met, list number of days exceeded for each sample:			
11.	Analysis Holding Time Met			✓
	If not met, list number of days exceeded for each sample:			

ADDITIONAL COMMENTS:

Sample RMW-02B-66-040425 was diluted due to high concentration.

The Form 6 is not included in the data package because the Initial Calibration was performed using 7 points.

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is >20% for the Initial Calibration curve for SW-846 analysis.

QA REVIEW

REVIEWED
By Sohil Jodhani, QA/QC Director at 9:02 am, Apr 17, 2025

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q1741

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: SOHIL JODHANI

Date: 04/17/2025

LAB CHRONICLE

OrderID:	Q1741	OrderDate:	4/7/2025 10:06:00 AM
Client:	JACOBS Engineering Group, Inc.	Project:	Former Schlumberger STC PTC Site D3868221
Contact:	John Ynfante	Location:	L33,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1741-01	RMW-02B-66-040425	Water	SVOC-SIMGroup1	8270-Modified	04/04/25	04/08/25	04/11/25	04/04/25
Q1741-01DL	RMW-02B-66-040425 DL	Water			04/04/25			04/04/25
Q1741-02	RMW-06B-74-040425	Water	SVOC-SIMGroup1	8270-Modified	04/04/25	04/08/25	04/14/25	04/04/25
			SVOC-SIMGroup1	8270-Modified		04/08/25	04/11/25	
Q1741-03	FB01-040425	Water	SVOC-SIMGroup1	8270-Modified	04/04/25	04/08/25	04/11/25	04/04/25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet SW-846

SDG No.: Q1741

Client: JACOBS Engineering Group, Inc.

Sample ID	Client ID	Parameter	Concentration	C	MDL	RDL	Units
Client ID :	RMW-02B-66-040425						
Q1741-01	RMW-02B-66-040425	WATER	1,4-Dioxane	30.700	E 0.07	0.21	ug/L
			Total Svoc :	30.70			
			Total Concentration:	30.70			
Client ID :	RMW-02B-66-040425DL						
Q1741-01DL	RMW-02B-66-040425DL	WATER	1,4-Dioxane	31.200	D 0.71	2.1	ug/L
			Total Svoc :	31.20			
			Total Concentration:	31.20			



QC SUMMARY

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

Surrogate Summary

SW-846

SDG No.: Q1741

Client: JACOBS Engineering Group, Inc.

Analytical Method: 8270-Modified

Lab Sample ID	Client ID	Parameter	Spike (PPM)	Result (PPM)	Recovery (%)	Qual	Limits (%)	
							Low	High
PB167519BL	PB167519BL	2-Methylnaphthalene-d10	0.4	0.34	85		30 (20)	150 (139)
		Fluoranthene-d10	0.4	0.35	88		30 (30)	150 (150)
		Nitrobenzene-d5	0.4	0.32	80		30 (27)	130 (154)
		2-Fluorobiphenyl	0.4	0.37	93		30 (25)	130 (149)
		Terphenyl-d14	0.4	0.42	104		30 (54)	130 (175)
PB167519BS	PB167519BS	2-Methylnaphthalene-d10	0.4	0.39	98		30 (20)	150 (139)
		Fluoranthene-d10	0.4	0.41	101		30 (30)	150 (150)
		Nitrobenzene-d5	0.4	0.36	90		30 (27)	130 (154)
		2-Fluorobiphenyl	0.4	0.39	97		30 (25)	130 (149)
		Terphenyl-d14	0.4	0.37	94		30 (54)	130 (175)
PB167519BSD	PB167519BSD	2-Methylnaphthalene-d10	0.4	0.40	100		30 (20)	150 (139)
		Fluoranthene-d10	0.4	0.42	105		30 (30)	150 (150)
		Nitrobenzene-d5	0.4	0.34	86		30 (27)	130 (154)
		2-Fluorobiphenyl	0.4	0.40	101		30 (25)	130 (149)
		Terphenyl-d14	0.4	0.38	96		30 (54)	130 (175)
Q1741-01	RMW-02B-66-040425	2-Methylnaphthalene-d10	0.4	0.34	85		30 (20)	150 (139)
		Fluoranthene-d10	0.4	0.41	103		30 (30)	150 (150)
		Nitrobenzene-d5	0.4	0.35	88		30 (27)	130 (154)
		2-Fluorobiphenyl	0.4	0.38	95		30 (25)	130 (149)
		Terphenyl-d14	0.4	0.43	107		30 (54)	130 (175)
Q1741-01DL	RMW-02B-66-040425DL	2-Methylnaphthalene-d10	0.4	0.33	83		30 (20)	150 (139)
		Fluoranthene-d10	0.4	0.42	105		30 (30)	150 (150)
		Nitrobenzene-d5	0.4	0.31	77		30 (27)	130 (154)
		2-Fluorobiphenyl	0.4	0.38	95		30 (25)	130 (149)
		Terphenyl-d14	0.4	0.48	120		30 (54)	130 (175)
Q1741-02	RMW-06B-74-040425	2-Methylnaphthalene-d10	0.4	0.35	86		30 (20)	150 (139)
		Fluoranthene-d10	0.4	0.41	102		30 (30)	150 (150)
		Nitrobenzene-d5	0.4	0.33	82		30 (27)	130 (154)
		2-Fluorobiphenyl	0.4	0.34	86		30 (25)	130 (149)
		Terphenyl-d14	0.4	0.42	104		30 (54)	130 (175)
Q1741-03	FB01-040425	2-Methylnaphthalene-d10	0.4	0.31	76		30 (20)	150 (139)
		Fluoranthene-d10	0.4	0.41	103		30 (30)	150 (150)
		Nitrobenzene-d5	0.4	0.30	74		30 (27)	130 (154)
		2-Fluorobiphenyl	0.4	0.36	91		30 (25)	130 (149)
		Terphenyl-d14	0.4	0.52	129		30 (54)	130 (175)

() = LABORATORY INHOUSE LIMIT

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q1741

Client: JACOBS Engineering Group, Inc.

Analytical Method: 8270-Modified DataFile: BN036893.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	RPD	Limits		RPD
								Qual	Low	High	
PB167519BS	1,4-Dioxane	0.4	0.34	ug/L	85				20 (42)	160 (127)	

() = LABORATORY INHOUSE LIMIT

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q1741

Client: JACOBS Engineering Group, Inc.

Analytical Method: 8270-Modified DataFile: BN036894.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	RPD	Limits		RPD
								Qual	Low	High	
PB167519BSD	1,4-Dioxane	0.4	0.39	ug/L	98	14			20 (42)	160 (127)	20 (20)

() = LABORATORY INHOUSE LIMIT

4B

SEMIVOLATILE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB167519BL

Lab Name: CHEMTECH

Contract: JAC005

Lab Code: CHEM Case No.: Q1741

SAS No.: Q1741 SDG NO.: Q1741

Lab File ID: BN036906.D

Lab Sample ID: PB167519BL

Instrument ID: BNA_N

Date Extracted: 04/08/2025

Matrix: (soil/water) Water

Date Analyzed: 04/14/2025

Level: (low/med) LOW

Time Analyzed: 18:51

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
PB167519BS	PB167519BS	BN036893.D	04/12/2025
PB167519BSD	PB167519BSD	BN036894.D	04/12/2025
RMW-02B-66-040425	Q1741-01	BN036886.D	04/11/2025
RMW-06B-74-040425	Q1741-02	BN036887.D	04/11/2025
FB01-040425	Q1741-03	BN036888.D	04/11/2025

COMMENTS: _____



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

5B

SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: CHEMTECHContract: JACO05Lab Code: CHEMSAS No.: Q1741SDG NO.: Q1741Lab File ID: BN036872.DDFTPP Injection Date: 04/11/2025Instrument ID: BNA_NDFTPP Injection Time: 11:03

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
51	10.0 - 80.0% of mass 198	64.6
68	Less than 2.0% of mass 69	0.9 (1.6) 1
69	Mass 69 relative abundance	54
70	Less than 2.0% of mass 69	0.0 (0.0) 1
127	10.0 - 80.0% of mass 198	50.2
197	Less than 2.0% of mass 198	0.0
198	Base Peak, 100% relative abundance	100
199	5.0 to 9.0% of mass 198	6.4
275	10.0 - 60.0% of mass 198	25.4
365	Greater than 1% of mass 198	3.9
441	Present, but less than mass 443	10.8
442	Greater than 50% of mass 198	100.0
443	15.0 - 24.0% of mass 442	11.3 (21.3) 2

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
SSTDICC0.1	SSTDICC0.1	BN036873.D	04/11/2025	11:42
SSTDICC0.2	SSTDICC0.2	BN036874.D	04/11/2025	12:37
SSTDICCC0.4	SSTDICCC0.4	BN036875.D	04/11/2025	13:17
SSTDICC0.8	SSTDICC0.8	BN036876.D	04/11/2025	13:53
SSTDICC1.6	SSTDICC1.6	BN036877.D	04/11/2025	14:30
SSTDICC3.2	SSTDICC3.2	BN036878.D	04/11/2025	15:06
SSTDICC5.0	SSTDICC5.0	BN036879.D	04/11/2025	15:42



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

5B

SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: CHEMTECHContract: JACO05Lab Code: CHEMSAS No.: Q1741 SDG NO.: Q1741Lab File ID: BN036883.DDFTPP Injection Date: 04/11/2025Instrument ID: BNA_NDFTPP Injection Time: 18:06

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
51	10.0 - 80.0% of mass 198	68.5
68	Less than 2.0% of mass 69	0.5 (0.9) 1
69	Mass 69 relative abundance	55.2
70	Less than 2.0% of mass 69	0.0 (0.0) 1
127	10.0 - 80.0% of mass 198	53.5
197	Less than 2.0% of mass 198	0.0
198	Base Peak, 100% relative abundance	100
199	5.0 to 9.0% of mass 198	6.5
275	10.0 - 60.0% of mass 198	21.7
365	Greater than 1% of mass 198	2.5
441	Present, but less than mass 443	10.2
442	Greater than 50% of mass 198	100.0
443	15.0 - 24.0% of mass 442	10.9 (19.6) 2

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
SSTDCCC0.4	SSTDCCC0.4	BN036884.D	04/11/2025	18:45
RMW-02B-66-040425	Q1741-01	BN036886.D	04/11/2025	19:57
RMW-06B-74-040425	Q1741-02	BN036887.D	04/11/2025	20:34
FB01-040425	Q1741-03	BN036888.D	04/11/2025	21:10
PB167519BS	PB167519BS	BN036893.D	04/12/2025	00:09
PB167519BSD	PB167519BSD	BN036894.D	04/12/2025	00:45



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

5B

SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: CHEMTECHContract: JAC005Lab Code: CHEMSAS No.: Q1741 SDG NO.: Q1741Lab File ID: BN036896.DDFTPP Injection Date: 04/14/2025Instrument ID: BNA_NDFTPP Injection Time: 10:10

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
51	10.0 - 80.0% of mass 198	72.9
68	Less than 2.0% of mass 69	0.3 (0.6) 1
69	Mass 69 relative abundance	59.2
70	Less than 2.0% of mass 69	0.3 (0.5) 1
127	10.0 - 80.0% of mass 198	56.2
197	Less than 2.0% of mass 198	0.0
198	Base Peak, 100% relative abundance	100
199	5.0 to 9.0% of mass 198	6.8
275	10.0 - 60.0% of mass 198	24.4
365	Greater than 1% of mass 198	4.2
441	Present, but less than mass 443	8.5
442	Greater than 50% of mass 198	100.0
443	15.0 - 24.0% of mass 442	10 (18.5) 2

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
SSTDICC0.1	SSTDICC0.1	BN036898.D	04/14/2025	13:26
SSTDICC0.2	SSTDICC0.2	BN036899.D	04/14/2025	14:02
SSTDICCC0.4	SSTDICCC0.4	BN036900.D	04/14/2025	14:38
SSTDICC0.8	SSTDICC0.8	BN036901.D	04/14/2025	15:15
SSTDICC1.6	SSTDICC1.6	BN036902.D	04/14/2025	15:51
SSTDICC3.2	SSTDICC3.2	BN036903.D	04/14/2025	16:27
SSTDICC5.0	SSTDICC5.0	BN036904.D	04/14/2025	17:03
PB167519BL	PB167519BL	BN036906.D	04/14/2025	18:51
RMW-02B-66-040425DL	Q1741-01DL	BN036908.D	04/14/2025	20:04

8B

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH

Lab Code: CHEM Case No.: Q1741 SAS No.: Q1741 SDG NO.: Q1741

EPA Sample No.: SSTDCCC0.4 Date Analyzed: 04/11/2025

Lab File ID: BN036884.D Time Analyzed: 18:45

Instrument ID: BNA_N GC Column: ZB-GR ID: 0.25 (mm)

	IS1 (DCB) AREA #	RT #	IS2 (NPT) AREA #	RT #	IS3 (ANT) AREA #	RT #
12 HOUR STD	254	7.64	679	10.43	407	14.29
UPPER LIMIT	508	8.14	1358	10.925	814	14.788
LOWER LIMIT	127	7.14	339.5	9.925	203.5	13.788
EPA SAMPLE NO.						
01 PB167519BS	385	7.64	924	10.43	537	14.29
02 PB167519BSD	195	7.64	480	10.43	292	14.29
03 RMW-02B-66-040425	274	7.64	725	10.43	456	14.29
04 RMW-06B-74-040425	257	7.64	678	10.43	429	14.29
05 FB01-040425	267	7.64	721	10.43	449	14.29

IS1 (DCB) = 1,4-Dichlorobenzene-d4

IS2 (NPT) = Naphthalene-d8

IS3 (ANT) = Acenaphthene-d10

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT UPPER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.

8C

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH

Lab Code: CHEM Case No.: Q1741 SAS No.: Q1741 SDG NO.: Q1741

EPA Sample No.: SSTDCCC0.4 Date Analyzed: 04/11/2025

Lab File ID: BN036884.D Time Analyzed: 18:45

Instrument ID: BNA_N GC Column: ZB-GR ID: 0.25 (mm)

	IS4 (PHN) AREA #	RT #	IS5 (CRY) AREA #	RT #	IS6 (PRY) AREA #	RT #
12 HOUR STD	865	17.033	1015	21.233	1369	23.447
UPPER LIMIT	1730	17.533	2030	21.733	2738	23.947
LOWER LIMIT	432.5	16.533	507.5	20.733	684.5	22.947
EPA SAMPLE NO.						
01 PB167519BS	1271	17.03	1512	21.22	1791	23.45
02 PB167519BSD	662	17.03	805	21.22	1051	23.44
03 RMW-02B-66-040425	993	17.03	1080	21.23	1296	23.45
04 RMW-06B-74-040425	971	17.03	1082	21.23	1366	23.45
05 FB01-040425	971	17.03	1105	21.23	1316	23.45

IS4 (PHN) = Phenanthrene-d10

IS5 (CRY) = Chrysene-d12

IS6 (PRY) = Perylene-d12

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT UPPER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.

8B

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH

Lab Code: CHEM Case No.: Q1741 SAS No.: Q1741 SDG NO.: Q1741

EPA Sample No.: SSTDICCC0.4 Date Analyzed: 04/14/2025

Lab File ID: BN036900.D Time Analyzed: 14:38

Instrument ID: BNA_N GC Column: ZB-GR ID: 0.25 (mm)

	IS1 (DCB) AREA #	RT #	IS2 (NPT) AREA #	RT #	IS3 (ANT) AREA #	RT #
12 HOUR STD	1387	7.633	3400	10.42	1899	14.28
UPPER LIMIT	2774	8.133	6800	10.915	3798	14.777
LOWER LIMIT	693.5	7.133	1700	9.915	949.5	13.777
EPA SAMPLE NO.						
01 PB167519BL	1898	7.63	4409	10.42	2284	14.28
02 RMW-02B-66-040425DL	1215	7.63	2952	10.42	1740	14.28

IS1 (DCB) = 1,4-Dichlorobenzene-d4

IS2 (NPT) = Naphthalene-d8

IS3 (ANT) = Acenaphthene-d10

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT UPPER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.

8C

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH

Lab Code: CHEM Case No.: Q1741 SAS No.: Q1741 SDG NO.: Q1741

EPA Sample No.: SSTDICCC0.4 Date Analyzed: 04/14/2025

Lab File ID: BN036900.D Time Analyzed: 14:38

Instrument ID: BNA_N GC Column: ZB-GR ID: 0.25 (mm)

	IS4 (PHN) AREA #	RT #	IS5 (CRY) AREA #	RT #	IS6 (PRY) AREA #	RT #
12 HOUR STD	3763	17.033	3219	21.224	3042	23.433
UPPER LIMIT	7526	17.533	6438	21.724	6084	23.933
LOWER LIMIT	1881.5	16.533	1609.5	20.724	1521	22.933
EPA SAMPLE NO.						
01 PB167519BL	4447	17.03	3070	21.23	1383 *	23.44
02 RMW-02B-66-040425DL	3461	17.03	2948	21.22	2817	23.43

IS4 (PHN) = Phenanthrene-d10

IS5 (CRY) = Chrysene-d12

IS6 (PRY) = Perylene-d12

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT UPPER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.



SAMPLE DATA

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	04/04/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	04/04/25
Client Sample ID:	RMW-02B-66-040425	SDG No.:	Q1741
Lab Sample ID:	Q1741-01	Matrix:	Water
Analytical Method:	SW8270ESIM	% Solid:	0
Sample Wt/Vol:	970 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	SVOC-SIMGroup1
Extraction Type :	Decanted : N	Level :	LOW
Injection Volume :	GPC Factor : 1.0	GPC Cleanup :	N PH :
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN036886.D	1	04/08/25 10:10	04/11/25 19:57	PB167519

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
123-91-1	1,4-Dioxane	30.7	E	0.070	0.21	ug/L
SURROGATES						
7297-45-2	2-Methylnaphthalene-d10	0.34		30 (20) - 150 (139)	85%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.41		30 (30) - 150 (150)	103%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.35		30 (27) - 130 (154)	88%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.38		30 (25) - 130 (149)	95%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.43		30 (54) - 130 (175)	107%	SPK: 0.4
INTERNAL STANDARDS						
3855-82-1	1,4-Dichlorobenzene-d4	274		7.64		
1146-65-2	Naphthalene-d8	725		10.426		
15067-26-2	Acenaphthene-d10	456		14.288		
1517-22-2	Phenanthrene-d10	993		17.033		
1719-03-5	Chrysene-d12	1080		21.233		
1520-96-3	Perylene-d12	1300		23.447		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036886.D
Acq On : 11 Apr 2025 19:57
Operator : RC/JU
Sample : Q1741-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425

Quant Time: Apr 11 23:06:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	274	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	725	0.400	ng	# 0.00
13) Acenaphthene-d10	14.288	164	456	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	993	0.400	ng	0.00
29) Chrysene-d12	21.233	240	1080	0.400	ng	0.00
35) Perylene-d12	23.447	264	1296	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.235	112	126m	0.195	ng	0.00
5) Phenol-d6	6.824	99	86	0.104	ng	0.00
8) Nitrobenzene-d5	8.792	82	283	0.352	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	358	0.340	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	98	0.446	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	832	0.380	ng	0.00
27) Fluoranthene-d10	19.073	212	1156	0.413	ng	0.00
31) Terphenyl-d14	19.676	244	881	0.429	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.148	88	9469m	29.808	ng	Qvalue
25) Phenanthrene	17.083	178	84	0.028	ng	# 53
34) Bis(2-ethylhexyl)phtha...	21.153	149	245	0.087	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036886.D
Acq On : 11 Apr 2025 19:57
Operator : RC/JU
Sample : Q1741-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425

Quant Time: Apr 11 23:06:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration




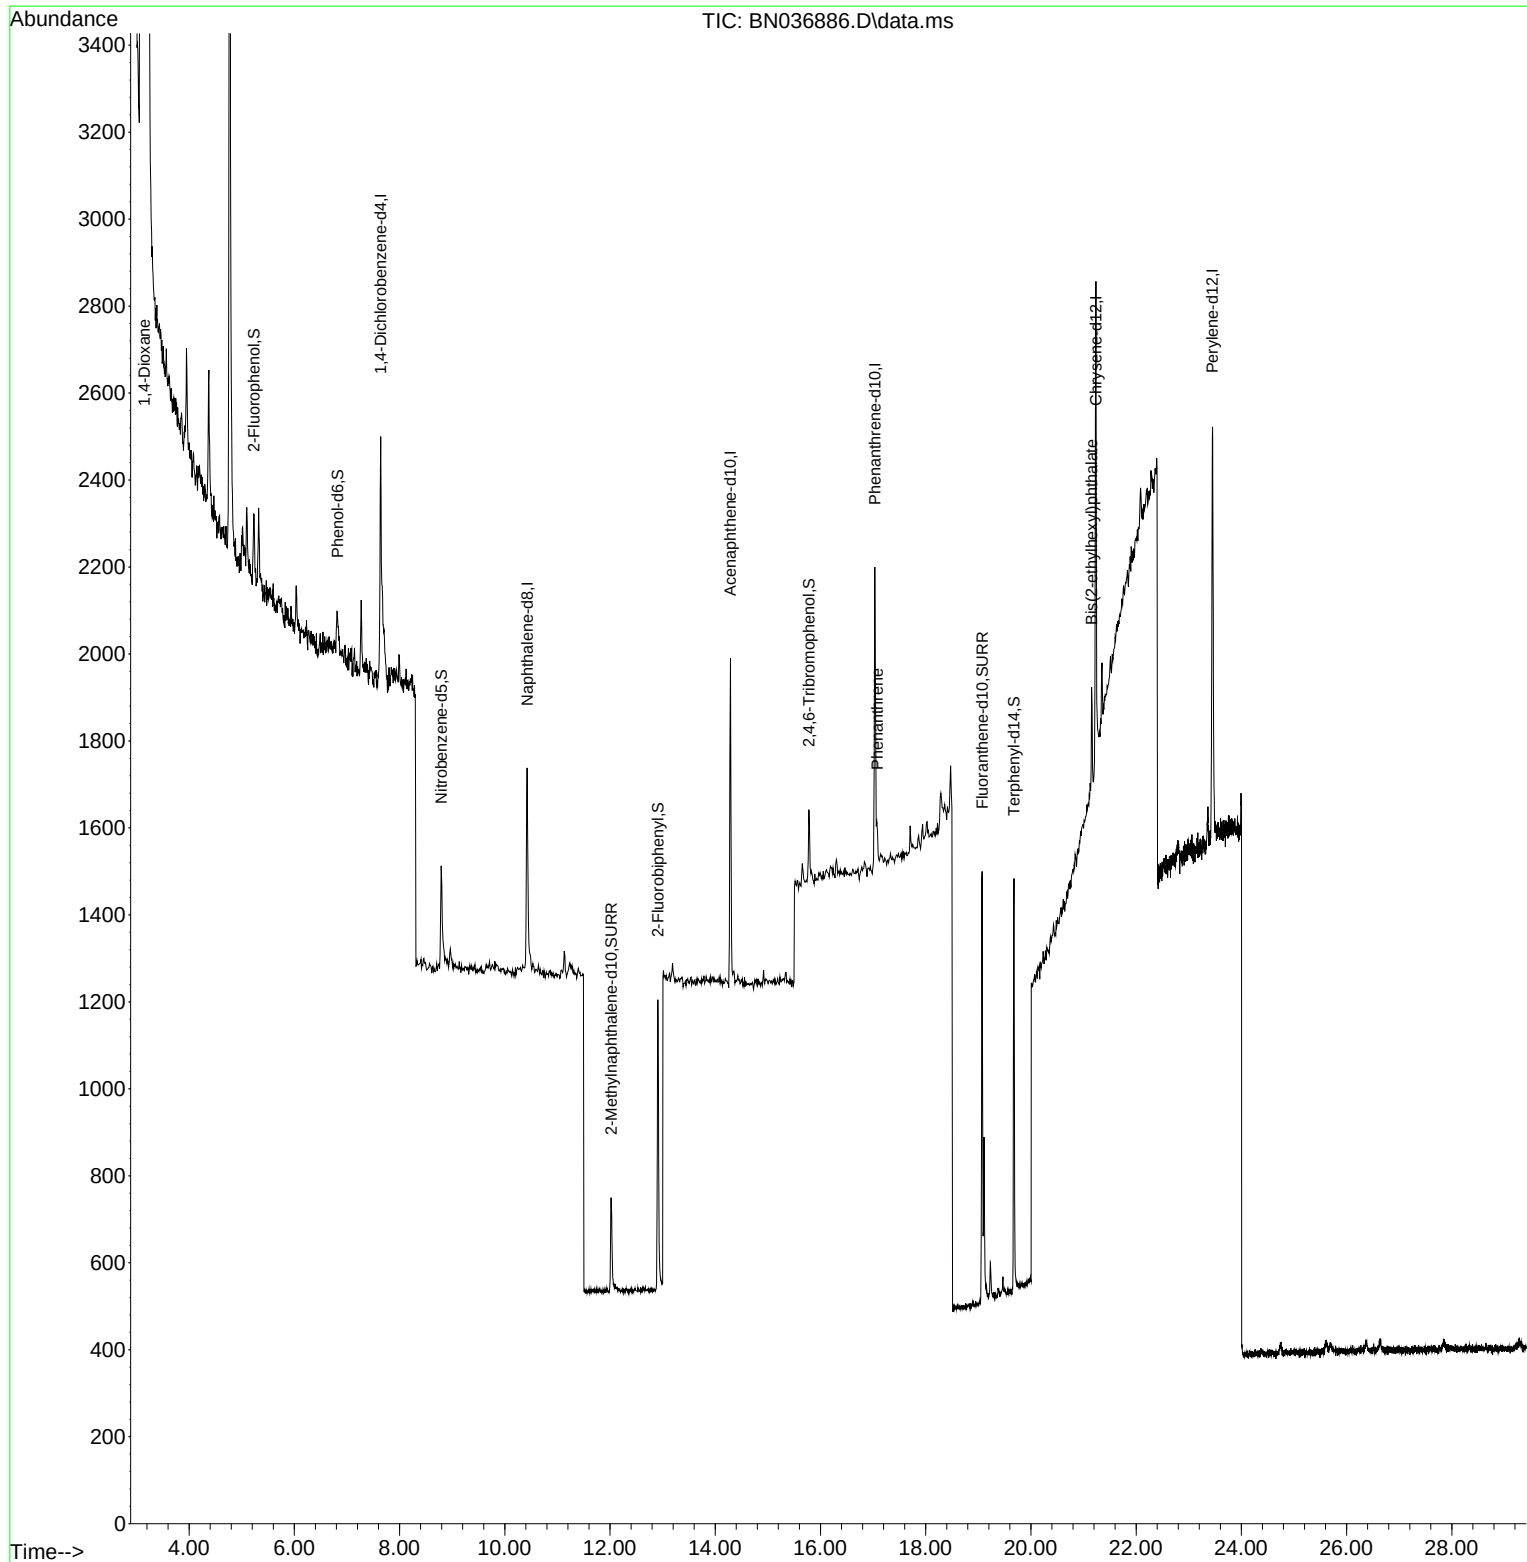




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425


Tgt Ion:152 Resp: 274
Ion Ratio Lower Upper
152 100
150 142.1 123.0 184.6
115 80.7 60.1 90.1



#2
1,4-Dioxane
Concen: 29.808 ng m
RT: 3.148 min Scan# 37
Delta R.T. -0.007 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57

Tgt Ion: 88 Resp: 9469
Ion Ratio Lower Upper
88 100
43 45.9 39.2 58.8
58 79.8 63.5 95.3





#4

2-Fluorophenol

Concen: 0.195 ng m

RT: 5.235 min Scan# 31

Delta R.T. 0.007 min

Lab File: BN036886.D

Acq: 11 Apr 2025 19:57

Instrument :

BNA_N

ClientSampleId :

RMW-02B-66-040425





Tgt Ion:112 Resp: 126

Ion Ratio Lower Upper

112 100

64 95.2 54.0 81.0#

63 46.8 35.1 52.7



#5

Phenol-d6

Concen: 0.104 ng

RT: 6.824 min Scan# 546

Delta R.T. 0.007 min

Lab File: BN036886.D

Acq: 11 Apr 2025 19:57




Tgt Ion: 99 Resp: 86


Ion Ratio Lower Upper

99 100

42 58.1 30.9 46.3#

71 62.8 38.6 58.0#









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425


Tgt Ion:	136	Resp:	725
Ion	Ratio	Lower	Upper
136	100		
137	23.2	13.5	20.3#
54	22.4	12.8	19.2#
68	17.0	10.1	15.1#



#8
Nitrobenzene-d5
Concen: 0.352 ng
RT: 8.792 min Scan# 797
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57

Tgt Ion:	82	Resp:	283
Ion	Ratio	Lower	Upper
82	100		
128	60.4	35.5	53.3#
54	81.2	56.2	84.4









#11
2-Methylnaphthalene-d10
Concen: 0.340 ng
RT: 12.021 min Scan# 1153
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425


Tgt Ion:152 Resp: 358
Ion Ratio Lower Upper
152 100
151 23.7 17.8 26.8



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57

Tgt Ion:164 Resp: 456
Ion Ratio Lower Upper
164 100
162 101.8 85.7 128.5
160 56.9 46.9 70.3









#14
2,4,6-Tribromophenol
Concen: 0.446 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425


Tgt Ion:	330	Resp:	98
Ion	Ratio	Lower	Upper
330	100		
332	99.0	87.0	130.6
141	64.3	45.3	67.9



#15
2-Fluorobiphenyl
Concen: 0.380 ng
RT: 12.909 min Scan# 1328
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57

Tgt Ion:	172	Resp:	832
Ion	Ratio	Lower	Upper
172	100		
171	40.5	32.7	49.1
170	31.1	23.3	34.9





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN036886.D

Acq: 11 Apr 2025 19:57

Instrument :

BNA_N

ClientSampleId :

RMW-02B-66-040425





Tgt Ion:188 Resp: 993

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 18.9 13.9 20.9

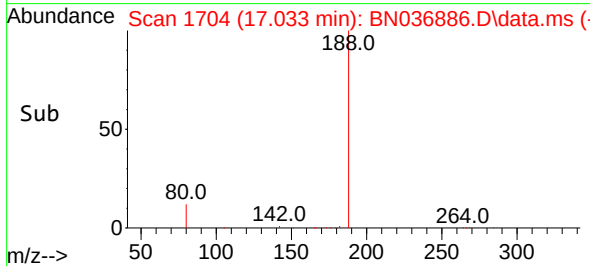

#25

Phenanthrene

Concen: 0.028 ng

RT: 17.083 min Scan# 1708

Delta R.T. -0.000 min

Lab File: BN036886.D

Acq: 11 Apr 2025 19:57




Tgt Ion:178 Resp: 84


Ion Ratio Lower Upper

178 100

176 31.0 16.6 25.0#

179 50.0 12.8 19.2#









#27
Fluoranthene-d10
Concen: 0.413 ng
RT: 19.073 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425


Tgt Ion:	212	Resp:	1156
Ion	Ratio	Lower	Upper
212	100		
106	13.4	11.2	16.8
104	8.9	7.5	11.3

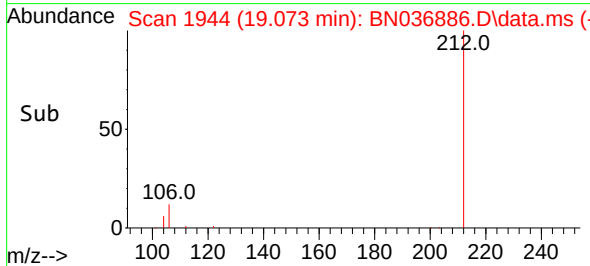

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.233 min Scan# 2282
Delta R.T. -0.000 min
Lab File: BN036886.D
Acq: 11 Apr 2025 19:57

Tgt Ion:	240	Resp:	1080
Ion	Ratio	Lower	Upper
240	100		
120	20.2	15.8	23.6
236	33.4	25.8	38.8









#31
 Terphenyl-d14
 Concen: 0.429 ng
 RT: 19.676 min Scan# 2075
 Delta R.T. -0.005 min
 Lab File: BN036886.D
 Acq: 11 Apr 2025 19:57




Instrument :
 BNA_N
 ClientSampleId :
 RMW-02B-66-040425


Tgt Ion:244 Resp: 881
 Ion Ratio Lower Upper
 244 100
 212 16.2 11.6 17.4
 122 21.2 14.9 22.3

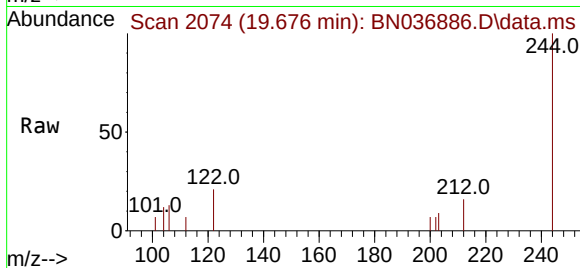

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.087 ng
 RT: 21.153 min Scan# 2273
 Delta R.T. -0.009 min
 Lab File: BN036886.D
 Acq: 11 Apr 2025 19:57

Tgt Ion:149 Resp: 245
 Ion Ratio Lower Upper
 149 100
 167 33.5 21.0 31.4#
 279 4.9 3.6 5.4

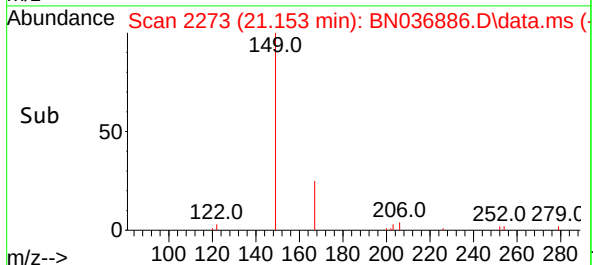



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.447 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN036886.D


Acq: 11 Apr 2025 19:57

Instrument :

BNA_N

ClientSampleId :

RMW-02B-66-040425





Tgt Ion:264 Resp: 1296

Ion Ratio Lower Upper

264 100

260 29.8 22.9 34.3

265 138.4 88.6 132.8#



Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	04/04/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	04/04/25
Client Sample ID:	RMW-02B-66-040425DL	SDG No.:	Q1741
Lab Sample ID:	Q1741-01DL	Matrix:	Water
Analytical Method:	SW8270ESIM	% Solid:	0
Sample Wt/Vol:	970 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	SVOC-SIMGroup1
Extraction Type :	Decanted : N	Level :	LOW
Injection Volume :	GPC Factor : 1.0	GPC Cleanup :	N PH :
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN036908.D	10	04/08/25 10:10	04/14/25 20:04	PB167519

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
123-91-1	1,4-Dioxane	31.2	D	0.71	2.10	ug/L
SURROGATES						
7297-45-2	2-Methylnaphthalene-d10	0.33		30 (20) - 150 (139)	83%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.42		30 (30) - 150 (150)	105%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.31		30 (27) - 130 (154)	77%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.38		30 (25) - 130 (149)	95%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.48		30 (54) - 130 (175)	120%	SPK: 0.4
INTERNAL STANDARDS						
3855-82-1	1,4-Dichlorobenzene-d4	1220		7.633		
1146-65-2	Naphthalene-d8	2950		10.415		
15067-26-2	Acenaphthene-d10	1740		14.277		
1517-22-2	Phenanthrene-d10	3460		17.033		
1719-03-5	Chrysene-d12	2950		21.224		
1520-96-3	Perylene-d12	2820		23.433		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036908.D
Acq On : 14 Apr 2025 20:04
Operator : RC/JU
Sample : Q1741-01DL 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425DL

Quant Time: Apr 15 01:04:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:58:02 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	1215	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	2952	0.400	ng	# 0.00
13) Acenaphthene-d10	14.277	164	1740	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	3461	0.400	ng	0.00
29) Chrysene-d12	21.224	240	2948	0.400	ng	0.00
35) Perylene-d12	23.433	264	2817	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	50	0.017	ng	0.00
5) Phenol-d6	6.817	99	42	0.012	ng	0.00
8) Nitrobenzene-d5	8.803	82	103	0.031	ng	0.02
11) 2-Methylnaphthalene-d10	12.026	152	144	0.033	ng	0.02
14) 2,4,6-Tribromophenol	15.792	330	37	0.044	ng	0.01
15) 2-Fluorobiphenyl	12.914	172	322	0.038	ng	0.01
27) Fluoranthene-d10	19.068	212	384	0.042	ng	0.00
31) Terphenyl-d14	19.672	244	311	0.048	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.148	88	4200	3.023	ng	99
34) Bis(2-ethylhexyl)phtha...	21.153	149	201	0.033	ng	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036908.D
Acq On : 14 Apr 2025 20:04
Operator : RC/JU
Sample : Q1741-01DL 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425DL

Quant Time: Apr 15 01:04:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:58:02 2025
Response via : Initial Calibration




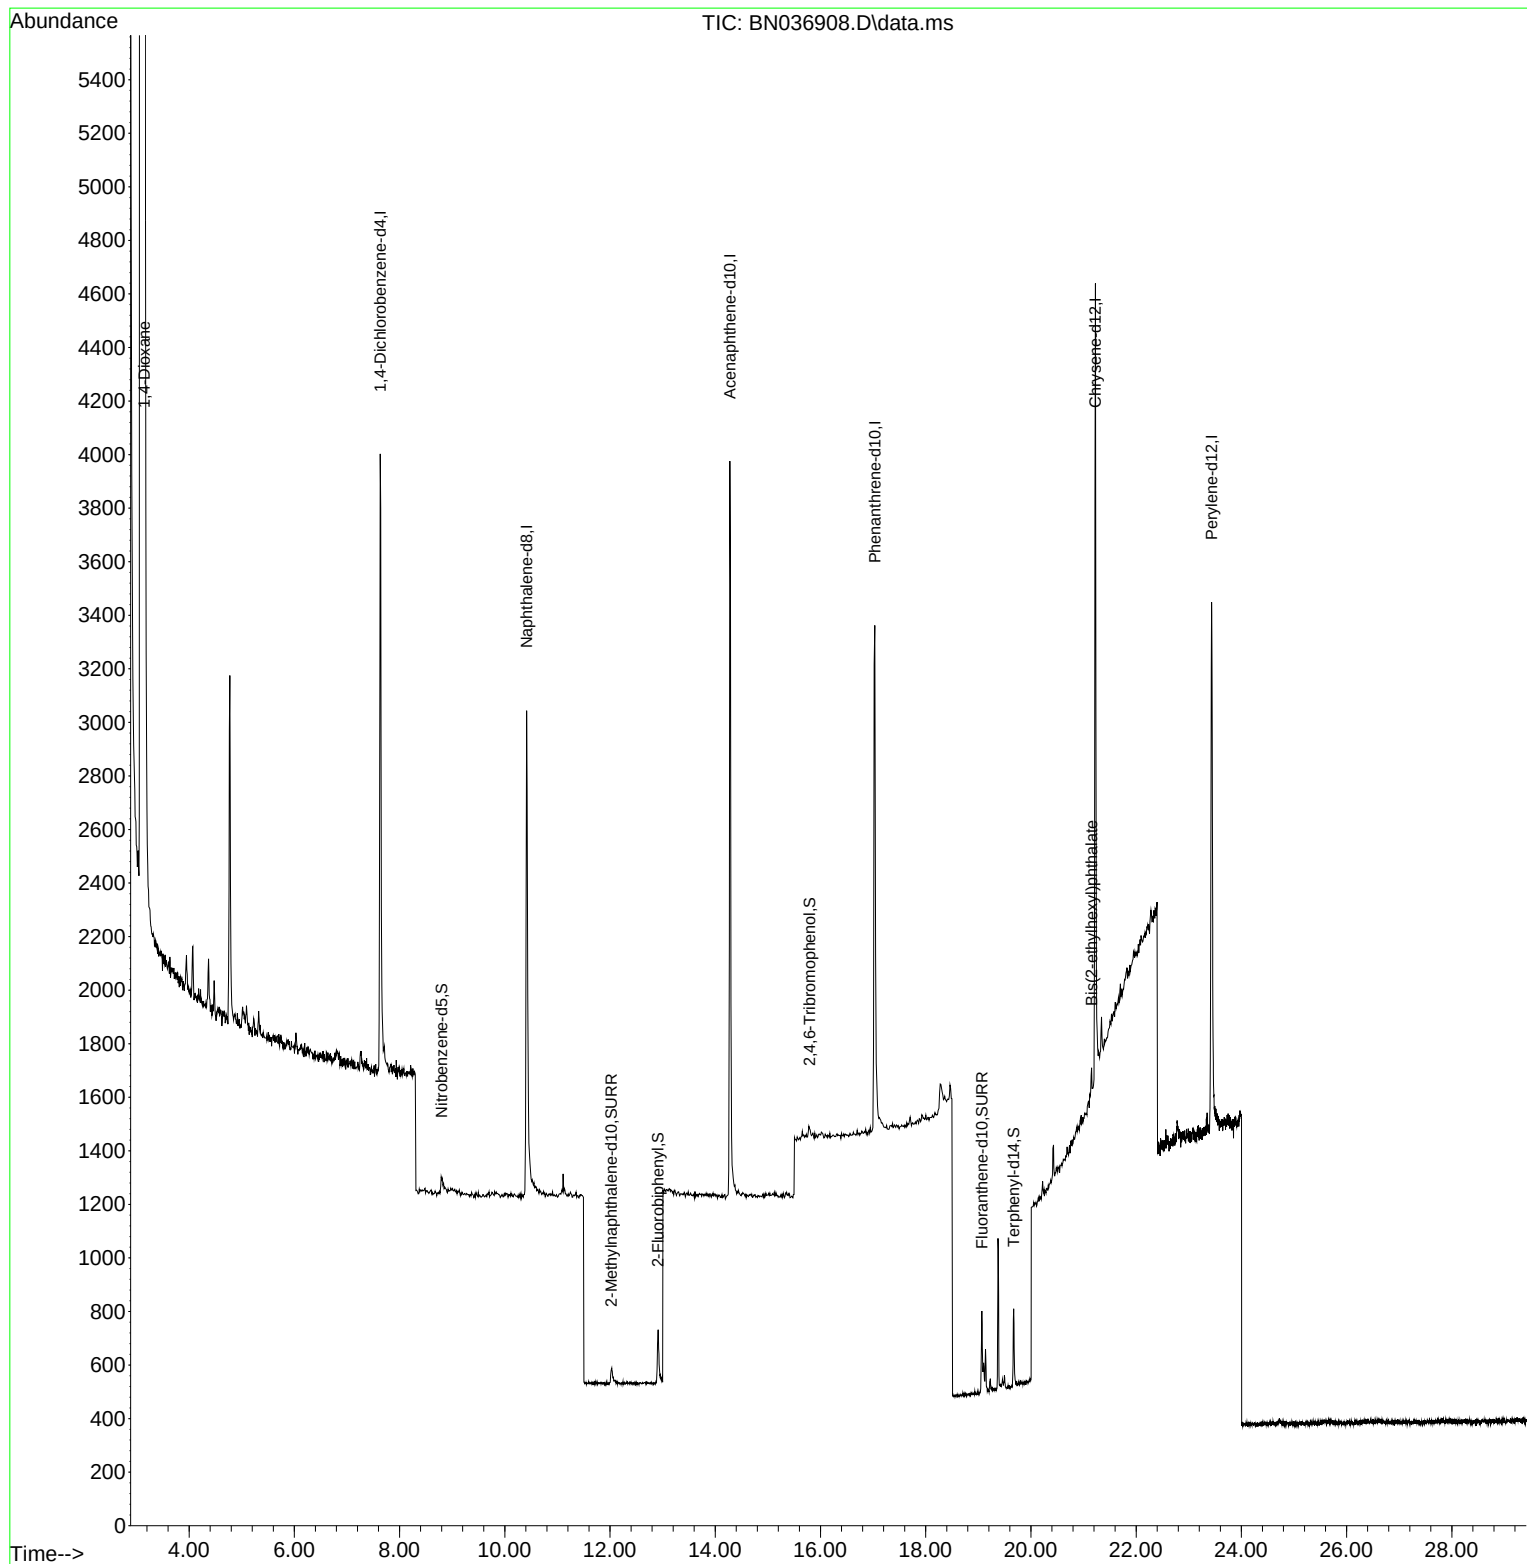




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425DL


Tgt Ion:152 Resp: 1215
Ion Ratio Lower Upper
152 100
150 146.9 121.4 182.2
115 67.9 55.4 83.2



#2
1,4-Dioxane
Concen: 3.023 ng
RT: 3.148 min Scan# 37
Delta R.T. -0.007 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04

Tgt Ion: 88 Resp: 4200
Ion Ratio Lower Upper
88 100
43 54.1 44.0 66.0
58 85.4 67.8 101.6









#4
2-Fluorophenol
Concen: 0.017 ng
RT: 5.228 min Scan# 31
Delta R.T. -0.000 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425DL


Tgt Ion:112 Resp: 50
Ion Ratio Lower Upper
112 100
64 74.0 54.4 81.6
63 58.0 35.1 52.7#



#5
Phenol-d6
Concen: 0.012 ng
RT: 6.817 min Scan# 545
Delta R.T. 0.007 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04

Tgt Ion: 99 Resp: 42
Ion Ratio Lower Upper
99 100
42 85.7 30.6 45.8#
71 47.6 38.0 57.0









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. -0.000 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425DL


Tgt Ion:	136	Resp:	2952
Ion	Ratio	Lower	Upper
136	100		
137	14.0	10.6	15.8
54	16.3	10.6	16.0#
68	9.2	6.1	9.1#



#8
Nitrobenzene-d5
Concen: 0.031 ng
RT: 8.803 min Scan# 798
Delta R.T. 0.021 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04

Tgt Ion:	82	Resp:	103
Ion	Ratio	Lower	Upper
82	100		
128	76.6	29.0	43.4#
54	85.7	60.8	91.2


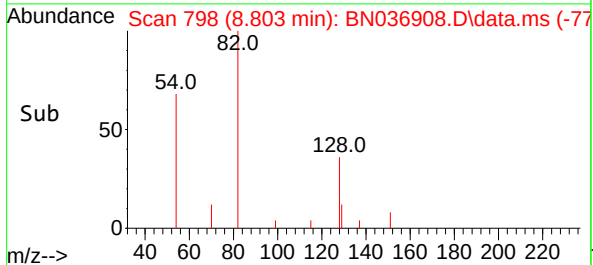
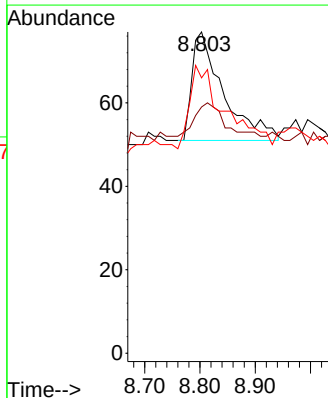





#11
2-Methylnaphthalene-d10
Concen: 0.033 ng
RT: 12.026 min Scan# 1154
Delta R.T. 0.015 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425DL


Tgt Ion:152 Resp: 144
Ion Ratio Lower Upper
152 100
151 18.8 17.1 25.7



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04

Tgt Ion:164 Resp: 1740
Ion Ratio Lower Upper
164 100
162 107.1 83.8 125.8
160 58.2 44.7 67.1









#14
2,4,6-Tribromophenol
Concen: 0.044 ng
RT: 15.792 min Scan# 1604
Delta R.T. 0.012 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425DL


Tgt Ion	330	Resp	37
Ion Ratio	Lower	Upper	
330	100		
332	94.6	77.0	115.6
141	54.1	44.5	66.7

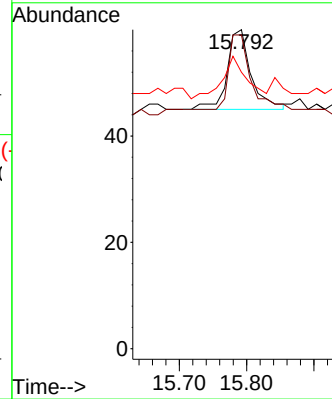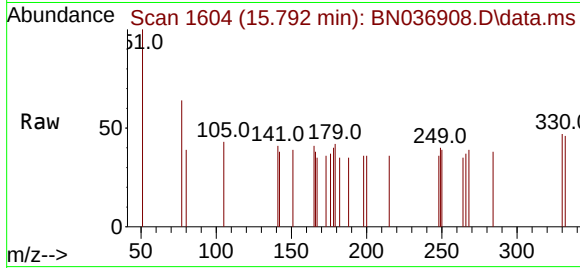

#15
2-Fluorobiphenyl
Concen: 0.038 ng
RT: 12.914 min Scan# 1329
Delta R.T. 0.010 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04

Tgt Ion	172	Resp	322
Ion Ratio	Lower	Upper	
172	100		
171	50.0	29.2	43.8#
170	41.7	20.5	30.7#

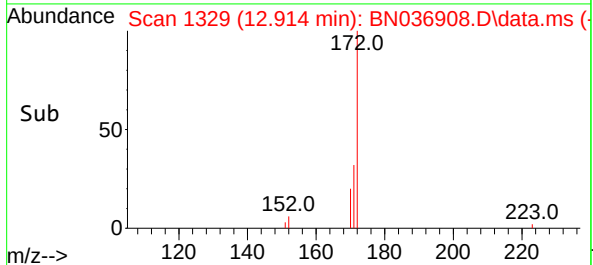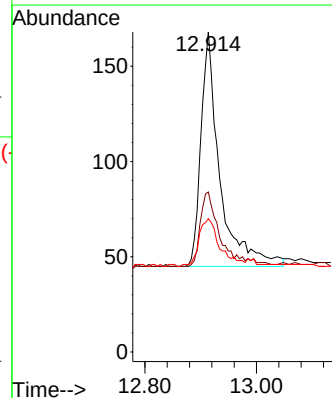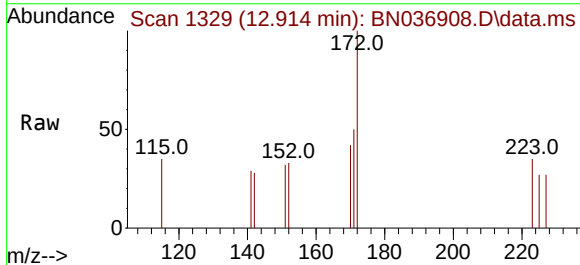



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN036908.D

Acq: 14 Apr 2025 20:04

Instrument :

BNA_N

ClientSampleId :

RMW-02B-66-040425DL





Tgt Ion:188 Resp: 3461

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 10.5 7.1 10.7

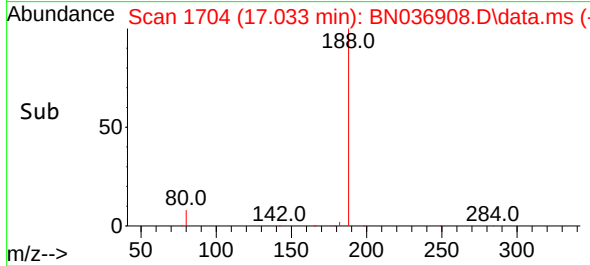

#27

Fluoranthene-d10

Concen: 0.042 ng

RT: 19.068 min Scan# 1943

Delta R.T. 0.005 min

Lab File: BN036908.D

Acq: 14 Apr 2025 20:04




Tgt Ion:212 Resp: 384


Ion Ratio Lower Upper

212 100

106 12.2 10.6 15.8

104 8.3 6.6 10.0





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036908.D

Acq: 14 Apr 2025 20:04

Instrument :

BNA_N

ClientSampleId :

RMW-02B-66-040425DL





Tgt Ion:240 Resp: 2948

Ion Ratio Lower Upper

240 100

120 12.8 9.8 14.6

236 30.6 23.1 34.7

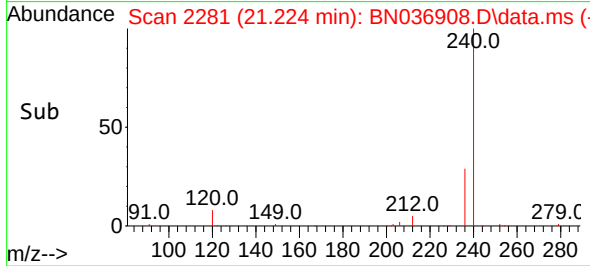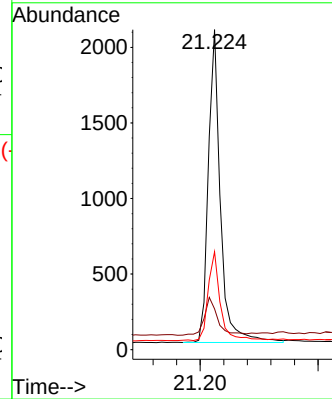

#31

Terphenyl-d14

Concen: 0.048 ng

RT: 19.672 min Scan# 2073

Delta R.T. 0.005 min

Lab File: BN036908.D

Acq: 14 Apr 2025 20:04




Tgt Ion:244 Resp: 311


Ion Ratio Lower Upper

244 100

212 27.3 10.1 15.1#

122 31.5 13.6 20.4#



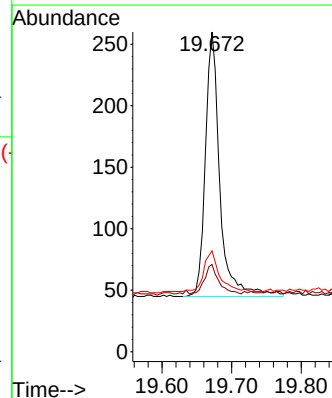





#34
Bis(2-ethylhexyl)phthalate
Concen: 0.033 ng
RT: 21.153 min Scan# 21153
Delta R.T. 0.009 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04




Instrument :
BNA_N
ClientSampleId :
RMW-02B-66-040425DL

Tgt Ion:149 Resp: 201
Ion Ratio Lower Upper
149 100
167 13.9 21.7 32.5#
279 7.5 3.0 4.4#

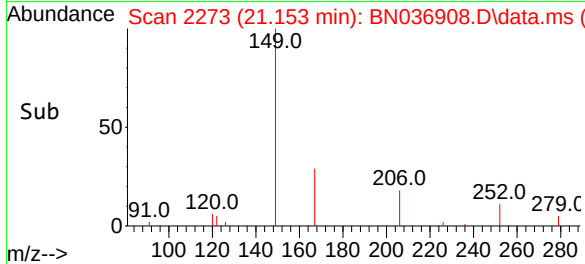

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.433 min Scan# 2764
Delta R.T. -0.000 min
Lab File: BN036908.D
Acq: 14 Apr 2025 20:04

Tgt Ion:264 Resp: 2817
Ion Ratio Lower Upper
264 100
260 28.1 22.3 33.5
265 77.7 57.6 86.4

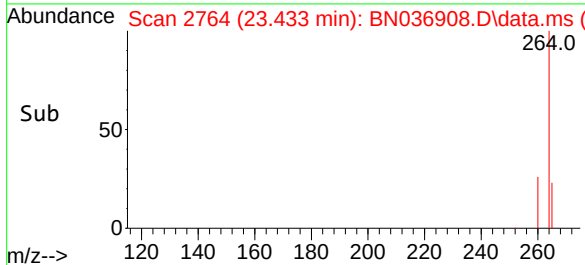

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	04/04/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	04/04/25
Client Sample ID:	RMW-06B-74-040425	SDG No.:	Q1741
Lab Sample ID:	Q1741-02	Matrix:	Water
Analytical Method:	SW8270ESIM	% Solid:	0
Sample Wt/Vol:	970 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	SVOC-SIMGroup1
Extraction Type :	Decanted : N	Level :	LOW
Injection Volume :	GPC Factor : 1.0	GPC Cleanup :	N PH :
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN036887.D	1	04/08/25 10:10	04/11/25 20:34	PB167519

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
123-91-1	1,4-Dioxane	0.070	U	0.070	0.21	ug/L
SURROGATES						
7297-45-2	2-Methylnaphthalene-d10	0.35		30 (20) - 150 (139)	86%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.41		30 (30) - 150 (150)	102%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.33		30 (27) - 130 (154)	82%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.34		30 (25) - 130 (149)	86%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.42		30 (54) - 130 (175)	104%	SPK: 0.4
INTERNAL STANDARDS						
3855-82-1	1,4-Dichlorobenzene-d4	257	7.64			
1146-65-2	Naphthalene-d8	678	10.426			
15067-26-2	Acenaphthene-d10	429	14.288			
1517-22-2	Phenanthrene-d10	971	17.033			
1719-03-5	Chrysene-d12	1080	21.233			
1520-96-3	Perylene-d12	1370	23.447			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036887.D
Acq On : 11 Apr 2025 20:34
Operator : RC/JU
Sample : Q1741-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425

Quant Time: Apr 11 23:06:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	257	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	678	0.400	ng	# 0.00
13) Acenaphthene-d10	14.288	164	429	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	971	0.400	ng	0.00
29) Chrysene-d12	21.233	240	1082	0.400	ng	0.00
35) Perylene-d12	23.447	264	1366	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.235	112	111	0.184	ng	0.00
5) Phenol-d6	6.817	99	87	0.113	ng	0.00
8) Nitrobenzene-d5	8.792	82	247	0.328	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	340	0.345	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	85	0.411	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	709	0.344	ng	0.00
27) Fluoranthene-d10	19.073	212	1122	0.410	ng	0.00
31) Terphenyl-d14	19.676	244	859	0.418	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.153	149	329	0.116	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036887.D
Acq On : 11 Apr 2025 20:34
Operator : RC/JU
Sample : Q1741-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425

Quant Time: Apr 11 23:06:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration




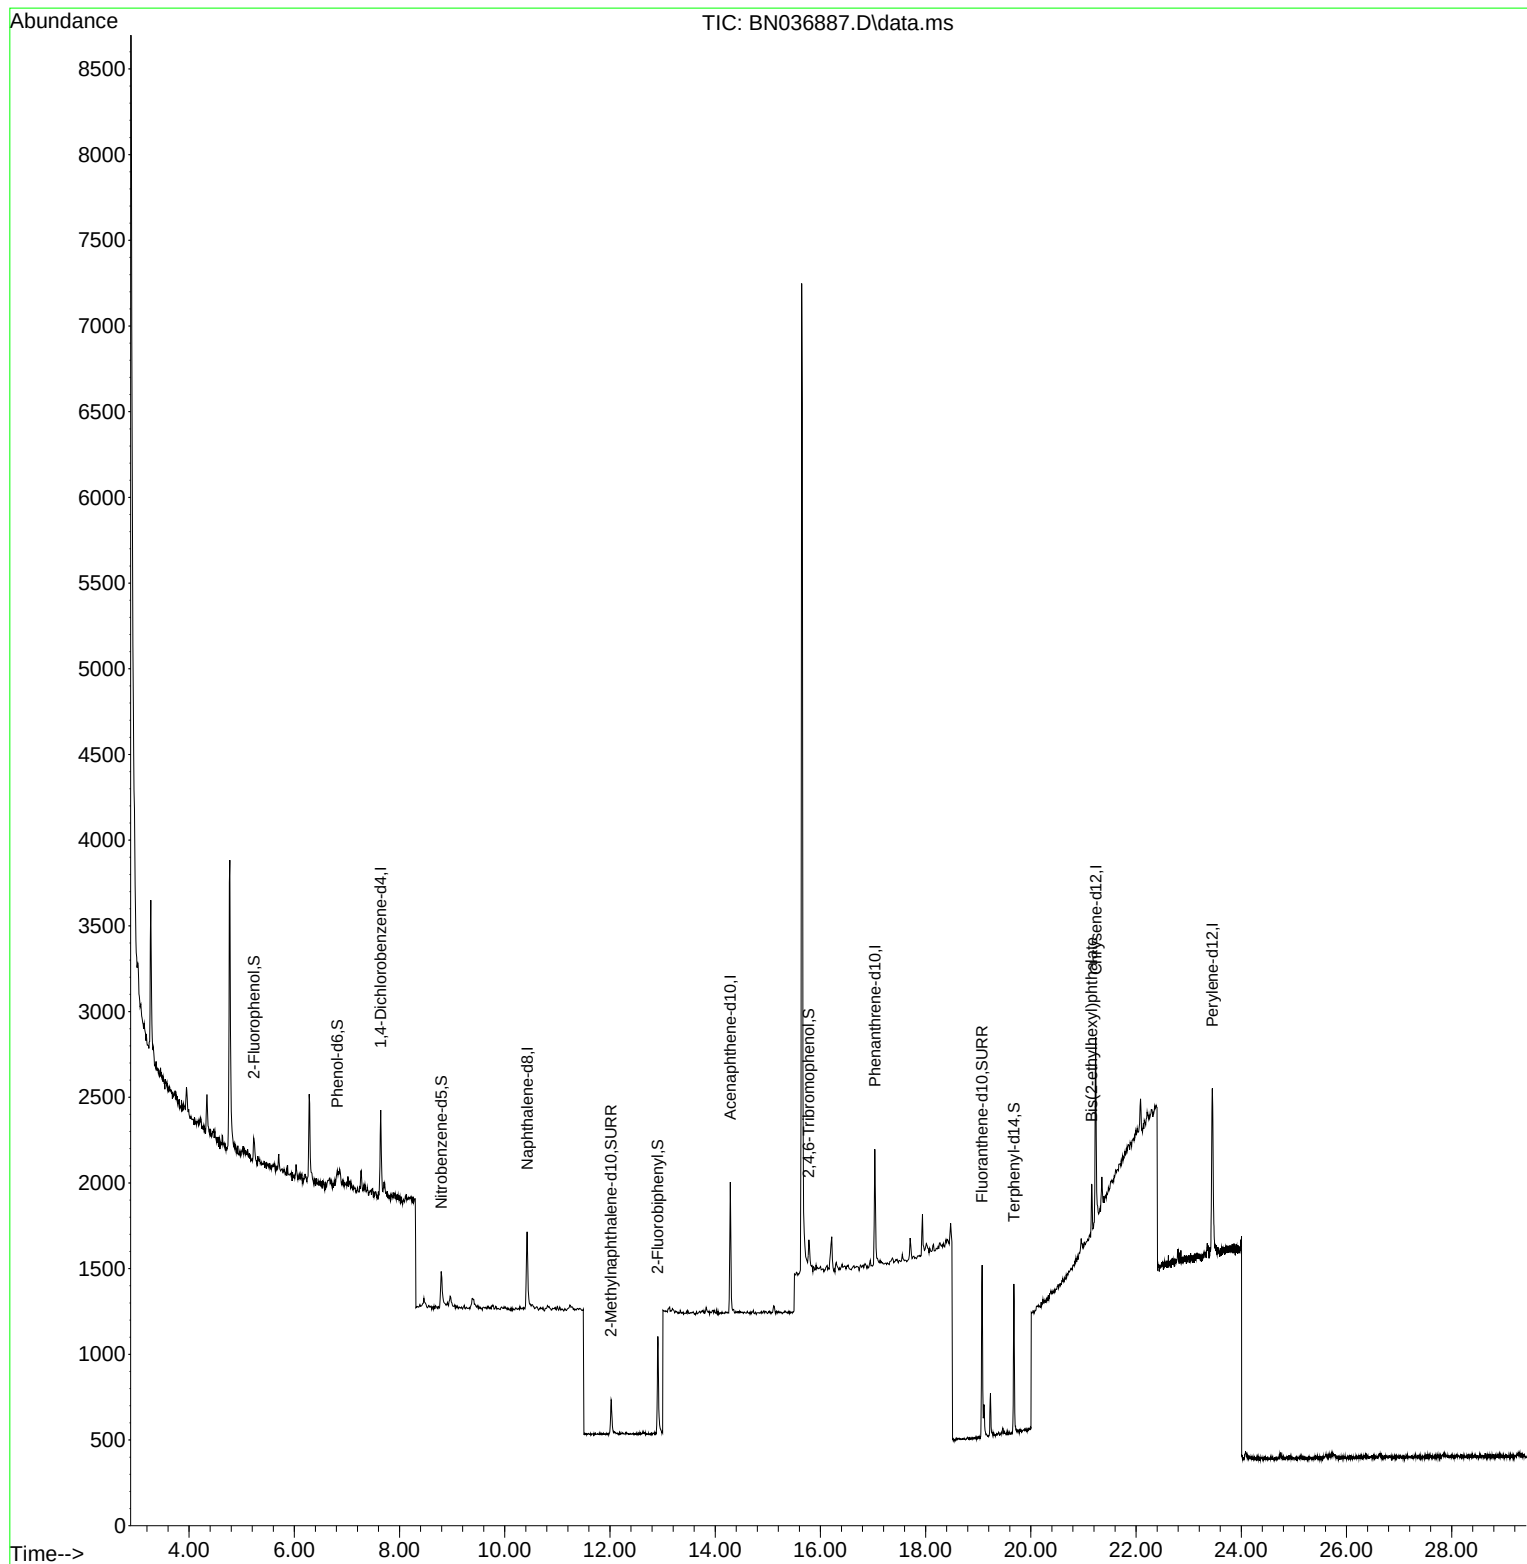




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34




Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425


Tgt Ion:152 Resp: 257
Ion Ratio Lower Upper
152 100
150 133.8 123.0 184.6
115 82.1 60.1 90.1



#4
2-Fluorophenol
Concen: 0.184 ng
RT: 5.235 min Scan# 326
Delta R.T. 0.007 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34

Tgt Ion:112 Resp: 111
Ion Ratio Lower Upper
112 100
64 73.9 54.0 81.0
63 46.8 35.1 52.7




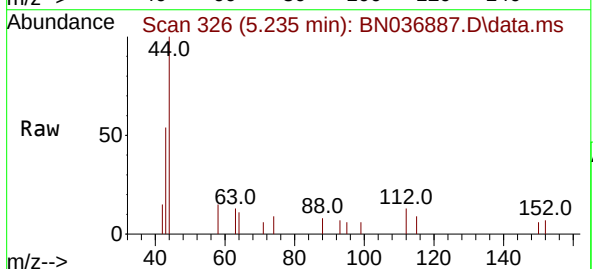




#5
Phenol-d6
Concen: 0.113 ng
RT: 6.817 min Scan# 54
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34




Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425


Tgt Ion	Ratio	Lower	Upper
99	100		
42	52.9	30.9	46.3#
71	51.7	38.6	58.0



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 950
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34

Tgt Ion	Ratio	Lower	Upper
136	100		
137	22.0	13.5	20.3#
54	22.3	12.8	19.2#
68	18.3	10.1	15.1#









#8
Nitrobenzene-d5
Concen: 0.328 ng
RT: 8.792 min Scan# 797
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34




Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425


Tgt Ion:	82	Resp:	247
Ion Ratio	Lower	Upper	
82	100		
128	62.7	35.5	53.3#
54	85.1	56.2	84.4#



#11
2-Methylnaphthalene-d10
Concen: 0.345 ng
RT: 12.021 min Scan# 1153
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34

Tgt Ion:	152	Resp:	340
Ion Ratio	Lower	Upper	
152	100		
151	21.2	17.8	26.8









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34




Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425


Tgt Ion:	164	Resp:	429
Ion	Ratio	Lower	Upper
164	100		
162	109.7	85.7	128.5
160	61.7	46.9	70.3

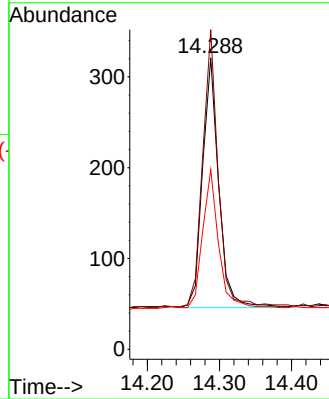

#14
2,4,6-Tribromophenol
Concen: 0.411 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34

Tgt Ion:	330	Resp:	85
Ion	Ratio	Lower	Upper
330	100		
332	114.1	87.0	130.6
141	70.6	45.3	67.9









#15
2-Fluorobiphenyl
Concen: 0.344 ng
RT: 12.909 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34




Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425


Tgt Ion:	172	Resp:	709
Ion	Ratio	Lower	Upper
172	100		
171	41.5	32.7	49.1
170	33.1	23.3	34.9



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.033 min Scan# 1704
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34

Tgt Ion:	188	Resp:	971
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	17.9	13.9	20.9









#27
Fluoranthene-d10
Concen: 0.410 ng
RT: 19.073 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34




Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425


Tgt Ion:212	Resp:	1122
Ion	Ratio	Lower Upper
212	100	
106	13.2	11.2 16.8
104	8.1	7.5 11.3



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.233 min Scan# 2282
Delta R.T. -0.000 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34

Tgt Ion:240	Resp:	1082
Ion	Ratio	Lower Upper
240	100	
120	23.5	15.8 23.6
236	32.8	25.8 38.8









#31
Terphenyl-d14
Concen: 0.418 ng
RT: 19.676 min Scan# 2075
Delta R.T. -0.005 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34




Instrument :
BNA_N
ClientSampleId :
RMW-06B-74-040425


Tgt Ion	Ratio	Lower	Upper
244	100		
212	17.0	11.6	17.4
122	22.0	14.9	22.3

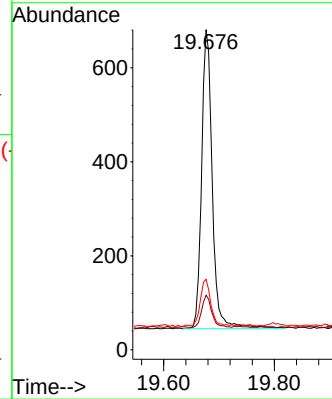

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.116 ng
RT: 21.153 min Scan# 2273
Delta R.T. -0.009 min
Lab File: BN036887.D
Acq: 11 Apr 2025 20:34

Tgt Ion	Ratio	Lower	Upper
149	100		
167	25.5	21.0	31.4
279	5.8	3.6	5.4

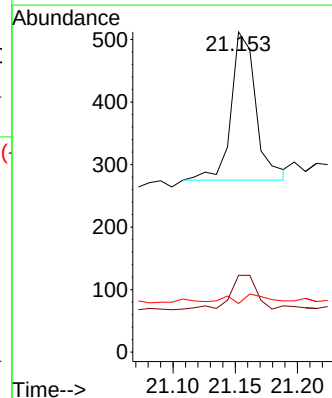



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.447 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN036887.D


Acq: 11 Apr 2025 20:34

Instrument :

BNA_N

ClientSampleId :

RMW-06B-74-040425





Tgt Ion:264 Resp: 1366

Ion Ratio Lower Upper

264 100

260 31.2 22.9 34.3

265 137.9 88.6 132.8#



Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	04/04/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	04/04/25
Client Sample ID:	FB01-040425	SDG No.:	Q1741
Lab Sample ID:	Q1741-03	Matrix:	Water
Analytical Method:	SW8270ESIM	% Solid:	0
Sample Wt/Vol:	980 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	SVOC-SIMGroup1
Extraction Type :	Decanted : N	Level :	LOW
Injection Volume :	GPC Factor : 1.0	GPC Cleanup :	N PH :
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN036888.D	1	04/08/25 10:10	04/11/25 21:10	PB167519

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
123-91-1	1,4-Dioxane	0.070	U	0.070	0.20	ug/L
SURROGATES						
7297-45-2	2-Methylnaphthalene-d10	0.31		30 (20) - 150 (139)	76%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.41		30 (30) - 150 (150)	103%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.30		30 (27) - 130 (154)	74%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.36		30 (25) - 130 (149)	91%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.52		30 (54) - 130 (175)	129%	SPK: 0.4
INTERNAL STANDARDS						
3855-82-1	1,4-Dichlorobenzene-d4	267	7.64			
1146-65-2	Naphthalene-d8	721	10.426			
15067-26-2	Acenaphthene-d10	449	14.288			
1517-22-2	Phenanthrene-d10	971	17.033			
1719-03-5	Chrysene-d12	1110	21.233			
1520-96-3	Perylene-d12	1320	23.45			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036888.D
Acq On : 11 Apr 2025 21:10
Operator : RC/JU
Sample : Q1741-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
FB01-040425

Quant Time: Apr 11 23:06:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	267	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	721	0.400	ng	# 0.00
13) Acenaphthene-d10	14.288	164	449	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	971	0.400	ng	0.00
29) Chrysene-d12	21.233	240	1105	0.400	ng	0.00
35) Perylene-d12	23.450	264	1316	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.235	112	125	0.199	ng	0.00
5) Phenol-d6	6.824	99	79	0.098	ng	0.00
8) Nitrobenzene-d5	8.792	82	237	0.296	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	320	0.305	ng	0.00
14) 2,4,6-Tribromophenol	15.792	330	95	0.439	ng	0.01
15) 2-Fluorobiphenyl	12.914	172	782	0.363	ng	0.00
27) Fluoranthene-d10	19.073	212	1132	0.414	ng	0.00
31) Terphenyl-d14	19.677	244	1085	0.517	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.153	149	513	0.177	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036888.D
Acq On : 11 Apr 2025 21:10
Operator : RC/JU
Sample : Q1741-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
FB01-040425

Quant Time: Apr 11 23:06:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration




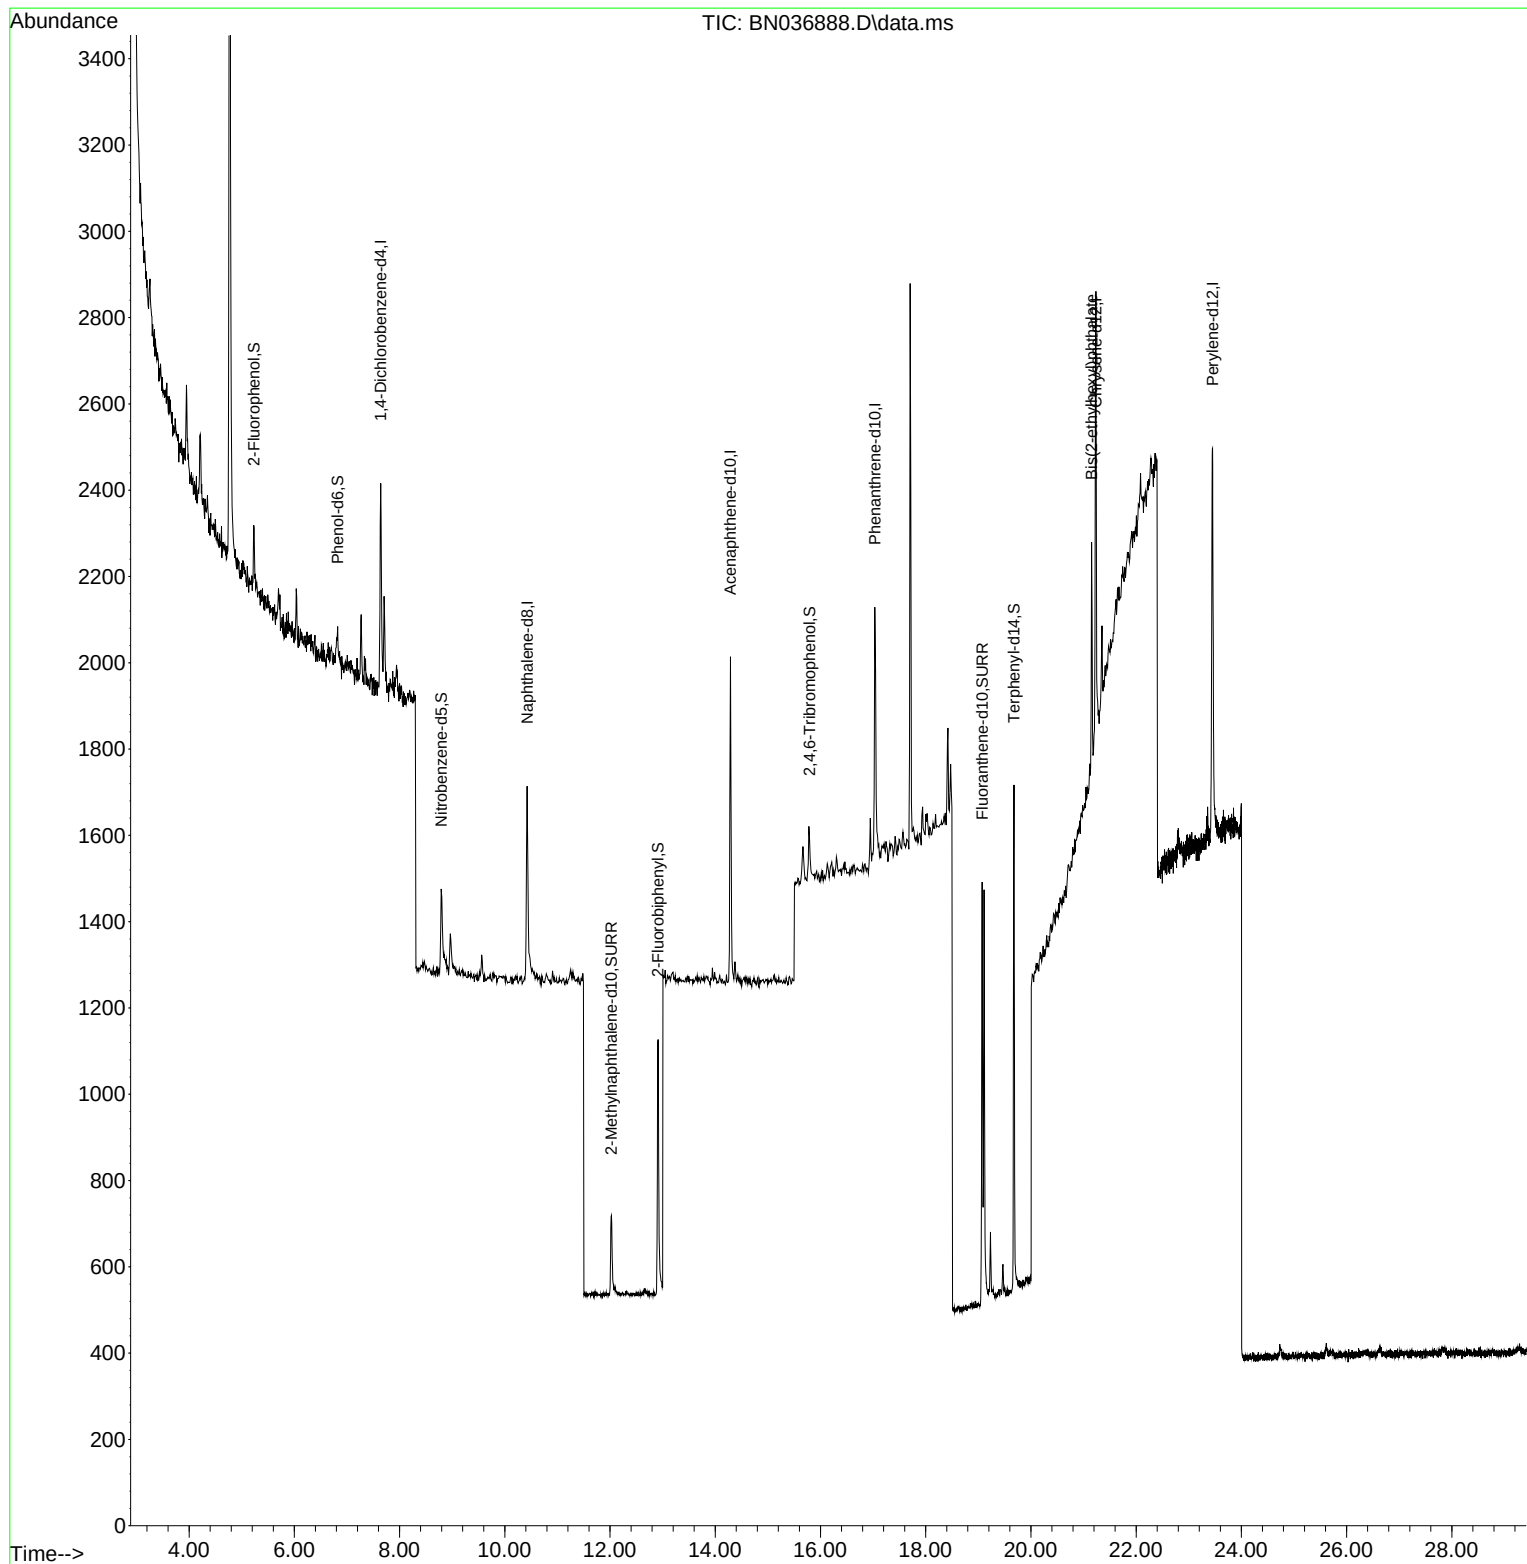




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10




Instrument :
BNA_N
ClientSampleId :
FB01-040425


Tgt Ion:152 Resp: 267
Ion Ratio Lower Upper
152 100
150 142.1 123.0 184.6
115 83.2 60.1 90.1



#4
2-Fluorophenol
Concen: 0.199 ng
RT: 5.235 min Scan# 326
Delta R.T. 0.007 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10

Tgt Ion:112 Resp: 125
Ion Ratio Lower Upper
112 100
64 64.0 54.0 81.0
63 46.4 35.1 52.7









#5
Phenol-d6
Concen: 0.098 ng
RT: 6.824 min Scan# 54
Delta R.T. 0.007 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10




Instrument :
BNA_N
ClientSampleId :
FB01-040425


Tgt Ion: 99 Resp: 79
Ion Ratio Lower Upper
99 100
42 49.4 30.9 46.3#
71 75.9 38.6 58.0#



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 950
Delta R.T. 0.000 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10

Tgt Ion: 136 Resp: 721
Ion Ratio Lower Upper
136 100
137 22.0 13.5 20.3#
54 23.9 12.8 19.2#
68 17.5 10.1 15.1#









#8
Nitrobenzene-d5
Concen: 0.296 ng
RT: 8.792 min Scan# 797
Delta R.T. 0.000 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10




Instrument :
BNA_N
ClientSampleId :
FB01-040425


Tgt Ion:	82	Resp:	237
Ion Ratio	Lower	Upper	
82	100		
128	61.1	35.5	53.3#
54	86.3	56.2	84.4#



#11
2-Methylnaphthalene-d10
Concen: 0.305 ng
RT: 12.021 min Scan# 1153
Delta R.T. 0.000 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10

Tgt Ion:	152	Resp:	320
Ion Ratio	Lower	Upper	
152	100		
151	23.4	17.8	26.8









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 14
Delta R.T. 0.000 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10




Instrument :
BNA_N
ClientSampleId :
FB01-040425


Tgt Ion:164 Resp: 449
Ion Ratio Lower Upper
164 100
162 107.7 85.7 128.5
160 59.8 46.9 70.3

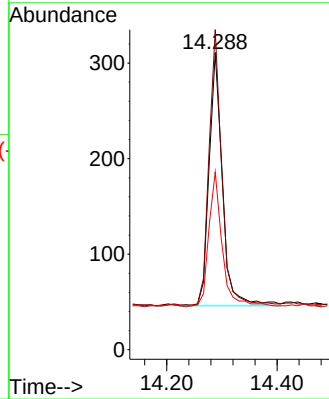

#14
2,4,6-Tribromophenol
Concen: 0.439 ng
RT: 15.792 min Scan# 1604
Delta R.T. 0.012 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10

Tgt Ion:330 Resp: 95
Ion Ratio Lower Upper
330 100
332 94.7 87.0 130.6
141 66.3 45.3 67.9









#15
2-Fluorobiphenyl
Concen: 0.363 ng
RT: 12.914 min Scan# 11
Delta R.T. 0.005 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10




Instrument :
BNA_N
ClientSampleId :
FB01-040425


Tgt Ion:172	Resp:	782
Ion	Ratio	Lower Upper
172	100	
171	43.7	32.7 49.1
170	34.3	23.3 34.9



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.033 min Scan# 1704
Delta R.T. 0.000 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10

Tgt Ion:188	Resp:	971
Ion	Ratio	Lower Upper
188	100	
94	0.0	0.0 0.0
80	19.4	13.9 20.9









#27
Fluoranthene-d10
Concen: 0.414 ng
RT: 19.073 min Scan# 1944
Delta R.T. 0.000 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10




Instrument :
BNA_N
ClientSampleId :
FB01-040425


Tgt Ion	Ratio	Lower	Upper
212	100		
106	12.7	11.2	16.8
104	8.4	7.5	11.3

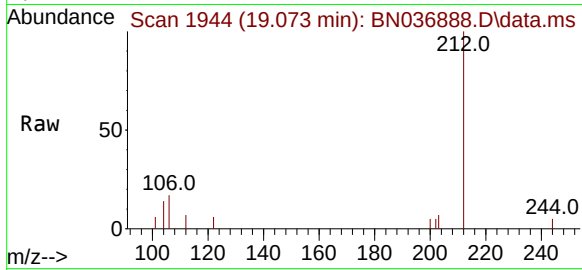

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.233 min Scan# 2282
Delta R.T. 0.000 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10

Tgt Ion	Ratio	Lower	Upper
240	100		
120	22.4	15.8	23.6
236	33.6	25.8	38.8









#31
Terphenyl-d14
Concen: 0.517 ng
RT: 19.677 min Scan# 2075
Delta R.T. -0.005 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10




Instrument :
BNA_N
ClientSampleId :
FB01-040425


Tgt Ion	Ratio	Lower	Upper
244	100		
212	16.0	11.6	17.4
122	18.6	14.9	22.3



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.177 ng
RT: 21.153 min Scan# 2273
Delta R.T. -0.009 min
Lab File: BN036888.D
Acq: 11 Apr 2025 21:10

Tgt Ion	Ratio	Lower	Upper
149	100		
167	28.5	21.0	31.4
279	3.9	3.6	5.4





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.450 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN036888.D


Acq: 11 Apr 2025 21:10

Instrument :

BNA_N

ClientSampleId :

FB01-040425





Tgt Ion:264 Resp: 1316

Ion Ratio Lower Upper

264 100

260 30.9 22.9 34.3

265 145.0 88.6 132.8#

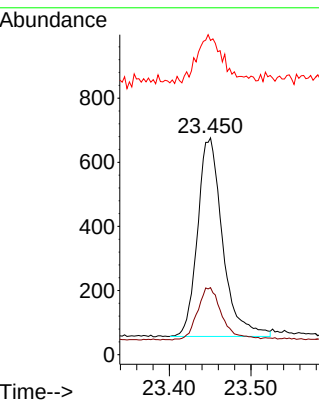



CALIBRATION SUMMARY

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\
Method File : 8270-SIM-BN041125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 11 16:11:08 2025
Response Via : Initial Calibration

Calibration Files

0.1 =BN036873.D 0.2 =BN036874.D 0.4 =BN036875.D 0.8 =BN036876.D 1.6 =BN036877.D 3.2 =BN036878.D 5.0 =BN036879.D

	Compound	0.1	0.2	0.4	0.8	1.6	3.2	5.0	Avg	%RSD
1) I	1,4-Dichlorobenzen...	-----ISTD-----								
2)	1,4-Dioxane		0.588	0.440	0.411	0.455	0.471	0.417	0.464	14.02
3)	n-Nitrosodimet...	1.024	1.092	1.084	0.971	1.022	1.058	0.943	1.028	5.43
4) S	2-Fluorophenol	1.000	0.941	0.965	0.920	0.892	0.981	0.888	0.941	4.61
5) S	Phenol-d6	1.315	1.199	1.198	1.134	1.147	1.263	1.166	1.203	5.40
6)	bis(2-Chloroet...	1.476	1.031	1.187	1.163	1.124	1.190	1.091	1.180	12.04
7) I	Naphthalene-d8	-----ISTD-----								
8) S	Nitrobenzene-d5	0.575	0.438	0.451	0.399	0.395	0.439	0.411	0.444	13.86
9)	Naphthalene	1.336	1.141	1.170	1.079	1.072	1.176	1.080	1.151	8.09
10)	Hexachlorobuta...	0.300	0.261	0.284	0.247	0.240	0.261	0.235	0.261	9.11
11) SURR	2-Methylnaphth...	0.600	0.564	0.594	0.554	0.572	0.616	0.571	0.582	3.78
12)	2-Methylnaphth...	0.803	0.703	0.759	0.704	0.711	0.784	0.724	0.741	5.50
13) I	Acenaphthene-d10	-----ISTD-----								
14) S	2,4,6-Tribromo...	0.215	0.188	0.183	0.187	0.185	0.202	0.191	0.193	5.97
15) S	2-Fluorobiphenyl	2.063	1.860	2.013	1.697	1.897	2.083	1.833	1.921	7.28
16)	Acenaphthylene	1.959	1.808	1.891	1.744	1.750	1.995	1.861	1.858	5.25
17)	Acenaphthene	1.227	1.175	1.234	1.162	1.152	1.316	1.205	1.210	4.65
18)	Fluorene	1.695	1.698	1.694	1.566	1.593	1.780	1.657	1.669	4.29
19) I	Phenanthrene-d10	-----ISTD-----								
20)	4,6-Dinitro-2-...	0.081	0.084	0.095	0.092	0.092	0.116	0.102	0.095	12.46
21)	4-Bromophenyl-...	0.239	0.230	0.260	0.229	0.230	0.258	0.231	0.240	5.77
22)	Hexachlorobenzene	0.308	0.293	0.310	0.262	0.261	0.288	0.263	0.284	7.64
23)	Atrazine	0.237	0.233	0.263	0.221	0.223	0.245	0.218	0.234	6.76
24)	Pentachlorophenol	0.153	0.154	0.162	0.130	0.134	0.160	0.149	0.149	8.32
25)	Phenanthrene	1.233	1.093	1.298	1.139	1.149	1.300	1.183	1.199	6.70
26)	Anthracene	1.033	0.999	1.150	0.991	1.036	1.182	1.094	1.069	6.97
27) SURR	Fluoranthene-d10	1.100	1.059	1.221	1.044	1.091	1.226	1.148	1.127	6.53
28)	Fluoranthene	1.448	1.405	1.606	1.395	1.463	1.677	1.570	1.509	7.21
29) I	Chrysene-d12	-----ISTD-----								
30)	Pyrene	1.488	1.512	1.604	1.477	1.469	1.582	1.451	1.512	3.88
31) S	Terphenyl-d14	0.743	0.751	0.815	0.741	0.739	0.802	0.730	0.760	4.45
32)	Benzo(a)anthra...	1.361	1.371	1.410	1.354	1.402	1.552	1.443	1.413	4.87
33)	Chrysene	1.436	1.567	1.669	1.519	1.553	1.641	1.517	1.558	5.06
34)	Bis(2-ethylhex...	1.205	1.197	1.023	0.957	0.990	1.022	0.947	1.049	10.29
35) I	Perylene-d12	-----ISTD-----								

Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\

Method File : 8270-SIM-BN041125.M

36)	Indeno(1,2,3-c...	1.781	1.803	2.021	1.816	1.925	2.099	1.919	1.909	6.24
37)	Benzo(b)fluora...	1.373	1.278	1.523	1.355	1.376	1.572	1.456	1.419	7.26
38)	Benzo(k)fluora...	1.486	1.302	1.482	1.370	1.384	1.545	1.452	1.432	5.83
39) C	Benzo(a)pyrene	1.121	1.154	1.345	1.204	1.226	1.378	1.279	1.244	7.66
40)	Dibenzo(a,h)an...	1.331	1.416	1.585	1.487	1.560	1.680	1.552	1.516	7.61
41)	Benzo(g,h,i)pe...	1.646	1.673	1.805	1.634	1.724	1.835	1.678	1.714	4.59

(#) = Out of Range

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036873.D
 Acq On : 11 Apr 2025 11:42
 Operator : RC/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Apr 11 15:34:30 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 15:32:59 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.645	152	496	0.400	ng	0.00
7) Naphthalene-d8	10.424	136	1266	0.400	ng	# 0.00
13) Acenaphthene-d10	14.291	164	727	0.400	ng	0.00
19) Phenanthrene-d10	17.037	188	1622	0.400	ng	0.00
29) Chrysene-d12	21.232	240	1643	0.400	ng	0.00
35) Perylene-d12	23.452	264	2037	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.233	112	124	0.105	ng	0.00
5) Phenol-d6	6.814	99	163	0.109	ng	0.00
8) Nitrobenzene-d5	8.790	82	182	0.128	ng	0.00
11) 2-Methylnaphthalene-d10	12.025	152	190	0.103	ng	0.00
14) 2,4,6-Tribromophenol	15.783	330	39	0.111	ng	0.00
15) 2-Fluorobiphenyl	12.912	172	375	0.107	ng	0.00
27) Fluoranthene-d10	19.076	212	446	0.098	ng	0.00
31) Terphenyl-d14	19.680	244	305	0.097	ng	0.00
Target Compounds						
3) n-Nitrosodimethylamine	3.478	42	127	0.098	ng	# 68
6) bis(2-Chloroethyl)ether	7.067	93	183	0.123	ng	88
9) Naphthalene	10.477	128	423	0.115	ng	# 75
10) Hexachlorobutadiene	10.765	225	95	0.113	ng	# 91
12) 2-Methylnaphthalene	12.101	142	254	0.108	ng	# 93
16) Acenaphthylene	14.003	152	356	0.105	ng	# 96
17) Acenaphthene	14.356	154	223	0.101	ng	98
18) Fluorene	15.339	166	308	0.101	ng	98
20) 4,6-Dinitro-2-methylph...	15.435	198	33	0.087	ng	# 18
21) 4-Bromophenyl-phenylether	16.243	248	97	0.099	ng	# 91
22) Hexachlorobenzene	16.354	284	125	0.107	ng	95
23) Atrazine	16.516	200	96	0.100	ng	# 68
24) Pentachlorophenol	16.702	266	62	0.103	ng	# 85
25) Phenanthrene	17.074	178	500	0.103	ng	99
26) Anthracene	17.173	178	419	0.097	ng	98
28) Fluoranthene	19.104	202	587	0.097	ng	98
30) Pyrene	19.466	202	611	0.098	ng	99
32) Benzo(a)anthracene	21.214	228	559	0.097	ng	# 83
33) Chrysene	21.268	228	590	0.092	ng	# 89
34) Bis(2-ethylhexyl)phtha...	21.161	149	495	0.113	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.686	276	907	0.093	ng	# 88
37) Benzo(b)fluoranthene	22.791	252	699	0.097	ng	# 54
38) Benzo(k)fluoranthene	22.832	252	757m	0.105	ng	
39) Benzo(a)pyrene	23.356	252	571	0.091	ng	# 53
40) Dibenzo(a,h)anthracene	25.703	278	678	0.088	ng	# 54
41) Benzo(g,h,i)perylene	26.367	276	838	0.096	ng	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036873.D
Acq On : 11 Apr 2025 11:42
Operator : RC/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Apr 11 15:34:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 15:32:59 2025
Response via : Initial Calibration

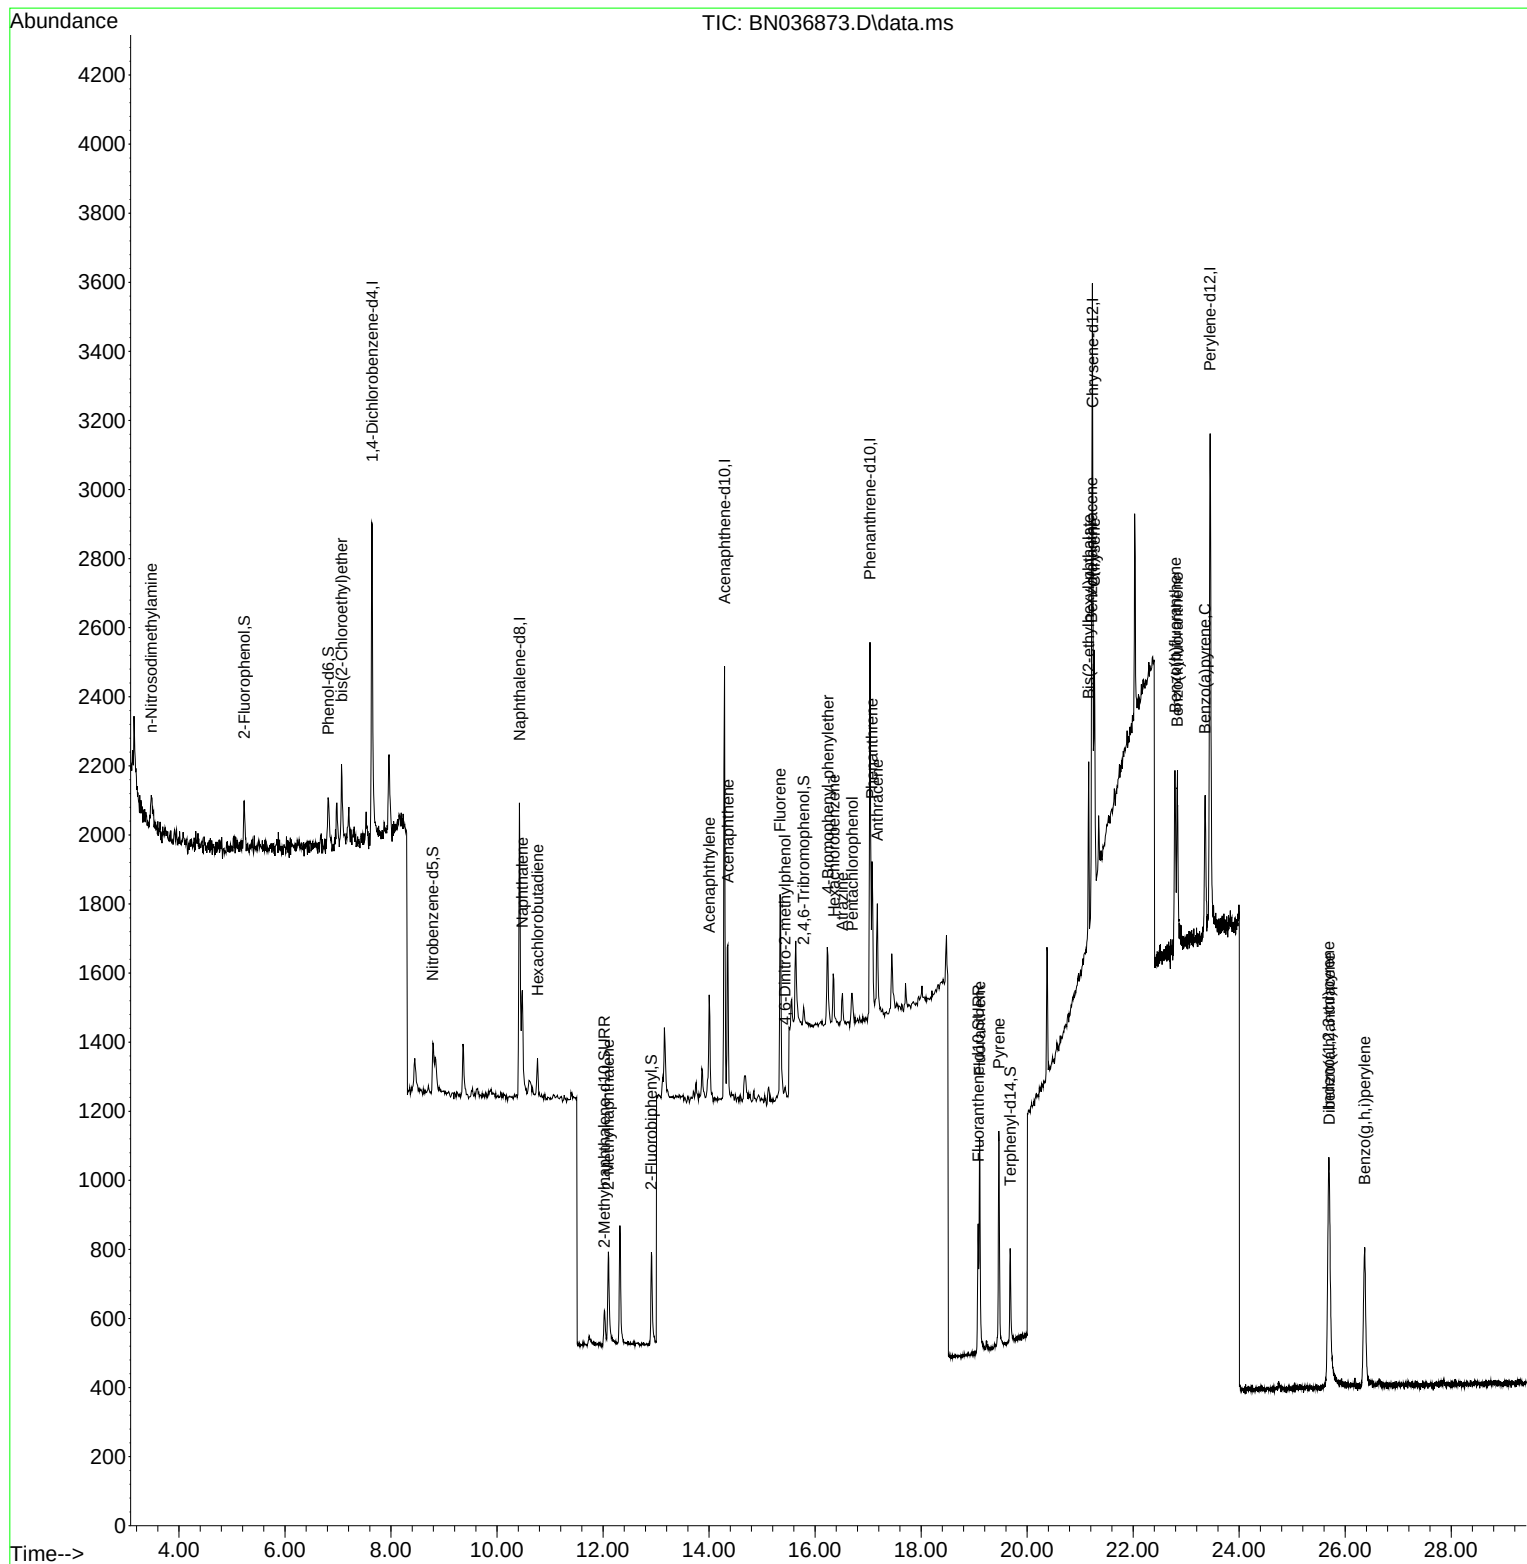



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.645 min Scan# 61

Delta R.T. 0.005 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:152 Resp: 496

Ion Ratio Lower Upper

152 100

150 147.6 123.0 184.6

115 76.5 60.1 90.1



#3

n-Nitrosodimethylamine

Concen: 0.098 ng

RT: 3.478 min Scan# 55

Delta R.T. 0.005 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion: 42 Resp: 127


Ion Ratio Lower Upper

42 100

74 94.5 54.6 81.8#

44 0.0 0.0 0.0

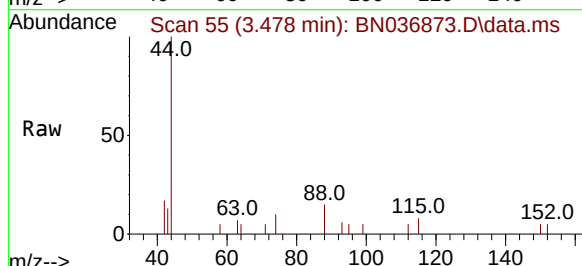



#4

2-Fluorophenol

Concen: 0.105 ng

RT: 5.233 min Scan# 24

Delta R.T. 0.005 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:112 Resp: 124

Ion Ratio Lower Upper

112 100

64 81.5 54.0 81.0#

63 46.0 35.1 52.7



#5

Phenol-d6

Concen: 0.109 ng

RT: 6.814 min Scan# 517

Delta R.T. -0.002 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion: 99 Resp: 163


Ion Ratio Lower Upper

99 100

42 35.0 30.9 46.3

71 41.7 38.6 58.0




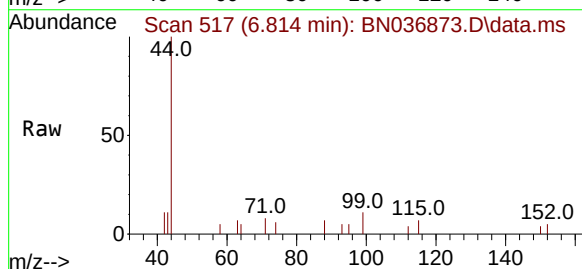




#6
bis(2-Chloroethyl)ether
Concen: 0.123 ng
RT: 7.067 min Scan# 51
Delta R.T. -0.002 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 93 Resp: 183
Ion Ratio Lower Upper
93 100
63 83.1 76.4 114.6
95 37.7 26.1 39.1



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.424 min Scan# 922
Delta R.T. -0.002 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion: 136 Resp: 1266
Ion Ratio Lower Upper
136 100
137 17.7 13.5 20.3
54 19.8 12.8 19.2#
68 13.3 10.1 15.1









#8
Nitrobenzene-d5
Concen: 0.128 ng
RT: 8.790 min Scan# 797
Delta R.T. -0.002 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion	82	Resp:	182
Ion Ratio	Lower	Upper	
82	100		
128	61.9	35.5	53.3#
54	85.8	56.2	84.4#



#9
Naphthalene
Concen: 0.115 ng
RT: 10.477 min Scan# 927
Delta R.T. 0.009 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion	128	Resp:	423
Ion Ratio	Lower	Upper	
128	100		
129	27.1	12.9	19.3#
127	29.9	15.0	22.6#





#10

Hexachlorobutadiene

Concen: 0.113 ng

RT: 10.765 min Scan# 91

Delta R.T. -0.002 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:225 Resp: 95

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 55.8 50.5 75.7



#11

2-Methylnaphthalene-d10

Concen: 0.103 ng

RT: 12.025 min Scan# 1125

Delta R.T. 0.004 min

Lab File: BN036873.D




Acq: 11 Apr 2025 11:42


Tgt Ion:152 Resp: 190

Ion Ratio Lower Upper

152 100

151 20.5 17.8 26.8





#12

2-Methylnaphthalene

Concen: 0.108 ng

RT: 12.101 min Scan# 1168

Delta R.T. 0.004 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:142 Resp: 254

Ion Ratio Lower Upper

142 100

141 94.4 73.8 110.8

115 65.6 43.3 64.9#



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.291 min Scan# 1439

Delta R.T. 0.004 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion:164 Resp: 727


Ion Ratio Lower Upper

164 100

162 107.2 85.7 128.5

160 58.1 46.9 70.3

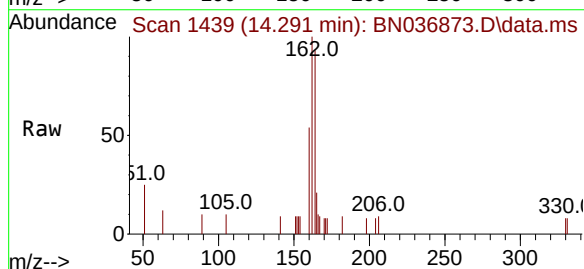



#14

2,4,6-Tribromophenol

Concen: 0.111 ng

RT: 15.783 min Scan# 11

Delta R.T. 0.004 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:330 Resp: 39

Ion Ratio Lower Upper

330 100

332 87.2 87.0 130.6

141 61.5 45.3 67.9



#15

2-Fluorobiphenyl

Concen: 0.107 ng

RT: 12.912 min Scan# 1300

Delta R.T. 0.004 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion:172 Resp: 375


Ion Ratio Lower Upper

172 100

171 53.9 32.7 49.1#

170 42.5 23.3 34.9#









#16
Acenaphthylene
Concen: 0.105 ng
RT: 14.003 min Scan# 1441
Delta R.T. -0.007 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 356
Ion Ratio Lower Upper
152 100
151 21.1 16.4 24.6
153 16.6 10.3 15.5#



#17
Acenaphthene
Concen: 0.101 ng
RT: 14.356 min Scan# 1445
Delta R.T. 0.004 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion:154 Resp: 223
Ion Ratio Lower Upper
154 100
153 124.7 97.8 146.6
152 64.1 52.7 79.1




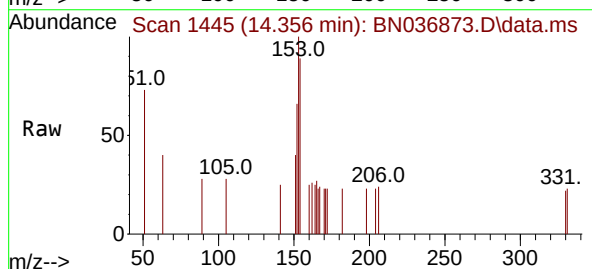




#18
Fluorene
Concen: 0.101 ng
RT: 15.339 min Scan# 11
Delta R.T. -0.007 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:166 Resp: 308
Ion Ratio Lower Upper
166 100
165 102.6 83.2 124.8
167 16.6 11.1 16.7



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.037 min Scan# 1676
Delta R.T. 0.004 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion:188 Resp: 1622
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 17.3 13.9 20.9









#20
4,6-Dinitro-2-methylphenol
Concen: 0.087 ng
RT: 15.435 min Scan# 1611
Delta R.T. 0.004 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:198 Resp: 33
Ion Ratio Lower Upper
198 100
51 250.0 107.6 161.4#
105 110.7 55.2 82.8#



#21
4-Bromophenyl-phenylether
Concen: 0.099 ng
RT: 16.243 min Scan# 1612
Delta R.T. 0.004 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion:248 Resp: 97
Ion Ratio Lower Upper
248 100
250 102.1 83.5 125.3
141 84.0 55.3 82.9#

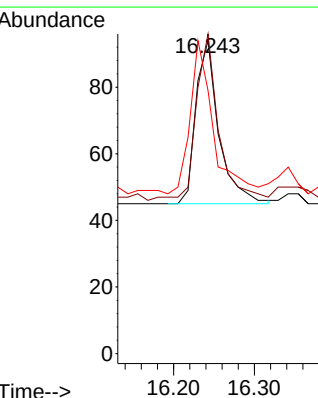



#22

Hexachlorobenzene

Concen: 0.107 ng

RT: 16.354 min Scan# 1621

Delta R.T. 0.004 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:284 Resp: 125

Ion Ratio Lower Upper

284 100

142 49.6 37.7 56.5

249 40.8 29.0 43.6

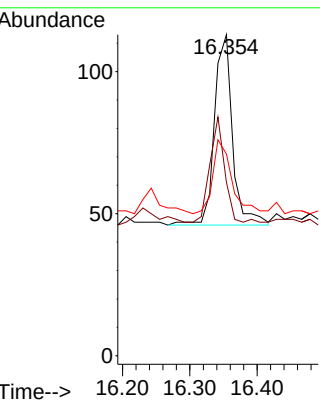

#23

Atrazine

Concen: 0.100 ng

RT: 16.516 min Scan# 1634

Delta R.T. 0.004 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion:200 Resp: 96


Ion Ratio Lower Upper

200 100

173 59.8 28.6 43.0#

215 68.0 40.5 60.7#



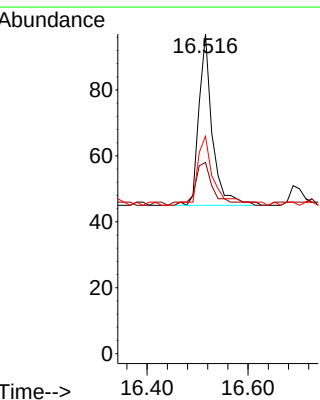





#24
Pentachlorophenol
Concen: 0.103 ng
RT: 16.702 min Scan# 1679
Delta R.T. 0.004 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:266 Resp: 62
Ion Ratio Lower Upper
266 100
264 69.4 44.6 66.8#
268 74.2 51.8 77.6



#25
Phenanthrene
Concen: 0.103 ng
RT: 17.074 min Scan# 1679
Delta R.T. -0.009 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion:178 Resp: 500
Ion Ratio Lower Upper
178 100
176 20.2 16.6 25.0
179 16.0 12.8 19.2









#26
Anthracene
Concen: 0.097 ng
RT: 17.173 min Scan# 1
Delta R.T. 0.004 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion	Ratio	Lower	Upper
178	100		
176	20.5	15.8	23.6
179	16.7	12.6	18.8



#27
Fluoranthene-d10
Concen: 0.098 ng
RT: 19.076 min Scan# 1916
Delta R.T. 0.004 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion	Ratio	Lower	Upper
212	100		
106	14.8	11.2	16.8
104	9.6	7.5	11.3









#28
Fluoranthene
Concen: 0.097 ng
RT: 19.104 min Scan# 1951
Delta R.T. -0.001 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:202 Resp: 587
Ion Ratio Lower Upper
202 100
101 11.8 8.5 12.7
203 17.9 13.8 20.6



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.232 min Scan# 2253
Delta R.T. -0.001 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion:240 Resp: 1643
Ion Ratio Lower Upper
240 100
120 21.4 15.8 23.6
236 34.4 25.8 38.8

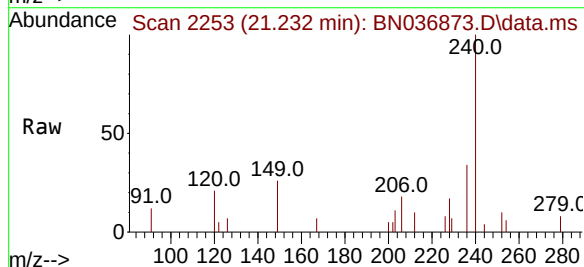



#30

Pyrene

Concen: 0.098 ng

RT: 19.466 min Scan# 2029

Delta R.T. -0.001 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:202 Resp: 611

Ion Ratio Lower Upper

202 100

200 21.1 17.1 25.7

203 17.2 14.5 21.7



#31

Terphenyl-d14

Concen: 0.097 ng

RT: 19.680 min Scan# 2046

Delta R.T. -0.001 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion:244 Resp: 305


Ion Ratio Lower Upper

244 100

212 29.2 11.6 17.4#

122 36.7 14.9 22.3#





#32

Benzo(a)anthracene

Concen: 0.097 ng

RT: 21.214 min Scan# 21

Delta R.T. -0.001 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:228 Resp: 559

Ion Ratio Lower Upper

228 100

226 39.6 24.5 36.7#

229 30.5 17.7 26.5#



#33

Chrysene

Concen: 0.092 ng

RT: 21.268 min Scan# 2257

Delta R.T. -0.001 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion:228 Resp: 590


Ion Ratio Lower Upper

228 100

226 38.1 26.1 39.1

229 27.3 17.0 25.4#









#34
Bis(2-ethylhexyl)phthalate
Concen: 0.113 ng
RT: 21.161 min Scan# 2116
Delta R.T. -0.001 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:149 Resp: 495
Ion Ratio Lower Upper
149 100
167 25.9 21.0 31.4
279 6.9 3.6 5.4#



#35
Perylene-d12
Concen: 0.400 ng
RT: 23.452 min Scan# 2742
Delta R.T. -0.004 min
Lab File: BN036873.D
Acq: 11 Apr 2025 11:42

Tgt Ion:264 Resp: 2037
Ion Ratio Lower Upper
264 100
260 30.7 22.9 34.3
265 112.3 88.6 132.8





#36

Indeno(1,2,3-cd)pyrene

Concen: 0.093 ng

RT: 25.686 min Scan# 3506

Delta R.T. -0.001 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:276 Resp: 907

Ion Ratio Lower Upper

276 100

138 25.4 21.0 31.6

277 12.7 19.3 28.9#



#37

Benzo(b)fluoranthene

Concen: 0.097 ng

RT: 22.791 min Scan# 2516

Delta R.T. 0.002 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion:252 Resp: 699


Ion Ratio Lower Upper

252 100

253 58.5 27.0 40.6#

125 45.7 17.7 26.5#





#38

Benzo(k)fluoranthene

Concen: 0.105 ng m

RT: 22.832 min Scan# 21

Delta R.T. -0.001 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:252 Resp: 757

Ion Ratio Lower Upper

252 100

253 59.5 26.7 40.1#

125 43.9 16.9 25.3#



#39

Benzo(a)pyrene

Concen: 0.091 ng

RT: 23.356 min Scan# 2709

Delta R.T. -0.001 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion:252 Resp: 571


Ion Ratio Lower Upper

252 100

253 64.3 31.5 47.3#

125 57.4 22.6 34.0#





#40

Dibenzo(a,h)anthracene

Concen: 0.088 ng

RT: 25.703 min Scan# 31

Delta R.T. 0.002 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:278 Resp: 678

Ion Ratio Lower Upper

278 100

139 37.0 17.6 26.4#

279 65.3 26.7 40.1#



#41

Benzo(g,h,i)perylene

Concen: 0.096 ng

RT: 26.367 min Scan# 3739

Delta R.T. 0.005 min

Lab File: BN036873.D

Acq: 11 Apr 2025 11:42




Tgt Ion:276 Resp: 838

Ion Ratio Lower Upper

276 100

277 39.0 21.8 32.8#

138 36.5 21.6 32.4#



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036874.D
 Acq On : 11 Apr 2025 12:37
 Operator : RC/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Apr 11 15:35:02 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 15:32:59 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	357	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	936	0.400	ng	0.00
13) Acenaphthene-d10	14.288	164	543	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	1263	0.400	ng	0.00
29) Chrysene-d12	21.233	240	1230	0.400	ng	# 0.00
35) Perylene-d12	23.456	264	1607	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	168	0.198	ng	0.00
5) Phenol-d6	6.817	99	214	0.198	ng	0.00
8) Nitrobenzene-d5	8.792	82	205	0.195	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	264	0.193	ng	0.00
14) 2,4,6-Tribromophenol	15.792	330	51	0.194	ng	0.01
15) 2-Fluorobiphenyl	12.914	172	505	0.192	ng	0.00
27) Fluoranthene-d10	19.077	212	669	0.189	ng	0.00
31) Terphenyl-d14	19.681	244	462	0.196	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	105	0.249	ng	99
3) n-Nitrosodimethylamine	3.473	42	195	0.210	ng	# 92
6) bis(2-Chloroethyl)ether	7.069	93	184	0.172	ng	85
9) Naphthalene	10.468	128	534	0.196	ng	# 78
10) Hexachlorobutadiene	10.767	225	122	0.196	ng	# 97
12) 2-Methylnaphthalene	12.097	142	329	0.189	ng	95
16) Acenaphthylene	14.010	152	491	0.195	ng	99
17) Acenaphthene	14.352	154	319	0.194	ng	99
18) Fluorene	15.346	166	461	0.203	ng	94
20) 4,6-Dinitro-2-methylph...	15.432	198	53	0.179	ng	# 56
21) 4-Bromophenyl-phenylether	16.239	248	145	0.191	ng	91
22) Hexachlorobenzene	16.351	284	185	0.204	ng	97
23) Atrazine	16.512	200	147	0.196	ng	# 67
24) Pentachlorophenol	16.698	266	97	0.207	ng	93
25) Phenanthrene	17.083	178	690	0.182	ng	99
26) Anthracene	17.170	178	631	0.188	ng	96
28) Fluoranthene	19.105	202	887	0.187	ng	99
30) Pyrene	19.468	202	930	0.199	ng	98
32) Benzo(a)anthracene	21.224	228	843	0.195	ng	93
33) Chrysene	21.269	228	964	0.200	ng	94
34) Bis(2-ethylhexyl)phtha...	21.162	149	736	0.225	ng	97
36) Indeno(1,2,3-cd)pyrene	25.693	276	1449	0.189	ng	# 84
37) Benzo(b)fluoranthene	22.793	252	1027	0.181	ng	# 75
38) Benzo(k)fluoranthene	22.836	252	1046	0.183	ng	# 71
39) Benzo(a)pyrene	23.357	252	927	0.186	ng	# 67
40) Dibenzo(a,h)anthracene	25.702	278	1138	0.188	ng	# 77
41) Benzo(g,h,i)perylene	26.368	276	1344	0.195	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036874.D
Acq On : 11 Apr 2025 12:37
Operator : RC/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Apr 11 15:35:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 15:32:59 2025
Response via : Initial Calibration




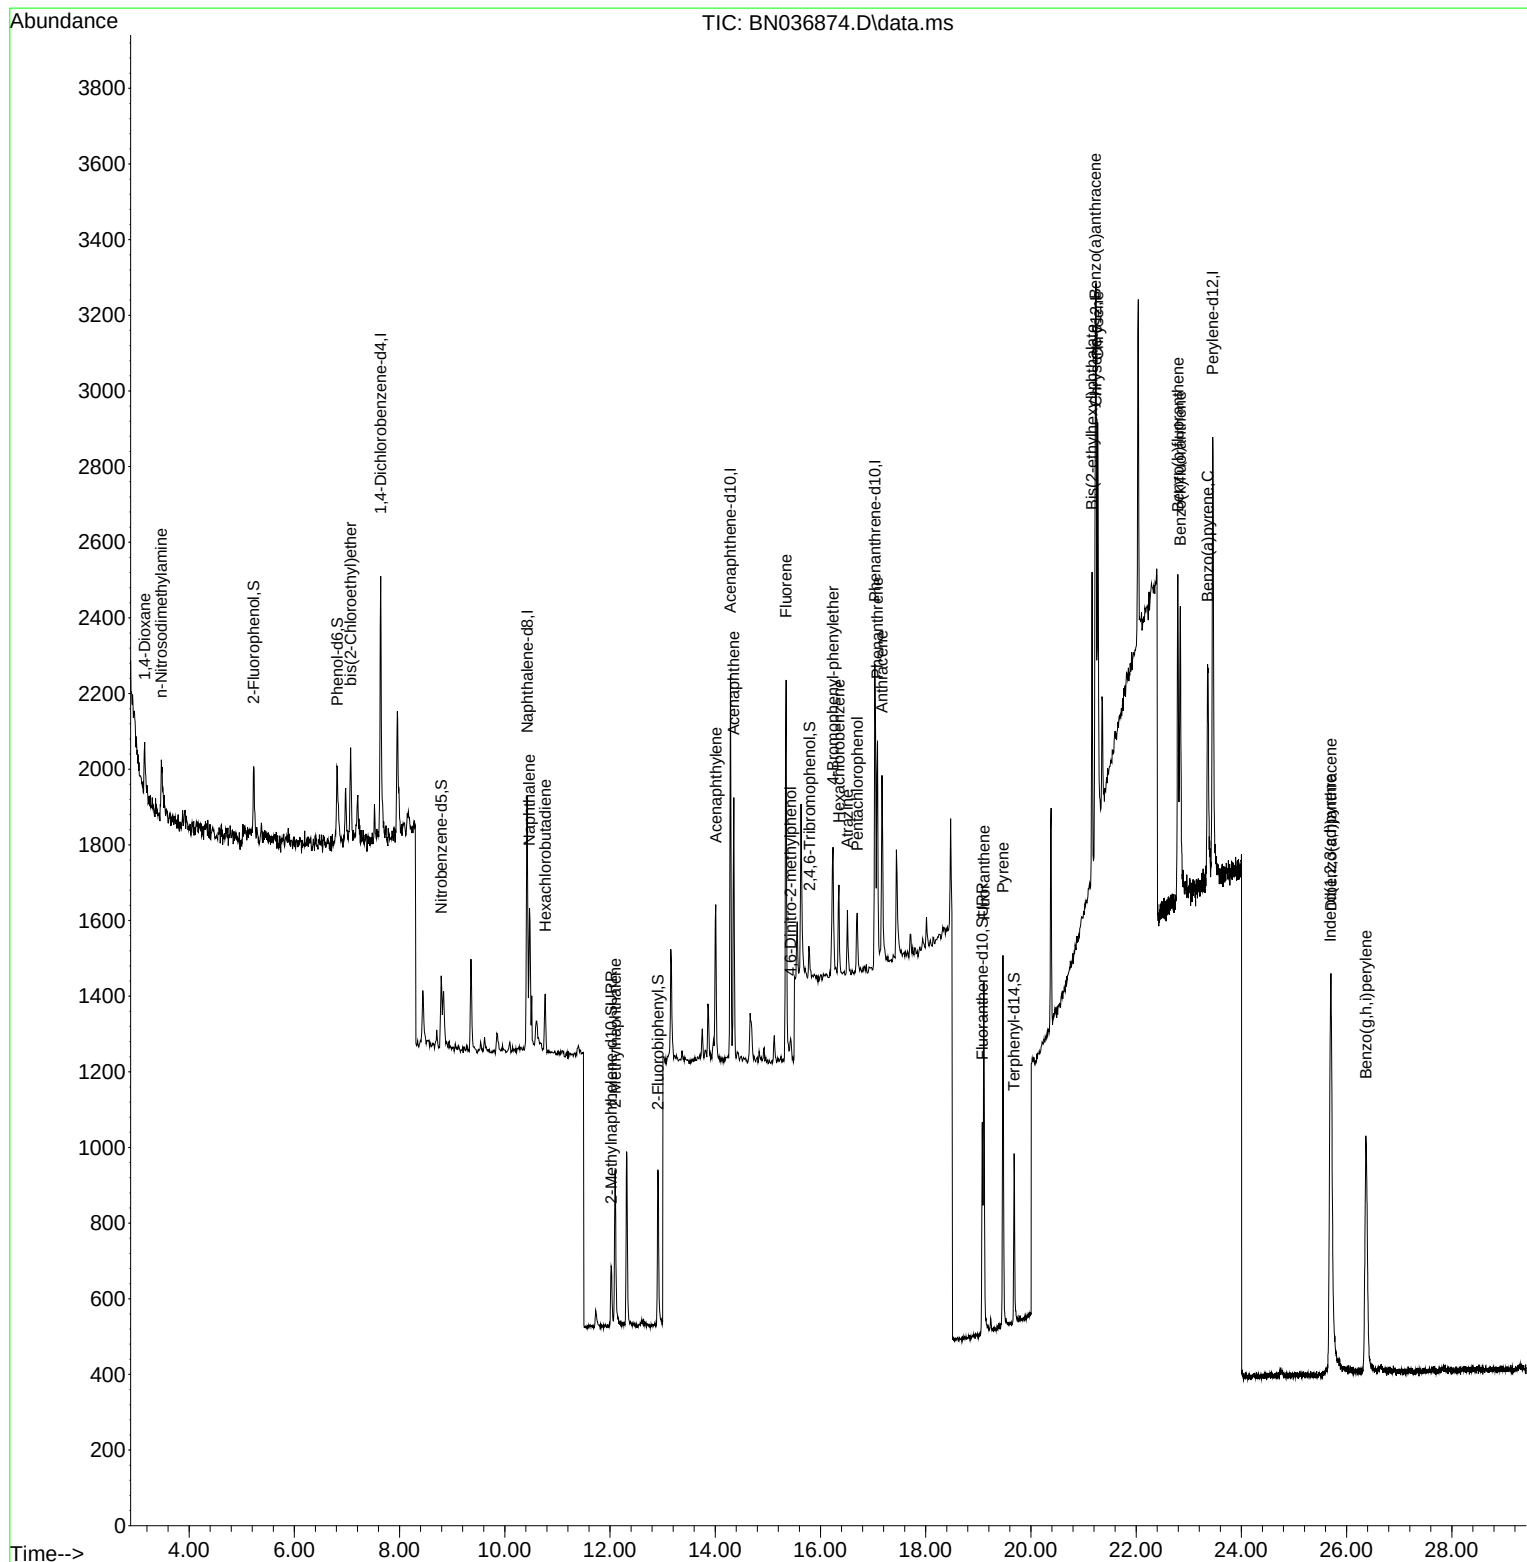




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:152 Resp: 357
Ion Ratio Lower Upper
152 100
150 137.6 123.0 184.6
115 73.4 60.1 90.1



#2
1,4-Dioxane
Concen: 0.249 ng
RT: 3.155 min Scan# 38
Delta R.T. -0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion: 88 Resp: 105
Ion Ratio Lower Upper
88 100
43 49.5 39.2 58.8
58 79.0 63.5 95.3









#3
n-Nitrosodimethylamine
Concen: 0.210 ng
RT: 3.473 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion: 42 Resp: 195
Ion Ratio Lower Upper
42 100
74 62.1 54.6 81.8
44 11.3 0.0 0.0#



#4
2-Fluorophenol
Concen: 0.198 ng
RT: 5.228 min Scan# 325
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion: 112 Resp: 168
Ion Ratio Lower Upper
112 100
64 70.8 54.0 81.0
63 44.6 35.1 52.7









#5
Phenol-d6
Concen: 0.198 ng
RT: 6.817 min Scan# 545
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion: 99 Resp: 214
Ion Ratio Lower Upper
99 100
42 43.0 30.9 46.3
71 48.6 38.6 58.0



#6
bis(2-Chloroethyl)ether
Concen: 0.172 ng
RT: 7.069 min Scan# 580
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion: 93 Resp: 184
Ion Ratio Lower Upper
93 100
63 113.6 76.4 114.6
95 35.3 26.1 39.1









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:	136	Resp:	936
Ion	Ratio	Lower	Upper
136	100		
137	18.6	13.5	20.3
54	18.6	12.8	19.2
68	13.9	10.1	15.1



#8
Nitrobenzene-d5
Concen: 0.195 ng
RT: 8.792 min Scan# 797
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion:	82	Resp:	205
Ion	Ratio	Lower	Upper
82	100		
128	60.6	35.5	53.3
54	79.6	56.2	84.4





#9
Naphthalene

Concen: 0.196 ng

RT: 10.468 min Scan# 954

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37





Instrument :

BN036874.D

ClientSampleId :

SSTDICC0.2

Tgt Ion:	128	Resp:	534
Ion	Ratio	Lower	Upper
128	100		
129	25.7	12.9	19.3#
127	28.3	15.0	22.6#



#10

Hexachlorobutadiene

Concen: 0.196 ng




RT: 10.767 min Scan# 982


Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Tgt Ion:	225	Resp:	122
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	60.7	50.5	75.7









#11
2-Methylnaphthalene-d10
Concen: 0.193 ng
RT: 12.021 min Scan# 1153
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:152 Resp: 264
Ion Ratio Lower Upper
152 100
151 22.3 17.8 26.8



#12
2-Methylnaphthalene
Concen: 0.189 ng
RT: 12.097 min Scan# 1168
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion:142 Resp: 329
Ion Ratio Lower Upper
142 100
141 92.8 73.8 110.8
115 63.1 43.3 64.9





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.288 min Scan# 14

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.2





Tgt Ion:164 Resp: 543

Ion Ratio Lower Upper

164 100

162 111.4 85.7 128.5

160 60.9 46.9 70.3



#14

2,4,6-Tribromophenol

Concen: 0.194 ng

RT: 15.792 min Scan# 1604

Delta R.T. 0.012 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37




Tgt Ion:330 Resp: 51


Ion Ratio Lower Upper

330 100

332 94.1 87.0 130.6

141 47.1 45.3 67.9









#15
2-Fluorobiphenyl
Concen: 0.192 ng
RT: 12.914 min Scan# 1329
Delta R.T. 0.005 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:172 Resp: 505
Ion Ratio Lower Upper
172 100
171 46.1 32.7 49.1
170 35.6 23.3 34.9#



#16
Acenaphthylene
Concen: 0.195 ng
RT: 14.010 min Scan# 1441
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion:152 Resp: 491
Ion Ratio Lower Upper
152 100
151 21.0 16.4 24.6
153 12.8 10.3 15.5









#17
Acenaphthene
Concen: 0.194 ng
RT: 14.352 min Scan# 1473
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:154 Resp: 319
Ion Ratio Lower Upper
154 100
153 121.6 97.8 146.6
152 64.6 52.7 79.1



#18
Fluorene
Concen: 0.203 ng
RT: 15.346 min Scan# 1566
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion:166 Resp: 461
Ion Ratio Lower Upper
166 100
165 97.8 83.2 124.8
167 13.2 11.1 16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:188 Resp: 1263

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 19.6 13.9 20.9



#20

4,6-Dinitro-2-methylphenol

Concen: 0.179 ng

RT: 15.432 min Scan# 1574

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37




Tgt Ion:198 Resp: 53


Ion Ratio Lower Upper

198 100

51 191.0 107.6 161.4#

105 98.5 55.2 82.8#









#21
4-Bromophenyl-phenylether
Concen: 0.191 ng
RT: 16.239 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion	Ratio	Lower	Upper
248	100		
250	94.0	83.5	125.3
141	75.4	55.3	82.9



#22
Hexachlorobenzene
Concen: 0.204 ng
RT: 16.351 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion	Ratio	Lower	Upper
284	100		
142	47.0	37.7	56.5
249	40.5	29.0	43.6









#23
Atrazine
Concen: 0.196 ng
RT: 16.512 min Scan# 1662
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:200 Resp: 147
Ion Ratio Lower Upper
200 100
173 57.9 28.6 43.0#
215 71.1 40.5 60.7#

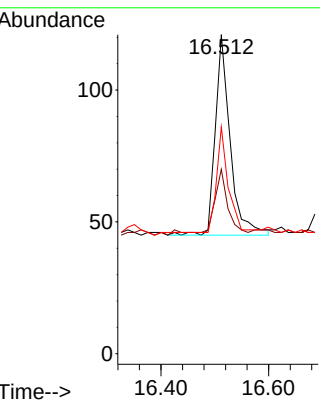

#24
Pentachlorophenol
Concen: 0.207 ng
RT: 16.698 min Scan# 1677
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion:266 Resp: 97
Ion Ratio Lower Upper
266 100
264 50.5 44.6 66.8
268 58.8 51.8 77.6

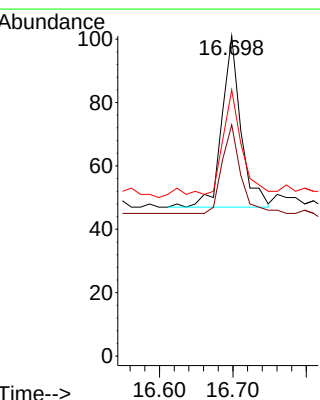



#25

Phenanthrene

Concen: 0.182 ng

RT: 17.083 min Scan# 1708

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:178 Resp: 690

Ion Ratio Lower Upper

178 100

176 19.9 16.6 25.0

179 16.2 12.8 19.2



#26

Anthracene

Concen: 0.188 ng

RT: 17.170 min Scan# 1715

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37




Tgt Ion:178 Resp: 631


Ion Ratio Lower Upper

178 100

176 16.8 15.8 23.6

179 15.2 12.6 18.8





#27

Fluoranthene-d10

Concen: 0.189 ng

RT: 19.077 min Scan# 1944

Delta R.T. 0.005 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:212 Resp: 669

Ion Ratio Lower Upper

212 100

106 13.8 11.2 16.8

104 9.7 7.5 11.3



#28

Fluoranthene

Concen: 0.187 ng

RT: 19.105 min Scan# 1951

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37




Tgt Ion:202 Resp: 887


Ion Ratio Lower Upper

202 100

101 9.9 8.5 12.7

203 17.0 13.8 20.6





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.233 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:240 Resp: 1230

Ion Ratio Lower Upper

240 100

120 26.1 15.8 23.6#

236 34.7 25.8 38.8



#30

Pyrene

Concen: 0.199 ng

RT: 19.468 min Scan# 2029

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37




Tgt Ion:202 Resp: 930


Ion Ratio Lower Upper

202 100

200 21.7 17.1 25.7

203 17.0 14.5 21.7









#31
Terphenyl-d14
Concen: 0.196 ng
RT: 19.681 min Scan# 2075
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:244 Resp: 462
Ion Ratio Lower Upper
244 100
212 22.4 11.6 17.4#
122 28.0 14.9 22.3#



#32
Benzo(a)anthracene
Concen: 0.195 ng
RT: 21.224 min Scan# 2281
Delta R.T. 0.009 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37

Tgt Ion:228 Resp: 843
Ion Ratio Lower Upper
228 100
226 34.0 24.5 36.7
229 26.3 17.7 26.5





#33

Chrysene

Concen: 0.200 ng

RT: 21.269 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:228 Resp: 964

Ion Ratio Lower Upper

228 100

226 36.1 26.1 39.1

229 24.1 17.0 25.4



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.225 ng

RT: 21.162 min Scan# 2274

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37




Tgt Ion:149 Resp: 736


Ion Ratio Lower Upper

149 100

167 24.6 21.0 31.4


279 4.8 3.6 5.4








#35
Perylene-d12
Concen: 0.400 ng
RT: 23.456 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37


Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2





Tgt Ion:264 Resp: 1607
Ion Ratio Lower Upper
264 100
260 29.3 22.9 34.3
265 133.3 88.6 132.8#




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.189 ng
RT: 25.693 min Scan# 3537
Delta R.T. 0.006 min
Lab File: BN036874.D
Acq: 11 Apr 2025 12:37



Tgt Ion:276 Resp: 1449
Ion Ratio Lower Upper
276 100
138 10.6 21.0 31.6#
277 24.2 19.3 28.9





#37

Benzo(b)fluoranthene

Concen: 0.181 ng

RT: 22.793 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:252 Resp: 1027

Ion Ratio Lower Upper

252 100

253 48.2 27.0 40.6#

125 34.3 17.7 26.5#



#38

Benzo(k)fluoranthene

Concen: 0.183 ng

RT: 22.836 min Scan# 2560

Delta R.T. 0.003 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37




Tgt Ion:252 Resp: 1046


Ion Ratio Lower Upper

252 100

253 48.1 26.7 40.1#

125 36.7 16.9 25.3#





#39

Benzo(a)pyrene

Concen: 0.186 ng

RT: 23.357 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:252 Resp: 927

Ion Ratio Lower Upper

252 100

253 57.5 31.5 47.3#

125 47.8 22.6 34.0#



#40

Dibenzo(a,h)anthracene

Concen: 0.188 ng

RT: 25.702 min Scan# 3540

Delta R.T. 0.000 min

Lab File: BN036874.D

Acq: 11 Apr 2025 12:37




Tgt Ion:278 Resp: 1138


Ion Ratio Lower Upper

278 100

139 29.5 17.6 26.4#

279 48.9 26.7 40.1#





#41

Benzo(g,h,i)perylene

Concen: 0.195 ng

RT: 26.368 min Scan# 31

Delta R.T. 0.006 min

Lab File: BN036874.D


Acq: 11 Apr 2025 12:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:276 Resp: 1344

Ion Ratio Lower Upper

276 100

277 31.6 21.8 32.8

138 32.9 21.6 32.4#



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036875.D
 Acq On : 11 Apr 2025 13:17
 Operator : RC/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Apr 11 15:35:31 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 15:32:59 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	491	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	1260	0.400	ng	0.00
13) Acenaphthene-d10	14.288	164	744	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	1575	0.400	ng	0.00
29) Chrysene-d12	21.233	240	1627	0.400	ng	0.00
35) Perylene-d12	23.456	264	1897	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	474	0.407	ng	0.00
5) Phenol-d6	6.817	99	588	0.396	ng	0.00
8) Nitrobenzene-d5	8.792	82	568	0.401	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	748	0.407	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	136	0.378	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	1498	0.416	ng	0.00
27) Fluoranthene-d10	19.073	212	1923	0.435	ng	0.00
31) Terphenyl-d14	19.681	244	1326	0.426	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	216	0.372	ng	# 78
3) n-Nitrosodimethylamine	3.473	42	532	0.416	ng	# 97
6) bis(2-Chloroethyl)ether	7.069	93	583	0.397	ng	100
9) Naphthalene	10.468	128	1474	0.403	ng	100
10) Hexachlorobutadiene	10.767	225	358	0.428	ng	# 100
12) 2-Methylnaphthalene	12.097	142	956	0.408	ng	100
16) Acenaphthylene	14.010	152	1407	0.407	ng	100
17) Acenaphthene	14.352	154	918	0.408	ng	100
18) Fluorene	15.346	166	1260	0.405	ng	100
20) 4,6-Dinitro-2-methylph...	15.432	198	150	0.407	ng	100
21) 4-Bromophenyl-phenylether	16.239	248	410	0.432	ng	100
22) Hexachlorobenzene	16.351	284	488	0.432	ng	100
23) Atrazine	16.512	200	414	0.444	ng	100
24) Pentachlorophenol	16.698	266	255	0.436	ng	100
25) Phenanthrene	17.083	178	2044	0.432	ng	100
26) Anthracene	17.170	178	1811	0.432	ng	100
28) Fluoranthene	19.105	202	2529	0.428	ng	100
30) Pyrene	19.467	202	2609	0.421	ng	100
32) Benzo(a)anthracene	21.215	228	2294	0.400	ng	100
33) Chrysene	21.269	228	2715	0.427	ng	100
34) Bis(2-ethylhexyl)phtha...	21.162	149	1665	0.384	ng	100
36) Indeno(1,2,3-cd)pyrene	25.687	276	3833	0.424	ng	100
37) Benzo(b)fluoranthene	22.790	252	2890	0.431	ng	100
38) Benzo(k)fluoranthene	22.833	252	2812	0.417	ng	100
39) Benzo(a)pyrene	23.357	252	2551	0.435	ng	100
40) Dibenzo(a,h)anthracene	25.702	278	3007	0.420	ng	100
41) Benzo(g,h,i)perylene	26.362	276	3425	0.420	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036875.D
Acq On : 11 Apr 2025 13:17
Operator : RC/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Apr 11 15:35:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 15:32:59 2025
Response via : Initial Calibration




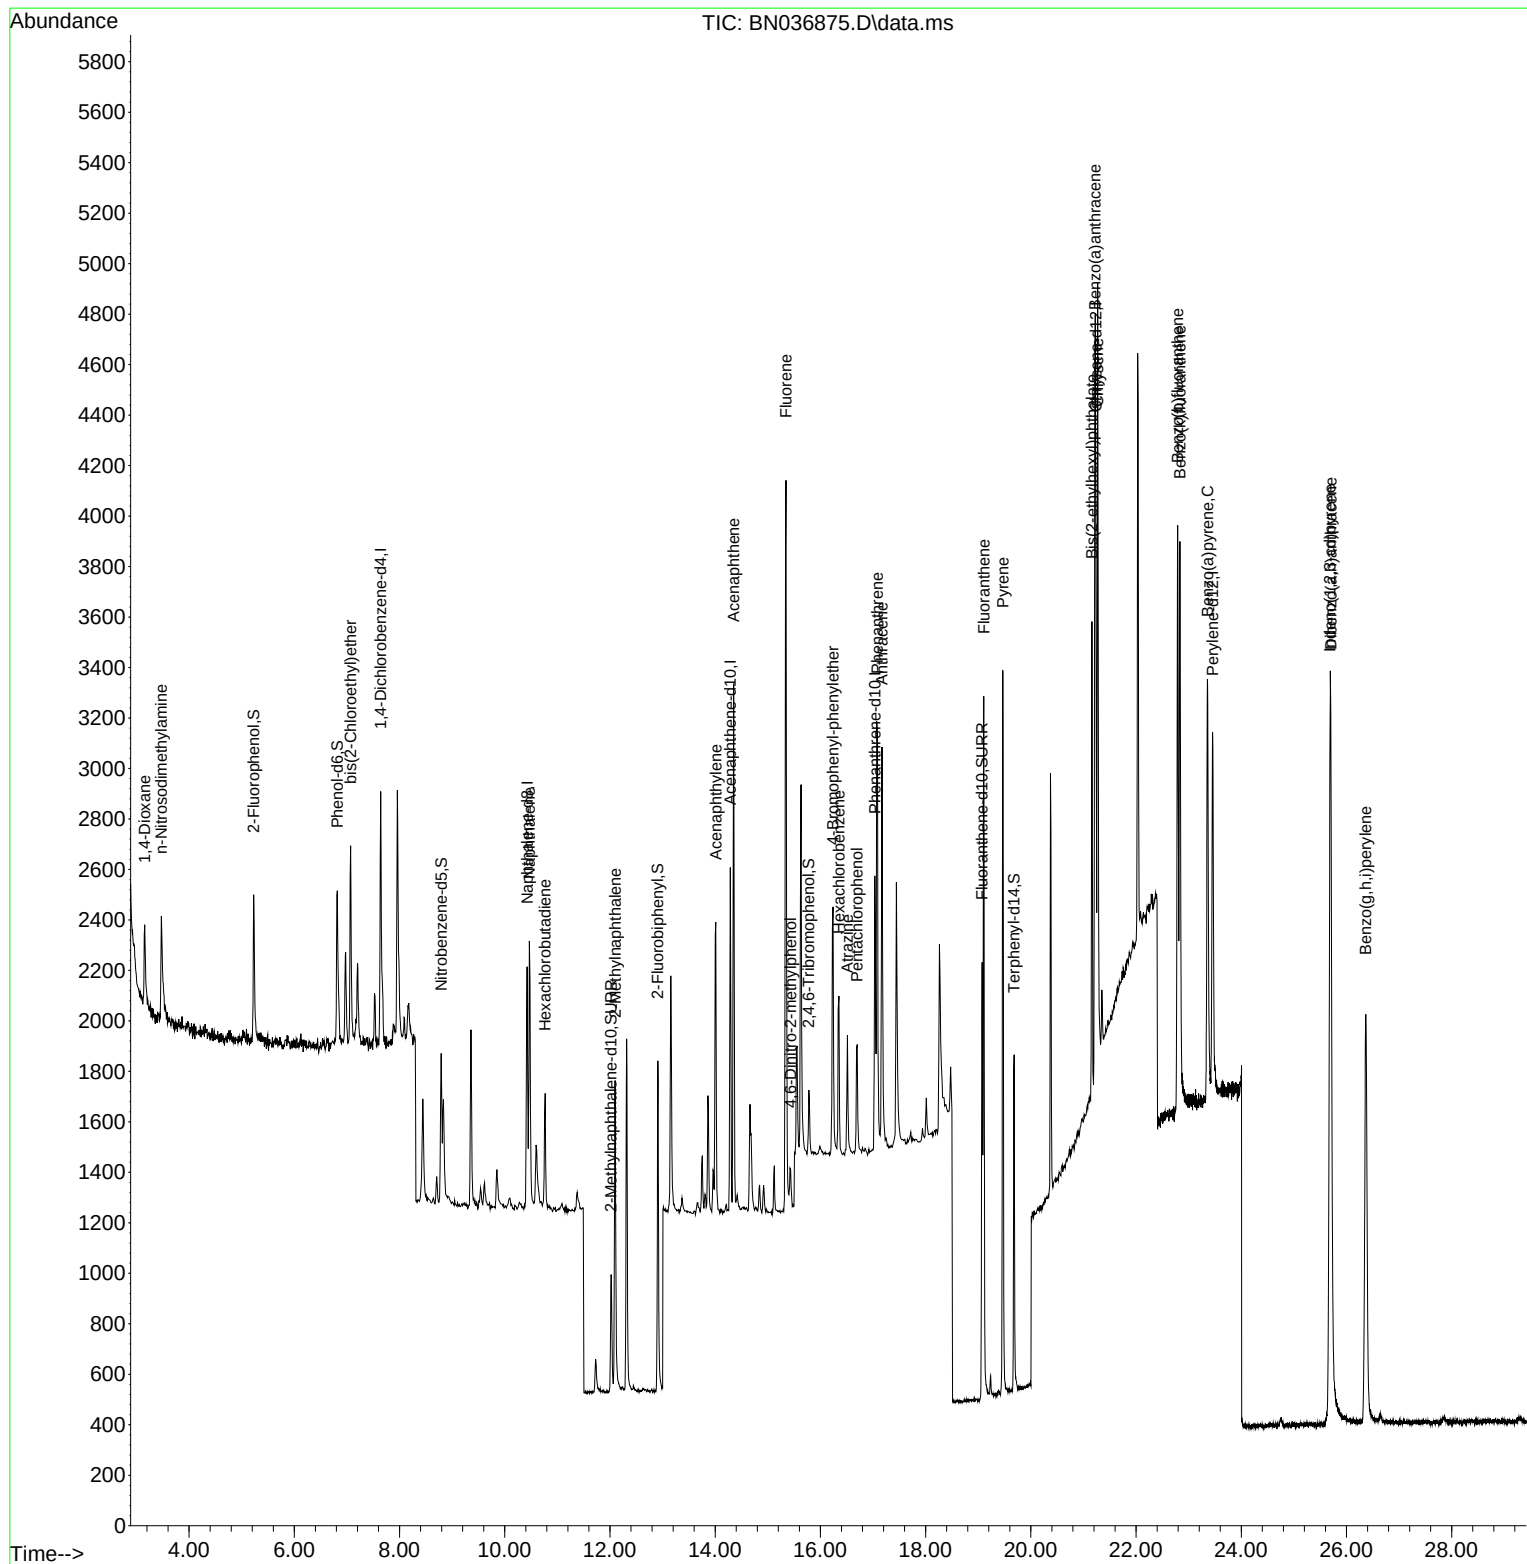




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 659
Delta R.T. -0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 491
Ion Ratio Lower Upper
152 100
150 153.8 123.0 184.6
115 75.1 60.1 90.1



#2
1,4-Dioxane
Concen: 0.372 ng
RT: 3.155 min Scan# 38
Delta R.T. -0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion: 88 Resp: 216
Ion Ratio Lower Upper
88 100
43 61.1 39.2 58.8#
58 100.5 63.5 95.3#









#3
n-Nitrosodimethylamine
Concen: 0.416 ng
RT: 3.473 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 42 Resp: 532
Ion Ratio Lower Upper
42 100
74 65.4 54.6 81.8
44 0.0 0.0 0.0



#4
2-Fluorophenol
Concen: 0.407 ng
RT: 5.228 min Scan# 325
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion: 112 Resp: 474
Ion Ratio Lower Upper
112 100
64 67.5 54.0 81.0
63 43.9 35.1 52.7





#5

Phenol-d6

Concen: 0.396 ng

RT: 6.817 min Scan# 545

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion: 99 Resp: 588

Ion Ratio Lower Upper

99 100

42 38.6 30.9 46.3

71 48.3 38.6 58.0



#6

bis(2-Chloroethyl)ether

Concen: 0.397 ng

RT: 7.069 min Scan# 580

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion: 93 Resp: 583


Ion Ratio Lower Upper

93 100

63 95.5 76.4 114.6

95 32.6 26.1 39.1




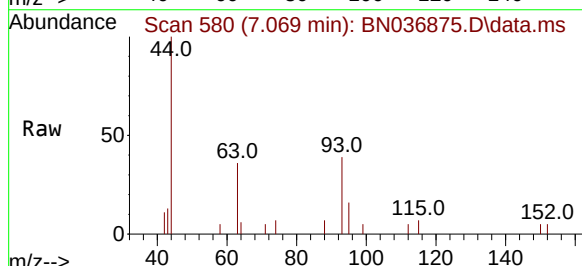




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	1260
Ion	Ratio	Lower	Upper
136	100		
137	16.9	13.5	20.3
54	16.0	12.8	19.2
68	12.6	10.1	15.1



#8
Nitrobenzene-d5
Concen: 0.401 ng
RT: 8.792 min Scan# 797
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion:	82	Resp:	568
Ion	Ratio	Lower	Upper
82	100		
128	44.4	35.5	53.3
54	70.3	56.2	84.4









#9
Naphthalene
Concen: 0.403 ng
RT: 10.468 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	Ratio	Lower	Upper
128	100		
129	16.1	12.9	19.3
127	18.8	15.0	22.6



#10
Hexachlorobutadiene
Concen: 0.428 ng
RT: 10.767 min Scan# 982
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.1	50.5	75.7









#11
2-Methylnaphthalene-d10
Concen: 0.407 ng
RT: 12.021 min Scan# 1153
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 748
Ion Ratio Lower Upper
152 100
151 22.3 17.8 26.8



#12
2-Methylnaphthalene
Concen: 0.408 ng
RT: 12.097 min Scan# 1168
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion:142 Resp: 956
Ion Ratio Lower Upper
142 100
141 92.3 73.8 110.8
115 54.1 43.3 64.9









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	164	Resp	744
Ion	Ratio	Lower	Upper
164	100		
162	107.1	85.7	128.5
160	58.6	46.9	70.3



#14
2,4,6-Tribromophenol
Concen: 0.378 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion	330	Resp	136
Ion	Ratio	Lower	Upper
330	100		
332	108.8	87.0	130.6
141	56.6	45.3	67.9









#15
2-Fluorobiphenyl
Concen: 0.416 ng
RT: 12.909 min Scan# 1328
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	172	Resp:	1498
Ion Ratio	Lower	Upper	
172	100		
171	40.9	32.7	49.1
170	29.1	23.3	34.9



#16
Acenaphthylene
Concen: 0.407 ng
RT: 14.010 min Scan# 1441
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion:	152	Resp:	1407
Ion Ratio	Lower	Upper	
152	100		
151	20.5	16.4	24.6
153	12.9	10.3	15.5





#17

Acenaphthene

Concen: 0.408 ng

RT: 14.352 min Scan# 1473

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:154 Resp: 918

Ion Ratio Lower Upper

154 100

153 122.2 97.8 146.6

152 65.9 52.7 79.1



#18

Fluorene

Concen: 0.405 ng

RT: 15.346 min Scan# 1566

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion:166 Resp: 1260


Ion Ratio Lower Upper

166 100

165 104.0 83.2 124.8

167 13.9 11.1 16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:188 Resp: 1575

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 17.4 13.9 20.9



#20

4,6-Dinitro-2-methylphenol

Concen: 0.407 ng

RT: 15.432 min Scan# 1574

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion:198 Resp: 150


Ion Ratio Lower Upper

198 100

51 134.5 107.6 161.4

105 69.0 55.2 82.8









#21
4-Bromophenyl-phenylether
Concen: 0.432 ng
RT: 16.239 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:248 Resp: 410
Ion Ratio Lower Upper
248 100
250 104.4 83.5 125.3
141 69.1 55.3 82.9



#22
Hexachlorobenzene
Concen: 0.432 ng
RT: 16.351 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion:284 Resp: 488
Ion Ratio Lower Upper
284 100
142 47.1 37.7 56.5
249 36.3 29.0 43.6





#23

Atrazine

Concen: 0.444 ng

RT: 16.512 min Scan# 1662

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:200 Resp: 414

Ion Ratio Lower Upper

200 100

173 35.8 28.6 43.0

215 50.6 40.5 60.7



#24

Pentachlorophenol

Concen: 0.436 ng

RT: 16.698 min Scan# 1677

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion:266 Resp: 255


Ion Ratio Lower Upper

266 100

264 55.7 44.6 66.8

268 64.7 51.8 77.6









#25
Phenanthrene
Concen: 0.432 ng
RT: 17.083 min Scan# 1708
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 2044
Ion Ratio Lower Upper
178 100
176 20.8 16.6 25.0
179 16.0 12.8 19.2



#26
Anthracene
Concen: 0.432 ng
RT: 17.170 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion:178 Resp: 1811
Ion Ratio Lower Upper
178 100
176 19.7 15.8 23.6
179 15.7 12.6 18.8





#27

Fluoranthene-d10

Concen: 0.435 ng

RT: 19.073 min Scan# 1944

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:212 Resp: 1923

Ion Ratio Lower Upper

212 100

106 14.0 11.2 16.8

104 9.4 7.5 11.3



#28

Fluoranthene

Concen: 0.428 ng

RT: 19.105 min Scan# 1951

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion:202 Resp: 2529


Ion Ratio Lower Upper

202 100

101 10.6 8.5 12.7

203 17.2 13.8 20.6





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.233 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:240 Resp: 1627

Ion Ratio Lower Upper

240 100

120 19.7 15.8 23.6

236 32.3 25.8 38.8



#30

Pyrene

Concen: 0.421 ng

RT: 19.467 min Scan# 2029

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion:202 Resp: 2609


Ion Ratio Lower Upper

202 100

200 21.4 17.1 25.7

203 18.1 14.5 21.7









#31
Terphenyl-d14
Concen: 0.426 ng
RT: 19.681 min Scan# 2075
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	Ratio	Lower	Upper
244	100		
212	14.5	11.6	17.4
122	18.6	14.9	22.3



#32
Benzo(a)anthracene
Concen: 0.400 ng
RT: 21.215 min Scan# 2280
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.6	24.5	36.7
229	22.1	17.7	26.5









#33
Chrysene
Concen: 0.427 ng
RT: 21.269 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	Ratio	Lower	Upper
228	100		
226	32.6	26.1	39.1
229	21.2	17.0	25.4



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.384 ng
RT: 21.162 min Scan# 2274
Delta R.T. 0.000 min
Lab File: BN036875.D
Acq: 11 Apr 2025 13:17

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.4	21.0	31.4
279	4.6	3.6	5.4





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.456 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:264 Resp: 1897

Ion Ratio Lower Upper

264 100

260 28.6 22.9 34.3

265 110.7 88.6 132.8



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.424 ng

RT: 25.687 min Scan# 3535

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion:276 Resp: 3833


Ion Ratio Lower Upper

276 100

138 26.3 21.0 31.6

277 24.1 19.3 28.9





#37

Benzo(b)fluoranthene

Concen: 0.431 ng

RT: 22.790 min Scan# 2544

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:252 Resp: 2890

Ion Ratio Lower Upper

252 100

253 33.8 27.0 40.6

125 22.1 17.7 26.5



#38

Benzo(k)fluoranthene

Concen: 0.417 ng

RT: 22.833 min Scan# 2559

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion:252 Resp: 2812


Ion Ratio Lower Upper

252 100

253 33.4 26.7 40.1

125 21.1 16.9 25.3





#39

Benzo(a)pyrene

Concen: 0.435 ng

RT: 23.357 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:252 Resp: 2551

Ion Ratio Lower Upper

252 100

253 39.4 31.5 47.3

125 28.3 22.6 34.0



#40

Dibenzo(a,h)anthracene

Concen: 0.420 ng

RT: 25.702 min Scan# 3540

Delta R.T. 0.000 min

Lab File: BN036875.D

Acq: 11 Apr 2025 13:17




Tgt Ion:278 Resp: 3007


Ion Ratio Lower Upper

278 100

139 22.0 17.6 26.4

279 33.4 26.7 40.1





#41

Benzo(g,h,i)perylene

Concen: 0.420 ng

RT: 26.362 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN036875.D


Acq: 11 Apr 2025 13:17

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:276 Resp: 3425

Ion Ratio Lower Upper

276 100

277 27.3 21.8 32.8

138 27.0 21.6 32.4



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036876.D
 Acq On : 11 Apr 2025 13:53
 Operator : RC/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Apr 11 15:36:01 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 15:32:59 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	666	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	1743	0.400	ng	# 0.00
13) Acenaphthene-d10	14.288	164	1033	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	2266	0.400	ng	# 0.00
29) Chrysene-d12	21.233	240	2195	0.400	ng	# 0.00
35) Perylene-d12	23.450	264	2663	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.235	112	1226	0.775	ng	0.00
5) Phenol-d6	6.817	99	1511	0.750	ng	0.00
8) Nitrobenzene-d5	8.792	82	1392	0.711	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	1932	0.760	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	386	0.774	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	3506	0.701	ng	0.00
27) Fluoranthene-d10	19.073	212	4730	0.743	ng	0.00
31) Terphenyl-d14	19.677	244	3251	0.774	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.162	88	548	0.696	ng	89
3) n-Nitrosodimethylamine	3.473	42	1294	0.746	ng	# 98
6) bis(2-Chloroethyl)ether	7.069	93	1549	0.778	ng	93
9) Naphthalene	10.468	128	3762	0.743	ng	# 91
10) Hexachlorobutadiene	10.767	225	860	0.744	ng	# 99
12) 2-Methylnaphthalene	12.092	142	2453	0.757	ng	97
16) Acenaphthylene	13.999	152	3604	0.751	ng	99
17) Acenaphthene	14.352	154	2400	0.768	ng	95
18) Fluorene	15.336	166	3235	0.750	ng	98
20) 4,6-Dinitro-2-methylph...	15.421	198	418	0.789	ng	85
21) 4-Bromophenyl-phenylether	16.239	248	1037	0.759	ng	# 90
22) Hexachlorobenzene	16.351	284	1187	0.730	ng	97
23) Atrazine	16.512	200	1001	0.746	ng	# 93
24) Pentachlorophenol	16.686	266	588	0.699	ng	94
25) Phenanthrene	17.071	178	5162	0.758	ng	98
26) Anthracene	17.170	178	4492	0.744	ng	99
28) Fluoranthene	19.105	202	6324	0.745	ng	99
30) Pyrene	19.468	202	6482	0.776	ng	99
32) Benzo(a)anthracene	21.215	228	5944	0.769	ng	96
33) Chrysene	21.269	228	6669	0.777	ng	98
34) Bis(2-ethylhexyl)phtha...	21.162	149	4201	0.718	ng	# 99
36) Indeno(1,2,3-cd)pyrene	25.684	276	9671	0.762	ng	98
37) Benzo(b)fluoranthene	22.787	252	7215	0.767	ng	# 86
38) Benzo(k)fluoranthene	22.828	252	7294	0.771	ng	# 87
39) Benzo(a)pyrene	23.354	252	6413	0.778	ng	# 81
40) Dibenzo(a,h)anthracene	25.696	278	7922	0.788	ng	93
41) Benzo(g,h,i)perylene	26.362	276	8703	0.760	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036876.D
Acq On : 11 Apr 2025 13:53
Operator : RC/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Apr 11 15:36:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 15:32:59 2025
Response via : Initial Calibration




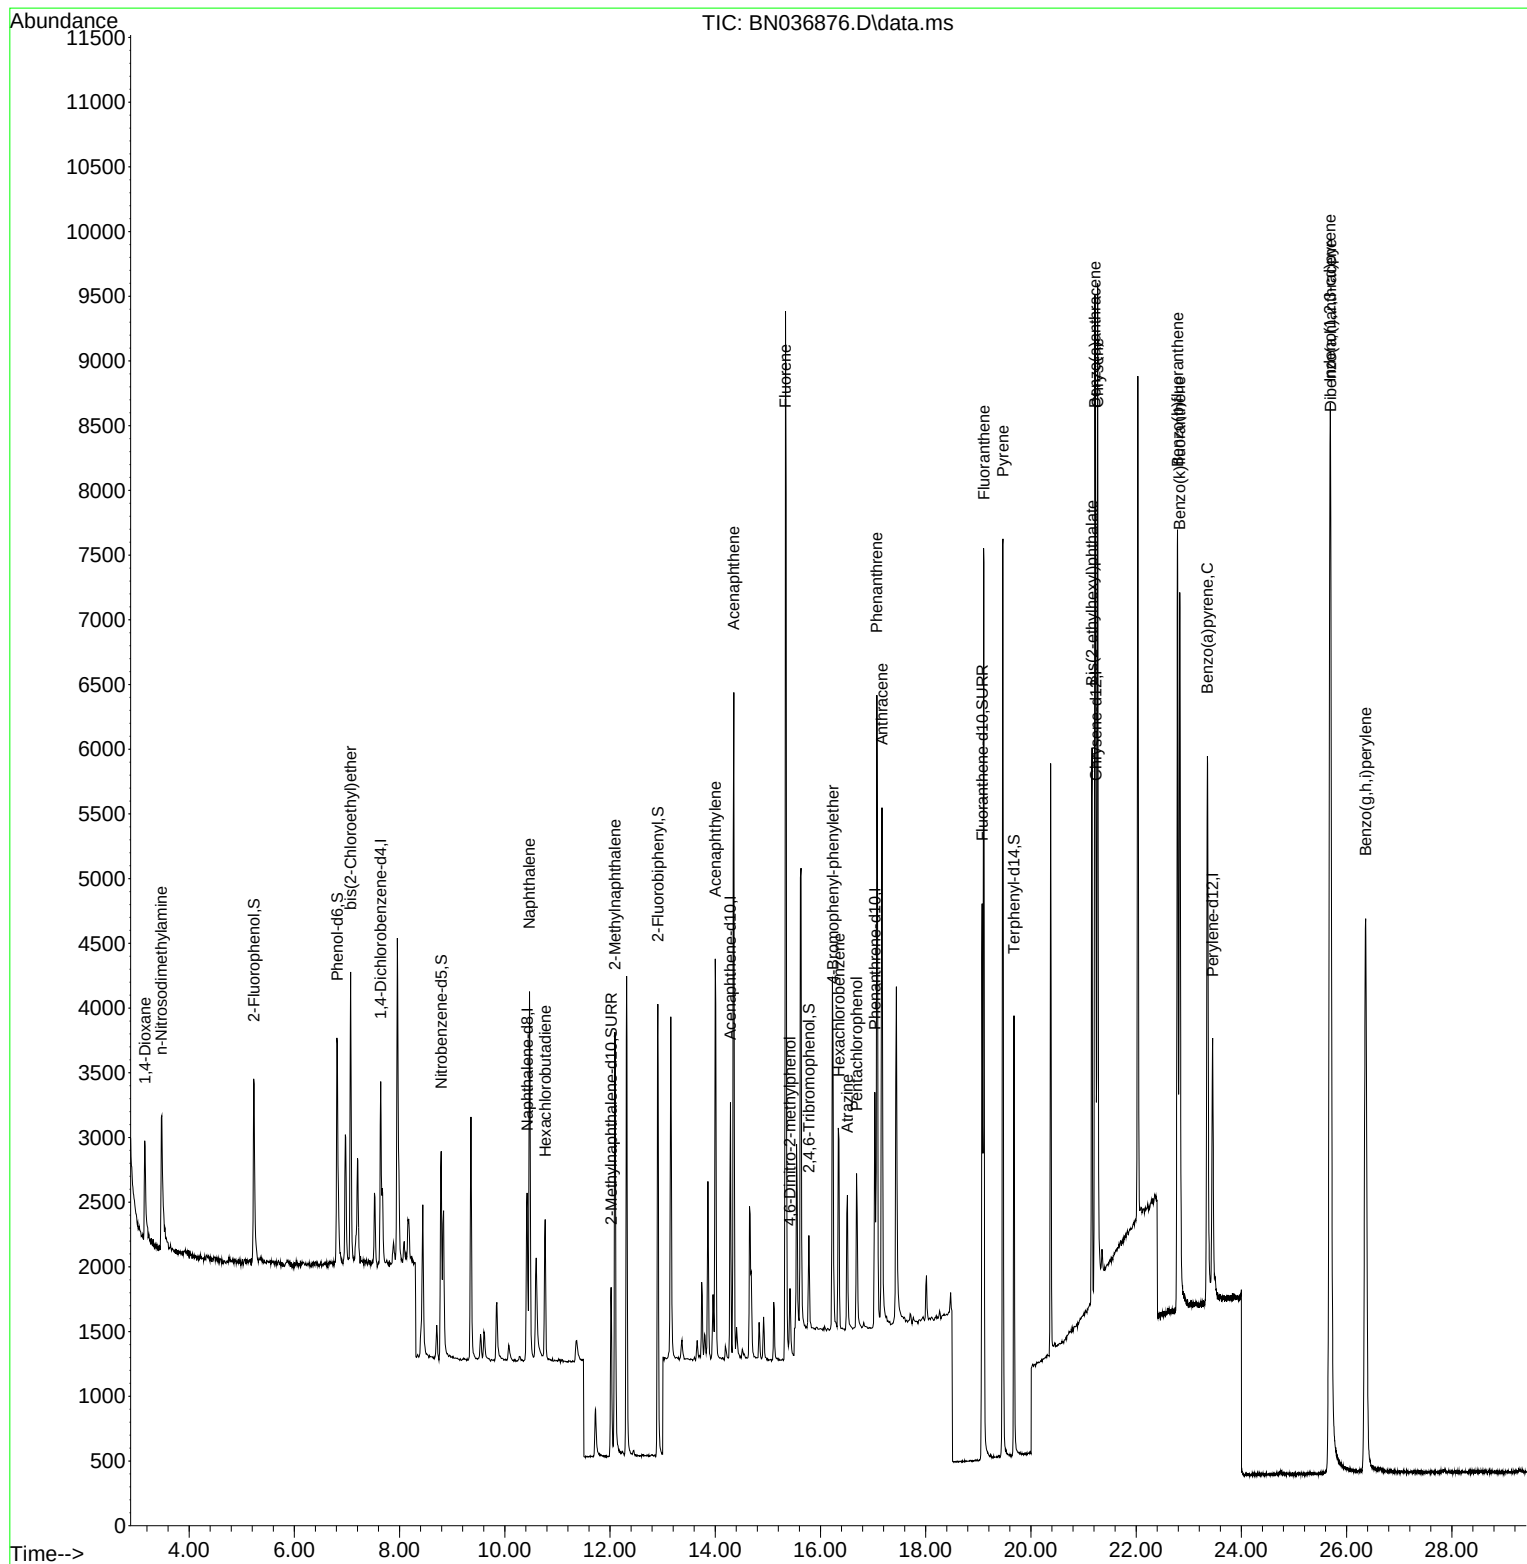




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 666
Ion Ratio Lower Upper
152 100
150 150.0 123.0 184.6
115 69.7 60.1 90.1



#2
1,4-Dioxane
Concen: 0.696 ng
RT: 3.162 min Scan# 39
Delta R.T. 0.007 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion: 88 Resp: 548
Ion Ratio Lower Upper
88 100
43 50.4 39.2 58.8
58 94.0 63.5 95.3









#3
n-Nitrosodimethylamine
Concen: 0.746 ng
RT: 3.473 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 42 Resp: 1294
Ion Ratio Lower Upper
42 100
74 69.9 54.6 81.8
44 9.9 0.0 0.0#



#4
2-Fluorophenol
Concen: 0.775 ng
RT: 5.235 min Scan# 326
Delta R.T. 0.007 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion: 112 Resp: 1226
Ion Ratio Lower Upper
112 100
64 67.9 54.0 81.0
63 42.8 35.1 52.7

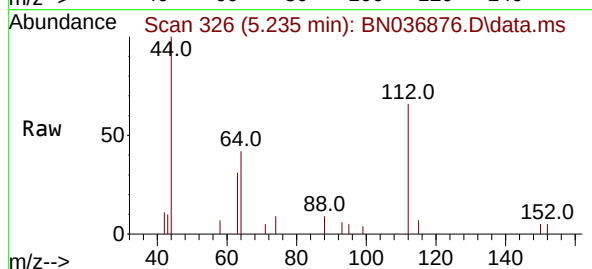



#5

Phenol-d6

Concen: 0.750 ng

RT: 6.817 min Scan# 545

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion: 99 Resp: 1511

Ion Ratio Lower Upper

99 100

42 37.9 30.9 46.3

71 45.6 38.6 58.0



#6

bis(2-Chloroethyl)ether

Concen: 0.778 ng

RT: 7.069 min Scan# 580

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion: 93 Resp: 1549


Ion Ratio Lower Upper

93 100

63 86.2 76.4 114.6

95 32.4 26.1 39.1




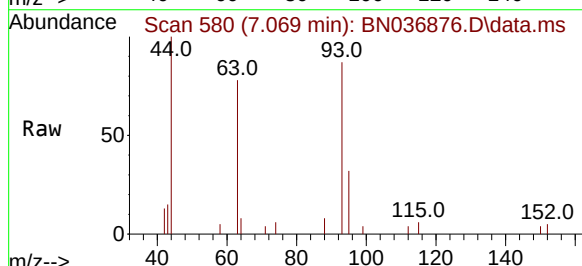




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	136	Resp:	1743
Ion	Ratio	Lower	Upper
136	100		
137	14.9	13.5	20.3
54	13.8	12.8	19.2
68	9.9	10.1	15.1



#8
Nitrobenzene-d5
Concen: 0.711 ng
RT: 8.792 min Scan# 797
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion:	82	Resp:	1392
Ion	Ratio	Lower	Upper
82	100		
128	41.7	35.5	53.3
54	65.5	56.2	84.4









#9
Naphthalene
Concen: 0.743 ng
RT: 10.468 min Scan# 954
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:128 Resp: 3762
Ion Ratio Lower Upper
128 100
129 12.4 12.9 19.3#
127 14.8 15.0 22.6#



#10
Hexachlorobutadiene
Concen: 0.744 ng
RT: 10.767 min Scan# 982
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion:225 Resp: 860
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 50.5 75.7









#11
2-Methylnaphthalene-d10
Concen: 0.760 ng
RT: 12.021 min Scan# 1153
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 1932
Ion Ratio Lower Upper
152 100
151 22.0 17.8 26.8



#12
2-Methylnaphthalene
Concen: 0.757 ng
RT: 12.092 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion:142 Resp: 2453
Ion Ratio Lower Upper
142 100
141 90.6 73.8 110.8
115 50.9 43.3 64.9




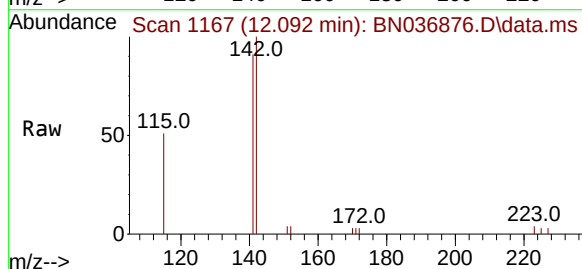




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.6	85.7	128.5
160	55.9	46.9	70.3



#14
2,4,6-Tribromophenol
Concen: 0.774 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion	Ratio	Lower	Upper
330	100		
332	93.0	87.0	130.6
141	52.6	45.3	67.9





#15

2-Fluorobiphenyl

Concen: 0.701 ng

RT: 12.909 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:172 Resp: 3506

Ion Ratio Lower Upper

172 100

171 37.4 32.7 49.1

170 24.9 23.3 34.9



#16

Acenaphthylene

Concen: 0.751 ng

RT: 13.999 min Scan# 1440

Delta R.T. -0.011 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:152 Resp: 3604


Ion Ratio Lower Upper

152 100

151 19.6 16.4 24.6

153 12.6 10.3 15.5





#17

Acenaphthene

Concen: 0.768 ng

RT: 14.352 min Scan# 1473

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.8





Tgt Ion:154 Resp: 2400

Ion Ratio Lower Upper

154 100

153 116.8 97.8 146.6

152 62.1 52.7 79.1



#18

Fluorene

Concen: 0.750 ng

RT: 15.336 min Scan# 1565

Delta R.T. -0.011 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:166 Resp: 3235


Ion Ratio Lower Upper

166 100

165 101.9 83.2 124.8

167 13.5 11.1 16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:188 Resp: 2266

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 13.7 13.9 20.9#



#20

4,6-Dinitro-2-methylphenol

Concen: 0.789 ng

RT: 15.421 min Scan# 1573

Delta R.T. -0.011 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:198 Resp: 418


Ion Ratio Lower Upper

198 100

51 114.3 107.6 161.4

105 60.1 55.2 82.8




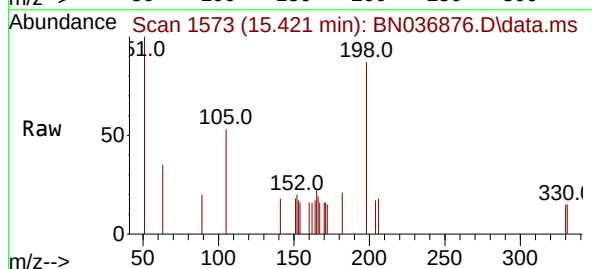




#21
4-Bromophenyl-phenylether
Concen: 0.759 ng
RT: 16.239 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion	Ratio	Lower	Upper
248	100		
250	101.3	83.5	125.3
141	51.7	55.3	82.9



#22
Hexachlorobenzene
Concen: 0.730 ng
RT: 16.351 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion	Ratio	Lower	Upper
284	100		
142	50.4	37.7	56.5
249	37.2	29.0	43.6









#23
Atrazine
Concen: 0.746 ng
RT: 16.512 min Scan# 1662
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:200 Resp: 1001
Ion Ratio Lower Upper
200 100
173 27.1 28.6 43.0#
215 50.2 40.5 60.7



#24
Pentachlorophenol
Concen: 0.699 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.012 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion:266 Resp: 588
Ion Ratio Lower Upper
266 100
264 64.8 44.6 66.8
268 65.6 51.8 77.6









#25
Phenanthrene
Concen: 0.758 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.012 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:178 Resp: 5162
Ion Ratio Lower Upper
178 100
176 20.0 16.6 25.0
179 15.2 12.8 19.2



#26
Anthracene
Concen: 0.744 ng
RT: 17.170 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion:178 Resp: 4492
Ion Ratio Lower Upper
178 100
176 19.4 15.8 23.6
179 15.0 12.6 18.8





#27

Fluoranthene-d10

Concen: 0.743 ng

RT: 19.073 min Scan# 1944

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:212 Resp: 4730

Ion Ratio Lower Upper

212 100

106 13.6 11.2 16.8

104 8.6 7.5 11.3



#28

Fluoranthene

Concen: 0.745 ng

RT: 19.105 min Scan# 1951

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:202 Resp: 6324


Ion Ratio Lower Upper

202 100

101 10.9 8.5 12.7

203 17.0 13.8 20.6





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.233 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:240 Resp: 2195

Ion Ratio Lower Upper

240 100

120 14.5 15.8 23.6#

236 29.7 25.8 38.8



#30

Pyrene

Concen: 0.776 ng

RT: 19.468 min Scan# 2029

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:202 Resp: 6482


Ion Ratio Lower Upper

202 100

200 21.5 17.1 25.7

203 17.7 14.5 21.7









#31
Terphenyl-d14
Concen: 0.774 ng
RT: 19.677 min Scan# 2074
Delta R.T. -0.005 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion	Ratio	Lower	Upper
244	100		
212	12.6	11.6	17.4
122	17.9	14.9	22.3



#32
Benzo(a)anthracene
Concen: 0.769 ng
RT: 21.215 min Scan# 2280
Delta R.T. 0.000 min
Lab File: BN036876.D
Acq: 11 Apr 2025 13:53

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.5	24.5	36.7
229	19.9	17.7	26.5





#33

Chrysene

Concen: 0.777 ng

RT: 21.269 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.8





Tgt Ion:228 Resp: 6669

Ion Ratio Lower Upper

228 100

226 31.1 26.1 39.1

229 20.5 17.0 25.4



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.718 ng

RT: 21.162 min Scan# 2274

Delta R.T. 0.000 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:149 Resp: 4201


Ion Ratio Lower Upper

149 100

167 25.9 21.0 31.4

279 3.0 3.6 5.4#





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.450 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.8





Tgt Ion:264 Resp: 2663

Ion Ratio Lower Upper

264 100

260 27.4 22.9 34.3

265 86.5 88.6 132.8#

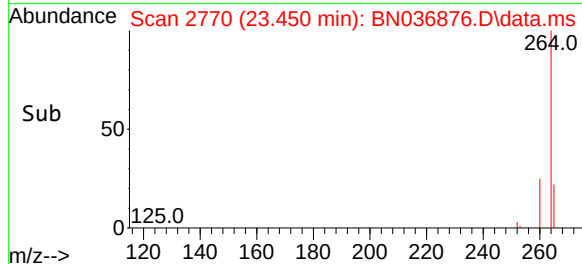

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.762 ng

RT: 25.684 min Scan# 3534

Delta R.T. -0.003 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:276 Resp: 9671


Ion Ratio Lower Upper

276 100

138 27.6 21.0 31.6

277 25.2 19.3 28.9

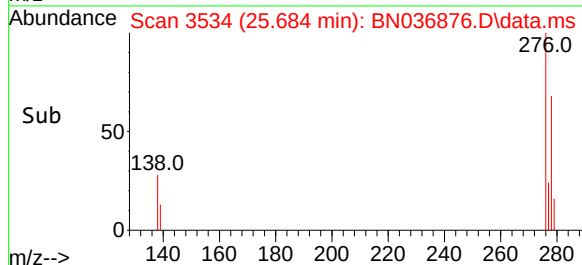



#37

Benzo(b)fluoranthene

Concen: 0.767 ng

RT: 22.787 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:252 Resp: 7215

Ion Ratio Lower Upper

252 100

253 25.4 27.0 40.6#

125 15.3 17.7 26.5#



#38

Benzo(k)fluoranthene

Concen: 0.771 ng

RT: 22.828 min Scan# 2557

Delta R.T. -0.006 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:252 Resp: 7294


Ion Ratio Lower Upper

252 100

253 26.2 26.7 40.1#

125 15.1 16.9 25.3#





#39

Benzo(a)pyrene

Concen: 0.778 ng

RT: 23.354 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.8





Tgt Ion:252 Resp: 6413

Ion Ratio Lower Upper

252 100

253 28.5 31.5 47.3#

125 17.5 22.6 34.0#



#40

Dibenzo(a,h)anthracene

Concen: 0.788 ng

RT: 25.696 min Scan# 3538

Delta R.T. -0.006 min

Lab File: BN036876.D

Acq: 11 Apr 2025 13:53




Tgt Ion:278 Resp: 7922


Ion Ratio Lower Upper

278 100

139 20.6 17.6 26.4

279 27.7 26.7 40.1





#41

Benzo(g,h,i)perylene

Concen: 0.760 ng

RT: 26.362 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN036876.D


Acq: 11 Apr 2025 13:53

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:276 Resp: 8703

Ion Ratio Lower Upper

276 100

277 25.5 21.8 32.8

138 25.9 21.6 32.4



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036877.D
 Acq On : 11 Apr 2025 14:30
 Operator : RC/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Apr 11 15:36:28 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 15:32:59 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	450	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	1197	0.400	ng	0.00
13) Acenaphthene-d10	14.288	164	725	0.400	ng	0.00
19) Phenanthrene-d10	17.034	188	1602	0.400	ng	0.00
29) Chrysene-d12	21.233	240	1632	0.400	ng	0.00
35) Perylene-d12	23.453	264	2020	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	1605	1.502	ng	0.00
5) Phenol-d6	6.817	99	2065	1.518	ng	0.00
8) Nitrobenzene-d5	8.792	82	1892	1.407	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	2739	1.569	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	536	1.531	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	5500	1.568	ng	0.00
27) Fluoranthene-d10	19.073	212	6992	1.554	ng	0.00
31) Terphenyl-d14	19.677	244	4823	1.545	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	819	1.539	ng	91
3) n-Nitrosodimethylamine	3.466	42	1839	1.569	ng	# 99
6) bis(2-Chloroethyl)ether	7.069	93	2024	1.505	ng	93
9) Naphthalene	10.468	128	5133	1.476	ng	# 91
10) Hexachlorobutadiene	10.767	225	1147	1.444	ng	# 100
12) 2-Methylnaphthalene	12.092	142	3403	1.529	ng	97
16) Acenaphthylene	13.999	152	5075	1.507	ng	100
17) Acenaphthene	14.352	154	3340	1.522	ng	96
18) Fluorene	15.336	166	4621	1.526	ng	97
20) 4,6-Dinitro-2-methylph...	15.421	198	589	1.573	ng	# 68
21) 4-Bromophenyl-phenylether	16.239	248	1476	1.529	ng	# 90
22) Hexachlorobenzene	16.351	284	1673	1.456	ng	97
23) Atrazine	16.512	200	1431	1.508	ng	# 92
24) Pentachlorophenol	16.686	266	857	1.440	ng	95
25) Phenanthrene	17.071	178	7364	1.530	ng	97
26) Anthracene	17.170	178	6636	1.555	ng	98
28) Fluoranthene	19.105	202	9374	1.562	ng	99
30) Pyrene	19.468	202	9592	1.545	ng	99
32) Benzo(a)anthracene	21.216	228	9153	1.593	ng	95
33) Chrysene	21.269	228	10135	1.588	ng	97
34) Bis(2-ethylhexyl)phtha...	21.162	149	6463	1.486	ng	# 99
36) Indeno(1,2,3-cd)pyrene	25.681	276	15556	1.615	ng	97
37) Benzo(b)fluoranthene	22.787	252	11121	1.559	ng	# 83
38) Benzo(k)fluoranthene	22.831	252	11185	1.558	ng	# 85
39) Benzo(a)pyrene	23.357	252	9906	1.585	ng	# 78
40) Dibenzo(a,h)anthracene	25.693	278	12606	1.653	ng	# 89
41) Benzo(g,h,i)perylene	26.362	276	13927	1.604	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036877.D
Acq On : 11 Apr 2025 14:30
Operator : RC/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Apr 11 15:36:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 15:32:59 2025
Response via : Initial Calibration




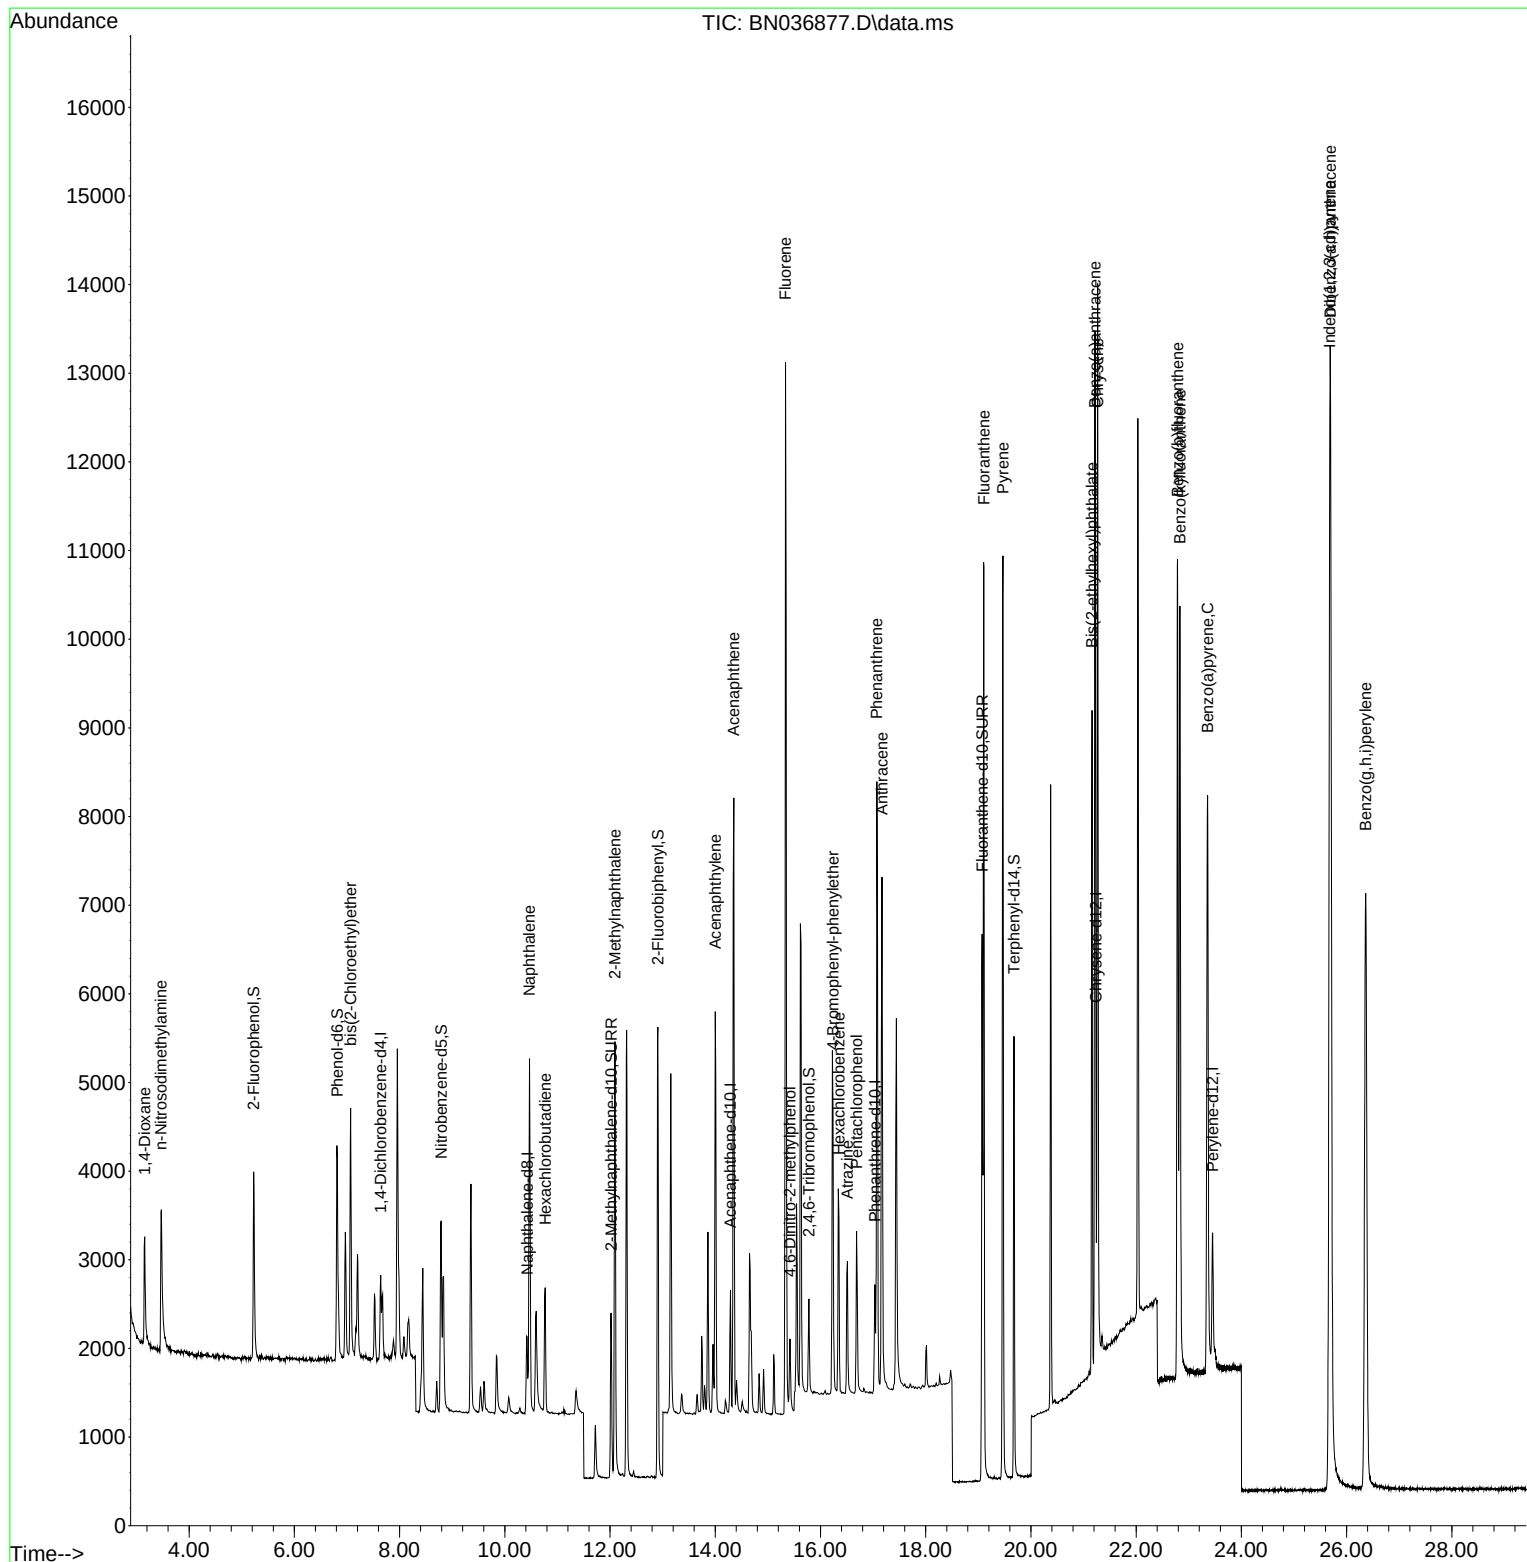




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 450
Ion Ratio Lower Upper
152 100
150 139.4 123.0 184.6
115 71.9 60.1 90.1



#2
1,4-Dioxane
Concen: 1.539 ng
RT: 3.155 min Scan# 38
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion: 88 Resp: 819
Ion Ratio Lower Upper
88 100
43 53.6 39.2 58.8
58 89.0 63.5 95.3









#3
n-Nitrosodimethylamine
Concen: 1.569 ng
RT: 3.466 min Scan# 81
Delta R.T. -0.007 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 1839
Ion Ratio Lower Upper
42 100
74 68.7 54.6 81.8
44 6.9 0.0 0.0#



#4
2-Fluorophenol
Concen: 1.502 ng
RT: 5.228 min Scan# 325
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion: 112 Resp: 1605
Ion Ratio Lower Upper
112 100
64 69.7 54.0 81.0
63 45.9 35.1 52.7









#5
Phenol-d6
Concen: 1.518 ng
RT: 6.817 min Scan# 54
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 2065
Ion Ratio Lower Upper
99 100
42 35.9 30.9 46.3
71 45.1 38.6 58.0



#6
bis(2-Chloroethyl)ether
Concen: 1.505 ng
RT: 7.069 min Scan# 580
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion: 93 Resp: 2024
Ion Ratio Lower Upper
93 100
63 86.2 76.4 114.6
95 31.9 26.1 39.1









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	1197
Ion	Ratio	Lower	Upper
136	100		
137	17.4	13.5	20.3
54	15.3	12.8	19.2
68	11.2	10.1	15.1



#8
Nitrobenzene-d5
Concen: 1.407 ng
RT: 8.792 min Scan# 797
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion:	82	Resp:	1892
Ion	Ratio	Lower	Upper
82	100		
128	41.5	35.5	53.3
54	66.9	56.2	84.4









#9
Naphthalene
Concen: 1.476 ng
RT: 10.468 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:128 Resp: 5133
Ion Ratio Lower Upper
128 100
129 12.3 12.9 19.3#
127 15.0 15.0 22.6#



#10
Hexachlorobutadiene
Concen: 1.444 ng
RT: 10.767 min Scan# 982
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion:225 Resp: 1147
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.4 50.5 75.7









#11
2-Methylnaphthalene-d10
Concen: 1.569 ng
RT: 12.021 min Scan# 1153
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 2739
Ion Ratio Lower Upper
152 100
151 21.0 17.8 26.8



#12
2-Methylnaphthalene
Concen: 1.529 ng
RT: 12.092 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion:142 Resp: 3403
Ion Ratio Lower Upper
142 100
141 92.0 73.8 110.8
115 48.9 43.3 64.9




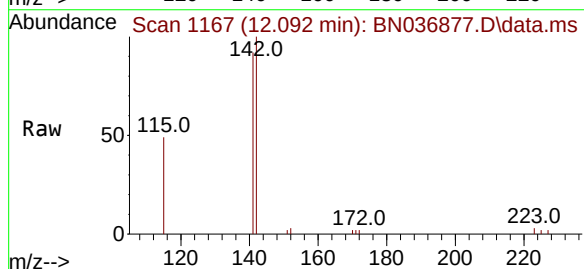




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 725
Ion Ratio Lower Upper
164 100
162 107.1 85.7 128.5
160 58.3 46.9 70.3



#14
2,4,6-Tribromophenol
Concen: 1.531 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion:330 Resp: 536
Ion Ratio Lower Upper
330 100
332 96.6 87.0 130.6
141 54.3 45.3 67.9

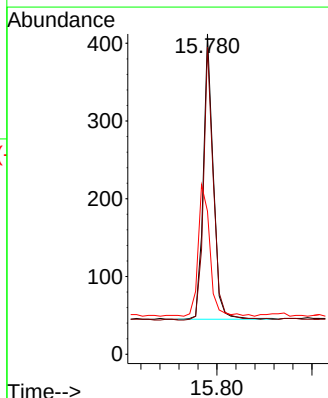



#15

2-Fluorobiphenyl

Concen: 1.568 ng

RT: 12.909 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:172 Resp: 5500

Ion Ratio Lower Upper

172 100

171 35.3 32.7 49.1

170 24.0 23.3 34.9



#16

Acenaphthylene

Concen: 1.507 ng

RT: 13.999 min Scan# 1440

Delta R.T. -0.011 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30




Tgt Ion:152 Resp: 5075


Ion Ratio Lower Upper

152 100

151 20.2 16.4 24.6

153 13.0 10.3 15.5









#17
Acenaphthene
Concen: 1.522 ng
RT: 14.352 min Scan# 1473
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 3340
Ion Ratio Lower Upper
154 100
153 117.6 97.8 146.6
152 63.2 52.7 79.1



#18
Fluorene
Concen: 1.526 ng
RT: 15.336 min Scan# 1565
Delta R.T. -0.011 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion:166 Resp: 4621
Ion Ratio Lower Upper
166 100
165 100.3 83.2 124.8
167 13.5 11.1 16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.034 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:188 Resp: 1602

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 15.4 13.9 20.9



#20

4,6-Dinitro-2-methylphenol

Concen: 1.573 ng

RT: 15.421 min Scan# 1573

Delta R.T. -0.011 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30




Tgt Ion:198 Resp: 589


Ion Ratio Lower Upper

198 100

51 88.3 107.6 161.4#

105 53.1 55.2 82.8#









#21
4-Bromophenyl-phenylether
Concen: 1.529 ng
RT: 16.239 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion	Ratio	Lower	Upper
248	100		
250	103.4	83.5	125.3
141	50.5	55.3	82.9



#22
Hexachlorobenzene
Concen: 1.456 ng
RT: 16.351 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion	Ratio	Lower	Upper
284	100		
142	50.1	37.7	56.5
249	36.3	29.0	43.6









#23
Atrazine
Concen: 1.508 ng
RT: 16.512 min Scan# 1662
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 1431
Ion Ratio Lower Upper
200 100
173 26.0 28.6 43.0#
215 49.3 40.5 60.7



#24
Pentachlorophenol
Concen: 1.440 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.012 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion:266 Resp: 857
Ion Ratio Lower Upper
266 100
264 63.9 44.6 66.8
268 64.8 51.8 77.6









#25
Phenanthrene
Concen: 1.530 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.012 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 7364
Ion Ratio Lower Upper
178 100
176 19.1 16.6 25.0
179 15.1 12.8 19.2



#26
Anthracene
Concen: 1.555 ng
RT: 17.170 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion:178 Resp: 6636
Ion Ratio Lower Upper
178 100
176 18.9 15.8 23.6
179 15.1 12.6 18.8





#27

Fluoranthene-d10

Concen: 1.554 ng

RT: 19.073 min Scan# 1944

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:212 Resp: 6992

Ion Ratio Lower Upper

212 100

106 13.5 11.2 16.8

104 8.6 7.5 11.3



#28

Fluoranthene

Concen: 1.562 ng

RT: 19.105 min Scan# 1951

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30




Tgt Ion:202 Resp: 9374


Ion Ratio Lower Upper

202 100

101 10.5 8.5 12.7

203 16.7 13.8 20.6





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.233 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:240 Resp: 1632

Ion Ratio Lower Upper

240 100

120 18.1 15.8 23.6

236 31.7 25.8 38.8



#30

Pyrene

Concen: 1.545 ng

RT: 19.468 min Scan# 2029

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30




Tgt Ion:202 Resp: 9592


Ion Ratio Lower Upper

202 100

200 21.2 17.1 25.7

203 17.6 14.5 21.7









#31
Terphenyl-d14
Concen: 1.545 ng
RT: 19.677 min Scan# 2074
Delta R.T. -0.005 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion	Ratio	Lower	Upper
244	100		
212	11.8	11.6	17.4
122	16.9	14.9	22.3



#32
Benzo(a)anthracene
Concen: 1.593 ng
RT: 21.216 min Scan# 2280
Delta R.T. 0.000 min
Lab File: BN036877.D
Acq: 11 Apr 2025 14:30

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.4	24.5	36.7
229	19.6	17.7	26.5





#33

Chrysene

Concen: 1.588 ng

RT: 21.269 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:228 Resp: 10135

Ion Ratio Lower Upper

228 100

226 30.6 26.1 39.1

229 19.9 17.0 25.4



#34

Bis(2-ethylhexyl)phthalate

Concen: 1.486 ng

RT: 21.162 min Scan# 2274

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30




Tgt Ion:149 Resp: 6463


Ion Ratio Lower Upper

149 100

167 26.0 21.0 31.4

279 3.3 3.6 5.4#





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.453 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:264 Resp: 2020

Ion Ratio Lower Upper

264 100

260 28.7 22.9 34.3

265 111.0 88.6 132.8



#36

Indeno(1,2,3-cd)pyrene

Concen: 1.615 ng

RT: 25.681 min Scan# 3533

Delta R.T. -0.006 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30




Tgt Ion:276 Resp: 15556


Ion Ratio Lower Upper

276 100

138 28.1 21.0 31.6

277 25.0 19.3 28.9





#37

Benzo(b)fluoranthene

Concen: 1.559 ng

RT: 22.787 min Scan# 2543

Delta R.T. -0.003 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:252 Resp: 11121

Ion Ratio Lower Upper

252 100

253 24.1 27.0 40.6#

125 13.8 17.7 26.5#



#38

Benzo(k)fluoranthene

Concen: 1.558 ng

RT: 22.831 min Scan# 2558

Delta R.T. -0.003 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30




Tgt Ion:252 Resp: 11185


Ion Ratio Lower Upper

252 100

253 25.0 26.7 40.1#

125 14.2 16.9 25.3#





#39

Benzo(a)pyrene

Concen: 1.585 ng

RT: 23.357 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:252 Resp: 9906

Ion Ratio Lower Upper

252 100

253 26.7 31.5 47.3#

125 16.0 22.6 34.0#



#40

Dibenzo(a,h)anthracene

Concen: 1.653 ng

RT: 25.693 min Scan# 3537

Delta R.T. -0.009 min

Lab File: BN036877.D

Acq: 11 Apr 2025 14:30




Tgt Ion:278 Resp: 12606


Ion Ratio Lower Upper

278 100

139 19.3 17.6 26.4

279 25.5 26.7 40.1#





#41

Benzo(g,h,i)perylene

Concen: 1.604 ng

RT: 26.362 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN036877.D


Acq: 11 Apr 2025 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:276 Resp: 13927

Ion Ratio Lower Upper

276 100

277 25.1 21.8 32.8

138 25.7 21.6 32.4



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036878.D
 Acq On : 11 Apr 2025 15:06
 Operator : RC/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Apr 11 15:36:59 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 15:32:59 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	606	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	1555	0.400	ng	0.00
13) Acenaphthene-d10	14.288	164	909	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	1989	0.400	ng	# 0.00
29) Chrysene-d12	21.233	240	2148	0.400	ng	# 0.00
35) Perylene-d12	23.450	264	2540	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	4754	3.304	ng	0.00
5) Phenol-d6	6.809	99	6125	3.343	ng	0.00
8) Nitrobenzene-d5	8.781	82	5458	3.123	ng	-0.01
11) 2-Methylnaphthalene-d10	12.016	152	7659	3.377	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	1472	3.352	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	15146	3.443	ng	0.00
27) Fluoranthene-d10	19.073	212	19501	3.491	ng	0.00
31) Terphenyl-d14	19.676	244	13773	3.353	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	2284	3.186	ng	Qvalue 94
3) n-Nitrosodimethylamine	3.465	42	5130	3.250	ng	# 97
6) bis(2-Chloroethyl)ether	7.069	93	5771	3.187	ng	93
9) Naphthalene	10.468	128	14629	3.237	ng	# 89
10) Hexachlorobutadiene	10.767	225	3248	3.148	ng	# 100
12) 2-Methylnaphthalene	12.092	142	9748	3.372	ng	96
16) Acenaphthylene	13.999	152	14508	3.436	ng	99
17) Acenaphthene	14.352	154	9568	3.477	ng	94
18) Fluorene	15.336	166	12941	3.408	ng	96
20) 4,6-Dinitro-2-methylph...	15.421	198	1852	3.983	ng	# 44
21) 4-Bromophenyl-phenylether	16.239	248	4104	3.424	ng	# 86
22) Hexachlorobenzene	16.351	284	4579	3.209	ng	96
23) Atrazine	16.512	200	3900	3.310	ng	# 86
24) Pentachlorophenol	16.686	266	2539	3.437	ng	95
25) Phenanthrene	17.071	178	20685	3.461	ng	98
26) Anthracene	17.170	178	18814	3.552	ng	98
28) Fluoranthene	19.100	202	26690	3.581	ng	100
30) Pyrene	19.463	202	27182	3.326	ng	99
32) Benzo(a)anthracene	21.215	228	26678	3.527	ng	95
33) Chrysene	21.269	228	28202	3.357	ng	96
34) Bis(2-ethylhexyl)phtha...	21.162	149	17563	3.069	ng	# 99
36) Indeno(1,2,3-cd)pyrene	25.678	276	42649	3.521	ng	96
37) Benzo(b)fluoranthene	22.784	252	31952	3.561	ng	# 80
38) Benzo(k)fluoranthene	22.828	252	31392	3.477	ng	# 81
39) Benzo(a)pyrene	23.354	252	28001	3.562	ng	# 73
40) Dibenzo(a,h)anthracene	25.693	278	34145	3.561	ng	# 89
41) Benzo(g,h,i)perylene	26.359	276	37283	3.415	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036878.D
Acq On : 11 Apr 2025 15:06
Operator : RC/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Apr 11 15:36:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 15:32:59 2025
Response via : Initial Calibration




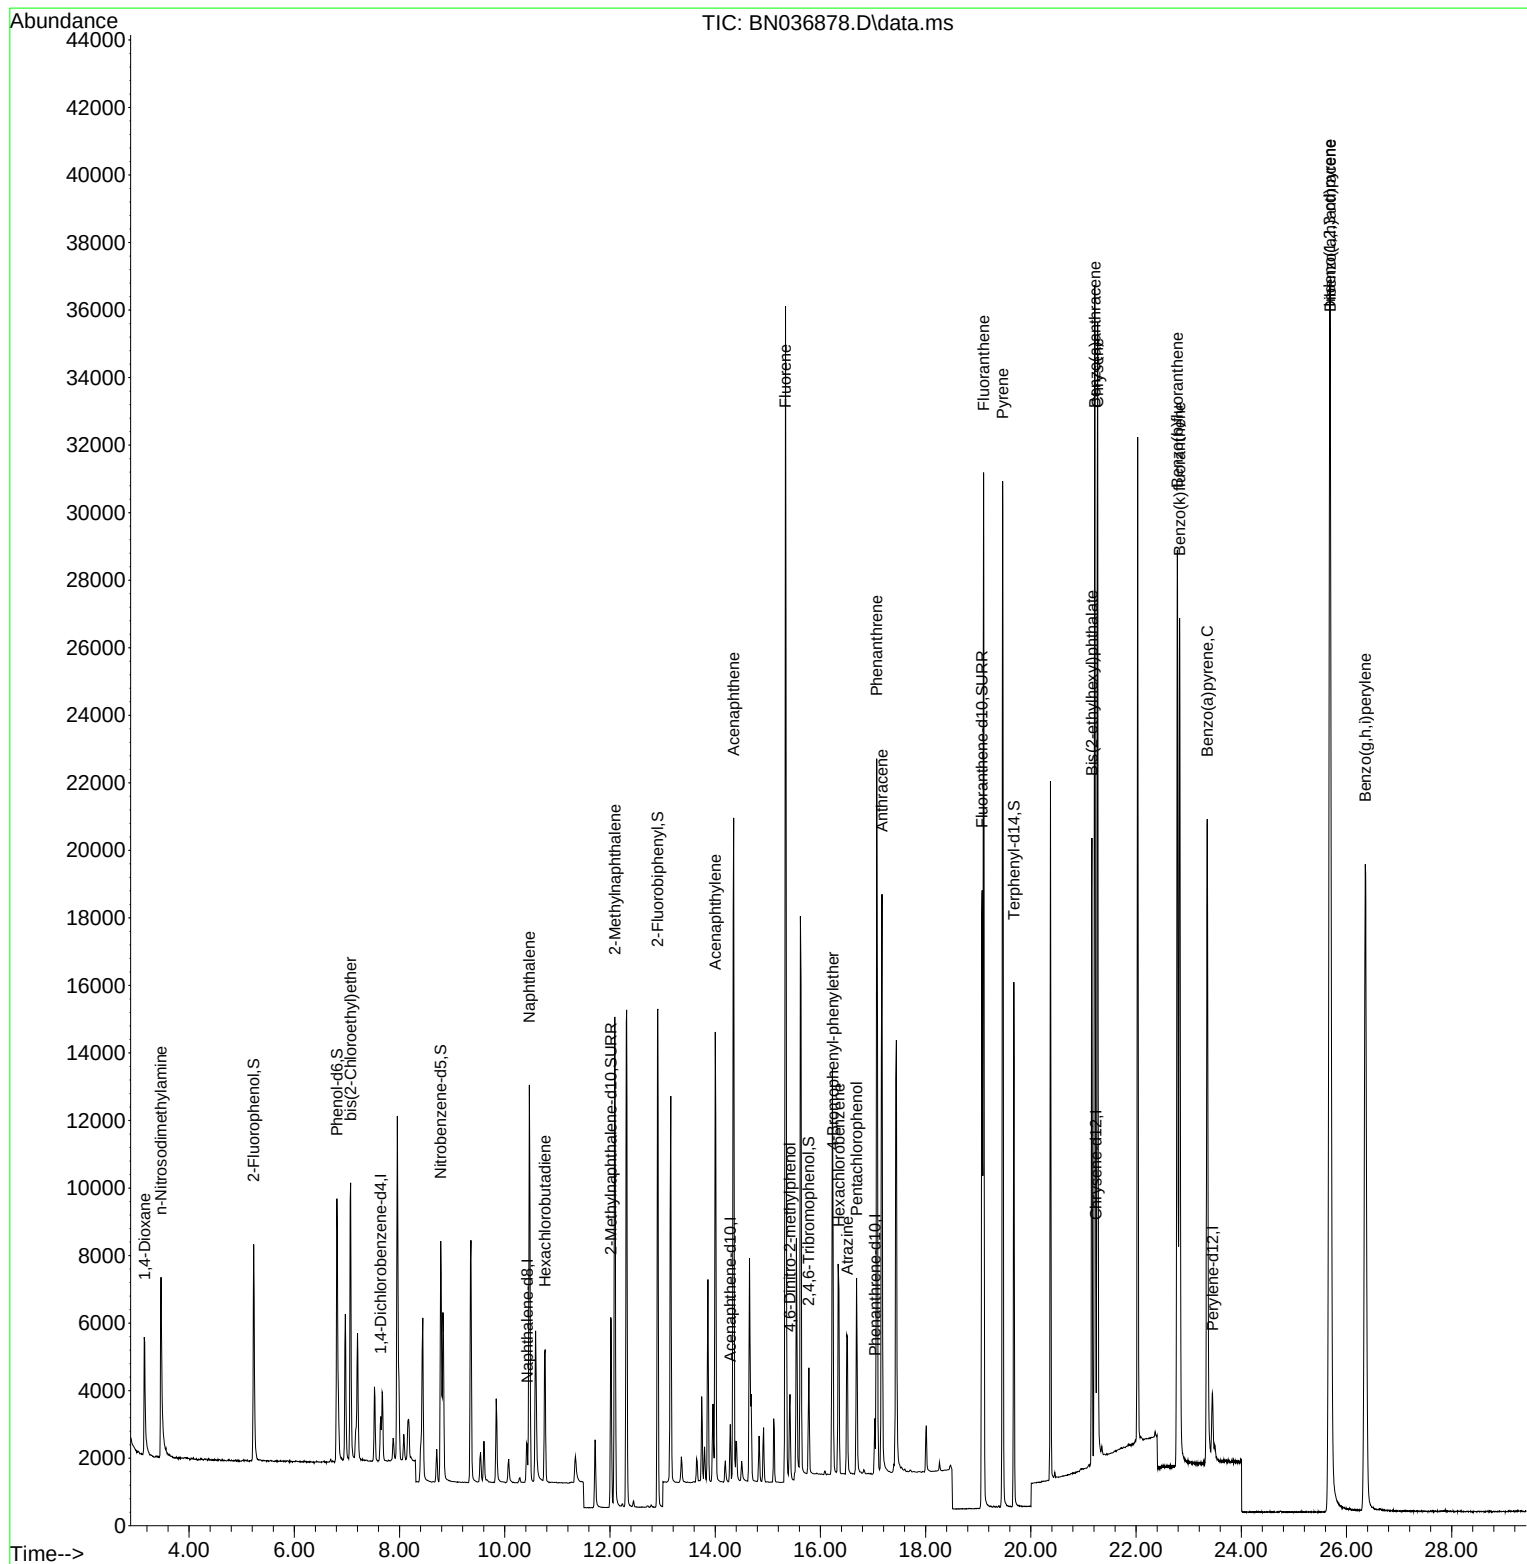




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 606
Ion Ratio Lower Upper
152 100
150 145.0 123.0 184.6
115 76.8 60.1 90.1



#2
1,4-Dioxane
Concen: 3.186 ng
RT: 3.155 min Scan# 38
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion: 88 Resp: 2284
Ion Ratio Lower Upper
88 100
43 49.3 39.2 58.8
58 88.2 63.5 95.3









#3
n-Nitrosodimethylamine
Concen: 3.250 ng
RT: 3.465 min Scan# 81
Delta R.T. -0.007 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 42 Resp: 5130
Ion Ratio Lower Upper
42 100
74 70.5 54.6 81.8
44 6.6 0.0 0.0#



#4
2-Fluorophenol
Concen: 3.304 ng
RT: 5.228 min Scan# 325
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion: 112 Resp: 4754
Ion Ratio Lower Upper
112 100
64 68.6 54.0 81.0
63 42.9 35.1 52.7









#5
Phenol-d6
Concen: 3.343 ng
RT: 6.809 min Scan# 54
Delta R.T. -0.007 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 6125
Ion Ratio Lower Upper
99 100
42 37.2 30.9 46.3
71 46.0 38.6 58.0



#6
bis(2-Chloroethyl)ether
Concen: 3.187 ng
RT: 7.069 min Scan# 580
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion: 93 Resp: 5771
Ion Ratio Lower Upper
93 100
63 86.6 76.4 114.6
95 31.4 26.1 39.1









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	1555
Ion	Ratio	Lower	Upper
136	100		
137	15.5	13.5	20.3
54	14.3	12.8	19.2
68	10.3	10.1	15.1



#8
Nitrobenzene-d5
Concen: 3.123 ng
RT: 8.781 min Scan# 796
Delta R.T. -0.011 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion:	82	Resp:	5458
Ion	Ratio	Lower	Upper
82	100		
128	31.5	35.5	53.3#
54	76.1	56.2	84.4





#9

Naphthalene

Concen: 3.237 ng

RT: 10.468 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:128 Resp: 14629

Ion Ratio Lower Upper

128 100

129 11.1 12.9 19.3#

127 14.1 15.0 22.6#



#10

Hexachlorobutadiene

Concen: 3.148 ng

RT: 10.767 min Scan# 982

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:225 Resp: 3248


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.4 50.5 75.7









#11
2-Methylnaphthalene-d10
Concen: 3.377 ng
RT: 12.016 min Scan# 1152
Delta R.T. -0.005 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 7659
Ion Ratio Lower Upper
152 100
151 21.5 17.8 26.8



#12
2-Methylnaphthalene
Concen: 3.372 ng
RT: 12.092 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion:142 Resp: 9748
Ion Ratio Lower Upper
142 100
141 91.1 73.8 110.8
115 48.4 43.3 64.9




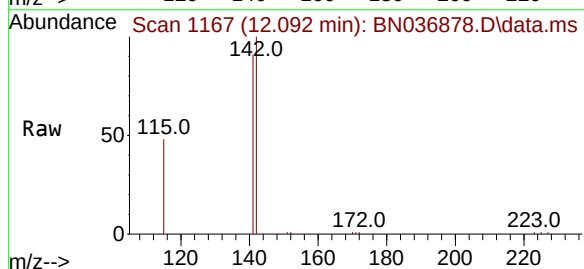




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 909
Ion Ratio Lower Upper
164 100
162 103.8 85.7 128.5
160 53.8 46.9 70.3



#14
2,4,6-Tribromophenol
Concen: 3.352 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion:330 Resp: 1472
Ion Ratio Lower Upper
330 100
332 95.8 87.0 130.6
141 58.0 45.3 67.9





#15

2-Fluorobiphenyl

Concen: 3.443 ng

RT: 12.909 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:172 Resp: 15146

Ion Ratio Lower Upper

172 100

171 35.8 32.7 49.1

170 23.6 23.3 34.9



#16

Acenaphthylene

Concen: 3.436 ng

RT: 13.999 min Scan# 1440

Delta R.T. -0.011 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:152 Resp: 14508


Ion Ratio Lower Upper

152 100

151 19.8 16.4 24.6

153 12.8 10.3 15.5





#17

Acenaphthene

Concen: 3.477 ng

RT: 14.352 min Scan# 1473

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:154 Resp: 9568

Ion Ratio Lower Upper

154 100

153 115.3 97.8 146.6

152 60.8 52.7 79.1



#18

Fluorene

Concen: 3.408 ng

RT: 15.336 min Scan# 1565

Delta R.T. -0.011 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:166 Resp: 12941


Ion Ratio Lower Upper

166 100

165 100.1 83.2 124.8

167 13.4 11.1 16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:188 Resp: 1989

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 12.9 13.9 20.9#



#20

4,6-Dinitro-2-methylphenol

Concen: 3.983 ng

RT: 15.421 min Scan# 1573

Delta R.T. -0.011 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:198 Resp: 1852


Ion Ratio Lower Upper

198 100

51 56.4 107.6 161.4#

105 39.0 55.2 82.8#









#21
4-Bromophenyl-phenylether
Concen: 3.424 ng
RT: 16.239 min Scan# 1640
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion	Ratio	Lower	Upper
248	100		
250	100.8	83.5	125.3
141	44.7	55.3	82.9



#22
Hexachlorobenzene
Concen: 3.209 ng
RT: 16.351 min Scan# 1649
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion	Ratio	Lower	Upper
284	100		
142	50.9	37.7	56.5
249	35.3	29.0	43.6









#23
Atrazine
Concen: 3.310 ng
RT: 16.512 min Scan# 1662
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:200 Resp: 3900
Ion Ratio Lower Upper
200 100
173 21.0 28.6 43.0#
215 45.9 40.5 60.7



#24
Pentachlorophenol
Concen: 3.437 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.012 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion:266 Resp: 2539
Ion Ratio Lower Upper
266 100
264 62.3 44.6 66.8
268 63.3 51.8 77.6









#25
Phenanthrene
Concen: 3.461 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.012 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion	178	176	179
Resp:	20685		
Ion Ratio	100	19.6	15.3
Lower		16.6	12.8
Upper		25.0	19.2



#26
Anthracene
Concen: 3.552 ng
RT: 17.170 min Scan# 1715
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion	178	176	179
Resp:	18814		
Ion Ratio	100	18.9	15.1
Lower		15.8	12.6
Upper		23.6	18.8





#27

Fluoranthene-d10

Concen: 3.491 ng

RT: 19.073 min Scan# 1944

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:212 Resp: 19501

Ion Ratio Lower Upper

212 100

106 13.6 11.2 16.8

104 8.4 7.5 11.3



#28

Fluoranthene

Concen: 3.581 ng

RT: 19.100 min Scan# 1950

Delta R.T. -0.005 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:202 Resp: 26690


Ion Ratio Lower Upper

202 100

101 10.7 8.5 12.7

203 17.0 13.8 20.6





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.233 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:240 Resp: 2148

Ion Ratio Lower Upper

240 100

120 14.5 15.8 23.6#

236 30.8 25.8 38.8



#30

Pyrene

Concen: 3.326 ng

RT: 19.463 min Scan# 2028

Delta R.T. -0.005 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:202 Resp: 27182


Ion Ratio Lower Upper

202 100

200 21.6 17.1 25.7


203 17.8 14.5 21.7








#31
Terphenyl-d14
Concen: 3.353 ng
RT: 19.676 min Scan# 2074
Delta R.T. -0.005 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2







Tgt Ion:244 Resp: 13773
Ion Ratio Lower Upper
244 100
212 11.1 11.6 17.4#
122 15.9 14.9 22.3

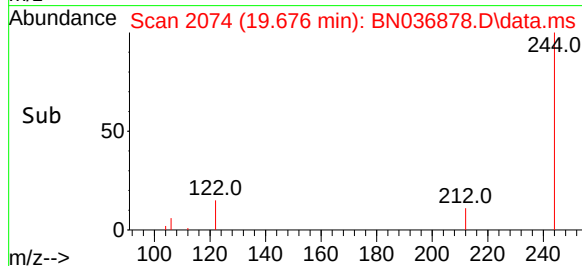

#32
Benzo(a)anthracene
Concen: 3.527 ng
RT: 21.215 min Scan# 2280
Delta R.T. -0.000 min
Lab File: BN036878.D
Acq: 11 Apr 2025 15:06

Tgt Ion:228 Resp: 26678
Ion Ratio Lower Upper
228 100
226 28.0 24.5 36.7
229 19.7 17.7 26.5

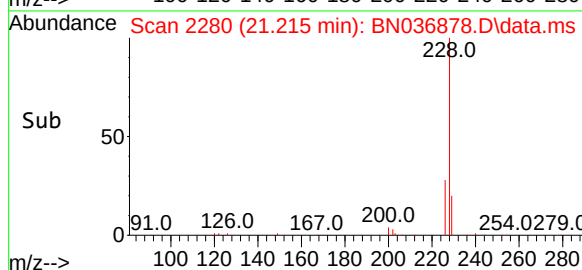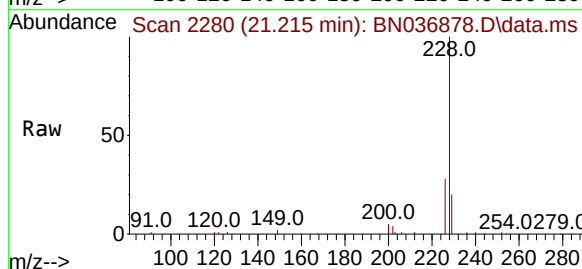



#33

Chrysene

Concen: 3.357 ng

RT: 21.269 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:228 Resp: 28202

Ion Ratio Lower Upper

228 100

226 30.3 26.1 39.1

229 19.5 17.0 25.4



#34

Bis(2-ethylhexyl)phthalate

Concen: 3.069 ng

RT: 21.162 min Scan# 2274

Delta R.T. -0.000 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:149 Resp: 17563


Ion Ratio Lower Upper

149 100

167 26.4 21.0 31.4

279 2.7 3.6 5.4#





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.450 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:264 Resp: 2540

Ion Ratio Lower Upper

264 100

260 28.1 22.9 34.3

265 95.9 88.6 132.8



#36

Indeno(1,2,3-cd)pyrene

Concen: 3.521 ng

RT: 25.678 min Scan# 3532

Delta R.T. -0.009 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:276 Resp: 42649


Ion Ratio Lower Upper

276 100

138 29.1 21.0 31.6

277 25.0 19.3 28.9





#37

Benzo(b)fluoranthene

Concen: 3.561 ng

RT: 22.784 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:252 Resp: 31952

Ion Ratio Lower Upper

252 100

253 22.5 27.0 40.6#

125 12.1 17.7 26.5#



#38

Benzo(k)fluoranthene

Concen: 3.477 ng

RT: 22.828 min Scan# 2557

Delta R.T. -0.006 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:252 Resp: 31392


Ion Ratio Lower Upper

252 100

253 22.5 26.7 40.1#

125 12.4 16.9 25.3#





#39

Benzo(a)pyrene

Concen: 3.562 ng

RT: 23.354 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN036878.D


Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:252 Resp: 28001

Ion Ratio Lower Upper

252 100

253 22.7 31.5 47.3#

125 13.8 22.6 34.0#



#40

Dibenzo(a,h)anthracene

Concen: 3.561 ng

RT: 25.693 min Scan# 3537

Delta R.T. -0.009 min

Lab File: BN036878.D

Acq: 11 Apr 2025 15:06




Tgt Ion:278 Resp: 34145


Ion Ratio Lower Upper

278 100

139 19.7 17.6 26.4

279 24.3 26.7 40.1#





#41

Benzo(g,h,i)perylene

Concen: 3.415 ng

RT: 26.359 min Scan# 31

Delta R.T. -0.003 min

Lab File: BN036878.D


Acq: 11 Apr 2025 15:06

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:276 Resp: 37283

Ion Ratio Lower Upper

276 100

277 24.0 21.8 32.8

138 25.4 21.6 32.4



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036879.D
 Acq On : 11 Apr 2025 15:42
 Operator : RC/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 11 16:10:04 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 15:54:19 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	567	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	1439	0.400	ng	0.00
13) Acenaphthene-d10	14.288	164	846	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	1883	0.400	ng	0.00
29) Chrysene-d12	21.233	240	2075	0.400	ng	# 0.00
35) Perylene-d12	23.450	264	2437	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	6296	4.676	ng	0.00
5) Phenol-d6	6.809	99	8262	4.820	ng	0.00
8) Nitrobenzene-d5	8.781	82	7400	4.576	ng	-0.01
11) 2-Methylnaphthalene-d10	12.016	152	10278	4.898	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	2017	4.936	ng	0.00
15) 2-Fluorobiphenyl	12.904	172	19383	4.735	ng	0.00
27) Fluoranthene-d10	19.073	212	27011	5.107	ng	0.00
31) Terphenyl-d14	19.677	244	18930	4.771	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.148	88	2954	4.405	ng	Qvalue 93
3) n-Nitrosodimethylamine	3.458	42	6680	4.523	ng	# 96
6) bis(2-Chloroethyl)ether	7.069	93	7731	4.563	ng	92
9) Naphthalene	10.468	128	19422	4.644	ng	# 89
10) Hexachlorobutadiene	10.767	225	4231	4.432	ng	# 100
12) 2-Methylnaphthalene	12.092	142	13024	4.868	ng	95
16) Acenaphthylene	13.999	152	19678	5.008	ng	99
17) Acenaphthene	14.352	154	12748	4.978	ng	94
18) Fluorene	15.336	166	17523	4.959	ng	96
20) 4,6-Dinitro-2-methylph...	15.421	198	2409	5.472	ng	# 42
21) 4-Bromophenyl-phenylether	16.239	248	5432	4.787	ng	# 86
22) Hexachlorobenzene	16.351	284	6185	4.578	ng	96
23) Atrazine	16.500	200	5134	4.603	ng	91
24) Pentachlorophenol	16.686	266	3504	5.010	ng	94
25) Phenanthrene	17.071	178	27851	4.922	ng	98
26) Anthracene	17.170	178	25741	5.133	ng	99
28) Fluoranthene	19.101	202	36952	5.237	ng	100
30) Pyrene	19.468	202	37628	4.766	ng	99
32) Benzo(a)anthracene	21.215	228	37427	5.123	ng	95
33) Chrysene	21.269	228	39358	4.850	ng	96
34) Bis(2-ethylhexyl)phtha...	21.162	149	24571	4.445	ng	# 99
36) Indeno(1,2,3-cd)pyrene	25.678	276	58462	5.031	ng	96
37) Benzo(b)fluoranthene	22.784	252	44349	5.152	ng	# 79
38) Benzo(k)fluoranthene	22.828	252	44237	5.084	ng	# 81
39) Benzo(a)pyrene	23.354	252	38961	5.166	ng	# 72
40) Dibenzo(a,h)anthracene	25.693	278	47274	5.138	ng	# 88
41) Benzo(g,h,i)perylene	26.362	276	51130	4.881	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036879.D
Acq On : 11 Apr 2025 15:42
Operator : RC/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 11 16:10:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 15:54:19 2025
Response via : Initial Calibration




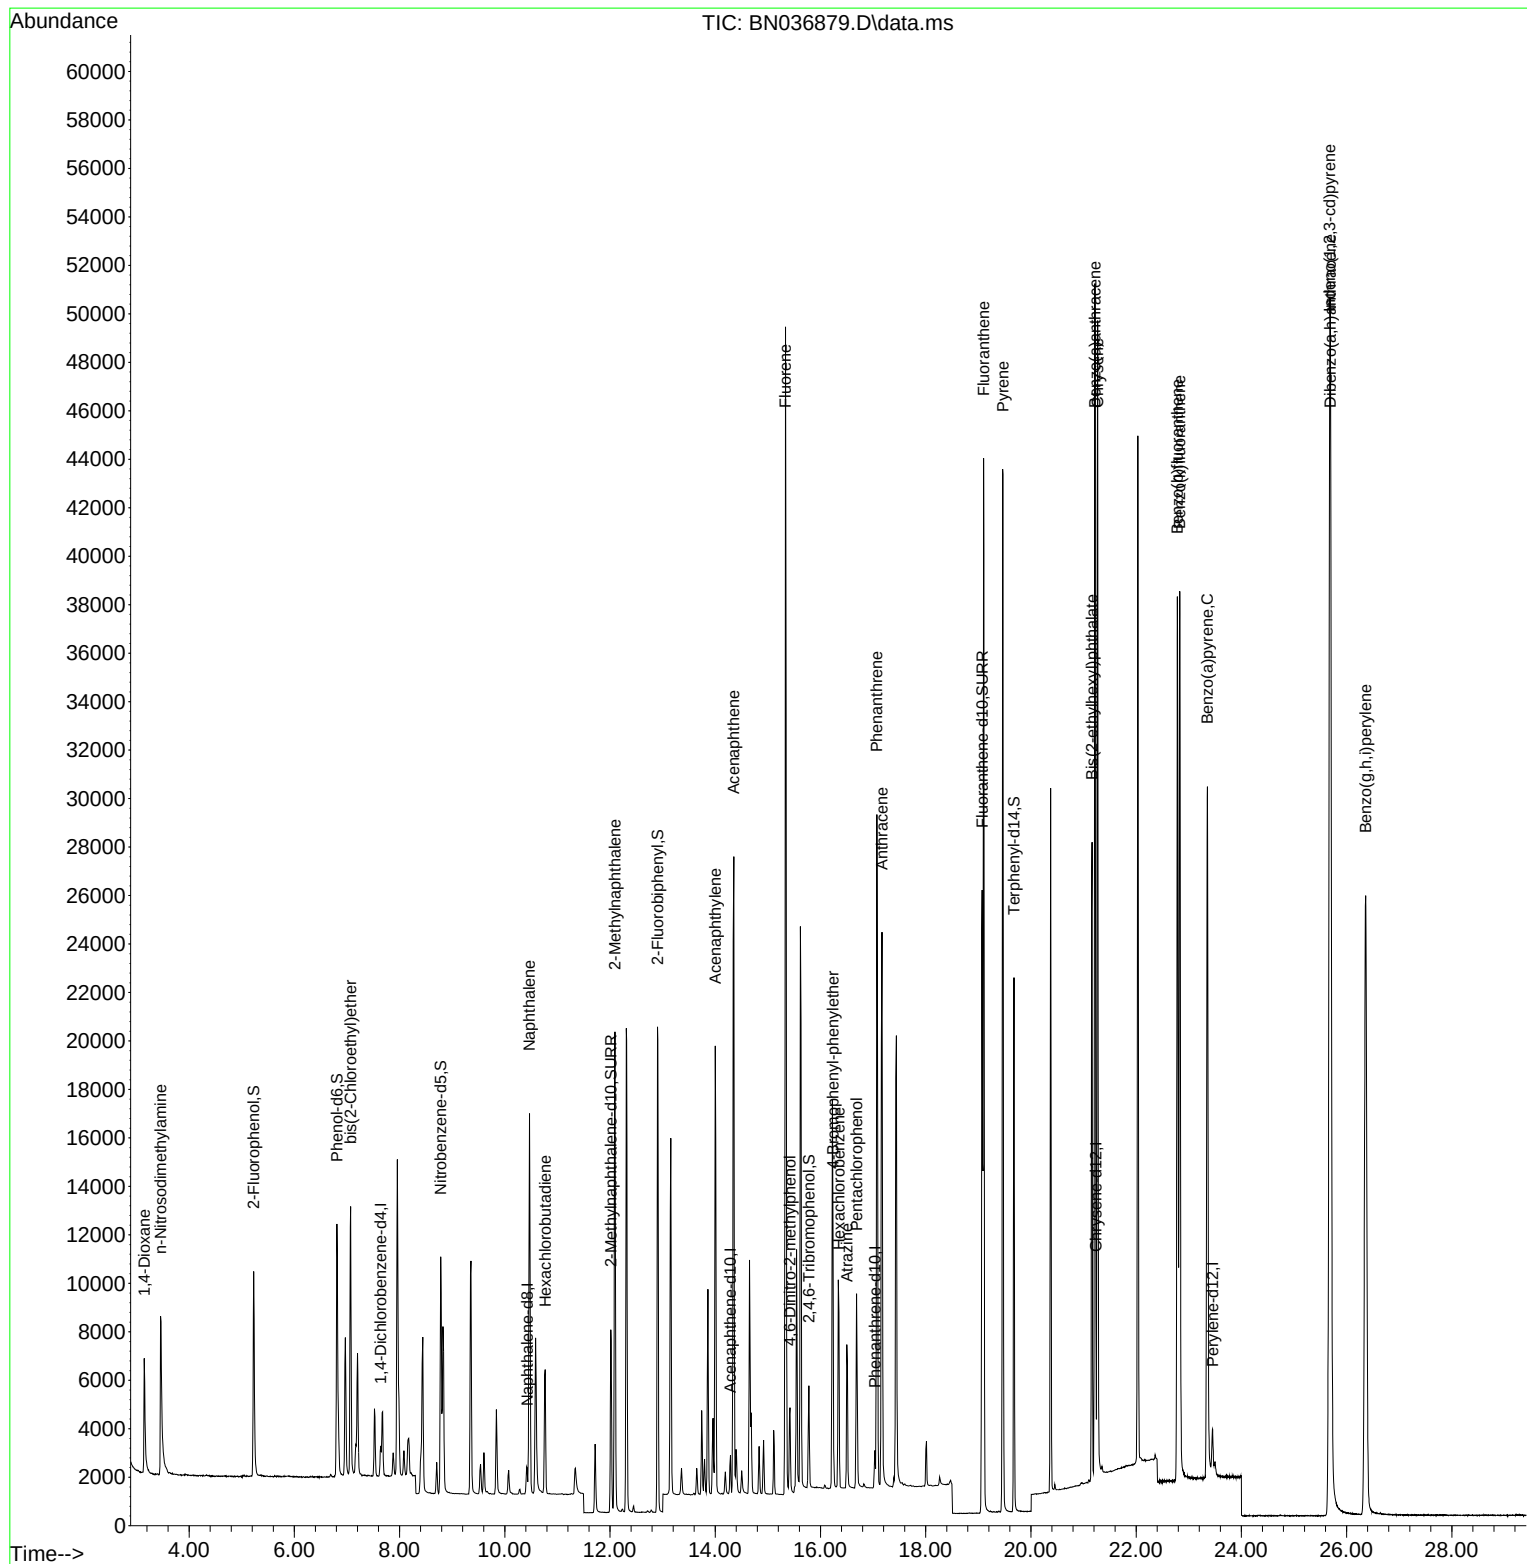




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 567
Ion Ratio Lower Upper
152 100
150 150.1 123.0 184.6
115 74.9 60.1 90.1



#2
1,4-Dioxane
Concen: 4.405 ng
RT: 3.148 min Scan# 37
Delta R.T. -0.007 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion: 88 Resp: 2954
Ion Ratio Lower Upper
88 100
43 49.9 39.2 58.8
58 88.5 63.5 95.3









#3
n-Nitrosodimethylamine
Concen: 4.523 ng
RT: 3.458 min Scan# 80
Delta R.T. -0.014 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 6680
Ion Ratio Lower Upper
42 100
74 71.6 54.6 81.8
44 4.9 0.0 0.0#



#4
2-Fluorophenol
Concen: 4.676 ng
RT: 5.228 min Scan# 325
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion: 112 Resp: 6296
Ion Ratio Lower Upper
112 100
64 68.8 54.0 81.0
63 43.1 35.1 52.7









#5
Phenol-d6
Concen: 4.820 ng
RT: 6.809 min Scan# 54
Delta R.T. -0.007 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 8262
Ion Ratio Lower Upper
99 100
42 36.5 30.9 46.3
71 45.2 38.6 58.0



#6
bis(2-Chloroethyl)ether
Concen: 4.563 ng
RT: 7.069 min Scan# 580
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion: 93 Resp: 7731
Ion Ratio Lower Upper
93 100
63 86.1 76.4 114.6
95 31.2 26.1 39.1









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	1439
Ion	Ratio	Lower	Upper
136	100		
137	15.5	13.5	20.3
54	14.1	12.8	19.2
68	10.3	10.1	15.1



#8
Nitrobenzene-d5
Concen: 4.576 ng
RT: 8.781 min Scan# 796
Delta R.T. -0.011 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion:	82	Resp:	7400
Ion	Ratio	Lower	Upper
82	100		
128	30.5	35.5	53.3#
54	74.3	56.2	84.4



#9
Naphthalene

Concen: 4.644 ng

RT: 10.468 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:128 Resp: 19422

Ion Ratio Lower Upper

128 100

129 11.0 12.9 19.3#

127 14.0 15.0 22.6#



#10

Hexachlorobutadiene

Concen: 4.432 ng

RT: 10.767 min Scan# 982

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42




Tgt Ion:225 Resp: 4231


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 62.8 50.5 75.7









#11
2-Methylnaphthalene-d10
Concen: 4.898 ng
RT: 12.016 min Scan# 1152
Delta R.T. -0.005 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 10278
Ion Ratio Lower Upper
152 100
151 21.4 17.8 26.8



#12
2-Methylnaphthalene
Concen: 4.868 ng
RT: 12.092 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion:142 Resp: 13024
Ion Ratio Lower Upper
142 100
141 90.3 73.8 110.8
115 46.7 43.3 64.9




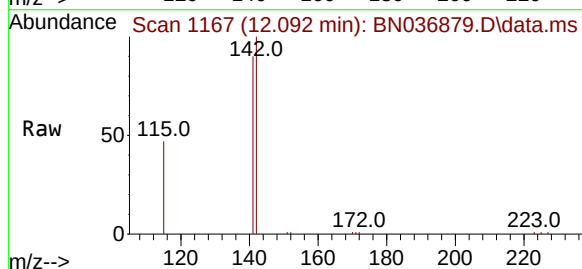




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	164	Resp:	846
Ion Ratio	Lower	Upper	
164	100		
162	107.8	85.7	128.5
160	55.9	46.9	70.3



#14
2,4,6-Tribromophenol
Concen: 4.936 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion	330	Resp:	2017
Ion Ratio	Lower	Upper	
330	100		
332	97.3	87.0	130.6
141	56.8	45.3	67.9









#15
2-Fluorobiphenyl
Concen: 4.735 ng
RT: 12.904 min Scan# 11
Delta R.T. -0.005 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172	Resp:	19383
Ion	Ratio	Lower Upper
172	100	
171	36.1	32.7 49.1
170	24.5	23.3 34.9



#16
Acenaphthylene
Concen: 5.008 ng
RT: 13.999 min Scan# 1440
Delta R.T. -0.011 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion:152	Resp:	19678
Ion	Ratio	Lower Upper
152	100	
151	19.9	16.4 24.6
153	12.9	10.3 15.5

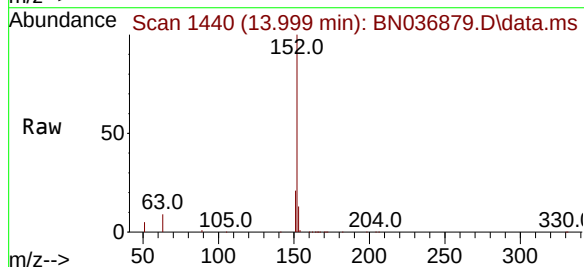



#17

Acenaphthene

Concen: 4.978 ng

RT: 14.352 min Scan# 1473

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:154 Resp: 12748

Ion Ratio Lower Upper

154 100

153 115.6 97.8 146.6

152 60.8 52.7 79.1



#18

Fluorene

Concen: 4.959 ng

RT: 15.336 min Scan# 1565

Delta R.T. -0.011 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42




Tgt Ion:166 Resp: 17523


Ion Ratio Lower Upper

166 100

165 99.7 83.2 124.8

167 13.3 11.1 16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:188 Resp: 1883

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 14.4 13.9 20.9



#20

4,6-Dinitro-2-methylphenol

Concen: 5.472 ng

RT: 15.421 min Scan# 1573

Delta R.T. -0.011 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42




Tgt Ion:198 Resp: 2409


Ion Ratio Lower Upper

198 100

51 53.3 107.6 161.4#

105 37.6 55.2 82.8#









#21
4-Bromophenyl-phenylether
Concen: 4.787 ng
RT: 16.239 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	Ratio	Lower	Upper
248	100		
250	103.2	83.5	125.3
141	42.0	55.3	82.9



#22
Hexachlorobenzene
Concen: 4.578 ng
RT: 16.351 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion	Ratio	Lower	Upper
284	100		
142	50.3	37.7	56.5
249	35.1	29.0	43.6









#23
Atrazine
Concen: 4.603 ng
RT: 16.500 min Scan# 1661
Delta R.T. -0.012 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	Ratio	Lower	Upper
200	100		
173	34.3	28.6	43.0
215	41.6	40.5	60.7



#24
Pentachlorophenol
Concen: 5.010 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.012 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion	Ratio	Lower	Upper
266	100		
264	63.1	44.6	66.8
268	63.3	51.8	77.6









#25
Phenanthrene
Concen: 4.922 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.012 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.7	16.6	25.0
179	15.2	12.8	19.2



#26
Anthracene
Concen: 5.133 ng
RT: 17.170 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.8	23.6
179	15.3	12.6	18.8





#27

Fluoranthene-d10

Concen: 5.107 ng

RT: 19.073 min Scan# 1944

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:212 Resp: 27011

Ion Ratio Lower Upper

212 100

106 14.1 11.2 16.8

104 8.5 7.5 11.3



#28

Fluoranthene

Concen: 5.237 ng

RT: 19.101 min Scan# 1950

Delta R.T. -0.005 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42




Tgt Ion:202 Resp: 36952


Ion Ratio Lower Upper

202 100

101 10.8 8.5 12.7

203 17.0 13.8 20.6





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.233 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:240 Resp: 2075

Ion Ratio Lower Upper

240 100

120 14.6 15.8 23.6#

236 31.3 25.8 38.8



#30

Pyrene

Concen: 4.766 ng

RT: 19.468 min Scan# 2029

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42




Tgt Ion:202 Resp: 37628


Ion Ratio Lower Upper

202 100

200 21.5 17.1 25.7

203 17.7 14.5 21.7









#31
Terphenyl-d14
Concen: 4.771 ng
RT: 19.677 min Scan# 2074
Delta R.T. -0.005 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	Ratio	Lower	Upper
244	100		
212	10.9	11.6	17.4#
122	16.2	14.9	22.3



#32
Benzo(a)anthracene
Concen: 5.123 ng
RT: 21.215 min Scan# 2280
Delta R.T. 0.000 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.0	24.5	36.7
229	19.6	17.7	26.5





#33

Chrysene

Concen: 4.850 ng

RT: 21.269 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 39358

Ion Ratio Lower Upper

228 100

226 30.6 26.1 39.1

229 19.3 17.0 25.4



#34

Bis(2-ethylhexyl)phthalate

Concen: 4.445 ng

RT: 21.162 min Scan# 2274

Delta R.T. 0.000 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42




Tgt Ion:149 Resp: 24571


Ion Ratio Lower Upper

149 100

167 26.0 21.0 31.4


279 2.7 3.6 5.4#








#35
Perylene-d12
Concen: 0.400 ng
RT: 23.450 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:264 Resp: 2437
Ion Ratio Lower Upper
264 100
260 29.1 22.9 34.3
265 104.2 88.6 132.8



#36
Indeno(1,2,3-cd)pyrene
Concen: 5.031 ng
RT: 25.678 min Scan# 3532
Delta R.T. -0.009 min
Lab File: BN036879.D
Acq: 11 Apr 2025 15:42

Tgt Ion:276 Resp: 58462
Ion Ratio Lower Upper
276 100
138 29.8 21.0 31.6
277 24.7 19.3 28.9





#37

Benzo(b)fluoranthene

Concen: 5.152 ng

RT: 22.784 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 44349

Ion Ratio Lower Upper

252 100

253 22.1 27.0 40.6#

125 11.9 17.7 26.5#



#38

Benzo(k)fluoranthene

Concen: 5.084 ng

RT: 22.828 min Scan# 2557

Delta R.T. -0.006 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42




Tgt Ion:252 Resp: 44237


Ion Ratio Lower Upper

252 100

253 22.5 26.7 40.1#

125 12.2 16.9 25.3#





#39

Benzo(a)pyrene

Concen: 5.166 ng

RT: 23.354 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN036879.D


Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 38961

Ion Ratio Lower Upper

252 100

253 22.6 31.5 47.3#

125 13.5 22.6 34.0#



#40

Dibenzo(a,h)anthracene

Concen: 5.138 ng

RT: 25.693 min Scan# 3537

Delta R.T. -0.009 min

Lab File: BN036879.D

Acq: 11 Apr 2025 15:42




Tgt Ion:278 Resp: 47274


Ion Ratio Lower Upper

278 100

139 19.9 17.6 26.4

279 23.7 26.7 40.1#





#41

Benzo(g,h,i)perylene

Concen: 4.881 ng

RT: 26.362 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN036879.D


Acq: 11 Apr 2025 15:42

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:276 Resp: 51130

Ion Ratio Lower Upper

276 100

277 23.7 21.8 32.8

138 25.8 21.6 32.4



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036880.D
 Acq On : 11 Apr 2025 16:18
 Operator : RC/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN041125

Quant Time: Apr 11 16:41:49 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 16:11:08 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	356	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	934	0.400	ng	0.00
13) Acenaphthene-d10	14.288	164	562	0.400	ng	0.00
19) Phenanthrene-d10	17.034	188	1227	0.400	ng	0.00
29) Chrysene-d12	21.233	240	1378	0.400	ng	0.00
35) Perylene-d12	23.450	264	1678	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	330	0.394	ng	0.00
5) Phenol-d6	6.817	99	364	0.340	ng	0.00
8) Nitrobenzene-d5	8.792	82	372	0.359	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	516	0.380	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	92	0.340	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	927	0.343	ng	0.00
27) Fluoranthene-d10	19.073	212	1345	0.389	ng	0.00
31) Terphenyl-d14	19.677	244	1023	0.391	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	176m	0.426	ng	
3) n-Nitrosodimethylamine	3.473	42	416	0.455	ng	# 100
6) bis(2-Chloroethyl)ether	7.070	93	423	0.403	ng	89
9) Naphthalene	10.468	128	1042	0.388	ng	95
10) Hexachlorobutadiene	10.767	225	245	0.402	ng	# 98
12) 2-Methylnaphthalene	12.092	142	620	0.358	ng	95
16) Acenaphthylene	14.010	152	1105	0.423	ng	98
17) Acenaphthene	14.352	154	664	0.391	ng	95
18) Fluorene	15.346	166	914	0.390	ng	96
20) 4,6-Dinitro-2-methylph...	15.432	198	95	0.327	ng	# 46
21) 4-Bromophenyl-phenylether	16.239	248	273	0.371	ng	98
22) Hexachlorobenzene	16.351	284	325	0.374	ng	92
23) Atrazine	16.512	200	322	0.448	ng	93
24) Pentachlorophenol	16.686	266	179	0.393	ng	93
25) Phenanthrene	17.071	178	1449	0.394	ng	100
26) Anthracene	17.170	178	1362	0.415	ng	97
28) Fluoranthene	19.101	202	1833	0.396	ng	99
30) Pyrene	19.468	202	1936	0.372	ng	98
32) Benzo(a)anthracene	21.216	228	1916	0.394	ng	99
33) Chrysene	21.269	228	2205	0.411	ng	99
34) Bis(2-ethylhexyl)phtha...	21.153	149	1487	0.412	ng	99
36) Indeno(1,2,3-cd)pyrene	25.675	276	3402	0.425	ng	98
37) Benzo(b)fluoranthene	22.787	252	2332	0.392	ng	96
38) Benzo(k)fluoranthene	22.828	252	2571	0.428	ng	96
39) Benzo(a)pyrene	23.354	252	2267	0.434	ng	96
40) Dibenzo(a,h)anthracene	25.699	278	2690	0.423	ng	96
41) Benzo(g,h,i)perylene	26.357	276	2966	0.413	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036880.D
Acq On : 11 Apr 2025 16:18
Operator : RC/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN041125

Quant Time: Apr 11 16:41:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration




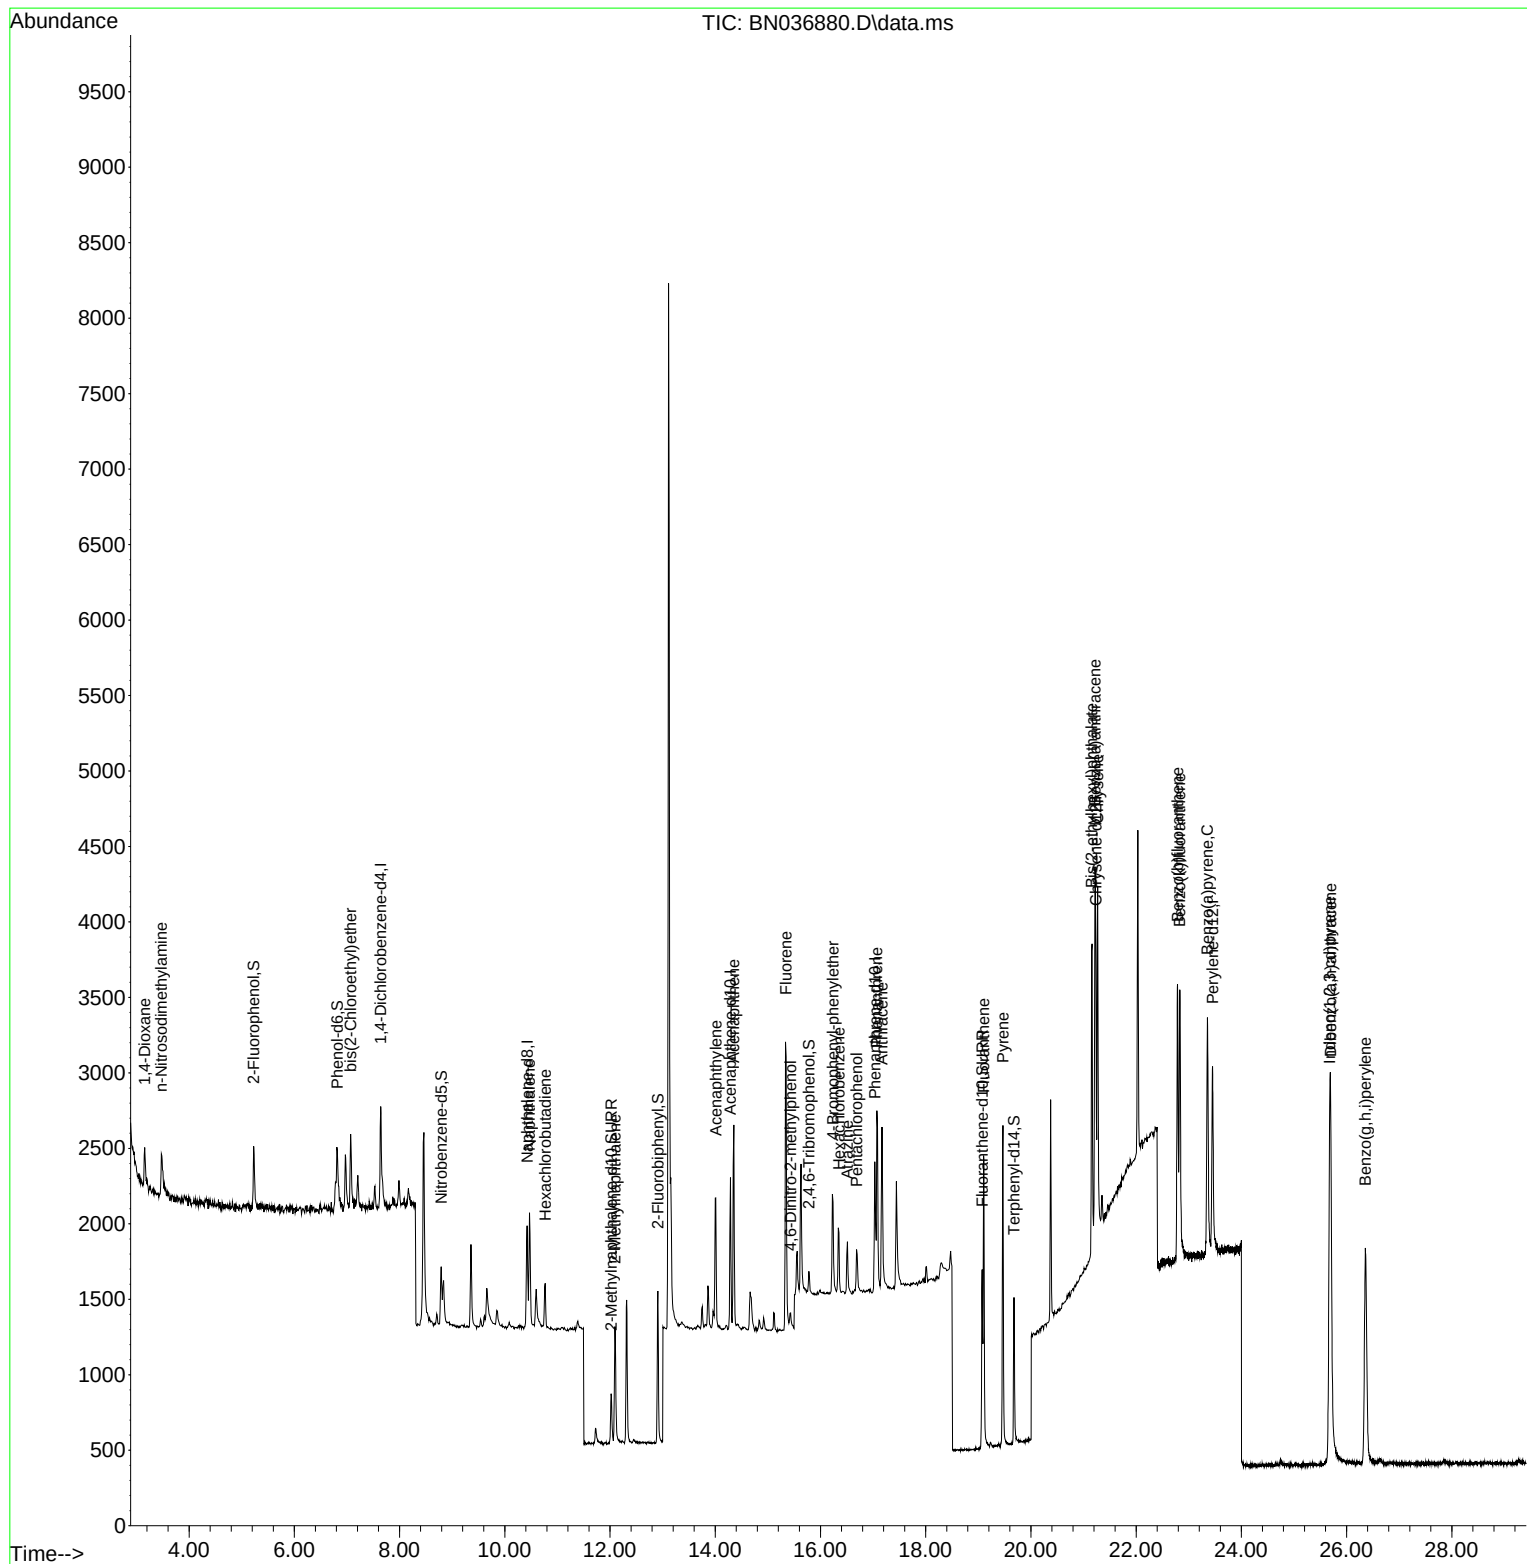




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion: 152 Resp: 356
Ion Ratio Lower Upper
152 100
150 144.0 123.0 184.6
115 79.6 60.1 90.1



#2
1,4-Dioxane
Concen: 0.426 ng m
RT: 3.155 min Scan# 38
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion: 88 Resp: 176
Ion Ratio Lower Upper
88 100
43 61.4 39.2 58.8#
58 96.6 63.5 95.3#









#3
n-Nitrosodimethylamine
Concen: 0.455 ng
RT: 3.473 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion: 42 Resp: 416
Ion Ratio Lower Upper
42 100
74 68.0 54.6 81.8
44 0.0 0.0 0.0



#4
2-Fluorophenol
Concen: 0.394 ng
RT: 5.228 min Scan# 325
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion: 112 Resp: 330
Ion Ratio Lower Upper
112 100
64 67.0 54.0 81.0
63 47.3 35.1 52.7









#5
Phenol-d6
Concen: 0.340 ng
RT: 6.817 min Scan# 545
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion: 99 Resp: 364
Ion Ratio Lower Upper
99 100
42 49.2 30.9 46.3#
71 49.2 38.6 58.0



#6
bis(2-Chloroethyl)ether
Concen: 0.403 ng
RT: 7.070 min Scan# 580
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion: 93 Resp: 423
Ion Ratio Lower Upper
93 100
63 83.9 76.4 114.6
95 28.4 26.1 39.1









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 950
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion:	136	Resp:	934
Ion	Ratio	Lower	Upper
136	100		
137	18.9	13.5	20.3
54	18.0	12.8	19.2
68	14.2	10.1	15.1



#8
Nitrobenzene-d5
Concen: 0.359 ng
RT: 8.792 min Scan# 797
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion:	82	Resp:	372
Ion	Ratio	Lower	Upper
82	100		
128	52.3	35.5	53.3
54	79.0	56.2	84.4









#9
Naphthalene
Concen: 0.388 ng
RT: 10.468 min Scan# 954
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion:	128	Resp:	1042
Ion	Ratio	Lower	Upper
128	100		
129	19.2	12.9	19.3
127	20.5	15.0	22.6



#10
Hexachlorobutadiene
Concen: 0.402 ng
RT: 10.767 min Scan# 982
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion:	225	Resp:	245
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	61.6	50.5	75.7









#11
2-Methylnaphthalene-d10
Concen: 0.380 ng
RT: 12.021 min Scan# 1153
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion:152 Resp: 516
Ion Ratio Lower Upper
152 100
151 22.1 17.8 26.8



#12
2-Methylnaphthalene
Concen: 0.358 ng
RT: 12.092 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion:142 Resp: 620
Ion Ratio Lower Upper
142 100
141 91.3 73.8 110.8
115 61.7 43.3 64.9









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.0	85.7	128.5
160	58.7	46.9	70.3



#14
2,4,6-Tribromophenol
Concen: 0.340 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion	Ratio	Lower	Upper
330	100		
332	100.0	87.0	130.6
141	57.6	45.3	67.9





#15

2-Fluorobiphenyl

Concen: 0.343 ng

RT: 12.909 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:172 Resp: 927

Ion Ratio Lower Upper

172 100

171 39.7 32.7 49.1

170 26.8 23.3 34.9



#16

Acenaphthylene

Concen: 0.423 ng

RT: 14.010 min Scan# 1441

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:152 Resp: 1105


Ion Ratio Lower Upper

152 100

151 19.2 16.4 24.6

153 12.7 10.3 15.5

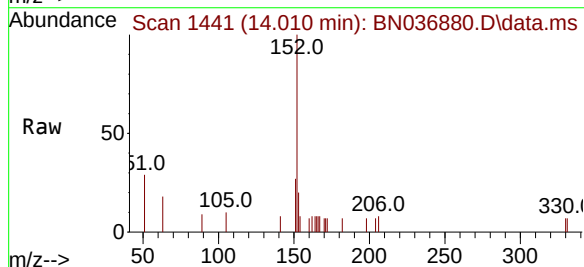



#17

Acenaphthene

Concen: 0.391 ng

RT: 14.352 min Scan# 1473

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:154 Resp: 664

Ion Ratio Lower Upper

154 100

153 117.0 97.8 146.6

152 61.6 52.7 79.1



#18

Fluorene

Concen: 0.390 ng

RT: 15.346 min Scan# 1566

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:166 Resp: 914


Ion Ratio Lower Upper

166 100

165 99.6 83.2 124.8

167 13.6 11.1 16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.034 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:188 Resp: 1227

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 18.2 13.9 20.9



#20

4,6-Dinitro-2-methylphenol

Concen: 0.327 ng

RT: 15.432 min Scan# 1574

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:198 Resp: 95


Ion Ratio Lower Upper

198 100

51 216.3 107.6 161.4#

105 89.5 55.2 82.8#









#21
4-Bromophenyl-phenylether
Concen: 0.371 ng
RT: 16.239 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion:	248	Resp:	273
Ion	Ratio	Lower	Upper
248	100		
250	100.5	83.5	125.3
141	68.9	55.3	82.9



#22
Hexachlorobenzene
Concen: 0.374 ng
RT: 16.351 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion:	284	Resp:	325
Ion	Ratio	Lower	Upper
284	100		
142	53.5	37.7	56.5
249	40.0	29.0	43.6









#23
Atrazine
Concen: 0.448 ng
RT: 16.512 min Scan# 1662
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion	Ratio	Lower	Upper
200	100		
173	39.8	28.6	43.0
215	55.0	40.5	60.7



#24
Pentachlorophenol
Concen: 0.393 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.012 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.0	44.6	66.8
268	68.7	51.8	77.6









#25
Phenanthrene
Concen: 0.394 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.012 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion:178 Resp: 1449
Ion Ratio Lower Upper
178 100
176 20.4 16.6 25.0
179 16.0 12.8 19.2



#26
Anthracene
Concen: 0.415 ng
RT: 17.170 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion:178 Resp: 1362
Ion Ratio Lower Upper
178 100
176 17.5 15.8 23.6
179 16.1 12.6 18.8





#27

Fluoranthene-d10

Concen: 0.389 ng

RT: 19.073 min Scan# 1944

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:212 Resp: 1345

Ion Ratio Lower Upper

212 100

106 13.3 11.2 16.8

104 9.3 7.5 11.3



#28

Fluoranthene

Concen: 0.396 ng

RT: 19.101 min Scan# 1950

Delta R.T. -0.005 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:202 Resp: 1833


Ion Ratio Lower Upper

202 100

101 10.7 8.5 12.7

203 17.6 13.8 20.6





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.233 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:240 Resp: 1378

Ion Ratio Lower Upper

240 100

120 20.2 15.8 23.6

236 33.9 25.8 38.8



#30

Pyrene

Concen: 0.372 ng

RT: 19.468 min Scan# 2029

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:202 Resp: 1936


Ion Ratio Lower Upper

202 100

200 22.2 17.1 25.7

203 17.4 14.5 21.7





#31

Terphenyl-d14

Concen: 0.391 ng

RT: 19.677 min Scan# 2075

Delta R.T. -0.005 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:244 Resp: 1023

Ion Ratio Lower Upper

244 100

212 16.3 11.6 17.4

122 21.1 14.9 22.3



#32

Benzo(a)anthracene

Concen: 0.394 ng

RT: 21.216 min Scan# 2280

Delta R.T. 0.000 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:228 Resp: 1916


Ion Ratio Lower Upper

228 100

226 30.5 24.5 36.7

229 21.5 17.7 26.5




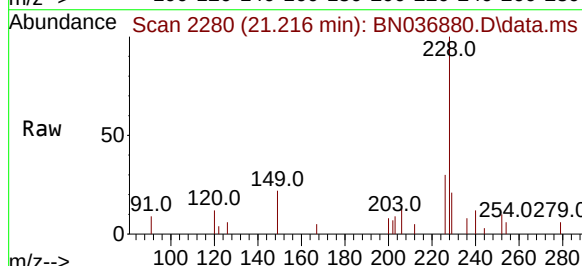




#33
Chrysene
Concen: 0.411 ng
RT: 21.269 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18




Instrument :
BNA_N
ClientSampleId :
ICVBN041125


Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.5	26.1	39.1
229	21.0	17.0	25.4



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.412 ng
RT: 21.153 min Scan# 2273
Delta R.T. -0.009 min
Lab File: BN036880.D
Acq: 11 Apr 2025 16:18

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.6	21.0	31.4
279	4.0	3.6	5.4





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.450 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:264 Resp: 1678

Ion Ratio Lower Upper

264 100

260 30.4 22.9 34.3

265 134.4 88.6 132.8#

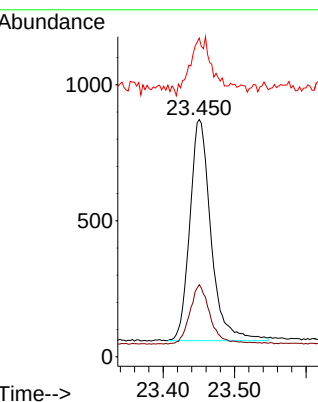

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.425 ng

RT: 25.675 min Scan# 3531

Delta R.T. -0.012 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:276 Resp: 3402


Ion Ratio Lower Upper

276 100

138 27.6 21.0 31.6

277 25.3 19.3 28.9





#37

Benzo(b)fluoranthene

Concen: 0.392 ng

RT: 22.787 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125




Tgt Ion:252 Resp: 2332

Ion Ratio Lower Upper

252 100

253 35.3 27.0 40.6

125 25.3 17.7 26.5



#38

Benzo(k)fluoranthene

Concen: 0.428 ng

RT: 22.828 min Scan# 2557

Delta R.T. -0.006 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:252 Resp: 2571


Ion Ratio Lower Upper

252 100

253 36.2 26.7 40.1

125 22.3 16.9 25.3





#39

Benzo(a)pyrene

Concen: 0.434 ng

RT: 23.354 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:252 Resp: 2267

Ion Ratio Lower Upper

252 100

253 39.9 31.5 47.3

125 32.4 22.6 34.0



#40

Dibenzo(a,h)anthracene

Concen: 0.423 ng

RT: 25.699 min Scan# 3539

Delta R.T. -0.003 min

Lab File: BN036880.D

Acq: 11 Apr 2025 16:18




Tgt Ion:278 Resp: 2690


Ion Ratio Lower Upper

278 100

139 22.8 17.6 26.4

279 36.4 26.7 40.1





#41

Benzo(g,h,i)perylene

Concen: 0.413 ng

RT: 26.357 min Scan# 31

Delta R.T. -0.006 min

Lab File: BN036880.D


Acq: 11 Apr 2025 16:18

Instrument :

BNA_N

ClientSampleId :

ICVBN041125





Tgt Ion:276 Resp: 2966

Ion Ratio Lower Upper

276 100

277 28.1 21.8 32.8

138 28.6 21.6 32.4



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036880.D
 Acq On : 11 Apr 2025 16:18
 Operator : RC/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN041125

Quant Time: Apr 11 16:41:49 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 16:11:08 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	73	0.00
2	1,4-Dioxane	0.464	0.494	-6.5	81	0.00
3	n-Nitrosodimethylamine	1.028	1.169	-13.7	78	0.00
4 S	2-Fluorophenol	0.941	0.927	1.5	70	0.00
5 S	Phenol-d6	1.203	1.022	15.0	62	0.00
6	bis(2-Chloroethyl)ether	1.180	1.188	-0.7	73	0.00
7 I	Naphthalene-d8	1.000	1.000	0.0	74	0.00
8 S	Nitrobenzene-d5	0.444	0.398	10.4	65	0.00
9	Naphthalene	1.151	1.116	3.0	71	0.00
10	Hexachlorobutadiene	0.261	0.262	-0.4	68	0.00
11 SURR	2-Methylnaphthalene-d10	0.582	0.552	5.2	69	0.00
12	2-Methylnaphthalene	0.741	0.664	10.4	65	0.00
13 I	Acenaphthene-d10	1.000	1.000	0.0	76	0.00
14 S	2,4,6-Tribromophenol	0.193	0.164	15.0	68	0.00
15 S	2-Fluorobiphenyl	1.921	1.649	14.2	62	0.00
16	Acenaphthylene	1.858	1.966	-5.8	79	0.00
17	Acenaphthene	1.210	1.181	2.4	72	0.00
18	Fluorene	1.669	1.626	2.6	73	0.00
19 I	Phenanthrene-d10	1.000	1.000	0.0	78	0.00
20	4,6-Dinitro-2-methylphenol	0.095	0.077	18.9	63	0.00
21	4-Bromophenyl-phenylether	0.240	0.222	7.5	67	0.00
22	Hexachlorobenzene	0.284	0.265	6.7	67	0.00
23	Atrazine	0.234	0.262	-12.0	78	0.00
24	Pentachlorophenol	0.149	0.146	2.0	70	-0.01
25	Phenanthrene	1.199	1.181	1.5	71	-0.01
26	Anthracene	1.069	1.110	-3.8	75	0.00
27 SURR	Fluoranthene-d10	1.127	1.096	2.8	70	0.00
28	Fluoranthene	1.509	1.494	1.0	72	0.00
29 I	Chrysene-d12	1.000	1.000	0.0	85	0.00
30	Pyrene	1.512	1.405	7.1	74	0.00
31 S	Terphenyl-d14	0.760	0.742	2.4	77	0.00
32	Benzo(a)anthracene	1.413	1.390	1.6	84	0.00
33	Chrysene	1.558	1.600	-2.7	81	0.00
34	Bis(2-ethylhexyl)phthalate	1.049	1.079	-2.9	89	0.00
35 I	Perylene-d12	1.000	1.000	0.0	88	0.00
36	Indeno(1,2,3-cd)pyrene	1.909	2.027	-6.2	89	-0.01
37	Benzo(b)fluoranthene	1.419	1.390	2.0	81	0.00
38	Benzo(k)fluoranthene	1.432	1.532	-7.0	91	0.00
39 C	Benzo(a)pyrene	1.244	1.351	-8.6	89	0.00
40	Dibenzo(a,h)anthracene	1.516	1.603	-5.7	89	0.00
41	Benzo(g,h,i)perylene	1.714	1.768	-3.2	87	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036880.D
Acq On : 11 Apr 2025 16:18
Operator : RC/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN041125

Quant Time: Apr 11 16:41:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	0.400	0.400	0.0	73	0.00
2	1,4-Dioxane	0.400	0.426	-6.5	81	0.00
3	n-Nitrosodimethylamine	0.400	0.455	-13.7	78	0.00
4 S	2-Fluorophenol	0.400	0.394	1.5	70	0.00
5 S	Phenol-d6	0.400	0.340	15.0	62	0.00
6	bis(2-Chloroethyl)ether	0.400	0.403	-0.8	73	0.00
7 I	Naphthalene-d8	0.400	0.400	0.0	74	0.00
8 S	Nitrobenzene-d5	0.400	0.359	10.3	65	0.00
9	Naphthalene	0.400	0.388	3.0	71	0.00
10	Hexachlorobutadiene	0.400	0.402	-0.5	68	0.00
11 SURR	2-Methylnaphthalene-d10	0.400	0.380	5.0	69	0.00
12	2-Methylnaphthalene	0.400	0.358	10.5	65	0.00
13 I	Acenaphthene-d10	0.400	0.400	0.0	76	0.00
14 S	2,4,6-Tribromophenol	0.400	0.340	15.0	68	0.00
15 S	2-Fluorobiphenyl	0.400	0.343	14.2	62	0.00
16	Acenaphthylene	0.400	0.423	-5.7	79	0.00
17	Acenaphthene	0.400	0.391	2.3	72	0.00
18	Fluorene	0.400	0.390	2.5	73	0.00
19 I	Phenanthrene-d10	0.400	0.400	0.0	78	0.00
20	4,6-Dinitro-2-methylphenol	0.400	0.327	18.3	63	0.00
21	4-Bromophenyl-phenylether	0.400	0.371	7.3	67	0.00
22	Hexachlorobenzene	0.400	0.374	6.5	67	0.00
23	Atrazine	0.400	0.448	-12.0	78	0.00
24	Pentachlorophenol	0.400	0.393	1.8	70	-0.01
25	Phenanthrene	0.400	0.394	1.5	71	-0.01
26	Anthracene	0.400	0.415	-3.7	75	0.00
27 SURR	Fluoranthene-d10	0.400	0.389	2.8	70	0.00
28	Fluoranthene	0.400	0.396	1.0	72	0.00
29 I	Chrysene-d12	0.400	0.400	0.0	85	0.00
30	Pyrene	0.400	0.372	7.0	74	0.00
31 S	Terphenyl-d14	0.400	0.391	2.3	77	0.00
32	Benzo(a)anthracene	0.400	0.394	1.5	84	0.00
33	Chrysene	0.400	0.411	-2.7	81	0.00
34	Bis(2-ethylhexyl)phthalate	0.400	0.412	-3.0	89	0.00
35 I	Perylene-d12	0.400	0.400	0.0	88	0.00
36	Indeno(1,2,3-cd)pyrene	0.400	0.425	-6.2	89	-0.01
37	Benzo(b)fluoranthene	0.400	0.392	2.0	81	0.00
38	Benzo(k)fluoranthene	0.400	0.428	-7.0	91	0.00
39 C	Benzo(a)pyrene	0.400	0.434	-8.5	89	0.00
40	Dibenzo(a,h)anthracene	0.400	0.423	-5.7	89	0.00
41	Benzo(g,h,i)perylene	0.400	0.413	-3.2	87	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\
 Method File : 8270-SIM-BN041425.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 14 17:58:02 2025
 Response Via : Initial Calibration

Calibration Files

0.1 =BN036898.D 0.2 =BN036899.D 0.4 =BN036900.D 0.8 =BN036901.D 1.6 =BN036902.D 3.2 =BN036903.D 5.0 =BN036904.D

	Compound	0.1	0.2	0.4	0.8	1.6	3.2	5.0	Avg	%RSD

1) I	1,4-Dichlorobenzen...	-----ISTD-----								
2)	1,4-Dioxane	0.488	0.462	0.500	0.459	0.431	0.458	0.404	0.457	7.10
3)	n-Nitrosodimet...	1.146	1.039	1.128	1.054	1.025	1.081	0.921	1.056	7.05
4) S	2-Fluorophenol	0.962	0.927	0.962	0.910	0.920	1.016	0.920	0.945	3.96
5) S	Phenol-d6	1.247	1.081	1.169	1.134	1.155	1.317	1.202	1.186	6.54
6)	bis(2-Chloroet...	1.354	1.076	1.149	1.108	1.087	1.209	1.069	1.150	8.91
7) I	Naphthalene-d8	-----ISTD-----								
8) S	Nitrobenzene-d5	0.588	0.413	0.444	0.410	0.418	0.467	0.425	0.452	13.96
9)	Naphthalene	1.326	1.123	1.198	1.090	1.090	1.215	1.095	1.162	7.65
10)	Hexachlorobuta...	0.287	0.273	0.286	0.256	0.255	0.274	0.241	0.267	6.39
11) SURR	2-Methylnaphth...	0.597	0.560	0.594	0.550	0.559	0.641	0.578	0.583	5.37
12)	2-Methylnaphth...	0.785	0.681	0.748	0.699	0.718	0.815	0.732	0.740	6.41
13) I	Acenaphthene-d10	-----ISTD-----								
14) S	2,4,6-Tribromo...	0.188	0.177	0.197	0.181	0.192	0.215	0.195	0.192	6.39
15) S	2-Fluorobiphenyl	2.001	1.954	2.026	1.673	1.914	2.052	1.895	1.931	6.59
16)	Acenaphthylene	1.914	1.791	1.902	1.797	1.853	2.091	1.934	1.897	5.37
17)	Acenaphthene	1.287	1.193	1.273	1.206	1.206	1.348	1.239	1.250	4.47
18)	Fluorene	1.629	1.556	1.671	1.593	1.624	1.832	1.648	1.650	5.35
19) I	Phenanthrene-d10	-----ISTD-----								
20)	4,6-Dinitro-2-...	0.082	0.108	0.102	0.107	0.129	0.125	0.109		15.78
21)	4-Bromophenyl-...	0.243	0.245	0.274	0.243	0.250	0.273	0.247	0.253	5.49
22)	Hexachlorobenzene	0.295	0.284	0.310	0.274	0.271	0.291	0.264	0.284	5.64
23)	Atrazine	0.198	0.186	0.238	0.209	0.206	0.234	0.206	0.211	8.88
24)	Pentachlorophenol	0.139	0.134	0.159	0.141	0.150	0.174	0.165	0.152	9.94
25)	Phenanthrene	1.198	1.158	1.318	1.163	1.191	1.329	1.225	1.226	5.75
26)	Anthracene	1.022	1.013	1.168	1.048	1.087	1.243	1.145	1.104	7.70
27) SURR	Fluoranthene-d10	0.988	0.964	1.136	1.021	1.034	1.185	1.078	1.058	7.54
28)	Fluoranthene	1.355	1.283	1.535	1.399	1.416	1.631	1.470	1.441	8.05
29) I	Chrysene-d12	-----ISTD-----								
30)	Pyrene	1.791	1.849	1.827	1.684	1.804	1.883	1.761	1.800	3.60
31) S	Terphenyl-d14	0.855	0.880	0.904	0.837	0.873	0.919	0.859	0.875	3.26
32)	Benzo(a)anthra...	1.379	1.332	1.465	1.400	1.474	1.613	1.498	1.452	6.35
33)	Chrysene	1.590	1.555	1.639	1.508	1.531	1.665	1.492	1.569	4.19
34)	Bis(2-ethylhex...	0.936	0.750	0.868	0.822	0.738	0.933	0.815	0.837	9.52
35) I	Perylene-d12	-----ISTD-----								

Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\

Method File : 8270-SIM-BN041425.M

36)	Indeno(1,2,3-c...	1.313	1.363	1.525	1.411	1.420	1.653	1.464	1.450	7.76
37)	Benzo(b)fluora...	1.376	1.465	1.636	1.465	1.559	1.702	1.627	1.547	7.53
38)	Benzo(k)fluora...	1.406	1.495	1.680	1.483	1.532	1.713	1.628	1.562	7.25
39) C	Benzo(a)pyrene	1.177	1.198	1.372	1.223	1.279	1.435	1.348	1.290	7.55
40)	Dibenzo(a,h)an...	1.030	1.049	1.183	1.092	1.102	1.289	1.148	1.128	7.86
41)	Benzo(g,h,i)pe...	1.169	1.211	1.332	1.201	1.202	1.385	1.211	1.244	6.50

(#) = Out of Range

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
 Data File : BN036898.D
 Acq On : 14 Apr 2025 13:26
 Operator : RC/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Apr 14 17:35:14 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 17:32:00 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	1941	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	4829	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	2579	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	5391	0.400	ng	0.00
29) Chrysene-d12	21.224	240	4097	0.400	ng	0.00
35) Perylene-d12	23.433	264	3972	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	467	0.102	ng	0.00
5) Phenol-d6	6.809	99	605	0.105	ng	0.00
8) Nitrobenzene-d5	8.781	82	710	0.130	ng	0.00
11) 2-Methylnaphthalene-d10	12.016	152	721	0.102	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	121	0.098	ng	0.00
15) 2-Fluorobiphenyl	12.904	172	1290	0.104	ng	0.00
27) Fluoranthene-d10	19.063	212	1332	0.093	ng	0.00
31) Terphenyl-d14	19.672	244	876	0.098	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	237m	0.105	ng	
3) n-Nitrosodimethylamine	3.473	42	556	0.108	ng	94
6) bis(2-Chloroethyl)ether	7.062	93	657	0.118	ng	97
9) Naphthalene	10.468	128	1601	0.114	ng	# 95
10) Hexachlorobutadiene	10.756	225	346	0.107	ng	# 99
12) 2-Methylnaphthalene	12.092	142	948	0.106	ng	99
16) Acenaphthylene	13.999	152	1234	0.101	ng	99
17) Acenaphthene	14.341	154	830	0.103	ng	97
18) Fluorene	15.336	166	1050	0.099	ng	99
21) 4-Bromophenyl-phenylether	16.227	248	327	0.096	ng	# 90
22) Hexachlorobenzene	16.338	284	398	0.104	ng	98
23) Atrazine	16.500	200	267	0.094	ng	# 78
24) Pentachlorophenol	16.686	266	187	0.091	ng	94
25) Phenanthrene	17.071	178	1615	0.098	ng	99
26) Anthracene	17.157	178	1378	0.093	ng	100
28) Fluoranthene	19.096	202	1826	0.094	ng	99
30) Pyrene	19.458	202	1834	0.099	ng	99
32) Benzo(a)anthracene	21.206	228	1412	0.095	ng	94
33) Chrysene	21.260	228	1629	0.101	ng	95
34) Bis(2-ethylhexyl)phtha...	21.144	149	959	0.112	ng	# 97
36) Indeno(1,2,3-cd)pyrene	25.658	276	1304	0.091	ng	98
37) Benzo(b)fluoranthene	22.772	252	1366	0.089	ng	# 70
38) Benzo(k)fluoranthene	22.816	252	1396	0.090	ng	# 68
39) Benzo(a)pyrene	23.339	252	1169	0.091	ng	# 66
40) Dibenzo(a,h)anthracene	25.669	278	1023	0.091	ng	# 67
41) Benzo(g,h,i)perylene	26.330	276	1161	0.094	ng	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036898.D
Acq On : 14 Apr 2025 13:26
Operator : RC/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Apr 14 17:35:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:32:00 2025
Response via : Initial Calibration




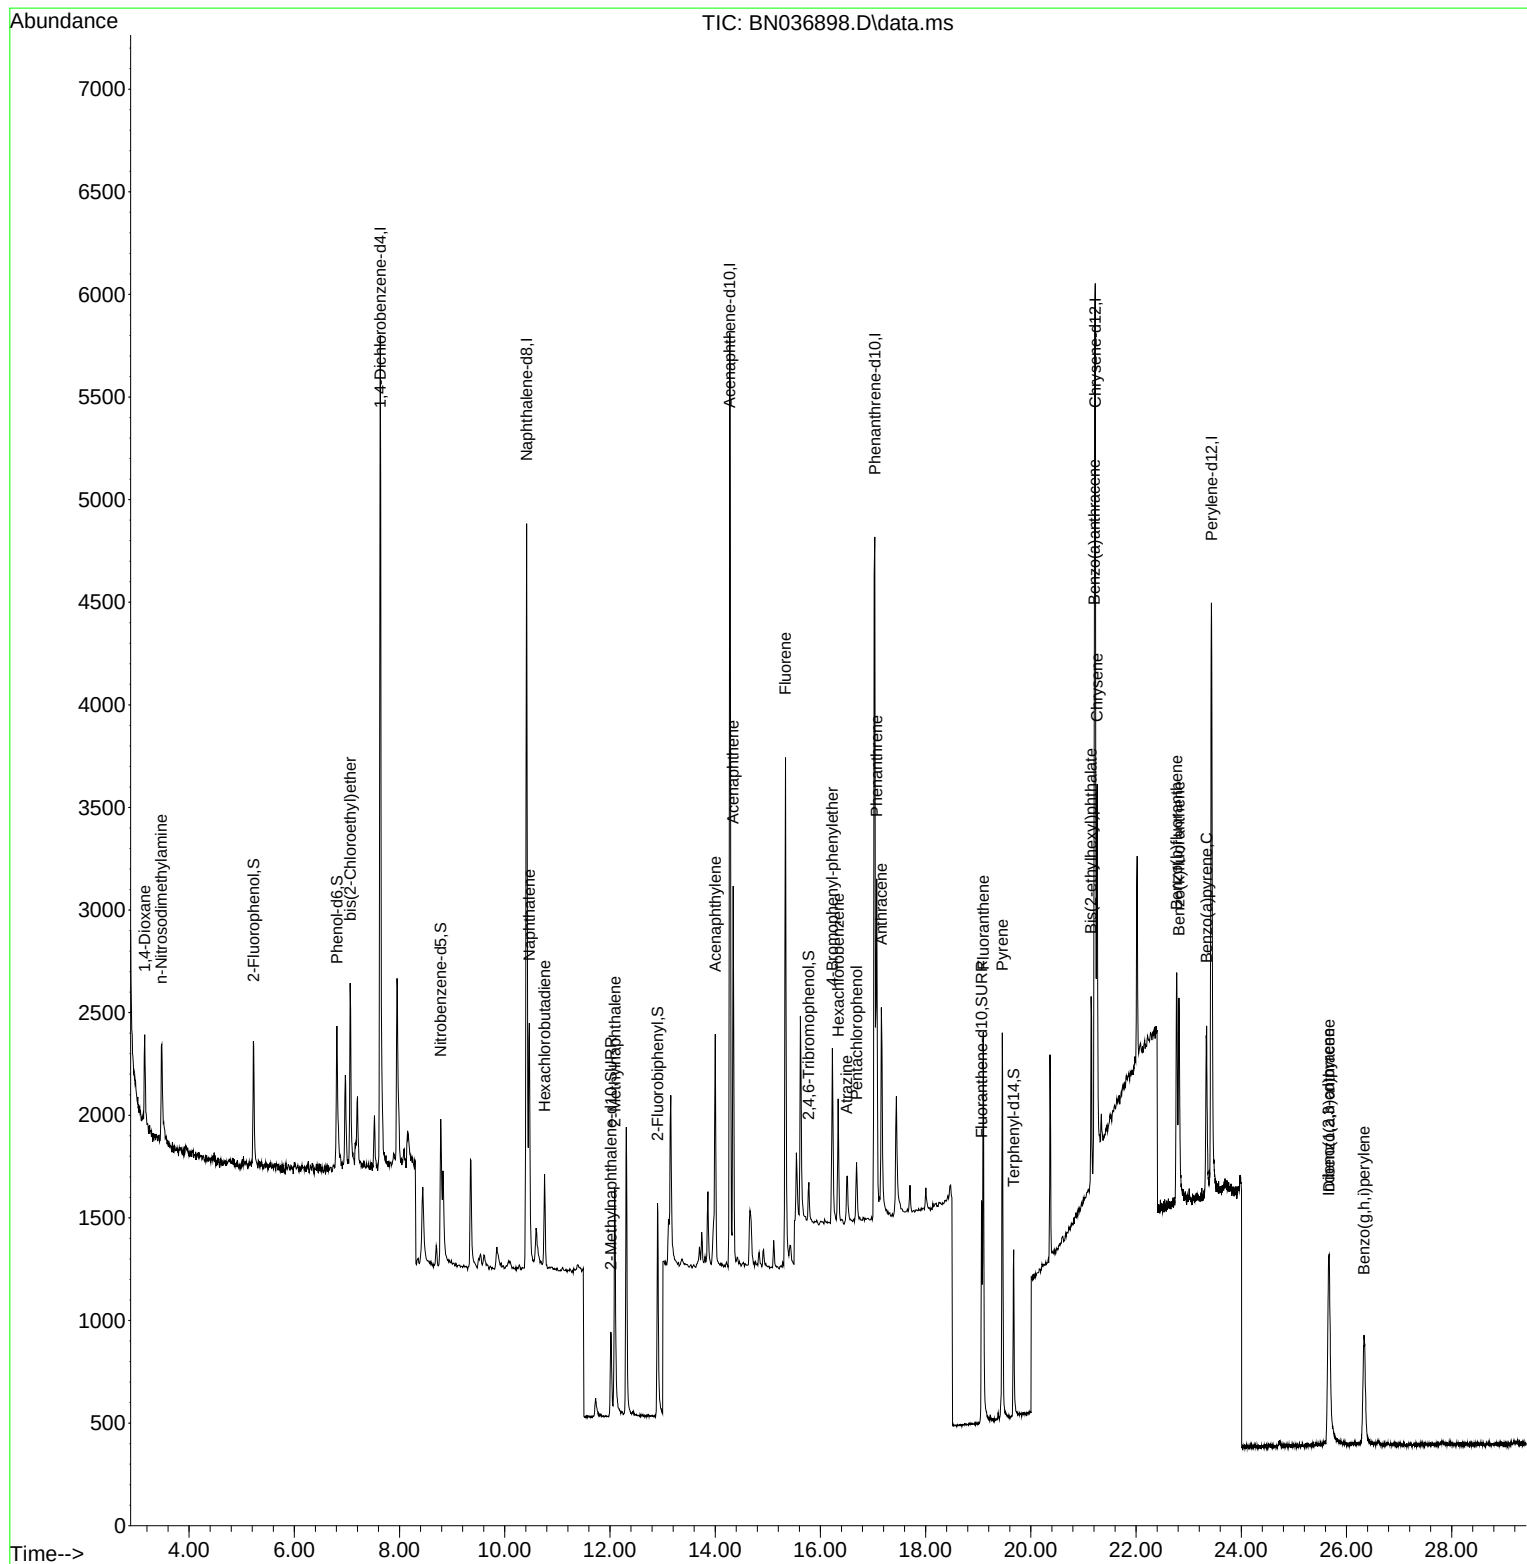




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 152 Resp: 1941
Ion Ratio Lower Upper
152 100
150 152.4 121.4 182.2
115 68.0 55.4 83.2



#2
1,4-Dioxane
Concen: 0.105 ng m
RT: 3.155 min Scan# 38
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26

Tgt Ion: 88 Resp: 237
Ion Ratio Lower Upper
88 100
43 65.8 43.7 65.5#
58 101.3 67.8 101.8









#3
n-Nitrosodimethylamine
Concen: 0.108 ng
RT: 3.473 min Scan# 81
Delta R.T. 0.007 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 42 Resp: 556
Ion Ratio Lower Upper
42 100
74 70.9 52.3 78.5
44 8.3 7.4 11.2



#4
2-Fluorophenol
Concen: 0.102 ng
RT: 5.228 min Scan# 325
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26

Tgt Ion: 112 Resp: 467
Ion Ratio Lower Upper
112 100
64 69.6 54.4 81.6
63 45.4 35.1 52.7









#5
Phenol-d6
Concen: 0.105 ng
RT: 6.809 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 99 Resp: 605
Ion Ratio Lower Upper
99 100
42 40.8 30.6 45.8
71 48.4 38.0 57.0



#6
bis(2-Chloroethyl)ether
Concen: 0.118 ng
RT: 7.062 min Scan# 579
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26

Tgt Ion: 93 Resp: 657
Ion Ratio Lower Upper
93 100
63 86.1 70.7 106.1
95 33.2 25.2 37.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	136	Resp:	4829
Ion	Ratio	Lower	Upper
136	100		
137	12.3	10.6	15.8
54	12.4	10.6	16.0
68	7.6	6.1	9.1



#8
Nitrobenzene-d5
Concen: 0.130 ng
RT: 8.781 min Scan# 796
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26

Tgt Ion:	82	Resp:	710
Ion	Ratio	Lower	Upper
82	100		
128	39.6	29.0	43.4
54	76.2	60.8	91.2





#9

Naphthalene

Concen: 0.114 ng

RT: 10.468 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:128 Resp: 1601

Ion Ratio Lower Upper

128 100

129 15.5 10.3 15.5#

127 17.6 12.7 19.1



#10

Hexachlorobutadiene

Concen: 0.107 ng

RT: 10.756 min Scan# 981

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:225 Resp: 346


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 64.2 51.0 76.4









#11
2-Methylnaphthalene-d10
Concen: 0.102 ng
RT: 12.016 min Scan# 1152
Delta R.T. 0.005 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 721
Ion Ratio Lower Upper
152 100
151 22.1 17.1 25.7



#12
2-Methylnaphthalene
Concen: 0.106 ng
RT: 12.092 min Scan# 1167
Delta R.T. 0.005 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26

Tgt Ion:142 Resp: 948
Ion Ratio Lower Upper
142 100
141 90.7 73.0 109.4
115 52.1 41.1 61.7









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:164 Resp: 2579
Ion Ratio Lower Upper
164 100
162 106.0 83.8 125.8
160 56.8 44.7 67.1



#14
2,4,6-Tribromophenol
Concen: 0.098 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26

Tgt Ion:330 Resp: 121
Ion Ratio Lower Upper
330 100
332 89.3 77.0 115.6
141 49.6 44.5 66.7





#15

2-Fluorobiphenyl

Concen: 0.104 ng

RT: 12.904 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:172 Resp: 1290

Ion Ratio Lower Upper

172 100

171 40.4 29.2 43.8

170 29.2 20.5 30.7



#16

Acenaphthylene

Concen: 0.101 ng

RT: 13.999 min Scan# 1440

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:152 Resp: 1234


Ion Ratio Lower Upper

152 100

151 19.9 15.8 23.8

153 13.7 10.2 15.4





#17

Acenaphthene

Concen: 0.103 ng

RT: 14.341 min Scan# 1472

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:154 Resp: 830

Ion Ratio Lower Upper

154 100

153 121.9 94.7 142.1

152 63.1 49.4 74.2



#18

Fluorene

Concen: 0.099 ng

RT: 15.336 min Scan# 1565

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:166 Resp: 1050


Ion Ratio Lower Upper

166 100

165 102.0 80.9 121.3

167 14.7 10.9 16.3





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:188 Resp: 5391

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.1 7.1 10.7



#21

4-Bromophenyl-phenylether

Concen: 0.096 ng

RT: 16.227 min Scan# 1639

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:248 Resp: 327


Ion Ratio Lower Upper

248 100

250 95.2 77.0 115.6

141 97.4 63.0 94.4#





#22

Hexachlorobenzene

Concen: 0.104 ng

RT: 16.338 min Scan# 1648

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:284 Resp: 398

Ion Ratio Lower Upper

284 100

142 50.8 42.6 64.0

249 36.9 29.1 43.7



#23

Atrazine

Concen: 0.094 ng

RT: 16.500 min Scan# 1661

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:200 Resp: 267


Ion Ratio Lower Upper

200 100

173 47.6 25.0 37.4#

215 57.1 37.2 55.8#





#24

Pentachlorophenol

Concen: 0.091 ng

RT: 16.686 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:266 Resp: 187

Ion Ratio Lower Upper

266 100

264 56.1 50.8 76.2

268 61.5 50.6 76.0



#25

Phenanthrene

Concen: 0.098 ng

RT: 17.071 min Scan# 1707

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:178 Resp: 1615


Ion Ratio Lower Upper

178 100

176 20.3 16.2 24.2

179 16.3 12.2 18.4





#26

Anthracene

Concen: 0.093 ng

RT: 17.157 min Scan# 1714

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:178 Resp: 1378

Ion Ratio Lower Upper

178 100

176 19.0 15.4 23.0

179 14.9 11.9 17.9



#27

Fluoranthene-d10

Concen: 0.093 ng

RT: 19.063 min Scan# 1942

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:212 Resp: 1332


Ion Ratio Lower Upper

212 100

106 13.3 10.6 15.8

104 9.2 6.6 10.0









#28
Fluoranthene
Concen: 0.094 ng
RT: 19.096 min Scan# 1949
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.9	8.2	12.4
203	16.7	13.6	20.4



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.224 min Scan# 2281
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26

Tgt Ion	Ratio	Lower	Upper
240	100		
120	11.7	9.8	14.6
236	29.8	23.1	34.7

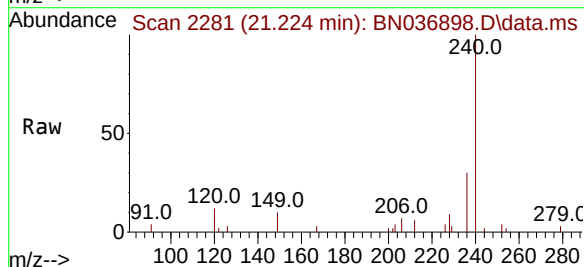



#30

Pyrene

Concen: 0.099 ng

RT: 19.458 min Scan# 2027

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1




Tgt Ion:202 Resp: 1834

Ion Ratio Lower Upper

202 100

200 21.5 17.0 25.6

203 18.2 14.1 21.1



#31

Terphenyl-d14

Concen: 0.098 ng

RT: 19.672 min Scan# 2073

Delta R.T. 0.004 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:244 Resp: 876


Ion Ratio Lower Upper

244 100

212 16.7 10.1 15.1#

122 22.2 13.6 20.4#









#32
Benzo(a)anthracene
Concen: 0.095 ng
RT: 21.206 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:228 Resp: 1412
Ion Ratio Lower Upper
228 100
226 31.0 22.5 33.7
229 23.7 16.2 24.4



#33
Chrysene
Concen: 0.101 ng
RT: 21.260 min Scan# 2285
Delta R.T. -0.000 min
Lab File: BN036898.D
Acq: 14 Apr 2025 13:26

Tgt Ion:228 Resp: 1629
Ion Ratio Lower Upper
228 100
226 33.1 24.9 37.3
229 23.0 15.9 23.9

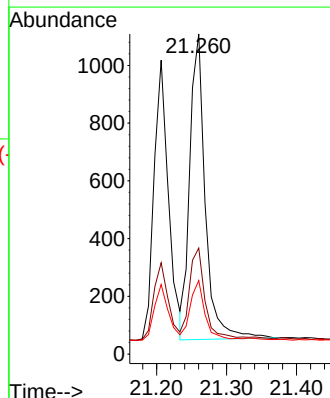



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.112 ng

RT: 21.144 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:149 Resp: 959

Ion Ratio Lower Upper

149 100

167 25.8 21.8 32.6

279 5.9 3.0 4.4#



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.433 min Scan# 2764

Delta R.T. -0.000 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:264 Resp: 3972


Ion Ratio Lower Upper

264 100

260 27.1 22.3 33.5

265 65.1 57.6 86.4





#36

Indeno(1,2,3-cd)pyrene

Concen: 0.091 ng

RT: 25.658 min Scan# 3525

Delta R.T. 0.006 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:276 Resp: 1304

Ion Ratio Lower Upper

276 100

138 24.1 20.3 30.5

277 25.0 20.3 30.5



#37

Benzo(b)fluoranthene

Concen: 0.089 ng

RT: 22.772 min Scan# 2538

Delta R.T. 0.003 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:252 Resp: 1366


Ion Ratio Lower Upper

252 100

253 42.9 22.0 33.0#

125 30.8 13.7 20.5#





#38

Benzo(k)fluoranthene

Concen: 0.090 ng

RT: 22.816 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:252 Resp: 1396

Ion Ratio Lower Upper

252 100

253 45.4 22.7 34.1#

125 28.9 12.5 18.7#



#39

Benzo(a)pyrene

Concen: 0.091 ng

RT: 23.339 min Scan# 2732

Delta R.T. 0.003 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:252 Resp: 1169


Ion Ratio Lower Upper

252 100

253 52.3 25.8 38.6#

125 42.4 20.7 31.1#





#40

Dibenzo(a,h)anthracene

Concen: 0.091 ng

RT: 25.669 min Scan# 3529

Delta R.T. -0.006 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:278 Resp: 1023

Ion Ratio Lower Upper

278 100

139 29.9 16.9 25.3#

279 56.1 25.7 38.5#



#41

Benzo(g,h,i)perylene

Concen: 0.094 ng

RT: 26.330 min Scan# 3755

Delta R.T. -0.006 min

Lab File: BN036898.D

Acq: 14 Apr 2025 13:26




Tgt Ion:276 Resp: 1161

Ion Ratio Lower Upper

276 100

277 36.5 21.3 31.9#

138 34.7 20.8 31.2#



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
 Data File : BN036899.D
 Acq On : 14 Apr 2025 14:02
 Operator : RC/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Apr 14 17:35:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 17:32:00 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	1758	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	4308	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	2368	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	4862	0.400	ng	0.00
29) Chrysene-d12	21.224	240	3423	0.400	ng	0.00
35) Perylene-d12	23.433	264	3030	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	815	0.196	ng	0.00
5) Phenol-d6	6.809	99	950	0.182	ng	0.00
8) Nitrobenzene-d5	8.781	82	890	0.183	ng	0.00
11) 2-Methylnaphthalene-d10	12.016	152	1206	0.192	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	210	0.185	ng	0.00
15) 2-Fluorobiphenyl	12.904	172	2314	0.202	ng	0.00
27) Fluoranthene-d10	19.063	212	2344	0.182	ng	0.00
31) Terphenyl-d14	19.672	244	1506	0.201	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	406m	0.198	ng	
3) n-Nitrosodimethylamine	3.473	42	913	0.197	ng	# 95
6) bis(2-Chloroethyl)ether	7.069	93	946	0.187	ng	100
9) Naphthalene	10.468	128	2420	0.193	ng	98
10) Hexachlorobutadiene	10.757	225	587	0.204	ng	# 100
12) 2-Methylnaphthalene	12.087	142	1467	0.184	ng	98
16) Acenaphthylene	13.999	152	2121	0.189	ng	100
17) Acenaphthene	14.341	154	1413	0.191	ng	100
18) Fluorene	15.336	166	1842	0.189	ng	99
20) 4,6-Dinitro-2-methylph...	15.421	198	199	0.150	ng	# 56
21) 4-Bromophenyl-phenylether	16.227	248	596	0.193	ng	96
22) Hexachlorobenzene	16.338	284	691	0.200	ng	97
23) Atrazine	16.500	200	451	0.176	ng	# 87
24) Pentachlorophenol	16.686	266	325	0.176	ng	97
25) Phenanthrene	17.071	178	2816	0.189	ng	99
26) Anthracene	17.158	178	2462	0.184	ng	98
28) Fluoranthene	19.096	202	3118	0.178	ng	99
30) Pyrene	19.458	202	3165	0.206	ng	99
32) Benzo(a)anthracene	21.207	228	2280	0.184	ng	97
33) Chrysene	21.260	228	2662	0.198	ng	98
34) Bis(2-ethylhexyl)phtha...	21.144	149	1283	0.179	ng	97
36) Indeno(1,2,3-cd)pyrene	25.655	276	2065	0.188	ng	98
37) Benzo(b)fluoranthene	22.772	252	2219	0.189	ng	# 83
38) Benzo(k)fluoranthene	22.813	252	2265	0.191	ng	# 86
39) Benzo(a)pyrene	23.339	252	1815	0.186	ng	# 86
40) Dibenzo(a,h)anthracene	25.678	278	1589	0.186	ng	# 85
41) Benzo(g,h,i)perylene	26.336	276	1834	0.195	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036899.D
Acq On : 14 Apr 2025 14:02
Operator : RC/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Apr 14 17:35:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:32:00 2025
Response via : Initial Calibration




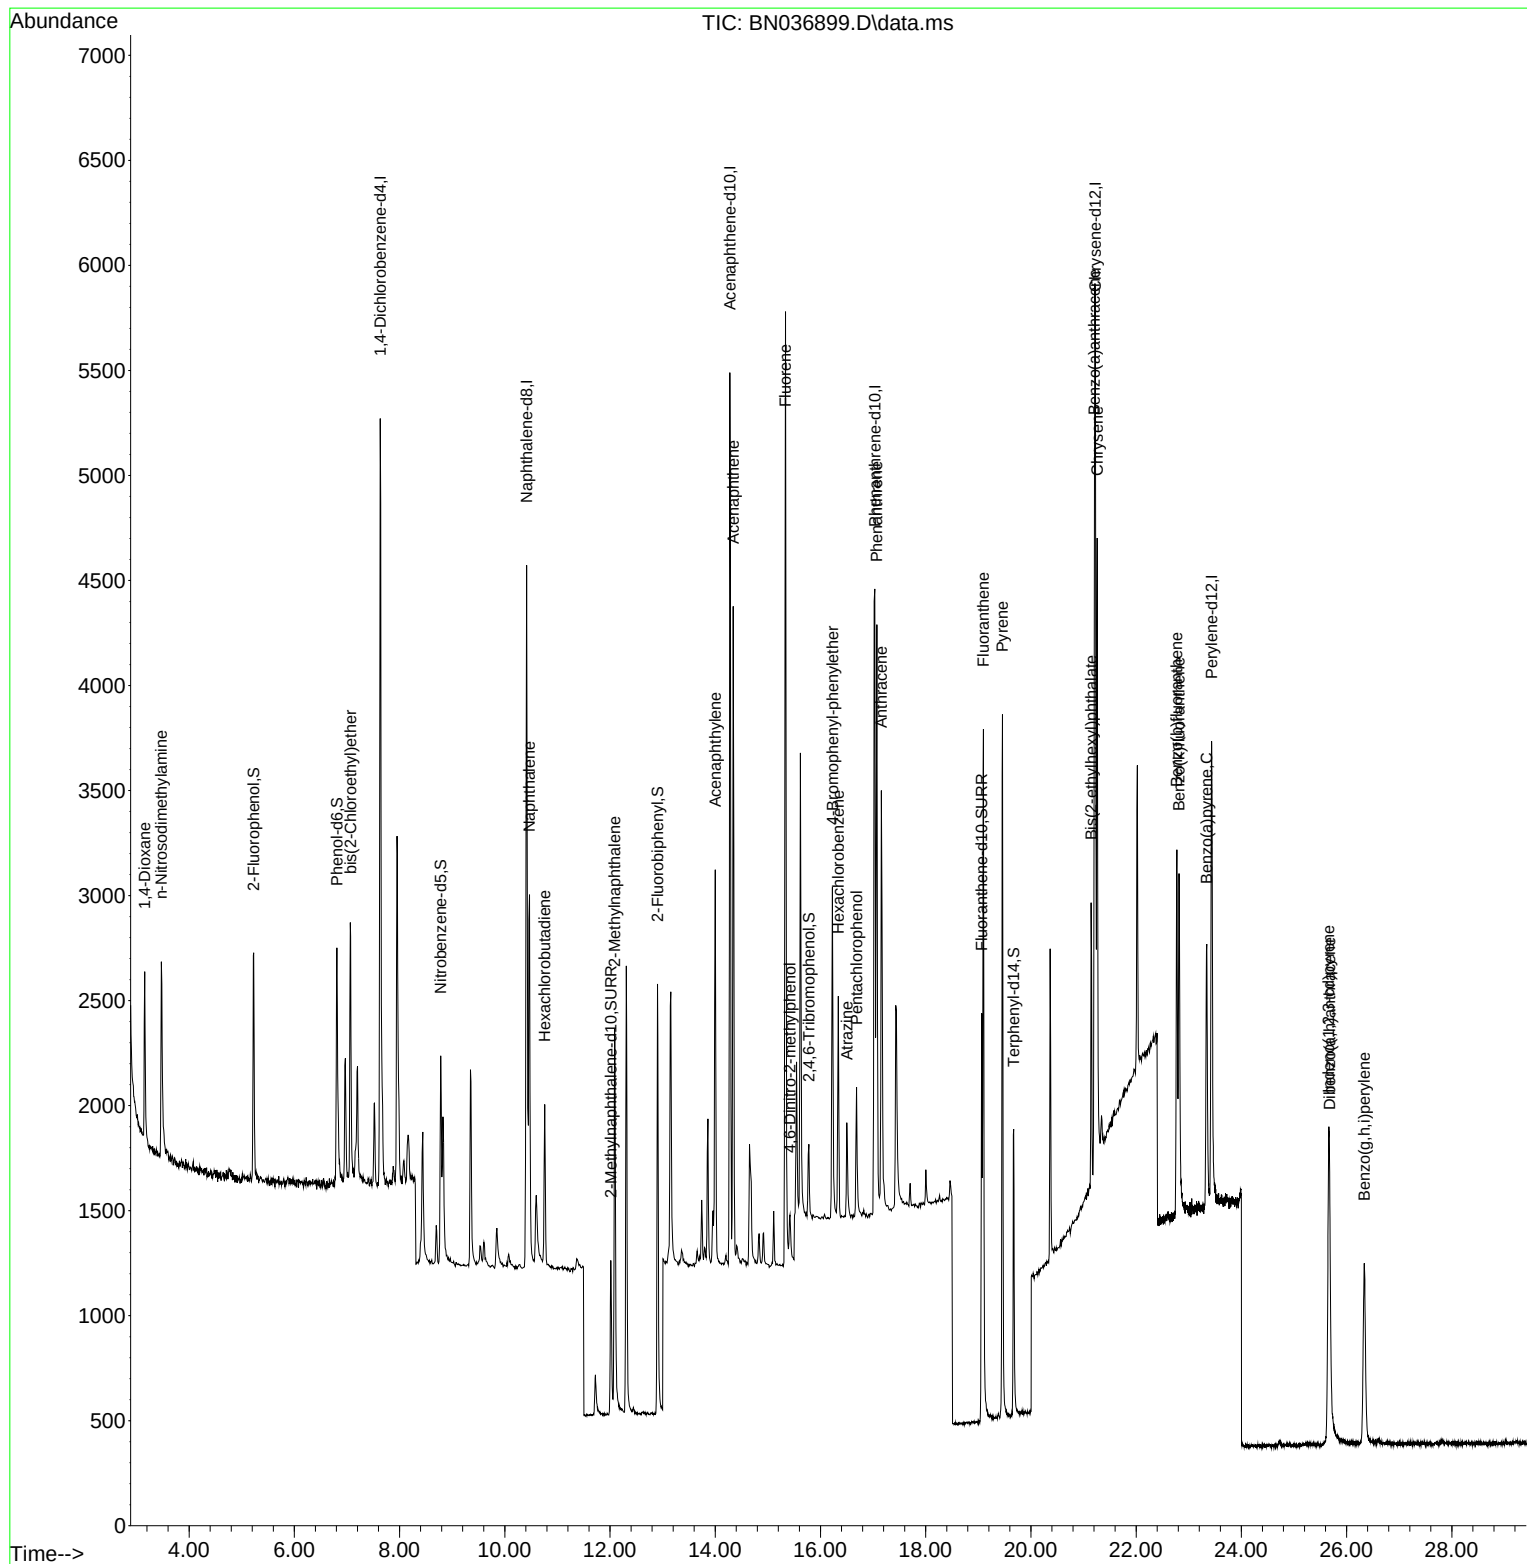




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:152 Resp: 1758
Ion Ratio Lower Upper
152 100
150 154.9 121.4 182.2
115 68.8 55.4 83.2



#2
1,4-Dioxane
Concen: 0.198 ng m
RT: 3.155 min Scan# 38
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion: 88 Resp: 406
Ion Ratio Lower Upper
88 100
43 54.4 43.7 65.5
58 91.6 67.8 101.8









#3
n-Nitrosodimethylamine
Concen: 0.197 ng
RT: 3.473 min Scan# 81
Delta R.T. 0.007 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion: 42 Resp: 913
Ion Ratio Lower Upper
42 100
74 64.8 52.3 78.5
44 22.1 7.4 11.2#



#4
2-Fluorophenol
Concen: 0.196 ng
RT: 5.228 min Scan# 325
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion: 112 Resp: 815
Ion Ratio Lower Upper
112 100
64 69.0 54.4 81.6
63 44.7 35.1 52.7









#5
Phenol-d6
Concen: 0.182 ng
RT: 6.809 min Scan# 54
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion	Resp		
Ion	Ratio	Lower	Upper
99	100		
42	38.2	30.6	45.8
71	46.9	38.0	57.0



#6
bis(2-Chloroethyl)ether
Concen: 0.187 ng
RT: 7.069 min Scan# 580
Delta R.T. 0.007 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion	Resp		
Ion	Ratio	Lower	Upper
93	100		
63	88.6	70.7	106.1
95	31.2	25.2	37.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:	136	Resp:	4308
Ion	Ratio	Lower	Upper
136	100		
137	12.1	10.6	15.8
54	13.5	10.6	16.0
68	7.6	6.1	9.1



#8
Nitrobenzene-d5
Concen: 0.183 ng
RT: 8.781 min Scan# 796
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion:	82	Resp:	890
Ion	Ratio	Lower	Upper
82	100		
128	40.5	29.0	43.4
54	78.8	60.8	91.2





#9

Naphthalene

Concen: 0.193 ng

RT: 10.468 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:128 Resp: 2420

Ion Ratio Lower Upper

128 100

129 14.5 10.3 15.5

127 15.8 12.7 19.1



#10

Hexachlorobutadiene

Concen: 0.204 ng

RT: 10.757 min Scan# 981

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:225 Resp: 587


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.9 51.0 76.4









#11
2-Methylnaphthalene-d10
Concen: 0.192 ng
RT: 12.016 min Scan# 1151
Delta R.T. 0.005 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:152 Resp: 1206
Ion Ratio Lower Upper
152 100
151 21.6 17.1 25.7



#12
2-Methylnaphthalene
Concen: 0.184 ng
RT: 12.087 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion:142 Resp: 1467
Ion Ratio Lower Upper
142 100
141 91.7 73.0 109.4
115 54.6 41.1 61.7









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. 0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion	164	Resp	2368
Ion	Ratio	Lower	Upper
164	100		
162	106.5	83.8	125.8
160	56.0	44.7	67.1



#14
2,4,6-Tribromophenol
Concen: 0.185 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion	330	Resp	210
Ion	Ratio	Lower	Upper
330	100		
332	99.5	77.0	115.6
141	51.4	44.5	66.7









#15
2-Fluorobiphenyl
Concen: 0.202 ng
RT: 12.904 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.5	29.2	43.8
170	26.8	20.5	30.7



#16
Acenaphthylene
Concen: 0.189 ng
RT: 13.999 min Scan# 1440
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.9	15.8	23.8
153	12.9	10.2	15.4

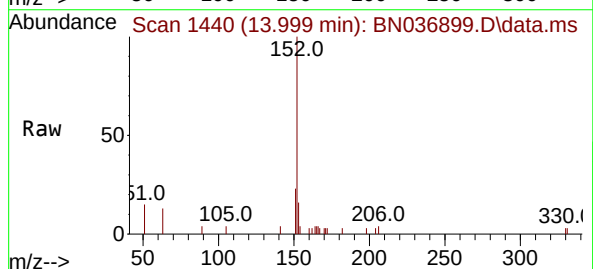



#17

Acenaphthene

Concen: 0.191 ng

RT: 14.341 min Scan# 1472

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:154 Resp: 1413

Ion Ratio Lower Upper

154 100

153 118.7 94.7 142.1

152 62.1 49.4 74.2



#18

Fluorene

Concen: 0.189 ng

RT: 15.336 min Scan# 1565

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:166 Resp: 1842


Ion Ratio Lower Upper

166 100

165 100.2 80.9 121.3

167 13.7 10.9 16.3





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:188 Resp: 4862

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.1 7.1 10.7



#20

4,6-Dinitro-2-methylphenol

Concen: 0.150 ng

RT: 15.421 min Scan# 1573

Delta R.T. 0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:198 Resp: 199


Ion Ratio Lower Upper

198 100

51 134.8 68.4 102.6#

105 66.7 38.7 58.1#









#21
4-Bromophenyl-phenylether
Concen: 0.193 ng
RT: 16.227 min Scan# 1639
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion	Ratio	Lower	Upper
248	100		
250	93.4	77.0	115.6
141	83.8	63.0	94.4



#22
Hexachlorobenzene
Concen: 0.200 ng
RT: 16.338 min Scan# 1648
Delta R.T. 0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion	Ratio	Lower	Upper
284	100		
142	50.4	42.6	64.0
249	36.0	29.1	43.7









#23
Atrazine
Concen: 0.176 ng
RT: 16.500 min Scan# 1661
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:200 Resp: 451
Ion Ratio Lower Upper
200 100
173 39.7 25.0 37.4#
215 54.3 37.2 55.8



#24
Pentachlorophenol
Concen: 0.176 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.000 min
Lab File: BN036899.D
Acq: 14 Apr 2025 14:02

Tgt Ion:266 Resp: 325
Ion Ratio Lower Upper
266 100
264 59.4 50.8 76.2
268 63.1 50.6 76.0





#25

Phenanthrene

Concen: 0.189 ng

RT: 17.071 min Scan# 1707

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:178 Resp: 2816

Ion Ratio Lower Upper

178 100

176 19.6 16.2 24.2

179 15.9 12.2 18.4



#26

Anthracene

Concen: 0.184 ng

RT: 17.158 min Scan# 1714

Delta R.T. 0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:178 Resp: 2462


Ion Ratio Lower Upper

178 100

176 18.8 15.4 23.0

179 16.4 11.9 17.9





#27

Fluoranthene-d10

Concen: 0.182 ng

RT: 19.063 min Scan# 1942

Delta R.T. 0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02





Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2

Tgt Ion:	212	Resp:	2344
Ion Ratio	Lower	Upper	
212	100		
106	12.5	10.6	15.8
104	8.2	6.6	10.0



#28

Fluoranthene

Concen: 0.178 ng




RT: 19.096 min Scan# 1949


Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Tgt Ion:	202	Resp:	3118
Ion Ratio	Lower	Upper	
202	100		
101	9.7	8.2	12.4
203	16.7	13.6	20.4

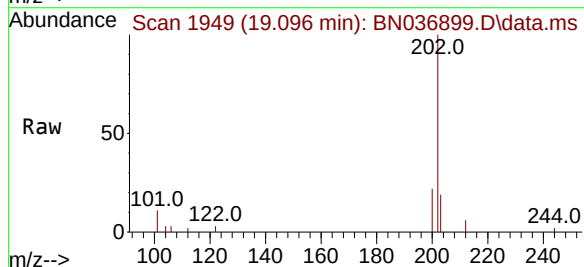



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:240 Resp: 3423

Ion Ratio Lower Upper

240 100

120 11.5 9.8 14.6

236 29.5 23.1 34.7



#30

Pyrene

Concen: 0.206 ng

RT: 19.458 min Scan# 2027

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:202 Resp: 3165


Ion Ratio Lower Upper

202 100

200 21.5 17.0 25.6

203 17.3 14.1 21.1





#31

Terphenyl-d14

Concen: 0.201 ng

RT: 19.672 min Scan# 2073

Delta R.T. 0.005 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:244 Resp: 1506

Ion Ratio Lower Upper

244 100

212 13.8 10.1 15.1

122 18.3 13.6 20.4



#32

Benzo(a)anthracene

Concen: 0.184 ng

RT: 21.207 min Scan# 2279

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:228 Resp: 2280


Ion Ratio Lower Upper

228 100

226 29.9 22.5 33.7

229 21.2 16.2 24.4

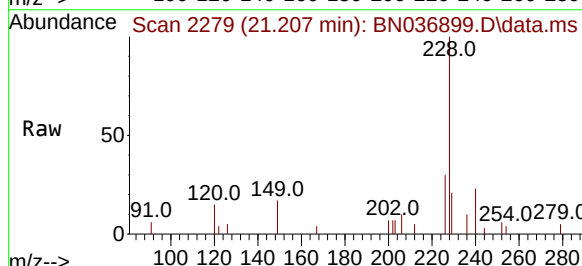



#33

Chrysene

Concen: 0.198 ng

RT: 21.260 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:228 Resp: 2662

Ion Ratio Lower Upper

228 100

226 32.0 24.9 37.3

229 21.3 15.9 23.9



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.179 ng

RT: 21.144 min Scan# 2272

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:149 Resp: 1283


Ion Ratio Lower Upper

149 100

167 25.6 21.8 32.6

279 3.7 3.0 4.4

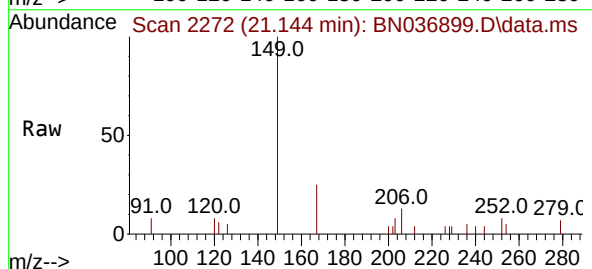



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.433 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.2





Tgt Ion:264 Resp: 3030

Ion Ratio Lower Upper

264 100

260 27.7 22.3 33.5

265 73.7 57.6 86.4



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.188 ng

RT: 25.655 min Scan# 3524

Delta R.T. 0.003 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:276 Resp: 2065


Ion Ratio Lower Upper

276 100

138 24.3 20.3 30.5

277 24.3 20.3 30.5





#37

Benzo(b)fluoranthene

Concen: 0.189 ng

RT: 22.772 min Scan# 2538

Delta R.T. 0.003 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:252 Resp: 2219

Ion Ratio Lower Upper

252 100

253 36.8 22.0 33.0#

125 24.2 13.7 20.5#



#38

Benzo(k)fluoranthene

Concen: 0.191 ng

RT: 22.813 min Scan# 2552

Delta R.T. -0.000 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:252 Resp: 2265


Ion Ratio Lower Upper

252 100

253 35.6 22.7 34.1#

125 21.8 12.5 18.7#





#39

Benzo(a)pyrene

Concen: 0.186 ng

RT: 23.339 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:252 Resp: 1815

Ion Ratio Lower Upper

252 100

253 42.2 25.8 38.6#

125 30.5 20.7 31.1



#40

Dibenzo(a,h)anthracene

Concen: 0.186 ng

RT: 25.678 min Scan# 3532

Delta R.T. 0.003 min

Lab File: BN036899.D

Acq: 14 Apr 2025 14:02




Tgt Ion:278 Resp: 1589


Ion Ratio Lower Upper

278 100

139 24.8 16.9 25.3

279 42.6 25.7 38.5#





#41

Benzo(g,h,i)perylene

Concen: 0.195 ng

RT: 26.336 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN036899.D


Acq: 14 Apr 2025 14:02

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:276 Resp: 1834

Ion Ratio Lower Upper

276 100

277 30.8 21.3 31.9

138 31.6 20.8 31.2#



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
 Data File : BN036900.D
 Acq On : 14 Apr 2025 14:38
 Operator : RC/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Apr 14 17:56:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 17:55:35 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	1387	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	3400	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	1899	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	3763	0.400	ng	0.00
29) Chrysene-d12	21.224	240	3219	0.400	ng	0.00
35) Perylene-d12	23.433	264	3042	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	1334	0.407	ng	0.00
5) Phenol-d6	6.809	99	1621	0.394	ng	0.00
8) Nitrobenzene-d5	8.781	82	1508	0.392	ng	0.00
11) 2-Methylnaphthalene-d10	12.011	152	2019	0.408	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	374	0.410	ng	0.00
15) 2-Fluorobiphenyl	12.904	172	3848	0.420	ng	0.00
27) Fluoranthene-d10	19.063	212	4276	0.430	ng	0.00
31) Terphenyl-d14	19.667	244	2909	0.413	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	693	0.437	ng	Qvalue 100
3) n-Nitrosodimethylamine	3.466	42	1564	0.427	ng	100
6) bis(2-Chloroethyl)ether	7.062	93	1593	0.399	ng	100
9) Naphthalene	10.468	128	4072	0.412	ng	100
10) Hexachlorobutadiene	10.757	225	974	0.429	ng	# 100
12) 2-Methylnaphthalene	12.087	142	2544	0.405	ng	100
16) Acenaphthylene	13.999	152	3612	0.401	ng	100
17) Acenaphthene	14.341	154	2417	0.407	ng	100
18) Fluorene	15.336	166	3173	0.405	ng	100
20) 4,6-Dinitro-2-methylph...	15.421	198	406	0.411	ng	100
21) 4-Bromophenyl-phenylether	16.227	248	1031	0.432	ng	100
22) Hexachlorobenzene	16.338	284	1166	0.436	ng	100
23) Atrazine	16.500	200	894	0.451	ng	100
24) Pentachlorophenol	16.686	266	600	0.420	ng	100
25) Phenanthrene	17.071	178	4960	0.430	ng	100
26) Anthracene	17.158	178	4394	0.423	ng	100
28) Fluoranthene	19.096	202	5775	0.426	ng	100
30) Pyrene	19.458	202	5880	0.406	ng	100
32) Benzo(a)anthracene	21.207	228	4716	0.404	ng	100
33) Chrysene	21.260	228	5277	0.418	ng	100
34) Bis(2-ethylhexyl)phtha...	21.144	149	2793	0.414	ng	100
36) Indeno(1,2,3-cd)pyrene	25.652	276	4638	0.421	ng	100
37) Benzo(b)fluoranthene	22.769	252	4978	0.423	ng	100
38) Benzo(k)fluoranthene	22.813	252	5110	0.430	ng	100
39) Benzo(a)pyrene	23.336	252	4174	0.425	ng	100
40) Dibenzo(a,h)anthracene	25.675	278	3598	0.420	ng	100
41) Benzo(g,h,i)perylene	26.336	276	4053	0.428	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036900.D
Acq On : 14 Apr 2025 14:38
Operator : RC/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Apr 14 17:56:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:55:35 2025
Response via : Initial Calibration




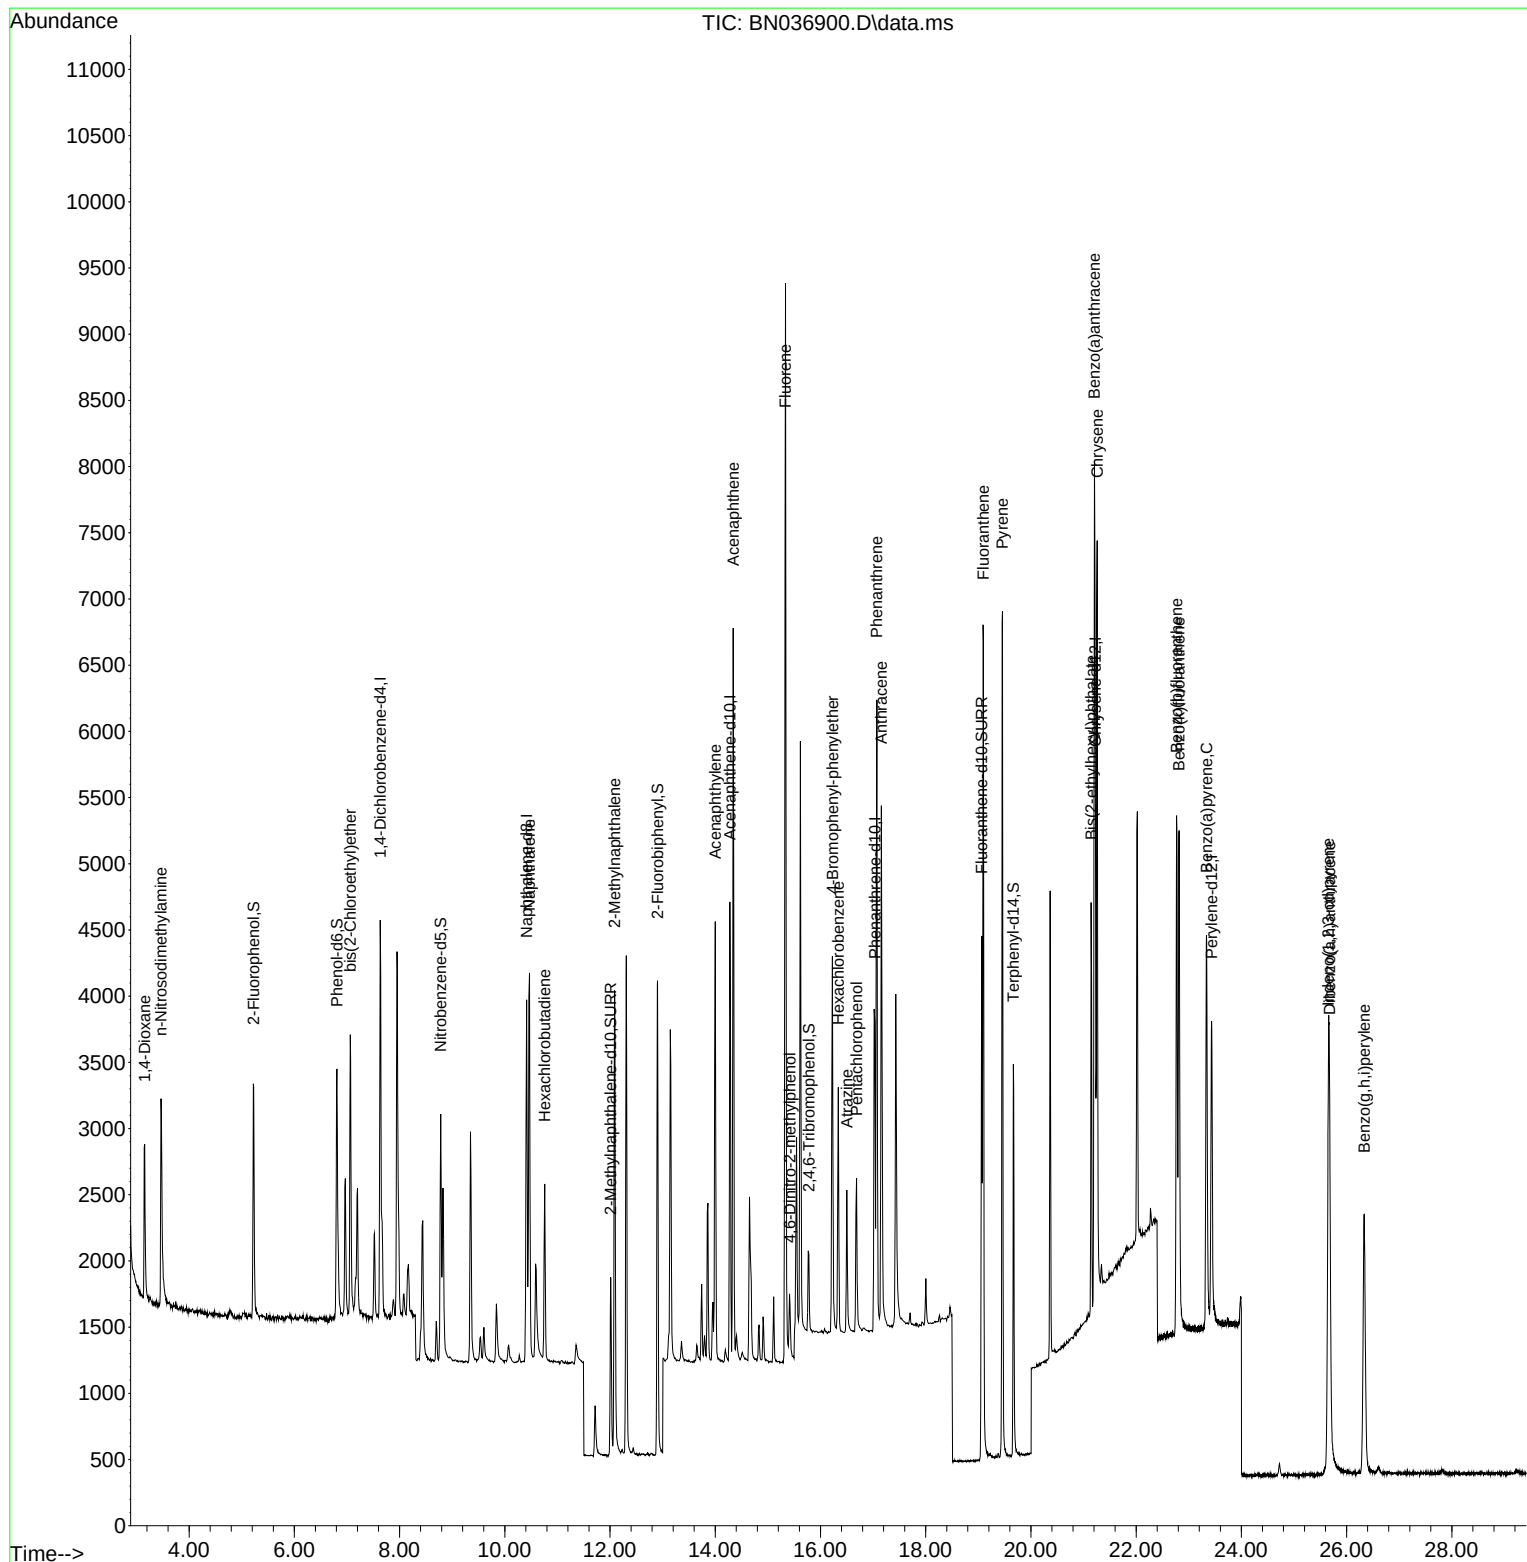




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 152 Resp: 1387
Ion Ratio Lower Upper
152 100
150 151.8 121.4 182.2
115 69.3 55.4 83.2



#2
1,4-Dioxane
Concen: 0.437 ng
RT: 3.155 min Scan# 38
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion: 88 Resp: 693
Ion Ratio Lower Upper
88 100
43 55.0 44.0 66.0
58 84.7 67.8 101.6









#3
n-Nitrosodimethylamine
Concen: 0.427 ng
RT: 3.466 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 42 Resp: 1564
Ion Ratio Lower Upper
42 100
74 65.4 52.3 78.5
44 9.3 7.4 11.2



#4
2-Fluorophenol
Concen: 0.407 ng
RT: 5.228 min Scan# 325
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion: 112 Resp: 1334
Ion Ratio Lower Upper
112 100
64 68.0 54.4 81.6
63 43.9 35.1 52.7









#5
Phenol-d6
Concen: 0.394 ng
RT: 6.809 min Scan# 544
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 99 Resp: 1621
Ion Ratio Lower Upper
99 100
42 38.2 30.6 45.8
71 47.5 38.0 57.0



#6
bis(2-Chloroethyl)ether
Concen: 0.399 ng
RT: 7.062 min Scan# 579
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion: 93 Resp: 1593
Ion Ratio Lower Upper
93 100
63 88.4 70.7 106.1
95 31.5 25.2 37.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	3400
Ion	Ratio	Lower	Upper
136	100		
137	13.2	10.6	15.8
54	13.3	10.6	16.0
68	7.6	6.1	9.1



#8
Nitrobenzene-d5
Concen: 0.392 ng
RT: 8.781 min Scan# 796
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion:	82	Resp:	1508
Ion	Ratio	Lower	Upper
82	100		
128	36.2	29.0	43.4
54	76.0	60.8	91.2









#9
Naphthalene
Concen: 0.412 ng
RT: 10.468 min Scan# 954
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	Ratio	Lower	Upper
128	100		
129	12.9	10.3	15.5
127	15.9	12.7	19.1



#10
Hexachlorobutadiene
Concen: 0.429 ng
RT: 10.757 min Scan# 981
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.7	51.0	76.4









#11
2-Methylnaphthalene-d10
Concen: 0.408 ng
RT: 12.011 min Scan# 1151
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 2019
Ion Ratio Lower Upper
152 100
151 21.4 17.1 25.7



#12
2-Methylnaphthalene
Concen: 0.405 ng
RT: 12.087 min Scan# 1166
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion:142 Resp: 2544
Ion Ratio Lower Upper
142 100
141 91.2 73.0 109.4
115 51.4 41.1 61.7









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.8	83.8	125.8
160	55.9	44.7	67.1



#14
2,4,6-Tribromophenol
Concen: 0.410 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.3	77.0	115.6
141	55.6	44.5	66.7





#15

2-Fluorobiphenyl

Concen: 0.420 ng

RT: 12.904 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:172 Resp: 3848

Ion Ratio Lower Upper

172 100

171 36.5 29.2 43.8

170 25.6 20.5 30.7



#16

Acenaphthylene

Concen: 0.401 ng

RT: 13.999 min Scan# 1440

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38




Tgt Ion:152 Resp: 3612


Ion Ratio Lower Upper

152 100

151 19.8 15.8 23.8

153 12.8 10.2 15.4


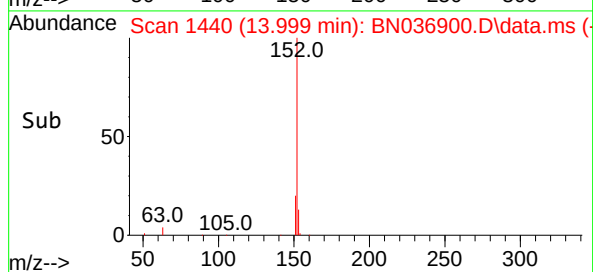






#17
Acenaphthene
Concen: 0.407 ng
RT: 14.341 min Scan# 1472
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 2417
Ion Ratio Lower Upper
154 100
153 118.4 94.7 142.1
152 61.8 49.4 74.2



#18
Fluorene
Concen: 0.405 ng
RT: 15.336 min Scan# 1565
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion:166 Resp: 3173
Ion Ratio Lower Upper
166 100
165 101.1 80.9 121.3
167 13.6 10.9 16.3





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:188 Resp: 3763

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 8.9 7.1 10.7



#20

4,6-Dinitro-2-methylphenol

Concen: 0.411 ng

RT: 15.421 min Scan# 1573

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38




Tgt Ion:198 Resp: 406


Ion Ratio Lower Upper

198 100

51 85.5 68.4 102.6

105 48.4 38.7 58.1









#21
4-Bromophenyl-phenylether
Concen: 0.432 ng
RT: 16.227 min Scan# 1639
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	Ratio	Lower	Upper
248	100		
250	96.3	77.0	115.6
141	78.7	63.0	94.4



#22
Hexachlorobenzene
Concen: 0.436 ng
RT: 16.338 min Scan# 1648
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion	Ratio	Lower	Upper
284	100		
142	53.3	42.6	64.0
249	36.4	29.1	43.7









#23
Atrazine
Concen: 0.451 ng
RT: 16.500 min Scan# 1661
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	Ratio	Lower	Upper
200	100		
173	31.2	25.0	37.4
215	46.5	37.2	55.8



#24
Pentachlorophenol
Concen: 0.420 ng
RT: 16.686 min Scan# 1676
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion	Ratio	Lower	Upper
266	100		
264	63.0	50.4	75.6
268	63.3	50.6	76.0









#25
Phenanthrene
Concen: 0.430 ng
RT: 17.071 min Scan# 1707
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 4960
Ion Ratio Lower Upper
178 100
176 20.2 16.2 24.2
179 15.3 12.2 18.4



#26
Anthracene
Concen: 0.423 ng
RT: 17.158 min Scan# 1714
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion:178 Resp: 4394
Ion Ratio Lower Upper
178 100
176 19.4 15.5 23.3
179 15.1 12.1 18.1





#27

Fluoranthene-d10

Concen: 0.430 ng

RT: 19.063 min Scan# 1942

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:212 Resp: 4276

Ion Ratio Lower Upper

212 100

106 13.2 10.6 15.8

104 8.3 6.6 10.0



#28

Fluoranthene

Concen: 0.426 ng

RT: 19.096 min Scan# 1949

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38




Tgt Ion:202 Resp: 5775


Ion Ratio Lower Upper

202 100

101 10.3 8.2 12.4

203 17.0 13.6 20.4





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:240 Resp: 3219

Ion Ratio Lower Upper

240 100

120 12.2 9.8 14.6

236 28.9 23.1 34.7

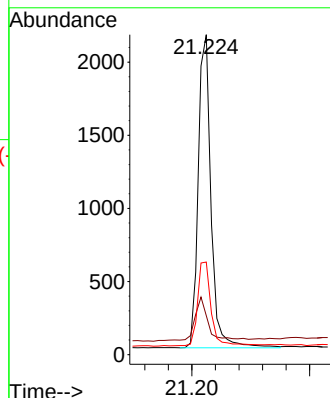

#30

Pyrene

Concen: 0.406 ng

RT: 19.458 min Scan# 2027

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38




Tgt Ion:202 Resp: 5880


Ion Ratio Lower Upper

202 100

200 21.3 17.0 25.6

203 17.6 14.1 21.1









#31
Terphenyl-d14
Concen: 0.413 ng
RT: 19.667 min Scan# 2072
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion	Ratio	Lower	Upper
244	100		
212	12.6	10.1	15.1
122	17.0	13.6	20.4



#32
Benzo(a)anthracene
Concen: 0.404 ng
RT: 21.207 min Scan# 2279
Delta R.T. 0.000 min
Lab File: BN036900.D
Acq: 14 Apr 2025 14:38

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.1	22.5	33.7
229	20.3	16.2	24.4





#33

Chrysene

Concen: 0.418 ng

RT: 21.260 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:228 Resp: 5277

Ion Ratio Lower Upper

228 100

226 31.1 24.9 37.3

229 19.9 15.9 23.9



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.414 ng

RT: 21.144 min Scan# 2272

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38




Tgt Ion:149 Resp: 2793


Ion Ratio Lower Upper

149 100

167 27.1 21.7 32.5

279 3.7 3.0 4.4





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.433 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:264 Resp: 3042

Ion Ratio Lower Upper

264 100

260 27.9 22.3 33.5

265 72.0 57.6 86.4



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.421 ng

RT: 25.652 min Scan# 3523

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38




Tgt Ion:276 Resp: 4638


Ion Ratio Lower Upper

276 100

138 25.4 20.3 30.5

277 25.4 20.3 30.5





#37

Benzo(b)fluoranthene

Concen: 0.423 ng

RT: 22.769 min Scan# 2537

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4




Tgt Ion:252 Resp: 4978

Ion Ratio Lower Upper

252 100

253 27.5 22.0 33.0

125 17.1 13.7 20.5



#38

Benzo(k)fluoranthene

Concen: 0.430 ng

RT: 22.813 min Scan# 2552

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38




Tgt Ion:252 Resp: 5110


Ion Ratio Lower Upper

252 100

253 28.4 22.7 34.1

125 15.6 12.5 18.7





#39

Benzo(a)pyrene

Concen: 0.425 ng

RT: 23.336 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:252 Resp: 4174

Ion Ratio Lower Upper

252 100

253 32.2 25.8 38.6

125 25.9 20.7 31.1



#40

Dibenzo(a,h)anthracene

Concen: 0.420 ng

RT: 25.675 min Scan# 3531

Delta R.T. 0.000 min

Lab File: BN036900.D

Acq: 14 Apr 2025 14:38




Tgt Ion:278 Resp: 3598


Ion Ratio Lower Upper

278 100

139 21.1 16.9 25.3

279 32.1 25.7 38.5





#41

Benzo(g,h,i)perylene

Concen: 0.428 ng

RT: 26.336 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN036900.D


Acq: 14 Apr 2025 14:38

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:276 Resp: 4053

Ion Ratio Lower Upper

276 100

277 26.6 21.3 31.9

138 26.0 20.8 31.2



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
 Data File : BN036901.D
 Acq On : 14 Apr 2025 15:15
 Operator : RC/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Apr 14 17:36:53 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 17:32:00 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	1469	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	3758	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	2072	0.400	ng	0.00
19) Phenanthrene-d10	17.021	188	4379	0.400	ng	#-0.01
29) Chrysene-d12	21.224	240	3653	0.400	ng	0.00
35) Perylene-d12	23.433	264	3591	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	2673	0.770	ng	0.00
5) Phenol-d6	6.809	99	3333	0.765	ng	0.00
8) Nitrobenzene-d5	8.781	82	3083	0.726	ng	0.00
11) 2-Methylnaphthalene-d10	12.011	152	4137	0.756	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	752	0.756	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	6934	0.693	ng	0.00
27) Fluoranthene-d10	19.063	212	8943	0.772	ng	0.00
31) Terphenyl-d14	19.667	244	6112	0.765	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	1350	0.787	ng	97
3) n-Nitrosodimethylamine	3.465	42	3096	0.798	ng	# 98
6) bis(2-Chloroethyl)ether	7.062	93	3254	0.770	ng	98
9) Naphthalene	10.468	128	8189	0.750	ng	97
10) Hexachlorobutadiene	10.756	225	1925	0.766	ng	# 99
12) 2-Methylnaphthalene	12.087	142	5251	0.756	ng	98
16) Acenaphthylene	13.999	152	7446	0.758	ng	99
17) Acenaphthene	14.341	154	4999	0.772	ng	98
18) Fluorene	15.336	166	6601	0.772	ng	100
20) 4,6-Dinitro-2-methylph...	15.421	198	894	0.749	ng	# 74
21) 4-Bromophenyl-phenylether	16.227	248	2124	0.766	ng	95
22) Hexachlorobenzene	16.338	284	2399	0.771	ng	98
23) Atrazine	16.500	200	1828	0.792	ng	96
24) Pentachlorophenol	16.686	266	1236	0.743	ng	98
25) Phenanthrene	17.071	178	10182	0.759	ng	100
26) Anthracene	17.157	178	9179	0.760	ng	99
28) Fluoranthene	19.096	202	12249	0.776	ng	100
30) Pyrene	19.458	202	12301	0.748	ng	99
32) Benzo(a)anthracene	21.206	228	10231	0.772	ng	99
33) Chrysene	21.260	228	11015	0.769	ng	100
34) Bis(2-ethylhexyl)phtha...	21.153	149	6003	0.785	ng	# 97
36) Indeno(1,2,3-cd)pyrene	25.652	276	10131	0.778	ng	98
37) Benzo(b)fluoranthene	22.769	252	10523	0.758	ng	# 93
38) Benzo(k)fluoranthene	22.813	252	10654	0.760	ng	93
39) Benzo(a)pyrene	23.336	252	8781	0.758	ng	# 86
40) Dibenzo(a,h)anthracene	25.666	278	7843	0.775	ng	93
41) Benzo(g,h,i)perylene	26.333	276	8625	0.772	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036901.D
Acq On : 14 Apr 2025 15:15
Operator : RC/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Apr 14 17:36:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:32:00 2025
Response via : Initial Calibration




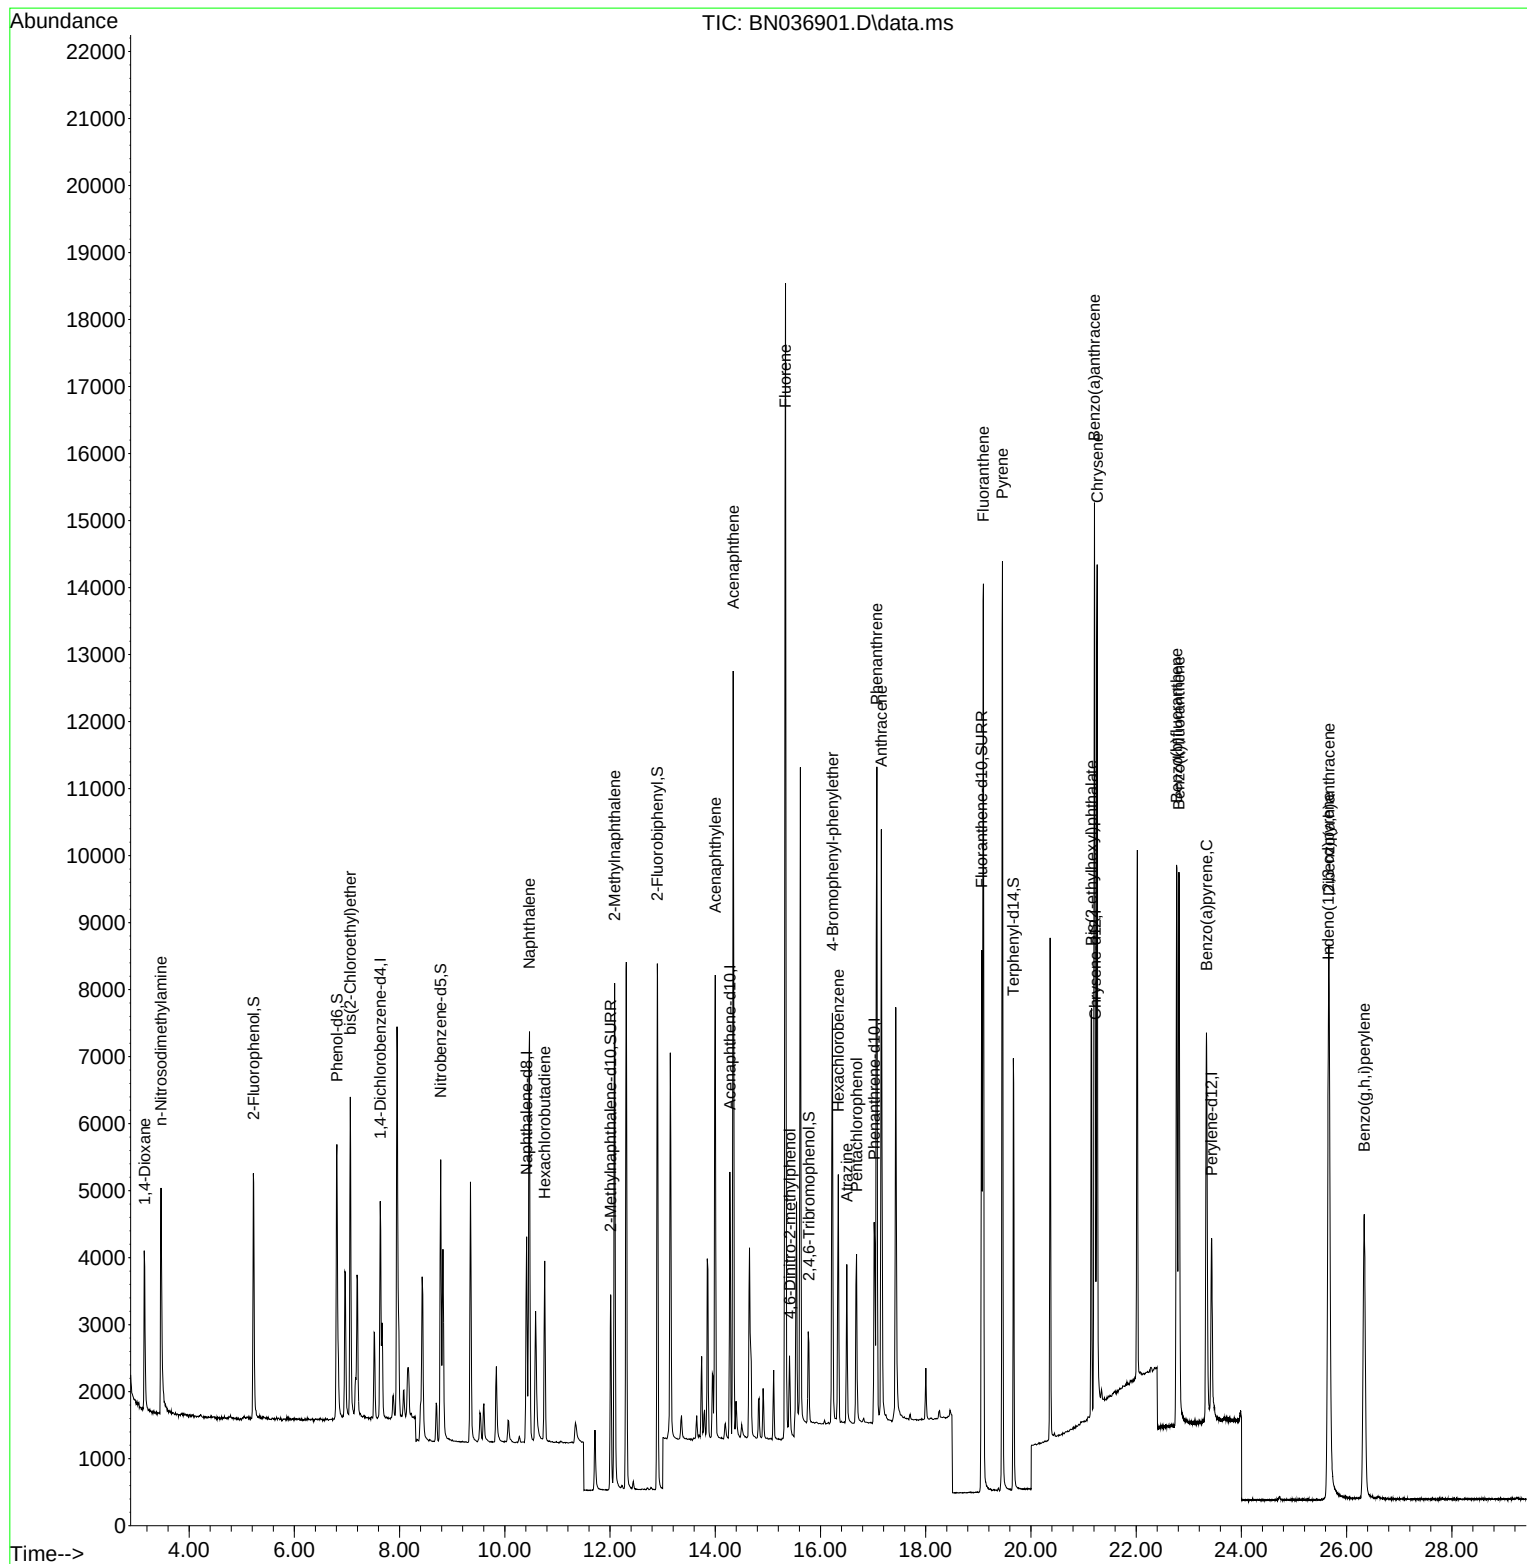




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 1469
Ion Ratio Lower Upper
152 100
150 154.2 121.4 182.2
115 70.3 55.4 83.2



#2
1,4-Dioxane
Concen: 0.787 ng
RT: 3.155 min Scan# 38
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion: 88 Resp: 1350
Ion Ratio Lower Upper
88 100
43 51.7 43.7 65.5
58 86.7 67.8 101.8









#3
n-Nitrosodimethylamine
Concen: 0.798 ng
RT: 3.465 min Scan# 81
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 42 Resp: 3096
Ion Ratio Lower Upper
42 100
74 64.3 52.3 78.5
44 7.1 7.4 11.2#



#4
2-Fluorophenol
Concen: 0.770 ng
RT: 5.228 min Scan# 325
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion: 112 Resp: 2673
Ion Ratio Lower Upper
112 100
64 69.4 54.4 81.6
63 45.2 35.1 52.7









#5
Phenol-d6
Concen: 0.765 ng
RT: 6.809 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	99	Resp:	3333
Ion	Ratio	Lower	Upper
99	100		
42	38.8	30.6	45.8
71	48.1	38.0	57.0



#6
bis(2-Chloroethyl)ether
Concen: 0.770 ng
RT: 7.062 min Scan# 579
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion:	93	Resp:	3254
Ion	Ratio	Lower	Upper
93	100		
63	86.4	70.7	106.1
95	31.5	25.2	37.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	136	Resp:	3758
Ion	Ratio	Lower	Upper
136	100		
137	12.4	10.6	15.8
54	12.8	10.6	16.0
68	6.9	6.1	9.1



#8
Nitrobenzene-d5
Concen: 0.726 ng
RT: 8.781 min Scan# 796
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion:	82	Resp:	3083
Ion	Ratio	Lower	Upper
82	100		
128	35.8	29.0	43.4
54	72.1	60.8	91.2





#9

Naphthalene

Concen: 0.750 ng

RT: 10.468 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:128 Resp: 8189

Ion Ratio Lower Upper

128 100

129 11.9 10.3 15.5

127 14.2 12.7 19.1



#10

Hexachlorobutadiene

Concen: 0.766 ng

RT: 10.756 min Scan# 981

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:225 Resp: 1925


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 64.3 51.0 76.4









#11
2-Methylnaphthalene-d10
Concen: 0.756 ng
RT: 12.011 min Scan# 1151
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 4137
Ion Ratio Lower Upper
152 100
151 22.0 17.1 25.7



#12
2-Methylnaphthalene
Concen: 0.756 ng
RT: 12.087 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion:142 Resp: 5251
Ion Ratio Lower Upper
142 100
141 90.0 73.0 109.4
115 49.9 41.1 61.7




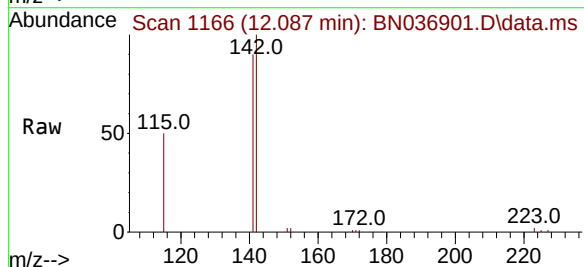




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion	Ratio	Lower	Upper
164	100		
162	107.9	83.8	125.8
160	57.2	44.7	67.1



#14
2,4,6-Tribromophenol
Concen: 0.756 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion	Ratio	Lower	Upper
330	100		
332	98.1	77.0	115.6
141	57.0	44.5	66.7









#15
2-Fluorobiphenyl
Concen: 0.693 ng
RT: 12.898 min Scan# 1326
Delta R.T. -0.005 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:172 Resp: 6934
Ion Ratio Lower Upper
172 100
171 36.6 29.2 43.8
170 25.0 20.5 30.7



#16
Acenaphthylene
Concen: 0.758 ng
RT: 13.999 min Scan# 1440
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion:152 Resp: 7446
Ion Ratio Lower Upper
152 100
151 20.0 15.8 23.8
153 13.3 10.2 15.4

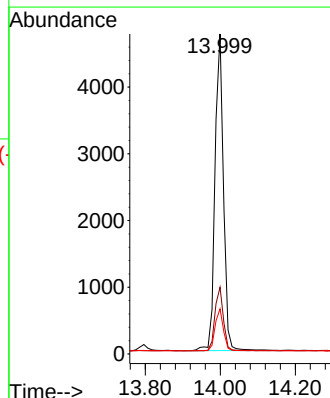



#17

Acenaphthene

Concen: 0.772 ng

RT: 14.341 min Scan# 1472

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:154 Resp: 4999

Ion Ratio Lower Upper

154 100

153 115.6 94.7 142.1

152 61.0 49.4 74.2



#18

Fluorene

Concen: 0.772 ng

RT: 15.336 min Scan# 1565

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:166 Resp: 6601


Ion Ratio Lower Upper

166 100

165 100.7 80.9 121.3

167 13.4 10.9 16.3

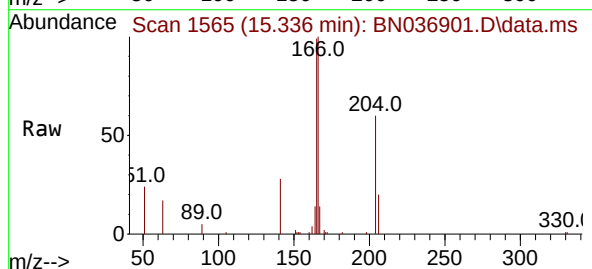



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.021 min Scan# 11

Delta R.T. -0.013 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:188 Resp: 4379

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 16.1 7.1 10.7#



#20

4,6-Dinitro-2-methylphenol

Concen: 0.749 ng

RT: 15.421 min Scan# 1573

Delta R.T. 0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:198 Resp: 894


Ion Ratio Lower Upper

198 100

51 60.5 68.4 102.6#

105 32.4 38.7 58.1#









#21
4-Bromophenyl-phenylether
Concen: 0.766 ng
RT: 16.227 min Scan# 1639
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion	Ratio	Lower	Upper
248	100		
250	98.9	77.0	115.6
141	72.0	63.0	94.4



#22
Hexachlorobenzene
Concen: 0.771 ng
RT: 16.338 min Scan# 1648
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion	Ratio	Lower	Upper
284	100		
142	51.1	42.6	64.0
249	35.6	29.1	43.7





#23

Atrazine

Concen: 0.792 ng

RT: 16.500 min Scan# 1661

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:200 Resp: 1828

Ion Ratio Lower Upper

200 100

173 28.0 25.0 37.4

215 45.1 37.2 55.8



#24

Pentachlorophenol

Concen: 0.743 ng

RT: 16.686 min Scan# 1676

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:266 Resp: 1236


Ion Ratio Lower Upper

266 100

264 63.1 50.8 76.2

268 65.5 50.6 76.0









#25
Phenanthrene
Concen: 0.759 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:178 Resp: 10182
Ion Ratio Lower Upper
178 100
176 20.2 16.2 24.2
179 15.4 12.2 18.4



#26
Anthracene
Concen: 0.760 ng
RT: 17.157 min Scan# 1714
Delta R.T. -0.000 min
Lab File: BN036901.D
Acq: 14 Apr 2025 15:15

Tgt Ion:178 Resp: 9179
Ion Ratio Lower Upper
178 100
176 19.0 15.4 23.0
179 15.3 11.9 17.9





#27

Fluoranthene-d10

Concen: 0.772 ng

RT: 19.063 min Scan# 1942

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:212 Resp: 8943

Ion Ratio Lower Upper

212 100

106 13.2 10.6 15.8

104 7.8 6.6 10.0



#28

Fluoranthene

Concen: 0.776 ng

RT: 19.096 min Scan# 1949

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:202 Resp: 12249


Ion Ratio Lower Upper

202 100

101 10.1 8.2 12.4

203 16.9 13.6 20.4





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:240 Resp: 3653

Ion Ratio Lower Upper

240 100

120 11.0 9.8 14.6

236 29.5 23.1 34.7



#30

Pyrene

Concen: 0.748 ng

RT: 19.458 min Scan# 2027

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:202 Resp: 12301


Ion Ratio Lower Upper

202 100

200 21.6 17.0 25.6

203 17.9 14.1 21.1





#31

Terphenyl-d14

Concen: 0.765 ng

RT: 19.667 min Scan# 2072

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:244 Resp: 6112

Ion Ratio Lower Upper

244 100

212 11.7 10.1 15.1

122 16.9 13.6 20.4



#32

Benzo(a)anthracene

Concen: 0.772 ng

RT: 21.206 min Scan# 2279

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:228 Resp: 10231


Ion Ratio Lower Upper

228 100

226 27.8 22.5 33.7

229 19.7 16.2 24.4

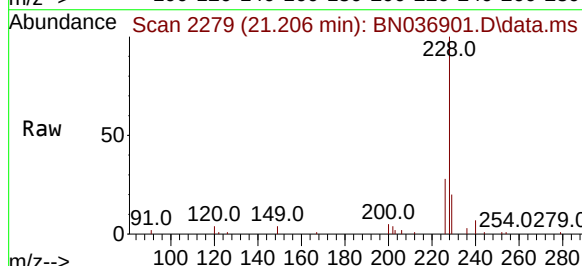



#33

Chrysene

Concen: 0.769 ng

RT: 21.260 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:228 Resp: 11015

Ion Ratio Lower Upper

228 100

226 31.2 24.9 37.3

229 20.2 15.9 23.9



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.785 ng

RT: 21.153 min Scan# 2273

Delta R.T. 0.009 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:149 Resp: 6003


Ion Ratio Lower Upper

149 100

167 25.8 21.8 32.6

279 2.9 3.0 4.4#





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.433 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036901.D


Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:264 Resp: 3591

Ion Ratio Lower Upper

264 100

260 26.0 22.3 33.5

265 64.6 57.6 86.4



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.778 ng

RT: 25.652 min Scan# 3523

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:276 Resp: 10131


Ion Ratio Lower Upper

276 100

138 26.7 20.3 30.5

277 24.9 20.3 30.5





#37

Benzo(b)fluoranthene

Concen: 0.758 ng

RT: 22.769 min Scan# 2537

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.8





Tgt Ion:252 Resp: 10523

Ion Ratio Lower Upper

252 100

253 24.3 22.0 33.0

125 13.5 13.7 20.5#



#38

Benzo(k)fluoranthene

Concen: 0.760 ng

RT: 22.813 min Scan# 2552

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:252 Resp: 10654


Ion Ratio Lower Upper

252 100

253 24.4 22.7 34.1

125 12.7 12.5 18.7





#39

Benzo(a)pyrene

Concen: 0.758 ng

RT: 23.336 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:252 Resp: 8781

Ion Ratio Lower Upper

252 100

253 26.0 25.8 38.6

125 17.3 20.7 31.1#



#40

Dibenzo(a,h)anthracene

Concen: 0.775 ng

RT: 25.666 min Scan# 3528

Delta R.T. -0.009 min

Lab File: BN036901.D

Acq: 14 Apr 2025 15:15




Tgt Ion:278 Resp: 7843


Ion Ratio Lower Upper

278 100

139 19.3 16.9 25.3

279 26.8 25.7 38.5





#41

Benzo(g,h,i)perylene

Concen: 0.772 ng

RT: 26.333 min Scan# 31

Delta R.T. -0.003 min

Lab File: BN036901.D


Acq: 14 Apr 2025 15:15

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:276 Resp: 8625

Ion Ratio Lower Upper

276 100

277 25.0 21.3 31.9

138 24.6 20.8 31.2



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
 Data File : BN036902.D
 Acq On : 14 Apr 2025 15:51
 Operator : RC/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Apr 14 17:37:26 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 17:32:00 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	1875	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	4741	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	2678	0.400	ng	0.00
19) Phenanthrene-d10	17.021	188	5516	0.400	ng	#-0.01
29) Chrysene-d12	21.224	240	4366	0.400	ng	0.00
35) Perylene-d12	23.433	264	3965	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	6900	1.557	ng	0.00
5) Phenol-d6	6.809	99	8666	1.558	ng	0.00
8) Nitrobenzene-d5	8.781	82	7932	1.480	ng	0.00
11) 2-Methylnaphthalene-d10	12.011	152	10598	1.535	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	2057	1.599	ng	0.00
15) 2-Fluorobiphenyl	12.899	172	20506	1.586	ng	0.00
27) Fluoranthene-d10	19.063	212	22814	1.564	ng	0.00
31) Terphenyl-d14	19.667	244	15252	1.597	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	3231	1.476	ng	97
3) n-Nitrosodimethylamine	3.465	42	7690	1.553	ng	# 98
6) bis(2-Chloroethyl)ether	7.062	93	8151	1.512	ng	100
9) Naphthalene	10.468	128	20671	1.500	ng	95
10) Hexachlorobutadiene	10.757	225	4843	1.528	ng	# 99
12) 2-Methylnaphthalene	12.087	142	13608	1.552	ng	97
16) Acenaphthylene	13.999	152	19849	1.563	ng	100
17) Acenaphthene	14.341	154	12915	1.543	ng	98
18) Fluorene	15.336	166	17393	1.574	ng	99
20) 4,6-Dinitro-2-methylph...	15.410	198	2369	1.576	ng	92
21) 4-Bromophenyl-phenylether	16.227	248	5510	1.577	ng	92
22) Hexachlorobenzene	16.338	284	5969	1.523	ng	99
23) Atrazine	16.500	200	4550	1.565	ng	94
24) Pentachlorophenol	16.686	266	3316	1.583	ng	99
25) Phenanthrene	17.071	178	26271	1.554	ng	99
26) Anthracene	17.157	178	23980	1.576	ng	100
28) Fluoranthene	19.096	202	31252	1.572	ng	100
30) Pyrene	19.458	202	31509	1.604	ng	100
32) Benzo(a)anthracene	21.206	228	25745	1.625	ng	99
33) Chrysene	21.260	228	26730	1.561	ng	99
34) Bis(2-ethylhexyl)phtha...	21.144	149	12891	1.411	ng	99
36) Indeno(1,2,3-cd)pyrene	25.658	276	22525	1.567	ng	98
37) Benzo(b)fluoranthene	22.769	252	24718	1.612	ng	# 90
38) Benzo(k)fluoranthene	22.813	252	24296	1.569	ng	# 90
39) Benzo(a)pyrene	23.336	252	20292	1.586	ng	# 82
40) Dibenzo(a,h)anthracene	25.669	278	17470	1.563	ng	# 90
41) Benzo(g,h,i)perylene	26.333	276	19061	1.545	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036902.D
Acq On : 14 Apr 2025 15:51
Operator : RC/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Apr 14 17:37:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:32:00 2025
Response via : Initial Calibration




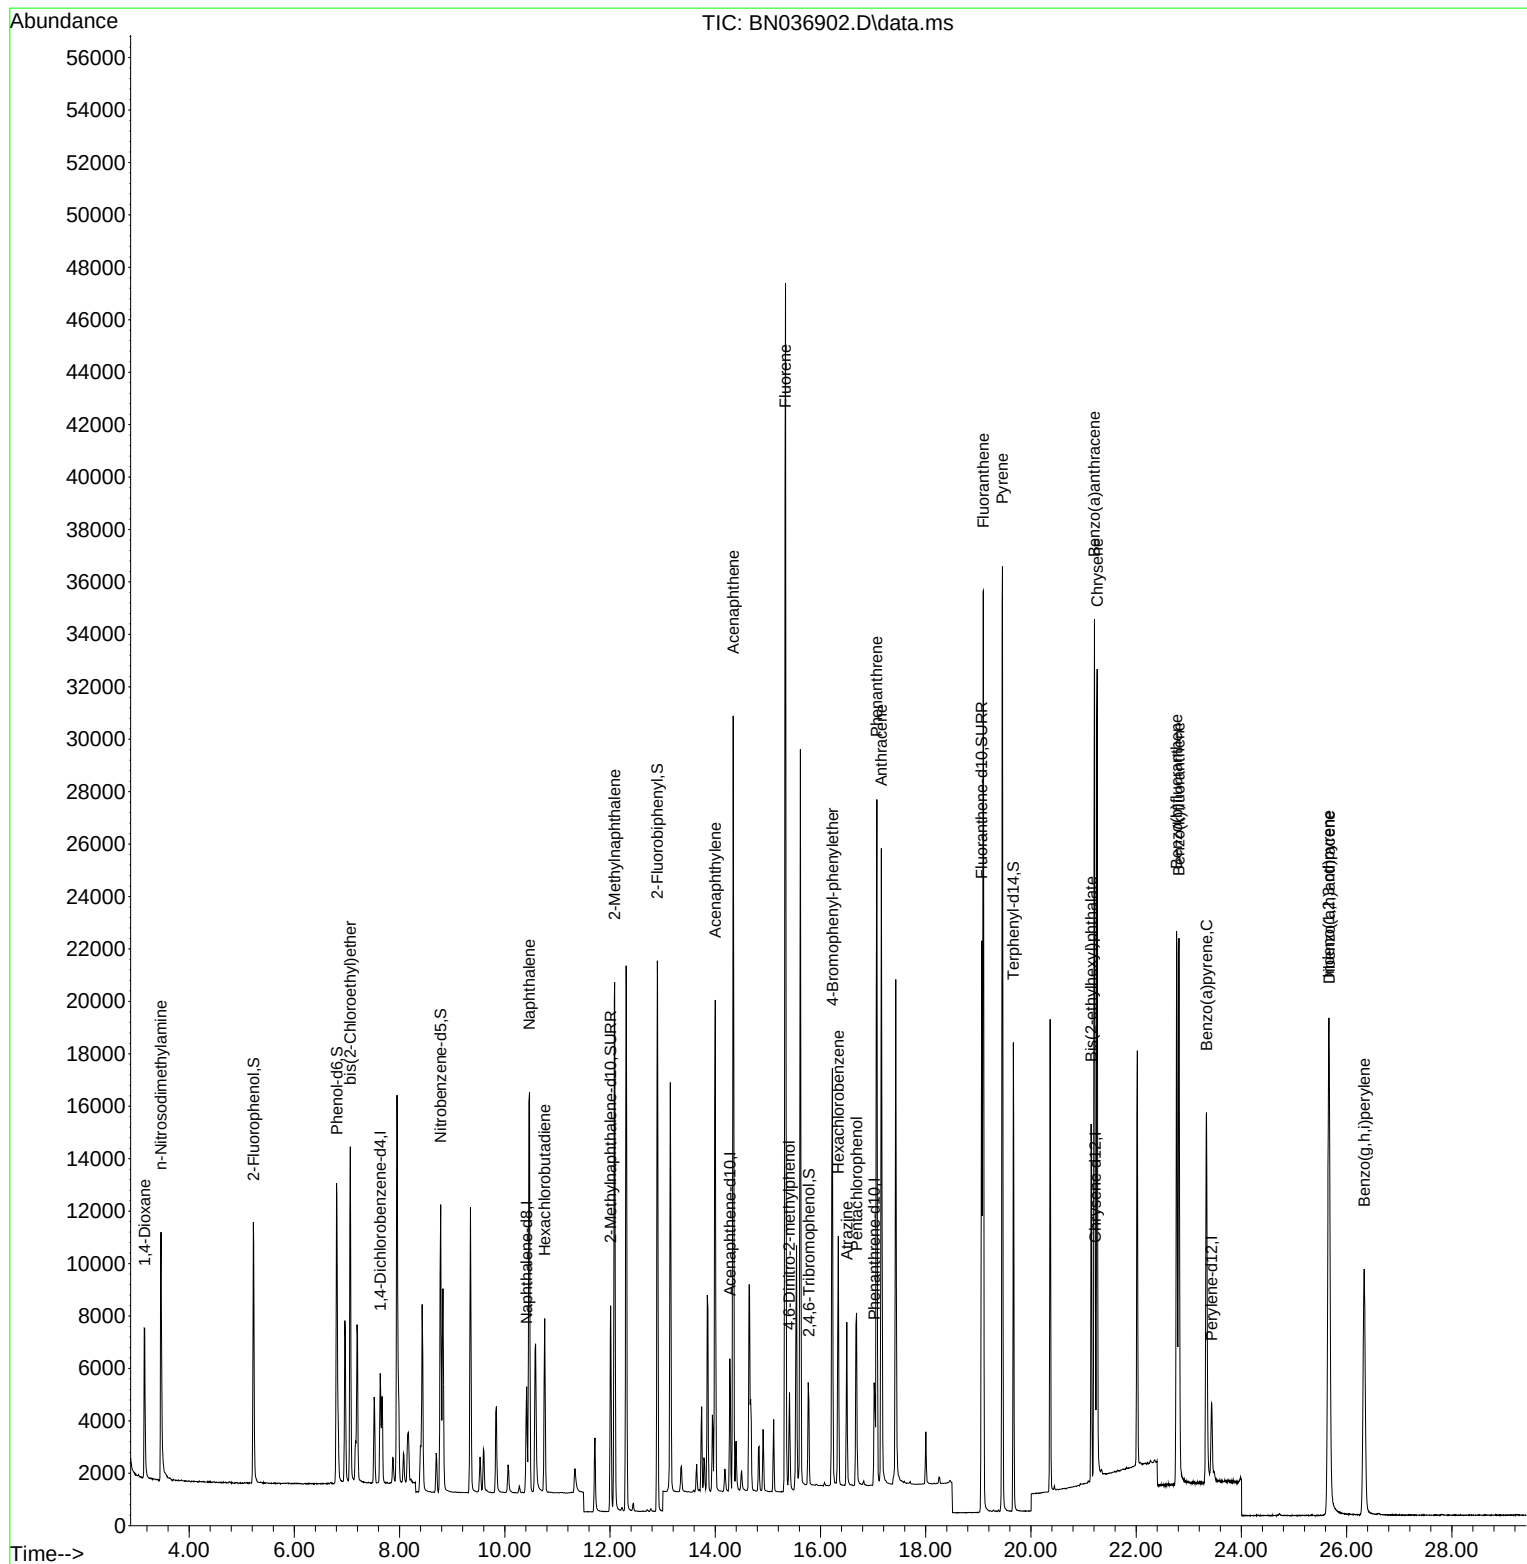




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 152 Resp: 1875
Ion Ratio Lower Upper
152 100
150 149.0 121.4 182.2
115 65.2 55.4 83.2



#2
1,4-Dioxane
Concen: 1.476 ng
RT: 3.155 min Scan# 38
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion: 88 Resp: 3231
Ion Ratio Lower Upper
88 100
43 52.3 43.7 65.5
58 87.6 67.8 101.8









#3
n-Nitrosodimethylamine
Concen: 1.553 ng
RT: 3.465 min Scan# 81
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 7690
Ion Ratio Lower Upper
42 100
74 65.2 52.3 78.5
44 4.8 7.4 11.2#



#4
2-Fluorophenol
Concen: 1.557 ng
RT: 5.228 min Scan# 325
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion: 112 Resp: 6900
Ion Ratio Lower Upper
112 100
64 68.8 54.4 81.6
63 44.2 35.1 52.7









#5
Phenol-d6
Concen: 1.558 ng
RT: 6.809 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion	Ratio	Lower	Upper
99	100		
42	39.0	30.6	45.8
71	48.3	38.0	57.0



#6
bis(2-Chloroethyl)ether
Concen: 1.512 ng
RT: 7.062 min Scan# 579
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion	Ratio	Lower	Upper
93	100		
63	88.2	70.7	106.1
95	32.1	25.2	37.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	4741
Ion	Ratio	Lower	Upper
136	100		
137	12.5	10.6	15.8
54	11.5	10.6	16.0
68	6.8	6.1	9.1



#8
Nitrobenzene-d5
Concen: 1.480 ng
RT: 8.781 min Scan# 796
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion:	82	Resp:	7932
Ion	Ratio	Lower	Upper
82	100		
128	36.1	29.0	43.4
54	69.0	60.8	91.2





#9

Naphthalene

Concen: 1.500 ng

RT: 10.468 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:128 Resp: 20671

Ion Ratio Lower Upper

128 100

129 11.4 10.3 15.5

127 13.4 12.7 19.1



#10

Hexachlorobutadiene

Concen: 1.528 ng

RT: 10.757 min Scan# 981

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:225 Resp: 4843


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 62.9 51.0 76.4




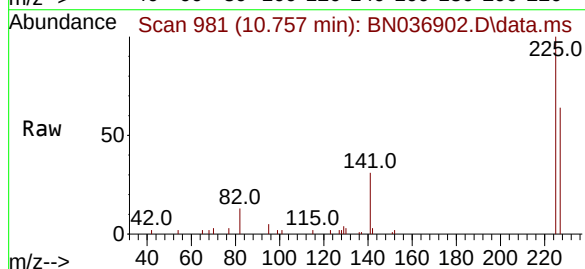




#11
2-Methylnaphthalene-d10
Concen: 1.535 ng
RT: 12.011 min Scan# 1151
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 10598
Ion Ratio Lower Upper
152 100
151 21.7 17.1 25.7



#12
2-Methylnaphthalene
Concen: 1.552 ng
RT: 12.087 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion:142 Resp: 13608
Ion Ratio Lower Upper
142 100
141 89.5 73.0 109.4
115 48.5 41.1 61.7









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.2	83.8	125.8
160	55.6	44.7	67.1



#14
2,4,6-Tribromophenol
Concen: 1.599 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion	Ratio	Lower	Upper
330	100		
332	94.7	77.0	115.6
141	57.4	44.5	66.7





#15

2-Fluorobiphenyl

Concen: 1.586 ng

RT: 12.899 min Scan# 11

Delta R.T. -0.005 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:172 Resp: 20506

Ion Ratio Lower Upper

172 100

171 36.2 29.2 43.8

170 25.0 20.5 30.7



#16

Acenaphthylene

Concen: 1.563 ng

RT: 13.999 min Scan# 1440

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:152 Resp: 19849


Ion Ratio Lower Upper

152 100

151 20.1 15.8 23.8

153 12.9 10.2 15.4





#17

Acenaphthene

Concen: 1.543 ng

RT: 14.341 min Scan# 1472

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:154 Resp: 12915

Ion Ratio Lower Upper

154 100

153 116.6 94.7 142.1

152 60.3 49.4 74.2



#18

Fluorene

Concen: 1.574 ng

RT: 15.336 min Scan# 1565

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:166 Resp: 17393


Ion Ratio Lower Upper

166 100

165 100.4 80.9 121.3

167 13.3 10.9 16.3





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.021 min Scan# 11

Delta R.T. -0.013 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:188 Resp: 5516

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 16.2 7.1 10.7#



#20

4,6-Dinitro-2-methylphenol

Concen: 1.576 ng

RT: 15.410 min Scan# 1572

Delta R.T. -0.011 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:198 Resp: 2369


Ion Ratio Lower Upper

198 100

51 75.7 68.4 102.6

105 51.0 38.7 58.1









#21
4-Bromophenyl-phenylether
Concen: 1.577 ng
RT: 16.227 min Scan# 1639
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 5510
Ion Ratio Lower Upper
248 100
250 97.9 77.0 115.6
141 64.1 63.0 94.4



#22
Hexachlorobenzene
Concen: 1.523 ng
RT: 16.338 min Scan# 1648
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion:284 Resp: 5969
Ion Ratio Lower Upper
284 100
142 52.7 42.6 64.0
249 36.2 29.1 43.7









#23
Atrazine
Concen: 1.565 ng
RT: 16.500 min Scan# 1661
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion	Ratio	Lower	Upper
200	100		
173	25.3	25.0	37.4
215	44.8	37.2	55.8



#24
Pentachlorophenol
Concen: 1.583 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.8	50.8	76.2
268	63.8	50.6	76.0









#25
Phenanthrene
Concen: 1.554 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 26271
Ion Ratio Lower Upper
178 100
176 19.6 16.2 24.2
179 15.2 12.2 18.4



#26
Anthracene
Concen: 1.576 ng
RT: 17.157 min Scan# 1714
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion:178 Resp: 23980
Ion Ratio Lower Upper
178 100
176 19.1 15.4 23.0
179 15.2 11.9 17.9





#27

Fluoranthene-d10

Concen: 1.564 ng

RT: 19.063 min Scan# 1942

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:212 Resp: 22814

Ion Ratio Lower Upper

212 100

106 13.3 10.6 15.8

104 8.2 6.6 10.0



#28

Fluoranthene

Concen: 1.572 ng

RT: 19.096 min Scan# 1949

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:202 Resp: 31252


Ion Ratio Lower Upper

202 100

101 10.4 8.2 12.4

203 17.1 13.6 20.4





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:240 Resp: 4366

Ion Ratio Lower Upper

240 100

120 10.4 9.8 14.6

236 29.3 23.1 34.7



#30

Pyrene

Concen: 1.604 ng

RT: 19.458 min Scan# 2027

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:202 Resp: 31509


Ion Ratio Lower Upper

202 100

200 21.6 17.0 25.6

203 17.7 14.1 21.1









#31
Terphenyl-d14
Concen: 1.597 ng
RT: 19.667 min Scan# 2072
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:244 Resp: 15252
Ion Ratio Lower Upper
244 100
212 11.3 10.1 15.1
122 16.1 13.6 20.4



#32
Benzo(a)anthracene
Concen: 1.625 ng
RT: 21.206 min Scan# 2279
Delta R.T. -0.000 min
Lab File: BN036902.D
Acq: 14 Apr 2025 15:51

Tgt Ion:228 Resp: 25745
Ion Ratio Lower Upper
228 100
226 27.7 22.5 33.7
229 19.5 16.2 24.4





#33

Chrysene

Concen: 1.561 ng

RT: 21.260 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:228 Resp: 26730

Ion Ratio Lower Upper

228 100

226 30.2 24.9 37.3

229 19.7 15.9 23.9



#34

Bis(2-ethylhexyl)phthalate

Concen: 1.411 ng

RT: 21.144 min Scan# 2272

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:149 Resp: 12891


Ion Ratio Lower Upper

149 100

167 26.5 21.8 32.6

279 3.1 3.0 4.4





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.433 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036902.D


Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:264 Resp: 3965

Ion Ratio Lower Upper

264 100

260 27.9 22.3 33.5

265 64.1 57.6 86.4



#36

Indeno(1,2,3-cd)pyrene


Concen: 1.567 ng

RT: 25.658 min Scan# 3525

Delta R.T. 0.006 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51





Tgt Ion:276 Resp: 22525


Ion Ratio Lower Upper

276 100

138 27.2 20.3 30.5

277 24.7 20.3 30.5





#37

Benzo(b)fluoranthene

Concen: 1.612 ng

RT: 22.769 min Scan# 2537

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6




Tgt Ion:252 Resp: 24718

Ion Ratio Lower Upper

252 100

253 22.6 22.0 33.0

125 11.8 13.7 20.5#



#38

Benzo(k)fluoranthene

Concen: 1.569 ng

RT: 22.813 min Scan# 2552

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:252 Resp: 24296


Ion Ratio Lower Upper

252 100

253 22.7 22.7 34.1#

125 11.8 12.5 18.7#





#39

Benzo(a)pyrene

Concen: 1.586 ng

RT: 23.336 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:252 Resp: 20292

Ion Ratio Lower Upper

252 100

253 23.8 25.8 38.6#

125 14.4 20.7 31.1#



#40

Dibenzo(a,h)anthracene

Concen: 1.563 ng

RT: 25.669 min Scan# 3529

Delta R.T. -0.006 min

Lab File: BN036902.D

Acq: 14 Apr 2025 15:51




Tgt Ion:278 Resp: 17470


Ion Ratio Lower Upper

278 100

139 19.3 16.9 25.3

279 24.5 25.7 38.5#





#41

Benzo(g,h,i)perylene

Concen: 1.545 ng

RT: 26.333 min Scan# 31

Delta R.T. -0.003 min

Lab File: BN036902.D


Acq: 14 Apr 2025 15:51

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:276 Resp: 19061

Ion Ratio Lower Upper

276 100

277 23.8 21.3 31.9

138 24.6 20.8 31.2



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
 Data File : BN036903.D
 Acq On : 14 Apr 2025 16:27
 Operator : RC/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Apr 14 17:37:59 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 17:32:00 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	1717	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	4325	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	2547	0.400	ng	0.00
19) Phenanthrene-d10	17.021	188	5334	0.400	ng	#-0.01
29) Chrysene-d12	21.224	240	4656	0.400	ng	0.00
35) Perylene-d12	23.436	264	4351	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	13953	3.439	ng	0.00
5) Phenol-d6	6.809	99	18091	3.552	ng	0.00
8) Nitrobenzene-d5	8.781	82	16162	3.305	ng	0.00
11) 2-Methylnaphthalene-d10	12.011	152	22172	3.519	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	4381	3.581	ng	0.00
15) 2-Fluorobiphenyl	12.899	172	41816	3.401	ng	0.00
27) Fluoranthene-d10	19.063	212	50558	3.583	ng	0.00
31) Terphenyl-d14	19.667	244	34219	3.359	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.148	88	6293	3.139	ng	97
3) n-Nitrosodimethylamine	3.458	42	14848	3.275	ng	# 98
6) bis(2-Chloroethyl)ether	7.062	93	16610	3.364	ng	100
9) Naphthalene	10.468	128	42047	3.345	ng	95
10) Hexachlorobutadiene	10.757	225	9465	3.273	ng	# 100
12) 2-Methylnaphthalene	12.087	142	28199	3.526	ng	98
16) Acenaphthylene	13.999	152	42600	3.526	ng	99
17) Acenaphthene	14.341	154	27469	3.450	ng	98
18) Fluorene	15.336	166	37322	3.552	ng	99
20) 4,6-Dinitro-2-methylph...	15.411	198	5526	3.801	ng	95
21) 4-Bromophenyl-phenylether	16.227	248	11646	3.446	ng	92
22) Hexachlorobenzene	16.338	284	12431	3.281	ng	99
23) Atrazine	16.500	200	9985	3.551	ng	# 92
24) Pentachlorophenol	16.686	266	7445	3.676	ng	100
25) Phenanthrene	17.071	178	56732	3.470	ng	99
26) Anthracene	17.158	178	53021	3.603	ng	99
28) Fluoranthene	19.096	202	69600	3.621	ng	99
30) Pyrene	19.458	202	70124	3.348	ng	100
32) Benzo(a)anthracene	21.207	228	60072	3.555	ng	99
33) Chrysene	21.260	228	62014	3.396	ng	99
34) Bis(2-ethylhexyl)phtha...	21.153	149	34748	3.565	ng	# 97
36) Indeno(1,2,3-cd)pyrene	25.655	276	57552	3.649	ng	96
37) Benzo(b)fluoranthene	22.772	252	59243	3.521	ng	# 89
38) Benzo(k)fluoranthene	22.816	252	59623	3.508	ng	# 89
39) Benzo(a)pyrene	23.336	252	49947	3.559	ng	# 79
40) Dibenzo(a,h)anthracene	25.669	278	44871	3.659	ng	# 90
41) Benzo(g,h,i)perylene	26.336	276	48224	3.563	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036903.D
Acq On : 14 Apr 2025 16:27
Operator : RC/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Apr 14 17:37:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:32:00 2025
Response via : Initial Calibration




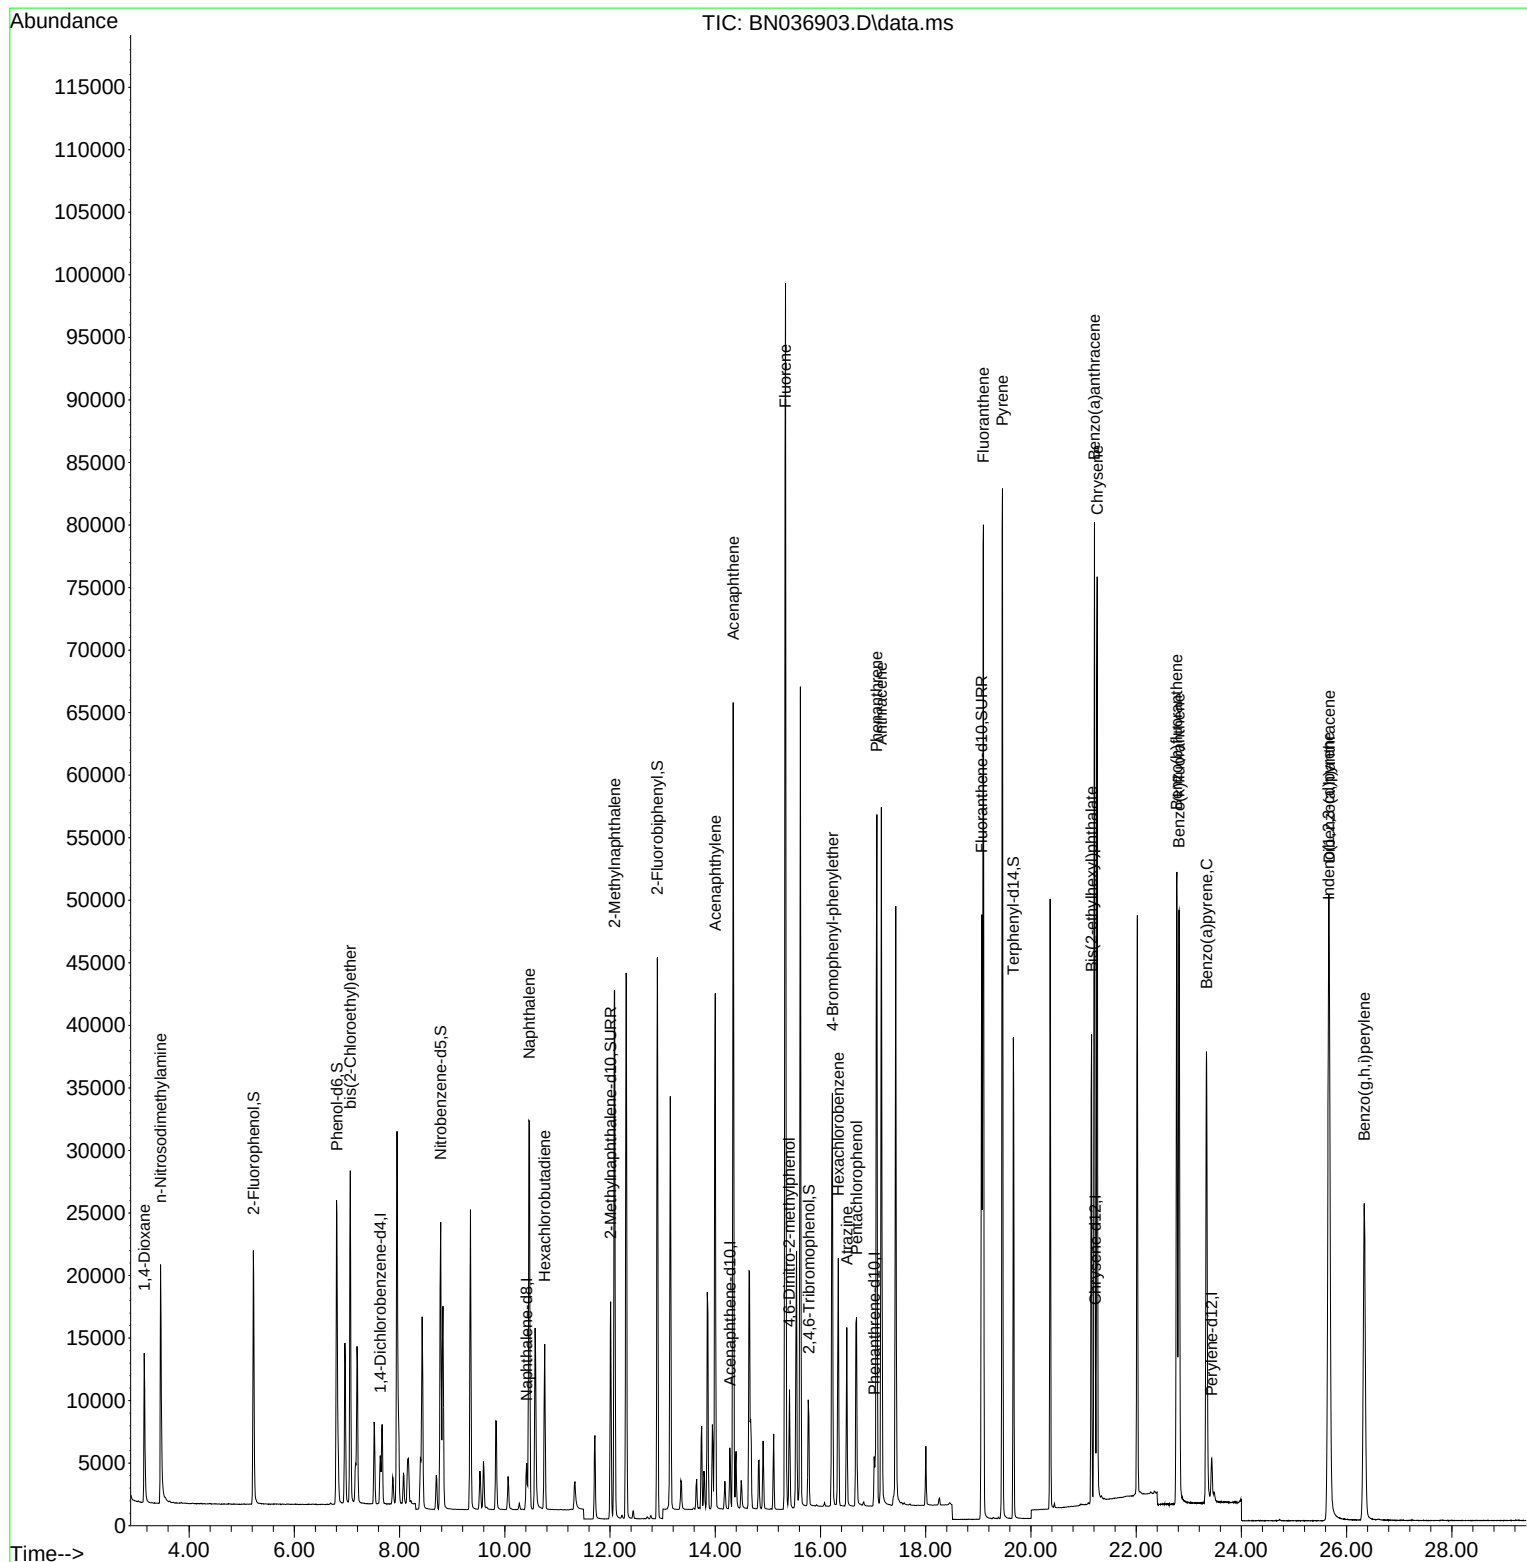




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 1717
Ion Ratio Lower Upper
152 100
150 152.1 121.4 182.2
115 69.9 55.4 83.2



#2
1,4-Dioxane
Concen: 3.139 ng
RT: 3.148 min Scan# 37
Delta R.T. -0.007 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion: 88 Resp: 6293
Ion Ratio Lower Upper
88 100
43 52.1 43.7 65.5
58 86.9 67.8 101.8









#3
n-Nitrosodimethylamine
Concen: 3.275 ng
RT: 3.458 min Scan# 80
Delta R.T. -0.007 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 42 Resp: 14848
Ion Ratio Lower Upper
42 100
74 64.6 52.3 78.5
44 5.3 7.4 11.2#



#4
2-Fluorophenol
Concen: 3.439 ng
RT: 5.228 min Scan# 325
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion: 112 Resp: 13953
Ion Ratio Lower Upper
112 100
64 69.2 54.4 81.6
63 43.6 35.1 52.7









#5
Phenol-d6
Concen: 3.552 ng
RT: 6.809 min Scan# 544
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 18091
Ion Ratio Lower Upper
99 100
42 38.2 30.6 45.8
71 47.5 38.0 57.0



#6
bis(2-Chloroethyl)ether
Concen: 3.364 ng
RT: 7.062 min Scan# 579
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion: 93 Resp: 16610
Ion Ratio Lower Upper
93 100
63 88.3 70.7 106.1
95 31.9 25.2 37.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	4325
Ion	Ratio	Lower	Upper
136	100		
137	12.6	10.6	15.8
54	12.3	10.6	16.0
68	6.8	6.1	9.1



#8
Nitrobenzene-d5
Concen: 3.305 ng
RT: 8.781 min Scan# 796
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion:	82	Resp:	16162
Ion	Ratio	Lower	Upper
82	100		
128	36.3	29.0	43.4
54	68.0	60.8	91.2





#9

Naphthalene

Concen: 3.345 ng

RT: 10.468 min Scan# 954

Delta R.T. 0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Instrument :





BNA_N

ClientSampleId :

SSTDICC3.2

Tgt Ion:128 Resp: 42047

Ion	Ratio	Lower	Upper
128	100		
129	11.1	10.3	15.5
127	13.4	12.7	19.1

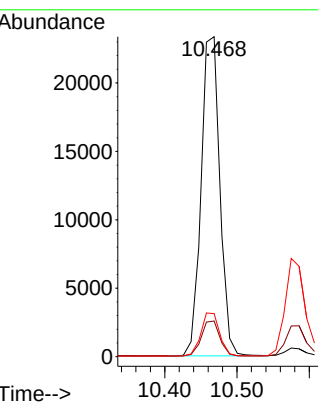

#10

Hexachlorobutadiene

Concen: 3.273 ng

RT: 10.757 min Scan# 981




Delta R.T. 0.000 min


Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Tgt Ion:225 Resp: 9465

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.8	51.0	76.4


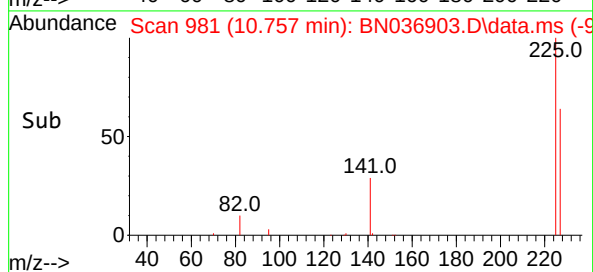

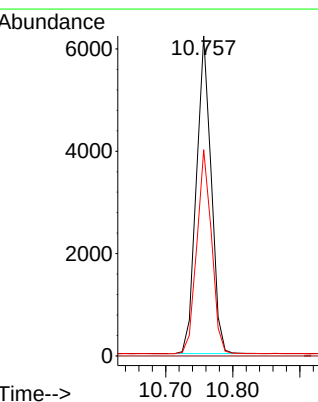




#11
2-Methylnaphthalene-d10
Concen: 3.519 ng
RT: 12.011 min Scan# 1151
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 22172
Ion Ratio Lower Upper
152 100
151 21.5 17.1 25.7



#12
2-Methylnaphthalene
Concen: 3.526 ng
RT: 12.087 min Scan# 1166
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion:142 Resp: 28199
Ion Ratio Lower Upper
142 100
141 90.1 73.0 109.4
115 48.0 41.1 61.7









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 2547
Ion Ratio Lower Upper
164 100
162 106.6 83.8 125.8
160 55.2 44.7 67.1



#14
2,4,6-Tribromophenol
Concen: 3.581 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion:330 Resp: 4381
Ion Ratio Lower Upper
330 100
332 95.9 77.0 115.6
141 61.5 44.5 66.7





#15

2-Fluorobiphenyl

Concen: 3.401 ng

RT: 12.899 min Scan# 11

Delta R.T. -0.005 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:172 Resp: 41816

Ion Ratio Lower Upper

172 100

171 36.3 29.2 43.8

170 24.4 20.5 30.7



#16

Acenaphthylene

Concen: 3.526 ng

RT: 13.999 min Scan# 1440

Delta R.T. 0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27




Tgt Ion:152 Resp: 42600


Ion Ratio Lower Upper

152 100

151 20.1 15.8 23.8

153 13.1 10.2 15.4





#17

Acenaphthene

Concen: 3.450 ng

RT: 14.341 min Scan# 1472

Delta R.T. 0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:154 Resp: 27469

Ion Ratio Lower Upper

154 100

153 116.2 94.7 142.1

152 60.1 49.4 74.2



#18

Fluorene

Concen: 3.552 ng

RT: 15.336 min Scan# 1565

Delta R.T. 0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27




Tgt Ion:166 Resp: 37322


Ion Ratio Lower Upper

166 100

165 100.3 80.9 121.3

167 13.4 10.9 16.3





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.021 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:188 Resp: 5334

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 16.1 7.1 10.7#



#20

4,6-Dinitro-2-methylphenol

Concen: 3.801 ng

RT: 15.411 min Scan# 1572

Delta R.T. -0.010 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27




Tgt Ion:198 Resp: 5526


Ion Ratio Lower Upper

198 100

51 84.3 68.4 102.6

105 56.8 38.7 58.1









#21
4-Bromophenyl-phenylether
Concen: 3.446 ng
RT: 16.227 min Scan# 1639
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion	Ratio	Lower	Upper
248	100		
250	96.9	77.0	115.6
141	64.3	63.0	94.4



#22
Hexachlorobenzene
Concen: 3.281 ng
RT: 16.338 min Scan# 1648
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion	Ratio	Lower	Upper
284	100		
142	52.4	42.6	64.0
249	35.9	29.1	43.7



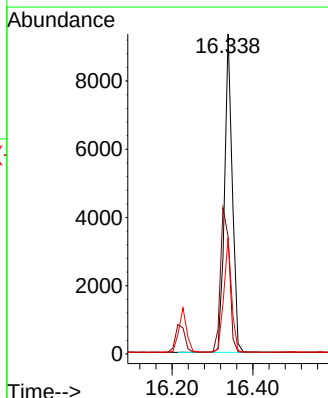





#23
Atrazine
Concen: 3.551 ng
RT: 16.500 min Scan# 1661
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion	Ratio	Lower	Upper
200	100		
173	24.4	25.0	37.4#
215	43.1	37.2	55.8



#24
Pentachlorophenol
Concen: 3.676 ng
RT: 16.686 min Scan# 1676
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion	Ratio	Lower	Upper
266	100		
264	63.5	50.8	76.2
268	63.2	50.6	76.0




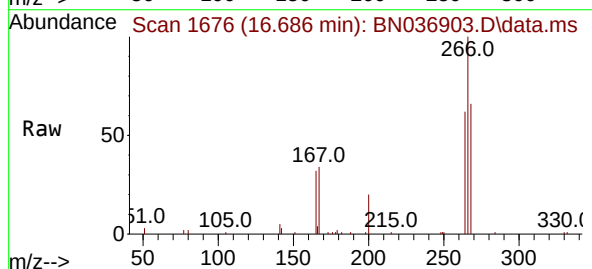




#25
Phenanthrene
Concen: 3.470 ng
RT: 17.071 min Scan# 1707
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:178 Resp: 56732
Ion Ratio Lower Upper
178 100
176 19.6 16.2 24.2
179 15.1 12.2 18.4



#26
Anthracene
Concen: 3.603 ng
RT: 17.158 min Scan# 1714
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion:178 Resp: 53021
Ion Ratio Lower Upper
178 100
176 19.0 15.4 23.0
179 15.2 11.9 17.9





#27

Fluoranthene-d10

Concen: 3.583 ng

RT: 19.063 min Scan# 1942

Delta R.T. 0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:212 Resp: 50558

Ion Ratio Lower Upper

212 100

106 13.6 10.6 15.8

104 8.3 6.6 10.0



#28

Fluoranthene

Concen: 3.621 ng

RT: 19.096 min Scan# 1949

Delta R.T. -0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27




Tgt Ion:202 Resp: 69600


Ion Ratio Lower Upper

202 100

101 10.6 8.2 12.4

203 17.2 13.6 20.4

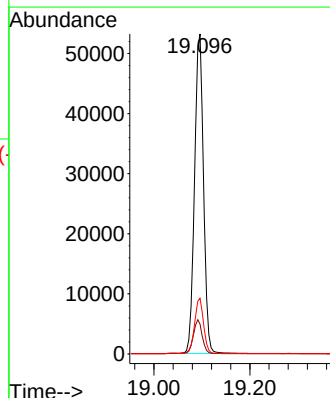



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:240 Resp: 4656

Ion Ratio Lower Upper

240 100

120 10.6 9.8 14.6

236 28.7 23.1 34.7



#30

Pyrene

Concen: 3.348 ng

RT: 19.458 min Scan# 2027

Delta R.T. 0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27




Tgt Ion:202 Resp: 70124


Ion Ratio Lower Upper

202 100

200 21.5 17.0 25.6

203 17.6 14.1 21.1









#31
Terphenyl-d14
Concen: 3.359 ng
RT: 19.667 min Scan# 2072
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion	Ratio	Lower	Upper
244	100		
212	11.0	10.1	15.1
122	16.5	13.6	20.4



#32
Benzo(a)anthracene
Concen: 3.555 ng
RT: 21.207 min Scan# 2279
Delta R.T. 0.000 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.0	22.5	33.7
229	19.4	16.2	24.4





#33

Chrysene

Concen: 3.396 ng

RT: 21.260 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:228 Resp: 62014

Ion Ratio Lower Upper

228 100

226 30.4 24.9 37.3

229 19.4 15.9 23.9



#34

Bis(2-ethylhexyl)phthalate

Concen: 3.565 ng

RT: 21.153 min Scan# 2273

Delta R.T. 0.009 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27




Tgt Ion:149 Resp: 34748


Ion Ratio Lower Upper

149 100

167 25.9 21.8 32.6

279 2.6 3.0 4.4#





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.436 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:264 Resp: 4351

Ion Ratio Lower Upper

264 100

260 27.1 22.3 33.5

265 64.2 57.6 86.4



#36

Indeno(1,2,3-cd)pyrene

Concen: 3.649 ng

RT: 25.655 min Scan# 3524

Delta R.T. 0.003 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27




Tgt Ion:276 Resp: 57552


Ion Ratio Lower Upper

276 100

138 29.0 20.3 30.5

277 25.0 20.3 30.5



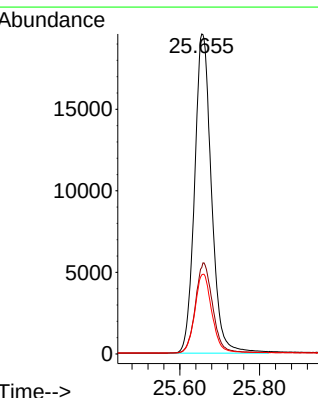





#37
Benzo(b)fluoranthene
Concen: 3.521 ng
RT: 22.772 min Scan# 2538
Delta R.T. 0.003 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 59243
Ion Ratio Lower Upper
252 100
253 22.0 22.0 33.0
125 11.7 13.7 20.5#



#38
Benzo(k)fluoranthene
Concen: 3.508 ng
RT: 22.816 min Scan# 2553
Delta R.T. 0.003 min
Lab File: BN036903.D
Acq: 14 Apr 2025 16:27

Tgt Ion:252 Resp: 59623
Ion Ratio Lower Upper
252 100
253 22.2 22.7 34.1#
125 11.7 12.5 18.7#





#39

Benzo(a)pyrene

Concen: 3.559 ng

RT: 23.336 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036903.D


Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:252 Resp: 49947

Ion Ratio Lower Upper

252 100

253 22.1 25.8 38.6#

125 13.3 20.7 31.1#



#40

Dibenzo(a,h)anthracene

Concen: 3.659 ng

RT: 25.669 min Scan# 3529

Delta R.T. -0.006 min

Lab File: BN036903.D

Acq: 14 Apr 2025 16:27




Tgt Ion:278 Resp: 44871


Ion Ratio Lower Upper

278 100

139 19.4 16.9 25.3

279 24.0 25.7 38.5#





#41

Benzo(g,h,i)perylene

Concen: 3.563 ng

RT: 26.336 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN036903.D


Acq: 14 Apr 2025 16:27

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:276 Resp: 48224

Ion Ratio Lower Upper

276 100

277 23.5 21.3 31.9

138 25.2 20.8 31.2



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
 Data File : BN036904.D
 Acq On : 14 Apr 2025 17:03
 Operator : RC/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 14 17:38:27 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 17:32:00 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	2526	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	6265	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	3616	0.400	ng	0.00
19) Phenanthrene-d10	17.021	188	7550	0.400	ng	#-0.01
29) Chrysene-d12	21.224	240	6382	0.400	ng	0.00
35) Perylene-d12	23.436	264	5326	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	29054	4.867	ng	0.00
5) Phenol-d6	6.809	99	37948	5.065	ng	0.00
8) Nitrobenzene-d5	8.781	82	33314	4.703	ng	0.00
11) 2-Methylnaphthalene-d10	12.011	152	45237	4.957	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	8793	5.062	ng	0.00
15) 2-Fluorobiphenyl	12.899	172	85634	4.906	ng	0.00
27) Fluoranthene-d10	19.063	212	101727	5.094	ng	0.00
31) Terphenyl-d14	19.667	244	68520	4.907	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.148	88	12754	4.325	ng	96
3) n-Nitrosodimethylamine	3.458	42	29084	4.361	ng	# 95
6) bis(2-Chloroethyl)ether	7.062	93	33742	4.646	ng	99
9) Naphthalene	10.468	128	85759	4.710	ng	94
10) Hexachlorobutadiene	10.757	225	18893	4.511	ng	# 100
12) 2-Methylnaphthalene	12.087	142	57358	4.951	ng	97
16) Acenaphthylene	13.999	152	87416	5.096	ng	100
17) Acenaphthene	14.341	154	56020	4.956	ng	97
18) Fluorene	15.336	166	74494	4.994	ng	99
20) 4,6-Dinitro-2-methylph...	15.410	198	11841	5.754	ng	92
21) 4-Bromophenyl-phenylether	16.227	248	23320	4.875	ng	# 90
22) Hexachlorobenzene	16.338	284	24901	4.643	ng	97
23) Atrazine	16.500	200	19423	4.880	ng	# 92
24) Pentachlorophenol	16.686	266	15597	5.441	ng	100
25) Phenanthrene	17.071	178	115620	4.996	ng	99
26) Anthracene	17.158	178	108061	5.188	ng	100
28) Fluoranthene	19.091	202	138759	5.101	ng	99
30) Pyrene	19.458	202	140457	4.892	ng	100
32) Benzo(a)anthracene	21.206	228	119518	5.160	ng	99
33) Chrysene	21.260	228	119027	4.756	ng	99
34) Bis(2-ethylhexyl)phtha...	21.153	149	65010	4.866	ng	# 97
36) Indeno(1,2,3-cd)pyrene	25.655	276	97485	5.050	ng	95
37) Benzo(b)fluoranthene	22.772	252	108304	5.258	ng	# 89
38) Benzo(k)fluoranthene	22.816	252	108417	5.211	ng	# 89
39) Benzo(a)pyrene	23.339	252	89751	5.224	ng	# 79
40) Dibenzo(a,h)anthracene	25.669	278	76444	5.092	ng	# 90
41) Benzo(g,h,i)perylene	26.333	276	80600	4.864	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036904.D
Acq On : 14 Apr 2025 17:03
Operator : RC/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 14 17:38:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:32:00 2025
Response via : Initial Calibration




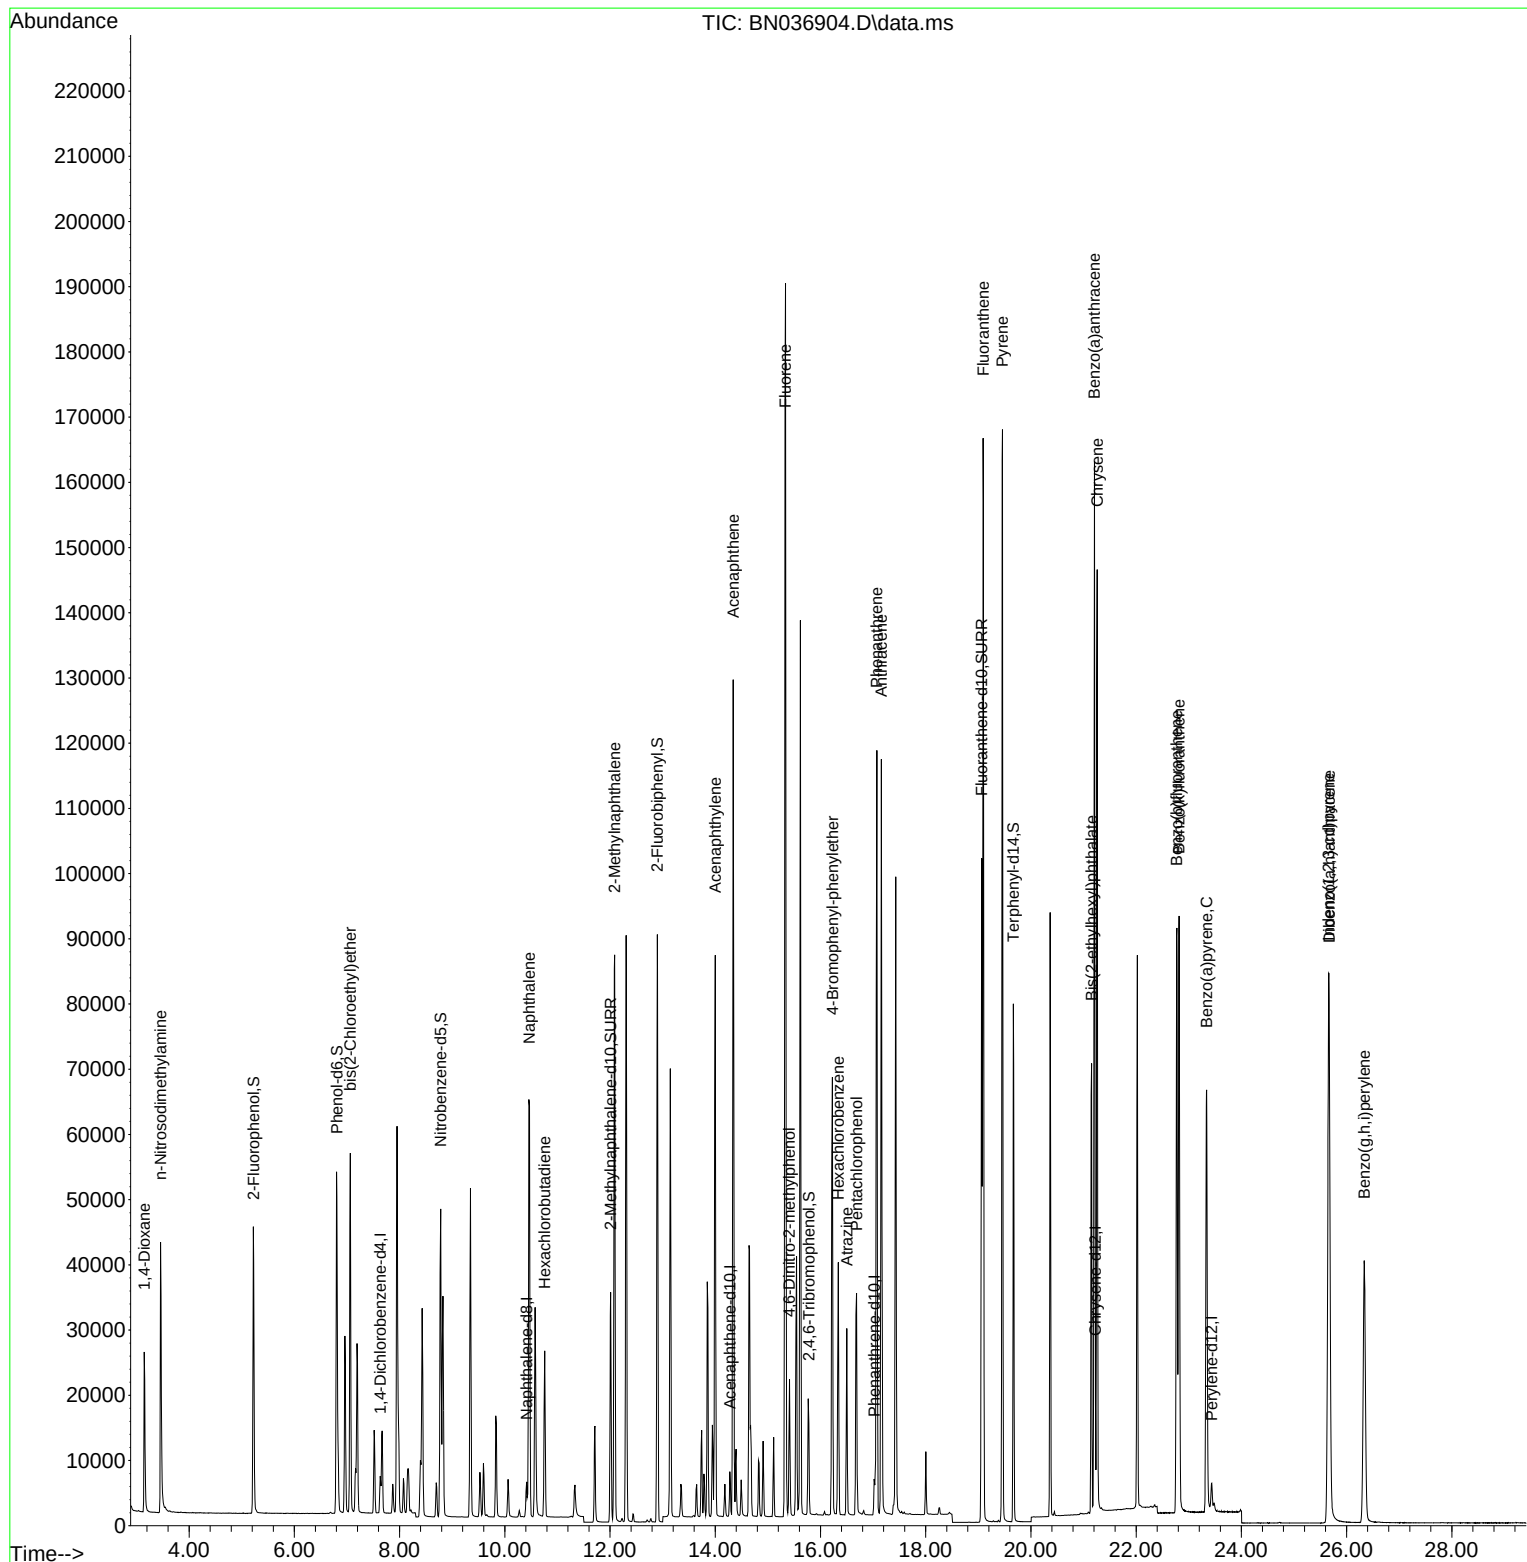




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 2526
Ion Ratio Lower Upper
152 100
150 154.2 121.4 182.2
115 67.9 55.4 83.2



#2
1,4-Dioxane
Concen: 4.325 ng
RT: 3.148 min Scan# 37
Delta R.T. -0.007 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion: 88 Resp: 12754
Ion Ratio Lower Upper
88 100
43 49.9 43.7 65.5
58 86.3 67.8 101.8









#3
n-Nitrosodimethylamine
Concen: 4.361 ng
RT: 3.458 min Scan# 80
Delta R.T. -0.007 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 29084
Ion Ratio Lower Upper
42 100
74 68.4 52.3 78.5
44 5.2 7.4 11.2#



#4
2-Fluorophenol
Concen: 4.867 ng
RT: 5.228 min Scan# 325
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion: 112 Resp: 29054
Ion Ratio Lower Upper
112 100
64 69.7 54.4 81.6
63 43.3 35.1 52.7









#5
Phenol-d6
Concen: 5.065 ng
RT: 6.809 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 37948
Ion Ratio Lower Upper
99 100
42 36.9 30.6 45.8
71 46.3 38.0 57.0



#6
bis(2-Chloroethyl)ether
Concen: 4.646 ng
RT: 7.062 min Scan# 579
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion: 93 Resp: 33742
Ion Ratio Lower Upper
93 100
63 87.9 70.7 106.1
95 32.0 25.2 37.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	6265
Ion	Ratio	Lower	Upper
136	100		
137	11.9	10.6	15.8
54	11.2	10.6	16.0
68	6.3	6.1	9.1



#8
Nitrobenzene-d5
Concen: 4.703 ng
RT: 8.781 min Scan# 796
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion:	82	Resp:	33314
Ion	Ratio	Lower	Upper
82	100		
128	36.7	29.0	43.4
54	64.4	60.8	91.2





#9

Naphthalene

Concen: 4.710 ng

RT: 10.468 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Instrument :





BNA_N

ClientSampleId :

SSTDICC5.0

Tgt Ion:128 Resp: 85759

Ion	Ratio	Lower	Upper
128	100		
129	10.9	10.3	15.5
127	13.3	12.7	19.1



#10

Hexachlorobutadiene

Concen: 4.511 ng

RT: 10.757 min Scan# 981




Delta R.T. -0.000 min


Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Tgt Ion:225 Resp: 18893

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.5	51.0	76.4









#11
2-Methylnaphthalene-d10
Concen: 4.957 ng
RT: 12.011 min Scan# 1151
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 45237
Ion Ratio Lower Upper
152 100
151 21.4 17.1 25.7



#12
2-Methylnaphthalene
Concen: 4.951 ng
RT: 12.087 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion:142 Resp: 57358
Ion Ratio Lower Upper
142 100
141 90.2 73.0 109.4
115 46.5 41.1 61.7









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	164	Resp:	3616
Ion	Ratio	Lower	Upper
164	100		
162	108.7	83.8	125.8
160	54.8	44.7	67.1



#14
2,4,6-Tribromophenol
Concen: 5.062 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion	330	Resp:	8793
Ion	Ratio	Lower	Upper
330	100		
332	96.1	77.0	115.6
141	62.4	44.5	66.7





#15

2-Fluorobiphenyl

Concen: 4.906 ng

RT: 12.899 min Scan# 11

Delta R.T. -0.005 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:172 Resp: 85634

Ion Ratio Lower Upper

172 100

171 35.7 29.2 43.8

170 24.3 20.5 30.7



#16

Acenaphthylene

Concen: 5.096 ng

RT: 13.999 min Scan# 1440

Delta R.T. -0.000 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03




Tgt Ion:152 Resp: 87416


Ion Ratio Lower Upper

152 100

151 20.1 15.8 23.8

153 12.9 10.2 15.4









#17
Acenaphthene
Concen: 4.956 ng
RT: 14.341 min Scan# 1472
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 56020
Ion Ratio Lower Upper
154 100
153 115.5 94.7 142.1
152 58.2 49.4 74.2



#18
Fluorene
Concen: 4.994 ng
RT: 15.336 min Scan# 1565
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion:166 Resp: 74494
Ion Ratio Lower Upper
166 100
165 99.8 80.9 121.3
167 13.4 10.9 16.3





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.021 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:188 Resp: 7550

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 16.7 7.1 10.7#



#20

4,6-Dinitro-2-methylphenol

Concen: 5.754 ng

RT: 15.410 min Scan# 1572

Delta R.T. -0.011 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03




Tgt Ion:198 Resp: 11841


Ion Ratio Lower Upper

198 100

51 79.7 68.4 102.6

105 55.6 38.7 58.1









#21
4-Bromophenyl-phenylether
Concen: 4.875 ng
RT: 16.227 min Scan# 1639
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 23320
Ion Ratio Lower Upper
248 100
250 97.0 77.0 115.6
141 59.3 63.0 94.4#



#22
Hexachlorobenzene
Concen: 4.643 ng
RT: 16.338 min Scan# 1648
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion:284 Resp: 24901
Ion Ratio Lower Upper
284 100
142 50.1 42.6 64.0
249 35.7 29.1 43.7









#23
Atrazine
Concen: 4.880 ng
RT: 16.500 min Scan# 1661
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:200 Resp: 19423
Ion Ratio Lower Upper
200 100
173 24.9 25.0 37.4#
215 42.8 37.2 55.8



#24
Pentachlorophenol
Concen: 5.441 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion:266 Resp: 15597
Ion Ratio Lower Upper
266 100
264 63.0 50.8 76.2
268 63.4 50.6 76.0









#25
Phenanthrene
Concen: 4.996 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 115620
Ion Ratio Lower Upper
178 100
176 19.7 16.2 24.2
179 15.1 12.2 18.4



#26
Anthracene
Concen: 5.188 ng
RT: 17.158 min Scan# 1714
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion:178 Resp: 108061
Ion Ratio Lower Upper
178 100
176 19.0 15.4 23.0
179 15.1 11.9 17.9





#27

Fluoranthene-d10

Concen: 5.094 ng

RT: 19.063 min Scan# 1942

Delta R.T. -0.000 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:212 Resp: 101727

Ion Ratio Lower Upper

212 100

106 14.4 10.6 15.8

104 8.7 6.6 10.0



#28

Fluoranthene

Concen: 5.101 ng

RT: 19.091 min Scan# 1948

Delta R.T. -0.005 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03




Tgt Ion:202 Resp: 138759


Ion Ratio Lower Upper

202 100

101 11.2 8.2 12.4

203 17.3 13.6 20.4





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:240 Resp: 6382

Ion Ratio Lower Upper

240 100

120 10.2 9.8 14.6

236 28.8 23.1 34.7



#30

Pyrene

Concen: 4.892 ng

RT: 19.458 min Scan# 2027

Delta R.T. -0.000 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03




Tgt Ion:202 Resp: 140457


Ion Ratio Lower Upper

202 100

200 21.5 17.0 25.6

203 17.6 14.1 21.1









#31
Terphenyl-d14
Concen: 4.907 ng
RT: 19.667 min Scan# 2072
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:244 Resp: 68520
Ion Ratio Lower Upper
244 100
212 10.8 10.1 15.1
122 16.5 13.6 20.4



#32
Benzo(a)anthracene
Concen: 5.160 ng
RT: 21.206 min Scan# 2279
Delta R.T. -0.000 min
Lab File: BN036904.D
Acq: 14 Apr 2025 17:03

Tgt Ion:228 Resp: 119518
Ion Ratio Lower Upper
228 100
226 27.9 22.5 33.7
229 19.4 16.2 24.4





#33

Chrysene

Concen: 4.756 ng

RT: 21.260 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 119027

Ion Ratio Lower Upper

228 100

226 30.3 24.9 37.3

229 19.8 15.9 23.9



#34

Bis(2-ethylhexyl)phthalate

Concen: 4.866 ng

RT: 21.153 min Scan# 2273

Delta R.T. 0.009 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03




Tgt Ion:149 Resp: 65010


Ion Ratio Lower Upper

149 100

167 25.7 21.8 32.6

279 2.6 3.0 4.4#





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.436 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN036904.D


Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0






Tgt Ion:264 Resp: 5326

Ion Ratio Lower Upper

264 100

260 27.0 22.3 33.5

265 60.5 57.6 86.4



#36

Indeno(1,2,3-cd)pyrene

Concen: 5.050 ng

RT: 25.655 min Scan# 3524

Delta R.T. 0.003 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03




Tgt Ion:276 Resp: 97485


Ion Ratio Lower Upper

276 100

138 30.3 20.3 30.5

277 25.0 20.3 30.5





#37

Benzo(b)fluoranthene

Concen: 5.258 ng

RT: 22.772 min Scan# 2537

Delta R.T. 0.003 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 108304

Ion Ratio Lower Upper

252 100

253 21.8 22.0 33.0#

125 12.1 13.7 20.5#



#38

Benzo(k)fluoranthene

Concen: 5.211 ng

RT: 22.816 min Scan# 2553

Delta R.T. 0.003 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03




Tgt Ion:252 Resp: 108417


Ion Ratio Lower Upper

252 100

253 21.8 22.7 34.1#

125 11.8 12.5 18.7#





#39

Benzo(a)pyrene

Concen: 5.224 ng

RT: 23.339 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 89751

Ion Ratio Lower Upper

252 100

253 22.0 25.8 38.6#

125 13.6 20.7 31.1#



#40

Dibenzo(a,h)anthracene

Concen: 5.092 ng

RT: 25.669 min Scan# 3529

Delta R.T. -0.006 min

Lab File: BN036904.D

Acq: 14 Apr 2025 17:03




Tgt Ion:278 Resp: 76444


Ion Ratio Lower Upper

278 100

139 19.8 16.9 25.3

279 23.5 25.7 38.5#





#41

Benzo(g,h,i)perylene

Concen: 4.864 ng

RT: 26.333 min Scan# 31

Delta R.T. -0.003 min

Lab File: BN036904.D


Acq: 14 Apr 2025 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:276 Resp: 80600

Ion Ratio Lower Upper

276 100

277 23.6 21.3 31.9

138 25.9 20.8 31.2



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
 Data File : BN036905.D
 Acq On : 14 Apr 2025 17:39
 Operator : RC/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN041425

Quant Time: Apr 14 18:01:54 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 17:58:02 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	2284	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	5795	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	3208	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	6273	0.400	ng	0.00
29) Chrysene-d12	21.224	240	5203	0.400	ng	0.00
35) Perylene-d12	23.436	264	4681	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	2109	0.391	ng	0.00
5) Phenol-d6	6.809	99	2518	0.372	ng	0.00
8) Nitrobenzene-d5	8.781	82	2553	0.390	ng	0.00
11) 2-Methylnaphthalene-d10	12.011	152	3366	0.399	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	510	0.331	ng	0.00
15) 2-Fluorobiphenyl	12.899	172	6990	0.451	ng	0.00
27) Fluoranthene-d10	19.063	212	6761	0.407	ng	0.00
31) Terphenyl-d14	19.672	244	5020	0.441	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	1219	0.467	ng	97
3) n-Nitrosodimethylamine	3.465	42	2281	0.378	ng	91
6) bis(2-Chloroethyl)ether	7.062	93	2742	0.418	ng	99
9) Naphthalene	10.468	128	6854	0.407	ng	96
10) Hexachlorobutadiene	10.757	225	1591	0.411	ng	# 98
12) 2-Methylnaphthalene	12.087	142	4031	0.376	ng	96
16) Acenaphthylene	13.999	152	6788	0.446	ng	99
17) Acenaphthene	14.341	154	4084	0.407	ng	99
18) Fluorene	15.336	166	5392	0.407	ng	100
20) 4,6-Dinitro-2-methylph...	15.421	198	621	0.363	ng	97
21) 4-Bromophenyl-phenylether	16.227	248	1688	0.425	ng	98
22) Hexachlorobenzene	16.338	284	1899	0.426	ng	98
23) Atrazine	16.500	200	1508	0.456	ng	99
24) Pentachlorophenol	16.686	266	853	0.358	ng	99
25) Phenanthrene	17.071	178	8446	0.439	ng	99
26) Anthracene	17.157	178	7704	0.445	ng	99
28) Fluoranthene	19.096	202	9368	0.414	ng	99
30) Pyrene	19.458	202	9483	0.405	ng	99
32) Benzo(a)anthracene	21.206	228	8028	0.425	ng	99
33) Chrysene	21.260	228	8745	0.429	ng	100
34) Bis(2-ethylhexyl)phtha...	21.144	149	4585	0.421	ng	# 99
36) Indeno(1,2,3-cd)pyrene	25.661	276	7286	0.429	ng	98
37) Benzo(b)fluoranthene	22.772	252	7575	0.418	ng	98
38) Benzo(k)fluoranthene	22.816	252	8145	0.445	ng	97
39) Benzo(a)pyrene	23.339	252	6835	0.453	ng	# 92
40) Dibenzo(a,h)anthracene	25.669	278	5596	0.424	ng	96
41) Benzo(g,h,i)perylene	26.336	276	5939	0.408	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036905.D
Acq On : 14 Apr 2025 17:39
Operator : RC/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN041425

Quant Time: Apr 14 18:01:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:58:02 2025
Response via : Initial Calibration




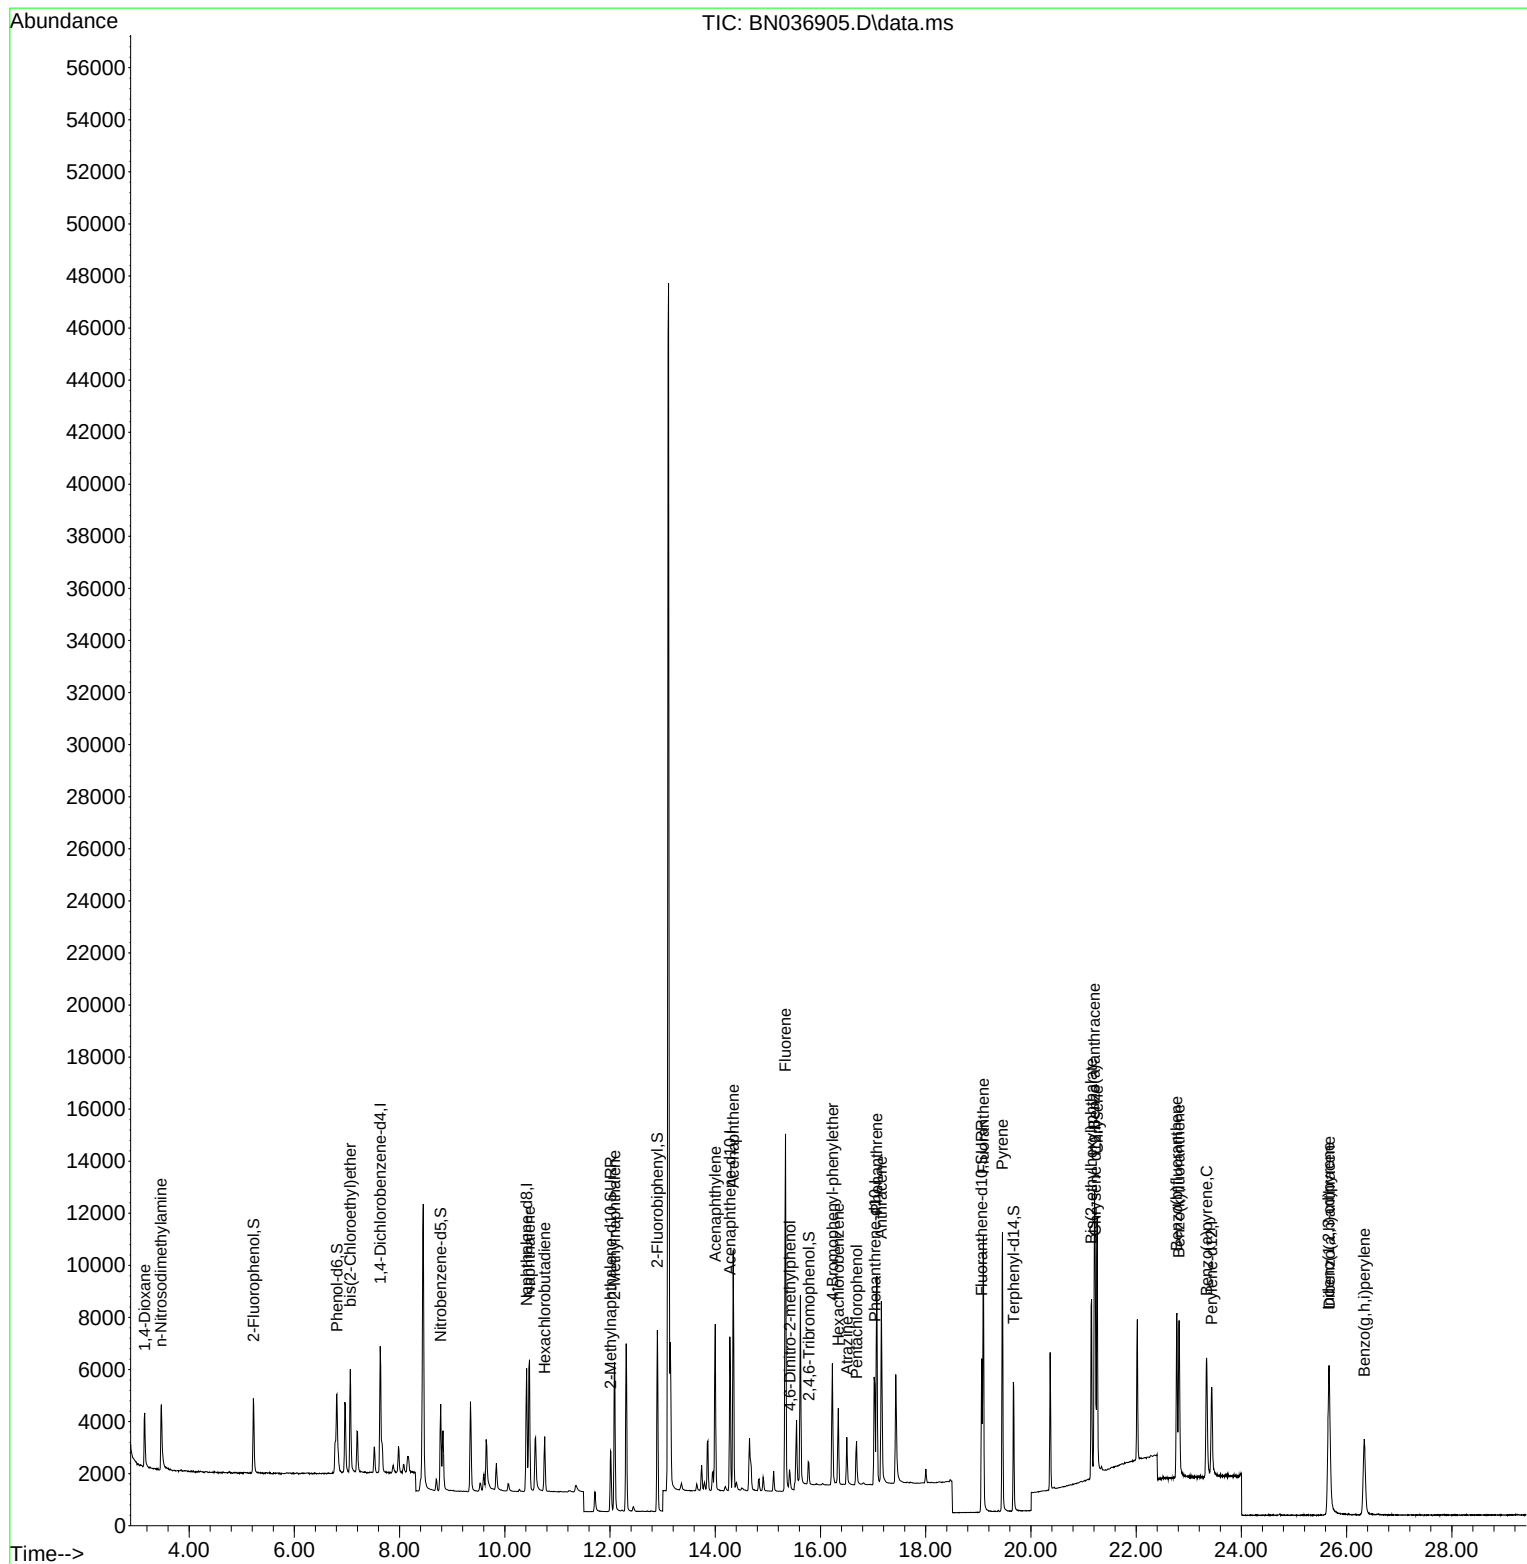




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion:152 Resp: 2284
Ion Ratio Lower Upper
152 100
150 154.3 121.4 182.2
115 68.6 55.4 83.2



#2
1,4-Dioxane
Concen: 0.467 ng
RT: 3.155 min Scan# 38
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion: 88 Resp: 1219
Ion Ratio Lower Upper
88 100
43 49.5 44.0 66.0
58 85.4 67.8 101.6









#3
n-Nitrosodimethylamine
Concen: 0.378 ng
RT: 3.465 min Scan# 81
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion: 42 Resp: 2281
Ion Ratio Lower Upper
42 100
74 73.1 52.3 78.5
44 11.0 7.4 11.2



#4
2-Fluorophenol
Concen: 0.391 ng
RT: 5.228 min Scan# 325
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion: 112 Resp: 2109
Ion Ratio Lower Upper
112 100
64 68.3 54.4 81.6
63 41.4 35.1 52.7









#5
Phenol-d6
Concen: 0.372 ng
RT: 6.809 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion	Ratio	Lower	Upper
99	100		
42	38.5	30.6	45.8
71	44.6	38.0	57.0



#6
bis(2-Chloroethyl)ether
Concen: 0.418 ng
RT: 7.062 min Scan# 579
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion	Ratio	Lower	Upper
93	100		
63	89.2	70.7	106.1
95	32.1	25.2	37.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion:	136	Resp:	5795
Ion	Ratio	Lower	Upper
136	100		
137	12.2	10.6	15.8
54	11.9	10.6	16.0
68	7.1	6.1	9.1



#8
Nitrobenzene-d5
Concen: 0.390 ng
RT: 8.781 min Scan# 796
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion:	82	Resp:	2553
Ion	Ratio	Lower	Upper
82	100		
128	35.8	29.0	43.4
54	67.2	60.8	91.2





#9

Naphthalene

Concen: 0.407 ng

RT: 10.468 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39

Instrument :

BNA_N

ClientSampleId :

ICVBN041425





Tgt Ion:128 Resp: 6854

Ion Ratio Lower Upper

128 100

129 11.9 10.3 15.5

127 13.9 12.7 19.1



#10

Hexachlorobutadiene

Concen: 0.411 ng

RT: 10.757 min Scan# 981

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39




Tgt Ion:225 Resp: 1591


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 62.0 51.0 76.4









#11
2-Methylnaphthalene-d10
Concen: 0.399 ng
RT: 12.011 min Scan# 1151
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion:152 Resp: 3366
Ion Ratio Lower Upper
152 100
151 21.7 17.1 25.7



#12
2-Methylnaphthalene
Concen: 0.376 ng
RT: 12.087 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion:142 Resp: 4031
Ion Ratio Lower Upper
142 100
141 89.0 73.0 109.4
115 47.0 41.1 61.7




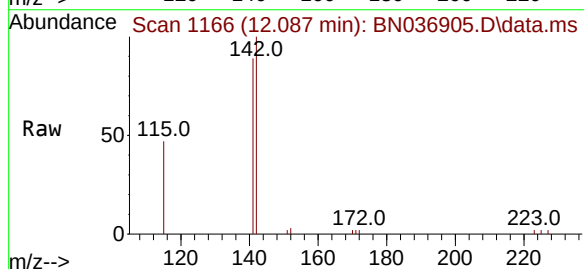




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion	Ratio	Lower	Upper
164	100		
162	109.5	83.8	125.8
160	54.7	44.7	67.1



#14
2,4,6-Tribromophenol
Concen: 0.331 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.3	77.0	115.6
141	58.6	44.5	66.7









#15
2-Fluorobiphenyl
Concen: 0.451 ng
RT: 12.899 min Scan# 1326
Delta R.T. -0.005 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion:	172	Resp:	6990
Ion	Ratio	Lower	Upper
172	100		
171	37.4	29.2	43.8
170	25.9	20.5	30.7



#16
Acenaphthylene
Concen: 0.446 ng
RT: 13.999 min Scan# 1440
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion:	152	Resp:	6788
Ion	Ratio	Lower	Upper
152	100		
151	20.2	15.8	23.8
153	13.1	10.2	15.4




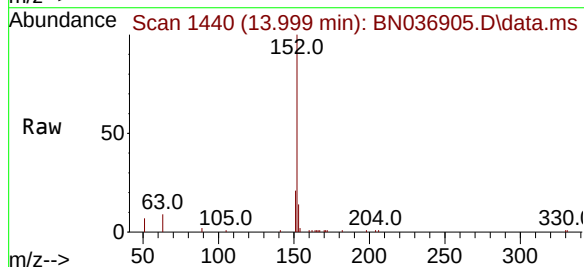




#17
Acenaphthene
Concen: 0.407 ng
RT: 14.341 min Scan# 1472
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion:154 Resp: 4084
Ion Ratio Lower Upper
154 100
153 117.6 94.7 142.1
152 63.3 49.4 74.2



#18
Fluorene
Concen: 0.407 ng
RT: 15.336 min Scan# 1565
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion:166 Resp: 5392
Ion Ratio Lower Upper
166 100
165 100.7 80.9 121.3
167 13.5 10.9 16.3





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.033 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39

Instrument :

BNA_N

ClientSampleId :

ICVBN041425





Tgt Ion:188 Resp: 6273

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 8.9 7.1 10.7



#20

4,6-Dinitro-2-methylphenol

Concen: 0.363 ng

RT: 15.421 min Scan# 1573

Delta R.T. 0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39




Tgt Ion:198 Resp: 621


Ion Ratio Lower Upper

198 100

51 85.1 68.4 102.6

105 42.8 38.7 58.1









#21
4-Bromophenyl-phenylether
Concen: 0.425 ng
RT: 16.227 min Scan# 1639
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion	Ratio	Lower	Upper
248	100		
250	94.9	77.0	115.6
141	77.0	63.0	94.4



#22
Hexachlorobenzene
Concen: 0.426 ng
RT: 16.338 min Scan# 1648
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion	Ratio	Lower	Upper
284	100		
142	50.6	42.6	64.0
249	36.7	29.1	43.7









#23
Atrazine
Concen: 0.456 ng
RT: 16.500 min Scan# 1661
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion	Ratio	Lower	Upper
200	100		
173	30.4	25.0	37.4
215	45.5	37.2	55.8



#24
Pentachlorophenol
Concen: 0.358 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.1	50.4	75.6
268	63.0	50.6	76.0









#25
Phenanthrene
Concen: 0.439 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion:178 Resp: 8446
Ion Ratio Lower Upper
178 100
176 19.8 16.2 24.2
179 15.2 12.2 18.4



#26
Anthracene
Concen: 0.445 ng
RT: 17.157 min Scan# 1714
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion:178 Resp: 7704
Ion Ratio Lower Upper
178 100
176 19.0 15.5 23.3
179 15.4 12.1 18.1





#27

Fluoranthene-d10

Concen: 0.407 ng

RT: 19.063 min Scan# 1942

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39

Instrument :

BNA_N

ClientSampleId :

ICVBN041425




Tgt Ion:212 Resp: 6761

Ion Ratio Lower Upper

212 100

106 14.2 10.6 15.8

104 8.8 6.6 10.0



#28

Fluoranthene

Concen: 0.414 ng

RT: 19.096 min Scan# 1949

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39




Tgt Ion:202 Resp: 9368


Ion Ratio Lower Upper

202 100

101 11.0 8.2 12.4

203 16.8 13.6 20.4





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39

Instrument :

BNA_N

ClientSampleId :

ICVBN041425





Tgt Ion:240 Resp: 5203

Ion Ratio Lower Upper

240 100

120 12.1 9.8 14.6

236 29.1 23.1 34.7



#30

Pyrene

Concen: 0.405 ng

RT: 19.458 min Scan# 2027

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39




Tgt Ion:202 Resp: 9483


Ion Ratio Lower Upper

202 100

200 21.0 17.0 25.6

203 17.8 14.1 21.1









#31
Terphenyl-d14
Concen: 0.441 ng
RT: 19.672 min Scan# 2073
Delta R.T. 0.005 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion	Ratio	Lower	Upper
244	100		
212	11.6	10.1	15.1
122	15.3	13.6	20.4



#32
Benzo(a)anthracene
Concen: 0.425 ng
RT: 21.206 min Scan# 2279
Delta R.T. -0.000 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.4	22.5	33.7
229	19.8	16.2	24.4





#33

Chrysene

Concen: 0.429 ng

RT: 21.260 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39

Instrument :

BNA_N

ClientSampleId :

ICVBN041425





Tgt Ion:228 Resp: 8745

Ion Ratio Lower Upper

228 100

226 31.0 24.9 37.3

229 19.9 15.9 23.9



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.421 ng

RT: 21.144 min Scan# 2272

Delta R.T. -0.000 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39




Tgt Ion:149 Resp: 4585


Ion Ratio Lower Upper

149 100

167 26.7 21.7 32.5

279 2.9 3.0 4.4#









#35
Perylene-d12
Concen: 0.400 ng
RT: 23.436 min Scan# 21
Delta R.T. 0.003 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39




Instrument :
BNA_N
ClientSampleId :
ICVBN041425


Tgt Ion:264 Resp: 4681
Ion Ratio Lower Upper
264 100
260 26.6 22.3 33.5
265 64.9 57.6 86.4



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.429 ng
RT: 25.661 min Scan# 3526
Delta R.T. 0.009 min
Lab File: BN036905.D
Acq: 14 Apr 2025 17:39

Tgt Ion:276 Resp: 7286
Ion Ratio Lower Upper
276 100
138 27.3 20.3 30.5
277 24.9 20.3 30.5





#37

Benzo(b)fluoranthene

Concen: 0.418 ng

RT: 22.772 min Scan# 2538

Delta R.T. 0.003 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39

Instrument :

BNA_N

ClientSampleId :

ICVBN041425





Tgt Ion:252 Resp: 7575

Ion Ratio Lower Upper

252 100

253 26.3 22.0 33.0

125 16.4 13.7 20.5



#38

Benzo(k)fluoranthene

Concen: 0.445 ng

RT: 22.816 min Scan# 2553

Delta R.T. 0.003 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39




Tgt Ion:252 Resp: 8145


Ion Ratio Lower Upper

252 100

253 26.7 22.7 34.1

125 16.2 12.5 18.7





#39

Benzo(a)pyrene

Concen: 0.453 ng

RT: 23.339 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39

Instrument :

BNA_N

ClientSampleId :

ICVBN041425





Tgt Ion:252 Resp: 6835

Ion Ratio Lower Upper

252 100

253 29.1 25.8 38.6

125 19.9 20.7 31.1#



#40

Dibenzo(a,h)anthracene

Concen: 0.424 ng

RT: 25.669 min Scan# 3529

Delta R.T. -0.006 min

Lab File: BN036905.D

Acq: 14 Apr 2025 17:39




Tgt Ion:278 Resp: 5596


Ion Ratio Lower Upper

278 100

139 22.0 16.9 25.3

279 28.9 25.7 38.5





#41

Benzo(g,h,i)perylene

Concen: 0.408 ng

RT: 26.336 min Scan# 31

Delta R.T. -0.000 min

Lab File: BN036905.D


Acq: 14 Apr 2025 17:39

Instrument :

BNA_N

ClientSampleId :

ICVBN041425





Tgt Ion:276 Resp: 5939

Ion Ratio Lower Upper

276 100

277 25.8 21.3 31.9

138 27.8 20.8 31.2



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036905.D
Acq On : 14 Apr 2025 17:39
Operator : RC/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN041425

Quant Time: Apr 14 18:01:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:58:02 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	165#	0.00
2	1,4-Dioxane	0.457	0.534	-16.8	176#	0.00
3	n-Nitrosodimethylamine	1.056	0.999	5.4	146	0.00
4 S	2-Fluorophenol	0.945	0.923	2.3	158#	0.00
5 S	Phenol-d6	1.186	1.102	7.1	155#	0.00
6	bis(2-Chloroethyl)ether	1.150	1.201	-4.4	172#	0.00
7 I	Naphthalene-d8	1.000	1.000	0.0	170#	0.00
8 S	Nitrobenzene-d5	0.452	0.441	2.4	169#	0.00
9	Naphthalene	1.162	1.183	-1.8	168#	0.00
10	Hexachlorobutadiene	0.267	0.275	-3.0	163#	0.00
11 SURR	2-Methylnaphthalene-d10	0.583	0.581	0.3	167#	0.00
12	2-Methylnaphthalene	0.740	0.696	5.9	158#	0.00
13 I	Acenaphthene-d10	1.000	1.000	0.0	169#	0.00
14 S	2,4,6-Tribromophenol	0.192	0.159	17.2	136	0.00
15 S	2-Fluorobiphenyl	1.931	2.179	-12.8	182#	0.00
16	Acenaphthylene	1.897	2.116	-11.5	188#	0.00
17	Acenaphthene	1.250	1.273	-1.8	169#	0.00
18	Fluorene	1.650	1.681	-1.9	170#	0.00
19 I	Phenanthrene-d10	1.000	1.000	0.0	167#	0.00
20	4,6-Dinitro-2-methylphenol	0.109	0.099	9.2	153#	0.00
21	4-Bromophenyl-phenylether	0.253	0.269	-6.3	164#	0.00
22	Hexachlorobenzene	0.284	0.303	-6.7	163#	0.00
23	Atrazine	0.211	0.240	-13.7	169#	0.00
24	Pentachlorophenol	0.152	0.136	10.5	142	0.00
25	Phenanthrene	1.226	1.346	-9.8	170#	0.00
26	Anthracene	1.104	1.228	-11.2	175#	0.00
27 SURR	Fluoranthene-d10	1.058	1.078	-1.9	158#	0.00
28	Fluoranthene	1.441	1.493	-3.6	162#	0.00
29 I	Chrysene-d12	1.000	1.000	0.0	162#	0.00
30	Pyrene	1.800	1.823	-1.3	161#	0.00
31 S	Terphenyl-d14	0.875	0.965	-10.3	173#	0.00
32	Benzo(a)anthracene	1.452	1.543	-6.3	170#	0.00
33	Chrysene	1.569	1.681	-7.1	166#	0.00
34	Bis(2-ethylhexyl)phthalate	0.837	0.881	-5.3	164#	0.00
35 I	Perylene-d12	1.000	1.000	0.0	154#	0.00
36	Indeno(1,2,3-cd)pyrene	1.450	1.557	-7.4	157#	0.00
37	Benzo(b)fluoranthene	1.547	1.618	-4.6	152#	0.00
38	Benzo(k)fluoranthene	1.562	1.740	-11.4	159#	0.00
39 C	Benzo(a)pyrene	1.290	1.460	-13.2	164#	0.00
40	Dibenzo(a,h)anthracene	1.128	1.195	-5.9	156#	0.00
41	Benzo(g,h,i)perylene	1.244	1.269	-2.0	147	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036905.D
Acq On : 14 Apr 2025 17:39
Operator : RC/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN041425

Quant Time: Apr 14 18:01:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:58:02 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	0.400	0.400	0.0	165	0.00
2	1,4-Dioxane	0.400	0.467	-16.8	176	0.00
3	n-Nitrosodimethylamine	0.400	0.378	5.5	146	0.00
4 S	2-Fluorophenol	0.400	0.391	2.3	158	0.00
5 S	Phenol-d6	0.400	0.372	7.0	155	0.00
6	bis(2-Chloroethyl)ether	0.400	0.418	-4.5	172	0.00
7 I	Naphthalene-d8	0.400	0.400	0.0	170	0.00
8 S	Nitrobenzene-d5	0.400	0.390	2.5	169	0.00
9	Naphthalene	0.400	0.407	-1.7	168	0.00
10	Hexachlorobutadiene	0.400	0.411	-2.7	163	0.00
11 SURR	2-Methylnaphthalene-d10	0.400	0.399	0.3	167	0.00
12	2-Methylnaphthalene	0.400	0.376	6.0	158	0.00
13 I	Acenaphthene-d10	0.400	0.400	0.0	169	0.00
14 S	2,4,6-Tribromophenol	0.400	0.331	17.3	136	0.00
15 S	2-Fluorobiphenyl	0.400	0.451	-12.7	182	0.00
16	Acenaphthylene	0.400	0.446	-11.5	188	0.00
17	Acenaphthene	0.400	0.407	-1.7	169	0.00
18	Fluorene	0.400	0.407	-1.7	170	0.00
19 I	Phenanthrene-d10	0.400	0.400	0.0	167	0.00
20	4,6-Dinitro-2-methylphenol	0.400	0.363	9.3	153	0.00
21	4-Bromophenyl-phenylether	0.400	0.425	-6.2	164	0.00
22	Hexachlorobenzene	0.400	0.426	-6.5	163	0.00
23	Atrazine	0.400	0.456	-14.0	169	0.00
24	Pentachlorophenol	0.400	0.358	10.5	142	0.00
25	Phenanthrene	0.400	0.439	-9.7	170	0.00
26	Anthracene	0.400	0.445	-11.2	175	0.00
27 SURR	Fluoranthene-d10	0.400	0.407	-1.7	158	0.00
28	Fluoranthene	0.400	0.414	-3.5	162	0.00
29 I	Chrysene-d12	0.400	0.400	0.0	162	0.00
30	Pyrene	0.400	0.405	-1.3	161	0.00
31 S	Terphenyl-d14	0.400	0.441	-10.2	173	0.00
32	Benzo(a)anthracene	0.400	0.425	-6.2	170	0.00
33	Chrysene	0.400	0.429	-7.2	166	0.00
34	Bis(2-ethylhexyl)phthalate	0.400	0.421	-5.2	164	0.00
35 I	Perylene-d12	0.400	0.400	0.0	154	0.00
36	Indeno(1,2,3-cd)pyrene	0.400	0.429	-7.2	157	0.00
37	Benzo(b)fluoranthene	0.400	0.418	-4.5	152	0.00
38	Benzo(k)fluoranthene	0.400	0.445	-11.2	159	0.00
39 C	Benzo(a)pyrene	0.400	0.453	-13.2	164	0.00
40	Dibenzo(a,h)anthracene	0.400	0.424	-6.0	156	0.00
41	Benzo(g,h,i)perylene	0.400	0.408	-2.0	147	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

7C

SEMIVOLATILE CONTINUING CALIBRATION CHECK

Lab Name: CHEMTECH Contract: JAC005

Lab Code: CHEM Case No.: Q1741 SAS No.: Q1741 SDG No.: Q1741

Instrument ID: BNA_N Calibration Date/Time: 04/11/2025 18:45

Lab File ID: BN036884.D Init. Calib. Date(s): 04/11/2025 04/11/2025

EPA Sample No.: SSTDCCC0.4 Init. Calib. Time(s): 11:42 15:42

GC Column: ZB-GR ID: 0.25 (mm)

COMPOUND	RRF	RRF0.4	MIN RRF	%D	MAX%D
2-Methylnaphthalene-d10	0.582	0.596		2.4	20.0
Fluoranthene-d10	1.127	1.290		14.5	20.0
2-Fluorophenol	0.941	0.980		4.1	20.0
Phenol-d6	1.203	1.244		3.4	20.0
Nitrobenzene-d5	0.444	0.442		-0.4	20.0
2-Fluorobiphenyl	1.921	2.017		5.0	20.0
2,4,6-Tribromophenol	0.193	0.204		5.7	20.0
Terphenyl-d14	0.760	0.770		1.3	20.0
1,4-Dioxane	0.464	0.386		-16.8	20.0

All other compounds must meet a minimum RRF of 0.010.

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036884.D
 Acq On : 11 Apr 2025 18:45
 Operator : RC/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Apr 11 23:05:46 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 16:11:08 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	254	0.400	ng	0.00
7) Naphthalene-d8	10.425	136	679	0.400	ng	# 0.00
13) Acenaphthene-d10	14.288	164	407	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	865	0.400	ng	0.00
29) Chrysene-d12	21.233	240	1015	0.400	ng	0.00
35) Perylene-d12	23.447	264	1369	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.235	112	249	0.417	ng	0.00
5) Phenol-d6	6.816	99	316	0.414	ng	0.00
8) Nitrobenzene-d5	8.792	82	300	0.398	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	405	0.410	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	83	0.423	ng	0.00
15) 2-Fluorobiphenyl	12.908	172	821	0.420	ng	0.00
27) Fluoranthene-d10	19.072	212	1116	0.458	ng	0.00
31) Terphenyl-d14	19.676	244	782	0.406	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.155	88	98m	0.333	ng	Qvalue
3) n-Nitrosodimethylamine	3.472	42	310	0.475	ng	# 93
6) bis(2-Chloroethyl)ether	7.069	93	312	0.416	ng	91
9) Naphthalene	10.468	128	821	0.420	ng	# 92
10) Hexachlorobutadiene	10.767	225	197	0.445	ng	# 97
12) 2-Methylnaphthalene	12.097	142	526	0.418	ng	# 91
16) Acenaphthylene	14.010	152	772	0.408	ng	98
17) Acenaphthene	14.352	154	527	0.428	ng	94
18) Fluorene	15.346	166	705	0.415	ng	99
20) 4,6-Dinitro-2-methylph...	15.432	198	81	0.395	ng	# 67
21) 4-Bromophenyl-phenylether	16.239	248	229	0.442	ng	96
22) Hexachlorobenzene	16.350	284	276	0.450	ng	99
23) Atrazine	16.512	200	253	0.499	ng	91
24) Pentachlorophenol	16.698	266	157	0.489	ng	# 91
25) Phenanthrene	17.070	178	1134	0.437	ng	96
26) Anthracene	17.170	178	1021	0.442	ng	99
28) Fluoranthene	19.100	202	1468	0.450	ng	99
30) Pyrene	19.467	202	1572	0.410	ng	98
32) Benzo(a)anthracene	21.215	228	1507	0.420	ng	97
33) Chrysene	21.269	228	1762	0.446	ng	98
34) Bis(2-ethylhexyl)phtha...	21.152	149	1203	0.452	ng	99
36) Indeno(1,2,3-cd)pyrene	25.675	276	3065	0.469	ng	96
37) Benzo(b)fluoranthene	22.784	252	1963	0.404	ng	96
38) Benzo(k)fluoranthene	22.830	252	2101m	0.429	ng	
39) Benzo(a)pyrene	23.351	252	1900	0.446	ng	# 94
40) Dibenzo(a,h)anthracene	25.693	278	2440	0.470	ng	97
41) Benzo(g,h,i)perylene	26.359	276	2713	0.463	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036884.D
Acq On : 11 Apr 2025 18:45
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Apr 11 23:05:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration




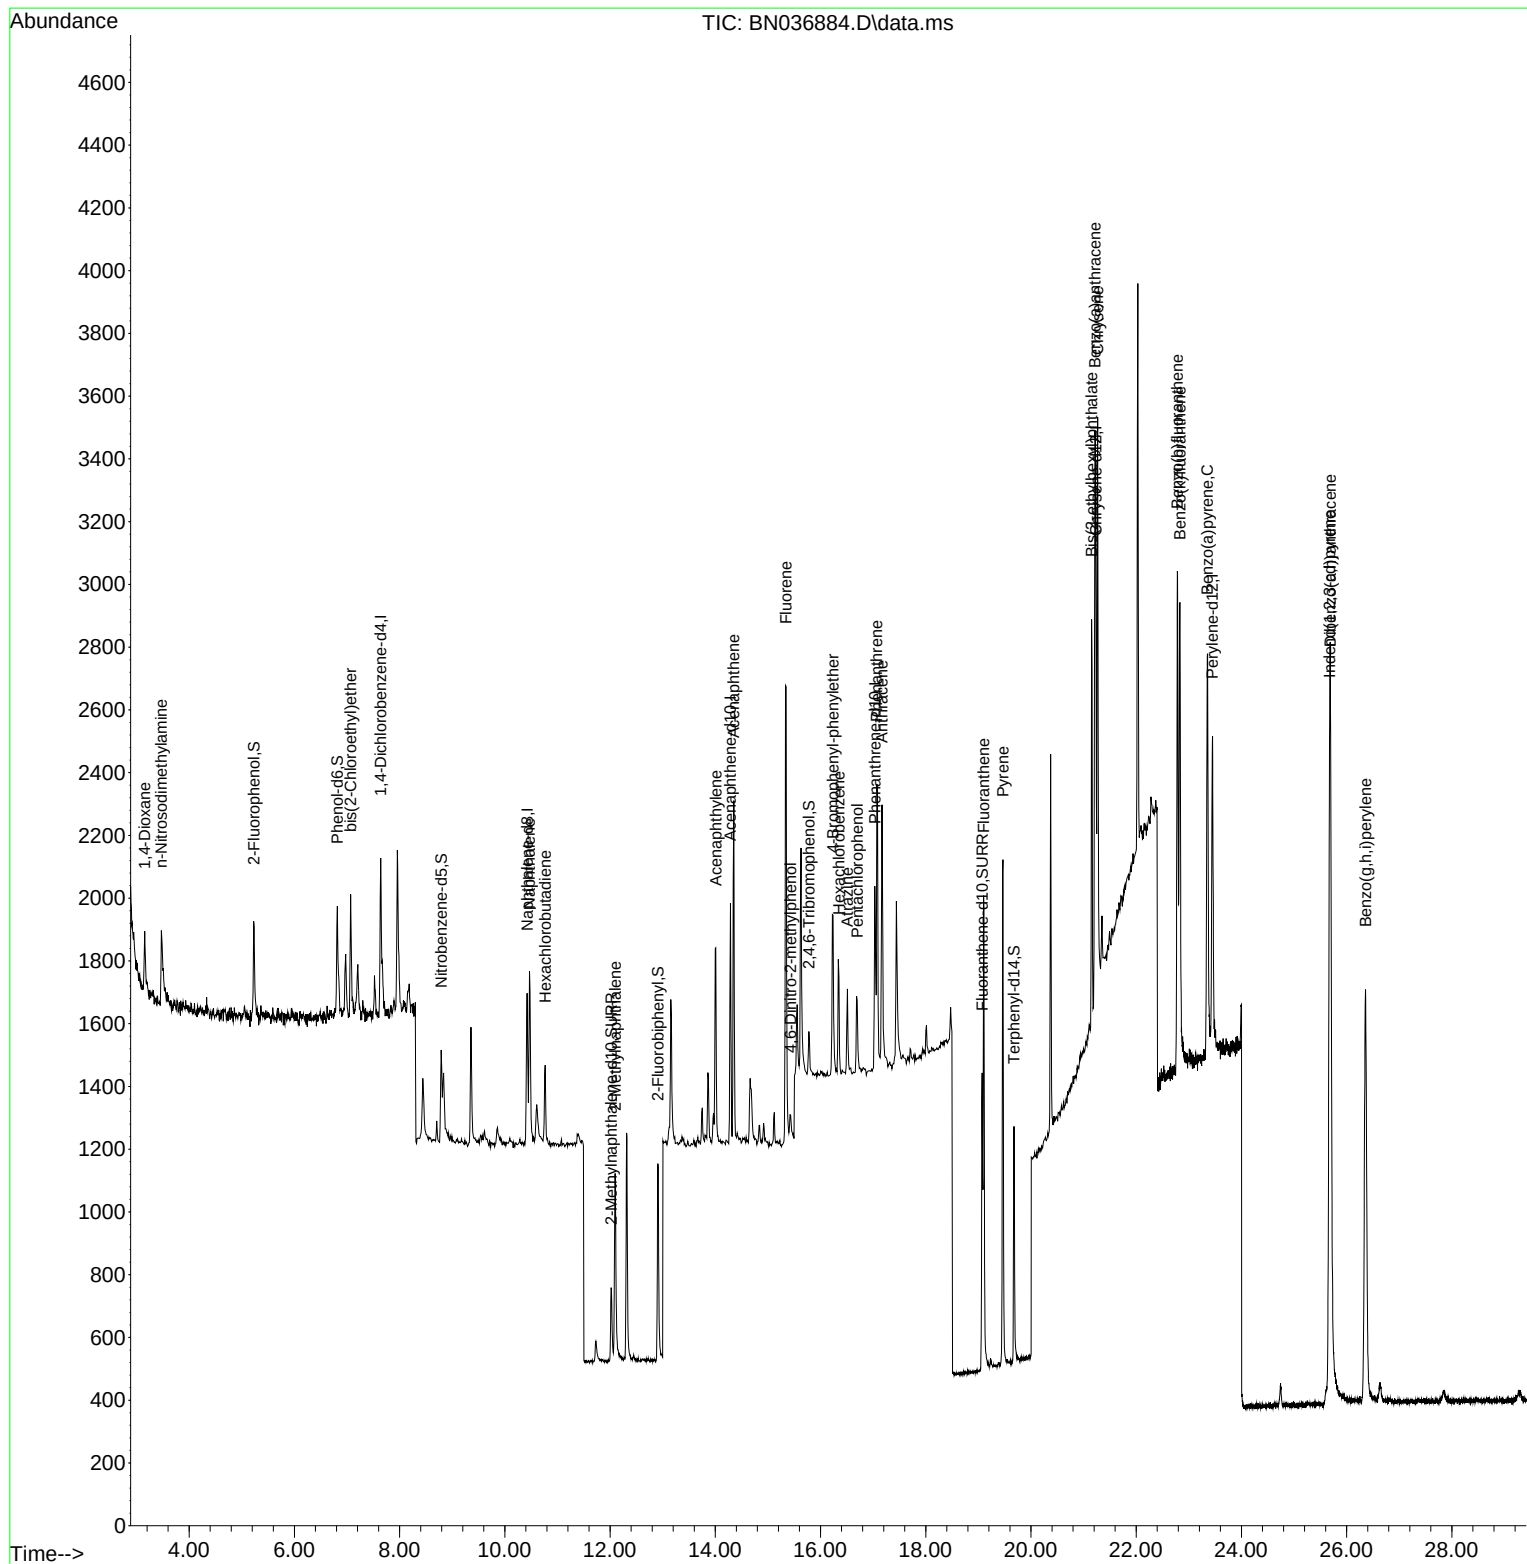




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.640 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN036884.D
 Acq: 11 Apr 2025 18:45




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:152 Resp: 254
 Ion Ratio Lower Upper
 152 100
 150 154.4 123.0 184.6
 115 85.7 60.1 90.1



#2
 1,4-Dioxane
 Concen: 0.333 ng m
 RT: 3.155 min Scan# 38
 Delta R.T. -0.000 min
 Lab File: BN036884.D
 Acq: 11 Apr 2025 18:45

Tgt Ion: 88 Resp: 98
 Ion Ratio Lower Upper
 88 100
 43 77.6 39.2 58.8#
 58 135.7 63.5 95.3#









#3
n-Nitrosodimethylamine
Concen: 0.475 ng
RT: 3.472 min Scan# 81
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 310
Ion Ratio Lower Upper
42 100
74 62.6 54.6 81.8
44 0.0 0.0 0.0



#4
2-Fluorophenol
Concen: 0.417 ng
RT: 5.235 min Scan# 326
Delta R.T. 0.007 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion: 112 Resp: 249
Ion Ratio Lower Upper
112 100
64 69.1 54.0 81.0
63 45.8 35.1 52.7









#5
Phenol-d6
Concen: 0.414 ng
RT: 6.816 min Scan# 54
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 99 Resp: 316




Ion	Ratio	Lower	Upper
99	100		
42	42.4	30.9	46.3
71	46.2	38.6	58.0




#6
bis(2-Chloroethyl)ether
Concen: 0.416 ng
RT: 7.069 min Scan# 580
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion: 93 Resp: 312

Ion	Ratio	Lower	Upper
93	100		
63	85.6	76.4	114.6
95	30.1	26.1	39.1









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.425 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	679
Ion	Ratio	Lower	Upper
136	100		
137	22.2	13.5	20.3#
54	21.0	12.8	19.2#
68	17.7	10.1	15.1#

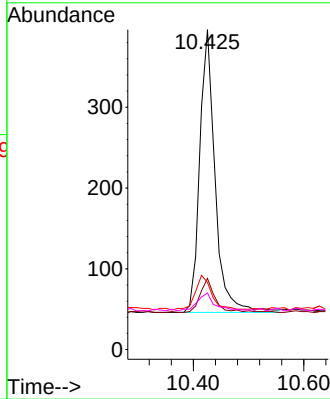

#8
Nitrobenzene-d5
Concen: 0.398 ng
RT: 8.792 min Scan# 797
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:	82	Resp:	300
Ion	Ratio	Lower	Upper
82	100		
128	54.9	35.5	53.3#
54	76.6	56.2	84.4



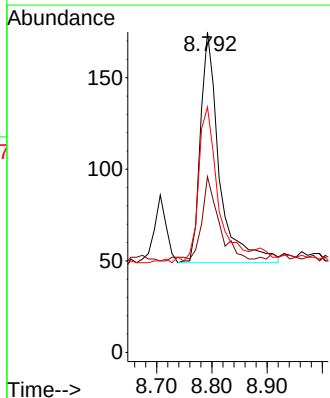





#9
Naphthalene
Concen: 0.420 ng
RT: 10.468 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	128	Resp:	821
Ion	Ratio	Lower	Upper
128	100		
129	20.9	12.9	19.3#
127	21.3	15.0	22.6

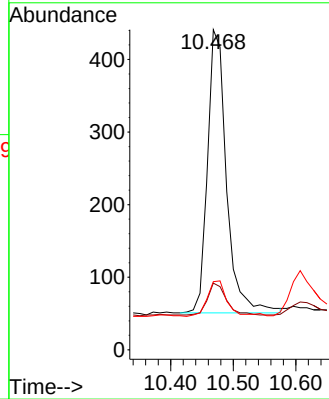

#10
Hexachlorobutadiene
Concen: 0.445 ng
RT: 10.767 min Scan# 982
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:	225	Resp:	197
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	60.4	50.5	75.7


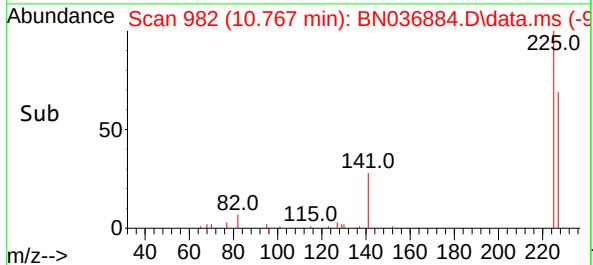






#11
2-Methylnaphthalene-d10
Concen: 0.410 ng
RT: 12.021 min Scan# 1153
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 405
Ion Ratio Lower Upper
152 100
151 22.0 17.8 26.8



#12
2-Methylnaphthalene
Concen: 0.418 ng
RT: 12.097 min Scan# 1168
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:142 Resp: 526
Ion Ratio Lower Upper
142 100
141 97.9 73.8 110.8
115 65.1 43.3 64.9#









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 407
Ion Ratio Lower Upper
164 100
162 103.4 85.7 128.5
160 59.6 46.9 70.3

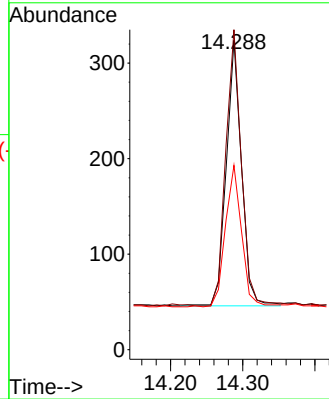

#14
2,4,6-Tribromophenol
Concen: 0.423 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:330 Resp: 83
Ion Ratio Lower Upper
330 100
332 103.6 87.0 130.6
141 63.9 45.3 67.9









#15
2-Fluorobiphenyl
Concen: 0.420 ng
RT: 12.908 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:172 Resp: 821




Ion	Ratio	Lower	Upper
172	100		
171	41.6	32.7	49.1
170	31.7	23.3	34.9




#16
Acenaphthylene
Concen: 0.408 ng
RT: 14.010 min Scan# 1441
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:152 Resp: 772

Ion	Ratio	Lower	Upper
152	100		
151	21.0	16.4	24.6
153	14.6	10.3	15.5





#17

Acenaphthene

Concen: 0.428 ng

RT: 14.352 min Scan# 1473

Delta R.T. -0.000 min

Lab File: BN036884.D

Acq: 11 Apr 2025 18:45

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:154 Resp: 527

Ion Ratio Lower Upper

154 100

153 114.8 97.8 146.6

152 62.2 52.7 79.1



#18

Fluorene

Concen: 0.415 ng

RT: 15.346 min Scan# 1566

Delta R.T. -0.000 min

Lab File: BN036884.D

Acq: 11 Apr 2025 18:45




Tgt Ion:166 Resp: 705


Ion Ratio Lower Upper

166 100

165 103.1 83.2 124.8

167 14.3 11.1 16.7




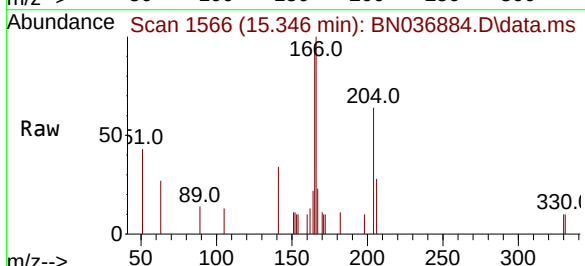




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.033 min Scan# 1704
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion	188	Resp	865
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	19.0	13.9	20.9



#20
4,6-Dinitro-2-methylphenol
Concen: 0.395 ng
RT: 15.432 min Scan# 1574
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion	198	Resp	81
Ion Ratio	Lower	Upper	
198	100		
51	176.0	107.6	161.4#
105	93.3	55.2	82.8#









#21
4-Bromophenyl-phenylether
Concen: 0.442 ng
RT: 16.239 min Scan# 1640
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 229
Ion Ratio Lower Upper
248 100
250 98.9 83.5 125.3
141 71.4 55.3 82.9



#22
Hexachlorobenzene
Concen: 0.450 ng
RT: 16.350 min Scan# 1649
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:284 Resp: 276
Ion Ratio Lower Upper
284 100
142 48.2 37.7 56.5
249 36.6 29.0 43.6









#23
Atrazine
Concen: 0.499 ng
RT: 16.512 min Scan# 1662
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion	Ratio	Lower	Upper
200	100		
173	41.5	28.6	43.0
215	56.4	40.5	60.7

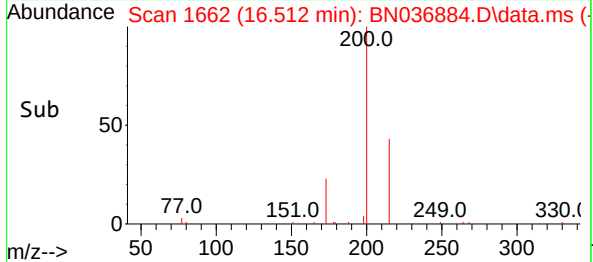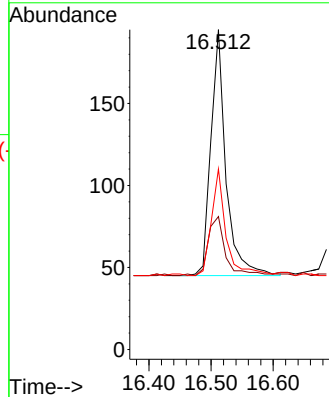

#24
Pentachlorophenol
Concen: 0.489 ng
RT: 16.698 min Scan# 1677
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion	Ratio	Lower	Upper
266	100		
264	69.4	44.6	66.8
268	64.3	51.8	77.6


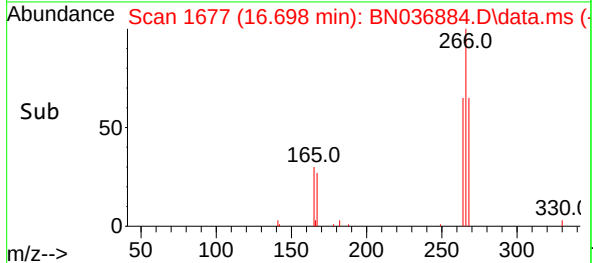






#25
Phenanthrene
Concen: 0.437 ng
RT: 17.070 min Scan# 1707
Delta R.T. -0.013 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178	Resp:	1134
Ion	Ratio	Lower Upper
178	100	
176	18.4	16.6 25.0
179	15.1	12.8 19.2

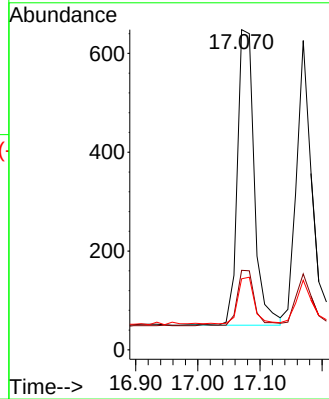

#26
Anthracene
Concen: 0.442 ng
RT: 17.170 min Scan# 1715
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:178	Resp:	1021
Ion	Ratio	Lower Upper
178	100	
176	19.6	15.8 23.6
179	15.3	12.6 18.8









#27
Fluoranthene-d10
Concen: 0.458 ng
RT: 19.072 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion	Ratio	Lower	Upper
212	100		
106	13.3	11.2	16.8
104	8.2	7.5	11.3

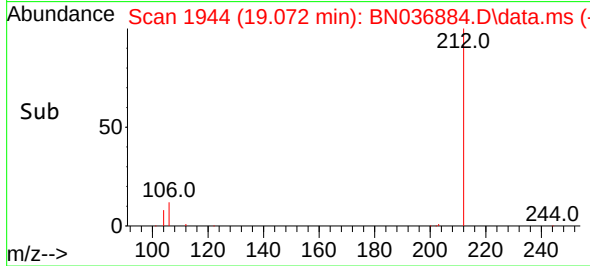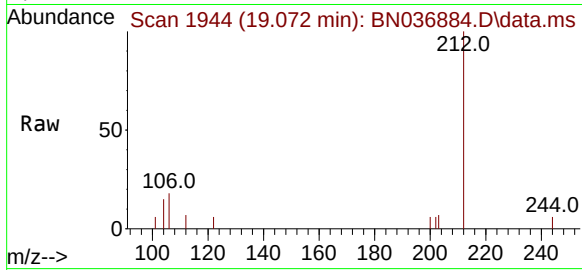

#28
Fluoranthene
Concen: 0.450 ng
RT: 19.100 min Scan# 1950
Delta R.T. -0.005 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.1	8.5	12.7
203	17.6	13.8	20.6









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.233 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	240	Resp:	1015
Ion Ratio	Lower	Upper	
240	100		
120	22.4	15.8	23.6
236	33.4	25.8	38.8

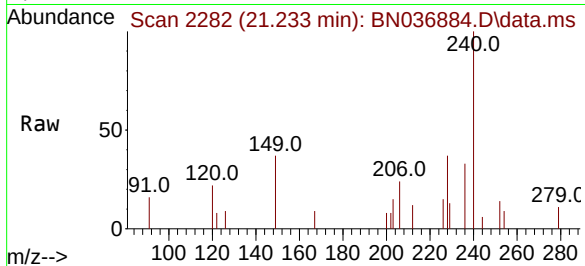

#30
Pyrene
Concen: 0.410 ng
RT: 19.467 min Scan# 2029
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:	202	Resp:	1572
Ion Ratio	Lower	Upper	
202	100		
200	20.4	17.1	25.7
203	16.8	14.5	21.7




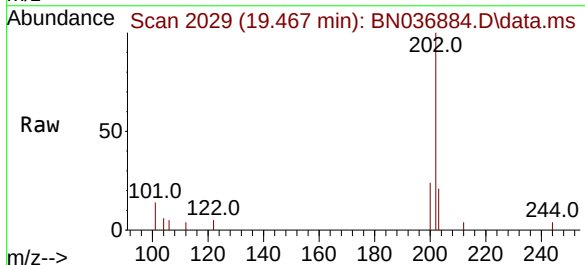




#31
Terphenyl-d14
Concen: 0.406 ng
RT: 19.676 min Scan# 2074
Delta R.T. -0.005 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 782
Ion Ratio Lower Upper
244 100
212 17.1 11.6 17.4
122 21.7 14.9 22.3



#32
Benzo(a)anthracene
Concen: 0.420 ng
RT: 21.215 min Scan# 2280
Delta R.T. -0.000 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:228 Resp: 1507
Ion Ratio Lower Upper
228 100
226 32.8 24.5 36.7
229 23.2 17.7 26.5

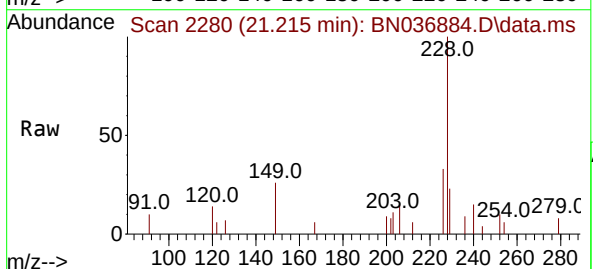



#33

Chrysene

Concen: 0.446 ng

RT: 21.269 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN036884.D

Acq: 11 Apr 2025 18:45

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:228 Resp: 1762

Ion Ratio Lower Upper

228 100

226 33.9 26.1 39.1

229 22.5 17.0 25.4



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.452 ng

RT: 21.152 min Scan# 2273

Delta R.T. -0.009 min

Lab File: BN036884.D

Acq: 11 Apr 2025 18:45




Tgt Ion:149 Resp: 1203


Ion Ratio Lower Upper

149 100

167 27.0 21.0 31.4

279 4.6 3.6 5.4





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.447 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN036884.D

Acq: 11 Apr 2025 18:45

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:264 Resp: 1369

Ion Ratio Lower Upper

264 100

260 29.6 22.9 34.3

265 130.8 88.6 132.8



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.469 ng

RT: 25.675 min Scan# 3531

Delta R.T. -0.012 min

Lab File: BN036884.D

Acq: 11 Apr 2025 18:45




Tgt Ion:276 Resp: 3065


Ion Ratio Lower Upper

276 100

138 23.2 21.0 31.6

277 25.1 19.3 28.9









#37
Benzo(b)fluoranthene
Concen: 0.404 ng
RT: 22.784 min Scan# 2542
Delta R.T. -0.006 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 1963
Ion Ratio Lower Upper
252 100
253 35.5 27.0 40.6
125 25.2 17.7 26.5

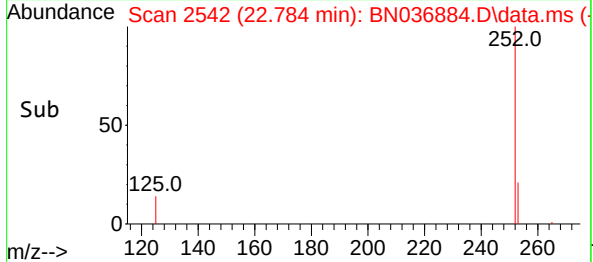

#38
Benzo(k)fluoranthene
Concen: 0.429 ng m
RT: 22.830 min Scan# 2558
Delta R.T. -0.003 min
Lab File: BN036884.D
Acq: 11 Apr 2025 18:45

Tgt Ion:252 Resp: 2101
Ion Ratio Lower Upper
252 100
253 35.8 26.7 40.1
125 21.8 16.9 25.3

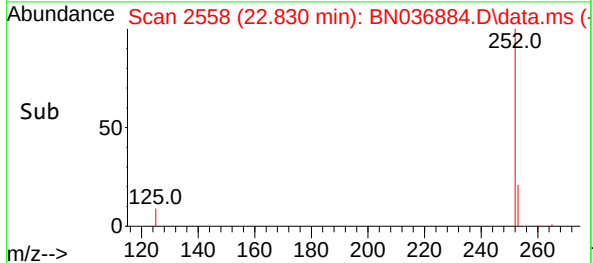



#39

Benzo(a)pyrene

Concen: 0.446 ng

RT: 23.351 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN036884.D

Acq: 11 Apr 2025 18:45

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:252 Resp: 1900

Ion Ratio Lower Upper

252 100

253 40.8 31.5 47.3

125 34.5 22.6 34.0#



#40

Dibenzo(a,h)anthracene

Concen: 0.470 ng

RT: 25.693 min Scan# 3537

Delta R.T. -0.009 min

Lab File: BN036884.D

Acq: 11 Apr 2025 18:45




Tgt Ion:278 Resp: 2440


Ion Ratio Lower Upper

278 100

139 21.7 17.6 26.4

279 35.8 26.7 40.1





#41

Benzo(g,h,i)perylene

Concen: 0.463 ng

RT: 26.359 min Scan# 31

Delta R.T. -0.003 min

Lab File: BN036884.D


Acq: 11 Apr 2025 18:45

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:276 Resp: 2713

Ion Ratio Lower Upper

276 100

277 26.5 21.8 32.8

138 28.2 21.6 32.4

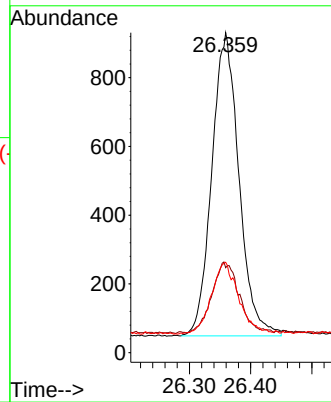

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036884.D
 Acq On : 11 Apr 2025 18:45
 Operator : RC/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Quant Time: Apr 11 23:05:46 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 16:11:08 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	52	0.00
2	1,4-Dioxane	0.464	0.386	16.8	45#	0.00
3	n-Nitrosodimethylamine	1.028	1.220	-18.7	58	0.00
4 S	2-Fluorophenol	0.941	0.980	-4.1	53	0.00
5 S	Phenol-d6	1.203	1.244	-3.4	54	0.00
6	bis(2-Chloroethyl)ether	1.180	1.228	-4.1	54	0.00
7 I	Naphthalene-d8	1.000	1.000	0.0	54	0.00
8 S	Nitrobenzene-d5	0.444	0.442	0.5	53	0.00
9	Naphthalene	1.151	1.209	-5.0	56	0.00
10	Hexachlorobutadiene	0.261	0.290	-11.1	55	0.00
11 SURR	2-Methylnaphthalene-d10	0.582	0.596	-2.4	54	0.00
12	2-Methylnaphthalene	0.741	0.775	-4.6	55	0.00
13 I	Acenaphthene-d10	1.000	1.000	0.0	55	0.00
14 S	2,4,6-Tribromophenol	0.193	0.204	-5.7	61	0.00
15 S	2-Fluorobiphenyl	1.921	2.017	-5.0	55	0.00
16	Acenaphthylene	1.858	1.897	-2.1	55	0.00
17	Acenaphthene	1.210	1.295	-7.0	57	0.00
18	Fluorene	1.669	1.732	-3.8	56	0.00
19 I	Phenanthrene-d10	1.000	1.000	0.0	55	0.00
20	4,6-Dinitro-2-methylphenol	0.095	0.094	1.1	54	0.00
21	4-Bromophenyl-phenylether	0.240	0.265	-10.4	56	0.00
22	Hexachlorobenzene	0.284	0.319	-12.3	57	0.00
23	Atrazine	0.234	0.292	-24.8	61	0.00
24	Pentachlorophenol	0.149	0.182	-22.1	62	0.00
25	Phenanthrene	1.199	1.311	-9.3	55	-0.01
26	Anthracene	1.069	1.180	-10.4	56	0.00
27 SURR	Fluoranthene-d10	1.127	1.290	-14.5	58	0.00
28	Fluoranthene	1.509	1.697	-12.5	58	0.00
29 I	Chrysene-d12	1.000	1.000	0.0	62	0.00
30	Pyrene	1.512	1.549	-2.4	60	0.00
31 S	Terphenyl-d14	0.760	0.770	-1.3	59	0.00
32	Benzo(a)anthracene	1.413	1.485	-5.1	66	0.00
33	Chrysene	1.558	1.736	-11.4	65	0.00
34	Bis(2-ethylhexyl)phthalate	1.049	1.185	-13.0	72	0.00
35 I	Perylene-d12	1.000	1.000	0.0	72	0.00
36	Indeno(1,2,3-cd)pyrene	1.909	2.239	-17.3	80	-0.01
37	Benzo(b)fluoranthene	1.419	1.434	-1.1	68	0.00
38	Benzo(k)fluoranthene	1.432	1.535	-7.2	75	0.00
39 C	Benzo(a)pyrene	1.244	1.388	-11.6	74	0.00
40	Dibenzo(a,h)anthracene	1.516	1.782	-17.5	81	0.00
41	Benzo(g,h,i)perylene	1.714	1.982	-15.6	79	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036884.D
Acq On : 11 Apr 2025 18:45
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4

Quant Time: Apr 11 23:05:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	0.400	0.400	0.0	52	0.00
2	1,4-Dioxane	0.400	0.333	16.8	45	0.00
3	n-Nitrosodimethylamine	0.400	0.475	-18.7	58	0.00
4 S	2-Fluorophenol	0.400	0.417	-4.2	53	0.00
5 S	Phenol-d6	0.400	0.414	-3.5	54	0.00
6	bis(2-Chloroethyl)ether	0.400	0.416	-4.0	54	0.00
7 I	Naphthalene-d8	0.400	0.400	0.0	54	0.00
8 S	Nitrobenzene-d5	0.400	0.398	0.5	53	0.00
9	Naphthalene	0.400	0.420	-5.0	56	0.00
10	Hexachlorobutadiene	0.400	0.445	-11.2	55	0.00
11 SURR	2-Methylnaphthalene-d10	0.400	0.410	-2.5	54	0.00
12	2-Methylnaphthalene	0.400	0.418	-4.5	55	0.00
13 I	Acenaphthene-d10	0.400	0.400	0.0	55	0.00
14 S	2,4,6-Tribromophenol	0.400	0.423	-5.7	61	0.00
15 S	2-Fluorobiphenyl	0.400	0.420	-5.0	55	0.00
16	Acenaphthylene	0.400	0.408	-2.0	55	0.00
17	Acenaphthene	0.400	0.428	-7.0	57	0.00
18	Fluorene	0.400	0.415	-3.7	56	0.00
19 I	Phenanthrene-d10	0.400	0.400	0.0	55	0.00
20	4,6-Dinitro-2-methylphenol	0.400	0.395	1.3	54	0.00
21	4-Bromophenyl-phenylether	0.400	0.442	-10.5	56	0.00
22	Hexachlorobenzene	0.400	0.450	-12.5	57	0.00
23	Atrazine	0.400	0.499	-24.7	61	0.00
24	Pentachlorophenol	0.400	0.489	-22.2	62	0.00
25	Phenanthrene	0.400	0.437	-9.2	55	-0.01
26	Anthracene	0.400	0.442	-10.5	56	0.00
27 SURR	Fluoranthene-d10	0.400	0.458	-14.5	58	0.00
28	Fluoranthene	0.400	0.450	-12.5	58	0.00
29 I	Chrysene-d12	0.400	0.400	0.0	62	0.00
30	Pyrene	0.400	0.410	-2.5	60	0.00
31 S	Terphenyl-d14	0.400	0.406	-1.5	59	0.00
32	Benzo(a)anthracene	0.400	0.420	-5.0	66	0.00
33	Chrysene	0.400	0.446	-11.5	65	0.00
34	Bis(2-ethylhexyl)phthalate	0.400	0.452	-13.0	72	0.00
35 I	Perylene-d12	0.400	0.400	0.0	72	0.00
36	Indeno(1,2,3-cd)pyrene	0.400	0.469	-17.2	80	-0.01
37	Benzo(b)fluoranthene	0.400	0.404	-1.0	68	0.00
38	Benzo(k)fluoranthene	0.400	0.429	-7.2	75	0.00
39 C	Benzo(a)pyrene	0.400	0.446	-11.5	74	0.00
40	Dibenzo(a,h)anthracene	0.400	0.470	-17.5	81	0.00
41	Benzo(g,h,i)perylene	0.400	0.463	-15.8	79	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



QC SAMPLE DATA


- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036872.D
Acq On : 11 Apr 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 11 16:11:08 2025

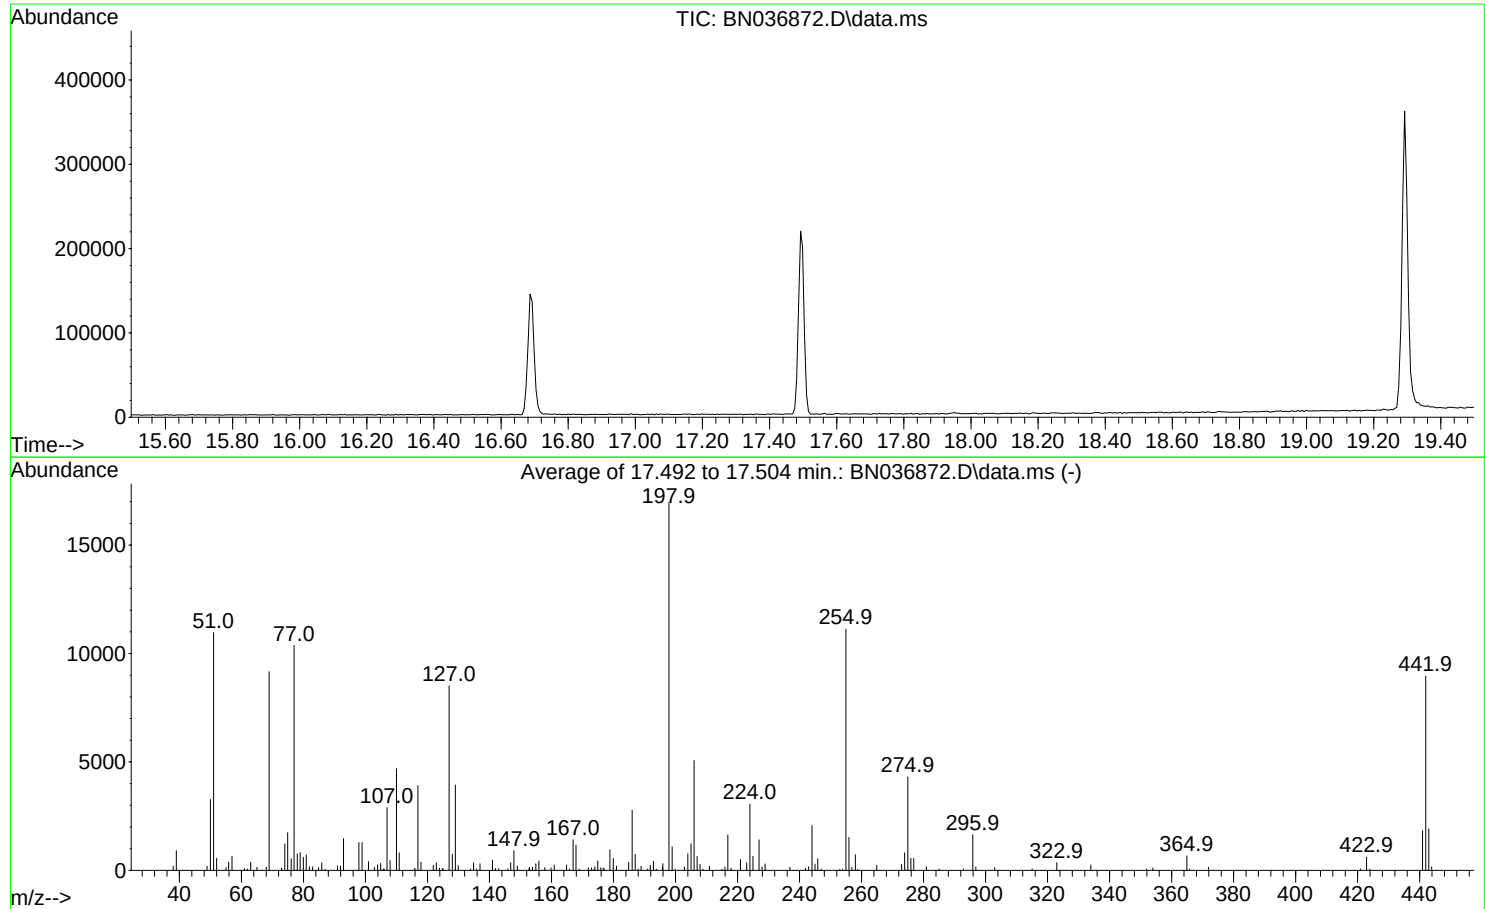

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.6	10965	PASS
68	69	0.00	2	1.6	147	PASS
69	198	0.00	100	54.0	9164	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	8509	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16964	PASS
199	198	5	9	6.4	1083	PASS
275	198	10	60	25.4	4308	PASS
365	198	1	100	3.9	661	PASS
441	198	0.01	100	10.8	1829	PASS
442	442	50	100	100.0	8955	PASS
443	442	15	24	21.3	1910	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/11/2025	BNA_N	<u>BN036872.D</u>
Compound Name	Response	Retention Time
DDT	68421	20.533
DDD	473	20.145
DDE	0	19.621
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
473	68894	0.69

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036872.D
Acq On : 11 Apr 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 11 16:50:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

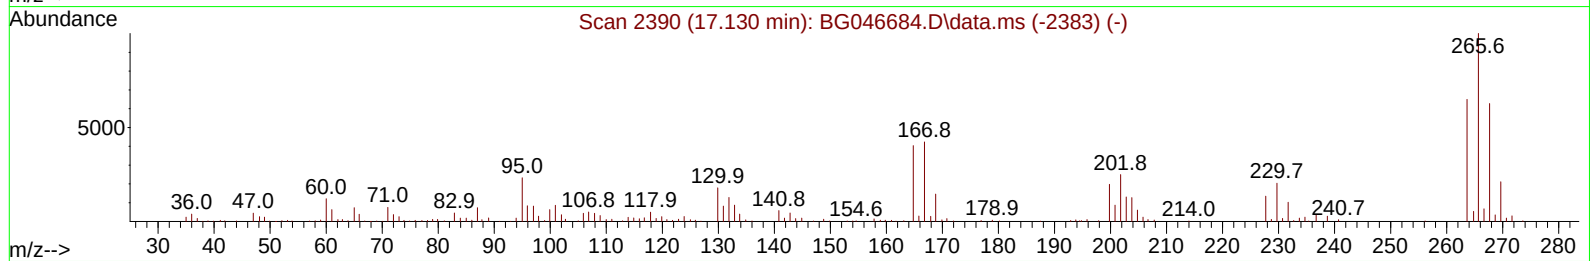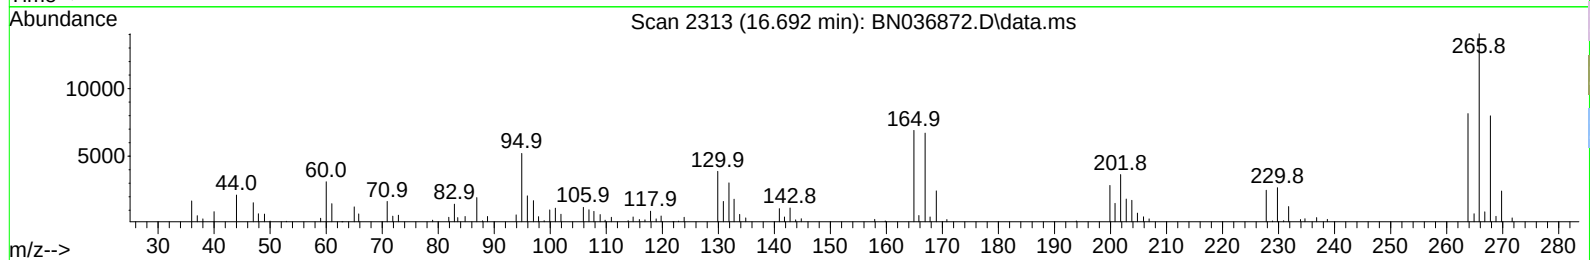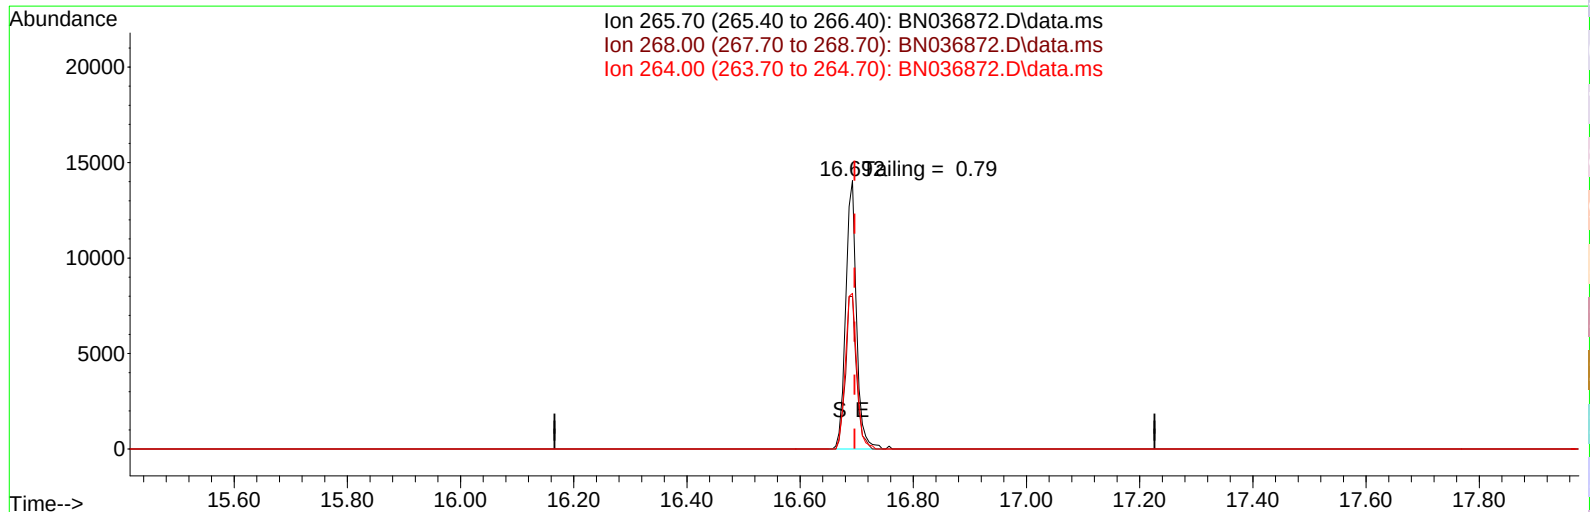

TIC: BN036872.D\data.ms

(70) Pentachlorophenol (C)

16.692min (-0.004) 36331.83 ng




response 18533

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.86
264.00	61.60	58.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036872.D
Acq On : 11 Apr 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 11 16:50:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

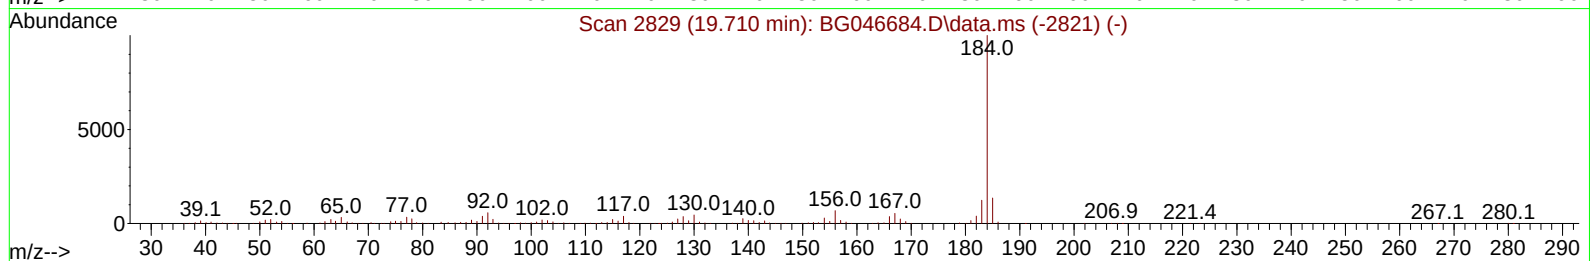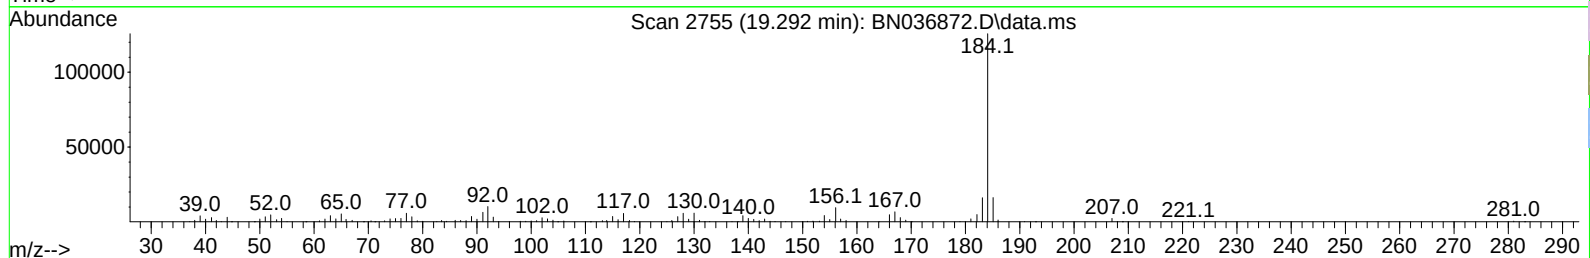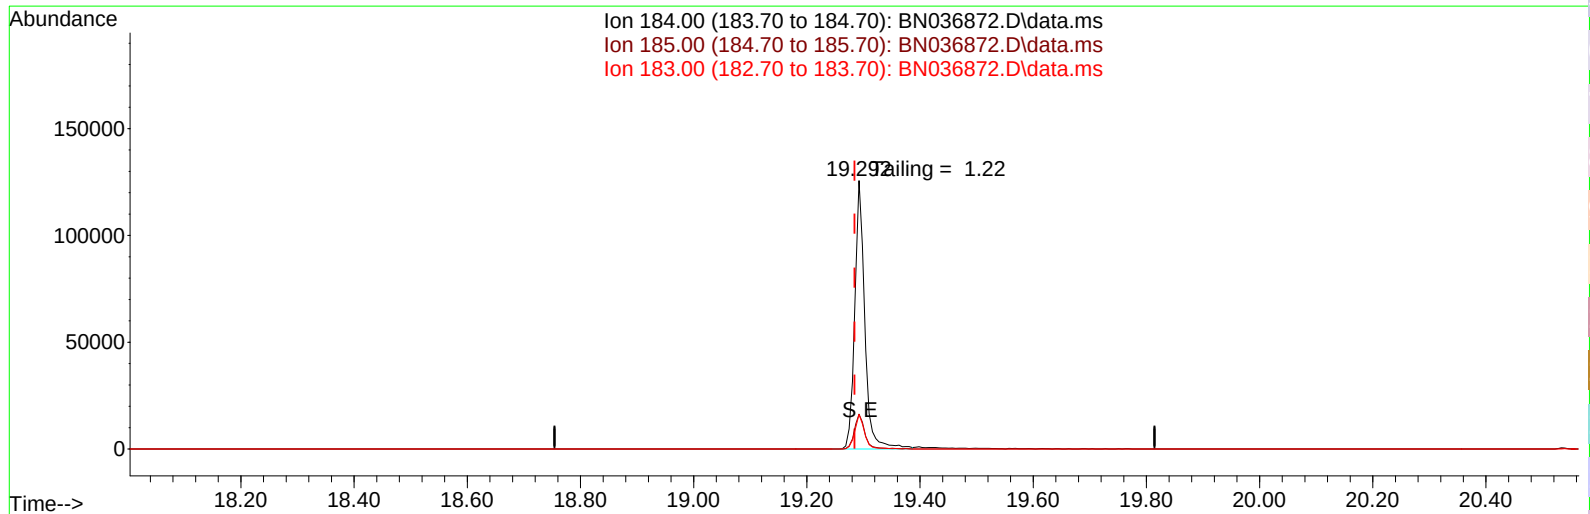

TIC: BN036872.D\data.ms

(77) Benzidine

19.292min (+ 0.008) 0.00 ng

response 156190



Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	12.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036883.D
Acq On : 11 Apr 2025 18:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 11 16:11:08 2025

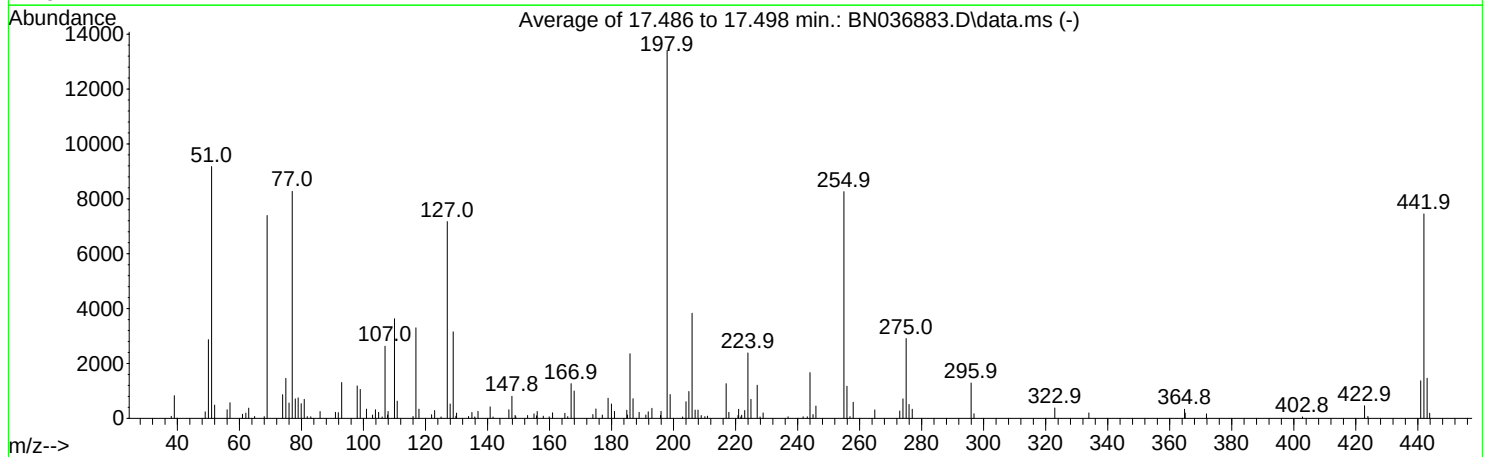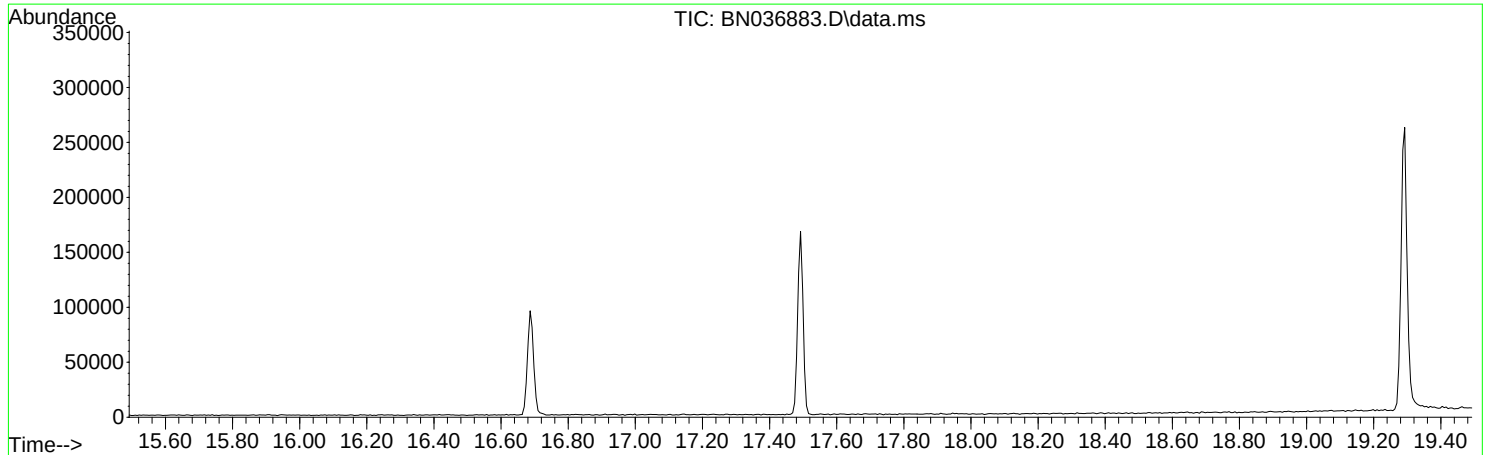

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	68.5	9178	PASS
68	69	0.00	2	0.9	64	PASS
69	198	0.00	100	55.2	7395	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	7172	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13404	PASS
199	198	5	9	6.5	866	PASS
275	198	10	60	21.7	2912	PASS
365	198	1	100	2.5	334	PASS
441	198	0.01	100	10.2	1368	PASS
442	442	50	100	100.0	7452	PASS
443	442	15	24	19.6	1464	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/11/2025	BNA_N	<u>BN036883.D</u>
Compound Name	Response	Retention Time
DDT	54631	20.533
DDD	872	20.145
DDE	0	19.621
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
872	55503	1.57

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036883.D
Acq On : 11 Apr 2025 18:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 11 23:52:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

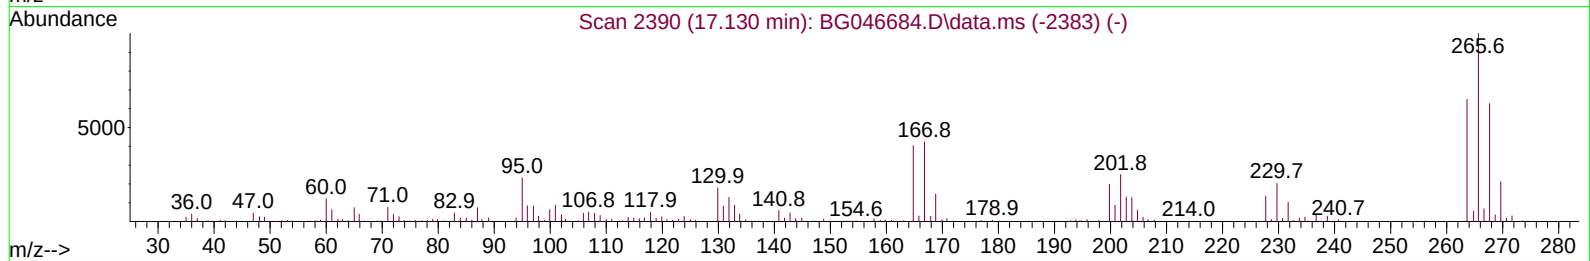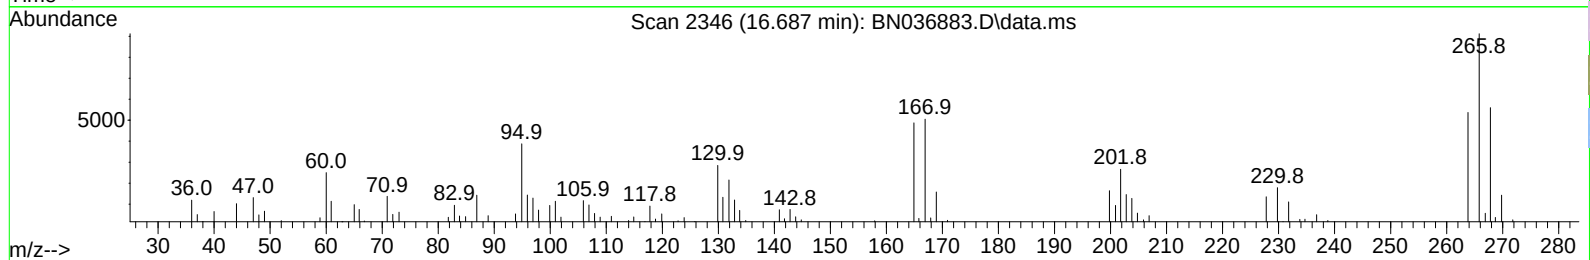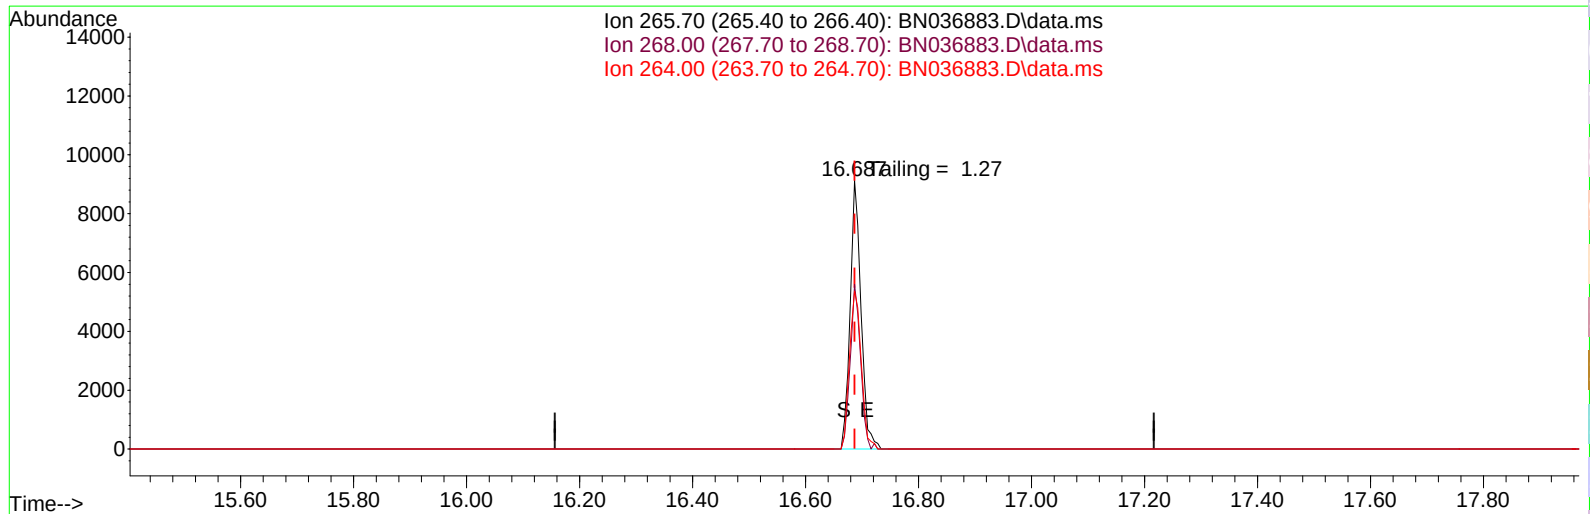

TIC: BN036883.D\data.ms

(70) Pentachlorophenol (C)

16.687min (0.000) 0.00 ng




response 12230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.36
264.00	61.60	58.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036883.D
Acq On : 11 Apr 2025 18:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 11 23:52:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

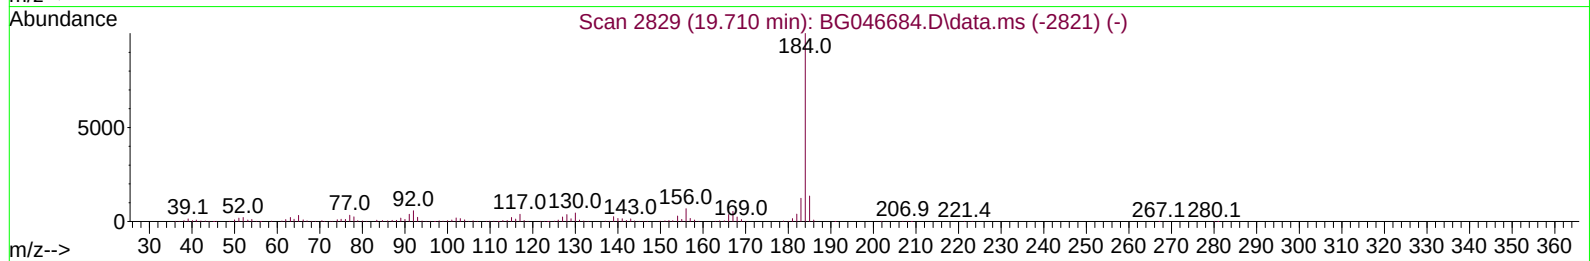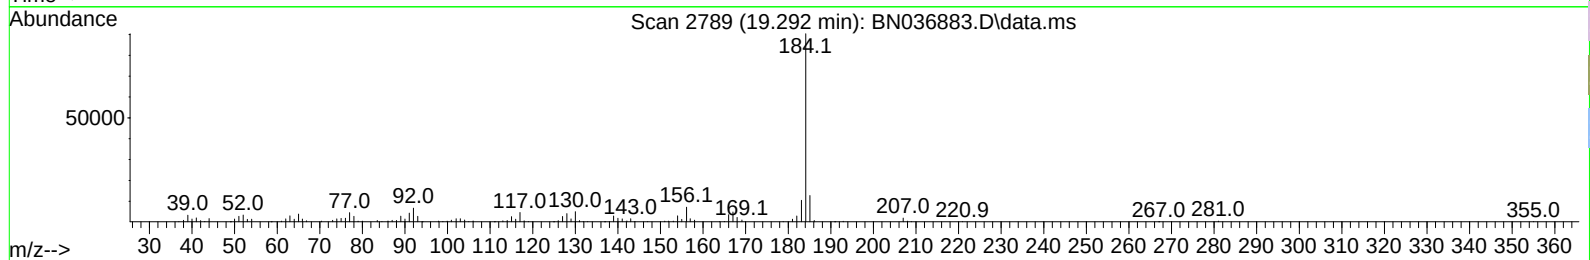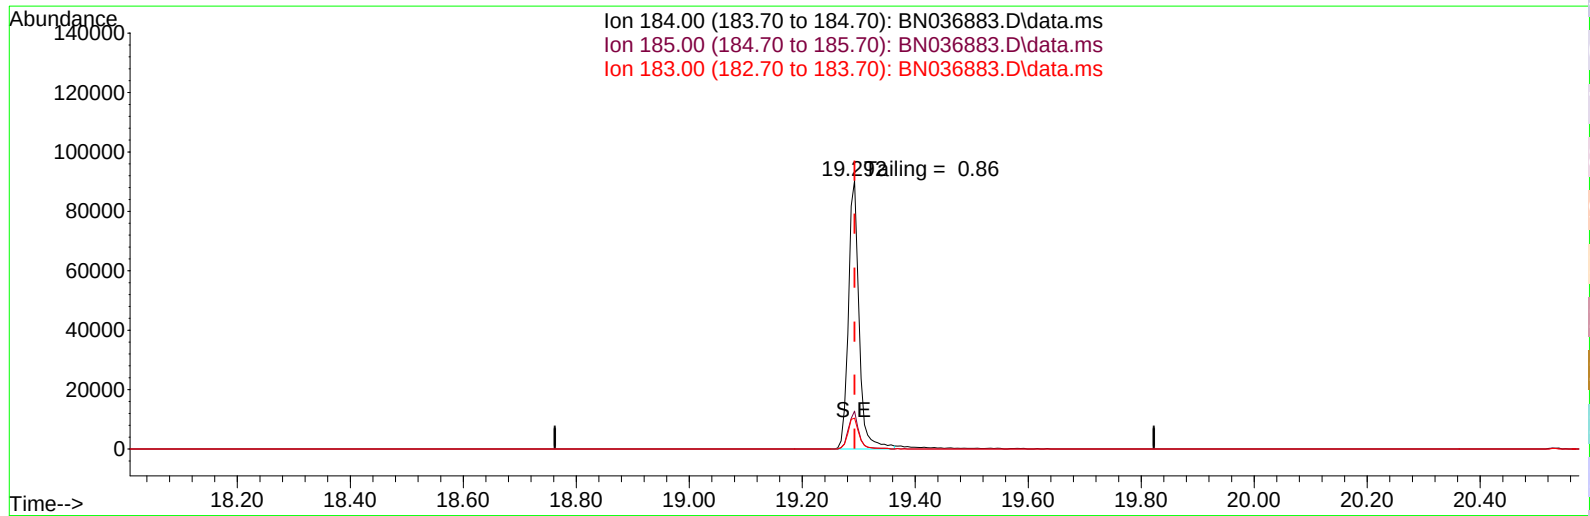

TIC: BN036883.D\data.ms

(77) Benzidine

19.292min (0.000) 0.00 ng

response 121284



Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036896.D
Acq On : 14 Apr 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 14 17:58:02 2025

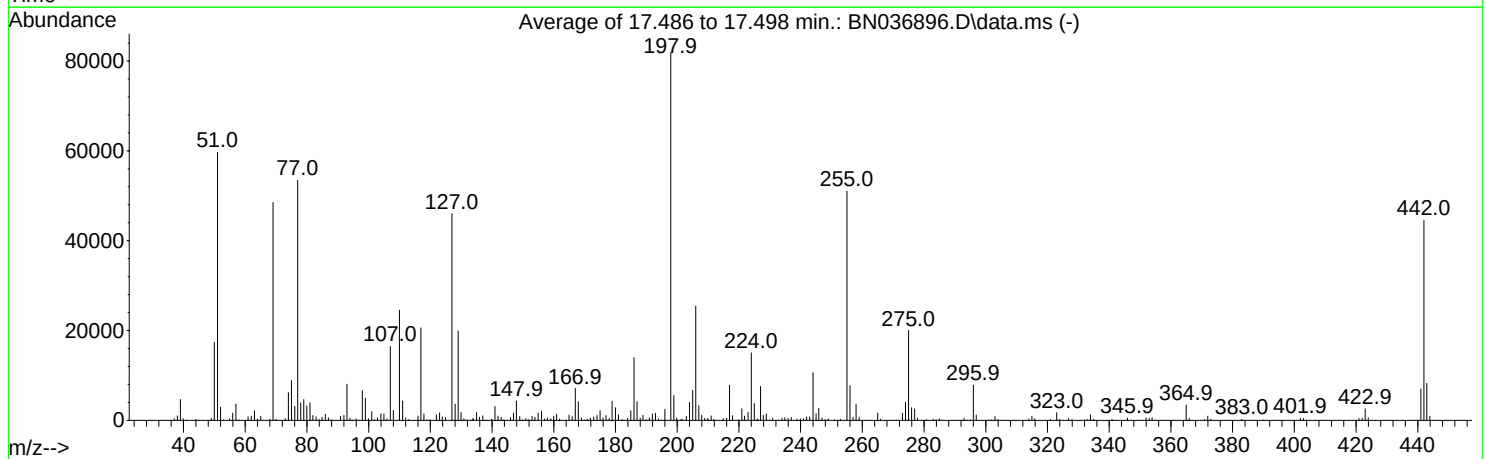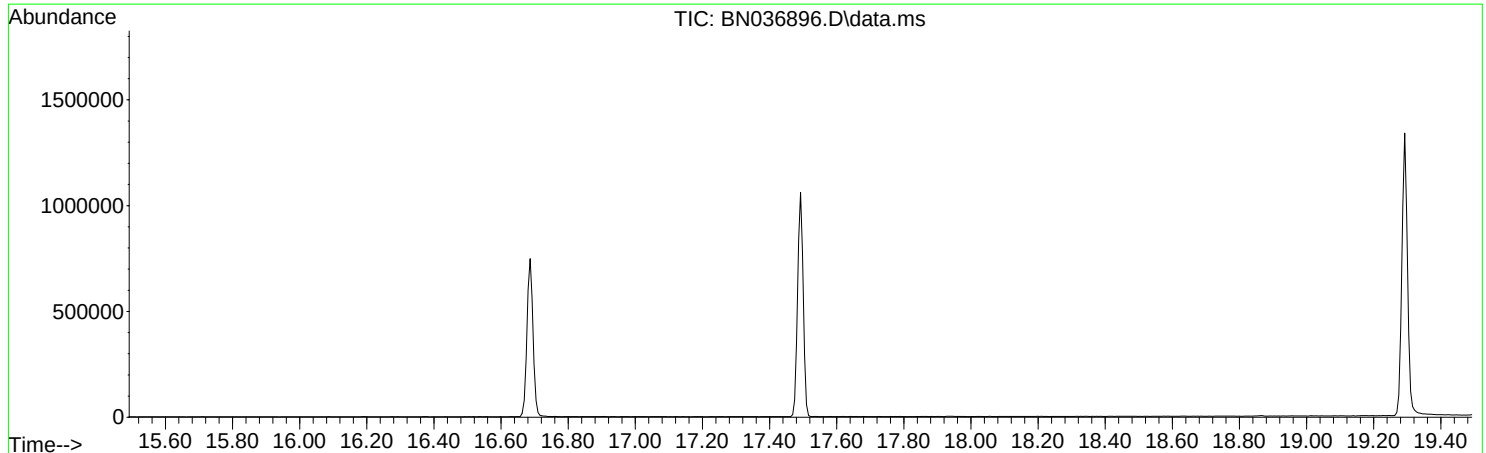

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	72.9	59683	PASS
68	69	0.00	2	0.6	275	PASS
69	198	0.00	100	59.2	48509	PASS
70	69	0.00	2	0.5	233	PASS
127	198	10	80	56.2	46043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81893	PASS
199	198	5	9	6.8	5540	PASS
275	198	10	60	24.4	20016	PASS
365	198	1	100	4.2	3404	PASS
441	198	0.01	100	8.5	6985	PASS
442	442	50	100	100.0	44557	PASS
443	442	15	24	18.5	8228	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/14/2025	BNA_N	<u>BN036896.D</u>
Compound Name	Response	Retention Time
DDT	288576	20.533
DDD	2965	20.145
DDE	0	19.621
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2965	291541	1.02

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036896.D
Acq On : 14 Apr 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 14 19:33:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

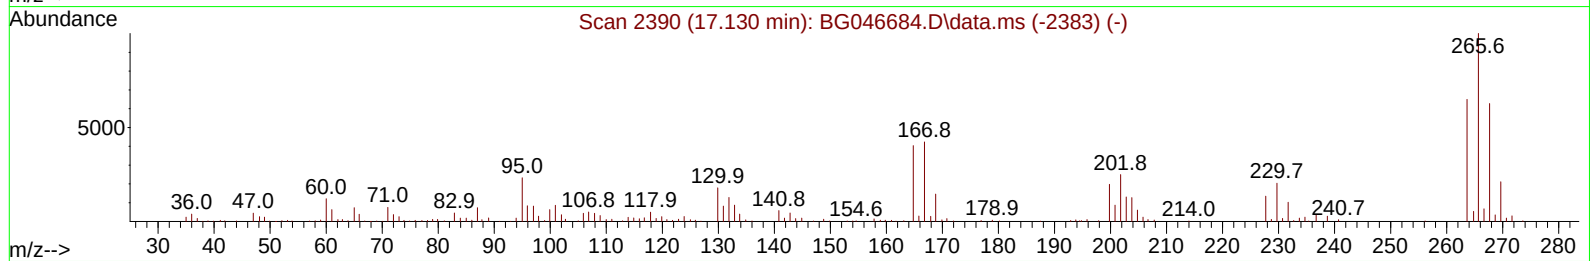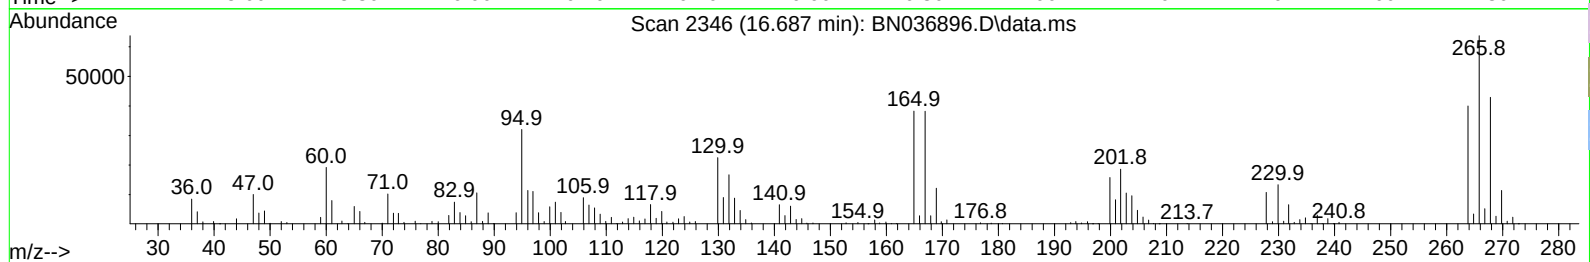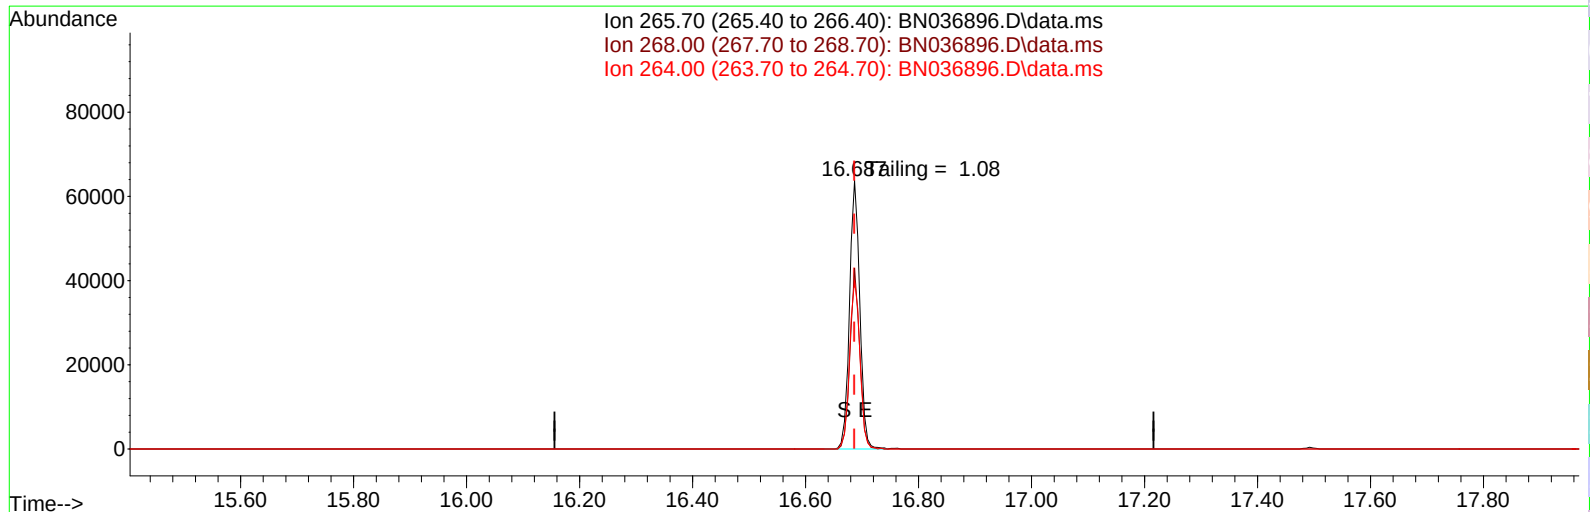

TIC: BN036896.D\data.ms

(70) Pentachlorophenol (C)

16.687min (+ 0.001) 15197.46 ng




response 80743

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.34
264.00	61.60	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036896.D
Acq On : 14 Apr 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 14 19:23:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

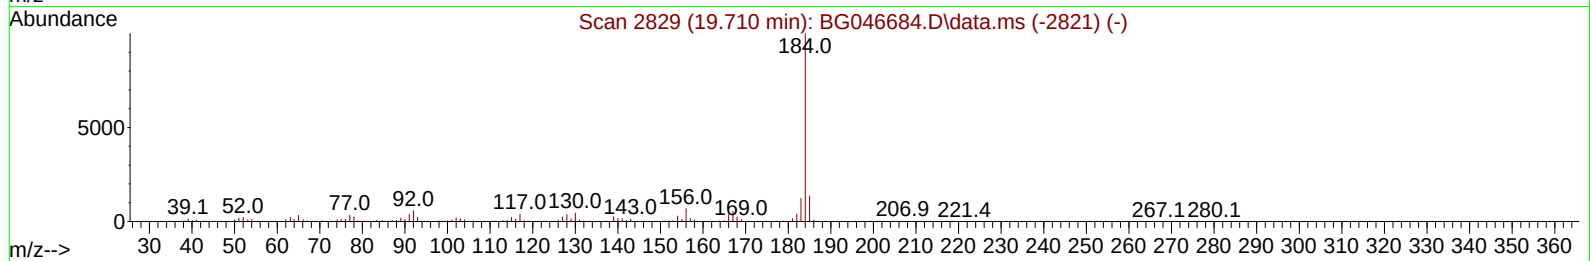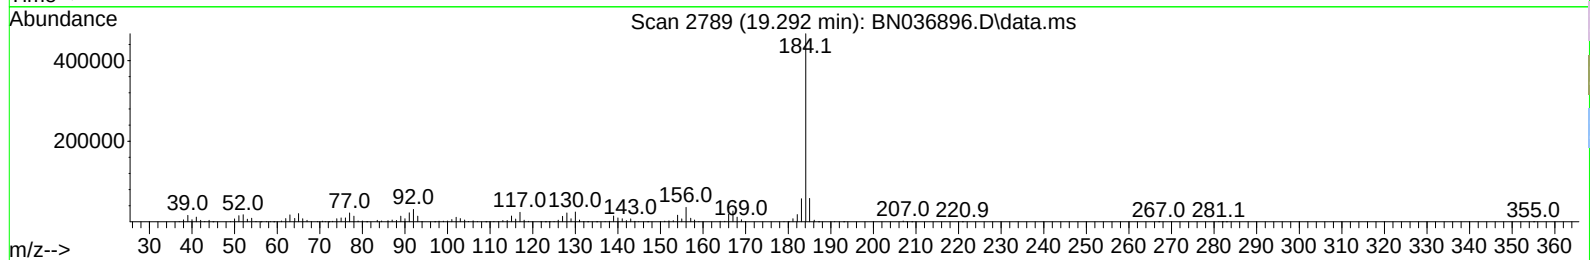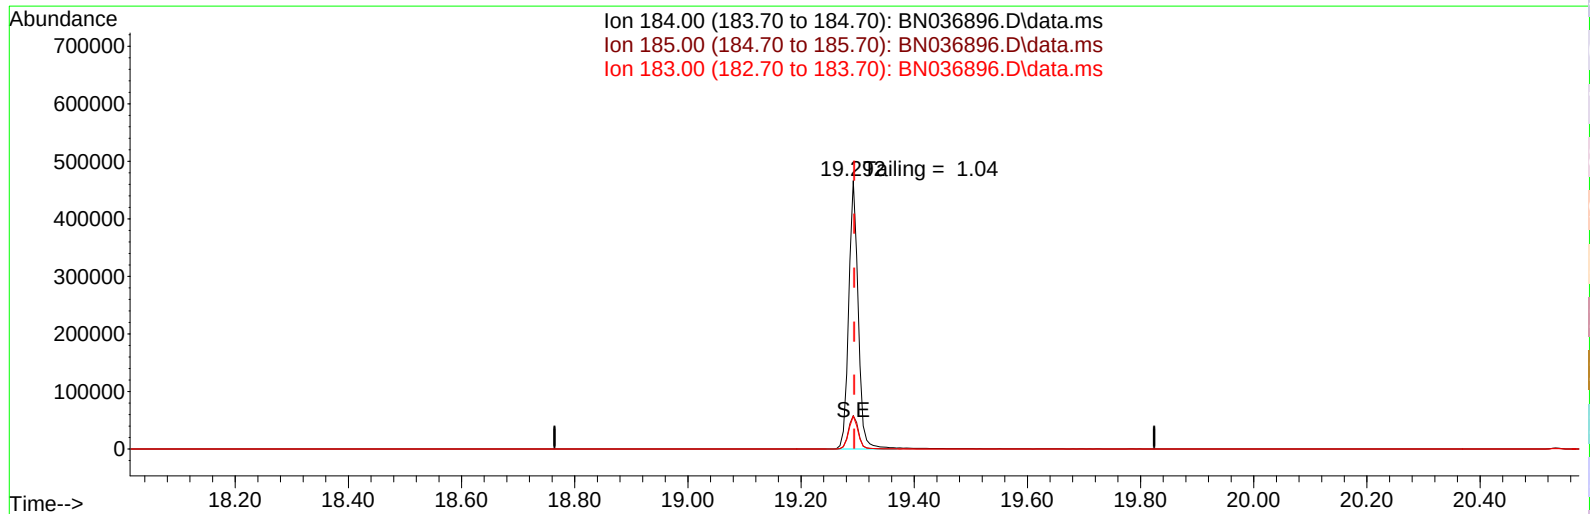

TIC: BN036896.D\data.ms

(77) Benzidine

19.292min (-0.002) 0.00 ng

response 549129

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.46
183.00	13.20	12.25
0.00	0.00	0.00

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	PB167519BL	SDG No.:	Q1741
Lab Sample ID:	PB167519BL	Matrix:	Water
Analytical Method:	SW8270ESIM	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	SVOC-SIMGroup1
Extraction Type :	Decanted : N	Level :	LOW
Injection Volume :	GPC Factor : 1.0	GPC Cleanup :	N PH :
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN036906.D	1	04/08/25 10:10	04/14/25 18:51	PB167519

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
123-91-1	1,4-Dioxane	0.070	U	0.070	0.20	ug/L
SURROGATES						
7297-45-2	2-Methylnaphthalene-d10	0.34		30 (20) - 150 (139)	85%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.35		30 (30) - 150 (150)	88%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.32		30 (27) - 130 (154)	80%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.37		30 (25) - 130 (149)	93%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.42		30 (54) - 130 (175)	104%	SPK: 0.4
INTERNAL STANDARDS						
3855-82-1	1,4-Dichlorobenzene-d4	1900	7.633			
1146-65-2	Naphthalene-d8	4410	10.415			
15067-26-2	Acenaphthene-d10	2280	14.277			
1517-22-2	Phenanthrene-d10	4450	17.034			
1719-03-5	Chrysene-d12	3070	21.225			
1520-96-3	Perylene-d12	1380	23.436			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036906.D
Acq On : 14 Apr 2025 18:51
Operator : RC/JU
Sample : PB167519BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB167519BL

Quant Time: Apr 15 01:03:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:58:02 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	1898	0.400	ng	0.00
7) Naphthalene-d8	10.415	136	4409	0.400	ng	0.00
13) Acenaphthene-d10	14.277	164	2284	0.400	ng	0.00
19) Phenanthrene-d10	17.034	188	4447	0.400	ng	0.00
29) Chrysene-d12	21.225	240	3070	0.400	ng	# 0.00
35) Perylene-d12	23.436	264	1383	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.228	112	1805	0.402	ng	0.00
5) Phenol-d6	6.809	99	2050	0.364	ng	0.00
8) Nitrobenzene-d5	8.782	82	1600	0.321	ng	0.00
11) 2-Methylnaphthalene-d10	12.016	152	2179	0.339	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	398	0.363	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	4107	0.373	ng	0.00
27) Fluoranthene-d10	19.063	212	4134	0.351	ng	0.00
31) Terphenyl-d14	19.672	244	2797	0.416	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036906.D
Acq On : 14 Apr 2025 18:51
Operator : RC/JU
Sample : PB167519BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB167519BL

Quant Time: Apr 15 01:03:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 14 17:58:02 2025
Response via : Initial Calibration




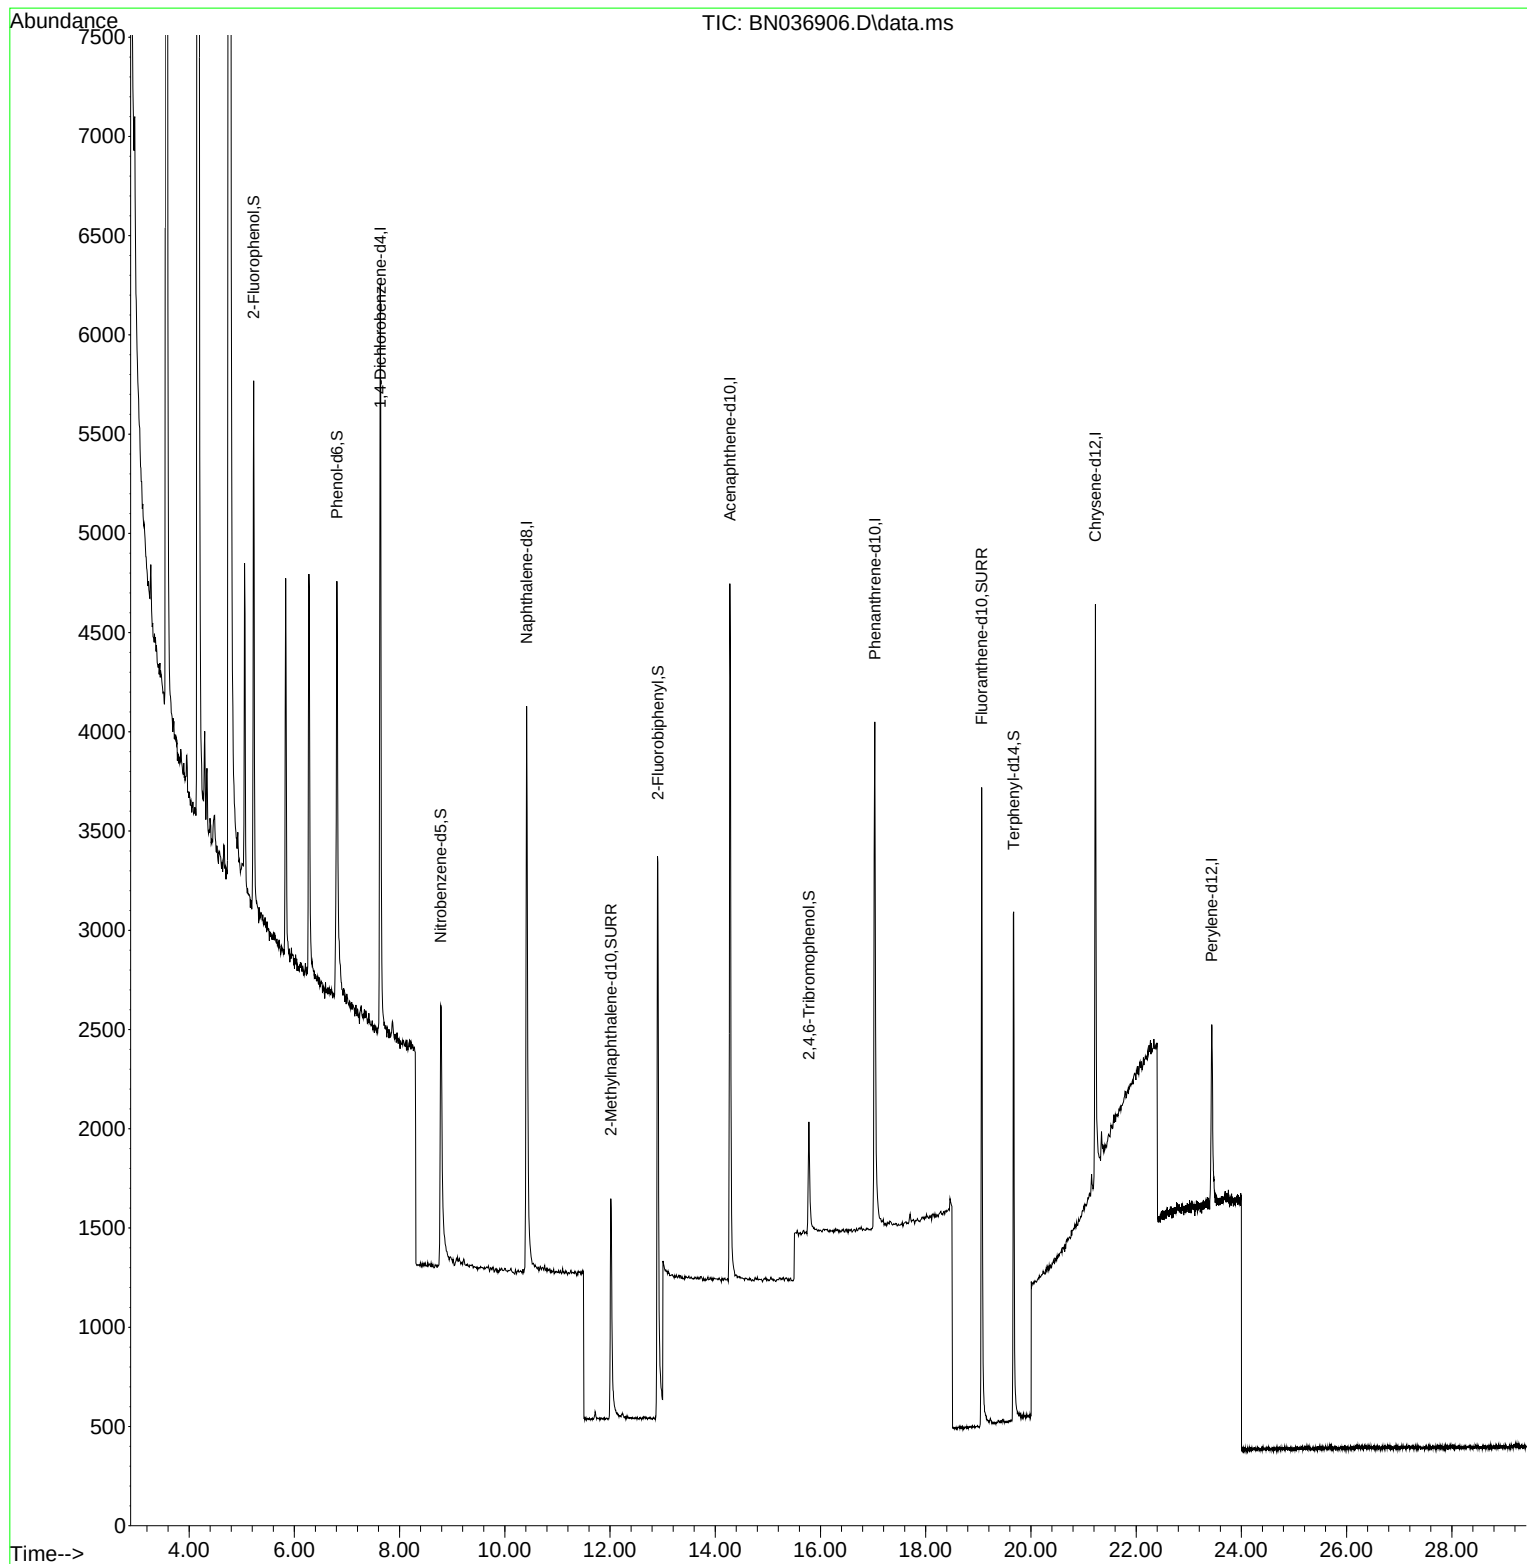




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51




Instrument :
BNA_N
ClientSampleId :
PB167519BL


Tgt Ion:152 Resp: 1898
Ion Ratio Lower Upper
152 100
150 155.1 121.4 182.2
115 68.9 55.4 83.2



#4
2-Fluorophenol
Concen: 0.402 ng
RT: 5.228 min Scan# 325
Delta R.T. 0.000 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51

Tgt Ion:112 Resp: 1805
Ion Ratio Lower Upper
112 100
64 66.7 54.4 81.6
63 42.9 35.1 52.7









#5
Phenol-d6
Concen: 0.364 ng
RT: 6.809 min Scan# 544
Delta R.T. 0.000 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51




Instrument :
BNA_N
ClientSampleId :
PB167519BL


Tgt Ion:	99	Resp:	2050
Ion	Ratio	Lower	Upper
99	100		
42	35.9	30.6	45.8
71	47.9	38.0	57.0

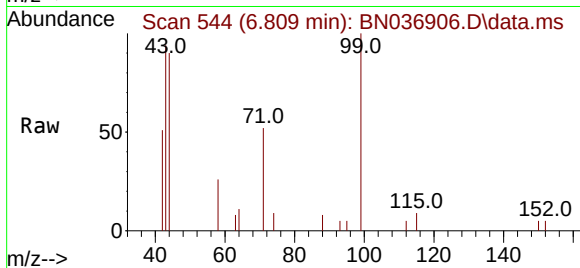

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.415 min Scan# 949
Delta R.T. 0.000 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51

Tgt Ion:	136	Resp:	4409
Ion	Ratio	Lower	Upper
136	100		
137	13.1	10.6	15.8
54	14.7	10.6	16.0
68	8.4	6.1	9.1









#8
Nitrobenzene-d5
Concen: 0.321 ng
RT: 8.782 min Scan# 796
Delta R.T. 0.000 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51




Instrument :
BNA_N
ClientSampleId :
PB167519BL


Tgt Ion:	82	Resp:	1600
Ion	Ratio	Lower	Upper
82	100		
128	34.8	29.0	43.4
54	76.1	60.8	91.2



#11
2-Methylnaphthalene-d10
Concen: 0.339 ng
RT: 12.016 min Scan# 1152
Delta R.T. 0.005 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51

Tgt Ion:	152	Resp:	2179
Ion	Ratio	Lower	Upper
152	100		
151	21.6	17.1	25.7









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.277 min Scan# 1466
Delta R.T. 0.000 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51




Instrument :
BNA_N
ClientSampleId :
PB167519BL


Tgt Ion:164 Resp: 2284
Ion Ratio Lower Upper
164 100
162 107.9 83.8 125.8
160 57.7 44.7 67.1



#14
2,4,6-Tribromophenol
Concen: 0.363 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51

Tgt Ion:330 Resp: 398
Ion Ratio Lower Upper
330 100
332 95.0 77.0 115.6
141 53.8 44.5 66.7









#15
2-Fluorobiphenyl
Concen: 0.373 ng
RT: 12.909 min Scan# 11
Delta R.T. 0.005 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51




Instrument :
BNA_N
ClientSampleId :
PB167519BL


Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.1	29.2	43.8
170	25.9	20.5	30.7



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.034 min Scan# 1704
Delta R.T. 0.000 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	10.6	7.1	10.7





#27

Fluoranthene-d10

Concen: 0.351 ng

RT: 19.063 min Scan# 1942

Delta R.T. 0.000 min

Lab File: BN036906.D

Acq: 14 Apr 2025 18:51

Instrument :

BNA_N

ClientSampleId :

PB167519BL





Tgt Ion:212 Resp: 4134

Ion Ratio Lower Upper

212 100

106 13.0 10.6 15.8

104 8.1 6.6 10.0

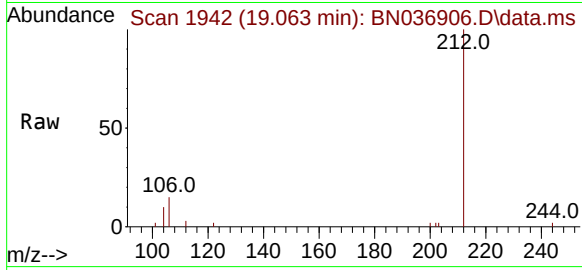

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.225 min Scan# 2281

Delta R.T. 0.000 min

Lab File: BN036906.D

Acq: 14 Apr 2025 18:51




Tgt Ion:240 Resp: 3070


Ion Ratio Lower Upper

240 100

120 15.4 9.8 14.6#

236 30.5 23.1 34.7









#31
Terphenyl-d14
Concen: 0.416 ng
RT: 19.672 min Scan# 2073
Delta R.T. 0.005 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51




Instrument :
BNA_N
ClientSampleId :
PB167519BL

Tgt Ion:244 Resp: 2797
Ion Ratio Lower Upper
244 100
212 12.8 10.1 15.1
122 17.3 13.6 20.4



#35
Perylene-d12
Concen: 0.400 ng
RT: 23.436 min Scan# 2765
Delta R.T. 0.003 min
Lab File: BN036906.D
Acq: 14 Apr 2025 18:51

Tgt Ion:264 Resp: 1383
Ion Ratio Lower Upper
264 100
260 31.9 22.3 33.5
265 156.7 57.6 86.4#



Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	PB167519BS	SDG No.:	Q1741
Lab Sample ID:	PB167519BS	Matrix:	Water
Analytical Method:	SW8270ESIM	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	SVOC-SIMGroup1
Extraction Type :	Decanted : N	Level :	LOW
Injection Volume :	GPC Factor : 1.0	GPC Cleanup :	N PH :
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN036893.D	1	04/08/25 10:10	04/12/25 00:09	PB167519

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
123-91-1	1,4-Dioxane	0.34		0.070	0.20	ug/L
SURROGATES						
7297-45-2	2-Methylnaphthalene-d10	0.39		30 (20) - 150 (139)	98%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.41		30 (30) - 150 (150)	101%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.36		30 (27) - 130 (154)	90%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.39		30 (25) - 130 (149)	97%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.37		30 (54) - 130 (175)	94%	SPK: 0.4
INTERNAL STANDARDS						
3855-82-1	1,4-Dichlorobenzene-d4	385	7.64			
1146-65-2	Naphthalene-d8	924	10.426			
15067-26-2	Acenaphthene-d10	537	14.288			
1517-22-2	Phenanthrene-d10	1270	17.034			
1719-03-5	Chrysene-d12	1510	21.224			
1520-96-3	Perylene-d12	1790	23.445			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036893.D
 Acq On : 12 Apr 2025 00:09
 Operator : RC/JU
 Sample : PB167519BS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB167519BS

Quant Time: Apr 12 01:02:00 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 16:11:08 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	385	0.400	ng	0.00
7) Naphthalene-d8	10.426	136	924	0.400	ng	0.00
13) Acenaphthene-d10	14.288	164	537	0.400	ng	0.00
19) Phenanthrene-d10	17.034	188	1271	0.400	ng	0.00
29) Chrysene-d12	21.224	240	1512	0.400	ng	0.00
35) Perylene-d12	23.445	264	1791	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.235	112	407	0.449	ng	0.00
5) Phenol-d6	6.817	99	472	0.408	ng	0.00
8) Nitrobenzene-d5	8.792	82	368	0.359	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	529m	0.394	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	109	0.421	ng	0.00
15) 2-Fluorobiphenyl	12.909	172	995	0.386	ng	0.00
27) Fluoranthene-d10	19.073	212	1452	0.406	ng	0.00
31) Terphenyl-d14	19.677	244	1073	0.374	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.148	88	153	0.343	ng	# 4
3) n-Nitrosodimethylamine	3.466	42	397	0.401	ng	# 97
6) bis(2-Chloroethyl)ether	7.069	93	400	0.352	ng	89
9) Naphthalene	10.468	128	1047	0.394	ng	95
10) Hexachlorobutadiene	10.767	225	244	0.405	ng	# 94
12) 2-Methylnaphthalene	12.092	142	665	0.389	ng	95
16) Acenaphthylene	13.999	152	1080	0.433	ng	98
17) Acenaphthene	14.352	154	683	0.420	ng	95
18) Fluorene	15.336	166	926	0.413	ng	98
20) 4,6-Dinitro-2-methylph...	15.432	198	106	0.352	ng	90
21) 4-Bromophenyl-phenylether	16.239	248	306	0.402	ng	96
22) Hexachlorobenzene	16.351	284	326	0.362	ng	95
23) Atrazine	16.512	200	336	0.451	ng	92
24) Pentachlorophenol	16.686	266	255	0.540	ng	94
25) Phenanthrene	17.071	178	1640	0.430	ng	98
26) Anthracene	17.170	178	1442	0.424	ng	99
28) Fluoranthene	19.101	202	2078	0.433	ng	99
30) Pyrene	19.463	202	2228	0.390	ng	100
32) Benzo(a)anthracene	21.216	228	2203	0.412	ng	99
33) Chrysene	21.260	228	2419	0.411	ng	98
34) Bis(2-ethylhexyl)phtha...	21.153	149	1579	0.398	ng	99
36) Indeno(1,2,3-cd)pyrene	25.675	276	3583	0.419	ng	98
37) Benzo(b)fluoranthene	22.781	252	2550	0.401	ng	100
38) Benzo(k)fluoranthene	22.825	252	2836m	0.442	ng	
39) Benzo(a)pyrene	23.348	252	2486	0.446	ng	95
40) Dibenzo(a,h)anthracene	25.690	278	2821	0.416	ng	99
41) Benzo(g,h,i)perylene	26.354	276	2977	0.388	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036893.D
Acq On : 12 Apr 2025 00:09
Operator : RC/JU
Sample : PB167519BS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB167519BS

Quant Time: Apr 12 01:02:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration




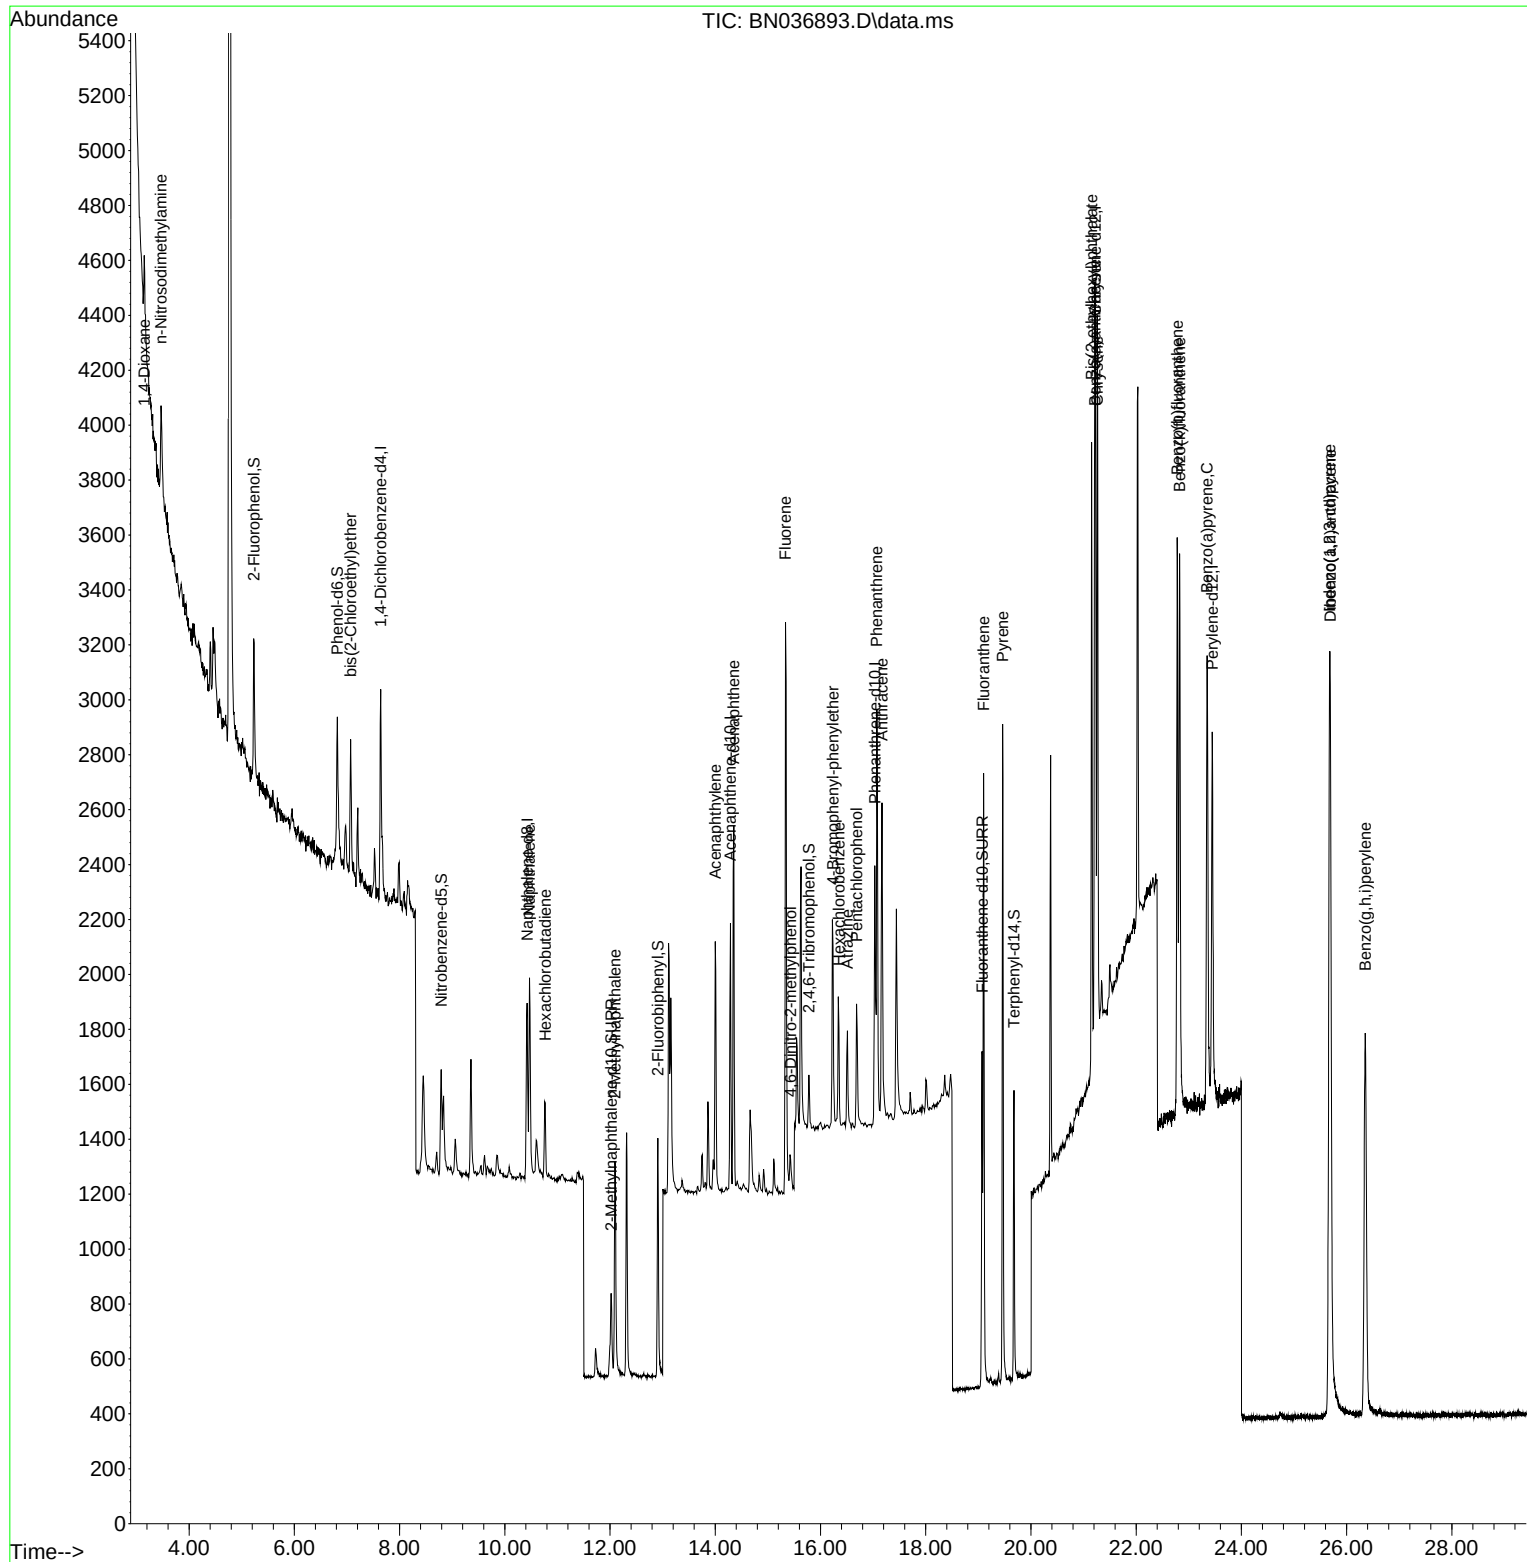




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.640 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN036893.D
 Acq: 12 Apr 2025 00:09




Instrument :
 BNA_N
 ClientSampleId :
 PB167519BS


Tgt Ion:152 Resp: 385
 Ion Ratio Lower Upper
 152 100
 150 138.1 123.0 184.6
 115 76.6 60.1 90.1



#2
 1,4-Dioxane
 Concen: 0.343 ng
 RT: 3.148 min Scan# 37
 Delta R.T. -0.007 min
 Lab File: BN036893.D
 Acq: 12 Apr 2025 00:09

Tgt Ion: 88 Resp: 153
 Ion Ratio Lower Upper
 88 100
 43 0.0 39.2 58.8#
 58 177.1 63.5 95.3#









#3
n-Nitrosodimethylamine
Concen: 0.401 ng
RT: 3.466 min Scan# 81
Delta R.T. -0.007 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion: 42 Resp: 397
Ion Ratio Lower Upper
42 100
74 70.8 54.6 81.8
44 8.3 0.0 0.0#



#4
2-Fluorophenol
Concen: 0.449 ng
RT: 5.235 min Scan# 326
Delta R.T. 0.007 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion: 112 Resp: 407
Ion Ratio Lower Upper
112 100
64 67.1 54.0 81.0
63 44.0 35.1 52.7









#5
Phenol-d6
Concen: 0.408 ng
RT: 6.817 min Scan# 545
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion: 99 Resp: 472
Ion Ratio Lower Upper
99 100
42 46.0 30.9 46.3
71 47.5 38.6 58.0



#6
bis(2-Chloroethyl)ether
Concen: 0.352 ng
RT: 7.069 min Scan# 580
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion: 93 Resp: 400
Ion Ratio Lower Upper
93 100
63 82.0 76.4 114.6
95 31.5 26.1 39.1


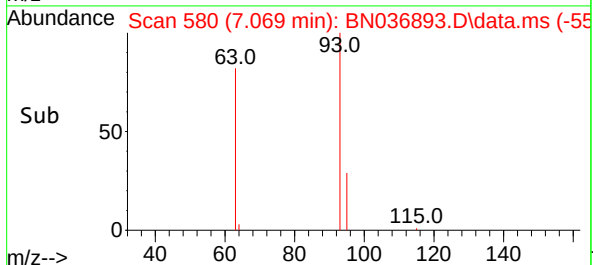






#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:	136	Resp:	924
Ion	Ratio	Lower	Upper
136	100		
137	20.2	13.5	20.3
54	18.0	12.8	19.2
68	13.1	10.1	15.1



#8
Nitrobenzene-d5
Concen: 0.359 ng
RT: 8.792 min Scan# 797
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:	82	Resp:	368
Ion	Ratio	Lower	Upper
82	100		
128	50.7	35.5	53.3
54	75.3	56.2	84.4









#9
Naphthalene
Concen: 0.394 ng
RT: 10.468 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:	128	Resp:	1047
Ion	Ratio	Lower	Upper
128	100		
129	18.4	12.9	19.3
127	21.0	15.0	22.6



#10
Hexachlorobutadiene
Concen: 0.405 ng
RT: 10.767 min Scan# 982
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:	225	Resp:	244
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	58.2	50.5	75.7









#11
2-Methylnaphthalene-d10
Concen: 0.394 ng m
RT: 12.021 min Scan# 1153
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:152 Resp: 529
Ion Ratio Lower Upper
152 100
151 20.8 17.8 26.8



#12
2-Methylnaphthalene
Concen: 0.389 ng
RT: 12.092 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:142 Resp: 665
Ion Ratio Lower Upper
142 100
141 89.8 73.8 110.8
115 60.1 43.3 64.9









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion	Ratio	Lower	Upper
164	100		
162	102.9	85.7	128.5
160	60.2	46.9	70.3

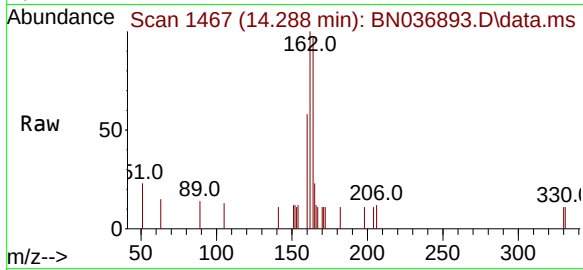

#14
2,4,6-Tribromophenol
Concen: 0.421 ng
RT: 15.780 min Scan# 1603
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion	Ratio	Lower	Upper
330	100		
332	108.3	87.0	130.6
141	53.2	45.3	67.9




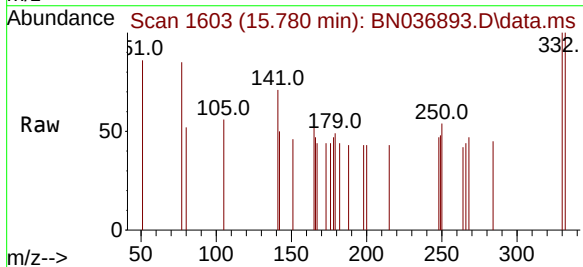




#15
2-Fluorobiphenyl
Concen: 0.386 ng
RT: 12.909 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:	172	Resp:	995
Ion	Ratio	Lower	Upper
172	100		
171	41.7	32.7	49.1
170	30.1	23.3	34.9



#16
Acenaphthylene
Concen: 0.433 ng
RT: 13.999 min Scan# 1440
Delta R.T. -0.011 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:	152	Resp:	1080
Ion	Ratio	Lower	Upper
152	100		
151	19.7	16.4	24.6
153	13.8	10.3	15.5









#17
Acenaphthene
Concen: 0.420 ng
RT: 14.352 min Scan# 1473
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:	154	Resp:	683
Ion Ratio	Lower	Upper	
154	100		
153	116.1	97.8	146.6
152	61.9	52.7	79.1



#18
Fluorene
Concen: 0.413 ng
RT: 15.336 min Scan# 1565
Delta R.T. -0.011 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:	166	Resp:	926
Ion Ratio	Lower	Upper	
166	100		
165	101.2	83.2	124.8
167	13.9	11.1	16.7

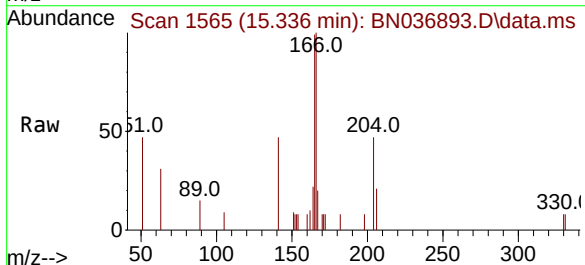

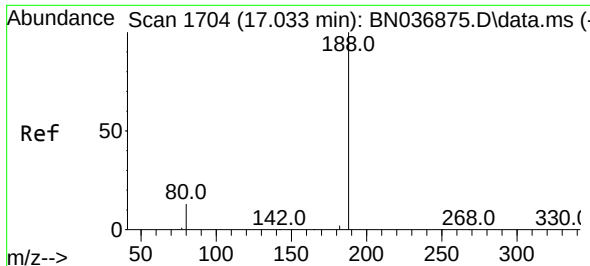

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.034 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN036893.D

Acq: 12 Apr 2025 00:09

Instrument :

BNA_N

ClientSampleId :

PB167519BS





Tgt Ion:188 Resp: 1271

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 15.7 13.9 20.9



#20

4,6-Dinitro-2-methylphenol

Concen: 0.352 ng

RT: 15.432 min Scan# 1574

Delta R.T. 0.000 min

Lab File: BN036893.D

Acq: 12 Apr 2025 00:09




Tgt Ion:198 Resp: 106


Ion Ratio Lower Upper

198 100

51 126.1 107.6 161.4

105 81.5 55.2 82.8









#21
4-Bromophenyl-phenylether
Concen: 0.402 ng
RT: 16.239 min Scan# 1640
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:	248	Resp:	306
Ion	Ratio	Lower	Upper
248	100		
250	100.0	83.5	125.3
141	65.2	55.3	82.9



#22
Hexachlorobenzene
Concen: 0.362 ng
RT: 16.351 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:	284	Resp:	326
Ion	Ratio	Lower	Upper
284	100		
142	52.1	37.7	56.5
249	37.4	29.0	43.6









#23
Atrazine
Concen: 0.451 ng
RT: 16.512 min Scan# 1662
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion	Ratio	Lower	Upper
200	100		
173	40.4	28.6	43.0
215	56.1	40.5	60.7

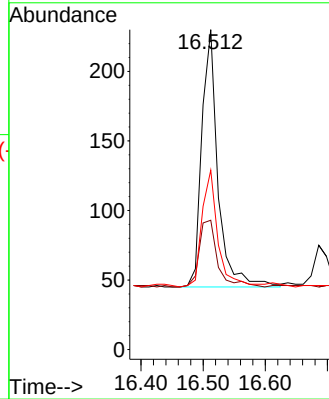

#24
Pentachlorophenol
Concen: 0.540 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.012 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion	Ratio	Lower	Upper
266	100		
264	61.2	44.6	66.8
268	60.8	51.8	77.6









#25
Phenanthrene
Concen: 0.430 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.012 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:	178	Resp:	1640
Ion	Ratio	Lower	Upper
178	100		
176	19.3	16.6	25.0
179	15.7	12.8	19.2



#26
Anthracene
Concen: 0.424 ng
RT: 17.170 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:	178	Resp:	1442
Ion	Ratio	Lower	Upper
178	100		
176	19.3	15.8	23.6
179	16.0	12.6	18.8









#27
Fluoranthene-d10
Concen: 0.406 ng
RT: 19.073 min Scan# 1944
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion	Ratio	Lower	Upper
212	100		
106	13.8	11.2	16.8
104	8.3	7.5	11.3

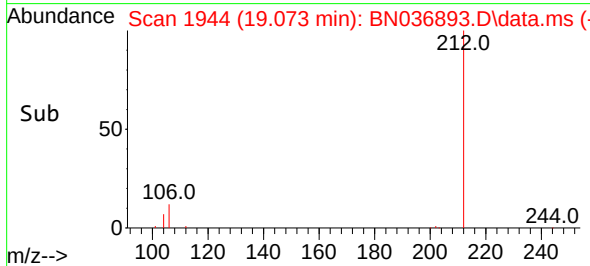

#28
Fluoranthene
Concen: 0.433 ng
RT: 19.101 min Scan# 1950
Delta R.T. -0.005 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.3	8.5	12.7
203	17.5	13.8	20.6









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.224 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:240 Resp: 1512
Ion Ratio Lower Upper
240 100
120 22.4 15.8 23.6
236 31.2 25.8 38.8

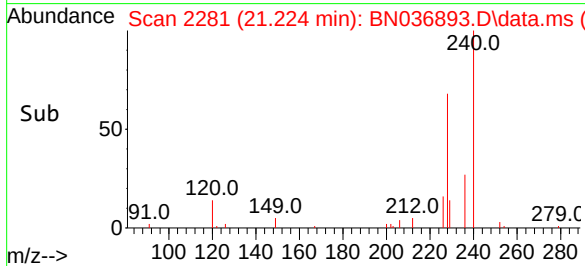

#30
Pyrene
Concen: 0.390 ng
RT: 19.463 min Scan# 2028
Delta R.T. -0.005 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:202 Resp: 2228
Ion Ratio Lower Upper
202 100
200 21.4 17.1 25.7
203 18.0 14.5 21.7









#31
Terphenyl-d14
Concen: 0.374 ng
RT: 19.677 min Scan# 2074
Delta R.T. -0.005 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:244 Resp: 1073
Ion Ratio Lower Upper
244 100
212 16.0 11.6 17.4
122 19.7 14.9 22.3

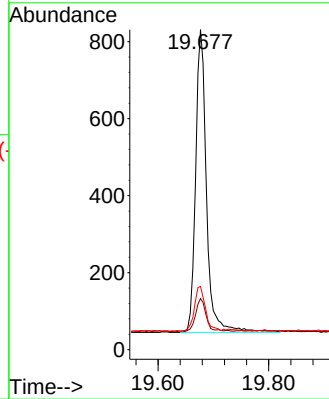

#32
Benzo(a)anthracene
Concen: 0.412 ng
RT: 21.216 min Scan# 2280
Delta R.T. 0.000 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:228 Resp: 2203
Ion Ratio Lower Upper
228 100
226 29.5 24.5 36.7
229 22.0 17.7 26.5





#33

Chrysene

Concen: 0.411 ng

RT: 21.260 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN036893.D

Acq: 12 Apr 2025 00:09

Instrument :

BNA_N

ClientSampleId :

PB167519BS





Tgt Ion:228 Resp: 2419

Ion Ratio Lower Upper

228 100

226 34.2 26.1 39.1

229 21.2 17.0 25.4

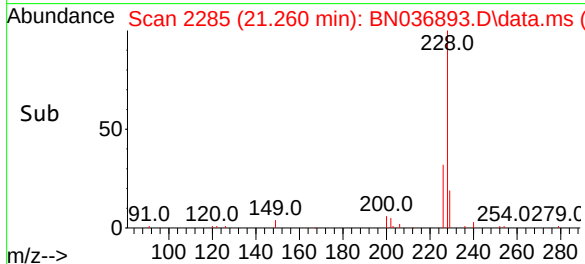

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.398 ng

RT: 21.153 min Scan# 2273

Delta R.T. -0.009 min

Lab File: BN036893.D

Acq: 12 Apr 2025 00:09




Tgt Ion:149 Resp: 1579


Ion Ratio Lower Upper

149 100

167 25.8 21.0 31.4

279 4.2 3.6 5.4









#35
Perylene-d12
Concen: 0.400 ng
RT: 23.445 min Scan# 21
Delta R.T. -0.012 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:264 Resp: 1791
Ion Ratio Lower Upper
264 100
260 29.4 22.9 34.3
265 103.4 88.6 132.8



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.419 ng
RT: 25.675 min Scan# 3531
Delta R.T. -0.012 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:276 Resp: 3583
Ion Ratio Lower Upper
276 100
138 27.1 21.0 31.6
277 25.1 19.3 28.9









#37
Benzo(b)fluoranthene
Concen: 0.401 ng
RT: 22.781 min Scan# 2541
Delta R.T. -0.009 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09




Instrument :
BNA_N
ClientSampleId :
PB167519BS


Tgt Ion:252 Resp: 2550
Ion Ratio Lower Upper
252 100
253 33.8 27.0 40.6
125 21.6 17.7 26.5



#38
Benzo(k)fluoranthene
Concen: 0.442 ng m
RT: 22.825 min Scan# 2556
Delta R.T. -0.009 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Tgt Ion:252 Resp: 2836
Ion Ratio Lower Upper
252 100
253 32.0 26.7 40.1
125 20.1 16.9 25.3





#39

Benzo(a)pyrene

Concen: 0.446 ng

RT: 23.348 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN036893.D

Acq: 12 Apr 2025 00:09

Instrument :

BNA_N

ClientSampleId :

PB167519BS





Tgt Ion:252 Resp: 2486

Ion Ratio Lower Upper

252 100

253 36.9 31.5 47.3

125 25.2 22.6 34.0



#40

Dibenzo(a,h)anthracene

Concen: 0.416 ng

RT: 25.690 min Scan# 3536

Delta R.T. -0.012 min

Lab File: BN036893.D

Acq: 12 Apr 2025 00:09




Tgt Ion:278 Resp: 2821


Ion Ratio Lower Upper

278 100

139 22.1 17.6 26.4


279 34.7 26.7 40.1







#41
Benzo(g,h,i)perylene
Concen: 0.388 ng
RT: 26.354 min Scan# 31
Delta R.T. -0.009 min
Lab File: BN036893.D
Acq: 12 Apr 2025 00:09

Instrument :
BNA_N
ClientSampleId :
PB167519BS



Tgt Ion:276 Resp: 2977
Ion Ratio Lower Upper
276 100
277 28.2 21.8 32.8
138 28.1 21.6 32.4



Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	PB167519BSD	SDG No.:	Q1741
Lab Sample ID:	PB167519BSD	Matrix:	Water
Analytical Method:	SW8270ESIM	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	SVOC-SIMGroup1
Extraction Type :	Decanted : N	Level :	LOW
Injection Volume :	GPC Factor : 1.0	GPC Cleanup :	N PH :
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN036894.D	1	04/08/25 10:10	04/12/25 00:45	PB167519

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
123-91-1	1,4-Dioxane	0.39		0.070	0.20	ug/L
SURROGATES						
7297-45-2	2-Methylnaphthalene-d10	0.40		30 (20) - 150 (139)	100%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.42		30 (30) - 150 (150)	105%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.34		30 (27) - 130 (154)	86%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.40		30 (25) - 130 (149)	101%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.38		30 (54) - 130 (175)	96%	SPK: 0.4
INTERNAL STANDARDS						
3855-82-1	1,4-Dichlorobenzene-d4	195	7.64			
1146-65-2	Naphthalene-d8	480	10.426			
15067-26-2	Acenaphthene-d10	292	14.288			
1517-22-2	Phenanthrene-d10	662	17.033			
1719-03-5	Chrysene-d12	805	21.224			
1520-96-3	Perylene-d12	1050	23.444			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
 Data File : BN036894.D
 Acq On : 12 Apr 2025 00:45
 Operator : RC/JU
 Sample : PB167519BSD
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB167519BSD

Quant Time: Apr 12 01:46:12 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 11 16:11:08 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	195	0.400	ng	# 0.00
7) Naphthalene-d8	10.426	136	480	0.400	ng	# 0.00
13) Acenaphthene-d10	14.288	164	292	0.400	ng	0.00
19) Phenanthrene-d10	17.033	188	662	0.400	ng	# 0.00
29) Chrysene-d12	21.224	240	805	0.400	ng	# 0.00
35) Perylene-d12	23.444	264	1051	0.400	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.235	112	226	0.493	ng	0.00
5) Phenol-d6	6.817	99	276	0.471	ng	0.00
8) Nitrobenzene-d5	8.792	82	183	0.343	ng	0.00
11) 2-Methylnaphthalene-d10	12.021	152	280m	0.401	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	54	0.384	ng	0.00
15) 2-Fluorobiphenyl	12.914	172	565	0.403	ng	0.00
27) Fluoranthene-d10	19.073	212	784	0.420	ng	0.00
31) Terphenyl-d14	19.676	244	587	0.384	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.148	88	88	0.389	ng	# 28
3) n-Nitrosodimethylamine	3.473	42	225	0.449	ng	# 84
6) bis(2-Chloroethyl)ether	7.069	93	223	0.388	ng	88
9) Naphthalene	10.468	128	576	0.417	ng	# 84
10) Hexachlorobutadiene	10.767	225	131	0.418	ng	# 100
12) 2-Methylnaphthalene	12.097	142	351	0.395	ng	# 93
16) Acenaphthylene	14.010	152	588	0.433	ng	97
17) Acenaphthene	14.352	154	369	0.418	ng	97
18) Fluorene	15.346	166	520	0.427	ng	92
20) 4,6-Dinitro-2-methylph...	15.432	198	51	0.325	ng	# 71
21) 4-Bromophenyl-phenylether	16.239	248	172	0.434	ng	95
22) Hexachlorobenzene	16.351	284	192	0.409	ng	91
23) Atrazine	16.512	200	200	0.516	ng	# 80
24) Pentachlorophenol	16.686	266	139	0.565	ng	# 90
25) Phenanthrene	17.071	178	880	0.443	ng	98
26) Anthracene	17.170	178	854	0.483	ng	98
28) Fluoranthene	19.100	202	1116	0.447	ng	98
30) Pyrene	19.467	202	1210	0.398	ng	99
32) Benzo(a)anthracene	21.215	228	1228	0.432	ng	99
33) Chrysene	21.260	228	1417	0.452	ng	96
34) Bis(2-ethylhexyl)phtha...	21.153	149	958	0.454	ng	99
36) Indeno(1,2,3-cd)pyrene	25.672	276	2458	0.490	ng	98
37) Benzo(b)fluoranthene	22.781	252	1513	0.406	ng	92
38) Benzo(k)fluoranthene	22.825	252	1692m	0.450	ng	
39) Benzo(a)pyrene	23.348	252	1529	0.468	ng	91
40) Dibenzo(a,h)anthracene	25.690	278	1912	0.480	ng	92
41) Benzo(g,h,i)perylene	26.356	276	2001	0.444	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036894.D
Acq On : 12 Apr 2025 00:45
Operator : RC/JU
Sample : PB167519BSD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB167519BSD

Quant Time: Apr 12 01:46:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 16:11:08 2025
Response via : Initial Calibration




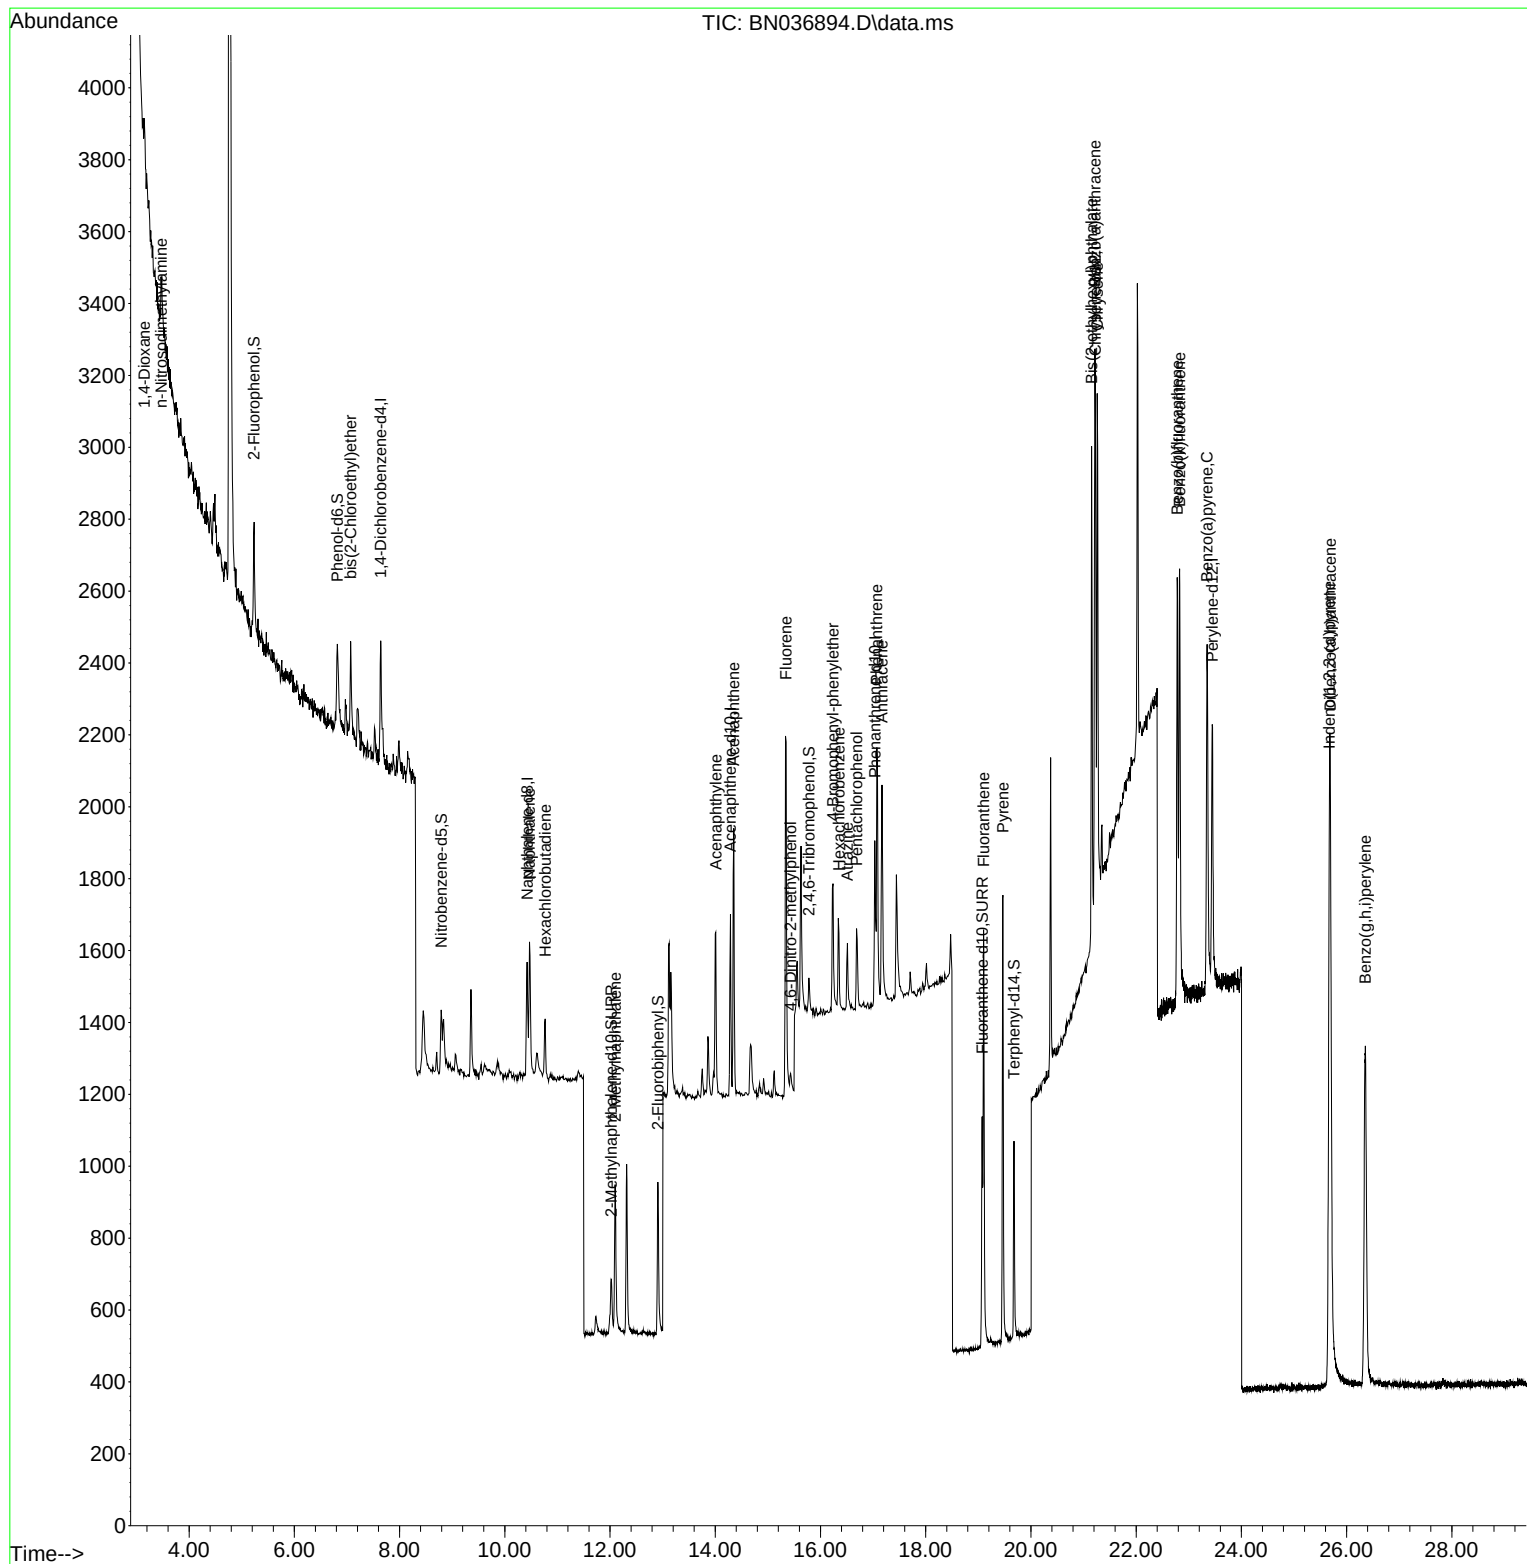




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.640 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:152 Resp: 195
Ion Ratio Lower Upper
152 100
150 137.6 123.0 184.6
115 91.3 60.1 90.1#



#2
1,4-Dioxane
Concen: 0.389 ng
RT: 3.148 min Scan# 37
Delta R.T. -0.007 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion: 88 Resp: 88
Ion Ratio Lower Upper
88 100
43 0.0 39.2 58.8#
58 142.0 63.5 95.3#









#3
n-Nitrosodimethylamine
Concen: 0.449 ng
RT: 3.473 min Scan# 81
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion: 42 Resp: 225
Ion Ratio Lower Upper
42 100
74 55.6 54.6 81.8
44 6.7 0.0 0.0#

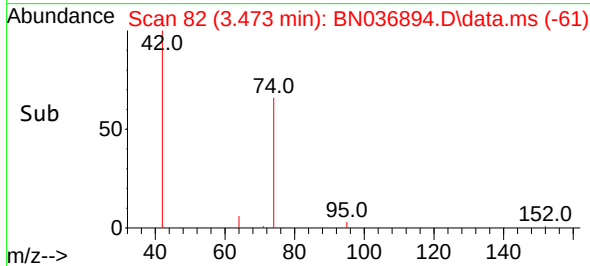

#4
2-Fluorophenol
Concen: 0.493 ng
RT: 5.235 min Scan# 326
Delta R.T. 0.007 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion: 112 Resp: 226
Ion Ratio Lower Upper
112 100
64 70.4 54.0 81.0
63 55.3 35.1 52.7#









#5
Phenol-d6
Concen: 0.471 ng
RT: 6.817 min Scan# 545
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion: 99 Resp: 276
Ion Ratio Lower Upper
99 100
42 39.9 30.9 46.3
71 46.0 38.6 58.0

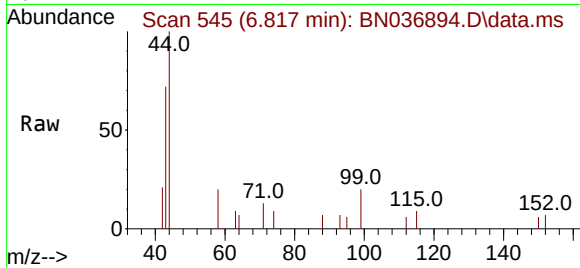

#6
bis(2-Chloroethyl)ether
Concen: 0.388 ng
RT: 7.069 min Scan# 580
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion: 93 Resp: 223
Ion Ratio Lower Upper
93 100
63 83.0 76.4 114.6
95 38.1 26.1 39.1


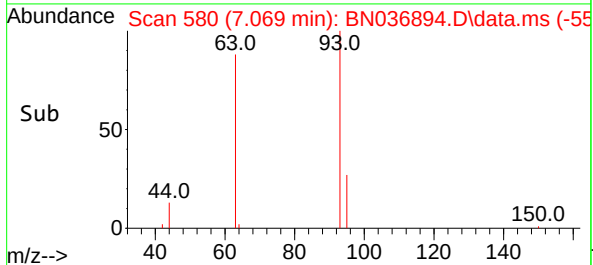






#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.426 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:	136	Resp:	480
Ion	Ratio	Lower	Upper
136	100		
137	25.4	13.5	20.3#
54	25.4	12.8	19.2#
68	20.9	10.1	15.1#



#8
Nitrobenzene-d5
Concen: 0.343 ng
RT: 8.792 min Scan# 797
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:	82	Resp:	183
Ion	Ratio	Lower	Upper
82	100		
128	59.5	35.5	53.3#
54	84.1	56.2	84.4




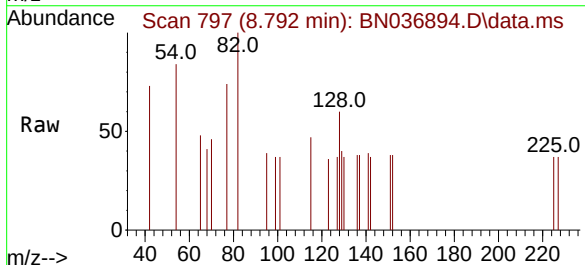




#9
Naphthalene
Concen: 0.417 ng
RT: 10.468 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:	128	Resp:	576
Ion	Ratio	Lower	Upper
128	100		
129	23.9	12.9	19.3#
127	25.2	15.0	22.6#



#10
Hexachlorobutadiene
Concen: 0.418 ng
RT: 10.767 min Scan# 982
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:	225	Resp:	131
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.4	50.5	75.7


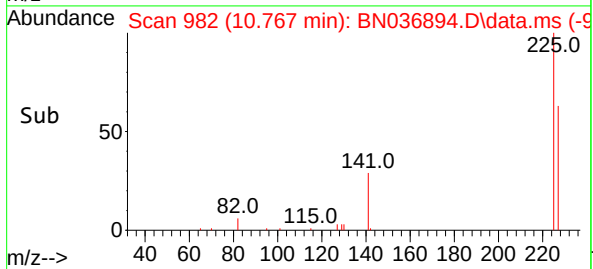






#11
2-Methylnaphthalene-d10
Concen: 0.401 ng m
RT: 12.021 min Scan# 1153
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:152 Resp: 280
Ion Ratio Lower Upper
152 100
151 22.9 17.8 26.8



#12
2-Methylnaphthalene
Concen: 0.395 ng
RT: 12.097 min Scan# 1168
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:142 Resp: 351
Ion Ratio Lower Upper
142 100
141 90.8 73.8 110.8
115 66.5 43.3 64.9#


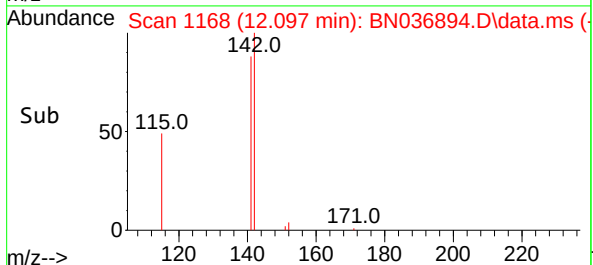
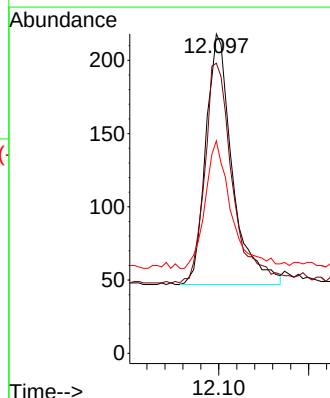





#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.288 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:164 Resp: 292
Ion Ratio Lower Upper
164 100
162 103.0 85.7 128.5
160 62.0 46.9 70.3

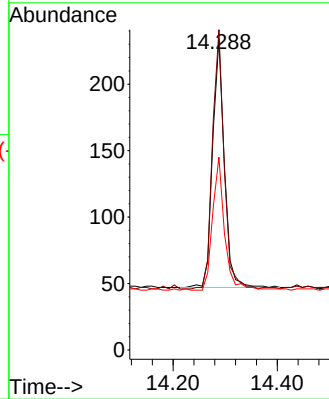

#14
2,4,6-Tribromophenol
Concen: 0.384 ng
RT: 15.780 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:330 Resp: 54
Ion Ratio Lower Upper
330 100
332 94.4 87.0 130.6
141 74.1 45.3 67.9#









#15
2-Fluorobiphenyl
Concen: 0.403 ng
RT: 12.914 min Scan# 1329
Delta R.T. 0.005 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:	172	Resp:	565
Ion	Ratio	Lower	Upper
172	100		
171	42.0	32.7	49.1
170	33.6	23.3	34.9



#16
Acenaphthylene
Concen: 0.433 ng
RT: 14.010 min Scan# 1441
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:	152	Resp:	588
Ion	Ratio	Lower	Upper
152	100		
151	21.8	16.4	24.6
153	13.8	10.3	15.5


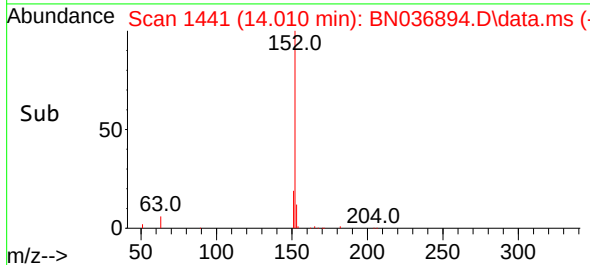






#17
Acenaphthene
Concen: 0.418 ng
RT: 14.352 min Scan# 1473
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:154 Resp: 369
Ion Ratio Lower Upper
154 100
153 118.4 97.8 146.6
152 66.7 52.7 79.1



#18
Fluorene
Concen: 0.427 ng
RT: 15.346 min Scan# 1566
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:166 Resp: 520
Ion Ratio Lower Upper
166 100
165 94.8 83.2 124.8
167 14.2 11.1 16.7









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.033 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	21.2	13.9	20.9#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.325 ng
RT: 15.432 min Scan# 1574
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion	Ratio	Lower	Upper
198	100		
51	160.3	107.6	161.4
105	104.8	55.2	82.8#









#21
4-Bromophenyl-phenylether
Concen: 0.434 ng
RT: 16.239 min Scan# 1640
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:	248	Resp:	172
Ion	Ratio	Lower	Upper
248	100		
250	101.4	83.5	125.3
141	74.8	55.3	82.9

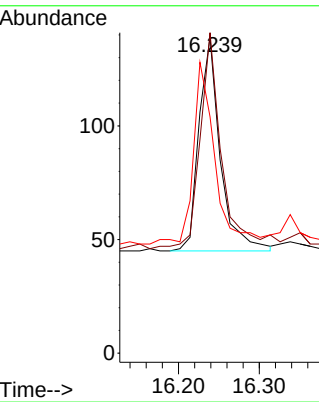

#22
Hexachlorobenzene
Concen: 0.409 ng
RT: 16.351 min Scan# 1649
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:	284	Resp:	192
Ion	Ratio	Lower	Upper
284	100		
142	54.2	37.7	56.5
249	40.1	29.0	43.6



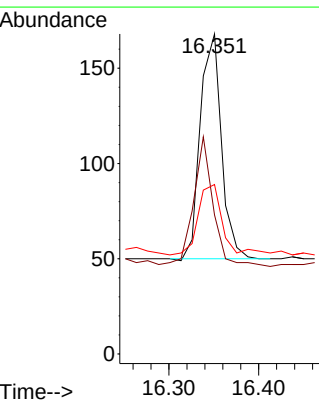





#23
Atrazine
Concen: 0.516 ng
RT: 16.512 min Scan# 1662
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:200 Resp: 200
Ion Ratio Lower Upper
200 100
173 46.6 28.6 43.0#
215 65.1 40.5 60.7#

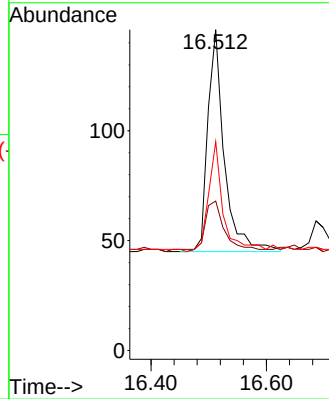

#24
Pentachlorophenol
Concen: 0.565 ng
RT: 16.686 min Scan# 1676
Delta R.T. -0.012 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:266 Resp: 139
Ion Ratio Lower Upper
266 100
264 54.0 44.6 66.8
268 77.7 51.8 77.6#









#25
Phenanthrene
Concen: 0.443 ng
RT: 17.071 min Scan# 1707
Delta R.T. -0.012 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:178 Resp: 880
Ion Ratio Lower Upper
178 100
176 20.0 16.6 25.0
179 17.3 12.8 19.2



#26
Anthracene
Concen: 0.483 ng
RT: 17.170 min Scan# 1715
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:178 Resp: 854
Ion Ratio Lower Upper
178 100
176 18.9 15.8 23.6
179 14.9 12.6 18.8









#27
Fluoranthene-d10
Concen: 0.420 ng
RT: 19.073 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion	Ratio	Lower	Upper
212	100		
106	13.0	11.2	16.8
104	9.7	7.5	11.3



#28
Fluoranthene
Concen: 0.447 ng
RT: 19.100 min Scan# 1950
Delta R.T. -0.005 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.1	8.5	12.7
203	17.9	13.8	20.6





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.224 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN036894.D

Acq: 12 Apr 2025 00:45

Instrument :

BNA_N

ClientSampleId :

PB167519BSD





Tgt Ion:240 Resp: 805

Ion Ratio Lower Upper

240 100

120 30.7 15.8 23.6#

236 37.1 25.8 38.8

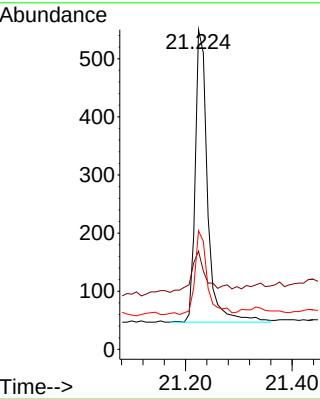

#30

Pyrene

Concen: 0.398 ng

RT: 19.467 min Scan# 2029

Delta R.T. -0.000 min

Lab File: BN036894.D

Acq: 12 Apr 2025 00:45




Tgt Ion:202 Resp: 1210


Ion Ratio Lower Upper

202 100

200 22.1 17.1 25.7

203 18.2 14.5 21.7



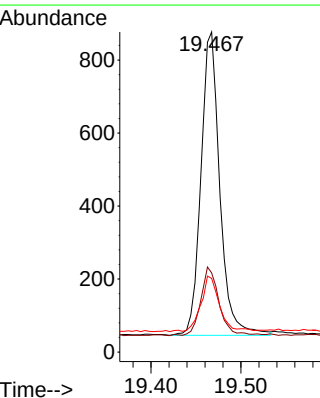





#31
Terphenyl-d14
Concen: 0.384 ng
RT: 19.676 min Scan# 2074
Delta R.T. -0.005 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:244 Resp: 587
Ion Ratio Lower Upper
244 100
212 20.2 11.6 17.4#
122 25.7 14.9 22.3#



#32
Benzo(a)anthracene
Concen: 0.432 ng
RT: 21.215 min Scan# 2280
Delta R.T. -0.000 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:228 Resp: 1228
Ion Ratio Lower Upper
228 100
226 31.2 24.5 36.7
229 22.6 17.7 26.5









#33
Chrysene
Concen: 0.452 ng
RT: 21.260 min Scan# 211
Delta R.T. -0.009 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:228 Resp: 1417
Ion Ratio Lower Upper
228 100
226 34.7 26.1 39.1
229 23.7 17.0 25.4

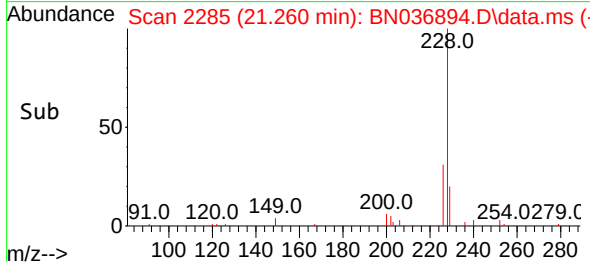

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.454 ng
RT: 21.153 min Scan# 2273
Delta R.T. -0.009 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:149 Resp: 958
Ion Ratio Lower Upper
149 100
167 25.7 21.0 31.4
279 4.0 3.6 5.4

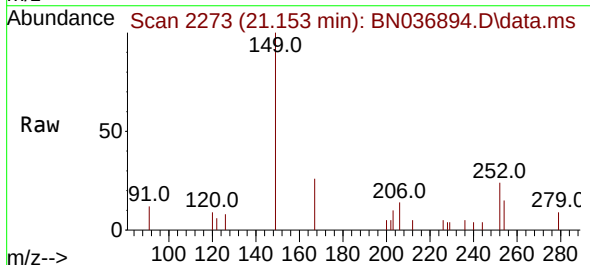



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.444 min Scan# 21

Delta R.T. -0.012 min

Lab File: BN036894.D

Acq: 12 Apr 2025 00:45

Instrument :

BNA_N

ClientSampleId :

PB167519BSD





Tgt Ion:264 Resp: 1051

Ion Ratio Lower Upper

264 100

260 31.6 22.9 34.3

265 159.2 88.6 132.8#



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.490 ng

RT: 25.672 min Scan# 3530

Delta R.T. -0.015 min

Lab File: BN036894.D

Acq: 12 Apr 2025 00:45




Tgt Ion:276 Resp: 2458


Ion Ratio Lower Upper

276 100

138 24.5 21.0 31.6

277 24.7 19.3 28.9


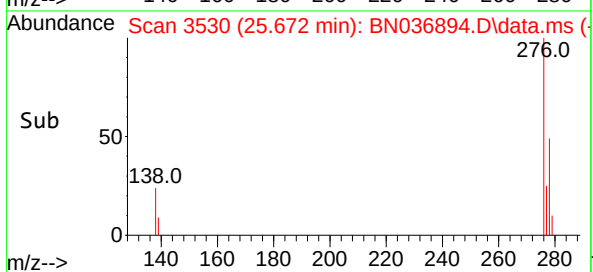






#37
Benzo(b)fluoranthene
Concen: 0.406 ng
RT: 22.781 min Scan# 2541
Delta R.T. -0.009 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45




Instrument :
BNA_N
ClientSampleId :
PB167519BSD


Tgt Ion:252 Resp: 1513
Ion Ratio Lower Upper
252 100
253 38.6 27.0 40.6
125 25.6 17.7 26.5



#38
Benzo(k)fluoranthene
Concen: 0.450 ng m
RT: 22.825 min Scan# 2556
Delta R.T. -0.009 min
Lab File: BN036894.D
Acq: 12 Apr 2025 00:45

Tgt Ion:252 Resp: 1692
Ion Ratio Lower Upper
252 100
253 40.7 26.7 40.1#
125 25.6 16.9 25.3#





#39

Benzo(a)pyrene

Concen: 0.468 ng

RT: 23.348 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN036894.D

Acq: 12 Apr 2025 00:45

Instrument :

BNA_N

ClientSampleId :

PB167519BSD





Tgt Ion:252 Resp: 1529

Ion Ratio Lower Upper

252 100

253 45.3 31.5 47.3

125 32.1 22.6 34.0



#40

Dibenzo(a,h)anthracene

Concen: 0.480 ng

RT: 25.690 min Scan# 3536

Delta R.T. -0.012 min

Lab File: BN036894.D

Acq: 12 Apr 2025 00:45




Tgt Ion:278 Resp: 1912


Ion Ratio Lower Upper

278 100

139 23.5 17.6 26.4

279 39.8 26.7 40.1





#41

Benzo(g,h,i)perylene

Concen: 0.444 ng

RT: 26.356 min Scan# 31

Delta R.T. -0.006 min

Lab File: BN036894.D


Acq: 12 Apr 2025 00:45

Instrument :

BNA_N

ClientSampleId :

PB167519BSD





Tgt Ion:276 Resp: 2001

Ion Ratio Lower Upper

276 100

277 30.1 21.8 32.8

138 28.9 21.6 32.4

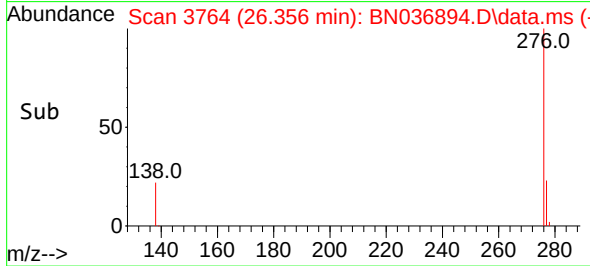

Manual Integration Report

Sequence:	bn041125	Instrument	BNA_n

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
SSTDICC0.1	BN036873.D	Benzo(k)fluoranthene	Rahul	4/14/2025 11:05:23 AM	Jagrut	4/14/2025 1:07:34 PM	Peak Integrated by Software
SSTDICV0.4	BN036880.D	1,4-Dioxane	Rahul	4/14/2025 11:05:25 AM	Jagrut	4/14/2025 1:07:37 PM	Peak Integrated by Software
SSTDCCC0.4	BN036884.D	1,4-Dioxane	Rahul	4/14/2025 11:05:28 AM	Jagrut	4/14/2025 1:07:40 PM	Peak Integrated by Software
SSTDCCC0.4	BN036884.D	Benzo(k)fluoranthene	Rahul	4/14/2025 11:05:28 AM	Jagrut	4/14/2025 1:07:40 PM	Peak Integrated by Software
Q1741-01	BN036886.D	1,4-Dioxane	Rahul	4/14/2025 11:05:59 AM	Jagrut	4/14/2025 1:07:42 PM	Peak Integrated by Software
Q1741-01	BN036886.D	2-Fluorophenol	Rahul	4/14/2025 11:05:59 AM	Jagrut	4/14/2025 1:07:42 PM	Peak Integrated by Software
PB167519BS	BN036893.D	2-Methylnaphthalene-d1 0	Rahul	4/14/2025 11:06:07 AM	Jagrut	4/14/2025 1:07:50 PM	Peak Integrated by Software
PB167519BS	BN036893.D	Benzo(k)fluoranthene	Rahul	4/14/2025 11:06:07 AM	Jagrut	4/14/2025 1:07:50 PM	Peak Integrated by Software
PB167519BSD	BN036894.D	2-Methylnaphthalene-d1 0	Rahul	4/14/2025 11:06:11 AM	Jagrut	4/14/2025 1:07:53 PM	Peak Integrated by Software
PB167519BSD	BN036894.D	Benzo(k)fluoranthene	Rahul	4/14/2025 11:06:11 AM	Jagrut	4/14/2025 1:07:53 PM	Peak Integrated by Software
SSTDCCC0.4	BN036895.D	1,4-Dioxane	Rahul	4/14/2025 11:06:14 AM	Jagrut	4/14/2025 1:07:55 PM	Peak Integrated by Software

Manual Integration Report

Sequence:	BN041425	Instrument	BNA_n

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
SSTDICC0.1	BN036898.D	1,4-Dioxane	Rahul	4/15/2025 9:32:24 AM	Jagrut	4/15/2025 9:43:18 AM	Peak Integrated by Software
SSTDICC0.2	BN036899.D	1,4-Dioxane	Rahul	4/15/2025 9:32:27 AM	Jagrut	4/15/2025 9:43:20 AM	Peak Integrated by Software

Instrument ID: **BNA_N**

Daily Analysis Runlog For Sequence/QC Batch ID # BN041125

Review By	Rahul	Review On	4/14/2025 11:08:44 AM
Supervise By	Jagrut	Supervise On	4/14/2025 1:08:14 PM
SubDirectory	BN041125	HP Acquire Method	BNA_N, 8270_SiM HP Processing Method bn041125
STD. NAME	STD REF.#		
Tune/Reschk	SP6757		
Initial Calibration Stds	SP6738,SP6736,SP6735,SP6734,SP6733,SP6732,SP6731		
CCC	SP6735		
Internal Standard/PEM	SP6740,1ul/100ul sample		
ICV/I.BLK	SP6768		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	DFTPP	BN036872.D	11 Apr 2025 11:03	RC/JU	Ok
2	SSTDIC0.1	BN036873.D	11 Apr 2025 11:42	RC/JU	Ok,M
3	SSTDIC0.2	BN036874.D	11 Apr 2025 12:37	RC/JU	Ok
4	SSTDIC0.4	BN036875.D	11 Apr 2025 13:17	RC/JU	Ok
5	SSTDIC0.8	BN036876.D	11 Apr 2025 13:53	RC/JU	Ok
6	SSTDIC1.6	BN036877.D	11 Apr 2025 14:30	RC/JU	Ok
7	SSTDIC3.2	BN036878.D	11 Apr 2025 15:06	RC/JU	Ok
8	SSTDIC5.0	BN036879.D	11 Apr 2025 15:42	RC/JU	Ok
9	SSTDICV0.4	BN036880.D	11 Apr 2025 16:18	RC/JU	Ok,M
10	PB167519BL	BN036881.D	11 Apr 2025 16:53	RC/JU	Not Ok
11	PB167565BL	BN036882.D	11 Apr 2025 17:29	RC/JU	Not Ok
12	DFTPP	BN036883.D	11 Apr 2025 18:06	RC/JU	Ok
13	SSTDIC0.4	BN036884.D	11 Apr 2025 18:45	RC/JU	Ok,M
14	PB167565BL	BN036885.D	11 Apr 2025 19:21	RC/JU	Ok
15	Q1741-01	BN036886.D	11 Apr 2025 19:57	RC/JU	Dilution
16	Q1741-02	BN036887.D	11 Apr 2025 20:34	RC/JU	Ok
17	Q1741-03	BN036888.D	11 Apr 2025 21:10	RC/JU	Ok
18	Q1773-02	BN036889.D	11 Apr 2025 21:46	RC/JU	Ok
19	Q1773-03	BN036890.D	11 Apr 2025 22:22	RC/JU	Ok
20	PB167565BS	BN036891.D	11 Apr 2025 22:57	RC/JU	Ok,M
21	PB167565BSD	BN036892.D	11 Apr 2025 23:33	RC/JU	Ok,M

Instrument ID: BNA_N

Daily Analysis Runlog For Sequence/QC Batch ID # BN041125

Review By	Rahul	Review On	4/14/2025 11:08:44 AM
Supervise By	Jagrut	Supervise On	4/14/2025 1:08:14 PM
SubDirectory	BN041125	HP Acquire Method	BNA_N, 8270_SiM HP Processing Method bn041125
STD. NAME	STD REF.#		
Tune/Reschk	SP6757		
Initial Calibration Stds	SP6738,SP6736,SP6735,SP6734,SP6733,SP6732,SP6731		
CCC	SP6735		
Internal Standard/PEM	SP6740,1ul/100ul sample		
ICV/I.BLK	SP6768		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	PB167519BS	BN036893.D	12 Apr 2025 00:09	RC/JU	Ok,M
23	PB167519BSD	BN036894.D	12 Apr 2025 00:45	RC/JU	Ok,M
24	SSTDCCC0.4	BN036895.D	12 Apr 2025 01:21	RC/JU	Ok,M

M : Manual Integration

Instrument ID: BNA_N

Daily Analysis Runlog For Sequence/QC Batch ID # BN041425

Review By	Rahul	Review On	4/15/2025 9:33:09 AM
Supervise By	Jagrut	Supervise On	4/15/2025 9:43:34 AM
SubDirectory	BN041425	HP Acquire Method	BNA_N, 8270_SiM HP Processing Method BN041425
STD. NAME	STD REF.#		
Tune/Reschk	SP6757		
Initial Calibration Stds	SP6738,SP6736,SP6735,SP6734,SP6733,SP6732,SP6731		
CCC	SP6735		
Internal Standard/PEM	SP6740,1ul/100ul sample		
ICV/I.BLK	SP6768		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	DFTPP	BN036896.D	14 Apr 2025 10:10	RC/JU	Ok
2	SSTDCCC0.4	BN036897.D	14 Apr 2025 12:50	RC/JU	Not Ok
3	SSTDICC0.1	BN036898.D	14 Apr 2025 13:26	RC/JU	Ok,M
4	SSTDICC0.2	BN036899.D	14 Apr 2025 14:02	RC/JU	Ok,M
5	SSTDICCC0.4	BN036900.D	14 Apr 2025 14:38	RC/JU	Ok
6	SSTDICC0.8	BN036901.D	14 Apr 2025 15:15	RC/JU	Ok
7	SSTDICC1.6	BN036902.D	14 Apr 2025 15:51	RC/JU	Ok
8	SSTDICC3.2	BN036903.D	14 Apr 2025 16:27	RC/JU	Ok
9	SSTDICC5.0	BN036904.D	14 Apr 2025 17:03	RC/JU	Ok
10	SSTDICV0.4	BN036905.D	14 Apr 2025 17:39	RC/JU	Ok
11	PB167519BL	BN036906.D	14 Apr 2025 18:51	RC/JU	Ok
12	PB167565BL	BN036907.D	14 Apr 2025 19:28	RC/JU	Ok
13	Q1741-01DL	BN036908.D	14 Apr 2025 20:04	RC/JU	Ok
14	SSTDCCC0.4	BN036909.D	14 Apr 2025 20:40	RC/JU	Ok

M : Manual Integration

Instrument ID: BNA_N

Daily Analysis Runlog For Sequence/QC Batch ID # BN041125

Review By	Rahul	Review On	4/14/2025 11:08:44 AM
Supervise By	Jagrut	Supervise On	4/14/2025 1:08:14 PM
SubDirectory	BN041125	HP Acquire Method	BNA_N, 8270_HP Processing Method bn041125

STD. NAME	STD REF.#
Tune/Reschk Initial Calibration Stds	SP6757 SP6738,SP6736,SP6735,SP6734,SP6733,SP6732,SP6731
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	SP6735 SP6740,1ul/100ul sample SP6768

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	DFTPP	DFTPP	BN036872.D	11 Apr 2025 11:03		RC/JU	Ok
2	SSTDICC0.1	SSTDICC0.1	BN036873.D	11 Apr 2025 11:42	Compound#02 removed from 0.1 ppm	RC/JU	Ok,M
3	SSTDICC0.2	SSTDICC0.2	BN036874.D	11 Apr 2025 12:37		RC/JU	Ok
4	SSTDICCC0.4	SSTDICCC0.4	BN036875.D	11 Apr 2025 13:17		RC/JU	Ok
5	SSTDICC0.8	SSTDICC0.8	BN036876.D	11 Apr 2025 13:53		RC/JU	Ok
6	SSTDICC1.6	SSTDICC1.6	BN036877.D	11 Apr 2025 14:30		RC/JU	Ok
7	SSTDICC3.2	SSTDICC3.2	BN036878.D	11 Apr 2025 15:06		RC/JU	Ok
8	SSTDICC5.0	SSTDICC5.0	BN036879.D	11 Apr 2025 15:42		RC/JU	Ok
9	SSTDICV0.4	ICVBN041125	BN036880.D	11 Apr 2025 16:18		RC/JU	Ok,M
10	PB167519BL	PB167519BL	BN036881.D	11 Apr 2025 16:53	Internal Standard Fail, Analyzed for contamination check	RC/JU	Not Ok
11	PB167565BL	PB167565BL	BN036882.D	11 Apr 2025 17:29	Internal Standard Fail, Analyzed for contamination check	RC/JU	Not Ok
12	DFTPP	DFTPP	BN036883.D	11 Apr 2025 18:06		RC/JU	Ok
13	SSTDCCC0.4	SSTDCCC0.4	BN036884.D	11 Apr 2025 18:45		RC/JU	Ok,M
14	PB167565BL	PB167565BL	BN036885.D	11 Apr 2025 19:21		RC/JU	Ok
15	Q1741-01	RMW-02B-66-040425	BN036886.D	11 Apr 2025 19:57	Need 10X Dilution	RC/JU	Dilution
16	Q1741-02	RMW-06B-74-040425	BN036887.D	11 Apr 2025 20:34		RC/JU	Ok
17	Q1741-03	FB01-040425	BN036888.D	11 Apr 2025 21:10		RC/JU	Ok

Instrument ID: BNA_N

Daily Analysis Runlog For Sequence/QC Batch ID # BN041125

Review By	Rahul	Review On	4/14/2025 11:08:44 AM
Supervise By	Jagrut	Supervise On	4/14/2025 1:08:14 PM
SubDirectory	BN041125	HP Acquire Method	BNA_N, 8270_HP Processing Method bn041125
STD. NAME	STD REF.#		
Tune/Reschk	SP6757		
Initial Calibration Stds	SP6738,SP6736,SP6735,SP6734,SP6733,SP6732,SP6731		
CCC	SP6735		
Internal Standard/PEM	SP6740,1ul/100ul sample		
ICV/I.BLK	SP6768		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

18	Q1773-02	BP-TT-190D2-GW-202	BN036889.D	11 Apr 2025 21:46		RC/JU	Ok
19	Q1773-03	BP-TT-190D1-GW-202	BN036890.D	11 Apr 2025 22:22		RC/JU	Ok
20	PB167565BS	PB167565BS	BN036891.D	11 Apr 2025 22:57		RC/JU	Ok,M
21	PB167565BSD	PB167565BSD	BN036892.D	11 Apr 2025 23:33		RC/JU	Ok,M
22	PB167519BS	PB167519BS	BN036893.D	12 Apr 2025 00:09		RC/JU	Ok,M
23	PB167519BSD	PB167519BSD	BN036894.D	12 Apr 2025 00:45		RC/JU	Ok,M
24	SSTDCCC0.4	SSTDCCC0.4EC	BN036895.D	12 Apr 2025 01:21		RC/JU	Ok,M

M : Manual Integration

Instrument ID: BNA_N

Daily Analysis Runlog For Sequence/QC Batch ID # BN041425

Review By	Rahul	Review On	4/15/2025 9:33:09 AM
Supervise By	Jagrut	Supervise On	4/15/2025 9:43:34 AM
SubDirectory	BN041425	HP Acquire Method	BNA_N, 8270_HP Processing Method BN041425

STD. NAME	STD REF.#
Tune/Reschk	SP6757
Initial Calibration Stds	SP6738,SP6736,SP6735,SP6734,SP6733,SP6732,SP6731
CCC	SP6735
Internal Standard/PEM	SP6740,1ul/100ul sample
ICV/I.BLK	SP6768
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	DFTPP	DFTPP	BN036896.D	14 Apr 2025 10:10		RC/JU	Ok
2	SSTDCCC0.4	SSTDCCC0.4	BN036897.D	14 Apr 2025 12:50	A Fresh Calibration is required.	RC/JU	Not Ok
3	SSTDICC0.1	SSTDICC0.1	BN036898.D	14 Apr 2025 13:26	Compound#20 removed from 0.1 ppm	RC/JU	Ok,M
4	SSTDICC0.2	SSTDICC0.2	BN036899.D	14 Apr 2025 14:02		RC/JU	Ok,M
5	SSTDICCC0.4	SSTDICCC0.4	BN036900.D	14 Apr 2025 14:38		RC/JU	Ok
6	SSTDICC0.8	SSTDICC0.8	BN036901.D	14 Apr 2025 15:15		RC/JU	Ok
7	SSTDICC1.6	SSTDICC1.6	BN036902.D	14 Apr 2025 15:51		RC/JU	Ok
8	SSTDICC3.2	SSTDICC3.2	BN036903.D	14 Apr 2025 16:27		RC/JU	Ok
9	SSTDICC5.0	SSTDICC5.0	BN036904.D	14 Apr 2025 17:03		RC/JU	Ok
10	SSTDICV0.4	ICVBN041425	BN036905.D	14 Apr 2025 17:39		RC/JU	Ok
11	PB167519BL	PB167519BL	BN036906.D	14 Apr 2025 18:51		RC/JU	Ok
12	PB167565BL	PB167565BL	BN036907.D	14 Apr 2025 19:28		RC/JU	Ok
13	Q1741-01DL	RMW-02B-66-040425D	BN036908.D	14 Apr 2025 20:04		RC/JU	Ok
14	SSTDCCC0.4	SSTDCCC0.4EC	BN036909.D	14 Apr 2025 20:40		RC/JU	Ok

M : Manual Integration

SOP ID:	M3510C,3580A-Extraction SVOC-20		
Clean Up SOP #:	N/A	Extraction Start Date :	04/08/2025
Matrix :	Water	Extraction Start Time :	10:10
Weigh By:	N/A	Extraction By:	RJ
Balance check:	N/A	Filter By:	RJ
Balance ID:	N/A	pH Meter ID:	N/A
pH Strip Lot#:	E3880	Hood ID:	4,5,6,7
Extraction Method:	☒ Separatory Funnel	☐ Continuous Liquid/Liquid	☐ Sonication
		☐ Waste Dilution	☐ Soxhlet
		Extraction End Date :	04/08/2025
		Extraction End Time :	15:10
		Concentration By:	EH
		Supervisor By :	rajesh

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	0.4 PPM	SP6739
Surrogate	1.0ML	0.4 PPM	SP6755
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3904
Baked Na2SO4	N/A	EP2597
10N NaOH	N/A	EP2559
H2SO4 1:1	N/A	EP2565
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

1.5 ML Vial lot# 2210673. pH Adjusted<2 with 1:1 H2SO4 &>11 with 10 N NaOH.

KD Bath ID:	WATER BATH-1,2	Envap ID:	NEVAP-02
KD Bath Temperature:	60 °C	Envap Temperature:	40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
04/08/25	RP (Ext Lab)	ACI/SVOC
15:15	Preparation Group	Analysis Group

Analytical Method: M3510C,3580A-Extraction SVOC-20

Concentration Date: 04/08/2025

Sample ID	Client Sample ID	Test	g / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB167519BL	SBLK519	SVOC-SIMGrou p1	1000	6	ritesh	rajesh	1			SEP-11
PB167519BS	SLCS519	SVOC-SIMGrou p1	1000	6	ritesh	rajesh	1			12
PB167519BS D	SLCSD519	SVOC-SIMGrou p1	1000	6	ritesh	rajesh	1			13
Q1741-01	RMW-02B-66-040425	SVOC-SIMGrou p1	970	6	ritesh	rajesh	1	C		14
Q1741-02	RMW-02B-74-040425	SVOC-SIMGrou p1	970	6	ritesh	rajesh	1	C		15
Q1741-03	FB01-040425	SVOC-SIMGrou p1	980	6	ritesh	rajesh	1	C		16

* Extracts relinquished on the same date as received.

2
4/8/25

10:10
167519
mo

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q1741

WorkList ID : 188807

Department : Extraction

Date : 04-08-2025 10:05:19

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1739-01	WC-LIQUID-20250404	Water	SVOC-TCL BNA -20	Cool 4 deg C	PARS02	L31	04/04/2025	8270E
Q1739-01	WC-LIQUID-20250404	Water	TPH GC	Cool 4 deg C	PARS02	L31	04/04/2025	8015D
Q1741-01	RMW-02B-66-040425	Water	SVOC-SIMGroup1	Cool 4 deg C	JACO05	L33	04/04/2025	8270-Modified
Q1741-02	RMW-02B-74-040425	Water	SVOC-SIMGroup1	Cool 4 deg C	JACO05	L33	04/04/2025	8270-Modified
Q1741-03	FB01-040425	Water	SVOC-SIMGroup1	Cool 4 deg C	JACO05	L33	04/04/2025	8270-Modified
Q1746-05	B-158-GW01	Water	SVOC-TCL BNA -20	Cool 4 deg C	PORT06	L41	04/05/2025	8270E
Q1746-06	B-149-GW01	Water	SVOC-TCL BNA -20	Cool 4 deg C	PORT06	L41	04/06/2025	8270E
Q1746-07	EB-2025-4-7	Water	SVOC-TCL BNA -20	Cool 4 deg C	PORT06	L41	04/07/2025	8270E

Date/Time 04/08/25 10:05

Raw Sample Received by: RJ (Det 1457)

Raw Sample Relinquished by: CR Sm

Date/Time 04/08/25 10:30

Raw Sample Received by: CR Sm

Raw Sample Relinquished by: RJ (Det 1457)

Prep Standard - Chemical Standard Summary

Order ID : Q1741
Test : SVOC-SIMGroup1
Prepbatch ID : PB167519,
Sequence ID/Qc Batch ID: bn041125,BN041425,

Standard ID :
EP2559,EP2565,EP2597,SP6682,SP6730,SP6731,SP6732,SP6733,SP6734,SP6735,SP6736,SP6738,SP6739,SP6740,SP6755,SP6757,SP6767,SP6768,

Chemical ID :
1ul/100ul
sample,E3551,E3657,E3828,E3873,E3874,E3902,E3904,E3926,M5173,S10104,S 11495,S11650,S11785,S11788,S11832,S12114,S12195,S12216,S12270,S12328,S12478,S12486,S12525,S12533,S12577,S12651,S12791,S12966,S12974,W3112,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1874	10 N SODIUM HYDROXIDE SOLN	EP2559	11/14/2024	05/14/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 11/14/2024

FROM 1000.00000ml of W3112 + 400.00000gram of E3657 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2565	11/20/2024	05/20/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/20/2024

FROM 1000.00000ml of M5173 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2597	03/28/2025	07/01/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	Evelyn Huang 03/28/2025

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3493	Internal Standard 0.4 PPM	SP6682	11/15/2024	05/09/2025	Jagrut Upadhyay	None	None	Yogesh Patel 12/03/2024

FROM 0.10000ml of S12328 + 4.90000ml of E3828 = Final Quantity: 5.000 ml

SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3339	8270 sim calibration stock 10ppm (CPI)	SP6730	02/04/2025	05/12/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.03350ml of S10104 + 0.05000ml of S11495 + 0.12500ml of S11832 + 0.12500ml of S12114 + 0.25000ml of S12270 + 0.25000ml of S12791 + 24.16650ml of E3874 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3361	8270-SIM MDL-5PPM CALIBRATION SOLUTION	SP6731	02/04/2025	05/09/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.50000ml of E3874 + 0.01000ml of SP6682 + 0.50000ml of SP6730 = Final Quantity: 1.010 ml

SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3341	8270-SIM MDL-3.2PPM CALIBRATION SOLUTION	SP6732	02/04/2025	05/09/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.68000ml of E3874 + 0.01000ml of SP6682 + 0.32000ml of SP6730 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3344	8270-SIM MDL-1.6PPM CALIBRATION SOLUTION	SP6733	02/04/2025	05/09/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.84000ml of E3874 + 0.01000ml of SP6682 + 0.16000ml of SP6730 = Final Quantity: 1.010 ml

SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3342	8270-SIM MDL-0.8PPM CALIBRATION SOLUTION	SP6734	02/04/2025	05/09/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.92000ml of E3874 + 0.01000ml of SP6682 + 0.08000ml of SP6730 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3343	8270-SIM MDL-0.4PPM CALIBRATION SOLUTION	SP6735	02/04/2025	05/09/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.96000ml of E3874 + 0.01000ml of SP6682 + 0.04000ml of SP6730 = Final Quantity: 1.010 ml

SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3345	8270-SIM MDL-0.2PPM CALIBRATION SOLUTION	SP6736	02/04/2025	05/09/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.50000ml of E3874 + 0.01000ml of SP6682 + 0.50000ml of SP6735 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3346	8270-SIM MDL-0.1PPM CALIBRATION SOLUTION	SP6738	02/04/2025	05/09/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.75000ml of E3874 + 0.01000ml of SP6682 + 0.25000ml of SP6735 = Final Quantity: 1.010 ml

SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3492	8270-SIM-Spike 0.4 PPM	SP6739	02/05/2025	07/29/2025	Jagrut Upadhyay	None	None	Yogesh Patel 02/07/2025

FROM 0.00080ml of S11650 + 0.01000ml of S11785 + 0.02000ml of S12478 + 0.02000ml of S12525 + 0.02000ml of S12966 + 49.92920ml of E3873 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3493	Internal Standard 0.4 PPM	SP6740	02/13/2025	07/30/2025	Rahul Chavli	None	None	Yogesh Patel 02/28/2025

FROM 0.10000ml of S12651 + 4.90000ml of E3874 = Final Quantity: 5.000 ml

SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3491	8270-SIM-Surrogate 0.4 PPM	SP6755	03/20/2025	07/24/2025	Jagrut Upadhyay	None	None	Rahul Chavli
								04/01/2025

FROM 0.00400ml of S12195 + 0.00800ml of S12216 + 0.02000ml of S11832 + 99.96800ml of E3902 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3895	50 ug/ml DFTPP 8270E	SP6757	03/31/2025	09/30/2025	Rahul Chavli	None	None	Jagrut Upadhyay
								04/01/2025

FROM 1.00000ml of S12577 + 19.00000ml of E3904 = Final Quantity: 20.000 ml

SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3355	8270-SIM MDL-3.2PPM CALIBRATION STOCK SOL- 2ND	SP6767	04/10/2025	07/24/2025	Jagrut Upadhyay	None	None	Sohil Jodhani
SOURCE FROM 0.00630ml of S12195 + 0.01280ml of S12216 + 0.03200ml of S11788 + 0.03200ml of S11832 + 0.06400ml of S12486 + 0.06400ml of S12533 + 0.06400ml of S12974 + 19.72490ml of E3926 = Final Quantity: 20.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3356	8270-SIM MDL-0.4PPM CALIBRATION SOL ICV-2ND	SP6768	04/10/2025	07/24/2025	Jagrut Upadhyay	None	None	Sohil Jodhani
SOURCE FROM 0.87500ml of E3926 + 0.01000ml of SP6740 + 0.12500ml of SP6767 = Final Quantity: 1.010 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19510-5 / Sodium Hydroxide Pellets 2.5 Kg, Pk of 4	23B1556310	12/31/2025	12/04/2023 / Rajesh	12/01/2023 / Rajesh	E3657

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24G0862003	05/09/2025	11/09/2024 / Rajesh	11/04/2024 / Rajesh	E3828

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	07/29/2025	01/29/2025 / Rajesh	01/29/2025 / Rajesh	E3873

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A0262002	07/30/2025	01/30/2025 / Rajesh	01/20/2025 / Rajesh	E3874

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	09/18/2025	03/18/2025 / RUPESH	02/12/2025 / RUPESH	E3902

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24K1762005	01/07/2026	03/13/2025 / RUPESH	12/27/2024 / RUPESH	E3904

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A0262002	10/08/2025	04/08/2025 / Rajesh	02/07/2025 / Rajesh	E3926

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	06/02/2025	06/01/2022 /	04/05/2022 / william	M5173

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-112090-04 / CLP Acid Surrogate Solution, 7500 mg/L, 1ml	440246	07/30/2025	01/30/2025 / anahy	12/09/2021 / Christian	S10104

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110094-02 / CLP Base/Neutral Surrogate Solution, 5000 mg/L, 1ml	506889	05/12/2025	11/12/2024 / Jagrut	08/11/2023 / Yogesh	S11495

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555872 / Custom Standard, pentachlorophenol Std [CS 5328-5]	A0201728	07/29/2025	01/29/2025 / anahy	11/09/2023 / Yogesh	S11650

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31853 / 1,4-Dioxane, 2000 ug/ml , Solvent: Methylene Chloride	A0196453	07/29/2025	01/29/2025 / anahy	11/21/2023 / Rahul	S11785

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31853 / 1,4-Dioxane, 2000 ug/ml , Solvent: Methylene Chloride	A0196453	09/10/2025	03/10/2025 / anahy	11/21/2023 / Rahul	S11788

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	33913 / SOM01.0 SIM Analysis Standard (Surrogate), 2000 PPM	A0201976	07/24/2025	01/24/2025 / anahy	11/21/2023 / rahul	S11832

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	z-010223-01 / 1,4-Dioxane Solution, 2,000mg/L, 1ml	454157	05/12/2025	11/12/2024 / Jagrut	03/08/2024 / Rahul	S12114

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31087 / Acid Surrogate 10,000ug/ml, methanol, 5ml/ ampul	A0206206	09/18/2025	03/18/2025 / anahy	03/15/2024 / Rahul	S12195

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31086 / Base Neutral Surrogate 5000ug/ml, CH ₂ Cl ₂ , 5ml	A0206381	09/18/2025	03/18/2025 / anahy	03/15/2024 / Rahul	S12216

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	z-110381-01 / 8270 Calibration Solution, 76-1, 500 & 1,000 mg/L, 1ml	520963	07/30/2025	01/30/2025 / anahy	05/24/2024 / Rahul	S12270

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31206 / SV Mix, CLP method, Internal Std, 2000ug/mL, CH2Cl2, 1mL	A0206540	05/13/2025	11/13/2024 / anahy	05/30/2024 / Rahul	S12328

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555223 / Custom 8270 Plus Std #1 [2nd lot at \$100 per ampul if requested - contact ARM with Request]	A0214021	07/29/2025	01/29/2025 / anahy	07/23/2024 / RAHUL	S12478

[CS 4978-1]

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555223 / Custom 8270 Plus Std #1 [2nd lot at \$100 per ampul if requested - contact ARM with Request]	A0214021	09/10/2025	03/10/2025 / anahy	07/23/2024 / RAHUL	S12486

[CS 4978-1]

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555224 / Custom 8270 Plus Std #2 [2nd lot at \$85 per ampul if requested - contact ARM with Request]	A0214017	07/29/2025	01/29/2025 / anahy	07/23/2024 / RAHUL	S12525

[CS 4978-2]

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555224 / Custom 8270 Plus Std #2 [2nd lot at \$85 per ampul if requested - contact ARM with Request]	A0214017	09/10/2025	03/10/2025 / anahy	07/23/2024 / RAHUL	S12533

[CS 4978-2]

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31615 / SV Mixture, GC/MS Tuning Mixture, CH ₂ Cl ₂ , 1mL,	A0212955	06/30/2027	03/31/2025 / Rahul	08/01/2024 / Rahul	S12577

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31206 / SV Mix, CLP method, Internal Std, 2000ug/mL, CH ₂ Cl ₂ , 1mL	A0212266	08/07/2025	02/07/2025 / anahy	09/20/2024 / anahy	S12651

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110816-01 / Custom 8270 Mix, 4-79, 1000 mg/L, 1 mL, (Maximum Expiration: 180 Days)	414127	06/21/2025	01/30/2025 / anahy	05/24/2024 / Rahul	S12791

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31850 / 8270 SV Mix, 8270 Mega Mix 1mL, 1000ug/mL, CH ₂ Cl ₂ [New Solvent 100% CH ₂ Cl ₂]	A0219438	07/29/2025	01/29/2025 / anahy	12/11/2024 / anahy	S12966

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31850 / 8270 SV Mix, 8270 Mega Mix 1mL, 1000ug/mL, CH ₂ Cl ₂ [New Solvent 100% CH ₂ Cl ₂]	A0219438	09/10/2025	03/10/2025 / anahy	12/11/2024 / anahy	S12974

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112



5580 Skylane Blvd
Santa Rosa, CA 95403

(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: **Storage:** **Solvent:** **Exp. Date:** **Description:**
Z-112090 440246 $\leq -10^{\circ}\text{C}$ Methylene Chloride 2/16/2026 CLP Acid Surrogate Solution, 7,500 mg/L, 1 mL
-04

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
2-chlorophenol-d ₄	93951-73-6	99.3	248.12.7P	7487 $\pm$ 17.2
2-fluorophenol	367-12-4	99.8	10.7.3.3P	7513 $\pm$ 17.26
phenol-d ₆	13127-88-3	99.9	949.120.8P	7481 $\pm$ 17.19
2,4,6-tribromophenol	118-79-6	99.8	12.1.6P	7469 $\pm$ 17.17

Received on

02/25/21

by
CG

S9236
to

S9240

*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.

Certified By: _____

Erica Castiglione
Chemist



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3



Certificate of Analysis

Sodium Hydroxide (Pellets)

Material: 0583
Grade: ACS GRADE
Batch Number: 23B1556310

Chemical Formula: NaOH
Molecular Weight: 40
CAS #: 1310-73-2
Appearance:

Manufacture Date: 12/14/2022
Expiration Date: 12/31/2025

Storage: Room Temperature

Pellets

TEST	SPECIFICATION	ANALYSIS	DISPOSITION
Calcium	$\leq 0.005 \%$	$< 0.005 \%$	PASS
Chloride	$\leq 0.005 \%$	0.002 %	PASS
Heavy Metals	$\leq 0.002 \%$	$< 0.002 \%$	PASS
Iron	$\leq 0.001 \%$	$< 0.001 \%$	PASS
Magnesium	$\leq 0.002 \%$	$< 0.002 \%$	PASS
Mercury	$\leq 0.1 \text{ ppm}$	$< 0.1 \text{ ppm}$	PASS
Nickel	$\leq 0.001 \%$	$< 0.001 \%$	PASS
Nitrogen Compounds	$\leq 0.001 \%$	$< 0.001 \%$	PASS
Phosphate	$\leq 0.001 \%$	$< 0.001 \%$	PASS
Potassium	$\leq 0.02 \%$	$< 0.02 \%$	PASS
Purity	$\geq 97.0 \%$	99.2 %	PASS
Sodium Carbonate	$\leq 1.0 \%$	0.5 %	PASS
Sulfate	$\leq 0.003 \%$	$< 0.003 \%$	PASS

Internal ID #: 710

Signature

We certify that this batch conforms to the specifications listed.


This document has been electronically produced and is valid without a signature.

Leona Edwardson, Quality Control Sr. Manager - Solon
VWR Chemicals, LLC.
28600 Fountain Parkway, Solon OH 44139 USA

Additional Information

Analysis may have been rounded to significant digits in specification limits.

Product meets analytical specifications of the grades listed.

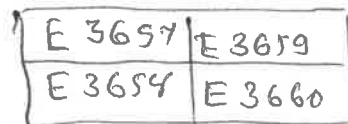

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)

avantor™



Material No.: 9266-A4

Batch No.: 24J0862003

Manufactured Date: 2024-09-12

Expiration Date: 2025-12-12

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	1
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3828

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	<= 0.3	0.2
Titration Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 1/29/25

E 3873

Jamie Croak

Director Quality Operations, Bioscience Production

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)

Avantor

Material No.: 9266-A4
Batch No.: 25A0262002
Manufactured Date: 2024-11-21
Expiration Date: 2026-02-20
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	4
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	99.9%
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.8 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3874



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E3902

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087 U.S.A. Phone 610.386.1700

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 25A0262002
Manufactured Date: 2024-11-21
Expiration Date: 2026-02-20
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol)Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	4
Assay (CH ₂ Cl ₂) (by GC, exclusive of preservative, corrected for water)	>= 99.8 %	99.9 %
Color (APHA)	<= 10	10
Residue after Evaporation	<= 1.0 ppm	0.8 ppm
Titration Acid (µeq/g)	<= 0.3	<0.1
Chloride (Cl)	<= 10 ppm	<5 ppm
Water (by KF, coulometric)	<= 0.02 %	<0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3926

J. Croak
Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis



Material No.: 9530-33
Batch No.: 0000281827
Manufactured Date: 2021/03/30
Retest Date: 2026/03/29
Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



5580 Skylane Blvd
Santa Rosa, CA 95403

(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.:	Lot No.:	Storage:	Solvent:	Exp. Date:	Description:
Z-110094-02	506889	≤ -10 °C	Methylene Chloride	7/25/2028	CLP Base/Neutral Surrogate Solution, 5,000 mg/L, 1 ml

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
1,2-dichlorobenzene-d ₄	2199-69-1	99.7	247.29.3P	5035 ± 28.02
2-fluorobiphenyl	321-60-8	99.69	8.286.1.1P	4999 ± 103.66
nitrobenzene-d5	4165-60-0	99.67	7.9.3P	4988 ± 27.32
p-terphenyl-d14	1718-51-0	99.3	9.120.8P	5005 ± 27.85

511494 } Y.P.
↓
511498 } 08/11/2023

*Not a certified value

Certified By: Shane C. Tipton
Clint Tipton
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555872 **Lot No.:** A0201728

Description : Custom Pentachlorophenol Standard

Custom Pentachlorophenol Standard 25,000µg/mL, Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : September 30, 2026 **Storage:** 10°C or colder

Ship: Ambient

511649
↓
511658
Y.P.
11/13/23

CERTIFIED VALUES

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Pentachlorophenol	87-86-5	RP230530RSR	99%	25,000.0 µg/mL	+/- 777.0837

Solvent: Methanol
CAS # 67-56-1
Purity 99%

Josh McCloskey - Operations Technician I

Date Mixed: 05-Sep-2023

Balance: B251644995

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31853 **Lot No.:** A0196453
Description : 1,4-dioxane
1,4-Dioxane 2,000µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : March 31, 2028 **Storage:** 0°C or colder
Ship: Ambient

S11749
↓
S11794 } RC / 11/30/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dioxane	123-91-1	SHBN3770	99%	2,013.0 µg/mL	+/- 25.0521

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant flow 1.8 mL/min.

Temp. Program:

80°C (hold 0.1 min.) to 330°C
@ 9.6°C/min. (hold 2.86 min.)

Inj. Temp:

250°C

Det. Temp:

340°C

Det. Type:


FID

Split Vent:

100 ml/min.

Inj. Vol

1µl

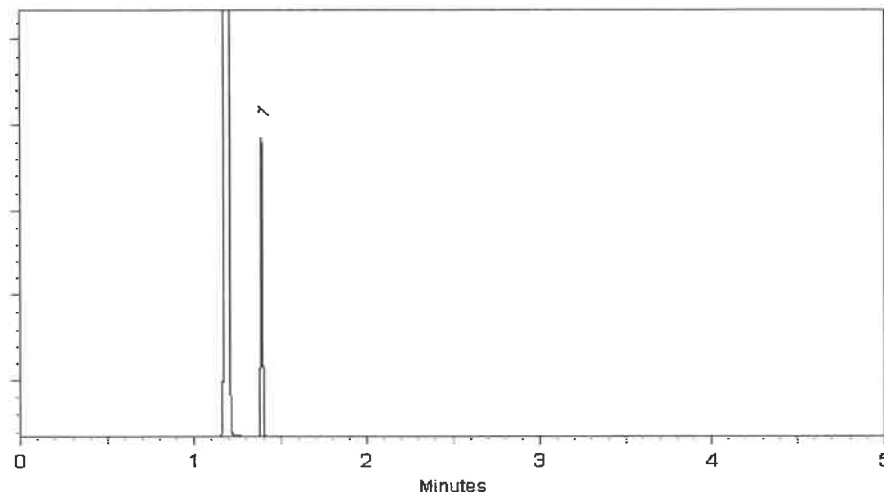

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 30-Mar-2023

Balance Serial # B707717271

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 31-Mar-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 33913 **Lot No.:** A0201976
Description : SOM01.0 SIM Analysis Standard
SOM01.0 SIM Analysis Standard 2000µg/mL, Methylene chloride, 1mL /ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : August 31, 2029 **Storage:** 10°C or colder
Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

S11828
↓
S11832 } RC/
11/30/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Methylnaphthalene-d10	7297-45-2	EF-135	98%	2,015.9 µg/mL	+/- 90.8098
2	Fluoranthene-d10	93951-69-0	PR-32557	99%	2,020.0 µg/mL	+/- 90.9963

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

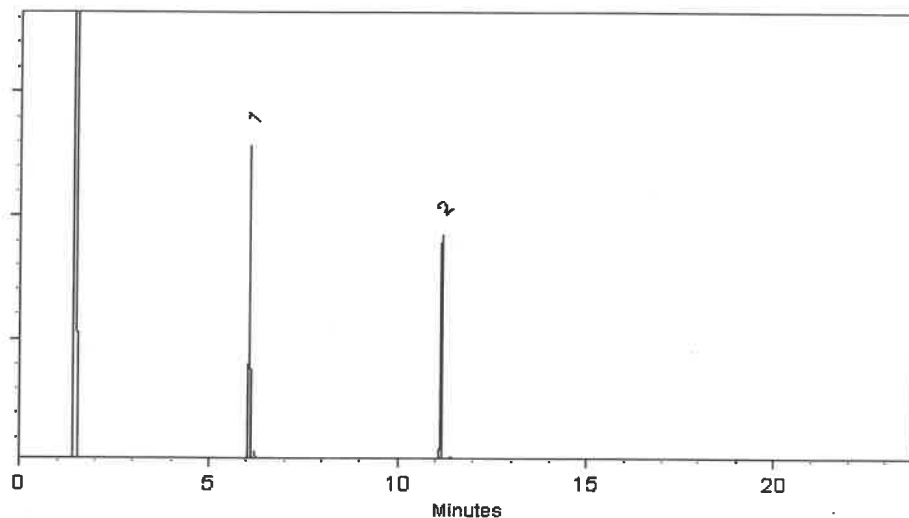


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 13-Sep-2023

Balance Serial # B442140311


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 28-Sep-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



5580 Skylane Blvd
Santa Rosa, CA 95403

(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.:	Lot No.:	Storage:	Solvent:	Exp. Date:	Description:
Z-020223-01	454157	≤ -10 °C	P/T Methanol	6/10/2026	1,4-Dioxane Solution, 2000 mg/L, 1 mL

<u>Compound</u>	<u>CAS No.</u>	<u>Purity (%)</u>	<u>Compound Lot No.</u>	<u>Concentration, mg/L</u>
1,4-dioxane	123-91-1	100	223.1.3P	1997 ± 57.08

512112 } RC/
↓
912116 } 03/08/24

*Not a certified value

Certified By: _____

Melissa Workoff
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31087 **Lot No.:** A0206206
Description : Acid Surrogate Mix (4/89 SOW)
Acid Surrogate 10, 000µg/mL, Methanol, 5mL/ampul
Container Size : 5 mL **Pkg Amt:** > 5 mL
Expiration Date : January 31, 2032 **Storage:** 10°C or colder
Ship: Ambient

512187 } RC/
↓
512206 } 03/18/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorophenol	367-12-4	STBK1705	99%	10,005.3 µg/mL	+/- 302.5390
2	Phenol-d6	13127-88-3	PR-33287A	99%	10,005.5 µg/mL	+/- 302.5475
3	2,4,6-Tribromophenol	118-79-6	RP230831RSR	99%	10,006.6 µg/mL	+/- 302.5783

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

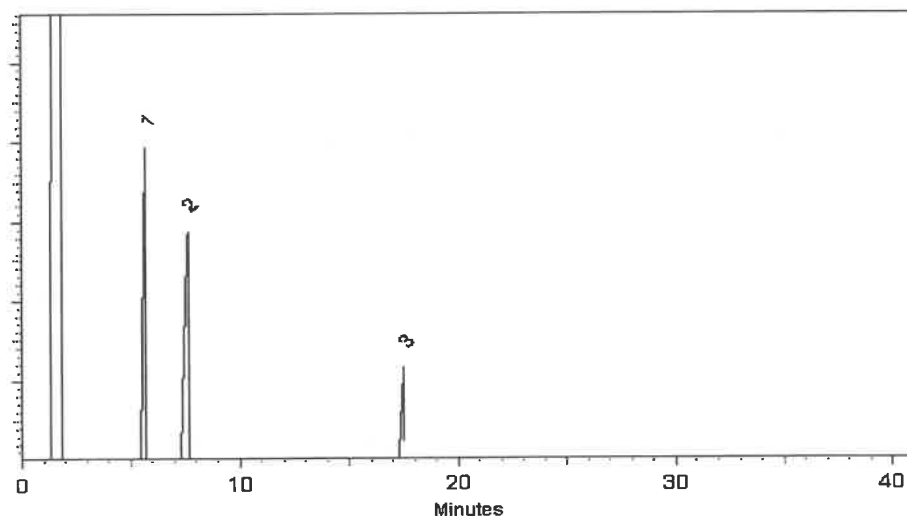

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope A. Riglin

Penelope Riglin - Operations Tech I

Christie Mills

Christie Mills - Operations Lead Tech - ARM QC

Date Mixed: 04-Jan-2024

Balance Serial # 1128360905

Date Passed: 08-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31086 **Lot No.:** A0206381
Description : B/N Surrogate Mix (4/89 SOW)
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul
Container Size : 5 mL **Pkg Amt:** > 5 mL
Expiration Date : December 31, 2029 **Storage:** 10°C or colder
Handling: Sonicate prior to use. **Ship:** Ambient

S12207 } RC/
↓
S12221 } 03/18/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Nitrobenzene-d5	4165-60-0	I-25158	99%	5,029.3 µg/mL	+/- 226.5204
2	2-Fluorobiphenyl	321-60-8	00021384	99%	5,030.9 µg/mL	+/- 226.5936
3	p-Terphenyl-d14	1718-51-0	PR-32599	99%	5,026.4 µg/mL	+/- 226.3909

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

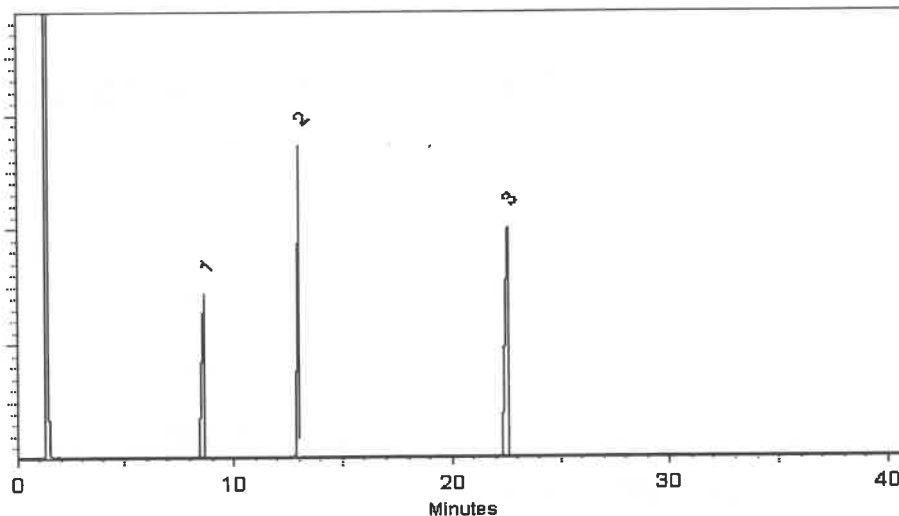

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Jess Hoy - Operations Tech I

Date Mixed: 09-Jan-2024

Balance Serial # 1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 11-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



5580 Skylane Blvd
Santa Rosa, CA 95403

(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Rev 0

Page 1 of 4

Catalog No.: Lot No.: Storage: Solvent: Exp. Date: Description:
Z-110381-01 520963 $\leq -10^{\circ}\text{C}$ Methylene Chloride 10/10/2028 Method 8270 Calibration Solution, 76-1, 500 & 1,000 mg/L, 1 mL

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
acenaphthene	83-32-9	99.9	13.1.5P	1010 $\pm$ 9.89
acenaphthylene	208-96-8	97.6	14.290.1P	1014 $\pm$ 9.93
aniline	62-53-3	99.97	64.1.4P	1001 $\pm$ 9.8
anthracene	120-12-7	99.5	15.7.1P	999.6 $\pm$ 9.79
azobenzene	103-33-3	98.1	252.7.2P	999.1 $\pm$ 9.8
benzo[a]anthracene	56-55-3	100	16.7.3P	1007 $\pm$ 9.86
benzo[b]fluoranthene	205-99-2	99.8	17.421.3P	1011 $\pm$ 14.11
benzo[k]fluoranthene	207-08-9	98.9	18.421.4P	1001 $\pm$ 10.96
benzo[ghi]perylene	191-24-2	93	19.286.4P	999.6 $\pm$ 13.95
benzo[a]pyrene	50-32-8	97	20.286.2P	999.9 $\pm$ 22.24
benzyl alcohol	100-51-6	99.9	65.18.1P	1001 $\pm$ 9.82
bis(2-chloroethoxy)methane	111-91-1	99.1	31.3.15P	1000 $\pm$ 14.69
bis(2-chloroethyl)ether	111-44-4	99.8	32.7.1P	1003 $\pm$ 13.89
bis(2-chloro-1-methylethyl) ether	108-60-1	99.5	34.3.15P	999.4 $\pm$ 14.68
bis(2-ethylhexyl)adipate	103-23-1	99.5	874.7.1P	999.5 $\pm$ 9.8
bis(2-ethylhexyl)phthalate	117-81-7	99.4	33.29.1P	998.8 $\pm$ 17.03
4-bromophenyl phenyl ether	101-55-3	99.4	35.7.1.1P	1000 $\pm$ 13.85
butyl benzyl phthalate	85-68-7	98.4	36.1.6P	984.7 $\pm$ 16.79
carbazole	86-74-8	99.4	239.7.2P	1000 $\pm$ 9.8

*Not a certified value

512270 } RC/
↓
512274 } 05/24/24

Kerry Kane

Certified By: _____

Kerry Kane
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.

Certificate of Analysis

Page 2 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
4-chloroaniline	106-47-8	100	66.7.1P	1000 ± 9.79
4-chlorophenylphenyl ether	7005-72-3	98	37.158.2P	1001 ± 17.07
4-chloro-3-methylphenol	59-50-7	99	102.1.2P	1006 ± 17.16
2-chloronaphthalene	91-58-7	99.9	42.7.6P	1000 ± 9.79
2-chlorophenol	95-57-8	99.8	103.7.1P	1007 ± 13.96
chrysene	218-01-9	96	21.286.2P	998.4 ± 12.85
dibenz[a,h]anthracene	53-70-3	99.44	22.286.3P	1000 ± 9.74
dibenzofuran	132-64-9	100	67.7.2.1P	1002 ± 9.77
di-n-butyl phthalate	84-74-2	99.84	40.286.1P	1007 ± 24.48
1,2-dichlorobenzene	95-50-1	99.8	43.7.1P	1000 ± 9.79
1,3-dichlorobenzene	541-73-1	99.5	44.1.3P	999.4 ± 9.79
1,4-dichlorobenzene	106-46-7	99.9	45.29.2P	1000 ± 9.79
2,4-dichlorophenol	120-83-2	99.6	104.7.1.1P	1005 ± 13.93
diethyl phthalate	84-66-2	99.8	38.7.1P	1011 ± 14
2,4-dimethylphenol	105-67-9	99.6	105.7.1.1P	1009 ± 13.98
dimethyl phthalate	131-11-3	99.9	39.9.2P	996.5 ± 13.8
1,2-dinitrobenzene	528-29-0	99.86	86.7.3.1P	999.5 ± 9.75
1,3-dinitrobenzene	99-65-0	100	313.7.2P	998 ± 9.79
1,4-dinitrobenzene	100-25-4	100	907.7.1P	999.5 ± 9.8
2,4-dinitrophenol	51-28-5	99.9	106.1.6DP	1002 ± 13.89
2,4-dinitrotoluene	121-14-2	100	87.7.3P	999.8 ± 13.85
2,6-dinitrotoluene	606-20-2	99.4	88.7.2.1P	999.6 ± 13.85
di-n-octyl phthalate	117-84-0	99.1	41.7.5P	991.6 ± 13.74
diphenylamine	122-39-4	100	78.1.6P	998 ± 13.79
2,3,5,6-tetrachlorophenol	935-95-5	97	1112.286.1P	1004 ± 14.02
fluoranthene	206-44-0	98.6	23.7.4P	999.6 ± 9.79
fluorene	86-73-7	98.4	24.7.1P	999.7 ± 9.79

*Not a certified value

Kerry Kane

Certified By:

Kerry Kane
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.

Certificate of Analysis

Page 3 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
hexachlorobenzene	118-74-1	99	46.158.4P	999.9 ± 13.96
hexachlorobutadiene	87-68-3	97.4	47.1.4P	1000 ± 9.79
hexachlorocyclopentadiene	77-47-4	99.2	48.2.2P	1001 ± 9.8
hexachloroethane	67-72-1	99.9	49.1.4P	1003 ± 9.82
indeno[1,2,3-cd]pyrene	193-39-5	98	25.286.4P	999.4 ± 22.23
isophorone	78-59-1	98.9	90.1.4P	999.9 ± 13.85
2-methyl-4,6-dinitrophenol	534-52-1	99.6	107.421.2DP	991 ± 24.09
1-methylnaphthalene	90-12-0	97.1	249.7.5P	999.2 ± 13.95
2-methylnaphthalene	91-57-6	97.4	68.7.2P	1006 ± 22.38
2-methylphenol	95-48-7	99.6	114.7.3P	1001 ± 13.87
3-methylphenol	108-39-4	99.1	115.7.4P	499.7 ± 6.92
4-methylphenol	106-44-5	99.5	116.7.1P	501.2 ± 6.94
naphthalene	91-20-3	99.8	26.9.1P	1018 ± 9.97
2-nitroaniline	88-74-4	99.7	69.29.1P	999.6 ± 9.79
3-nitroaniline	99-09-2	100	70.7.3P	1000 ± 9.74
4-nitroaniline	100-01-6	99.7	71.29.1P	1001 ± 9.8
nitrobenzene	98-95-3	100	94.7.1P	1000 ± 13.85
2-nitrophenol	88-75-5	99.1	108.29.1P	996.5 ± 13.81
4-nitrophenol	100-02-7	100	109.7.1P	1000 ± 13.82
N-nitrosodimethylamine	62-75-9	99.5	57.3.19P	998.5 ± 14.67
N-nitrosodi-n-propylamine	621-64-7	99.8	59.286.1P	996.8 ± 17
pentachlorophenol	87-86-5	99	110.1.7P	1004 ± 13.92
phenanthrene	85-01-8	99.7	27.1.5P	999 ± 12.87
phenol	108-95-2	100	112.7.1P	998.5 ± 13.8
pyrene	129-00-0	99.2	28.9.2P	998.9 ± 9.78
pyridine	110-86-1	100	101.24.1P	999 ± 9.73
2,3,4,6-Tetrachlorophenol	58-90-2	91.8	120.421.1P	996.5 ± 13.92

*Not a certified value

Kerry Kane

Certified By:

Kerry Kane
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.

Certificate of Analysis

Page 4 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
1,2,4-trichlorobenzene	120-82-1	99.6	54.29.1P	999.6 ± 9.79
2,4,5-trichlorophenol	95-95-4	96.5	121.7.1.1P	999.5 ± 13.85
2,4,6-trichlorophenol	88-06-2	99.6	113.7.1P	996 ± 13.8

*Not a certified value



Certified By:

Kerry Kane
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31206 **Lot No.:** A0206540

Description : SV Internal Standard Mix 2mg/ml
SV Internal Standard Mix 2mg/ml 2000 µg/ml, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

S12312 } RC/
↓ 05/30/24
S12331 }

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	2,007.1 µg/mL	+/- 90.4025
2	Naphthalene-d8	1146-65-2	M-2180	99%	2,005.9 µg/mL	+/- 90.3454
3	Acenaphthene-d10	15067-26-2	PR-33507	99%	2,007.9 µg/mL	+/- 90.4385
4	Phenanthrene-d10	1517-22-2	PR-32303	99%	2,006.7 µg/mL	+/- 90.3845
5	Chrysene-d12	1719-03-5	PR-32210	99%	2,015.5 µg/mL	+/- 90.7778
6	Perylene-d12	1520-96-3	PR-33205	99%	2,014.7 µg/mL	+/- 90.7448

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

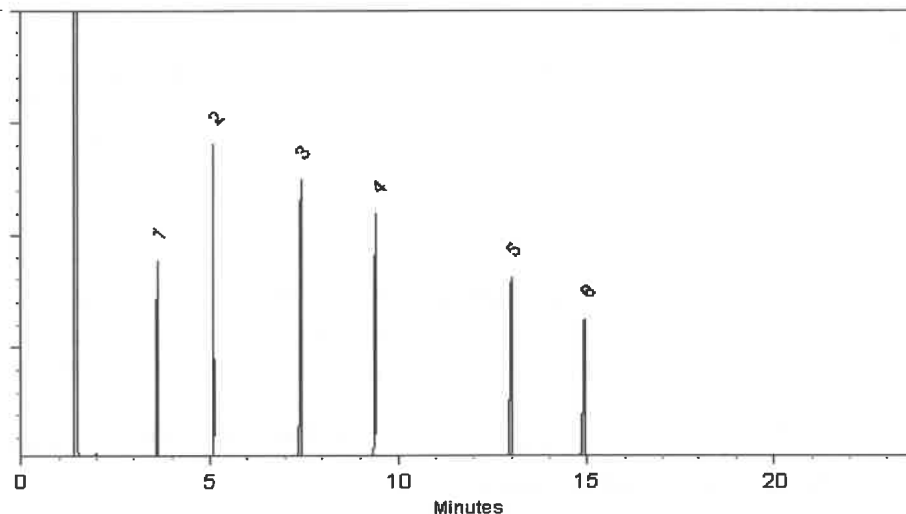

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Malina Homan
Malina Homan - Operations Technician I

Date Mixed: 12-Jan-2024

Balance Serial # 1128360905

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555223 **Lot No.:** A0214021

Description : Custom 8270 Plus Standard #1
Custom 8270 Plus Standard #1 1,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2026 **Storage:** 10°C or colder

Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	3,3'-Dichlorobenzidine	91-94-1	S240326RSR	99%	1,004.0 µg/mL	+/- 23.0487
2	Atrazine	1912-24-9	5FYWL	99%	1,005.0 µg/mL	+/- 23.0717
3	Benzidine	92-87-5	S240430RSR	99%	1,006.0 µg/mL	+/- 23.0947
4	epsilon-Caprolactam	105-60-2	Y16H012	99%	1,000.0 µg/mL	+/- 22.9569

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

S12449 } RC/
↓
S12508 } 7/24/24

Rebecca Gingerich - Operations Tech II

Date Mixed: 18-Jul-2024

Balance: 1128353505

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555224 **Lot No.:** A0214017

Description : Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2026 **Storage:** 10°C or colder

Ship: Ambient

CERTIFIED VALUES

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,4,5-Tetrachlorobenzene	95-94-3	MKCT9480	99%	1,005.0 µg/mL	+/- 29.541899
2	Acetophenone	98-86-2	STBH8205	99%	1,005.0 µg/mL	+/- 29.541899
3	Benzaldehyde	100-52-7	RD231129RSRA	99%	1,008.0 µg/mL	+/- 29.630084
4	Benzoic acid	65-85-0	MKCR2694	99%	1,010.0 µg/mL	+/- 29.688874
5	Biphenyl	92-52-4	MKCS5928	99%	1,008.0 µg/mL	+/- 29.630084

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

S12509 } RC/
↓
S12568 } 7/24/24

Jess Hoy - Operations Tech I

Date Mixed: 18-Jul-2024

Balance: 1128360905

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31615 **Lot No.:** A0212955
Description : GC/MS Tuning Mixture
GC/MS Tuning Mixture 1,000µg/mL, Methylene Chloride, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : June 30, 2027 **Storage:** 10°C or colder
Handling: Contains carcinogen/reproductive toxin. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Pentachlorophenol	87-86-5	RP240517RSR	99%	1,004.5 µg/mL	+/- 44.8902
2	DFTPP (Decafluorotriphenylphosphine)	5074-71-5	Q117-147	99%	1,004.5 µg/mL	+/- 44.8902
3	Benzidine	92-87-5	S240430RSR	99%	1,006.0 µg/mL	+/- 44.9572
4	4,4'-DDT	50-29-3	S240530RSR	97%	1,000.1 µg/mL	+/- 44.6922

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

S12577 } RC
↓
S12579 } 8/2/24

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

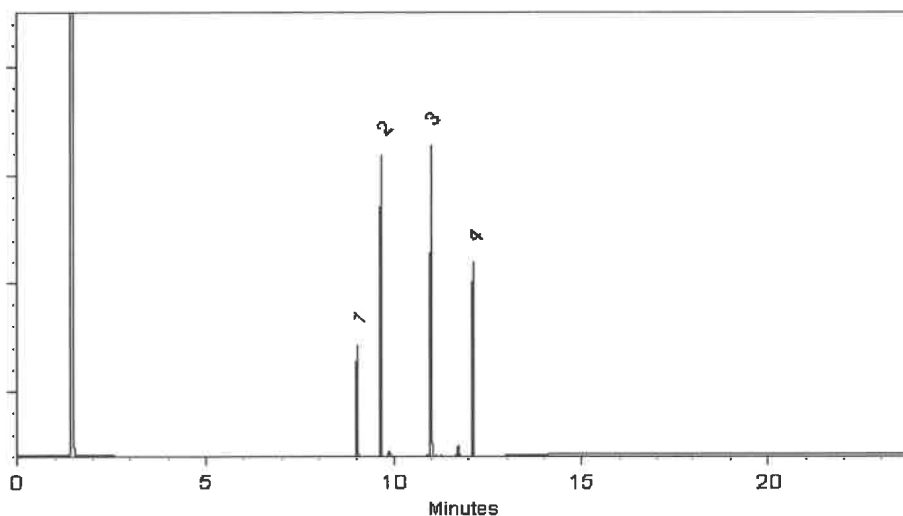


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Ethan Winiarski - Operations Tech I

Date Mixed: 19-Jun-2024

Balance Serial # 1128353505


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 26-Jun-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31206 **Lot No.:** A0212266

Description : SV Internal Standard Mix 2mg/ml
SV Internal Standard Mix 2mg/ml 2000 µg/ml, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	2,000.6 µg/mL	+/- 90.1075
2	Naphthalene-d8	1146-65-2	M-2180	99%	2,000.3 µg/mL	+/- 90.0925
3	Acenaphthene-d10	15067-26-2	PR-33507	99%	2,000.4 µg/mL	+/- 90.1000
4	Phenanthrene-d10	1517-22-2	PR-34099	99%	2,000.5 µg/mL	+/- 90.1037
5	Chrysene-d12	1719-03-5	PR-33506	99%	2,000.7 µg/mL	+/- 90.1112
6	Perylene-d12	1520-96-3	PR-33205	99%	2,000.6 µg/mL	+/- 90.1075

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

S12645
↓
S12674 } AC
10/1/24



5580 Skylane Blvd
Santa Rosa, CA 95403

(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.:	Lot No.:	Storage:	Solvent:	Exp. Date:	Description:
Z-110816-01	414127	≤ -10 °C	Methylene Chloride	6/21/2025	Custom 8270 Mix, 4-79, 1000 mg/L, 1 mL

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
atrazine	1912-24-9	99.5	337.7.3P	997 ± 5.81
benzidine	92-87-5	99.9	124.18.6.2P	991.8 ± 5.77
caprolactam	105-60-2	99.9	271.1.6P	999 ± 5.82

~~512280~~ } RCL
↓
~~512284~~ } 05/24/24

New Numbers Generated.

512790 } RCL
↓
512794 } 11/12/24

*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

Certified By: _____

Shane Overcash
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31850 **Lot No.:** A0219438

Description : 8270 MegaMix®
8270 MegaMix® 500-1000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : September 30, 2025 **Storage:** 0°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

S12963
↓
S12992 } AC
12/17/20

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Pyridine	110-86-1	SHBP6240	99%	1,008.3 µg/mL	+/- 36.6849
2	N-Nitrosodimethylamine	62-75-9	S240313RSR	99%	1,008.6 µg/mL	+/- 36.6985
3	Phenol	108-95-2	MKCK1120	99%	1,003.5 µg/mL	+/- 36.5120
4	Aniline	62-53-3	X22F726	99%	1,002.9 µg/mL	+/- 36.4893
5	Bis(2-chloroethyl)ether	111-44-4	002891T24M	99%	1,003.0 µg/mL	+/- 36.4938
6	2-Chlorophenol	95-57-8	STBJ3909	99%	1,005.6 µg/mL	+/- 36.5894
7	1,3-Dichlorobenzene	541-73-1	BCCD5315	99%	1,004.1 µg/mL	+/- 36.5348
8	1,4-Dichlorobenzene	106-46-7	MKBS7929V	99%	1,002.1 µg/mL	+/- 36.4620
9	Benzyl alcohol	100-51-6	SHBK5469	99%	1,003.5 µg/mL	+/- 36.5120
10	1,2-Dichlorobenzene	95-50-1	SHBL6287	99%	1,005.3 µg/mL	+/- 36.5757
11	2-Methylphenol (o-cresol)	95-48-7	SHBN7598	99%	1,008.4 µg/mL	+/- 36.6894
12	2,2'-oxybis(1-chloropropane)	108-60-1	29-MAR-45-5	99%	1,004.6 µg/mL	+/- 36.5530
13	3-Methylphenol (m-cresol)	108-39-4	STBJ0710	99%	502.1 µg/mL	+/- 18.2697
14	4-Methylphenol (p-cresol)	106-44-5	SHBN3411	99%	503.8 µg/mL	+/- 18.3288
15	N-Nitroso-di-n-propylamine	621-64-7	N63MG	99%	1,006.5 µg/mL	+/- 36.6212
16	Hexachloroethane	67-72-1	DAXRI	99%	1,004.5 µg/mL	+/- 36.5484
17	Nitrobenzene	98-95-3	10224044	99%	1,002.5 µg/mL	+/- 36.4757

18	Isophorone	78-59-1	MKCR3249	99%	1,003.4	µg/mL	+/- 36.5075
19	2-Nitrophenol	88-75-5	RP230710	99%	1,002.5	µg/mL	+/- 36.4757
20	2,4-Dimethylphenol	105-67-9	XW5GK	99%	1,006.5	µg/mL	+/- 36.6212
21	Bis(2-chloroethoxy)methane	111-91-1	15705100	99%	1,006.6	µg/mL	+/- 36.6257
22	2,4-Dichlorophenol	120-83-2	BCKK6969	99%	1,001.5	µg/mL	+/- 36.4393
23	1,2,4-Trichlorobenzene	120-82-1	SHBP5900	99%	1,006.4	µg/mL	+/- 36.6166
24	Naphthalene	91-20-3	STBL1057	99%	1,002.1	µg/mL	+/- 36.4620
25	4-Chloroaniline	106-47-8	BCCJ3217	99%	1,004.4	µg/mL	+/- 36.5439
26	Hexachlorobutadiene	87-68-3	X05J	98%	1,002.5	µg/mL	+/- 36.4771
27	4-Chloro-3-methylphenol	59-50-7	BCCD4461	99%	1,004.5	µg/mL	+/- 36.5484
28	2-Methylnaphthalene	91-57-6	STBL3028	99%	1,000.0	µg/mL	+/- 36.3847
29	1-Methylnaphthalene	90-12-0	5234.00-8	98%	990.2	µg/mL	+/- 36.0269
30	Hexachlorocyclopentadiene	77-47-4	099063I14L	98%	1,001.3	µg/mL	+/- 36.4325
31	2,4,6-Trichlorophenol	88-06-2	STBK8870	99%	1,006.4	µg/mL	+/- 36.6166
32	2,4,5-Trichlorophenol	95-95-4	3YFRE	97%	1,004.6	µg/mL	+/- 36.5505
33	2-Chloronaphthalene	91-58-7	RPN7O	99%	1,004.3	µg/mL	+/- 36.5393
34	2-Nitroaniline	88-74-4	RP240715RSR	99%	1,004.4	µg/mL	+/- 36.5439
35	1,4-Dinitrobenzene	100-25-4	RP240703RSR	99%	1,002.8	µg/mL	+/- 36.4847
36	Acenaphthylene	208-96-8	RP241029RSR	98%	1,000.0	µg/mL	+/- 36.3835
37	1,3-Dinitrobenzene	99-65-0	TRC3-1075941-2-1	99%	1,006.3	µg/mL	+/- 36.6121
38	Dimethylphthalate	131-11-3	358221L17K	99%	1,008.9	µg/mL	+/- 36.7076
39	2,6-Dinitrotoluene	606-20-2	BCCG1833	99%	1,006.6	µg/mL	+/- 36.6257
40	1,2-Dinitrobenzene	528-29-0	RP240701RSR	99%	1,002.5	µg/mL	+/- 36.4757
41	Acenaphthene	83-32-9	MKCR7169	99%	1,000.0	µg/mL	+/- 36.3847
42	3-Nitroaniline	99-09-2	RP240708RSR	99%	1,004.6	µg/mL	+/- 36.5530
43	2,4-Dinitrophenol	51-28-5	D240927RSR	----%	1,005.6	µg/mL	+/- 36.5894
44	Dibenzofuran	132-64-9	MKCN1772	99%	1,003.5	µg/mL	+/- 36.5120
45	2,4-Dinitrotoluene	121-14-2	102869V26E	99%	1,008.3	µg/mL	+/- 36.6849
46	4-Nitrophenol	100-02-7	20241029-2-AN	99%	1,004.8	µg/mL	+/- 36.5575
47	2,3,4,6-Tetrachlorophenol	58-90-2	PR-34476	99%	1,005.8	µg/mL	+/- 36.5939
48	2,3,5,6-Tetrachlorophenol	935-95-5	RP231219RSR	99%	1,006.4	µg/mL	+/- 36.6166
49	Fluorene	86-73-7	10246250	98%	1,000.7	µg/mL	+/- 36.4102
50	4-Chlorophenyl phenyl ether	7005-72-3	MKCT7248	99%	1,004.9	µg/mL	+/- 36.5621
51	Diethylphthalate	84-66-2	BCCJ6241	99%	1,003.9	µg/mL	+/- 36.5257
52	4-Nitroaniline	100-01-6	RP230111	99%	1,006.6	µg/mL	+/- 36.6257
53	4,6-Dinitro-2-methylphenol (Dinitro-o-cresol)	534-52-1	S241008RSR	99%	1,001.3	µg/mL	+/- 36.4302

54	Diphenylamine	122-39-4	MKCT1512	99%	1,003.0	µg/mL	+/- 36.4938
55	Azobenzene	103-33-3	BCKK0887	99%	1,002.4	µg/mL	+/- 36.4711
56	4-Bromophenyl phenyl ether	101-55-3	STBH6361	99%	1,008.8	µg/mL	+/- 36.7031
57	Hexachlorobenzene	118-74-1	15458400	99%	1,005.1	µg/mL	+/- 36.5712
58	Pentachlorophenol	87-86-5	RP240517RSR	99%	1,005.9	µg/mL	+/- 36.5984
59	Phenanthrene	85-01-8	MKCT3391	99%	1,004.9	µg/mL	+/- 36.5621
60	Anthracene	120-12-7	101492T18R	99%	1,005.1	µg/mL	+/- 36.5712
61	Carbazole	86-74-8	15276700	99%	1,005.4	µg/mL	+/- 36.5803
62	Di-n-butylphthalate	84-74-2	MKCN4337	99%	1,006.3	µg/mL	+/- 36.6121
63	Fluoranthene	206-44-0	MKCQ4728	99%	1,003.5	µg/mL	+/- 36.5120
64	Pyrene	129-00-0	BCKK2592	99%	1,002.0	µg/mL	+/- 36.4575
65	Benzyl butyl phthalate	85-68-7	X12I018	99%	1,007.5	µg/mL	+/- 36.6576
66	Bis(2-ethylhexyl)adipate	103-23-1	MKCM1988	99%	1,005.9	µg/mL	+/- 36.5984
67	Benz(a)anthracene	56-55-3	I70012022BAA	99%	1,005.5	µg/mL	+/- 36.5848
68	Chrysene	218-01-9	RP241007RSR	99%	1,005.3	µg/mL	+/- 36.5757
69	Bis(2-ethylhexyl)phthalate	117-81-7	MKCS8065	99%	1,007.5	µg/mL	+/- 36.6576
70	Di-n-octyl phthalate	117-84-0	15566400	99%	1,002.3	µg/mL	+/- 36.4666
71	Benzo(b)fluoranthene	205-99-2	052013B	99%	1,004.1	µg/mL	+/- 36.5348
72	Benzo(k)fluoranthene	207-08-9	012022K	99%	1,002.8	µg/mL	+/- 36.4847
73	Benzo(a)pyrene	50-32-8	NQLXA	98%	1,006.2	µg/mL	+/- 36.6108
74	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	1,001.8	µg/mL	+/- 36.4490
75	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	1,003.3	µg/mL	+/- 36.5029
76	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	1,003.8	µg/mL	+/- 36.5217

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Tech Tips:

N-Nitrosodiphenylamine (86-30-6) is prone to breakdown in the injection port and will be converted to Diphenylamine (122-39-4). When comparing the response of Diphenylamine to mixtures manufactured using N-Nitrosodiphenylamine, a difference in response will be observed. The ratio of the MW can be used to calculate the theoretical concentration of the N-Nitrosodiphenylamine.



SHIPPING DOCUMENTS

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: Jacobs
ADDRESS: 412 Mt. Kemble Ave Suite # 100
CITY: Morris Plains STATE: NJ ZIP: 07960
ATTENTION: John Infante John.Infante@Jacobs.com
PHONE: FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Mary Murphy
PROJECT NO.: D3868221 LOCATION: Princeton Junction
PROJECT MANAGER: Mary Murphy
e-mail: Mary.Murphy@Jacobs.com
PHONE: FAX:

CLIENT BILLING INFORMATION

BILL TO: Mary Murphy PO#:
ADDRESS:
CITY: STATE: ZIP:
ATTENTION: PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) Standard TAT DAYS*
HARDCOPY (DATA PACKAGE): DAYS*
EDD: DAYS*

*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☐ NJ Reduced ☐ US EPA CLP
☒ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other
☐ EDD FORMAT

Site specific VOCs (S2105) and 1,4 Dioxins (S2105-S2106)

PRESERVATIVES

COMMENTS

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									Specify Preservatives		
			COMP	GRAB	DATE	TIME		A/E	E									A-HCl	D-NaOH
								1	2	3	4	5	6	7	8	9	B-HNO3	E-ICE	
																		C-H2SO4	F-OTHER
1.	RMW-02B-66-040425	GW		X	4-4-25	1155	4	✓	✓										
2.	RMW-06B-74-040425	GW		X	4-4-25	1200	4	✓	✓										
3.	~~RMW-06B-74-040425~~ TRB-040425	DI		X	4-4-25	1215	4	✓	✓										
4.	TRB-040425	DI		X	4-4-25	1300	2	✓											
5.																			
6.																			
7.																			
8.																			
9.																			
10.																			

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP
1. <u>[Signature]</u>	<u>4-4-25 1547</u>	1. <u>[Signature]</u> <u>4/4/25 15:47</u>	Comments: <u>See work order for list of site specific VOCs</u>
RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	
2. <u>[Signature]</u>		2. <u>[Signature]</u>	
RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	
3. <u>[Signature]</u>		3. <u>[Signature]</u>	

Page 1 of 1

CLIENT: ☐ Hand Delivered ☐ Other

Shipment Complete

☐ YES ☐ NO

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q1741	JACO05	Order Date : 4/7/2025 10:06:00 AM	Project Mgr :
Client Name : JACOBS Engineering Grou		Project Name : Former Schlumberger STC	Report Type : Level 4
Client Contact : John Ynfante		Receive DateTime : ~~4/7/2025~~ 3:47:00 PM	EDD Type : CH2MHILL
Invoice Name : JACOBS Engineering Grou		Purchase Order : 4/4/2025	Hard Copy Date :
Invoice Contact : John Ynfante			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q1741-01	RMW-02B-66-040425	Water	04/04/2025	11:55					
					VOCMS Group3		8260-Low	10 2 Bus. Days	
Q1741-02	RMW-02B-74-040425 06B	Water	04/04/2025	12:00					
					VOCMS Group3		8260-Low	10 2 Bus. Days	
Q1741-03	FB01-040425	Water	04/04/2025	12:15					
					VOCMS Group3		8260-Low	10 2 Bus. Days	
Q1741-04	TB01-040425	Water	04/04/2025	13:00					
					VOCMS Group3		8260-Low	10 2 Bus. Days	

YG 04/15/2025

Relinquished By :

Date / Time :


4/7/25 1032

Received By :

Date / Time :


4/7/25 10:32 Apr 4

Storage Area : VOA Refridgerator Room