
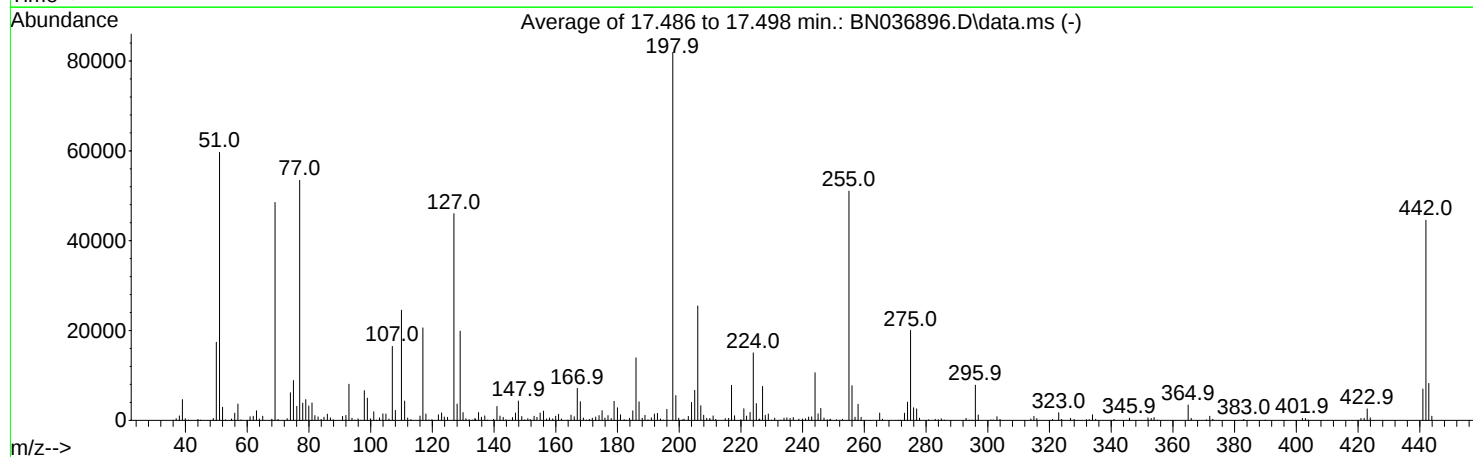


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036896.D
Acq On : 14 Apr 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 14 17:58:02 2025

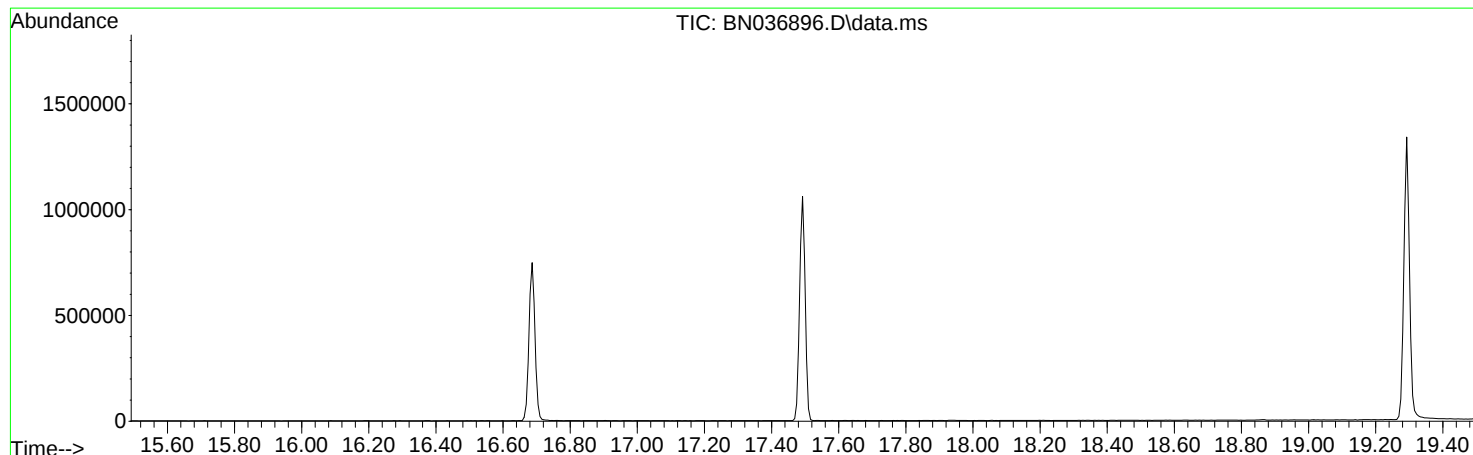

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	72.9	59683	PASS
68	69	0.00	2	0.6	275	PASS
69	198	0.00	100	59.2	48509	PASS
70	69	0.00	2	0.5	233	PASS
127	198	10	80	56.2	46043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81893	PASS
199	198	5	9	6.8	5540	PASS
275	198	10	60	24.4	20016	PASS
365	198	1	100	4.2	3404	PASS
441	198	0.01	100	8.5	6985	PASS
442	442	50	100	100.0	44557	PASS
443	442	15	24	18.5	8228	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/14/2025	BNA_N	<u>BN036896.D</u>
Compound Name	Response	Retention Time
DDT	288576	20.533
DDD	2965	20.145
DDE	0	19.621
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2965	291541	1.02

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036896.D
Acq On : 14 Apr 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 14 19:33:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

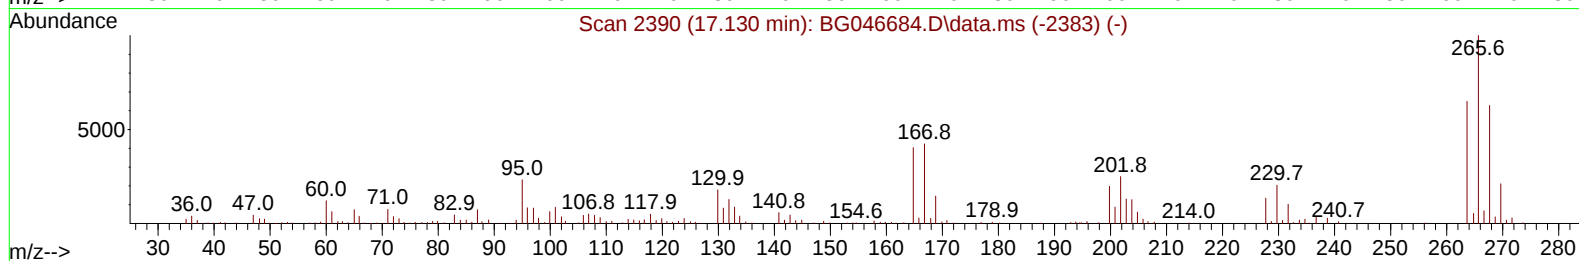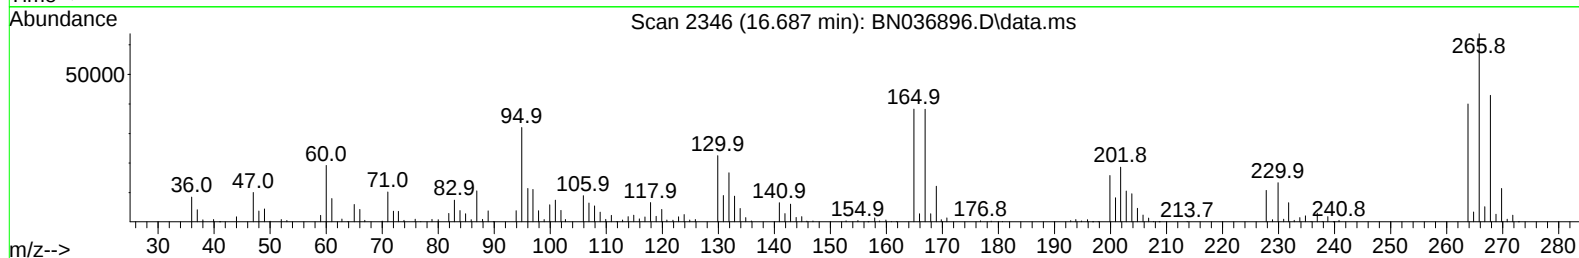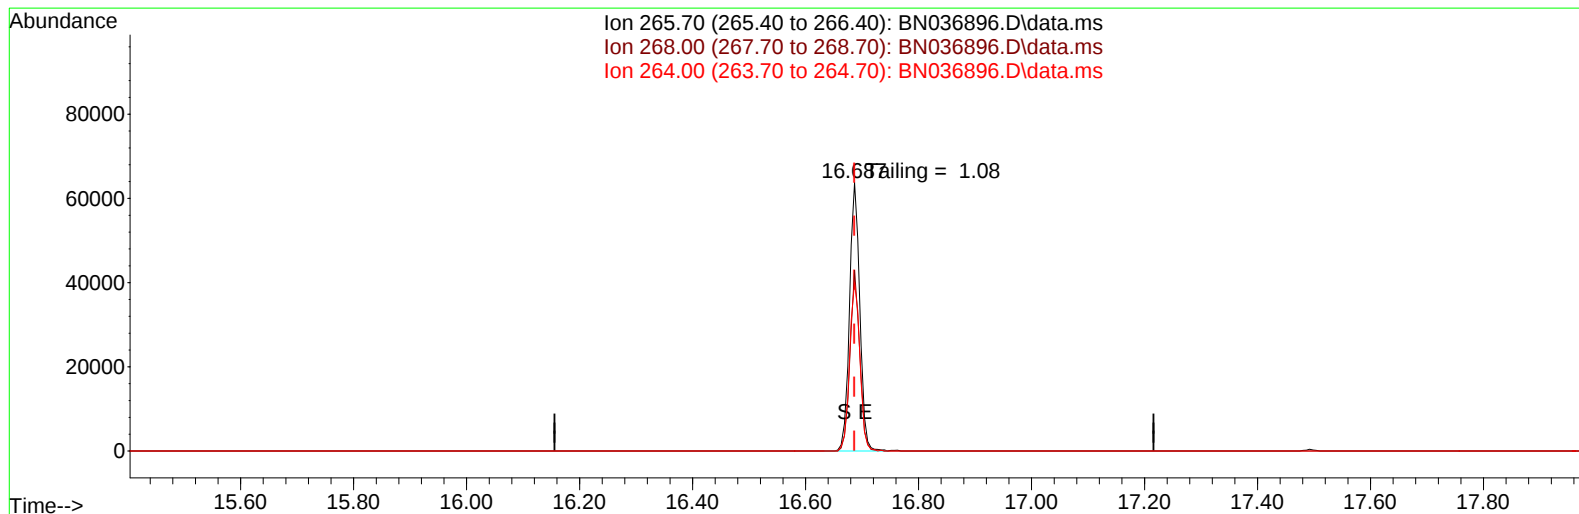

TIC: BN036896.D\data.ms

(70) Pentachlorophenol (C)

16.687min (+ 0.001) 15197.46 ng




response 80743

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.34
264.00	61.60	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041425\
Data File : BN036896.D
Acq On : 14 Apr 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 14 19:23:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

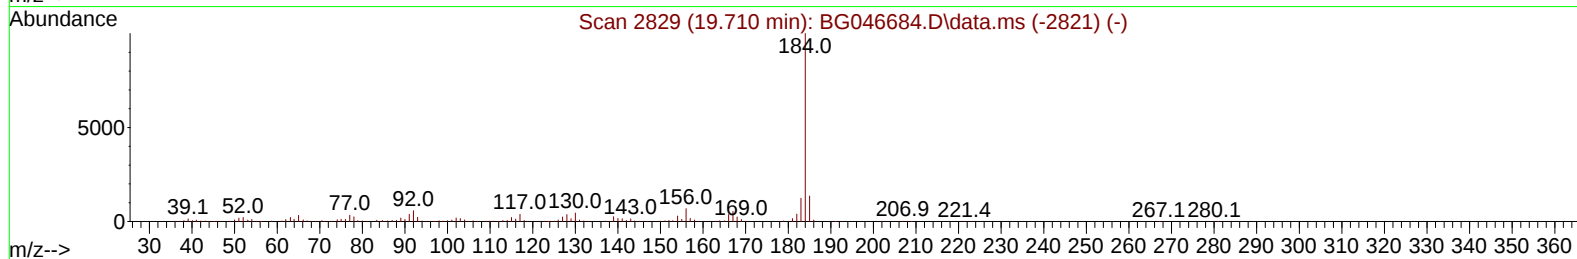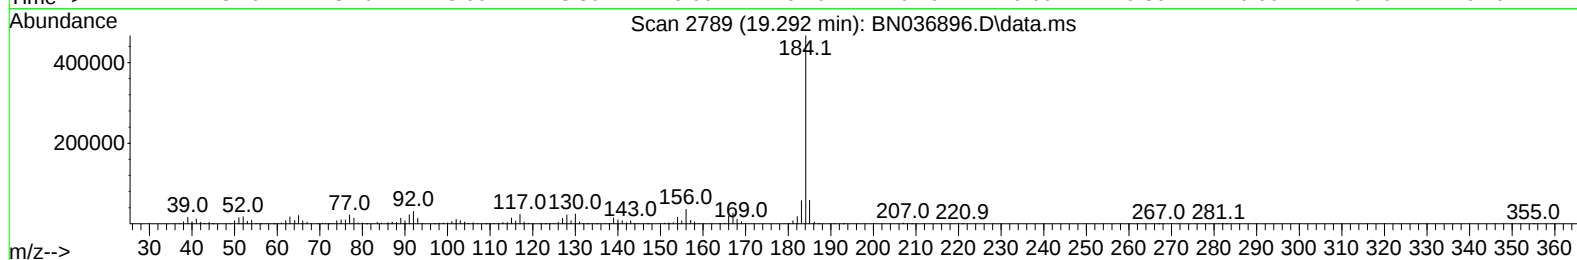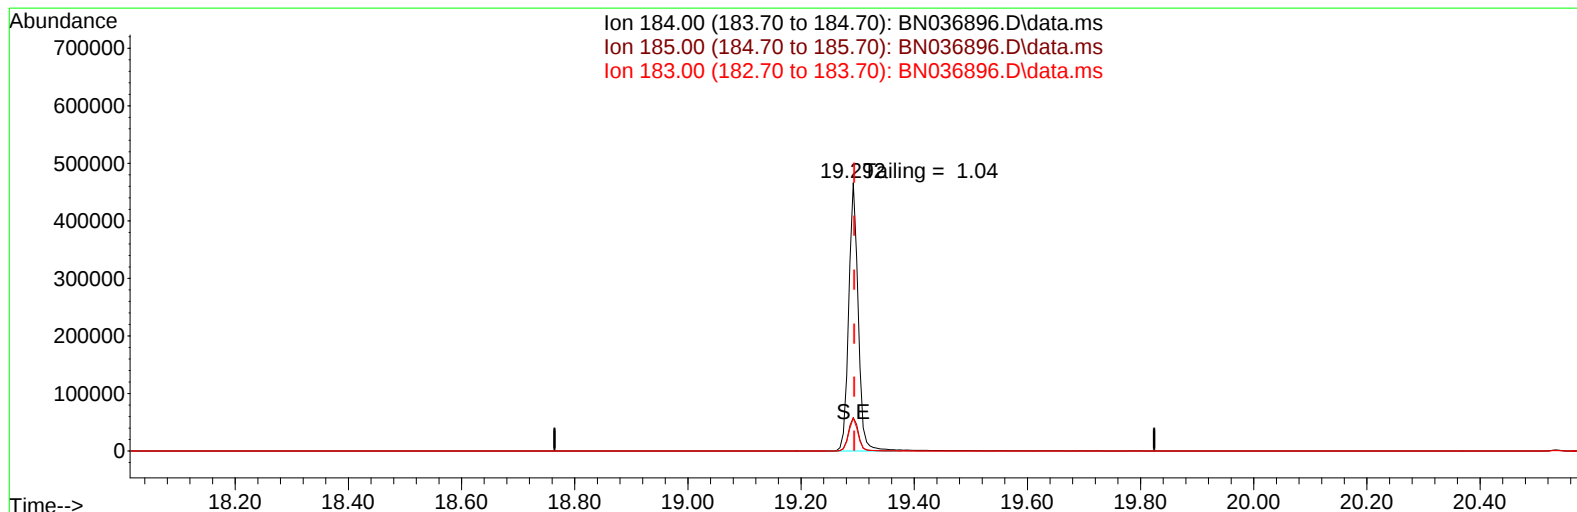

TIC: BN036896.D\data.ms

(77) Benzidine

19.292min (-0.002) 0.00 ng

response 549129

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.46
183.00	13.20	12.25
0.00	0.00	0.00