


LB135354

7471B

INSTRUMENT ID: CV1

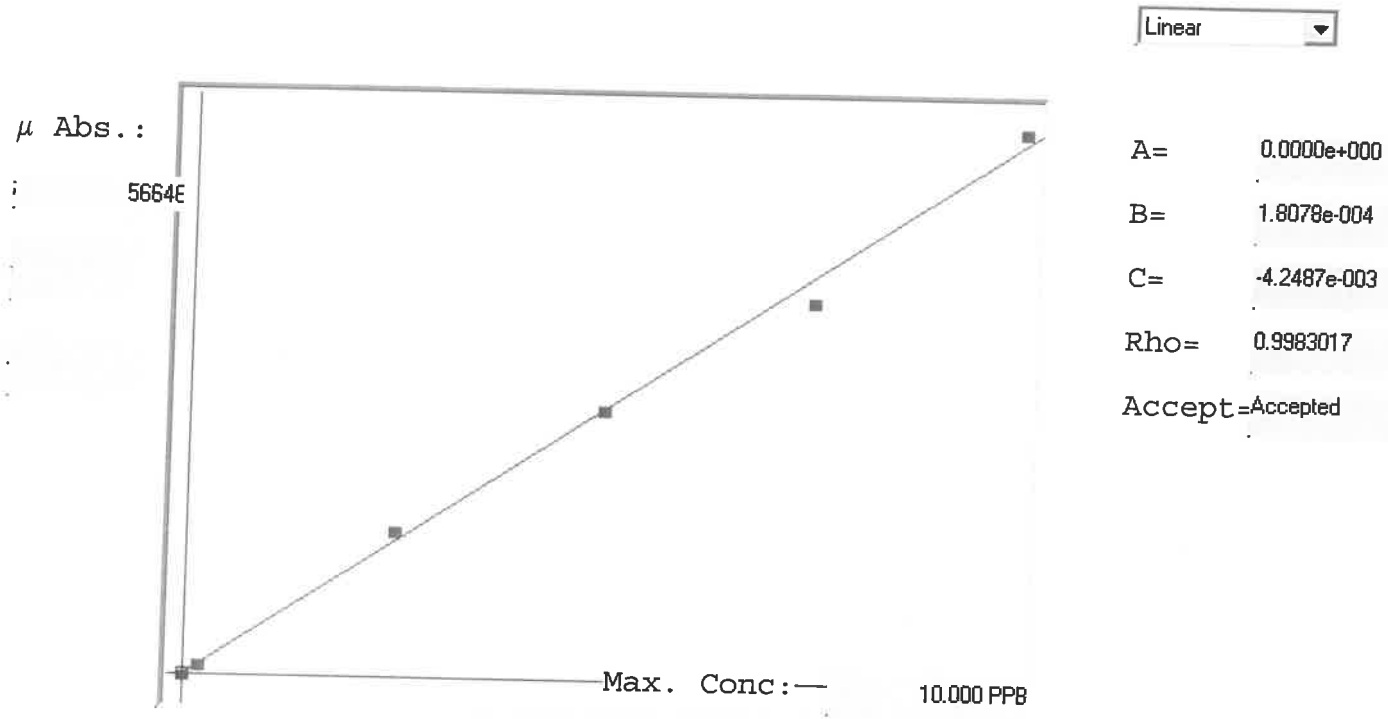

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.004	0.004	46	0.000	46					0/11
0.2	0.200	0.176	-0.024	998	0.0 %	998					-12
2.5	2.500	2.692	0.192	14914	0.0 %	14914					8
5.0	5.000	5.021	0.021	27796	0.0 %	27796					0
7.5	7.500	7.071	-0.429	39140	0.0 %	39140					-6
10.0	10.000	10.236	0.236	56646	0.0 %	56646					2

LB135354 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 09 Apr 2025 10:53:09

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	46	-	0.0000	7471B	PPB	09 Apr 2025 11:06:45	S	Std
0.2 - 1	50.2	998	-	0.2000	7471B	PPB	09 Apr 2025 11:09:03	S	Std
2.5 - 1	72.5	14914	-	2.5000	7471B	PPB	09 Apr 2025 11:11:20	S	Std
5.0 - 1	51	27796	-	5.0000	7471B	PPB	09 Apr 2025 11:13:36	S	Std
7.5 - 1	57.5	39140	-	7.5000	7471B	PPB	09 Apr 2025 11:15:55	S	Std
10.0 - 1	51	56646	-	10.0000	7471B	PPB	09 Apr 2025 11:31:05	S	Std
ICV82 - 1	ICV82	20031	3.6169	-	7471B	PPB	09 Apr 2025 11:34:23	U	SMPL
ICB82 - 1	ICB82	-327	-0.0634	-	7471B	PPB	09 Apr 2025 11:36:38	U	SMPL
CCV49 - 1	CCV49	28389	5.1278	-	7471B	PPB	09 Apr 2025 11:43:16	U	SMPL
CCB49 - 1	CCB49	-272	-0.0534	-	7471B	PPB	09 Apr 2025 11:45:31	U	SMPL
CRA - 1	CRA	976	0.1722	-	7471B	PPB	09 Apr 2025 11:47:51	U	SMPL
HighStd - 1	HighStd	56708	10.2472	-	7471B	PPB	09 Apr 2025 11:50:07	U	SMPL
ChkStd - 1	ChkStd	35877	6.4815	-	7471B	PPB	09 Apr 2025 11:52:23	U	SMPL
PB167532BL - 1	PBS	97	0.0133	-	7471B	PPB	09 Apr 2025 11:58:46	U	SMPL
PB167532BS - 1	LCSS	20099	3.6292	-	7471B	PPB	09 Apr 2025 12:03:44	U	SMPL
Q1742-01 - 1	TR-06-040725	3519	0.6319	-	7471B	PPB	09 Apr 2025 12:05:59	U	SMPL
Q1744-01 - 1	B-158-SB01	1605	0.2859	-	7471B	PPB	09 Apr 2025 12:08:19	U	SMPL
Q1744-03 - 1	B-158-SB02	5376	0.9676	-	7471B	PPB	09 Apr 2025 12:10:39	U	SMPL
Q1745-01 - 1	IB-6A-WC	572527	HIGH	-	7471B	PPB	09 Apr 2025 12:12:57	X	
Q1745-09 - 1	IB-6.5-WC	71324	12.8894	-	7471B	PPB	09 Apr 2025 12:14:47	U	SMPL
CCV50 - 1	CCV50	26600	4.8044	-	7471B	PPB	09 Apr 2025 12:17:55	U	SMPL
CCB50 - 1	CCB50	-468	-0.0889	-	7471B	PPB	09 Apr 2025 12:20:26	U	SMPL
Q1746-01 - 1	B-149-SB01	43051	7.7783	-	7471B	PPB	09 Apr 2025 12:22:45	U	SMPL
Q1746-03 - 1	B-149-SB02	-126	-0.0270	-	7471B	PPB	09 Apr 2025 12:25:01	U	SMPL
Q1747-01 - 1	ARS20-0008	195	0.0310	-	7471B	PPB	09 Apr 2025 12:27:27	U	SMPL
Q1748-01 - 1	IB-1.5-WC	159931	28.9074	-	7471B	PPB	09 Apr 2025 12:29:42	U	SMPL
Q1748-05 - 1	IB-2A-WC	44324	8.0085	-	7471B	PPB	09 Apr 2025 12:31:58	U	SMPL
Q1749-01 - 1	TP-14	963	0.1698	-	7471B	PPB	09 Apr 2025 12:34:40	U	SMPL
Q1752-01 - 1	TP-1	1483	0.2638	-	7471B	PPB	09 Apr 2025 12:37:05	U	SMPL
Q1752-03 - 1	TP-2	35238	6.3659	-	7471B	PPB	09 Apr 2025 12:39:22	U	SMPL
Q1752-05 - 1	TP-3	1095	0.1937	-	7471B	PPB	09 Apr 2025 12:41:40	U	SMPL
Q1752-07 - 1	TP-4	5241	0.9432	-	7471B	PPB	09 Apr 2025 12:44:01	U	SMPL
CCV51 - 1	CCV51	28077	5.0714	-	7471B	PPB	09 Apr 2025 12:46:16	U	SMPL
CCB51 - 1	CCB51	-348	-0.0672	-	7471B	PPB	09 Apr 2025 12:48:34	U	SMPL
Q1753-01 - 1	WC-1	81	0.0104	-	7471B	PPB	09 Apr 2025 12:53:07	U	SMPL
Q1753-05 - 1	WC-2	1958	0.3497	-	7471B	PPB	09 Apr 2025 12:55:22	U	SMPL
Q1753-05DUP - 1	WC-2DUP	2067	0.3694	-	7471B	PPB	09 Apr 2025 12:57:38	U	SMPL
Q1753-05MS - 1	WC-2MS	17067	3.0811	-	7471B	PPB	09 Apr 2025 12:59:54	U	SMPL
Q1753-05MSD - 1	WC-2MSD	14371	2.5937	-	7471B	PPB	09 Apr 2025 13:02:09	U	SMPL
Q1753-05LX5 - 1		438	0.0749	-	7471B	PPB	09 Apr 2025 13:34:29	U	SMPL
Q1753-05A - 1		19337	3.4914	-	7471B	PPB	09 Apr 2025 13:36:45	U	SMPL
Q1745-01DLX10 - 1		140670	25.4255	-	7471B	PPB	09 Apr 2025 13:41:22	U	SMPL
Q1745-09DLX5 - 1		16179	2.9205	-	7471B	PPB	09 Apr 2025 13:48:40	U	SMPL
Q1748-01DLX5 - 1		26371	4.7630	-	7471B	PPB	09 Apr 2025 13:56:38	U	SMPL
CCV52 - 1	CCV52	25494	4.6045	-	7471B	PPB	09 Apr 2025 13:58:54	U	SMPL
CCB52 - 1	CCB52	16	-0.0014	-	7471B	PPB	09 Apr 2025 14:04:52	U	SMPL
Q1745-01DL2X50 - 1		25538	4.6124	-	7471B	PPB	09 Apr 2025 14:13:49	U	SMPL
CCV53 - 1	CCV53	27475	4.9626	-	7471B	PPB	09 Apr 2025 14:18:49	U	SMPL
CCB53 - 1	CCB53	-526	-0.0993	-	7471B	PPB	09 Apr 2025 14:21:04	U	SMPL