
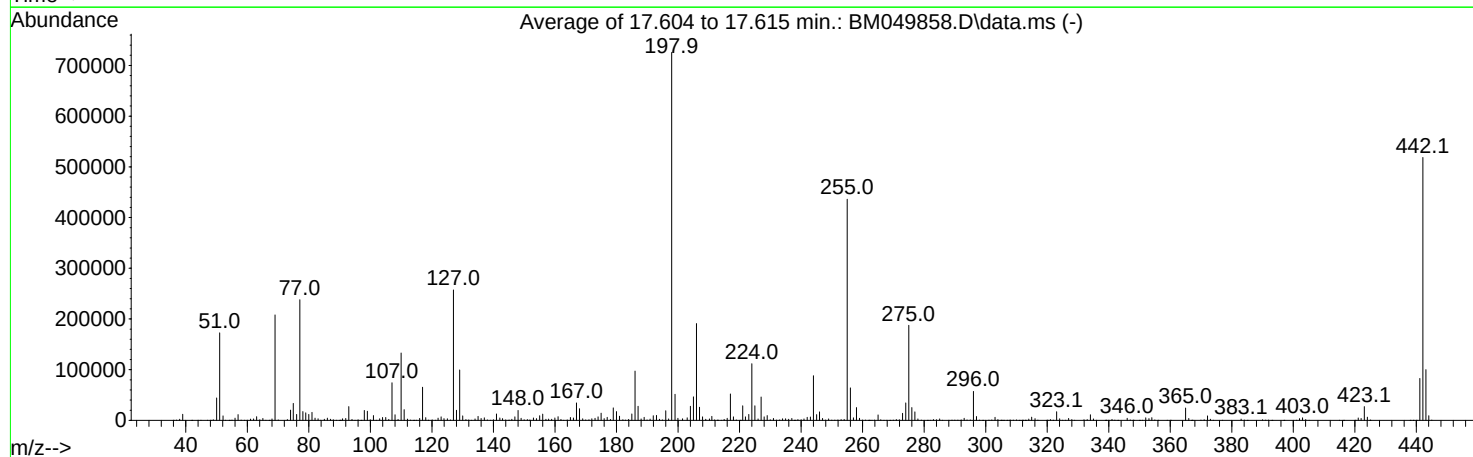


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040925\
Data File : BM049858.D
Acq On : 09 Apr 2025 08:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

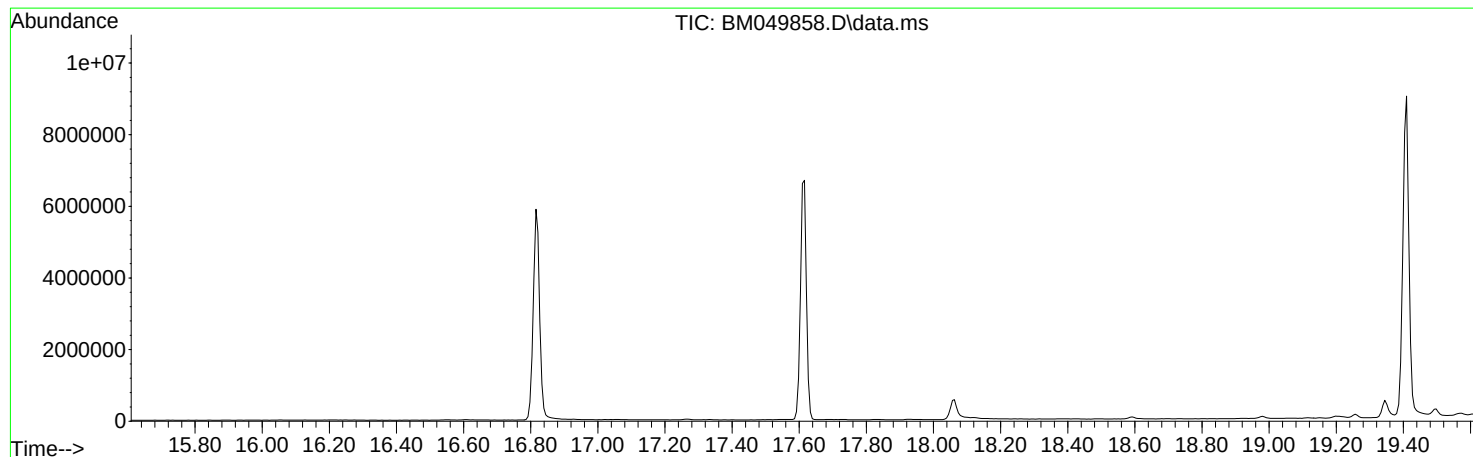

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	172767	PASS
68	69	0.00	2	1.4	2844	PASS
69	198	0.00	100	28.7	208079	PASS
70	69	0.00	2	0.5	979	PASS
127	198	10	80	35.4	257109	PASS
197	198	0.00	2	0.4	2927	PASS
198	198	100	100	100.0	725525	PASS
199	198	5	9	7.1	51557	PASS
275	198	10	60	25.8	187432	PASS
365	198	1	100	3.4	24319	PASS
441	198	0.01	100	11.4	82643	PASS
442	442	50	100	100.0	518613	PASS
443	442	15	24	19.3	100059	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/9/2025	BNA_M	<u>BM049858.D</u>
Compound Name	Response	Retention Time
DDT	2465394	20.645
DDD	31585	20.262
DDE	2023	19.698
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33608	2499002	1.34

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040925\
Data File : BM049858.D
Acq On : 09 Apr 2025 08:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 09 11:47:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

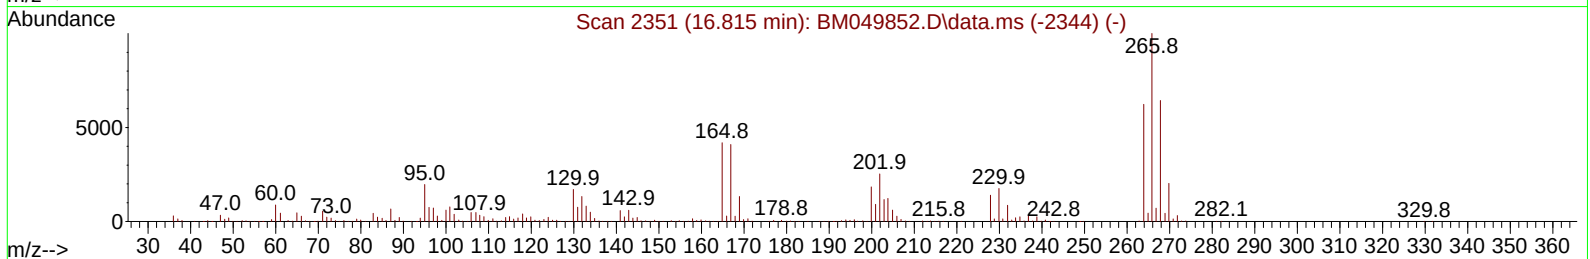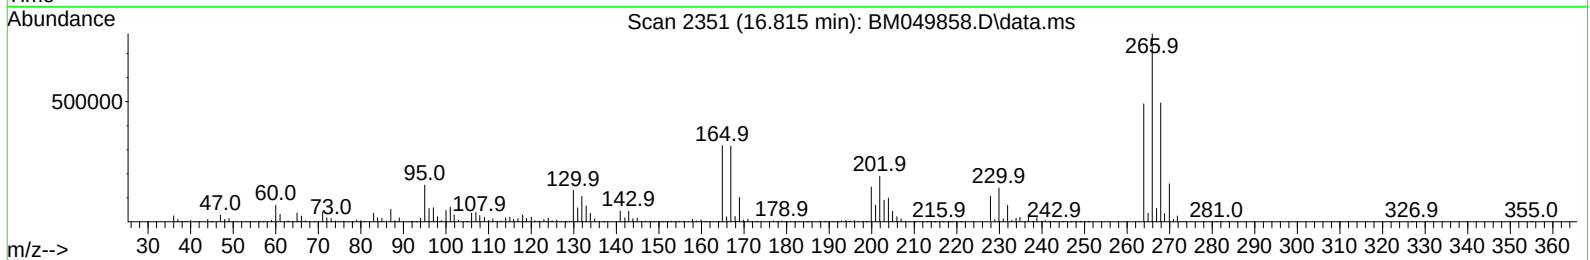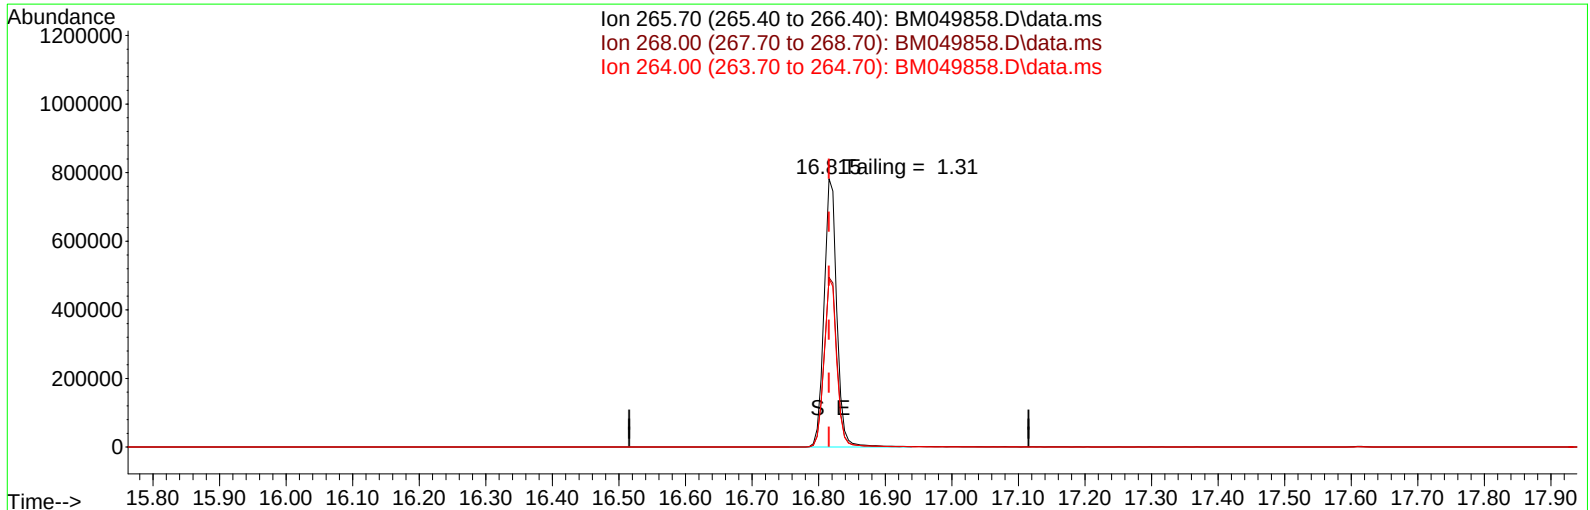

TIC: BM049858.D\data.ms

(70) Pentachlorophenol (C)

16.815min (-0.000) 710298.89 ng




response 1044481

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.17
264.00	62.30	62.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040925\
Data File : BM049858.D
Acq On : 09 Apr 2025 08:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 09 11:47:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

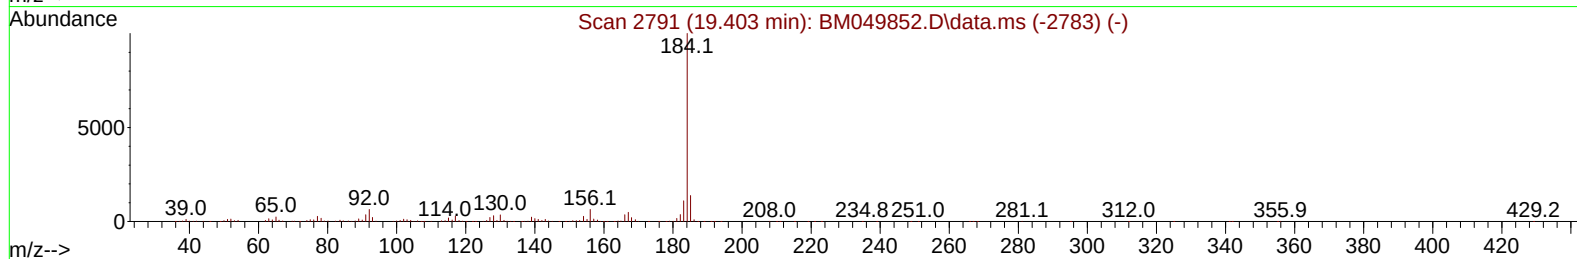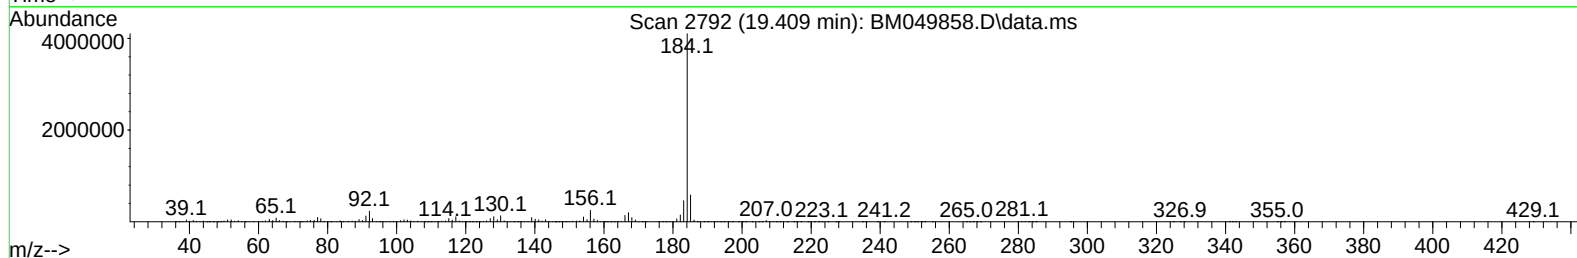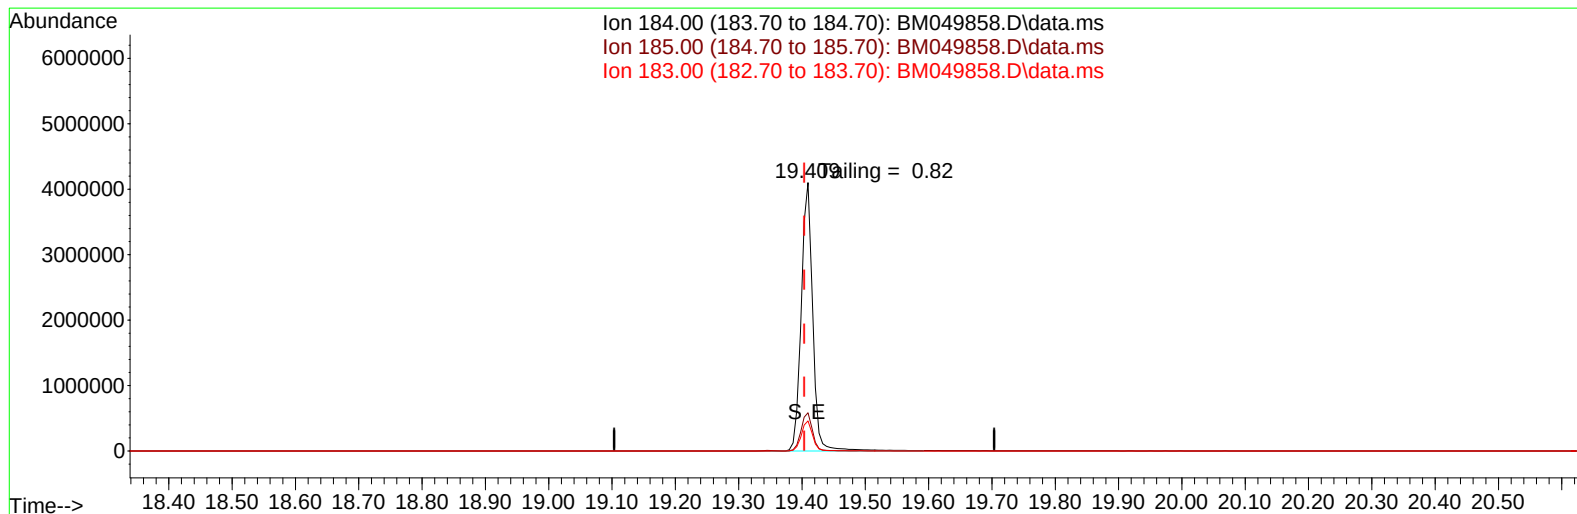

TIC: BM049858.D\data.ms

(77) Benzidine

19.409min (+ 0.006) 7036.51 ng

response 5211317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.26
183.00	11.00	11.25
0.00	0.00	0.00