
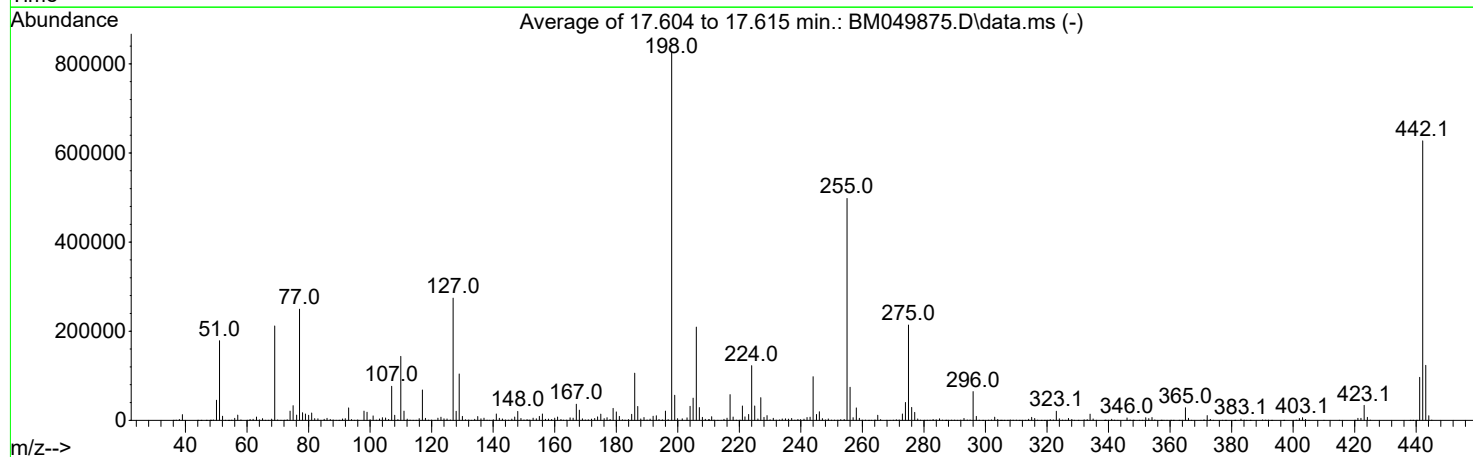


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041025\
Data File : BM049875.D
Acq On : 10 Apr 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

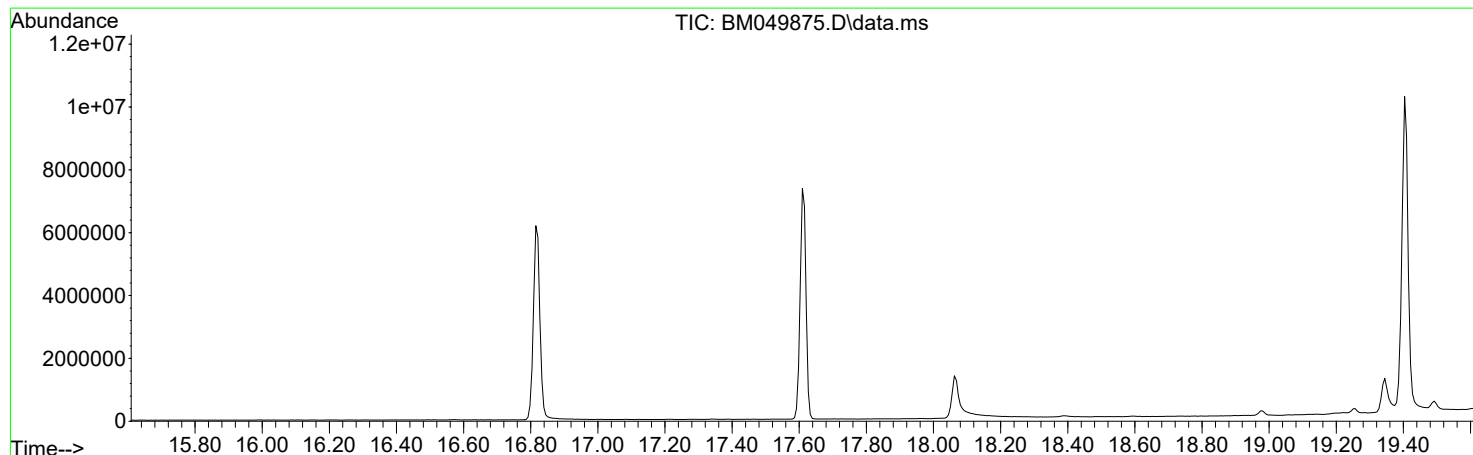

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.6	178667	PASS
68	69	0.00	2	1.4	2914	PASS
69	198	0.00	100	25.7	212021	PASS
70	69	0.00	2	0.5	1019	PASS
127	198	10	80	33.2	274475	PASS
197	198	0.00	2	0.2	1888	PASS
198	198	100	100	100.0	825515	PASS
199	198	5	9	6.8	56387	PASS
275	198	10	60	25.9	214123	PASS
365	198	1	100	3.4	28392	PASS
441	198	0.01	100	11.7	96741	PASS
442	442	50	100	100.0	627136	PASS
443	442	15	24	19.7	123464	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/10/2025	BNA_M	<u>BM049875.D</u>
Compound Name	Response	Retention Time
DDT	2746524	20.644
DDD	35768	20.256
DDE	2756	19.698
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38524	2785048	1.38

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041025\
Data File : BM049875.D
Acq On : 10 Apr 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 10 12:01:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

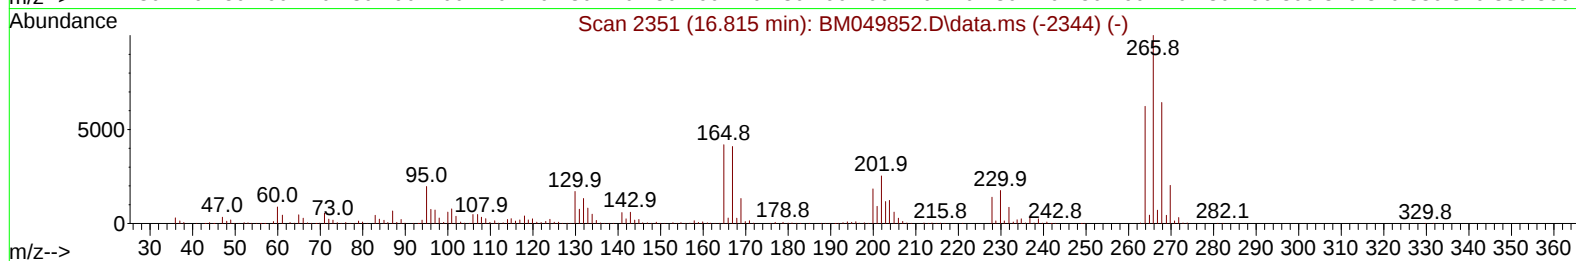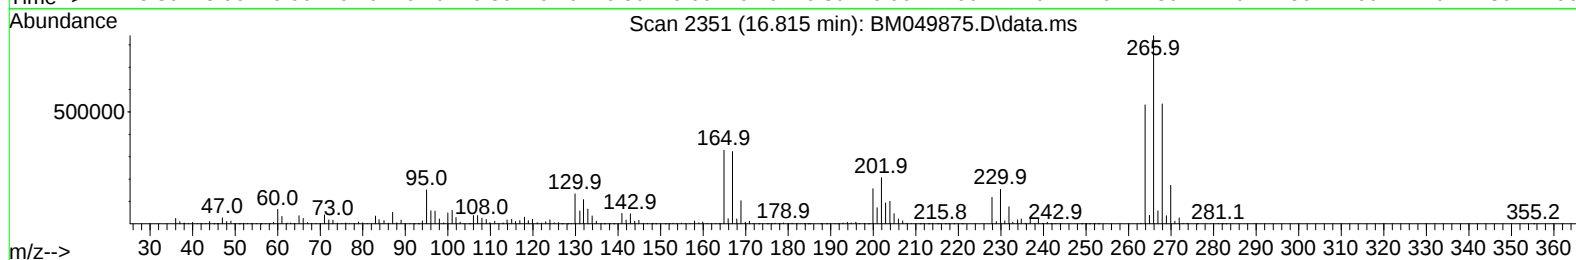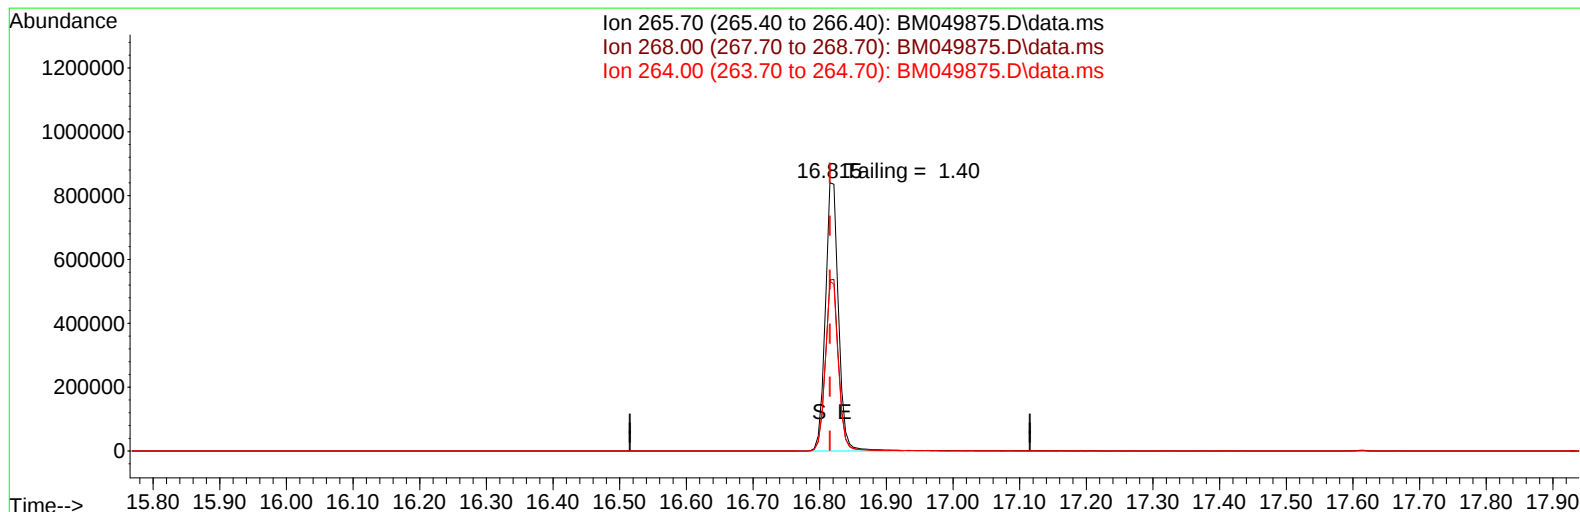

TIC: BM049875.D\data.ms

(70) Pentachlorophenol (C)

16.815min (-0.000) 211954.15 ng




response 1151118

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.75
264.00	62.30	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041025\
Data File : BM049875.D
Acq On : 10 Apr 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 10 12:01:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

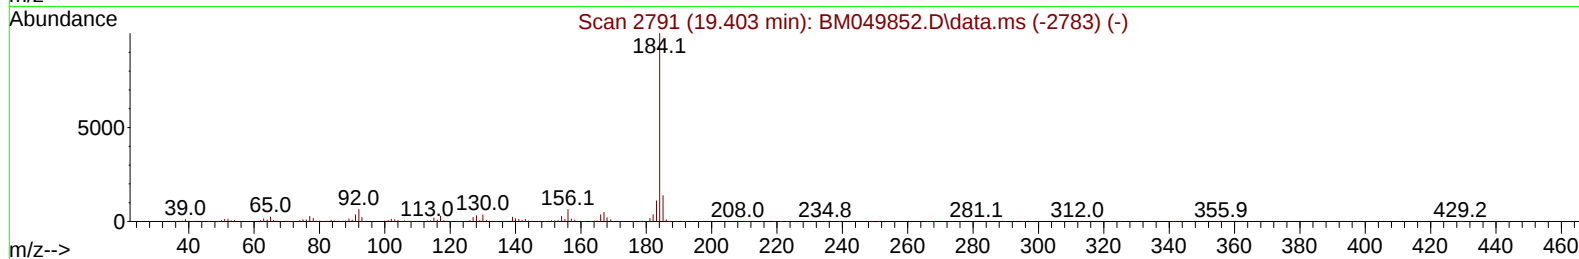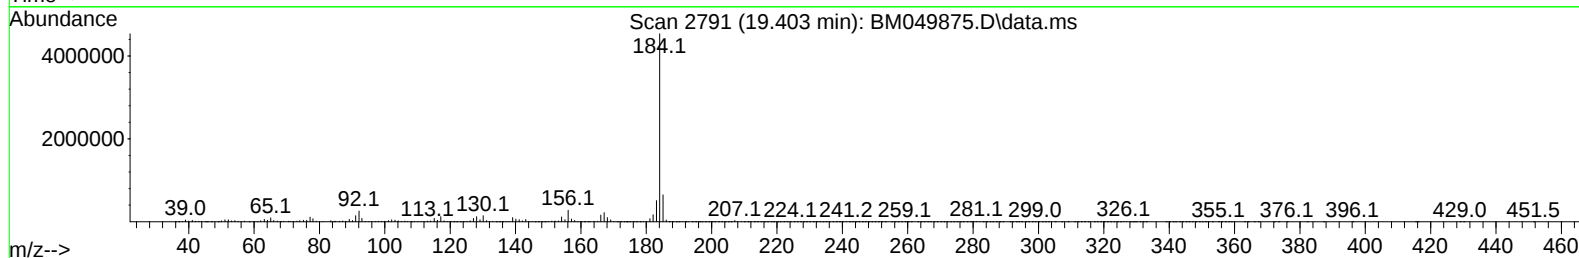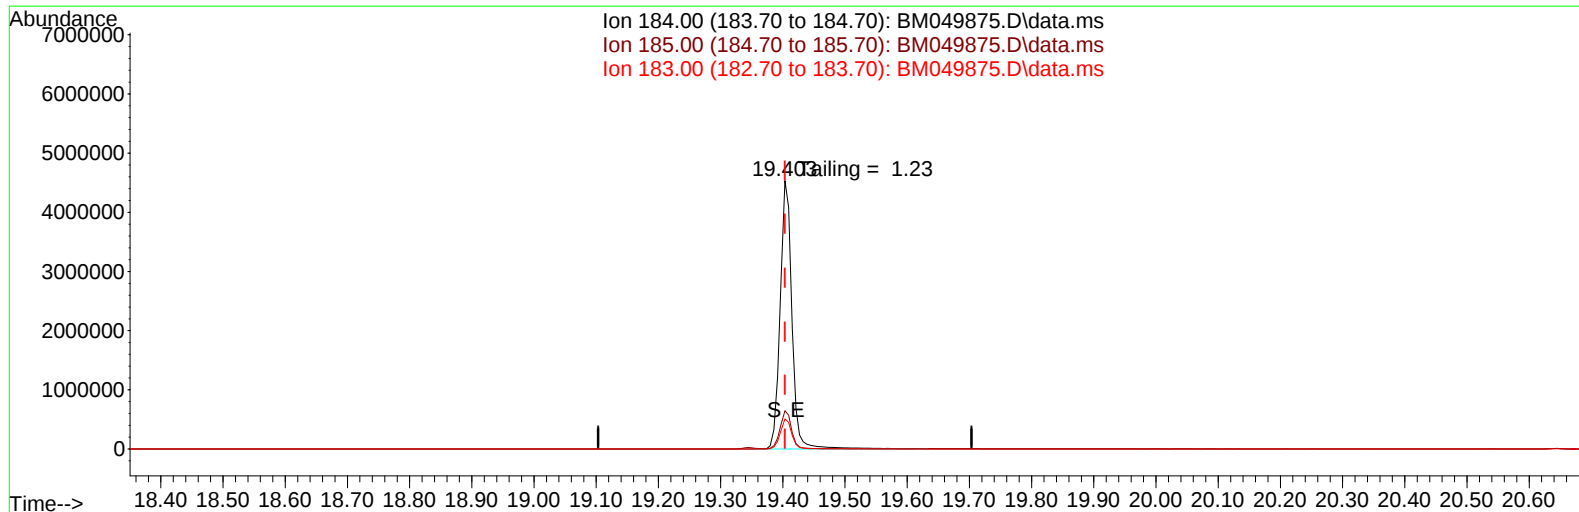

TIC: BM049875.D\data.ms

(77) Benzidine

19.403min (-0.000) 194071.13 ng

response 5998885

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.29
183.00	11.00	11.22
0.00	0.00	0.00