
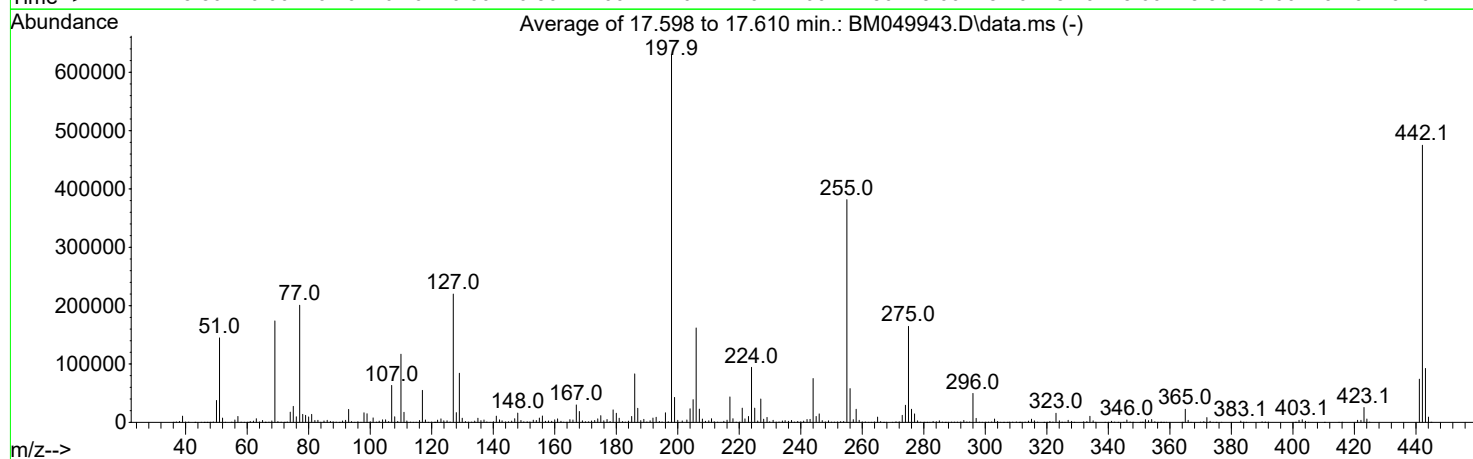


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041625\
Data File : BM049943.D
Acq On : 16 Apr 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

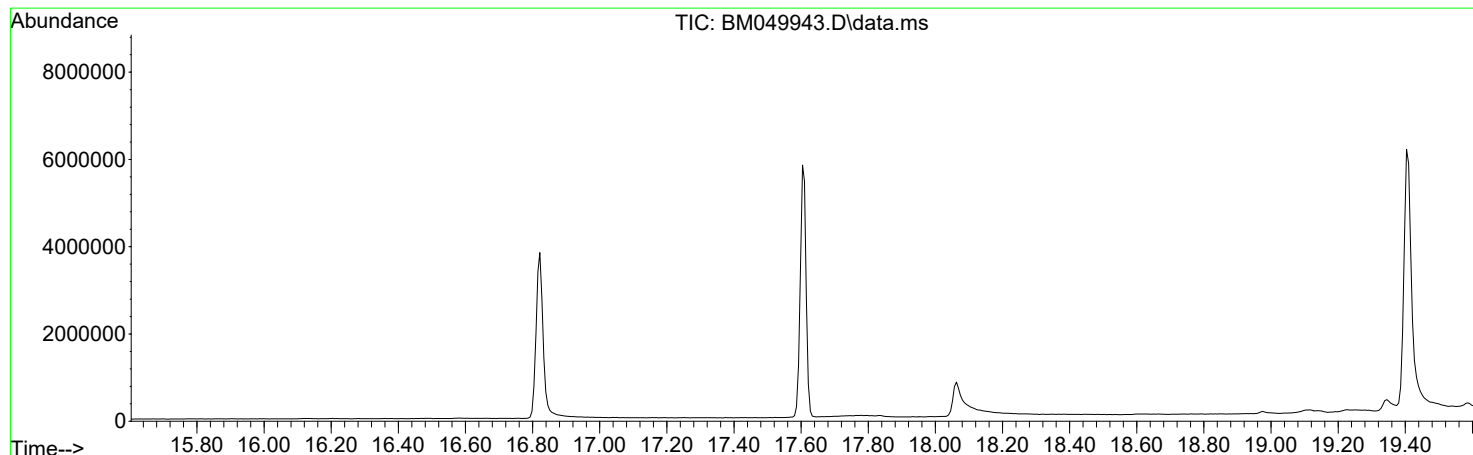

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	144954	PASS
68	69	0.00	2	1.5	2535	PASS
69	198	0.00	100	27.6	173898	PASS
70	69	0.00	2	0.7	1264	PASS
127	198	10	80	34.9	219925	PASS
197	198	0.00	2	0.1	865	PASS
198	198	100	100	100.0	630485	PASS
199	198	5	9	6.8	42927	PASS
275	198	10	60	26.1	164576	PASS
365	198	1	100	3.6	22401	PASS
441	198	0.01	100	11.7	73973	PASS
442	442	50	100	100.0	475008	PASS
443	442	15	24	19.4	92325	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/16/2025	BNA_M	<u>BM049943.D</u>
Compound Name	Response	Retention Time
DDT	1961082	20.645
DDD	51139	20.204
DDE	2728	19.698
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53867	2014949	2.67

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041625\
Data File : BM049943.D
Acq On : 16 Apr 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 16 11:06:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

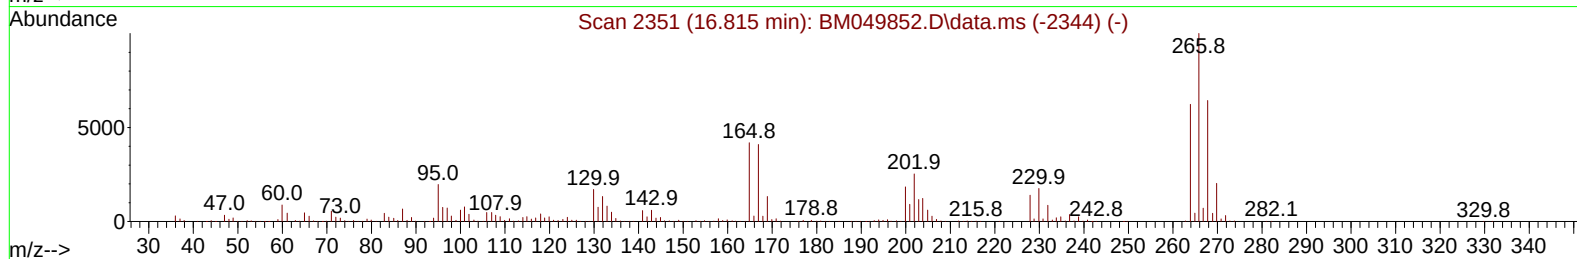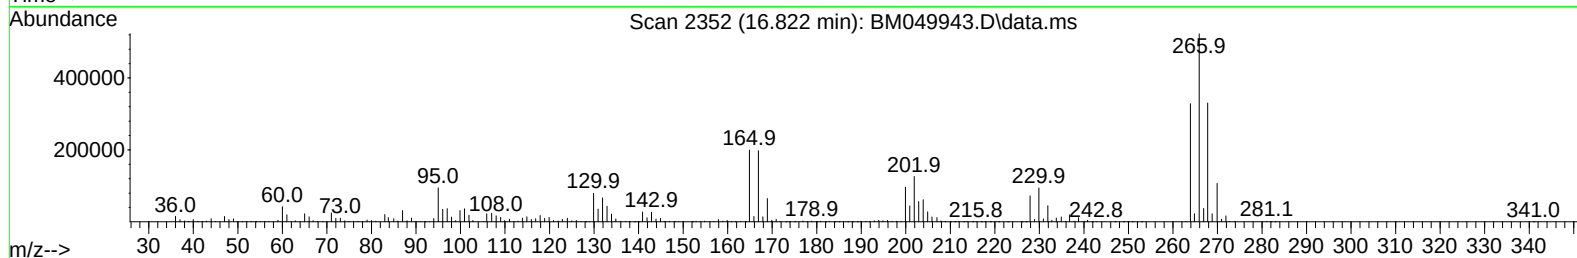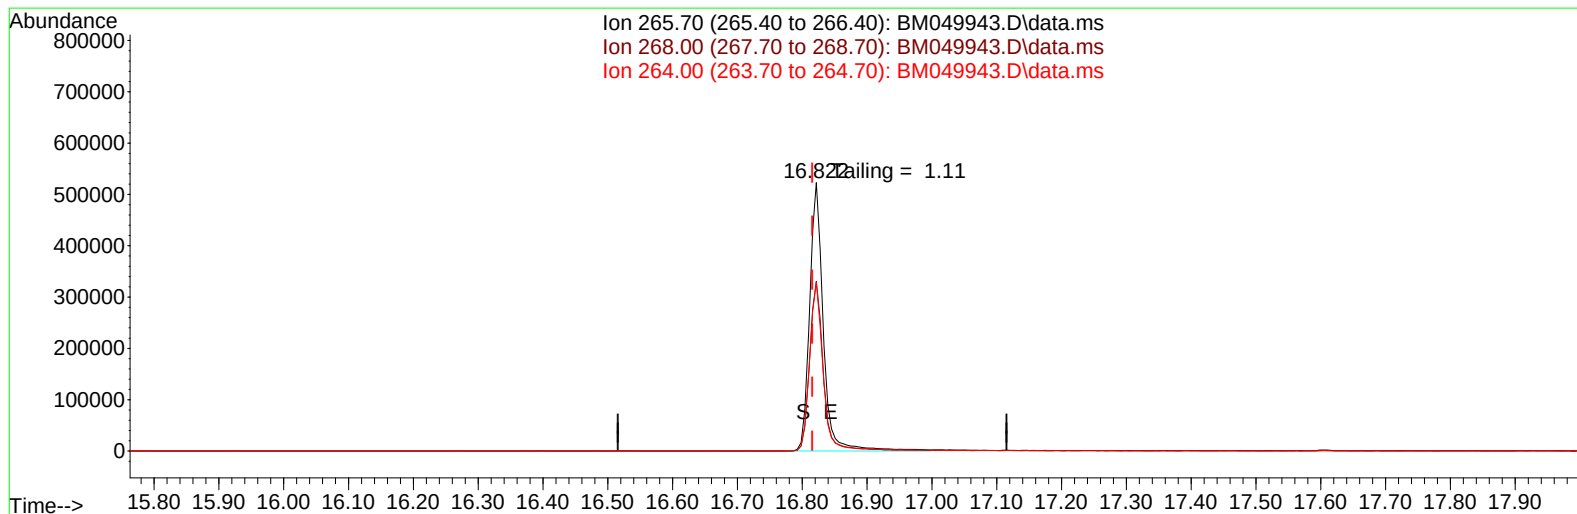

TIC: BM049943.D\data.ms

(70) Pentachlorophenol (C)

16.822min (+ 0.006) 1377107.60 ng




response 769504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.19
264.00	62.30	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041625\
Data File : BM049943.D
Acq On : 16 Apr 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 16 11:06:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

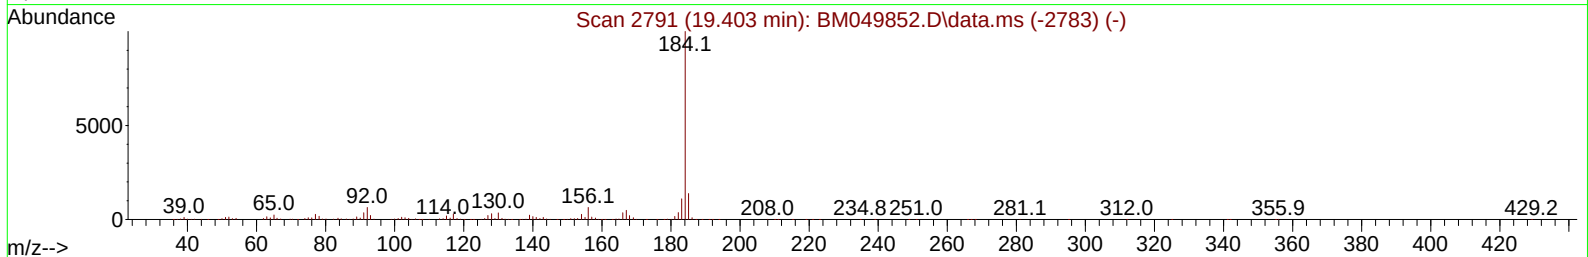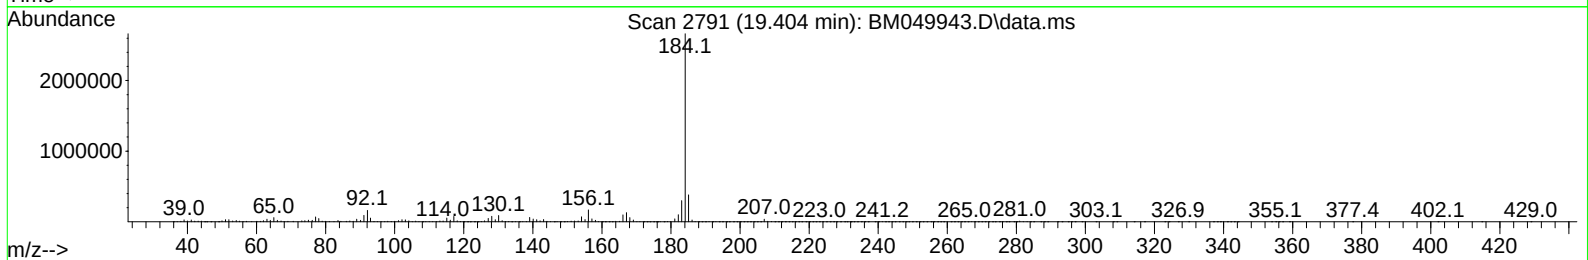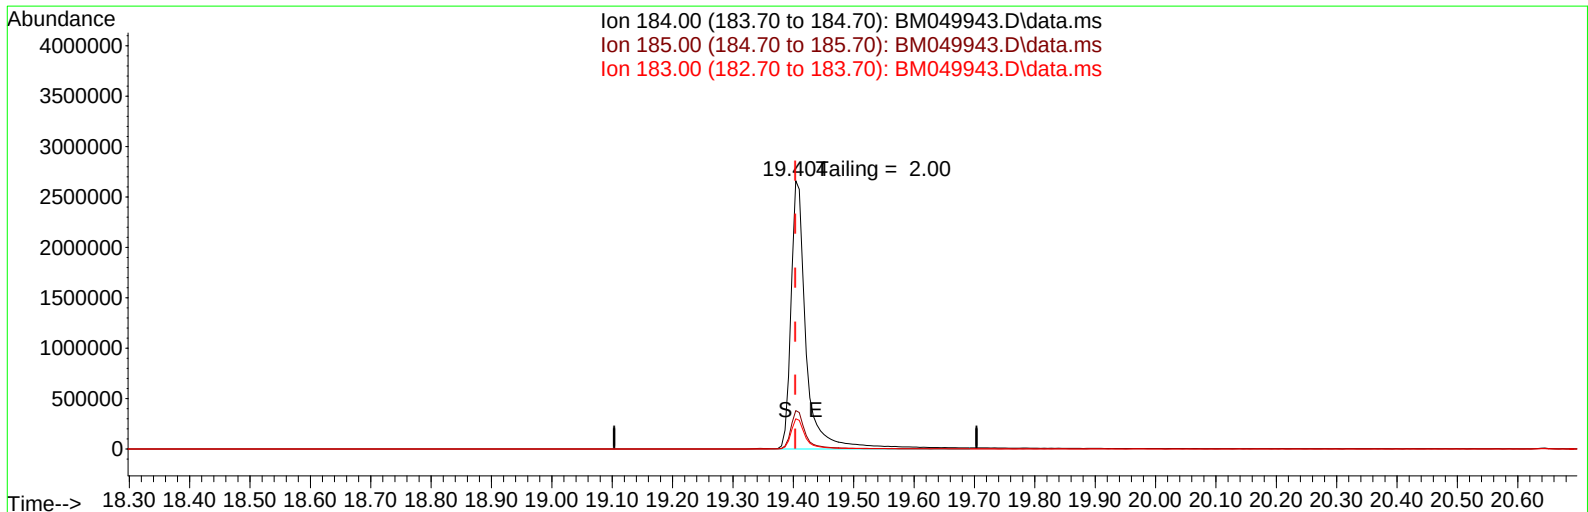

TIC: BM049943.D\data.ms

(77) Benzidine

19.404min (+ 0.000) 473739.12 ng

response 4713616

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.31
183.00	11.00	11.26
0.00	0.00	0.00