
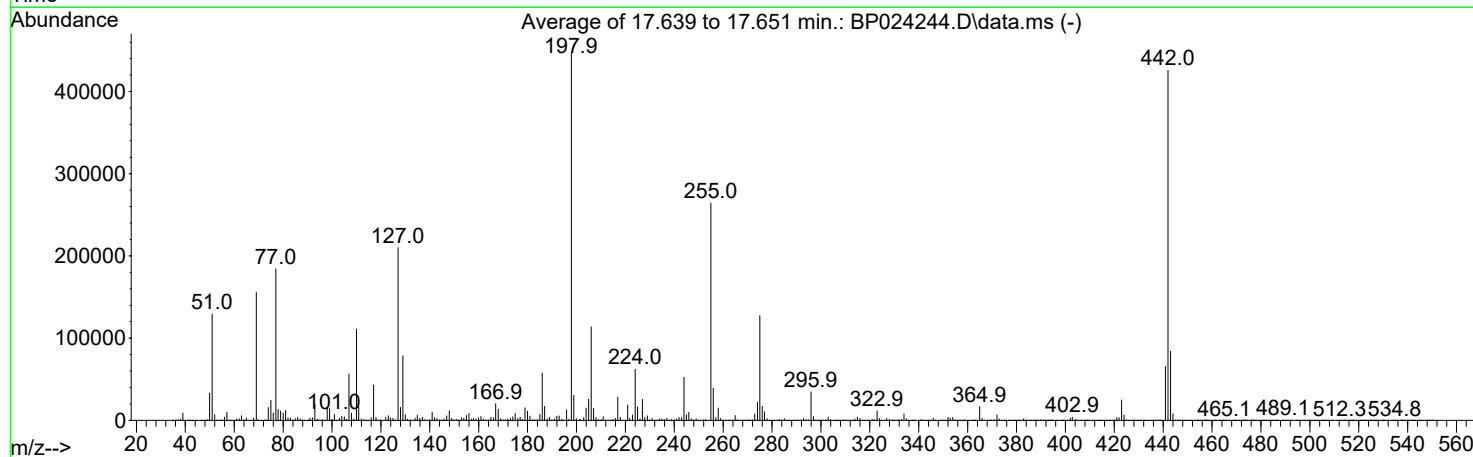


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041025\
Data File : BP024244.D
Acq On : 10 Apr 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 10 11:43:37 2025

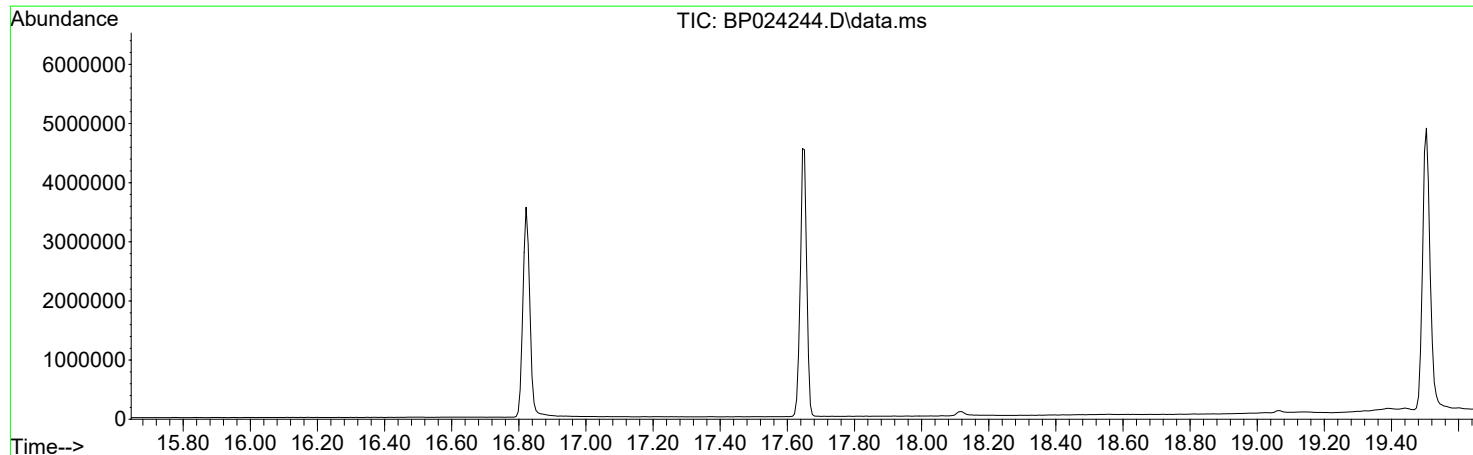

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	129060	PASS
68	69	0.00	2	1.7	2569	PASS
69	198	0.00	100	34.8	155535	PASS
70	69	0.00	2	0.5	814	PASS
127	198	10	80	47.0	210293	PASS
197	198	0.00	2	0.3	1397	PASS
198	198	100	100	100.0	447453	PASS
199	198	5	9	6.8	30328	PASS
275	198	10	60	28.5	127342	PASS
365	198	1	100	3.7	16767	PASS
441	198	0.01	100	14.6	65533	PASS
442	442	100	100	100.0	425856	PASS
443	442	15	24	19.7	84104	PASS

Instrument :
BNA_P
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/10/2025	BNA_P	<u>BP024244.D</u>
Compound Name	Response	Retention Time
DDT	1572605	20.798
DDD	41488	20.333
DDE	2088	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43576	1616181	2.70

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041025\
Data File : BP024244.D
Acq On : 10 Apr 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 10 14:43:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 10 11:43:37 2025
Response via : Initial Calibration

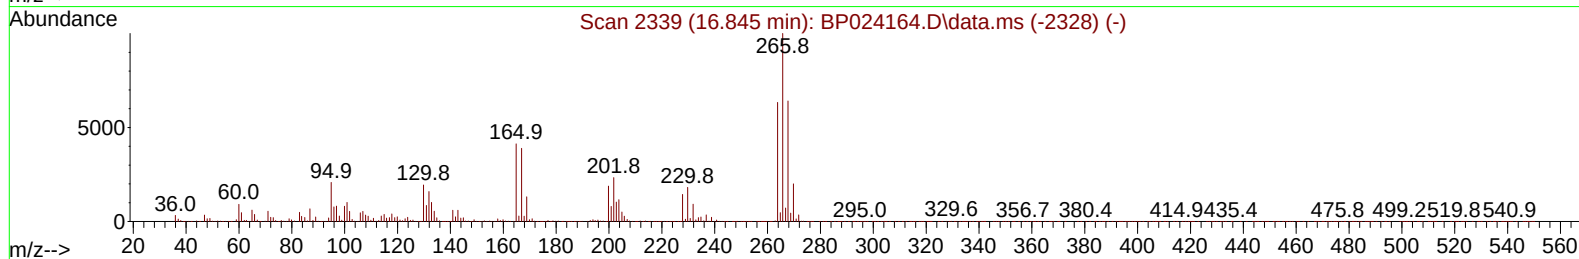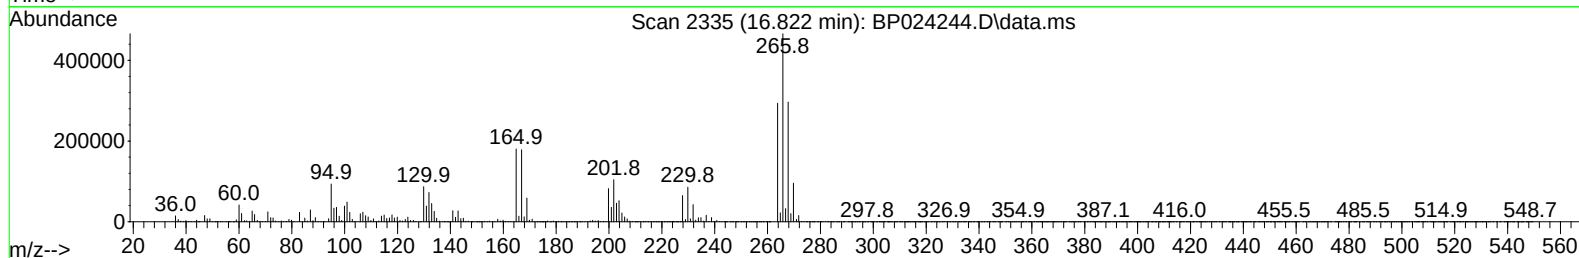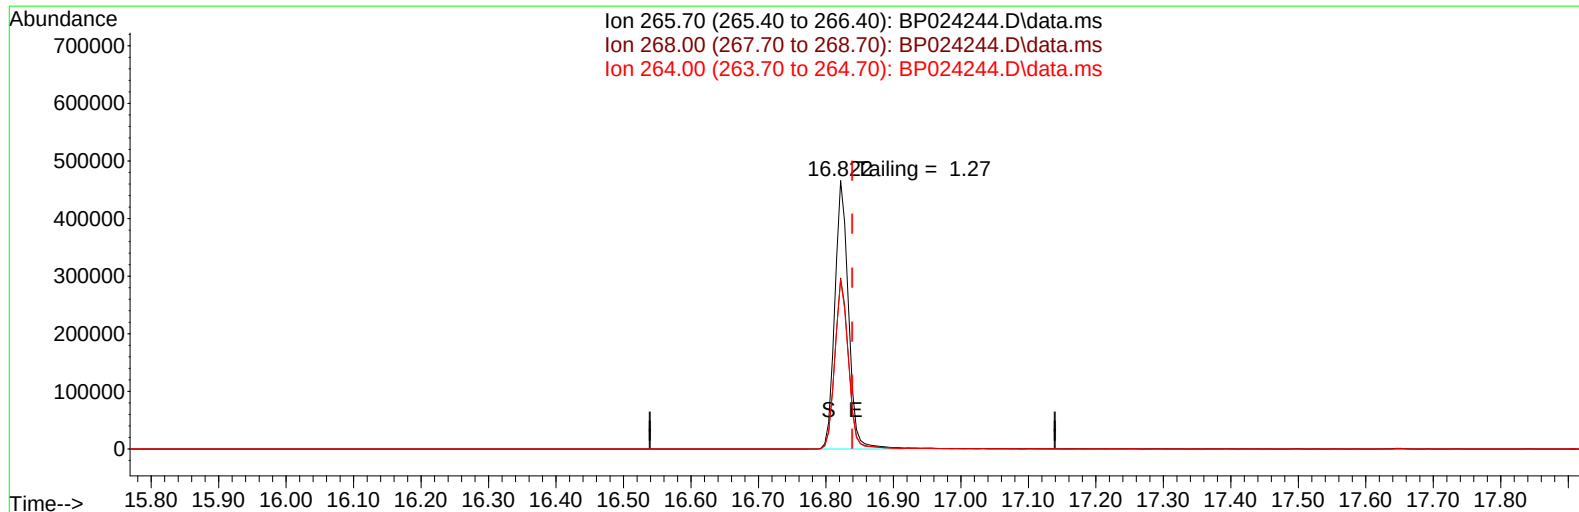

TIC: BP024244.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.018) 2689216.60 ng




response 655373

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.70
264.00	63.30	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041025\
Data File : BP024244.D
Acq On : 10 Apr 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 10 14:43:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 10 11:43:37 2025
Response via : Initial Calibration

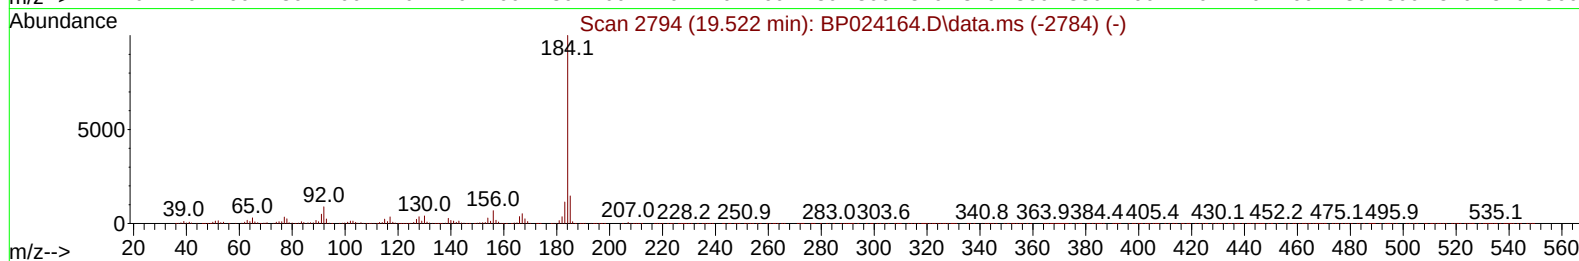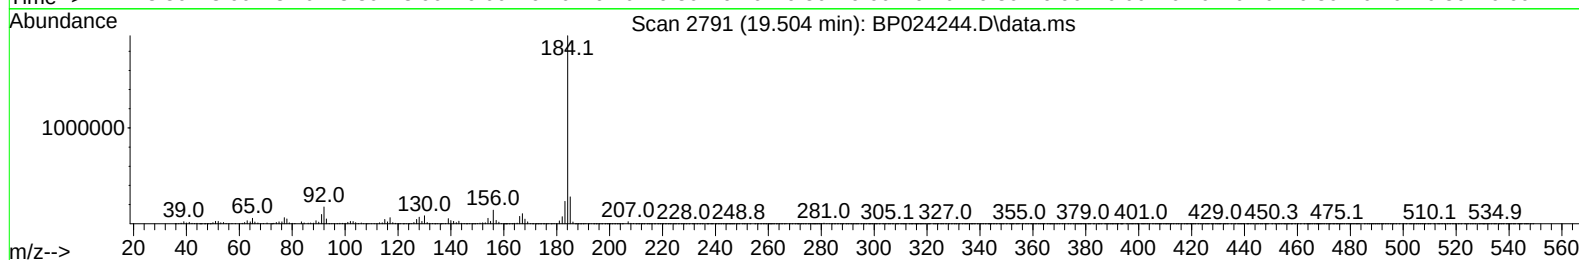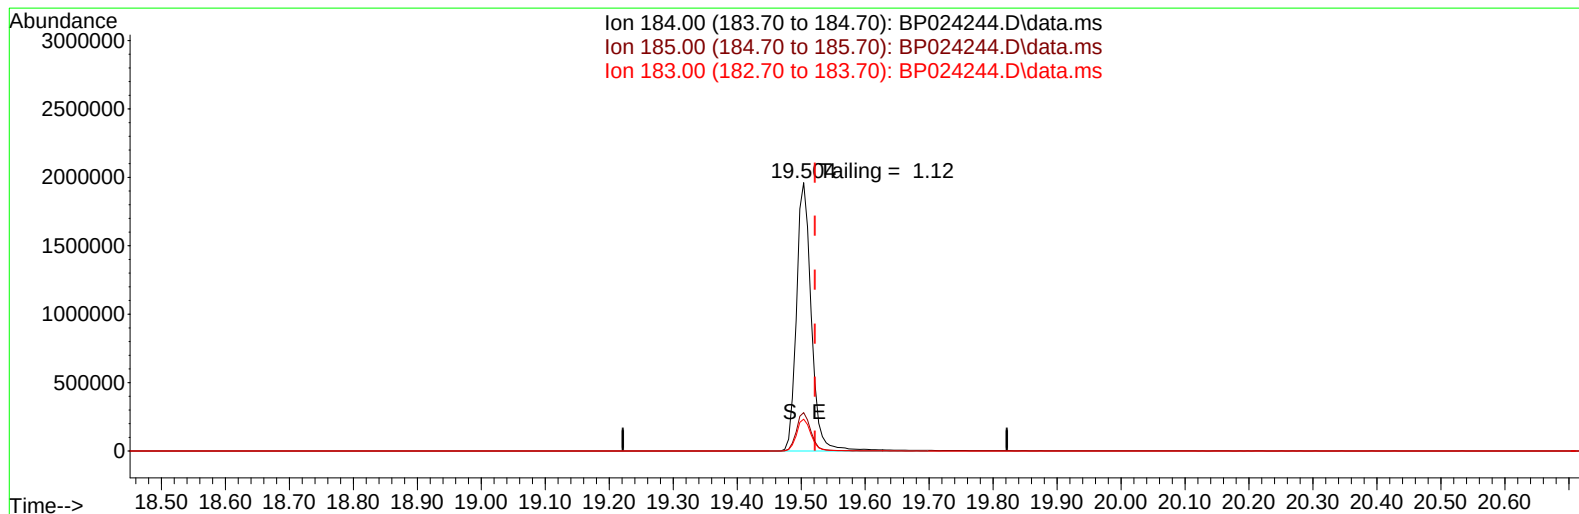

TIC: BP024244.D\data.ms

(77) Benzidine

19.504min (-0.018) 3933451.82 ng

response 3182452

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.33
183.00	11.40	11.89
0.00	0.00	0.00