
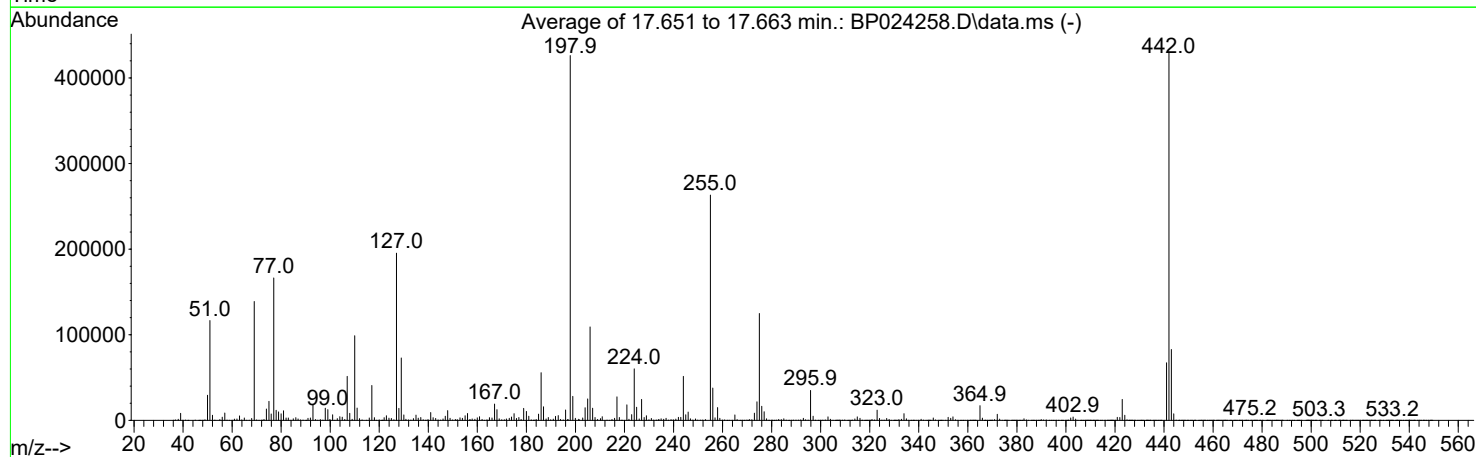


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041125\
Data File : BP024258.D
Acq On : 11 Apr 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 10 11:43:37 2025

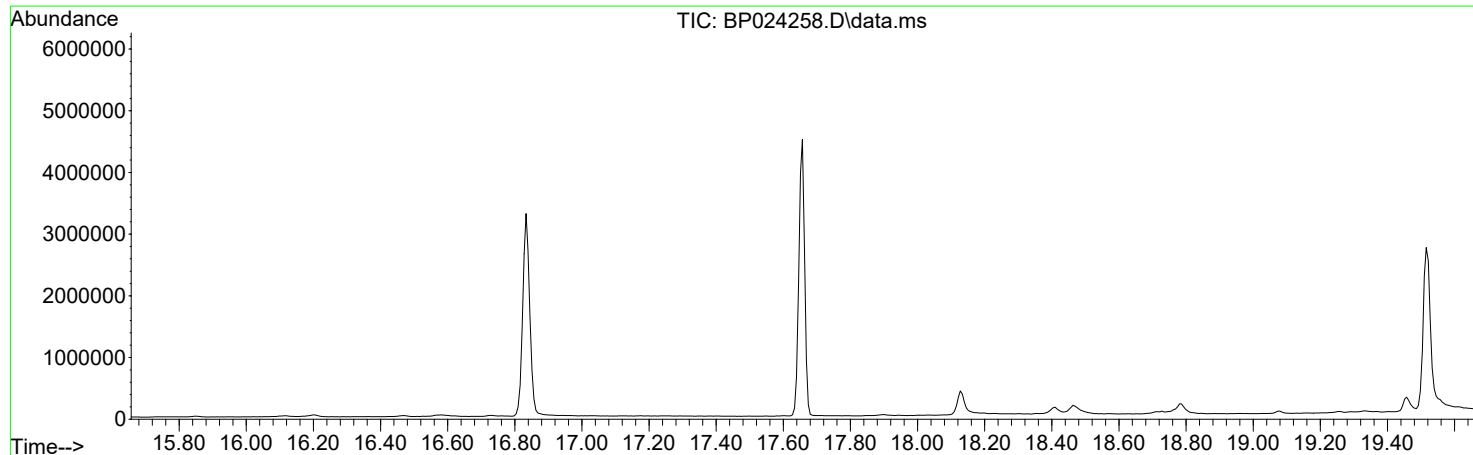

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	116544	PASS
68	69	0.00	2	1.6	2269	PASS
69	198	0.00	100	32.6	138884	PASS
70	69	0.00	2	0.5	666	PASS
127	198	10	80	45.8	195236	PASS
197	198	0.00	2	0.3	1196	PASS
198	198	100	100	100.0	426139	PASS
199	198	5	9	6.6	28093	PASS
275	198	10	60	29.3	124879	PASS
365	198	1	100	4.0	17122	PASS
441	198	0.01	100	15.8	67363	PASS
442	442	100	100	100.0	429674	PASS
443	442	15	24	19.3	82798	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/11/2025	BNA_P	<u>BP024258.D</u>
Compound Name	Response	Retention Time
DDT	1500117	20.81
DDD	28536	20.351
DDE	1243	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29779	1529896	1.95

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041125\
Data File : BP024258.D
Acq On : 11 Apr 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 11 11:43:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 10 11:43:37 2025
Response via : Initial Calibration

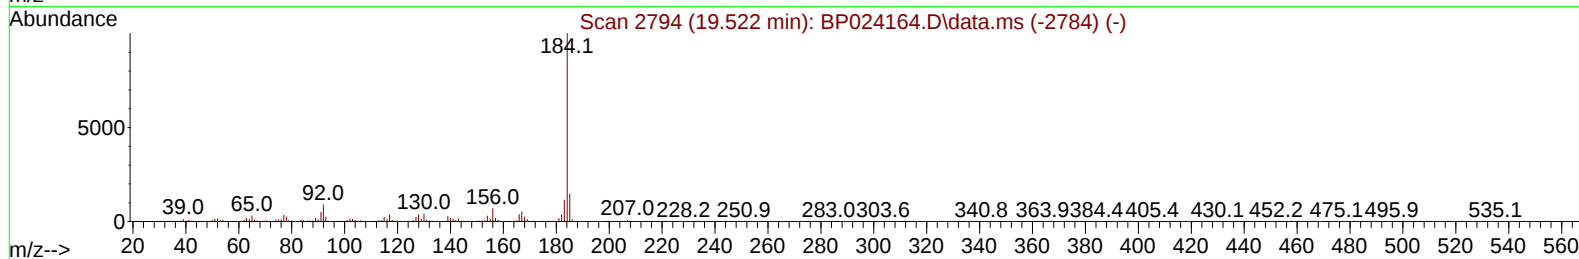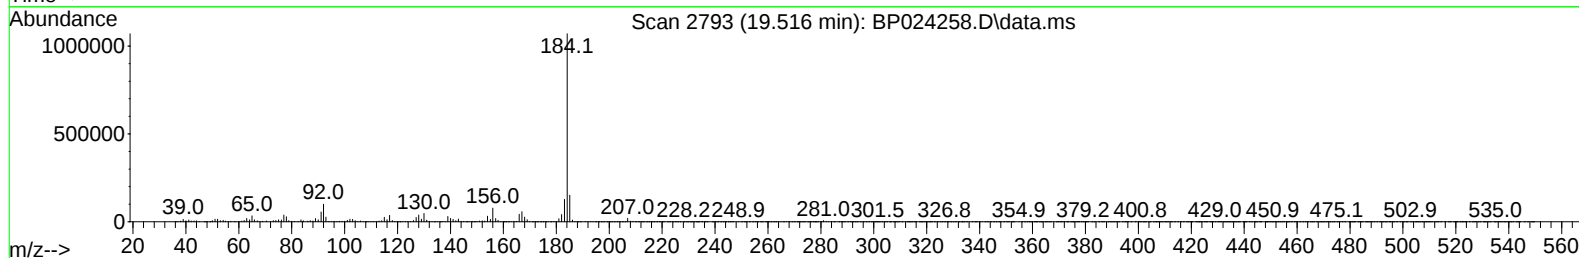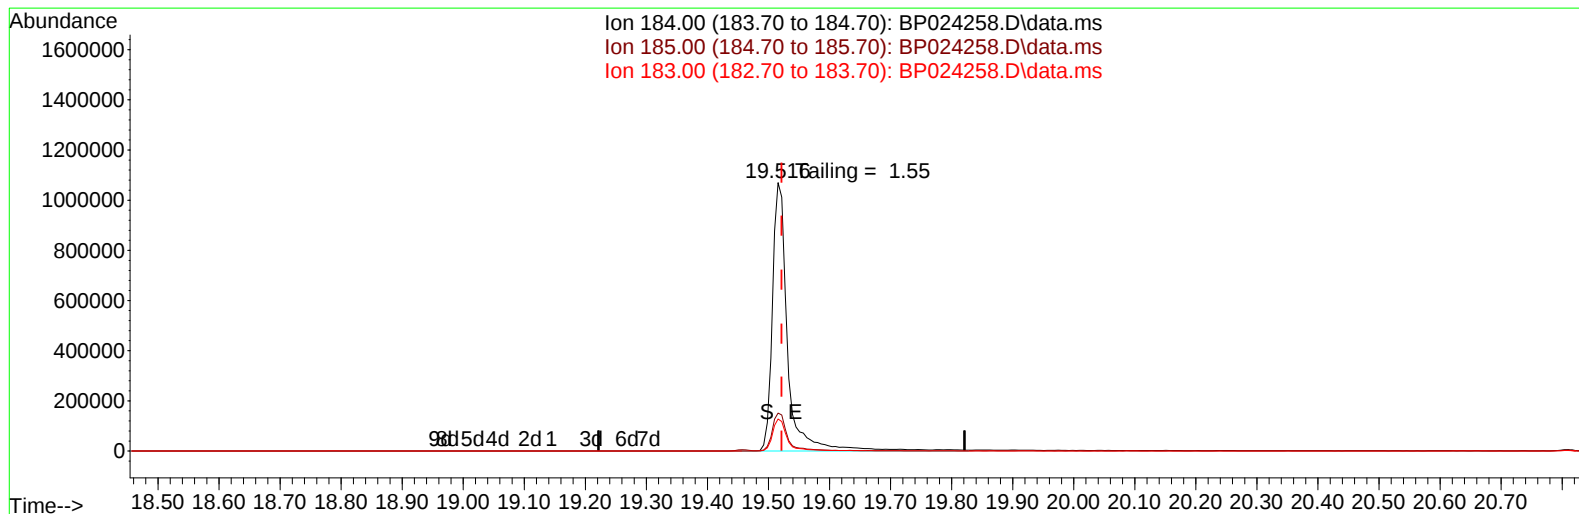

TIC: BP024258.D\data.ms

(77) Benzidine

19.516min (-0.006) 993482.96 ng m

response 1879156

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.14
183.00	11.40	11.94
0.00	0.00	0.00