
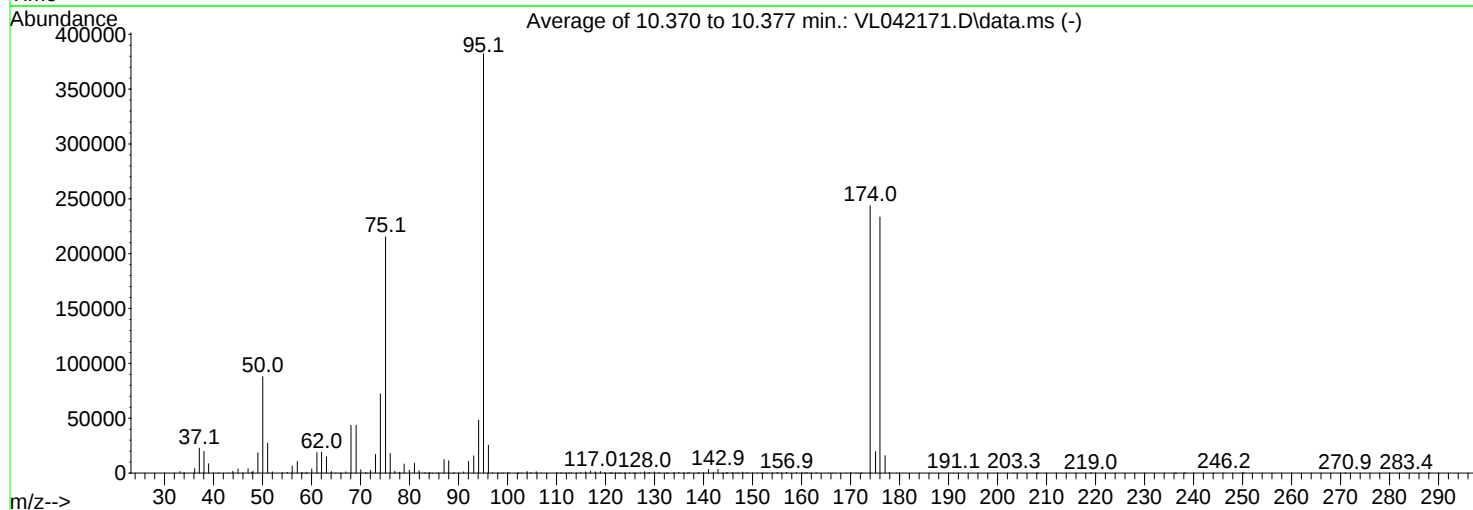


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042171.D
Acq On : 27 Mar 2025 07:44
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

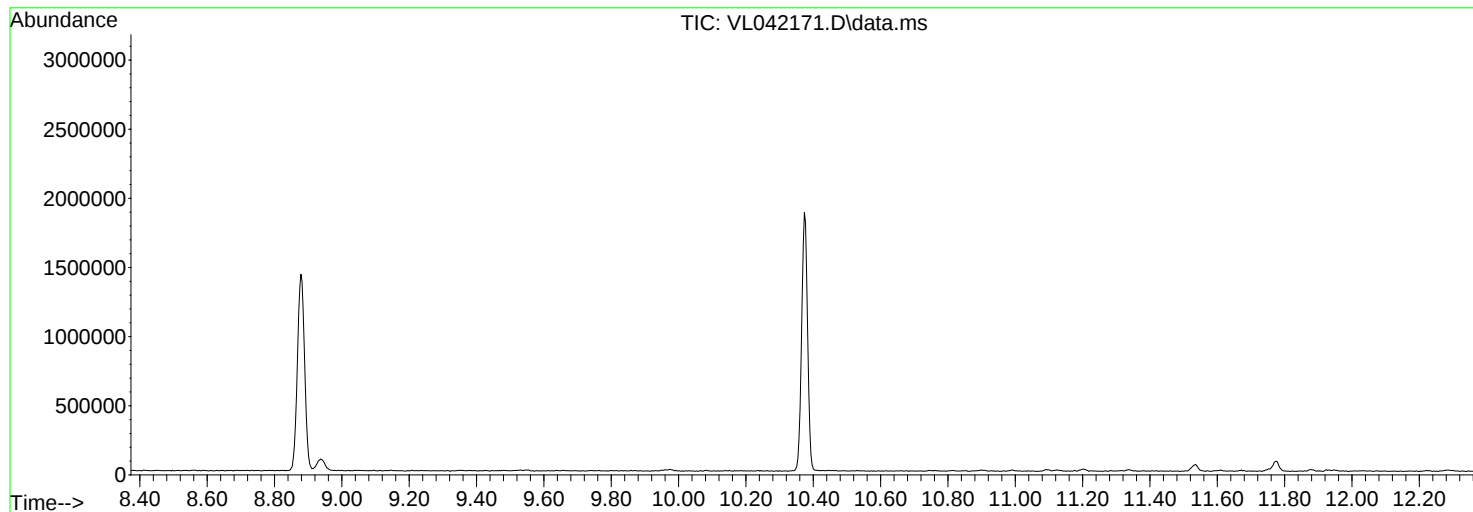

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3150

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	87995	PASS
75	95	30	66	56.3	215296	PASS
95	95	100	100	100.0	382268	PASS
96	95	5	9	6.6	25383	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.8	243904	PASS
175	174	4	9	8.0	19539	PASS
176	174	93	101	95.7	233493	PASS
177	176	5	9	6.8	15877	PASS

Average of 10.370 to 10.377 min.: VL042171.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	1400	47.05	4001	57.95	183	67.00	1161
33.90	31	47.80	824	58.15	219	68.05	43530
36.15	4138	48.05	1739	58.80	27	69.10	43612
37.10	22759	49.05	18477	59.20	62	70.05	3072
38.05	19773	50.05	87995	60.05	3842	71.05	391
39.00	8558	51.05	27372	61.10	18723	71.30	148
41.00	270	52.00	1090	62.05	19083	72.05	2510
43.05	65	54.00	265	63.05	14806	73.05	17047
43.95	1610	55.05	633	64.05	1355	74.05	72175
45.00	3695	56.05	6441	64.95	108	75.10	215296
46.00	111	57.10	10669	65.95	87	76.05	17968

Average of 10.370 to 10.377 min.: VL042171.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	1756	84.70	60	96.10	25383	105.85	1266
77.90	365	85.50	69	96.95	454	106.85	241
78.00	749	85.90	91	98.20	118	108.10	78
78.90	8287	87.05	12260	98.80	119	110.00	6
79.95	2770	88.00	11240	99.15	113	110.80	163
81.00	8994	88.95	27	100.10	27	111.10	228
81.95	2105	91.05	1113	102.10	25	111.80	169
83.05	87	92.05	10732	102.80	142	112.40	56
83.30	152	93.10	15706	104.00	1429	112.60	56
83.95	3	94.10	48315	104.70	208	113.05	295
84.20	78	95.10	382268	104.95	148	114.15	45

Average of 10.370 to 10.377 min.: VL042171.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.90	395	123.10	107	132.40	22	141.00	3317
115.95	1131	123.85	235	132.90	67	142.00	364
116.95	1918	124.95	222	133.80	40	142.95	3384
117.90	1124	125.80	79	134.10	121	143.95	131
118.95	1429	126.10	146	134.95	750	144.60	27
119.80	193	127.10	144	135.95	199	144.95	267
120.90	128	127.95	1262	136.70	145	145.90	507
121.10	24	128.70	250	137.05	545	146.60	55
122.00	119	129.00	312	138.80	28	146.95	155
122.50	33	129.95	1135	139.10	132	147.20	55
122.90	76	130.90	590	139.95	372	148.00	938

Average of 10.370 to 10.377 min.: VL042171.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.80	166	156.95	650	169.10	175	179.40	63
149.05	162	158.95	474	169.90	95	191.05	70
149.95	274	160.00	21	170.15	82	203.35	48
151.00	148	160.70	162	171.10	216	208.10	24
151.80	110	160.90	233	171.55	165	219.00	22
152.25	182	161.15	346	172.30	258	236.30	19
152.95	205	161.80	102	174.00	243904	238.10	24
154.00	201	162.90	25	175.10	19539	244.05	44
155.00	271	165.50	37	176.00	233493	246.20	61
155.15	639	166.35	72	177.05	15877	250.10	21
155.90	116	167.00	175	177.90	397	270.90	18

Average of 10.370 to 10.377 min.: VL042171.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
283.40	34						
288.00	20						

Instrument :

MSVOA_L

ClientSampleId :

BFB