
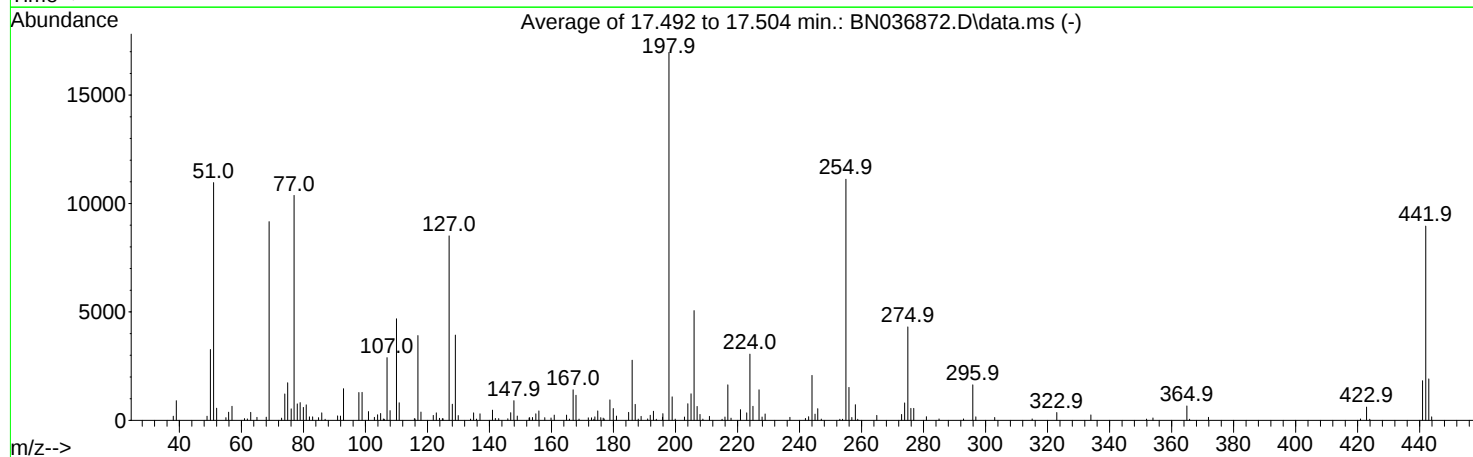


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN041125\  
Data File : BN036872.D  
Acq On : 11 Apr 2025 11:03  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN041125.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Apr 11 16:11:08 2025

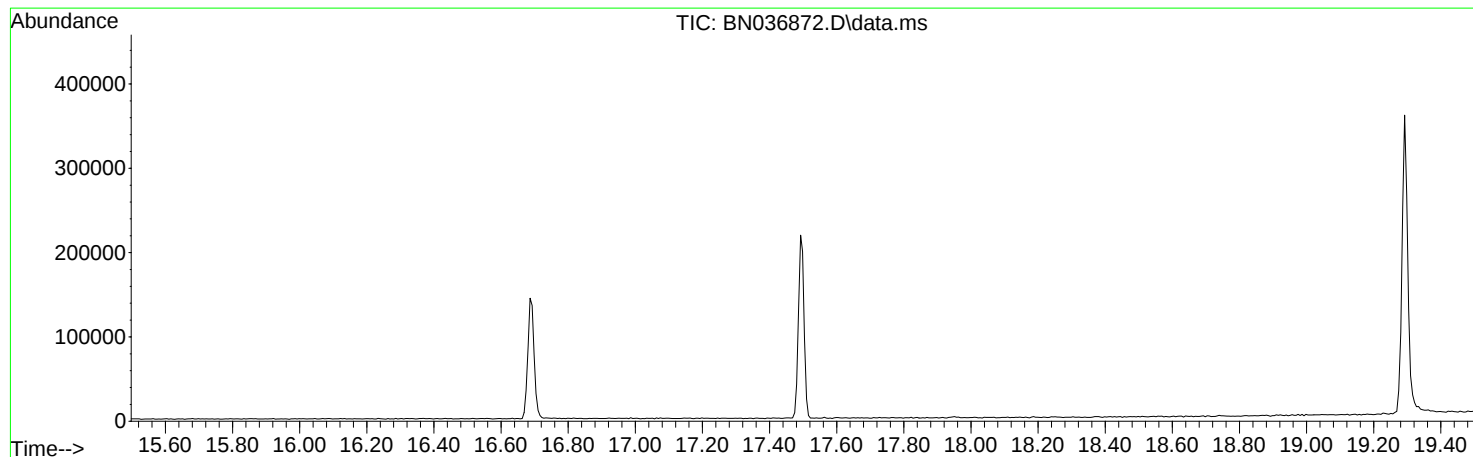

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 64.6         | 10965      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 147        | PASS                |
| 69             | 198             | 0.00            | 100             | 54.0         | 9164       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 50.2         | 8509       | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 16964      | PASS                |
| 199            | 198             | 5               | 9               | 6.4          | 1083       | PASS                |
| 275            | 198             | 10              | 60              | 25.4         | 4308       | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 661        | PASS                |
| 441            | 198             | 0.01            | 100             | 10.8         | 1829       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 8955       | PASS                |
| 443            | 442             | 15              | 24              | 21.3         | 1910       | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/11/2025     | BNA_N            | <u>BN036872.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 68421            | 20.533             |
| DDD           | 473              | 20.145             |
| DDE           | 0                | 19.621             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 473           | 68894            | 0.69               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN041125\  
Data File : BN036872.D  
Acq On : 11 Apr 2025 11:03  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Apr 11 16:50:38 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 01 00:16:52 2025  
Response via : Initial Calibration

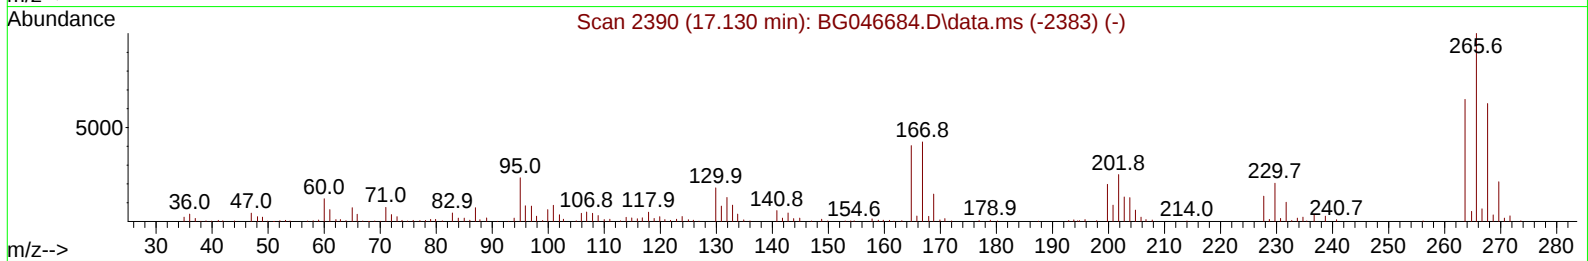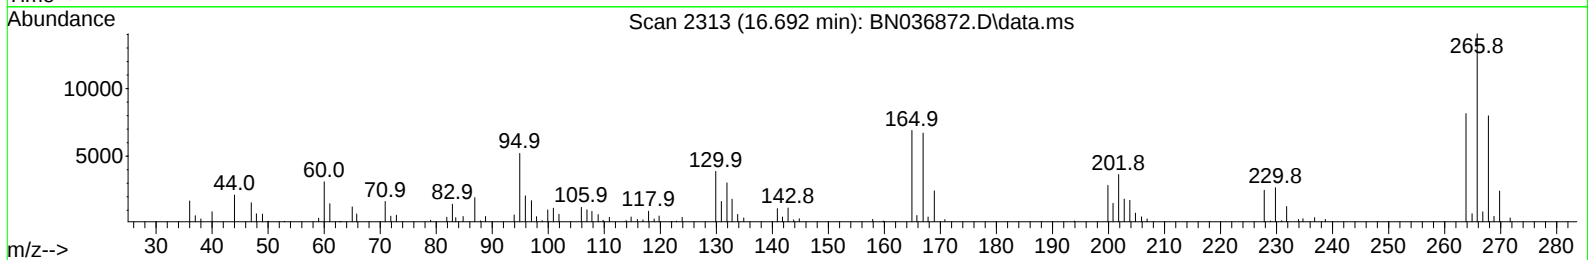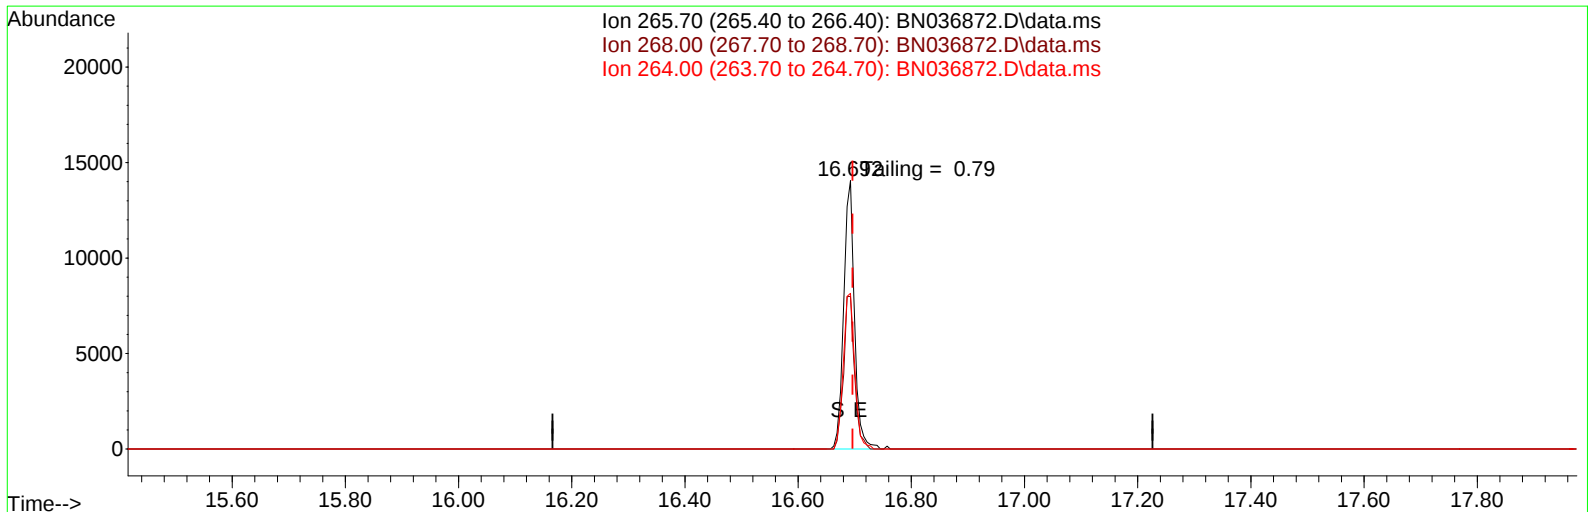

TIC: BN036872.D\data.ms

**(70) Pentachlorophenol (C)**

**16.692min (-0.004) 36331.83 ng**




**response 18533**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 56.86  |
| 264.00 | 61.60  | 58.03  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN041125\  
Data File : BN036872.D  
Acq On : 11 Apr 2025 11:03  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Apr 11 16:50:38 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 01 00:16:52 2025  
Response via : Initial Calibration

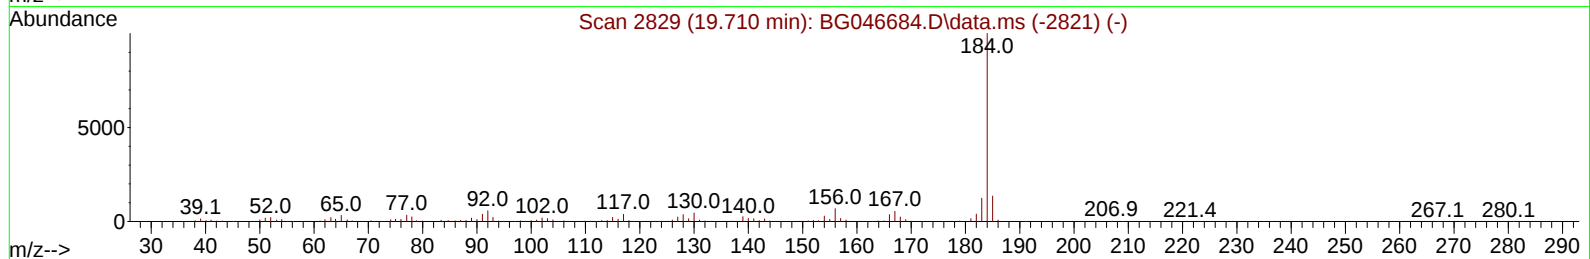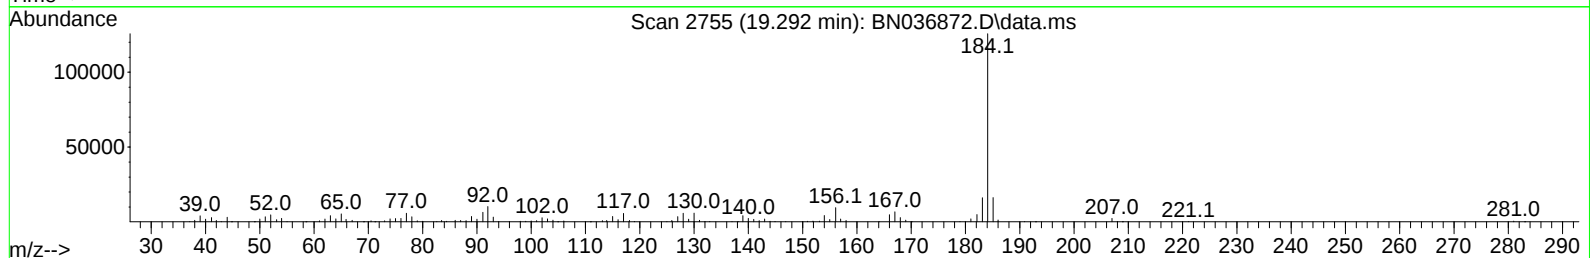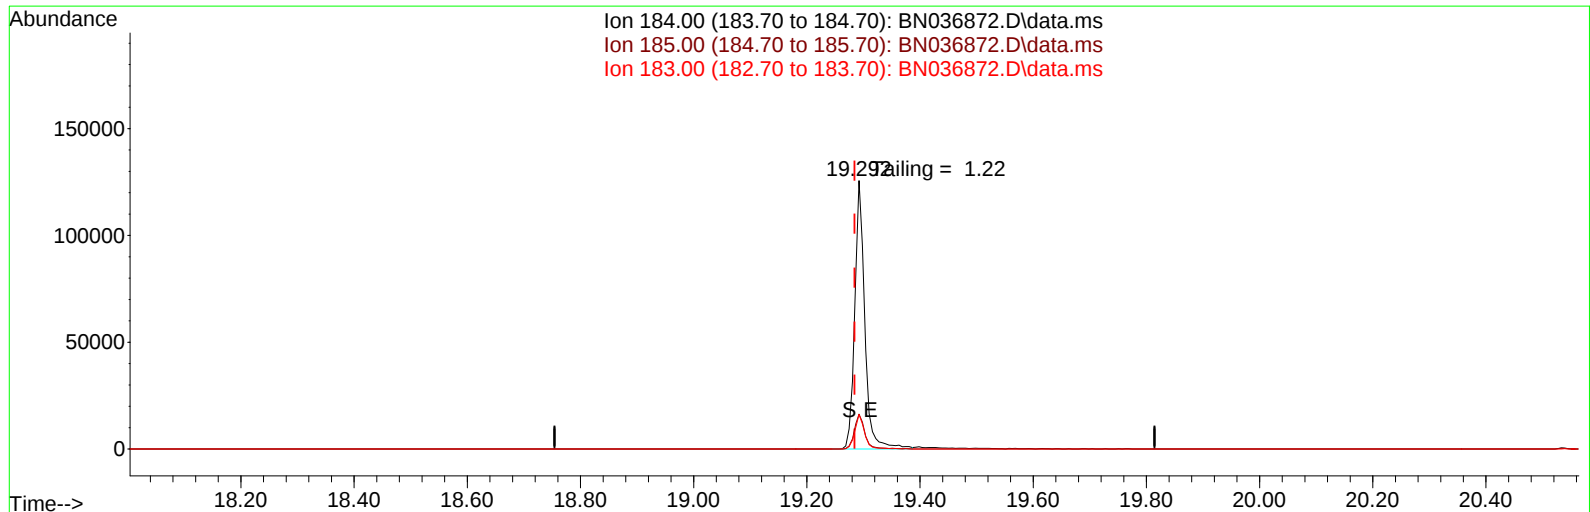

TIC: BN036872.D\data.ms

**(77) Benzidine**

**19.292min (+ 0.008) 0.00 ng**

**response 156190**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.01  |
| 183.00 | 13.20  | 12.90  |
| 0.00   | 0.00   | 0.00   |