
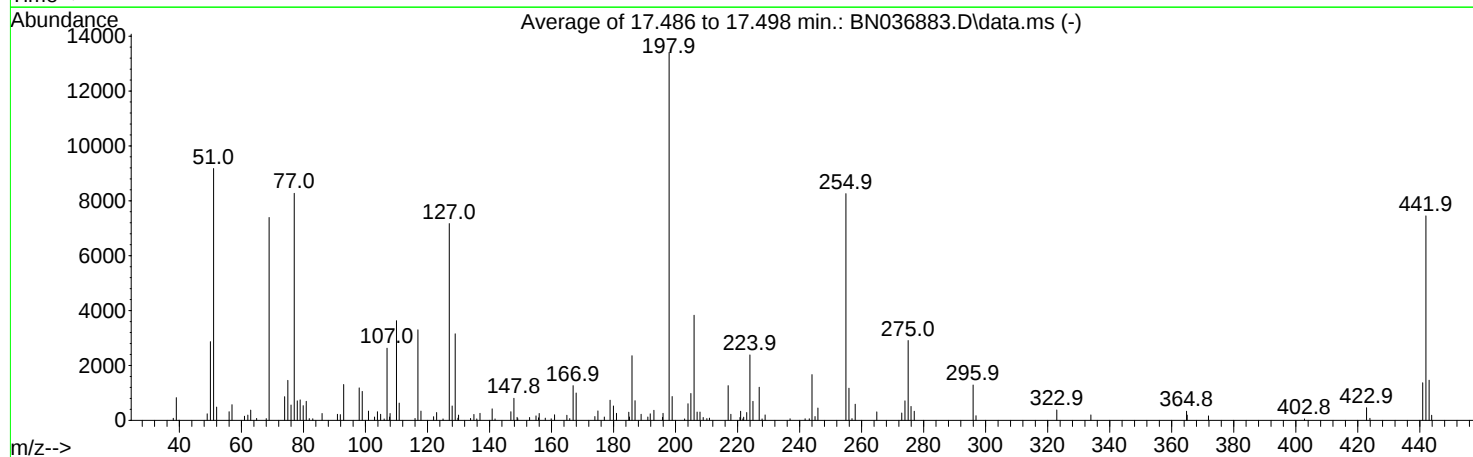


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN041125\  
Data File : BN036883.D  
Acq On : 11 Apr 2025 18:06  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN041125.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Apr 11 16:11:08 2025

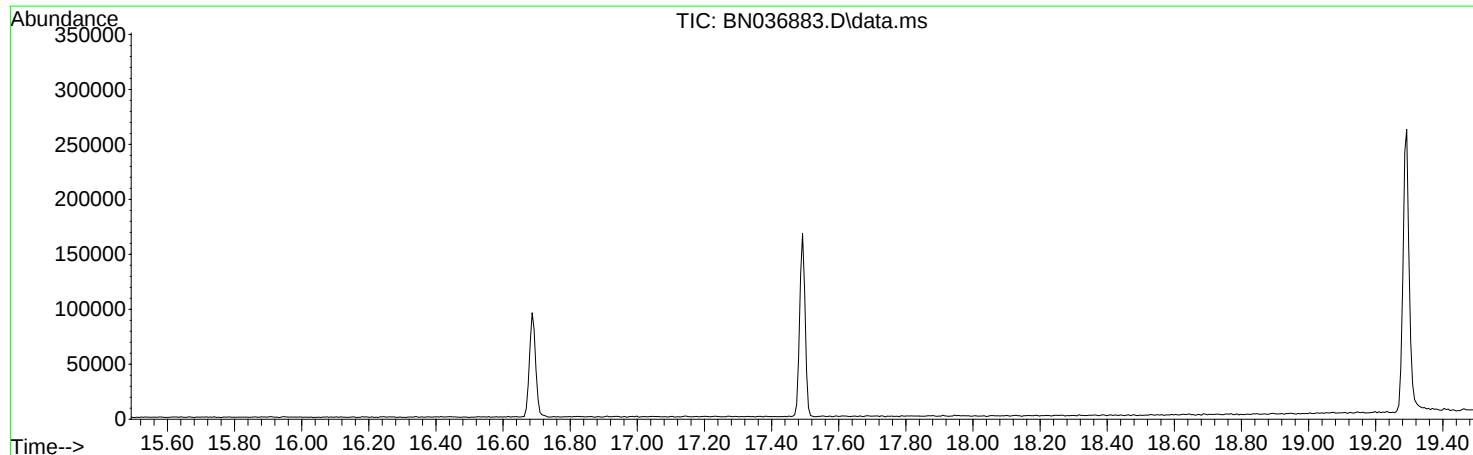

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 51     | 198     | 10     | 80     | 68.5  | 9178  | PASS      |
| 68     | 69      | 0.00   | 2      | 0.9   | 64    | PASS      |
| 69     | 198     | 0.00   | 100    | 55.2  | 7395  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.0   | 0     | PASS      |
| 127    | 198     | 10     | 80     | 53.5  | 7172  | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0     | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 13404 | PASS      |
| 199    | 198     | 5      | 9      | 6.5   | 866   | PASS      |
| 275    | 198     | 10     | 60     | 21.7  | 2912  | PASS      |
| 365    | 198     | 1      | 100    | 2.5   | 334   | PASS      |
| 441    | 198     | 0.01   | 100    | 10.2  | 1368  | PASS      |
| 442    | 442     | 50     | 100    | 100.0 | 7452  | PASS      |
| 443    | 442     | 15     | 24     | 19.6  | 1464  | PASS      |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/11/2025     | BNA_N            | <u>BN036883.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 54631            | 20.533             |
| DDD           | 872              | 20.145             |
| DDE           | 0                | 19.621             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 872           | 55503            | 1.57               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN041125\  
Data File : BN036883.D  
Acq On : 11 Apr 2025 18:06  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Apr 11 23:52:18 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 11 23:51:57 2025  
Response via : Initial Calibration

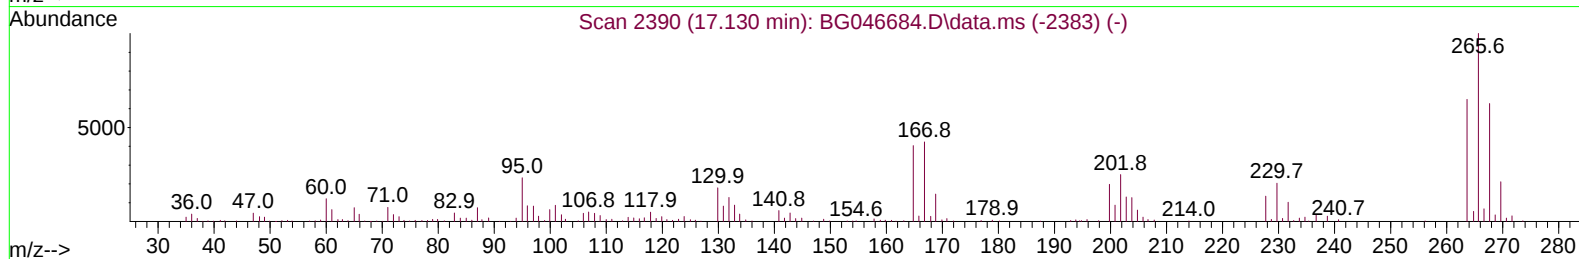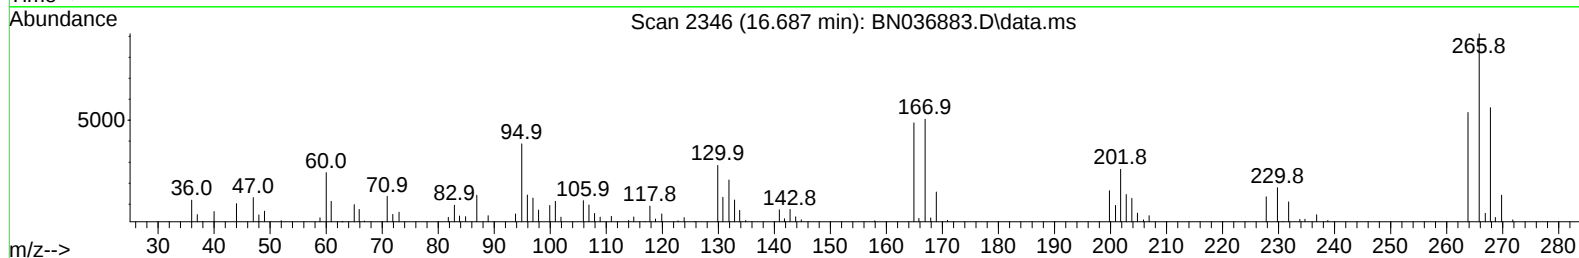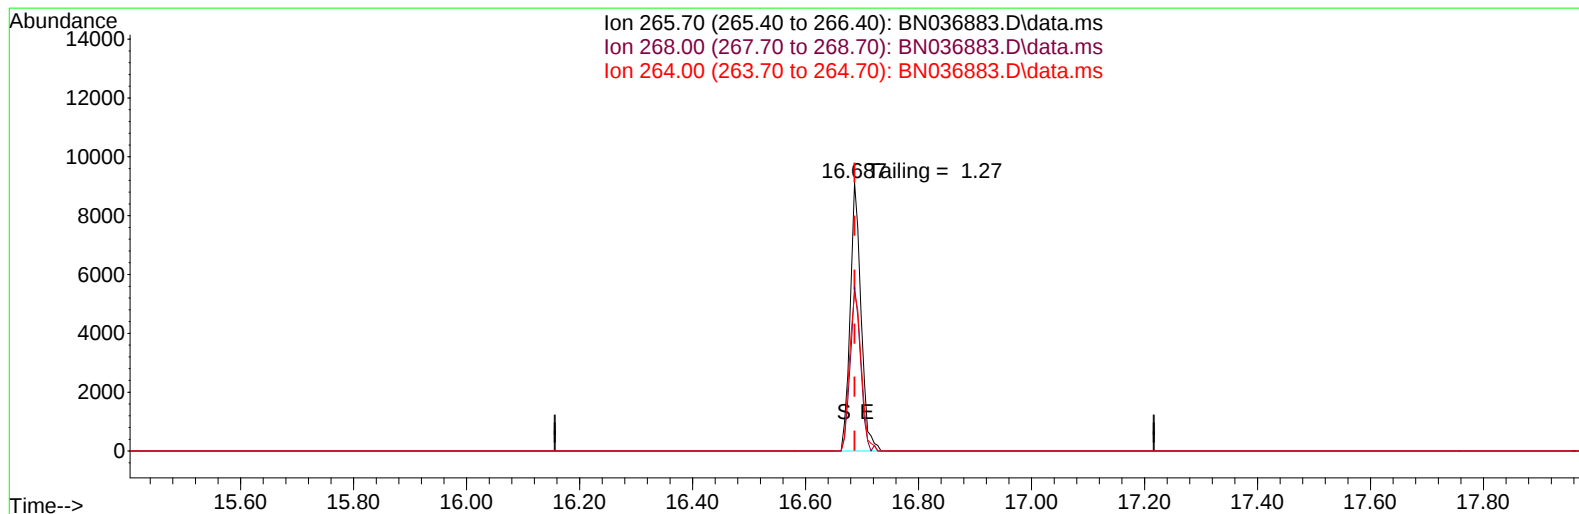

TIC: BN036883.D\data.ms

**(70) Pentachlorophenol (C)**

16.687min ( 0.000) 0.00 ng




response 12230

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 65.36  |
| 264.00 | 61.60  | 58.86  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN041125\  
Data File : BN036883.D  
Acq On : 11 Apr 2025 18:06  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Apr 11 23:52:18 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 11 23:51:57 2025  
Response via : Initial Calibration

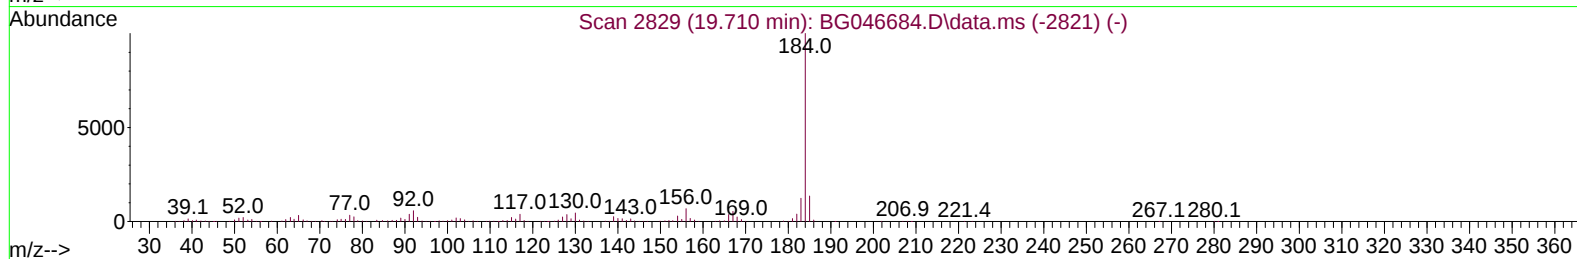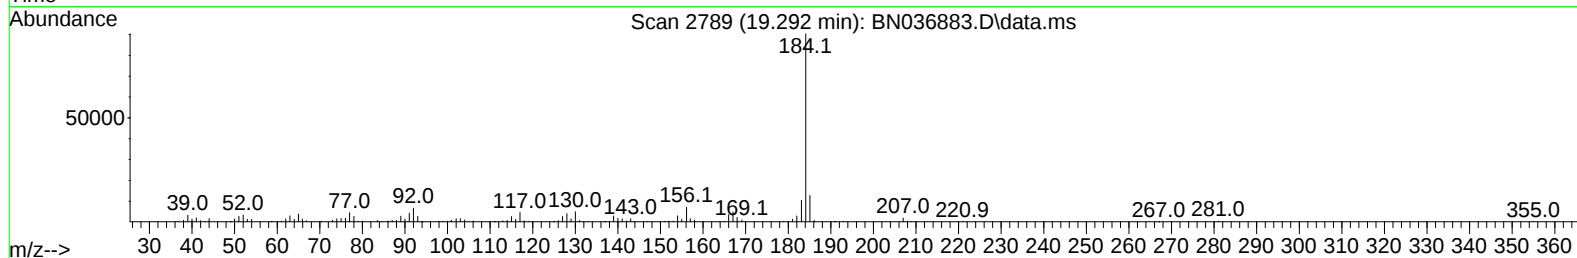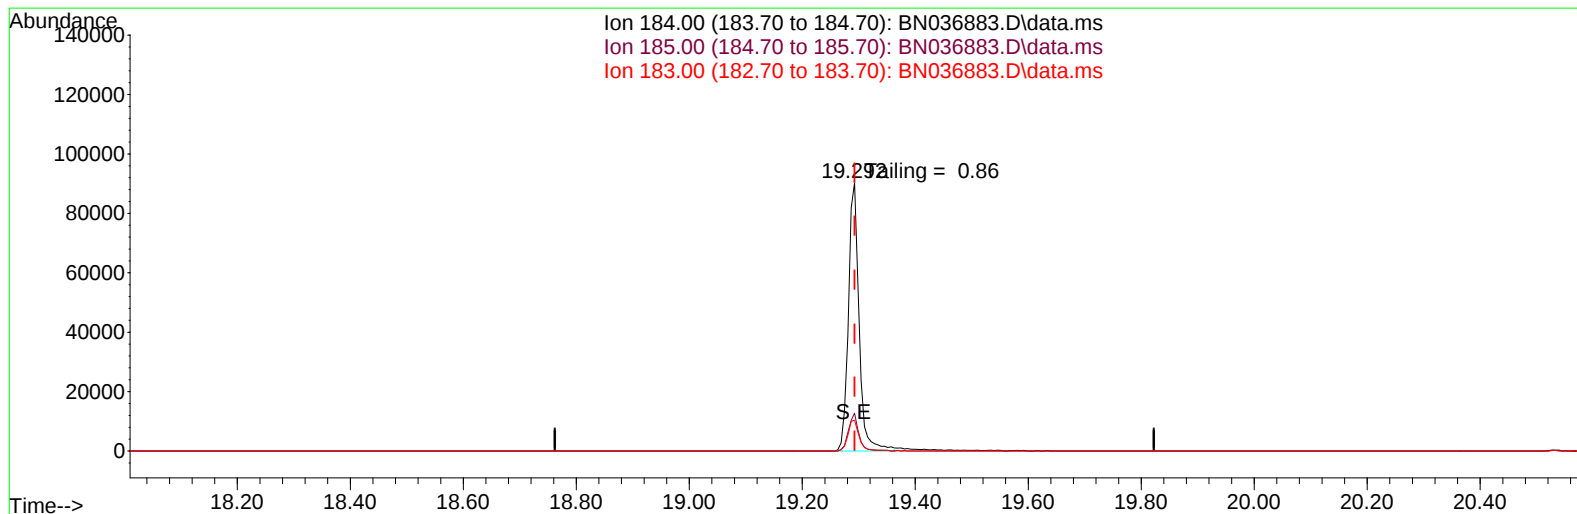

TIC: BN036883.D\data.ms

(77) Benzidine

19.292min ( 0.000) 0.00 ng

response 121284

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.14  |
| 183.00 | 13.20  | 11.53  |
| 0.00   | 0.00   | 0.00   |