

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041125\
 Data File : VX045732.D
 Acq On : 11 Apr 2025 11:32
 Operator : JC/MD
 Sample : VX0411WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0411WBL01

Quant Time: Apr 11 23:03:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	65554	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	128675	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	118153	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	48353	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	64154	53.515	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 107.020%	
35) Dibromofluoromethane	5.379	113	46741	51.198	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.400%	
50) Toluene-d8	8.647	98	159396	50.021	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.040%	
62) 4-Bromofluorobenzene	11.079	95	58527	50.424	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 100.840%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041125\
Data File : VX045732.D
Acq On : 11 Apr 2025 11:32
Operator : JC/MD
Sample : VX0411WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0411WBL01

Quant Time: Apr 11 23:03:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration

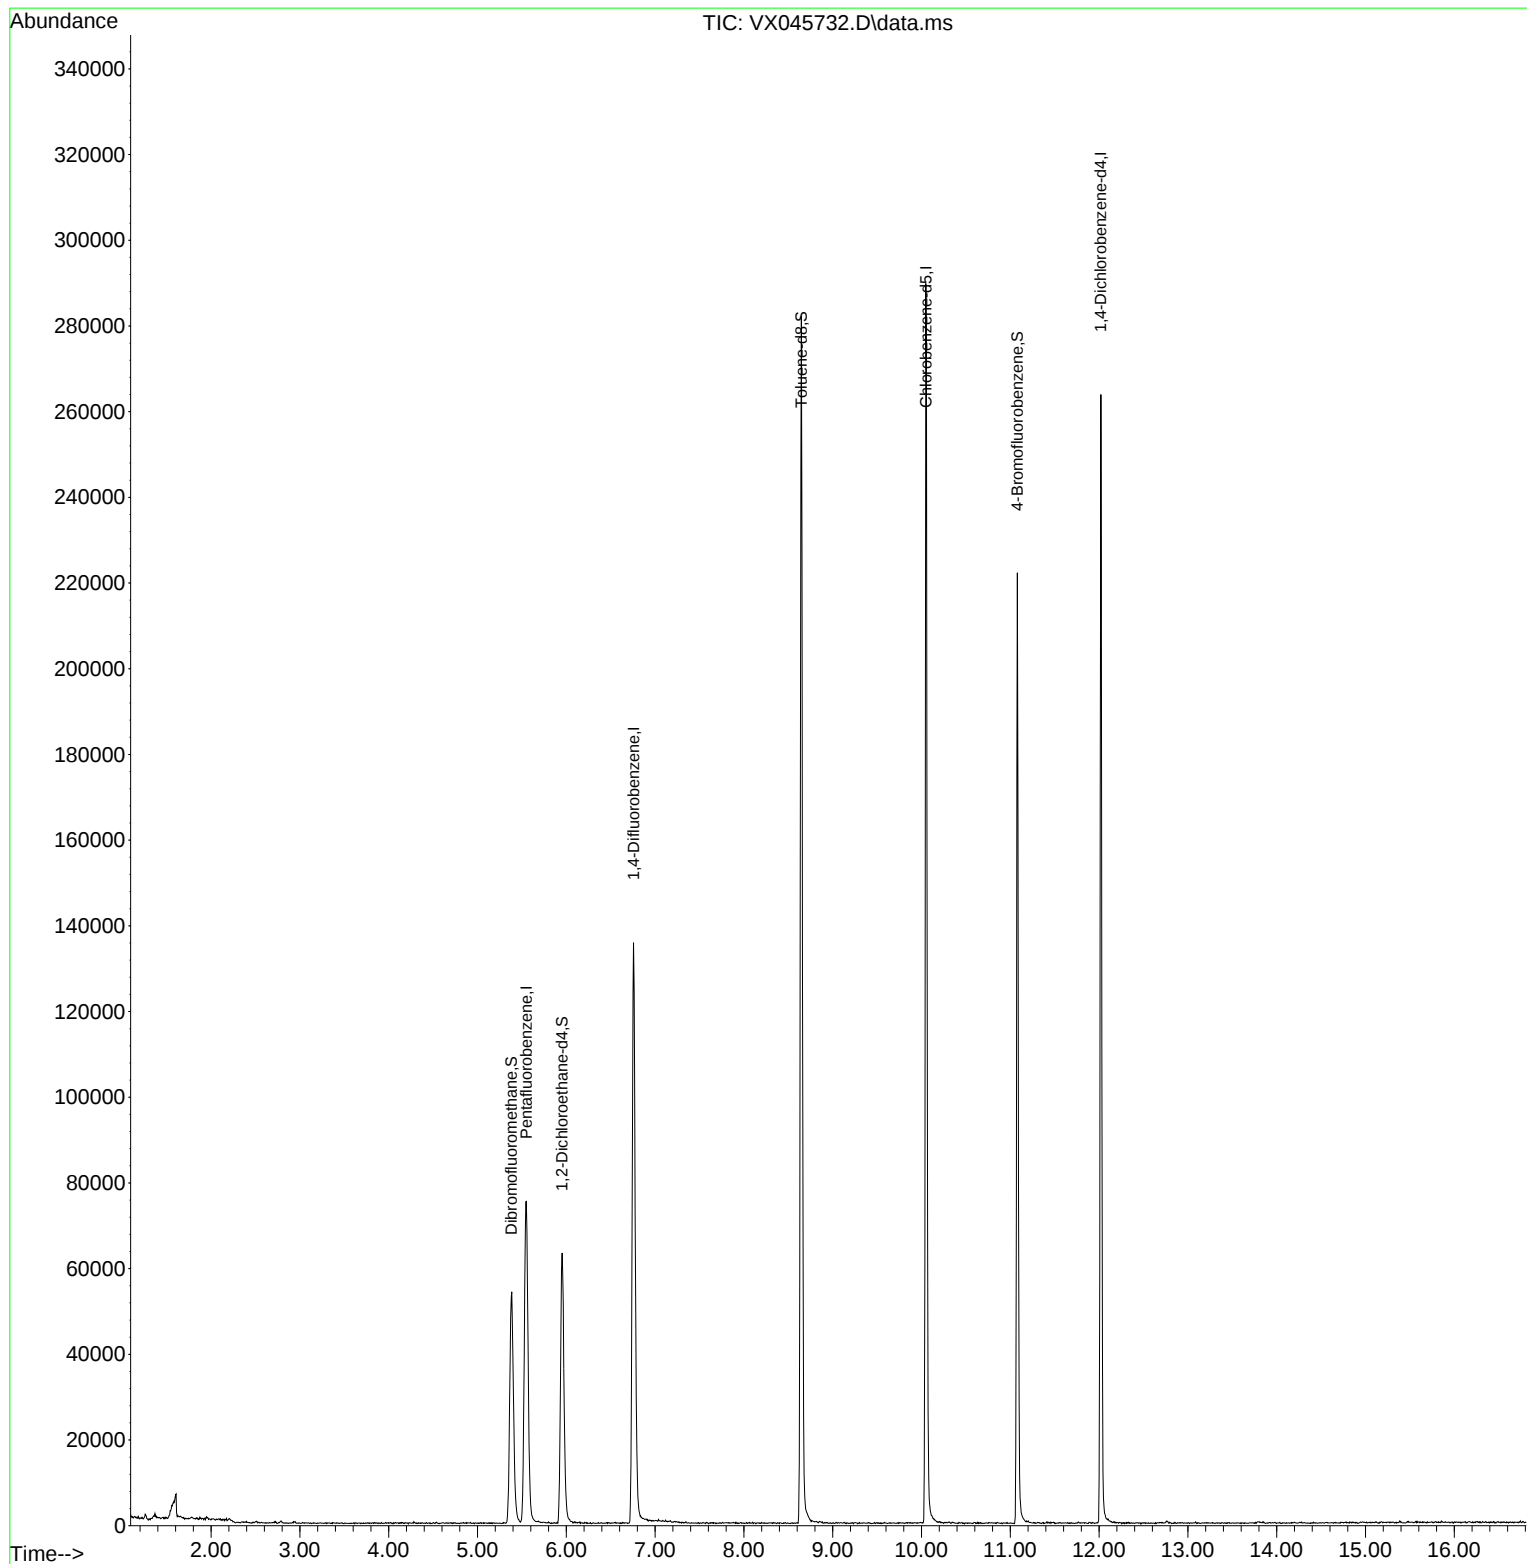



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.000 min

Lab File: VX045732.D

Acq: 11 Apr 2025 11:32

Instrument :

MSVOA_X

ClientSampleId :





VX0411WBL01

Tgt Ion:168 Resp: 65554

Ion Ratio Lower Upper

168 100

99 70.1 52.3 78.5

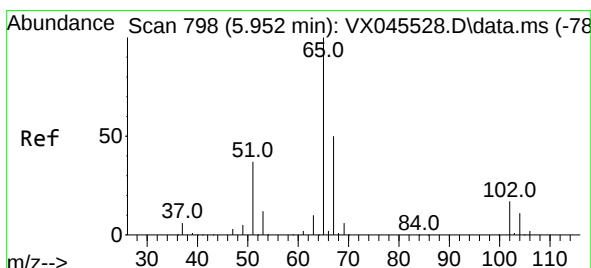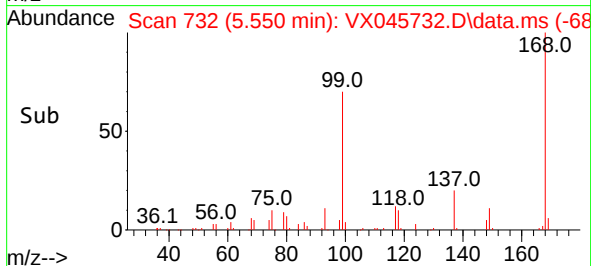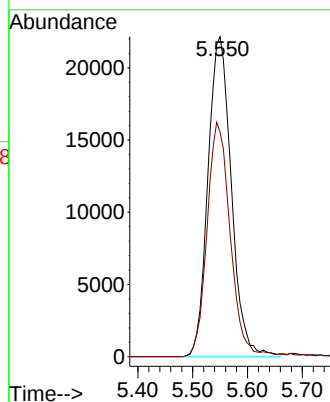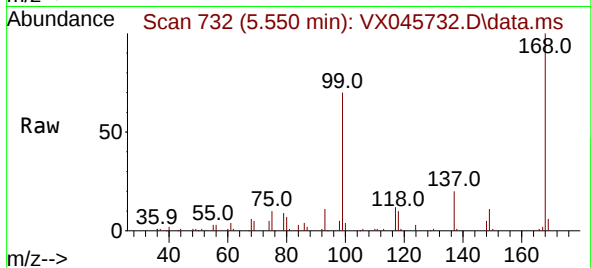

#33

1,2-Dichloroethane-d4

Concen: 53.515 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX045732.D




Acq: 11 Apr 2025 11:32

Tgt Ion: 65 Resp: 64154

Ion Ratio Lower Upper

65 100

67 49.6 0.0 99.0

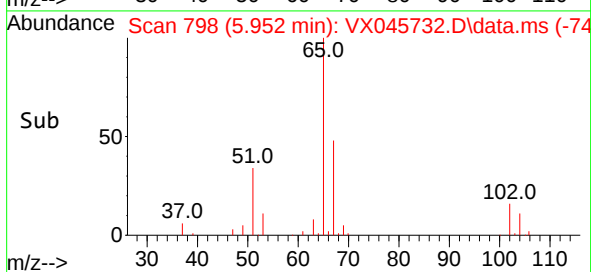
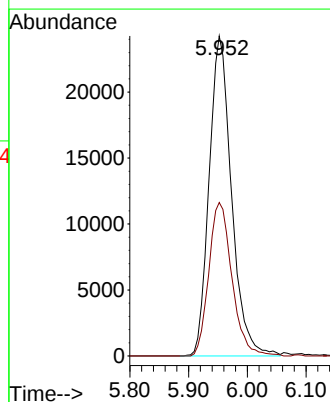
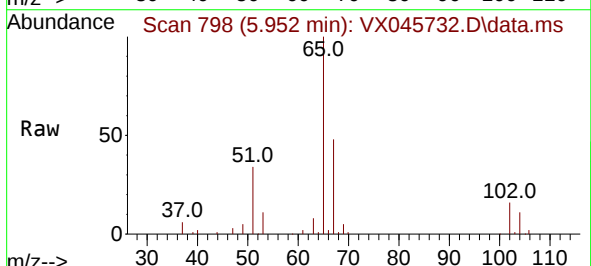




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 911
 Delta R.T. 0.000 min
 Lab File: VX045732.D
 Acq: 11 Apr 2025 11:32




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0411WBL01


Tgt Ion:114 Resp: 128675
 Ion Ratio Lower Upper
 114 100
 63 23.4 0.0 46.8
 88 16.8 0.0 35.4

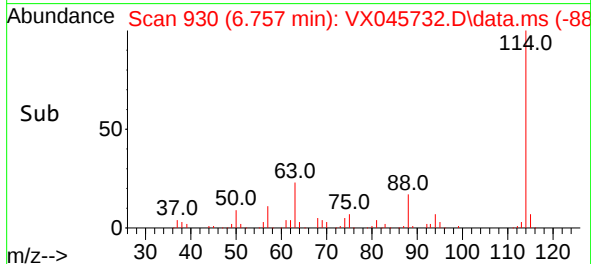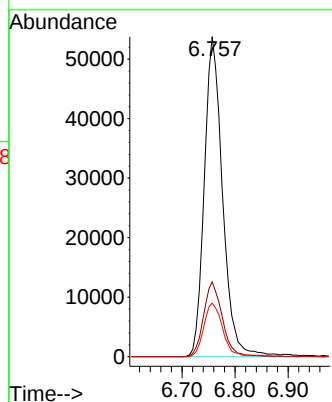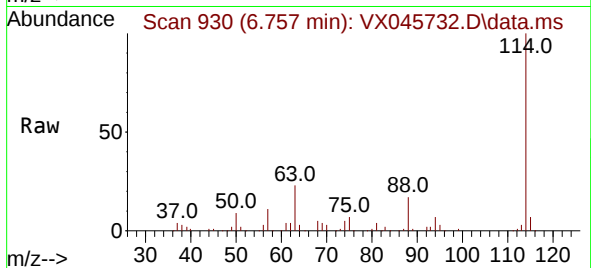

#35
 Dibromofluoromethane
 Concen: 51.198 ug/l
 RT: 5.379 min Scan# 704
 Delta R.T. 0.000 min
 Lab File: VX045732.D
 Acq: 11 Apr 2025 11:32

Tgt Ion:113 Resp: 46741
 Ion Ratio Lower Upper
 113 100
 111 102.1 81.8 122.6
 192 16.9 13.8 20.6

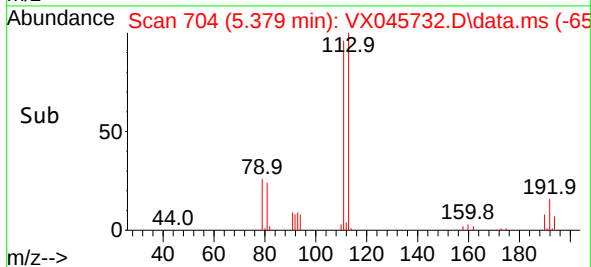
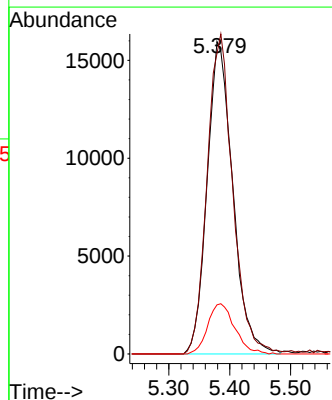
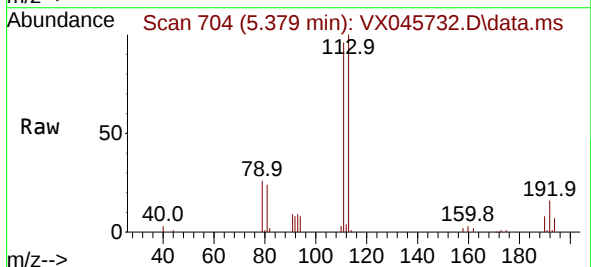


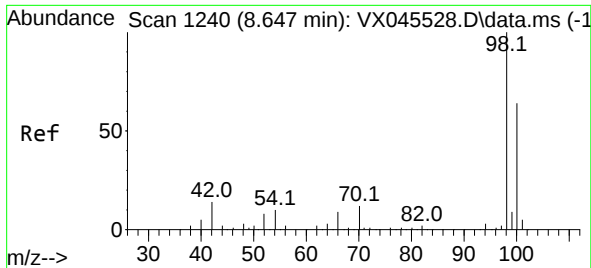

#50
Toluene-d8
Concen: 50.021 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045732.D
Acq: 11 Apr 2025 11:32




Instrument :
MSVOA_X
ClientSampleId :
VX0411WBL01


Tgt Ion: 98 Resp: 159396
Ion Ratio Lower Upper
98 100
100 64.9 52.2 78.4

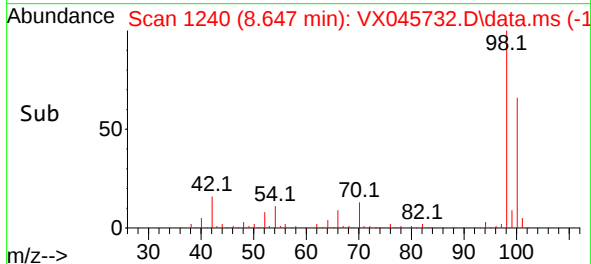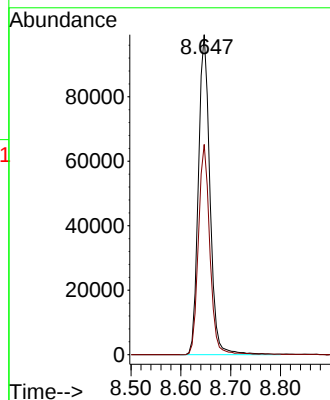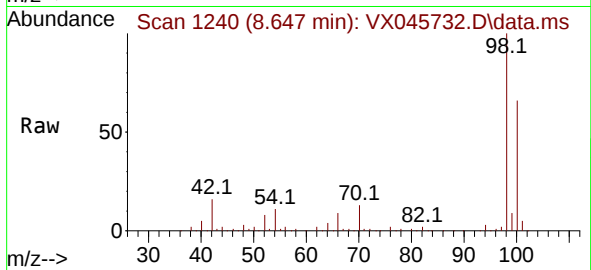

#62
4-Bromofluorobenzene
Concen: 50.424 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045732.D
Acq: 11 Apr 2025 11:32

Tgt Ion: 95 Resp: 58527
Ion Ratio Lower Upper
95 100
174 67.8 0.0 135.8
176 65.5 0.0 131.4

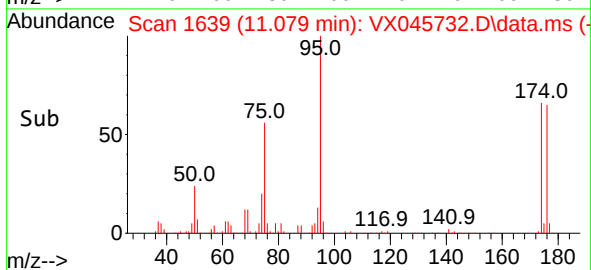
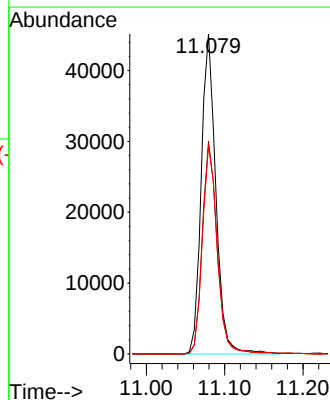
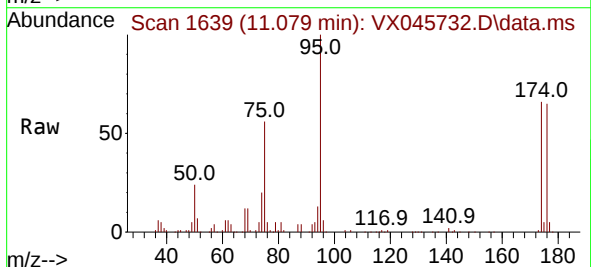


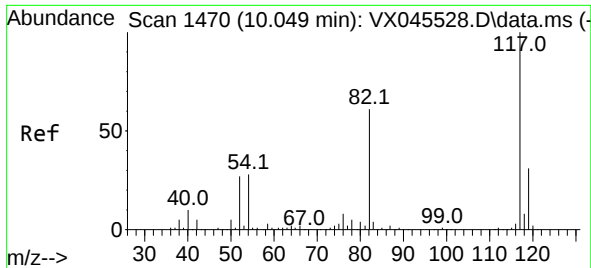

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045732.D
Acq: 11 Apr 2025 11:32

Instrument :
MSVOA_X
ClientSampleId :
VX0411WBL01

Tgt Ion:117 Resp: 118153
Ion Ratio Lower Upper
117 100
82 62.0 49.2 73.8
119 31.9 25.1 37.7

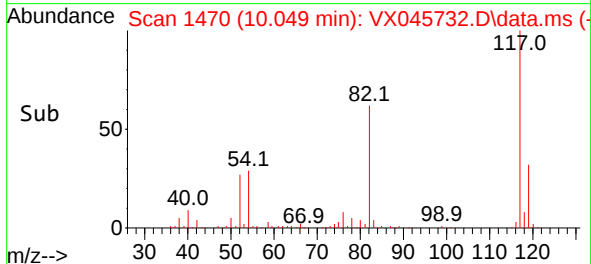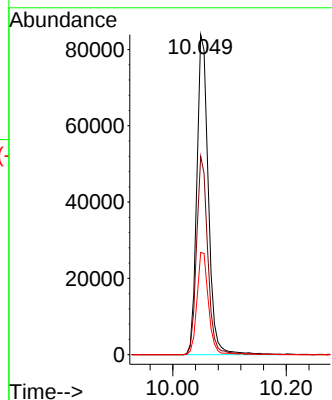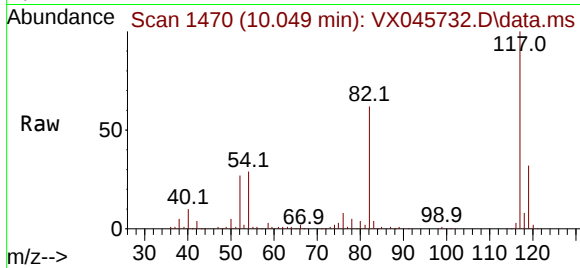

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045732.D
Acq: 11 Apr 2025 11:32

Tgt Ion:152 Resp: 48353
Ion Ratio Lower Upper
152 100
115 65.6 46.9 140.7
150 157.7 0.0 349.4

