

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041125\
 Data File : VX045747.D
 Acq On : 11 Apr 2025 17:23
 Operator : JC/MD
 Sample : Q1773-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TB-20250407

Quant Time: Apr 11 23:06:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	64635	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	127456	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	119779	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	50320	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	64048	54.186	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	108.380%
35) Dibromofluoromethane	5.379	113	46129	51.011	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.020%
50) Toluene-d8	8.647	98	158270	50.143	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.280%
62) 4-Bromofluorobenzene	11.079	95	60732	52.824	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	105.640%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041125\
Data File : VX045747.D
Acq On : 11 Apr 2025 17:23
Operator : JC/MD
Sample : Q1773-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250407

Quant Time: Apr 11 23:06:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




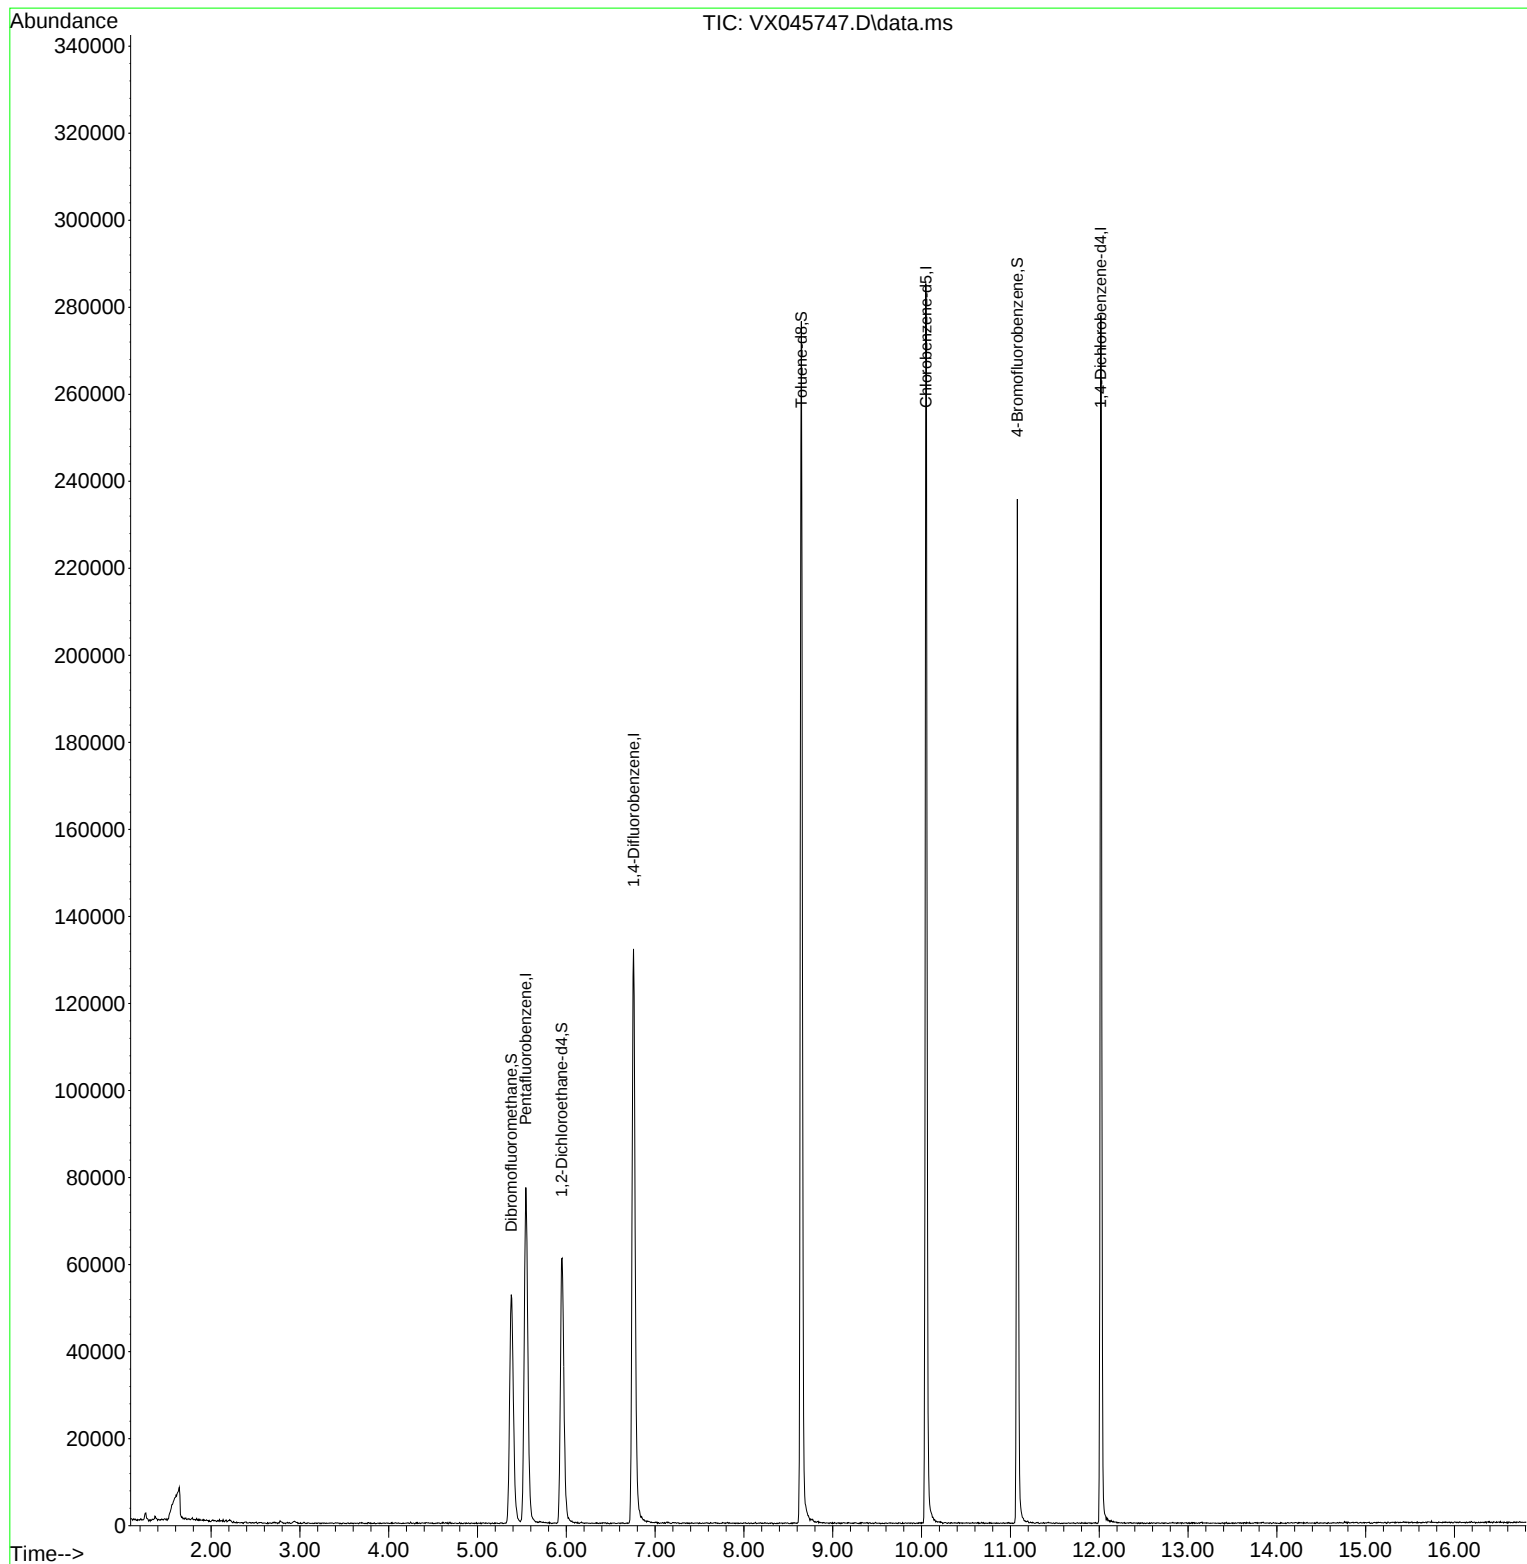




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045747.D
Acq: 11 Apr 2025 17:23




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250407


Tgt Ion:168 Resp: 64635
Ion Ratio Lower Upper
168 100
99 74.4 52.3 78.5

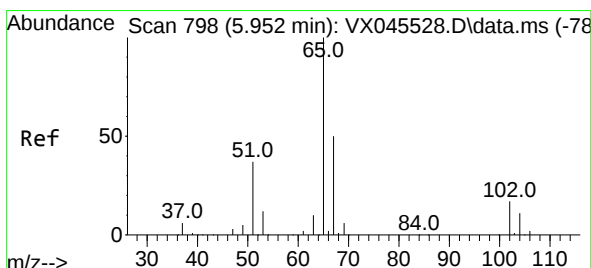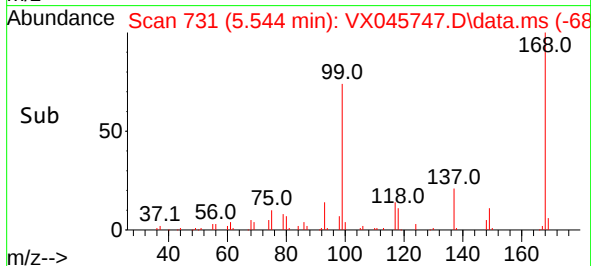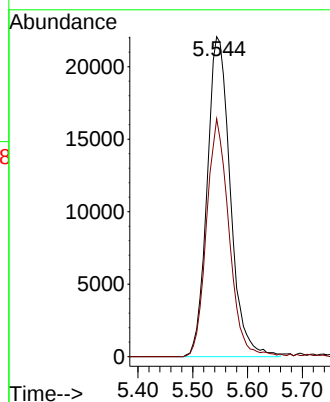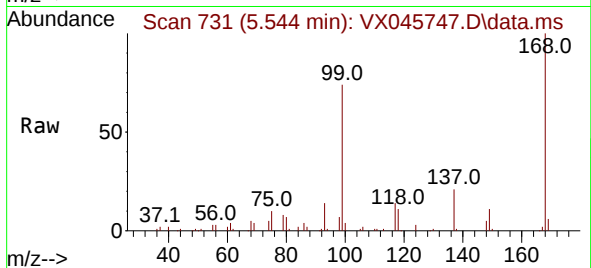

#33
1,2-Dichloroethane-d4
Concen: 54.186 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX045747.D
Acq: 11 Apr 2025 17:23

Tgt Ion: 65 Resp: 64048
Ion Ratio Lower Upper
65 100
67 49.1 0.0 99.0

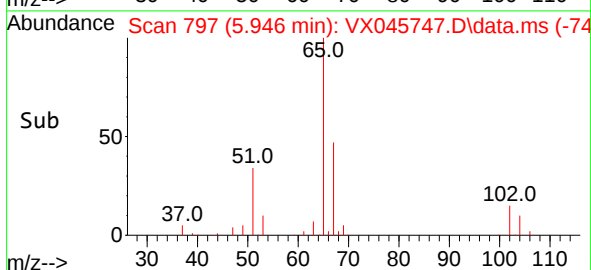
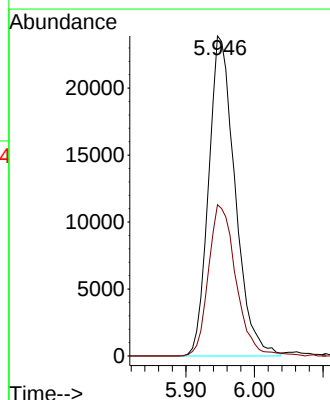
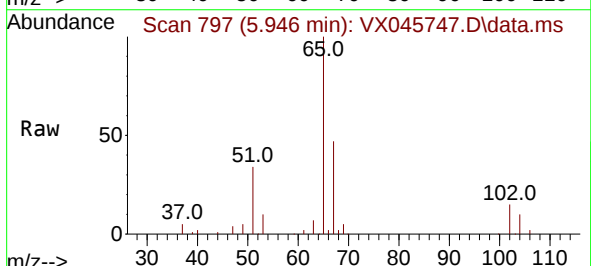


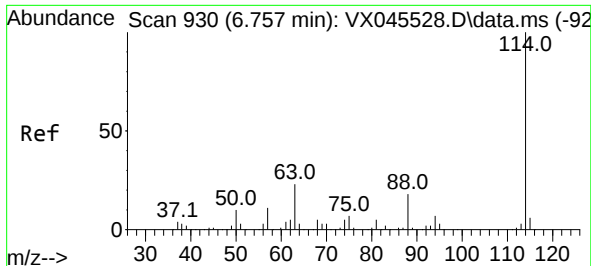

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045747.D
Acq: 11 Apr 2025 17:23




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250407


Tgt Ion:	114	Resp:	127456
Ion	Ratio	Lower	Upper
114	100		
63	24.9	0.0	46.8
88	18.0	0.0	35.4

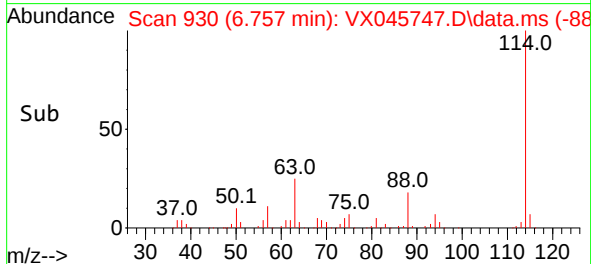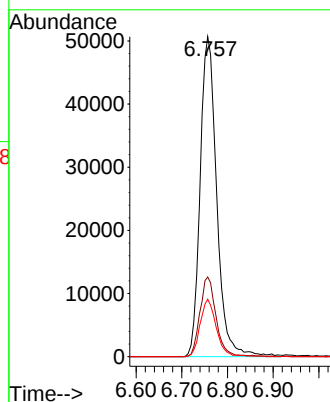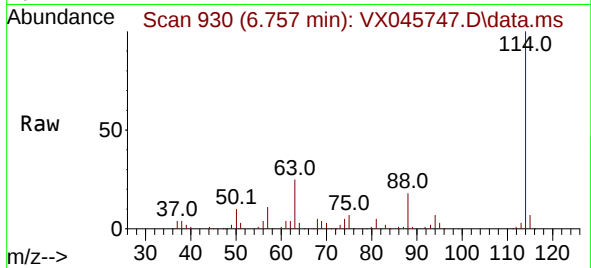

#35
Dibromofluoromethane
Concen: 51.011 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX045747.D
Acq: 11 Apr 2025 17:23

Tgt Ion:	113	Resp:	46129
Ion	Ratio	Lower	Upper
113	100		
111	101.8	81.8	122.6
192	16.8	13.8	20.6


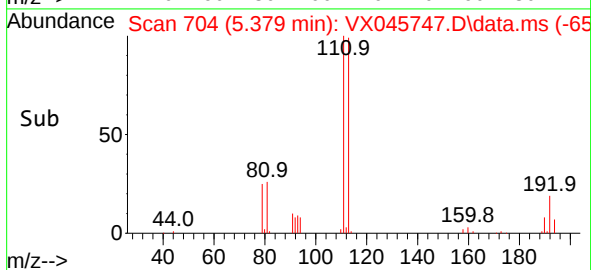
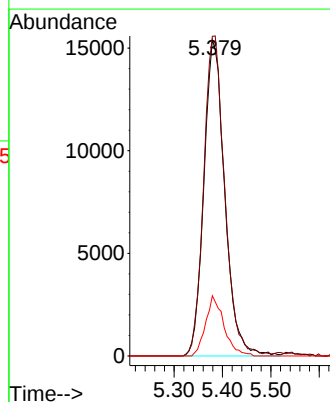
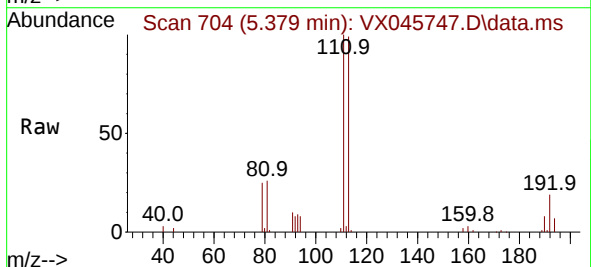


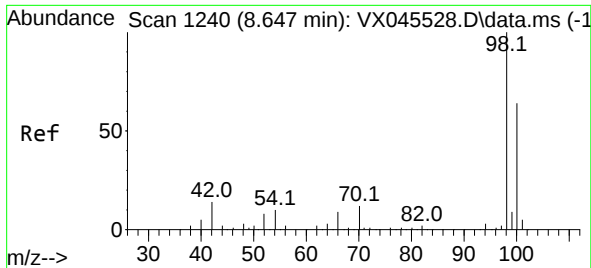

#50
Toluene-d8
Concen: 50.143 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045747.D
Acq: 11 Apr 2025 17:23




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250407


Tgt Ion: 98 Resp: 158270
Ion Ratio Lower Upper
98 100
100 65.0 52.2 78.4

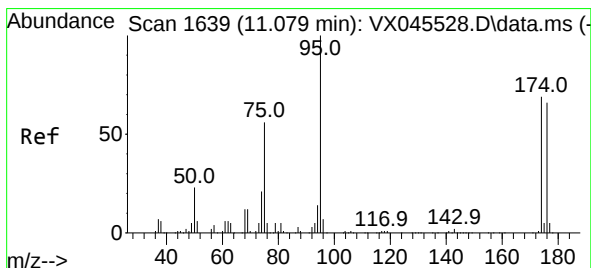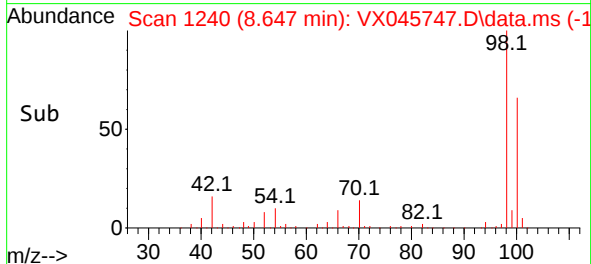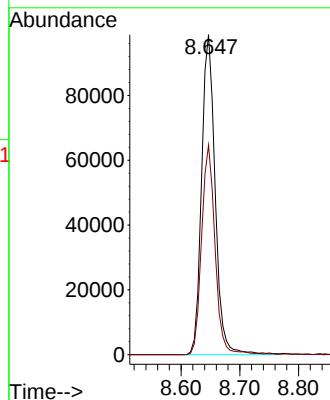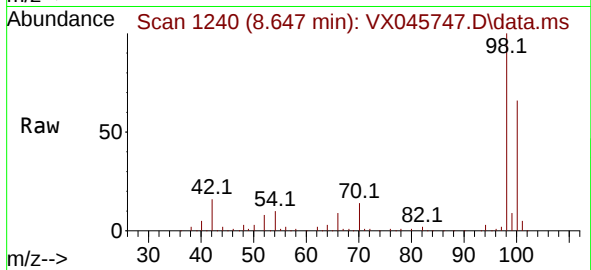

#62
4-Bromofluorobenzene
Concen: 52.824 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045747.D
Acq: 11 Apr 2025 17:23

Tgt Ion: 95 Resp: 60732
Ion Ratio Lower Upper
95 100
174 67.2 0.0 135.8
176 64.3 0.0 131.4

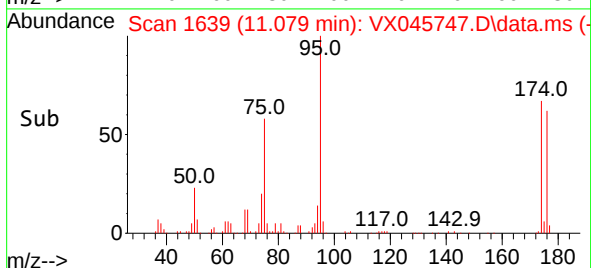
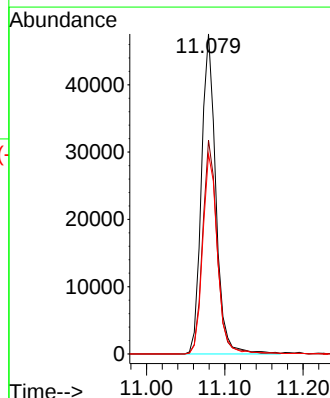
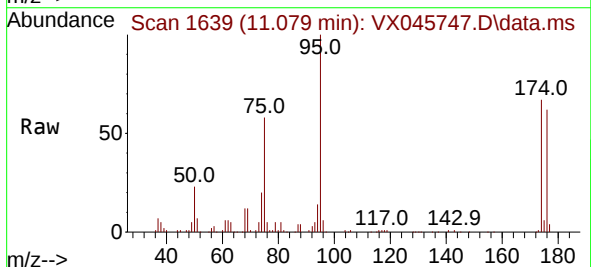


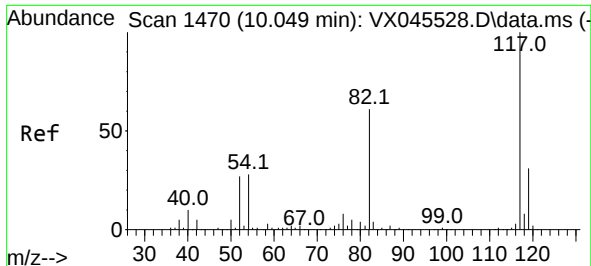

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX045747.D
Acq: 11 Apr 2025 17:23

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250407

Tgt Ion:117 Resp: 119779
Ion Ratio Lower Upper
117 100
82 59.5 49.2 73.8
119 32.0 25.1 37.7

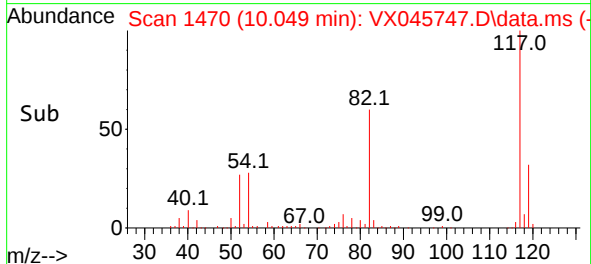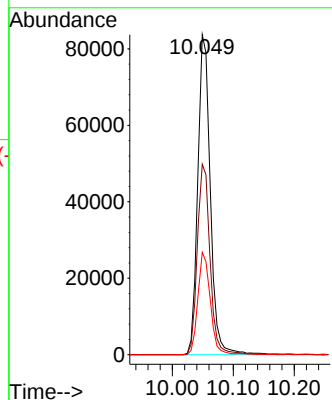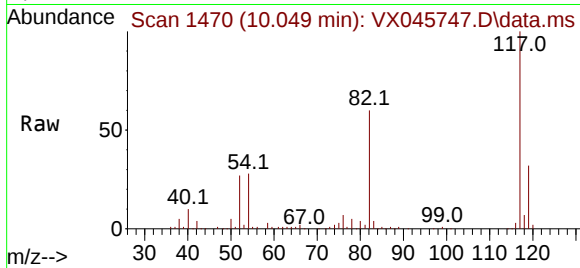

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045747.D
Acq: 11 Apr 2025 17:23

Tgt Ion:152 Resp: 50320
Ion Ratio Lower Upper
152 100
115 66.0 46.9 140.7
150 157.8 0.0 349.4

