
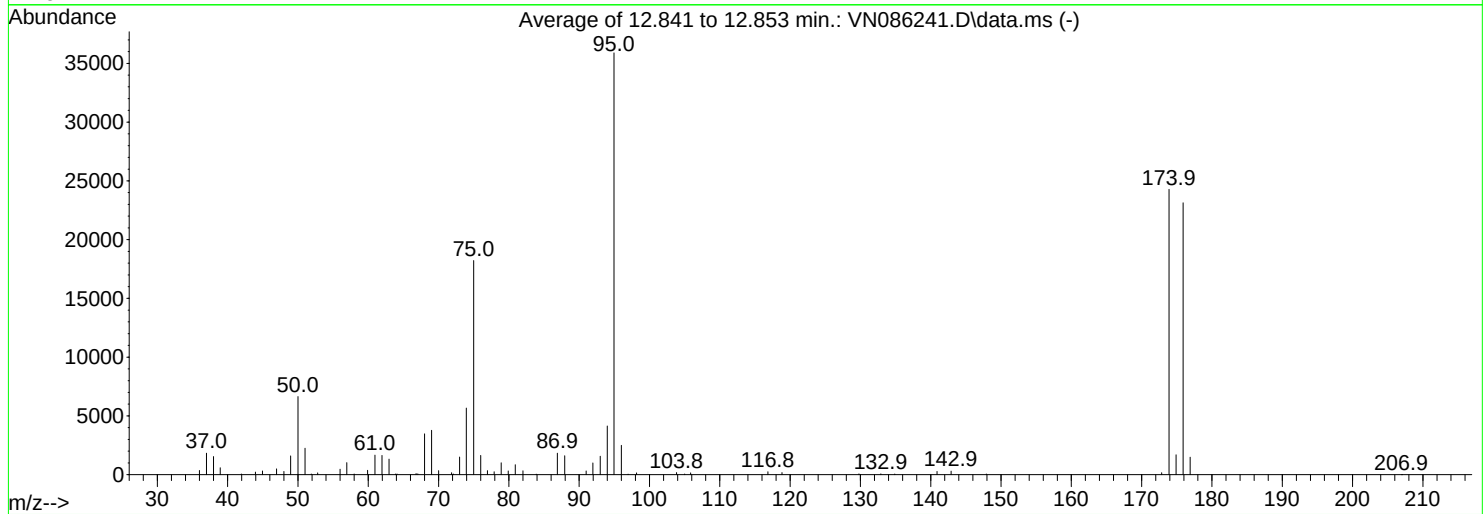


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041125\
Data File : VN086241.D
Acq On : 11 Apr 2025 09:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Tue Apr 08 14:20:04 2025

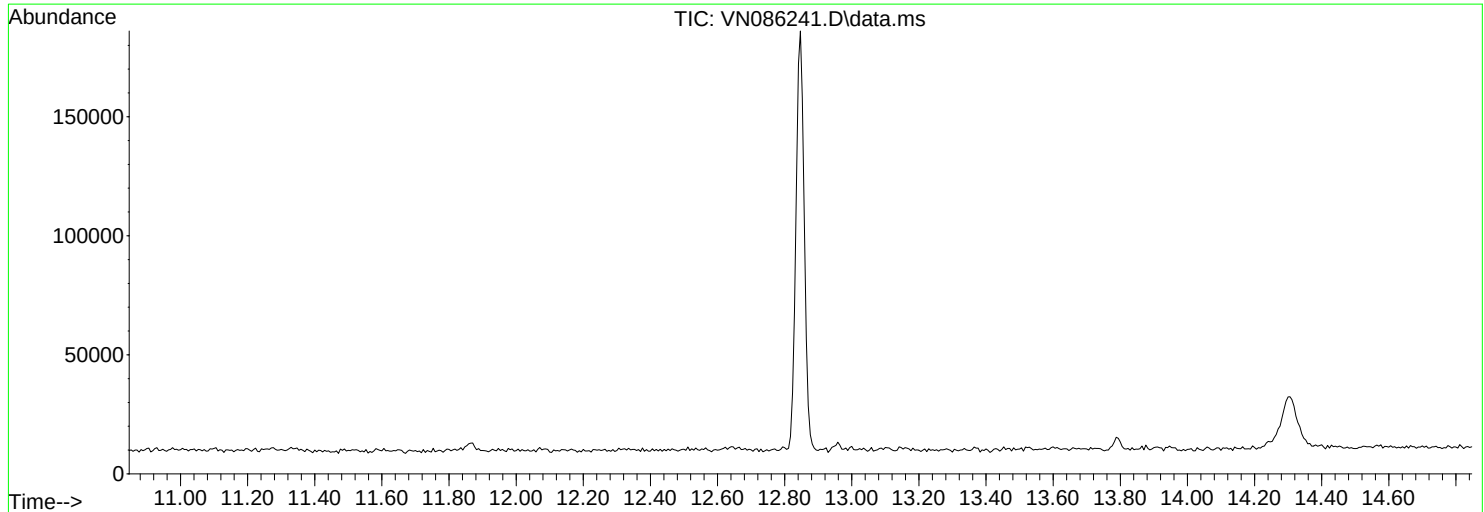

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	6647	PASS
75	95	30	60	50.8	18224	PASS
95	95	100	100	100.0	35896	PASS
96	95	5	9	6.9	2487	PASS
173	174	0.00	2	0.7	164	PASS
174	95	50	100	67.6	24277	PASS
175	174	5	9	7.0	1691	PASS
176	174	95	101	95.3	23128	PASS
177	176	5	9	6.4	1490	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	358	51.00	2252	64.10	58	76.00	1631
37.00	1820	51.90	51	66.80	90	76.95	341
38.00	1545	52.80	146	67.05	73	77.90	241
38.95	586	56.00	465	68.00	3478	78.90	1011
41.95	50	56.95	1020	69.00	3774	79.90	320
43.95	213	58.00	57	70.00	338	80.90	841
44.95	311	59.90	369	71.85	163	82.00	327
46.95	494	60.95	1668	72.10	61	83.90	41
48.00	270	61.95	1638	73.00	1497	86.90	1825
48.95	1601	62.95	1322	73.95	5669	87.95	1606
50.00	6647	63.90	55	75.00	18224	91.00	312

Average of 12.841 to 12.853 min.: VN086241.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.95	998	118.85	184	176.90	1490		
93.00	1567	129.80	62	206.95	1		
94.00	4145	132.90	71				
94.95	35896	134.90	51				
96.00	2487	140.90	269				
96.95	37	142.90	300				
98.15	155	147.90	55				
103.85	178	172.85	164				
105.00	51	173.90	24277				
105.85	149	174.90	1691				
116.85	250	175.90	23128				

Instrument :

MSVOA_N

ClientSampleId :

BFB