



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041425\
Data File : VX045754.D
Acq On : 14 Apr 2025 09:20
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Title : SW846 8260
Last Update : Wed Apr 02 03:11:43 2025

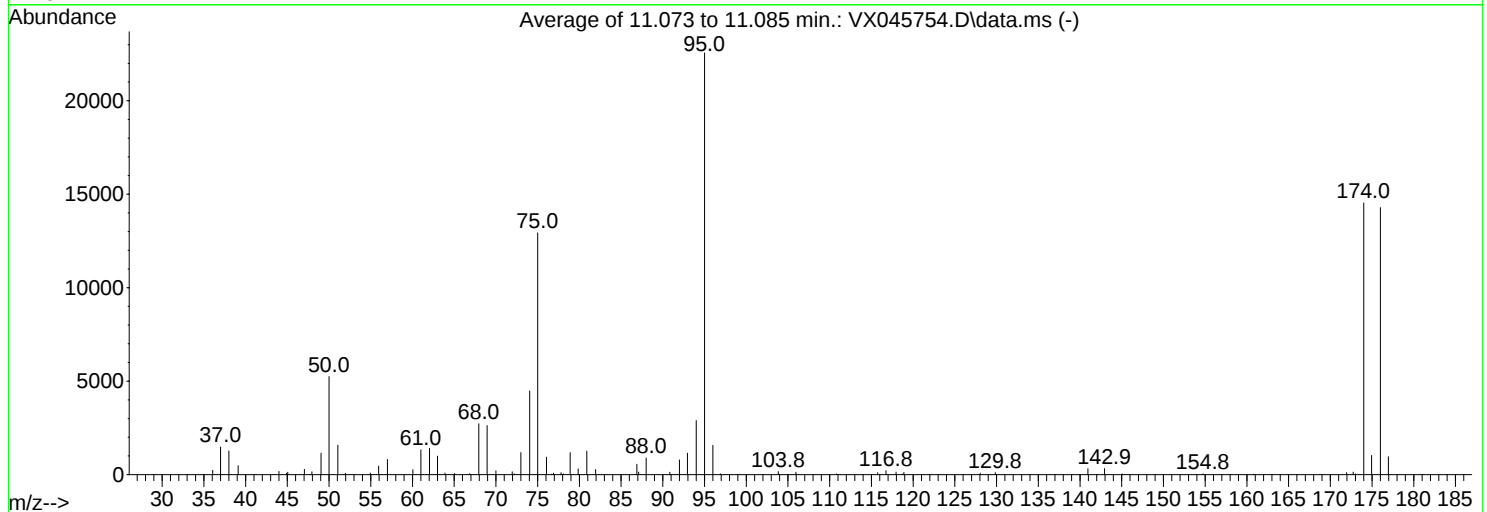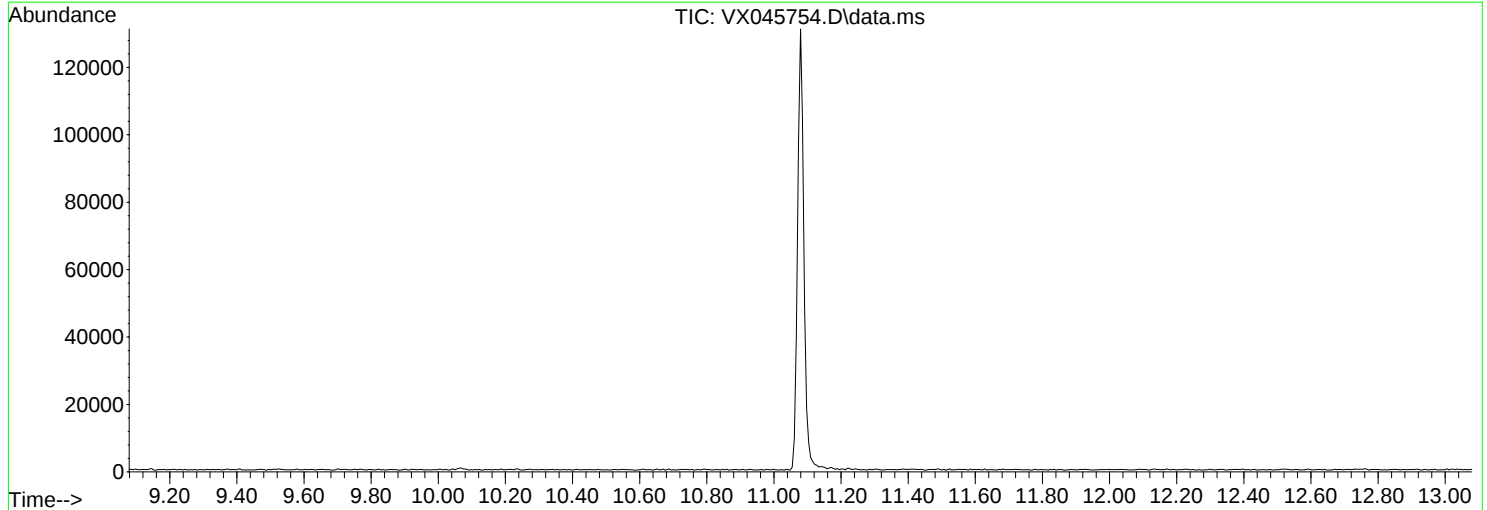

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.3	5250	PASS
75	95	30	60	57.3	12936	PASS
95	95	100	100	100.0	22563	PASS
96	95	5	9	6.9	1565	PASS
173	174	0.00	2	0.9	134	PASS
174	95	50	100	64.4	14532	PASS
175	174	5	9	7.1	1029	PASS
176	174	95	101	98.3	14284	PASS
177	176	5	9	6.7	956	PASS