
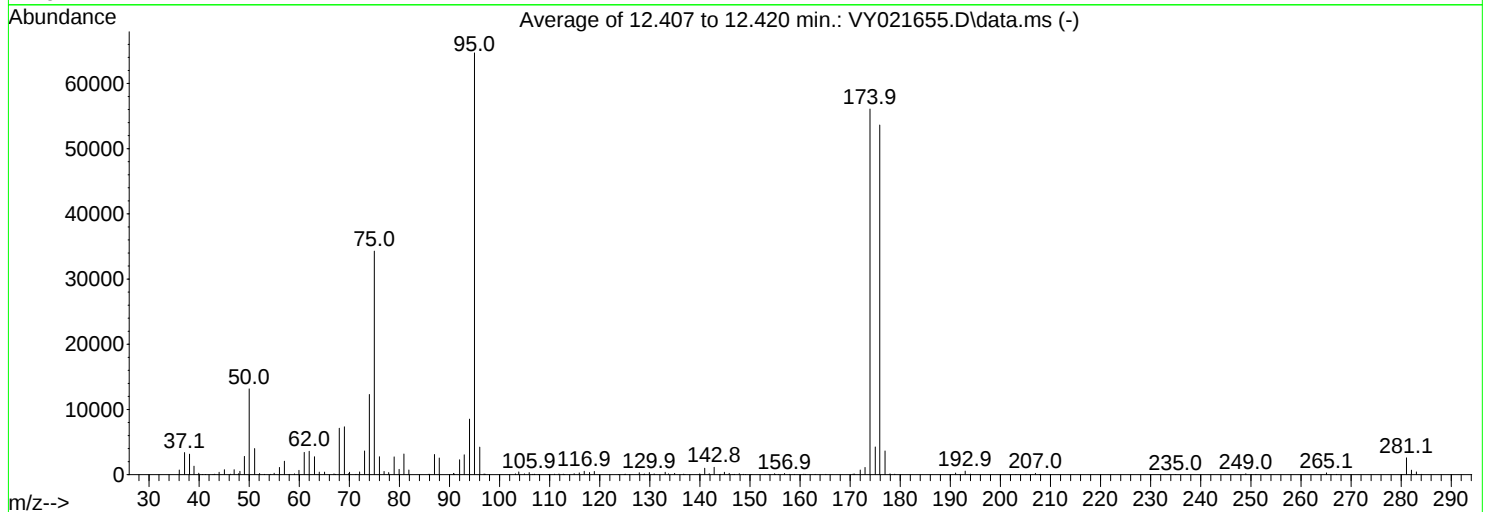


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032725\
Data File : VY021655.D
Acq On : 27 Mar 2025 09:23
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Title : SW846 8260
Last Update : Fri Mar 28 02:30:29 2025

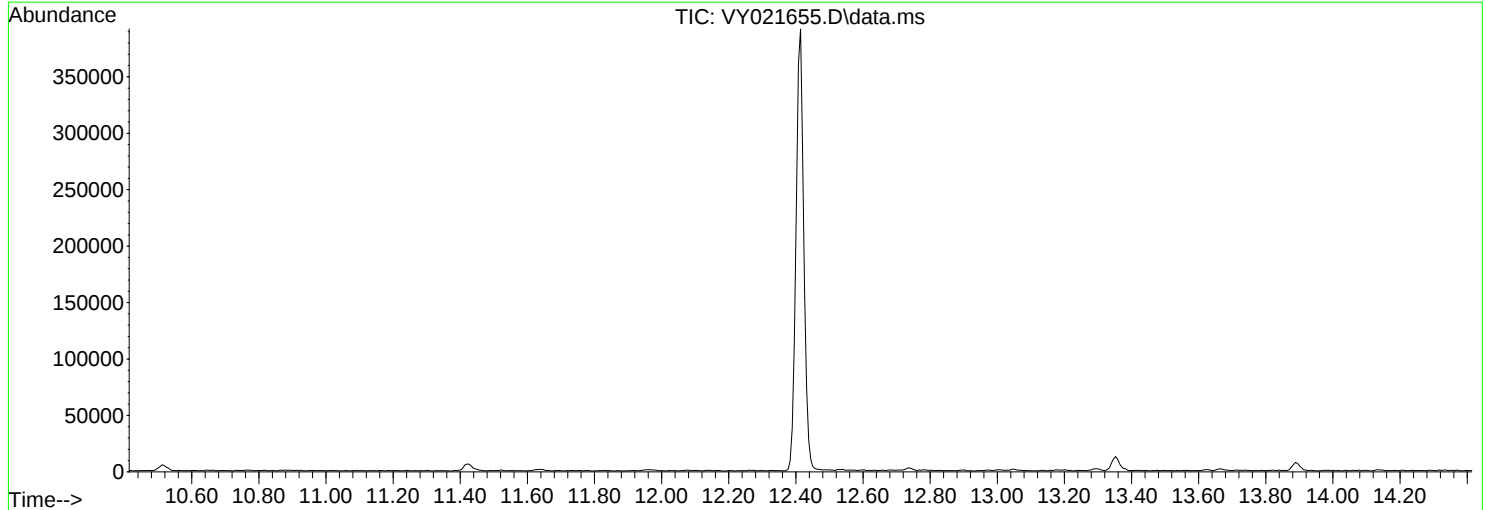

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	13171	PASS
75	95	30	60	53.0	34296	PASS
95	95	100	100	100.0	64701	PASS
96	95	5	9	6.5	4216	PASS
173	174	0.00	2	2.0	1112	PASS
174	95	50	100	86.7	56080	PASS
175	174	5	9	7.6	4256	PASS
176	174	95	101	95.6	53624	PASS
177	176	5	9	6.8	3635	PASS