
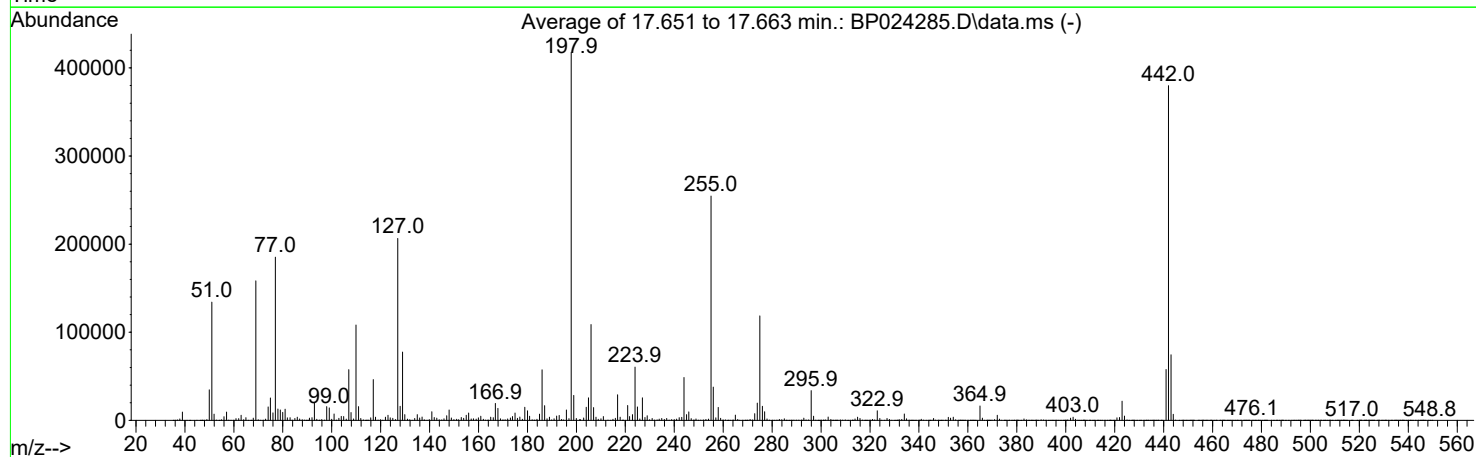


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041525\
Data File : BP024285.D
Acq On : 15 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 15 04:48:42 2025

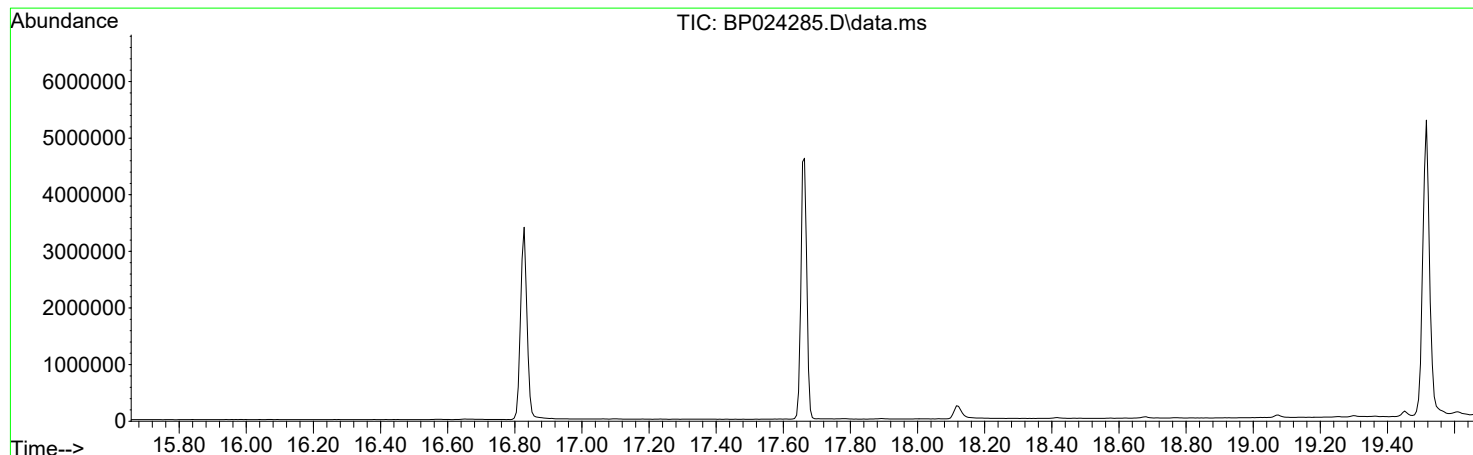

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	134290	PASS
68	69	0.00	2	1.6	2534	PASS
69	198	0.00	100	37.9	158323	PASS
70	69	0.00	2	0.5	753	PASS
127	198	10	80	49.5	206529	PASS
197	198	0.00	2	0.5	1994	PASS
198	198	100	100	100.0	417478	PASS
199	198	5	9	6.8	28386	PASS
275	198	10	60	28.4	118669	PASS
365	198	1	100	3.9	16401	PASS
441	198	0.01	100	13.8	57731	PASS
442	442	100	100	100.0	379838	PASS
443	442	15	24	19.6	74376	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/15/2025	BNA_P	<u>BP024285.D</u>
Compound Name	Response	Retention Time
DDT	1626693	20.804
DDD	24498	20.392
DDE	2415	19.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26913	1653606	1.63

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041525\
Data File : BP024285.D
Acq On : 15 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 15 12:53:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

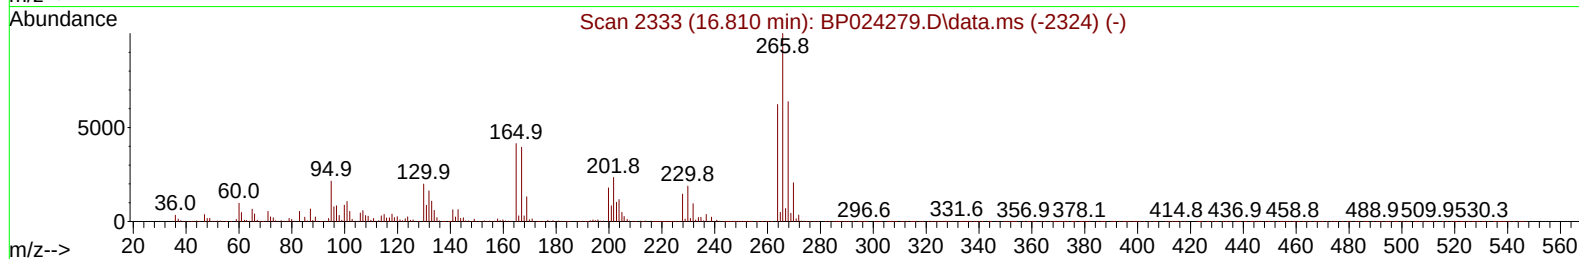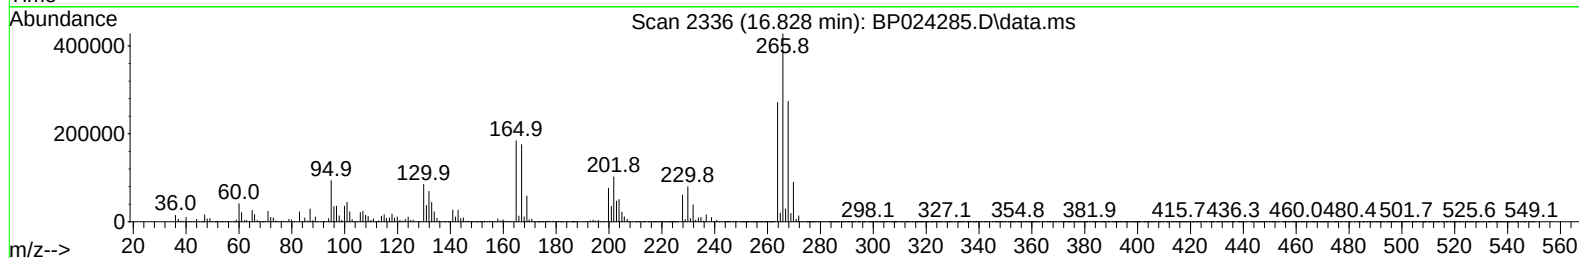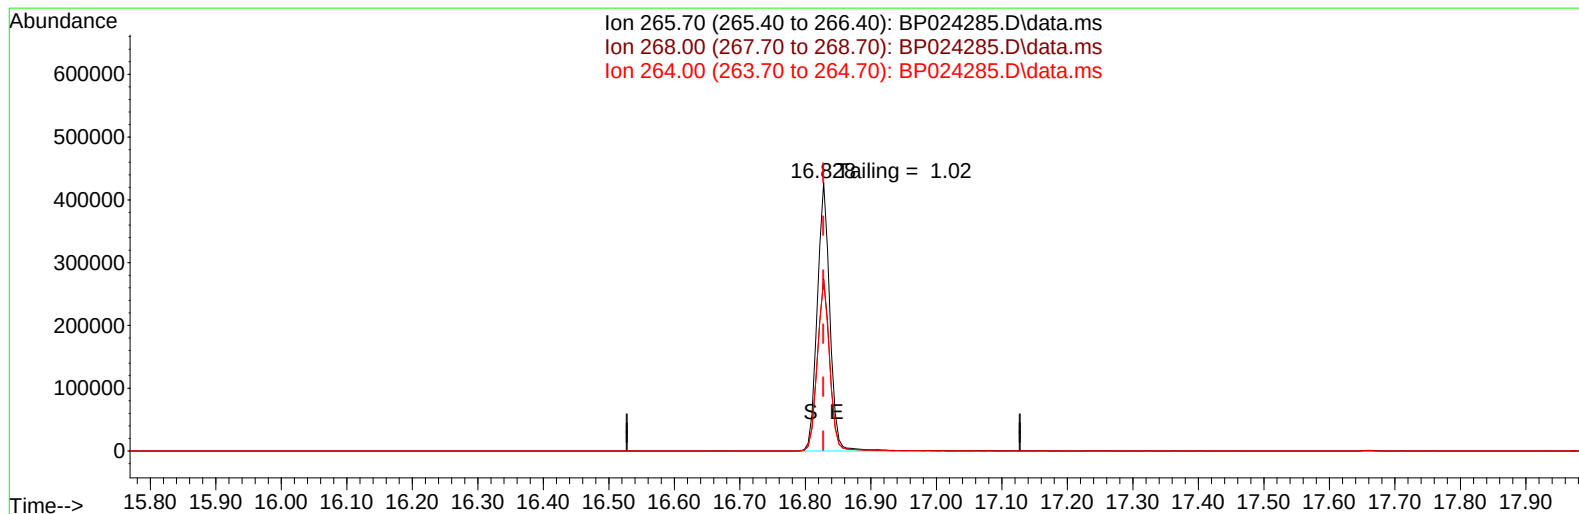

TIC: BP024285.D\data.ms

(70) Pentachlorophenol (C)

16.828min (+ 0.000) 207154.57 ng




response 569074

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.97
264.00	62.20	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041525\
Data File : BP024285.D
Acq On : 15 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 15 12:53:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

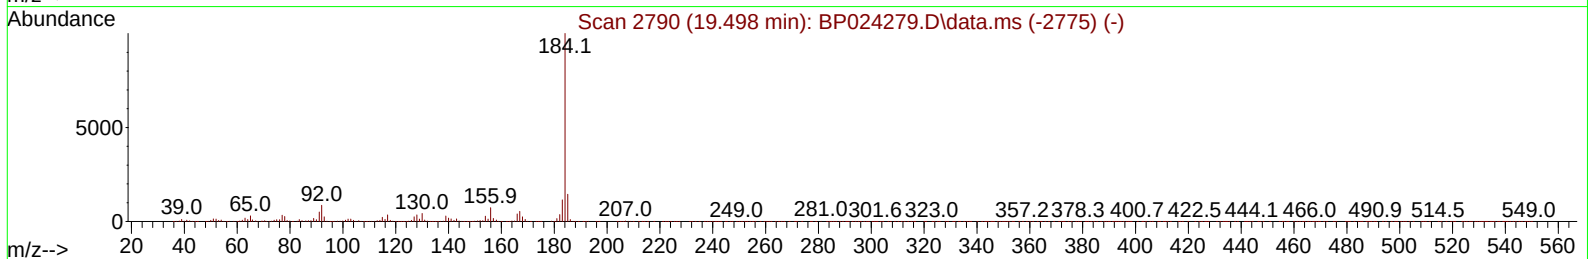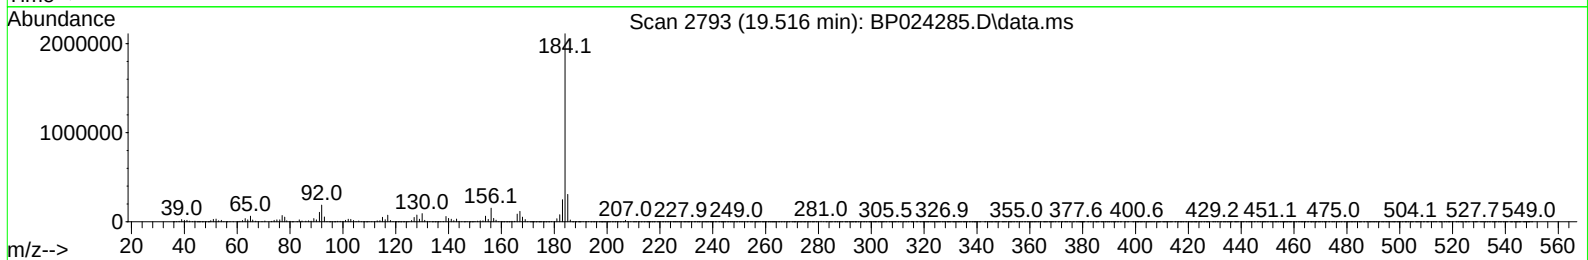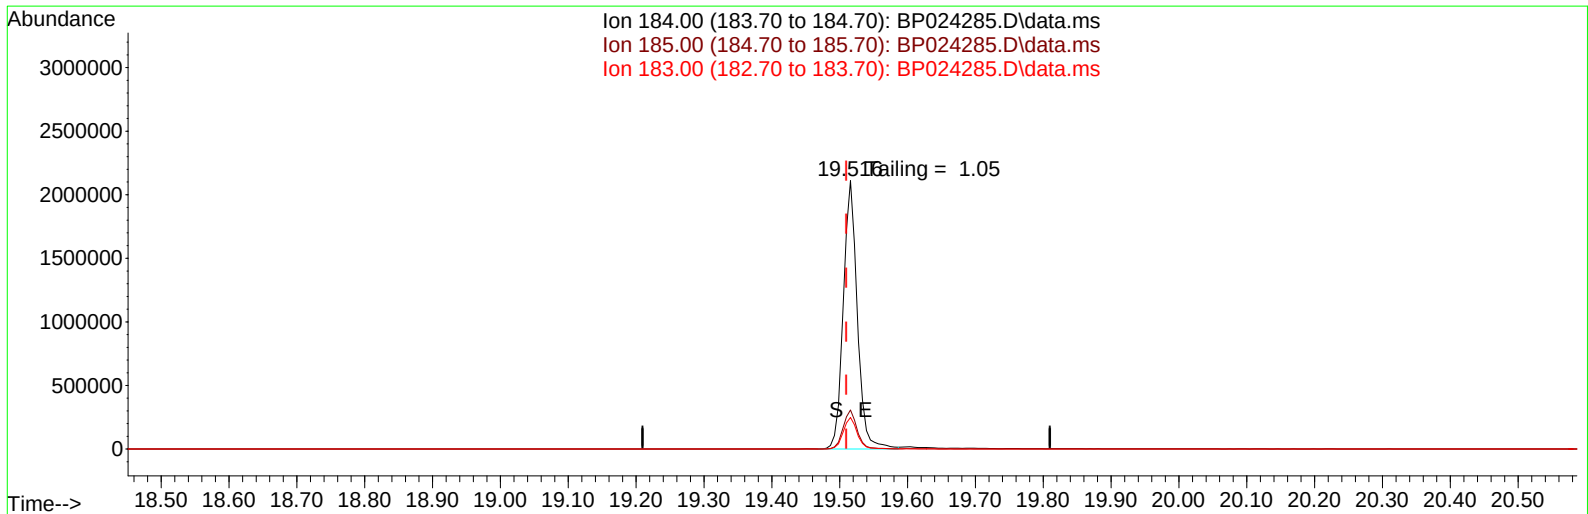

TIC: BP024285.D\data.ms

(77) Benzidine

19.516min (+ 0.006) 25118.03 ng

response 3032050

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.58
183.00	11.50	11.75
0.00	0.00	0.00