
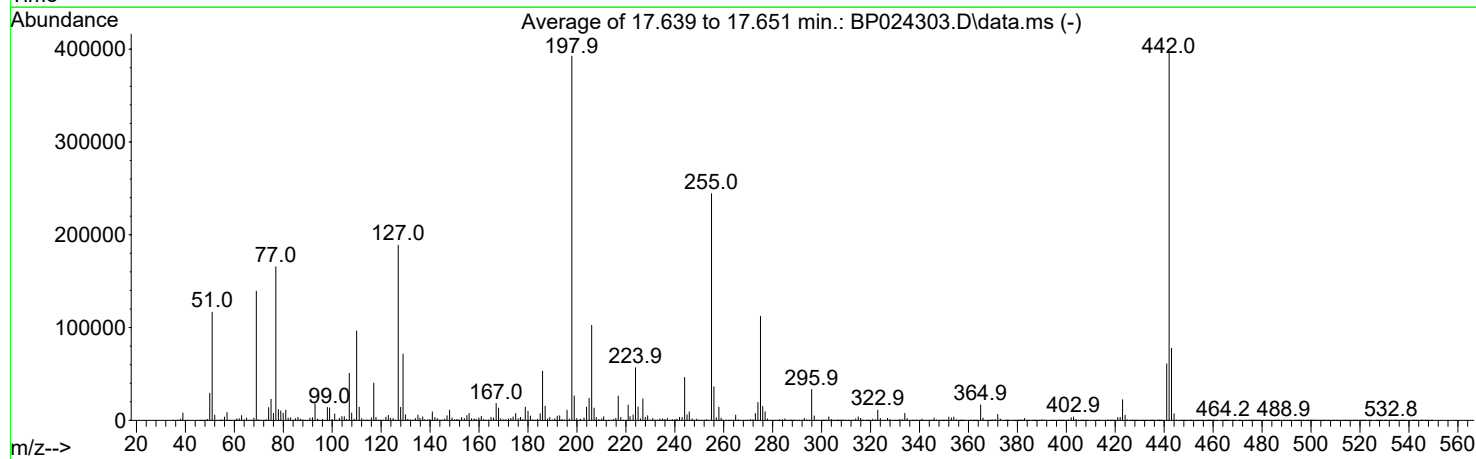


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041625\
Data File : BP024303.D
Acq On : 16 Apr 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 15 04:48:42 2025

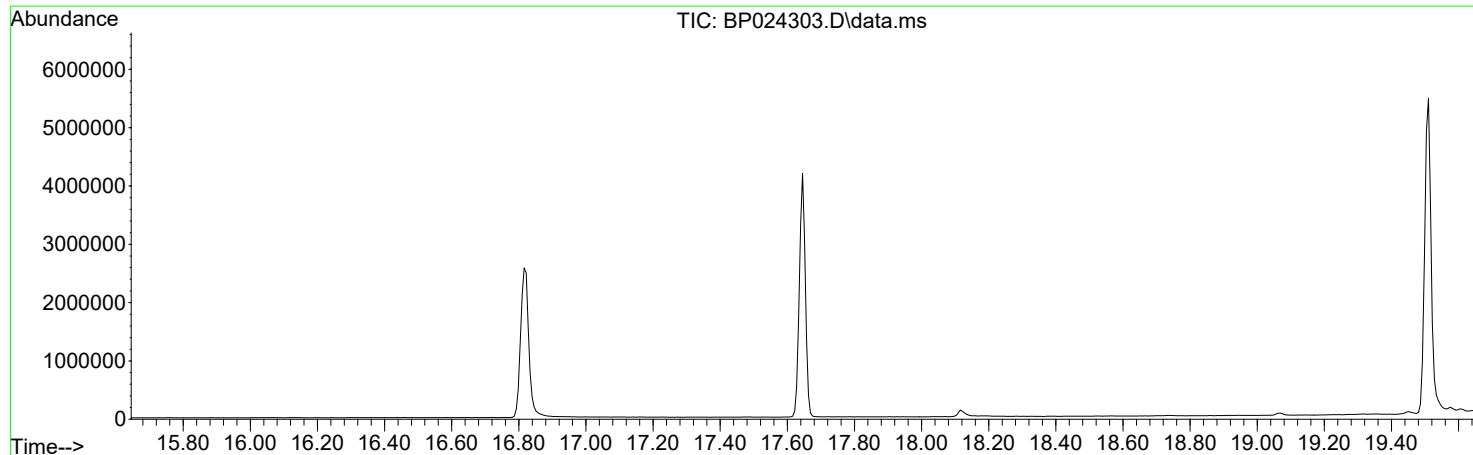

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	116586	PASS
68	69	0.00	2	1.7	2375	PASS
69	198	0.00	100	35.5	139114	PASS
70	69	0.00	2	0.5	719	PASS
127	198	10	80	48.1	188795	PASS
197	198	0.00	2	0.3	1342	PASS
198	198	100	100	100.0	392321	PASS
199	198	5	9	6.7	26445	PASS
275	198	10	60	28.6	112299	PASS
365	198	1	100	4.3	16793	PASS
441	198	0.01	100	15.5	60943	PASS
442	442	100	100	100.0	396330	PASS
443	442	15	24	19.6	77746	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/16/2025	BNA_P	<u>BP024303.D</u>
Compound Name	Response	Retention Time
DDT	1484042	20.792
DDD	46977	20.345
DDE	1465	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48442	1532484	3.16

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041625\
Data File : BP024303.D
Acq On : 16 Apr 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 16 11:22:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

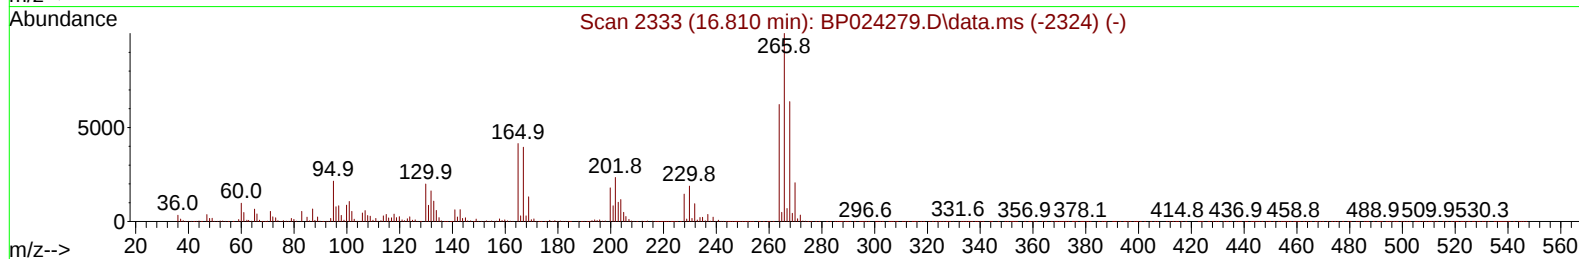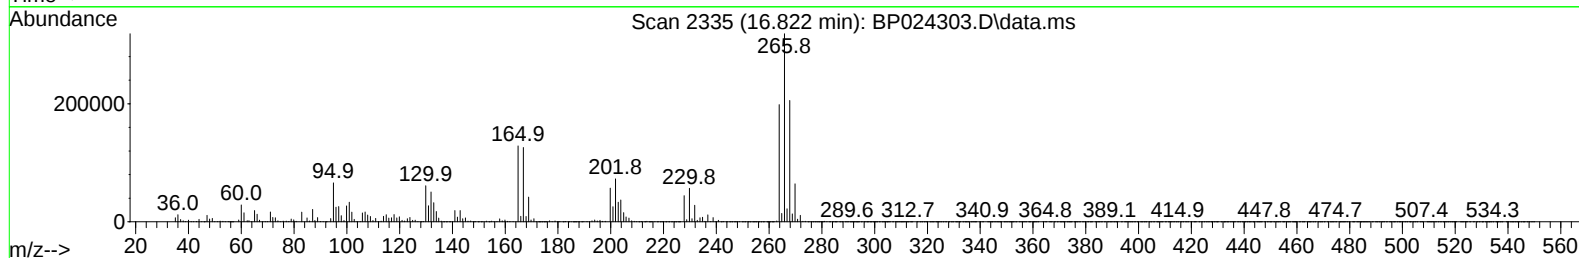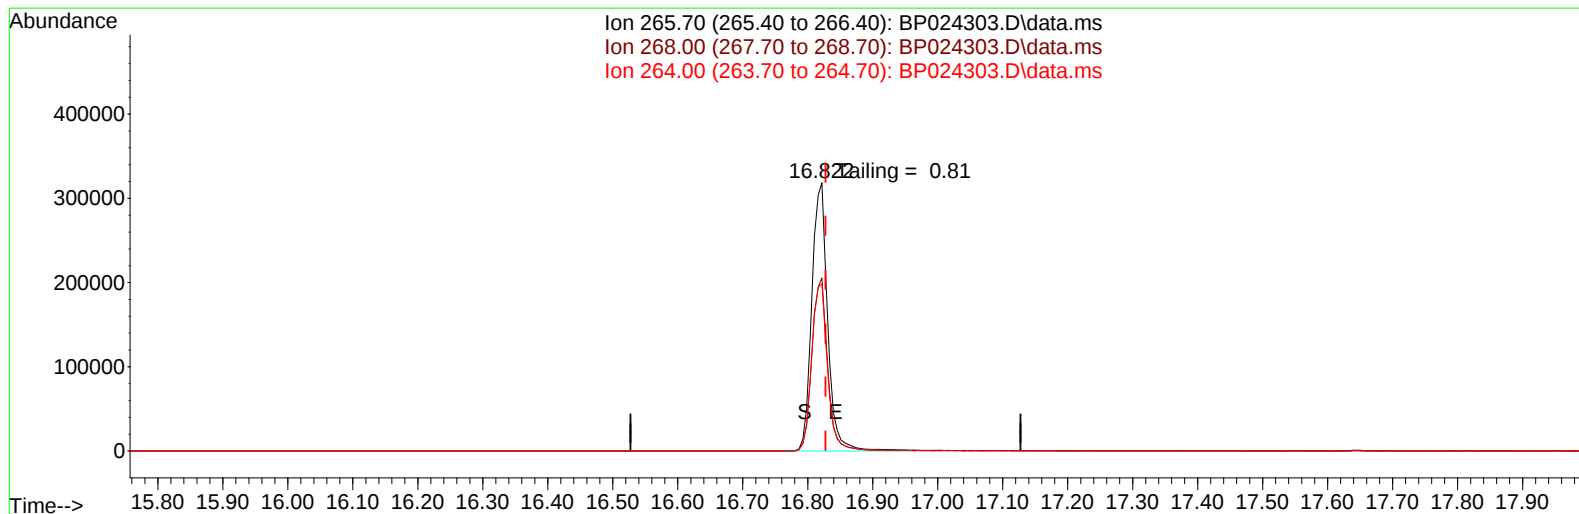

TIC: BP024303.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.006) 63083.83 ng




response 543342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.53
264.00	62.20	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041625\
Data File : BP024303.D
Acq On : 16 Apr 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 16 11:22:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

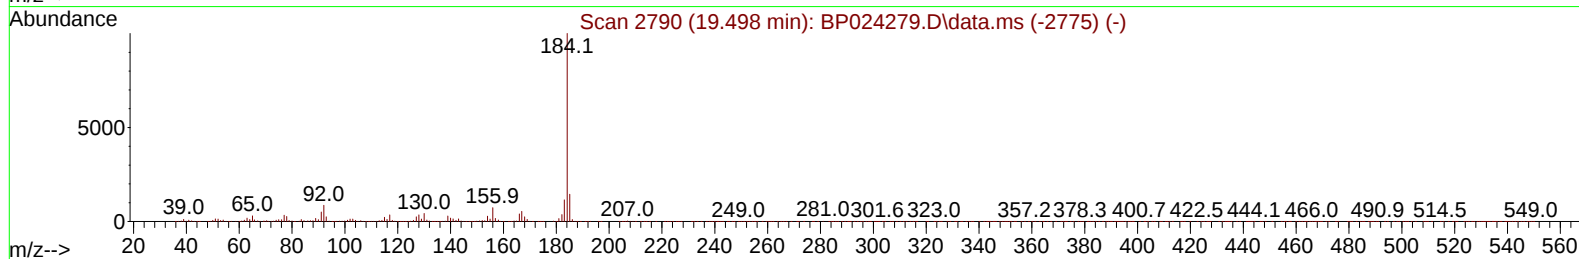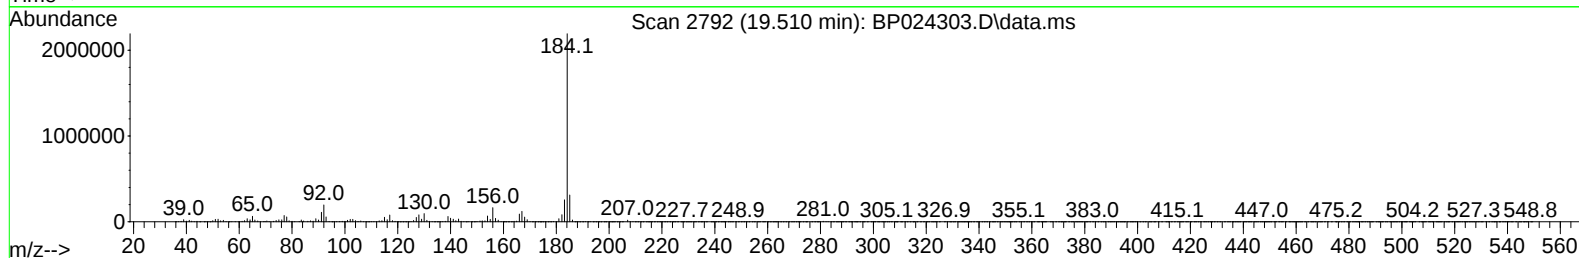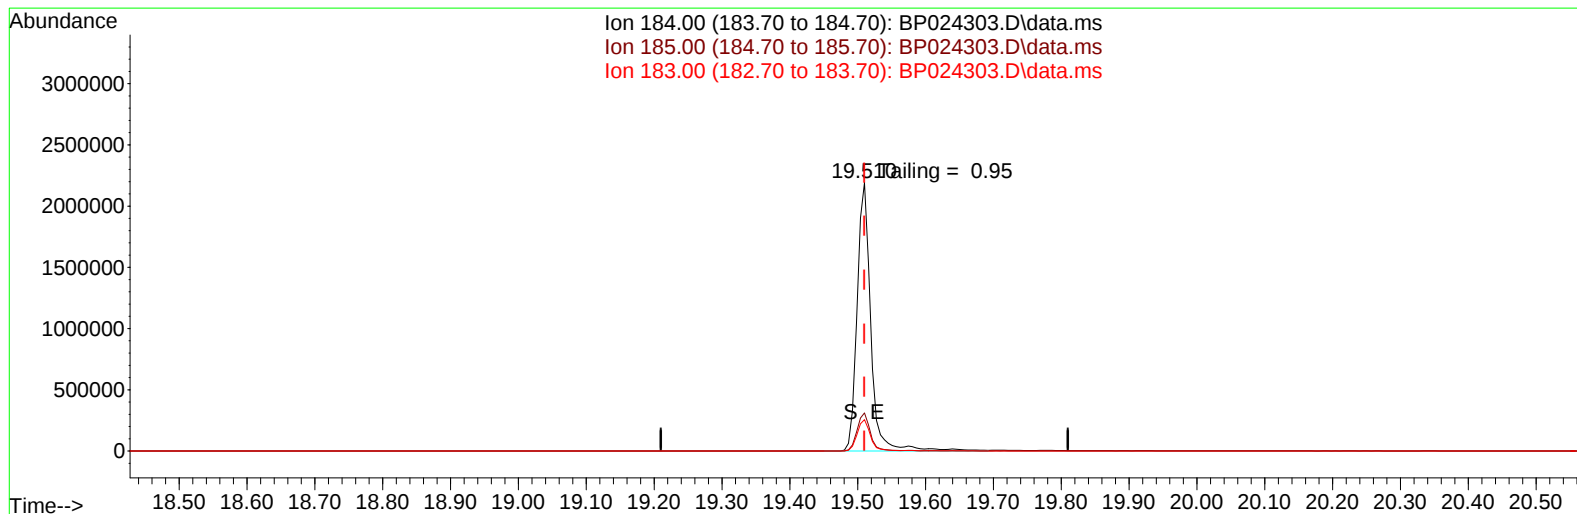

TIC: BP024303.D\data.ms

(77) Benzidine

19.510min (+ 0.000) 173060.25 ng

response 2961475

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.19
183.00	11.50	11.69
0.00	0.00	0.00