

**SOP ID:** M3510C,3580A-Extraction DRO-12

**Clean Up SOP #:** N/A **Extraction Start Date :** 04/16/2025

**Matrix :** Water **Extraction Start Time :** 10:05

**Weigh By:** N/A **Extraction By:** RJ **Extraction End Date :** 04/16/2025

**Balance check:** N/A **Filter By:** RJ **Extraction End Time :** 14:40

**Balance ID:** N/A **pH Meter ID:** N/A **Concentration By:** EH

**pH Strip Lot#:** E3880 **Hood ID:** 4,6,7 **Supervisor By :** RUPESH

**Extraction Method:** ☒ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☐ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Surrogate	1.0ML	20 PPM	PP24162
Spike Sol 1	1.0ML	20 PPM	PP24180
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3926
Baked Na2SO4	N/A	EP2599
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

**Extraction Conformance/Non-Conformance Comments:**

1.5 ML Vial lot# 2210443.

**KD Bath ID:** WATER BATH-1 **Envap ID:** NEVAP-02


**KD Bath Temperature:** 60 °C **Envap Temperature:** 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
4/16/25	RS (Bath Lab)	Y-P PestipCB
14:45	Preparation Group	Analysis Group

Analytical Method: M3510C,3580A-Extraction DRO-12

Concentration Date: 04/16/2025

Sample ID	Client Sample ID	Test	g / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB167614BL	PB167614BL	Diesel Range Organics	1000	6	ritesh	Evelyn	1			SEP-1
PB167614BS	PB167614BS	Diesel Range Organics	1000	6	ritesh	Evelyn	1			2
PB167614BSD	PB167614BSD	Diesel Range Organics	1000	6	ritesh	Evelyn	1			3
Q1812-02	RINSE-EB-TANK-041525	Diesel Range Organics	900	6	ritesh	Evelyn	1	H		4
Q1812-03	RINSE-EB-PUMP-041525	Diesel Range Organics	990	6	ritesh	Evelyn	1	H		5

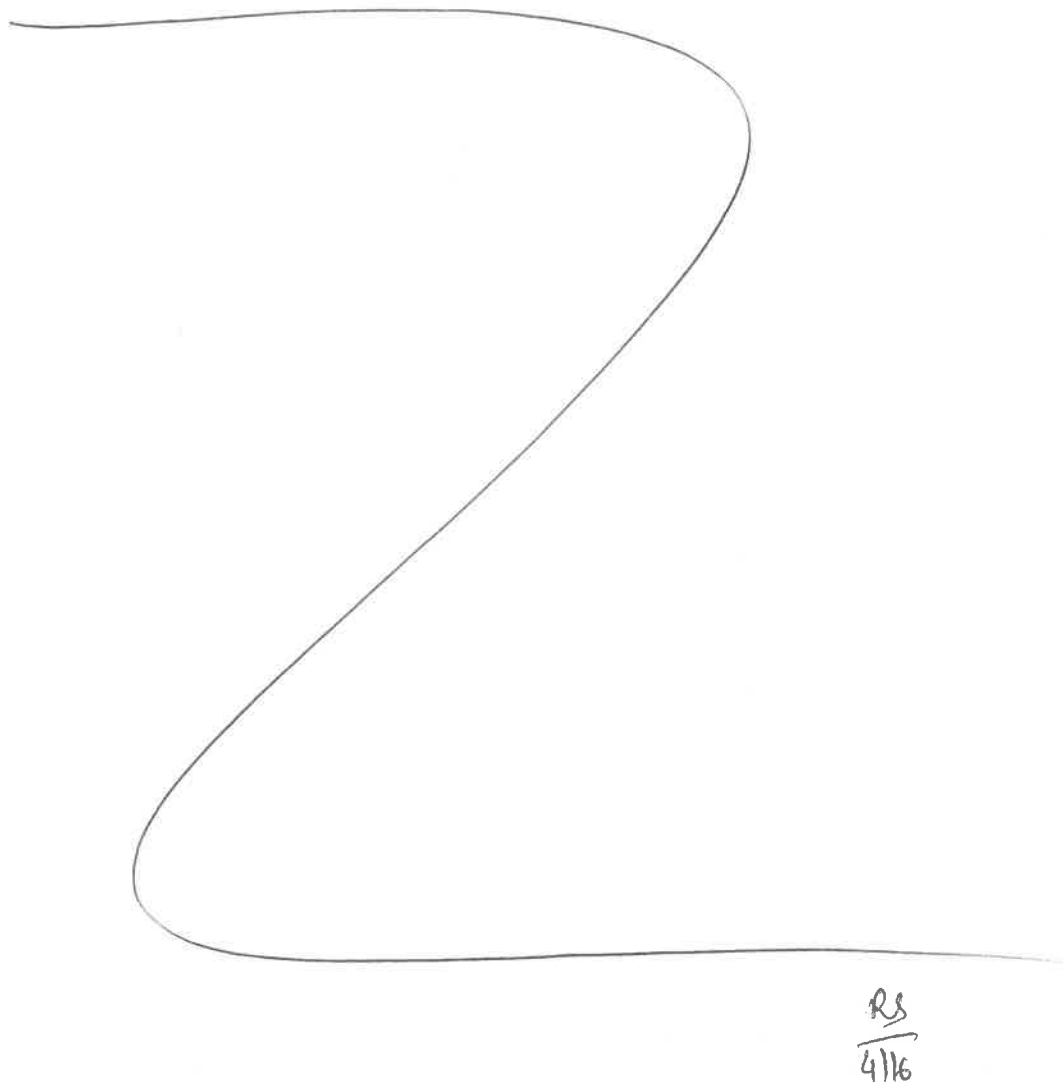

RS  
4/16