

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032625\
 Data File : FB031620.D
 Signal(s) : FID2B.CH
 Acq On : 26 Mar 2025 13:26
 Operator : YP/AJ
 Sample : FB032625GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB032625GROICV

Integration File: Calibration.e
 Quant Time: Mar 26 13:18:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032625.M
 Quant Title :
 QLast Update : Wed Mar 26 12:17:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	403306	18.168 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.724	735906	28.901 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	1022563	28.813 ng/ml
3) t n-Heptane	7.754	301313	9.272 ng/ml
4) t Benzene	7.895	406758	9.636 ng/ml
6) t Toluene	10.622	1199206	30.198 ng/ml
7) t Ethylbenzene	13.059	361336	10.094 ng/ml
8) t m-Xylene	13.193	805981	20.544 ng/ml
9) t O-Xylene	13.921	769117	20.798 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	618790	22.500 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032625\
Data File : FB031620.D
Signal(s) : FID2B.CH
Acq On : 26 Mar 2025 13:26
Operator : YP/AJ
Sample : FB032625GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB032625GROICV

Integration File: Calibration.e
Quant Time: Mar 26 13:18:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032625.M
Quant Title :
QLast Update : Wed Mar 26 12:17:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

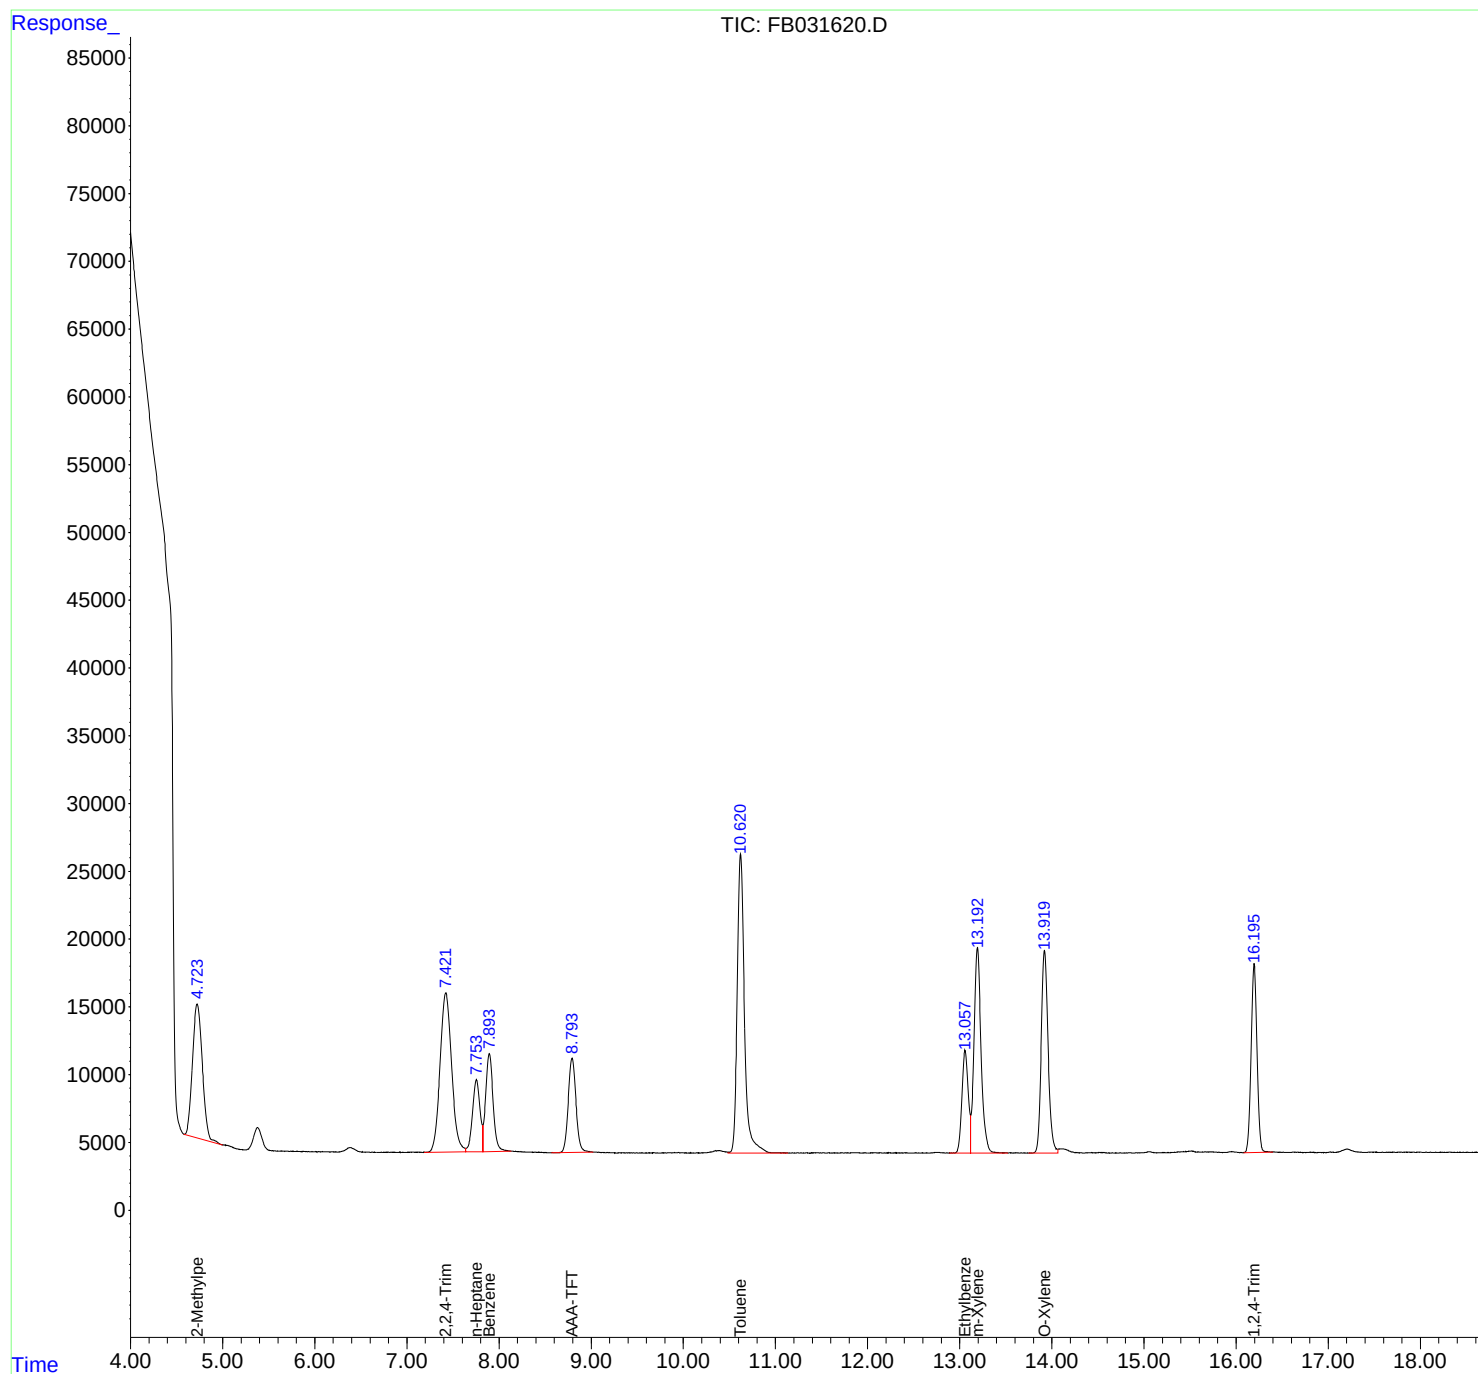


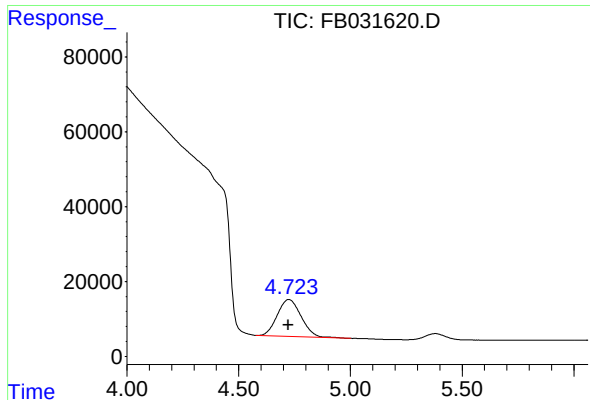

#1 2-Methylpentane


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 735906
Conc: 28.90 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032625GROICV

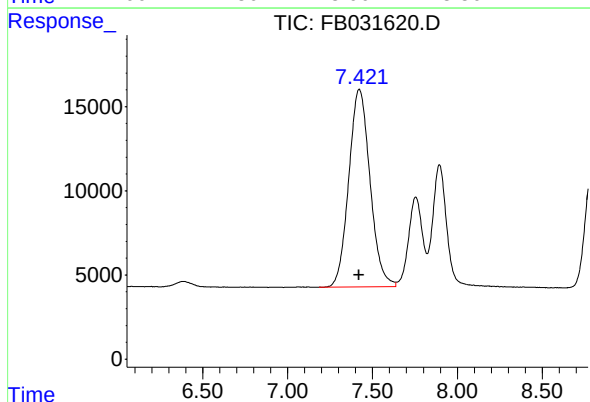


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.001 min
Response: 1022563
Conc: 28.81 ng/ml

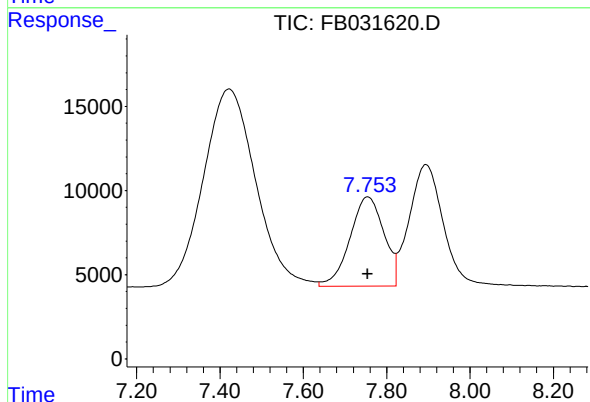


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 301313
Conc: 9.27 ng/ml

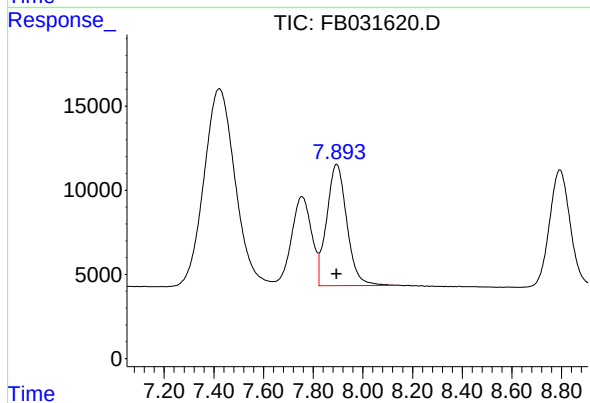

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 406758
Conc: 9.64 ng/ml

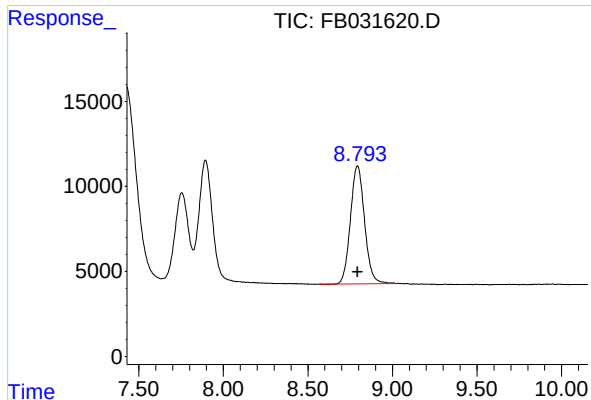

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.001 min
Response: 403306
Conc: 18.17 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032625GROICV

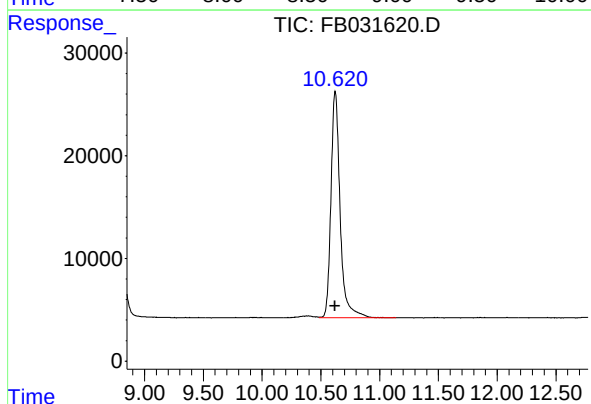


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 1199206
Conc: 30.20 ng/ml

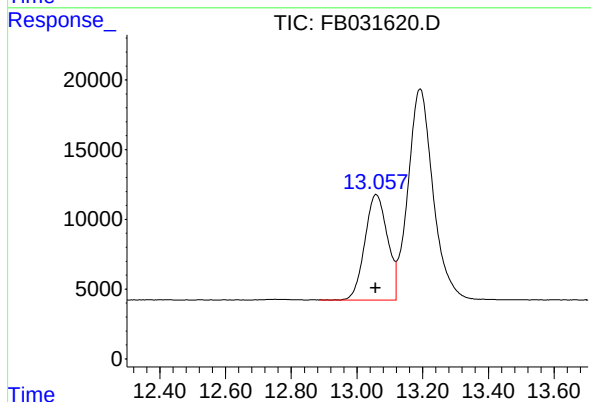


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.002 min
Response: 361336
Conc: 10.09 ng/ml

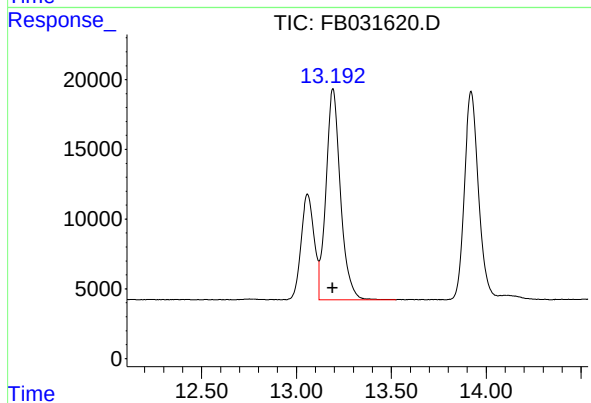

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.002 min
Response: 805981
Conc: 20.54 ng/ml

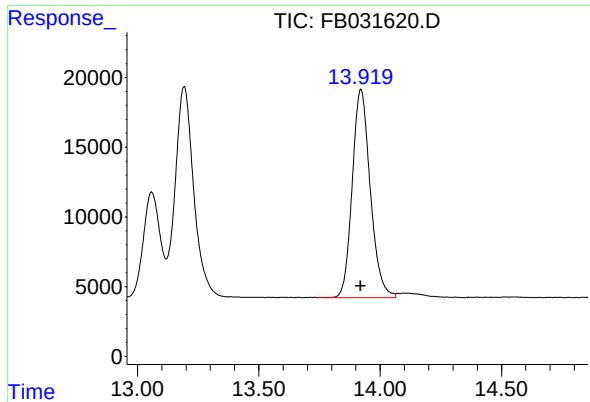

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.001 min
Response: 769117
Conc: 20.80 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032625GROICV

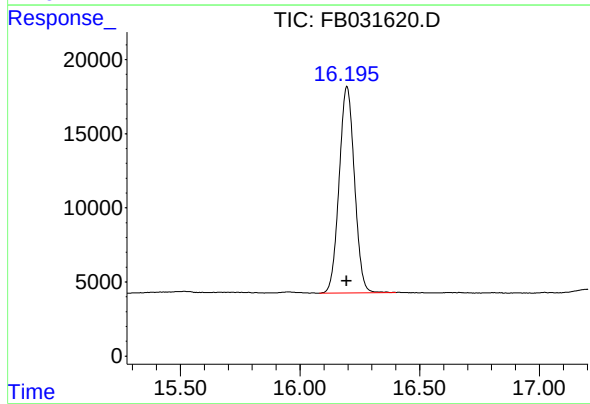

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.000 min
Response: 618790
Conc: 22.50 ng/ml