
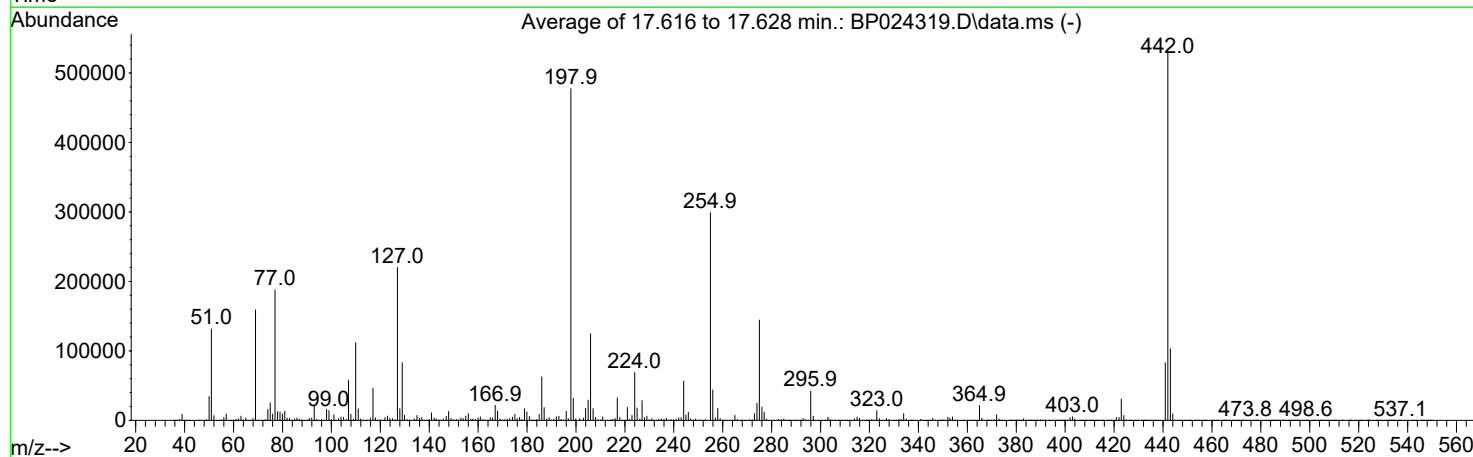


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041725\
Data File : BP024319.D
Acq On : 17 Apr 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 15 04:48:42 2025

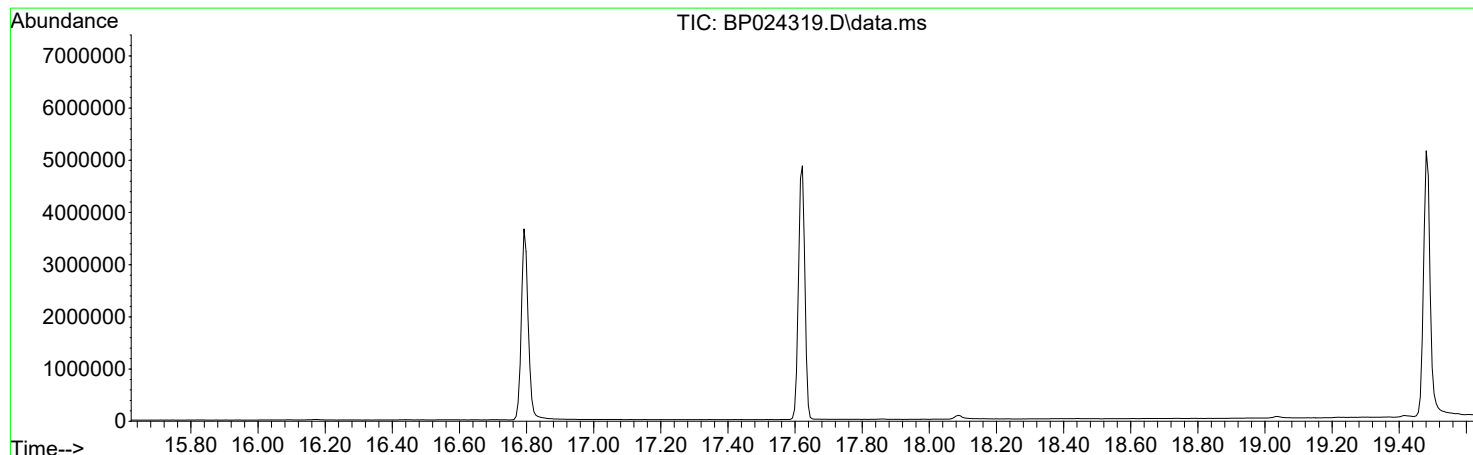

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	131819	PASS
68	69	0.00	2	1.7	2691	PASS
69	198	0.00	100	33.3	159149	PASS
70	69	0.00	2	0.4	664	PASS
127	198	10	80	46.1	219887	PASS
197	198	0.00	2	0.5	2326	PASS
198	198	100	100	100.0	477482	PASS
199	198	5	9	6.7	32125	PASS
275	198	10	60	30.2	144359	PASS
365	198	1	100	4.5	21282	PASS
441	198	0.01	100	17.4	82883	PASS
442	442	100	100	100.0	529482	PASS
443	442	15	24	19.4	102868	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/17/2025	BNA_P	<u>BP024319.D</u>
Compound Name	Response	Retention Time
DDT	1782977	20.769
DDD	41005	20.31
DDE	3233	19.781
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44238	1827215	2.42

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041725\
Data File : BP024319.D
Acq On : 17 Apr 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 17 12:47:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

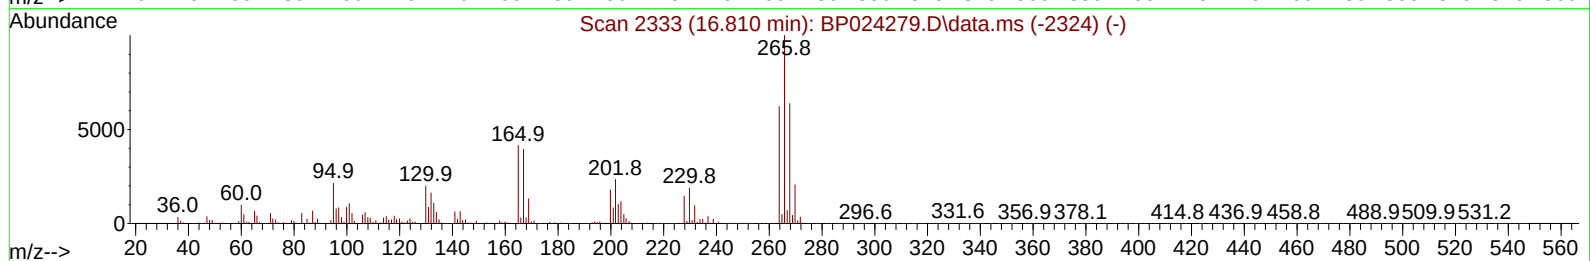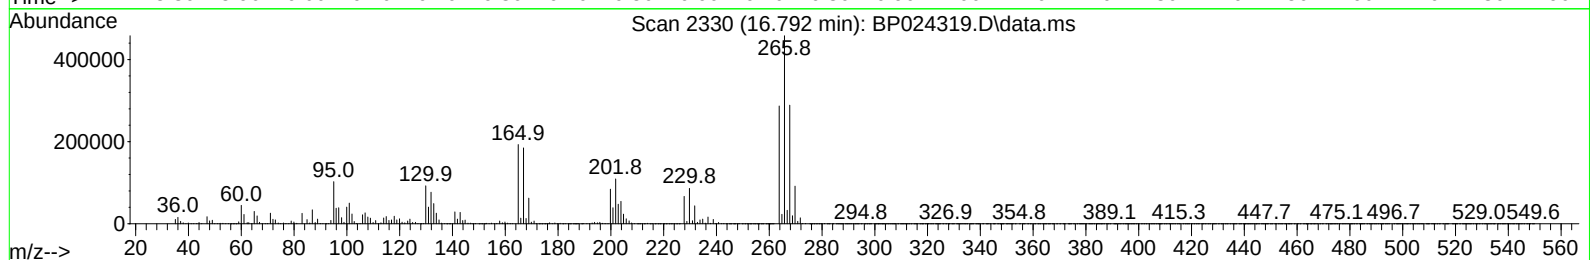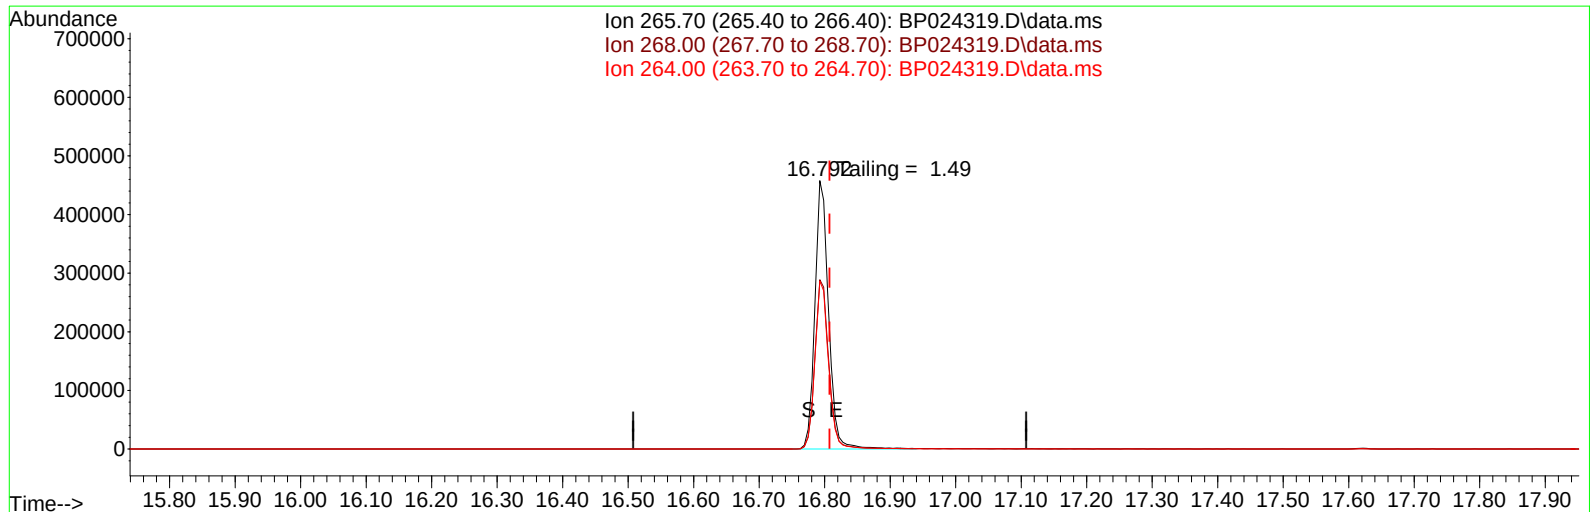

TIC: BP024319.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.015) 3494703.78 ng




response 665367

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.09
264.00	62.20	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041725\
Data File : BP024319.D
Acq On : 17 Apr 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 17 12:47:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 15 04:48:42 2025
Response via : Initial Calibration

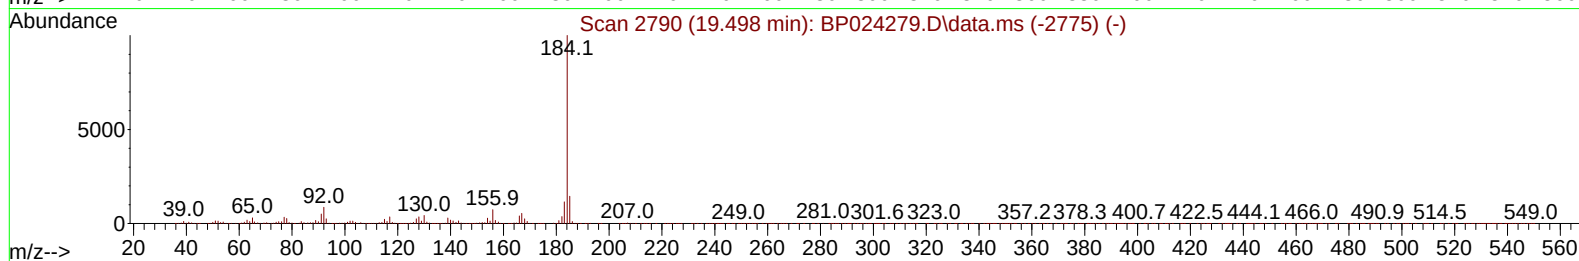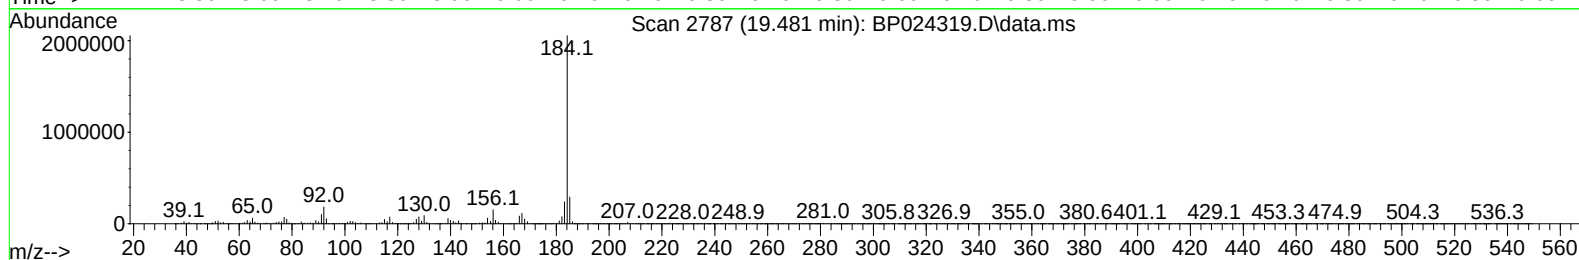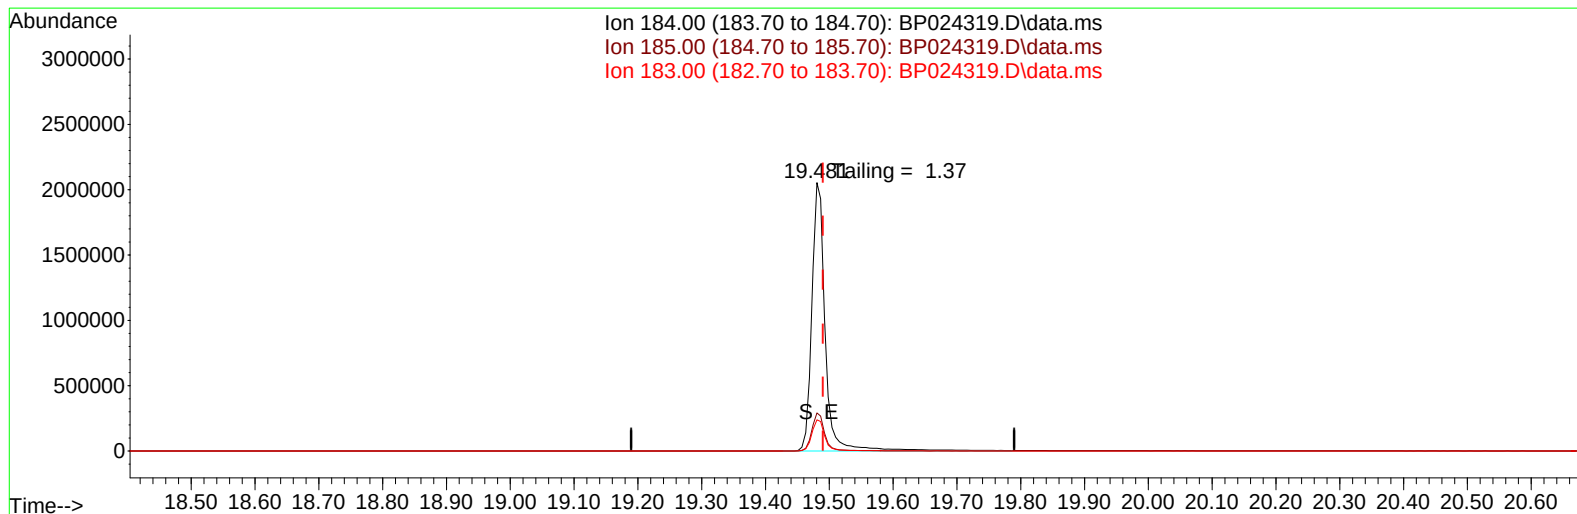

TIC: BP024319.D\data.ms

(77) Benzidine

19.481min (-0.009) 4514488.36 ng

response 2975698

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.21
183.00	11.50	11.67
0.00	0.00	0.00