
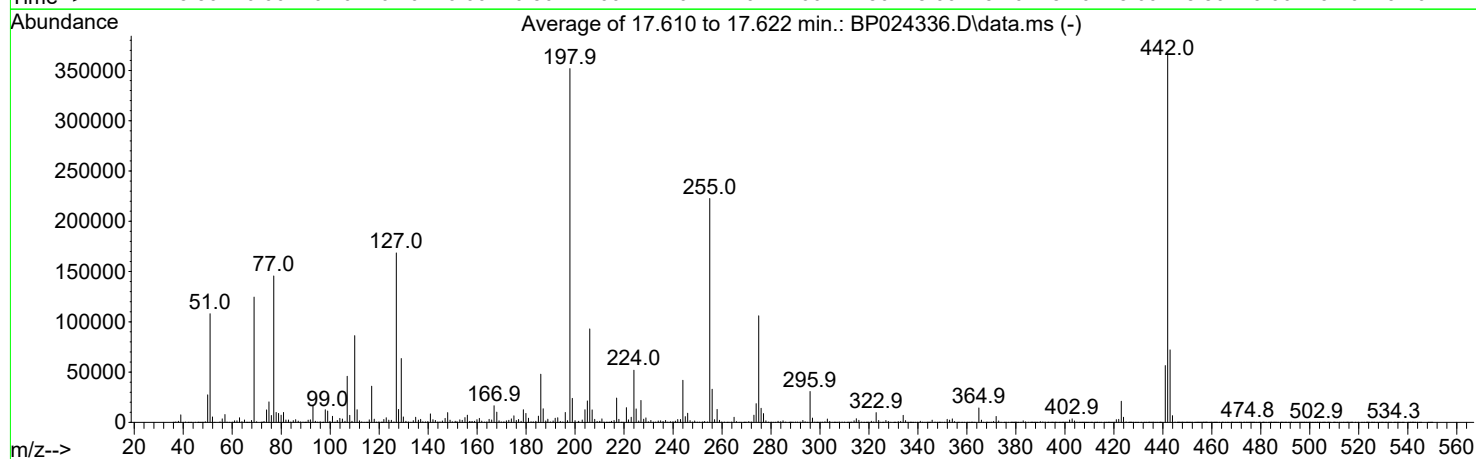


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041825\
Data File : BP024336.D
Acq On : 18 Apr 2025 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

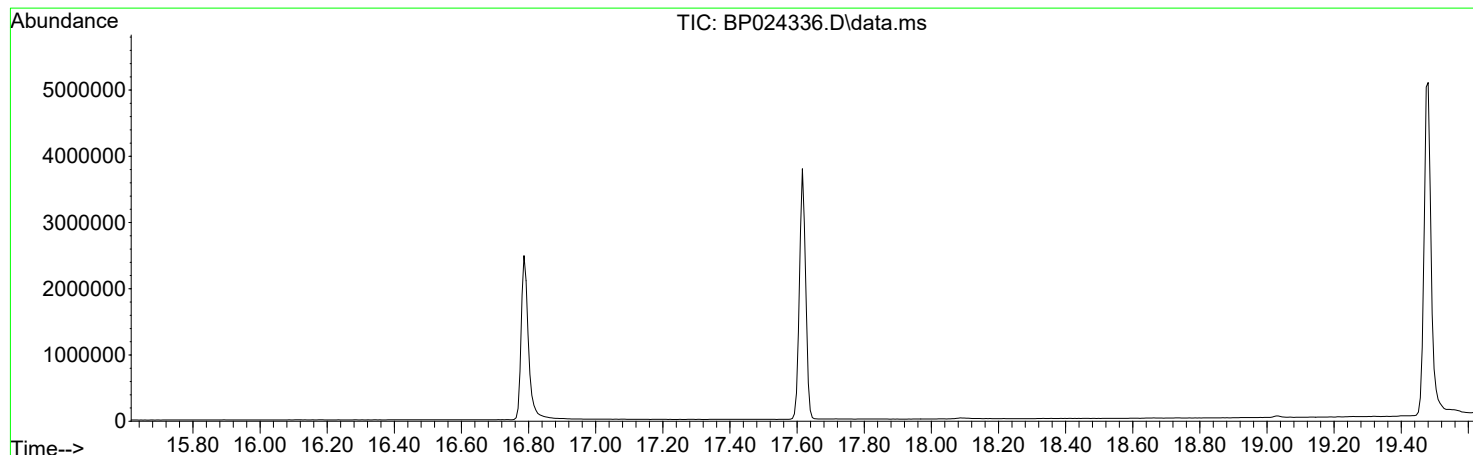

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	108143	PASS
68	69	0.00	2	1.6	1996	PASS
69	198	0.00	100	35.4	124683	PASS
70	69	0.00	2	0.5	644	PASS
127	198	10	80	47.9	168583	PASS
197	198	0.00	2	0.5	1755	PASS
198	198	100	100	100.0	351930	PASS
199	198	5	9	6.8	23888	PASS
275	198	10	60	30.1	106019	PASS
365	198	1	100	4.1	14287	PASS
441	198	0.01	100	16.0	56472	PASS
442	442	100	100	100.0	365874	PASS
443	442	15	24	19.7	72056	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/18/2025	BNA_P	<u>BP024336.D</u>
Compound Name	Response	Retention Time
DDT	1361256	20.763
DDD	28179	20.304
DDE	2295	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30474	1391730	2.19

Instrument :
BNA_P
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041825\  
Data File : BP024336.D  
Acq On    : 18 Apr 2025  10:32  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 18 12:10:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

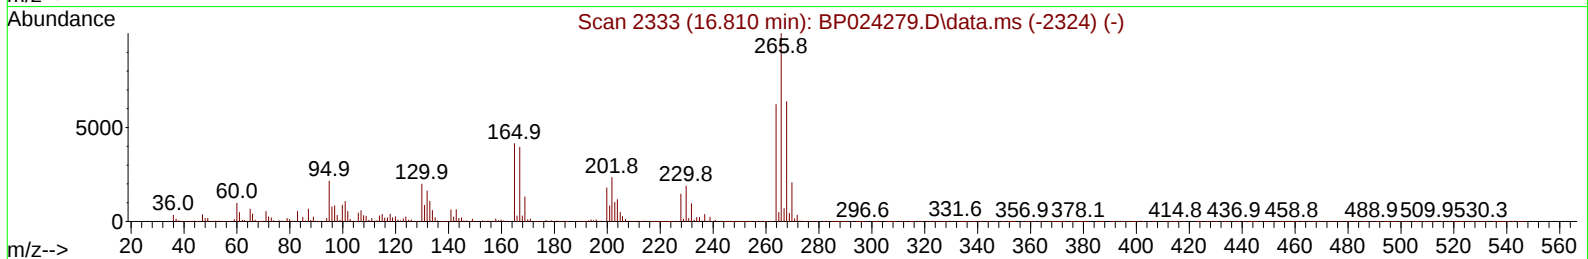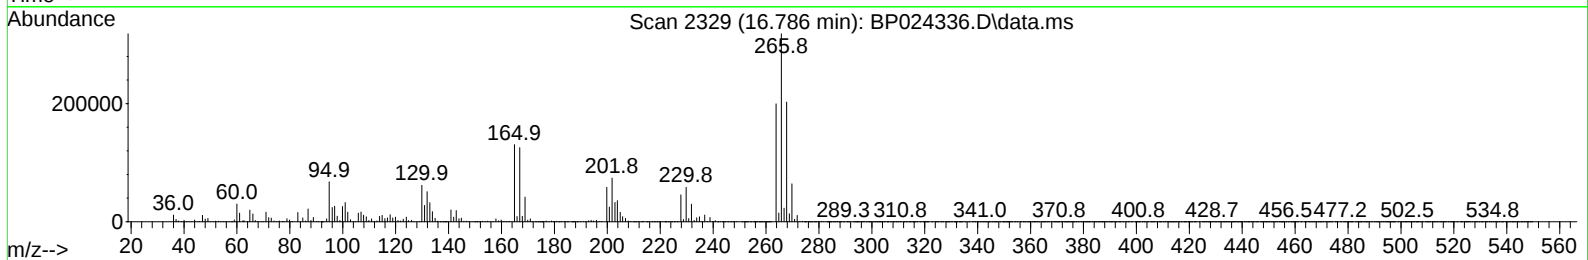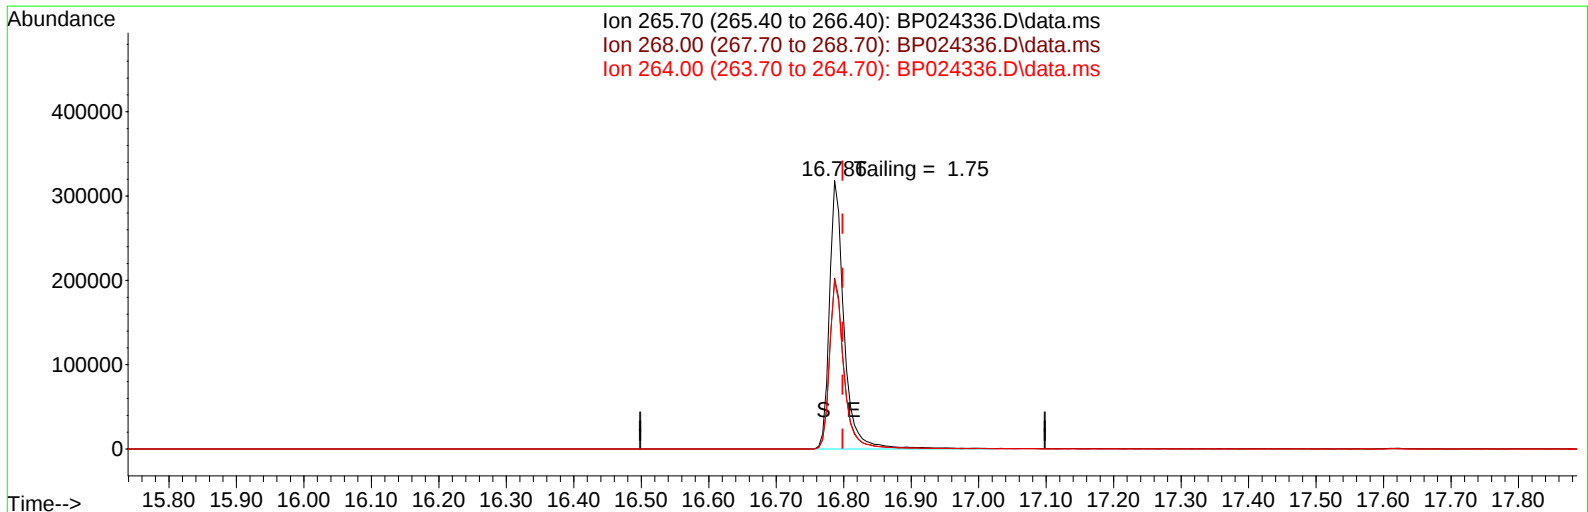

TIC: BP024336.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.012) 2010562.17 ng




response **473939**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.69
264.00	62.20	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041825\
Data File : BP024336.D
Acq On : 18 Apr 2025 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 18 12:10:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

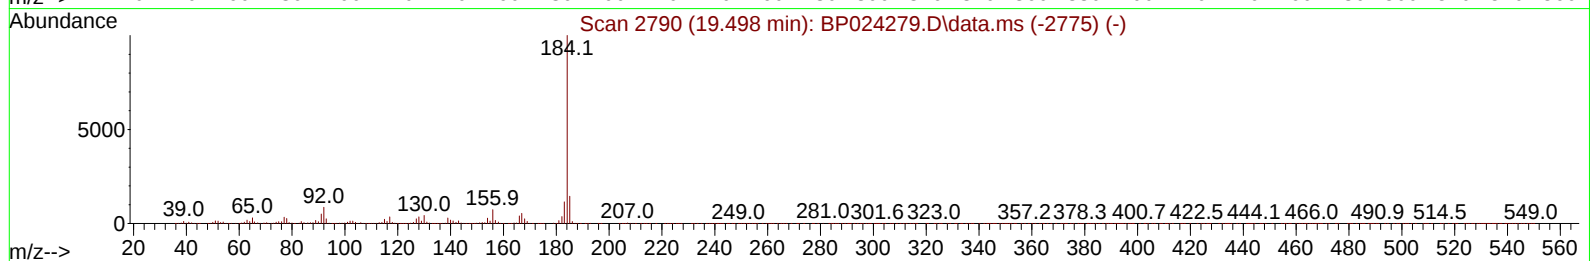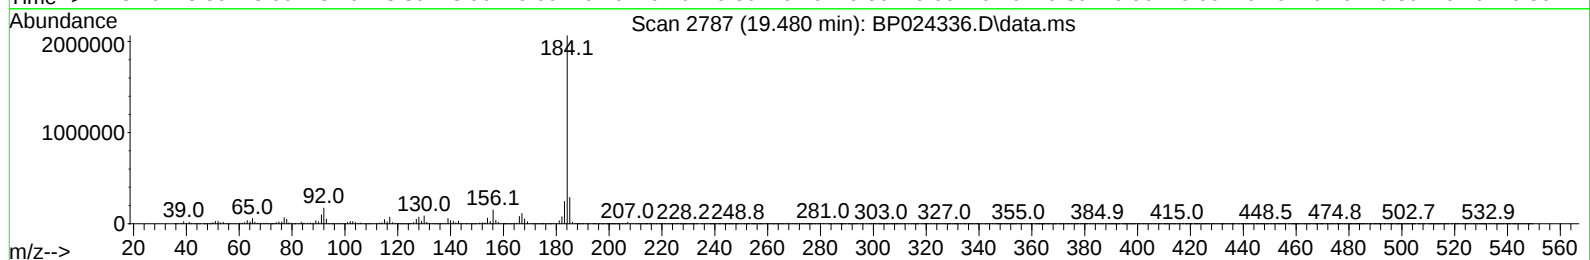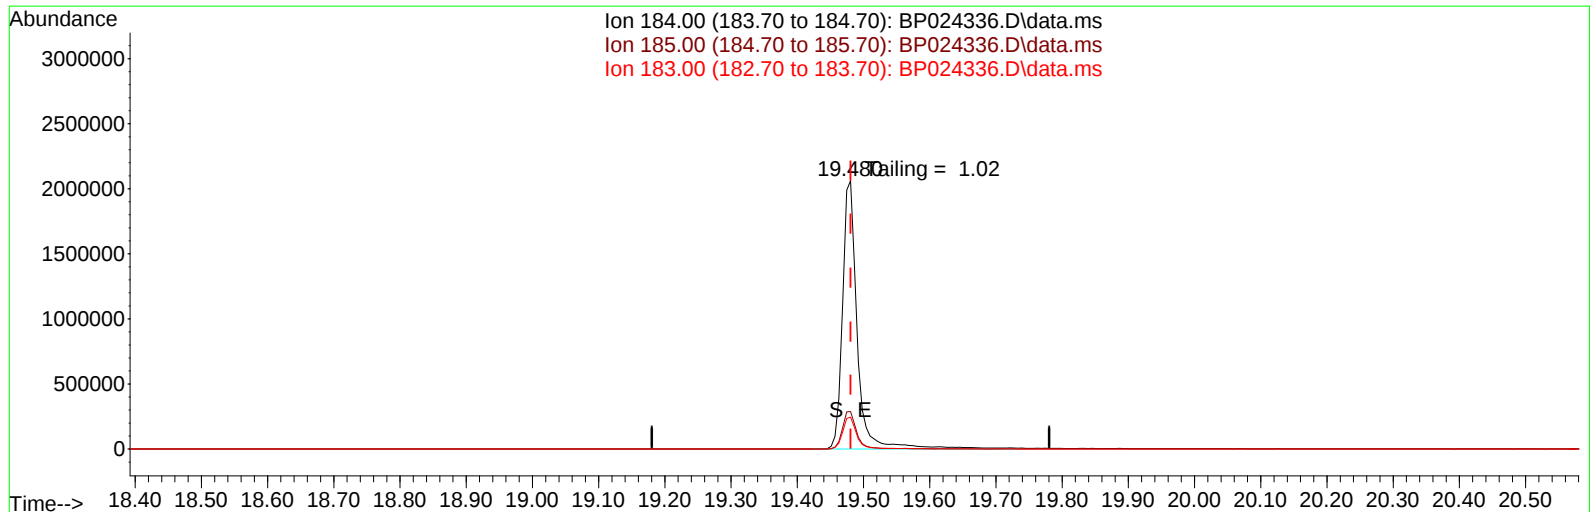

TIC: BP024336.D\data.ms

(77) Benzidine

19.480min (+ 0.000) 1458069.24 ng

response 3105020

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.99
183.00	11.50	11.86
0.00	0.00	0.00