


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042125\
Data File : BF142198.D
Acq On : 21 Apr 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 22 02:14:30 2025

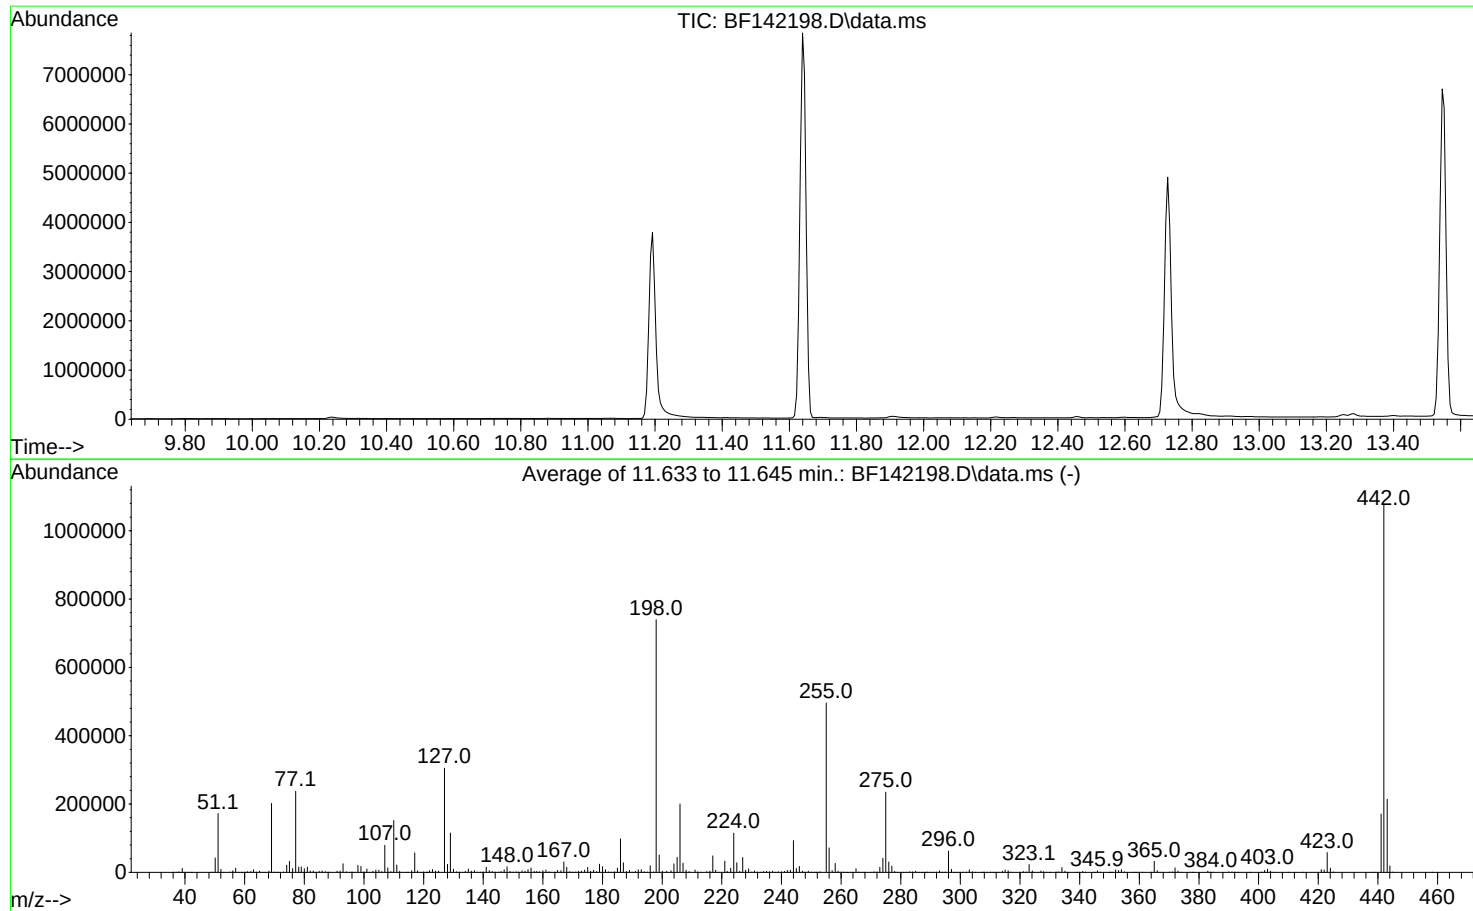




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.3	172267	PASS
68	69	0.00	2	1.8	3667	PASS
69	198	0.00	100	27.3	201908	PASS
70	69	0.00	2	0.5	956	PASS
127	198	10	80	41.2	304917	PASS
197	198	0.00	2	0.2	1446	PASS
198	198	100	100	100.0	739648	PASS
199	198	5	9	6.9	50875	PASS
275	198	10	60	31.8	234880	PASS
365	198	1	100	4.3	32168	PASS
441	198	0.01	100	23.1	170768	PASS
442	442	50	100	100.0	1076864	PASS
443	442	15	24	19.9	214315	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042125\
Data File : BF142198.D
Acq On : 21 Apr 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 22 02:45:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 22 02:14:30 2025
Response via : Initial Calibration

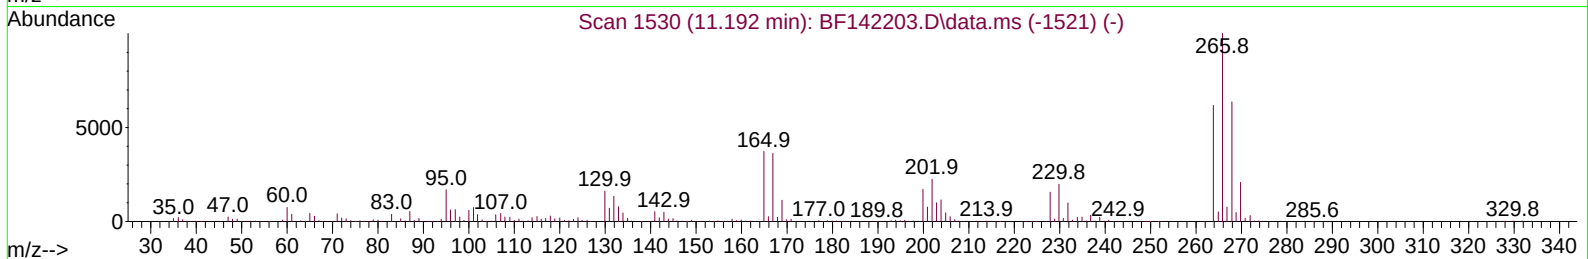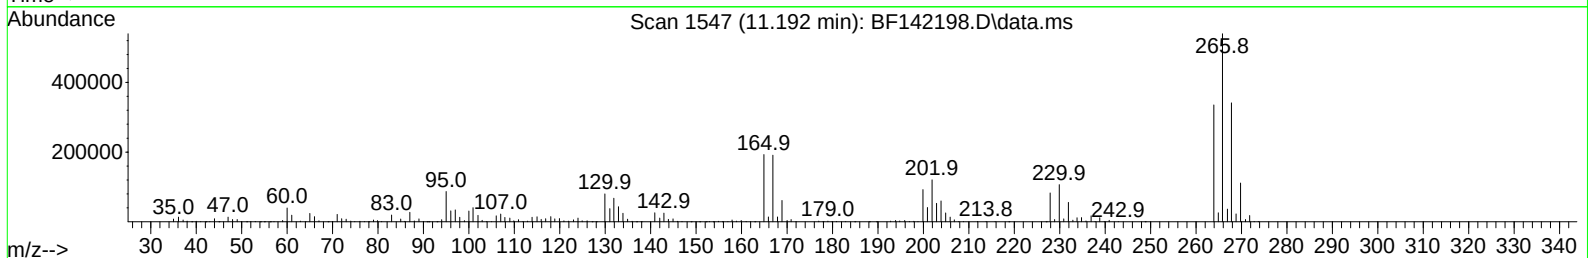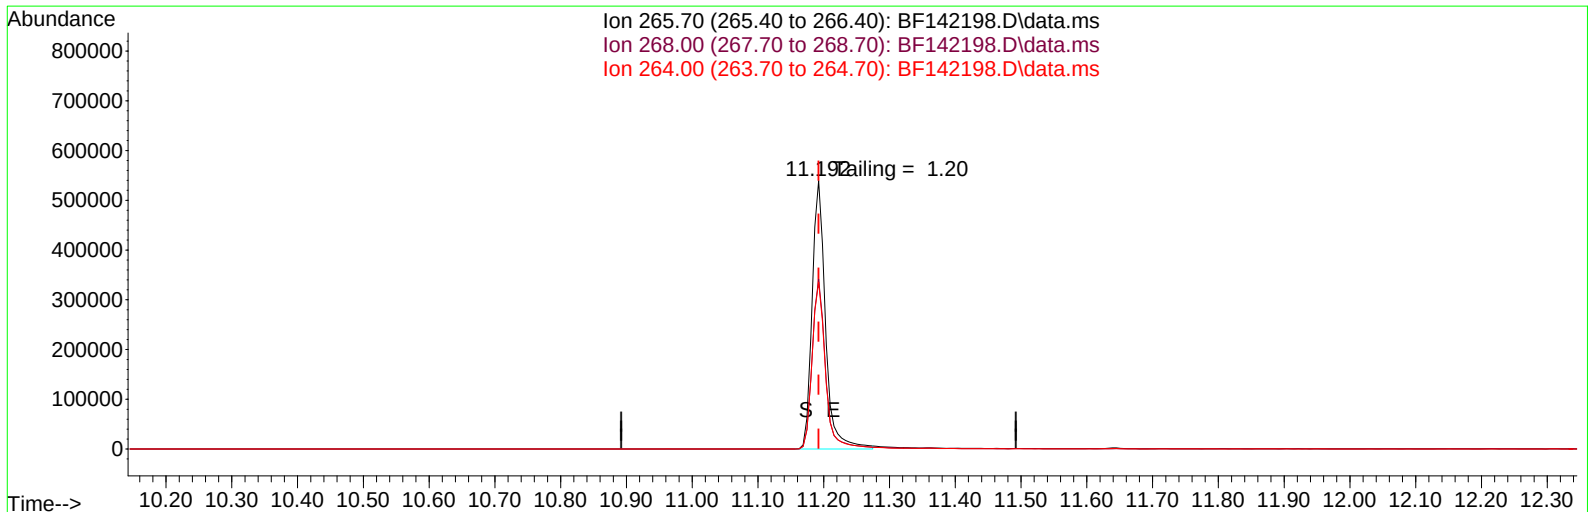

TIC: BF142198.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.000) 204849.53 ng




response 780132

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.26
264.00	61.80	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042125\
Data File : BF142198.D
Acq On : 21 Apr 2025 10:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 22 02:45:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 22 02:14:30 2025
Response via : Initial Calibration

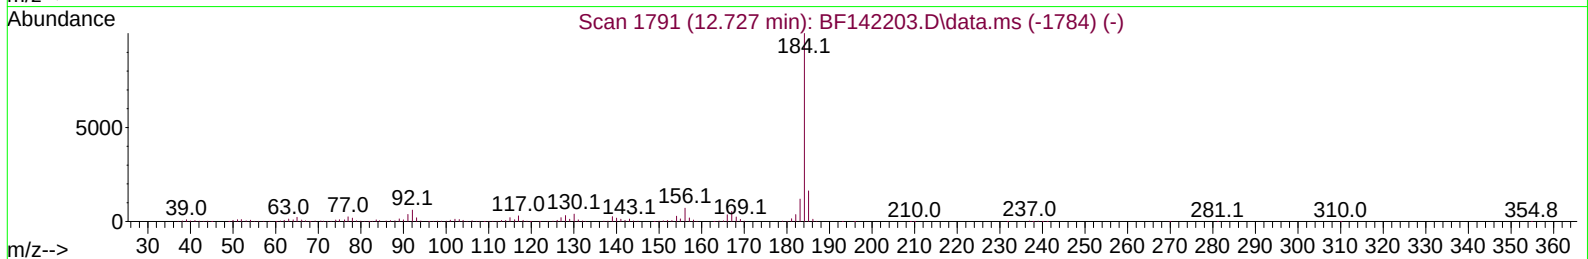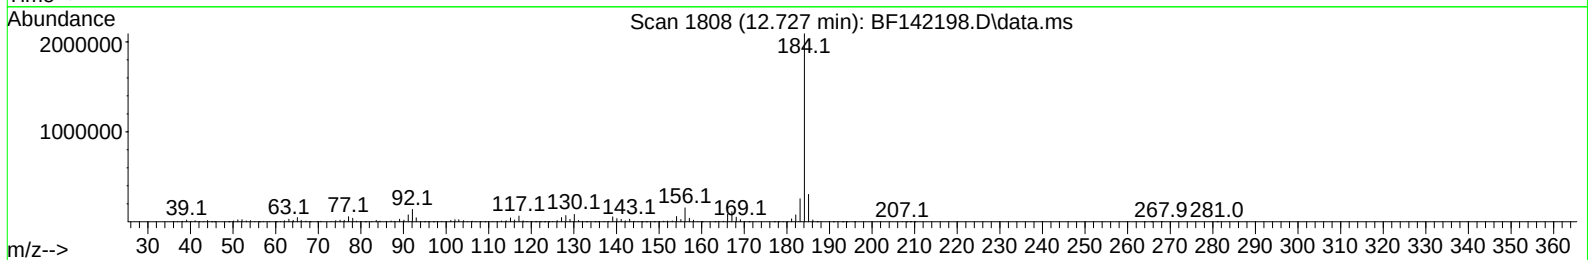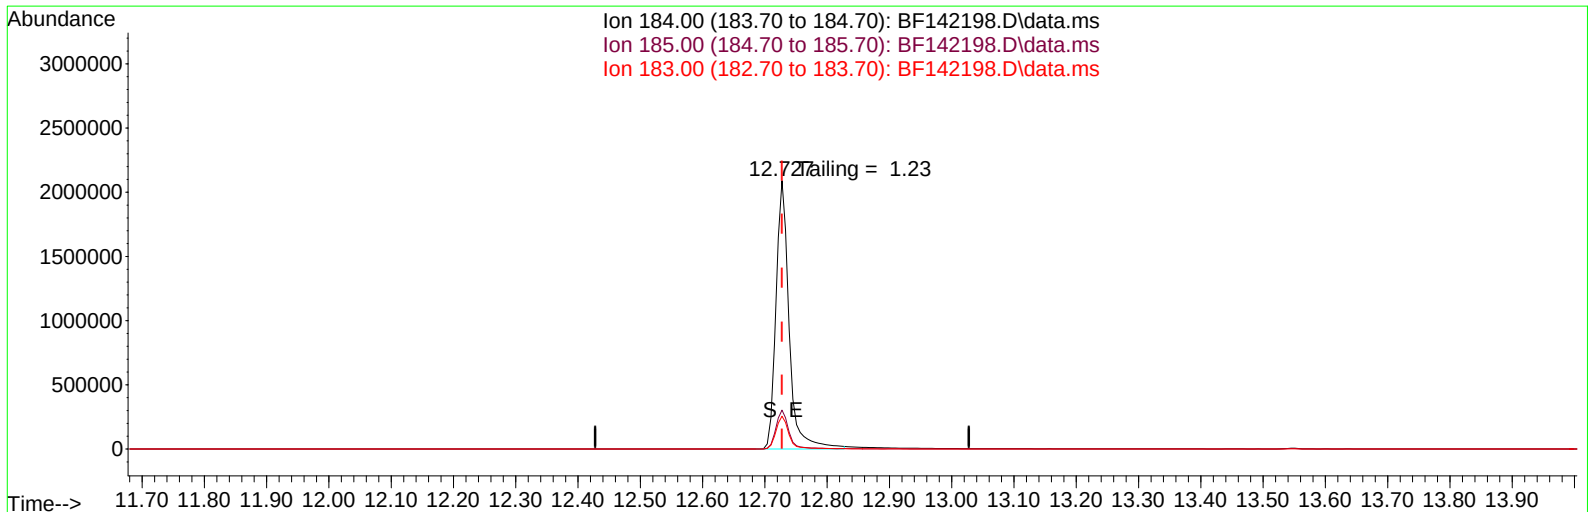

TIC: BF142198.D\data.ms

(77) Benzidine

12.727min (-0.000) 321157.70 ng

response 3162201

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.30	14.52
183.00	12.00	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/21/2025	BNA_F	<u>BF142198.D</u>
Compound Name	Response	Retention Time
DDT	1679767	13.545
DDD	27375	13.28
DDE	4146	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31521	1711288	1.84

Instrument :
BNA_F
ClientSampleId :
DFTPP