
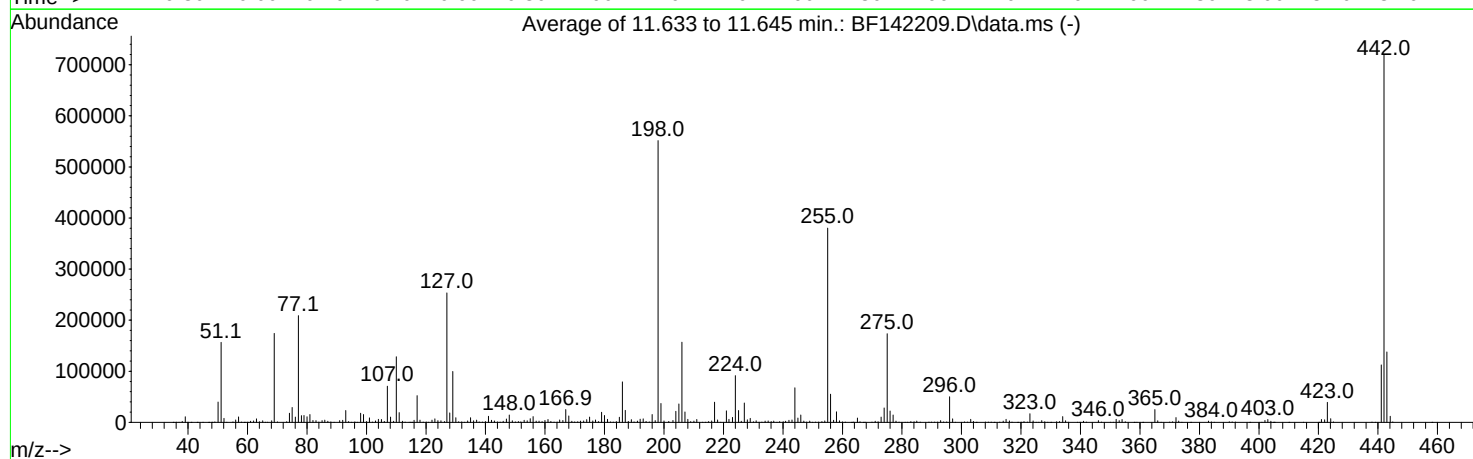


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042225\
Data File : BF142209.D
Acq On : 22 Apr 2025 08:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 22 02:14:30 2025

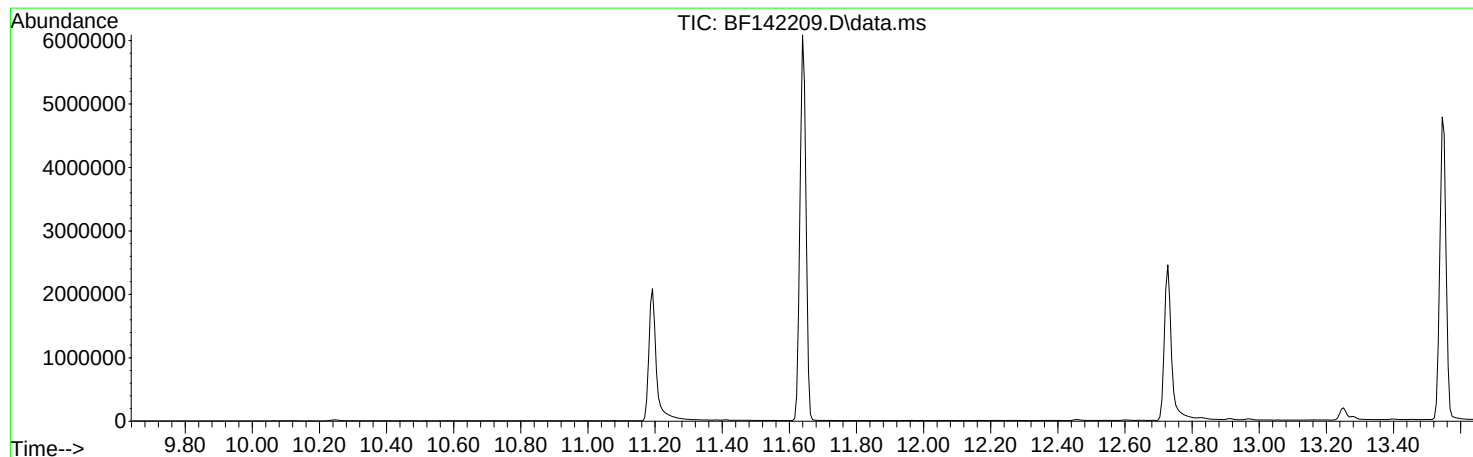

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	156565	PASS
68	69	0.00	2	1.8	3109	PASS
69	198	0.00	100	31.6	174144	PASS
70	69	0.00	2	0.6	971	PASS
127	198	10	80	45.9	253333	PASS
197	198	0.00	2	0.6	3384	PASS
198	198	100	100	100.0	551488	PASS
199	198	5	9	6.7	37045	PASS
275	198	10	60	31.5	173653	PASS
365	198	1	100	4.5	25077	PASS
441	198	0.01	100	20.4	112384	PASS
442	442	50	100	100.0	720043	PASS
443	442	15	24	19.2	137947	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/22/2025	BNA_F	<u>BF142209.D</u>
Compound Name	Response	Retention Time
DDT	1165785	13.545
DDD	61077	13.251
DDE	4133	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
65210	1230995	5.30

Instrument :
BNA_F
ClientSampleId :
DFTPP