

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042825\
 Data File : PD088292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2025 10:18
 Operator : AR\AJ
 Sample : Q1858-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 02:18:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 19 06:32:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.881	40460364	285.2E6	20.257	19.506
28)	SA Decachlor...	9.072	8.074	64536920	277.4E6	19.509m	15.012
Target Compounds							
10)	B gamma-Chl...	5.943	5.126	1724945	9779468	0.476m	0.482m
11)	B alpha-Chl...	6.027	5.190	2839501	8343756	0.787m	0.426m#
13)	MA Dieldrin	6.347	5.512	2187155	29013503	0.613m	1.456m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042825\
Data File : PD088292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2025 10:18
Operator : AR\AJ
Sample : Q1858-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 02:18:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
Quant Title : GC Extractables
QLast Update : Sat Apr 19 06:32:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

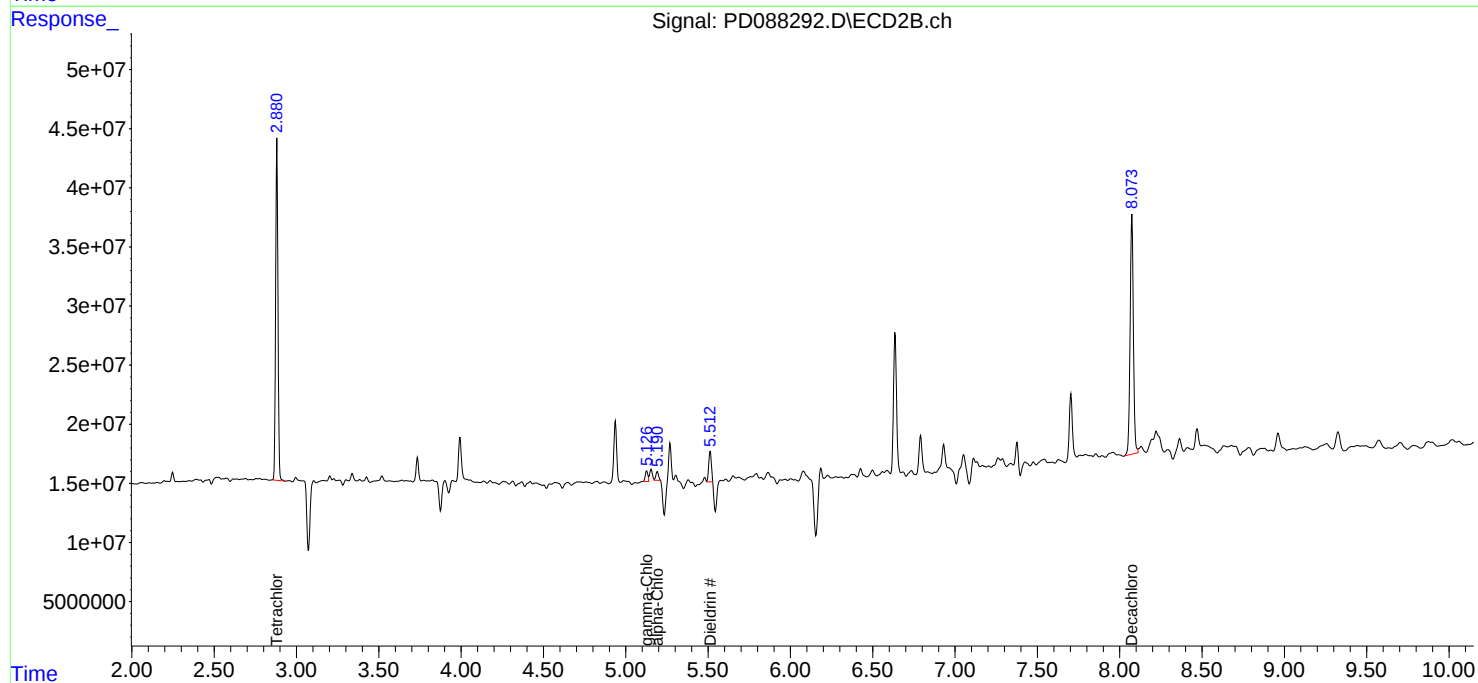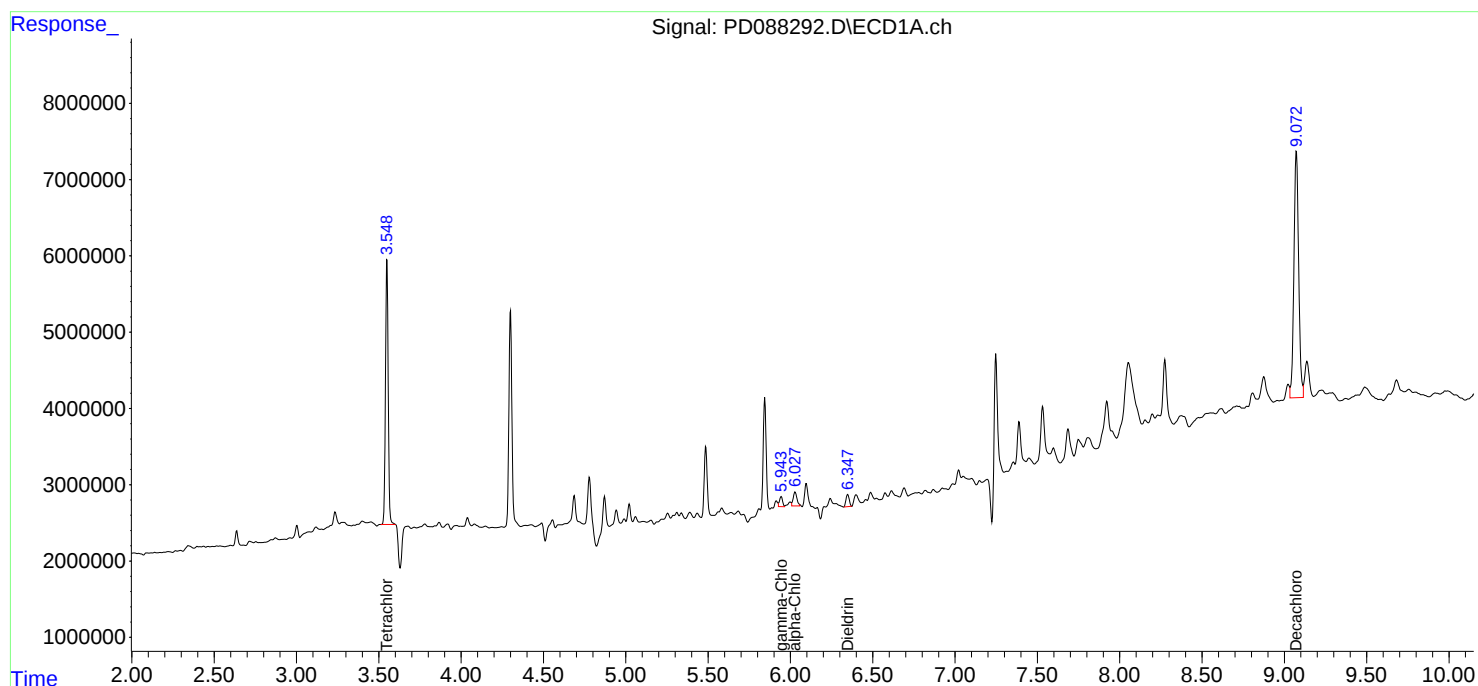


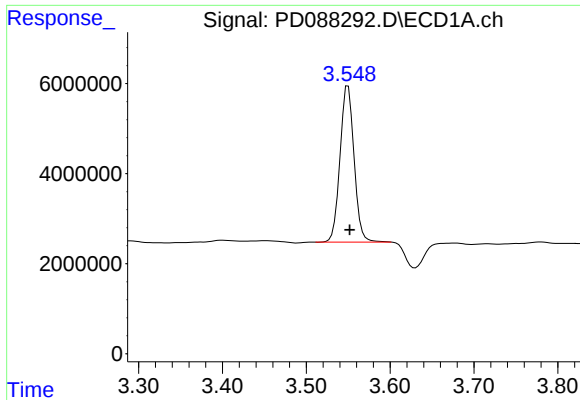

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: -0.002 min
Response: 40460364
Conc: 20.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

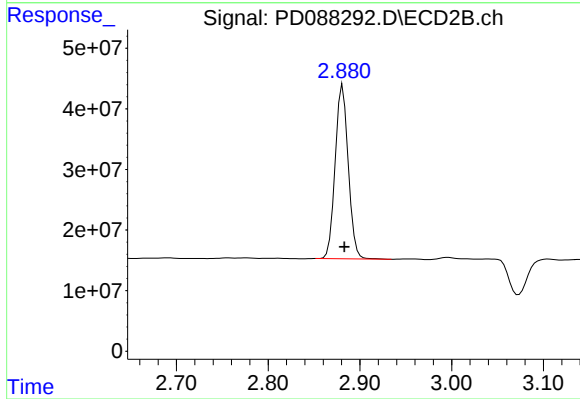


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: -0.002 min
Response: 285210909
Conc: 19.51 ng/ml

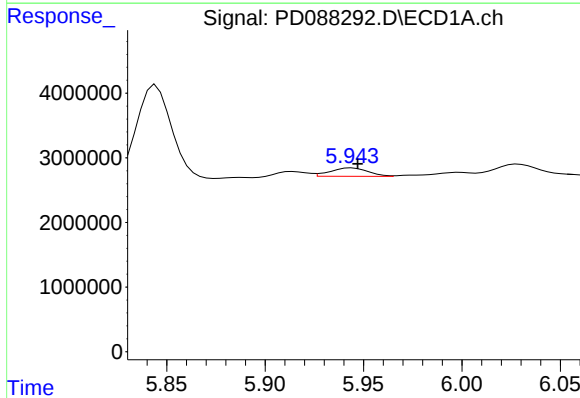


#10 gamma-Chlordane

R.T.: 5.943 min
Delta R.T.: -0.004 min
Response: 1724945
Conc: 0.48 ng/ml m

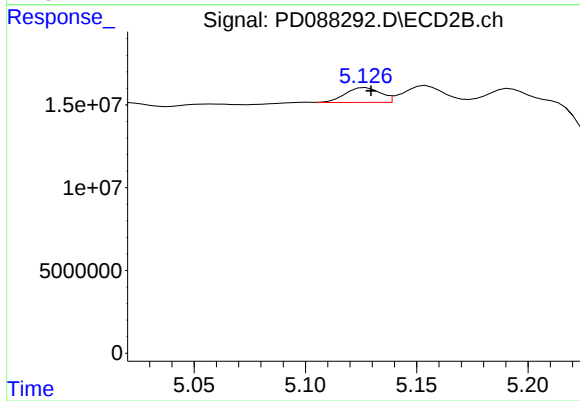

#10 gamma-Chlordane


R.T.: 5.126 min
Delta R.T.: -0.004 min
Response: 9779468
Conc: 0.48 ng/ml m

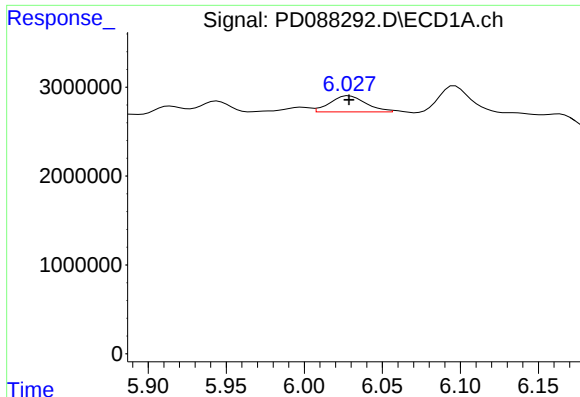

#11 alpha-Chlordane


R.T.: 6.027 min
Delta R.T.: -0.001 min
Response: 2839501
Conc: 0.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

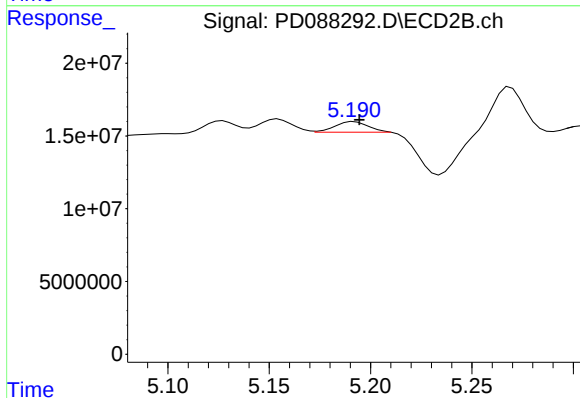


#11 alpha-Chlordane

R.T.: 5.190 min
Delta R.T.: -0.004 min
Response: 8343756
Conc: 0.43 ng/ml m

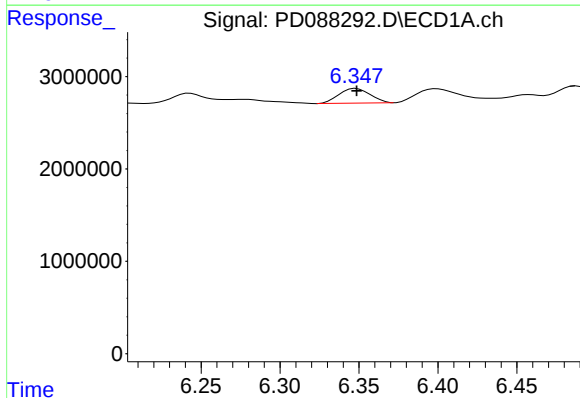


#13 Dieldrin

R.T.: 6.347 min
Delta R.T.: -0.002 min
Response: 2187155
Conc: 0.61 ng/ml m

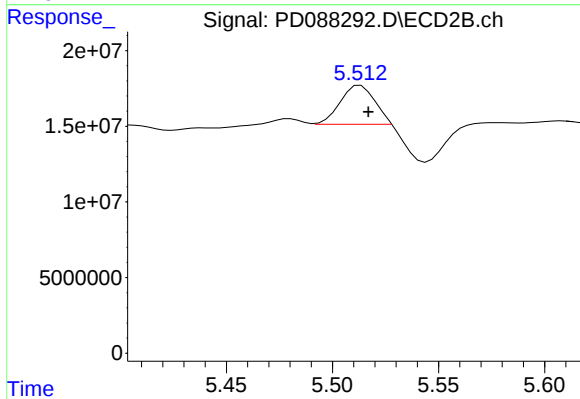

#13 Dieldrin


R.T.: 5.512 min
Delta R.T.: -0.005 min
Response: 29013503
Conc: 1.46 ng/ml m

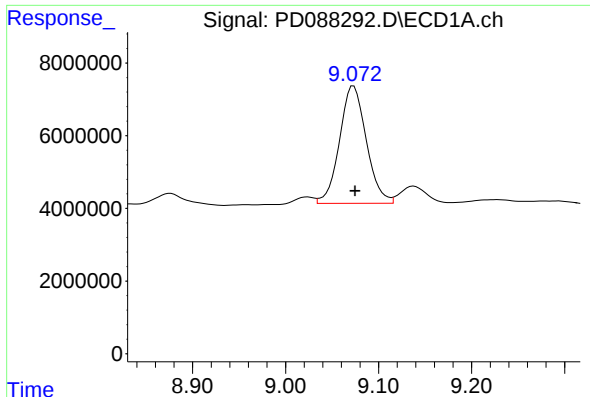

#28 Decachlorobiphenyl

R.T.: 9.072 min
Delta R.T.: -0.003 min
Response: 64536920
Conc: 19.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2

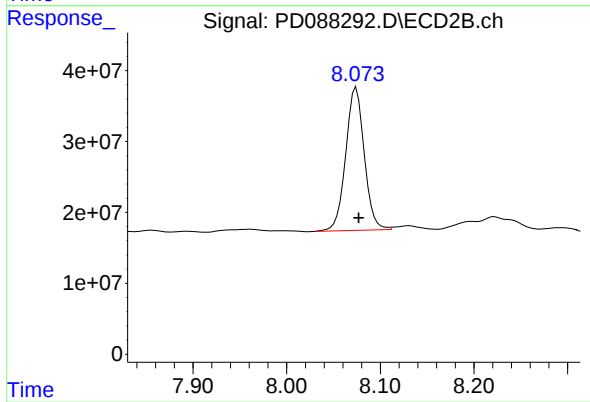

#28 Decachlorobiphenyl

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 277420247
Conc: 15.01 ng/ml