


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042325\
Data File : BM050006.D
Acq On : 23 Apr 2025 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 09 04:00:55 2025

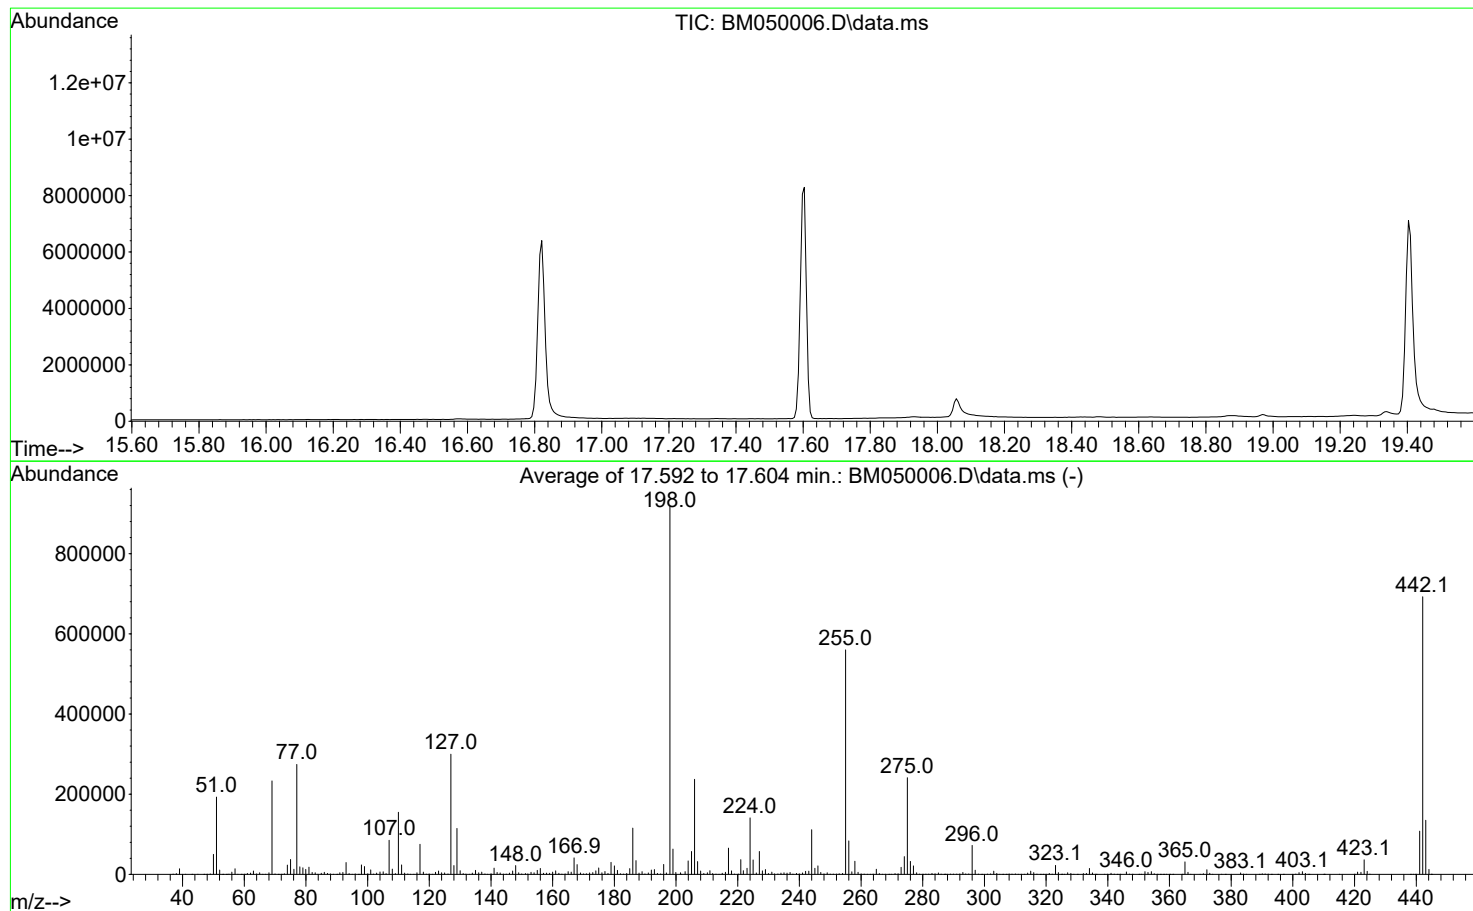

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	192612	PASS
68	69	0.00	2	1.6	3841	PASS
69	198	0.00	100	25.4	233033	PASS
70	69	0.00	2	0.6	1328	PASS
127	198	10	80	32.7	299883	PASS
197	198	0.00	2	0.4	3585	PASS
198	198	100	100	100.0	917653	PASS
199	198	5	9	6.9	63249	PASS
275	198	10	60	26.3	241259	PASS
365	198	1	100	3.4	31304	PASS
441	198	0.01	100	11.7	107717	PASS
442	442	50	100	100.0	692331	PASS
443	442	15	24	19.5	134877	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/23/2025	BNA_M	<u>BM050006.D</u>
Compound Name	Response	Retention Time
DDT	3184215	20.639
DDD	62677	20.197
DDE	4399	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
67076	3251291	2.06

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042325\
Data File : BM050006.D
Acq On : 23 Apr 2025 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 23 11:32:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

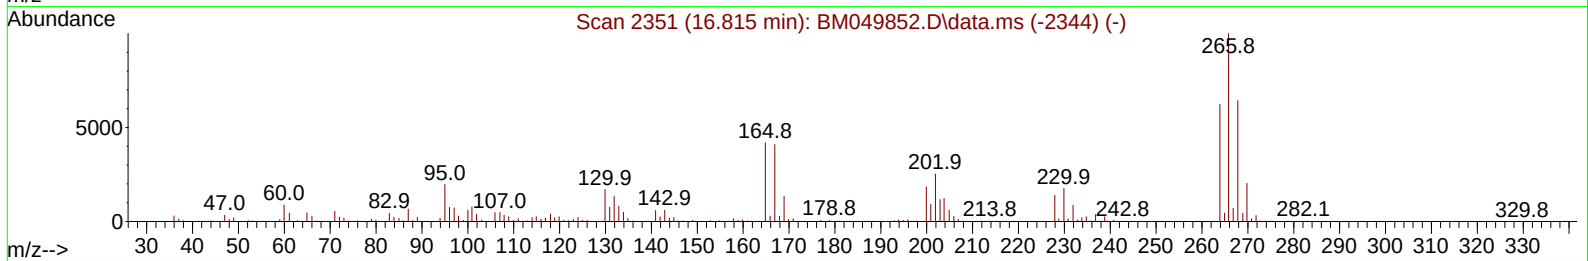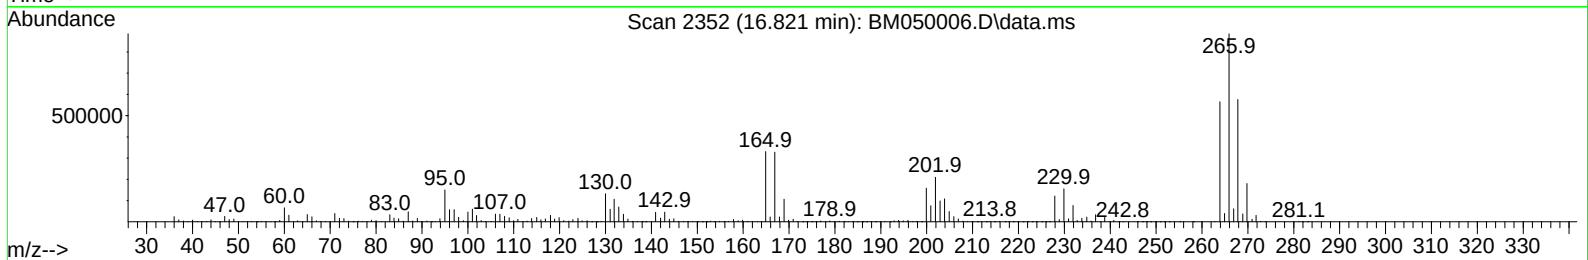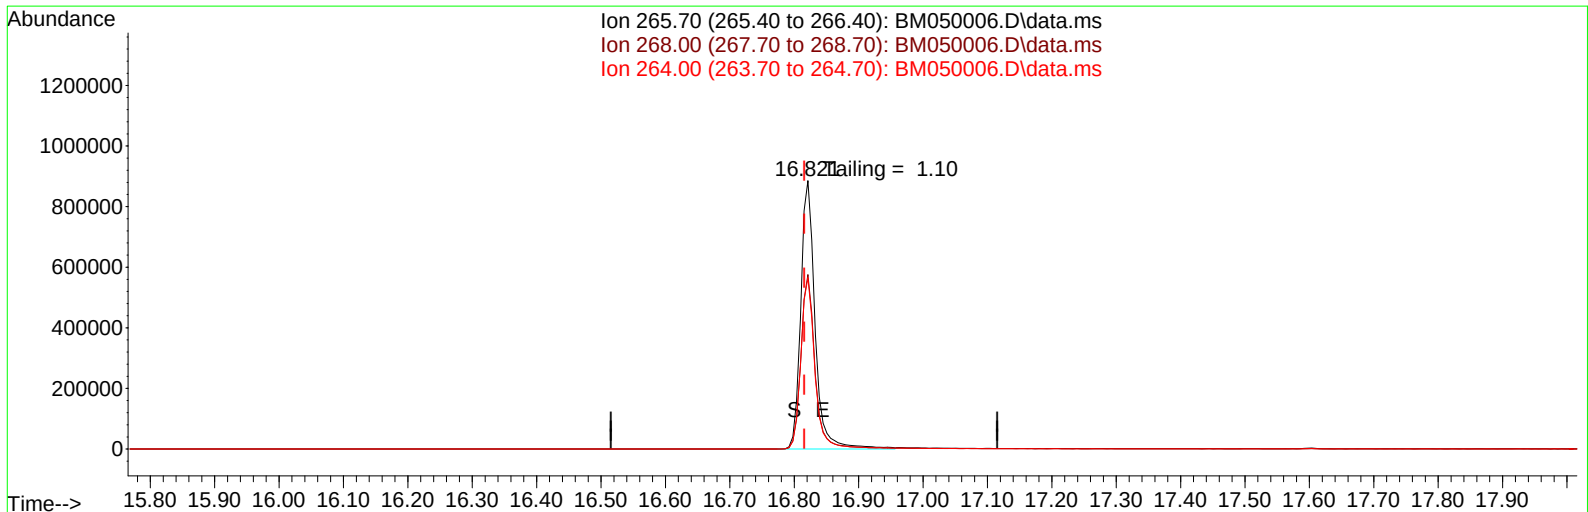

TIC: BM050006.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.006) 187980.23 ng




response 1389478

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	65.00
264.00	62.30	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042325\
Data File : BM050006.D
Acq On : 23 Apr 2025 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 23 11:32:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

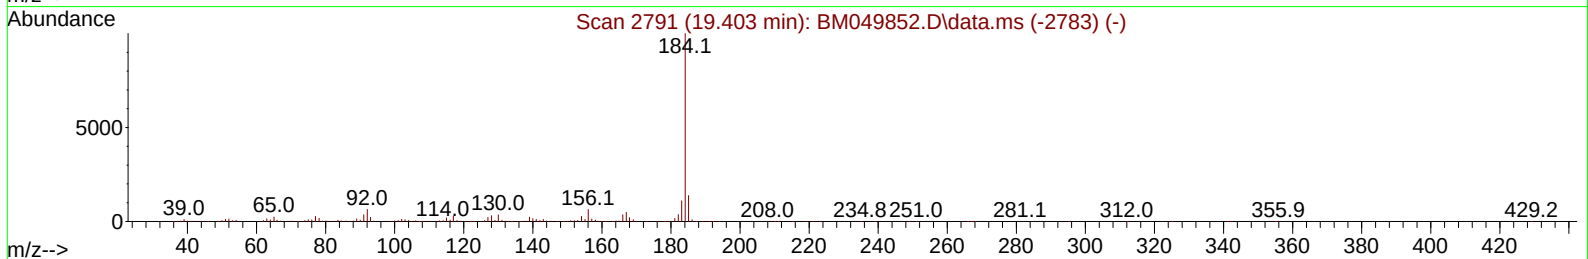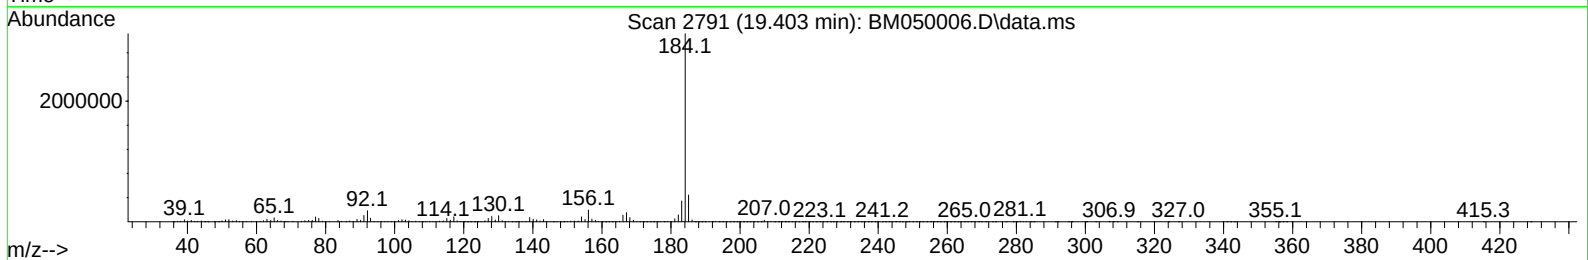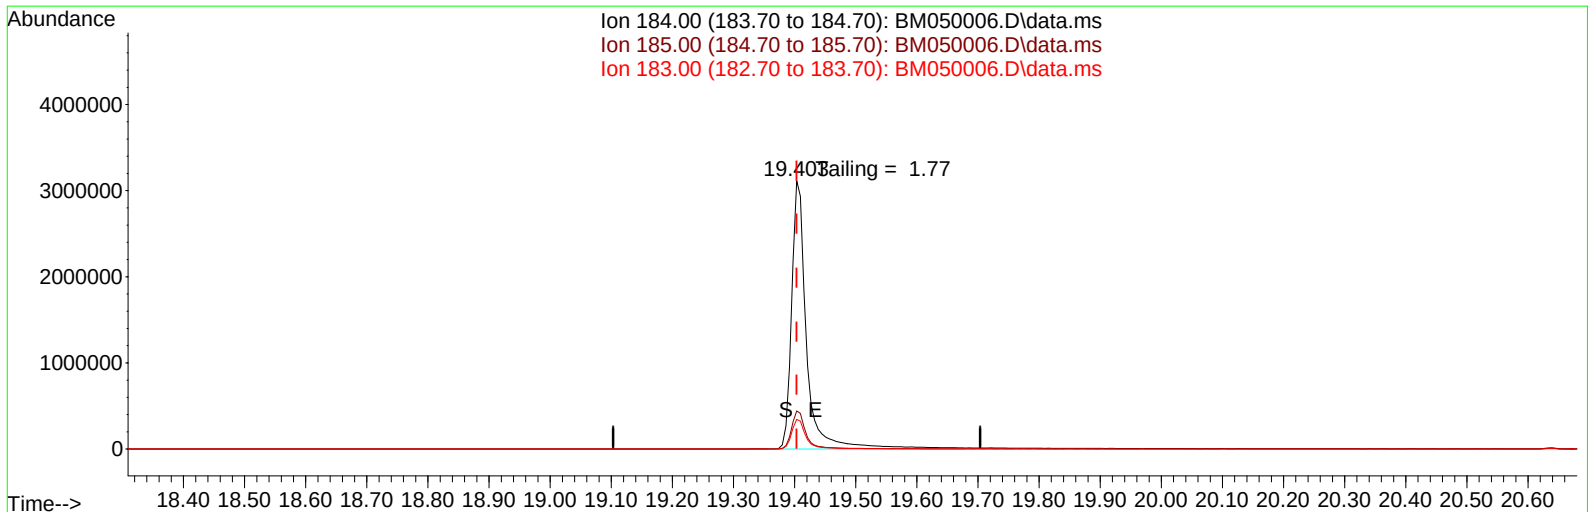

TIC: BM050006.D\data.ms

(77) Benzidine

19.403min (-0.000) 191649.01 ng

response 5336699

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.24
183.00	11.00	11.04
0.00	0.00	0.00