
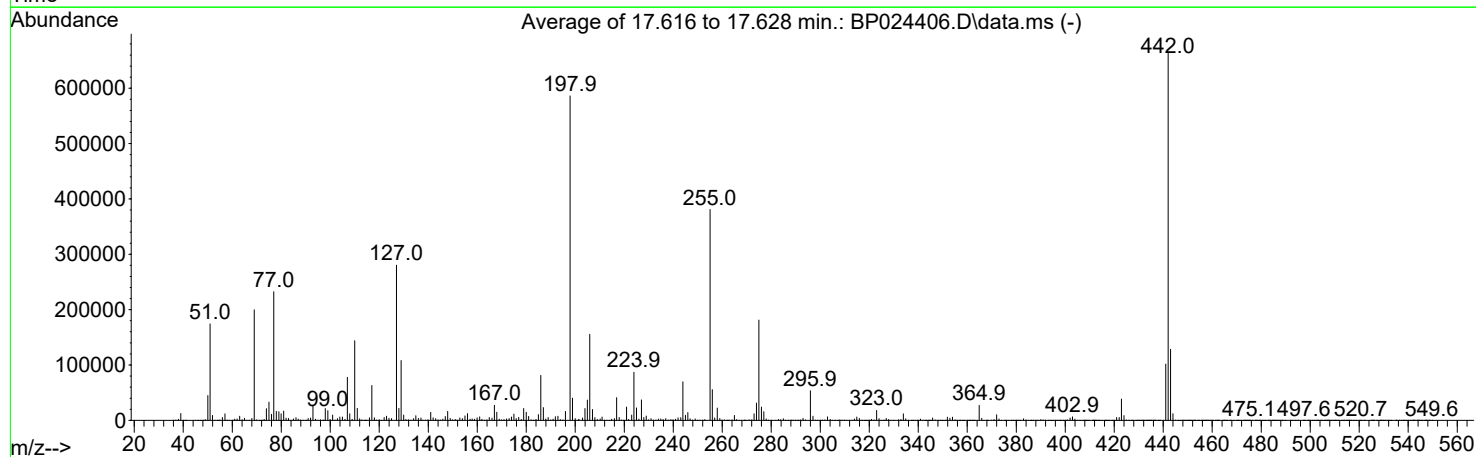


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042425\
Data File : BP024406.D
Acq On : 24 Apr 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

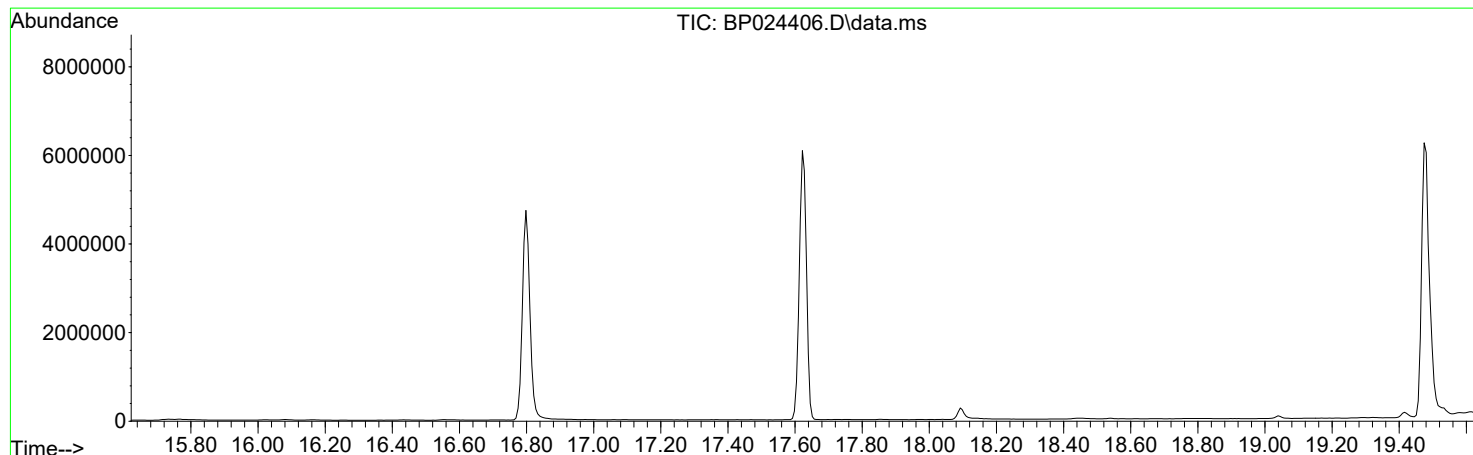

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	174345	PASS
68	69	0.00	2	1.7	3425	PASS
69	198	0.00	100	34.1	199717	PASS
70	69	0.00	2	0.5	989	PASS
127	198	10	80	47.8	280405	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	586148	PASS
199	198	5	9	6.8	40140	PASS
275	198	10	60	30.9	181200	PASS
365	198	1	100	4.7	27301	PASS
441	198	0.01	100	17.4	101899	PASS
442	442	100	100	100.0	664554	PASS
443	442	15	24	19.3	128227	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/24/2025	BNA_P	<u>BP024406.D</u>
Compound Name	Response	Retention Time
DDT	2177853	20.763
DDD	50858	20.31
DDE	2680	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53538	2231391	2.40

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042425\
Data File : BP024406.D
Acq On : 24 Apr 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 24 11:48:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

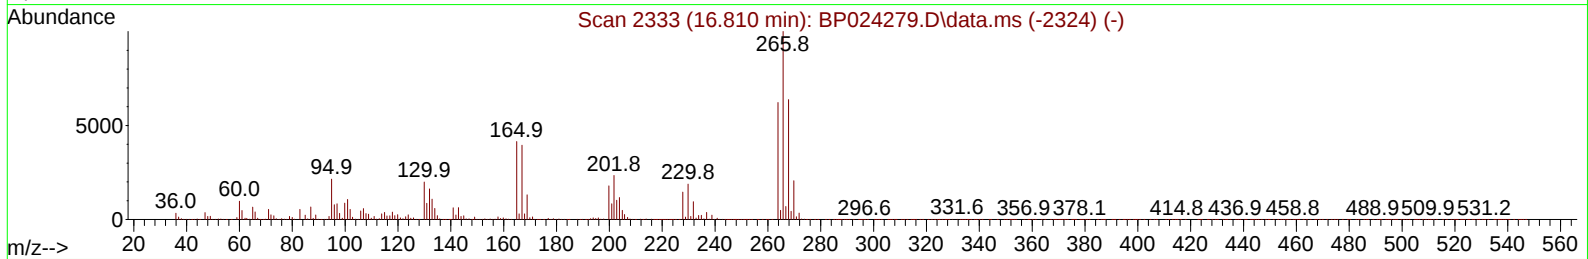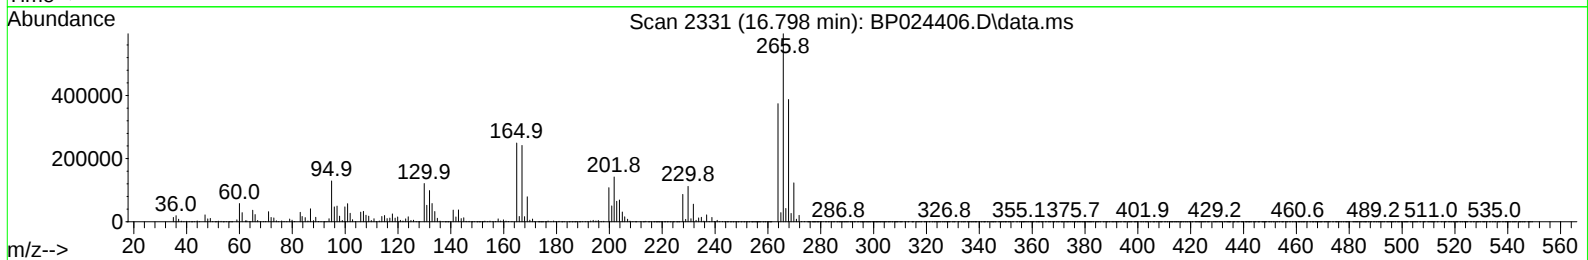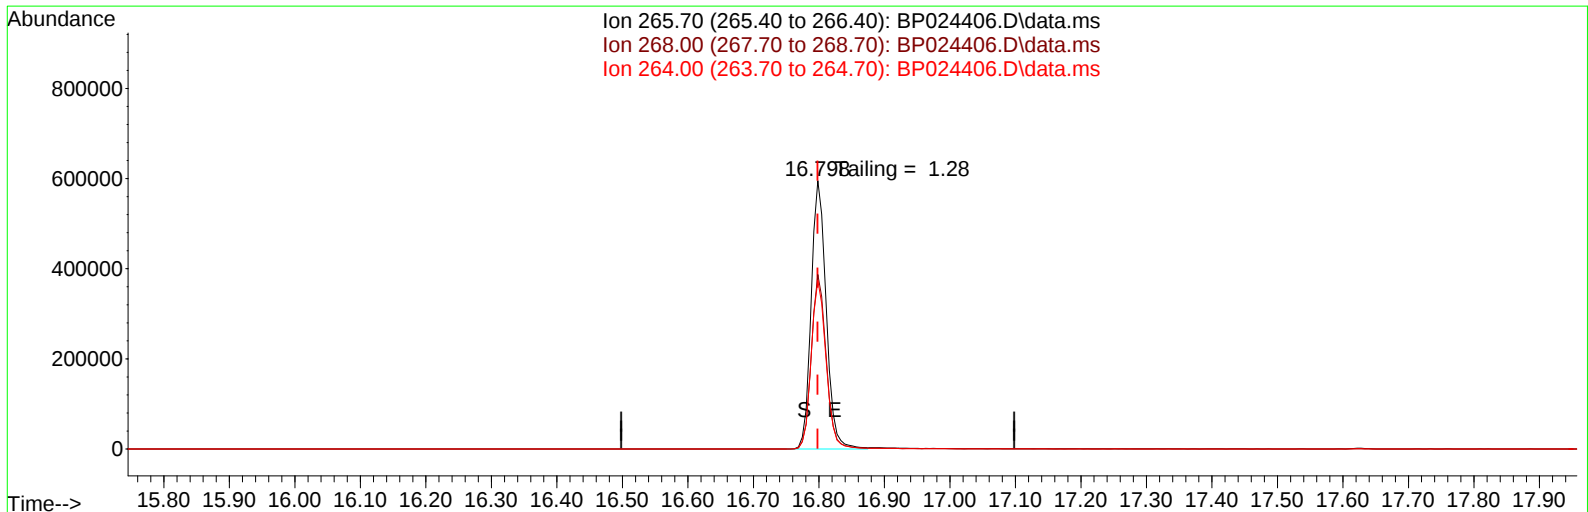

TIC: BP024406.D\data.ms

(70) Pentachlorophenol (C)

16.798min (+ 0.000) 1949769.80 ng




response 954572

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.02
264.00	62.20	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042425\
Data File : BP024406.D
Acq On : 24 Apr 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 24 11:48:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

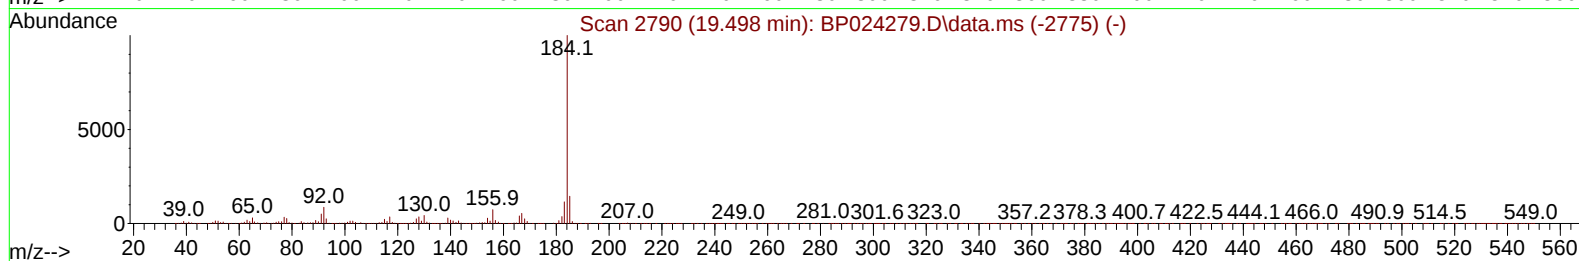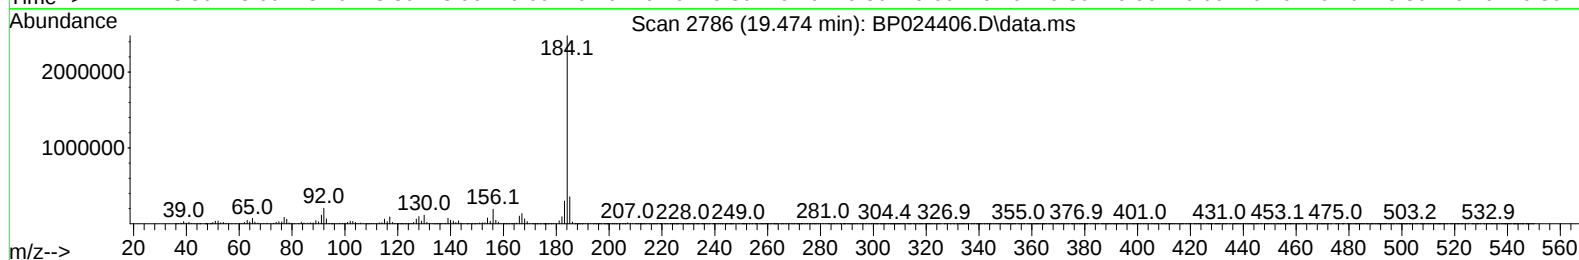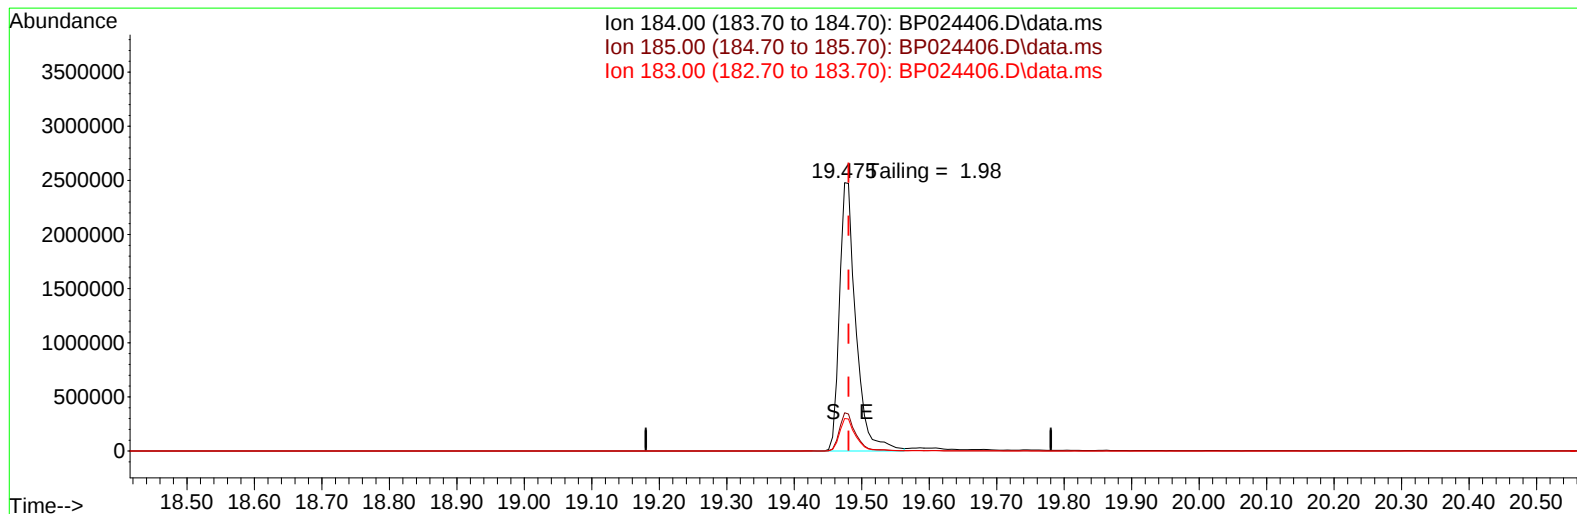

TIC: BP024406.D\data.ms

(77) Benzidine

19.474min (-0.006) 159548.41 ng

response 4190436

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.28
183.00	11.50	12.13
0.00	0.00	0.00