
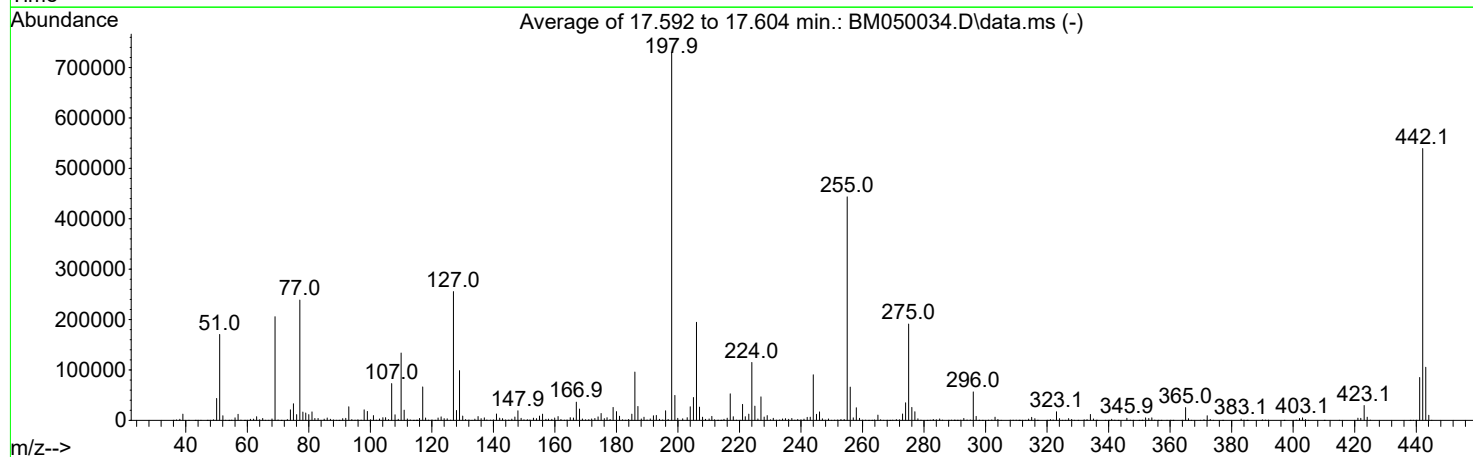


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042925\
Data File : BM050034.D
Acq On : 29 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

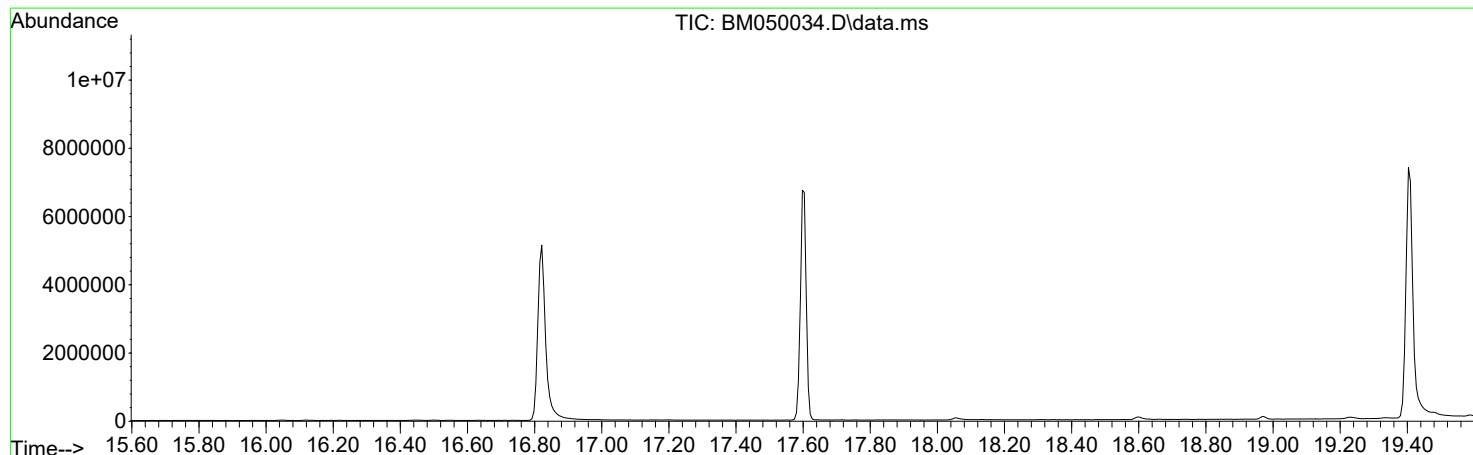

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.3	170310	PASS
68	69	0.00	2	1.4	2912	PASS
69	198	0.00	100	28.2	205819	PASS
70	69	0.00	2	0.5	1046	PASS
127	198	10	80	35.0	255467	PASS
197	198	0.00	2	0.2	1793	PASS
198	198	100	100	100.0	729771	PASS
199	198	5	9	6.8	49669	PASS
275	198	10	60	26.2	190984	PASS
365	198	1	100	3.5	25487	PASS
441	198	0.01	100	11.6	84955	PASS
442	442	50	100	100.0	539392	PASS
443	442	15	24	19.6	105480	PASS

Instrument :
BNA_M
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/29/2025	BNA_M	<u>BM050034.D</u>
Compound Name	Response	Retention Time
DDT	2527785	20.639
DDD	21730	20.251
DDE	1438	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23168	2550953	0.91

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042925\
Data File : BM050034.D
Acq On : 29 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 29 10:46:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

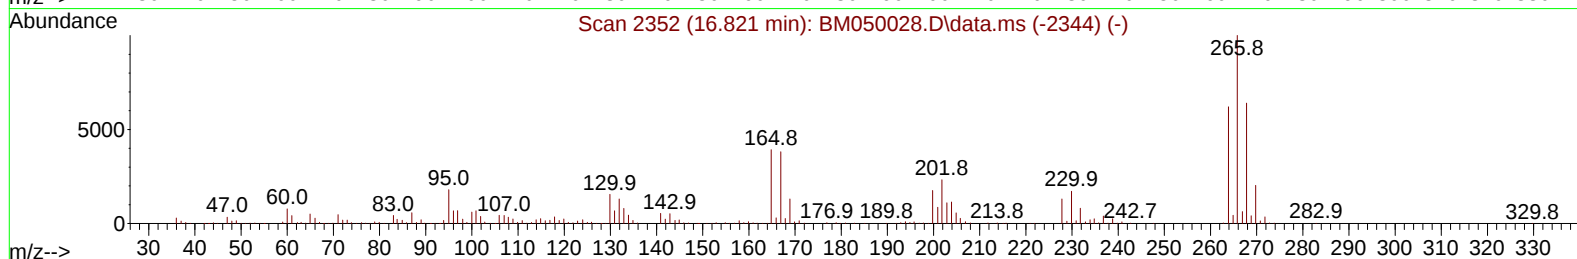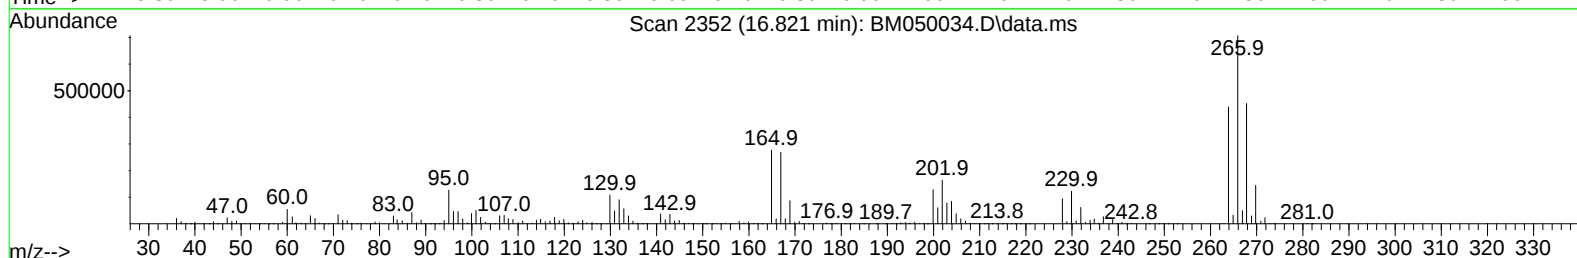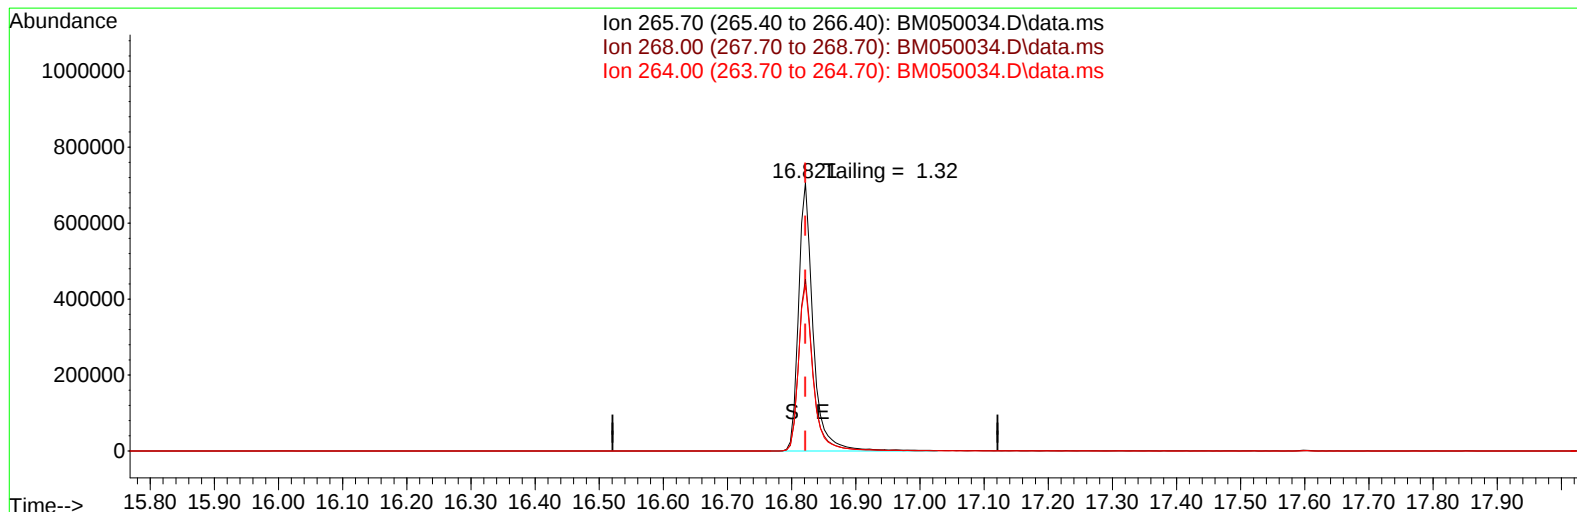

TIC: BM050034.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.000) 30619.08 ng




response 1122917

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.94
264.00	62.00	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042925\
Data File : BM050034.D
Acq On : 29 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 29 10:46:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

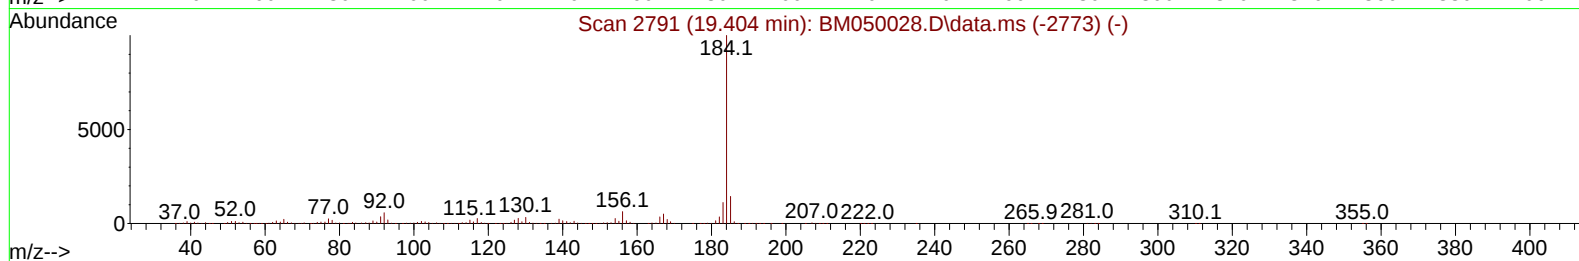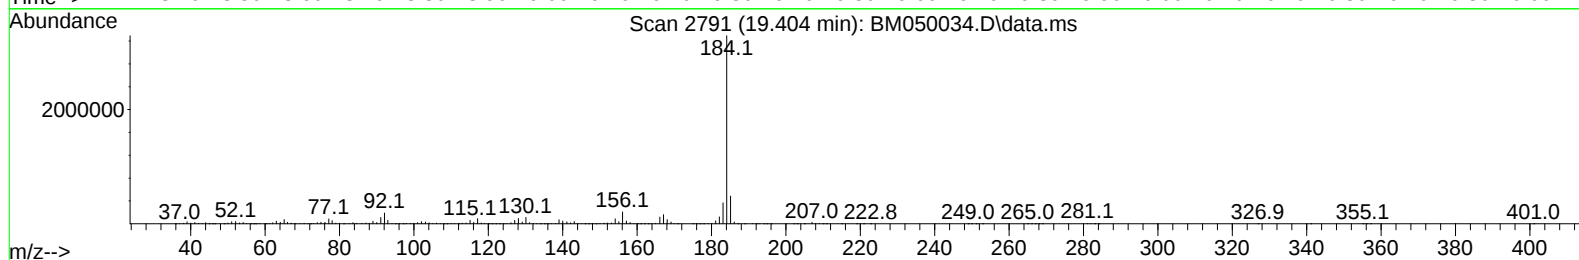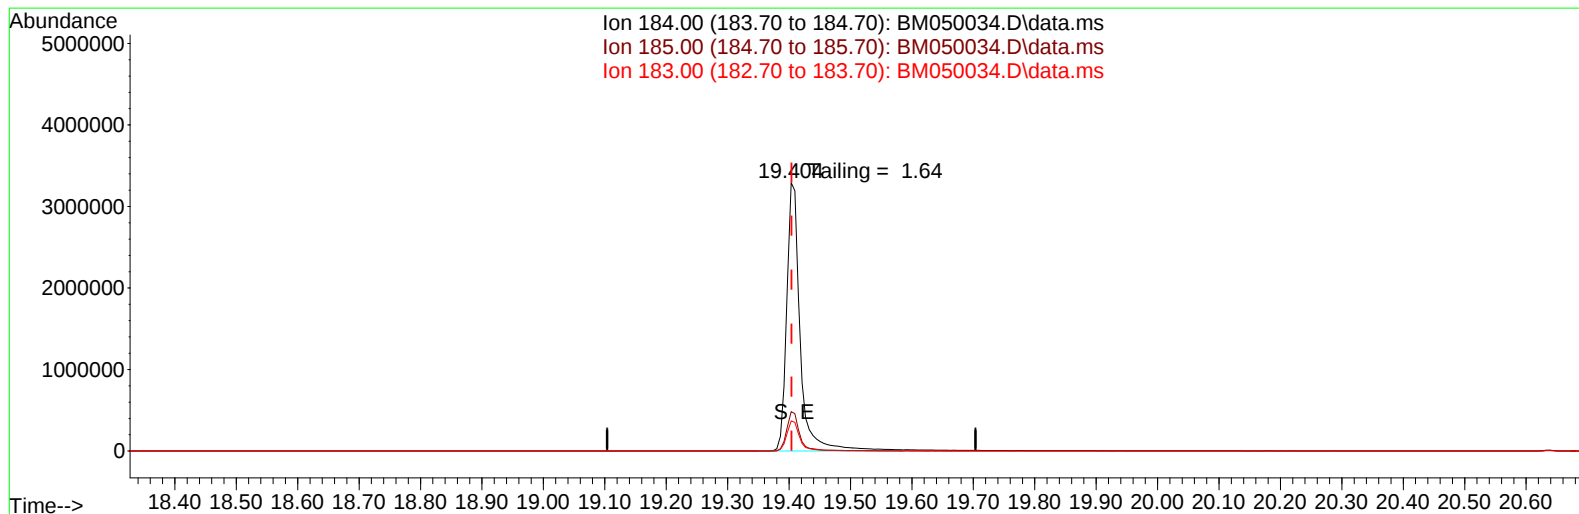

TIC: BM050034.D\data.ms

(77) Benzidine

19.404min (-0.000) 11929.52 ng

response 5130701

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.69
183.00	11.10	11.20
0.00	0.00	0.00