
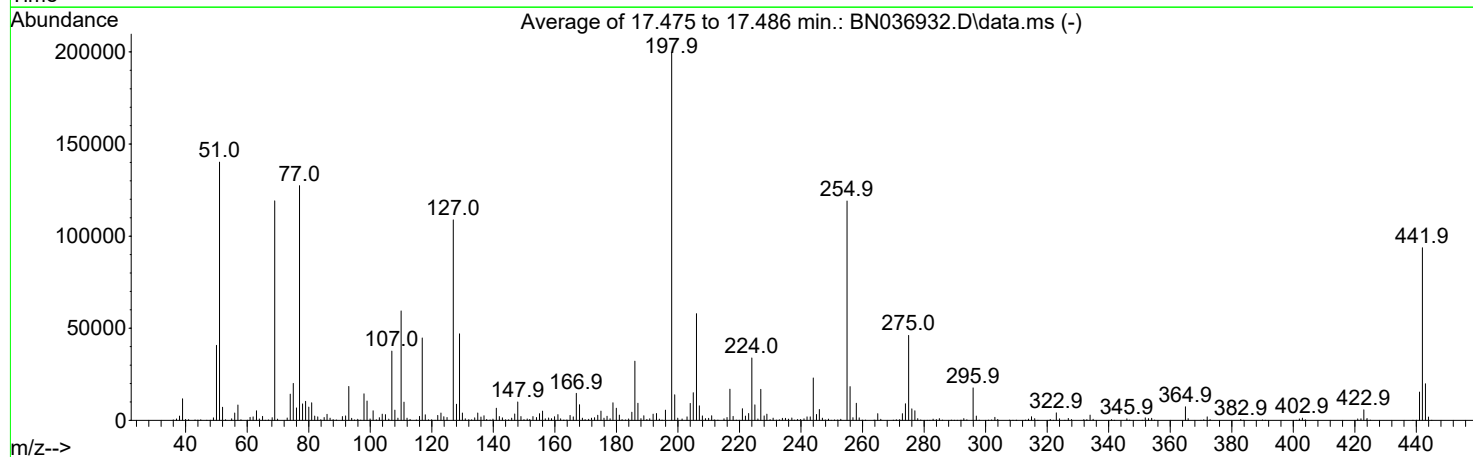


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042925\
Data File : BN036932.D
Acq On : 29 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 15:35:03 2025

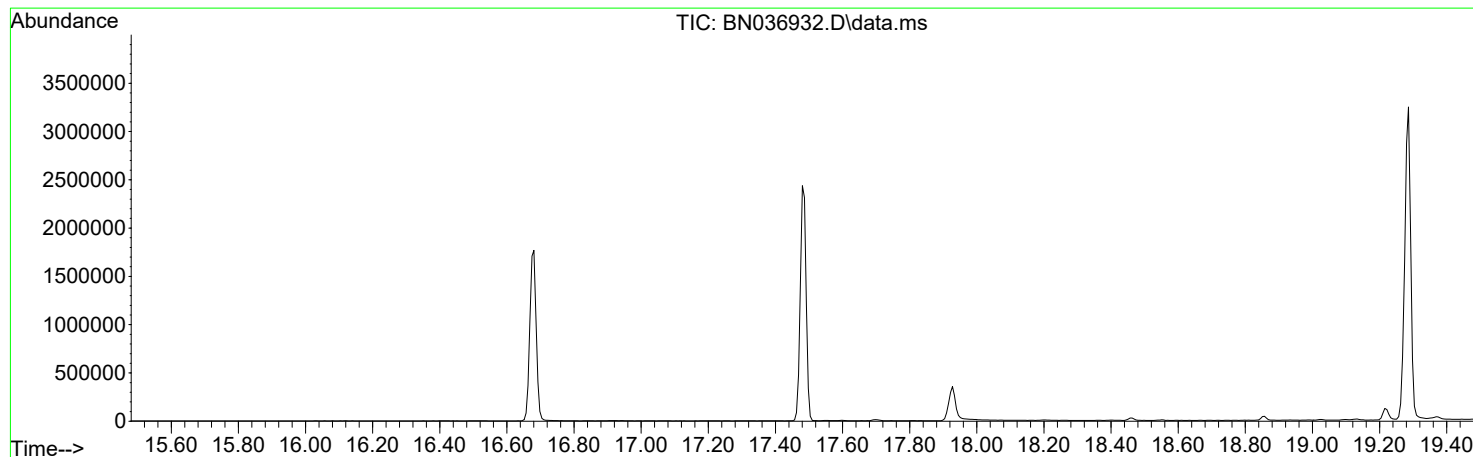

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.2	140221	PASS
68	69	0.00	2	1.3	1520	PASS
69	198	0.00	100	59.7	119197	PASS
70	69	0.00	2	0.6	660	PASS
127	198	10	80	54.5	108805	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	199680	PASS
199	198	5	9	7.0	13909	PASS
275	198	10	60	23.1	46163	PASS
365	198	1	100	3.7	7389	PASS
441	198	0.01	100	7.7	15337	PASS
442	442	50	100	100.0	93763	PASS
443	442	15	24	21.2	19866	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/29/2025	BNA_N	<u>BN036934.D</u>
Compound Name	Response	Retention Time
DDT	722011	20.521
DDD	5913	20.133
DDE	58	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5971	727982	0.82

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042925\
Data File : BN036932.D
Acq On : 29 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 29 17:24:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

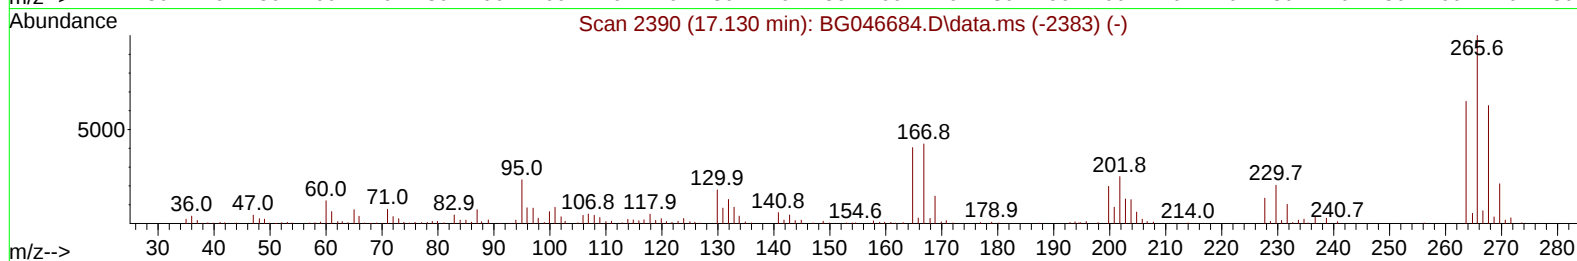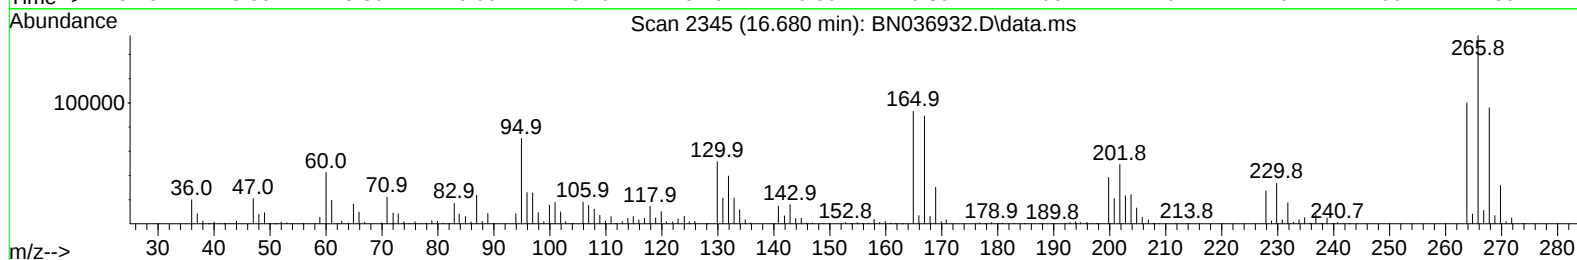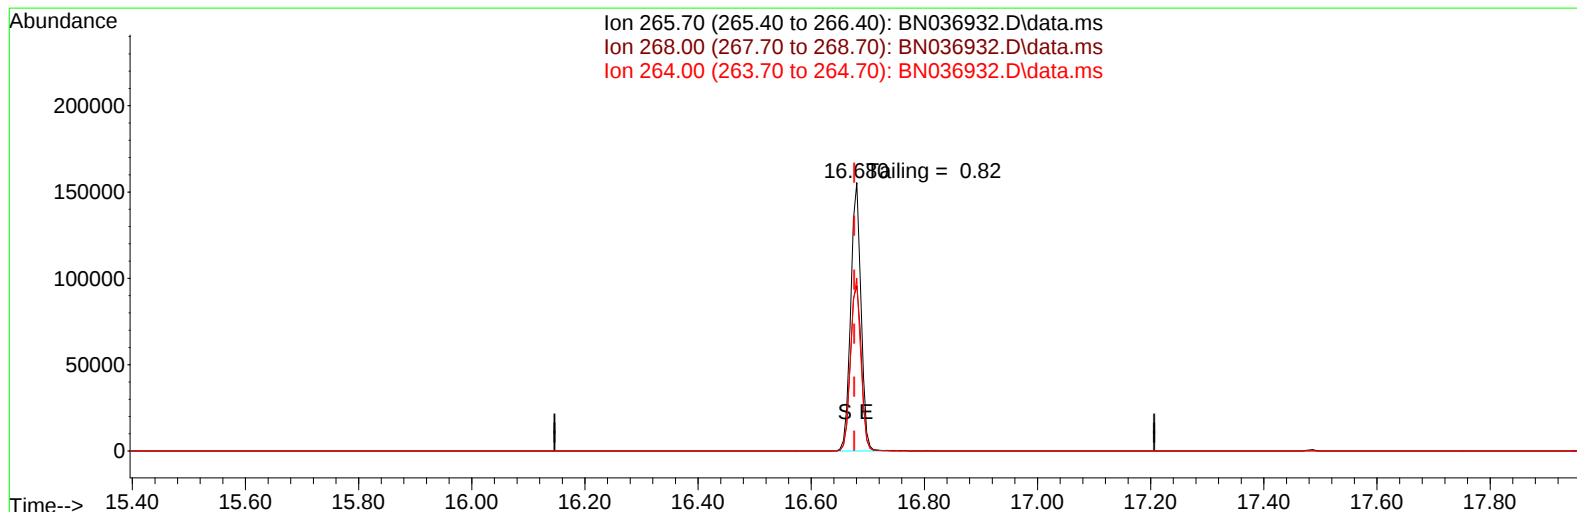

TIC: BN036932.D\data.ms

(70) Pentachlorophenol (C)

16.680min (+ 0.005) 17951.16 ng




response 196804

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.62
264.00	61.60	64.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042925\
Data File : BN036932.D
Acq On : 29 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 29 17:26:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

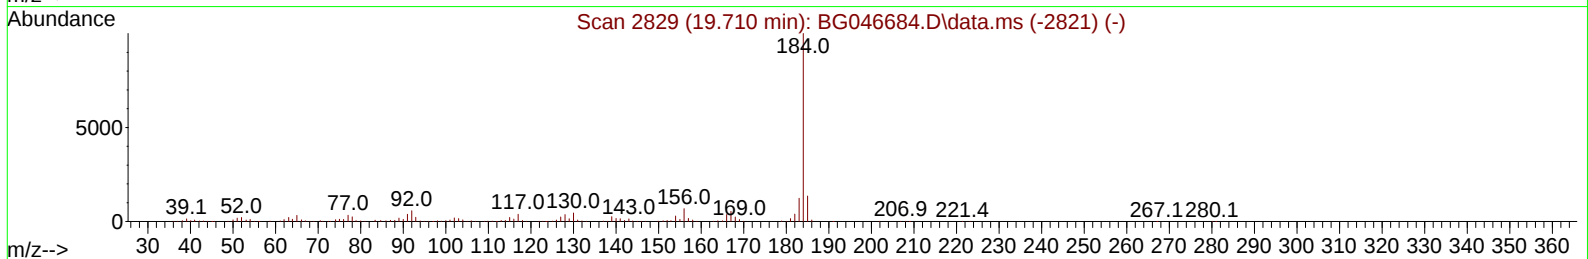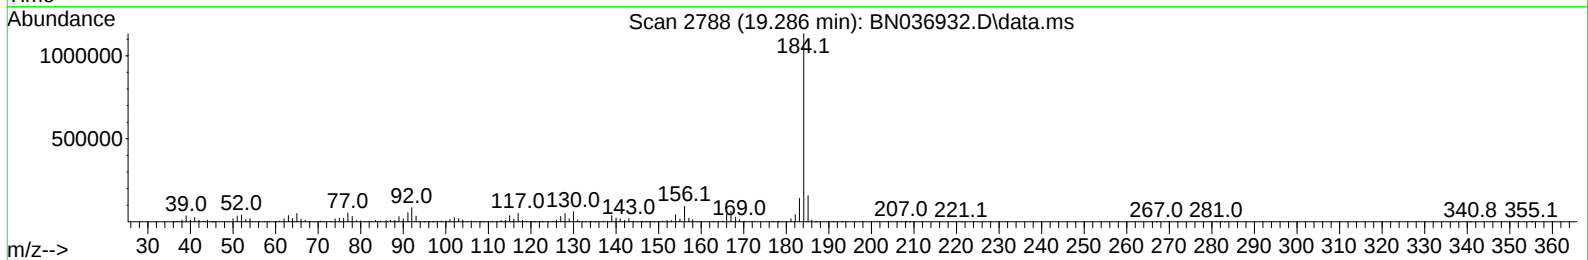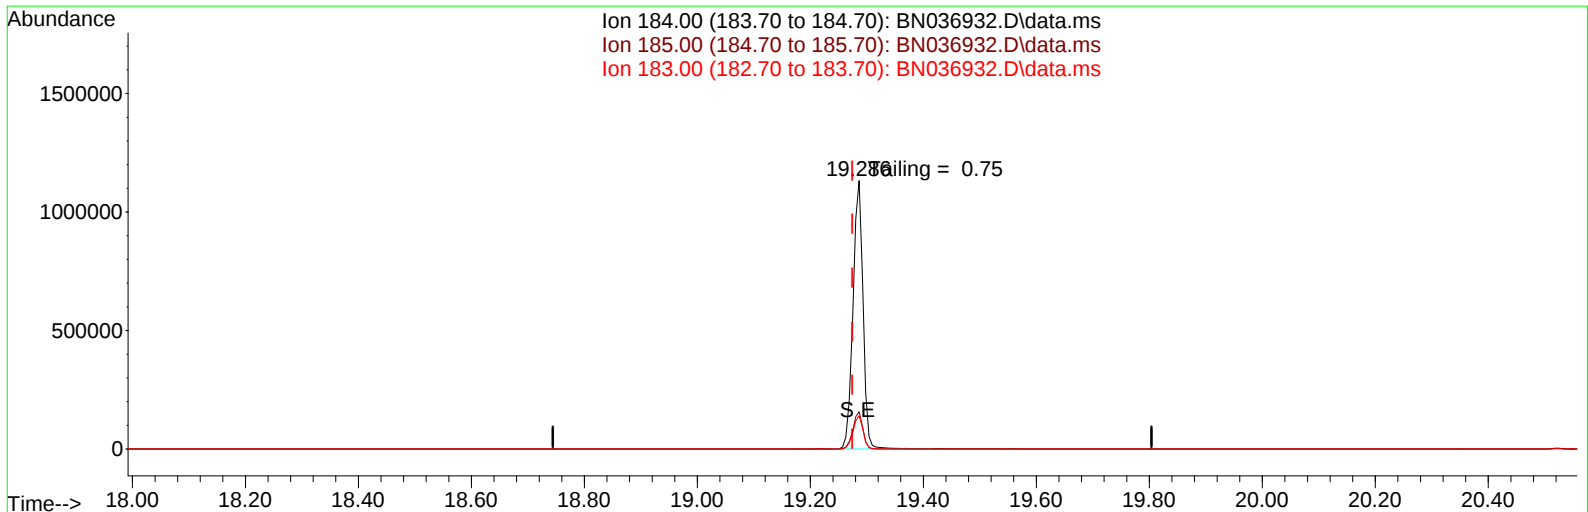

TIC: BN036932.D\data.ms

(77) Benzidine

19.286min (+ 0.012) 0.00 ng

response 1411976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	12.44
0.00	0.00	0.00