
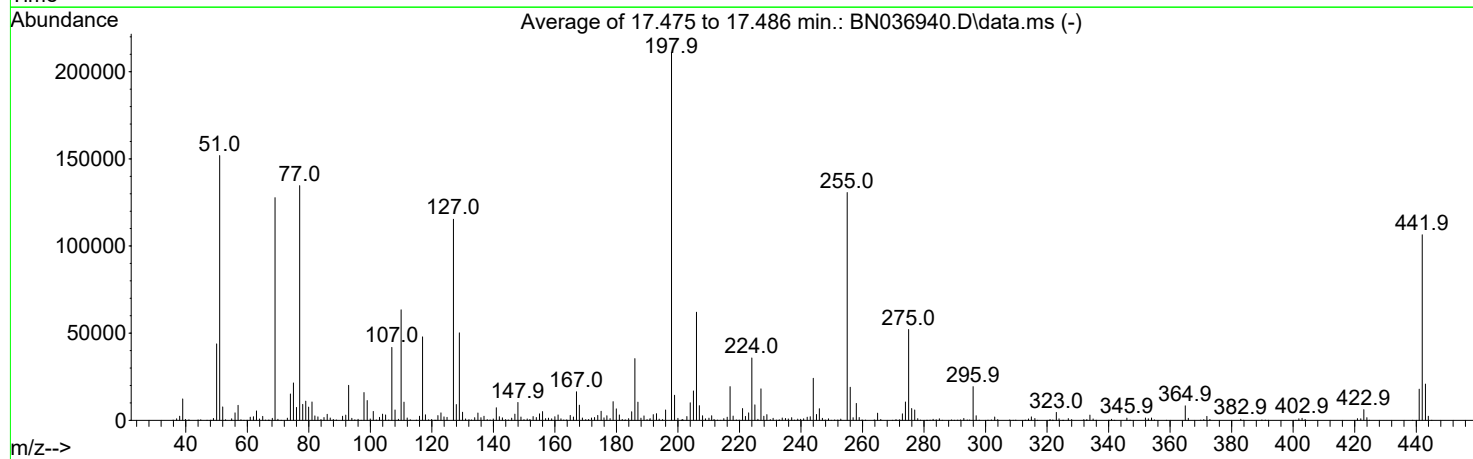


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043025\
Data File : BN036940.D
Acq On : 30 Apr 2025 10:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 15:35:03 2025

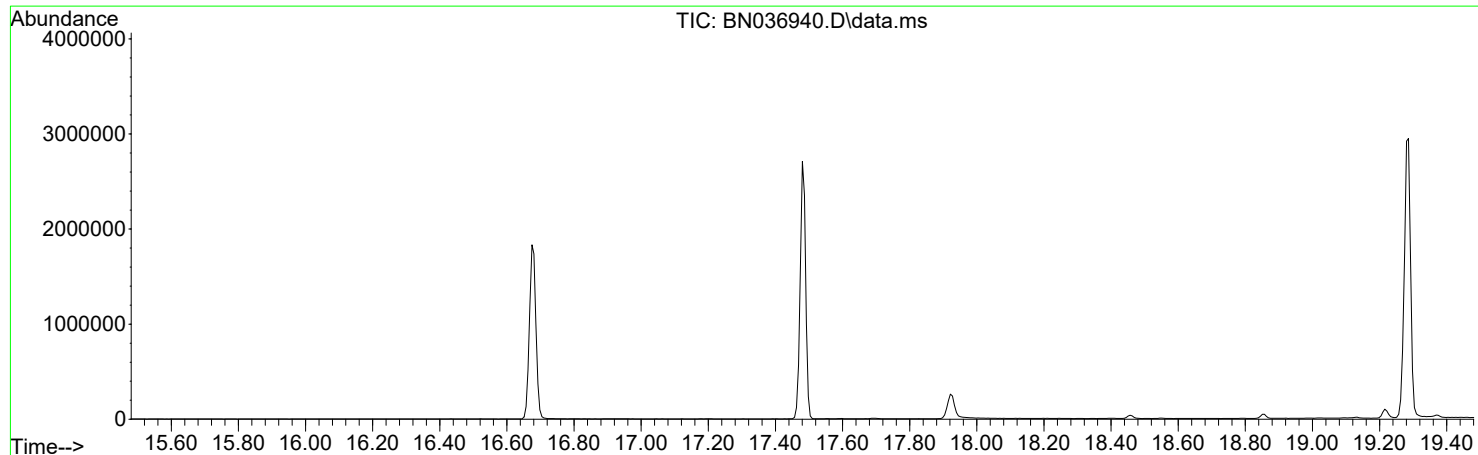

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	72.0	151907	PASS
68	69	0.00	2	0.9	1191	PASS
69	198	0.00	100	60.6	127800	PASS
70	69	0.00	2	0.5	628	PASS
127	198	10	80	54.7	115331	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	211008	PASS
199	198	5	9	6.8	14432	PASS
275	198	10	60	24.7	52133	PASS
365	198	1	100	4.0	8390	PASS
441	198	0.01	100	8.5	17889	PASS
442	442	50	100	100.0	106467	PASS
443	442	15	24	19.5	20798	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/30/2025	BNA_N	<u>BN036940.D</u>
Compound Name	Response	Retention Time
DDT	689285	20.521
DDD	5971	20.133
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5971	695256	0.86

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043025\
Data File : BN036940.D
Acq On : 30 Apr 2025 10:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 30 17:05:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

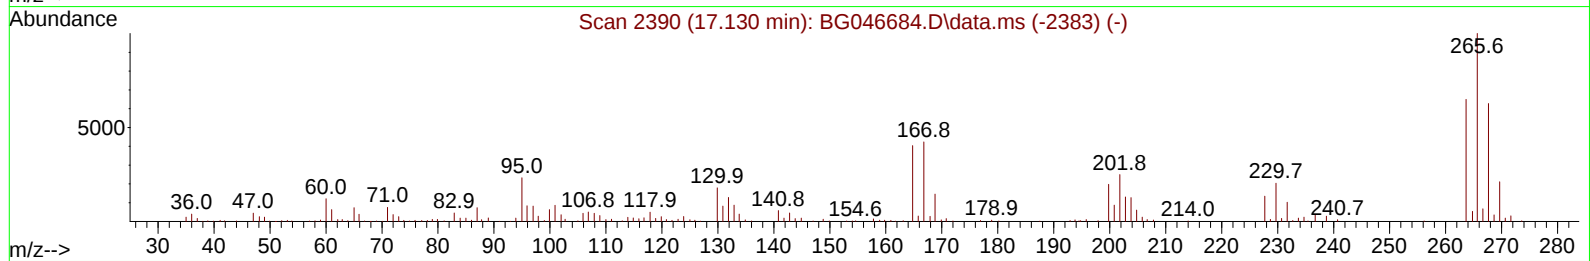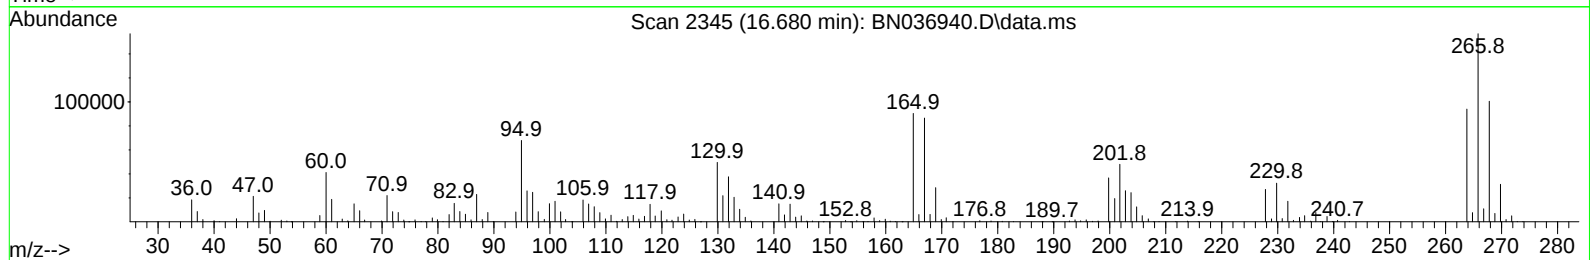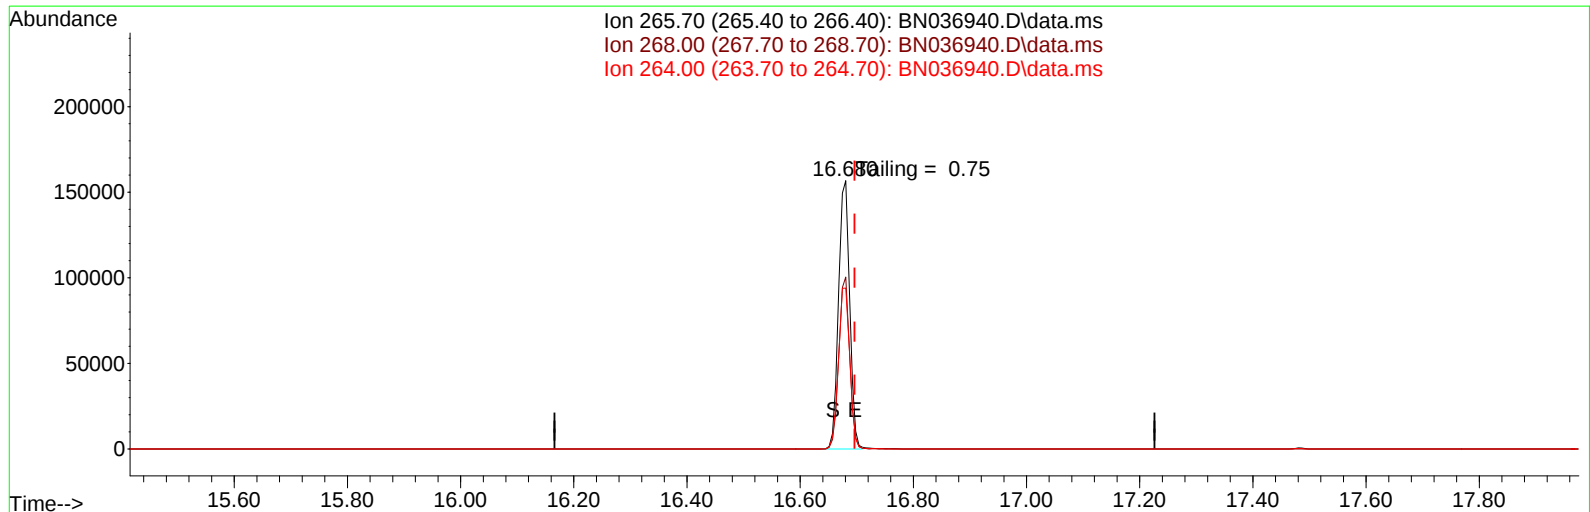

TIC: BN036940.D\data.ms

(70) Pentachlorophenol (C)

16.680min (-0.016) 16606.24 ng




response 213988

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.09
264.00	61.60	59.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043025\
Data File : BN036940.D
Acq On : 30 Apr 2025 10:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 30 17:05:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

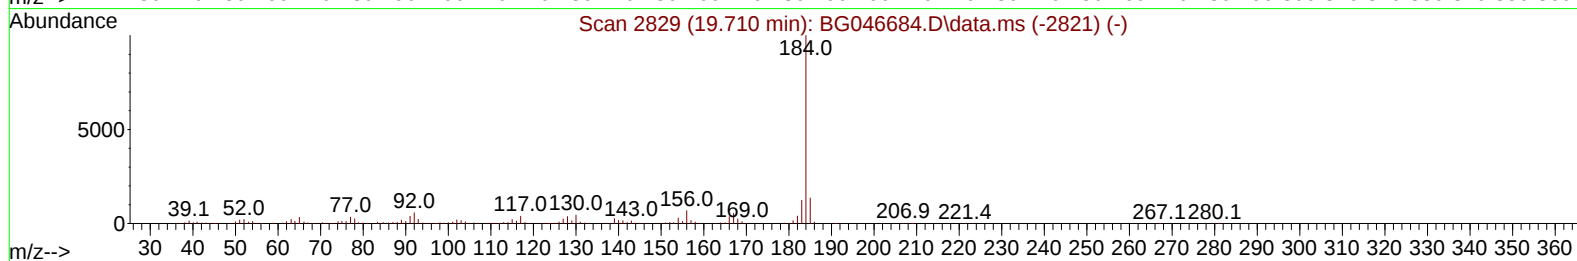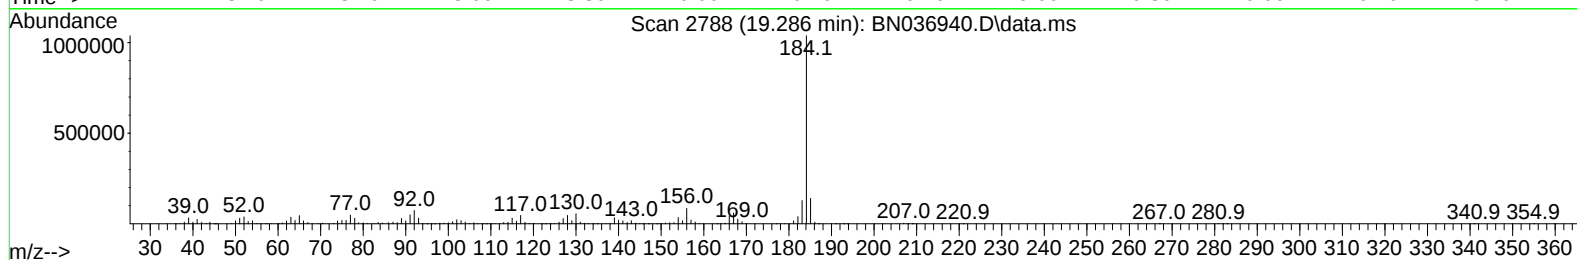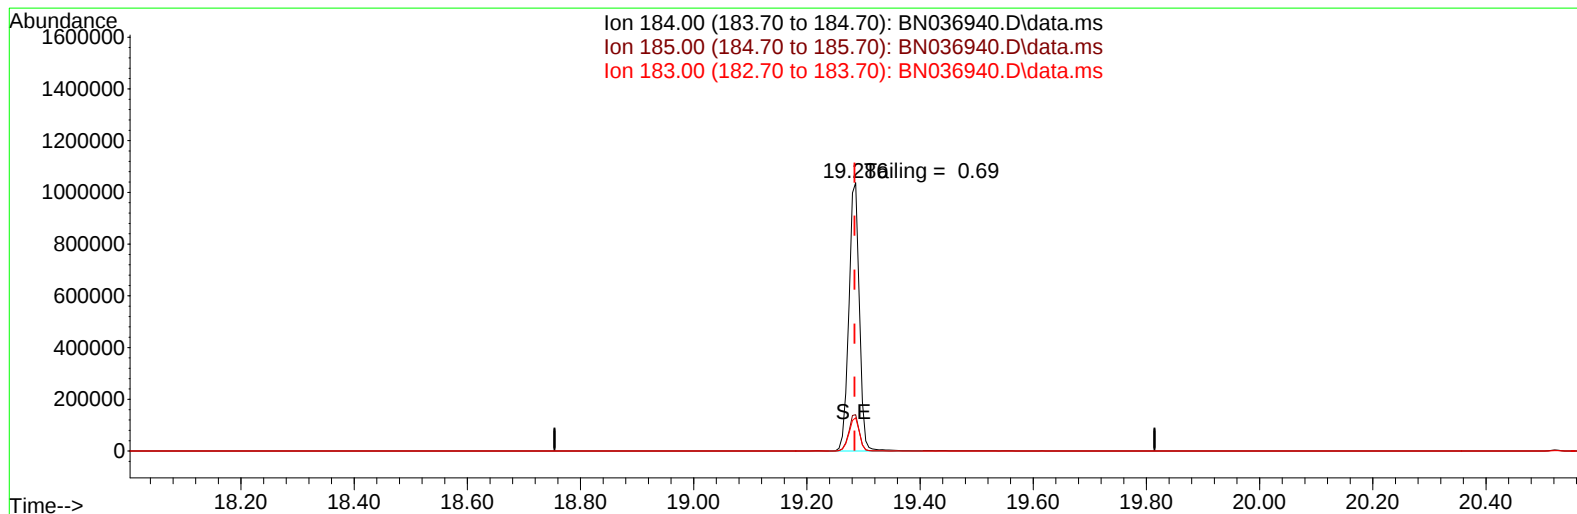

TIC: BN036940.D\data.ms

(77) Benzidine

19.286min (+ 0.002) 0.00 ng

response 1344463

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.57
183.00	13.20	12.39
0.00	0.00	0.00