

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051325\
 Data File : FG015818.D
 Signal(s) : FID1A.ch
 Acq On : 13 May 2025 11:40
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: May 14 03:54:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042425.M
 Quant Title :
 QLast Update : Thu Apr 24 12:54:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.998	5482459	46.565 ug/ml
Target Compounds			
2) N-DECANE	4.499	5351365	48.066 ug/ml
3) N-DODECANE	6.681	5643937	49.248 ug/ml
4) N-TETRADECANE	8.517	5889484	48.604 ug/ml
5) N-HEXADECANE	10.131	6050592	48.196 ug/ml
6) N-OCTADECANE	11.579	6240717	47.620 ug/ml
7) N-EICOSANE	12.895	6359506	46.907 ug/ml
8) N-DOCOSANE	14.097	6209146	46.816 ug/ml
10) N-TETRACOSANE	15.204	6232751	46.903 ug/ml
11) N-HEXACOSANE	16.228	6221359	46.911 ug/ml
12) N-OCTACOSANE	17.181	6278020	47.621 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG051325\
Data File : FG015818.D
Signal(s) : FID1A.ch
Acq On : 13 May 2025 11:40
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: May 14 03:54:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG042425.M
Quant Title :
QLast Update : Thu Apr 24 12:54:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

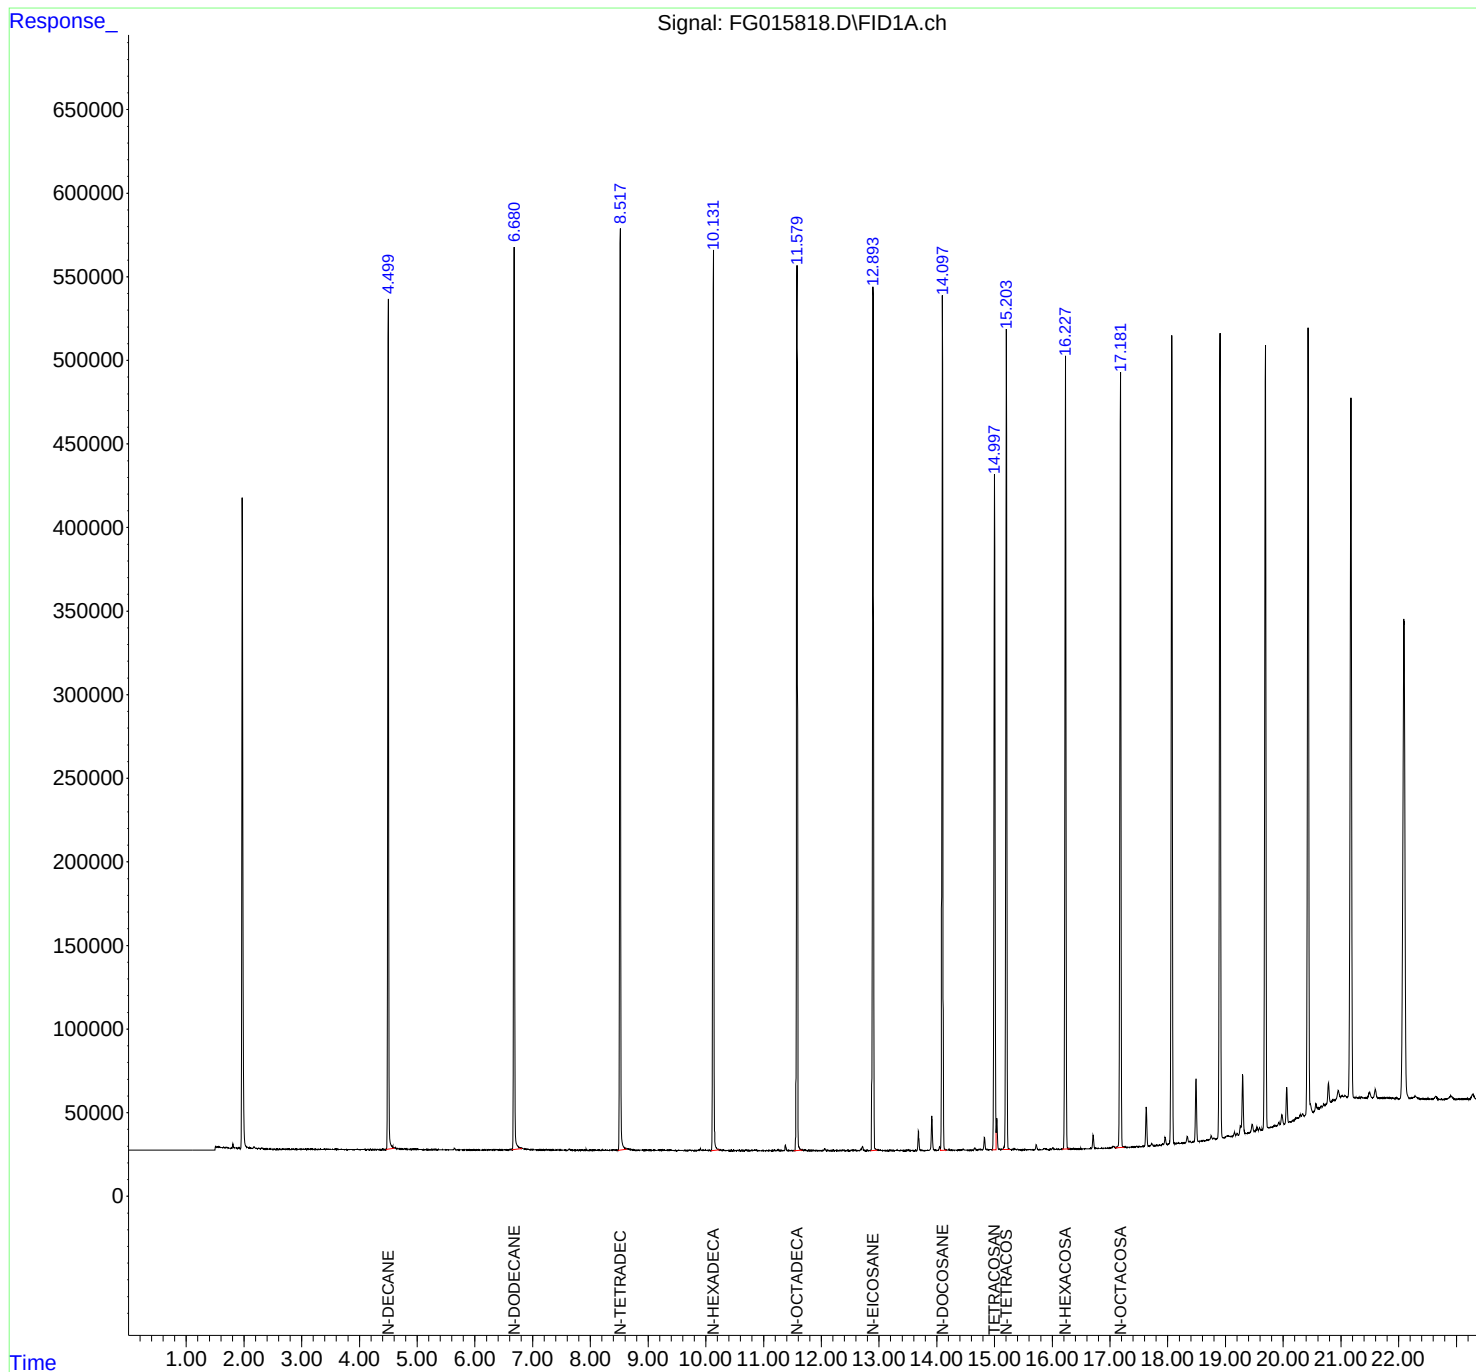


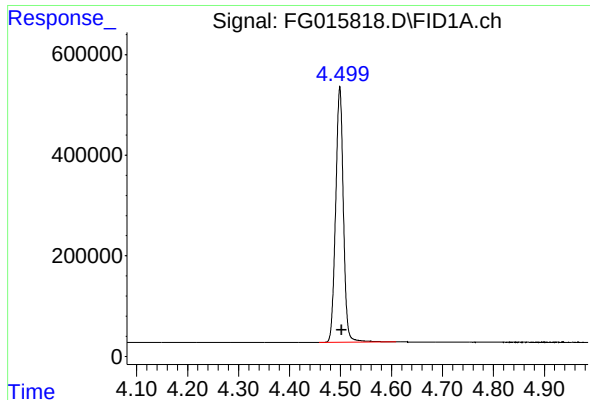

#2 N-DECANE


R.T.: 4.499 min
Delta R.T.: -0.004 min
Response: 5351365
Conc: 48.07 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

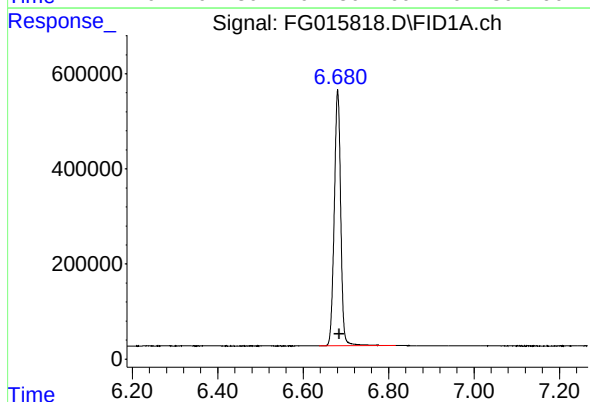


#3 N-DODECANE

R.T.: 6.681 min
Delta R.T.: -0.003 min
Response: 5643937
Conc: 49.25 ug/ml

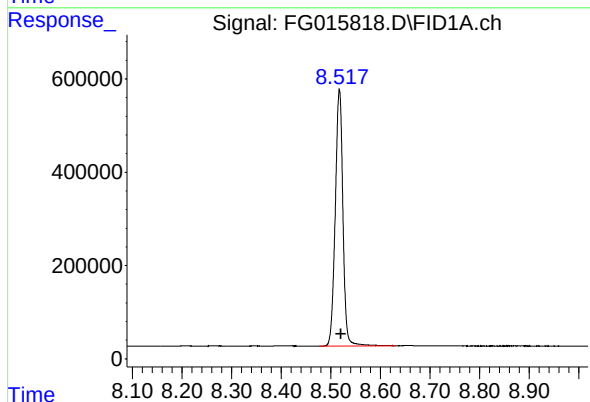


#4 N-TETRADECANE

R.T.: 8.517 min
Delta R.T.: -0.003 min
Response: 5889484
Conc: 48.60 ug/ml

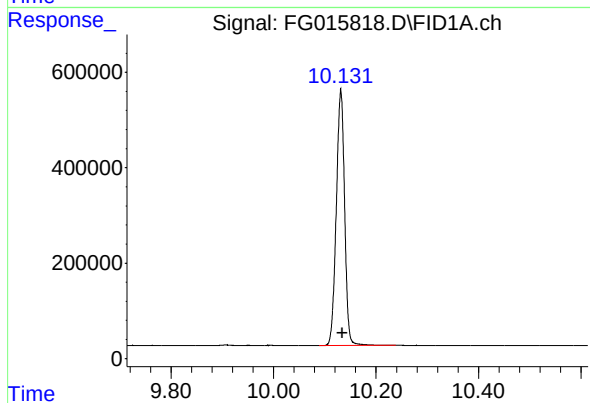

#5 N-HEXADECANE


R.T.: 10.131 min
Delta R.T.: -0.003 min
Response: 6050592
Conc: 48.20 ug/ml

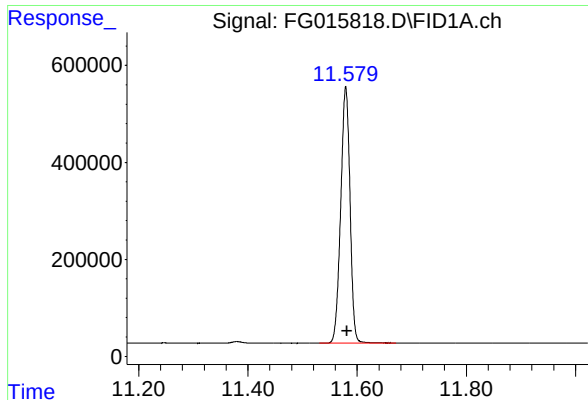

#6 N-OCTADECANE


R.T.: 11.579 min
Delta R.T.: -0.002 min
Response: 6240717
Conc: 47.62 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

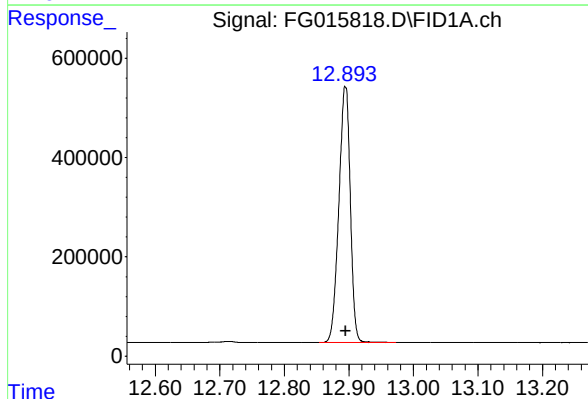


#7 N-EICOSANE

R.T.: 12.895 min
Delta R.T.: 0.000 min
Response: 6359506
Conc: 46.91 ug/ml

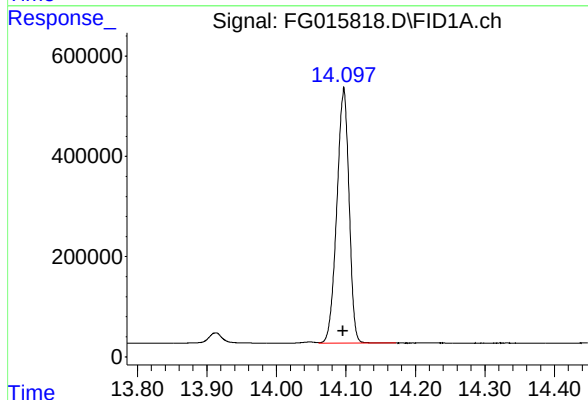


#8 N-DOCOSANE

R.T.: 14.097 min
Delta R.T.: 0.001 min
Response: 6209146
Conc: 46.82 ug/ml

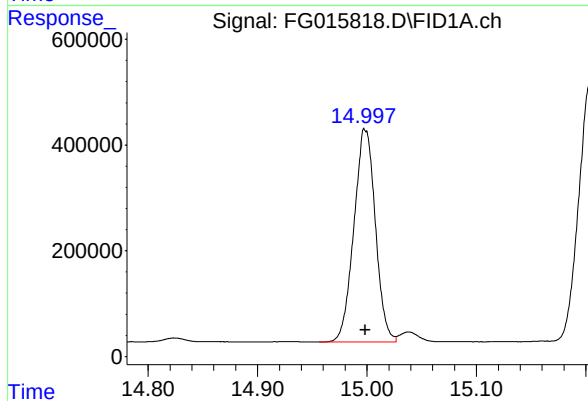

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.998 min
Delta R.T.: 0.000 min
Response: 5482459
Conc: 46.57 ug/ml

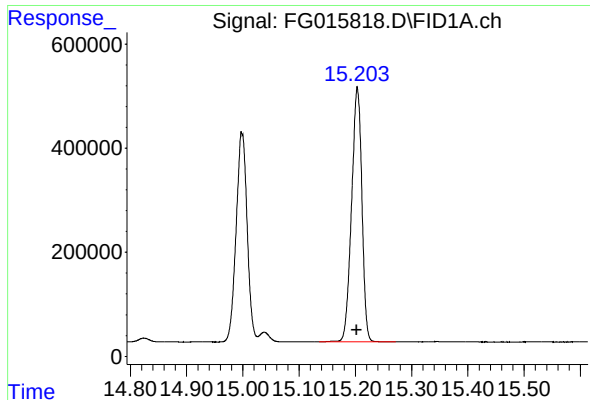

#10 N-TETRACOSANE


R.T.: 15.204 min
Delta R.T.: 0.001 min
Response: 6232751
Conc: 46.90 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

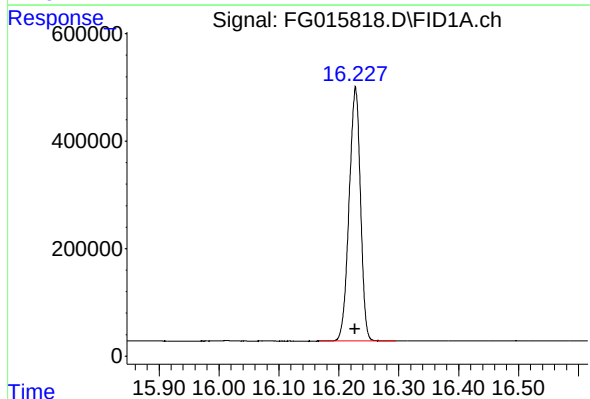

#11 N-HEXACOSANE

R.T.: 16.228 min
Delta R.T.: 0.001 min
Response: 6221359
Conc: 46.91 ug/ml

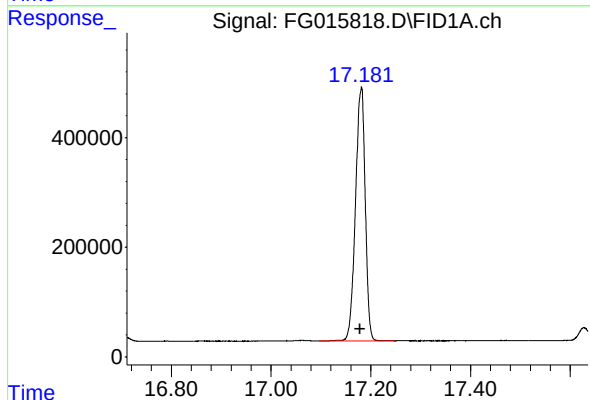

#12 N-OCTACOSANE

R.T.: 17.181 min
Delta R.T.: 0.002 min
Response: 6278020
Conc: 47.62 ug/ml