

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051925\
 Data File : PD088585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2025 11:17
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 14:00:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051925.M
 Quant Title : GC Extractables
 QLast Update : Mon May 19 13:57:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.881	41487143	300.1E6	19.174	19.836
28) SA Decachlor...	9.077	8.075	69355454	365.4E6	20.266	20.017
Target Compounds						
9) A Endosulfan I	6.076	5.249	33273453	185.2E6	8.842	9.760
10) B gamma-Chl...	5.948	5.128	36597267	220.9E6	9.175	10.355
12) B 4,4'-DDE	6.198	5.377	66676699	417.9E6	18.576	19.993
13) MA Dieldrin	6.350	5.515	73699578	411.2E6	18.371	19.539
19) B Endosulfa...	7.152	6.485	60919862	351.5E6	19.019	19.795
20) A Methoxychlor	7.495	6.757	152.5E6	804.8E6	91.284	84.053
21) B Endrin ke...	7.633	6.994	64436060	381.7E6	18.824	19.728



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051925\
Data File : PD088585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2025 11:17
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 14:00:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051925.M
Quant Title : GC Extractables
QLast Update : Mon May 19 13:57:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

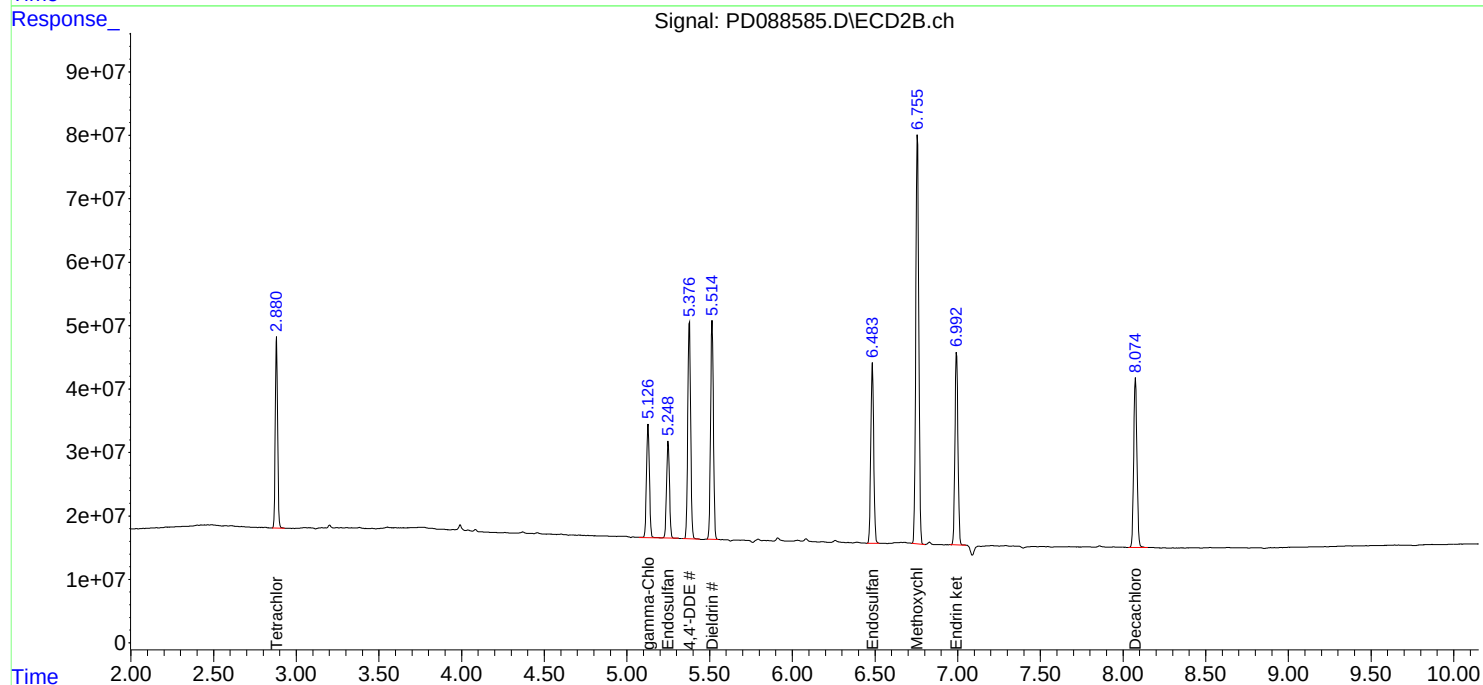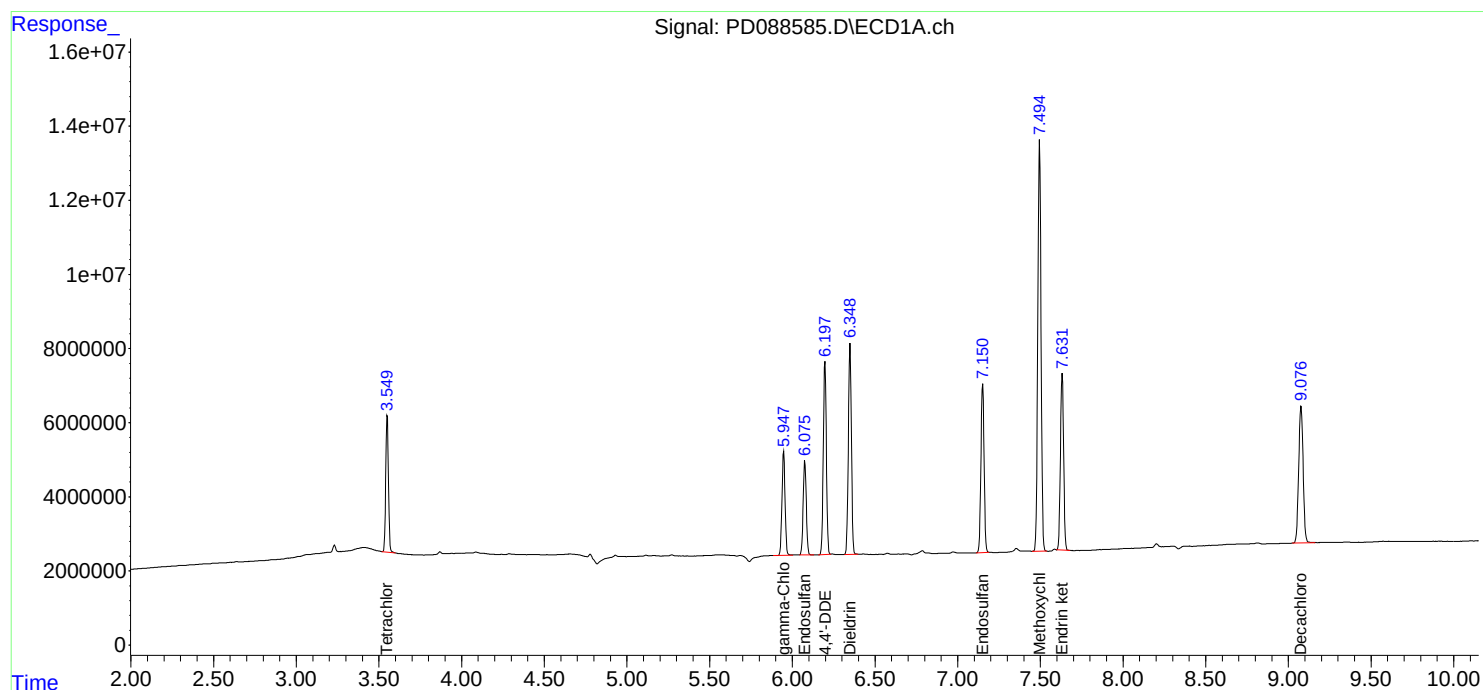


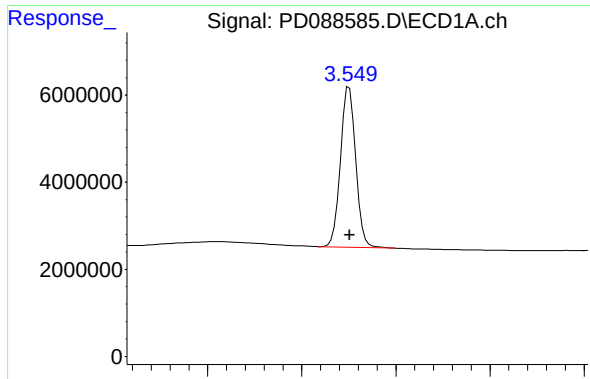

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 41487143
Conc: 19.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

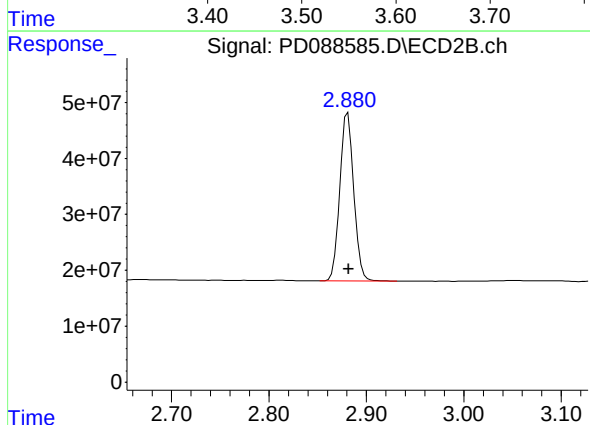


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 300055852
Conc: 19.84 ng/ml

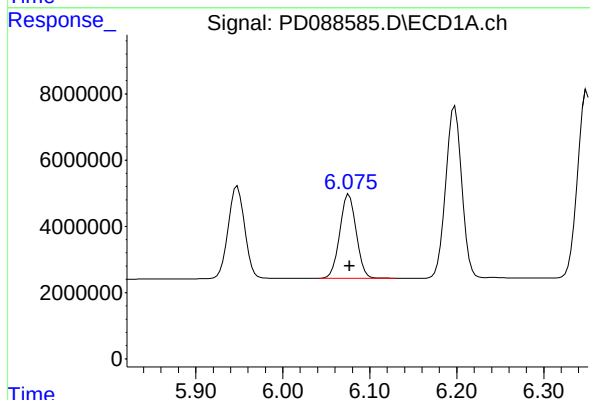


#9 Endosulfan I

R.T.: 6.076 min
Delta R.T.: -0.001 min
Response: 33273453
Conc: 8.84 ng/ml

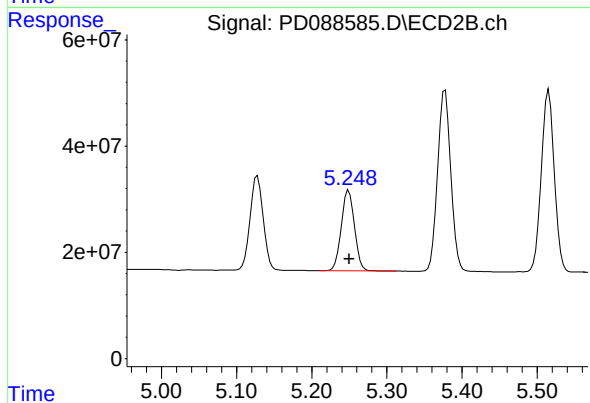

#9 Endosulfan I


R.T.: 5.249 min
Delta R.T.: 0.000 min
Response: 185230529
Conc: 9.76 ng/ml

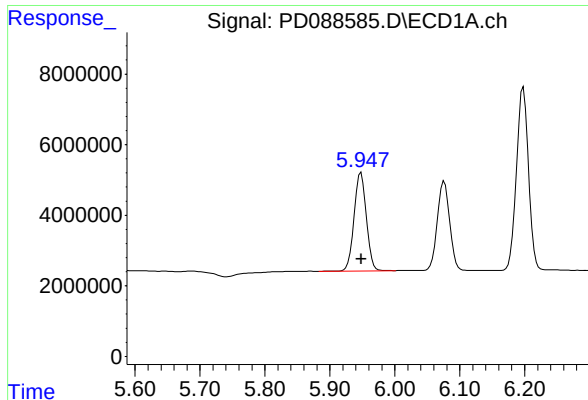

#10 gamma-Chlordane


R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 36597267
Conc: 9.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

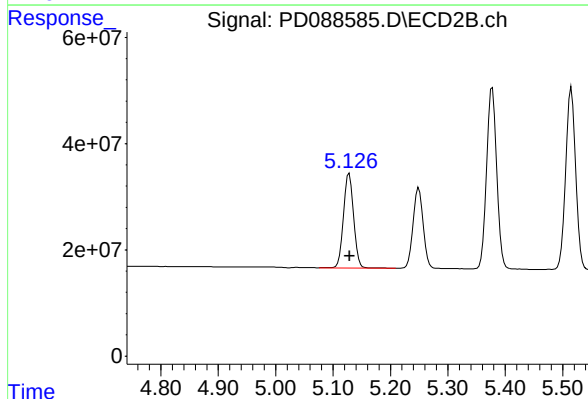


#10 gamma-Chlordane

R.T.: 5.128 min
Delta R.T.: 0.000 min
Response: 220885783
Conc: 10.35 ng/ml

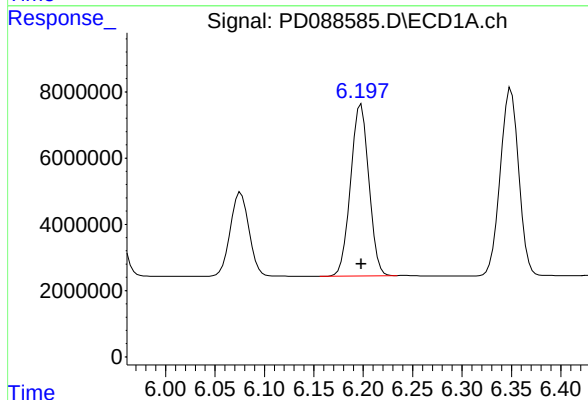


#12 4,4'-DDE

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 66676699
Conc: 18.58 ng/ml

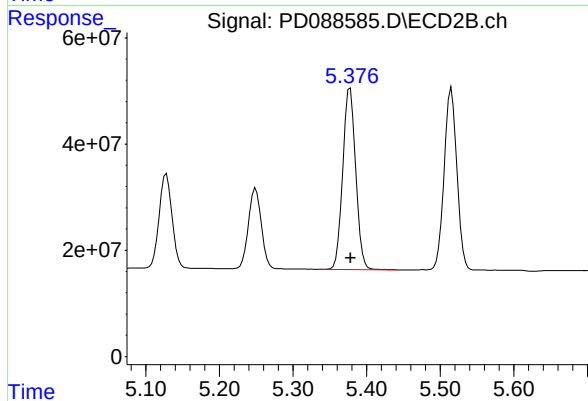

#12 4,4'-DDE


R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 417897527
Conc: 19.99 ng/ml

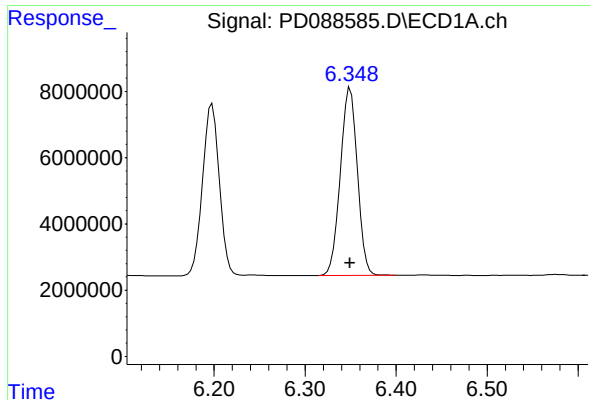

#13 Dieldrin


R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 73699578
Conc: 18.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

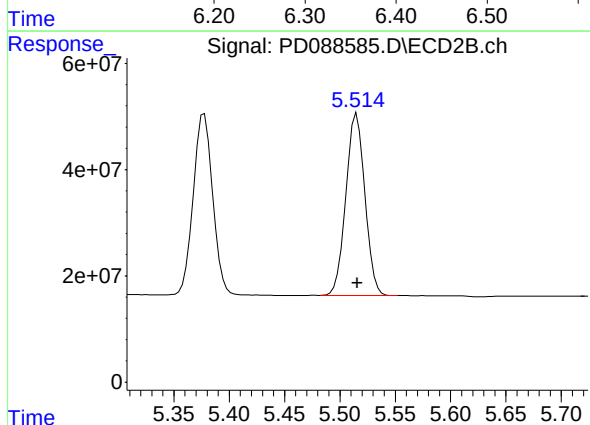


#13 Dieldrin

R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 411171083
Conc: 19.54 ng/ml

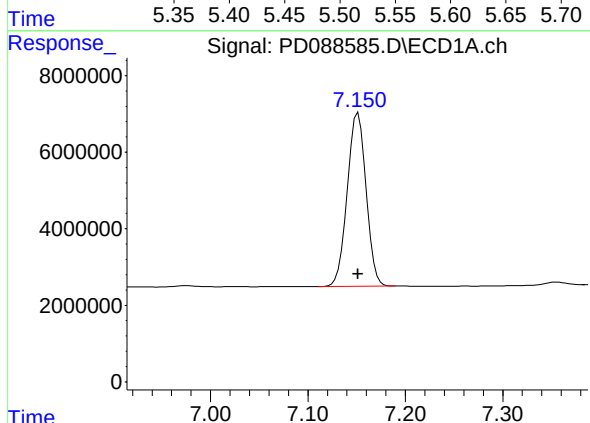


#19 Endosulfan Sulfate

R.T.: 7.152 min
Delta R.T.: 0.000 min
Response: 60919862
Conc: 19.02 ng/ml

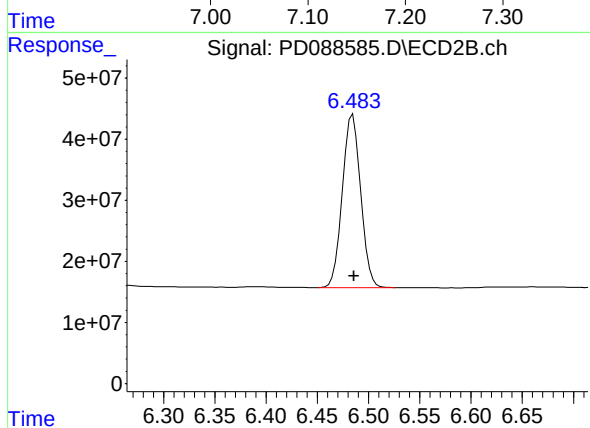

#19 Endosulfan Sulfate


R.T.: 6.485 min
Delta R.T.: -0.001 min
Response: 351483349
Conc: 19.80 ng/ml

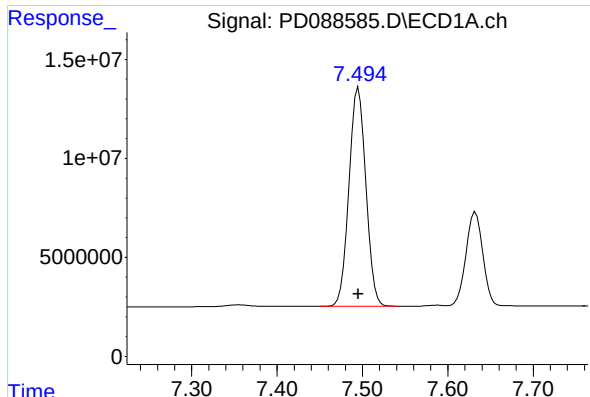

#20 Methoxychlor


R.T.: 7.495 min
Delta R.T.: 0.000 min
Response: 152495142
Conc: 91.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

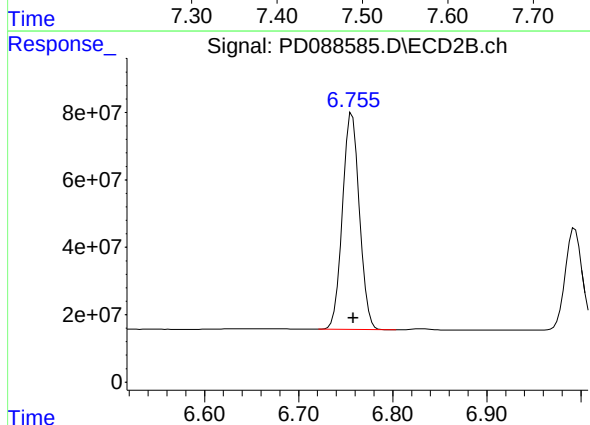


#20 Methoxychlor

R.T.: 6.757 min
Delta R.T.: -0.001 min
Response: 804794407
Conc: 84.05 ng/ml

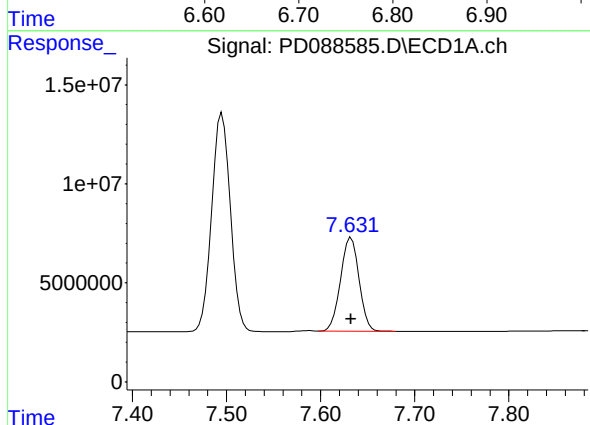


#21 Endrin ketone

R.T.: 7.633 min
Delta R.T.: 0.000 min
Response: 64436060
Conc: 18.82 ng/ml

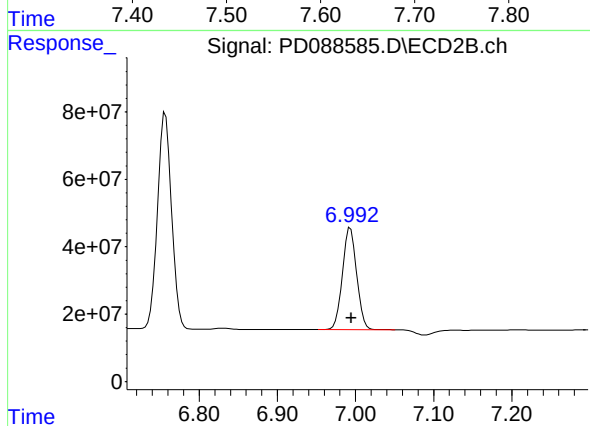

#21 Endrin ketone


R.T.: 6.994 min
Delta R.T.: -0.001 min
Response: 381682681
Conc: 19.73 ng/ml

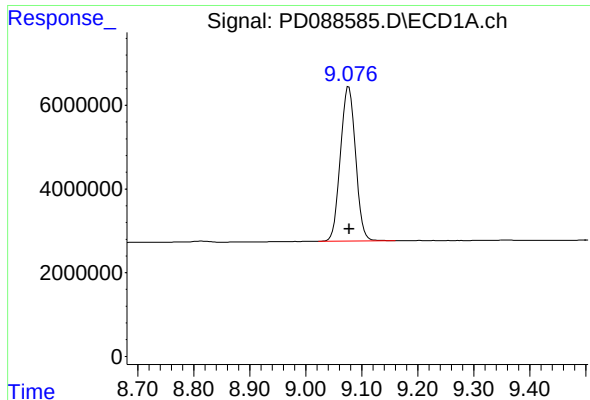

#28 Decachlorobiphenyl

R.T.: 9.077 min
Delta R.T.: 0.000 min
Response: 69355454
Conc: 20.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

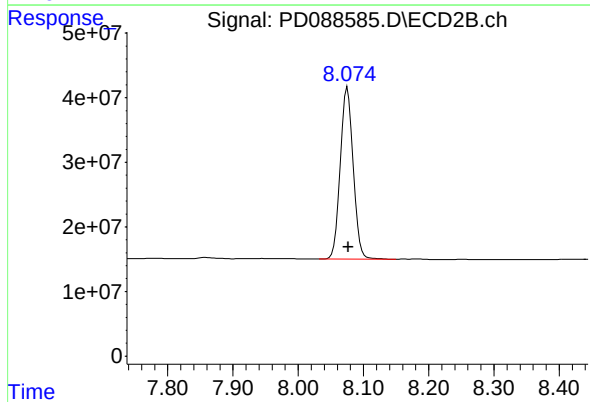

#28 Decachlorobiphenyl

R.T.: 8.075 min
Delta R.T.: -0.001 min
Response: 365434486
Conc: 20.02 ng/ml