


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
Data File : BM050023.D
Acq On : 28 Apr 2025 11:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

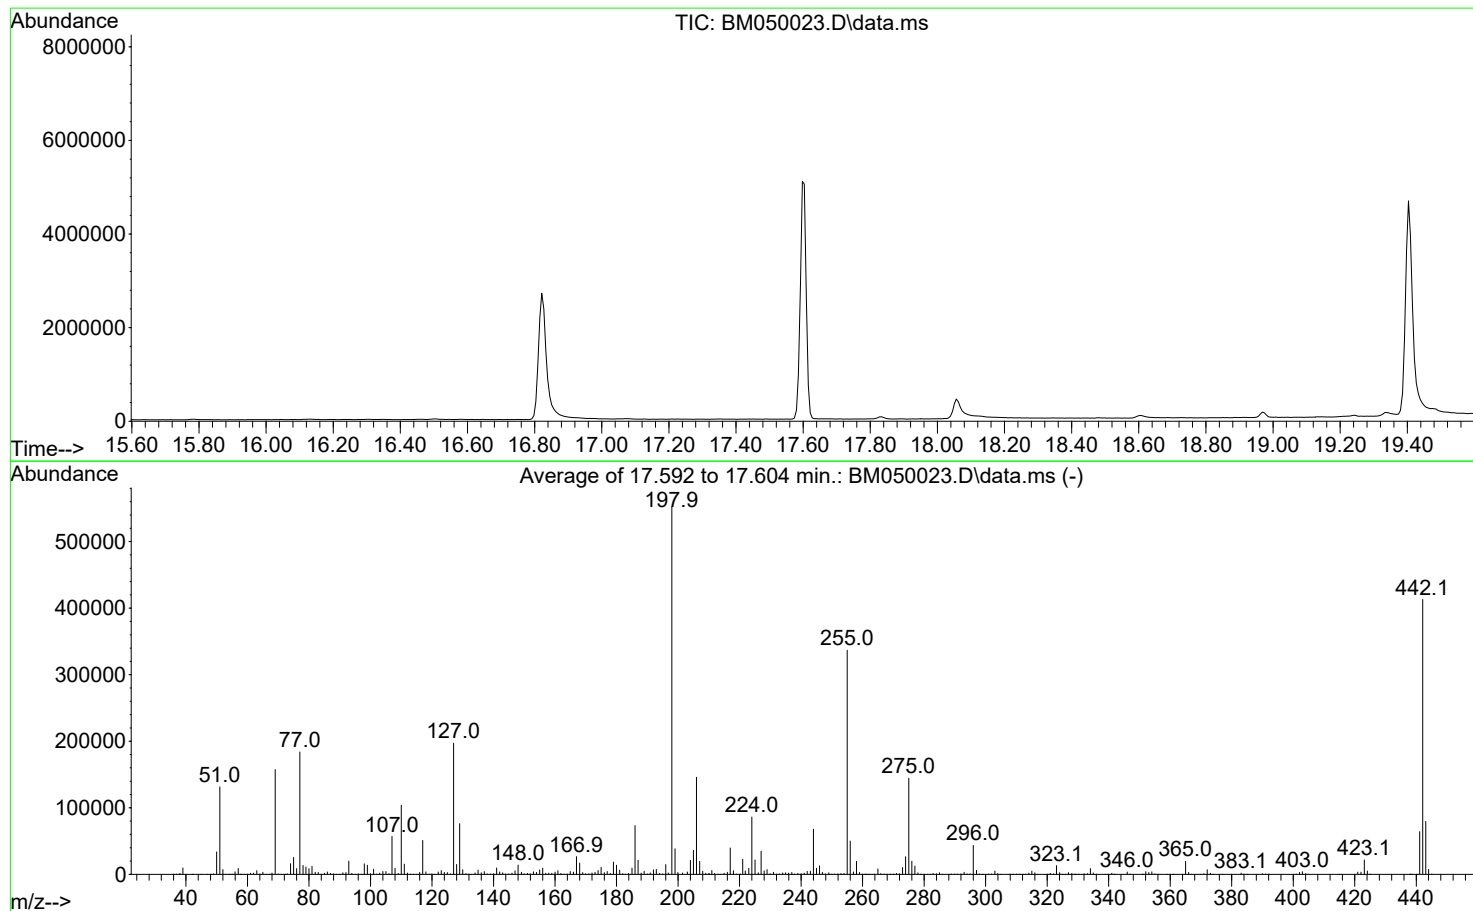

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	131521	PASS
68	69	0.00	2	1.3	2026	PASS
69	198	0.00	100	28.5	157569	PASS
70	69	0.00	2	0.4	660	PASS
127	198	10	80	35.7	197099	PASS
197	198	0.00	2	0.4	2228	PASS
198	198	100	100	100.0	552704	PASS
199	198	5	9	7.0	38461	PASS
275	198	10	60	26.2	144571	PASS
365	198	1	100	3.5	19537	PASS
441	198	0.01	100	11.6	64259	PASS
442	442	50	100	100.0	413099	PASS
443	442	15	24	19.3	79557	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
4/28/2025	BNA_M	<u>BM050023.D</u>
Compound Name	Response	Retention Time
DDT	1978095	20.639
DDD	17600	20.251
DDE	1351	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18951	1997046	0.95

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
Data File : BM050023.D
Acq On : 28 Apr 2025 11:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 28 15:37:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

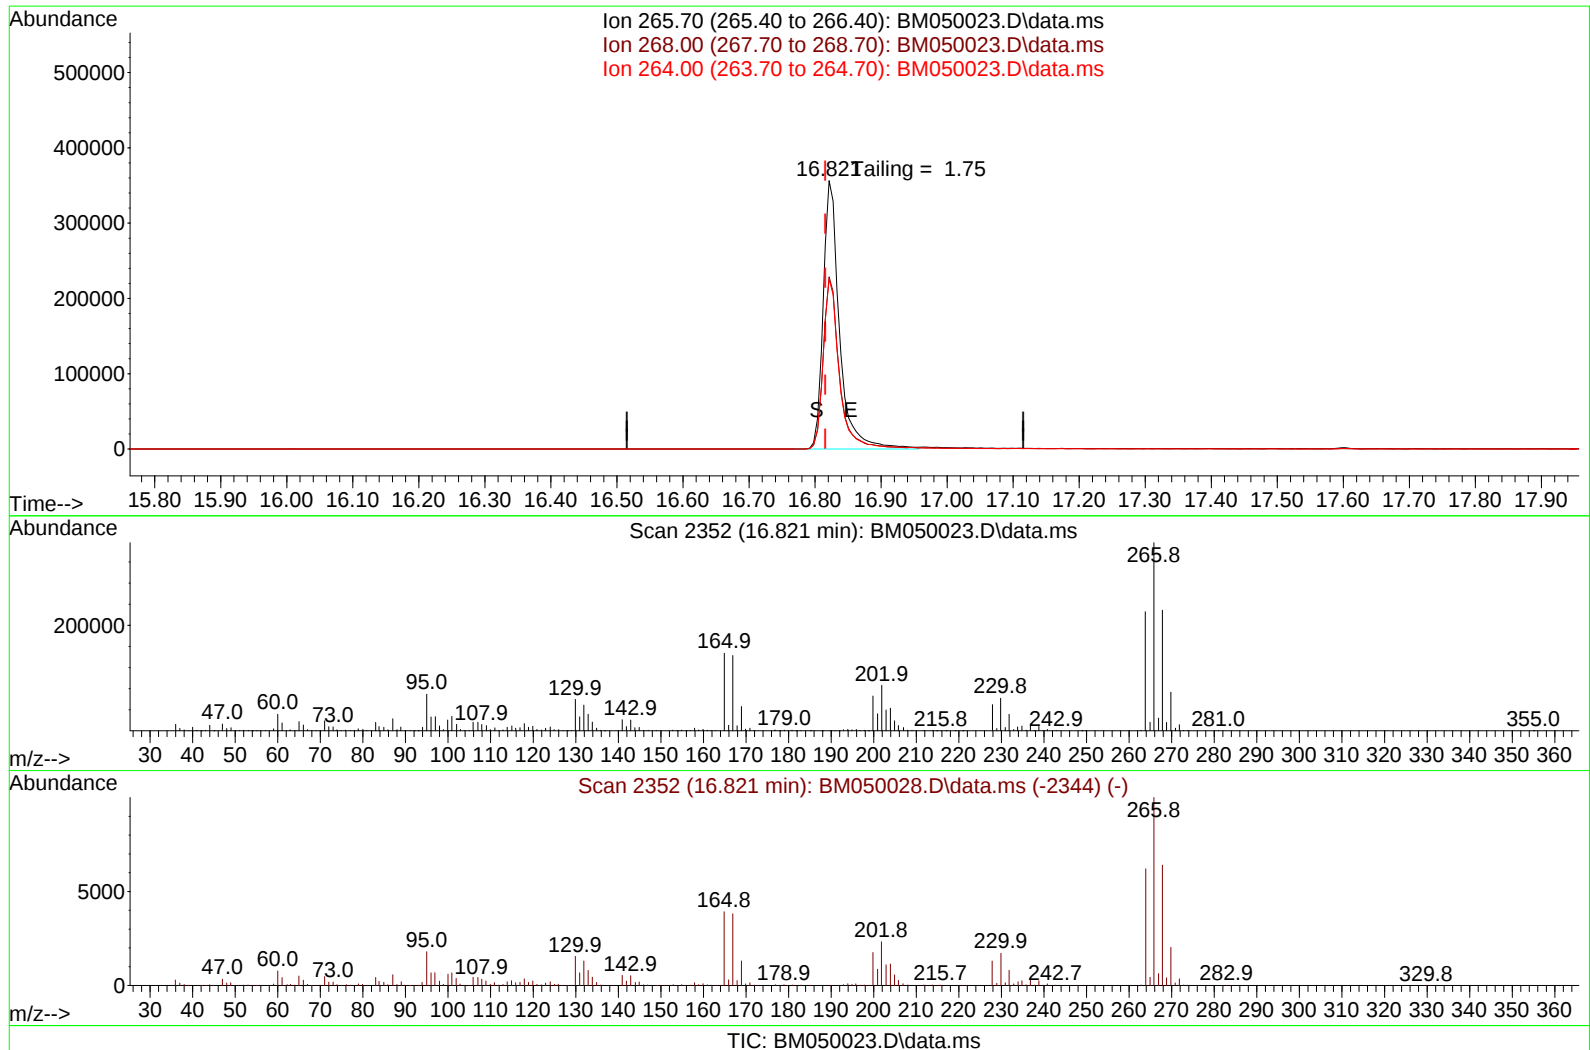

TIC: BM050023.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.006) 652247.26 ng




response 613835

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.13
264.00	62.30	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042825\
Data File : BM050023.D
Acq On : 28 Apr 2025 11:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 28 15:37:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 09 04:00:55 2025
Response via : Initial Calibration

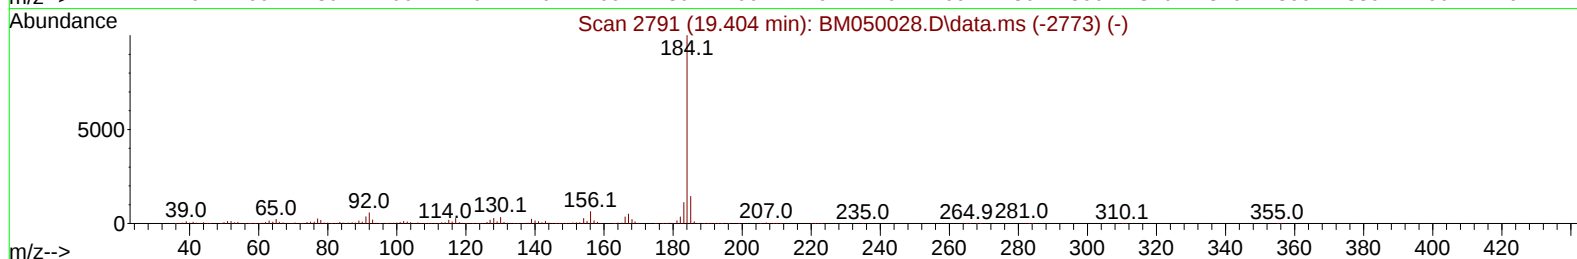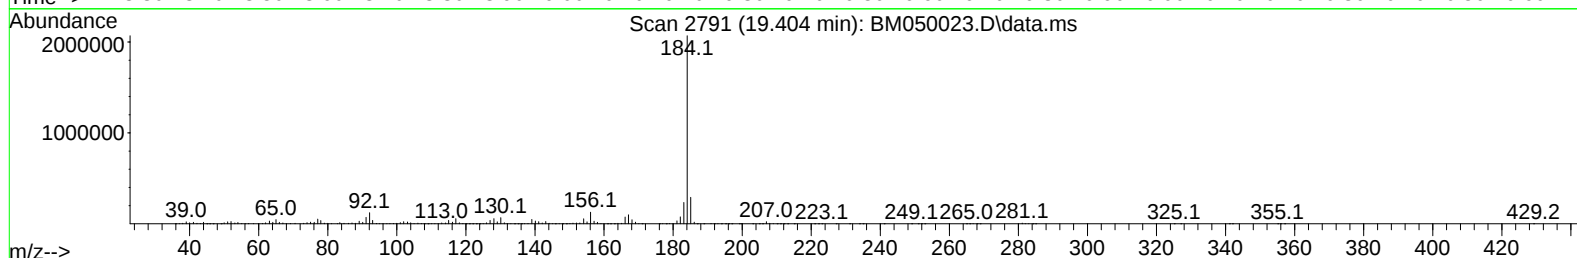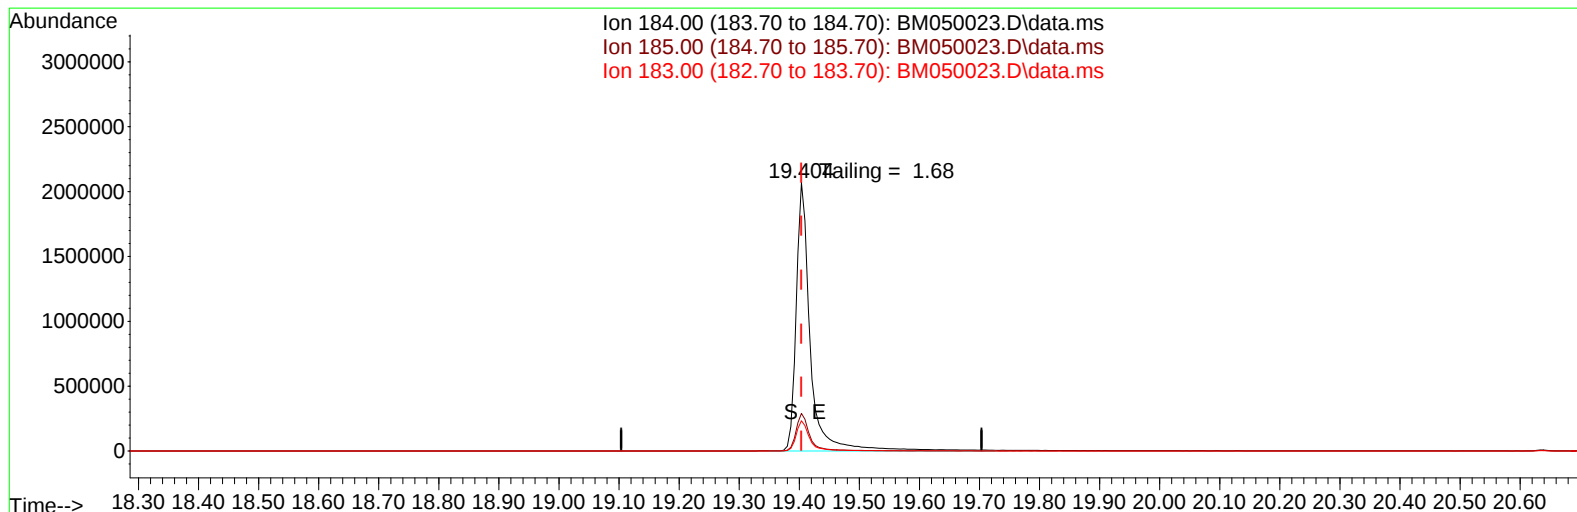

TIC: BM050023.D\data.ms

(77) Benzidine**19.404min (+ 0.000) 1761877.84 ng****response 3412576**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.06
183.00	11.00	11.29
0.00	0.00	0.00