


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050825\
Data File : BP024567.D
Acq On : 08 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

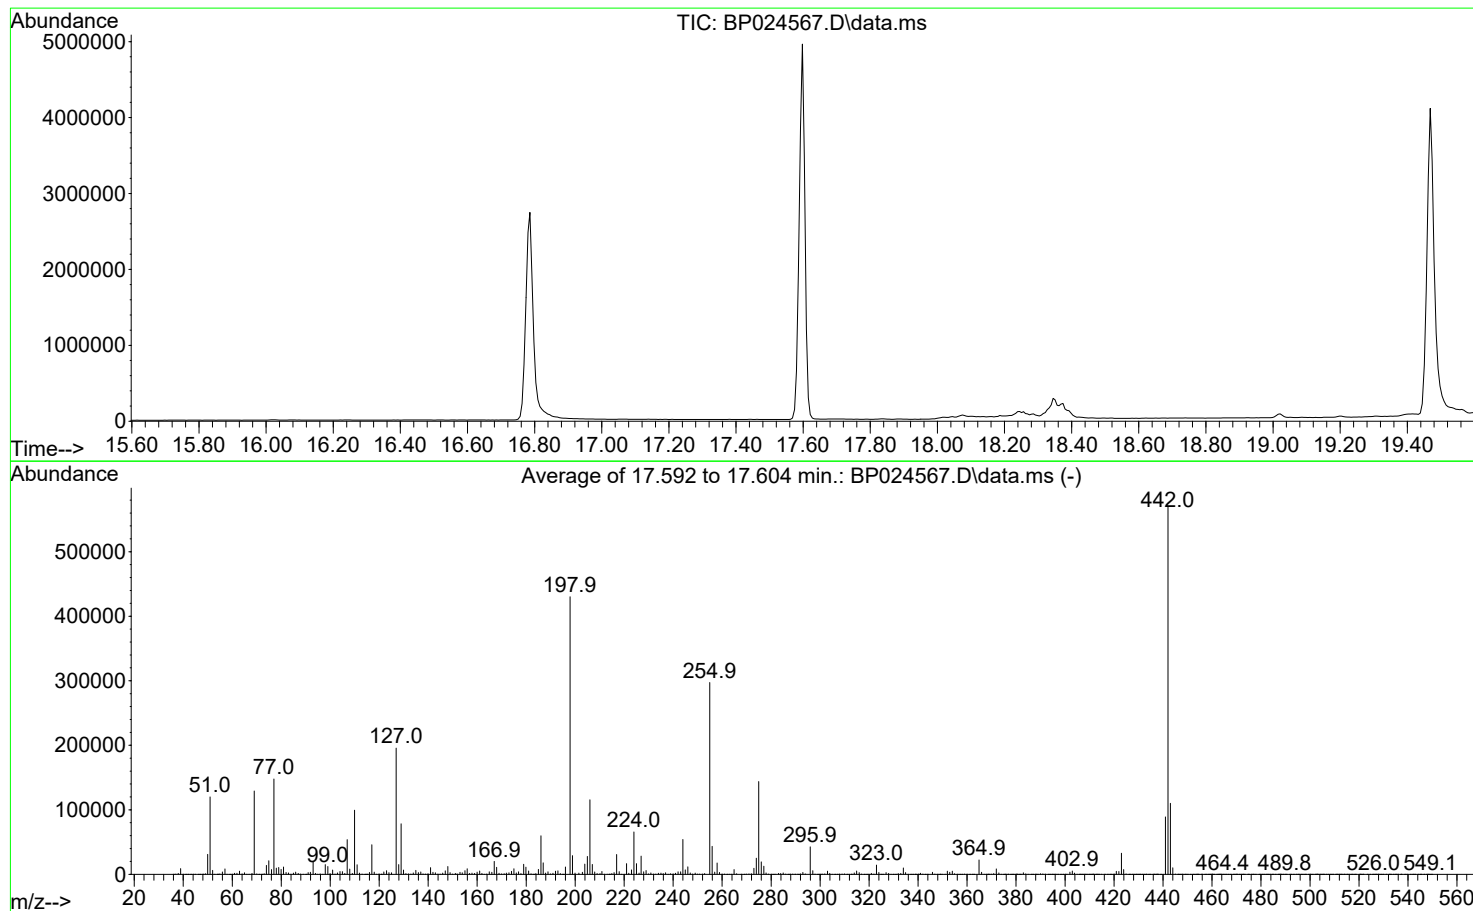

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	120114	PASS
68	69	0.00	2	1.2	1591	PASS
69	198	0.00	100	30.1	129294	PASS
70	69	0.00	2	0.6	754	PASS
127	198	10	80	45.5	195716	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	430133	PASS
199	198	5	9	6.8	29109	PASS
275	198	10	60	33.5	143952	PASS
365	198	1	100	5.2	22422	PASS
441	198	0.01	100	20.7	89080	PASS
442	442	100	100	100.0	570069	PASS
443	442	15	24	19.3	110223	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/8/2025	BNA_P	<u>BP024567.D</u>
Compound Name	Response	Retention Time
DDT	1299893	20.756
DDD	30641	20.298
DDE	2361	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33002	1332895	2.48

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050825\
Data File : BP024567.D
Acq On : 08 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 08 15:11:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

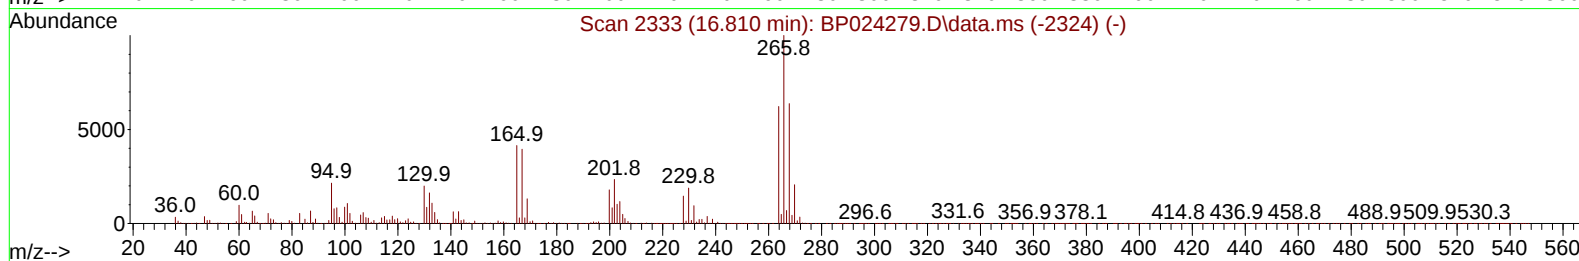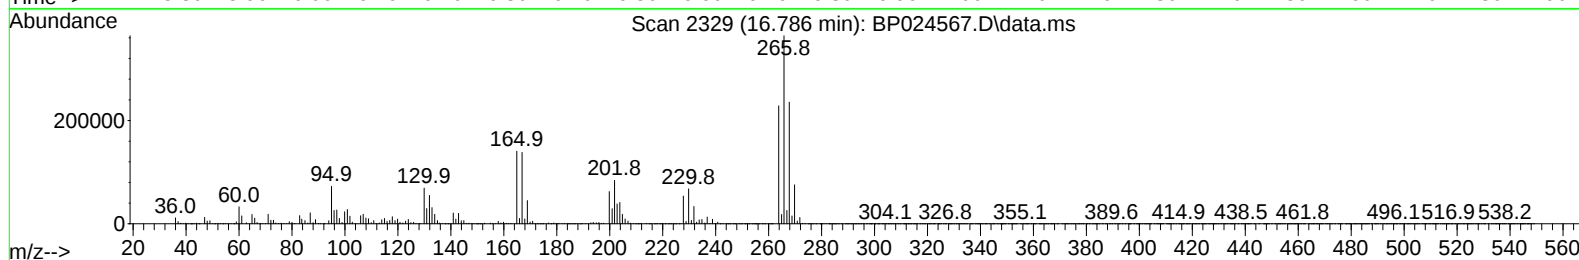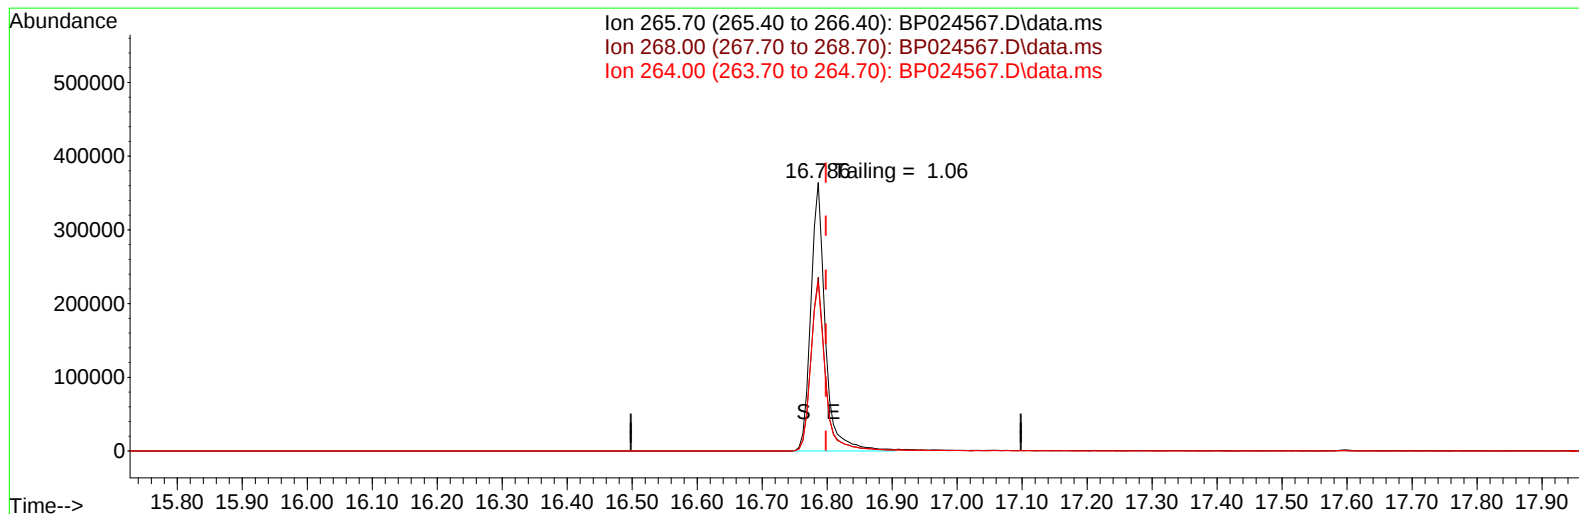

TIC: BP024567.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.012) 35045.60 ng




response 573194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.70
264.00	62.20	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050825\
Data File : BP024567.D
Acq On : 08 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 08 15:11:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

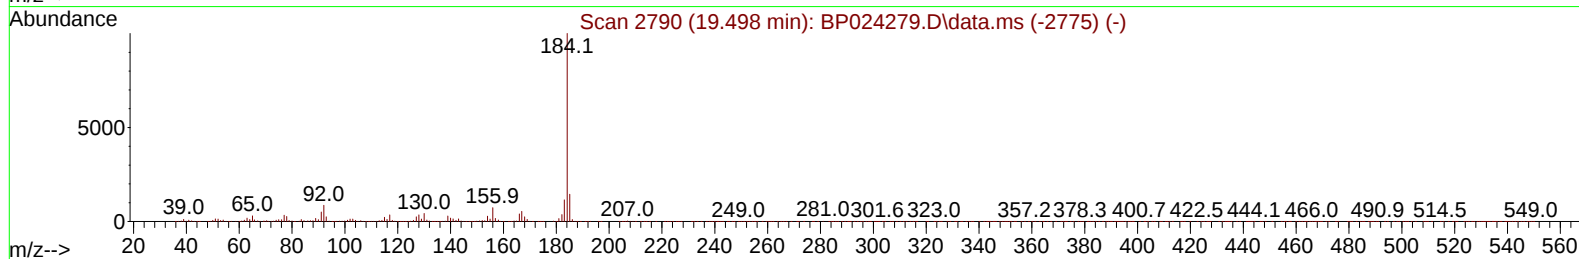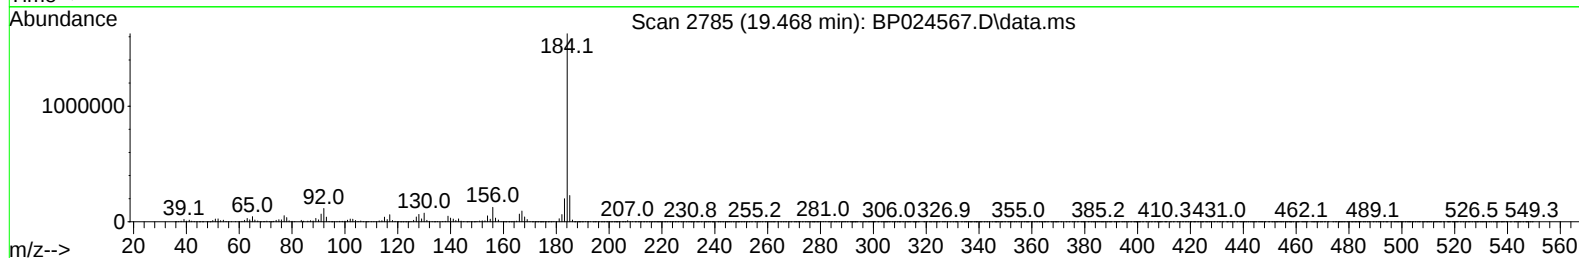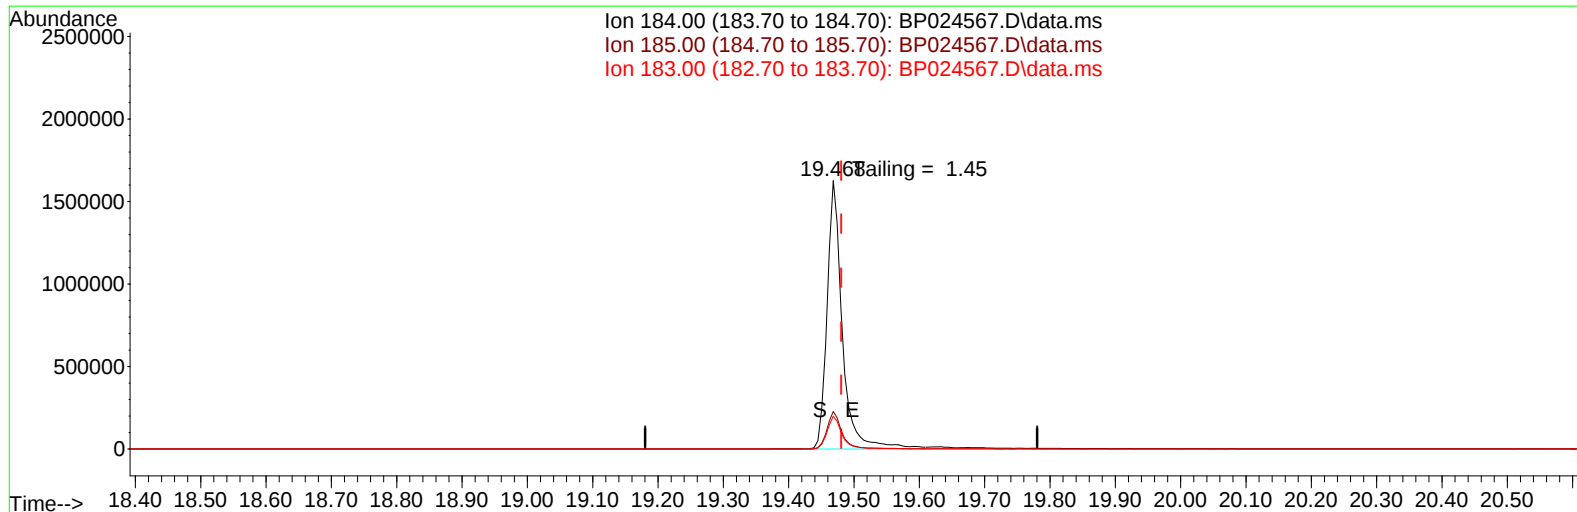

TIC: BP024567.D\data.ms

(77) Benzidine

19.468min (-0.012) 33720.75 ng

response 2634734

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.96
183.00	11.50	12.24
0.00	0.00	0.00