
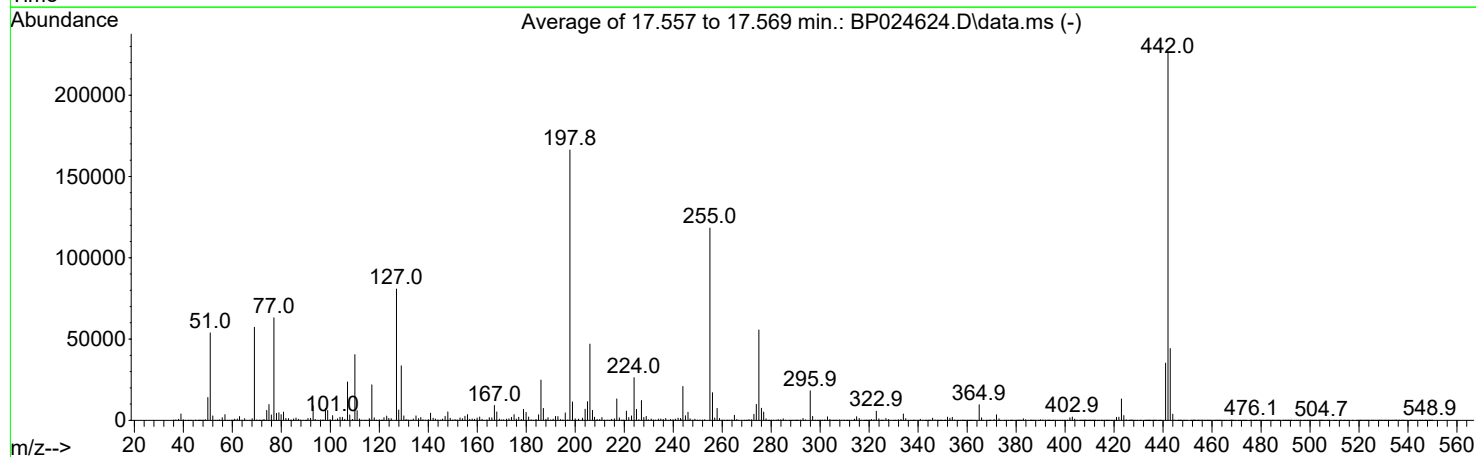


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051425\
Data File : BP024624.D
Acq On : 14 May 2025 10:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

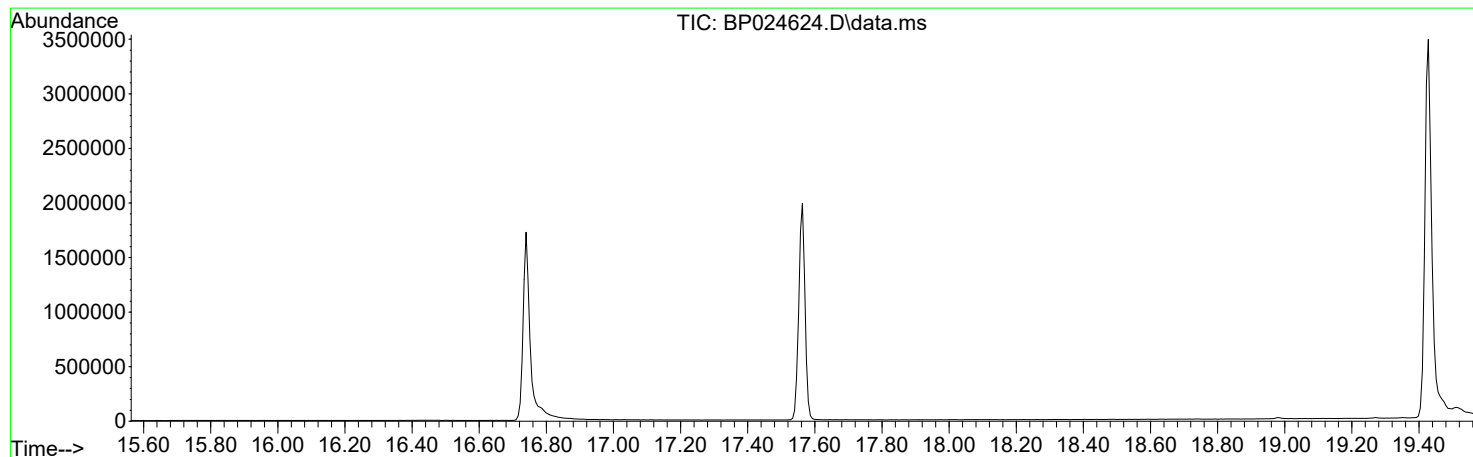

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	53822	PASS
68	69	0.00	2	1.9	1106	PASS
69	198	0.00	100	34.4	57285	PASS
70	69	0.00	2	0.6	340	PASS
127	198	10	80	48.6	80786	PASS
197	198	0.00	2	0.2	309	PASS
198	198	100	100	100.0	166319	PASS
199	198	5	9	6.8	11274	PASS
275	198	10	60	33.4	55576	PASS
365	198	1	100	5.8	9657	PASS
441	198	0.01	100	21.2	35184	PASS
442	442	100	100	100.0	226240	PASS
443	442	15	24	19.5	44145	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/14/2025	BNA_P	<u>BP024624.D</u>
Compound Name	Response	Retention Time
DDT	712469	20.71
DDD	10959	20.304
DDE	1350	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12309	724778	1.70

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051425\
Data File : BP024624.D
Acq On : 14 May 2025 10:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 14 11:18:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

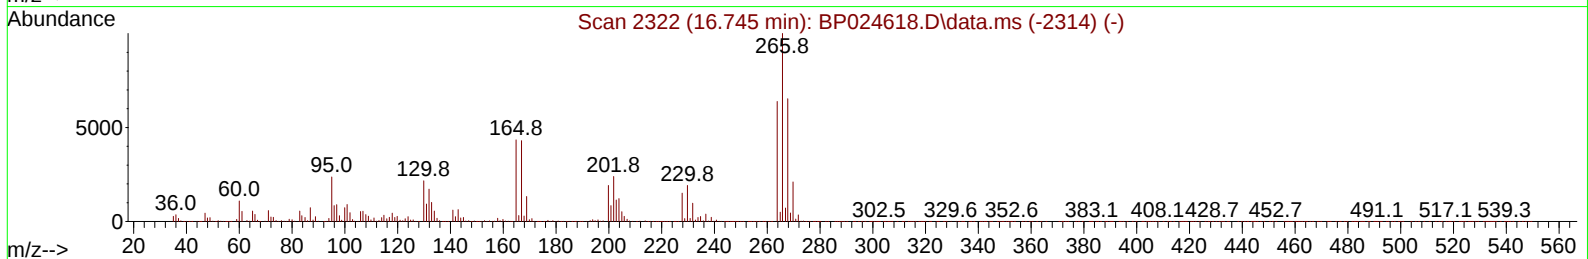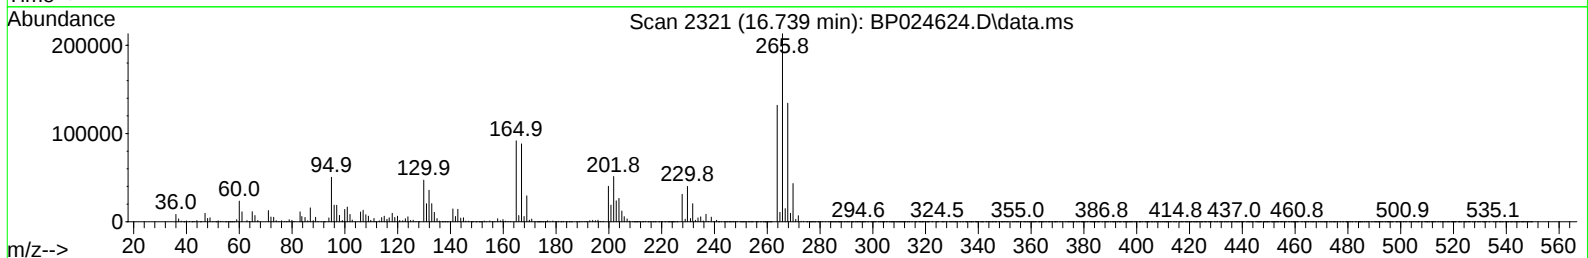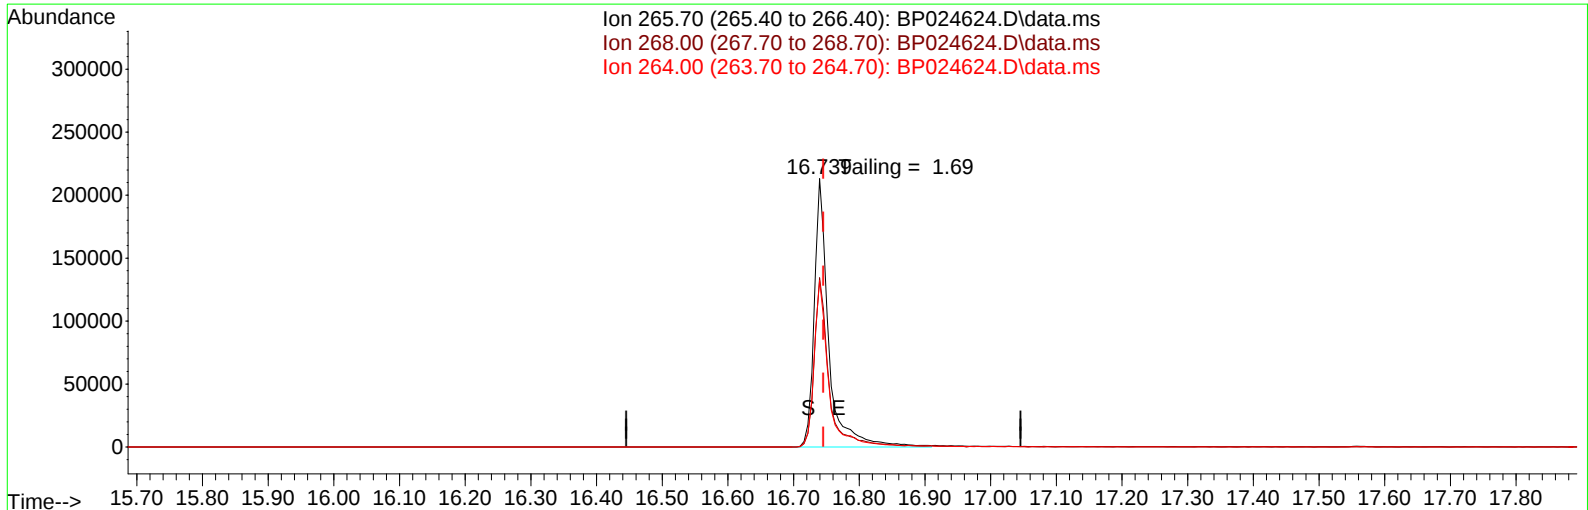

TIC: BP024624.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.006) 4865870.98 ng




response 327184

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.09
264.00	63.90	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051425\
Data File : BP024624.D
Acq On : 14 May 2025 10:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 14 11:18:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

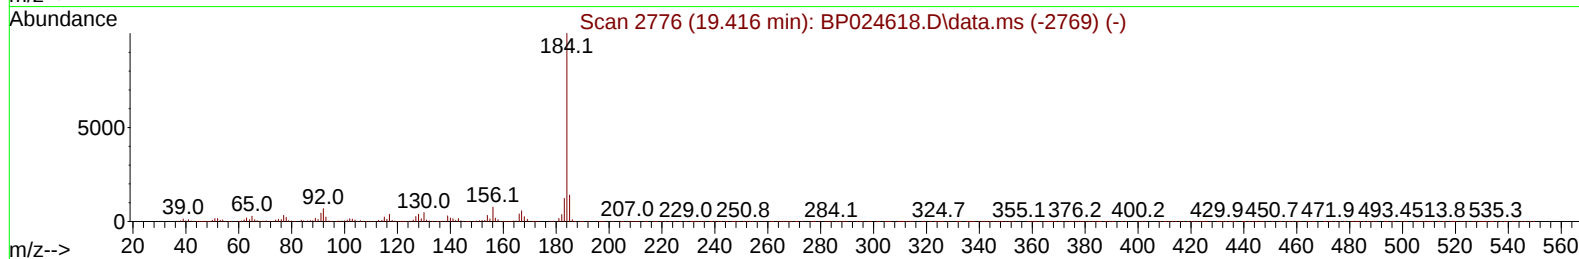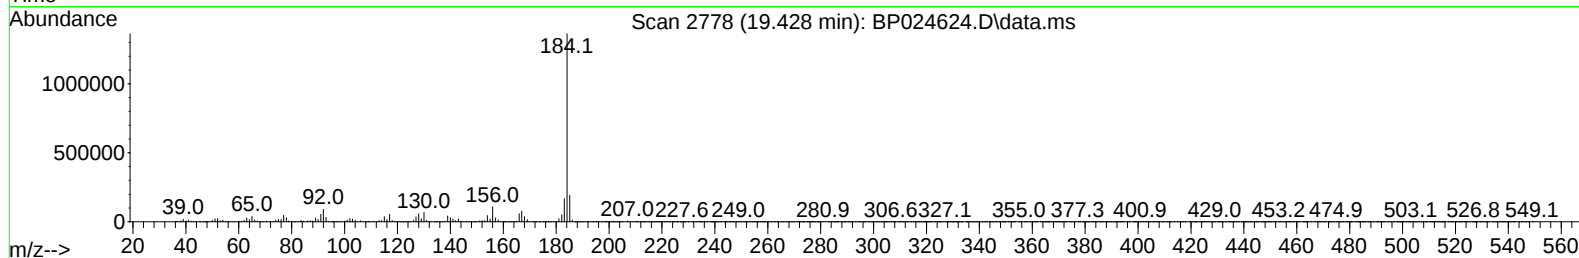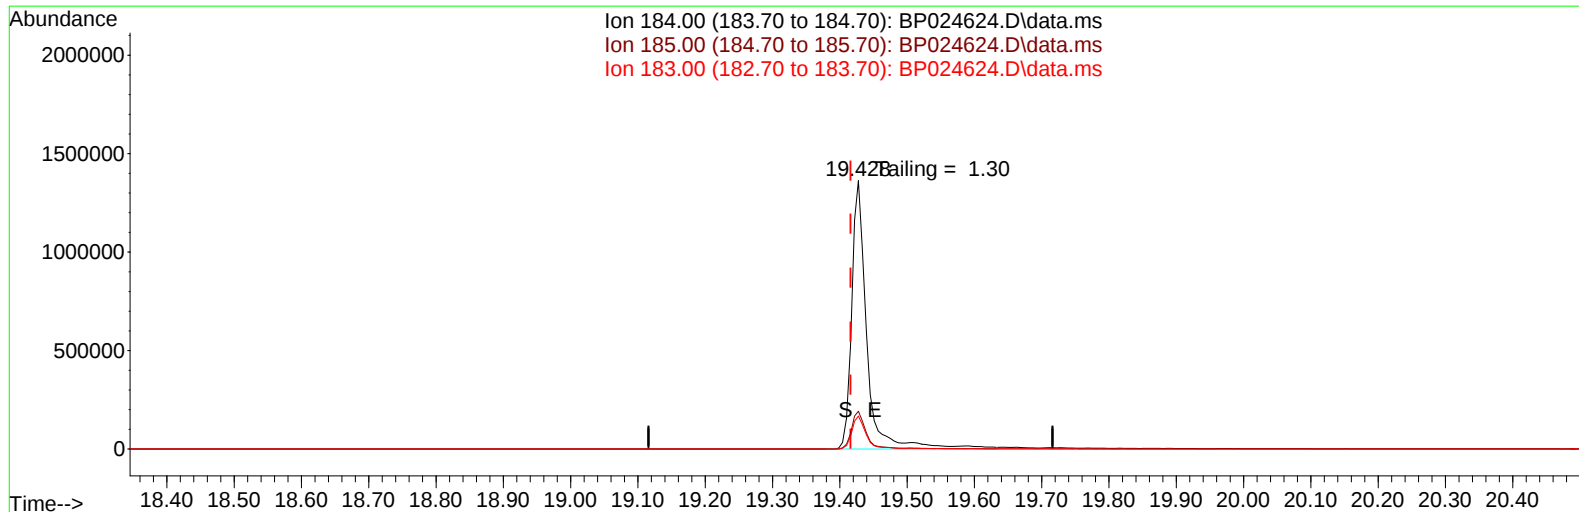

TIC: BP024624.D\data.ms

(77) Benzidine

19.428min (+ 0.012) 72527.19 ng

response 2010903

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.07
183.00	12.30	12.28
0.00	0.00	0.00